


Instrument IC-1										Analyst: NF		Method: 300.0 / 9056A			
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial Analyst					
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 11:09	10 NF/IZ					
STD2	0.430	0.640	0.649	2.129	0.543	1.098	3.287	IC1-052225	5/22/2025 11:30	10 NF/IZ					
STD3	0.795	1.207	1.205	4.018	1.004	1.867	6.069	IC1-052225	5/22/2025 11:52	10 NF/IZ					
STD4	0.977	1.480	1.479	4.929	1.229	2.477	7.415	IC1-052225	5/22/2025 12:13	10 NF/IZ					
STD5	1.991	2.968	2.960	9.916	2.467	5.110	14.621	IC1-052225	5/22/2025 12:35	10 NF/IZ					
STD6	4.001	5.967	5.959	19.868	4.966	9.870	29.848	IC1-052225	5/22/2025 12:56	10 NF/IZ					
STD7	5.006	7.539	7.548	25.140	6.290	12.578	37.260	IC1-052225	5/22/2025 13:17	10 NF/IZ					
ICV	2.054	3.101	3.056	10.229	2.610	5.286	15.128	IC1-052225	5/22/2025 13:39	10 NF/IZ					
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 14:22	10 NF/IZ					
CCV	2.099	3.134	3.113	10.491	2.612	5.230	15.517	IC1-052225	6/3/2025 14:34	10 NF/IZ					
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/3/2025 14:55	10 NF/IZ					
LB135991BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/3/2025 15:17	10 NF/IZ					
LB135991BSW	2.110	3.127	3.120	10.470	2.609	5.333	15.532	IC1-052225	6/3/2025 15:38	10 NF/IZ					
Q2189-01	0.090	462.470	0.000	0.433	9.180	0.000	64.157	IC1-052225	6/3/2025 16:00	10 NF/IZ					
Q2189-01MS	2.097	445.282	3.043	10.535	11.607	5.212	78.254	IC1-052225	6/3/2025 16:21	10 NF/IZ					
Q2189-01MSD	2.104	444.161	3.020	10.474	11.598	5.236	78.268	IC1-052225	6/3/2025 16:43	10 NF/IZ					
Q2189-02	0.065	336.812	0.000	0.634	4.315	0.000	25.003	IC1-052225	6/3/2025 17:05	10 NF/IZ					
CCV	2.083	3.144	3.134	10.499	2.618	5.385	15.566	IC1-052225	6/3/2025 17:26	10 NF/IZ					
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/3/2025 17:48	10 NF/IZ					
CCV	2.129	3.173	3.152	10.567	2.638	5.242	15.665	IC1-052225	6/4/2025 10:15	10 NF/IZ					
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/4/2025 10:37	10 NF/IZ					
LB135991BLW2	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/4/2025 10:58	10 NF/IZ					
LB135991BSW2	2.151	3.196	3.186	10.665	2.659	5.403	15.827	IC1-052225	6/4/2025 11:20	10 NF/IZ					
Q2189-01DLX5	0.037	77.607	0.000	0.208	1.757	0.000	12.157	IC1-052225	6/4/2025 11:41	10 NF/IZ					
Q2202-01	0.183	145.087	0.000	0.338	1.962	0.000	80.447	IC1-052225	6/4/2025 12:46	10 NF/IZ					
Q2202-05	0.037	59.654	0.095	0.000	1.180	0.000	9.093	IC1-052225	6/4/2025 13:08	10 NF/IZ					
Q2202-01DLX5	0.063	23.210	0.000	0.000	0.423	0.000	14.807	IC1-052225	6/4/2025 13:29	10 NF/IZ					
CCV	2.063	3.111	3.102	10.390	2.587	5.266	15.384	IC1-052225	6/4/2025 13:51	10 NF/IZ					
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/4/2025 14:12	10 NF/IZ					

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-052225	10 NF/IZ
STD2	0.4300	0.6400	0.6490	2.1290	0.5430	1.0980	3.2870	IC1-052225	10 NF/IZ
STD3	0.7950	1.2070	1.2050	4.0180	1.0040	1.8670	6.0690	IC1-052225	10 NF/IZ
STD4	0.9770	1.4800	1.4790	4.9290	1.2290	2.4770	7.4150	IC1-052225	10 NF/IZ
STD5	1.9910	2.9680	2.9600	9.9160	2.4670	5.1100	14.6210	IC1-052225	10 NF/IZ
STD6	4.0010	5.9670	5.9590	19.8680	4.9660	9.8700	29.8480	IC1-052225	10 NF/IZ
STD7	5.0060	7.5390	7.5480	25.1400	6.2900	12.5780	37.2600	IC1-052225	10 NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1	7.5000	6.6667	8.1667	6.4500	8.6000	9.8000	9.5667		
STD2	-0.6250	0.5833	0.4167	0.4500	0.4000	-6.6500	1.1500		
STD3	-2.3000	-1.3333	-1.4000	-1.4200	-1.6800	-0.9200	-1.1333		
STD4	-0.4500	-1.0667	-1.3333	-0.8400	-1.3200	2.2000	-2.5267		
STD5	0.0250	-0.5500	-0.6833	-0.6600	-0.6800	-1.3000	-0.5067		
STD6	0.1200	0.5200	0.6400	0.5600	0.6400	0.6240	0.7027		
STD7									

Fluoride (Anions)

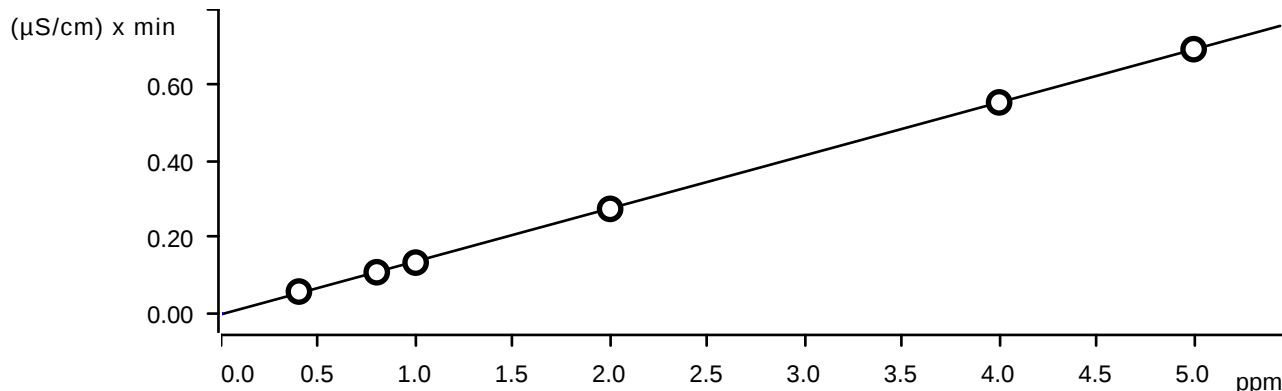


Function: $A = -2.82659E-3 + 0.0139492 \times Q$

Relative standard deviation 0.920519 %

Correlation coefficient 0.999955

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.108	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.133	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.275	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.555	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.695	STD7	2025-05-22 13:17:57 UTC-4	used

Chloride (Anions)

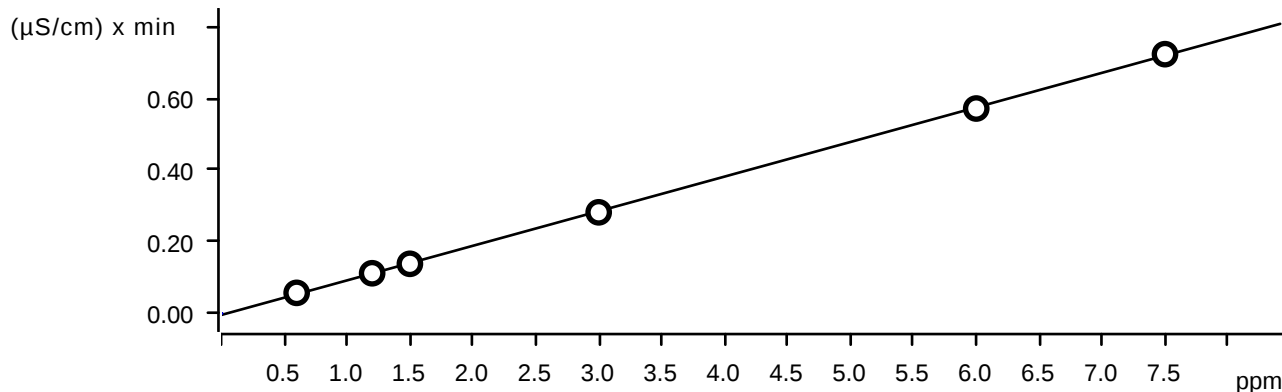

Function: $A = -4.33057E-3 + 9.64673E-3 \times Q$


Relative standard deviation 1.154335 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.138	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.282	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.571	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.723	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

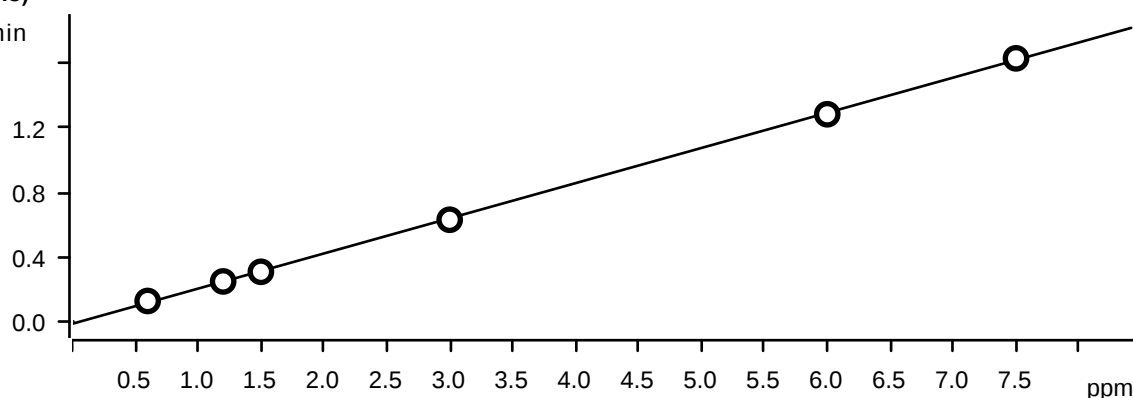Function: $A = -0.0150155 + 0.0217890 \times Q$


Relative standard deviation 1.428639 %

Correlation coefficient 0.999893

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.307	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.630	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.283	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.630	STD7	2025-05-22 13:17:57 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

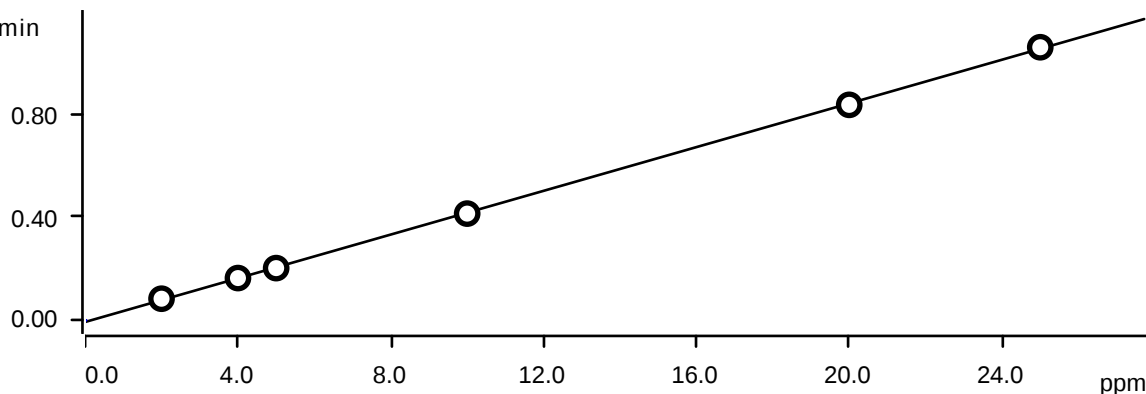

Function: $A = -6.27114E-3 + 4.23162E-3 \times Q$


Relative standard deviation: 1.185575 %

Correlation coefficient: 0.999925

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.164	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.202	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.413	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.834	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.058	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

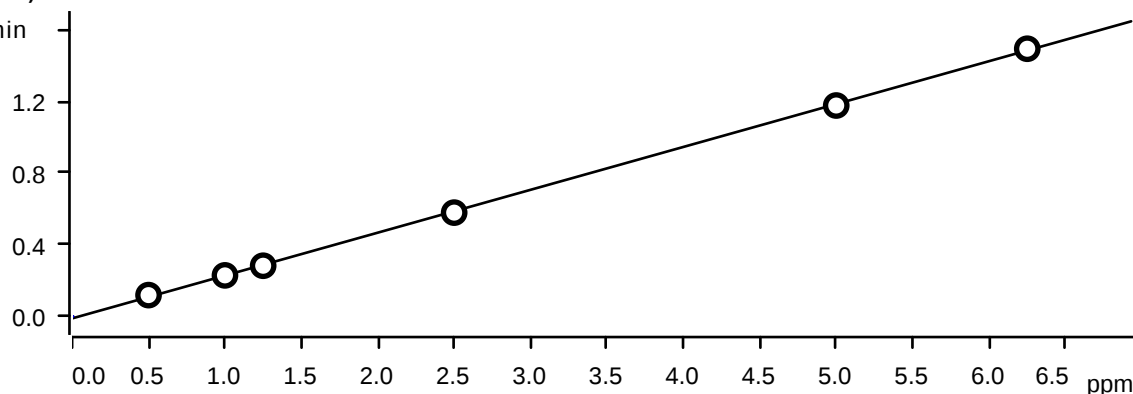


Function: $A = -0.0109593 + 0.0239055 \times Q$

Relative standard deviation: 1.451672 %

Correlation coefficient 0.999889

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.119	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.283	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.176	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.493	STD7	2025-05-22 13:17:57 UTC-4	used

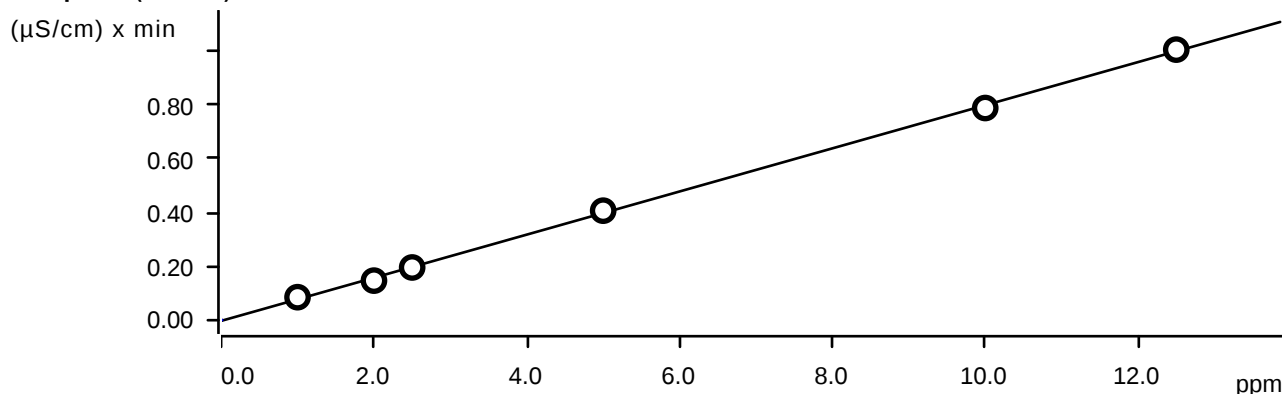
Phosphate (Anions)Function: $A = -3.02035E-3 + 8.01761E-3 \times Q$

Relative standard deviation 2.297726 %

Correlation coefficient 0.999716

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.085	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.147	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.196	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.407	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.788	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.005	STD7	2025-05-22 13:17:57 UTC-4	used

Sulfate (Anions)

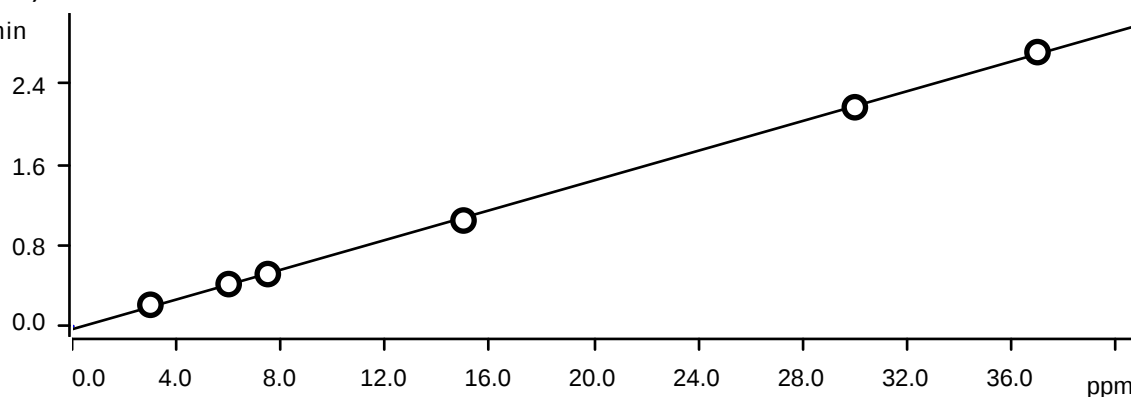 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0303663 + 7.37295E-3 \times Q$

Relative standard deviation 1.792871 %

Correlation coefficient 0.999832

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.417	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.516	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.048	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.170	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.717	STD7	2025-05-22 13:17:57 UTC-4	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-05-22 11:09:38 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

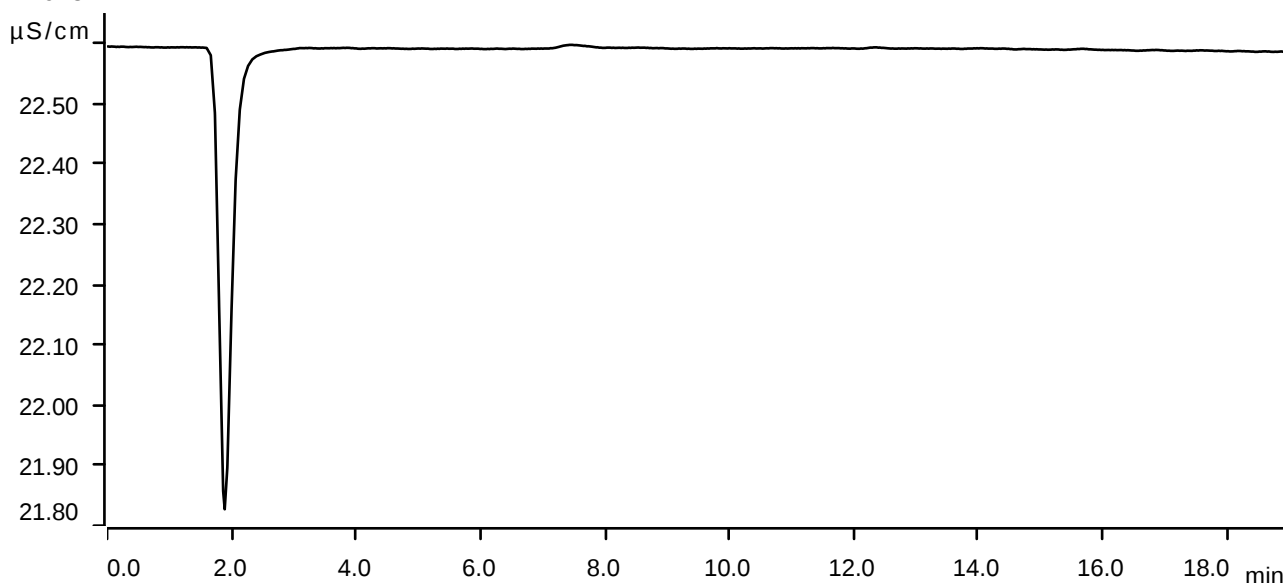


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-05-22 11:30:53 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

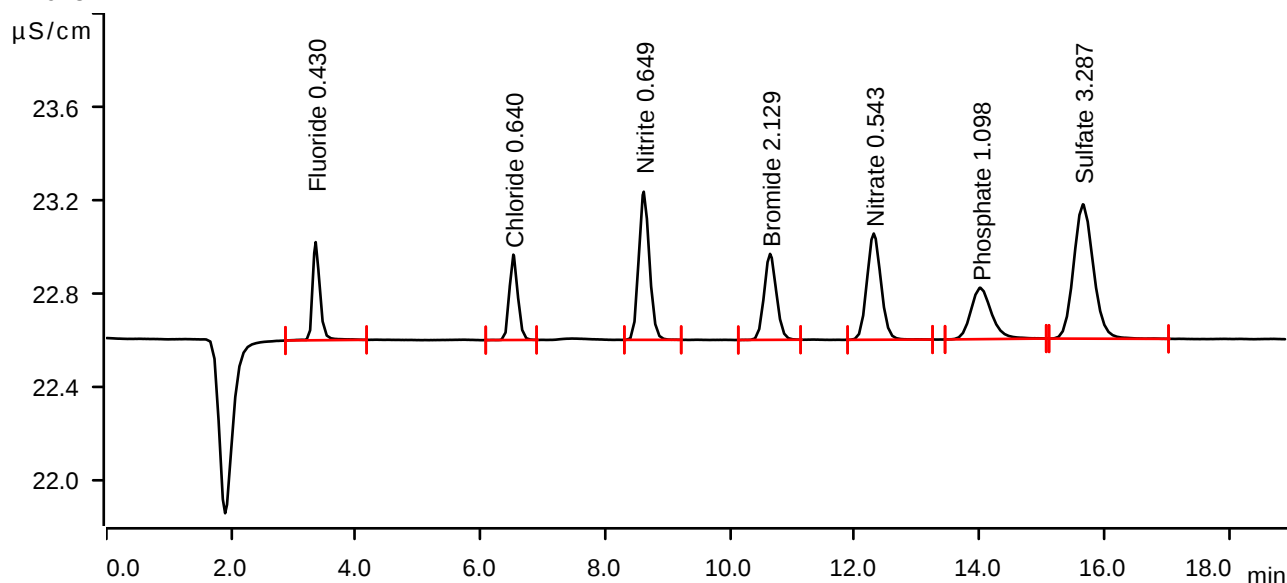

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0572	0.421	0.430	Fluoride
2	6.525	0.0574	0.366	0.640	Chloride
3	8.617	0.1264	0.636	0.649	Nitrite
4	10.642	0.0838	0.369	2.129	Bromide
5	12.303	0.1190	0.456	0.543	Nitrate
6	14.013	0.0850	0.221	1.098	Phosphate
7	15.657	0.2120	0.577	3.287	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-05-22 11:52:16 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

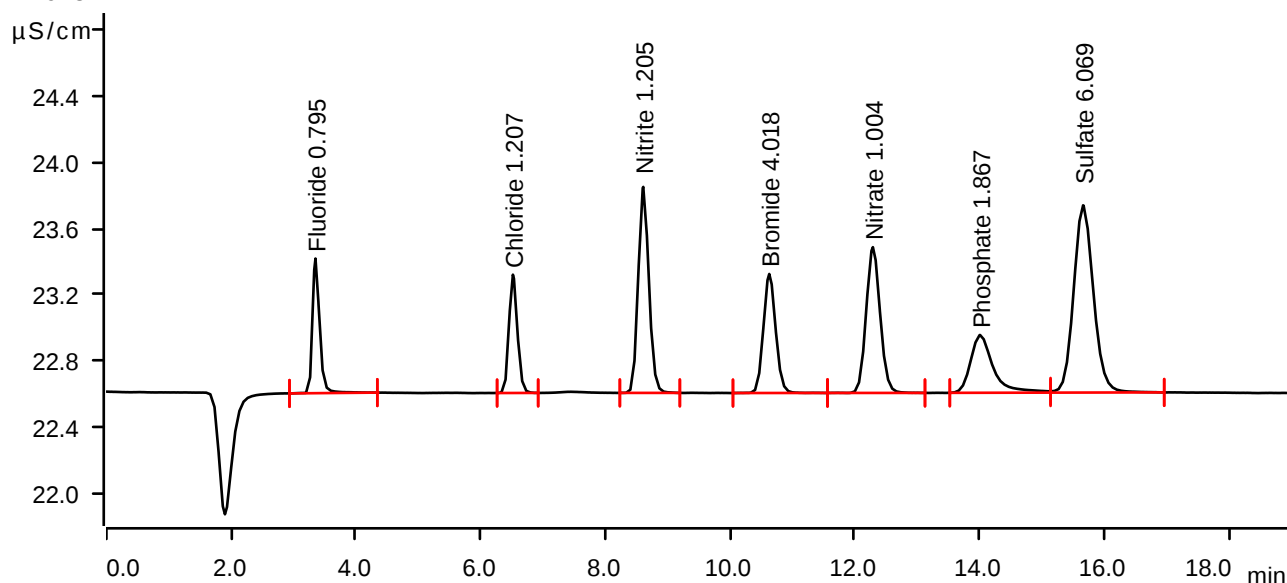

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1081	0.814	0.795	Fluoride
2	6.518	0.1121	0.716	1.207	Chloride
3	8.608	0.2475	1.247	1.205	Nitrite
4	10.628	0.1637	0.720	4.018	Bromide
5	12.290	0.2290	0.882	1.004	Nitrate
6	14.008	0.1467	0.350	1.867	Phosphate
7	15.660	0.4171	1.133	6.069	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-05-22 12:13:41 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

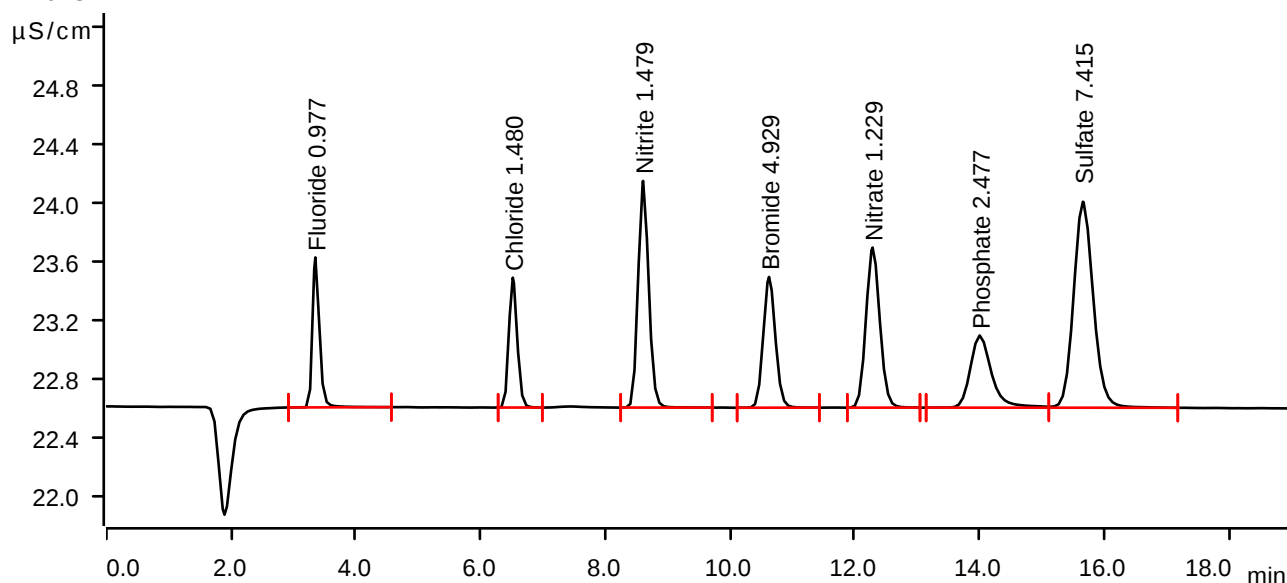

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.352	0.1334	1.024	0.977	Fluoride
2	6.517	0.1384	0.888	1.480	Chloride
3	8.607	0.3073	1.549	1.479	Nitrite
4	10.625	0.2023	0.894	4.929	Bromide
5	12.285	0.2828	1.094	1.229	Nitrate
6	14.003	0.1955	0.493	2.477	Phosphate
7	15.657	0.5164	1.408	7.415	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-05-22 12:35:06 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

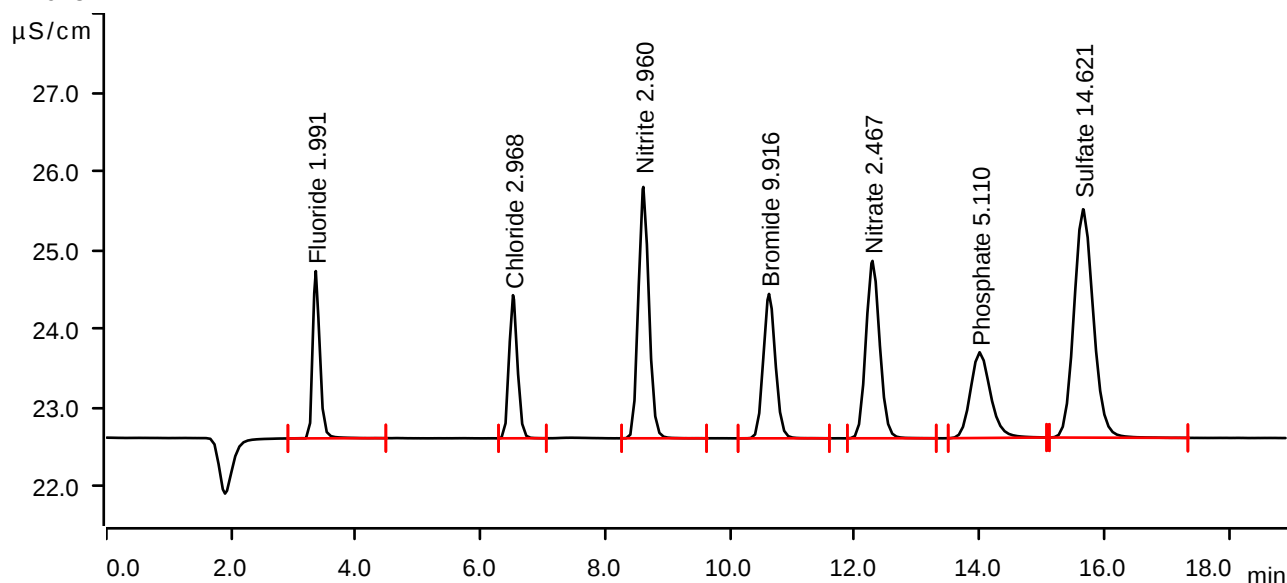

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2749	2.123	1.991	Fluoride
2	6.520	0.2820	1.816	2.968	Chloride
3	8.610	0.6298	3.190	2.960	Nitrite
4	10.625	0.4133	1.833	9.916	Bromide
5	12.283	0.5789	2.251	2.467	Nitrate
6	14.002	0.4067	1.087	5.110	Phosphate
7	15.660	1.0476	2.898	14.621	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-05-22 12:56:31 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

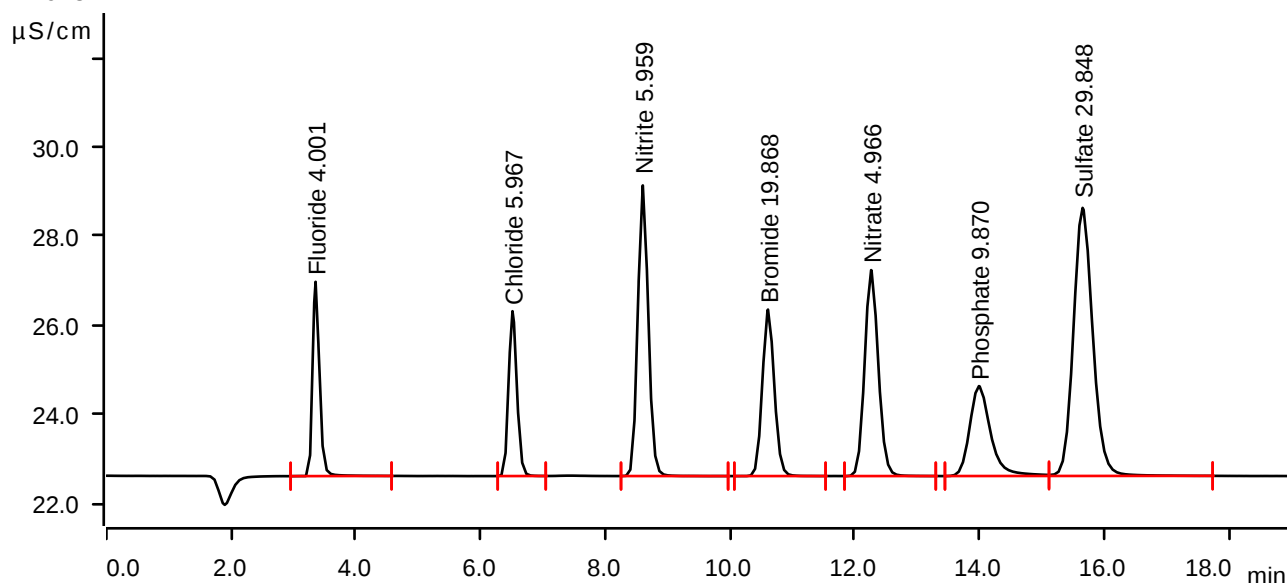

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.5553	4.361	4.001	Fluoride
2	6.512	0.5713	3.701	5.967	Chloride
3	8.602	1.2834	6.525	5.959	Nitrite
4	10.608	0.8345	3.739	19.868	Bromide
5	12.262	1.1762	4.624	4.966	Nitrate
6	13.990	0.7883	2.019	9.870	Phosphate
7	15.652	2.1703	6.019	29.848	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-05-22 13:17:57 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

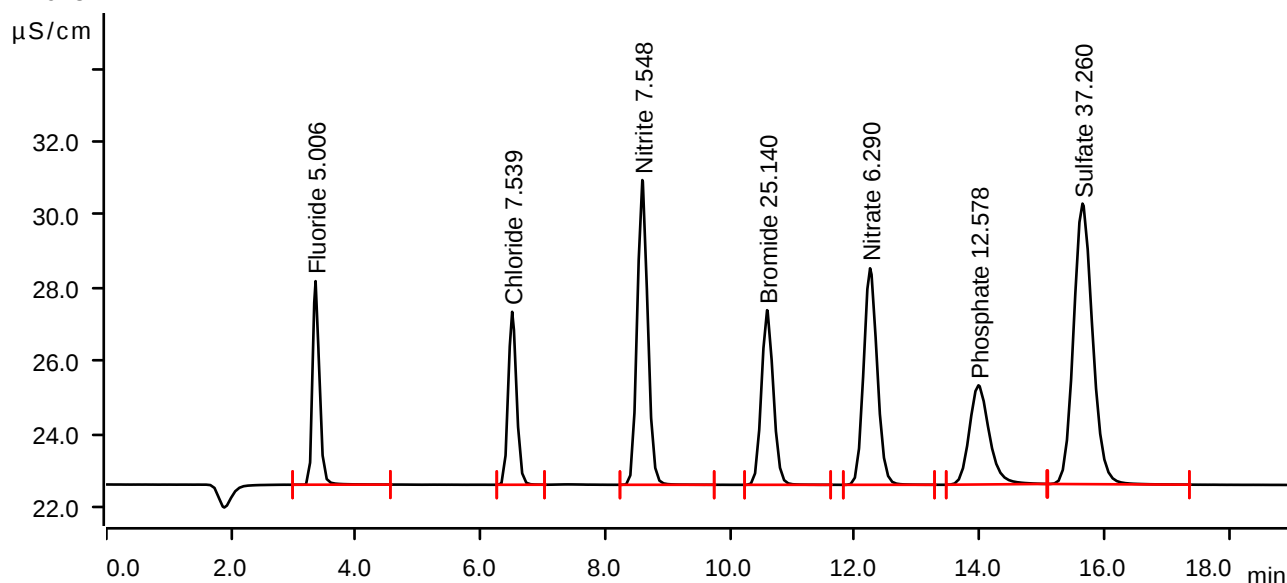

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.6954	5.562	5.006	Fluoride
2	6.507	0.7229	4.726	7.539	Chloride
3	8.593	1.6297	8.328	7.548	Nitrite
4	10.593	1.0576	4.774	25.140	Bromide
5	12.245	1.4927	5.918	6.290	Nitrate
6	13.982	1.0054	2.711	12.578	Phosphate
7	15.650	2.7168	7.668	37.260	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-05-22 13:39:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

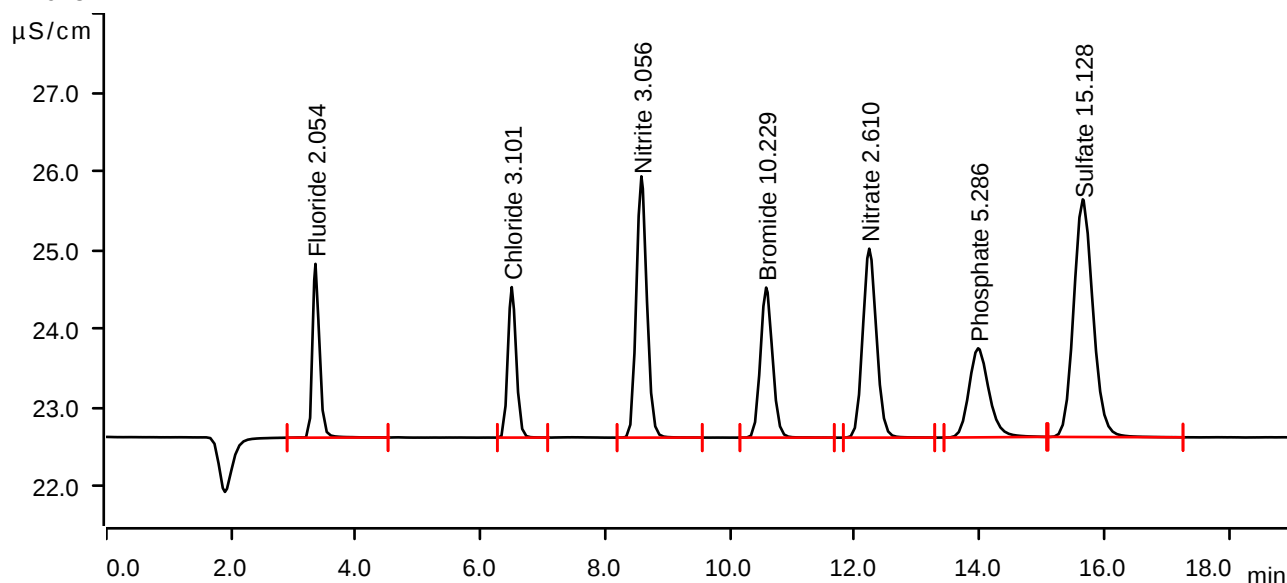


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2837	2.205	2.054	Fluoride
2	6.500	0.2948	1.910	3.101	Chloride
3	8.578	0.6509	3.316	3.056	Nitrite
4	10.578	0.4266	1.904	10.229	Bromide
5	12.232	0.6129	2.398	2.610	Nitrate
6	13.977	0.4208	1.130	5.286	Phosphate
7	15.655	1.0850	3.016	15.128	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-05-22 14:22:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

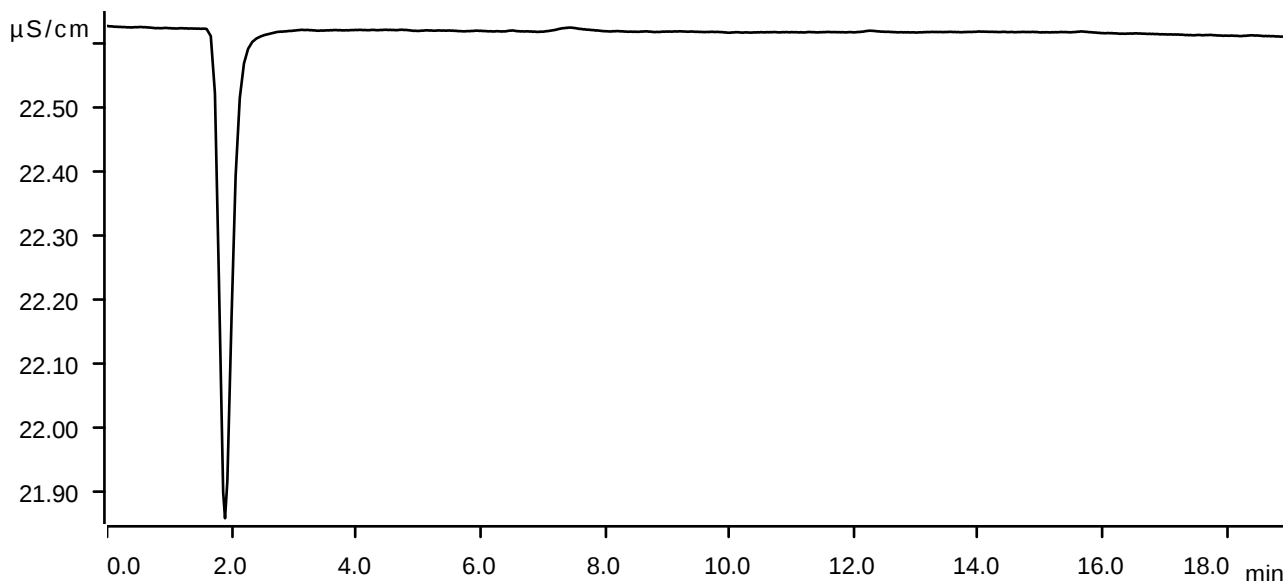Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-03 14:34:19 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

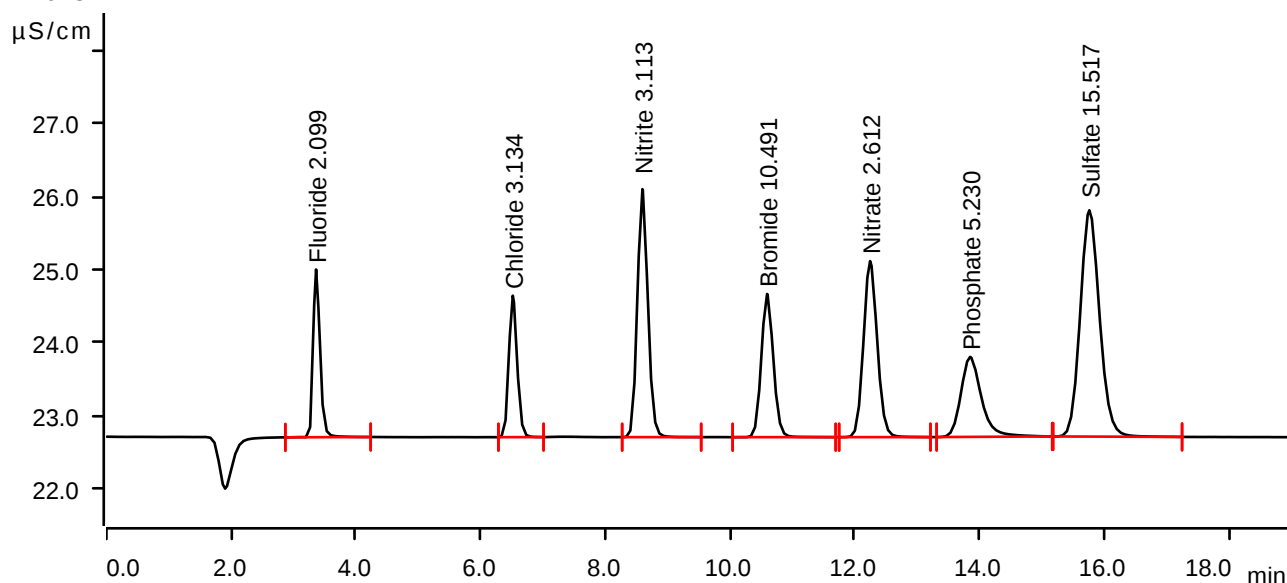


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.2899	2.292	2.099	Fluoride
2	6.517	0.2980	1.933	3.134	Chloride
3	8.595	0.6632	3.389	3.113	Nitrite
4	10.593	0.4377	1.957	10.491	Bromide
5	12.245	0.6134	2.406	2.612	Nitrate
6	13.848	0.4163	1.093	5.230	Phosphate
7	15.760	1.1137	3.093	15.517	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-03 14:55:49 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

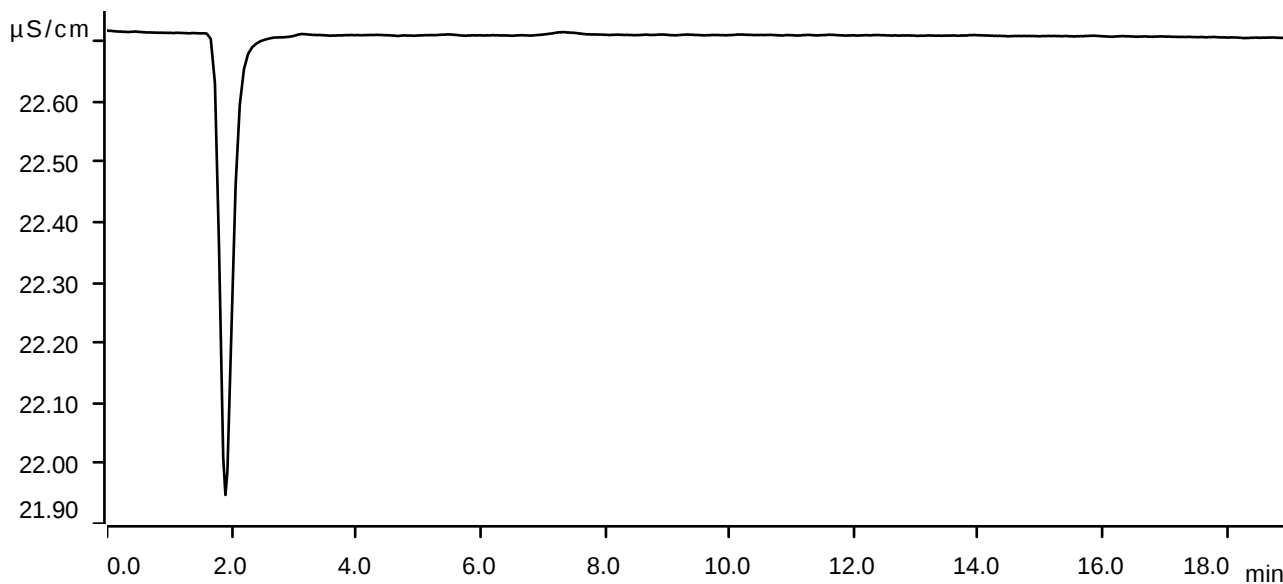
Anions

Sample data

Ident LB135991BLW
Sample type Sample
Determination start 2025-06-03 15:17:19 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

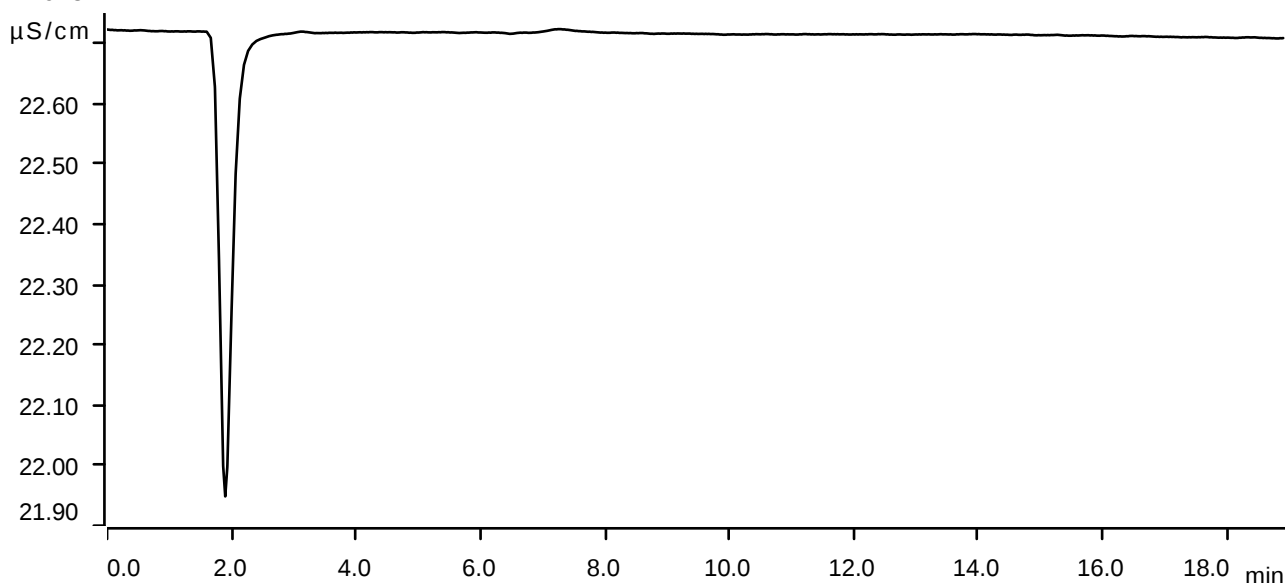Anions


Sample data

Ident LB135991BSW
Sample type Check standard 1
Determination start 2025-06-03 15:38:49 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

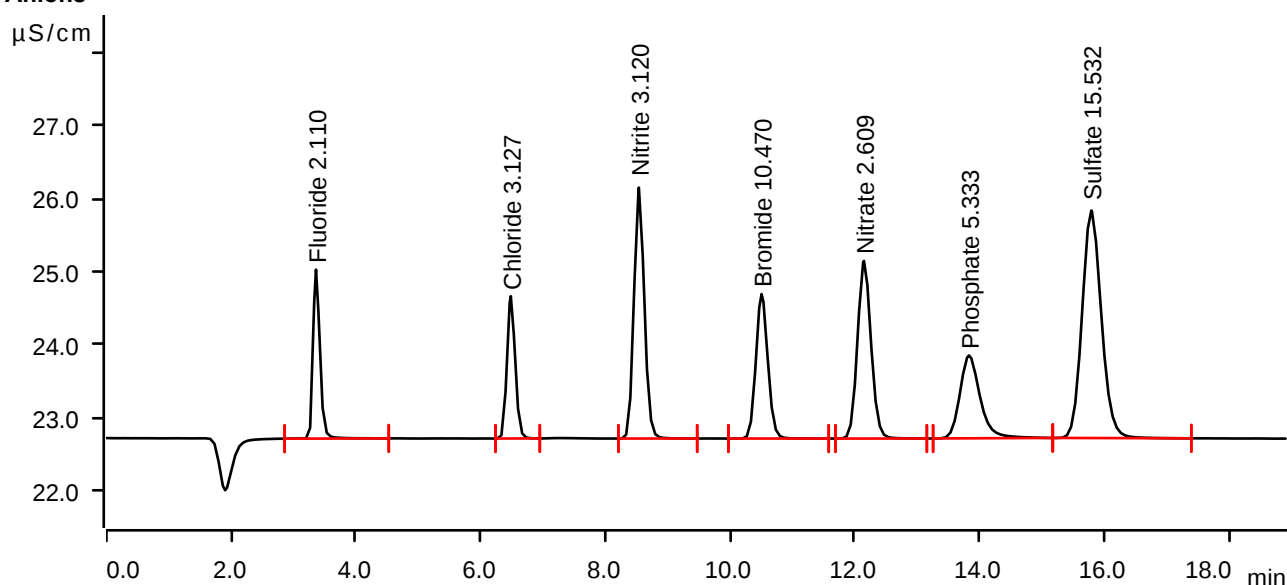

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2915	2.309	2.110	Fluoride
2	6.485	0.2973	1.944	3.127	Chloride
3	8.538	0.6647	3.429	3.120	Nitrite
4	10.505	0.4368	1.975	10.470	Bromide
5	12.147	0.6127	2.429	2.609	Nitrate
6	13.830	0.4246	1.132	5.333	Phosphate
7	15.792	1.1148	3.109	15.532	Sulfate


Sample data

Ident Q2189-01
Sample type Sample
Determination start 2025-06-03 16:00:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

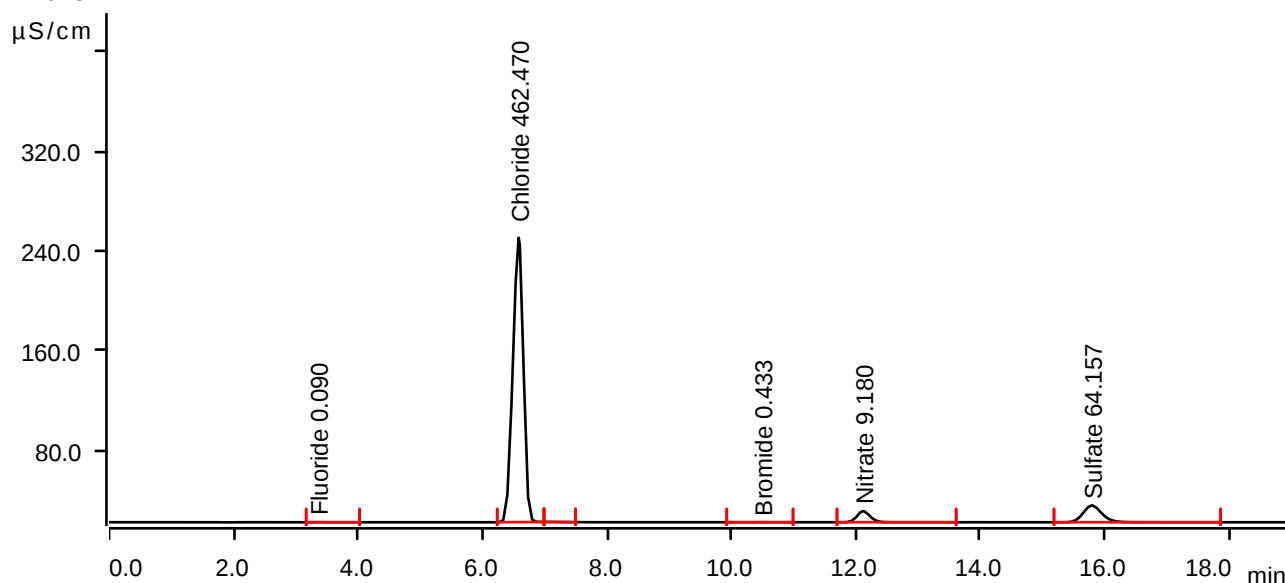

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.0097	0.071	0.090	Fluoride
2	6.583	44.6089	227.716	462.470	Chloride
3	7.077	0.0104	0.035	invalid	
4	10.495	0.0121	0.052	0.433	Bromide
5	12.118	2.1835	8.940	9.180	Nitrate
6	15.792	4.6999	13.519	64.157	Sulfate


Sample data

Ident Q2189-01MS
Sample type Sample
Determination start 2025-06-03 16:21:54 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

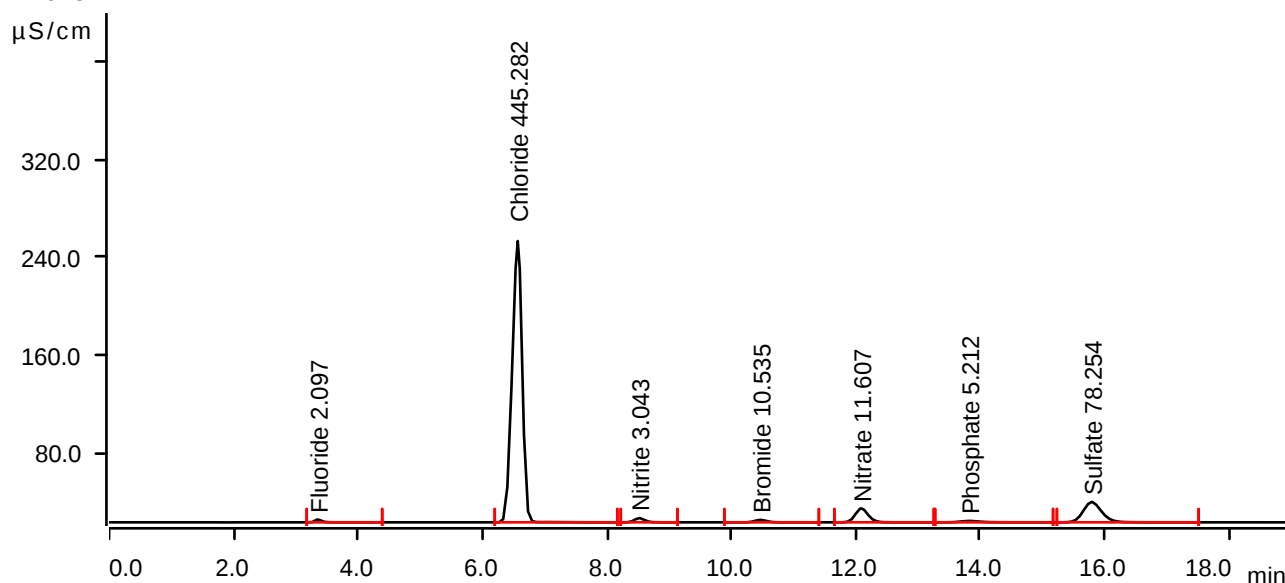

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.2898	2.295	2.097	Fluoride
2	6.568	42.9509	230.631	445.282	Chloride
3	8.522	0.6481	3.425	3.043	Nitrite
4	10.467	0.4395	2.022	10.535	Bromide
5	12.088	2.7638	11.442	11.607	Nitrate
6	13.822	0.4149	1.108	5.212	Phosphate
7	15.790	5.7393	16.663	78.254	Sulfate


Sample data

Ident Q2189-01MSD
Sample type Sample
Determination start 2025-06-03 16:43:27 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

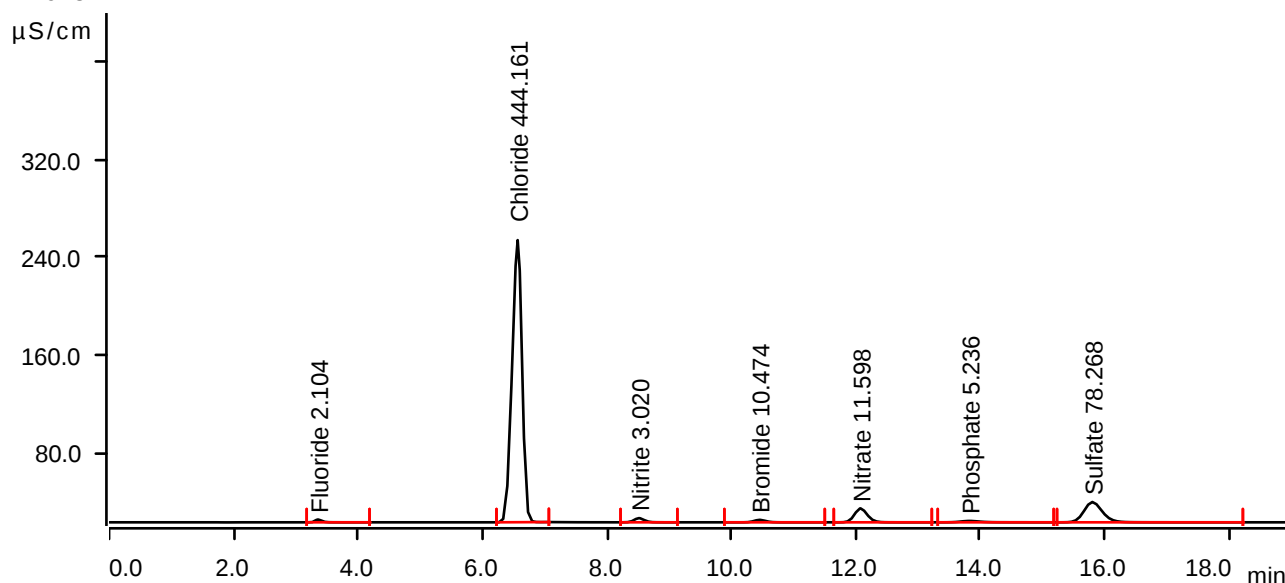

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2907	2.294	2.104	Fluoride
2	6.567	42.8427	231.316	444.161	Chloride
3	8.515	0.6431	3.399	3.020	Nitrite
4	10.455	0.4369	2.008	10.474	Bromide
5	12.077	2.7617	11.431	11.598	Nitrate
6	13.825	0.4168	1.113	5.236	Phosphate
7	15.802	5.7403	16.631	78.268	Sulfate


Sample data

Ident Q2189-02
Sample type Sample
Determination start 2025-06-03 17:05:00 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

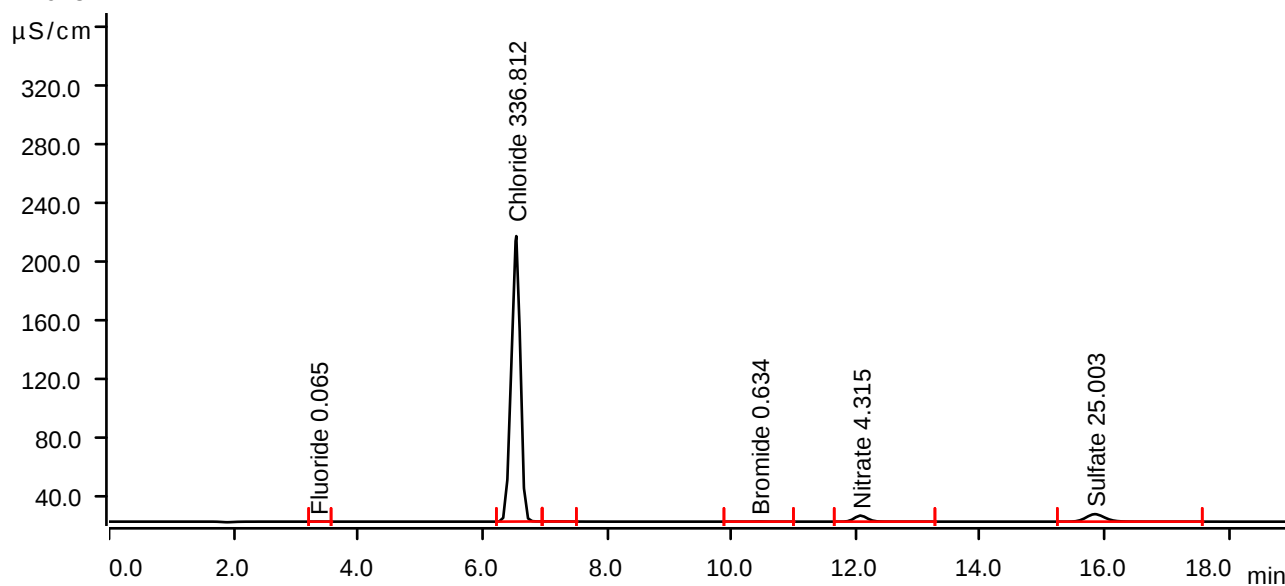

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0063	0.050	0.065	Fluoride
2	6.545	32.4870	195.058	336.812	Chloride
3	7.078	0.0093	0.030	invalid	
4	10.448	0.0206	0.090	0.634	Bromide
5	12.075	1.0205	4.136	4.315	Nitrate
6	15.842	1.8131	5.123	25.003	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-03 17:26:35 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

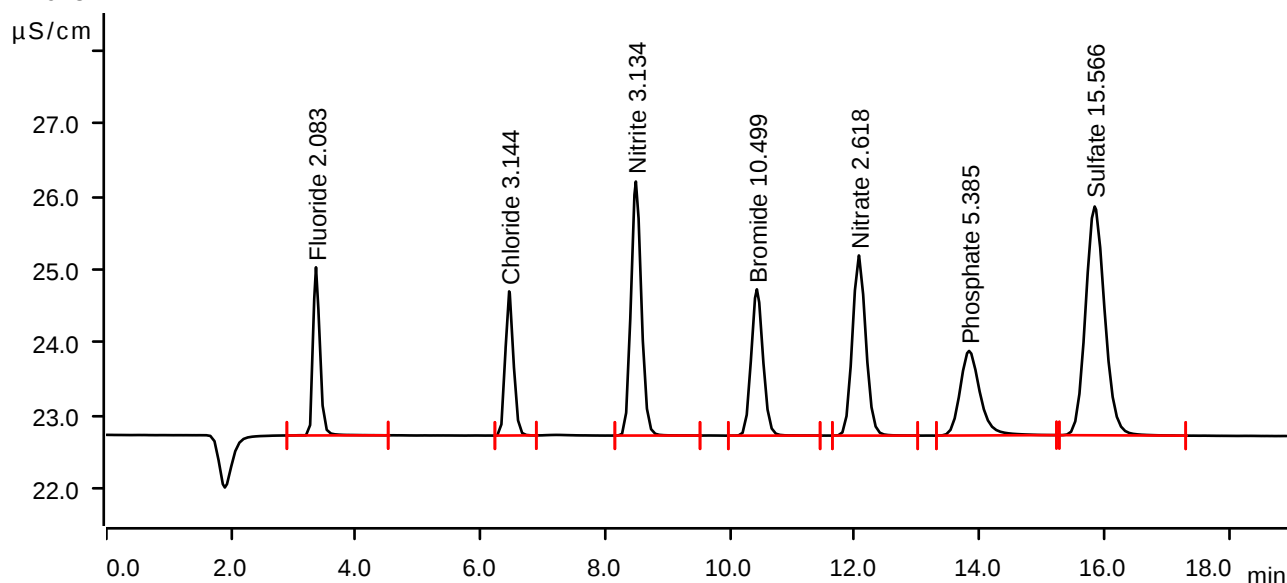


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2878	2.297	2.083	Fluoride
2	6.458	0.2989	1.969	3.144	Chloride
3	8.490	0.6679	3.471	3.134	Nitrite
4	10.430	0.4380	2.000	10.499	Bromide
5	12.065	0.6148	2.462	2.618	Nitrate
6	13.832	0.4288	1.155	5.385	Phosphate
7	15.845	1.1173	3.127	15.566	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-03 17:48:04 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

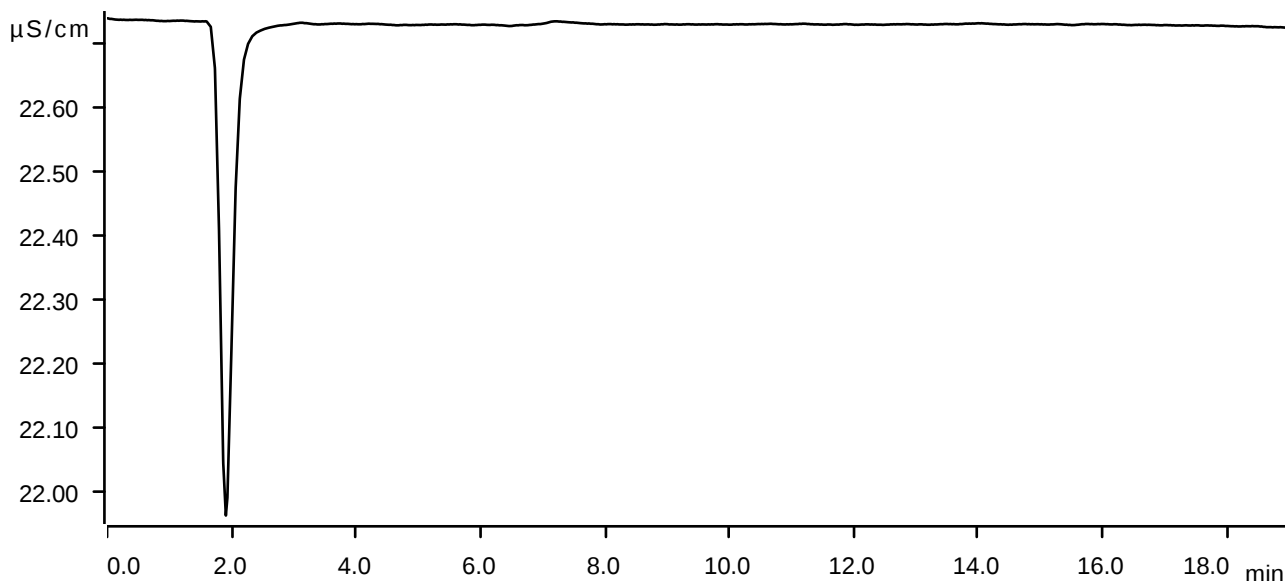Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-04 10:15:52 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

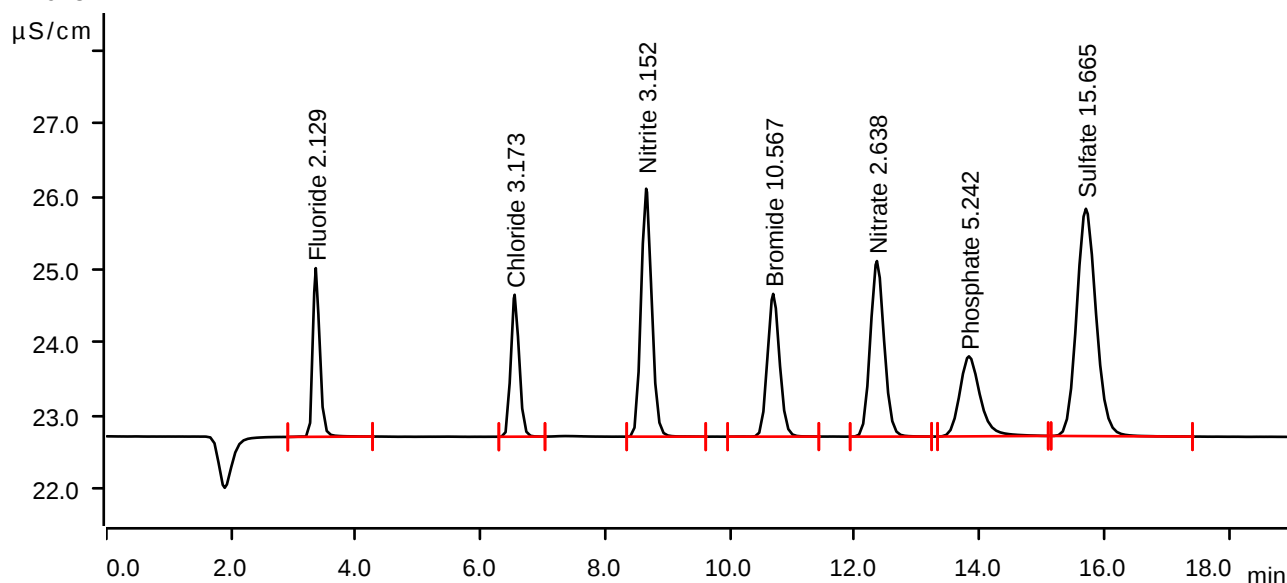


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2942	2.305	2.129	Fluoride
2	6.547	0.3018	1.940	3.173	Chloride
3	8.655	0.6717	3.389	3.152	Nitrite
4	10.692	0.4409	1.951	10.567	Bromide
5	12.355	0.6197	2.400	2.638	Nitrate
6	13.830	0.4173	1.094	5.242	Phosphate
7	15.705	1.1246	3.107	15.665	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-04 10:37:22 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

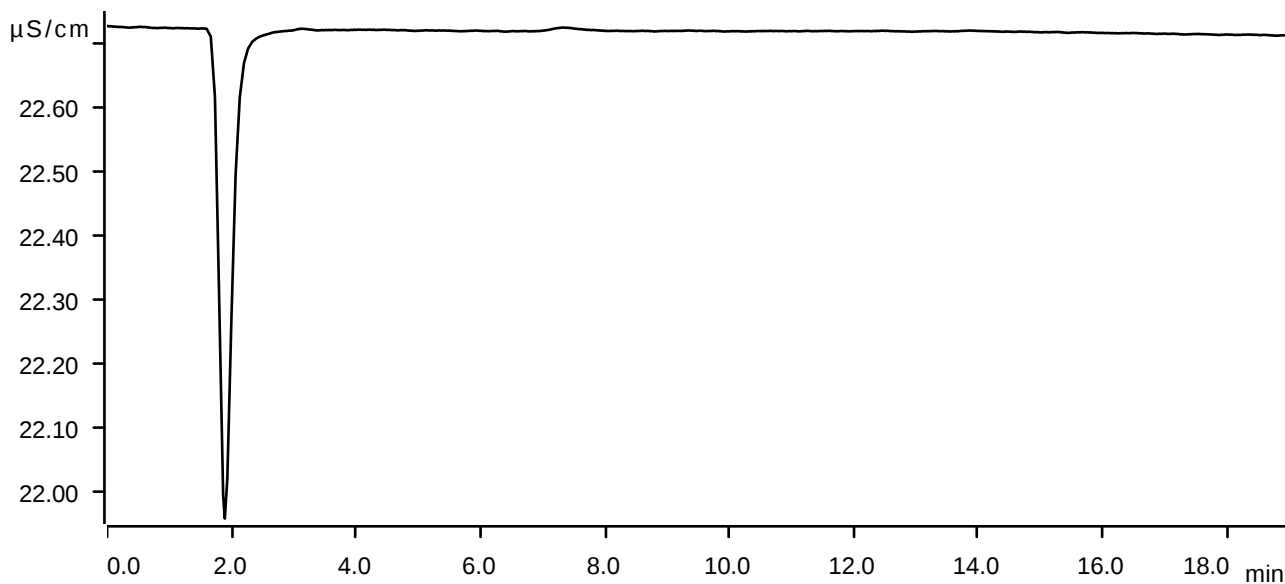
Anions

Sample data

Ident LB135991BLW2
Sample type Sample
Determination start 2025-06-04 10:58:52 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

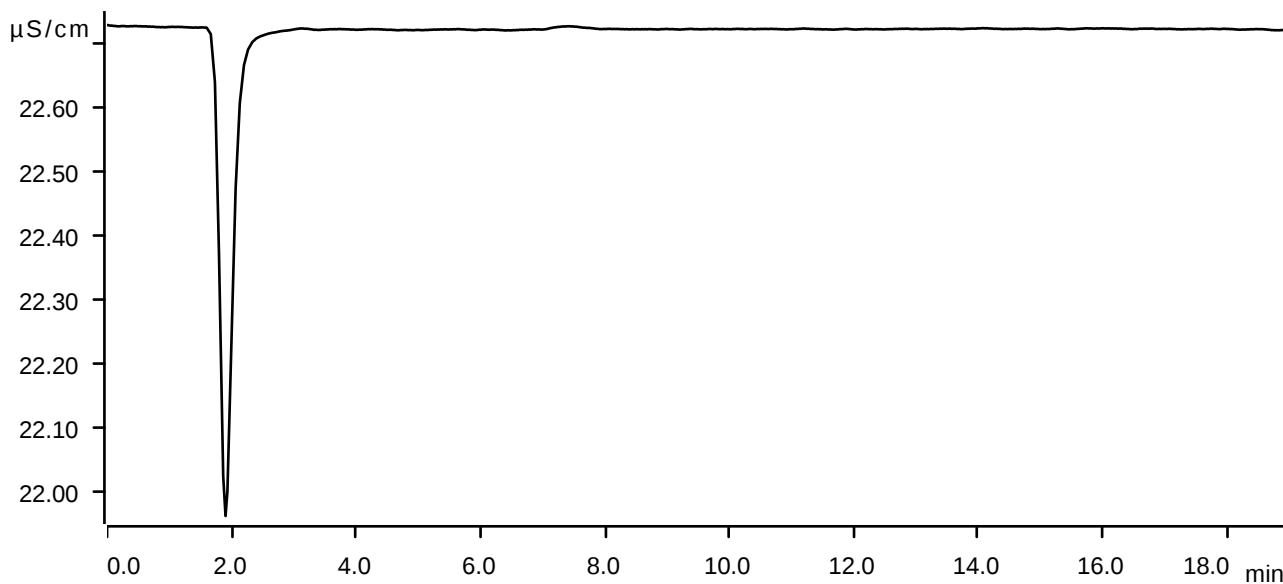Anions


Sample data

Ident LB135991BSW2
Sample type Check standard 1
Determination start 2025-06-04 11:20:23 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

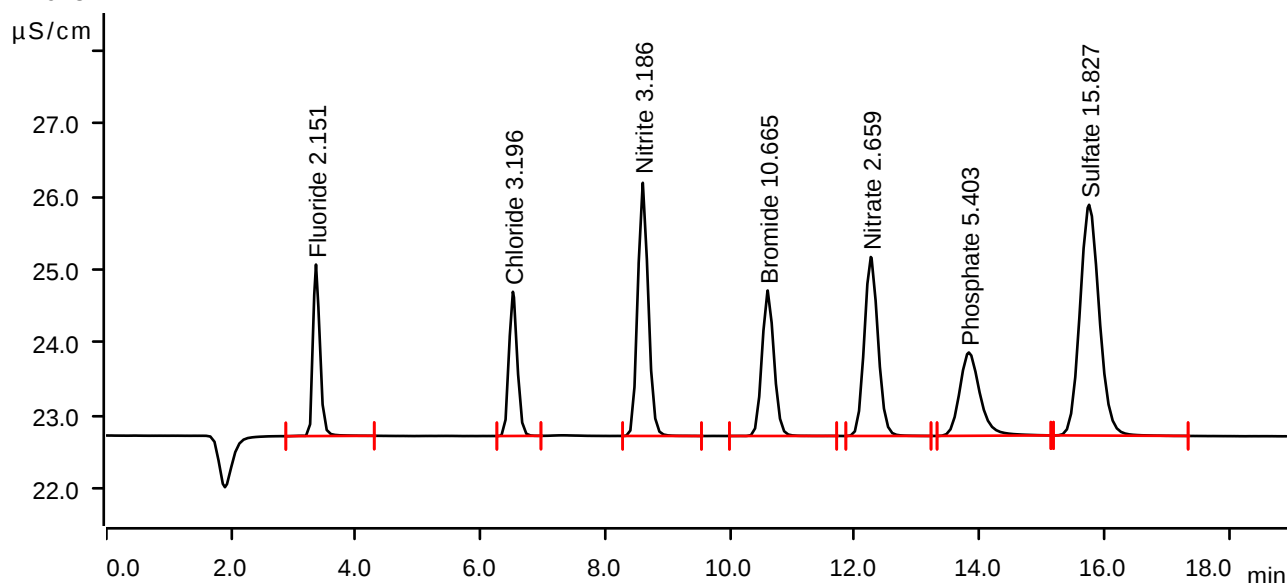

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2972	2.343	2.151	Fluoride
2	6.518	0.3040	1.970	3.196	Chloride
3	8.600	0.6791	3.459	3.186	Nitrite
4	10.603	0.4450	1.988	10.665	Bromide
5	12.257	0.6248	2.446	2.659	Nitrate
6	13.828	0.4302	1.139	5.403	Phosphate
7	15.757	1.1366	3.153	15.827	Sulfate


Sample data

Ident Q2189-01DLX5
Sample type Sample
Determination start 2025-06-04 11:41:55 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

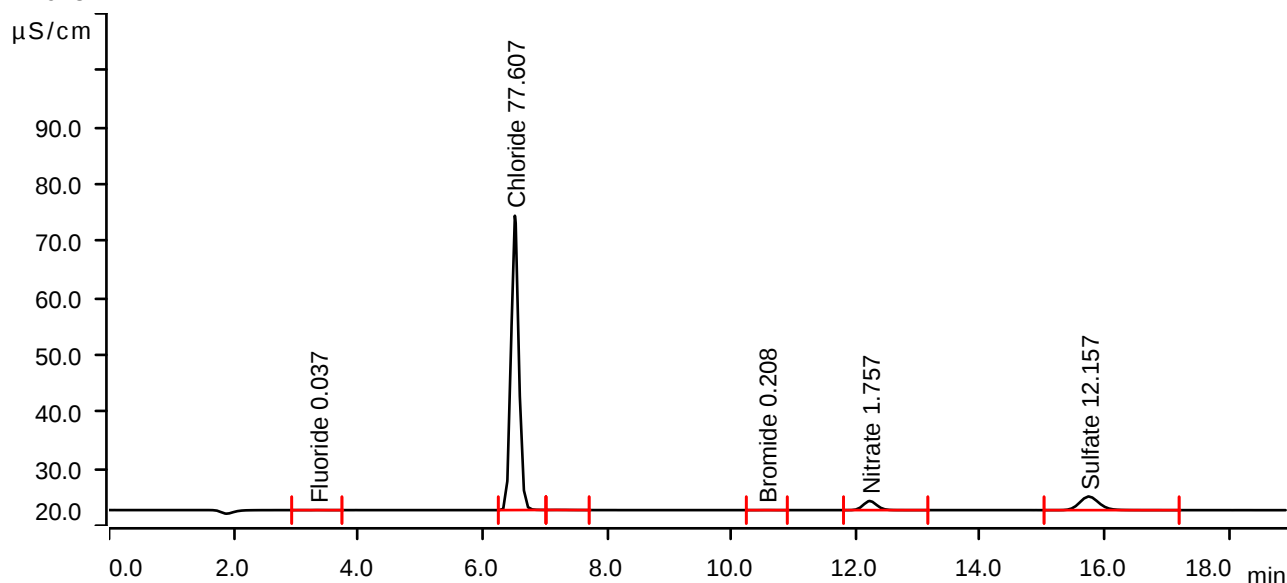

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.0024	0.014	0.037	Fluoride
2	6.522	7.4822	51.710	77.607	Chloride
3	7.205	0.0043	0.013	invalid	
4	10.567	0.0025	0.011	0.208	Bromide
5	12.223	0.4091	1.602	1.757	Nitrate
6	15.743	0.8659	2.397	12.157	Sulfate


Sample data

Ident Q2202-01
Sample type Sample
Determination start 2025-06-04 12:46:30 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

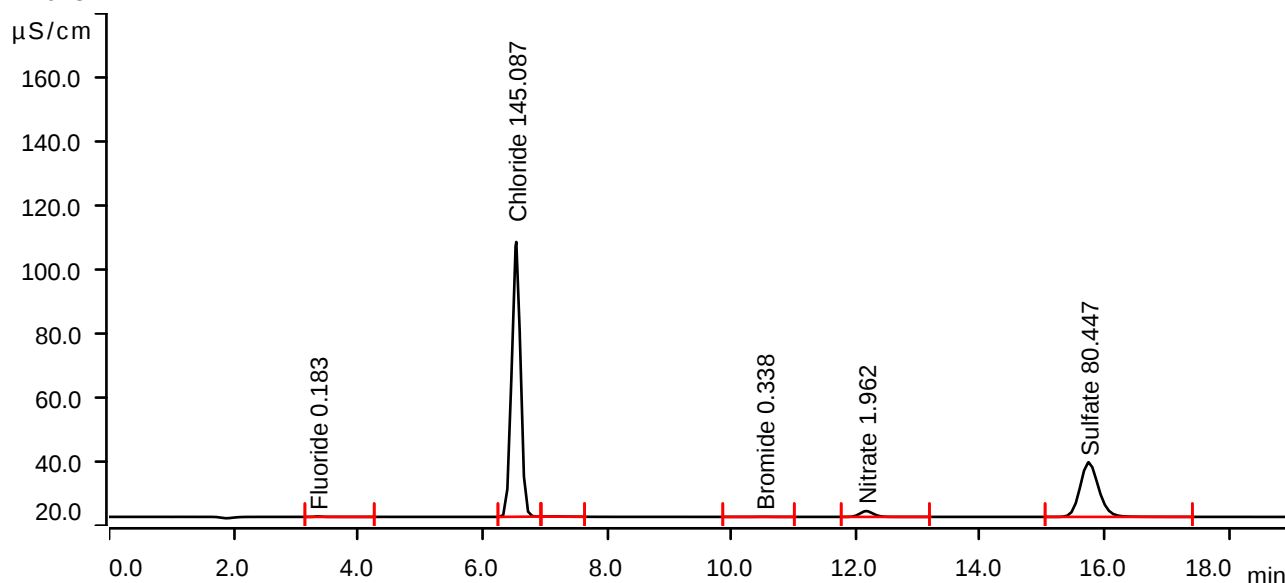

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.0227	0.158	0.183	Fluoride
2	6.545	13.9919	85.826	145.087	Chloride
3	7.117	0.0189	0.056	invalid	
4	10.527	0.0080	0.035	0.338	Bromide
5	12.168	0.4580	1.818	1.962	Nitrate
6	15.742	5.9009	17.058	80.447	Sulfate


Sample data

Ident Q2202-05
Sample type Sample
Determination start 2025-06-04 13:08:03 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

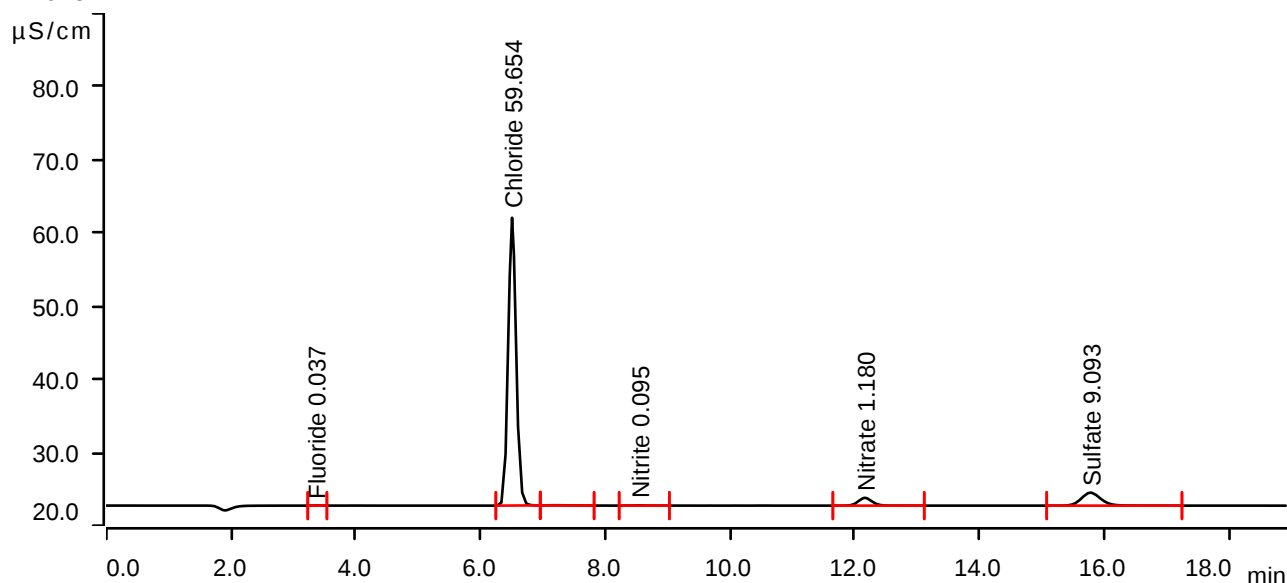

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0024	0.020	0.037	Fluoride
2	6.505	5.7503	39.327	59.654	Chloride
3	7.183	0.0105	0.029	invalid	
4	8.543	0.0057	0.028	0.095	Nitrite
5	12.162	0.2711	1.067	1.180	Nitrate
6	15.778	0.6401	1.774	9.093	Sulfate


Sample data

Ident Q2202-01DLX5
Sample type Sample
Determination start 2025-06-04 13:29:36 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

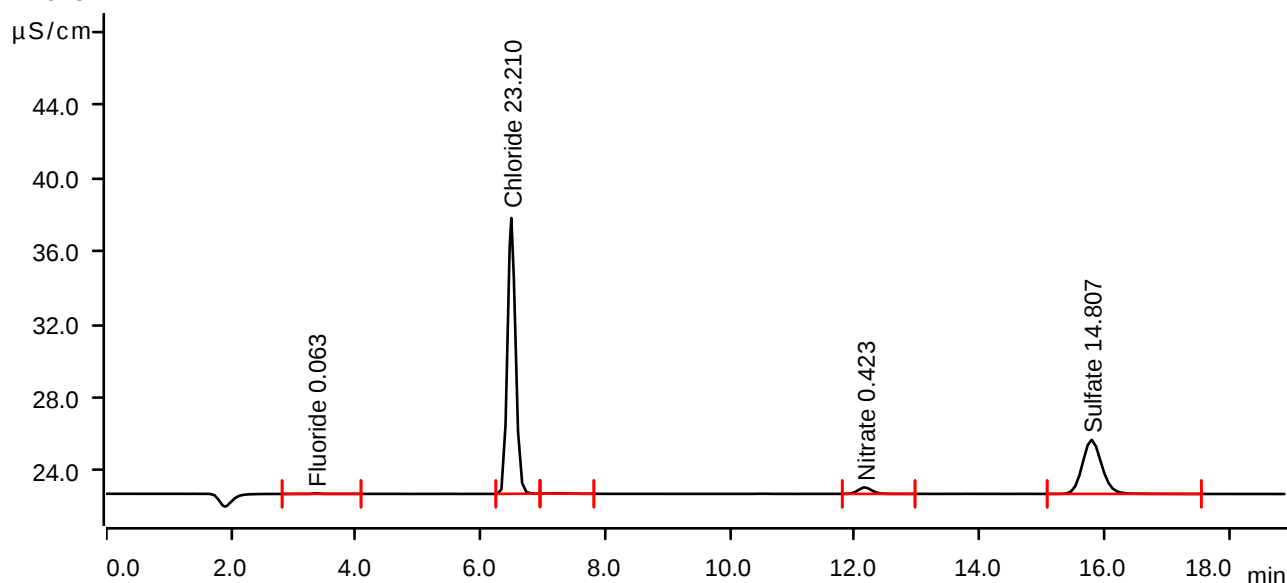

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0060	0.033	0.063	Fluoride
2	6.493	2.2347	15.075	23.210	Chloride
3	7.227	0.0071	0.019	invalid	
4	12.158	0.0903	0.354	0.423	Nitrate
5	15.795	1.0613	2.949	14.807	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-04 13:51:08 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

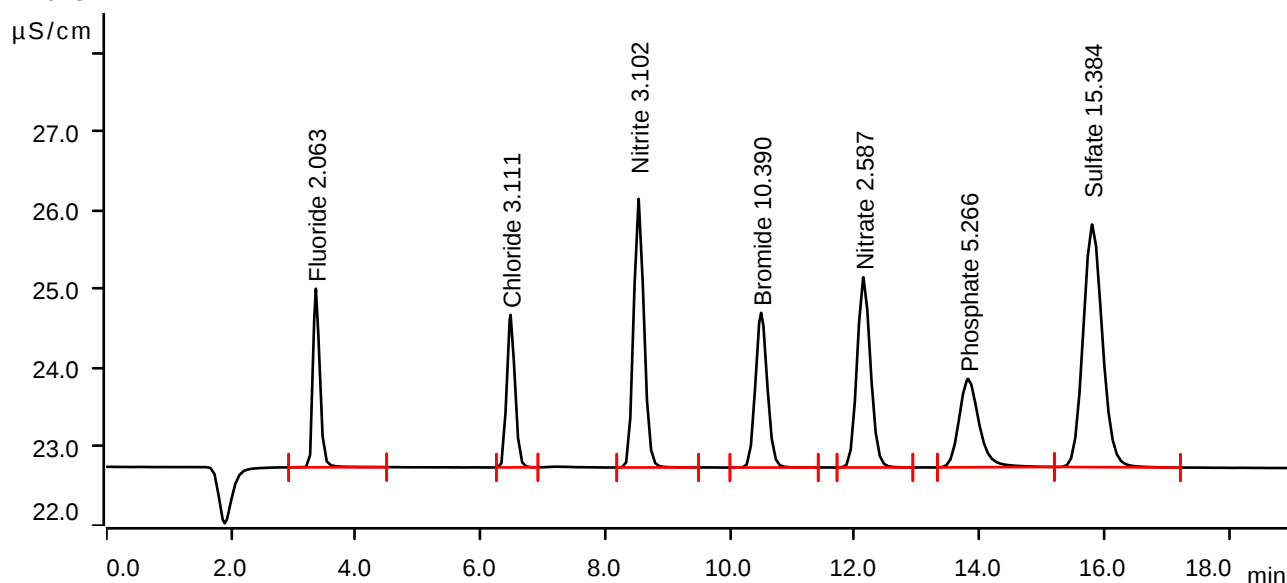

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.2850	2.266	2.063	Fluoride
2	6.482	0.2958	1.935	3.111	Chloride
3	8.533	0.6610	3.408	3.102	Nitrite
4	10.498	0.4334	1.963	10.390	Bromide
5	12.138	0.6076	2.414	2.587	Nitrate
6	13.815	0.4191	1.123	5.266	Phosphate
7	15.807	1.1039	3.079	15.384	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-04 14:12:38 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions