

LB 136 036

7470A

INSTRUMENT NO. CV2

$$\mu \text{ Abs.} :$$

36331

Linear


A= 0.0000e+000

B= 2.7248e-004

C= -7.3944e-003

Rho= 0.9996667

Accept=Accepted

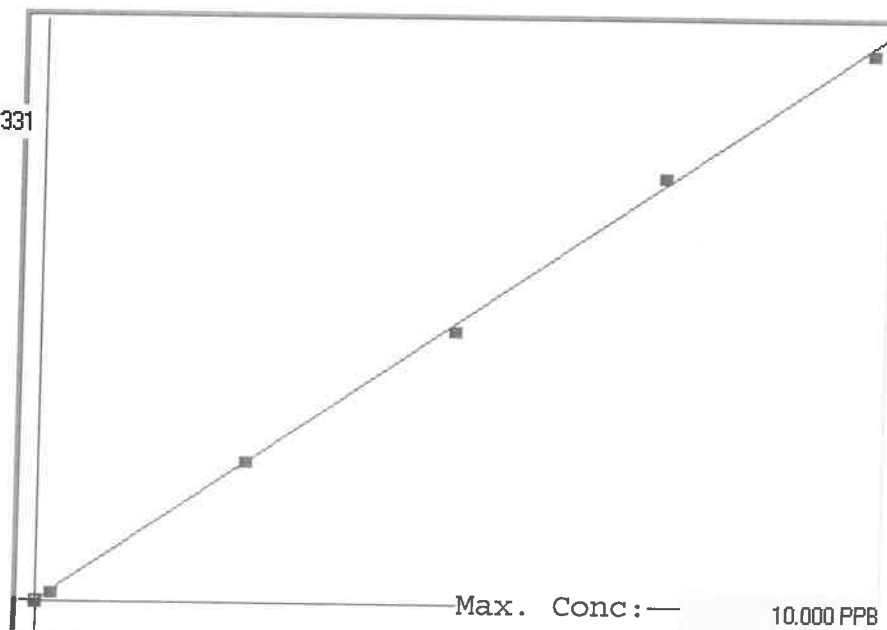

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	O/G
0.0	0.000	-0.005	-0.005	9	0.000	9	0				-
0.2	0.200	0.180	-0.020	686	0.0 %	686					10
2.5	2.500	2.538	0.038	9341	0.0 %	9341					2
5.0	5.000	4.913	-0.087	18057	0.0 %	18057					3
7.5	7.500	7.683	0.183	28222	0.0 %	28222					2
10.0	10.000	9.892	-0.108	36331	0.0 %	36331					-1

LB136036 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Jun 2025 09:14:06

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	9	-	0.0000	7470A	PPB	06 Jun 2025 09:48:36	S	Std
0.2 - 1	50.2	686	-	0.2000	7470A	PPB	06 Jun 2025 09:50:53	S	Std
2.5 - 1	52.5	9341	-	2.5000	7470A	PPB	06 Jun 2025 09:53:10	S	Std
5.0 - 1	55	18057	-	5.0000	7470A	PPB	06 Jun 2025 09:55:27	S	Std
7.5 - 1	55.5	28222	-	7.5000	7470A	PPB	06 Jun 2025 09:57:44	S	Std
10.0 - 1	31.6	36331	-	10.0000	7470A	PPB	06 Jun 2025 10:00:02	S	Std
ICV29 - 1	ICV29	13585	3.6943	-	7470A	PPB	06 Jun 2025 10:03:18	U	SMPL
ICB29 - 1	ICB29	-72	-0.0270	-	7470A	PPB	06 Jun 2025 10:05:33	U	SMPL
CCV08 - 1	CCV08	17437	4.7439	-	7470A	PPB	06 Jun 2025 10:07:50	U	SMPL
CCB08 - 1	CCB08	-149	-0.0480	-	7470A	PPB	06 Jun 2025 10:10:05	U	SMPL
CRA - 1	CRA	812	0.2139	-	7470A	PPB	06 Jun 2025 10:12:22	U	SMPL
HighStd - 1	HighStd	35704	9.7213	-	7470A	PPB	06 Jun 2025 10:14:38	U	SMPL
ChkStd - 1	ChkStd	24259	6.6027	-	7470A	PPB	06 Jun 2025 10:16:53	U	SMPL
PB168316BL - 1	PBW	-216	-0.0663	-	7470A	PPB	06 Jun 2025 10:19:11	U	SMPL
PB168316BS - 1	LCSW	13802	3.7534	-	7470A	PPB	06 Jun 2025 10:24:10	U	SMPL
Q2192-01 - 1	SB-1	-48	-0.0205	-	7470A	PPB	06 Jun 2025 10:26:26	U	SMPL
Q2194-02 - 1	COMP-12	43	0.0043	-	7470A	PPB	06 Jun 2025 10:28:44	U	SMPL
Q2194-04 - 1	COMP-13	262	0.0640	-	7470A	PPB	06 Jun 2025 10:31:01	U	SMPL
Q2198-02 - 1	B-202-SB02	55	0.0076	-	7470A	PPB	06 Jun 2025 10:33:17	U	SMPL
Q2198-04 - 1	B-207-SB02	49	0.0060	-	7470A	PPB	06 Jun 2025 10:35:33	U	SMPL
CCV09 - 1	CCV09	17947	4.8828	-	7470A	PPB	06 Jun 2025 10:37:48	U	SMPL
CCB09 - 1	CCB09	-231	-0.0703	-	7470A	PPB	06 Jun 2025 10:40:03	U	SMPL
Q2206-04 - 1	TP-1	18	-0.0025	-	7470A	PPB	06 Jun 2025 10:42:21	U	SMPL
Q2207-09 - 1	BU-703-COMP-01	42	0.0040	-	7470A	PPB	06 Jun 2025 10:44:36	U	SMPL
Q2207-18 - 1	BU-703-COMP-02	36	0.0024	-	7470A	PPB	06 Jun 2025 10:46:51	U	SMPL
Q2207-27 - 1	BU-703-COMP-03	47	0.0054	-	7470A	PPB	06 Jun 2025 10:49:07	U	SMPL
Q2207-36 - 1	BU-703-COMP-04	47	0.0054	-	7470A	PPB	06 Jun 2025 10:51:22	U	SMPL
Q2207-45 - 1	BU-703-COMP-05	20	-0.0019	-	7470A	PPB	06 Jun 2025 10:53:38	U	SMPL
Q2208-09 - 1	BU-703-COMP-06	41	0.0038	-	7470A	PPB	06 Jun 2025 10:55:55	U	SMPL
Q2208-18 - 1	BU-703-COMP-07	28	0.0002	-	7470A	PPB	06 Jun 2025 10:58:12	U	SMPL
Q2208-27 - 1	BU-703-COMP-08	28	0.0002	-	7470A	PPB	06 Jun 2025 11:00:28	U	SMPL
Q2208-36 - 1	BU-703-COMP-09	40	0.0035	-	7470A	PPB	06 Jun 2025 11:02:44	U	SMPL
CCV10 - 1	CCV10	17318	4.7114	-	7470A	PPB	06 Jun 2025 11:04:59	U	SMPL
CCB10 - 1	CCB10	-56	-0.0227	-	7470A	PPB	06 Jun 2025 11:07:15	U	SMPL
Q2208-36DUP - 1	BU-703-COMP-09DUP	23	-0.0011	-	7470A	PPB	06 Jun 2025 11:09:32	U	SMPL
Q2208-36MS - 1	BU-703-COMP-09MS	15129	4.1150	-	7470A	PPB	06 Jun 2025 11:11:48	U	SMPL
Q2208-36MSD - 1	BU-703-COMP-09MSD	15077	4.1008	-	7470A	PPB	06 Jun 2025 11:14:03	U	SMPL
PB168317BL - 1	PBW	-140	-0.0455	-	7470A	PPB	06 Jun 2025 11:16:21	U	SMPL
PB168317BS - 1	LCSW	12967	3.5259	-	7470A	PPB	06 Jun 2025 11:21:19	U	SMPL
Q2175-09DLX10 - 1	52725	1265	0.3373	-	7470A	PPB	06 Jun 2025 11:23:35	U	SMPL
Q2198-05 - 1	B-202-GW01	1164	0.3098	-	7470A	PPB	06 Jun 2025 11:25:53	U	SMPL
Q2210-01 - 1	TW1	457	0.1171	-	7470A	PPB	06 Jun 2025 11:28:12	U	SMPL
Q2216-02 - 1	3887	50	0.0062	-	7470A	PPB	06 Jun 2025 11:30:29	U	SMPL
Q2216-02DUP - 1	3887DUP	66	0.0106	-	7470A	PPB	06 Jun 2025 11:32:44	U	SMPL
CCV11 - 1	CCV11	16711	4.5461	-	7470A	PPB	06 Jun 2025 11:41:10	U	SMPL
CCB11 - 1	CCB11	-20	-0.0128	-	7470A	PPB	06 Jun 2025 11:43:26	U	SMPL
Q2216-02MS - 1	3887MS	15285	4.1575	-	7470A	PPB	06 Jun 2025 11:48:21	U	SMPL
Q2216-02MSD - 1	3887MSD	13436	3.6537	-	7470A	PPB	06 Jun 2025 11:50:36	U	SMPL
Q2216-03 - 1	3888	-27	-0.0148	-	7470A	PPB	06 Jun 2025 11:52:53	U	SMPL
Q2216-04 - 1	3864	77	0.0136	-	7470A	PPB	06 Jun 2025 11:55:10	U	SMPL
Q2216-05 - 1	3865	-7	-0.0093	-	7470A	PPB	06 Jun 2025 11:57:26	U	SMPL
Q2216-06 - 1	3851	44	0.0046	-	7470A	PPB	06 Jun 2025 12:01:59	U	SMPL
Q2218-03 - 1	3309	342	0.0858	-	7470A	PPB	06 Jun 2025 12:04:16	U	SMPL
Q2221-02 - 1	34900	1149	0.3057	-	7470A	PPB	06 Jun 2025 12:06:33	U	SMPL
CCV12 - 1	CCV12	17551	4.7749	-	7470A	PPB	06 Jun 2025 12:08:51	U	SMPL
CCB12 - 1	CCB12	-63	-0.0246	-	7470A	PPB	06 Jun 2025 12:11:09	U	SMPL
PB168271TB - 1	PB168271TB	-2	-0.0079	-	7470A	PPB	06 Jun 2025 12:13:24	U	SMPL
Q2208-36LX5 - 1		-2	-0.0079	-	7470A	PPB	06 Jun 2025 12:20:13	U	SMPL
Q2208-36A - 1		12341	3.3553	-	7470A	PPB	06 Jun 2025 12:22:28	U	SMPL
Q2216-02LX5 - 1		-73	-0.0273	-	7470A	PPB	06 Jun 2025 12:24:45	U	SMPL
Q2216-02A - 1		14019	3.8125	-	7470A	PPB	06 Jun 2025 12:33:42	U	SMPL
CCV13 - 1	CCV13	18753	5.1025	-	7470A	PPB	06 Jun 2025 12:35:58	U	SMPL
CCB13 - 1	CCB13	-69	-0.0262	-	7470A	PPB			