

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060425\
 Data File : P0111473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2025 16:52
 Operator : YP/AJ
 Sample : Q2198-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-207-SB02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/05/2025
 Supervised By :mohammad ahmed 06/06/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:43:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.677	3.675	111.5E6	95470208	18.950	17.513
2) SA Decachlor...	8.713	8.664	59323512	20332372	11.490m	10.990m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060425\
Data File : PO111473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2025 16:52
Operator : YP/AJ
Sample : Q2198-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B-207-SB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/05/2025
Supervised By :mohammad ahmed 06/06/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:43:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

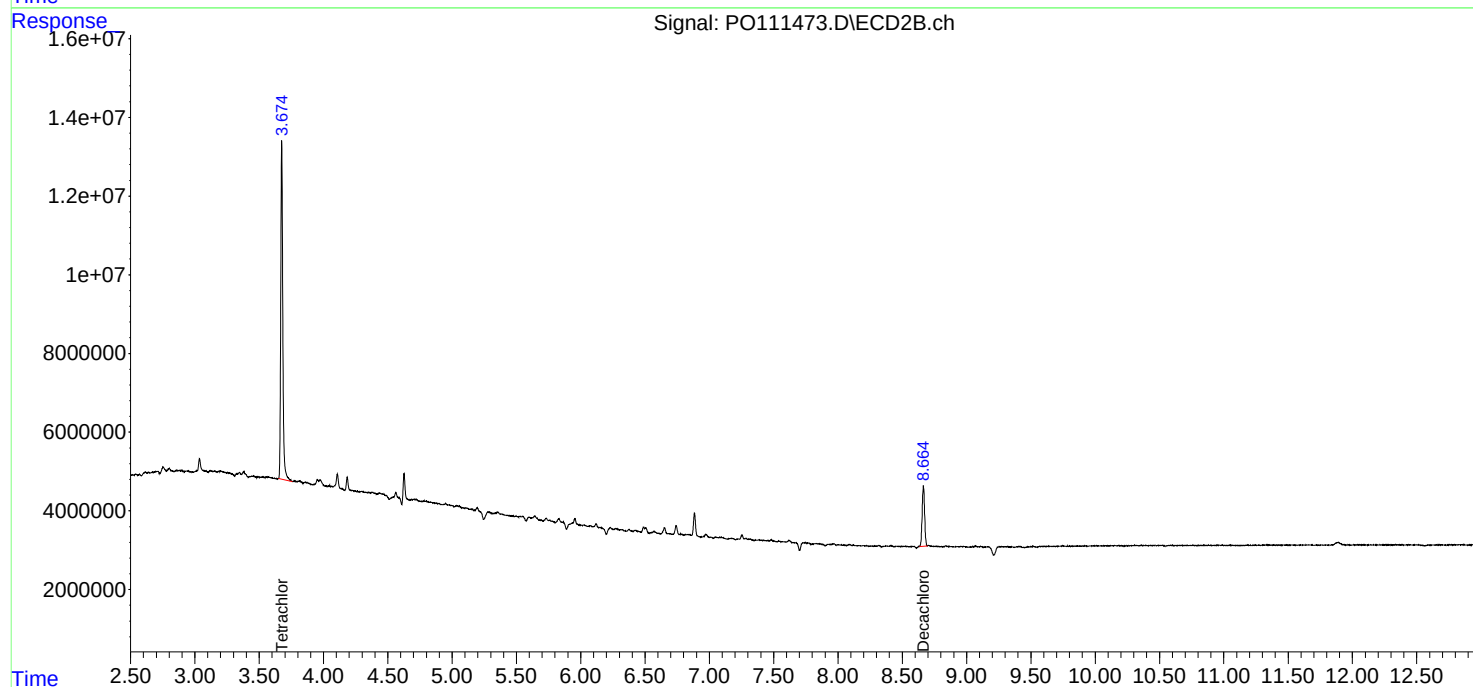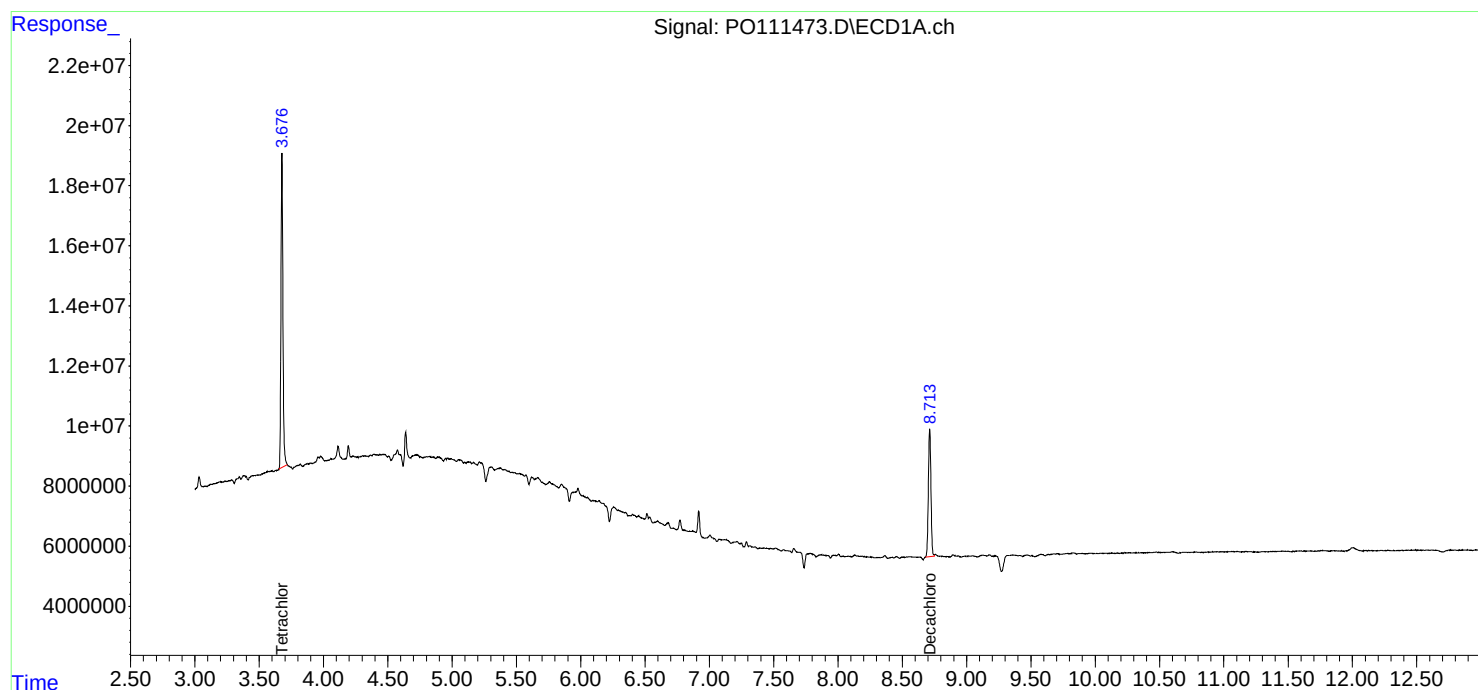

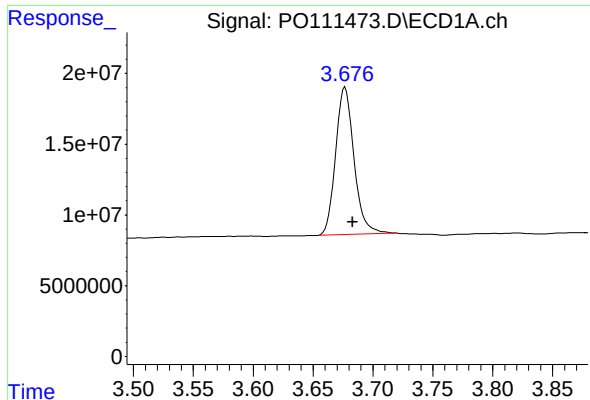


#1 Tetrachloro-m-xylene

R.T.: 3.677 min
Delta R.T.: -0.006 min
Response: 111487366
Conc: 18.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-207-SB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/05/2025
Supervised By :mohammad ahmed 06/06/2025

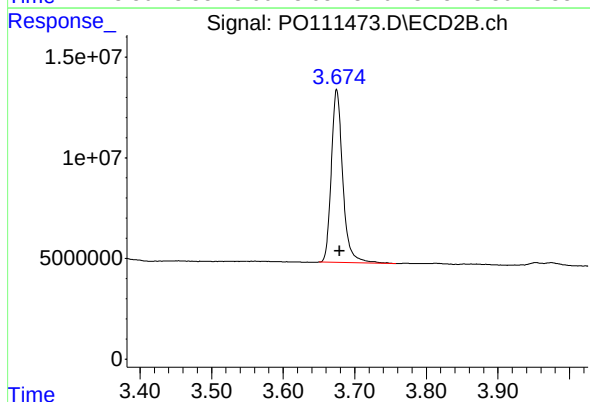


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.004 min
Response: 95470208
Conc: 17.51 ng/ml

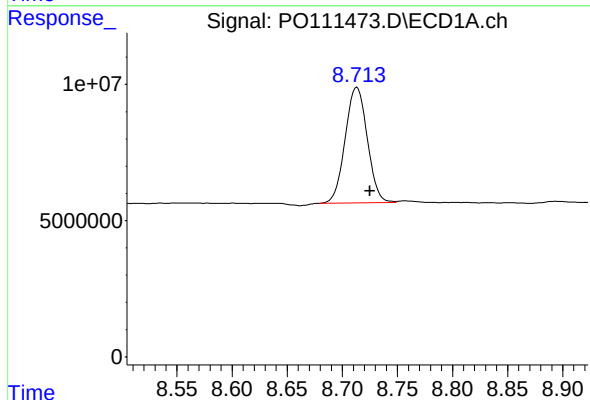

#2 Decachlorobiphenyl

R.T.: 8.713 min
Delta R.T.: -0.012 min
Response: 59323512
Conc: 11.49 ng/ml m

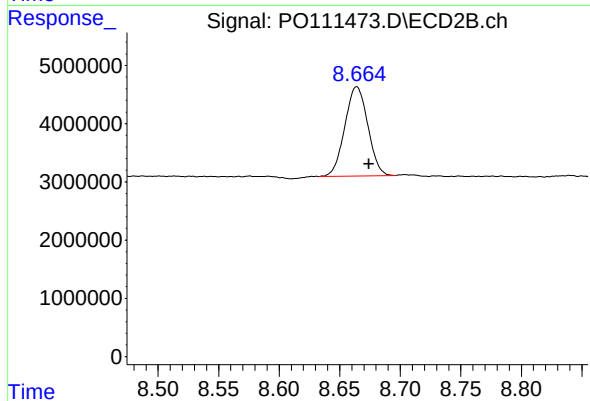

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: -0.010 min
Response: 20332372
Conc: 10.99 ng/ml m