
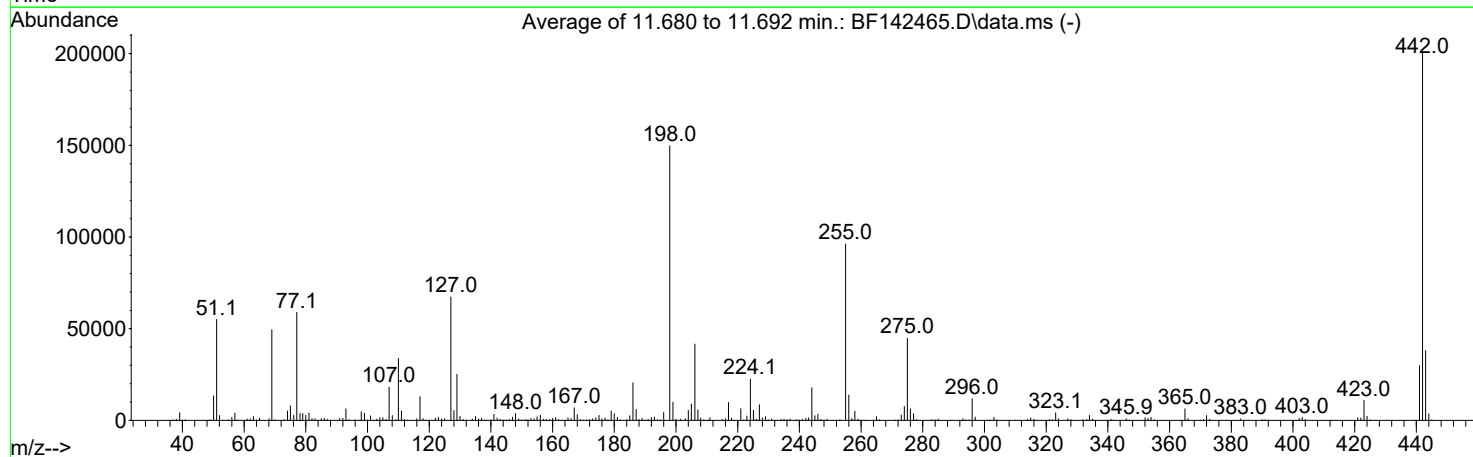


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052025\
Data File : BF142465.D
Acq On : 20 May 2025 11:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

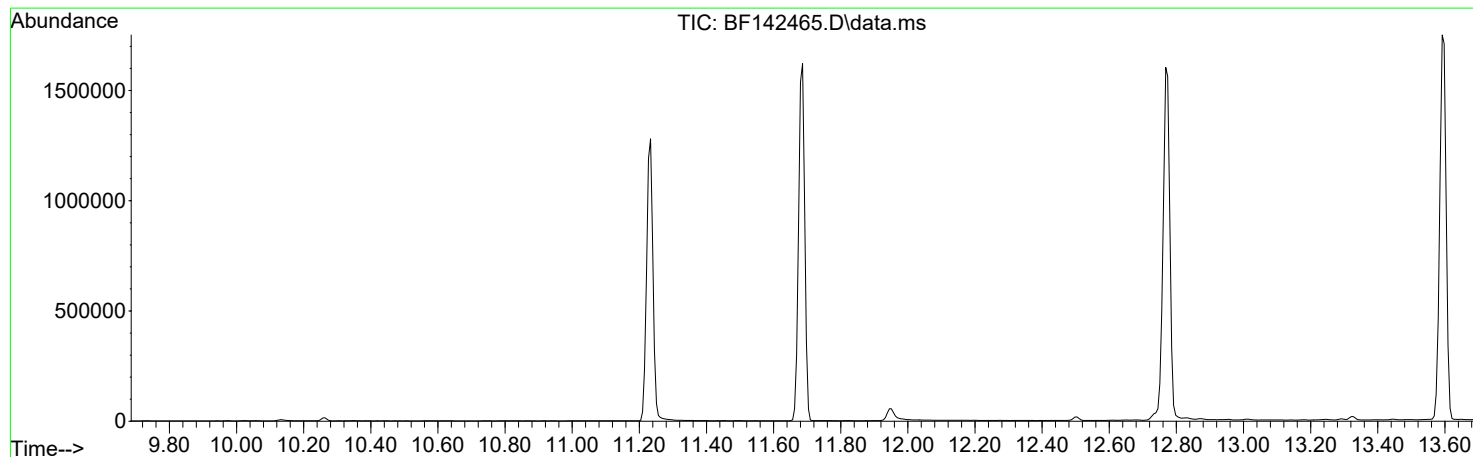

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	55035	PASS
68	69	0.00	2	1.9	918	PASS
69	198	0.00	100	33.1	49499	PASS
70	69	0.00	2	0.5	254	PASS
127	198	10	80	44.9	67277	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149731	PASS
199	198	5	9	6.6	9853	PASS
275	198	10	60	29.9	44779	PASS
365	198	1	100	4.2	6269	PASS
441	198	0.01	100	19.9	29837	PASS
442	442	50	100	100.0	200661	PASS
443	442	15	24	19.0	38045	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/20/2025	BNA_F	<u>BF142465.D</u>
Compound Name	Response	Retention Time
DDT	467874	13.598
DDD	6363	13.327
DDE	709	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7072	474946	1.49

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052025\
Data File : BF142465.D
Acq On : 20 May 2025 11:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 20 14:09:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

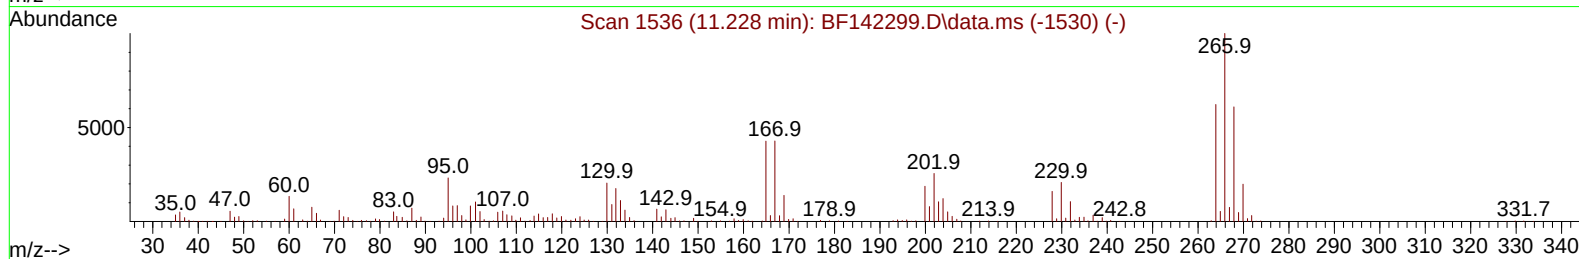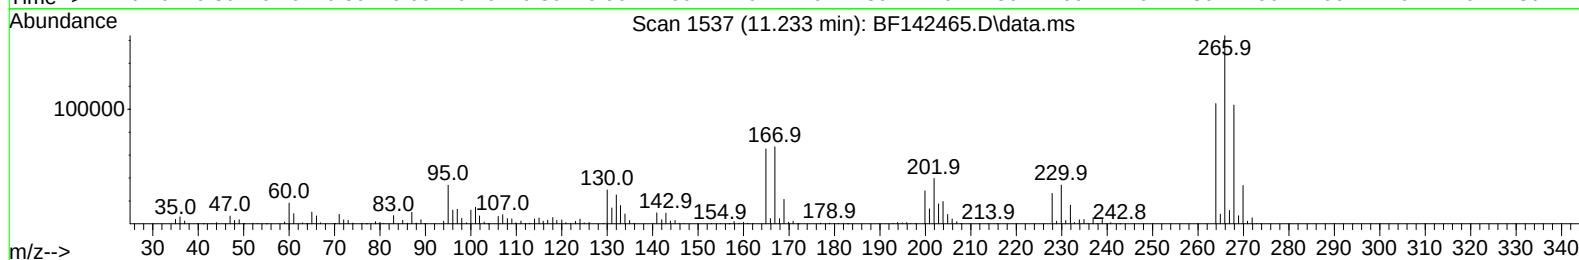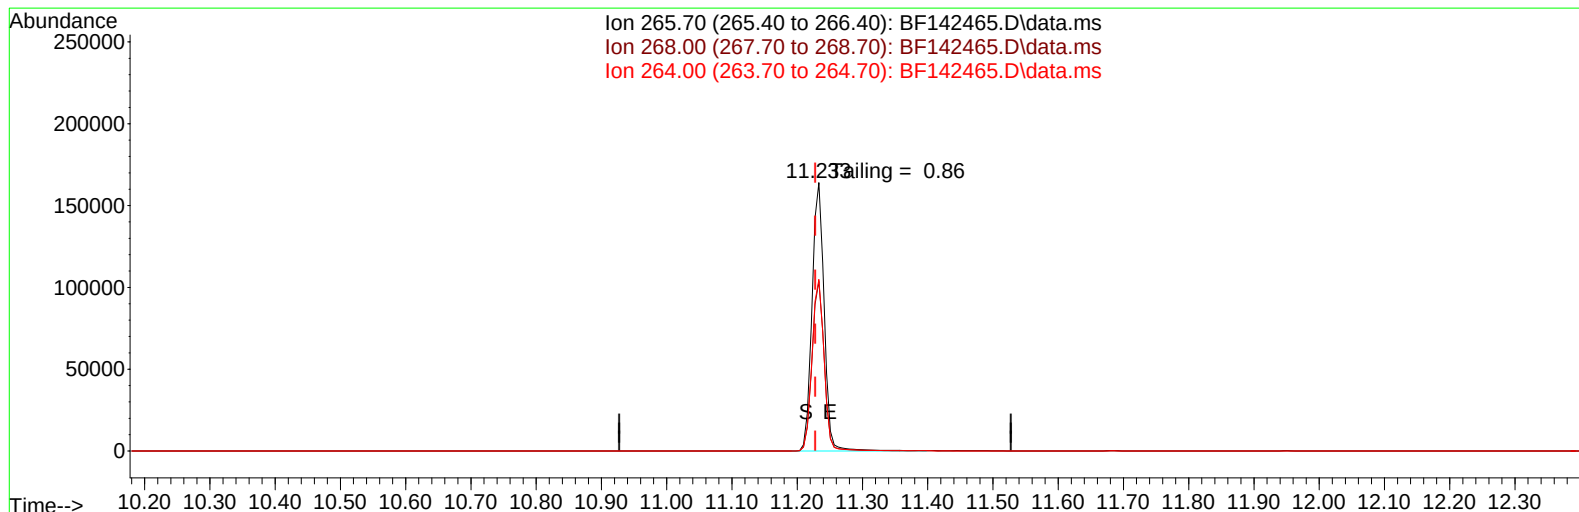

TIC: BF142465.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 45340.77 ng

response 213501

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	63.21
264.00	62.20	63.93
0.00	0.00	0.00

