
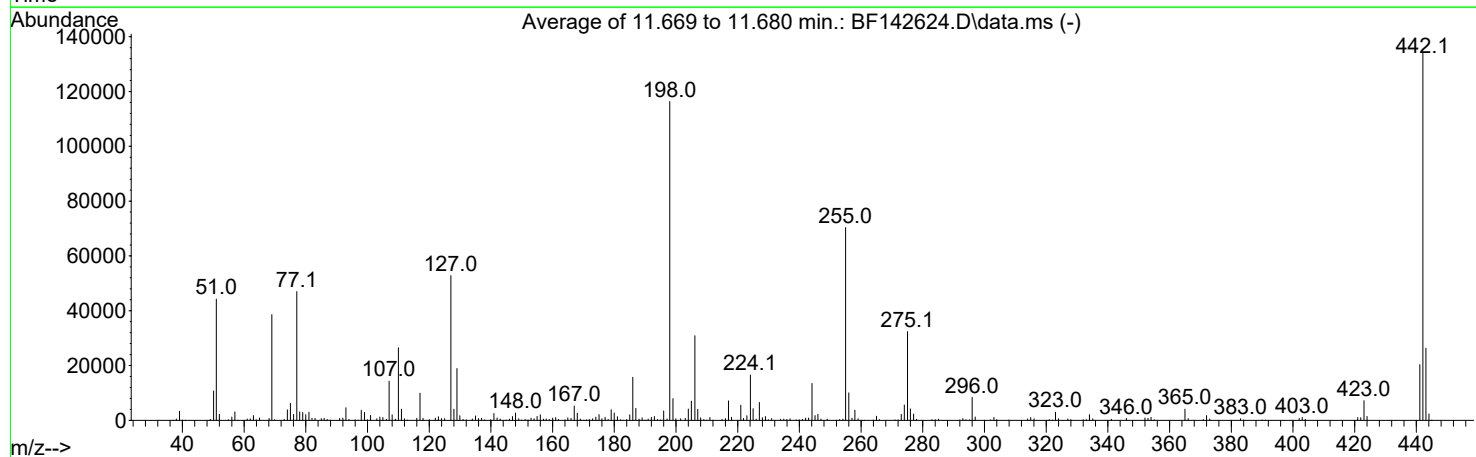


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060525\
Data File : BF142624.D
Acq On : 05 Jun 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

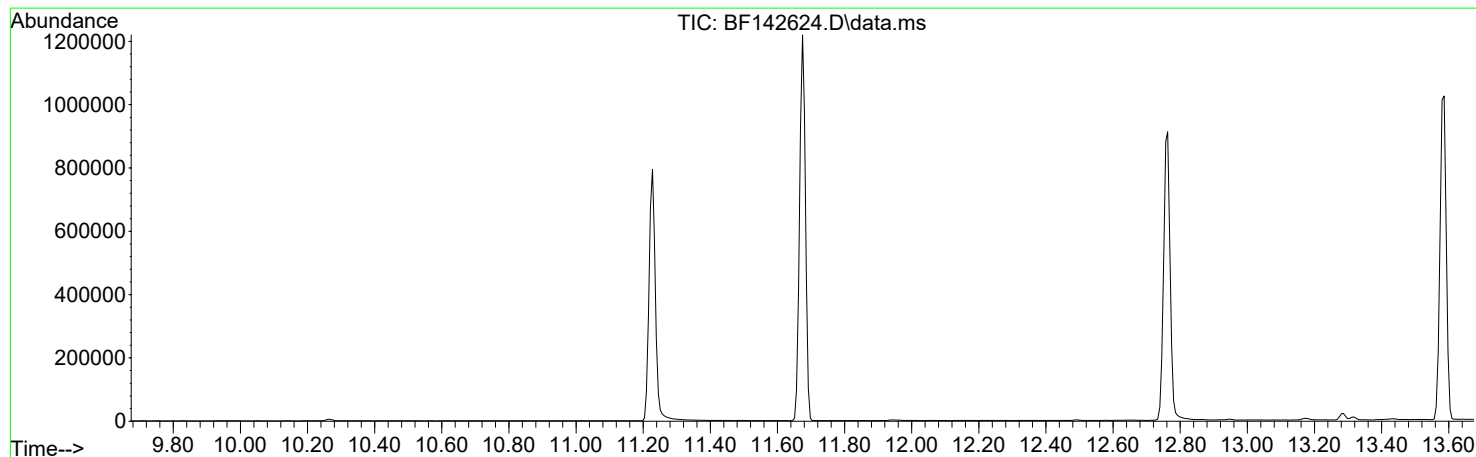

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	38.0	44267	PASS
68	69	0.00	2	1.8	691	PASS
69	198	0.00	100	33.2	38579	PASS
70	69	0.00	2	0.6	236	PASS
127	198	10	80	45.4	52819	PASS
197	198	0.00	2	0.5	550	PASS
198	198	100	100	100.0	116347	PASS
199	198	5	9	6.8	7924	PASS
275	198	10	60	27.9	32424	PASS
365	198	1	100	3.5	4075	PASS
441	198	0.01	100	17.5	20310	PASS
442	442	50	100	100.0	134237	PASS
443	442	15	24	19.6	26320	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/3/2025	BNA_F	<u>BF142601.D</u>
Compound Name	Response	Retention Time
DDT	279286	13.586
DDD	6433	13.286
DDE	730	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7163	286449	2.50

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060525\
Data File : BF142624.D
Acq On : 05 Jun 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 05 12:57:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

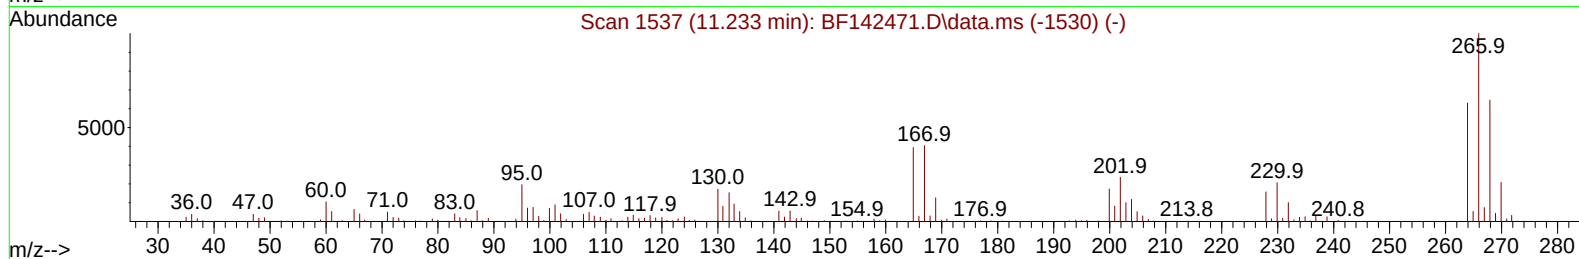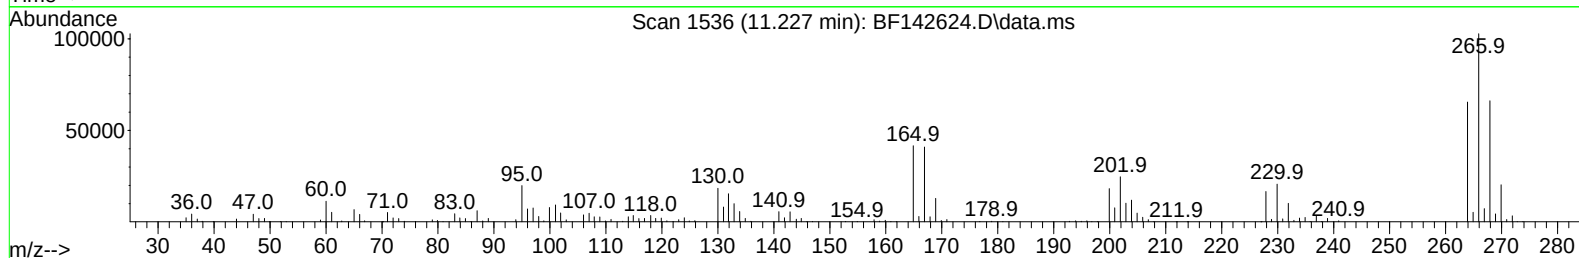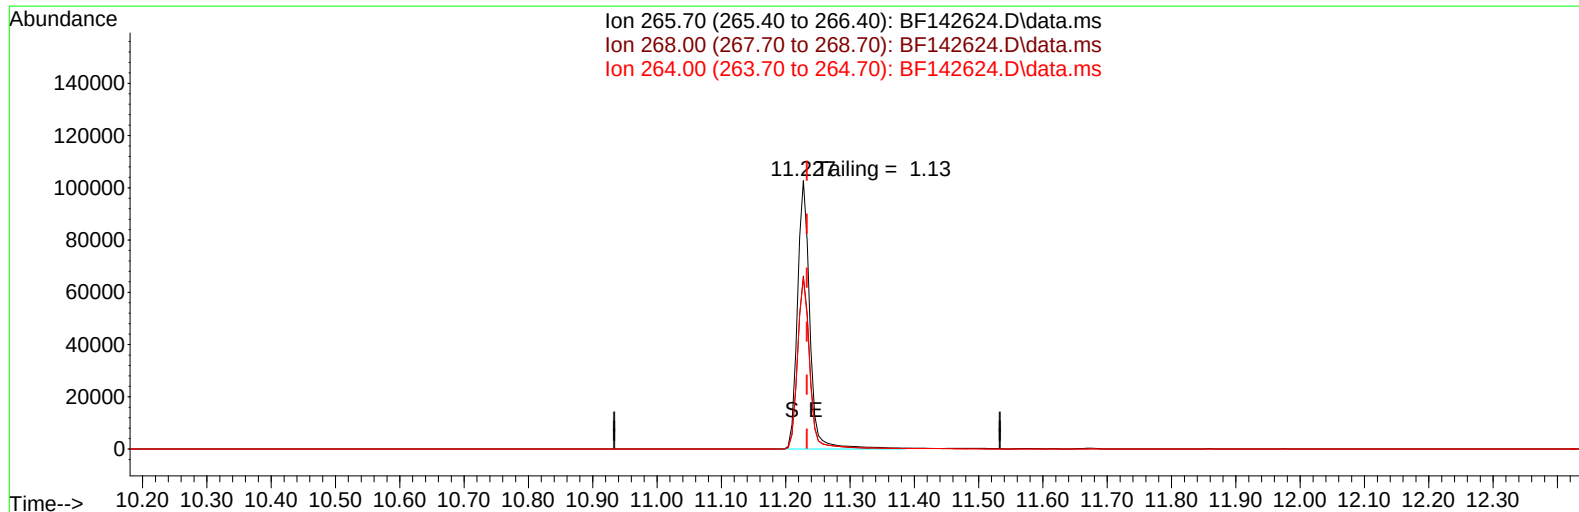

TIC: BF142624.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 0.00 ng




response 138743

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.43
264.00	63.00	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060525\
Data File : BF142624.D
Acq On : 05 Jun 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 05 12:57:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

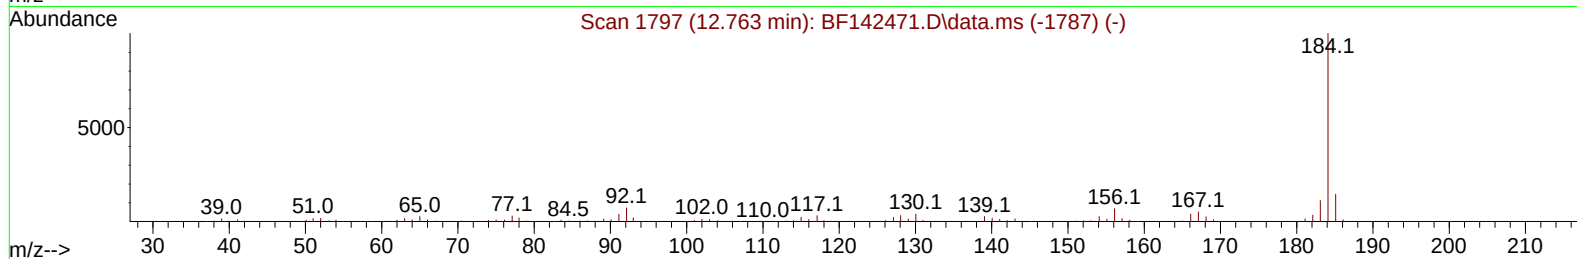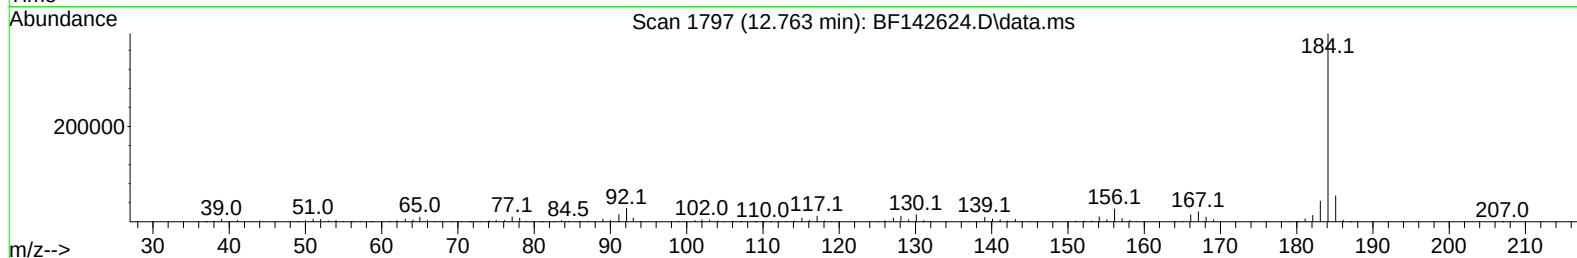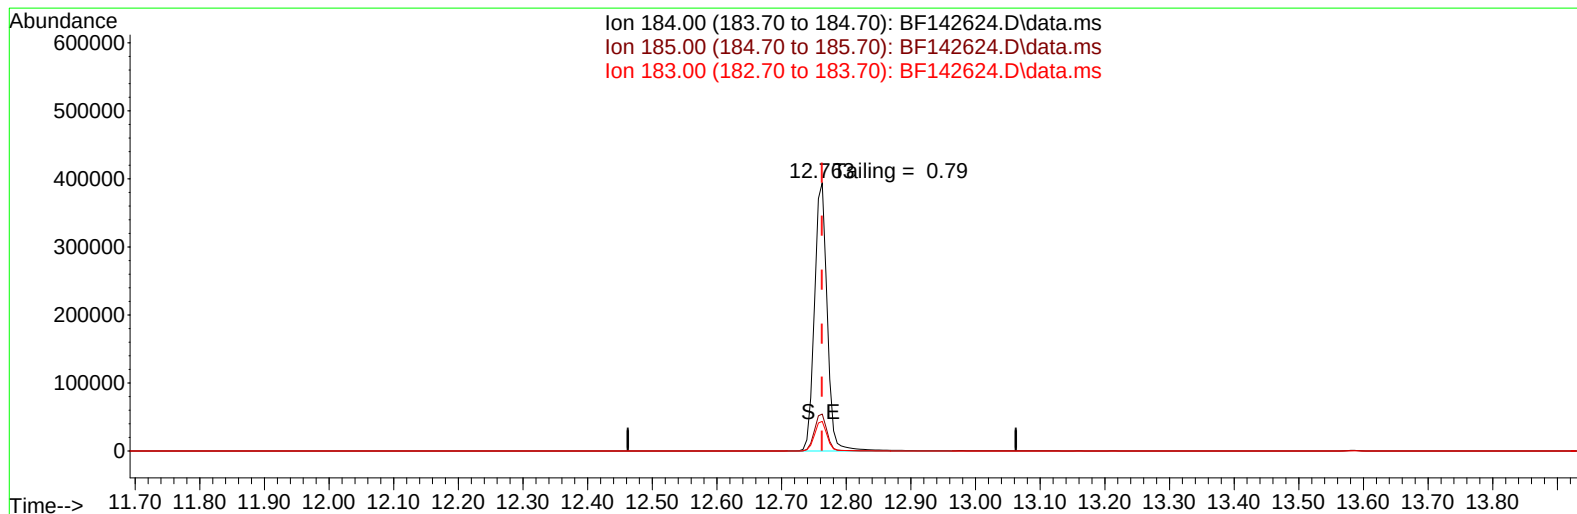

TIC: BF142624.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 543002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.80
183.00	11.20	11.04
0.00	0.00	0.00