
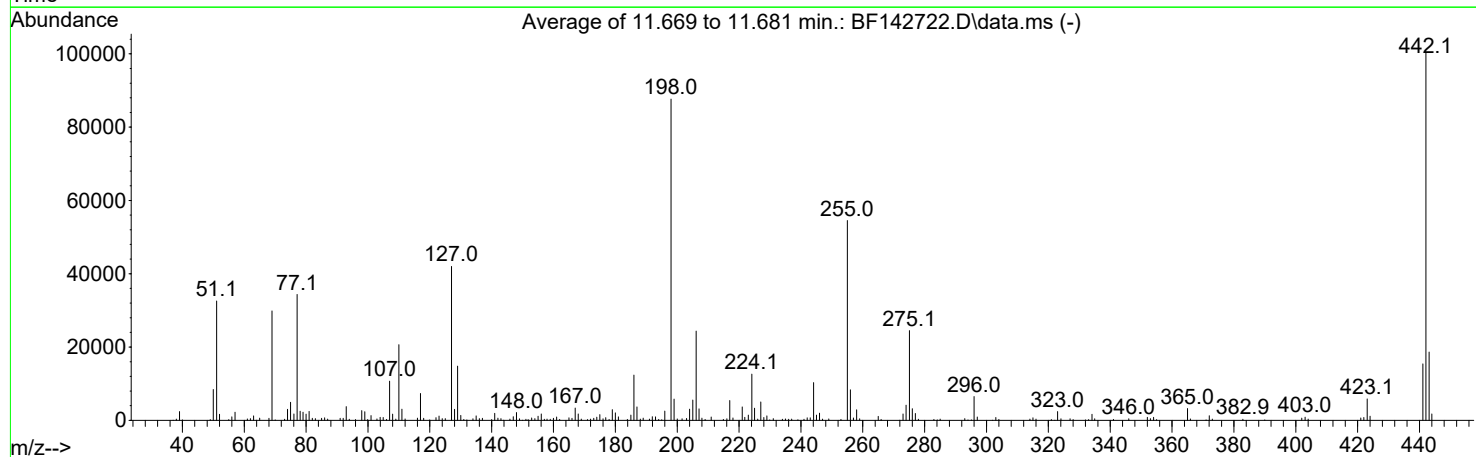


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142722.D
Acq On : 11 Jun 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 11 05:56:09 2025

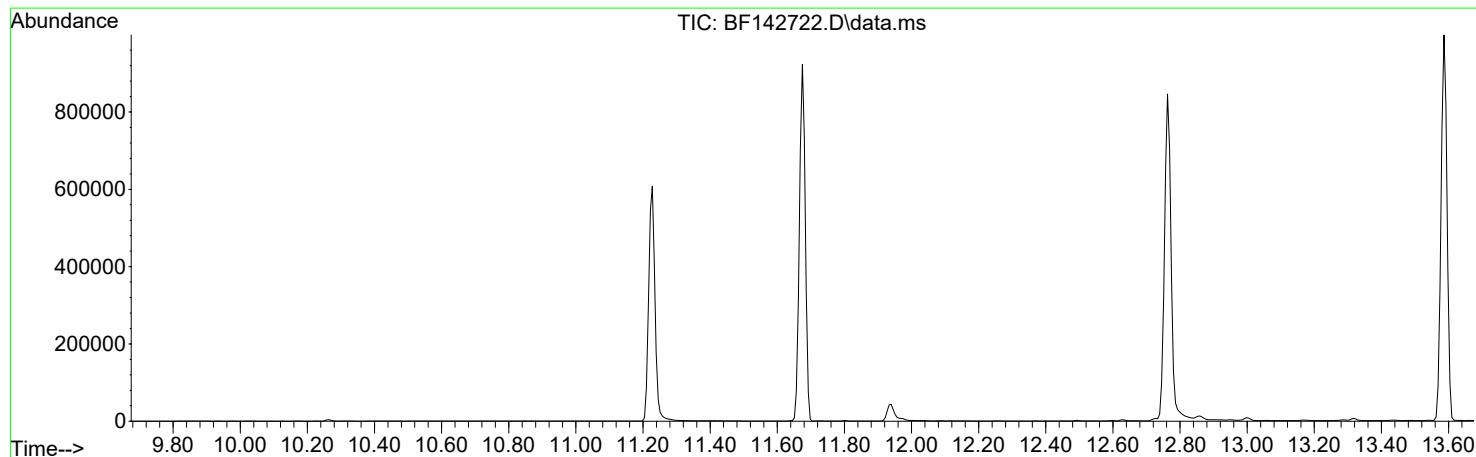

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	32576	PASS
68	69	0.00	2	1.9	580	PASS
69	198	0.00	100	34.1	29851	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	47.9	41997	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87651	PASS
199	198	5	9	6.6	5826	PASS
275	198	10	60	27.9	24485	PASS
365	198	1	100	3.7	3221	PASS
441	198	0.01	100	17.6	15408	PASS
442	442	50	100	100.0	100365	PASS
443	442	15	24	18.6	18630	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/11/2025	BNA_F	<u>BF142722.D</u>
Compound Name	Response	Retention Time
DDT	254780	13.586
DDD	3377	13.316
DDE	546	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3923	258703	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142722.D
Acq On : 11 Jun 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 11 11:00:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

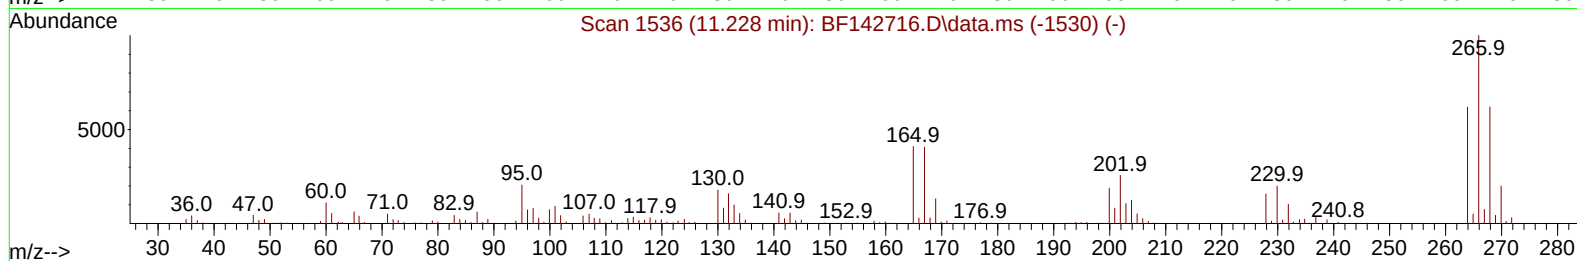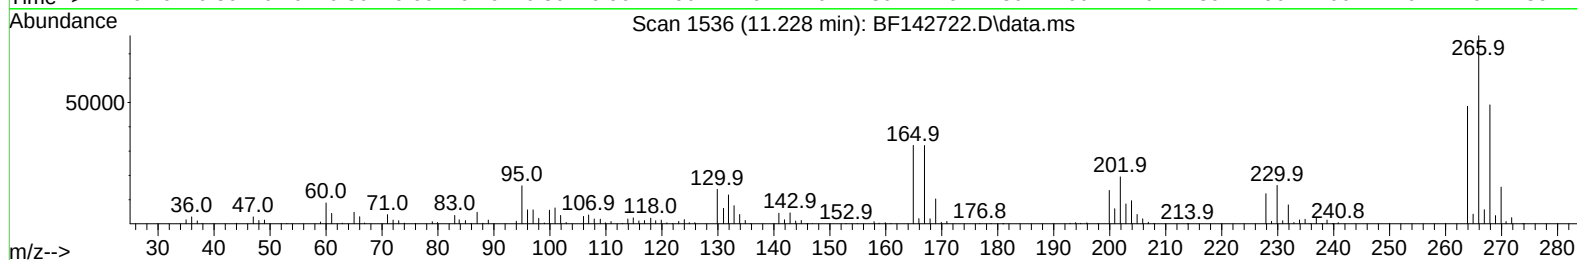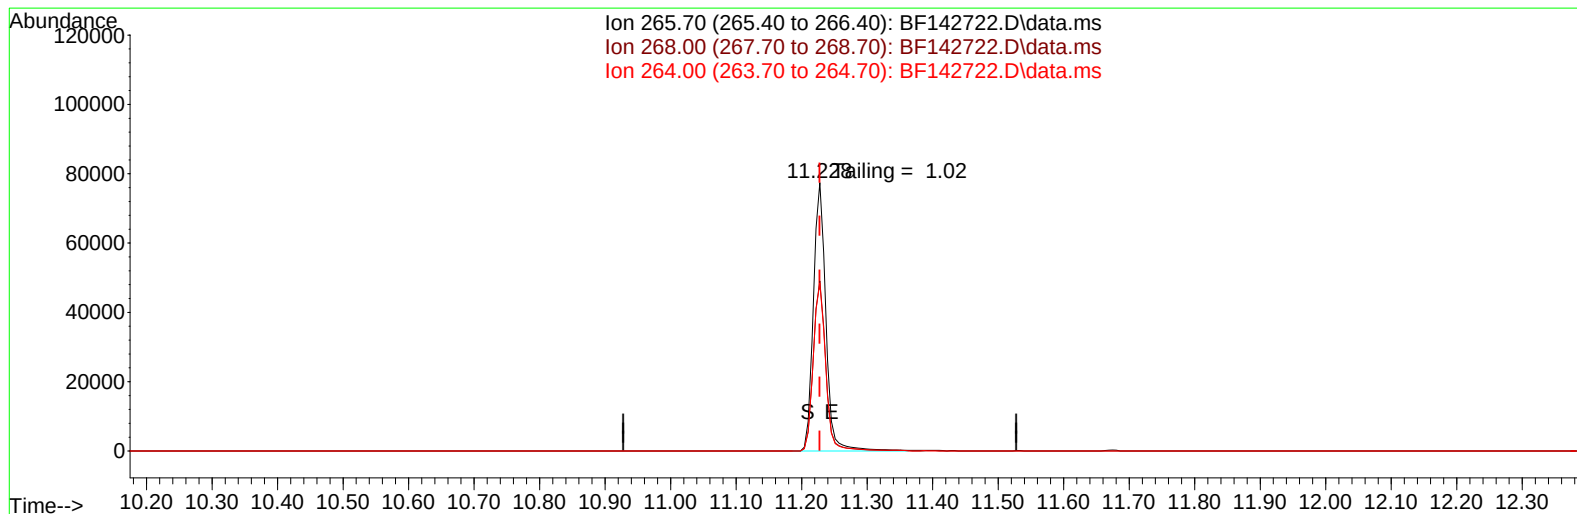

TIC: BF142722.D\data.ms

(70) Pentachlorophenol (C)

11.228min (+ 0.000) 36233.28 ng




response 103277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	63.33
264.00	61.90	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142722.D
Acq On : 11 Jun 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 11 11:00:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

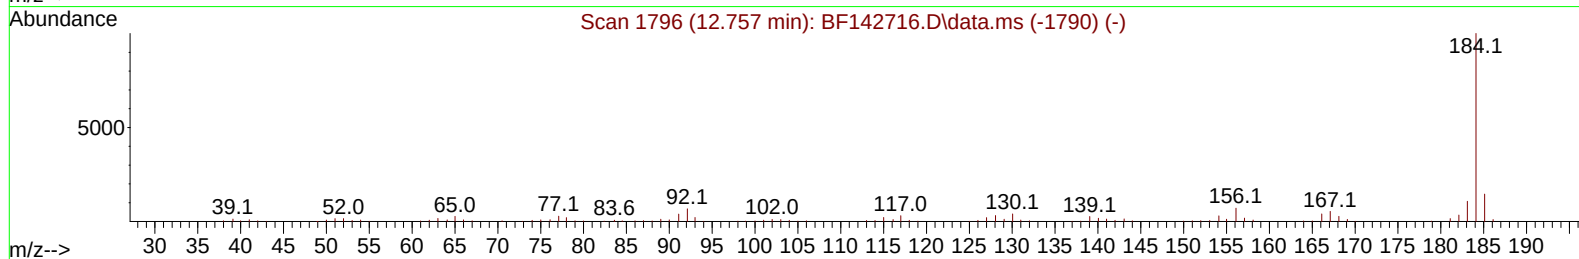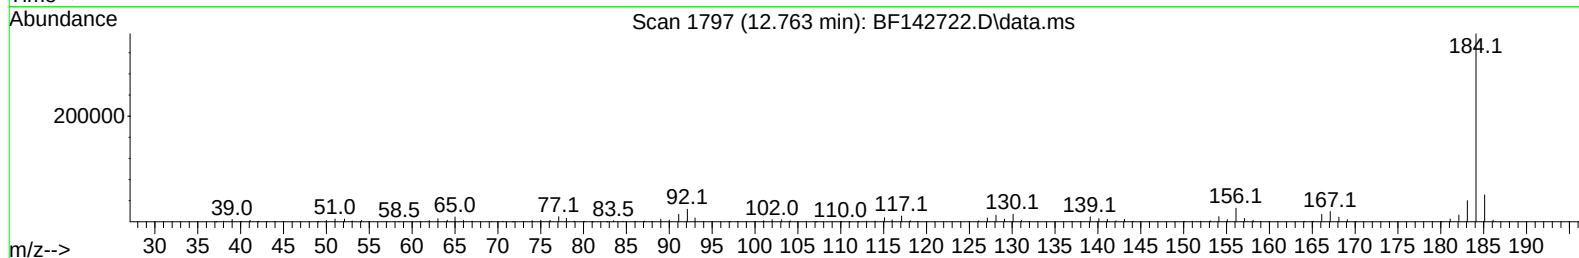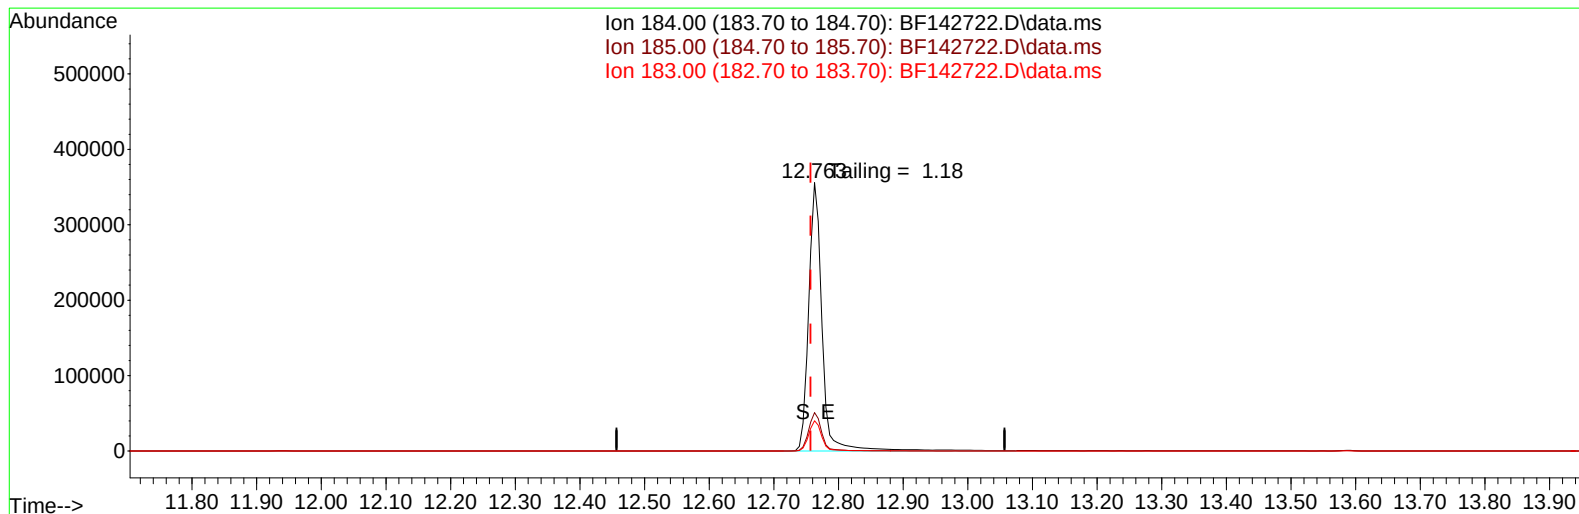

TIC: BF142722.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 11814.89 ng

response 510816

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	10.70	11.31
0.00	0.00	0.00