


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050205.D
Acq On : 06 Jun 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 05 16:20:25 2025

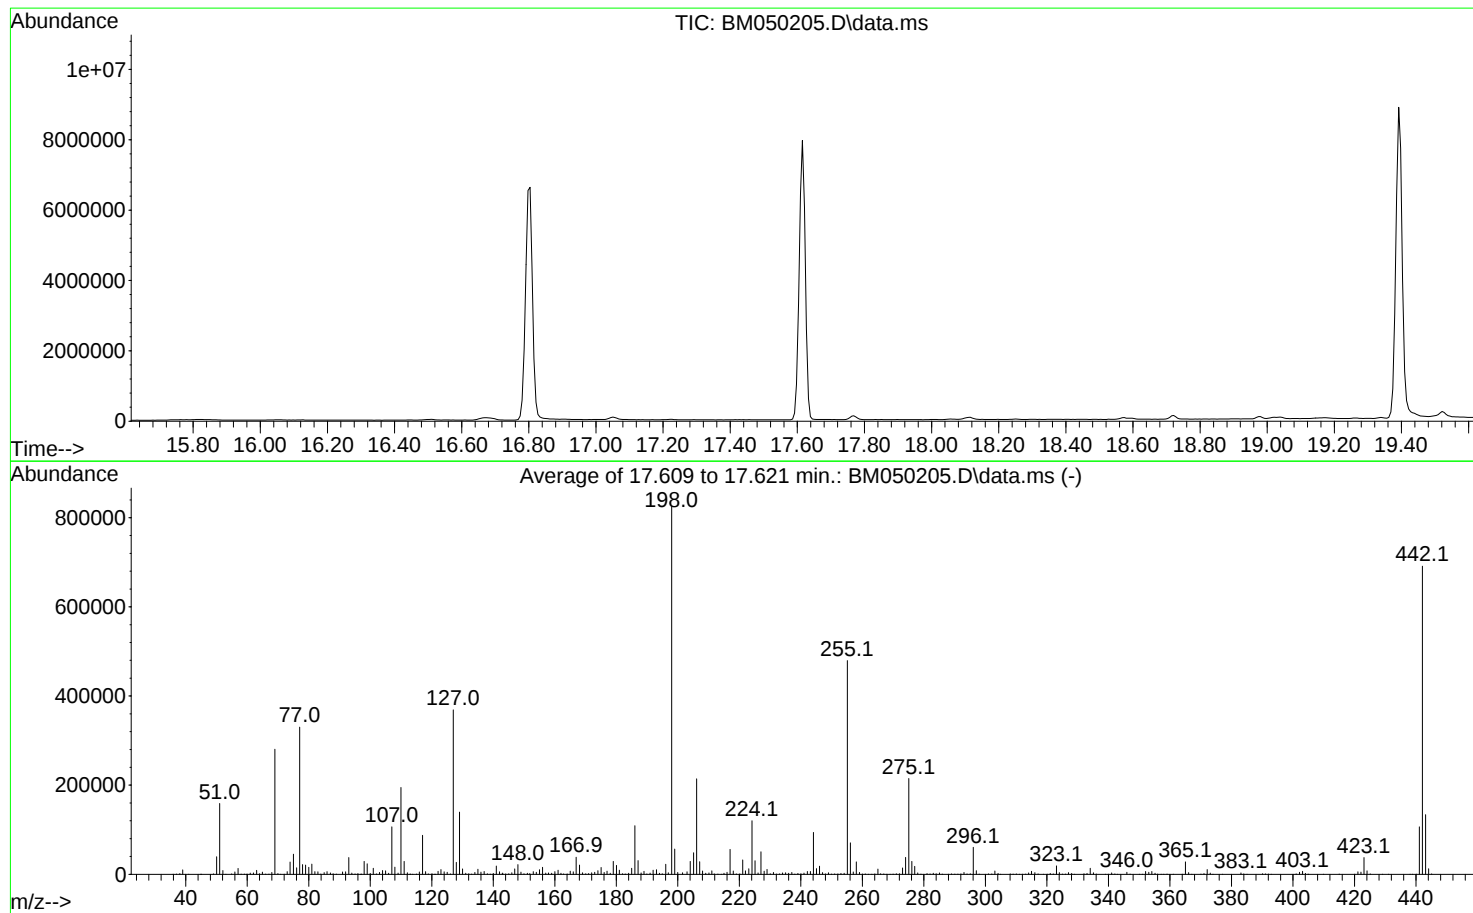




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.3	158878	PASS
68	69	0.00	2	1.5	4204	PASS
69	198	0.00	100	34.0	280427	PASS
70	69	0.00	2	0.6	1554	PASS
127	198	10	80	44.7	369024	PASS
197	198	0.00	2	0.4	3387	PASS
198	198	100	100	100.0	825301	PASS
199	198	5	9	6.8	56509	PASS
275	198	10	60	26.0	214848	PASS
365	198	1	100	3.4	27976	PASS
441	198	0.01	100	12.9	106333	PASS
442	442	50	100	100.0	691392	PASS
443	442	15	24	19.4	133885	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050205.D
Acq On : 06 Jun 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 06 10:51:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

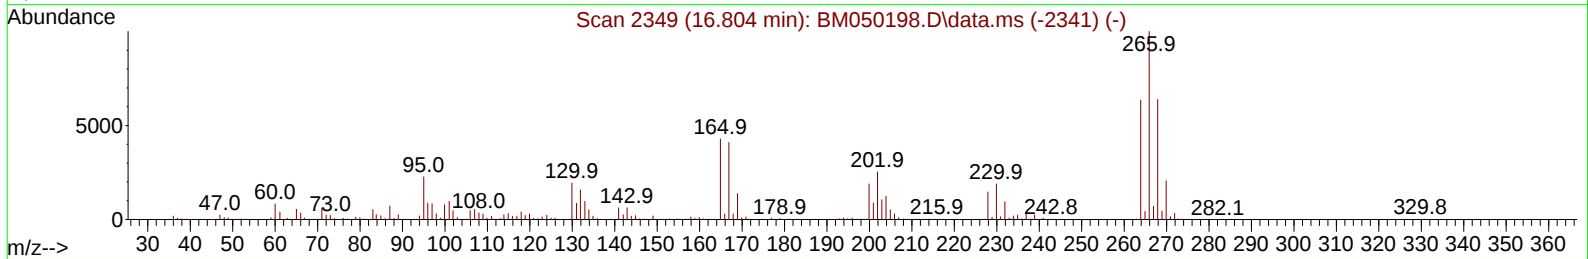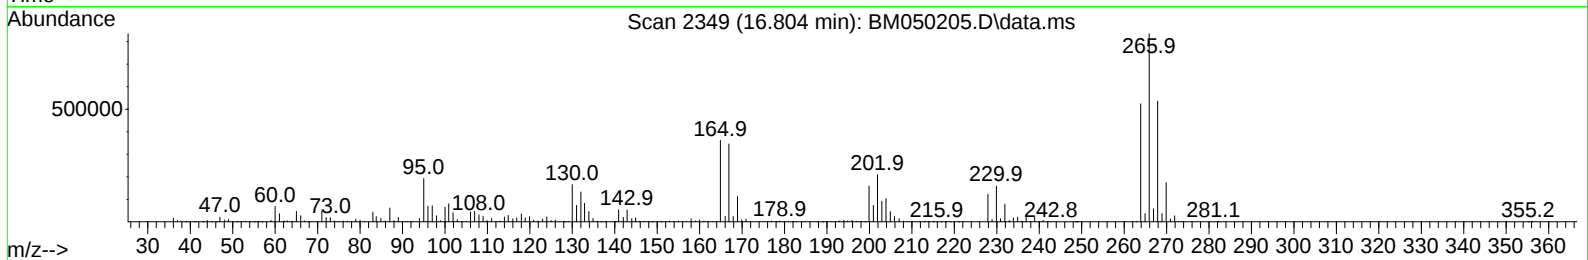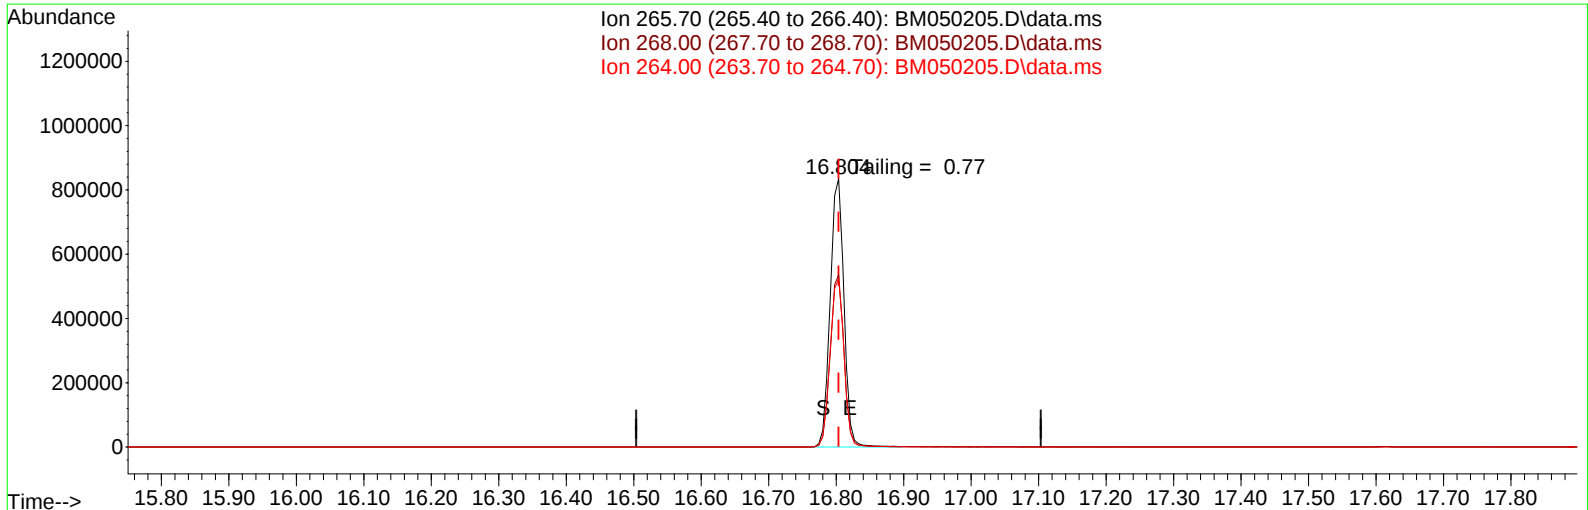

TIC: BM050205.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.000) 651895.98 ng




response 1182854

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.16
264.00	63.50	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060625\
Data File : BM050205.D
Acq On : 06 Jun 2025 08:50
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 06 10:51:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

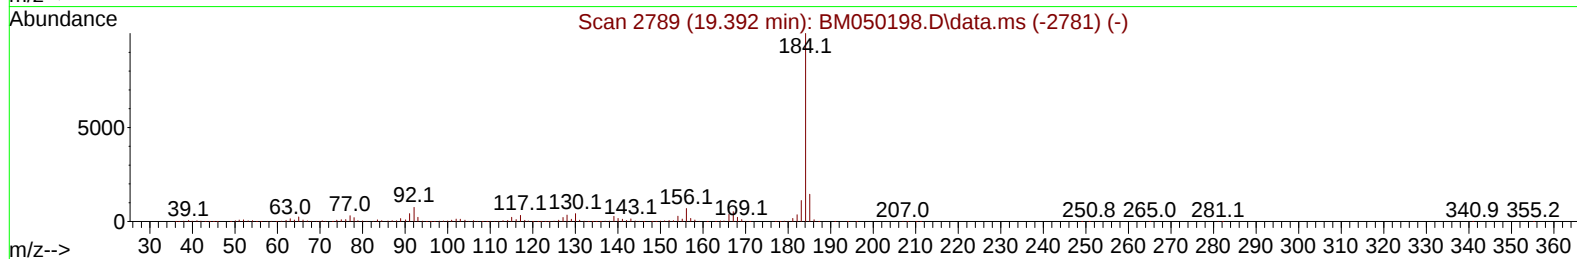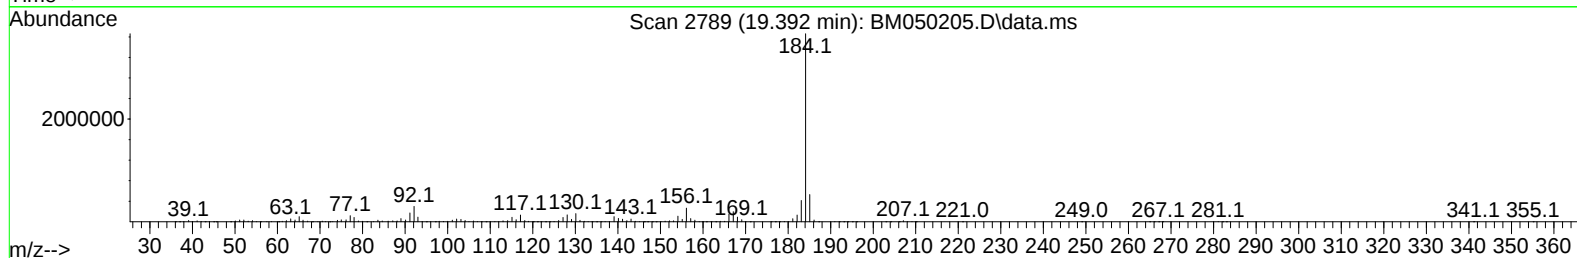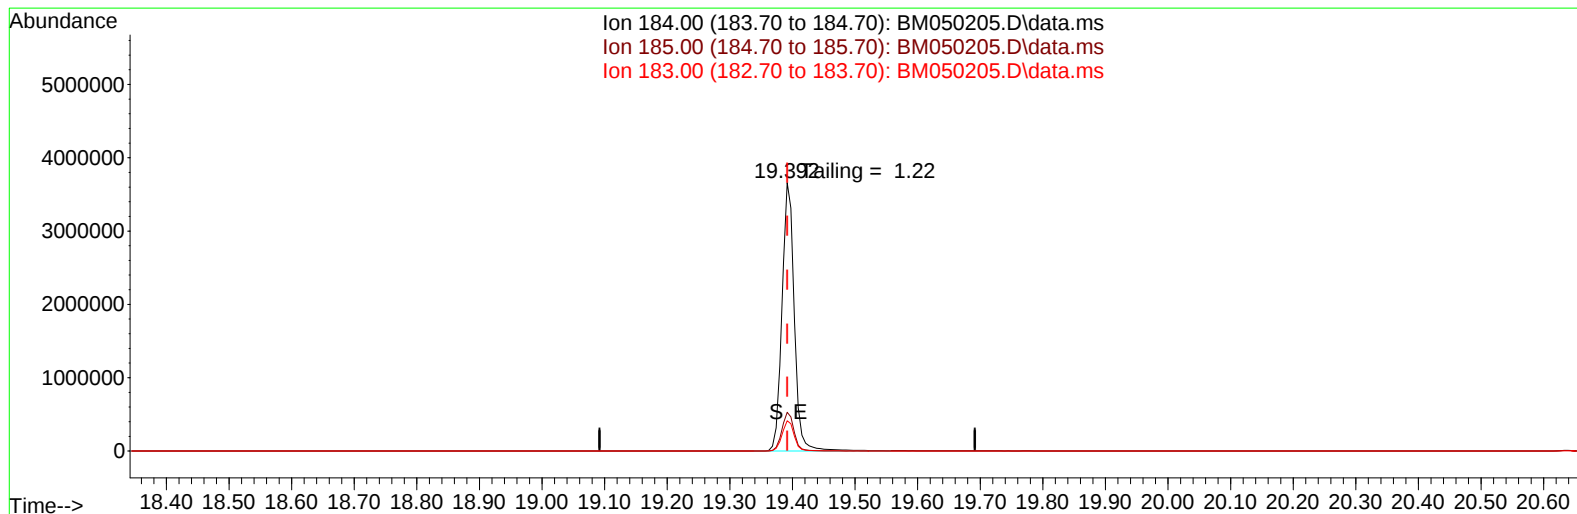

TIC: BM050205.D\data.ms

(77) Benzidine

19.392min (-0.000) 12050.92 ng

response 5030019

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.46
183.00	11.20	11.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/6/2025	BNA_M	<u>BM050205.D</u>
Compound Name	Response	Retention Time
DDT	2500193	20.639
DDD	30877	20.25
DDE	2038	19.686
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32915	2533108	1.30

Instrument :
BNA_M
ClientSampleId :
DFTPP