
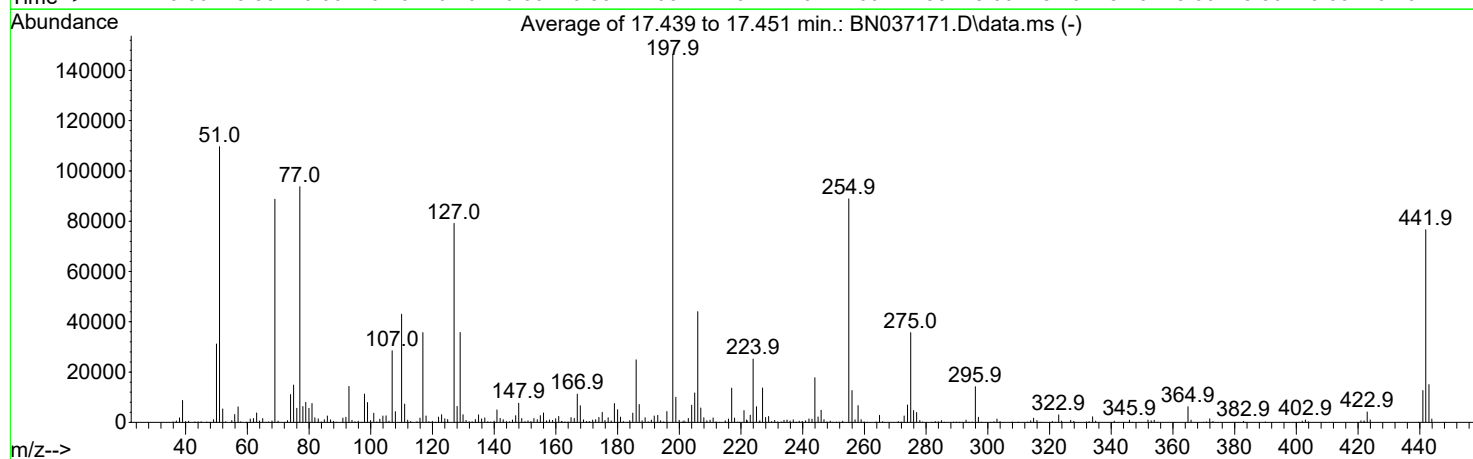


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037171.D
Acq On : 05 Jun 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 04 01:52:03 2025

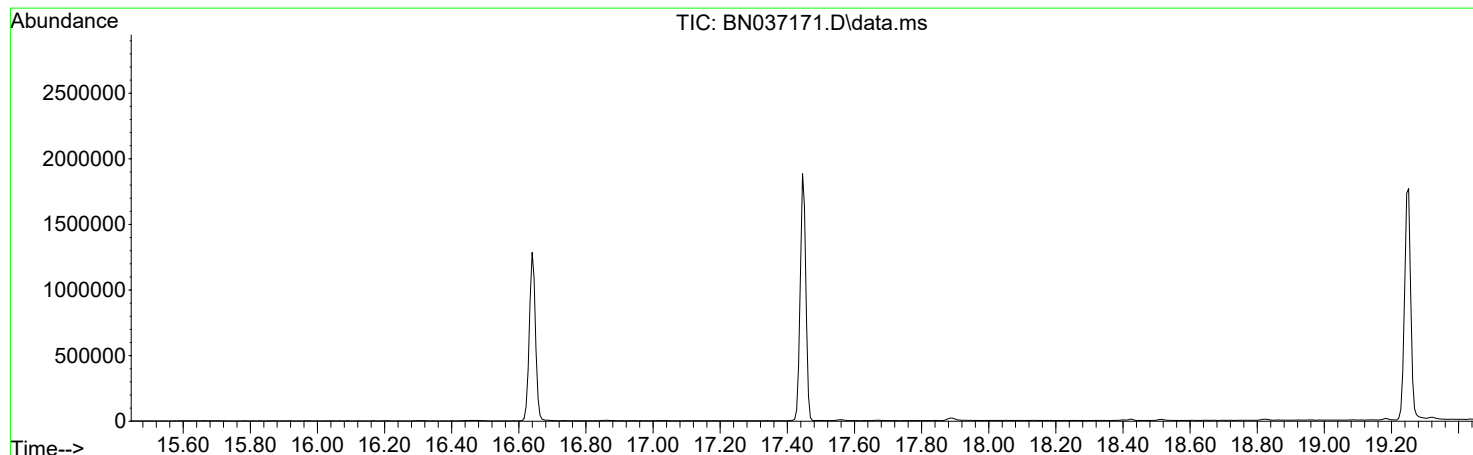

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	74.9	109648	PASS
68	69	0.00	2	0.7	598	PASS
69	198	0.00	100	60.7	88808	PASS
70	69	0.00	2	0.6	492	PASS
127	198	10	80	54.1	79149	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146312	PASS
199	198	5	9	6.8	9995	PASS
275	198	10	60	24.4	35715	PASS
365	198	1	100	4.3	6223	PASS
441	198	0.01	100	8.7	12664	PASS
442	442	50	100	100.0	76632	PASS
443	442	15	24	19.6	15055	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/5/2025	BNA_N	<u>BN037171.D</u>
Compound Name	Response	Retention Time
DDT	480704	20.492
DDD	7476	20.098
DDE	585	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8061	488765	1.65

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037171.D
Acq On : 05 Jun 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 05 19:08:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

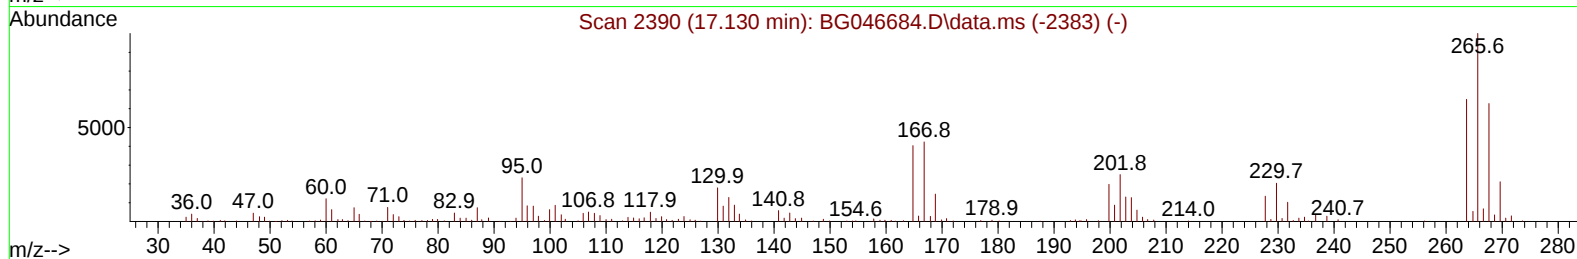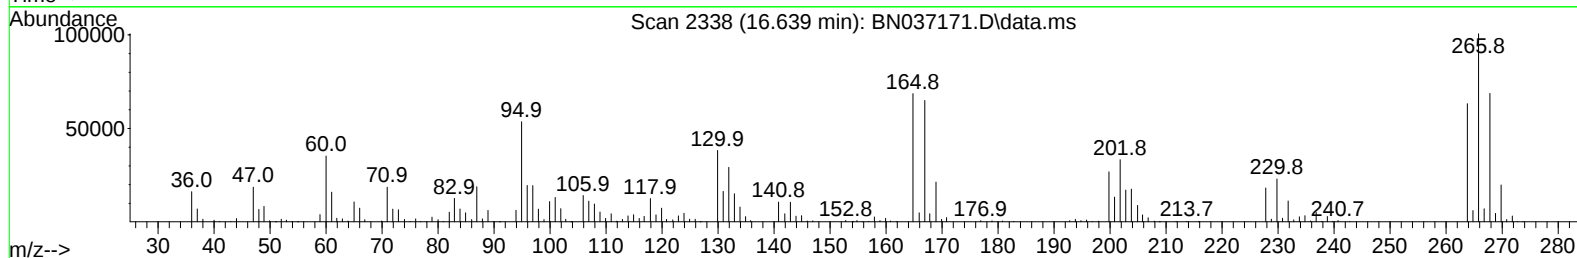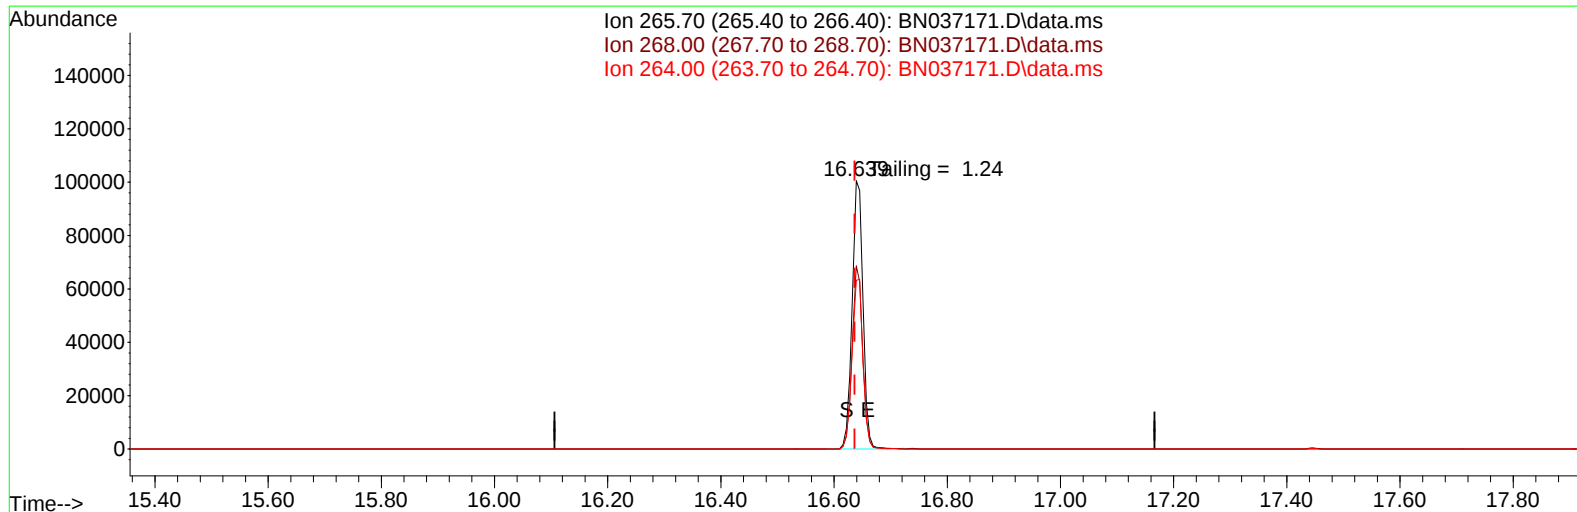

TIC: BN037171.D\data.ms

(70) Pentachlorophenol (C)

16.639min (+ 0.003) 18579.66 ng




response 133998

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.28
264.00	61.60	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037171.D
Acq On : 05 Jun 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 05 19:10:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

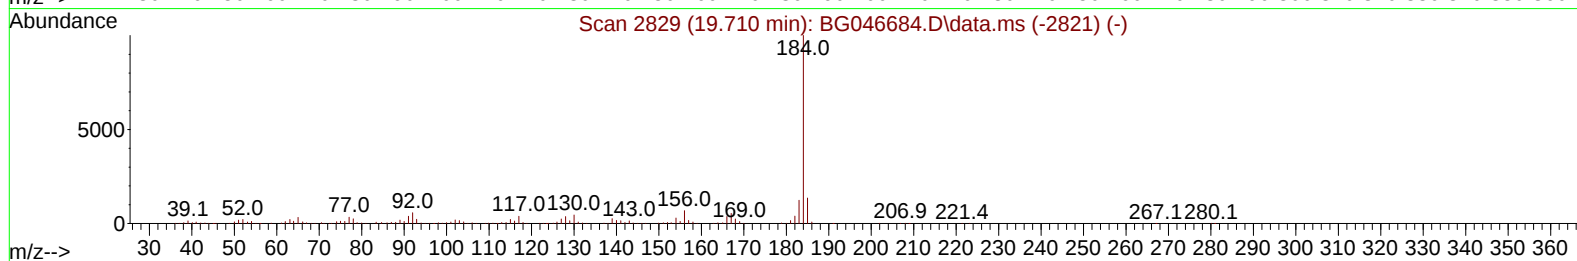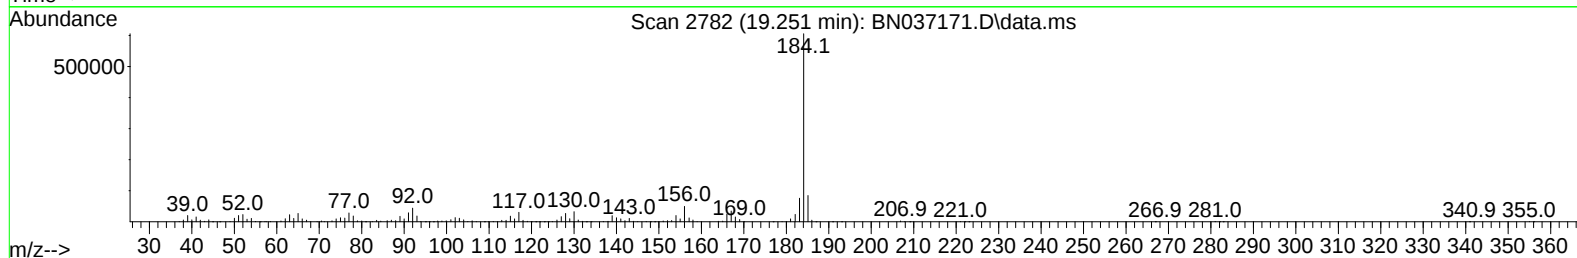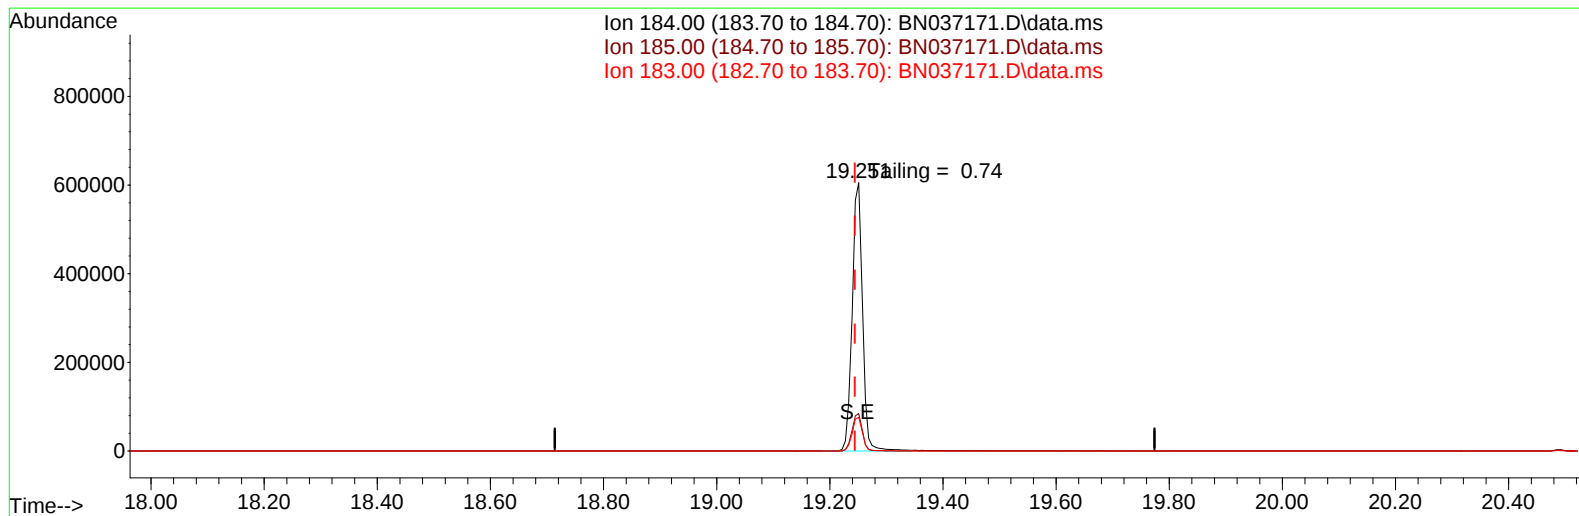

TIC: BN037171.D\data.ms

(77) Benzidine

19.251min (+ 0.007) 0.00 ng

response 772403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.95
183.00	13.20	12.58
0.00	0.00	0.00