

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
 Data File : BN037180.D
 Acq On : 05 Jun 2025 14:32
 Operator : RC/JU
 Sample : Q2200-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-01-6.5-060325

Quant Time: Jun 05 15:24:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 04 01:52:03 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.589	152	1856	0.400	ng	0.00
7) Naphthalene-d8	10.372	136	4772	0.400	ng	0.00
13) Acenaphthene-d10	14.234	164	2549	0.400	ng	0.00
19) Phenanthrene-d10	16.984	188	4645	0.400	ng	0.00
29) Chrysene-d12	21.189	240	3039	0.400	ng	0.00
35) Perylene-d12	23.377	264	2764	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.192	112	733	0.160	ng	0.00
5) Phenol-d6	6.773	99	566	0.102	ng	0.00
8) Nitrobenzene-d5	8.739	82	1652	0.328	ng	0.00
11) 2-Methylnaphthalene-d10	11.965	152	2122	0.319	ng	0.00
14) 2,4,6-Tribromophenol	15.730	330	377	0.367	ng	-0.01
15) 2-Fluorobiphenyl	12.858	172	3699	0.340	ng	0.00
27) Fluoranthene-d10	19.026	212	4158	0.352	ng	0.00
31) Terphenyl-d14	19.630	244	3085	0.431	ng	0.00
Target Compounds						
25) Phenanthrene	17.021	178	442	0.029	ng	Qvalue # 92
34) Bis(2-ethylhexyl)phtha...	21.117	149	1241	0.179	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060525\
Data File : BN037180.D
Acq On : 05 Jun 2025 14:32
Operator : RC/JU
Sample : Q2200-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW-01-6.5-060325


Quant Time: Jun 05 15:24:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 01:52:03 2025
Response via : Initial Calibration

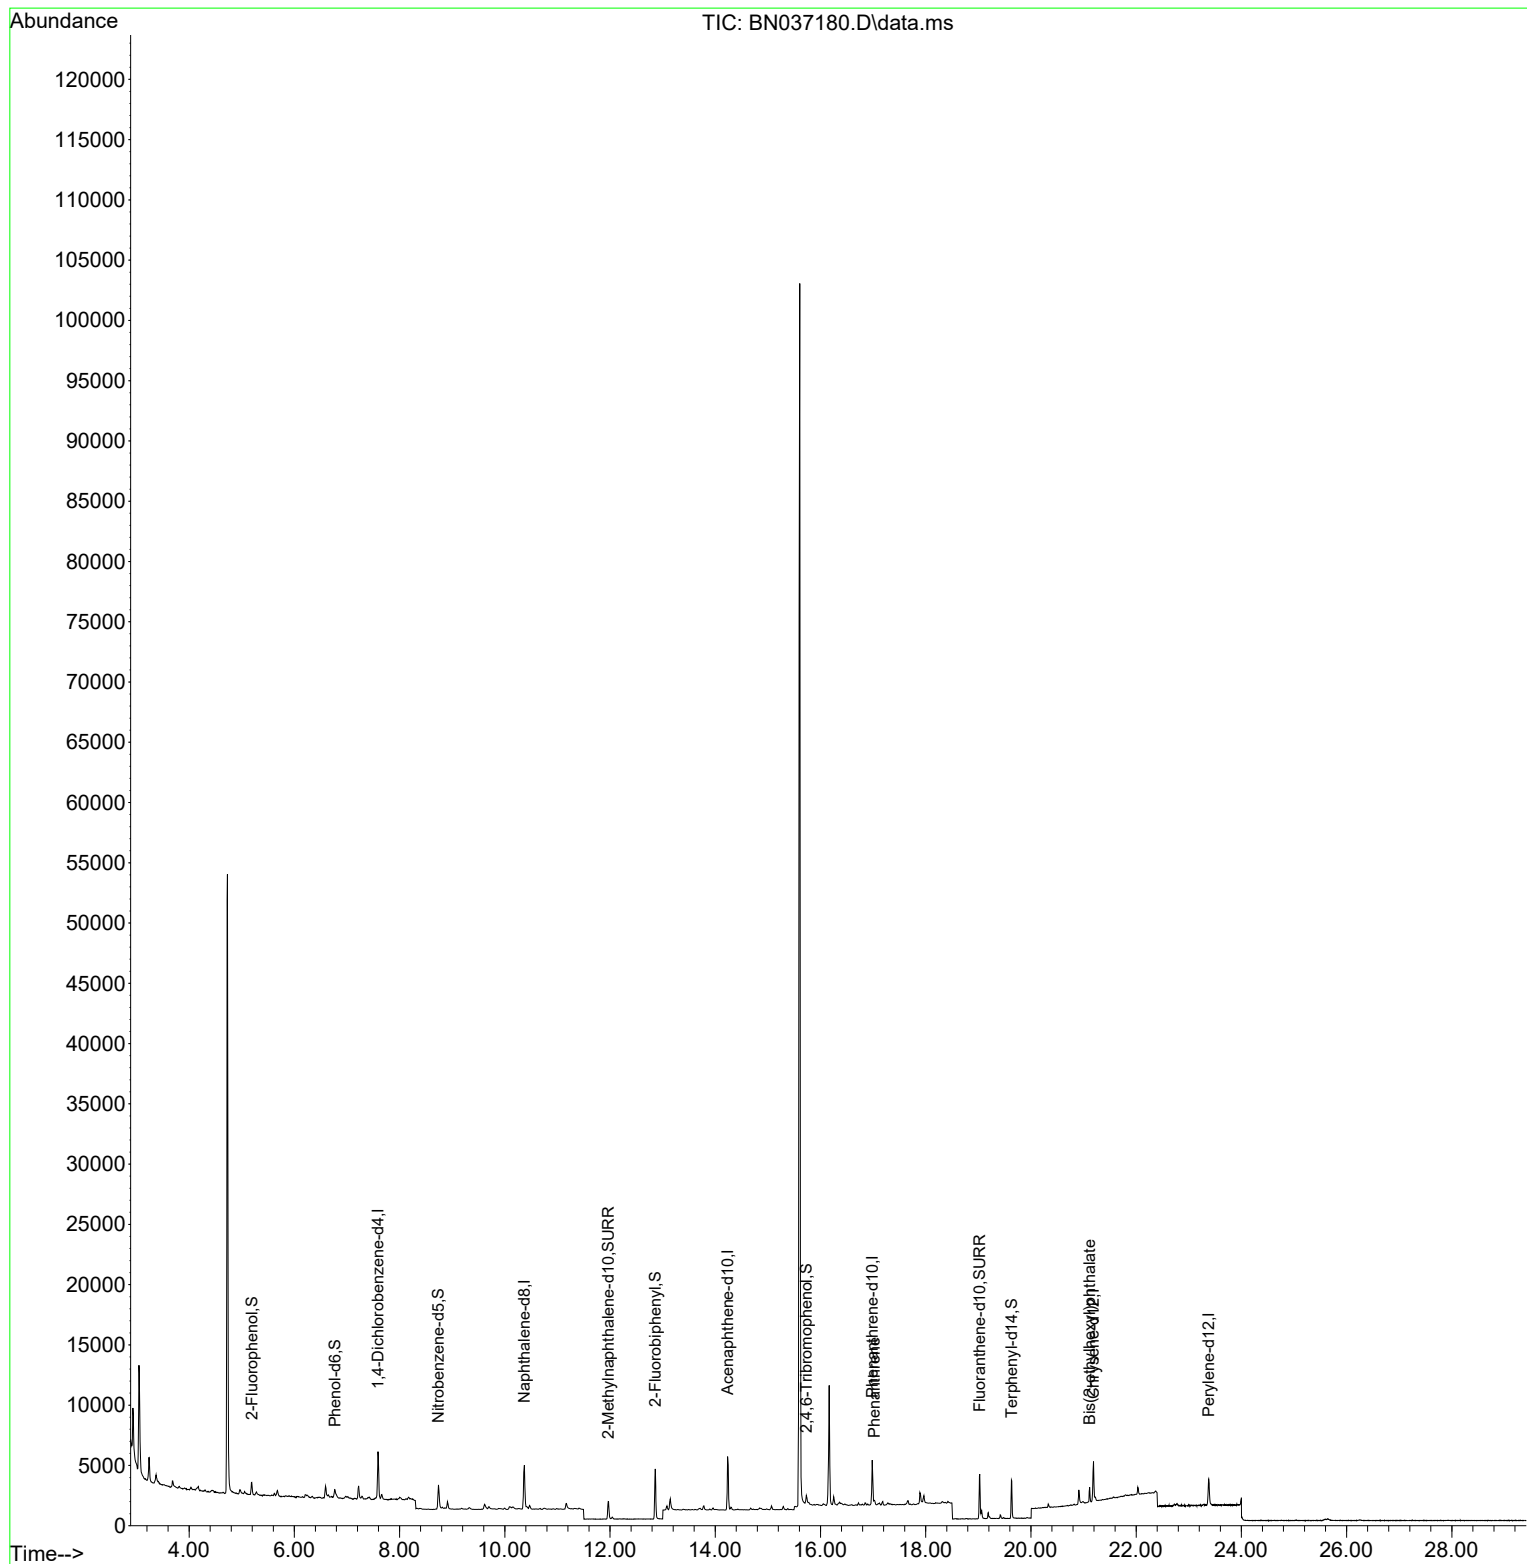






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.589 min Scan# 61
 Delta R.T. -0.001 min
 Lab File: BN037180.D
 Acq: 05 Jun 2025 14:32

Instrument :
 BNA_N
 ClientSampleId :
 MW-01-6.5-060325



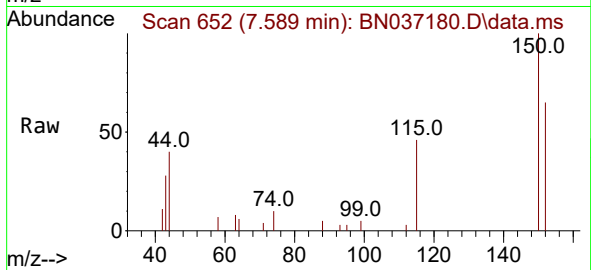



Tgt Ion:152 Resp: 1856
 Ion Ratio Lower Upper
 152 100
 150 154.2 123.2 184.8
 115 70.8 56.6 85.0

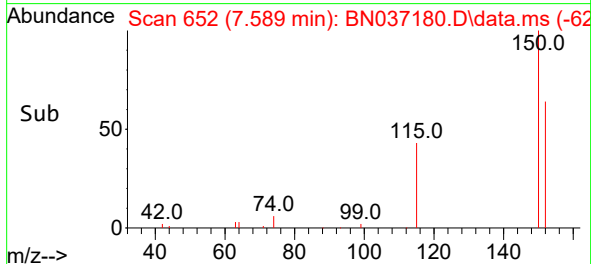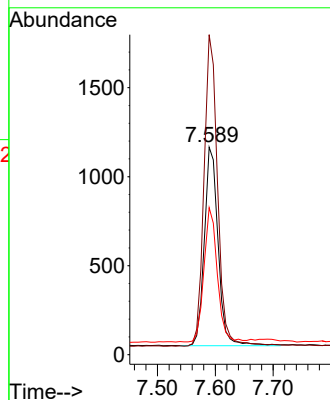

#4
 2-Fluorophenol
 Concen: 0.160 ng
 RT: 5.192 min Scan# 320
 Delta R.T. 0.007 min
 Lab File: BN037180.D
 Acq: 05 Jun 2025 14:32


Tgt Ion:112 Resp: 733
 Ion Ratio Lower Upper
 112 100
 64 70.4 56.3 84.5
 63 45.6 36.2 54.4

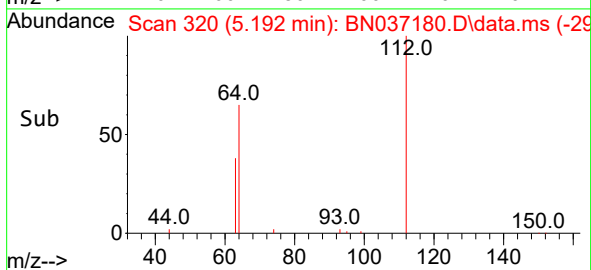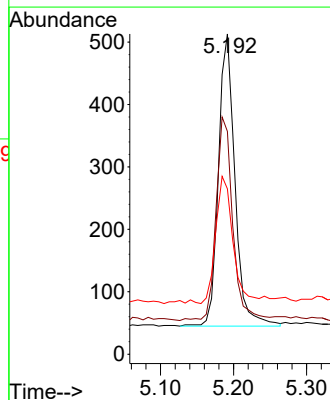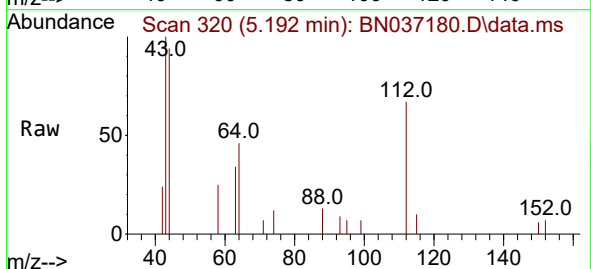






#5
Phenol-d6
Concen: 0.102 ng
RT: 6.773 min Scan# 511
Delta R.T. -0.000 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32

Instrument :
BNA_N
ClientSampleId :
MW-01-6.5-060325



Tgt Ion: 99 Resp: 566




Ion	Ratio	Lower	Upper
99	100		
42	38.0	31.3	46.9
71	56.9	38.2	57.2

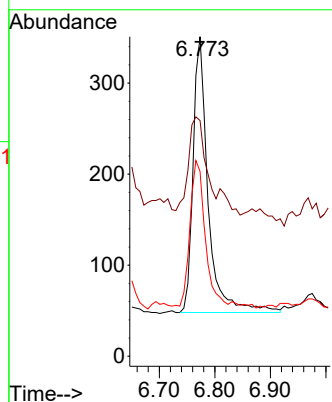


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.372 min Scan# 945
Delta R.T. -0.000 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32

Tgt Ion: 136 Resp: 4772

Ion	Ratio	Lower	Upper
136	100		
137	12.4	9.7	14.5
54	11.3	9.7	14.5
68	6.6	5.4	8.2


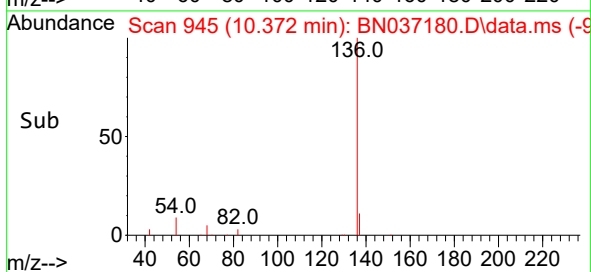
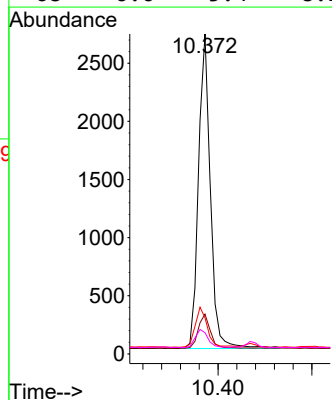



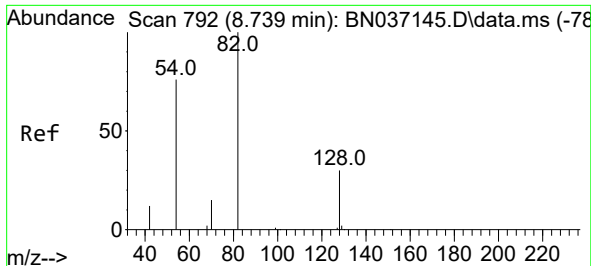

#8
Nitrobenzene-d5
Concen: 0.328 ng
RT: 8.739 min Scan# 792
Delta R.T. -0.000 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32




Instrument :
BNA_N
ClientSampleId :
MW-01-6.5-060325


Tgt Ion: 82 Resp: 1652
Ion Ratio Lower Upper
82 100
128 35.6 26.9 40.3
54 75.2 61.4 92.2

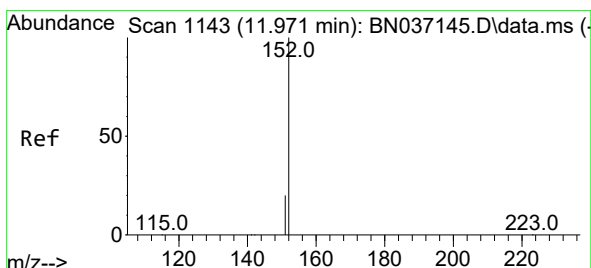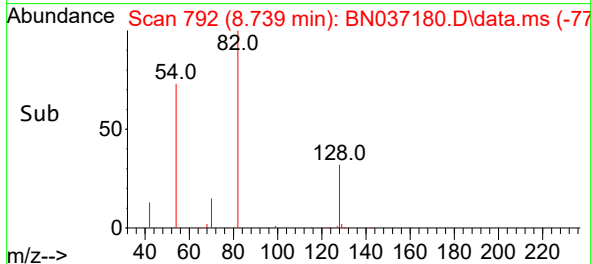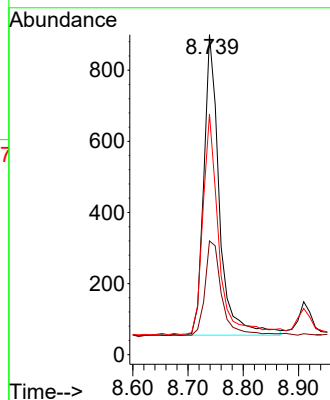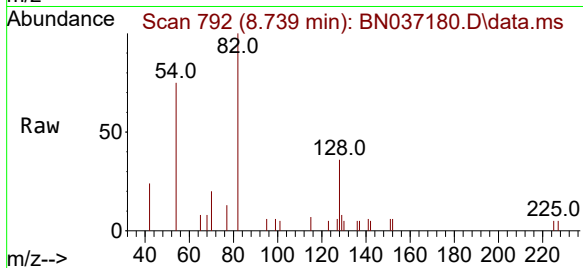

#11
2-Methylnaphthalene-d10
Concen: 0.319 ng
RT: 11.965 min Scan# 1142
Delta R.T. -0.005 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32

Tgt Ion: 152 Resp: 2122
Ion Ratio Lower Upper
152 100
151 21.7 17.1 25.7

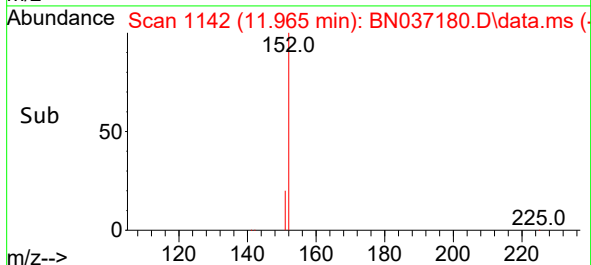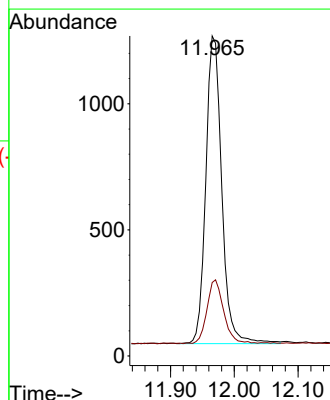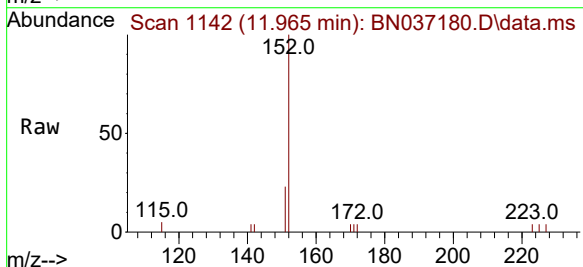



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.234 min Scan# 1462

Delta R.T. -0.000 min

Lab File: BN037180.D

Acq: 05 Jun 2025 14:32

Instrument :

BNA_N

ClientSampleId :

MW-01-6.5-060325





Tgt Ion:164 Resp: 2549

Ion Ratio Lower Upper

164 100

162 108.4 85.5 128.3

160 56.0 44.6 67.0

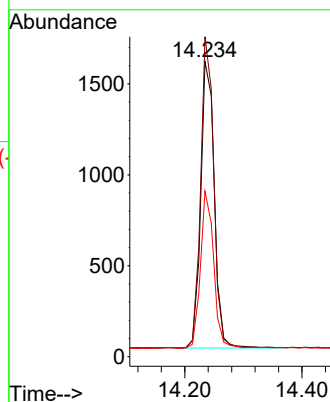

#14

2,4,6-Tribromophenol

Concen: 0.367 ng

RT: 15.730 min Scan# 1599

Delta R.T. -0.013 min

Lab File: BN037180.D

Acq: 05 Jun 2025 14:32




Tgt Ion:330 Resp: 377


Ion Ratio Lower Upper

330 100

332 95.0 77.1 115.7

141 64.5 46.4 69.6

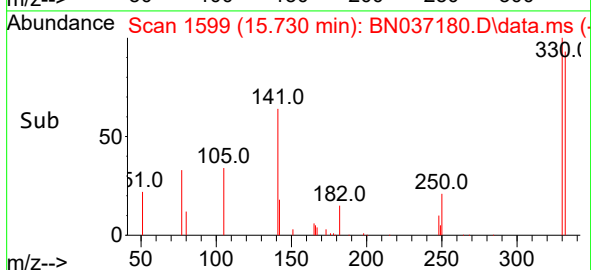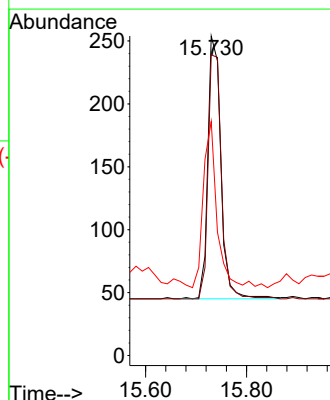

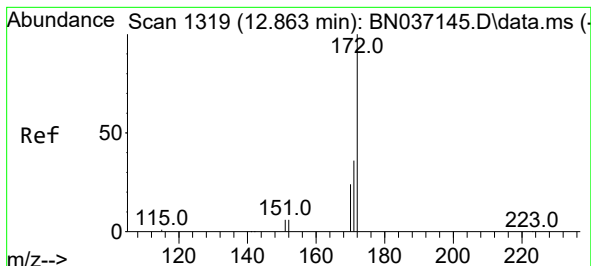

#15

2-Fluorobiphenyl

Concen: 0.340 ng

RT: 12.858 min Scan# 11

Delta R.T. -0.005 min

Lab File: BN037180.D


Acq: 05 Jun 2025 14:32

Instrument :

BNA_N

ClientSampleId :

MW-01-6.5-060325

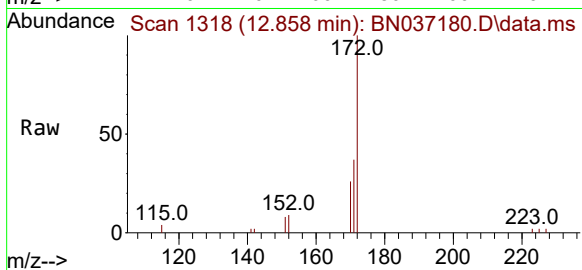




Tgt Ion:172 Resp: 3699

Ion Ratio Lower Upper

172 100

171 36.7 29.6 44.4

170 26.2 20.3 30.5

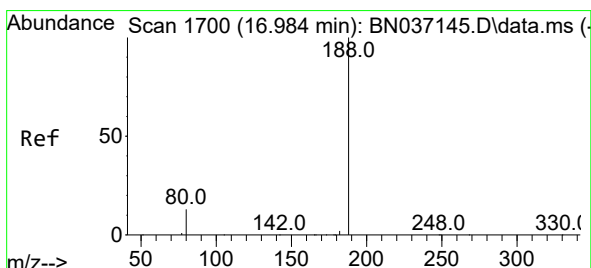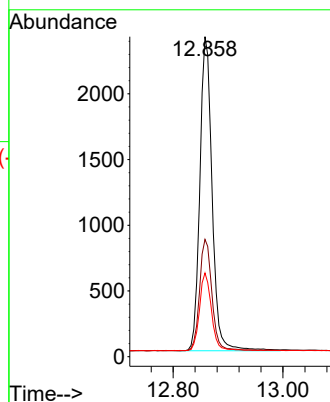

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.984 min Scan# 1700

Delta R.T. -0.000 min

Lab File: BN037180.D

Acq: 05 Jun 2025 14:32




Tgt Ion:188 Resp: 4645


Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 13.5 11.3 16.9


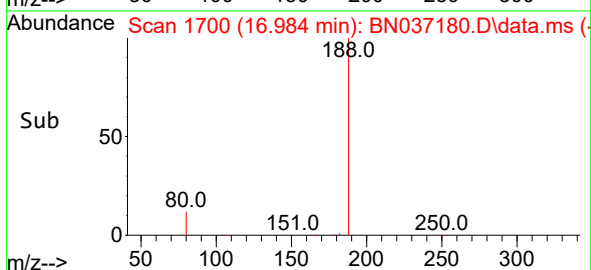

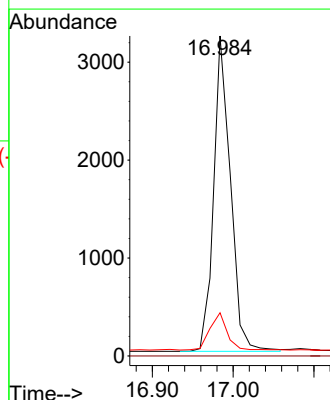




#25
Phenanthrene
Concen: 0.029 ng
RT: 17.021 min Scan# 1703
Delta R.T. -0.013 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32




Instrument :
BNA_N
ClientSampleId :
MW-01-6.5-060325


Tgt Ion:178 Resp: 442
Ion Ratio Lower Upper
178 100
176 20.6 15.7 23.5
179 21.7 12.3 18.5#

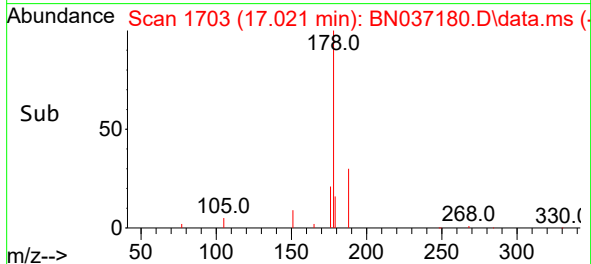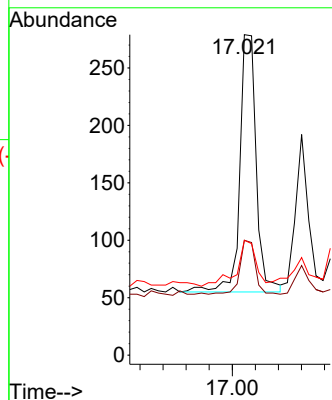

#27
Fluoranthene-d10
Concen: 0.352 ng
RT: 19.026 min Scan# 1934
Delta R.T. -0.000 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32

Tgt Ion:212 Resp: 4158
Ion Ratio Lower Upper
212 100
106 13.4 10.6 15.8
104 8.1 6.6 9.8


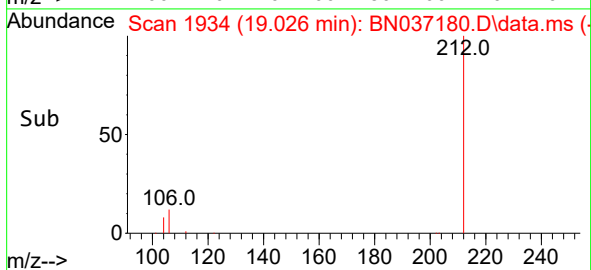
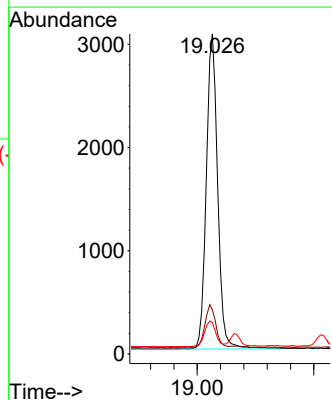
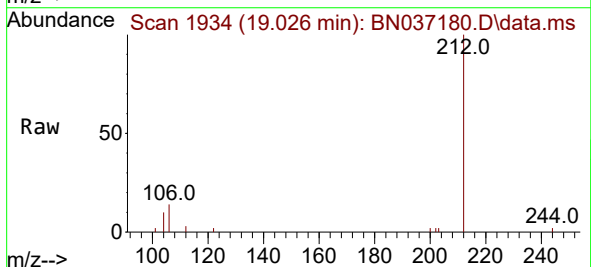




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.189 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32




Instrument :
BNA_N
ClientSampleId :
MW-01-6.5-060325


Tgt Ion:240 Resp: 3039
Ion Ratio Lower Upper
240 100
120 13.1 9.0 13.4
236 30.2 23.0 34.4

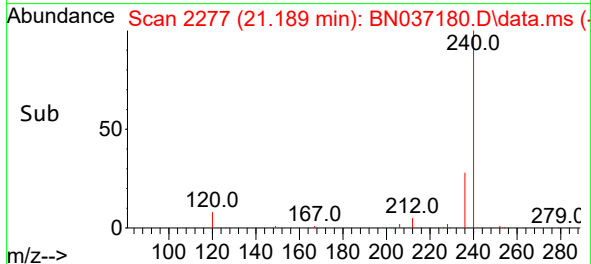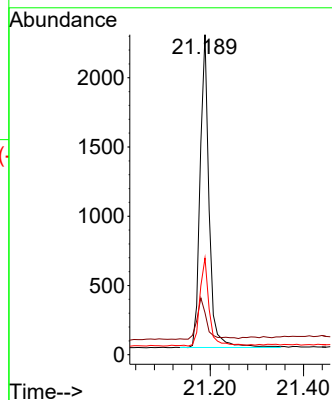

#31
Terphenyl-d14
Concen: 0.431 ng
RT: 19.630 min Scan# 2064
Delta R.T. -0.005 min
Lab File: BN037180.D
Acq: 05 Jun 2025 14:32

Tgt Ion:244 Resp: 3085
Ion Ratio Lower Upper
244 100
212 12.8 10.0 15.0
122 18.7 13.2 19.8


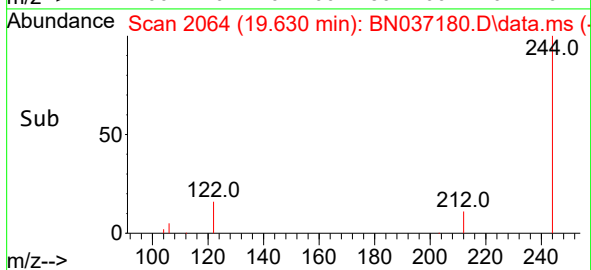
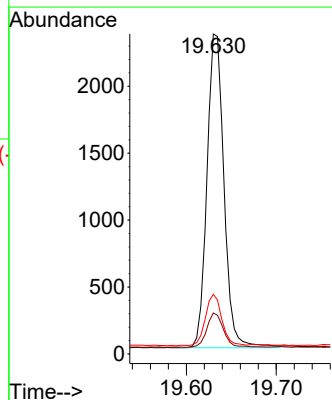
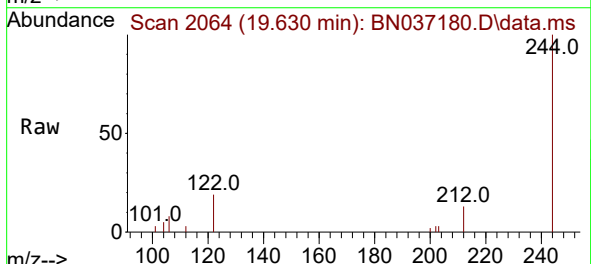


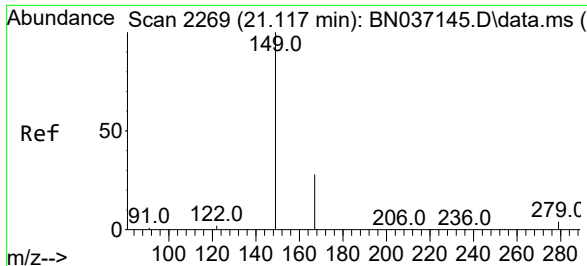

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.179 ng
 RT: 21.117 min Scan# 2117
 Delta R.T. -0.000 min
 Lab File: BN037180.D
 Acq: 05 Jun 2025 14:32

Instrument :
 BNA_N
 ClientSampleId :
 MW-01-6.5-060325

Tgt Ion:149 Resp: 1241
 Ion Ratio Lower Upper
 149 100
 167 24.8 21.0 31.4
 279 3.6 2.9 4.3

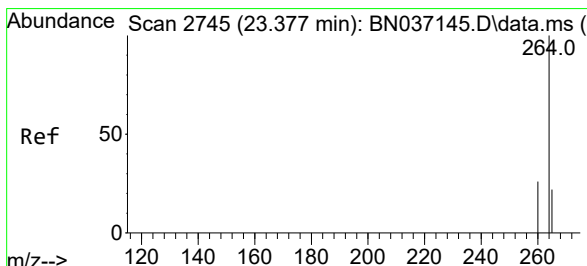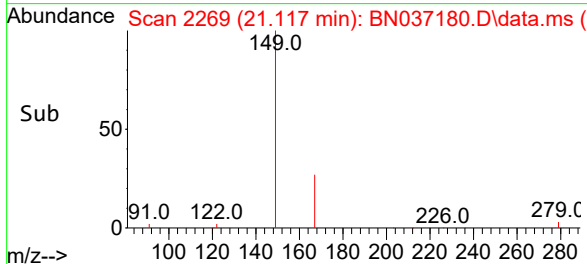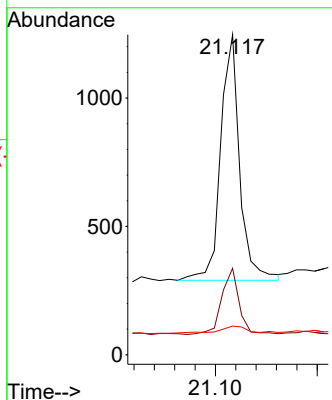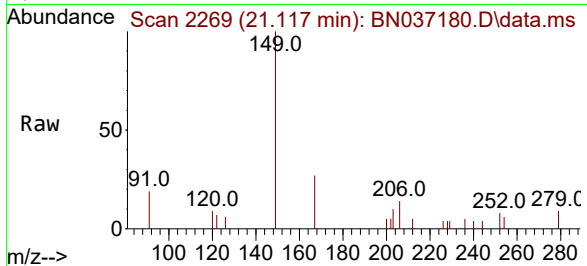

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.377 min Scan# 2745
 Delta R.T. -0.000 min
 Lab File: BN037180.D
 Acq: 05 Jun 2025 14:32

Tgt Ion:264 Resp: 2764
 Ion Ratio Lower Upper
 264 100
 260 27.1 22.1 33.1
 265 78.6 55.8 83.8

