

## **DATA PACKAGE VOLATILE ORGANICS**

**PROJECT NAME : FORMER SCHLUMBERGER STC PTC SITE D3868221**

**JACOBS ENGINEERING GROUP, INC.**

**412 Mt. Kemble Ave**

**Downtown Building**

**Morristown, NJ - 07960**

**Phone No: 9732670555**

**ORDER ID : Q2200**

**ATTENTION : John Ynfante**



**Laboratory Certification ID # 20012**

<b>1) VOLATILES DATA</b>	<b>2</b>
<b>2) Signature Page</b>	<b>4</b>
<b>3) Case Narrative</b>	<b>5</b>
<b>4) Qualifier Page</b>	<b>7</b>
<b>5) Conformance/Non Conformance</b>	<b>8</b>
<b>6) QA Checklist</b>	<b>10</b>
<b>7) Chronicle</b>	<b>11</b>
<b>8) Hit Summary</b>	<b>12</b>
<b>9) QC Data Summary For VOCMS Group3</b>	<b>13</b>
<b>9.1) Deuterated Monitoring Compound Summary</b>	<b>14</b>
<b>9.2) LCS/LCSD Summary</b>	<b>15</b>
<b>9.3) Method Blank Summary</b>	<b>17</b>
<b>9.4) GS/MS Tune Summary</b>	<b>18</b>
<b>9.5) Internal Standard Area and RT Summary</b>	<b>20</b>
<b>10) Sample Data</b>	<b>22</b>
<b>10.1) RMW-02B-66-060325</b>	<b>23</b>
<b>10.2) RMW-02B-66-060325DL</b>	<b>34</b>
<b>10.3) RMW-03B-90-060325</b>	<b>44</b>
<b>10.4) EB01-060325</b>	<b>53</b>
<b>10.5) MW-11B-37.5-060325</b>	<b>62</b>
<b>10.6) MW-11B-37.5-060325DL</b>	<b>71</b>
<b>10.7) TB-01-060325</b>	<b>79</b>
<b>11) Calibration Data Summary</b>	<b>86</b>
<b>11.1) Initial Calibration Data</b>	<b>87</b>
<b>11.1.1) VX050525</b>	<b>87</b>
<b>11.2) Continued Calibration Data</b>	<b>456</b>
<b>11.2.1) VX046488.D</b>	<b>456</b>
<b>12) QC Sample Data</b>	<b>515</b>
<b>12.1) Tune Raw Data</b>	<b>516</b>
<b>12.2) Method Blank Data</b>	<b>518</b>
<b>12.3) LCS Data</b>	<b>525</b>
<b>12.4) LCSD Data</b>	<b>578</b>
<b>13) Manual Integration</b>	<b>631</b>
<b>14) Analytical Runlogs</b>	<b>634</b>
<b>15) Standard Prep Logs</b>	<b>640</b>

## Table Of Contents for Q2200

<b>16) Shipping Document</b>	<b>735</b>	<b>1</b>
<b>16.1) Chain Of Custody</b>	<b>736</b>	<b>2</b>
<b>16.2) Lab Certificate</b>	<b>737</b>	<b>3</b>
<b>16.3) Internal COC</b>	<b>738</b>	<b>4</b>
		<b>5</b>
		<b>6</b>
		<b>7</b>
		<b>8</b>
		<b>9</b>
		<b>10</b>
		<b>11</b>
		<b>12</b>
		<b>13</b>
		<b>14</b>
		<b>15</b>
		<b>16</b>

## Cover Page

**Order ID :** Q2200

**Project ID :** Former Schlumberger STC PTC Site D3868221

**Client :** JACOBS Engineering Group, Inc.

### Lab Sample Number

Q2200-01  
Q2200-02  
Q2200-03  
Q2200-04  
Q2200-05  
Q2200-06

### Client Sample Number

RMW-02B-66-060325  
RMW-03B-90-060325  
EB01-060325  
MW-01-6.5-060325  
MW-11B-37.5-060325  
TB-01-060325

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : \_\_\_\_\_

Date: 6/9/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

## CASE NARRATIVE

**JACOBS Engineering Group, Inc.**

**Project Name:** Former Schlumberger STC PTC Site D3868221

**Project # N/A**

**Order ID # Q2200**

**Test Name:** VOCMS Group3

**A. Number of Samples and Date of Receipt:**

6 Water samples were received on 06/03/2025.

**B. Parameters**

According to the Chain of Custody document, the following analyses were requested:  
SVOC-SIMGroup1 and VOCMS Group3. This data package contains results for  
VOCMS Group3.

**C. Analytical Techniques:**

The analysis performed on instrument MSVOA\_X were done using GC column DB-624UI 20m 0.18mm 1.0 um. Cat#121-1324UIThe analysis of VOCMS Group3 was based on method 8260D.

**D. QA/ QC Samples:**

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria.

The Internal Standards Areas met the acceptable requirements.

The Retention Times were acceptable for all samples.

The RPD met criteria.

The Blank Spike met requirements for all samples.

The Blank Spike Duplicate met requirements for all samples.

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements.

The Continuous Calibration met the requirements.

The Tuning criteria met requirements.

Samples RMW-02B-66-060325, RMW-03B-90-060325 and MW-11B-37.5-060325 were diluted at straight dilution after checking past history of these samples.

Samples RMW-02B-66-060325 and MW-11B-37.5-060325 were diluted due to high concentrations.

**E. Additional Comments:**

Samples for MS/MSD for VOC analysis were not provided with this set of samples. The Blank Spike Duplicate is reported with the data.



284 Sheffield Street, Mountainside, NJ 07092  
Phone: 908 789 8900 Fax: 908 789 8922

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

**F. Manual Integration Comments:**

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

---

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature \_\_\_\_\_

**DATA REPORTING QUALIFIERS- ORGANIC**

For reporting results, the following "Results Qualifiers" are used:

- Value** If the result is a value greater than or equal to the detection limit, report the value
- U** Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
- ND** Indicates the analyte was analyzed for, but not detected
- J** Indicates an estimated value. This flag is used:  
(1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.)  
(2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
- B** Indicates the analyte was found in the blank as well as the sample report as "12 B".
- E** Indicates the analyte's concentration exceeds the calibrated range of the instrument for that specific analysis.
- D** This flag identifies all compounds identified in an analysis at a secondary dilution factor.
- P** This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
- N** This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
- A** This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
- Q** Indicates the LCS did not meet the control limits requirements

# **ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092**

NEW JERSEY LAB ID#: 20012; NEW YORK LAB ID#: 11376

## **GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY**

ORDER ID: Q2200

MATRIX: Water

METHOD: 8260D

	NA	NO	YES
1. Chromatograms Labeled/Compounds Identified. (Field samples and Method Blanks)			✓
2. GC/MS Tuning Specifications BFB Meet Criteria (NOTE THAT THERE ARE DIFFERENT CRITERIA FOR NY ASP CLP, CLP AND NJ)			✓
3. GC/MS Tuning Frequency - Performed every 24 hours for 600 series and 12 hours for 8000 Series.			✓
4. GC/MS Calibration - Initial Calibration performed before sample analysis and continuing calibration performed within 24 hours of sample analysis for 600 series and 12 hours for 8000 series.			✓
5. GC/MS Calibration Requirements. The Initial Calibration met the requirements. The Continuous Calibration met the requirements.			✓
6. Blank Contamination - If yes, list compounds and concentrations in each blank.			✓
7. Surrogate Recoveries Meet Criteria  If not met, list those compounds and their recoveries which fall outside the acceptable ranges.			✓
8. Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria  If not met, list those compounds and their recoveries which fall outside the acceptable range.  The Blank Spike met requirements for all samples.			✓
			The Blank Spike Duplicate met requirements for all samples.
9. Internal Standard Area/Retention Time Shift Meet Criteria  Comments:			✓
10. Analysis Holding Time Met  If not met, list number of days exceeded for each sample:			✓

**ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092**

NEW JERSEY LAB ID#: 20012; NEW YORK LAB ID#: 11376

**GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)**

NA      NO      YES

**ADDITIONAL COMMENTS:**

Samples RMW-02B-66-060325, RMW-03B-90-060325 and MW-11B-37.5-060325 were diluted at straight dilution after checking past history of these samples.

Samples RMW-02B-66-060325 and MW-11B-37.5-060325 were diluted due to high concentrations.

Samples for MS/MSD for VOC analysis were not provided with this set of samples. The Blank Spike Duplicate is reported with the data.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is >20% for the Initial Calibration curve for SW-846 analysis.

---

QA REVIEW

---

Date

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

## APPENDIX A

### QA REVIEW GENERAL DOCUMENTATION

Project #: Q2200

Completed

For thorough review, the report must have the following:

#### GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page) ✓

Check chain-of-custody for proper relinquish/return of samples ✓

Is the chain of custody signed and complete ✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts ✓

Collect information for each project id from server. Were all requirements followed ✓

#### COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page ✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody ✓

#### CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results ✓

Do requested analyses on Chain of Custody agree with the log-in page ✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody ✓

Were the samples received within hold time ✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle ✓

#### ANALYTICAL:

Was method requirement followed? ✓

Was client requirement followed? ✓

Does the case narrative summarize all QC failure? ✓

All runlogs and manual integration are reviewed for requirements ✓

All manual calculations and /or hand notations verified ✓

QA Review Signature: SOHIL JODHANI

Date: 06/09/2025

## LAB CHRONICLE

<b>OrderID:</b>	Q2200	<b>OrderDate:</b>	6/3/2025 4:06:00 PM
<b>Client:</b>	JACOBS Engineering Group, Inc.	<b>Project:</b>	Former Schlumberger STC PTC Site D3868221
<b>Contact:</b>	John Ynfante	<b>Location:</b>	L31, VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2200-01	RMW-02B-66-060325	Water	VOCMS Group3	8260-Low	<b>06/03/25</b>		<b>06/03/25</b>	
Q2200-01DL	RMW-02B-66-060325 DL	Water	VOCMS Group3	8260-Low	<b>06/03/25</b>		<b>06/03/25</b>	
Q2200-02	RMW-03B-90-060325	Water	VOCMS Group3	8260-Low	<b>06/03/25</b>		<b>06/03/25</b>	
Q2200-03	EB01-060325	Water	VOCMS Group3	8260-Low	<b>06/03/25</b>		<b>06/03/25</b>	
Q2200-05	MW-11B-37.5-060325	Water	VOCMS Group3	8260-Low	<b>06/03/25</b>		<b>06/03/25</b>	
Q2200-05DL	MW-11B-37.5-060325 DL	Water	VOCMS Group3	8260-Low	<b>06/03/25</b>		<b>06/03/25</b>	
Q2200-06	TB-01-060325	Water	VOCMS Group3	8260-Low	<b>06/03/25</b>		<b>06/03/25</b>	

### Hit Summary Sheet SW-846

**SDG No.:** Q2200  
**Client:** JACOBS Engineering Group, Inc.

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
<b>Client ID:</b>	<b>RMW-02B-66-060325</b>							
Q2200-01	RMW-02B-66-0603 Water	Vinyl Chloride		93.7		2.60	10.0	ug/L
Q2200-01	RMW-02B-66-0603 Water	1,1-Dichloroethene		180		2.30	10.0	ug/L
Q2200-01	RMW-02B-66-0603 Water	1,1-Dichloroethane		25.2		2.30	10.0	ug/L
Q2200-01	RMW-02B-66-0603 Water	cis-1,2-Dichloroethene		1800	E	1.90	10.0	ug/L
Q2200-01	RMW-02B-66-0603 Water	Trichloroethene		4400	E	0.93	10.0	ug/L
Q2200-01	RMW-02B-66-0603 Water	Tetrachloroethene		63.3		2.30	10.0	ug/L
<b>Total Voc :</b>				6560				
<b>Total Concentration:</b>				6560				
<b>Client ID:</b>	<b>RMW-02B-66-060325DL</b>							
Q2200-01DL	RMW-02B-66-0603 Water	Vinyl Chloride		82.3	JD	26.0	100	ug/L
Q2200-01DL	RMW-02B-66-0603 Water	1,1-Dichloroethene		210	D	23.0	100	ug/L
Q2200-01DL	RMW-02B-66-0603 Water	cis-1,2-Dichloroethene		1700	D	19.0	100	ug/L
Q2200-01DL	RMW-02B-66-0603 Water	Trichloroethene		4300	D	9.30	100	ug/L
Q2200-01DL	RMW-02B-66-0603 Water	Tetrachloroethene		61.6	JD	23.0	100	ug/L
<b>Total Voc :</b>				6350				
<b>Total Concentration:</b>				6350				
<b>Client ID:</b>	<b>RMW-03B-90-060325</b>							
Q2200-02	RMW-03B-90-0603 Water	cis-1,2-Dichloroethene		3900		9.50	50.0	ug/L
Q2200-02	RMW-03B-90-0603 Water	Trichloroethene		220		4.70	50.0	ug/L
<b>Total Voc :</b>				4120				
<b>Total Concentration:</b>				4120				
<b>Client ID:</b>	<b>MW-11B-37.5-060325</b>							
Q2200-05	MW-11B-37.5-0603 Water	1,1-Dichloroethene		86.9		11.5	50.0	ug/L
Q2200-05	MW-11B-37.5-0603 Water	cis-1,2-Dichloroethene		1200		9.50	50.0	ug/L
Q2200-05	MW-11B-37.5-0603 Water	Trichloroethene		11300	E	4.70	50.0	ug/L
<b>Total Voc :</b>				12600				
<b>Total Concentration:</b>				12600				
<b>Client ID:</b>	<b>MW-11B-37.5-060325DL</b>							
Q2200-05DL	MW-11B-37.5-0603 Water	cis-1,2-Dichloroethene		1200	D	38.0	200	ug/L
Q2200-05DL	MW-11B-37.5-0603 Water	Trichloroethene		11100	D	18.6	200	ug/L
<b>Total Voc :</b>				12300				
<b>Total Concentration:</b>				12300				



# QC SUMMARY

### Surrogate Summary

**SDG No.:** Q2200

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

Lab Sample ID	Client ID	Parameter	Spike	Result	RecoveryQual	Limits	
						Low	High
Q2200-01	RMW-02B-66-060325	1,2-Dichloroethane-d4	50	51.6	103	70 (74)	130 (125)
		Dibromofluoromethane	50	48.8	98	70 (75)	130 (124)
		Toluene-d8	50	49.7	99	70 (86)	130 (113)
Q2200-01DL	RMW-02B-66-060325DL	4-Bromofluorobenzene	50	48.8	98	70 (77)	130 (121)
		1,2-Dichloroethane-d4	50	51.3	103	70 (74)	130 (125)
		Dibromofluoromethane	50	50.4	101	70 (75)	130 (124)
Q2200-02	RMW-03B-90-060325	Toluene-d8	50	50.0	100	70 (86)	130 (113)
		4-Bromofluorobenzene	50	53.4	107	70 (77)	130 (121)
		1,2-Dichloroethane-d4	50	51.0	102	70 (74)	130 (125)
Q2200-03	EB01-060325	Dibromofluoromethane	50	50.2	100	70 (75)	130 (124)
		Toluene-d8	50	50.4	101	70 (86)	130 (113)
		4-Bromofluorobenzene	50	50.6	101	70 (77)	130 (121)
Q2200-05	MW-11B-37.5-060325	1,2-Dichloroethane-d4	50	52.3	105	70 (74)	130 (125)
		Dibromofluoromethane	50	49.5	99	70 (75)	130 (124)
		Toluene-d8	50	50.7	101	70 (86)	130 (113)
Q2200-05DL	MW-11B-37.5-060325DL	4-Bromofluorobenzene	50	52.7	105	70 (77)	130 (121)
		1,2-Dichloroethane-d4	50	52.1	104	70 (74)	130 (125)
		Dibromofluoromethane	50	49.8	100	70 (75)	130 (124)
Q2200-06	TB-01-060325	Toluene-d8	50	49.8	100	70 (86)	130 (113)
		4-Bromofluorobenzene	50	50.6	101	70 (77)	130 (121)
		1,2-Dichloroethane-d4	50	52.7	105	70 (74)	130 (125)
VX0604WBL01	VX0604WBL01	Dibromofluoromethane	50	49.9	100	70 (75)	130 (124)
		Toluene-d8	50	49.6	99	70 (86)	130 (113)
		4-Bromofluorobenzene	50	50.3	101	70 (77)	130 (121)
VX0604WBS01	VX0604WBS01	1,2-Dichloroethane-d4	50	53.2	106	70 (74)	130 (125)
		Dibromofluoromethane	50	50.0	100	70 (75)	130 (124)
		Toluene-d8	50	49.7	99	70 (86)	130 (113)
VX0604WBSD01	VX0604WBSD01	4-Bromofluorobenzene	50	50.7	101	70 (77)	130 (121)
		1,2-Dichloroethane-d4	50	53.4	107	70 (74)	130 (125)
		Dibromofluoromethane	50	50.4	101	70 (75)	130 (124)
VX0604WBSD01	VX0604WBSD01	Toluene-d8	50	50.4	101	70 (86)	130 (113)
		4-Bromofluorobenzene	50	53.1	106	70 (77)	130 (121)
		1,2-Dichloroethane-d4	50	50.1	100	70 (74)	130 (125)
VX0604WBSD01	VX0604WBSD01	Dibromofluoromethane	50	51.3	103	70 (75)	130 (124)
		Toluene-d8	50	47.3	95	70 (86)	130 (113)
		4-Bromofluorobenzene	50	49.1	98	70 (77)	130 (121)
VX0604WBSD01	VX0604WBSD01	1,2-Dichloroethane-d4	50	51.7	103	70 (74)	130 (125)
		Dibromofluoromethane	50	52.1	104	70 (75)	130 (124)
		Toluene-d8	50	49.0	98	70 (86)	130 (113)
VX0604WBSD01	VX0604WBSD01	4-Bromofluorobenzene	50	51.4	103	70 (77)	130 (121)

( ) = LABORATORY INHOUSE LIMIT

**Laboratory Control Sample/Laboratory Control Sample Duplicate Summary**

**SW-846**

**SDG No.:** Q2200

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

**Datafile :** VX046491.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		RPD
								Low	High	
VX0604WBS01	Vinyl chloride	20	15.5	ug/L	78			70 (65)	130 (117)	
	1,1-Dichloroethene	20	17.2	ug/L	86			70 (74)	130 (110)	
	1,1-Dichloroethane	20	19.6	ug/L	98			70 (78)	130 (112)	
	cis-1,2-Dichloroethene	20	19.6	ug/L	98			70 (77)	130 (110)	
	1,1,1-Trichloroethane	20	19.4	ug/L	97			70 (80)	130 (108)	
	Benzene	20	18.6	ug/L	93			70 (82)	130 (109)	
	1,2-Dichloroethane	20	19.8	ug/L	99			70 (80)	130 (115)	
	Trichloroethene	20	18.4	ug/L	92			70 (77)	130 (113)	
	1,1,2-Trichloroethane	20	20.5	ug/L	103			70 (83)	130 (112)	
	Tetrachloroethene	20	19.0	ug/L	95			70 (67)	130 (123)	

( ) = LABORATORY INHOUSE LIMIT

**Laboratory Control Sample/Laboratory Control Sample Duplicate Summary**

**SW-846**

**SDG No.:** Q2200

**Client:** JACOBS Engineering Group, Inc.

**Analytical Method:** SW8260-Low

**Datafile :** VX046497.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VX0604WBSD01	Vinyl chloride	20	18.8	ug/L	94	19		70 (65)	130 (117)	20 (20)
	1,1-Dichloroethene	20	20.3	ug/L	102	17		70 (74)	130 (110)	20 (20)
	1,1-Dichloroethane	20	22.2	ug/L	111	12		70 (78)	130 (112)	20 (20)
	cis-1,2-Dichloroethene	20	22.0	ug/L	110	12		70 (77)	130 (110)	20 (20)
	1,1,1-Trichloroethane	20	22.5	ug/L	113	15		70 (80)	130 (108)	20 (20)
	Benzene	20	21.4	ug/L	107	14		70 (82)	130 (109)	20 (20)
	1,2-Dichloroethane	20	21.6	ug/L	108	9		70 (80)	130 (115)	20 (20)
	Trichloroethene	20	21.3	ug/L	106	14		70 (77)	130 (113)	20 (20)
	1,1,2-Trichloroethane	20	22.2	ug/L	111	7		70 (83)	130 (112)	20 (20)
	Tetrachloroethene	20	20.6	ug/L	103	8		70 (67)	130 (123)	20 (20)

( ) = LABORATORY INHOUSE LIMIT



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

VOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

VX0604WBL01

Lab Name: CHEMTECH

Contract: JACO05

Lab Code: CHEM Case No.: Q2200

SAS No.: Q2200 SDG No.: Q2200

Lab File ID: VX046490.D

Lab Sample ID: VX0604WBL01

Date Analyzed: 06/04/2025

Time Analyzed: 11:04

GC Column: DB-624UI ID: 0.18 (mm)

Heated Purge: (Y/N) N

Instrument ID: MSVOA\_X

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VX0604WBS01	VX0604WBS01	VX046491.D	06/04/2025
VX0604WBSD01	VX0604WBSD01	VX046497.D	06/04/2025
RMW-02B-66-060325DL	Q2200-01DL	VX046498.D	06/04/2025
RMW-03B-90-060325	Q2200-02	VX046499.D	06/04/2025
MW-11B-37.5-060325	Q2200-05	VX046500.D	06/04/2025
EB01-060325	Q2200-03	VX046504.D	06/04/2025
RMW-02B-66-060325	Q2200-01	VX046508.D	06/04/2025
MW-11B-37.5-060325DL	Q2200-05DL	VX046509.D	06/04/2025
TB-01-060325	Q2200-06	VX046510.D	06/04/2025

COMMENTS:

---

---



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
BROMOFLUOROBENZENE (BFB)

Lab Name:	CHEMTECH	Contract:	JAC005
Lab Code:	CHEM	Case No.:	Q2200
Lab File ID:	VX046038.D	SAS No.:	Q2200
Instrument ID:	MSVOA_X	SDG NO.:	Q2200
GC Column:	DB-624UI ID: 0.18 (mm)	BFB Injection Date:	05/05/2025
		BFB Injection Time:	09:37
		Heated Purge:	Y/N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	22.1
75	30.0 - 60.0% of mass 95	56.2
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.4
173	Less than 2.0% of mass 174	0.5 ( 0.7 ) 1
174	50.0 - 100.0% of mass 95	68.8
175	5.0 - 9.0% of mass 174	5 ( 7.3 ) 1
176	95.0 - 101.0% of mass 174	66.7 ( 97 ) 1
177	5.0 - 9.0% of mass 176	4.6 ( 6.9 ) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDICC020	VSTDICC020	VX046041.D	05/05/2025	11:35
VSTDICCC050	VSTDICCC050	VX046042.D	05/05/2025	11:58
VSTDICC100	VSTDICC100	VX046043.D	05/05/2025	12:21
VSTDICC150	VSTDICC150	VX046044.D	05/05/2025	12:45
VSTDICC005	VSTDICC005	VX046046.D	05/05/2025	16:04
VSTDICC001	VSTDICC001	VX046047.D	05/05/2025	16:27



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
BROMOFLUOROBENZENE (BFB)

Lab Name:	CHEMTECH	Contract:	JAC005
Lab Code:	CHEM	Case No.:	Q2200
Lab File ID:	VX046487.D	SAS No.:	Q2200
Instrument ID:	MSVOA_X	SDG NO.:	Q2200
GC Column:	DB-624UI ID: 0.18 (mm)	BFB Injection Date:	06/04/2025
		BFB Injection Time:	09:43
		Heated Purge:	Y/N
			N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	22
75	30.0 - 60.0% of mass 95	55.2
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.9
173	Less than 2.0% of mass 174	0.8 ( 1.2 ) 1
174	50.0 - 100.0% of mass 95	68.4
175	5.0 - 9.0% of mass 174	4.8 ( 7 ) 1
176	95.0 - 101.0% of mass 174	67.2 ( 98.3 ) 1
177	5.0 - 9.0% of mass 176	4.5 ( 6.8 ) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VX046488.D	06/04/2025	10:12
VX0604WBL01	VX0604WBL01	VX046490.D	06/04/2025	11:04
VX0604WBS01	VX0604WBS01	VX046491.D	06/04/2025	11:27
VX0604WBSD01	VX0604WBSD01	VX046497.D	06/04/2025	13:52
RMW-02B-66-060325DL	Q2200-01DL	VX046498.D	06/04/2025	14:15
RMW-03B-90-060325	Q2200-02	VX046499.D	06/04/2025	14:39
MW-11B-37.5-060325	Q2200-05	VX046500.D	06/04/2025	15:02
EB01-060325	Q2200-03	VX046504.D	06/04/2025	16:37
RMW-02B-66-060325	Q2200-01	VX046508.D	06/04/2025	18:12
MW-11B-37.5-060325DL	Q2200-05DL	VX046509.D	06/04/2025	18:36
TB-01-060325	Q2200-06	VX046510.D	06/04/2025	19:00

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: JAC005  
 Lab Code: CHEM Case No.: Q2200 SAS No.: Q2200 SDG No.: Q2200  
 Lab File ID: VX046488.D Date Analyzed: 06/04/2025  
 Instrument ID: MSVOA\_X Time Analyzed: 10:12  
 GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	97475	5.54	165033	6.75	141151	10.05
	194950	6.043	330066	7.25	282302	10.549
	48737.5	5.043	82516.5	6.25	70575.5	9.549
EPA SAMPLE NO.						
RMW-02B-66-060325	59475	5.55	118649	6.76	107657	10.06
RMW-02B-66-060325DL	62989	5.55	125027	6.76	118665	10.06
RMW-03B-90-060325	65911	5.55	132066	6.76	121549	10.06
EB01-060325	64028	5.54	128366	6.76	122354	10.06
MW-11B-37.5-060325	61191	5.55	121976	6.76	112952	10.06
MW-11B-37.5-060325DL	63962	5.55	127435	6.76	117554	10.06
TB-01-060325	58762	5.54	118020	6.76	111037	10.06
VX0604WBL01	69580	5.55	139946	6.76	133992	10.05
VX0604WBS01	92897	5.54	164481	6.76	139452	10.05
VX0604WBSD01	84483	5.55	152834	6.76	133225	10.06

IS1 = Pentafluorobenzene

IS2 = 1,4-Difluorobenzene

IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name:	CHEMTECH	Contract:	JAC005
Lab Code:	CHEM	Case No.:	Q2200
Lab File ID:	VX046488.D	Date Analyzed:	06/04/2025
Instrument ID:	MSVOA_X	Time Analyzed:	10:12
GC Column:	DB-624UI	ID:	0.18 (mm)
		Heated Purge:	(Y/N) <u>N</u>

	IS4 AREA #	RT #				
12 HOUR STD	69016	12.018				
UPPER LIMIT	138032	12.518				
LOWER LIMIT	34508	11.518				
EPA SAMPLE NO.						
RMW-02B-66-060325	43595	12.02				
RMW-02B-66-060325DL	53639	12.02				
RMW-03B-90-060325	49186	12.02				
EB01-060325	53968	12.02				
MW-11B-37.5-060325	47128	12.02				
MW-11B-37.5-060325DL	50632	12.02				
TB-01-060325	47922	12.02				
VX0604WBL01	59967	12.02				
VX0604WBS01	63937	12.02				
VX0604WBSD01	62838	12.02				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.



# SAMPLE

# DATA

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	06/03/25
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	06/03/25
Client Sample ID:	RMW-02B-66-060325			SDG No.:	Q2200
Lab Sample ID:	Q2200-01			Matrix:	Water
Analytical Method:	8260D			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046508.D	10		06/04/25 18:12	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	93.7		2.60	10.0	ug/L
75-35-4	1,1-Dichloroethene	180		2.30	10.0	ug/L
75-34-3	1,1-Dichloroethane	25.2		2.30	10.0	ug/L
156-59-2	cis-1,2-Dichloroethene	1800	E	1.90	10.0	ug/L
71-55-6	1,1,1-Trichloroethane	2.00	U	2.00	10.0	ug/L
71-43-2	Benzene	1.50	U	1.50	10.0	ug/L
107-06-2	1,2-Dichloroethane	2.20	U	2.20	10.0	ug/L
79-01-6	Trichloroethene	4400	E	0.93	10.0	ug/L
79-00-5	1,1,2-Trichloroethane	2.10	U	2.10	10.0	ug/L
127-18-4	Tetrachloroethene	63.3		2.30	10.0	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	51.6		70 (74) - 130 (125)	103%	SPK: 50
1868-53-7	Dibromofluoromethane	48.8		70 (75) - 130 (124)	98%	SPK: 50
2037-26-5	Toluene-d8	49.7		70 (86) - 130 (113)	99%	SPK: 50
460-00-4	4-Bromofluorobenzene	48.8		70 (77) - 130 (121)	98%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	59500	5.55			
540-36-3	1,4-Difluorobenzene	119000	6.763			
3114-55-4	Chlorobenzene-d5	108000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	43600	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046508.D  
 Acq On : 04 Jun 2025 18:12  
 Operator : JC/MD  
 Sample : Q2200-01 10X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 22 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**RMW-02B-66-060325**

Quant Time: Jun 05 02:04:31 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	59475	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	118649	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	107657	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	43595	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	57267	51.648	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	103.300%	
35) Dibromofluoromethane	5.385	113	41659	48.758	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	97.520%	
50) Toluene-d8	8.647	98	147066	49.732	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	99.460%	
62) 4-Bromofluorobenzene	11.079	95	55309	48.759	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	97.520%	
<b>Target Compounds</b>						
				Qvalue		
4) Vinyl Chloride	1.374	62	7697	9.368	ug/l	96
12) 1,1-Dichloroethene	2.312	96	12979	18.404	ug/l	99
21) trans-1,2-Dichloroethene	3.093	96	775	1.093	ug/l #	78
24) 1,1-Dichloroethane	3.611	63	3655	2.521	ug/l #	93
27) cis-1,2-Dichloroethene	4.483	96	156809	183.666	ug/l	89
44) Trichloroethene	7.123	130	357950	442.298	ug/l	95
64) Tetrachloroethene	9.275	164	4825	6.334	ug/l	97







(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
Data File : VX046508.D  
Acq On : 04 Jun 2025 18:12  
Operator : JC/MD  
Sample : Q2200-01 10X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RMW-02B-66-060325

Quant Time: Jun 05 02:04:31 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

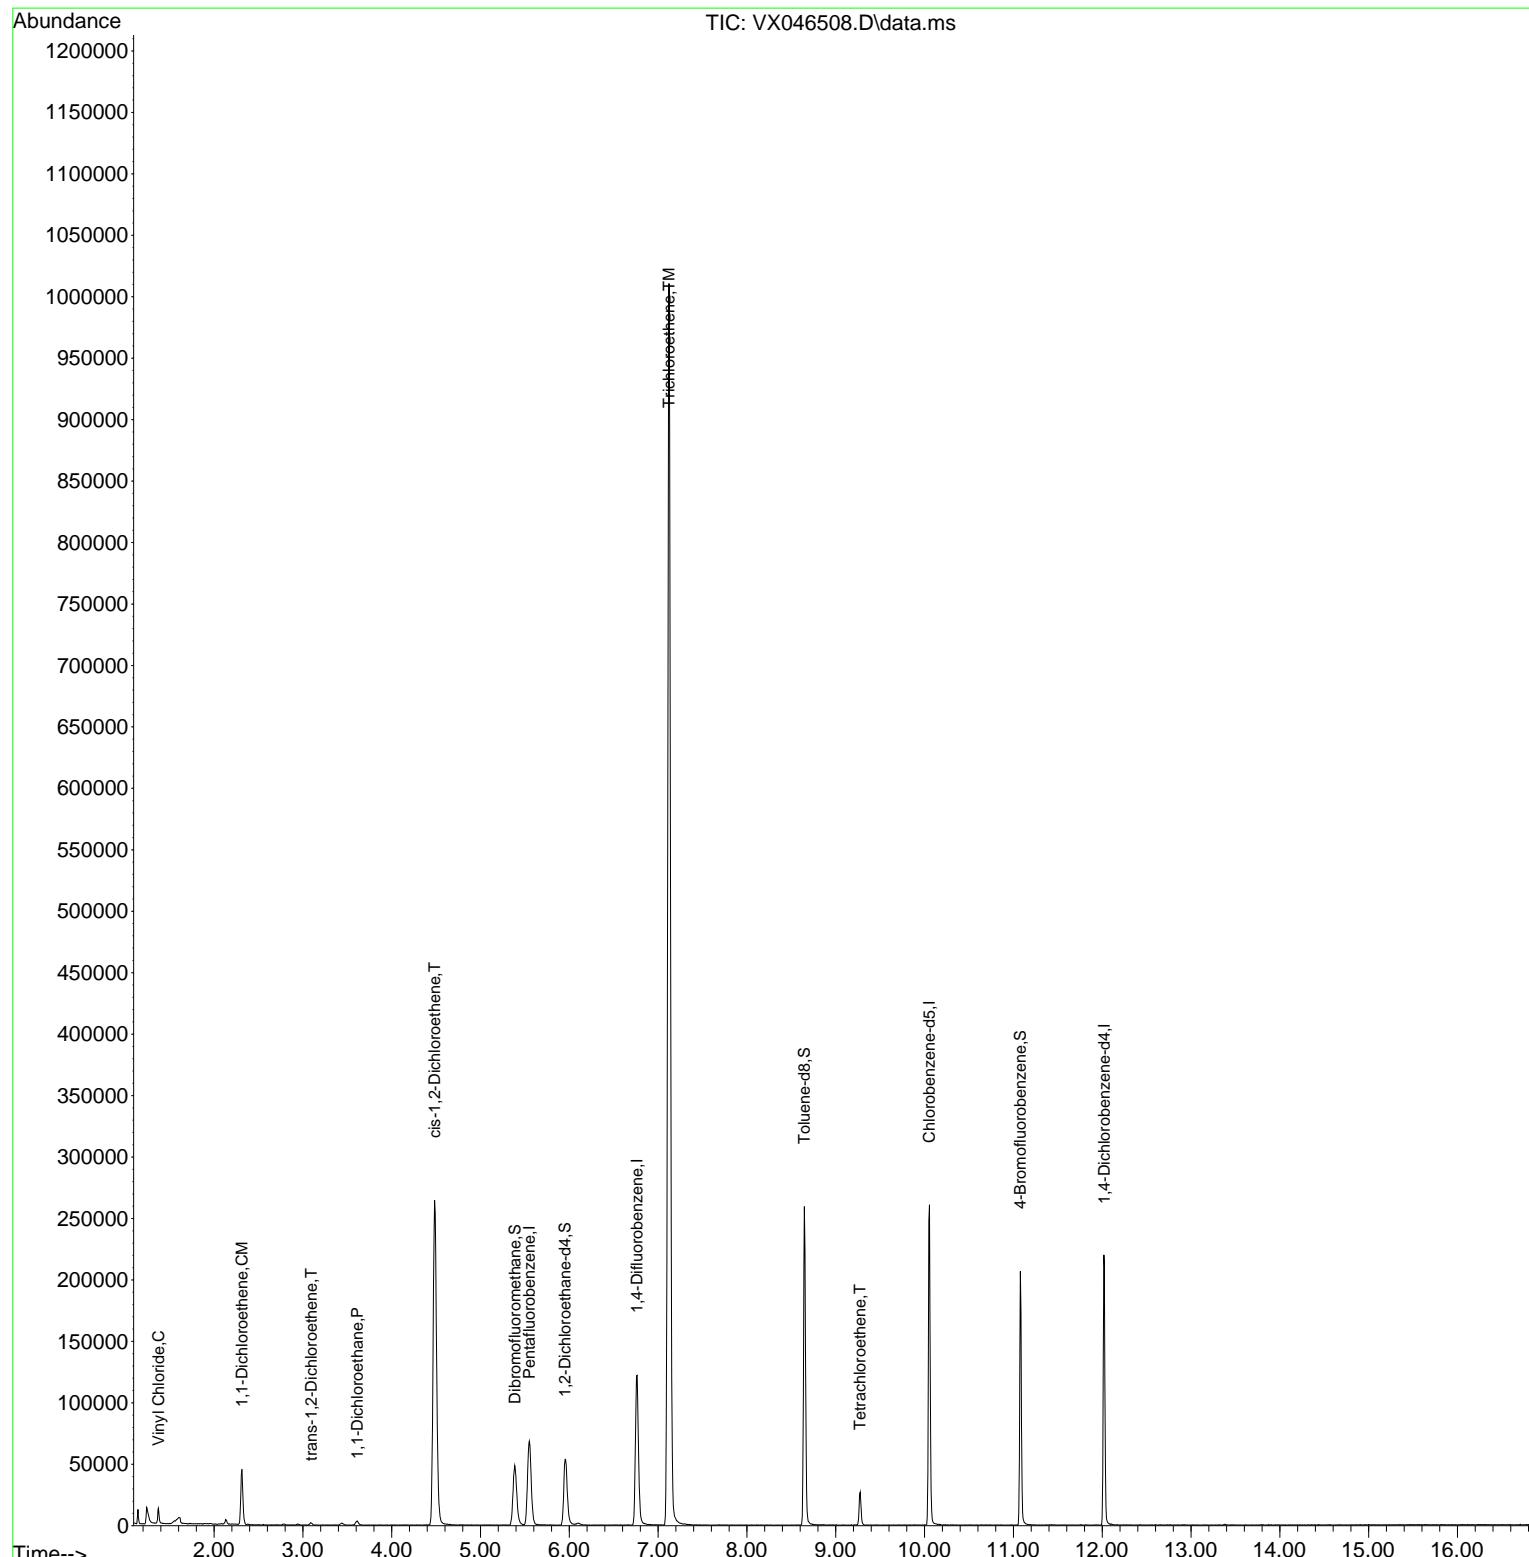




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX046508.D  
Acq: 04 Jun 2025 18:12  
ClientSampleId : RMW-02B-66-060325

Tgt Ion:168 Resp: 59475

Ion Ratio Lower Upper

168 100

99 68.1 54.9 82.3

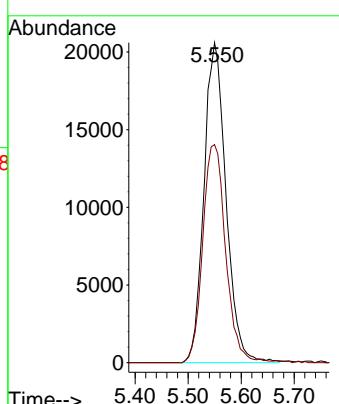


#4  
Vinyl Chloride  
Concen: 9.368 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. -0.000 min  
Lab File: VX046508.D  
Acq: 04 Jun 2025 18:12




Tgt Ion: 62 Resp: 7697

Ion Ratio Lower Upper

62 100

64 33.8 25.2 37.8

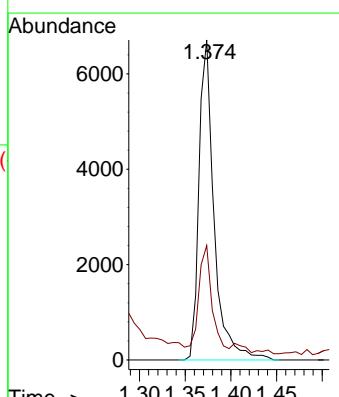

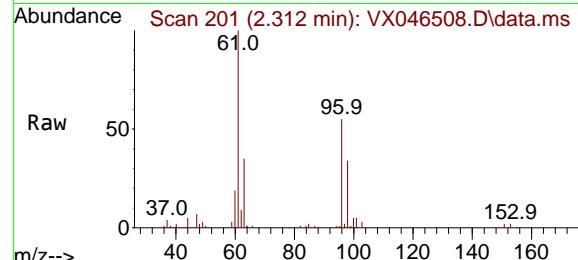

#12

1,1-Dichloroethene

Concen: 18.404 ug/l

RT: 2.312 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12

Instrument:

MSVOA\_X

ClientSampleId :

RMW-02B-66-060325





Tgt Ion: 96 Resp: 12979

Ion Ratio Lower Upper

96 100

61 181.1 146.2 219.2

98 62.4 51.0 76.6

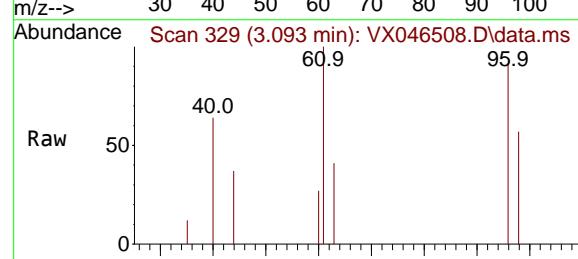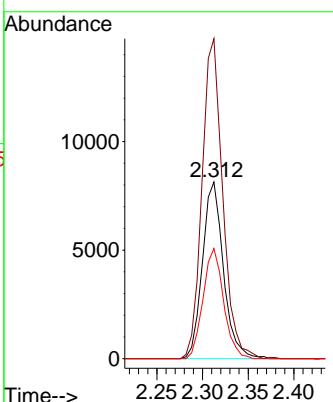

#21

trans-1,2-Dichloroethene

Concen: 1.093 ug/l

RT: 3.093 min Scan# 329

Delta R.T. 0.006 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12


Tgt Ion: 96 Resp: 775







Ion Ratio Lower Upper

96 100

61 110.5 119.5 179.3#

98 62.6 50.0 75.0



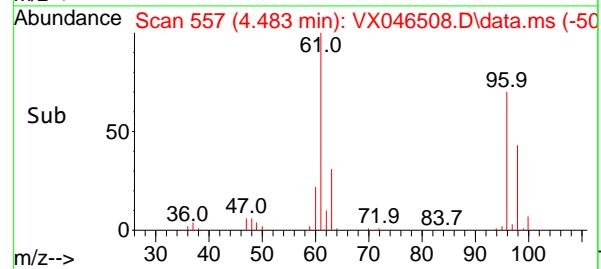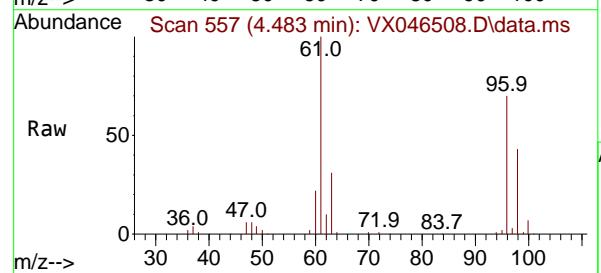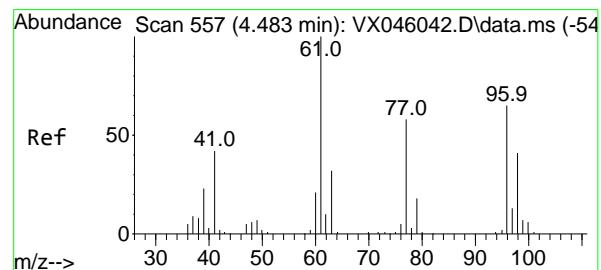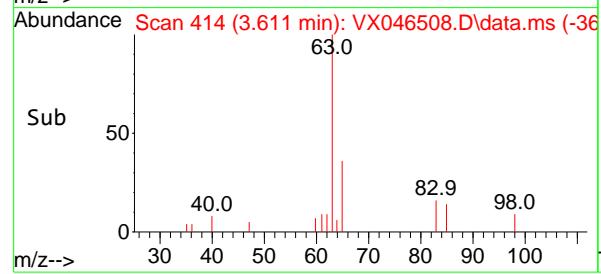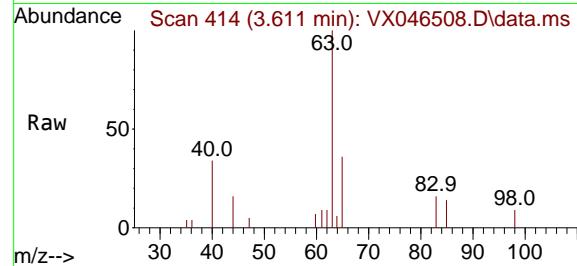

#24

1,1-Dichloroethane

Concen: 2.521 ug/l

RT: 3.611 min Scan# 4

Delta R.T. 0.006 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12

Instrument:

MSVOA\_X

ClientSampleId :

RMW-02B-66-060325


Tgt Ion: 63 Resp: 3655

Ion Ratio Lower Upper

63 100

98 8.7 3.6 10.8

100 0.0 2.1 6.3#

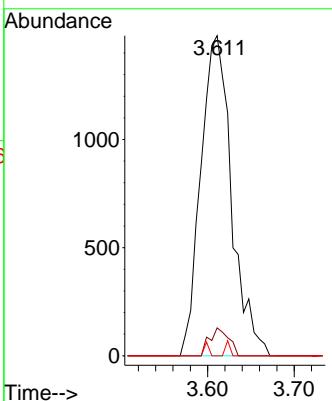

#27

cis-1,2-Dichloroethene

Concen: 183.666 ug/l

RT: 4.483 min Scan# 557

Delta R.T. -0.000 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12


Tgt Ion: 96 Resp: 156809







Ion Ratio Lower Upper

96 100

61 141.7 0.0 322.8

98 63.5 0.0 129.0

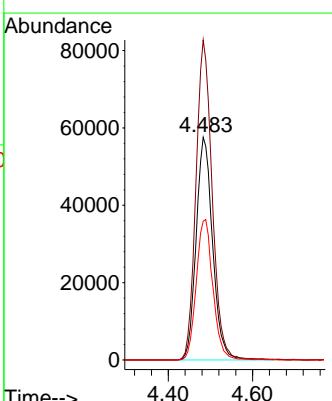

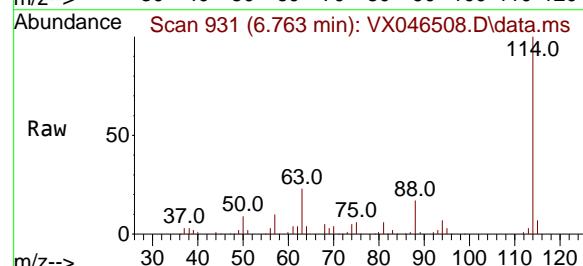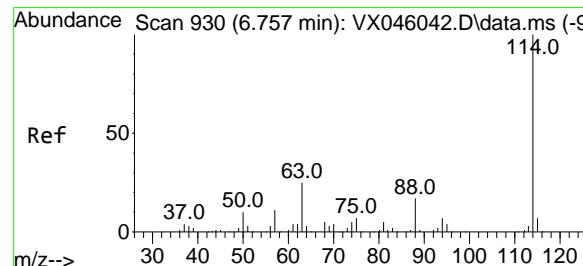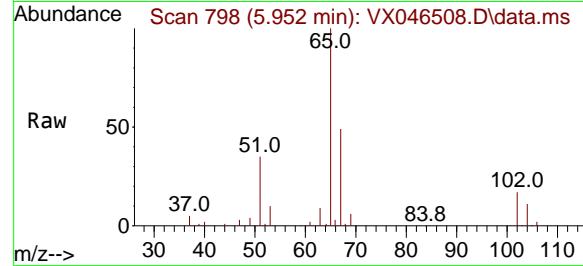

#33

1,2-Dichloroethane-d4

Concen: 51.648 ug/l

RT: 5.952 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12

Instrument:

MSVOA\_X

ClientSampleId :


RMW-02B-66-060325

Tgt Ion: 65 Resp: 57267

Ion Ratio Lower Upper

65 100

67 49.3 0.0 99.0

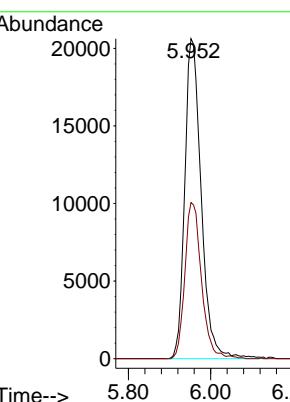

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12


Tgt Ion:114 Resp: 118649




Ion Ratio Lower Upper

114 100

63 22.9 0.0 49.2

88 16.8 0.0 33.6

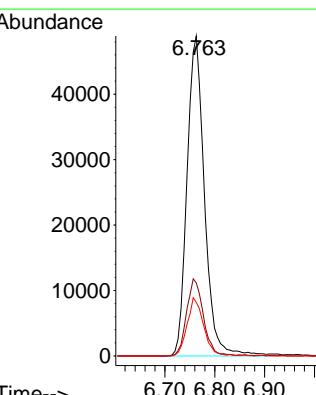

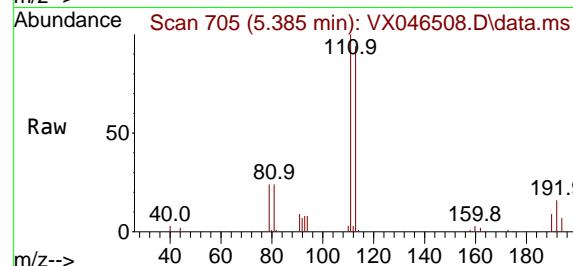

#35

Dibromofluoromethane

Concen: 48.758 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046508.D




Acq: 04 Jun 2025 18:12

Instrument:

MSVOA\_X

ClientSampleId :

RMW-02B-66-060325



#44

Trichloroethene

Concen: 442.298 ug/l

RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12




Tgt Ion:130 Resp: 357950

Ion Ratio Lower Upper

130 100





95 107.1 0.0 204.2

Abundance

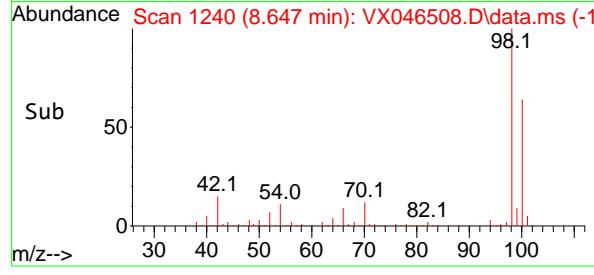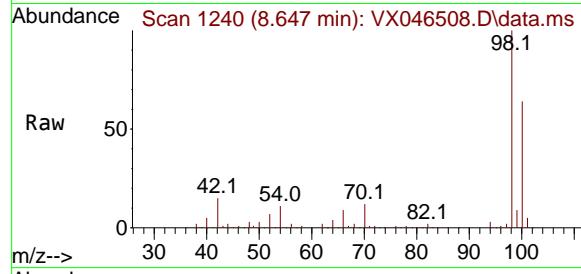


#50  
Toluene-d8  
Concen: 49.732 ug/l  
RT: 8.647 min Scan# 1  
Instrument: MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046508.D  
ClientSampleId : RMW-02B-66-060325  
Acq: 04 Jun 2025 18:12




Tgt Ion: 98 Resp: 147066  
Ion Ratio Lower Upper  
98 100  
100 64.0 53.5 80.3

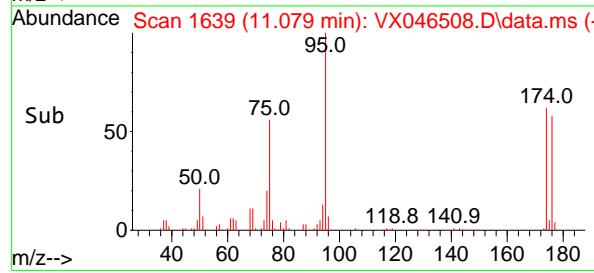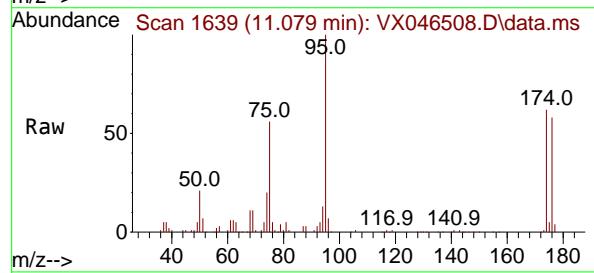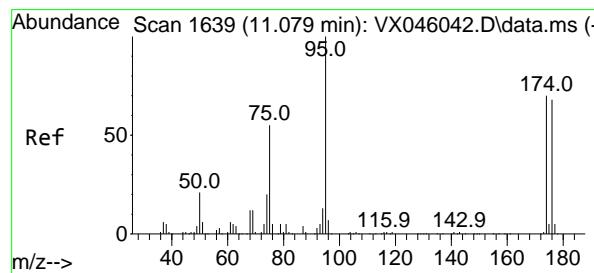

#62  
4-Bromofluorobenzene  
Concen: 48.759 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX046508.D  
Acq: 04 Jun 2025 18:12

Tgt Ion: 95 Resp: 55309  
Ion Ratio Lower Upper  
95 100  
174 66.7 0.0 135.8  
176 63.6 0.0 131.4

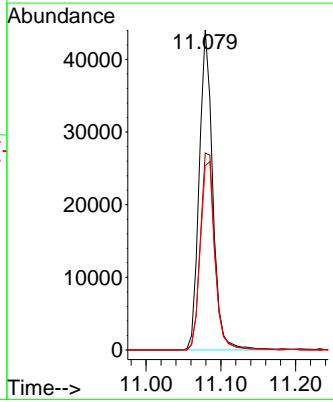

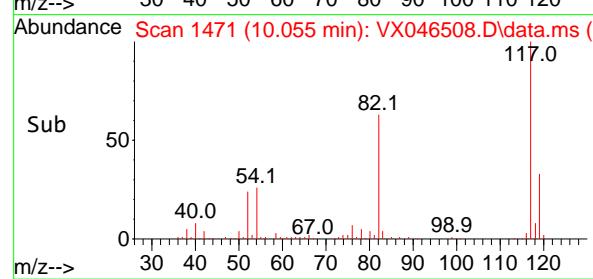

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046508.D




Acq: 04 Jun 2025 18:12

Instrument:

MSVOA\_X

ClientSampleId :

RMW-02B-66-060325

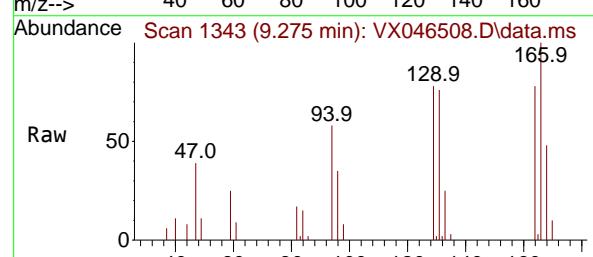

#64

Tetrachloroethene

Concen: 6.334 ug/l

RT: 9.275 min Scan# 1343

Delta R.T. 0.006 min

Lab File: VX046508.D

Acq: 04 Jun 2025 18:12

Tgt Ion:164 Resp: 4825



Ion Ratio Lower Upper


164 100

166 127.9 105.0 157.6

129 99.4 83.5 125.3

131 97.2 76.5 114.7

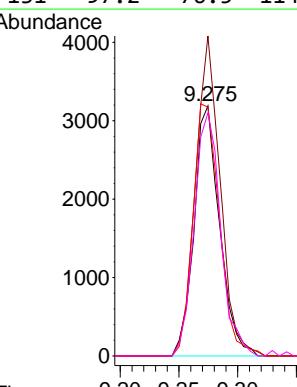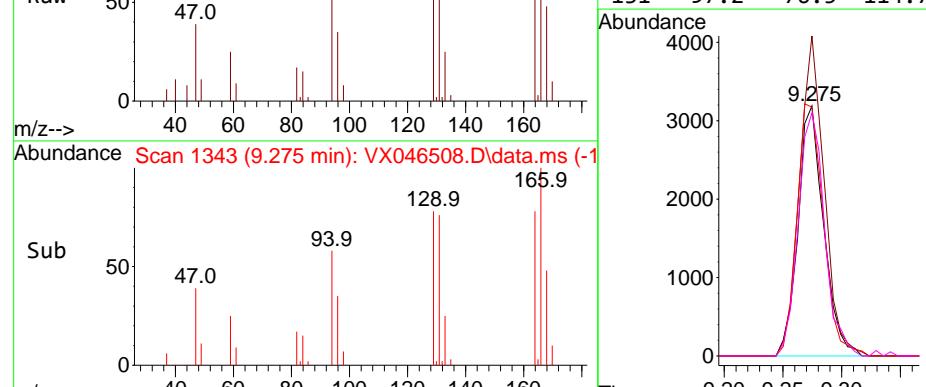


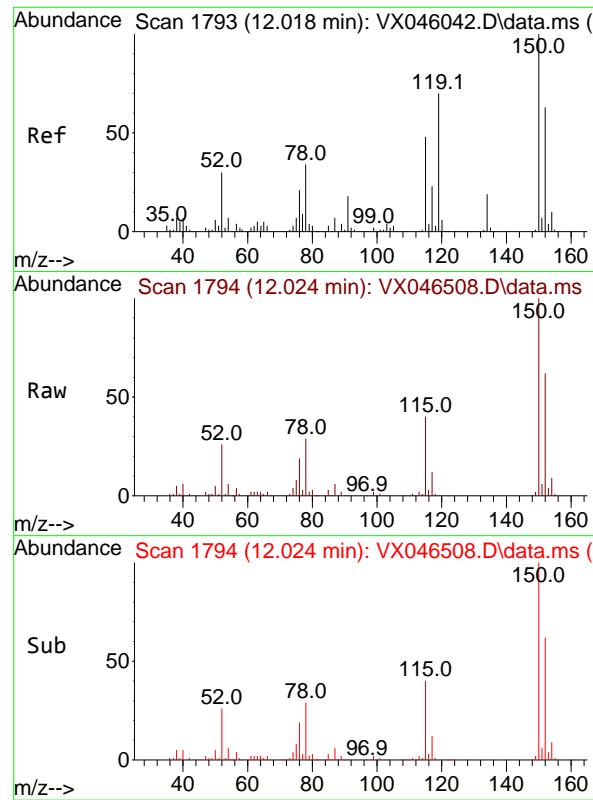

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX046508.D  
Acq: 04 Jun 2025 18:12

Instrument : MSVOA\_X  
ClientSampleId : RMW-02B-66-060325

Tgt Ion:152 Resp: 43595  
Ion Ratio Lower Upper  
152 100  
115 65.7 46.9 140.7  
150 157.9 0.0 351.0

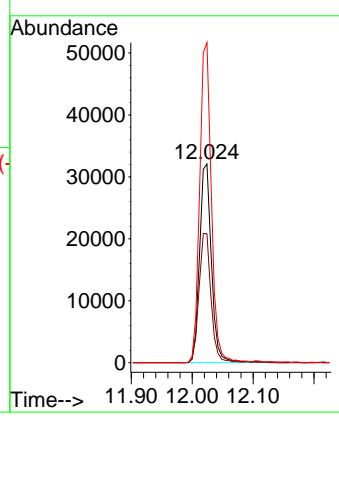



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	06/03/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	06/03/25	
Client Sample ID:	RMW-02B-66-060325DL			SDG No.:	Q2200	
Lab Sample ID:	Q2200-01DL			Matrix:	Water	
Analytical Method:	8260D			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046498.D	100		06/04/25 14:15	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	82.3	JD	26.0	100	ug/L
75-35-4	1,1-Dichloroethene	210	D	23.0	100	ug/L
75-34-3	1,1-Dichloroethane	23.0	UD	23.0	100	ug/L
156-59-2	cis-1,2-Dichloroethene	1700	D	19.0	100	ug/L
71-55-6	1,1,1-Trichloroethane	20.0	UD	20.0	100	ug/L
71-43-2	Benzene	15.0	UD	15.0	100	ug/L
107-06-2	1,2-Dichloroethane	22.0	UD	22.0	100	ug/L
79-01-6	Trichloroethene	4300	D	9.30	100	ug/L
79-00-5	1,1,2-Trichloroethane	21.0	UD	21.0	100	ug/L
127-18-4	Tetrachloroethene	61.6	JD	23.0	100	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	51.3		70 (74) - 130 (125)	103%	SPK: 50
1868-53-7	Dibromofluoromethane	50.4		70 (75) - 130 (124)	101%	SPK: 50
2037-26-5	Toluene-d8	50.0		70 (86) - 130 (113)	100%	SPK: 50
460-00-4	4-Bromofluorobenzene	53.4		70 (77) - 130 (121)	107%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	63000	5.55			
540-36-3	1,4-Difluorobenzene	125000	6.757			
3114-55-4	Chlorobenzene-d5	119000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	53600	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046498.D  
 Acq On : 04 Jun 2025 14:15  
 Operator : JC/MD  
 Sample : Q2200-01DL 100X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**RMW-02B-66-060325DL**

Quant Time: Jun 05 01:54:31 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	62989	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	125027	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	118665	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	53639	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	60283	51.335	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	102.660%	
35) Dibromofluoromethane	5.385	113	45387	50.412	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	100.820%	
50) Toluene-d8	8.646	98	155704	49.967	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	99.940%	
62) 4-Bromofluorobenzene	11.079	95	63770	53.350	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	106.700%	
<b>Target Compounds</b>						
				Qvalue		
4) Vinyl Chloride	1.373	62	716	0.823	ug/l	98
12) 1,1-Dichloroethene	2.312	96	1603	2.146	ug/l	# 91
27) cis-1,2-Dichloroethene	4.489	96	15418	17.051	ug/l	88
44) Trichloroethene	7.122	130	36397	42.679	ug/l	97
64) Tetrachloroethene	9.268	164	517	0.616	ug/l	91







(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046498.D  
 Acq On : 04 Jun 2025 14:15  
 Operator : JC/MD  
 Sample : Q2200-01DL 100X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RMW-02B-66-060325DL

Quant Time: Jun 05 01:54:31 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

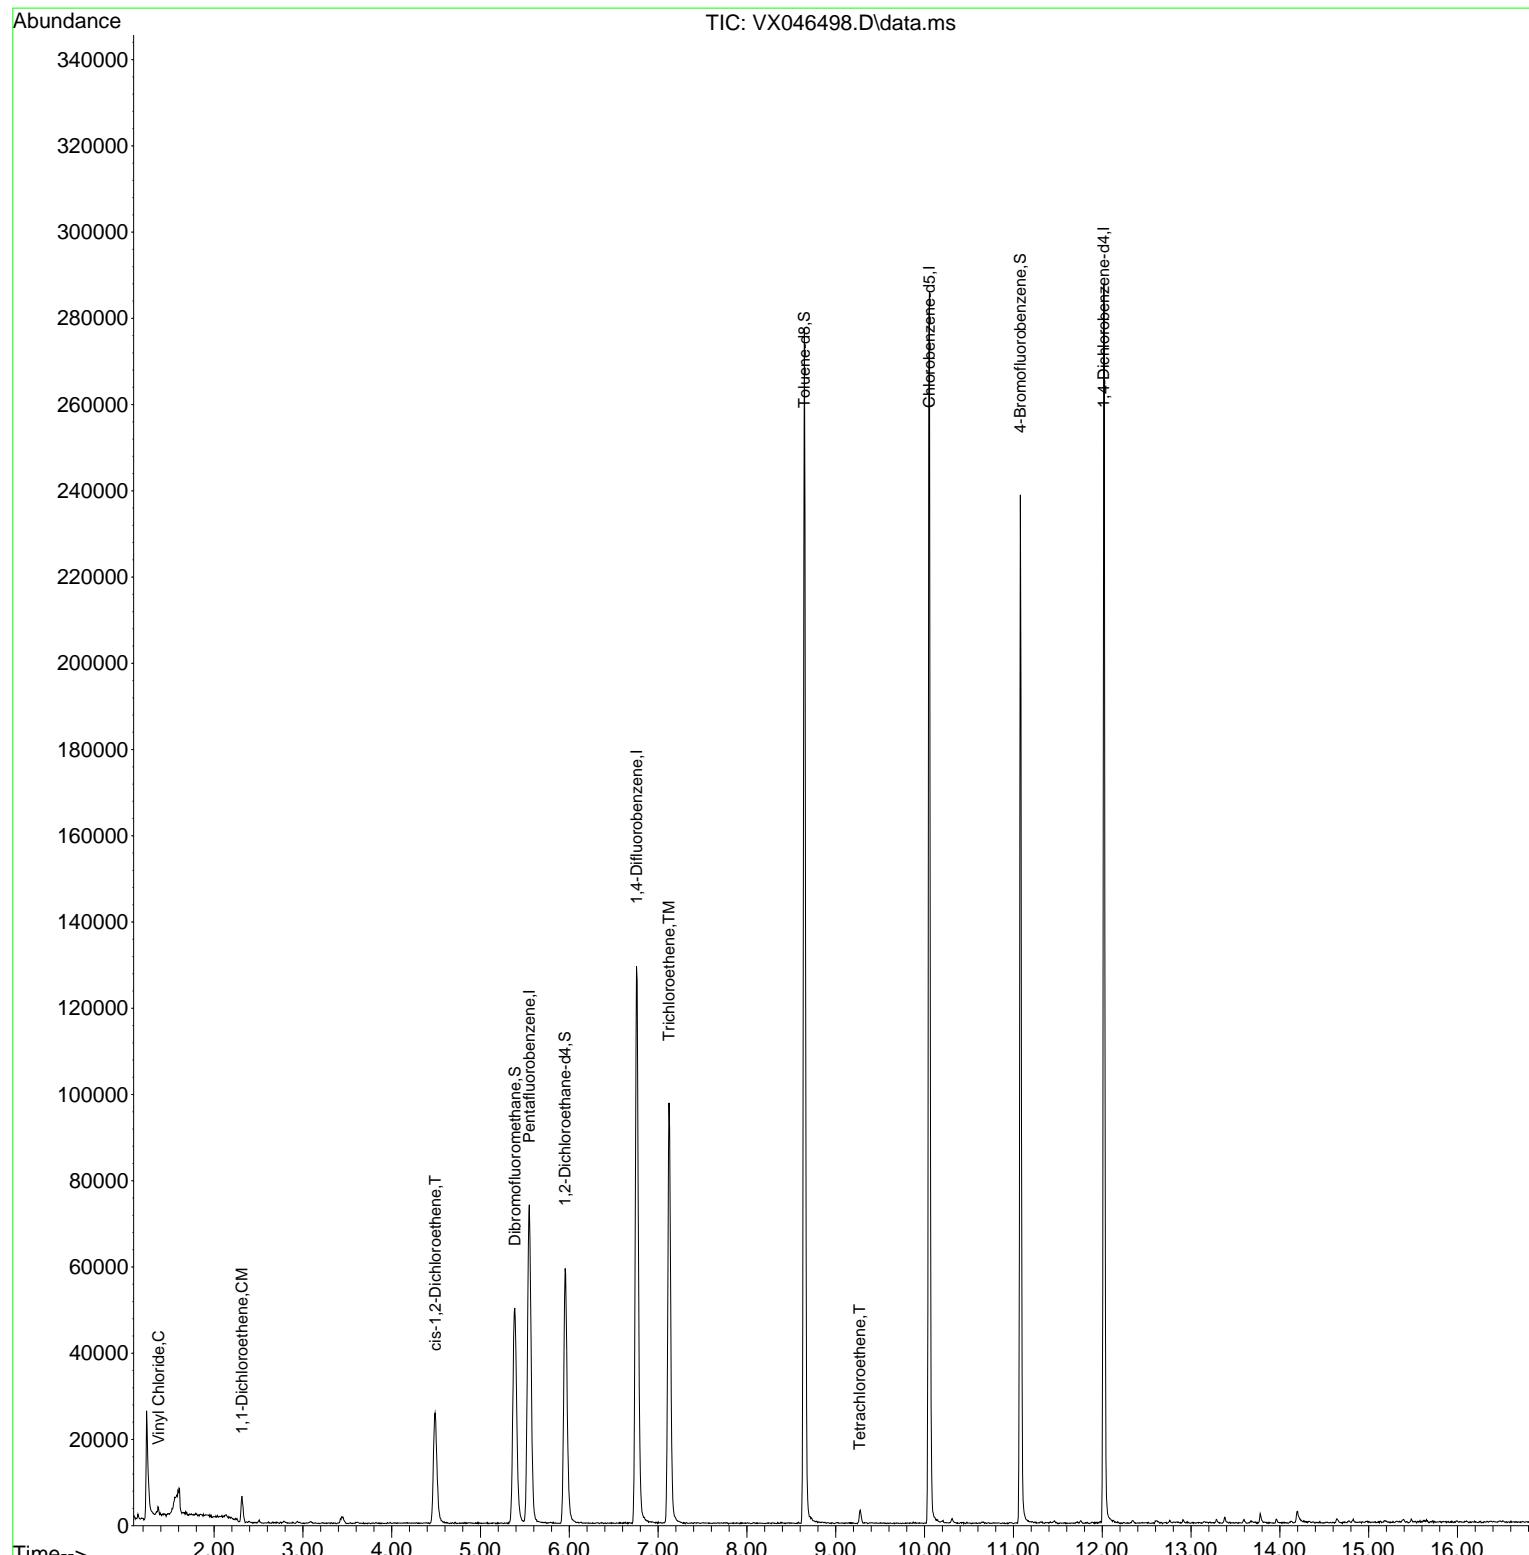

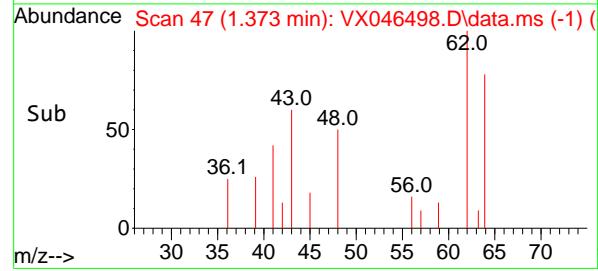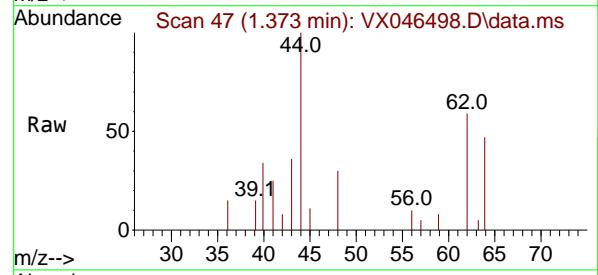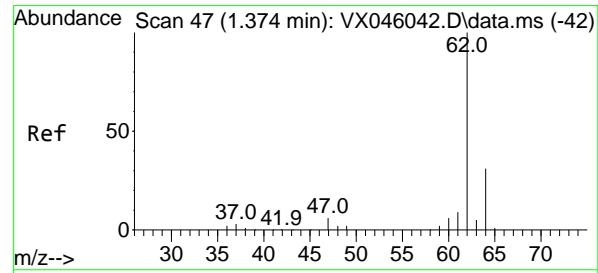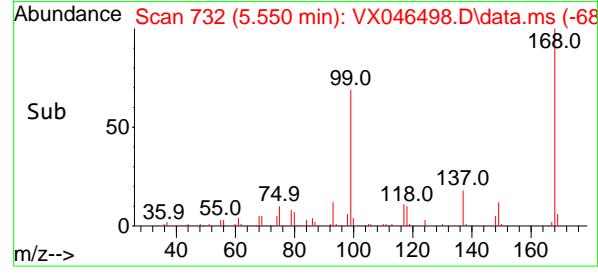

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15

Instrument :

MSVOA\_X

ClientSampleId :

RMW-02B-66-060325DL

Tgt Ion:168 Resp: 62989


Ion Ratio Lower Upper

168 100

99 69.3

54.9

82.3

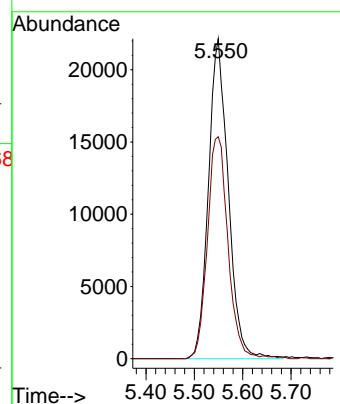

#4

Vinyl Chloride

Concen: 0.823 ug/l

RT: 1.373 min Scan# 47

Delta R.T. -0.000 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15

Tgt Ion: 62 Resp: 716


Ion Ratio Lower Upper




62 100

64 32.4

25.2

37.8

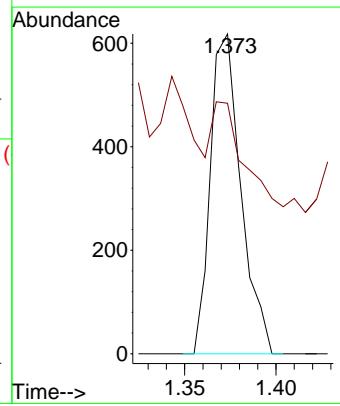



#12

1,1-Dichloroethene

Concen: 2.146 ug/l

RT: 2.312 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15

Instrument:

MSVOA\_X

ClientSampleId :

RMW-02B-66-060325DL





Tgt Ion: 96 Resp: 1603

Ion Ratio Lower Upper

96 100

61 175.4 146.2 219.2

98 47.9 51.0 76.6#

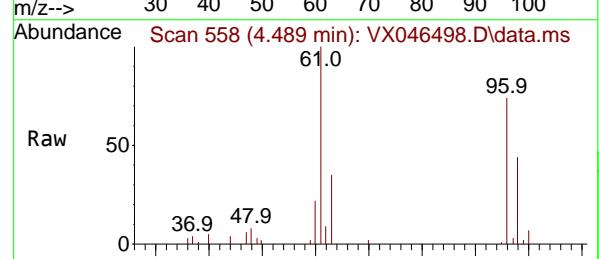

#27

cis-1,2-Dichloroethene

Concen: 17.051 ug/l

RT: 4.489 min Scan# 558

Delta R.T. 0.006 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15


Tgt Ion: 96 Resp: 15418







Ion Ratio Lower Upper

96 100

61 141.3 0.0 322.8

98 68.6 0.0 129.0

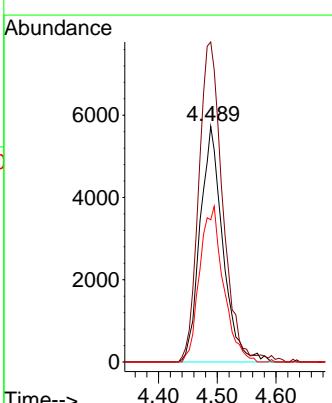

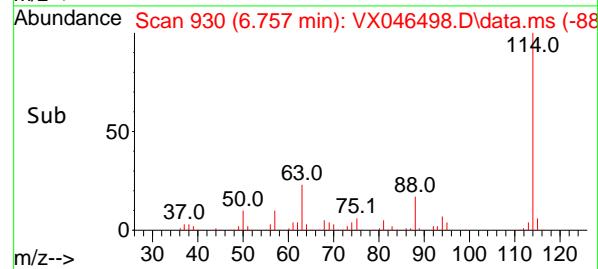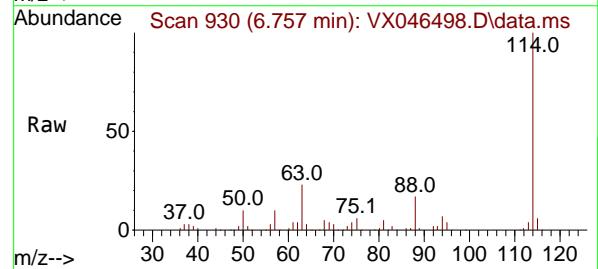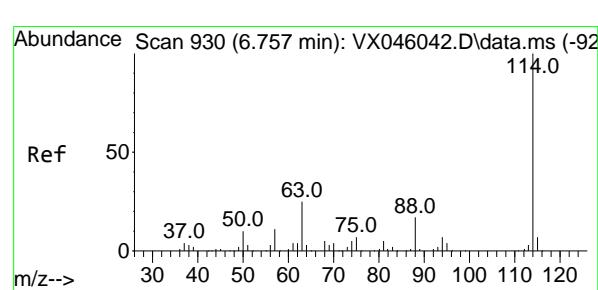

#33

1,2-Dichloroethane-d4

Concen: 51.335 ug/l

RT: 5.952 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15

Instrument:

MSVOA\_X

ClientSampleId :


RMW-02B-66-060325DL

Tgt Ion: 65 Resp: 60283

Ion Ratio Lower Upper

65 100

67 50.0 0.0 99.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15


Tgt Ion: 114 Resp: 125027


Ion Ratio Lower Upper

114 100

63 23.3 0.0 49.2

88 17.0 0.0 33.6



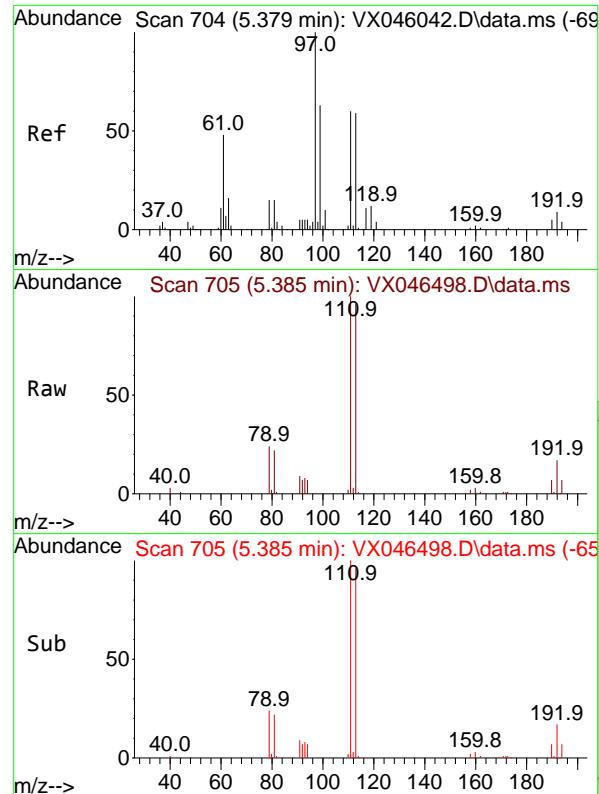

#35

Dibromofluoromethane

Concen: 50.412 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15

Instrument : MSVOA\_X  
 ClientSampleId : RMW-02B-66-060325DL

Tgt Ion:113 Resp: 45387

Ion Ratio Lower Upper

113 100

111 101.3 83.1 124.7

192 16.1 13.3 19.9

Abundance

15000

10000


5000

0

5.385

Time--&gt;

5.20 5.40 5.60

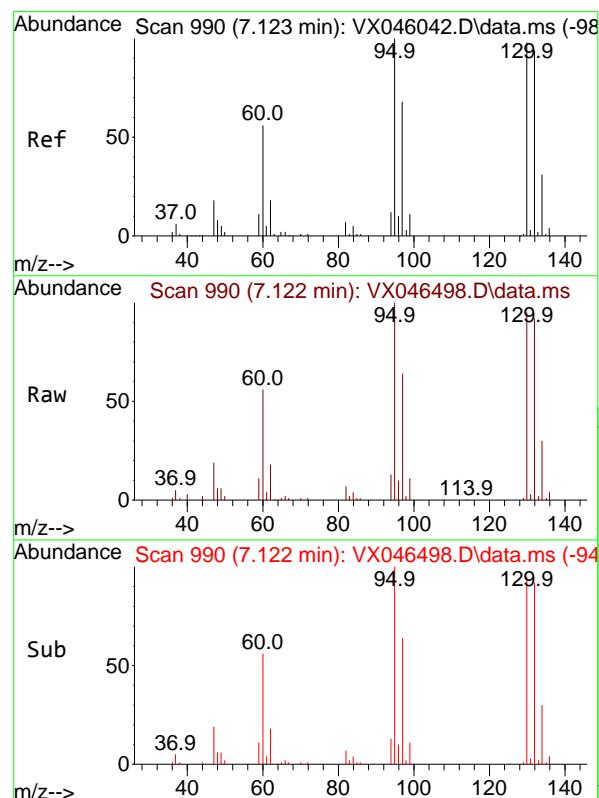

#44

Trichloroethene

Concen: 42.679 ug/l

RT: 7.122 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15

Tgt Ion:130 Resp: 36397

Ion Ratio Lower Upper

130 100

95 104.8 0.0 204.2

Abundance

15000

10000


5000

0

7.122


Time--&gt;

7.00 7.10 7.20 7.30






#50  
Toluene-d8  
Concen: 49.967 ug/l  
RT: 8.646 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046498.D  
Acq: 04 Jun 2025 14:15


Instrument : MSVOA\_X  
ClientSampleId : RMW-02B-66-060325DL





Tgt Ion: 98 Resp: 155704  
Ion Ratio Lower Upper  
98 100  
100 65.0 53.5 80.3

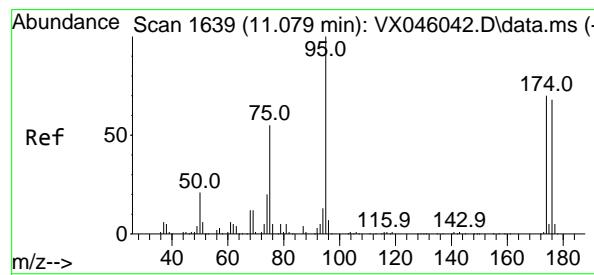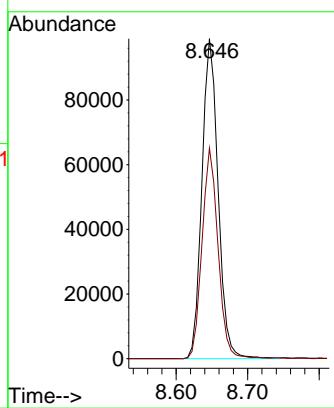


#62  
4-Bromofluorobenzene  
Concen: 53.350 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX046498.D  
Acq: 04 Jun 2025 14:15

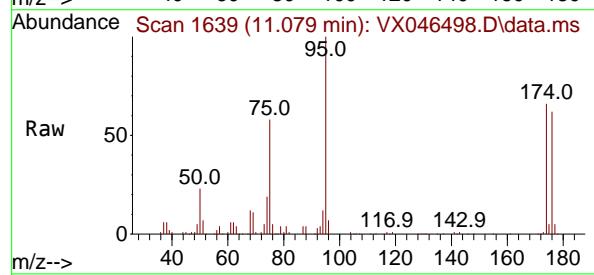



Tgt Ion: 95 Resp: 63770  
Ion Ratio Lower Upper  
95 100  
174 67.4 0.0 135.8  
176 64.0 0.0 131.4

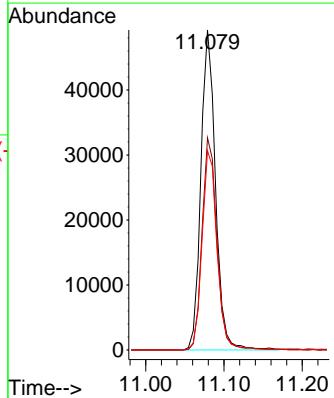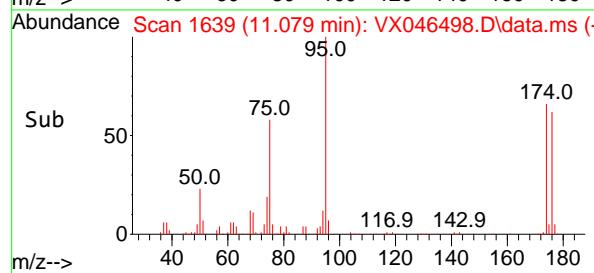

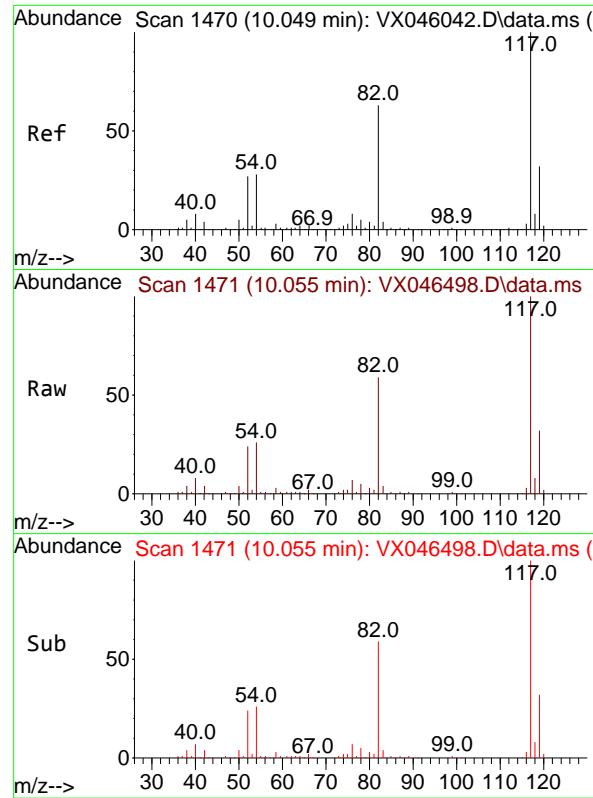


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX046498.D  
Acq: 04 Jun 2025 14:15  
ClientSampleId : RMW-02B-66-060325DL


Tgt Ion:117 Resp: 118665  
Ion Ratio Lower Upper  
117 100  
82 59.1 50.6 76.0  
119 31.7 25.8 38.6

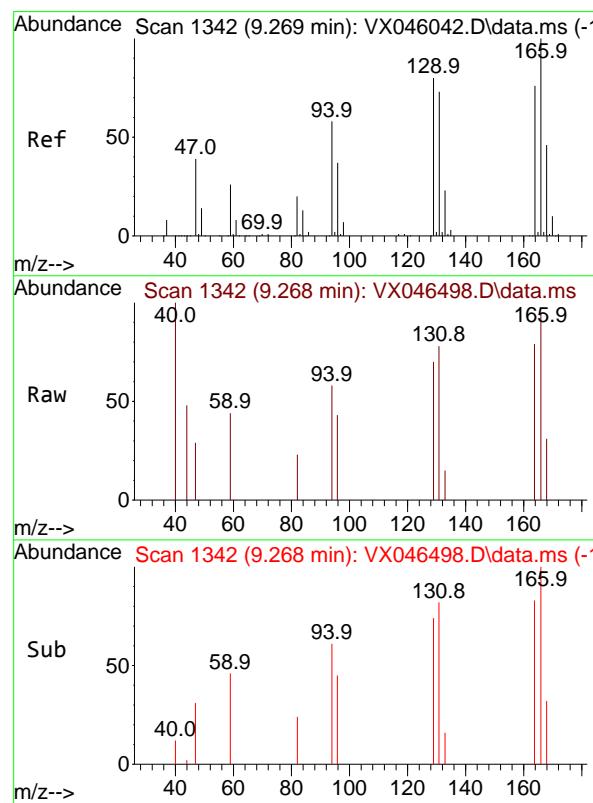

#64  
Tetrachloroethene  
Concen: 0.616 ug/l  
RT: 9.268 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX046498.D  
Acq: 04 Jun 2025 14:15

Tgt Ion:164 Resp: 517  
Ion Ratio Lower Upper  
164 100  
166 121.0 105.0 157.6  
129 89.3 83.5 125.3  
131 99.7 76.5 114.7

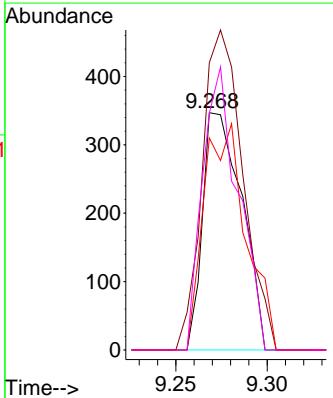

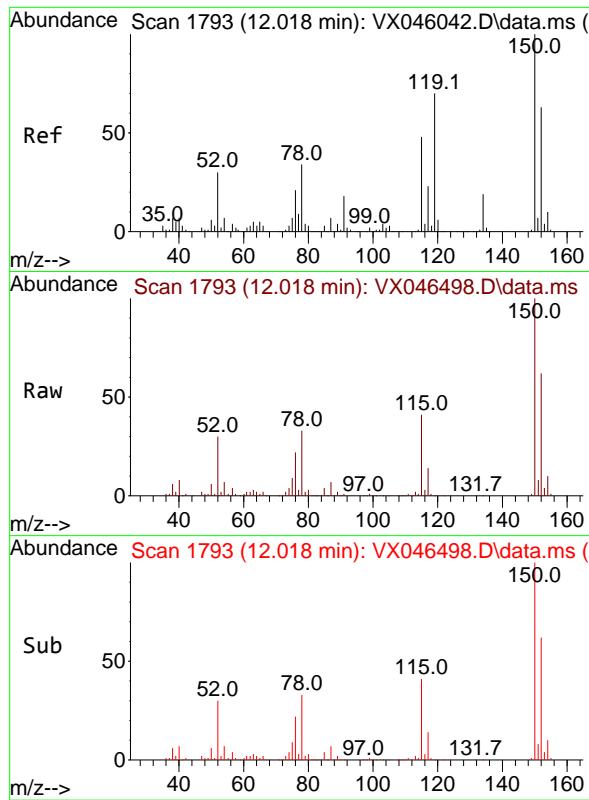

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046498.D

Acq: 04 Jun 2025 14:15

Instrument:

MSVOA\_X

ClientSampleId :

RMW-02B-66-060325DL


Tgt Ion:152 Resp: 53639

Ion Ratio Lower Upper

152 100

115 65.3 46.9 140.7

150 160.9 0.0 351.0

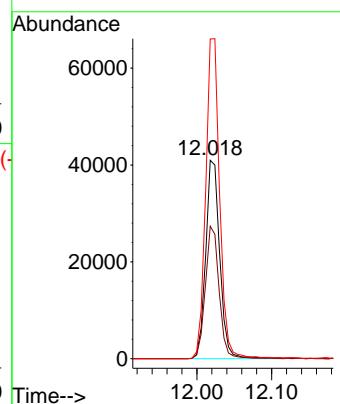



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	06/03/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	06/03/25	
Client Sample ID:	RMW-03B-90-060325			SDG No.:	Q2200	
Lab Sample ID:	Q2200-02			Matrix:	Water	
Analytical Method:	8260D			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046499.D	50		06/04/25 14:39	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	13.0	U	13.0	50.0	ug/L
75-35-4	1,1-Dichloroethene	11.5	U	11.5	50.0	ug/L
75-34-3	1,1-Dichloroethane	11.5	U	11.5	50.0	ug/L
156-59-2	cis-1,2-Dichloroethene	3900		9.50	50.0	ug/L
71-55-6	1,1,1-Trichloroethane	10.0	U	10.0	50.0	ug/L
71-43-2	Benzene	7.50	U	7.50	50.0	ug/L
107-06-2	1,2-Dichloroethane	11.0	U	11.0	50.0	ug/L
79-01-6	Trichloroethene	220		4.70	50.0	ug/L
79-00-5	1,1,2-Trichloroethane	10.5	U	10.5	50.0	ug/L
127-18-4	Tetrachloroethene	11.5	U	11.5	50.0	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	51.0		70 (74) - 130 (125)	102%	SPK: 50
1868-53-7	Dibromofluoromethane	50.2		70 (75) - 130 (124)	100%	SPK: 50
2037-26-5	Toluene-d8	50.4		70 (86) - 130 (113)	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	50.6		70 (77) - 130 (121)	101%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	65900	5.55			
540-36-3	1,4-Difluorobenzene	132000	6.757			
3114-55-4	Chlorobenzene-d5	122000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	49200	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046499.D  
 Acq On : 04 Jun 2025 14:39  
 Operator : JC/MD  
 Sample : Q2200-02 50X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**RMW-03B-90-060325**

Quant Time: Jun 05 01:55:24 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	65911	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	132066	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	121549	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	49186	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	62626	50.965	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	101.940%	
35) Dibromofluoromethane	5.385	113	47755	50.215	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	100.420%	
50) Toluene-d8	8.647	98	165809	50.374	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	100.740%	
62) 4-Bromofluorobenzene	11.079	95	63901	50.610	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	101.220%	
<b>Target Compounds</b>						
				Qvalue		
9) 1,1,2-Trichlorotrifluo...	2.319	101	51247	61.541	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	73087	77.246	ug/l	89
44) Trichloroethene	7.123	130	3998	4.438	ug/l	92







(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
Data File : VX046499.D  
Acq On : 04 Jun 2025 14:39  
Operator : JC/MD  
Sample : Q2200-02 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RMW-03B-90-060325

Quant Time: Jun 05 01:55:24 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

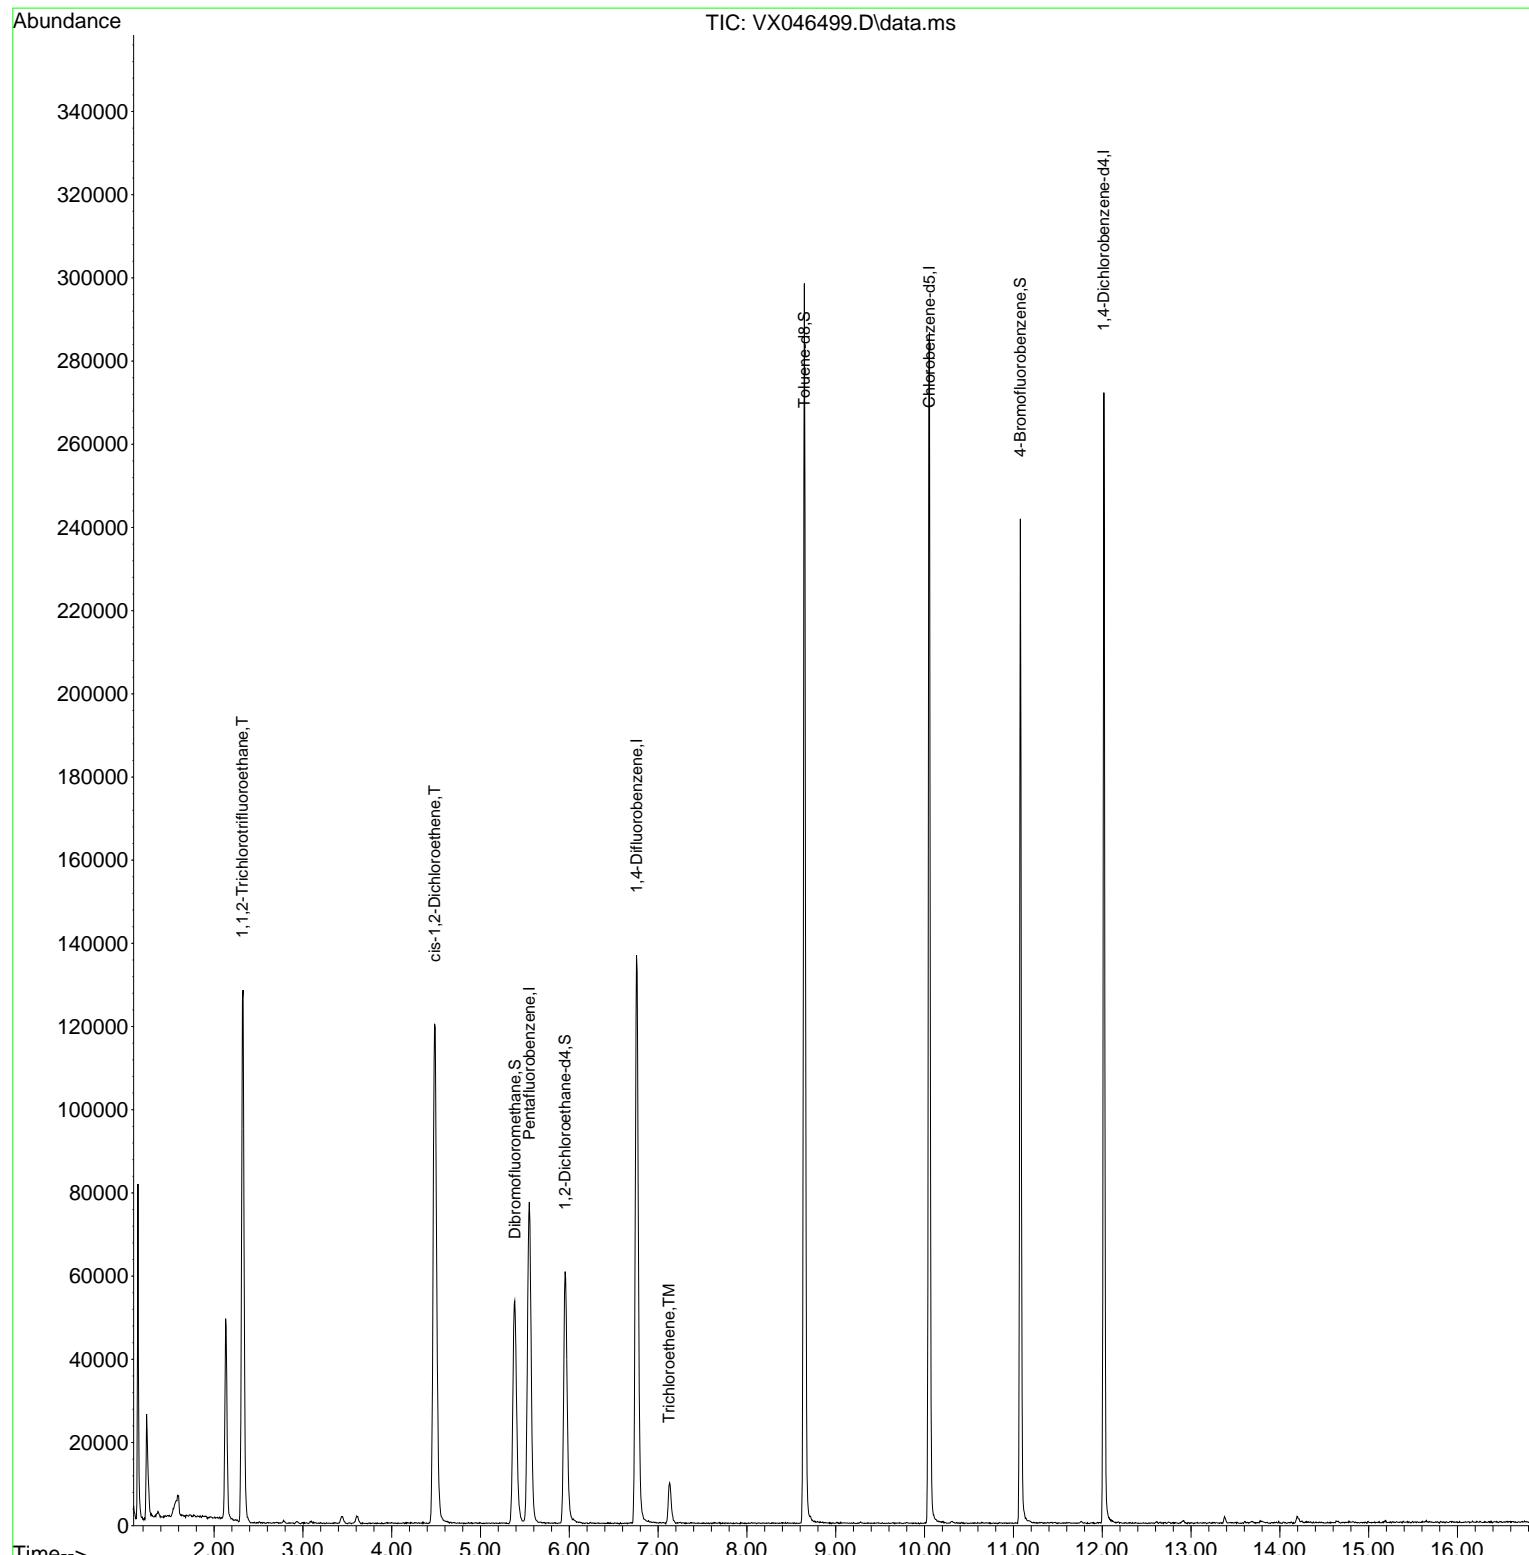



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046499.D

Acq: 04 Jun 2025 14:39

Instrument:

MSVOA\_X

ClientSampleId :

RMW-03B-90-060325

Tgt Ion:168 Resp: 65911


Ion Ratio Lower Upper

168 100

99 76.7

54.9

82.3

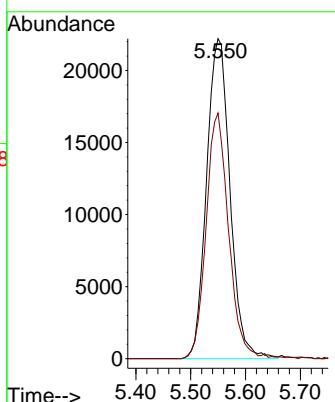

#9

1,1,2-Trichlorotrifluoroethane

Concen: 61.541 ug/l

RT: 2.319 min Scan# 202

Delta R.T. -0.000 min

Lab File: VX046499.D

Acq: 04 Jun 2025 14:39

Tgt Ion:101 Resp: 51247

Ion Ratio Lower Upper

101 100

85 47.4


38.6




58.0

151 70.2

55.2

82.8



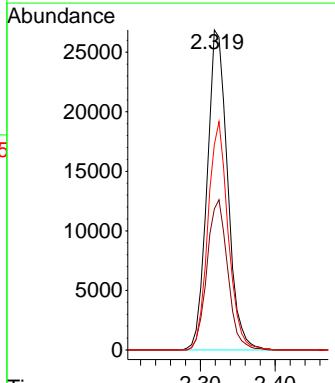




#27  
cis-1,2-Dichloroethene  
Concen: 77.246 ug/l  
RT: 4.483 min Scan# 5  
Delta R.T. -0.000 min  
Lab File: VX046499.D  
Acq: 04 Jun 2025 14:39



Instrument : MSVOA\_X  
ClientSampleId : RMW-03B-90-060325


Tgt Ion: 96 Resp: 73087  
Ion Ratio Lower Upper  
96 100  
61 140.7 0.0 322.8  
98 64.8 0.0 129.0

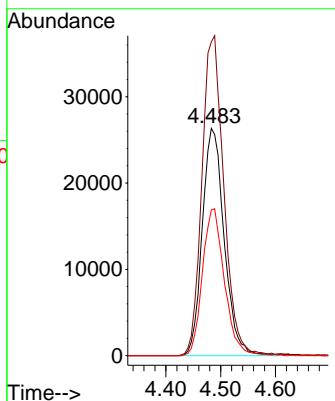

#33  
1,2-Dichloroethane-d4  
Concen: 50.965 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.000 min  
Lab File: VX046499.D  
Acq: 04 Jun 2025 14:39

Tgt Ion: 65 Resp: 62626  
Ion Ratio Lower Upper  
65 100  
67 50.3 0.0 99.0

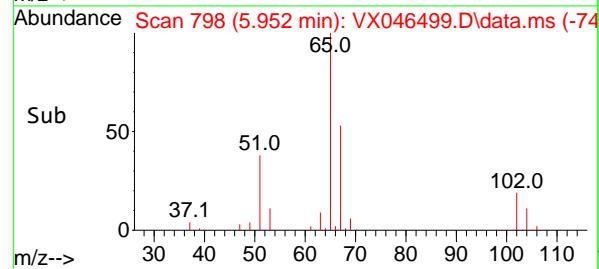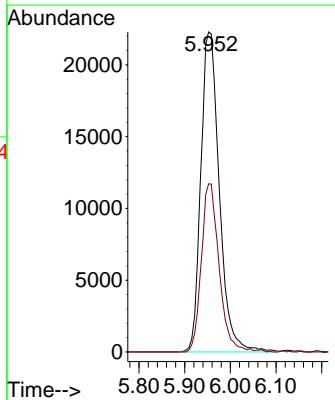

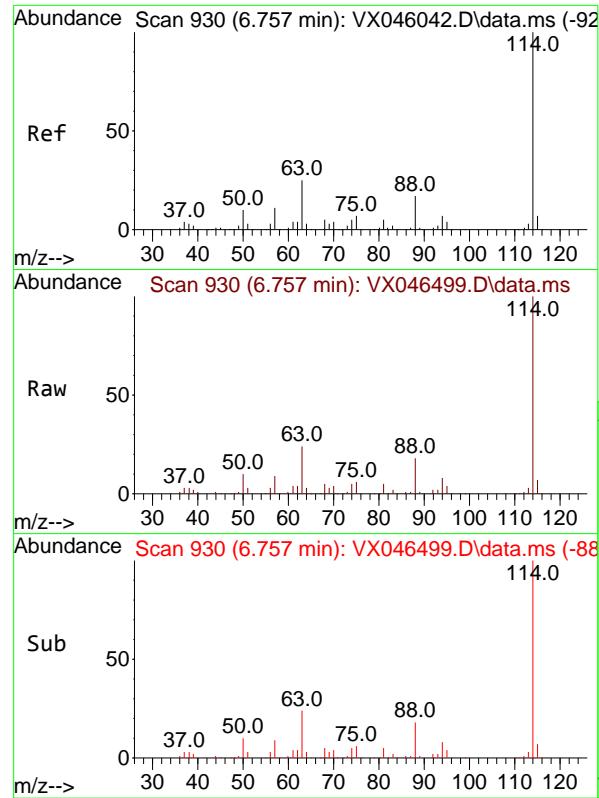

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Delta R.T. -0.000 min

Lab File: VX046499.D


Acq: 04 Jun 2025 14:39

Instrument:

MSVOA\_X

ClientSampleId :

RMW-03B-90-060325

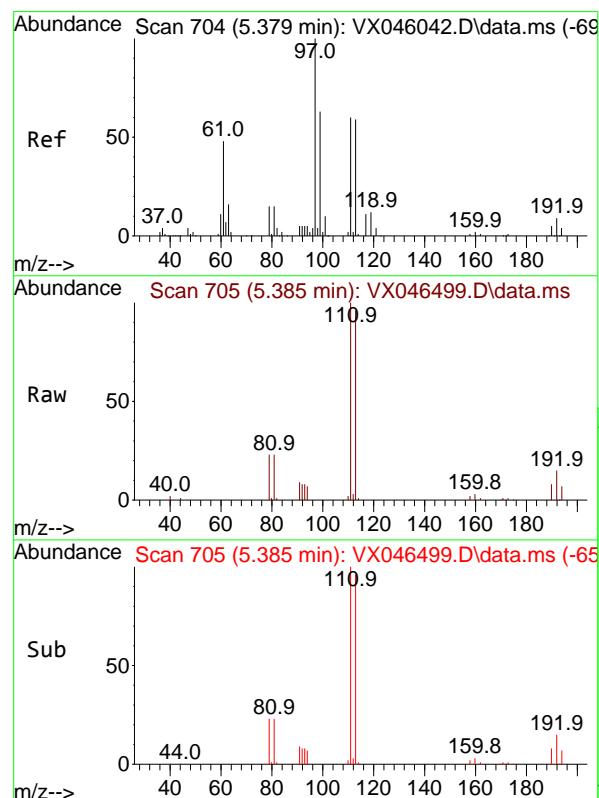

#35

Dibromofluoromethane

Concen: 50.215 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX046499.D

Acq: 04 Jun 2025 14:39


Tgt Ion:113 Resp: 47755


Ion Ratio Lower Upper

113 100

111 101.8 83.1 124.7


192 16.5 13.3 19.9

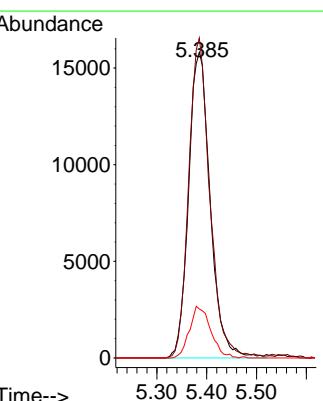






#44  
Trichloroethene  
Concen: 4.438 ug/l  
RT: 7.123 min Scan# 990  
Delta R.T. -0.000 min  
Lab File: VX046499.D  
Acq: 04 Jun 2025 14:39


Instrument: MSVOA\_X  
ClientSampleId : RMW-03B-90-060325





Tgt Ion:130 Resp: 3998  
Ion Ratio Lower Upper  
130 100  
95 110.0 0.0 204.2



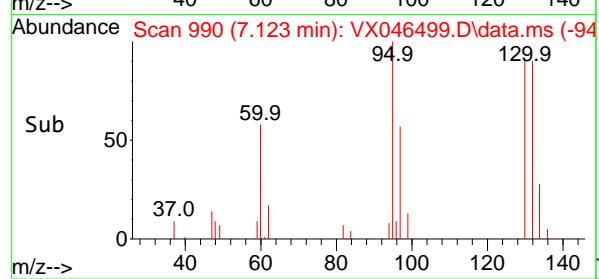


#50  
Toluene-d8  
Concen: 50.374 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. -0.000 min  
Lab File: VX046499.D  
Acq: 04 Jun 2025 14:39



Tgt Ion: 98 Resp: 165809  
Ion Ratio Lower Upper  
98 100  
100 65.7 53.5 80.3

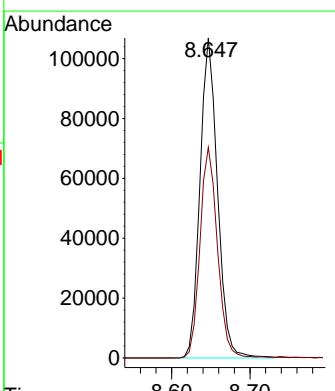



#62

4-Bromofluorobenzene

Concen: 50.610 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046499.D

Acq: 04 Jun 2025 14:39

Instrument:

MSVOA\_X

ClientSampleId :

RMW-03B-90-060325





Tgt Ion: 95 Resp: 63901

Ion Ratio Lower Upper

95 100

174 65.9 0.0 135.8

176 63.6 0.0 131.4

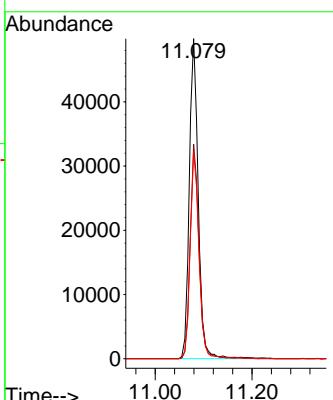

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.006 min

Lab File: VX046499.D

Acq: 04 Jun 2025 14:39


Tgt Ion:117 Resp: 121549


Ion Ratio Lower Upper

117 100

82 60.4 50.6 76.0

119 31.8 25.8 38.6




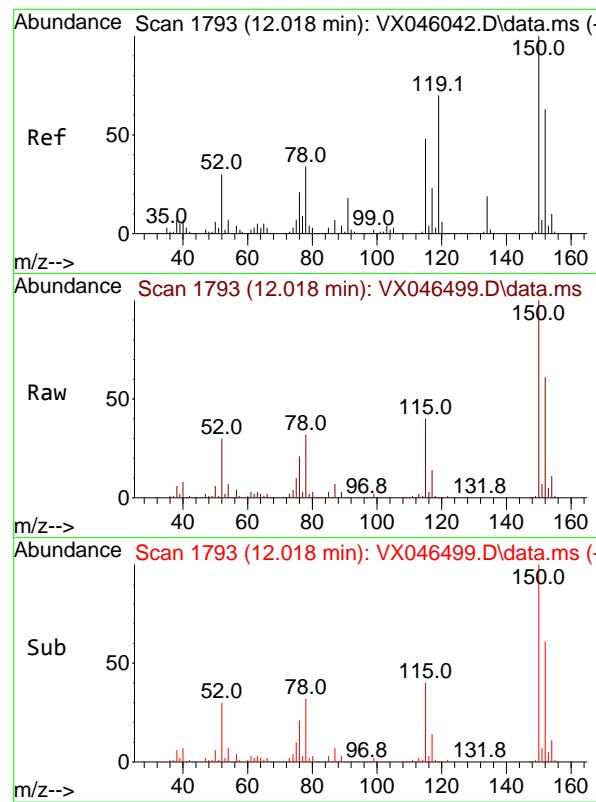

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046499.D  
Acq: 04 Jun 2025 14:39

Instrument : MSVOA\_X  
ClientSampleId : RMW-03B-90-060325

Tgt Ion:152 Resp: 49186  
Ion Ratio Lower Upper  
152 100  
115 66.0 46.9 140.7  
150 163.5 0.0 351.0

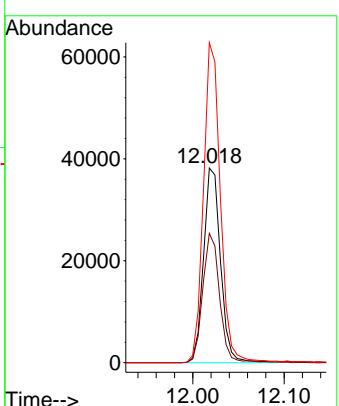



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	06/03/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	06/03/25	
Client Sample ID:	EB01-060325			SDG No.:	Q2200	
Lab Sample ID:	Q2200-03			Matrix:	Water	
Analytical Method:	8260D			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046504.D	1		06/04/25 16:37	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	52.3		70 (74) - 130 (125)	105%	SPK: 50
1868-53-7	Dibromofluoromethane	49.5		70 (75) - 130 (124)	99%	SPK: 50
2037-26-5	Toluene-d8	50.7		70 (86) - 130 (113)	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	52.7		70 (77) - 130 (121)	105%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	64000	5.544			
540-36-3	1,4-Difluorobenzene	128000	6.763			
3114-55-4	Chlorobenzene-d5	122000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	54000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046504.D  
 Acq On : 04 Jun 2025 16:37  
 Operator : JC/MD  
 Sample : Q2200-03  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EB01-060325

Quant Time: Jun 05 02:01:09 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	64028	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	128366	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	122354	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	53968	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.958	65	62415	52.288	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	104.580%	
35) Dibromofluoromethane	5.385	113	45744	49.487	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	98.980%	
50) Toluene-d8	8.647	98	162070	50.657	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	101.320%	
62) 4-Bromofluorobenzene	11.079	95	64642	52.673	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	105.340%	
<b>Target Compounds</b>						
				Qvalue		
16) Acetone	2.380	43	3467	7.244	ug/l	96
30) Chloroform	5.092	83	2645	1.626	ug/l	96
37) Ethyl Acetate	4.733	43	5638	3.674	ug/l #	81




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046504.D  
 Acq On : 04 Jun 2025 16:37  
 Operator : JC/MD  
 Sample : Q2200-03  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EB01-060325




Quant Time: Jun 05 02:01:09 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

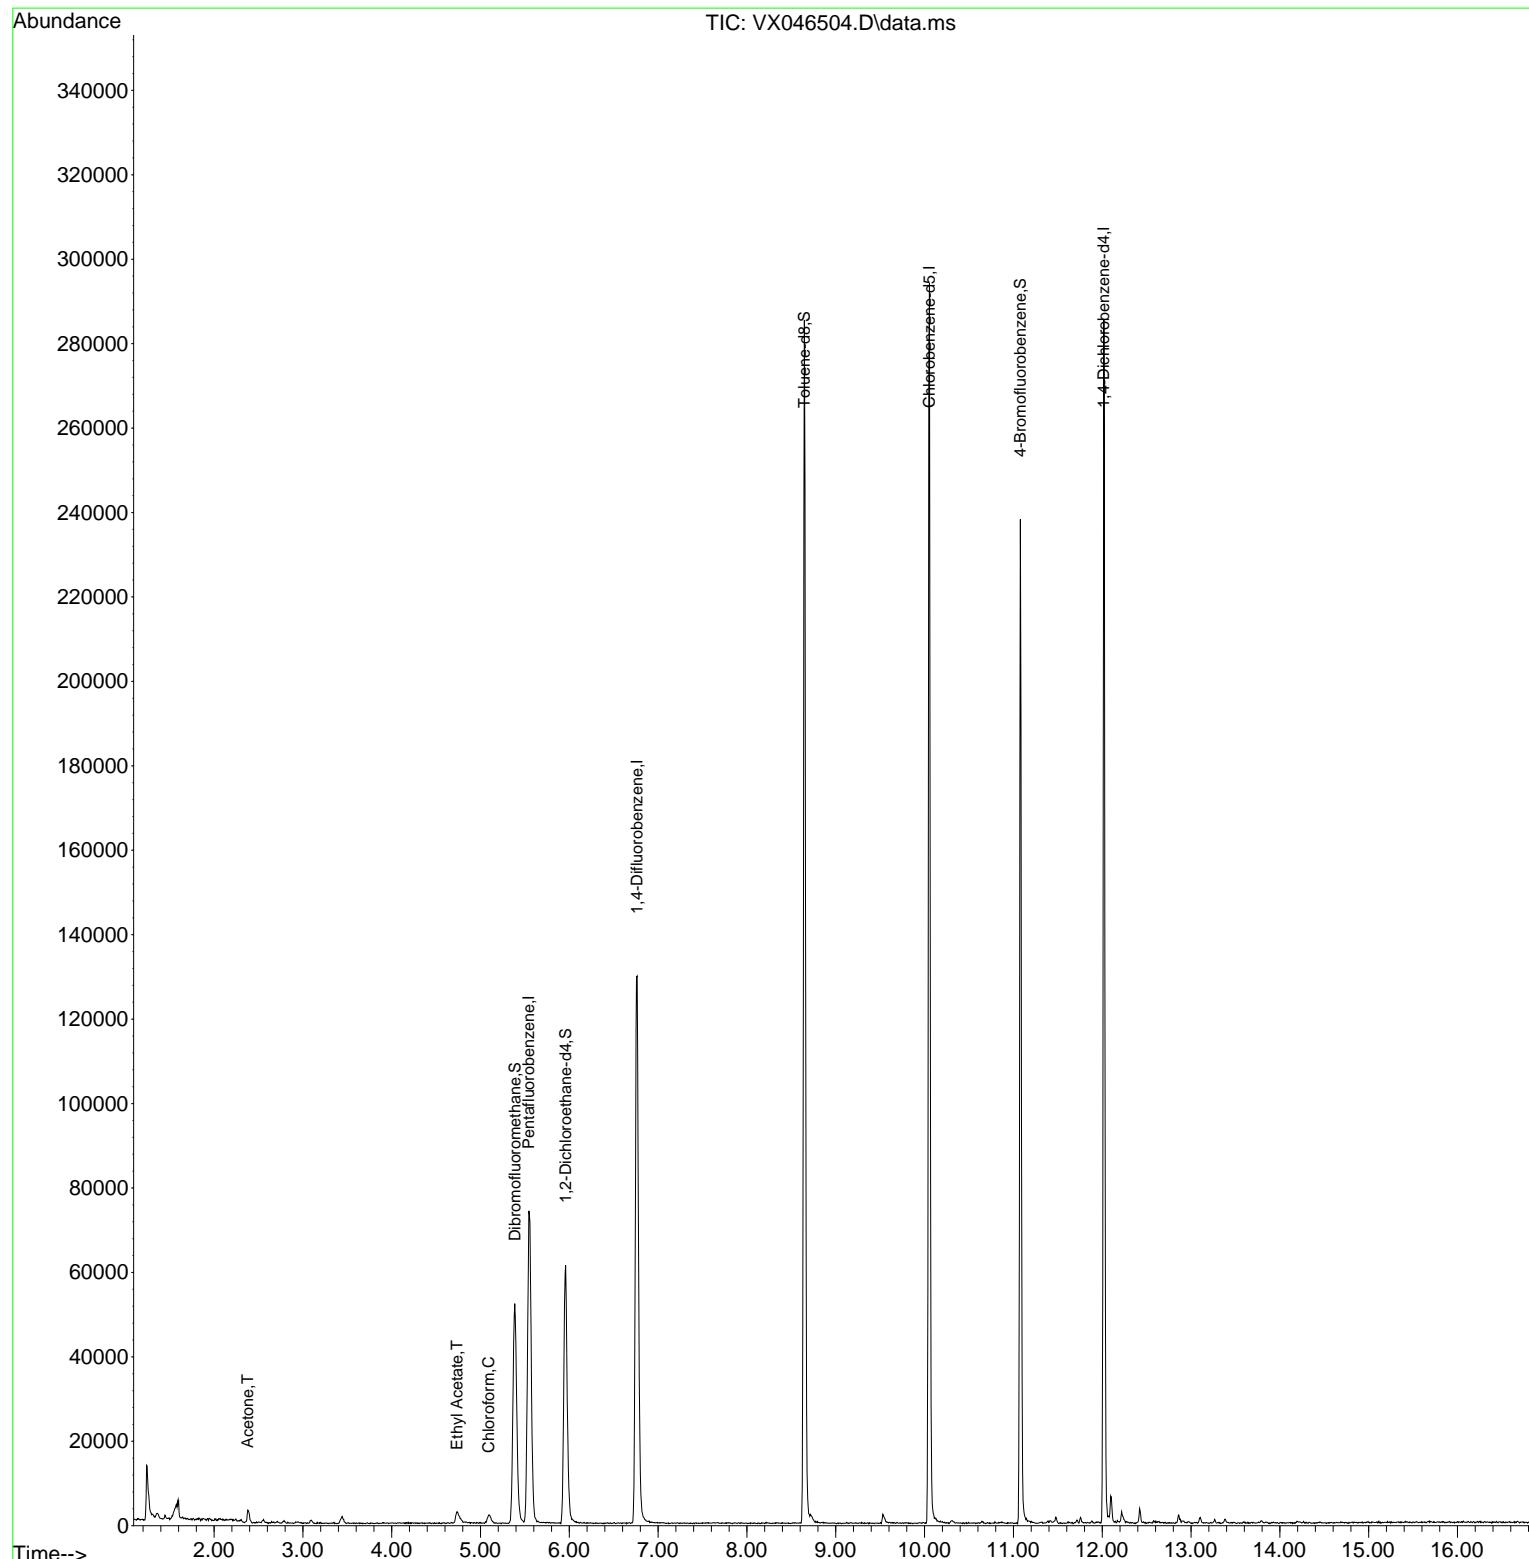

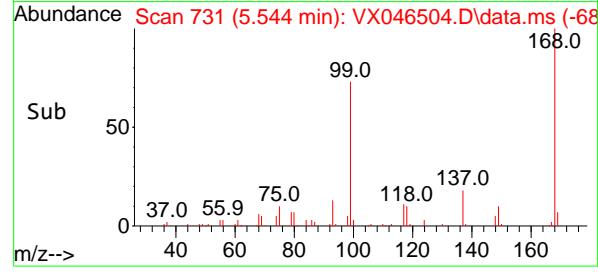



#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.544 min Scan# 7  
Instrument: MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046504.D  
Acq: 04 Jun 2025 16:37  
ClientSampleId : EB01-060325







Tgt Ion:168 Resp: 64028  
Ion Ratio Lower Upper  
168 100  
99 72.6 54.9 82.3

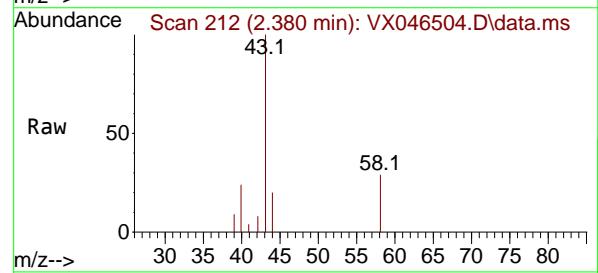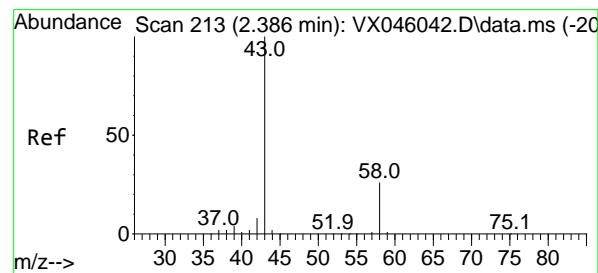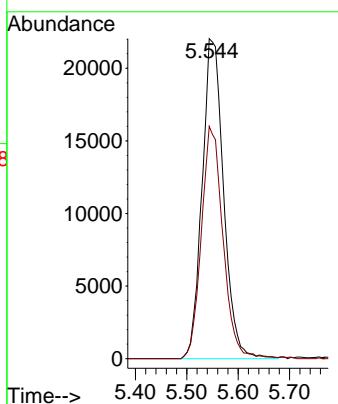

#16  
Acetone  
Concen: 7.244 ug/l  
RT: 2.380 min Scan# 212  
Delta R.T. -0.006 min  
Lab File: VX046504.D  
Acq: 04 Jun 2025 16:37

Tgt Ion: 43 Resp: 3467  
Ion Ratio Lower Upper  
43 100  
58 28.6 21.2 31.8

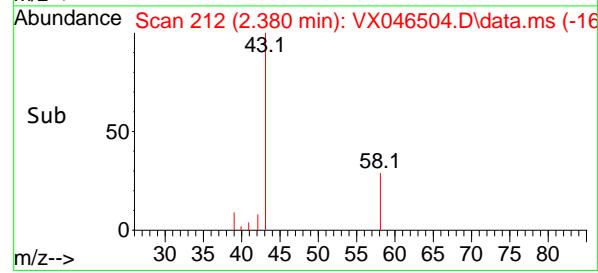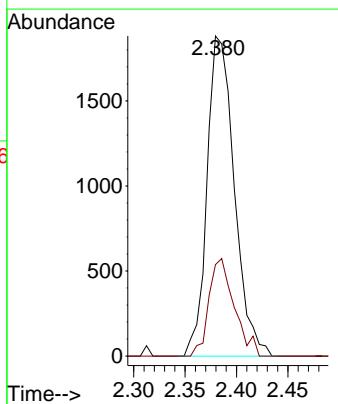

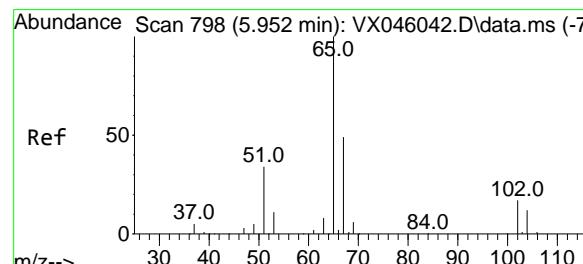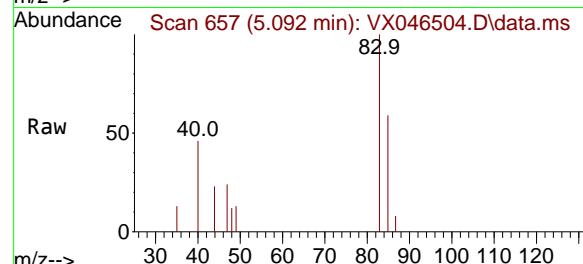

#30

Chloroform

Concen: 1.626 ug/l

RT: 5.092 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX046504.D

Acq: 04 Jun 2025 16:37

Instrument:

MSVOA\_X

ClientSampleId :


EB01-060325

Tgt Ion: 83 Resp: 2645

Ion Ratio Lower Upper

83 100

85 58.7 49.3 73.9

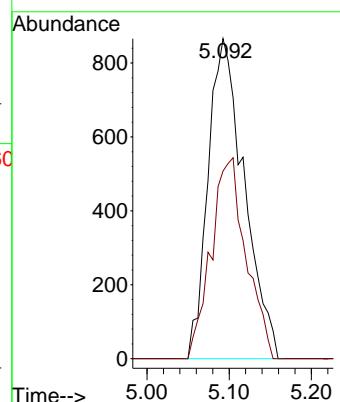

#33

1,2-Dichloroethane-d4

Concen: 52.288 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.006 min

Lab File: VX046504.D


Acq: 04 Jun 2025 16:37


Tgt Ion: 65 Resp: 62415

Ion Ratio Lower Upper

65 100

67 49.2 0.0 99.0

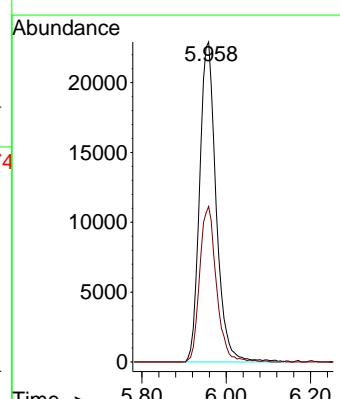

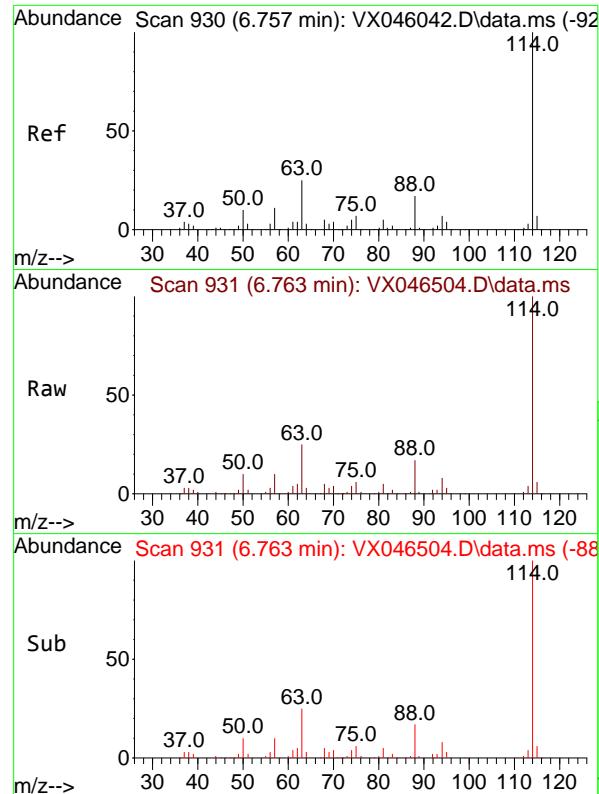



#34

1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 9

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB01-060325

Tgt Ion:114 Resp: 128366

Ion	Ratio	Lower	Upper
114	100		
63	24.8	0.0	49.2
88	16.7	0.0	33.6

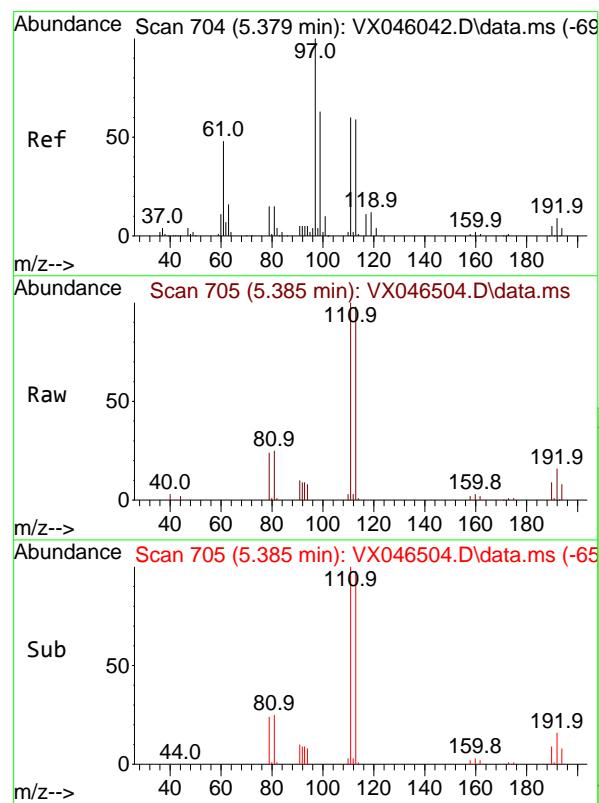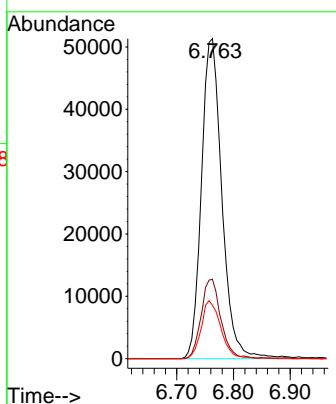





#35

Dibromofluoromethane  
Concen: 49.487 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.006 min  
Lab File: VX046504.D  
Acq: 04 Jun 2025 16:37

Tgt Ion:113 Resp: 45744

Ion	Ratio	Lower	Upper
113	100		
111	102.9	83.1	124.7
192	16.6	13.3	19.9

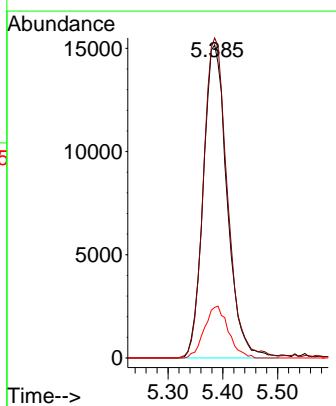



#37

**Ethyl Acetate**

Concen: 3.674 ug/l

RT: 4.733 min Scan# 5

Delta R.T. 0.018 min

Lab File: VX046504.D

Acq: 04 Jun 2025 16:37

Instrument:

MSVOA\_X

ClientSampleId :

EB01-060325





Tgt Ion: 43 Resp: 5638

Ion Ratio Lower Upper

43 100

61 0.0 10.3 15.5#

70 10.5 7.9 11.9



#50

**Toluene-d8**

Concen: 50.657 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX046504.D


Acq: 04 Jun 2025 16:37




Tgt Ion: 98 Resp: 162070

Ion Ratio Lower Upper

98 100

100 65.3 53.5 80.3



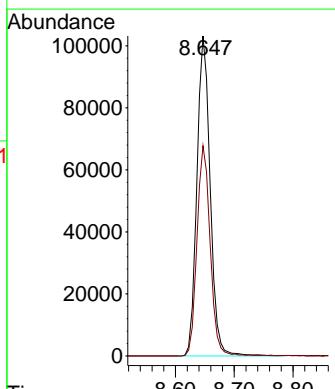




#62  
4-Bromofluorobenzene  
Concen: 52.673 ug/l  
RT: 11.079 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046504.D  
Acq: 04 Jun 2025 16:37



Instrument : MSVOA\_X  
ClientSampleId : EB01-060325


Tgt Ion: 95 Resp: 64642  
Ion Ratio Lower Upper  
95 100  
174 66.3 0.0 135.8  
176 63.9 0.0 131.4

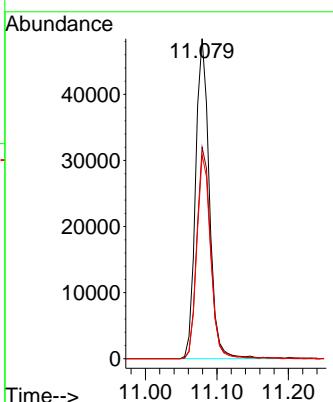

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.006 min  
Lab File: VX046504.D  
Acq: 04 Jun 2025 16:37

Tgt Ion:117 Resp: 122354  
Ion Ratio Lower Upper  
117 100  
82 60.2 50.6 76.0  
119 33.5 25.8 38.6




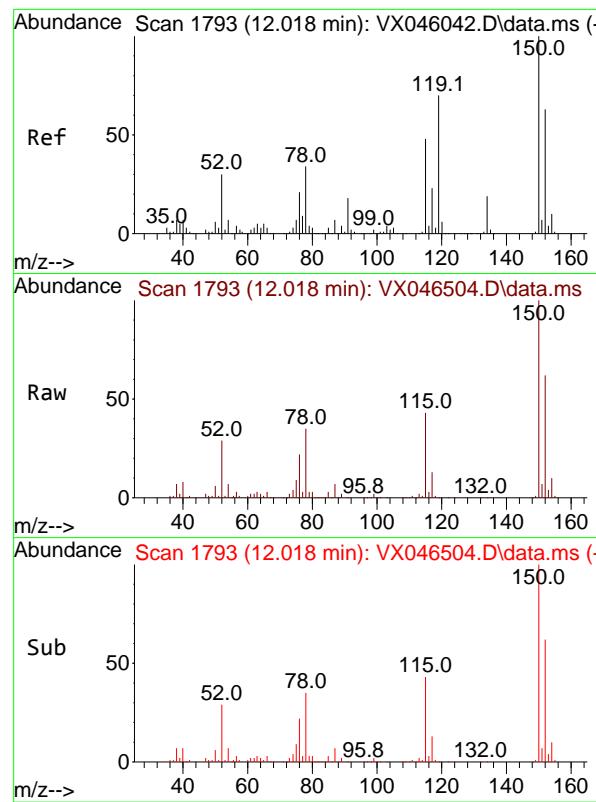

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046504.D  
Acq: 04 Jun 2025 16:37

Instrument : MSVOA\_X  
ClientSampleId : EB01-060325

Tgt Ion:152 Resp: 53968  
Ion Ratio Lower Upper  
152 100  
115 65.5 46.9 140.7  
150 156.7 0.0 351.0

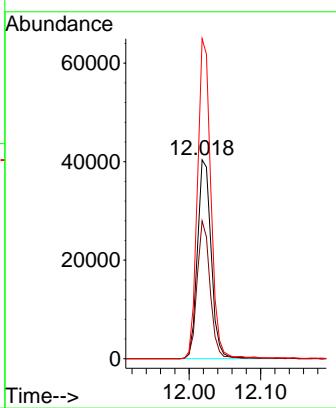



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	06/03/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	06/03/25	
Client Sample ID:	MW-11B-37.5-060325			SDG No.:	Q2200	
Lab Sample ID:	Q2200-05			Matrix:	Water	
Analytical Method:	8260D			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046500.D	50		06/04/25 15:02	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	13.0	U	13.0	50.0	ug/L
75-35-4	1,1-Dichloroethene	86.9		11.5	50.0	ug/L
75-34-3	1,1-Dichloroethane	11.5	U	11.5	50.0	ug/L
156-59-2	cis-1,2-Dichloroethene	1200		9.50	50.0	ug/L
71-55-6	1,1,1-Trichloroethane	10.0	U	10.0	50.0	ug/L
71-43-2	Benzene	7.50	U	7.50	50.0	ug/L
107-06-2	1,2-Dichloroethane	11.0	U	11.0	50.0	ug/L
79-01-6	Trichloroethene	11300	E	4.70	50.0	ug/L
79-00-5	1,1,2-Trichloroethane	10.5	U	10.5	50.0	ug/L
127-18-4	Tetrachloroethene	11.5	U	11.5	50.0	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	52.1		70 (74) - 130 (125)	104%	SPK: 50
1868-53-7	Dibromofluoromethane	49.8		70 (75) - 130 (124)	100%	SPK: 50
2037-26-5	Toluene-d8	49.8		70 (86) - 130 (113)	100%	SPK: 50
460-00-4	4-Bromofluorobenzene	50.6		70 (77) - 130 (121)	101%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	61200	5.55			
540-36-3	1,4-Difluorobenzene	122000	6.763			
3114-55-4	Chlorobenzene-d5	113000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	47100	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046500.D  
 Acq On : 04 Jun 2025 15:02  
 Operator : JC/MD  
 Sample : Q2200-05 50X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 14 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**MW-11B-37.5-060325**

Quant Time: Jun 05 01:56:36 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	61191	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	121976	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	112952	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	47128	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	59444	52.107	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	104.220%	
35) Dibromofluoromethane	5.385	113	43765	49.826	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	99.660%	
50) Toluene-d8	8.647	98	151455	49.819	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	99.640%	
62) 4-Bromofluorobenzene	11.079	95	59009	50.602	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	101.200%	
<b>Target Compounds</b>						
				Qvalue		
12) 1,1-Dichloroethene	2.313	96	1260	1.737 ug/l	#	95
27) cis-1,2-Dichloroethene	4.489	96	20620	23.474 ug/l		89
44) Trichloroethene	7.123	130	188738	226.852 ug/l		96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046500.D  
 Acq On : 04 Jun 2025 15:02  
 Operator : JC/MD  
 Sample : Q2200-05 50X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-11B-37.5-060325

Quant Time: Jun 05 01:56:36 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration



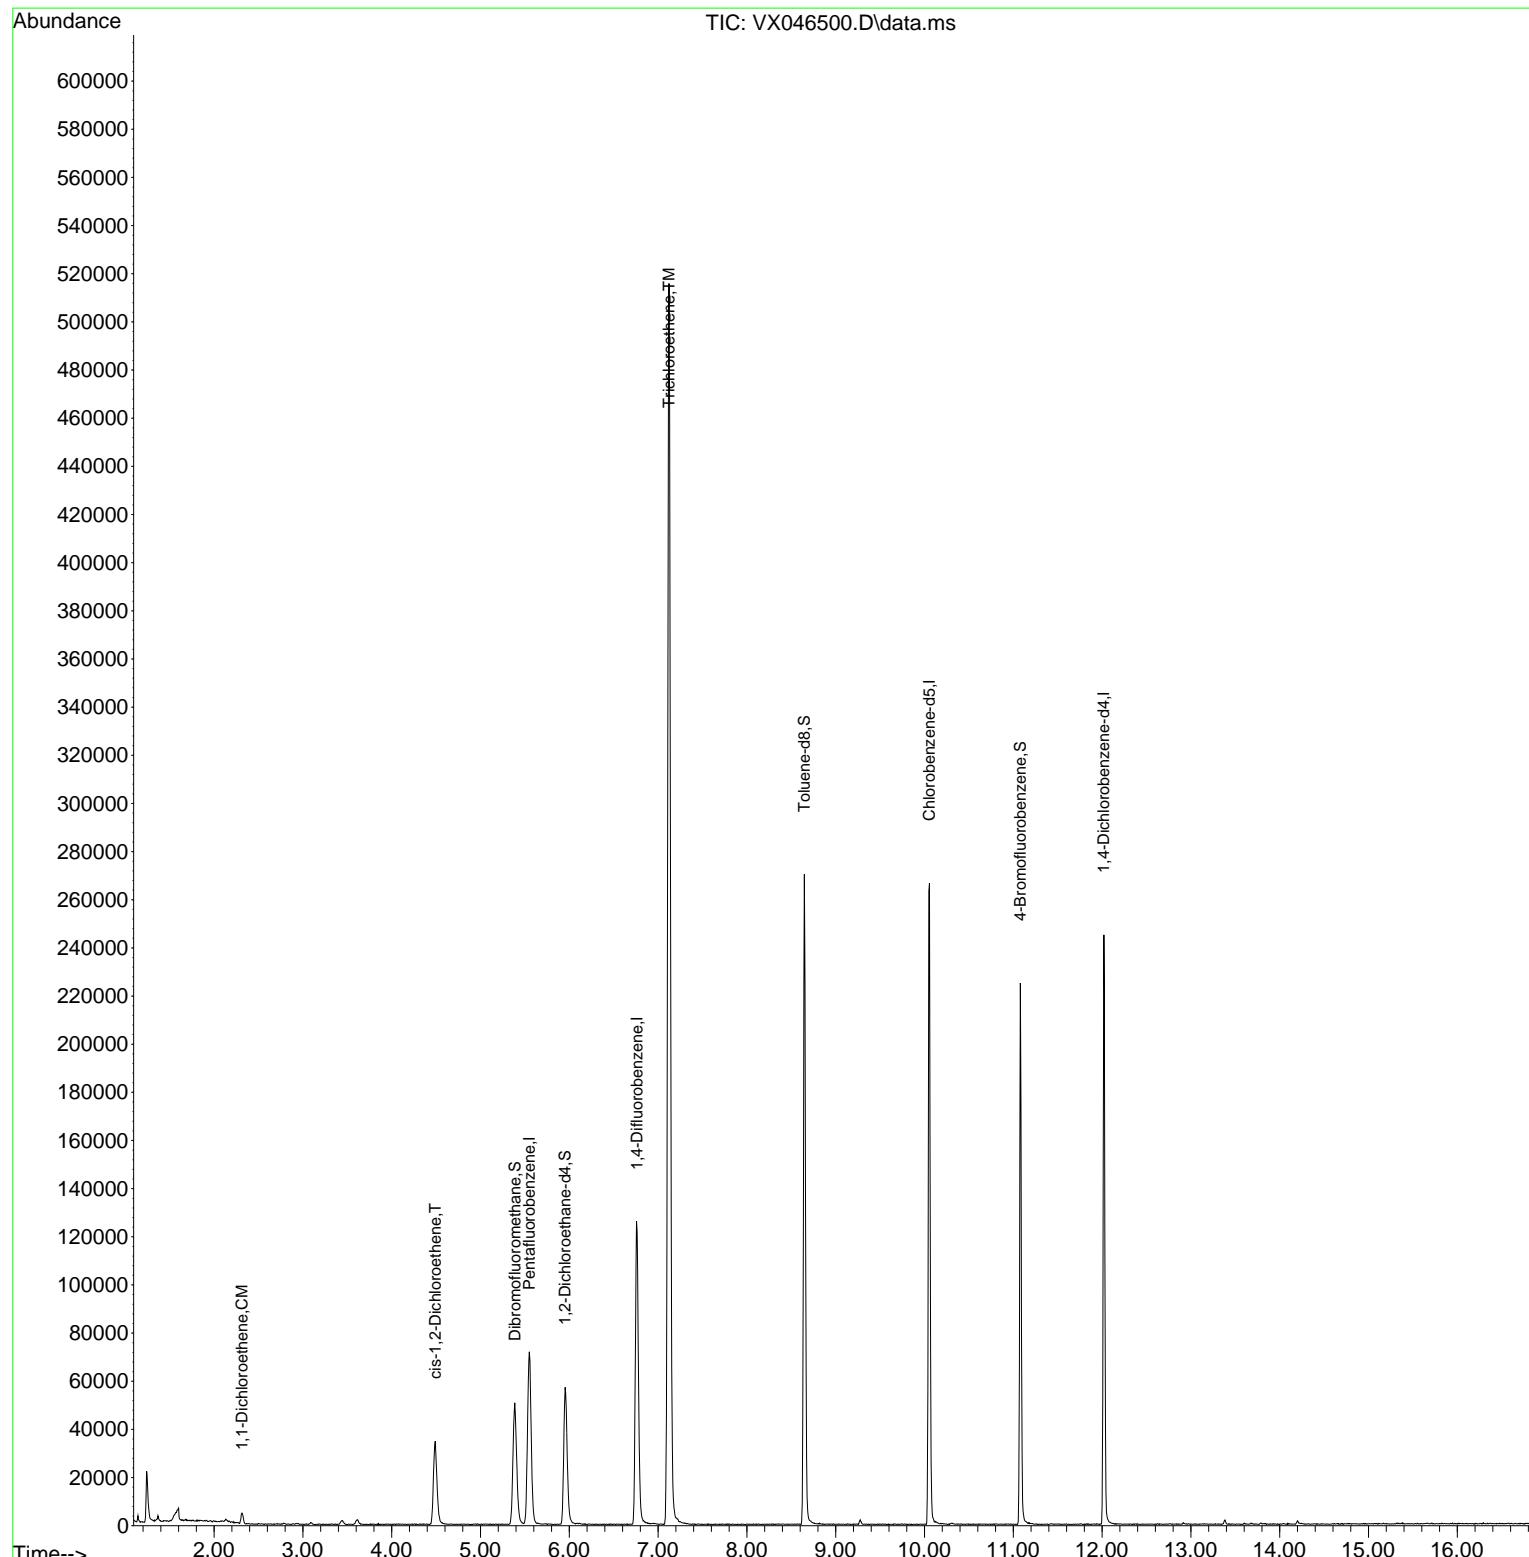




#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.550 min Scan# 7  
 Delta R.T. 0.006 min  
 Lab File: VX046500.D  
 Acq: 04 Jun 2025 15:02



Instrument : MSVOA\_X  
 ClientSampleId : MW-11B-37.5-060325




Tgt Ion:168 Resp: 61191  
 Ion Ratio Lower Upper  
 168 100  
 99 66.8 54.9 82.3

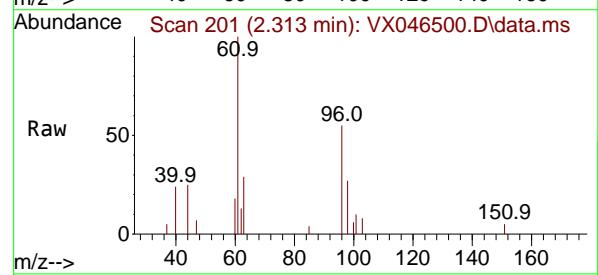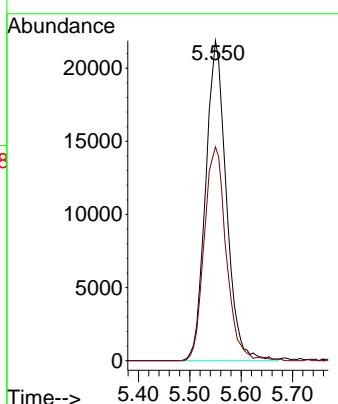

#12  
 1,1-Dichloroethene  
 Concen: 1.737 ug/l  
 RT: 2.313 min Scan# 201  
 Delta R.T. 0.000 min  
 Lab File: VX046500.D  
 Acq: 04 Jun 2025 15:02

Tgt Ion: 96 Resp: 1260  
 Ion Ratio Lower Upper  
 96 100  
 61 183.3 146.2 219.2  
 98 49.4 51.0 76.6#



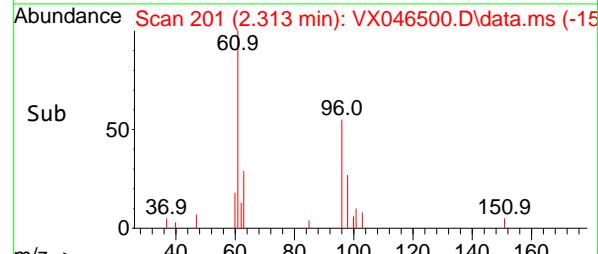
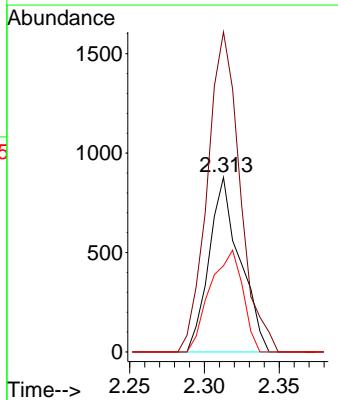




#27  
cis-1,2-Dichloroethene  
Concen: 23.474 ug/l  
RT: 4.489 min Scan# 5  
Delta R.T. 0.006 min  
Lab File: VX046500.D  
Acq: 04 Jun 2025 15:02


Instrument : MSVOA\_X  
ClientSampleId : MW-11B-37.5-060325


Tgt Ion: 96 Resp: 20620  
Ion Ratio Lower Upper  
96 100  
61 141.8 0.0 322.8  
98 64.3 0.0 129.0

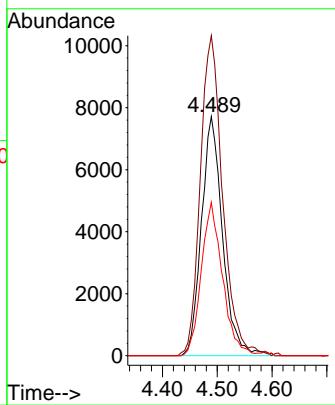

#33  
1,2-Dichloroethane-d4  
Concen: 52.107 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. 0.000 min  
Lab File: VX046500.D  
Acq: 04 Jun 2025 15:02

Tgt Ion: 65 Resp: 59444  
Ion Ratio Lower Upper  
65 100  
67 48.2 0.0 99.0

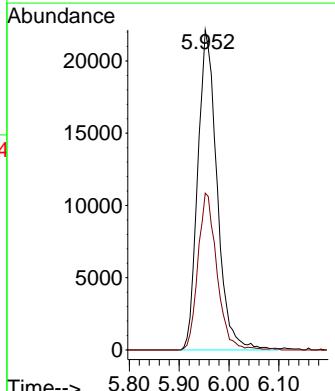

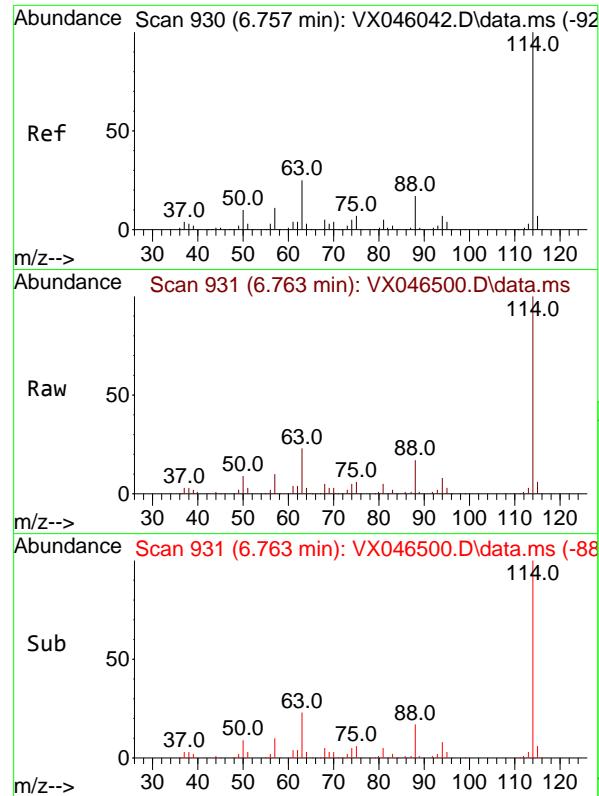

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 9

Delta R.T. 0.006 min

Lab File: VX046500.D

Acq: 04 Jun 2025 15:02

Instrument:

MSVOA\_X

ClientSampleId :

MW-11B-37.5-060325

Tgt Ion:114 Resp: 121976

Ion Ratio Lower Upper



114 100

63 23.3 0.0 49.2

88 17.3 0.0 33.6

Abundance

6.763

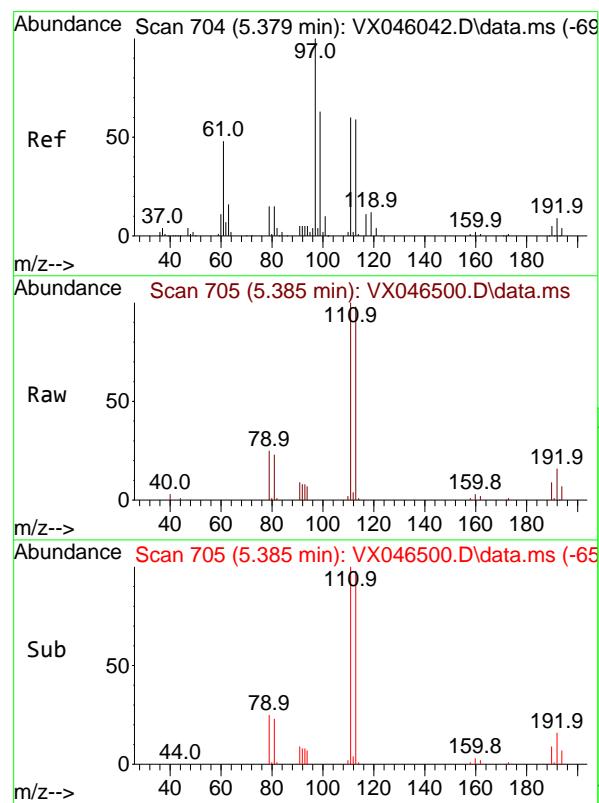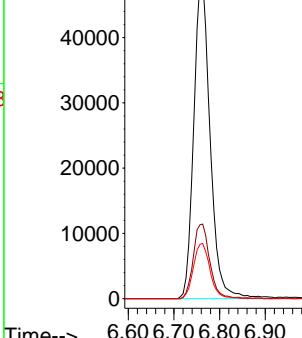

#35

Dibromofluoromethane

Concen: 49.826 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX046500.D

Acq: 04 Jun 2025 15:02

Tgt Ion:113 Resp: 43765

Ion Ratio Lower Upper


113 100


111 102.4 83.1 124.7

192 16.6 13.3 19.9

Abundance


5.385

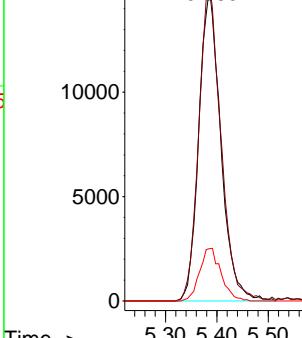






#44  
Trichloroethene  
Concen: 226.852 ug/l  
RT: 7.123 min Scan# 990  
Delta R.T. 0.000 min  
Lab File: VX046500.D  
Acq: 04 Jun 2025 15:02


Instrument : MSVOA\_X  
ClientSampleId : MW-11B-37.5-060325

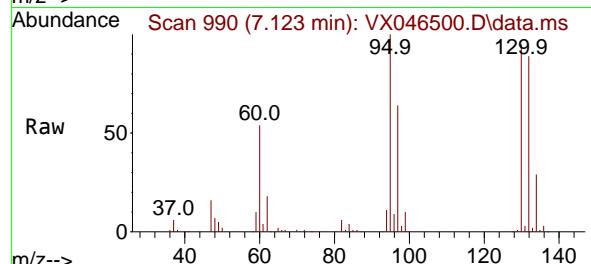



Tgt Ion:130 Resp: 188738  
Ion Ratio Lower Upper  
130 100  
95 105.8 0.0 204.2

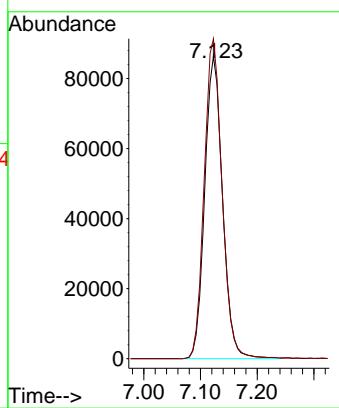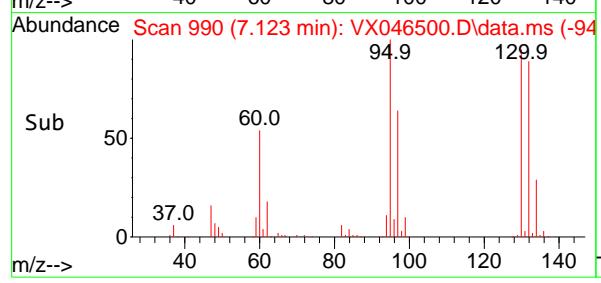


#50  
Toluene-d8  
Concen: 49.819 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. 0.000 min  
Lab File: VX046500.D  
Acq: 04 Jun 2025 15:02





Tgt Ion: 98 Resp: 151455  
Ion Ratio Lower Upper  
98 100  
100 66.5 53.5 80.3

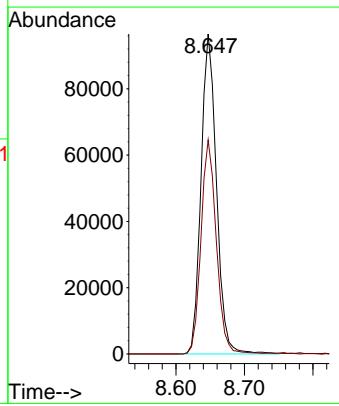

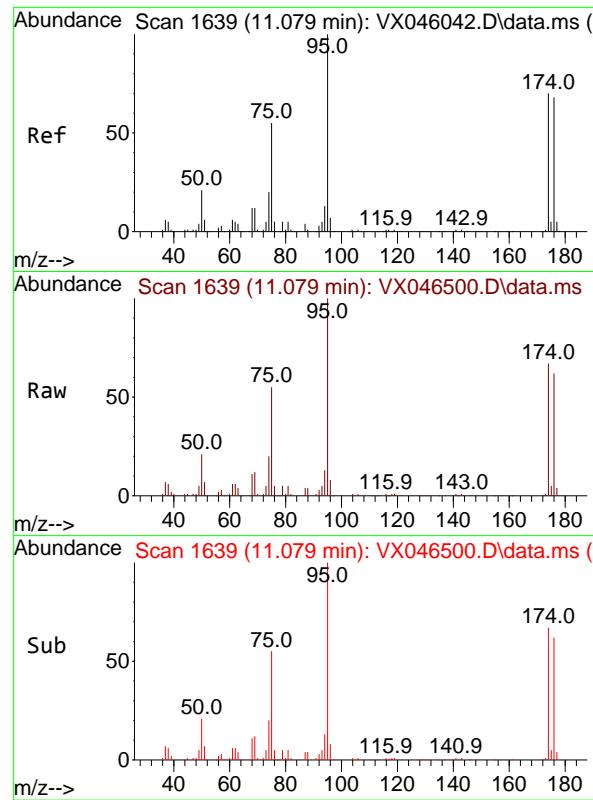


#62  
4-Bromofluorobenzene  
Concen: 50.602 ug/l  
RT: 11.079 min Scan# 1  
Instrument: MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX046500.D  
ClientSampleId :  
Acq: 04 Jun 2025 15:02 MW-11B-37.5-060325


Tgt Ion: 95 Resp: 59009  
Ion Ratio Lower Upper  
95 100  
174 65.9 0.0 135.8  
176 62.9 0.0 131.4

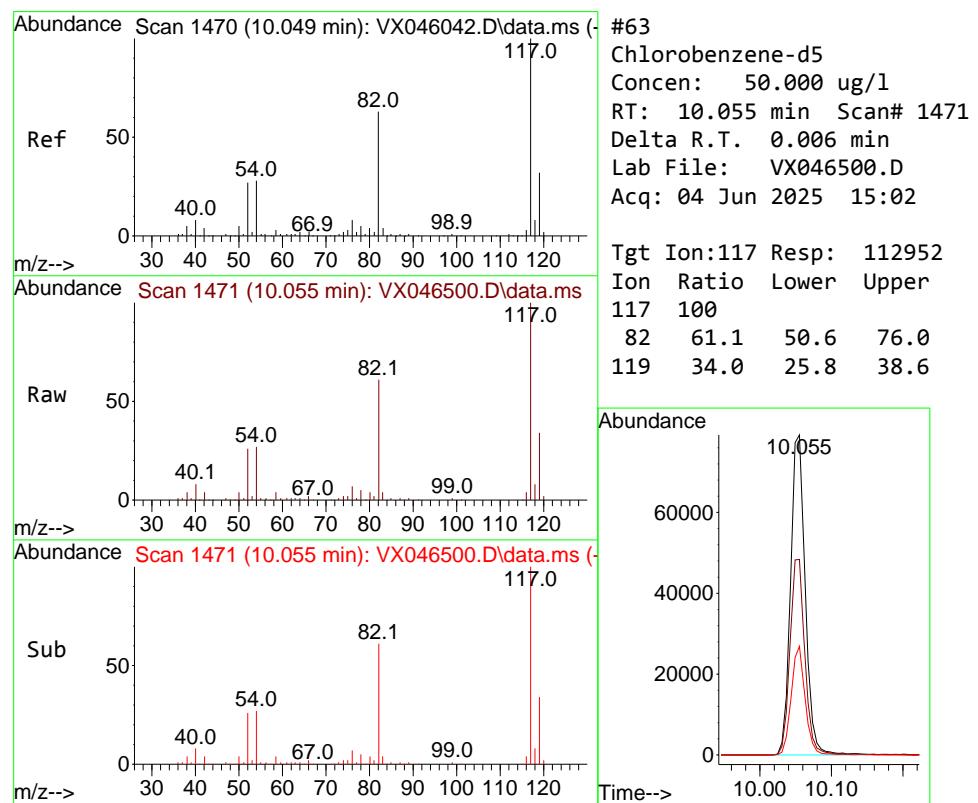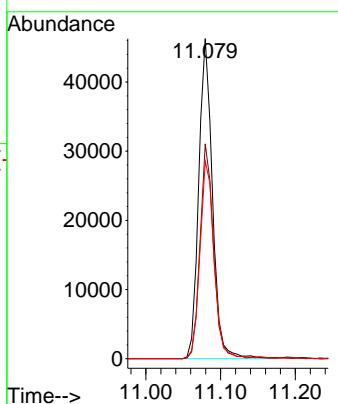

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.006 min  
Lab File: VX046500.D  
Acq: 04 Jun 2025 15:02

Tgt Ion:117 Resp: 112952  
Ion Ratio Lower Upper  
117 100  
82 61.1 50.6 76.0  
119 34.0 25.8 38.6

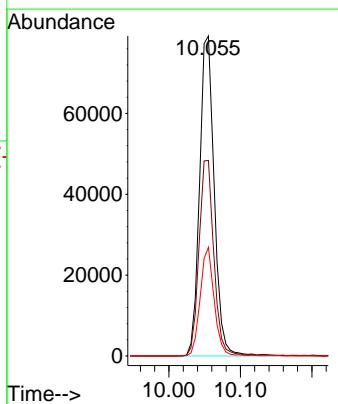


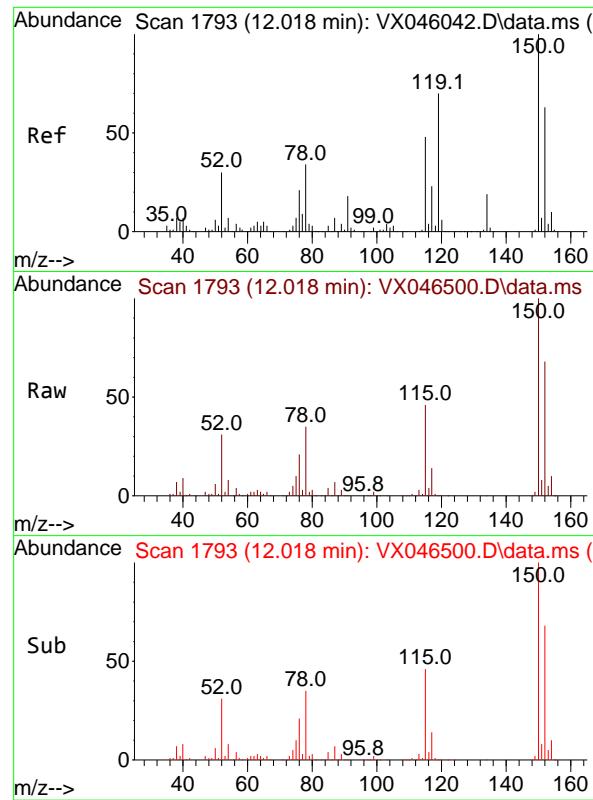

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046500.D  
Acq: 04 Jun 2025 15:02

Instrument : MSVOA\_X  
ClientSampleId : MW-11B-37.5-060325

Tgt Ion:152 Resp: 47128  
Ion Ratio Lower Upper  
152 100  
115 67.6 46.9 140.7  
150 153.4 0.0 351.0

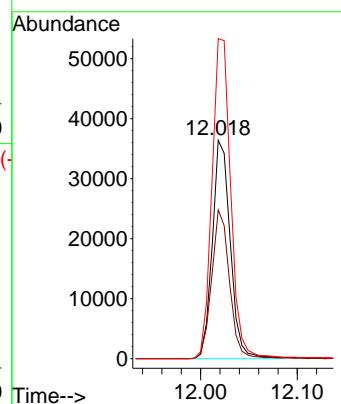



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	06/03/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	06/03/25	
Client Sample ID:	MW-11B-37.5-060325DL			SDG No.:	Q2200	
Lab Sample ID:	Q2200-05DL			Matrix:	Water	
Analytical Method:	8260D			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046509.D	200		06/04/25 18:36	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	52.0	UD	52.0	200	ug/L
75-35-4	1,1-Dichloroethene	46.0	UD	46.0	200	ug/L
75-34-3	1,1-Dichloroethane	46.0	UD	46.0	200	ug/L
156-59-2	cis-1,2-Dichloroethene	1200	D	38.0	200	ug/L
71-55-6	1,1,1-Trichloroethane	40.0	UD	40.0	200	ug/L
71-43-2	Benzene	30.0	UD	30.0	200	ug/L
107-06-2	1,2-Dichloroethane	44.0	UD	44.0	200	ug/L
79-01-6	Trichloroethene	11100	D	18.6	200	ug/L
79-00-5	1,1,2-Trichloroethane	42.0	UD	42.0	200	ug/L
127-18-4	Tetrachloroethene	46.0	UD	46.0	200	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	52.7		70 (74) - 130 (125)	105%	SPK: 50
1868-53-7	Dibromofluoromethane	49.9		70 (75) - 130 (124)	100%	SPK: 50
2037-26-5	Toluene-d8	49.6		70 (86) - 130 (113)	99%	SPK: 50
460-00-4	4-Bromofluorobenzene	50.3		70 (77) - 130 (121)	101%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	64000	5.55			
540-36-3	1,4-Difluorobenzene	127000	6.763			
3114-55-4	Chlorobenzene-d5	118000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	50600	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046509.D  
 Acq On : 04 Jun 2025 18:36  
 Operator : JC/MD  
 Sample : Q2200-05DL 200X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 23 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**MW-11B-37.5-060325DL**

Quant Time: Jun 05 04:54:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	63962	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	127435	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	117554	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	50632	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	62846	52.703	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	105.400%	
35) Dibromofluoromethane	5.391	113	45821	49.932	ug/l	0.01
Spiked Amount 50.000	Range 75 - 124		Recovery	=	99.860%	
50) Toluene-d8	8.647	98	157691	49.648	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	99.300%	
62) 4-Bromofluorobenzene	11.079	95	61278	50.297	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	100.600%	
<b>Target Compounds</b>						
				Qvalue		
27) cis-1,2-Dichloroethene	4.495	96	5624	6.125	ug/l	90
44) Trichloroethene	7.123	130	48234	55.491	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046509.D  
 Acq On : 04 Jun 2025 18:36  
 Operator : JC/MD  
 Sample : Q2200-05DL 200X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 MW-11B-37.5-060325DL



Quant Time: Jun 05 04:54:00 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

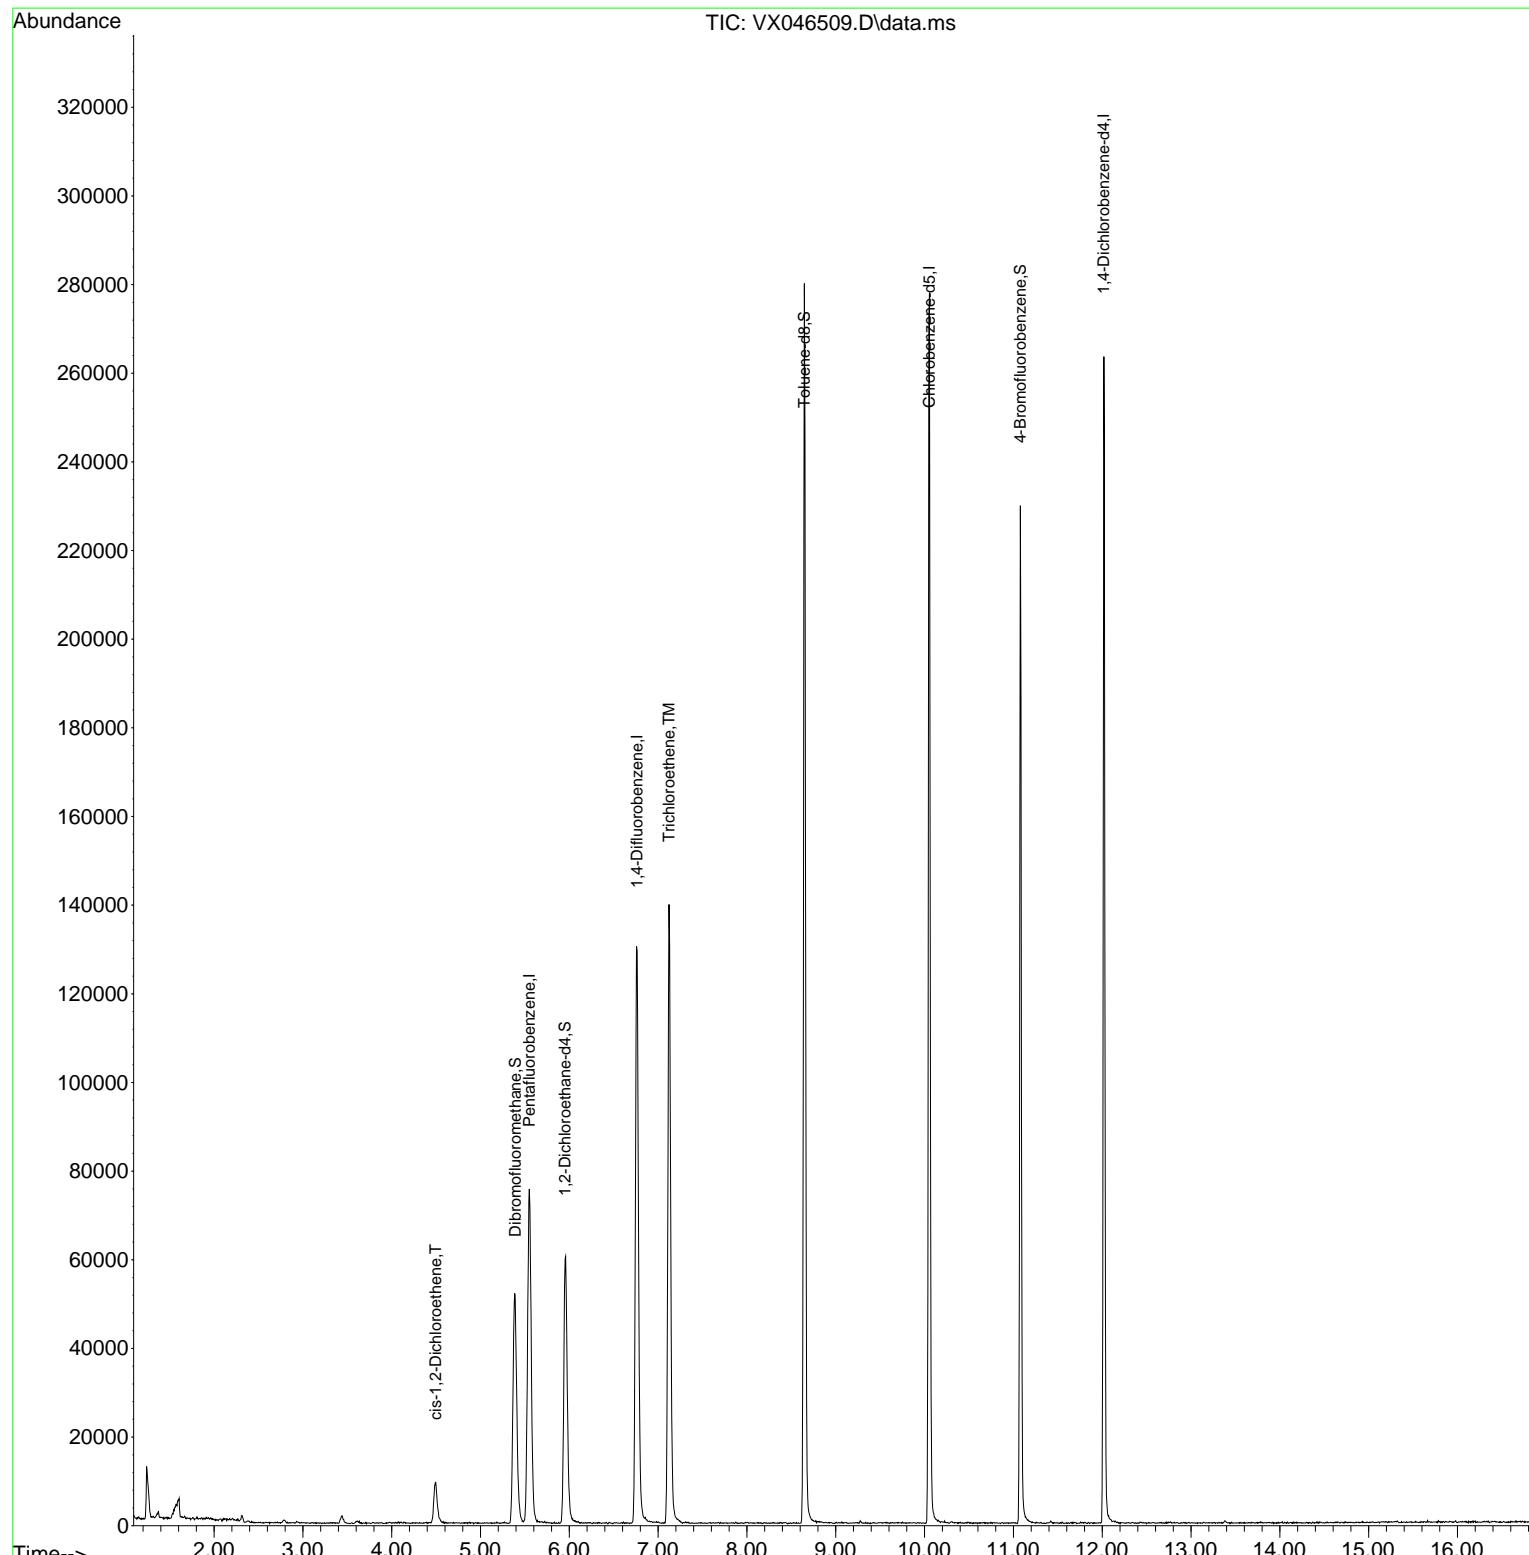

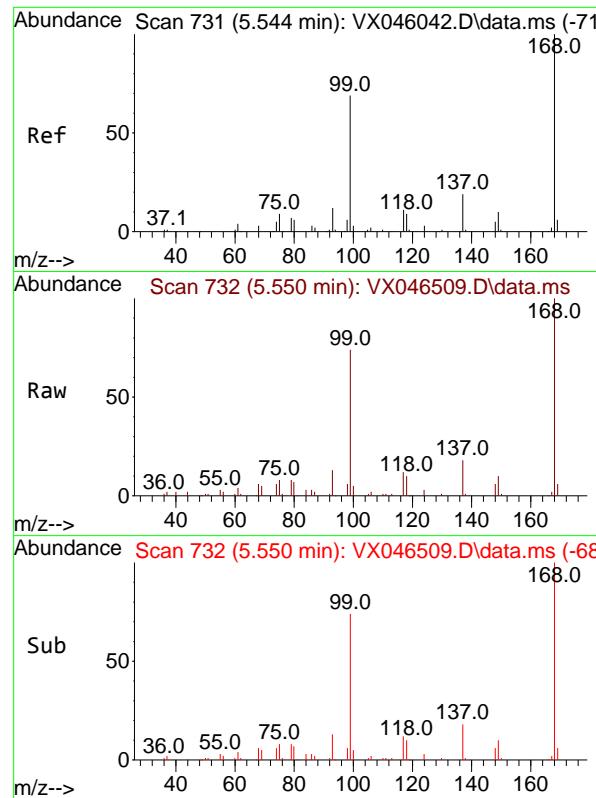


#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX046509.D  
Acq: 04 Jun 2025 18:36  
ClientSampleId : MW-11B-37.5-060325DL







Tgt Ion:168 Resp: 63962  
Ion Ratio Lower Upper  
168 100  
99 73.8 54.9 82.3

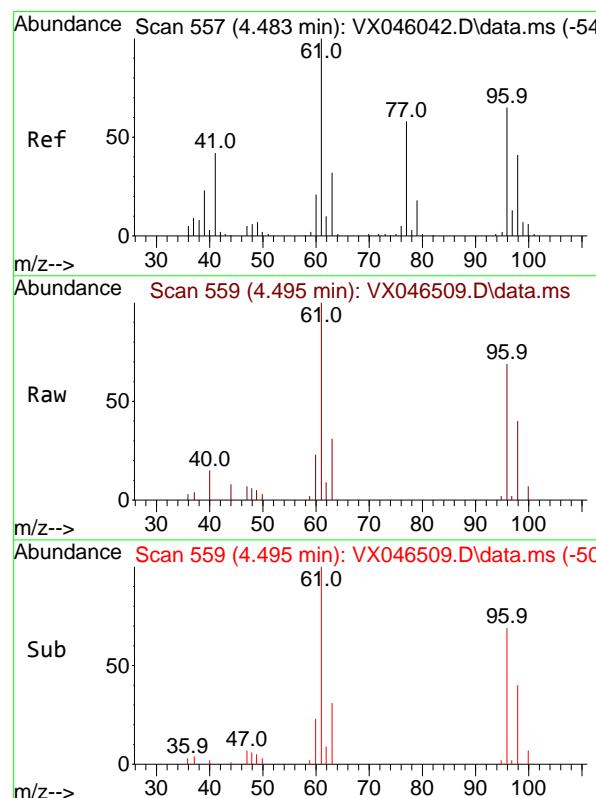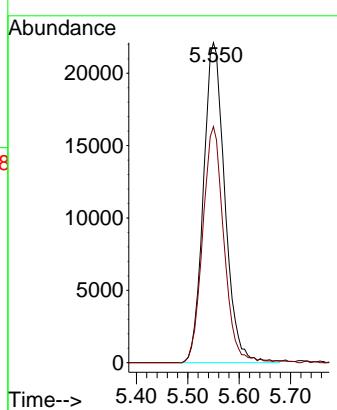

#27  
cis-1,2-Dichloroethene  
Concen: 6.125 ug/l  
RT: 4.495 min Scan# 559  
Delta R.T. 0.012 min  
Lab File: VX046509.D  
Acq: 04 Jun 2025 18:36

Tgt Ion: 96 Resp: 5624  
Ion Ratio Lower Upper  
96 100  
61 143.6 0.0 322.8  
98 62.4 0.0 129.0

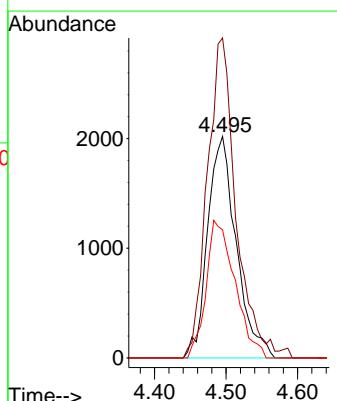

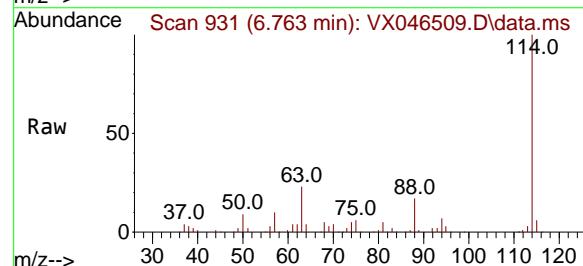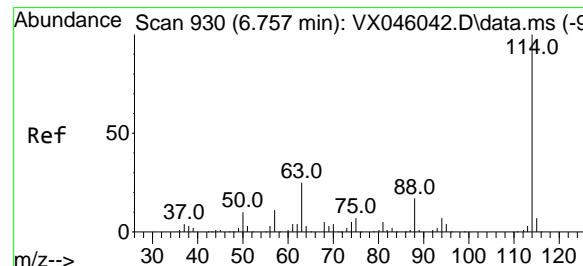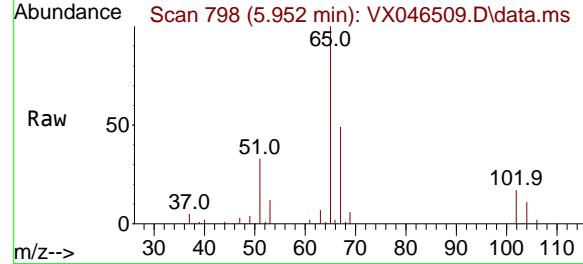

#33

1,2-Dichloroethane-d4

Concen: 52.703 ug/l

RT: 5.952 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046509.D

Acq: 04 Jun 2025 18:36

Instrument:

MSVOA\_X

ClientSampleId :

MW-11B-37.5-060325DL

Tgt Ion: 65 Resp: 62846


Ion Ratio Lower Upper

65 100

67 49.4 0.0 99.0

Abundance

5.952

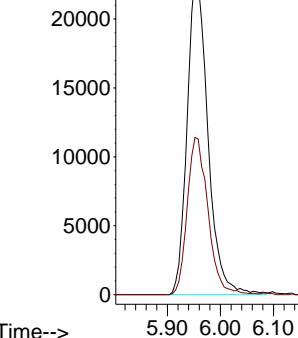

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX046509.D

Acq: 04 Jun 2025 18:36

Tgt Ion:114 Resp: 127435

Ion Ratio Lower Upper


114 100


63 23.0 0.0 49.2

88 17.3 0.0 33.6

Abundance

6.763

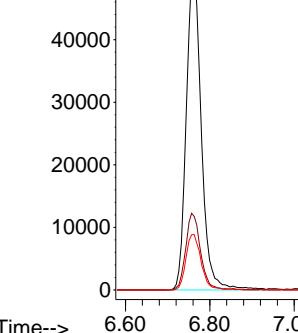

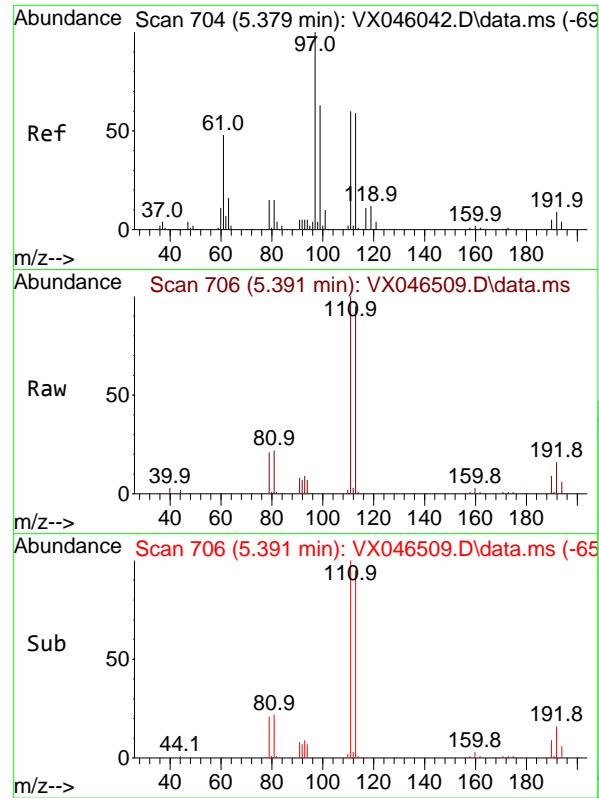

#35

Dibromofluoromethane

Concen: 49.932 ug/l

RT: 5.391 min Scan# 7

Delta R.T. 0.012 min

Lab File: VX046509.D


Acq: 04 Jun 2025 18:36

Instrument:

MSVOA\_X

ClientSampleId :

MW-11B-37.5-060325DL

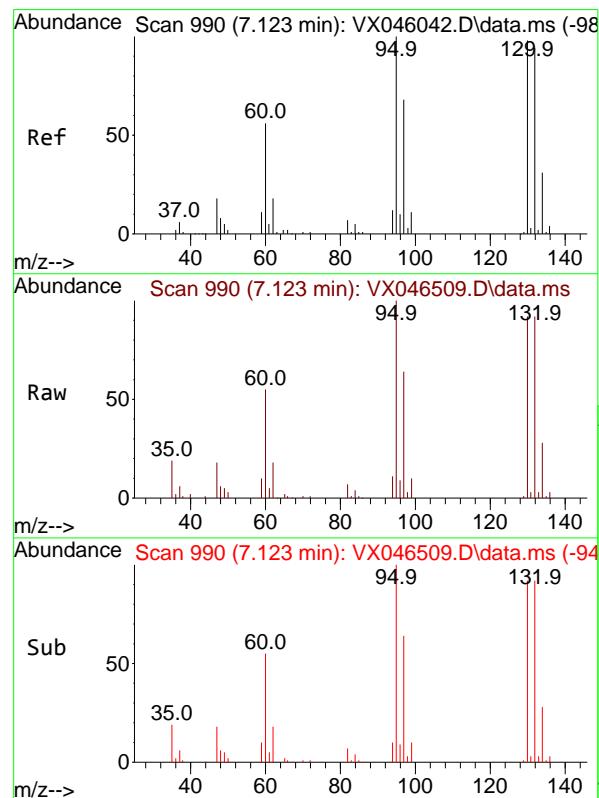

#44

Trichloroethene

Concen: 55.491 ug/l

RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX046509.D


Acq: 04 Jun 2025 18:36

Tgt Ion:130 Resp: 48234

Ion Ratio Lower Upper

130 100

95 108.2 0.0 204.2

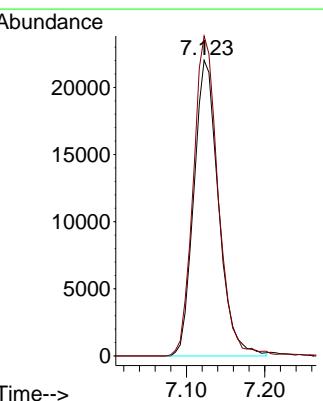

Time--&gt;


Tgt Ion:113 Resp: 45821


Ion Ratio Lower Upper

113 100

111 103.8 83.1 124.7

192 16.8 13.3 19.9


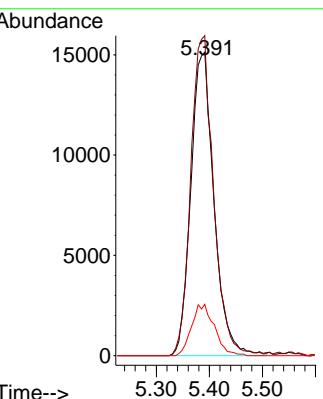


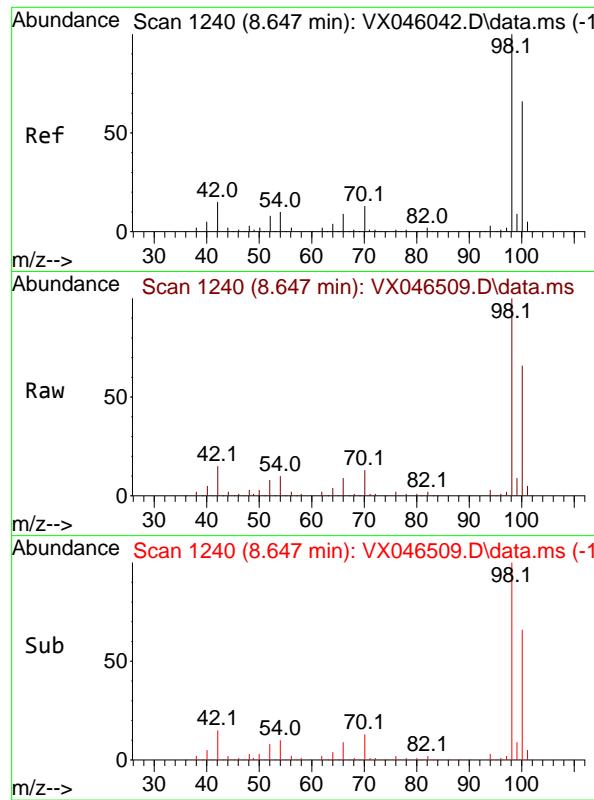

#50  
Toluene-d8  
Concen: 49.648 ug/l  
RT: 8.647 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046509.D  
Acq: 04 Jun 2025 18:36


Instrument: MSVOA\_X  
ClientSampleId: MW-11B-37.5-060325DL


Tgt Ion: 98 Resp: 157691  
Ion Ratio Lower Upper  
98 100  
100 65.4 53.5 80.3

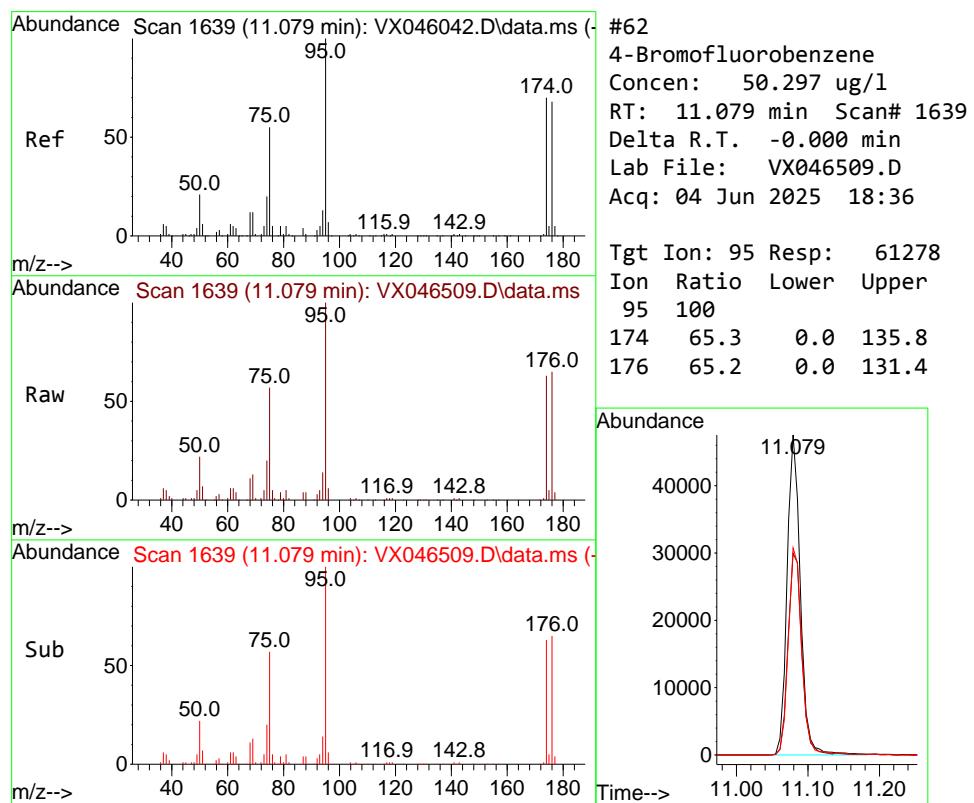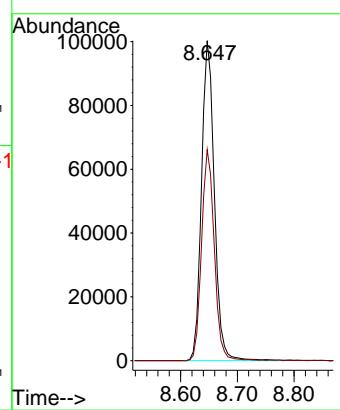

#62  
4-Bromofluorobenzene  
Concen: 50.297 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX046509.D  
Acq: 04 Jun 2025 18:36



Tgt Ion: 95 Resp: 61278  
Ion Ratio Lower Upper  
95 100  
174 65.3 0.0 135.8  
176 65.2 0.0 131.4

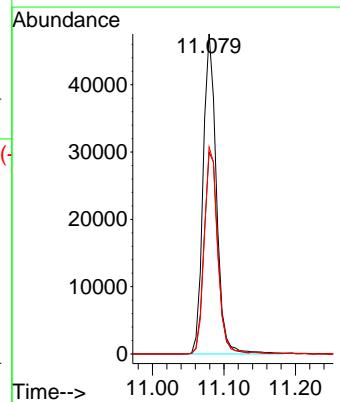

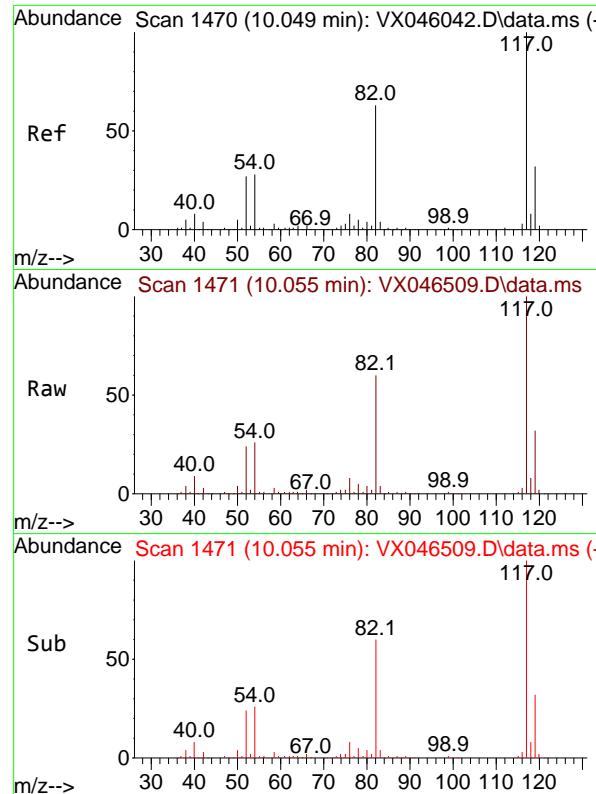


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX046509.D  
Acq: 04 Jun 2025 18:36  
ClientSampleId : MW-11B-37.5-060325DL

Tgt Ion:117 Resp: 117554  
Ion Ratio Lower Upper  
117 100  
82 59.9 50.6 76.0  
119 31.7 25.8 38.6

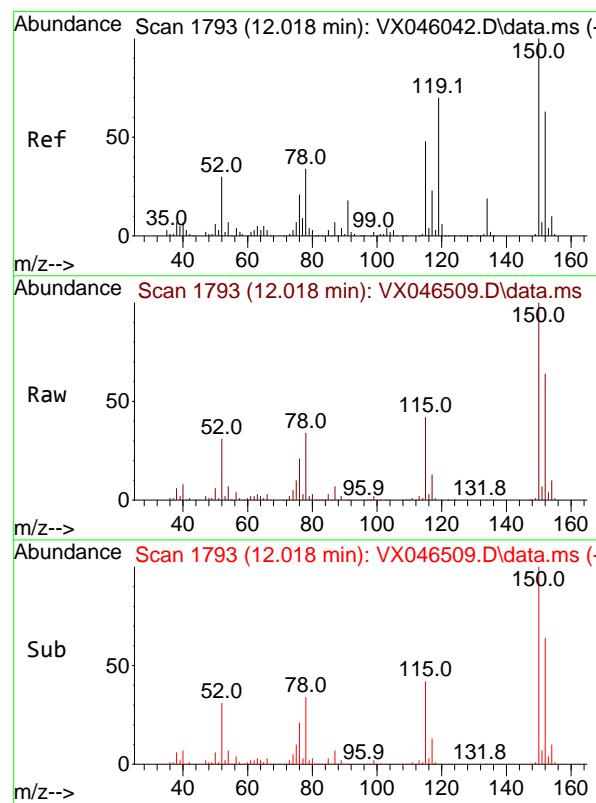

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. -0.000 min  
Lab File: VX046509.D  
Acq: 04 Jun 2025 18:36

Tgt Ion:152 Resp: 50632  
Ion Ratio Lower Upper  
152 100  
115 66.2 46.9 140.7  
150 156.5 0.0 351.0

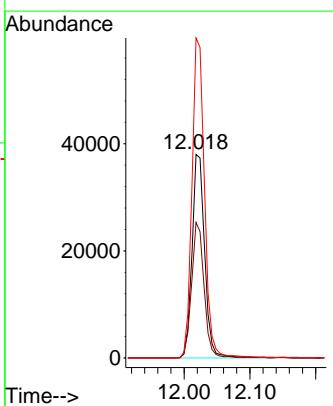



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	06/03/25	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	06/03/25	
Client Sample ID:	TB-01-060325			SDG No.:	Q2200	
Lab Sample ID:	Q2200-06			Matrix:	Water	
Analytical Method:	8260D			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group3	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046510.D	1		06/04/25 19:00	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	53.2		70 (74) - 130 (125)	106%	SPK: 50
1868-53-7	Dibromofluoromethane	50.0		70 (75) - 130 (124)	100%	SPK: 50
2037-26-5	Toluene-d8	49.7		70 (86) - 130 (113)	99%	SPK: 50
460-00-4	4-Bromofluorobenzene	50.7		70 (77) - 130 (121)	101%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	58800	5.543			
540-36-3	1,4-Difluorobenzene	118000	6.763			
3114-55-4	Chlorobenzene-d5	111000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	47900	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

( ) = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046510.D  
 Acq On : 04 Jun 2025 19:00  
 Operator : JC/MD  
 Sample : Q2200-06  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 24 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**TB-01-060325**

Quant Time: Jun 05 02:07:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.543	168	58762	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	118020	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	111037	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	47922	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	58326	53.241	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	106.480%		
35) Dibromofluoromethane	5.385	113	42480	49.984	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.960%		
50) Toluene-d8	8.646	98	146129	49.678	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	99.360%		
62) 4-Bromofluorobenzene	11.079	95	57197	50.692	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	101.380%		




Target Compounds	Qvalue
(#= qualifier out of range (m) = manual integration (+) = signals summed	

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046510.D  
 Acq On : 04 Jun 2025 19:00  
 Operator : JC/MD  
 Sample : Q2200-06  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 TB-01-060325




Quant Time: Jun 05 02:07:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

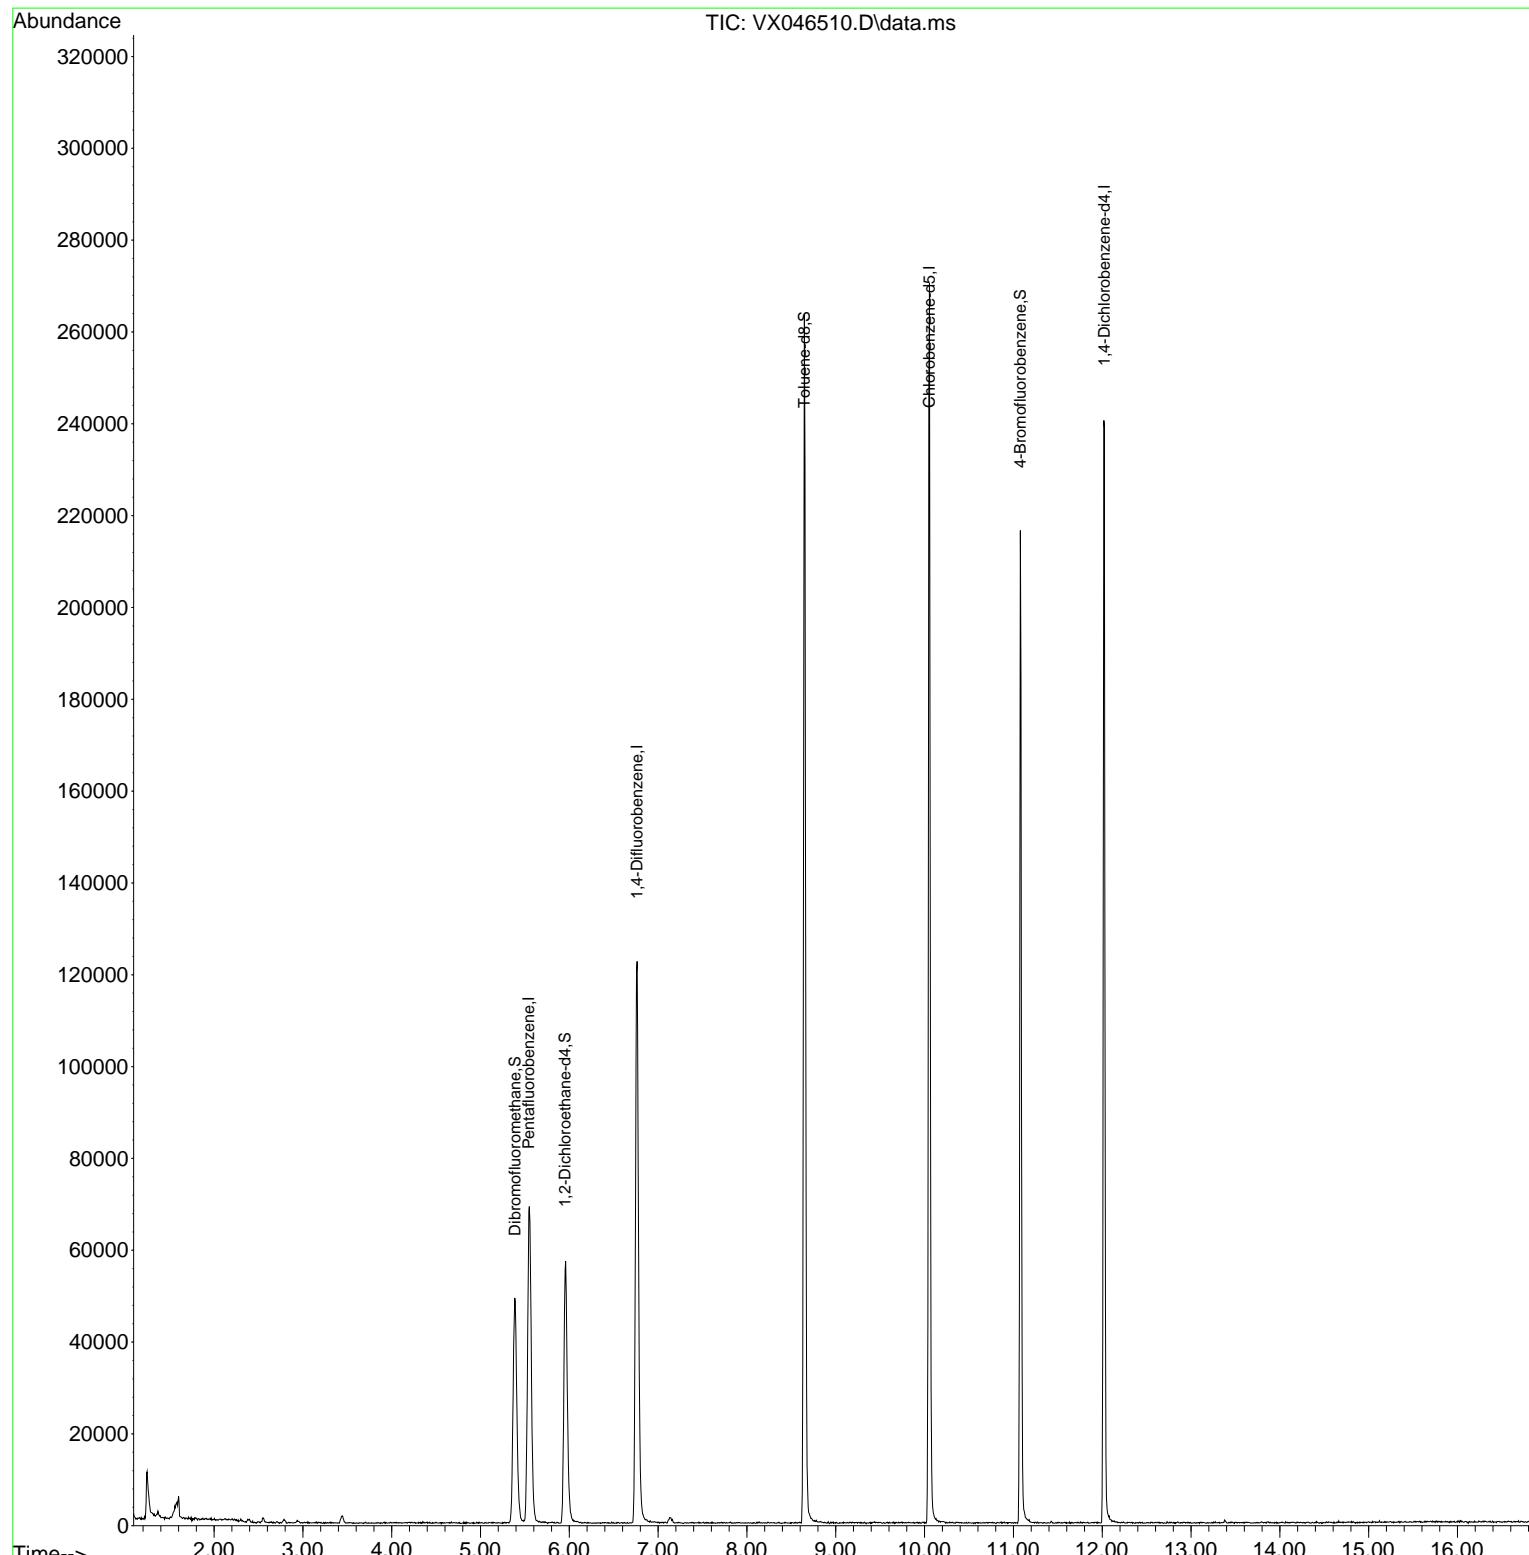





#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.543 min Scan# 7  
Instrument: MSVOA\_X  
Delta R.T. -0.001 min  
Lab File: VX046510.D  
ClientSampleId : TB-01-060325  
Acq: 04 Jun 2025 19:00




Tgt Ion:168 Resp: 58762  
Ion Ratio Lower Upper  
168 100  
99 71.4 54.9 82.3

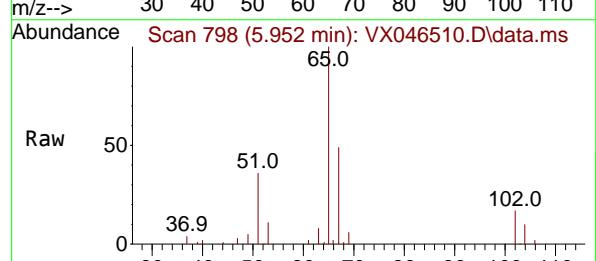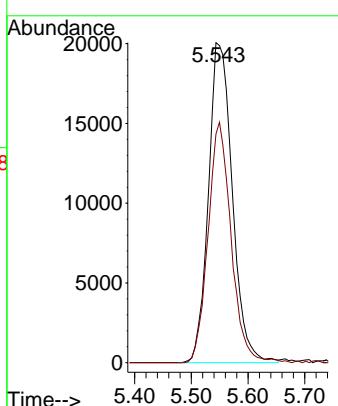

#33  
1,2-Dichloroethane-d4  
Concen: 53.241 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.000 min  
Lab File: VX046510.D  
Acq: 04 Jun 2025 19:00

Tgt Ion: 65 Resp: 58326  
Ion Ratio Lower Upper  
65 100  
67 49.8 0.0 99.0

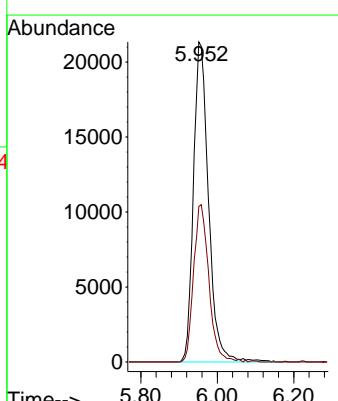

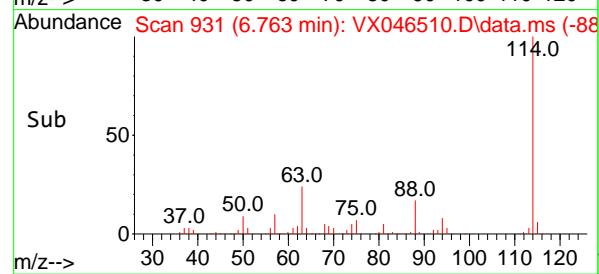

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 9

Delta R.T. 0.006 min

Lab File: VX046510.D

Acq: 04 Jun 2025 19:00

Instrument:

MSVOA\_X

ClientSampleId :

TB-01-060325

Tgt Ion:114 Resp: 118020

Ion Ratio Lower Upper





114 100

63 23.5

88 17.0

0.0 49.2

0.0 33.6

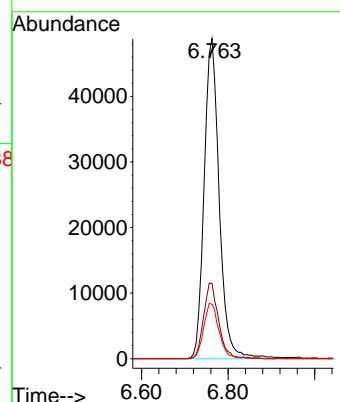

#35

Dibromofluoromethane

Concen: 49.984 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX046510.D

Acq: 04 Jun 2025 19:00

Tgt Ion:113 Resp: 42480

Ion Ratio Lower Upper


113 100


111 103.2

192 16.6

83.1 124.7


13.3 19.9

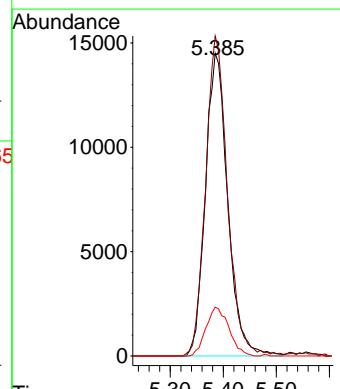






#50  
Toluene-d8  
Concen: 49.678 ug/l  
RT: 8.646 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046510.D  
Acq: 04 Jun 2025 19:00


Instrument: MSVOA\_X  
ClientSampleId : TB-01-060325





Tgt Ion: 98 Resp: 146129  
Ion Ratio Lower Upper  
98 100  
100 65.5 53.5 80.3

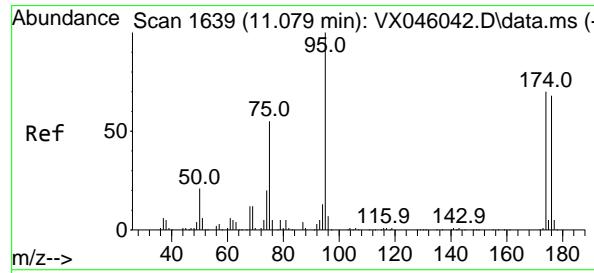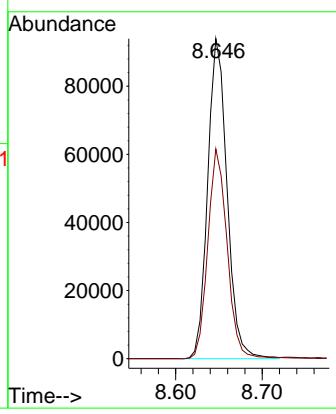


#62  
4-Bromofluorobenzene  
Concen: 50.692 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX046510.D  
Acq: 04 Jun 2025 19:00

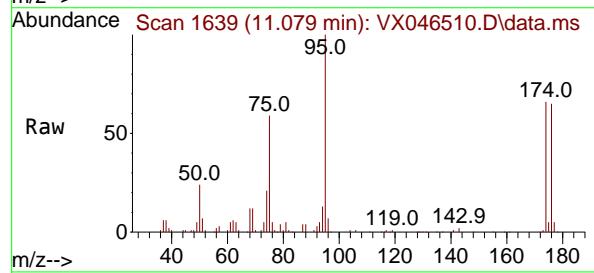



Tgt Ion: 95 Resp: 57197  
Ion Ratio Lower Upper  
95 100  
174 67.4 0.0 135.8  
176 64.9 0.0 131.4

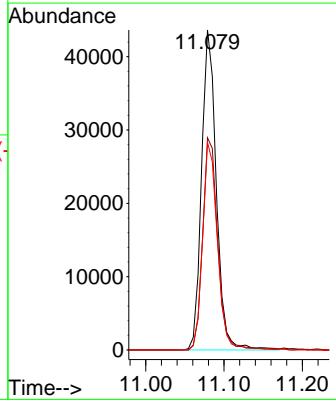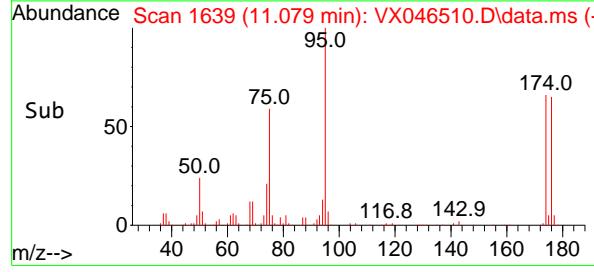

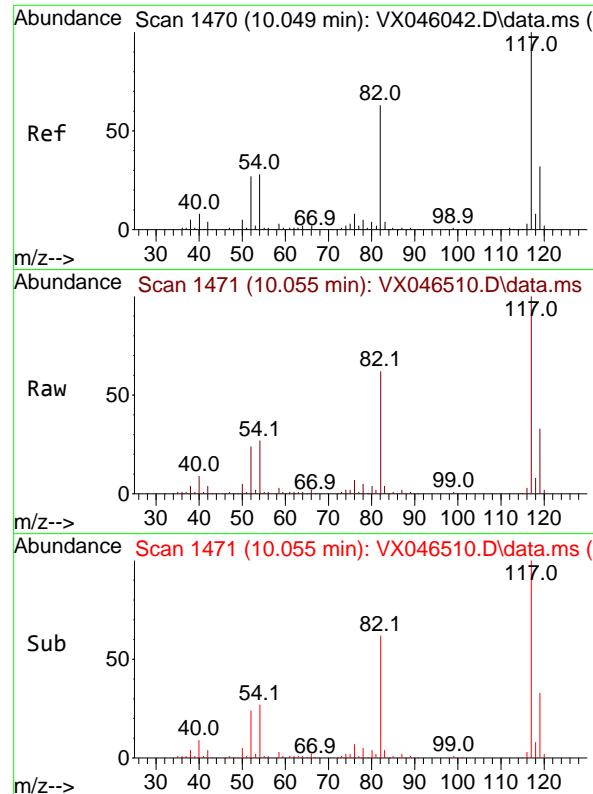


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX046510.D  
Acq: 04 Jun 2025 19:00  
ClientSampleId : TB-01-060325

Tgt Ion:117 Resp: 111037  
Ion Ratio Lower Upper  
117 100  
82 61.6 50.6 76.0  
119 33.1 25.8 38.6

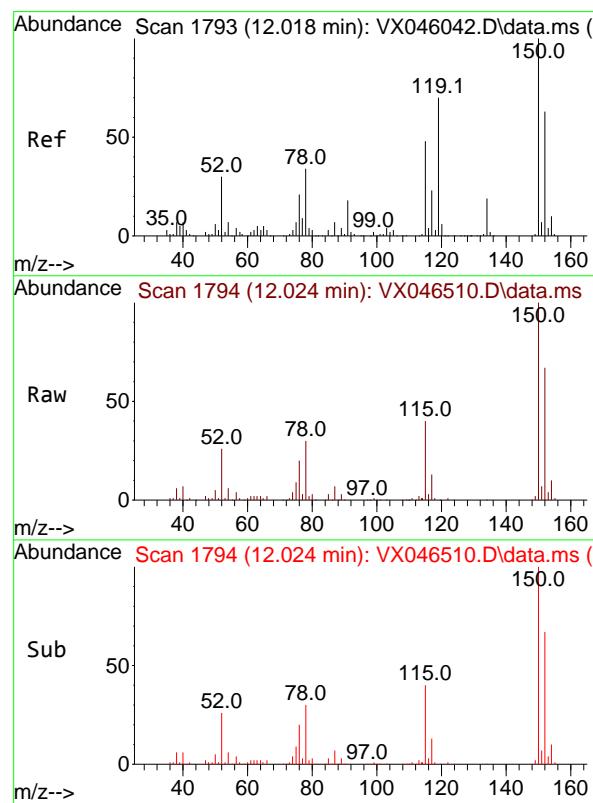

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.006 min  
Lab File: VX046510.D  
Acq: 04 Jun 2025 19:00

Tgt Ion:152 Resp: 47922  
Ion Ratio Lower Upper  
152 100  
115 65.1 46.9 140.7  
150 154.2 0.0 351.0

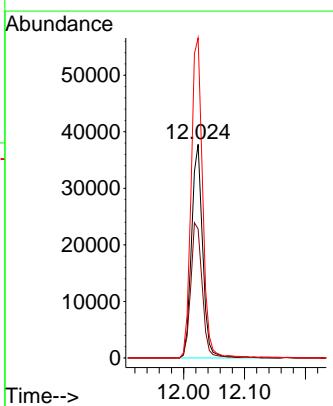



# CALIBRATION

# SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

### VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name:	<u>CHEMTECH</u>		Contract:	<u>JAC005</u>				
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q2200</u>		SAS No.:	<u>Q2200</u>	SDG No.:	<u>Q2200</u>
Instrument ID:	<u>MSVOA_X</u>		Calibration Date(s):	<u>05/05/2025</u>		Calibration Time(s):	<u>11:35</u>	<u>16:27</u>
Heated Purge:	(Y/N)	<u>N</u>						
GC Column:	<u>DB-624UI</u>	ID:	<u>0.18</u>	(mm)				

LAB FILE ID:	RRF020 = VX046041.D	RRF050 = VX046042.D	RRF100 = VX046043.D					
COMPOUND	RRF020	RRF050	RRF100	RRF150	RRF005	RRF001	RRF	% RSD
Vinyl Chloride	0.660	0.710	0.727	0.755	0.619	0.673	0.691	7.2
1,1-Dichloroethene	0.565	0.601	0.607	0.625	0.567	0.594	0.593	3.9
1,1-Dichloroethane	1.233	1.263	1.263	1.286	1.154	1.116	1.219	5.6
cis-1,2-Dichloroethene	0.716	0.737	0.738	0.755	0.642	0.719	0.718	5.5
1,1,1-Trichloroethane	1.106	1.131	1.155	1.188	1.013	1.015	1.101	6.6
Benzene	1.426	1.474	1.441	1.477	1.337	1.348	1.417	4.3
1,2-Dichloroethane	0.632	0.627	0.611	0.625	0.594	0.579	0.612	3.5
Trichloroethene	0.344	0.355	0.345	0.362	0.315	0.324	0.341	5.3
1,1,2-Trichloroethane	0.349	0.354	0.351	0.356	0.337	0.308	0.343	5.3
Tetrachloroethene	0.390	0.375	0.345	0.344	0.323	0.347	0.354	6.8
1,2-Dichloroethane-d4	0.953	0.910	0.930	0.932	0.935		0.932	1.6
Dibromofluoromethane	0.359	0.355	0.364	0.368	0.354		0.360	1.7
Toluene-d8	1.246	1.223	1.266	1.275	1.221		1.246	2
4-Bromofluorobenzene	0.455	0.470	0.500	0.500	0.464		0.478	4.4

- \* Compounds with required minimum RRF and maximum %RSD values.
- All other compounds must meet a minimum RRF of 0.010.
- RRF of 1,4-Dioxane = Value should be divide by 1000.

Method Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\

Method File : 82X050525W.M

Title : SW846 8260

Last Update : Tue May 06 07:12:22 2025

Response Via : Initial Calibration

## Calibration Files

1 =VX046047.D 5 =VX046046.D 20 =VX046041.D 50 =VX046042.D 100 =VX046043.D 150 =VX046044.D

Compound	1	5	20	50	100	150	Avg	%RSD
----------	---	---	----	----	-----	-----	-----	------

1) I	Pentafluorobenzene	-----	ISTD-----					
2) T	Dichlorodifluo...	0.658	0.639	0.697	0.864	0.859	0.875	0.765
3) P	Chloromethane	0.694	0.679	0.727	0.775	0.787	0.791	0.742
4) C	Vinyl Chloride	0.673	0.619	0.660	0.710	0.727	0.755	0.691
5) T	Bromomethane	0.305	0.296	0.326	0.340	0.334	0.320	0.320
6) T	Chloroethane	0.467	0.368	0.354	0.378	0.329	0.317	0.369
7) T	Trichlorofluor...	1.064	0.990	1.035	1.068	0.983	0.985	1.021
8) T	Diethyl Ether	0.403	0.311	0.340	0.337	0.338	0.355	0.347
9) T	1,1,2-Trichlor...	0.633	0.610	0.628	0.641	0.629	0.648	0.632
10) T	Methyl Iodide	0.608	0.767	0.806	0.793	0.763	0.747	10.68
11) T	Tert butyl alc...	0.114	0.122	0.129	0.144	0.146	0.131	10.45
12) CM	1,1-Dichloroet...	0.594	0.567	0.565	0.601	0.607	0.625	0.593
13) T	Acrolein	0.117	0.158	0.152	0.154	0.163	0.149	12.33
14) T	Allyl chloride	1.052	1.058	1.127	1.179	1.187	1.196	1.133
15) T	Acrylonitrile	0.363	0.345	0.378	0.388	0.381	0.390	0.374
16) T	Acetone	0.380	0.408	0.361	0.362	0.361	0.370	0.374
17) T	Carbon Disulfide	1.423	1.141	1.295	1.455	1.522	1.597	1.406
18) T	Methyl Acetate	1.006	0.816	0.814	0.848	0.845	0.875	0.867
19) T	Methyl tert-bu...	1.949	1.908	2.044	2.160	2.172	2.239	2.079
20) T	Methylene Chlo...	0.853	0.689	0.689	0.684	0.691	0.691	0.716
21) T	trans-1,2-Dich...	0.604	0.557	0.573	0.610	0.612	0.622	0.596
22) T	Diisopropyl ether	2.095	1.924	2.219	2.278	2.295	2.321	2.189
23) T	Vinyl Acetate	1.660	1.698	1.928	2.048	2.082	2.134	1.925
24) P	1,1-Dichloroet...	1.116	1.154	1.233	1.263	1.263	1.286	1.219
25) T	2-Butanone	0.495	0.539	0.540	0.555	0.558	0.569	0.543
26) T	2,2-Dichloropr...	0.965	0.850	0.910	0.957	1.003	1.039	0.954
27) T	cis-1,2-Dichlo...	0.719	0.642	0.716	0.737	0.738	0.755	0.718
28) T	Bromochloromet...	0.576	0.553	0.628	0.578	0.595	0.590	0.587
29) T	Tetrahydrofuran	0.318	0.318	0.340	0.350	0.351	0.362	0.340
30) C	Chloroform	1.265	1.199	1.287	1.296	1.277	1.300	1.271
31) T	Cyclohexane	1.059	1.090	1.128	1.128	1.150	1.111	3.26
32) T	1,1,1-Trichlor...	1.015	1.013	1.106	1.131	1.155	1.188	1.101
33) S	1,2-Dichloroet...	0.935	0.953	0.910	0.930	0.932	0.932	1.65
34) I	1,4-Difluorobenzene	-----	ISTD-----					
35) S	Dibromofluorom...	0.354	0.359	0.355	0.364	0.368	0.360	1.70
36) T	1,1-Dichloropr...	0.493	0.462	0.463	0.495	0.483	0.505	0.484
37) T	Ethyl Acetate	0.586	0.582	0.569	0.611	0.609	0.631	0.598
38) T	Carbon Tetrach...	0.541	0.505	0.528	0.558	0.552	0.577	0.544
39) T	Methylcyclohexane	0.627	0.587	0.596	0.641	0.627	0.658	0.623
40) TM	Benzene	1.348	1.337	1.426	1.474	1.441	1.477	1.417
41) T	Methacrylonitrile	0.233	0.288	0.318	0.346	0.343	0.348	0.313
42) TM	1,2-Dichloroet...	0.579	0.594	0.632	0.627	0.611	0.625	0.612
43) T	Isopropyl Acetate	0.764	0.826	0.905	0.963	0.982	1.030	0.912
44) TM	Trichloroethene	0.324	0.315	0.344	0.355	0.345	0.362	0.341
45) C	1,2-Dichloropr...	0.317	0.324	0.356	0.371	0.368	0.378	0.352
46) T	Dibromomethane	0.263	0.262	0.285	0.287	0.280	0.289	0.278
47) T	Bromodichlorom...	0.485	0.498	0.557	0.577	0.573	0.594	0.547
48) T	Methyl methacr...	0.370	0.426	0.465	0.502	0.500	0.531	0.466
49) T	1,4-Dioxane	0.007	0.009	0.009	0.009	0.009	0.010	0.009
50) S	Toluene-d8	1.221	1.246	1.223	1.266	1.275	1.246	1.95
51) T	4-Methyl-2-Pen...	0.561	0.555	0.620	0.634	0.630	0.631	0.605
52) CM	Toluene	0.803	0.838	0.884	0.898	0.885	0.904	0.869
53) T	t-1,3-Dichloro...	0.371	0.406	0.468	0.528	0.555	0.591	0.487
54) T	cis-1,3-Dichlo...	0.423	0.469	0.531	0.578	0.602	0.623	0.538
55) T	1,1,2-Trichlor...	0.308	0.337	0.349	0.354	0.351	0.356	0.343
56) T	Ethyl methacry...	0.377	0.508	0.540	0.595	0.617	0.639	0.546

Method Path :	Z:\voasrv\HPCHEM1\MSVOA_X\Method\
Method File :	82X050525W.M
57) T	1,3-Dichloropr... 0.610 0.601 0.618 0.623 0.613 0.627 0.615 1.53
58) T	2-Chloroethyl ... 0.230 0.247 0.270 0.307 0.303 0.313 0.278 12.41
59) T	2-Hexanone 0.385 0.414 0.466 0.473 0.477 0.473 0.448 8.69
60) T	Dibromochlorom... 0.306 0.326 0.378 0.400 0.415 0.431 0.376 13.28
61) T	1,2-Dibromoethane 0.322 0.333 0.359 0.373 0.368 0.381 0.356 6.54
62) S	4-Bromofluorob... 0.464 0.455 0.470 0.500 0.500 0.478 4.41
63) I	Chlorobenzene-d5 -----ISTD-----
64) T	Tetrachloroethene 0.347 0.323 0.390 0.375 0.345 0.344 0.354 6.84
65) PM	Chlorobenzene 1.131 1.046 1.093 1.098 1.085 1.114 1.094 2.65
66) T	1,1,1,2-Tetra... 0.369 0.341 0.365 0.390 0.382 0.395 0.374 5.22
67) C	Ethyl Benzene 1.803 1.816 1.919 2.022 1.979 2.036 1.929 5.24#
68) T	m/p-Xylenes 0.648 0.678 0.706 0.740 0.721 0.740 0.706 5.21
69) T	o-Xylene 0.642 0.639 0.688 0.727 0.706 0.726 0.688 5.75
70) T	Styrene 0.951 1.012 1.135 1.219 1.214 1.230 1.127 10.56
71) P	Bromoform 0.234 0.236 0.270 0.304 0.312 0.327 0.281 14.17
72) I	1,4-Dichlorobenzen... -----ISTD-----
73) T	Isopropylbenzene 3.789 3.562 3.843 4.130 3.876 4.156 3.893 5.72
74) T	N-amyl acetate 1.715 1.652 1.846 2.067 2.068 2.192 1.924 11.32
75) P	1,1,2,2-Tetra... 1.552 1.350 1.315 1.338 1.284 1.345 1.364 6.97
76) T	1,2,3-Trichlor... 1.405 1.167 1.151 1.187 1.131 1.181 1.204 8.36
77) T	Bromobenzene 0.926 0.862 0.896 0.928 0.883 0.928 0.904 3.08
78) T	n-propylbenzene 4.272 4.186 4.394 4.854 4.583 4.868 4.526 6.45
79) T	2-Chlorotoluene 3.184 2.748 2.832 2.994 2.805 2.953 2.919 5.45
80) T	1,3,5-Trimethy... 3.036 3.053 3.275 3.487 3.255 3.405 3.252 5.60
81) T	trans-1,4-Dich... 0.269 0.335 0.385 0.410 0.449 0.370 18.91
82) T	4-Chlorotoluene 3.226 2.939 3.196 3.430 3.255 3.379 3.238 5.32
83) T	tert-Butylbenzene 3.341 3.098 3.115 3.435 3.255 3.411 3.276 4.44
84) T	1,2,4-Trimethyl... 3.150 3.034 3.274 3.522 3.335 3.444 3.293 5.52
85) T	sec-Butylbenzene 3.708 3.767 3.937 4.282 4.095 4.343 4.022 6.55
86) T	p-Isopropyltol... 3.025 3.084 3.206 3.555 3.450 3.599 3.320 7.44
87) T	1,3-Dichlorobe... 1.619 1.558 1.633 1.701 1.656 1.729 1.649 3.71
88) T	1,4-Dichlorobe... 1.817 1.606 1.629 1.693 1.639 1.722 1.684 4.64
89) T	n-Butylbenzene 2.443 2.650 2.748 3.147 3.139 3.346 2.912 12.00
90) T	Hexachloroethane 0.511 0.523 0.551 0.622 0.622 0.680 0.585 11.44
91) T	1,2-Dichlorobe... 1.710 1.577 1.613 1.696 1.634 1.702 1.655 3.34
92) T	1,2-Dibromo-3.... 0.259 0.248 0.299 0.322 0.329 0.356 0.302 13.89
93) T	1,2,4-Trichlor... 0.862 0.842 0.861 0.981 1.035 1.123 0.951 12.03
94) T	Hexachlorobuta... 0.393 0.414 0.394 0.427 0.418 0.445 0.415 4.79
95) T	Naphthalene 3.499 2.929 3.204 3.613 3.690 3.984 3.487 10.69
96) T	1,2,3-Trichlor... 0.941 0.846 0.921 1.019 1.051 1.107 0.981 9.74

(#= Out of Range)

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046041.D  
 Acq On : 05 May 2025 11:35  
 Operator : JC/MD  
 Sample : VSTDICC020  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC020

Quant Time: May 06 06:08:45 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.543	168	83671	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	147096	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	127829	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	60503	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	31909	12.820	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 25.640%	#	
35) Dibromofluoromethane	5.385	113	21112	12.804	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 25.600%	#	
50) Toluene-d8	8.646	98	73333	13.200	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 26.400%	#	
62) 4-Bromofluorobenzene	11.079	95	26760	13.236	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 26.480%	#	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	23341	12.638	ug/l	96
3) Chloromethane	1.306	50	24316	13.371	ug/l	98
4) Vinyl Chloride	1.373	62	22096	13.868	ug/l	94
5) Bromomethane	1.593	94	9920	12.279	ug/l	93
6) Chloroethane	1.666	64	11832	14.414	ug/l	95
7) Trichlorofluoromethane	1.873	101	34636	14.271	ug/l	100
8) Diethyl Ether	2.129	74	11392	14.278	ug/l	94
9) 1,1,2-Trichlorotrifluo...	2.324	101	21027	14.499	ug/l	98
10) Methyl Iodide	2.446	142	25661	15.070	ug/l	99
11) Tert butyl alcohol	2.971	59	20370	68.662	ug/l	97
12) 1,1-Dichloroethene	2.312	96	18899	13.385	ug/l	98
13) Acrolein	2.233	56	26427	76.689	ug/l	95
14) Allyl chloride	2.660	41	37708	14.133	ug/l	99
15) Acrylonitrile	3.062	53	63290	71.312	ug/l	98
16) Acetone	2.379	43	60363	70.884	ug/l	99
17) Carbon Disulfide	2.501	76	43348	13.251	ug/l	100
18) Methyl Acetate	2.702	43	27234	13.397	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	68402	13.890	ug/l	100
20) Methylene Chloride	2.782	84	23050	13.362	ug/l	96
21) trans-1,2-Dichloroethene	3.086	96	19161	13.294	ug/l	96
22) Diisopropyl ether	3.763	45	74257	14.896	ug/l	95
23) Vinyl Acetate	3.720	43	322598	73.230	ug/l	100
24) 1,1-Dichloroethane	3.605	63	41257	14.082	ug/l	98
25) 2-Butanone	4.556	43	90331	73.489	ug/l	98
26) 2,2-Dichloropropane	4.470	77	30472	13.729	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	23970	13.791	ug/l	98
28) Bromochloromethane	4.897	49	21028	13.497	ug/l	99
29) Tetrahydrofuran	5.007	42	56819	71.175	ug/l	100
30) Chloroform	5.086	83	43065	14.144	ug/l	95
31) Cyclohexane	5.458	56	36470	14.769	ug/l	95
32) 1,1,1-Trichloroethane	5.379	97	37003	14.092	ug/l	98
36) 1,1-Dichloropropene	5.684	75	27242	14.231	ug/l	98
37) Ethyl Acetate	4.720	43	33458	13.931	ug/l	98
38) Carbon Tetrachloride	5.671	117	31091	14.137	ug/l	98
39) Methylcyclohexane	7.372	83	35077	14.623	ug/l	99
40) Benzene	6.031	78	83898	14.140	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046041.D  
 Acq On : 05 May 2025 11:35  
 Operator : JC/MD  
 Sample : VSTDICC020  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC020

Quant Time: May 06 06:08:45 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.915	41	18732	14.038	ug/1	95
42) 1,2-Dichloroethane	6.080	62	37203	15.165	ug/1	100
43) Isopropyl Acetate	6.342	43	53275	14.512	ug/1	99
44) Trichloroethene	7.116	130	20239	14.429	ug/1	99
45) 1,2-Dichloropropane	7.427	63	20940	14.204	ug/1	98
46) Dibromomethane	7.580	93	16781	14.439	ug/1	99
47) Bromodichloromethane	7.817	83	32762	14.545	ug/1	94
48) Methyl methacrylate	7.689	41	27374	14.521	ug/1	100
49) 1,4-Dioxane	7.659	88	10585	282.442	ug/1	98
51) 4-Methyl-2-Pentanone	8.573	43	182455	75.775	ug/1	98
52) Toluene	8.713	92	52030	14.788	ug/1	99
53) t-1,3-Dichloropropene	8.976	75	27549	14.566	ug/1	100
54) cis-1,3-Dichloropropene	8.366	75	31226	14.154	ug/1	98
55) 1,1,2-Trichloroethane	9.152	97	20536	14.442	ug/1	96
56) Ethyl methacrylate	9.116	69	31787	14.425	ug/1	98
57) 1,3-Dichloropropane	9.305	76	36341	14.417	ug/1	98
58) 2-Chloroethyl Vinyl ether	8.238	63	79531	80.312	ug/1	100
59) 2-Hexanone	9.427	43	137054	74.997	ug/1	99
60) Dibromochloromethane	9.518	129	22267	14.387	ug/1	99
61) 1,2-Dibromoethane	9.610	107	21113	14.458	ug/1	96
64) Tetrachloroethene	9.268	164	19924	15.263	ug/1	97
65) Chlorobenzene	10.079	112	55863	14.202	ug/1	100
66) 1,1,1,2-Tetrachloroethane	10.158	131	18671	14.231	ug/1	98
67) Ethyl Benzene	10.189	91	98113	14.631	ug/1	100
68) m/p-Xylenes	10.299	106	72202	29.806	ug/1	99
69) o-Xylene	10.640	106	35178	14.408	ug/1	96
70) Styrene	10.652	104	58034	14.853	ug/1	98
71) Bromoform	10.799	173	13825	14.030	ug/1 #	100
73) Isopropylbenzene	10.957	105	93013	14.096	ug/1	99
74) N-amyl acetate	10.841	43	44684	13.581	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	31830	13.560	ug/1	99
76) 1,2,3-Trichloropropane	11.237	75	27845m	11.039	ug/1	
77) Bromobenzene	11.195	156	21695	14.212	ug/1	96
78) n-propylbenzene	11.298	91	106337	14.376	ug/1	99
79) 2-Chlorotoluene	11.359	91	68534	13.748	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	79261	14.468	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	8104	13.371	ug/1	91
82) 4-Chlorotoluene	11.451	91	77338	14.116	ug/1	100
83) tert-Butylbenzene	11.713	119	75382	14.011	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	79232	14.480	ug/1	99
85) sec-Butylbenzene	11.890	105	95271	14.263	ug/1	100
86) p-Isopropyltoluene	12.006	119	77599	14.387	ug/1	98
87) 1,3-Dichlorobenzene	11.969	146	39520	13.898	ug/1	98
88) 1,4-Dichlorobenzene	12.036	146	39419	14.146	ug/1	99
89) n-Butylbenzene	12.329	91	66506	14.184	ug/1	99
90) Hexachloroethane	12.536	117	13332	13.287	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	39031	14.092	ug/1	98
92) 1,2-Dibromo-3-Chloropr...	12.938	75	7232	13.535	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	20846	13.745	ug/1	99
94) Hexachlorobutadiene	13.725	225	9524	13.426	ug/1	97
95) Naphthalene	13.774	128	77542	14.040	ug/1	99
96) 1,2,3-Trichlorobenzene	13.956	180	22301	14.023	ug/1	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046041.D  
 Acq On : 05 May 2025 11:35  
 Operator : JC/MD  
 Sample : VSTDICC020  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC020

Quant Time: May 06 06:08:45 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046041.D  
Acq On : 05 May 2025 11:35  
Operator : JC/MD  
Sample : VSTDIICC020  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC020

## Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

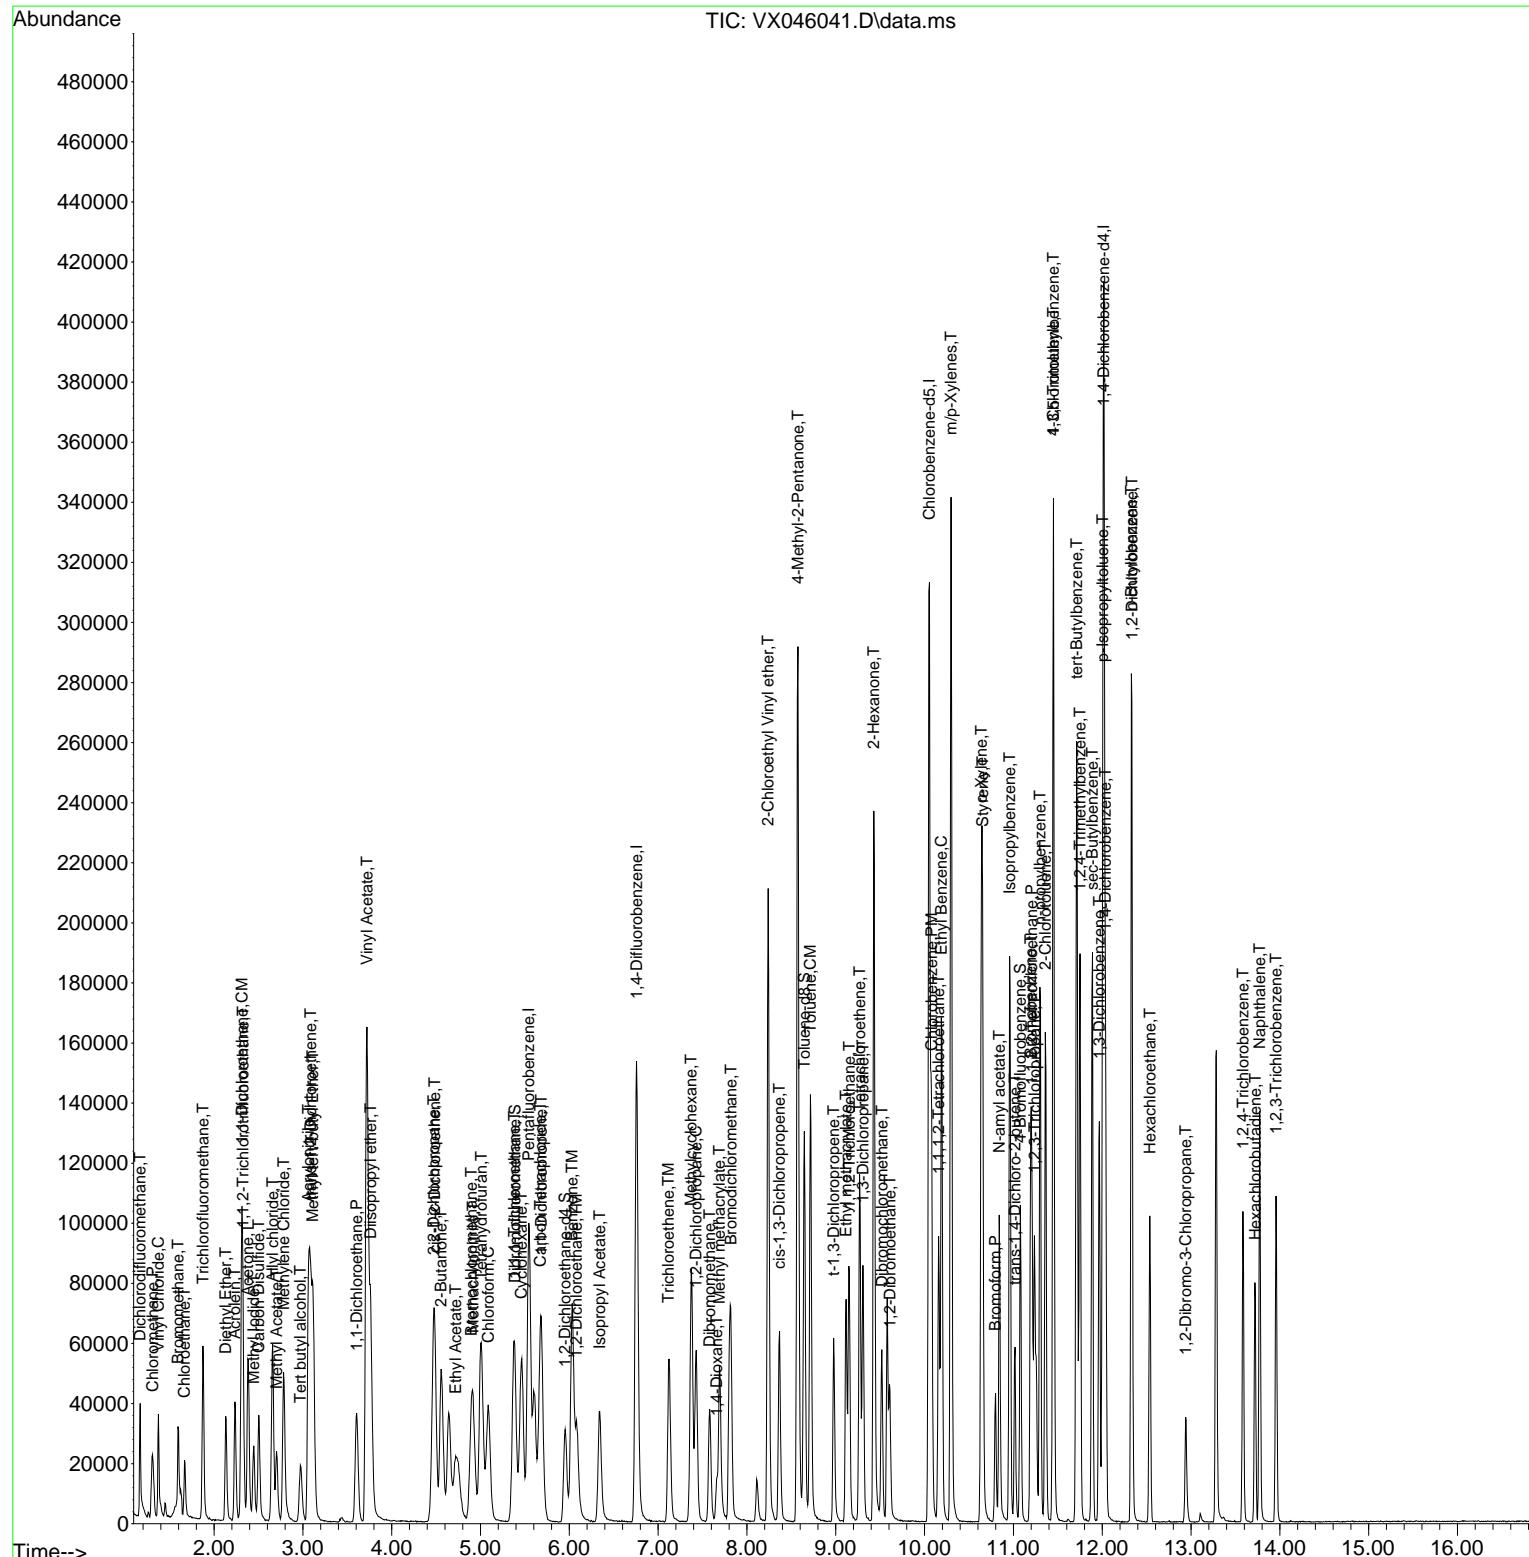


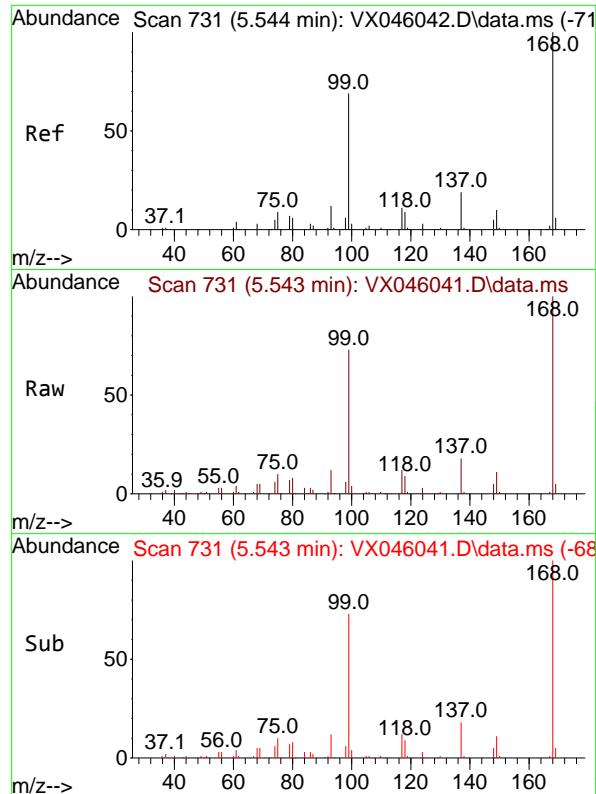


#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.543 min Scan# 7  
Delta R.T. -0.001 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


1 Manual Integrations  
2 APPROVED


3 Reviewed By :John Carlone 05/06/2025  
4 Supervised By :Mahesh Dadoda 05/06/2025

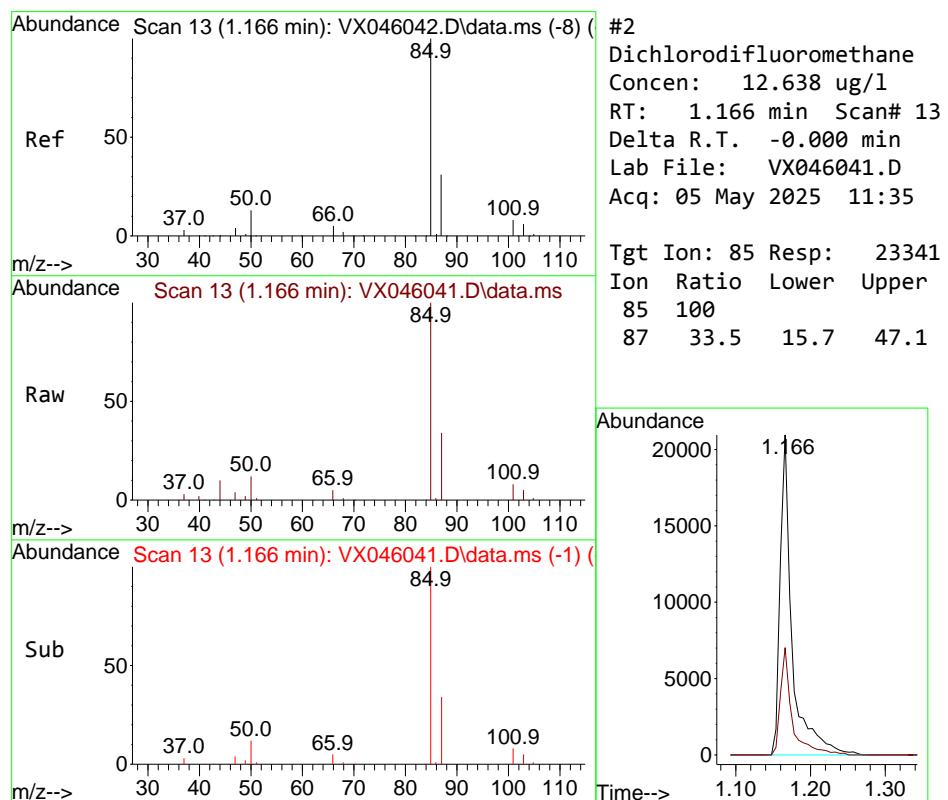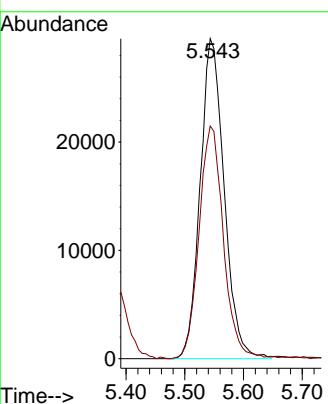


#2  
Dichlorodifluoromethane  
Concen: 12.638 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion: 85 Resp: 23341  
Ion Ratio Lower Upper  
85 100  
87 33.5 15.7 47.1

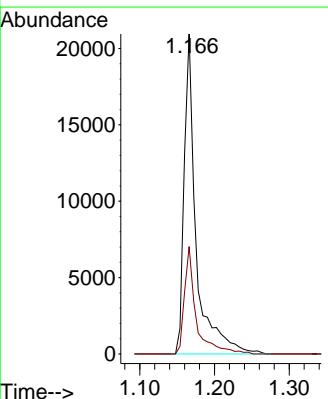




Ref Scan 36 (1.306 min): VX046041.D\data.ms

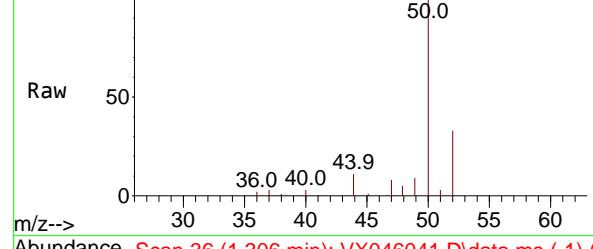

Raw Scan 36 (1.306 min): VX046041.D\data.ms (-1)

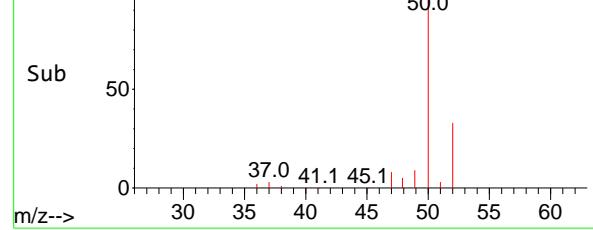

#3

Chloromethane

Concen: 13.371 ug/l

RT: 1.306 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020


**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025


Supervised By :Mahesh Dadoda 05/06/2025



Ref Scan 47 (1.373 min): VX046041.D\data.ms

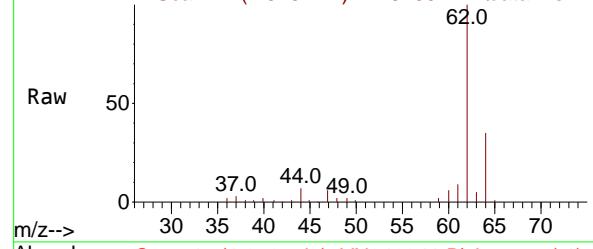

Sub Scan 47 (1.373 min): VX046041.D\data.ms (-1)

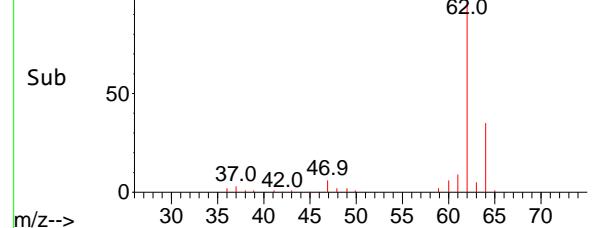

#4

Vinyl Chloride

Concen: 13.868 ug/l

RT: 1.373 min Scan# 47

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35




Tgt Ion: 62 Resp: 22096

Ion Ratio Lower Upper

62 100

64 34.9 25.2 37.8

1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16







#5  
Bromomethane  
Concen: 12.279 ug/l  
RT: 1.593 min Scan# 8  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#6  
Chloroethane  
Concen: 14.414 ug/l  
RT: 1.666 min Scan# 95  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion: 64 Resp: 11832  
Ion Ratio Lower Upper  
64 100  
66 32.9 24.3 36.5




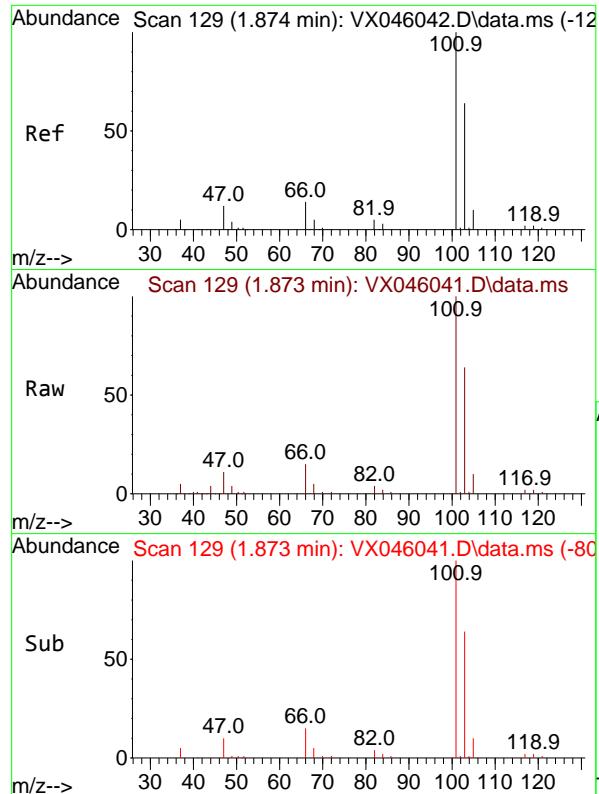


#7  
Trichlorofluoromethane  
Concen: 14.271 ug/l  
RT: 1.873 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**







Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

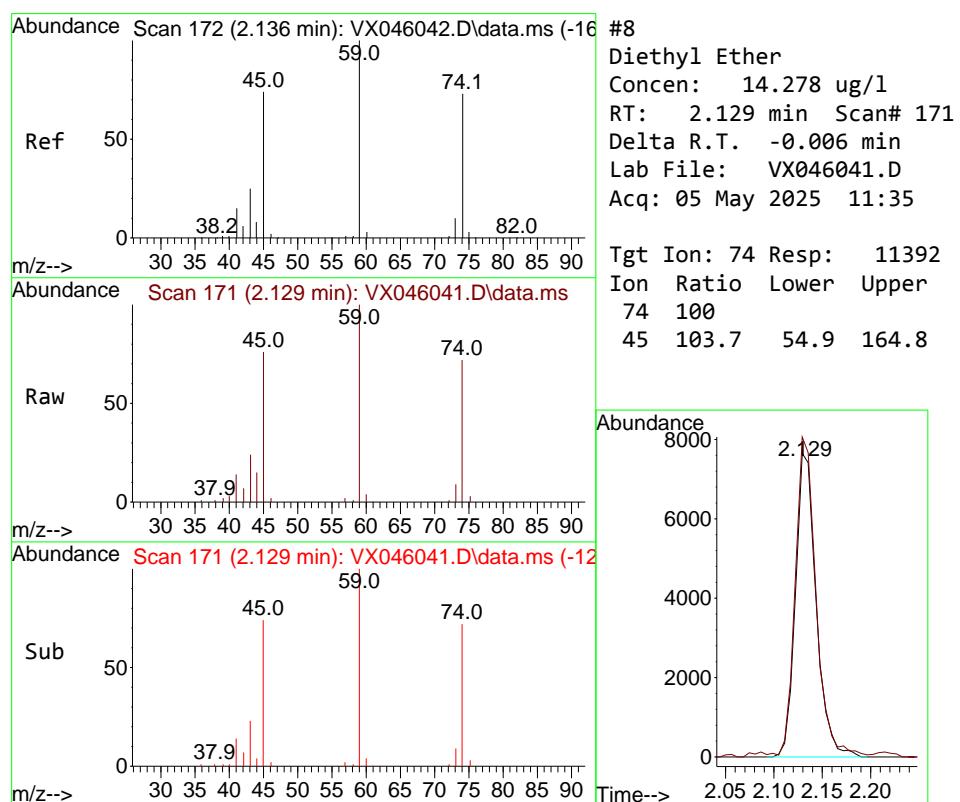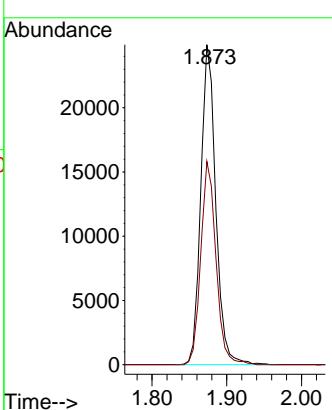

#8  
Diethyl Ether  
Concen: 14.278 ug/l  
RT: 2.129 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion: 74 Resp: 11392  
Ion Ratio Lower Upper  
74 100  
45 103.7 54.9 164.8

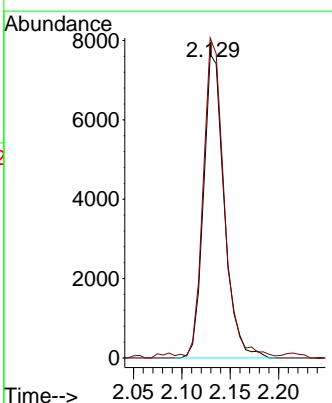

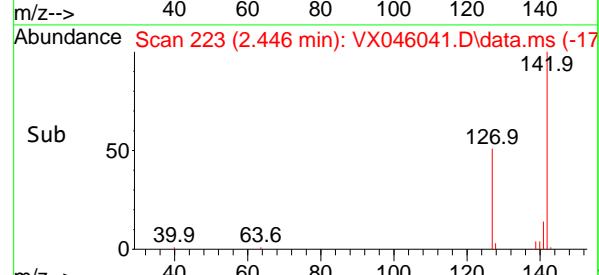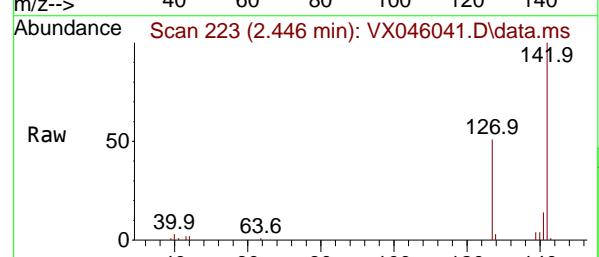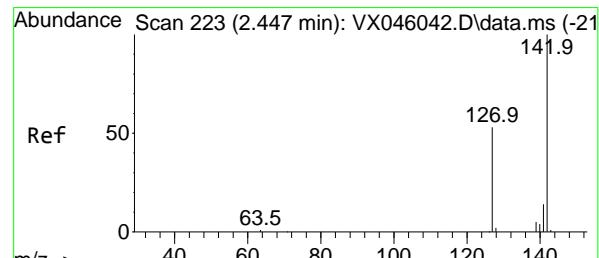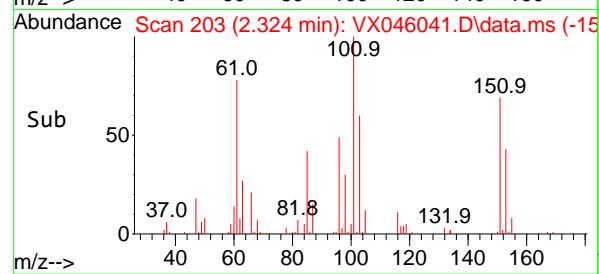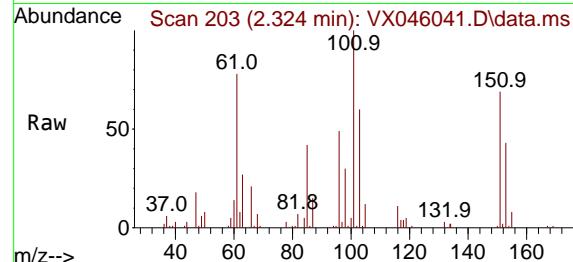

#9

1,1,2-Trichlorotrifluoroethane

Concen: 14.499 ug/l

RT: 2.324 min Scan# 2102

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

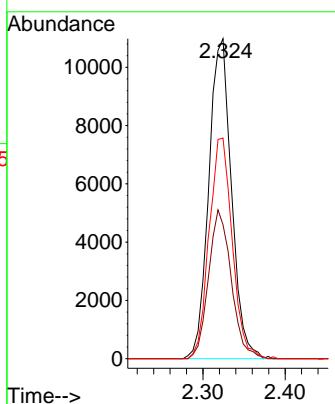

#10  
Methyl Iodide

Concen: 15.070 ug/l


RT: 2.446 min Scan# 223




Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion:142 Resp: 25661  
Ion Ratio Lower Upper  
142 100  
127 53.0 41.7 62.5  
141 14.7 11.5 17.3

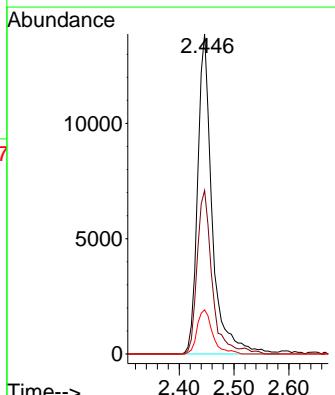

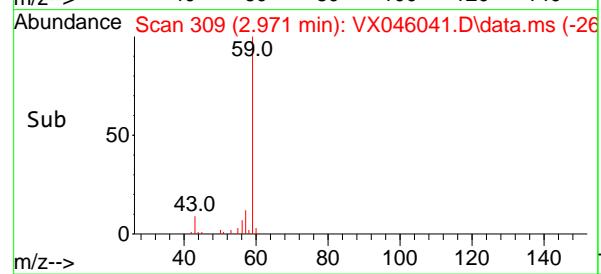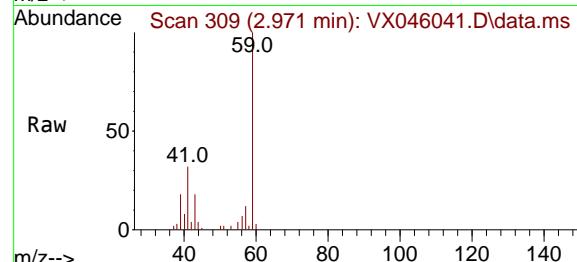

#11

Tert butyl alcohol

Concen: 68.662 ug/l

RT: 2.971 min Scan# 309

Delta R.T. -0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

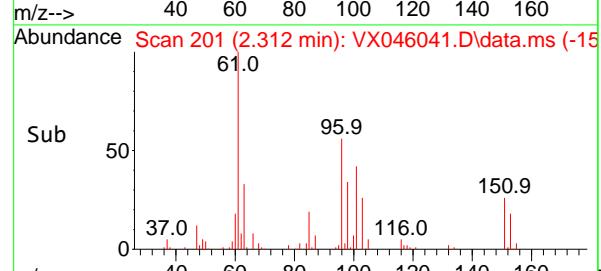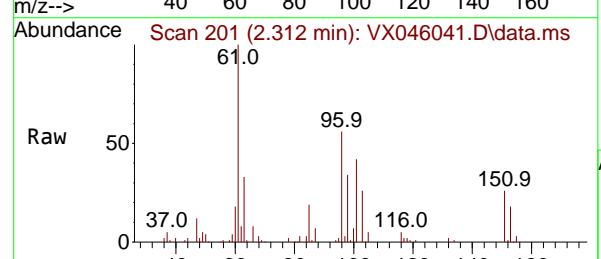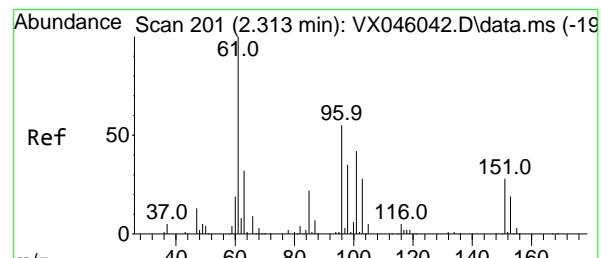

#12

1,1-Dichloroethene

Concen: 13.385 ug/l

RT: 2.312 min Scan# 201

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion: 96 Resp: 18899


Ion Ratio Lower Upper

96 100

61 179.8 146.2 219.2

98 61.8 51.0 76.6




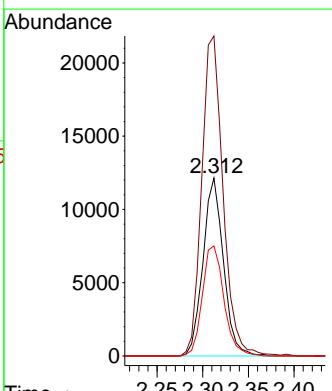





#13

Acrolein  
Concen: 76.689 ug/l  
RT: 2.233 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020

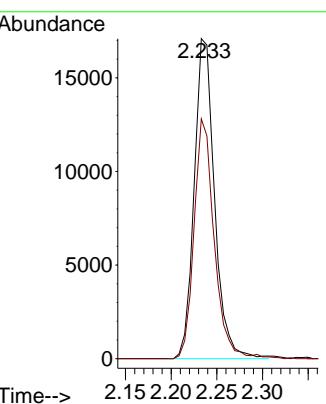


#14  
Allyl chloride  
Concen: 14.133 ug/l  
RT: 2.660 min Scan# 258  
Delta R.T. 0.006 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35



Tgt Ion: 41 Resp: 37708  
Ion Ratio Lower Upper  
41 100  
39 75.0 60.6 90.8  
76 30.6 24.9 37.3

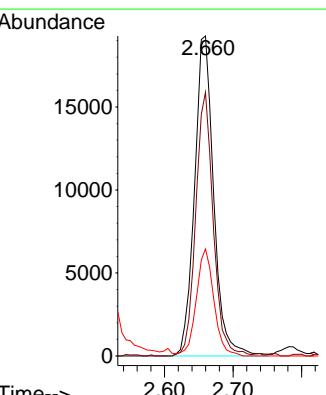

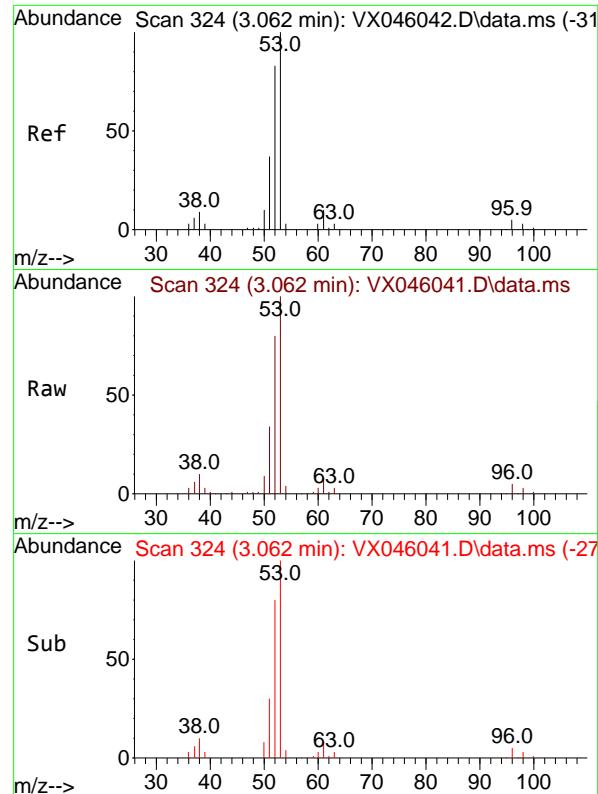

#15

Acrylonitrile

Concen: 71.312 ug/l

RT: 3.062 min Scan# 31

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

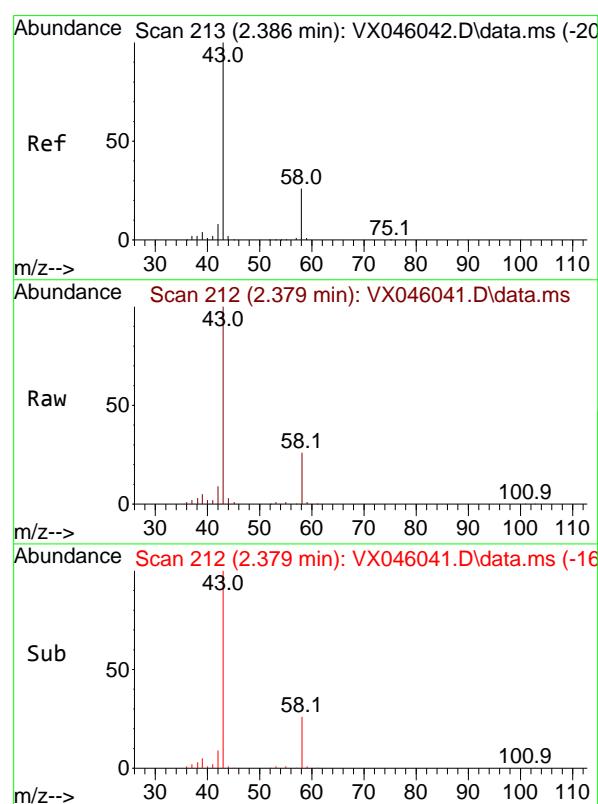

#16

Acetone

Concen: 70.884 ug/l

RT: 2.379 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35


Tgt Ion: 43 Resp: 60363

Ion Ratio Lower Upper



43 100

58 26.0 21.2 31.8

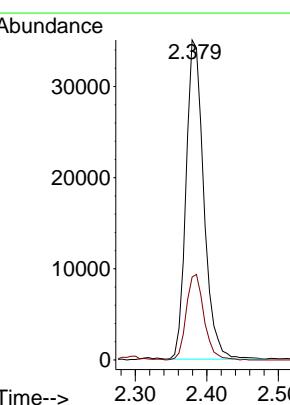




Abundance Scan 232 (2.501 min): VX046041.D\data.ms

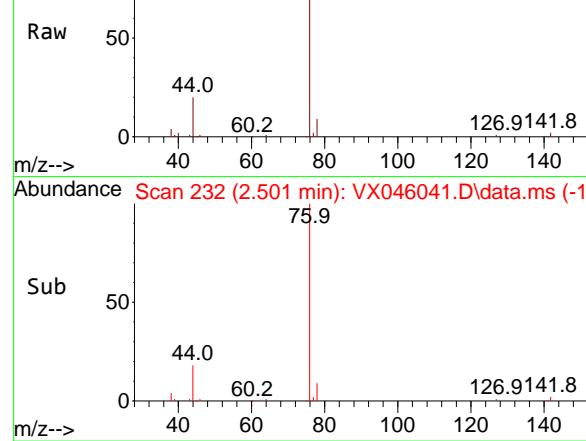

Abundance Scan 265 (2.702 min): VX046041.D\data.ms

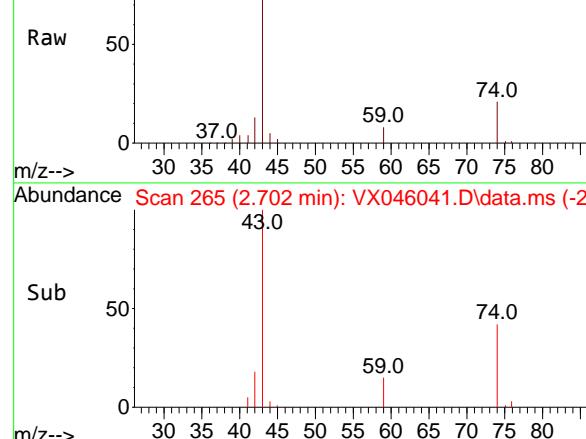

#17

Carbon Disulfide

Concen: 13.251 ug/l

RT: 2.501 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

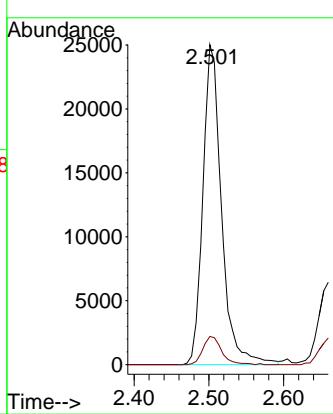

#18

Methyl Acetate

Concen: 13.397 ug/l

RT: 2.702 min Scan# 265

Delta R.T. -0.000 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35




Tgt Ion: 43 Resp: 27234

Ion Ratio Lower Upper

43 100

74 20.7 16.7 25.1





#19

Methyl tert-butyl Ether

Concen: 13.890 ug/l

RT: 3.111 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

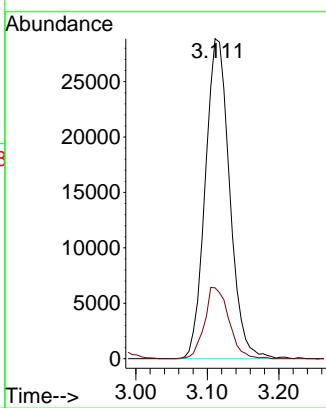

#20

Methylene Chloride

Concen: 13.362 ug/l

RT: 2.782 min Scan# 278

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion: 84 Resp: 23050


Ion Ratio Lower Upper


84 100

49 146.0 113.9 170.9



51 43.8 33.5 50.3

86 62.2 53.8 80.8

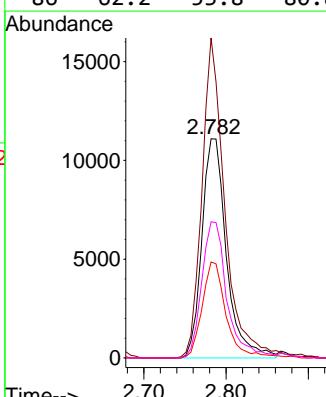




Abundance Scan 328 (3.086 min): VX046041.D\data.ms

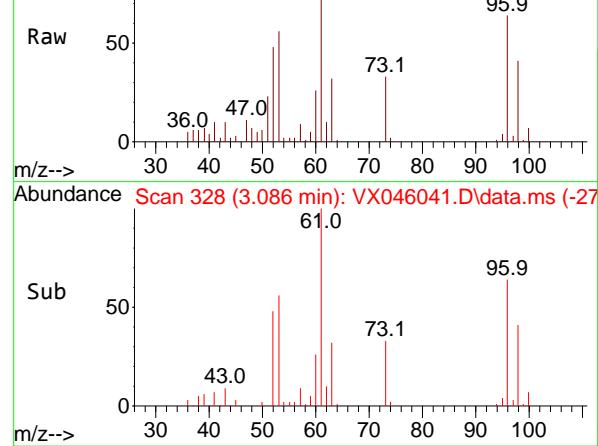

Abundance Scan 439 (3.763 min): VX046041.D\data.ms

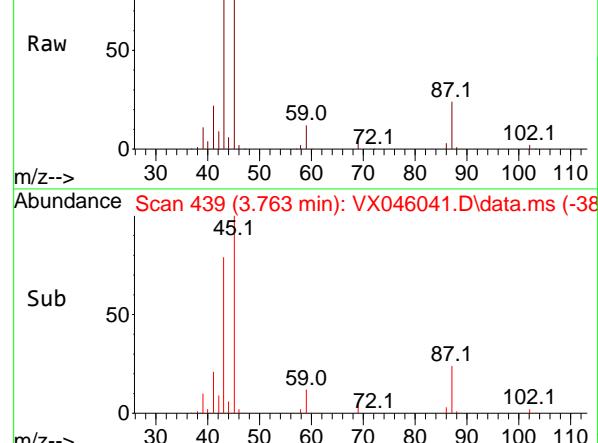

Abundance Scan 439 (3.763 min): VX046041.D\data.ms (-38)

Sub

50

0

45.1  
102.1  
87.1  
59.0  
72.1

#21

trans-1,2-Dichloroethene

Concen: 13.294 ug/l

RT: 3.086 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#22

Diisopropyl ether

Concen: 14.896 ug/l

RT: 3.763 min Scan# 439

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion: 45 Resp: 74257


Ion Ratio Lower Upper


45 100

43 78.2 66.6 100.0

87 24.0 19.8 29.6

59 11.7 8.6 12.8





#23

## Vinyl Acetate

Concen: 73.230 ug/l


RT: 3.720 min Scan# 413

Delta R.T. -0.000 min


Lab File: VX046041.D

Acq: 05 May 2025 11:35

Abundance Scan 432 (3.720 min): VX046041.D\data.ms

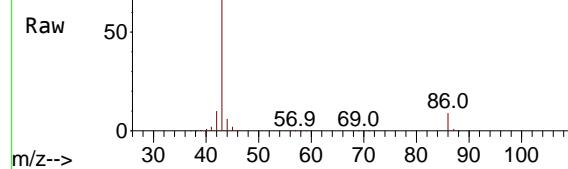

Abundance Scan 432 (3.720 min): VX046041.D\data.ms (-38)

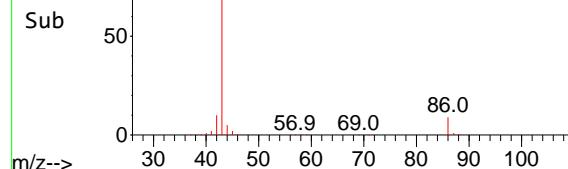

Tgt Ion: 43 Resp: 32259

Ion Ratio Lower Upper

43 100



86 9.3 7.5 11.3

## Manual Integrations

## APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

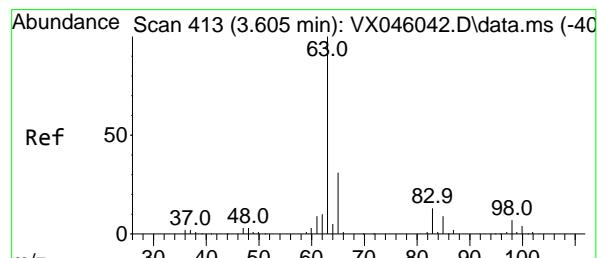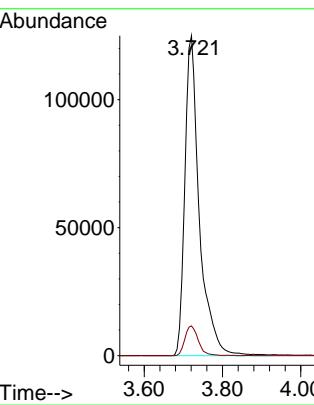

#24

## 1,1-Dichloroethane

Concen: 14.082 ug/l


RT: 3.605 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Abundance Scan 413 (3.605 min): VX046041.D\data.ms

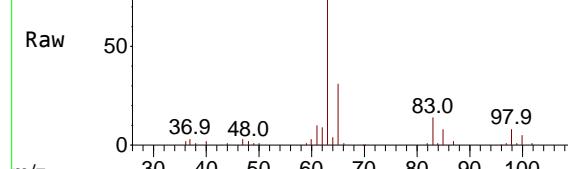

Tgt Ion: 63 Resp: 41257



Ion Ratio Lower Upper


63 100

98 7.9 3.6 10.8

100 5.0 2.1 6.3



Abundance Scan 413 (3.605 min): VX046041.D\data.ms (-36)

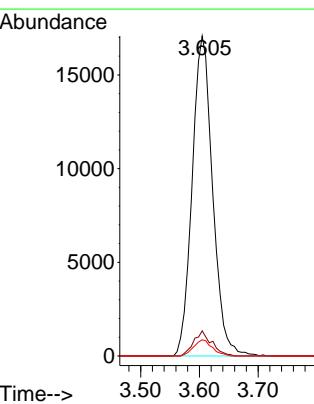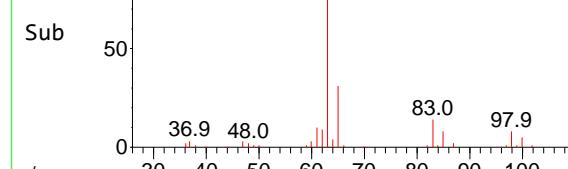



#25  
2-Butanone  
Concen: 73.489 ug/l  
RT: 4.556 min Scan# 5  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020

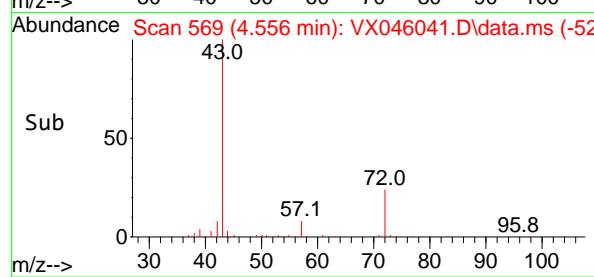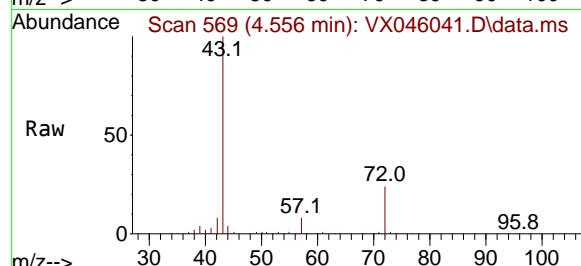


Tgt Ion: 43 Resp: 9033  
Ion Ratio Lower Upper  
43 100  
72 23.8 18.4 27.6

Manual Integrations  
**APPROVED**



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025


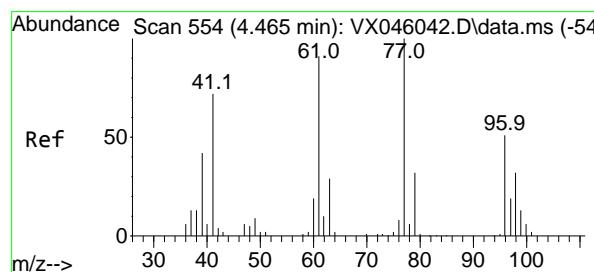
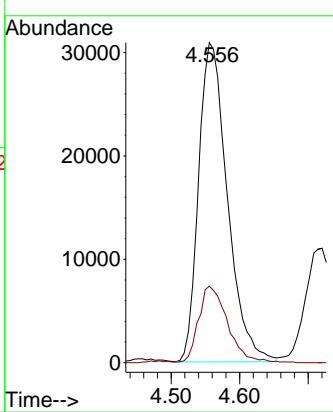


#26  
2,2-Dichloropropane  
Concen: 13.729 ug/l  
RT: 4.470 min Scan# 555  
Delta R.T. 0.006 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

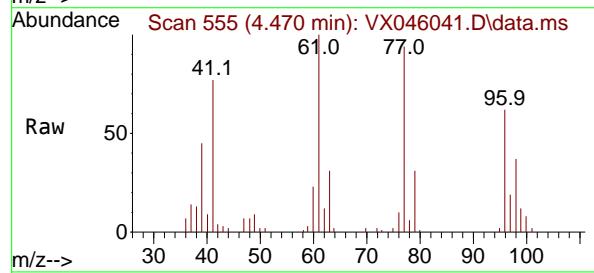

Tgt Ion: 77 Resp: 30472  
Ion Ratio Lower Upper  
77 100  
97 20.9 10.5 31.5

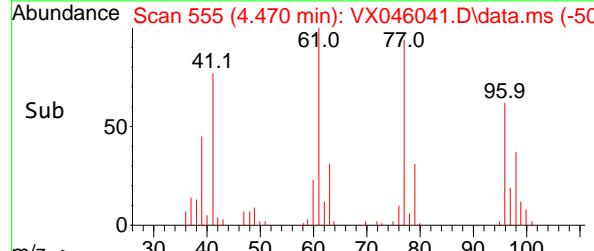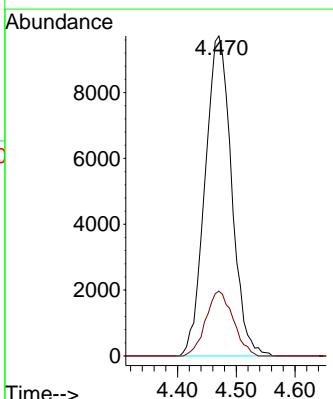






#27  
cis-1,2-Dichloroethene  
Concen: 13.791 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020



**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025




#28  
Bromochloromethane  
Concen: 13.497 ug/l  
RT: 4.897 min Scan# 625  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35


Tgt Ion: 49 Resp: 21028  
Ion Ratio Lower Upper  
49 100  
129 1.9 0.0 4.0  
130 70.9 56.2 84.2



Abundance Scan 642 (5.001 min): VX046042.D\data.ms (-63)

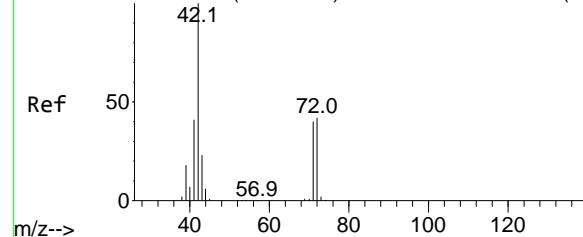

Abundance Scan 643 (5.007 min): VX046041.D\data.ms

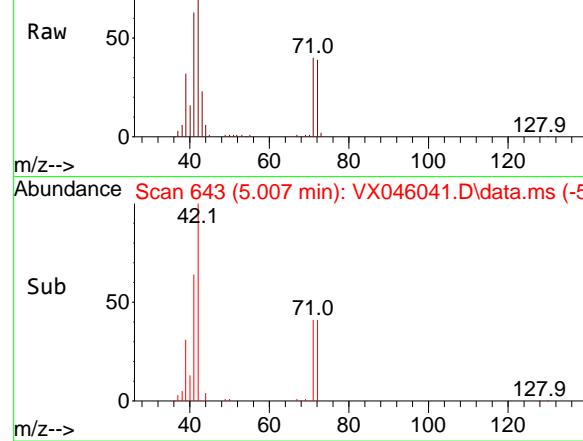

#29

Tetrahydrofuran

Concen: 71.175 ug/l

RT: 5.007 min Scan# 643

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument : MSVOA\_X


ClientSampleId : VSTDICC020

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance Scan 656 (5.087 min): VX046042.D\data.ms (-64)

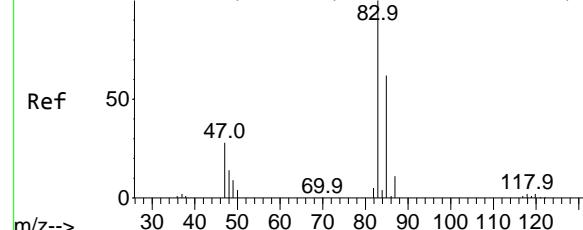

Abundance Scan 656 (5.086 min): VX046041.D\data.ms

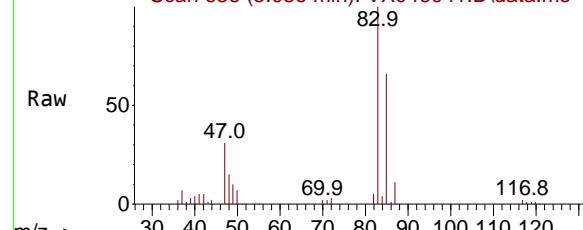

#30

Chloroform

Concen: 14.144 ug/l

RT: 5.086 min Scan# 656

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion: 83 Resp: 43065

Ion Ratio Lower Upper

83 100

85 65.7 49.3 73.9

Abundance Scan 656 (5.086 min): VX046041.D\data.ms (-60)

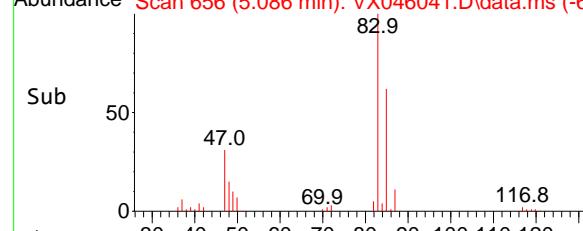

Abundance




Time--&gt;

4.90

5.00

5.10

5.20



#31

Cyclohexane

Concen: 14.769 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#32

1,1,1-Trichloroethane

Concen: 14.092 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion: 97 Resp: 37003







Ion Ratio Lower Upper

97 100

99 62.8 51.8 77.6

61 49.5 40.1 60.1

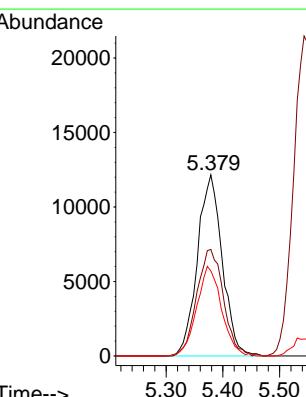

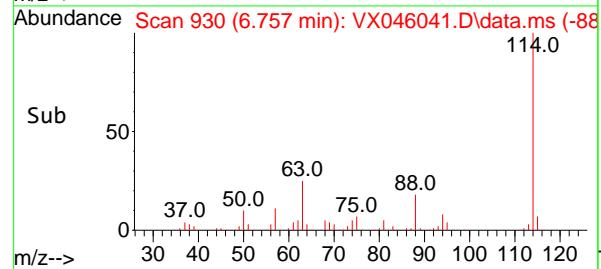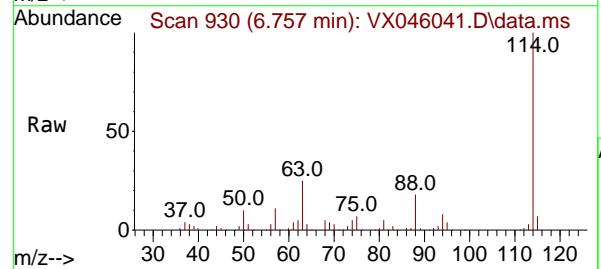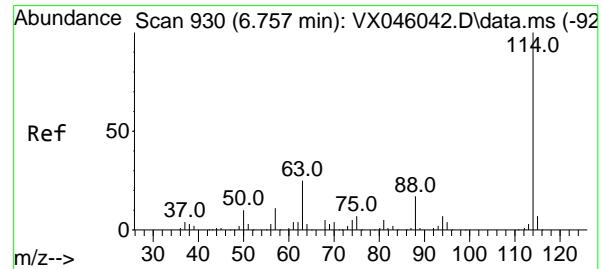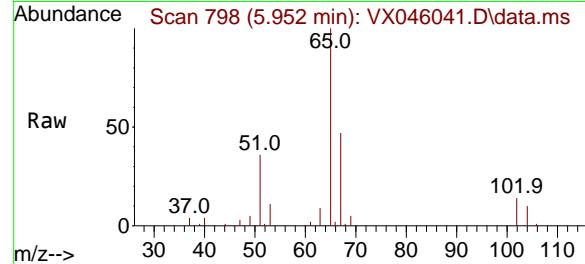

#33

1,2-Dichloroethane-d4

Concen: 12.820 ug/l

RT: 5.952 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025







Supervised By :Mahesh Dadoda 05/06/2025

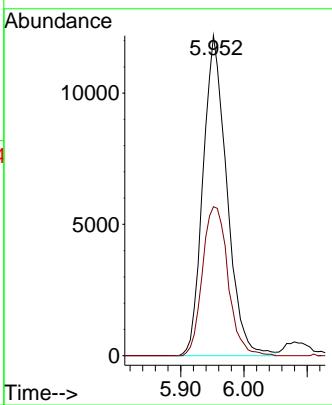

#34

Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
114	100	147096		
63	25.2	0.0	49.2	
88	18.0	0.0	33.6	

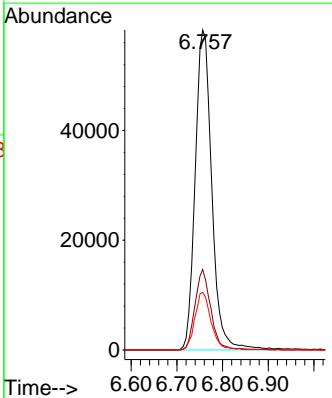

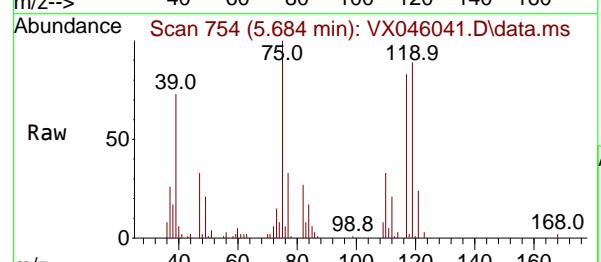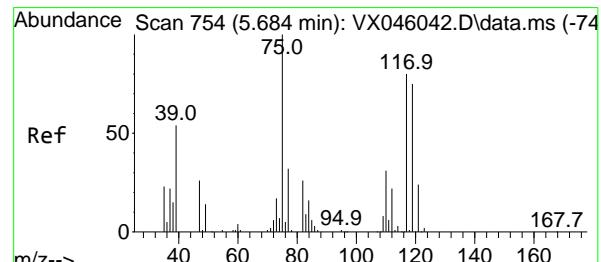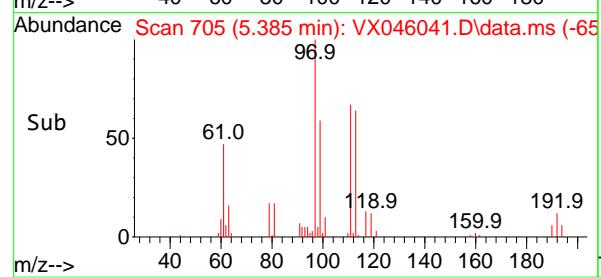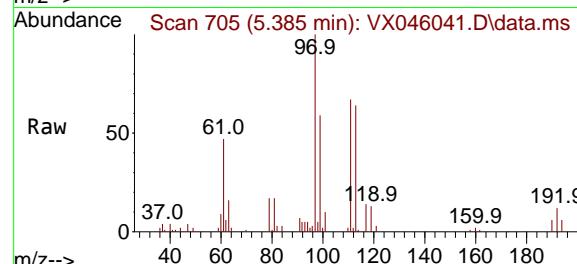

#35

Dibromofluoromethane

Concen: 12.804 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#36

1,1-Dichloropropene

Concen: 14.231 ug/l

RT: 5.684 min Scan# 754

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion: 75 Resp: 27242


Ion Ratio Lower Upper

75 100

110 31.6 16.3 48.9

77 31.9 24.3 36.5

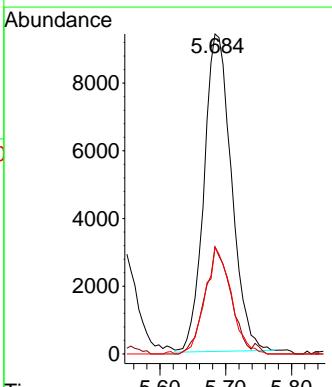

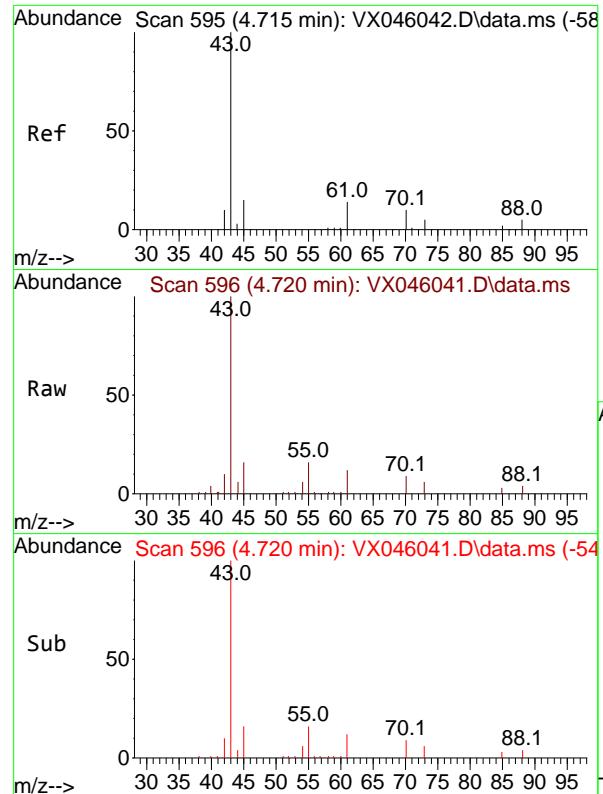

#37

Ethyl Acetate

Concen: 13.931 ug/l

RT: 4.720 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC020

Tgt Ion: 43 Resp: 33453

Ion Ratio Lower Upper

43 100

61 12.6 10.3 15.5



70 10.9 7.9 11.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

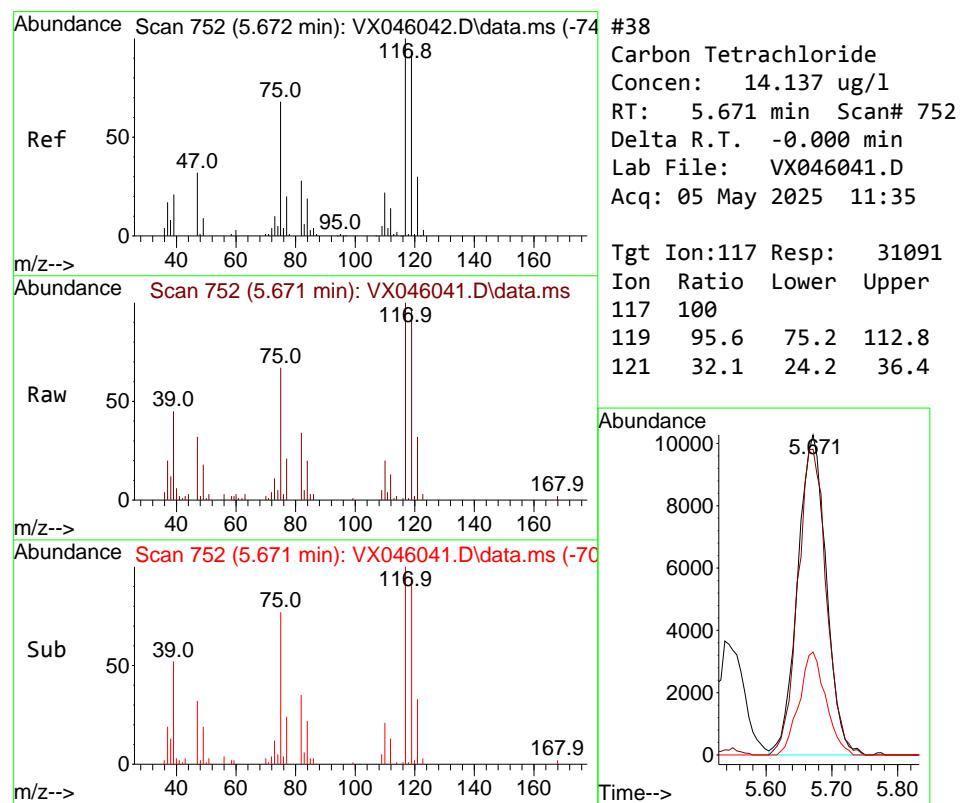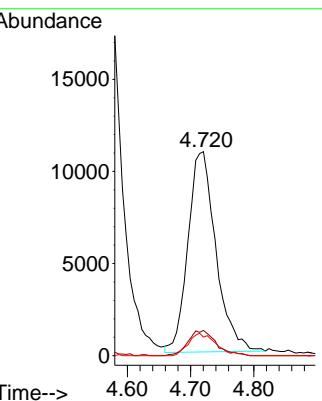

#38

Carbon Tetrachloride

Concen: 14.137 ug/l

RT: 5.671 min Scan# 752

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion:117 Resp: 31091


Ion Ratio Lower Upper

117 100

119 95.6 75.2 112.8

121 32.1 24.2 36.4

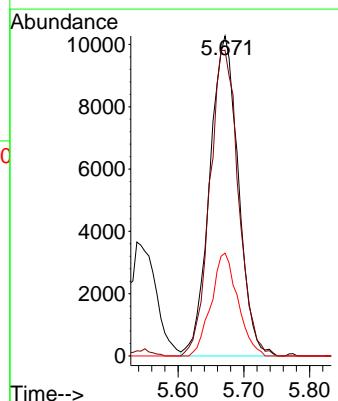

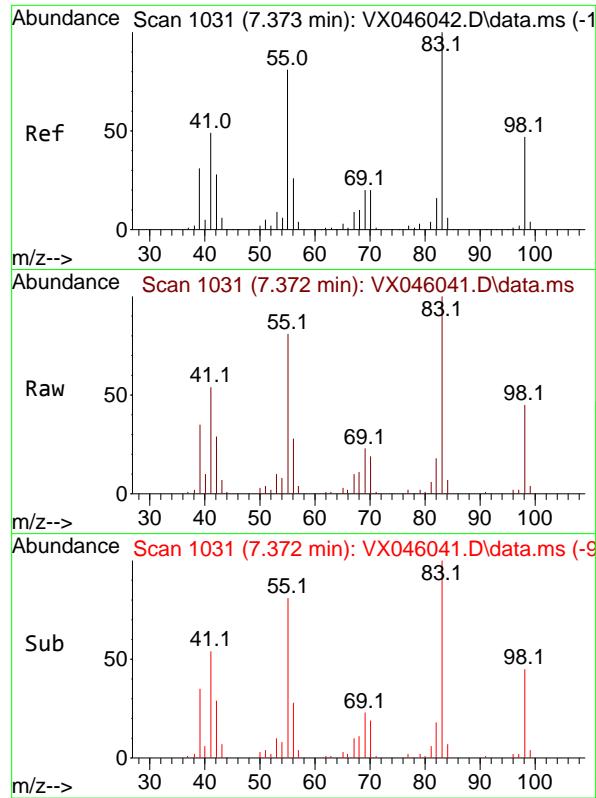

#39

Methylcyclohexane

Concen: 14.623 ug/l

RT: 7.372 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

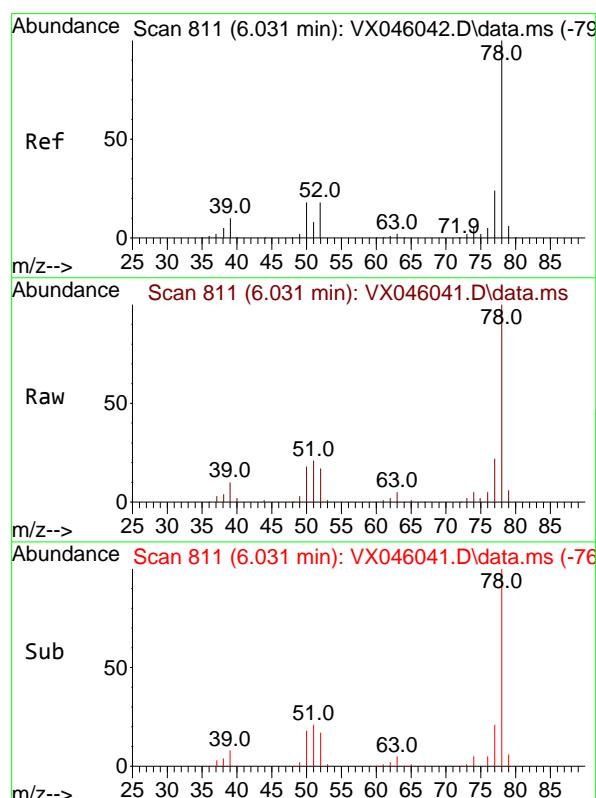

#40

Benzene

Concen: 14.140 ug/l

RT: 6.031 min Scan# 811

Delta R.T. -0.000 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35


Tgt Ion: 78 Resp: 83898

Ion Ratio Lower Upper

78 100

77 22.3 19.0 28.4

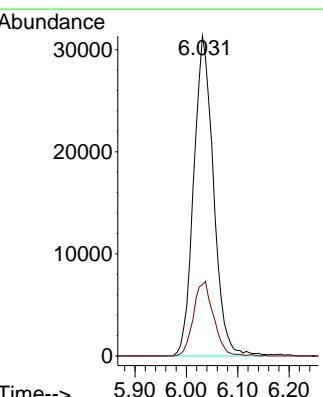

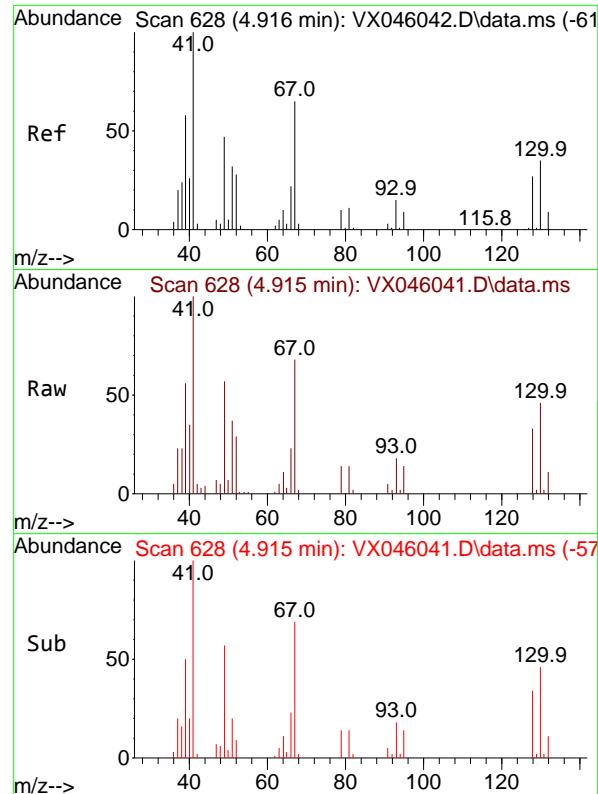

#41

Methacrylonitrile

Concen: 14.038 ug/l

RT: 4.915 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

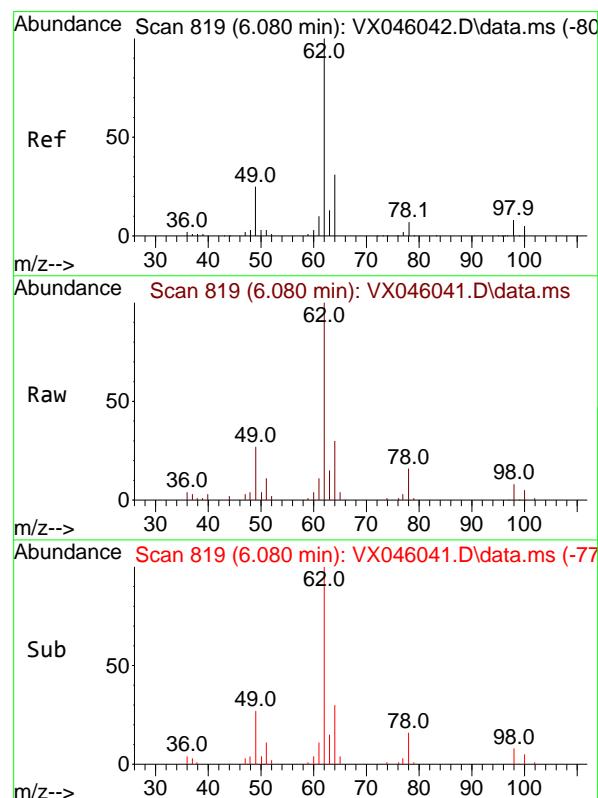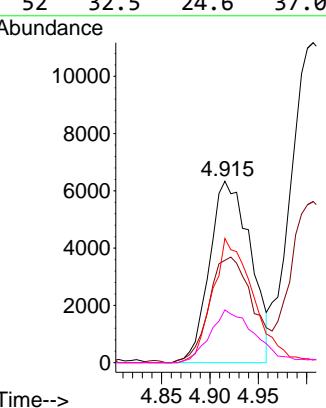

#42

1,2-Dichloroethane

Concen: 15.165 ug/l

RT: 6.080 min Scan# 819


Delta R.T. -0.000 min


Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion: 62 Resp: 37203

Ion	Ratio	Lower	Upper
62	100		
98	7.6	0.0	15.2

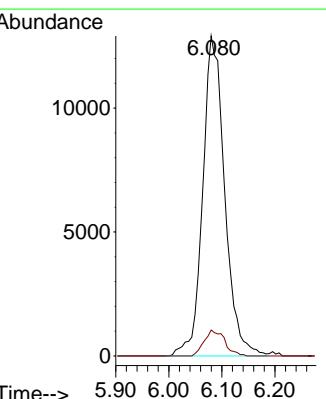



#43

Isopropyl Acetate

Concen: 14.512 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC020



Tgt Ion: 43 Resp: 5327

Ion Ratio Lower Upper

43 100

61 17.3 14.3 21.5




87 11.6 9.5 14.3

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

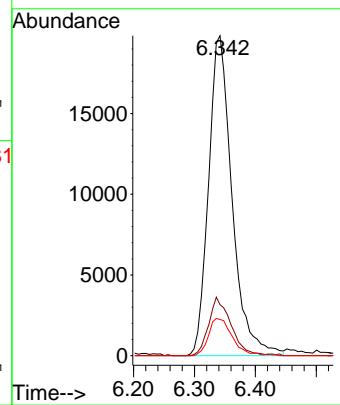

#44

Trichloroethene


Concen: 14.429 ug/l

RT: 7.116 min Scan# 989

Delta R.T. -0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35








Tgt Ion:130 Resp: 20239

Ion Ratio Lower Upper

130 100

95 102.8 0.0 204.2

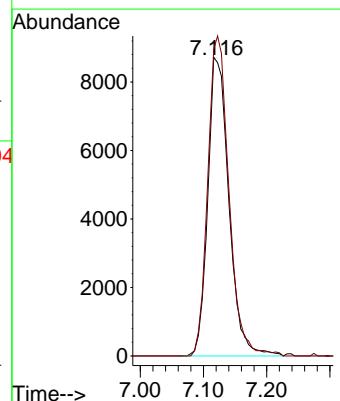

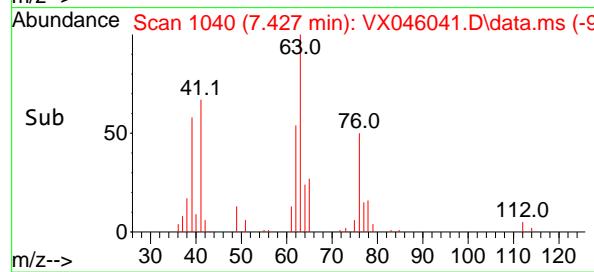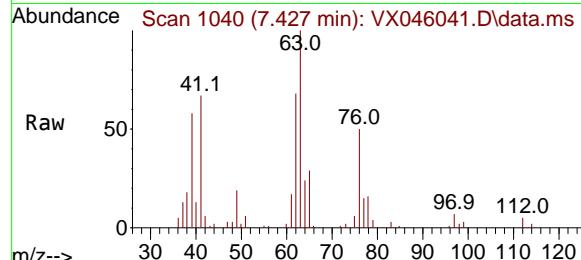

#45

1,2-Dichloropropane

Concen: 14.204 ug/l

RT: 7.427 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

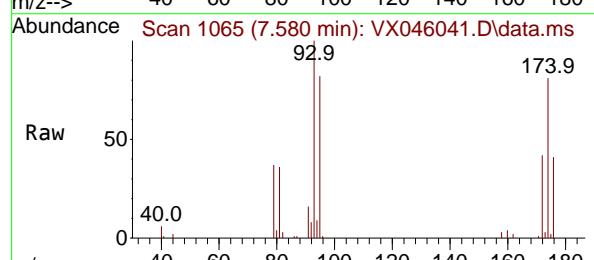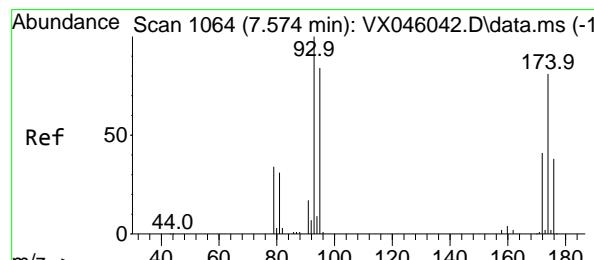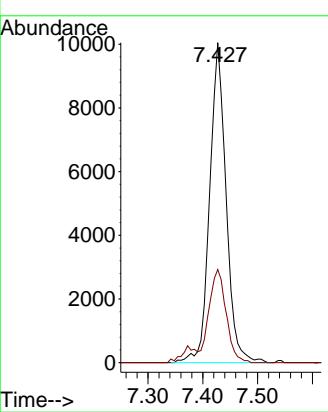

#46

Dibromomethane

Concen: 14.439 ug/l


RT: 7.580 min Scan# 1065



Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt	Ion	Resp:		
	Ion	Ratio	Lower	Upper
	93	100		
	95	81.5	65.6	98.4
	174	83.1	68.2	102.2

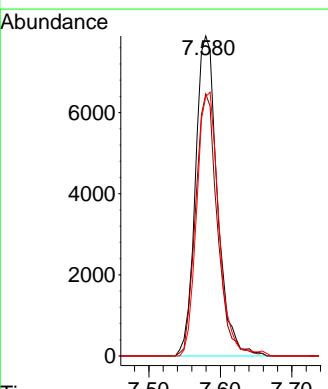

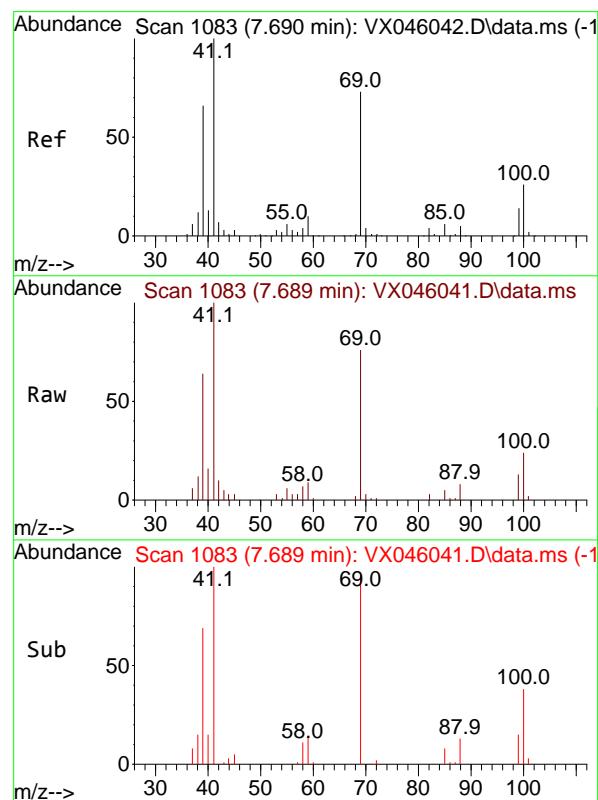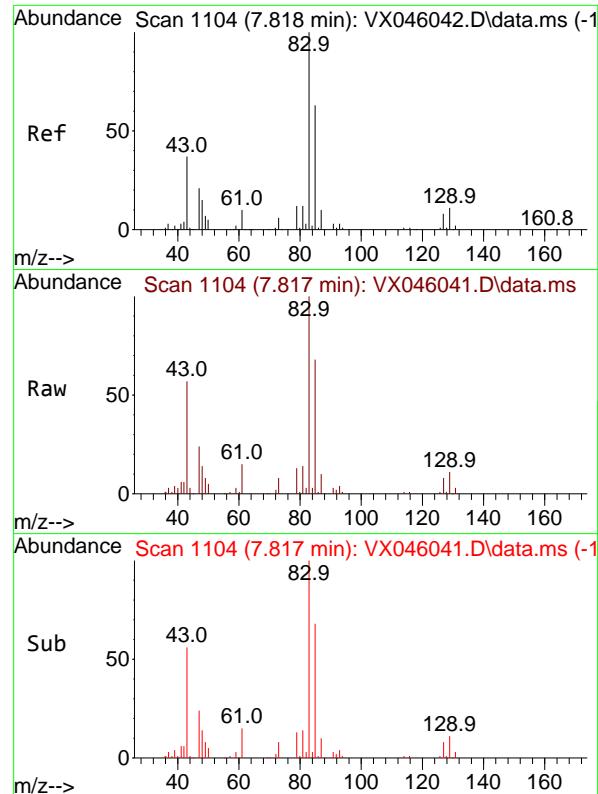

#47

Bromodichloromethane

Concen: 14.545 ug/l

RT: 7.817 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#48

Methyl methacrylate

Concen: 14.521 ug/l

RT: 7.689 min Scan# 1083

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion: 41 Resp: 27374


Ion Ratio Lower Upper

41 100



69 73.5 58.5 87.7

39 64.9 51.7 77.5






Abundance Scan 1078 (7.659 min): VX046041.D\data.ms

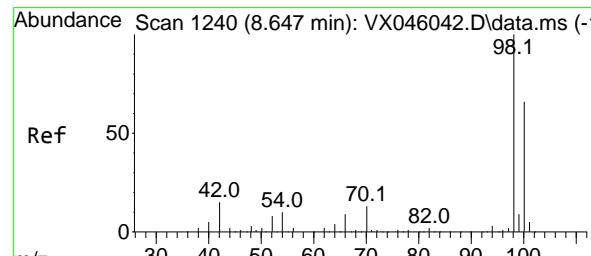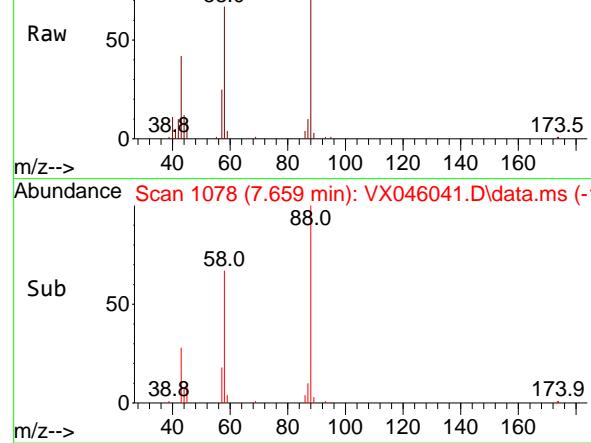

Abundance Scan 1240 (8.646 min): VX046041.D\data.ms

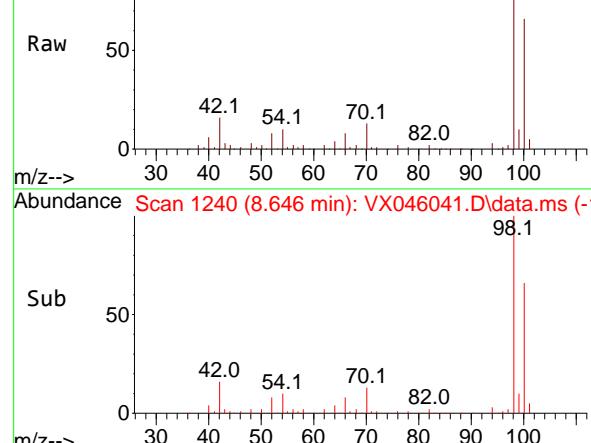

#49

1,4-Dioxane

Concen: 282.442 ug/l

RT: 7.659 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#50

Toluene-d8

Concen: 13.200 ug/l

RT: 8.646 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35


Tgt Ion: 98 Resp: 73333

Ion Ratio Lower Upper


98 100

100 64.8 53.5 80.3








Abundance Scan 1228 (8.573 min): VX046041.D\data.ms

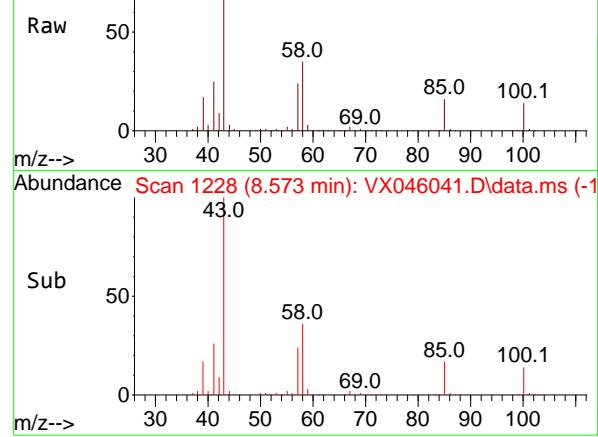


Abundance Scan 1228 (8.573 min): VX046041.D\data.ms (-1)

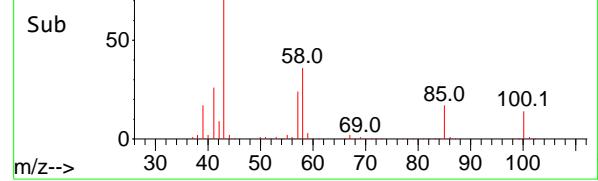

Abundance Scan 1251 (8.713 min): VX046041.D\data.ms

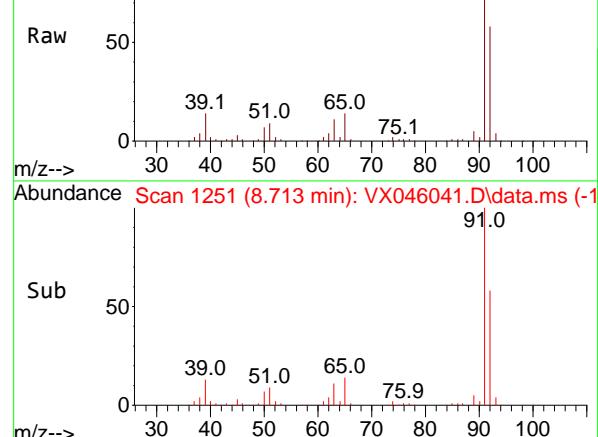

Abundance Scan 1251 (8.713 min): VX046041.D\data.ms (-1)

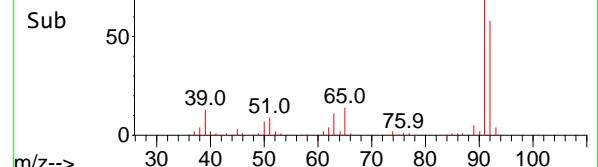

#51

4-Methyl-2-Pentanone

Concen: 75.775 ug/l

RT: 8.573 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:


MSVOA\_X

ClientSampleId :

VSTDICC020

Manual Integrations  
APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#52

Toluene

Concen: 14.788 ug/l

RT: 8.713 min Scan# 1251

Delta R.T. -0.000 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35




Tgt Ion: 92 Resp: 52030

Ion Ratio Lower Upper

92 100

91 172.2 136.6 205.0

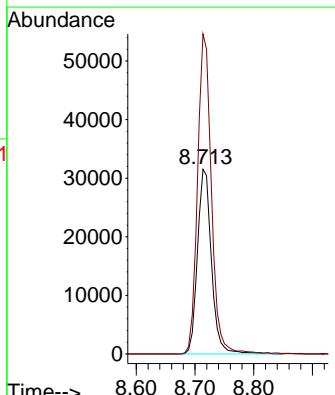



#53

t-1,3-Dichloropropene

Concen: 14.566 ug/l

RT: 8.976 min Scan# 1194

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

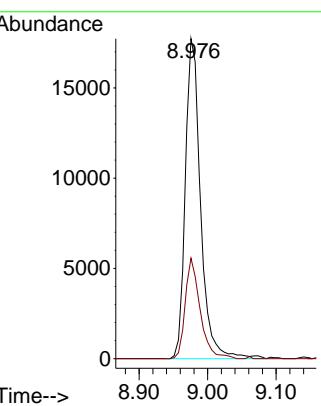

#54

cis-1,3-Dichloropropene

Concen: 14.154 ug/l


RT: 8.366 min Scan# 1194







Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt	Ion: 75	Resp: 31226
Ion Ratio	Lower	Upper
75	100	
77	30.8	25.4 38.0
39	64.0	52.2 78.4

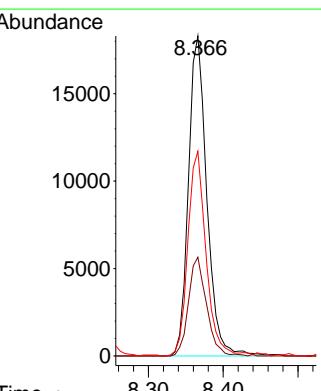



#55

1,1,2-Trichloroethane

Concen: 14.442 ug/l

RT: 9.152 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X

ClientSampleId :


VSTDICC020

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

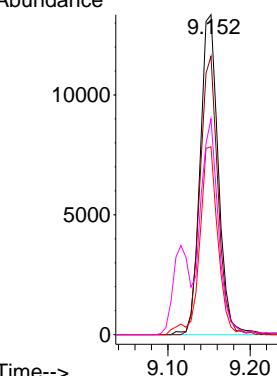

#56

Ethyl methacrylate

Concen: 14.425 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion: 69 Resp: 31787


Ion Ratio Lower Upper


69 100

41 78.2 60.8 91.2

39 49.3 39.0 58.6

Abundance

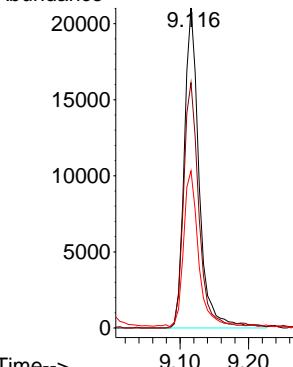

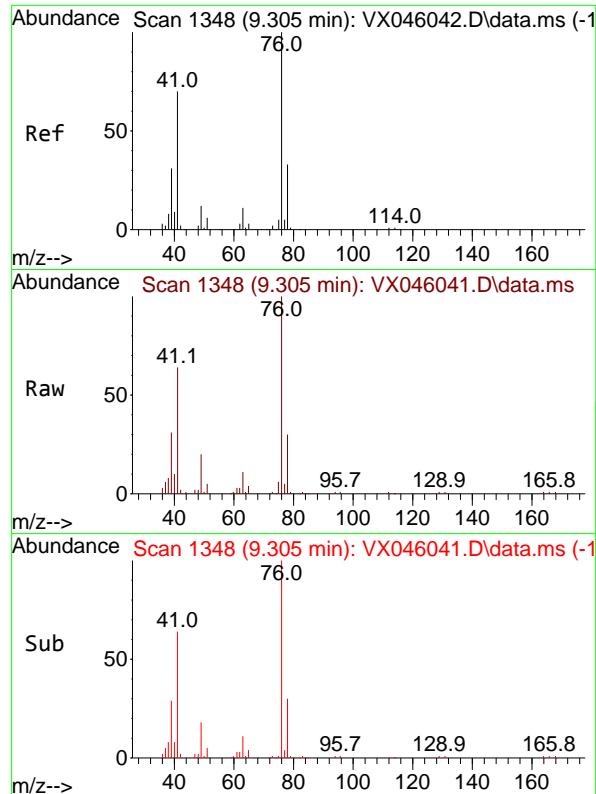

#57

1,3-Dichloropropane

Concen: 14.417 ug/l

RT: 9.305 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

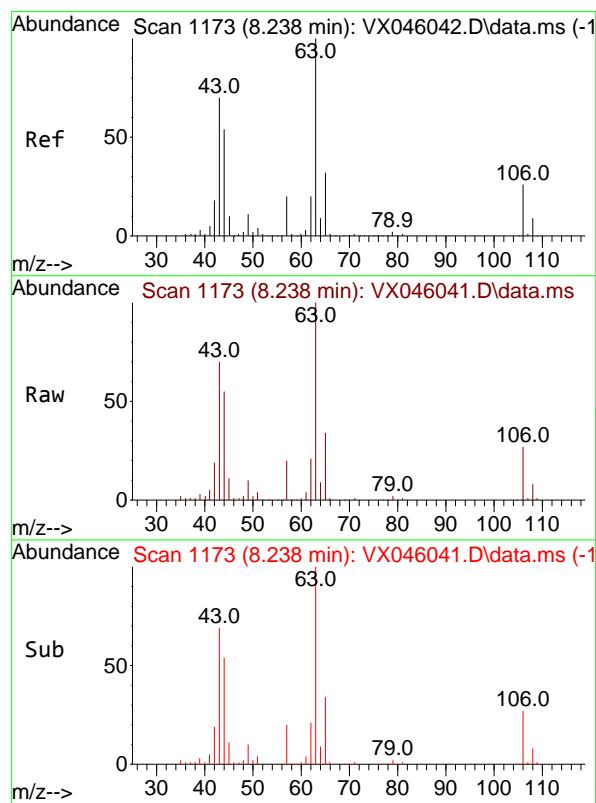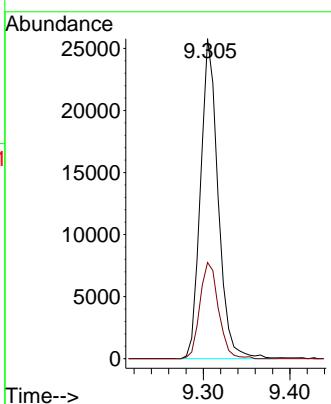

#58

2-Chloroethyl Vinyl ether

Concen: 80.312 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. -0.000 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35







Tgt Ion: 63 Resp: 79531

Ion Ratio Lower Upper

63 100

106 26.7 21.5 32.3

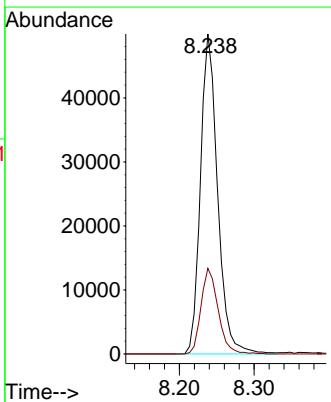

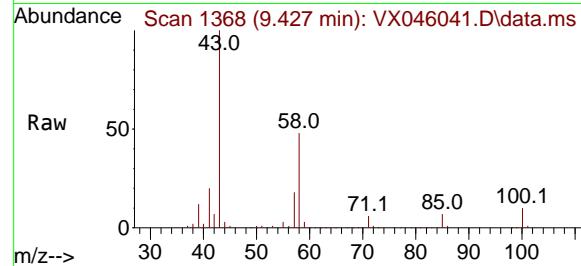

#59

2-Hexanone

Concen: 74.997 ug/l

RT: 9.427 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

Manual Integrations  
APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#60

Dibromochloromethane

Concen: 14.387 ug/l

RT: 9.518 min Scan# 1383

Delta R.T. -0.000 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35




Tgt Ion:129 Resp: 22267

Ion Ratio Lower Upper

129 100

127 78.0 39.3 117.8



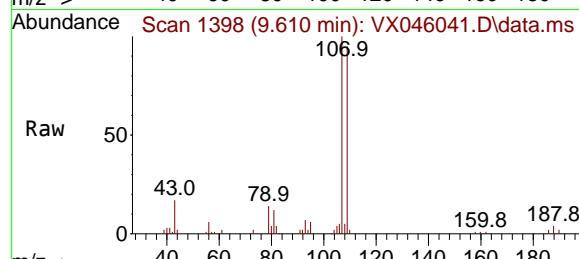

#61

1,2-Dibromoethane

Concen: 14.458 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

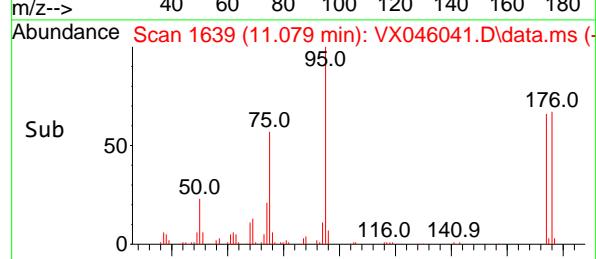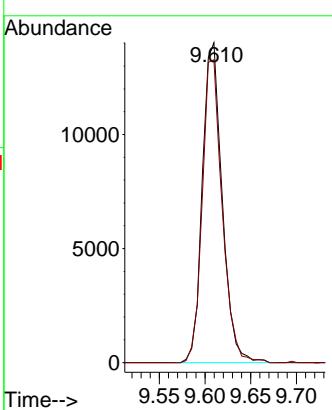

#62

4-Bromofluorobenzene

Concen: 13.236 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion: 95 Resp: 26760


Ion Ratio Lower Upper

95 100

174 67.4 0.0 135.8

176 67.0 0.0 131.4

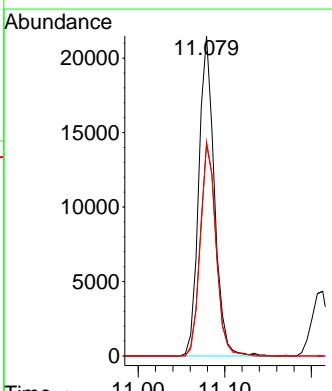

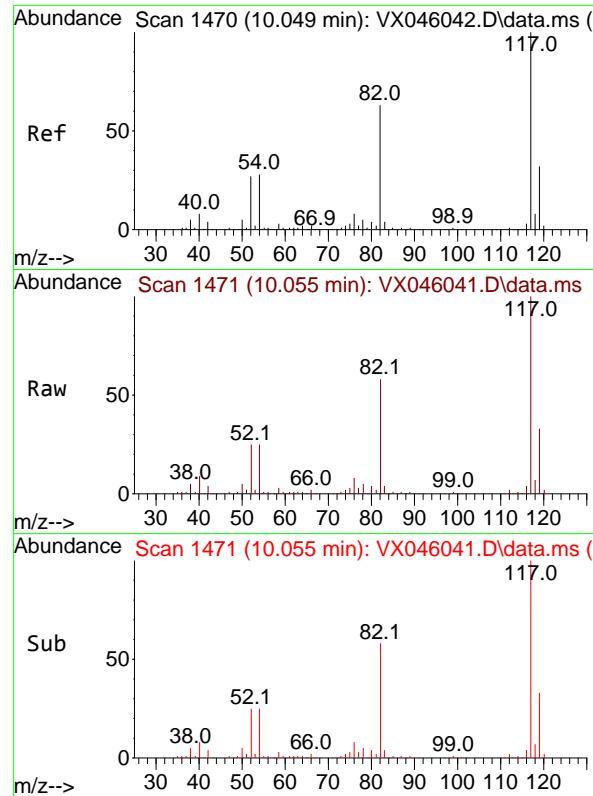

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1470

Delta R.T. 0.006 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

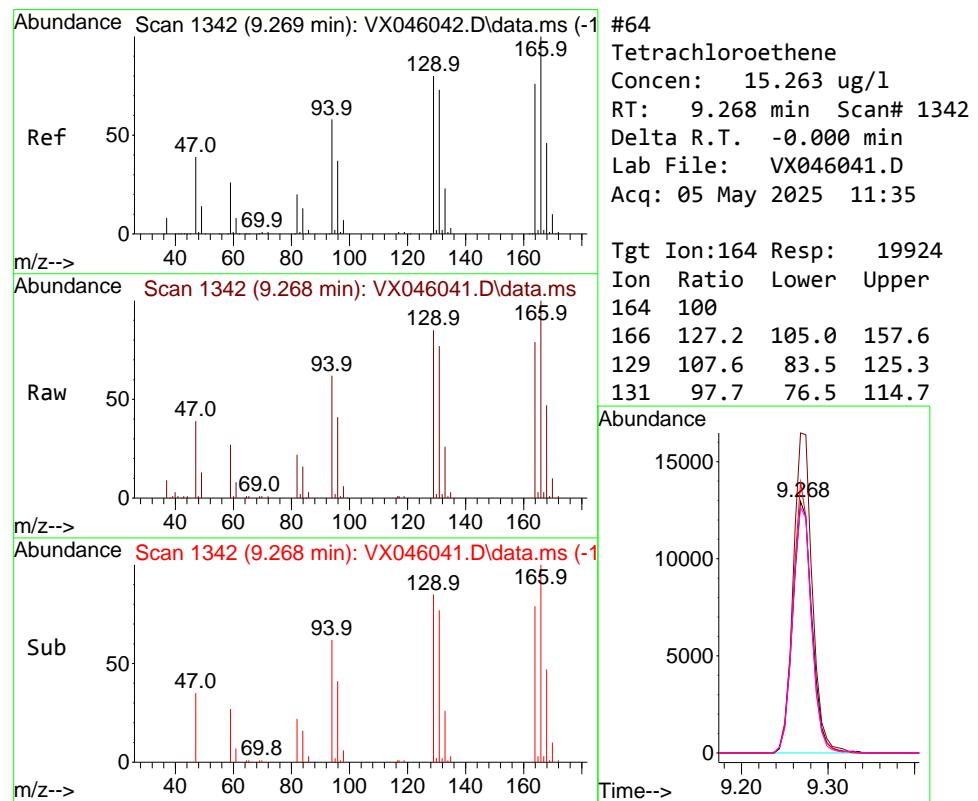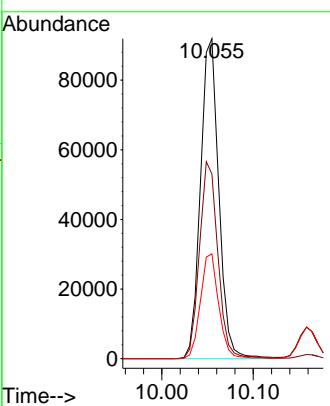

#64

Tetrachloroethene


Concen: 15.263 ug/l


RT: 9.268 min Scan# 1342

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

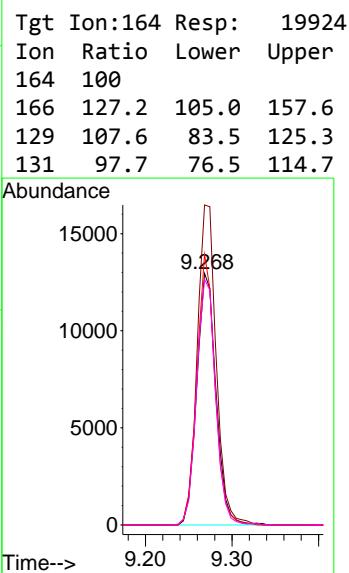

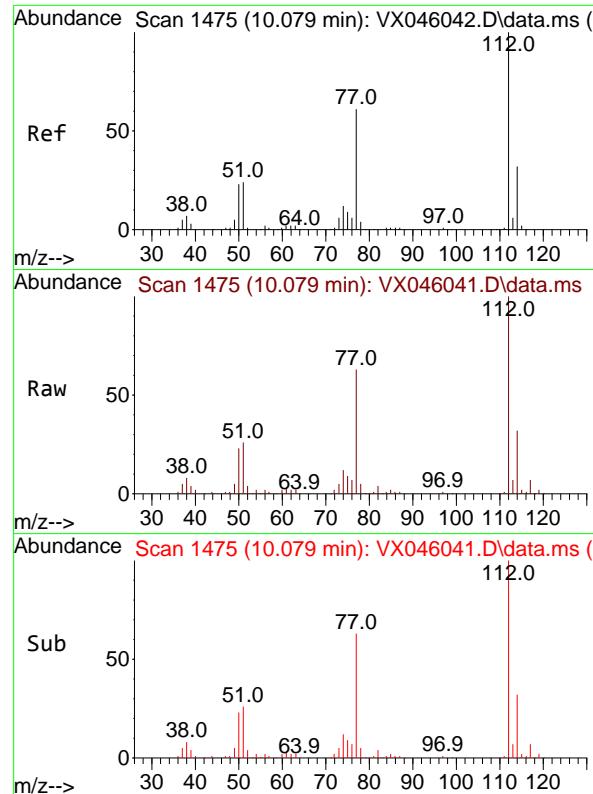

#65

Chlorobenzene

Concen: 14.202 ug/l

RT: 10.079 min Scan# 1475

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

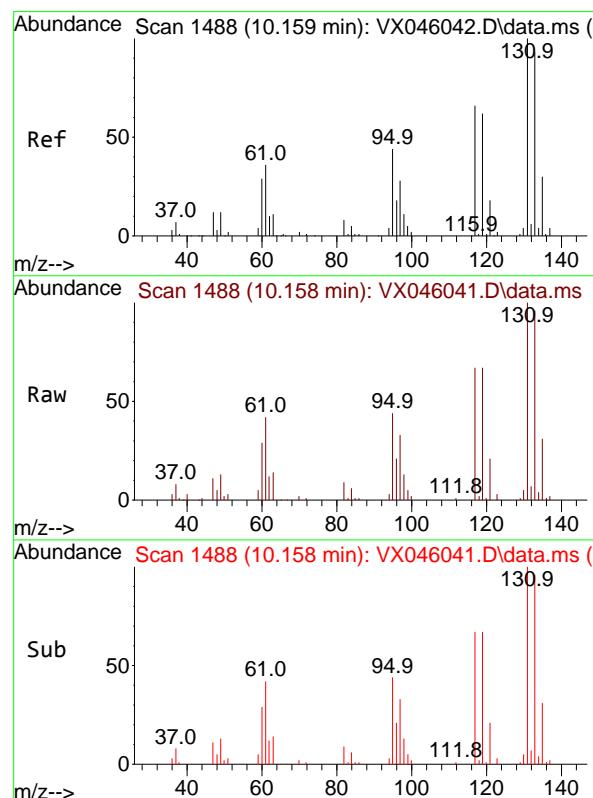

#66

1,1,1,2-Tetrachloroethane

Concen: 14.231 ug/l

RT: 10.158 min Scan# 1488

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion:131 Resp: 18671




Ion Ratio Lower Upper

131 100

133 94.5 47.3 141.9

119 66.7 31.6 95.0

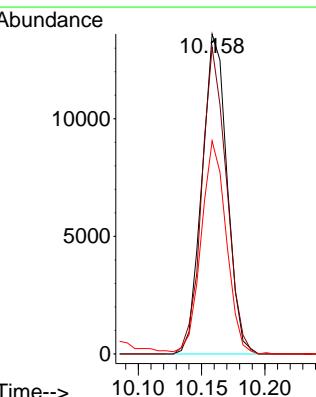



#67

Ethyl Benzene

Concen: 14.631 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#68

m/p-Xylenes

Concen: 29.806 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX046041.D



Acq: 05 May 2025 11:35

Tgt Ion:106 Resp: 72202


Ion Ratio Lower Upper

106 100

91 216.1 171.2 256.8

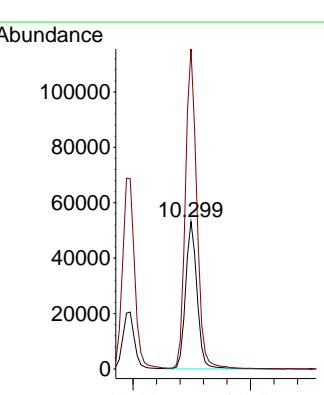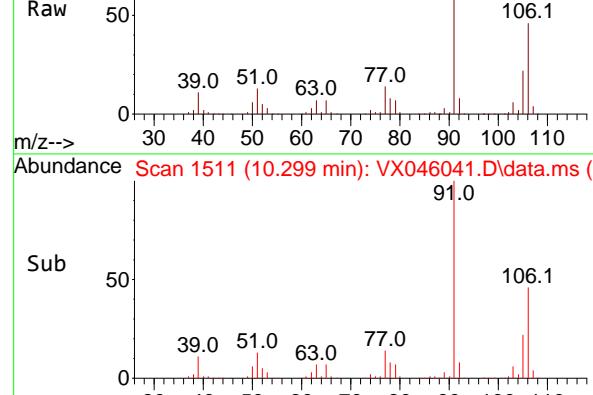

Time--&gt; 10.10 10.20 10.30 10.40


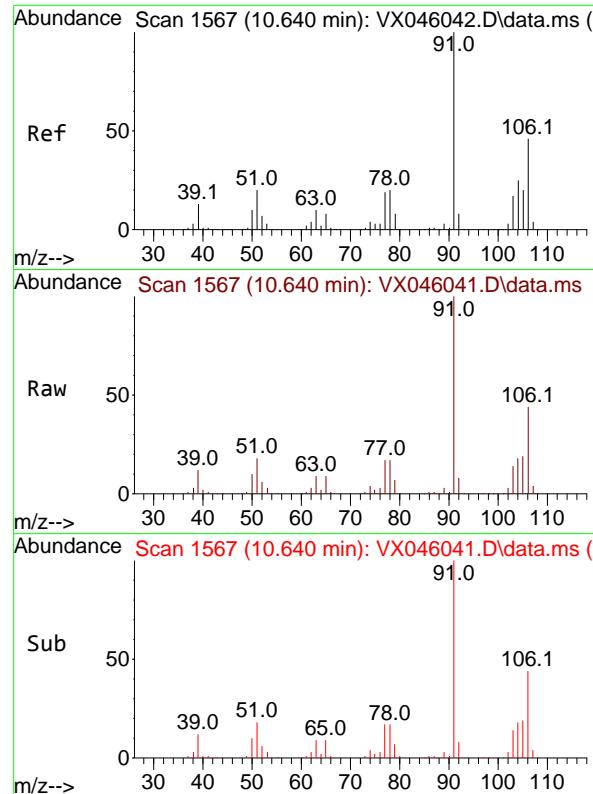


#69  
o-Xylene  
Concen: 14.408 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35  
ClientSampleId : VSTDICC020

Tgt Ion:106 Resp: 35173  
Ion Ratio Lower Upper  
106 100  
91 231.7 112.7 338.1


### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

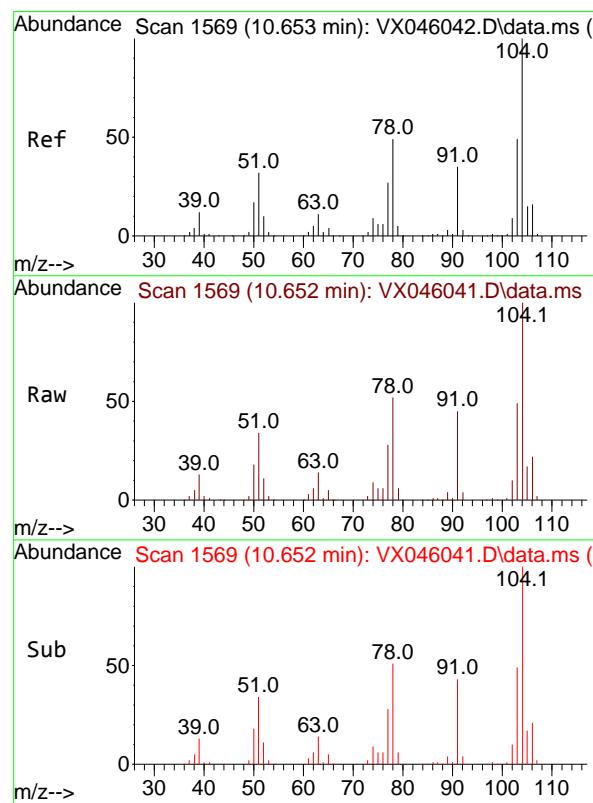

#70  
Styrene  
Concen: 14.853 ug/l  
RT: 10.652 min Scan# 1569  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion:104 Resp: 58034  
Ion Ratio Lower Upper  
104 100  
78 58.7 45.7 68.5  
103 55.6 43.7 65.5





#71

Bromoform

Concen: 14.030 ug/l

RT: 10.799 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion:152 Resp: 60503

Ion Ratio Lower Upper


152 100


115 76.6 46.9 140.7

150 163.6 0.0 351.0

Time--&gt;

Time--&gt;

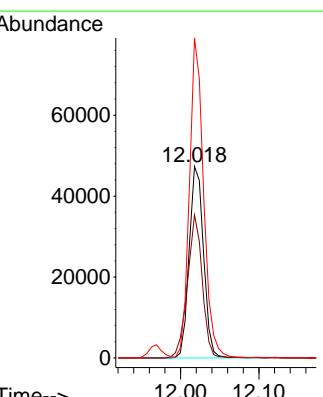

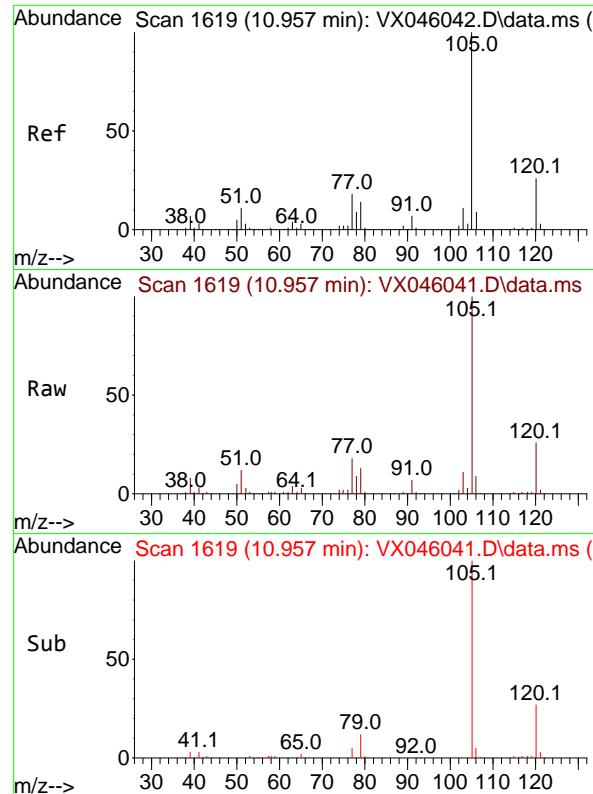

#73

Isopropylbenzene

Concen: 14.096 ug/l

RT: 10.957 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

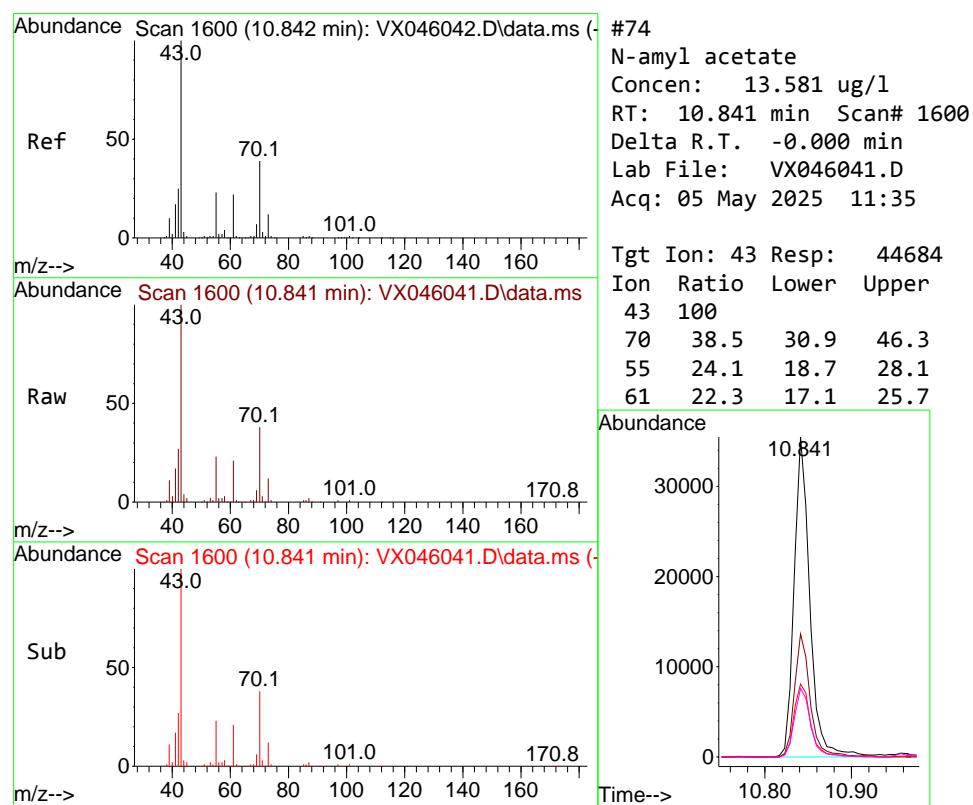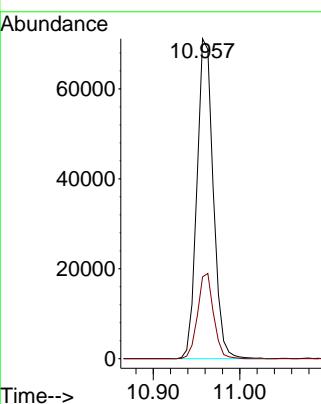

#74

N-amyl acetate

Concen: 13.581 ug/l

RT: 10.841 min Scan# 1600

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion: 43 Resp: 44684


Ion Ratio Lower Upper


43 100

70 38.5 30.9 46.3

55 24.1 18.7 28.1

61 22.3 17.1 25.7

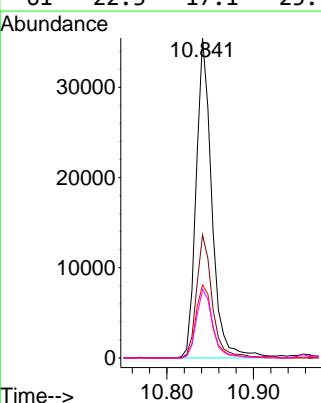

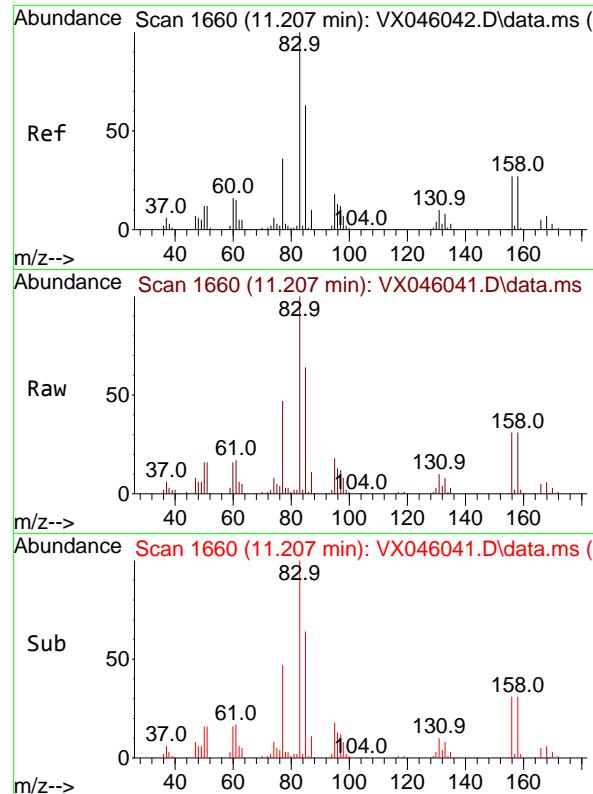


#75  
1,1,2,2-Tetrachloroethane  
Concen: 13.560 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

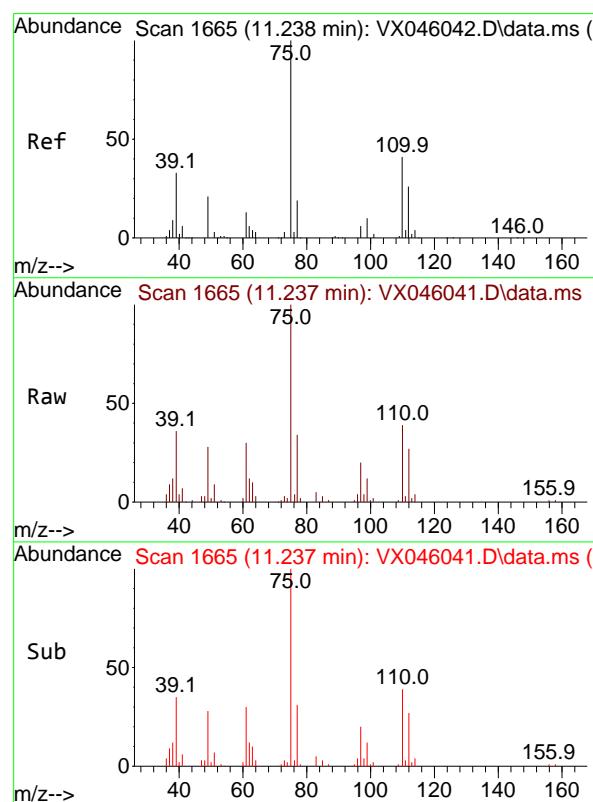

#76  
1,2,3-Trichloropropane  
Concen: 11.039 ug/l  
RT: 11.237 min Scan# 1665  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion: 75 Resp: 27845  
Ion Ratio Lower Upper  
75 100  
77 43.0 20.5 61.5

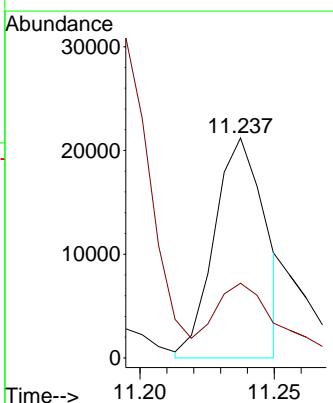

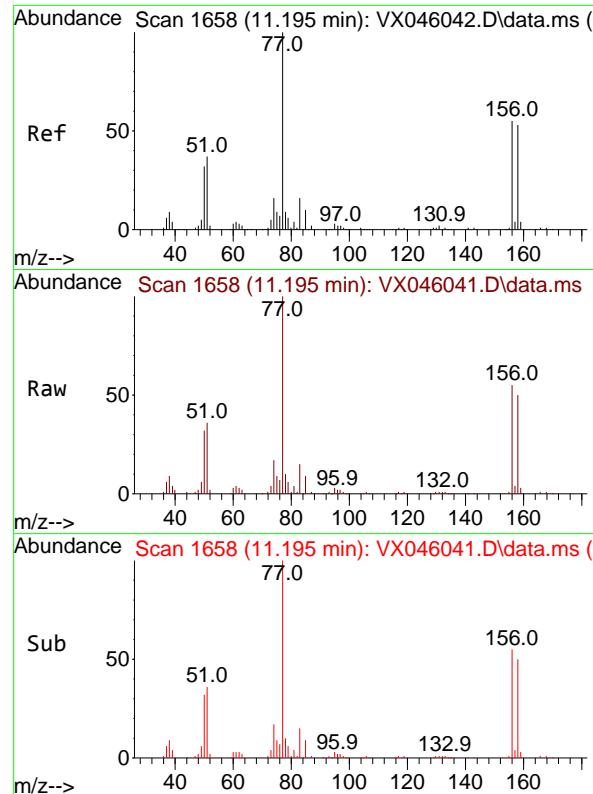

#77

Bromobenzene

Concen: 14.212 ug/l

RT: 11.195 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

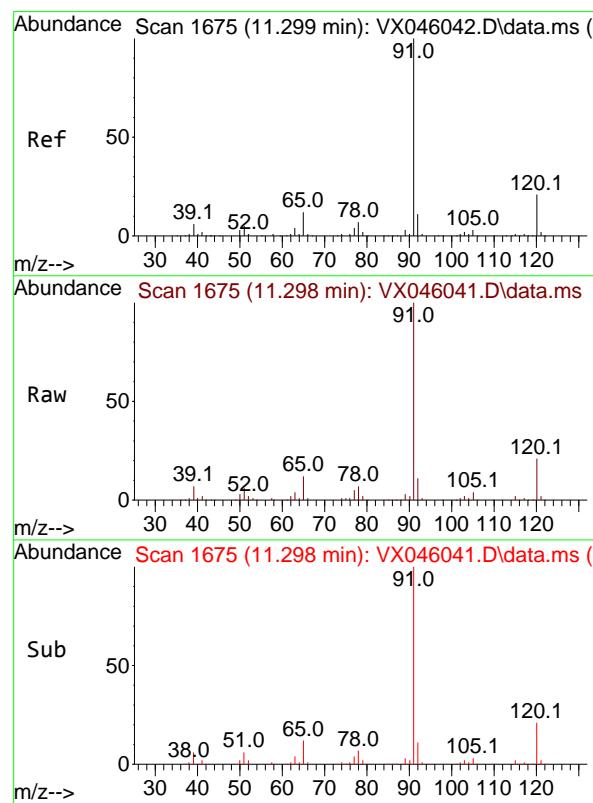

#78

n-propylbenzene

Concen: 14.376 ug/l

RT: 11.298 min Scan# 1675


Delta R.T. -0.000 min




Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion: 91 Resp: 106337

Ion Ratio	Lower	Upper
91	100	
120	22.0	10.8
		32.4



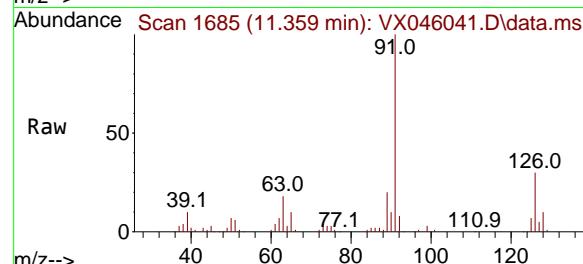

#79

2-Chlorotoluene

Concen: 13.748 ug/l

RT: 11.359 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#80

1,3,5-Trimethylbenzene

Concen: 14.468 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX046041.D


Acq: 05 May 2025 11:35

Tgt Ion:105 Resp: 79261

Ion Ratio Lower Upper

105 100

120 45.9 23.1 69.2

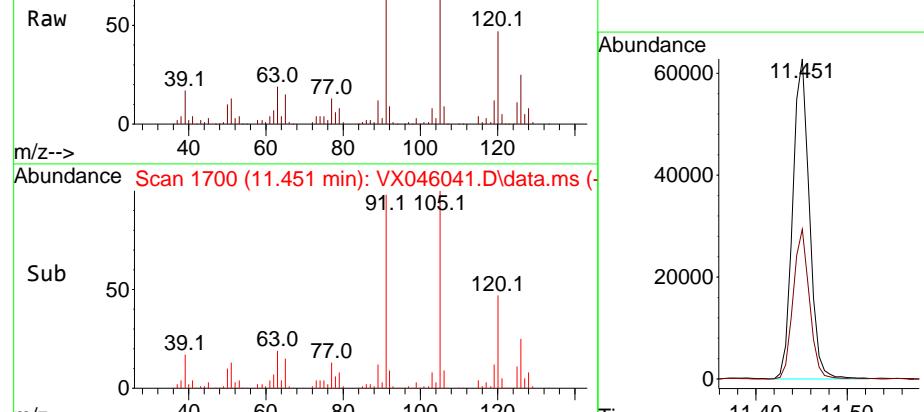

Abundance


60000 11.451

40000

20000

0

11.40 11.45 11.50


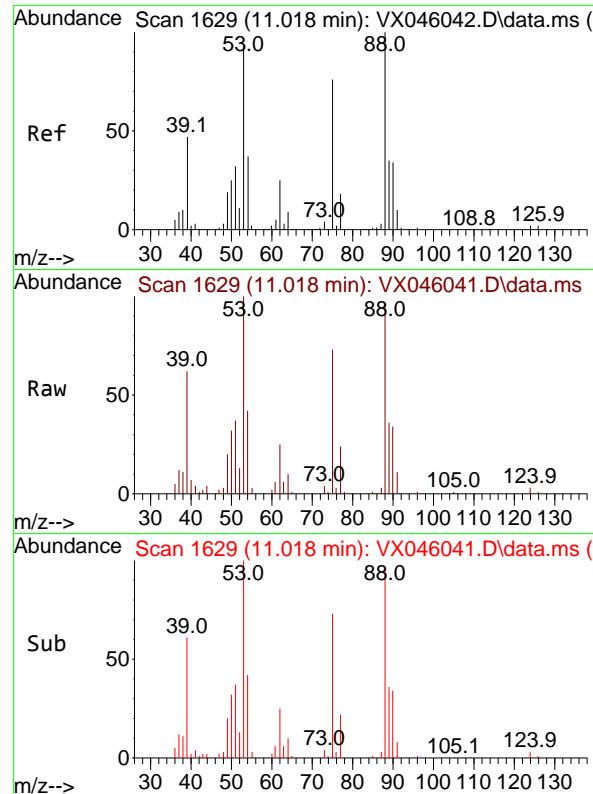


#81  
trans-1,4-Dichloro-2-butene  
Concen: 13.371 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carbone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

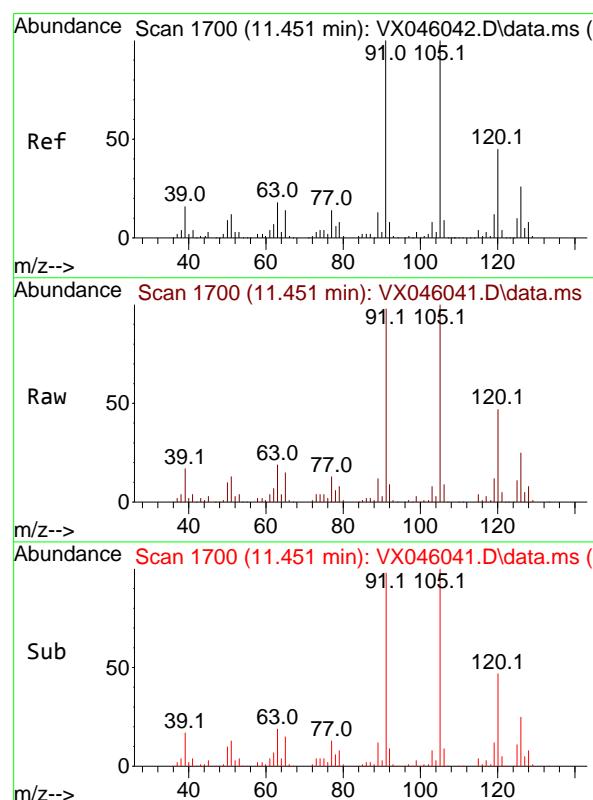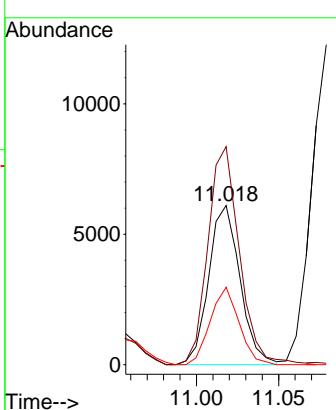

#82  
4-Chlorotoluene  
Concen: 14.116 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion: 91 Resp: 77338  
Ion Ratio Lower Upper  
91 100  
126 26.5 13.3 39.8

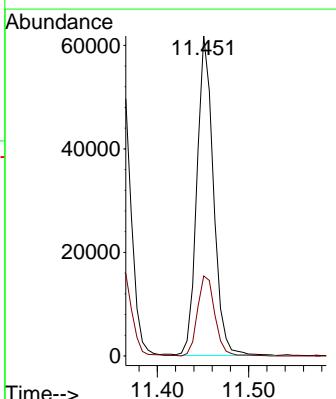



#83

tert-Butylbenzene

Concen: 14.011 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

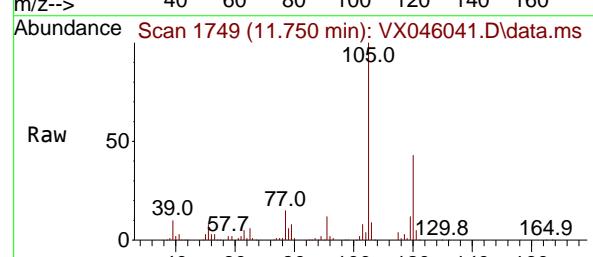

#84

1,2,4-Trimethylbenzene

Concen: 14.480 ug/l


RT: 11.750 min Scan# 1749




Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
105	100		79232		
120	42.0	21.2		63.6	

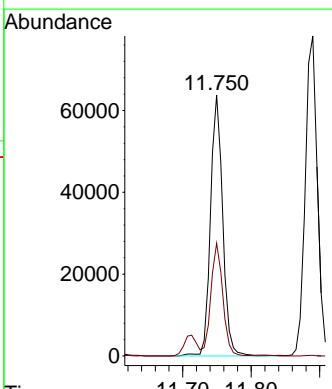



#85

sec-Butylbenzene

Concen: 14.263 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#86

p-Isopropyltoluene

Concen: 14.387 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35


Tgt Ion:119 Resp: 77599


Ion Ratio Lower Upper

119 100

134 25.9 12.5 37.5

91 28.8 13.8 41.4

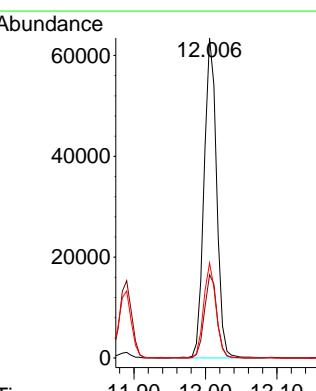

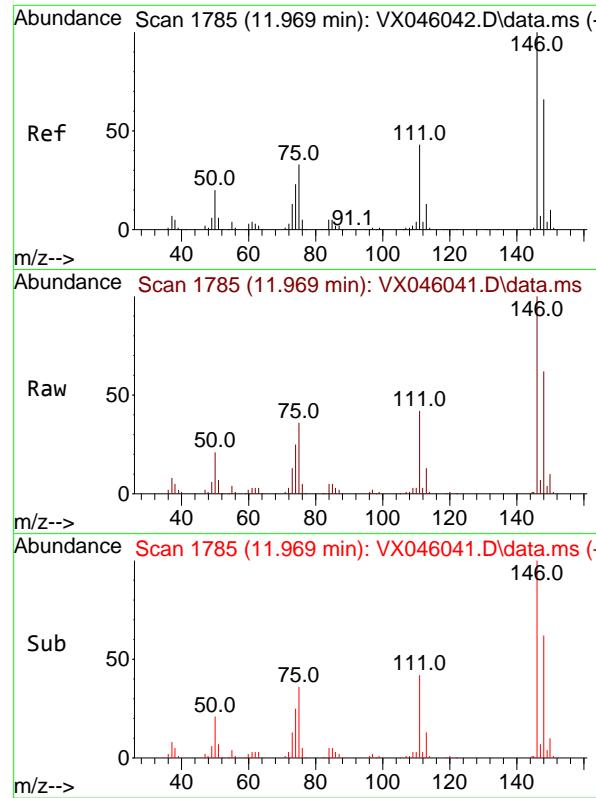

#87

1,3-Dichlorobenzene

Concen: 13.898 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC020

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

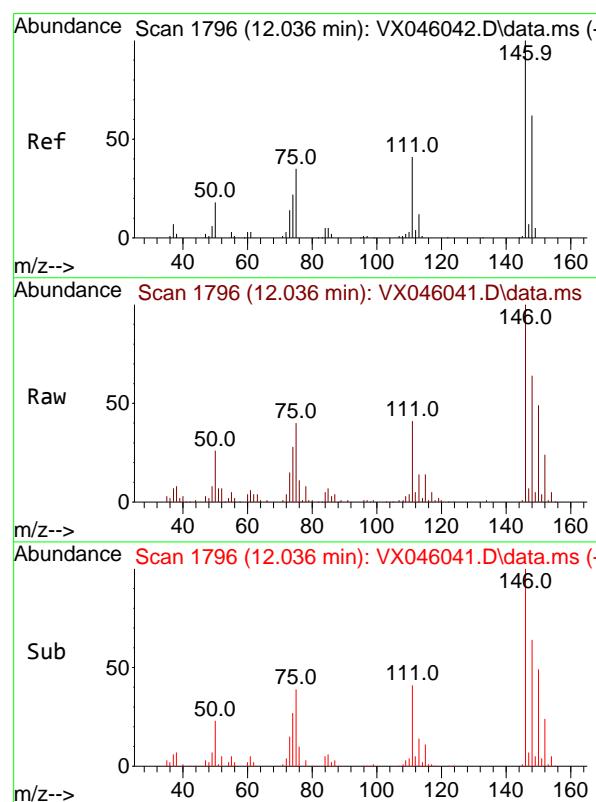

#88

1,4-Dichlorobenzene

Concen: 14.146 ug/l

RT: 12.036 min Scan# 1796

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Tgt Ion:146 Resp: 39419

Ion Ratio Lower Upper

146 100

111 42.8 21.3 63.9

148 64.2 31.9 95.5

Abundance


30000 12.036

20000

10000

0

Time--&gt;

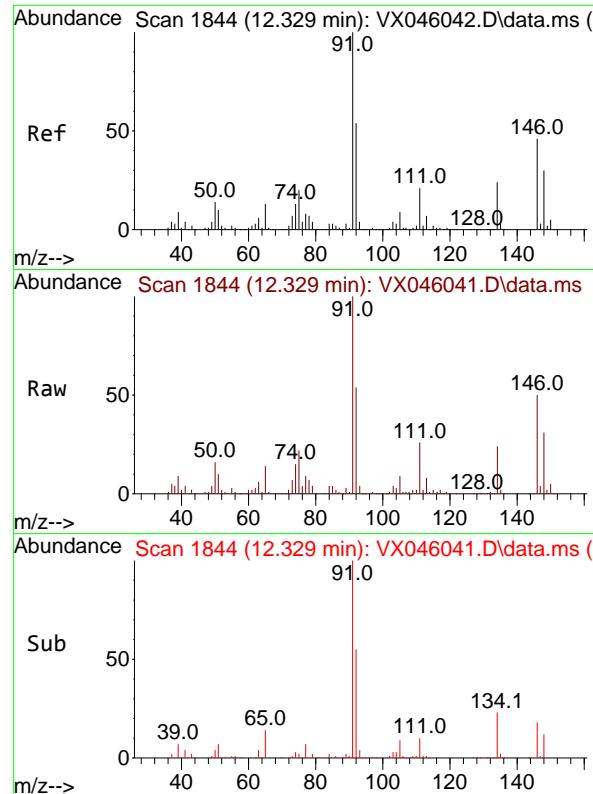

#89

n-Butylbenzene

Concen: 14.184 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX046041.D

Acq: 05 May 2025 11:35

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC020

**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025


Supervised By :Mahesh Dadoda 05/06/2025

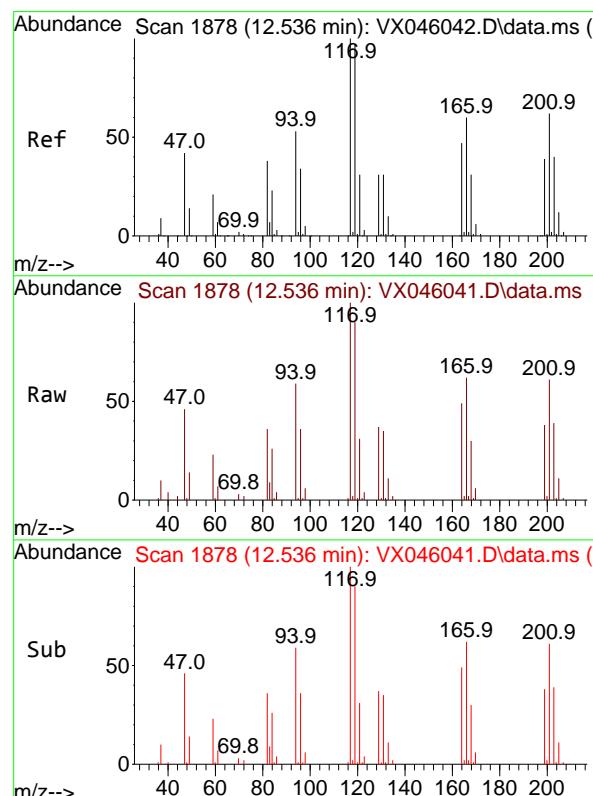

#90  
Hexachloroethane  
Concen: 13.287 ug/l  
RT: 12.536 min Scan# 1878  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion:117 Resp: 13332  
Ion Ratio Lower Upper  
117 100  
201 62.9 31.6 94.7




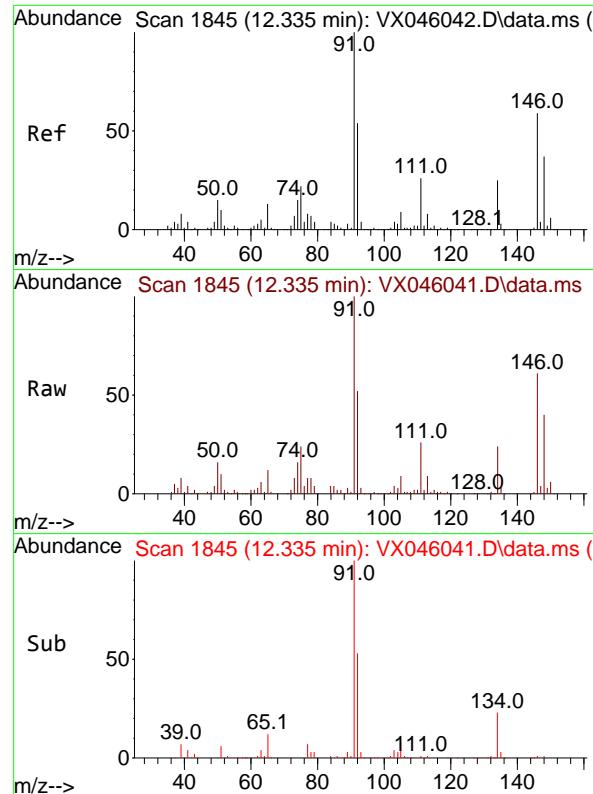


#91  
1,2-Dichlorobenzene  
Concen: 14.092 ug/l  
RT: 12.335 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

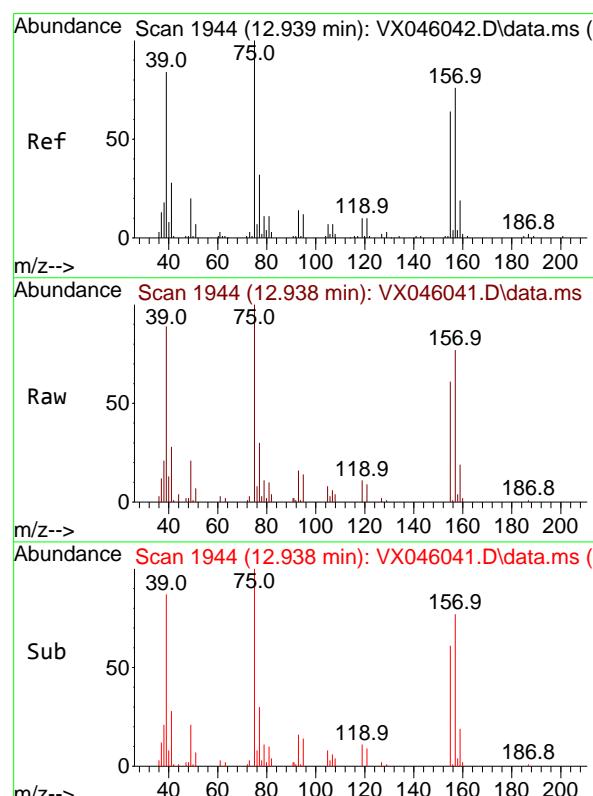

#92  
1,2-Dibromo-3-Chloropropane  
Concen: 13.535 ug/l  
RT: 12.938 min Scan# 1944  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion: 75 Resp: 7232  
Ion Ratio Lower Upper  
75 100  
155 69.4 34.9 104.8  
157 88.4 43.8 131.4





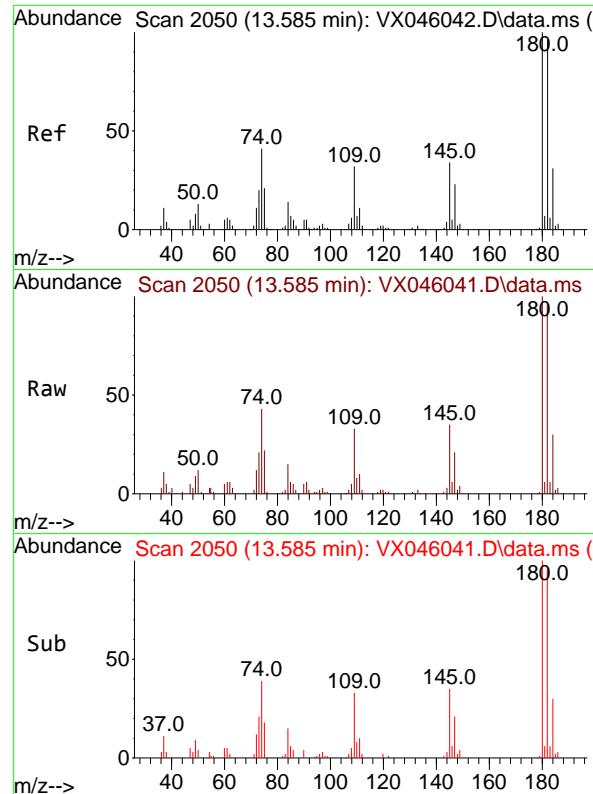

#93  
1,2,4-Trichlorobenzene  
Concen: 13.745 ug/l  
RT: 13.585 min Scan# 2  
Instrument: MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

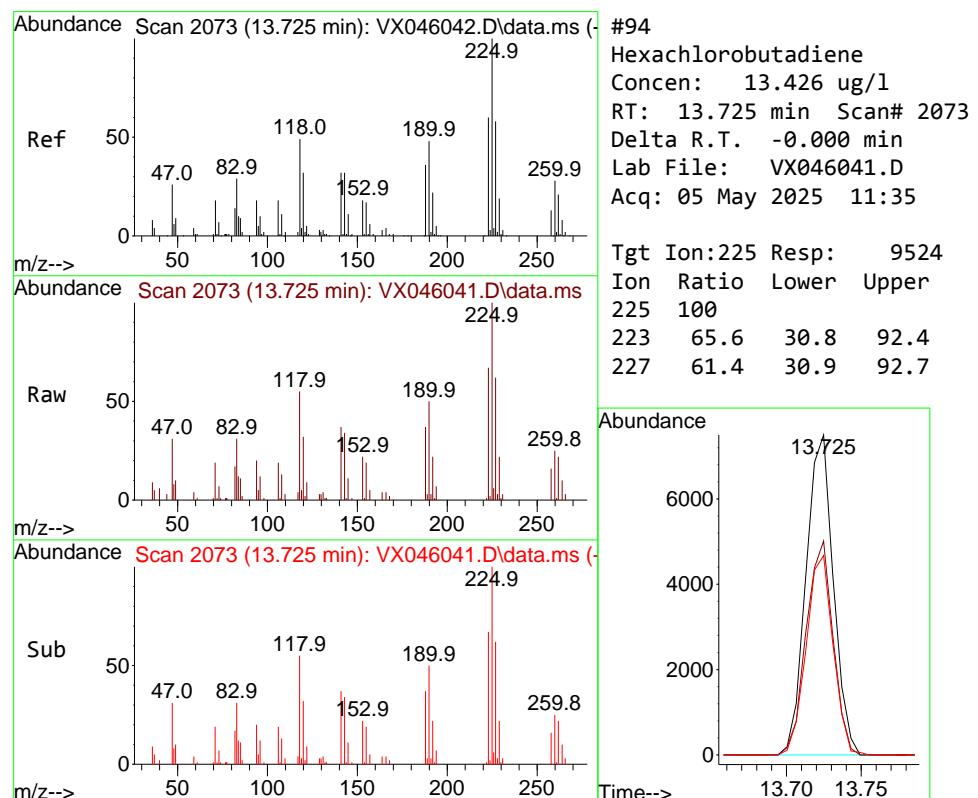

#94  
Hexachlorobutadiene  
Concen: 13.426 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion:225 Resp: 9524  
Ion Ratio Lower Upper  
225 100  
223 65.6 30.8 92.4  
227 61.4 30.9 92.7




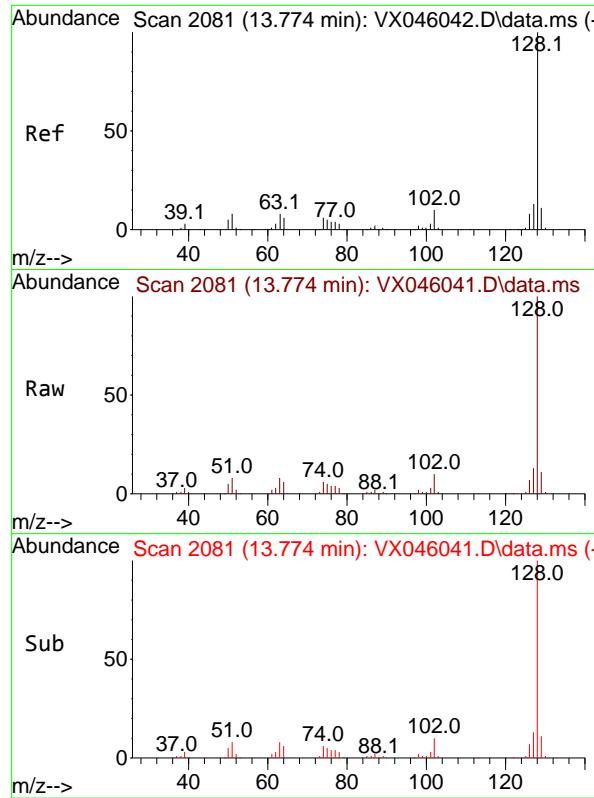


#95  
Naphthalene  
Concen: 14.040 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC020


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

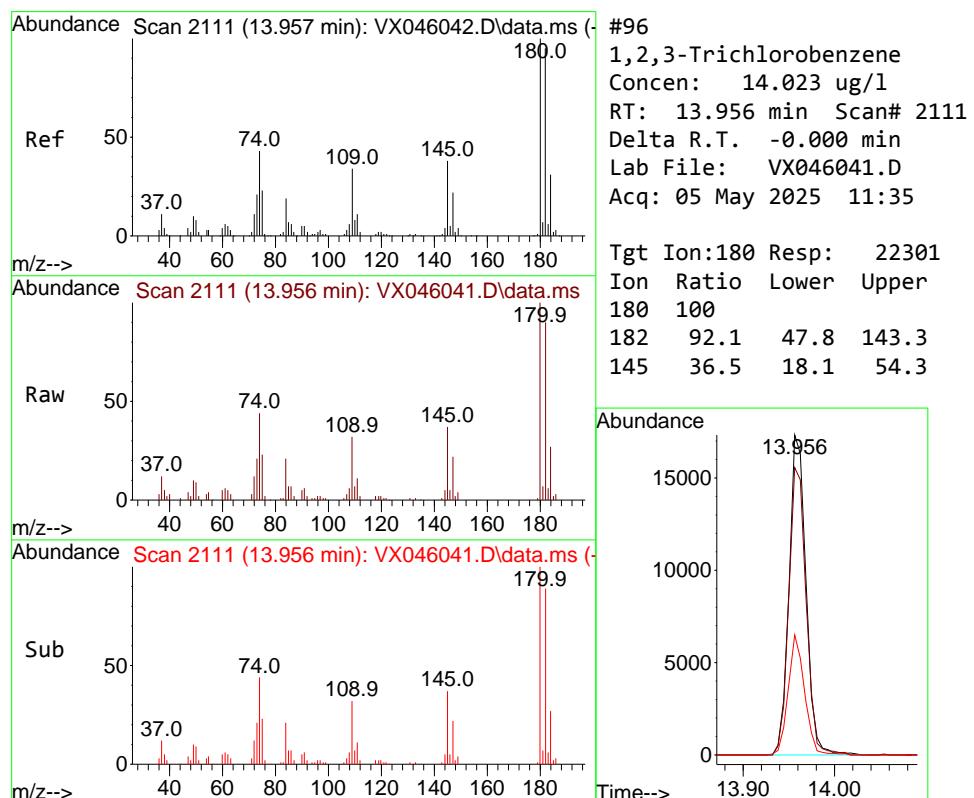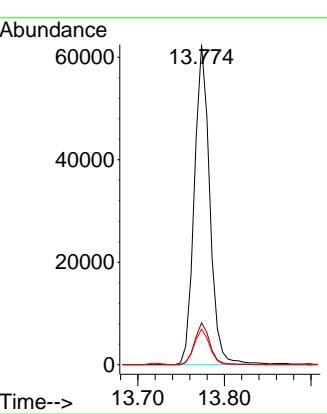

#96  
1,2,3-Trichlorobenzene  
Concen: 14.023 ug/l  
RT: 13.956 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046041.D  
Acq: 05 May 2025 11:35

Tgt Ion:180 Resp: 22301  
Ion Ratio Lower Upper  
180 100  
182 92.1 47.8 143.3  
145 36.5 18.1 54.3

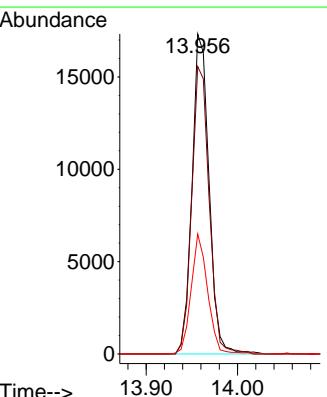

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046042.D  
 Acq On : 05 May 2025 11:58  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICCC050

Quant Time: May 06 06:09:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	97076	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	167947	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	146257	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	67976	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	88371	30.601	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 61.200%#			
35) Dibromofluoromethane	5.379	113	59550	31.633	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 63.260%#			
50) Toluene-d8	8.647	98	205479	32.395	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 64.780%#			
62) 4-Bromofluorobenzene	11.079	95	79012	34.229	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 68.460%#			
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	83826	39.120	ug/l	100
3) Chloromethane	1.307	50	75238	35.658	ug/l	100
4) Vinyl Chloride	1.374	62	68901	37.273	ug/l	100
5) Bromomethane	1.593	94	31648	33.765	ug/l	100
6) Chloroethane	1.666	64	36722	38.558	ug/l	100
7) Trichlorofluoromethane	1.874	101	103693	36.824	ug/l	100
8) Diethyl Ether	2.136	74	32724	35.350	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.319	101	62251	36.997	ug/l	100
10) Methyl Iodide	2.447	142	78277	39.622	ug/l	100
11) Tert butyl alcohol	2.977	59	62557	181.745	ug/l	100
12) 1,1-Dichloroethene	2.313	96	58334	35.610	ug/l	100
13) Acrolein	2.233	56	73927	184.907	ug/l	100
14) Allyl chloride	2.654	41	114445	36.971	ug/l	100
15) Acrylonitrile	3.062	53	188304	182.874	ug/l	100
16) Acetone	2.386	43	175777	177.910	ug/l	100
17) Carbon Disulfide	2.502	76	141281	37.223	ug/l	100
18) Methyl Acetate	2.703	43	82347	34.915	ug/l	100
19) Methyl tert-butyl Ether	3.111	73	209665	36.695	ug/l	100
20) Methylene Chloride	2.782	84	66412	33.182	ug/l	100
21) trans-1,2-Dichloroethene	3.087	96	59234	35.421	ug/l	100
22) Diisopropyl ether	3.757	45	221172	38.241	ug/l	100
23) Vinyl Acetate	3.721	43	994236	194.528	ug/l	100
24) 1,1-Dichloroethane	3.605	63	122601	36.067	ug/l	100
25) 2-Butanone	4.556	43	269224	188.783	ug/l	100
26) 2,2-Dichloropropane	4.465	77	92857	36.059	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	71518	35.466	ug/l	100
28) Bromochloromethane	4.898	49	56091	31.031	ug/l	100
29) Tetrahydrofuran	5.001	42	170124	183.679	ug/l	100
30) Chloroform	5.087	83	125850	35.626	ug/l	100
31) Cyclohexane	5.464	56	109459	38.205	ug/l	100
32) 1,1,1-Trichloroethane	5.373	97	109781	36.034	ug/l	100
36) 1,1-Dichloropropene	5.684	75	83215	38.073	ug/l	100
37) Ethyl Acetate	4.715	43	102537	37.394	ug/l	100
38) Carbon Tetrachloride	5.672	117	93712	37.320	ug/l	100
39) Methylcyclohexane	7.373	83	107651	39.307	ug/l	100
40) Benzene	6.031	78	247476	36.530	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046042.D  
 Acq On : 05 May 2025 11:58  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICCC050

Quant Time: May 06 06:09:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	58082	38.123	ug/1	100
42) 1,2-Dichloroethane	6.080	62	105332	37.605	ug/1	100
43) Isopropyl Acetate	6.336	43	161787	38.598	ug/1	100
44) Trichloroethene	7.123	130	59623	37.230	ug/1	100
45) 1,2-Dichloropropane	7.428	63	62387	37.064	ug/1	100
46) Dibromomethane	7.574	93	48201	36.326	ug/1	100
47) Bromodichloromethane	7.818	83	96916	37.685	ug/1	100
48) Methyl methacrylate	7.690	41	84277	39.157	ug/1	100
49) 1,4-Dioxane	7.659	88	30529	713.477	ug/1	100
51) 4-Methyl-2-Pentanone	8.574	43	532388	193.653	ug/1	100
52) Toluene	8.714	92	150757	37.530	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	88655	41.056	ug/1	100
54) cis-1,3-Dichloropropene	8.360	75	97031	38.521	ug/1	100
55) 1,1,2-Trichloroethane	9.147	97	59499	36.648	ug/1	100
56) Ethyl methacrylate	9.116	69	99947	39.726	ug/1	100
57) 1,3-Dichloropropane	9.305	76	104606	36.347	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	257678	227.902	ug/1	100
59) 2-Hexanone	9.427	43	396784	190.168	ug/1	100
60) Dibromochloromethane	9.519	129	67198	38.027	ug/1	100
61) 1,2-Dibromoethane	9.604	107	62633	37.567	ug/1	100
64) Tetrachloroethene	9.269	164	54853	36.726	ug/1	100
65) Chlorobenzene	10.079	112	160600	35.686	ug/1	100
66) 1,1,1,2-Tetrachloroethane	10.159	131	57066	38.017	ug/1	100
67) Ethyl Benzene	10.189	91	295712	38.543	ug/1	100
68) m/p-Xylenes	10.299	106	216578	78.142	ug/1	100
69) o-Xylene	10.640	106	106335	38.064	ug/1	100
70) Styrene	10.653	104	178313	39.888	ug/1	100
71) Bromoform	10.799	173	44486	39.457	ug/1 #	100
73) Isopropylbenzene	10.957	105	280719	37.865	ug/1	100
74) N-amyl acetate	10.842	43	140509	38.012	ug/1	100
75) 1,1,2,2-Tetrachloroethane	11.207	83	90975	34.495	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	80678m	28.468	ug/1	
77) Bromobenzene	11.195	156	63053	36.763	ug/1	100
78) n-propylbenzene	11.299	91	329981	39.707	ug/1	100
79) 2-Chlorotoluene	11.360	91	203509	36.336	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	237066	38.516	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	26179	38.445	ug/1	100
82) 4-Chlorotoluene	11.451	91	233172	37.880	ug/1	100
83) tert-Butylbenzene	11.713	119	233468	38.622	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	239433	38.946	ug/1	100
85) sec-Butylbenzene	11.890	105	291074	38.786	ug/1	100
86) p-Isopropyltoluene	12.006	119	241658	39.879	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	115651	36.199	ug/1	100
88) 1,4-Dichlorobenzene	12.036	146	115097	36.763	ug/1	100
89) n-Butylbenzene	12.329	91	213899	40.603	ug/1	100
90) Hexachloroethane	12.536	117	42314	37.534	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	115286	37.047	ug/1	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	21909	36.496	ug/1	100
93) 1,2,4-Trichlorobenzene	13.585	180	66655	39.117	ug/1	100
94) Hexachlorobutadiene	13.725	225	29007	36.395	ug/1	100
95) Naphthalene	13.774	128	245568	39.575	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	69262	38.765	ug/1	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046042.D  
 Acq On : 05 May 2025 11:58  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDICCC050**

Quant Time: May 06 06:09:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046042.D  
 Acq On : 05 May 2025 11:58  
 Operator : JC/MD  
 Sample : VSTDICCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 6 Sample Multiplier: 1




Quant Time: May 06 06:09:42 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

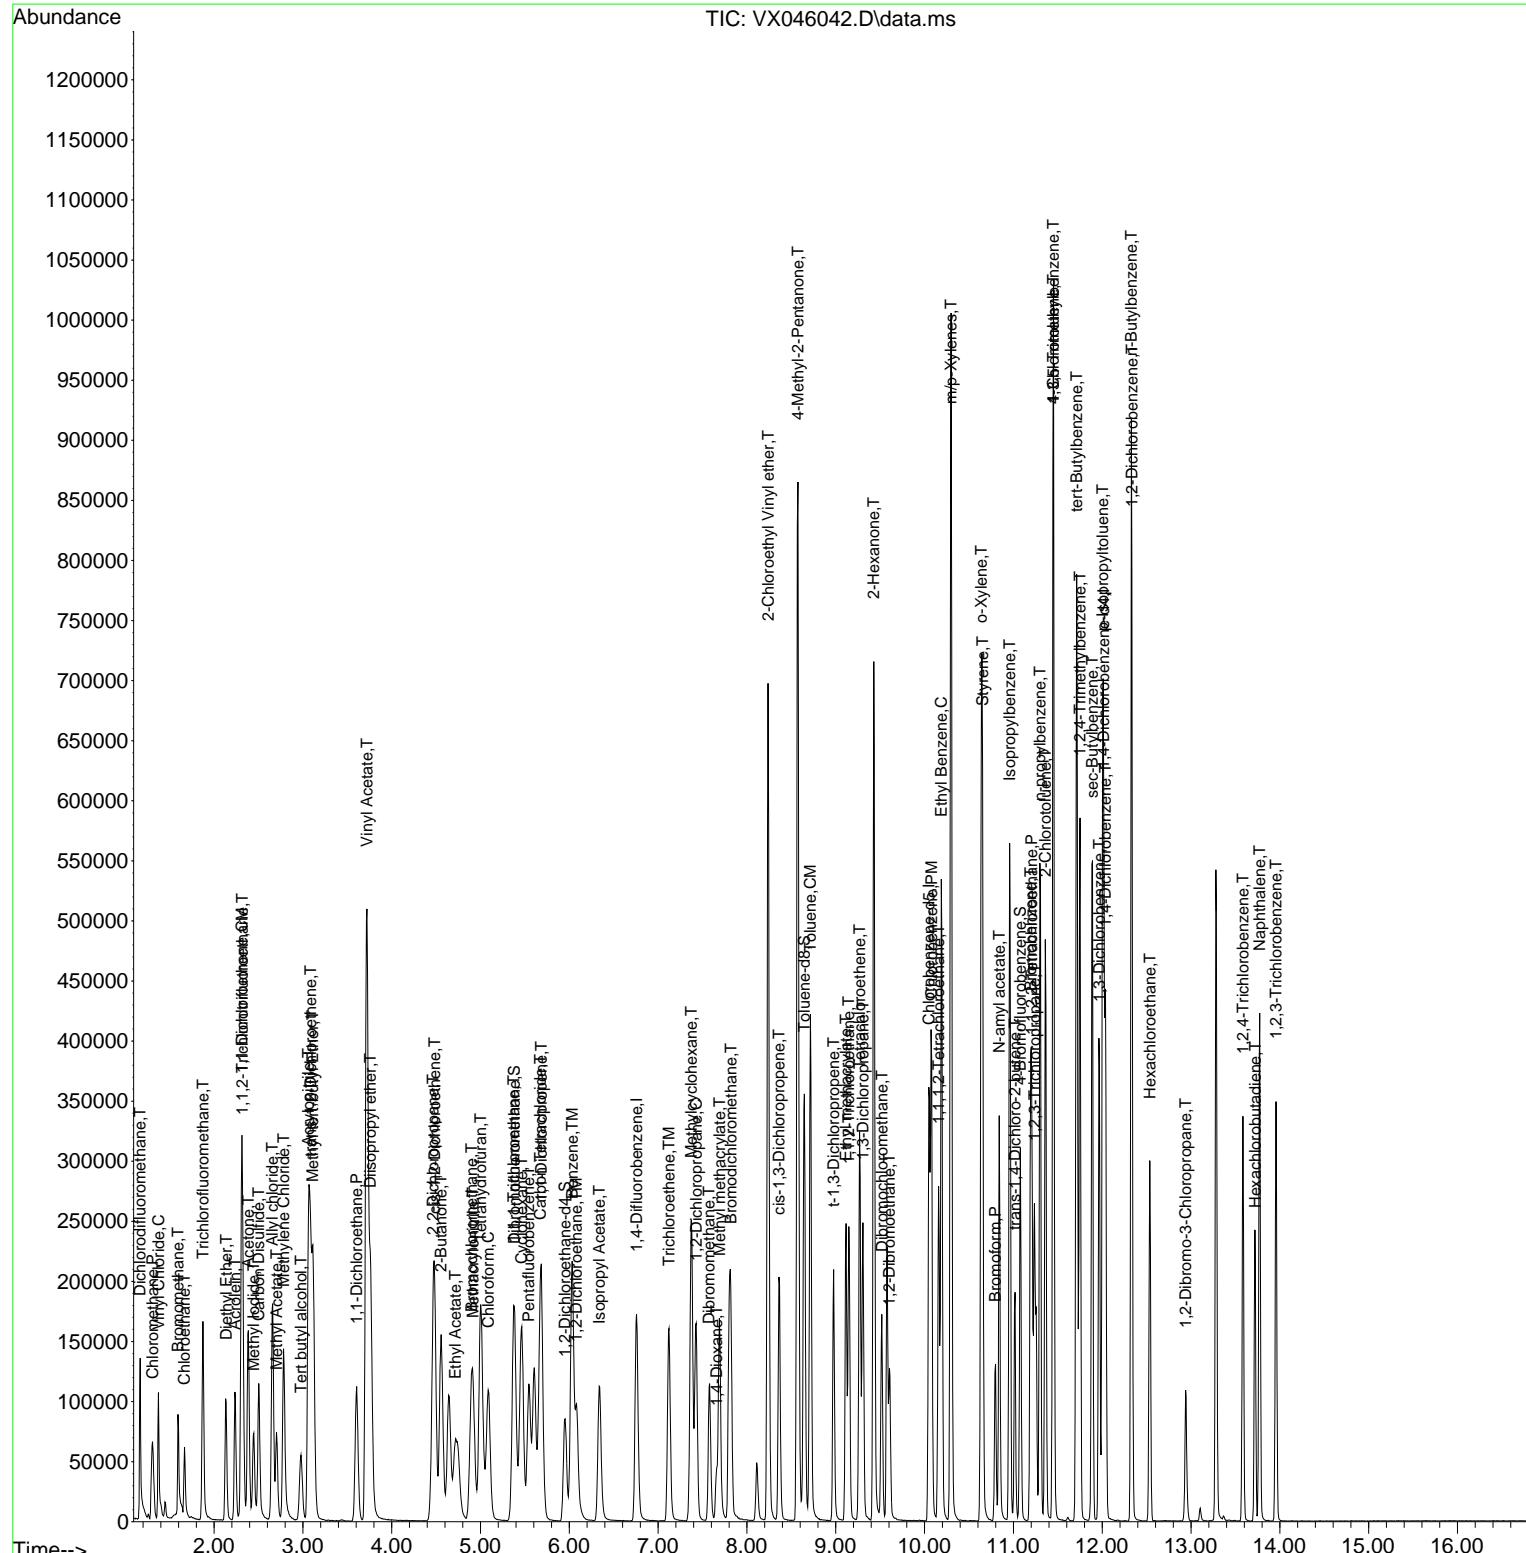



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.544 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

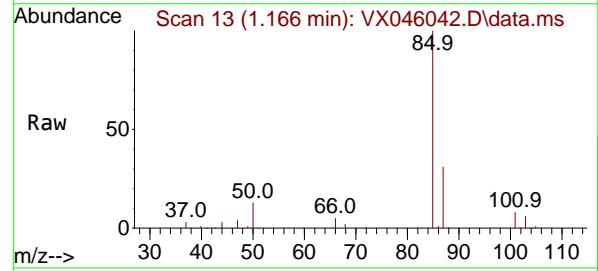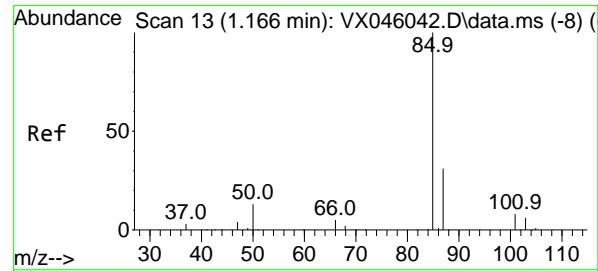

#2

Dichlorodifluoromethane

Concen: 39.120 ug/l

RT: 1.166 min Scan# 13

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion: 85 Resp: 83826



Ion Ratio Lower Upper

85 100

87 31.4 15.7 47.1

Abundance

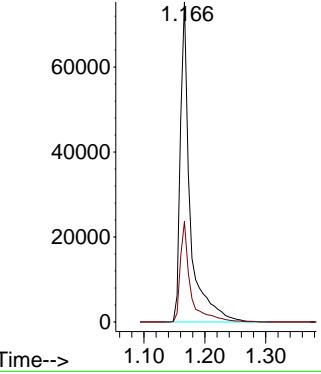


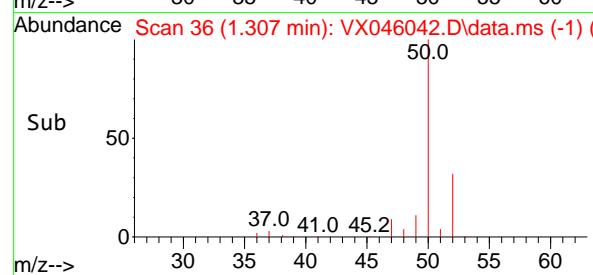



#3  
Chloromethane  
Concen: 35.658 ug/l  
RT: 1.307 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

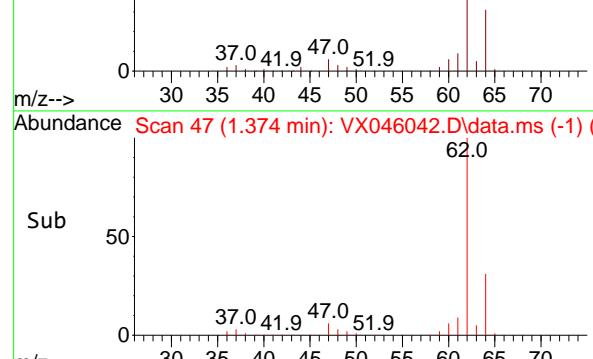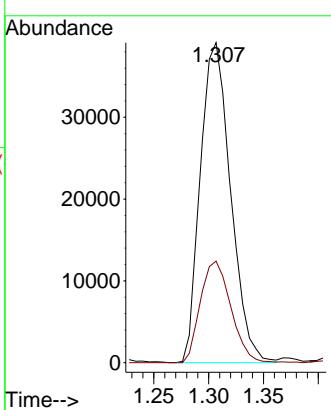

#4  
Vinyl Chloride  
Concen: 37.273 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 62 Resp: 68901  
Ion Ratio Lower Upper  
62 100  
64 31.5 25.2 37.8

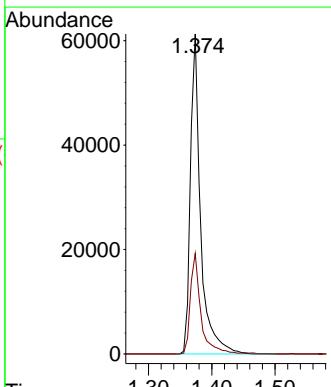



#5

Bromomethane

Concen: 33.765 ug/l

RT: 1.593 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#6

Chloroethane

Concen: 38.558 ug/l

RT: 1.666 min Scan# 95

Delta R.T. 0.000 min

Lab File: VX046042.D



Acq: 05 May 2025 11:58


Tgt Ion: 64 Resp: 36722

Ion Ratio Lower Upper

64 100

66 30.4 24.3 36.5

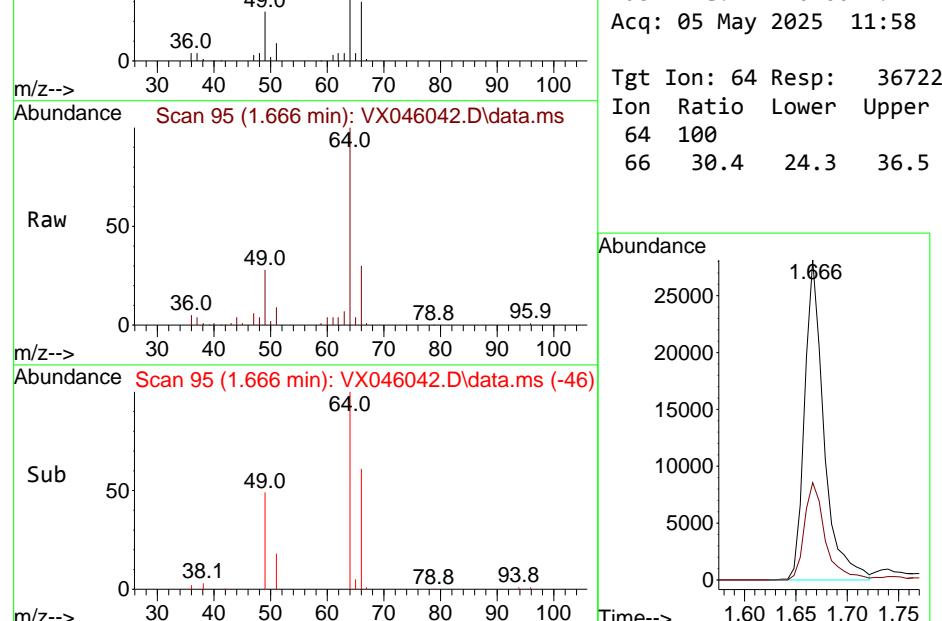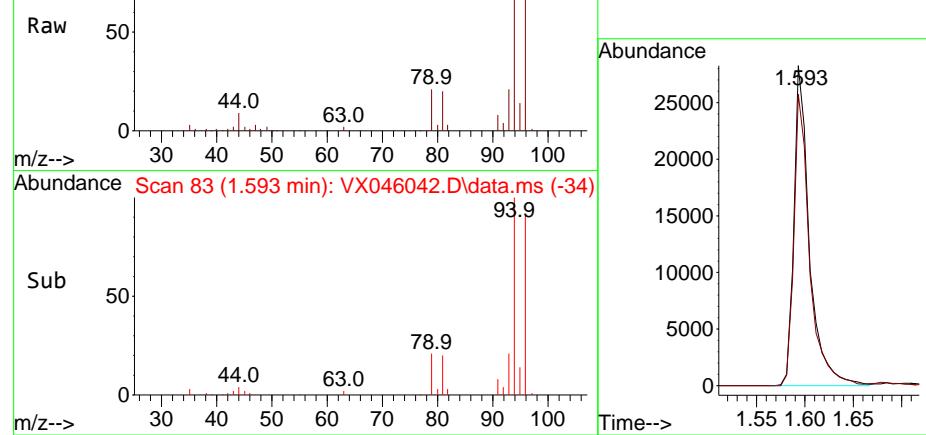


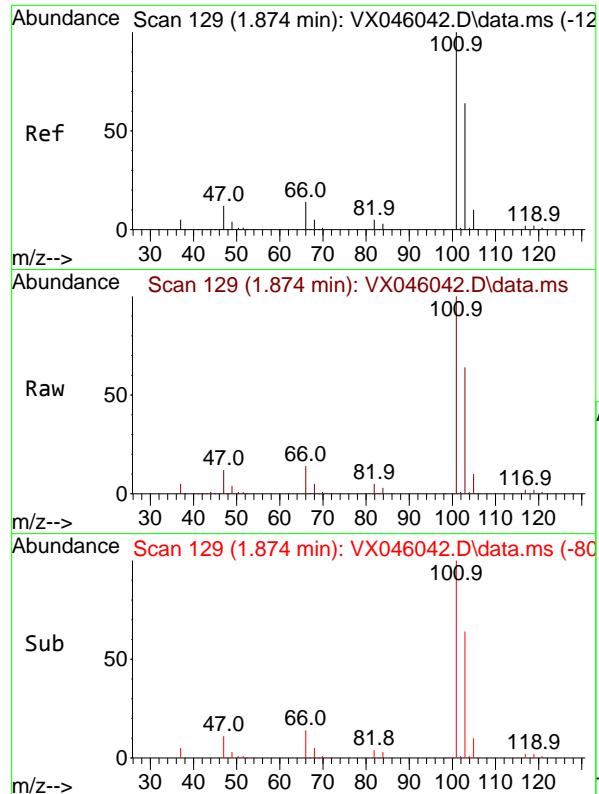


#7  
Trichlorofluoromethane  
Concen: 36.824 ug/l  
RT: 1.874 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

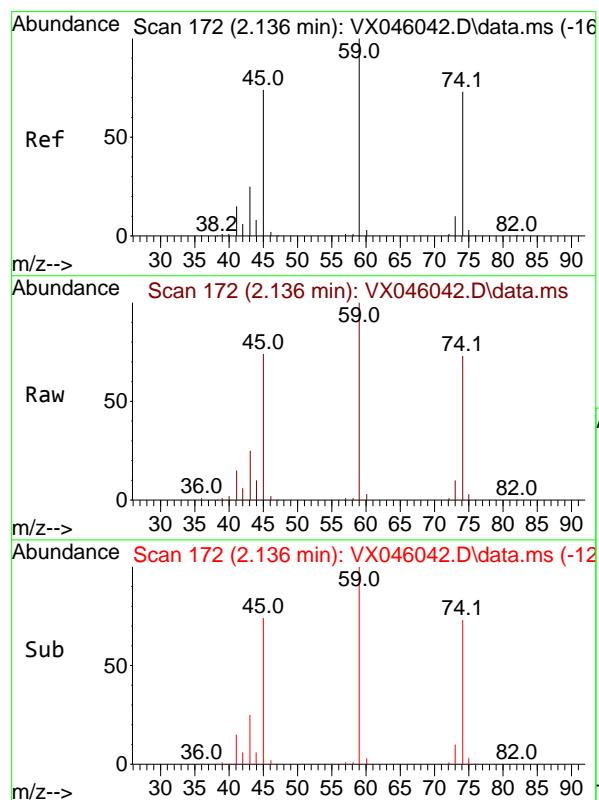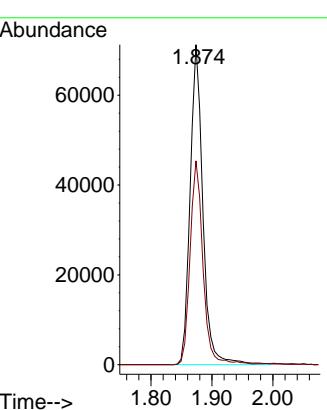

#8  
Diethyl Ether  
Concen: 35.350 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 74 Resp: 32724  
Ion Ratio Lower Upper  
74 100  
45 109.9 54.9 164.8

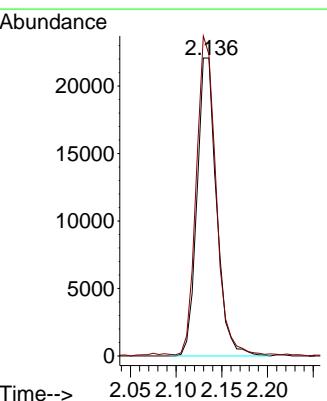

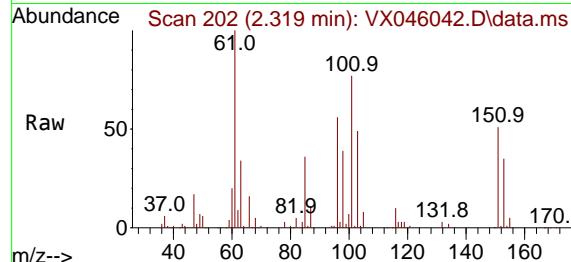

#9

1,1,2-Trichlorotrifluoroethane

Concen: 36.997 ug/l

RT: 2.319 min Scan# 202

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X

ClientSampleId :





VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

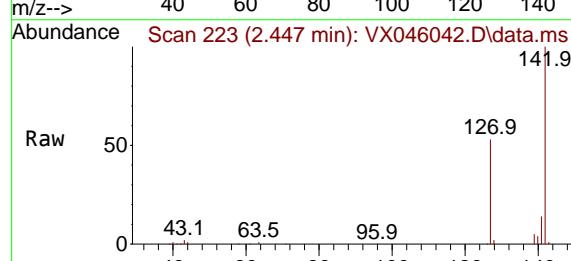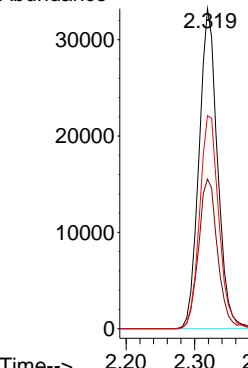

#10

Methyl Iodide

Concen: 39.622 ug/l

RT: 2.447 min Scan# 223

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt Ion:142 Resp: 78277


Ion Ratio Lower Upper




142 100

127 52.1 41.7 62.5

141 14.4 11.5 17.3

Abundance

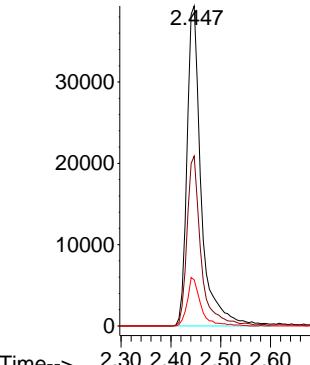

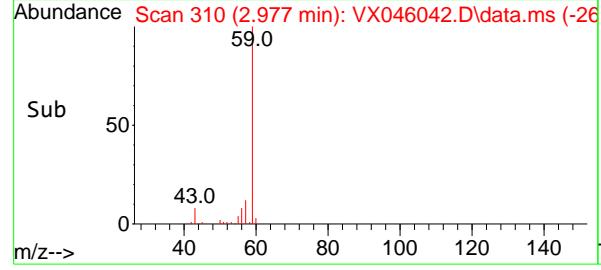

#11

Tert butyl alcohol

Concen: 181.745 ug/l

RT: 2.977 min Scan# 310

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

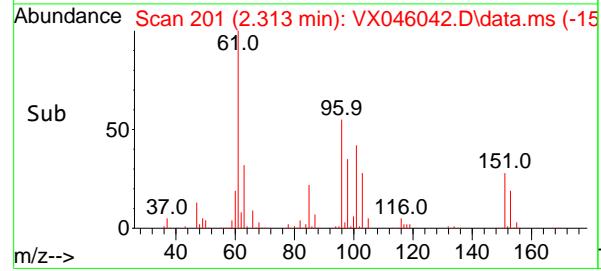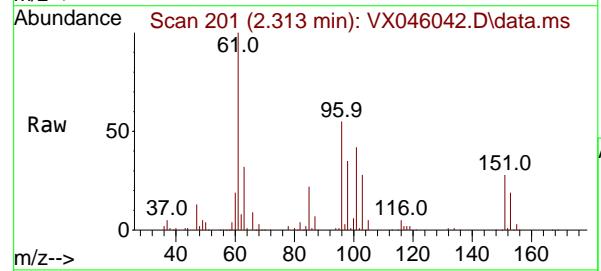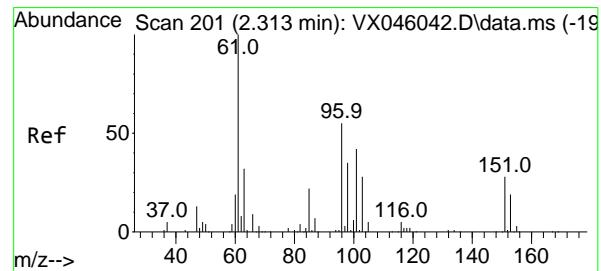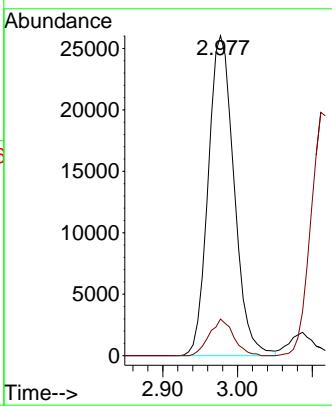

#12

1,1-Dichloroethene

Concen: 35.610 ug/l

RT: 2.313 min Scan# 201

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion: 96 Resp: 58334


Ion Ratio Lower Upper

96 100

61 182.7 146.2 219.2

98 63.8 51.0 76.6










#13

Acrolein  
Concen: 184.907 ug/l  
RT: 2.233 min Scan# 188  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58



Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


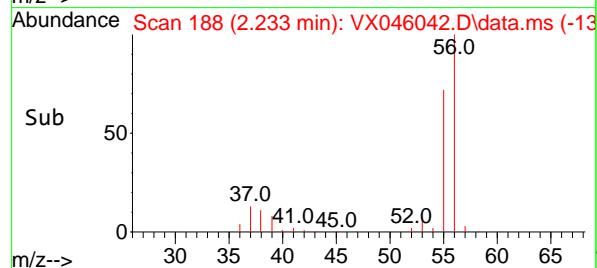



#14  
Allyl chloride  
Concen: 36.971 ug/l  
RT: 2.654 min Scan# 257  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58



Tgt Ion: 41 Resp: 114445  
Ion Ratio Lower Upper  
41 100  
39 75.7 60.6 90.8  
76 31.1 24.9 37.3





#15

Acrylonitrile

Concen: 182.874 ug/l

RT: 3.062 min Scan# 3

Instrument : MSVOA\_X

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

ClientSampleId :

VSTDICCC050

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Tgt Ion: 53 Resp: 188304

Ion Ratio Lower Upper





53 100

52 81.6 65.3 97.9

51 37.3 29.8 44.8

Abundance

3.062

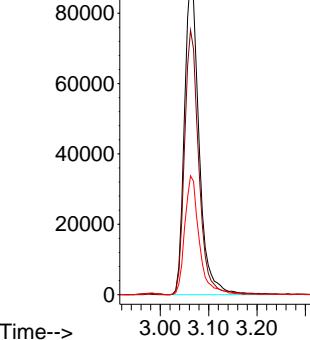

#16

Acetone

Concen: 177.910 ug/l

RT: 2.386 min Scan# 213

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt Ion: 43 Resp: 175777


Ion Ratio Lower Upper




43 100

58 26.5 21.2 31.8

Abundance

2.386

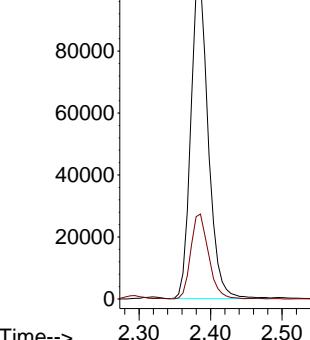

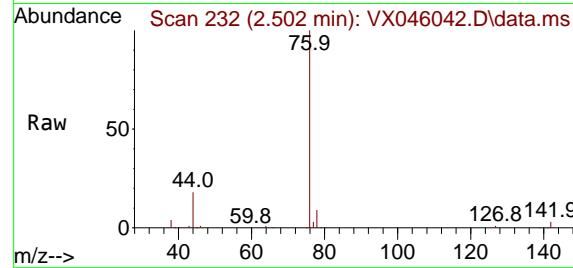

#17

Carbon Disulfide

Concen: 37.223 ug/l

RT: 2.502 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

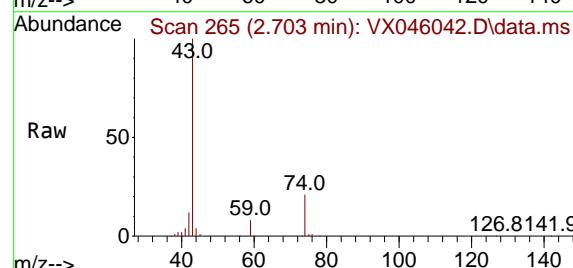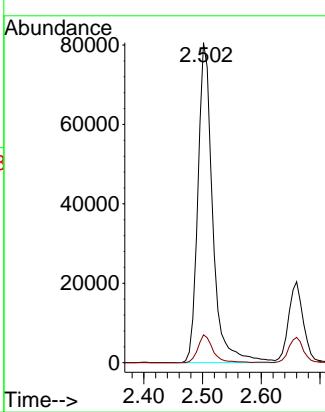

#18

Methyl Acetate

Concen: 34.915 ug/l


RT: 2.703 min Scan# 265







Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt Ion: 43 Resp: 82347  
 Ion Ratio Lower Upper  
 43 100  
 74 20.9 16.7 25.1

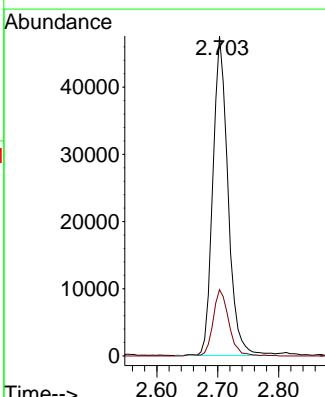




#19

Methyl tert-butyl Ether  
Concen: 36.695 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025






#20

Methylene Chloride  
Concen: 33.182 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 84 Resp: 66412  
Ion Ratio Lower Upper  
84 100  
49 142.4 113.9 170.9  
51 41.9 33.5 50.3  
86 67.3 53.8 80.8

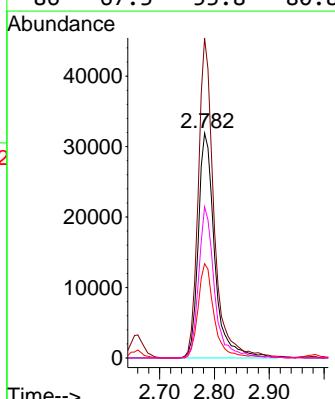



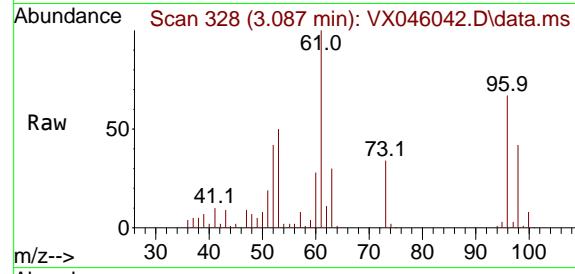
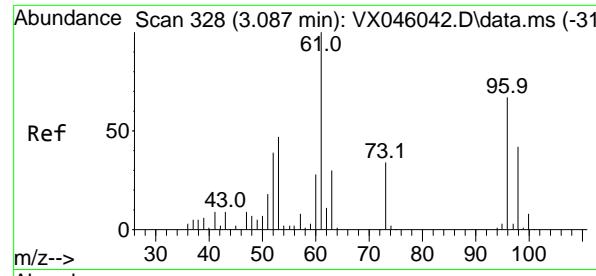


#21  
trans-1,2-Dichloroethene  
Concen: 35.421 ug/l  
RT: 3.087 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

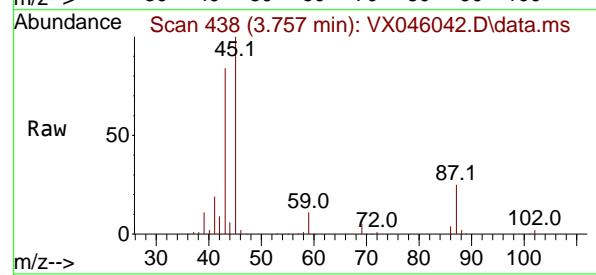


#22  
Diisopropyl ether  
Concen: 38.241 ug/l  
RT: 3.757 min Scan# 438  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 45 Resp: 221172  
Ion Ratio Lower Upper  
45 100  
43 83.3 66.6 100.0  
87 24.7 19.8 29.6  
59 10.7 8.6 12.8

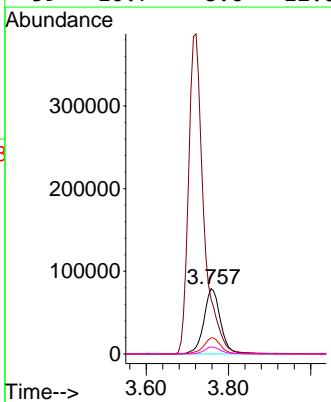




Abundance Scan 432 (3.721 min): VX046042.D\data.ms

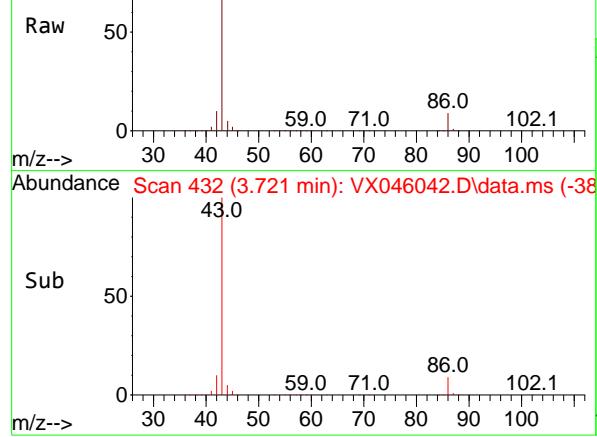

Abundance Scan 432 (3.721 min): VX046042.D\data.ms (-38)

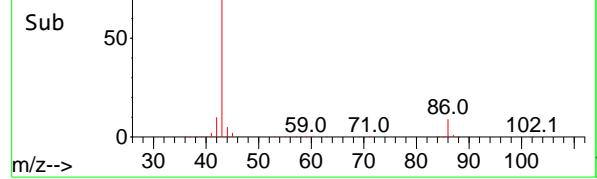

#23

Vinyl Acetate

Concen: 194.528 ug/l

RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050


**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025


Supervised By :Mahesh Dadoda 05/06/2025

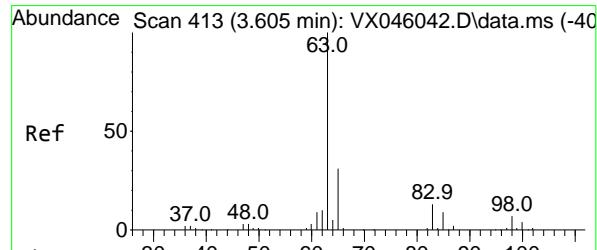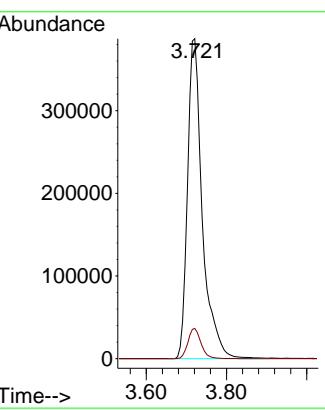

Abundance Scan 413 (3.605 min): VX046042.D\data.ms

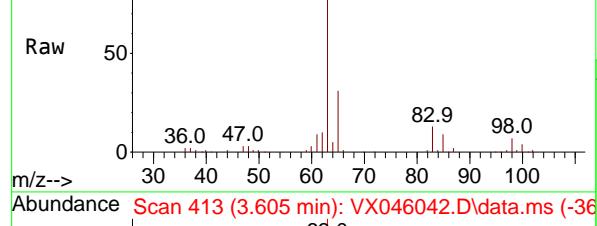

Abundance Scan 413 (3.605 min): VX046042.D\data.ms (-36)

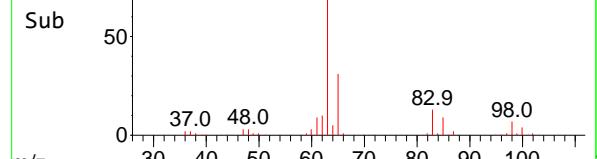

#24

1,1-Dichloroethane

Concen: 36.067 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion: 63 Resp: 122601


Ion Ratio Lower Upper

63 100

98 7.2 3.6 10.8





100 4.2 2.1 6.3

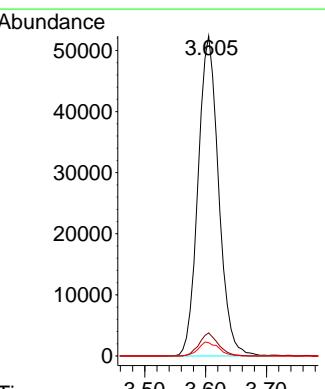






#25  
2-Butanone  
Concen: 188.783 ug/l  
RT: 4.556 min Scan# 569  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

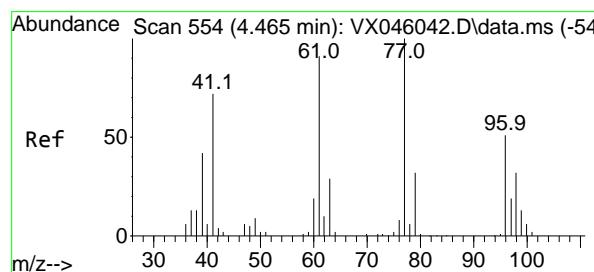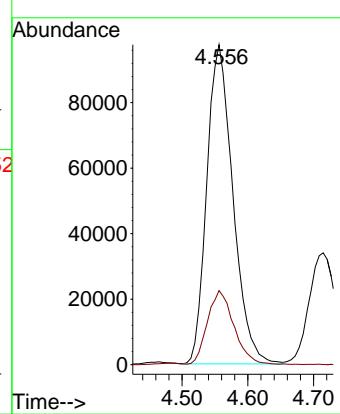




#26  
2,2-Dichloropropane  
Concen: 36.059 ug/l  
RT: 4.465 min Scan# 554  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

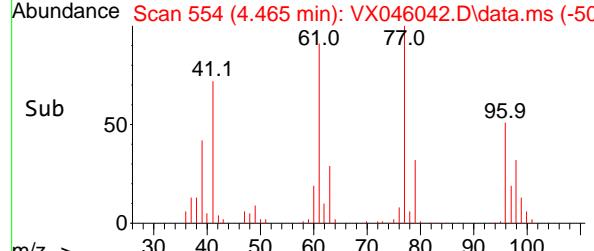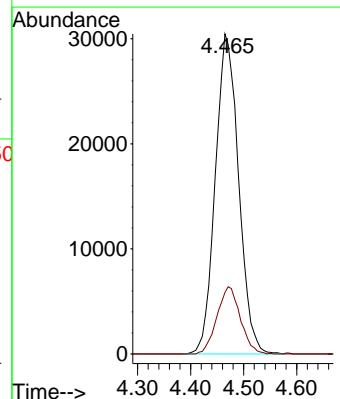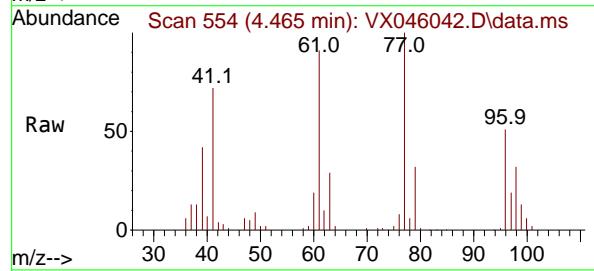

1 Manual Integrations  
2 APPROVED

3 Reviewed By :John Carlone 05/06/2025  
4 Supervised By :Mahesh Dadoda 05/06/2025







#27  
cis-1,2-Dichloroethene  
Concen: 35.466 ug/l  
RT: 4.483 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#28  
Bromochloromethane  
Concen: 31.031 ug/l  
RT: 4.898 min Scan# 625  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 49 Resp: 56091  
Ion Ratio Lower Upper  
49 100  
129 2.0 0.0 4.0  
130 70.2 56.2 84.2



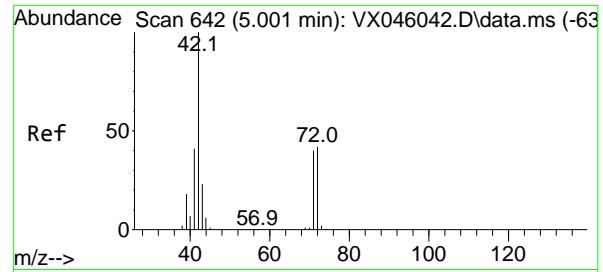

#29

Tetrahydrofuran

Concen: 183.679 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument :

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

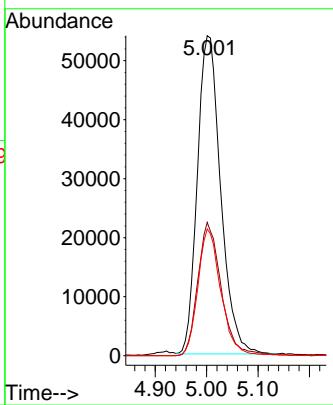

#30

Chloroform

Concen: 35.626 ug/l

RT: 5.087 min Scan# 656

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58




Tgt Ion: 83 Resp: 125850

Ion Ratio Lower Upper

83 100

85 61.6 49.3 73.9



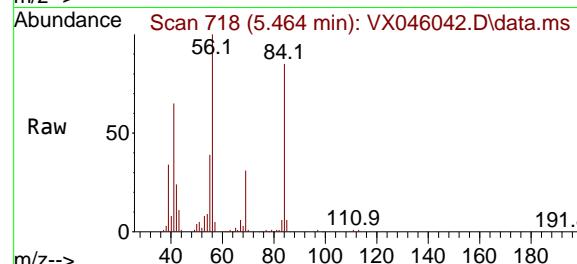

#31

Cyclohexane

Concen: 38.205 ug/l

RT: 5.464 min Scan# 718

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

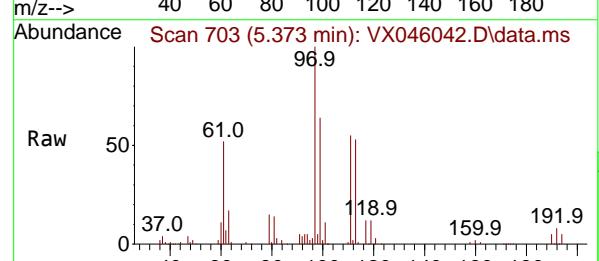

#32

1,1,1-Trichloroethane

Concen: 36.034 ug/l

RT: 5.373 min Scan# 703

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion: 97 Resp: 109781




Ion Ratio Lower Upper

97 100

99 64.7 51.8 77.6

61 50.1 40.1 60.1

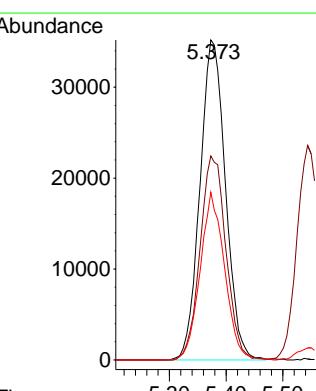

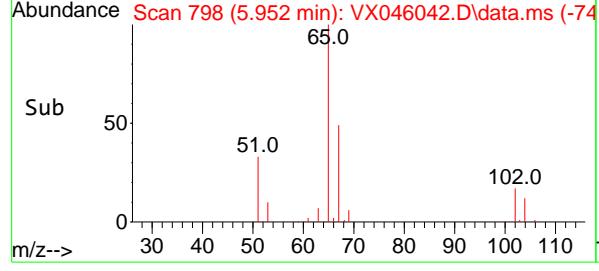

#33

1,2-Dichloroethane-d4

Concen: 30.601 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58




Instrument :



MSVOA\_X

ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

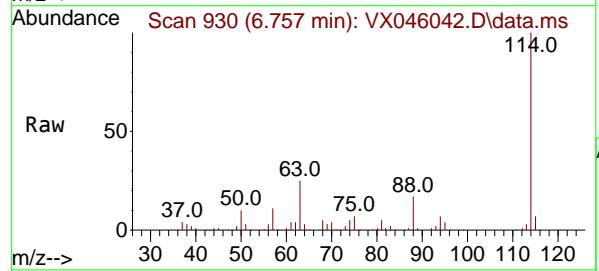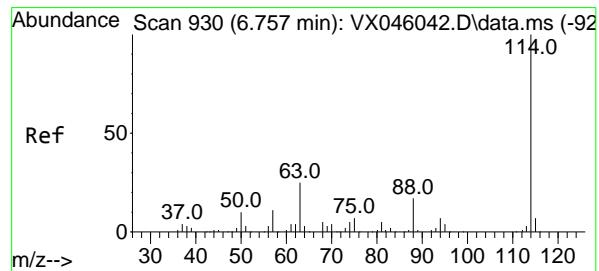 Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

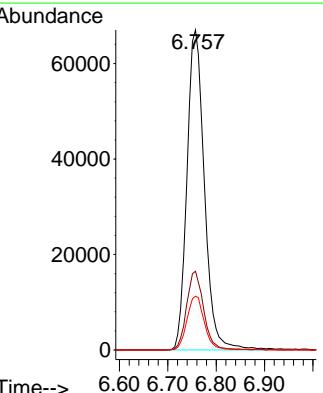 #34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 6.757 min Scan# 930  
 Delta R.T. 0.000 min  
 Lab File: VX046042.D  
 Acq: 05 May 2025 11:58


 Tgt Ion:114 Resp: 167947  
 Ion Ratio Lower Upper  
 114 100  
 63 24.6 0.0 49.2  
 88 16.8 0.0 33.6


Sub

50

0

m/z--&gt;

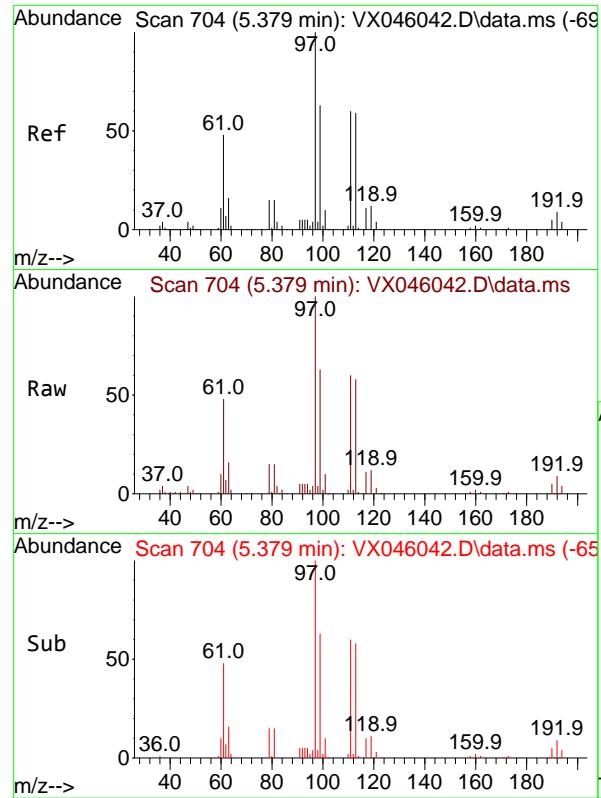

#35

Dibromofluoromethane

Concen: 31.633 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

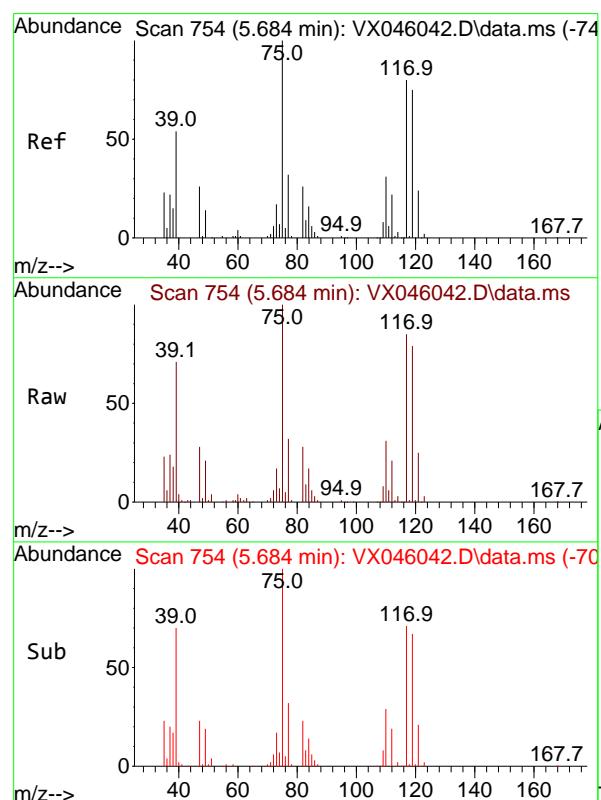

#36

1,1-Dichloropropene

Concen: 38.073 ug/l

RT: 5.684 min Scan# 754

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion: 75 Resp: 83215




Ion Ratio Lower Upper

75 100

110 32.6 16.3 48.9

77 30.4 24.3 36.5

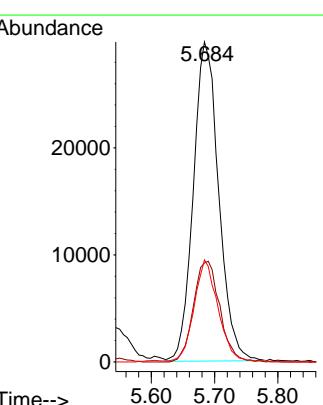

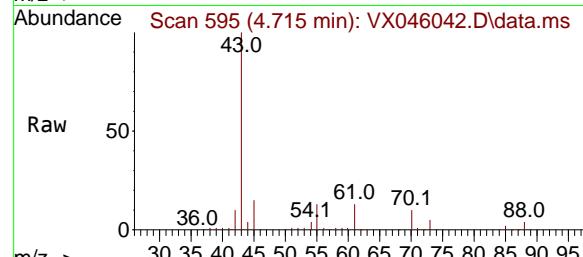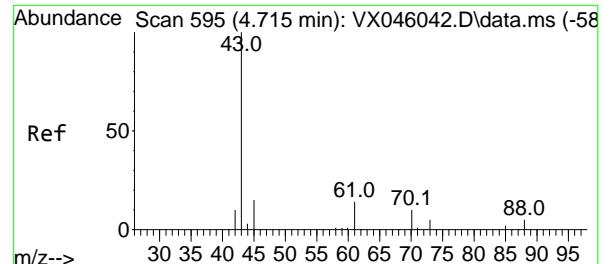

#37

**Ethyl Acetate**

Concen: 37.394 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

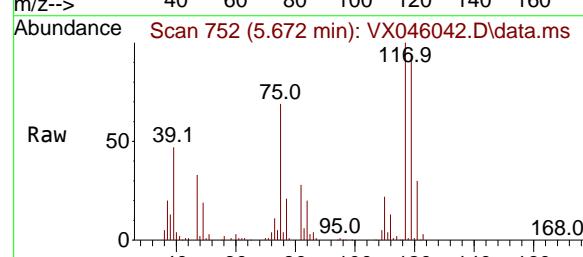

#38

**Carbon Tetrachloride**

Concen: 37.320 ug/l


RT: 5.672 min Scan# 752


Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt	Ion:117	Resp:	93712
Ion	Ratio	Lower	Upper
117	100		
119	94.0	75.2	112.8
121	30.3	24.2	36.4

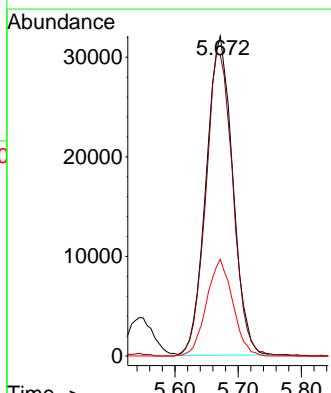

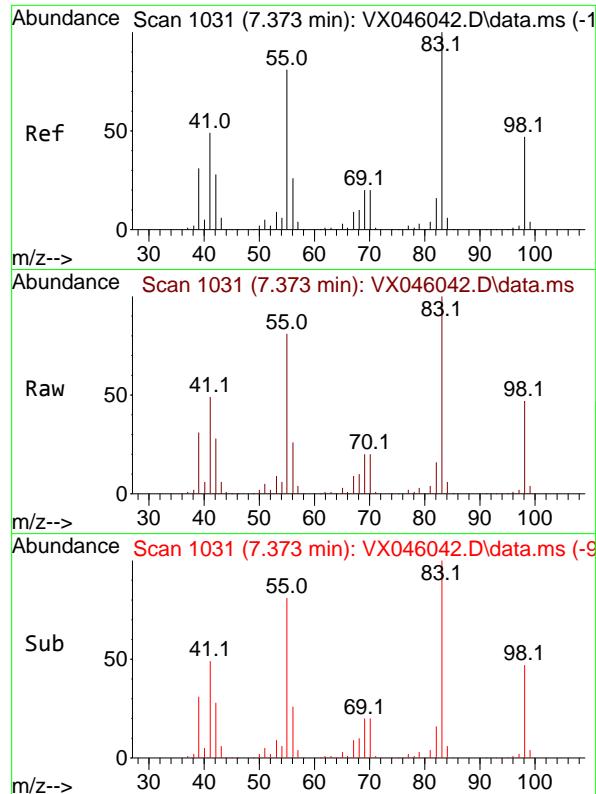

#39

Methylcyclohexane

Concen: 39.307 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICCC050

Tgt Ion: 83 Resp: 10765:

Ion Ratio Lower Upper

83 100

55 80.9 64.7 97.1



98 46.8 37.4 56.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

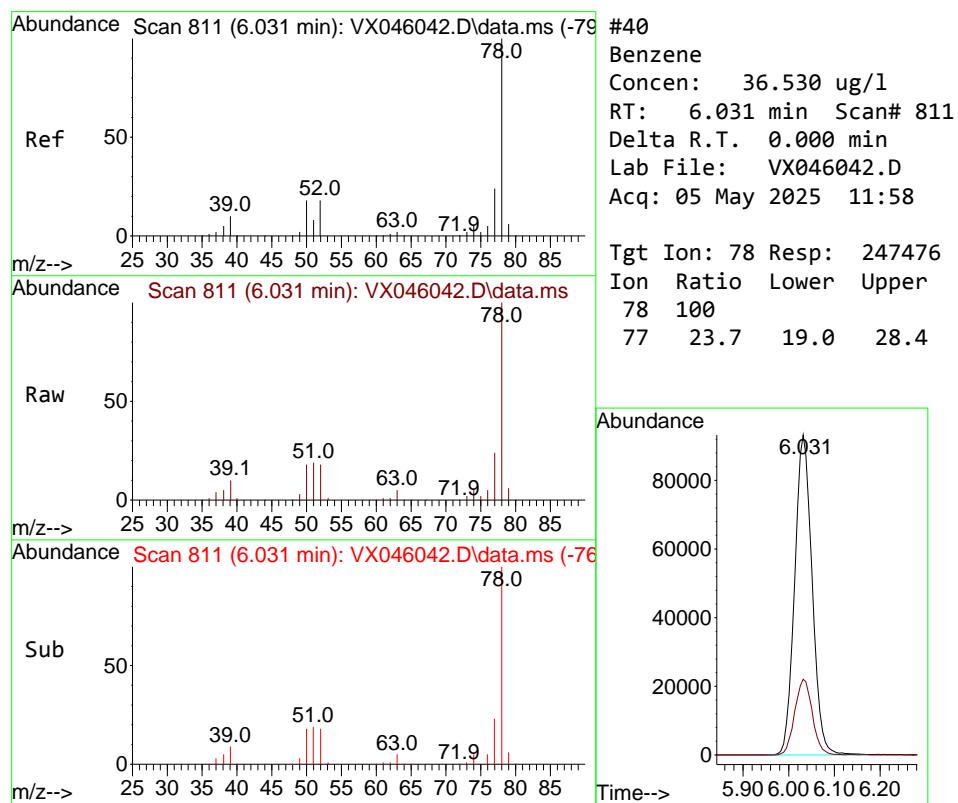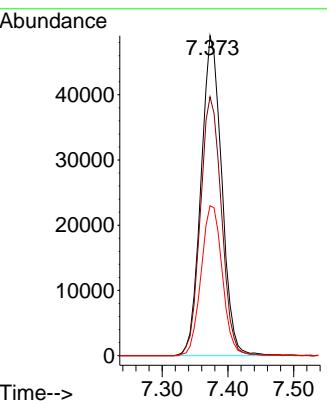

#40

Benzene

Concen: 36.530 ug/l

RT: 6.031 min Scan# 811

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58




Tgt Ion: 78 Resp: 247476

Ion Ratio Lower Upper

78 100

77 23.7 19.0 28.4

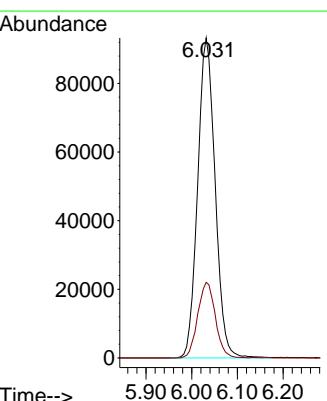

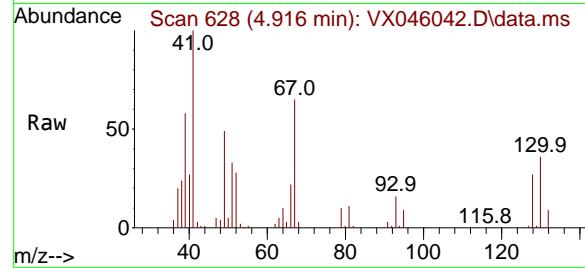

#41

Methacrylonitrile

Concen: 38.123 ug/l

RT: 4.916 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#42

1,2-Dichloroethane

Concen: 37.605 ug/l

RT: 6.080 min Scan# 819

Delta R.T. 0.000 min

Lab File: VX046042.D



Acq: 05 May 2025 11:58


Tgt Ion: 62 Resp: 105332

Ion Ratio Lower Upper

62 100

98 7.6 0.0 15.2

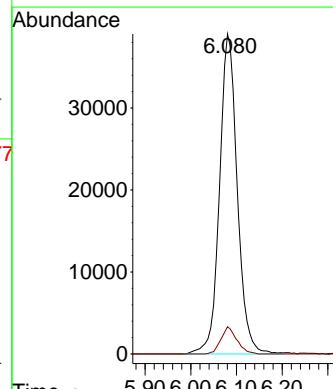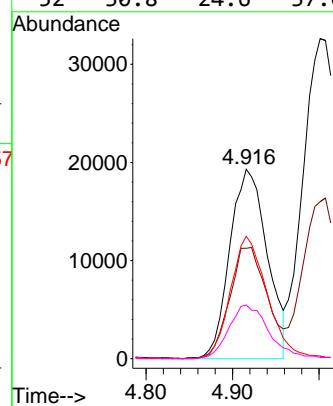



#43

Isopropyl Acetate


Concen: 38.598 ug/l

RT: 6.336 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

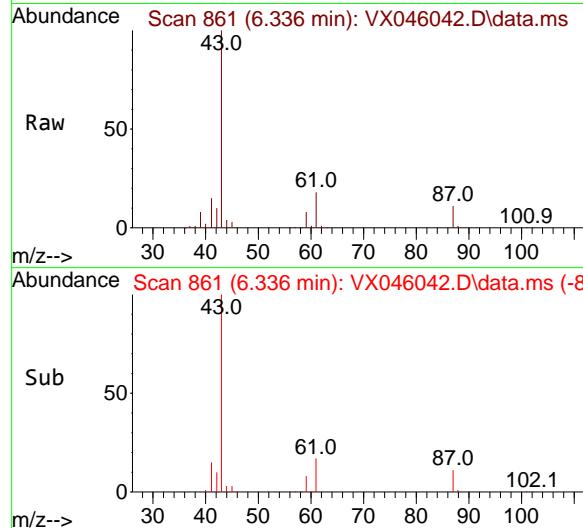

Tgt Ion: 43 Resp: 16178

Ion Ratio Lower Upper

43 100




61 17.9 14.3 21.5

87 11.9 9.5 14.3




**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025




Supervised By :Mahesh Dadoda 05/06/2025

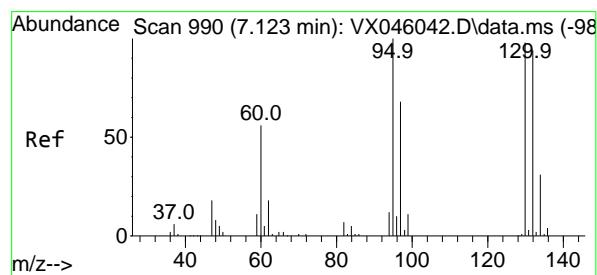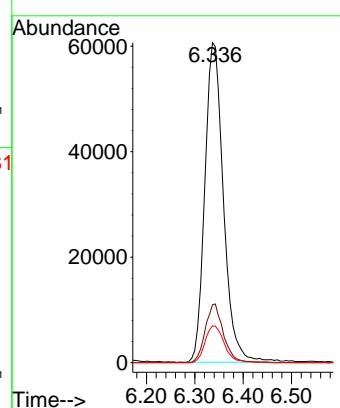

#44  
Trichloroethene  
Concen: 37.230 ug/l  
RT: 7.123 min Scan# 990  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

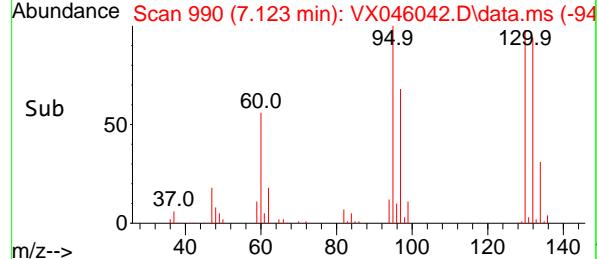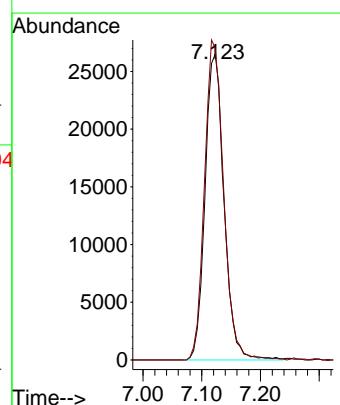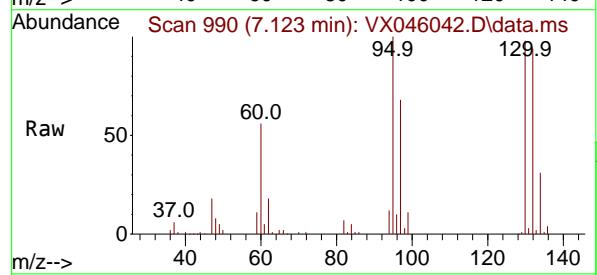

Tgt Ion:130 Resp: 59623  
Ion Ratio Lower Upper  
130 100  
95 102.1 0.0 204.2



#45

1,2-Dichloropropane

Concen: 37.064 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

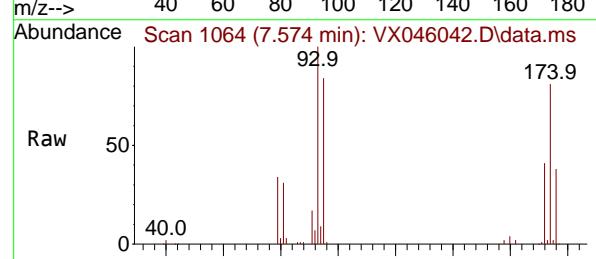

#46

Dibromomethane

Concen: 36.326 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion: 93 Resp: 48201




Ion Ratio Lower Upper

93 100

95 82.0 65.6 98.4

174 85.2 68.2 102.2

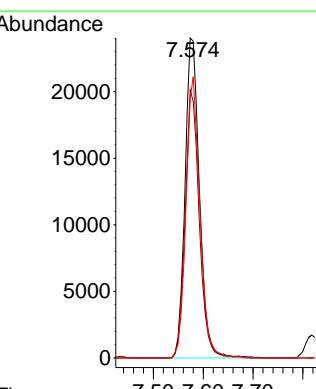

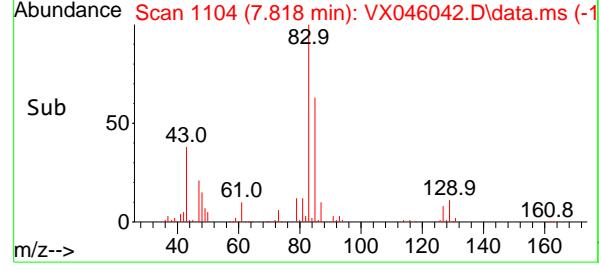

#47

Bromodichloromethane

Concen: 37.685 ug/l

RT: 7.818 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

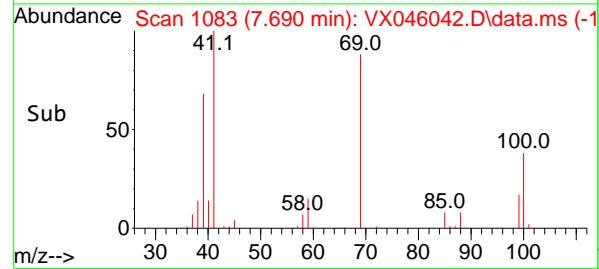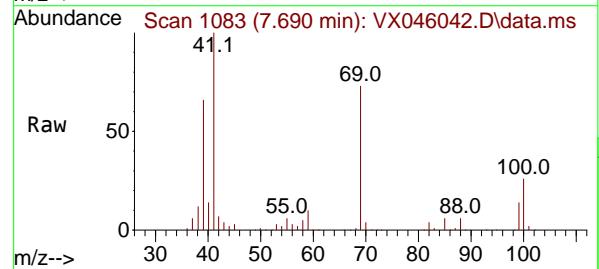

#48

Methyl methacrylate

Concen: 39.157 ug/l


RT: 7.690 min Scan# 1083


Delta R.T. 0.000 min

Lab File: VX046042.D



Acq: 05 May 2025 11:58

Tgt	Ion	Resp:	84277
Ion	Ratio	Lower	Upper
41	100		
69	73.1	58.5	87.7
39	64.6	51.7	77.5

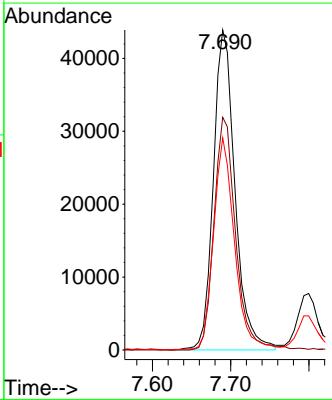




Abundance Scan 1078 (7.659 min): VX046042.D\data.ms

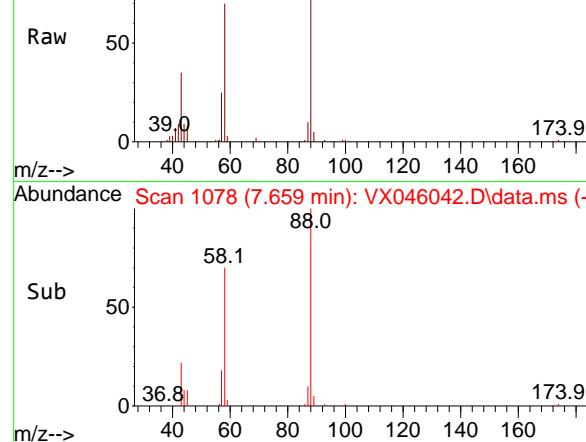

Abundance Scan 1240 (8.647 min): VX046042.D\data.ms

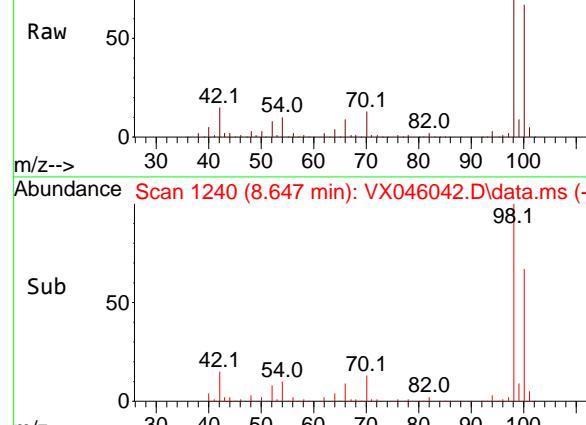

#49

1,4-Dioxane

Concen: 713.477 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#50

Toluene-d8

Concen: 32.395 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58


Tgt Ion: 98 Resp: 205479

Ion Ratio Lower Upper

98 100

100 66.9 53.5 80.3

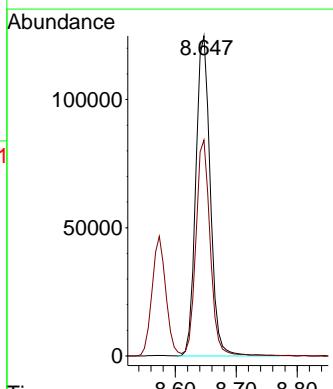

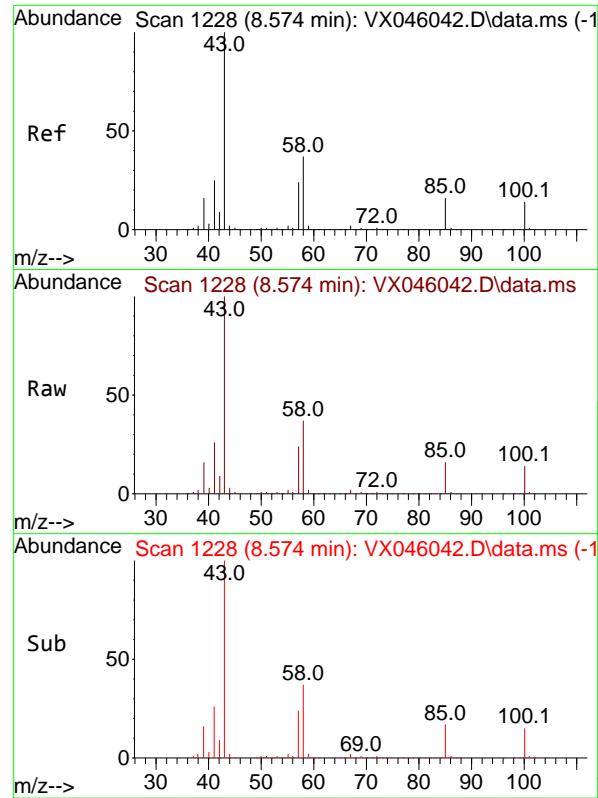

#51

4-Methyl-2-Pentanone

Concen: 193.653 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

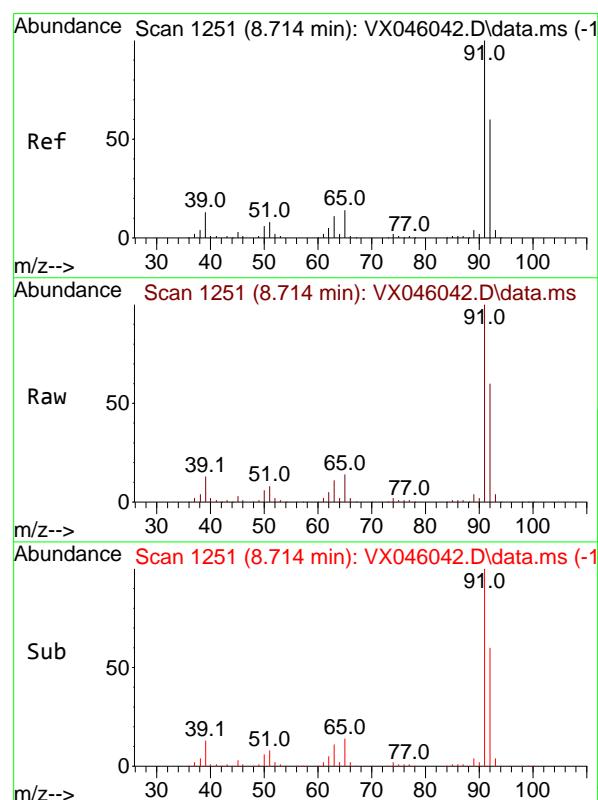

#52

Toluene

Concen: 37.530 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58




Tgt Ion: 92 Resp: 150757

Ion Ratio Lower Upper

92 100

91 170.8 136.6 205.0

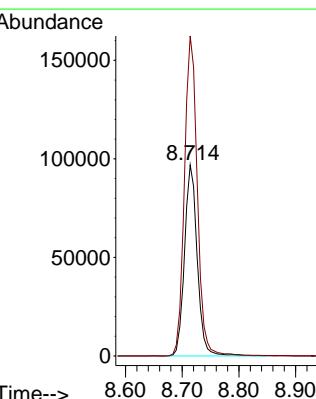



#53

t-1,3-Dichloropropene

Concen: 41.056 ug/l

RT: 8.976 min Scan# 1193

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

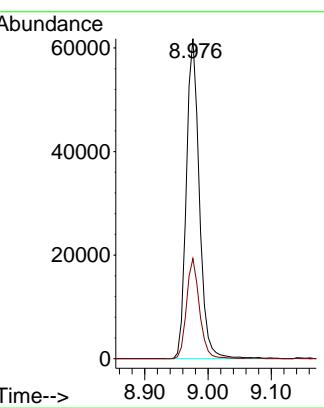

#54

cis-1,3-Dichloropropene

Concen: 38.521 ug/l

RT: 8.360 min Scan# 1193



Delta R.T. 0.000 min




Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt Ion: 75 Resp: 97031

Ion Ratio	Lower	Upper	
75	100		
77	31.7	25.4	38.0
39	65.3	52.2	78.4

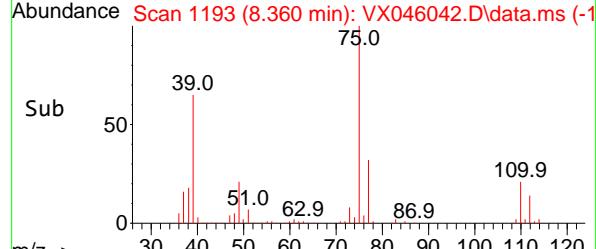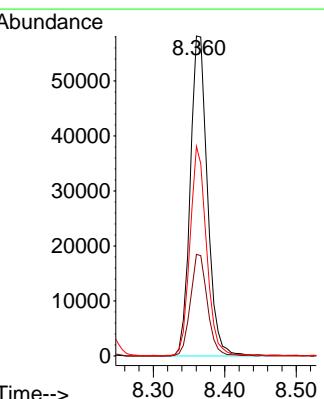



#55

1,1,2-Trichloroethane

Concen: 36.648 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

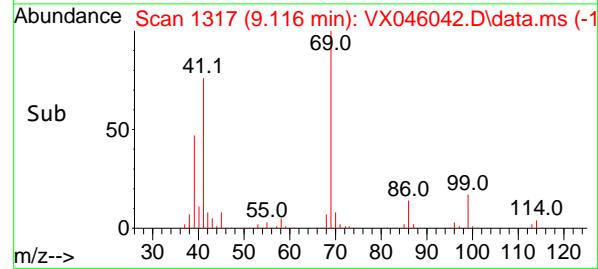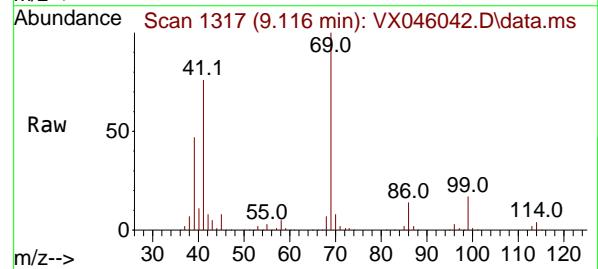

#56

Ethyl methacrylate

Concen: 39.726 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58



Tgt Ion: 69 Resp: 99947







Ion Ratio Lower Upper

69 100

41 76.0 60.8 91.2

39 48.8 39.0 58.6

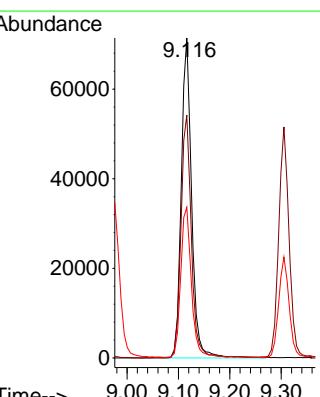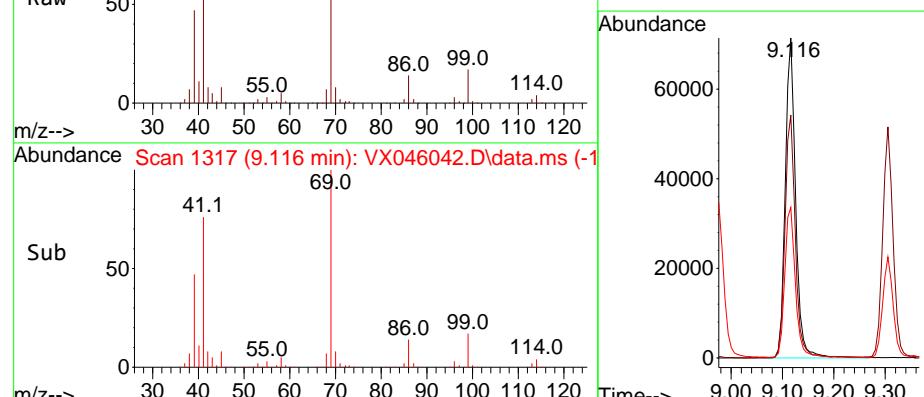




#57

1,3-Dichloropropane  
Concen: 36.347 ug/l  
RT: 9.305 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

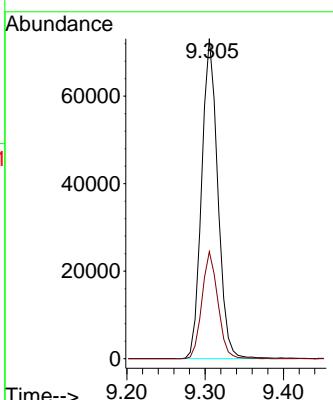


#58



2-Chloroethyl Vinyl ether  
Concen: 227.902 ug/l  
RT: 8.238 min Scan# 1173  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 63 Resp: 257678  
Ion Ratio Lower Upper  
63 100  
106 26.9 21.5 32.3






Abundance Scan 1368 (9.427 min): VX046042.D\data.ms

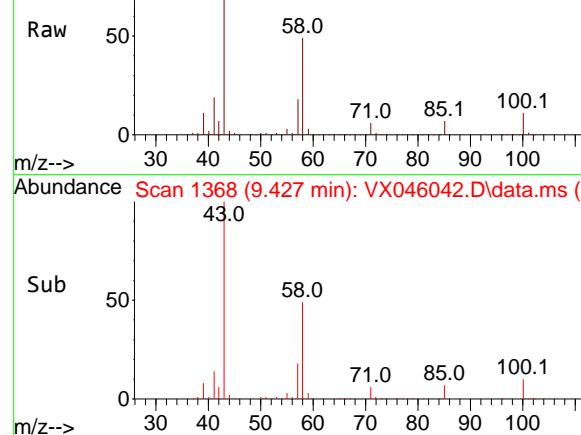

Abundance Scan 1383 (9.519 min): VX046042.D\data.ms

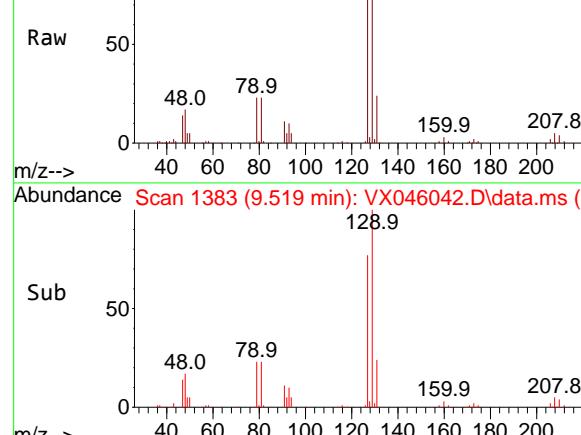

Abundance Scan 1383 (9.519 min): VX046042.D\data.ms (-1)

#59

2-Hexanone

Concen: 190.168 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#60

Dibromochloromethane

Concen: 38.027 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58




Tgt Ion:129 Resp: 67198

Ion Ratio Lower Upper

129 100

127 78.5 39.3 117.8

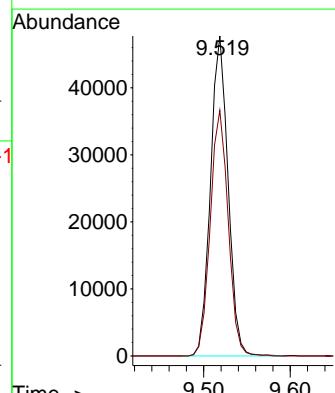

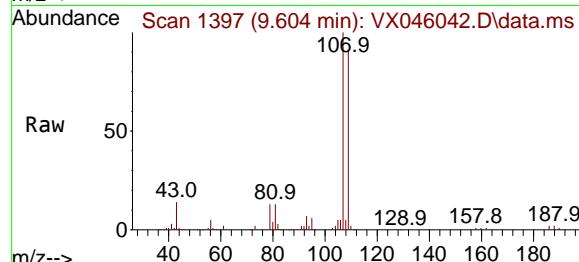

#61

1,2-Dibromoethane

Concen: 37.567 ug/l

RT: 9.604 min Scan# 1397

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

40000

30000

20000




10000

0

9.50 9.60 9.70

Time--&gt;

9.50 9.60 9.70



#62

4-Bromofluorobenzene

Concen: 34.229 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt Ion: 95 Resp: 79012

Ion Ratio Lower Upper

95 100

174 67.9 0.0 135.8

176 65.7 0.0 131.4

Abundance

60000

40000


20000

0

11.00 11.079 11.10

Time--&gt;

11.00 11.079 11.10


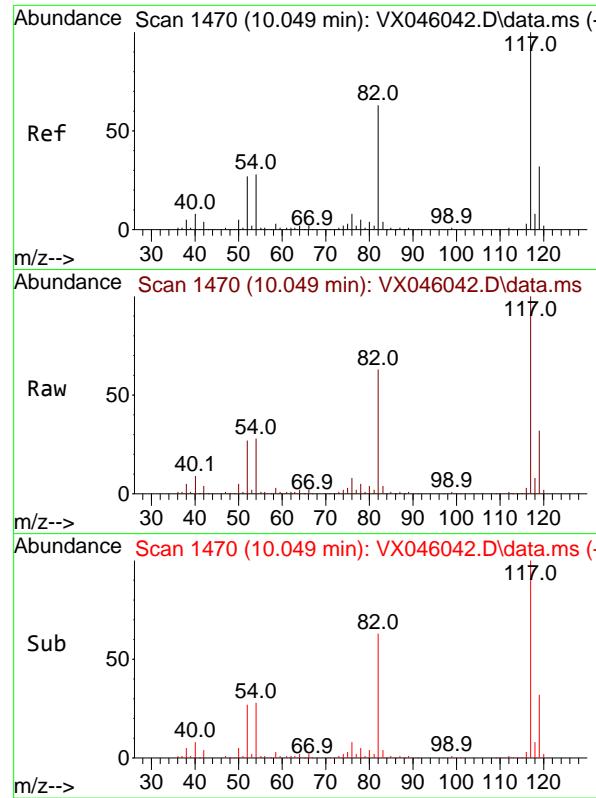


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 146251  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carbone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

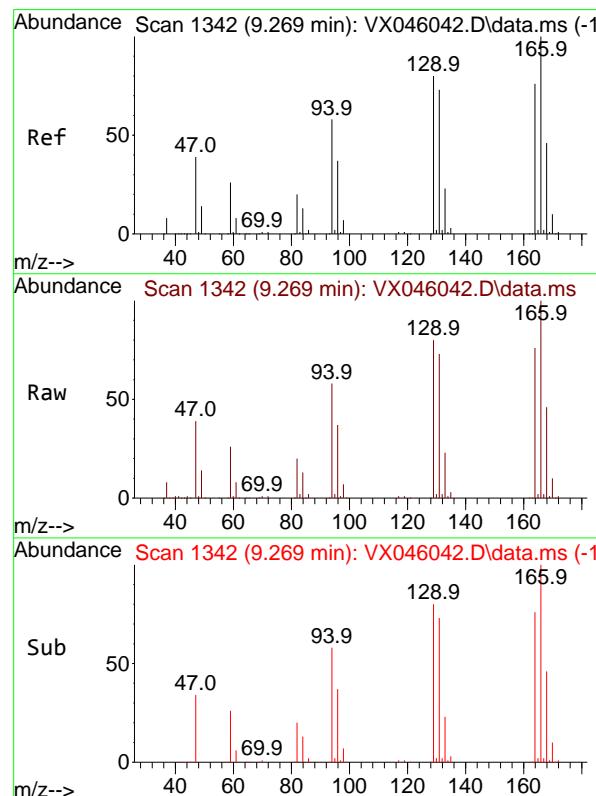

#64  
Tetrachloroethene  
Concen: 36.726 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion:164 Resp: 54853  
Ion Ratio Lower Upper  
164 100  
166 131.3 105.0 157.6  
129 104.4 83.5 125.3  
131 95.6 76.5 114.7



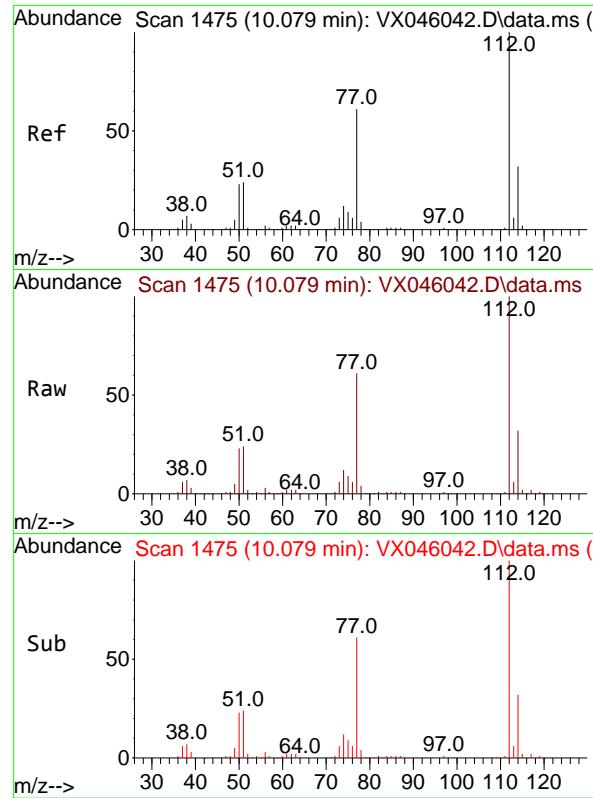

#65

Chlorobenzene

Concen: 35.686 ug/l

RT: 10.079 min Scan# 1475

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

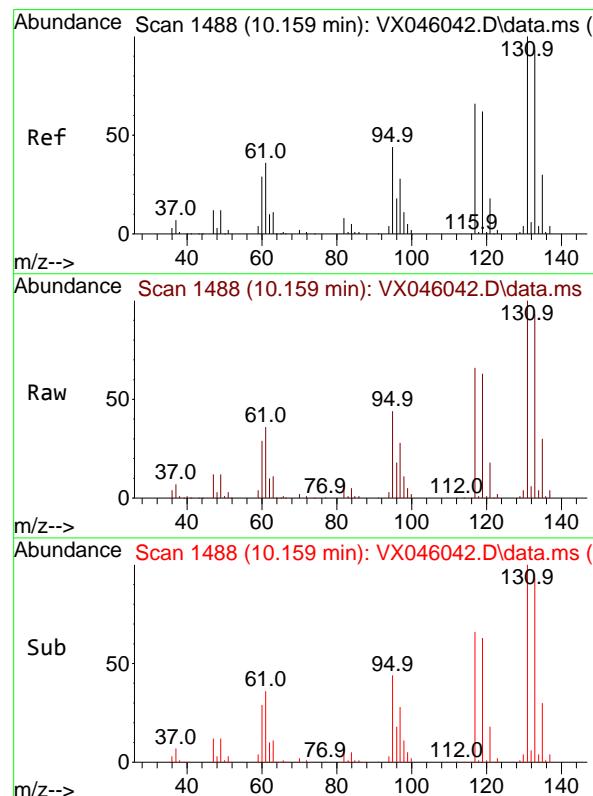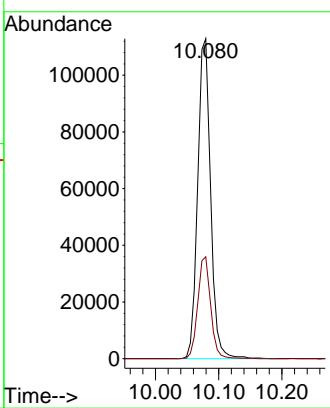

#66

1,1,1,2-Tetrachloroethane

Concen: 38.017 ug/l

RT: 10.159 min Scan# 1488


Delta R.T. 0.000 min




Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt Ion:131 Resp: 57066

Ion	Ratio	Lower	Upper
131	100		
133	94.6	47.3	141.9
119	63.3	31.6	95.0

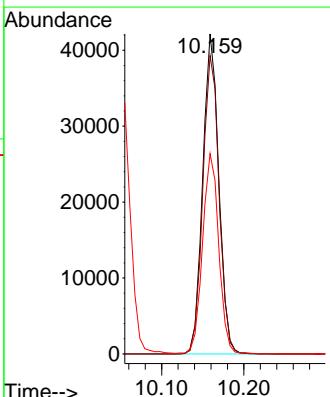



#67

Ethyl Benzene

Concen: 38.543 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#68

m/p-Xylenes

Concen: 78.142 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58


Tgt Ion:106 Resp: 216578

Ion Ratio Lower Upper

106 100

91 214.0 171.2 256.8

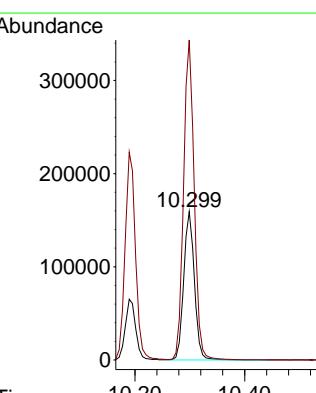

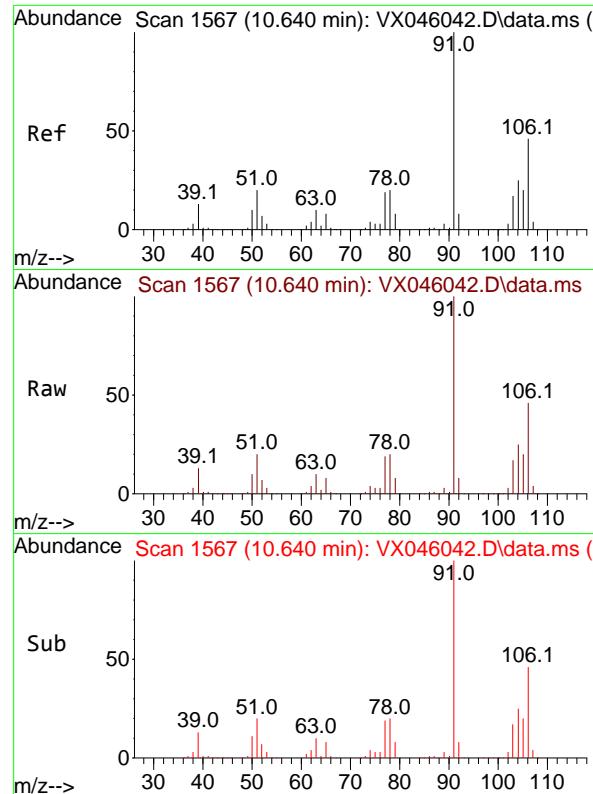


#69  
o-Xylene  
Concen: 38.064 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58  
ClientSampleId : VSTDICCC050

Tgt Ion:106 Resp: 106339  
Ion Ratio Lower Upper  
106 100  
91 225.4 112.7 338.1


### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

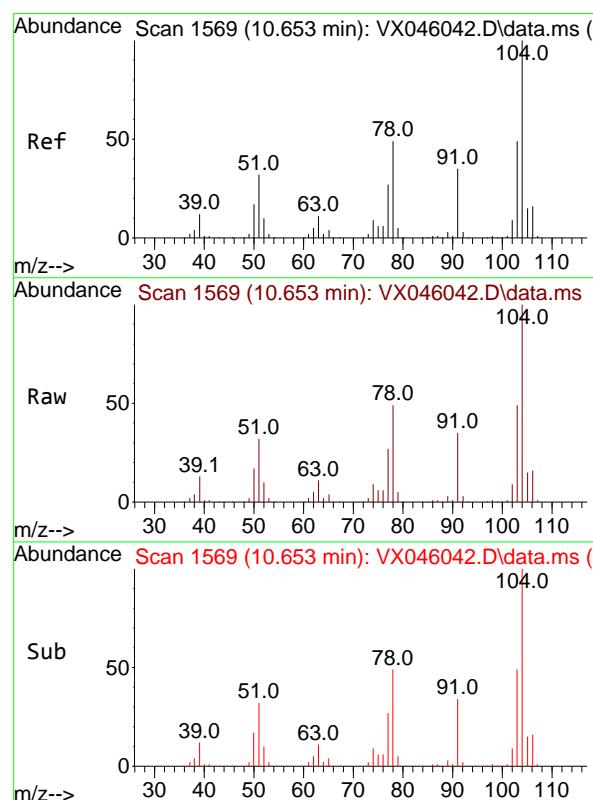

#70  
Styrene  
Concen: 39.888 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion:104 Resp: 178313  
Ion Ratio Lower Upper  
104 100  
78 57.1 45.7 68.5  
103 54.6 43.7 65.5

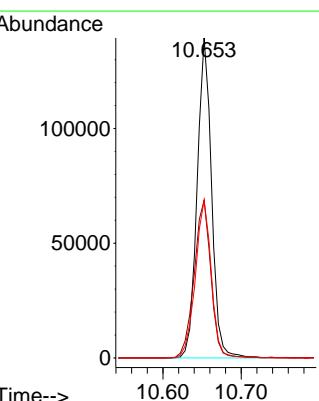

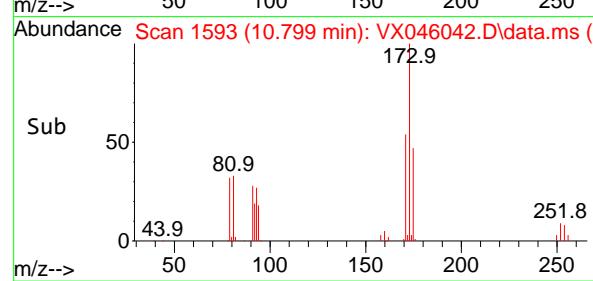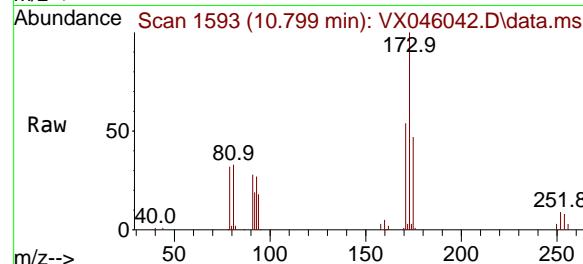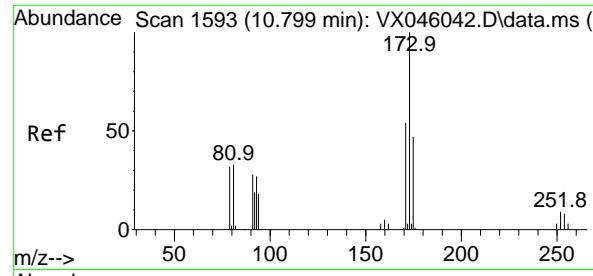

#71

Bromoform

Concen: 39.457 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion:152 Resp: 67976


Ion Ratio Lower Upper

152 100

115 93.8 46.9 140.7

150 175.5 0.0 351.0

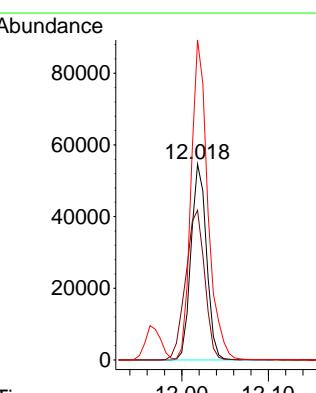

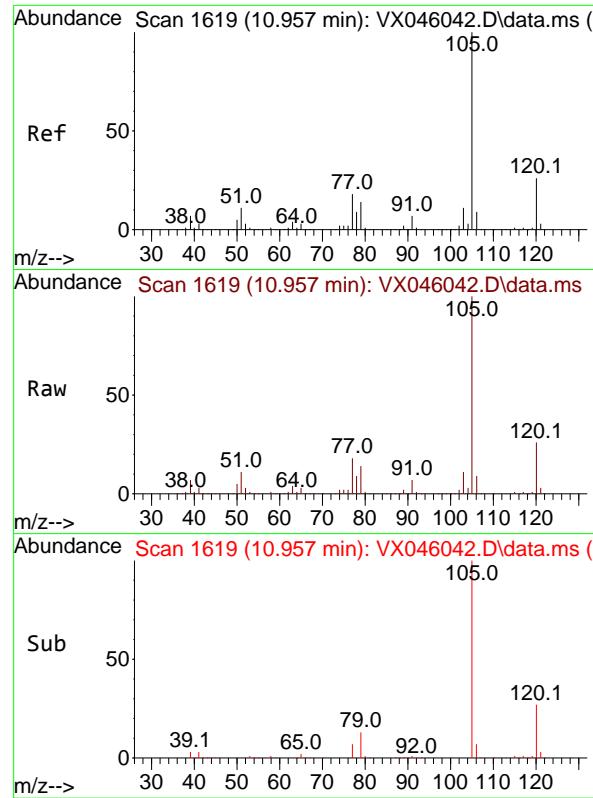

#73

Isopropylbenzene

Concen: 37.865 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

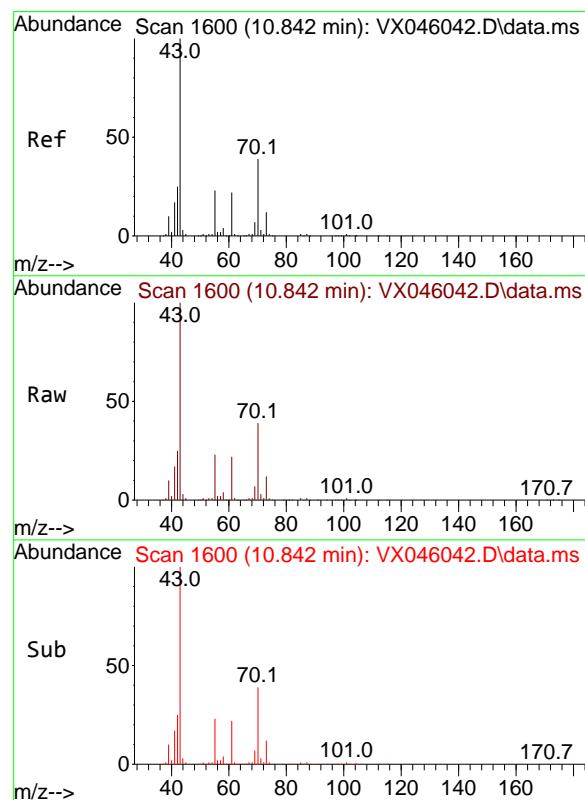

#74

N-amyl acetate

Concen: 38.012 ug/l


RT: 10.842 min Scan# 1600


Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt	Ion:	Resp:	
	43	140509	
	100		
43	100		
70	38.6	30.9	46.3
55	23.4	18.7	28.1
61	21.4	17.1	25.7




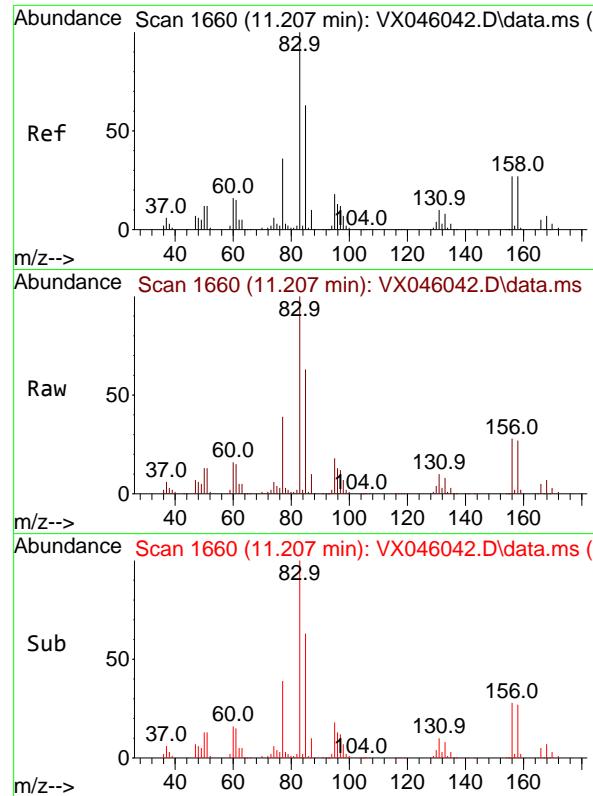


#75  
1,1,2,2-Tetrachloroethane  
Concen: 34.495 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

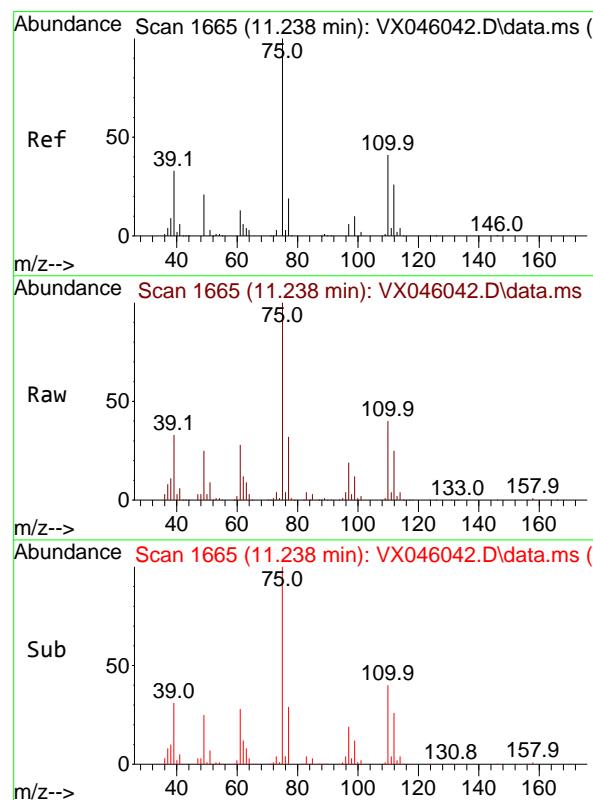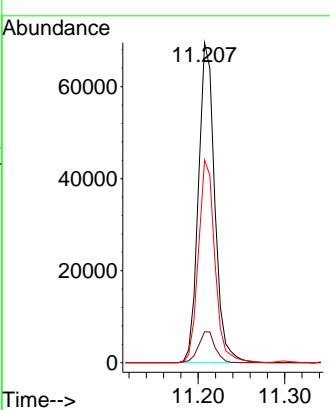

#76  
1,2,3-Trichloropropane  
Concen: 28.468 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 75 Resp: 80678  
Ion Ratio Lower Upper  
75 100  
77 41.0 20.5 61.5

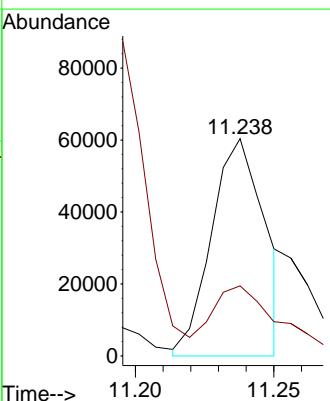

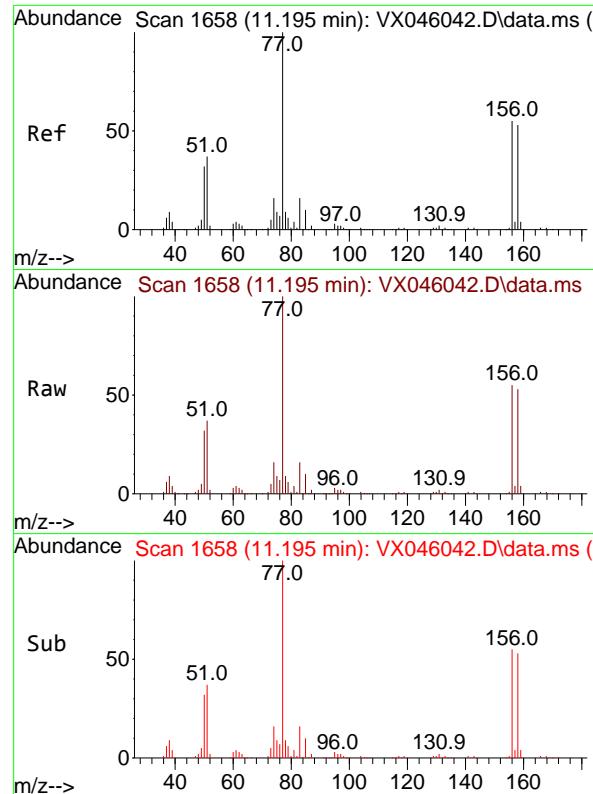

#77

Bromobenzene

Concen: 36.763 ug/l

RT: 11.195 min Scan# 1658

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

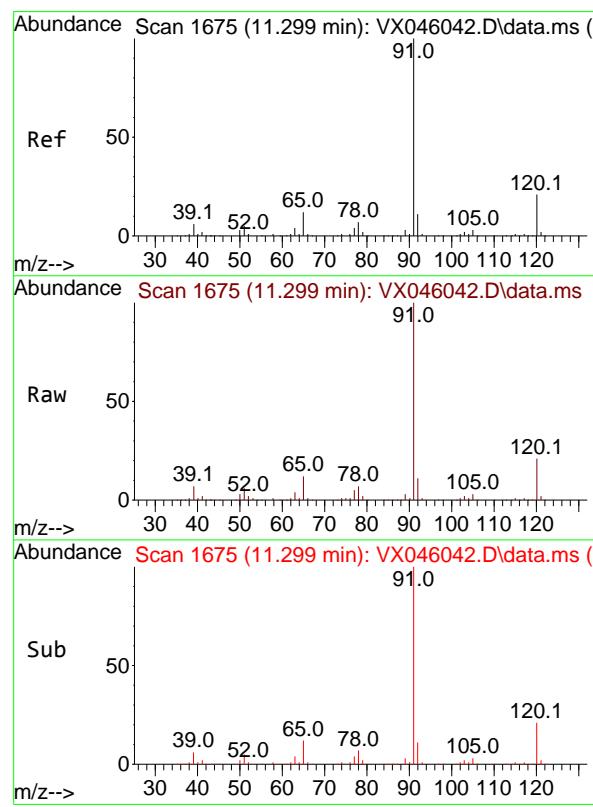

#78

n-propylbenzene

Concen: 39.707 ug/l

RT: 11.299 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58


Tgt Ion: 91 Resp: 329981

Ion Ratio Lower Upper


91 100

120 21.6 10.8 32.4


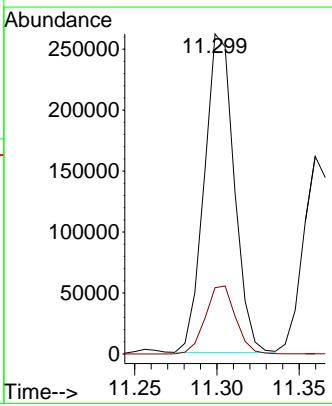





Abundance Scan 1685 (11.360 min): VX046042.D\data.ms (-)

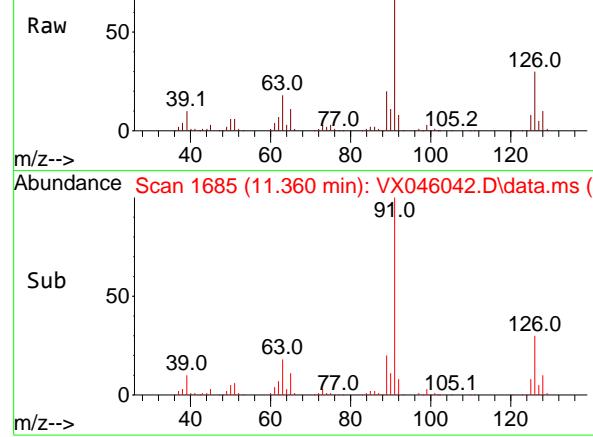


Abundance Scan 1685 (11.360 min): VX046042.D\data.ms (-)

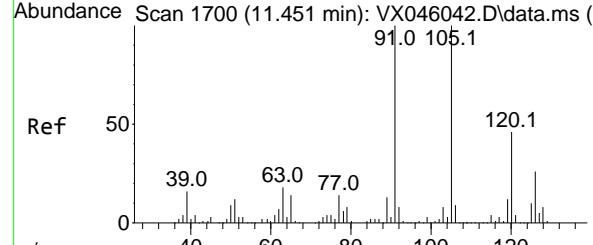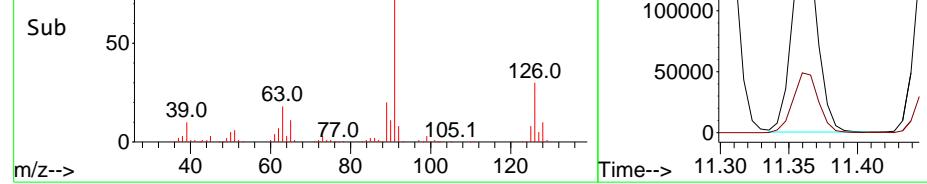

Abundance Scan 1700 (11.451 min): VX046042.D\data.ms (-)

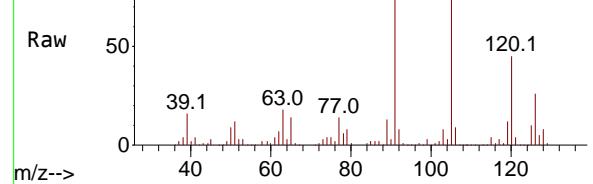

Abundance Scan 1700 (11.451 min): VX046042.D\data.ms (-)

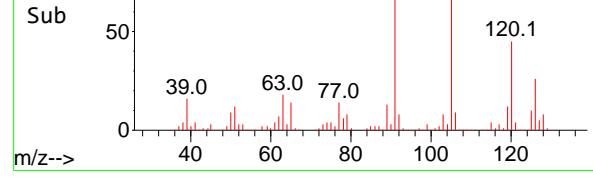

Abundance Scan 1700 (11.451 min): VX046042.D\data.ms (-)

#79

2-Chlorotoluene

Concen: 36.336 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICCC050

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025


Supervised By :Mahesh Dadoda 05/06/2025

Tgt Ion: 91 Resp: 203509

Ion Ratio Lower Upper

91 100

126 31.1 15.6 46.7

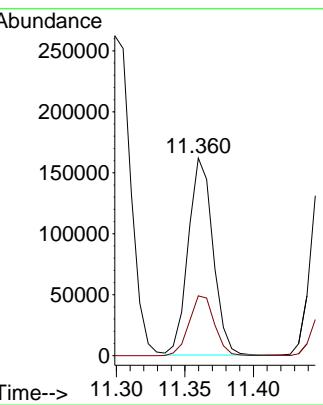

#80

1,3,5-Trimethylbenzene

Concen: 38.516 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58


Tgt Ion:105 Resp: 237066

Ion Ratio Lower Upper

105 100

120 46.1 23.1 69.2

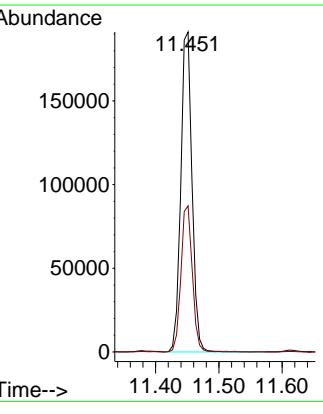


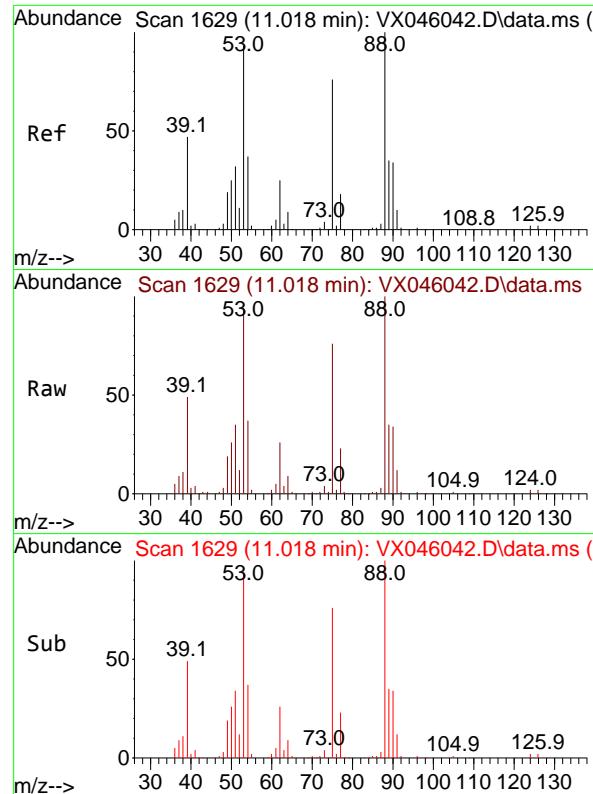


#81  
trans-1,4-Dichloro-2-butene  
Concen: 38.445 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

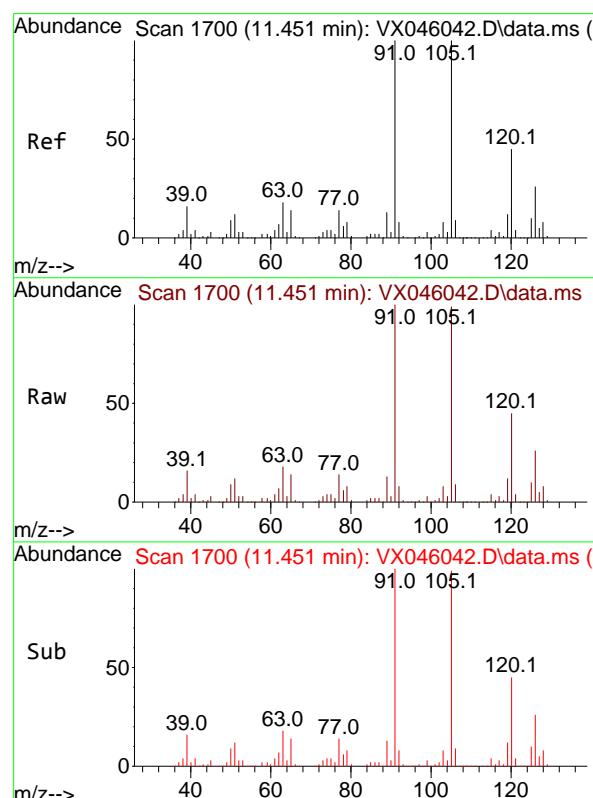

#82  
4-Chlorotoluene  
Concen: 37.880 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 91 Resp: 233172  
Ion Ratio Lower Upper  
91 100  
126 26.5 13.3 39.8





#83

tert-Butylbenzene

Concen: 38.622 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

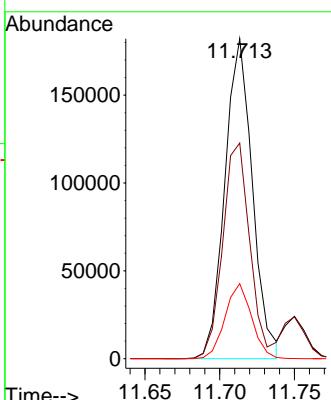

#84

1,2,4-Trimethylbenzene

Concen: 38.946 ug/l


RT: 11.750 min Scan# 1749


Delta R.T. 0.000 min

Lab File: VX046042.D


Acq: 05 May 2025 11:58

Tgt	Ion:105	Resp: 239433
Ion	Ratio	Lower Upper
105	100	
120	42.4	21.2 63.6

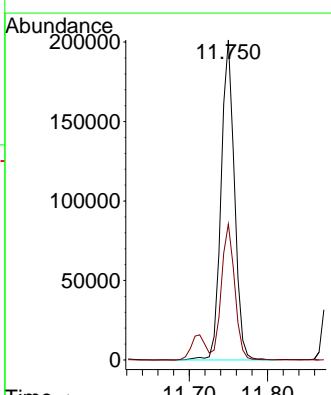



Abundance Scan 1772 (11.890 min): VX046042.D\data.ms (-)

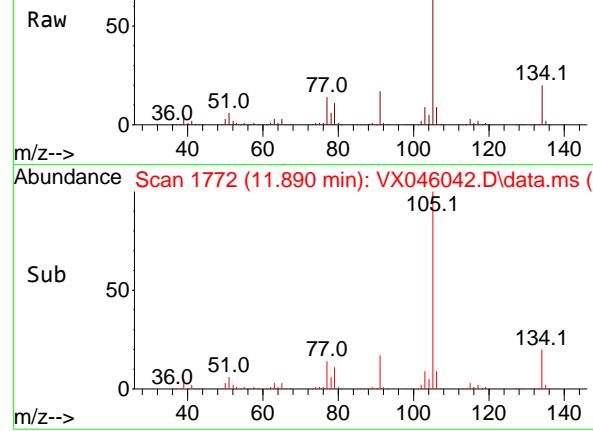

#85

sec-Butylbenzene

Concen: 38.786 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

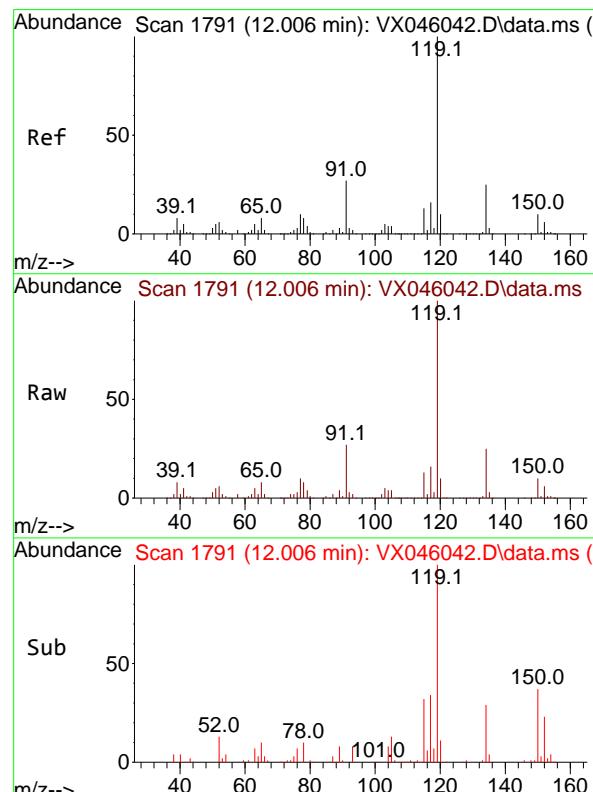

#86

p-Isopropyltoluene

Concen: 39.879 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58


Tgt Ion:119 Resp: 241658


Ion Ratio Lower Upper

119 100

134 25.0 12.5 37.5

91 27.6 13.8 41.4

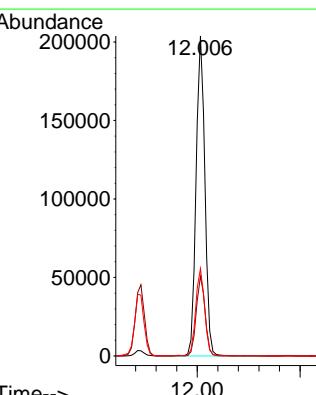

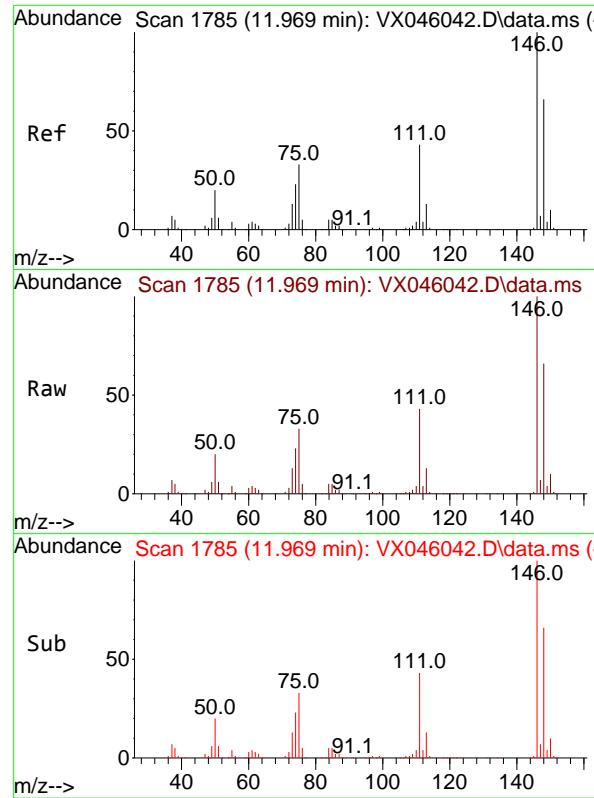

#87

1,3-Dichlorobenzene

Concen: 36.199 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

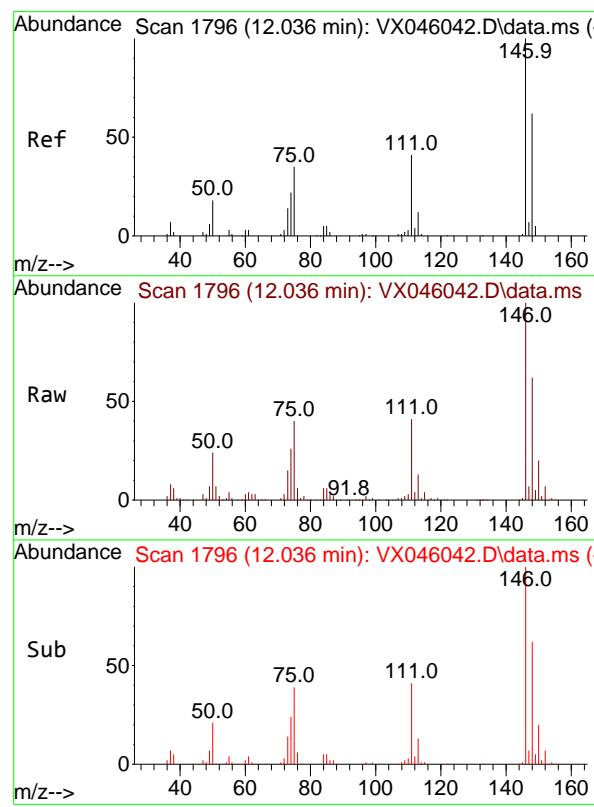

#88

1,4-Dichlorobenzene

Concen: 36.763 ug/l

RT: 12.036 min Scan# 1796


Delta R.T. 0.000 min




Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt Ion:146 Resp: 115097

Ion	Ratio	Lower	Upper
146	100		
111	42.6	21.3	63.9
148	63.7	31.9	95.5





#89

n-Butylbenzene

Concen: 40.603 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58





Instrument : MSVOA\_X

ClientSampleId : VSTDICCC050

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#90

Hexachloroethane

Concen: 37.534 ug/l


RT: 12.536 min Scan# 1878


Delta R.T. 0.000 min

Lab File: VX046042.D

Acq: 05 May 2025 11:58

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
	117	100	42314		
	201	63.1	31.6	94.7	

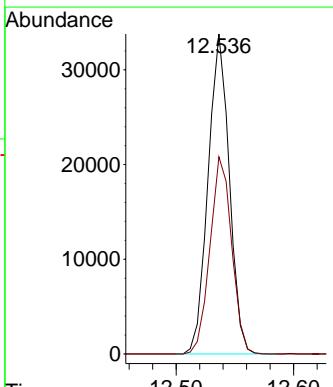


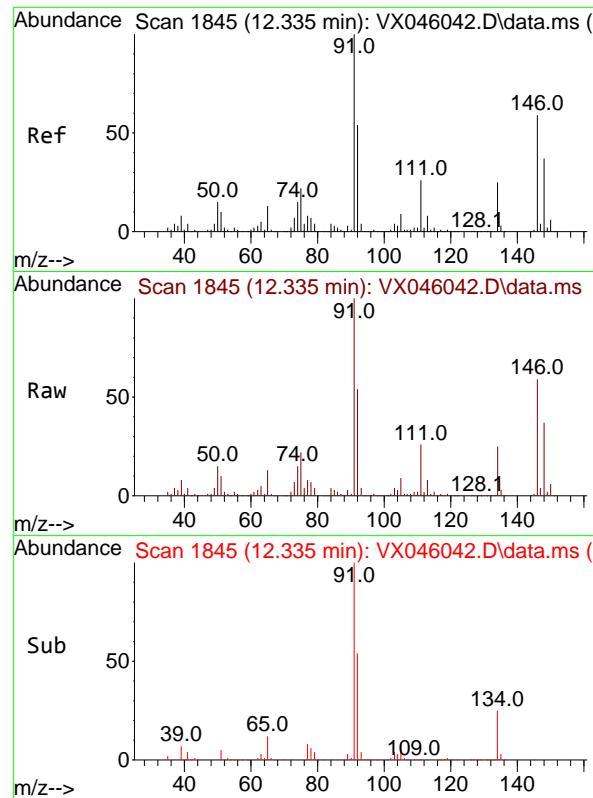


#91  
1,2-Dichlorobenzene  
Concen: 37.047 ug/l  
RT: 12.335 min Scan# 115280  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

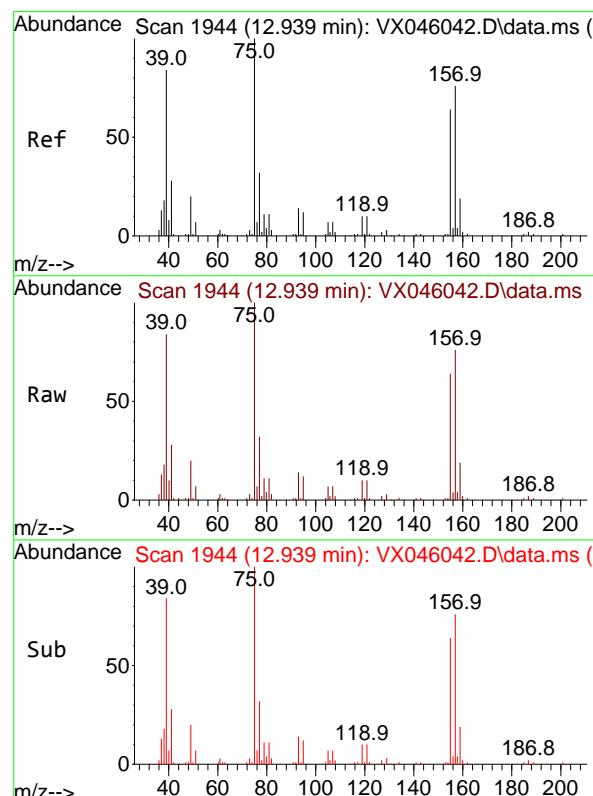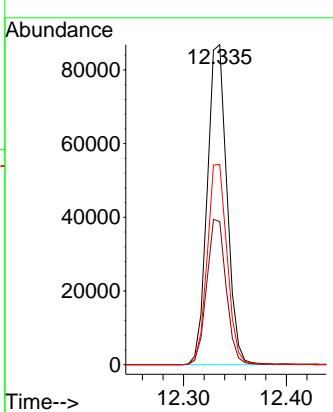

#92  
1,2-Dibromo-3-Chloropropane  
Concen: 36.496 ug/l  
RT: 12.939 min Scan# 1944  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion: 75 Resp: 21909  
Ion Ratio Lower Upper  
75 100  
155 69.9 34.9 104.8  
157 87.6 43.8 131.4




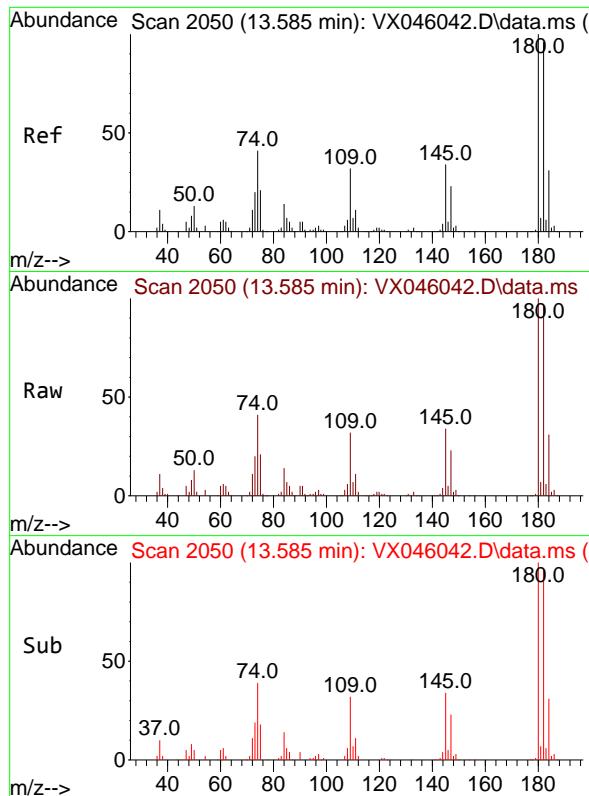


#93  
1,2,4-Trichlorobenzene  
Concen: 39.117 ug/l  
RT: 13.585 min Scan#  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

2 **Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICCC050


## **Manual Integrations APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

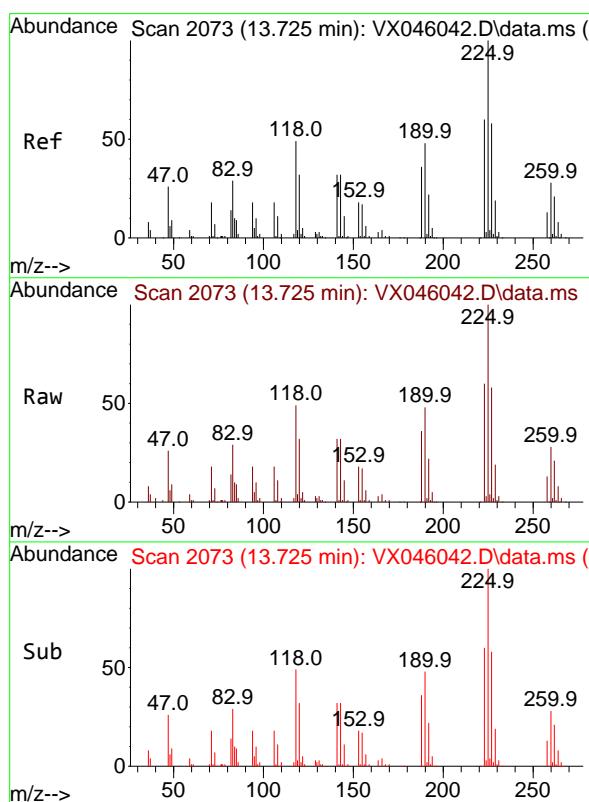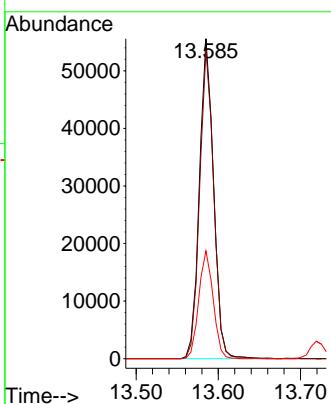

#94  
Hexachlorobutadiene  
Concen: 36.395 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt	Ion:225	Resp:	29007
Ion	Ratio	Lower	Upper
225	100		
223	61.6	30.8	92.4
227	61.8	30.9	92.7

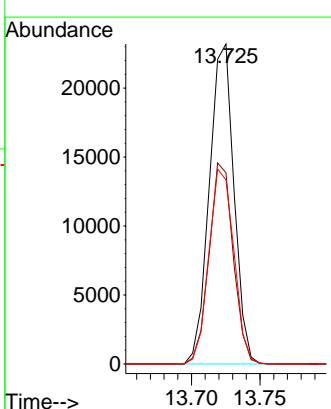


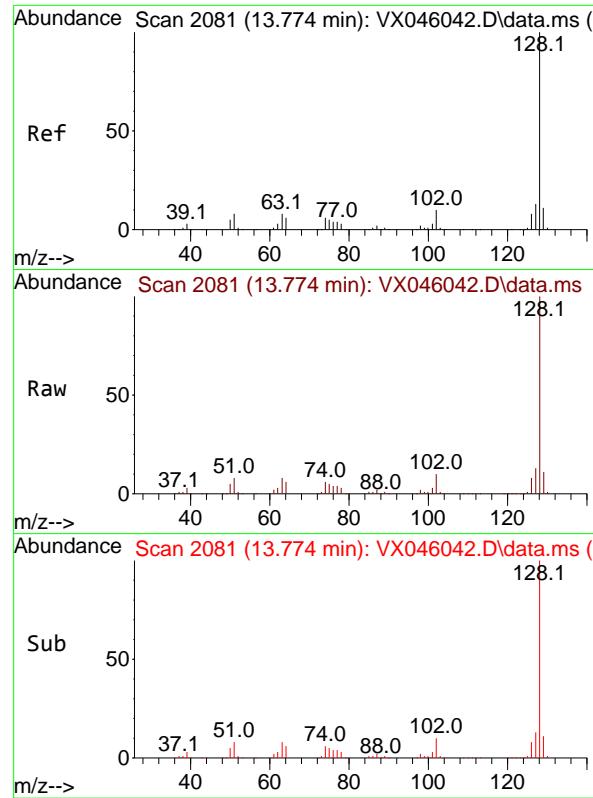


#95  
Naphthalene  
Concen: 39.575 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Instrument : MSVOA\_X  
ClientSampleId : VSTDICCC050


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

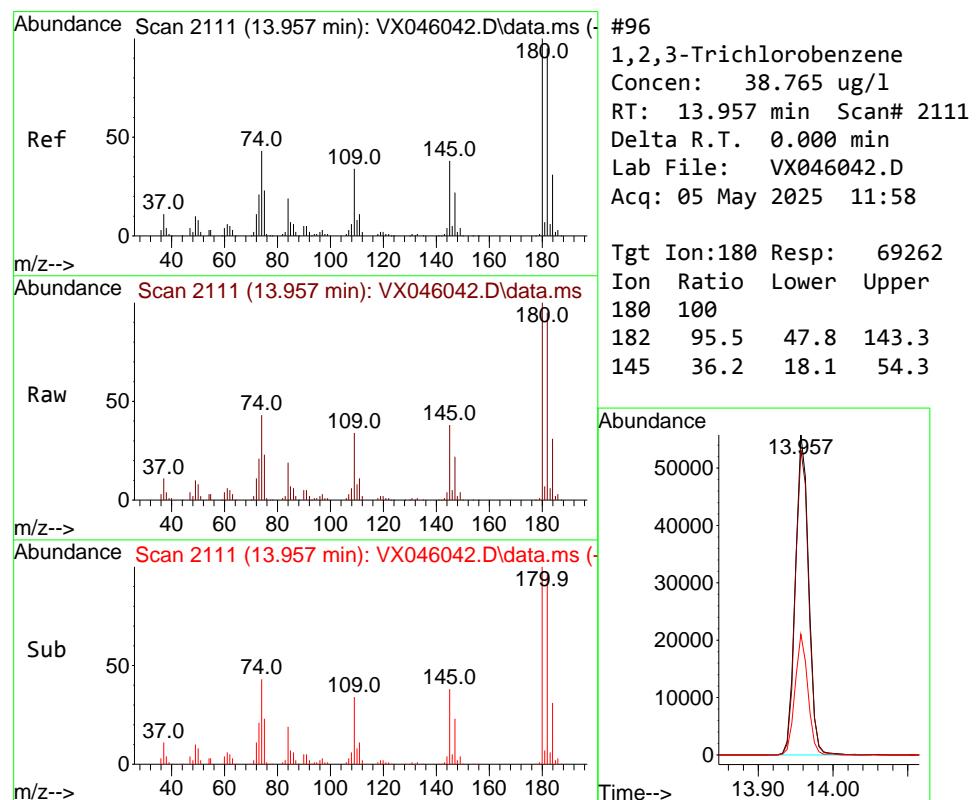

#96  
1, 2, 3-Trichlorobenzene  
Concen: 38.765 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046042.D  
Acq: 05 May 2025 11:58

Tgt Ion:180 Resp: 69262  
Ion Ratio Lower Upper  
180 100  
182 95.5 47.8 143.3  
145 36.2 18.1 54.3



Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046043.D  
 Acq On : 05 May 2025 12:21  
 Operator : JC/MD  
 Sample : VSTDICC100  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC100

Quant Time: May 06 06:10:38 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	87028	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	152958	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	135214	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	66369	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	161877	62.526	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 125.060%	#	
35) Dibromofluoromethane	5.379	113	111455	65.006	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 130.020%	#	
50) Toluene-d8	8.647	98	387230	67.031	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 134.060%	#	
62) 4-Bromofluorobenzene	11.079	95	153085	72.818	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 145.640%	#	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	149508	77.828	ug/l	99
3) Chloromethane	1.307	50	136937	72.392	ug/l	98
4) Vinyl Chloride	1.374	62	126609	76.398	ug/l	98
5) Bromomethane	1.593	94	59246	70.507	ug/l	99
6) Chloroethane	1.660	64	57332	67.148	ug/l	99
7) Trichlorofluoromethane	1.867	101	171042	67.754	ug/l	99
8) Diethyl Ether	2.136	74	58762	70.807	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.319	101	109520	72.604	ug/l	99
10) Methyl Iodide	2.440	142	138045	77.943	ug/l	100
11) Tert butyl alcohol	2.995	59	125094	405.394	ug/l	100
12) 1,1-Dichloroethene	2.306	96	105566	71.884	ug/l	96
13) Acrolein	2.239	56	134456	375.132	ug/l	99
14) Allyl chloride	2.660	41	206519	74.419	ug/l	98
15) Acrylonitrile	3.068	53	331142	358.723	ug/l	97
16) Acetone	2.386	43	314383	354.936	ug/l	98
17) Carbon Disulfide	2.501	76	264956	77.867	ug/l	100
18) Methyl Acetate	2.703	43	147014	69.531	ug/l	96
19) Methyl tert-butyl Ether	3.117	73	378113	73.818	ug/l	100
20) Methylene Chloride	2.782	84	120270	67.030	ug/l	96
21) trans-1,2-Dichloroethene	3.087	96	106606	71.109	ug/l	99
22) Diisopropyl ether	3.763	45	399494	77.048	ug/l	90
23) Vinyl Acetate	3.721	43	1811550	395.363	ug/l	100
24) 1,1-Dichloroethane	3.605	63	219759	72.114	ug/l	99
25) 2-Butanone	4.556	43	485448	379.704	ug/l	100
26) 2,2-Dichloropropane	4.464	77	174579	75.621	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	128454	71.056	ug/l	99
28) Bromochloromethane	4.891	49	103602	63.932	ug/l	100
29) Tetrahydrofuran	5.001	42	305757	368.234	ug/l	99
30) Chloroform	5.086	83	222253	70.180	ug/l	95
31) Cyclohexane	5.458	56	196302	76.428	ug/l	99
32) 1,1,1-Trichloroethane	5.373	97	201112	73.635	ug/l	98
36) 1,1-Dichloropropene	5.690	75	147873	74.285	ug/l	99
37) Ethyl Acetate	4.714	43	186215	74.565	ug/l	99
38) Carbon Tetrachloride	5.672	117	168946	73.875	ug/l	99
39) Methylcyclohexane	7.372	83	191941	76.952	ug/l	96
40) Benzene	6.031	78	440885	71.457	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046043.D  
 Acq On : 05 May 2025 12:21  
 Operator : JC/MD  
 Sample : VSTDICC100  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC100

Quant Time: May 06 06:10:38 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	104863	75.574	ug/1	98
42) 1,2-Dichloroethane	6.080	62	187036	73.318	ug/1	99
43) Isopropyl Acetate	6.342	43	300491	78.714	ug/1	100
44) Trichloroethene	7.123	130	105628	72.420	ug/1	98
45) 1,2-Dichloropropane	7.427	63	112554	73.420	ug/1	100
46) Dibromomethane	7.574	93	85728	70.938	ug/1	100
47) Bromodichloromethane	7.818	83	175301	74.845	ug/1	99
48) Methyl methacrylate	7.689	41	153093	78.101	ug/1	99
49) 1,4-Dioxane	7.659	88	57313	1470.687	ug/1	99
51) 4-Methyl-2-Pentanone	8.573	43	963319	384.740	ug/1	100
52) Toluene	8.714	92	270763	74.010	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	169863	86.372	ug/1	100
54) cis-1,3-Dichloropropene	8.366	75	184134	80.264	ug/1	95
55) 1,1,2-Trichloroethane	9.147	97	107264	72.543	ug/1	99
56) Ethyl methacrylate	9.116	69	188717	82.359	ug/1	99
57) 1,3-Dichloropropane	9.305	76	187649	71.590	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.238	63	463169	449.791	ug/1	100
59) 2-Hexanone	9.433	43	729602	383.945	ug/1	100
60) Dibromochloromethane	9.518	129	127012	78.918	ug/1	98
61) 1,2-Dibromoethane	9.610	107	112669	74.200	ug/1	98
64) Tetrachloroethene	9.268	164	93195	67.493	ug/1	96
65) Chlorobenzene	10.079	112	293284	70.490	ug/1	100
66) 1,1,1,2-Tetrachloroethane	10.159	131	103177	74.349	ug/1	99
67) Ethyl Benzene	10.189	91	535122	75.444	ug/1	99
68) m/p-Xylenes	10.299	106	389935	152.181	ug/1	99
69) o-Xylene	10.640	106	190833	73.890	ug/1	97
70) Styrene	10.652	104	328195	79.411	ug/1	100
71) Bromoform	10.799	173	84353	80.927	ug/1 #	98
73) Isopropylbenzene	10.957	105	514528	71.083	ug/1	100
74) N-amyl acetate	10.841	43	274553	76.073	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	170481	66.207	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	150182m	54.277	ug/1	
77) Bromobenzene	11.195	156	117151	69.959	ug/1	99
78) n-propylbenzene	11.305	91	608332	74.974	ug/1	100
79) 2-Chlorotoluene	11.360	91	372392	68.100	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	432096	71.903	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	54398	81.820	ug/1	93
82) 4-Chlorotoluene	11.451	91	432053	71.890	ug/1	100
83) tert-Butylbenzene	11.713	119	432011	73.197	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	442728	73.758	ug/1	100
85) sec-Butylbenzene	11.890	105	543597	74.188	ug/1	100
86) p-Isopropyltoluene	12.006	119	457898	77.393	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	219753	70.449	ug/1	99
88) 1,4-Dichlorobenzene	12.036	146	217613	71.190	ug/1	99
89) n-Butylbenzene	12.329	91	416602	80.996	ug/1	100
90) Hexachloroethane	12.536	117	82528	74.978	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	216834	71.367	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	43673	74.512	ug/1	98
93) 1,2,4-Trichlorobenzene	13.585	180	137430	82.605	ug/1	98
94) Hexachlorobutadiene	13.725	225	55494	71.314	ug/1	98
95) Naphthalene	13.774	128	489778	80.842	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	139525	79.981	ug/1	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046043.D  
 Acq On : 05 May 2025 12:21  
 Operator : JC/MD  
 Sample : VSTDICC100  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDICC100**

Quant Time: May 06 06:10:38 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046043.D  
Acq On : 05 May 2025 12:21  
Operator : JC/MD  
Sample : VSTDIICC100  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC100

## Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

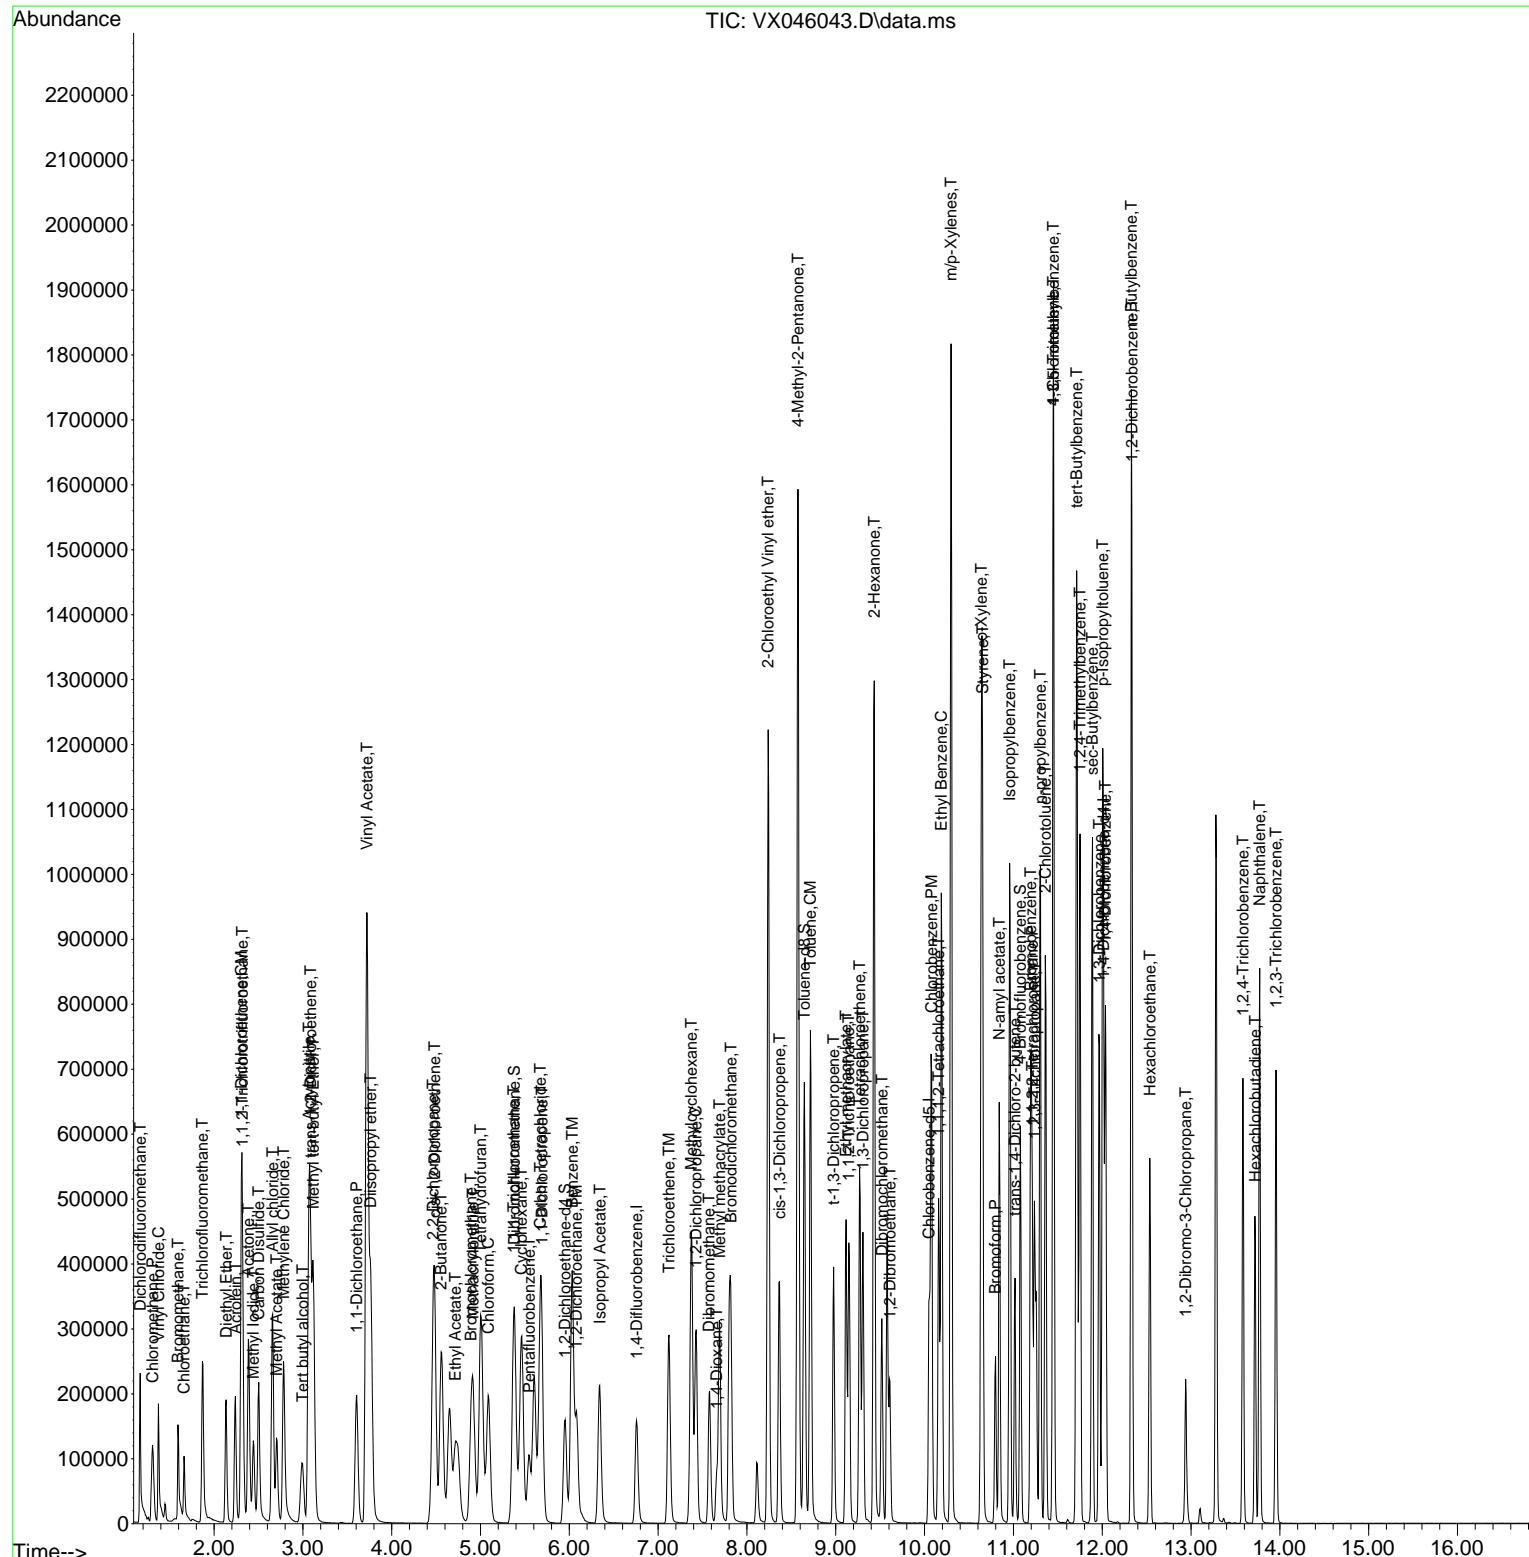



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

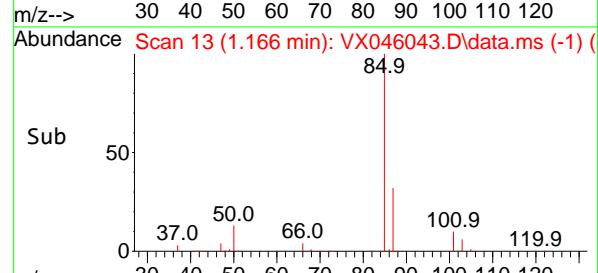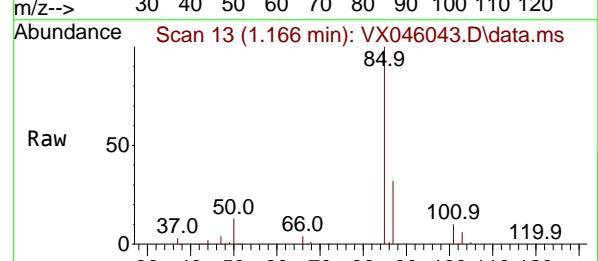

#2

Dichlorodifluoromethane

Concen: 77.828 ug/l

RT: 1.166 min Scan# 13

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21







Tgt Ion: 85 Resp: 149508

Ion Ratio Lower Upper

85 100

87 32.0 15.7 47.1

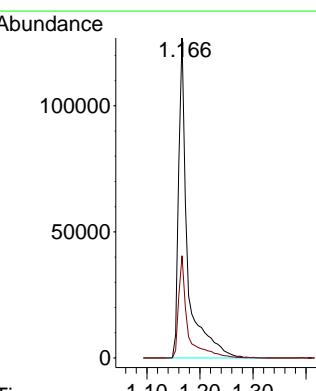

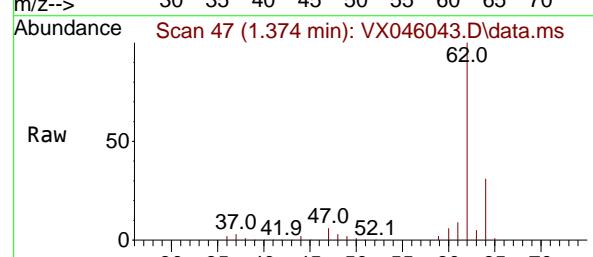

#3

Chloromethane

Concen: 72.392 ug/l

RT: 1.307 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**
Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

#4

Vinyl Chloride


Concen: 76.398 ug/l




RT: 1.374 min Scan# 47

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 62 Resp: 126609  
Ion Ratio Lower Upper  
62 100  
64 30.6 25.2 37.8



#5

Bromomethane

Concen: 70.507 ug/l

RT: 1.593 min Scan# 8

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

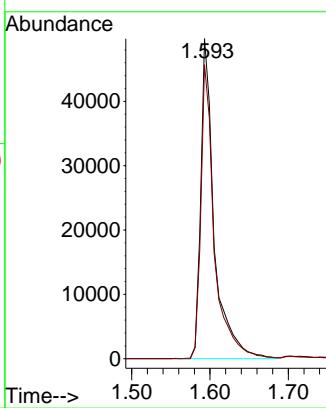

#6

Chloroethane

Concen: 67.148 ug/l


RT: 1.660 min Scan# 94




Delta R.T. -0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 64 Resp: 57332  
 Ion Ratio Lower Upper  
 64 100  
 66 30.8 24.3 36.5

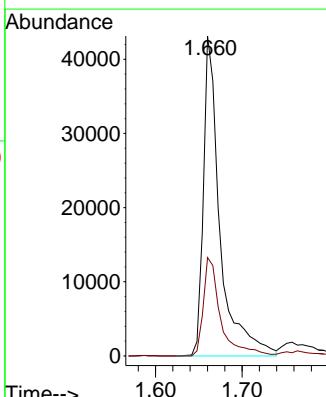

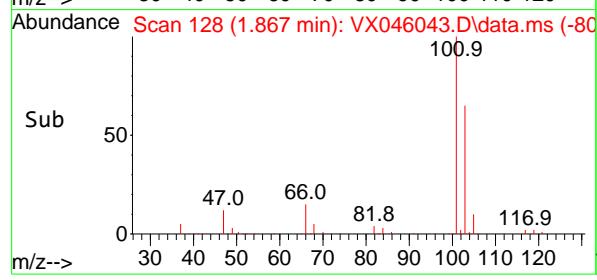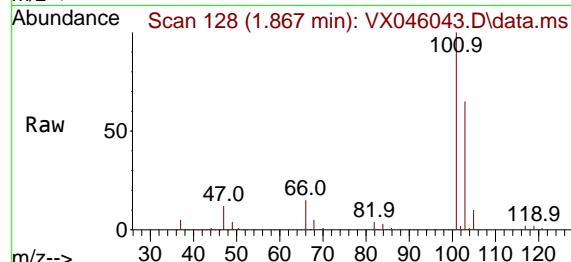





#7

Trichlorofluoromethane  
Concen: 67.754 ug/l  
RT: 1.867 min Scan# 128  
Delta R.T. -0.006 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025




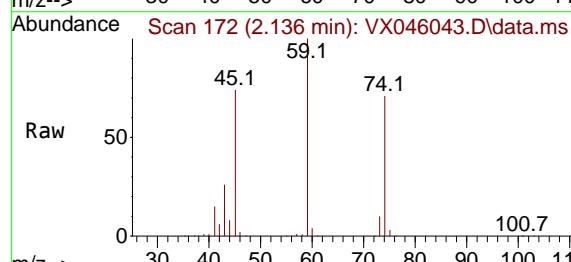

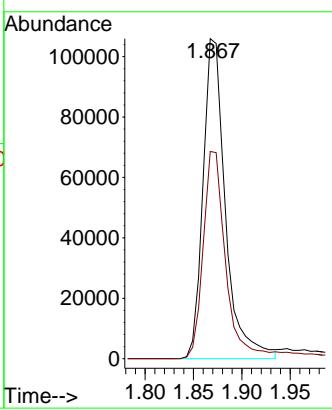


#8

Diethyl Ether  
Concen: 70.807 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion: 74 Resp: 58762  
Ion Ratio Lower Upper  
74 100  
45 110.1 54.9 164.8

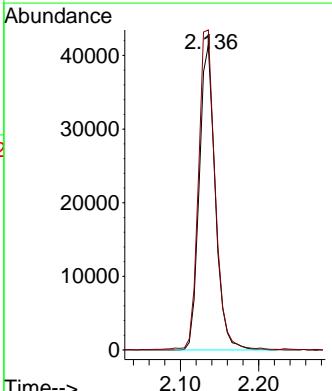

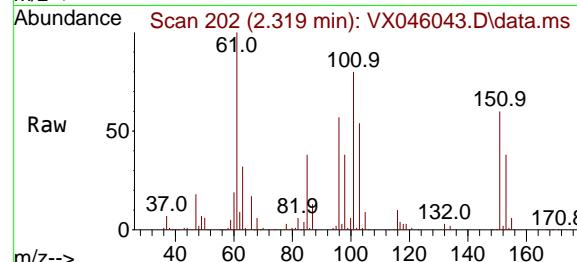

#9

1,1,2-Trichlorotrifluoroethane

Concen: 72.604 ug/l

RT: 2.319 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100


### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

2.319

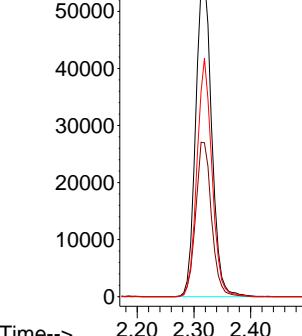

#10

Methyl Iodide

Concen: 77.943 ug/l

RT: 2.440 min Scan# 222

Delta R.T. -0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion:142 Resp: 138045


Ion Ratio Lower Upper

142	100		
127	52.0	41.7	62.5
141	14.5	11.5	17.3

Abundance

2.440

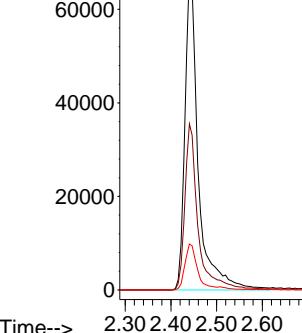

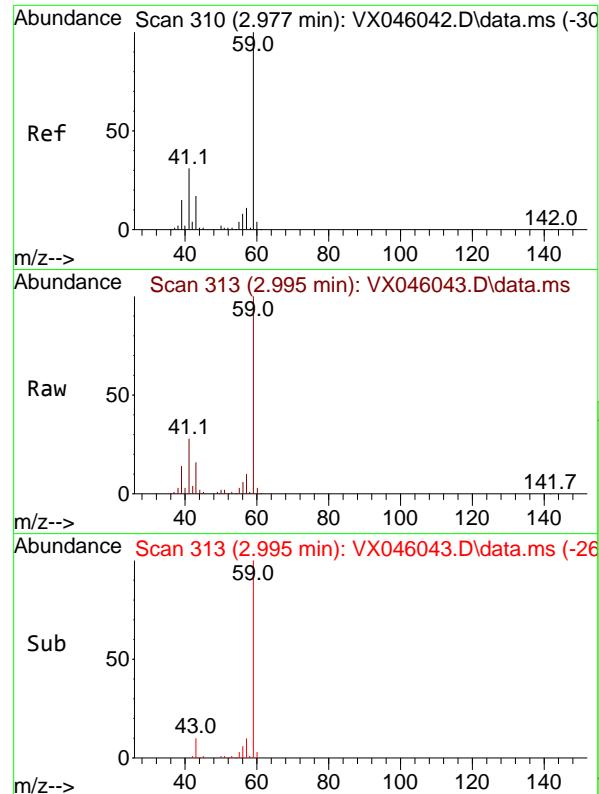



#11

Tert butyl alcohol  
Concen: 405.394 ug/l  
RT: 2.995 min Scan# 3  
Delta R.T. 0.018 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

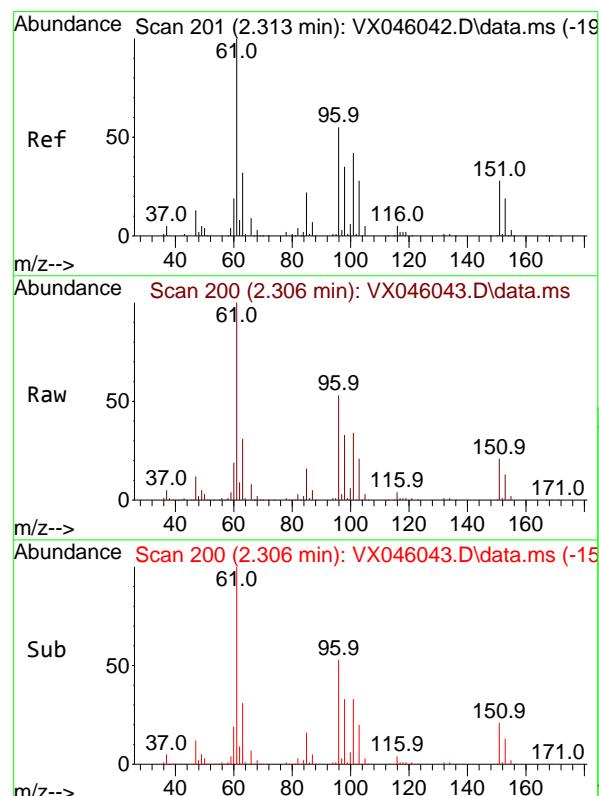


#12

1,1-Dichloroethene  
Concen: 71.884 ug/l  
RT: 2.306 min Scan# 200  
Delta R.T. -0.006 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion: 96 Resp: 105566  
Ion Ratio Lower Upper  
96 100  
61 189.9 146.2 219.2  
98 63.3 51.0 76.6





#13

Acrolein

Concen: 375.132 ug/l

RT: 2.239 min Scan# 188

Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

Abundance Scan 189 (2.239 min): VX046043.D\data.ms

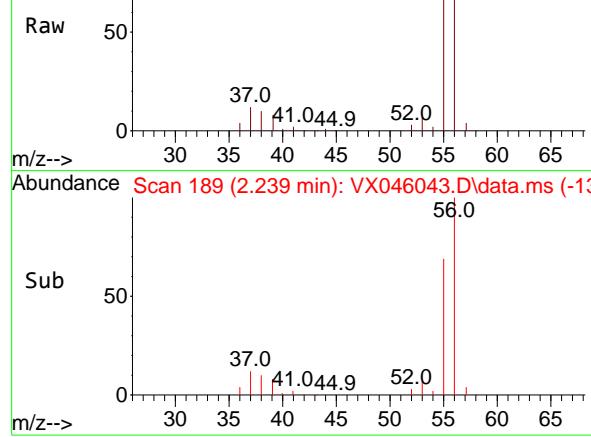

Tgt Ion: 56 Resp: 134450

Ion Ratio Lower Upper

56 100



55 71.3 56.2 84.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

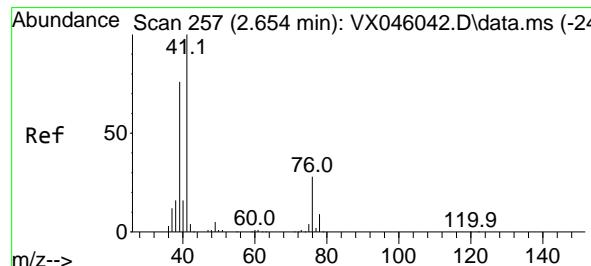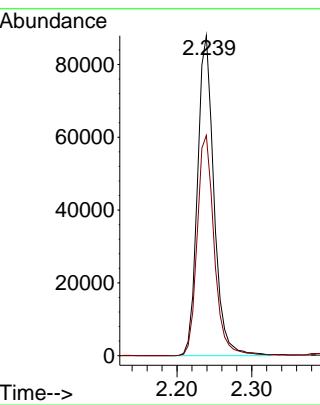

#14

Allyl chloride


Concen: 74.419 ug/l

RT: 2.660 min Scan# 258

Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

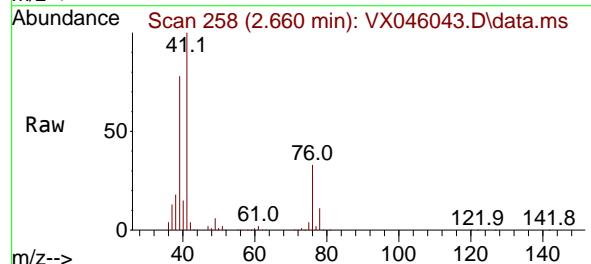



Tgt Ion: 41 Resp: 206519







Ion Ratio Lower Upper

41 100

39 73.8 60.6 90.8

76 31.4 24.9 37.3

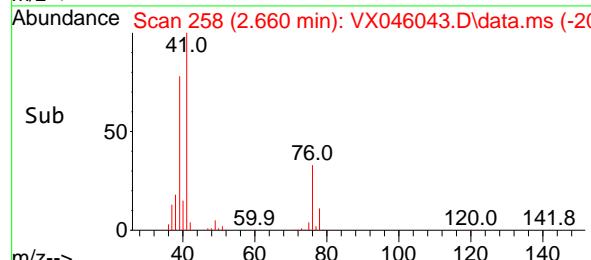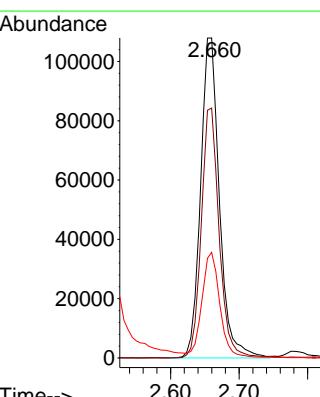

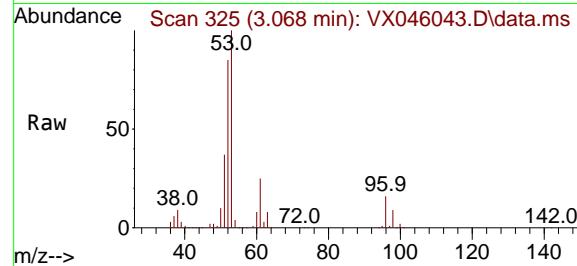

#15

Acrylonitrile

Concen: 358.723 ug/l

RT: 3.068 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

Tgt Ion: 53 Resp: 33114:

Ion Ratio Lower Upper

53 100

52 84.7 65.3 97.9


51 37.9 29.8 44.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#16

Acetone

Concen: 354.936 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21







Tgt Ion: 43 Resp: 314383

Ion Ratio Lower Upper

43 100

58 27.6 21.2 31.8





#17

Carbon Disulfide

Concen: 77.867 ug/l

RT: 2.501 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

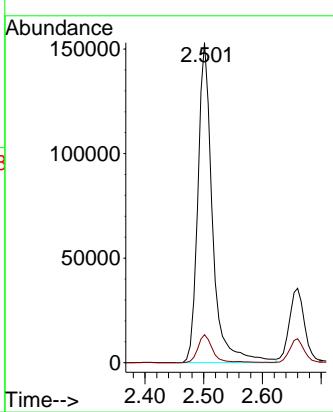

#18

Methyl Acetate

Concen: 69.531 ug/l

RT: 2.703 min Scan# 265

Delta R.T. -0.000 min


Lab File: VX046043.D







Acq: 05 May 2025 12:21

Tgt Ion: 43 Resp: 147014

Ion Ratio Lower Upper

43	100
74	22.6 16.7 25.1



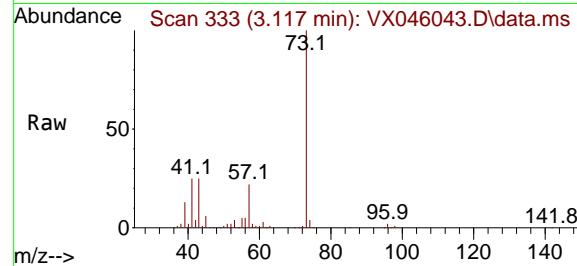


#19

Methyl tert-butyl Ether  
Concen: 73.818 ug/l  
RT: 3.117 min Scan# 3  
Delta R.T. 0.006 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



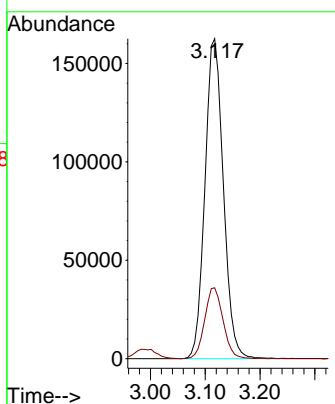


#20

Methylene Chloride  
Concen: 67.030 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion: 84 Resp: 120270  
Ion Ratio Lower Upper  
84 100  
49 136.4 113.9 170.9  
51 41.1 33.5 50.3  
86 64.0 53.8 80.8

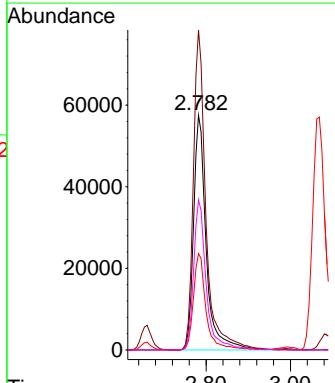

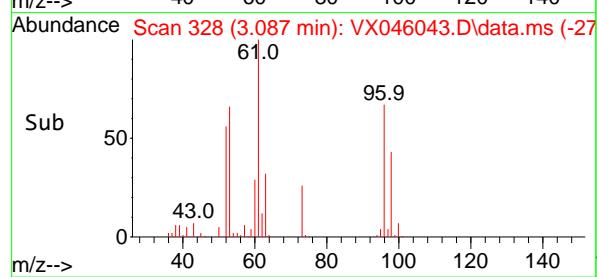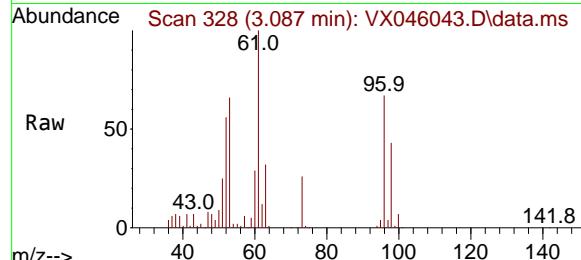

#21

trans-1,2-Dichloroethene

Concen: 71.109 ug/l

RT: 3.087 min Scan# 328

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

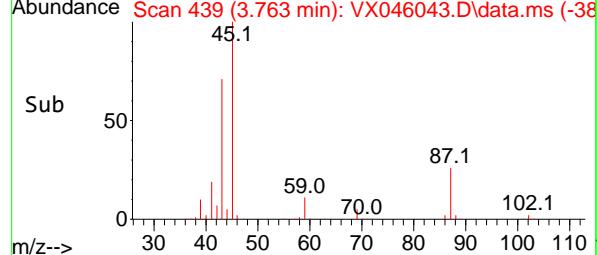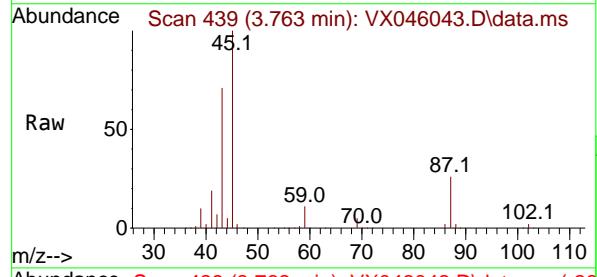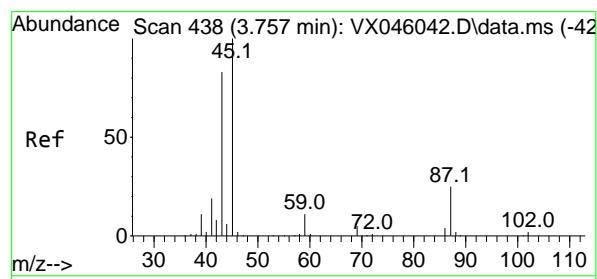

#22

Diisopropyl ether

Concen: 77.048 ug/l

RT: 3.763 min Scan# 439

Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 45 Resp: 399494


Ion Ratio Lower Upper




45 100

43 71.2 66.6 100.0

87 25.7 19.8 29.6

59 11.0 8.6 12.8

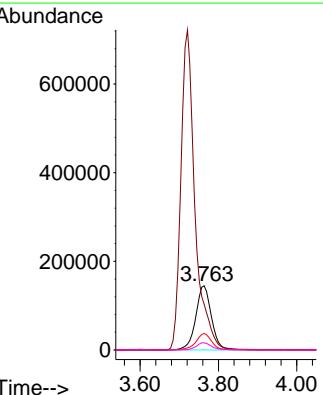

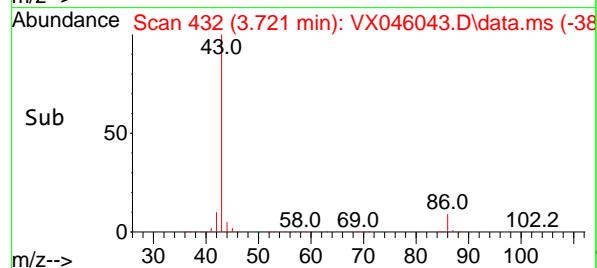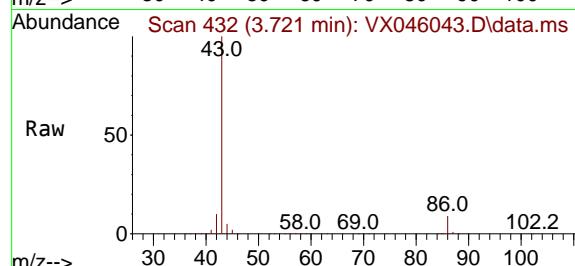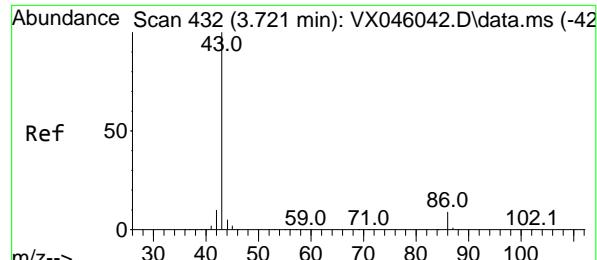

#23

**Vinyl Acetate**

Concen: 395.363 ug/l

RT: 3.721 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

Tgt Ion: 43 Resp: 1811550

Ion Ratio Lower Upper





43 100

86 9.5 7.5 11.3

**Manual Integrations****APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

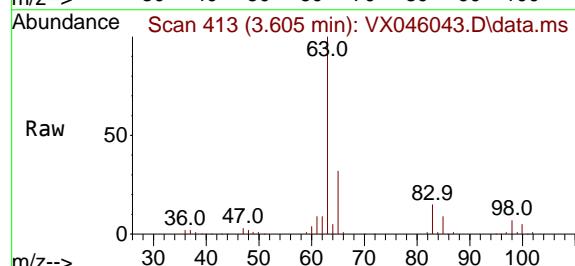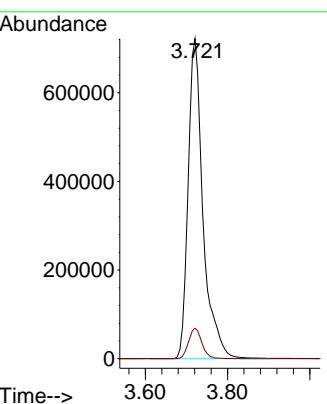

#24

**1,1-Dichloroethane**

Concen: 72.114 ug/l

RT: 3.605 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion: 63 Resp: 219759


Ion Ratio Lower Upper

63 100

98 6.8 3.6 10.8


100 4.5 2.1 6.3

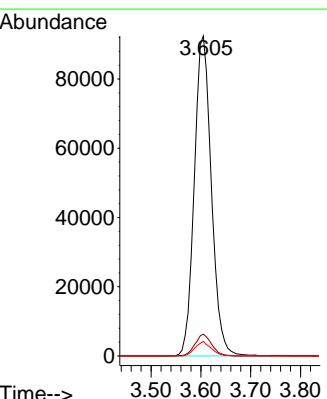



#25  
2-Butanone  
Concen: 379.704 ug/l  
RT: 4.556 min Scan# 569  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100




Tgt Ion: 43 Resp: 485448  
Ion Ratio Lower Upper  
43 100  
72 23.1 18.4 27.6

Manual Integrations  
APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

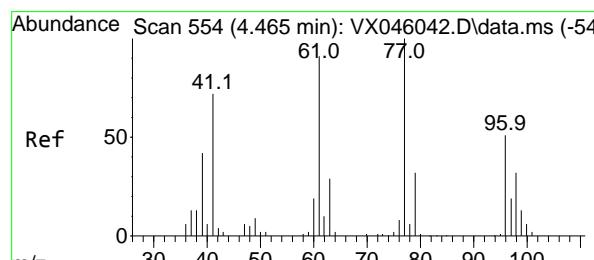
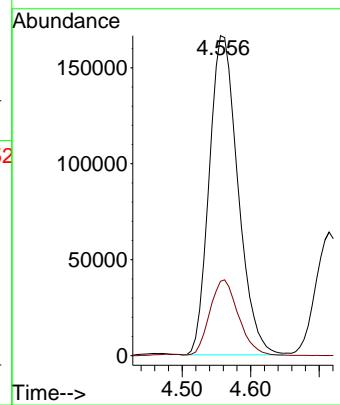
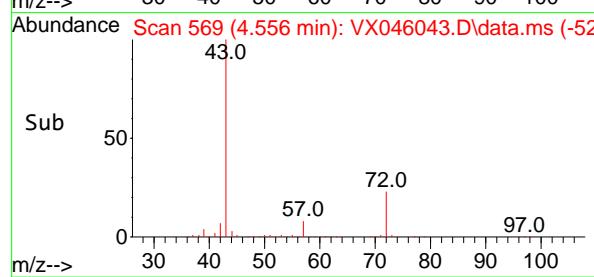


#26  
2,2-Dichloropropane  
Concen: 75.621 ug/l  
RT: 4.464 min Scan# 554  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

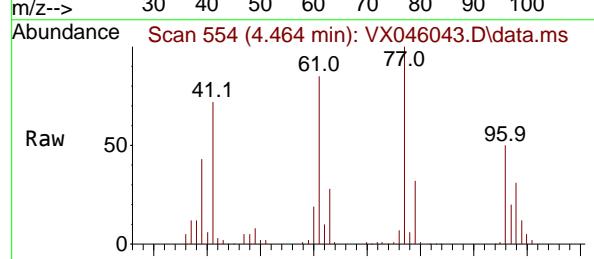

Tgt Ion: 77 Resp: 174579  
Ion Ratio Lower Upper  
77 100  
97 21.1 10.5 31.5

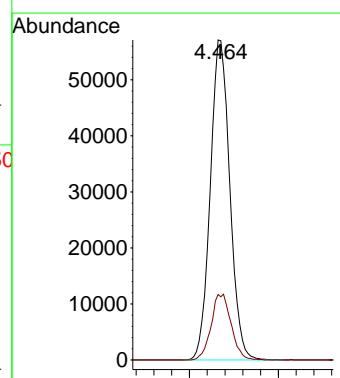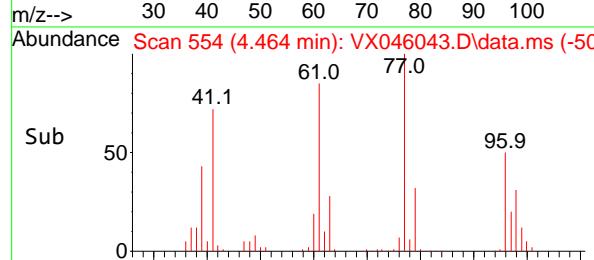



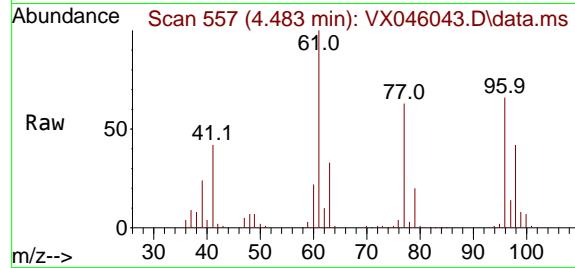



#27  
cis-1,2-Dichloroethene  
Concen: 71.056 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

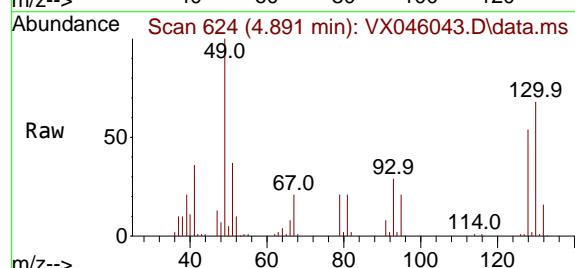


#28  
Bromochloromethane  
Concen: 63.932 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21


Tgt Ion: 49 Resp: 103602  
Ion Ratio Lower Upper  
49 100  
129 1.8 0.0 4.0  
130 70.1 56.2 84.2




Abundance Scan 642 (5.001 min): VX046042.D\data.ms (-63)

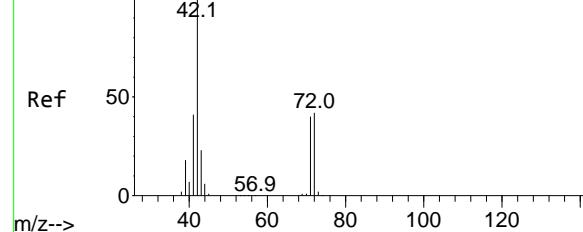

Abundance Scan 642 (5.001 min): VX046043.D\data.ms

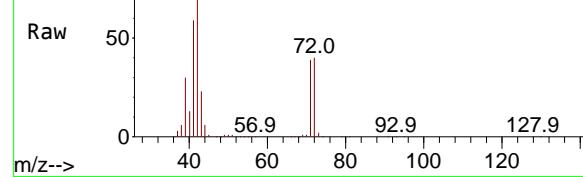

Abundance Scan 642 (5.001 min): VX046043.D\data.ms (-59)

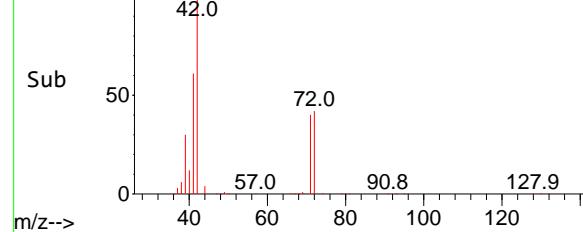

#29

Tetrahydrofuran

Concen: 368.234 ug/l

RT: 5.001 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :


VSTDICC100

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025


Abundance Scan 656 (5.087 min): VX046042.D\data.ms (-64)

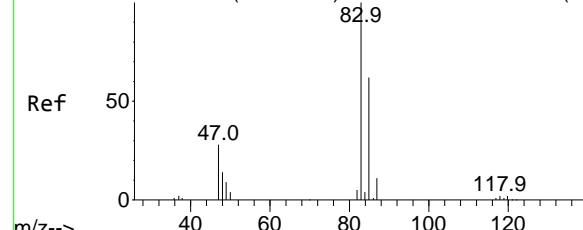

Abundance Scan 656 (5.086 min): VX046043.D\data.ms

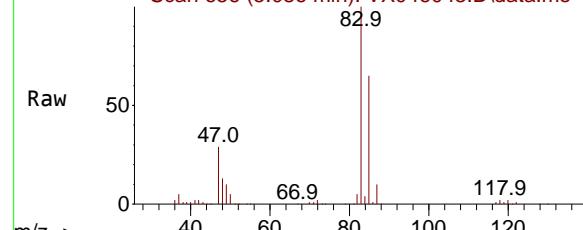

Abundance Scan 656 (5.086 min): VX046043.D\data.ms (-60)

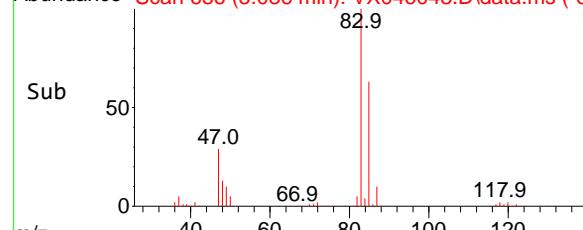

#30

Chloroform

Concen: 70.180 ug/l

RT: 5.086 min Scan# 656

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21


Tgt Ion: 83 Resp: 222253

Ion Ratio Lower Upper



83 100

85 65.1 49.3 73.9

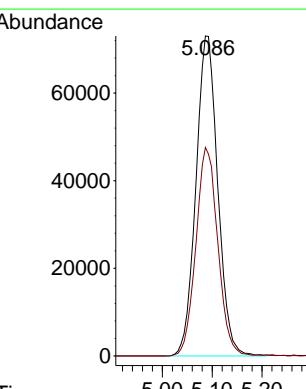




Abundance Scan 717 (5.458 min): VX046043.D\data.ms

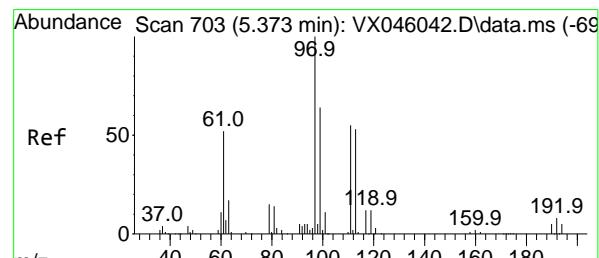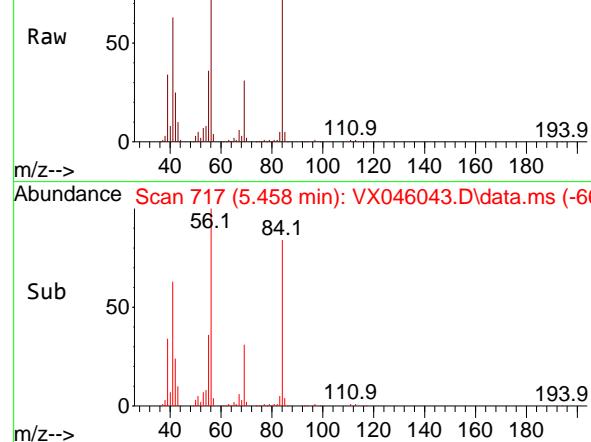

Abundance Scan 703 (5.373 min): VX046043.D\data.ms

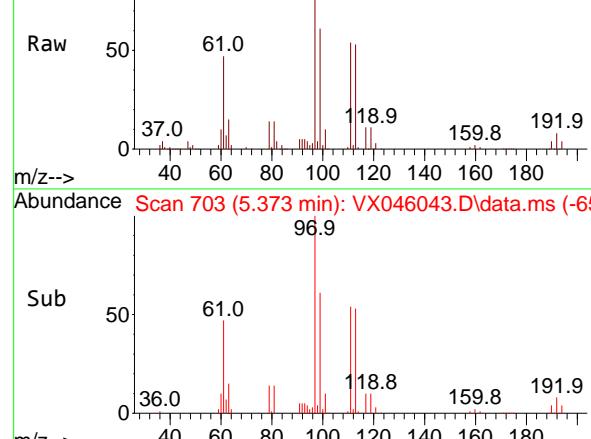

#31

Cyclohexane

Concen: 76.428 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#32

1,1,1-Trichloroethane

Concen: 73.635 ug/l

RT: 5.373 min Scan# 703

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion: 97 Resp: 201112




Ion Ratio Lower Upper

97 100

99 63.8 51.8 77.6

61 48.7 40.1 60.1

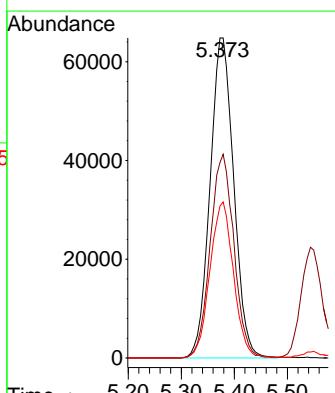

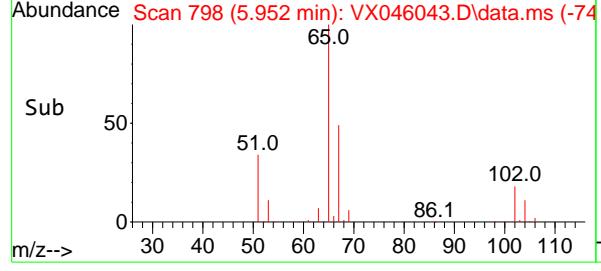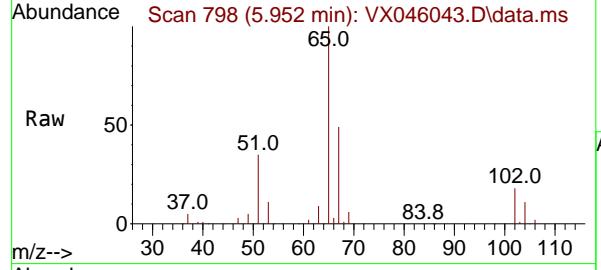

#33

1,2-Dichloroethane-d4

Concen: 62.526 ug/l

RT: 5.952 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

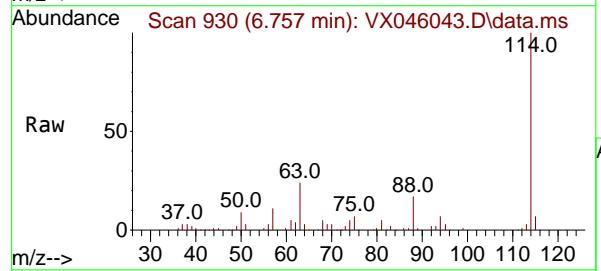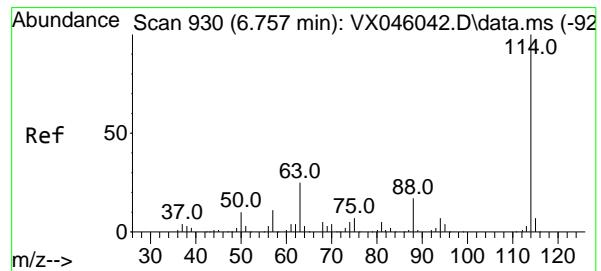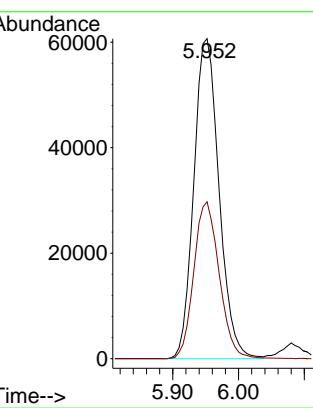

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l



RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt	Ion:	Resp:		
	114	152958	Lower	Upper
	100			
114	100			
63	24.3	0.0	49.2	
88	17.1	0.0	33.6	

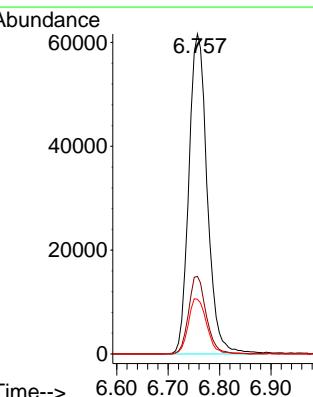

#35

1,4-Difluorobenzene







Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

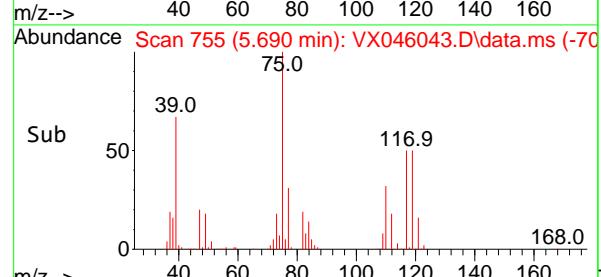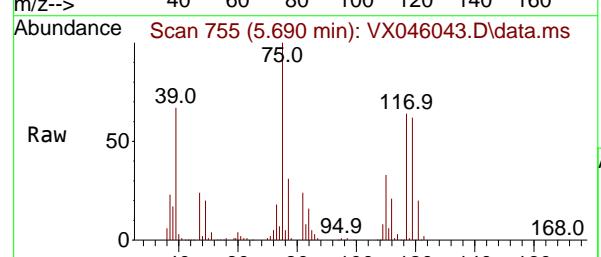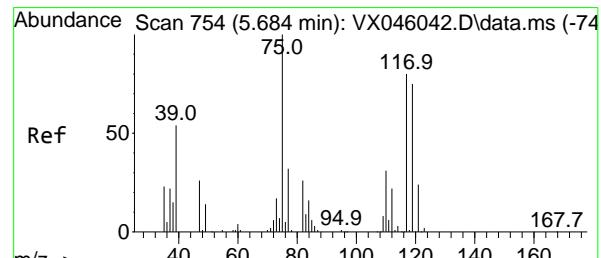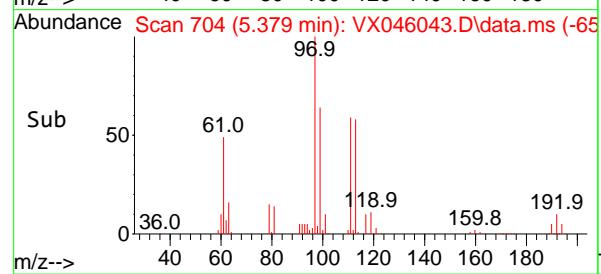

#35

Dibromofluoromethane

Concen: 65.006 ug/l

RT: 5.379 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

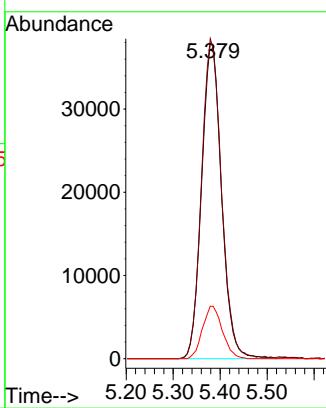

#36

1,1-Dichloropropene

Concen: 74.285 ug/l

RT: 5.690 min Scan# 755

Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion: 75 Resp: 147873







Ion Ratio Lower Upper

75 100

110 33.5 16.3 48.9

77 31.1 24.3 36.5

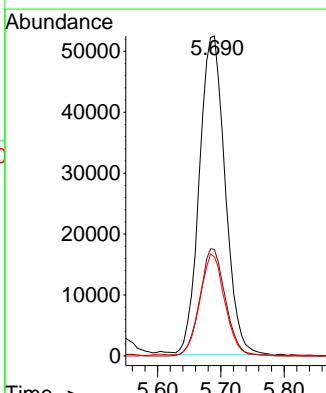

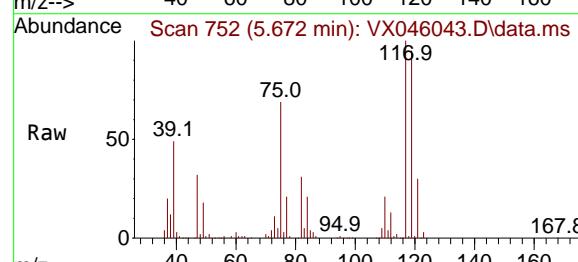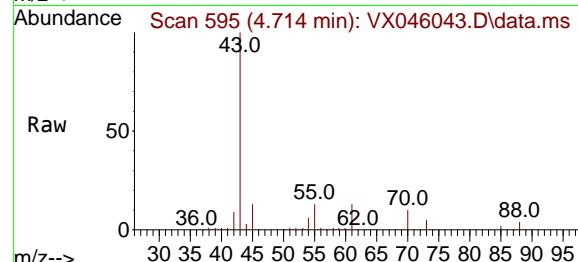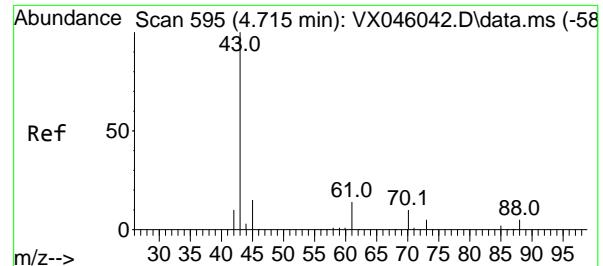

#37

**Ethyl Acetate**

Concen: 74.565 ug/l

RT: 4.714 min Scan# 5

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

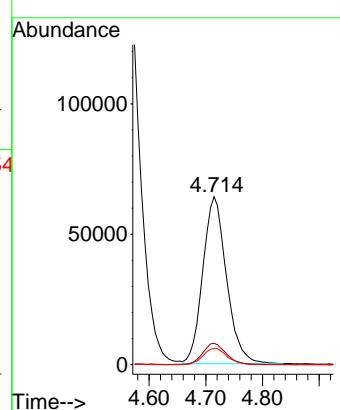

#38

**Carbon Tetrachloride**

Concen: 73.875 ug/l


RT: 5.672 min Scan# 752


Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt	Ion:117	Resp:	168946
Ion	Ratio	Lower	Upper
117	100		
119	95.0	75.2	112.8
121	29.6	24.2	36.4

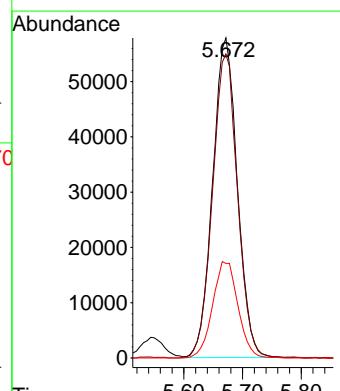

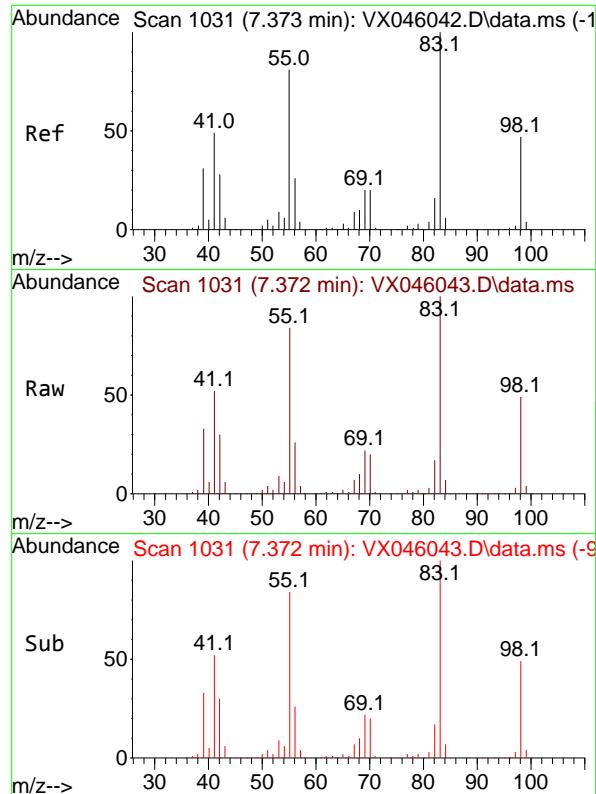

#39

Methylcyclohexane

Concen: 76.952 ug/l

RT: 7.372 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

Tgt Ion: 83 Resp: 19194

Ion Ratio Lower Upper

83 100

55 84.2 64.7 97.1

98 49.0 37.4 56.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

80000


60000

40000

20000


0

Time--&gt;



Abundance

Scan 811 (6.031 min): VX046042.D\data.ms (-79)



Tgt Ion: 78 Resp: 440885

Ion Ratio Lower Upper

78 100

77 24.6 19.0 28.4

Abundance


150000

100000

50000




0

Time--&gt;



VX046043.D 82X050525W.M

Q2200-VOCMS Group3



#41

Methacrylonitrile

Concen: 75.574 ug/l

RT: 4.916 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#42

1,2-Dichloroethane

Concen: 73.318 ug/l

RT: 6.080 min Scan# 819

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21


Tgt Ion: 62 Resp: 187036

Ion Ratio Lower Upper

62 100

98 7.4 0.0 15.2

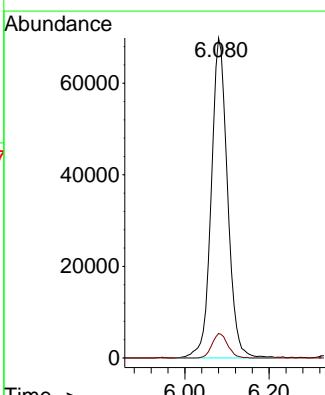



#43

Isopropyl Acetate

Concen: 78.714 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC100

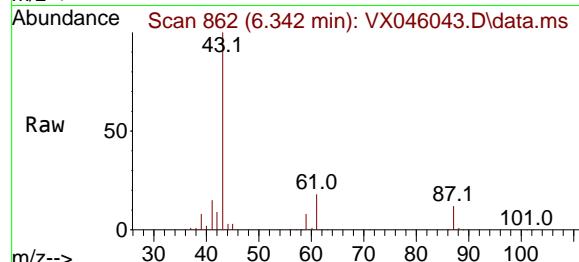

Tgt Ion: 43 Resp: 30049:

Ion Ratio Lower Upper

43 100

61 18.0 14.3 21.5




87 11.6 9.5 14.3

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

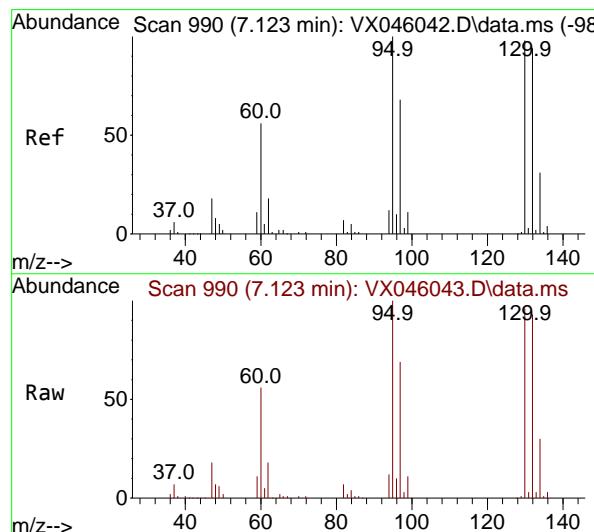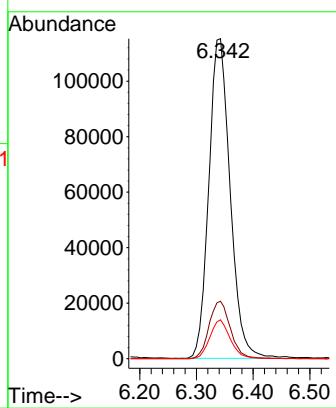

#44

Trichloroethene




Concen: 72.420 ug/l




RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

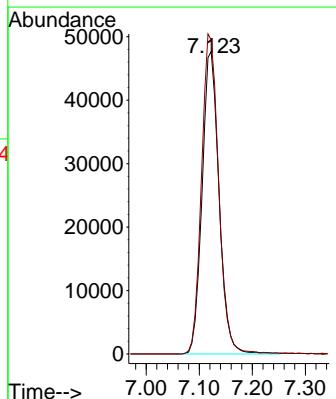



#45

1,2-Dichloropropane

Concen: 73.420 ug/l

RT: 7.427 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

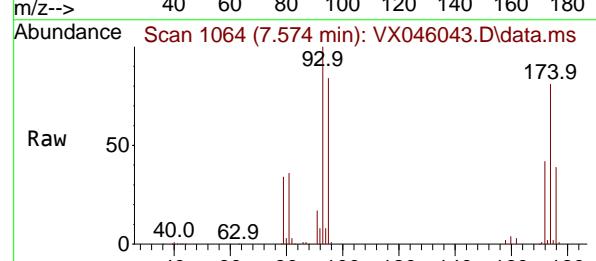

#46

Dibromomethane

Concen: 70.938 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 93 Resp: 85728

Ion Ratio Lower Upper

93 100

95 82.4 65.6 98.4

174 85.0 68.2 102.2

Abundance

40000

30000

20000

10000

0

7.50 7.60 7.70

Time--&gt;

Abundance

40000

30000


20000

10000

0

7.50 7.60 7.70

Time--&gt;

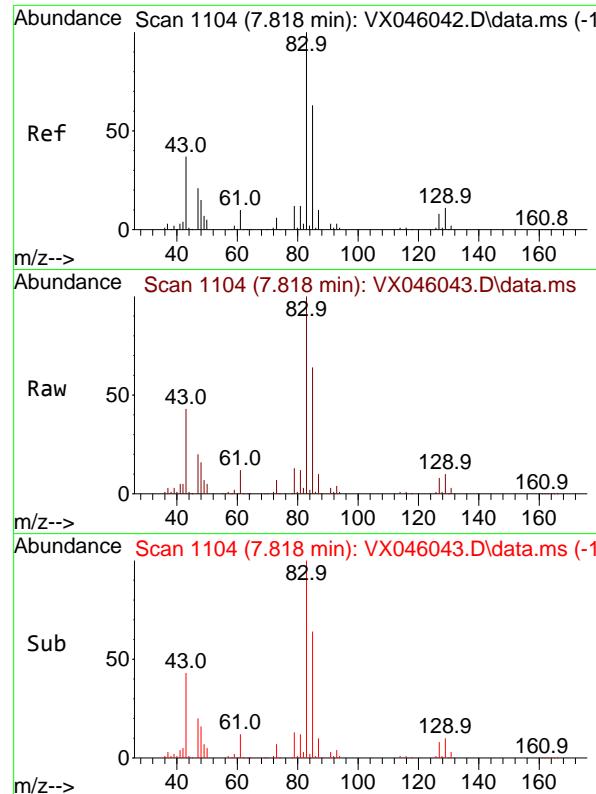

#47

Bromodichloromethane

Concen: 74.845 ug/l

RT: 7.818 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

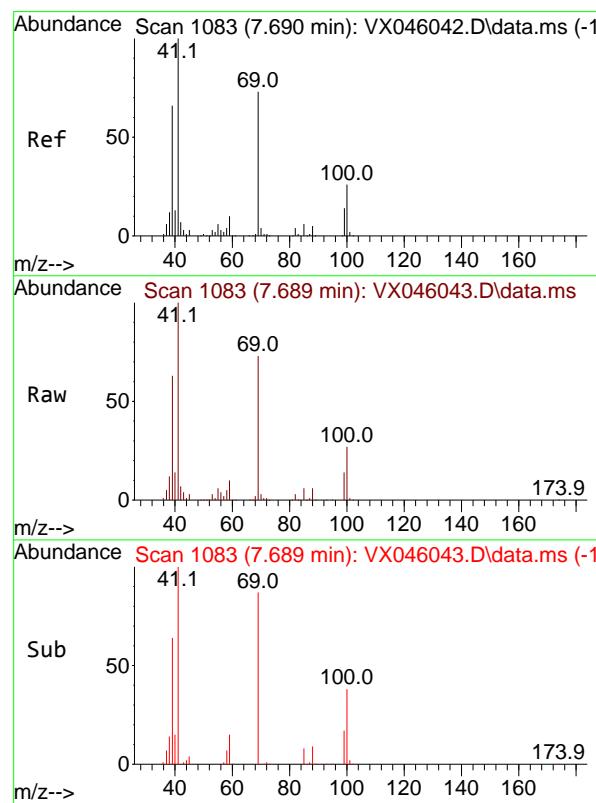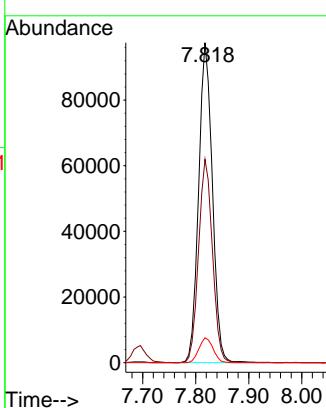

#48

Methyl methacrylate

Concen: 78.101 ug/l

RT: 7.689 min Scan# 1083


Delta R.T. -0.000 min







Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 41 Resp: 153093

Ion	Ratio	Lower	Upper
41	100		
69	74.1	58.5	87.7
39	65.5	51.7	77.5

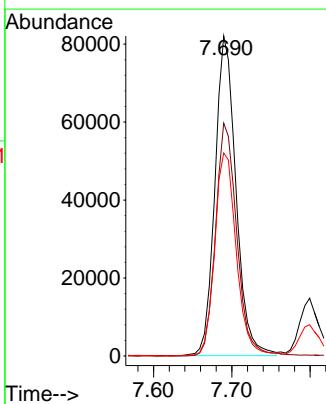

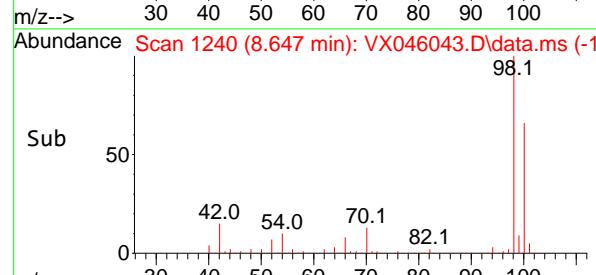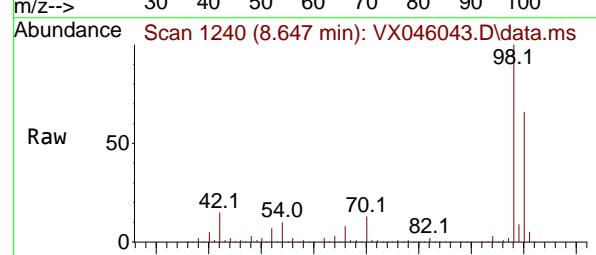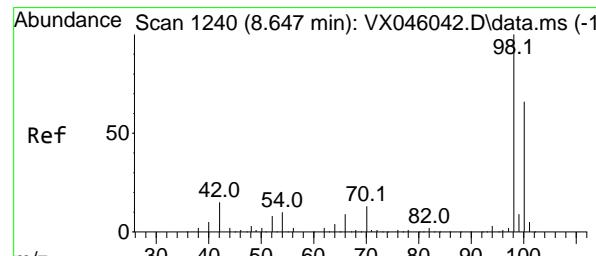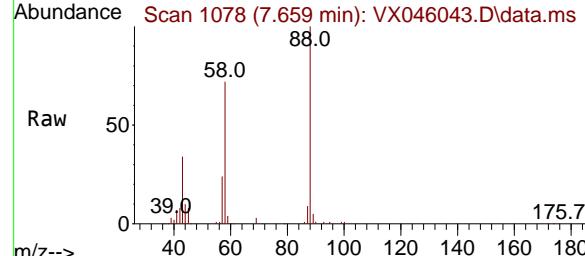

#49

1,4-Dioxane

Concen: 1470.687 ug/l

RT: 7.659 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#50

Toluene-d8

Concen: 67.031 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21



Tgt Ion: 98 Resp: 387230

Ion Ratio Lower Upper

98 100

100 65.2 53.5 80.3

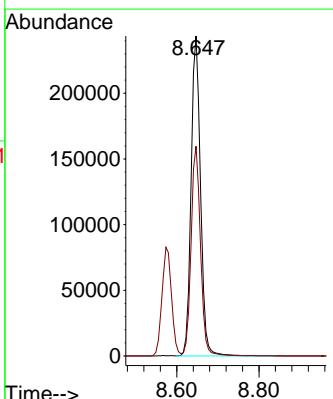

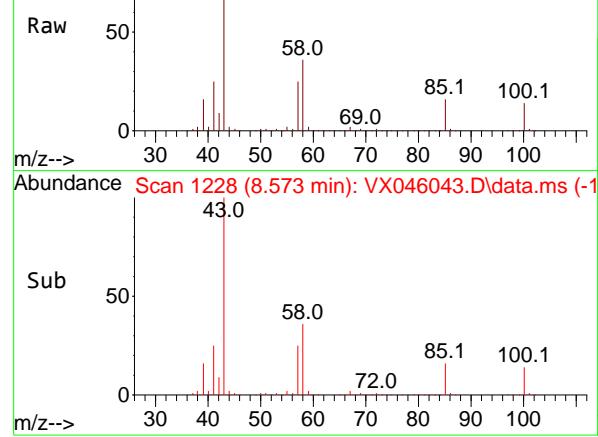

#51

4-Methyl-2-Pentanone

Concen: 384.740 ug/l

RT: 8.573 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

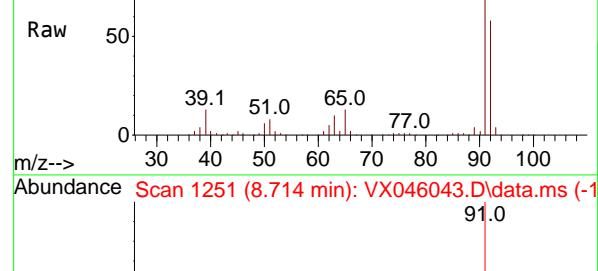

#52

Toluene

Concen: 74.010 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21


Tgt Ion: 92 Resp: 270763

Ion Ratio Lower Upper

92 100

91 171.2 136.6 205.0

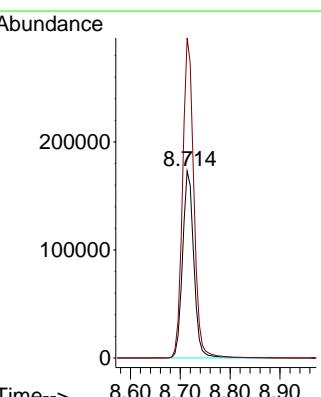


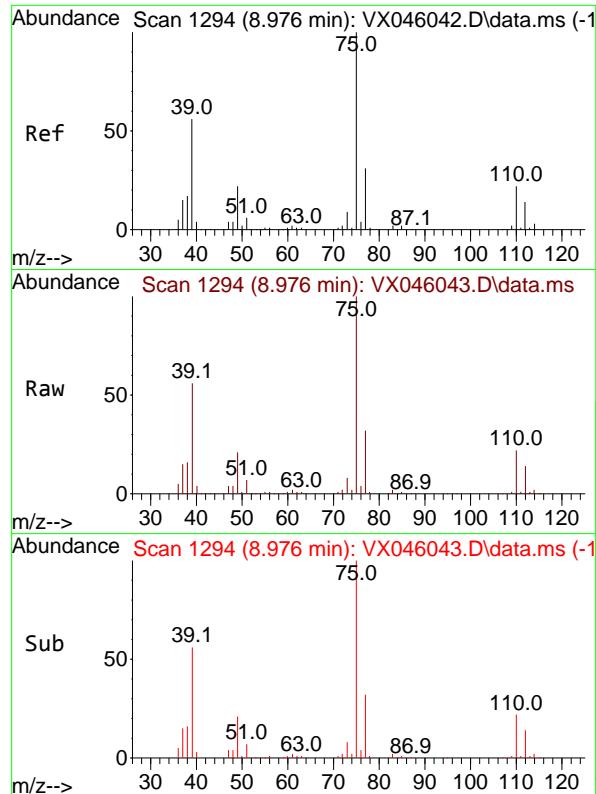


#53  
t-1,3-Dichloropropene  
Concen: 86.372 ug/l  
RT: 8.976 min Scan# 1193  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**







Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

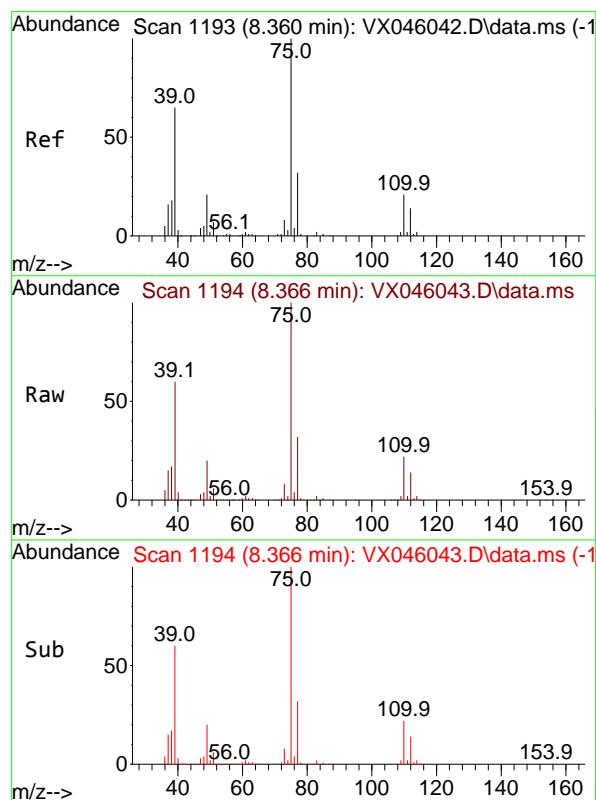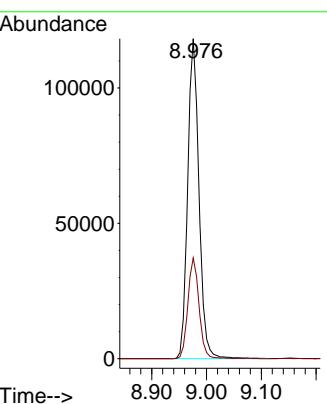

#54  
cis-1,3-Dichloropropene  
Concen: 80.264 ug/l  
RT: 8.366 min Scan# 1194  
Delta R.T. 0.006 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion: 75 Resp: 184134  
Ion Ratio Lower Upper  
75 100  
77 31.9 25.4 38.0  
39 59.6 52.2 78.4

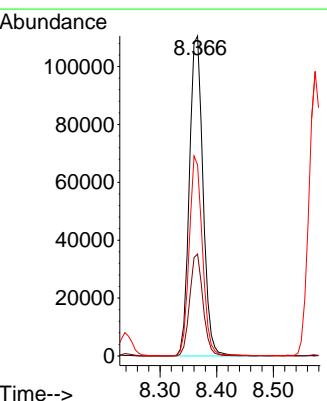



#55

1,1,2-Trichloroethane

Concen: 72.543 ug/l

RT: 9.147 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100


### Manual Integrations APPROVED

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

Time--&gt;

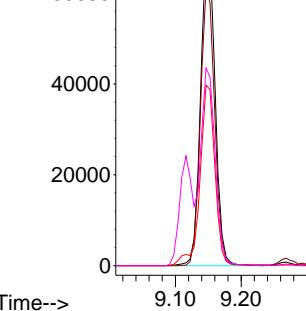

#56

Ethyl methacrylate

Concen: 82.359 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 69 Resp: 188717

Ion Ratio Lower Upper


69 100



41 75.7 60.8 91.2

39 47.7 39.0 58.6

Abundance

Time--&gt;

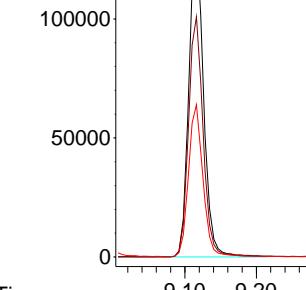

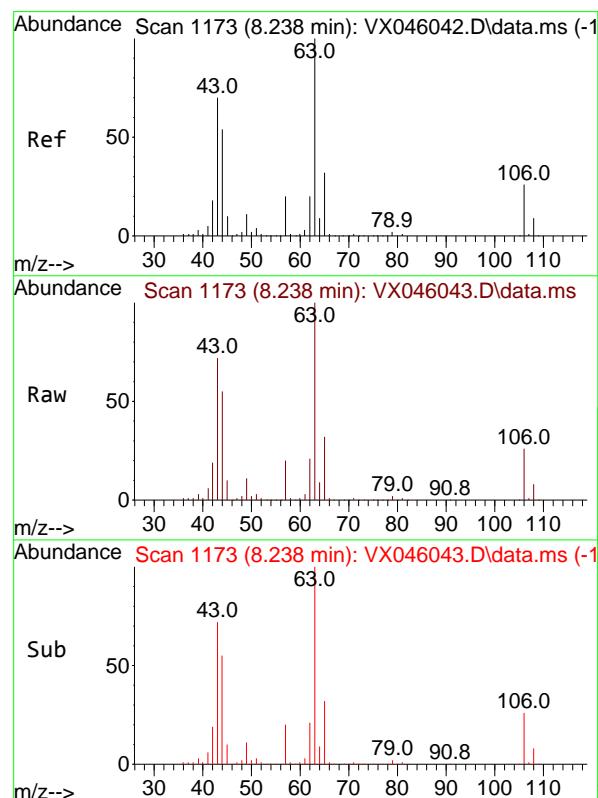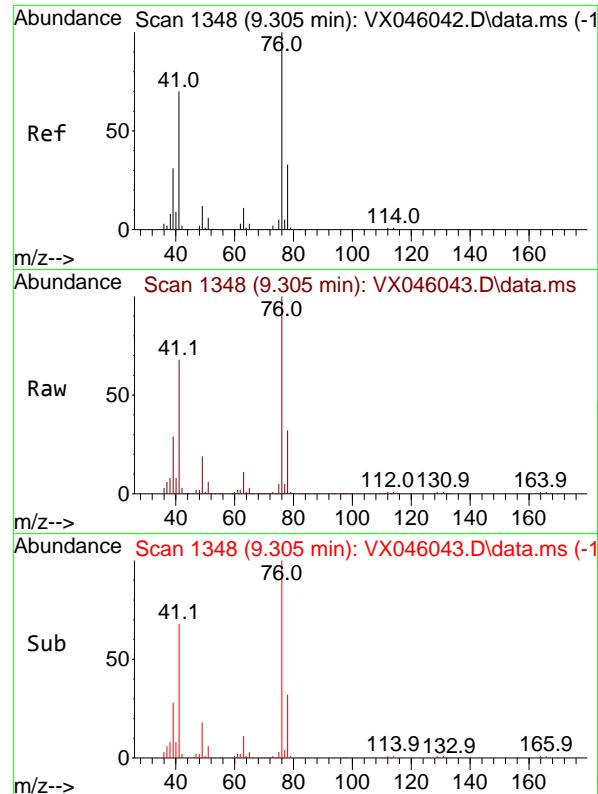

#57

1,3-Dichloropropane

Concen: 71.590 ug/l

RT: 9.305 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#58

2-Chloroethyl Vinyl ether

Concen: 449.791 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21




Tgt Ion: 63 Resp: 463169

Ion Ratio Lower Upper

63 100

106 26.7 21.5 32.3



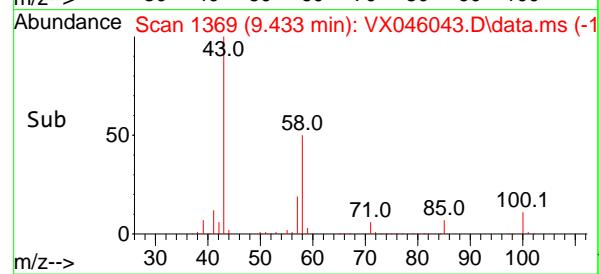




#59  
2-Hexanone  
Concen: 383.945 ug/l  
RT: 9.433 min Scan# 1368  
Delta R.T. 0.006 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#60  
Dibromochloromethane  
Concen: 78.918 ug/l  
RT: 9.518 min Scan# 1383  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion:129 Resp: 127012  
Ion Ratio Lower Upper  
129 100  
127 77.0 39.3 117.8

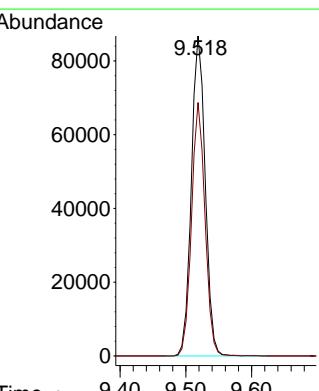

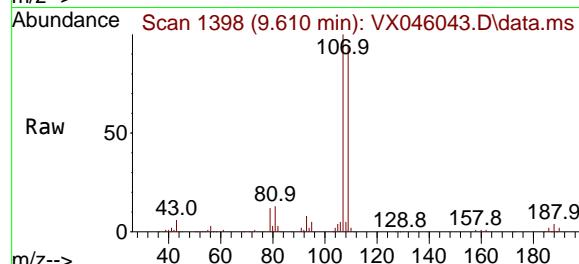

#61

1,2-Dibromoethane

Concen: 74.200 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#62

4-Bromofluorobenzene

Concen: 72.818 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion: 95 Resp: 153085




Ion Ratio Lower Upper

95 100

174 67.1 0.0 135.8

176 65.3 0.0 131.4





#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025


Supervised By :Mahesh Dadoda 05/06/2025



#64  
Tetrachloroethene  
Concen: 67.493 ug/l  
RT: 9.268 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion:164 Resp: 93195  
Ion Ratio Lower Upper  
164 100  
166 123.4 105.0 157.6  
129 101.4 83.5 125.3  
131 98.0 76.5 114.7

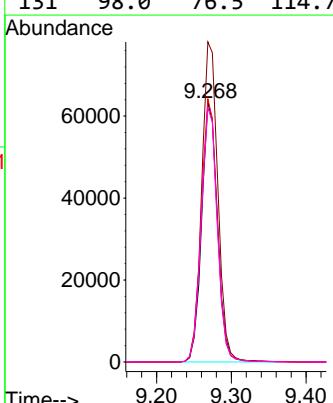


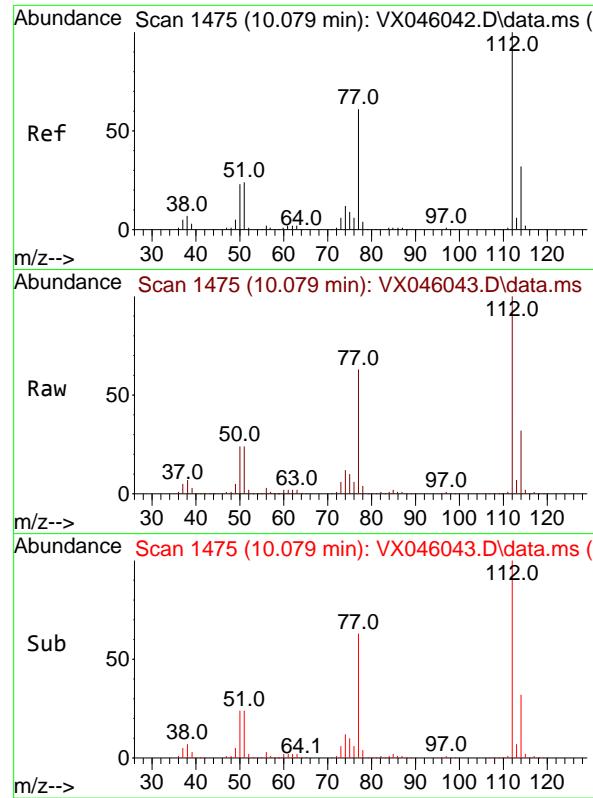


#65  
Chlorobenzene  
Concen: 70.490 ug/l  
RT: 10.079 min Scan# 1475  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

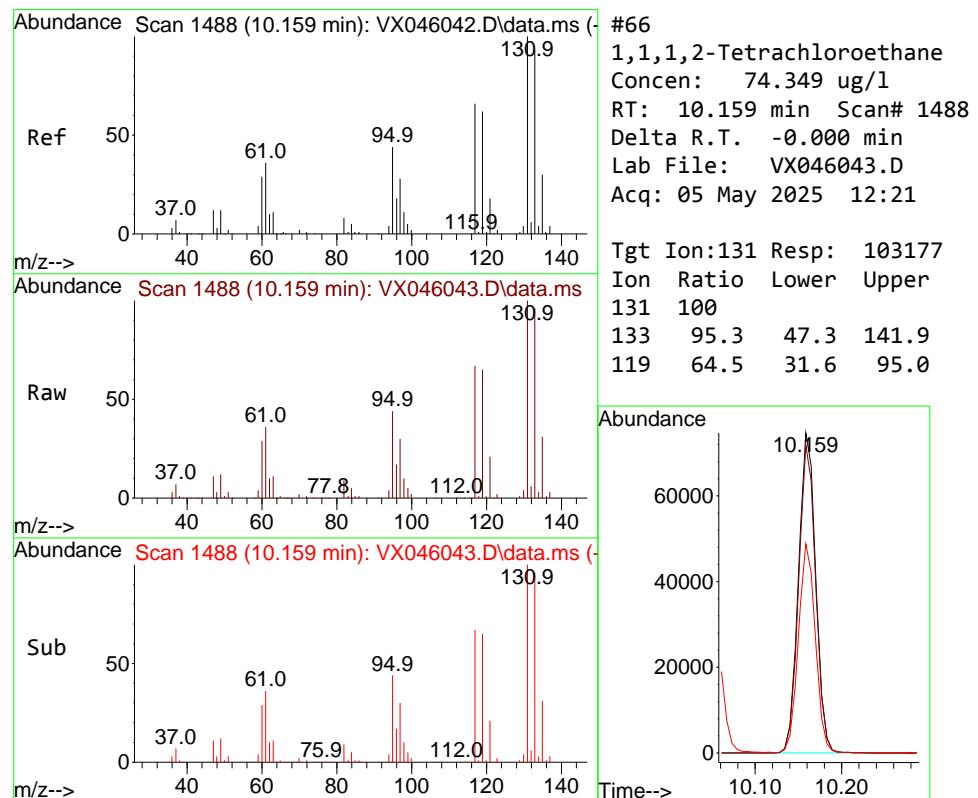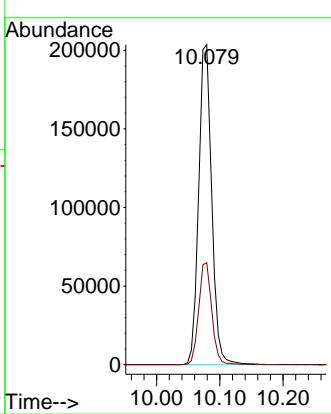

#66  
1,1,1,2-Tetrachloroethane  
Concen: 74.349 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion:131 Resp: 103177  
Ion Ratio Lower Upper  
131 100  
133 95.3 47.3 141.9  
119 64.5 31.6 95.0

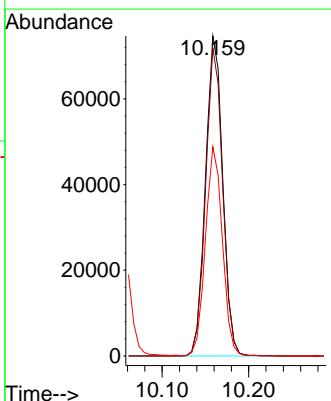



#67

Ethyl Benzene

Concen: 75.444 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#68

m/p-Xylenes

Concen: 152.181 ug/l


RT: 10.299 min Scan# 1511


Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 106 Resp: 389935  
 Ion Ratio Lower Upper  
 106 100  
 91 215.8 171.2 256.8

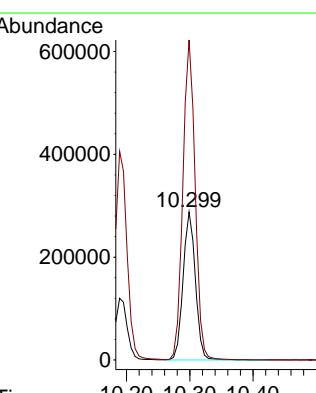


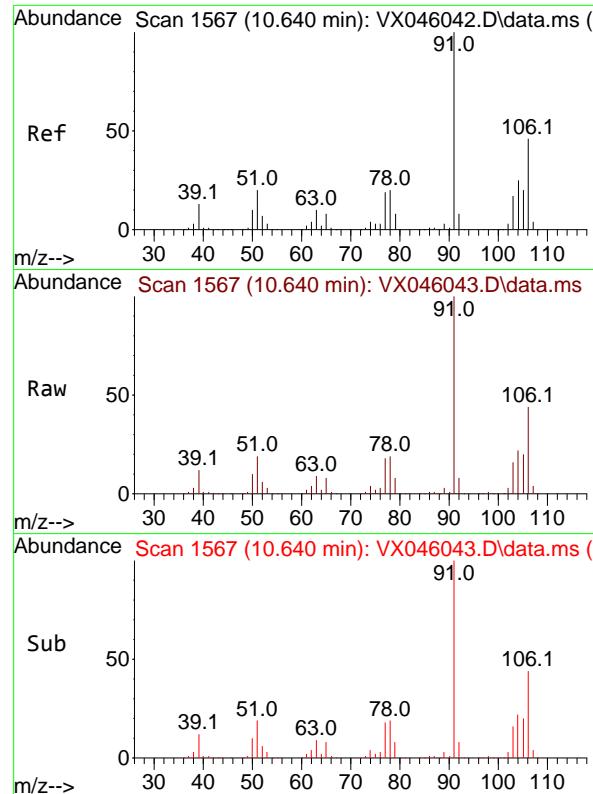


#69  
o-Xylene  
Concen: 73.890 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

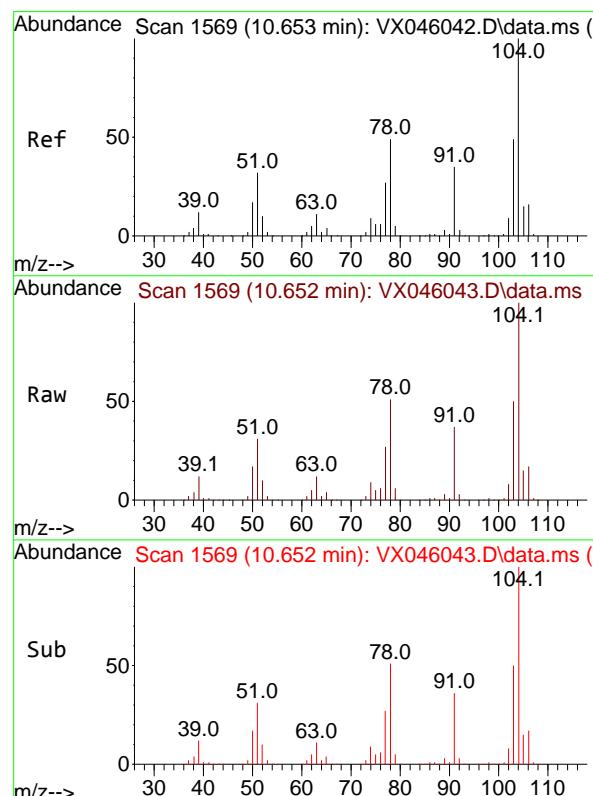

#70  
Styrene  
Concen: 79.411 ug/l  
RT: 10.652 min Scan# 1569  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion:104 Resp: 328195  
Ion Ratio Lower Upper  
104 100  
78 57.4 45.7 68.5  
103 54.8 43.7 65.5

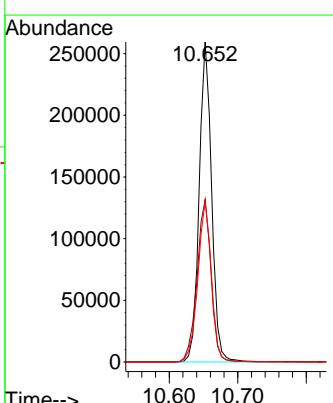



#71

Bromoform

Concen: 80.927 ug/l

RT: 10.799 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

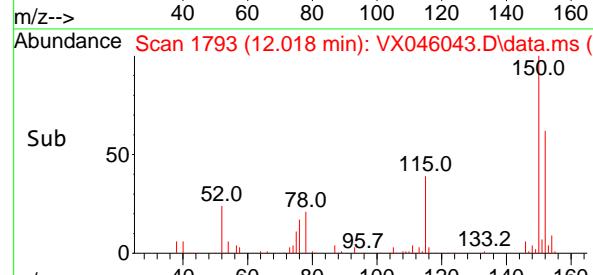

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l


RT: 12.018 min Scan# 1793


Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt	Ion:152	Resp:	66369
Ion	Ratio	Lower	Upper
152	100		
115	120.4	46.9	140.7
150	190.4	0.0	351.0

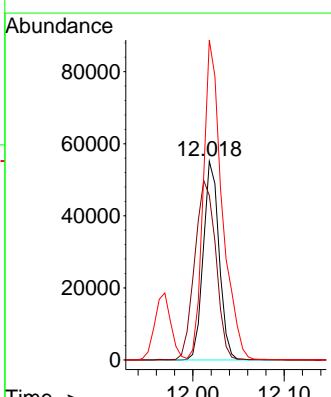

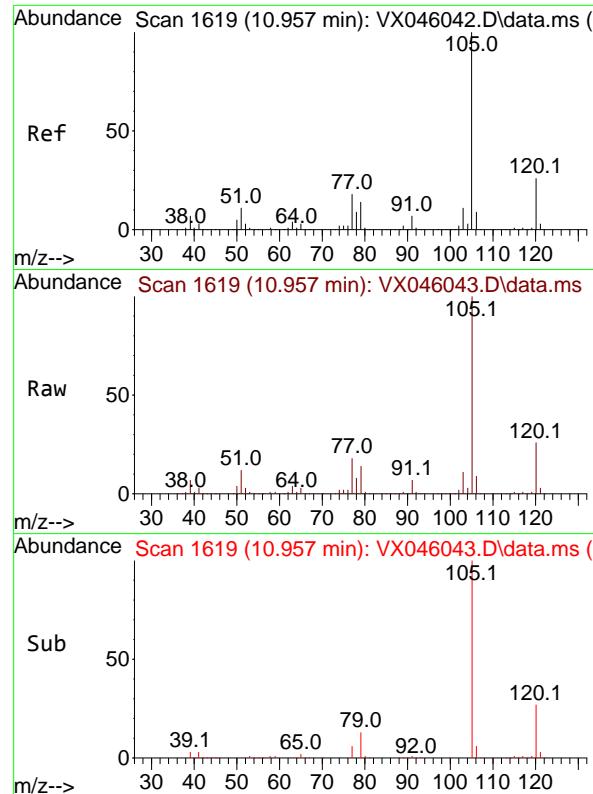

#73

Isopropylbenzene

Concen: 71.083 ug/l

RT: 10.957 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

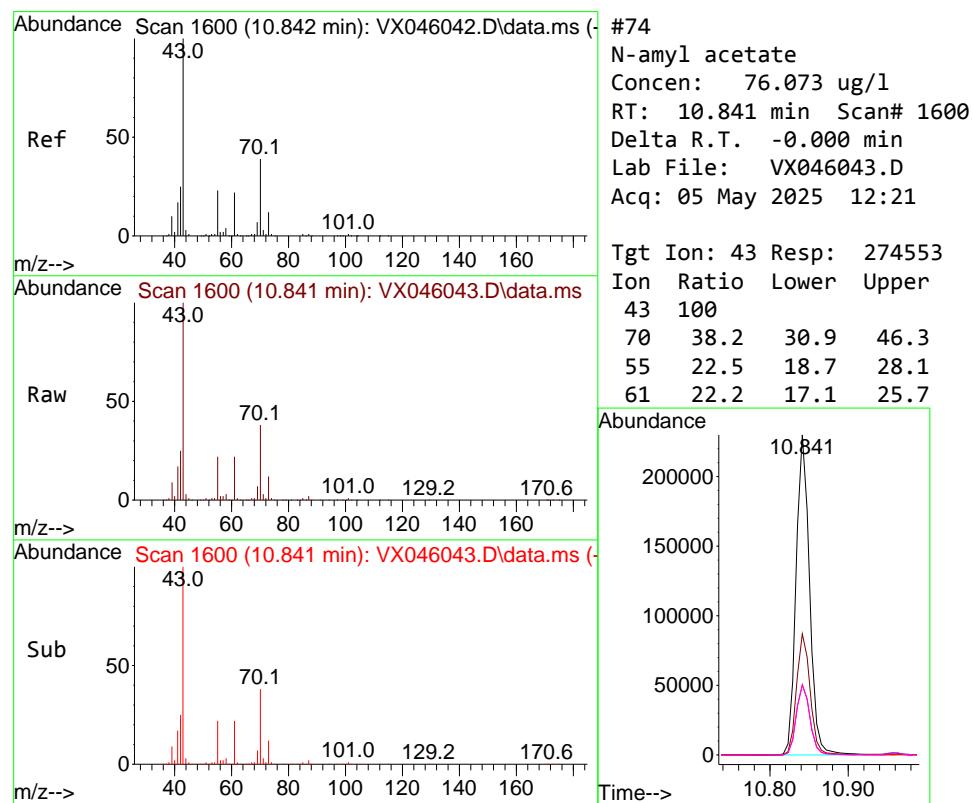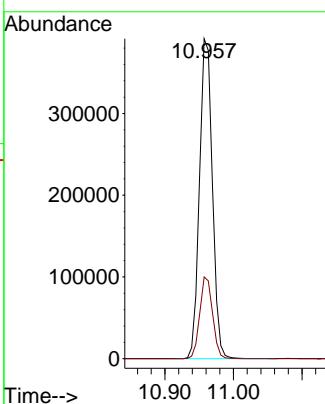

#74

N-amyl acetate

Concen: 76.073 ug/l


RT: 10.841 min Scan# 1600


Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt	Ion:	43	Resp:	274553
Ion	Ratio	Lower	Upper	
43	100			
70	38.2	30.9	46.3	
55	22.5	18.7	28.1	
61	22.2	17.1	25.7	

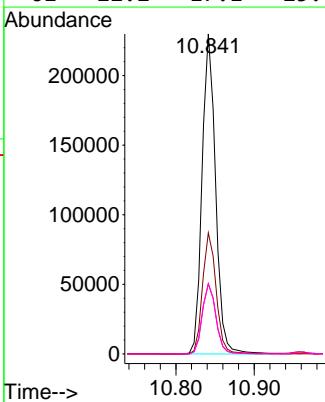


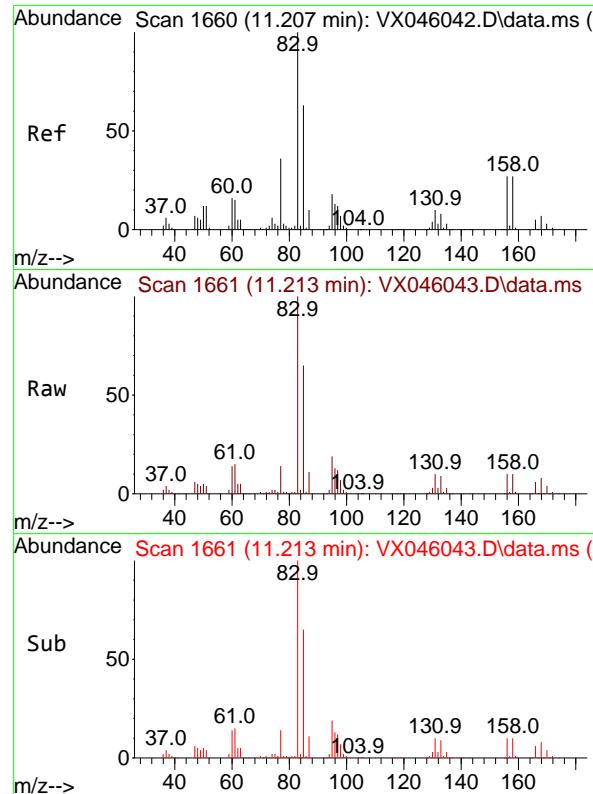


#75  
1,1,2,2-Tetrachloroethane  
Concen: 66.207 ug/l  
RT: 11.213 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carbone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

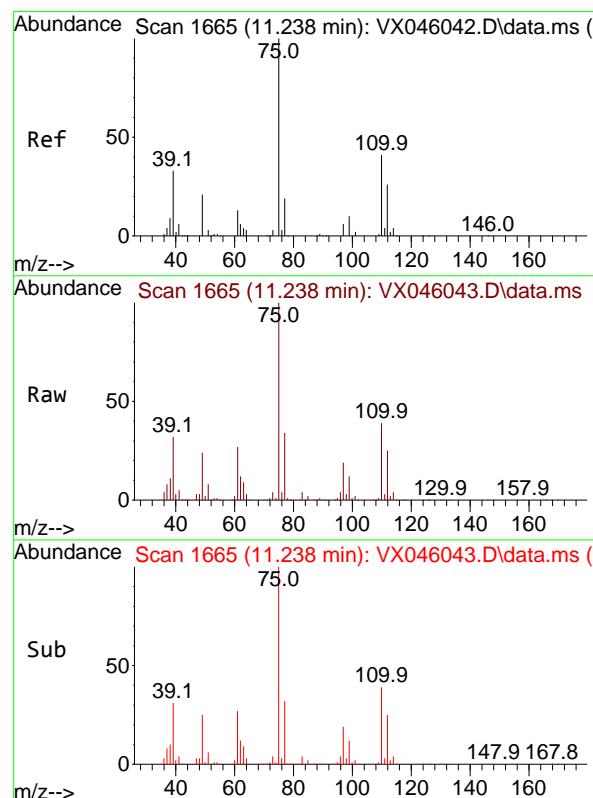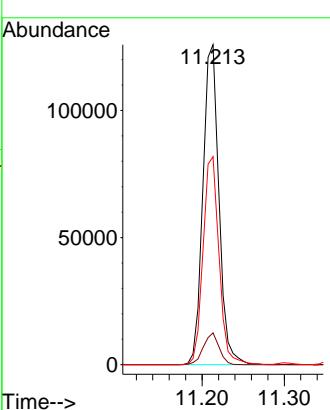

#76  
1,2,3-Trichloropropane  
Concen: 54.277 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion: 75 Resp: 150182  
Ion Ratio Lower Upper  
75 100  
77 42.2 20.5 61.5

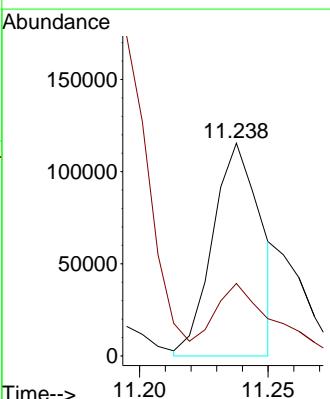

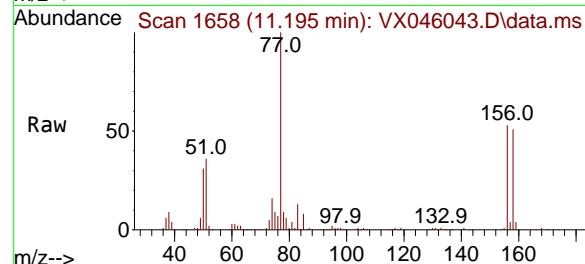

#77

Bromobenzene

Concen: 69.959 ug/l

RT: 11.195 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

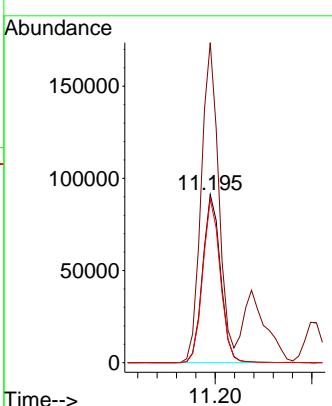

#78

n-propylbenzene

Concen: 74.974 ug/l


RT: 11.305 min Scan# 1676




Delta R.T. 0.006 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
	91	100			
	120	21.7	608332	10.8	32.4

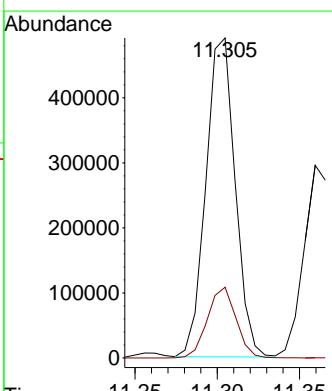



#79

2-Chlorotoluene

Concen: 68.100 ug/l

RT: 11.360 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

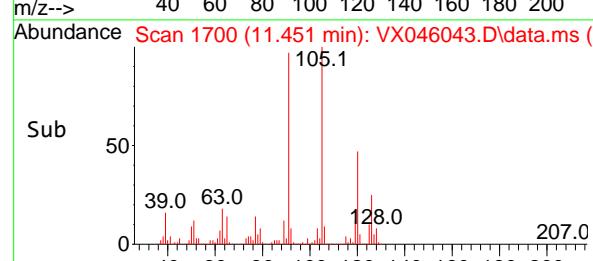

#80

1,3,5-Trimethylbenzene

Concen: 71.903 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21


Tgt Ion:105 Resp: 432096

Ion Ratio Lower Upper

105 100

120 46.3 23.1 69.2

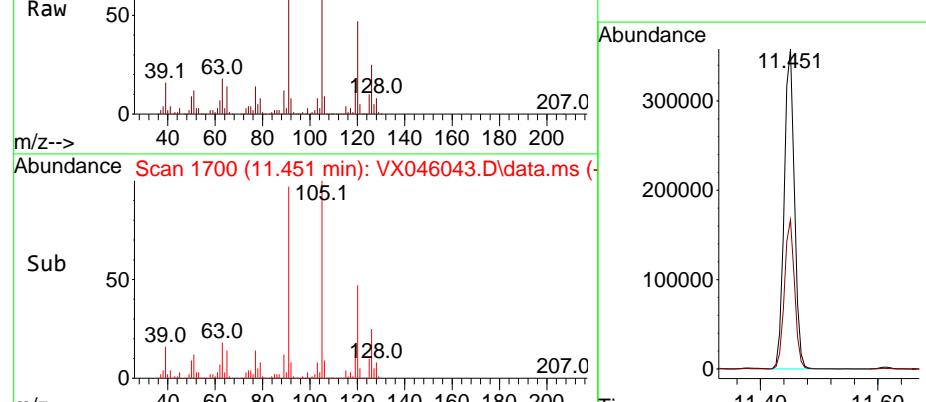


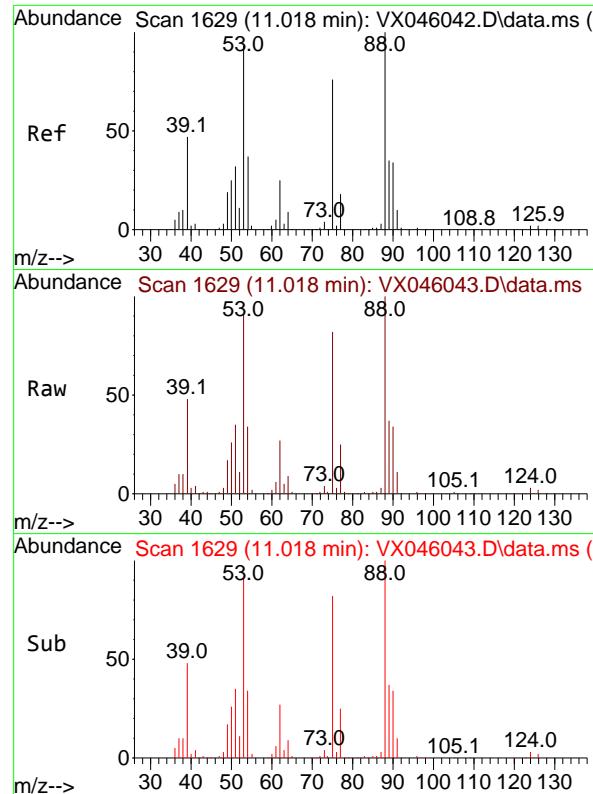


#81  
trans-1,4-Dichloro-2-butene  
Concen: 81.820 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

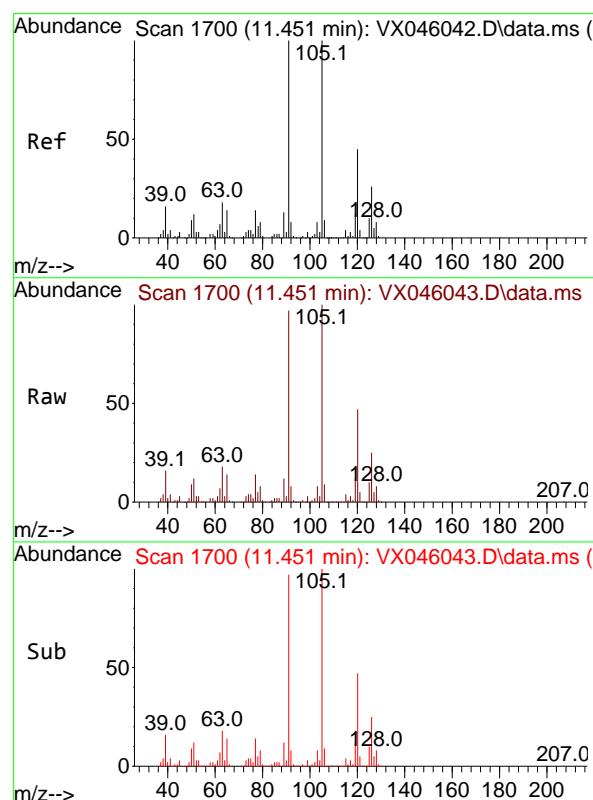

#82  
4-Chlorotoluene  
Concen: 71.890 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion: 91 Resp: 432053  
Ion Ratio Lower Upper  
91 100  
126 26.5 13.3 39.8

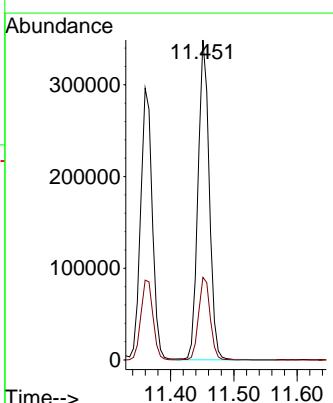

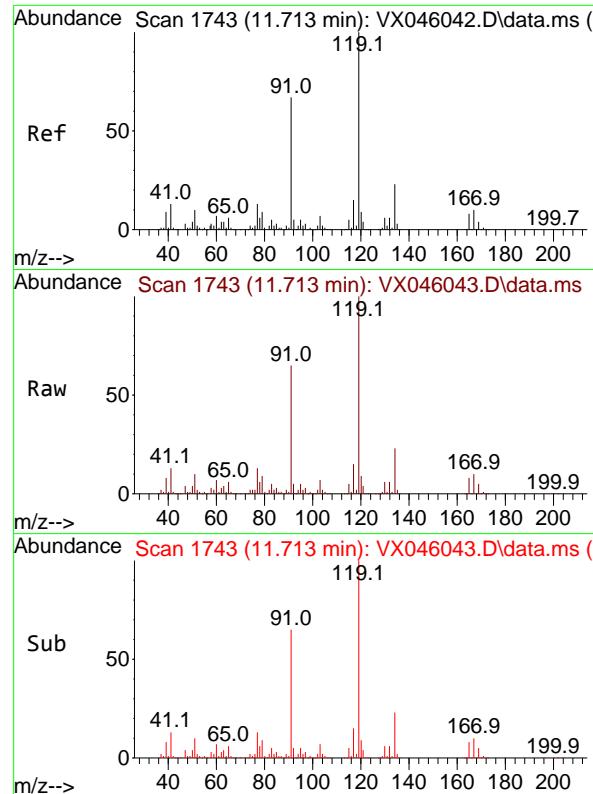

#83

tert-Butylbenzene

Concen: 73.197 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

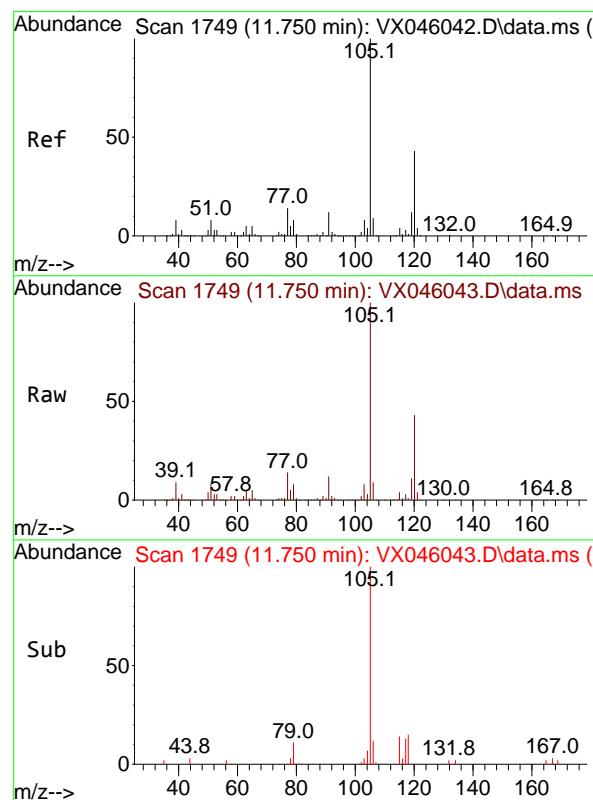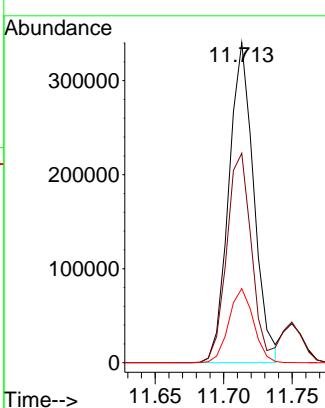

#84

1,2,4-Trimethylbenzene

Concen: 73.758 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21


Tgt Ion:105 Resp: 442728

Ion Ratio Lower Upper



105 100

120 42.4 21.2 63.6

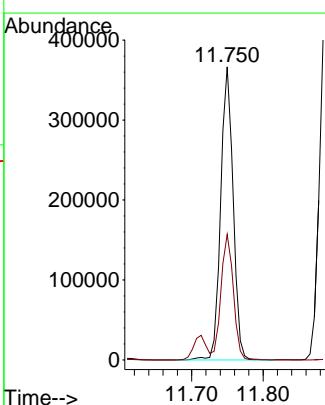




Abundance Scan 1772 (11.890 min): VX046043.D\data.ms (-)

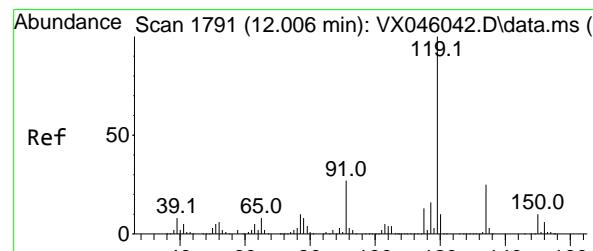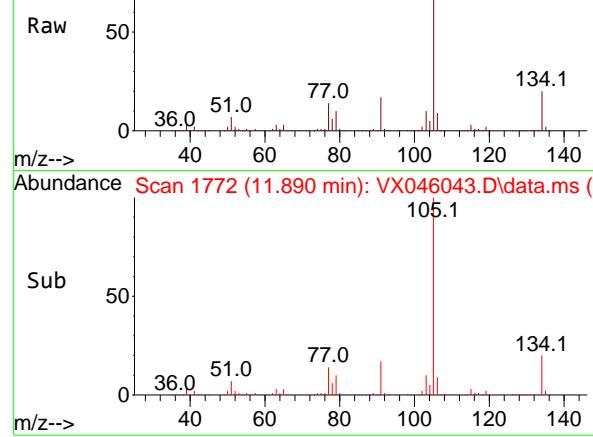

Abundance Scan 1791 (12.006 min): VX046043.D\data.ms (-)

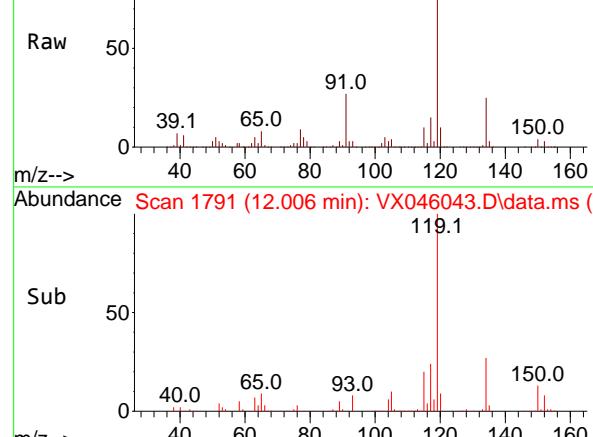

Abundance Scan 1791 (12.006 min): VX046043.D\data.ms (-)

#85

sec-Butylbenzene

Concen: 74.188 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

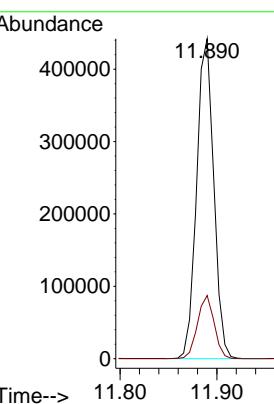

#86

p-Isopropyltoluene

Concen: 77.393 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion:119 Resp: 457898


Ion Ratio Lower Upper

119 100

134 24.6 12.5 37.5

91 26.8 13.8 41.4

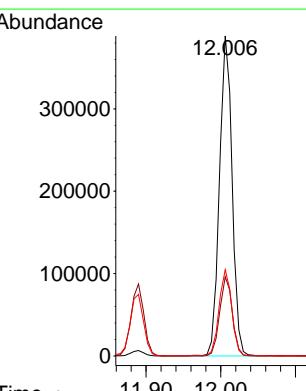

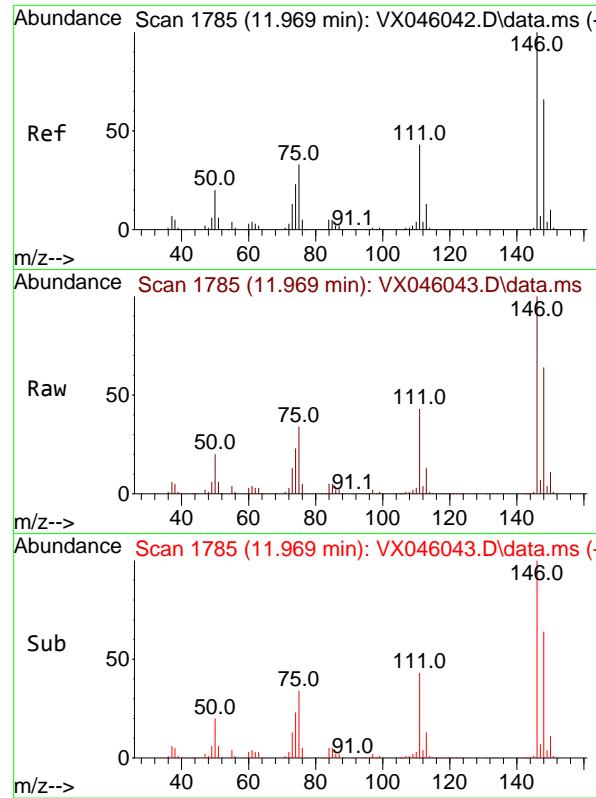

#87

1,3-Dichlorobenzene

Concen: 70.449 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC100

Tgt Ion:146 Resp: 21975

Ion Ratio Lower Upper

146 100

111 44.1 22.1 66.3



148 63.5 32.1 96.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

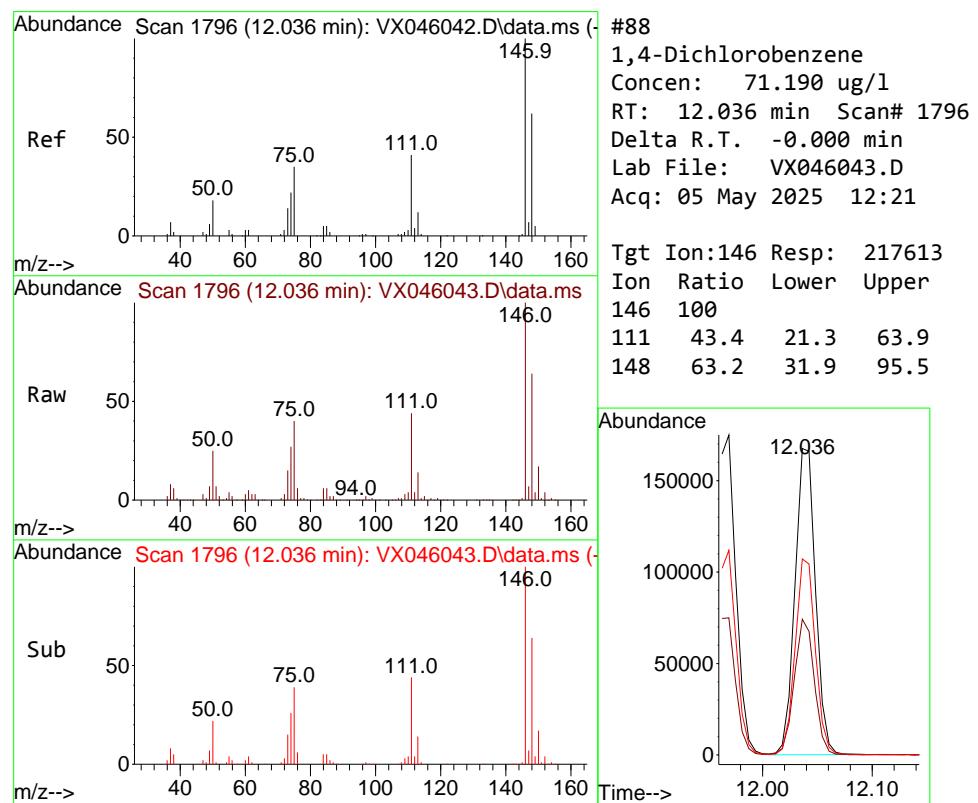

#88

1,4-Dichlorobenzene

Concen: 71.190 ug/l

RT: 12.036 min Scan# 1796

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion:146 Resp: 217613




Ion Ratio Lower Upper

146 100

111 43.4 21.3 63.9

148 63.2 31.9 95.5

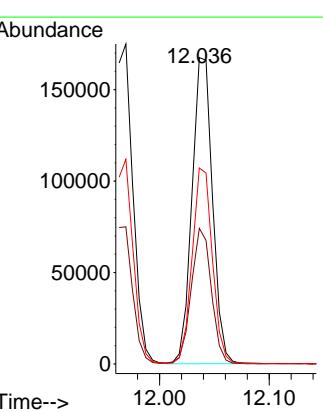



#89

n-Butylbenzene

Concen: 80.996 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

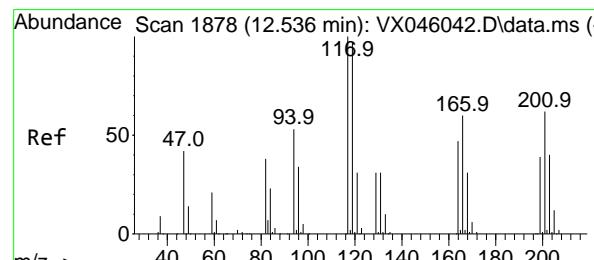

#90

Hexachloroethane

Concen: 74.978 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. -0.000 min

Lab File: VX046043.D


Acq: 05 May 2025 12:21



Tgt Ion:117 Resp: 82528

Ion Ratio Lower Upper

117 100

201 63.3 31.6 94.7



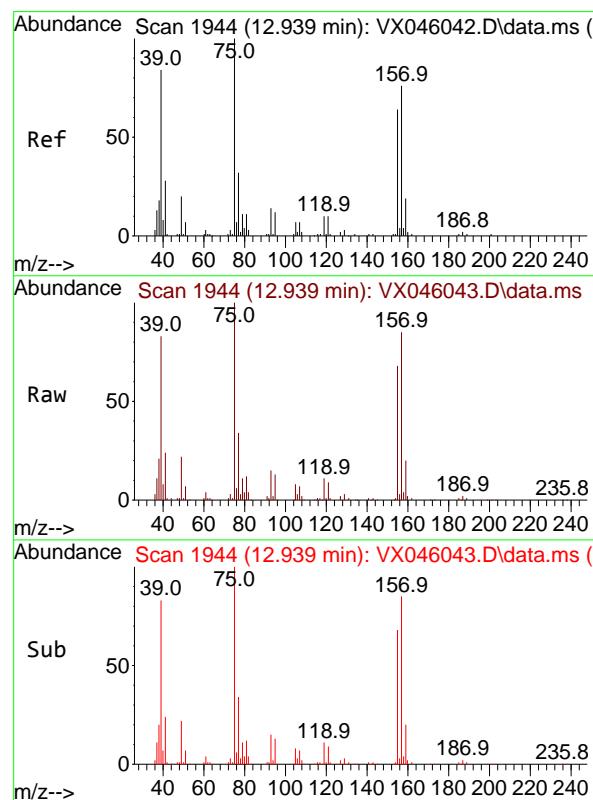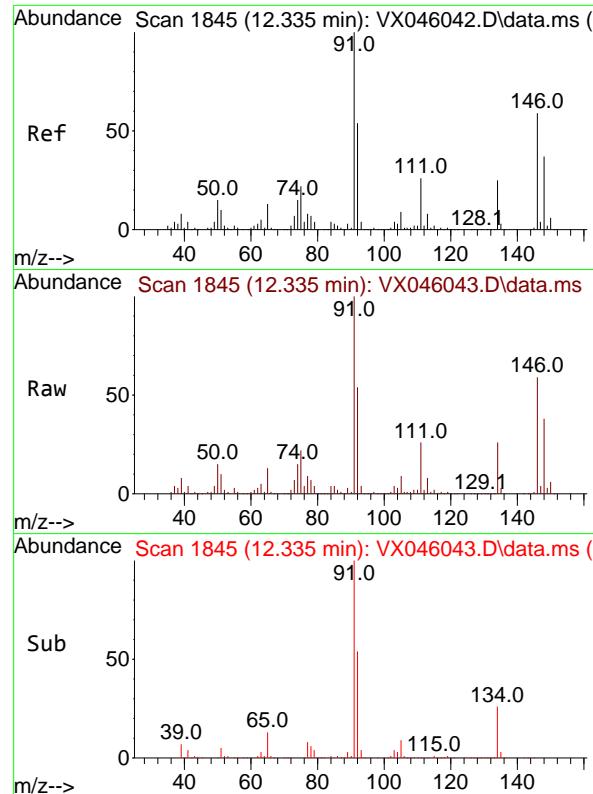

#91

1,2-Dichlorobenzene

Concen: 71.367 ug/l

RT: 12.335 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 74.512 ug/l

RT: 12.939 min Scan# 1944


Delta R.T. -0.000 min


Lab File: VX046043.D

Acq: 05 May 2025 12:21

Tgt Ion: 75 Resp: 43673

Ion	Ratio	Lower	Upper
75	100		
155	69.4	34.9	104.8
157	90.1	43.8	131.4

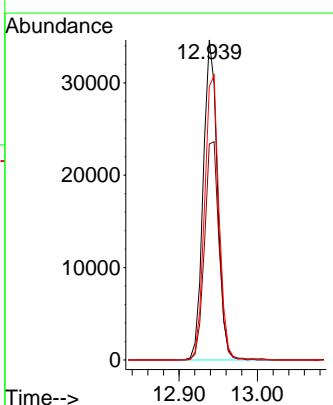

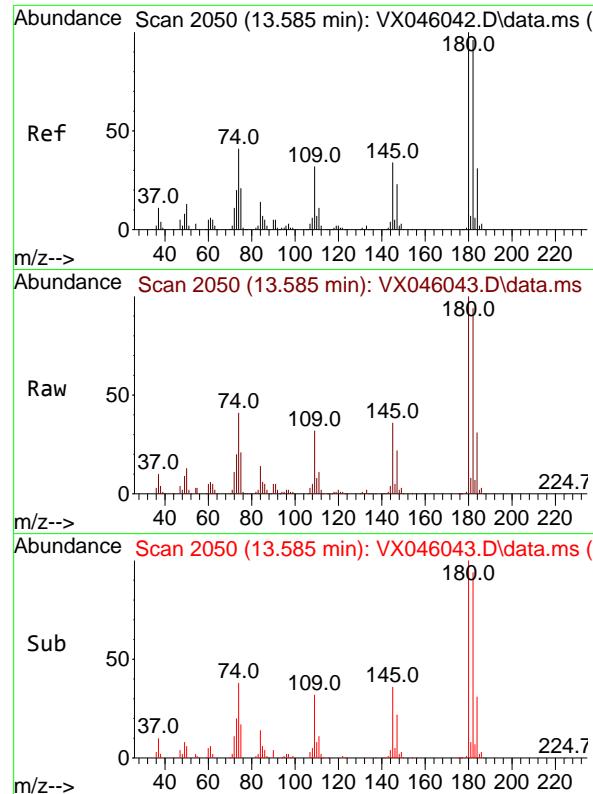

#93

1,2,4-Trichlorobenzene

Concen: 82.605 ug/l

RT: 13.585 min Scan# 2050

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC100

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

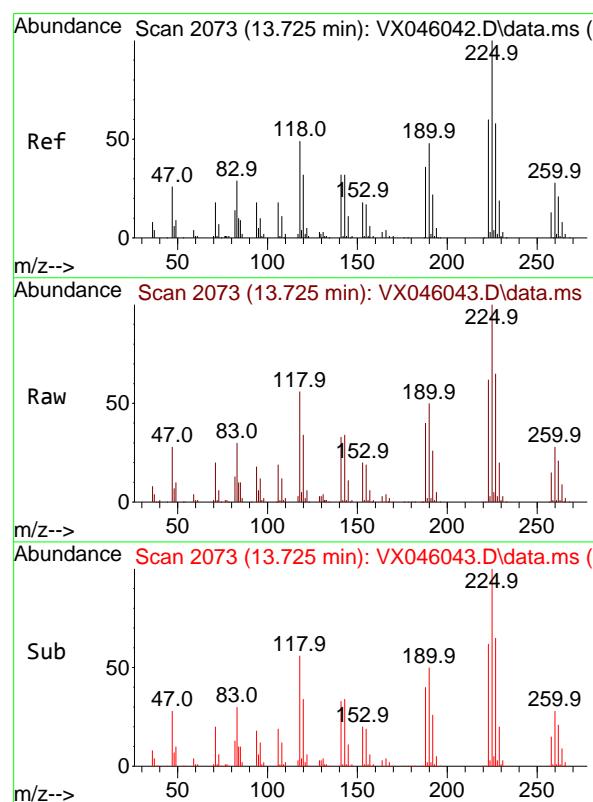

#94

Hexachlorobutadiene

Concen: 71.314 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. -0.000 min

Lab File: VX046043.D

Acq: 05 May 2025 12:21


Tgt Ion:225 Resp: 55494



Ion Ratio Lower Upper

225 100

223 62.3 30.8 92.4

227 64.9 30.9 92.7

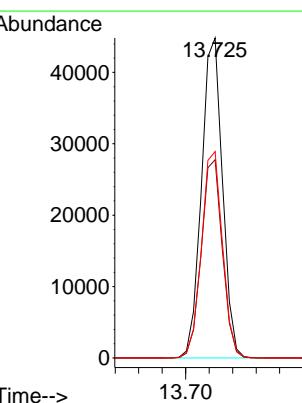

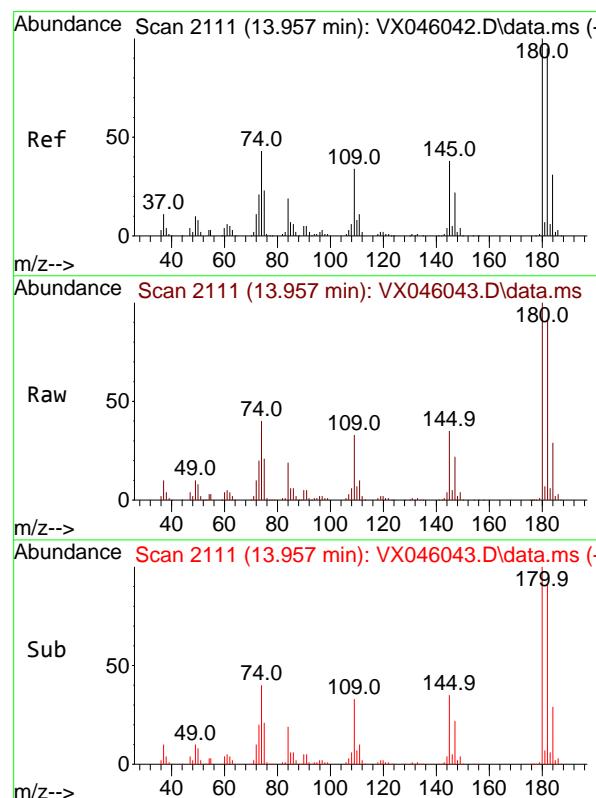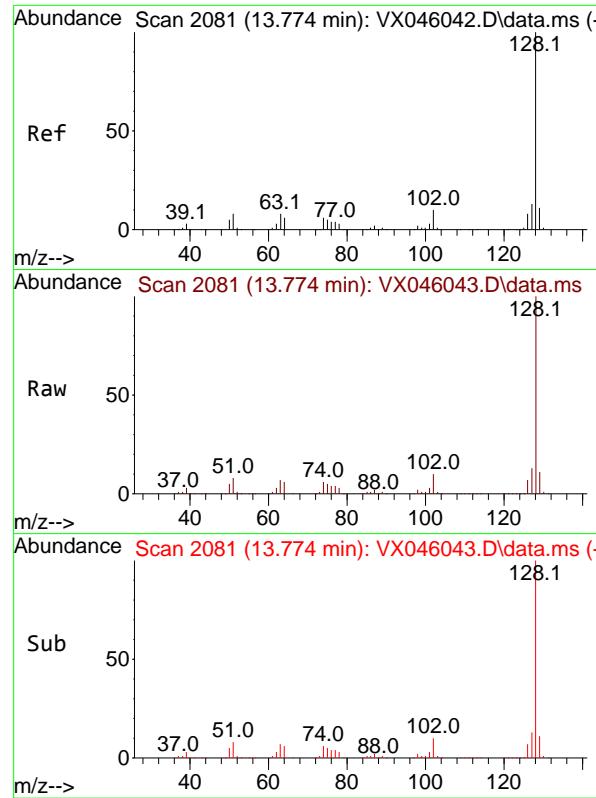



#95  
Naphthalene  
Concen: 80.842 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC100

Tgt Ion:128 Resp: 489773  
Ion Ratio Lower Upper  
128 100  
127 12.9 10.4 15.6  
129 10.9 8.6 13.0


### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

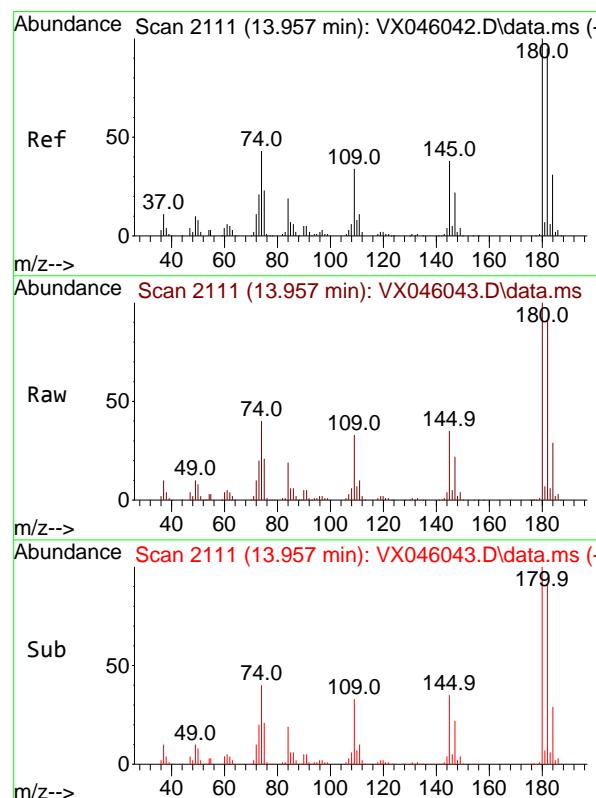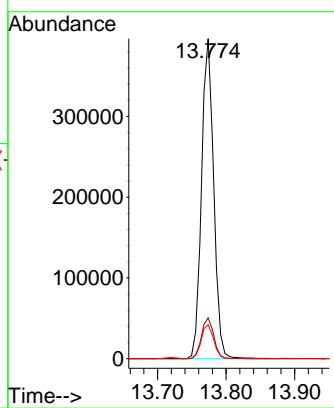

#96  
1,2,3-Trichlorobenzene  
Concen: 79.981 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046043.D  
Acq: 05 May 2025 12:21

Tgt Ion:180 Resp: 139525  
Ion Ratio Lower Upper  
180 100  
182 93.7 47.8 143.3  
145 35.3 18.1 54.3

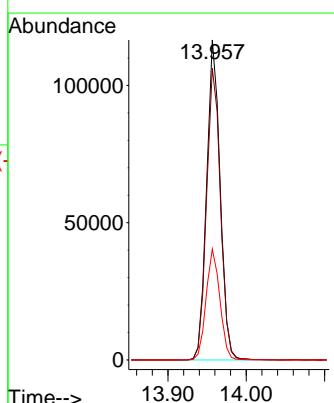

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046044.D  
 Acq On : 05 May 2025 12:45  
 Operator : JC/MD  
 Sample : VSTDICC150  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC150

Quant Time: May 06 06:11:37 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	82963	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	144975	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	128557	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	60345	50.000	ug/l	# 0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	231952	93.983	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 187.960%	#	
35) Dibromofluoromethane	5.385	113	160168	98.562	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 197.120%	#	
50) Toluene-d8	8.647	98	554390	101.252	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 202.500%	#	
62) 4-Bromofluorobenzene	11.079	95	217536	109.174	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 218.340%	#	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	217793	118.929	ug/l	98
3) Chloromethane	1.307	50	196843	109.161	ug/l	99
4) Vinyl Chloride	1.374	62	187924	118.953	ug/l	100
5) Bromomethane	1.593	94	83008	103.625	ug/l	95
6) Chloroethane	1.660	64	78806	96.822	ug/l	98
7) Trichlorofluoromethane	1.868	101	245108	101.851	ug/l	97
8) Diethyl Ether	2.136	74	88441	111.791	ug/l	95
9) 1,1,2-Trichlorotrifluo...	2.313	101	161404	112.243	ug/l	99
10) Methyl Iodide	2.441	142	189843	112.441	ug/l	100
11) Tert butyl alcohol	3.002	59	181238	616.119	ug/l	100
12) 1,1-Dichloroethene	2.307	96	155451	111.039	ug/l	99
13) Acrolein	2.239	56	203257	594.872	ug/l	98
14) Allyl chloride	2.654	41	297776	112.561	ug/l	98
15) Acrylonitrile	3.069	53	484854	550.973	ug/l	98
16) Acetone	2.392	43	460820	545.754	ug/l	98
17) Carbon Disulfide	2.502	76	397353	122.499	ug/l	100
18) Methyl Acetate	2.709	43	217885	108.099	ug/l	98
19) Methyl tert-butyl Ether	3.117	73	557210	114.112	ug/l	100
20) Methylene Chloride	2.782	84	172035	100.579	ug/l	96
21) trans-1,2-Dichloroethene	3.081	96	154694	108.241	ug/l	96
22) Diisopropyl ether	3.764	45	577610	116.858	ug/l	90
23) Vinyl Acetate	3.721	43	2655751	608.005	ug/l	100
24) 1,1-Dichloroethane	3.605	63	320083	110.182	ug/l	99
25) 2-Butanone	4.562	43	708463	581.292	ug/l	98
26) 2,2-Dichloropropane	4.471	77	258698	117.548	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	187835	108.994	ug/l	99
28) Bromochloromethane	4.898	49	146923	95.108	ug/l	100
29) Tetrahydrofuran	5.007	42	450456	569.081	ug/l	99
30) Chloroform	5.087	83	323659	107.208	ug/l	95
31) Cyclohexane	5.458	56	286312	116.934	ug/l	99
32) 1,1,1-Trichloroethane	5.373	97	295702	113.572	ug/l	98
36) 1,1-Dichloropropene	5.684	75	219731	116.462	ug/l	99
37) Ethyl Acetate	4.715	43	274312	115.889	ug/l	99
38) Carbon Tetrachloride	5.666	117	250916	115.760	ug/l	99
39) Methylcyclohexane	7.373	83	286311	121.107	ug/l	97
40) Benzene	6.031	78	642178	109.813	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046044.D  
 Acq On : 05 May 2025 12:45  
 Operator : JC/MD  
 Sample : VSTDICC150  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC150

Quant Time: May 06 06:11:37 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	151424	115.139	ug/1	98
42) 1,2-Dichloroethane	6.080	62	271992	112.492	ug/1	99
43) Isopropyl Acetate	6.342	43	447871	123.780	ug/1	100
44) Trichloroethene	7.117	130	157641	114.032	ug/1	96
45) 1,2-Dichloropropane	7.428	63	164505	113.217	ug/1	99
46) Dibromomethane	7.574	93	125846	109.869	ug/1	100
47) Bromodichloromethane	7.818	83	258326	116.365	ug/1	98
48) Methyl methacrylate	7.690	41	231040	124.356	ug/1	99
49) 1,4-Dioxane	7.665	88	82800	2241.695	ug/1	98
51) 4-Methyl-2-Pentanone	8.574	43	1371275	577.831	ug/1	100
52) Toluene	8.714	92	393323	113.430	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	257233	138.001	ug/1	99
54) cis-1,3-Dichloropropene	8.366	75	271054	124.658	ug/1	95
55) 1,1,2-Trichloroethane	9.147	97	154932	110.551	ug/1	97
56) Ethyl methacrylate	9.116	69	277921	127.968	ug/1	99
57) 1,3-Dichloropropane	9.305	76	272814	109.813	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.244	63	680608	697.344	ug/1	100
59) 2-Hexanone	9.433	43	1028597	571.094	ug/1	99
60) Dibromochloromethane	9.519	129	187497	122.915	ug/1	98
61) 1,2-Dibromoethane	9.604	107	165634	115.087	ug/1	97
64) Tetrachloroethene	9.269	164	132488	100.918	ug/1	96
65) Chlorobenzene	10.080	112	429656	108.615	ug/1	100
66) 1,1,1,2-Tetrachloroethane	10.159	131	152173	115.333	ug/1	99
67) Ethyl Benzene	10.189	91	785121	116.421	ug/1	99
68) m/p-Xylenes	10.299	106	570913	234.349	ug/1	100
69) o-Xylene	10.640	106	279906	113.990	ug/1	99
70) Styrene	10.653	104	474254	120.694	ug/1	99
71) Bromoform	10.799	173	125986	127.128	ug/1 #	99
73) Isopropylbenzene	10.957	105	752337	114.312	ug/1	99
74) N-amyl acetate	10.842	43	396877	120.944	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	243532	104.018	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	213744m	84.960	ug/1	
77) Bromobenzene	11.195	156	167934	110.297	ug/1	99
78) n-propylbenzene	11.305	91	881218	119.448	ug/1	100
79) 2-Chlorotoluene	11.360	91	534560	107.514	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	616477	112.825	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	81372	134.609	ug/1	93
82) 4-Chlorotoluene	11.451	91	611736	111.948	ug/1	100
83) tert-Butylbenzene	11.713	119	617473	115.065	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	623456	114.236	ug/1	99
85) sec-Butylbenzene	11.890	105	786293	118.023	ug/1	99
86) p-Isopropyltoluene	12.006	119	651531	121.113	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	313100	110.394	ug/1	100
88) 1,4-Dichlorobenzene	12.036	146	311752	112.167	ug/1	100
89) n-Butylbenzene	12.329	91	605783	129.533	ug/1	100
90) Hexachloroethane	12.536	117	123188	123.091	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	308039	111.506	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	64438	120.915	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	203255	134.366	ug/1	98
94) Hexachlorobutadiene	13.719	225	80558	113.857	ug/1	99
95) Naphthalene	13.774	128	721236	130.929	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	200379	126.331	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046044.D  
 Acq On : 05 May 2025 12:45  
 Operator : JC/MD  
 Sample : VSTDICC150  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 8 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC150

Quant Time: May 06 06:11:37 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046044.D  
Acq On : 05 May 2025 12:45  
Operator : JC/MD  
Sample : VSTDIICC150  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1




Quant Time: May 06 06:11:37 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 06:04:56 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC150

## Manual Integrations APPROVED

Reviewed By :John Caralone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

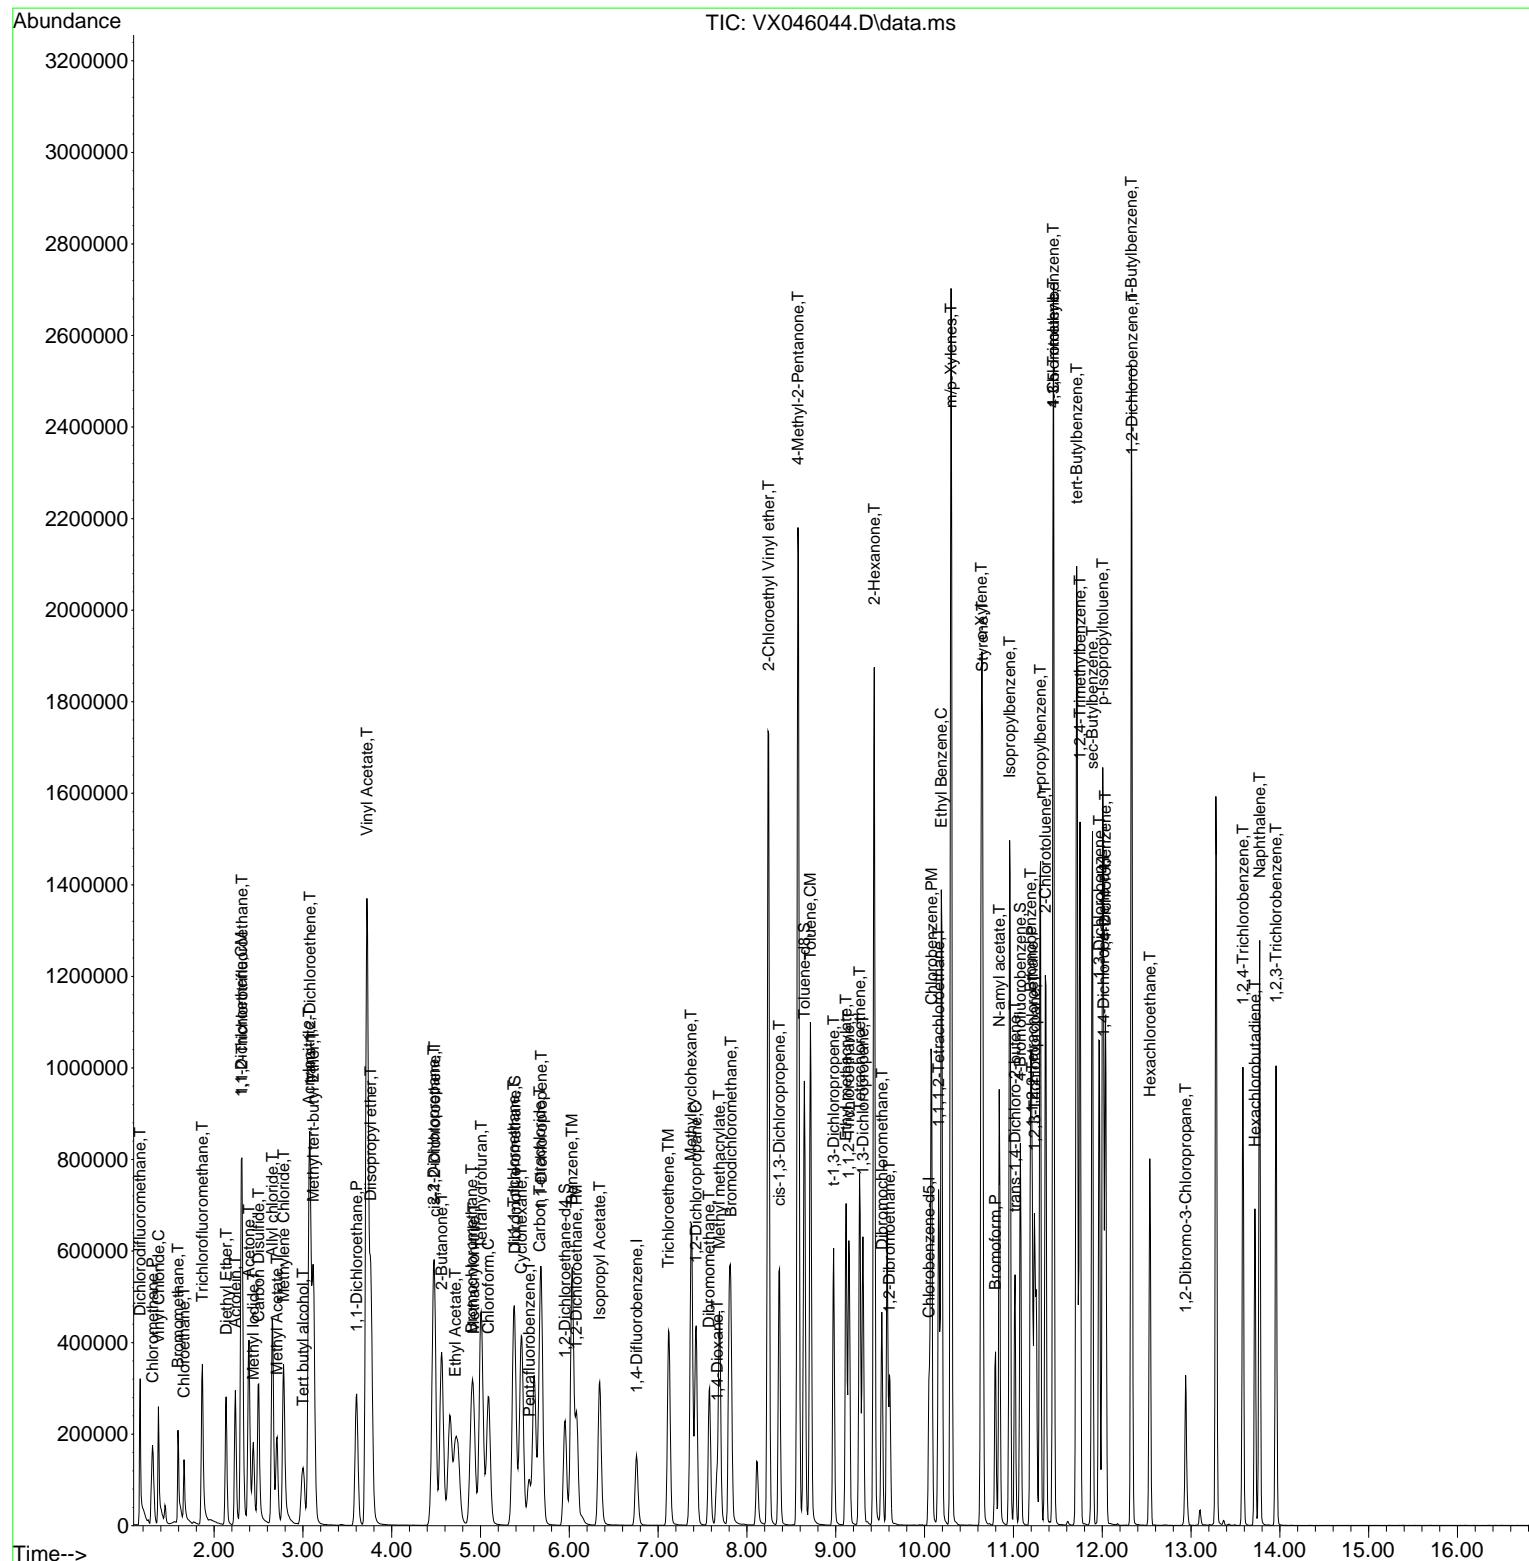







#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Delta R.T. 0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#2  
Dichlorodifluoromethane  
Concen: 118.929 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Tgt Ion: 85 Resp: 217793  
Ion Ratio Lower Upper  
85 100  
87 32.5 15.7 47.1

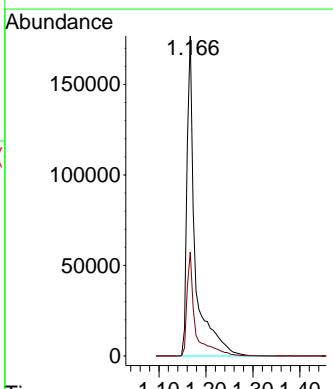

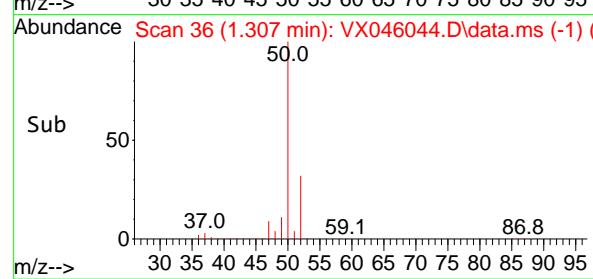

#3

Chloromethane

Concen: 109.161 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

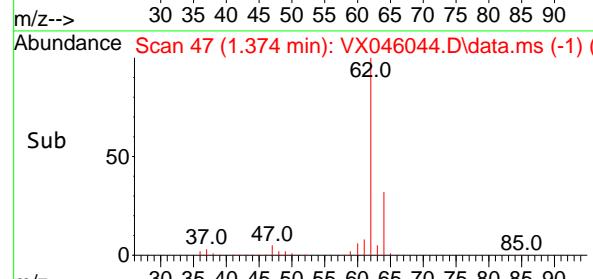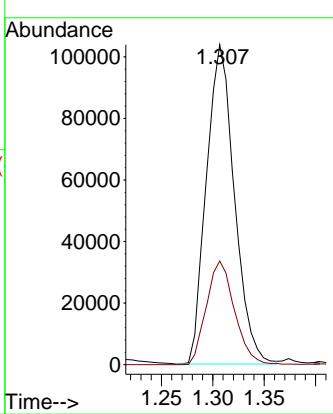

#4

Vinyl Chloride

Concen: 118.953 ug/l


RT: 1.374 min Scan# 47




Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 62 Resp: 187924  
 Ion Ratio Lower Upper  
 62 100  
 64 31.7 25.2 37.8





#5

Bromomethane

Concen: 103.625 ug/l

RT: 1.593 min Scan# 83

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45




Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

 Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025


#6

Chloroethane



Concen: 96.822 ug/l




RT: 1.660 min Scan# 94

Delta R.T. -0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

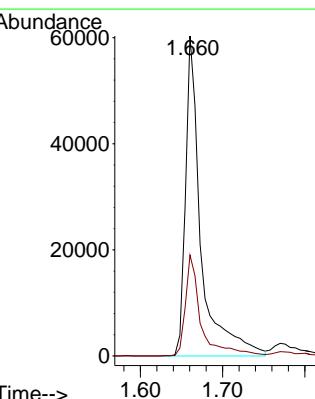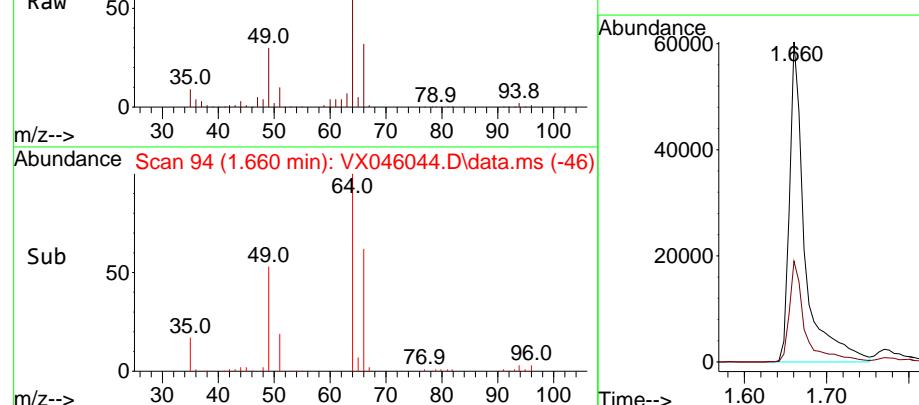 Tgt Ion: 64 Resp: 78806  
 Ion Ratio Lower Upper  
 64 100  
 66 31.3 24.3 36.5

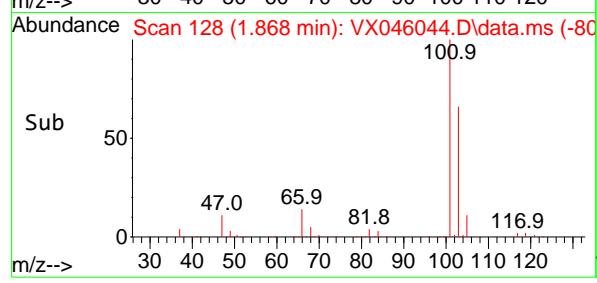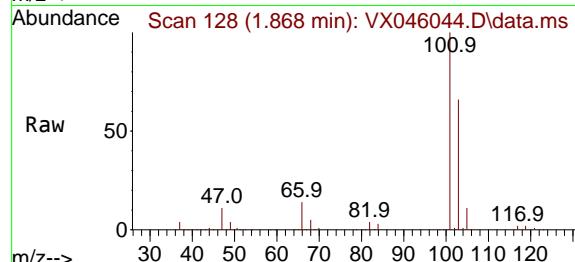


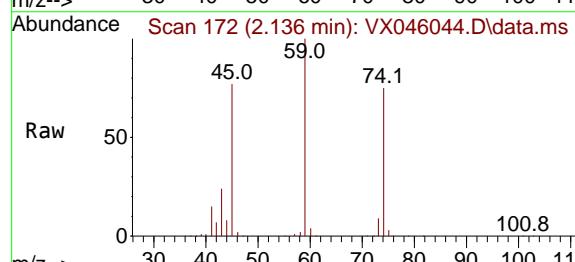


#7

Trichlorofluoromethane  
Concen: 101.851 ug/l  
RT: 1.868 min Scan# 128  
Delta R.T. -0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150

### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025




#8

Diethyl Ether  
Concen: 111.791 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45


Tgt Ion: 74 Resp: 88441  
Ion Ratio Lower Upper  
74 100  
45 104.7 54.9 164.8

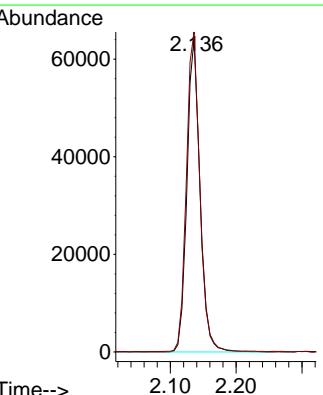



#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 112.243 ug/l  
RT: 2.313 min Scan# 2  
Delta R.T. -0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150

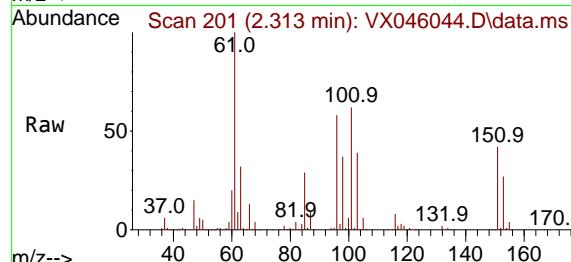


Tgt Ion:101 Resp: 16140  
Ion Ratio Lower Upper  
101 100  
85 46.8 38.6 58.0  
151 69.8 55.2 82.8

Manual Integrations  
APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

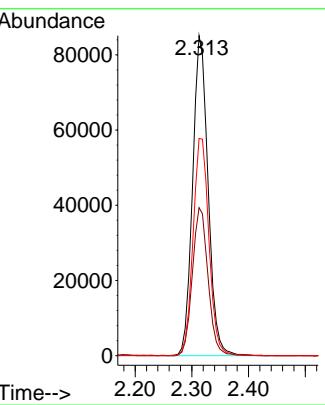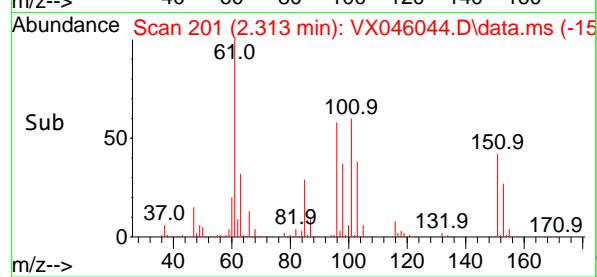


#10  
Methyl Iodide  
Concen: 112.441 ug/l  
RT: 2.441 min Scan# 222  
Delta R.T. -0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45



Tgt Ion:142 Resp: 189843  
Ion Ratio Lower Upper  
142 100  
127 52.4 41.7 62.5  
141 14.4 11.5 17.3

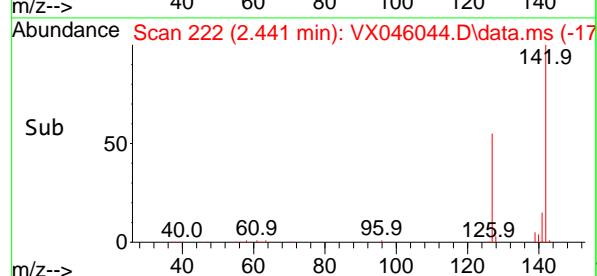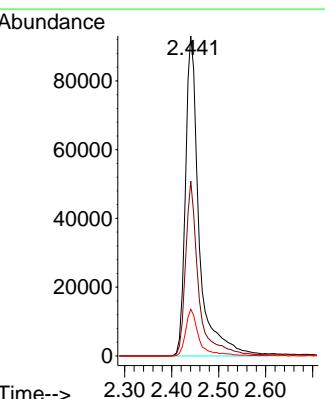

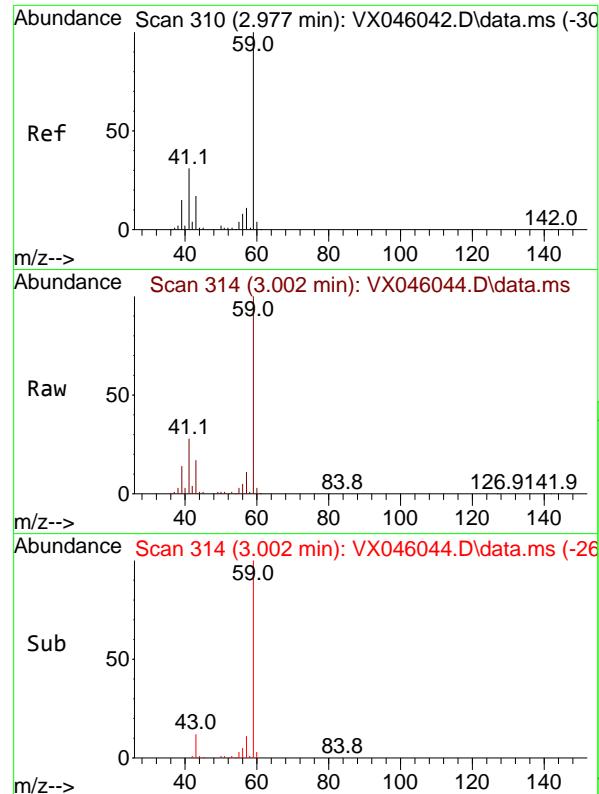

#11

Tert butyl alcohol

Concen: 616.119 ug/l

RT: 3.002 min Scan# 3

Delta R.T. 0.024 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150

Tgt Ion: 59 Resp: 181238

Ion Ratio Lower Upper

59 100



57 10.8 8.6 12.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

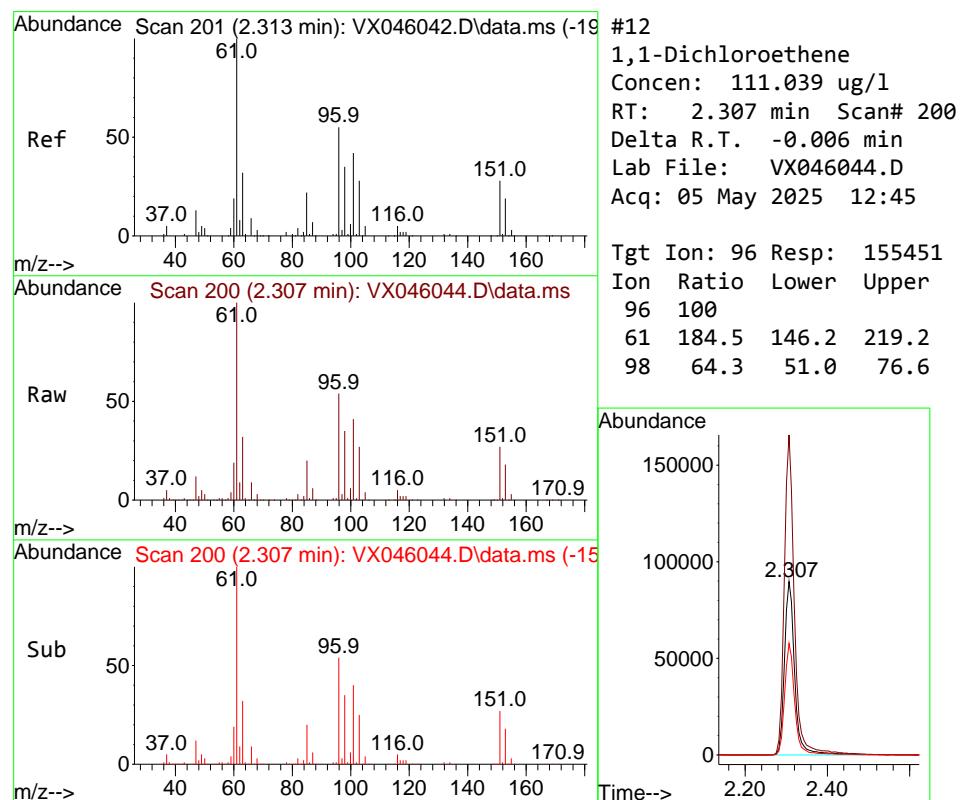

#12

1,1-Dichloroethene

Concen: 111.039 ug/l

RT: 2.307 min Scan# 200

Delta R.T. -0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45


Tgt Ion: 96 Resp: 155451


Ion Ratio Lower Upper

96 100

61 184.5 146.2 219.2

98 64.3 51.0 76.6

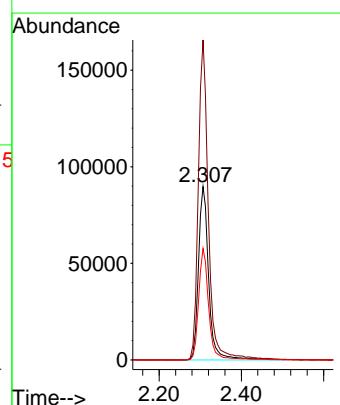




#13

Acrolein  
Concen: 594.872 ug/l  
RT: 2.239 min Scan# 188  
Delta R.T. 0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150




Tgt Ion: 56 Resp: 203251  
Ion Ratio Lower Upper  
56 100  
55 72.1 56.2 84.4

Manual Integrations  
APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025






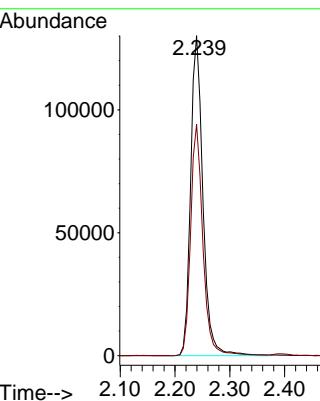


#14  
Allyl chloride  
Concen: 112.561 ug/l  
RT: 2.654 min Scan# 257  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

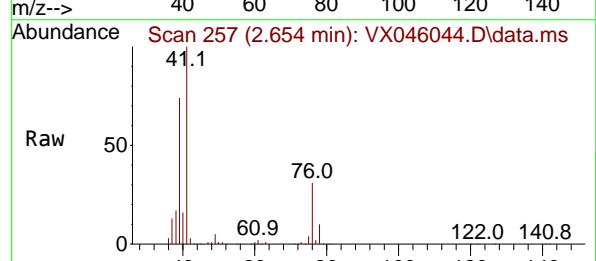

Tgt Ion: 41 Resp: 297776  
Ion Ratio Lower Upper  
41 100  
39 73.7 60.6 90.8  
76 31.8 24.9 37.3

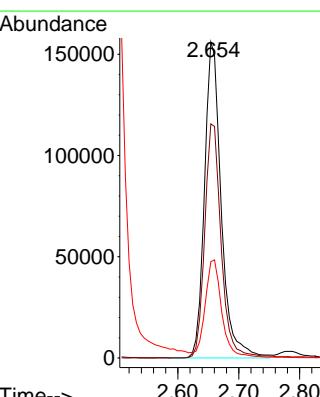



#15

Acrylonitrile

Concen: 550.973 ug/l

RT: 3.069 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150

Tgt Ion: 53 Resp: 484854

Ion Ratio Lower Upper

53 100

52 84.2 65.3 97.9


51 37.5 29.8 44.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#16

Acetone

Concen: 545.754 ug/l

RT: 2.392 min Scan# 214

Delta R.T. 0.006 min

Lab File: VX046044.D


Acq: 05 May 2025 12:45




Tgt Ion: 43 Resp: 460820

Ion Ratio Lower Upper

43 100

58 27.3 21.2 31.8

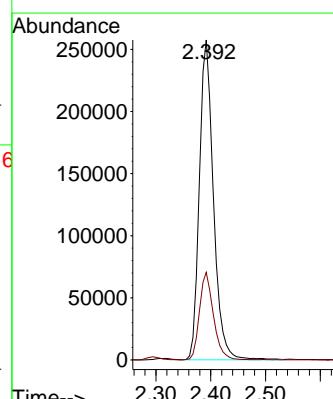



#17

Carbon Disulfide

Concen: 122.499 ug/l

RT: 2.502 min Scan# 2

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#18

Methyl Acetate

Concen: 108.099 ug/l


RT: 2.709 min Scan# 266







Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 43	Resp: 217885
Ion Ratio	Lower Upper
43 100	
74 21.9	16.7 25.1

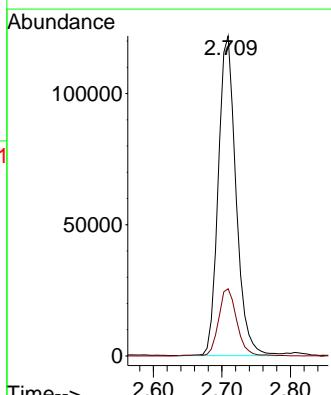

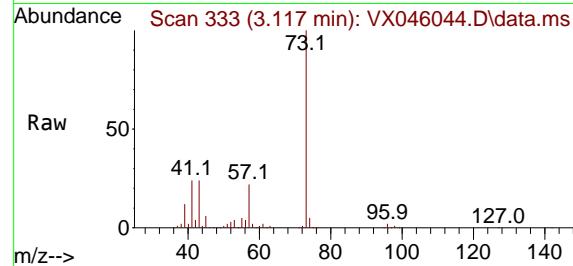

#19

Methyl tert-butyl Ether

Concen: 114.112 ug/l

RT: 3.117 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

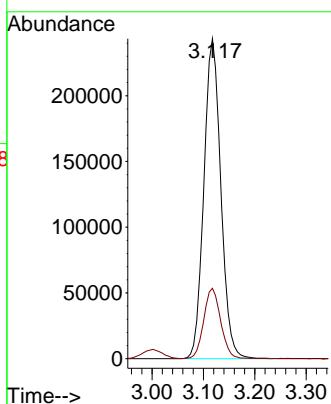

#20

Methylene Chloride

Concen: 100.579 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 84 Resp: 172035


Ion Ratio Lower Upper







84 100

49 136.0 113.9 170.9

51 41.5 33.5 50.3

86 63.7 53.8 80.8

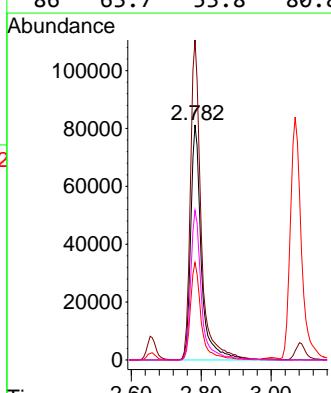

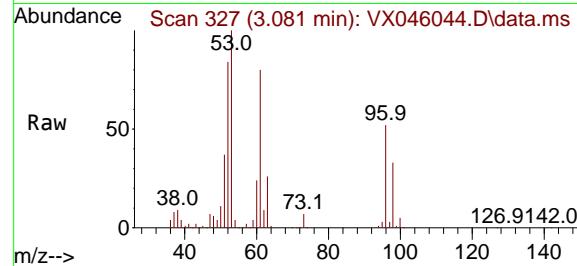

#21

trans-1,2-Dichloroethene

Concen: 108.241 ug/l

RT: 3.081 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#22

Diisopropyl ether

Concen: 116.858 ug/l

RT: 3.764 min Scan# 439

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 45 Resp: 577610


Ion Ratio Lower Upper


45 100

43 70.3 66.6 100.0

87 24.7 19.8 29.6

59 10.6 8.6 12.8

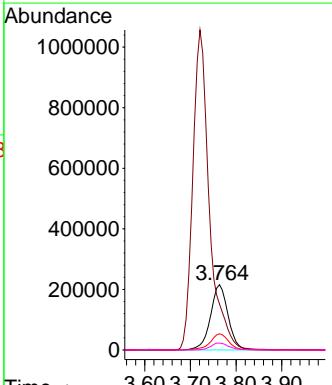



#23

**Vinyl Acetate**

Concen: 608.005 ug/l

RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150



Tgt Ion: 43 Resp: 265575

Ion Ratio Lower Upper


43 100

86 9.6 7.5 11.3



**Manual Integrations****APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

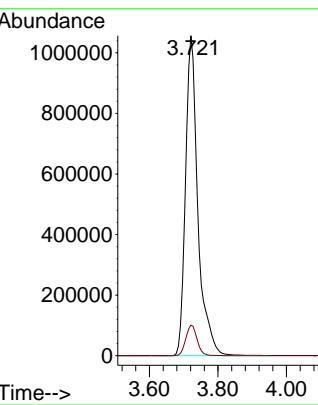

Time--&gt;

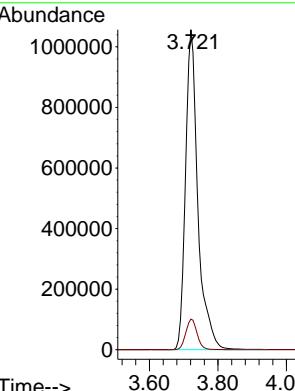

#24

**1,1-Dichloroethane**


Concen: 110.182 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45





Tgt Ion: 63 Resp: 320083


Ion Ratio Lower Upper

63 100

98 7.0 3.6 10.8


100 4.7 2.1 6.3

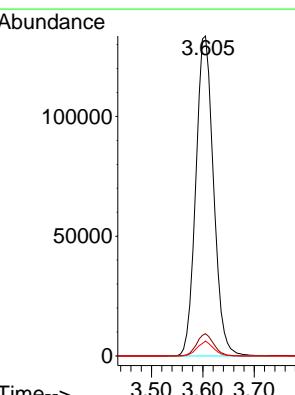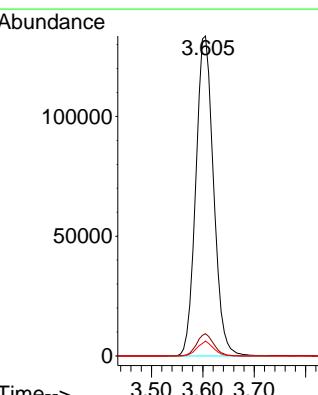

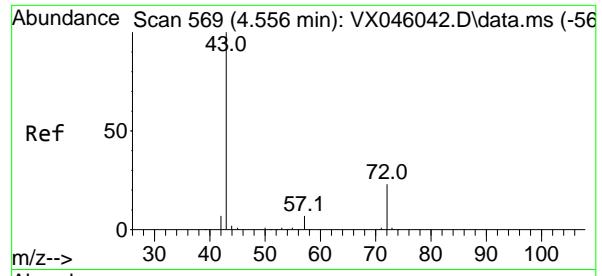

#25  
2-Butanone  
Concen: 581.292 ug/l  
RT: 4.562 min Scan# 51  
Delta R.T. 0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45



Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150

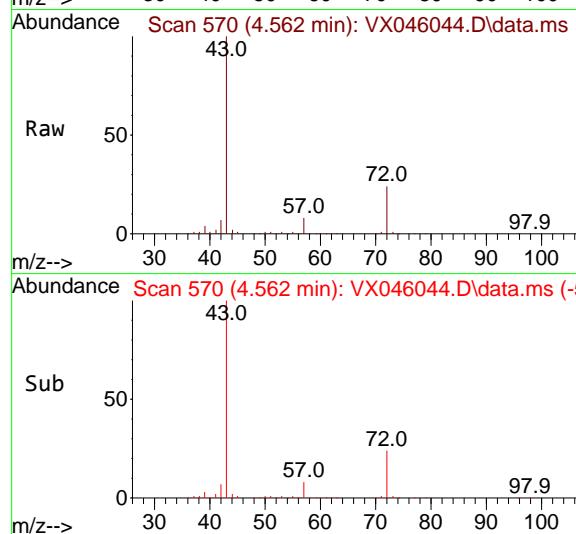


Tgt Ion: 43 Resp: 708461  
Ion Ratio Lower Upper  
43 100  
72 24.0 18.4 27.6

Manual Integrations  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025


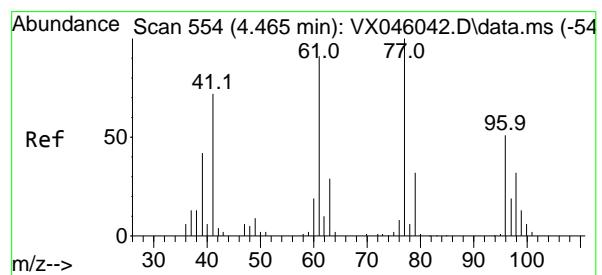
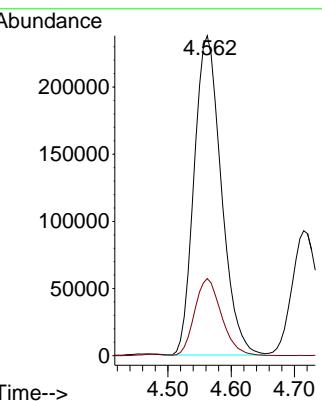


#26  
2,2-Dichloropropane  
Concen: 117.548 ug/l  
RT: 4.471 min Scan# 555  
Delta R.T. 0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

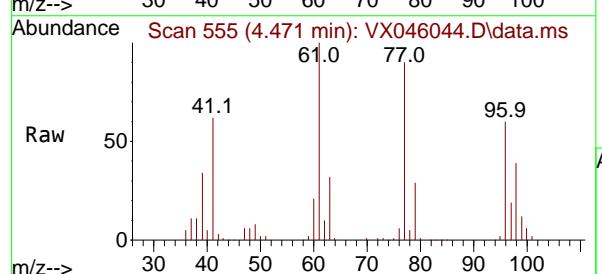

Tgt Ion: 77 Resp: 258698  
Ion Ratio Lower Upper  
77 100  
97 21.1 10.5 31.5

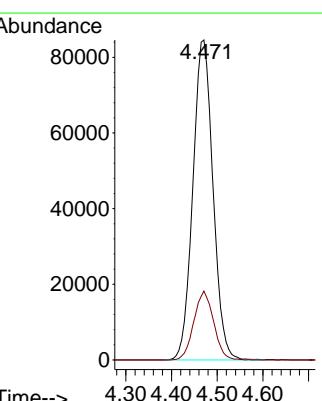







#27

cis-1,2-Dichloroethene  
Concen: 108.994 ug/l  
RT: 4.483 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

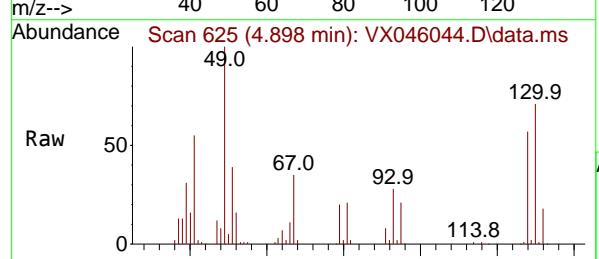


#28

Bromochloromethane  
Concen: 95.108 ug/l  
RT: 4.898 min Scan# 625  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45


Tgt Ion: 49 Resp: 146923  
Ion Ratio Lower Upper  
49 100  
129 1.8 0.0 4.0  
130 70.5 56.2 84.2




Abundance Scan 642 (5.001 min): VX046042.D\data.ms (-63)

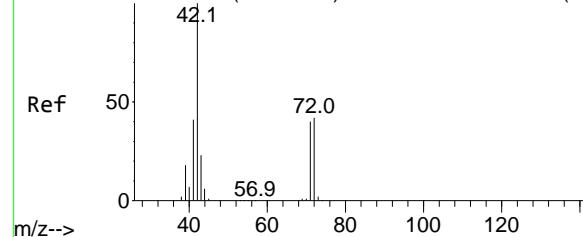


Abundance Scan 643 (5.007 min): VX046044.D\data.ms

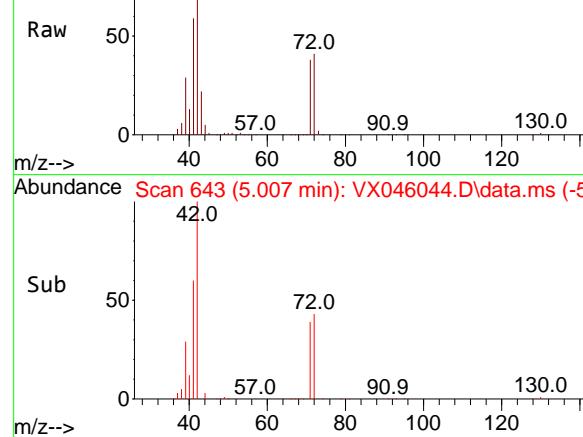


Abundance Scan 643 (5.007 min): VX046044.D\data.ms (-59)

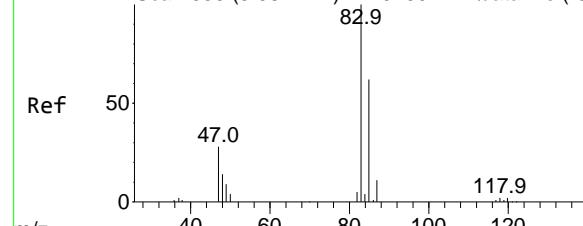

Abundance Scan 656 (5.087 min): VX046042.D\data.ms (-64)

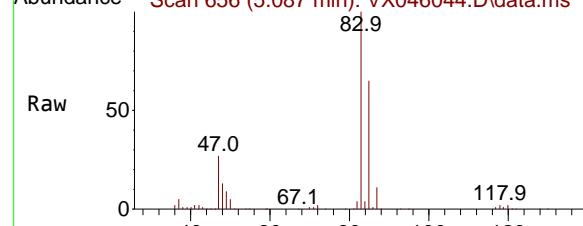

Abundance Scan 656 (5.087 min): VX046044.D\data.ms

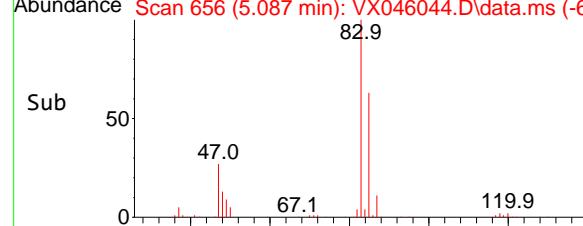

Abundance Scan 656 (5.087 min): VX046044.D\data.ms (-60)



#29

Tetrahydrofuran

Concen: 569.081 ug/l

RT: 5.007 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45


Instrument : MSVOA\_X

ClientSampleId : VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

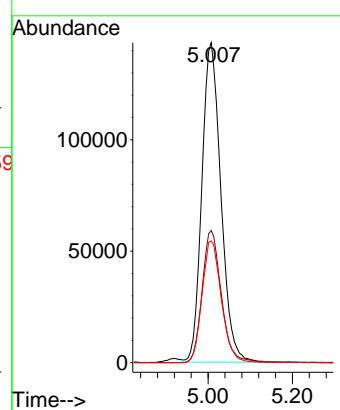

#30

Chloroform

Concen: 107.208 ug/l

RT: 5.087 min Scan# 656

Delta R.T. 0.000 min

Lab File: VX046044.D


Acq: 05 May 2025 12:45


Tgt Ion: 83 Resp: 323659

Ion Ratio Lower Upper

83 100

85 65.1 49.3 73.9



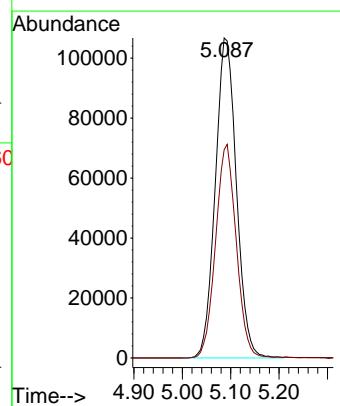




Ref 50  
0

#31  
Cyclohexane  
Concen: 116.934 ug/l  
RT: 5.458 min Scan# 717  
Delta R.T. -0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

&lt;/div



#33

1,2-Dichloroethane-d4

Concen: 93.983 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45




Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

 Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025


#34

1,4-Difluorobenzene



Concen: 50.000 ug/l

RT: 6.757 min Scan# 930







Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

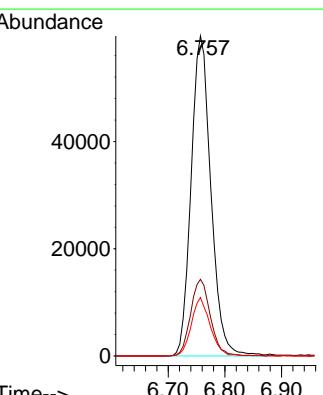 Tgt Ion:114 Resp: 144975  
 Ion Ratio Lower Upper  
 114 100  
 63 23.9 0.0 49.2  
 88 18.3 0.0 33.6


Sub

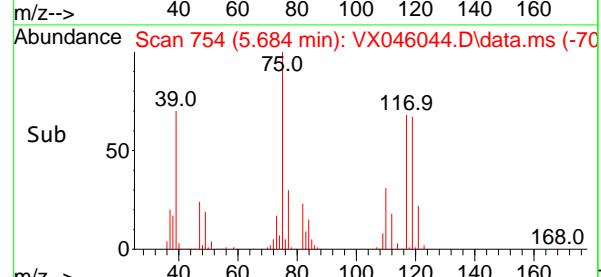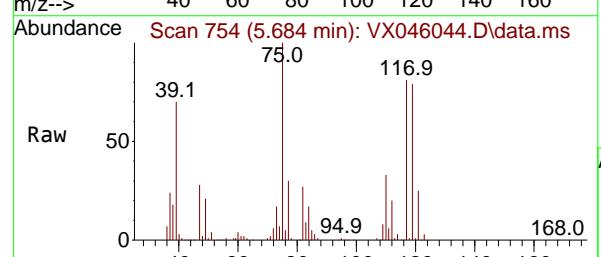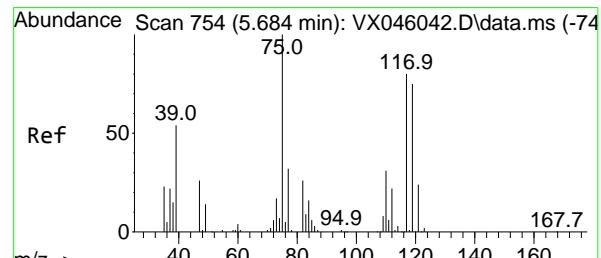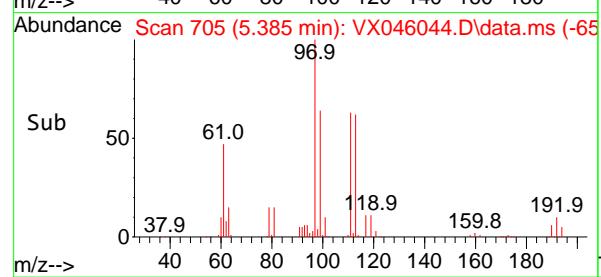

#35

Dibromofluoromethane

Concen: 98.562 ug/l

RT: 5.385 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

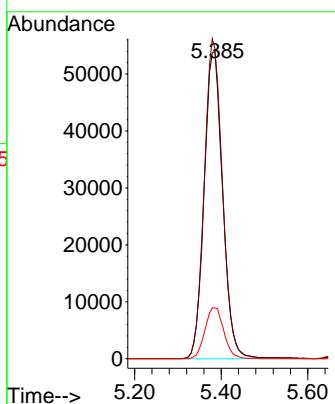

#36

1,1-Dichloropropene

Concen: 116.462 ug/l

RT: 5.684 min Scan# 754

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45


Tgt Ion: 75 Resp: 219731




Ion Ratio Lower Upper

75 100

110 32.9 16.3 48.9

77 30.8 24.3 36.5

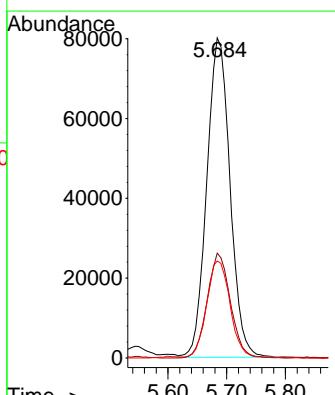

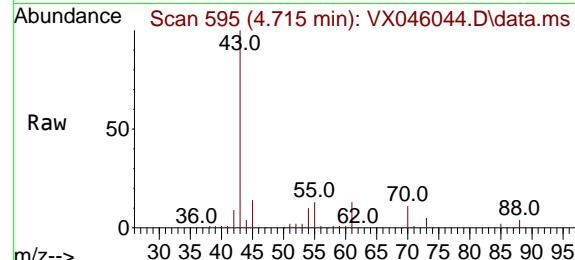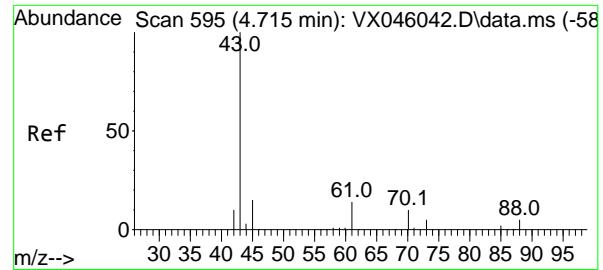

#37

Ethyl Acetate

Concen: 115.889 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

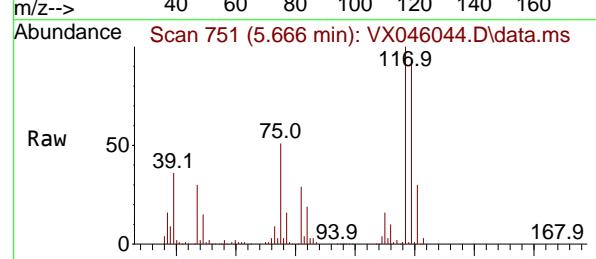

#38

Carbon Tetrachloride

Concen: 115.760 ug/l

RT: 5.666 min Scan# 751

Delta R.T. -0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45


Tgt Ion:117 Resp: 250916




Ion Ratio Lower Upper

117 100

119 94.3 75.2 112.8

121 29.7 24.2 36.4

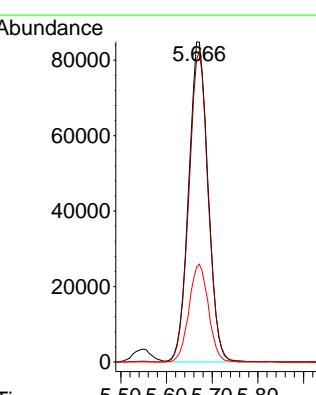



#39

Methylcyclohexane

Concen: 121.107 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

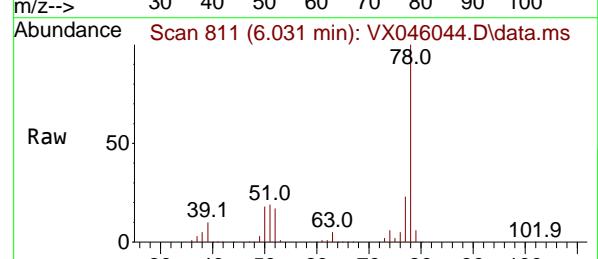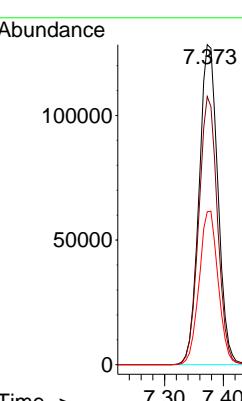

#40

Benzene

Concen: 109.813 ug/l


RT: 6.031 min Scan# 811







Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 78 Resp: 642178  
 Ion Ratio Lower Upper  
 78 100  
 77 23.4 19.0 28.4

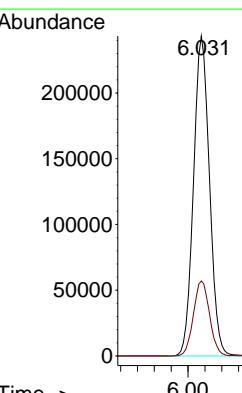



#41

Methacrylonitrile

Concen: 115.139 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

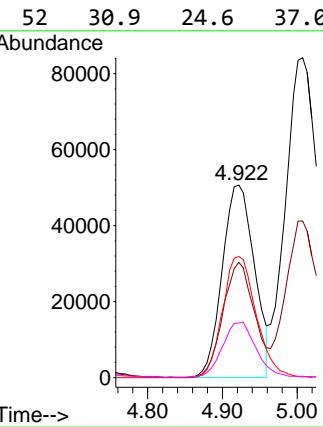

#42

1,2-Dichloroethane

Concen: 112.492 ug/l

RT: 6.080 min Scan# 819

Delta R.T. 0.000 min

Lab File: VX046044.D


Acq: 05 May 2025 12:45


Tgt Ion: 62 Resp: 271992

Ion Ratio Lower Upper

62 100

98 7.4 0.0 15.2

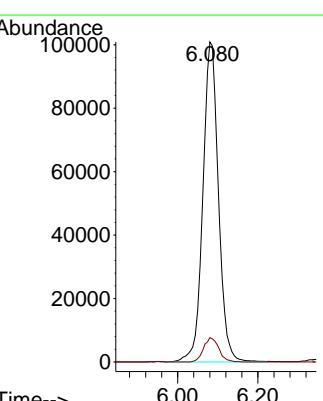



#43

Isopropyl Acetate

Concen: 123.780 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX046044.D


Acq: 05 May 2025 12:45

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC150

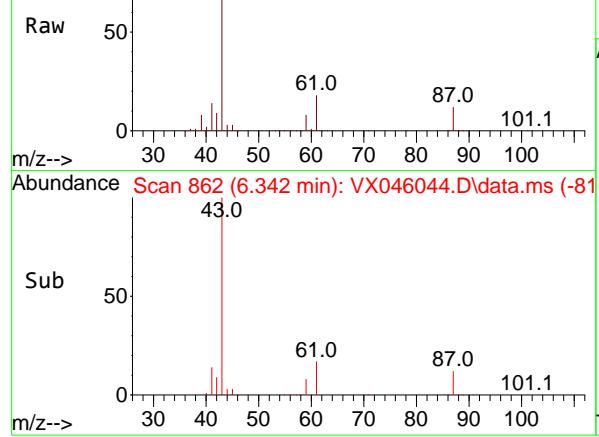Tgt Ion: 43 Resp: 44787  
Ion Ratio Lower Upper

43 100




61 18.1 14.3 21.5

87 11.7 9.5 14.3

Manual Integrations  
APPROVED



Reviewed By :John Carlone 05/06/2025




Supervised By :Mahesh Dadoda 05/06/2025
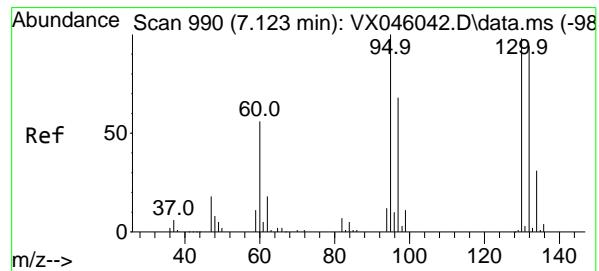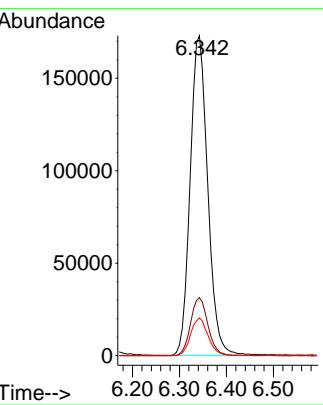
#44  
Trichloroethene  
Concen: 114.032 ug/l  
RT: 7.117 min Scan# 989  
Delta R.T. -0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45Tgt Ion:130 Resp: 157641  
Ion Ratio Lower Upper

130 100

95 105.9 0.0 204.2

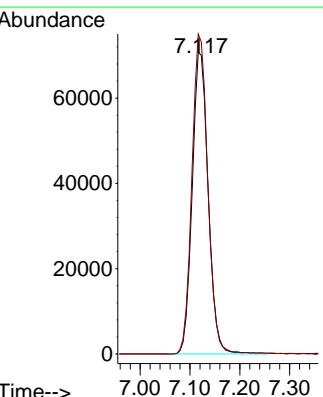



#45

1,2-Dichloropropane

Concen: 113.217 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

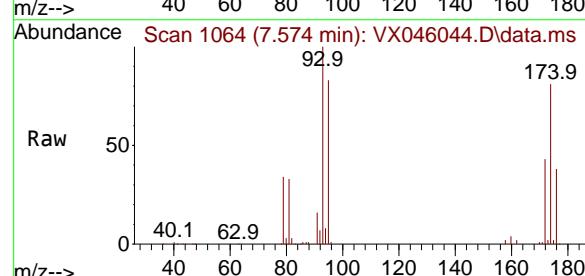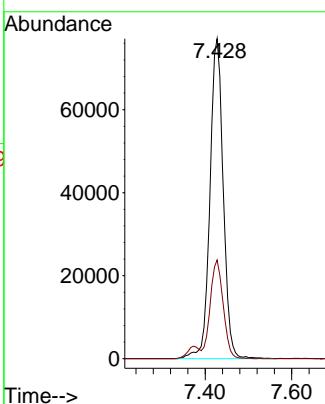

#46

Dibromomethane

Concen: 109.869 ug/l

RT: 7.574 min Scan# 1064

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45


Tgt Ion: 93 Resp: 125846


Ion Ratio Lower Upper

93 100

95 82.4 65.6 98.4

174 85.0 68.2 102.2

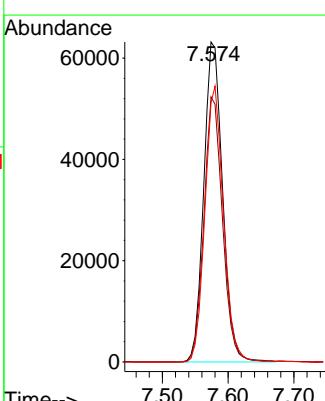

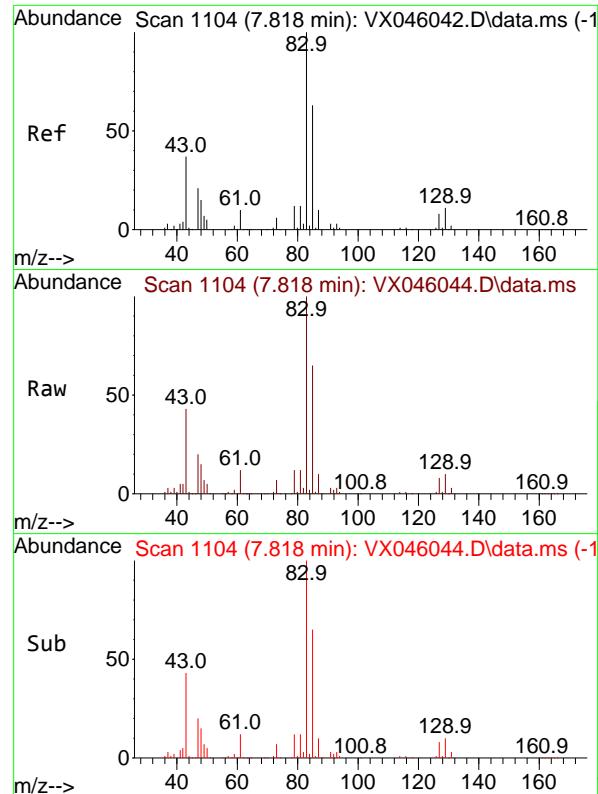


#47  
 Bromodichloromethane  
 Concen: 116.365 ug/l  
 RT: 7.818 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: VX046044.D  
 Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

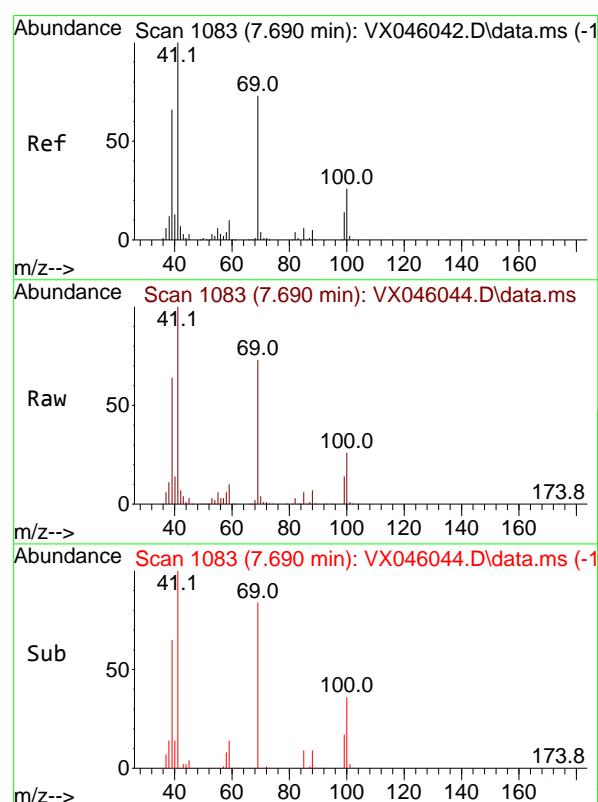


#48  
 Methyl methacrylate  
 Concen: 124.356 ug/l  
 RT: 7.690 min Scan# 1083  
 Delta R.T. 0.000 min  
 Lab File: VX046044.D  
 Acq: 05 May 2025 12:45

Tgt Ion: 41 Resp: 231040  
 Ion Ratio Lower Upper  
 41 100  
 69 73.0 58.5 87.7  
 39 63.8 51.7 77.5

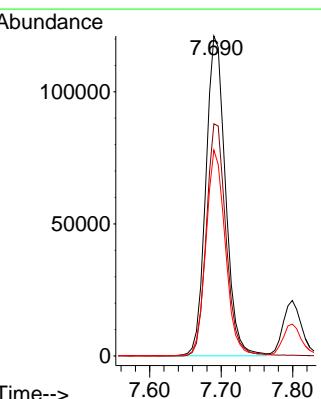



Abundance Scan 1079 (7.665 min): VX046044.D\data.ms

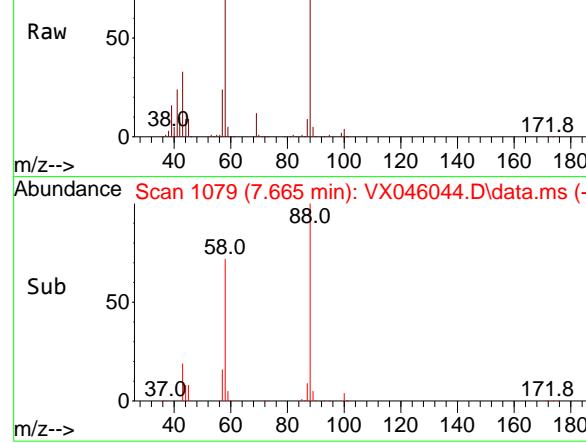

Sub

Abundance Scan 1079 (7.665 min): VX046044.D\data.ms (-1)

m/z-->

Time-->

Abundance

#49

1,4-Dioxane

Concen: 2241.695 ug/l

RT: 7.665 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC150

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance Scan 1240 (8.647 min): VX046042.D\data.ms (-1)

m/z-->

Ref

Abundance Scan 1240 (8.647 min): VX046044.D\data.ms

m/z-->

Raw

Abundance Scan 1240 (8.647 min): VX046044.D\data.ms (-1)

m/z-->

Sub

Abundance Scan 1240 (8.647 min): VX046044.D\data.ms (-1)

m/z-->

Time-->

Abundance

#50

Toluene-d8

Concen: 101.252 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45






Tgt Ion: 98 Resp: 554390

Ion Ratio Lower Upper

98 100

100 65.4 53.5 80.3

Abundance

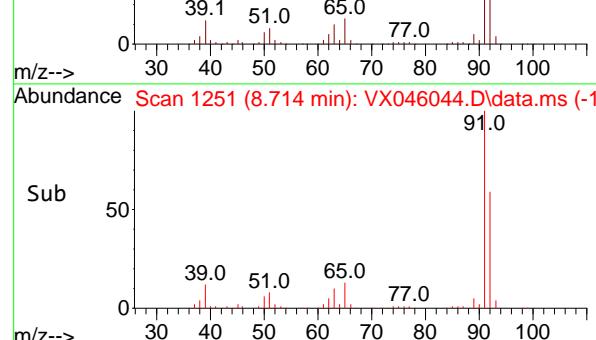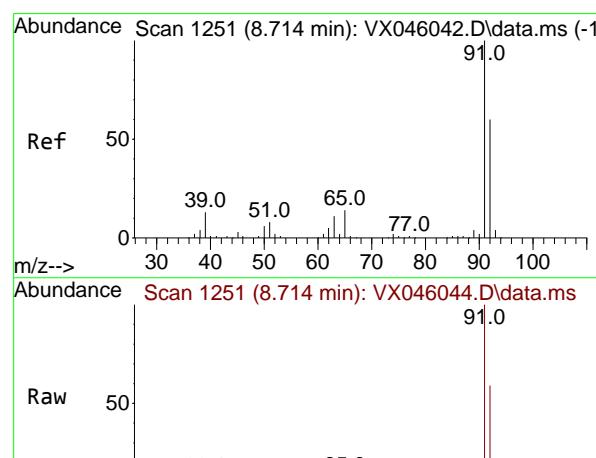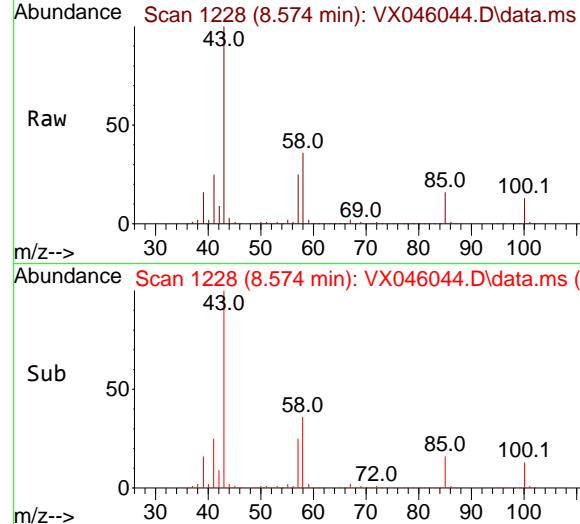

#51

4-Methyl-2-Pentanone

Concen: 577.831 ug/l

RT: 8.574 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument :

MSVOA\_X





ClientSampleId :


VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

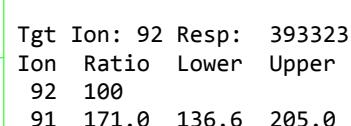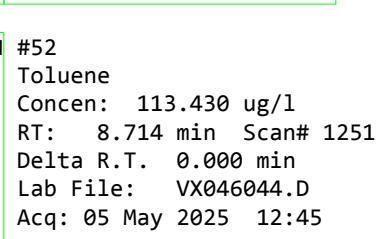


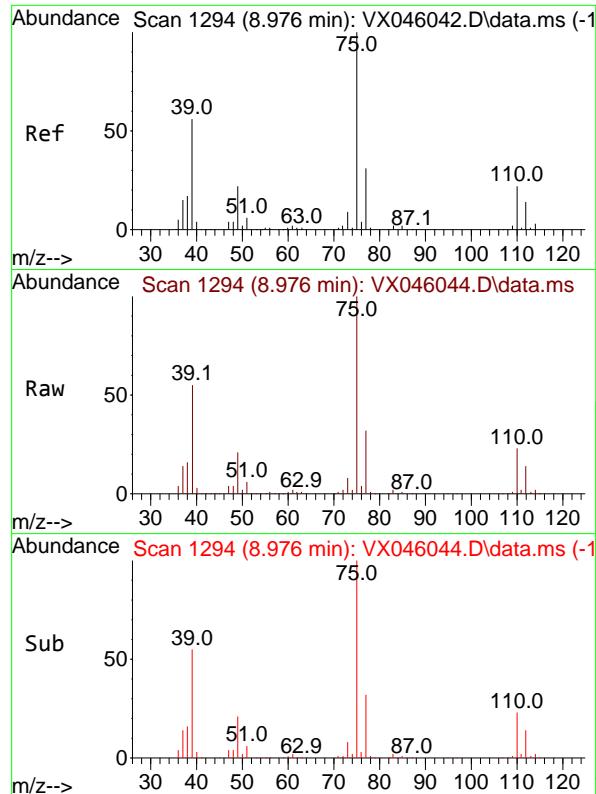


#53  
t-1,3-Dichloropropene  
Concen: 138.001 ug/l  
RT: 8.976 min Scan# 1194  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

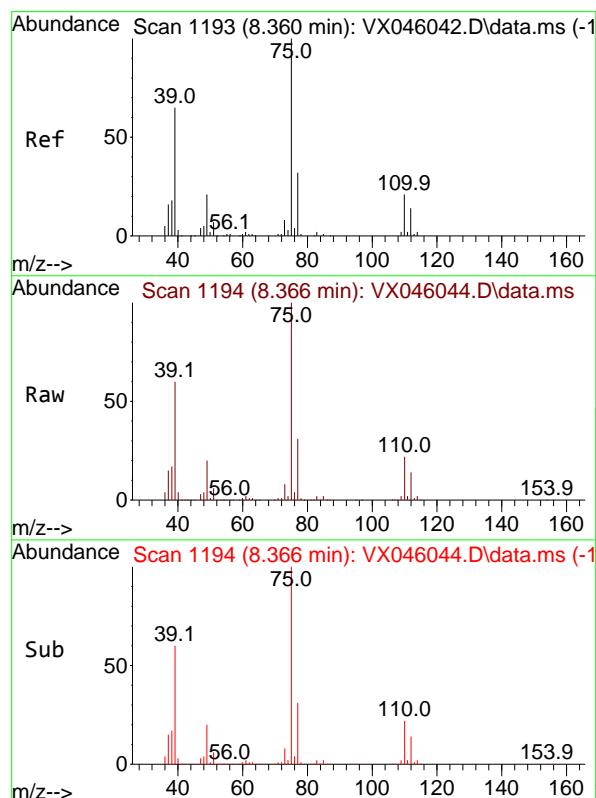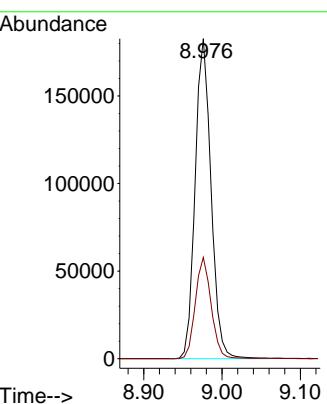

#54  
cis-1,3-Dichloropropene  
Concen: 124.658 ug/l  
RT: 8.366 min Scan# 1194  
Delta R.T. 0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Tgt Ion: 75 Resp: 271054  
Ion Ratio Lower Upper  
75 100  
77 31.4 25.4 38.0  
39 60.0 52.2 78.4

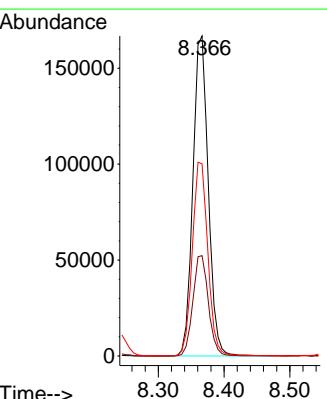

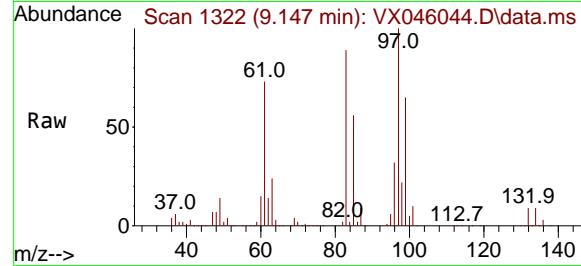

#55

1,1,2-Trichloroethane

Concen: 110.551 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#56

Ethyl methacrylate

Concen: 127.968 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45


Tgt Ion: 69 Resp: 277921



Ion Ratio Lower Upper

69 100

41 75.4 60.8 91.2

39 47.2 39.0 58.6

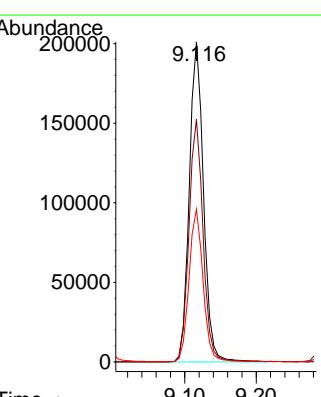

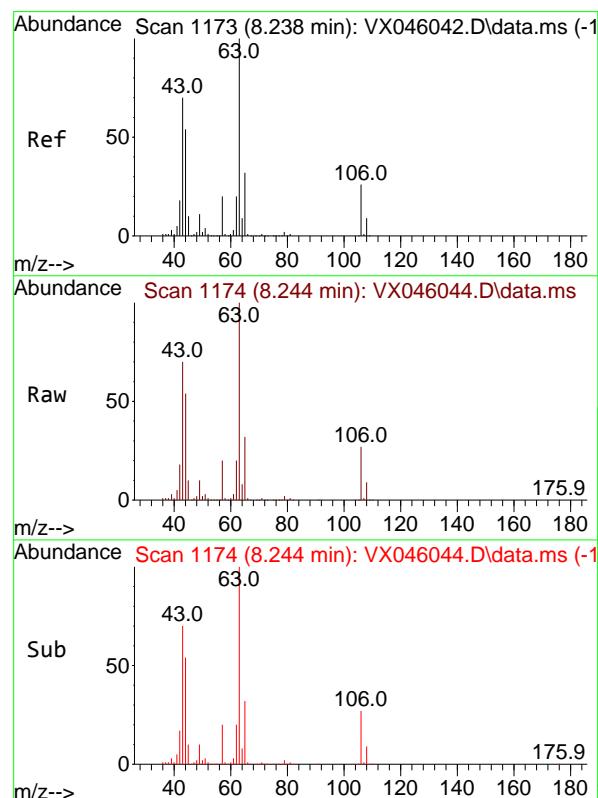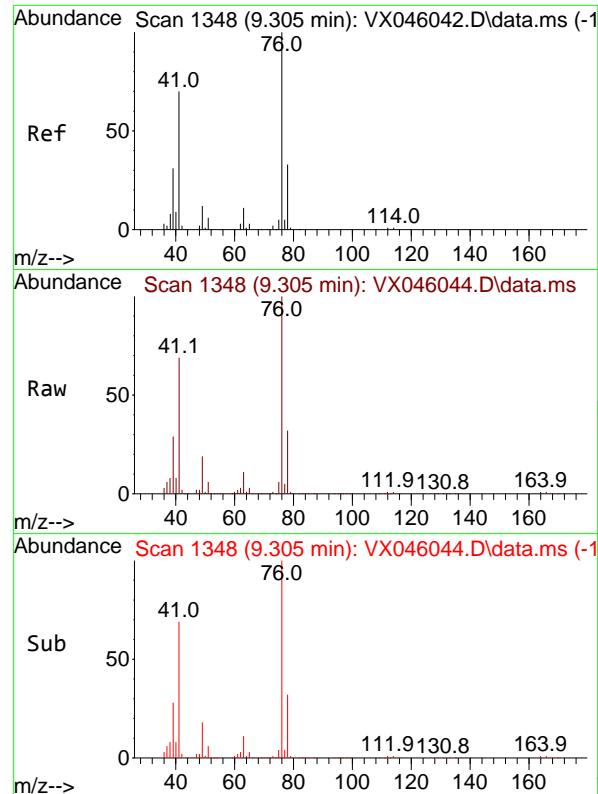

#57

1,3-Dichloropropane

Concen: 109.813 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#58

2-Chloroethyl Vinyl ether

Concen: 697.344 ug/l

RT: 8.244 min Scan# 1174

Delta R.T. 0.006 min

Lab File: VX046044.D


Acq: 05 May 2025 12:45







Tgt Ion: 63 Resp: 680608

Ion Ratio Lower Upper

63 100

106 26.7 21.5 32.3





#59

2-Hexanone

Concen: 571.094 ug/l

RT: 9.433 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#60

Dibromochloromethane

Concen: 122.915 ug/l

RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX046044.D


Acq: 05 May 2025 12:45




Tgt Ion:129 Resp: 187497

Ion Ratio Lower Upper

129 100

127 77.1 39.3 117.8

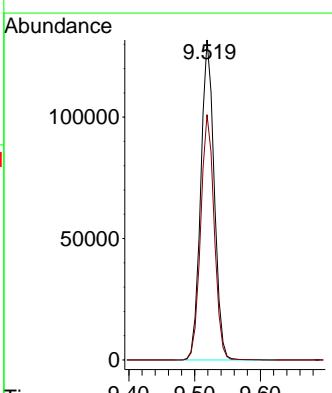

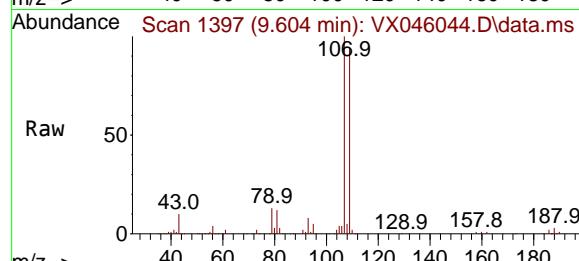

#61

1,2-Dibromoethane

Concen: 115.087 ug/l

RT: 9.604 min Scan# 1397

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

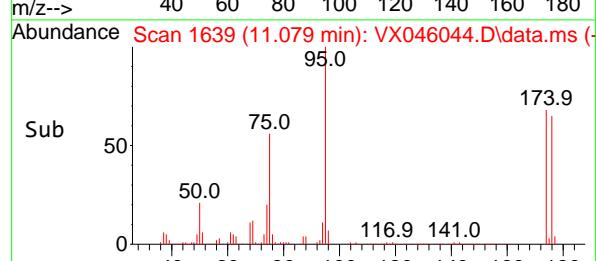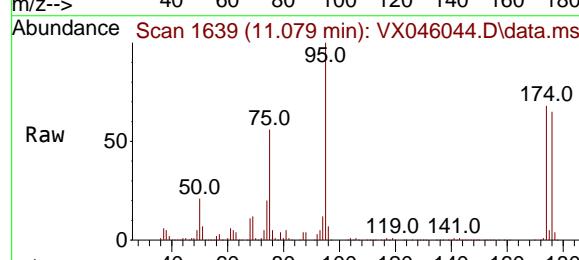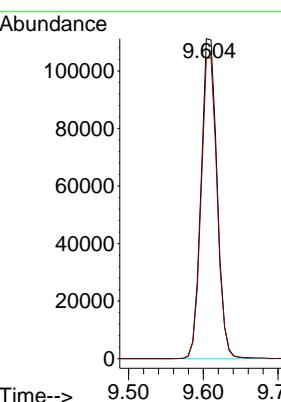

#62

4-Bromofluorobenzene

Concen: 109.174 ug/l

RT: 11.079 min Scan# 1639


Delta R.T. 0.000 min


Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 95 Resp: 217536

Ion	Ratio	Lower	Upper
95	100		
174	67.5	0.0	135.8
176	64.4	0.0	131.4

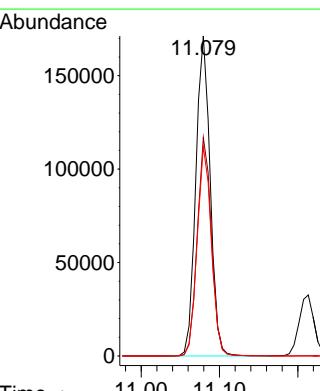

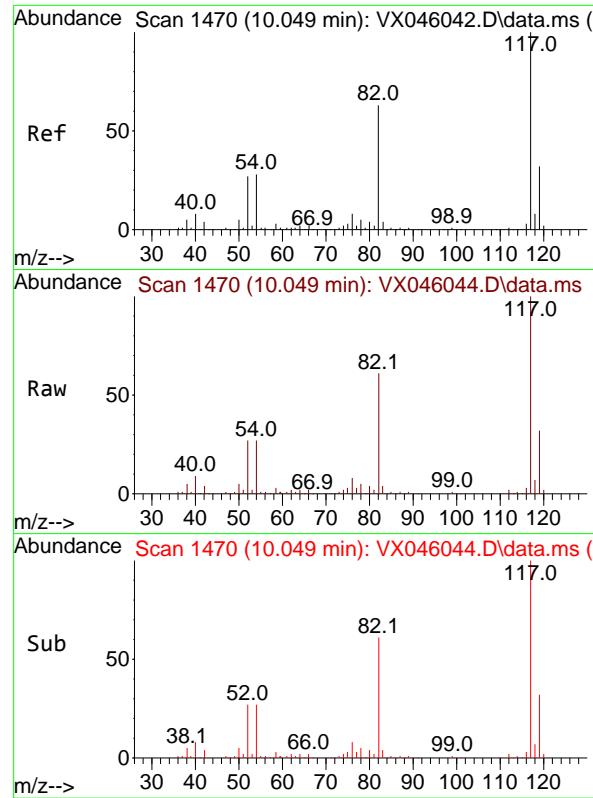

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

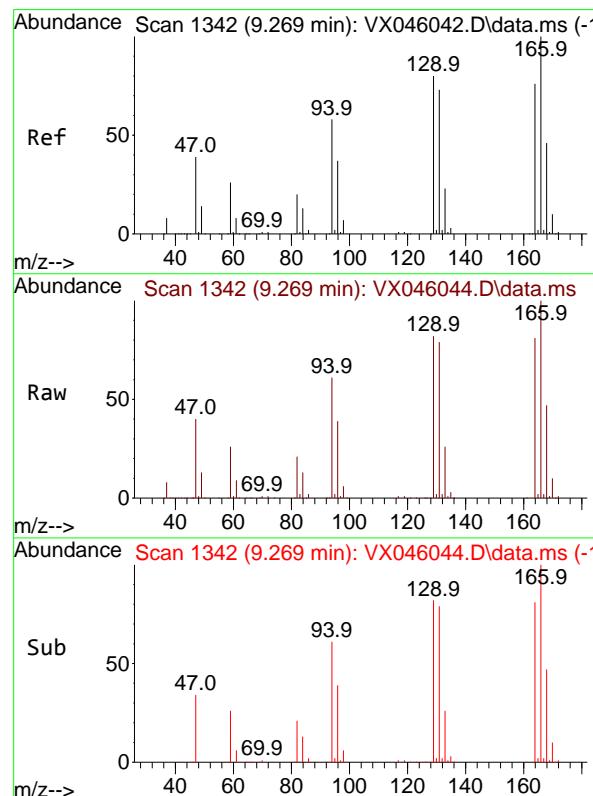

#64

Tetrachloroethene


Concen: 100.918 ug/l


RT: 9.269 min Scan# 1342

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

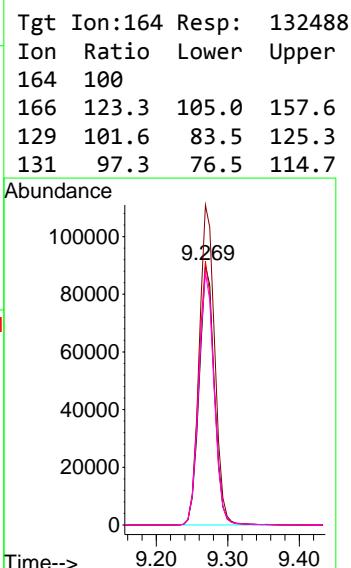


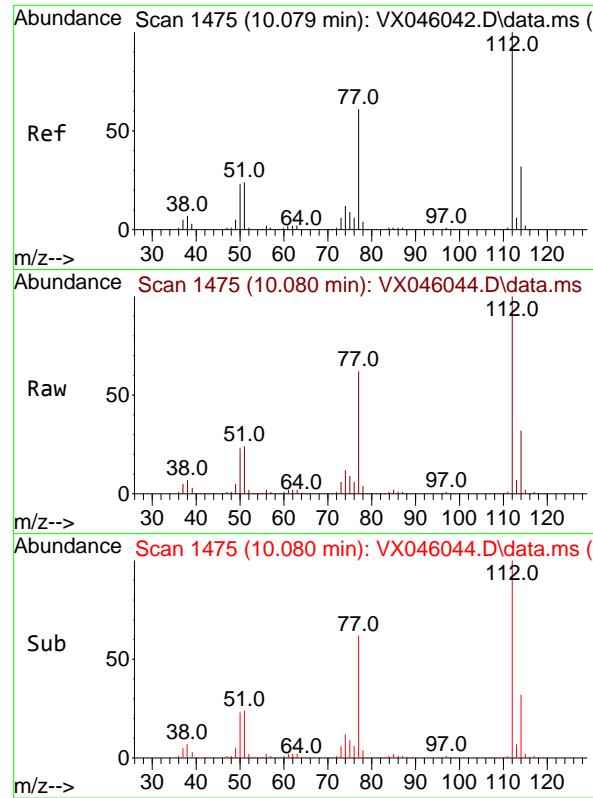


#65  
Chlorobenzene  
Concen: 108.615 ug/l  
RT: 10.080 min Scan# 1475  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

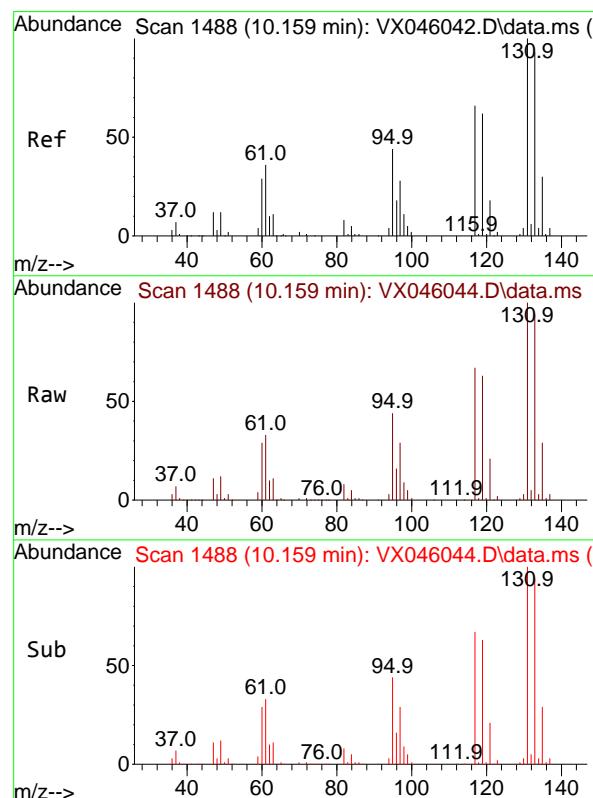

#66  
1,1,1,2-Tetrachloroethane  
Concen: 115.333 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Tgt Ion:131 Resp: 152173  
Ion Ratio Lower Upper  
131 100  
133 95.7 47.3 141.9  
119 64.0 31.6 95.0

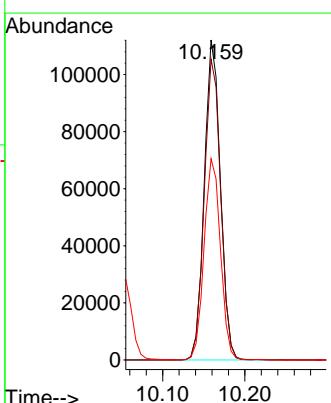



#67

Ethyl Benzene

Concen: 116.421 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#68

m/p-Xylenes

Concen: 234.349 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX046044.D



Acq: 05 May 2025 12:45


Tgt Ion:106 Resp: 570913

Ion Ratio Lower Upper

106 100

91 214.2 171.2 256.8




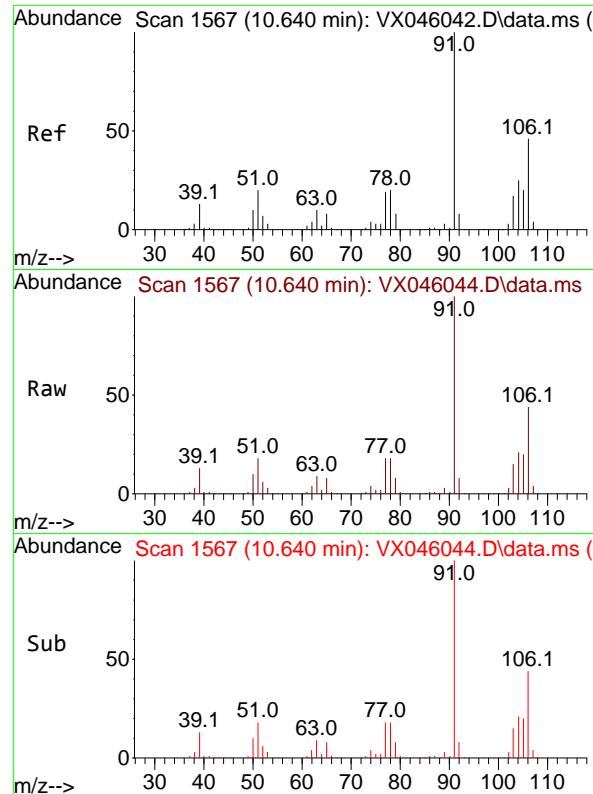

#69  
o-Xylene  
Concen: 113.990 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45  
ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

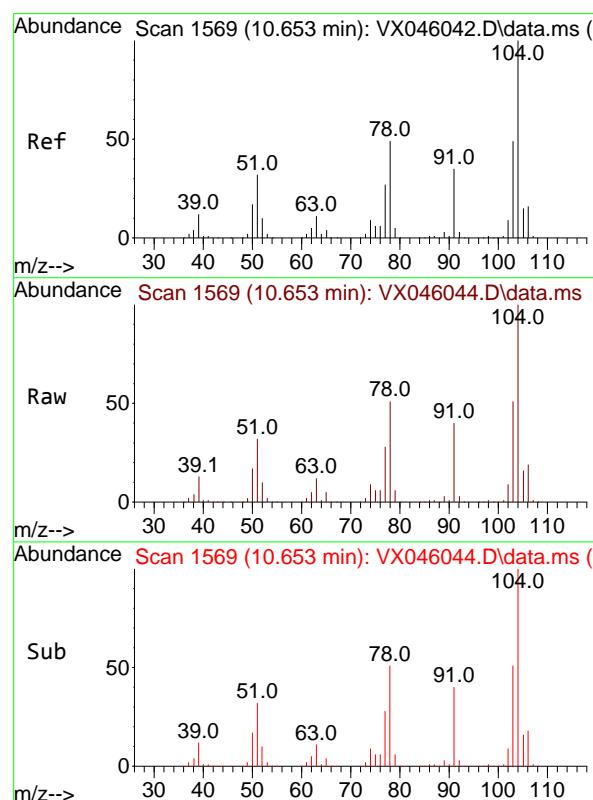

#70  
Styrene  
Concen: 120.694 ug/l  
RT: 10.653 min Scan# 1569  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45


Tgt Ion:104 Resp: 474254  
Ion Ratio Lower Upper  
104 100  
78 57.2 45.7 68.5  
103 55.5 43.7 65.5

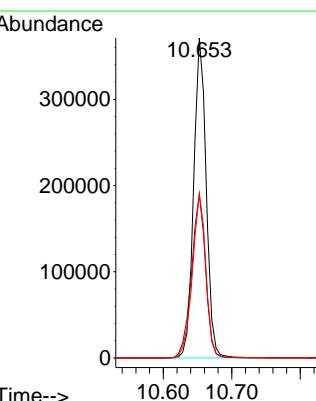

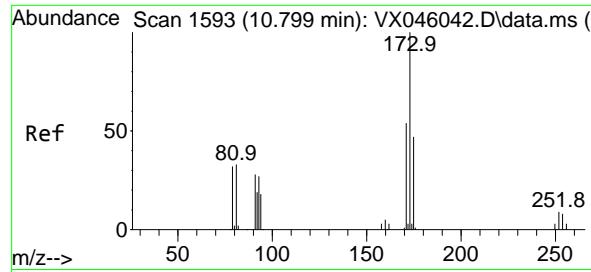



#71  
Bromoform  
Concen: 127.128 ug/l  
RT: 10.799 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150

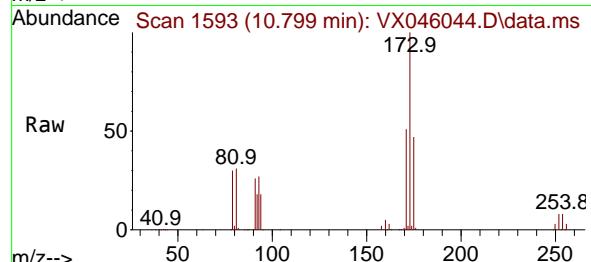


Tgt Ion:173 Resp: 125980  
Ion Ratio Lower Upper  
173 100  
175 47.3 23.4 70.0  
254 0.1 0.0 0.0



Manual Integrations APPROVED  
Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

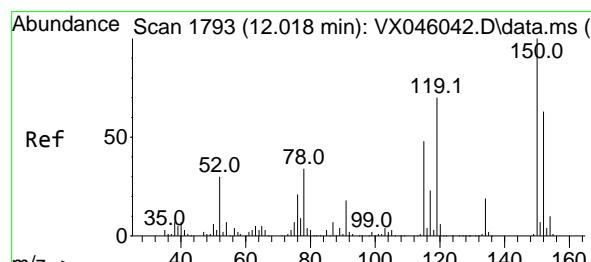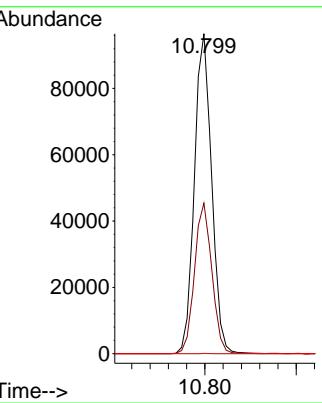


#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

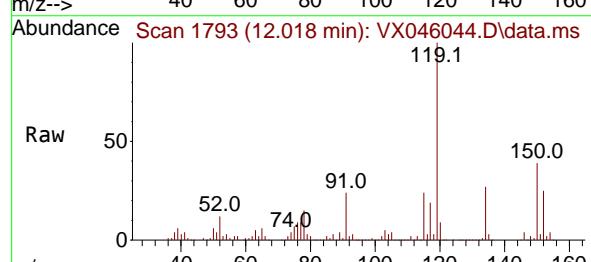

Tgt Ion:152 Resp: 60345  
Ion Ratio Lower Upper  
152 100  
115 150.7 46.9 140.7#  
150 211.6 0.0 351.0

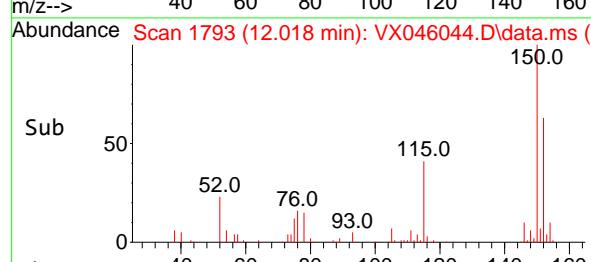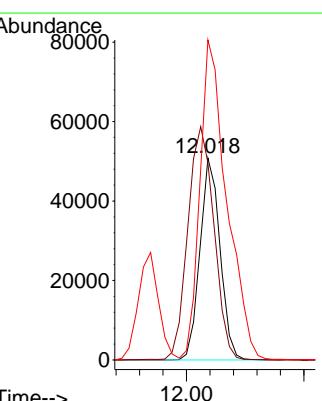

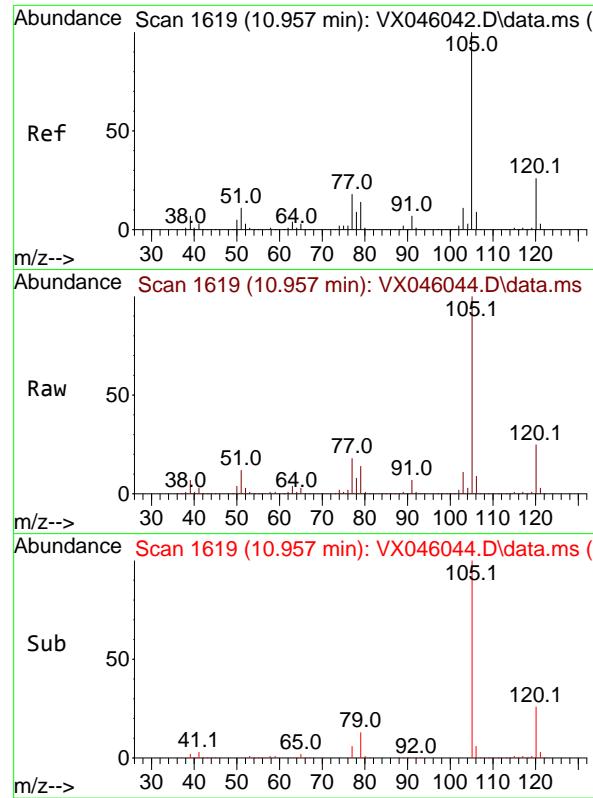

#73

Isopropylbenzene

Concen: 114.312 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

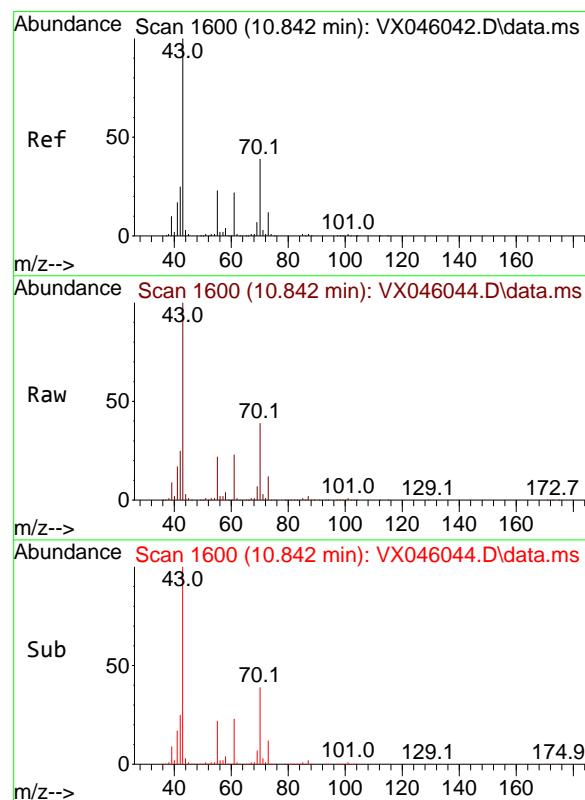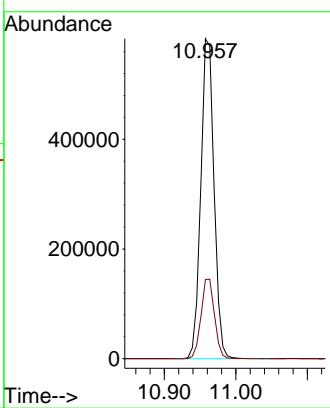

#74

N-amyl acetate

Concen: 120.944 ug/l


RT: 10.842 min Scan# 1600


Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt	Ion:	43	Resp:	396877
Ion	Ratio	Lower	Upper	
43	100			
70	38.5	30.9	46.3	
55	22.5	18.7	28.1	
61	22.5	17.1	25.7	

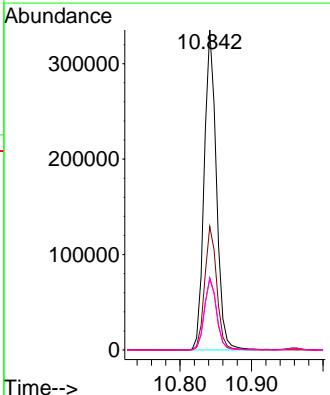


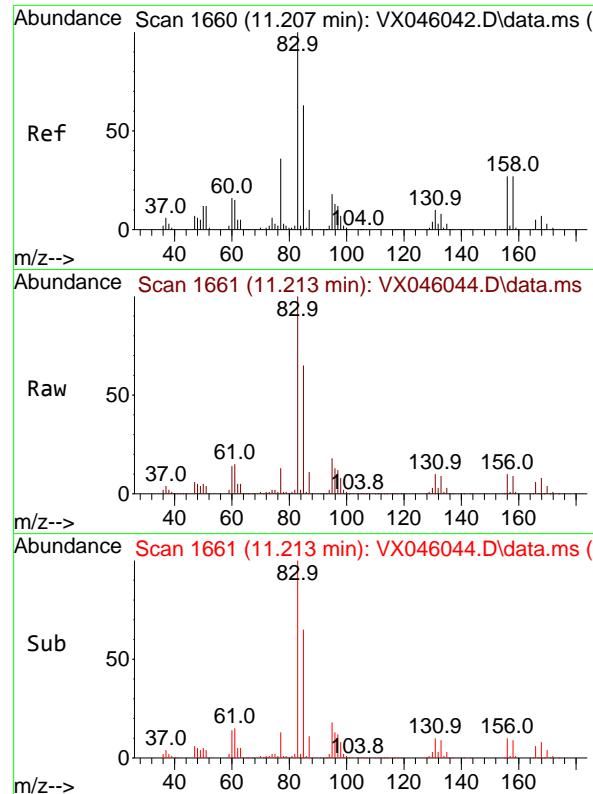


#75  
1,1,2,2-Tetrachloroethane  
Concen: 104.018 ug/l  
RT: 11.213 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carbone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

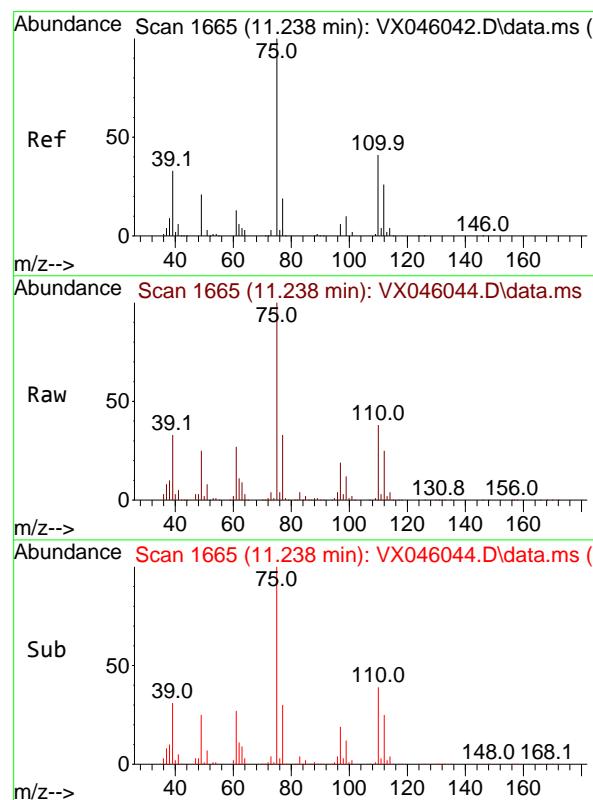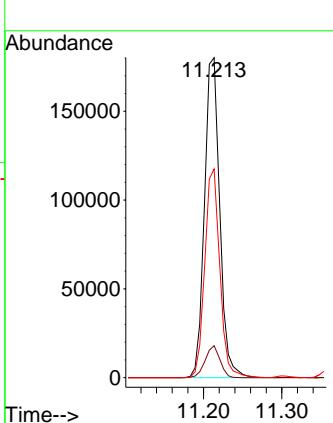

#76  
1,2,3-Trichloropropane  
Concen: 84.960 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Tgt Ion: 75 Resp: 213744  
Ion Ratio Lower Upper  
75 100  
77 42.4 20.5 61.5



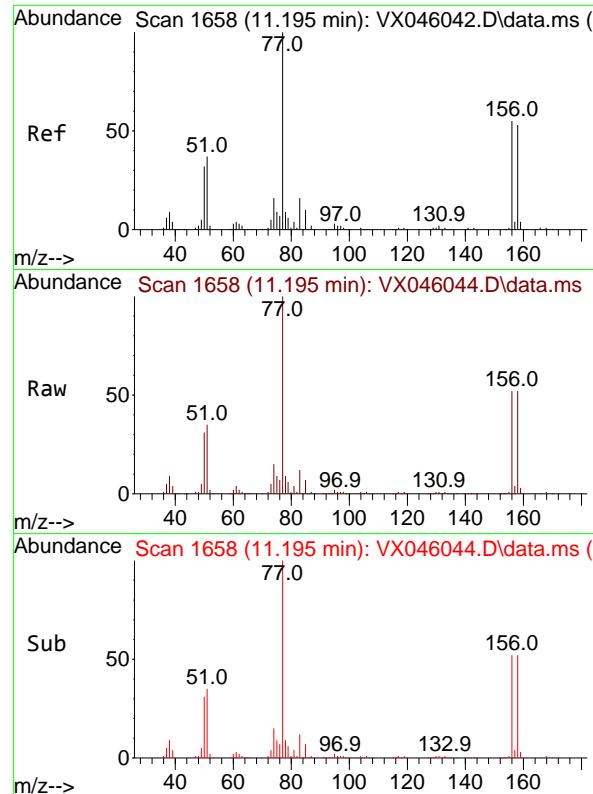

#77

Bromobenzene

Concen: 110.297 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

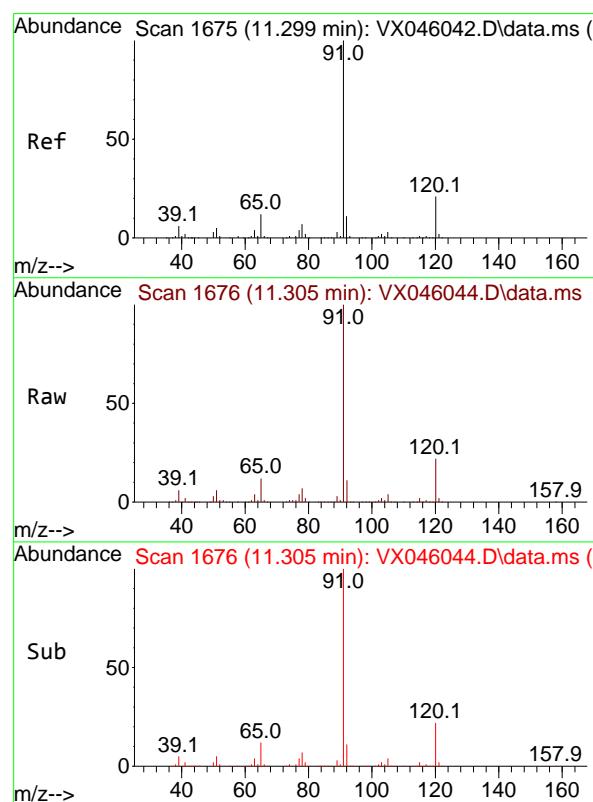

#78

n-propylbenzene

Concen: 119.448 ug/l

RT: 11.305 min Scan# 1676


Delta R.T. 0.006 min







Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 91 Resp: 881218

Ion	Ratio	Lower	Upper
91	100		
120	21.7	10.8	32.4

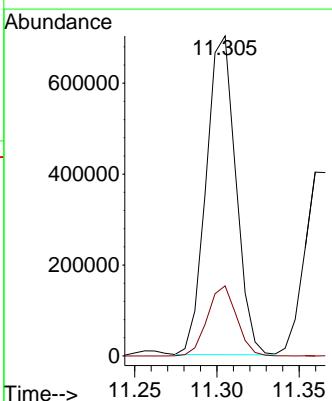



#79

2-Chlorotoluene

Concen: 107.514 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

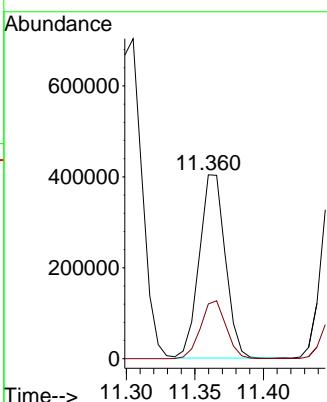

#80

1,3,5-Trimethylbenzene

Concen: 112.825 ug/l


RT: 11.451 min Scan# 1700


Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion:105 Resp: 616477  
 Ion Ratio Lower Upper  
 105 100  
 120 46.0 23.1 69.2

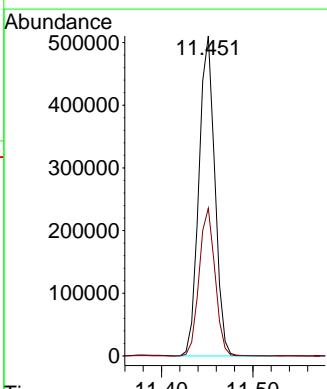


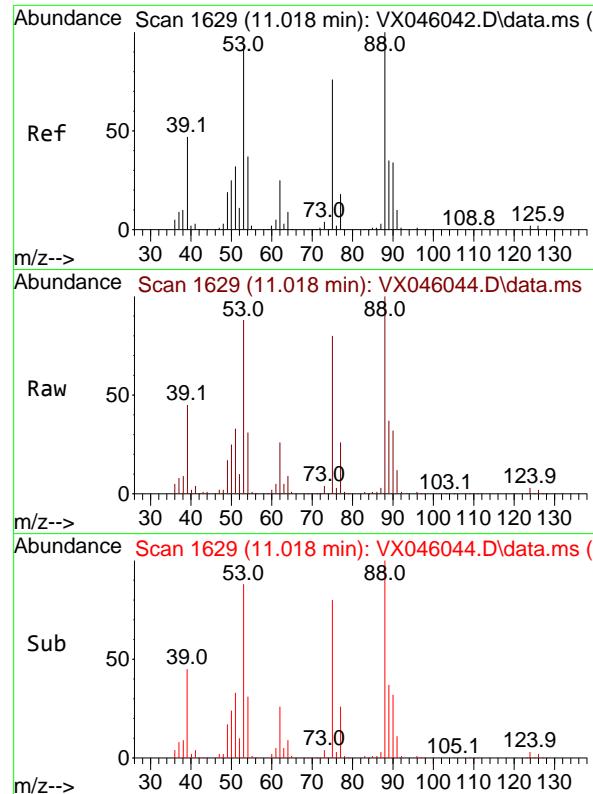


#81  
trans-1,4-Dichloro-2-butene  
Concen: 134.609 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

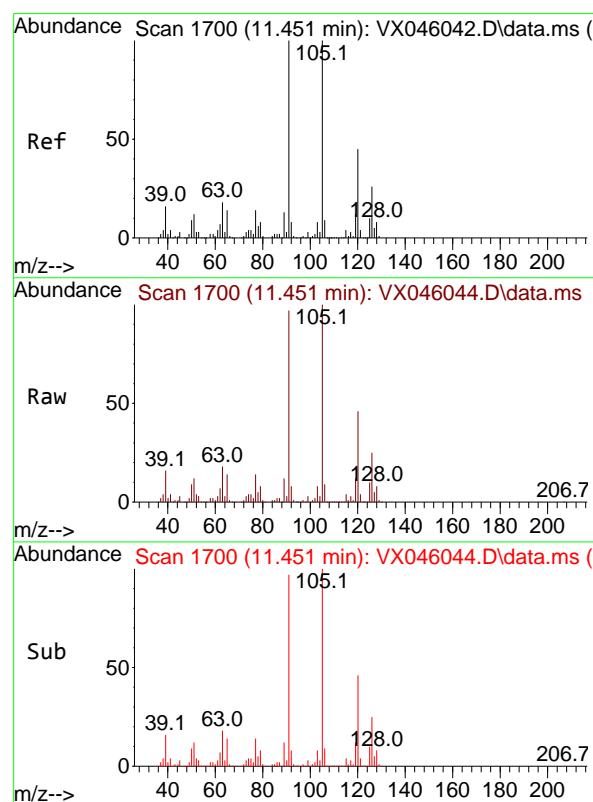

#82  
4-Chlorotoluene  
Concen: 111.948 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Tgt Ion: 91 Resp: 611736  
Ion Ratio Lower Upper  
91 100  
126 26.7 13.3 39.8

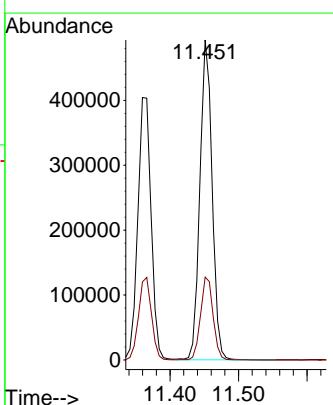



#83

tert-Butylbenzene

Concen: 115.065 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

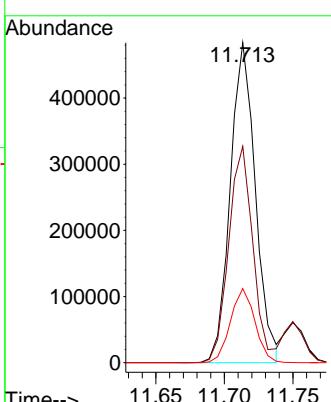

#84

1,2,4-Trimethylbenzene

Concen: 114.236 ug/l


RT: 11.750 min Scan# 1749




Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt	Ion:105	Resp:	623456
Ion	Ratio	Lower	Upper
105	100		
120	43.1	21.2	63.6

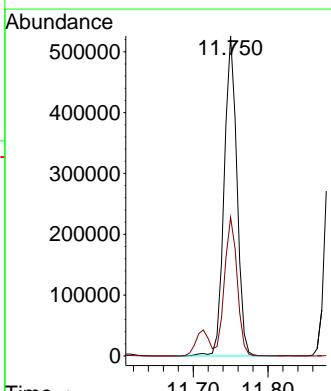



#85

sec-Butylbenzene

Concen: 118.023 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#86

p-Isopropyltoluene

Concen: 121.113 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt

Ion

Ratio

Lower

Upper

100


100


19.1

9.7

29.1

Tgt	Ion	Ion	Resp:	651531
			Lower	
119	100			
134	25.4	12.5	37.5	
91	27.0	13.8	41.4	

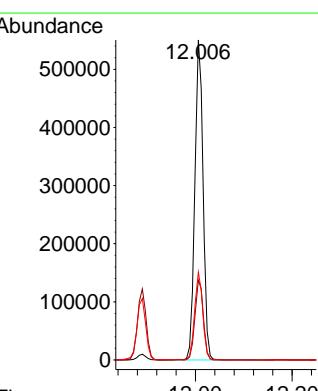

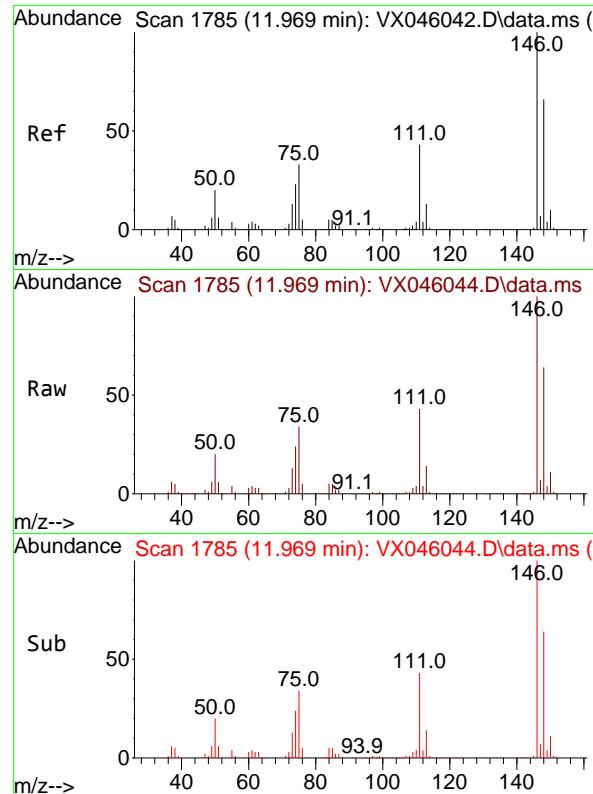

#87

1,3-Dichlorobenzene

Concen: 110.394 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

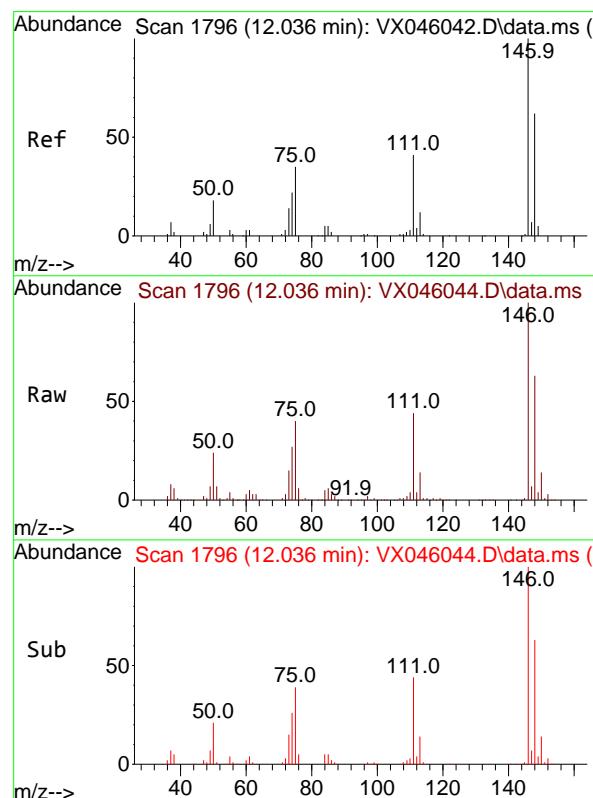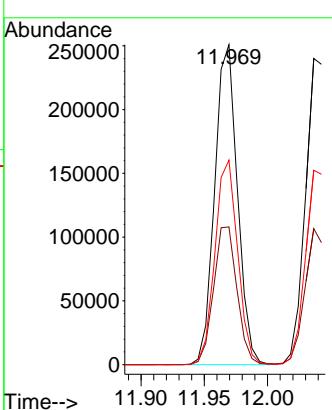

#88

1,4-Dichlorobenzene

Concen: 112.167 ug/l


RT: 12.036 min Scan# 1796


Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt	Ion:146	Resp:	311752
Ion	Ratio	Lower	Upper
146	100		
111	43.0	21.3	63.9
148	63.9	31.9	95.5



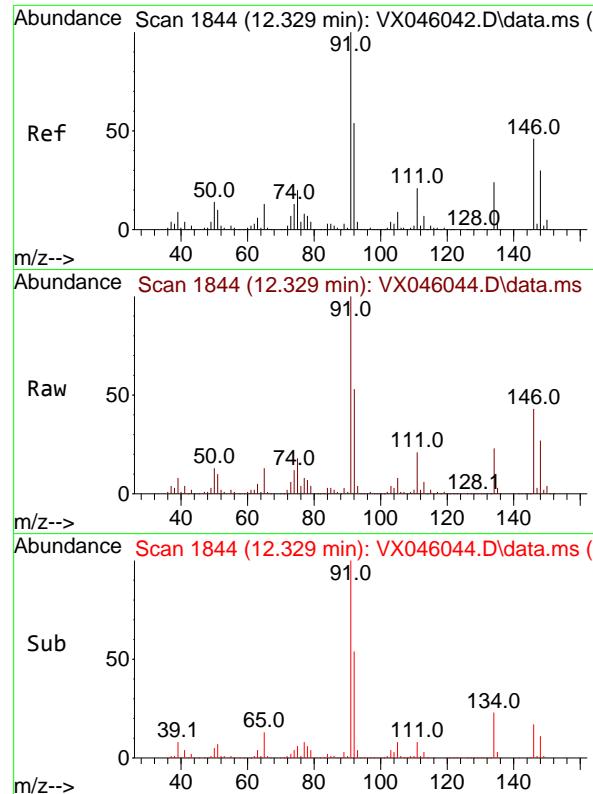

#89

n-Butylbenzene

Concen: 129.533 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

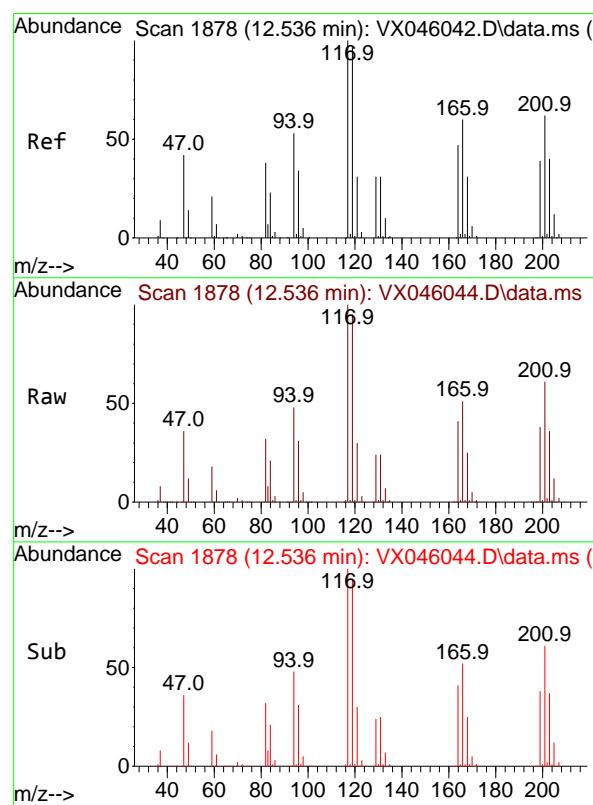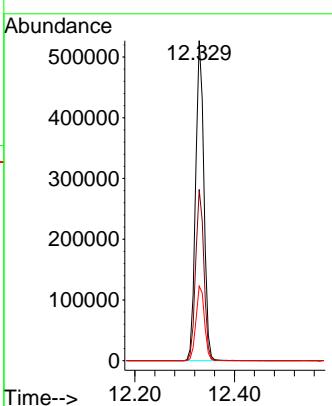

#90

Hexachloroethane

Concen: 123.091 ug/l

RT: 12.536 min Scan# 1878


Delta R.T. 0.000 min


Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion:117 Resp: 123188

		Lower	Upper
117	100		
201	63.2	31.6	94.7



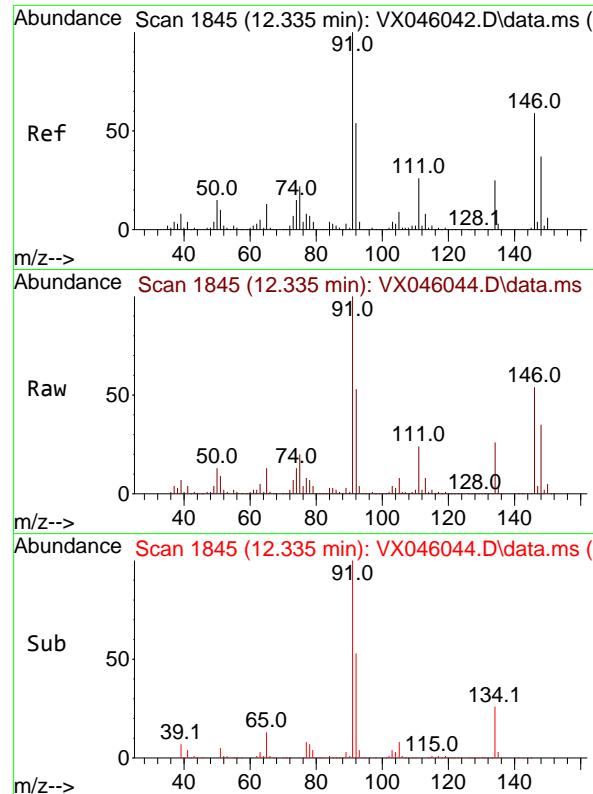

#91

1,2-Dichlorobenzene

Concen: 111.506 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

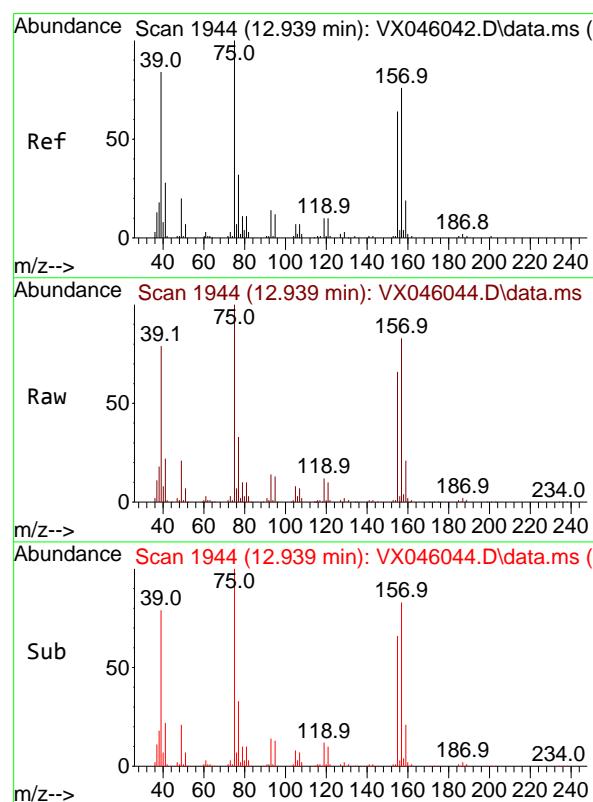

#92

1,2-Dibromo-3-Chloropropane

Concen: 120.915 ug/l

RT: 12.939 min Scan# 1944


Delta R.T. 0.000 min


Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt Ion: 75 Resp: 64438

Ion	Ratio	Lower	Upper
75	100		
155	69.6	34.9	104.8
157	88.4	43.8	131.4

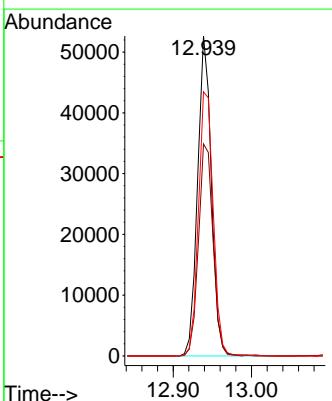

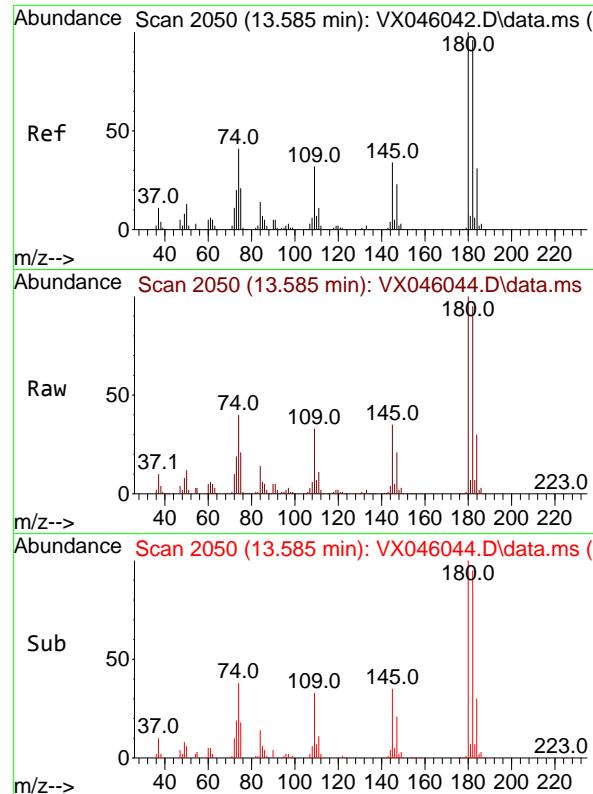

#93

1,2,4-Trichlorobenzene

Concen: 134.366 ug/l

RT: 13.585 min Scan# 20325

Delta R.T. 0.000 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC150

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

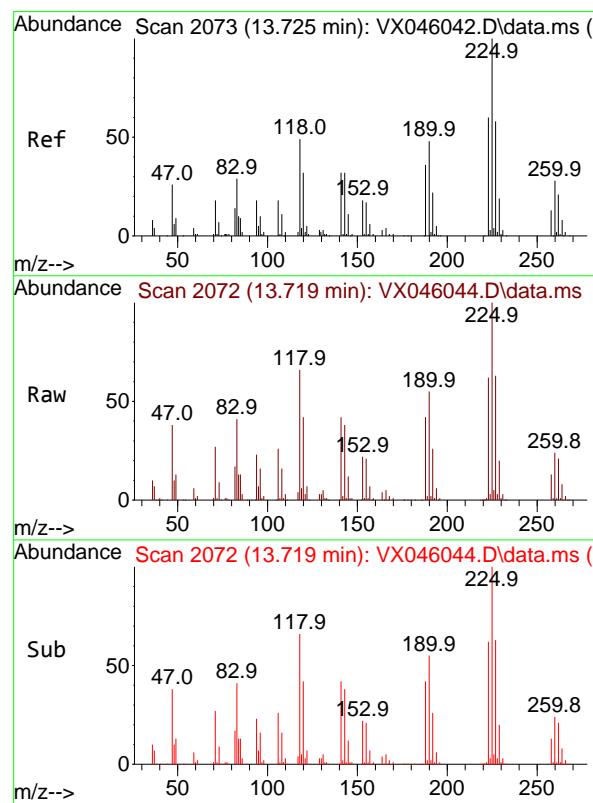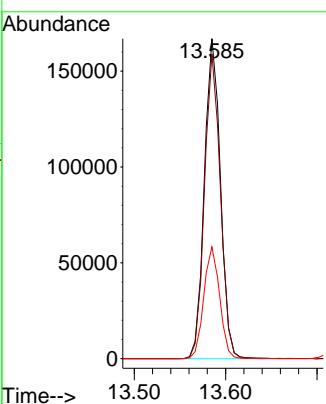

#94

Hexachlorobutadiene

Concen: 113.857 ug/l


RT: 13.719 min Scan# 2072


Delta R.T. -0.006 min

Lab File: VX046044.D

Acq: 05 May 2025 12:45

Tgt	Ion:225	Resp:	80558
Ion	Ratio	Lower	Upper
225	100		
223	62.5	30.8	92.4
227	63.1	30.9	92.7

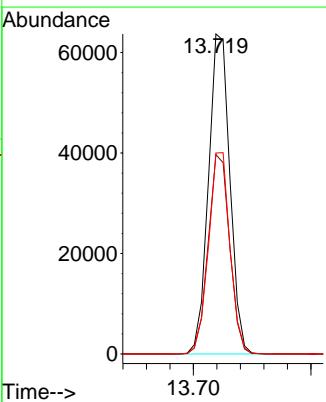


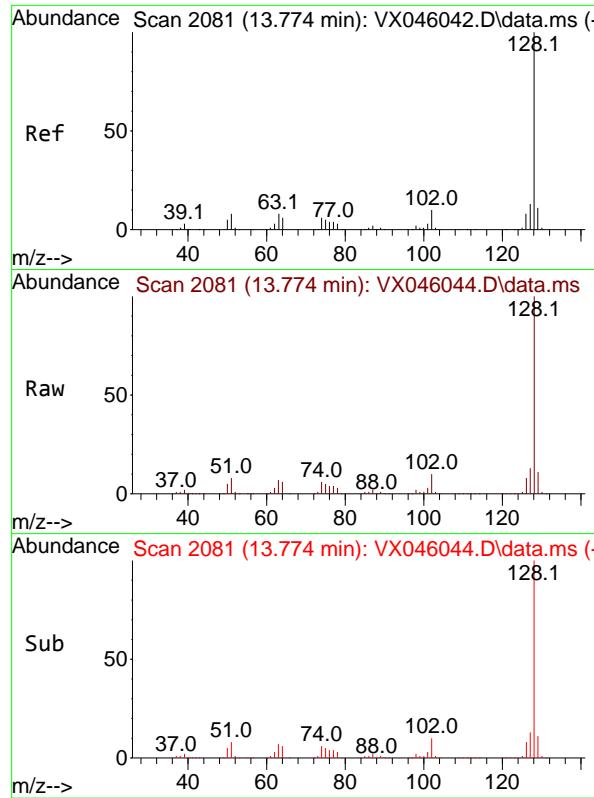


#95  
Naphthalene  
Concen: 130.929 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC150


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

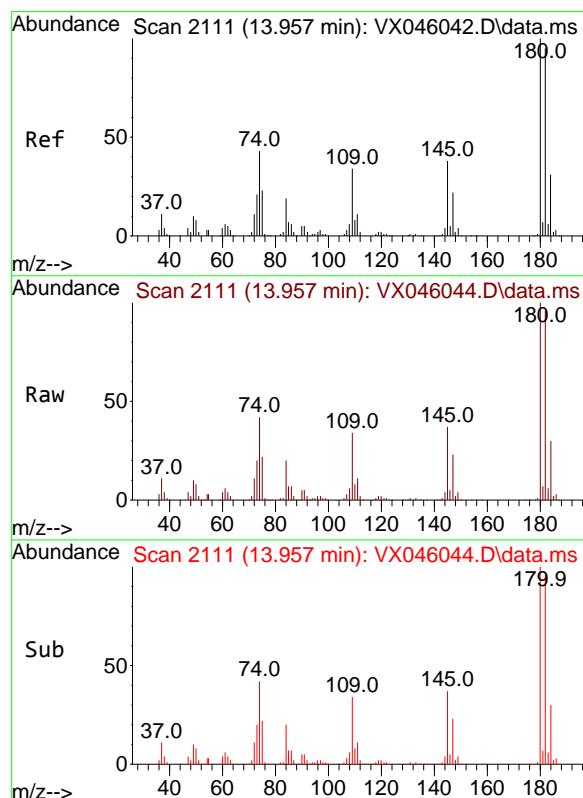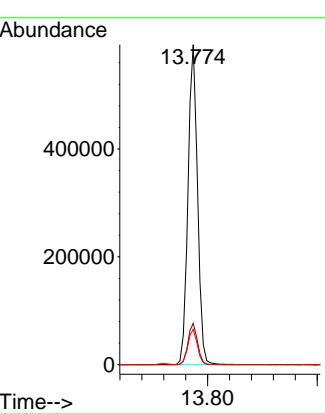

#96  
1,2,3-Trichlorobenzene  
Concen: 126.331 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046044.D  
Acq: 05 May 2025 12:45

Tgt Ion:180 Resp: 200379  
Ion Ratio Lower Upper  
180 100  
182 96.5 47.8 143.3  
145 36.7 18.1 54.3

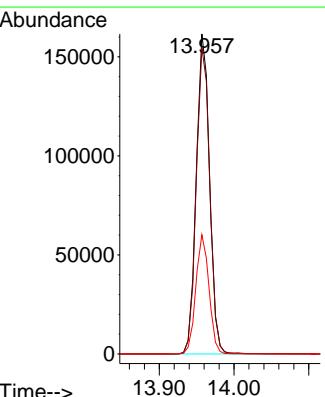

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046046.D  
 Acq On : 05 May 2025 16:04  
 Operator : JC/MD  
 Sample : VSTDICC005  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC005

Quant Time: May 06 06:12:34 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.538	168	96964	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	168484	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	147167	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	67939	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.946	65	9067	3.143	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	6.280%#	
35) Dibromofluoromethane	5.373	113	5969	3.161	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	6.320%#	
50) Toluene-d8	8.647	98	20566	3.232	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	6.460%#	
62) 4-Bromofluorobenzene	11.079	95	7822	3.378	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	6.760%#	
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	6195	2.894	ug/l	95
3) Chloromethane	1.307	50	6587	3.125	ug/l	99
4) Vinyl Chloride	1.374	62	5999	3.249	ug/l	96
5) Bromomethane	1.593	94	2962	3.164	ug/l	88
6) Chloroethane	1.666	64	3567	3.750	ug/l	94
7) Trichlorofluoromethane	1.874	101	9599	3.413	ug/l	88
8) Diethyl Ether	2.130	74	3020	3.266	ug/l	95
9) 1,1,2-Trichlorotrifluo...	2.325	101	5911	3.517	ug/l	99
10) Methyl Iodide	2.441	142	5900	2.990	ug/l	99
11) Tert butyl alcohol	2.965	59	5539	16.111	ug/l	98
12) 1,1-Dichloroethene	2.306	96	5496	3.359	ug/l	97
13) Acrolein	2.233	56	5673	14.206	ug/l	95
14) Allyl chloride	2.654	41	10262	3.319	ug/l	98
15) Acrylonitrile	3.062	53	16746	16.282	ug/l	97
16) Acetone	2.380	43	19773	20.036	ug/l	98
17) Carbon Disulfide	2.501	76	11068	2.919	ug/l	96
18) Methyl Acetate	2.703	43	7909	3.357	ug/l	100
19) Methyl tert-butyl Ether	3.111	73	18497	3.241	ug/l	97
20) Methylene Chloride	2.782	84	6680	3.341	ug/l	97
21) trans-1,2-Dichloroethene	3.081	96	5402	3.234	ug/l	100
22) Diisopropyl ether	3.751	45	18657	3.230	ug/l #	65
23) Vinyl Acetate	3.715	43	82328	16.127	ug/l	99
24) 1,1-Dichloroethane	3.605	63	11193	3.297	ug/l	99
25) 2-Butanone	4.562	43	26125	18.340	ug/l	98
26) 2,2-Dichloropropane	4.465	77	8245	3.205	ug/l	96
27) cis-1,2-Dichloroethene	4.483	96	6222	3.089	ug/l	95
28) Bromochloromethane	4.891	49	5360	2.969	ug/l #	100
29) Tetrahydrofuran	5.001	42	15431	16.680	ug/l	98
30) Chloroform	5.080	83	11624	3.294	ug/l	89
31) Cyclohexane	5.458	56	10269	3.588	ug/l	96
32) 1,1,1-Trichloroethane	5.367	97	9827	3.229	ug/l	97
36) 1,1-Dichloropropene	5.678	75	7787	3.551	ug/l	98
37) Ethyl Acetate	4.721	43	9806m	3.565	ug/l	
38) Carbon Tetrachloride	5.659	117	8505	3.376	ug/l	97
39) Methylcyclohexane	7.373	83	9882	3.597	ug/l	93
40) Benzene	6.031	78	22528	3.315	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046046.D  
 Acq On : 05 May 2025 16:04  
 Operator : JC/MD  
 Sample : VSTDICC005  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC005

Quant Time: May 06 06:12:34 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	4851	3.174	ug/1	# 65
42) 1,2-Dichloroethane	6.080	62	10011	3.563	ug/1	100
43) Isopropyl Acetate	6.348	43	13914	3.309	ug/1	96
44) Trichloroethene	7.123	130	5313	3.307	ug/1	94
45) 1,2-Dichloropropane	7.427	63	5451	3.228	ug/1	# 89
46) Dibromomethane	7.580	93	4417	3.318	ug/1	98
47) Bromodichloromethane	7.818	83	8394	3.254	ug/1	98
48) Methyl methacrylate	7.696	41	7171	3.321	ug/1	97
49) 1,4-Dioxane	7.659	88	2907	67.721	ug/1	96
51) 4-Methyl-2-Pentanone	8.567	43	46794	16.967	ug/1	98
52) Toluene	8.714	92	14126	3.505	ug/1	97
53) t-1,3-Dichloropropene	8.976	75	6834	3.155	ug/1	100
54) cis-1,3-Dichloropropene	8.366	75	7908	3.129	ug/1	91
55) 1,1,2-Trichloroethane	9.153	97	5685	3.490	ug/1	98
56) Ethyl methacrylate	9.116	69	8555	3.390	ug/1	98
57) 1,3-Dichloropropane	9.305	76	10127	3.508	ug/1	94
58) 2-Chloroethyl Vinyl ether	8.238	63	20809	18.346	ug/1	99
59) 2-Hexanone	9.427	43	34853	16.651	ug/1	97
60) Dibromochloromethane	9.518	129	5500	3.102	ug/1	98
61) 1,2-Dibromoethane	9.604	107	5614	3.356	ug/1	99
64) Tetrachloroethene	9.269	164	4752	3.162	ug/1	96
65) Chlorobenzene	10.079	112	15391	3.399	ug/1	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	5024	3.326	ug/1	99
67) Ethyl Benzene	10.195	91	26732	3.463	ug/1	99
68) m/p-Xylenes	10.299	106	19957	7.156	ug/1	98
69) o-Xylene	10.640	106	9398	3.343	ug/1	95
70) Styrene	10.652	104	14900	3.312	ug/1	99
71) Bromoform	10.799	173	3470	3.059	ug/1	# 99
73) Isopropylbenzene	10.957	105	24201	3.266	ug/1	98
74) N-amyl acetate	10.841	43	11224	3.038	ug/1	96
75) 1,1,2,2-Tetrachloroethane	11.207	83	9170	3.479	ug/1	97
76) 1,2,3-Trichloropropane	11.238	75	7928m	2.799	ug/1	
77) Bromobenzene	11.195	156	5857	3.417	ug/1	96
78) n-propylbenzene	11.299	91	28436	3.424	ug/1	100
79) 2-Chlorotoluene	11.360	91	18672	3.336	ug/1	97
80) 1,3,5-Trimethylbenzene	11.451	105	20742	3.372	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	1828	2.686	ug/1	99
82) 4-Chlorotoluene	11.451	91	19966	3.245	ug/1	98
83) tert-Butylbenzene	11.713	119	21049	3.484	ug/1	98
84) 1,2,4-Trimethylbenzene	11.750	105	20613	3.355	ug/1	97
85) sec-Butylbenzene	11.890	105	25590	3.412	ug/1	99
86) p-Isopropyltoluene	12.006	119	20955	3.460	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	10585	3.315	ug/1	97
88) 1,4-Dichlorobenzene	12.036	146	10908	3.486	ug/1	90
89) n-Butylbenzene	12.329	91	18004	3.419	ug/1	94
90) Hexachloroethane	12.536	117	3553	3.153	ug/1	94
91) 1,2-Dichlorobenzene	12.335	146	10712	3.444	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.945	75	1687	2.812	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	5720	3.359	ug/1	96
94) Hexachlorobutadiene	13.719	225	2816	3.535	ug/1	96
95) Naphthalene	13.774	128	19902	3.209	ug/1	99
96) 1,2,3-Trichlorobenzene	13.957	180	5745	3.217	ug/1	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046046.D  
 Acq On : 05 May 2025 16:04  
 Operator : JC/MD  
 Sample : VSTDICC005  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 10 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC005

Quant Time: May 06 06:12:34 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046046.D  
Acq On : 05 May 2025 16:04  
Operator : JC/MD  
Sample : VSTDIICC005  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1




Quant Time: May 06 06:12:34 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 06:04:56 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC005

## Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

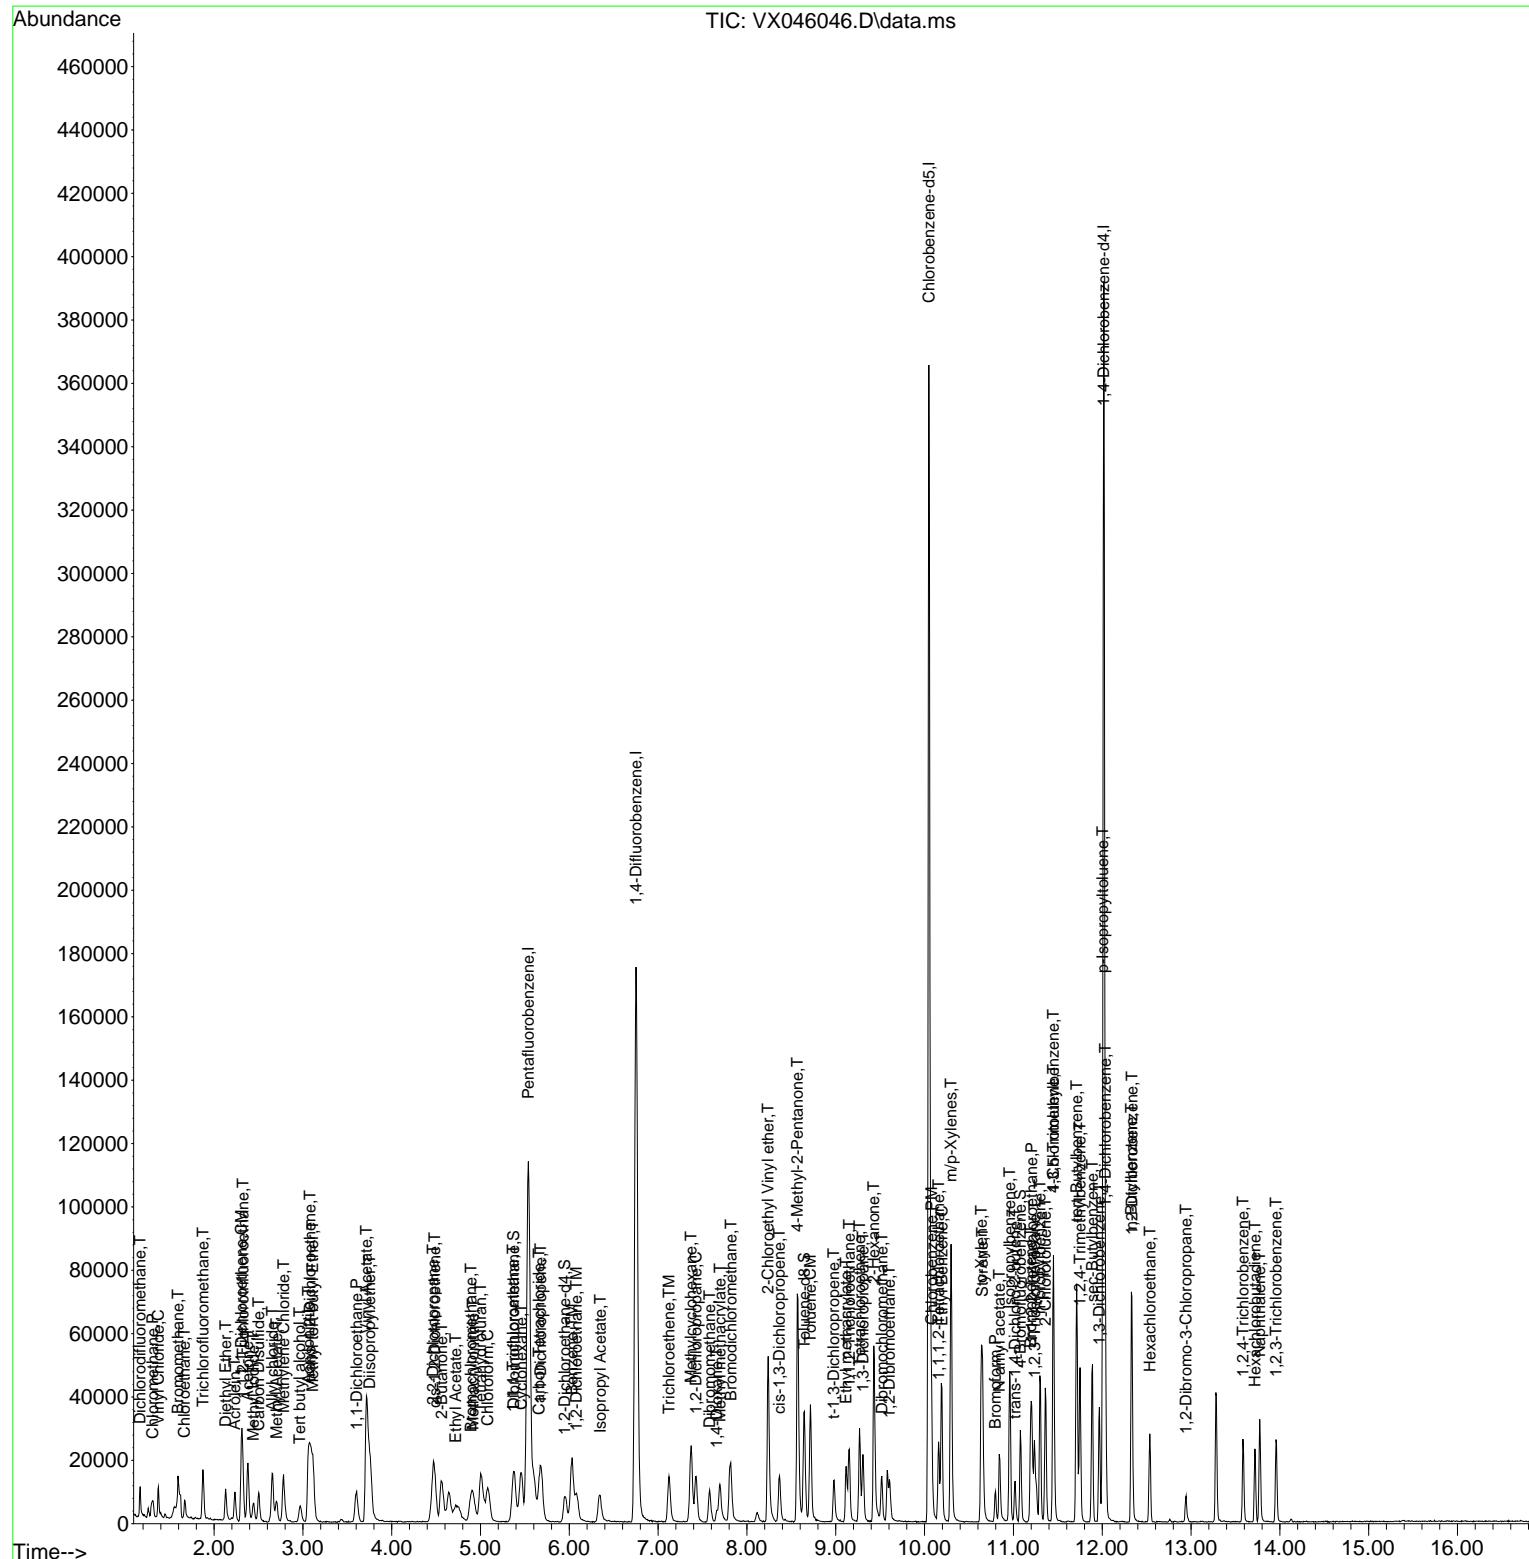

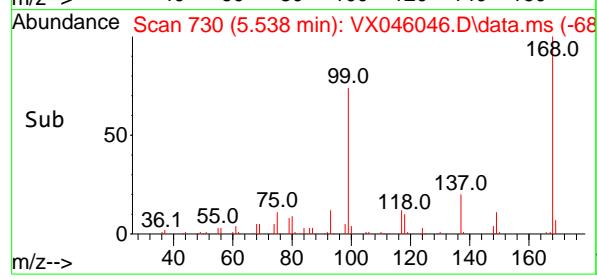

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.538 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

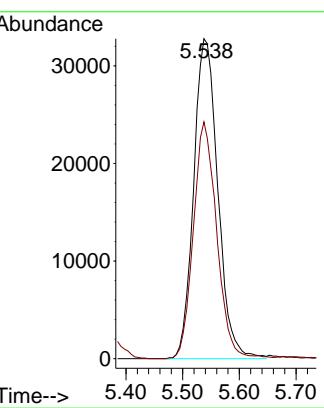

#2

Dichlorodifluoromethane

Concen: 2.894 ug/l




RT: 1.166 min Scan# 13


Delta R.T. -0.000 min

Lab File: VX046046.D



Acq: 05 May 2025 16:04

Tgt	Ion	Resp:	6195
Ion	Ratio	Lower	Upper
85	100		
87	28.7	15.7	47.1

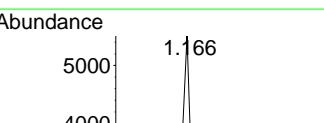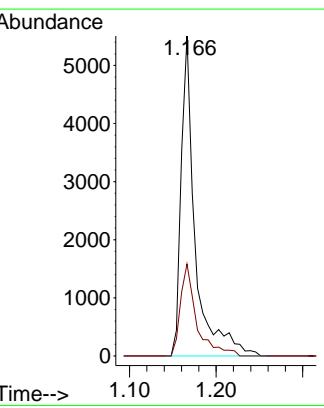




Ref Scan 36 (1.307 min): VX046046.D\data.ms

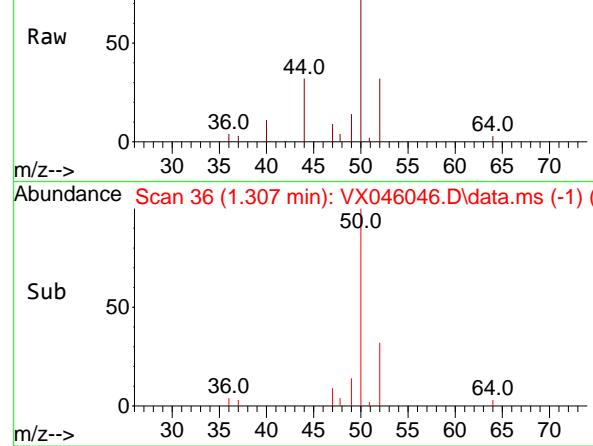

Ref Scan 47 (1.374 min): VX046046.D\data.ms

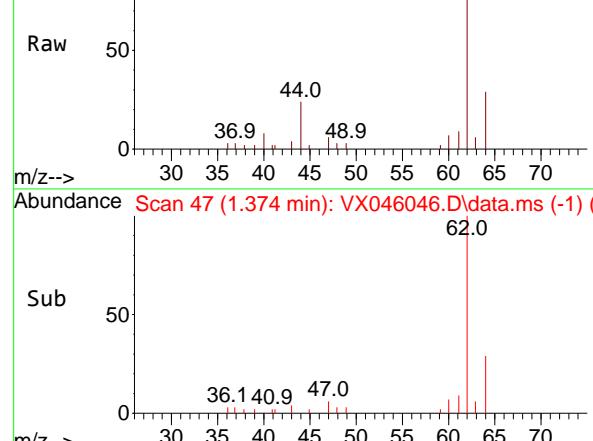

#3

Chloromethane

Concen: 3.125 ug/l

RT: 1.307 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

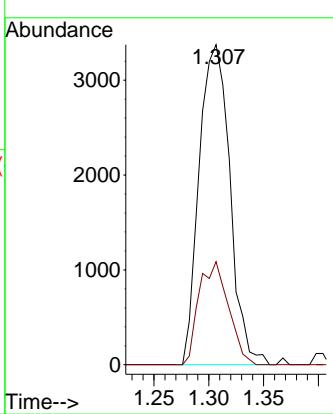

#4

Vinyl Chloride

Concen: 3.249 ug/l


RT: 1.374 min Scan# 47




Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt Ion: 62 Resp: 5999  
 Ion Ratio Lower Upper  
 62 100  
 64 29.1 25.2 37.8





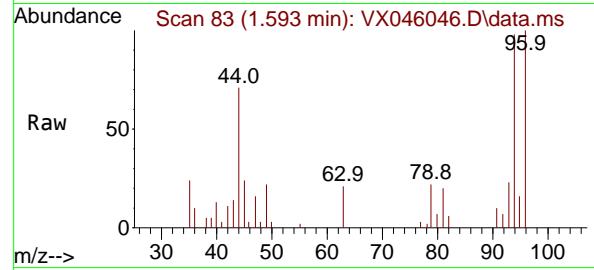
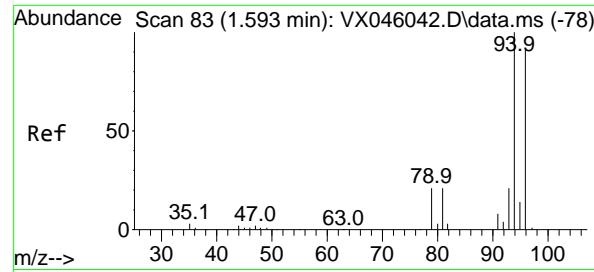


#5  
 Bromomethane  
 Concen: 3.164 ug/l  
 RT: 1.593 min Scan# 8  
 Delta R.T. -0.000 min  
 Lab File: VX046046.D  
 Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

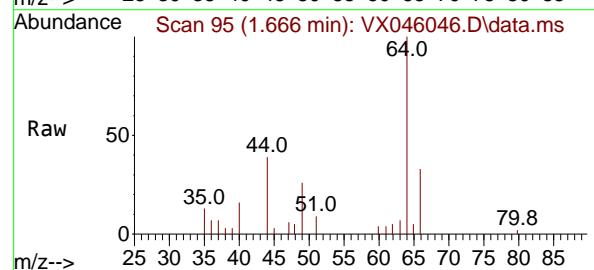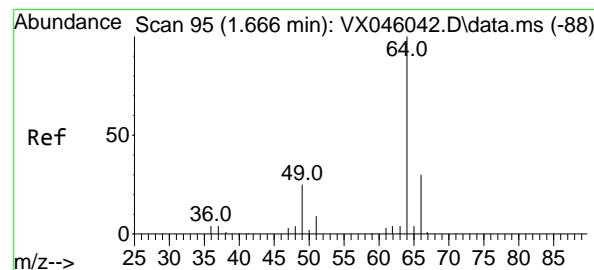

#6  
 Chloroethane  
 Concen: 3.750 ug/l  
 RT: 1.666 min Scan# 95  
 Delta R.T. -0.000 min  
 Lab File: VX046046.D  
 Acq: 05 May 2025 16:04

Tgt Ion: 64 Resp: 3567  
 Ion Ratio Lower Upper  
 64 100  
 66 33.7 24.3 36.5




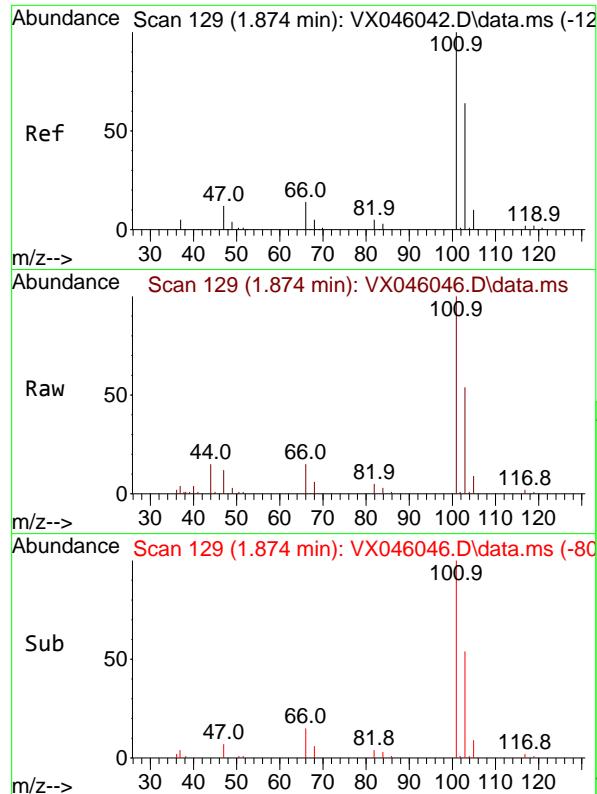


#7  
Trichlorofluoromethane  
Concen: 3.413 ug/l  
RT: 1.874 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

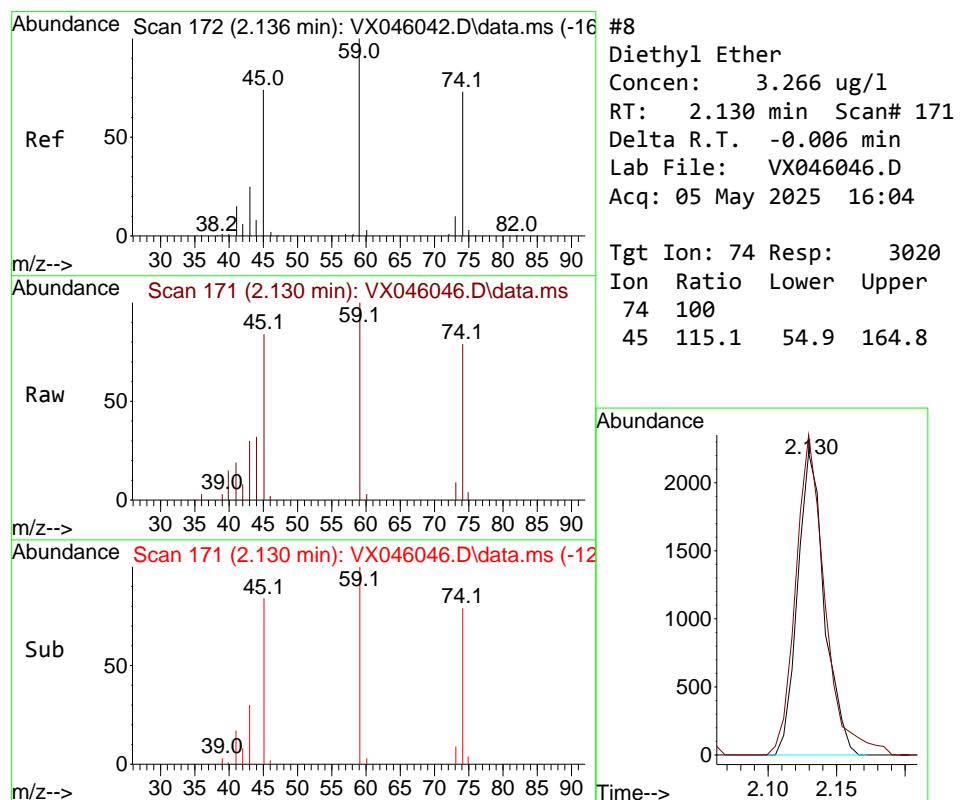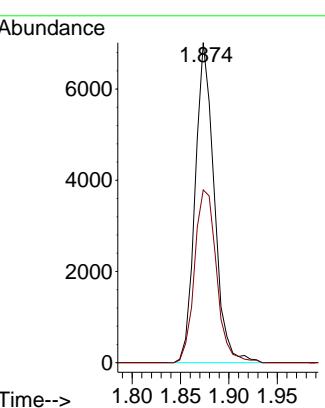

#8  
Diethyl Ether  
Concen: 3.266 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04


Tgt Ion: 74 Resp: 3020  
Ion Ratio Lower Upper  
74 100  
45 115.1 54.9 164.8

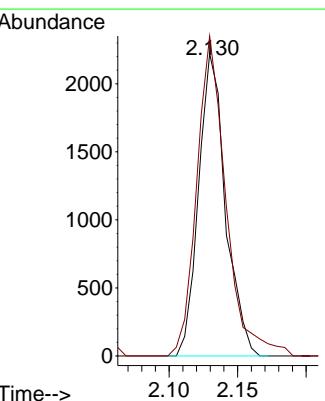



#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 3.517 ug/l  
RT: 2.325 min Scan# 2  
Delta R.T. 0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

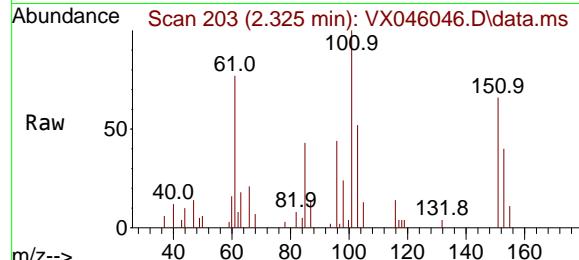


Tgt Ion:101 Resp: 591:  
Ion Ratio Lower Upper  
101 100  
85 46.3 38.6 58.0  
151 68.8 55.2 82.8

Manual Integrations  
APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025









#10  
Methyl Iodide  
Concen: 2.990 ug/l  
RT: 2.441 min Scan# 222  
Delta R.T. -0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

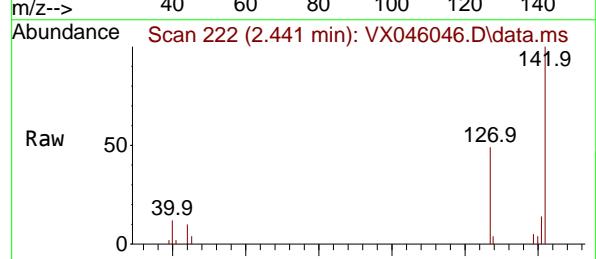

Tgt Ion:142 Resp: 5900  
Ion Ratio Lower Upper  
142 100  
127 52.8 41.7 62.5  
141 14.3 11.5 17.3

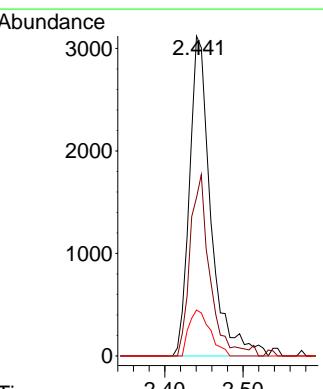

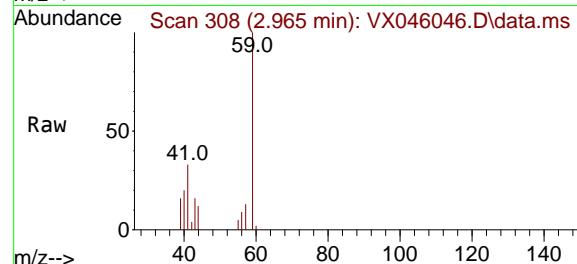

#11

Tert butyl alcohol

Concen: 16.111 ug/l

RT: 2.965 min Scan# 3

Delta R.T. -0.012 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

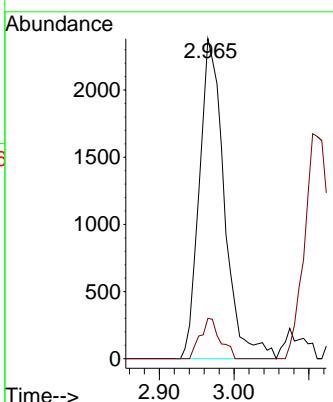

#12

1,1-Dichloroethene

Concen: 3.359 ug/l

RT: 2.306 min Scan# 200

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 96 Resp: 5496


Ion Ratio Lower Upper

96 100

61 178.7 146.2 219.2

98 59.5 51.0 76.6

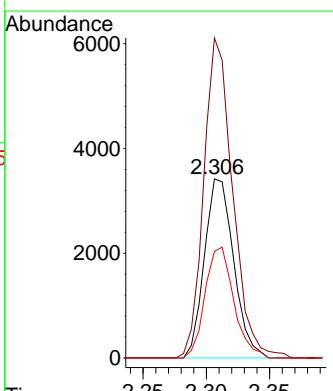


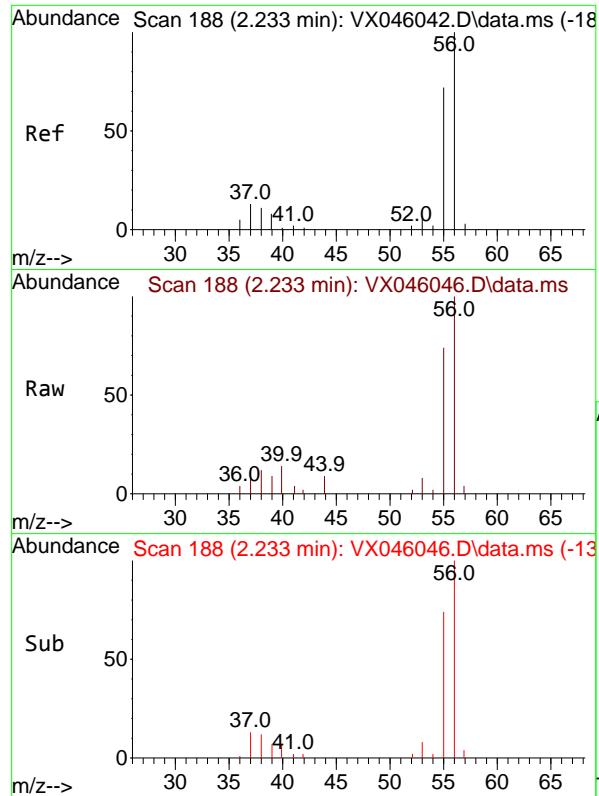


#13  
Acrolein  
Concen: 14.206 ug/l  
RT: 2.233 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

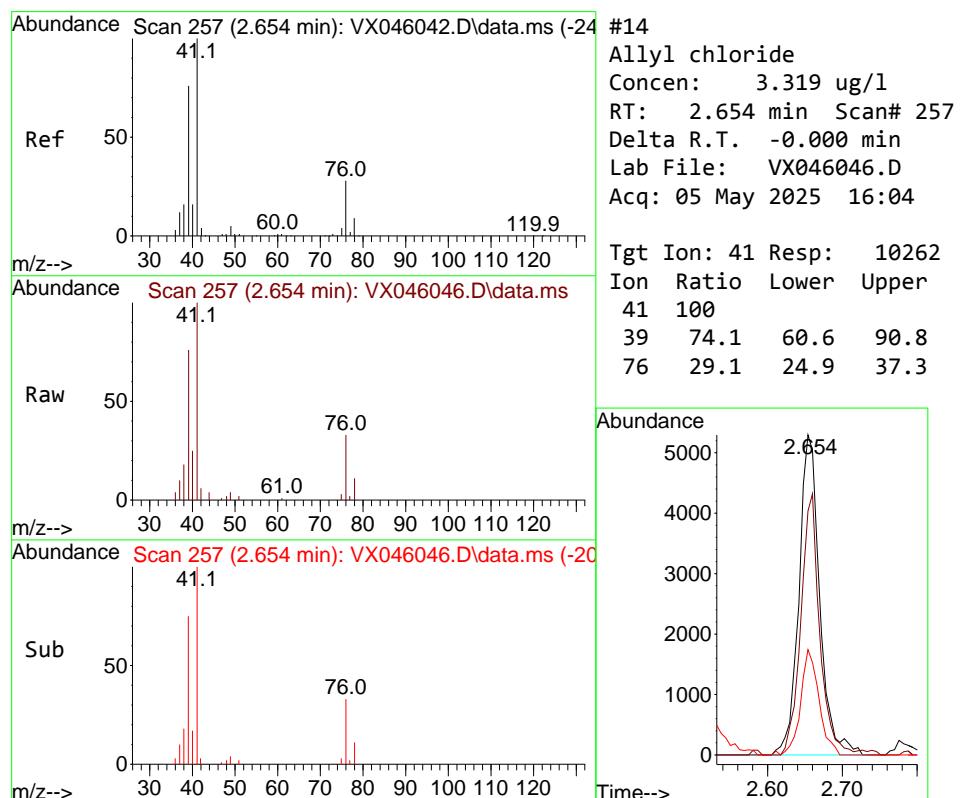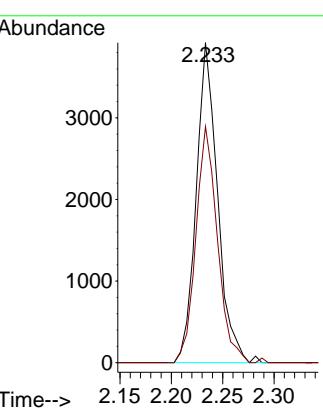

#14  
Allyl chloride  
Concen: 3.319 ug/l  
RT: 2.654 min Scan# 257  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion: 41 Resp: 10262  
Ion Ratio Lower Upper  
41 100  
39 74.1 60.6 90.8  
76 29.1 24.9 37.3

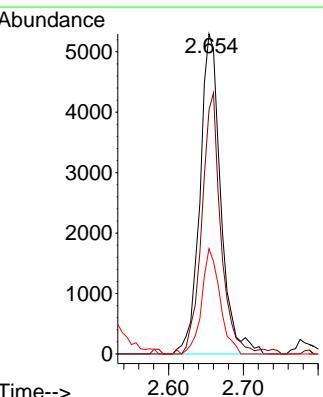

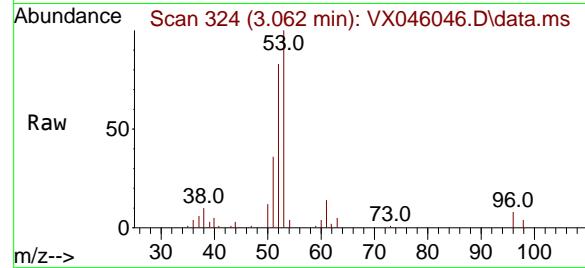

#15

**Acrylonitrile**

Concen: 16.282 ug/l

RT: 3.062 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC005

Tgt Ion: 53 Resp: 16740

Ion Ratio Lower Upper

53 100




52 84.3 65.3 97.9

51 38.5 29.8 44.8

**Manual Integrations****APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

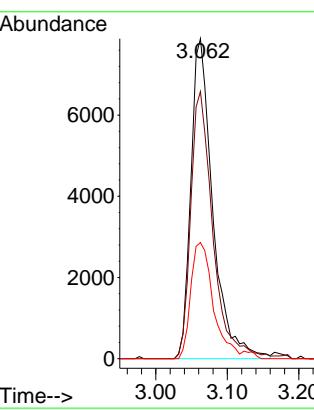



#16  
Acetone  
Concen: 20.036 ug/l  
RT: 2.380 min Scan# 212  
Delta R.T. -0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04


Tgt Ion: 43 Resp: 19773

Ion Ratio Lower Upper


43 100

58 27.7 21.2 31.8

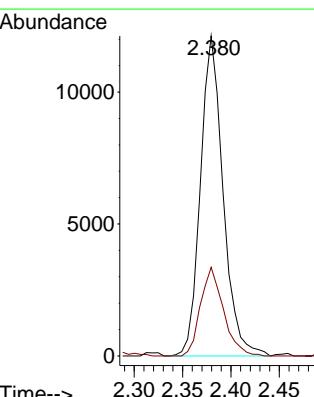



Abundance Scan 232 (2.501 min): VX046046.D\data.ms

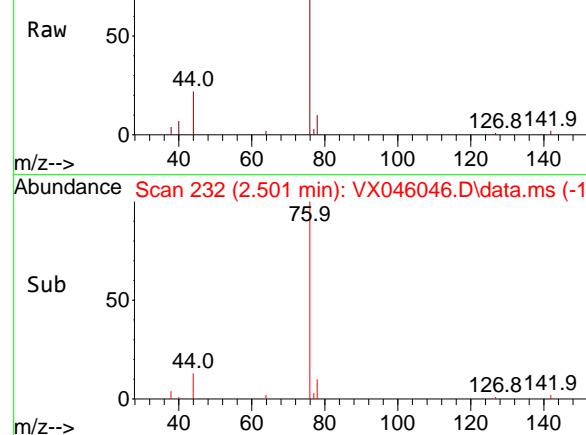

#17

Carbon Disulfide

Concen: 2.919 ug/l

RT: 2.501 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC005


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



Abundance Scan 265 (2.703 min): VX046046.D\data.ms

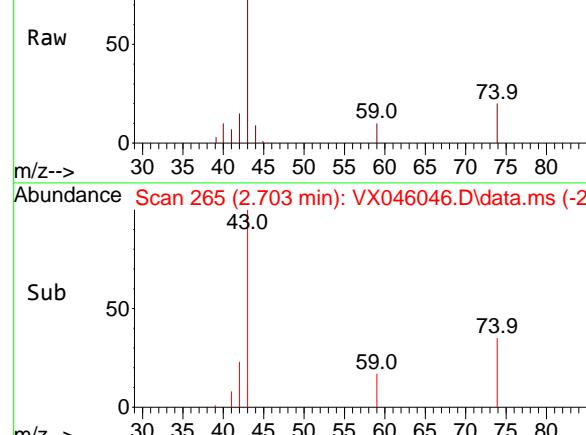

#18

Methyl Acetate

Concen: 3.357 ug/l


RT: 2.703 min Scan# 265




Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt Ion: 43 Resp: 7909  
 Ion Ratio Lower Upper  
 43 100  
 74 20.9 16.7 25.1









#19

Methyl tert-butyl Ether  
Concen: 3.241 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

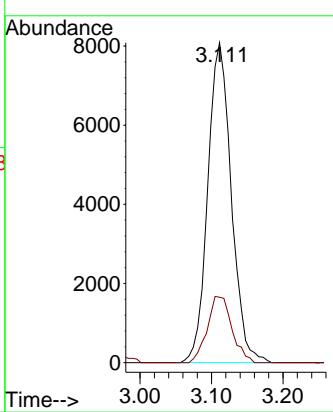


#20

Methylene Chloride  
Concen: 3.341 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion: 84 Resp: 6680  
Ion Ratio Lower Upper  
84 100  
49 137.0 113.9 170.9  
51 43.8 33.5 50.3  
86 67.6 53.8 80.8

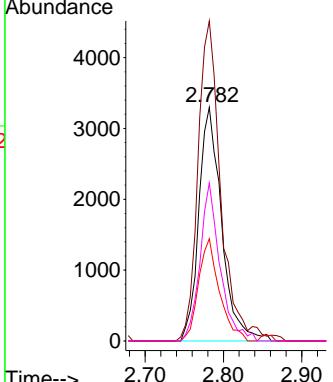


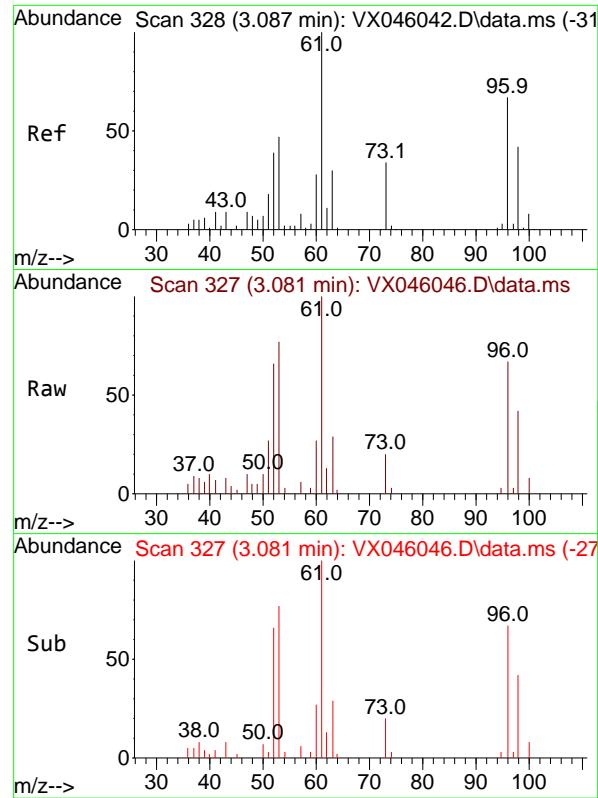


#21  
trans-1,2-Dichloroethene  
Concen: 3.234 ug/l  
RT: 3.081 min Scan# 3  
Delta R.T. -0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carbone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

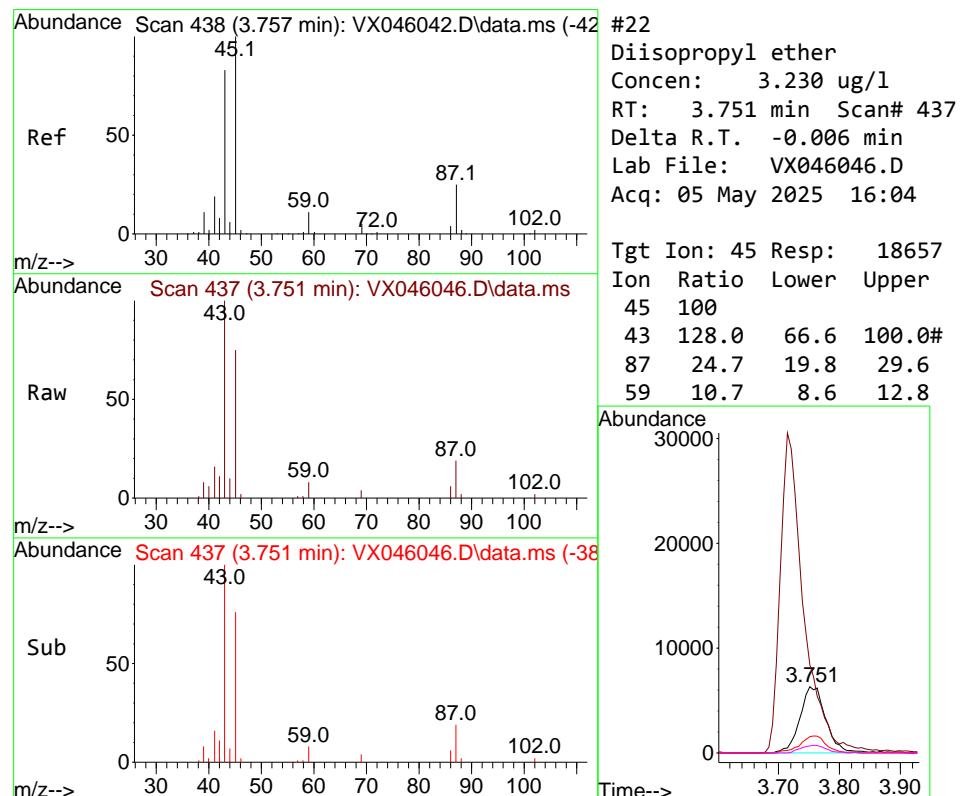



#22  
Diisopropyl ether  
Concen: 3.230 ug/l  
RT: 3.751 min Scan# 437  
Delta R.T. -0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion: 45 Resp: 18657  
Ion Ratio Lower Upper  
45 100  
43 128.0 66.6 100.0#  
87 24.7 19.8 29.6  
59 10.7 8.6 12.8

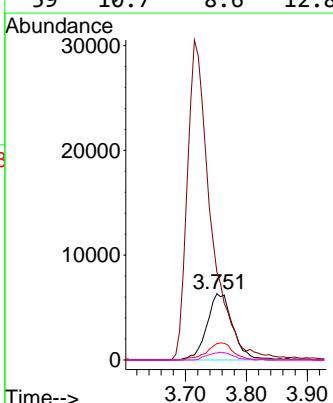




Ref Abundance Scan 431 (3.715 min): VX046046.D\data.ms

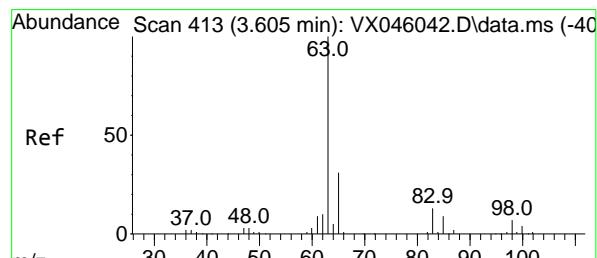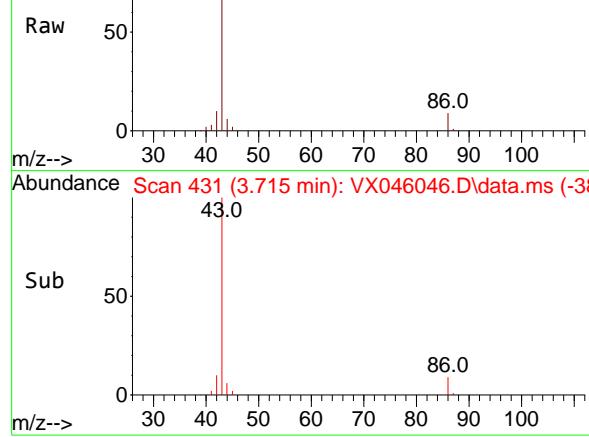

Ref Abundance Scan 413 (3.605 min): VX046046.D\data.ms

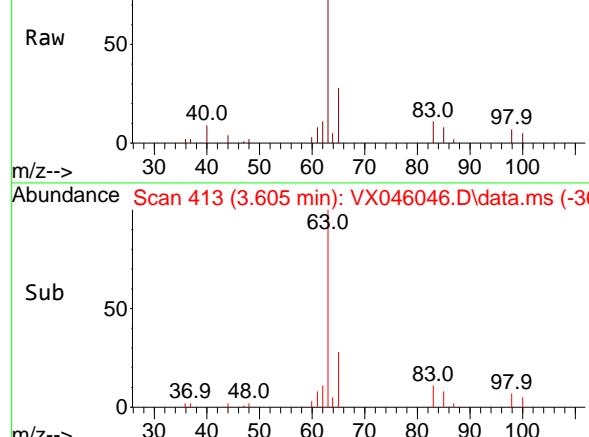

Sub Abundance Scan 413 (3.605 min): VX046046.D\data.ms (-36)

#23

**Vinyl Acetate**

Concen: 16.127 ug/l

RT: 3.715 min Scan# 413

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

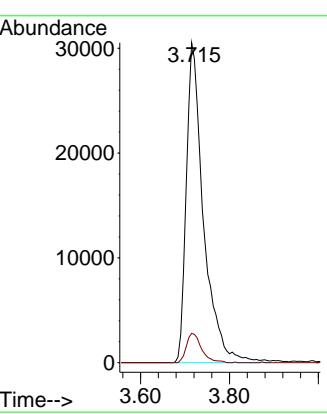

#24

**1,1-Dichloroethane**

Concen: 3.297 ug/l

RT: 3.605 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 63 Resp: 11193







Ion Ratio Lower Upper

63 100

98 6.9 3.6 10.8

100 4.7 2.1 6.3

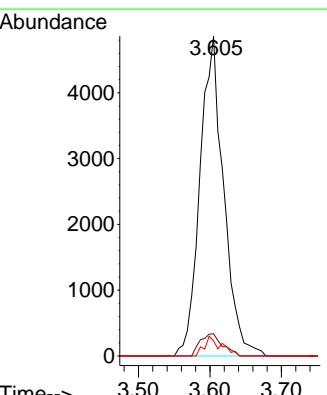

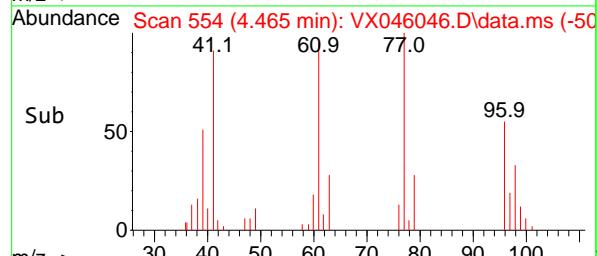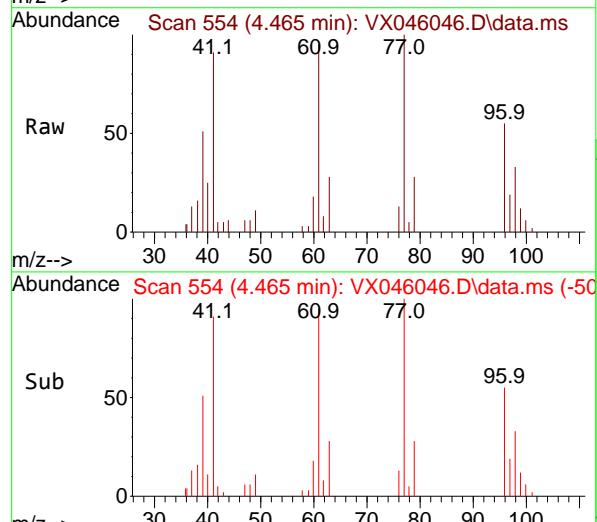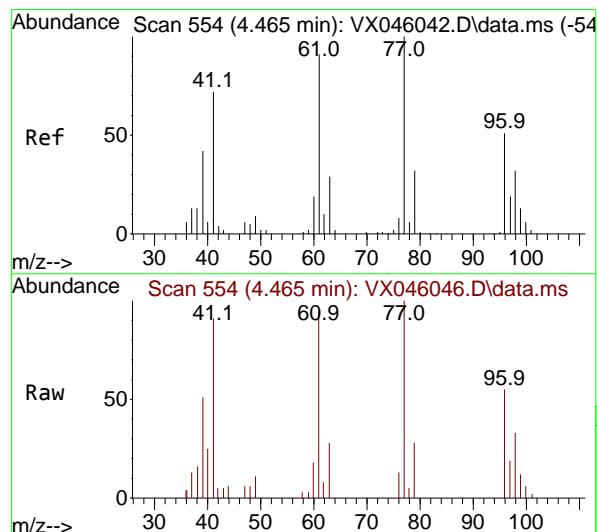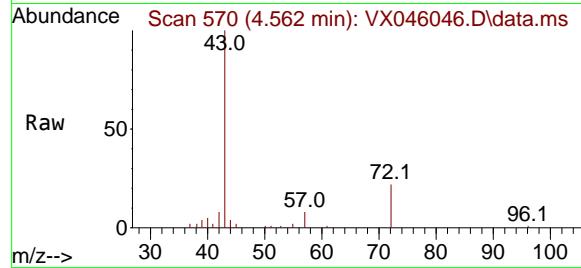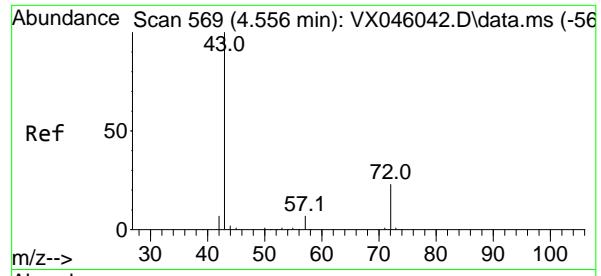

#25

2-Butanone

Concen: 18.340 ug/l

RT: 4.562 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

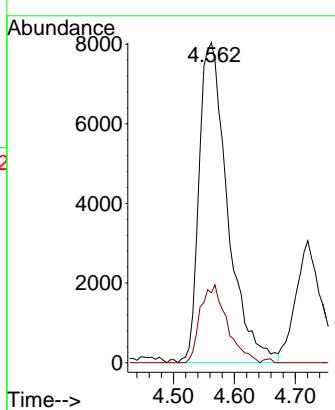

#26

2,2-Dichloropropane

Concen: 3.205 ug/l

RT: 4.465 min Scan# 554

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04




Tgt Ion: 77 Resp: 8245

Ion Ratio Lower Upper

77 100

97 23.1 10.5 31.5

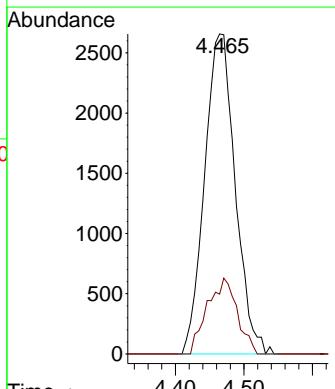

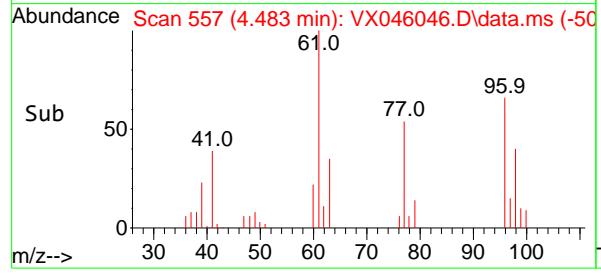
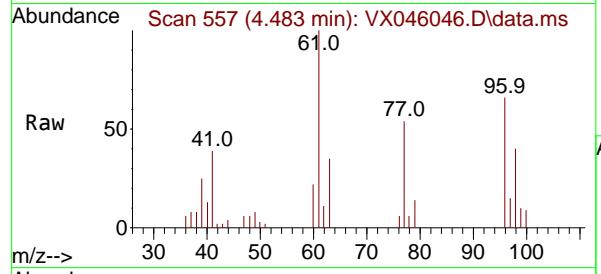
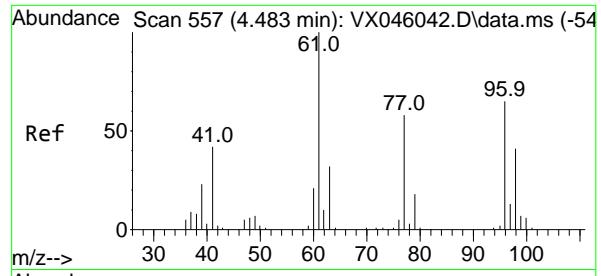


#27  
cis-1,2-Dichloroethene  
Concen: 3.089 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005



### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

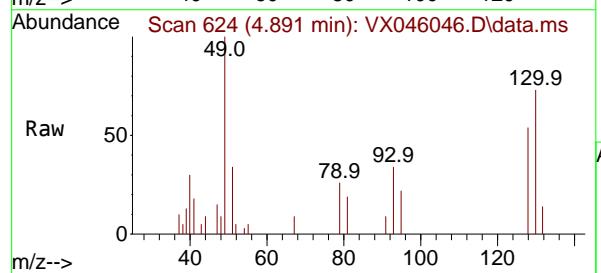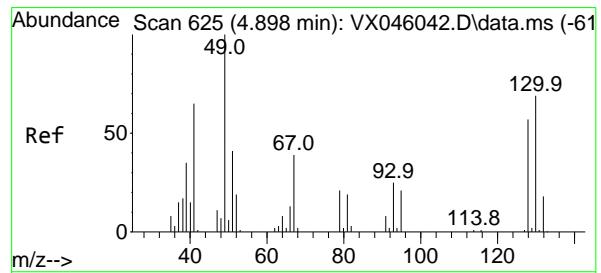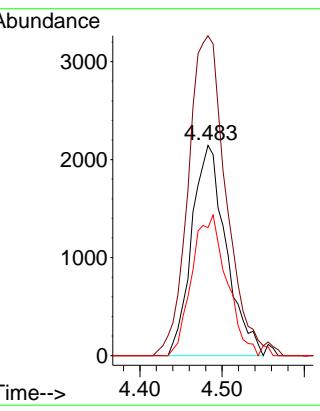

#28  
Bromochloromethane  
Concen: 2.969 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion: 49 Resp: 5360  
Ion Ratio Lower Upper  
49 100  
129 0.0 0.0 4.0  
130 70.5 56.2 84.2

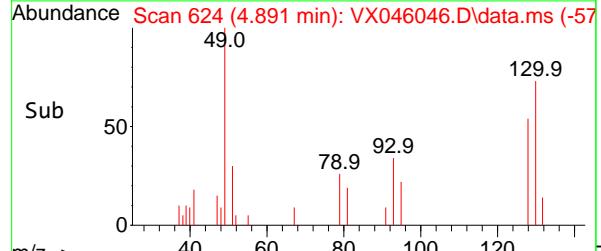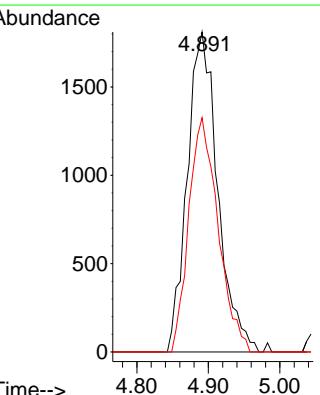

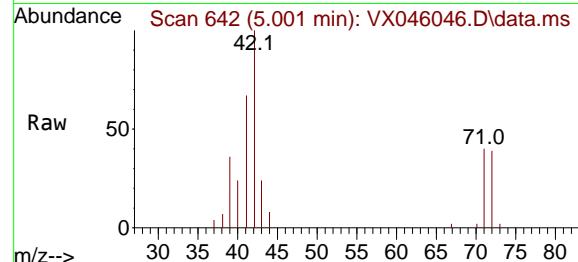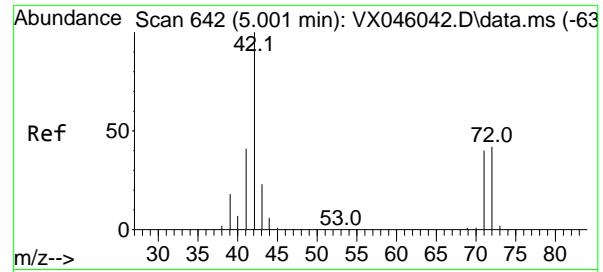

#29

Tetrahydrofuran

Concen: 16.680 ug/l

RT: 5.001 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

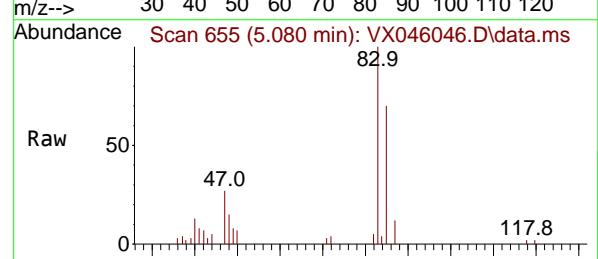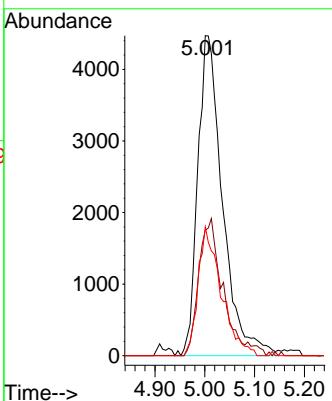

#30

Chloroform

Concen: 3.294 ug/l

RT: 5.080 min Scan# 655



Delta R.T. -0.006 min


Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt Ion: 83 Resp: 11624


Ion	Ratio	Lower	Upper
83	100		
85	69.9	49.3	73.9



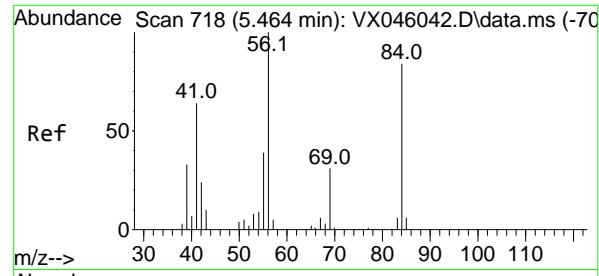

Ref 50

Scan 717 (5.458 min): VX046046.D\data.ms

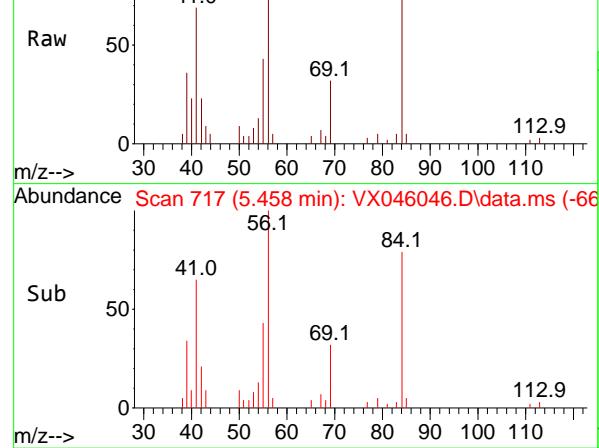

Raw 50

Scan 717 (5.458 min): VX046046.D\data.ms (-66)

Sub 50

Scan 717 (5.458 min): VX046046.D\data.ms (-66)

m/z-->

Time-->

#31

Cyclohexane

Concen: 3.588 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

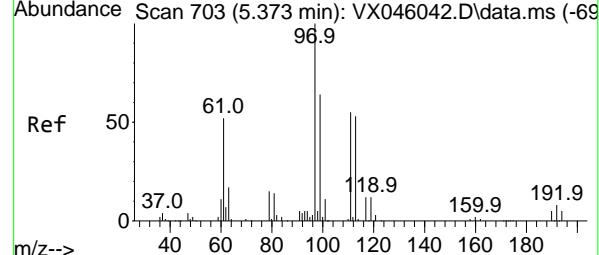

Ref 50

Scan 702 (5.367 min): VX046046.D\data.ms

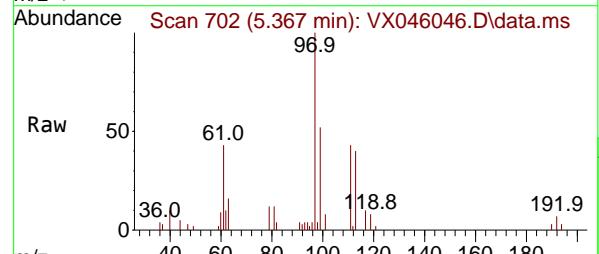

Raw 50

Scan 702 (5.367 min): VX046046.D\data.ms (-65)

Sub 50

Scan 702 (5.367 min): VX046046.D\data.ms (-65)

m/z-->

#32

1,1,1-Trichloroethane

Concen: 3.229 ug/l

RT: 5.367 min Scan# 702

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 97 Resp: 9827

Ion Ratio Lower Upper

97 100

99 62.6 51.8 77.6

61 51.8 40.1 60.1

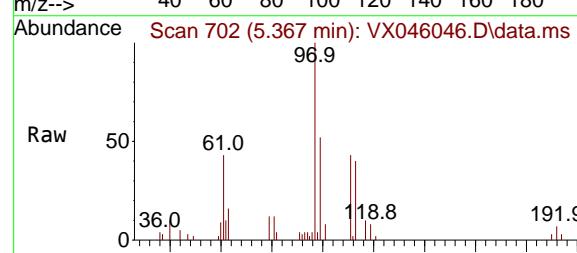

Ref 50

Scan 702 (5.367 min): VX046046.D\data.ms

Raw 50

Scan 702 (5.367 min): VX046046.D\data.ms (-65)

Sub 50

Scan 702 (5.367 min): VX046046.D\data.ms (-65)

m/z-->


Abundance

Time--&gt;

5.30 5.35 5.40 5.45 5.50

5.367

5.373

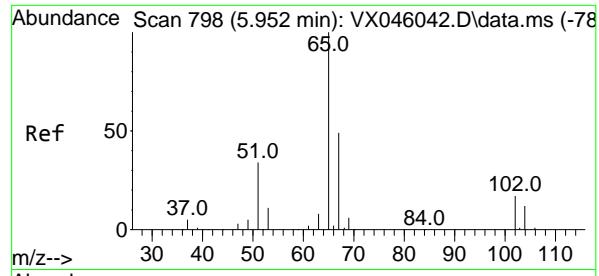

#33

1,2-Dichloroethane-d4




Concen: 3.143 ug/l

RT: 5.946 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

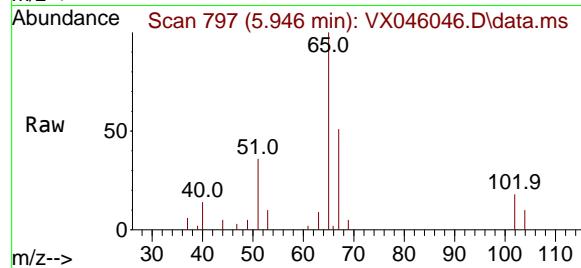

#34

1,4-Difluorobenzene



Concen: 50.000 ug/l

RT: 6.751 min Scan# 929

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04



Tgt Ion:114 Resp: 168484

Ion Ratio Lower Upper







114 100

63 24.5 0.0 49.2

88 17.7 0.0 33.6

Abundance

Time--&gt;

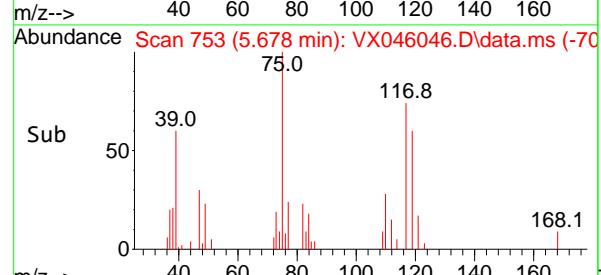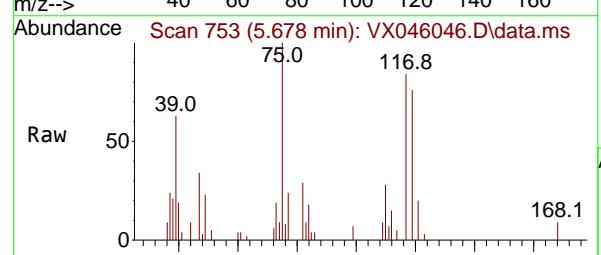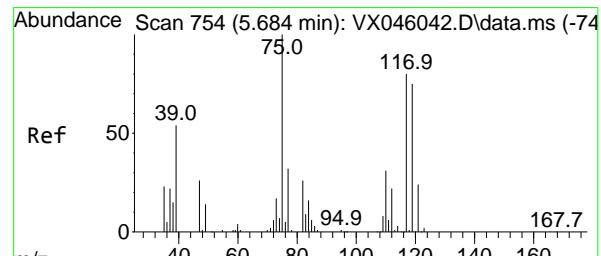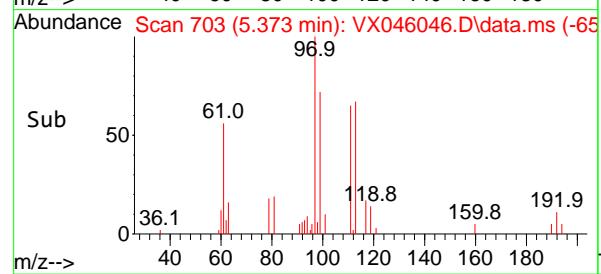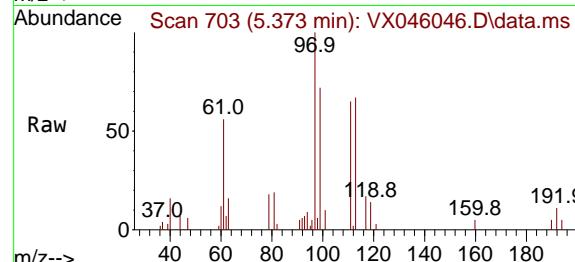

#35

Dibromofluoromethane

Concen: 3.161 ug/l

RT: 5.373 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#36

1,1-Dichloropropene

Concen: 3.551 ug/l

RT: 5.678 min Scan# 753

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 75 Resp: 7787




Ion Ratio Lower Upper

75 100

110 30.6 16.3 48.9

77 30.5 24.3 36.5

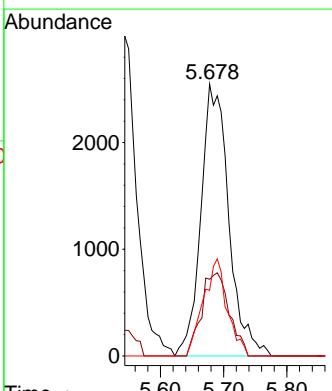

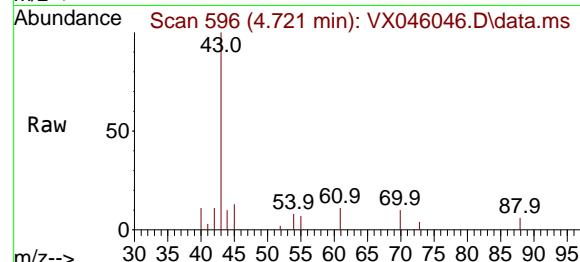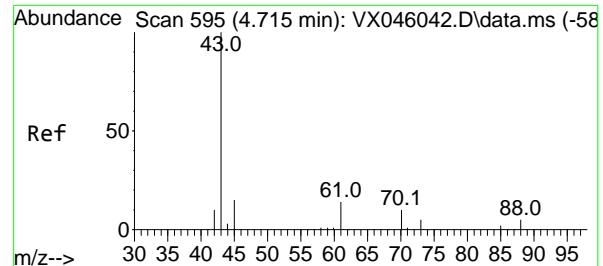

#37

**Ethyl Acetate**

Concen: 3.565 ug/l m

RT: 4.721 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

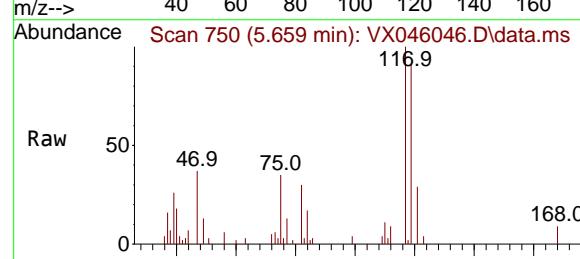

#38

**Carbon Tetrachloride**

Concen: 3.376 ug/l


RT: 5.659 min Scan# 750


Delta R.T. -0.012 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt	Ion:117	Resp:	8505
Ion	Ratio	Lower	Upper
117	100		
119	90.6	75.2	112.8
121	29.5	24.2	36.4

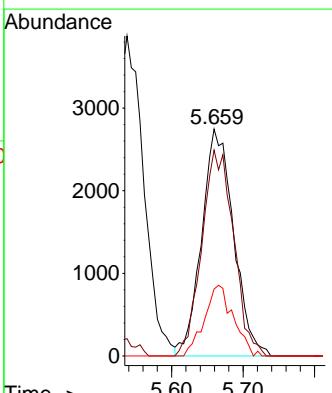

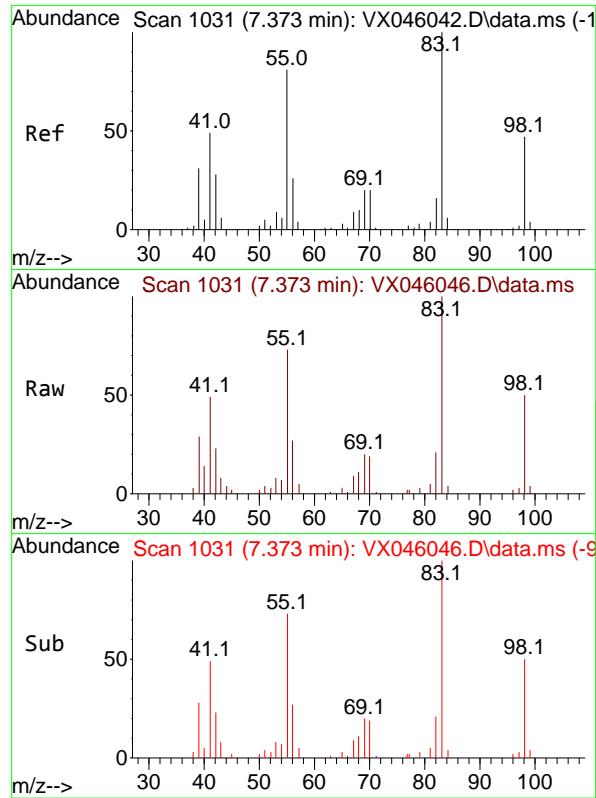

#39

Methylcyclohexane

Concen: 3.597 ug/l

RT: 7.373 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC005

Tgt Ion: 83 Resp: 988.2

Ion Ratio Lower Upper

83 100

55 73.3 64.7 97.1


98 50.3 37.4 56.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

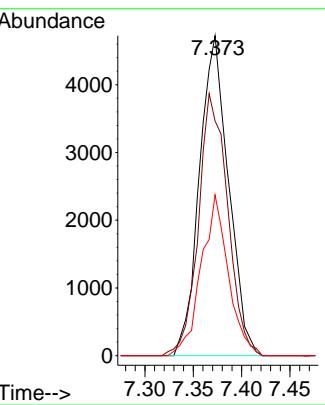

#40

Benzene

Concen: 3.315 ug/l

RT: 6.031 min Scan# 811

Delta R.T. -0.000 min

Lab File: VX046046.D



Acq: 05 May 2025 16:04







Tgt Ion: 78 Resp: 22528

Ion Ratio Lower Upper

78 100

77 23.9 19.0 28.4

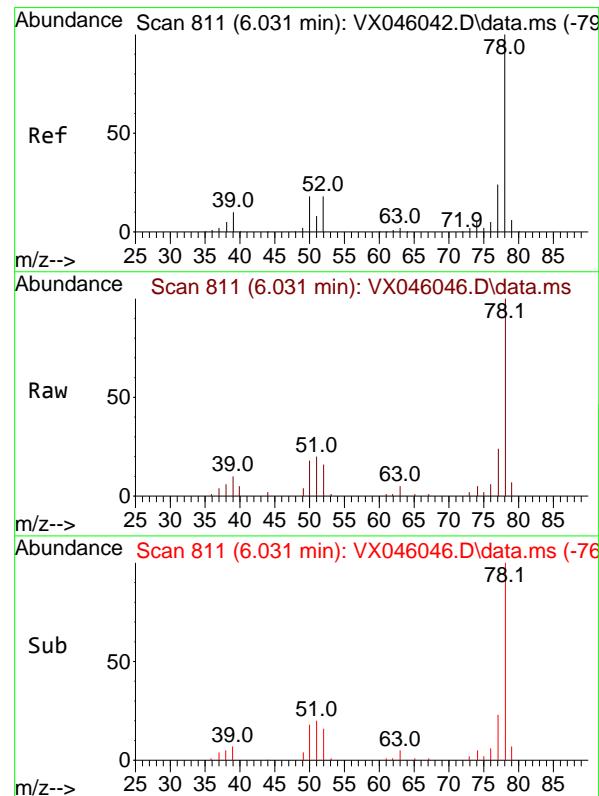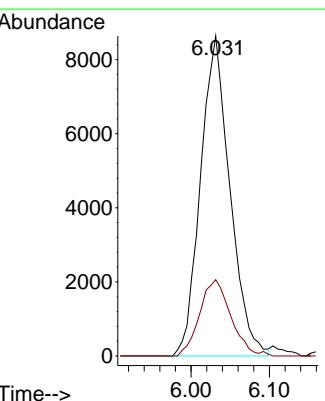



#41

Methacrylonitrile

Concen: 3.174 ug/l

RT: 4.916 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument : MSVOA\_X


ClientSampleId : VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

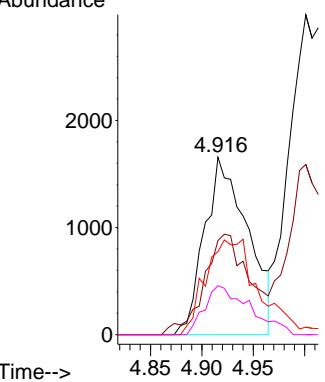

#42

1,2-Dichloroethane

Concen: 3.563 ug/l

RT: 6.080 min Scan# 819

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 62 Resp: 10011


Ion Ratio Lower Upper

62 100


98 7.8 0.0 15.2

Abundance

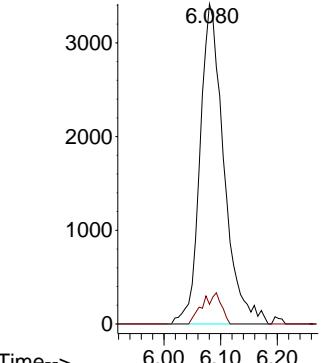




Abundance Scan 863 (6.348 min): VX046046.D\data.ms

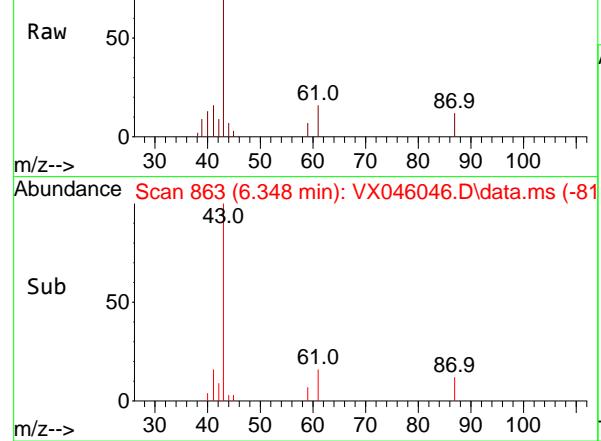

Abundance Scan 863 (6.348 min): VX046046.D\data.ms (-81)

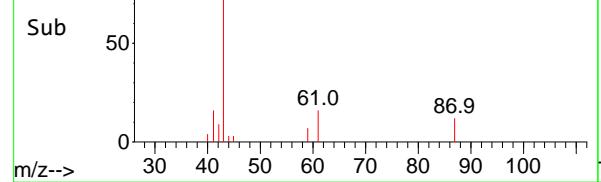

#43

Isopropyl Acetate

Concen: 3.309 ug/l

RT: 6.348 min Scan# 8

Delta R.T. 0.012 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument :

MSVOA\_X

ClientSampleId :

VSTDICC005

Tgt Ion: 43 Resp: 1391

Ion Ratio Lower Upper

43 100

61 16.2 14.3 21.5


87 10.6 9.5 14.3

Manual Integrations


APPROVED

Reviewed By :John Carlone 05/06/2025


Supervised By :Mahesh Dadoda 05/06/2025

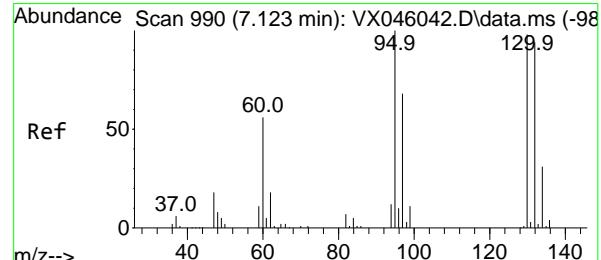

Abundance Scan 990 (7.123 min): VX046046.D\data.ms

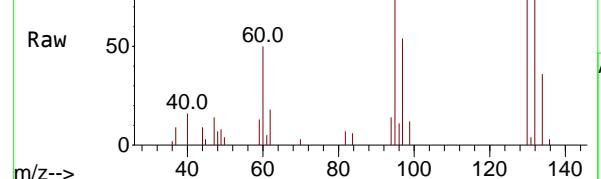

Abundance Scan 990 (7.123 min): VX046046.D\data.ms (-94)

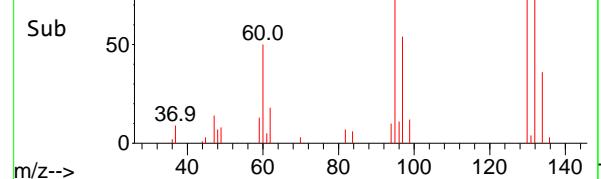

#44

Trichloroethene

Concen: 3.307 ug/l

RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04




Tgt Ion:130 Resp: 5313

Ion Ratio Lower Upper

130 100

95 108.1 0.0 204.2

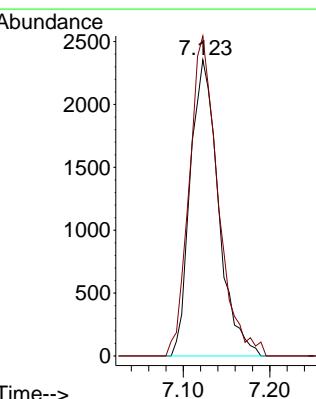

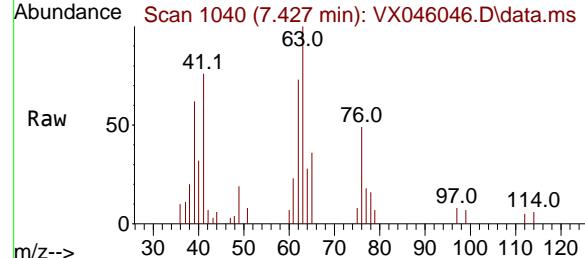

#45

1,2-Dichloropropane

Concen: 3.228 ug/l

RT: 7.427 min Scan# 1040

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

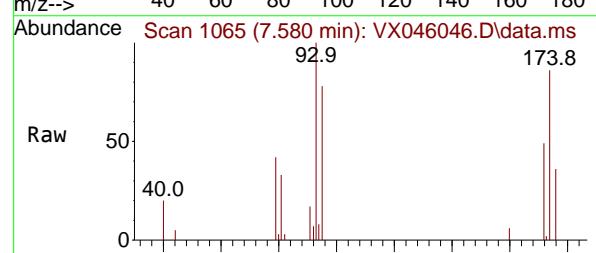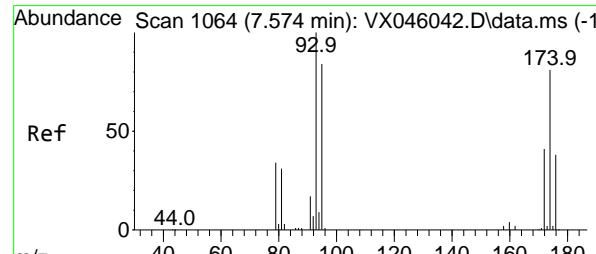

#46

Dibromomethane

Concen: 3.318 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 93 Resp: 4417


Ion Ratio Lower Upper

93 100


95 80.1 65.6 98.4

174 87.6 68.2 102.2

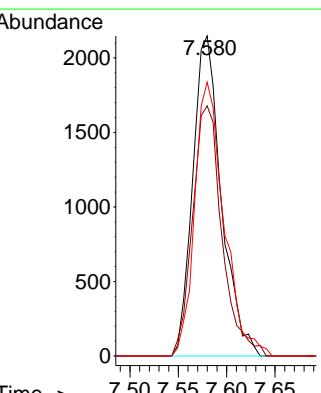


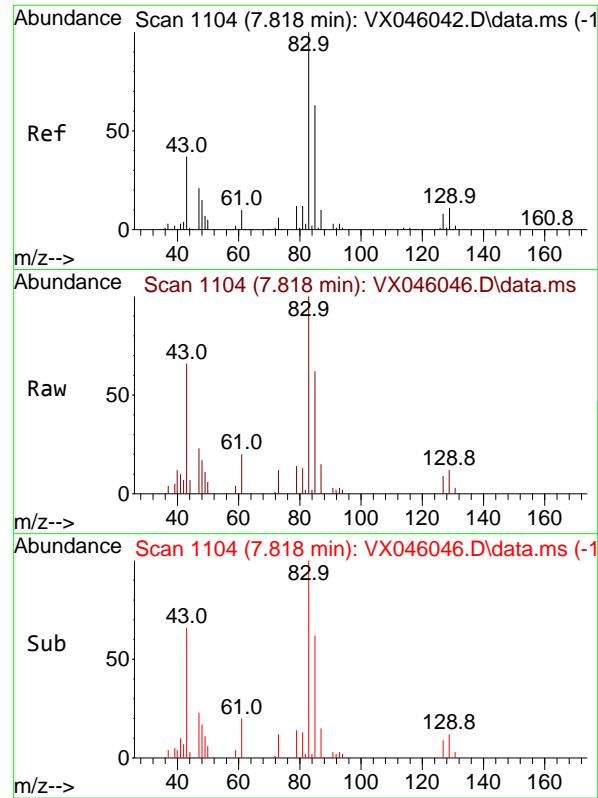


#47

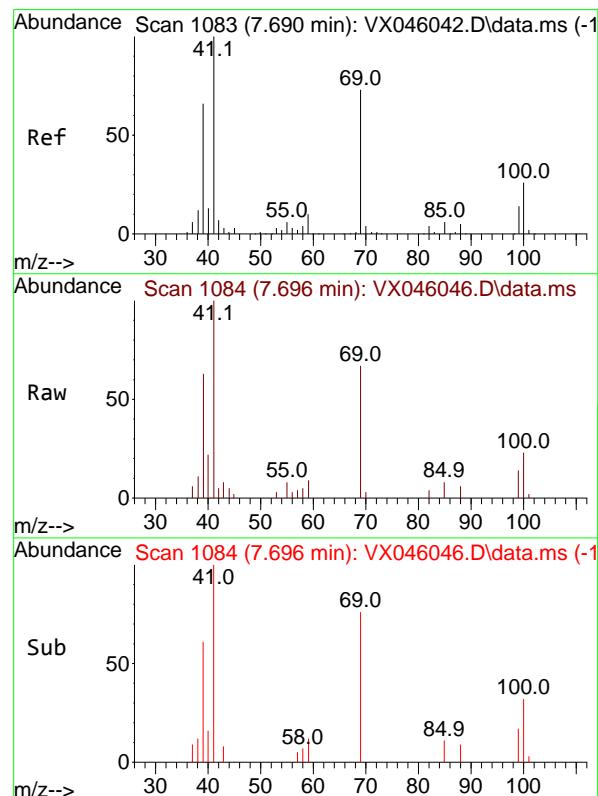Bromodichloromethane  
Concen: 3.254 ug/lRT: 7.818 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005**Manual Integrations  
APPROVED**Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

#48

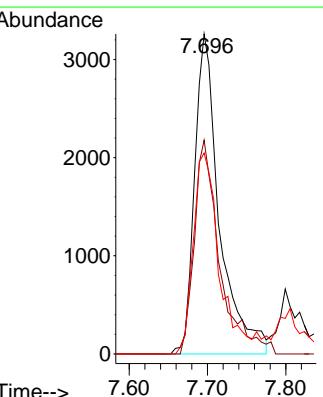Methyl methacrylate  
Concen: 3.321 ug/l  
RT: 7.696 min Scan# 1084  
Delta R.T. 0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04Tgt Ion: 41 Resp: 7171  
Ion Ratio Lower Upper  
41 100  
69 68.4 58.5 87.7  
39 65.1 51.7 77.5



#49

1,4-Dioxane

Concen: 67.721 ug/l

RT: 7.659 min Scan# 1078

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X

ClientSampleId :




VSTDICC005

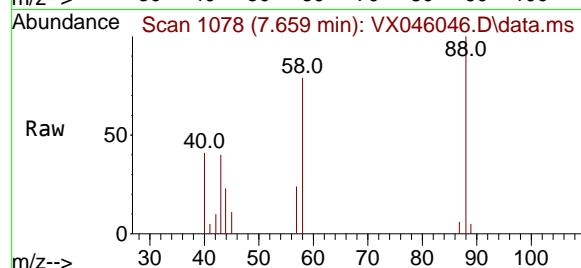


Tgt Ion:	88	Ion Ratio	2901
Ion	100	Lower	Upper
43	45.3	33.4	50.2
58	71.0	58.6	88.0

### Manual Integrations APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025




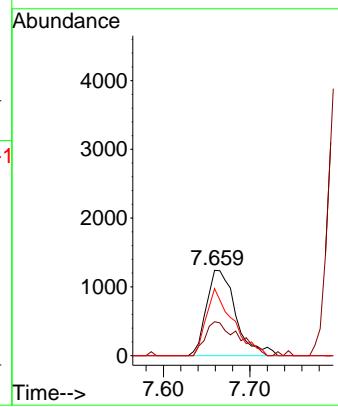
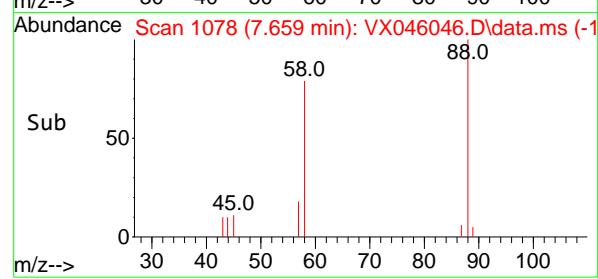


#50  
Toluene-d8  
Concen: 3.232 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04



Tgt Ion:	98	Ion Ratio	20566
Ion	100	Lower	Upper
100	66.1	53.5	80.3

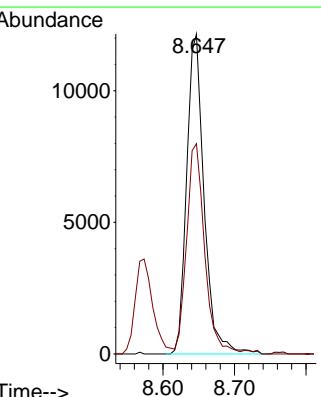

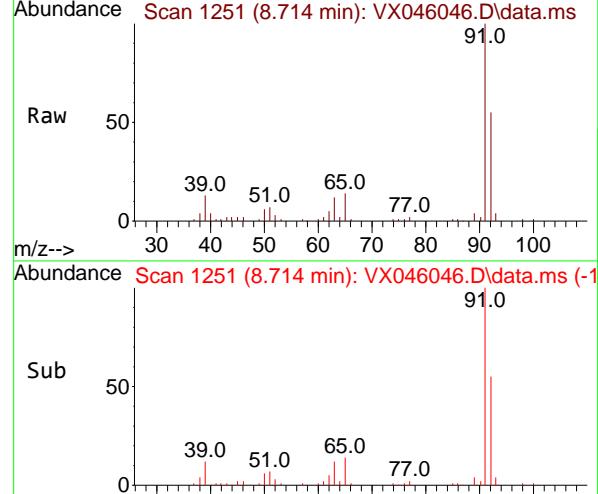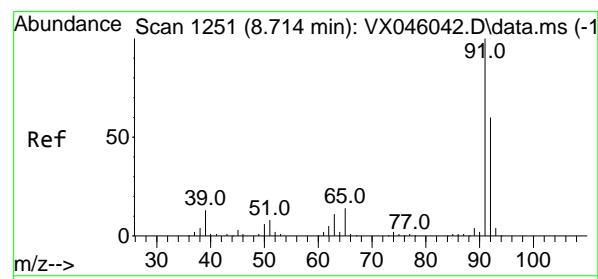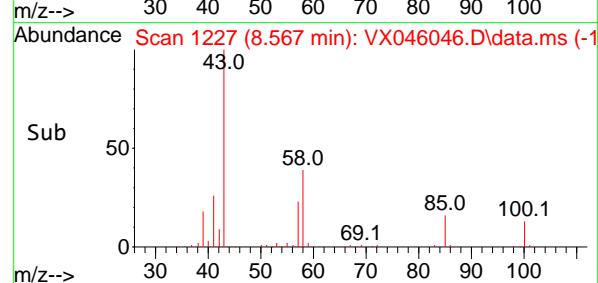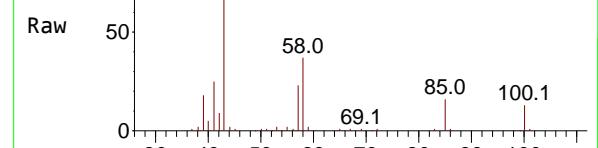

#51

4-Methyl-2-Pentanone

Concen: 16.967 ug/l

RT: 8.567 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#52

Toluene

Concen: 3.505 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04




Tgt Ion: 92 Resp: 14126

Ion Ratio Lower Upper

92 100

91 167.2 136.6 205.0

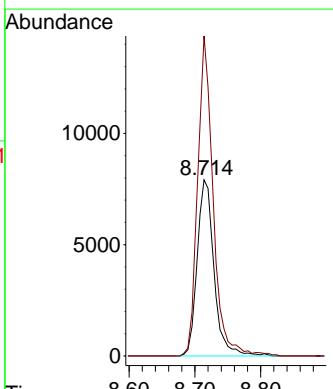



#53

t-1,3-Dichloropropene

Concen: 3.155 ug/l

RT: 8.976 min Scan# 1294

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#54

cis-1,3-Dichloropropene

Concen: 3.129 ug/l

RT: 8.366 min Scan# 1194

Delta R.T. 0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 75 Resp: 7908







Ion Ratio Lower Upper

75 100

77 31.9 25.4 38.0

39 55.3 52.2 78.4

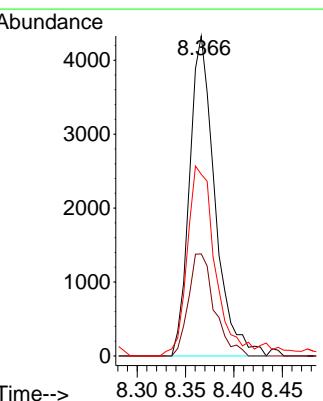




#55

1,1,2-Trichloroethane  
Concen: 3.490 ug/l  
RT: 9.153 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025


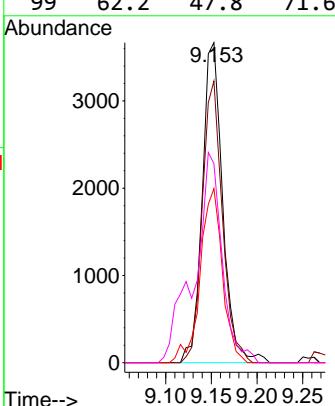


#56

Ethyl methacrylate  
Concen: 3.390 ug/l  
RT: 9.116 min Scan# 1317  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion: 69 Resp: 8555  
Ion Ratio Lower Upper  
69 100  
41 73.7 60.8 91.2  
39 49.3 39.0 58.6

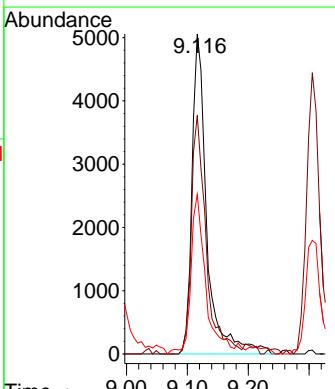

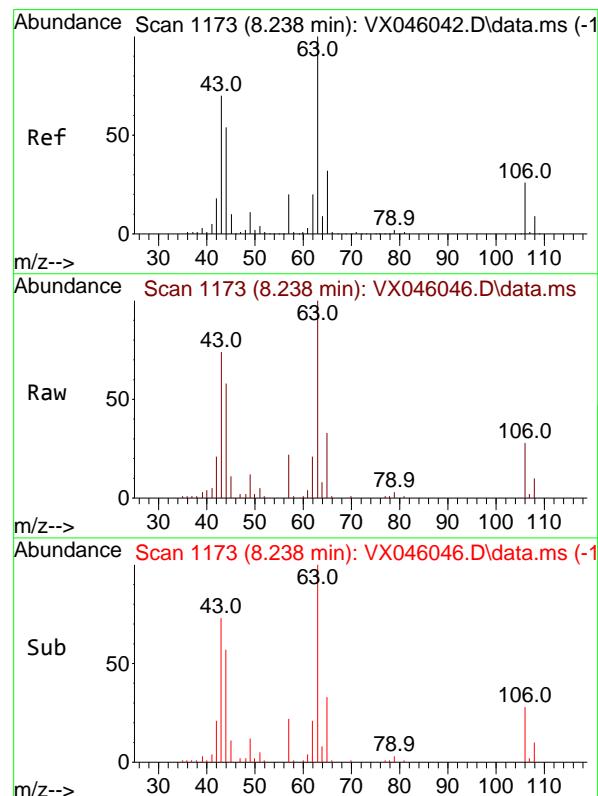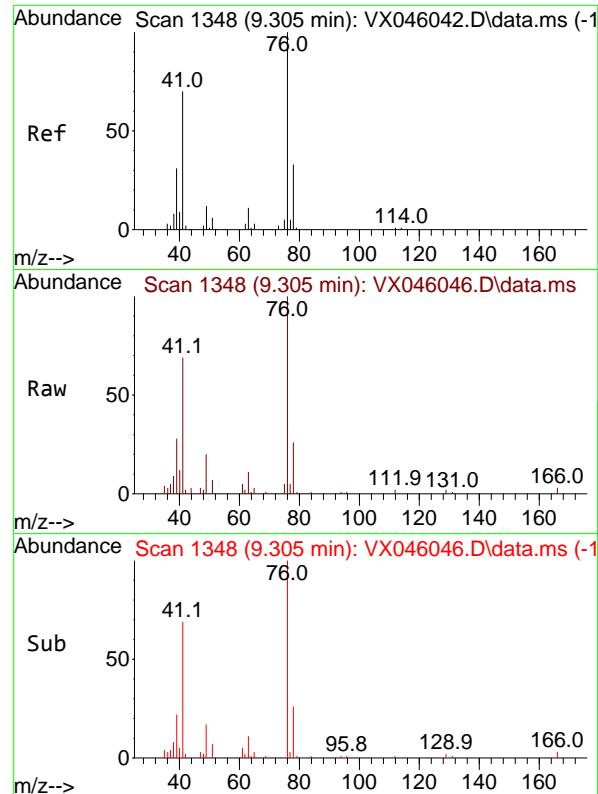

#57

1,3-Dichloropropane

Concen: 3.508 ug/l

RT: 9.305 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

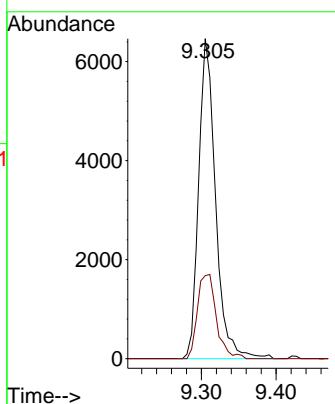

#58

2-Chloroethyl Vinyl ether

Concen: 18.346 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04


Tgt Ion: 63 Resp: 20809

Ion Ratio Lower Upper

63 100

106 26.4 21.5 32.3

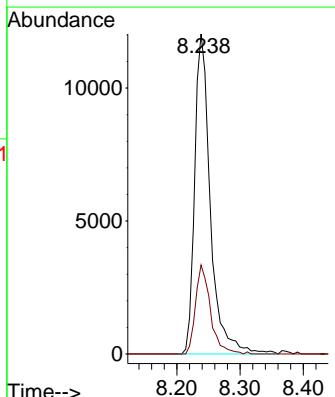

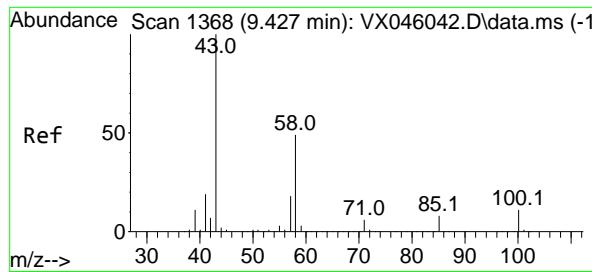

#59  
2-Hexanone  
Concen: 16.651 ug/l  
RT: 9.427 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC005




```

Tgt Ion: 43 Resp: 3485
Ion Ratio Lower Upper
 43 100
 58 47.5 24.9 74.6

```

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025


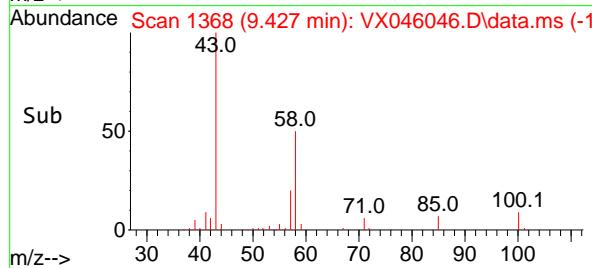
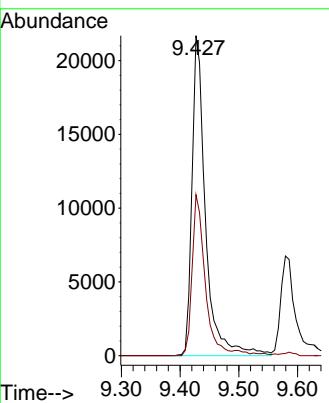
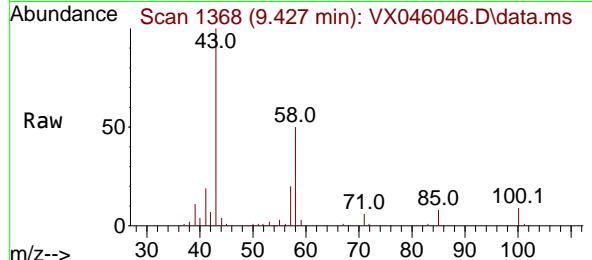





#60  
Dibromochloromethane  
Concen: 3.102 ug/l  
RT: 9.518 min Scan# 1383  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

```

Tgt Ion:129 Resp:      5500
Ion    Ratio   Lower   Upper
129    100
127    80.4    39.3   117.8

```

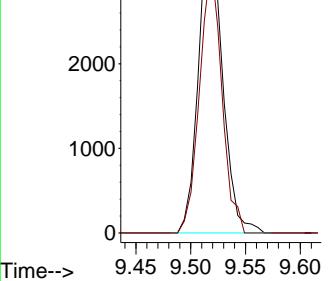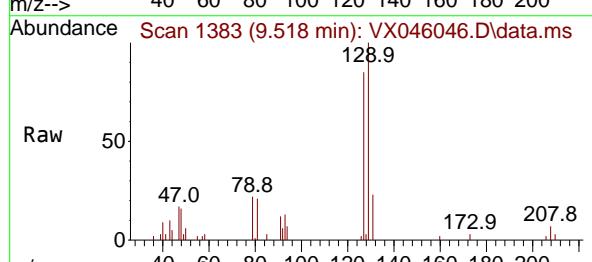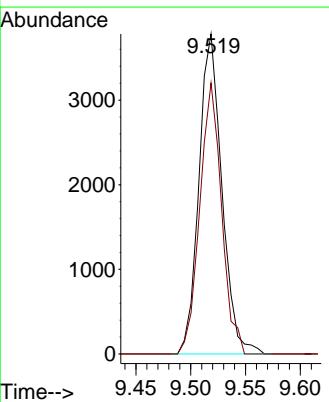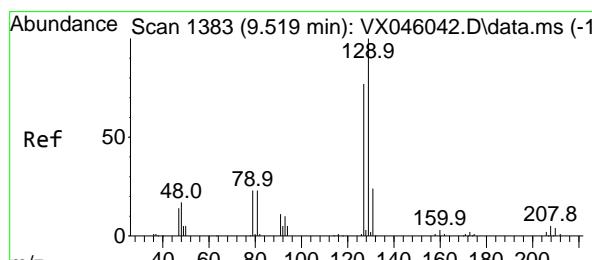

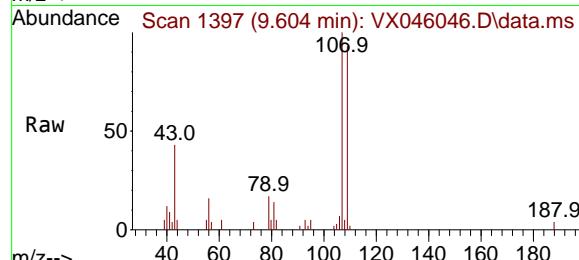

#61

1,2-Dibromoethane

Concen: 3.356 ug/l

RT: 9.604 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#62

4-Bromofluorobenzene

Concen: 3.378 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion: 95 Resp: 7822


Ion Ratio Lower Upper

95 100

174 65.0 0.0 135.8

176 66.6 0.0 131.4

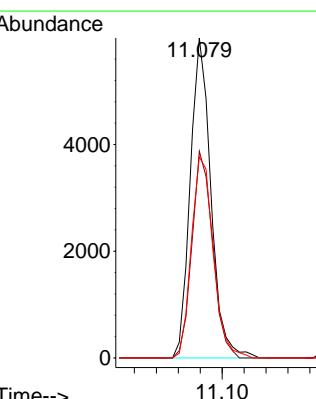


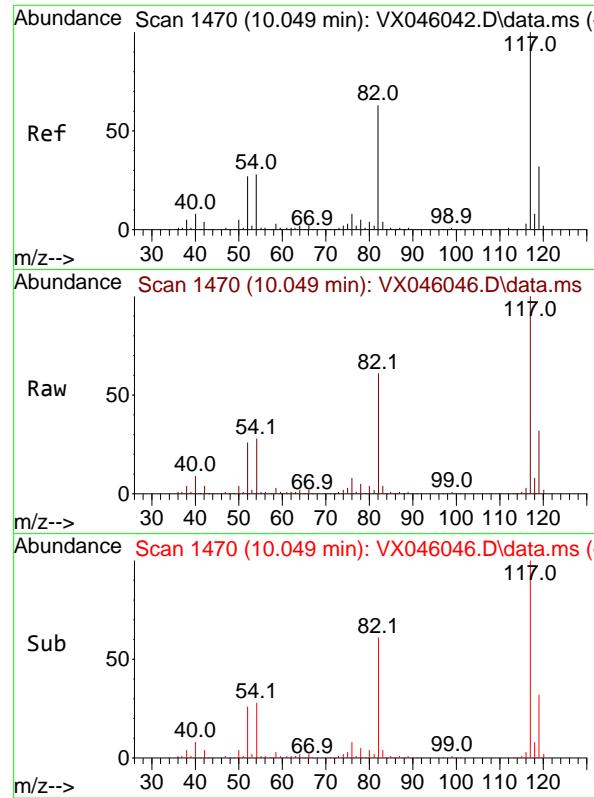


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

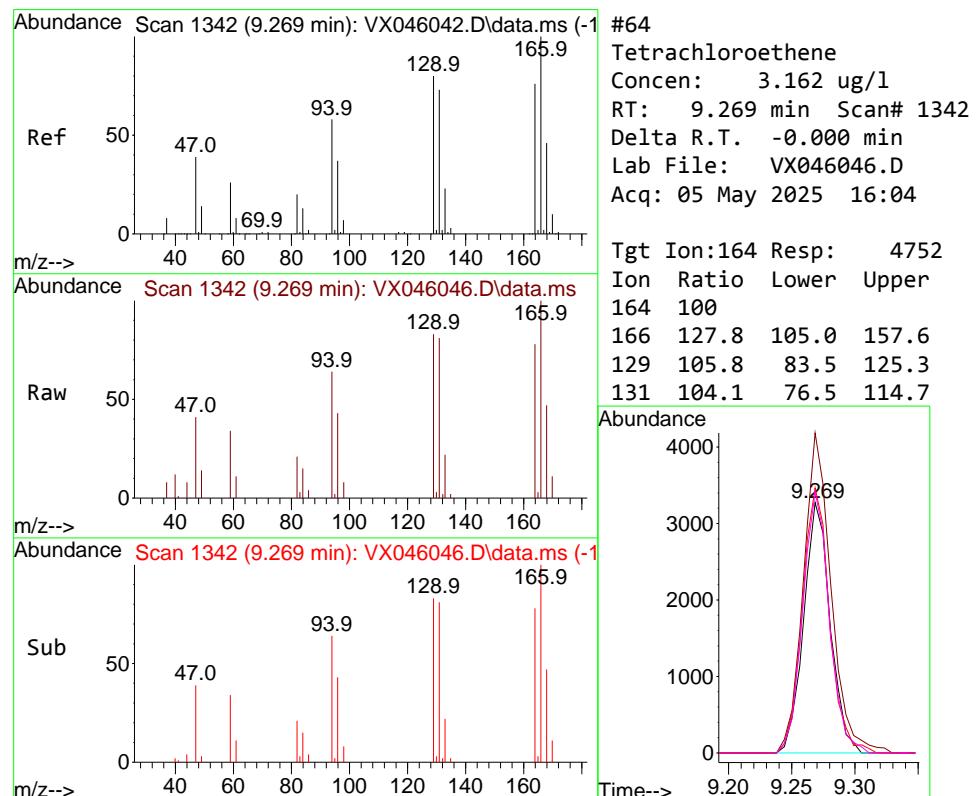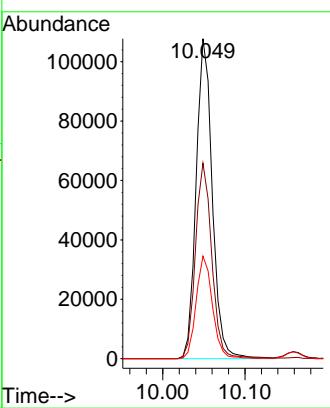

#64  
Tetrachloroethene  
Concen: 3.162 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion:164 Resp: 4752  
Ion Ratio Lower Upper  
164 100  
166 127.8 105.0 157.6  
129 105.8 83.5 125.3  
131 104.1 76.5 114.7

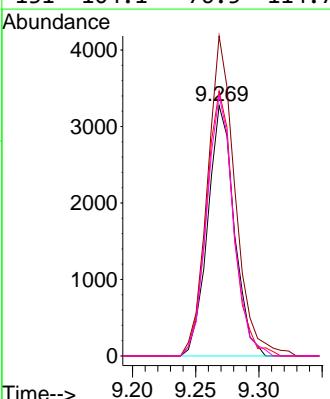

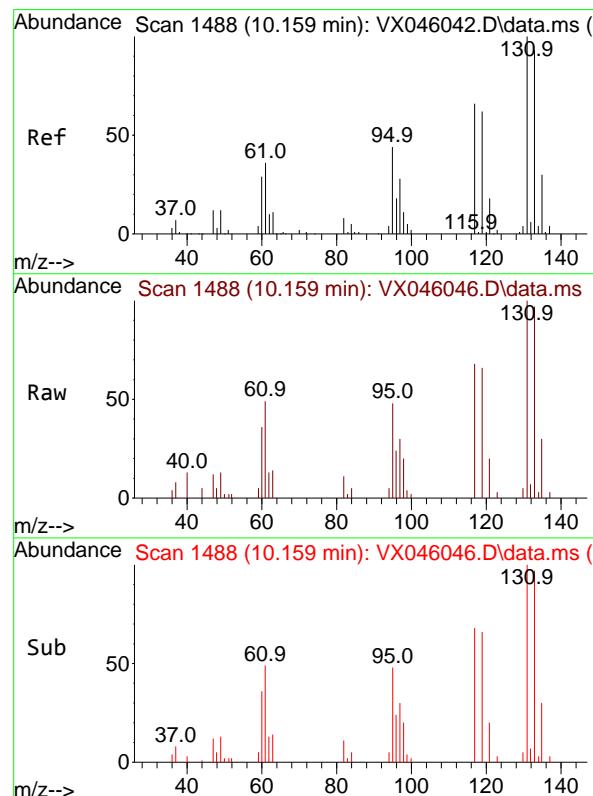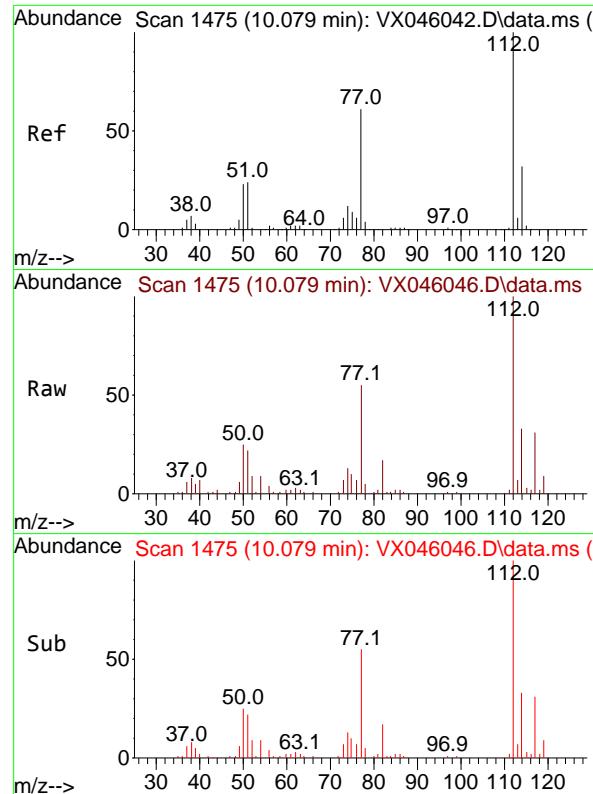


#65  
Chlorobenzene  
Concen: 3.399 ug/l  
RT: 10.079 min Scan# 1475  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005

Tgt Ion:112 Resp: 1539  
Ion Ratio Lower Upper  
112 100  
114 32.6 25.4 38.2


### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025






#66  
1,1,1,2-Tetrachloroethane  
Concen: 3.326 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion:131 Resp: 5024  
Ion Ratio Lower Upper  
131 100  
133 95.0 47.3 141.9  
119 64.8 31.6 95.0







Abundance Scan 1494 (10.195 min): VX046046.D\data.ms (-)

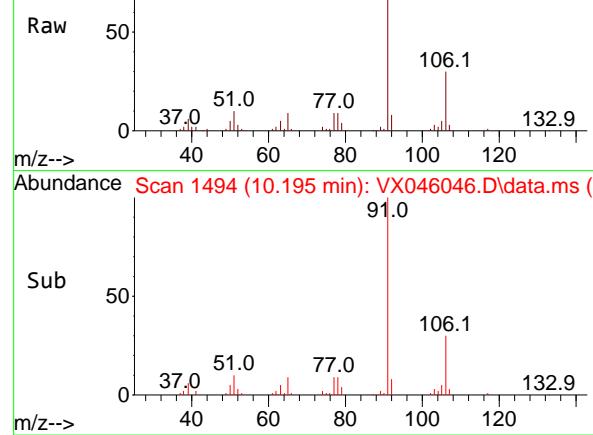

Abundance Scan 1511 (10.299 min): VX046046.D\data.ms (-)

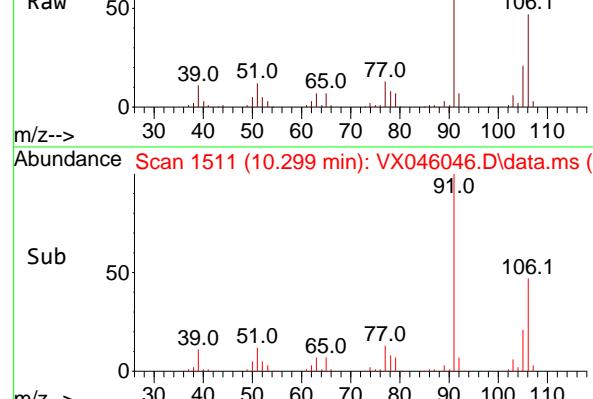

Abundance Scan 1511 (10.299 min): VX046046.D\data.ms (-)

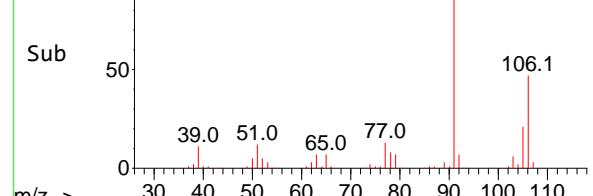

#67

Ethyl Benzene

Concen: 3.463 ug/l

RT: 10.195 min Scan# 1493

Delta R.T. 0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC005

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#68

m/p-Xylenes

Concen: 7.156 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04


Tgt Ion:106 Resp: 19957

Ion Ratio Lower Upper

106 100

91 210.1 171.2 256.8




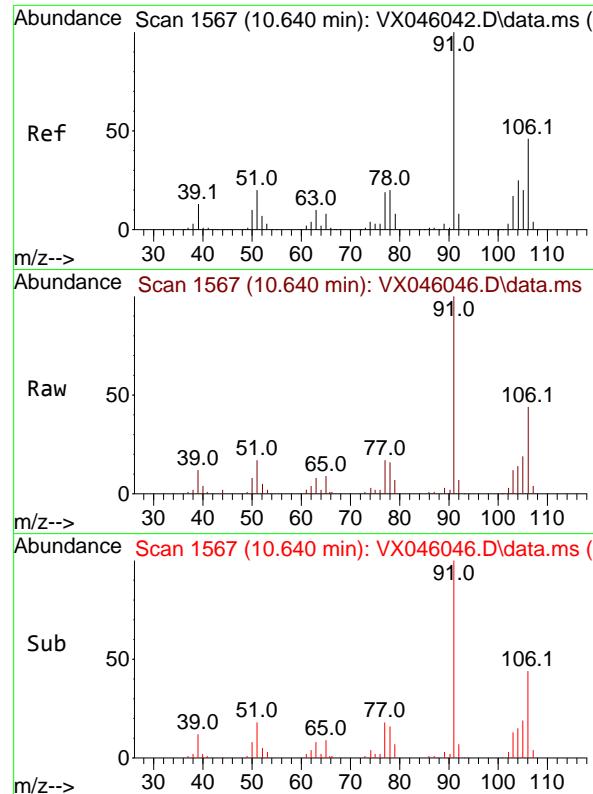


#69  
o-Xylene  
Concen: 3.343 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

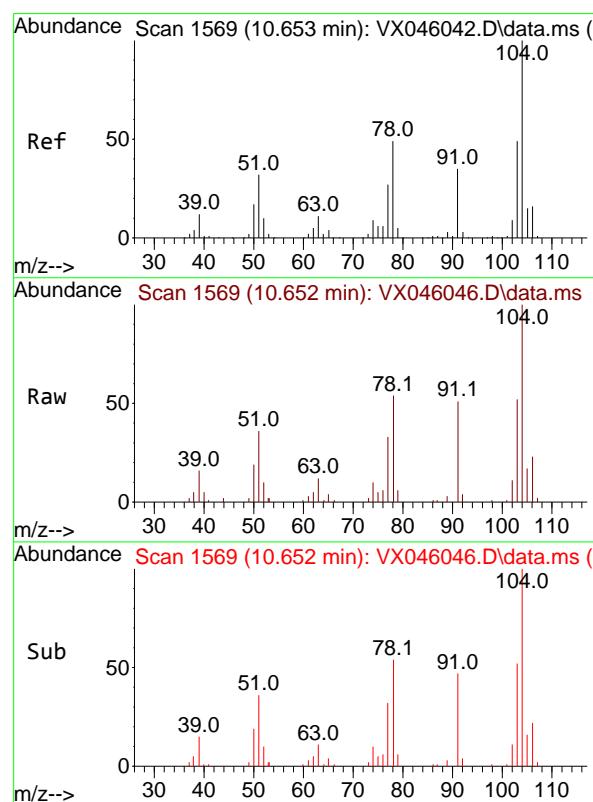

#70  
Styrene  
Concen: 3.312 ug/l  
RT: 10.652 min Scan# 1569  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion:104 Resp: 14900  
Ion Ratio Lower Upper  
104 100  
78 57.9 45.7 68.5  
103 55.6 43.7 65.5

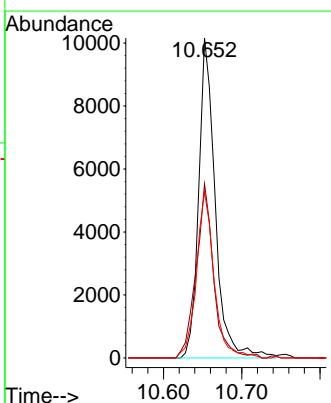

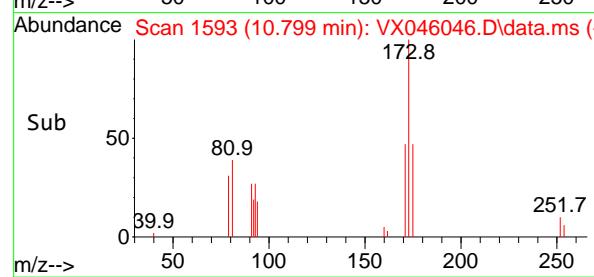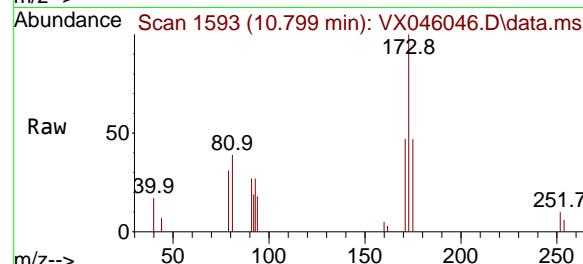

#71

Bromoform

Concen: 3.059 ug/l

RT: 10.799 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion:152 Resp: 67939


Ion Ratio Lower Upper

152 100

115 66.8 46.9 140.7

150 157.5 0.0 351.0

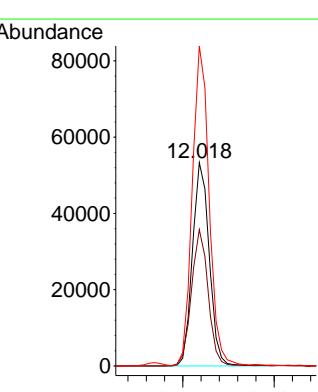

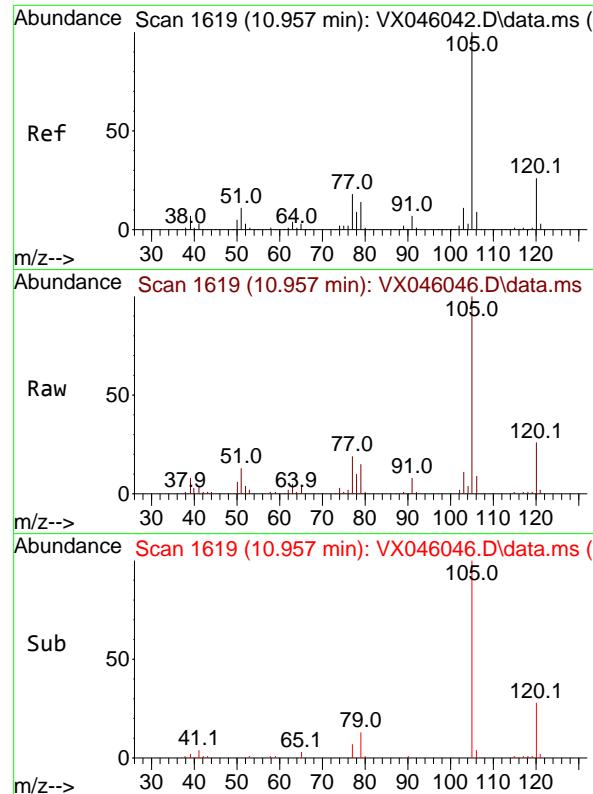

#73

Isopropylbenzene

Concen: 3.266 ug/l

RT: 10.957 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC005

Tgt Ion:105 Resp: 2420  
Ion Ratio Lower Upper  
105 100  
120 26.4 12.8 38.4

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

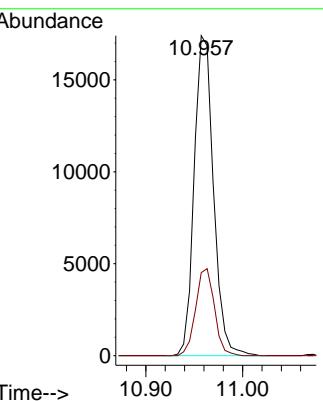

#74

N-amyl acetate

Concen: 3.038 ug/l


RT: 10.841 min Scan# 1600


Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt Ion: 43 Resp: 11224  
Ion Ratio Lower Upper  
43 100  
70 35.4 30.9 46.3  
55 25.0 18.7 28.1  
61 19.6 17.1 25.7

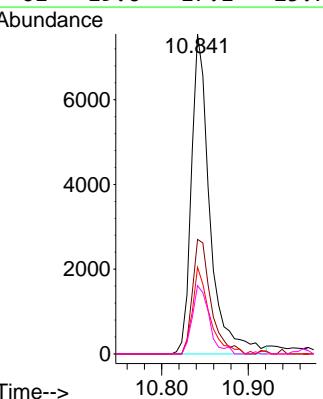

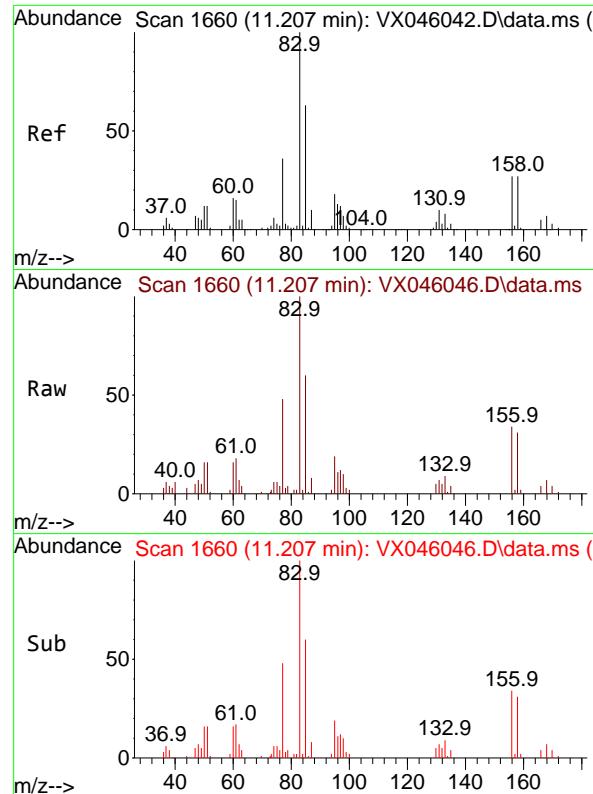


#75  
1,1,2,2-Tetrachloroethane  
Concen: 3.479 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

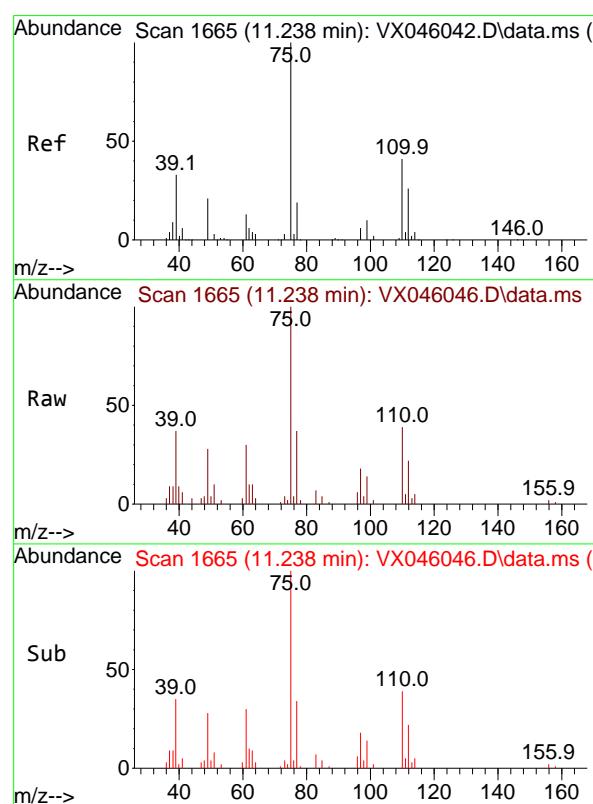

#76  
1,2,3-Trichloropropane  
Concen: 2.799 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion: 75 Resp: 7928  
Ion Ratio Lower Upper  
75 100  
77 40.6 20.5 61.5

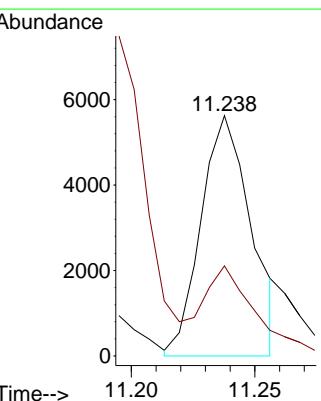



#77

Bromobenzene

Concen: 3.417 ug/l

RT: 11.195 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#78

n-propylbenzene

Concen: 3.424 ug/l

RT: 11.299 min Scan# 1675

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04




Tgt Ion: 91 Resp: 28436

Ion Ratio Lower Upper

91 100

120 21.7 10.8 32.4

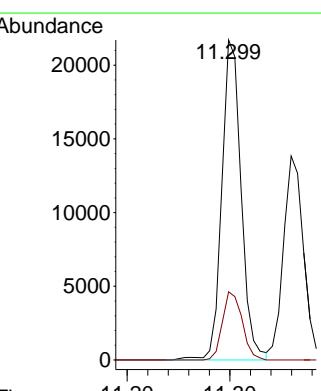



#79

2-Chlorotoluene

Concen: 3.336 ug/l

RT: 11.360 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#80

1,3,5-Trimethylbenzene

Concen: 3.372 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX046046.D


Acq: 05 May 2025 16:04

Tgt Ion:105 Resp: 20742

Ion Ratio Lower Upper

105 100

120 45.9 23.1 69.2

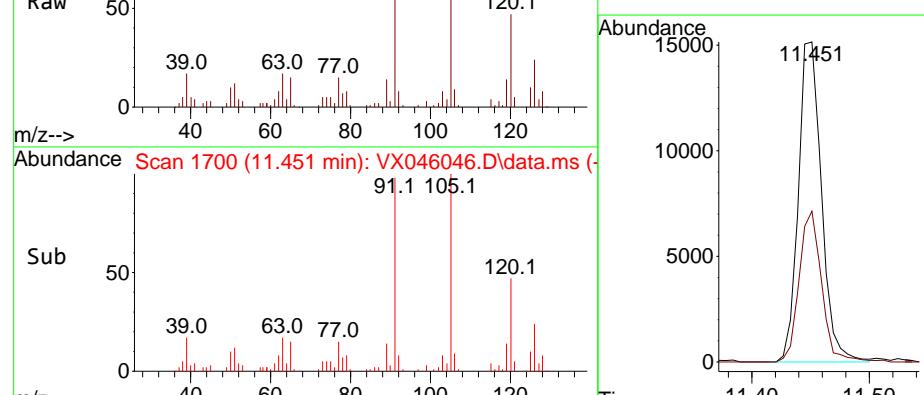



#13

#14

#15

#16

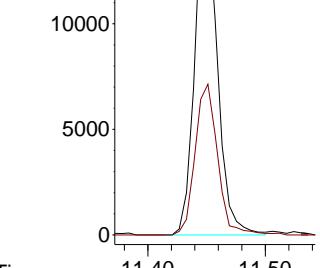


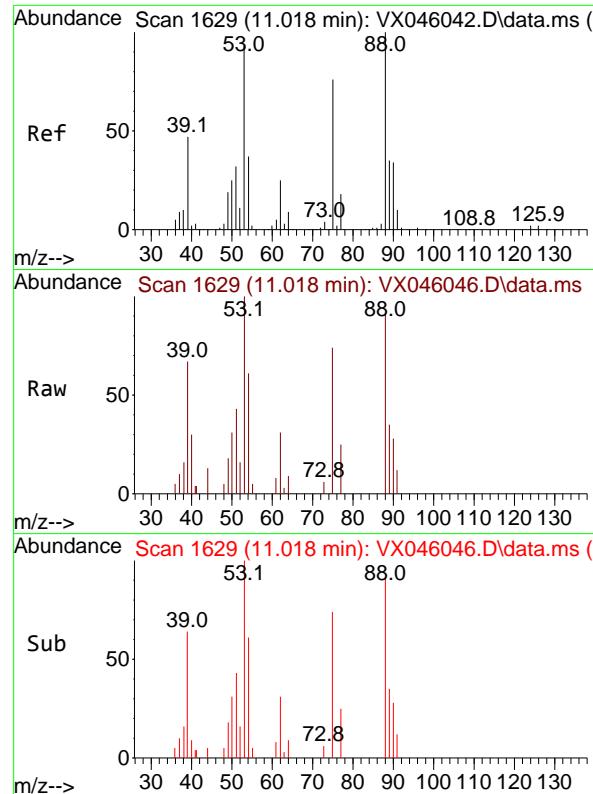


#81  
trans-1,4-Dichloro-2-butene  
Concen: 2.686 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

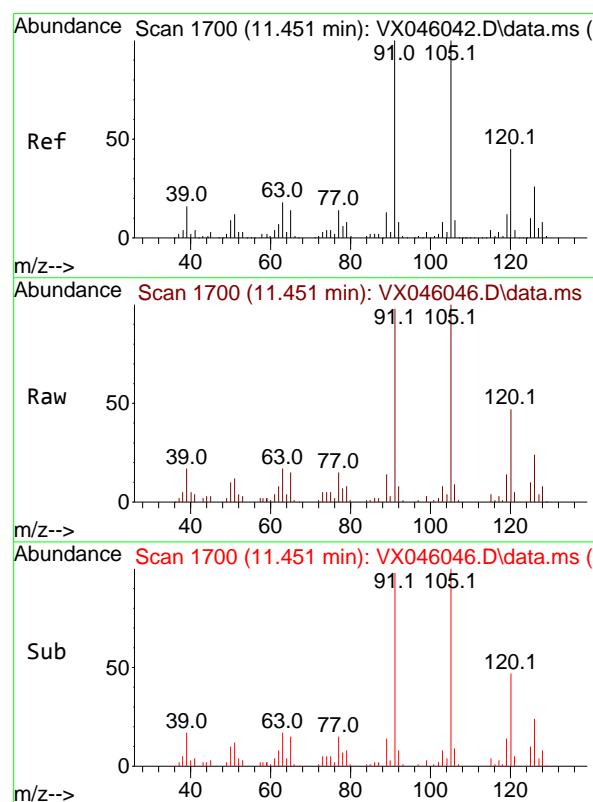

#82  
4-Chlorotoluene  
Concen: 3.245 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion: 91 Resp: 19966  
Ion Ratio Lower Upper  
91 100  
126 27.3 13.3 39.8

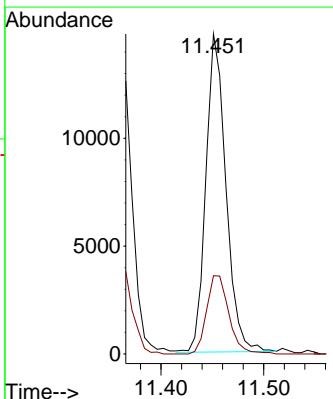

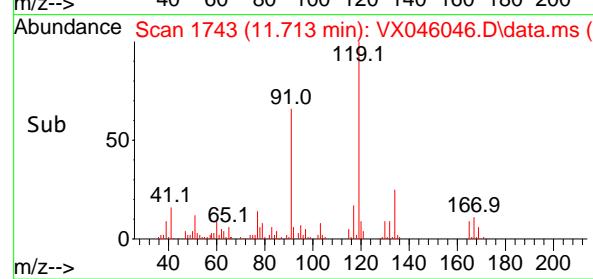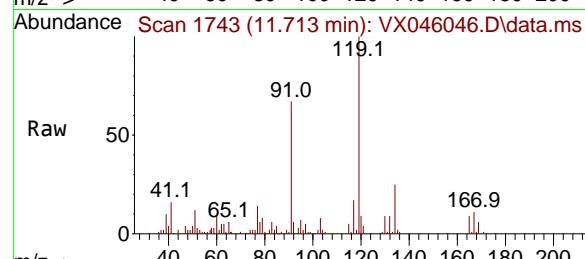

#83

tert-Butylbenzene

Concen: 3.484 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

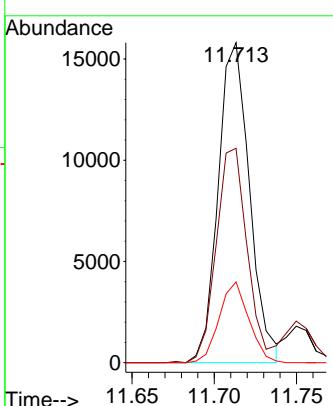

#84

1,2,4-Trimethylbenzene

Concen: 3.355 ug/l


RT: 11.750 min Scan# 1749




Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt	Ion:105	Resp:	20613
Ion	Ratio	Lower	Upper
105	100		
120	44.5	21.2	63.6





#85

sec-Butylbenzene

Concen: 3.412 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC005

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

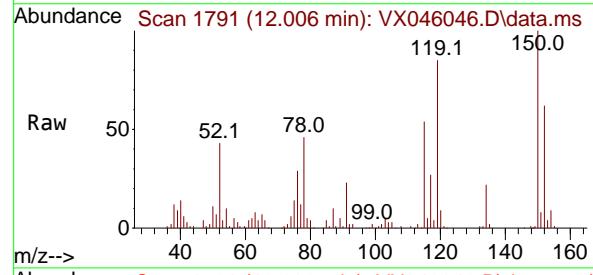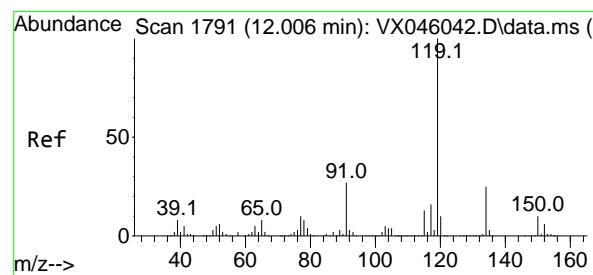

#86

p-Isopropyltoluene

Concen: 3.460 ug/l


RT: 12.006 min Scan# 1791


Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt	Ion:119	Resp:	20955
Ion	Ratio	Lower	Upper
119	100		
134	25.6	12.5	37.5
91	28.0	13.8	41.4

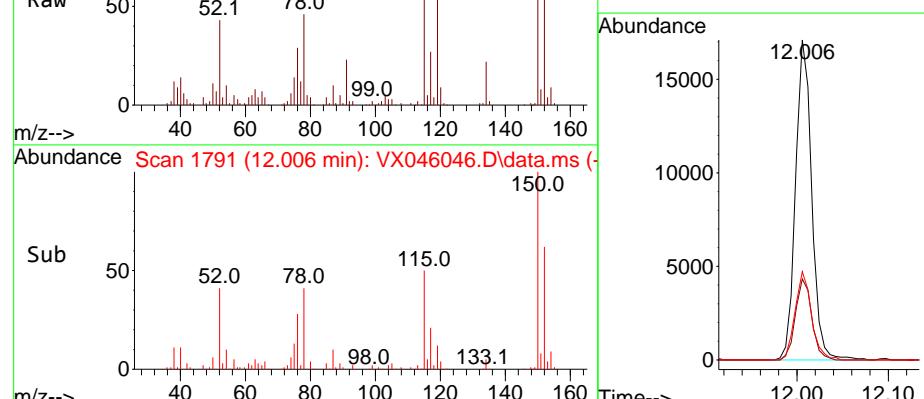

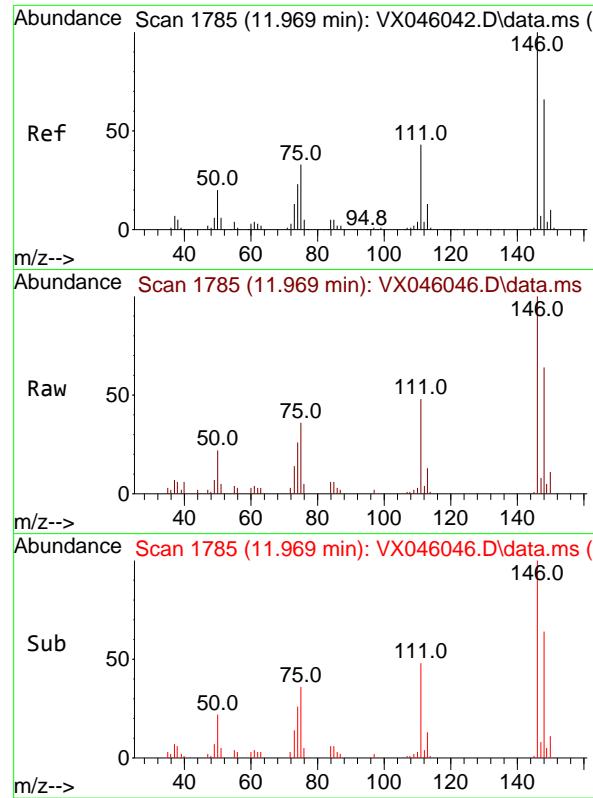

#87

1,3-Dichlorobenzene

Concen: 3.315 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC005

Tgt Ion:146 Resp: 10589

Ion Ratio Lower Upper

146 100

111 46.2 22.1 66.3



148 62.4 32.1 96.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

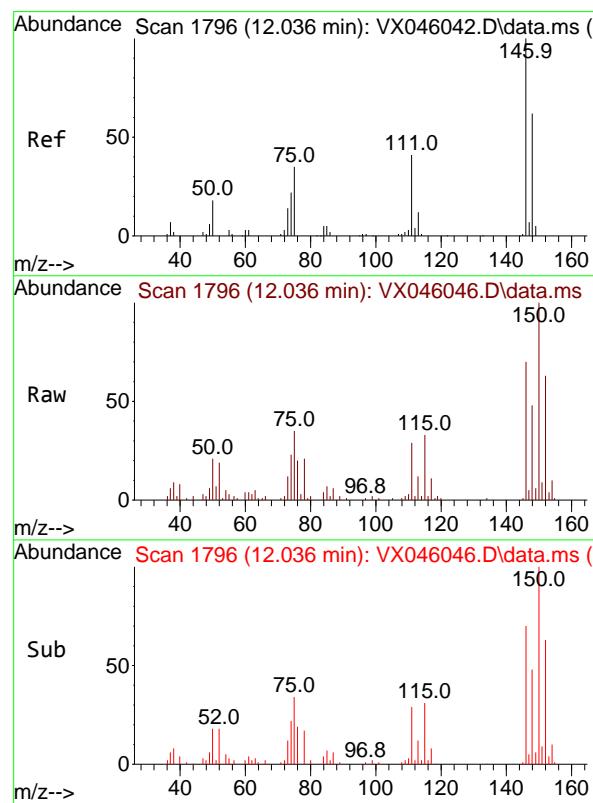

#88

1,4-Dichlorobenzene

Concen: 3.486 ug/l

RT: 12.036 min Scan# 1796

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04


Tgt Ion:146 Resp: 10908




Ion Ratio Lower Upper

146 100

111 52.1 21.3 63.9

148 69.4 31.9 95.5

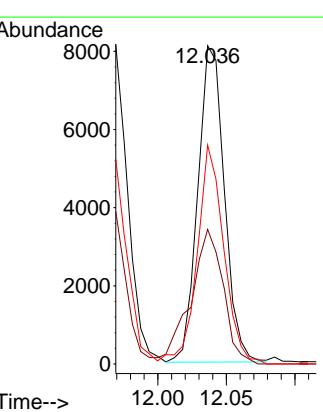



#89

n-Butylbenzene

Concen: 3.419 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04




Instrument: MSVOA\_X

ClientSampleId: VSTDICC005

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025







Supervised By :Mahesh Dadoda 05/06/2025

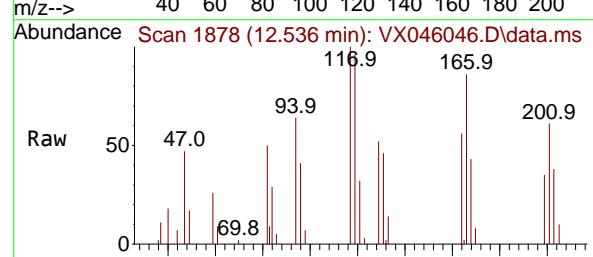

#90  
Hexachloroethane  
Concen: 3.153 ug/l  
RT: 12.536 min Scan# 1878  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion:117 Resp: 3553  
Ion Ratio Lower Upper  
117 100  
201 58.5 31.6 94.7



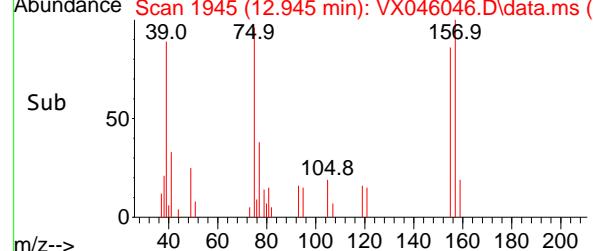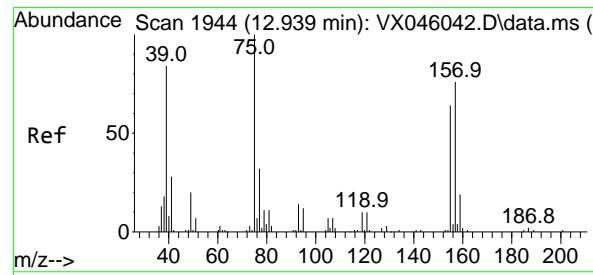

#91

1,2-Dichlorobenzene

Concen: 3.444 ug/l

RT: 12.335 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC005

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 2.812 ug/l


RT: 12.945 min Scan# 1945


Delta R.T. 0.006 min

Lab File: VX046046.D

Acq: 05 May 2025 16:04

Tgt	Ion	Resp:	1687
Ion	Ratio	Lower	Upper
75	100		
155	71.7	34.9	104.8
157	87.0	43.8	131.4

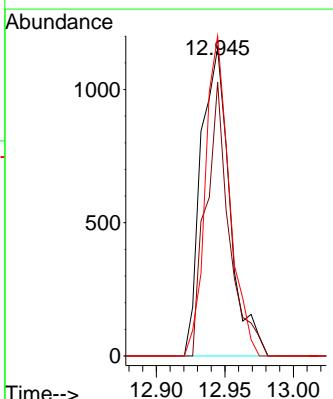


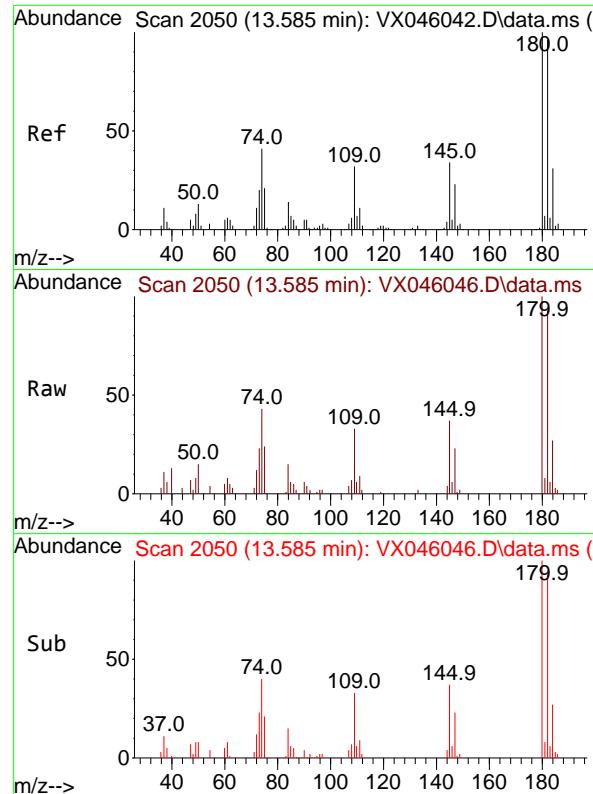


#93  
1,2,4-Trichlorobenzene  
Concen: 3.359 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

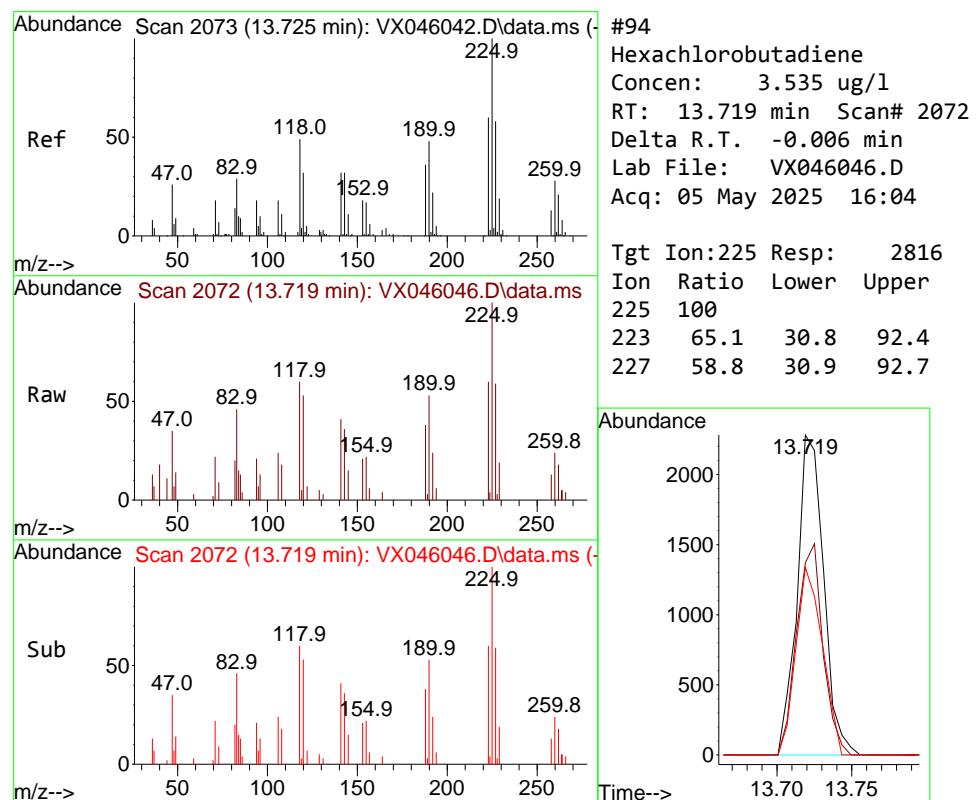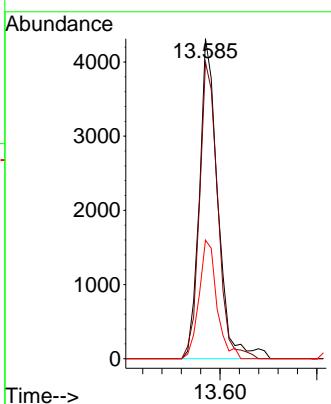

#94  
Hexachlorobutadiene  
Concen: 3.535 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. -0.006 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion:225 Resp: 2816  
Ion Ratio Lower Upper  
225 100  
223 65.1 30.8 92.4  
227 58.8 30.9 92.7

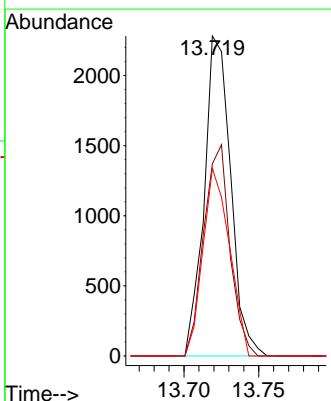


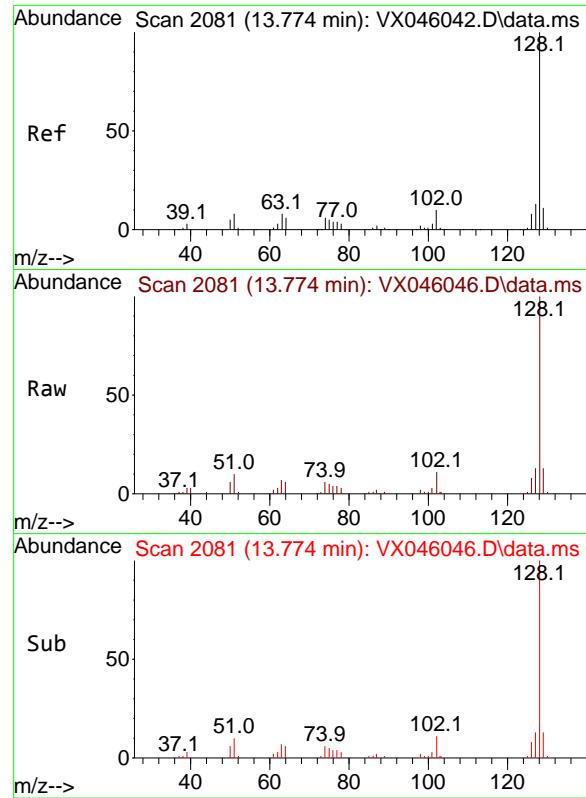


#95  
Naphthalene  
Concen: 3.209 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC005


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

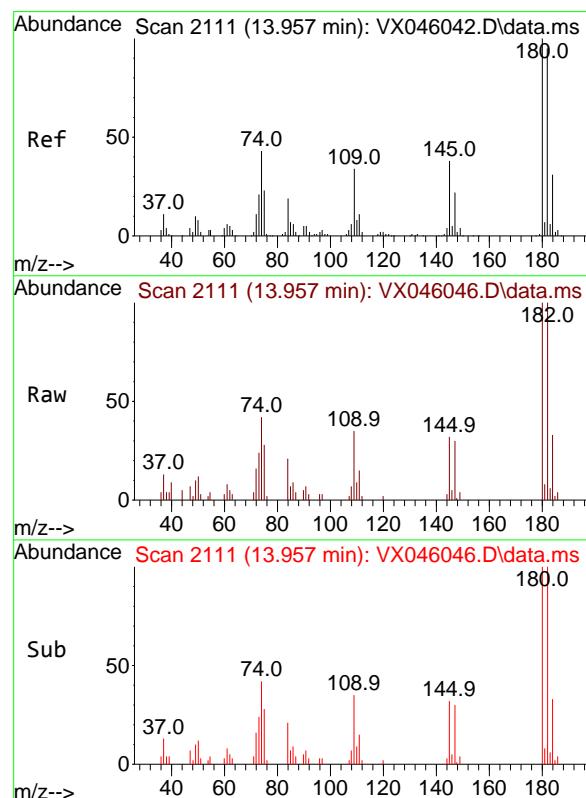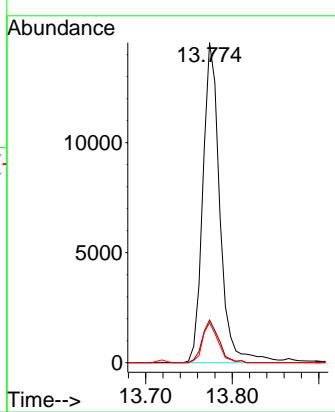

#96  
1,2,3-Trichlorobenzene  
Concen: 3.217 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046046.D  
Acq: 05 May 2025 16:04

Tgt Ion:180 Resp: 5745  
Ion Ratio Lower Upper  
180 100  
182 99.1 47.8 143.3  
145 34.8 18.1 54.3

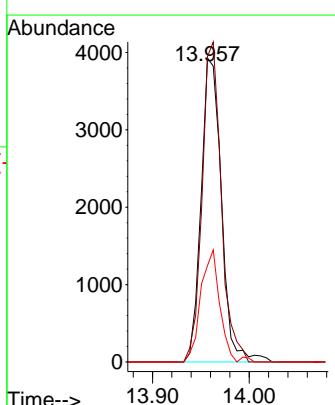

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046047.D  
 Acq On : 05 May 2025 16:27  
 Operator : JC/MD  
 Sample : VSTDICC001  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC001

Quant Time: May 06 06:13:30 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	92040	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	167022	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	140108	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	59123	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	0.000	65	0d	0.000	ug/l	
Spiked Amount	50.000	Range	74 - 125	Recovery	=	0.000%#
35) Dibromofluoromethane	0.000	113	0d	0.000	ug/l	
Spiked Amount	50.000	Range	75 - 124	Recovery	=	0.000%#
50) Toluene-d8	0.000	98	0d	0.000	ug/l	
Spiked Amount	50.000	Range	86 - 113	Recovery	=	0.000%#
62) 4-Bromofluorobenzene	0.000	95	0d	0.000	ug/l	
Spiked Amount	50.000	Range	77 - 121	Recovery	=	0.000%#
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	1211	0.596	ug/l	98
3) Chloromethane	1.307	50	1278	0.639	ug/l	97
4) Vinyl Chloride	1.374	62	1239	0.707	ug/l #	82
6) Chloroethane	1.678	64	859	0.951	ug/l	91
7) Trichlorofluoromethane	1.880	101	1959	0.734	ug/l	95
8) Diethyl Ether	2.130	74	742	0.845	ug/l	87
9) 1,1,2-Trichlorotrifluo...	2.319	101	1166	0.731	ug/l	96
12) 1,1-Dichloroethene	2.313	96	1093	0.704	ug/l #	87
14) Allyl chloride	2.654	41	1936	0.660	ug/l	89
15) Acrylonitrile	3.075	53	3343	3.424	ug/l	98
16) Acetone	2.380	43	3500	3.736	ug/l	97
17) Carbon Disulfide	2.508	76	2619	0.728	ug/l	98
18) Methyl Acetate	2.709	43	1852	0.828	ug/l	98
19) Methyl tert-butyl Ether	3.117	73	3588	0.662	ug/l	96
20) Methylene Chloride	2.782	84	1571	0.828	ug/l #	90
21) trans-1,2-Dichloroethene	3.081	96	1111	0.701	ug/l #	71
22) Diisopropyl ether	3.757	45	3857	0.703	ug/l #	26
23) Vinyl Acetate	3.727	43	15283	3.154	ug/l	96
24) 1,1-Dichloroethane	3.605	63	2054	0.637	ug/l	97
25) 2-Butanone	4.593	43	4558	3.371	ug/l	92
26) 2,2-Dichloropropane	4.458	77	1777	0.728	ug/l	84
27) cis-1,2-Dichloroethene	4.483	96	1324	0.693	ug/l	91
28) Bromochloromethane	4.910	49	1061m	0.619	ug/l	
29) Tetrahydrofuran	5.019	42	2931	3.338	ug/l	99
30) Chloroform	5.093	83	2328	0.695	ug/l	98
32) 1,1,1-Trichloroethane	5.379	97	1869	0.647	ug/l #	51
36) 1,1-Dichloropropene	5.684	75	1648	0.758	ug/l #	83
37) Ethyl Acetate	4.733	43	1956m	0.717	ug/l	
38) Carbon Tetrachloride	5.678	117	1807	0.724	ug/l #	78
39) Methylcyclohexane	7.373	83	2096	0.770	ug/l	97
40) Benzene	6.044	78	4502	0.668	ug/l #	89
41) Methacrylonitrile	4.946	41	778	0.513	ug/l #	56
42) 1,2-Dichloroethane	6.092	62	1934	0.694	ug/l	81
43) Isopropyl Acetate	6.354	43	2553	0.612	ug/l #	81
44) Trichloroethene	7.135	130	1083	0.680	ug/l	85
45) 1,2-Dichloropropane	7.440	63	1059	0.633	ug/l	89

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046047.D  
 Acq On : 05 May 2025 16:27  
 Operator : JC/MD  
 Sample : VSTDICC001  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDICC001

Quant Time: May 06 06:13:30 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 06:04:56 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) Dibromomethane	7.586	93	880	0.667	ug/1	97
47) Bromodichloromethane	7.818	83	1620	0.633	ug/1 #	91
48) Methyl methacrylate	7.714	41	1235m	0.577	ug/1	
49) 1,4-Dioxane	7.677	88	498	11.703	ug/1 #	66
51) 4-Methyl-2-Pentanone	8.580	43	9378	3.430	ug/1	97
52) Toluene	8.720	92	2684	0.672	ug/1	96
53) t-1,3-Dichloropropene	8.988	75	1238	0.576	ug/1 #	79
54) cis-1,3-Dichloropropene	8.379	75	1414	0.564	ug/1 #	87
55) 1,1,2-Trichloroethane	9.153	97	1029	0.637	ug/1	92
56) Ethyl methacrylate	9.128	69	1260	0.504	ug/1 #	76
57) 1,3-Dichloropropane	9.311	76	2036	0.711	ug/1	97
58) 2-Chloroethyl Vinyl ether	8.244	63	3846	3.420	ug/1	94
59) 2-Hexanone	9.439	43	6424	3.096	ug/1	88
60) Dibromochloromethane	9.525	129	1023	0.582	ug/1	93
61) 1,2-Dibromoethane	9.610	107	1077	0.650	ug/1	98
64) Tetrachloroethene	9.275	164	972	0.679	ug/1	95
65) Chlorobenzene	10.079	112	3170	0.735	ug/1	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	1035	0.720	ug/1 #	67
67) Ethyl Benzene	10.195	91	5052	0.687	ug/1	94
68) m/p-Xylenes	10.299	106	3630	1.367	ug/1	97
69) o-Xylene	10.640	106	1799	0.672	ug/1	94
70) Styrene	10.659	104	2664	0.622	ug/1	98
71) Bromoform	10.799	173	657	0.608	ug/1 #	100
73) Isopropylbenzene	10.963	105	4480	0.695	ug/1	96
74) N-amyl acetate	10.854	43	2028	0.631	ug/1 #	91
75) 1,1,2,2-Tetrachloroethane	11.213	83	1835	0.800	ug/1	94
76) 1,2,3-Trichloropropane	11.244	75	1661m	0.674	ug/1	
77) Bromobenzene	11.201	156	1095	0.734	ug/1	96
78) n-propylbenzene	11.305	91	5052	0.699	ug/1	97
79) 2-Chlorotoluene	11.360	91	3765	0.773	ug/1	94
80) 1,3,5-Trimethylbenzene	11.451	105	3590	0.671	ug/1	96
82) 4-Chlorotoluene	11.457	91	3815	0.713	ug/1	97
83) tert-Butylbenzene	11.713	119	3951	0.751	ug/1	97
84) 1,2,4-Trimethylbenzene	11.756	105	3725	0.697	ug/1	97
85) sec-Butylbenzene	11.890	105	4385	0.672	ug/1	100
86) p-Isopropyltoluene	12.006	119	3577	0.679	ug/1	94
87) 1,3-Dichlorobenzene	11.969	146	1914	0.689	ug/1	99
88) 1,4-Dichlorobenzene	12.036	146	2149m	0.789	ug/1	
89) n-Butylbenzene	12.335	91	2889	0.631	ug/1	92
90) Hexachloroethane	12.536	117	604	0.616	ug/1	99
91) 1,2-Dichlorobenzene	12.341	146	2022	0.747	ug/1	95
92) 1,2-Dibromo-3-Chloropr...	12.945	75	306	0.586	ug/1	83
93) 1,2,4-Trichlorobenzene	13.591	180	1019	0.688	ug/1	94
94) Hexachlorobutadiene	13.725	225	465	0.671	ug/1	89
95) Naphthalene	13.780	128	4138	0.767	ug/1	97
96) 1,2,3-Trichlorobenzene	13.963	180	1113	0.716	ug/1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed







Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046047.D  
Acq On : 05 May 2025 16:27  
Operator : JC/MD  
Sample : VSTDIICC001  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC001

## Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

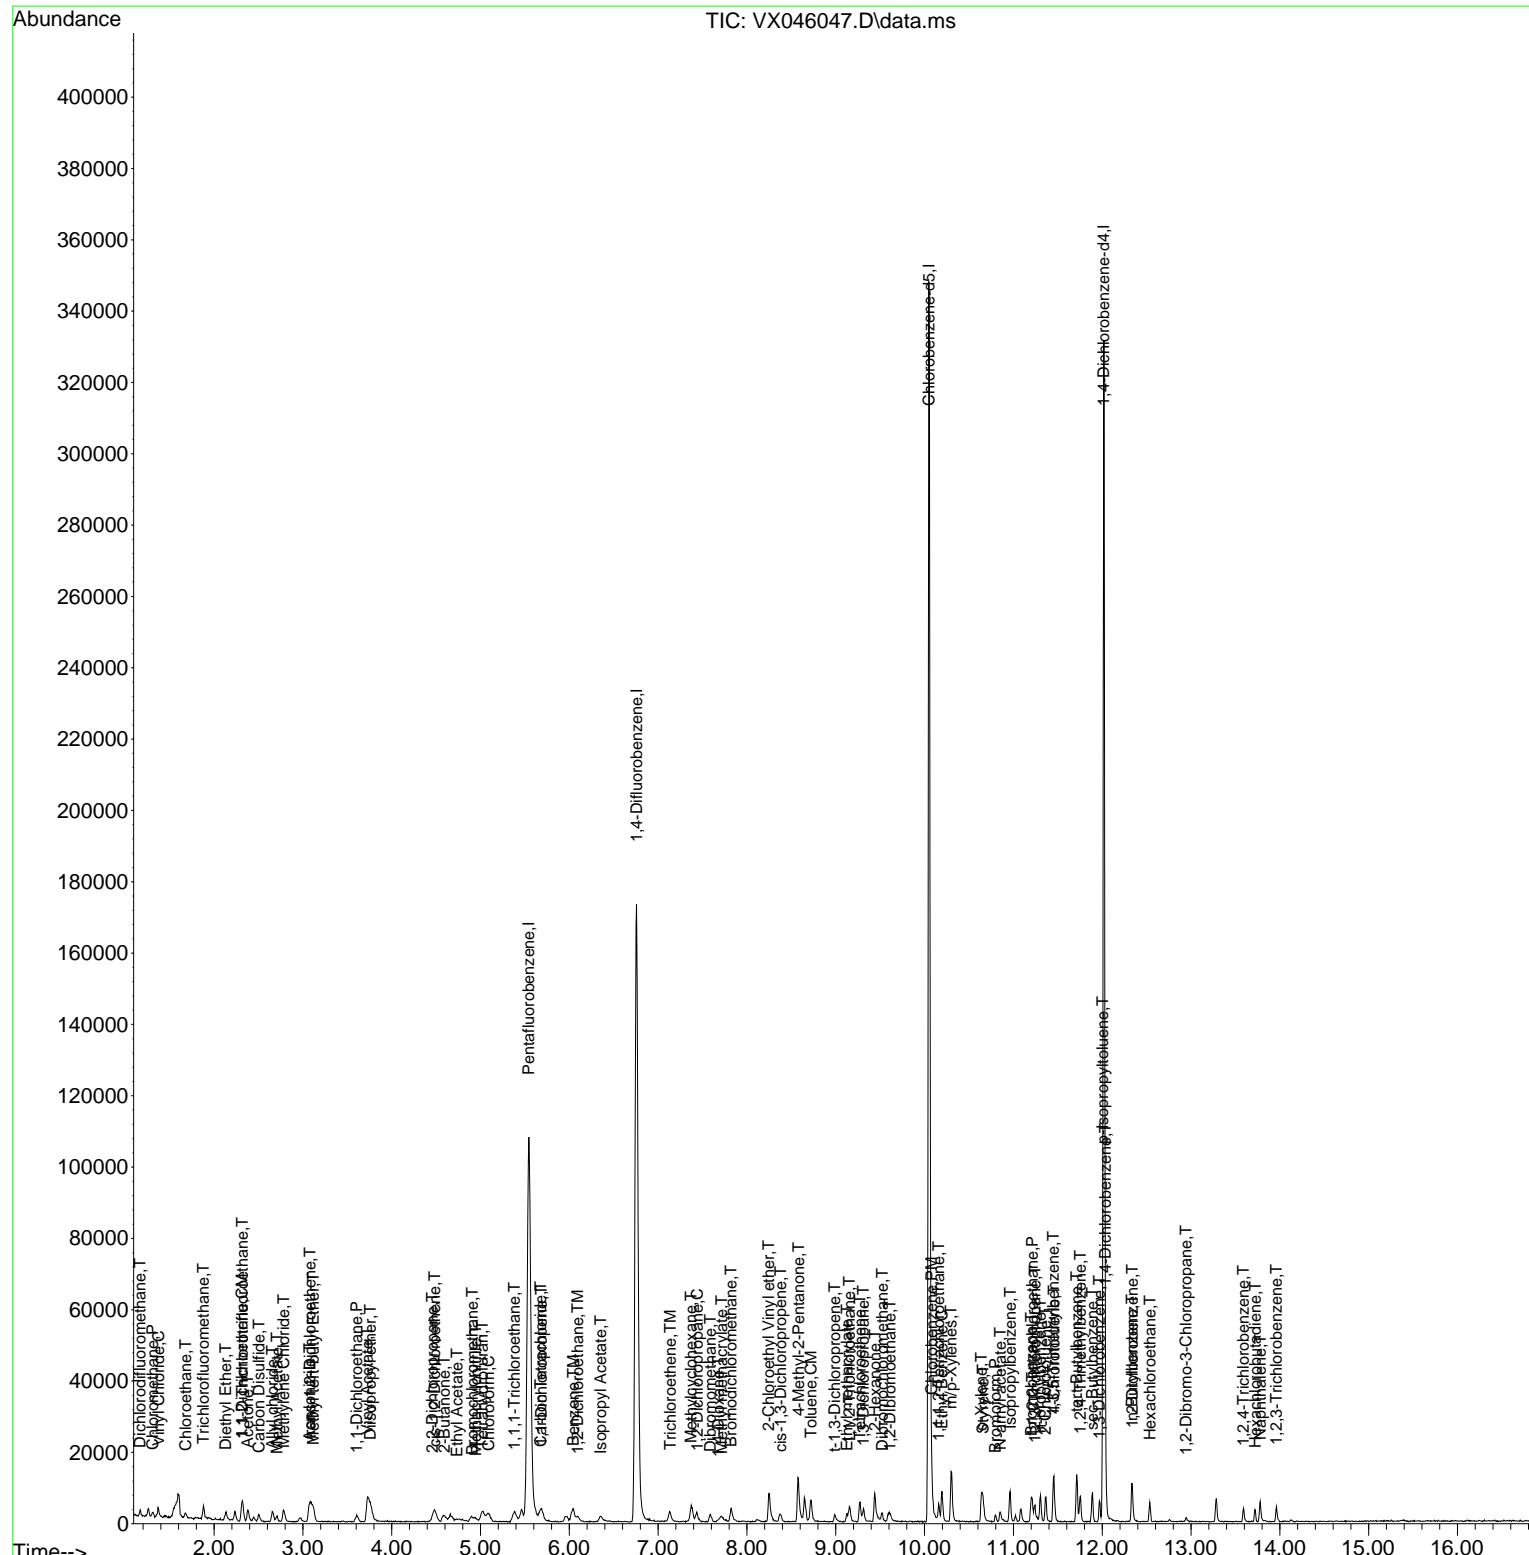



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.544 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

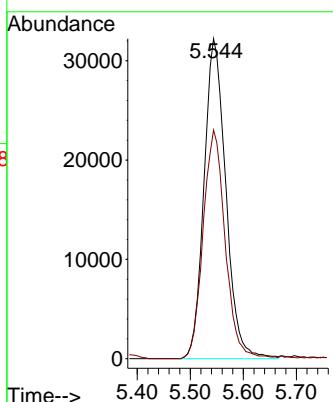

#2

Dichlorodifluoromethane

Concen: 0.596 ug/l


RT: 1.166 min Scan# 13


Delta R.T. -0.000 min

Lab File: VX046047.D


Acq: 05 May 2025 16:27

Tgt Ion: 85 Resp: 1211  
 Ion Ratio Lower Upper  
 85 100  
 87 32.4 15.7 47.1

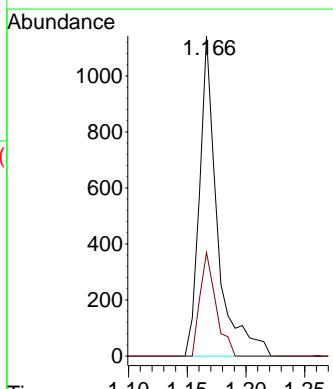



Abundance Scan 36 (1.307 min): VX046047.D\data.ms

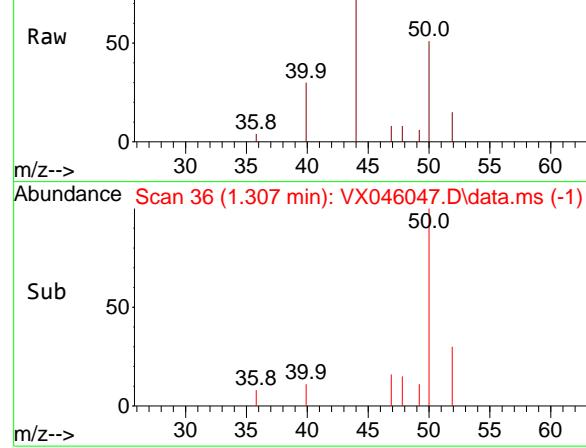

#3

Chloromethane

Concen: 0.639 ug/l

RT: 1.307 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC001


**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

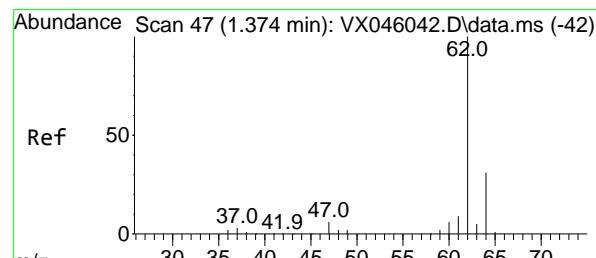

Abundance Scan 47 (1.374 min): VX046047.D\data.ms

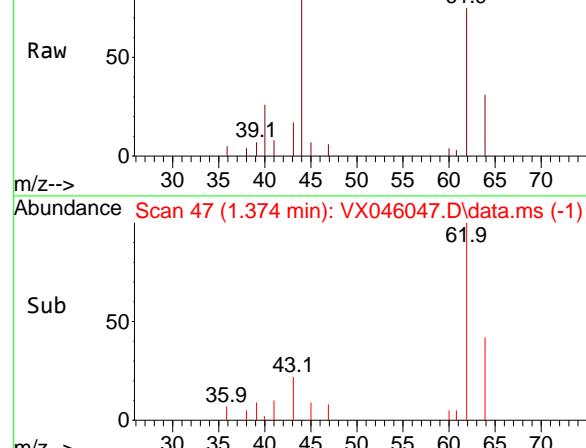

#4

Vinyl Chloride

Concen: 0.707 ug/l


RT: 1.374 min Scan# 47




Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion: 62 Resp: 1239  
Ion Ratio Lower Upper  
62 100  
64 41.7 25.2 37.8#

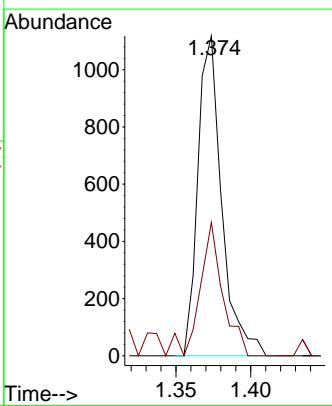

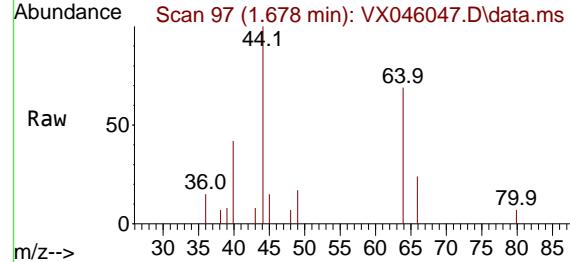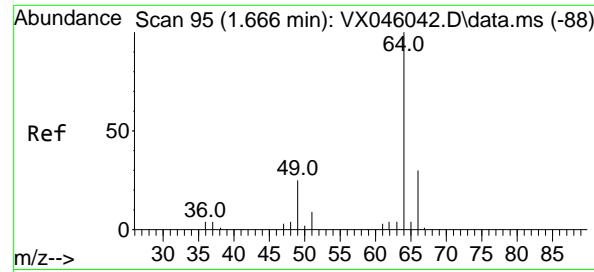

#6

Chloroethane

Concen: 0.951 ug/l

RT: 1.678 min Scan# 9

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X





ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#7

Trichlorofluoromethane

Concen: 0.734 ug/l


RT: 1.880 min Scan# 130


Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion:101 Resp: 1959  
 Ion Ratio Lower Upper  
 101 100  
 103 67.8 51.0 76.4

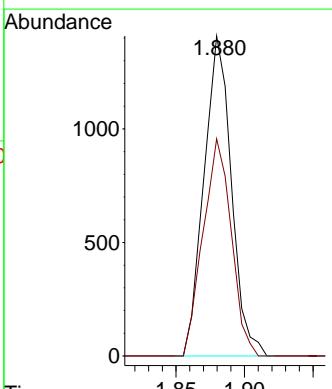

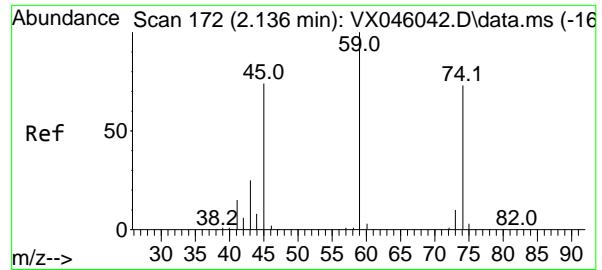

#8

Diethyl Ether

Concen: 0.845 ug/l

RT: 2.130 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX046047.D


Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC001

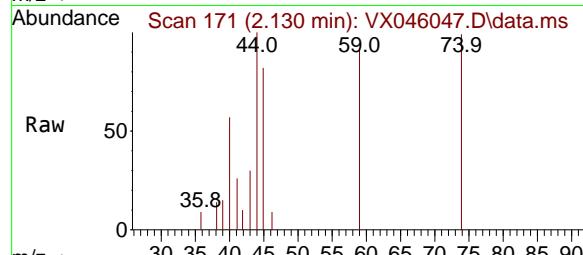

Tgt Ion: 74 Resp: 74.2

Ion Ratio Lower Upper







74 100


45 123.6 54.9 164.8

**Manual Integrations****APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025
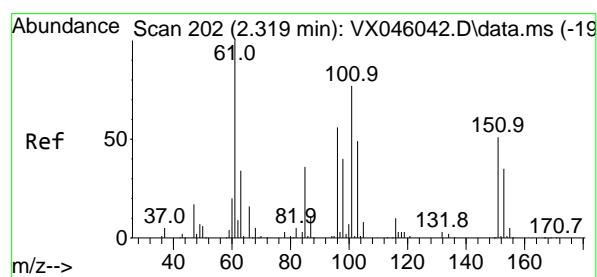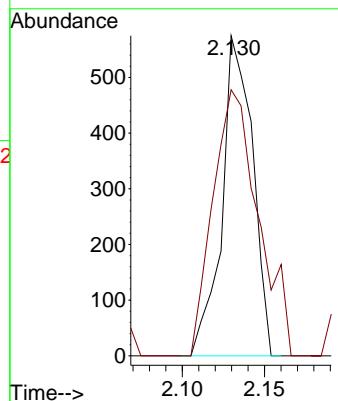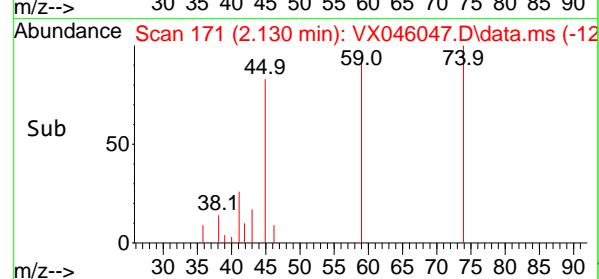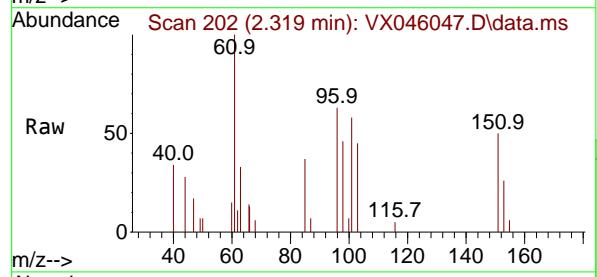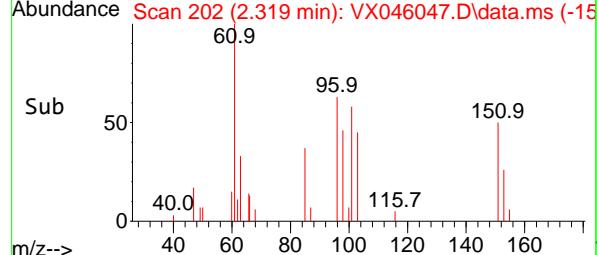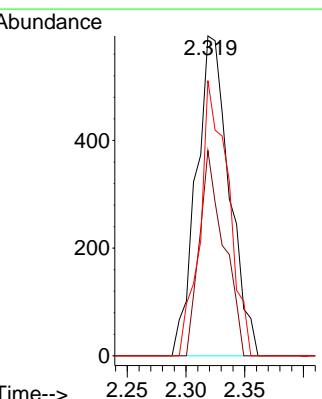
#9  
1,1,2-Trichlorotrifluoroethane  
Concen: 0.731 ug/l  
RT: 2.319 min Scan# 202  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27Tgt Ion:101 Resp: 1166  
Ion Ratio Lower Upper  
101 100  
85 47.3 38.6 58.0  
151 73.1 55.2 82.8

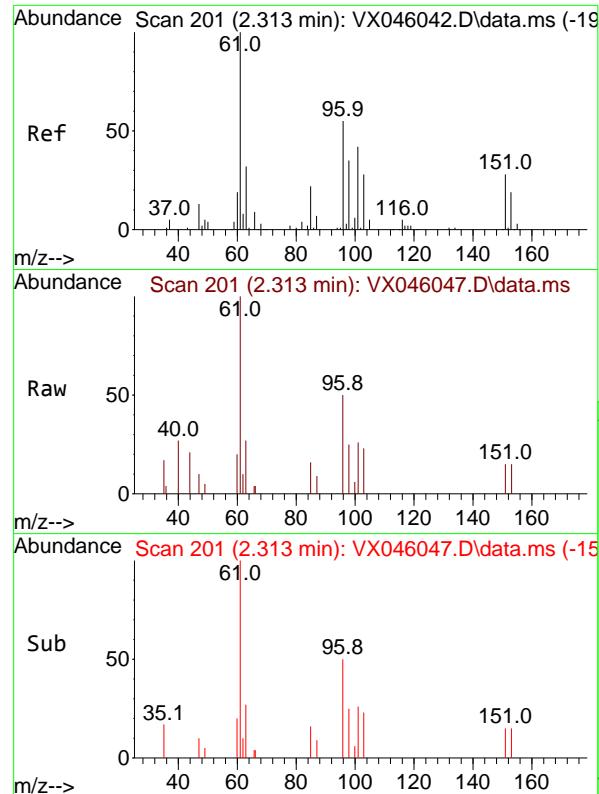

#12

1,1-Dichloroethene

Concen: 0.704 ug/l

RT: 2.313 min Scan# 201

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

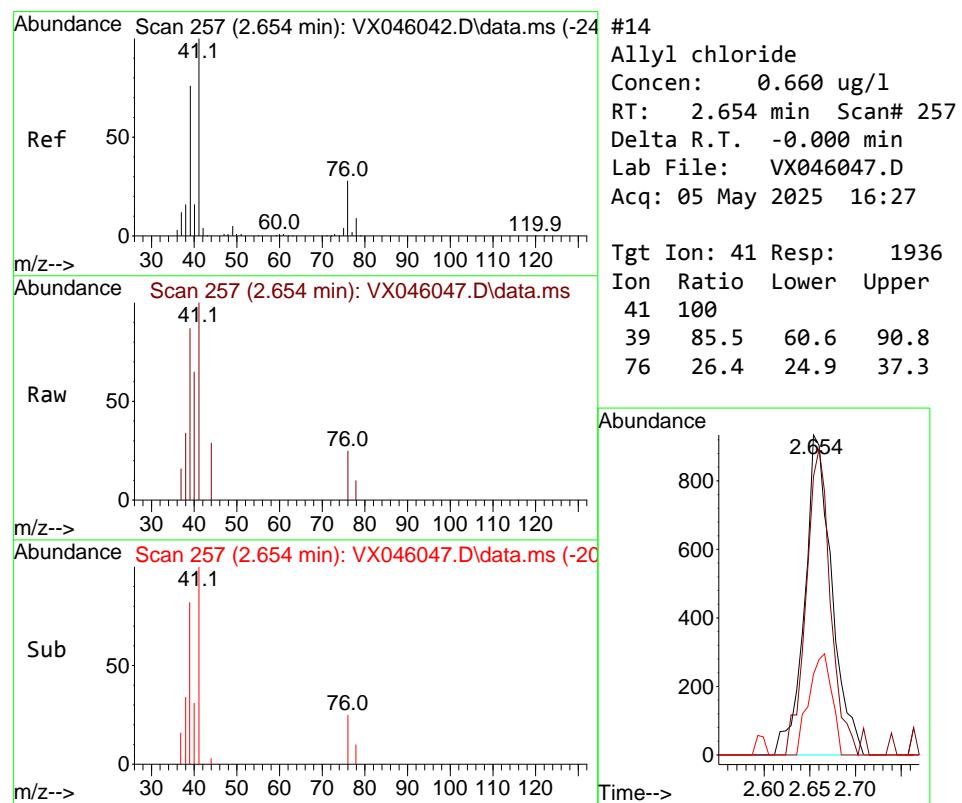

#14

Allyl chloride

Concen: 0.660 ug/l

RT: 2.654 min Scan# 257


Delta R.T. -0.000 min







Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion: 41 Resp: 1936

Ion	Ratio	Lower	Upper
41	100		
39	85.5	60.6	90.8
76	26.4	24.9	37.3

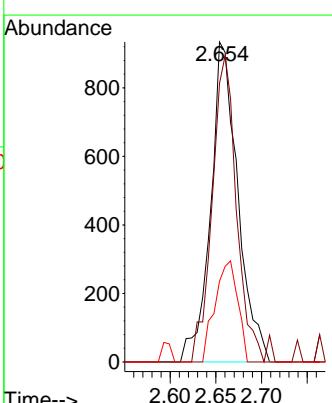

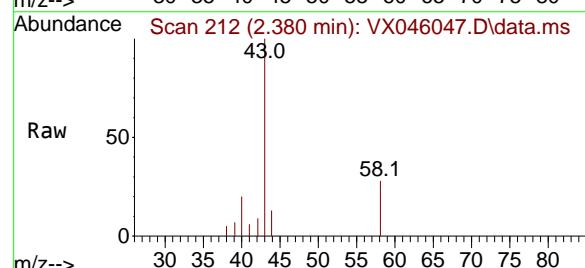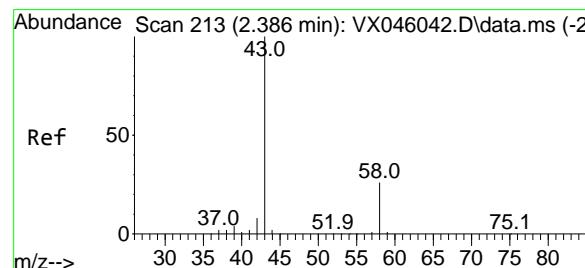

#15

**Acrylonitrile**

Concen: 3.424 ug/l

RT: 3.075 min Scan# 3

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X

ClientSampleId :

VSTDICC001


**Manual Integrations****APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

**Abundance**

3.075

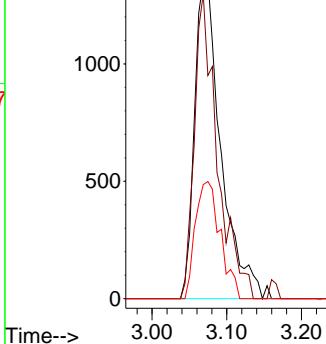

#16

**Acetone**

Concen: 3.736 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion: 43 Resp: 3500


Ion Ratio Lower Upper


43 100

58 28.1 21.2 31.8



**Abundance**

2.380

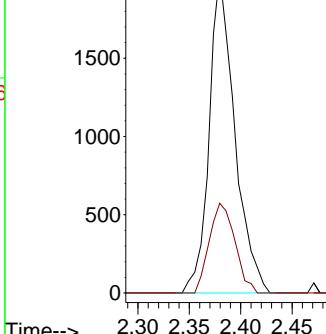




Abundance Scan 233 (2.508 min): VX046047.D\data.ms

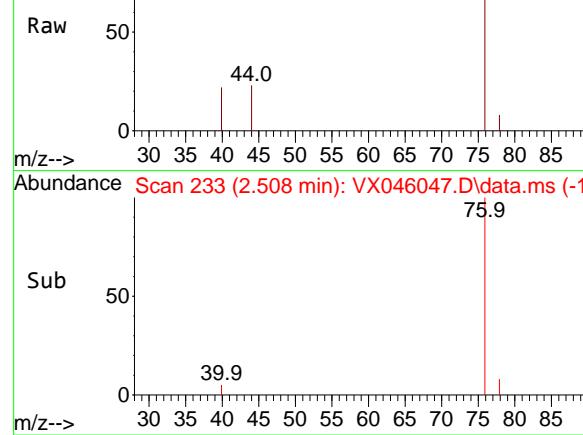

Abundance Scan 266 (2.709 min): VX046047.D\data.ms

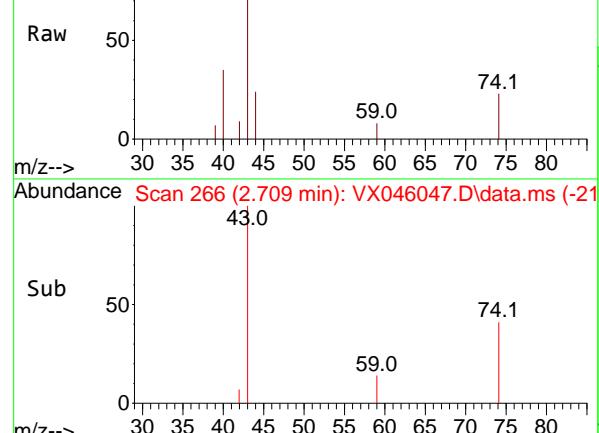

#17

Carbon Disulfide

Concen: 0.728 ug/l

RT: 2.508 min Scan# 2619

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations****APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

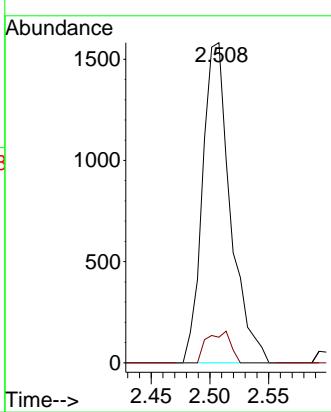

#18

Methyl Acetate

Concen: 0.828 ug/l

RT: 2.709 min Scan# 266

Delta R.T. 0.006 min

Lab File: VX046047.D


Acq: 05 May 2025 16:27







Tgt Ion: 43 Resp: 1852

Ion Ratio Lower Upper

43 100

74 22.0 16.7 25.1

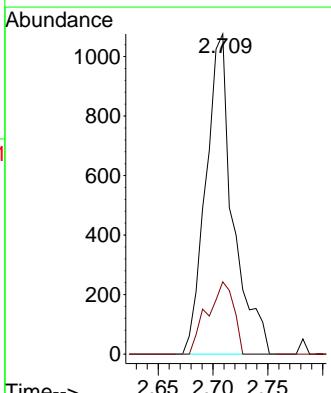




#19

Methyl tert-butyl Ether  
Concen: 0.662 ug/l  
RT: 3.117 min Scan# 3  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025




#20

Methylene Chloride  
Concen: 0.828 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion: 84 Resp: 1571  
Ion Ratio Lower Upper  
84 100  
49 140.0 113.9 170.9  
51 51.3 33.5 50.3#  
86 85.2 53.8 80.8#




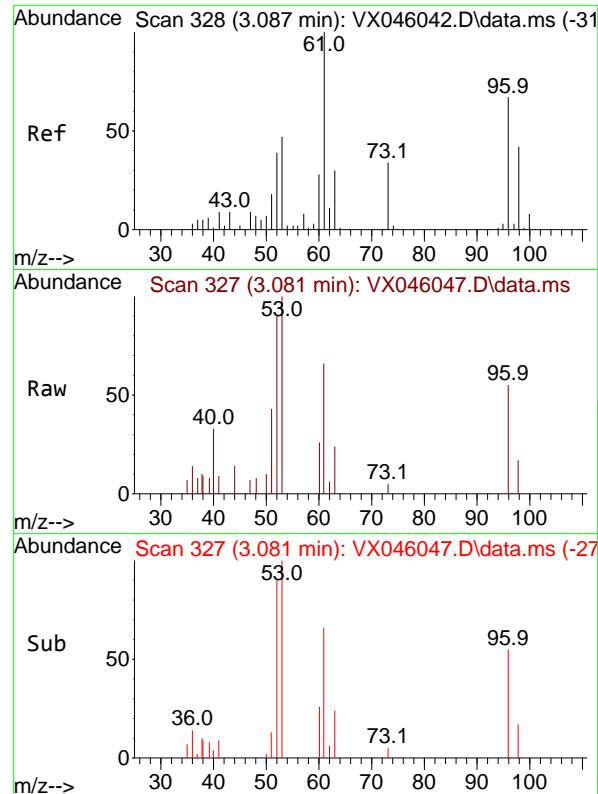


#21  
 trans-1,2-Dichloroethene  
 Concen: 0.701 ug/l  
 RT: 3.081 min Scan# 3  
 Delta R.T. -0.006 min  
 Lab File: VX046047.D  
 Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
 ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

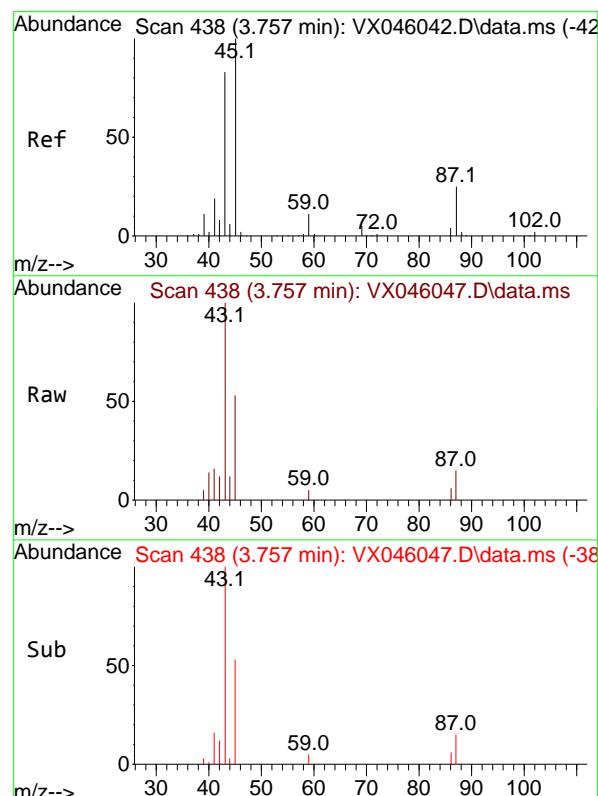

#22  
 Diisopropyl ether  
 Concen: 0.703 ug/l  
 RT: 3.757 min Scan# 438  
 Delta R.T. -0.000 min  
 Lab File: VX046047.D  
 Acq: 05 May 2025 16:27

Tgt Ion: 45 Resp: 3857  
 Ion Ratio Lower Upper  
 45 100  
 43 176.2 66.6 100.0#  
 87 28.9 19.8 29.6  
 59 9.1 8.6 12.8



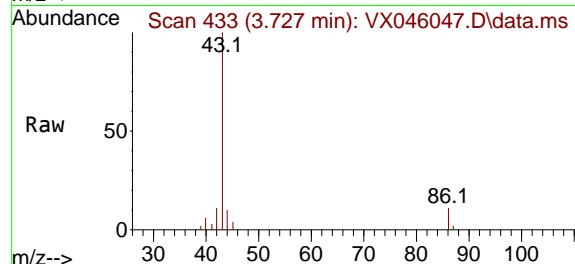

#23

**Vinyl Acetate**

Concen: 3.154 ug/l

RT: 3.727 min Scan# 413

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

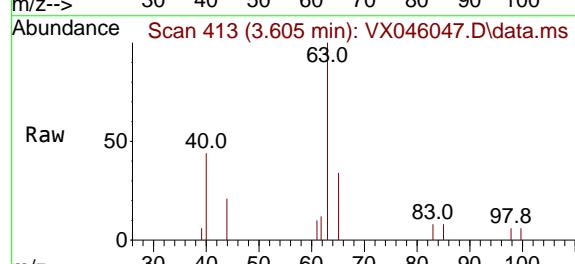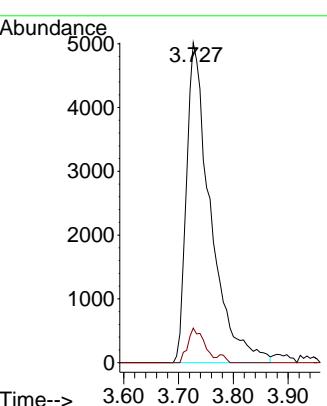

#24

**1,1-Dichloroethane**

Concen: 0.637 ug/l

RT: 3.605 min Scan# 413


Delta R.T. -0.000 min


Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion: 63 Resp: 2054


Ion	Ratio	Lower	Upper
63	100		
98	6.3	3.6	10.8
100	5.8	2.1	6.3

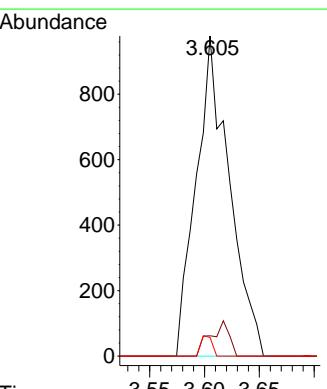

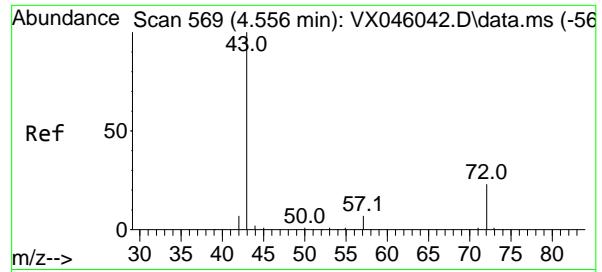

#25  
2-Butanone  
Concen: 3.371 ug/l  
RT: 4.593 min Scan# 5  
Delta R.T. 0.037 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001




Tgt Ion: 43 Resp: 4555  
Ion Ratio Lower Upper  
43 100  
72 19.2 18.4 27.6

Manual Integrations  
APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

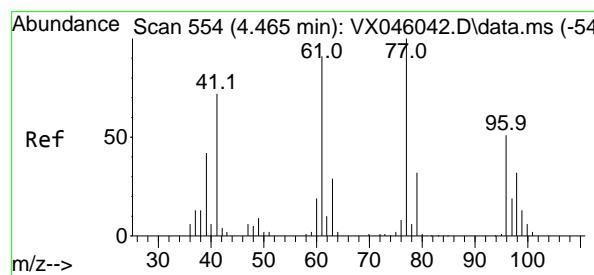
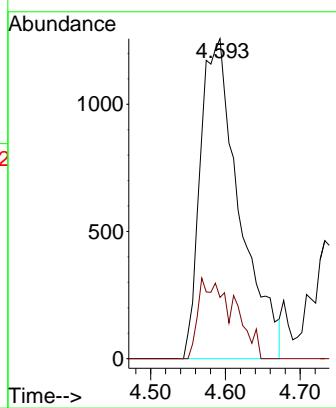



#26  
2,2-Dichloropropane  
Concen: 0.728 ug/l  
RT: 4.458 min Scan# 553  
Delta R.T. -0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

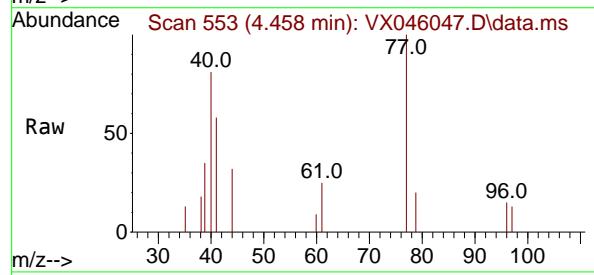

Tgt Ion: 77 Resp: 1777  
Ion Ratio Lower Upper  
77 100  
97 13.7 10.5 31.5

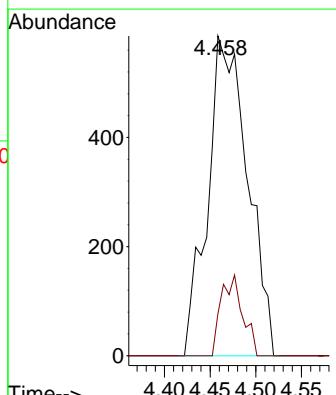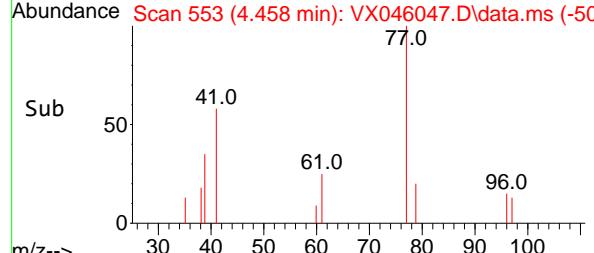





#27  
cis-1,2-Dichloroethene  
Concen: 0.693 ug/l  
RT: 4.483 min Scan# 557  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27


Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

### Manual Integrations APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

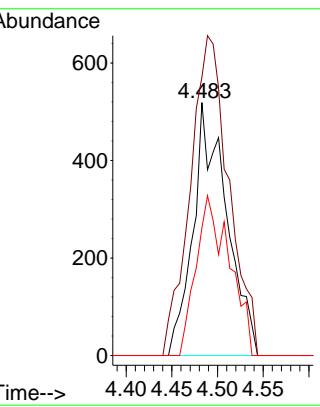


#28  
Bromochloromethane  
Concen: 0.619 ug/l m  
RT: 4.910 min Scan# 627  
Delta R.T. 0.012 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27



Tgt Ion: 49 Resp: 1061  
Ion Ratio Lower Upper  
49 100  
129 0.0 0.0 4.0  
130 65.3 56.2 84.2

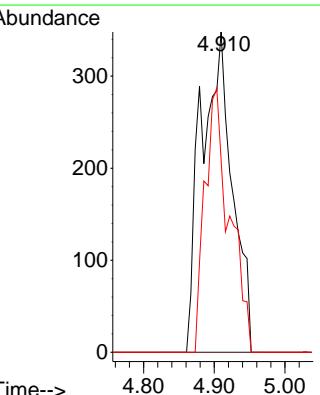

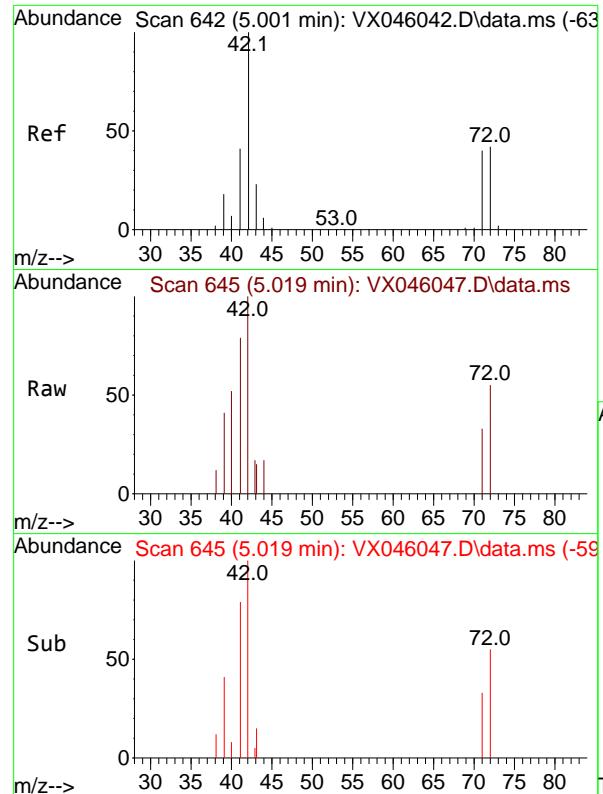

#29

Tetrahydrofuran

Concen: 3.338 ug/l

RT: 5.019 min Scan# 6

Delta R.T. 0.018 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

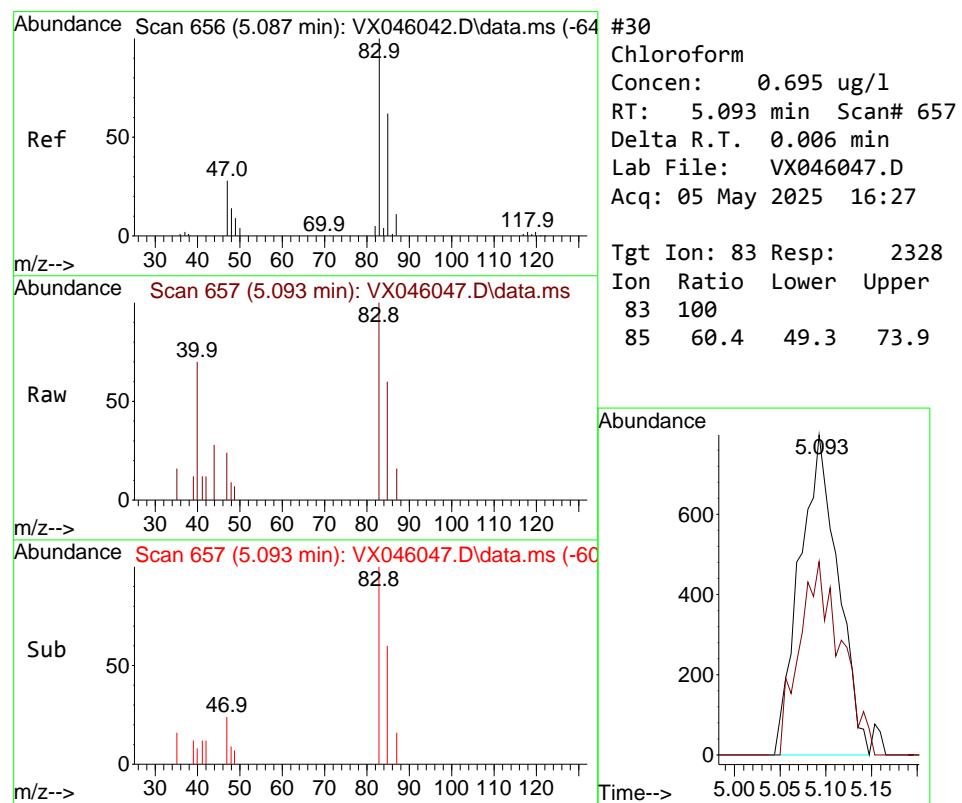

#30

Chloroform

Concen: 0.695 ug/l

RT: 5.093 min Scan# 657


Delta R.T. 0.006 min


Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion: 83 Resp: 2328

Ion	Ratio	Lower	Upper
83	100		
85	60.4	49.3	73.9

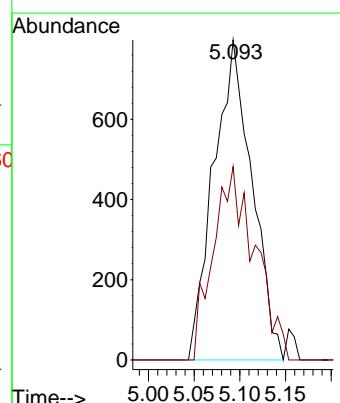


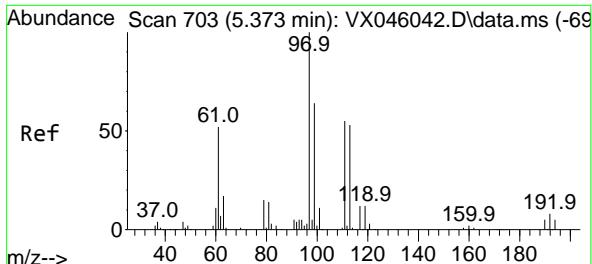

#32  
1,1,1-Trichloroethane  
Concen: 0.647 ug/l  
RT: 5.379 min Scan# 7  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDICC001



Abundance Scan 704 (5.379 min): VX046047.D\data.ms

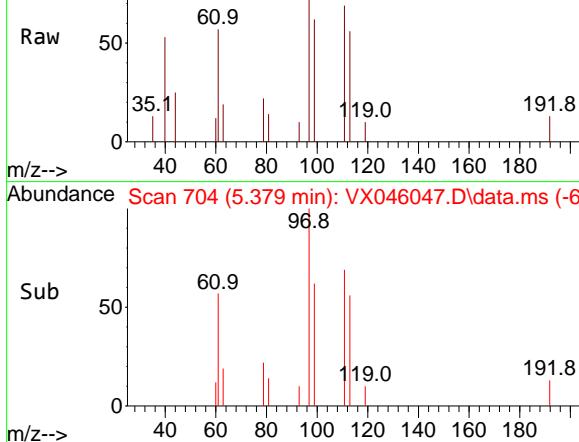

Tgt	Ion:	97	Resp:	1869
Ion	Ratio		Lower	Upper
97	100			
99	0.0	51.8	77.6	
61	55.0	40.1	60.1	

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

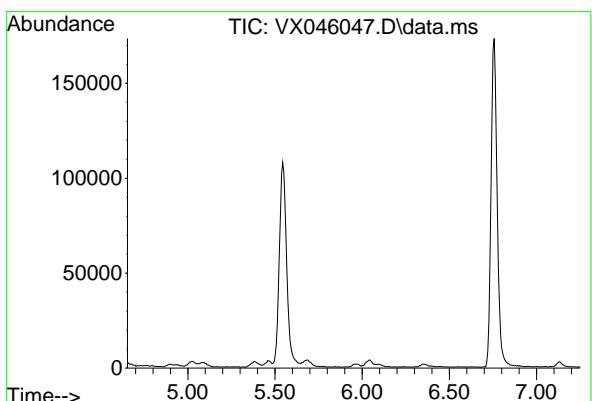
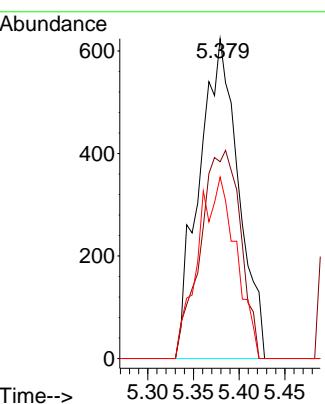



#33  
1,2-Dichloroethane-d4  
Concen: 0.000 ug/l  
Expected RT: 5.95 min

Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion: 65  
Sig Exp Ratio  
65 100  
67 49.5

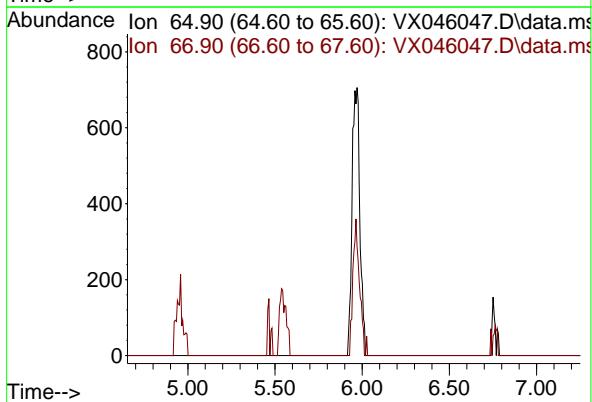

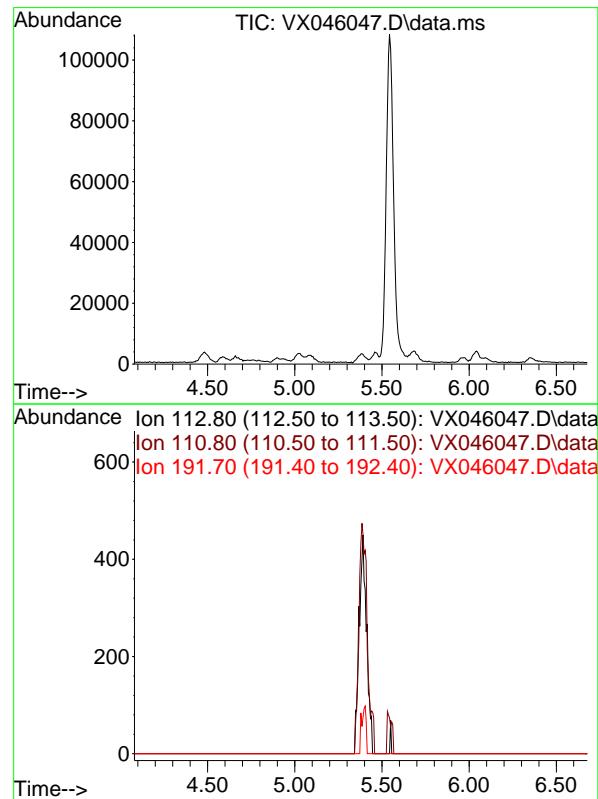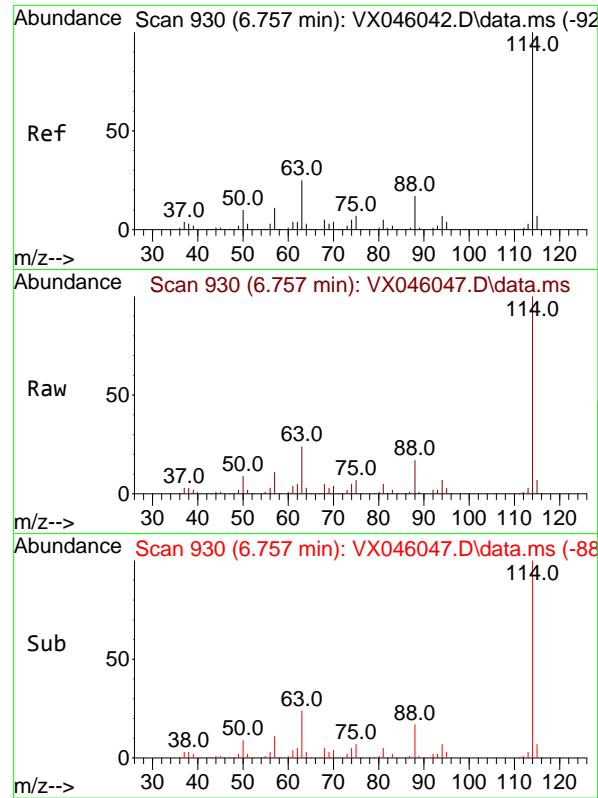




#36

1,1-Dichloropropene  
Concen: 0.758 ug/l  
RT: 5.684 min Scan# 74  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27




Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

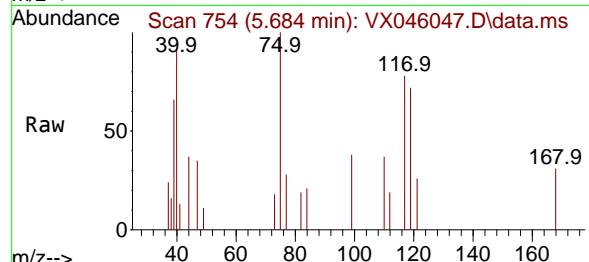


Tgt Ion: 75 Resp: 1643  
Ion Ratio Lower Upper  
75 100  
110 28.2 16.3 48.9  
77 15.8 24.3 36.5

### Manual Integrations APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025






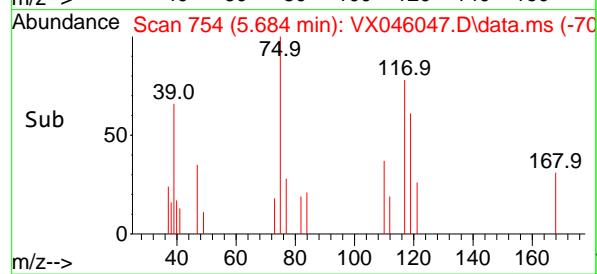


#37  
Ethyl Acetate  
Concen: 0.717 ug/l m  
RT: 4.733 min Scan# 598  
Delta R.T. 0.018 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27



Tgt Ion: 43 Resp: 1956  
Ion Ratio Lower Upper  
43 100  
61 0.0 10.3 15.5#  
70 1.0 7.9 11.9#



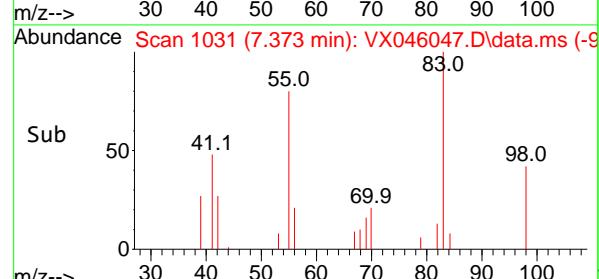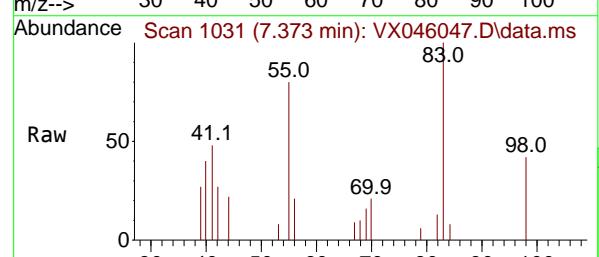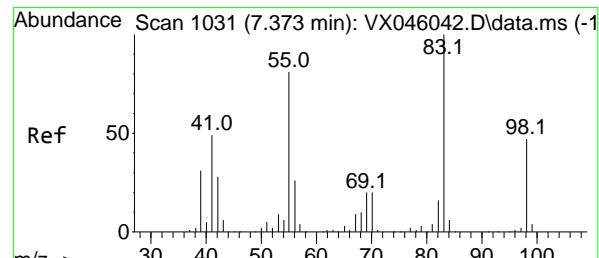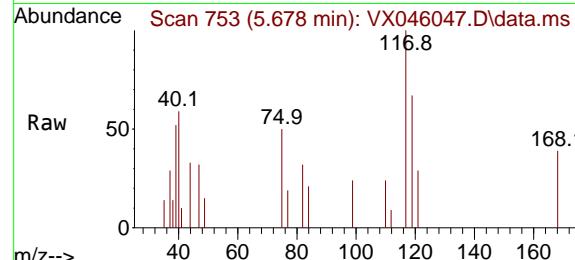

#38

Carbon Tetrachloride

Concen: 0.724 ug/l

RT: 5.678 min Scan# 7

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#39

Methylcyclohexane

Concen: 0.770 ug/l


RT: 7.373 min Scan# 1031




Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt	Ion:	83	Resp:	2096
Ion	Ratio	Lower	Upper	
83	100			
55	80.1	64.7	97.1	
98	41.9	37.4	56.2	

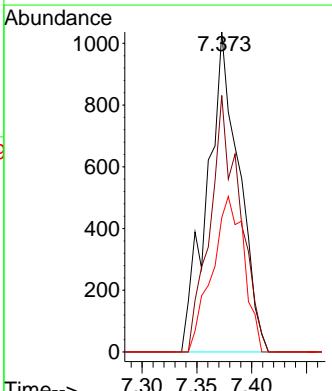

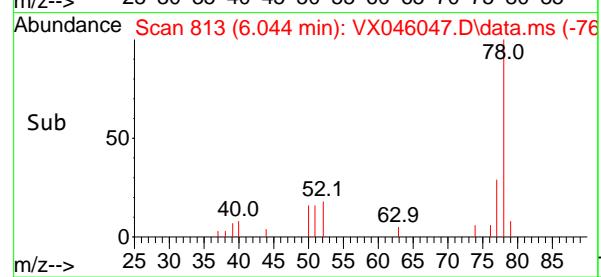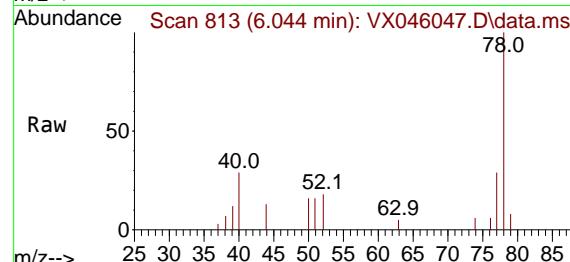

#40

Benzene

Concen: 0.668 ug/l

RT: 6.044 min Scan# 8

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

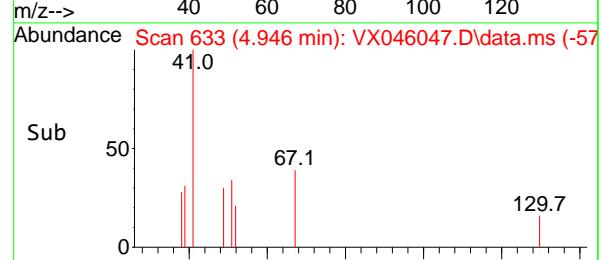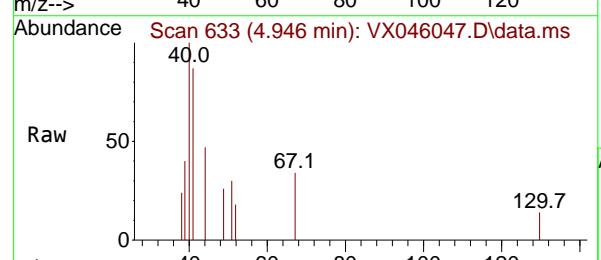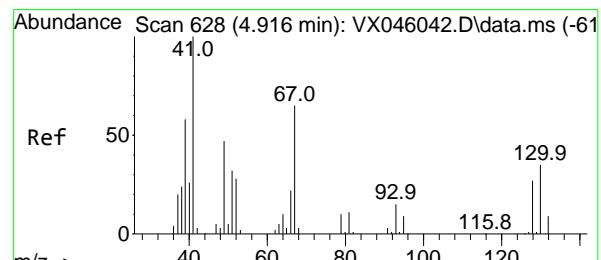

#41

Methacrylonitrile

Concen: 0.513 ug/l

RT: 4.946 min Scan# 633

Delta R.T. 0.030 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion: 41 Resp: 778


Ion Ratio Lower Upper







41 100

39 51.7 47.2 70.8

67 0.0 50.7 76.1#

52 13.6 24.6 37.0#

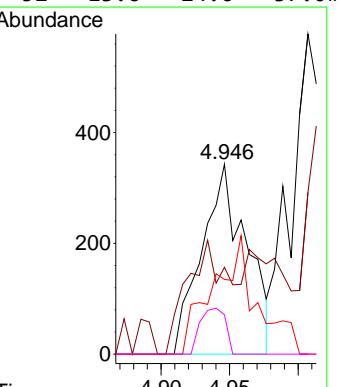



#42

1,2-Dichloroethane

Concen: 0.694 ug/l

RT: 6.092 min Scan# 8

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#43

Isopropyl Acetate

Concen: 0.612 ug/l

RT: 6.354 min Scan# 864

Delta R.T. 0.018 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27


Tgt Ion: 43 Resp: 2553


Ion Ratio Lower Upper

43 100

61 10.7 14.3 21.5#

87 3.2 9.5 14.3#

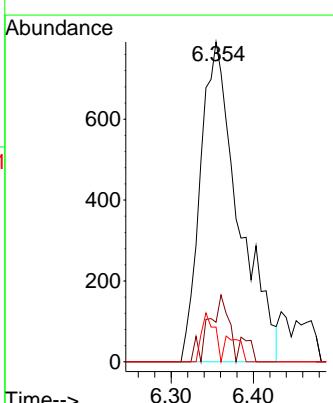

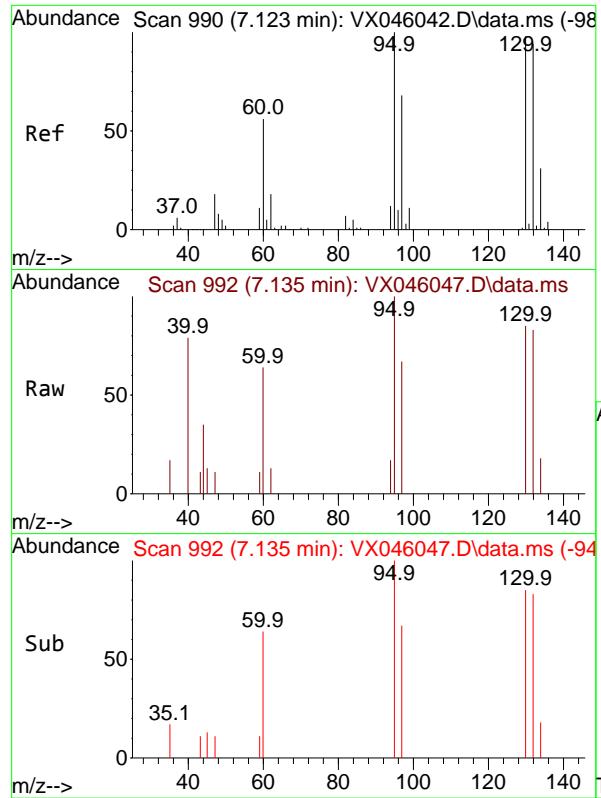

#44

Trichloroethene

Concen: 0.680 ug/l

RT: 7.135 min Scan# 990

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

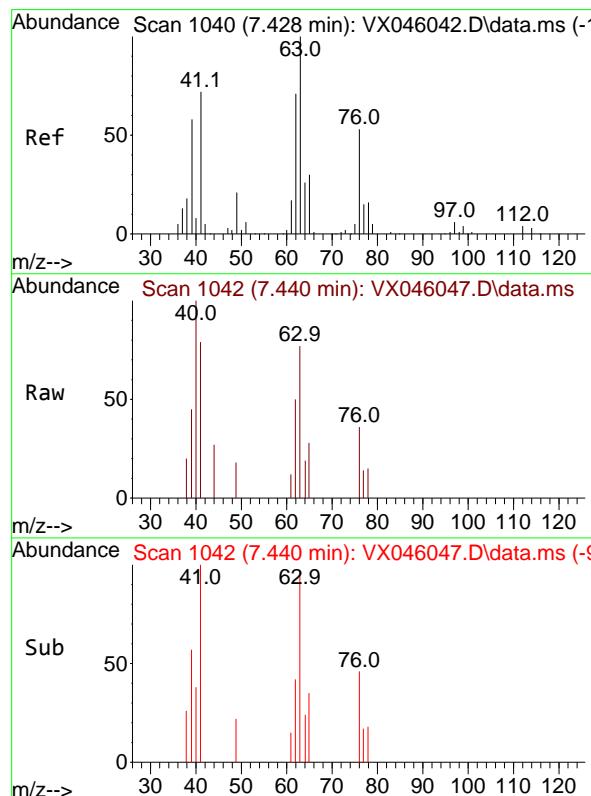

#45

1,2-Dichloropropane

Concen: 0.633 ug/l

RT: 7.440 min Scan# 1042


Delta R.T. 0.012 min







Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion: 63 Resp: 1059

Ion	Ratio	Lower	Upper
63	100		
65	36.1	24.1	36.1

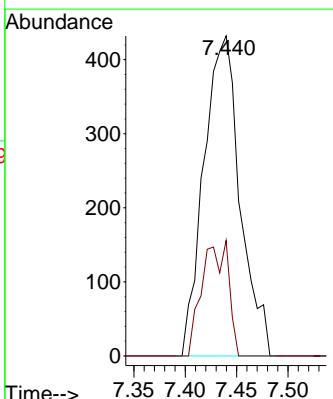

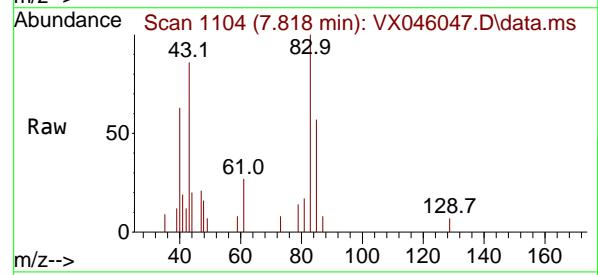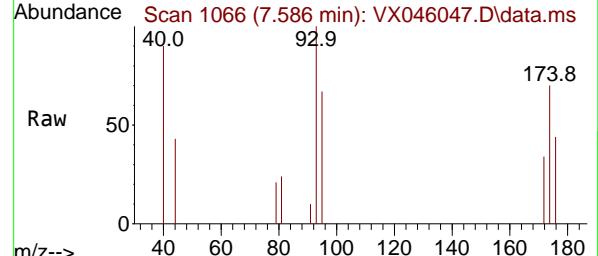

#46

Dibromomethane

Concen: 0.667 ug/l

RT: 7.586 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#47

Bromodichloromethane

Concen: 0.633 ug/l

RT: 7.818 min Scan# 1104

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27


Tgt Ion: 83 Resp: 1620







Ion Ratio Lower Upper

83 100

85 57.3 50.5 75.7

127 0.0 6.5 9.7#

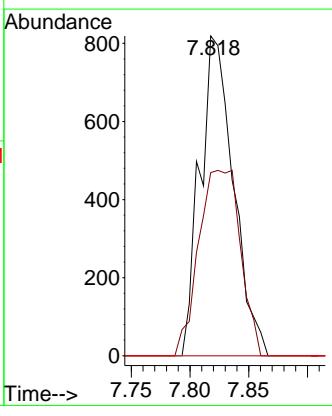

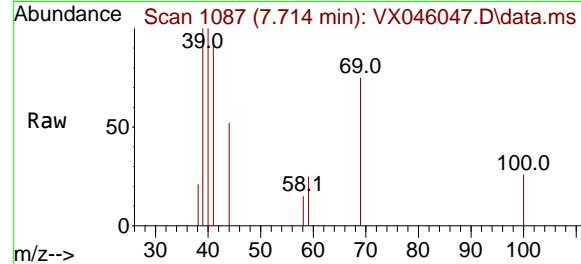

#48

Methyl methacrylate

Concen: 0.577 ug/l m

RT: 7.714 min Scan# 1081

Delta R.T. 0.024 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

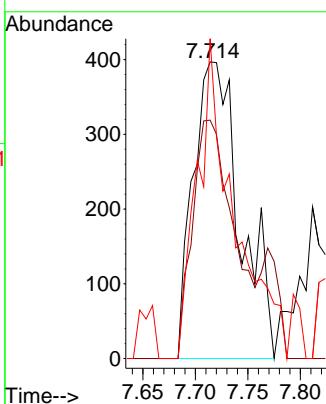

#49

1,4-Dioxane

Concen: 11.703 ug/l

RT: 7.677 min Scan# 1081

Delta R.T. 0.018 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27


Tgt Ion: 88 Resp: 498






Ion Ratio Lower Upper

88 100

43 44.4 33.4 50.2

58 30.3 58.6 88.0#

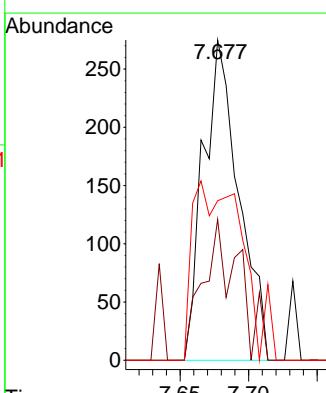

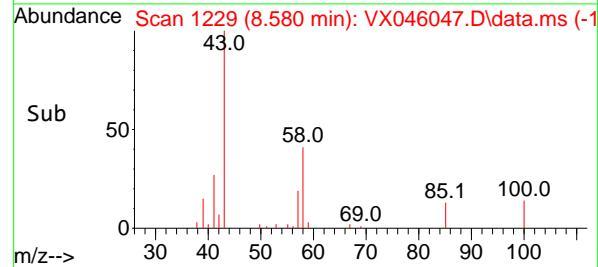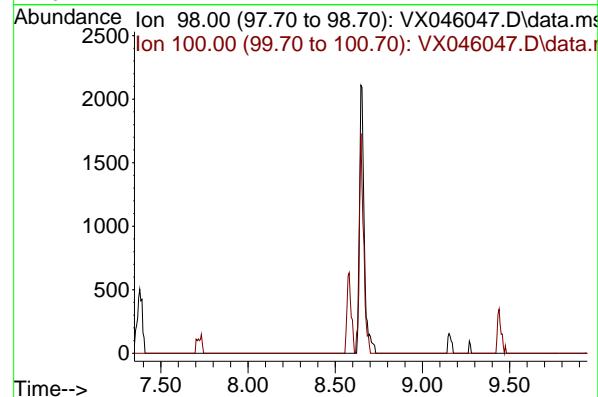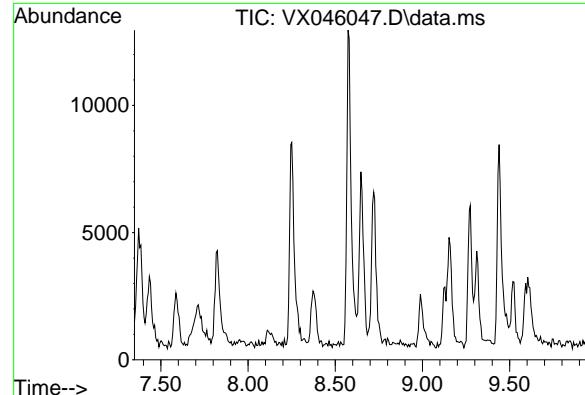

#50  
Toluene-d8  
Concen: 0.000 ug/l  
Expected RT: 8.65 min  
  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27  
  
Tgt Ion: 98  
Sig Exp Ratio  
98 100  
100 66.9


Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDICC001




Manual Integrations  
APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

#51  
4-Methyl-2-Pentanone  
Concen: 3.430 ug/l  
RT: 8.580 min Scan# 1229  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion: 43 Resp: 9378  
Ion Ratio Lower Upper  
43 100  
58 34.4 28.9 43.3

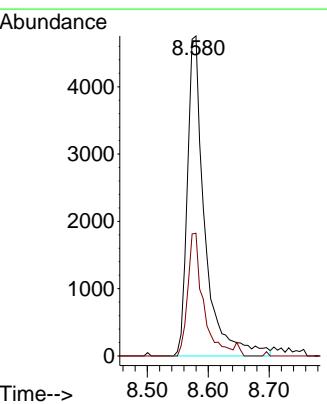







#52  
Toluene  
Concen: 0.672 ug/l  
RT: 8.720 min Scan# 1252  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


### Manual Integrations APPROVED







Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#53  
t-1,3-Dichloropropene  
Concen: 0.576 ug/l  
RT: 8.988 min Scan# 1296  
Delta R.T. 0.012 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion: 75 Resp: 1238  
Ion Ratio Lower Upper  
75 100  
77 42.7 25.0 37.6#



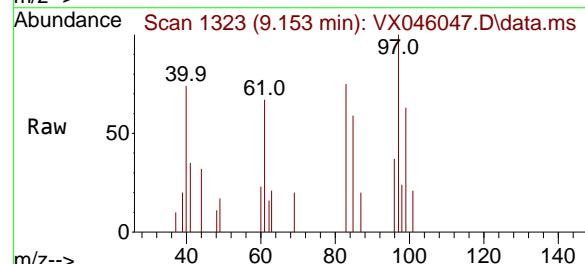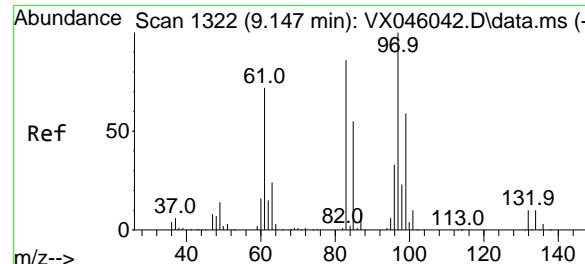

#54

cis-1,3-Dichloropropene

Concen: 0.564 ug/l

RT: 8.379 min Scan# 1

Delta R.T. 0.018 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#55

1,1,2-Trichloroethane

Concen: 0.637 ug/l


RT: 9.153 min Scan# 1323




Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt	Ion	Resp:	1029
Ion	Ratio	Lower	Upper
97	100		
83	74.8	69.0	103.6
85	59.5	44.3	66.5
99	63.0	47.8	71.6

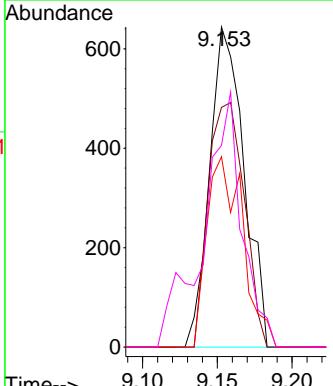



#56

Ethyl methacrylate

Concen: 0.504 ug/l

RT: 9.128 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

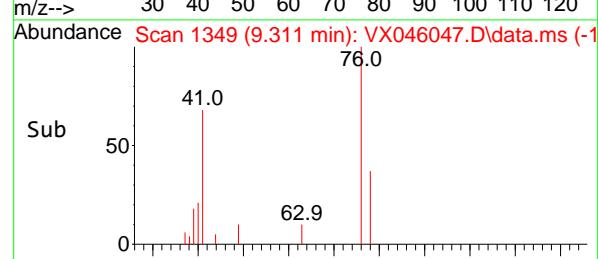

#57

1,3-Dichloropropane

Concen: 0.711 ug/l


RT: 9.311 min Scan# 1349




Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt	Ion	Resp:	2036
Ion	Ratio	Lower	Upper
76	100		
78	31.4	26.3	39.5

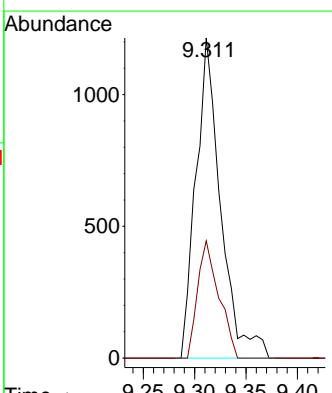

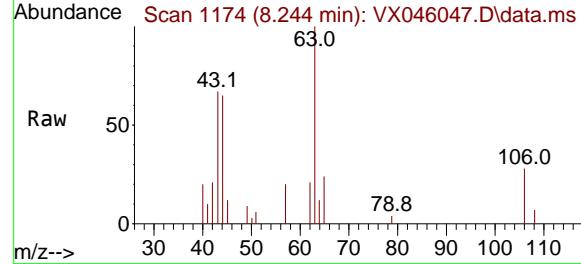

#58

2-Chloroethyl Vinyl ether

Concen: 3.420 ug/l

RT: 8.244 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#59

2-Hexanone

Concen: 3.096 ug/l


RT: 9.439 min Scan# 1370

Delta R.T. 0.012 min


Lab File: VX046047.D




Acq: 05 May 2025 16:27

Tgt	Ion	Resp:	6424
Ion	Ratio	Lower	Upper
43	100		
58	41.6	24.9	74.6

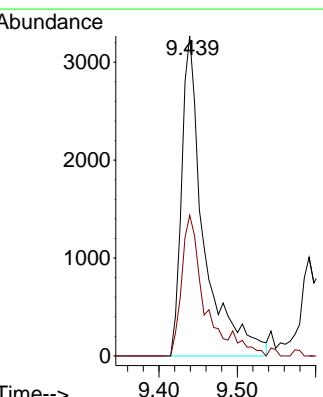

Abundance Scan 1370 (9.439 min): VX046047.D\data.ms (-1)

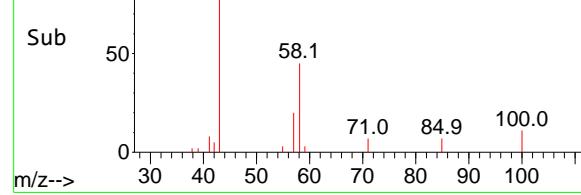

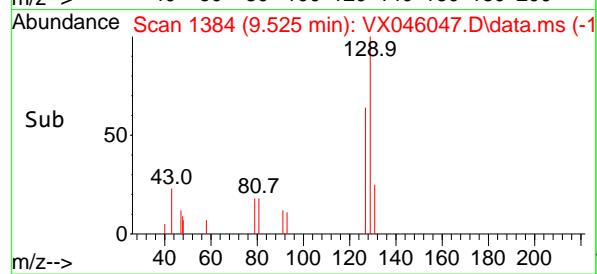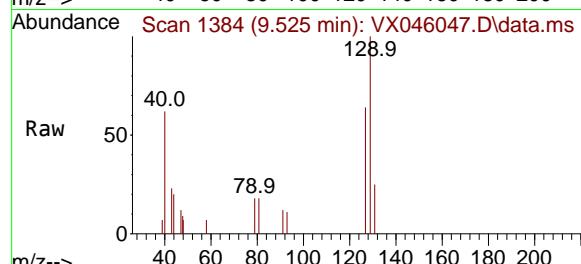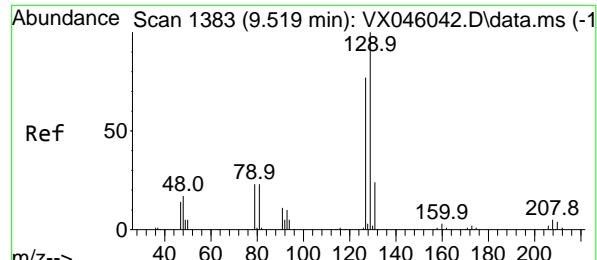





#60

Dibromochloromethane  
Concen: 0.582 ug/l  
RT: 9.525 min Scan# 1383  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

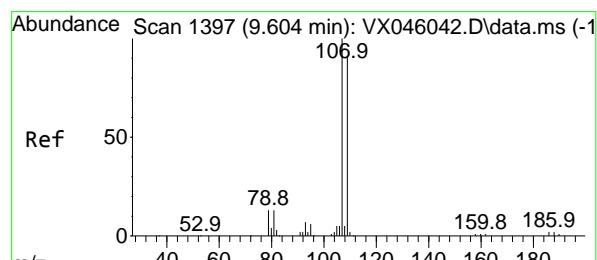


#61

1,2-Dibromoethane  
Concen: 0.650 ug/l  
RT: 9.610 min Scan# 1398  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion:107 Resp: 1077  
Ion Ratio Lower Upper  
107 100  
109 94.0 73.3 109.9

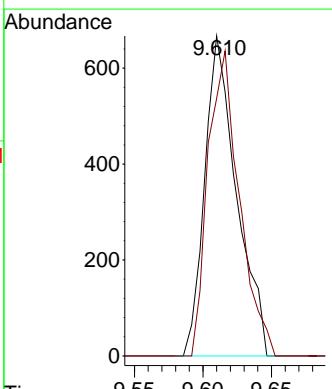


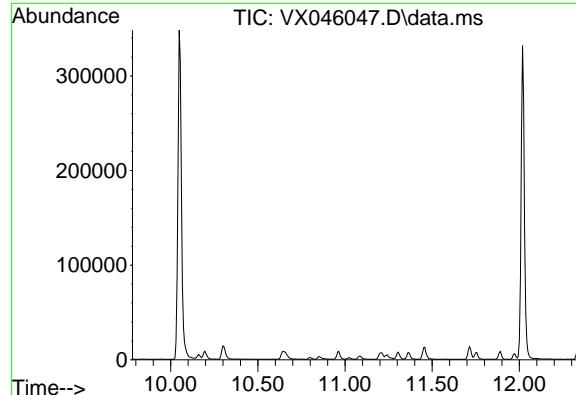


#62  
4-Bromofluorobenzene  
Concen: 0.000 ug/l  
Expected RT: 11.08 min  
  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27  
  
Tgt Ion: 95  
Sig Exp Ratio  
95 100  
174 67.9  
176 65.7

Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDICC001

**Manual Integrations**  
**APPROVED**



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025


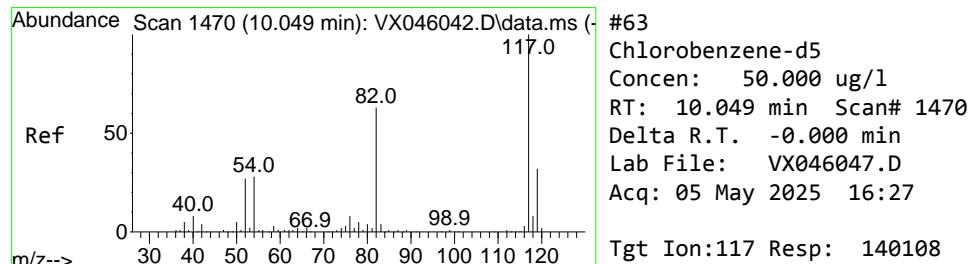
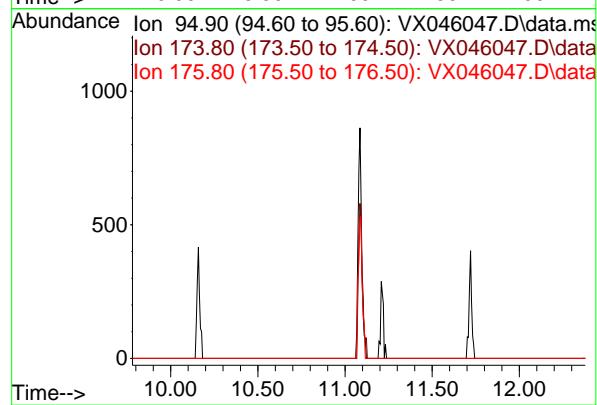


Abundance

Scan 1470 (10.049 min): VX046047.D\data.ms

Tgt Ion:	117	Resp:	140108
Ion	Ratio	Lower	Upper
117	100		
82	61.0	50.6	76.0
119	32.1	25.8	38.6

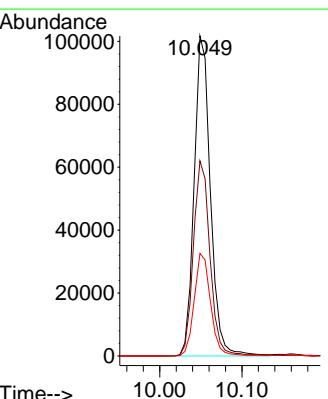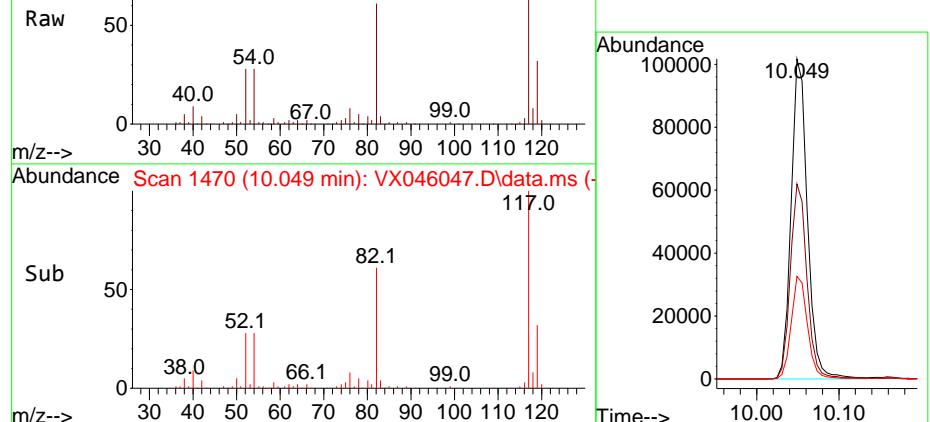



#64

Tetrachloroethene

Concen: 0.679 ug/l

RT: 9.275 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X

ClientSampleId :




VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Abundance

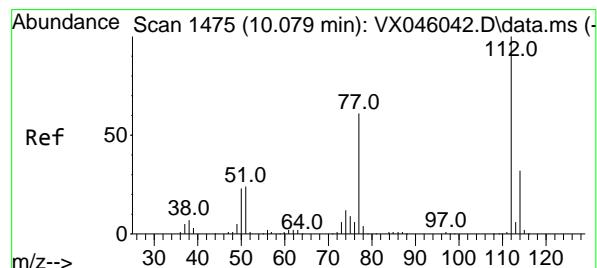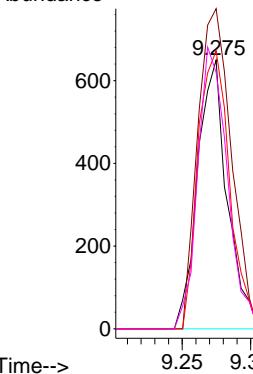

#65

Chlorobenzene

Concen: 0.735 ug/l

RT: 10.079 min Scan# 1475

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27



Tgt Ion:112 Resp: 3170


Ion Ratio Lower Upper

112 100

114 30.6 25.4 38.2

Abundance

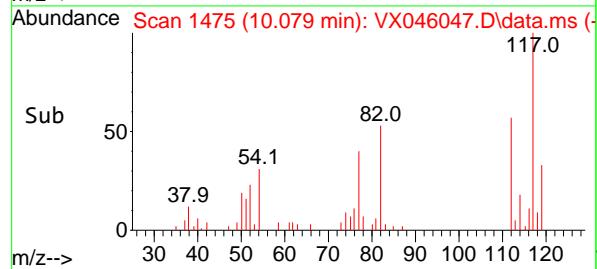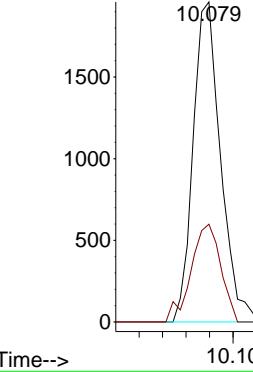



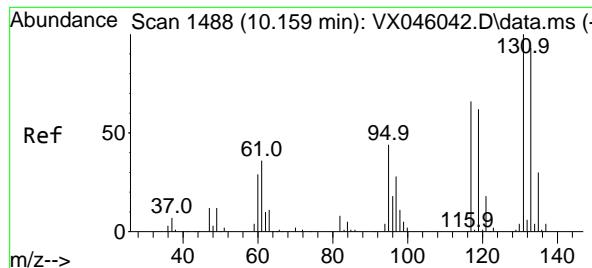


#66  
1,1,1,2-Tetrachloroethane  
Concen: 0.720 ug/l  
RT: 10.159 min Scan# 14  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27


RT: 10.159 min Scan# 1 Instrument :  
Delta R.T. -0.000 min MSVOA\_X  
Lab File: VX046047.D ClientSampleId :  
Acq: 05 May 2025 16:27 VSTDICC001

## Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

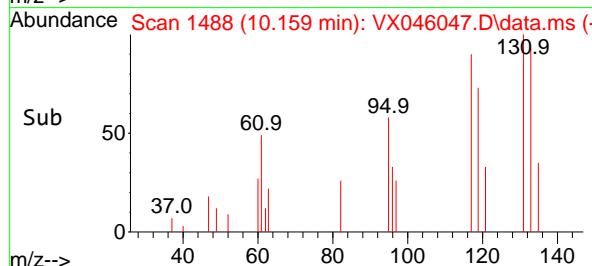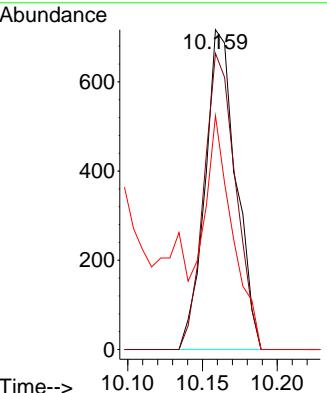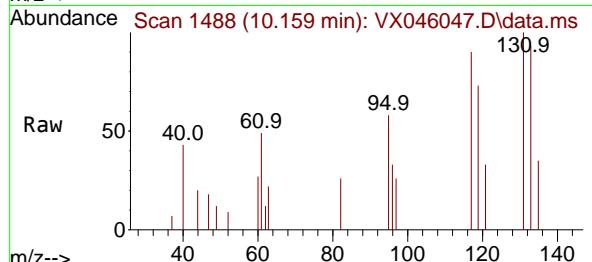




#67  
Ethyl Benzene  
Concen: 0.687 ug/l  
RT: 10.195 min Scan# 1494  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27



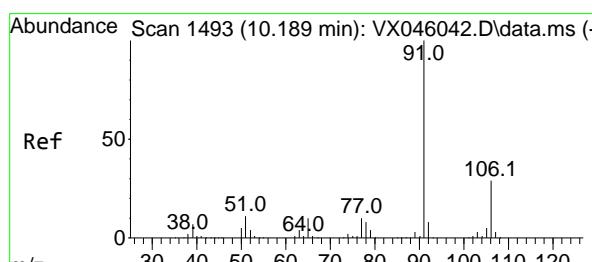


```

Tgt Ion: 91 Resp:      5052
Ion    Ratio   Lower   Upper
  91    100
  106   32.5    23.4    35.2

```


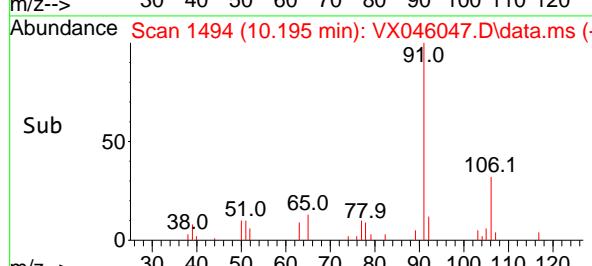
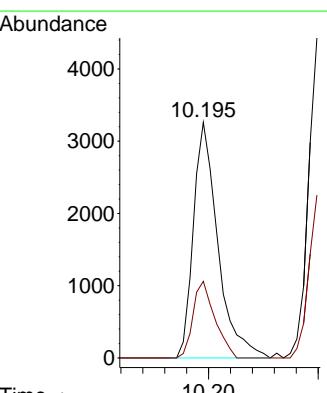
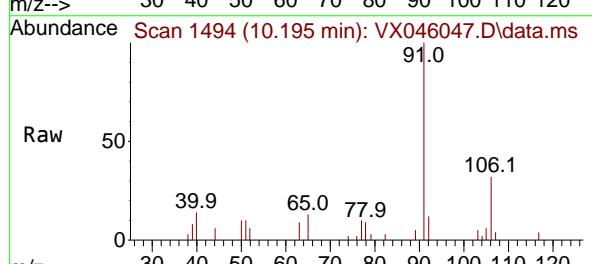




#68  
m/p-Xylenes  
Concen: 1.367 ug/l  
RT: 10.299 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27  
ClientSampleId : VSTDICC001


### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

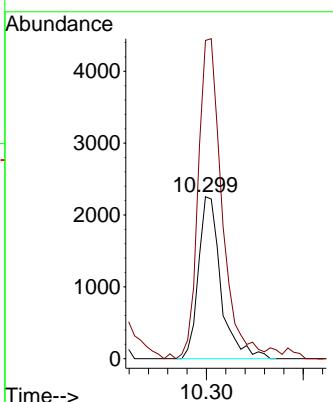

#69  
o-Xylene  
Concen: 0.672 ug/l  
RT: 10.640 min Scan# 1567  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion:106 Resp: 1799  
Ion Ratio Lower Upper  
106 100  
91 214.9 112.7 338.1

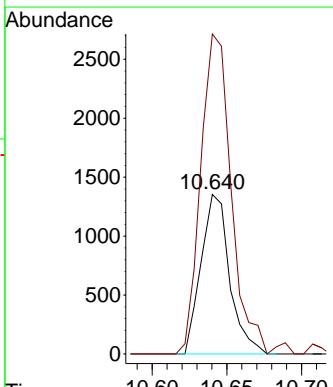


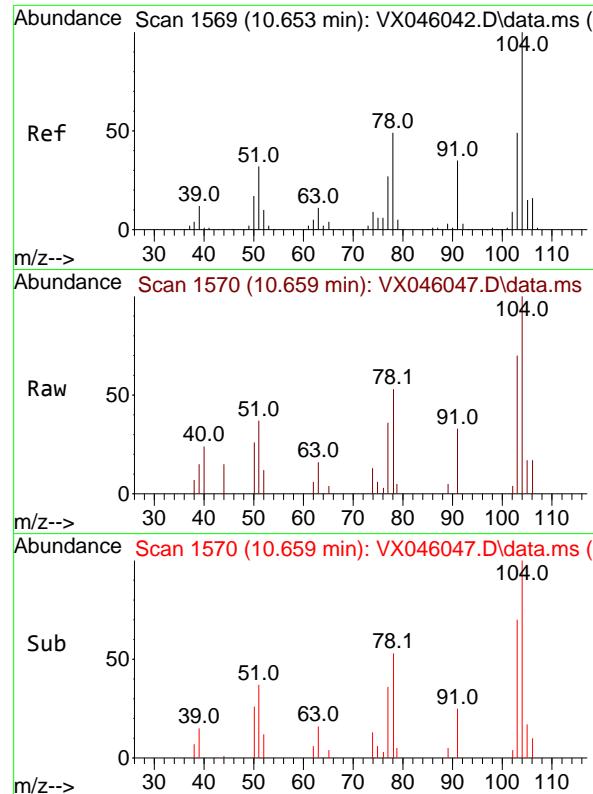


#70  
Styrene  
Concen: 0.622 ug/l  
RT: 10.659 min Scan# 1  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

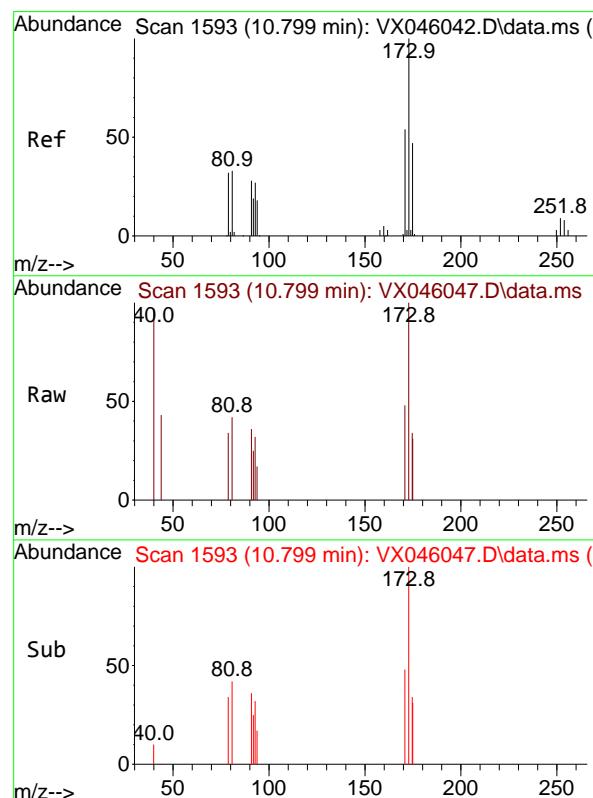

#71  
Bromoform  
Concen: 0.608 ug/l  
RT: 10.799 min Scan# 1593  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion:173 Resp: 657  
Ion Ratio Lower Upper  
173 100  
175 46.6 23.4 70.0  
254 0.0 0.0 0.0




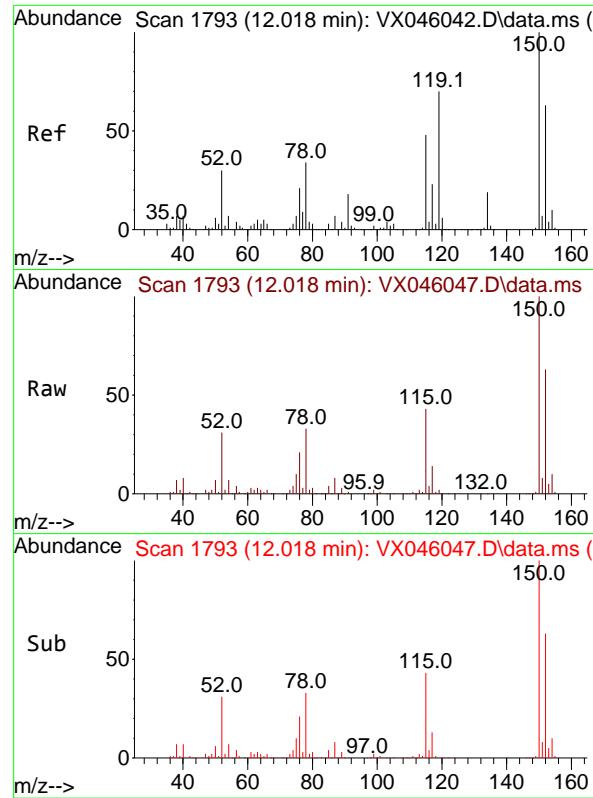


#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

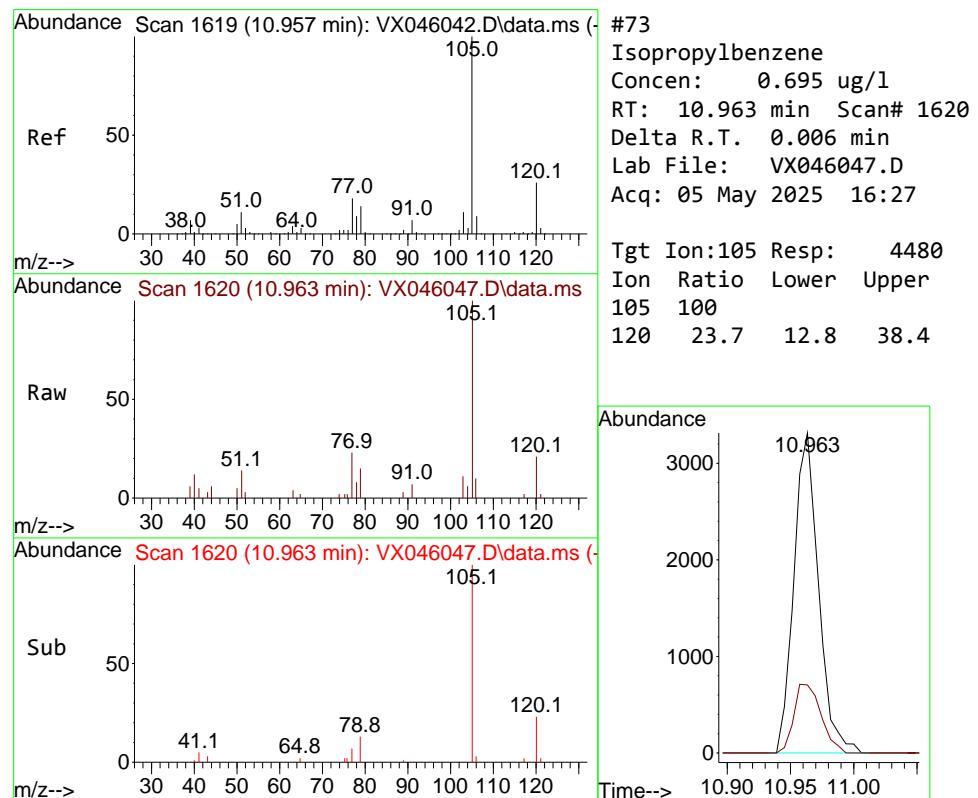

#73  
Isopropylbenzene  
Concen: 0.695 ug/l  
RT: 10.963 min Scan# 1620  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion:105 Resp: 4480  
Ion Ratio Lower Upper  
105 100  
120 23.7 12.8 38.4



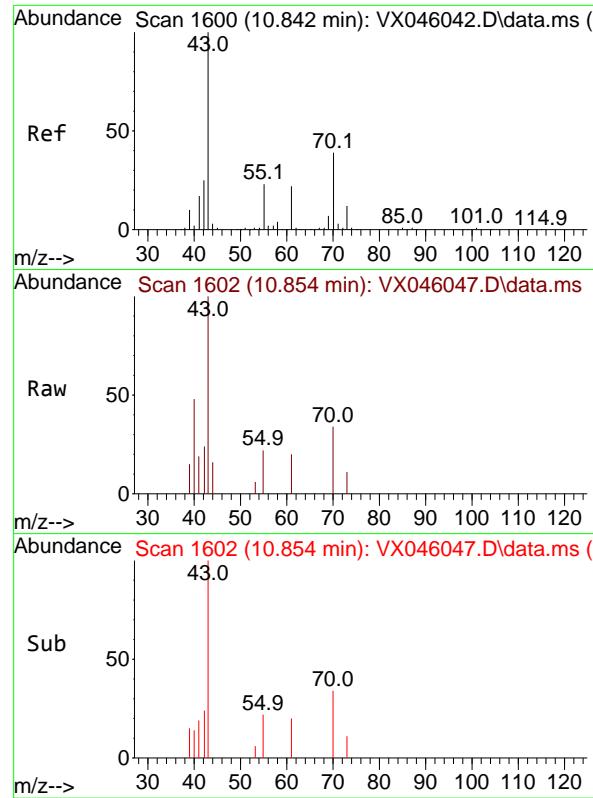

#74

N-amyl acetate

Concen: 0.631 ug/l

RT: 10.854 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X



ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

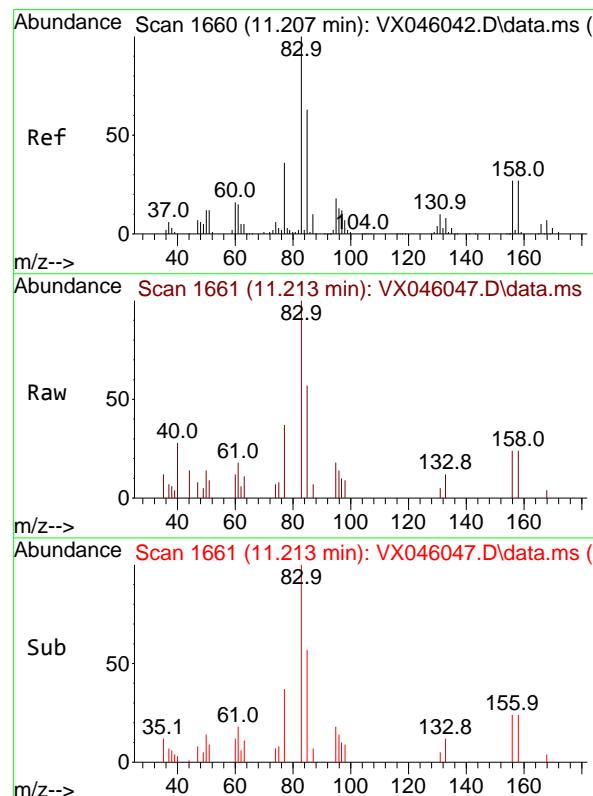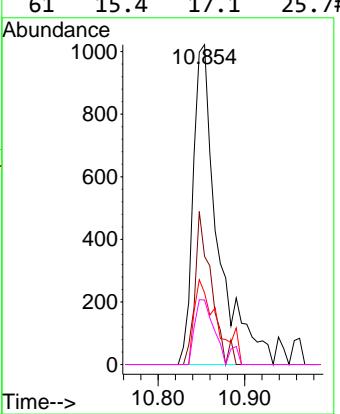

#75

1,1,2,2-Tetrachloroethane

Concen: 0.800 ug/l

RT: 11.213 min Scan# 1661

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27


Tgt Ion: 83 Resp: 1835




Ion Ratio Lower Upper

83 100

131 7.5 5.0 14.9

85 58.7 31.9 95.7

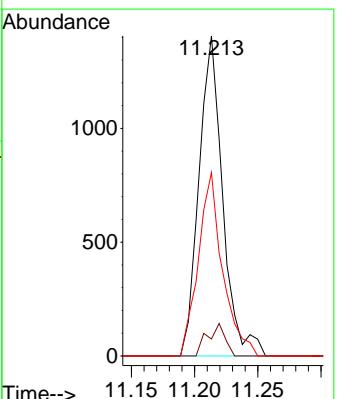

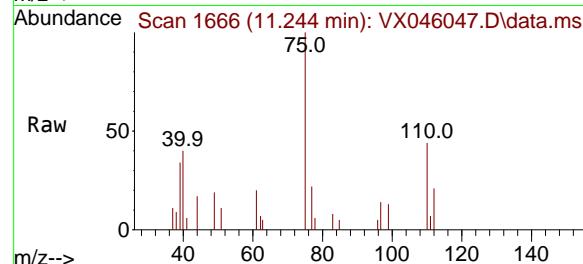

#76

1,2,3-Trichloropropane

Concen: 0.674 ug/l m

RT: 11.244 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#77

Bromobenzene

Concen: 0.734 ug/l

RT: 11.201 min Scan# 1659

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27


Tgt Ion:156 Resp: 1095

Ion Ratio Lower Upper




156 100

77 179.5 92.8 278.3

158 93.5 48.8 146.3

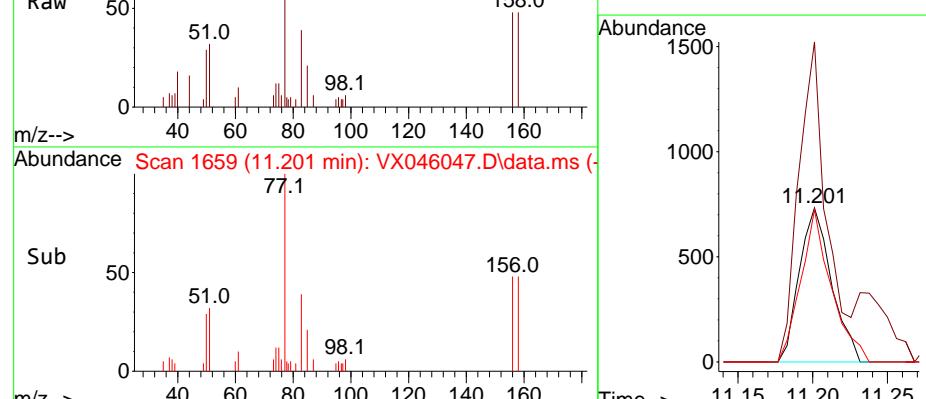

Time--&gt;

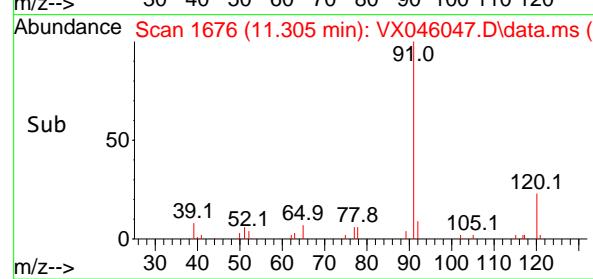

#78

n-propylbenzene

Concen: 0.699 ug/l

RT: 11.305 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#79

2-Chlorotoluene

Concen: 0.773 ug/l

RT: 11.360 min Scan# 1685

Delta R.T. -0.000 min

Lab File: VX046047.D


Acq: 05 May 2025 16:27




Tgt Ion: 91 Resp: 3765

Ion Ratio Lower Upper

91 100

126 28.0 15.6 46.7

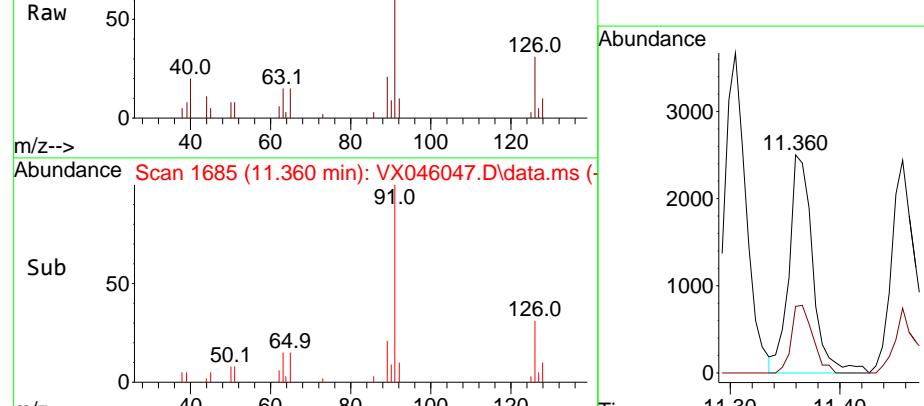







#80

1,3,5-Trimethylbenzene  
Concen: 0.671 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

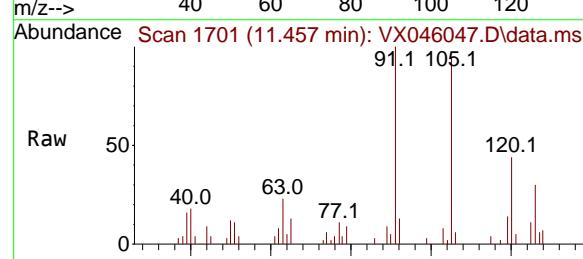

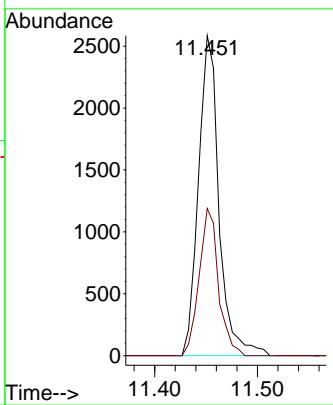


#82

4-Chlorotoluene  
Concen: 0.713 ug/l  
RT: 11.457 min Scan# 1701  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion: 91 Resp: 3815  
Ion Ratio Lower Upper  
91 100  
126 24.8 13.3 39.8





#83

tert-Butylbenzene

Concen: 0.751 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X




ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

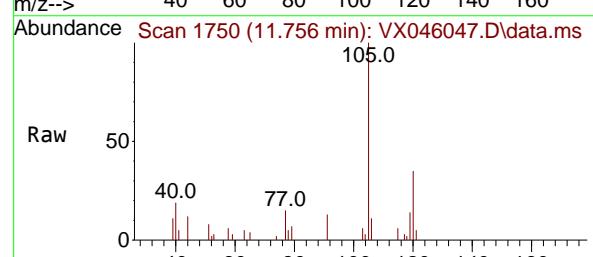

#84

1,2,4-Trimethylbenzene

Concen: 0.697 ug/l


RT: 11.756 min Scan# 1750

Delta R.T. 0.006 min




Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt	Ion:105	Resp:	3725
Ion	Ratio	Lower	Upper
105	100		
120	40.3	21.2	63.6



VX046047.D 82X050525W.M



#85

sec-Butylbenzene

Concen: 0.672 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X





ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

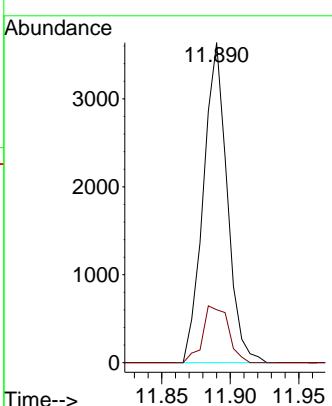

#86

p-Isopropyltoluene

Concen: 0.679 ug/l

RT: 12.006 min Scan# 1791


Delta R.T. -0.000 min


Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt Ion:119 Resp: 3577

Ion	Ratio	Lower	Upper
119	100		
134	25.0	12.5	37.5
91	33.1	13.8	41.4



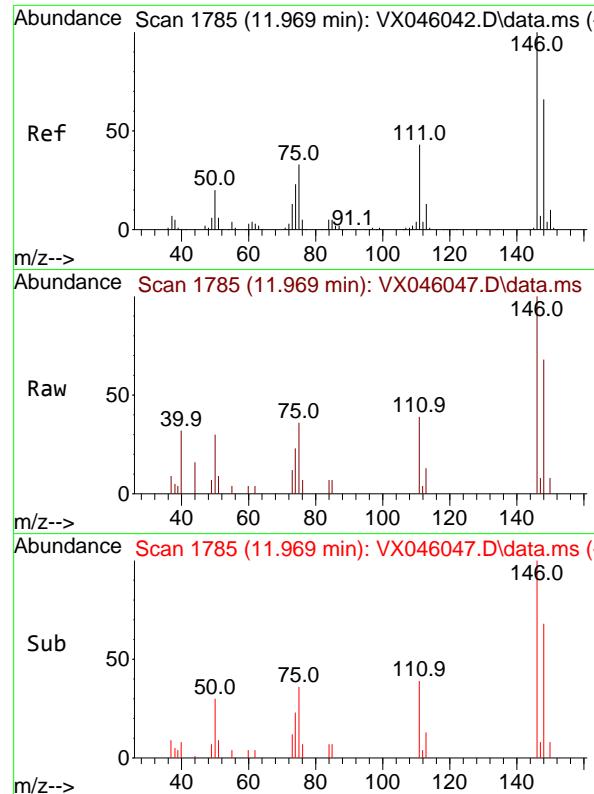

#87

1,3-Dichlorobenzene

Concen: 0.689 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument:

MSVOA\_X


ClientSampleId :

VSTDICC001

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

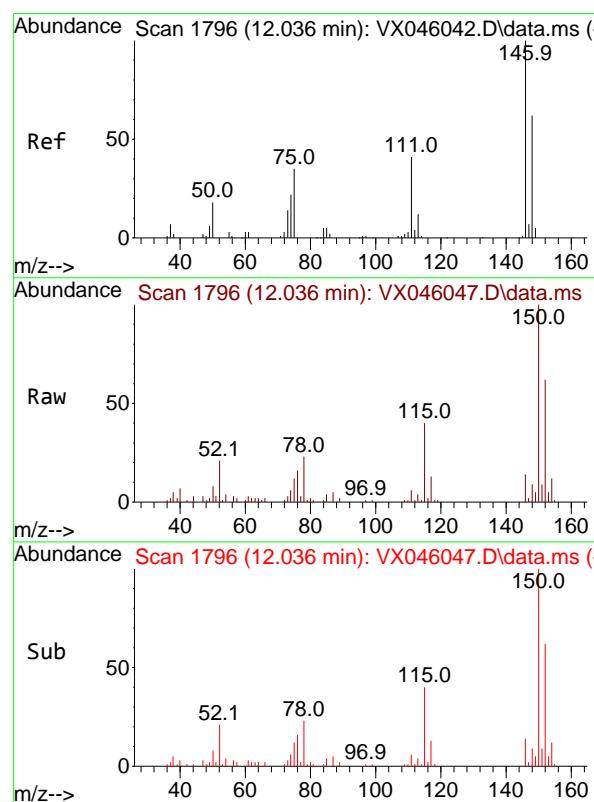

#88

1,4-Dichlorobenzene

Concen: 0.789 ug/l

RT: 12.036 min Scan# 1796

Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27


Tgt Ion:146 Resp: 2149







Ion Ratio Lower Upper

146 100

111 39.1 21.3 63.9

148 58.2 31.9 95.5

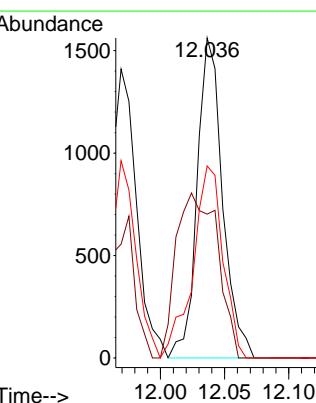



#89

n-Butylbenzene

Concen: 0.631 ug/l

RT: 12.335 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

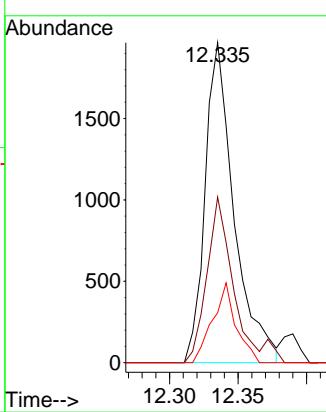

#90

Hexachloroethane

Concen: 0.616 ug/l


RT: 12.536 min Scan# 1878







Delta R.T. -0.000 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Tgt	Ion:	Ion Ratio	Resp:	Lower	Upper
	117	100	604		
	201	64.2	31.6	94.7	

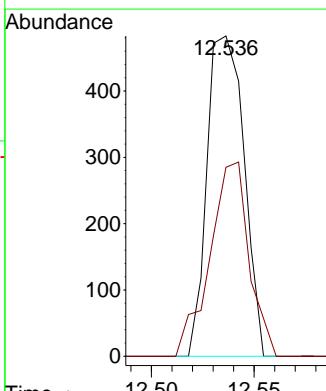



#91

1,2-Dichlorobenzene

Concen: 0.747 ug/l

RT: 12.341 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27

Instrument :

MSVOA\_X


ClientSampleId :

VSTDICC001

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

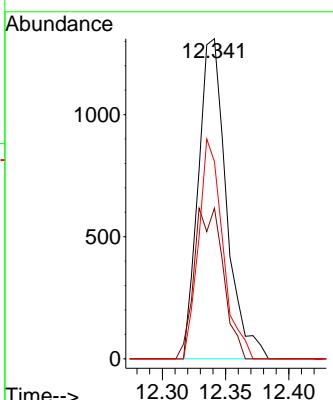

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.586 ug/l

RT: 12.945 min Scan# 1945

Delta R.T. 0.006 min

Lab File: VX046047.D

Acq: 05 May 2025 16:27


Tgt Ion: 75 Resp: 306


Ion Ratio Lower Upper

75 100

155 49.3 34.9 104.8

157 78.1 43.8 131.4

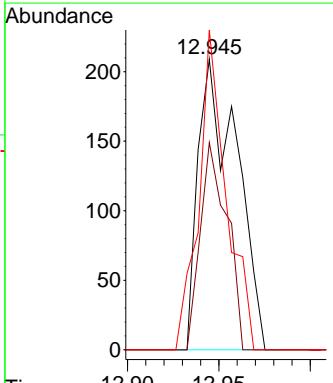


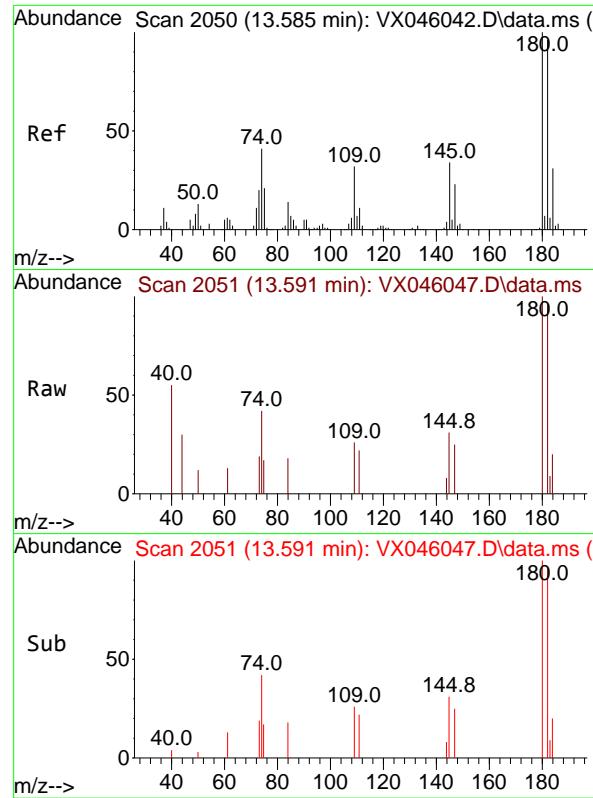


#93  
1,2,4-Trichlorobenzene  
Concen: 0.688 ug/l  
RT: 13.591 min Scan# 2  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

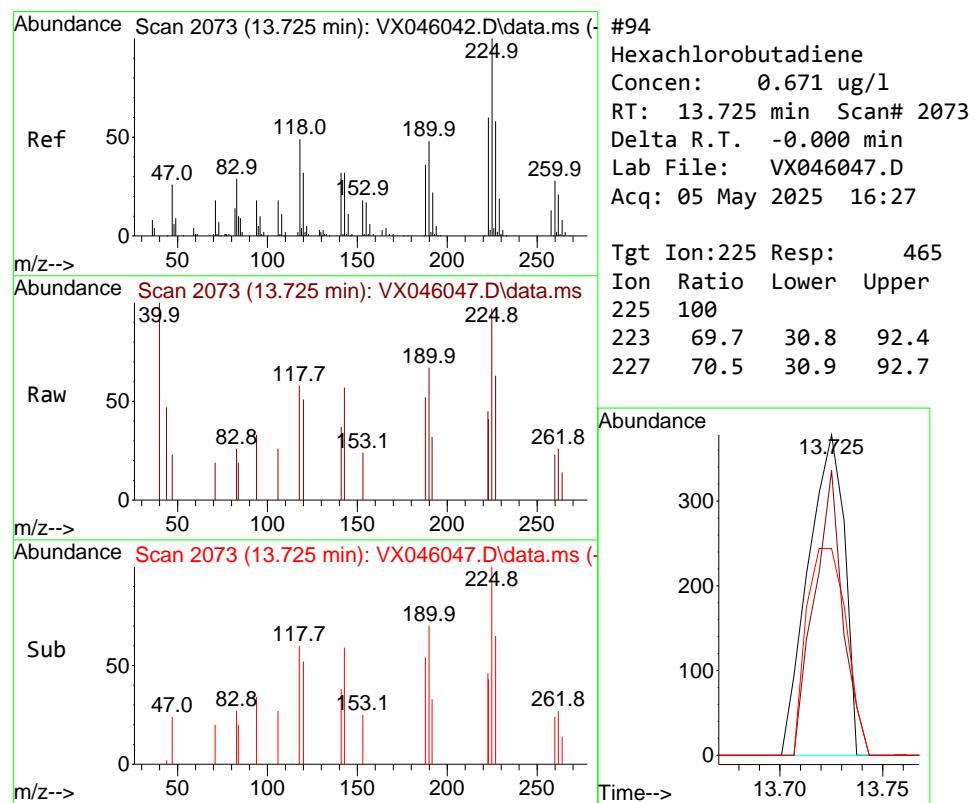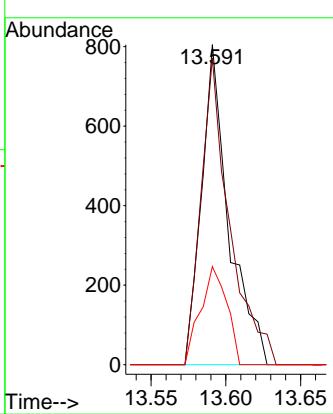

#94  
Hexachlorobutadiene  
Concen: 0.671 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. -0.000 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion:225 Resp: 465  
Ion Ratio Lower Upper  
225 100  
223 69.7 30.8 92.4  
227 70.5 30.9 92.7




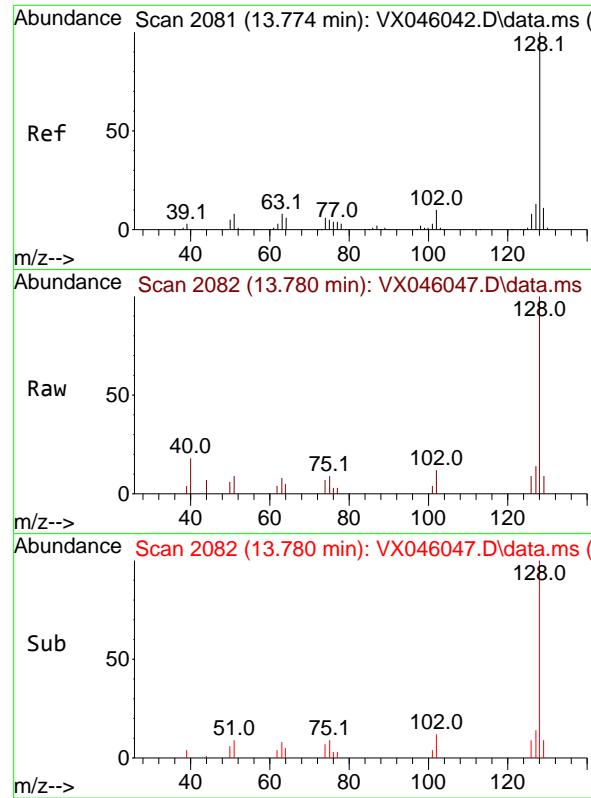


#95  
Naphthalene  
Concen: 0.767 ug/l  
RT: 13.780 min Scan# 2111  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Instrument : MSVOA\_X  
ClientSampleId : VSTDICC001


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

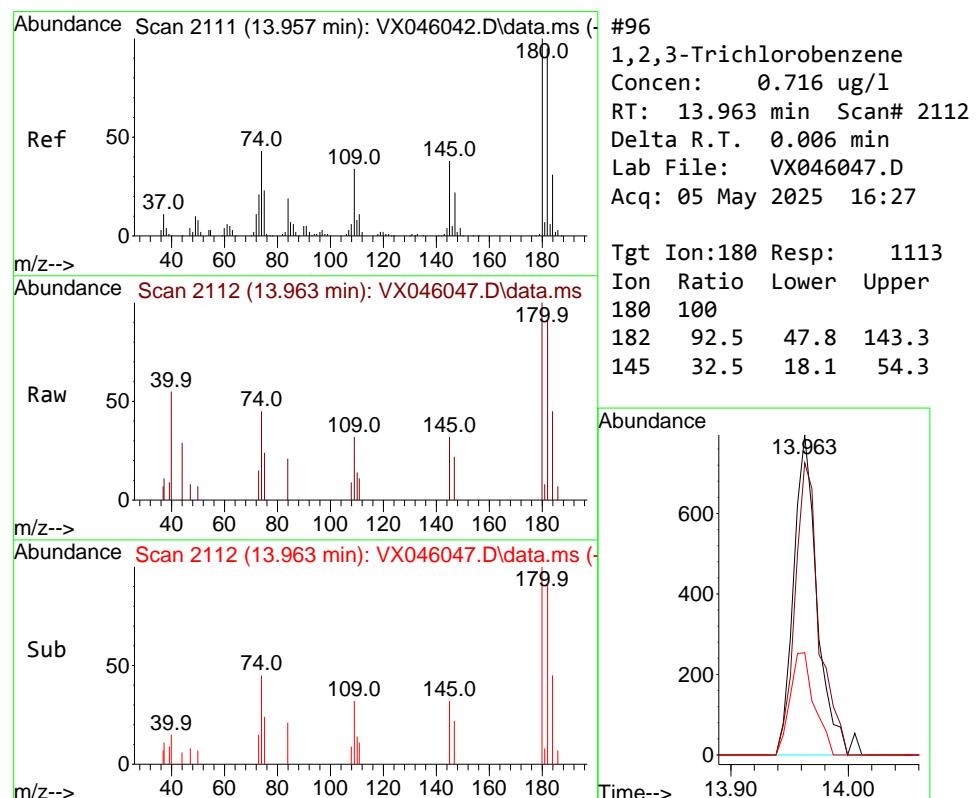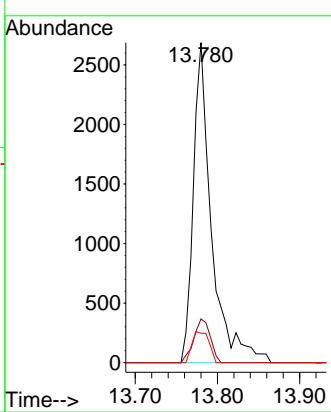

#96  
1,2,3-Trichlorobenzene  
Concen: 0.716 ug/l  
RT: 13.963 min Scan# 2112  
Delta R.T. 0.006 min  
Lab File: VX046047.D  
Acq: 05 May 2025 16:27

Tgt Ion:180 Resp: 1113  
Ion Ratio Lower Upper  
180 100  
182 92.5 47.8 143.3  
145 32.5 18.1 54.3

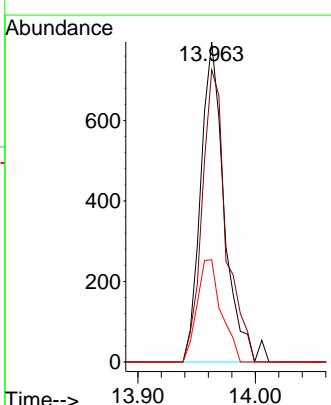

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046048.D  
 Acq On : 05 May 2025 16:50  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX050525**

Quant Time: May 06 07:17:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	92588	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	162651	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	145078	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68229	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	83733	48.509	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.020%		
35) Dibromofluoromethane	5.379	113	58192	49.683	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.360%		
50) Toluene-d8	8.647	98	198575	48.984	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.960%		
62) 4-Bromofluorobenzene	11.079	95	75568	48.596	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	97.200%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.167	85	78783	55.594	ug/l	99
3) Chloromethane	1.307	50	72275	52.592	ug/l	100
4) Vinyl Chloride	1.374	62	65994	51.598	ug/l	98
5) Bromomethane	1.593	94	30033	50.627	ug/l	97
6) Chloroethane	1.666	64	35690	52.271	ug/l	94
7) Trichlorofluoromethane	1.874	101	99352	52.560	ug/l	99
8) Diethyl Ether	2.130	74	31875	49.536	ug/l	97
9) 1,1,2-Trichlorotrifluo...	2.319	101	59451	50.822	ug/l	99
10) Methyl Iodide	2.447	142	73940	53.419	ug/l	99
11) Tert butyl alcohol	2.977	59	61065	252.025	ug/l	99
12) 1,1-Dichloroethene	2.313	96	56097	51.097	ug/l	98
13) Acrolein	2.233	56	64157	232.505	ug/l	99
14) Allyl chloride	2.660	41	108757	51.833	ug/l	100
15) Acrylonitrile	3.063	53	181808	262.412	ug/l	99
16) Acetone	2.380	43	169923	245.518	ug/l	98
17) Carbon Disulfide	2.502	76	132695	50.981	ug/l	99
18) Methyl Acetate	2.703	43	80251	49.968	ug/l	97
19) Methyl tert-butyl Ether	3.111	73	195442	50.777	ug/l	99
20) Methylene Chloride	2.782	84	63369	47.779	ug/l	99
21) trans-1,2-Dichloroethene	3.087	96	55770	50.513	ug/l	99
22) Diisopropyl ether	3.757	45	209946	51.800	ug/l	97
23) Vinyl Acetate	3.715	43	946746	265.585	ug/l	100
24) 1,1-Dichloroethane	3.605	63	114733	50.825	ug/l	98
25) 2-Butanone	4.556	43	258339	257.110	ug/l	97
26) 2,2-Dichloropropane	4.471	77	88229	49.934	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	67727	50.956	ug/l	100
28) Bromochloromethane	4.891	49	55390	50.975	ug/l	98
29) Tetrahydrofuran	5.001	42	163675	259.958	ug/l	99
30) Chloroform	5.093	83	120782	51.332	ug/l	97
31) Cyclohexane	5.458	56	103158	50.147	ug/l	96
32) 1,1,1-Trichloroethane	5.373	97	104243	51.108	ug/l	100
36) 1,1-Dichloropropene	5.690	75	77931	49.521	ug/l	99
37) Ethyl Acetate	4.715	43	98604	50.714	ug/l	100
38) Carbon Tetrachloride	5.666	117	88100	49.825	ug/l	97
39) Methylcyclohexane	7.373	83	100808	49.757	ug/l	98
40) Benzene	6.031	78	233977	50.759	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046048.D  
 Acq On : 05 May 2025 16:50  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX050525**

Quant Time: May 06 07:17:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlane 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	56017	55.076	ug/1	100
42) 1,2-Dichloroethane	6.080	62	101185	50.861	ug/1	98
43) Isopropyl Acetate	6.336	43	154818	52.195	ug/1	99
44) Trichloroethene	7.123	130	55491	50.018	ug/1	100
45) 1,2-Dichloropropane	7.428	63	59582	51.983	ug/1	98
46) Dibromomethane	7.580	93	45181	49.978	ug/1	99
47) Bromodichloromethane	7.818	83	92388	51.889	ug/1	100
48) Methyl methacrylate	7.690	41	82144	54.226	ug/1	98
49) 1,4-Dioxane	7.659	88	30477	1059.599	ug/1	97
51) 4-Methyl-2-Pentanone	8.574	43	510206	259.133	ug/1	100
52) Toluene	8.714	92	144574	51.150	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	83751	52.920	ug/1	100
54) cis-1,3-Dichloropropene	8.360	75	92517	52.892	ug/1	98
55) 1,1,2-Trichloroethane	9.147	97	56713	50.887	ug/1	96
56) Ethyl methacrylate	9.116	69	95772	53.918	ug/1	99
57) 1,3-Dichloropropane	9.305	76	99663	49.793	ug/1	97
58) 2-Chloroethyl Vinyl ether	8.238	63	240681	265.780	ug/1	99
59) 2-Hexanone	9.427	43	390701	268.218	ug/1	100
60) Dibromochloromethane	9.519	129	63738	52.075	ug/1	99
61) 1,2-Dibromoethane	9.610	107	59134	51.050	ug/1	98
64) Tetrachloroethene	9.269	164	48034	46.795	ug/1	98
65) Chlorobenzene	10.073	112	154640	48.699	ug/1	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	53735	49.557	ug/1	100
67) Ethyl Benzene	10.189	91	281239	50.245	ug/1	100
68) m/p-Xylenes	10.299	106	206813	101.022	ug/1	99
69) o-Xylene	10.640	106	101469	50.841	ug/1	99
70) Styrene	10.653	104	169703	51.907	ug/1	99
71) Bromoform	10.799	173	40364	49.583	ug/1 #	97
73) Isopropylbenzene	10.957	105	269484	50.733	ug/1	100
74) N-amyl acetate	10.842	43	137559	52.407	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	89027	47.827	ug/1	98
76) 1,2,3-Trichloropropane	11.238	75	79763m	48.568	ug/1	
77) Bromobenzene	11.195	156	59871	48.549	ug/1	98
78) n-propylbenzene	11.299	91	312285	50.562	ug/1	100
79) 2-Chlorotoluene	11.360	91	195630	49.107	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	228538	51.500	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	24857	49.276	ug/1	98
82) 4-Chlorotoluene	11.451	91	223811	50.661	ug/1	100
83) tert-Butylbenzene	11.713	119	225783	50.511	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	231371	51.485	ug/1	100
85) sec-Butylbenzene	11.890	105	280578	51.122	ug/1	99
86) p-Isopropyltoluene	12.006	119	231942	51.198	ug/1	100
87) 1,3-Dichlorobenzene	11.963	146	113146	50.272	ug/1	99
88) 1,4-Dichlorobenzene	12.037	146	111173	48.368	ug/1	99
89) n-Butylbenzene	12.329	91	205858	51.804	ug/1	100
90) Hexachloroethane	12.536	117	39823	49.895	ug/1	99
91) 1,2-Dichlorobenzene	12.335	146	111482	49.361	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	21220	51.458	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	64421	49.662	ug/1	100
94) Hexachlorobutadiene	13.719	225	27425	48.408	ug/1	98
95) Naphthalene	13.774	128	239805	50.404	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	64950	48.525	ug/1	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046048.D  
 Acq On : 05 May 2025 16:50  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
ICVVX050525

Quant Time: May 06 07:17:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carbone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046048.D  
Acq On : 05 May 2025 16:50  
Operator : JC/MD  
Sample : VSTDICV050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1




Quant Time: May 06 07:17:12 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
ICVVX050525

## Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

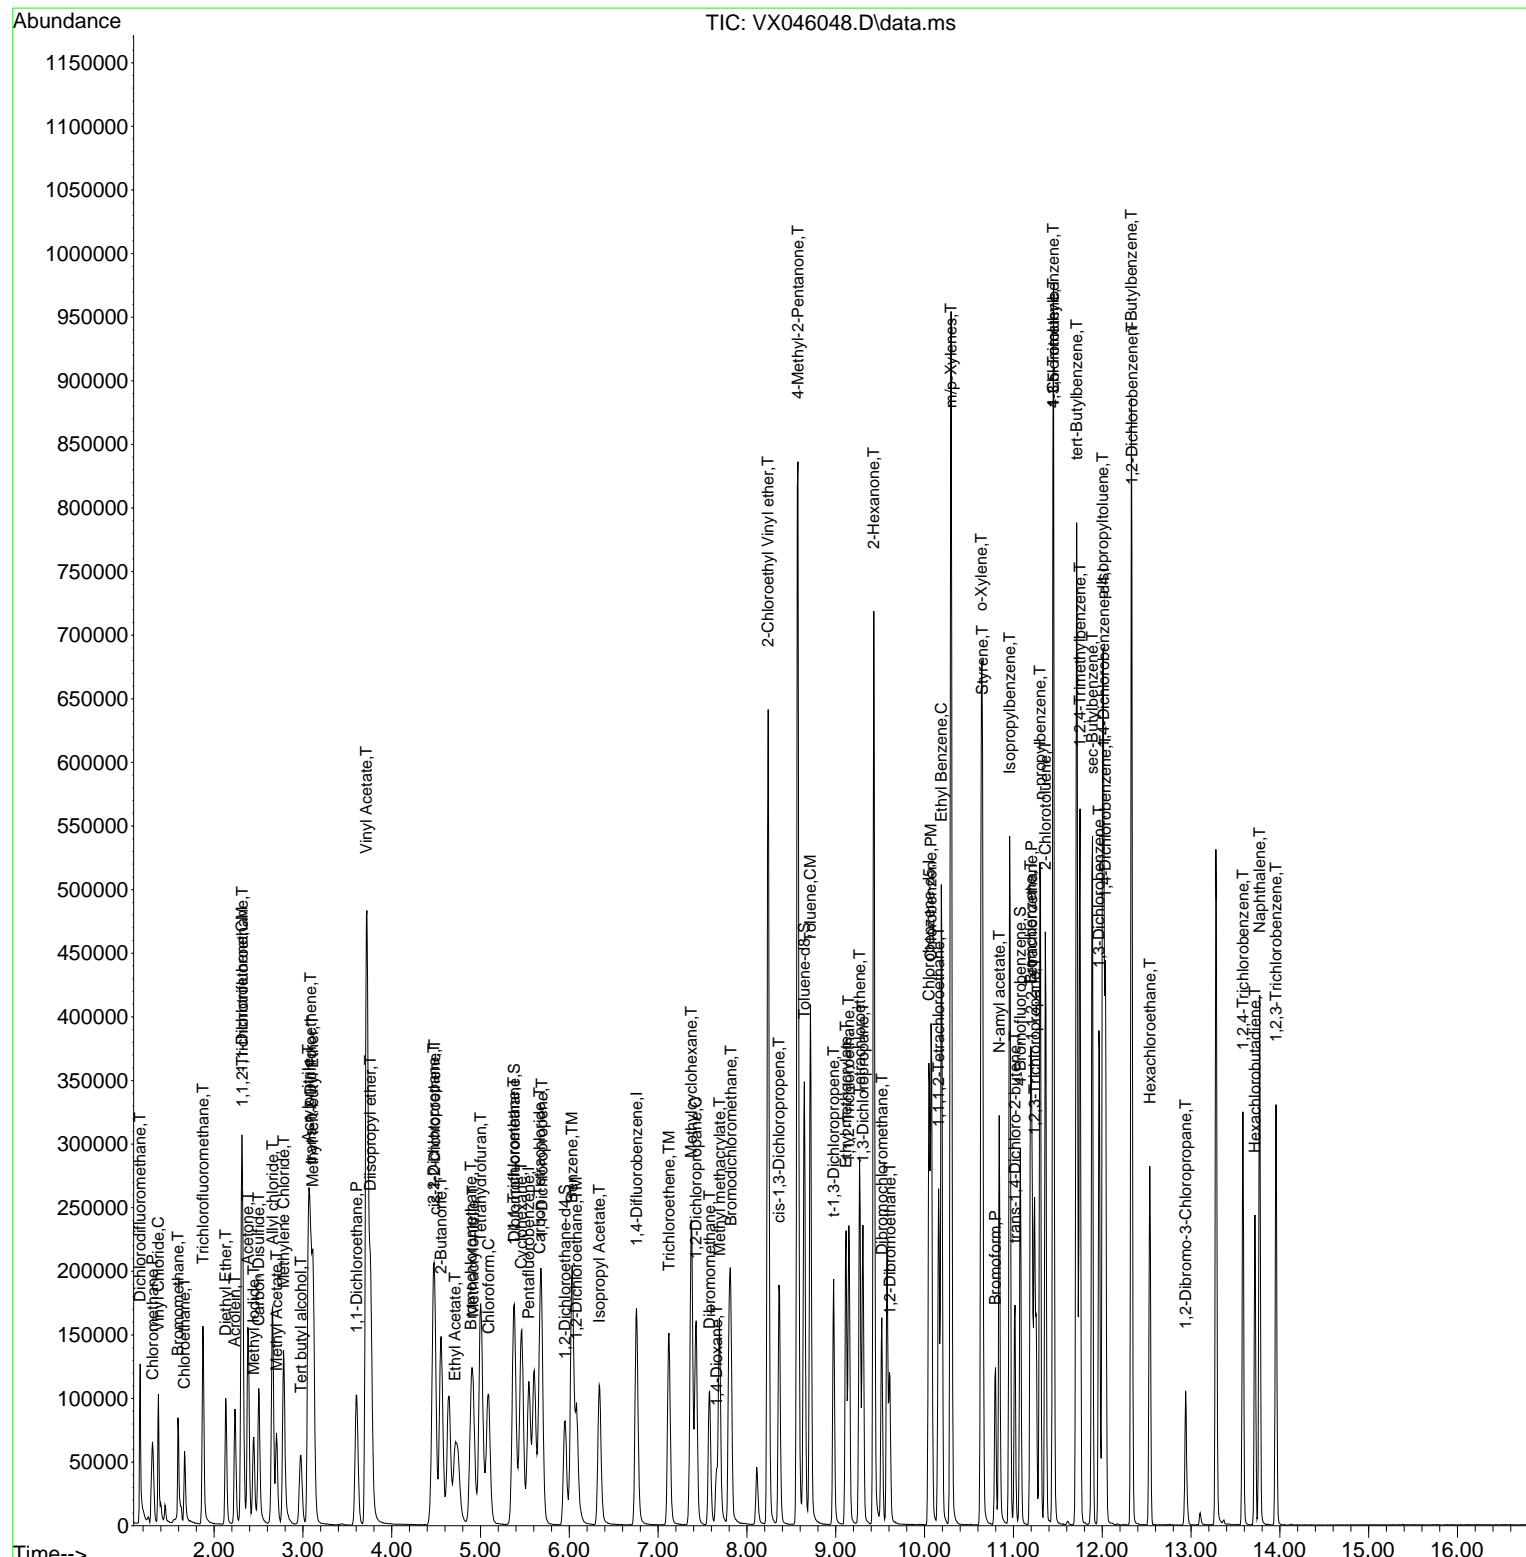







#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.544 min Scan# 7  
 Delta R.T. -0.000 min  
 Lab File: VX046048.D  
 Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
 ClientSampleId : ICVVX050525


Manual Integrations  
**APPROVED**



Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025



#2  
 Dichlorodifluoromethane  
 Concen: 55.594 ug/l  
 RT: 1.167 min Scan# 13  
 Delta R.T. 0.000 min  
 Lab File: VX046048.D  
 Acq: 05 May 2025 16:50

Tgt Ion: 85 Resp: 78783  
 Ion Ratio Lower Upper  
 85 100  
 87 32.2 15.7 47.1

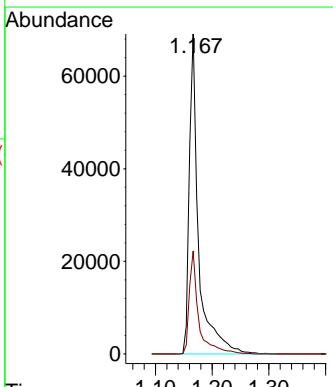

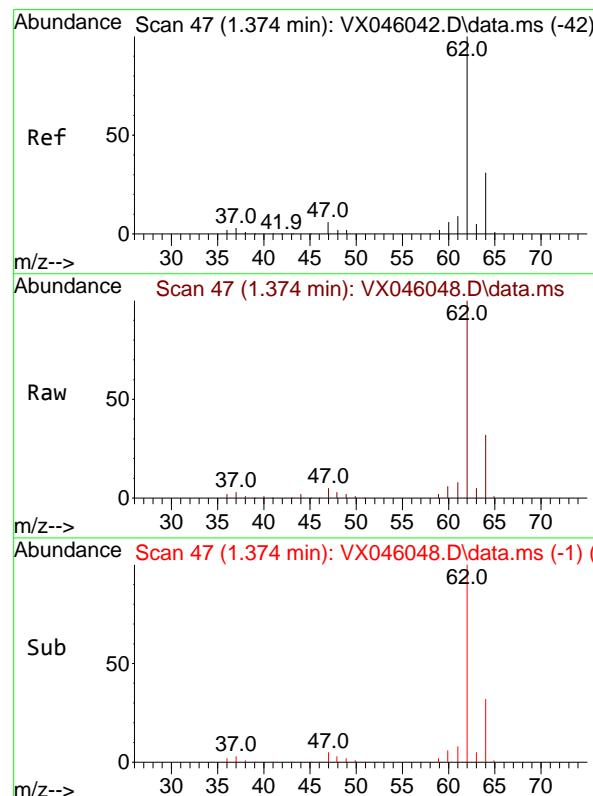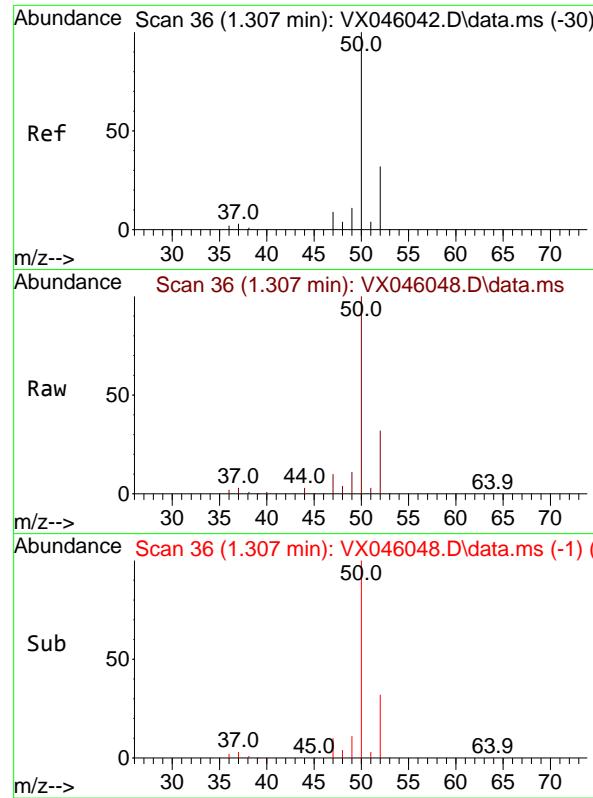


#3  
Chloromethane  
Concen: 52.592 ug/l  
RT: 1.307 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525

Tgt Ion: 50 Resp: 7227  
Ion Ratio Lower Upper  
50 100  
52 31.8 25.4 38.2


### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#4  
Vinyl Chloride  
Concen: 51.598 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 62 Resp: 65994  
Ion Ratio Lower Upper  
62 100  
64 32.3 25.2 37.8

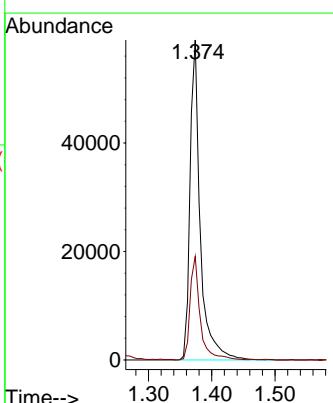



#5

Bromomethane

Concen: 50.627 ug/l

RT: 1.593 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#6

Chloroethane

Concen: 52.271 ug/l

RT: 1.666 min Scan# 95


Delta R.T. 0.000 min


Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion: 64 Resp: 35690  
 Ion Ratio Lower Upper  
 64 100  
 66 33.7 24.3 36.5


Time--&gt; 1.55 1.60 1.65

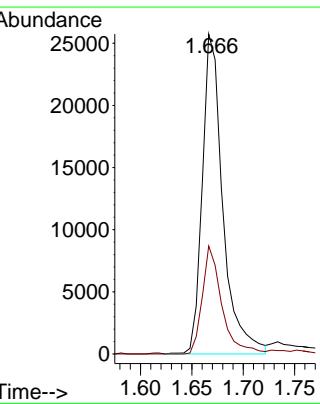



#7  
Trichlorofluoromethane  
Concen: 52.560 ug/l  
RT: 1.874 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50




Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525




Tgt Ion:101 Resp: 9935  
Ion Ratio Lower Upper  
101 100  
103 62.6 51.0 76.4

Manual Integrations  
APPROVED



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025




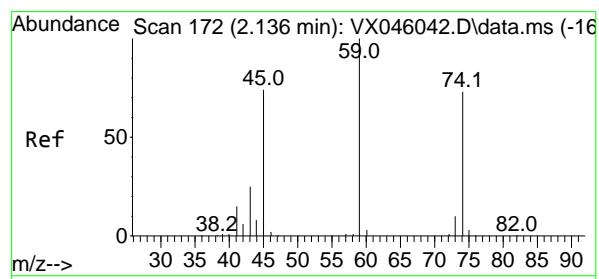
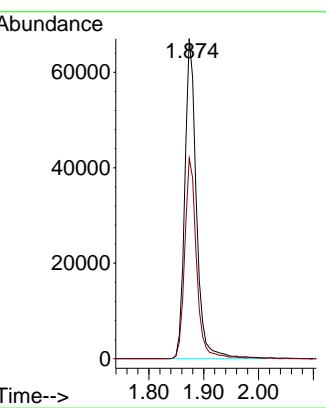



#8  
Diethyl Ether  
Concen: 49.536 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50



Tgt Ion: 74 Resp: 31875  
Ion Ratio Lower Upper  
74 100  
45 107.1 54.9 164.8

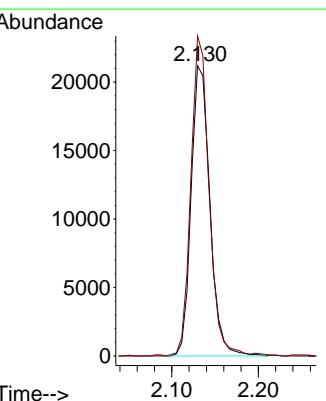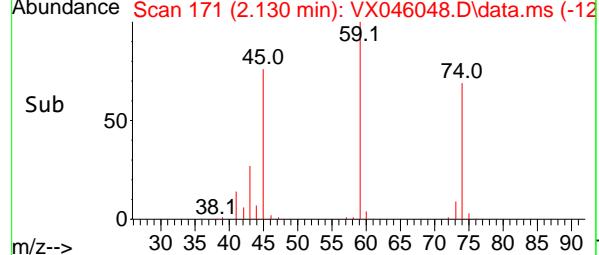

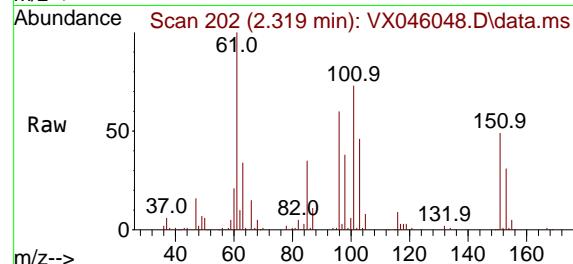

#9

1,1,2-Trichlorotrifluoroethane

Concen: 50.822 ug/l

RT: 2.319 min Scan# 202

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025




Supervised By :Mahesh Dadoda 05/06/2025

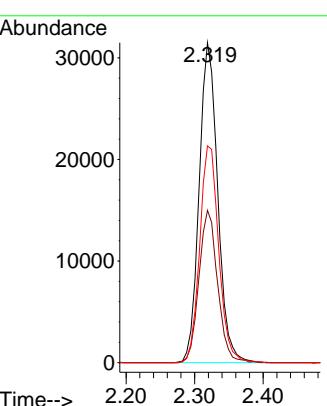

#10  
Methyl Iodide  
Concen: 53.419 ug/l  
RT: 2.447 min Scan# 223  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion:142 Resp: 73940  
Ion Ratio Lower Upper  
142 100  
127 52.9 41.7 62.5  
141 14.4 11.5 17.3

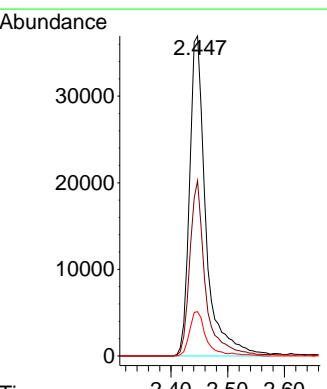

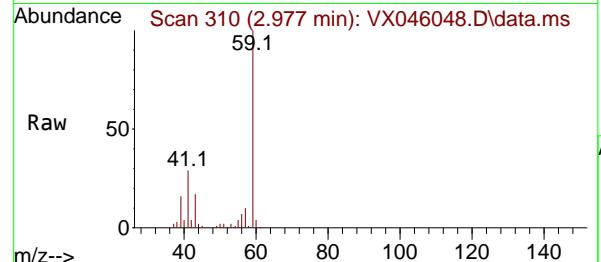

#11

Tert butyl alcohol

Concen: 252.025 ug/l

RT: 2.977 min Scan# 310

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

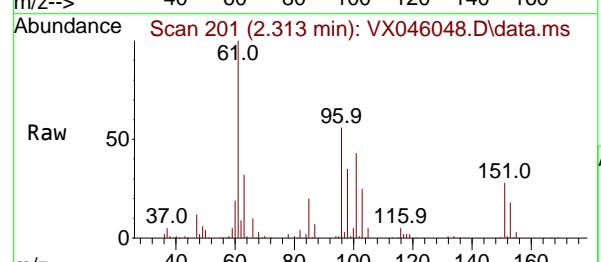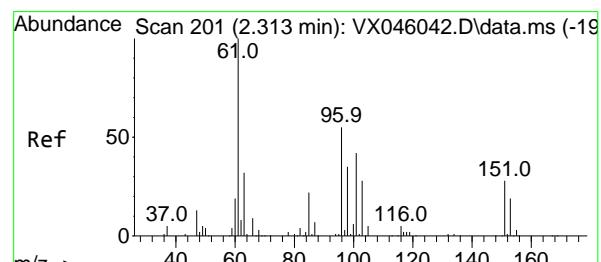

#12

1,1-Dichloroethene

Concen: 51.097 ug/l


RT: 2.313 min Scan# 201







Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion: 96 Resp: 56097  
 Ion Ratio Lower Upper  
 96 100  
 61 179.7 146.2 219.2  
 98 62.1 51.0 76.6

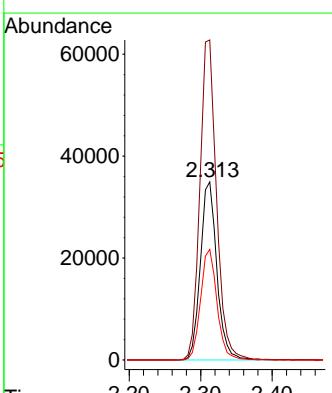

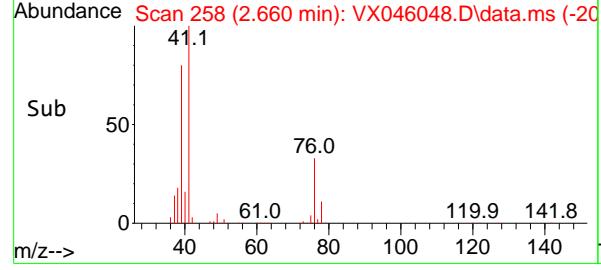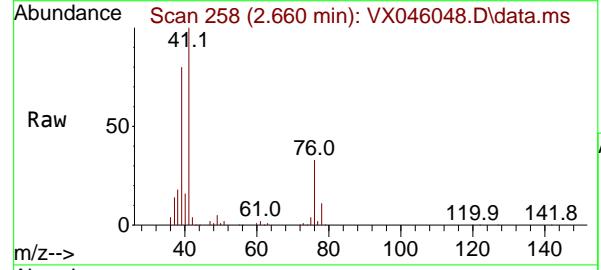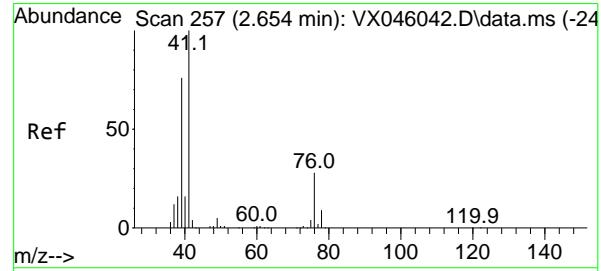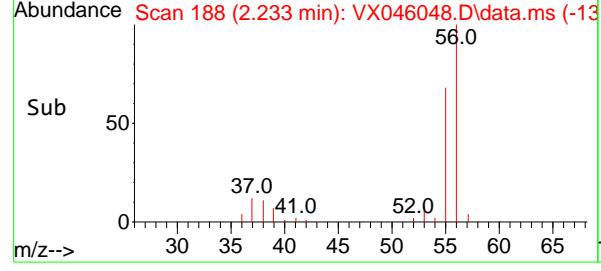

#13

Acrolein

Concen: 232.505 ug/l

RT: 2.233 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:


MSVOA\_X

ClientSampleId :

ICVVX050525

Manual Integrations  
APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#14

Allyl chloride

Concen: 51.833 ug/l


RT: 2.660 min Scan# 258




Delta R.T. 0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion: 41 Resp: 108757  
Ion Ratio Lower Upper  
41 100  
39 75.6 60.6 90.8  
76 31.1 24.9 37.3

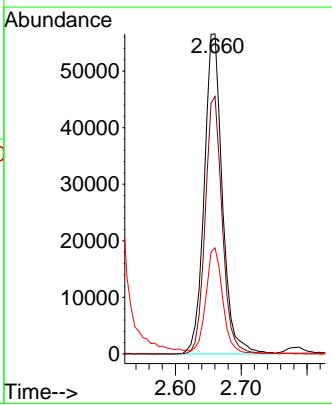



#15

Acrylonitrile

Concen: 262.412 ug/l

RT: 3.063 min Scan# 3

Instrument: MSVOA\_X

Delta R.T. 0.000 min




Lab File: VX046048.D ClientSampleId :

Acq: 05 May 2025 16:50 ICVVX050525

Tgt Ion:	Ion Ratio	Lower	Upper
53	100		
52	82.9	65.3	97.9
51	36.5	29.8	44.8

Manual Integrations  
APPROVED

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

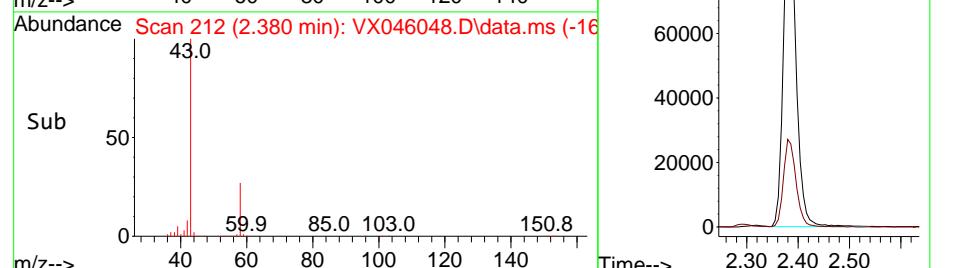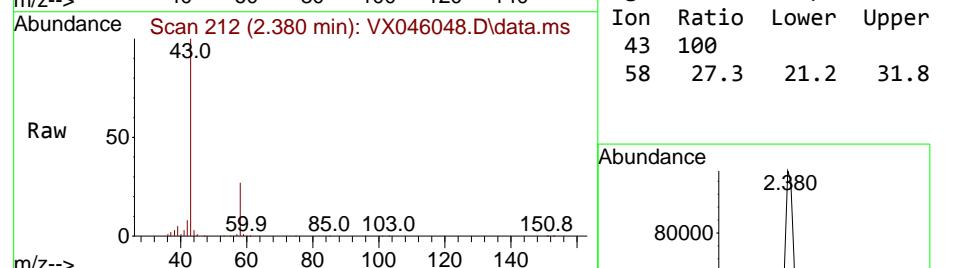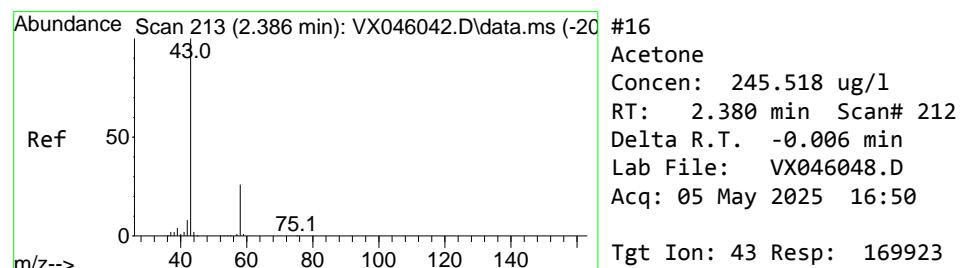

#16

Acetone

Concen: 245.518 ug/l


RT: 2.380 min Scan# 212







Delta R.T. -0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion:	Ion Ratio	Lower	Upper
43	100		
58	27.3	21.2	31.8

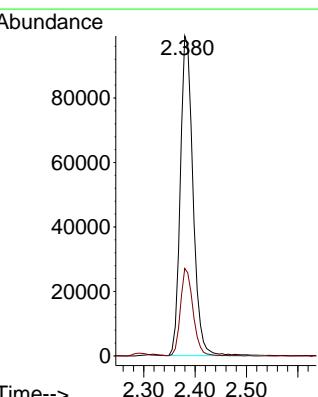



#17

Carbon Disulfide

Concen: 50.981 ug/l

RT: 2.502 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#18

Methyl Acetate

Concen: 49.968 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50




Tgt Ion: 43 Resp: 80251

Ion Ratio Lower Upper

43 100

74 22.1 16.7 25.1

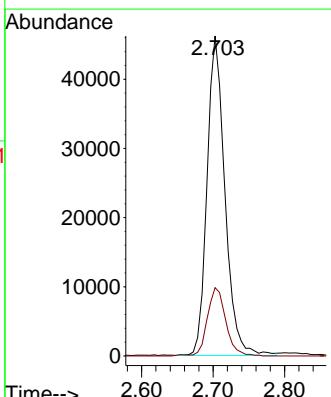







#19

Methyl tert-butyl Ether  
Concen: 50.777 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025






#20

Methylene Chloride  
Concen: 47.779 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 84 Resp: 63369  
Ion Ratio Lower Upper  
84 100  
49 142.7 113.9 170.9  
51 43.3 33.5 50.3  
86 66.8 53.8 80.8

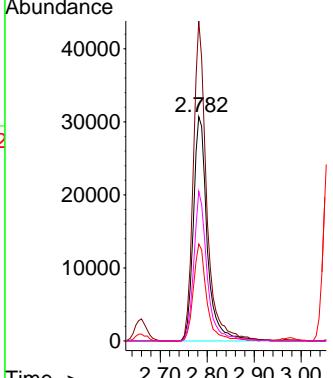







#21  
trans-1,2-Dichloroethene  
Concen: 50.513 ug/l  
RT: 3.087 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525


Manual Integrations  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025



#22  
Diisopropyl ether  
Concen: 51.800 ug/l  
RT: 3.757 min Scan# 438  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 45 Resp: 209946  
Ion Ratio Lower Upper  
45 100  
43 86.9 66.6 100.0  
87 24.8 19.8 29.6  
59 10.8 8.6 12.8





#23

## Vinyl Acetate

Concen: 265.585 ug/l

RT: 3.715 min Scan# 413

Delta R.T. -0.006 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X

ClientSampleId :

ICVVX050525



Tgt Ion: 43 Resp: 946740

Ion Ratio Lower Upper

43 100




86 9.4 7.5 11.3

## Manual Integrations

## APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

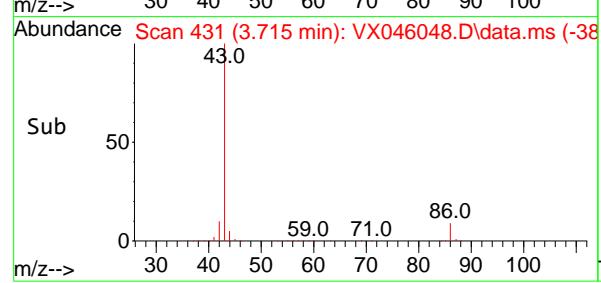

#24

## 1,1-Dichloroethane


Concen: 50.825 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50





Tgt Ion: 63 Resp: 114733


Ion Ratio Lower Upper

63 100

98 6.4 3.6 10.8

100 4.8 2.1 6.3

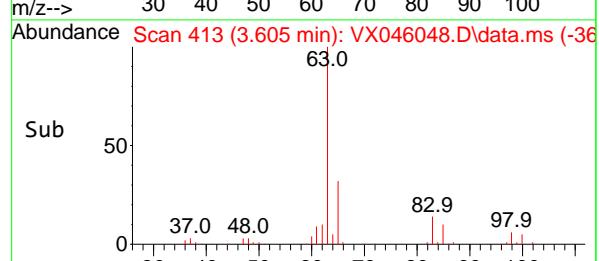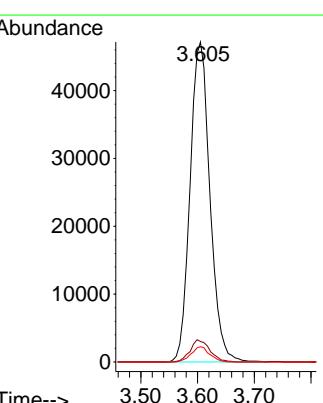


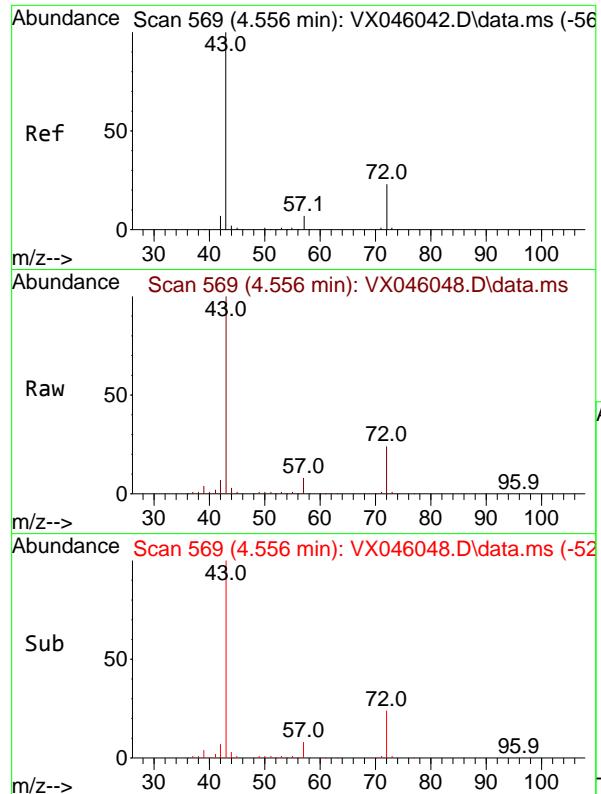


#25  
2-Butanone  
Concen: 257.110 ug/l  
RT: 4.556 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525


**Manual Integrations**  
**APPROVED**


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

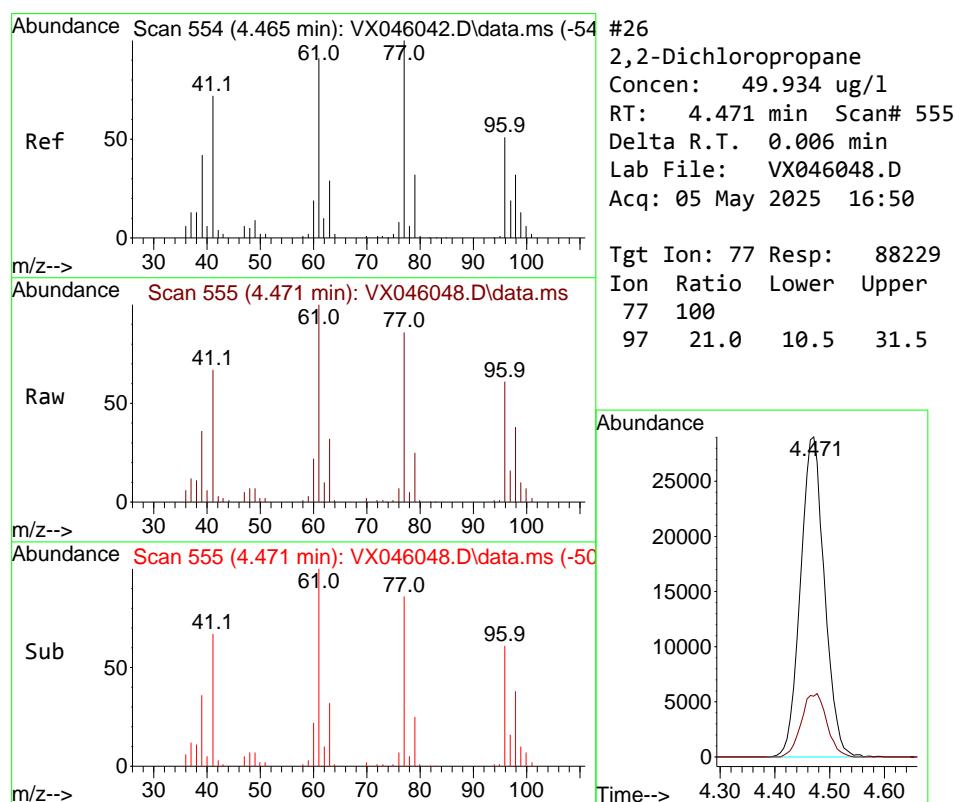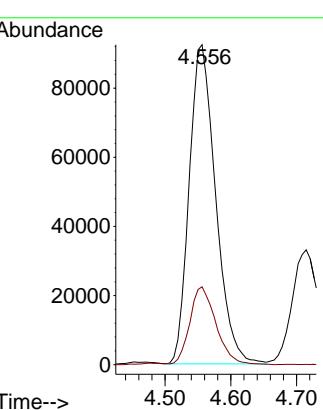



#26  
2,2-Dichloropropane  
Concen: 49.934 ug/l  
RT: 4.471 min Scan# 555  
Delta R.T. 0.006 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 77 Resp: 88229  
Ion Ratio Lower Upper  
77 100  
97 21.0 10.5 31.5

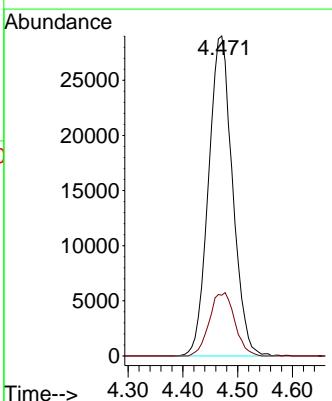





#27  
**cis-1,2-Dichloroethene**  
Concen: 50.956 ug/l  
RT: 4.483 min Scan# 51  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

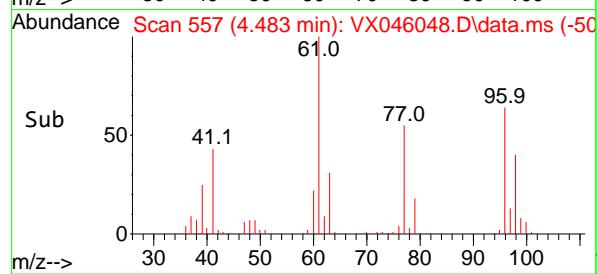


Tgt Ion: 96 Resp: 6772  
Ion Ratio Lower Upper  
96 100  
61 160.7 0.0 322.8  
98 64.4 0.0 129.0

**Manual Integrations**  
**APPROVED**



Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025


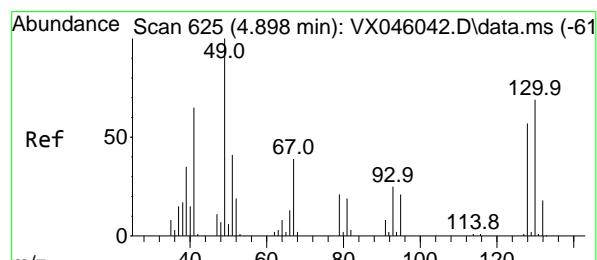
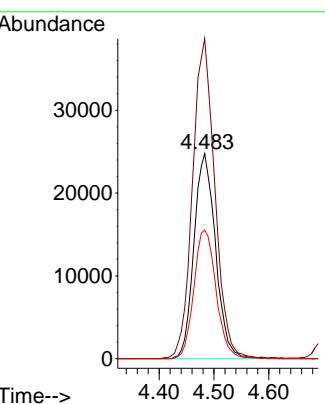


#28  
**Bromochloromethane**  
Concen: 50.975 ug/l  
RT: 4.891 min Scan# 624  
Delta R.T. -0.006 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

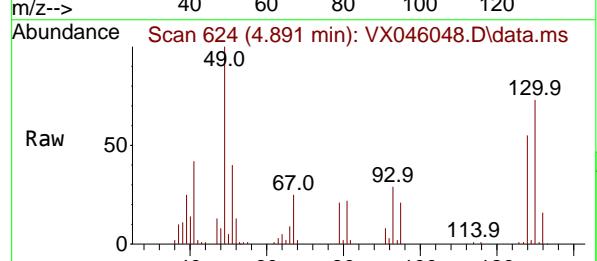

Tgt Ion: 49 Resp: 55390  
Ion Ratio Lower Upper  
49 100  
129 1.8 0.0 4.0  
130 68.7 56.2 84.2

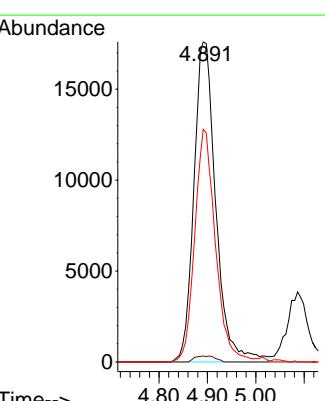

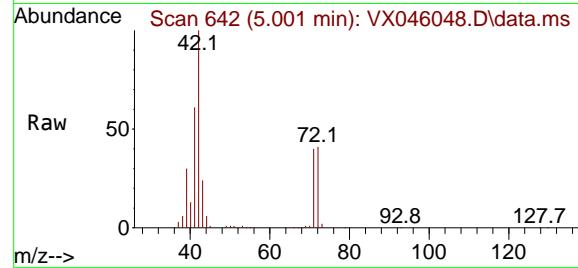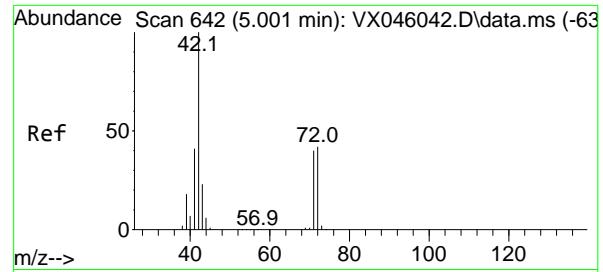

#29

Tetrahydrofuran

Concen: 259.958 ug/l

RT: 5.001 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument :

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#30

Chloroform

Concen: 51.332 ug/l

RT: 5.093 min Scan# 657

Delta R.T. 0.006 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50


Tgt Ion: 83 Resp: 120782

Ion Ratio Lower Upper

83 100

85 63.6 49.3 73.9

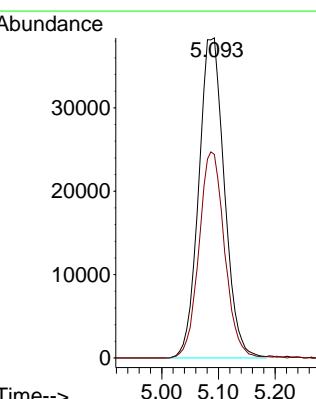

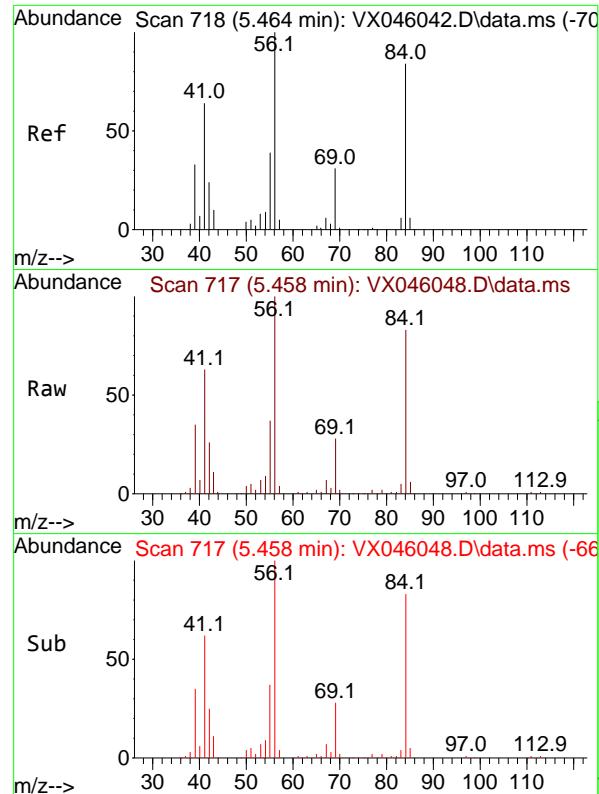

#31

Cyclohexane

Concen: 50.147 ug/l

RT: 5.458 min Scan# 718

Delta R.T. -0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

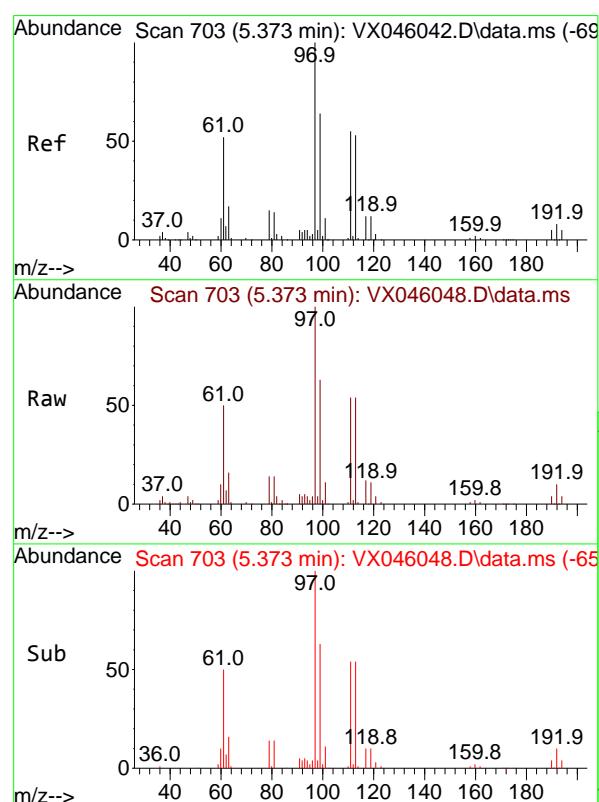

#32

1,1,1-Trichloroethane

Concen: 51.108 ug/l

RT: 5.373 min Scan# 703

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion: 97 Resp: 104243




Ion Ratio Lower Upper

97 100

99 64.5 51.8 77.6

61 50.2 40.1 60.1

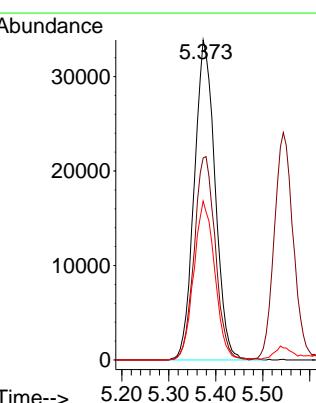



#33

1,2-Dichloroethane-d4

Concen: 48.509 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument :

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

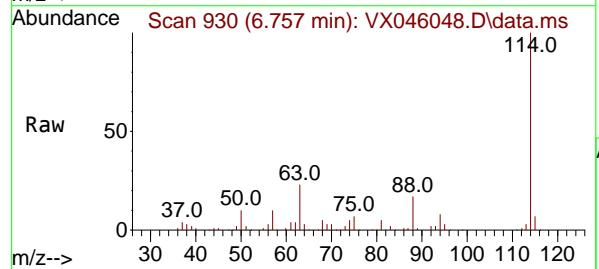

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l


RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt	Ion	Ion Ratio	Lower	Upper
114	100			
63	23.1	0.0	49.2	
88	17.2	0.0	33.6	



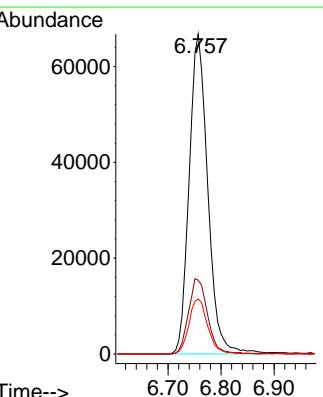


13

14

15

16

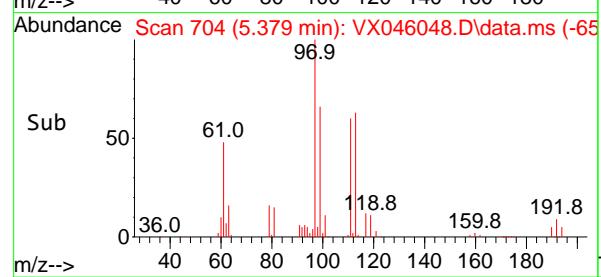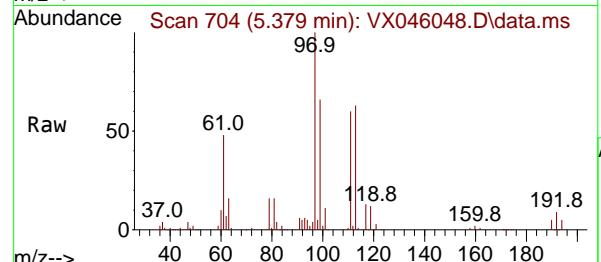

#35

Dibromofluoromethane

Concen: 49.683 ug/l

RT: 5.379 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument :

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

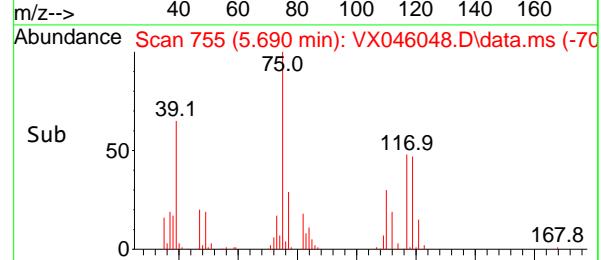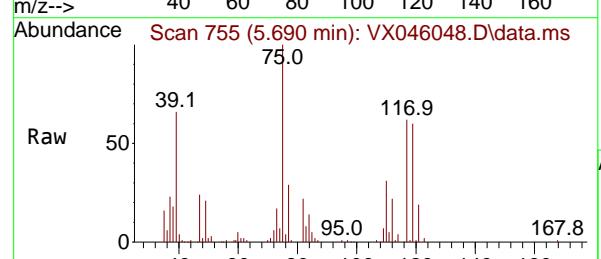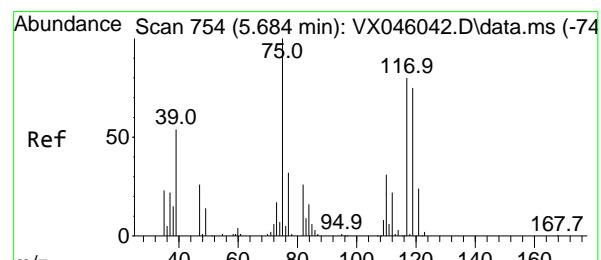

#36

1,1-Dichloropropene

Concen: 49.521 ug/l

RT: 5.690 min Scan# 755

Delta R.T. 0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion: 75 Resp: 77931


Ion Ratio Lower Upper

75 100

110 32.7 16.3 48.9

77 31.1 24.3 36.5

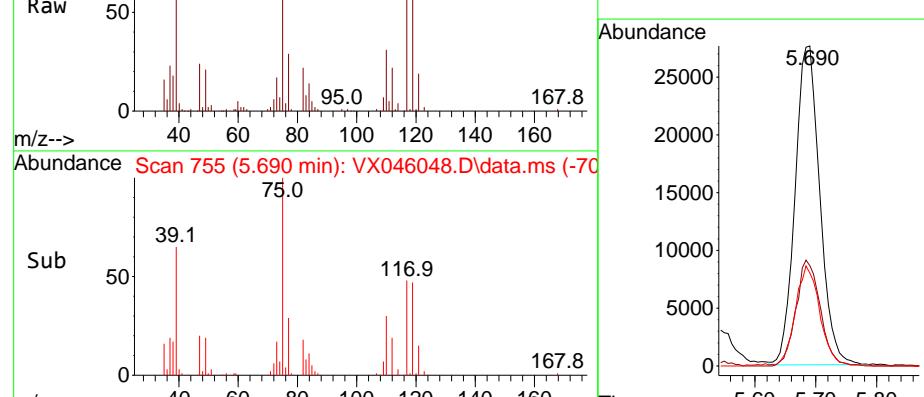

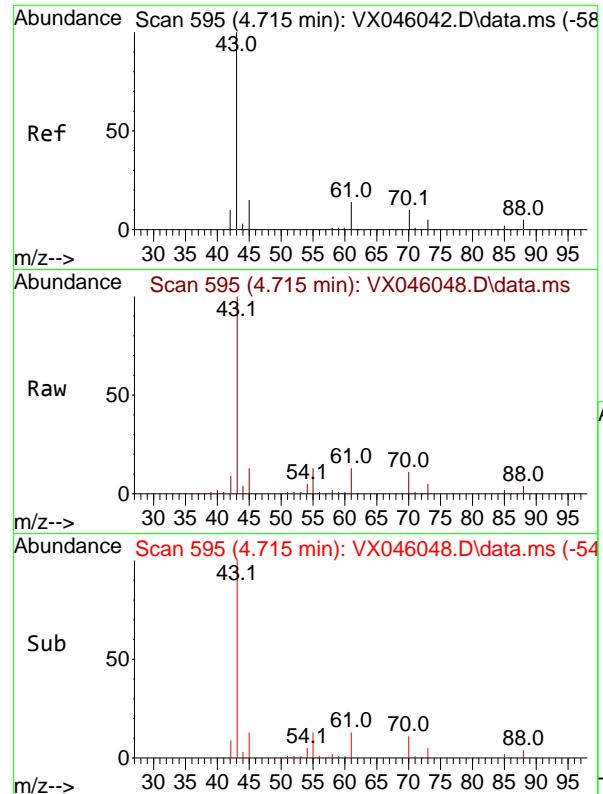

#37

Ethyl Acetate

Concen: 50.714 ug/l

RT: 4.715 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X

ClientSampleId :

ICVVX050525

Tgt Ion: 43 Resp: 9860

Ion Ratio Lower Upper

43 100

61 12.6 10.3 15.5



70 10.0 7.9 11.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

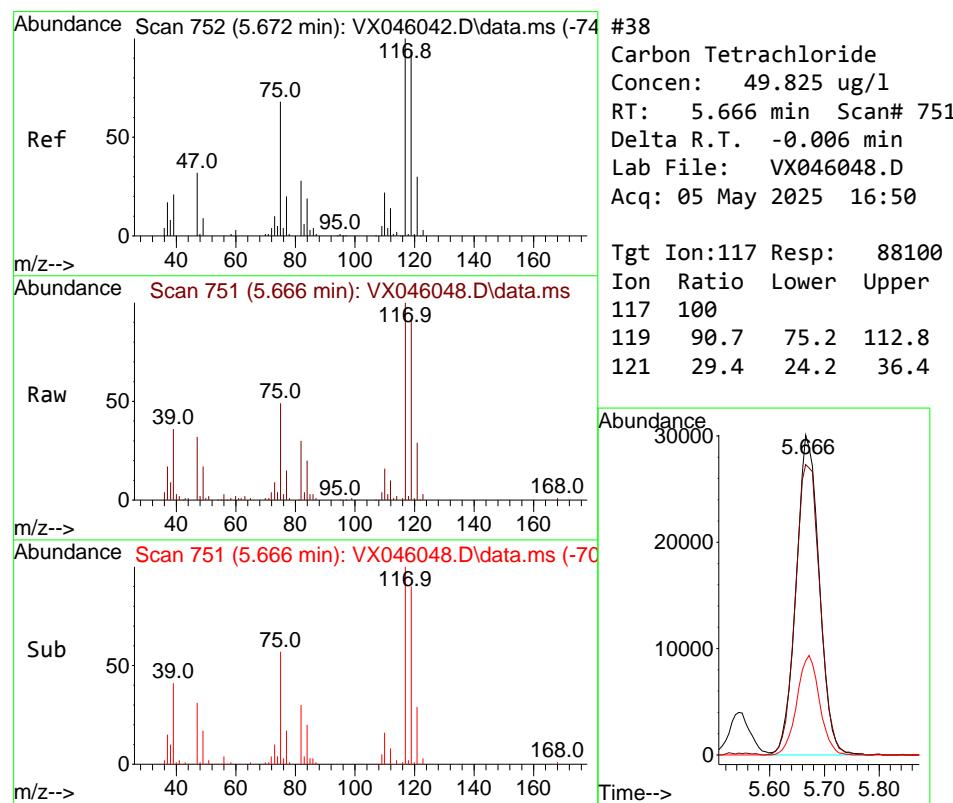

#38

Carbon Tetrachloride

Concen: 49.825 ug/l

RT: 5.666 min Scan# 751

Delta R.T. -0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion: 117 Resp: 88100


Ion Ratio Lower Upper

117 100

119 90.7 75.2 112.8

121 29.4 24.2 36.4

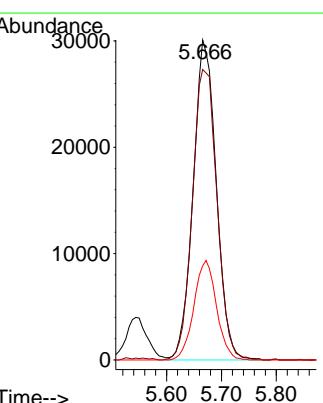

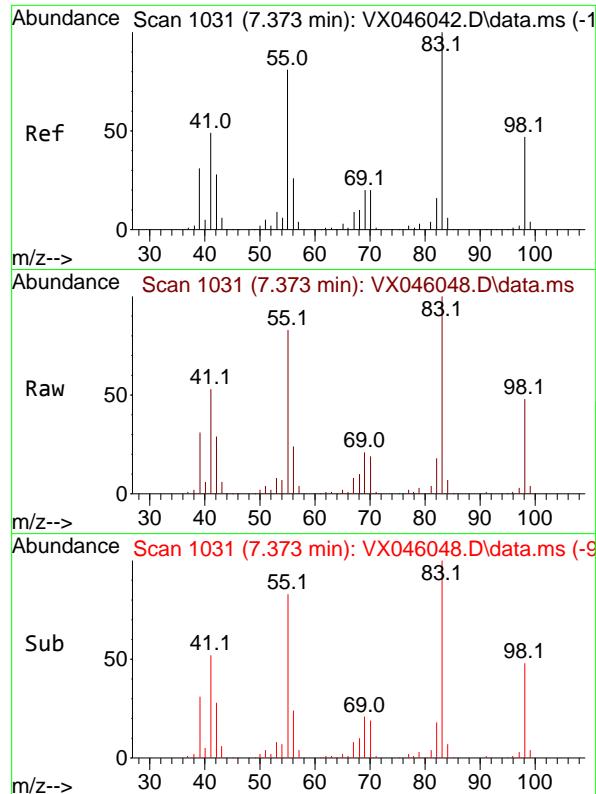

#39

Methylcyclohexane

Concen: 49.757 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

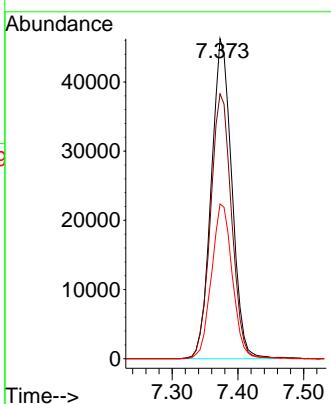

#40

Benzene

Concen: 50.759 ug/l

RT: 6.031 min Scan# 811


Delta R.T. 0.000 min







Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion: 78 Resp: 233977

Ion	Ratio	Lower	Upper
78	100		
77	24.0	19.0	28.4

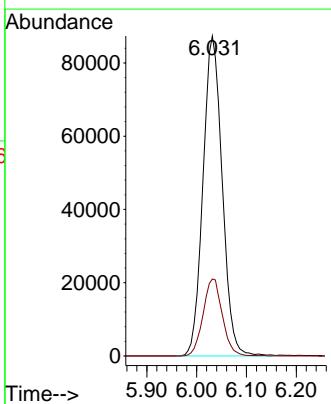

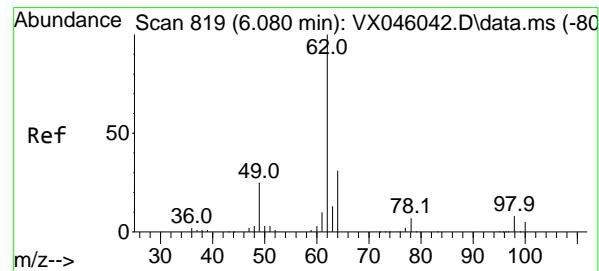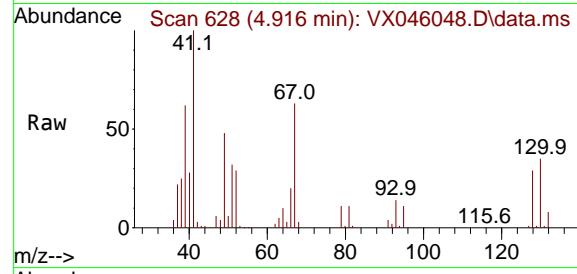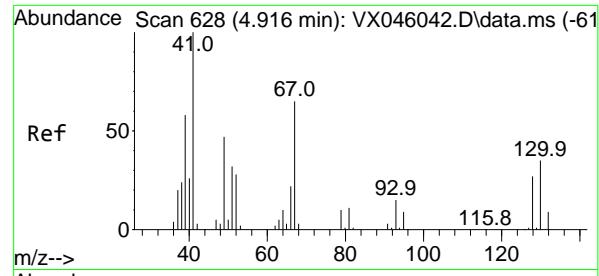

#41

Methacrylonitrile

Concen: 55.076 ug/l

RT: 4.916 min Scan# 6

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument : MSVOA\_X

ClientSampleId : ICVVX050525

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

Tgt Ion: 41 Resp: 5601


Ion Ratio Lower Upper

41 100

39 58.7 47.2 70.8

67 63.7 50.7 76.1

52 30.5 24.6 37.0

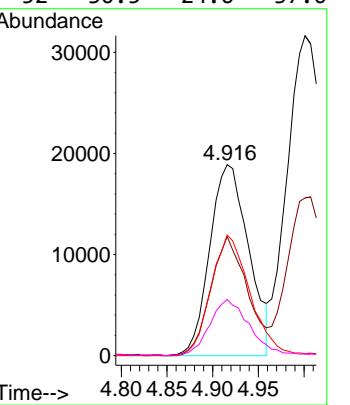

#42

1,2-Dichloroethane

Concen: 50.861 ug/l

RT: 6.080 min Scan# 819

Delta R.T. 0.000 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50


Tgt Ion: 62 Resp: 101185

Ion Ratio Lower Upper





62 100

98 7.1 0.0 15.2

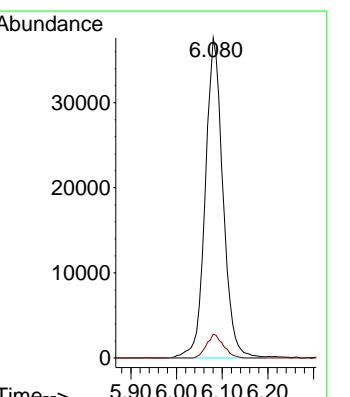



Abundance Scan 861 (6.336 min): VX046048.D\data.ms

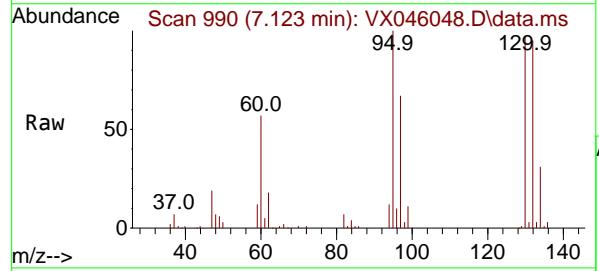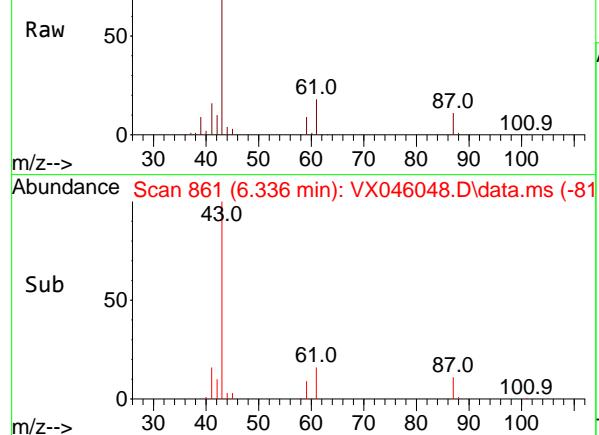

#43

Isopropyl Acetate

Concen: 52.195 ug/l

RT: 6.336 min Scan# 8

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument :

MSVOA\_X





ClientSampleId :

ICVVX050525

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

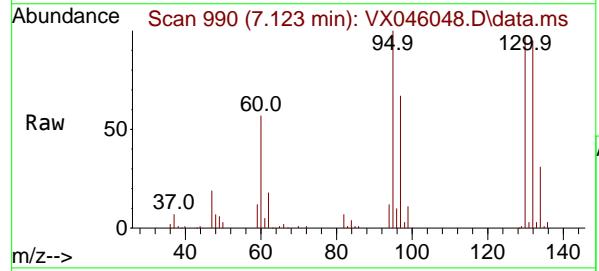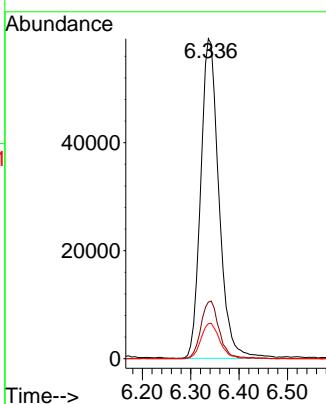

#44

Trichloroethene

Concen: 50.018 ug/l

RT: 7.123 min Scan# 990

Delta R.T. 0.000 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50




Tgt Ion:130 Resp: 55491

Ion Ratio Lower Upper

130 100

95 102.6 0.0 204.2

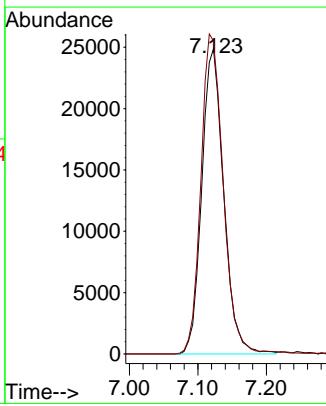



#45

1,2-Dichloropropane

Concen: 51.983 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

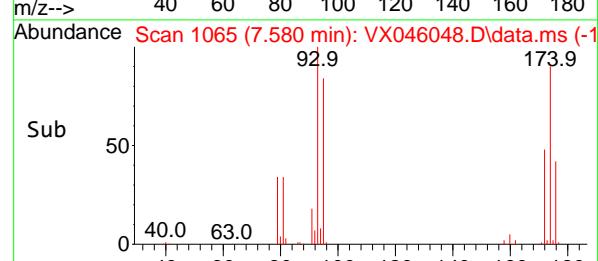

#46

Dibromomethane

Concen: 49.978 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion: 93 Resp: 45181




Ion Ratio Lower Upper

93 100

95 83.0 65.6 98.4

174 84.8 68.2 102.2

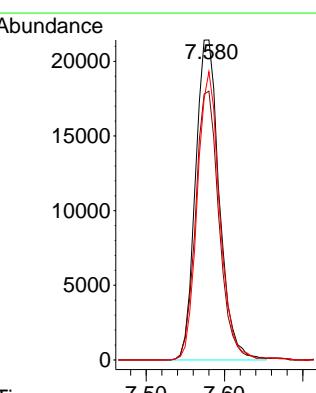



#47

Bromodichloromethane

Concen: 51.889 ug/l

RT: 7.818 min Scan# 1104

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carbone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

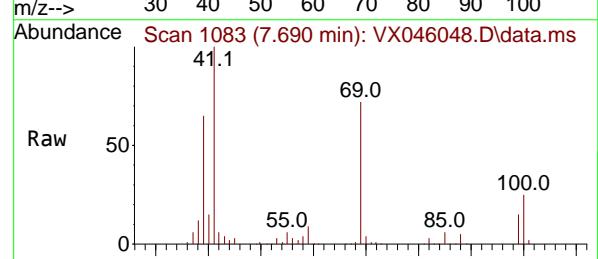

#48

Methyl methacrylate

Concen: 54.226 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion: 41 Resp: 82144


Ion Ratio Lower Upper

41 100


69 70.4 58.5 87.7

39 64.2 51.7 77.5

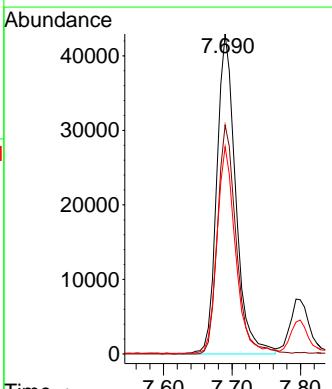





Abundance Scan 1078 (7.659 min): VX046048.D\data.ms

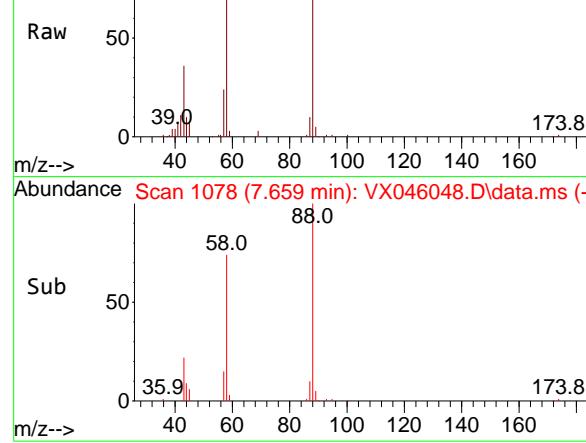


Abundance Scan 1078 (7.659 min): VX046048.D\data.ms (-1)

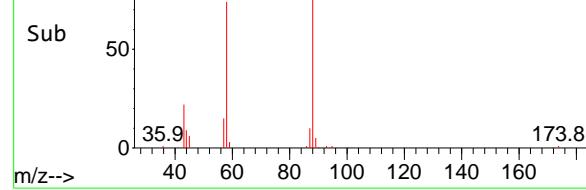


Abundance Scan 1240 (8.647 min): VX046042.D\data.ms (-1)

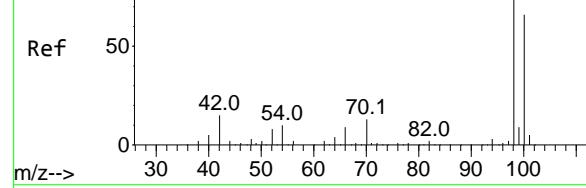

Abundance Scan 1240 (8.647 min): VX046048.D\data.ms

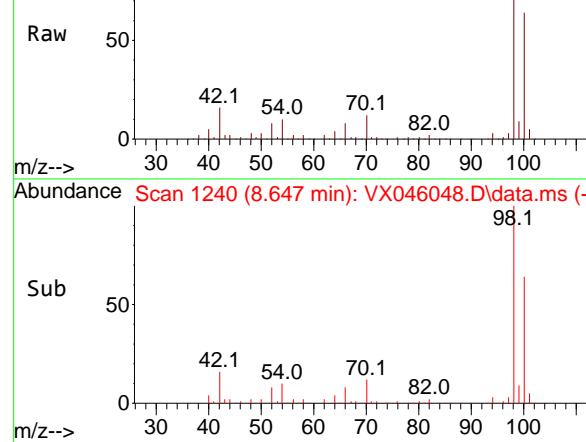

Abundance Scan 1240 (8.647 min): VX046048.D\data.ms (-1)

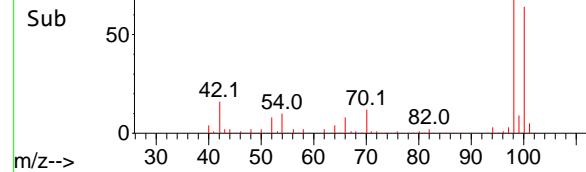

#49

1,4-Dioxane

Concen: 1059.599 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument :

MSVOA\_X


ClientSampleId :

ICVVX050525

### Manual Integrations APPROVED

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

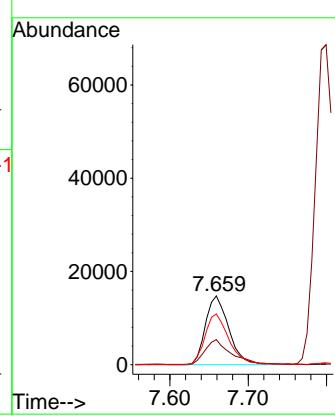

#50

Toluene-d8

Concen: 48.984 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50






Tgt Ion: 98 Resp: 198575

Ion Ratio Lower Upper

98 100

100 65.6 53.5 80.3

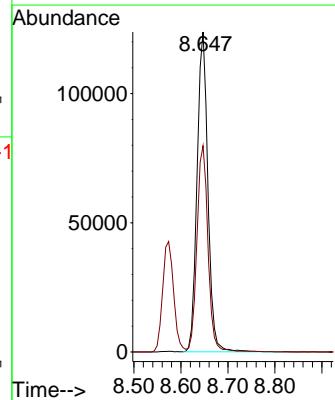

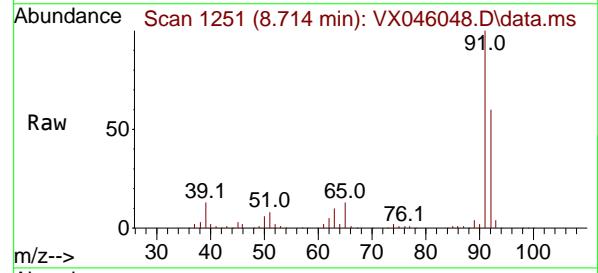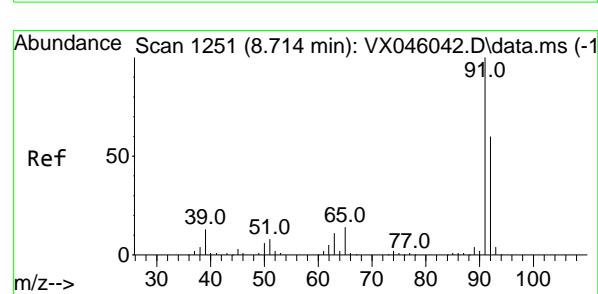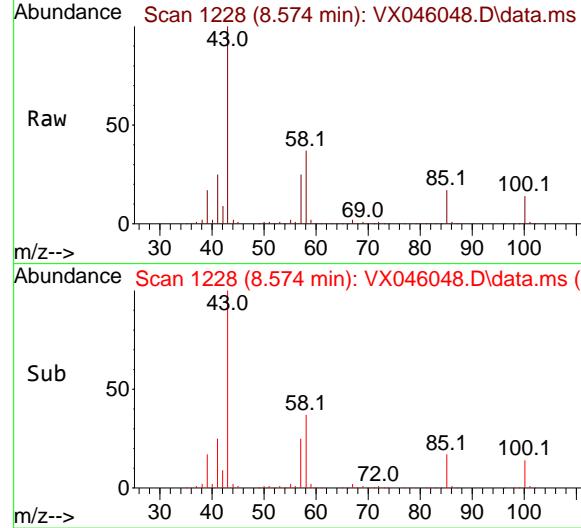

#51

4-Methyl-2-Pentanone

Concen: 259.133 ug/l

RT: 8.574 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument :

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**


Reviewed By :John Carlone 05/06/2025




Supervised By :Mahesh Dadoda 05/06/2025

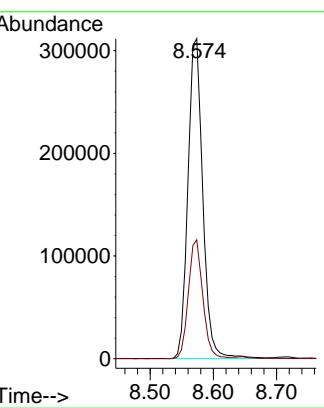

#52  
Toluene  
Concen: 51.150 ug/l  
RT: 8.714 min Scan# 1251  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 92 Resp: 144574  
Ion Ratio Lower Upper  
92 100  
91 171.4 136.6 205.0

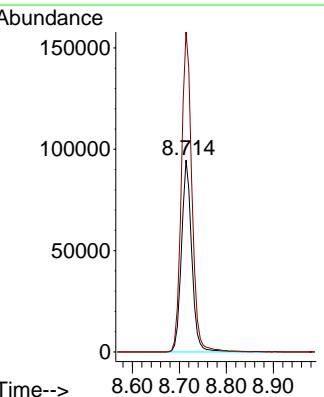



#53

t-1,3-Dichloropropene

Concen: 52.920 ug/l

RT: 8.976 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

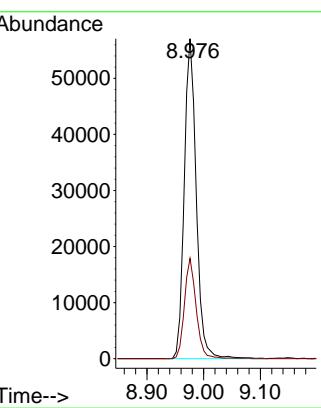

#54

cis-1,3-Dichloropropene

Concen: 52.892 ug/l


RT: 8.360 min Scan# 1193







Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt	Ion	75	100	Ion	Ratio	Lower	Upper
		75	100				
		77	31.5		25.4	38.0	
		39	63.2		52.2	78.4	

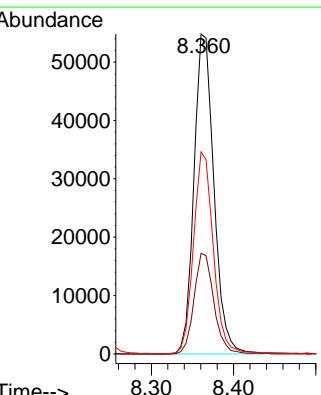



#55

1,1,2-Trichloroethane

Concen: 50.887 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025



Supervised By :Mahesh Dadoda 05/06/2025

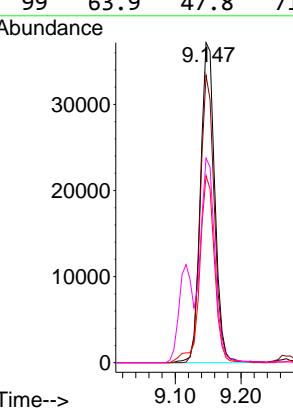

#56  
Ethyl methacrylate  
Concen: 53.918 ug/l  
RT: 9.116 min Scan# 1317  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 69 Resp: 95772  
Ion Ratio Lower Upper  
69 100  
41 76.1 60.8 91.2  
39 47.4 39.0 58.6

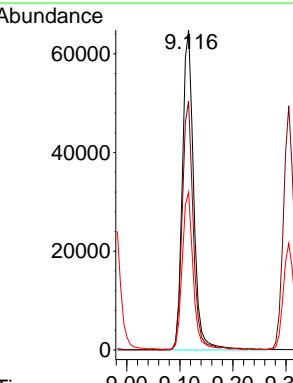

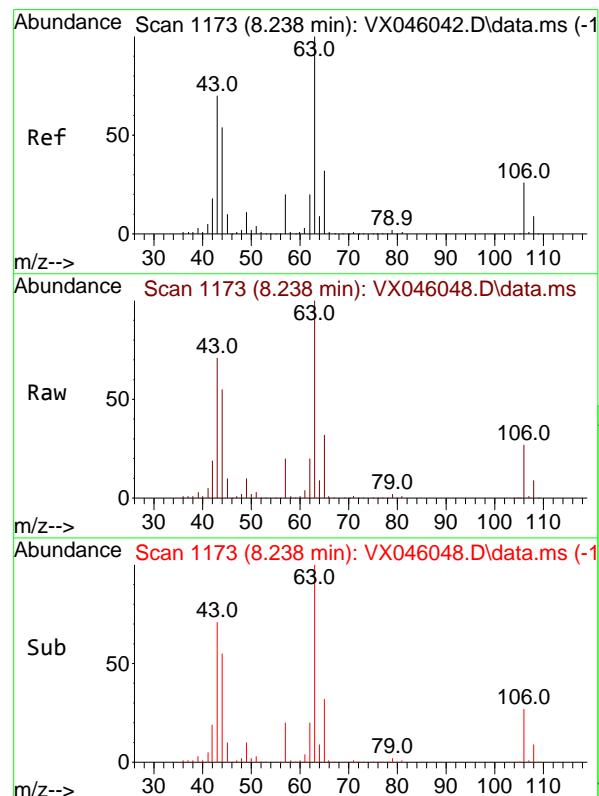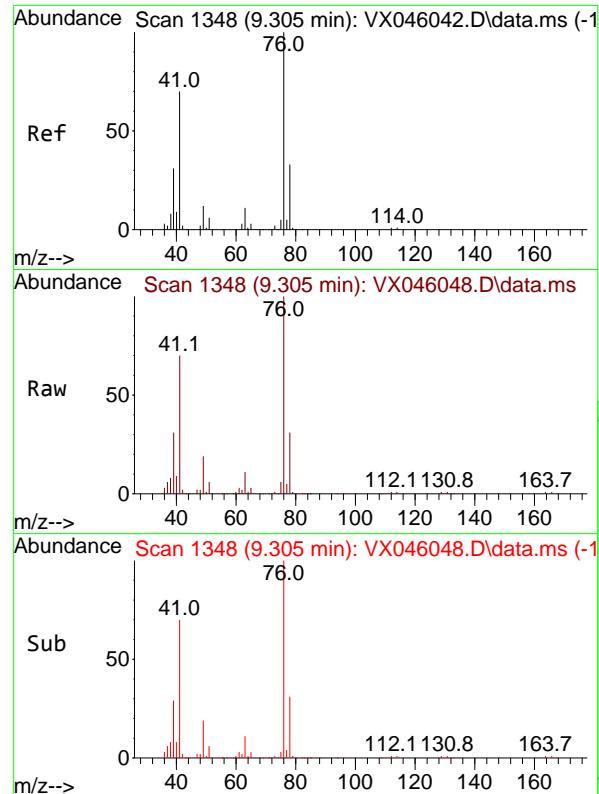

#57

1,3-Dichloropropane

Concen: 49.793 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

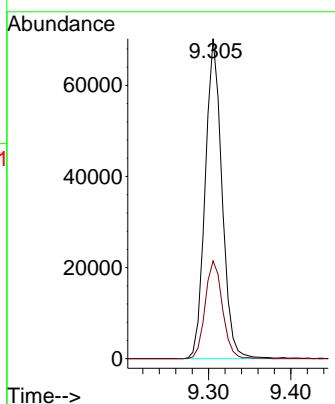

#58

2-Chloroethyl Vinyl ether

Concen: 265.780 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. 0.000 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50







Tgt Ion: 63 Resp: 240681

Ion Ratio Lower Upper

63 100

106 26.6 21.5 32.3

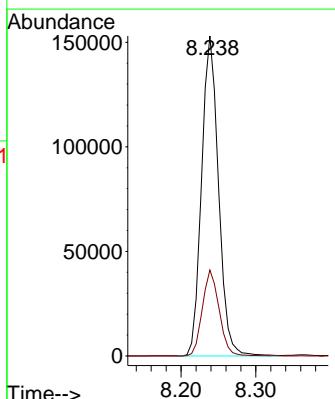

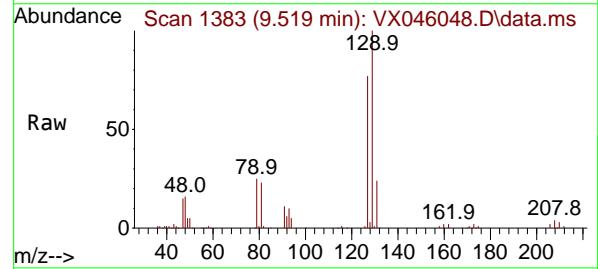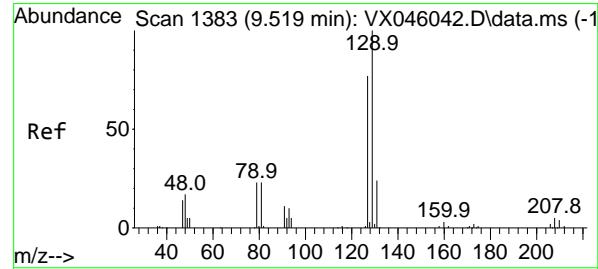

#59

2-Hexanone

Concen: 268.218 ug/l

RT: 9.427 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

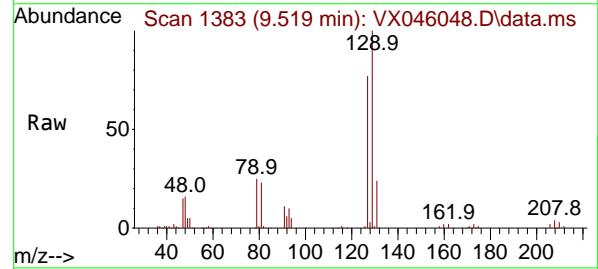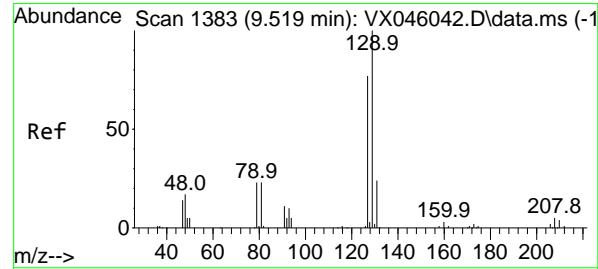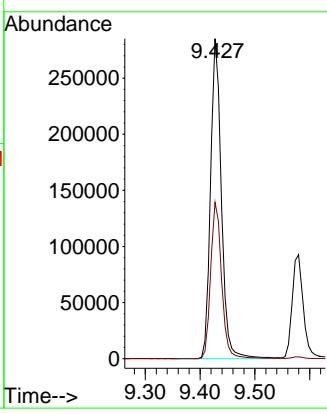

#60

Dibromochloromethane


Concen: 52.075 ug/l




RT: 9.519 min Scan# 1383

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

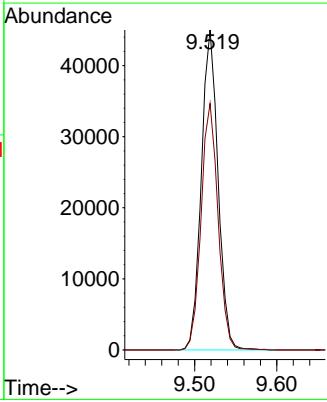 Tgt Ion:129 Resp: 63738  
 Ion Ratio Lower Upper  
 129 100  
 127 77.9 39.3 117.8




#61

1,2-Dibromoethane

Concen: 51.050 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X





ClientSampleId :

ICVVX050525

**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#62

4-Bromofluorobenzene

Concen: 48.596 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion: 95 Resp: 75568




Ion Ratio Lower Upper

95 100

174 68.2 0.0 135.8

176 66.5 0.0 131.4





#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 145073

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50




Instrument : MSVOA\_X

ClientSampleId : ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#64

Tetrachloroethene

Concen: 46.795 ug/l


RT: 9.269 min Scan# 1342


Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt	Ion:164	Resp:	48034
Ion	Ratio	Lower	Upper
164	100		
166	129.9	105.0	157.6
129	105.3	83.5	125.3
131	98.8	76.5	114.7

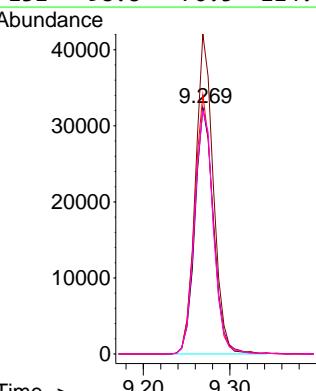


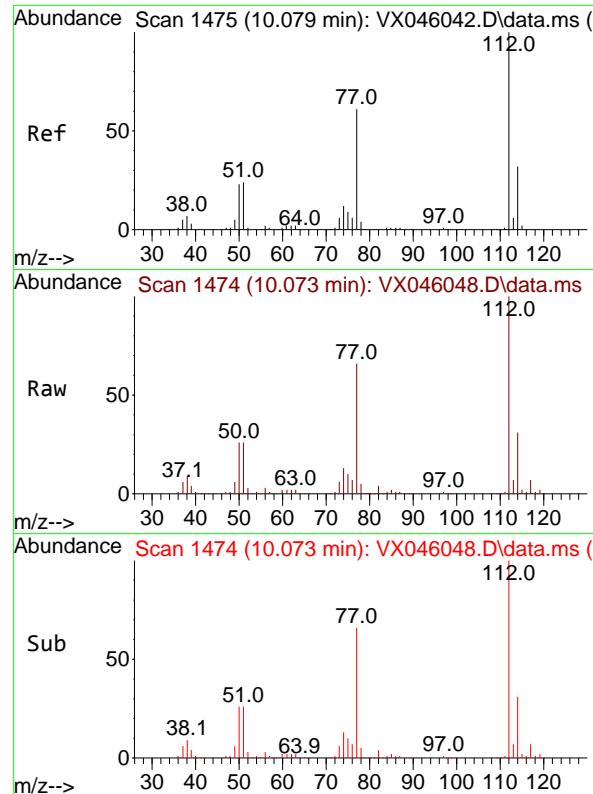


#65  
Chlorobenzene  
Concen: 48.699 ug/l  
RT: 10.073 min Scan# 1474  
Delta R.T. -0.006 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50


Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525




**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

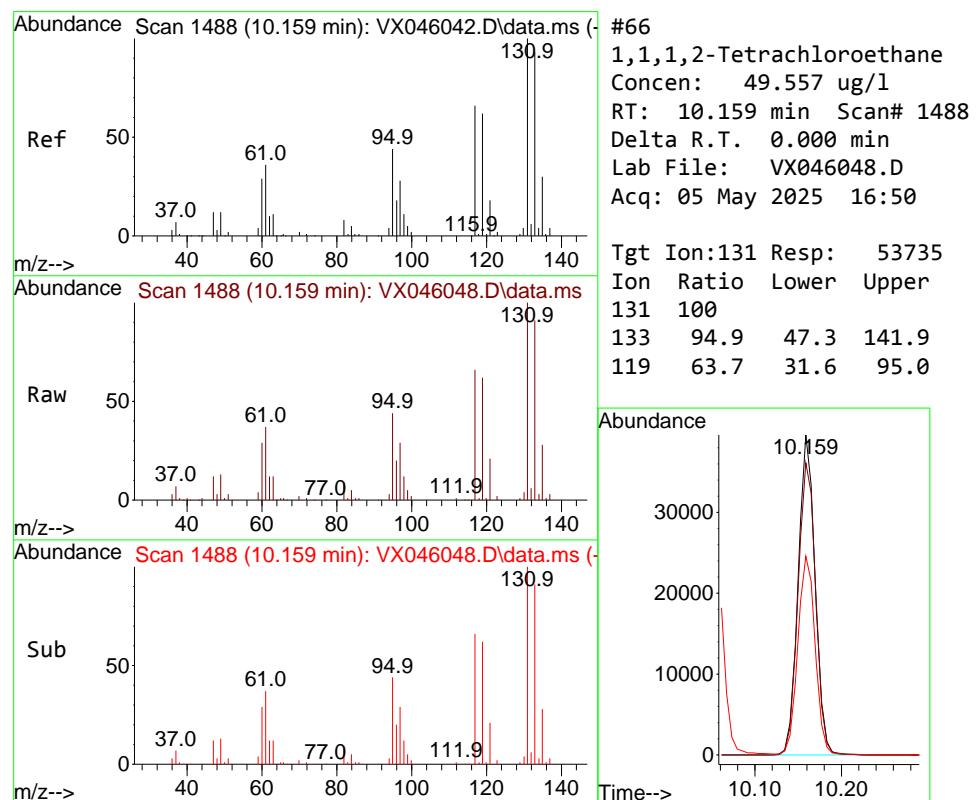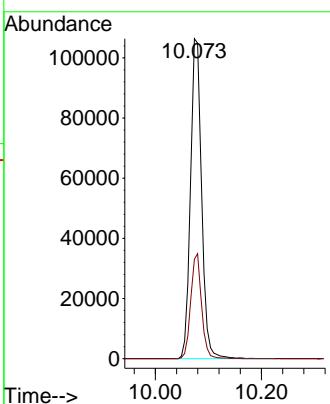

#66  
1,1,1,2-Tetrachloroethane  
Concen: 49.557 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

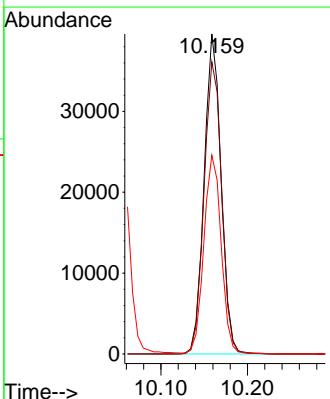



#67

Ethyl Benzene

Concen: 50.245 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#68

m/p-Xylenes

Concen: 101.022 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion:106 Resp: 206813


Ion Ratio Lower Upper

106 100

91 215.6 171.2 256.8

Time--&gt; 10.10 10.20 10.30 10.40


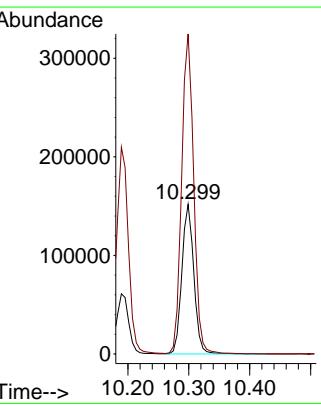


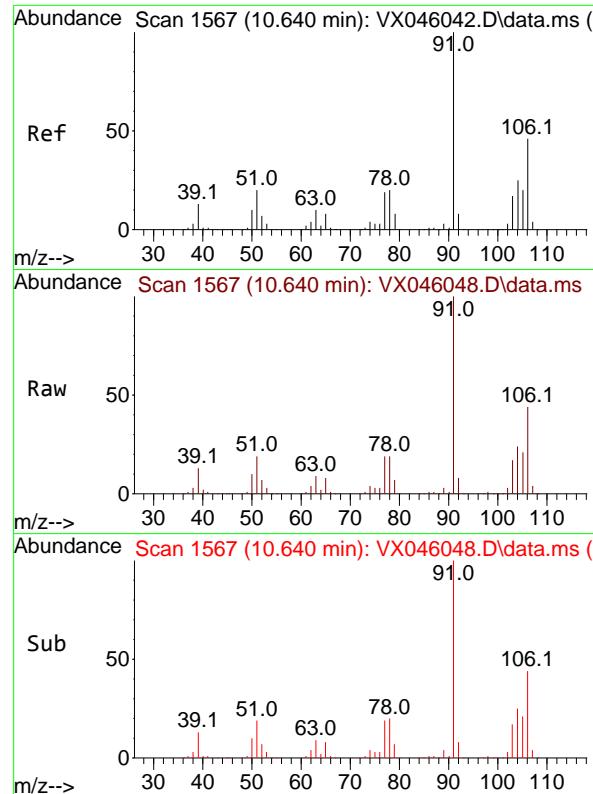

#69  
o-Xylene  
Concen: 50.841 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50  
ClientSampleId : ICVVX050525


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

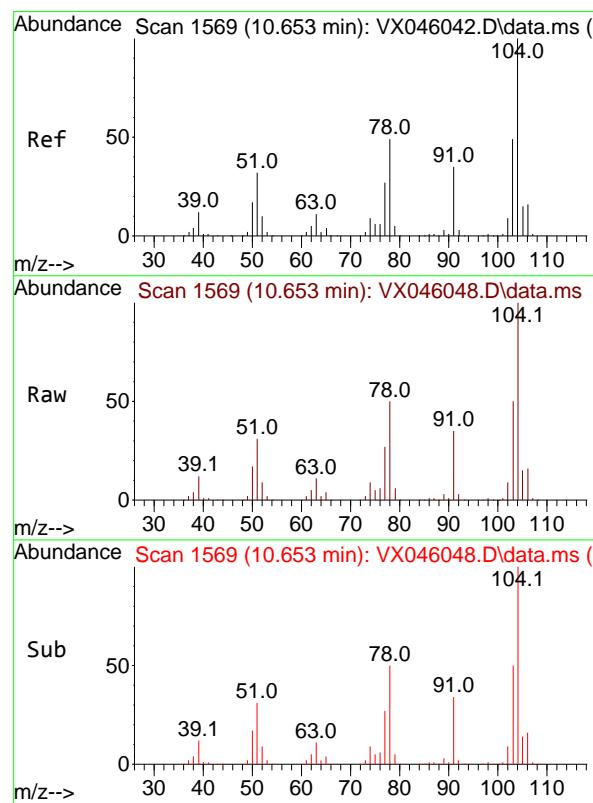

#70  
Styrene  
Concen: 51.907 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion:104 Resp: 169703  
Ion Ratio Lower Upper  
104 100  
78 57.6 45.7 68.5  
103 55.5 43.7 65.5



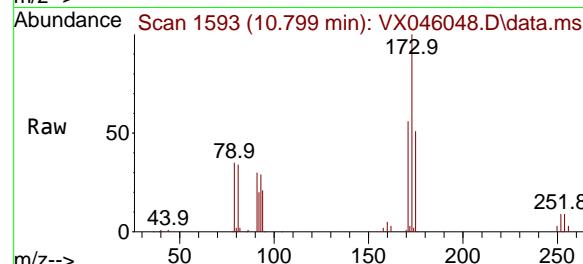

#71

Bromoform

Concen: 49.583 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion:152 Resp: 68229


Ion Ratio Lower Upper

152 100

115 93.3 46.9 140.7

150 175.3 0.0 351.0

12 10.799

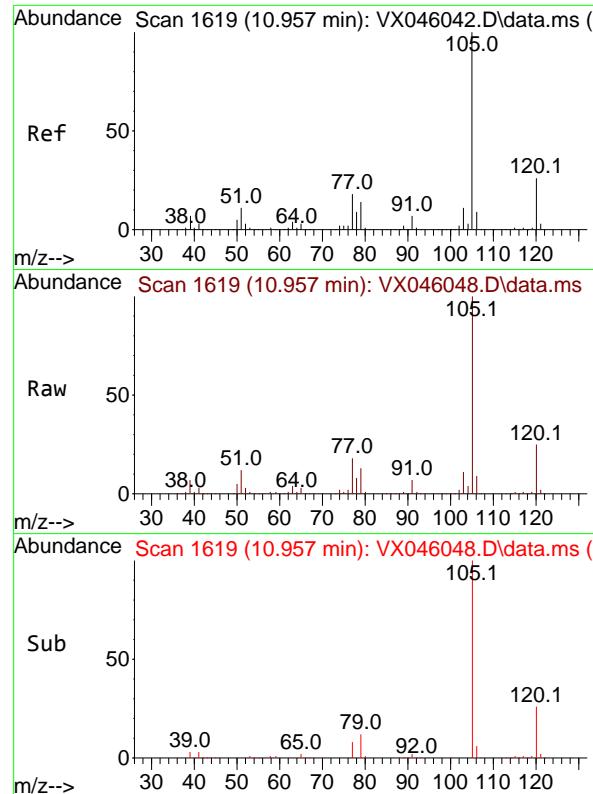

#73

Isopropylbenzene

Concen: 50.733 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

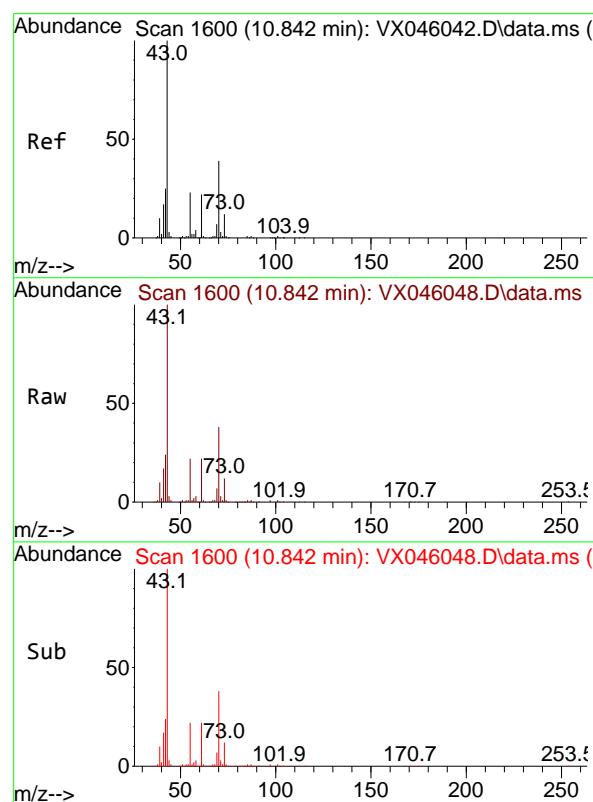

#74

N-amyl acetate

Concen: 52.407 ug/l

RT: 10.842 min Scan# 1600

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Abundance



Scan 1600 (10.842 min): VX046048.D\data.ms (-)

Time--&gt;

Abundance

Scan 1600 (10.842 min): VX046048.D\data.ms (-)

Time--&gt;

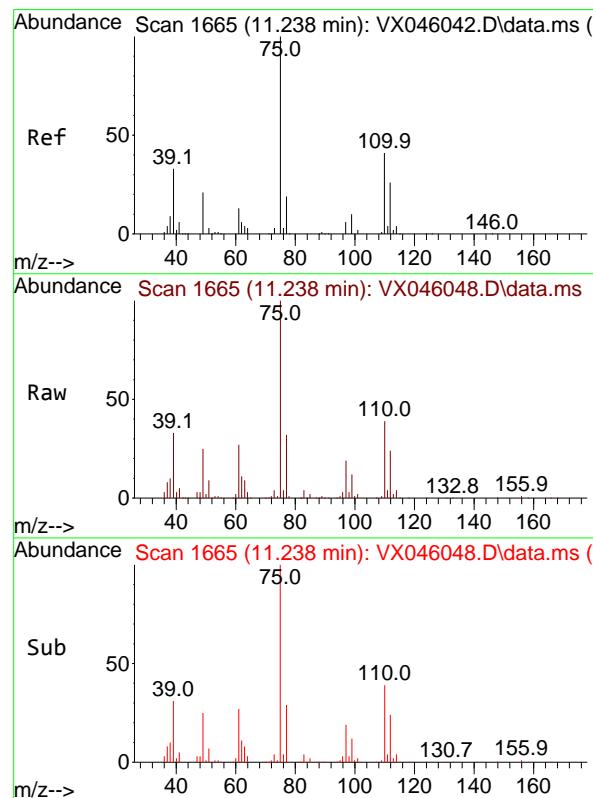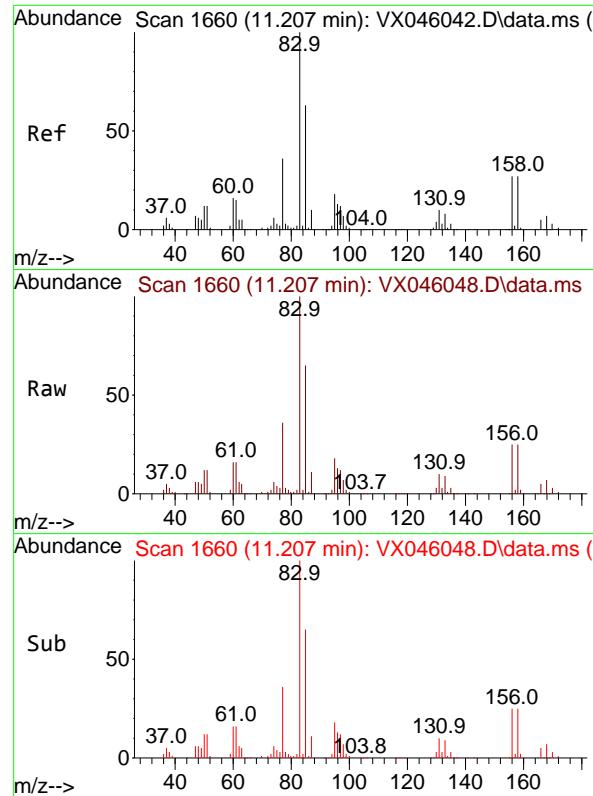


#75  
1,1,2,2-Tetrachloroethane  
Concen: 47.827 ug/l  
RT: 11.207 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525


### Manual Integrations APPROVED




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

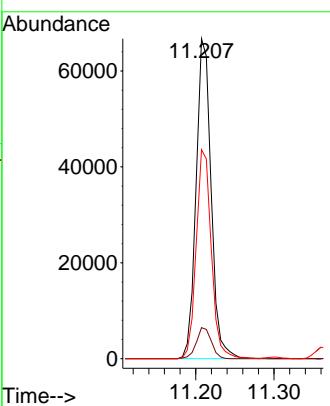

#76  
1,2,3-Trichloropropane  
Concen: 48.568 ug/l  
RT: 11.238 min Scan# 1665  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 75 Resp: 79763  
Ion Ratio Lower Upper  
75 100  
77 40.8 20.5 61.5

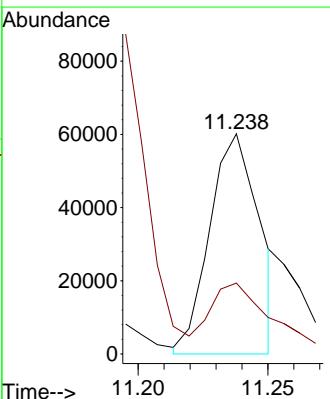



#77

Bromobenzene

Concen: 48.549 ug/l

RT: 11.195 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

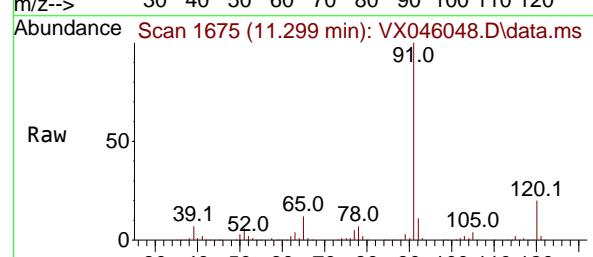

#78

n-propylbenzene

Concen: 50.562 ug/l

RT: 11.299 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VX046048.D


Acq: 05 May 2025 16:50




Tgt Ion: 91 Resp: 312285

Ion Ratio Lower Upper

91 100

120 21.4 10.8 32.4

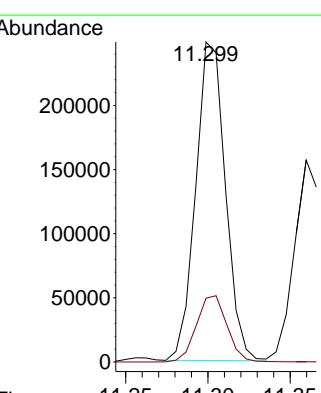



#79

2-Chlorotoluene

Concen: 49.107 ug/l

RT: 11.360 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X




ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

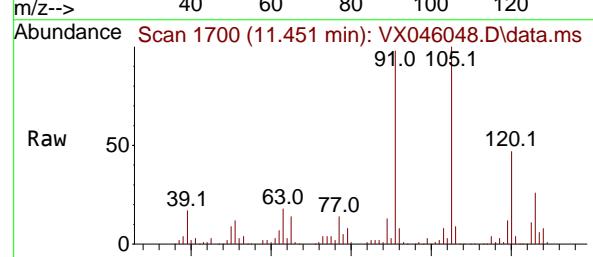

#80

1,3,5-Trimethylbenzene

Concen: 51.500 ug/l



RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion:105 Resp: 228538  
 Ion Ratio Lower Upper  
 105 100  
 120 46.3 23.1 69.2

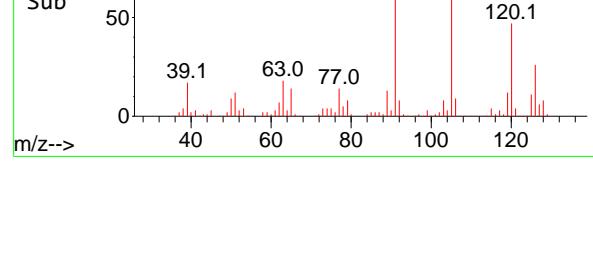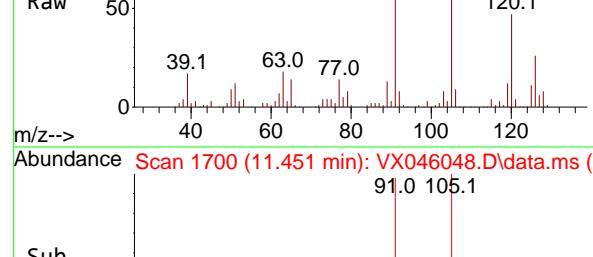


Abundance

11.451

Time--&gt;

11.40 11.45 11.50 11.55 11.60


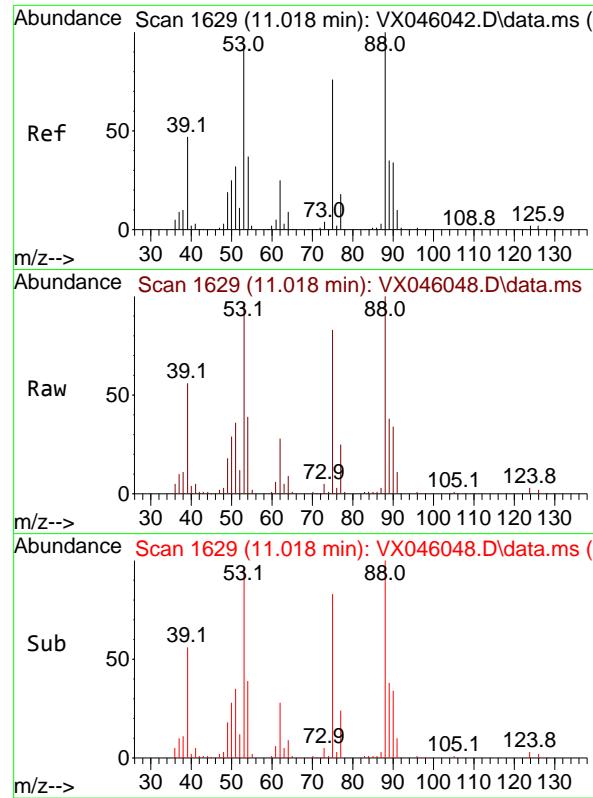


#81  
trans-1,4-Dichloro-2-butene  
Concen: 49.276 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525


**Manual Integrations**  
**APPROVED**




Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

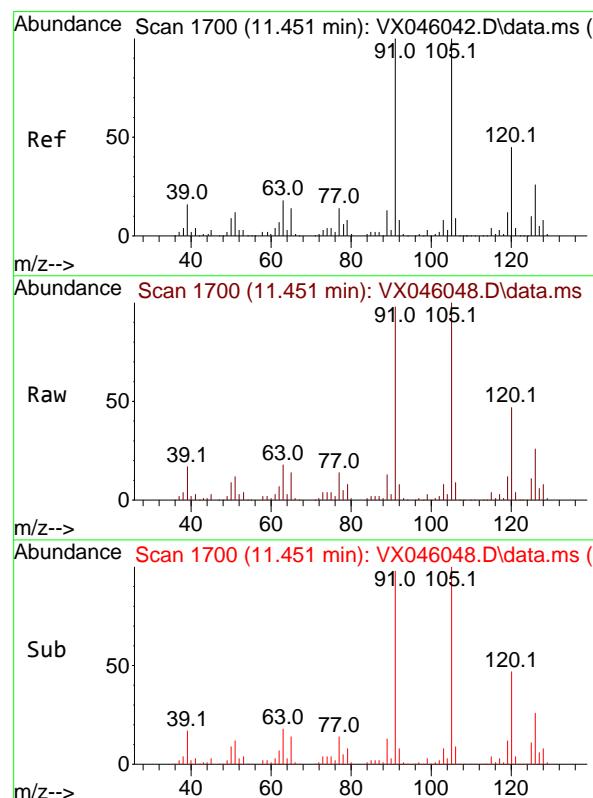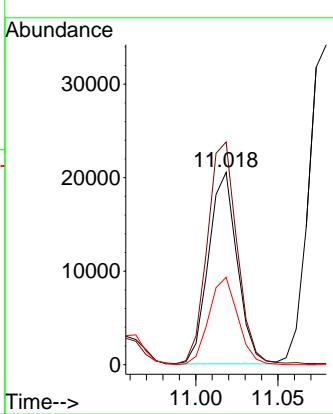

#82  
4-Chlorotoluene  
Concen: 50.661 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion: 91 Resp: 223811  
Ion Ratio Lower Upper  
91 100  
126 26.5 13.3 39.8

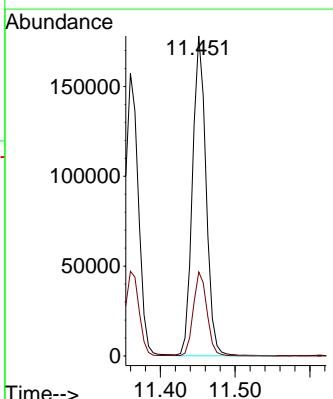



#83

tert-Butylbenzene

Concen: 50.511 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50





Instrument:

MSVOA\_X

ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

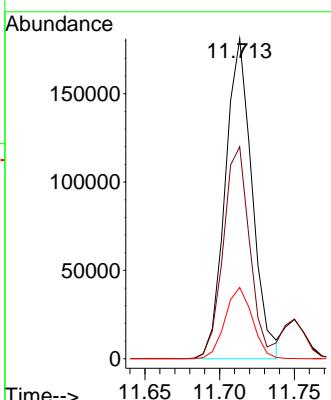 Reviewed By :John Carlone 05/06/2025  
 Supervised By :Mahesh Dadoda 05/06/2025


#84

1,2,4-Trimethylbenzene


Concen: 51.485 ug/l


RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min


Lab File: VX046048.D

Acq: 05 May 2025 16:50

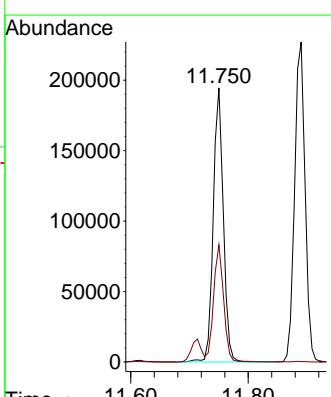
 Tgt Ion:105 Resp: 231371  
 Ion Ratio Lower Upper  
 105 100  
 120 42.3 21.2 63.6




Abundance Scan 1772 (11.890 min): VX046048.D\data.ms (-)

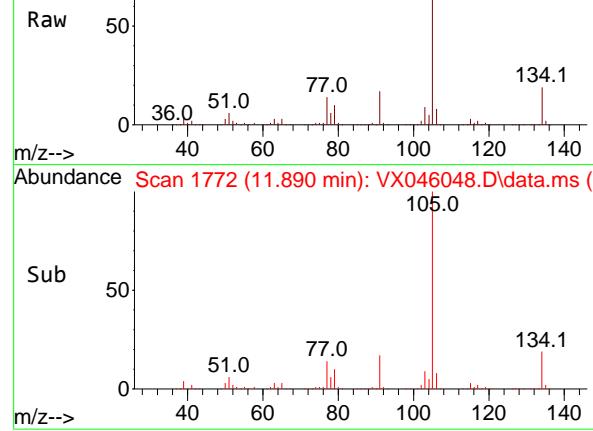

Abundance Scan 1772 (11.890 min): VX046048.D\data.ms (-)

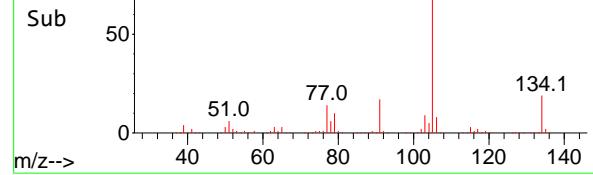

#85

sec-Butylbenzene

Concen: 51.122 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:


MSVOA\_X

ClientSampleId :

ICVVX050525

Manual Integrations  
APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

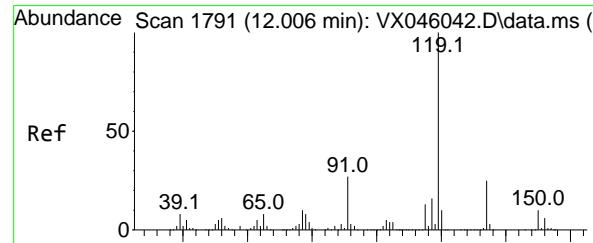

Abundance Scan 1791 (12.006 min): VX046048.D\data.ms (-)



Abundance Scan 1791 (12.006 min): VX046048.D\data.ms (-)

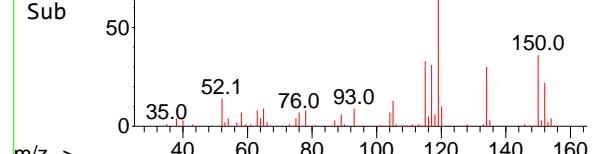

#86

p-Isopropyltoluene

Concen: 51.198 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt Ion:119 Resp: 231942


Ion Ratio Lower Upper

119 100

134 25.0 12.5 37.5

91 27.5 13.8 41.4

VX046048.D 82X050525W.M

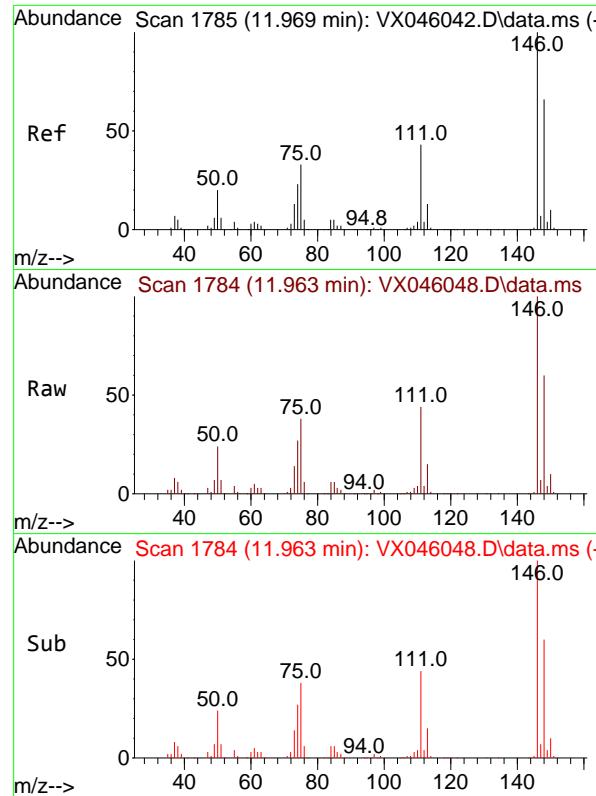

#87

1,3-Dichlorobenzene

Concen: 50.272 ug/l

RT: 11.963 min Scan# 1784

Delta R.T. -0.006 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X



ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

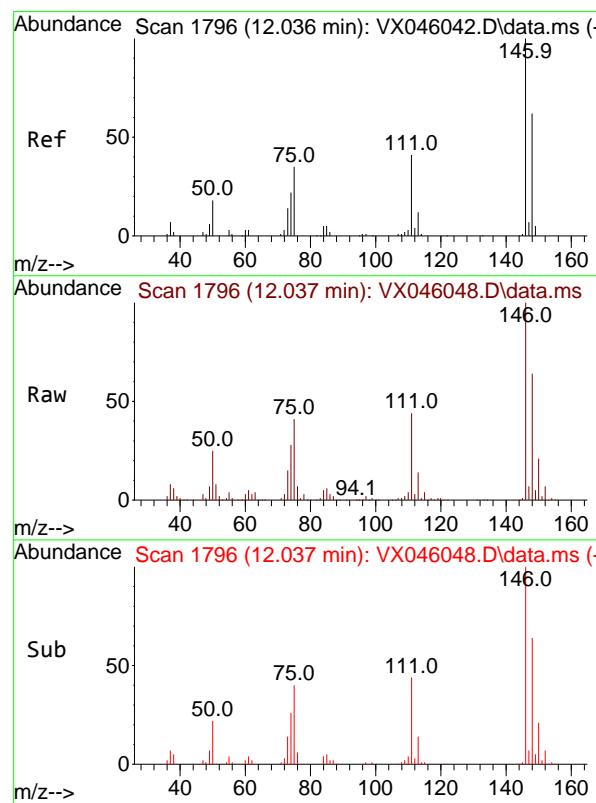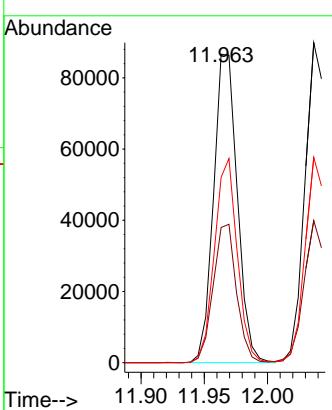

#88

1,4-Dichlorobenzene

Concen: 48.368 ug/l


RT: 12.037 min Scan# 1796




Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt	Ion:146	Resp:	111173
Ion	Ratio	Lower	Upper
146	100		
111	43.9	21.3	63.9
148	63.3	31.9	95.5





#89

n-Butylbenzene

Concen: 51.804 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50





Instrument : MSVOA\_X

ClientSampleId : ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

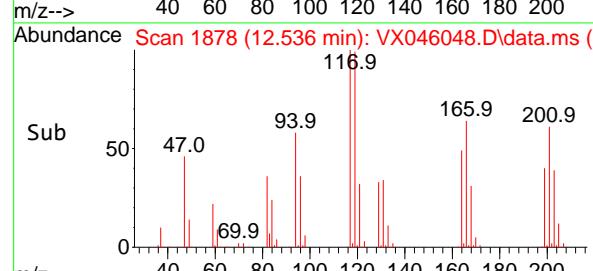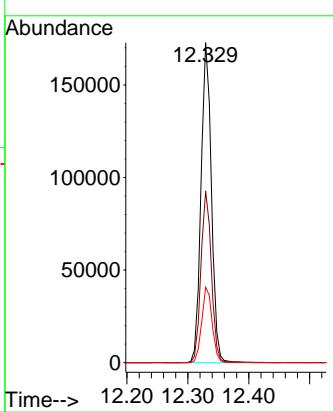

#90

Hexachloroethane

Concen: 49.895 ug/l


RT: 12.536 min Scan# 1878


Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Tgt	Ion	Ion Ratio	Lower	Upper
	117	100		
	201	62.4	31.6	94.7

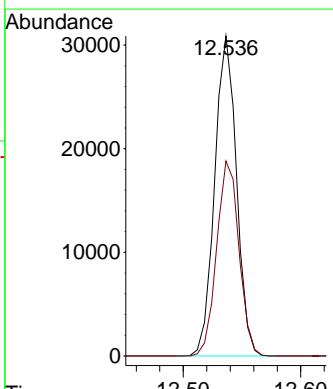

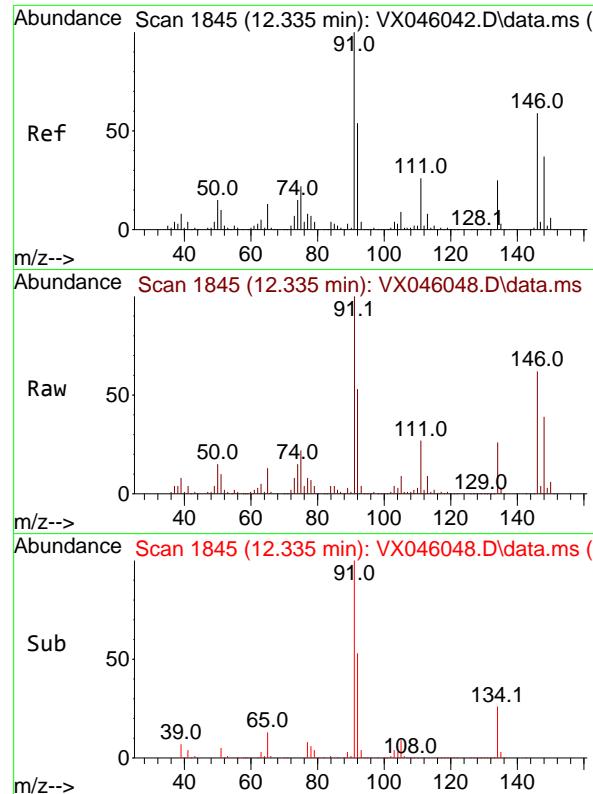

#91

1,2-Dichlorobenzene

Concen: 49.361 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50

Instrument:

MSVOA\_X


ClientSampleId :

ICVVX050525

**Manual Integrations  
APPROVED**

Reviewed By :John Carlone 05/06/2025

Supervised By :Mahesh Dadoda 05/06/2025

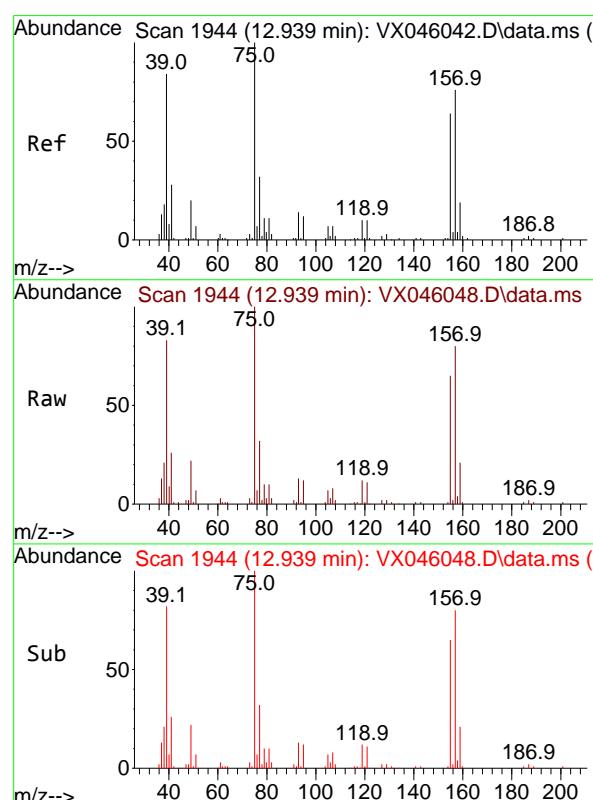

#92

1,2-Dibromo-3-Chloropropane

Concen: 51.458 ug/l

RT: 12.939 min Scan# 1944

Delta R.T. 0.000 min

Lab File: VX046048.D

Acq: 05 May 2025 16:50


Tgt Ion: 75 Resp: 21220


Ion Ratio Lower Upper

75 100

155 68.6 34.9 104.8

157 86.7 43.8 131.4

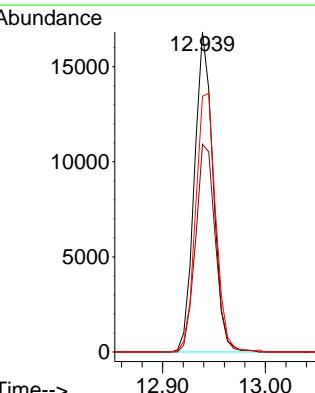


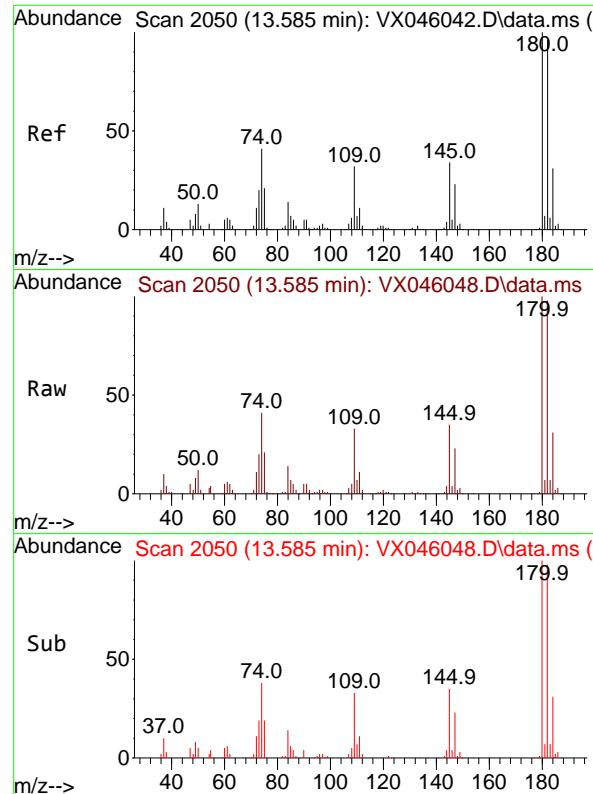


#93  
1,2,4-Trichlorobenzene  
Concen: 49.662 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525


### Manual Integrations APPROVED


Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

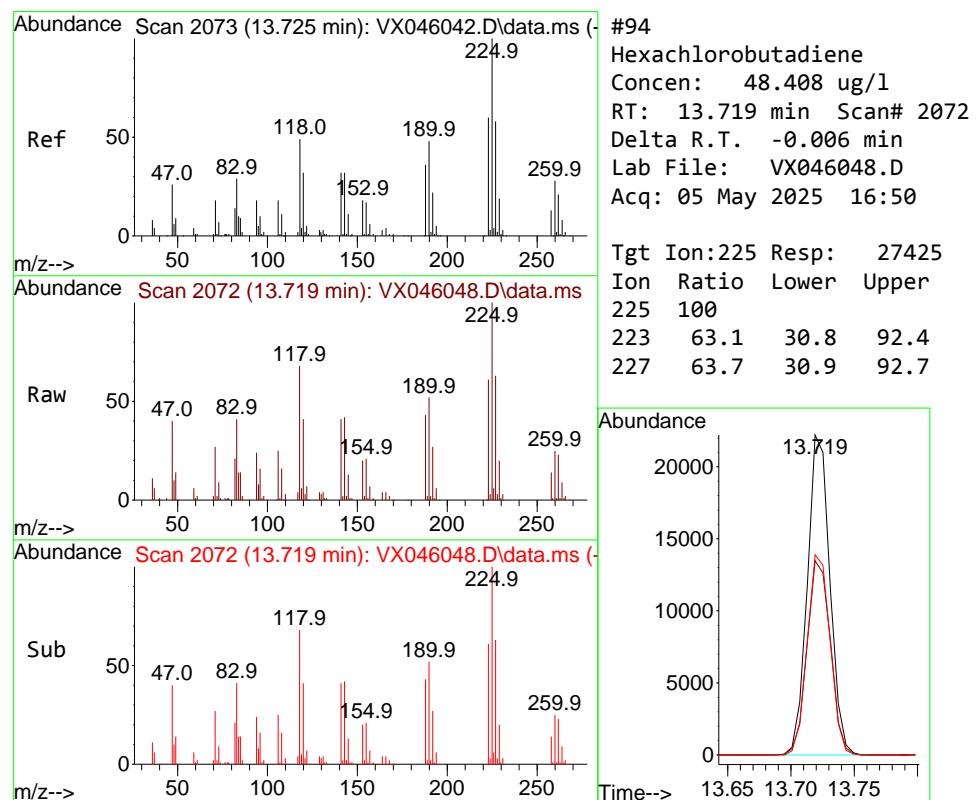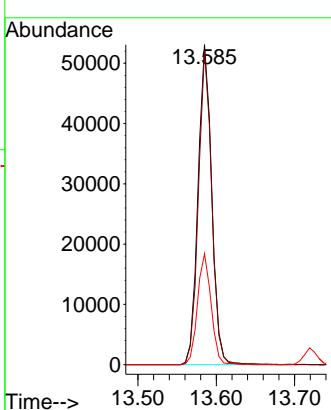

#94  
Hexachlorobutadiene  
Concen: 48.408 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. -0.006 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion:225 Resp: 27425  
Ion Ratio Lower Upper  
225 100  
223 63.1 30.8 92.4  
227 63.7 30.9 92.7

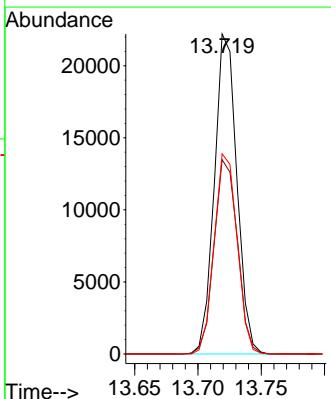


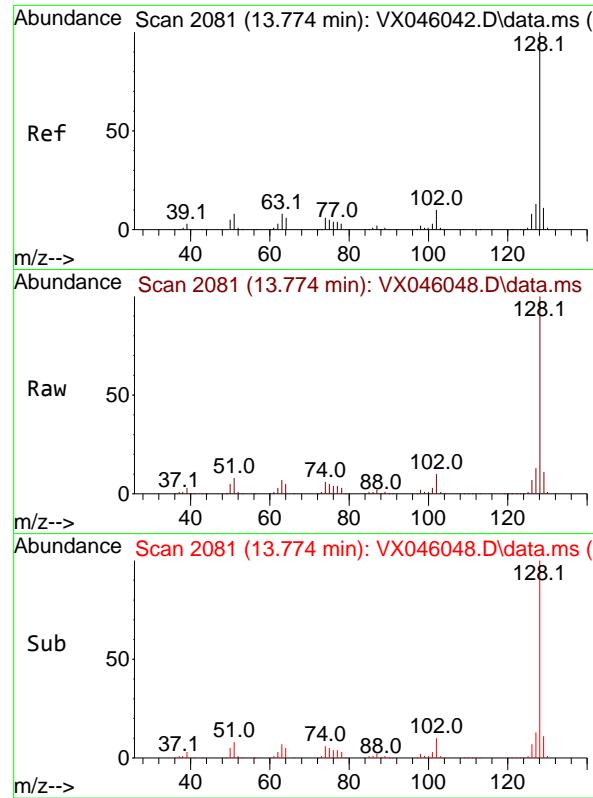


#95  
Naphthalene  
Concen: 50.404 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Instrument : MSVOA\_X  
ClientSampleId : ICVVX050525


**Manual Integrations**  
**APPROVED**

Reviewed By :John Carlone 05/06/2025  
Supervised By :Mahesh Dadoda 05/06/2025

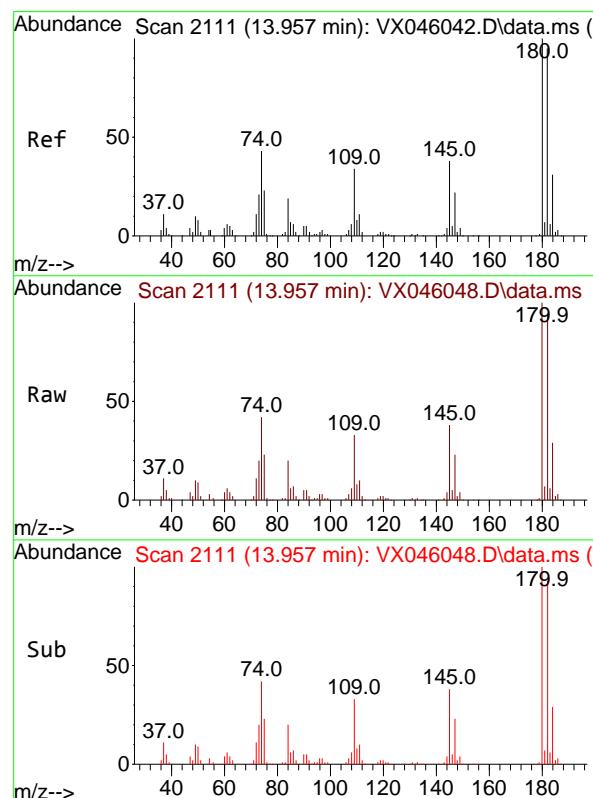

#96  
1,2,3-Trichlorobenzene  
Concen: 48.525 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046048.D  
Acq: 05 May 2025 16:50

Tgt Ion:180 Resp: 64950  
Ion Ratio Lower Upper  
180 100  
182 97.0 47.8 143.3  
145 37.5 18.1 54.3

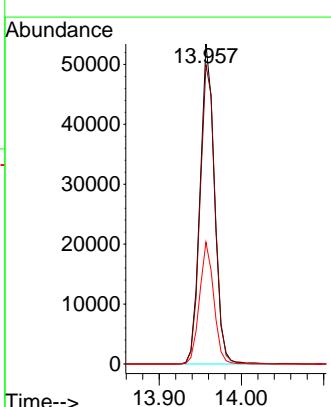

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046048.D  
 Acq On : 05 May 2025 16:50  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX050525**

Quant Time: May 06 07:17:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	95	0.00
2 T	Dichlorodifluoromethane	0.765	0.851	-11.2	94	0.00
3 P	Chloromethane	0.742	0.781	-5.3	96	0.00
4 C	Vinyl Chloride	0.691	0.713	-3.2#	96	0.00
5 T	Bromomethane	0.320	0.324	-1.3	95	0.00
6 T	Chloroethane	0.369	0.385	-4.3	97	0.00
7 T	Trichlorofluoromethane	1.021	1.073	-5.1	96	0.00
8 T	Diethyl Ether	0.347	0.344	0.9	97	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.632	0.642	-1.6	96	0.00
10 T	Methyl Iodide	0.747	0.799	-7.0	94	0.00
11 T	Tert butyl alcohol	0.131	0.132	-0.8	98	0.00
12 CM	1,1-Dichloroethene	0.593	0.606	-2.2#	96	0.00
13 T	Acrolein	0.149	0.139	6.7	87	0.00
14 T	Allyl chloride	1.133	1.175	-3.7	95	0.00
15 T	Acrylonitrile	0.374	0.393	-5.1	97	0.00
16 T	Acetone	0.374	0.367	1.9	97	0.00
17 T	Carbon Disulfide	1.406	1.433	-1.9	94	0.00
18 T	Methyl Acetate	0.867	0.867	0.0	97	0.00
19 T	Methyl tert-butyl Ether	2.079	2.111	-1.5	93	0.00
20 T	Methylene Chloride	0.716	0.684	4.5	95	0.00
21 T	trans-1,2-Dichloroethene	0.596	0.602	-1.0	94	0.00
22 T	Diisopropyl ether	2.189	2.268	-3.6	95	0.00
23 T	Vinyl Acetate	1.925	2.045	-6.2	95	0.00
24 P	1,1-Dichloroethane	1.219	1.239	-1.6	94	0.00
25 T	2-Butanone	0.543	0.558	-2.8	96	0.00
26 T	2,2-Dichloropropane	0.954	0.953	0.1	95	0.00
27 T	cis-1,2-Dichloroethene	0.718	0.731	-1.8	95	0.00
28 T	Bromochloromethane	0.587	0.598	-1.9	99	0.00
29 T	Tetrahydrofuran	0.340	0.354	-4.1	96	0.00
30 C	Chloroform	1.271	1.305	-2.7#	96	0.00
31 T	Cyclohexane	1.111	1.114	-0.3	94	0.00
32 T	1,1,1-Trichloroethane	1.101	1.126	-2.3	95	0.00
33 S	1,2-Dichloroethane-d4	0.932	0.904	3.0	95	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	97	0.00
35 S	Dibromofluoromethane	0.360	0.358	0.6	98	0.00
36 T	1,1-Dichloropropene	0.484	0.479	1.0	94	0.00
37 T	Ethyl Acetate	0.598	0.606	-1.3	96	0.00
38 T	Carbon Tetrachloride	0.544	0.542	0.4	94	0.00
39 T	Methylcyclohexane	0.623	0.620	0.5	94	0.00
40 TM	Benzene	1.417	1.439	-1.6	95	0.00
41 T	Methacrylonitrile	0.313	0.344	-9.9	96	0.00
42 TM	1,2-Dichloroethane	0.612	0.622	-1.6	96	0.00
43 T	Isopropyl Acetate	0.912	0.952	-4.4	96	0.00
44 TM	Trichloroethene	0.341	0.341	0.0	93	0.00
45 C	1,2-Dichloropropane	0.352	0.366	-4.0#	96	0.00
46 T	Dibromomethane	0.278	0.278	0.0	94	0.00
47 T	Bromodichloromethane	0.547	0.568	-3.8	95	0.00
48 T	Methyl methacrylate	0.466	0.505	-8.4	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046048.D  
 Acq On : 05 May 2025 16:50  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX050525**

Quant Time: May 06 07:17:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.009	0.009	0.0	100	0.00
50 S	Toluene-d8	1.246	1.221	2.0	97	0.00
51 T	4-Methyl-2-Pentanone	0.605	0.627	-3.6	96	0.00
52 CM	Toluene	0.869	0.889	-2.3#	96	0.00
53 T	t-1,3-Dichloropropene	0.487	0.515	-5.7	94	0.00
54 T	cis-1,3-Dichloropropene	0.538	0.569	-5.8	95	0.00
55 T	1,1,2-Trichloroethane	0.343	0.349	-1.7	95	0.00
56 T	Ethyl methacrylate	0.546	0.589	-7.9	96	0.00
57 T	1,3-Dichloropropane	0.615	0.613	0.3	95	0.00
58 T	2-Chloroethyl Vinyl ether	0.278	0.296	-6.5	93	0.00
59 T	2-Hexanone	0.448	0.480	-7.1	98	0.00
60 T	Dibromochloromethane	0.376	0.392	-4.3	95	0.00
61 T	1,2-Dibromoethane	0.356	0.364	-2.2	94	0.00
62 S	4-Bromofluorobenzene	0.478	0.465	2.7	96	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	99	0.00
64 T	Tetrachloroethene	0.354	0.331	6.5	88	0.00
65 PM	Chlorobenzene	1.094	1.066	2.6	96	0.00
66 T	1,1,1,2-Tetrachloroethane	0.374	0.370	1.1	94	0.00
67 C	Ethyl Benzene	1.929	1.939	-0.5#	95	0.00
68 T	m/p-Xylenes	0.706	0.713	-1.0	95	0.00
69 T	o-Xylene	0.688	0.699	-1.6	95	0.00
70 T	Styrene	1.127	1.170	-3.8	95	0.00
71 P	Bromoform	0.281	0.278	1.1	91	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	100	0.00
73 T	Isopropylbenzene	3.893	3.950	-1.5	96	0.00
74 T	N-amyl acetate	1.924	2.016	-4.8	98	0.00
75 P	1,1,2,2-Tetrachloroethane	1.364	1.305	4.3	98	0.00
76 T	1,2,3-Trichloropropane	1.204	1.169	2.9	99	0.00
77 T	Bromobenzene	0.904	0.878	2.9	95	0.00
78 T	n-propylbenzene	4.526	4.577	-1.1	95	0.00
79 T	2-Chlorotoluene	2.919	2.867	1.8	96	0.00
80 T	1,3,5-Trimethylbenzene	3.252	3.350	-3.0	96	0.00
81 T	trans-1,4-Dichloro-2-butene	0.370	0.364	1.6	95	0.00
82 T	4-Chlorotoluene	3.238	3.280	-1.3	96	0.00
83 T	tert-Butylbenzene	3.276	3.309	-1.0	97	0.00
84 T	1,2,4-Trimethylbenzene	3.293	3.391	-3.0	97	0.00
85 T	sec-Butylbenzene	4.022	4.112	-2.2	96	0.00
86 T	p-Isopropyltoluene	3.320	3.399	-2.4	96	0.00
87 T	1,3-Dichlorobenzene	1.649	1.658	-0.5	98	0.00
88 T	1,4-Dichlorobenzene	1.684	1.629	3.3	97	0.00
89 T	n-Butylbenzene	2.912	3.017	-3.6	96	0.00
90 T	Hexachloroethane	0.585	0.584	0.2	94	0.00
91 T	1,2-Dichlorobenzene	1.655	1.634	1.3	97	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.302	0.311	-3.0	97	0.00
93 T	1,2,4-Trichlorobenzene	0.951	0.944	0.7	97	0.00
94 T	Hexachlorobutadiene	0.415	0.402	3.1	95	0.00
95 T	Naphthalene	3.487	3.515	-0.8	98	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046048.D  
Acq On : 05 May 2025 16:50  
Operator : JC/MD  
Sample : VSTDICV050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
ICVVX050525

Quant Time: May 06 07:17:12 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	0.981	0.952	3.0	94	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046048.D  
 Acq On : 05 May 2025 16:50  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 ICVVX050525

Quant Time: May 06 07:17:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	95	0.00
2 T	Dichlorodifluoromethane	50.000	55.594	-11.2	94	0.00
3 P	Chloromethane	50.000	52.592	-5.2	96	0.00
4 C	Vinyl Chloride	50.000	51.598	-3.2#	96	0.00
5 T	Bromomethane	50.000	50.627	-1.3	95	0.00
6 T	Chloroethane	50.000	52.271	-4.5	97	0.00
7 T	Trichlorofluoromethane	50.000	52.560	-5.1	96	0.00
8 T	Diethyl Ether	50.000	49.536	0.9	97	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	50.822	-1.6	96	0.00
10 T	Methyl Iodide	50.000	53.419	-6.8	94	0.00
11 T	Tert butyl alcohol	250.000	252.025	-0.8	98	0.00
12 CM	1,1-Dichloroethene	50.000	51.097	-2.2#	96	0.00
13 T	Acrolein	250.000	232.505	7.0	87	0.00
14 T	Allyl chloride	50.000	51.833	-3.7	95	0.00
15 T	Acrylonitrile	250.000	262.412	-5.0	97	0.00
16 T	Acetone	250.000	245.518	1.8	97	0.00
17 T	Carbon Disulfide	50.000	50.981	-2.0	94	0.00
18 T	Methyl Acetate	50.000	49.968	0.1	97	0.00
19 T	Methyl tert-butyl Ether	50.000	50.777	-1.6	93	0.00
20 T	Methylene Chloride	50.000	47.779	4.4	95	0.00
21 T	trans-1,2-Dichloroethene	50.000	50.513	-1.0	94	0.00
22 T	Diisopropyl ether	50.000	51.800	-3.6	95	0.00
23 T	Vinyl Acetate	250.000	265.585	-6.2	95	0.00
24 P	1,1-Dichloroethane	50.000	50.825	-1.7	94	0.00
25 T	2-Butanone	250.000	257.110	-2.8	96	0.00
26 T	2,2-Dichloropropane	50.000	49.934	0.1	95	0.00
27 T	cis-1,2-Dichloroethene	50.000	50.956	-1.9	95	0.00
28 T	Bromochloromethane	50.000	50.975	-2.0	99	0.00
29 T	Tetrahydrofuran	250.000	259.958	-4.0	96	0.00
30 C	Chloroform	50.000	51.332	-2.7#	96	0.00
31 T	Cyclohexane	50.000	50.147	0.3	94	0.00
32 T	1,1,1-Trichloroethane	50.000	51.108	-2.2	95	0.00
33 S	1,2-Dichloroethane-d4	50.000	48.509	3.0	95	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	97	0.00
35 S	Dibromofluoromethane	50.000	49.683	0.6	98	0.00
36 T	1,1-Dichloropropene	50.000	49.521	1.0	94	0.00
37 T	Ethyl Acetate	50.000	50.714	-1.4	96	0.00
38 T	Carbon Tetrachloride	50.000	49.825	0.3	94	0.00
39 T	Methylcyclohexane	50.000	49.757	0.5	94	0.00
40 TM	Benzene	50.000	50.759	-1.5	95	0.00
41 T	Methacrylonitrile	50.000	55.076	-10.2	96	0.00
42 TM	1,2-Dichloroethane	50.000	50.861	-1.7	96	0.00
43 T	Isopropyl Acetate	50.000	52.195	-4.4	96	0.00
44 TM	Trichloroethene	50.000	50.018	-0.0	93	0.00
45 C	1,2-Dichloropropane	50.000	51.983	-4.0#	96	0.00
46 T	Dibromomethane	50.000	49.978	0.0	94	0.00
47 T	Bromodichloromethane	50.000	51.889	-3.8	95	0.00
48 T	Methyl methacrylate	50.000	54.226	-8.5	97	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046048.D  
 Acq On : 05 May 2025 16:50  
 Operator : JC/MD  
 Sample : VSTDICV050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**ICVVX050525**

Quant Time: May 06 07:17:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	1059.599	-6.0	100	0.00
50 S	Toluene-d8	50.000	48.984	2.0	97	0.00
51 T	4-Methyl-2-Pentanone	250.000	259.133	-3.7	96	0.00
52 CM	Toluene	50.000	51.150	-2.3#	96	0.00
53 T	t-1,3-Dichloropropene	50.000	52.920	-5.8	94	0.00
54 T	cis-1,3-Dichloropropene	50.000	52.892	-5.8	95	0.00
55 T	1,1,2-Trichloroethane	50.000	50.887	-1.8	95	0.00
56 T	Ethyl methacrylate	50.000	53.918	-7.8	96	0.00
57 T	1,3-Dichloropropane	50.000	49.793	0.4	95	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	265.780	-6.3	93	0.00
59 T	2-Hexanone	250.000	268.218	-7.3	98	0.00
60 T	Dibromochloromethane	50.000	52.075	-4.2	95	0.00
61 T	1,2-Dibromoethane	50.000	51.050	-2.1	94	0.00
62 S	4-Bromofluorobenzene	50.000	48.596	2.8	96	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	99	0.00
64 T	Tetrachloroethene	50.000	46.795	6.4	88	0.00
65 PM	Chlorobenzene	50.000	48.699	2.6	96	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	49.557	0.9	94	0.00
67 C	Ethyl Benzene	50.000	50.245	-0.5#	95	0.00
68 T	m/p-Xylenes	100.000	101.022	-1.0	95	0.00
69 T	o-Xylene	50.000	50.841	-1.7	95	0.00
70 T	Styrene	50.000	51.907	-3.8	95	0.00
71 P	Bromoform	50.000	49.583	0.8	91	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	100	0.00
73 T	Isopropylbenzene	50.000	50.733	-1.5	96	0.00
74 T	N-amyl acetate	50.000	52.407	-4.8	98	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	47.827	4.3	98	0.00
76 T	1,2,3-Trichloropropane	50.000	48.568	2.9	99	0.00
77 T	Bromobenzene	50.000	48.549	2.9	95	0.00
78 T	n-propylbenzene	50.000	50.562	-1.1	95	0.00
79 T	2-Chlorotoluene	50.000	49.107	1.8	96	0.00
80 T	1,3,5-Trimethylbenzene	50.000	51.500	-3.0	96	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	49.276	1.4	95	0.00
82 T	4-Chlorotoluene	50.000	50.661	-1.3	96	0.00
83 T	tert-Butylbenzene	50.000	50.511	-1.0	97	0.00
84 T	1,2,4-Trimethylbenzene	50.000	51.485	-3.0	97	0.00
85 T	sec-Butylbenzene	50.000	51.122	-2.2	96	0.00
86 T	p-Isopropyltoluene	50.000	51.198	-2.4	96	0.00
87 T	1,3-Dichlorobenzene	50.000	50.272	-0.5	98	0.00
88 T	1,4-Dichlorobenzene	50.000	48.368	3.3	97	0.00
89 T	n-Butylbenzene	50.000	51.804	-3.6	96	0.00
90 T	Hexachloroethane	50.000	49.895	0.2	94	0.00
91 T	1,2-Dichlorobenzene	50.000	49.361	1.3	97	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	51.458	-2.9	97	0.00
93 T	1,2,4-Trichlorobenzene	50.000	49.662	0.7	97	0.00
94 T	Hexachlorobutadiene	50.000	48.408	3.2	95	0.00
95 T	Naphthalene	50.000	50.404	-0.8	98	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
Data File : VX046048.D  
Acq On : 05 May 2025 16:50  
Operator : JC/MD  
Sample : VSTDICV050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
ICVVX050525

Quant Time: May 06 07:17:12 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	Amount	Calc.	%Dev	Area	% Dev(min)
96 T 1,2,3-Trichlorobenzene	50.000	48.525	3.0	94	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>CHEMTECH</u>		Contract:	<u>JAC005</u>	
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q2200</u>	SAS No.:	<u>Q2200</u>
Instrument ID:	<u>MSVOA_X</u>		Calibration Date/Time:	<u>06/04/2025</u>	<u>10:12</u>
Lab File ID:	<u>VX046488.D</u>		Init. Calib. Date(s):	<u>05/05/2025</u>	<u>05/05/2025</u>
Heated Purge:	(Y/N)	N	Init. Calib. Time(s):	<u>11:35</u>	<u>16:27</u>
GC Column:	<u>DB-624UI</u>	ID: <u>0.18</u> (mm)			

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Vinyl Chloride	0.691	0.665		-3.76	20
1,1-Dichloroethene	0.593	0.593		0	20
1,1-Dichloroethane	1.219	1.302	0.1	6.81	20
cis-1,2-Dichloroethene	0.718	0.747		4.04	20
1,1,1-Trichloroethane	1.101	1.161		5.45	20
Benzene	1.417	1.496		5.57	20
1,2-Dichloroethane	0.612	0.651		6.37	20
Trichloroethene	0.341	0.364		6.74	20
1,1,2-Trichloroethane	0.343	0.370		7.87	20
Tetrachloroethene	0.354	0.378		6.78	20
1,2-Dichloroethane-d4	0.932	0.862		-7.51	20
Dibromofluoromethane	0.360	0.356		-1.11	20
Toluene-d8	1.246	1.135		-8.91	20
4-Bromofluorobenzene	0.478	0.469		-1.88	20

All other compounds must meet a minimum RRF of 0.010.  
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046488.D  
 Acq On : 04 Jun 2025 10:12  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.543	168	97475	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.750	114	165033	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	141151	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	69016	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.946	65	83988	46.217	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	92.440%		
35) Dibromofluoromethane	5.373	113	58786	49.466	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.940%		
50) Toluene-d8	8.646	98	187253	45.524	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	91.040%		
62) 4-Bromofluorobenzene	11.079	95	77443	49.083	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	98.160%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	73169	49.043	ug/l	96
3) Chloromethane	1.306	50	69991	48.377	ug/l	98
4) Vinyl Chloride	1.373	62	64836	48.151	ug/l	100
5) Bromomethane	1.599	94	27003	43.237	ug/l	91
6) Chloroethane	1.672	64	36727	51.093	ug/l	98
7) Trichlorofluoromethane	1.879	101	103198	51.858	ug/l	99
8) Diethyl Ether	2.135	74	34758	51.308	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.318	101	65312	53.034	ug/l	99
10) Methyl Iodide	2.446	142	70274	48.225	ug/l	99
11) Tert butyl alcohol	2.971	59	71909	281.901	ug/l	99
12) 1,1-Dichloroethene	2.312	96	57779	49.990	ug/l	97
13) Acrolein	2.233	56	72503	249.577	ug/l	99
14) Allyl chloride	2.660	41	120766	54.671	ug/l	97
15) Acrylonitrile	3.062	53	196655	269.611	ug/l	98
16) Acetone	2.379	43	215178	295.318	ug/l	99
17) Carbon Disulfide	2.501	76	126198	46.054	ug/l	100
18) Methyl Acetate	2.702	43	116961	69.175	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	223672	55.198	ug/l	99
20) Methylene Chloride	2.782	84	67521	48.357	ug/l	95
21) trans-1,2-Dichloroethene	3.086	96	58349	50.199	ug/l	100
22) Diisopropyl ether	3.757	45	234578	54.976	ug/l	96
23) Vinyl Acetate	3.714	43	983901	262.170	ug/l	100
24) 1,1-Dichloroethane	3.605	63	126924	53.406	ug/l	100
25) 2-Butanone	4.550	43	295497	279.346	ug/l	99
26) 2,2-Dichloropropane	4.464	77	103262	55.512	ug/l	99
27) cis-1,2-Dichloroethene	4.476	96	72840	52.056	ug/l	98
28) Bromochloromethane	4.885	49	53251	46.549	ug/l	97
29) Tetrahydrofuran	5.001	42	181777	274.234	ug/l	98
30) Chloroform	5.086	83	130154	52.542	ug/l	96
31) Cyclohexane	5.458	56	107767	49.761	ug/l	99
32) 1,1,1-Trichloroethane	5.373	97	113144	52.691	ug/l	99
36) 1,1-Dichloropropene	5.677	75	83522	52.307	ug/l	99
37) Ethyl Acetate	4.708	43	105142	53.296	ug/l	99
38) Carbon Tetrachloride	5.671	117	96961	54.045	ug/l	99
39) Methylcyclohexane	7.372	83	107311	52.202	ug/l	97
40) Benzene	6.031	78	246896	52.789	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046488.D  
 Acq On : 04 Jun 2025 10:12  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.909	41	61057m	59.164	ug/1	
42) 1,2-Dichloroethane	6.080	62	107364	53.188	ug/1	99
43) Isopropyl Acetate	6.336	43	172534	57.328	ug/1	100
44) Trichloroethene	7.116	130	60052	53.347	ug/1	93
45) 1,2-Dichloropropane	7.421	63	63728	54.797	ug/1	100
46) Dibromomethane	7.573	93	48150	52.494	ug/1	99
47) Bromodichloromethane	7.817	83	99979	55.341	ug/1	99
48) Methyl methacrylate	7.689	41	88716	57.719	ug/1	99
49) 1,4-Dioxane	7.653	88	31277	1071.717	ug/1	98
51) 4-Methyl-2-Pentanone	8.567	43	559427	280.031	ug/1	100
52) Toluene	8.713	92	148931	51.931	ug/1	99
53) t-1,3-Dichloropropene	8.976	75	91872	57.213	ug/1	98
54) cis-1,3-Dichloropropene	8.360	75	101352	57.106	ug/1	95
55) 1,1,2-Trichloroethane	9.146	97	61136	54.064	ug/1	98
56) Ethyl methacrylate	9.110	69	105633	58.611	ug/1	98
57) 1,3-Dichloropropane	9.305	76	107331	52.850	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.238	63	252660	274.981	ug/1	100
59) 2-Hexanone	9.427	43	423096	286.265	ug/1	100
60) Dibromochloromethane	9.518	129	69918	56.300	ug/1	100
61) 1,2-Dibromoethane	9.604	107	62700	53.347	ug/1	97
64) Tetrachloroethene	9.268	164	53293	53.362	ug/1	93
65) Chlorobenzene	10.073	112	164933	53.386	ug/1	99
66) 1,1,1,2-Tetrachloroethane	10.158	131	57986	54.966	ug/1	99
67) Ethyl Benzene	10.189	91	298815	54.870	ug/1	100
68) m/p-Xylenes	10.299	106	215687	108.288	ug/1	97
69) o-Xylene	10.640	106	106763	54.982	ug/1	97
70) Styrene	10.652	104	181074	56.926	ug/1	100
71) Bromoform	10.798	173	44870	56.651	ug/1 #	98
73) Isopropylbenzene	10.957	105	288460	53.686	ug/1	100
74) N-amyl acetate	10.841	43	147771	55.656	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	95562	50.752	ug/1	99
76) 1,2,3-Trichloropropane	11.237	75	86142m	51.854	ug/1	
77) Bromobenzene	11.195	156	65831	52.773	ug/1	98
78) n-propylbenzene	11.298	91	338759	54.223	ug/1	100
79) 2-Chlorotoluene	11.359	91	207728	51.549	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	241792	53.865	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	28928	56.693	ug/1	96
82) 4-Chlorotoluene	11.451	91	240706	53.864	ug/1	99
83) tert-Butylbenzene	11.713	119	240573	53.206	ug/1	100
84) 1,2,4-Trimethylbenzene	11.749	105	244850	53.863	ug/1	99
85) sec-Butylbenzene	11.890	105	304738	54.891	ug/1	99
86) p-Isopropyltoluene	12.006	119	251225	54.822	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	119595	52.532	ug/1	99
88) 1,4-Dichlorobenzene	12.036	146	120210	51.703	ug/1	99
89) n-Butylbenzene	12.329	91	228216	56.775	ug/1	100
90) Hexachloroethane	12.536	117	44135	54.668	ug/1	98
91) 1,2-Dichlorobenzene	12.329	146	120071	52.558	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.938	75	22836	54.746	ug/1	98
93) 1,2,4-Trichlorobenzene	13.585	180	71028	54.131	ug/1	99
94) Hexachlorobutadiene	13.719	225	31559	55.070	ug/1	99
95) Naphthalene	13.774	128	258228	53.657	ug/1	100
96) 1,2,3-Trichlorobenzene	13.956	180	73266	54.114	ug/1	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046488.D  
 Acq On : 04 Jun 2025 10:12  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
**MSVOA\_X**  
**ClientSampleId :**  
**VSTDCCC050**

Quant Time: Jun 05 01:34:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
Data File : VX046488.D  
Acq On : 04 Jun 2025 10:12  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1







Quant Time: Jun 05 01:34:12 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VSTDCCC050

## Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

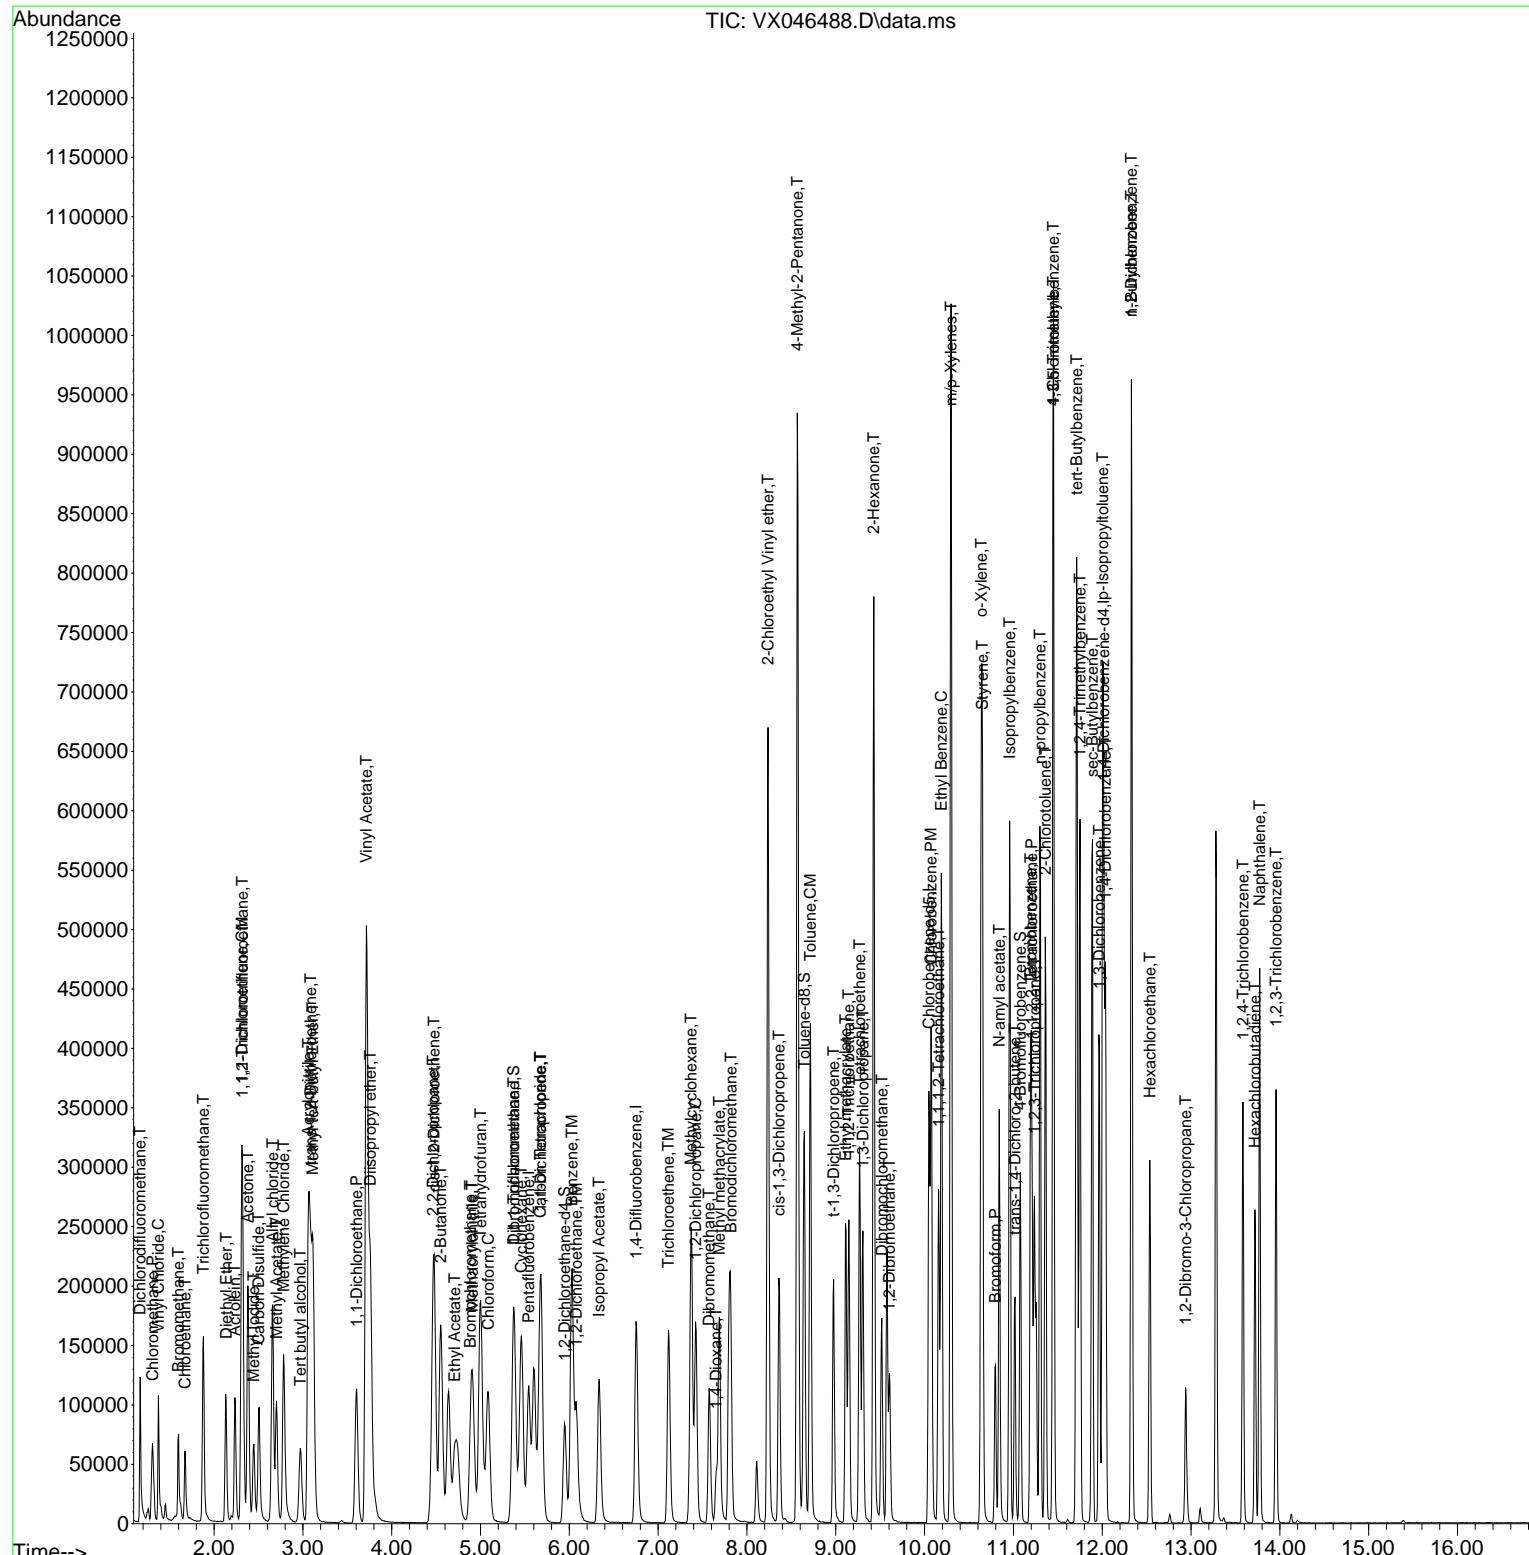




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.543 min Scan# 7  
Instrument: MSVOA\_X  
Delta R.T. -0.001 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12  
ClientSampleId : VSTDCCC050

Tgt Ion:168 Resp: 97479  
Ion Ratio Lower Upper  
168 100  
99 71.2 54.9 82.3


Manual Integrations  
APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025




#2  
Dichlorodifluoromethane  
Concen: 49.043 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 85 Resp: 73169  
Ion Ratio Lower Upper  
85 100  
87 33.4 15.7 47.1

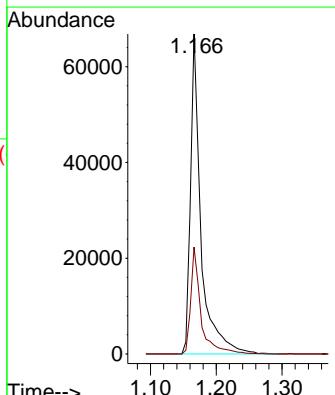



Abundance Scan 36 (1.306 min): VX046488.D\data.ms

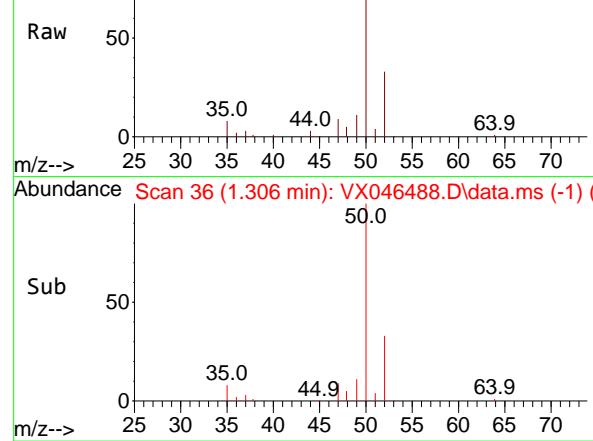

#3

Chloromethane

Concen: 48.377 ug/l

RT: 1.306 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050



**Manual Integrations  
APPROVED**







Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

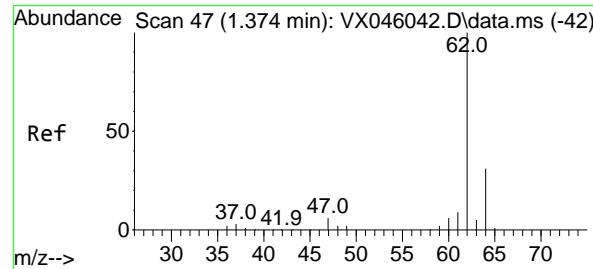

Abundance Scan 47 (1.373 min): VX046488.D\data.ms
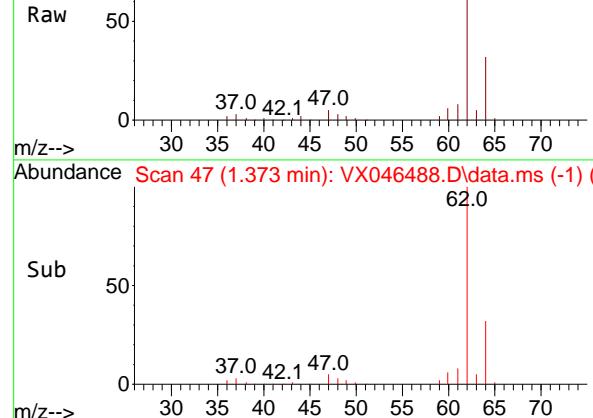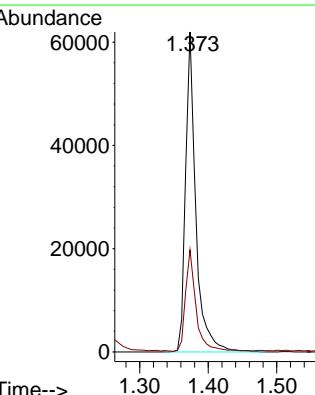
#4  
Vinyl Chloride  
Concen: 48.151 ug/l  
RT: 1.373 min Scan# 47  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12Tgt Ion: 62 Resp: 64836  
Ion Ratio Lower Upper  
62 100  
64 31.5 25.2 37.8

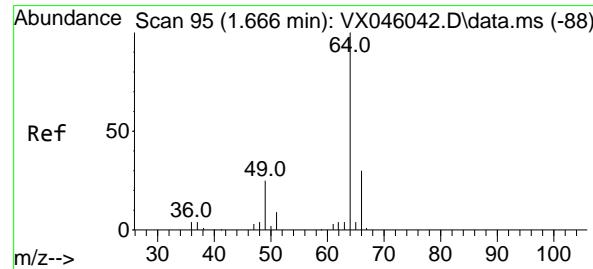

#5

Bromomethane

Concen: 43.237 ug/l

RT: 1.599 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#6

Chloroethane

Concen: 51.093 ug/l


RT: 1.672 min Scan# 96




Delta R.T. 0.006 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt Ion: 64 Resp: 36727  
 Ion Ratio Lower Upper  
 64 100  
 66 31.5 24.3 36.5



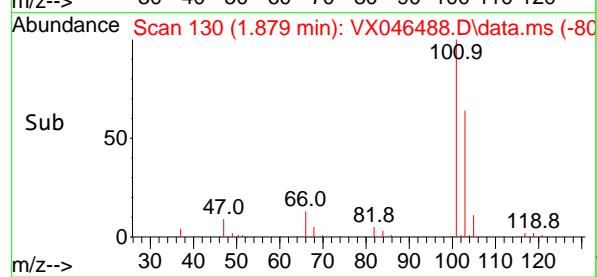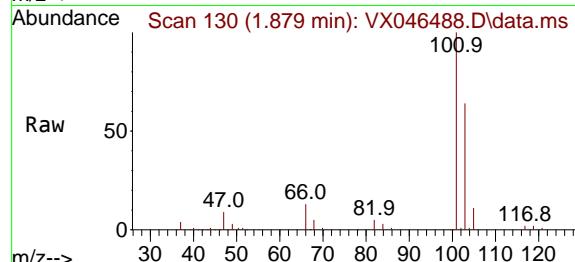




#7

Trichlorofluoromethane  
Concen: 51.858 ug/l  
RT: 1.879 min Scan# 129  
Delta R.T. 0.006 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument: MSVOA\_X  
Client SampleId: VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025




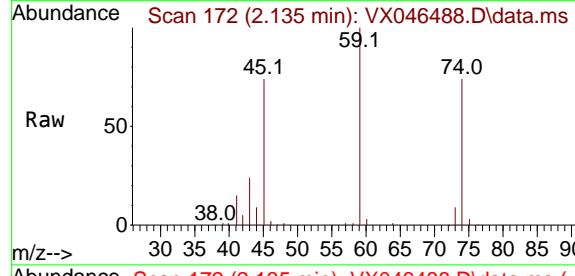
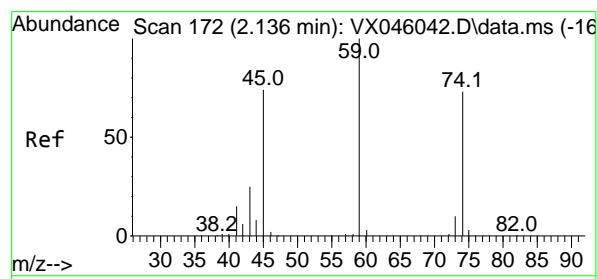
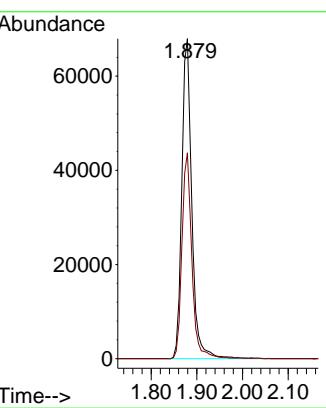


#8

Diethyl Ether  
Concen: 51.308 ug/l  
RT: 2.135 min Scan# 172  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 74 Resp: 34758  
Ion Ratio Lower Upper  
74 100  
45 107.9 54.9 164.8

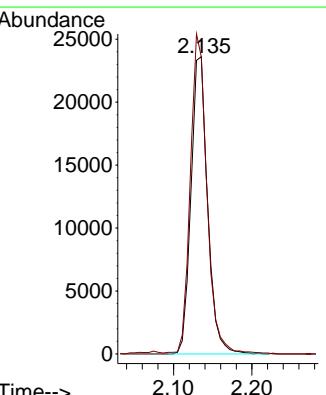

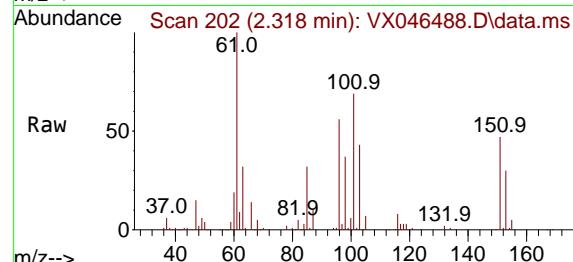

#9

1,1,2-Trichlorotrifluoroethane

Concen: 53.034 ug/l

RT: 2.318 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

Abundance

30000

20000

10000

0

Time--&gt; 2.20 2.30 2.40

#10

Methyl Iodide

Concen: 48.225 ug/l

RT: 2.446 min Scan# 223

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt Ion:142 Resp: 70274

Ion Ratio Lower Upper

142 100

127 51.6 41.7 62.5

141 14.5 11.5 17.3

Abundance




30000

20000

10000

0

Time--&gt; 2.40 2.50 2.60

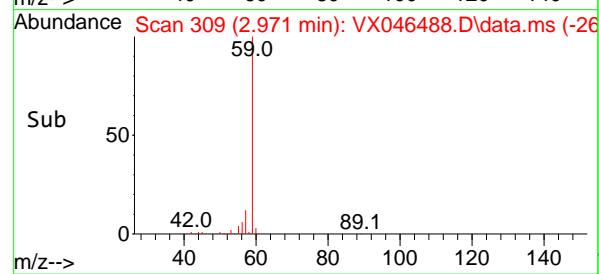





#11

Tert butyl alcohol  
Concen: 281.901 ug/l  
RT: 2.971 min Scan# 3  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

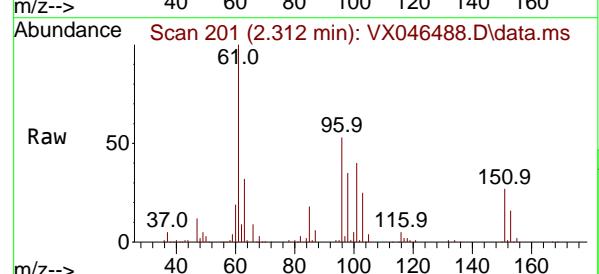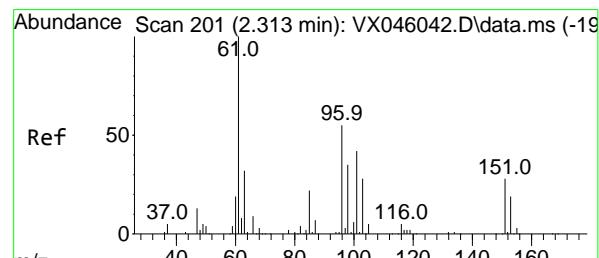


#12

1,1-Dichloroethene  
Concen: 49.990 ug/l  
RT: 2.312 min Scan# 201  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12



Tgt Ion: 96 Resp: 57779  
Ion Ratio Lower Upper  
96 100  
61 187.2 146.2 219.2  
98 65.4 51.0 76.6





#13  
Acrolein  
Concen: 249.577 ug/l  
RT: 2.233 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12



Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

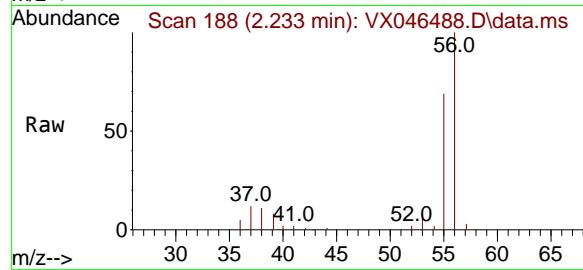


Tgt Ion: 56 Resp: 7250  
Ion Ratio Lower Upper  
56 100  
55 71.0 56.2 84.4

### Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025






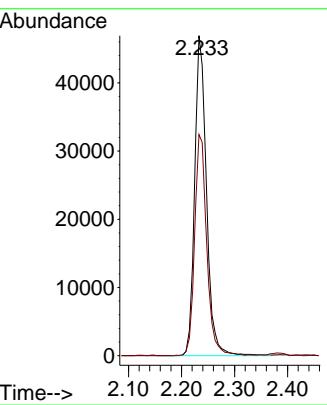


#14  
Allyl chloride  
Concen: 54.671 ug/l  
RT: 2.660 min Scan# 258  
Delta R.T. 0.006 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12



Tgt Ion: 41 Resp: 120766  
Ion Ratio Lower Upper  
41 100  
39 73.0 60.6 90.8  
76 29.8 24.9 37.3

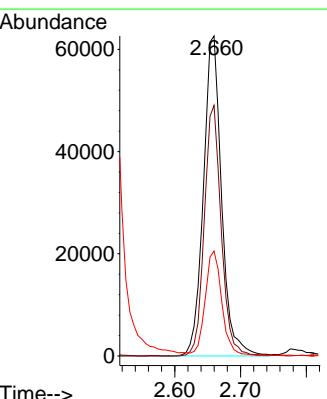



#15

Acrylonitrile

Concen: 269.611 ug/l

RT: 3.062 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X

ClientSampleId :


VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

Abundance

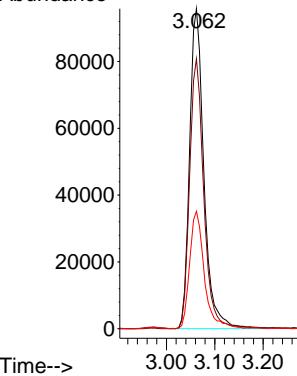

#16

Acetone

Concen: 295.318 ug/l

RT: 2.379 min Scan# 212

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12


Tgt Ion: 43 Resp: 215178







Ion Ratio Lower Upper

43 100

58 27.0 21.2 31.8

Abundance

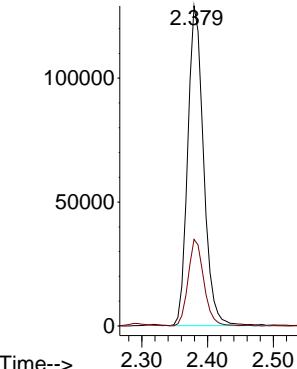



#17

Carbon Disulfide

Concen: 46.054 ug/l

RT: 2.501 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

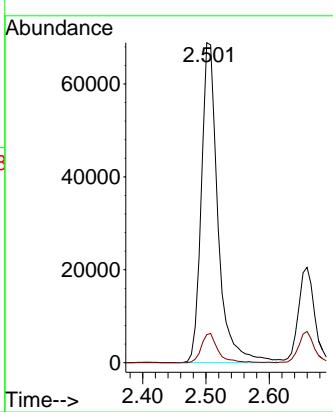

#18

Methyl Acetate

Concen: 69.175 ug/l


RT: 2.702 min Scan# 265







Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt Ion: 43 Resp: 116961  
 Ion Ratio Lower Upper  
 43 100  
 74 21.5 16.7 25.1






#19

Methyl tert-butyl Ether  
Concen: 55.198 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument: MSVOA\_X  
ClientSampleId: VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025









#20

Methylene Chloride  
Concen: 48.357 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 84 Resp: 67521  
Ion Ratio Lower Upper  
84 100  
49 134.2 113.9 170.9  
51 42.4 33.5 50.3  
86 64.9 53.8 80.8

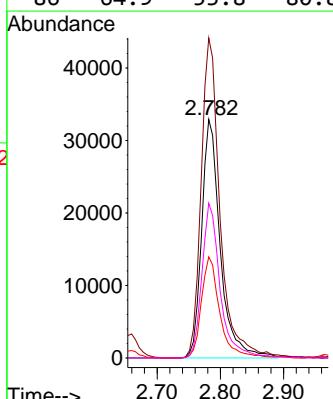




#21

trans-1,2-Dichloroethene  
Concen: 50.199 ug/l  
RT: 3.086 min Scan# 3  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

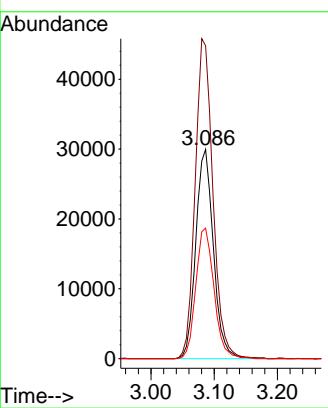


#22

Diisopropyl ether  
Concen: 54.976 ug/l  
RT: 3.757 min Scan# 438  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 45 Resp: 234578  
Ion Ratio Lower Upper  
45 100  
43 78.9 66.6 100.0  
87 24.6 19.8 29.6  
59 10.8 8.6 12.8

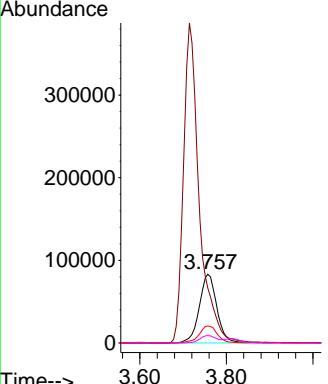



#23

**Vinyl Acetate**

Concen: 262.170 ug/l

RT: 3.714 min Scan# 413

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12



Tgt Ion: 43 Resp: 98390

Ion Ratio Lower Upper

43 100

86 9.4 7.5 11.3

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**



Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

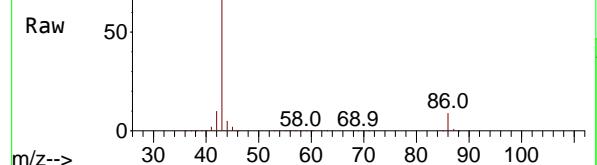


Abundance

3.714

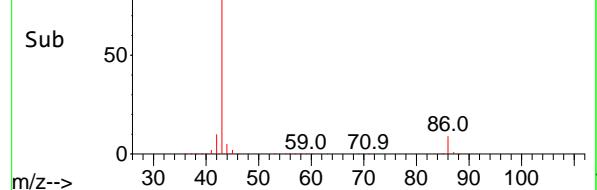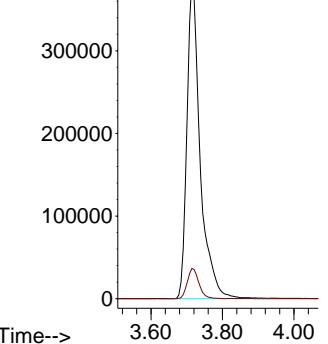

#24  
1,1-Dichloroethane  
Concen: 53.406 ug/l  
RT: 3.605 min Scan# 413  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12





Tgt Ion: 63 Resp: 126924


Ion Ratio Lower Upper

63 100

98 7.0 3.6 10.8


100 4.3 2.1 6.3

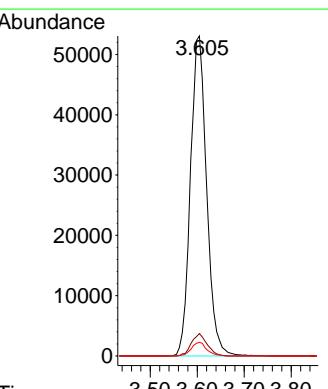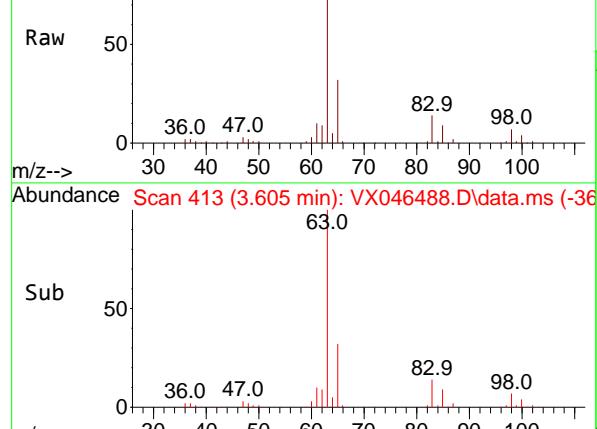



#25  
2-Butanone  
Concen: 279.346 ug/l  
RT: 4.550 min Scan# 5  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12




Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050




Tgt Ion: 43 Resp: 295491  
Ion Ratio Lower Upper  
43 100  
72 23.6 18.4 27.6

Manual Integrations  
**APPROVED**



Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

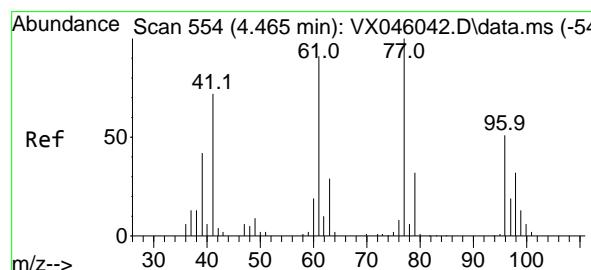
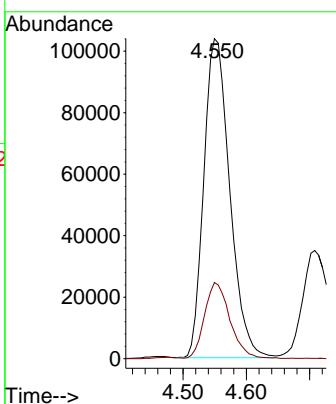
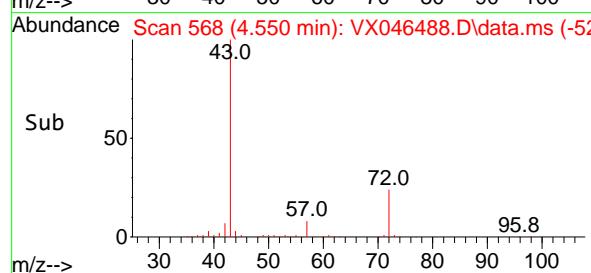


#26  
2,2-Dichloropropane  
Concen: 55.512 ug/l  
RT: 4.464 min Scan# 554  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

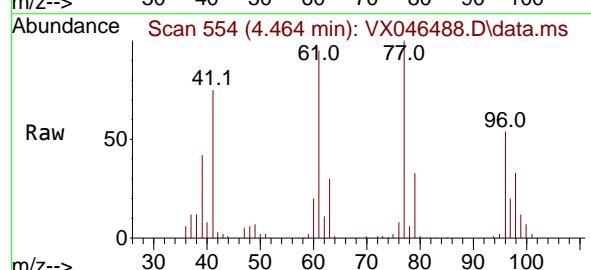

Tgt Ion: 77 Resp: 103262  
Ion Ratio Lower Upper  
77 100  
97 20.5 10.5 31.5

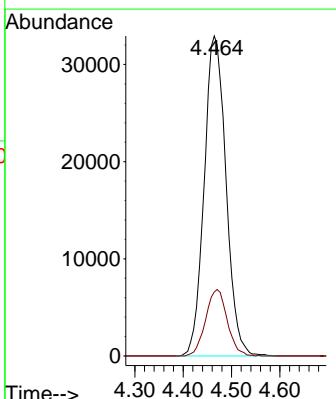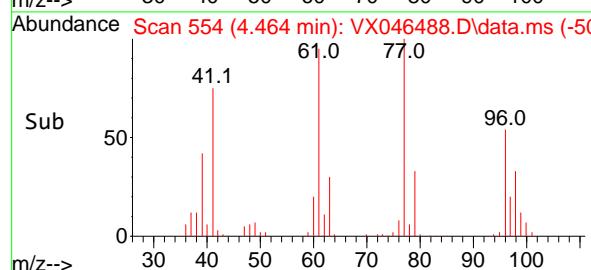


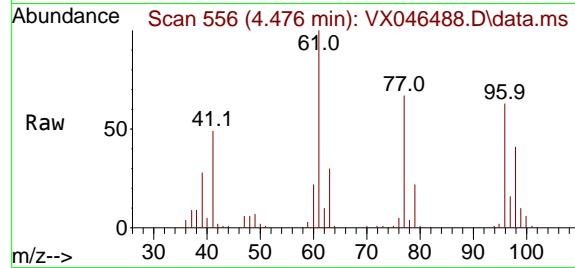



#27  
cis-1,2-Dichloroethene  
Concen: 52.056 ug/l  
RT: 4.476 min Scan# 51  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050



### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

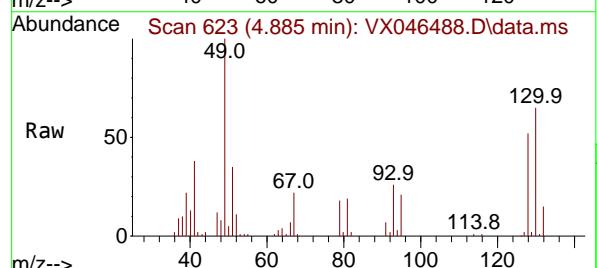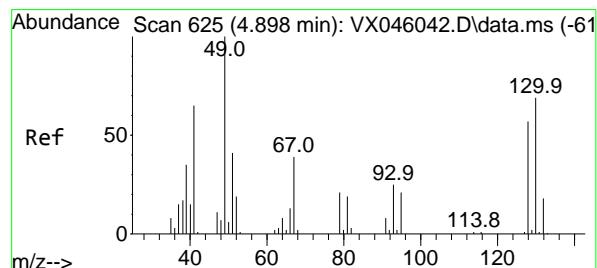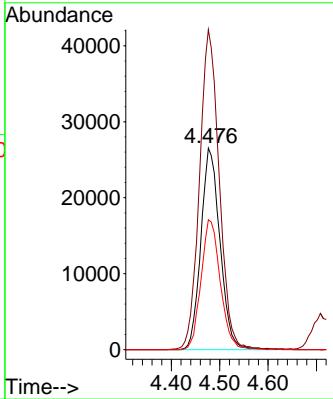

#28  
Bromochloromethane  
Concen: 46.549 ug/l  
RT: 4.885 min Scan# 623  
Delta R.T. -0.013 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 49 Resp: 53251  
Ion Ratio Lower Upper  
49 100  
129 1.6 0.0 4.0  
130 67.3 56.2 84.2



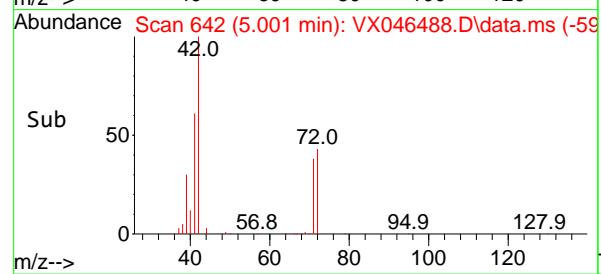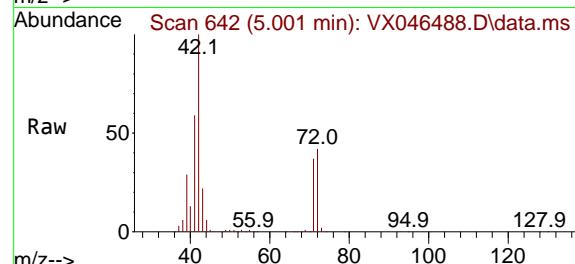

#29

Tetrahydrofuran

Concen: 274.234 ug/l

RT: 5.001 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X




ClientSampleId :

VSTDCCC050

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#30

Chloroform

Concen: 52.542 ug/l

RT: 5.086 min Scan# 656

Delta R.T. -0.000 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12


Tgt Ion: 83 Resp: 130154

Ion Ratio Lower Upper

83 100

85 64.4 49.3 73.9

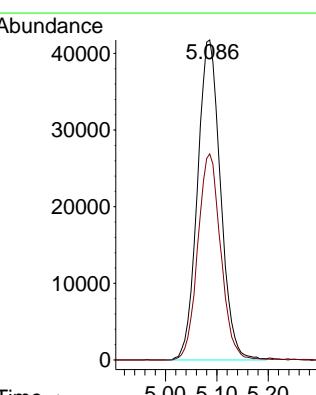



#31

Cyclohexane

Concen: 49.761 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.007 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050



Tgt Ion: 56 Resp: 10776

Ion Ratio Lower Upper

56 100




69 31.3 24.4 36.6

84 84.7 66.9 100.3


**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025



Supervised By :Semsettin Yesilyurt 06/05/2025





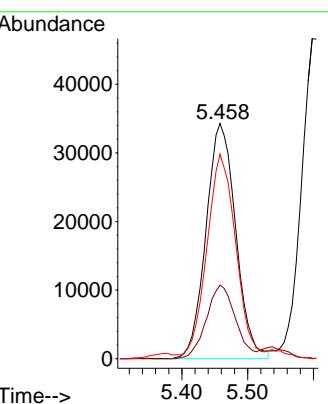
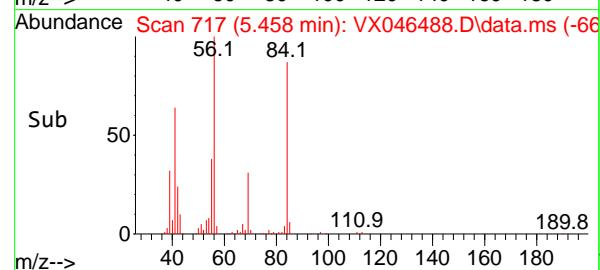


#32  
1,1,1-Trichloroethane  
Concen: 52.691 ug/l  
RT: 5.373 min Scan# 703  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12



Tgt Ion: 97 Resp: 113144  
Ion Ratio Lower Upper  
97 100  
99 63.9 51.8 77.6  
61 49.1 40.1 60.1

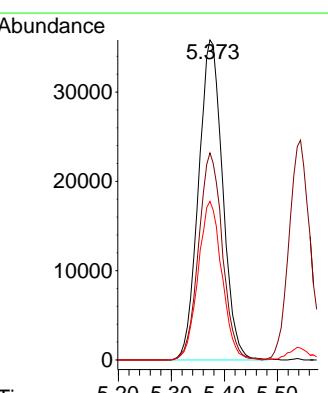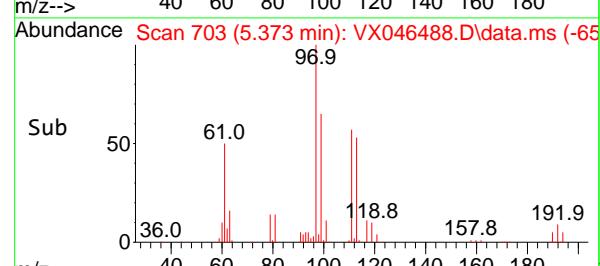

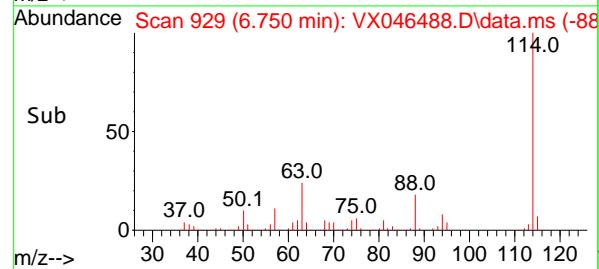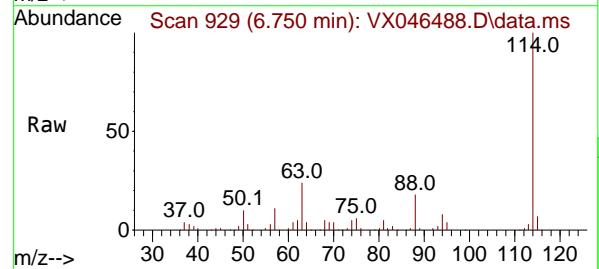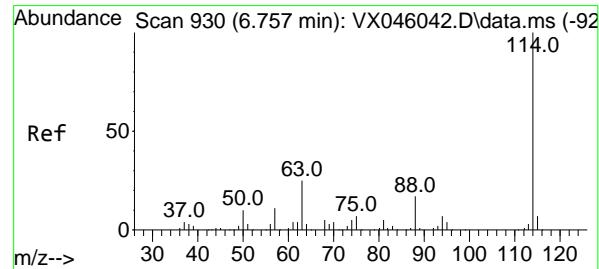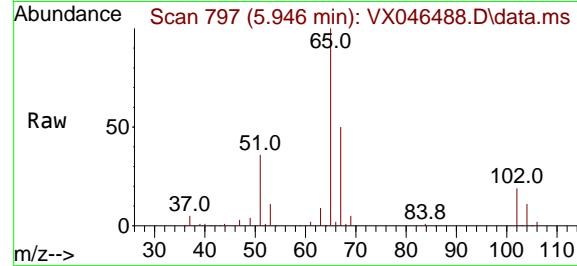

#33

1,2-Dichloroethane-d4

Concen: 46.217 ug/l

RT: 5.946 min Scan# 7

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025







Supervised By :Semsettin Yesilyurt 06/05/2025



#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.750 min Scan# 929  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion:114 Resp: 165033  
Ion Ratio Lower Upper  
114 100  
63 24.4 0.0 49.2  
88 18.1 0.0 33.6



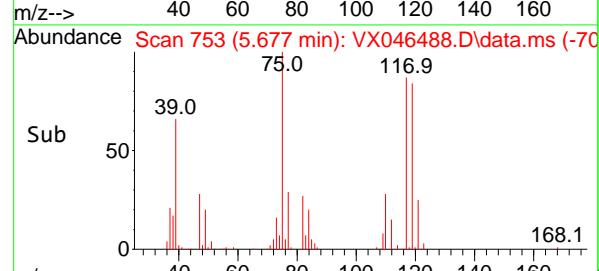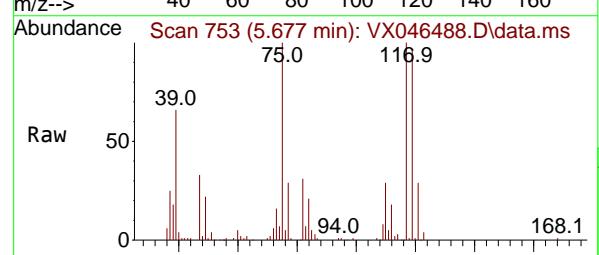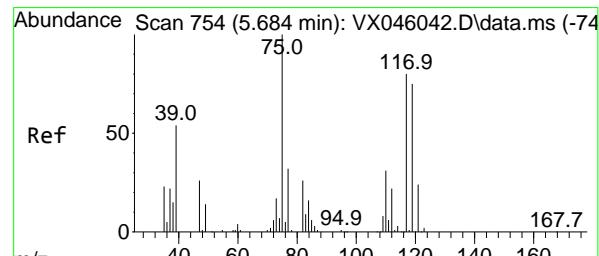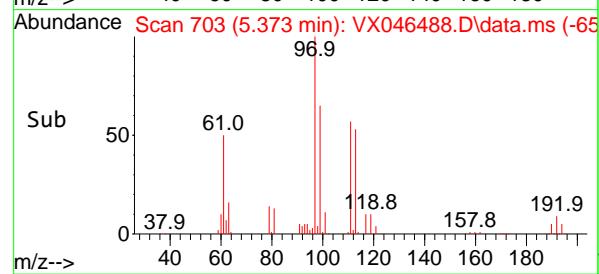


#35

Dibromofluoromethane  
Concen: 49.466 ug/l  
RT: 5.373 min Scan# 7  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument :  
MSVOA\_X  
ClientSampleId :  
VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

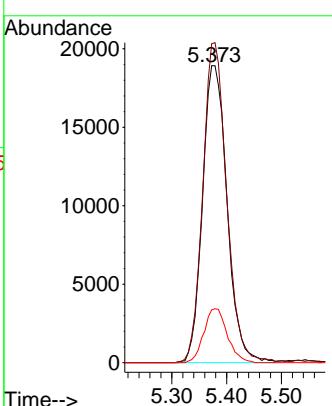


#36


1,1-Dichloropropene  
Concen: 52.307 ug/l  
RT: 5.677 min Scan# 753  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 75 Resp: 83522  
Ion Ratio Lower Upper  
75 100  
110 32.3 16.3 48.9  
77 31.1 24.3 36.5

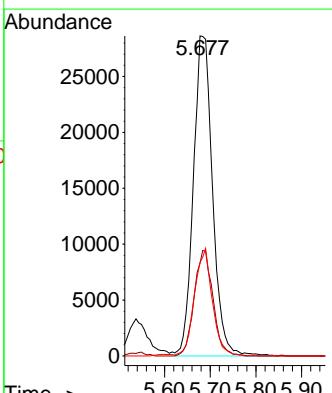




Abundance Scan 594 (4.708 min): VX046488.D\data.ms

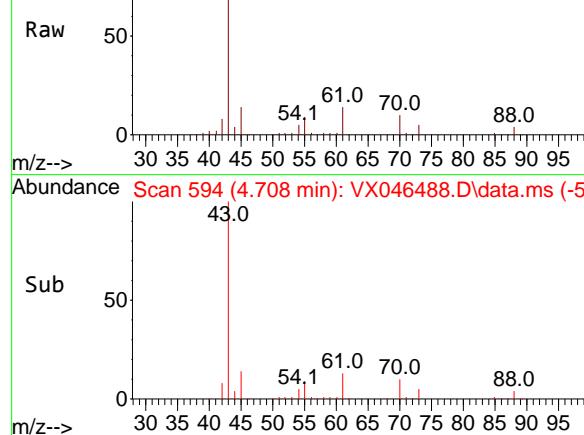

Abundance Scan 594 (4.708 min): VX046488.D\data.ms (-54)

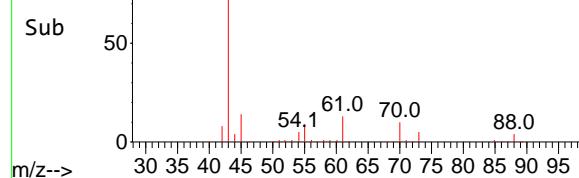

#37

## Ethyl Acetate

Concen: 53.296 ug/l

RT: 4.708 min Scan# 5

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

Tgt Ion: 43 Resp: 10514:

Ion Ratio Lower Upper

43 100

61 12.7 10.3 15.5



70 9.7 7.9 11.9

## Manual Integrations


APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025


Supervised By :Semsettin Yesilyurt 06/05/2025

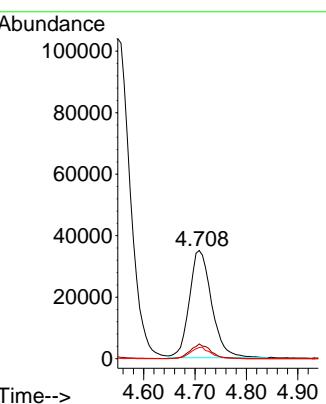

Abundance Scan 752 (5.671 min): VX046488.D\data.ms

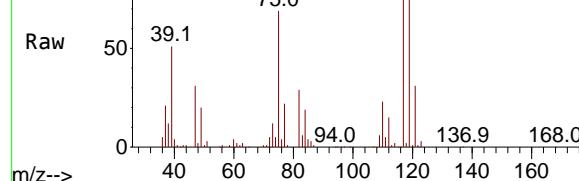

Abundance Scan 752 (5.671 min): VX046488.D\data.ms (-70)

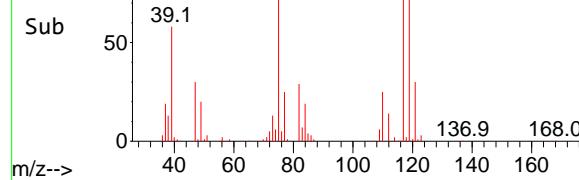

#38

## Carbon Tetrachloride

Concen: 54.045 ug/l

RT: 5.671 min Scan# 752

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12


Tgt Ion: 117 Resp: 96961







Ion Ratio Lower Upper

117 100

119 93.0 75.2 112.8

121 30.9 24.2 36.4

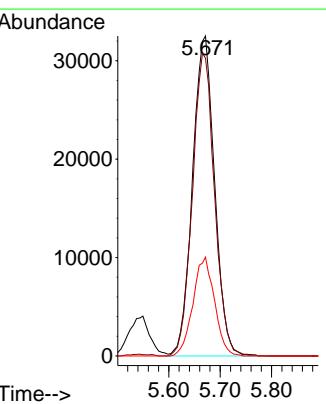

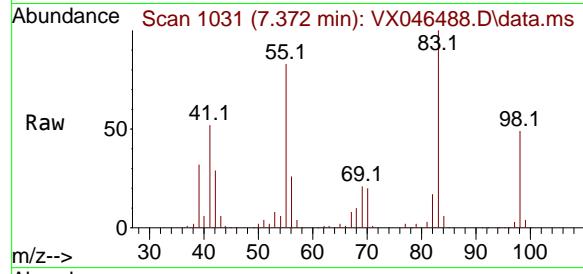

#39

Methylcyclohexane

Concen: 52.202 ug/l

RT: 7.372 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#40

Benzene

Concen: 52.789 ug/l

RT: 6.031 min Scan# 811

Delta R.T. -0.000 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12







Tgt Ion: 78 Resp: 246896

Ion Ratio Lower Upper

78 100

77 23.9 19.0 28.4



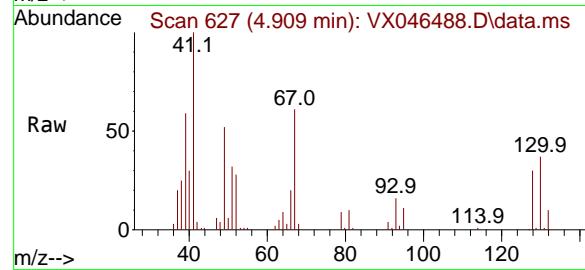

#41

Methacrylonitrile  
Concen: 59.164 ug/l m  
RT: 4.909 min Scan# 61051  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

Tgt Ion: 41 Resp: 61051

Ion Ratio Lower Upper

41 100

39 58.5 47.2 70.8

67 64.4 50.7 76.1

52 30.6 24.6 37.0

Abundance

Time-->

30000  
20000  
10000  
0

4.85 4.90 4.95

4.909

#42


1,2-Dichloroethane  
Concen: 53.188 ug/l  
RT: 6.080 min Scan# 819  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12


Tgt Ion: 62 Resp: 107364

Ion Ratio Lower Upper

62 100

98 7.3 0.0 15.2





#43

Isopropyl Acetate

Concen: 57.328 ug/l

RT: 6.336 min Scan# 8

Delta R.T. -0.000 min

Lab File: VX046488.D



Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X

ClientSampleId :

VSTDCCC050

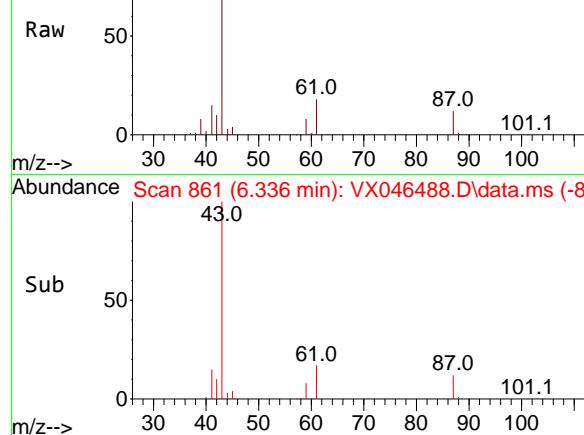

Tgt Ion: 43 Resp: 172534

Ion Ratio Lower Upper

43 100

61 17.8 14.3 21.5

87 11.7 9.5 14.3

Manual Integrations



APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



6.336

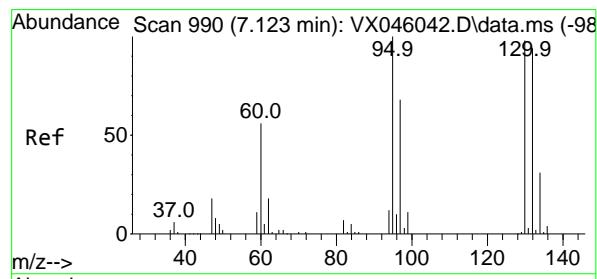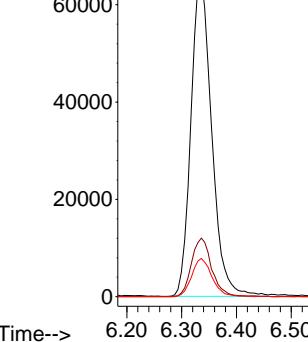

#44

Trichloroethene


Concen: 53.347 ug/l

RT: 7.116 min Scan# 989

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

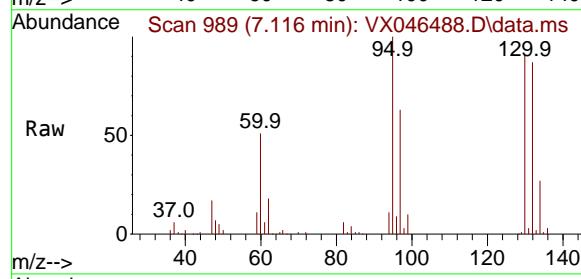

Tgt Ion:130 Resp: 60052



Ion Ratio Lower Upper




130 100

95 109.6 0.0 204.2



7.116

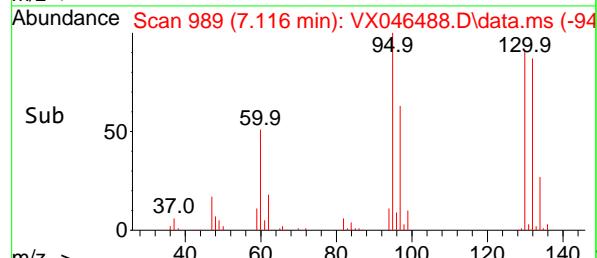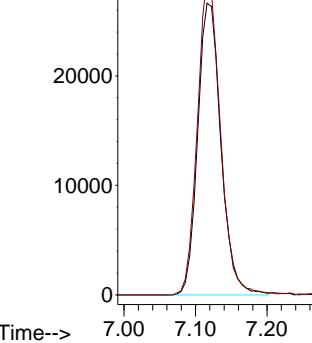



#45

1,2-Dichloropropane

Concen: 54.797 ug/l

RT: 7.421 min Scan# 1

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

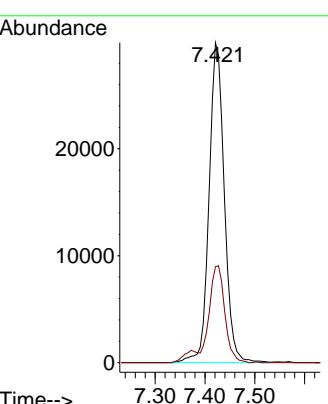

#46

Dibromomethane

Concen: 52.494 ug/l

RT: 7.573 min Scan# 1064


Delta R.T. -0.000 min


Lab File: VX046488.D

Acq: 04 Jun 2025 10:12



Tgt Ion: 93 Resp: 48150

Ion	Ratio	Lower	Upper
93	100		
95	82.4	65.6	98.4
174	86.7	68.2	102.2


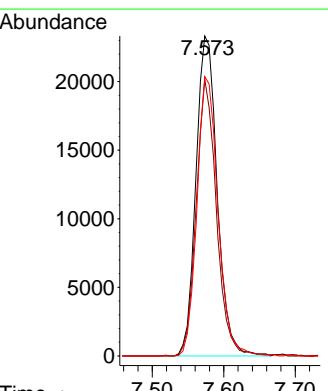




Abundance Scan 1104 (7.817 min): VX046488.D\data.ms

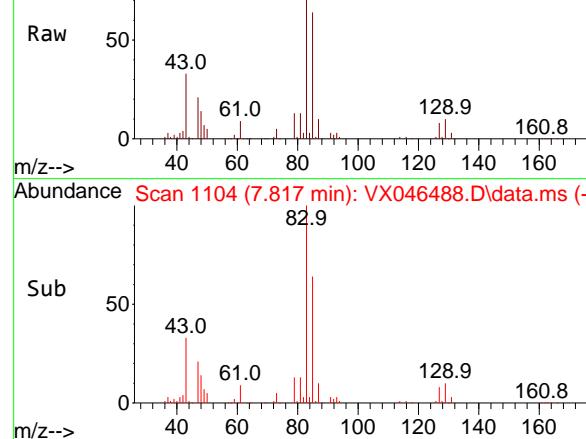

Abundance Scan 1083 (7.689 min): VX046488.D\data.ms

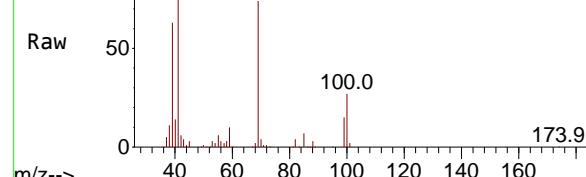

#47

Bromodichloromethane

Concen: 55.341 ug/l

RT: 7.817 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X

ClientSampleId :


VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

Abundance

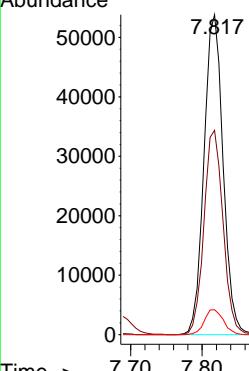

#48

Methyl methacrylate

Concen: 57.719 ug/l

RT: 7.689 min Scan# 1083

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12


Tgt Ion: 41 Resp: 88716


Ion Ratio Lower Upper

41 100





69 72.6 58.5 87.7

39 62.9 51.7 77.5

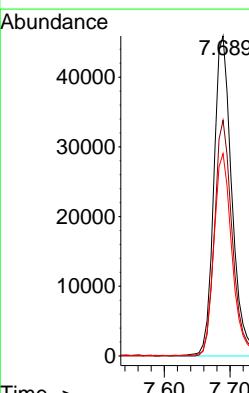



Abundance Scan 1077 (7.653 min): VX046488.D\data.ms

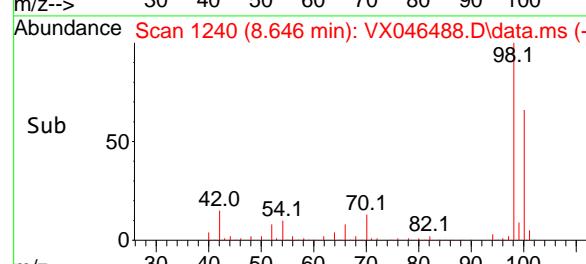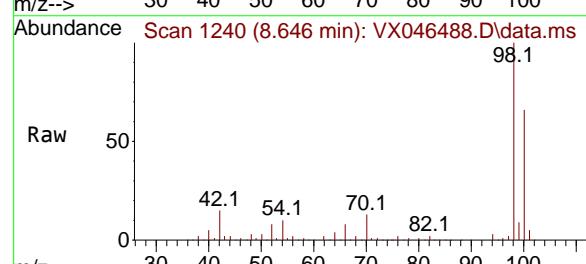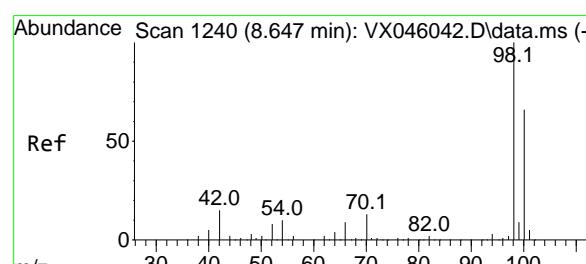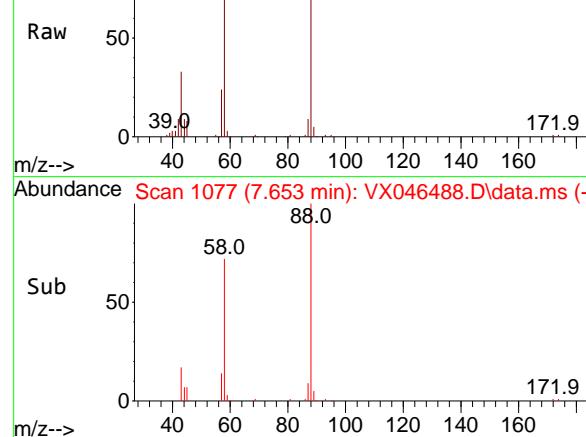

#49

1,4-Dioxane

Concen: 1071.717 ug/l

RT: 7.653 min Scan# 1

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

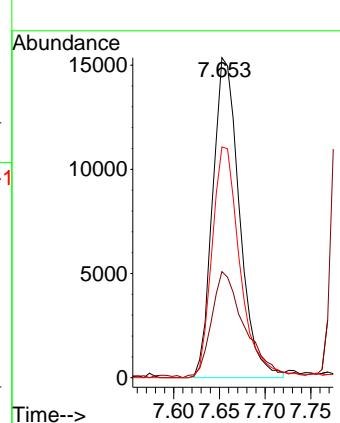

Tgt Ion: 88

Ion Ratio Lower Upper

88 100

43 41.5 33.4 50.2

58 75.7 58.6 88.0

#50

Toluene-d8

Concen: 45.524 ug/l

RT: 8.646 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12


Tgt Ion: 98

Ion Ratio Lower Upper

98 100



100 66.0 53.5 80.3

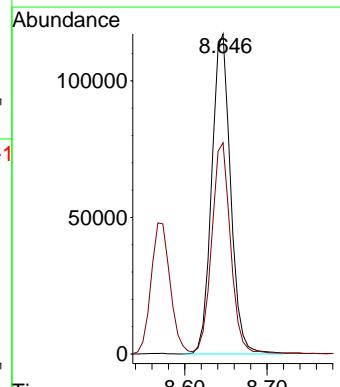



#51  
4-Methyl-2-Pentanone  
Concen: 280.031 ug/l  
RT: 8.567 min Scan# 1  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12



Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050

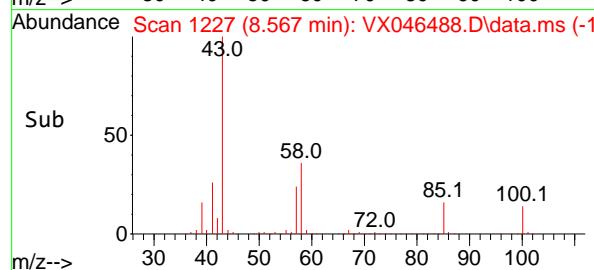


Tgt Ion: 43 Resp: 55942  
Ion Ratio Lower Upper  
43 100  
58 35.9 28.9 43.3

Manual Integrations  
APPROVED



Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025


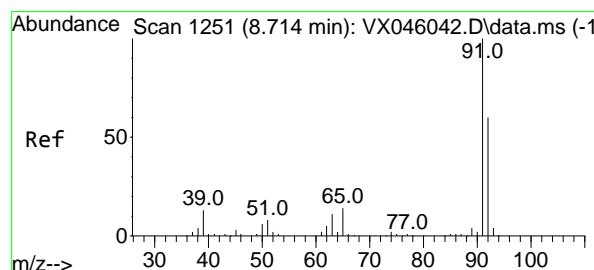
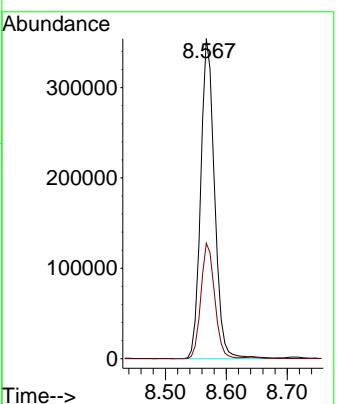


#52  
Toluene  
Concen: 51.931 ug/l  
RT: 8.713 min Scan# 1251  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

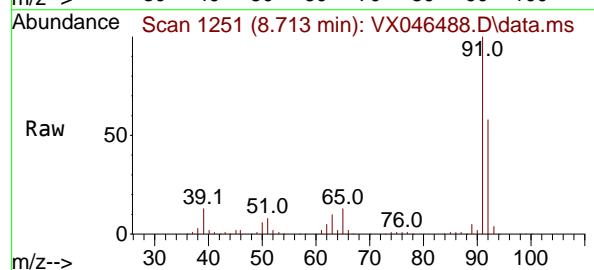

Tgt Ion: 92 Resp: 148931  
Ion Ratio Lower Upper  
92 100  
91 172.6 136.6 205.0

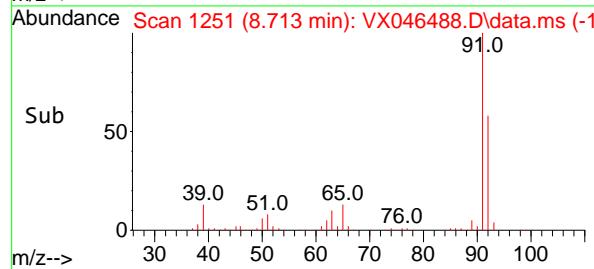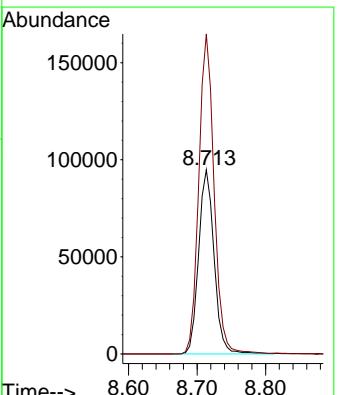







#53

t-1,3-Dichloropropene  
Concen: 57.213 ug/l  
RT: 8.976 min Scan# 1193  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument: MSVOA\_X  
Client SampleId: VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025






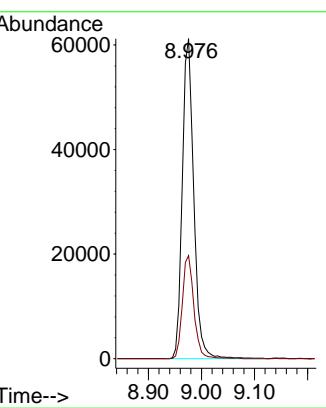


#54

cis-1,3-Dichloropropene  
Concen: 57.106 ug/l  
RT: 8.360 min Scan# 1193  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 75 Resp: 101352  
Ion Ratio Lower Upper  
75 100  
77 30.2 25.4 38.0  
39 60.0 52.2 78.4

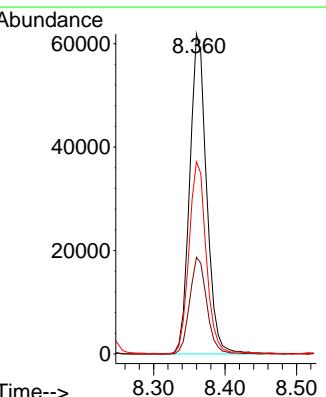



#55

1,1,2-Trichloroethane

Concen: 54.064 ug/l

RT: 9.146 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025



Supervised By :Semsettin Yesilyurt 06/05/2025

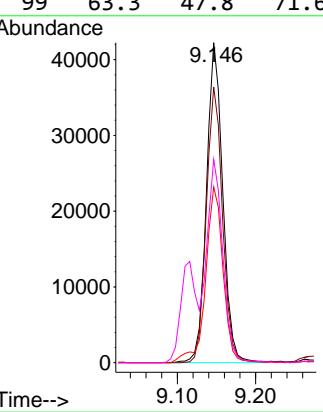

#56  
Ethyl methacrylate  
Concen: 58.611 ug/l  
RT: 9.110 min Scan# 1316  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 69 Resp: 105633  
Ion Ratio Lower Upper  
69 100  
41 77.1 60.8 91.2  
39 46.3 39.0 58.6

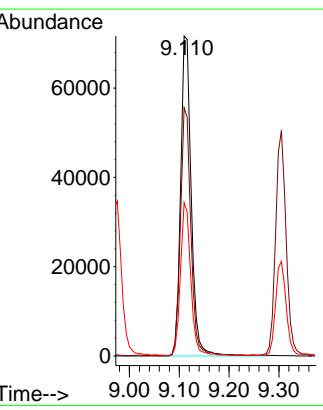

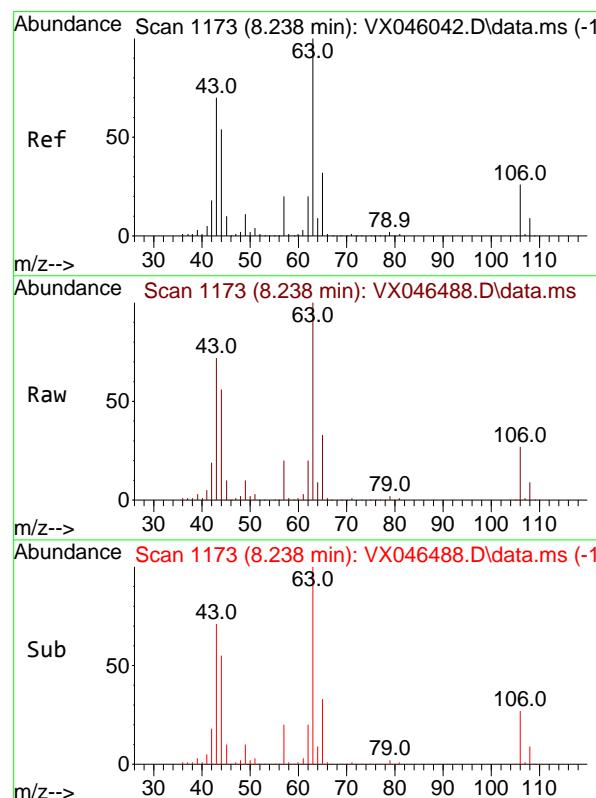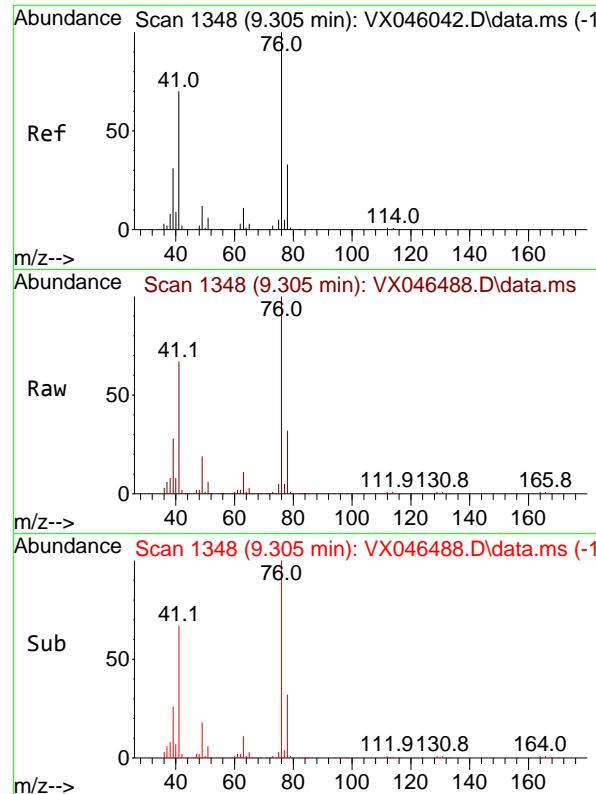


#57

1,3-Dichloropropane  
Concen: 52.850 ug/l  
RT: 9.305 min Scan# 1173  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument: MSVOA\_X  
ClientSampleId: VSTDCCC050

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025




#58



2-Chloroethyl Vinyl ether  
Concen: 274.981 ug/l  
RT: 8.238 min Scan# 1173  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 63 Resp: 252660  
Ion Ratio Lower Upper  
63 100  
106 27.0 21.5 32.3






Abundance Scan 1368 (9.427 min): VX046488.D\data.ms

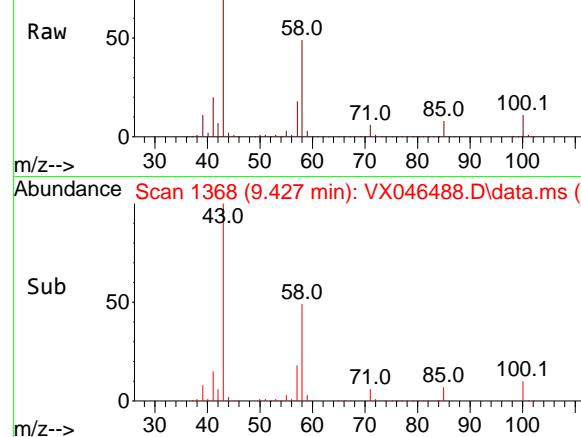

Abundance Scan 1383 (9.518 min): VX046488.D\data.ms

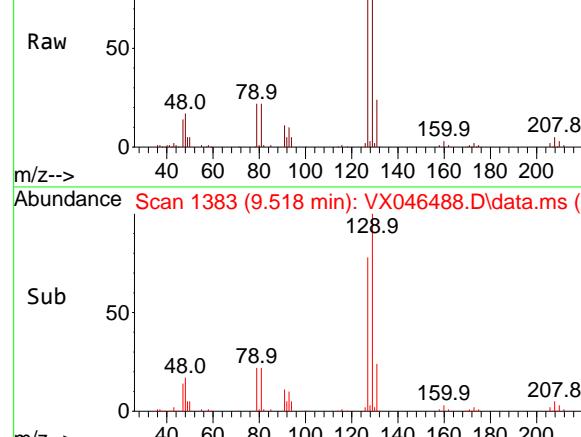

Abundance Scan 1383 (9.518 min): VX046488.D\data.ms (-1)

#59

2-Hexanone

Concen: 286.265 ug/l

RT: 9.427 min Scan# 1368

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

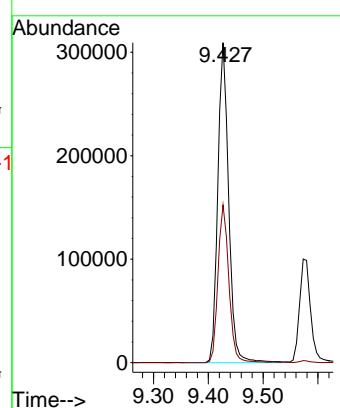

#60

Dibromochloromethane

Concen: 56.300 ug/l

RT: 9.518 min Scan# 1383

Delta R.T. -0.000 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12




Tgt Ion:129 Resp: 69918

Ion Ratio Lower Upper

129 100

127 78.1 39.3 117.8

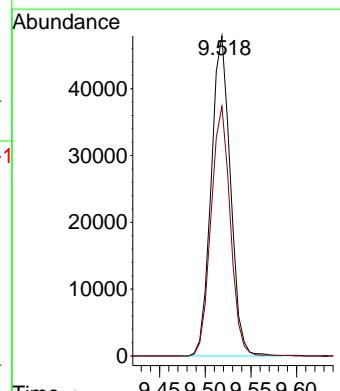

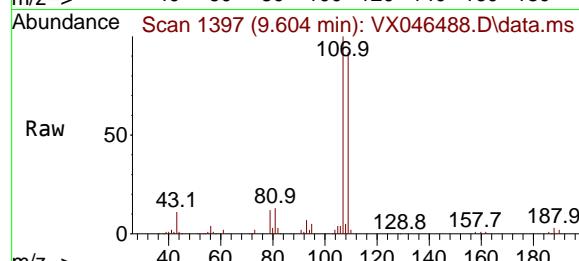

#61

1,2-Dibromoethane

Concen: 53.347 ug/l

RT: 9.604 min Scan# 1397

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

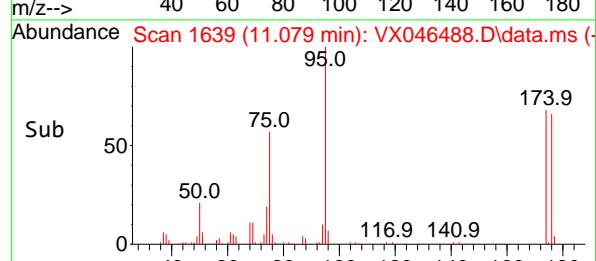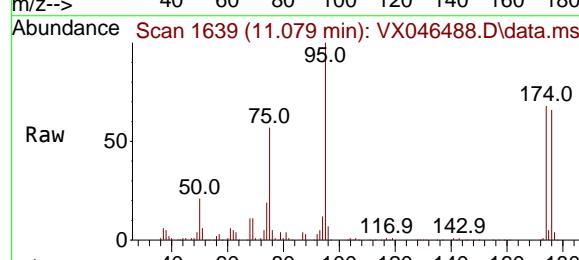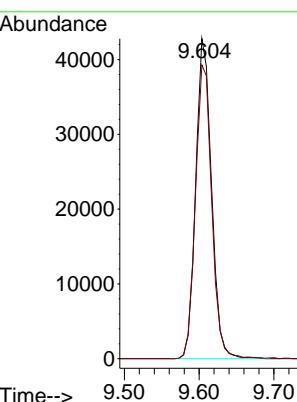

#62

4-Bromofluorobenzene

Concen: 49.083 ug/l


RT: 11.079 min Scan# 1639


Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt	Ion:	95	Resp:	77443
Ion	Ratio	Lower	Upper	
95	100			
174	66.9	0.0	135.8	
176	65.0	0.0	131.4	

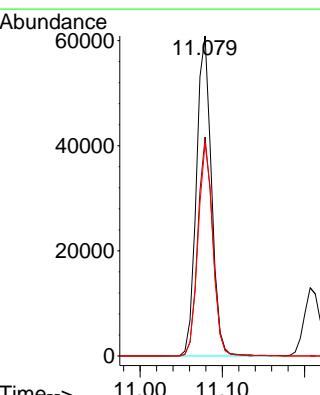


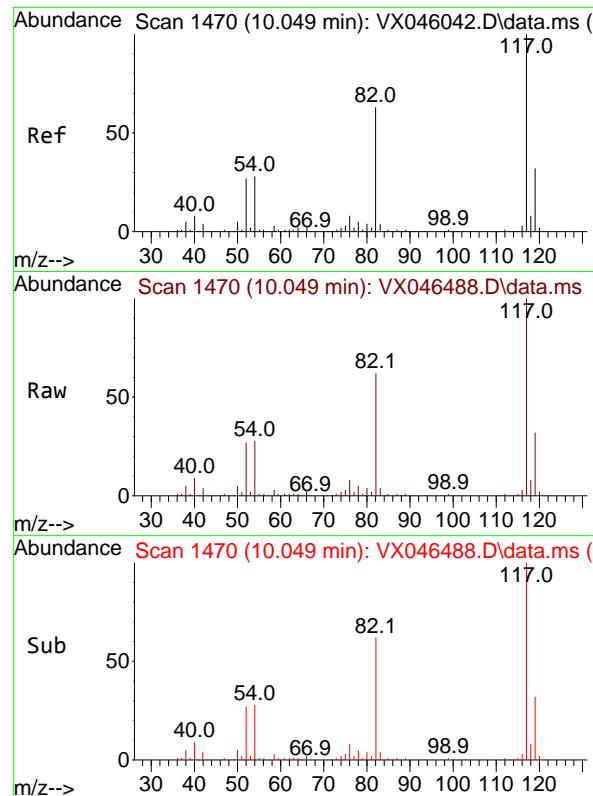


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 14115  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


**Manual Integrations**  
**APPROVED**


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

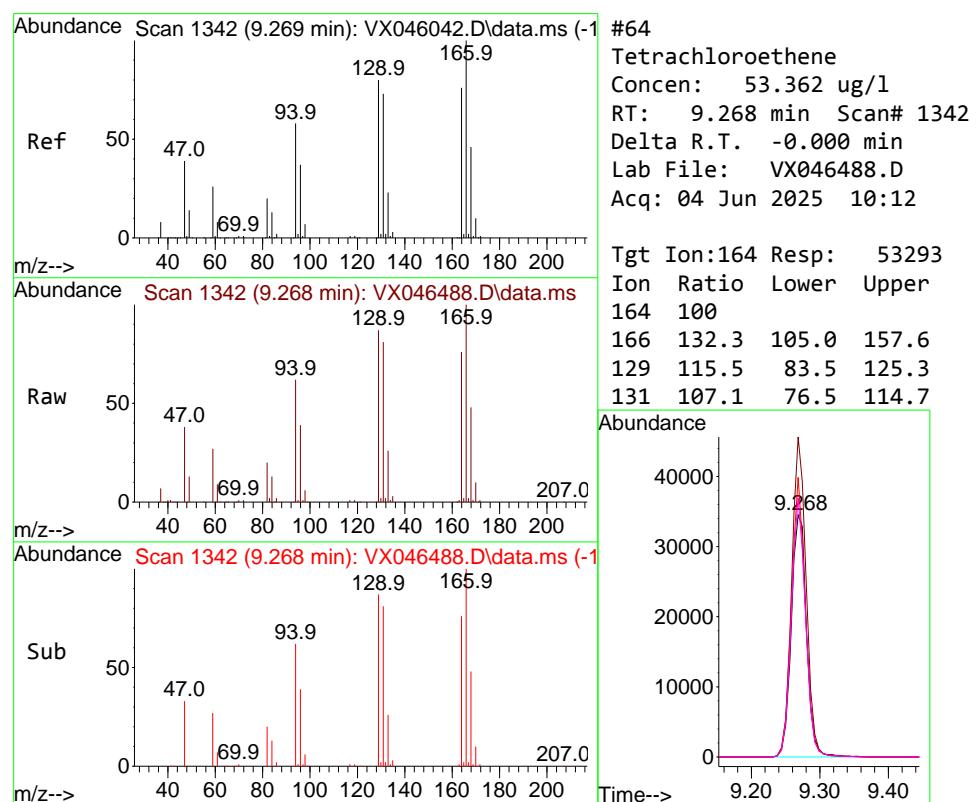

#64  
Tetrachloroethene  
Concen: 53.362 ug/l  
RT: 9.268 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion:164 Resp: 53293  
Ion Ratio Lower Upper  
164 100  
166 132.3 105.0 157.6  
129 115.5 83.5 125.3  
131 107.1 76.5 114.7




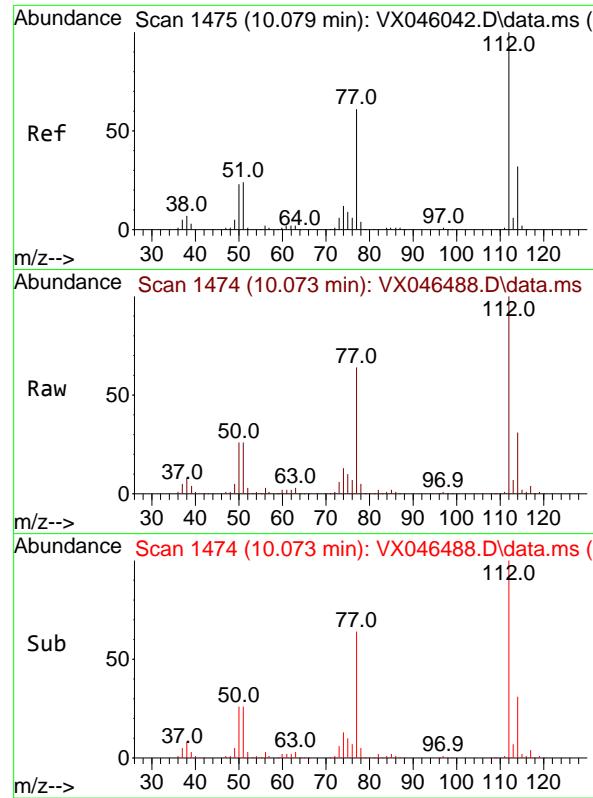


#65  
Chlorobenzene  
Concen: 53.386 ug/l  
RT: 10.073 min Scan# 1474  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12


Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050




**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

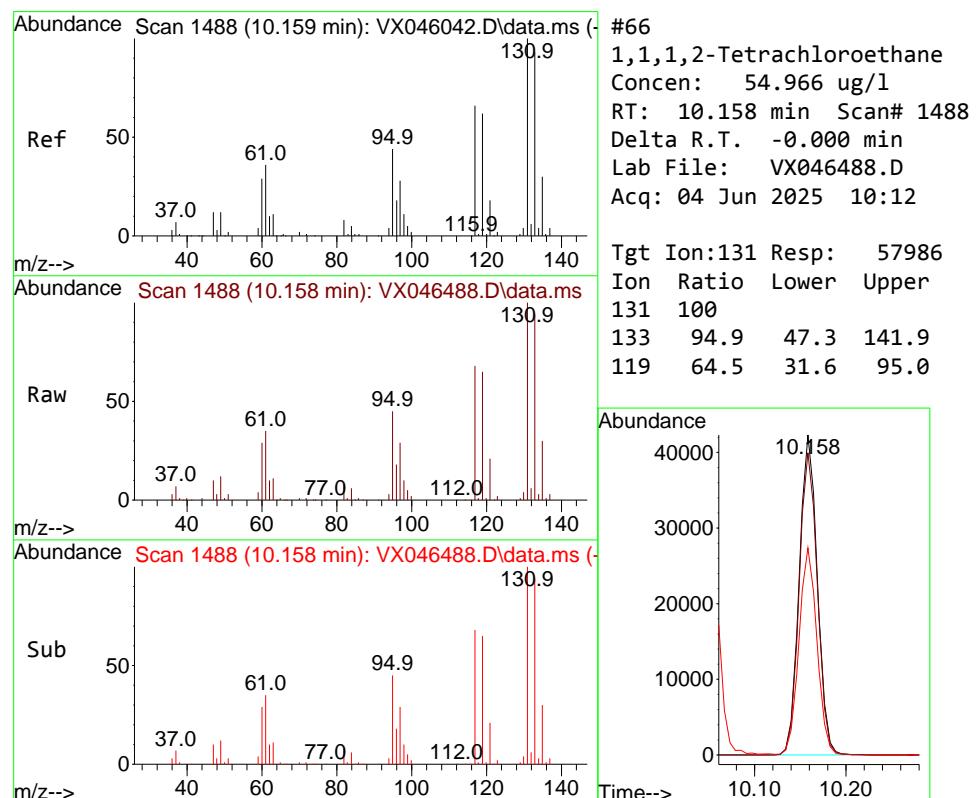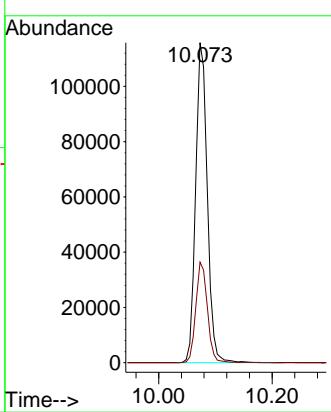

#66  
1,1,1,2-Tetrachloroethane  
Concen: 54.966 ug/l  
RT: 10.158 min Scan# 1488  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

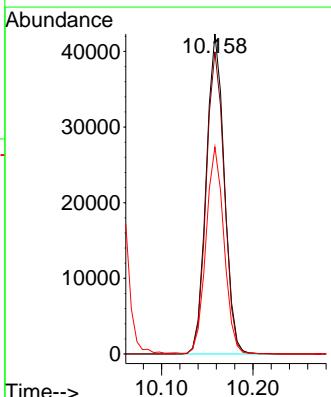

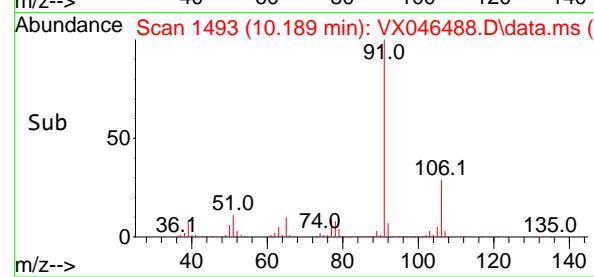

#67

Ethyl Benzene

Concen: 54.870 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

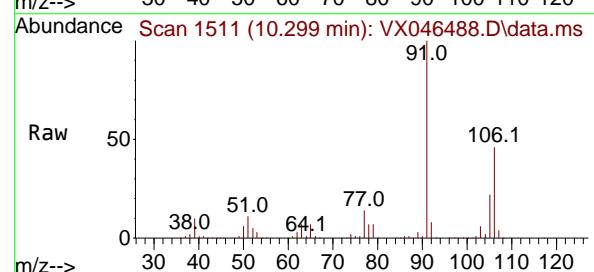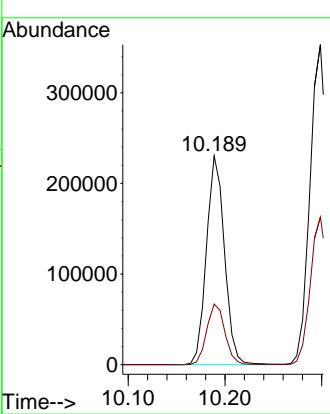

#68

m/p-Xylenes

Concen: 108.288 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12




Tgt Ion:106 Resp: 215687

Ion Ratio Lower Upper

106 100

91 218.1 171.2 256.8

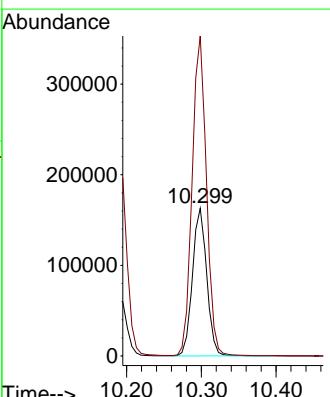







#69  
o-Xylene  
Concen: 54.982 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


Manual Integrations  
**APPROVED**




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

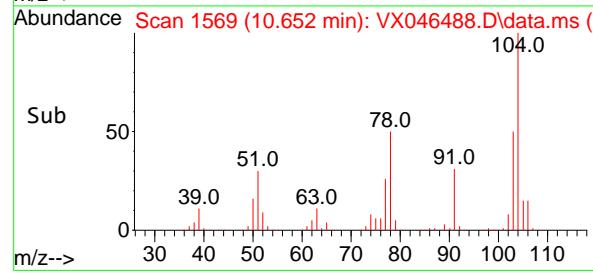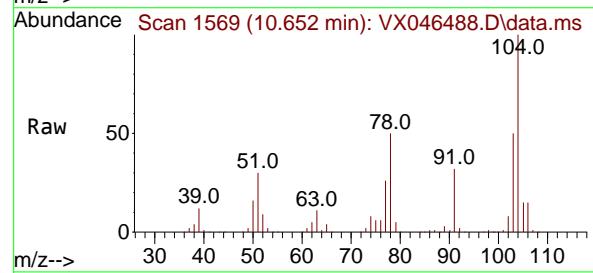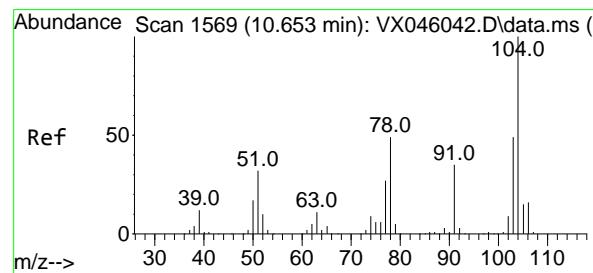

#70  
Styrene  
Concen: 56.926 ug/l  
RT: 10.652 min Scan# 1569  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion:104 Resp: 181074  
Ion Ratio Lower Upper  
104 100  
78 57.5 45.7 68.5  
103 54.9 43.7 65.5



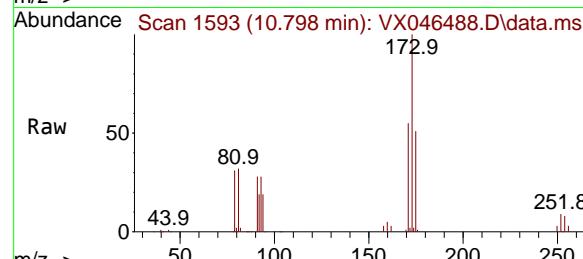

#71

Bromoform

Concen: 56.651 ug/l

RT: 10.798 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X




ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12


Tgt Ion:152 Resp: 69016


Ion Ratio Lower Upper

152 100

115 94.5 46.9 140.7

150 172.5 0.0 351.0

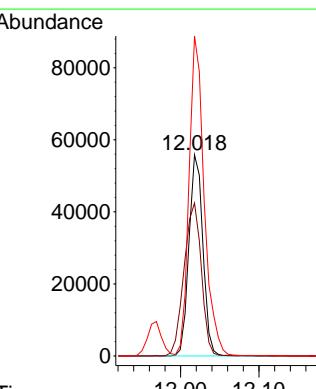

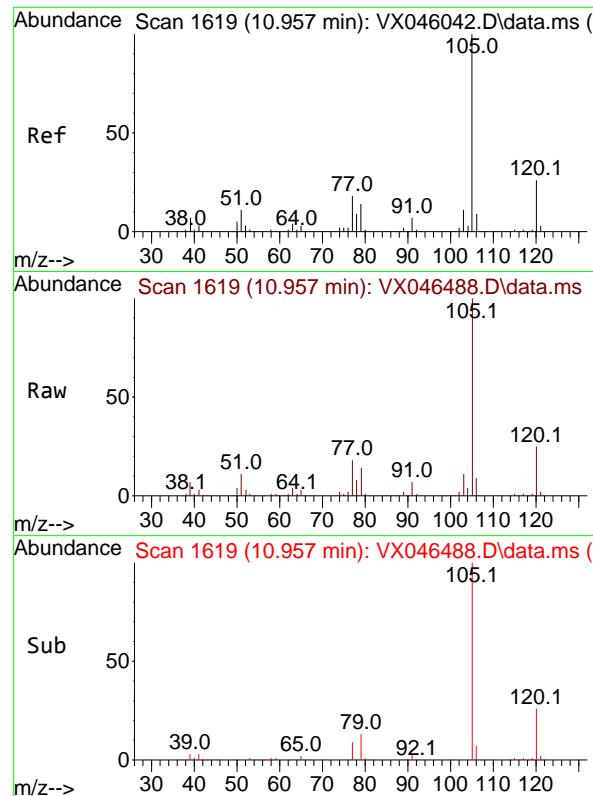

#73

Isopropylbenzene

Concen: 53.686 ug/l

RT: 10.957 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X



ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

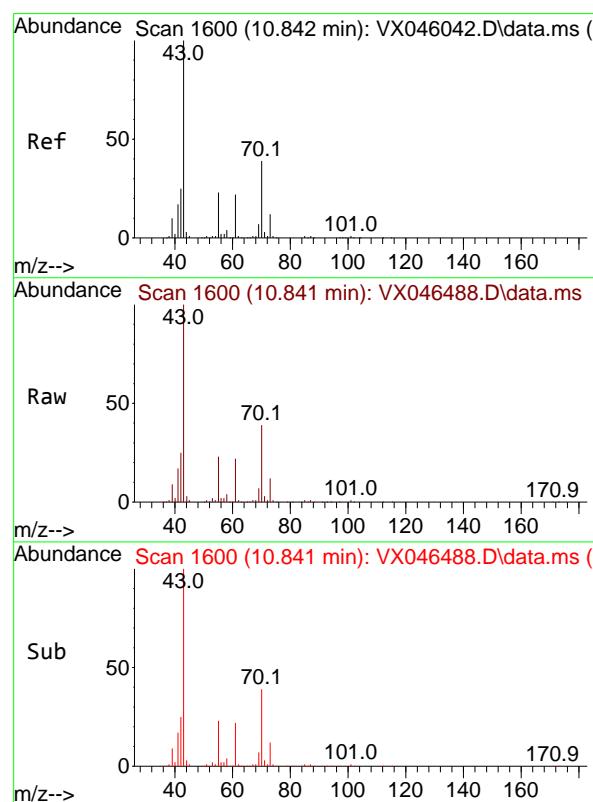

#74

N-amyl acetate

Concen: 55.656 ug/l


RT: 10.841 min Scan# 1600

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt	Ion:	43	Resp:	147771
Ion	Ratio	Lower	Upper	
43	100			
70	38.3	30.9	46.3	
55	22.8	18.7	28.1	
61	21.9	17.1	25.7	




#75  
 1,1,2,2-Tetrachloroethane  
 Concen: 50.752 ug/l  
 RT: 11.207 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: VX046488.D  
 Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
 ClientSampleId : VSTDCCC050

Tgt Ion: 83 Resp: 9556  
 Ion Ratio Lower Upper  
 83 100  
 131 10.1 5.0 14.9  
 85 64.5 31.9 95.7


### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

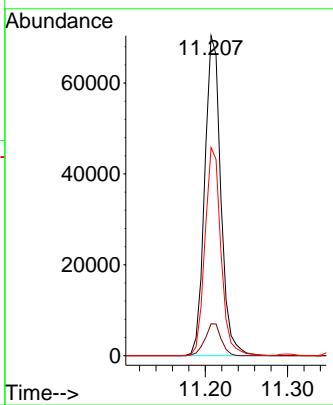



#76  
 1,2,3-Trichloropropane  
 Concen: 51.854 ug/l m  
 RT: 11.237 min Scan# 1665  
 Delta R.T. -0.000 min  
 Lab File: VX046488.D  
 Acq: 04 Jun 2025 10:12

Tgt Ion: 75 Resp: 86142  
 Ion Ratio Lower Upper  
 75 100  
 77 40.0 20.5 61.5




#76  
 1,2,3-Trichloropropane  
 Concen: 51.854 ug/l m  
 RT: 11.237 min Scan# 1665  
 Delta R.T. -0.000 min  
 Lab File: VX046488.D  
 Acq: 04 Jun 2025 10:12




Tgt Ion: 75 Resp: 86142  
 Ion Ratio Lower Upper  
 75 100  
 77 40.0 20.5 61.5

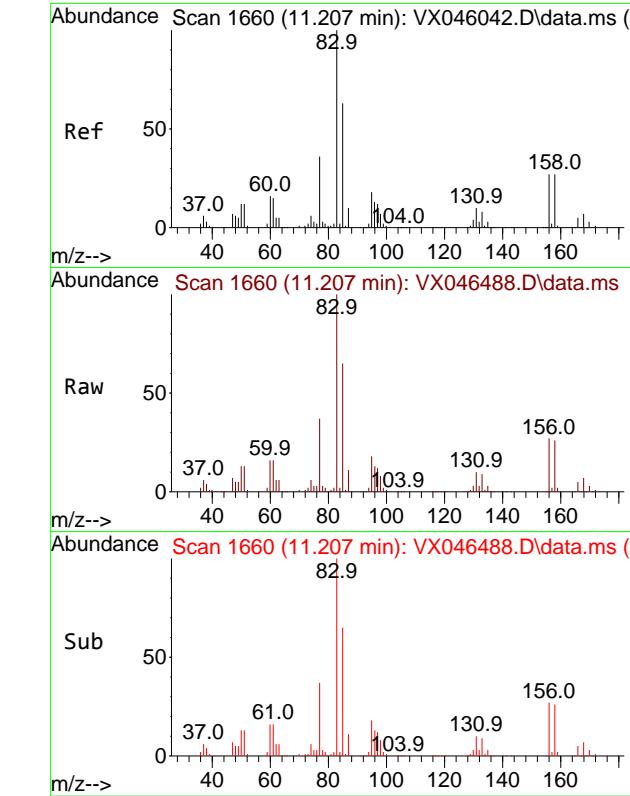

#75  
 1,1,2,2-Tetrachloroethane  
 Concen: 50.752 ug/l  
 RT: 11.207 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: VX046488.D  
 Acq: 04 Jun 2025 10:12

Tgt Ion: 83 Resp: 9556  
 Ion Ratio Lower Upper  
 83 100  
 131 10.1 5.0 14.9  
 85 64.5 31.9 95.7



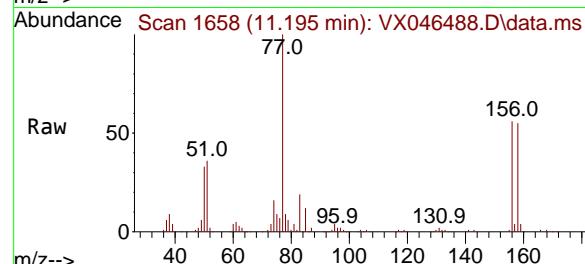

#77

Bromobenzene

Concen: 52.773 ug/l

RT: 11.195 min Scan# 1658

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

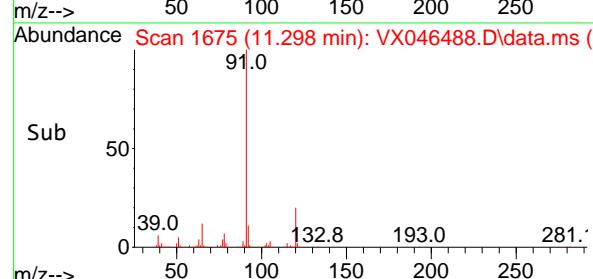

#78

n-propylbenzene

Concen: 54.223 ug/l

RT: 11.298 min Scan# 1675

Delta R.T. -0.000 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12

Tgt Ion: 91 Resp: 338759

Ion Ratio Lower Upper

91 100

120 21.5 10.8 32.4



#79

2-Chlorotoluene

Concen: 51.549 ug/l

RT: 11.359 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D




Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X





ClientSampleId :

VSTDCCC050

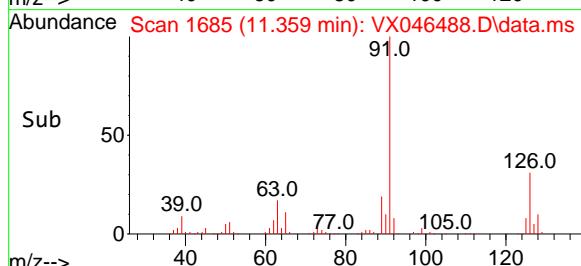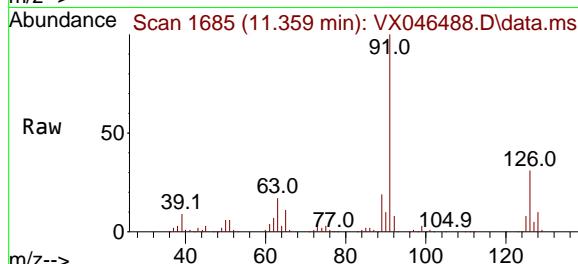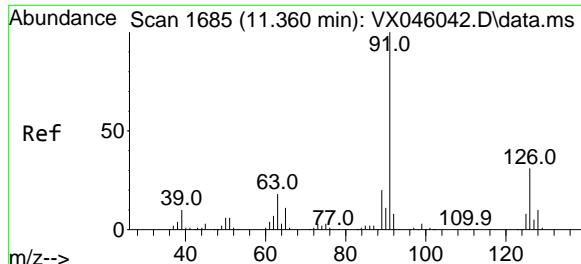
**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

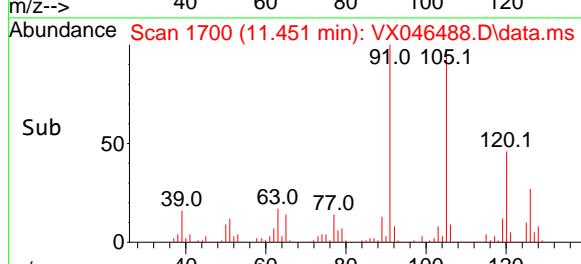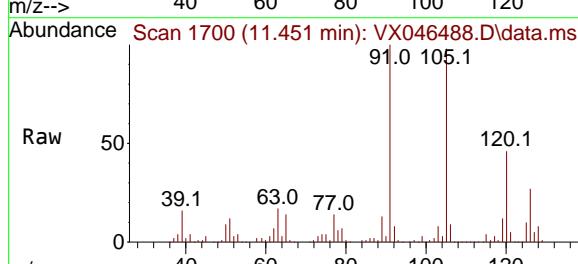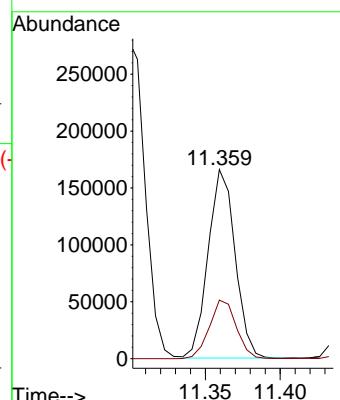

#80

1,3,5-Trimethylbenzene

Concen: 53.865 ug/l


RT: 11.451 min Scan# 1700


Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt Ion:105 Resp: 241792  
 Ion Ratio Lower Upper  
 105 100  
 120 46.4 23.1 69.2

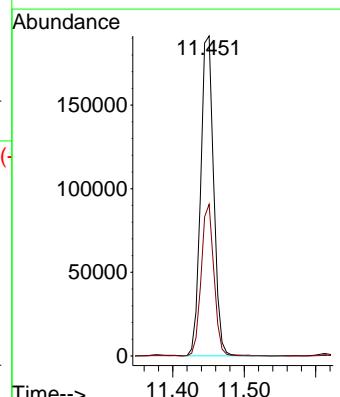


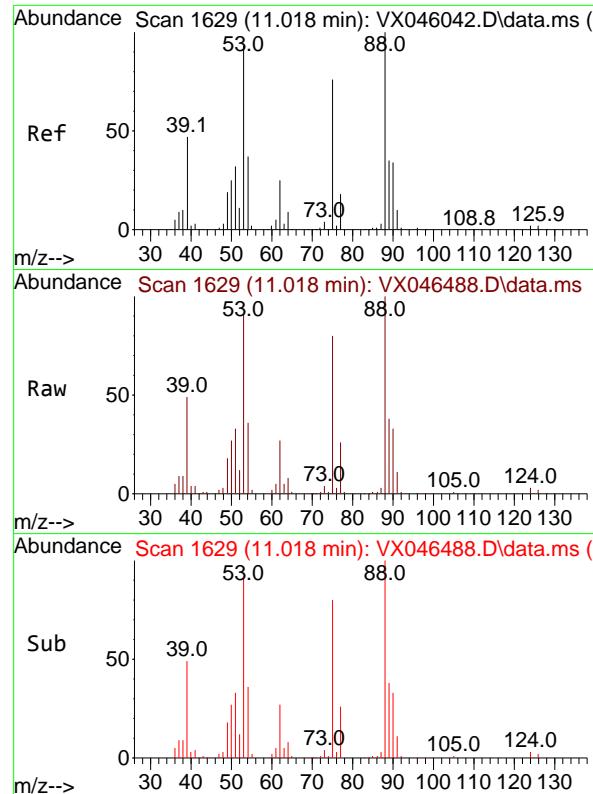


#81  
trans-1,4-Dichloro-2-butene  
Concen: 56.693 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

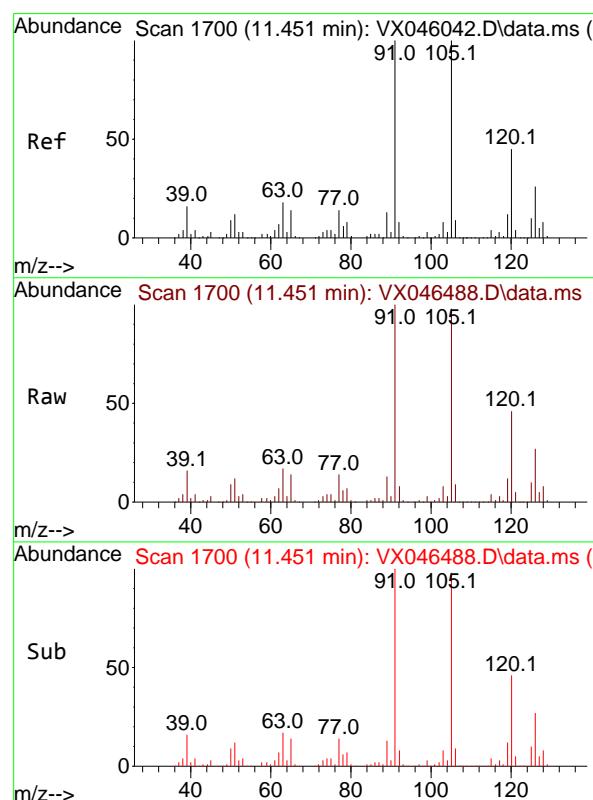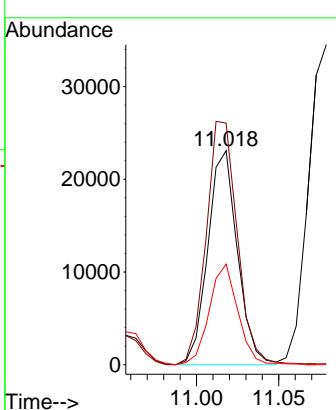

#82  
4-Chlorotoluene  
Concen: 53.864 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion: 91 Resp: 240706  
Ion Ratio Lower Upper  
91 100  
126 26.8 13.3 39.8

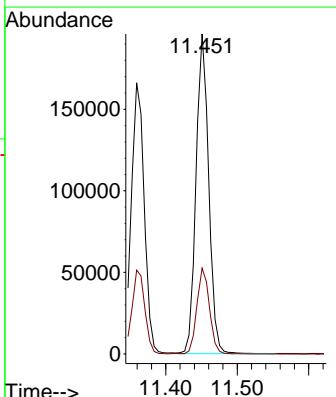



#83

tert-Butylbenzene

Concen: 53.206 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

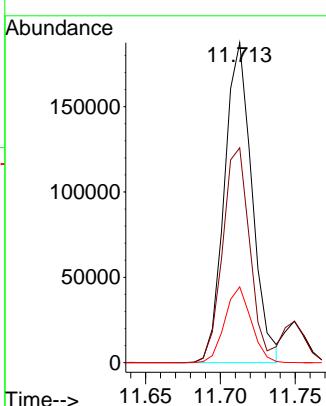

#84

1,2,4-Trimethylbenzene

Concen: 53.863 ug/l

RT: 11.749 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX046488.D


Acq: 04 Jun 2025 10:12




Tgt Ion:105 Resp: 244850

Ion Ratio Lower Upper

105 100

120 42.9 21.2 63.6

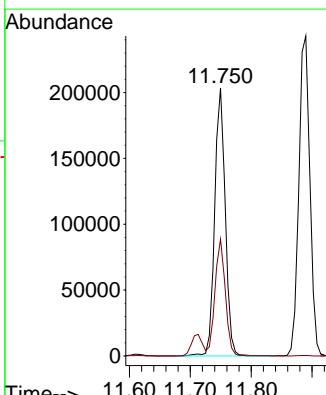



#85

sec-Butylbenzene

Concen: 54.891 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X




ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#86

p-Isopropyltoluene

Concen: 54.822 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12


Tgt Ion:119 Resp: 251225


Ion Ratio Lower Upper

119 100

134 25.6 12.5 37.5

91 27.6 13.8 41.4

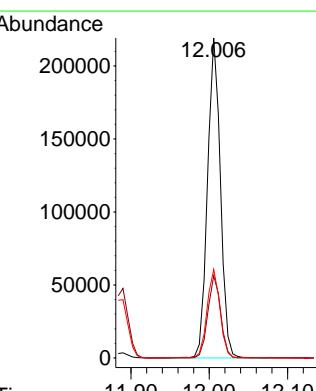

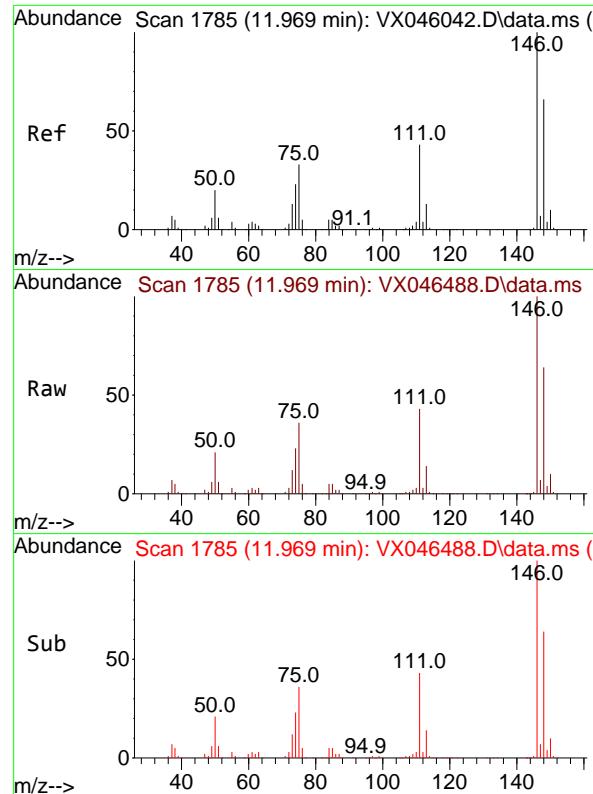

#87

1,3-Dichlorobenzene

Concen: 52.532 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X



ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

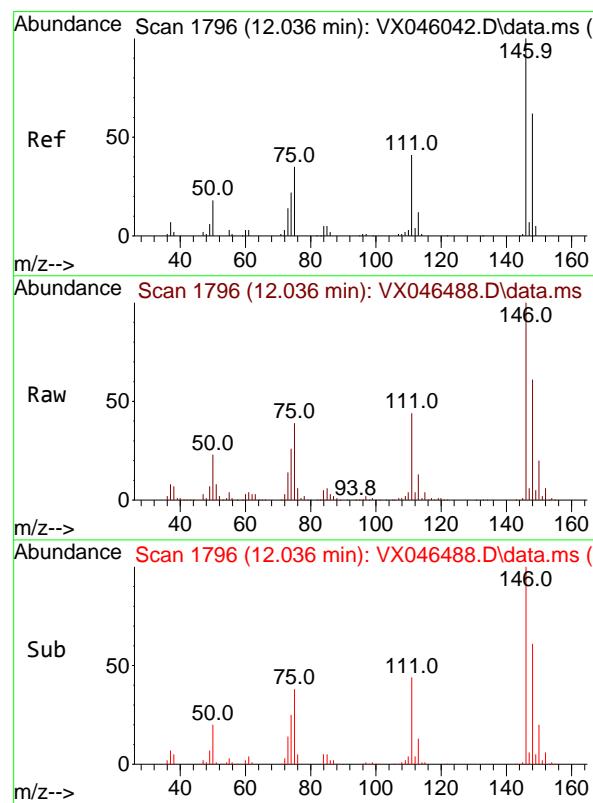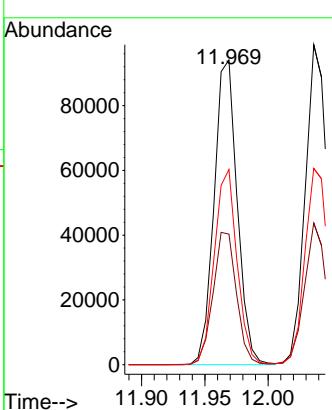

#88

1,4-Dichlorobenzene

Concen: 51.703 ug/l


RT: 12.036 min Scan# 1796




Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt	Ion:146	Resp:	120210
Ion	Ratio	Lower	Upper
146	100		
111	43.8	21.3	63.9
148	64.0	31.9	95.5



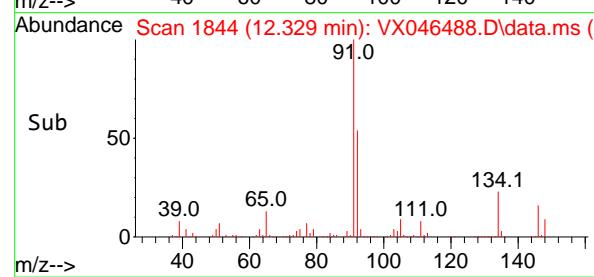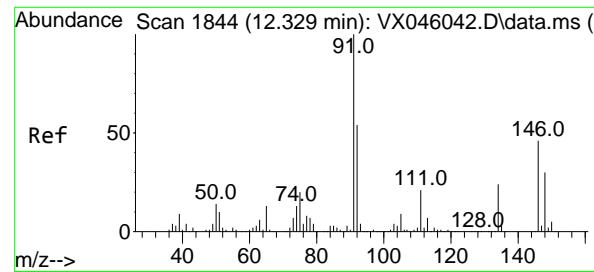

#89

n-Butylbenzene

Concen: 56.775 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X




ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

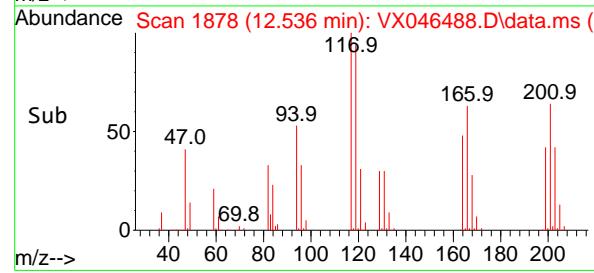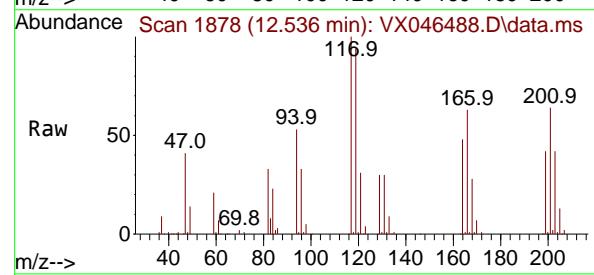

#90

Hexachloroethane

Concen: 54.668 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12



Tgt Ion:117 Resp: 44135

Ion Ratio Lower Upper

117 100

201 64.3 31.6 94.7



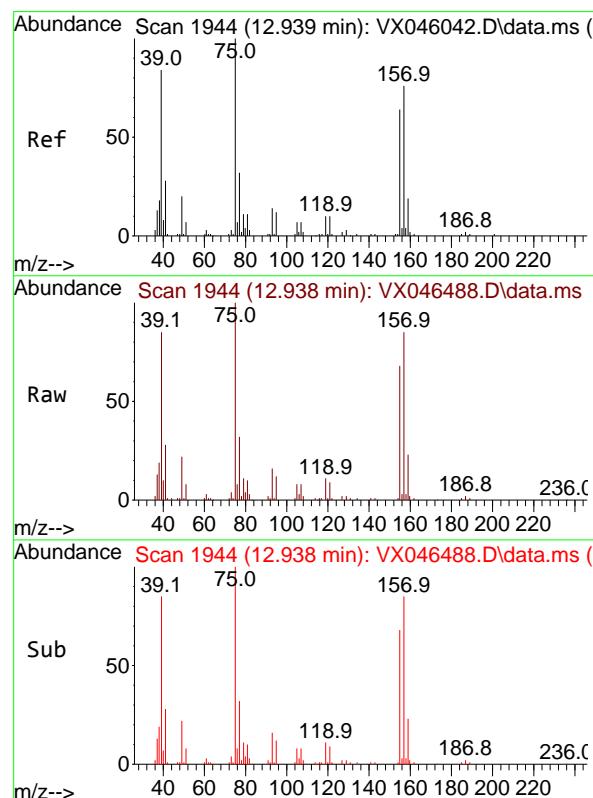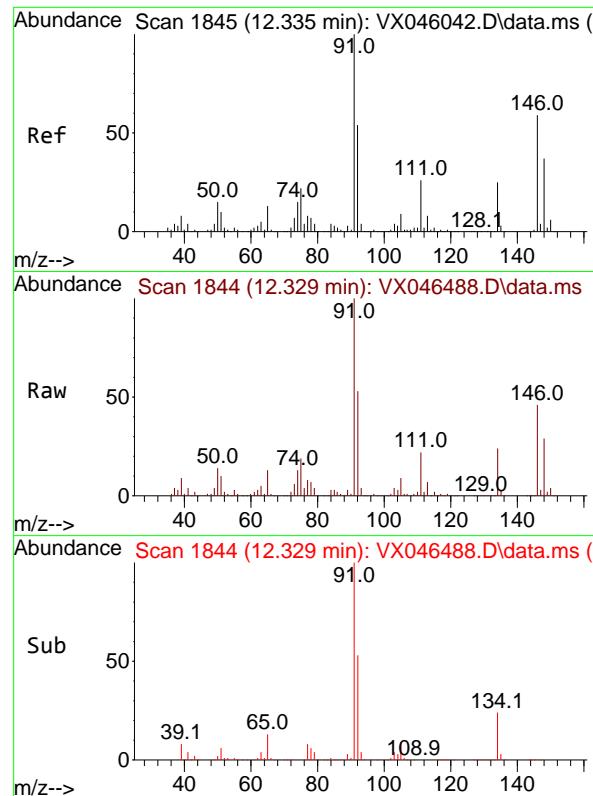

#91

1,2-Dichlorobenzene

Concen: 52.558 ug/l

RT: 12.329 min Scan# 1

Delta R.T. -0.007 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Instrument:

MSVOA\_X


ClientSampleId :

VSTDCCC050

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 54.746 ug/l


RT: 12.938 min Scan# 1944


Delta R.T. -0.000 min

Lab File: VX046488.D

Acq: 04 Jun 2025 10:12

Tgt	Ion:	Resp:	22836
Ion	Ratio	Lower	Upper
	75	100	
155	70.2	34.9	104.8
157	90.3	43.8	131.4




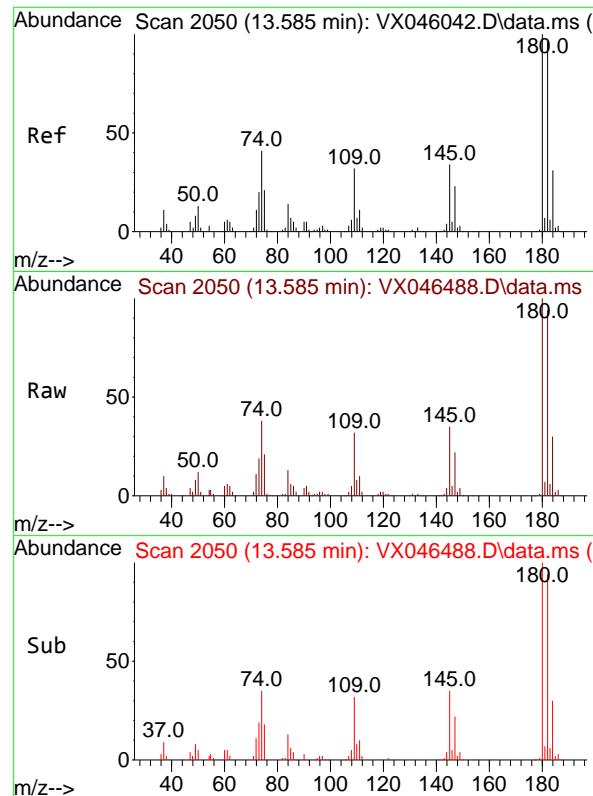


#93  
1,2,4-Trichlorobenzene  
Concen: 54.131 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument : MSVOA\_X  
ClientSampleId : VSTDCCC050


### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

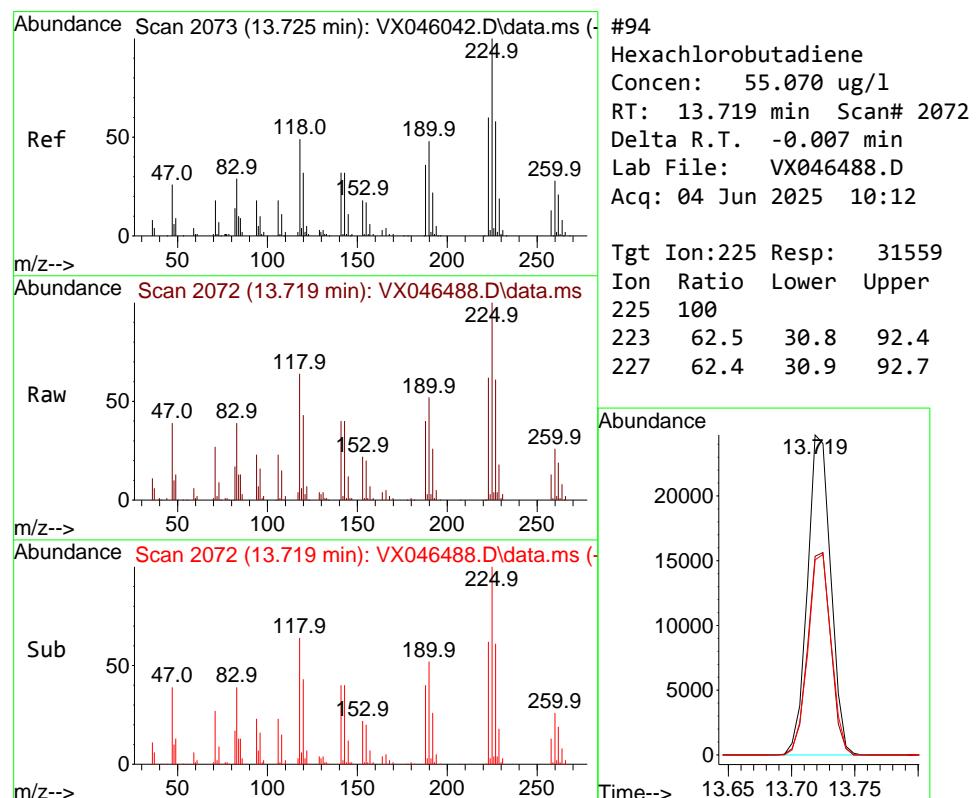

#94  
Hexachlorobutadiene  
Concen: 55.070 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. -0.007 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt Ion:225 Resp: 31559  
Ion Ratio Lower Upper  
225 100  
223 62.5 30.8 92.4  
227 62.4 30.9 92.7

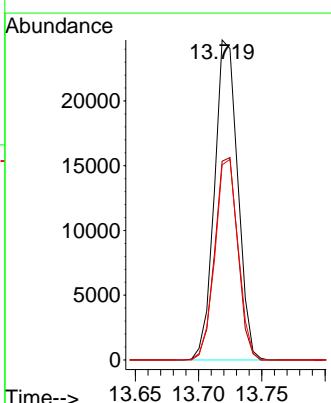

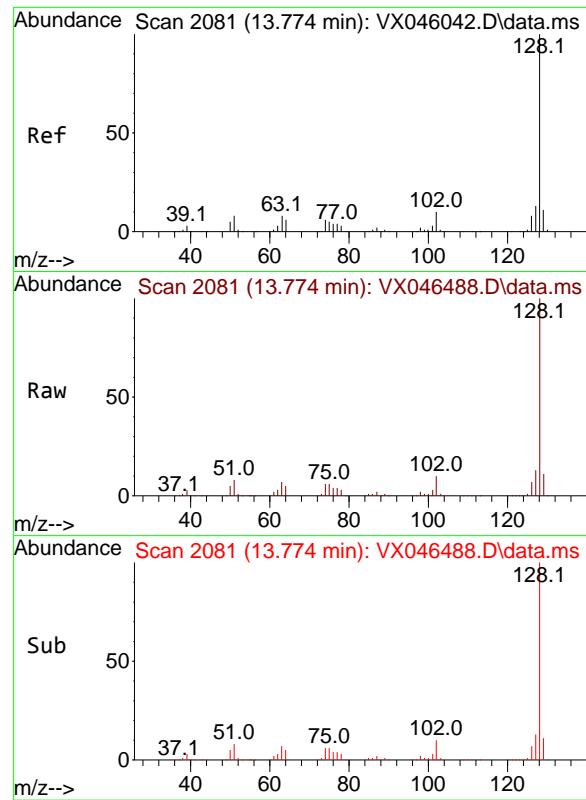



#95  
Naphthalene  
Concen: 53.657 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Instrument: MSVOA\_X  
Client SampleId: VSTDCCC050

Tgt	Ion:128	Resp:	258222
	Ion Ratio	Lower	Upper
128	100		
127	12.8	10.4	15.6
129	10.7	8.6	13.0


### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

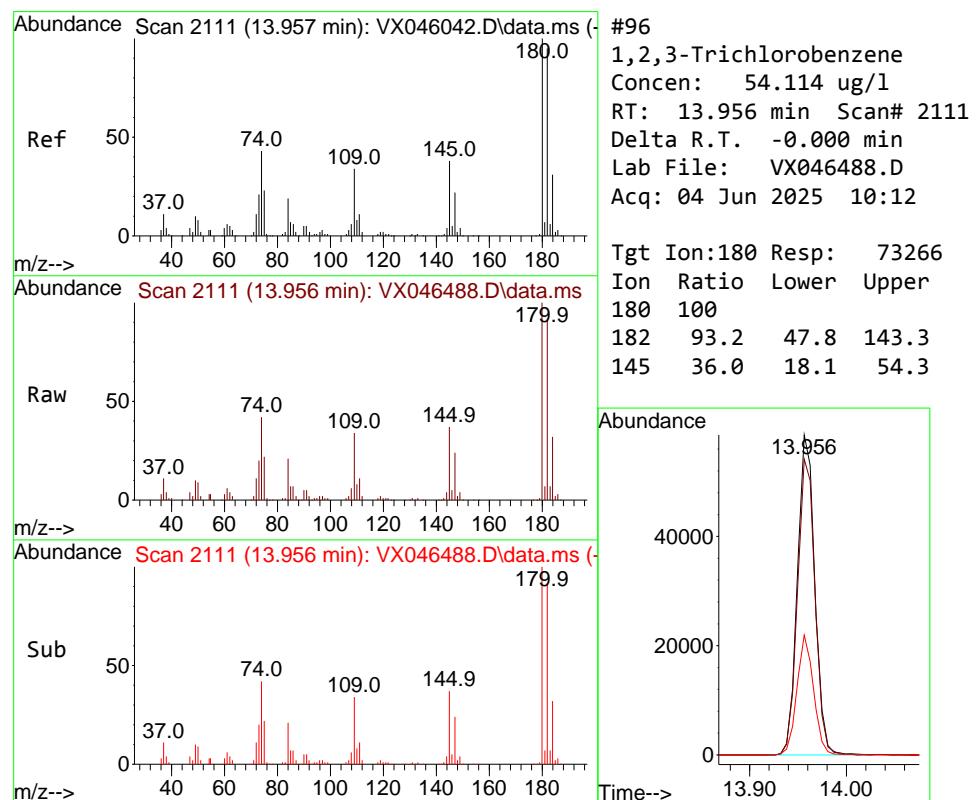

#96  
1,2,3-Trichlorobenzene  
Concen: 54.114 ug/l  
RT: 13.956 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046488.D  
Acq: 04 Jun 2025 10:12

Tgt	Ion:180	Resp:	73266
	Ion Ratio	Lower	Upper
180	100		
182	93.2	47.8	143.3
145	36.0	18.1	54.3

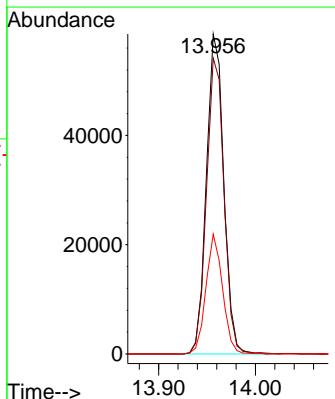

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046488.D  
 Acq On : 04 Jun 2025 10:12  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	100	0.00
2 T	Dichlorodifluoromethane	0.765	0.751	1.8	87	0.00
3 P	Chloromethane	0.742	0.718	3.2	93	0.00
4 C	Vinyl Chloride	0.691	0.665	3.8#	94	0.00
5 T	Bromomethane	0.320	0.277	13.4	85	0.00
6 T	Chloroethane	0.369	0.377	-2.2	100	0.00
7 T	Trichlorofluoromethane	1.021	1.059	-3.7	100	0.00
8 T	Diethyl Ether	0.347	0.357	-2.9	106	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.632	0.670	-6.0	105	0.00
10 T	Methyl Iodide	0.747	0.721	3.5	90	0.00
11 T	Tert butyl alcohol	0.131	0.148	-13.0	115	0.00
12 CM	1,1-Dichloroethene	0.593	0.593	0.0	99	0.00
13 T	Acrolein	0.149	0.149	0.0	98	0.00
14 T	Allyl chloride	1.133	1.239	-9.4	106	0.00
15 T	Acrylonitrile	0.374	0.403	-7.8	104	0.00
16 T	Acetone	0.374	0.442	-18.2	122	0.00
17 T	Carbon Disulfide	1.406	1.295	7.9	89	0.00
18 T	Methyl Acetate	0.867	1.200	-38.4#	142	0.00
19 T	Methyl tert-butyl Ether	2.079	2.295	-10.4	107	0.00
20 T	Methylene Chloride	0.716	0.693	3.2	102	0.00
21 T	trans-1,2-Dichloroethene	0.596	0.599	-0.5	99	0.00
22 T	Diisopropyl ether	2.189	2.407	-10.0	106	0.00
23 T	Vinyl Acetate	1.925	2.019	-4.9	99	0.00
24 P	1,1-Dichloroethane	1.219	1.302	-6.8	104	0.00
25 T	2-Butanone	0.543	0.606	-11.6	110	0.00
26 T	2,2-Dichloropropane	0.954	1.059	-11.0	111	0.00
27 T	cis-1,2-Dichloroethene	0.718	0.747	-4.0	102	0.00
28 T	Bromochloromethane	0.587	0.546	7.0	95	-0.01
29 T	Tetrahydrofuran	0.340	0.373	-9.7	107	0.00
30 C	Chloroform	1.271	1.335	-5.0#	103	0.00
31 T	Cyclohexane	1.111	1.106	0.5	98	0.00
32 T	1,1,1-Trichloroethane	1.101	1.161	-5.4	103	0.00
33 S	1,2-Dichloroethane-d4	0.932	0.862	7.5	95	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	98	0.00
35 S	Dibromofluoromethane	0.360	0.356	1.1	99	0.00
36 T	1,1-Dichloropropene	0.484	0.506	-4.5	100	0.00
37 T	Ethyl Acetate	0.598	0.637	-6.5	103	0.00
38 T	Carbon Tetrachloride	0.544	0.588	-8.1	103	0.00
39 T	Methylcyclohexane	0.623	0.650	-4.3	100	0.00
40 TM	Benzene	1.417	1.496	-5.6	100	0.00
41 T	Methacrylonitrile	0.313	0.370	-18.2	105	0.00
42 TM	1,2-Dichloroethane	0.612	0.651	-6.4	102	0.00
43 T	Isopropyl Acetate	0.912	1.045	-14.6	107	0.00
44 TM	Trichloroethene	0.341	0.364	-6.7	101	0.00
45 C	1,2-Dichloropropane	0.352	0.386	-9.7#	102	0.00
46 T	Dibromomethane	0.278	0.292	-5.0	100	0.00
47 T	Bromodichloromethane	0.547	0.606	-10.8	103	0.00
48 T	Methyl methacrylate	0.466	0.538	-15.5	105	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046488.D  
 Acq On : 04 Jun 2025 10:12  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.009	0.009	0.0	102	0.00
50 S	Toluene-d8	1.246	1.135	8.9	91	0.00
51 T	4-Methyl-2-Pentanone	0.605	0.678	-12.1	105	0.00
52 CM	Toluene	0.869	0.902	-3.8#	99	0.00
53 T	t-1,3-Dichloropropene	0.487	0.557	-14.4	104	0.00
54 T	cis-1,3-Dichloropropene	0.538	0.614	-14.1	104	0.00
55 T	1,1,2-Trichloroethane	0.343	0.370	-7.9	103	0.00
56 T	Ethyl methacrylate	0.546	0.640	-17.2	106	0.00
57 T	1,3-Dichloropropane	0.615	0.650	-5.7	103	0.00
58 T	2-Chloroethyl Vinyl ether	0.278	0.306	-10.1	98	0.00
59 T	2-Hexanone	0.448	0.513	-14.5	107	0.00
60 T	Dibromochloromethane	0.376	0.424	-12.8	104	0.00
61 T	1,2-Dibromoethane	0.356	0.380	-6.7	100	0.00
62 S	4-Bromofluorobenzene	0.478	0.469	1.9	98	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	97	0.00
64 T	Tetrachloroethene	0.354	0.378	-6.8	97	0.00
65 PM	Chlorobenzene	1.094	1.168	-6.8	103	0.00
66 T	1,1,1,2-Tetrachloroethane	0.374	0.411	-9.9	102	0.00
67 C	Ethyl Benzene	1.929	2.117	-9.7#	101	0.00
68 T	m/p-Xylenes	0.706	0.764	-8.2	100	0.00
69 T	o-Xylene	0.688	0.756	-9.9	100	0.00
70 T	Styrene	1.127	1.283	-13.8	102	0.00
71 P	Bromoform	0.281	0.318	-13.2	101	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	102	0.00
73 T	Isopropylbenzene	3.893	4.180	-7.4	103	0.00
74 T	N-amyl acetate	1.924	2.141	-11.3	105	0.00
75 P	1,1,2,2-Tetrachloroethane	1.364	1.385	-1.5	105	0.00
76 T	1,2,3-Trichloropropane	1.204	1.248	-3.7	107	0.00
77 T	Bromobenzene	0.904	0.954	-5.5	104	0.00
78 T	n-propylbenzene	4.526	4.908	-8.4	103	0.00
79 T	2-Chlorotoluene	2.919	3.010	-3.1	102	0.00
80 T	1,3,5-Trimethylbenzene	3.252	3.503	-7.7	102	0.00
81 T	trans-1,4-Dichloro-2-butene	0.370	0.419	-13.2	111	0.00
82 T	4-Chlorotoluene	3.238	3.488	-7.7	103	0.00
83 T	tert-Butylbenzene	3.276	3.486	-6.4	103	0.00
84 T	1,2,4-Trimethylbenzene	3.293	3.548	-7.7	102	0.00
85 T	sec-Butylbenzene	4.022	4.415	-9.8	105	0.00
86 T	p-Isopropyltoluene	3.320	3.640	-9.6	104	0.00
87 T	1,3-Dichlorobenzene	1.649	1.733	-5.1	103	0.00
88 T	1,4-Dichlorobenzene	1.684	1.742	-3.4	104	0.00
89 T	n-Butylbenzene	2.912	3.307	-13.6	107	0.00
90 T	Hexachloroethane	0.585	0.639	-9.2	104	0.00
91 T	1,2-Dichlorobenzene	1.655	1.740	-5.1	104	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.302	0.331	-9.6	104	0.00
93 T	1,2,4-Trichlorobenzene	0.951	1.029	-8.2	107	0.00
94 T	Hexachlorobutadiene	0.415	0.457	-10.1	109	0.00
95 T	Naphthalene	3.487	3.742	-7.3	105	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
Data File : VX046488.D  
Acq On : 04 Jun 2025 10:12  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
LabSampleId :  
VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	0.981	1.062	-8.3	106	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 5

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046488.D  
 Acq On : 04 Jun 2025 10:12  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	100	0.00
2 T	Dichlorodifluoromethane	50.000	49.043	1.9	87	0.00
3 P	Chloromethane	50.000	48.377	3.2	93	0.00
4 C	Vinyl Chloride	50.000	48.151	3.7#	94	0.00
5 T	Bromomethane	50.000	43.237	13.5	85	0.00
6 T	Chloroethane	50.000	51.093	-2.2	100	0.00
7 T	Trichlorofluoromethane	50.000	51.858	-3.7	100	0.00
8 T	Diethyl Ether	50.000	51.308	-2.6	106	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	53.034	-6.1	105	0.00
10 T	Methyl Iodide	50.000	48.225	3.5	90	0.00
11 T	Tert butyl alcohol	250.000	281.901	-12.8	115	0.00
12 CM	1,1-Dichloroethene	50.000	49.990	0.0#	99	0.00
13 T	Acrolein	250.000	249.577	0.2	98	0.00
14 T	Allyl chloride	50.000	54.671	-9.3	106	0.00
15 T	Acrylonitrile	250.000	269.611	-7.8	104	0.00
16 T	Acetone	250.000	295.318	-18.1	122	0.00
17 T	Carbon Disulfide	50.000	46.054	7.9	89	0.00
18 T	Methyl Acetate	50.000	69.175	-38.3#	142	0.00
19 T	Methyl tert-butyl Ether	50.000	55.198	-10.4	107	0.00
20 T	Methylene Chloride	50.000	48.357	3.3	102	0.00
21 T	trans-1,2-Dichloroethene	50.000	50.199	-0.4	99	0.00
22 T	Diisopropyl ether	50.000	54.976	-10.0	106	0.00
23 T	Vinyl Acetate	250.000	262.170	-4.9	99	0.00
24 P	1,1-Dichloroethane	50.000	53.406	-6.8	104	0.00
25 T	2-Butanone	250.000	279.346	-11.7	110	0.00
26 T	2,2-Dichloropropane	50.000	55.512	-11.0	111	0.00
27 T	cis-1,2-Dichloroethene	50.000	52.056	-4.1	102	0.00
28 T	Bromochloromethane	50.000	46.549	6.9	95	-0.01
29 T	Tetrahydrofuran	250.000	274.234	-9.7	107	0.00
30 C	Chloroform	50.000	52.542	-5.1#	103	0.00
31 T	Cyclohexane	50.000	49.761	0.5	98	0.00
32 T	1,1,1-Trichloroethane	50.000	52.691	-5.4	103	0.00
33 S	1,2-Dichloroethane-d4	50.000	46.217	7.6	95	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	98	0.00
35 S	Dibromofluoromethane	50.000	49.466	1.1	99	0.00
36 T	1,1-Dichloropropene	50.000	52.307	-4.6	100	0.00
37 T	Ethyl Acetate	50.000	53.296	-6.6	103	0.00
38 T	Carbon Tetrachloride	50.000	54.045	-8.1	103	0.00
39 T	Methylcyclohexane	50.000	52.202	-4.4	100	0.00
40 TM	Benzene	50.000	52.789	-5.6	100	0.00
41 T	Methacrylonitrile	50.000	59.164	-18.3	105	0.00
42 TM	1,2-Dichloroethane	50.000	53.188	-6.4	102	0.00
43 T	Isopropyl Acetate	50.000	57.328	-14.7	107	0.00
44 TM	Trichloroethene	50.000	53.347	-6.7	101	0.00
45 C	1,2-Dichloropropane	50.000	54.797	-9.6#	102	0.00
46 T	Dibromomethane	50.000	52.494	-5.0	100	0.00
47 T	Bromodichloromethane	50.000	55.341	-10.7	103	0.00
48 T	Methyl methacrylate	50.000	57.719	-15.4	105	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046488.D  
 Acq On : 04 Jun 2025 10:12  
 Operator : JC/MD  
 Sample : VSTDCCC050  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 LabSampleId :  
 VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	1071.717	-7.2	102	0.00
50 S	Toluene-d8	50.000	45.524	9.0	91	0.00
51 T	4-Methyl-2-Pentanone	250.000	280.031	-12.0	105	0.00
52 CM	Toluene	50.000	51.931	-3.9#	99	0.00
53 T	t-1,3-Dichloropropene	50.000	57.213	-14.4	104	0.00
54 T	cis-1,3-Dichloropropene	50.000	57.106	-14.2	104	0.00
55 T	1,1,2-Trichloroethane	50.000	54.064	-8.1	103	0.00
56 T	Ethyl methacrylate	50.000	58.611	-17.2	106	0.00
57 T	1,3-Dichloropropane	50.000	52.850	-5.7	103	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	274.981	-10.0	98	0.00
59 T	2-Hexanone	250.000	286.265	-14.5	107	0.00
60 T	Dibromochloromethane	50.000	56.300	-12.6	104	0.00
61 T	1,2-Dibromoethane	50.000	53.347	-6.7	100	0.00
62 S	4-Bromofluorobenzene	50.000	49.083	1.8	98	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	97	0.00
64 T	Tetrachloroethene	50.000	53.362	-6.7	97	0.00
65 PM	Chlorobenzene	50.000	53.386	-6.8	103	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	54.966	-9.9	102	0.00
67 C	Ethyl Benzene	50.000	54.870	-9.7#	101	0.00
68 T	m/p-Xylenes	100.000	108.288	-8.3	100	0.00
69 T	o-Xylene	50.000	54.982	-10.0	100	0.00
70 T	Styrene	50.000	56.926	-13.9	102	0.00
71 P	Bromoform	50.000	56.651	-13.3	101	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	102	0.00
73 T	Isopropylbenzene	50.000	53.686	-7.4	103	0.00
74 T	N-amyl acetate	50.000	55.656	-11.3	105	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	50.752	-1.5	105	0.00
76 T	1,2,3-Trichloropropane	50.000	51.854	-3.7	107	0.00
77 T	Bromobenzene	50.000	52.773	-5.5	104	0.00
78 T	n-propylbenzene	50.000	54.223	-8.4	103	0.00
79 T	2-Chlorotoluene	50.000	51.549	-3.1	102	0.00
80 T	1,3,5-Trimethylbenzene	50.000	53.865	-7.7	102	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	56.693	-13.4	111	0.00
82 T	4-Chlorotoluene	50.000	53.864	-7.7	103	0.00
83 T	tert-Butylbenzene	50.000	53.206	-6.4	103	0.00
84 T	1,2,4-Trimethylbenzene	50.000	53.863	-7.7	102	0.00
85 T	sec-Butylbenzene	50.000	54.891	-9.8	105	0.00
86 T	p-Isopropyltoluene	50.000	54.822	-9.6	104	0.00
87 T	1,3-Dichlorobenzene	50.000	52.532	-5.1	103	0.00
88 T	1,4-Dichlorobenzene	50.000	51.703	-3.4	104	0.00
89 T	n-Butylbenzene	50.000	56.775	-13.5	107	0.00
90 T	Hexachloroethane	50.000	54.668	-9.3	104	0.00
91 T	1,2-Dichlorobenzene	50.000	52.558	-5.1	104	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	54.746	-9.5	104	0.00
93 T	1,2,4-Trichlorobenzene	50.000	54.131	-8.3	107	0.00
94 T	Hexachlorobutadiene	50.000	55.070	-10.1	109	0.00
95 T	Naphthalene	50.000	53.657	-7.3	105	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
Data File : VX046488.D  
Acq On : 04 Jun 2025 10:12  
Operator : JC/MD  
Sample : VSTDCCC050  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
LabSampleId :  
VSTDCCC050

Quant Time: Jun 05 01:34:12 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
Quant Title : SW846 8260  
QLast Update : Tue May 06 07:12:22 2025  
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	Amount	Calc.	%Dev	Area	% Dev(min)
96 T 1,2,3-Trichlorobenzene	50.000	54.114	-8.2	106	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



# QC SAMPLE


# DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX050525\  
 Data File : VX046038.D  
 Acq On : 05 May 2025 09:37  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Title : SW846 8260  
 Last Update : Tue May 06 07:12:22 2025

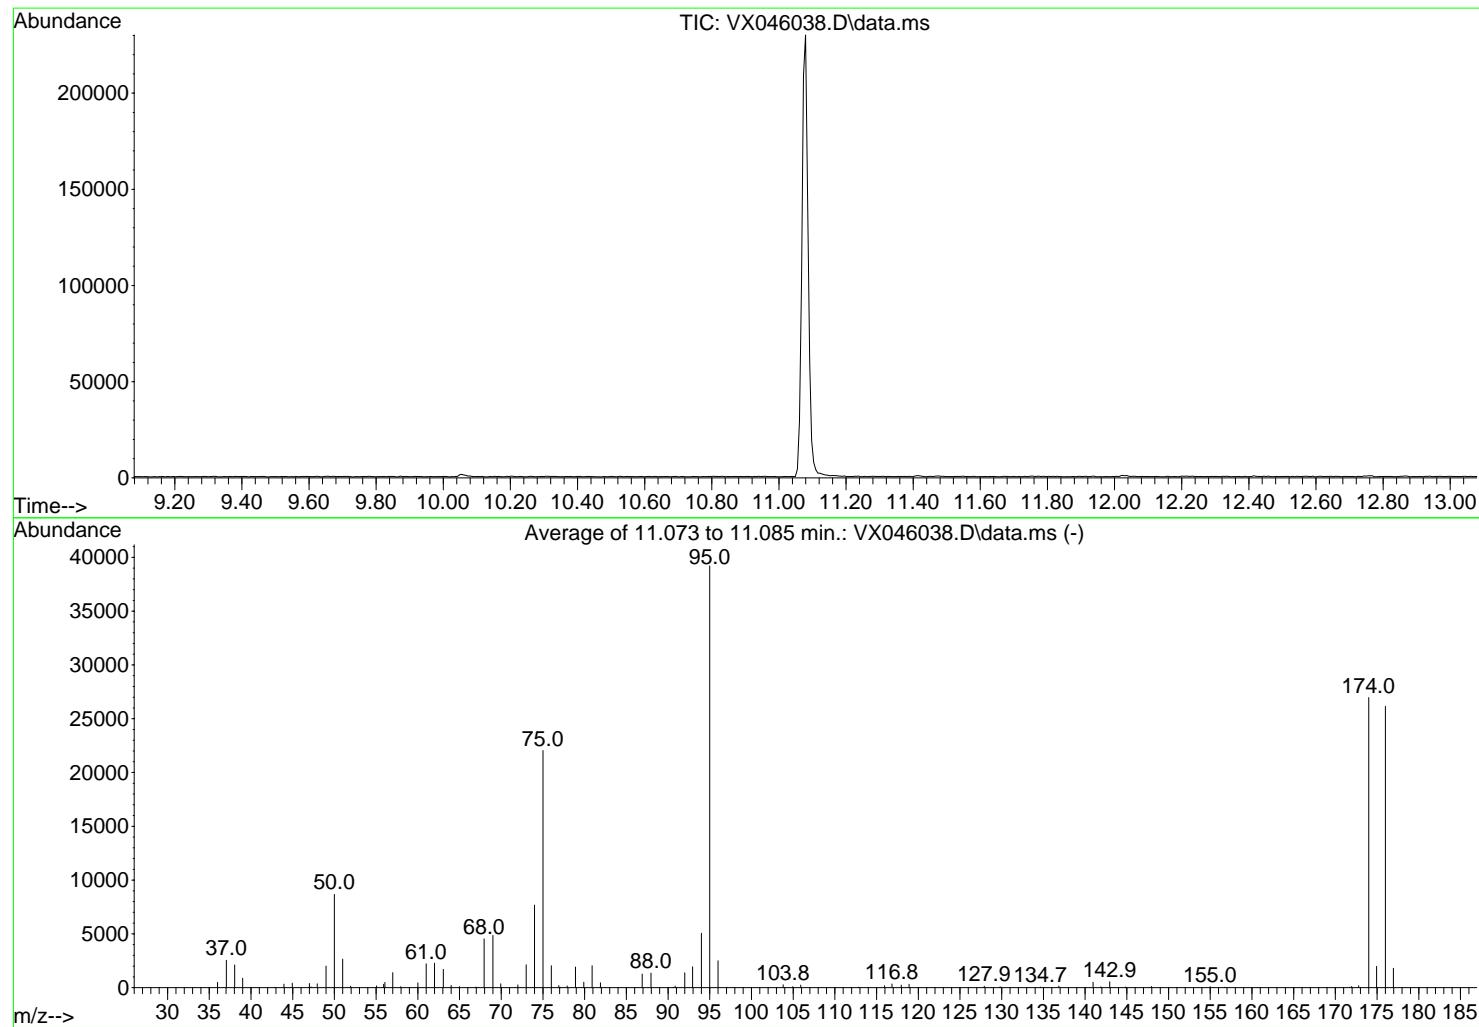

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	8676	PASS
75	95	30	60	56.2	22052	PASS
95	95	100	100	100.0	39213	PASS
96	95	5	9	6.4	2505	PASS
173	174	0.00	2	0.7	185	PASS
174	95	50	100	68.8	26963	PASS
175	174	5	9	7.3	1980	PASS
176	174	95	101	97.0	26147	PASS
177	176	5	9	6.9	1802	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046487.D  
 Acq On : 04 Jun 2025 09:43  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Title : SW846 8260  
 Last Update : Tue May 06 07:12:22 2025

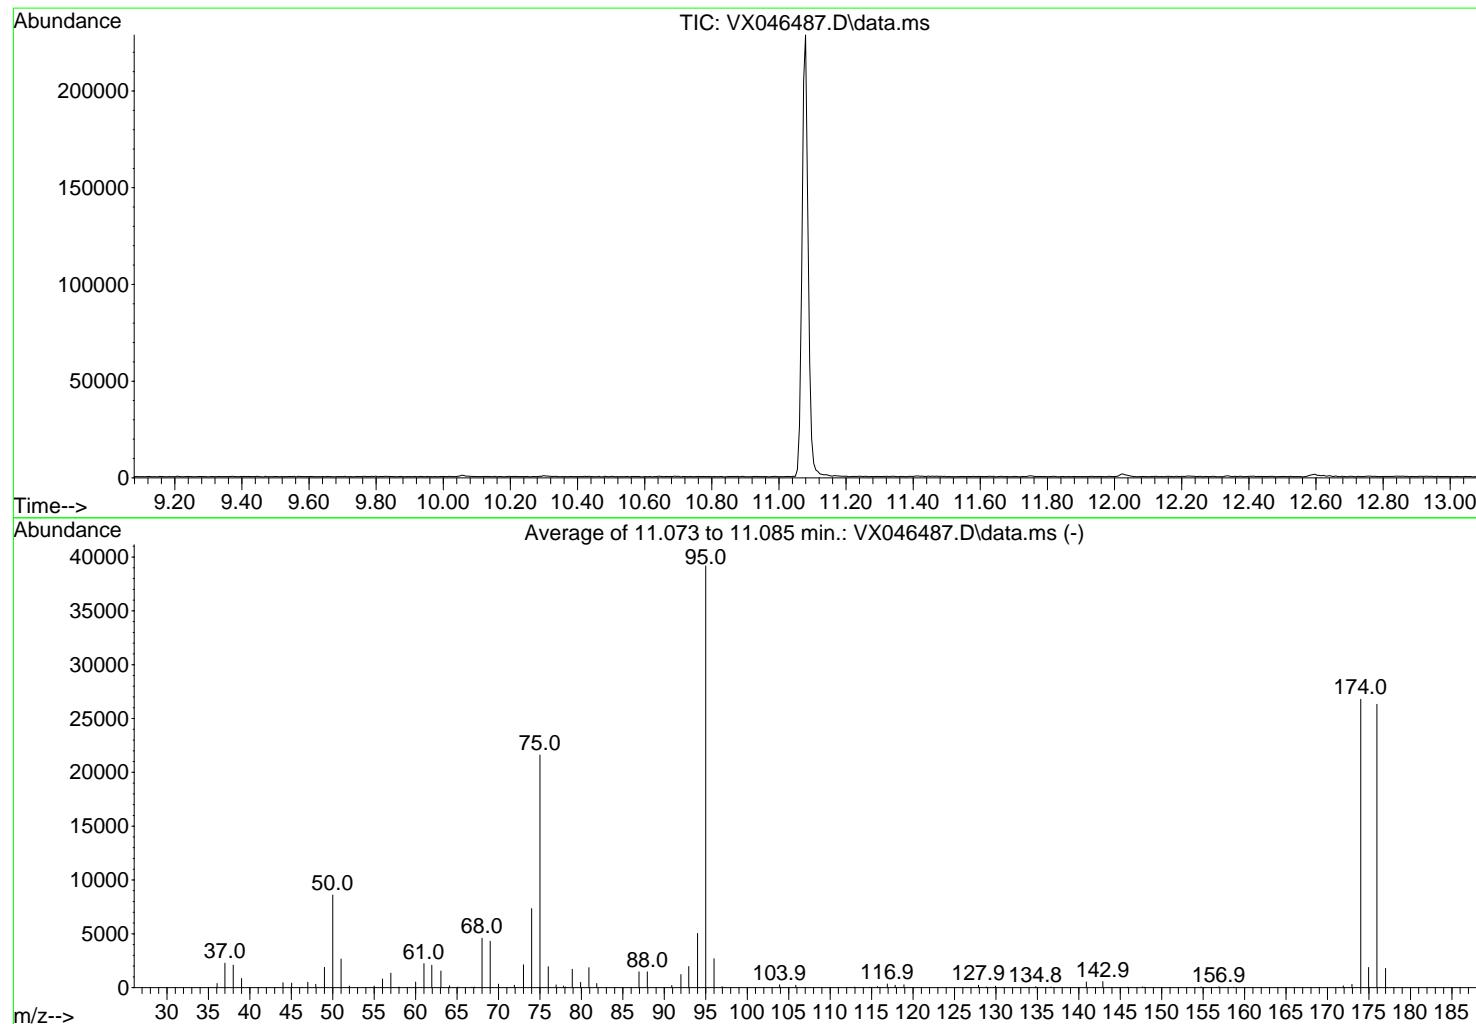

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	8608	PASS
75	95	30	60	55.2	21617	PASS
95	95	100	100	100.0	39181	PASS
96	95	5	9	6.9	2684	PASS
173	174	0.00	2	1.2	316	PASS
174	95	50	100	68.4	26784	PASS
175	174	5	9	7.0	1878	PASS
176	174	95	101	98.3	26320	PASS
177	176	5	9	6.8	1780	PASS



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	
Client Sample ID:	VX0604WBL01			SDG No.:	Q2200
Lab Sample ID:	VX0604WBL01			Matrix:	Water
Analytical Method:	8260D			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046490.D	1		06/04/25 11:04	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	53.4		70 (74) - 130 (125)	107%	SPK: 50
1868-53-7	Dibromofluoromethane	50.4		70 (75) - 130 (124)	101%	SPK: 50
2037-26-5	Toluene-d8	50.4		70 (86) - 130 (113)	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	53.1		70 (77) - 130 (121)	106%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	69600	5.55			
540-36-3	1,4-Difluorobenzene	140000	6.757			
3114-55-4	Chlorobenzene-d5	134000	10.049			
3855-82-1	1,4-Dichlorobenzene-d4	60000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046490.D  
 Acq On : 04 Jun 2025 11:04  
 Operator : JC/MD  
 Sample : VX0604WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBL01

Quant Time: Jun 05 01:39:03 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	69580	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	139946	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	133992	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	59967	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	69212	53.355	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 106.720%			
35) Dibromofluoromethane	5.379	113	50780	50.389	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 100.780%			
50) Toluene-d8	8.647	98	175770	50.393	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 100.780%			
62) 4-Bromofluorobenzene	11.079	95	71016	53.079	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 106.160%			




Target Compounds	Qvalue
(#= qualifier out of range (m) = manual integration (+) = signals summed	

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046490.D  
 Acq On : 04 Jun 2025 11:04  
 Operator : JC/MD  
 Sample : VX0604WBL01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBL01




Quant Time: Jun 05 01:39:03 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

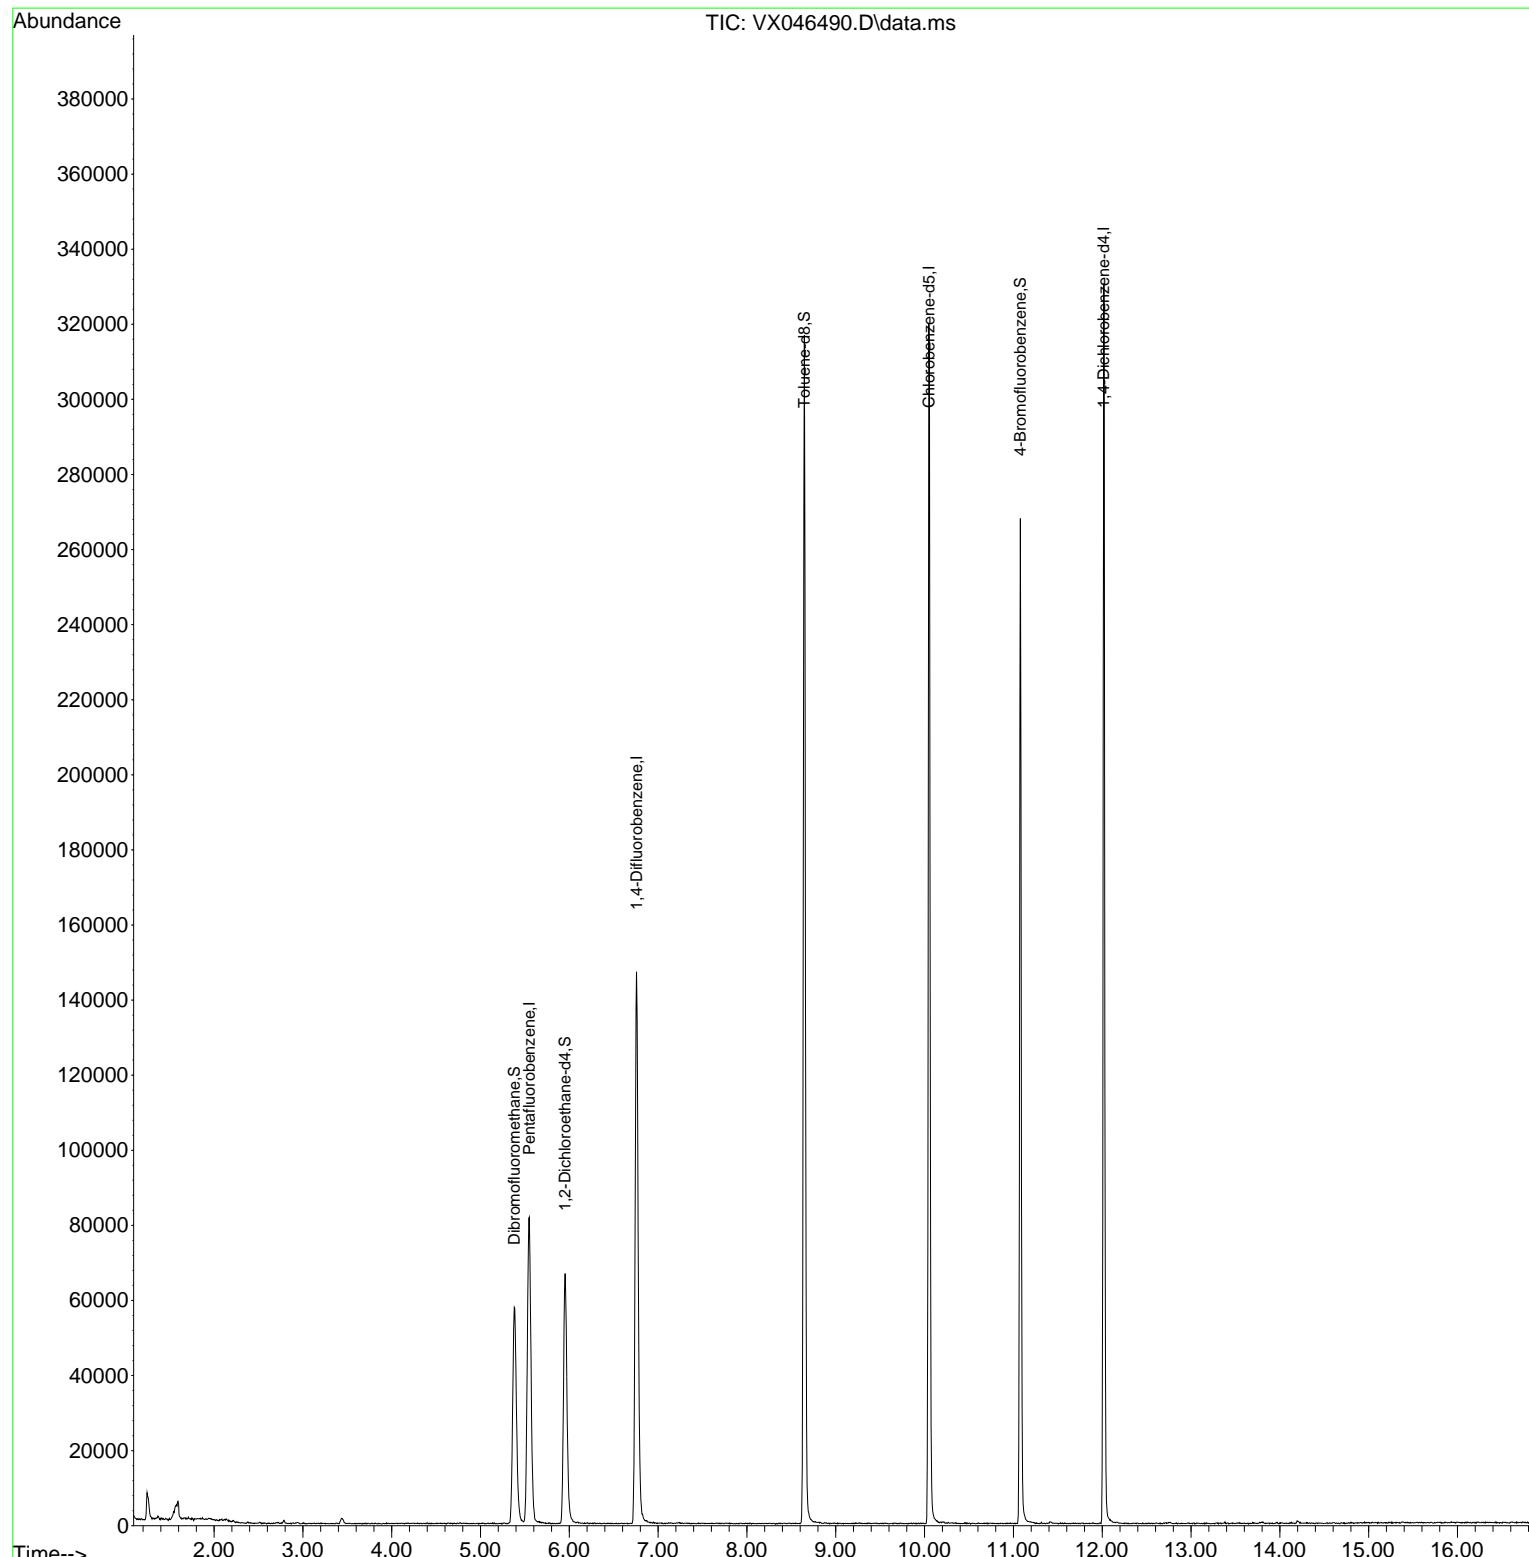





#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Instrument : MSVOA\_X  
Delta R.T. 0.006 min  
Lab File: VX046490.D  
Acq: 04 Jun 2025 11:04  
ClientSampleId : VX0604WBL01


Tgt Ion:168 Resp: 69580  
Ion Ratio Lower Upper  
168 100  
99 73.9 54.9 82.3

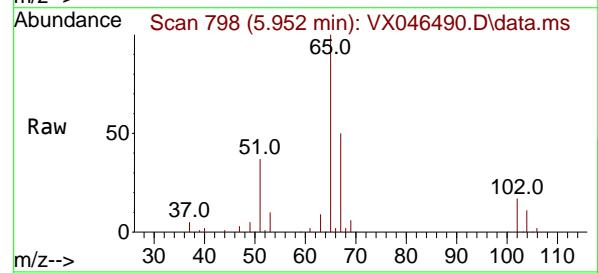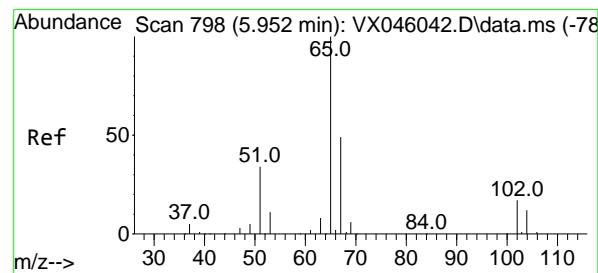

#33  
1,2-Dichloroethane-d4  
Concen: 53.355 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.000 min  
Lab File: VX046490.D  
Acq: 04 Jun 2025 11:04

Tgt Ion: 65 Resp: 69212  
Ion Ratio Lower Upper  
65 100  
67 48.1 0.0 99.0

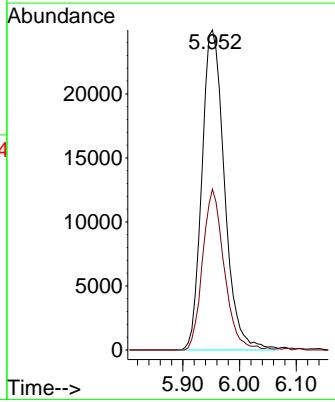

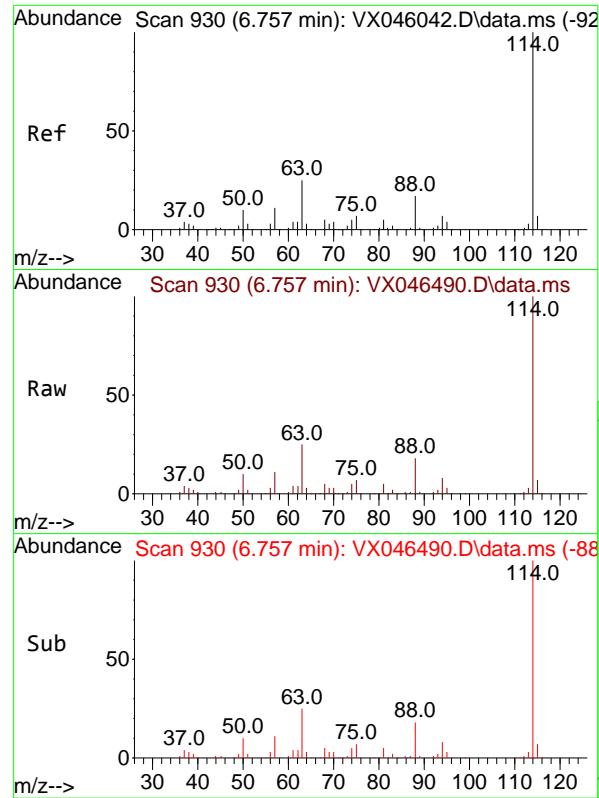

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 9

Delta R.T. -0.000 min

Lab File: VX046490.D

Acq: 04 Jun 2025 11:04

Instrument:

MSVOA\_X

ClientSampleId :

VX0604WBL01

Tgt Ion:114 Resp: 139946

Ion Ratio Lower Upper

114 100

63 24.8 0.0 49.2

88 18.0 0.0 33.6

Abundance

50000

40000


30000

20000

10000

0

Time--&gt; 6.60 6.70 6.80 6.90

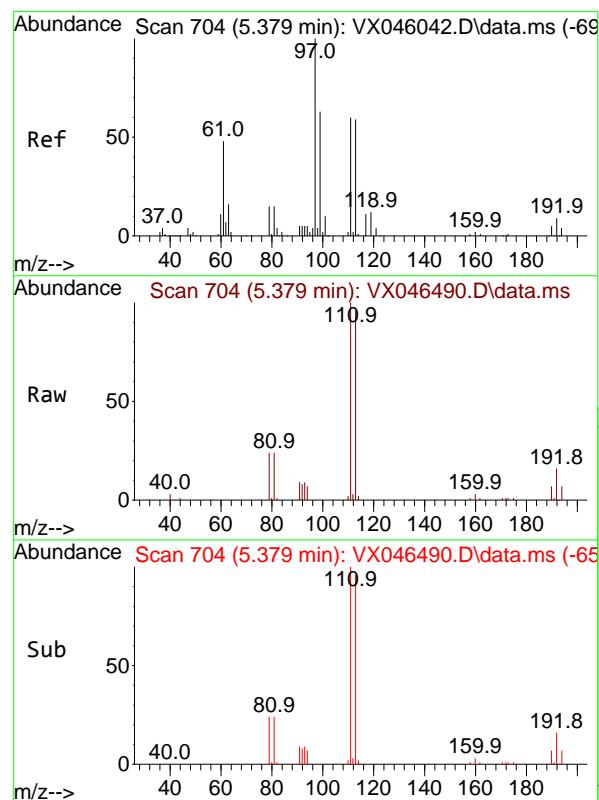

#35

Dibromofluoromethane

Concen: 50.389 ug/l

RT: 5.379 min Scan# 704

Delta R.T. -0.000 min

Lab File: VX046490.D

Acq: 04 Jun 2025 11:04

Tgt Ion:113 Resp: 50780

Ion Ratio Lower Upper

113 100

111 102.0 83.1 124.7

192 16.4 13.3 19.9

Abundance




15000

10000

5000

0





Time--&gt; 5.30 5.40 5.50

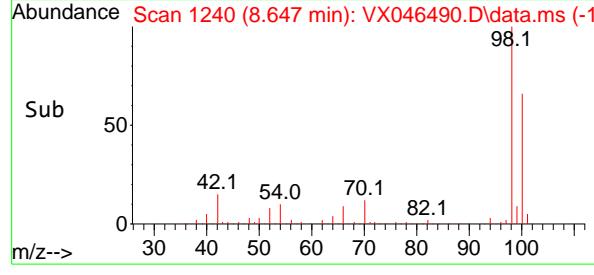

#50  
Toluene-d8  
Concen: 50.393 ug/l  
RT: 8.647 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046490.D  
Acq: 04 Jun 2025 11:04


Instrument : MSVOA\_X  
ClientSampleId : VX0604WBL01


Tgt Ion: 98 Resp: 175770  
Ion Ratio Lower Upper  
98 100  
100 65.3 53.5 80.3

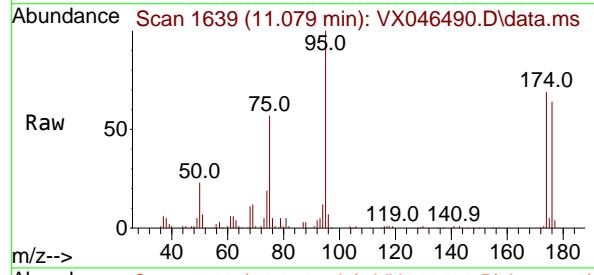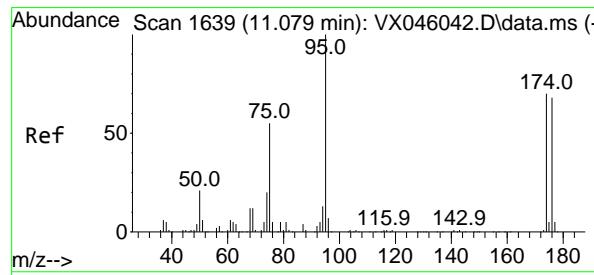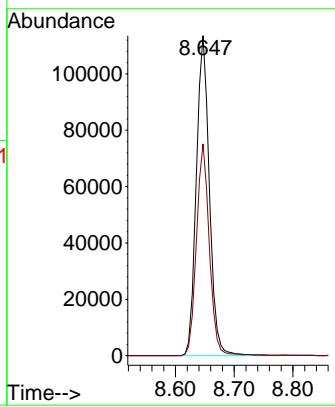

#62  
4-Bromofluorobenzene  
Concen: 53.079 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX046490.D  
Acq: 04 Jun 2025 11:04



Tgt Ion: 95 Resp: 71016  
Ion Ratio Lower Upper  
95 100  
174 67.4 0.0 135.8  
176 65.5 0.0 131.4

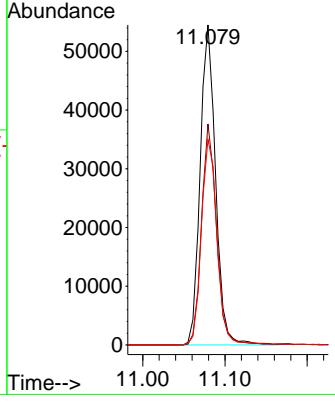

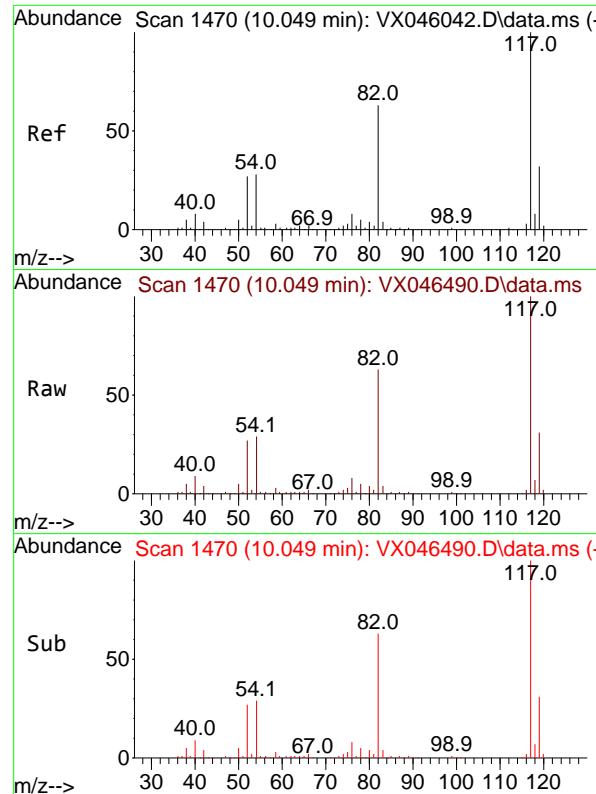


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046490.D  
ClientSampleId : VX0604WBL01  
Acq: 04 Jun 2025 11:04

Tgt Ion:117 Resp: 133992  
Ion Ratio Lower Upper  
117 100  
82 63.0 50.6 76.0  
119 31.0 25.8 38.6

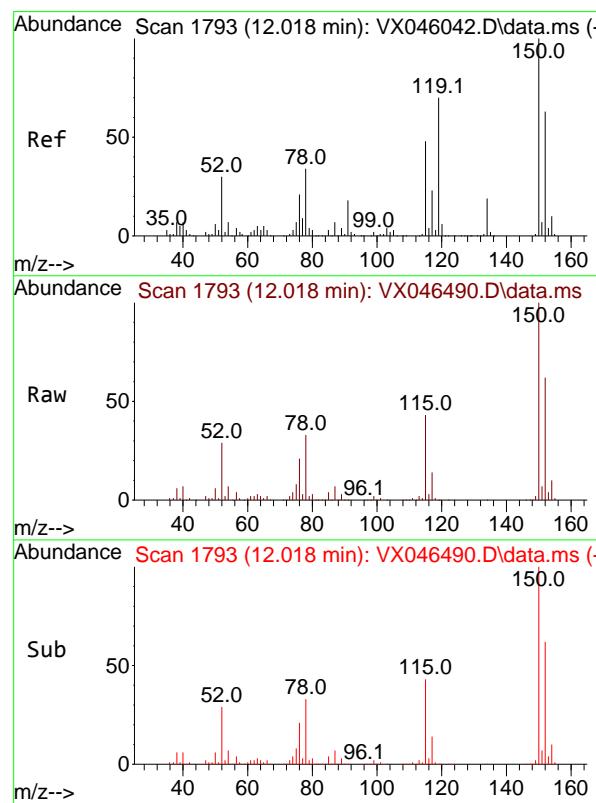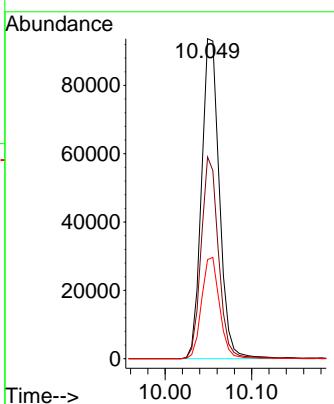

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.018 min Scan# 1793  
Delta R.T. -0.000 min  
Lab File: VX046490.D  
Acq: 04 Jun 2025 11:04

Tgt Ion:152 Resp: 59967  
Ion Ratio Lower Upper  
152 100  
115 66.8 46.9 140.7  
150 160.7 0.0 351.0

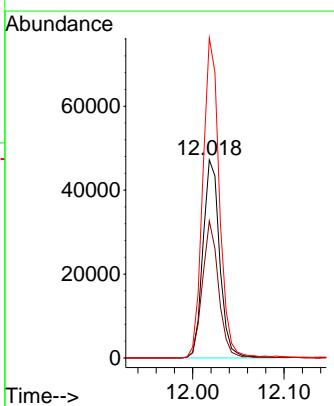



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	
Client Sample ID:	VX0604WBS01			SDG No.:	Q2200
Lab Sample ID:	VX0604WBS01			Matrix:	Water
Analytical Method:	8260D			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046491.D	1		06/04/25 11:27	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	15.5		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	17.2		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	19.6		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	19.6		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	19.4		0.20	1.00	ug/L
71-43-2	Benzene	18.6		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	19.8		0.22	1.00	ug/L
79-01-6	Trichloroethene	18.4		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	20.5		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	19.0		0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	50.1		70 (74) - 130 (125)	100%	SPK: 50
1868-53-7	Dibromofluoromethane	51.3		70 (75) - 130 (124)	103%	SPK: 50
2037-26-5	Toluene-d8	47.3		70 (86) - 130 (113)	95%	SPK: 50
460-00-4	4-Bromofluorobenzene	49.1		70 (77) - 130 (121)	98%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	92900		5.544		
540-36-3	1,4-Difluorobenzene	164000		6.757		
3114-55-4	Chlorobenzene-d5	139000		10.049		
3855-82-1	1,4-Dichlorobenzene-d4	63900		12.018		

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046491.D  
 Acq On : 04 Jun 2025 11:27  
 Operator : JC/MD  
 Sample : VX0604WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBS01

Quant Time: Jun 05 01:39:52 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.544	168	92897	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	164481	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	139452	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	63937	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	86820	50.130	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 100.260%		
35) Dibromofluoromethane	5.379	113	60723	51.267	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 102.540%		
50) Toluene-d8	8.647	98	193713	47.253	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 94.500%		
62) 4-Bromofluorobenzene	11.079	95	77214	49.102	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 98.200%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.167	85	22743	15.995	ug/l	99
3) Chloromethane	1.307	50	20855	15.125	ug/l	98
4) Vinyl Chloride	1.374	62	19920	15.523	ug/l	94
5) Bromomethane	1.599	94	9608	16.142	ug/l	100
6) Chloroethane	1.673	64	11730	17.122	ug/l	96
7) Trichlorofluoromethane	1.880	101	34089	17.974	ug/l	95
8) Diethyl Ether	2.130	74	11717	18.148	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.319	101	21471	18.294	ug/l	99
10) Methyl Iodide	2.447	142	20760	14.948	ug/l	99
11) Tert butyl alcohol	2.971	59	28971	119.170	ug/l	99
12) 1,1-Dichloroethene	2.313	96	18932	17.187	ug/l	97
13) Acrolein	2.233	56	29271	105.725	ug/l	98
14) Allyl chloride	2.660	41	40362	19.172	ug/l	96
15) Acrylonitrile	3.063	53	74090	106.582	ug/l	98
16) Acetone	2.380	43	73753	106.210	ug/l	99
17) Carbon Disulfide	2.508	76	33026	12.646	ug/l	# 95
18) Methyl Acetate	2.703	43	44506	27.620	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	79431	20.568	ug/l	99
20) Methylene Chloride	2.782	84	23740	17.840	ug/l	91
21) trans-1,2-Dichloroethene	3.087	96	19363	17.479	ug/l	95
22) Diisopropyl ether	3.758	45	83789	20.604	ug/l	90
23) Vinyl Acetate	3.721	43	346082	96.761	ug/l	99
24) 1,1-Dichloroethane	3.605	63	44360	19.585	ug/l	99
25) 2-Butanone	4.556	43	111365	110.466	ug/l	97
26) 2,2-Dichloropropane	4.471	77	34526	19.475	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	26144	19.605	ug/l	97
28) Bromochloromethane	4.898	49	23833	21.860	ug/l	97
29) Tetrahydrofuran	5.007	42	69831	110.541	ug/l	99
30) Chloroform	5.093	83	47227	20.005	ug/l	97
31) Cyclohexane	5.465	56	34657	16.791	ug/l	99
32) 1,1,1-Trichloroethane	5.373	97	39783	19.440	ug/l	100
36) 1,1-Dichloropropene	5.690	75	27602	17.344	ug/l	98
37) Ethyl Acetate	4.721	43	39738	20.211	ug/l	99
38) Carbon Tetrachloride	5.672	117	32904	18.402	ug/l	95
39) Methylcyclohexane	7.373	83	33061	16.137	ug/l	98
40) Benzene	6.031	78	86835	18.629	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046491.D  
 Acq On : 04 Jun 2025 11:27  
 Operator : JC/MD  
 Sample : VX0604WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBS01

Quant Time: Jun 05 01:39:52 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.928	41	23318	22.671	ug/1	98
42) 1,2-Dichloroethane	6.086	62	39852	19.809	ug/1	99
43) Isopropyl Acetate	6.342	43	63564	21.191	ug/1	99
44) Trichloroethene	7.123	130	20599	18.361	ug/1	97
45) 1,2-Dichloropropane	7.428	63	22961	19.810	ug/1	96
46) Dibromomethane	7.580	93	17290	18.913	ug/1	98
47) Bromodichloromethane	7.818	83	35372	19.645	ug/1	99
48) Methyl methacrylate	7.696	41	32412	21.158	ug/1	98
49) 1,4-Dioxane	7.659	88	13462	462.828	ug/1	98
51) 4-Methyl-2-Pentanone	8.574	43	215594	108.282	ug/1	100
52) Toluene	8.714	92	54715	19.143	ug/1	99
53) t-1,3-Dichloropropene	8.976	75	30645	19.148	ug/1	95
54) cis-1,3-Dichloropropene	8.366	75	34352	19.420	ug/1	97
55) 1,1,2-Trichloroethane	9.147	97	23114	20.509	ug/1	98
56) Ethyl methacrylate	9.116	69	37067	20.636	ug/1	97
57) 1,3-Dichloropropane	9.305	76	39627	19.578	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.238	63	97808	106.806	ug/1	99
59) 2-Hexanone	9.427	43	163451	110.961	ug/1	100
60) Dibromochloromethane	9.519	129	25342	20.474	ug/1	98
61) 1,2-Dibromoethane	9.610	107	23528	20.086	ug/1	100
64) Tetrachloroethene	9.269	164	18715	18.968	ug/1	95
65) Chlorobenzene	10.080	112	59399	19.461	ug/1	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	21063	20.209	ug/1	98
67) Ethyl Benzene	10.189	91	105678	19.642	ug/1	99
68) m/p-Xylenes	10.299	106	78322	39.802	ug/1	99
69) o-Xylene	10.640	106	39544	20.613	ug/1	99
70) Styrene	10.653	104	64399	20.492	ug/1	99
71) Bromoform	10.799	173	15687	20.047	ug/1 #	97
73) Isopropylbenzene	10.957	105	105573	21.209	ug/1	99
74) N-amyl acetate	10.842	43	53645	21.810	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	37218	21.336	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	32568m	21.162	ug/1	
77) Bromobenzene	11.195	156	23492	20.328	ug/1	99
78) n-propylbenzene	11.299	91	117360	20.277	ug/1	98
79) 2-Chlorotoluene	11.360	91	75768	20.296	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	85839	20.642	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	9522	20.143	ug/1	99
82) 4-Chlorotoluene	11.451	91	83569	20.186	ug/1	98
83) tert-Butylbenzene	11.713	119	87673	20.930	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	86879	20.630	ug/1	100
85) sec-Butylbenzene	11.890	105	108045	21.008	ug/1	100
86) p-Isopropyltoluene	12.006	119	87255	20.553	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	42116	19.969	ug/1	98
88) 1,4-Dichlorobenzene	12.037	146	44193	20.518	ug/1	98
89) n-Butylbenzene	12.329	91	75030	20.149	ug/1	99
90) Hexachloroethane	12.536	117	14661	19.602	ug/1	96
91) 1,2-Dichlorobenzene	12.329	146	44415	20.986	ug/1	98
92) 1,2-Dibromo-3-Chloropr...	12.939	75	9196	23.797	ug/1	98
93) 1,2,4-Trichlorobenzene	13.585	180	25497	20.975	ug/1	97
94) Hexachlorobutadiene	13.719	225	10415	19.618	ug/1	96
95) Naphthalene	13.774	128	94780	21.259	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	25741	20.522	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046491.D  
 Acq On : 04 Jun 2025 11:27  
 Operator : JC/MD  
 Sample : VX0604WBS01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBS01

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Quant Time: Jun 05 01:39:52 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
Data File : VX046491.D  
Acq On : 04 Jun 2025 11:27  
Operator : JC/MD  
Sample : VX0604WBS01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VX0604WBS01

## Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

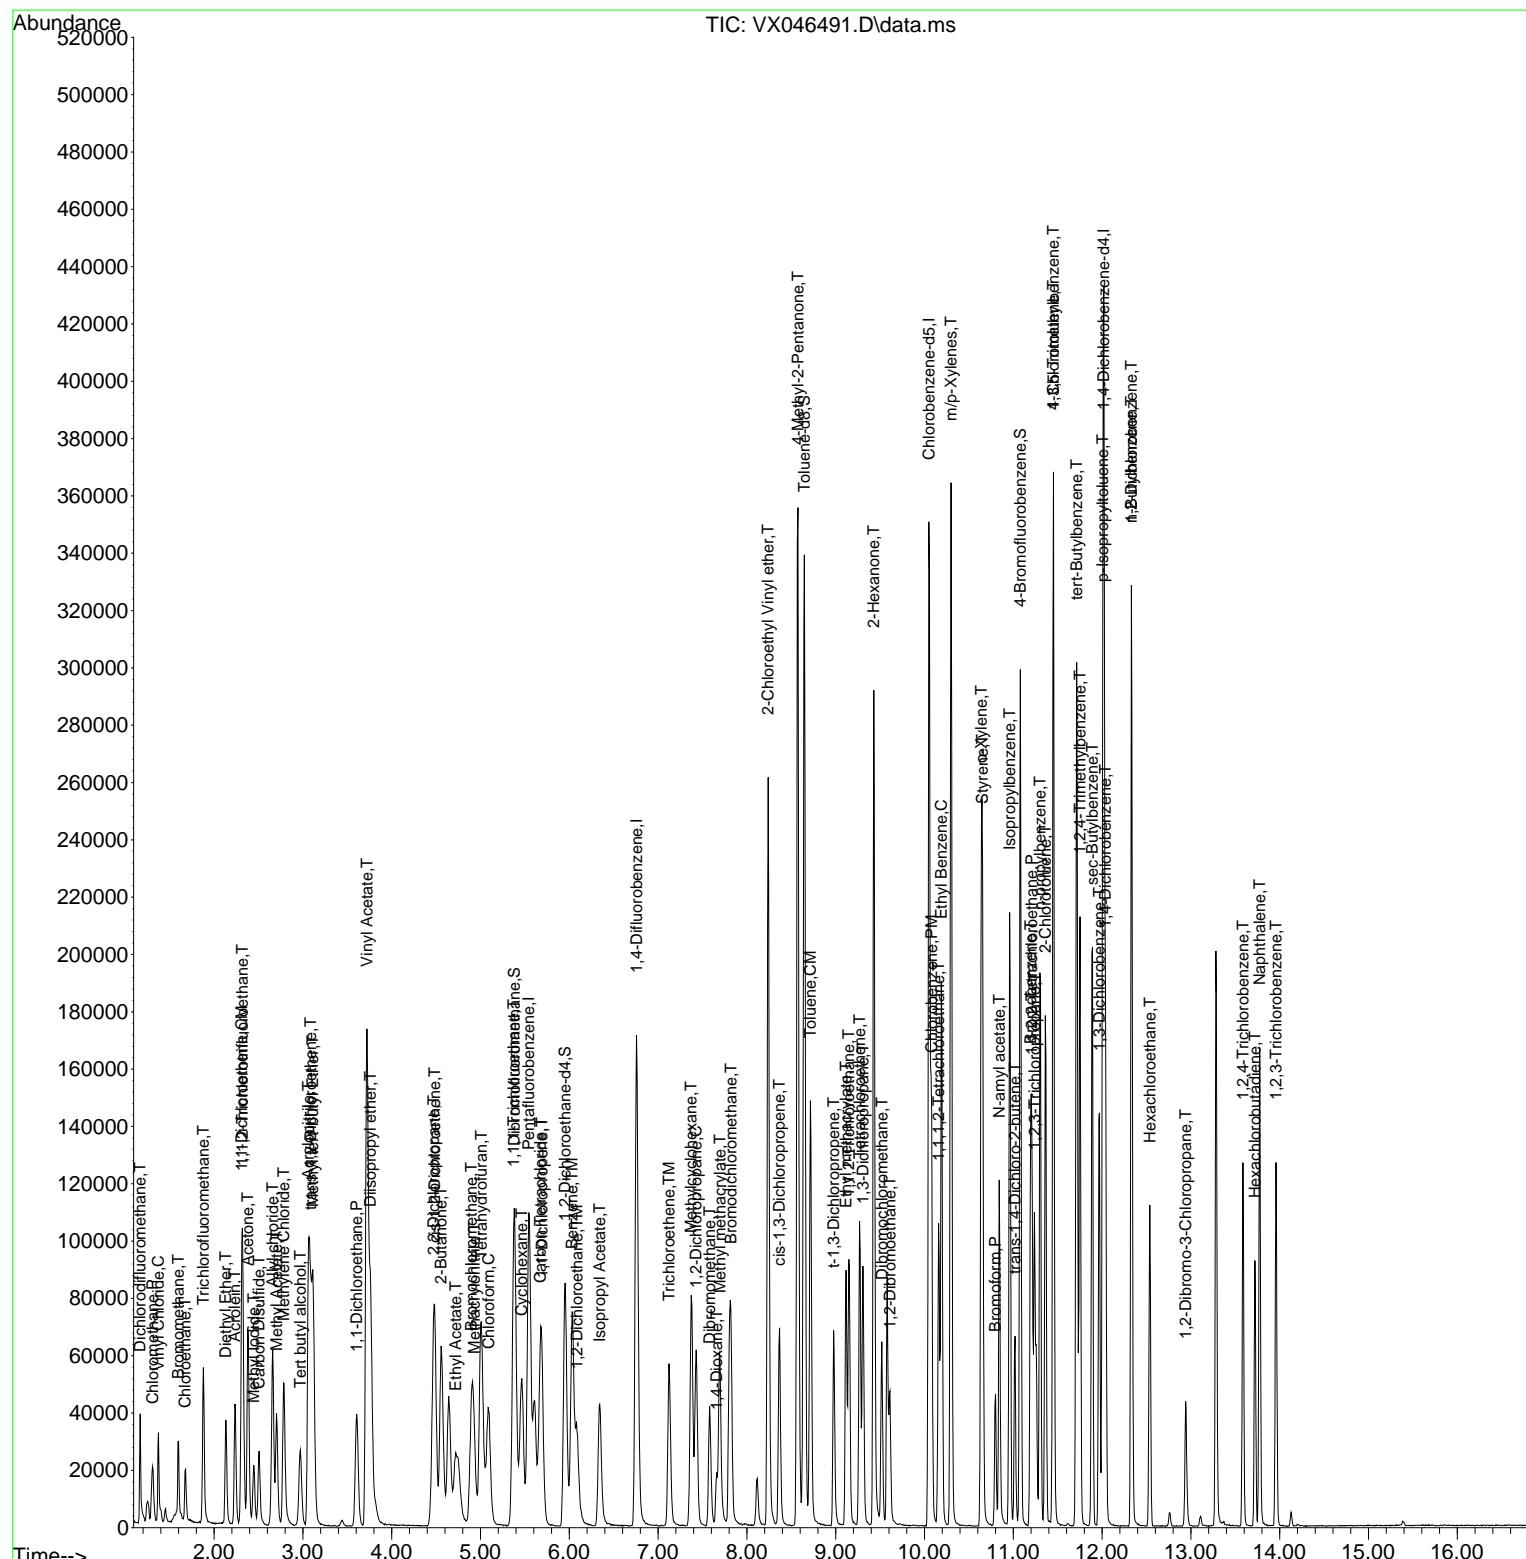





#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.544 min Scan# 71  
 Delta R.T. -0.000 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
 ClientSampleId : VX0604WBS01




Manual Integrations  
APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

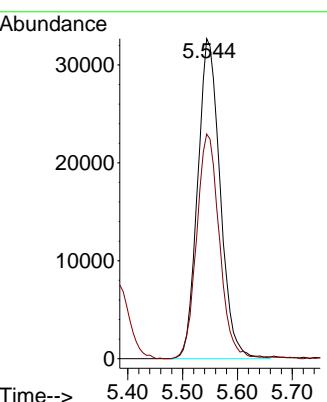


#2  
 Dichlorodifluoromethane  
 Concen: 15.995 ug/l  
 RT: 1.167 min Scan# 13  
 Delta R.T. 0.000 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Tgt Ion: 85 Resp: 22743  
 Ion Ratio Lower Upper  
 85 100  
 87 31.8 15.7 47.1

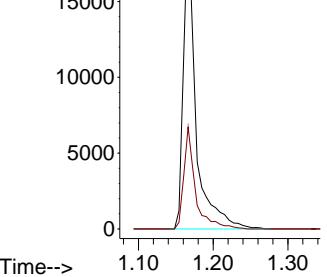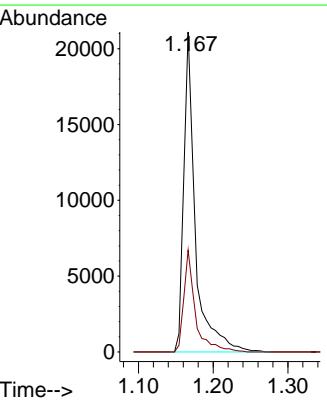



Abundance Scan 36 (1.307 min): VX046491.D\data.ms

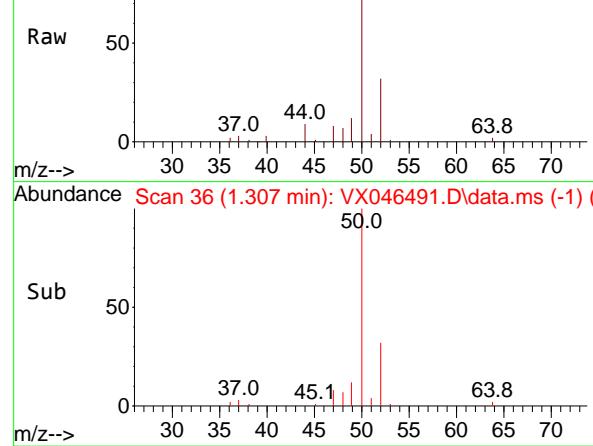

#3

Chloromethane

Concen: 15.125 ug/l

RT: 1.307 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X

ClientSampleId :

VX0604WBS01

Tgt Ion: 50 Resp: 2085

Ion Ratio Lower Upper



50 100

52 32.6 25.4 38.2

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

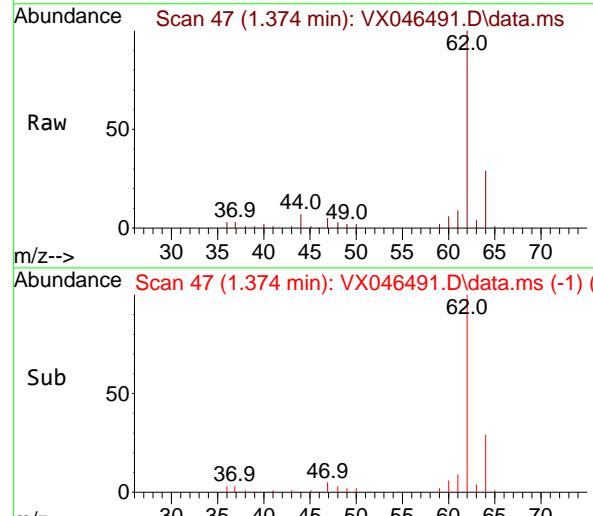
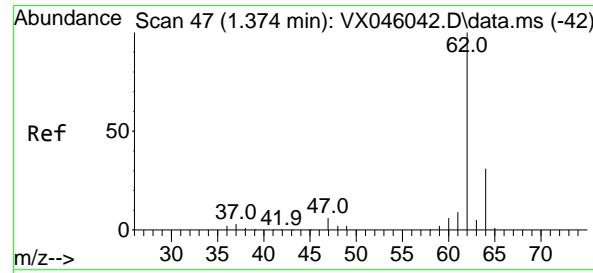
#4  
Vinyl Chloride  
Concen: 15.523 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27




Tgt Ion: 62 Resp: 19920

Ion Ratio Lower Upper

62 100

64 28.0 25.2 37.8

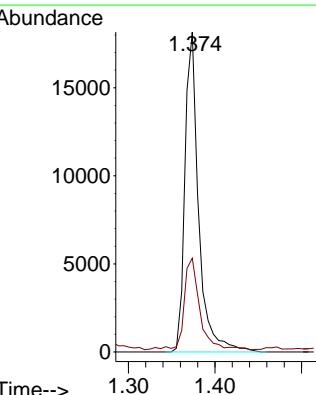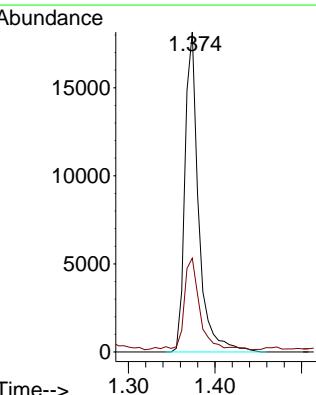







#5  
Bromomethane  
Concen: 16.142 ug/l  
RT: 1.599 min Scan# 8  
Delta R.T. 0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


**Manual Integrations**  
**APPROVED**




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025



#6  
Chloroethane  
Concen: 17.122 ug/l  
RT: 1.673 min Scan# 96  
Delta R.T. 0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 64 Resp: 11730  
Ion Ratio Lower Upper  
64 100  
66 32.8 24.3 36.5



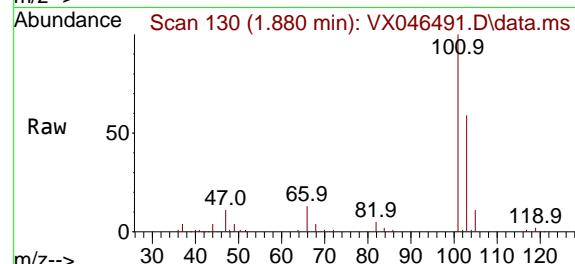





#7

Trichlorofluoromethane  
Concen: 17.974 ug/l  
RT: 1.880 min Scan# 129  
Delta R.T. 0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025



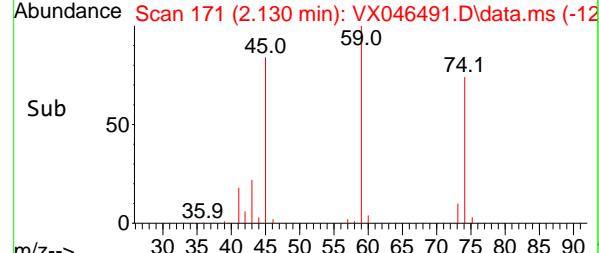
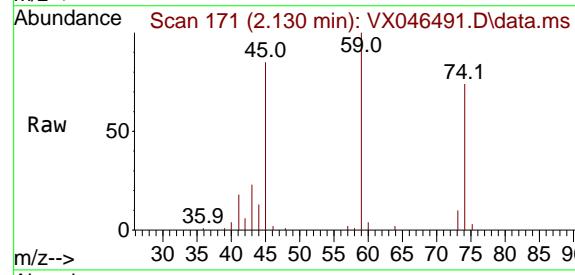
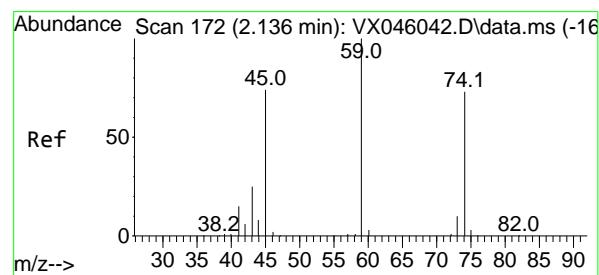



#8

Diethyl Ether  
Concen: 18.148 ug/l  
RT: 2.130 min Scan# 171  
Delta R.T. -0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 74 Resp: 11717  
Ion Ratio Lower Upper  
74 100  
45 111.4 54.9 164.8

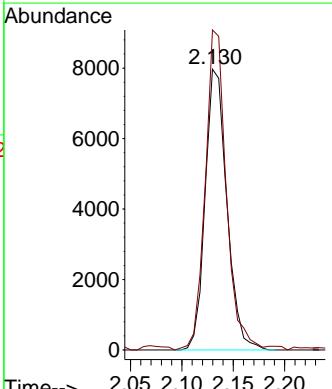

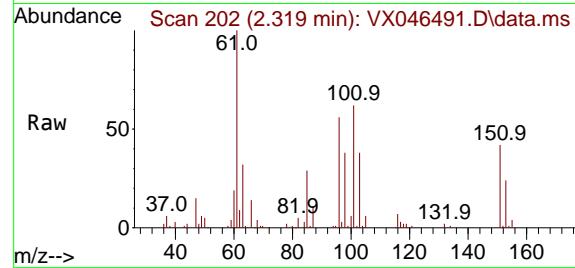

#9

1,1,2-Trichlorotrifluoroethane

Concen: 18.294 ug/l

RT: 2.319 min Scan# 202

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X

ClientSampleId :


VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

Abundance

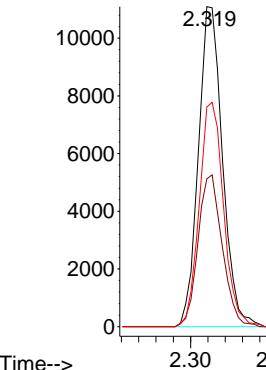

#10

Methyl Iodide

Concen: 14.948 ug/l

RT: 2.447 min Scan# 223

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt Ion:142 Resp: 20760


Ion Ratio Lower Upper




142 100

127 52.6 41.7 62.5

141 14.4 11.5 17.3

Abundance

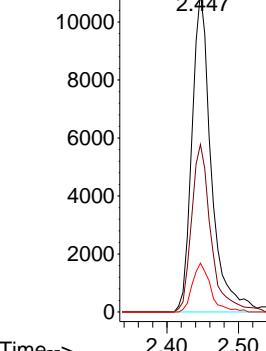







#11

Tert butyl alcohol  
Concen: 119.170 ug/l  
RT: 2.971 min Scan# 3  
Delta R.T. -0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025









#12

1,1-Dichloroethene  
Concen: 17.187 ug/l  
RT: 2.313 min Scan# 201  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 96 Resp: 18932  
Ion Ratio Lower Upper  
96 100  
61 186.8 146.2 219.2  
98 65.7 51.0 76.6

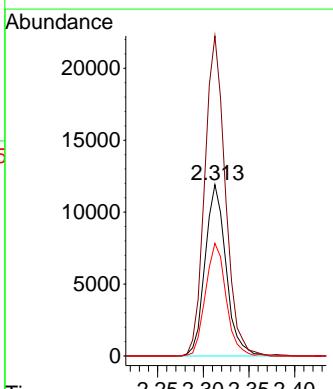

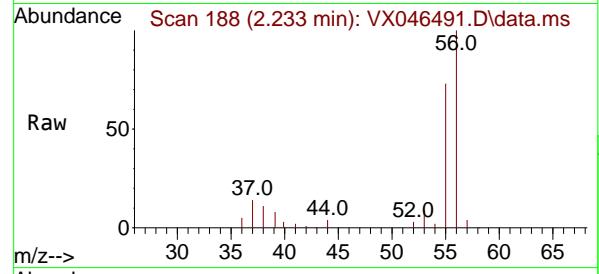


#13

Acrolein  
Concen: 105.725 ug/l  
RT: 2.233 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0604WBS01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025









#14

Allyl chloride  
Concen: 19.172 ug/l  
RT: 2.660 min Scan# 258  
Delta R.T. 0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 41 Resp: 40362  
Ion Ratio Lower Upper  
41 100  
39 72.5 60.6 90.8  
76 28.6 24.9 37.3



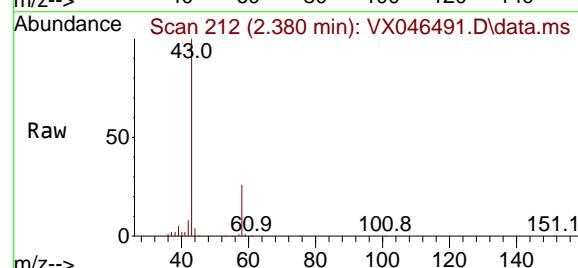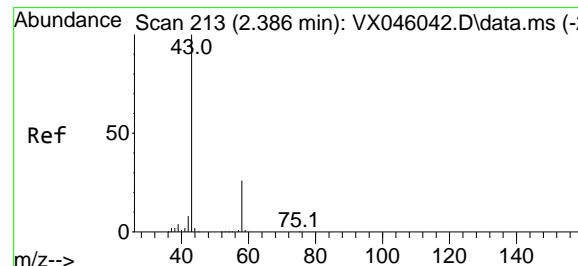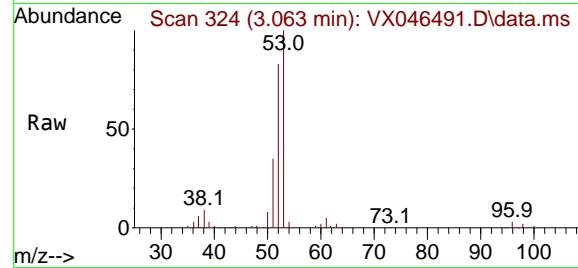

#15

Acrylonitrile

Concen: 106.582 ug/l

RT: 3.063 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBS01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025


Supervised By :Semsettin Yesilyurt 06/05/2025

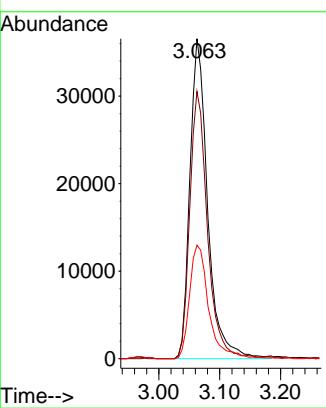




#16  
Acetone  
Concen: 106.210 ug/l  
RT: 2.380 min Scan# 212  
Delta R.T. -0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 43 Resp: 73753  
Ion Ratio Lower Upper  
43 100  
58 26.2 21.2 31.8

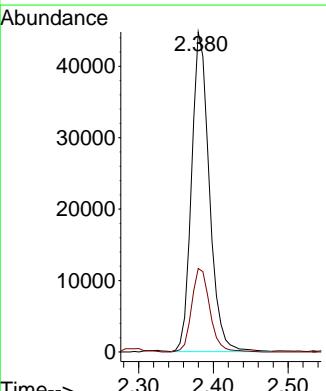



Abundance Scan 233 (2.508 min): VX046491.D\data.ms

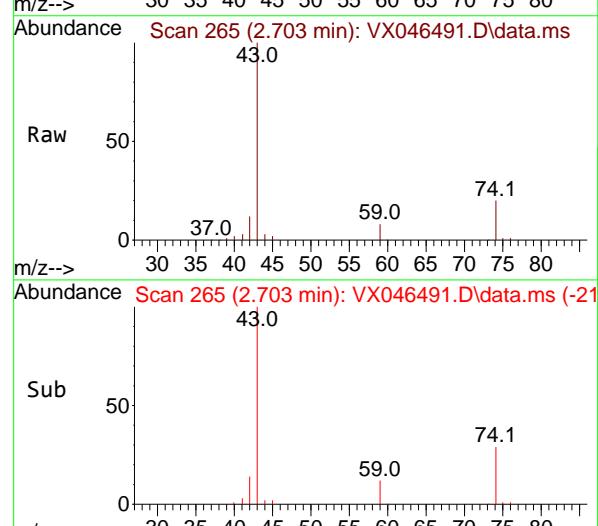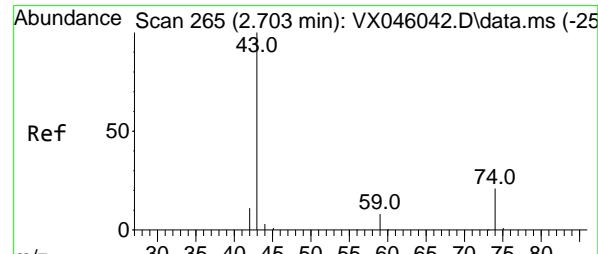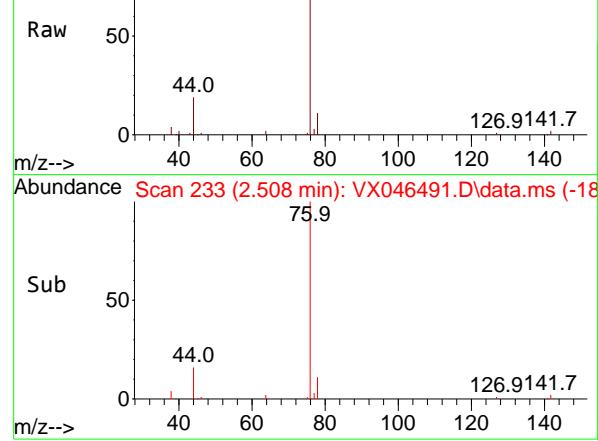


Abundance Scan 265 (2.703 min): VX046491.D\data.ms (-21)

#17  
 Carbon Disulfide  
 Concen: 12.646 ug/l  
 RT: 2.508 min Scan# 21  
 Delta R.T. 0.006 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
 ClientSampleId : VX0604WBS01


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025



#18  
 Methyl Acetate  
 Concen: 27.620 ug/l  
 RT: 2.703 min Scan# 265  
 Delta R.T. 0.000 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Tgt Ion: 43 Resp: 44506  
 Ion Ratio Lower Upper  
 43 100  
 74 21.2 16.7 25.1

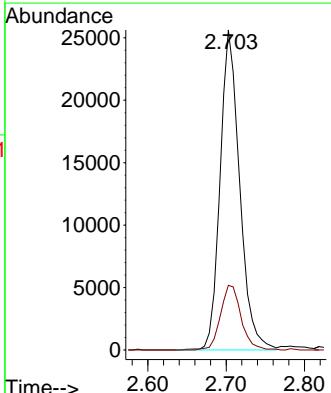







#19

Methyl tert-butyl Ether  
Concen: 20.568 ug/l  
RT: 3.111 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025




#20



Methylene Chloride  
Concen: 17.840 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 84 Resp: 23740  
Ion Ratio Lower Upper  
84 100  
49 129.4 113.9 170.9  
51 41.3 33.5 50.3  
86 59.8 53.8 80.8







Abundance Scan 328 (3.087 min): VX046491.D\data.ms

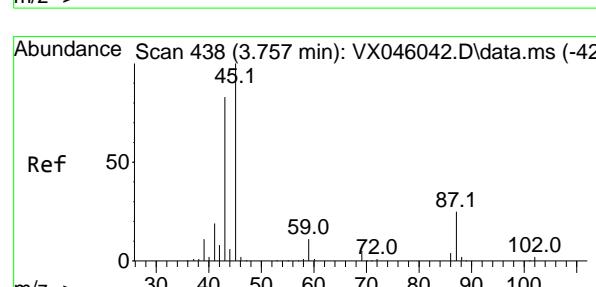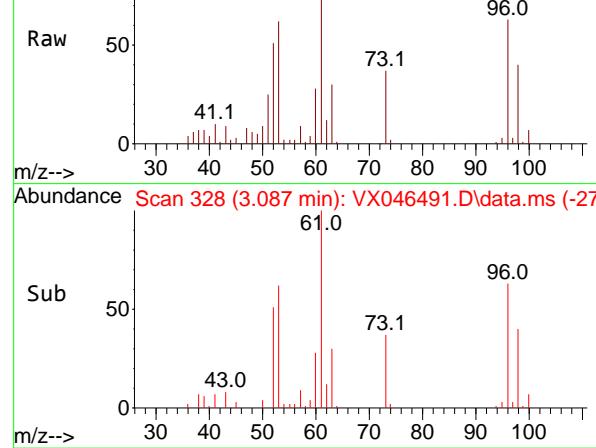

Abundance Scan 438 (3.758 min): VX046491.D\data.ms

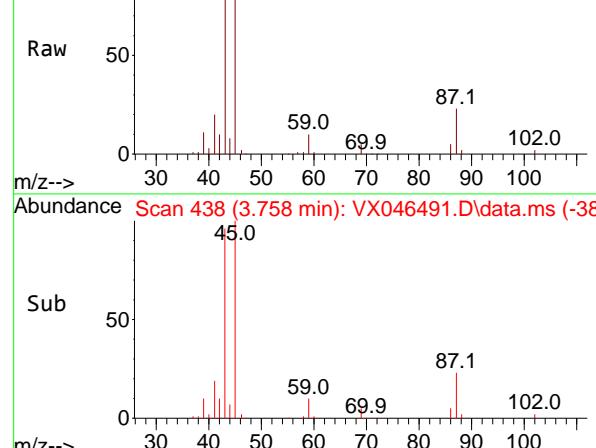

Abundance Scan 438 (3.758 min): VX046491.D\data.ms (-38)

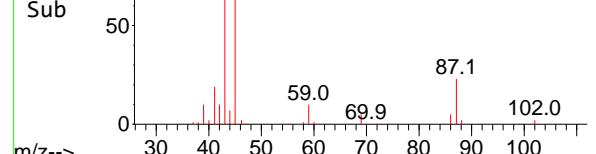

#21

trans-1,2-Dichloroethene

Concen: 17.479 ug/l

RT: 3.087 min Scan# 3

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#22

Diisopropyl ether

Concen: 20.604 ug/l

RT: 3.758 min Scan# 438

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt Ion: 45 Resp: 83789


Ion Ratio Lower Upper


45 100

43 95.4 66.6 100.0



87 23.3 19.8 29.6

59 9.8 8.6 12.8

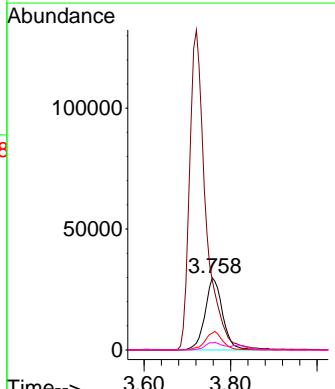




Abundance Scan 432 (3.721 min): VX046491.D\data.ms

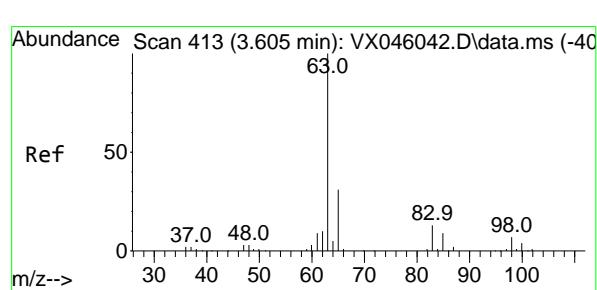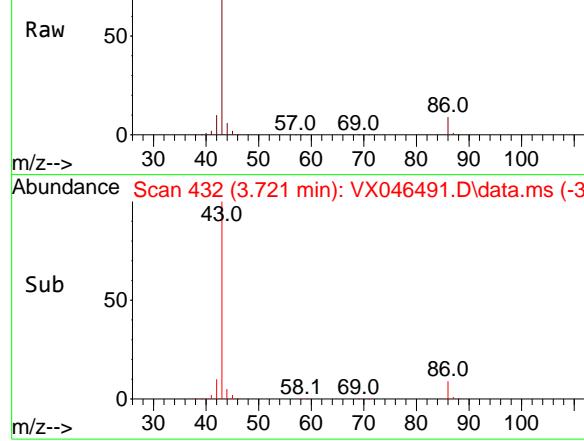

Abundance Scan 413 (3.605 min): VX046491.D\data.ms

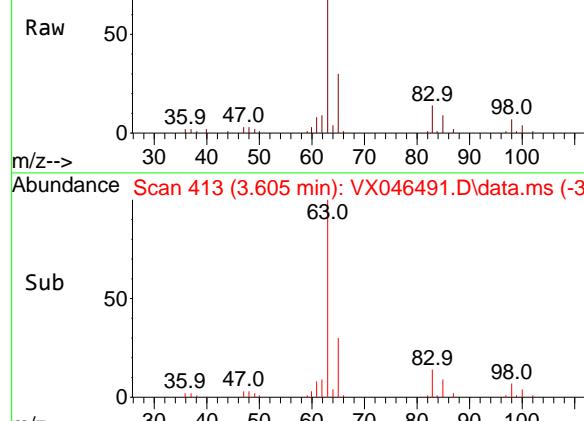

Abundance Scan 413 (3.605 min): VX046491.D\data.ms (-36)

#23

Vinyl Acetate

Concen: 96.761 ug/l

RT: 3.721 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#24

1,1-Dichloroethane

Concen: 19.585 ug/l

RT: 3.605 min Scan# 413

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 63 Resp: 44360


Ion Ratio Lower Upper

63 100



98 6.7 3.6 10.8

100 4.2 2.1 6.3






Abundance Scan 569 (4.556 min): VX046491.D\data.ms

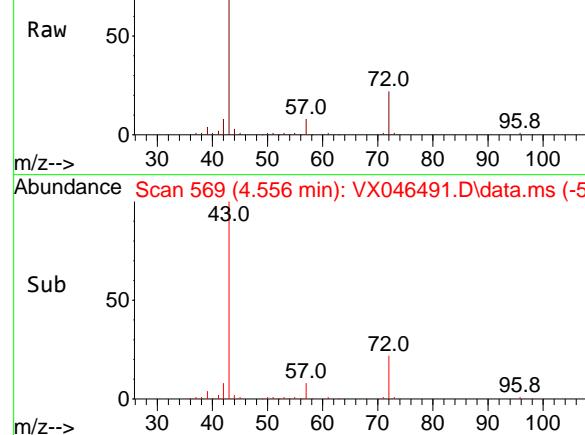

Abundance Scan 555 (4.471 min): VX046491.D\data.ms

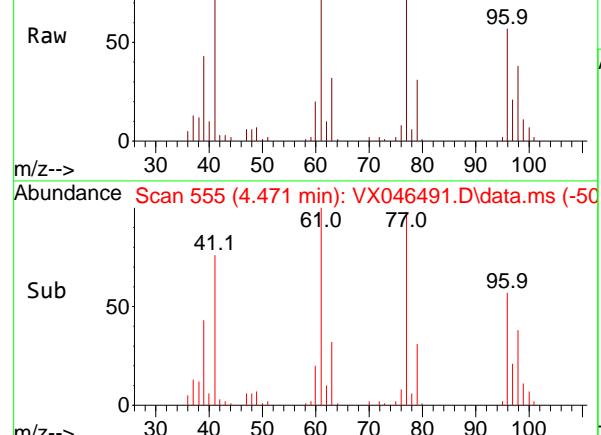

#25

2-Butanone

Concen: 110.466 ug/l

RT: 4.556 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

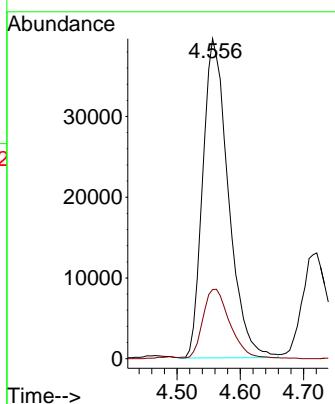

#26

2,2-Dichloropropane

Concen: 19.475 ug/l

RT: 4.471 min Scan# 555

Delta R.T. 0.006 min

Lab File: VX046491.D


Acq: 04 Jun 2025 11:27







Tgt Ion: 77 Resp: 34526

Ion Ratio Lower Upper

77 100

97 21.4 10.5 31.5

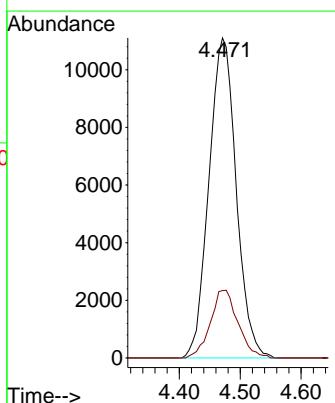

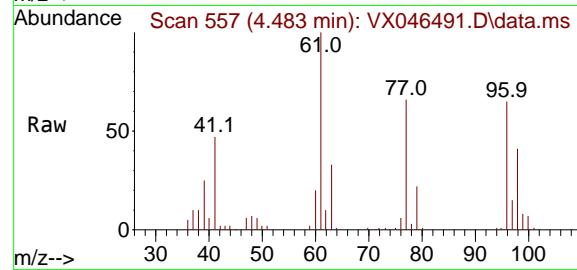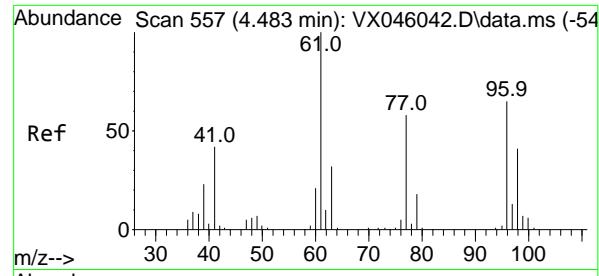


#27  
cis-1,2-Dichloroethene  
Concen: 19.605 ug/l  
RT: 4.483 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025



#28  
Bromochloromethane  
Concen: 21.860 ug/l  
RT: 4.898 min Scan# 625  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 49 Resp: 23833  
Ion Ratio Lower Upper  
49 100  
129 1.6 0.0 4.0  
130 68.0 56.2 84.2



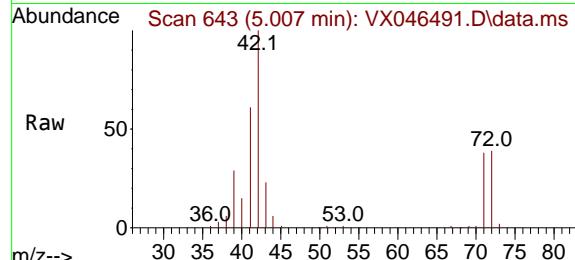

#29

Tetrahydrofuran

Concen: 110.541 ug/l

RT: 5.007 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X




ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**



Reviewed By :Mahesh Dadoda 06/05/2025







Supervised By :Semsettin Yesilyurt 06/05/2025

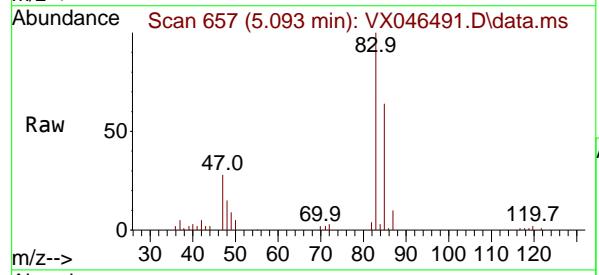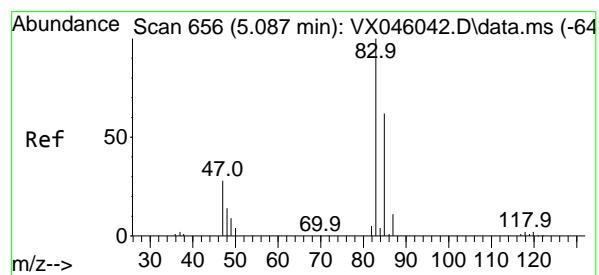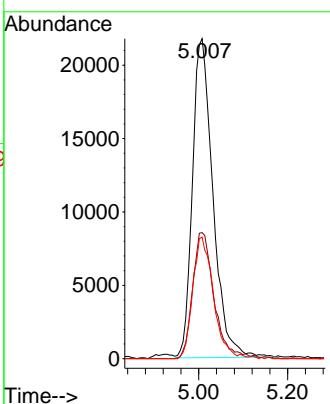

#30  
Chloroform  
Concen: 20.005 ug/l  
RT: 5.093 min Scan# 657  
Delta R.T. 0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 83 Resp: 47227  
Ion Ratio Lower Upper  
83 100  
85 64.1 49.3 73.9

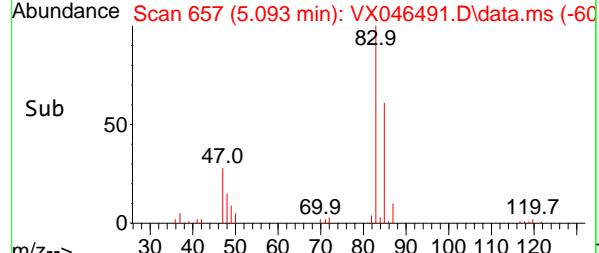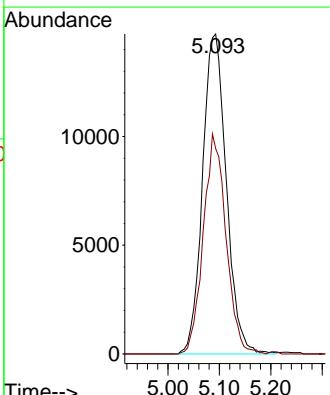

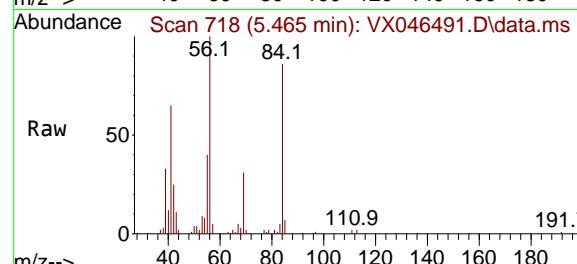

#31

Cyclohexane

Concen: 16.791 ug/l

RT: 5.465 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#32

1,1,1-Trichloroethane

Concen: 19.440 ug/l


RT: 5.373 min Scan# 703







Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt	Ion:	Resp:	
	97	39783	
	100		
97	100		
99	65.2	51.8	77.6
61	50.0	40.1	60.1

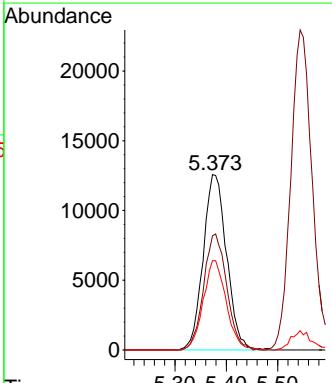



#33

1,2-Dichloroethane-d4

Concen: 50.130 ug/l

RT: 5.952 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**


Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

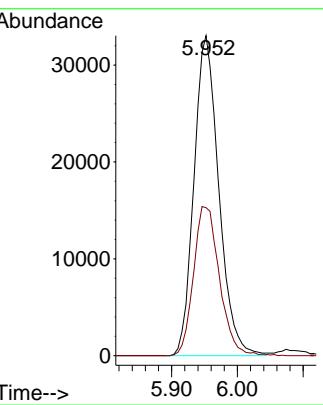

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 930  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion:114 Resp: 164481  
Ion Ratio Lower Upper  
114 100  
63 22.7 0.0 49.2  
88 17.1 0.0 33.6



#35


Dibromofluoromethane  
 Concen: 51.267 ug/l  
 RT: 5.379 min Scan# 704  
 Delta R.T. 0.000 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
 ClientSampleId : VX0604WBS01

Tgt Ion:113 Resp: 6072  
 Ion Ratio Lower Upper  
 113 100  
 111 102.7 83.1 124.7  
 192 16.8 13.3 19.9



### Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

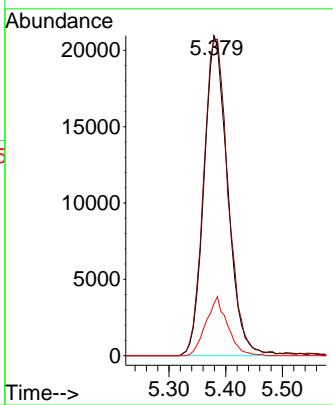

#36  
 1,1-Dichloropropene  
 Concen: 17.344 ug/l  
 RT: 5.690 min Scan# 755  
 Delta R.T. 0.006 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Tgt Ion: 75 Resp: 27602  
 Ion Ratio Lower Upper  
 75 100  
 110 33.2 16.3 48.9  
 77 32.1 24.3 36.5

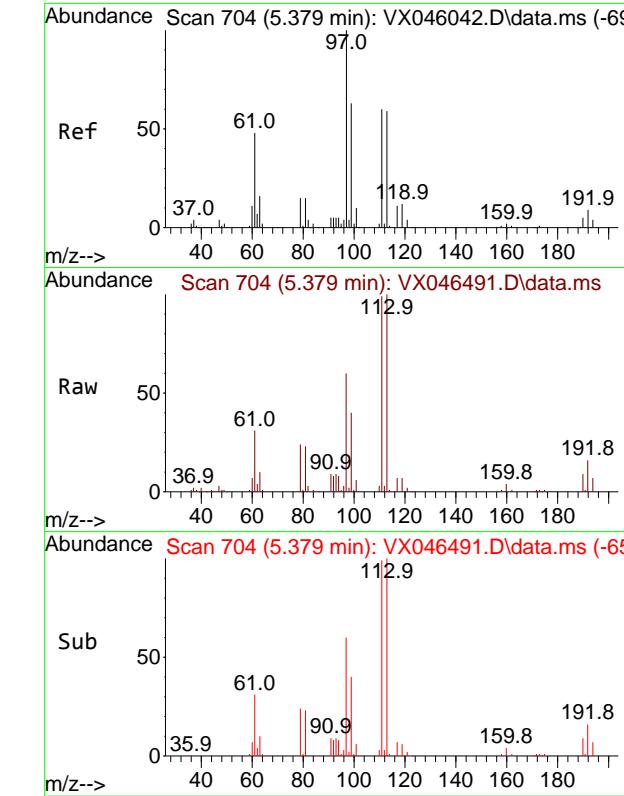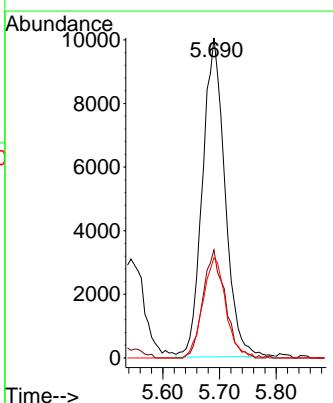

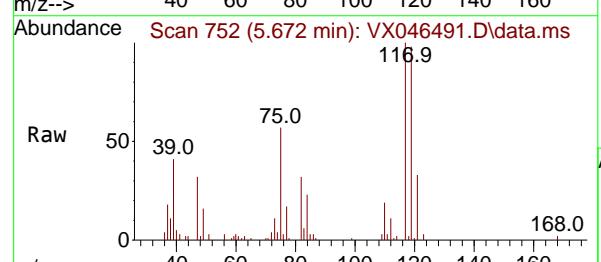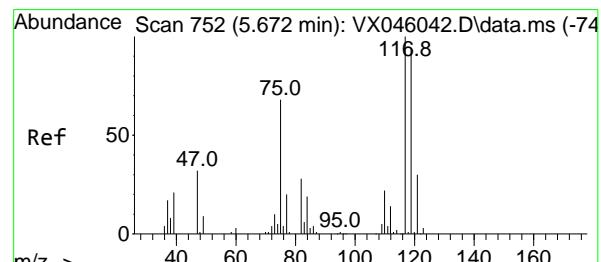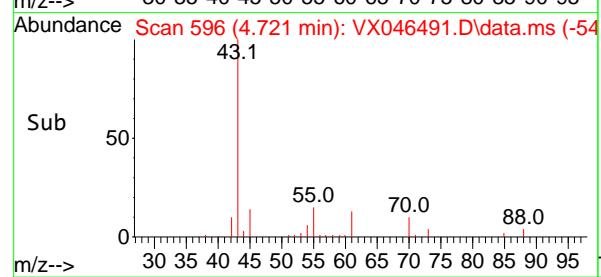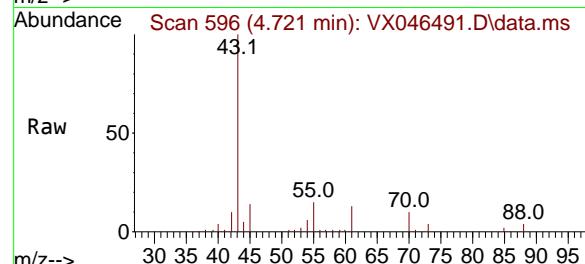

#37

**Ethyl Acetate**

Concen: 20.211 ug/l

RT: 4.721 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#38

**Carbon Tetrachloride**

Concen: 18.402 ug/l


RT: 5.672 min Scan# 752




Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt	Ion:117	Resp:	32904
Ion	Ratio	Lower	Upper
117	100		
119	98.4	75.2	112.8
121	32.9	24.2	36.4

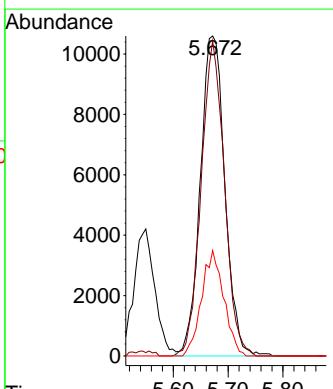



#39

Methylcyclohexane

Concen: 16.137 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#40

Benzene

Concen: 18.629 ug/l

RT: 6.031 min Scan# 811

Delta R.T. 0.000 min

Lab File: VX046491.D



Acq: 04 Jun 2025 11:27







Tgt Ion: 78 Resp: 86835

Ion Ratio Lower Upper

78 100

77 24.0 19.0 28.4

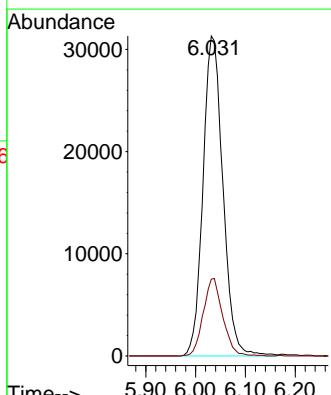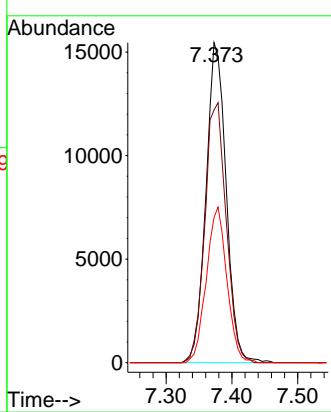



#41

Methacrylonitrile

Concen: 22.671 ug/l

RT: 4.928 min Scan# 6

Delta R.T. 0.012 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X

ClientSampleId :

VX0604WBS01

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

Tgt Ion: 41 Resp: 2331:

Ion Ratio Lower Upper


41 100

39 55.2 47.2 70.8

67 63.8 50.7 76.1

52 29.9 24.6 37.0

Abundance

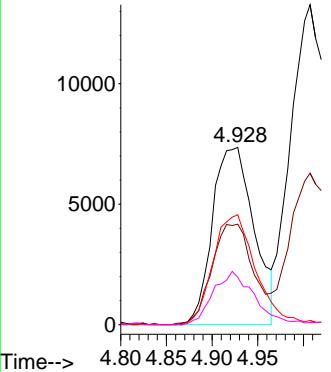

#42

1,2-Dichloroethane

Concen: 19.809 ug/l

RT: 6.086 min Scan# 820

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 62 Resp: 39852


Ion Ratio Lower Upper

62 100

98 7.3 0.0 15.2

Abundance

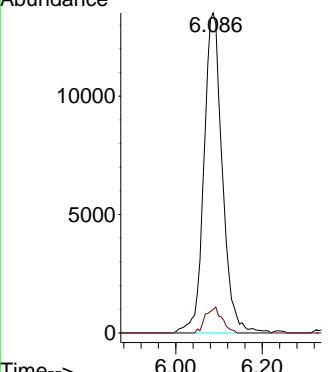



#43

Isopropyl Acetate

Concen: 21.191 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X

ClientSampleId :

VX0604WBS01



Tgt Ion: 43 Resp: 6356

Ion Ratio Lower Upper

43 100




61 17.5 14.3 21.5

87 11.7 9.5 14.3


**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

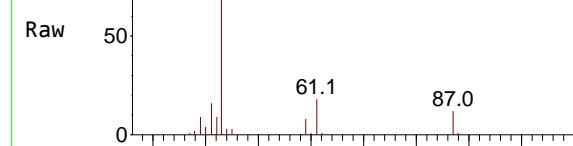



#44  
Trichloroethene  
Concen: 18.361 ug/l  
RT: 7.123 min Scan# 990  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27






Tgt Ion:130 Resp: 20599  
Ion Ratio Lower Upper

130 100

95 98.7 0.0 204.2

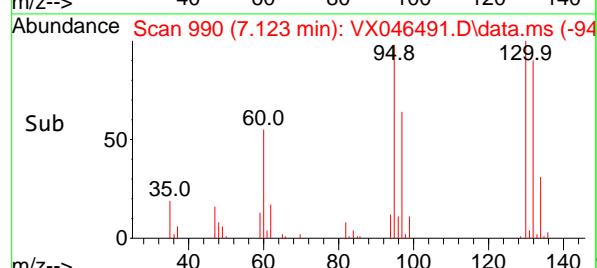



#45

1,2-Dichloropropane

Concen: 19.810 ug/l

RT: 7.428 min Scan# 1040

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27




Instrument : MSVOA\_X

ClientSampleId : VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#46

Dibromomethane

Concen: 18.913 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 93 Resp: 17290




Ion Ratio Lower Upper

93 100

95 84.3 65.6 98.4

174 85.7 68.2 102.2

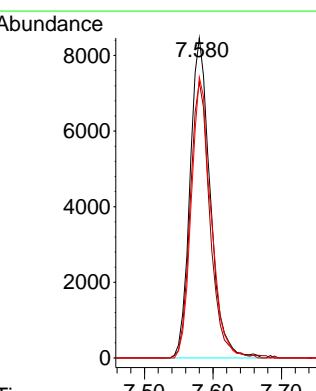

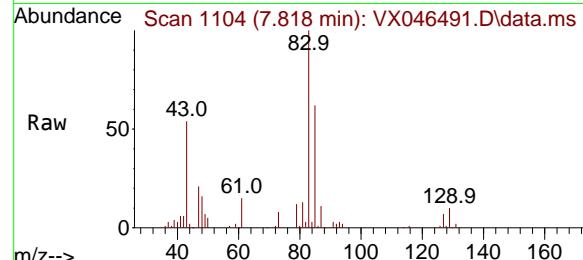

#47

Bromodichloromethane

Concen: 19.645 ug/l

RT: 7.818 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

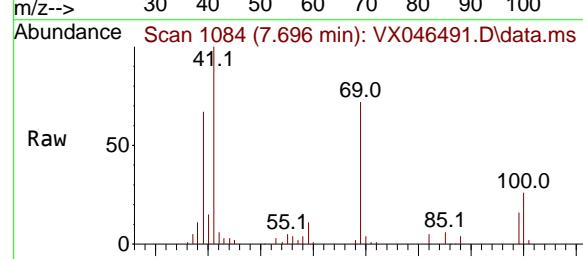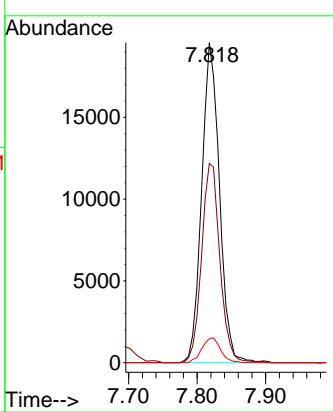

#48

Methyl methacrylate

Concen: 21.158 ug/l

RT: 7.696 min Scan# 1084

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 41 Resp: 32412







Ion Ratio Lower Upper

41 100

69 71.1 58.5 87.7

39 66.4 51.7 77.5





#49

1,4-Dioxane

Concen: 462.828 ug/l

RT: 7.659 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

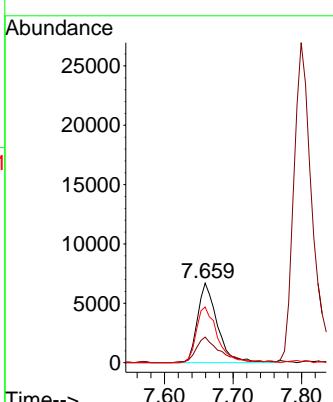

#50

Toluene-d8

Concen: 47.253 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX046491.D


Acq: 04 Jun 2025 11:27


Tgt Ion: 98 Resp: 193713

Ion Ratio Lower Upper



98 100

100 66.1 53.5 80.3






Abundance Scan 1228 (8.574 min): VX046491.D\data.ms

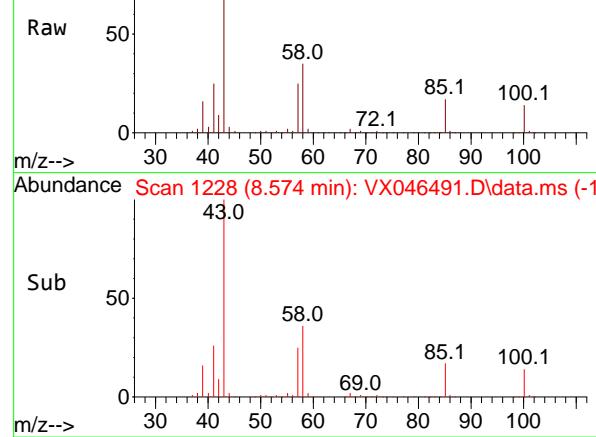

Abundance Scan 1251 (8.714 min): VX046491.D\data.ms

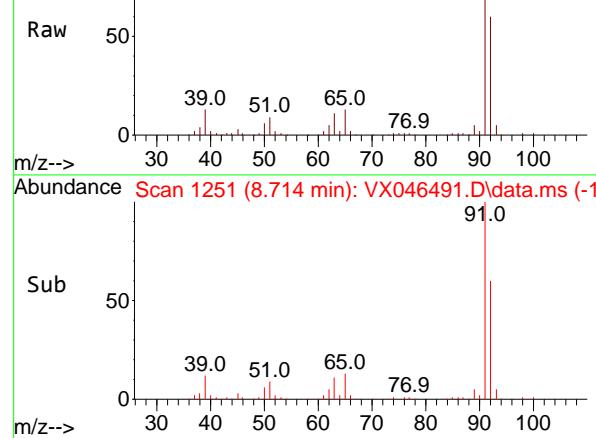

Abundance Scan 1251 (8.714 min): VX046491.D\data.ms

#51

4-Methyl-2-Pentanone

Concen: 108.282 ug/l

RT: 8.574 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#52

Toluene

Concen: 19.143 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. 0.000 min

Lab File: VX046491.D


Acq: 04 Jun 2025 11:27




Tgt Ion: 92 Resp: 54715

Ion Ratio Lower Upper

92 100

91 168.9 136.6 205.0



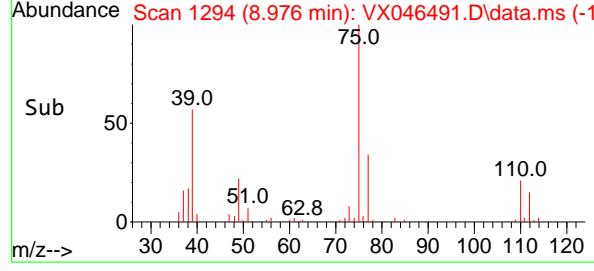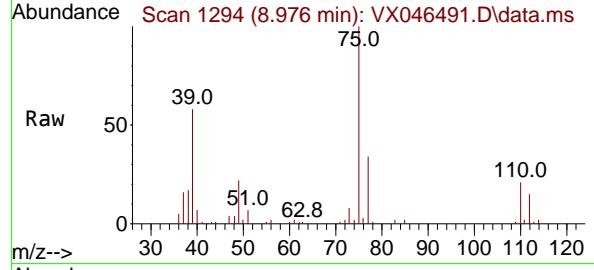

#53

t-1,3-Dichloropropene

Concen: 19.148 ug/l

RT: 8.976 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

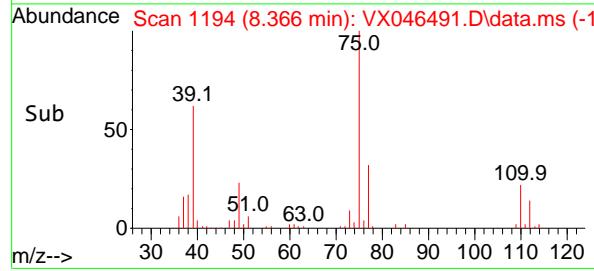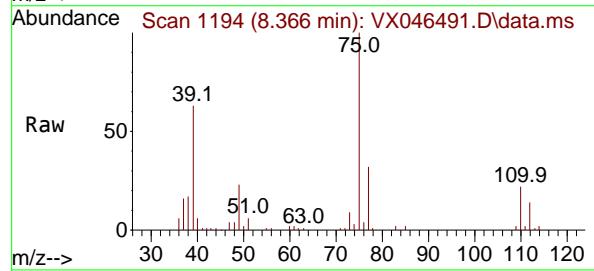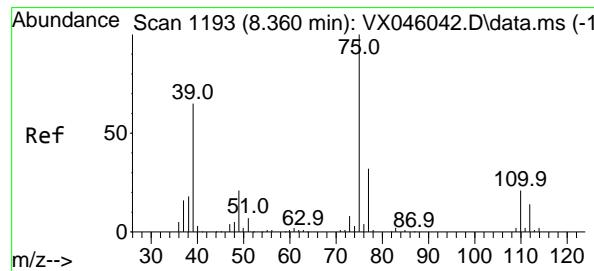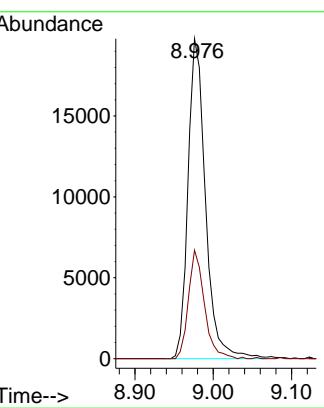

#54

cis-1,3-Dichloropropene

Concen: 19.420 ug/l

RT: 8.366 min Scan# 1194

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 75 Resp: 34352







Ion Ratio Lower Upper

75 100

77 32.4 25.4 38.0

39 62.6 52.2 78.4

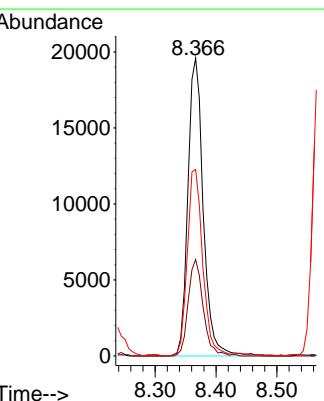

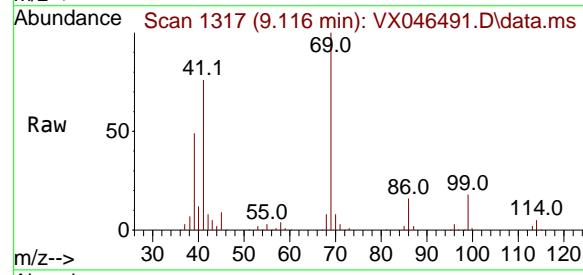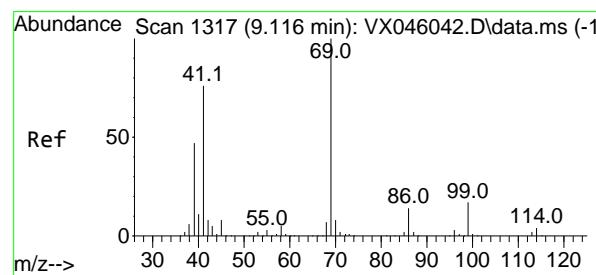

#55

1,1,2-Trichloroethane

Concen: 20.509 ug/l

RT: 9.147 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBS01

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

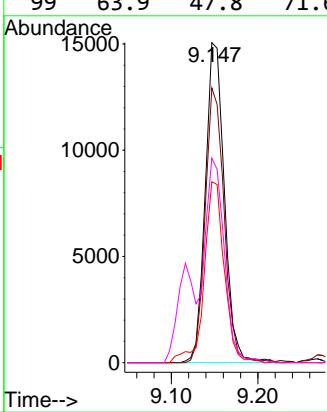

#56

Ethyl methacrylate

Concen: 20.636 ug/l

RT: 9.116 min Scan# 1317

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 69 Resp: 37067




Ion Ratio Lower Upper

69 100

41 79.5 60.8 91.2

39 49.5 39.0 58.6

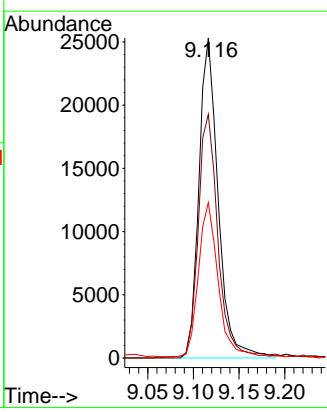

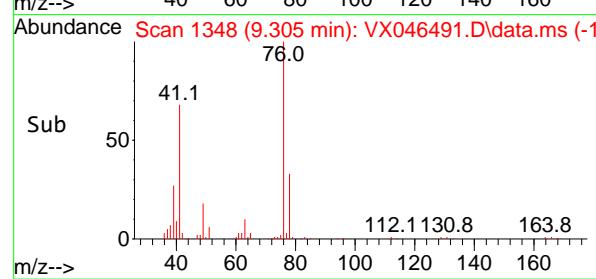

#57

1,3-Dichloropropane

Concen: 19.578 ug/l

RT: 9.305 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#58

2-Chloroethyl Vinyl ether

Concen: 106.806 ug/l

RT: 8.238 min Scan# 1173

Delta R.T. 0.000 min

Lab File: VX046491.D


Acq: 04 Jun 2025 11:27




Tgt Ion: 63 Resp: 97808

Ion Ratio Lower Upper

63 100

106 27.2 21.5 32.3

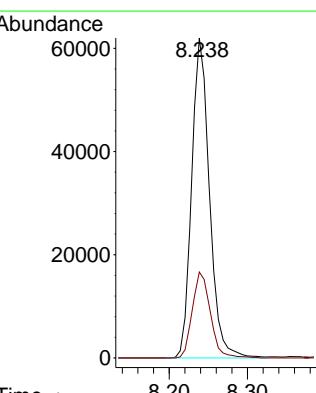







#59  
2-Hexanone  
Concen: 110.961 ug/l  
RT: 9.427 min Scan# 1368  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


**Manual Integrations**  
**APPROVED**




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025



#60  
Dibromochloromethane  
Concen: 20.474 ug/l  
RT: 9.519 min Scan# 1383  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion:129 Resp: 25342  
Ion Ratio Lower Upper  
129 100  
127 76.9 39.3 117.8

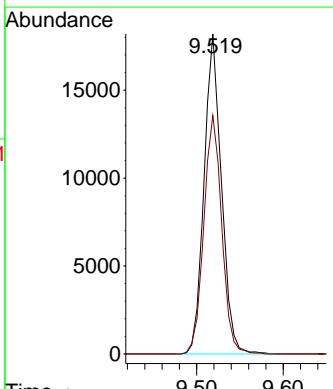

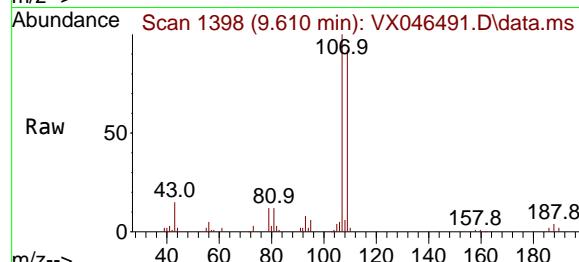

#61

1,2-Dibromoethane

Concen: 20.086 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

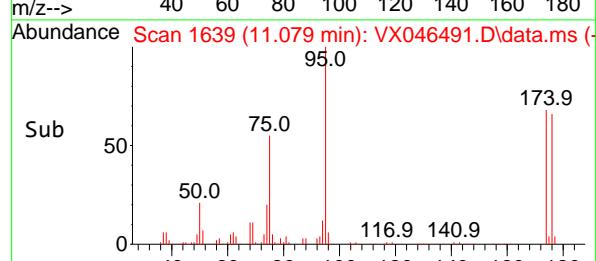

#62

4-Bromofluorobenzene

Concen: 49.102 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 95 Resp: 77214


Ion Ratio Lower Upper

95 100

174 67.0 0.0 135.8

176 64.9 0.0 131.4




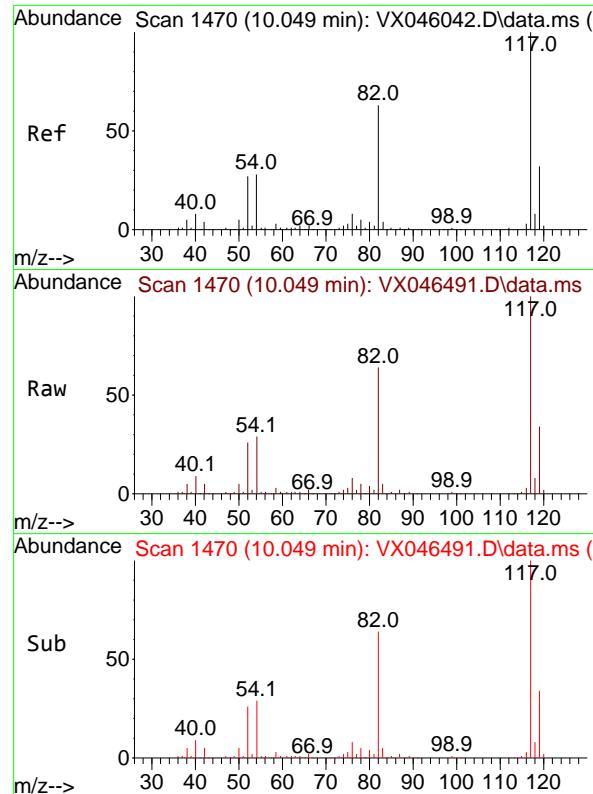


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.049 min Scan# 1470  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


**Manual Integrations**  
**APPROVED**


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

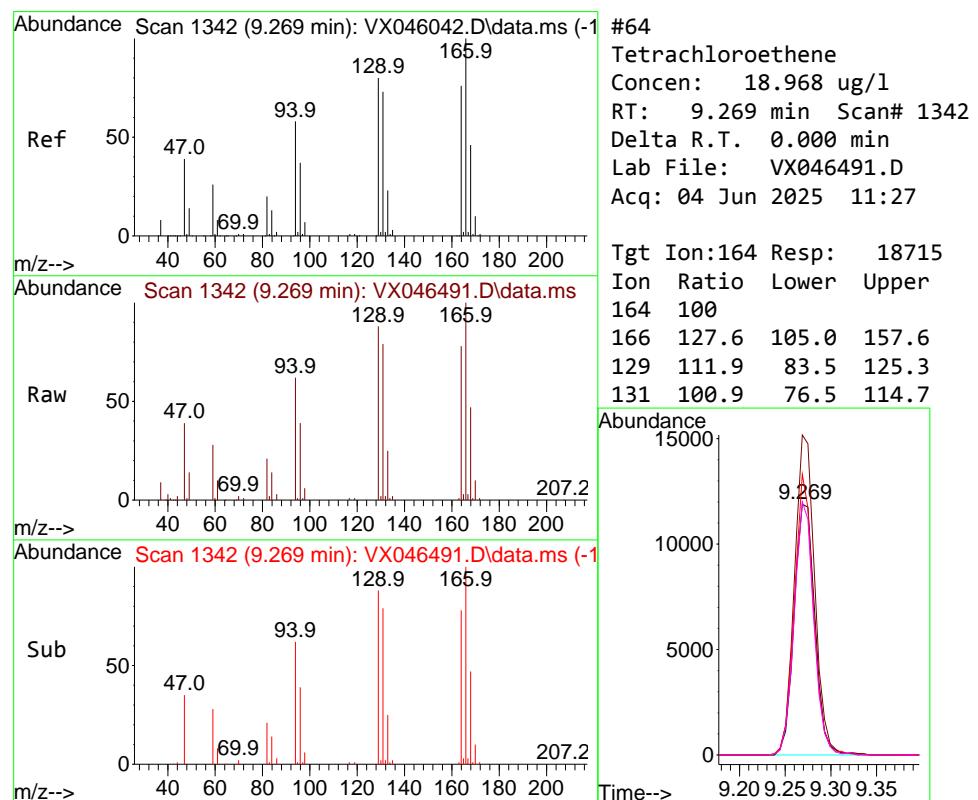

#64  
Tetrachloroethene  
Concen: 18.968 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion:164 Resp: 18715  
Ion Ratio Lower Upper  
164 100  
166 127.6 105.0 157.6  
129 111.9 83.5 125.3  
131 100.9 76.5 114.7




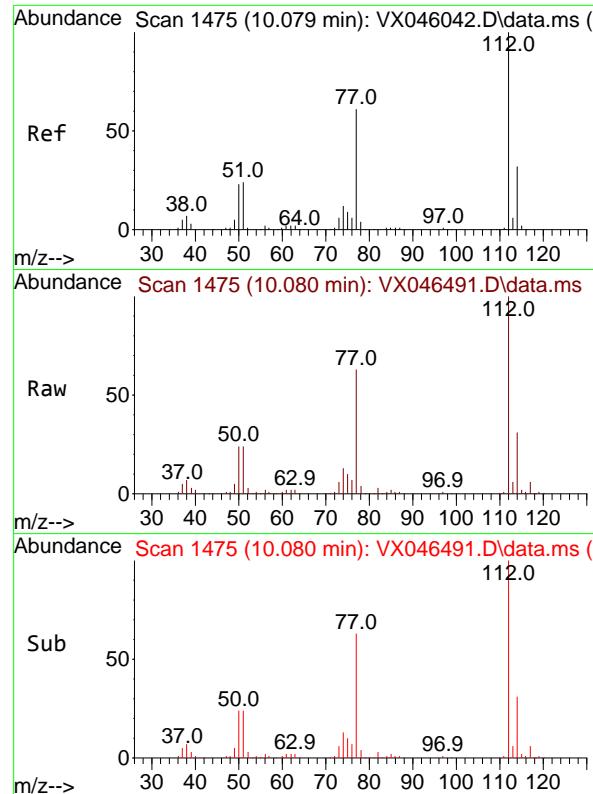


#65  
Chlorobenzene  
Concen: 19.461 ug/l  
RT: 10.080 min Scan# 1475  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

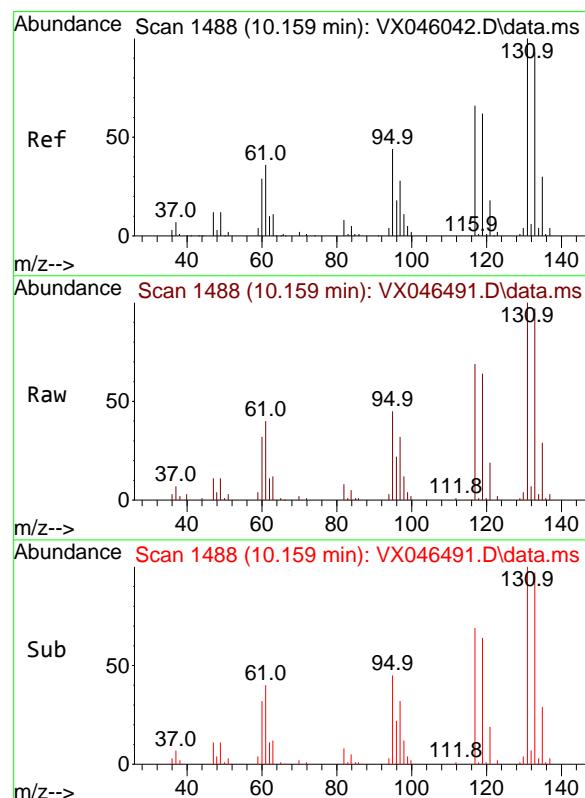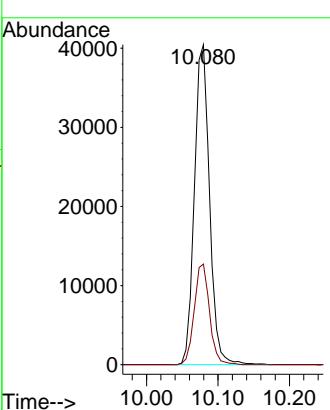

#66  
1,1,1,2-Tetrachloroethane  
Concen: 20.209 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion:131 Resp: 21063  
Ion Ratio Lower Upper  
131 100  
133 96.8 47.3 141.9  
119 64.7 31.6 95.0

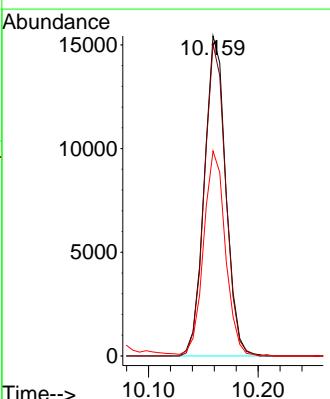



#67

Ethyl Benzene

Concen: 19.642 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27




Instrument : MSVOA\_X

ClientSampleId : VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#68

m/p-Xylenes


Concen: 39.802 ug/l




RT: 10.299 min Scan# 1511

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

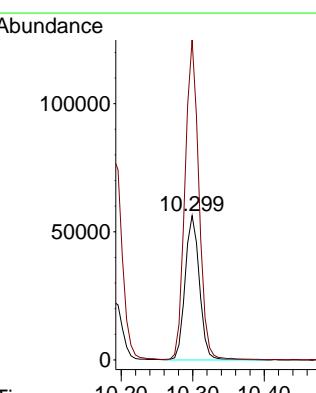Tgt Ion:106 Resp: 78322  
Ion Ratio Lower Upper  
106 100  
91 215.1 171.2 256.8





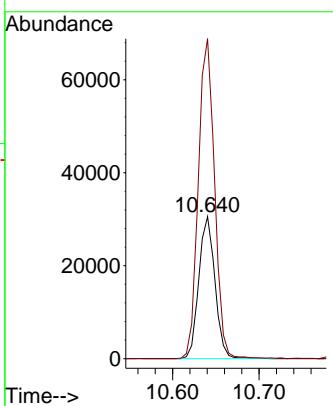


#69  
o-Xylene  
Concen: 20.613 ug/l  
RT: 10.640 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


1 Manual Integrations  
2 APPROVED




3 Reviewed By :Mahesh Dadoda 06/05/2025  
4 Supervised By :Semsettin Yesilyurt 06/05/2025



#70  
Styrene  
Concen: 20.492 ug/l  
RT: 10.653 min Scan# 1569  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion:104 Resp: 64399  
Ion Ratio Lower Upper  
104 100  
78 58.2 45.7 68.5  
103 55.0 43.7 65.5

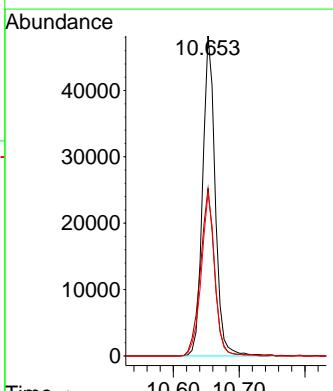



#71

Bromoform

Concen: 20.047 ug/l

RT: 10.799 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion:152 Resp: 63937


Ion Ratio Lower Upper

152 100

115 77.5 46.9 140.7

150 167.6 0.0 351.0

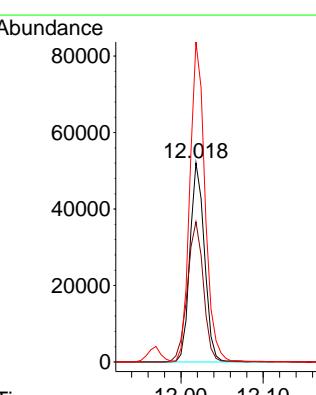

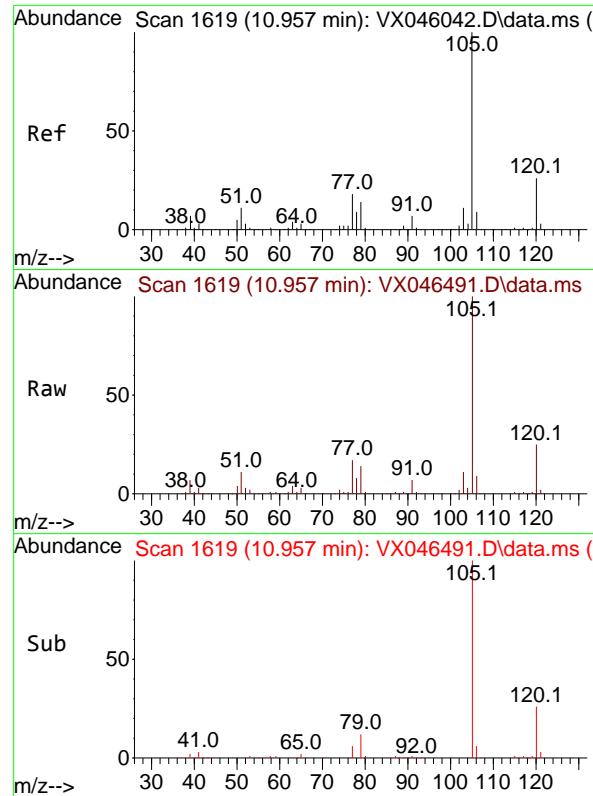

#73

Isopropylbenzene

Concen: 21.209 ug/l

RT: 10.957 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument :

MSVOA\_X



ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

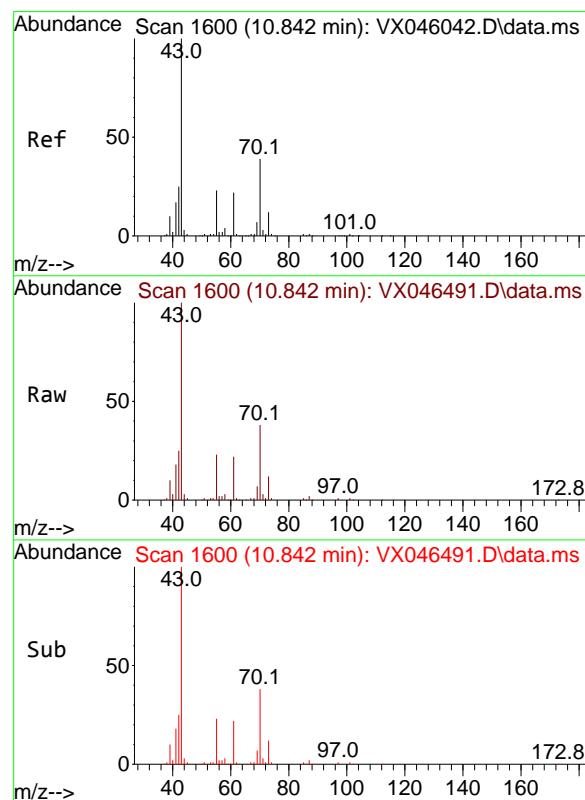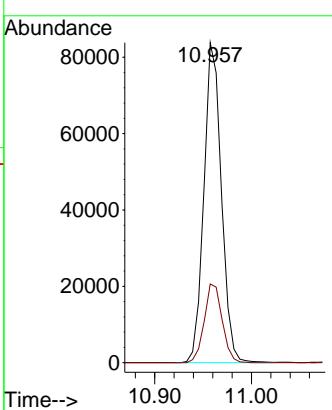

#74

N-amyl acetate

Concen: 21.810 ug/l


RT: 10.842 min Scan# 1600

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt	Ion:	43	Resp:	53645
Ion	Ratio	Lower	Upper	
43	100			
70	37.4	30.9	46.3	
55	22.5	18.7	28.1	
61	21.5	17.1	25.7	




#75  
 1,1,2,2-Tetrachloroethane  
 Concen: 21.336 ug/l  
 RT: 11.207 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
 ClientSampleId : VX0604WBS01

Tgt Ion: 83 Resp: 3721:  
 Ion Ratio Lower Upper  
 83 100  
 131 10.1 5.0 14.9  
 85 64.6 31.9 95.7


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

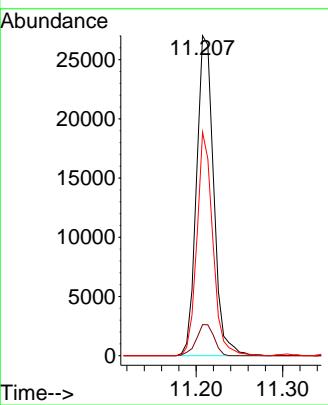

#76  
 1,2,3-Trichloropropane  
 Concen: 21.162 ug/l  
 RT: 11.238 min Scan# 1665  
 Delta R.T. 0.000 min  
 Lab File: VX046491.D  
 Acq: 04 Jun 2025 11:27

Tgt Ion: 75 Resp: 32568  
 Ion Ratio Lower Upper  
 75 100  
 77 39.7 20.5 61.5

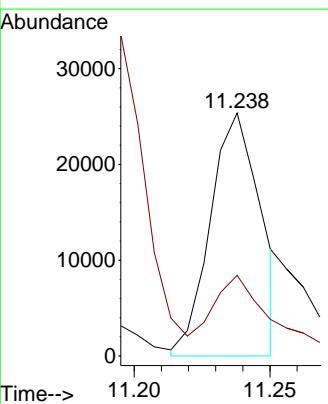

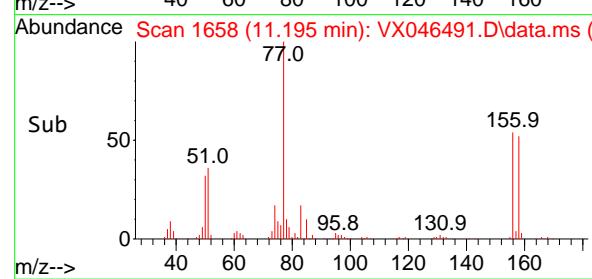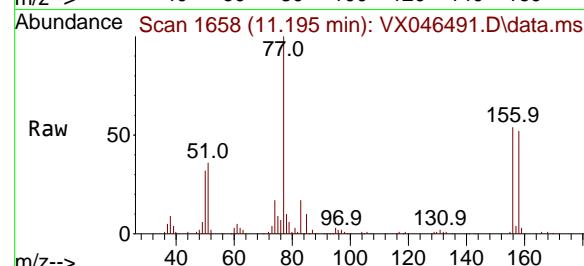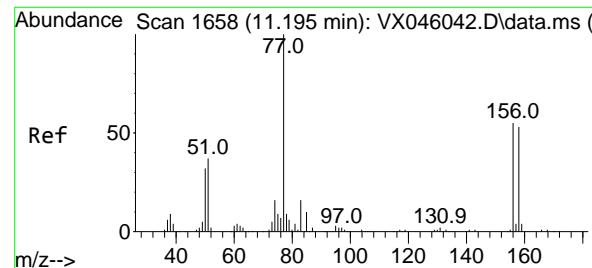

#77

Bromobenzene

Concen: 20.328 ug/l

RT: 11.195 min Scan# 1658

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27





Instrument : MSVOA\_X

ClientSampleId : VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

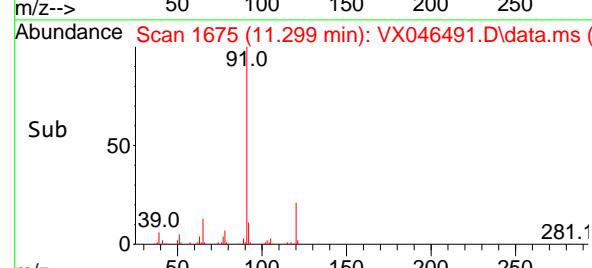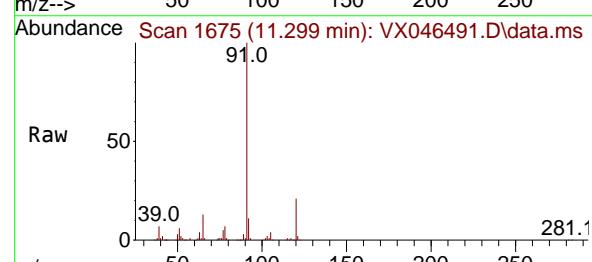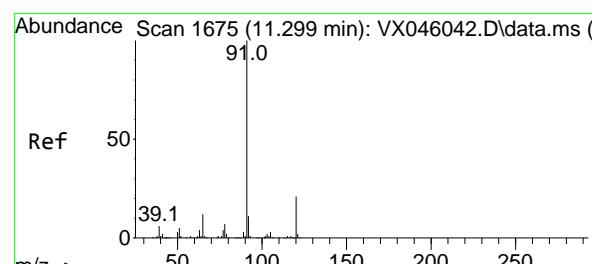

#78

n-propylbenzene

Concen: 20.277 ug/l

RT: 11.299 min Scan# 1675

Delta R.T. 0.000 min


Lab File: VX046491.D




Acq: 04 Jun 2025 11:27

Tgt Ion: 91 Resp: 117360

Ion Ratio Lower Upper

91	100		
120	22.3	10.8	32.4

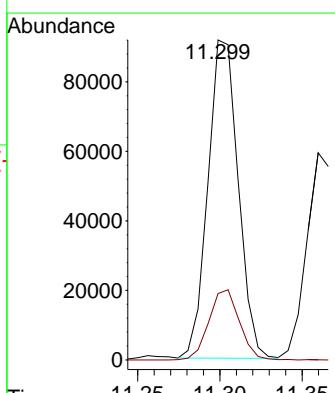



#79

2-Chlorotoluene

Concen: 20.296 ug/l

RT: 11.360 min Scan# 1685

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27




Instrument : MSVOA\_X

ClientSampleId : VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#80

1,3,5-Trimethylbenzene

Concen: 20.642 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt Ion:105 Resp: 85839

Ion Ratio Lower Upper

105 100

120 46.8 23.1 69.2

Time--&gt; 11.30 11.35 11.40

Time--&gt; 11.40 11.45 11.50

Abundance


60000

40000

20000

0

11.360

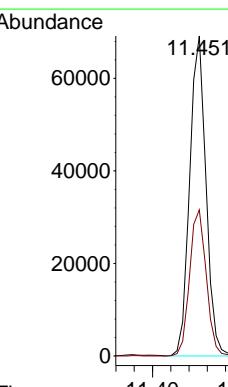

Abundance


60000


40000

20000

0

11.451

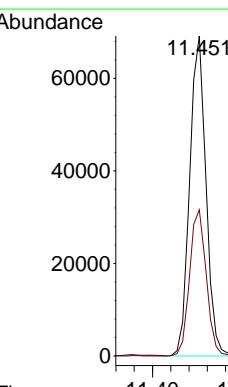


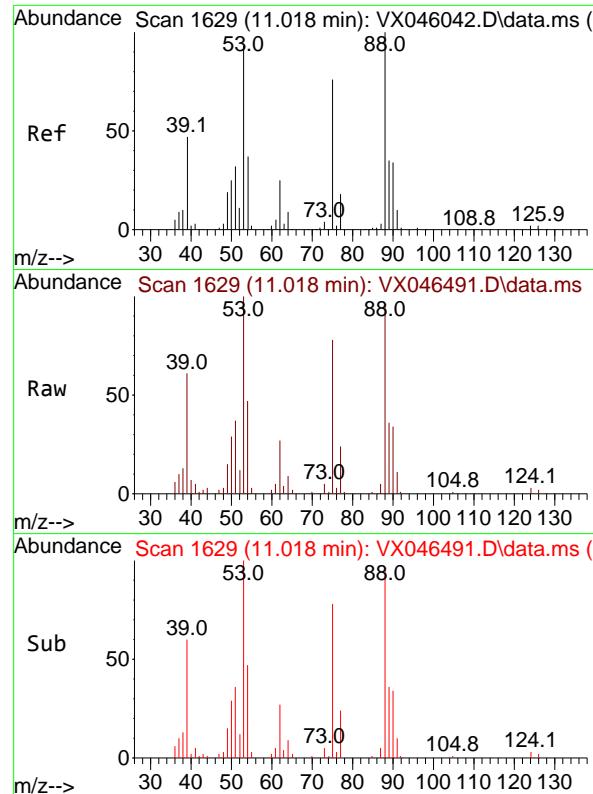


#81  
trans-1,4-Dichloro-2-butene  
Concen: 20.143 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


**Manual Integrations**  
**APPROVED**




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

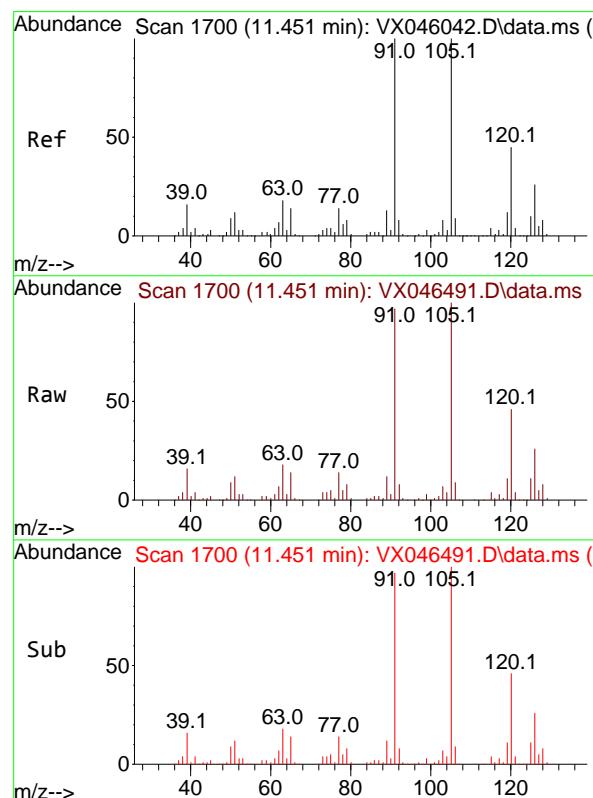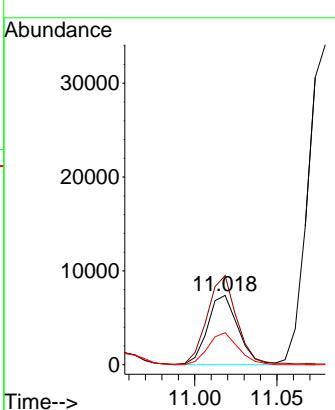

#82  
4-Chlorotoluene  
Concen: 20.186 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion: 91 Resp: 83569  
Ion Ratio Lower Upper  
91 100  
126 27.7 13.3 39.8

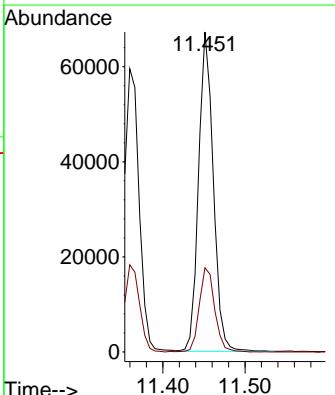



#83

tert-Butylbenzene

Concen: 20.930 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#84

1,2,4-Trimethylbenzene

Concen: 20.630 ug/l


RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt	Ion:105	Resp:	86879
Ion	Ratio	Lower	Upper
105	100		
120	42.5	21.2	63.6

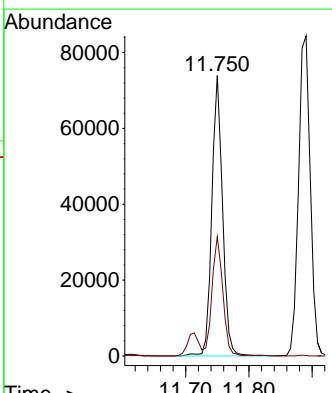

Abundance Scan 1749 (11.750 min): VX046491.D\data.ms (-)

Sub

m/z--&gt;

#84

1,2,4-Trimethylbenzene

Concen: 20.630 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min




Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Tgt	Ion:105	Resp:	86879
Ion	Ratio	Lower	Upper
105	100		
120	42.5	21.2	63.6

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#85

sec-Butylbenzene

Concen: 21.008 ug/l

RT: 11.890 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#86

p-Isopropyltoluene

Concen: 20.553 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion:119 Resp: 87255


Ion Ratio Lower Upper

119 100

134 24.8 12.5 37.5

91 27.6 13.8 41.4

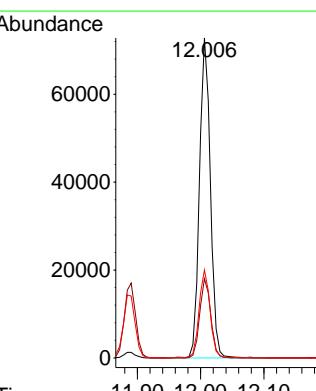

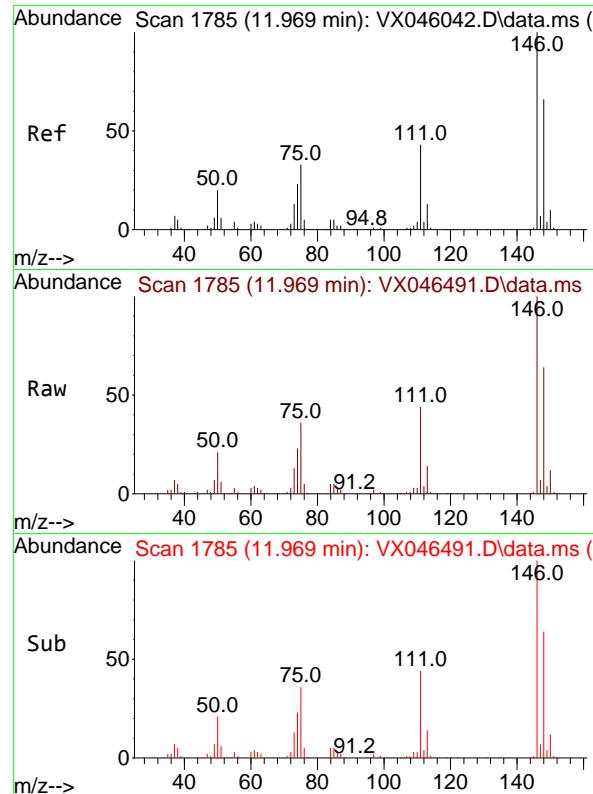

#87

1,3-Dichlorobenzene

Concen: 19.969 ug/l

RT: 11.969 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X

ClientSampleId :

VX0604WBS01

Tgt Ion:146 Resp: 42110

Ion Ratio Lower Upper

146 100

111 46.1 22.1 66.3



148 63.9 32.1 96.5

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

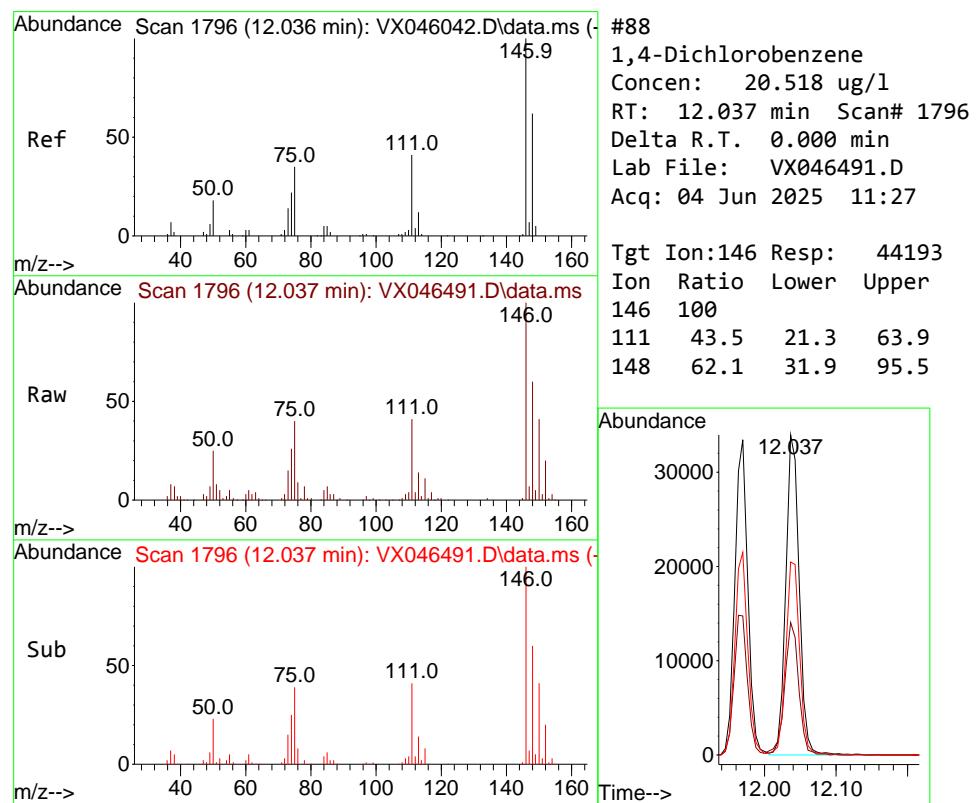

#88

1,4-Dichlorobenzene

Concen: 20.518 ug/l

RT: 12.037 min Scan# 1796

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion:146 Resp: 44193




Ion Ratio Lower Upper

146 100

111 43.5 21.3 63.9

148 62.1 31.9 95.5

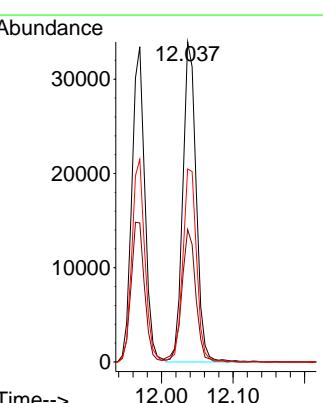

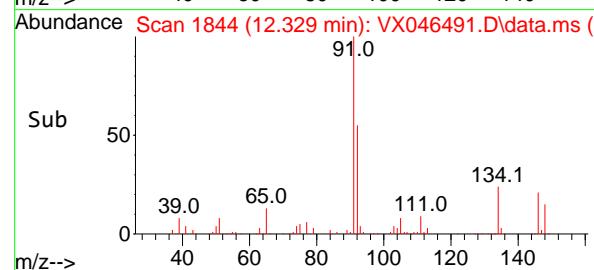

#89

n-Butylbenzene

Concen: 20.149 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#90

Hexachloroethane

Concen: 19.602 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. 0.000 min

Lab File: VX046491.D


Acq: 04 Jun 2025 11:27




Tgt Ion:117 Resp: 14661

Ion Ratio Lower Upper

117 100

201 66.5 31.6 94.7

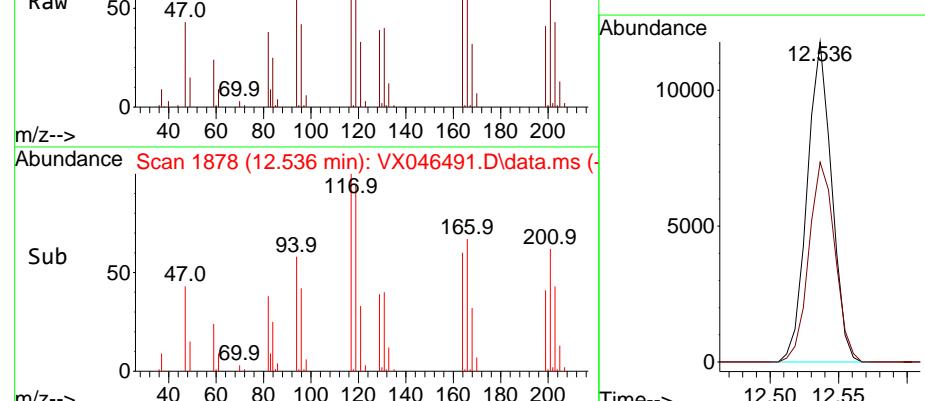



#91

1,2-Dichlorobenzene

Concen: 20.986 ug/l

RT: 12.329 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBS01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 23.797 ug/l

RT: 12.939 min Scan# 1944

Delta R.T. 0.000 min

Lab File: VX046491.D

Acq: 04 Jun 2025 11:27


Tgt Ion: 75 Resp: 9196


Ion Ratio Lower Upper

75 100

155 69.7 34.9 104.8

157 83.7 43.8 131.4




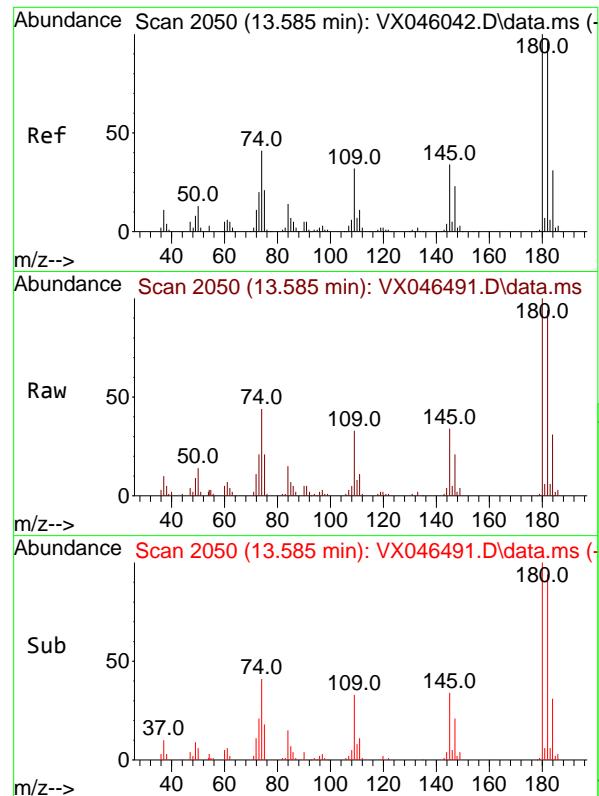


#93  
1,2,4-Trichlorobenzene  
Concen: 20.975 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

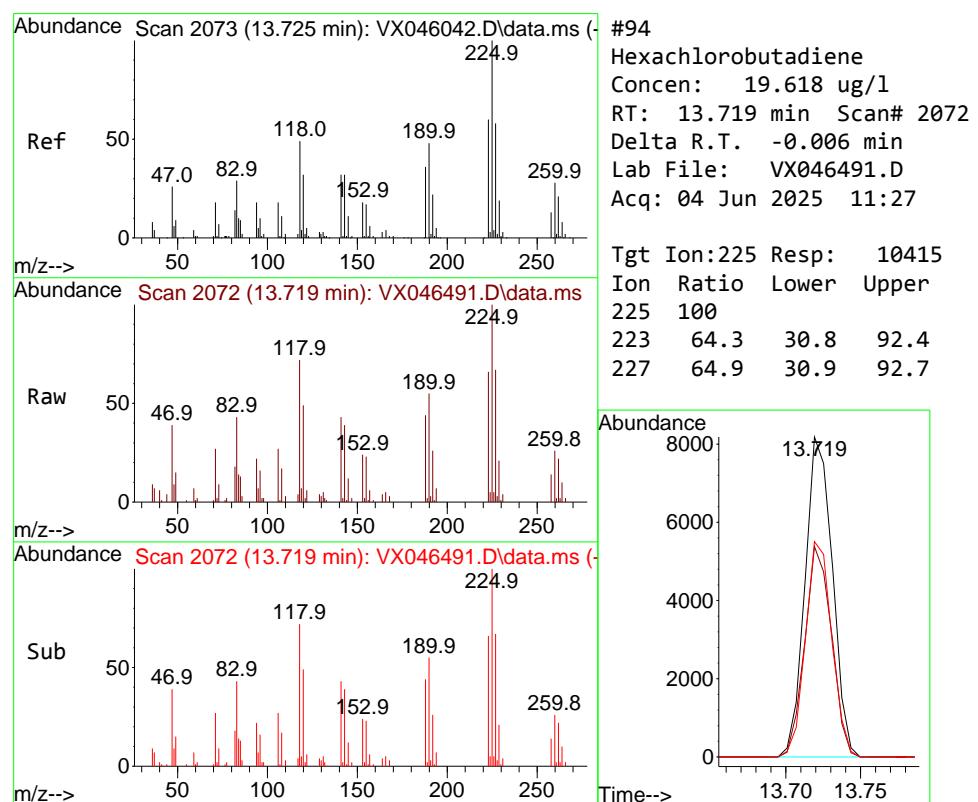

#94  
Hexachlorobutadiene  
Concen: 19.618 ug/l  
RT: 13.719 min Scan# 2072  
Delta R.T. -0.006 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion:225 Resp: 10415  
Ion Ratio Lower Upper  
225 100  
223 64.3 30.8 92.4  
227 64.9 30.9 92.7

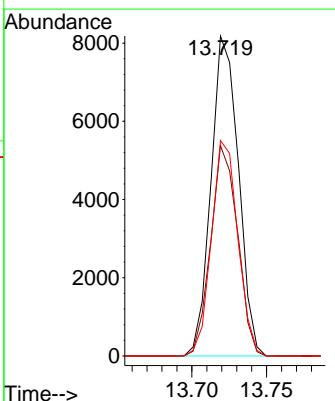


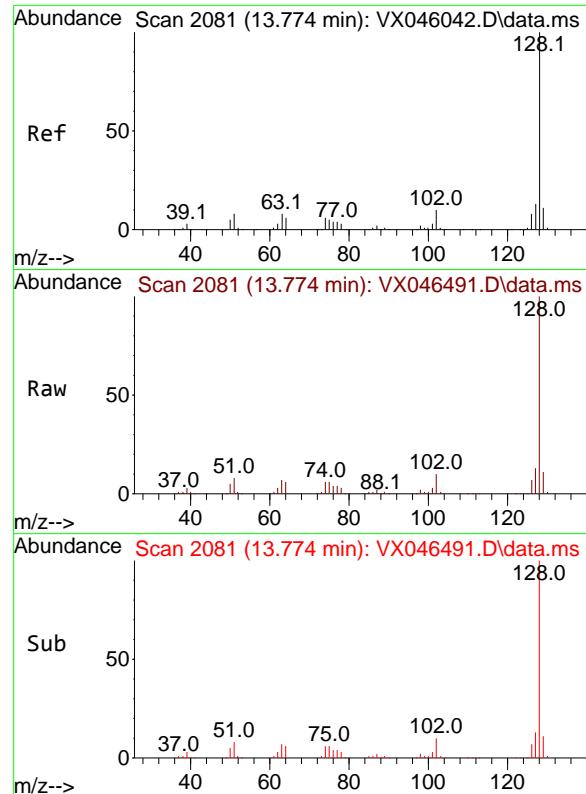


#95  
Naphthalene  
Concen: 21.259 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBS01


**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

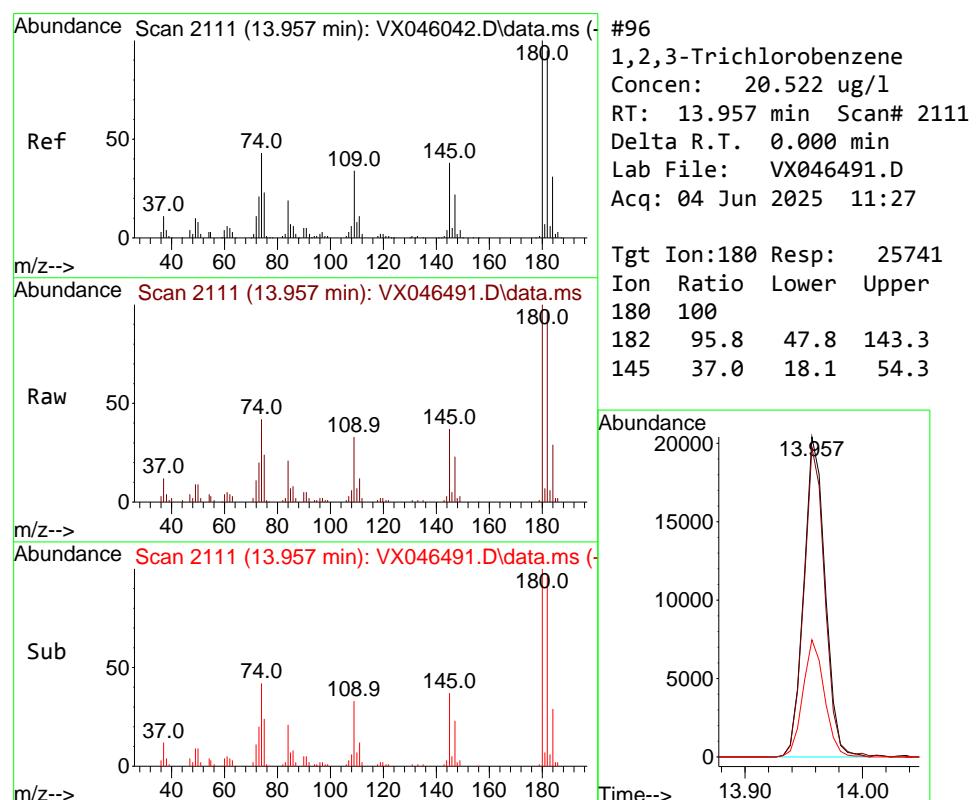

#96  
1,2,3-Trichlorobenzene  
Concen: 20.522 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. 0.000 min  
Lab File: VX046491.D  
Acq: 04 Jun 2025 11:27

Tgt Ion:180 Resp: 25741  
Ion Ratio Lower Upper  
180 100  
182 95.8 47.8 143.3  
145 37.0 18.1 54.3

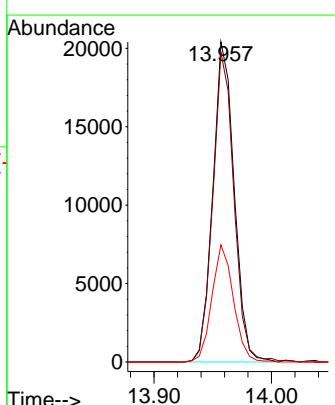



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	JACOBS Engineering Group, Inc.			Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221			Date Received:	
Client Sample ID:	VX0604WBSD01			SDG No.:	Q2200
Lab Sample ID:	VX0604WBSD01			Matrix:	Water
Analytical Method:	8260D			% Solid:	0
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000 uL
Soil Aliquot Vol:			uL	Test:	VOCMS Group3
GC Column:	DB-624UI	ID :	0.18	Level :	LOW
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046497.D	1		06/04/25 13:52	VX060425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
<b>TARGETS</b>						
75-01-4	Vinyl Chloride	18.8		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	20.3		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	22.2		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	22.0		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	22.5		0.20	1.00	ug/L
71-43-2	Benzene	21.4		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	21.6		0.22	1.00	ug/L
79-01-6	Trichloroethene	21.3		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	22.2		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	20.6		0.23	1.00	ug/L
<b>SURROGATES</b>						
17060-07-0	1,2-Dichloroethane-d4	51.7		70 (74) - 130 (125)	103%	SPK: 50
1868-53-7	Dibromofluoromethane	52.1		70 (75) - 130 (124)	104%	SPK: 50
2037-26-5	Toluene-d8	49.0		70 (86) - 130 (113)	98%	SPK: 50
460-00-4	4-Bromofluorobenzene	51.3		70 (77) - 130 (121)	103%	SPK: 50
<b>INTERNAL STANDARDS</b>						
363-72-4	Pentafluorobenzene	84500	5.55			
540-36-3	1,4-Difluorobenzene	153000	6.757			
3114-55-4	Chlorobenzene-d5	133000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	62800	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046497.D  
 Acq On : 04 Jun 2025 13:52  
 Operator : JC/MD  
 Sample : VX0604WBSD01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBSD01

Quant Time: Jun 05 01:51:31 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) Pentafluorobenzene	5.550	168	84483	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	152834	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	133225	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	62838	50.000	ug/l	0.00
<b>System Monitoring Compounds</b>						
33) 1,2-Dichloroethane-d4	5.952	65	81368	51.661	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 103.320%		
35) Dibromofluoromethane	5.385	113	57316	52.079	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 104.160%		
50) Toluene-d8	8.647	98	186769	49.031	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 98.060%		
62) 4-Bromofluorobenzene	11.079	95	75026	51.347	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 102.700%		
<b>Target Compounds</b>						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	24632	19.049	ug/l	99
3) Chloromethane	1.307	50	23757	18.946	ug/l	97
4) Vinyl Chloride	1.374	62	21918	18.781	ug/l	98
5) Bromomethane	1.593	94	9220	17.033	ug/l	98
6) Chloroethane	1.672	64	15446	24.792	ug/l	94
7) Trichlorofluoromethane	1.880	101	35809	20.761	ug/l	97
8) Diethyl Ether	2.136	74	12725	21.673	ug/l	95
9) 1,1,2-Trichlorotrifluo...	2.319	101	21610	20.246	ug/l	97
10) Methyl Iodide	2.447	142	24073	19.060	ug/l	100
11) Tert butyl alcohol	2.971	59	27971	126.516	ug/l	99
12) 1,1-Dichloroethene	2.312	96	20333	20.297	ug/l	100
13) Acrolein	2.233	56	25349	100.678	ug/l	97
14) Allyl chloride	2.660	41	42621	22.262	ug/l	95
15) Acrylonitrile	3.062	53	73994	117.045	ug/l	99
16) Acetone	2.386	43	72770	115.231	ug/l	98
17) Carbon Disulfide	2.501	76	39956	16.824	ug/l	100
18) Methyl Acetate	2.703	43	45782	31.241	ug/l	99
19) Methyl tert-butyl Ether	3.117	73	82120	23.382	ug/l	100
20) Methylene Chloride	2.782	84	24899	20.575	ug/l	98
21) trans-1,2-Dichloroethene	3.087	96	20553	20.402	ug/l	98
22) Diisopropyl ether	3.763	45	85964	23.245	ug/l	98
23) Vinyl Acetate	3.721	43	352257	108.297	ug/l	100
24) 1,1-Dichloroethane	3.605	63	45805	22.237	ug/l	98
25) 2-Butanone	4.562	43	110519	120.545	ug/l	99
26) 2,2-Dichloropropane	4.471	77	32995	20.465	ug/l	99
27) cis-1,2-Dichloroethene	4.489	96	26678	21.998	ug/l	98
28) Bromochloromethane	4.897	49	22848	23.044	ug/l	98
29) Tetrahydrofuran	5.013	42	69743	121.397	ug/l	99
30) Chloroform	5.092	83	48458	22.570	ug/l	97
31) Cyclohexane	5.458	56	39649	21.123	ug/l	96
32) 1,1,1-Trichloroethane	5.379	97	41875	22.500	ug/l	97
36) 1,1-Dichloropropene	5.690	75	30800	20.829	ug/l	99
37) Ethyl Acetate	4.721	43	40135	21.968	ug/l	98
38) Carbon Tetrachloride	5.678	117	33893	20.399	ug/l	97
39) Methylcyclohexane	7.379	83	37949	19.934	ug/l	92
40) Benzene	6.031	78	92846	21.436	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046497.D  
 Acq On : 04 Jun 2025 13:52  
 Operator : JC/MD  
 Sample : VX0604WBSD01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBSD01

Quant Time: Jun 05 01:51:31 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	24996	26.155	ug/1	95
42) 1,2-Dichloroethane	6.086	62	40404	21.614	ug/1	99
43) Isopropyl Acetate	6.342	43	64639	23.192	ug/1	99
44) Trichloroethene	7.123	130	22185	21.281	ug/1	96
45) 1,2-Dichloropropane	7.427	63	23770	22.070	ug/1	98
46) Dibromomethane	7.580	93	18288	21.529	ug/1	99
47) Bromodichloromethane	7.818	83	36336	21.718	ug/1	99
48) Methyl methacrylate	7.696	41	33430	23.486	ug/1	99
49) 1,4-Dioxane	7.659	88	12861	475.862	ug/1	100
51) 4-Methyl-2-Pentanone	8.574	43	220370	119.115	ug/1	99
52) Toluene	8.714	92	57666	21.713	ug/1	98
53) t-1,3-Dichloropropene	8.976	75	30745	20.675	ug/1	99
54) cis-1,3-Dichloropropene	8.366	75	35234	21.437	ug/1	96
55) 1,1,2-Trichloroethane	9.153	97	23253	22.204	ug/1	96
56) Ethyl methacrylate	9.116	69	39616	23.736	ug/1	99
57) 1,3-Dichloropropane	9.305	76	41148	21.879	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.238	63	98765	116.070	ug/1	99
59) 2-Hexanone	9.427	43	168301	122.961	ug/1	99
60) Dibromochloromethane	9.518	129	24794	21.558	ug/1	99
61) 1,2-Dibromoethane	9.610	107	23687	21.762	ug/1	96
64) Tetrachloroethene	9.269	164	19397	20.578	ug/1	94
65) Chlorobenzene	10.079	112	62199	21.331	ug/1	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	21656	21.749	ug/1	99
67) Ethyl Benzene	10.195	91	113326	22.048	ug/1	99
68) m/p-Xylenes	10.299	106	80924	43.046	ug/1	94
69) o-Xylene	10.640	106	41048	22.397	ug/1	97
70) Styrene	10.652	104	67392	22.447	ug/1	97
71) Bromoform	10.799	173	15427	20.636	ug/1 #	98
73) Isopropylbenzene	10.963	105	110318	22.550	ug/1	100
74) N-amyl acetate	10.841	43	55422	22.926	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	38648	22.544	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	32723m	21.634	ug/1	
77) Bromobenzene	11.195	156	24841	21.872	ug/1	99
78) n-propylbenzene	11.305	91	124223	21.838	ug/1	99
79) 2-Chlorotoluene	11.360	91	78907	21.507	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	92894	22.729	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	9297	20.011	ug/1	99
82) 4-Chlorotoluene	11.451	91	88804	21.826	ug/1	99
83) tert-Butylbenzene	11.713	119	92557	22.483	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	92688	22.395	ug/1	99
85) sec-Butylbenzene	11.890	105	111854	22.129	ug/1	99
86) p-Isopropyltoluene	12.006	119	93040	22.299	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	44995	21.707	ug/1	99
88) 1,4-Dichlorobenzene	12.036	146	44540	21.040	ug/1	98
89) n-Butylbenzene	12.329	91	79526	21.729	ug/1	98
90) Hexachloroethane	12.536	117	15772	21.457	ug/1	98
91) 1,2-Dichlorobenzene	12.335	146	46207	22.214	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	9047	23.821	ug/1	98
93) 1,2,4-Trichlorobenzene	13.585	180	25914	21.691	ug/1	99
94) Hexachlorobutadiene	13.725	225	11422	21.891	ug/1	100
95) Naphthalene	13.774	128	102748	23.449	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	26637	21.608	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
 Data File : VX046497.D  
 Acq On : 04 Jun 2025 13:52  
 Operator : JC/MD  
 Sample : VX0604WBSD01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBSD01

**Manual Integrations**  
**APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

Quant Time: Jun 05 01:51:31 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X050525W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue May 06 07:12:22 2025  
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060425\  
Data File : VX046497.D  
Acq On : 04 Jun 2025 13:52  
Operator : JC/MD  
Sample : VX0604WBSD01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
MSVOA\_X  
**ClientSampleId :**  
VX0604WBSD01

## **Manual Integrations APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

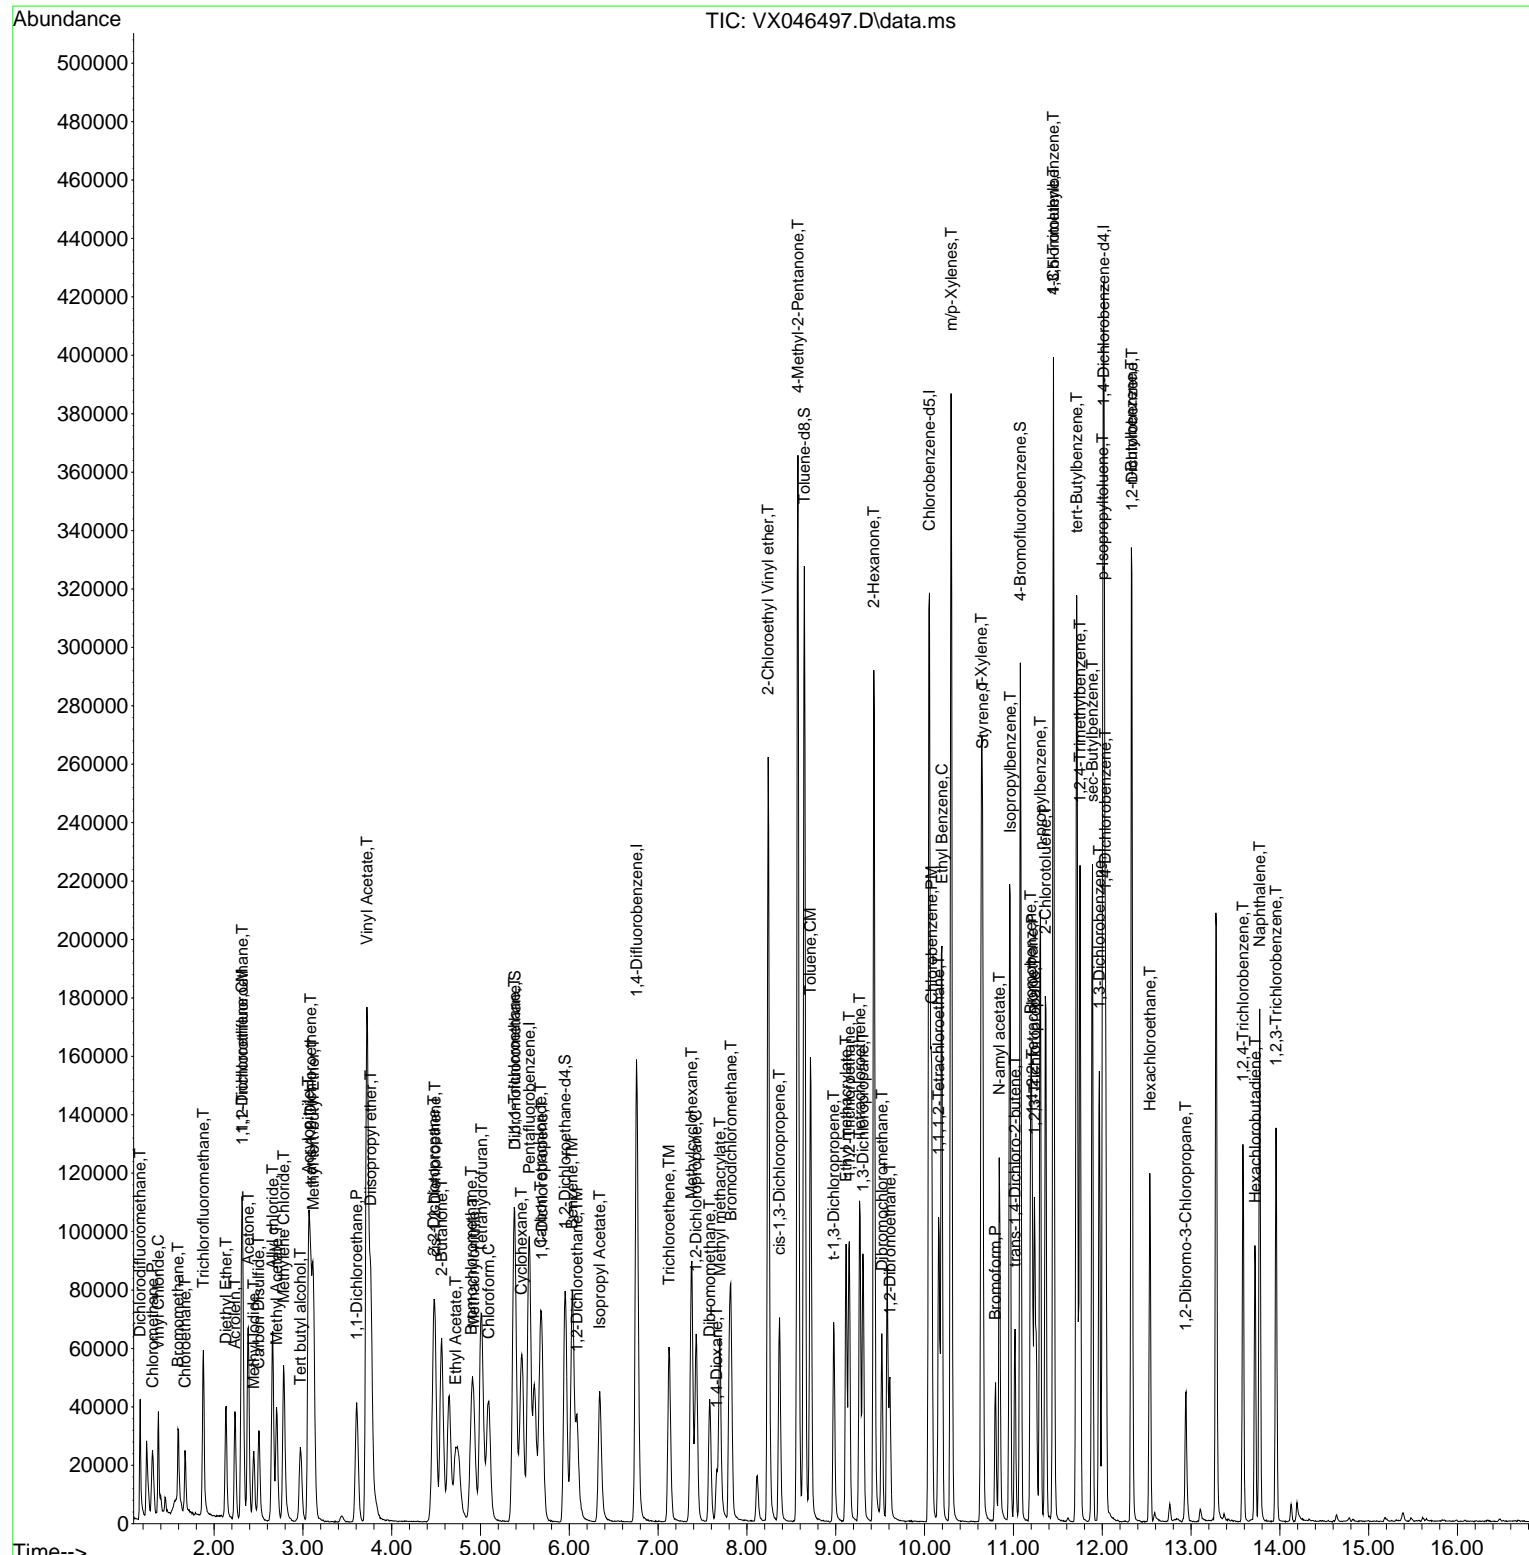


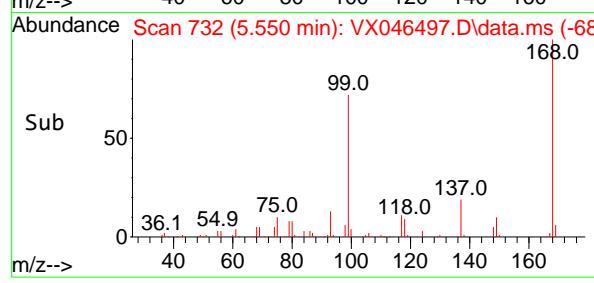




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 7  
Delta R.T. 0.006 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025



#2  
Dichlorodifluoromethane  
Concen: 19.049 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 85 Resp: 24632  
Ion Ratio Lower Upper  
85 100  
87 30.8 15.7 47.1

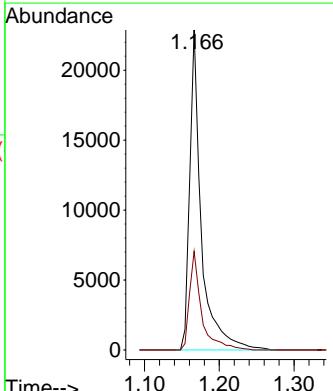



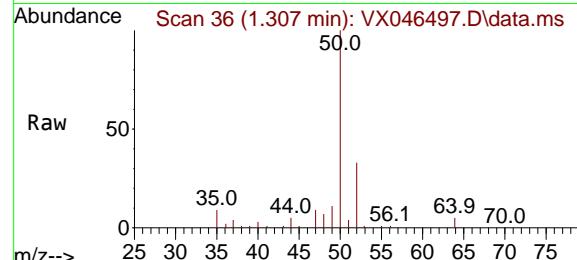



#3  
Chloromethane  
Concen: 18.946 ug/l  
RT: 1.307 min Scan# 3  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

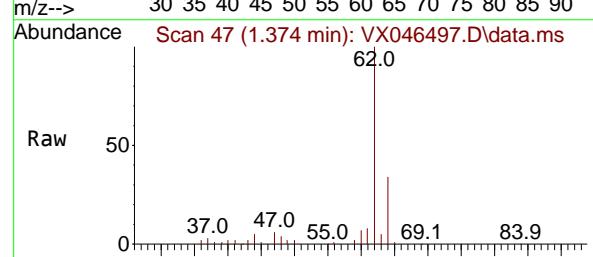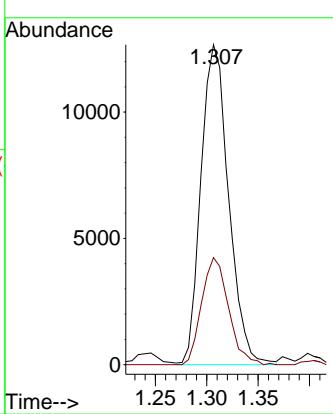

#4  
Vinyl Chloride  
Concen: 18.781 ug/l  
RT: 1.374 min Scan# 47  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 62 Resp: 21918  
Ion Ratio Lower Upper  
62 100  
64 32.7 25.2 37.8









#5  
Bromomethane  
Concen: 17.033 ug/l  
RT: 1.593 min Scan# 8  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

ClientSampleId :  
VX0604WBSD01


### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025




#6  
Chloroethane  
Concen: 24.792 ug/l  
RT: 1.672 min Scan# 96  
Delta R.T. 0.006 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 64 Resp: 15446  
Ion Ratio Lower Upper  
64 100  
66 33.6 24.3 36.5








#7  
Trichlorofluoromethane  
Concen: 20.761 ug/l  
RT: 1.880 min Scan# 129  
Delta R.T. 0.006 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52




Tgt Ion: 101 Resp: 35809  
Ion Ratio Lower Upper  
101 100  
103 61.6 51.0 76.4

### Manual Integrations APPROVED



Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025





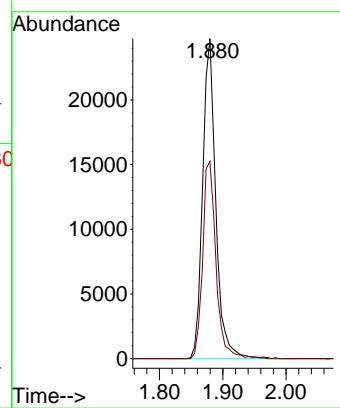
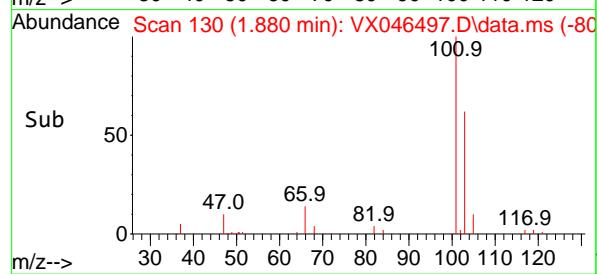


#8  
Diethyl Ether  
Concen: 21.673 ug/l  
RT: 2.136 min Scan# 172  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52



Tgt Ion: 74 Resp: 12725  
Ion Ratio Lower Upper  
74 100  
45 104.6 54.9 164.8

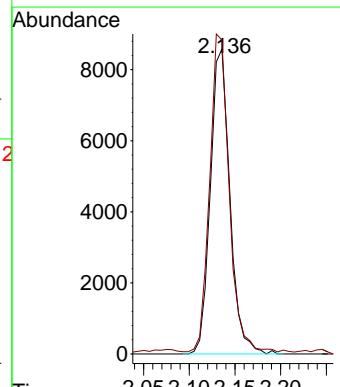

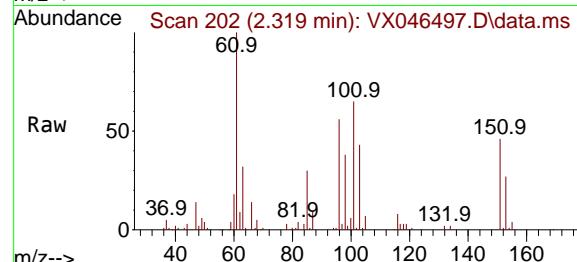

#9

1,1,2-Trichlorotrifluoroethane

Concen: 20.246 ug/l

RT: 2.319 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument :

MSVOA\_X

ClientSampleId :


VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

Abundance

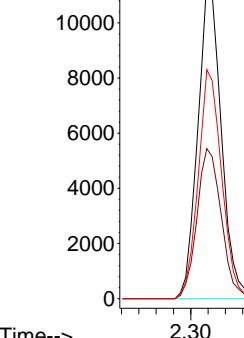

#10

Methyl Iodide

Concen: 19.060 ug/l

RT: 2.447 min Scan# 223

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Tgt Ion:142 Resp: 24073


Ion Ratio Lower Upper







142 100

127 52.3 41.7 62.5

141 14.2 11.5 17.3

Abundance

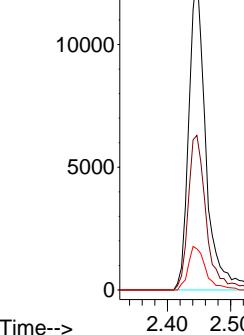



#11

Tert butyl alcohol

Concen: 126.516 ug/l

RT: 2.971 min Scan# 3

Delta R.T. -0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

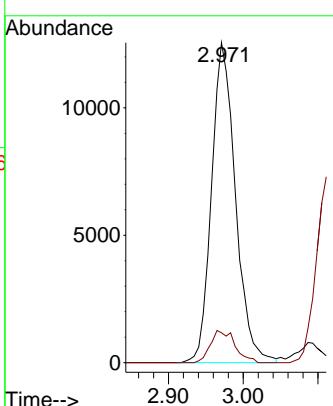

#12

1,1-Dichloroethene

Concen: 20.297 ug/l

RT: 2.312 min Scan# 201

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion: 96 Resp: 20333




Ion Ratio Lower Upper

96 100

61 183.0 146.2 219.2

98 63.3 51.0 76.6









#13

Acrolein  
Concen: 100.678 ug/l  
RT: 2.233 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

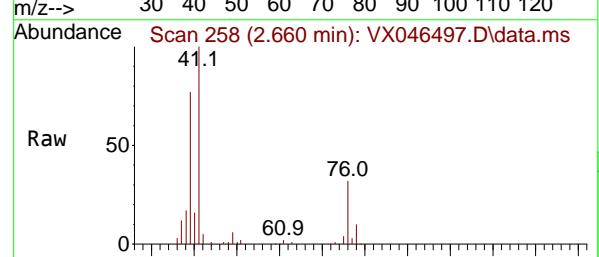
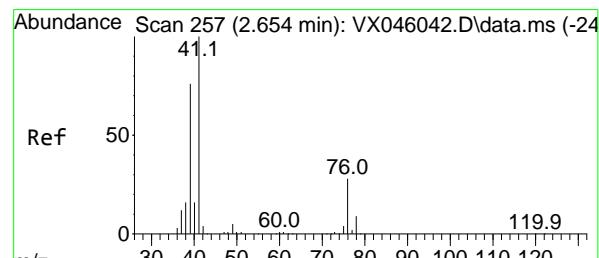



#14

Allyl chloride  
Concen: 22.262 ug/l  
RT: 2.660 min Scan# 258  
Delta R.T. 0.006 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 41 Resp: 42621  
Ion Ratio Lower Upper  
41 100  
39 70.8 60.6 90.8  
76 29.2 24.9 37.3



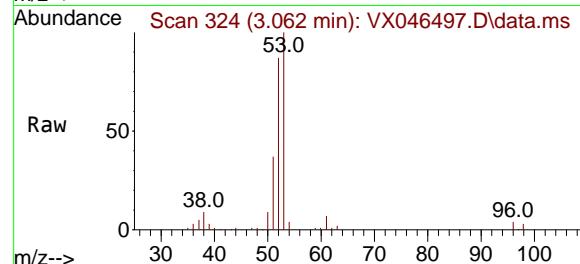

#15

Acrylonitrile

Concen: 117.045 ug/l

RT: 3.062 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

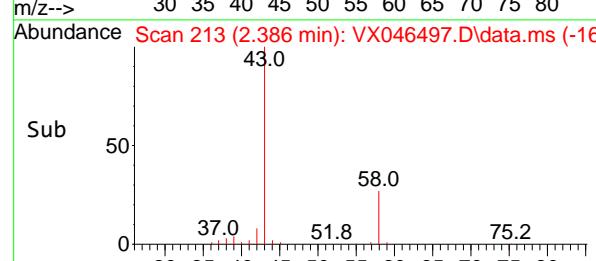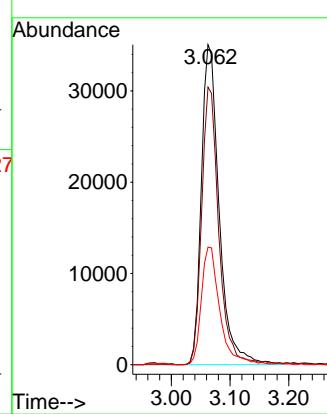

#16

Acetone

Concen: 115.231 ug/l


RT: 2.386 min Scan# 213




Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Tgt	Ion	Resp:	72770
Ion	Ratio	Lower	Upper
43	100		
58	27.5	21.2	31.8

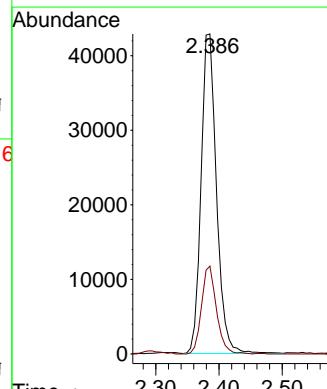



#17

Carbon Disulfide

Concen: 16.824 ug/l

RT: 2.501 min Scan# 2

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#18

Methyl Acetate

Concen: 31.241 ug/l


RT: 2.703 min Scan# 265







Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Tgt Ion: 43 Resp: 45782  
 Ion Ratio Lower Upper  
 43 100  
 74 20.5 16.7 25.1





#19

Methyl tert-butyl Ether

Concen: 23.382 ug/l

RT: 3.117 min Scan# 3

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X

ClientSampleId :

VX0604WBSD01

Tgt Ion: 73 Resp: 82120

Ion Ratio Lower Upper

73 100


57 21.9 17.7 26.5

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

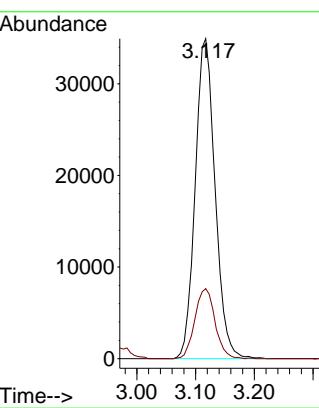

#20

Methylene Chloride

Concen: 20.575 ug/l

RT: 2.782 min Scan# 278

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Tgt Ion: 84 Resp: 24899


Ion Ratio Lower Upper







84 100

49 141.9 113.9 170.9

51 44.1 33.5 50.3

86 62.5 53.8 80.8

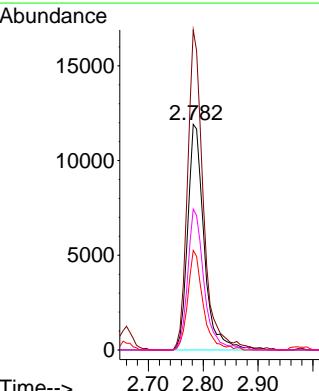

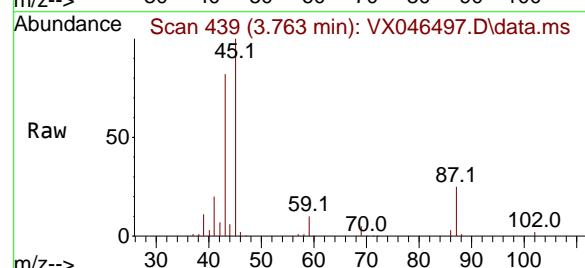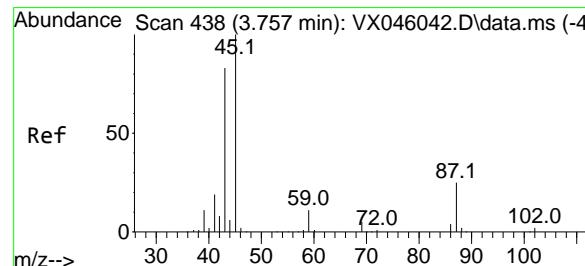

#21

trans-1,2-Dichloroethene

Concen: 20.402 ug/l

RT: 3.087 min Scan# 3

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01


### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

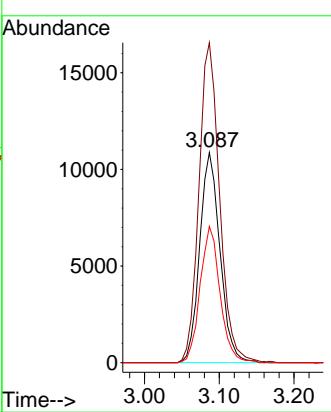

3.087



#23

**Vinyl Acetate**

Concen: 108.297 ug/l

RT: 3.721 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX046497.D





Acq: 04 Jun 2025 13:52

Instrument:


MSVOA\_X

ClientSampleId :



VX0604WBSD01

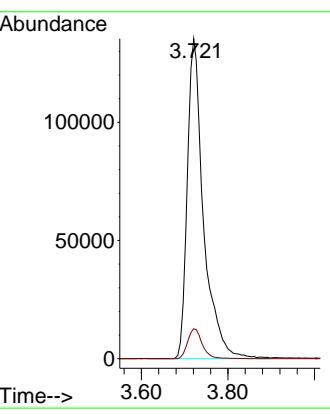


#24  
1,1-Dichloroethane  
Concen: 22.237 ug/l  
RT: 3.605 min Scan# 413  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52




Tgt Ion: 63 Resp: 45805  
Ion Ratio Lower Upper  
63 100  
98 6.3 3.6 10.8  
100 3.7 2.1 6.3

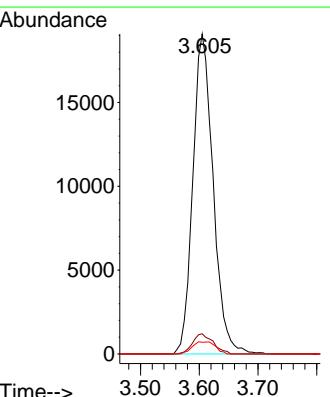


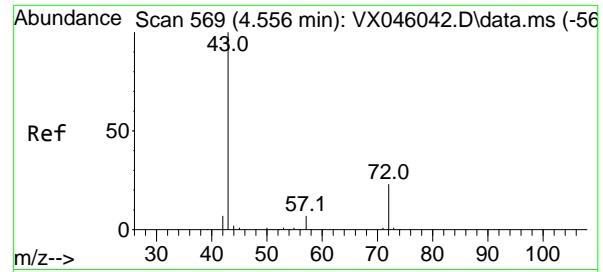


Abundance Scan 570 (4.562 min): VX046497.D\data.ms

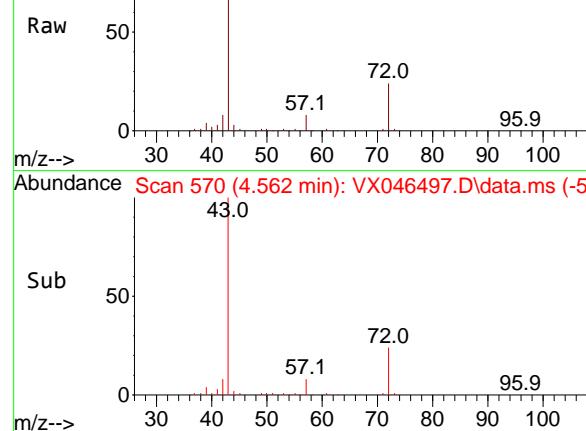


Abundance Scan 570 (4.562 min): VX046497.D\data.ms (-52)

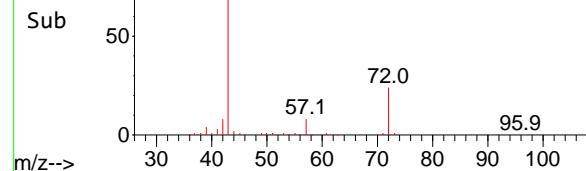


Abundance Scan 554 (4.465 min): VX046042.D\data.ms (-54)

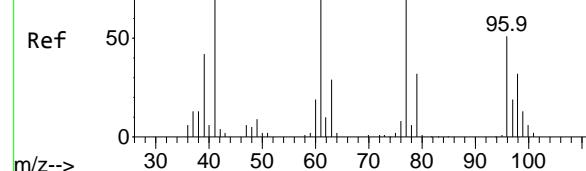

Abundance Scan 555 (4.471 min): VX046497.D\data.ms

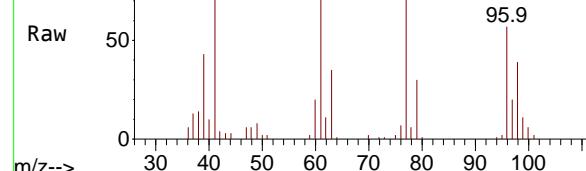

Abundance Scan 555 (4.471 min): VX046497.D\data.ms (-50)

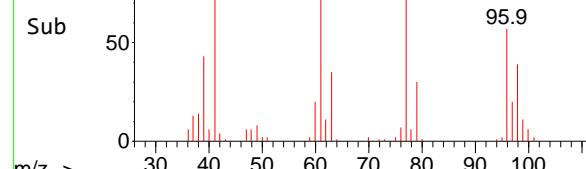

#25

2-Butanone

Concen: 120.545 ug/l

RT: 4.562 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBSD01

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#26

2,2-Dichloropropane

Concen: 20.465 ug/l

RT: 4.471 min Scan# 555

Delta R.T. 0.006 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52







Tgt Ion: 77 Resp: 32995

Ion Ratio Lower Upper

77 100

97 20.4 10.5 31.5

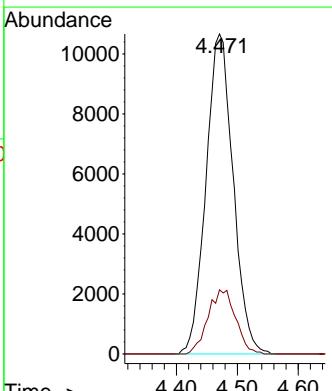

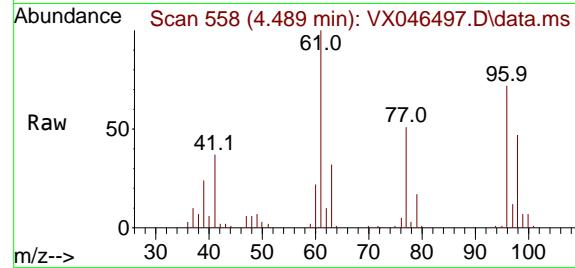


#27  
cis-1,2-Dichloroethene  
Concen: 21.998 ug/l  
RT: 4.489 min Scan# 5  
Delta R.T. 0.006 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


### Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025



#28  
Bromochloromethane  
Concen: 23.044 ug/l  
RT: 4.897 min Scan# 625  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 49 Resp: 22848  
Ion Ratio Lower Upper  
49 100  
129 1.5 0.0 4.0  
130 68.2 56.2 84.2

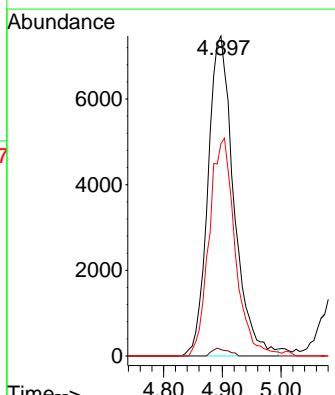

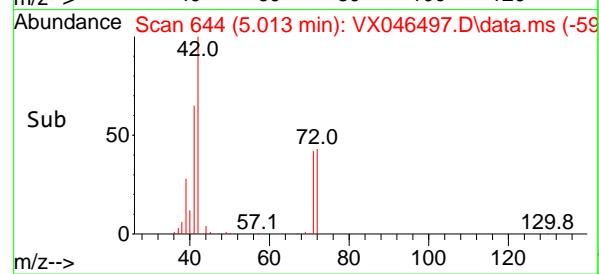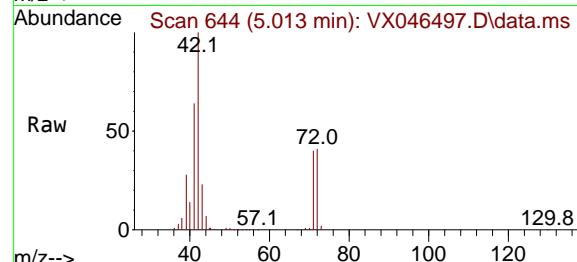

#29

Tetrahydrofuran

Concen: 121.397 ug/l

RT: 5.013 min Scan# 6

Delta R.T. 0.012 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

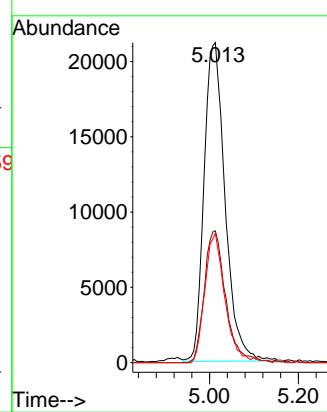

#30

Chloroform

Concen: 22.570 ug/l

RT: 5.092 min Scan# 657

Delta R.T. 0.006 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52


Tgt Ion: 83 Resp: 48458

Ion Ratio Lower Upper


83 100

85 63.6 49.3 73.9


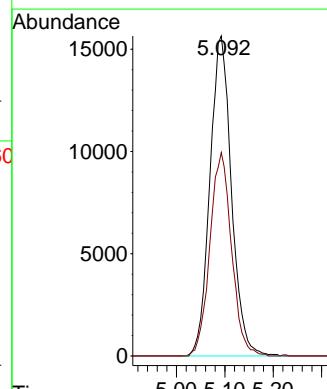





Abundance Scan 717 (5.458 min): VX046497.D\data.ms

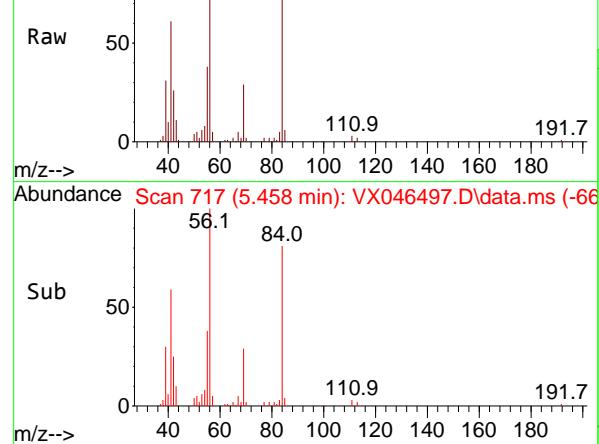


Abundance Scan 717 (5.458 min): VX046497.D\data.ms (-66)

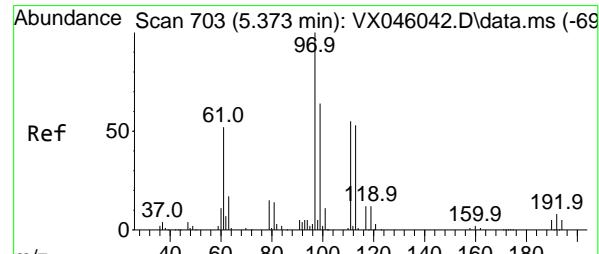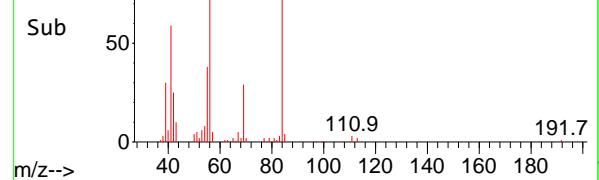

Abundance Scan 704 (5.379 min): VX046497.D\data.ms

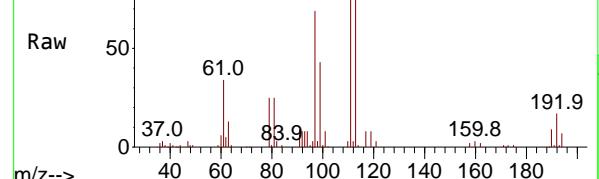

Abundance Scan 704 (5.379 min): VX046497.D\data.ms (-65)

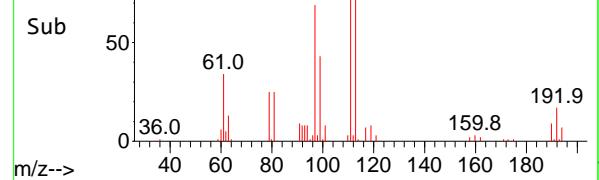

#31

Cyclohexane

Concen: 21.123 ug/l

RT: 5.458 min Scan# 7

Delta R.T. -0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBSD01


**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

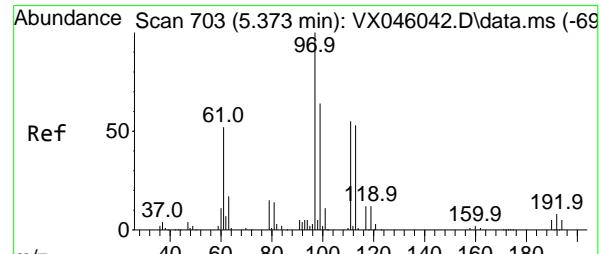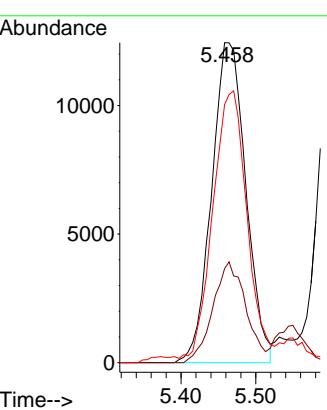

Abundance Scan 704 (5.379 min): VX046497.D\data.ms (-65)

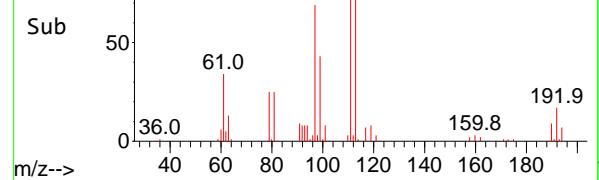

#32

1,1,1-Trichloroethane

Concen: 22.500 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion: 97 Resp: 41875







Ion Ratio Lower Upper

97 100

99 63.1 51.8 77.6

61 47.9 40.1 60.1

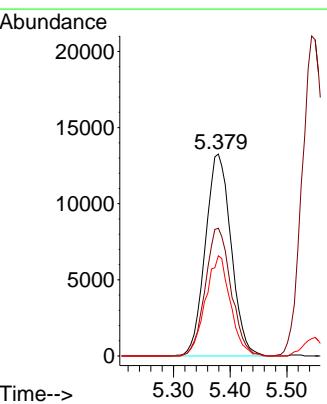

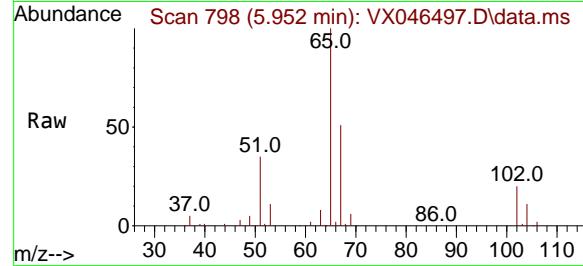

#33

1,2-Dichloroethane-d4

Concen: 51.661 ug/l

RT: 5.952 min Scan# 7

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBSD01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 930  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion:114 Resp: 152834  
Ion Ratio Lower Upper  
114 100  
63 24.9 0.0 49.2  
88 17.9 0.0 33.6

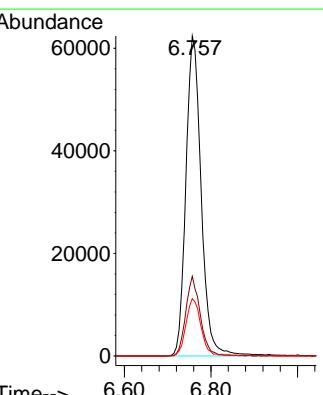

#35


Dibromofluoromethane  
 Concen: 52.079 ug/l  
 RT: 5.385 min Scan# 7  
 Delta R.T. 0.006 min  
 Lab File: VX046497.D  
 Acq: 04 Jun 2025 13:52

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0604WBSD01

Tgt Ion:113 Resp: 57310  
 Ion Ratio Lower Upper  
 113 100  
 111 102.9 83.1 124.7  
 192 16.6 13.3 19.9








### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

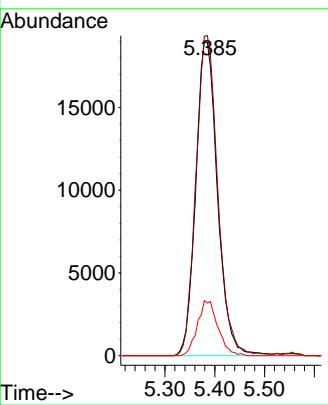

#36  
 1,1-Dichloropropene  
 Concen: 20.829 ug/l  
 RT: 5.690 min Scan# 755  
 Delta R.T. 0.006 min  
 Lab File: VX046497.D  
 Acq: 04 Jun 2025 13:52

Tgt Ion: 75 Resp: 30800  
 Ion Ratio Lower Upper  
 75 100  
 110 31.5 16.3 48.9  
 77 30.0 24.3 36.5

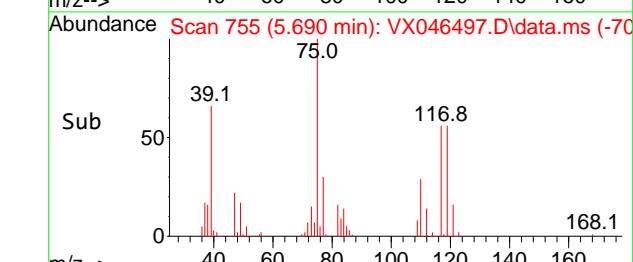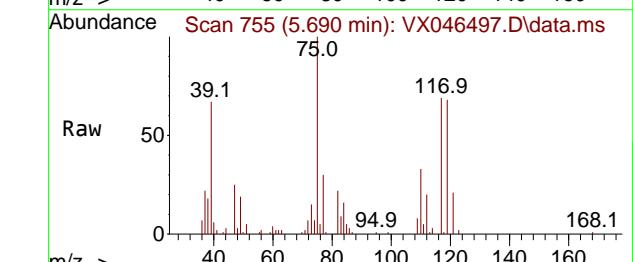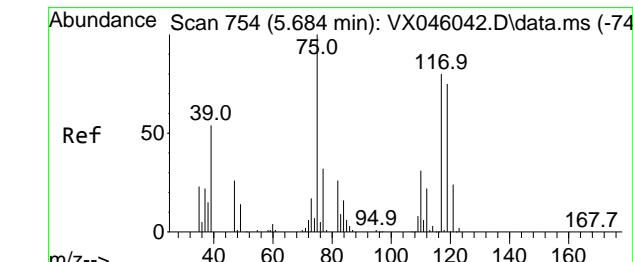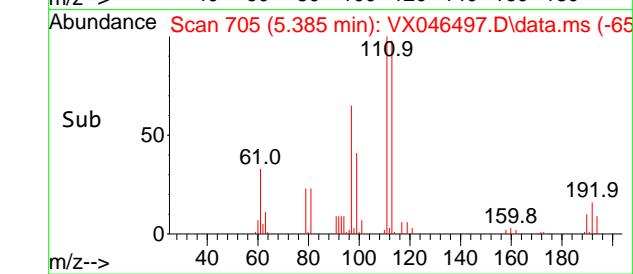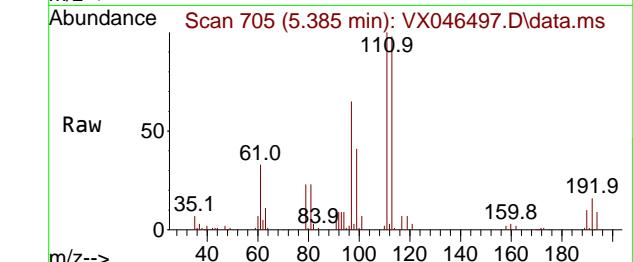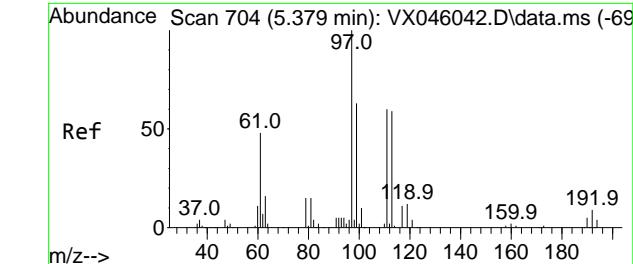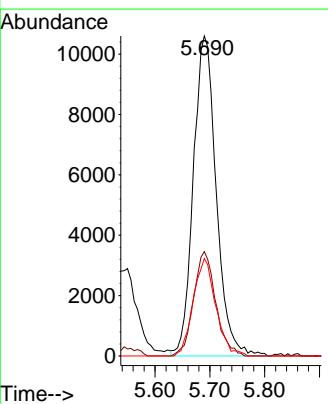

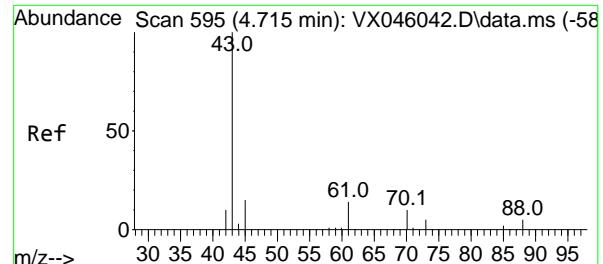

#37

**Ethyl Acetate**

Concen: 21.968 ug/l

RT: 4.721 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X

ClientSampleId :

VX0604WBSD01

Tgt Ion: 43 Resp: 40139

Ion Ratio Lower Upper

43 100





61 12.1 10.3 15.5

70 10.4 7.9 11.9

**Manual Integrations****APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#38

**Carbon Tetrachloride**

Concen: 20.399 ug/l

RT: 5.678 min Scan# 753

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion: 117 Resp: 33893







Ion Ratio Lower Upper

117 100

119 91.9 75.2 112.8

121 32.2 24.2 36.4

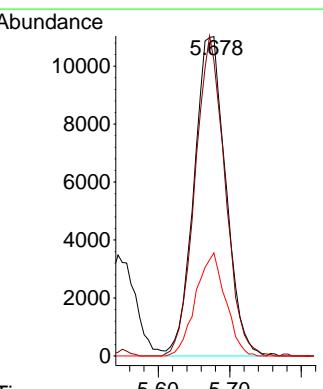



#39

Methylcyclohexane

Concen: 19.934 ug/l

RT: 7.379 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument :

MSVOA\_X


ClientSampleId :

VX0604WBSD01

### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

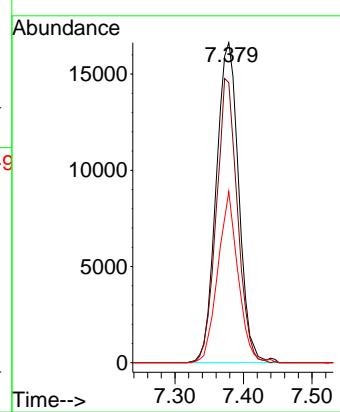

#40

Benzene

Concen: 21.436 ug/l

RT: 6.031 min Scan# 811

Delta R.T. -0.000 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52




Tgt Ion: 78 Resp: 92846

Ion Ratio Lower Upper

78 100

77 23.1 19.0 28.4

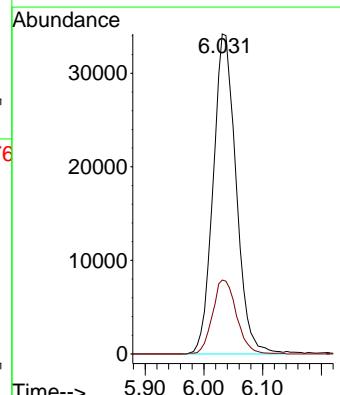

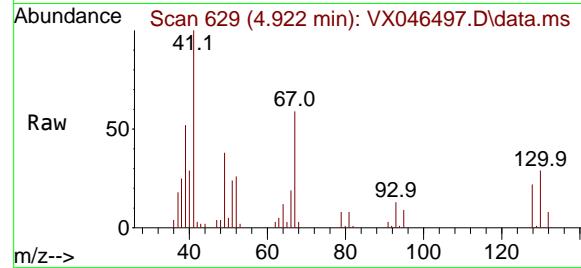

#41

Methacrylonitrile

Concen: 26.155 ug/l

RT: 4.922 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument :

MSVOA\_X




ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#42

1,2-Dichloroethane

Concen: 21.614 ug/l

RT: 6.086 min Scan# 820

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion: 62 Resp: 40404

Ion Ratio Lower Upper

62 100

98 7.4 0.0 15.2

Abundance



#43

Isopropyl Acetate

Concen: 23.192 ug/l

RT: 6.342 min Scan# 8

Instrument:

Delta R.T. 0.006 min

MSVOA\_X


Lab File: VX046497.D

ClientSampleId :


Acq: 04 Jun 2025 13:52

VX0604WBSD01

Abundance Scan 862 (6.342 min): VX046497.D\data.ms

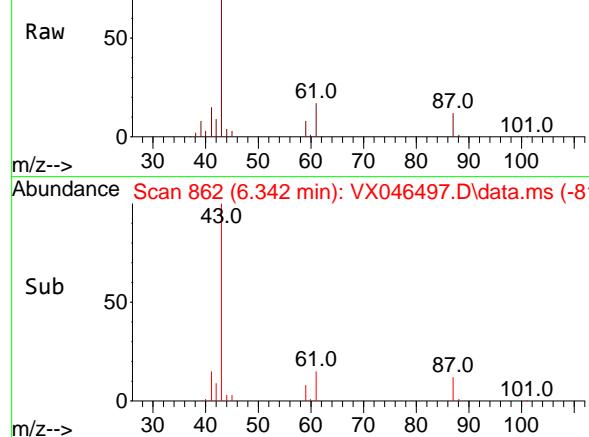

Abundance Scan 862 (6.342 min): VX046497.D\data.ms (-81)

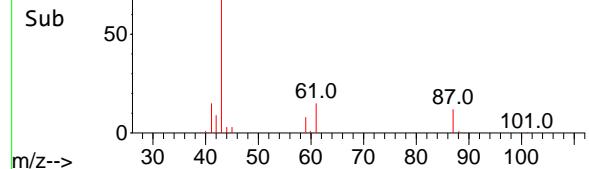

Tgt Ion: 43 Resp: 64639

Ion Ratio Lower Upper

43 100


61 17.6 14.3 21.5

87 11.7 9.5 14.3


Manual Integrations  
APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

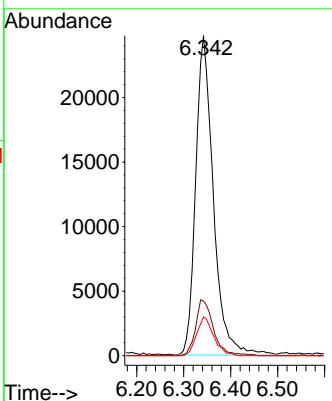

Abundance Scan 990 (7.123 min): VX046042.D\data.ms (-98)

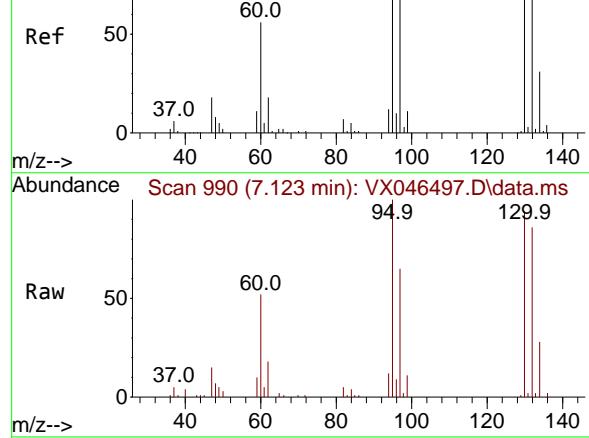

#44

Trichloroethene

Concen: 21.281 ug/l


RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Abundance Scan 990 (7.123 min): VX046497.D\data.ms

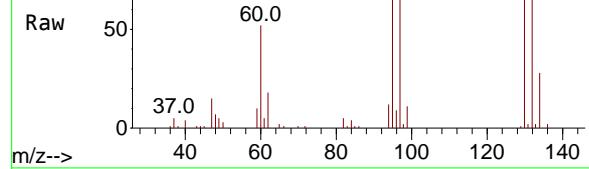


Tgt Ion:130 Resp: 22185


Ion Ratio Lower Upper







130 100

95 106.1 0.0 204.2



Abundance Scan 990 (7.123 min): VX046497.D\data.ms (-94)

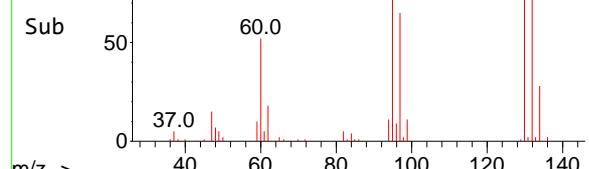1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16



#45

1,2-Dichloropropane

Concen: 22.070 ug/l

RT: 7.427 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

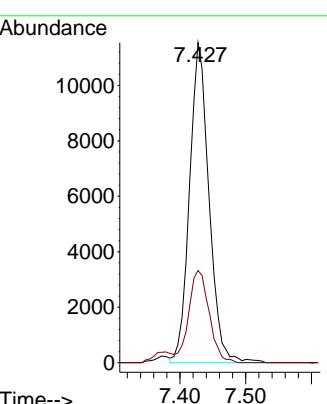

#46

Dibromomethane

Concen: 21.529 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion: 93 Resp: 18288




Ion Ratio Lower Upper

93 100

95 80.1 65.6 98.4

174 84.8 68.2 102.2

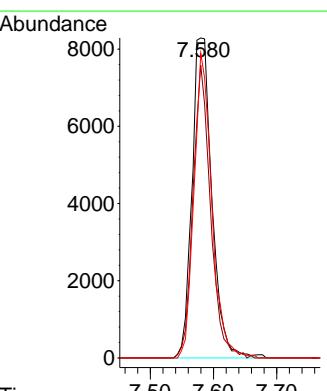







#47

Bromodichloromethane  
Concen: 21.718 ug/l  
RT: 7.818 min Scan# 1104  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument: MSVOA\_X  
ClientSampleId: VX0604WBSD01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025









#48

Methyl methacrylate  
Concen: 23.486 ug/l  
RT: 7.696 min Scan# 1084  
Delta R.T. 0.006 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 41 Resp: 33430  
Ion Ratio Lower Upper  
41 100  
69 72.0 58.5 87.7  
39 64.7 51.7 77.5



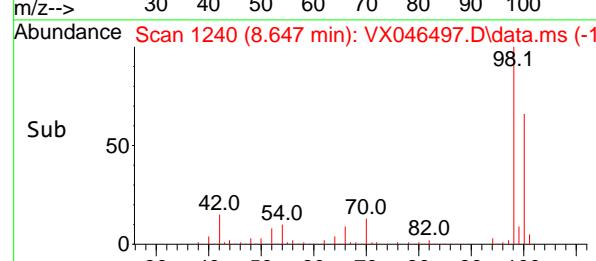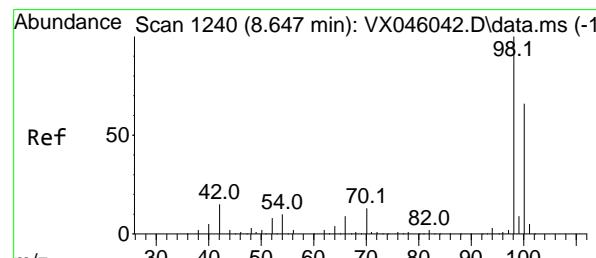

#49

1,4-Dioxane

Concen: 475.862 ug/l

RT: 7.659 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

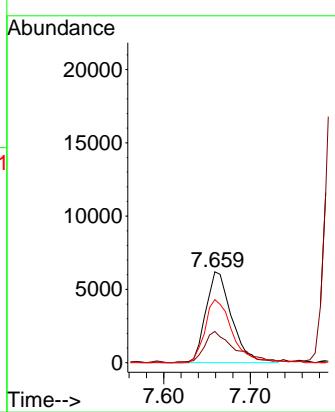

#50

Toluene-d8

Concen: 49.031 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52


Tgt Ion: 98 Resp: 186769

Ion Ratio Lower Upper





98 100

100 64.9 53.5 80.3

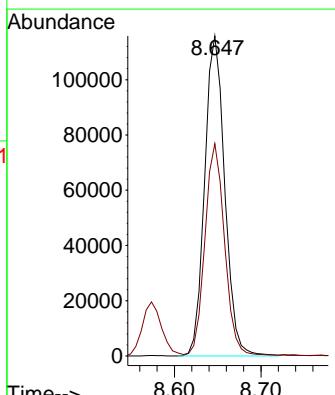



Abundance Scan 1228 (8.574 min): VX046497.D\data.ms

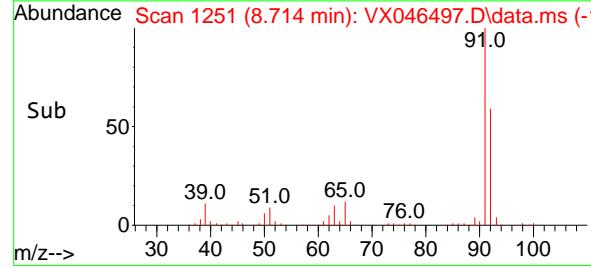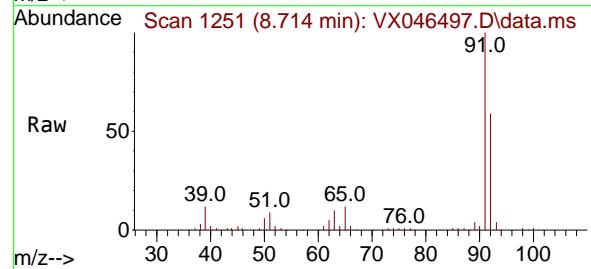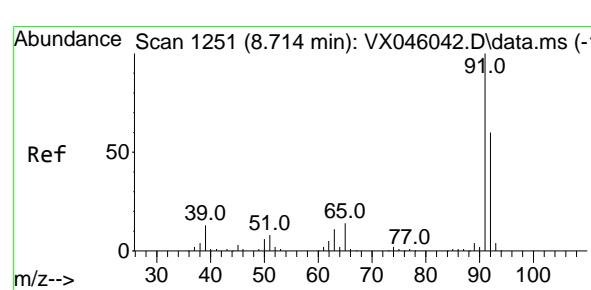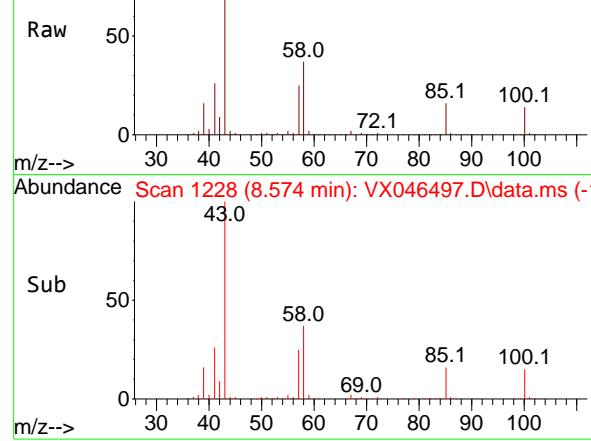

#51

4-Methyl-2-Pentanone

Concen: 119.115 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**


Reviewed By :Mahesh Dadoda 06/05/2025







Supervised By :Semsettin Yesilyurt 06/05/2025

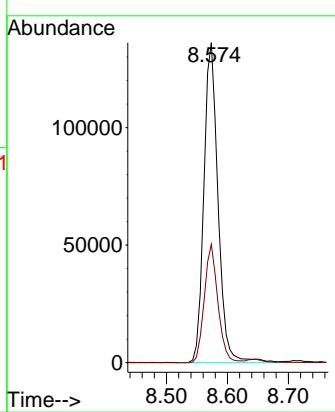

#52  
Toluene  
Concen: 21.713 ug/l  
RT: 8.714 min Scan# 1251  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 92 Resp: 57666  
Ion Ratio Lower Upper  
92 100  
91 173.6 136.6 205.0

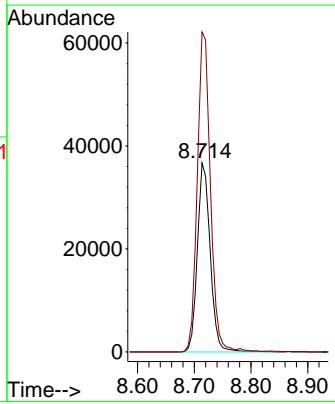



#53

t-1,3-Dichloropropene

Concen: 20.675 ug/l

RT: 8.976 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#54

cis-1,3-Dichloropropene

Concen: 21.437 ug/l

RT: 8.366 min Scan# 1194

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion: 75 Resp: 35234







Ion Ratio Lower Upper

75 100

77 30.9 25.4 38.0

39 60.6 52.2 78.4



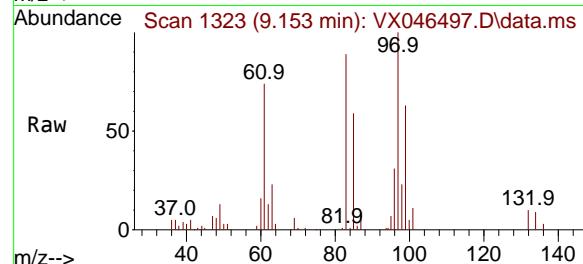

#55

1,1,2-Trichloroethane

Concen: 22.204 ug/l

RT: 9.153 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

### Manual Integrations APPROVED


Reviewed By :Mahesh Dadoda 06/05/2025




Supervised By :Semsettin Yesilyurt 06/05/2025

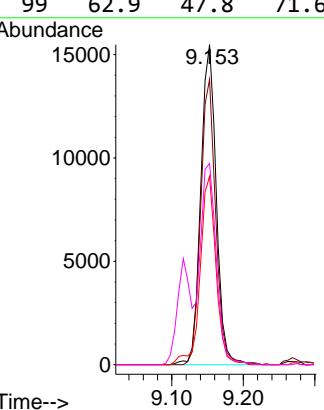

#56  
Ethyl methacrylate  
Concen: 23.736 ug/l  
RT: 9.116 min Scan# 1317  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 69 Resp: 39616  
Ion Ratio Lower Upper  
69 100  
41 75.9 60.8 91.2  
39 47.0 39.0 58.6

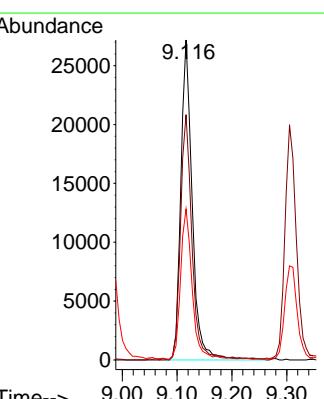

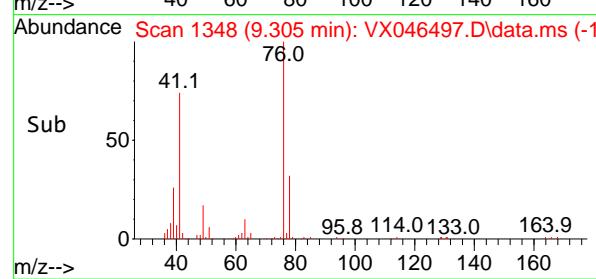

#57

1,3-Dichloropropane

Concen: 21.879 ug/l

RT: 9.305 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

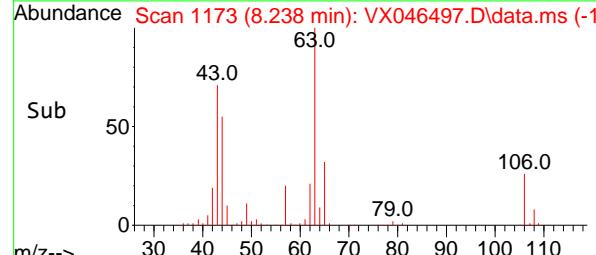

#58

2-Chloroethyl Vinyl ether

Concen: 116.070 ug/l


RT: 8.238 min Scan# 1173


Delta R.T. -0.000 min

Lab File: VX046497.D



Acq: 04 Jun 2025 13:52

Tgt Ion: 63 Resp: 98765  
 Ion Ratio Lower Upper  
 63 100  
 106 27.3 21.5 32.3






Abundance Scan 1368 (9.427 min): VX046497.D\data.ms

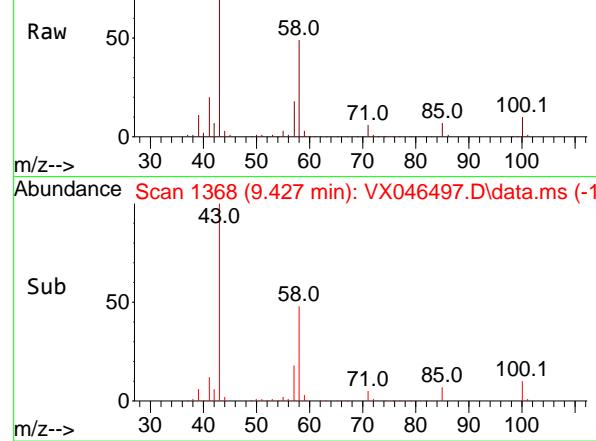

Abundance Scan 1383 (9.518 min): VX046497.D\data.ms

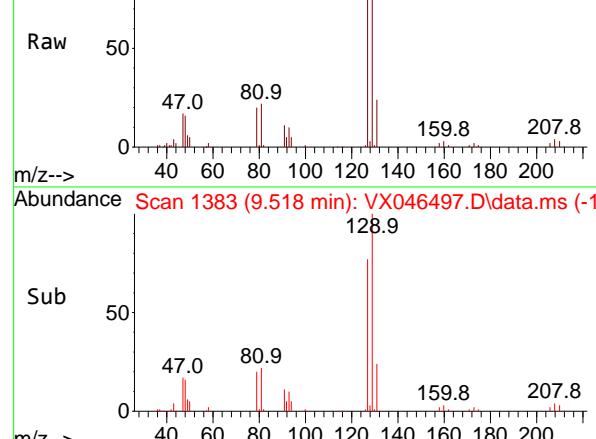

Abundance Scan 1383 (9.518 min): VX046497.D\data.ms (-1)

#59

2-Hexanone

Concen: 122.961 ug/l

RT: 9.427 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

Manual Integrations  
APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#60

Dibromochloromethane

Concen: 21.558 ug/l

RT: 9.518 min Scan# 1383

Delta R.T. -0.000 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52




Tgt Ion:129 Resp: 24794

Ion Ratio Lower Upper

129 100

127 77.3 39.3 117.8

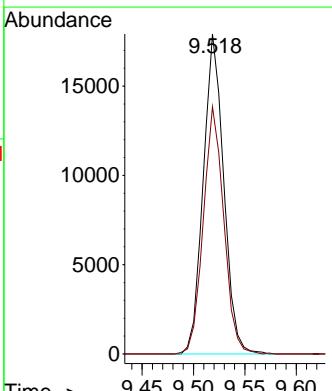

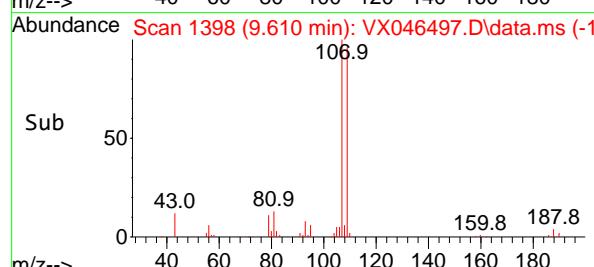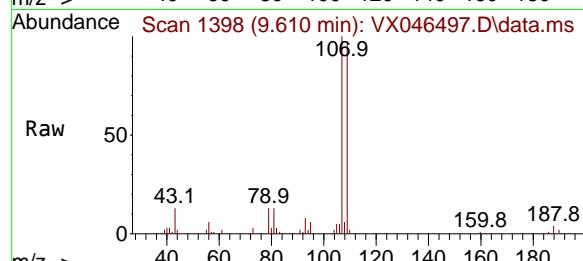

#61

1,2-Dibromoethane

Concen: 21.762 ug/l

RT: 9.610 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X



ClientSampleId :

VX0604WBSD01


**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025


Supervised By :Semsettin Yesilyurt 06/05/2025

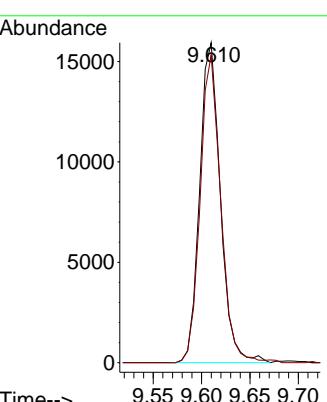


#62  
4-Bromofluorobenzene  
Concen: 51.347 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52



Tgt Ion: 95 Resp: 75026  
Ion Ratio Lower Upper  
95 100  
174 68.2 0.0 135.8  
176 66.1 0.0 131.4

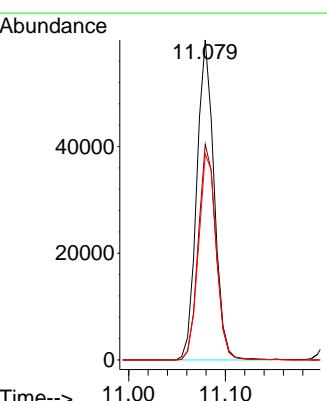


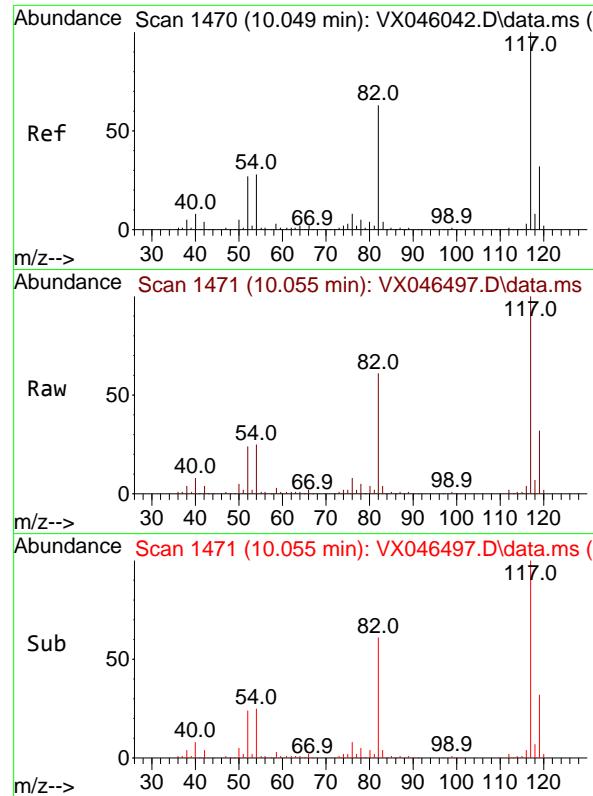


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1470  
Delta R.T. 0.006 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

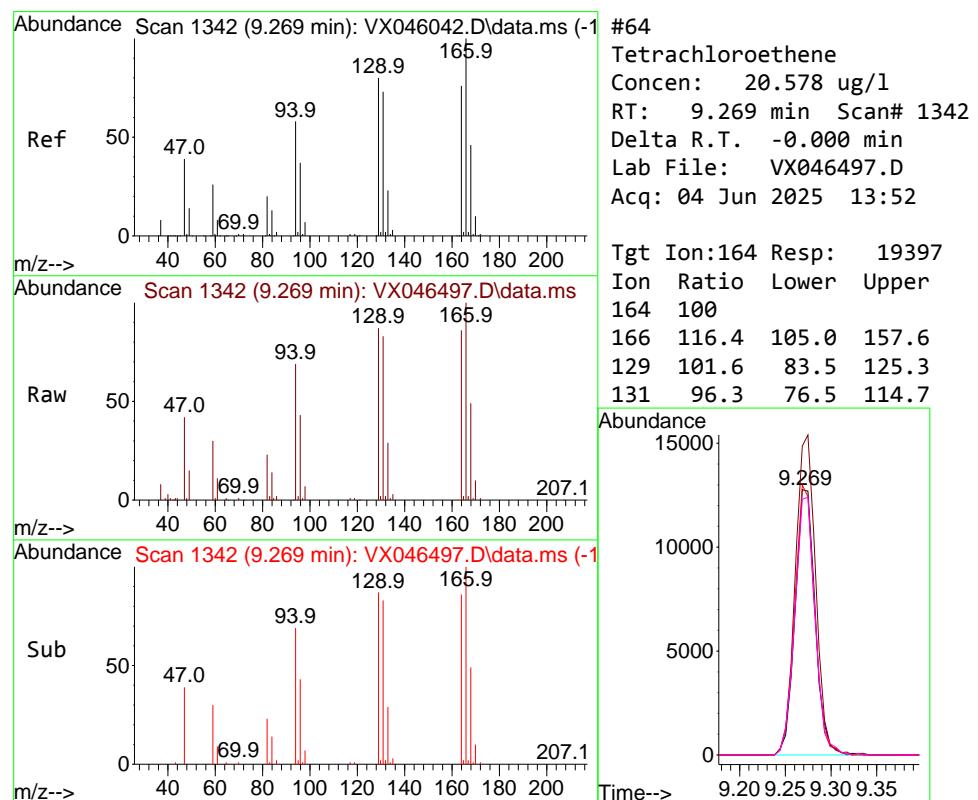

#64  
Tetrachloroethene  
Concen: 20.578 ug/l  
RT: 9.269 min Scan# 1342  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion:164 Resp: 19397  
Ion Ratio Lower Upper  
164 100  
166 116.4 105.0 157.6  
129 101.6 83.5 125.3  
131 96.3 76.5 114.7

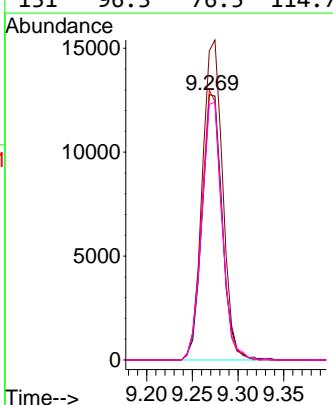







#65  
Chlorobenzene  
Concen: 21.331 ug/l  
RT: 10.079 min Scan# 1475  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


### Manual Integrations APPROVED







Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025



#66  
1,1,1,2-Tetrachloroethane  
Concen: 21.749 ug/l  
RT: 10.159 min Scan# 1488  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion:131 Resp: 21656  
Ion Ratio Lower Upper  
131 100  
133 94.9 47.3 141.9  
119 64.9 31.6 95.0





#67

Ethyl Benzene

Concen: 22.048 ug/l

RT: 10.195 min Scan# 1493

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

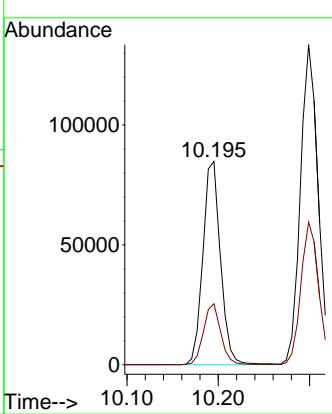

#68

m/p-Xylenes

Concen: 43.046 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52




Tgt Ion:106 Resp: 80924

Ion Ratio Lower Upper

106 100

91 223.3 171.2 256.8

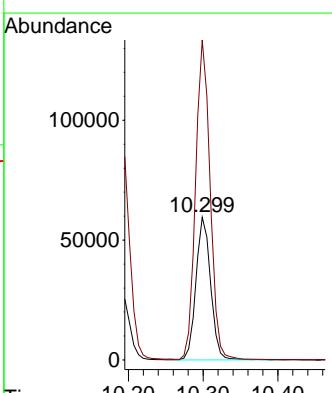







#69  
o-Xylene  
Concen: 22.397 ug/l  
RT: 10.640 min Scan# 1  
Instrument : MSVOA\_X  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52  
ClientSampleId : VX0604WBSD01

Tgt Ion:106 Resp: 41048  
Ion Ratio Lower Upper  
106 100  
91 230.6 112.7 338.1


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

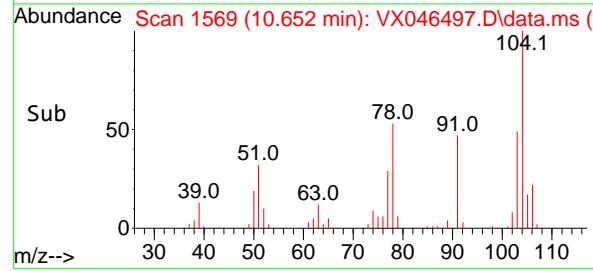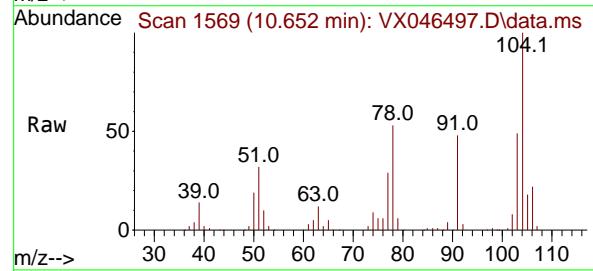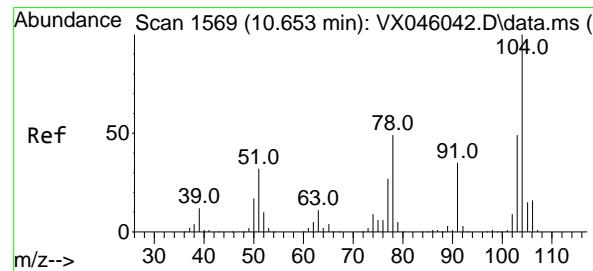

#70  
Styrene  
Concen: 22.447 ug/l  
RT: 10.652 min Scan# 1569  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion:104 Resp: 67392  
Ion Ratio Lower Upper  
104 100  
78 59.9 45.7 68.5  
103 55.7 43.7 65.5



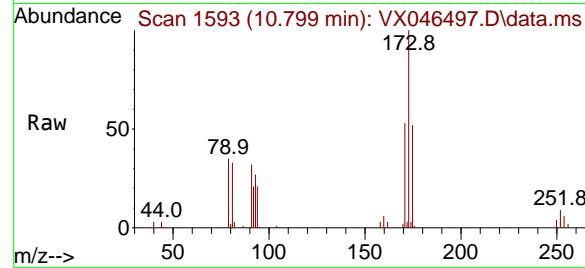

#71

Bromoform

Concen: 20.636 ug/l

RT: 10.799 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion:152 Resp: 62838


Ion Ratio Lower Upper

152 100

115 76.8 46.9 140.7

150 160.6 0.0 351.0

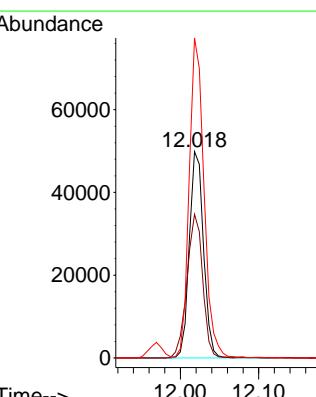

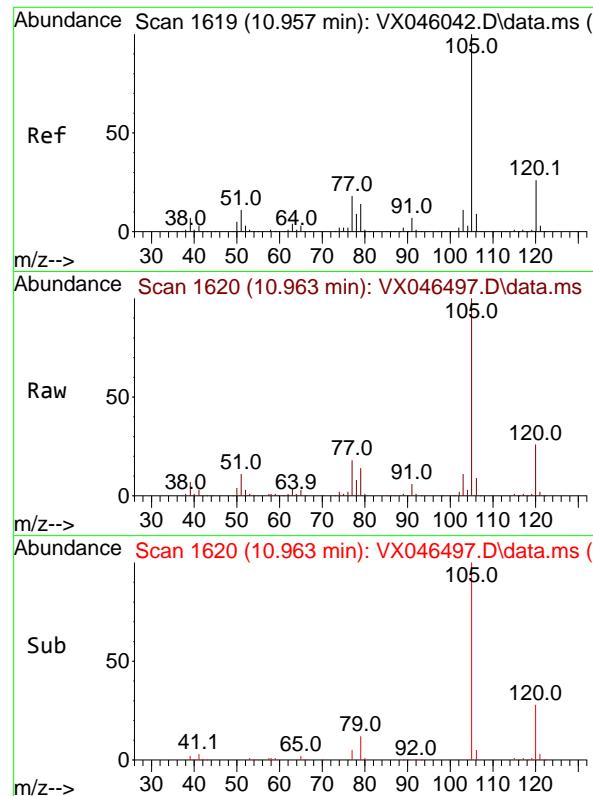

#73

Isopropylbenzene

Concen: 22.550 ug/l

RT: 10.963 min Scan# 1600

Delta R.T. 0.006 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X



ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

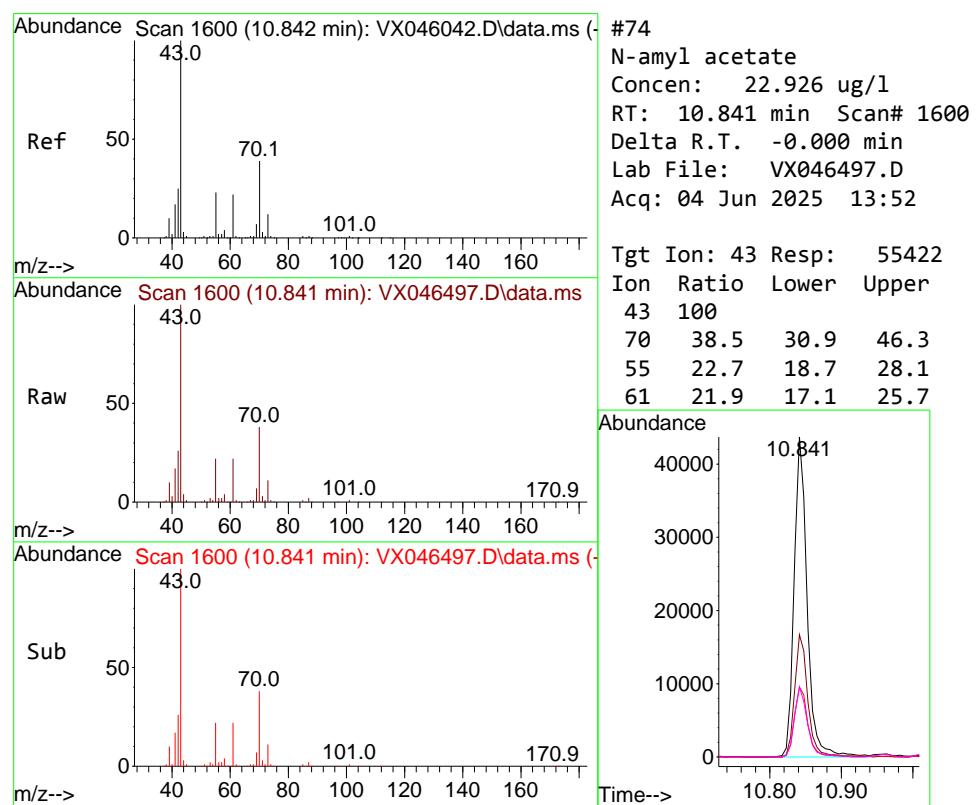

#74

N-amyl acetate

Concen: 22.926 ug/l

RT: 10.841 min Scan# 1600


Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Tgt Ion: 43 Resp: 55422

	Ion	Ratio	Lower	Upper
43	100			
70	38.5	30.9	46.3	
55	22.7	18.7	28.1	
61	21.9	17.1	25.7	

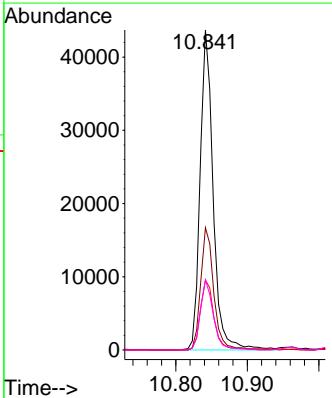


#75  
 1,1,2,2-Tetrachloroethane  
 Concen: 22.544 ug/l  
 RT: 11.213 min Scan# 1  
 Delta R.T. 0.006 min  
 Lab File: VX046497.D  
 Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
 ClientSampleId : VX0604WBSD01

Tgt Ion: 83 Resp: 38643  
 Ion Ratio Lower Upper  
 83 100  
 131 9.7 5.0 14.9  
 85 62.8 31.9 95.7




### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
 Supervised By :Semsettin Yesilyurt 06/05/2025

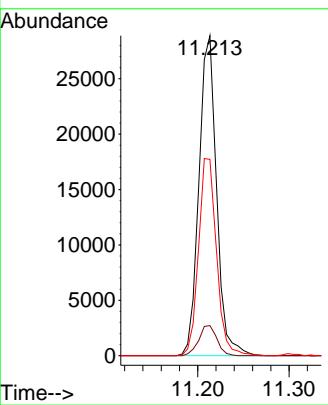

#76  
 1,2,3-Trichloropropane  
 Concen: 21.634 ug/l m  
 RT: 11.238 min Scan# 1665  
 Delta R.T. -0.000 min  
 Lab File: VX046497.D  
 Acq: 04 Jun 2025 13:52

Tgt Ion: 75 Resp: 32723  
 Ion Ratio Lower Upper  
 75 100  
 77 41.8 20.5 61.5

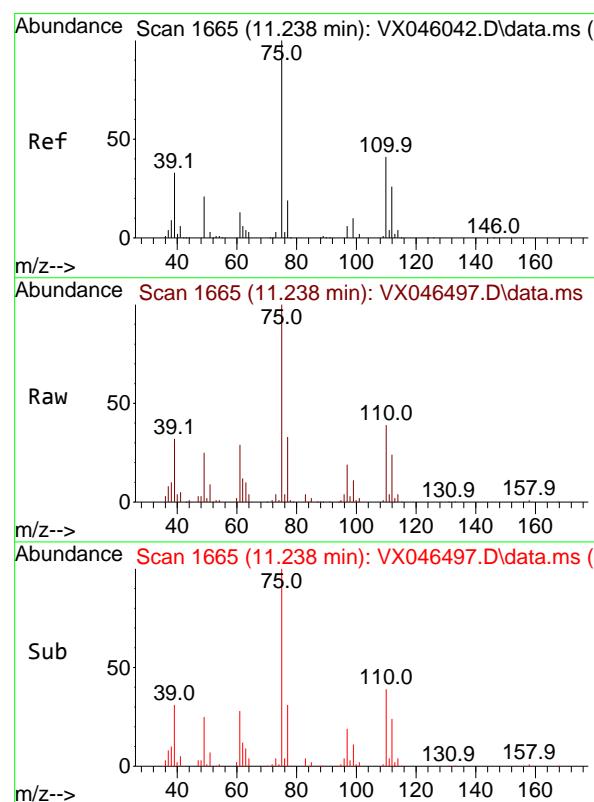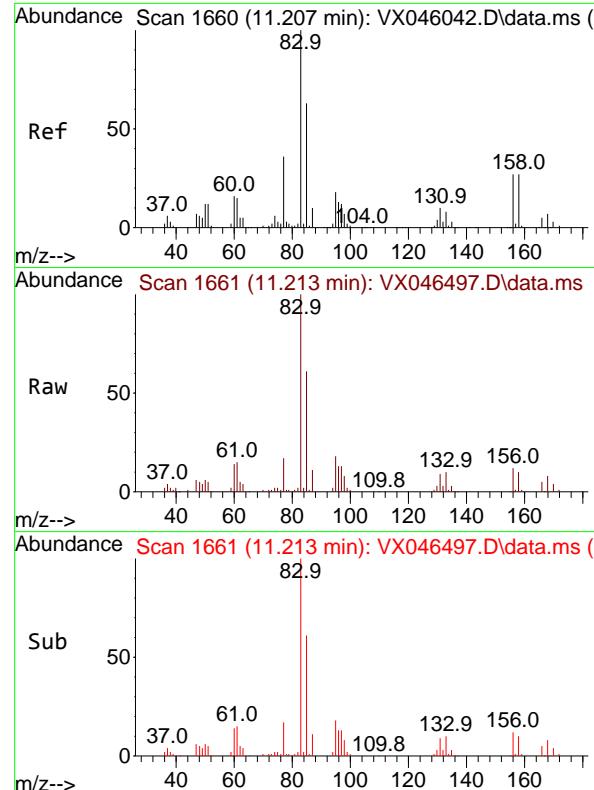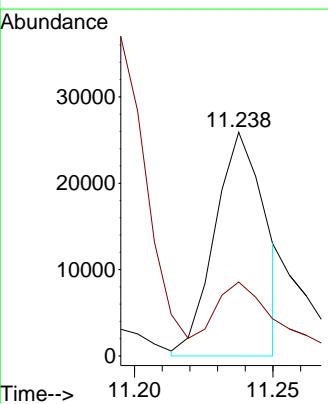

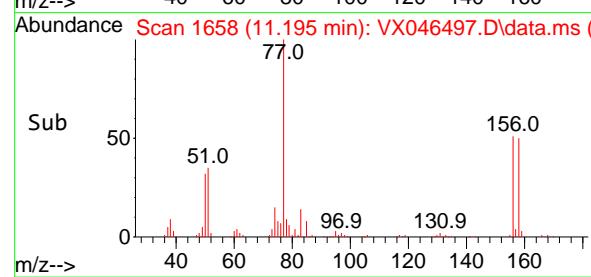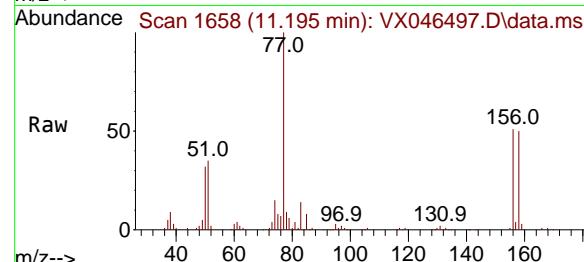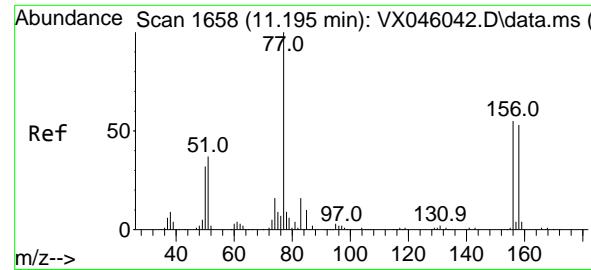

#77

Bromobenzene

Concen: 21.872 ug/l

RT: 11.195 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X





ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

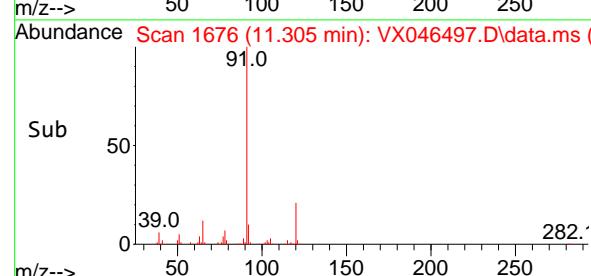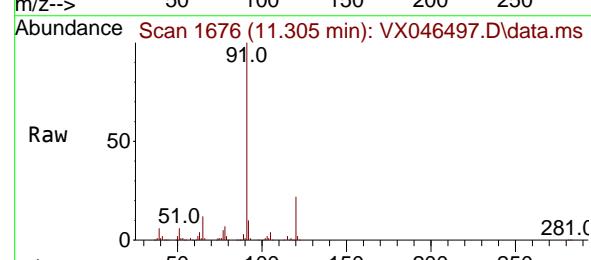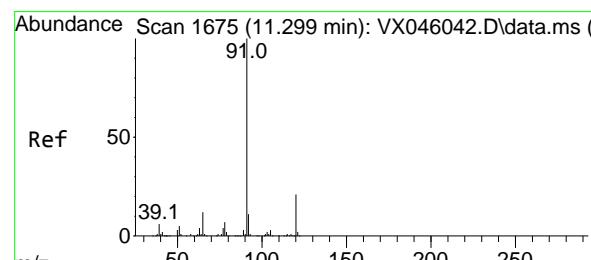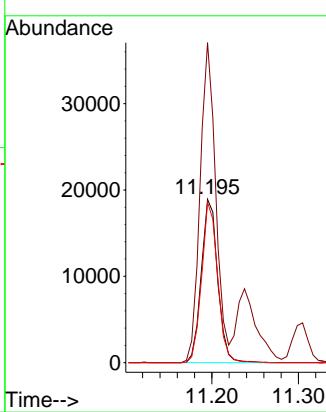

#78

n-propylbenzene

Concen: 21.838 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.006 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52

Tgt Ion: 91 Resp: 124223

Ion Ratio Lower Upper

91 100

120 21.3 10.8 32.4

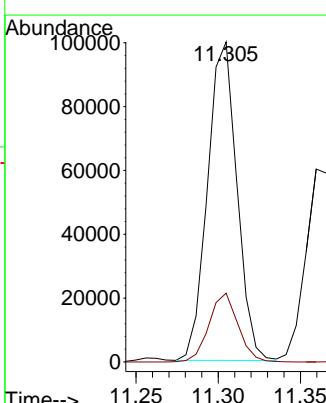

#79

2-Chlorotoluene

Concen: 21.507 ug/l

RT: 11.360 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D




Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X

ClientSampleId :

VX0604WBSD01

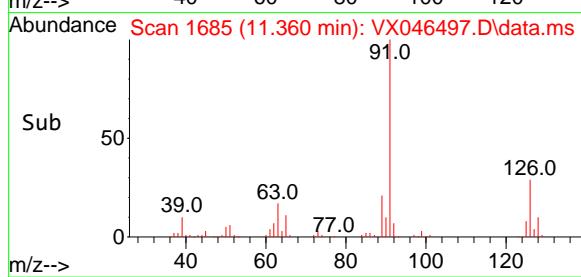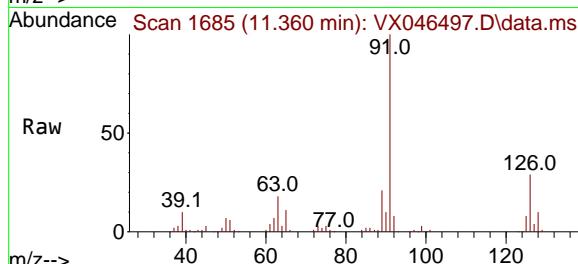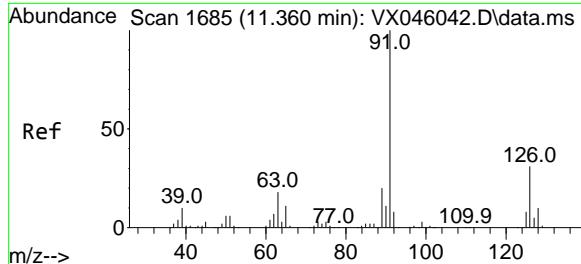

Tgt Ion: 91 Resp: 7890

Ion Ratio Lower Upper





91 100

126 31.6 15.6 46.7

**Manual Integrations****APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

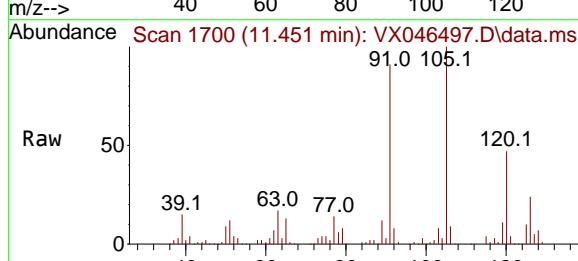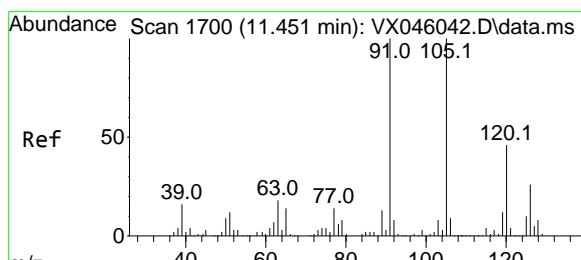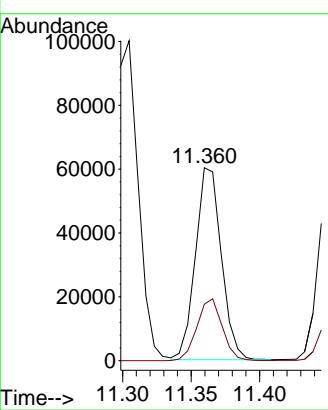

#80

1,3,5-Trimethylbenzene

Concen: 22.729 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52


Tgt Ion:105 Resp: 92894

Ion Ratio Lower Upper

105 100

120 46.2 23.1 69.2

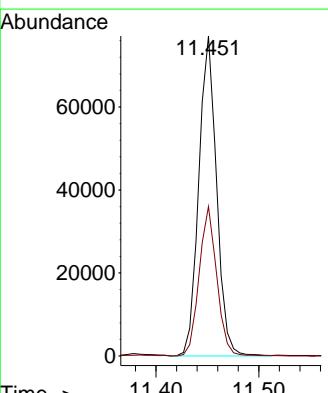


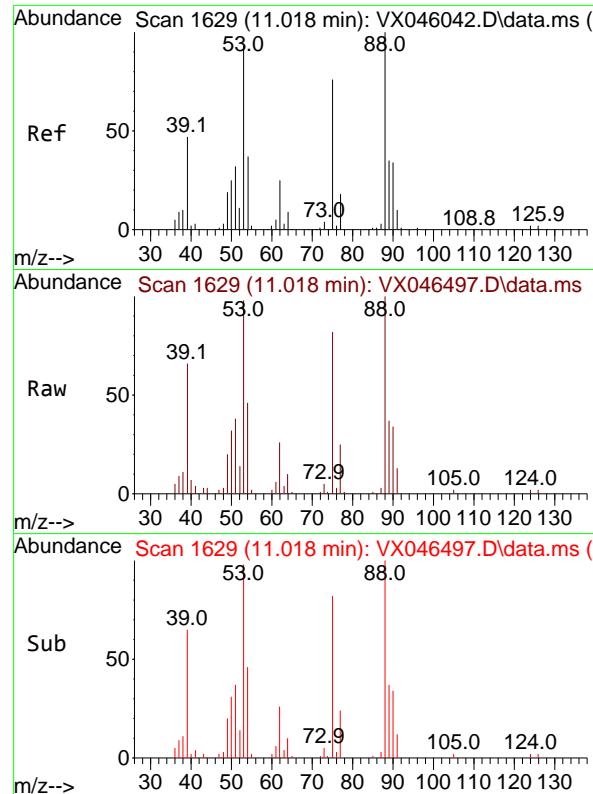


#81  
trans-1,4-Dichloro-2-butene  
Concen: 20.011 ug/l  
RT: 11.018 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


**Manual Integrations**  
**APPROVED**







Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

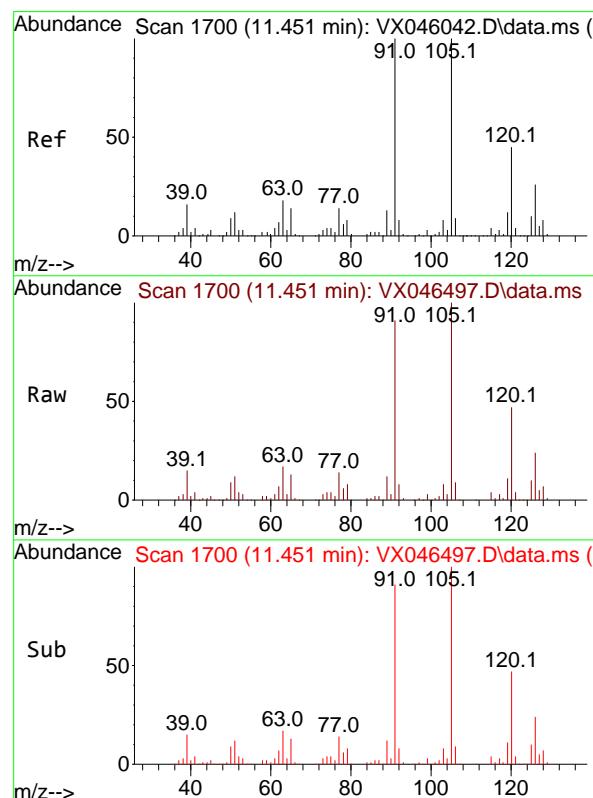

#82  
4-Chlorotoluene  
Concen: 21.826 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion: 91 Resp: 88804  
Ion Ratio Lower Upper  
91 100  
126 27.0 13.3 39.8





#83

tert-Butylbenzene

Concen: 22.483 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X


ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

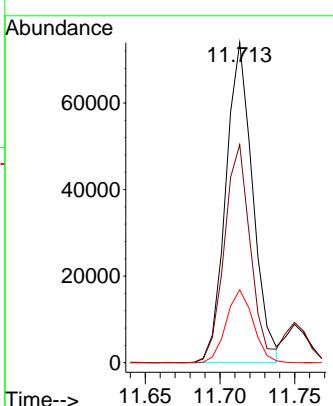

#84

1,2,4-Trimethylbenzene

Concen: 22.395 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52




Tgt Ion:105 Resp: 92688

Ion Ratio Lower Upper

105 100

120 41.7 21.2 63.6





#85

sec-Butylbenzene

Concen: 22.129 ug/l

RT: 11.890 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#86

p-Isopropyltoluene

Concen: 22.299 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion:119 Resp: 93040


Ion Ratio Lower Upper

119 100

134 24.9 12.5 37.5

91 27.6 13.8 41.4

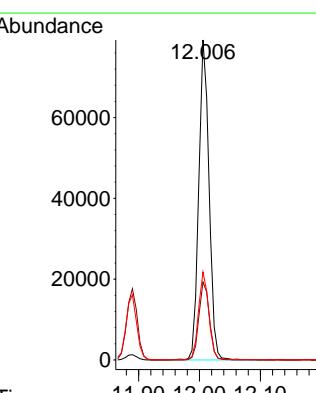

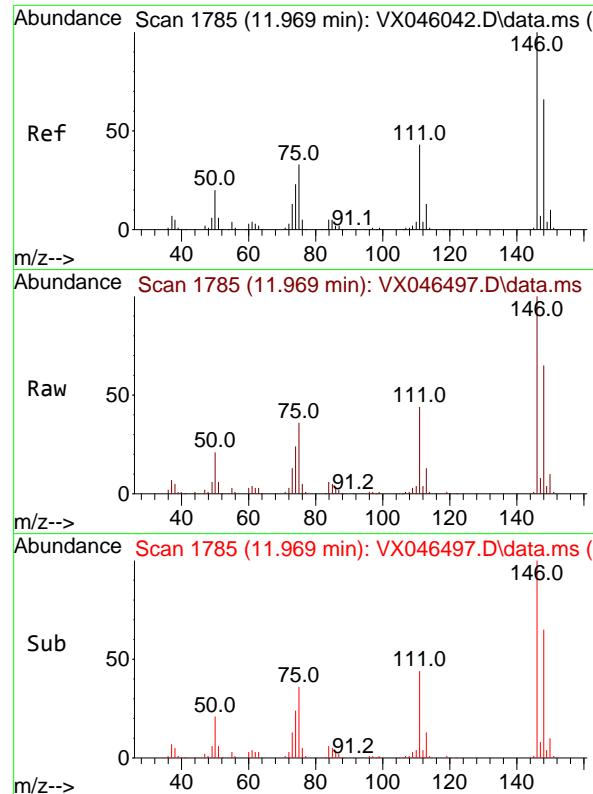

#87

1,3-Dichlorobenzene

Concen: 21.707 ug/l

RT: 11.969 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X



ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025

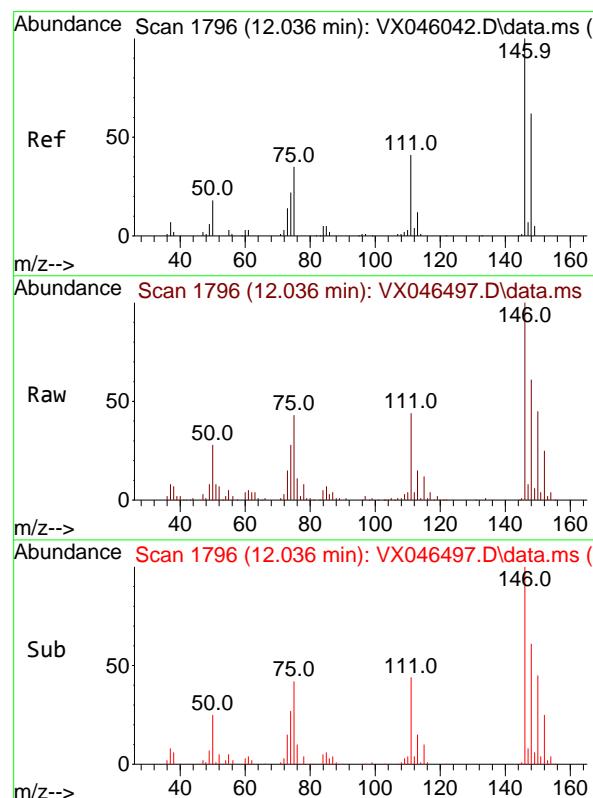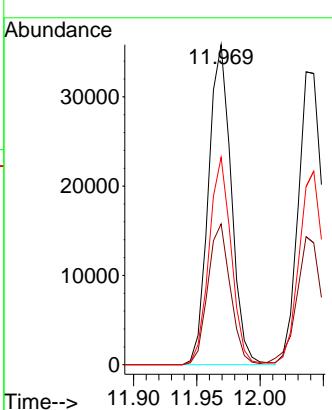

#88

1,4-Dichlorobenzene

Concen: 21.040 ug/l


RT: 12.036 min Scan# 1796




Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Tgt	Ion:146	Resp:	44540
Ion	Ratio	Lower	Upper
146	100		
111	44.0	21.3	63.9
148	64.9	31.9	95.5





#89

n-Butylbenzene

Concen: 21.729 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52




Instrument : MSVOA\_X

ClientSampleId : VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#90

Hexachloroethane

Concen: 21.457 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. -0.000 min

Lab File: VX046497.D


Acq: 04 Jun 2025 13:52




Tgt Ion:117 Resp: 15772

Ion Ratio Lower Upper

117 100

201 61.7 31.6 94.7

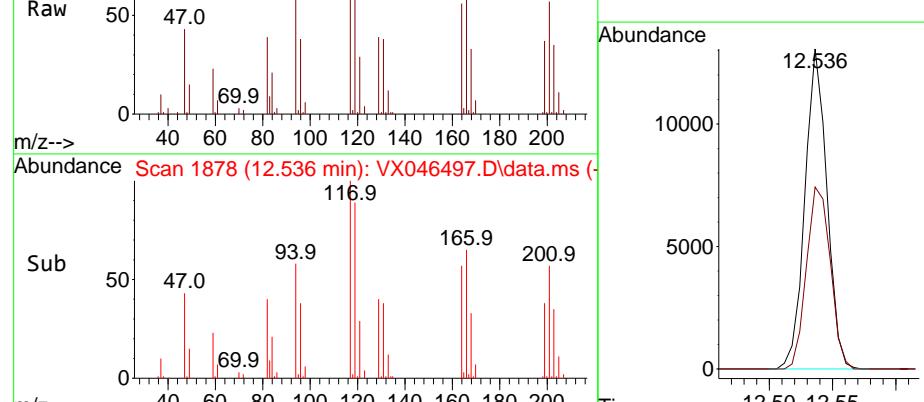



#91

1,2-Dichlorobenzene

Concen: 22.214 ug/l

RT: 12.335 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52

Instrument:

MSVOA\_X




ClientSampleId :

VX0604WBSD01

**Manual Integrations  
APPROVED**

Reviewed By :Mahesh Dadoda 06/05/2025

Supervised By :Semsettin Yesilyurt 06/05/2025



#92

1,2-Dibromo-3-Chloropropane

Concen: 23.821 ug/l

RT: 12.939 min Scan# 1944

Delta R.T. -0.000 min

Lab File: VX046497.D

Acq: 04 Jun 2025 13:52


Tgt Ion: 75 Resp: 9047


Ion Ratio Lower Upper

75 100

155 69.4 34.9 104.8

157 91.2 43.8 131.4




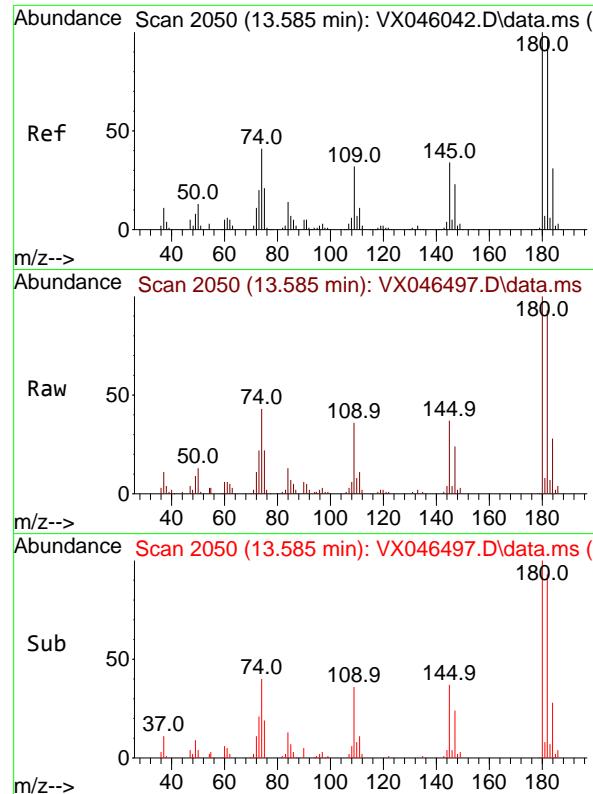


#93  
1,2,4-Trichlorobenzene  
Concen: 21.691 ug/l  
RT: 13.585 min Scan# 2050  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


### Manual Integrations APPROVED




Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

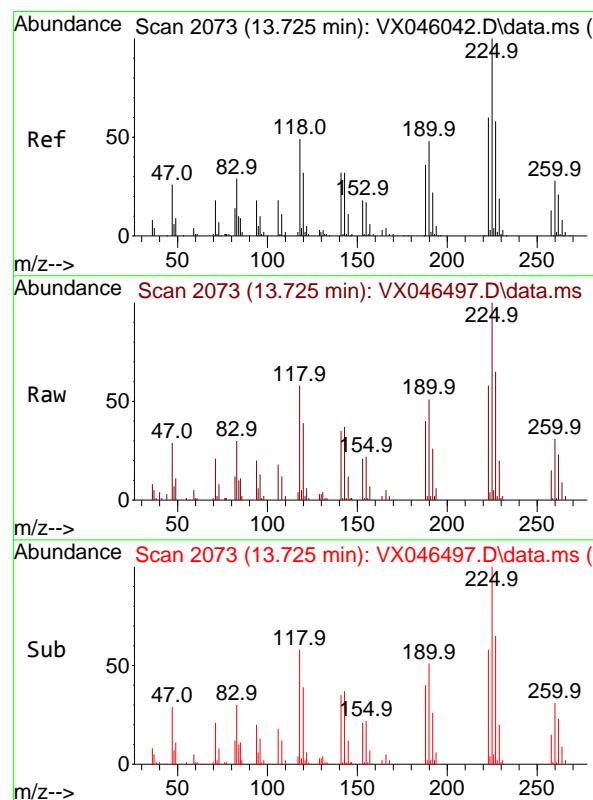

#94  
Hexachlorobutadiene  
Concen: 21.891 ug/l  
RT: 13.725 min Scan# 2073  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion:225 Resp: 11422  
Ion Ratio Lower Upper  
225 100  
223 61.4 30.8 92.4  
227 61.7 30.9 92.7




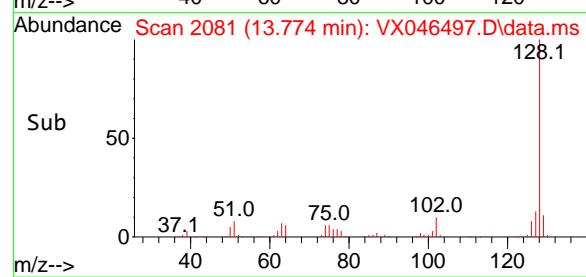
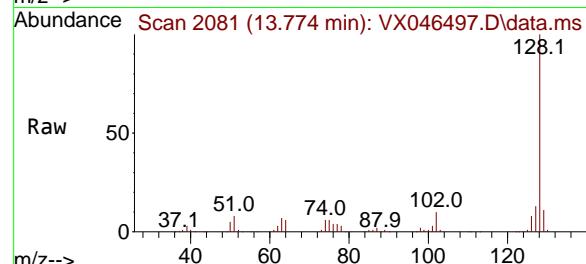
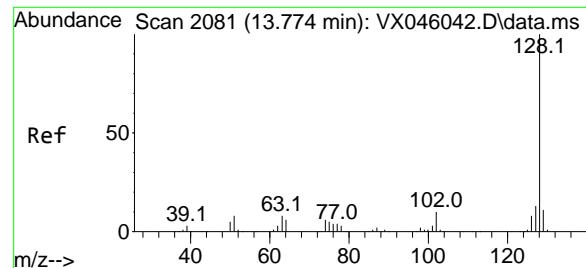


#95  
Naphthalene  
Concen: 23.449 ug/l  
RT: 13.774 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Instrument : MSVOA\_X  
ClientSampleId : VX0604WBSD01


### Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 06/05/2025  
Supervised By :Semsettin Yesilyurt 06/05/2025

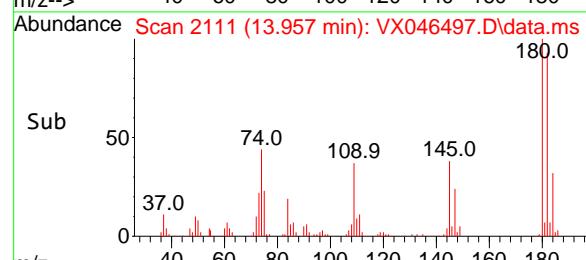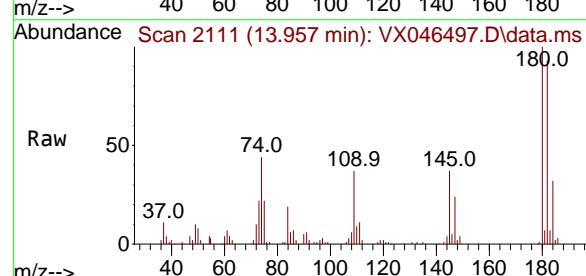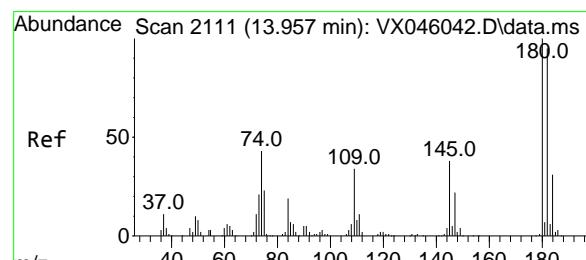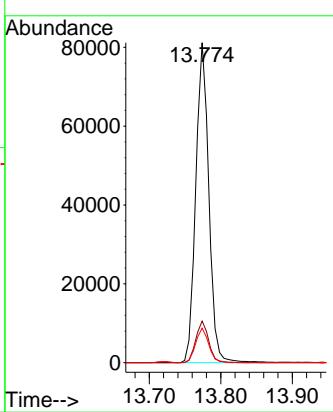

#96  
1,2,3-Trichlorobenzene  
Concen: 21.608 ug/l  
RT: 13.957 min Scan# 2111  
Delta R.T. -0.000 min  
Lab File: VX046497.D  
Acq: 04 Jun 2025 13:52

Tgt Ion:180 Resp: 26637  
Ion Ratio Lower Upper  
180 100  
182 94.6 47.8 143.3  
145 37.5 18.1 54.3



## Manual Integration Report

Sequence:	VX050525	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICC020	VX046041.D	1,2,3-Trichloropropane	JOHN	5/6/2025 9:53:13 AM	MMDadoda	5/6/2025 12:42:46 PM	Peak Integrated by Software
VSTDICCC050	VX046042.D	1,2,3-Trichloropropane	JOHN	5/6/2025 9:53:18 AM	MMDadoda	5/6/2025 12:42:48 PM	Peak Integrated by Software
VSTDICC100	VX046043.D	1,2,3-Trichloropropane	JOHN	5/6/2025 9:53:22 AM	MMDadoda	5/6/2025 12:42:50 PM	Peak Integrated by Software
VSTDICC150	VX046044.D	1,2,3-Trichloropropane	JOHN	5/6/2025 9:53:27 AM	MMDadoda	5/6/2025 12:42:53 PM	Peak Integrated by Software
VSTDICC005	VX046046.D	1,2,3-Trichloropropane	JOHN	5/6/2025 9:53:32 AM	MMDadoda	5/6/2025 12:42:56 PM	Peak Integrated by Software
VSTDICC005	VX046046.D	Ethyl Acetate	JOHN	5/6/2025 9:53:32 AM	MMDadoda	5/6/2025 12:42:56 PM	Peak Integrated by Software
VSTDICC001	VX046047.D	1,2,3-Trichloropropane	JOHN	5/6/2025 9:53:38 AM	MMDadoda	5/6/2025 12:41:35 PM	Peak Integrated by Software
VSTDICC001	VX046047.D	1,4-Dichlorobenzene	JOHN	5/6/2025 9:53:38 AM	MMDadoda	5/6/2025 12:41:35 PM	Peak Integrated by Software
VSTDICC001	VX046047.D	Bromochloromethane	JOHN	5/6/2025 9:53:38 AM	MMDadoda	5/6/2025 12:41:35 PM	Peak Integrated by Software
VSTDICC001	VX046047.D	Ethyl Acetate	JOHN	5/6/2025 9:53:38 AM	MMDadoda	5/6/2025 12:41:35 PM	Peak Integrated by Software
VSTDICC001	VX046047.D	Methyl methacrylate	JOHN	5/6/2025 9:53:38 AM	MMDadoda	5/6/2025 12:41:35 PM	Peak Integrated by Software
VSTDICV050	VX046048.D	1,2,3-Trichloropropane	JOHN	5/6/2025 9:53:45 AM	MMDadoda	5/6/2025 12:41:37 PM	Peak Integrated by Software

 1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

## Manual Integration Report

Sequence:	VX050525	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
-----------	---------	-----------	-----------	-----------	---------------	---------------	--------

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

### Manual Integration Report

Sequence:	VX060425	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VX046488.D	1,2,3-Trichloropropane	MMDadoda	6/5/2025 4:44:18 PM	SAM	6/5/2025 4:47:19 PM	Peak Integrated by Software
VSTDCCC050	VX046488.D	Methacrylonitrile	MMDadoda	6/5/2025 4:44:18 PM	SAM	6/5/2025 4:47:19 PM	Peak Integrated by Software
VX0604WBS01	VX046491.D	1,2,3-Trichloropropane	MMDadoda	6/5/2025 4:44:20 PM	SAM	6/5/2025 4:47:20 PM	Peak Integrated by Software
VX0604WBSD01	VX046497.D	1,2,3-Trichloropropane	MMDadoda	6/5/2025 4:44:23 PM	SAM	6/5/2025 4:47:24 PM	Peak Integrated by Software
VSTDCCC050	VX046515.D	1,2,3-Trichloropropane	SAM	6/5/2025 4:47:29 PM	MMdadoda	6/6/2025 1:00:26 AM	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX050525**

Review By	John Carbone	Review On	5/6/2025 9:53:58 AM
Supervise By	Mahesh Dadoda	Supervise On	5/6/2025 12:43:00 PM
SubDirectory	VX050525	HP Acquire Method	HP Processing Method 82X050525W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds  CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133811 VP133832,VP133833,VP133834,VP133835,VP133836,VP133837  VP133838		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX046038.D	05 May 2025 09:37	JC/MD	Ok
2	VSTDICCC001	VX046039.D	05 May 2025 10:49	JC/MD	Not Ok
3	VSTDICCC005	VX046040.D	05 May 2025 11:12	JC/MD	Not Ok
4	VSTDICCC020	VX046041.D	05 May 2025 11:35	JC/MD	Ok,M
5	VSTDICCC050	VX046042.D	05 May 2025 11:58	JC/MD	Ok,M
6	VSTDICCC100	VX046043.D	05 May 2025 12:21	JC/MD	Ok,M
7	VSTDICCC150	VX046044.D	05 May 2025 12:45	JC/MD	Ok,M
8	IBLK	VX046045.D	05 May 2025 13:08	JC/MD	Ok
9	VSTDICCC005	VX046046.D	05 May 2025 16:04	JC/MD	Ok,M
10	VSTDICCC001	VX046047.D	05 May 2025 16:27	JC/MD	Ok,M
11	VSTDICCV050	VX046048.D	05 May 2025 16:50	JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX060425**

Review By	Mahesh Dadoda	Review On	6/5/2025 4:44:40 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/5/2025 4:48:33 PM
SubDirectory	VX060425	HP Acquire Method	HP Processing Method 82X050525W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134124		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134125,VP134126		

Sr #	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX046487.D	04 Jun 2025 09:43	JC/MD	Ok
2	VSTDCCC050	VX046488.D	04 Jun 2025 10:12	JC/MD	Ok,M
3	VX0604MBL01	VX046489.D	04 Jun 2025 10:40	JC/MD	Ok
4	VX0604WBL01	VX046490.D	04 Jun 2025 11:04	JC/MD	Ok
5	VX0604WBS01	VX046491.D	04 Jun 2025 11:27	JC/MD	Ok,M
6	Q2169-03DL	VX046492.D	04 Jun 2025 11:55	JC/MD	Ok
7	Q2168-08DL	VX046493.D	04 Jun 2025 12:18	JC/MD	Ok
8	Q2168-12DL	VX046494.D	04 Jun 2025 12:41	JC/MD	Ok
9	Q2169-01	VX046495.D	04 Jun 2025 13:05	JC/MD	Dilution
10	Q2175-05	VX046496.D	04 Jun 2025 13:28	JC/MD	Ok
11	VX0604WBSD01	VX046497.D	04 Jun 2025 13:52	JC/MD	Ok,M
12	Q2200-01DL	VX046498.D	04 Jun 2025 14:15	JC/MD	Ok
13	Q2200-02	VX046499.D	04 Jun 2025 14:39	JC/MD	Ok
14	Q2200-05	VX046500.D	04 Jun 2025 15:02	JC/MD	Dilution
15	Q2175-06	VX046501.D	04 Jun 2025 15:26	JC/MD	Dilution
16	IBLK	VX046502.D	04 Jun 2025 15:50	JC/MD	Ok
17	IBLK	VX046503.D	04 Jun 2025 16:13	JC/MD	Ok
18	Q2200-03	VX046504.D	04 Jun 2025 16:37	JC/MD	Ok
19	Q2201-01	VX046505.D	04 Jun 2025 17:01	JC/MD	Ok
20	Q2198-05	VX046506.D	04 Jun 2025 17:25	JC/MD	ReRun
21	IBLK	VX046507.D	04 Jun 2025 17:49	JC/MD	Ok

Instrument ID: MSVOA\_X

**Daily Analysis Runlog For Sequence/QCBatch ID # VX060425**

Review By	Mahesh Dadoda	Review On	6/5/2025 4:44:40 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/5/2025 4:48:33 PM
SubDirectory	VX060425	HP Acquire Method	HP Processing Method 82X050525W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134124		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134125,VP134126		

22	Q2200-01	VX046508.D	04 Jun 2025 18:12	JC/MD	Dilution
23	Q2200-05DL	VX046509.D	04 Jun 2025 18:36	JC/MD	Ok
24	Q2200-06	VX046510.D	04 Jun 2025 19:00	JC/MD	Ok
25	Q2175-06DL	VX046511.D	04 Jun 2025 19:24	JC/MD	Ok,M
26	VX0604MBS01	VX046512.D	04 Jun 2025 19:47	JC/MD	Ok,M
27	Q2168-11ME	VX046513.D	04 Jun 2025 20:11	JC/MD	Dilution
28	Q2168-07ME	VX046514.D	04 Jun 2025 20:35	JC/MD	Ok
29	VSTDCCCC050	VX046515.D	04 Jun 2025 20:59	JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX050525

Review By	John Carlone	Review On	5/6/2025 9:53:58 AM
Supervise By	Mahesh Dadoda	Supervise On	5/6/2025 12:43:00 PM
SubDirectory	VX050525	HP Acquire Method	HP Processing Method 82X050525W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP133811		
Initial Calibration Stds	VP133832,VP133833,VP133834,VP133835,VP133836,VP133837		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133838		

Sr #	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX046038.D	05 May 2025 09:37		JC/MD	Ok
2	VSTDICCC001	VSTDICCC001	VX046039.D	05 May 2025 10:49	Not used	JC/MD	Not Ok
3	VSTDICCC005	VSTDICCC005	VX046040.D	05 May 2025 11:12	Not used	JC/MD	Not Ok
4	VSTDICCC020	VSTDICCC020	VX046041.D	05 May 2025 11:35		JC/MD	Ok,M
5	VSTDICCC050	VSTDICCC050	VX046042.D	05 May 2025 11:58		JC/MD	Ok,M
6	VSTDICCC100	VSTDICCC100	VX046043.D	05 May 2025 12:21		JC/MD	Ok,M
7	VSTDICCC150	VSTDICCC150	VX046044.D	05 May 2025 12:45		JC/MD	Ok,M
8	IBLK	IBLK	VX046045.D	05 May 2025 13:08		JC/MD	Ok
9	VSTDICCC005	VSTDICCC005	VX046046.D	05 May 2025 16:04		JC/MD	Ok,M
10	VSTDICCC001	VSTDICCC001	VX046047.D	05 May 2025 16:27		JC/MD	Ok,M
11	VSTDICCV050	ICVVX050525	VX046048.D	05 May 2025 16:50		JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX060425

Review By	Mahesh Dadoda	Review On	6/5/2025 4:44:40 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/5/2025 4:48:33 PM
SubDirectory	VX060425	HP Acquire Method	HP Processing Method 82X050525W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134124		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134125,VP134126		

Sr #	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX046487.D	04 Jun 2025 09:43		JC/MD	Ok
2	VSTDCCC050	VSTDCCC050	VX046488.D	04 Jun 2025 10:12	pH#Lot#V12668	JC/MD	Ok,M
3	VX0604MBL01	VX0604MBL01	VX046489.D	04 Jun 2025 10:40		JC/MD	Ok
4	VX0604WBL01	VX0604WBL01	VX046490.D	04 Jun 2025 11:04		JC/MD	Ok
5	VX0604WBS01	VX0604WBS01	VX046491.D	04 Jun 2025 11:27	BS failed low for comp. #17	JC/MD	Ok,M
6	Q2169-03DL	303-PPR-2DL	VX046492.D	04 Jun 2025 11:55	vial B pH<2	JC/MD	Ok
7	Q2168-08DL	B3DL	VX046493.D	04 Jun 2025 12:18	vial B pH#5.0	JC/MD	Ok
8	Q2168-12DL	C2DL	VX046494.D	04 Jun 2025 12:41	vial B pH#5.0	JC/MD	Ok
9	Q2169-01	303-PPR-1	VX046495.D	04 Jun 2025 13:05	vial B pH<2;Need 2X	JC/MD	Dilution
10	Q2175-05	52525-B	VX046496.D	04 Jun 2025 13:28	vial A pH<2 foamy sample	JC/MD	Ok
11	VX0604WBSD01	VX0604WBSD01	VX046497.D	04 Jun 2025 13:52		JC/MD	Ok,M
12	Q2200-01DL	RMW-02B-66-060325D	VX046498.D	04 Jun 2025 14:15		JC/MD	Ok
13	Q2200-02	RMW-03B-90-060325	VX046499.D	04 Jun 2025 14:39		JC/MD	Ok
14	Q2200-05	MW-11B-37.5-060325	VX046500.D	04 Jun 2025 15:02	Need 200X	JC/MD	Dilution
15	Q2175-06	EGR-LIQUID	VX046501.D	04 Jun 2025 15:26	Need 2000X	JC/MD	Dilution
16	IBLK	IBLK	VX046502.D	04 Jun 2025 15:50		JC/MD	Ok
17	IBLK	IBLK	VX046503.D	04 Jun 2025 16:13		JC/MD	Ok
18	Q2200-03	EB01-060325	VX046504.D	04 Jun 2025 16:37	EB	JC/MD	Ok

Instrument ID: MSVOA\_X

### Daily Analysis Runlog For Sequence/QCBatch ID # VX060425

Review By	Mahesh Dadoda	Review On	6/5/2025 4:44:40 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/5/2025 4:48:33 PM
SubDirectory	VX060425	HP Acquire Method	HP Processing Method 82X050525W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds  CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134124  VP134125,VP134126		

19	Q2201-01	MW-01-6.5-060225	VX046505.D	04 Jun 2025 17:01	vial A pH<2	JC/MD	Ok
20	Q2198-05	B-202-GW01	VX046506.D	04 Jun 2025 17:25	BS failed low for comp. #17	JC/MD	ReRun
21	IBLK	IBLK	VX046507.D	04 Jun 2025 17:49		JC/MD	Ok
22	Q2200-01	RMW-02B-66-060325	VX046508.D	04 Jun 2025 18:12	Need 100X	JC/MD	Dilution
23	Q2200-05DL	MW-11B-37.5-060325D	VX046509.D	04 Jun 2025 18:36		JC/MD	Ok
24	Q2200-06	TB-01-060325	VX046510.D	04 Jun 2025 19:00	TB	JC/MD	Ok
25	Q2175-06DL	EGR-LIQUIDDL	VX046511.D	04 Jun 2025 19:24		JC/MD	Ok,M
26	VX0604MBS01	VX0604MBS01	VX046512.D	04 Jun 2025 19:47		JC/MD	Ok,M
27	Q2168-11ME	C2ME	VX046513.D	04 Jun 2025 20:11	Need 10X	JC/MD	Dilution
28	Q2168-07ME	B3ME	VX046514.D	04 Jun 2025 20:35		JC/MD	Ok
29	VSTDCCC050	VSTDCCC050EC	VX046515.D	04 Jun 2025 20:59		JC/MD	Ok,M

M : Manual Integration

## Prep Standard - Chemical Standard Summary

**Order ID :** Q2200

**Test :** VOCMS Group3

**Prepbatch ID :**

**Sequence ID/Qc Batch ID:** VX060425,

**Standard ID :**

VP132035,VP132096,VP133174,VP133887,VP133935,VP133953,VP133991,VP134124,VP134125,VP134126,

**Chemical ID :**

V13391,V13457,V13460,V13465,V13466,V13706,V14290,V14432,V14435,V14503,V14504,V14525,V14526,V14613,V14614,V14620,V14626,V14630,V14631,V14632,V14633,V14711,V14717,V14718,V14721,V14749,V14750,V14811,V14812,V14843,V14921,V14944,V14945,V14946,V14947,W3112,

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1810	8260 Working Std(2-CVE)-800ppm	<a href="#">VP132035</a>	12/10/2024	06/10/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 12/12/2024

**FROM** 1.00000ml of V14630 + 1.00000ml of V14631 + 1.00000ml of V14632 + 1.00000ml of V14633 + 46.00000ml of V14614 = Final  
Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
719	8260 Working STD (BCM)-First source, 400PPM	<a href="#">VP132096</a>	12/12/2024	06/10/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 12/19/2024

**FROM** 1.00000ml of V13465 + 1.00000ml of V13466 + 1.50000ml of V13457 + 1.50000ml of V13460 + 20.00000ml of V14614 = Final  
Quantity: 25.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
617	8260 Surrogate, 400PPM	<a href="#">VP133174</a>	02/27/2025	08/27/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 03/04/2025

FROM 0.40000ml of V13706 + 24.60000ml of V14613 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
257	8260 Calibration Working STD Mix-First source, 160PPM	<a href="#">VP133887</a>	05/12/2025	06/23/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 05/14/2025

FROM 0.40000ml of V14843 + 1.00000ml of V14432 + 1.00000ml of V14435 + 1.00000ml of V14503 + 1.00000ml of V14504 + 1.00000ml of V14525 + 1.00000ml of V14526 + 1.00000ml of V14711 + 1.00000ml of V14717 + 1.00000ml of V14718 + 1.00000ml of V14721 + 1.00000ml of V14749 + 1.00000ml of V14750 + 1.00000ml of V14811 + 1.00000ml of V14812 + 10.60000ml of V14921 = Final Quantity: 25.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
247	8260 Internal Standard, 250PPM	<a href="#">VP133935</a>	05/16/2025	11/12/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 05/21/2025

FROM 0.25000ml of V14290 + 24.75000ml of V14921 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
218	BFB, 25PPM	<a href="#">VP133953</a>	05/19/2025	11/09/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 05/21/2025

FROM 0.25000ml of V13391 + 24.75000ml of V14626 = Final Quantity: 25.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
51	8260 Working STD (Acrolein) -first source, 800PPM	<a href="#">VP133991</a>	05/22/2025	06/19/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 05/24/2025

FROM 1.00000ml of V14944 + 1.00000ml of V14945 + 1.00000ml of V14946 + 1.00000ml of V14947 + 21.00000ml of V14620 = Final  
Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
589	BFB TUNE CHECK	<a href="#">VP134124</a>	06/04/2025	06/05/2025	John Carlone	None	None	Mahesh Dadoda 06/06/2025

FROM 39.98400ml of W3112 + 0.01600ml of VP133953 = Final Quantity: 40.000 ml

## VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	<a href="#">VP134125</a>	06/04/2025	06/05/2025	John Carlone	None	None	Mahesh Dadoda 06/06/2025

FROM 39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP133935 + 0.01250ml of VP132035 + 0.01250ml of VP133887 + 0.01250ml of VP133991 = Final Quantity: 40.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	<a href="#">VP134126</a>	06/04/2025	06/05/2025	John Carlone	None	None	Mahesh Dadoda 06/06/2025

FROM 39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP133935 + 0.01250ml of VP132035 + 0.01250ml of VP133887 + 0.01250ml of VP133991 = Final Quantity: 40.000 ml

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30067 / BFB tuneing solution	A0191805	11/22/2025	11/22/2024 / SAM	01/13/2023 / SAM	V13391
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13457
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13460
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13465
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13466
Restek	555582 / Custom Mixture, 8260 A/B Surrogate Mix [CS 5179-2]	A0196865	02/27/2026	02/27/2025 / SAM	04/12/2023 / SAM	V13706

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555581 / Custom Standard, 8260 Internal Std [CS 5179-1]	A0210184	12/12/2025	12/12/2024 / SAM	04/15/2024 / SAM	V14290
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	09/30/2025	05/12/2025 / SAM	08/15/2024 / SAM	V14432
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	09/20/2025	03/20/2025 / SAM	08/15/2024 / SAM	V14435
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	11/12/2025	05/12/2025 / SAM	09/17/2024 / SAM	V14503
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	11/12/2025	05/12/2025 / SAM	09/17/2024 / SAM	V14504
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	11/12/2025	05/12/2025 / SAM	09/18/2024 / SAM	V14525

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	11/12/2025	05/12/2025 / SAM	09/18/2024 / SAM	V14526
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	08/27/2025	02/27/2025 / SAM	11/26/2024 / SAM	V14613
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	06/10/2025	12/10/2024 / SAM	11/26/2024 / SAM	V14614
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	10/25/2025	05/09/2025 / SAM	11/26/2024 / SAM	V14620
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	23I0762004	11/09/2025	05/09/2025 / SAM	11/26/2024 / SAM	V14626
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14630

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14631
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14632
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14633
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14711
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14717
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14718

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14721
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	11/13/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14749
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14750
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE	A0220471	11/12/2025	05/12/2025 / SAM	01/08/2025 / SAM	V14811
LOTS						
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE	A0220471	06/30/2026	05/12/2025 / SAM	01/08/2025 / SAM	V14812
LOTS						
Restek	30470 / VOA Stock Solution, tert-butanol std, 1mL, P&TM	A0217535	11/12/2025	05/12/2025 / SAM	01/21/2025 / SAM	V14843

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	24G0262002	11/12/2025	05/12/2025 / SAM	05/09/2025 / SAM	V14921
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14944
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14945
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14946
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14947
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis



Material No.: 9077-02  
Batch No.: 23I0762004  
Manufactured Date: 2023-08-11  
Expiration Date: 2026-08-10  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.5 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.01
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Ken Koehnlein  
Sr. Manager, Quality Assurance

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis

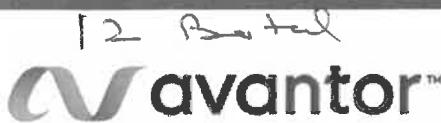

Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier  
Vice President Global Quality

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis

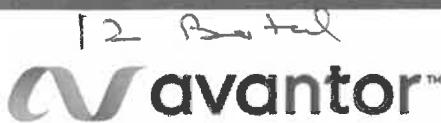

Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier  
Vice President Global Quality

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis

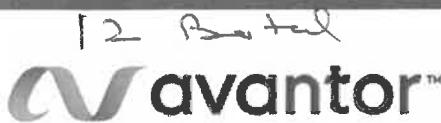

Material No.: 9077-02  
Batch No.: 22L0562016  
Manufactured Date: 2022-10-26  
Expiration Date: 2025-10-25  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier  
Vice President Global Quality

Ree 09/17/24

## CERTIFIED WEIGHT REPORT

Part Number: 95317  
 Lot Number: 021624  
 Description: Universal VOA Megamix  
 69 components

Solvent(s): Lot#  
 Methanol EG359-USQ12

Expiration Date: 02/2027  
 Recommended Storage: Freeze (0 °C)

Nominal Concentration (ug/mL): 2000NIST Test ID#: 8UTBWeight(s) shown below were combined and diluted to (mL): 100.0 0.021 Flask Uncertainty

5E-05 Balance Uncertainty

Compound	(RM#)	Lot Number	Dil. Factor	Initial Vol. (mL)	Initial Conc. (ug/mL)	Nominal Conc. (ug/mL)	Purity (%)	Purity Uncertainty	Uncertainty Pipette (mL)	Target Weight(g)	Actual Weight(g)	Actual Conc. (ug/mL)	Actual (+/-) (ug/mL)	SDS Information		
														CAS#	OSHA PEL (TWA)	LD50
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m <sup>3</sup> /BH)	orl-rat 2400mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102398	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m <sup>3</sup> /BH)	orl-rat 700mg/kg
3. Carbon disulfide	(0060)	MKCR8581	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.8	8.1	75-15-0	4 ppm (12mg/m <sup>3</sup> ) (skin)	orl-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1198)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21058	0.21069	2001.1	8.5	1478-11-6	N/A	N/A
5. trans-1,4-Dichloro-2-butene	(0486)	MKBPE041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20748	2001.7	8.4	110-57-6	N/A	N/A
6. Diethyl ether	(0153)	K18CA500K	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	N/A	N/A
7. Ethyl methacrylate	(0381)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	N/A	orl-rat 14800mg/kg
8. Iodomethane	(0489)	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20121	2001.5	8.2	74-88-4	5 ppm (28mg/m <sup>3</sup> /BH) (skin)	orl-rat 76mg/kg
9. 2-Methyl-1-propanol	(0445)	18241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m <sup>3</sup> /BH)	orl-rat 240mg/kg
10. Methylacrylonitrile	(0442)	0042ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	126-98-7	1 ppm (3mg/m <sup>3</sup> /BH) (skin)	orl-rat 120mg/kg
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm (35mg/m <sup>3</sup> /BH) (skin)	orl-rat 277mg/kg
12. Methyl methacrylate	(0404)	MKBW5137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-82-6	100 ppm (410mg/m <sup>3</sup> /BH)	orl-rat 787mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-85-3	1 ppm (3mg/m <sup>3</sup> /BH) (skin)	orl-rat 780mg/kg
14. 2-Nitropropane	(0481)	14002JK	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	79-48-9	10 ppm (35mg/m <sup>3</sup> /BH)	orl-rat 720mg/kg
15. Pentachloroethane	(0450)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	N/A	N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18590	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1	1000 ppm (7600mg/m <sup>3</sup> /BH)	orl-rat 45mg/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1988.6	22.8	75-27-4	N/A	orl-rat 916mg/kg
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	N/A	orl-rat 848mg/kg
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	N/A	N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	N/A	orl-rat 1235mg/kg
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.5	22.9	75-09-2	500 ppm	orl-rat 820mg/kg
22. 1,1-Dichloroethene	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m <sup>3</sup> /BH)	orl-rat 200mg/kg
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	0.5 ppm (5mg/m <sup>3</sup> ) (skin)	orl-rat 933mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	2 ppm (12.8mg/m <sup>3</sup> /BH)	orl-rat 2350mg/kg
25. Chloroform	95321	020724	0.10	10.00	20024.0	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	1 ppm (4mg/m <sup>3</sup> /BH)	orl-rat 908mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	2001.9	20.5	67-88-3	60 ppm (240mg/m <sup>3</sup> ) (CL)	orl-rat 908mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-85-3	N/A	orl-rat 108mg/kg
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	2002.0	22.9	75-34-3	100 ppm	orl-rat 725mg/kg
29. Tetrachloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	1999.8	20.4	59-20-7	N/A	N/A
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	2018.9	20.8	127-18-4	25 ppm (170mg/m <sup>3</sup> /BH)(final)	orl-rat 2620mg/kg
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40018.5	2000	NA	NA	0.017	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m <sup>3</sup> /BH)	orl-rat 10300mg/kg
32. 1,2-Dibromopentane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.3	22.9	98-12-8	0.001 ppm	orl-rat 170mg/kg
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-03-4	20 ppm (BH)	orl-rat 108mg/kg
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (BH)	orl-rat 670mg/kg
35. 1,2-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5	75 ppm (350mg/m <sup>3</sup> /BH)	orl-rat 1847mg/kg
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-29-9	N/A	im-mus 3600mg/kg
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.1	28.7	583-58-6	N/A	N/A
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10081-01-5	N/A	N/A
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.4	23.0	10061-02-6	N/A	N/A
40. 1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-08-3	0.02 ppm (0.24mg/m <sup>3</sup> /BH)	orl-rat 82mg/kg
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	N/A	orl-rat 670mg/kg
42. 1,1,2-Tetrafluoroethane	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.9	22.9	78-34-5	5 ppm (55mg/m <sup>3</sup> /BH) (skin)	orl-rat 600mg/kg
43. Trichloroethene	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	1999.8	23.0	78-00-5	10 ppm (45mg/m <sup>3</sup> /BH) (skin)	orl-rat 836mg/kg
44. 1,2,2-Trichloropropane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.9	22.9	78-01-6	50 ppm (270mg/m <sup>3</sup> /BH)	orl-mus 240mg/kg
45. Benzene	35162	050823	0.05	5.00	40005.0	2000	NA	NA	0.017	NA	NA	1999.9	22.9	98-18-4	10 ppm (60mg/m <sup>3</sup> /BH)	orl-rat 149.8mg/kg
46. Bromobenzene	35162	050823	0.05	5.00	40006.9	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm	orl-rat 480mg/kg
47. n-Butyl benzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-1	N/A	orl-rat 269mg/kg
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8	N/A	N/A
49. p-Isopropyl tolue	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m <sup>3</sup> /BH)	orl-rat >2000mg/kg
50. Naphthalene	35162	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	99-57-6	N/A	orl-rat 475mg/kg
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m <sup>3</sup> /BH)	orl-rat 490mg/kg
52. Toluene	35162	050823	0.05	5.00	40008.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm	orl-rat 5000mg/kg
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-3	200 ppm	orl-rat 5000mg/kg
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m <sup>3</sup> )	orl-rat 756mg/kg
55. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.6	23.0	95-63-6	N/A	orl-rat 5g/kg
56. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-67-8	N/A	orl-rat 5000mg/kg
57. <i>t</i> -Butyl benzene	35163	101923	0.05	5.00												



Run 16, "P95317 L021624 [2000µg/mL in MeOH]"

Run Length: 60.00 min, 35998 points at 10 points/second.

Created: Sat, Feb 17, 2024 at 8:56:46 AM.

Sampled: Sequence "021624-GC5M1", Method "GC5-M1".

Analyzed using Method "GC5-M1".

#### Comments

GC5-M1 Analysis by Candice Warren

Column ID SPB-Vocol 105 meter X 0.53mm X 3.0µm film thickness

Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,


Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.

Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.).

Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.

FID Signal = Edaq Channel 1

Standard injection = 0.5µL, Range=3

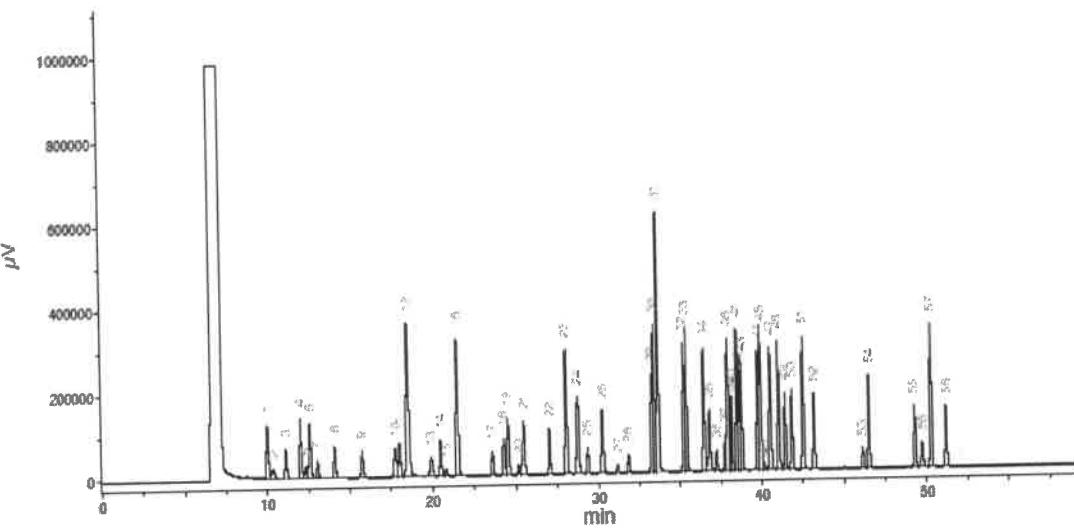

Peak #	Name	FID RT (min.)
1	Ether	0.97
2	1,1,2-Trichloro-1,2,3-trifluoropropane	10.33
3	1,1-Dichloroethane	11.10
4	Acetonitrile	12.00
5	Iodomethane	12.21
6	Allyl chloride	12.56
7	Carbon disulfide/Methylene chloride	13.74
8	trans-1,2-Dichloroethane	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,3-Dichloropropene	18.60
12	Methyl vinyl ketone/Methyl acrylate/Chloroform	18.49
13	Isobutanol/1,1,1-Trichloroethane	19.91
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethane	23.68
18	1,2-Dichloropropane	24.26
19	Methyl methacrylate	24.52
20	Bromoacetylbenzene	25.13
21	Dibromoethane/1,2-Dibromoethane	25.48
22	cis-1,3-Dichloropropene	27.07
23	Toluene	28.03
24	Ethyl methacrylate/trans-1,3-Dichloropropene	29.73
25	1,1,2-Trichloroethane	29.94
26	Toluene/butanone/1,2-Dichloropropane	30.84
27	Dibromochloromethane	31.16
28	1,2-Dibromoethane	31.89
29	Chlorobutane	33.20
30	Ethyleneglycerol,1,3,2-Tetrahydroethane	33.60
31	m-Xylene/p-Xylene	33.89
32	o-Xylene	33.93
33	Glyrene	35.94
34	Isopropylbenzene/Bromoform	36.48
35	cis-1,4-Dichloro-1-butene	36.60
36	1,1,2,2-Tetrachloroethane	37.23
37	j,2,3-Trichloropropene	37.77
38	n-Propylbenzene	37.92
39	trans-1,3-Dichloro-3-butene	38.05
40	Bromobenzene	38.14
41	1,3,5-Trimethylbenzene	38.50
42	2-Chlorotoluene	38.63
43	4-Chlorotoluene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	40.91
46	Pentachloroethane	40.17
47	tert-Butylbenzene	40.53
48	p Isopropyltoluene	41.03
49	1,3-Dichloropropane	41.13
50	1,4-Dichlorobenzene	41.83
51	n-Butylbenzene	42.62
52	1,2-Dichlorobenzene	42.16
53	1,2-Dibromo-3-chloropropane	46.17
54	Nitrobenzene	46.49
55	1,3,4-Trimethoxybenzene	49.26
56	Hexachlorobutadiene	49.32
57	Naphthalene	50.16
58	1,2,3-Trichlorobenzene	51.16



Boiling Point	65°C	Specific Gravity (H <sub>2</sub> O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US)  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

Ree 09/17/24

## CERTIFIED WEIGHT REPORT

Part Number: 95317  
 Lot Number: 021624  
 Description: Universal VOA Megamix  
 69 components

Solvent(s): Lot#  
 Methanol EG359-USQ12

Expiration Date: 02/16/27  
 Recommended Storage: Freeze (0 °C)

Nominal Concentration (ug/mL): 2000NIST Test ID#: 8UTBWeight(s) shown below were combined and diluted to (mL): 100.0 0.021 Flask Uncertainty

5E-05 Balance Uncertainty

Compound	(RM#)	Lot Number	Dil. Factor	Initial Vol. (mL)	Initial Conc. (ug/mL)	Nominal Conc. (ug/mL)	Purity (%)	Purity Uncertainty	Uncertainty Pipette (mL)	Target Weight(g)	Actual Weight(g)	Actual Conc. (ug/mL)	Actual Conc. (ug/mL) (+/-) (ug/mL)	Expanded Uncertainty	SDS Information
	Part Number											CAS#	OSHA PEL (TWA)	LD50	
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m <sup>3</sup> /BH) orl-rat 2400mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102398	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m <sup>3</sup> /BH) orl-rat 700mg/kg
3. Carbon disulfide	(0600)	MKCR8581	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.8	8.1	75-15-0	4 ppm (12mg/m <sup>3</sup> ) (skin) orl-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1198)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21058	0.21069	2001.1	8.5	1478-11-6	N/A
5. trans-1,4-Dichloro-2-butene	(0486)	MKBP6041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20748	2001.7	8.4	110-57-6	N/A
6. Diethyl ether	(0153)	K18CA5000K	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	N/A
7. Ethyl methacrylate	(0381)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	N/A
8. Iodomethane	(0489)	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20121	2001.5	8.2	74-88-4	5 ppm (28mg/m <sup>3</sup> /BH) (skin) orl-rat 14800mg/kg
9. 2-Methyl-1-propanol	(0445)	18241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20108	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m <sup>3</sup> /BH) orl-rat 240mg/kg
10. Methylacrylonitrile	(0442)	0042ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	126-98-7	1 ppm (3mg/m <sup>3</sup> /BH) (skin) orl-rat 120mg/kg
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm (35mg/m <sup>3</sup> /BH) (skin) orl-rat 277mg/kg
12. Methyl methacrylate	(0404)	MKBW6137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-82-6	100 ppm (410mg/m <sup>3</sup> /BH) orl-rat 787mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-85-3	1 ppm (5mg/m <sup>3</sup> /BH) (skin) orl-rat 780mg/kg
14. 2-Nitropropane	(0481)	14002JK	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	79-48-9	10 ppm (35mg/m <sup>3</sup> /BH) orl-rat 720mg/kg
15. Pentachloroethane	(0450)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18590	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1	1000 ppm (7600mg/m <sup>3</sup> /BH) orl-rat 45mg/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1988.6	22.8	75-27-4	N/A
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	N/A
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	N/A
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2	500 ppm orl-rat 820mg/kg
22. 1,1-Dichloroethene	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m <sup>3</sup> /BH) orl-rat 200mg/kg
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	0.5 ppm (5mg/m <sup>3</sup> ) (skin) orl-rat 933mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	2 ppm (12.8mg/m <sup>3</sup> /BH) orl-rat 235mg/kg
25. Chloroform	95321	020724	0.10	10.00	20024.0	2000	NA	NA	0.042	NA	NA	1999.8	20.4	67-83-3	60 ppm (240mg/m <sup>3</sup> ) (CL) orl-rat 90mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	2001.9	20.5	77-08-3	100 ppm (410mg/m <sup>3</sup> /BH) orl-rat 200mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-85-3	N/A
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	57-34-3	100 ppm orl-rat 725mg/kg
29. Tetrachloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	1999.8	20.4	59-20-7	N/A
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	1999.8	20.8	127-18-4	25 ppm (170mg/m <sup>3</sup> /BH)(final) orl-rat 262mg/kg
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40018.5	2000	NA	NA	0.017	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m <sup>3</sup> /BH) orl-rat 10300mg/kg
32. 1,2-Dibromopentane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.3	22.9	98-12-8	0.001 ppm orl-rat 170mg/kg
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-03-4	20 ppm (BH) orl-rat 108mg/kg
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (BH) orl-rat 670mg/kg
35. 1,2-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5	75 ppm (350mg/m <sup>3</sup> /BH) orl-rat 1847mg/kg
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-29-9	N/A orl-mus 3600mg/kg
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.1	28.7	583-56-6	N/A
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10081-01-5	N/A
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.4	23.0	106-01-2	N/A
40. 1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-08-3	0.02 ppm (0.24mg/m <sup>3</sup> /BH) orl-rat 82mg/kg
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	N/A orl-rat 670mg/kg
42. 1,1,2-Tetrafluoroethane	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.9	22.9	78-34-5	5 ppm (55mg/m <sup>3</sup> /BH) (skin) orl-rat 600mg/kg
43. Trichloroethene	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	1999.8	23.0	78-00-5	10 ppm (45mg/m <sup>3</sup> /BH) (skin) orl-rat 833mg/kg
44. 1,2,2-Trichloropropane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	2000.9	22.9	78-01-6	50 ppm (270mg/m <sup>3</sup> /BH) orl-mus 240mg/kg
45. Benzene	35162	050823	0.05	5.00	40005.0	2000	NA	NA	0.017	NA	NA	1999.9	22.9	98-18-4	10 ppm (60mg/m <sup>3</sup> /BH) orl-rat 149.8mg/kg
46. Bromobenzene	35162	050823	0.05	5.00	40006.9	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm orl-rat 480mg/kg
47. n-Butyl benzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-1	N/A orl-rat 269mg/kg
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8	N/A
49. p-Isopropyl tolue	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m <sup>3</sup> /BH) orl-rat >2000mg/kg
50. Naphthalene	35162	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	99-57-6	N/A orl-rat 475mg/kg
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m <sup>3</sup> /BH) orl-rat 490mg/kg
52. Toluene	35162	050823	0.05	5.00	40008.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm orl-rat 5000mg/kg
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	108-88-3	200 ppm orl-rat 5000mg/kg
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m <sup>3</sup> ) orl-rat 756mg/kg
55. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.6	23.0	95-63-6	N/A orl-rat 5g/kg
56. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-67-8	N/A orl-rat 5000mg/kg
57. <i>t</i> -Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3	100 ppm (435mg/m <sup>3</sup> /BH) orl-rat 5g/kg
58. <i>sec</i> -Butyl benzene	35163	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.8	22.9	98-06-6	N/A orl-rat 5g/kg
59. <i>tert</i> -Butyl benzene	35163	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	135-98-8	N/A orl-rat 2240mg/kg
60. Chlorobenzene	35163	101923	0.05	5.00											



Run 16, "P95317 L021624 [2000µg/mL in MeOH]"

Run Length: 60.00 min, 35998 points at 10 points/second.

Created: Sat, Feb 17, 2024 at 8:56:46 AM.

Sampled: Sequence "021624-GC5M1", Method "GC5-M1".

Analyzed using Method "GC5-M1".

#### Comments

GC5-M1 Analysis by Candice Warren

Column ID SPB-Vocel 105 meter X 0.53mm X 3.0µm film thickness

Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,


Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.

Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.).

Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.

FID Signal = Edaq Channel 1

Standard injection = 0.5µL, Range=3

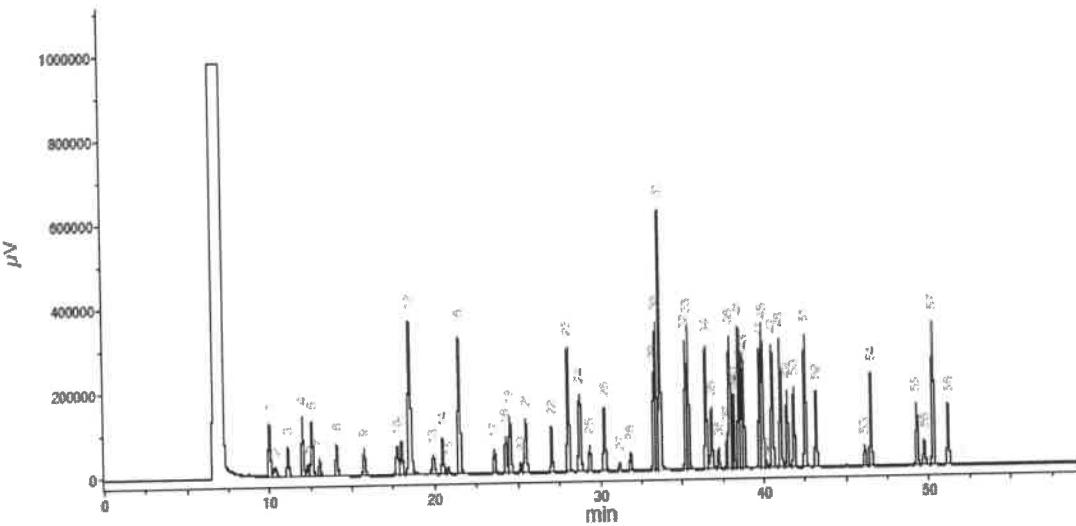

Peak #	Name	FID RT (min.)
1	Ether	0.97
2	1,1,2-Trichloro-1,2,3-trifluoropropane	10.33
3	1,1-Dichloroethane	11.10
4	Acetonitrile	12.00
5	Iodomethane	12.21
6	Allyl chloride	12.56
7	Carbon disulfide/Methylene chloride	13.74
8	trans-1,2-Dichloroethane	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,3-Dichloropropene	18.60
12	Methylacrylonitrile/Methyl acrylate/Chloroform	18.49
13	Isobutanol/1,1,1-Trichloropropane	19.91
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethane	23.68
18	1,2-Dichloropropane	24.26
19	Methyl methacrylate	24.52
20	Bromoacetylbenzene	25.13
21	Dibromoethane/1,2-Dibromoethane	25.48
22	cis-1,3-Dichloropropene	27.07
23	Toluene	28.03
24	Ethyl methacrylate/trans-1,3-Dichloropropene	29.73
25	1,1,2-Trichloroethane	29.94
26	Tetrahydroanthracene/1,2-Dichloroethane	30.84
27	Dibromochloromethane	31.16
28	1,2-Dibromoethane	31.89
29	Chlorobutane	33.20
30	Ethylobenzene/1,1,2-Tetradecadiene	33.60
31	m-Xylene/p-Xylene	33.89
32	o-Xylene	33.93
33	Glyrene	35.94
34	Isopropylbenzene/Bromoform	36.46
35	cis-1,4-Dichloro-1-butene	36.60
36	1,1,2,2-Tetrachloroethane	37.23
37	j,2,3-Trichloropropene	37.77
38	n-Propylbenzene	37.92
39	trans-1,3-Dichloro-3-butene	38.05
40	Bromobenzene	38.14
41	1,3,5-Trimethylbenzene	38.50
42	2-Chlorotoluene	38.63
43	4-Chlorotoluene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	40.91
46	Pentachloroethane	40.17
47	tert-Butylbenzene	40.53
48	p Isopropyltoluene	41.03
49	1,3-Dichloropropane	41.13
50	1,4-Dichlorobenzene	41.83
51	n-Butylbenzene	42.62
52	1,2-Dichlorobenzene	42.16
53	1,2-Dibromo-3-chloropropane	46.17
54	Nitrobenzene	46.49
55	1,3,4-Trimethoxybenzene	49.26
56	Hexachlorobutadiene	49.32
57	Naphthalene	50.16
58	1,2,3-Trichlorobenzene	51.16



Boiling Point	65°C	Specific Gravity (H <sub>2</sub> O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



## Certified Reference Material CRM

Dec 09/17/24

2 Uvof

ANAB ISO 17034 Accredited  
AR-1539 Certificate Num:  
<https://Absolutestandards.co...>


## CERTIFIED WEIGHT REPORT

Part Number:	<u>91980</u>	Solvent(s):	Lot#
Lot Number:	<u>091424</u>	Water	072324Q
Description:	Acrolein		
Expiration Date:	101424		
Recommended Storage:	Refrigerate (4 °C)		
Nominal Concentration (µg/mL):	5000		
NIST Test ID#:	6UTB	5E-05 Balance Uncertainty	
Weight(s) shown below were combined and diluted to (mL):	10.0	0.001 Flask Uncertainty	

	091424
Formulated By: Justin Dippold	DATE
	091424
Reviewed By: Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
				(%)	Purity	Weight(g)	Conc (µg/mL)	(+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5µm film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.). **Rate** = 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

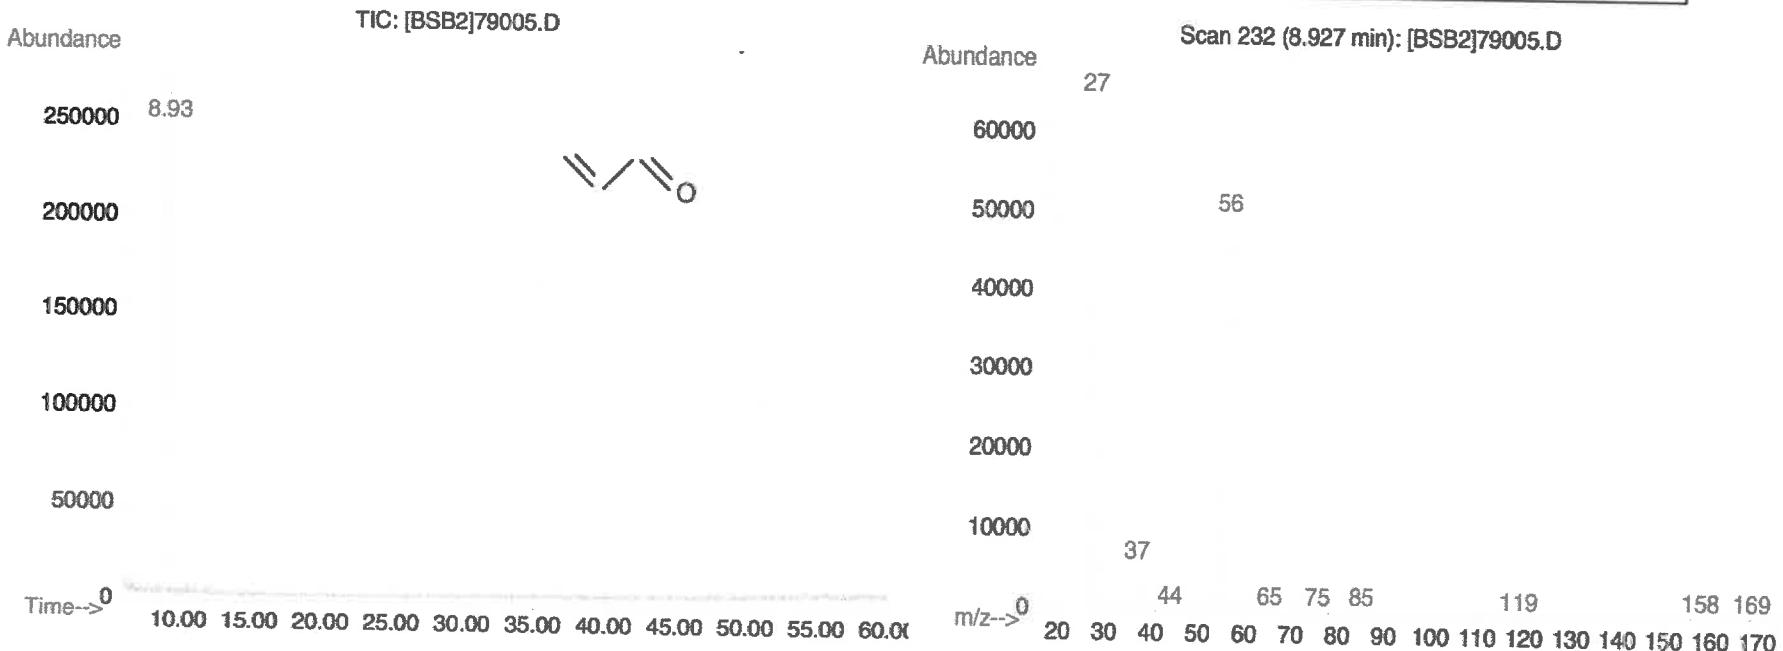

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



## Certified Reference Material CRM

Dec 09/17/24

2 Uvof

ANAB ISO 17034 Accredited  
AR-1539 Certificate Num:  
<https://Absolutestandards.co...>


## CERTIFIED WEIGHT REPORT

Part Number:	<u>91980</u>	Solvent(s):	Lot#
Lot Number:	<u>091424</u>	Water	072324Q
Description:	Acrolein		
Expiration Date:	101424		
Recommended Storage:	Refrigerate (4 °C)		
Nominal Concentration (µg/mL):	5000		
NIST Test ID#:	6UTB	5E-05 Balance Uncertainty	
Weight(s) shown below were combined and diluted to (mL):	10.0	0.001 Flask Uncertainty	

	091424
Formulated By: Justin Dippold	DATE
	091424
Reviewed By: Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
				(%)	Purity	Weight(g)	Conc (µg/mL)	(+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5µm film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.). **Rate** = 4°C/min., **Injector Temp.** = 200°C, **Detector Temp.** = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

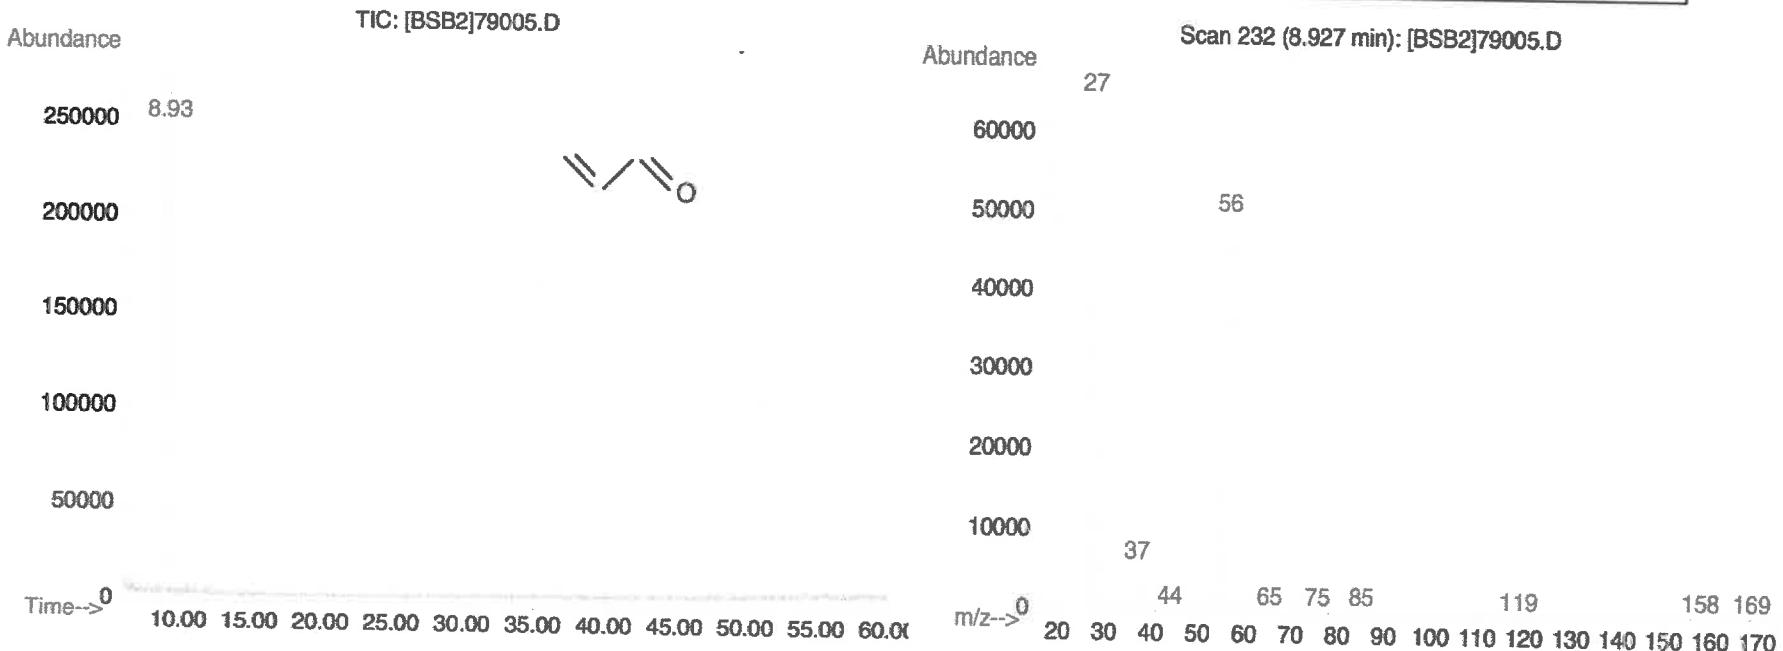

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




✓ 14630 to  
✓ 14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

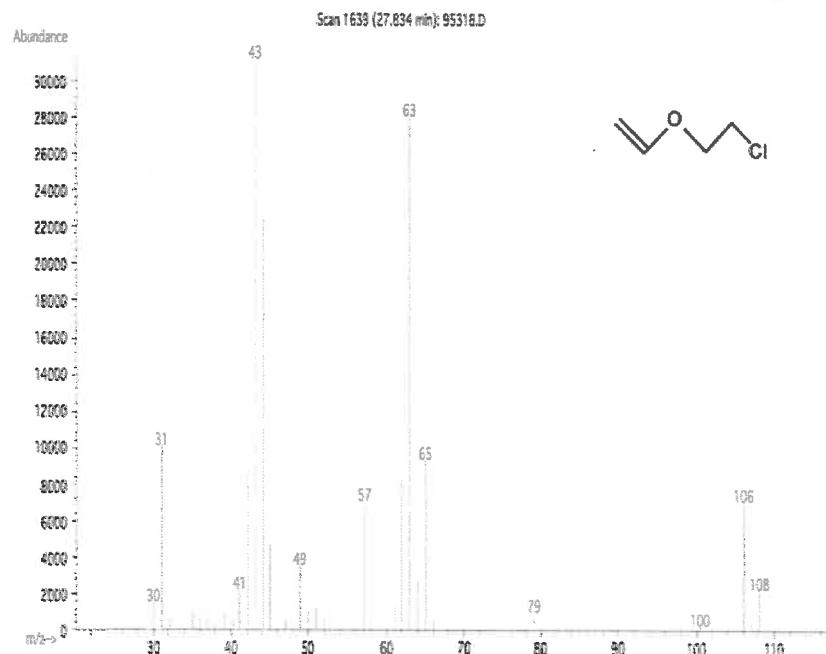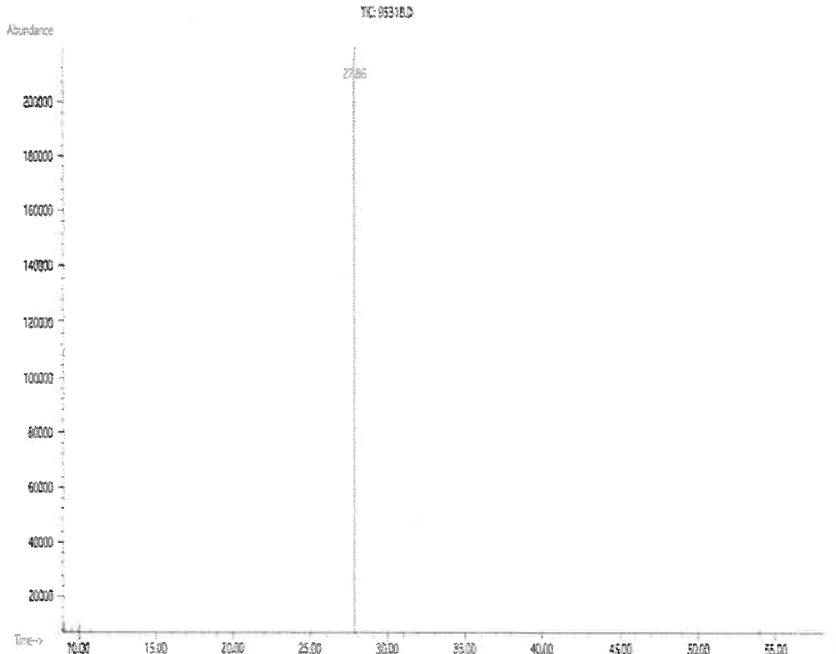

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

## **Safety Data Sheet (SDS)      GHS/OSHA Compliant**

## **Section I Product and Company Identification**

**IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

## **Section II - Hazards Identification**

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



## **Signal Word: DANGER**

### **Section III - Composition**

Components (Specific Chemical Identity; Common Name(s)) % (optional)  
Methanol METHYL ALCOHOL CAS#: 67-56-1 > 97

**See Certified Weight Report For Other Analytes Present At Trace Quantities.**

**INTENDED USE: REFERENCE MATERIAL**

#### **Section IV. FIRST AID MEASURES**

**General advice** Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.  
**If inhaled** If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.  
**In case of skin contact** Wash with soap and water. Consult a physician.  
**In case of eye contact** Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.  
**If swallowed** Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

## **Section V. FIREFIGHTING MEASURES**

**Flammability** Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.  
**Suitable extinguishing media** Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.  
**Protective equipment for fire** Wear self contained breathing apparatus for fire fighting if necessary.

## **Section VI. ACCIDENTAL RELEASE MEASURES**

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

## **Section VII. HANDLING AND STORAGE**

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

## **Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION**

**Methanol** 67-56-1 TWA 200 ppm  
**Skin notation** TWA 200 ppm  
Potential for skin absorption, ingestion and inhalation.  
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

## **Section IX - Physical/Chemical Characteristics**

Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




✓ 14630 to  
✓ 14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

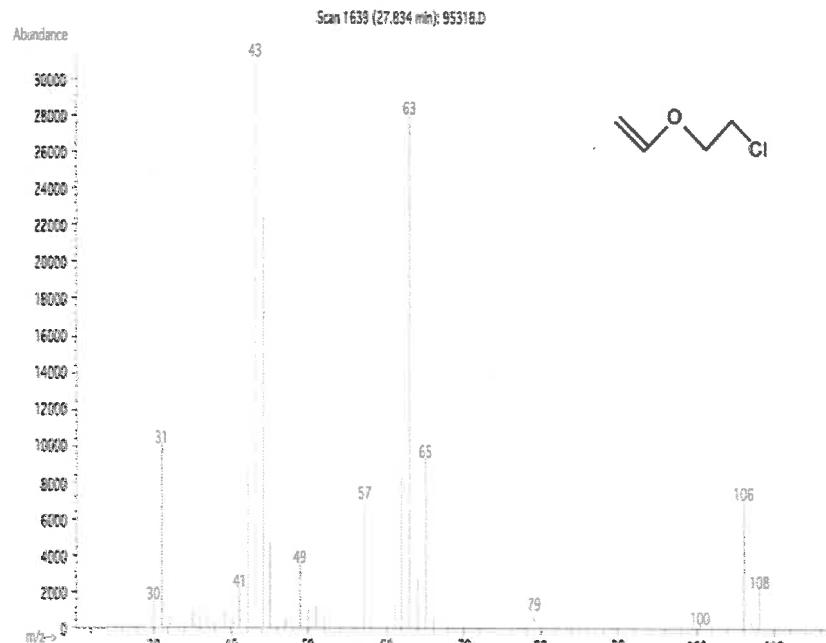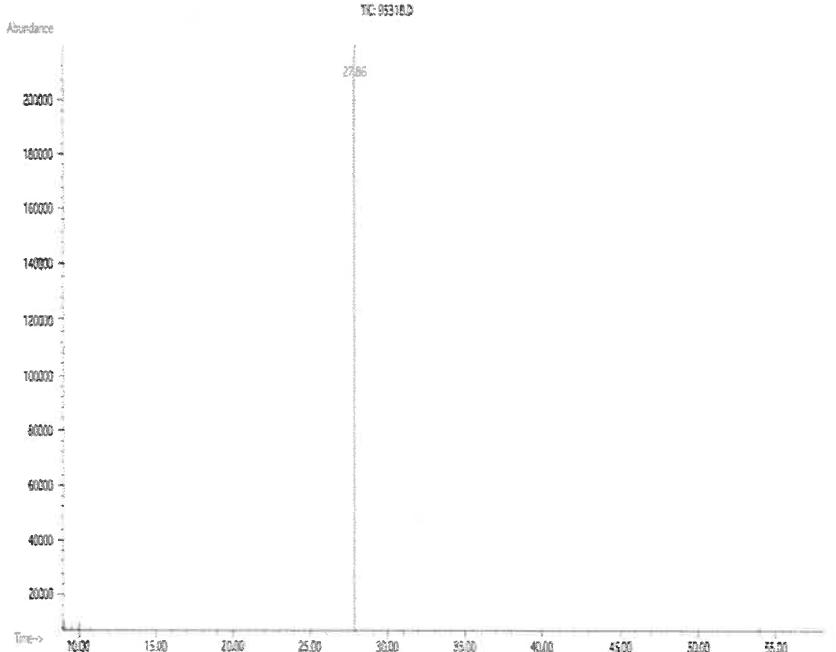

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

## Safety Data Sheet (SDS) GHS/OSHA Compliant

**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL**

Manufacturer's Name      ABSOLUTE STANDARDS INC      Emergency Telephone USA & CANADA      1-800-535-5053  
 Address      44 Rossotto Dr.      Emergency Telephone International      1-352-323-3500  
                  Hamden CT, 06514      Date Prepared/Revised      January 1, 2024

**Section II - Hazards Identification****GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))      % (optional)  
 Methanol      METHYL ALCOHOL      > 97

**See Certified Weight Report For Other Analytes Present At Trace Quantities.****INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

**Section V. FIREFIGHTING MEASURES**

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.

Protective equipment for fire      Wear self contained breathing apparatus for fire fighting if necessary.

**Section VI. ACCIDENTAL RELEASE MEASURES**

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

Clean up      Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

**Section VII. HANDLING AND STORAGE**

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

**Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION**

Methanol	67-56-1 TWA 200 ppm
Skin notation	TWA 200 ppm
Potential for skin absorption , ingestion and inhalation.	
Personal protective equipment	Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.	

**Section IX - Physical/Chemical Characteristics**

Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




✓ 14630 to  
✓ 14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

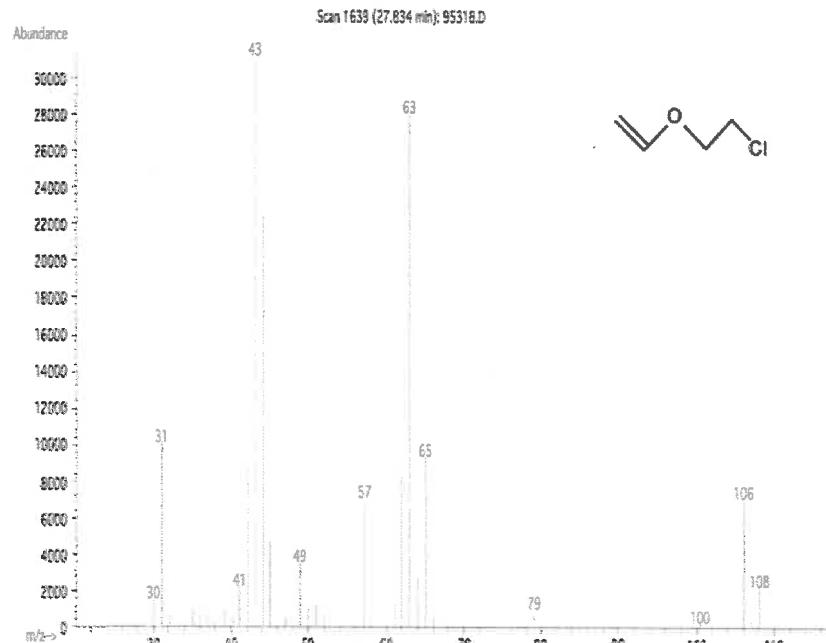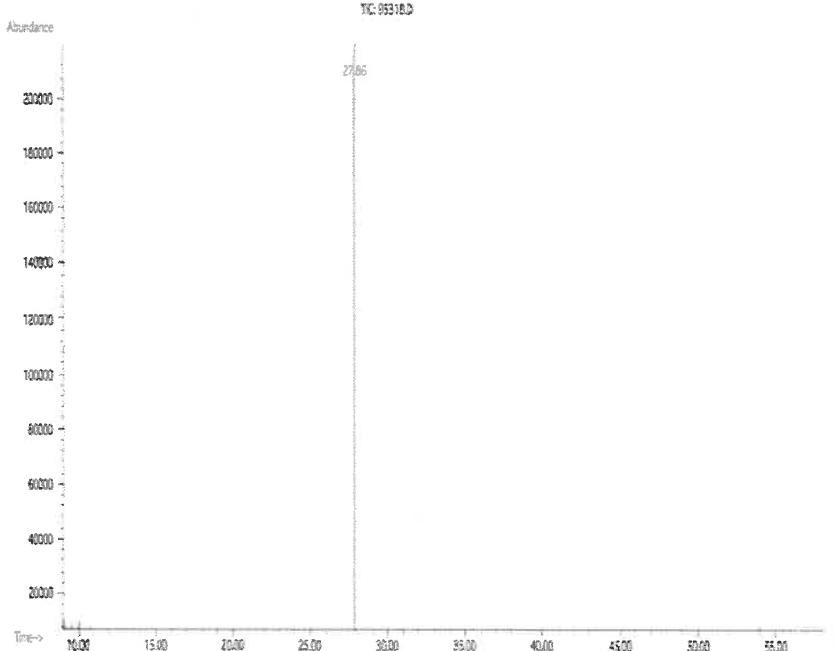

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24



CERTIFIED WEIGHT REPORT

Part Number: 95318  
Lot Number: 120524  
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#  
Methanol EJ143-US

Expiration Date: 120527  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test ID#: 6UTB




V14630 to  
V14649

Weight(s) shown below were combined and diluted to (mL): 50.0      5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Prashant Chauhan</i>		120524
Formulated By:	Prashant Chauhan	DATE
<i>Pedro L. Rentas</i>		120524
Reviewed By:	Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min.,  
Injector B Temp.= 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

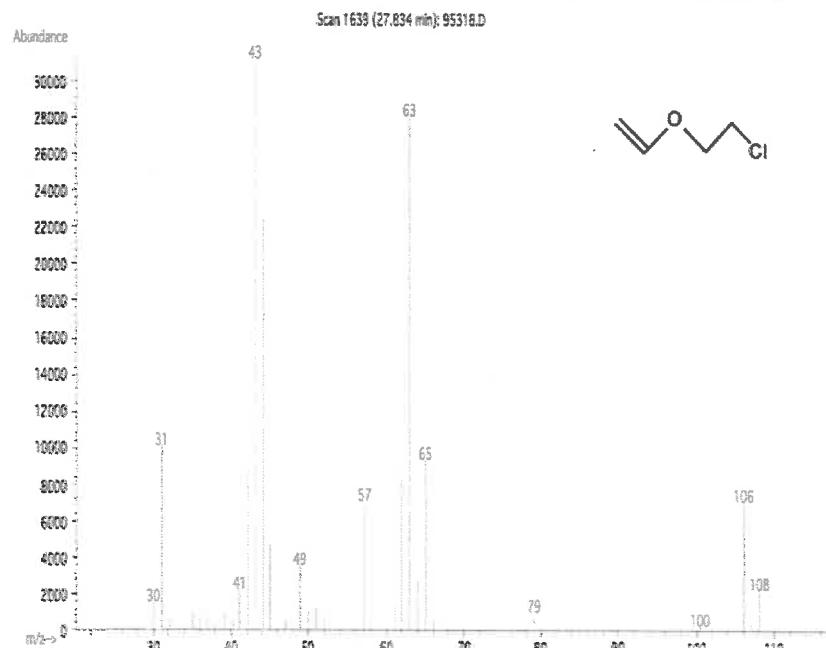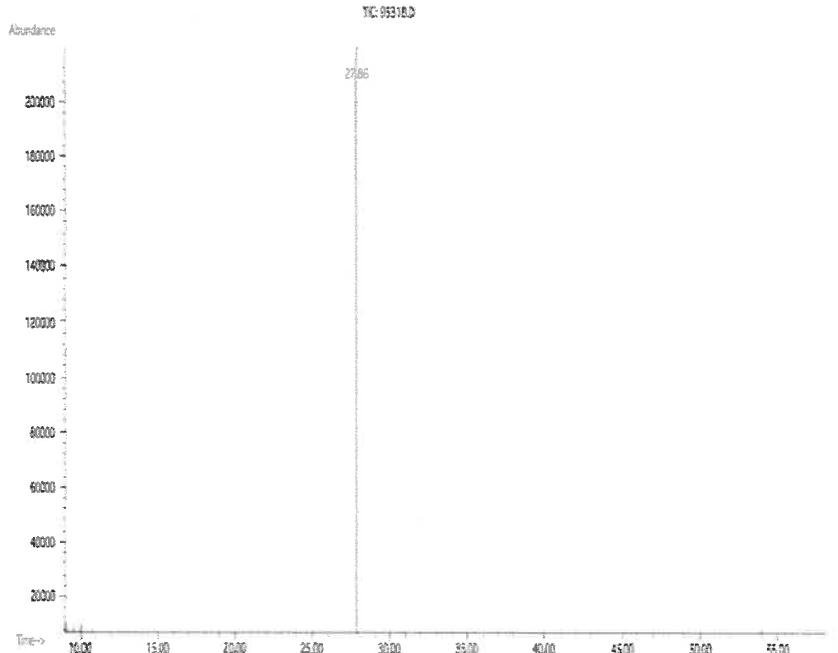

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ( $\pm$ ) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

## **Safety Data Sheet (SDS)      GHS/OSHA Compliant**

## **Section I Product and Company Identification**

**IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

## **Section II - Hazards Identification**

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



## **Signal Word: DANGER**

### **Section III - Composition**

Components (Specific Chemical Identity; Common Name(s)) % (optional)  
Methanol METHYLALCOHOL CAS#: 67-56-1 > 97

**See Certified Weight Report For Other Analytes Present At Trace Quantities.**

**INTENDED USE: REFERENCE MATERIAL**

## **Section IV. FIRST AID MEASURES**

<b>General advice</b>	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
<b>If inhaled</b>	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
<b>In case of skin contact</b>	Wash with soap and water. Consult a physician.
<b>In case of eye contact</b>	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
<b>If swallowed</b>	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

## **Section V. FIREFIGHTING MEASURES**

**Flammability** Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.  
**Suitable extinguishing media** Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.  
**Protective equipment for fire** Wear self contained breathing apparatus for fire fighting if necessary.

## **Section VI. ACCIDENTAL RELEASE MEASURES**

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

## **Section VII. HANDLING AND STORAGE**

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

## **Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION**

**Methanol** 67-56-1 TWA 200 ppm  
**Skin notation** TWA 200 ppm  
Potential for skin absorption, ingestion and inhalation.  
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

## **Section IX - Physical/Chemical Characteristics**

Boiling Point		Specific Gravity (H <sub>2</sub> O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
 Possibility of hazardous reactions Vapours may form explosive mixture with air.  
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids  
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - rat - 5,628 mg/kg  
 LC50 Inhalation - rat - 4 h - 64000 ppm  
 LD50 Dermal - rabbit - 15,800 mg/kg  
 Toxic if absorbed through skin. Causes skin irritation.  
 Eye damage/eye irritation  
 Toxic if inhaled. Causes respiratory tract irritation.  
 Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.**

LC50 15,400 mg/l - 96 h  
 EC50 24,500.00 mg/l - 48 h  
 EC100 10,000.00 mg/l - 24 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol  
 UN number: 1230 Class: 3 Packing group: II  
 Proper shipping name: Methanol

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30067

**Lot No.:** A0191805

**Description :** 4-Bromofluorobenzene Standard

4-Bromofluorobenzene Standard 2,500 $\mu$ g/mL, P&T Methanol,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	2,483.9 $\mu$ g/mL	+/- 139.5488

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**


40 ml/min

**Inj. Vol**

1 $\mu$ l

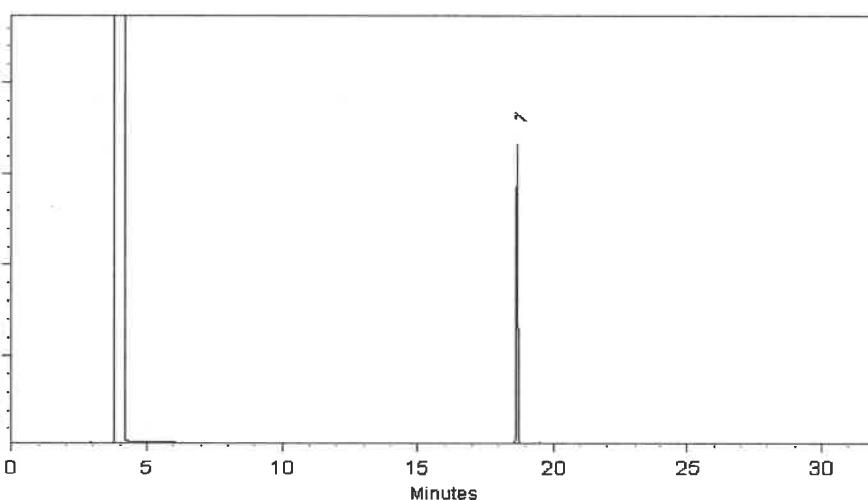

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Alicia Leathers - Operation Technician I

Date Mixed: 17-Nov-2022      Balance Serial #: B251644995

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Nov-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/pECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

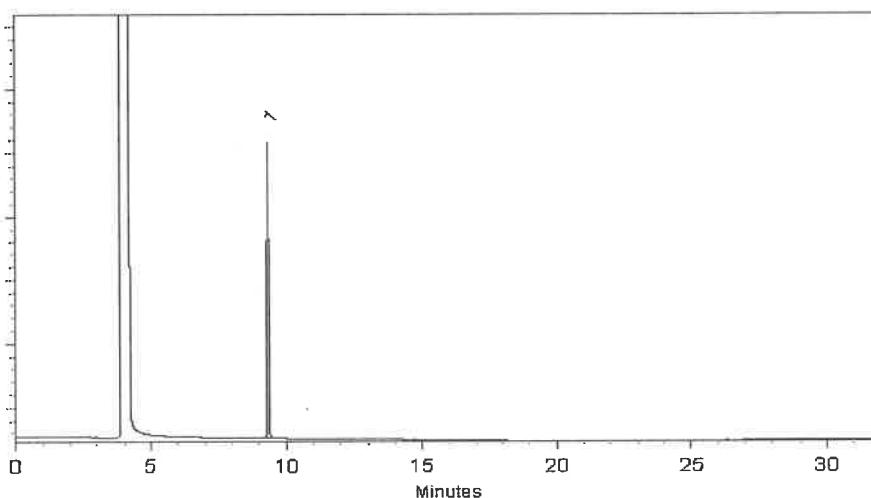

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

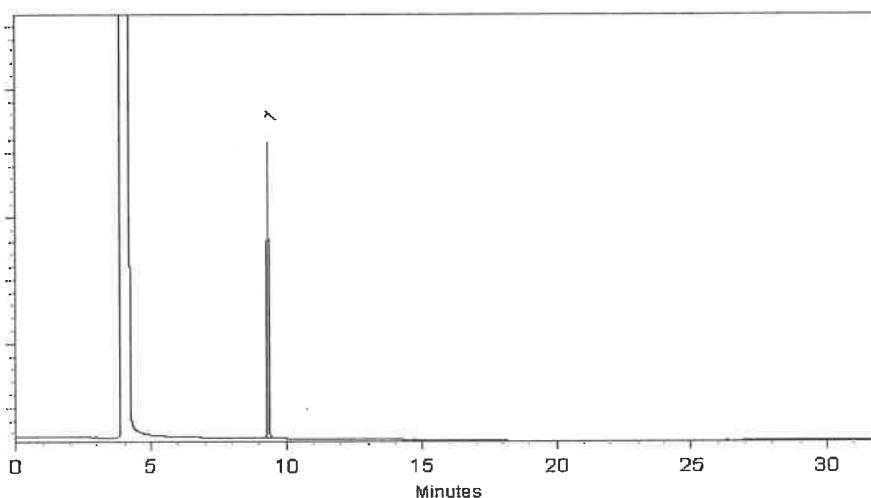

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

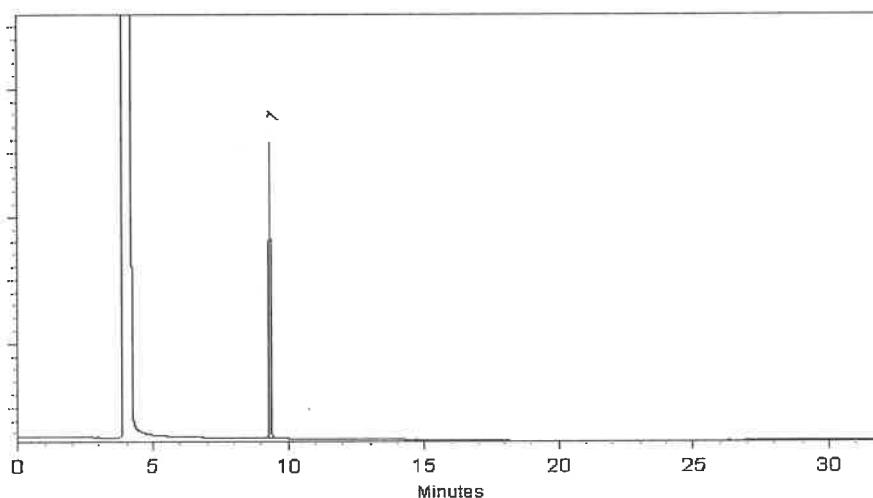

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

  
Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309  
[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30225

**Lot No.:** A0193071

**Description :** Bromochloromethane Standard

Bromochloromethane 2000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 $\mu$ g/mL	+/- 113.3890

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

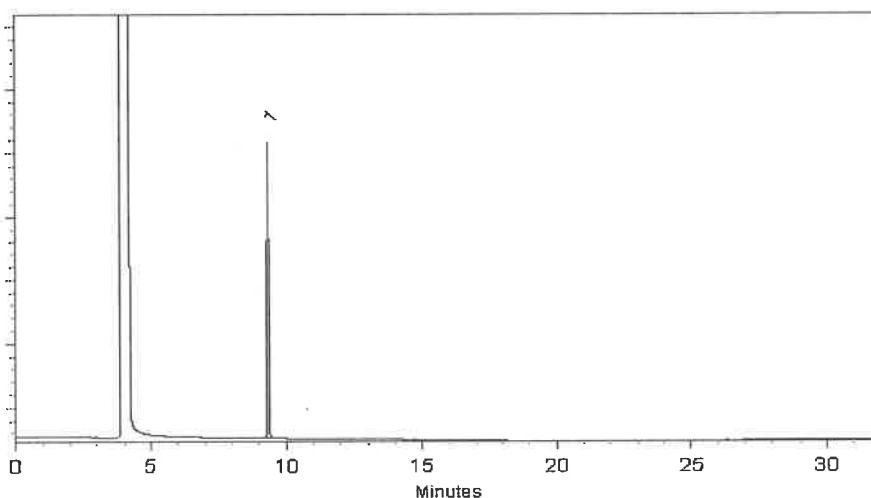

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022      Balance Serial #: B707717271

Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis *gravimetric*



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555582

**Lot No.:** A0196865

**Description :** Custom 8260A/B Surrogate Mix

Custom 8260A/B Surrogate Mix 25,000 $\mu$ g/mL, P&T Methanol,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2026


**Storage:** 10°C or colder

**Ship:** Ambient

#### C E R T I F I E D   V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2-Dichloroethane-d4	17060-07-0	PR-32845	99%	25,036.0 $\mu$ g/mL	+/- 1,417.9179
2	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	25,132.0 $\mu$ g/mL	+/- 1,423.3549
3	Dibromofluoromethane	1868-53-7	022013	99%	25,040.0 $\mu$ g/mL	+/- 1,418.1445
4	Toluene-d8	2037-26-5	PR-33397	99%	25,028.0 $\mu$ g/mL	+/- 1,417.4648

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

  
Russ Bookhamer - Operations Technician

Date Mixed: 11-Apr-2023 Balance: 1127510105

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30489

**Lot No.:** A0209618

**Description :** 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2025

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

## Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

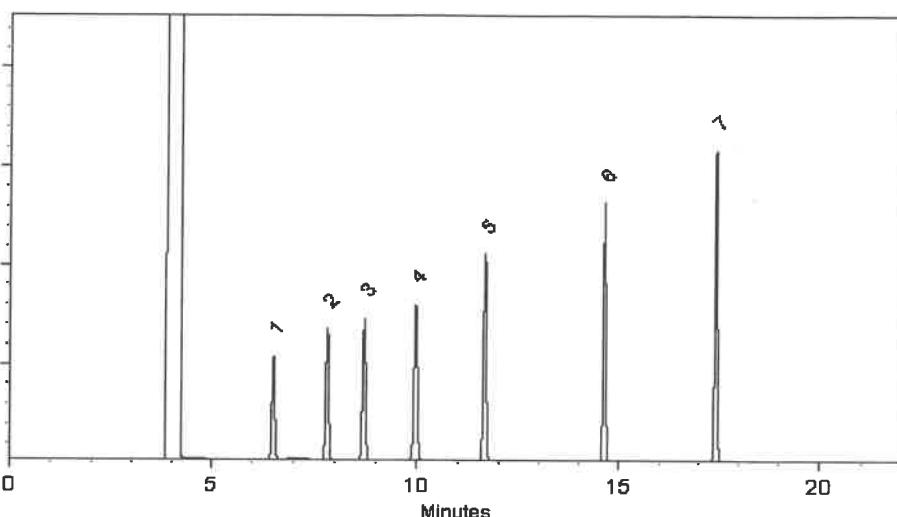

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodier*  
Sam Moodier - Operations Tech I

Date Mixed: 28-Mar-2024 Balance Serial #: B707717271

*Dillan Murphy*  
Dillan Murphy - Operations Technician |

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30489

**Lot No.:** A0209618

**Description :** 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2025

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

## Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

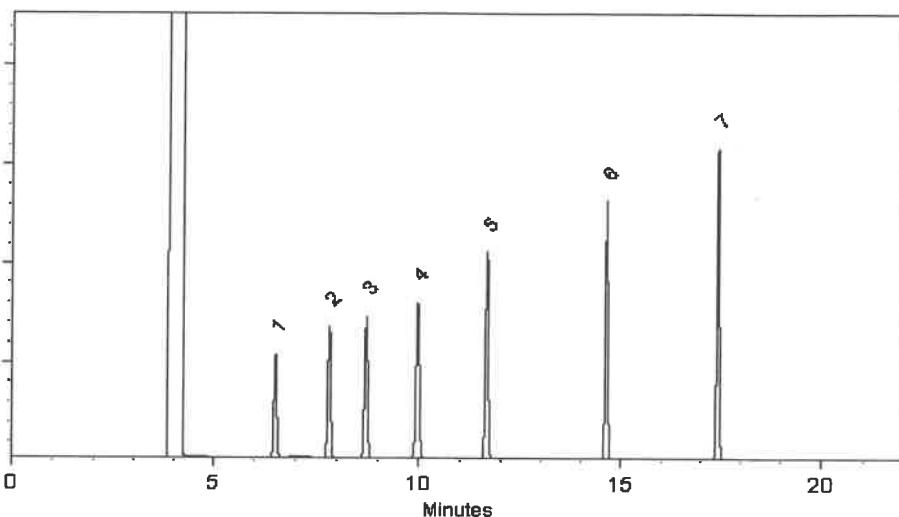

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Samuel Moodier*  
Sam Moodier - Operations Tech I

Date Mixed: 28-Mar-2024 Balance Serial #: B707717271

*Dillan Murphy*  
Dillan Murphy - Operations Technician |

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis *gravimetric*



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 555581

**Lot No.:** A0210184

**Description :** Custom 8260 Internal Standard Mix

Custom 8260 Internal Standard Mix 25,000 $\mu$ g/mL, P&T Methanol,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2027


**Storage:** 10°C or colder

**Ship:** Ambient

#### C E R T I F I E D   V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	25,212.0 $\mu$ g/mL	+/- 1,427.8857
2	1,4-Difluorobenzene	540-36-3	MKCS8657	99%	25,220.0 $\mu$ g/mL	+/- 1,428.3388
3	Chlorobenzene-d5	3114-55-4	PR-31132	99%	25,116.0 $\mu$ g/mL	+/- 1,422.4487
4	Pentafluorobenzene	363-72-4	MKCR9383	99%	25,180.0 $\mu$ g/mL	+/- 1,426.0734

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

  
John Friedline - Operations Technician I

Date Mixed: 11-Apr-2024

Balance: 1127510105

APPROVED  
By Analyst Name: 1.80 mg/g, 0.1%, 0.01

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

# Certificate of Analysis

*chromatographic plus*

V14697-to-14726



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 30006

**Lot No.:** A0210618

**Description :** VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 $\mu$ g/mL, P&T Methanol/Water(90:10),  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 $\mu$ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 $\mu$ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 $\mu$ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 $\mu$ g/mL	+/- 173.2261

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol/Water (90:10)

**CAS #** 67-56-1/7732-18-5

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**


1 $\mu$ l

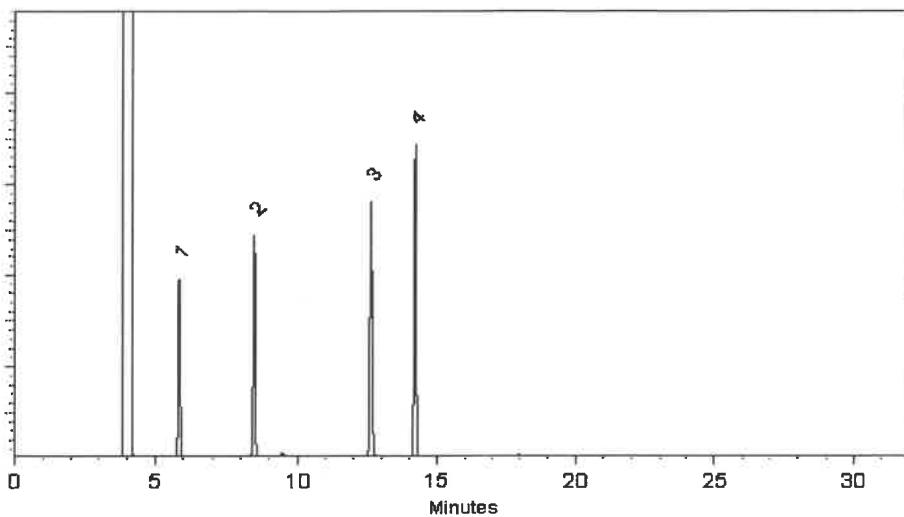

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024      Balance Serial #: B707717271

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

# Certificate of Analysis

chromatographic plus

V14697-to-14726



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 30006

**Lot No.:** A0210618

**Description :** VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 $\mu$ g/mL, P&T Methanol/Water(90:10),  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 $\mu$ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 $\mu$ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 $\mu$ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 $\mu$ g/mL	+/- 173.2261

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol/Water (90:10)

**CAS #** 67-56-1/7732-18-5

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**


1 $\mu$ l

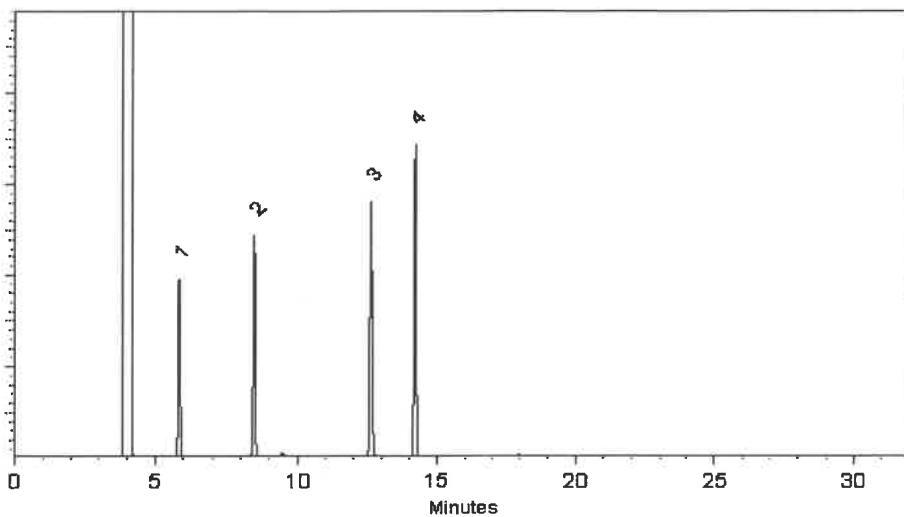

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024      Balance Serial #: B707717271

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

# Certificate of Analysis

*chromatographic plus*

V14697-to-14726



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 30006

**Lot No.:** A0210618

**Description :** VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 $\mu$ g/mL, P&T Methanol/Water(90:10),  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 $\mu$ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 $\mu$ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 $\mu$ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 $\mu$ g/mL	+/- 173.2261

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol/Water (90:10)

**CAS #** 67-56-1/7732-18-5

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**


1 $\mu$ l

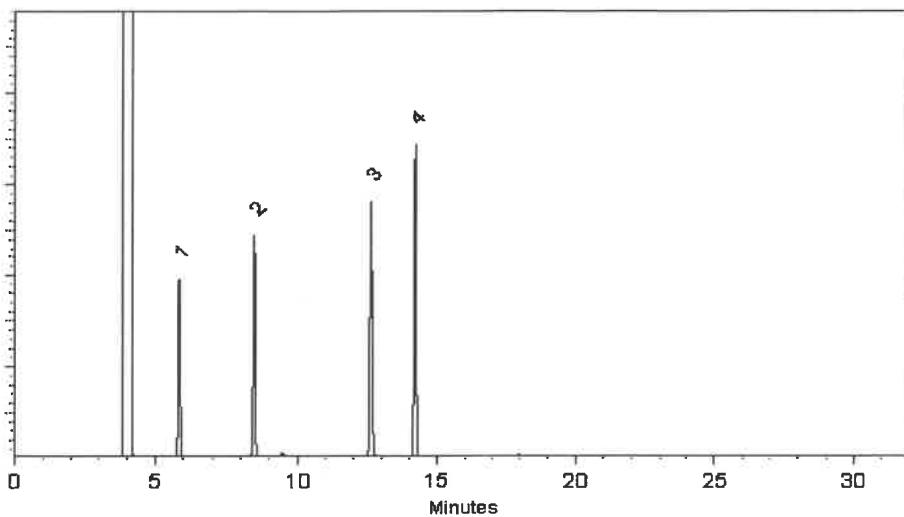

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024      Balance Serial #: B707717271

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

# Certificate of Analysis

*chromatographic plus*

V14697-to-14726



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No. :** 30006

**Lot No.:** A0210618

**Description :** VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 $\mu$ g/mL, P&T Methanol/Water(90:10),  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 $\mu$ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 $\mu$ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 $\mu$ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 $\mu$ g/mL	+/- 173.2261

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol/Water (90:10)

**CAS #** 67-56-1/7732-18-5

**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**


1 $\mu$ l

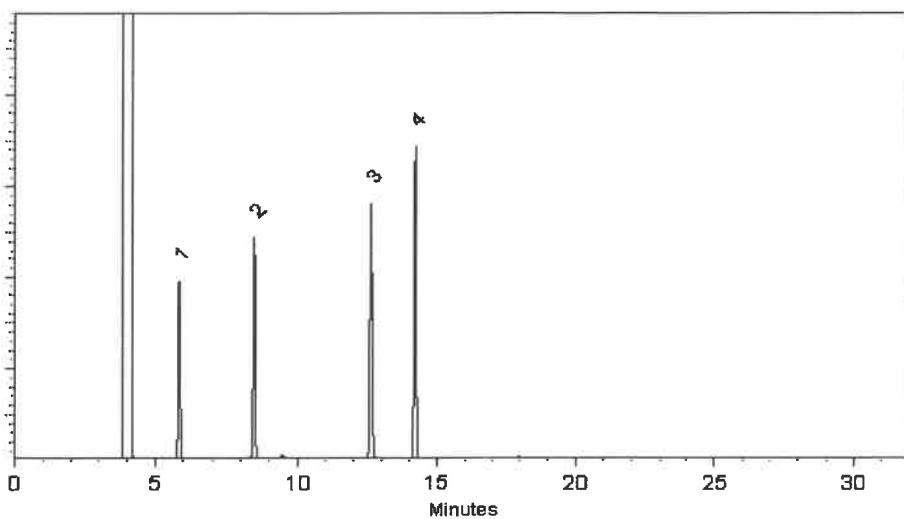

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024      Balance Serial #: B707717271

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

*Rev 12/17/24*  
**CERTIFIED REFERENCE MATERIAL**

*30 mL*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222-01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222-02

**Certificate of Analysis**  
*chromatographic plus*

*V14727 +  
V14756*

**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30042

**Lot No.:** A0216826

**Description :** 502.2 Calibration Mix #1

502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** May 31, 2031

**Storage:** 0°C or colder

**Ship:** Ambient

**C E R T I F I E D V A L U E S**

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

60m x 0.25mm x 1.4 $\mu$ m  
Rtx-502.2 (cat.#10916)

**Carrier Gas:**

helium-constant flow 2.0 mL/min.

**Temp. Program:**

40°C (hold 6 min.) to 100°C  
@ 6°C/min.

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


MSD

**Split Vent:**

Split ratio 10:1

**Inj. Vol**

1 $\mu$ L

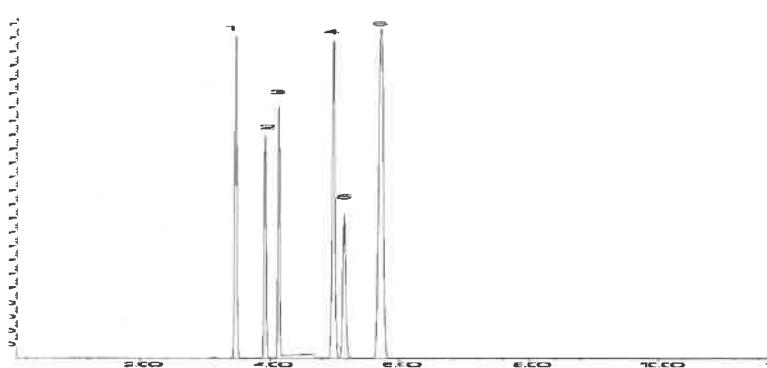

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar Mix Technician

Date Mixed: 23-Sep-2024 Balance Serial #: B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

*Rev 12/17/24*  
**CERTIFIED REFERENCE MATERIAL**

*30 mL*



**ILAC**  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222-01



**ILAC**  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222-02

**Certificate of Analysis**  
*chromatographic plus*

*V14727 +  
V14756*

**FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.**

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 30042

**Lot No.:** A0216826

**Description :** 502.2 Calibration Mix #1

502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** May 31, 2031

**Storage:** 0°C or colder

**Ship:** Ambient

**C E R T I F I E D   V A L U E S**

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

60m x 0.25mm x 1.4 $\mu$ m  
Rtx-502.2 (cat.#10916)

**Carrier Gas:**

helium-constant flow 2.0 mL/min.

**Temp. Program:**

40°C (hold 6 min.) to 100°C  
@ 6°C/min.

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


MSD

**Split Vent:**

Split ratio 10:1

**Inj. Vol**

1 $\mu$ L

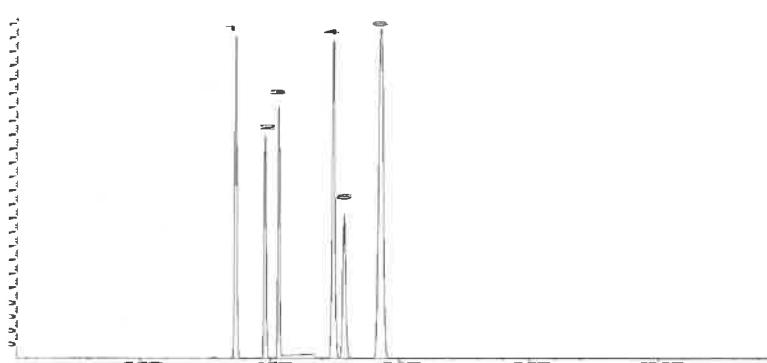

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar Mix Technician

Date Mixed: 23-Sep-2024 Balance Serial #: B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis

*chromatographic plus*

✓ 14842 to 14846

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 30470

**Lot No.:** A0217535

**Description :** tert-Butanol Standard

tert-Butanol Std 50,000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2027

**Storage:** 0°C or colder

**Ship:** Ambient

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	tert-Butanol (TBA)	75-65-0	SHBQ8002-1	99%	50,007.5 $\mu$ g/mL	+/- 717.6137

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol  
**CAS #** 67-56-1  
**Purity** 99%

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

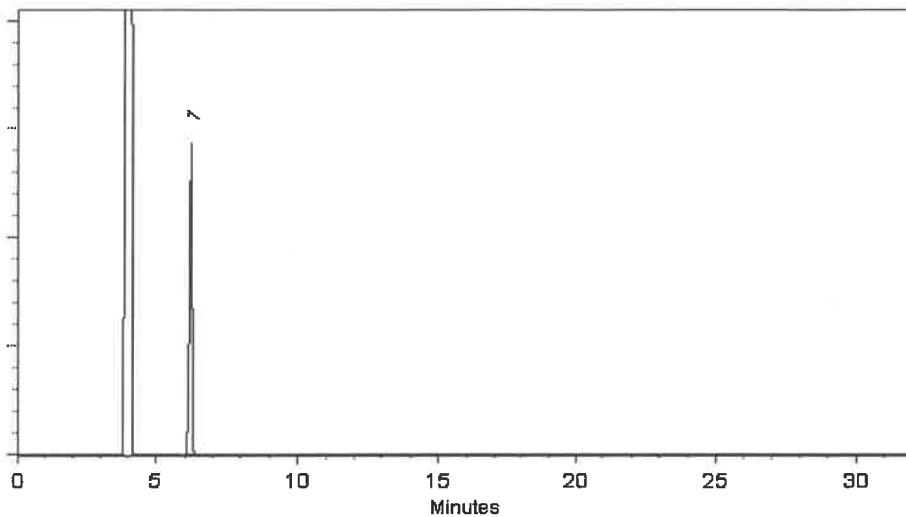

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Aaron Enyart*  
Aaron Enyart - Operations Tech I

Date Mixed: 07-Oct-2024      Balance Serial #: B251644995

*Brittany Federinko*  
Brittany Federinko - Operations Tech I

Date Passed: 09-Oct-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

2014 Dec 01 (08/21)



ILAC  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ILAC  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis

chromatographic

J14803 - J14822

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No.:** 555408-SL

**Lot No.:** A0220471

**Description :** Custom Vinyl Acetate Standard

Custom Vinyl Acetate Standard 8,000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** June 30, 2026

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 $\mu$ g/mL	+/- 278.7979

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

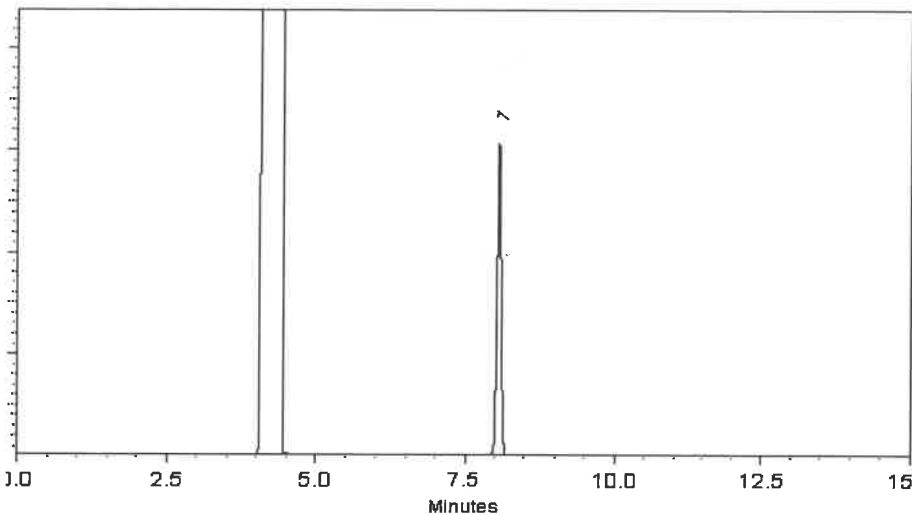

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ethan Winiarski*  
Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024      Balance Serial #: 1127510105

*Dillan Murphy*  
Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED  
By Jennifer Polson at 7:17 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

2014 Dec 01 (08/21)



ILAC  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ILAC  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis

chromatographic

J14803 - J14822

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

**Catalog No.:** 555408-SL

**Lot No.:** A0220471

**Description :** Custom Vinyl Acetate Standard

Custom Vinyl Acetate Standard 8,000 $\mu$ g/mL, P&T Methanol, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** June 30, 2026

**Storage:** -20°C or colder

**Handling:** This product is photosensitive.

**Ship:** On Ice

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 $\mu$ g/mL	+/- 278.7979

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** P&T Methanol

**CAS #** 67-56-1

**Purity** 99%

### Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

# Quality Confirmation Test

**Column:**

105m x 0.53mm x 3.0 $\mu$ m  
Rtx-502.2 (cat.#10910)

**Carrier Gas:**

hydrogen-constant pressure 11.0 psi.

**Temp. Program:**

40°C (hold 2 min.) to 240°C  
@ 8°C/min. (hold 5 min.)

**Inj. Temp:**

200°C

**Det. Temp:**

250°C

**Det. Type:**


FID

**Split Vent:**

40 ml/min

**Inj. Vol**

1 $\mu$ l

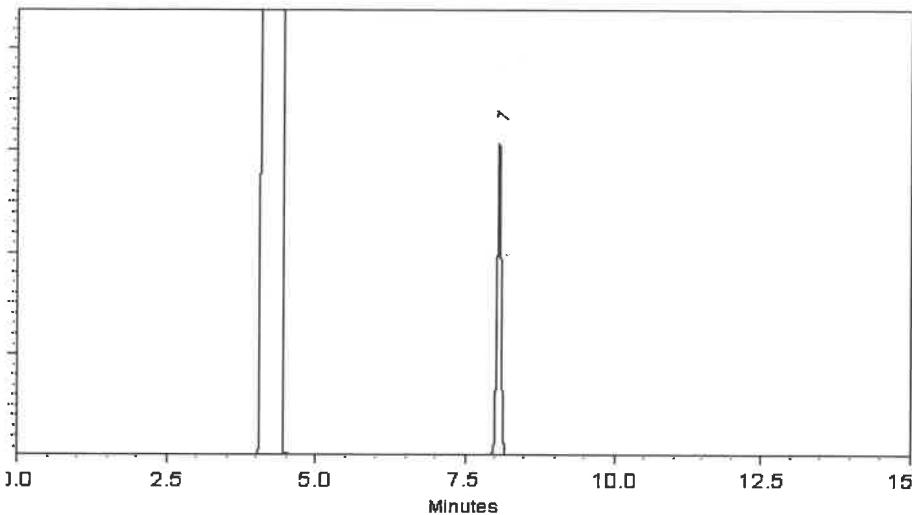

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ethan Winiarski*  
Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024      Balance Serial #: 1127510105

*Dillan Murphy*  
Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED  
By Jennifer Polson at 7:17 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

Methanol  
ULTRA RESI-ANALYZED  
For Purge and Trap Analysis

Rev 05/09/25  
**avantor™**



V14921 to  
V14938

Material No.: 9077-02  
Batch No.: 24G0262002  
Manufactured Date: 2024-05-14  
Expiration Date: 2027-05-14  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay (CH <sub>3</sub> OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.3
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use  
Performance Tested for Use in EPA Methods  
500 Series for Drinking Water  
600 Series for Wastewater  
846 for Solid Waste

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature of the name "Jamie Croak".

Jamie Croak  
Director Quality Operations, Bioscience Production



see 05/21/25



CERTIFIED WEIGHT REPORT

Part Number: 91980  
Lot Number: 051925  
Description: Acrolein

Solvent(s): Water  
Lot# 041725Q

5. v1g  
J14944-V14948

Expiration Date: 061925  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration ( $\mu\text{g/mL}$ ): 5000  
NIST Test ID#: 6UTB


Weight(s) shown below were combined and diluted to (mL): 10.0

5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Lawrence Barry</i>	051925
Formulated By: Lawrence Barry	DATE
<i>Pedro L. Rentas</i>	051925
Reviewed By: Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc ( $\mu\text{g/mL}$ )	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ( $\mu\text{g/mL}$ )	Expanded Uncertainty (+/-) ( $\mu\text{g/mL}$ )	SDS Information			
										(+/-) ( $\mu\text{g/mL}$ )	CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg	

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5 $\mu\text{m}$  film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately Long term storage is not recommended. Please contact our technical department if further information is required.

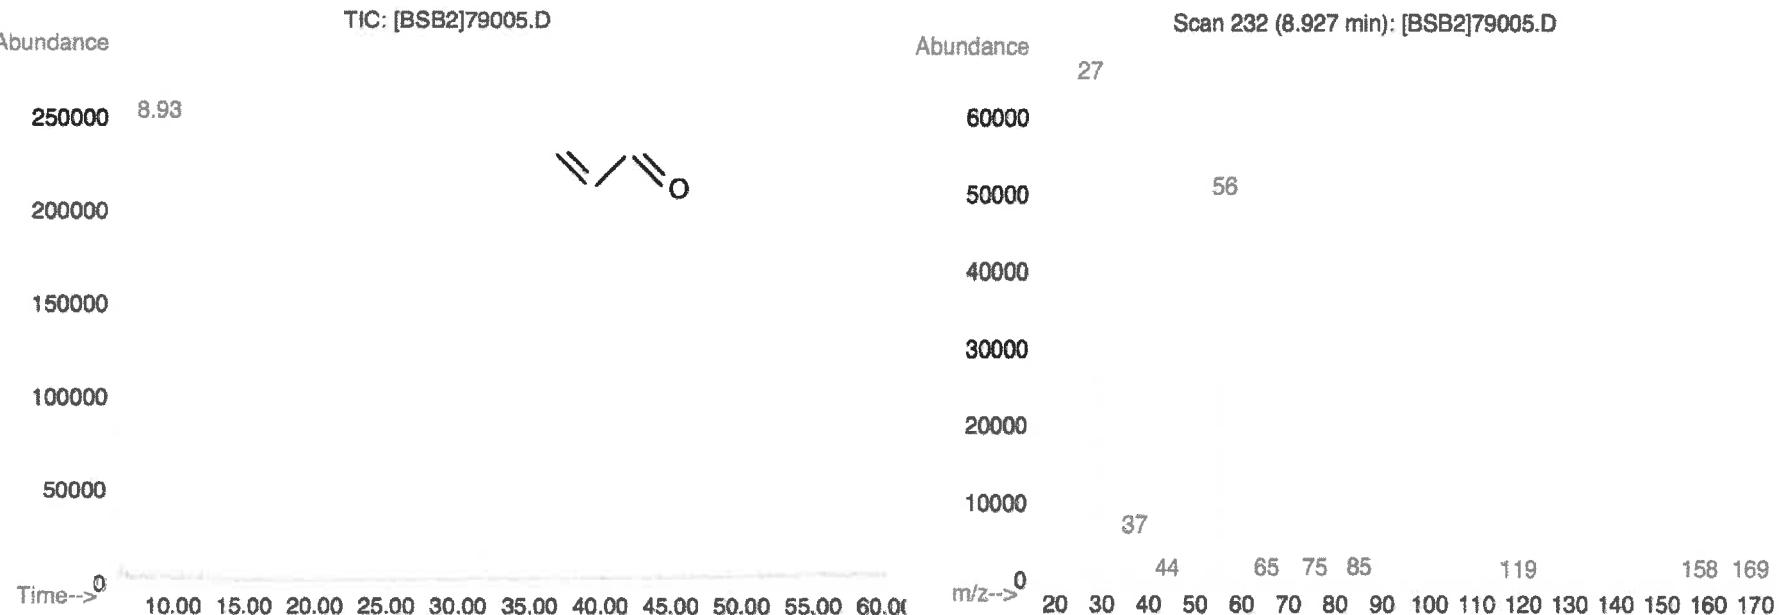

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
  - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
  - Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
  - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
  - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
- Rev 1.0, 2/25/2025



see US/21(25)



CERTIFIED WEIGHT REPORT

**Part Number:** 91980  
**Lot Number:** 051925  
**Description:** Acrolein

Solvent(s): Water Lot# 041725Q


Expiration Date: 061925  
Recommended Storage: Refrigerate (4 °C)  
Concentration (µg/mL): 5000  
NIST Test ID#: 61TR

**Weight(s) shown below were combined and diluted to (mL):** 10.0 0.001 **Flask Uncertainty:**

		051925
Formulated By:	Lawrence Barry	DATE
		051925
Reviewed By:	Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10E	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	cd-rat 46mg/kg

**Method:** GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5 $\mu$ m film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. **Analyst:** Pedro Renias. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

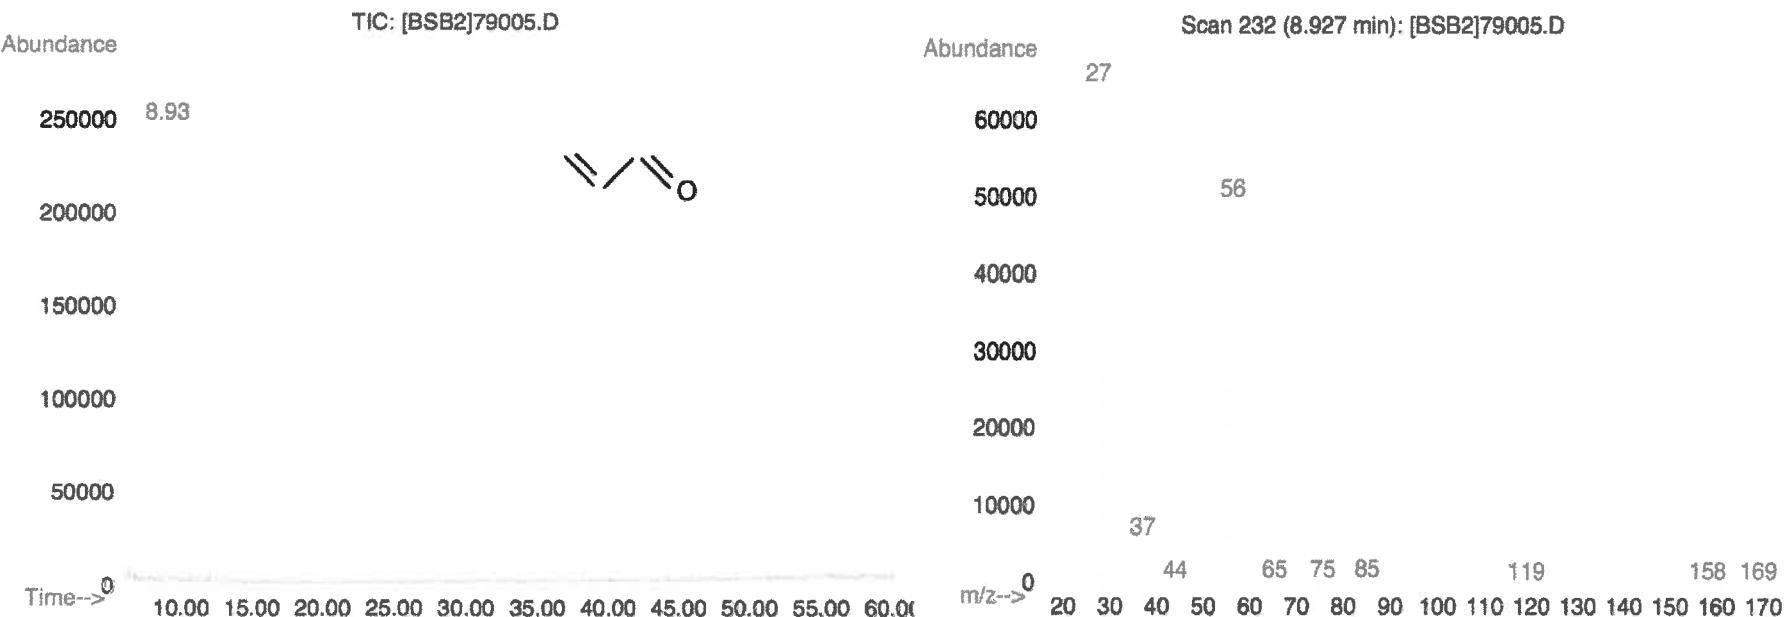

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
  - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
  - Standards are certified ( $\pm$ 0.5% of the stated value, unless otherwise stated.
  - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
  - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



see 05/21/25



CERTIFIED WEIGHT REPORT

Part Number: 91980  
Lot Number: 051925  
Description: Acrolein

Solvent(s): Water  
Lot# 041725Q

5. v1g  
J14944-V14948

Expiration Date: 061925  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration ( $\mu\text{g/mL}$ ): 5000  
NIST Test ID#: 6UTB


Weight(s) shown below were combined and diluted to (mL): 10.0

5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Lawrence Barry</i>	051925
Formulated By: Lawrence Barry	DATE
<i>Pedro L. Rentas</i>	051925
Reviewed By: Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc ( $\mu\text{g/mL}$ )	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ( $\mu\text{g/mL}$ )	SDS Information			
									(+/-) ( $\mu\text{g/mL}$ )	CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5 $\mu\text{m}$  film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately Long term storage is not recommended. Please contact our technical department if further information is required.

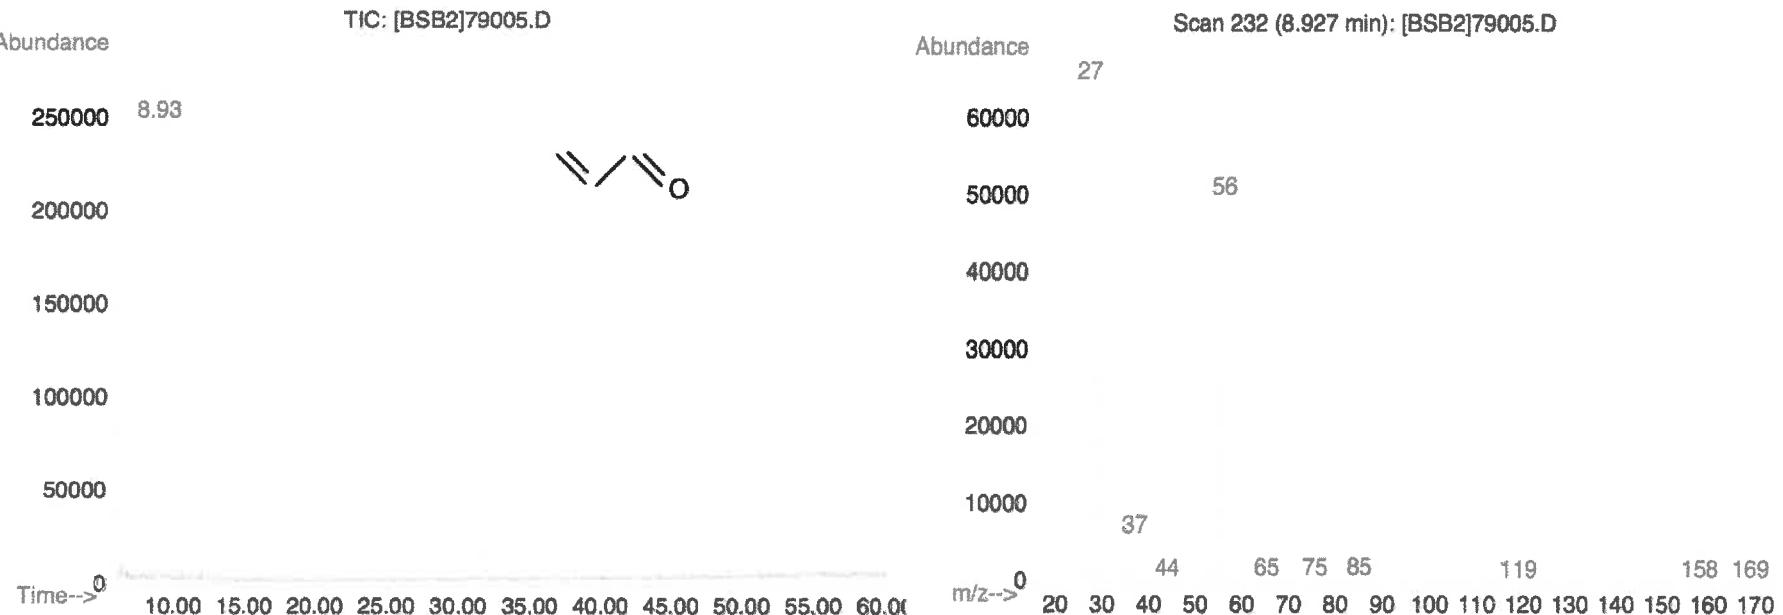

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
  - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
  - Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
  - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
  - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
- Rev 1.0, 2/25/2025



see 05/21/25



CERTIFIED WEIGHT REPORT

Part Number: 91980  
Lot Number: 051925  
Description: Acrolein

Solvent(s): Water  
Lot# 041725Q

5. v1g  
J14944-V14948

Expiration Date: 061925  
Recommended Storage: Refrigerate (4 °C)  
Nominal Concentration ( $\mu$ g/mL): 5000  
NIST Test ID#: 6UTB


Weight(s) shown below were combined and diluted to (mL): 10.0

5E-05 Balance Uncertainty  
0.001 Flask Uncertainty

<i>Lawrence Barry</i>	051925
Formulated By: Lawrence Barry	DATE
<i>Pedro L. Rentas</i>	051925
Reviewed By: Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc ( $\mu$ g/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ( $\mu$ g/mL)	Expanded Uncertainty (+/-) ( $\mu$ g/mL)	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5 $\mu$ m film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C ( Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately Long term storage is not recommended. Please contact our technical department if further information is required.

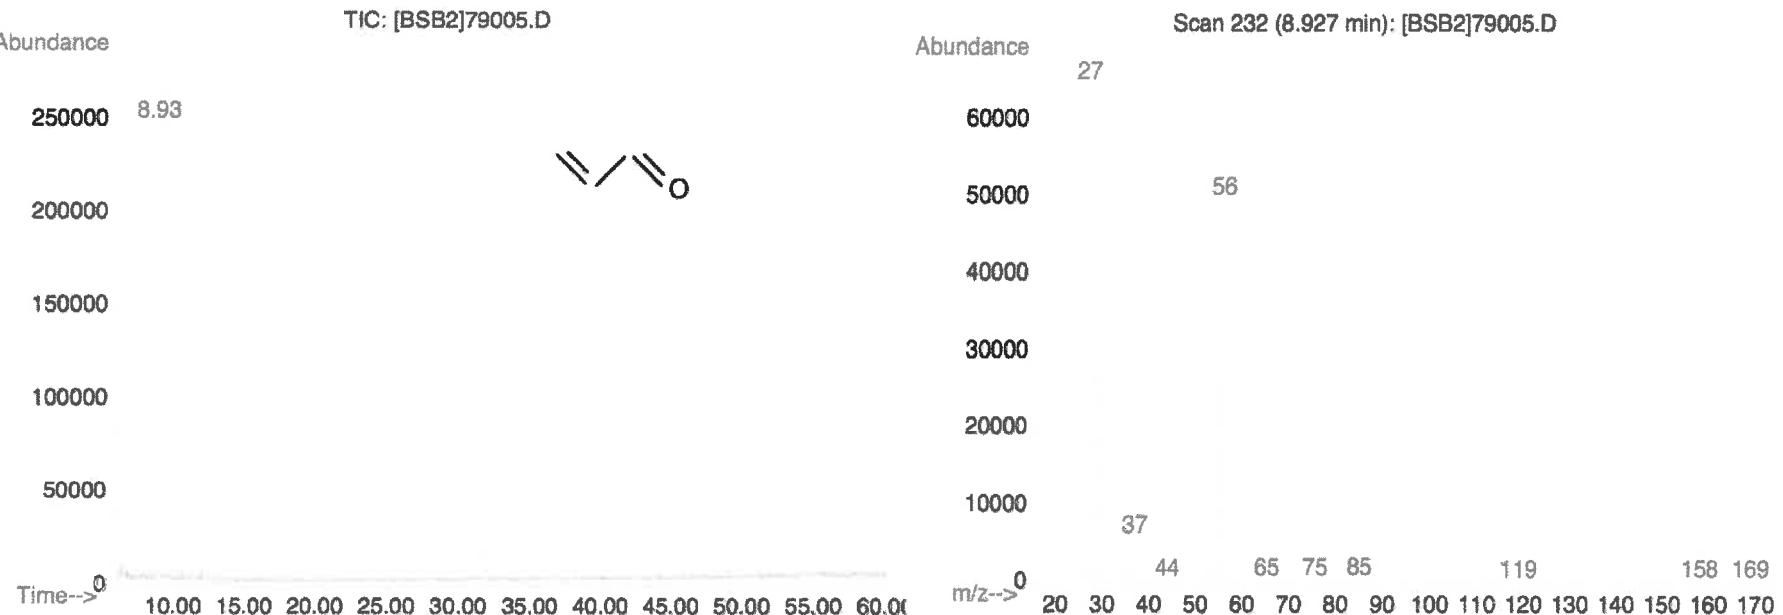

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
  - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
  - Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
  - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
  - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
- Rev 1.0, 2/25/2025



# SHIPPING DOCUMENTS

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16



284 Sheffield Street, Mountainside, NJ 07092

(908) 789-8900 • Fax (908) 789-8922

www.chemtech.net

ALLIANCE PROJECT NO.

QUOTE NO.

COC Number

QZ200

2046476

## CLIENT INFORMATION

## CLIENT PROJECT INFORMATION

## CLIENT BILLING INFORMATION

REPORT TO BE SENT TO:

COMPANY: Jacobs

ADDRESS: 412 Mt. Kemble Ave., Suite 100

CITY Morristown STATE: NJ ZIP: 07960

ATTENTION: John Ynfante John.Ynfante@Jacobs.com

PHONE: FAX:

PROJECT NAME: STC Princeton

PROJECT NO.: D3868221 LOCATION: Princeton Junction

PROJECT MANAGER: Mary Murphy

e-mail: Mary.Murphy@Jacobs.com

PHONE: FAX:

BILL TO: Mary Murphy

PO#:

ADDRESS:

CITY STATE: ZIP:

ATTENTION: PHONE:

## ANALYSIS

## DATA TURNAROUND INFORMATION

## DATA DELIVERABLE INFORMATION

FAX (RUSH) Standard TAT DAYS\*

HARDCOPY (DATA PACKAGE): DAYS\*

EDD: DAYS\*

\*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

 Level 1 (Results Only)  Level 4 (QC + Full Raw Data) Level 2 (Results + QC)  NJ Reduced  US EPA CLP Level 3 (Results + QC)  NYS ASP A  NYS ASP B  
+ Raw Data)  Other EDD FORMATSite specific VOC's  
(8160 D-Low)  
1/4 - Dioxane  
(8162 DE-GH)

1 2 3 4 5 6 7 8 9

## PRESERVATIVES

## COMMENTS

← Specify Preservatives  
 A-HCl D-NaOH  
 B-HNO3 E-ICE  
 C-H2SO4 F-OTHER

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS	
			COMP	GRAB	DATE	TIME		A/E	E									
1.	RMW-02B-60-060325	GW	X		6/3/25	1020	3	X	X									
2.	RMW-03B-90-060325	GW	X		6/3/25	1100	3	X	X									
3.	ER01-060325	DI	X		6/3/25	1300	3	X	X									
4.	MW-01-6.5-060325	GW	X		6/3/25	1400	1		X									
5.	MW-11B-37.5-060325	GW	X		6/3/25	1420	3	X	X									
6.	TB-01-060325	DI	X		6/3/25	1530	2	X										
7.																		
8.																		
9.																		
10.																		

## SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER:

DATE/TIME:  
6/3/25 1600RECEIVED BY:  
1. 16:20

RELINQUISHED BY SAMPLER:

DATE/TIME:

RECEIVED BY:  
2.

RELINQUISHED BY SAMPLER:

DATE/TIME:

RECEIVED BY:  
3.Conditions of bottles or coolers at receipt:  COMPLIANT  NON COMPLIANT  COOLER TEMP 3.42 °CComments: See work order for list of site specific VOC's  
PO# 148064311

Page 1 of 2

CLIENT:  Hand Delivered  Other

Shipment Complete

 YES  NO

**Laboratory Certification**

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

## LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q2200 JAC005	Order Date : 6/3/2025 4:06:00 PM	Project Mgr :
Client Name : JACOBS Engineering Grou	Project Name : Former Schlumberger STC	Report Type : <u>Level 4</u> level 3
Client Contact : John Ynfante	Receive Date/Time : 6/3/2025 12:00:00 AM	EDD Type : CH2MHILL
Invoice Name : JACOBS Engineering Grou	Purchase Order : 17:20	Hard Copy Date :
Invoice Contact : John Ynfante		Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DU <sup>E</sup> DATES
Q2200-01	RMW-02B-66-060325	Water	06/03/2025	10:20	VOCMS Group3		8260-Low	10 Bus. Days	
Q2200-02	RMW-03B-90-060325	Water	06/03/2025	11:00	VOCMS Group3		8260-Low	10 Bus. Days	
Q2200-03	EB01-060325	Water	06/03/2025	13:00	VOCMS Group3		8260-Low	10 Bus. Days	
Q2200-05	MW-11B-37.5-060325	Water	06/03/2025	14:20	VOCMS Group3		8260-Low	10 Bus. Days	
Q2200-06	TB-01-060325	Water	06/03/2025	15:30	VOCMS Group3		8260-Low	10 Bus. Days	

Relinquished By :

Date / Time : 6/4/25 1040

Samples received on 6/3/25  
Samples placed in SM-REF-2

Received By :

Date / Time : 06/04/25 10:40 AM Leg# 4

Storage Area : VOA Refrigerator Room