
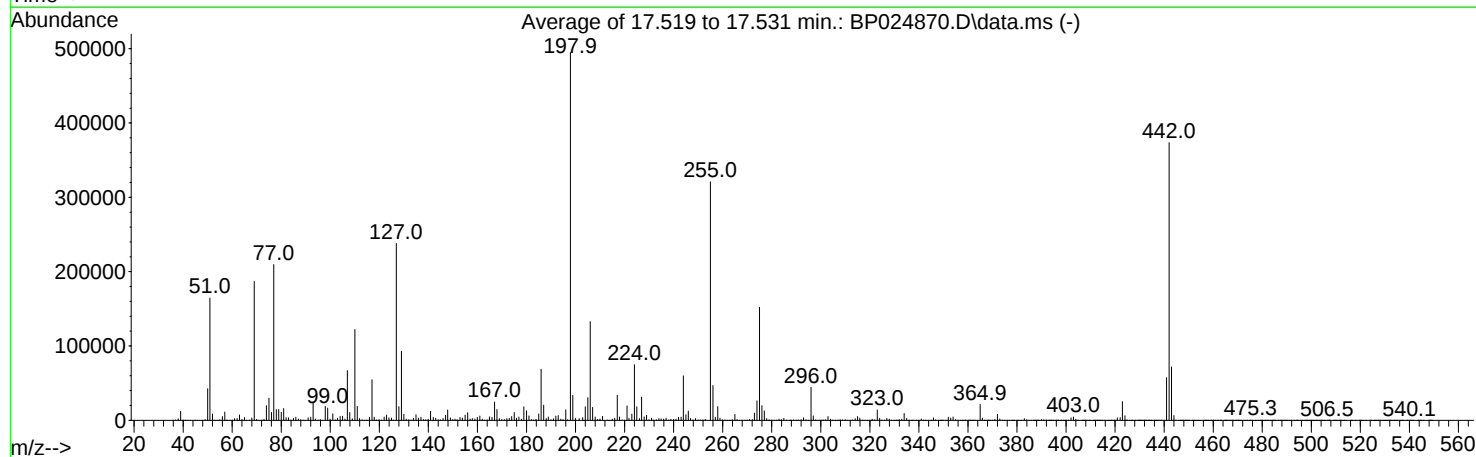


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060925\
Data File : BP024870.D
Acq On : 09 Jun 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

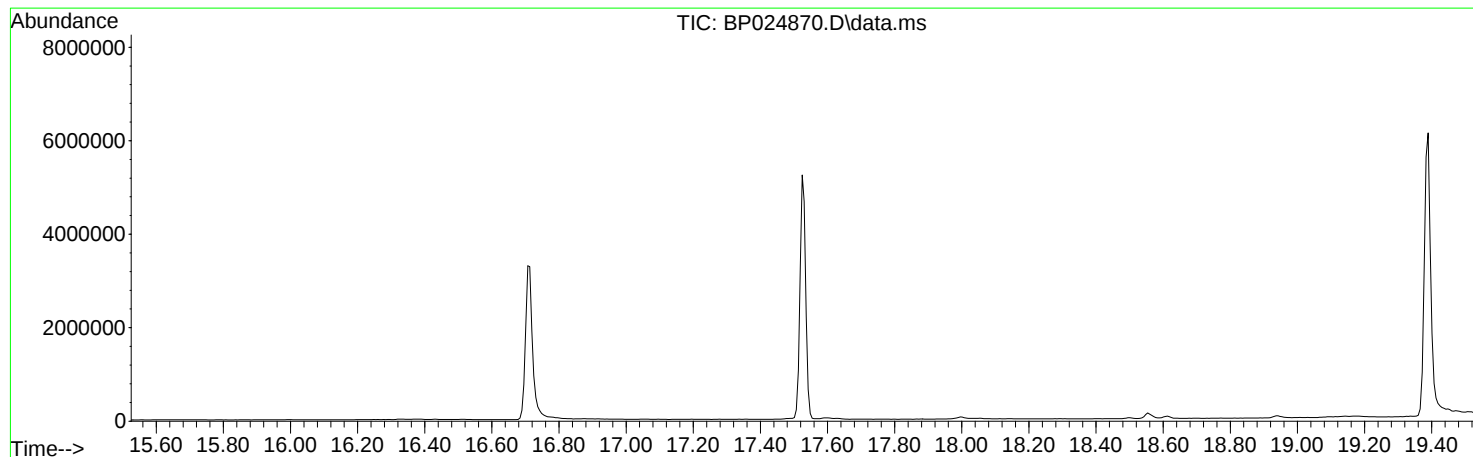




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	164298	PASS
68	69	0.00	2	1.7	3127	PASS
69	198	0.00	100	37.7	186800	PASS
70	69	0.00	2	0.6	1208	PASS
127	198	10	80	48.1	237925	PASS
197	198	0.00	2	0.1	705	PASS
198	198	100	100	100.0	494936	PASS
199	198	5	9	6.8	33502	PASS
275	198	10	60	30.7	152082	PASS
365	198	1	100	4.3	21354	PASS
441	198	0.01	100	11.6	57460	PASS
442	442	100	100	100.0	373547	PASS
443	442	15	24	19.2	71751	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060925\
Data File : BP024870.D
Acq On : 09 Jun 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 09 10:53:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

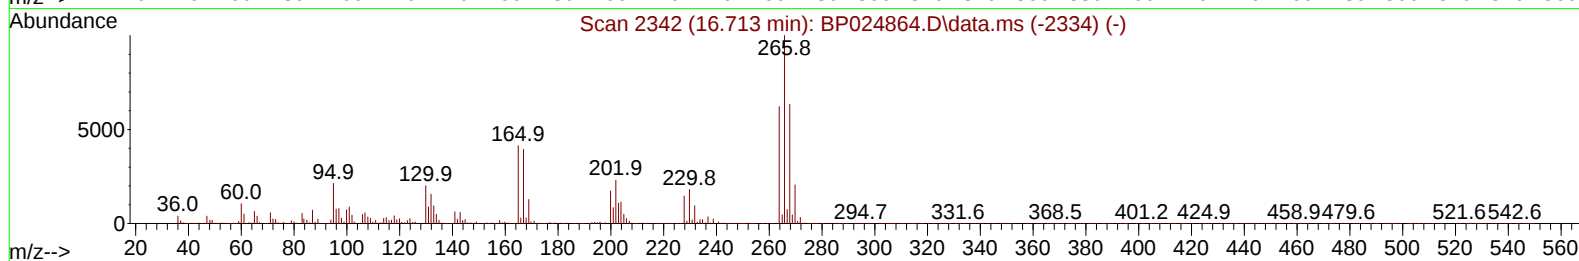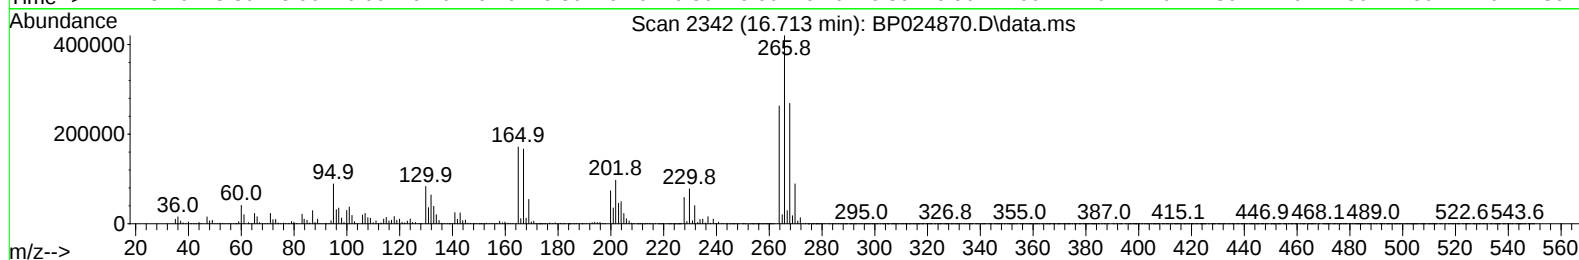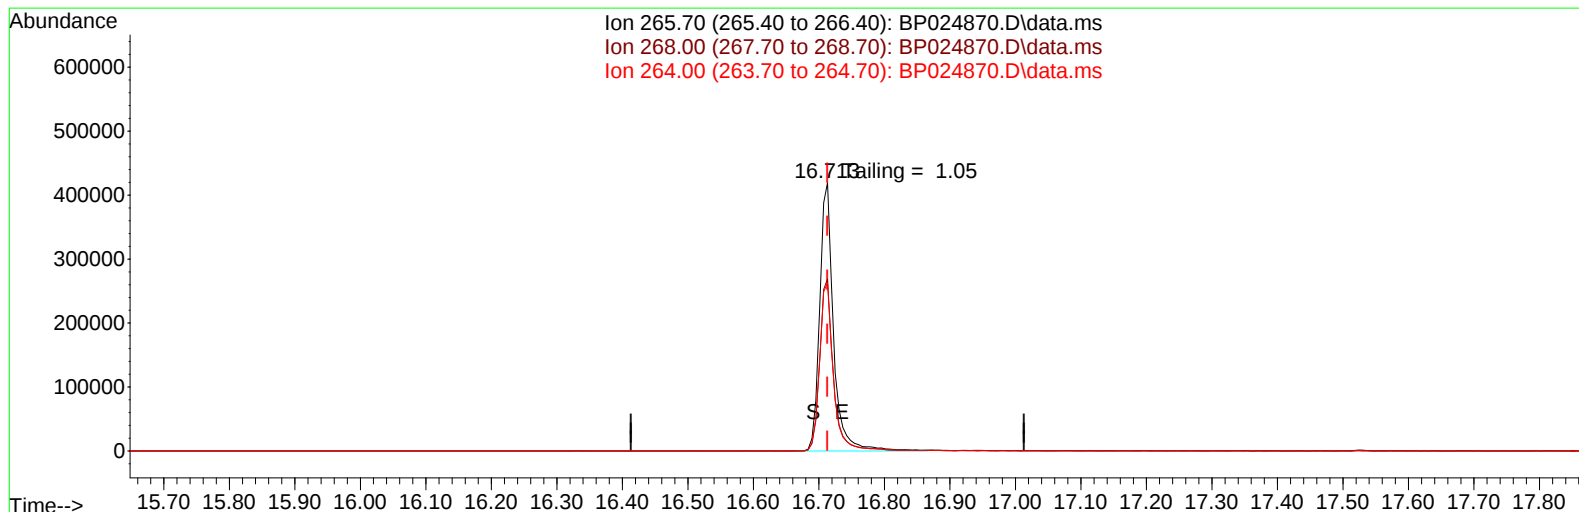

TIC: BP024870.D\data.ms

(70) Pentachlorophenol (C)

16.713min (-0.000) 92926.84 ng




response 615758

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.02
264.00	62.10	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060925\
Data File : BP024870.D
Acq On : 09 Jun 2025 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 09 10:53:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

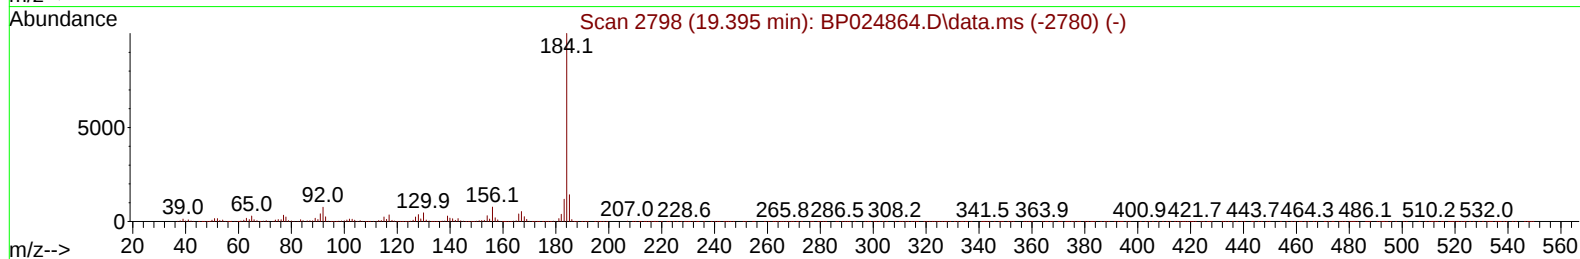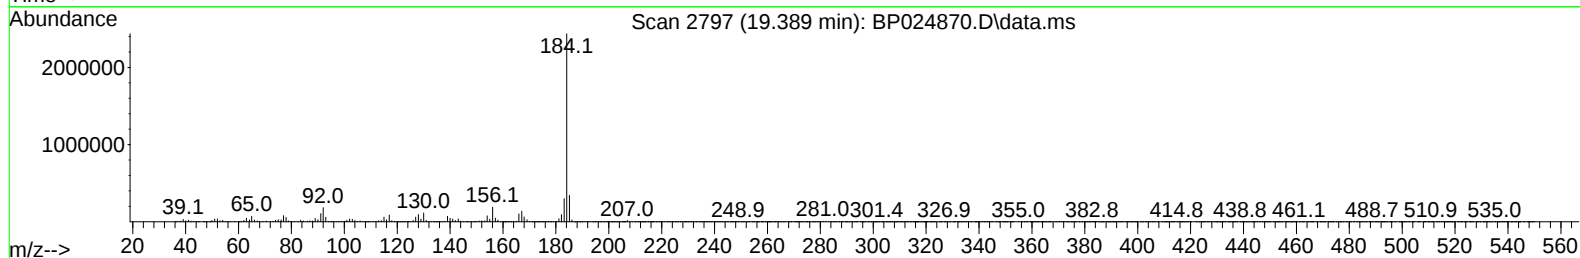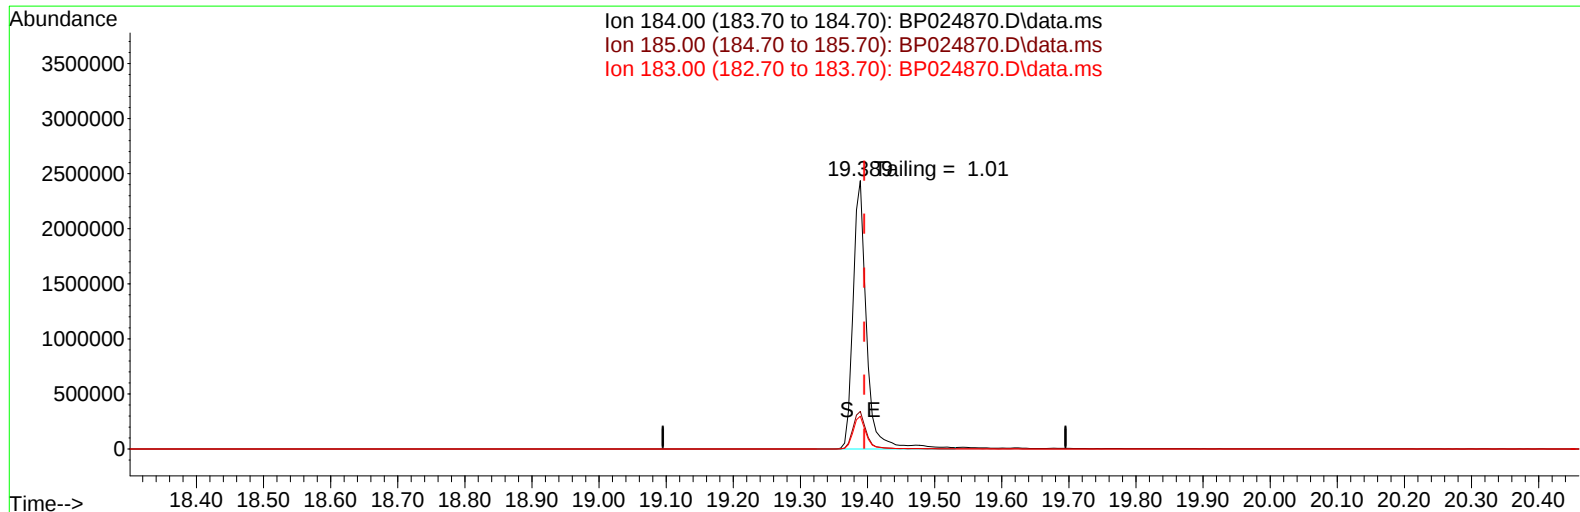

TIC: BP024870.D\data.ms

(77) Benzidine

19.389min (-0.006) 1294.06 ng

response 3322112

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.01
183.00	11.90	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2025	BNA_P	<u>BP024870.D</u>
Compound Name	Response	Retention Time
DDT	1823097	20.672
DDD	22597	20.26
DDE	2048	19.689
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24645	1847742	1.33

Instrument :
BNA_P
ClientSampleId :
DFTPP