

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\
 Method File : 8270-SIM-BN060325.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 04 01:52:03 2025
 Response Via : Initial Calibration

Calibration Files

0.1 =BN037143.D 0.2 =BN037144.D 0.4 =BN037145.D 0.8 =BN037146.D 1.6 =BN037147.D 3.2 =BN037148.D 5.0 =BN037149.D

	Compound	0.1	0.2	0.4	0.8	1.6	3.2	5.0	Avg	%RSD
1) I	1,4-Dichlorobenzen...	-----ISTD-----								
2)	1,4-Dioxane	0.598	0.657	0.510	0.506	0.526	0.477	0.458	0.533	13.16
3)	n-Nitrosodimet...	1.098	1.031	1.061	1.067	1.163	1.061	1.012	1.071	4.60
4) S	2-Fluorophenol	1.027	1.017	0.940	0.945	1.036	0.984	0.975	0.989	3.91
5) S	Phenol-d6	1.156	1.144	1.127	1.126	1.293	1.261	1.285	1.199	6.42
6)	bis(2-Chloroet...	1.138	1.139	1.128	1.089	1.223	1.146	1.146	1.144	3.51
7) I	Naphthalene-d8	-----ISTD-----								
8) S	Nitrobenzene-d5	0.393	0.383	0.421	0.407	0.455	0.450	0.446	0.422	6.86
9)	Naphthalene	1.183	1.125	1.119	1.111	1.215	1.165	1.160	1.154	3.31
10)	Hexachlorobuta...	0.253	0.249	0.261	0.247	0.266	0.246	0.238	0.251	3.81
11) SURR	2-Methylnaphth...	0.520	0.515	0.562	0.536	0.598	0.577	0.588	0.557	5.97
12)	2-Methylnaphth...	0.704	0.680	0.691	0.719	0.809	0.783	0.793	0.740	7.22
13) I	Acenaphthene-d10	-----ISTD-----								
14) S	2,4,6-Tribromo...	0.124	0.147	0.146	0.157	0.185	0.182	0.186	0.161	15.03
15) S	2-Fluorobiphenyl	1.722	1.691	1.626	1.654	1.814	1.706	1.725	1.705	3.52
16)	Acenaphthylene	1.946	1.905	1.768	1.871	2.112	2.050	2.075	1.961	6.32
17)	Acenaphthene	1.290	1.253	1.159	1.212	1.370	1.309	1.320	1.273	5.59
18)	Fluorene	1.701	1.577	1.518	1.611	1.823	1.736	1.752	1.674	6.48
19) I	Phenanthrene-d10	-----ISTD-----								
20)	4,6-Dinitro-2-...	0.039	0.050	0.067	0.090	0.102	0.114	0.077		38.58
21)	4-Bromophenyl-...	0.256	0.253	0.244	0.254	0.281	0.276	0.271	0.262	5.32
22)	Hexachlorobenzene	0.289	0.284	0.269	0.279	0.301	0.284	0.274	0.283	3.72
23)	Atrazine	0.194	0.200	0.187	0.209	0.241	0.238	0.247	0.216	11.42
24)	Pentachlorophenol	0.086	0.086	0.092	0.107	0.140	0.153	0.165	0.124	26.72
25)	Phenanthrene	1.285	1.242	1.193	1.248	1.386	1.357	1.361	1.296	5.64
26)	Anthracene	1.098	1.099	1.036	1.143	1.294	1.290	1.317	1.183	9.71
27) SURR	Fluoranthene-d10	0.969	0.937	0.975	0.956	1.092	1.071	1.114	1.016	7.22
28)	Fluoranthene	1.339	1.294	1.277	1.365	1.579	1.563	1.605	1.432	10.09
29) I	Chrysene-d12	-----ISTD-----								
30)	Pyrene	2.051	1.974	1.827	1.928	2.048	1.955	1.885	1.953	4.20
31) S	Terphenyl-d14	0.964	0.909	0.896	0.941	1.006	0.952	0.923	0.942	3.96
32)	Benzo(a)anthra...	1.369	1.367	1.291	1.404	1.582	1.553	1.570	1.448	8.15
33)	Chrysene	1.755	1.636	1.473	1.582	1.698	1.584	1.556	1.612	5.81
34)	Bis(2-ethylhex...	1.032	0.859	0.774	0.858	0.956	0.914	1.002	0.914	9.90
35) I	Perylene-d12	-----ISTD-----								

Method Path : Z:\svoasrv\HPCHEM1\BNA_N\Methods\


Method File : 8270-SIM-BN060325.M

36)	Indeno(1,2,3-c...	1.443	1.605	1.501	1.526	1.695	1.673	1.697	1.591	6.44
37)	Benzo(b)fluora...	1.529	1.520	1.421	1.575	1.763	1.713	1.781	1.615	8.58
38)	Benzo(k)fluora...	1.576	1.565	1.461	1.612	1.777	1.743	1.805	1.648	7.79
39) C	Benzo(a)pyrene	1.310	1.287	1.219	1.294	1.451	1.426	1.481	1.352	7.32
40)	Dibenzo(a,h)an...	1.074	1.167	1.160	1.196	1.333	1.332	1.328	1.227	8.48
41)	Benzo(g,h,i)pe...	1.368	1.450	1.351	1.372	1.477	1.424	1.425	1.410	3.33

(#) = Out of Range

Pentachlorophenol

Response Ratio

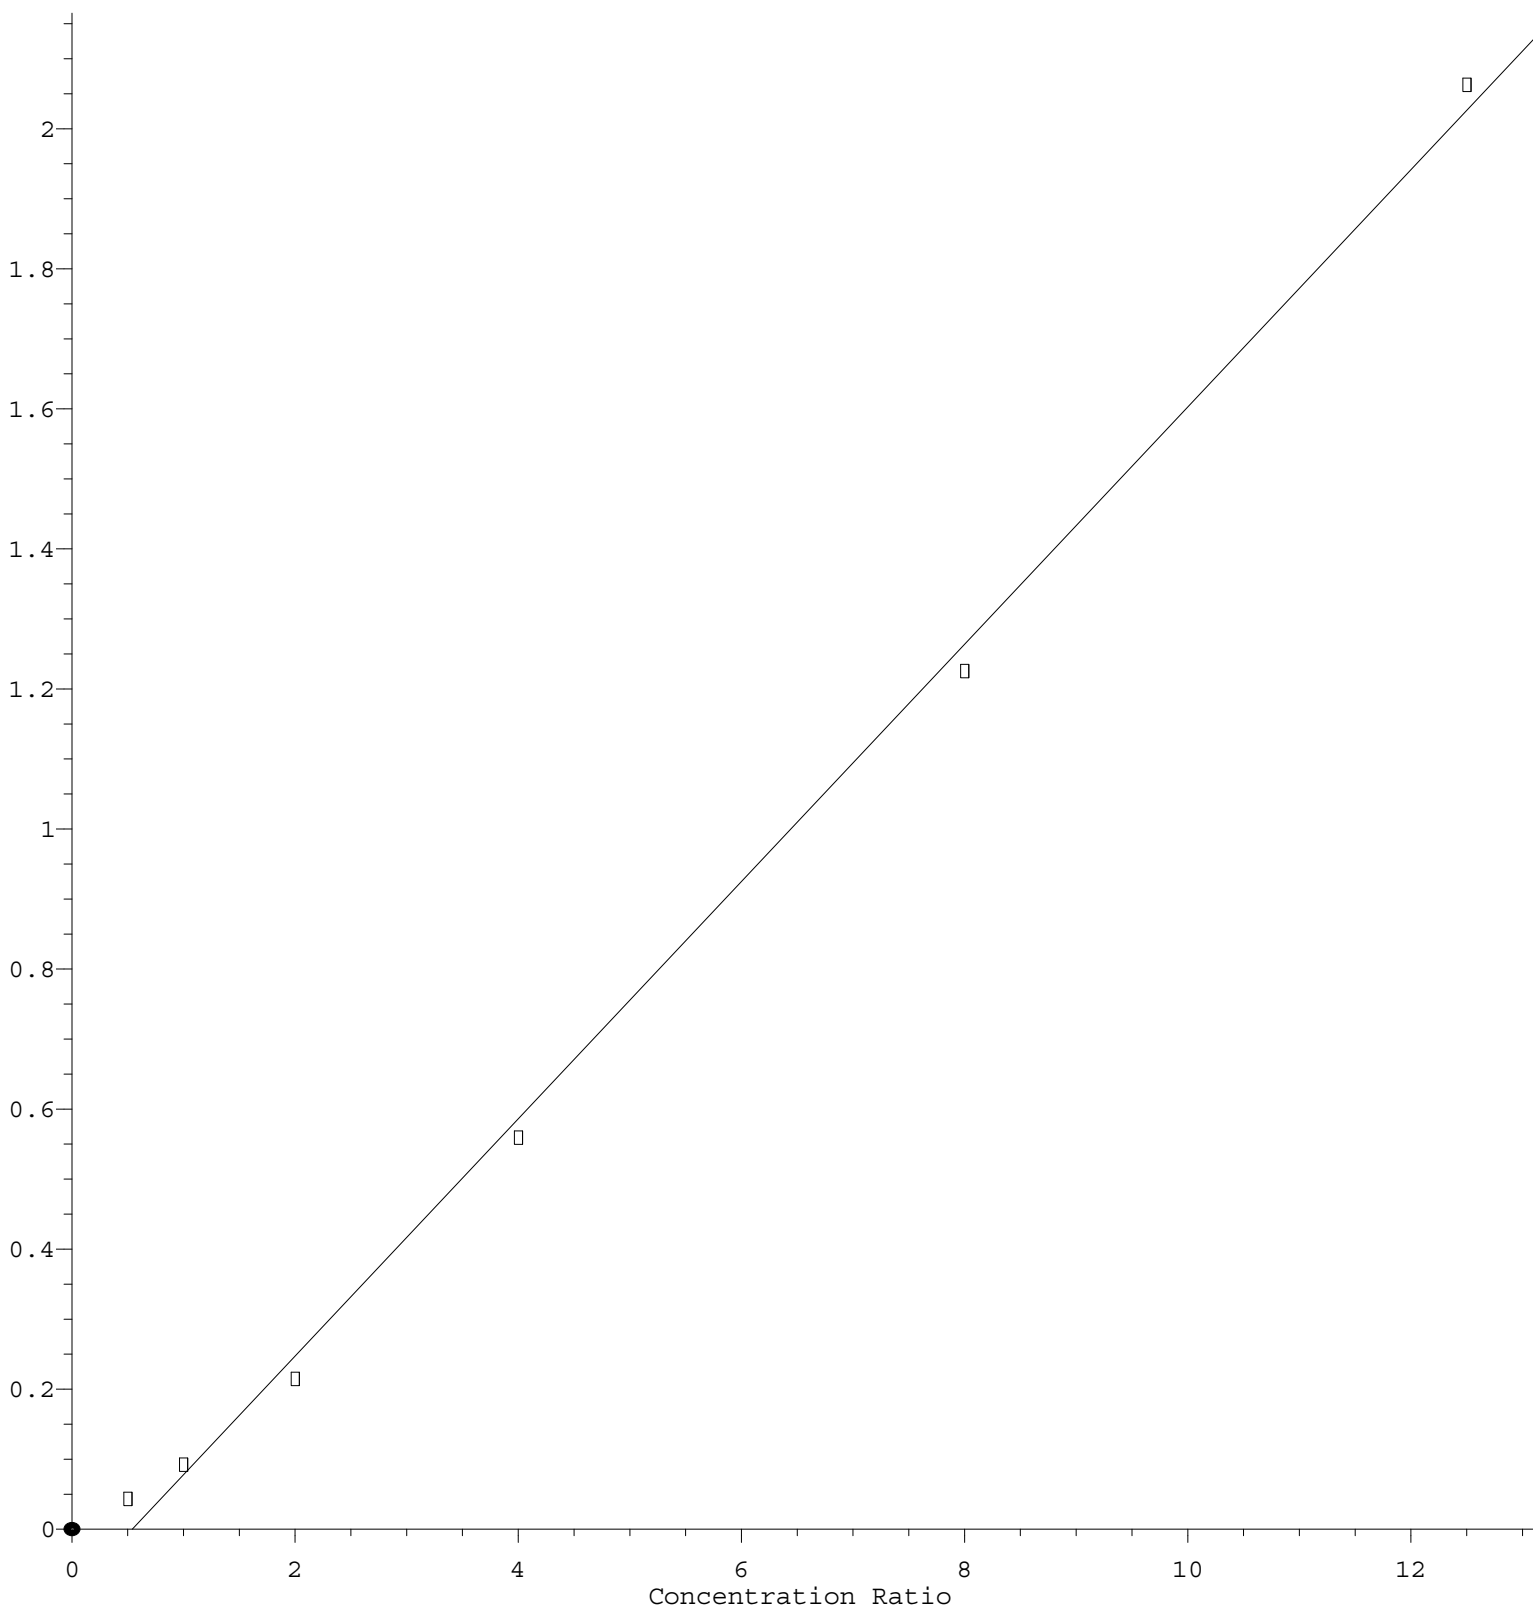

$$\text{Response} = 1.694\text{e-}001 * \text{Amt} - 9.118\text{e-}002$$


Coef of Det (r^2) = 0.997707 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA N\Methods\8270-SIM-BN060325.M

Calibration Table Last Updated: Wed Jun 04 01:52:03 2025

4,6-Dinitro-2-methylphenol

Response Ratio

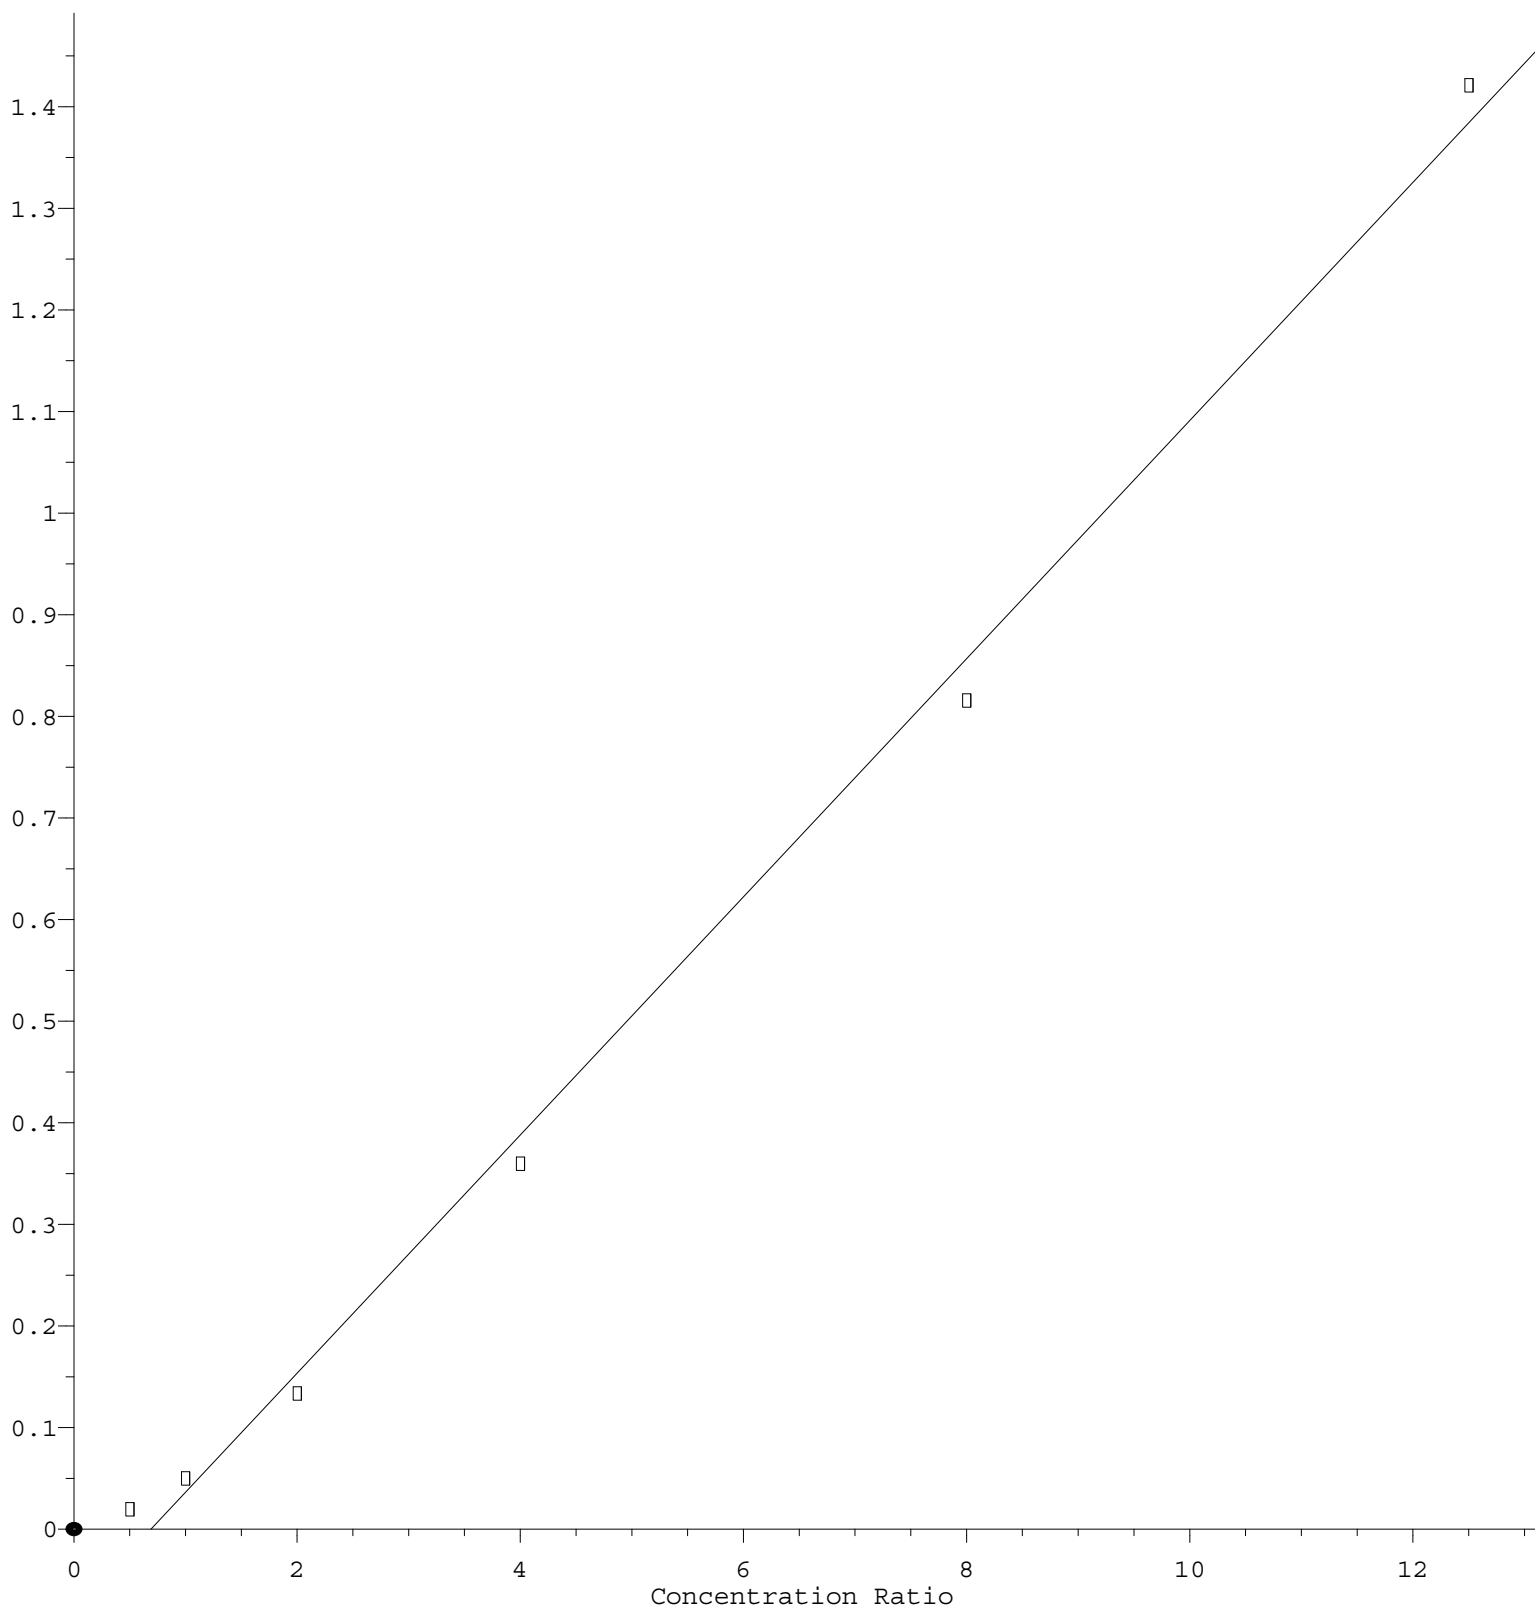

$$\text{Response} = 1.172\text{e-}001 * \text{Amt} - 8.037\text{e-}002$$

Coef of Det (r^2) = 0.995947 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA N\Methods\8270-SIM-BN060325.M

Calibration Table Last Updated: Wed Jun 04 01:52:03 2025