
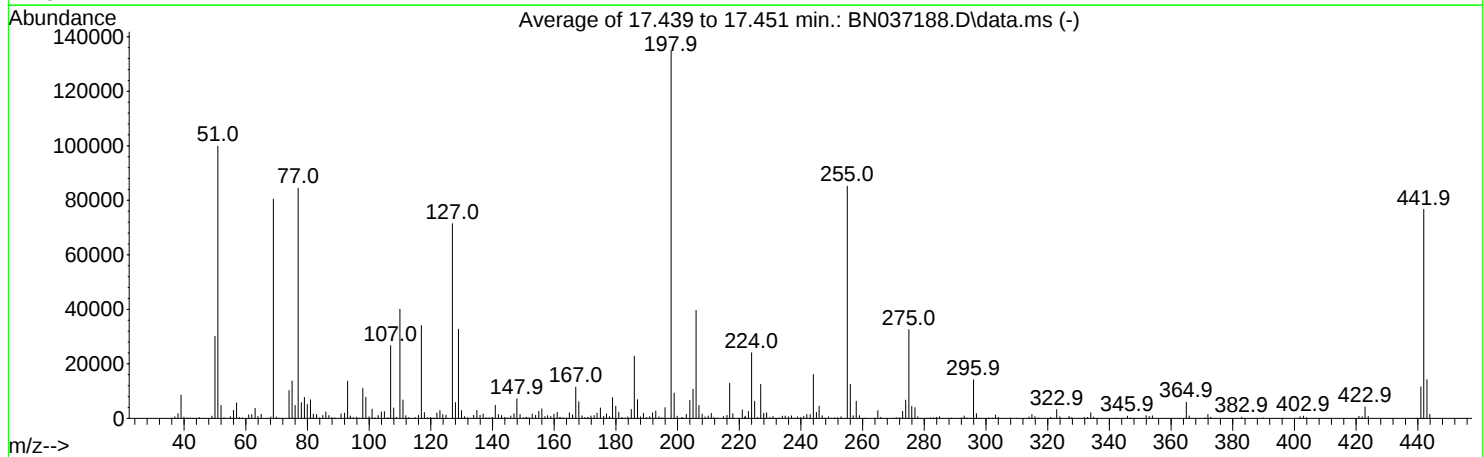


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037188.D
Acq On : 09 Jun 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 04 01:52:03 2025

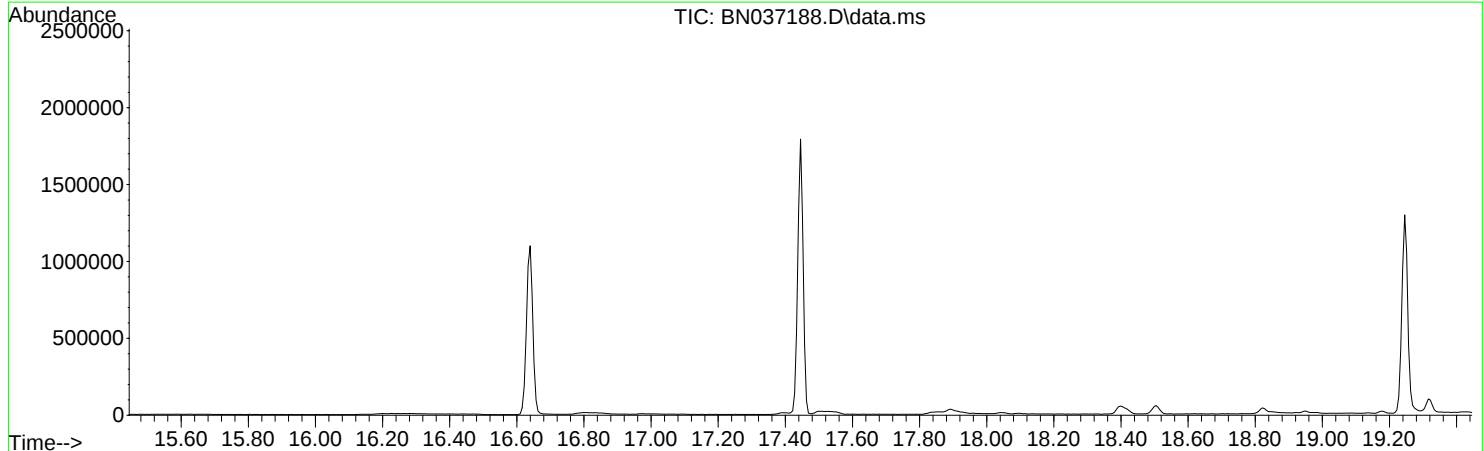




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	74.0	99844	PASS
68	69	0.00	2	0.7	559	PASS
69	198	0.00	100	59.6	80408	PASS
70	69	0.00	2	0.6	489	PASS
127	198	10	80	53.0	71472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134965	PASS
199	198	5	9	6.9	9301	PASS
275	198	10	60	24.1	32565	PASS
365	198	1	100	4.4	5933	PASS
441	198	0.01	100	8.6	11593	PASS
442	442	50	100	100.0	76653	PASS
443	442	15	24	18.5	14197	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037188.D
Acq On : 09 Jun 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 09 14:37:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

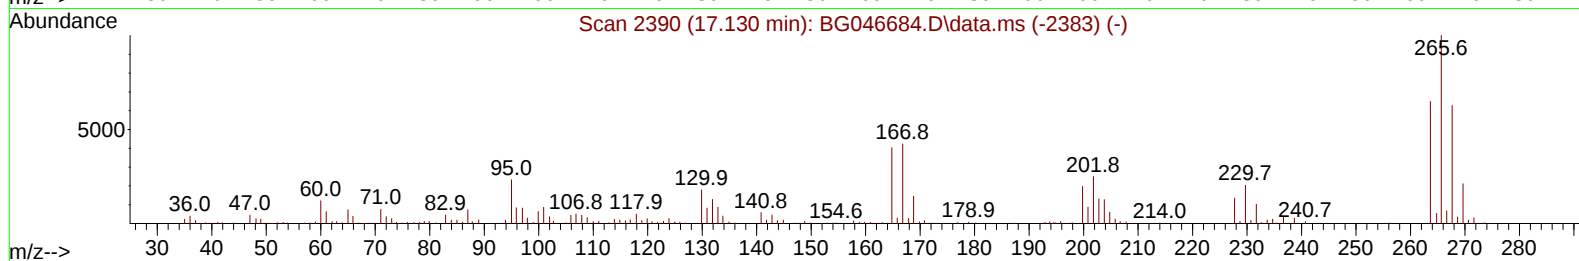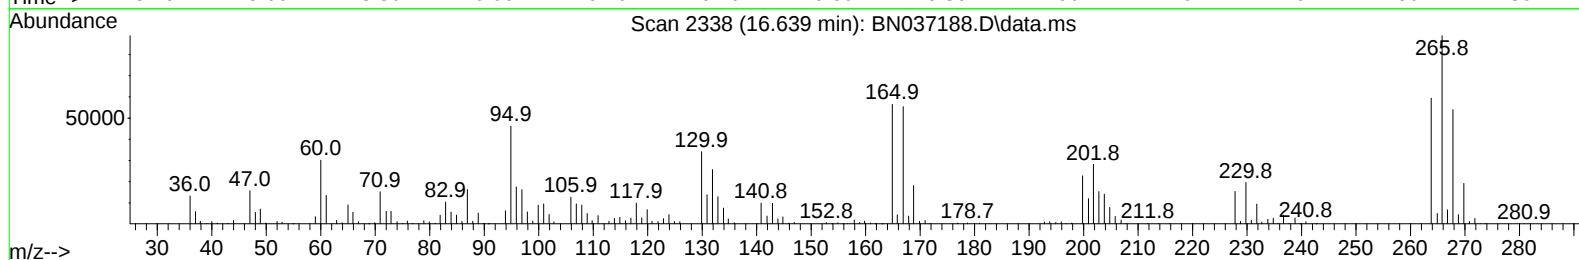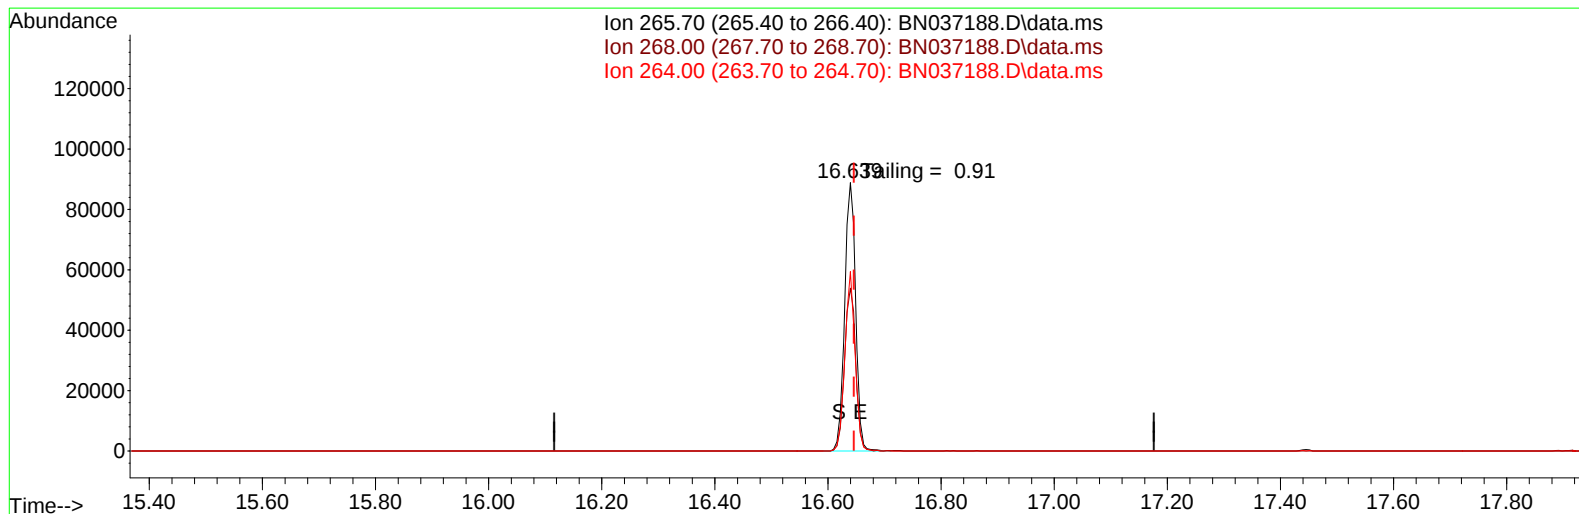

TIC: BN037188.D\data.ms

(70) Pentachlorophenol (C)

16.639min (-0.007) 18937.43 ng




response 119636

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.72
264.00	61.60	66.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037188.D
Acq On : 09 Jun 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 09 14:33:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

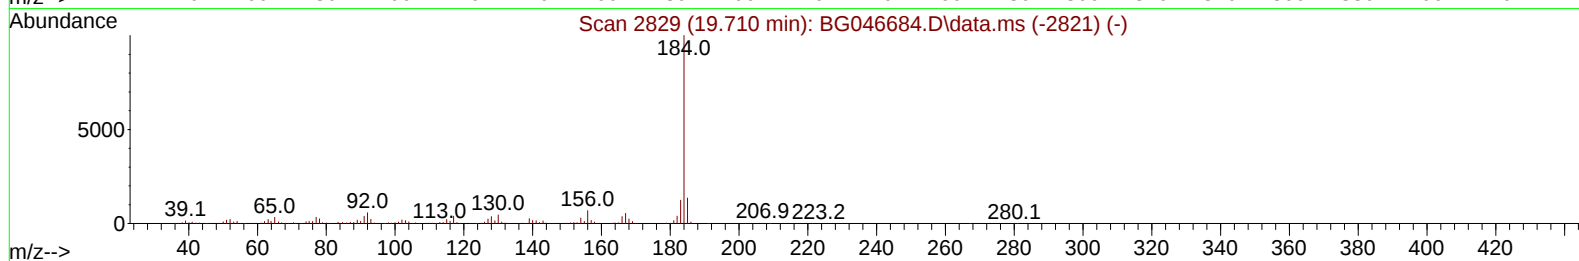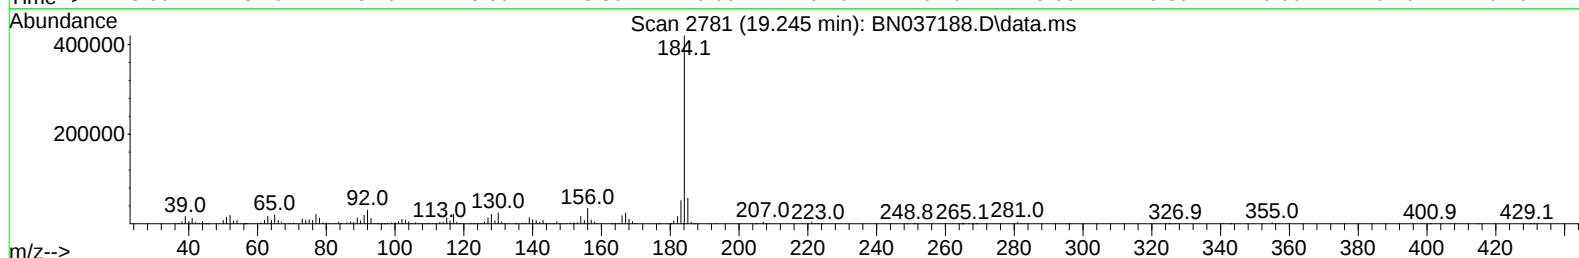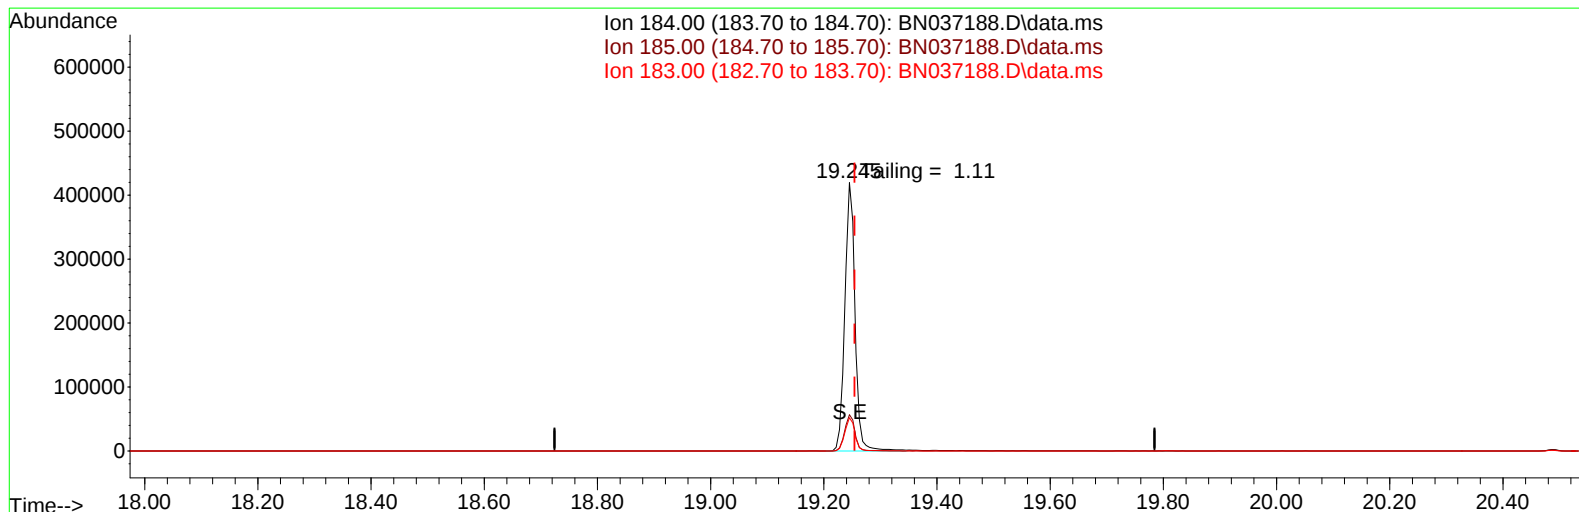

TIC: BN037188.D\data.ms

(77) Benzidine

19.245min (-0.009) 0.00 ng

response 528346

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.53
183.00	13.20	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2025	BNA_N	<u>BN037188.D</u>
Compound Name	Response	Retention Time
DDT	398680	20.486
DDD	7508	20.045
DDE	1010	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8518	407198	2.09

Instrument :
BNA_N
ClientSampleId :
DFTPP