
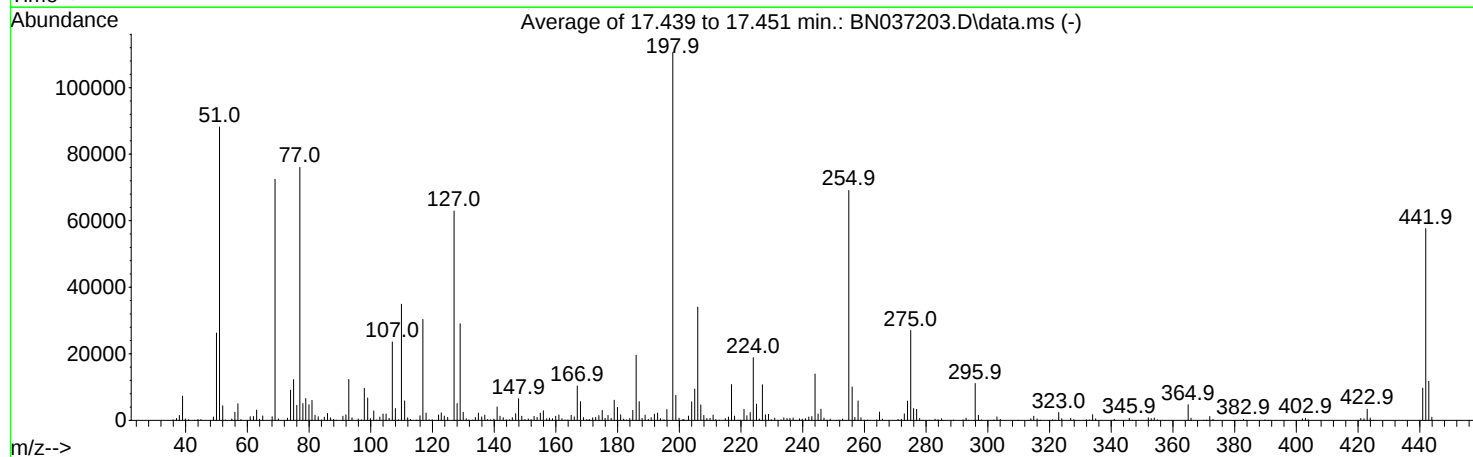


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037203.D
Acq On : 09 Jun 2025 22:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN060325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 04 01:52:03 2025

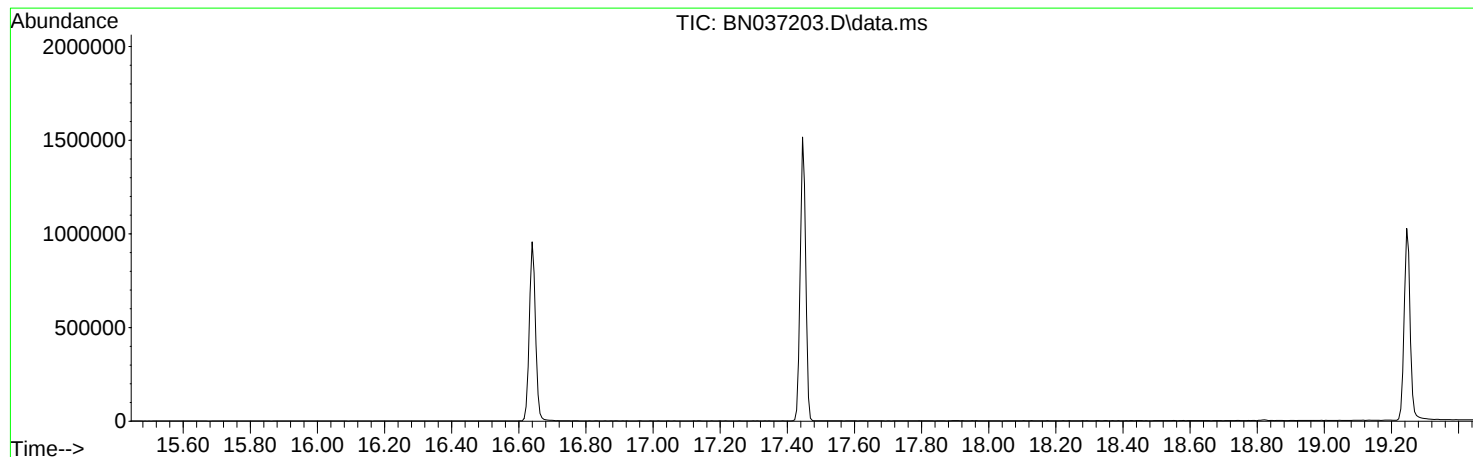




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	79.8	88176	PASS
68	69	0.00	2	1.5	1111	PASS
69	198	0.00	100	65.5	72469	PASS
70	69	0.00	2	0.6	429	PASS
127	198	10	80	56.9	62893	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	110557	PASS
199	198	5	9	6.8	7484	PASS
275	198	10	60	24.4	27021	PASS
365	198	1	100	4.3	4720	PASS
441	198	0.01	100	8.8	9692	PASS
442	442	50	100	100.0	57680	PASS
443	442	15	24	20.4	11739	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037203.D
Acq On : 09 Jun 2025 22:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 10 06:02:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 10 06:01:37 2025
Response via : Initial Calibration

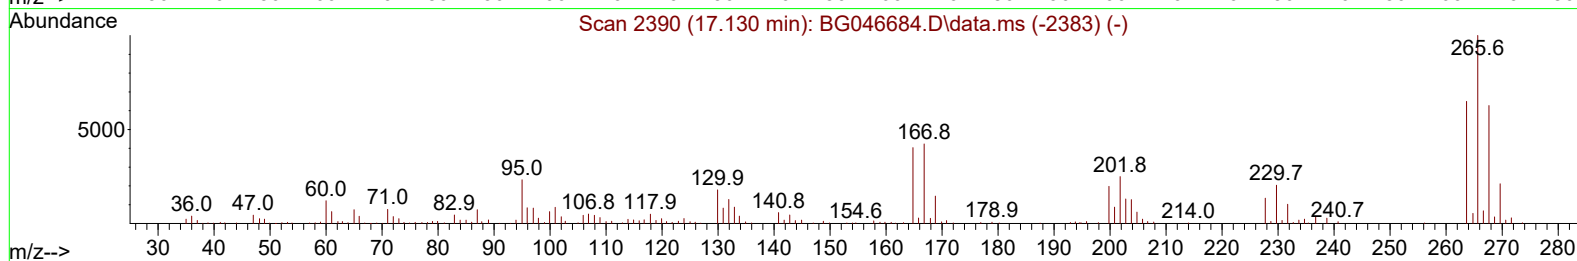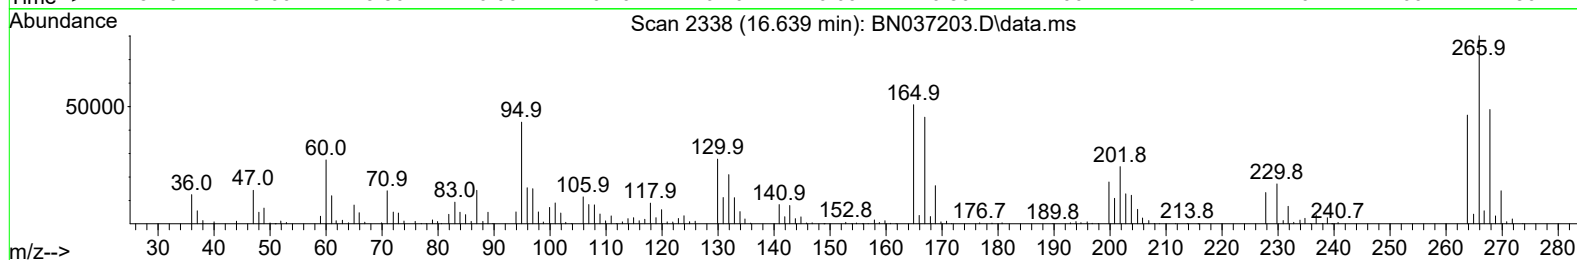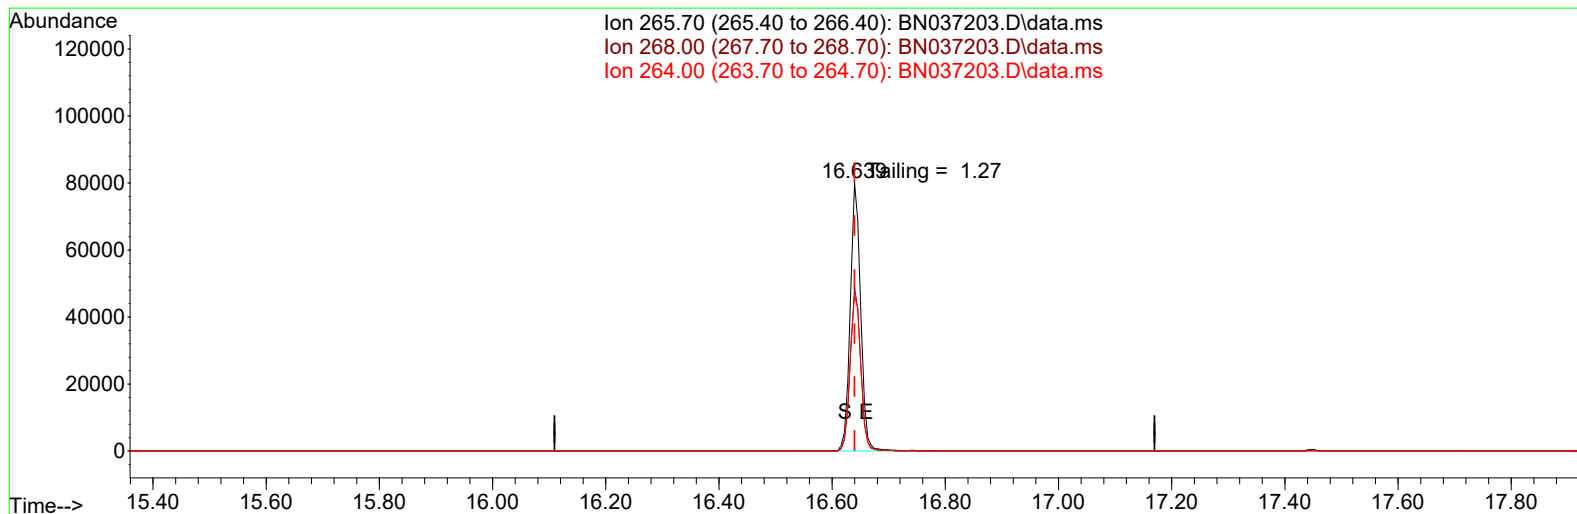

TIC: BN037203.D\data.ms

(70) Pentachlorophenol (C)

16.639min (0.000) 275.85 ng




response 102519

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.86
264.00	61.60	57.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037203.D
Acq On : 09 Jun 2025 22:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 10 06:02:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 10 06:01:37 2025
Response via : Initial Calibration

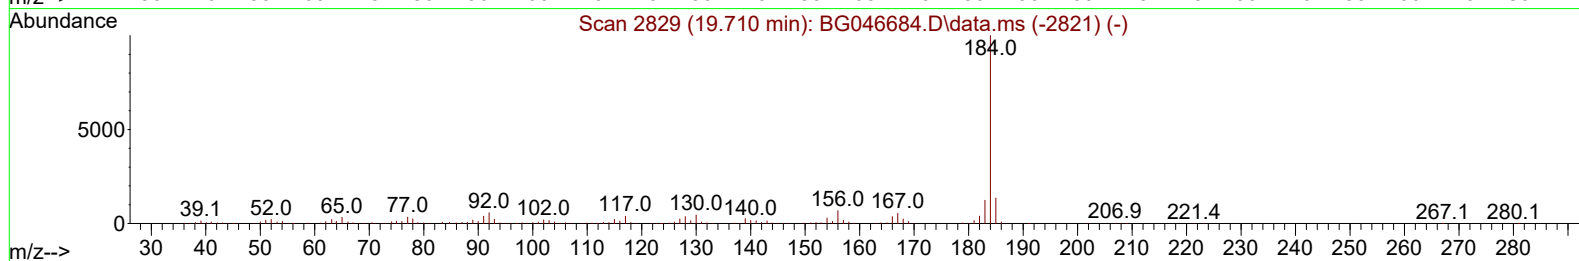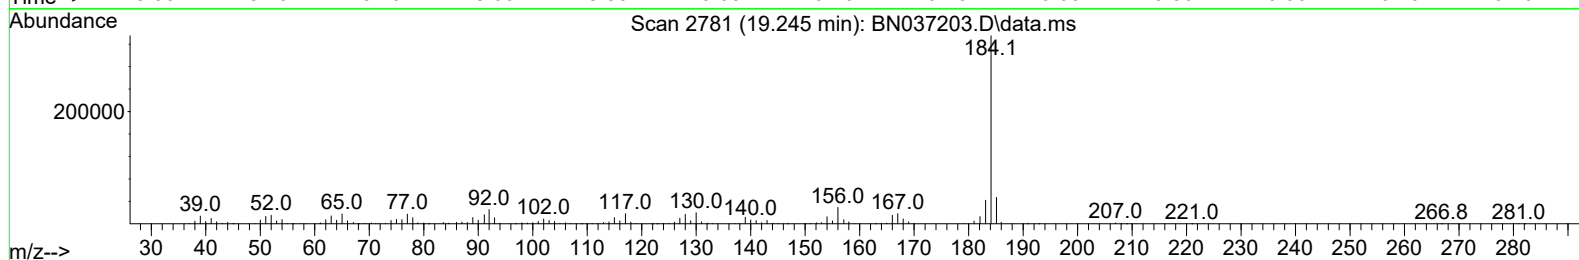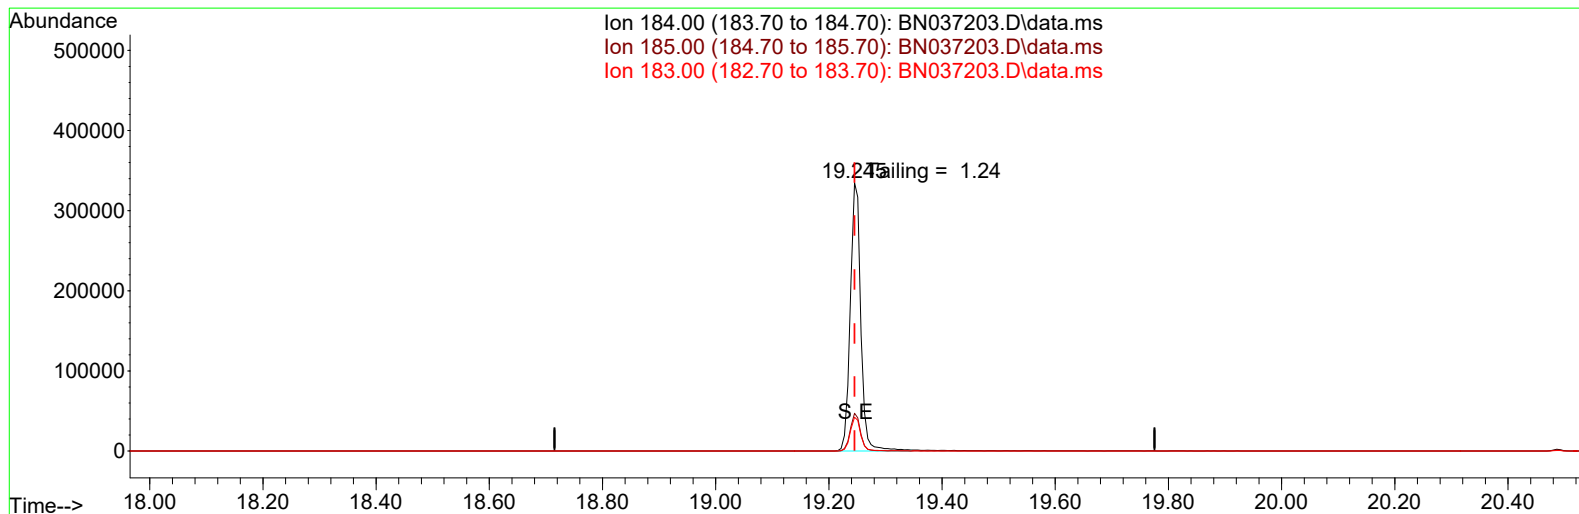

TIC: BN037203.D\data.ms

(77) Benzidine

19.245min (0.000) 0.00 ng

response 432254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.09
183.00	13.20	12.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2025	BNA_N	<u>BN037203.D</u>
Compound Name	Response	Retention Time
DDT	300238	20.486
DDD	4412	20.051
DDE	217	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4629	304867	1.52

Instrument :
BNA_N
ClientSampleId :
DFTPP