


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061125\
Data File : VN086939.D
Acq On : 11 Jun 2025 10:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

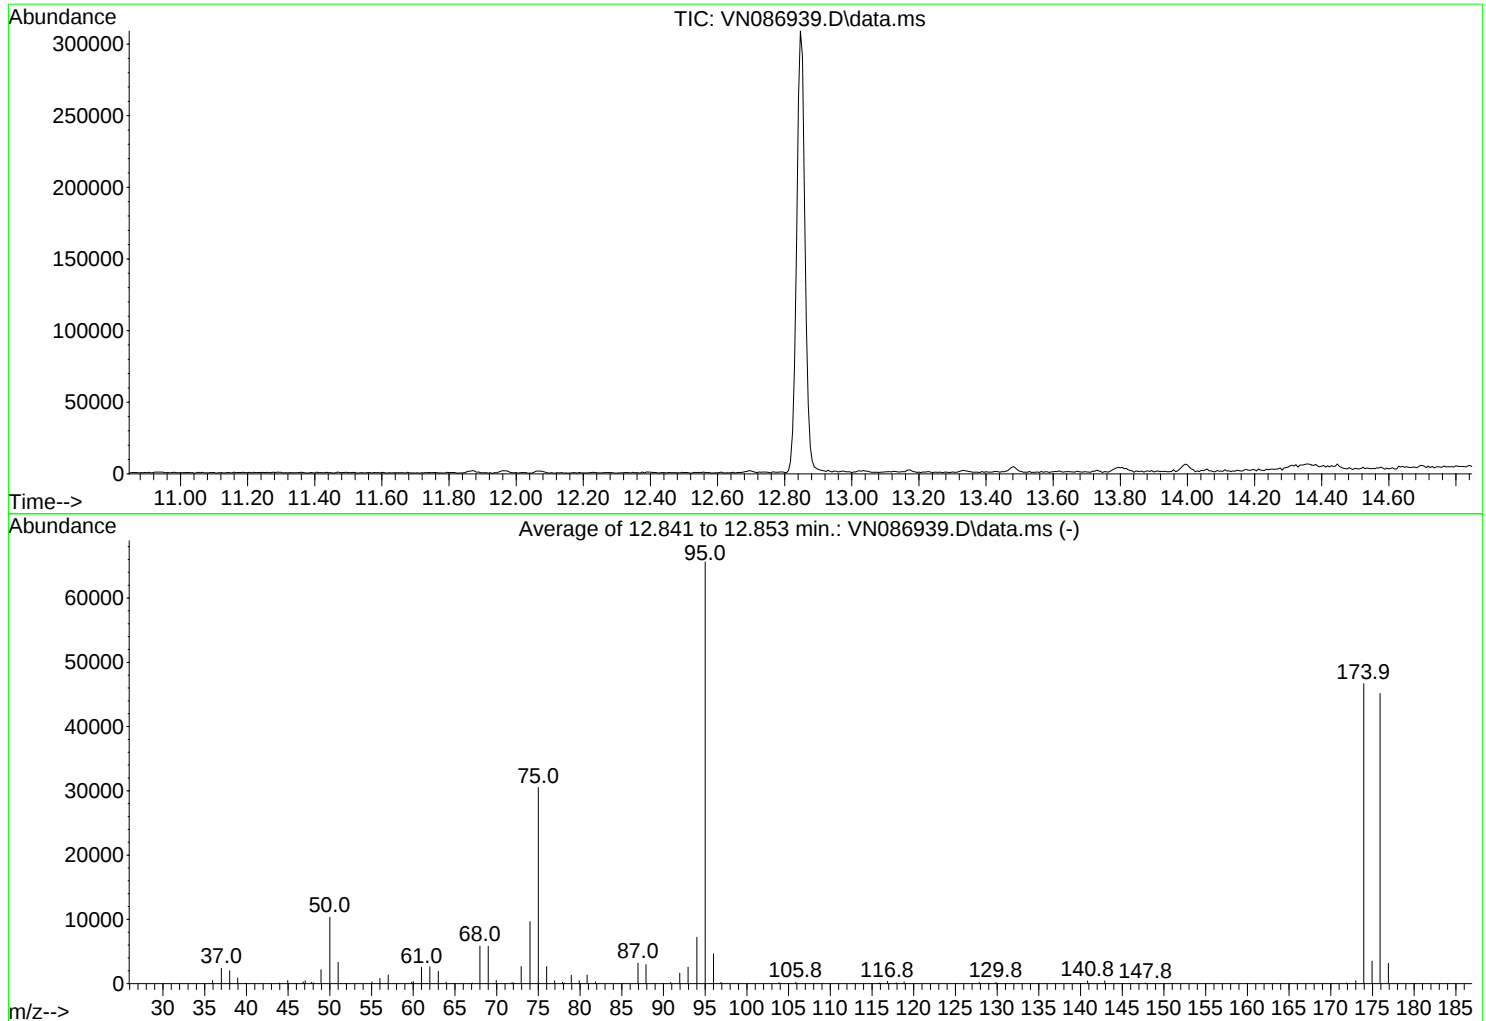

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	10335	PASS
75	95	30	60	46.5	30525	PASS
95	95	100	100	100.0	65627	PASS
96	95	5	9	7.1	4656	PASS
173	174	0.00	2	1.0	446	PASS
174	95	50	100	71.1	46675	PASS
175	174	5	9	7.5	3520	PASS
176	174	95	101	96.8	45165	PASS
177	176	5	9	7.0	3156	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	494	48.95	2163	63.00	1912	74.00	964
37.00	2403	50.00	10335	63.95	253	75.00	3052
38.00	2017	51.00	3344	64.90	57	76.00	263
38.95	867	51.90	62	66.80	56	76.95	44
39.90	50	55.05	275	67.10	81	77.90	239
43.95	113	56.00	819	68.00	5863	78.10	106
44.95	490	57.00	1338	69.00	5810	78.95	1316
46.80	268	59.80	202	69.95	516	79.90	417
47.05	461	60.00	356	71.85	193	80.85	1355
47.80	192	61.00	2534	72.10	100	81.85	284
48.00	136	62.00	2606	72.95	2656	86.95	3197

Average of 12.841 to 12.853 min.: VN086939.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	2968	115.90	106	171.90	125		
90.85	197	116.85	346	173.00	446		
91.95	1650	117.90	153	173.95	46675		
92.95	2576	118.85	289	174.95	3520		
94.00	7225	127.85	197	175.90	45165		
95.00	65627	129.00	74	176.90	3156		
96.00	4656	129.85	202				
96.90	194	140.85	437				
103.85	167	142.90	425				
105.85	223	147.00	54				
115.70	63	147.80	119				

Instrument :

MSVOA_N

ClientSampleId :

BFB