

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046602.D
 Acq On : 10 Jun 2025 14:59
 Operator : JC/MD
 Sample : Q2230-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-MW01-060425

Quant Time: Jun 11 01:48:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	112673	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	225413	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	232357	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	117788	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	99814	49.793	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	99.580%		
35) Dibromofluoromethane	5.403	113	82766	49.929	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.860%		
50) Toluene-d8	8.653	98	296381	54.231	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	108.460%		
62) 4-Bromofluorobenzene	11.079	95	126825	56.088	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	112.180%		
Target Compounds						Qvalue
3) Chloromethane	1.307	50	385	0.270	ug/l	90
16) Acetone	2.392	43	36663	50.314	ug/l	95
17) Carbon Disulfide	2.532	76	238	0.286	ug/l #	76
25) 2-Butanone	4.593	43	9858	8.834	ug/l	91
28) Bromochloromethane	5.117	49	531	0.386	ug/l #	17
30) Chloroform	5.111	83	7992	2.642	ug/l	90
31) Cyclohexane	5.489	56	1227	0.527	ug/l	96
36) 1,1-Dichloropropene	5.562	75	10187	4.302	ug/l #	52
37) Ethyl Acetate	4.593	43	9858	4.266	ug/l #	70
38) Carbon Tetrachloride	5.562	117	13249	4.996	ug/l #	17
39) Methylcyclohexane	7.385	83	2716	0.972	ug/l	91
40) Benzene	6.062	78	2386	0.358	ug/l #	73
52) Toluene	8.726	92	6540	1.597	ug/l	98
55) 1,1,2-Trichloroethane	9.110	97	901	0.548	ug/l #	15
67) Ethyl Benzene	10.195	91	36138	3.788	ug/l	95
68) m/p-Xylenes	10.299	106	55836	16.134	ug/l	98
69) o-Xylene	10.640	106	66951	20.001	ug/l	99
70) Styrene	10.640	104	3115	0.544	ug/l #	1
73) Isopropylbenzene	10.963	105	12369	1.336	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	69321	27.785	ug/l #	36
78) n-propylbenzene	11.305	91	28458	2.539	ug/l	99
79) 2-Chlorotoluene	11.378	91	18979	2.808	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.451	105	56897	7.374	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	69321	80.149	ug/l #	1
82) 4-Chlorotoluene	11.451	91	6636	0.828	ug/l #	48
83) tert-Butylbenzene	11.750	119	23460	2.987	ug/l #	57
84) 1,2,4-Trimethylbenzene	11.750	105	203323	26.048	ug/l	98
85) sec-Butylbenzene	11.890	105	10047	0.995	ug/l	88
86) p-Isopropyltoluene	12.006	119	6693	0.795	ug/l	90
89) n-Butylbenzene	12.329	91	17920	2.169	ug/l #	39
90) Hexachloroethane	12.530	117	3066	2.050	ug/l #	19
92) 1,2-Dibromo-3-Chloropr...	12.920	75	341	0.514	ug/l #	10
95) Naphthalene	13.774	128	32304	3.707	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046602.D
Acq On : 10 Jun 2025 14:59
Operator : JC/MD
Sample : Q2230-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425

Quant Time: Jun 11 01:48:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration




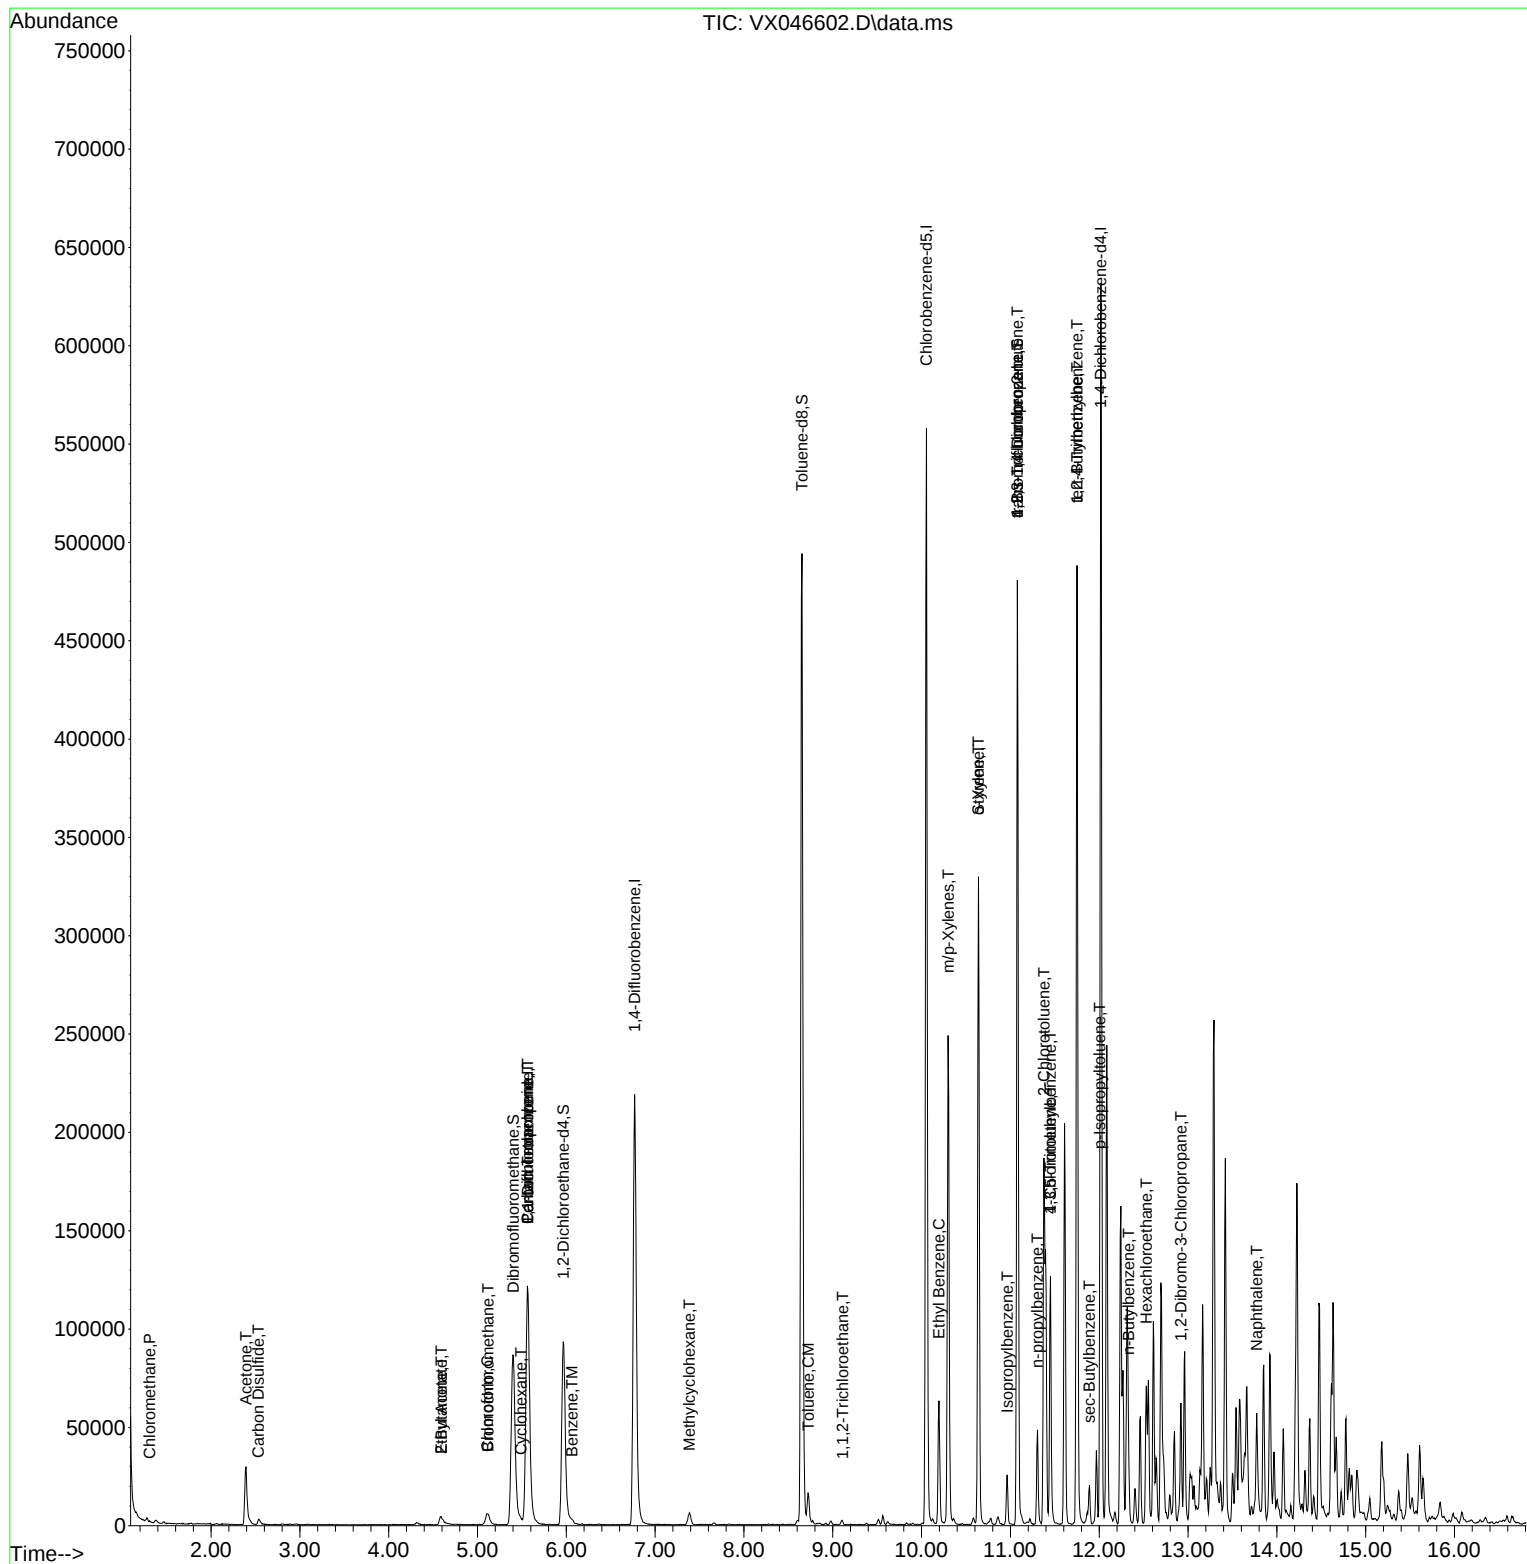




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:168 Resp: 112673
Ion Ratio Lower Upper
168 100
99 70.8 54.9 82.3

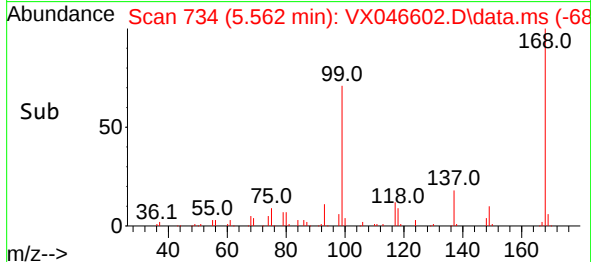

#3
Chloromethane
Concen: 0.270 ug/l
RT: 1.307 min Scan# 36
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 50 Resp: 385
Ion Ratio Lower Upper
50 100
52 37.2 25.4 38.2


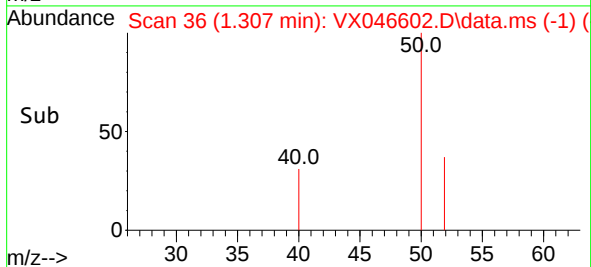






#16
Acetone
Concen: 50.314 ug/l
RT: 2.392 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion: 43 Resp: 36663
Ion Ratio Lower Upper
43 100
58 28.8 21.2 31.8

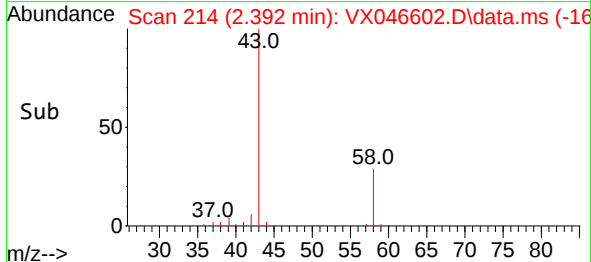

#17
Carbon Disulfide
Concen: 0.286 ug/l
RT: 2.532 min Scan# 237
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 76 Resp: 238
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#




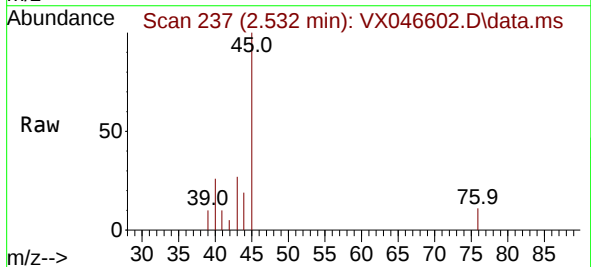


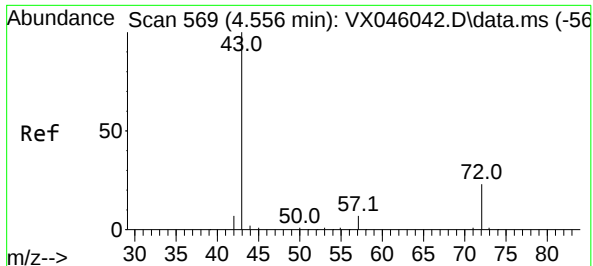

#25
2-Butanone
Concen: 8.834 ug/l
RT: 4.593 min Scan# 51
Delta R.T. 0.019 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion: 43 Resp: 9858
Ion Ratio Lower Upper
43 100
72 27.2 18.4 27.6

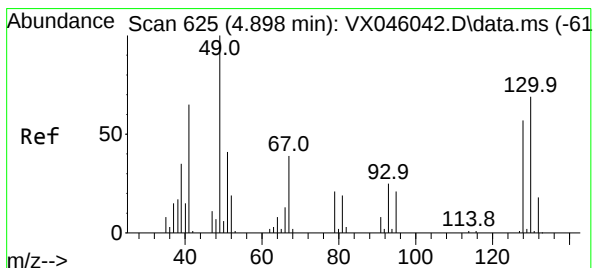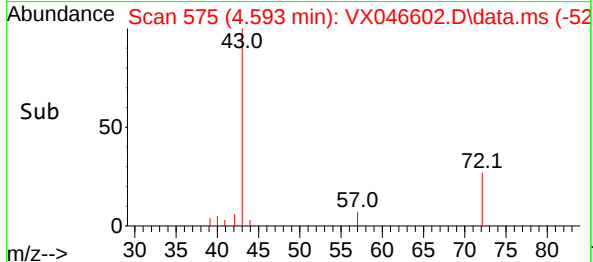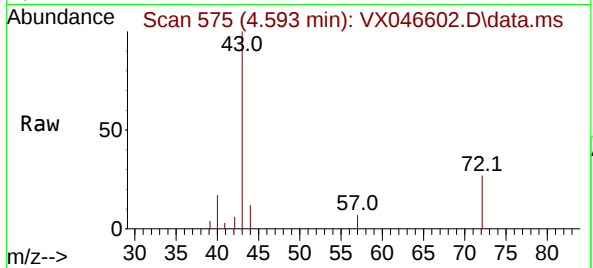

#28
Bromochloromethane
Concen: 0.386 ug/l
RT: 5.117 min Scan# 661
Delta R.T. 0.201 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 49 Resp: 531
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.0
130 0.0 56.2 84.2#


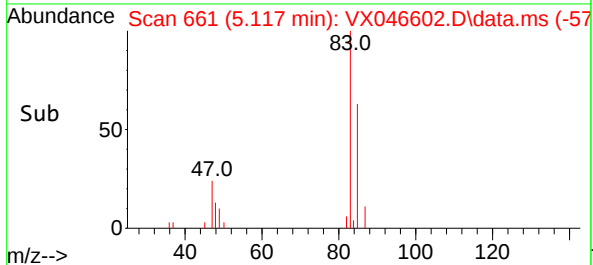

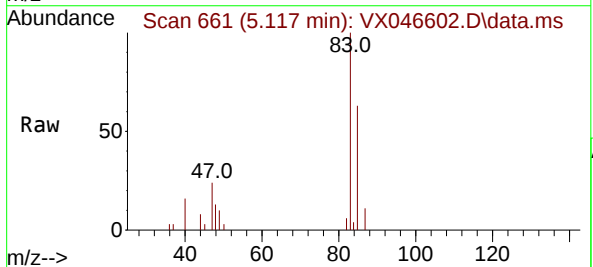




#30
Chloroform
Concen: 2.642 ug/l
RT: 5.111 min Scan# 611
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion: 83 Resp: 7992
Ion Ratio Lower Upper
83 100
85 54.1 49.3 73.9

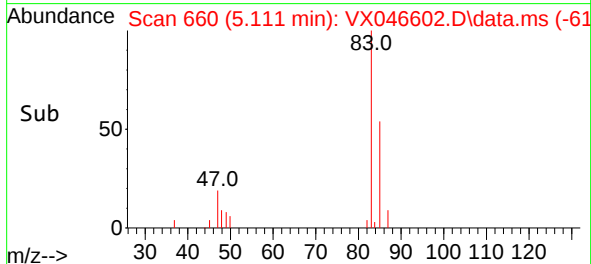

#31
Cyclohexane
Concen: 0.527 ug/l
RT: 5.489 min Scan# 722
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 56 Resp: 1227
Ion Ratio Lower Upper
56 100
69 24.8 24.4 36.6
84 82.6 66.9 100.3


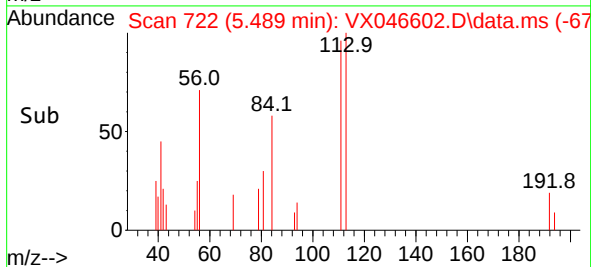






#33
 1,2-Dichloroethane-d4
 Concen: 49.793 ug/l
 RT: 5.964 min Scan# 80
 Delta R.T. -0.006 min
 Lab File: VX046602.D
 Acq: 10 Jun 2025 14:59




Instrument :
 MSVOA_X
 ClientSampleId :
 GW-MW01-060425


Tgt Ion: 65 Resp: 99814
 Ion Ratio Lower Upper
 65 100
 67 51.1 0.0 99.0

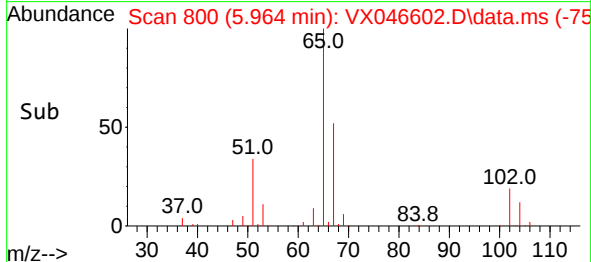

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.769 min Scan# 932
 Delta R.T. -0.006 min
 Lab File: VX046602.D
 Acq: 10 Jun 2025 14:59

Tgt Ion: 114 Resp: 225413
 Ion Ratio Lower Upper
 114 100
 63 22.9 0.0 49.2
 88 16.7 0.0 33.6


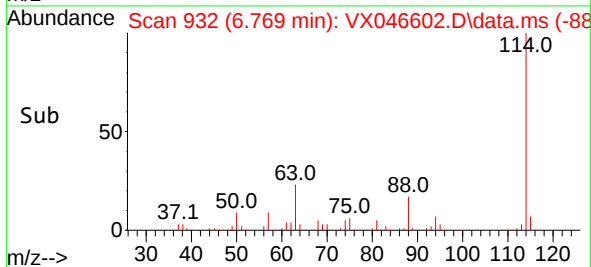




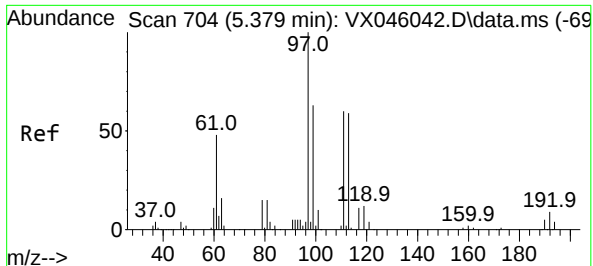

#35
Dibromofluoromethane
Concen: 49.929 ug/l
RT: 5.403 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:113 Resp: 82766
Ion Ratio Lower Upper
113 100
111 102.4 83.1 124.7
192 16.9 13.3 19.9

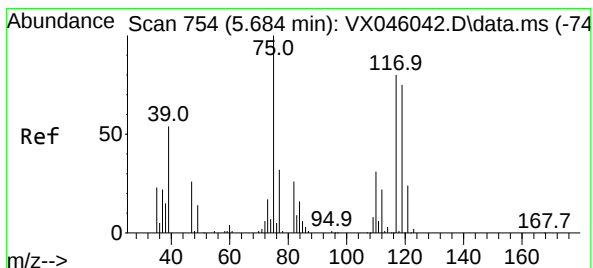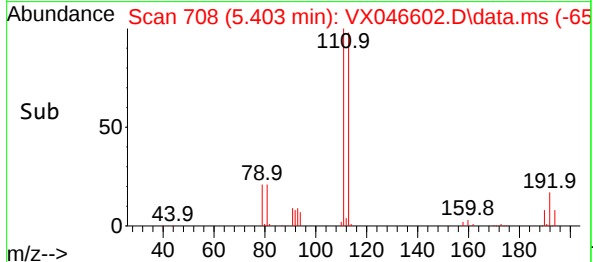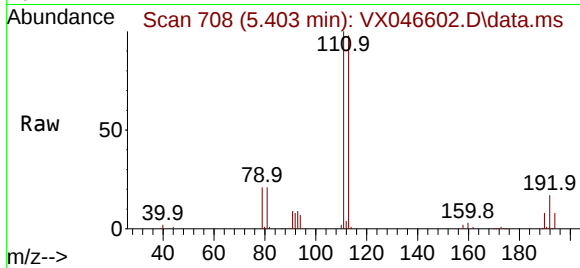

#36
1,1-Dichloropropene
Concen: 4.302 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.152 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 75 Resp: 10187
Ion Ratio Lower Upper
75 100
110 9.4 16.3 48.9#
77 0.0 24.3 36.5#

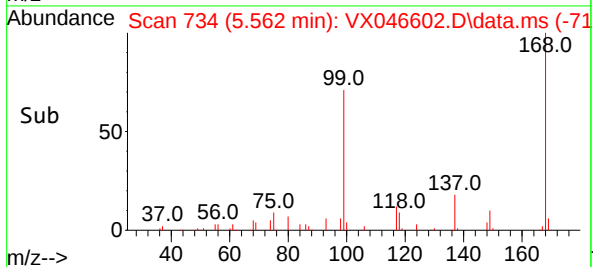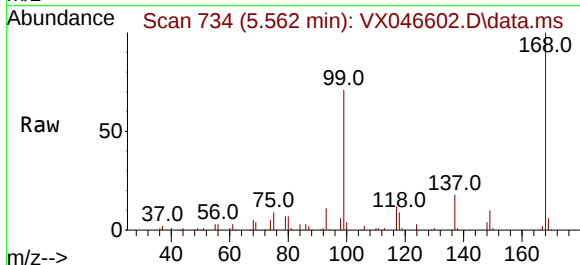



#37

Ethyl Acetate

Concen: 4.266 ug/l

RT: 4.593 min Scan# 51

Delta R.T. -0.140 min

Lab File: VX046602.D

Acq: 10 Jun 2025 14:59

Instrument :

MSVOA_X

ClientSampleId :

GW-MW01-060425





Tgt Ion: 43 Resp: 9858

Ion Ratio Lower Upper

43 100

61 0.0 10.3 15.5#

70 0.0 7.9 11.9#

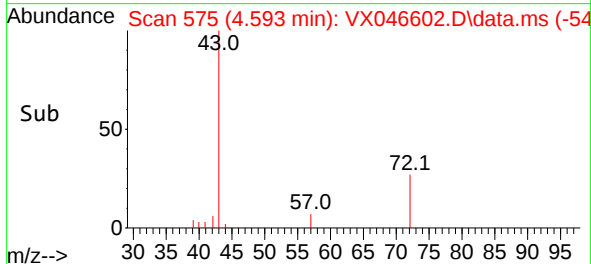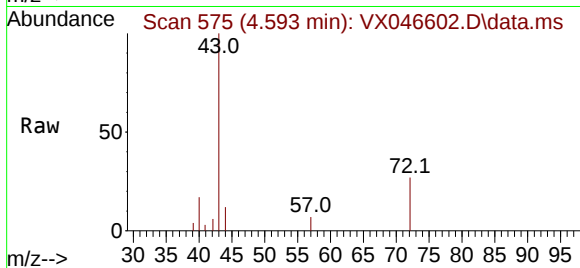

#38

Carbon Tetrachloride

Concen: 4.996 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.134 min

Lab File: VX046602.D

Acq: 10 Jun 2025 14:59




Tgt Ion: 117 Resp: 13249


Ion Ratio Lower Upper

117 100

119 5.1 75.2 112.8#

121 0.0 24.2 36.4#



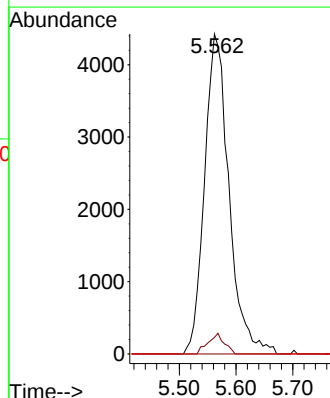
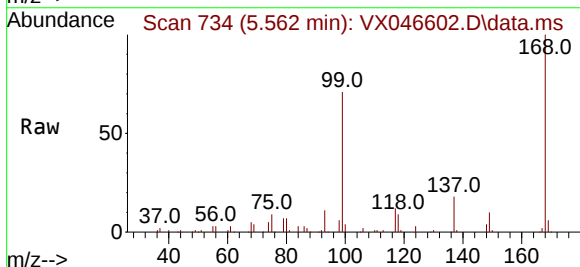


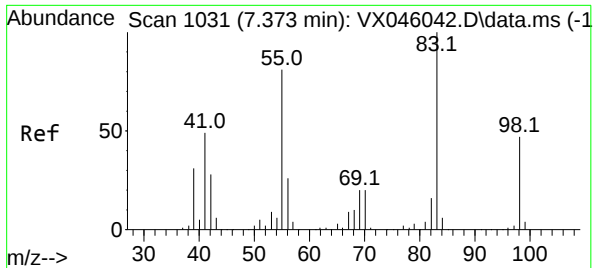

#39
Methylcyclohexane
Concen: 0.972 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.006 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion: 83 Resp: 2716
Ion Ratio Lower Upper
83 100
55 93.2 64.7 97.1
98 45.6 37.4 56.2

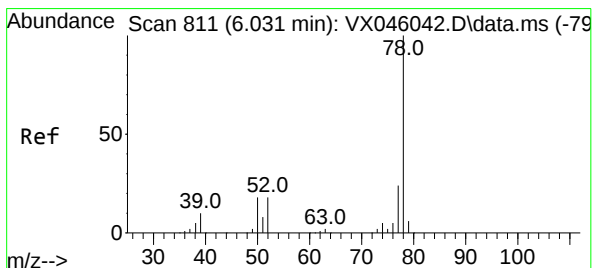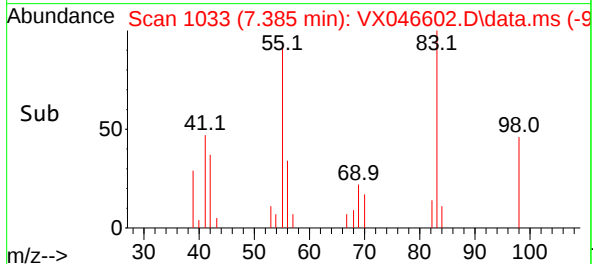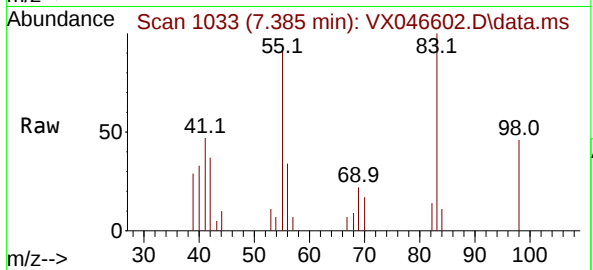

#40
Benzene
Concen: 0.358 ug/l
RT: 6.062 min Scan# 816
Delta R.T. 0.006 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 78 Resp: 2386
Ion Ratio Lower Upper
78 100
77 10.5 19.0 28.4#


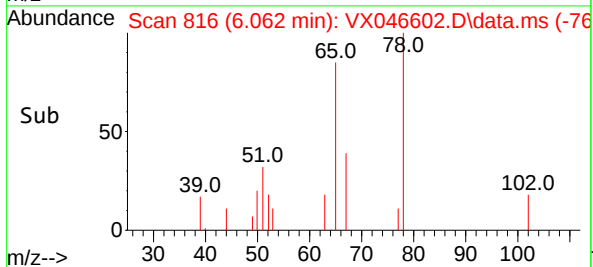

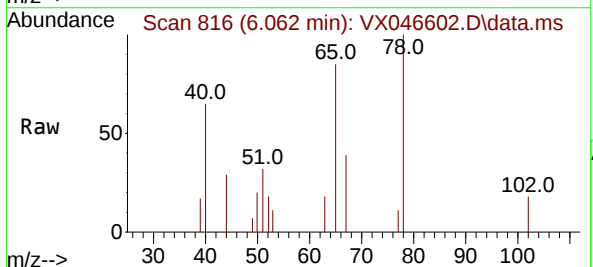


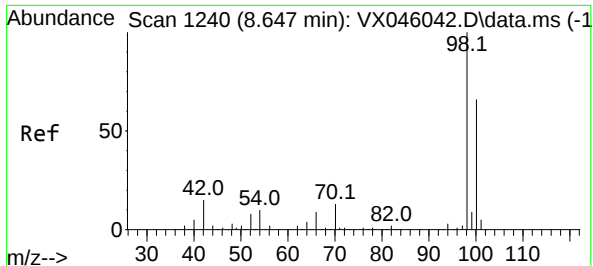

#50
Toluene-d8
Concen: 54.231 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion: 98 Resp: 296381
Ion Ratio Lower Upper
98 100
100 66.1 53.5 80.3

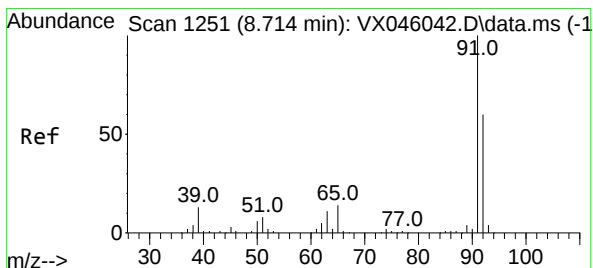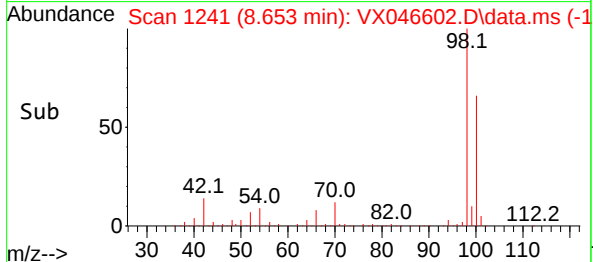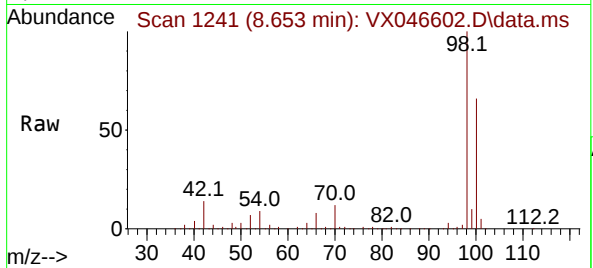

#52
Toluene
Concen: 1.597 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 92 Resp: 6540
Ion Ratio Lower Upper
92 100
91 173.7 136.6 205.0


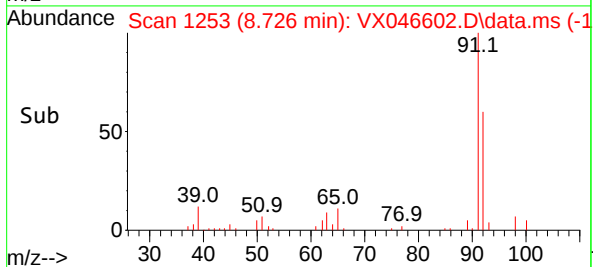

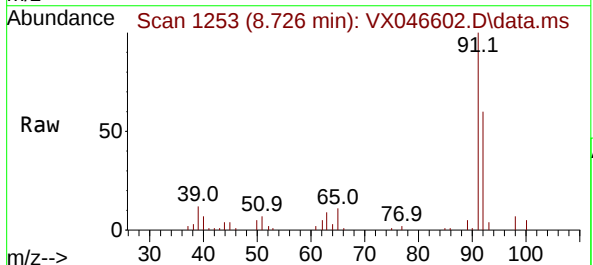




#55
1,1,2-Trichloroethane
Concen: 0.548 ug/l
RT: 9.110 min Scan# 11
Delta R.T. -0.043 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:	97	Resp:	901
Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.0	103.6#
85	0.0	44.3	66.5#
99	0.0	47.8	71.6#

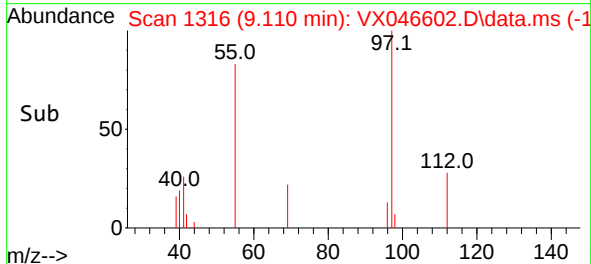

#62
4-Bromofluorobenzene
Concen: 56.088 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion:	95	Resp:	126825
Ion	Ratio	Lower	Upper
95	100		
174	70.4	0.0	135.8
176	67.3	0.0	131.4


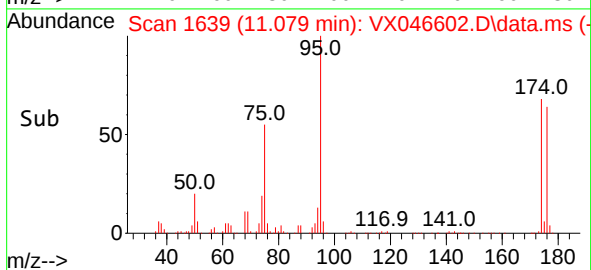

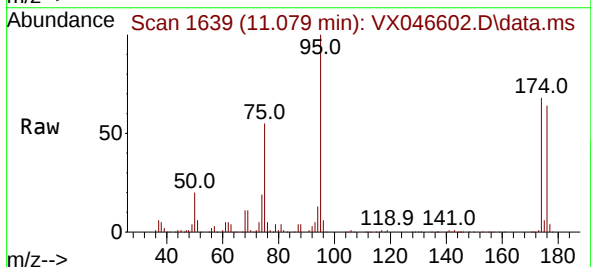




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:117 Resp: 232357
Ion Ratio Lower Upper
117 100
82 58.1 50.6 76.0
119 32.8 25.8 38.6

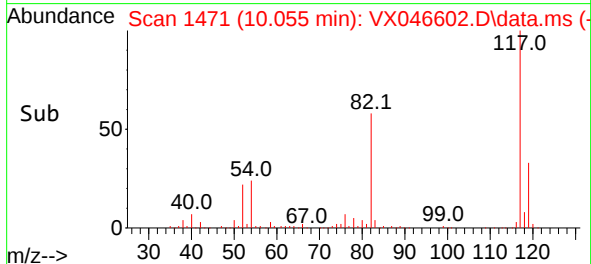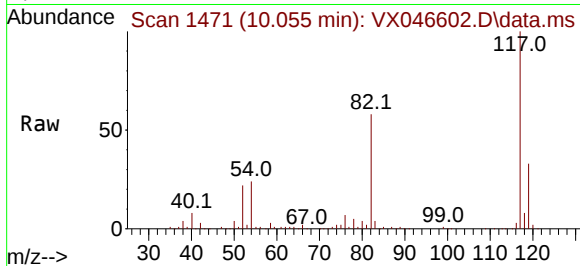

#67
Ethyl Benzene
Concen: 3.788 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 91 Resp: 36138
Ion Ratio Lower Upper
91 100
106 31.7 23.4 35.2



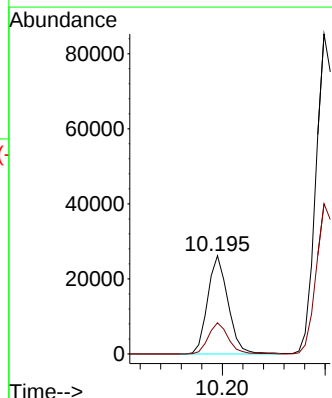
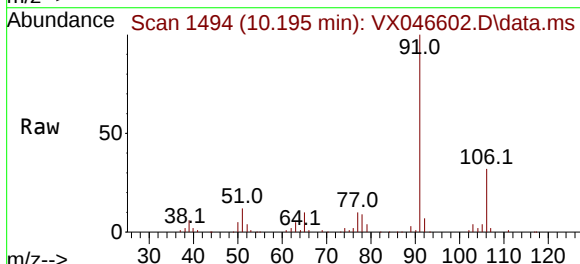




#68
m/p-Xylenes
Concen: 16.134 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:106 Resp: 55836
Ion Ratio Lower Upper
106 100
91 210.7 171.2 256.8

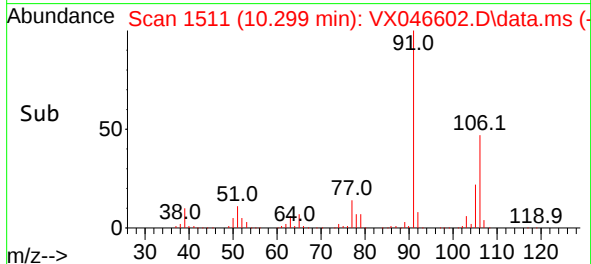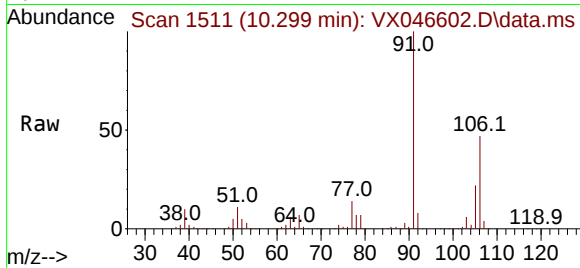

#69
o-Xylene
Concen: 20.001 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion:106 Resp: 66951
Ion Ratio Lower Upper
106 100
91 227.4 112.7 338.1

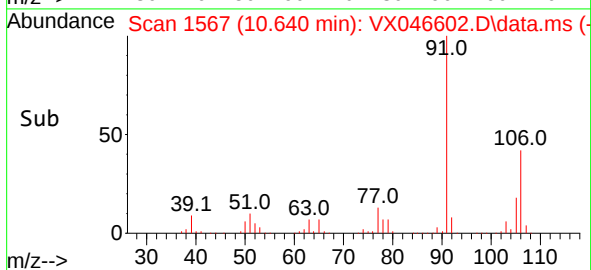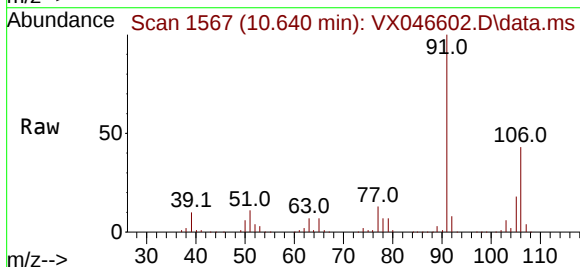



#70

Styrene

Concen: 0.544 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.018 min

Lab File: VX046602.D

Acq: 10 Jun 2025 14:59

Instrument :

MSVOA_X

ClientSampleId :

GW-MW01-060425





Tgt Ion:104 Resp: 3115

Ion Ratio Lower Upper

104 100

78 358.7 45.7 68.5#

103 284.7 43.7 65.5#

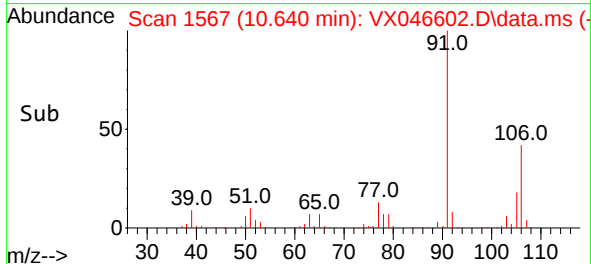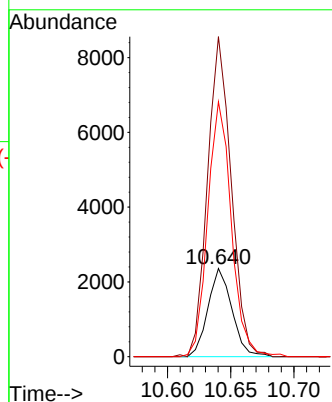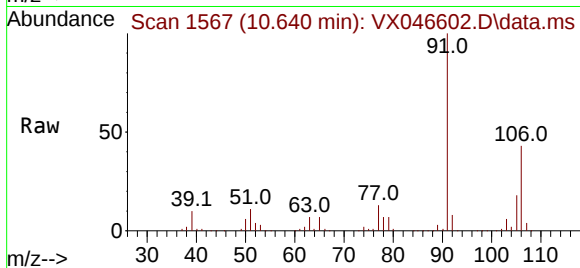

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX046602.D

Acq: 10 Jun 2025 14:59




Tgt Ion:152 Resp: 117788


Ion Ratio Lower Upper

152 100

115 65.0 46.9 140.7

150 159.4 0.0 351.0

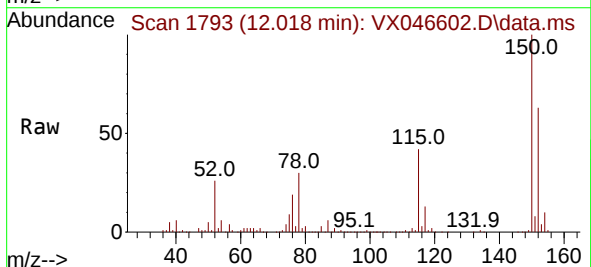

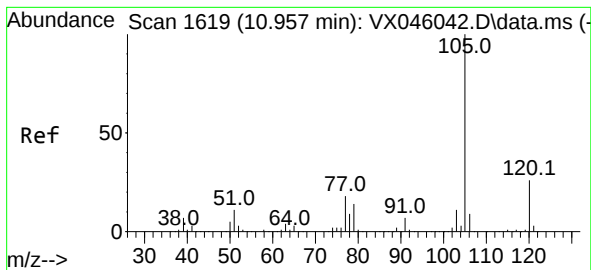

#73

Isopropylbenzene

Concen: 1.336 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX046602.D

Acq: 10 Jun 2025 14:59

Instrument :

MSVOA_X

ClientSampleId :





GW-MW01-060425

Tgt Ion:105 Resp: 12369

Ion Ratio Lower Upper

105 100

120 25.0 12.8 38.4

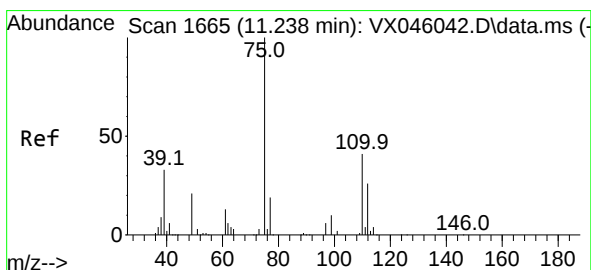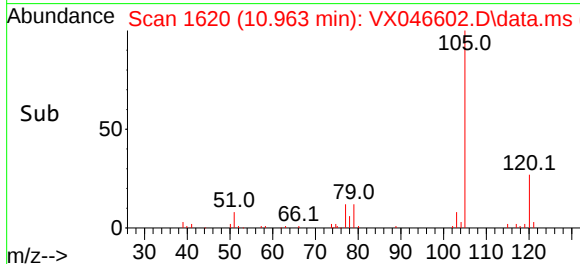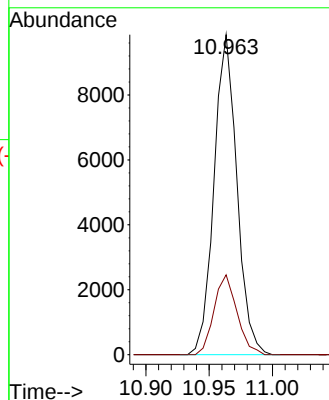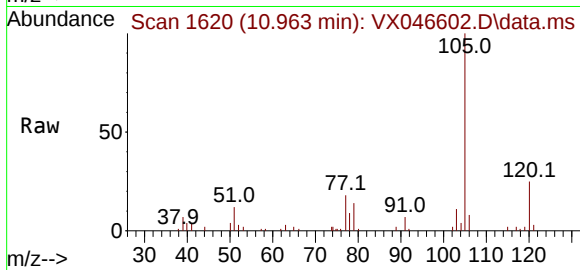

#76

1,2,3-Trichloropropane

Concen: 27.785 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX046602.D




Acq: 10 Jun 2025 14:59


Tgt Ion: 75 Resp: 69321

Ion Ratio Lower Upper

75 100

77 1.0 20.5 61.5#


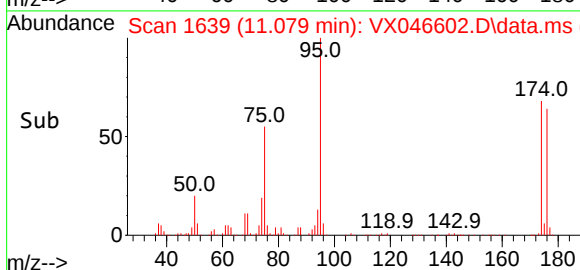
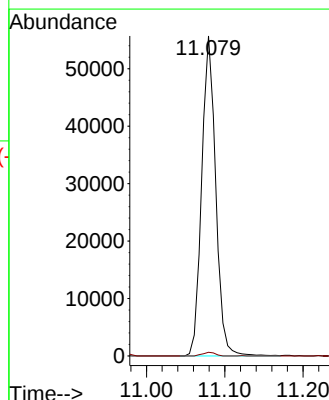
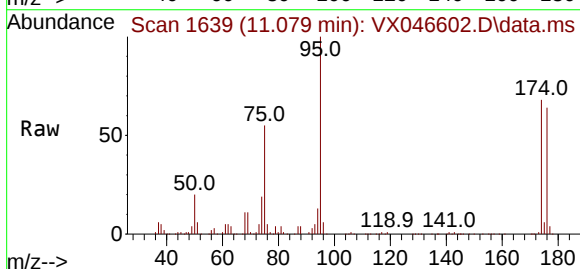




#78
n-propylbenzene
Concen: 2.539 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion: 91 Resp: 28458
Ion Ratio Lower Upper
91 100
120 21.9 10.8 32.4

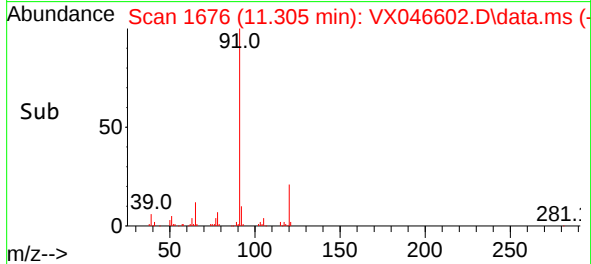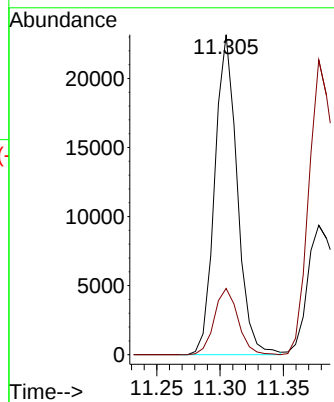

#79
2-Chlorotoluene
Concen: 2.808 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 91 Resp: 18979
Ion Ratio Lower Upper
91 100
126 0.0 15.6 46.7#



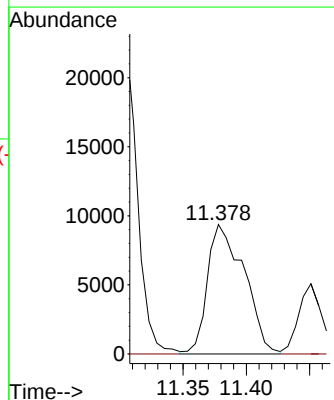
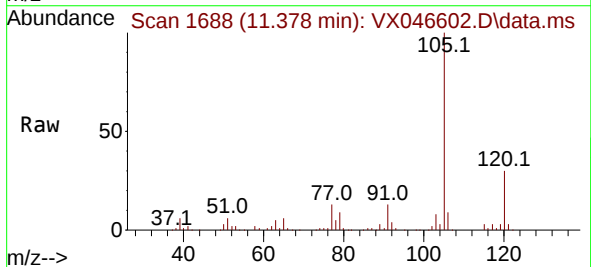




#80
1,3,5-Trimethylbenzene
Concen: 7.374 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:105 Resp: 56897
Ion Ratio Lower Upper
105 100
120 46.4 23.1 69.2

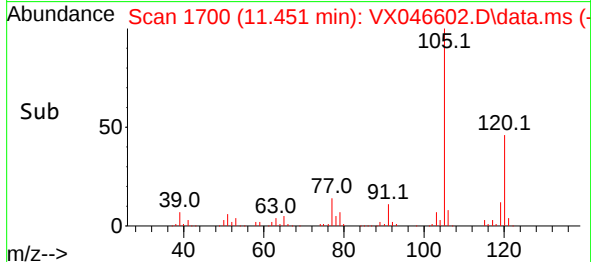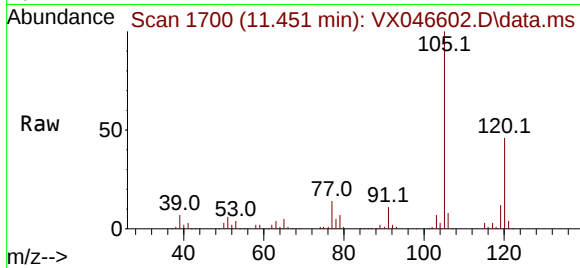

#81
trans-1,4-Dichloro-2-butene
Concen: 80.149 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 75 Resp: 69321
Ion Ratio Lower Upper
75 100
53 0.0 100.5 150.7#
89 0.0 37.0 55.6#




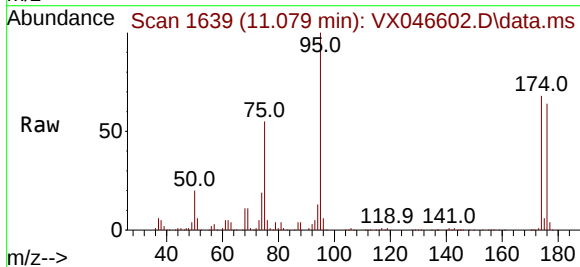




#82
4-Chlorotoluene
Concen: 0.828 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion: 91 Resp: 6636
Ion Ratio Lower Upper
91 100
126 0.0 13.3 39.8#

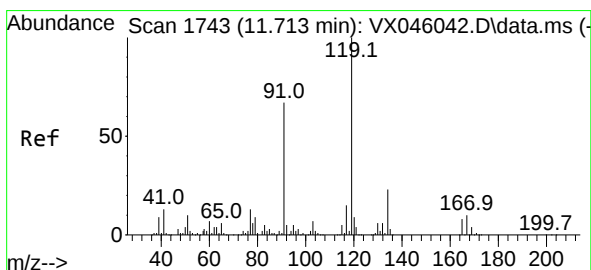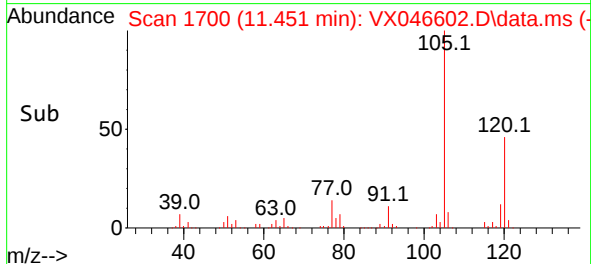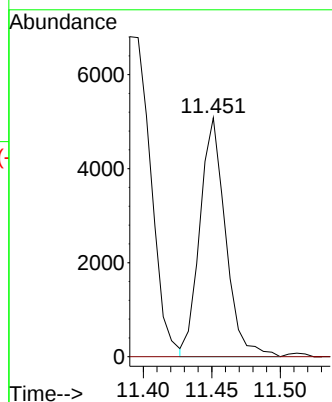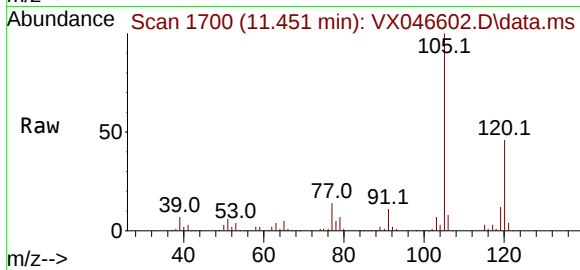

#83
tert-Butylbenzene
Concen: 2.987 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.037 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 119 Resp: 23460
Ion Ratio Lower Upper
119 100
91 99.3 32.9 98.7#
134 0.0 11.4 34.1#


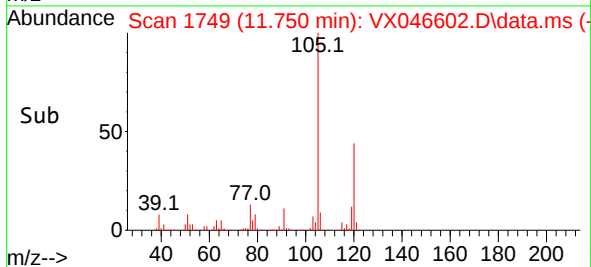
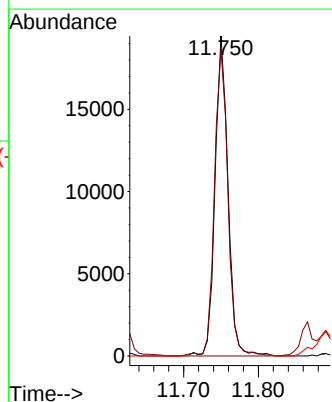
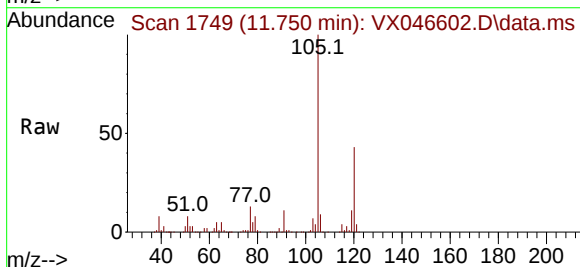




#84
1,2,4-Trimethylbenzene
Concen: 26.048 ug/l
RT: 11.750 min Scan# 11749
Delta R.T. -0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:105 Resp: 203323
Ion Ratio Lower Upper
105 100
120 43.7 21.2 63.6

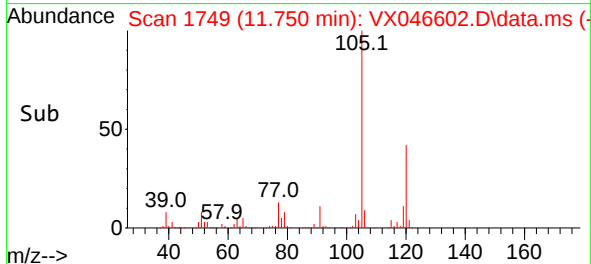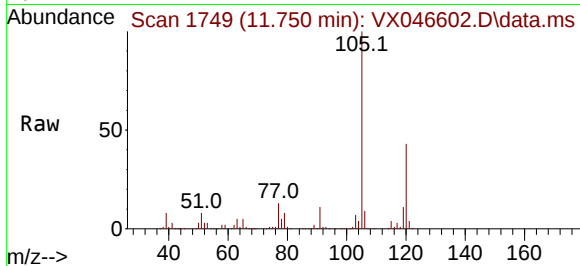

#85
sec-Butylbenzene
Concen: 0.995 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion:105 Resp: 10047
Ion Ratio Lower Upper
105 100
134 25.0 9.7 29.1

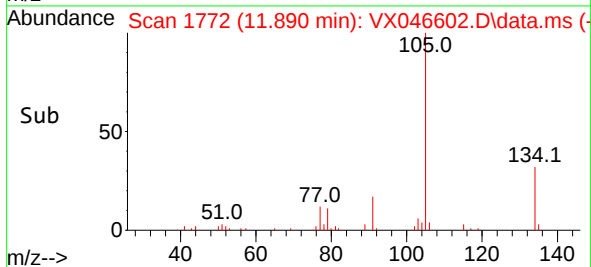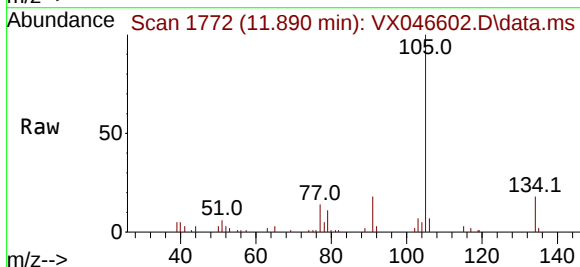



#86

p-Isopropyltoluene

Concen: 0.795 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX046602.D

Acq: 10 Jun 2025 14:59

Instrument :

MSVOA_X

ClientSampleId :

GW-MW01-060425





Tgt Ion:119 Resp: 6693

Ion Ratio Lower Upper

119 100

134 27.3 12.5 37.5

91 34.9 13.8 41.4

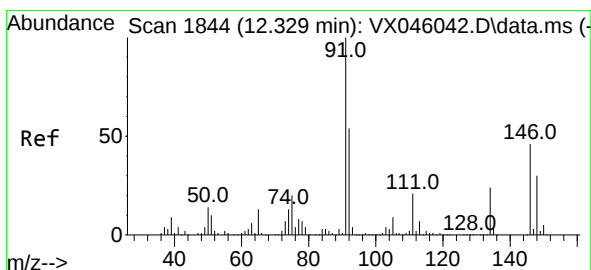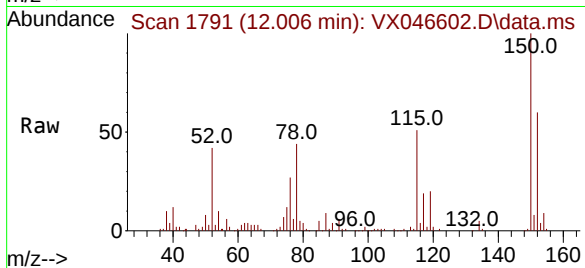

#89

n-Butylbenzene

Concen: 2.169 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX046602.D

Acq: 10 Jun 2025 14:59




Tgt Ion: 91 Resp: 17920


Ion Ratio Lower Upper

91 100

92 35.6 26.9 80.7

134 93.3 11.8 35.3#



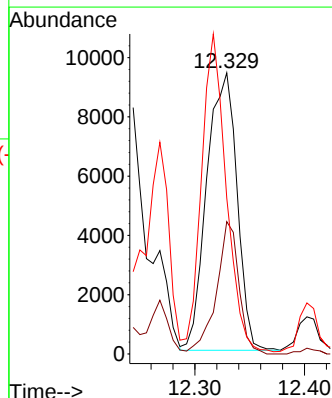
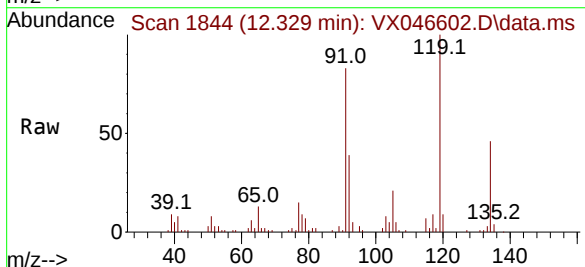




#90
Hexachloroethane
Concen: 2.050 ug/l
RT: 12.530 min Scan# 117
Delta R.T. -0.006 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59




Instrument :
MSVOA_X
ClientSampleId :
GW-MW01-060425


Tgt Ion:117 Resp: 3066
Ion Ratio Lower Upper
117 100
201 0.0 31.6 94.7#

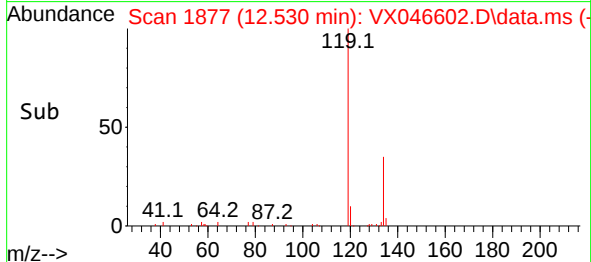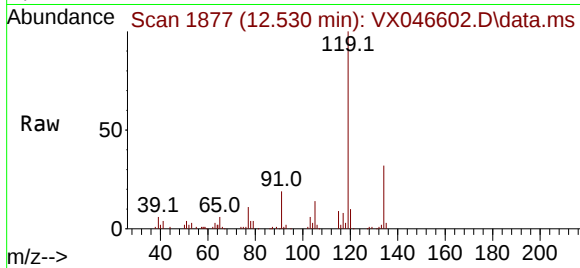

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.514 ug/l
RT: 12.920 min Scan# 1941
Delta R.T. -0.019 min
Lab File: VX046602.D
Acq: 10 Jun 2025 14:59

Tgt Ion: 75 Resp: 341
Ion Ratio Lower Upper
75 100
155 0.0 34.9 104.8#
157 0.0 43.8 131.4#

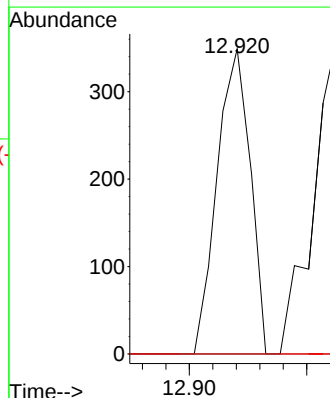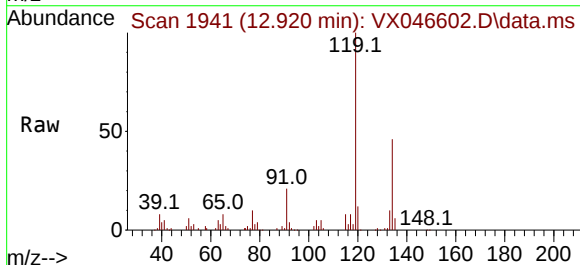

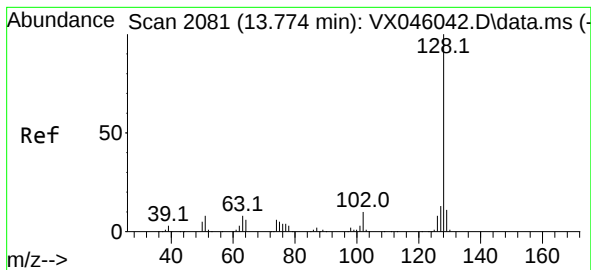

#95

Naphthalene

Concen: 3.707 ug/l

RT: 13.774 min Scan# 20

Delta R.T. -0.000 min

Lab File: VX046602.D


Acq: 10 Jun 2025 14:59

Instrument :

MSVOA_X

ClientSampleId :

GW-MW01-060425

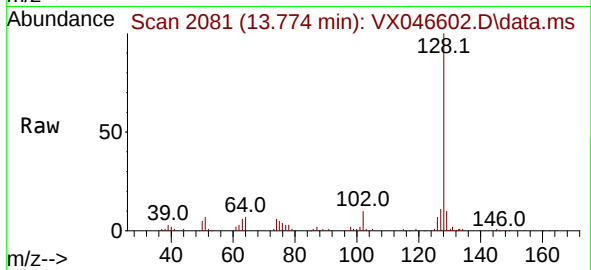

Tgt Ion:128 Resp: 32304

Ion Ratio Lower Upper

128 100

127 13.0 10.4 15.6

129 12.2 8.6 13.0

