
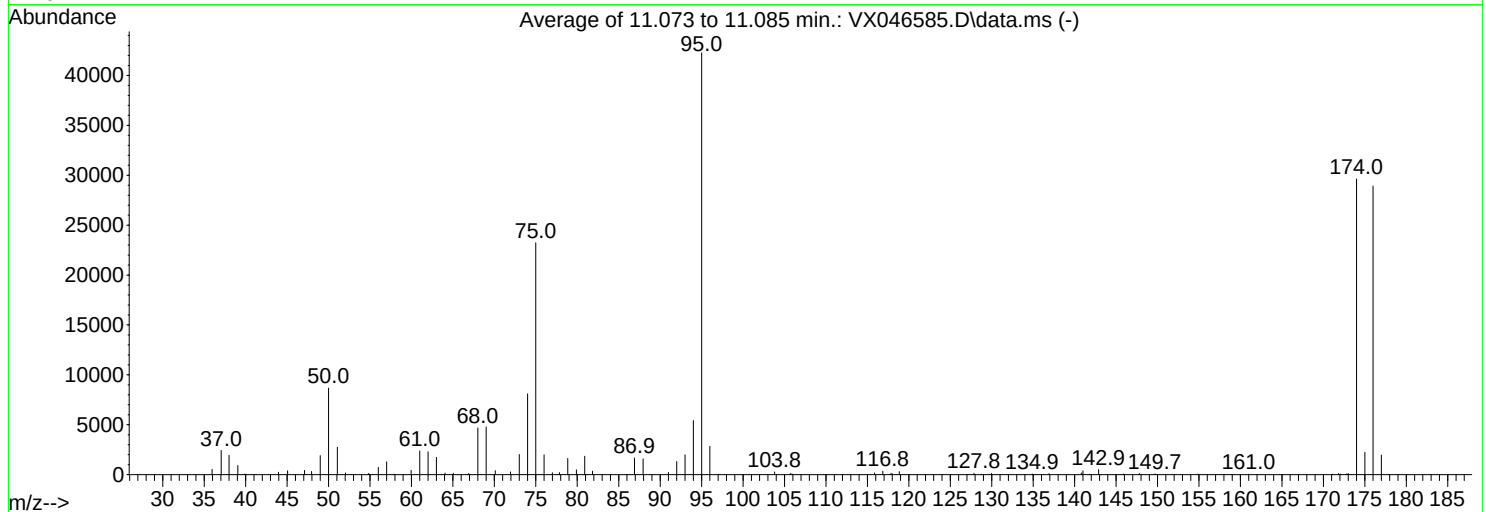


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046585.D
Acq On : 10 Jun 2025 08:36
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Title : SW846 8260
Last Update : Fri Jun 06 16:56:12 2025

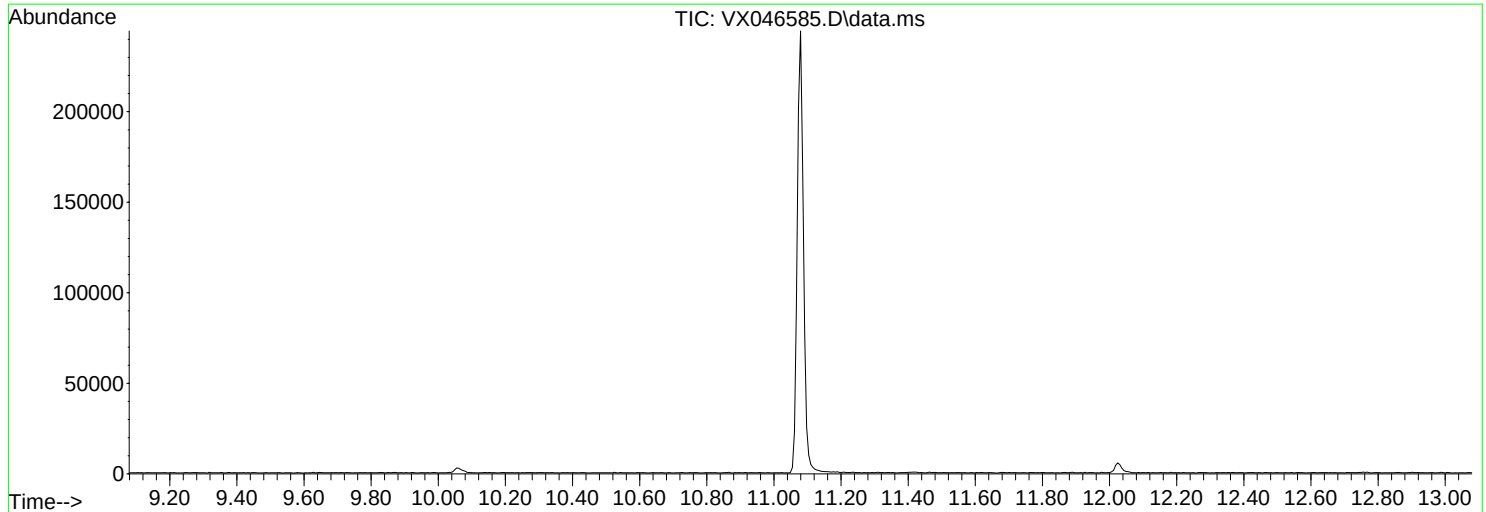

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	8668	PASS
75	95	30	60	55.0	23232	PASS
95	95	100	100	100.0	42264	PASS
96	95	5	9	6.7	2835	PASS
173	174	0.00	2	0.4	107	PASS
174	95	50	100	70.1	29635	PASS
175	174	5	9	7.6	2246	PASS
176	174	95	101	97.6	28920	PASS
177	176	5	9	6.8	1965	PASS