

Cover Page

Order ID : Q2234

Project ID : Former Schlumberger STC PTC Site D3868221

Client : JACOBS Engineering Group, Inc.

Lab Sample Number

Q2234-01
Q2234-02
Q2234-03
Q2234-04
Q2234-05
Q2234-06
Q2234-07
Q2234-08
Q2234-09
Q2234-10
Q2234-11
Q2234-12
Q2234-13

Client Sample Number

MW-17B-55-060425
Q2234-01MS
Q2234-01MSD
MW-17B-55-060425-SIM
MW-18B-56-060425
MW-18B-56-060425-FD
MW-19B-72-060425
MW-17B-55-060425
Q2234-08MS
Q2234-08MSD
MW-18B-56-060425
MW-18B-56-060425-FD
MW-19B-72-060425

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 6/17/2025

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q2234

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Custody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: KETAN PATEL

Date: 06/17/2025

LAB CHRONICLE

OrderID:	Q2234	OrderDate:	6/5/2025 10:52:00 AM
Client:	JACOBS Engineering Group, Inc.	Project:	Former Schlumberger STC PTC Site D3868221
Contact:	John Ynfante	Location:	N31,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2234-01	MW-17B-55-060425	Water	VOCMS Group3	8260-Low	06/04/25		06/10/25	06/05/25
Q2234-01DL	MW-17B-55-060425D L	Water	VOCMS Group3	8260-Low	06/04/25		06/10/25	06/05/25

Hit Summary Sheet
SW-846

SDG No.: Q2234

Client: JACOBS Engineering Group, Inc.

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
Client ID:	MW-17B-55-060425							
Q2234-01	MW-17B-55-06042	Water	Vinyl Chloride	13.5		2.60	10.0	ug/L
Q2234-01	MW-17B-55-06042	Water	1,1-Dichloroethene	26.9		2.30	10.0	ug/L
Q2234-01	MW-17B-55-06042	Water	cis-1,2-Dichloroethene	1900	E	1.90	10.0	ug/L
Q2234-01	MW-17B-55-06042	Water	Trichloroethene	4000	E	0.93	10.0	ug/L
Q2234-01	MW-17B-55-06042	Water	Tetrachloroethene	49.1		2.30	10.0	ug/L
			Total Voc :	5990				
			Total Concentration:	5990				
Client ID:	MW-17B-55-060425DL							
Q2234-01DL	MW-17B-55-06042	Water	cis-1,2-Dichloroethene	1600	D	19.0	100	ug/L
Q2234-01DL	MW-17B-55-06042	Water	Trichloroethene	3700	D	9.30	100	ug/L
Q2234-01DL	MW-17B-55-06042	Water	Tetrachloroethene	44.2	JD	23.0	100	ug/L
			Total Voc :	5340				
			Total Concentration:	5340				



QC SUMMARY

Surrogate Summary

SDG No.: Q2234

Client: JACOBS Engineering Group, Inc.

Analytical Method: SW8260-Low

Lab Sample ID	Client ID	Parameter	Spike	Result	RecoveryQual	Limits	
						Low	High
Q2234-01	MW-17B-55-060425	1,2-Dichloroethane-d4	50	50.7	101	70 (74)	130 (125)
		Dibromofluoromethane	50	50.0	100	70 (75)	130 (124)
		Toluene-d8	50	53.7	107	70 (86)	130 (113)
		4-Bromofluorobenzene	50	55.8	112	70 (77)	130 (121)
Q2234-01DL	MW-17B-55-060425DL	1,2-Dichloroethane-d4	50	50.4	101	70 (74)	130 (125)
		Dibromofluoromethane	50	50.2	100	70 (75)	130 (124)
		Toluene-d8	50	54.4	109	70 (86)	130 (113)
		4-Bromofluorobenzene	50	54.7	109	70 (77)	130 (121)
VX0610WBL01	VX0610WBL01	1,2-Dichloroethane-d4	50	50.1	100	70 (74)	130 (125)
		Dibromofluoromethane	50	50.1	100	70 (75)	130 (124)
		Toluene-d8	50	54.3	109	70 (86)	130 (113)
		4-Bromofluorobenzene	50	54.8	110	70 (77)	130 (121)
VX0610WBS01	VX0610WBS01	1,2-Dichloroethane-d4	50	47.4	95	70 (74)	130 (125)
		Dibromofluoromethane	50	53.0	106	70 (75)	130 (124)
		Toluene-d8	50	51.5	103	70 (86)	130 (113)
		4-Bromofluorobenzene	50	53.1	106	70 (77)	130 (121)
VX0610WBSD0	VX0610WBSD01	1,2-Dichloroethane-d4	50	49.3	99	70 (74)	130 (125)
		Dibromofluoromethane	50	52.3	105	70 (75)	130 (124)
		Toluene-d8	50	51.0	102	70 (86)	130 (113)
		4-Bromofluorobenzene	50	52.4	105	70 (77)	130 (121)

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2234

Client: JACOBS Engineering Group, Inc.

Analytical Method: SW8260D

Datafile : VX046589.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VX0610WBS01	Vinyl chloride	20	18.7	ug/L	94			70 (65)	130 (117)	
	1,1-Dichloroethene	20	19.2	ug/L	96			70 (74)	130 (110)	
	1,1-Dichloroethane	20	20.4	ug/L	102			70 (78)	130 (112)	
	cis-1,2-Dichloroethene	20	20.6	ug/L	103			70 (77)	130 (110)	
	1,1,1-Trichloroethane	20	20.6	ug/L	103			70 (80)	130 (108)	
	Benzene	20	21.0	ug/L	105			70 (82)	130 (109)	
	1,2-Dichloroethane	20	20.8	ug/L	104			70 (80)	130 (115)	
	Trichloroethene	20	20.1	ug/L	101			70 (77)	130 (113)	
	1,1,2-Trichloroethane	20	21.6	ug/L	108			70 (83)	130 (112)	
	Tetrachloroethene	20	20.3	ug/L	102			70 (67)	130 (123)	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2234

Client: JACOBS Engineering Group, Inc.

Analytical Method: SW8260D

Datafile : VX046590.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VX0610WBSD01	Vinyl chloride	20	19.1	ug/L	96	2		70 (65)	130 (117)	20 (19)
	1,1-Dichloroethene	20	19.8	ug/L	99	3		70 (74)	130 (110)	20 (20)
	1,1-Dichloroethane	20	20.7	ug/L	104	2		70 (78)	130 (112)	20 (20)
	cis-1,2-Dichloroethene	20	20.5	ug/L	103	0		70 (77)	130 (110)	20 (20)
	1,1,1-Trichloroethane	20	20.9	ug/L	104	1		70 (80)	130 (108)	20 (20)
	Benzene	20	20.6	ug/L	103	2		70 (82)	130 (109)	20 (15)
	1,2-Dichloroethane	20	20.6	ug/L	103	1		70 (80)	130 (115)	20 (20)
	Trichloroethene	20	19.8	ug/L	99	2		70 (77)	130 (113)	20 (15)
	1,1,2-Trichloroethane	20	22.3	ug/L	112	4		70 (83)	130 (112)	20 (20)
	Tetrachloroethene	20	19.8	ug/L	99	3		70 (67)	130 (123)	20 (15)

VOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

VX0610WBL01

Lab Name: CHEMTECH

Contract: JACO05

Lab Code: CHEM Case No.: Q2234

SAS No.: Q2234 SDG NO.: Q2234

Lab File ID: VX046588.D

Lab Sample ID: VX0610WBL01

Date Analyzed: 06/10/2025

Time Analyzed: 09:57

GC Column: DB-624UI ID: 0.18 (mm)

Heated Purge: (Y/N) N

Instrument ID: MSVOA_X

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VX0610WBS01	VX0610WBS01	VX046589.D	06/10/2025
VX0610WBSD01	VX0610WBSD01	VX046590.D	06/10/2025
MW-17B-55-060425DL	Q2234-01DL	VX046599.D	06/10/2025
MW-17B-55-060425	Q2234-01	VX046611.D	06/10/2025

COMMENTS: _____



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: CHEMTECH Contract: JACO05
Lab Code: CHEM Case No.: Q2234 SAS No.: Q2234 SDG NO.: Q2234
Lab File ID: VX046516.D BFB Injection Date: 06/06/2025
Instrument ID: MSVOA_X BFB Injection Time: 08:47
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	21
75	30.0 - 60.0% of mass 95	56.5
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.5
173	Less than 2.0% of mass 174	0.6 (1) 1
174	50.0 - 100.0% of mass 95	65.2
175	5.0 - 9.0% of mass 174	5 (7.7) 1
176	95.0 - 101.0% of mass 174	62.7 (96.1) 1
177	5.0 - 9.0% of mass 176	4.2 (6.6) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDIC005	VSTDIC005	VX046518.D	06/06/2025	09:42
VSTDIC020	VSTDIC020	VX046519.D	06/06/2025	10:18
VSTDIC050	VSTDIC050	VX046520.D	06/06/2025	10:40
VSTDIC100	VSTDIC100	VX046521.D	06/06/2025	11:02
VSTDIC150	VSTDIC150	VX046522.D	06/06/2025	11:25
VSTDIC001	VSTDIC001	VX046524.D	06/06/2025	12:57



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: CHEMTECH Contract: JACO05
Lab Code: CHEM Case No.: Q2234 SAS No.: Q2234 SDG NO.: Q2234
Lab File ID: VX046585.D BFB Injection Date: 06/10/2025
Instrument ID: MSVOA_X BFB Injection Time: 08:36
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	20.5
75	30.0 - 60.0% of mass 95	55
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.7
173	Less than 2.0% of mass 174	0.3 (0.4) 1
174	50.0 - 100.0% of mass 95	70.1
175	5.0 - 9.0% of mass 174	5.3 (7.6) 1
176	95.0 - 101.0% of mass 174	68.4 (97.6) 1
177	5.0 - 9.0% of mass 176	4.6 (6.8) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VX046586.D	06/10/2025	09:07
VX0610WBL01	VX0610WBL01	VX046588.D	06/10/2025	09:57
VX0610WBS01	VX0610WBS01	VX046589.D	06/10/2025	10:18
VX0610WBSD01	VX0610WBSD01	VX046590.D	06/10/2025	10:44
MW-17B-55-060425DL	Q2234-01DL	VX046599.D	06/10/2025	13:55
MW-17B-55-060425	Q2234-01	VX046611.D	06/10/2025	18:11

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: JACO05
Lab Code: CHEM Case No.: Q2234 SAS No.: Q2234 SDG NO.: Q2234
Lab File ID: VX046586.D Date Analyzed: 06/10/2025
Instrument ID: MSVOA_X Time Analyzed: 09:07
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	90758	5.56	150623	6.76	134767	10.06
UPPER LIMIT	181516	6.056	301246	7.263	269534	10.555
LOWER LIMIT	45379	5.056	75311.5	6.263	67383.5	9.555
EPA SAMPLE NO.						
MW-17B-55-060425	110890	5.57	220616	6.77	227088	10.06
MW-17B-55-060425DL	110214	5.56	218656	6.77	224113	10.06
VX0610WBL01	106110	5.56	211553	6.77	217338	10.06
VX0610WBS01	84052	5.56	143506	6.77	131426	10.06
VX0610WBSD01	79698	5.56	139229	6.77	126313	10.06

IS1 = Pentafluorobenzene
IS2 = 1,4-Difluorobenzene
IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area
AREA LOWER LIMIT = -50% of internal standard area
RT UPPER LIMIT = +0.50 minutes of internal standard RT
RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
* Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: JACO05
 Lab Code: CHEM Case No.: Q2234 SAS No.: Q2234 SDG NO.: Q2234
 Lab File ID: VX046586.D Date Analyzed: 06/10/2025
 Instrument ID: MSVOA_X Time Analyzed: 09:07
 GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS4 AREA #	RT #				
12 HOUR STD	66941	12.018				
UPPER LIMIT	133882	12.518				
LOWER LIMIT	33470.5	11.518				
EPA SAMPLE NO.						
MW-17B-55-060425	116641	12.02				
MW-17B-55-060425DL	112148	12.02				
VX0610WBL01	104374	12.02				
VX0610WBS01	68222	12.02				
VX0610WBSD01	65284	12.02				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area
 AREA LOWER LIMIT = -50% of internal standard area
 RT UPPER LIMIT = +0.50 minutes of internal standard RT
 RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.



SAMPLE DATA

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	06/04/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	06/05/25
Client Sample ID:	MW-17B-55-060425	SDG No.:	Q2234
Lab Sample ID:	Q2234-01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046611.D	10		06/10/25 18:11	VX061025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	13.5		2.60	10.0	ug/L
75-35-4	1,1-Dichloroethene	26.9		2.30	10.0	ug/L
75-34-3	1,1-Dichloroethane	2.30	U	2.30	10.0	ug/L
156-59-2	cis-1,2-Dichloroethene	1900	E	1.90	10.0	ug/L
71-55-6	1,1,1-Trichloroethane	2.00	U	2.00	10.0	ug/L
71-43-2	Benzene	1.50	U	1.50	10.0	ug/L
107-06-2	1,2-Dichloroethane	2.20	U	2.20	10.0	ug/L
79-01-6	Trichloroethene	4000	E	0.93	10.0	ug/L
79-00-5	1,1,2-Trichloroethane	2.10	U	2.10	10.0	ug/L
127-18-4	Tetrachloroethene	49.1		2.30	10.0	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	50.7		70 (74) - 130 (125)	101%	SPK: 50
1868-53-7	Dibromofluoromethane	50.1		70 (75) - 130 (124)	100%	SPK: 50
2037-26-5	Toluene-d8	53.7		70 (86) - 130 (113)	107%	SPK: 50
460-00-4	4-Bromofluorobenzene	55.8		70 (77) - 130 (121)	112%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	111000	5.568			
540-36-3	1,4-Difluorobenzene	221000	6.769			
3114-55-4	Chlorobenzene-d5	227000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	117000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of OC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046611.D
 Acq On : 10 Jun 2025 18:11
 Operator : JC/MD
 Sample : Q2234-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-17B-55-060425

Quant Time: Jun 11 01:53:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.568	168	110890	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	220616	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	227088	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	116641	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	99959	50.667	ug/l	0.00
Spiked Amount	50.000	Range 74 - 125	Recovery	= 101.340%		
35) Dibromofluoromethane	5.404	113	81202	50.050	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 100.100%		
50) Toluene-d8	8.653	98	287387	53.729	ug/l	0.00
Spiked Amount	50.000	Range 86 - 113	Recovery	= 107.460%		
62) 4-Bromofluorobenzene	11.079	95	123534	55.820	ug/l	0.00
Spiked Amount	50.000	Range 77 - 121	Recovery	= 111.640%		
Target Compounds						Qvalue
4) Vinyl Chloride	1.386	62	1884	1.349	ug/l	95
9) 1,1,2-Trichlorotrifluo...	2.349	101	8884	6.101	ug/l	93
12) 1,1-Dichloroethene	2.337	96	3540	2.689	ug/l	85
21) trans-1,2-Dichloroethene	3.111	96	604	0.434	ug/l #	75
27) cis-1,2-Dichloroethene	4.501	96	317398	185.057	ug/l	86
44) Trichloroethene	7.135	130	662594	399.712	ug/l	97
64) Tetrachloroethene	9.275	164	7455	4.909	ug/l	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046611.D
Acq On : 10 Jun 2025 18:11
Operator : JC/MD
Sample : Q2234-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-17B-55-060425

Quant Time: Jun 11 01:53:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration




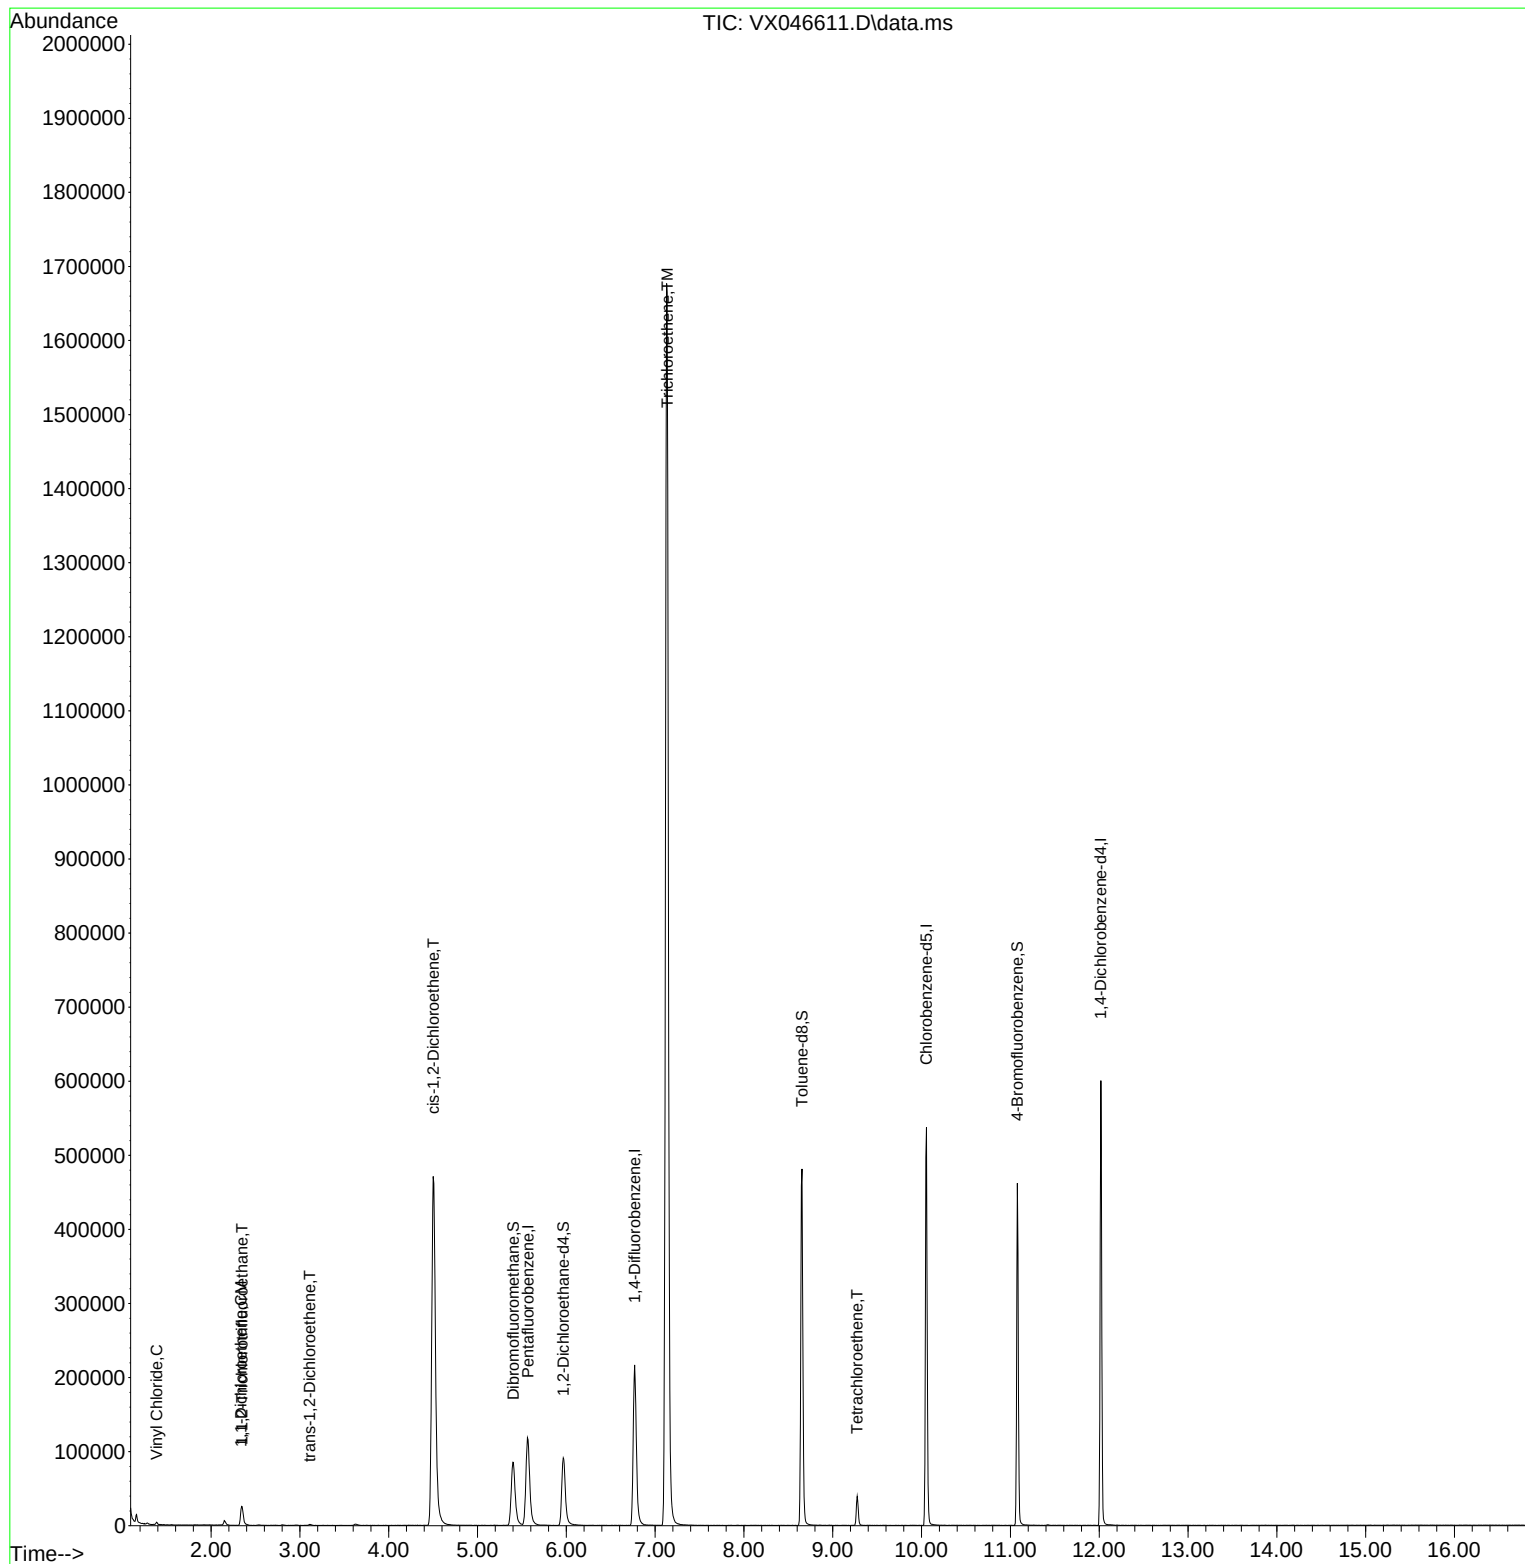


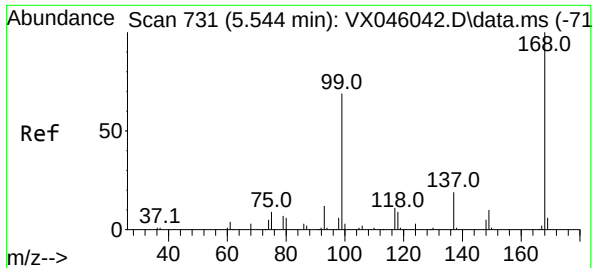

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX046611.D
Acq: 10 Jun 2025 18:11




Instrument :
MSVOA_X
ClientSampleId :
MW-17B-55-060425


Tgt Ion:168 Resp: 110890
Ion Ratio Lower Upper
168 100
99 66.9 54.9 82.3

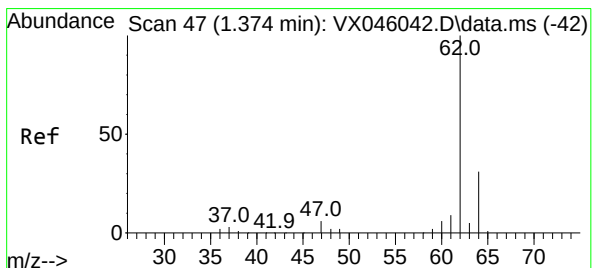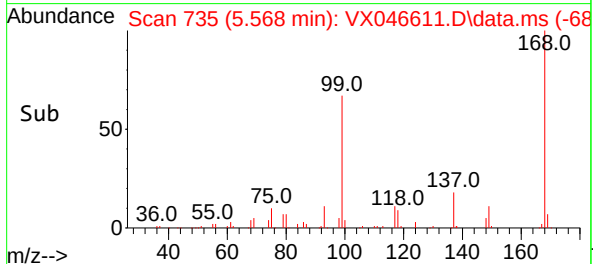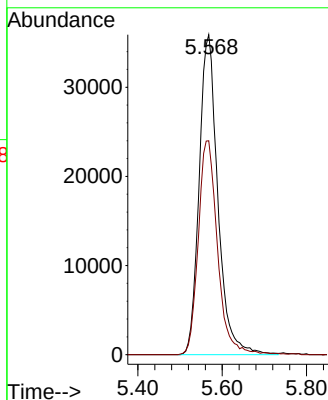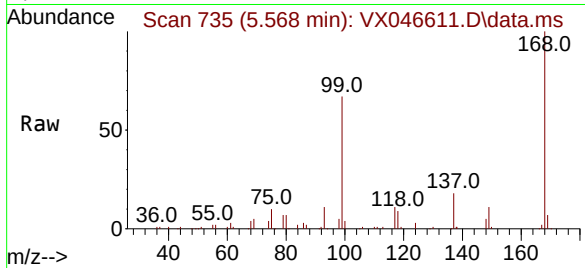

#4
Vinyl Chloride
Concen: 1.349 ug/l
RT: 1.386 min Scan# 49
Delta R.T. -0.000 min
Lab File: VX046611.D
Acq: 10 Jun 2025 18:11

Tgt Ion: 62 Resp: 1884
Ion Ratio Lower Upper
62 100
64 34.2 25.2 37.8


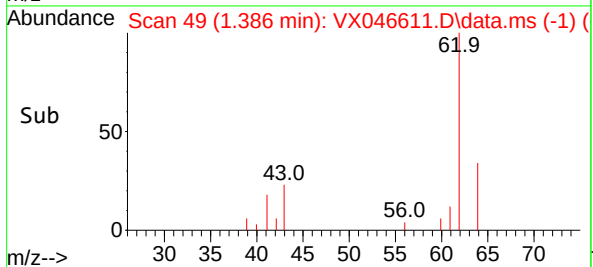
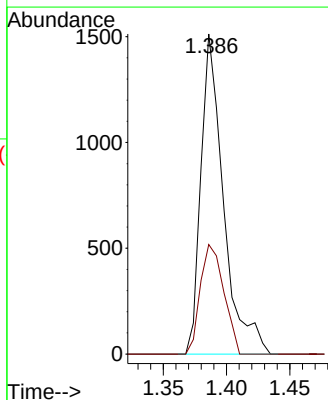
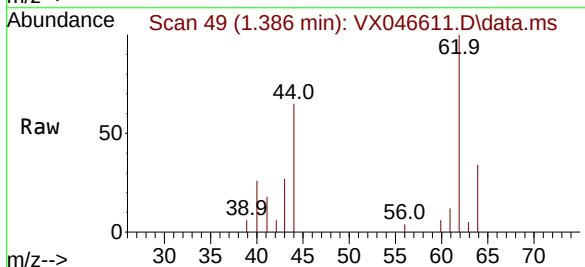


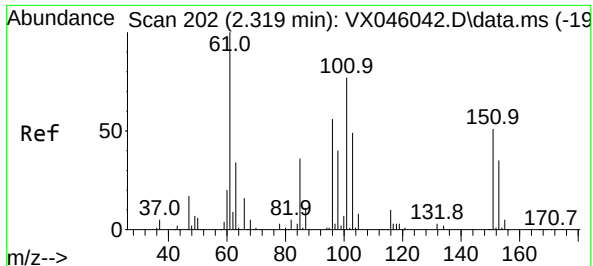

#9
1,1,2-Trichlorotrifluoroethane
Concen: 6.101 ug/l
RT: 2.349 min Scan# 205
Delta R.T. 0.000 min
Lab File: VX046611.D
Acq: 10 Jun 2025 18:11




Instrument :
MSVOA_X
ClientSampleId :
MW-17B-55-060425


Tgt Ion:101 Resp: 8884
Ion Ratio Lower Upper
101 100
85 46.3 38.6 58.0
151 76.7 55.2 82.8

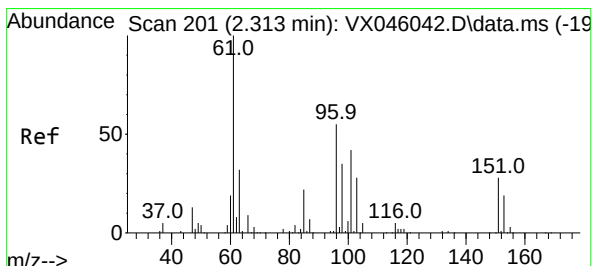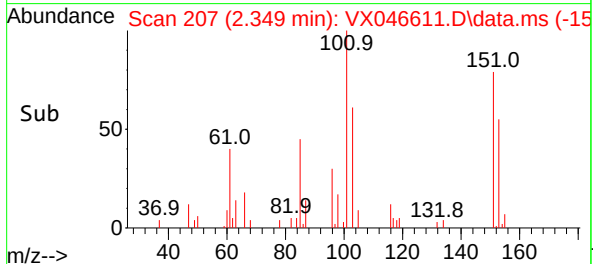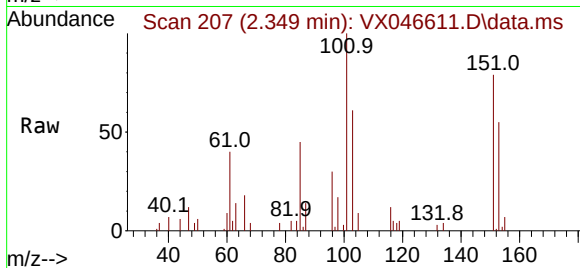

#12
1,1-Dichloroethene
Concen: 2.689 ug/l
RT: 2.337 min Scan# 205
Delta R.T. -0.000 min
Lab File: VX046611.D
Acq: 10 Jun 2025 18:11

Tgt Ion: 96 Resp: 3540
Ion Ratio Lower Upper
96 100
61 159.1 146.2 219.2
98 55.7 51.0 76.6


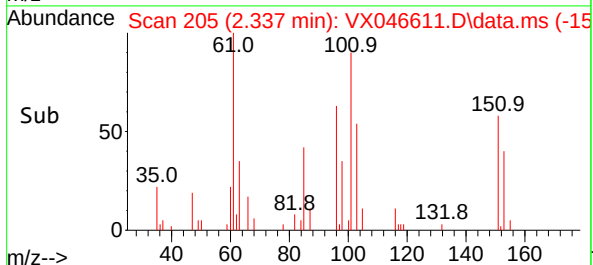
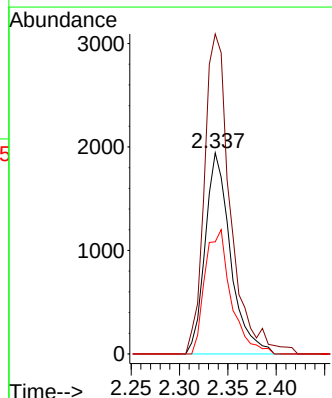
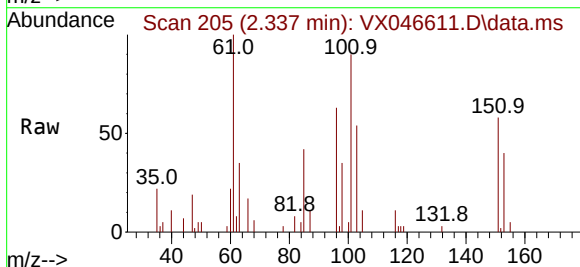


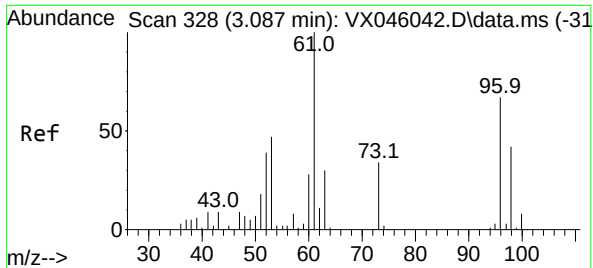

#21
trans-1,2-Dichloroethene
Concen: 0.434 ug/l
RT: 3.111 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX046611.D
Acq: 10 Jun 2025 18:11




Instrument :
MSVOA_X
ClientSampleId :
MW-17B-55-060425


Tgt Ion: 96 Resp: 604
Ion Ratio Lower Upper
96 100
61 114.5 119.5 179.3#
98 47.1 50.0 75.0#

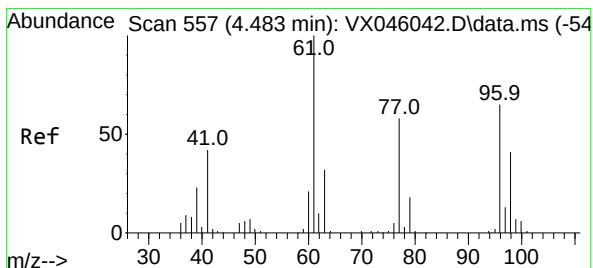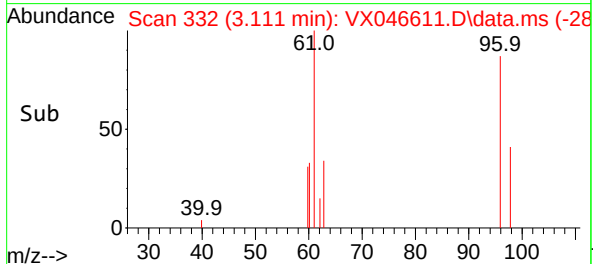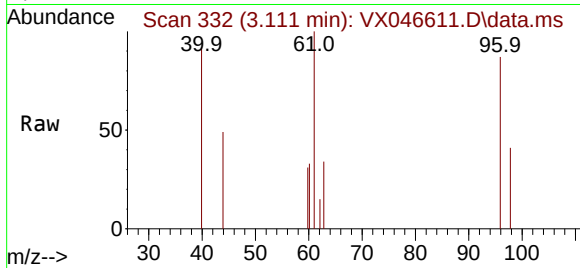

#27
cis-1,2-Dichloroethene
Concen: 185.057 ug/l
RT: 4.501 min Scan# 560
Delta R.T. -0.006 min
Lab File: VX046611.D
Acq: 10 Jun 2025 18:11

Tgt Ion: 96 Resp: 317398
Ion Ratio Lower Upper
96 100
61 135.3 0.0 322.8
98 63.6 0.0 129.0

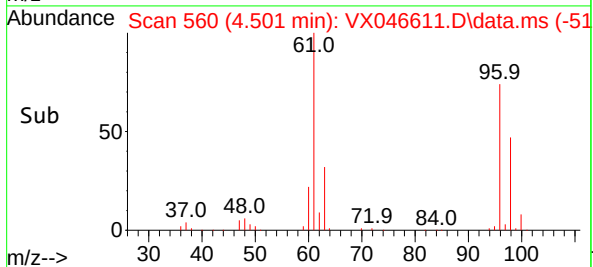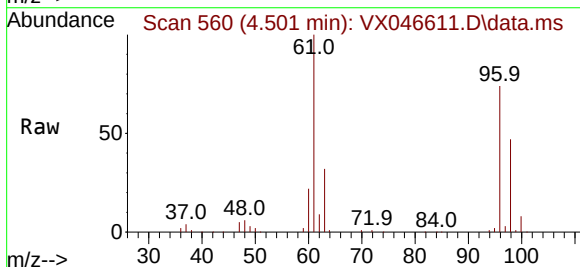



#33

1,2-Dichloroethane-d4

Concen: 50.667 ug/l

RT: 5.964 min Scan# 80

Delta R.T. -0.006 min

Lab File: VX046611.D

Acq: 10 Jun 2025 18:11

Instrument :

MSVOA_X

ClientSampleId :





MW-17B-55-060425

Tgt Ion: 65 Resp: 99959

Ion Ratio Lower Upper

65 100

67 50.3 0.0 99.0

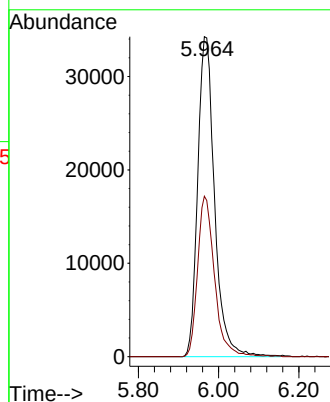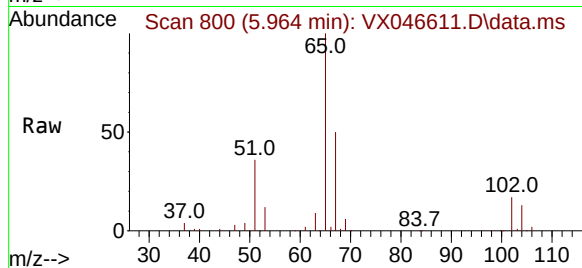

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.006 min

Lab File: VX046611.D

Acq: 10 Jun 2025 18:11




Tgt Ion: 114 Resp: 220616


Ion Ratio Lower Upper

114 100

63 22.0 0.0 49.2

88 16.4 0.0 33.6

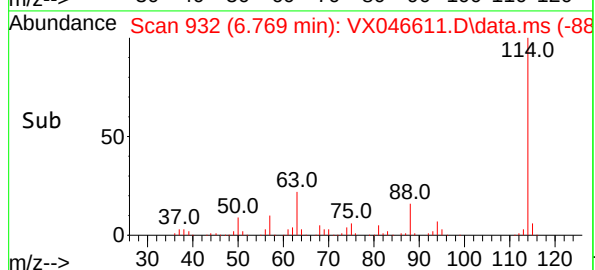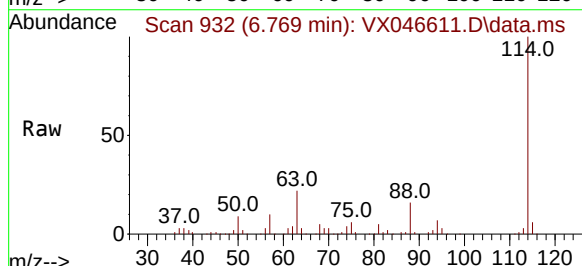

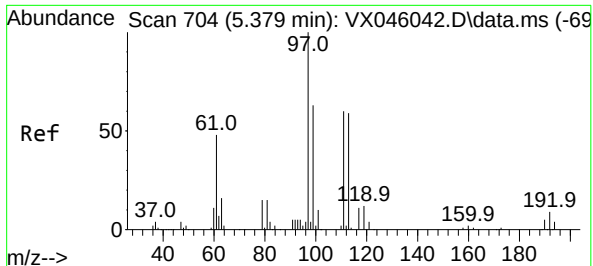

#35

Dibromofluoromethane

Concen: 50.050 ug/l

RT: 5.404 min Scan# 704

Delta R.T. 0.001 min

Lab File: VX046611.D

Acq: 10 Jun 2025 18:11

Instrument :

MSVOA_X

ClientSampleId :

MW-17B-55-060425





Tgt Ion:113 Resp: 81202

Ion Ratio Lower Upper

113 100

111 101.8 83.1 124.7

192 17.3 13.3 19.9

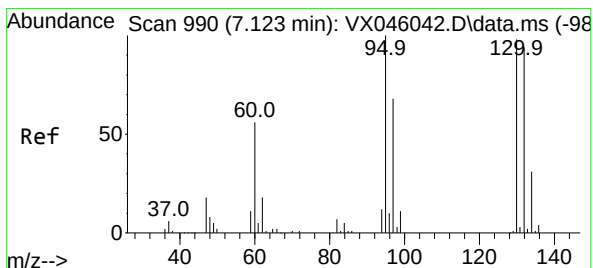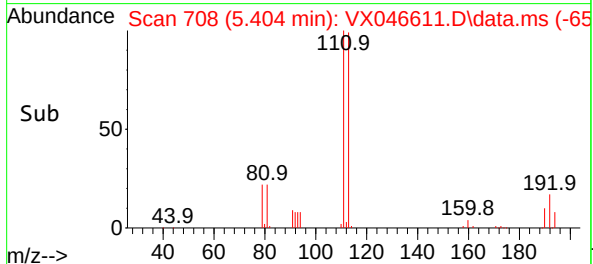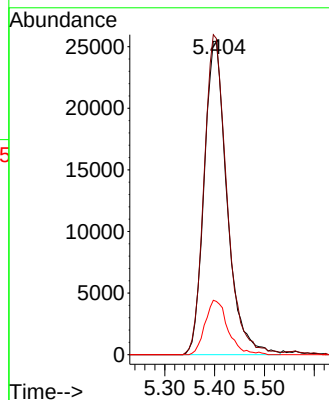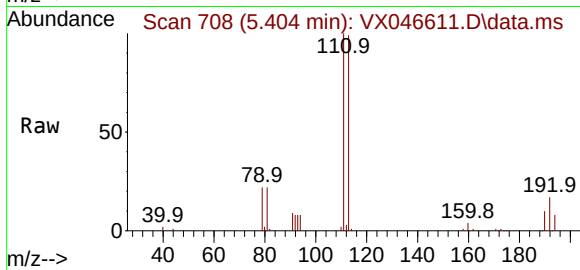

#44

Trichloroethene

Concen: 399.712 ug/l

RT: 7.135 min Scan# 992

Delta R.T. -0.000 min

Lab File: VX046611.D




Acq: 10 Jun 2025 18:11


Tgt Ion:130 Resp: 662594

Ion Ratio Lower Upper

130 100

95 105.1 0.0 204.2

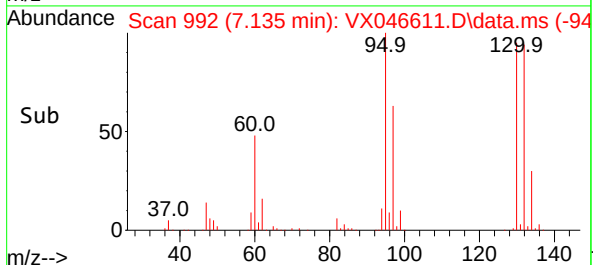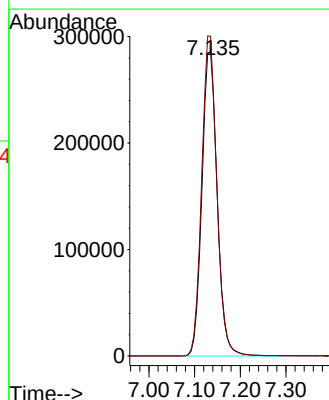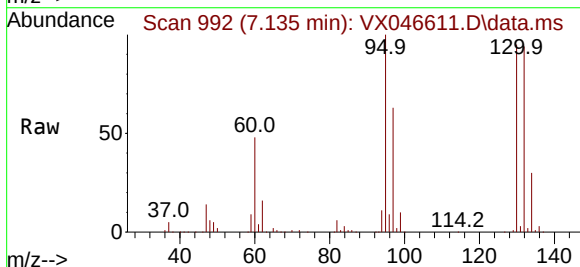



#50

Toluene-d8

Concen: 53.729 ug/l

RT: 8.653 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX046611.D

Acq: 10 Jun 2025 18:11

Instrument :

MSVOA_X

ClientSampleId :





MW-17B-55-060425

Tgt Ion: 98 Resp: 287387

Ion Ratio Lower Upper

98 100

100 65.7 53.5 80.3

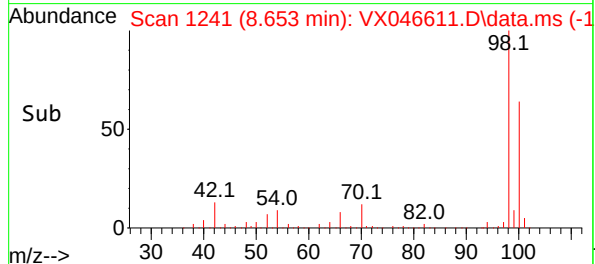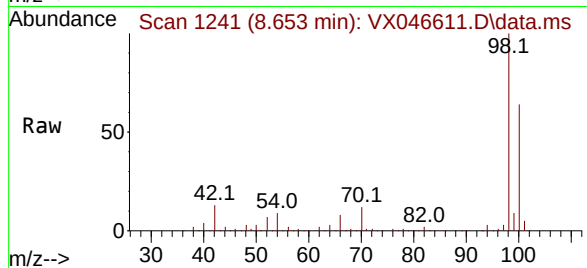

#62

4-Bromofluorobenzene

Concen: 55.820 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046611.D

Acq: 10 Jun 2025 18:11




Tgt Ion: 95 Resp: 123534


Ion Ratio Lower Upper

95 100

174 69.0 0.0 135.8

176 66.3 0.0 131.4

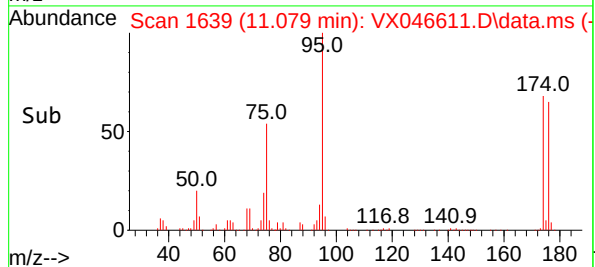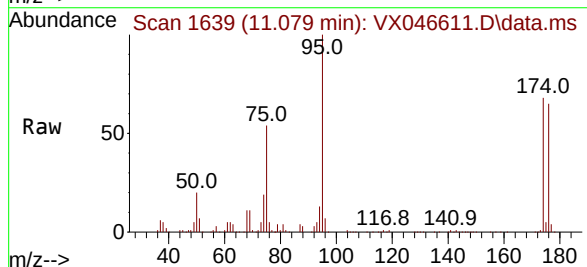



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX046611.D

Acq: 10 Jun 2025 18:11

Instrument :

MSVOA_X

ClientSampleId :

MW-17B-55-060425





Tgt Ion:117 Resp: 227088

Ion Ratio Lower Upper

117 100

82 57.7 50.6 76.0

119 32.1 25.8 38.6

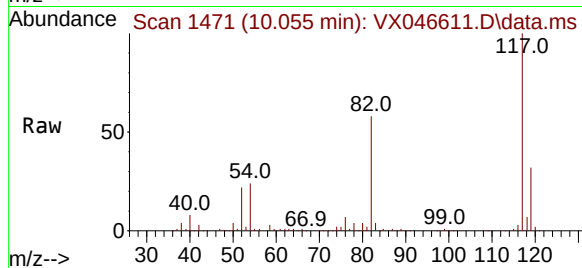

#64

Tetrachloroethene

Concen: 4.909 ug/l

RT: 9.275 min Scan# 1343

Delta R.T. -0.000 min

Lab File: VX046611.D

Acq: 10 Jun 2025 18:11

Tgt Ion:164 Resp: 7455




Ion Ratio Lower Upper


164 100

166 109.5 105.0 157.6

129 94.0 83.5 125.3

131 90.1 76.5 114.7

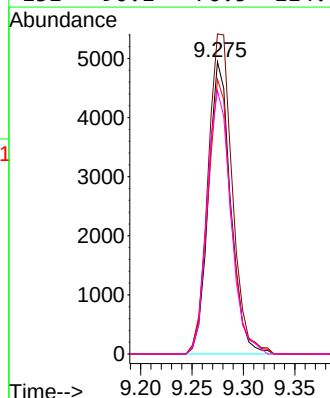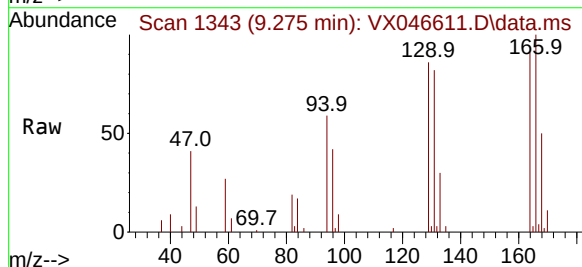



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX046611.D


Acq: 10 Jun 2025 18:11

Instrument :

MSVOA_X

ClientSampleId :

MW-17B-55-060425

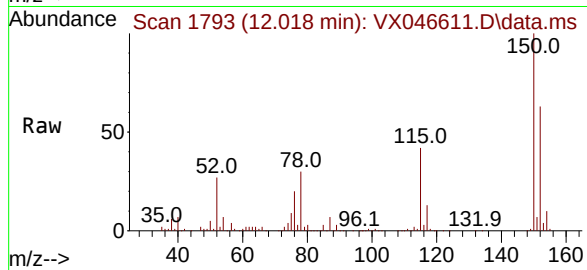



Tgt Ion:152 Resp: 116641

Ion Ratio Lower Upper

152 100

115 62.8 46.9 140.7

150 156.3 0.0 351.0

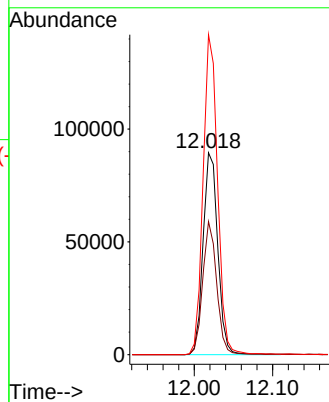

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	06/04/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	06/05/25
Client Sample ID:	MW-17B-55-060425DL	SDG No.:	Q2234
Lab Sample ID:	Q2234-01DL	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046599.D	100		06/10/25 13:55	VX061025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	26.0	UD	26.0	100	ug/L
75-35-4	1,1-Dichloroethene	23.0	UD	23.0	100	ug/L
75-34-3	1,1-Dichloroethane	23.0	UD	23.0	100	ug/L
156-59-2	cis-1,2-Dichloroethene	1600	D	19.0	100	ug/L
71-55-6	1,1,1-Trichloroethane	20.0	UD	20.0	100	ug/L
71-43-2	Benzene	15.0	UD	15.0	100	ug/L
107-06-2	1,2-Dichloroethane	22.0	UD	22.0	100	ug/L
79-01-6	Trichloroethene	3700	D	9.30	100	ug/L
79-00-5	1,1,2-Trichloroethane	21.0	UD	21.0	100	ug/L
127-18-4	Tetrachloroethene	44.2	JD	23.0	100	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	50.4		70 (74) - 130 (125)	101%	SPK: 50
1868-53-7	Dibromofluoromethane	50.2		70 (75) - 130 (124)	100%	SPK: 50
2037-26-5	Toluene-d8	54.4		70 (86) - 130 (113)	109%	SPK: 50
460-00-4	4-Bromofluorobenzene	54.7		70 (77) - 130 (121)	109%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	110000	5.562			
540-36-3	1,4-Difluorobenzene	219000	6.769			
3114-55-4	Chlorobenzene-d5	224000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	112000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046599.D
 Acq On : 10 Jun 2025 13:55
 Operator : JC/MD
 Sample : Q2234-01DL 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-17B-55-060425DL

Quant Time: Jun 11 01:47:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	110214	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	218656	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	224113	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	112148	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	98868	50.422	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 100.840%	
35) Dibromofluoromethane	5.397	113	80756	50.222	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.440%	
50) Toluene-d8	8.653	98	288466	54.414	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 108.820%	
62) 4-Bromofluorobenzene	11.079	95	120075	54.744	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 109.480%	
Target Compounds						Qvalue
9) 1,1,2-Trichlorotrifluo...	2.355	101	976	0.674	ug/l	93
27) cis-1,2-Dichloroethene	4.507	96	27823	16.322	ug/l	86
44) Trichloroethene	7.135	130	61302	37.312	ug/l	98
64) Tetrachloroethene	9.281	164	662	0.442	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046599.D
Acq On : 10 Jun 2025 13:55
Operator : JC/MD
Sample : Q2234-01DL 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-17B-55-060425DL

Quant Time: Jun 11 01:47:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

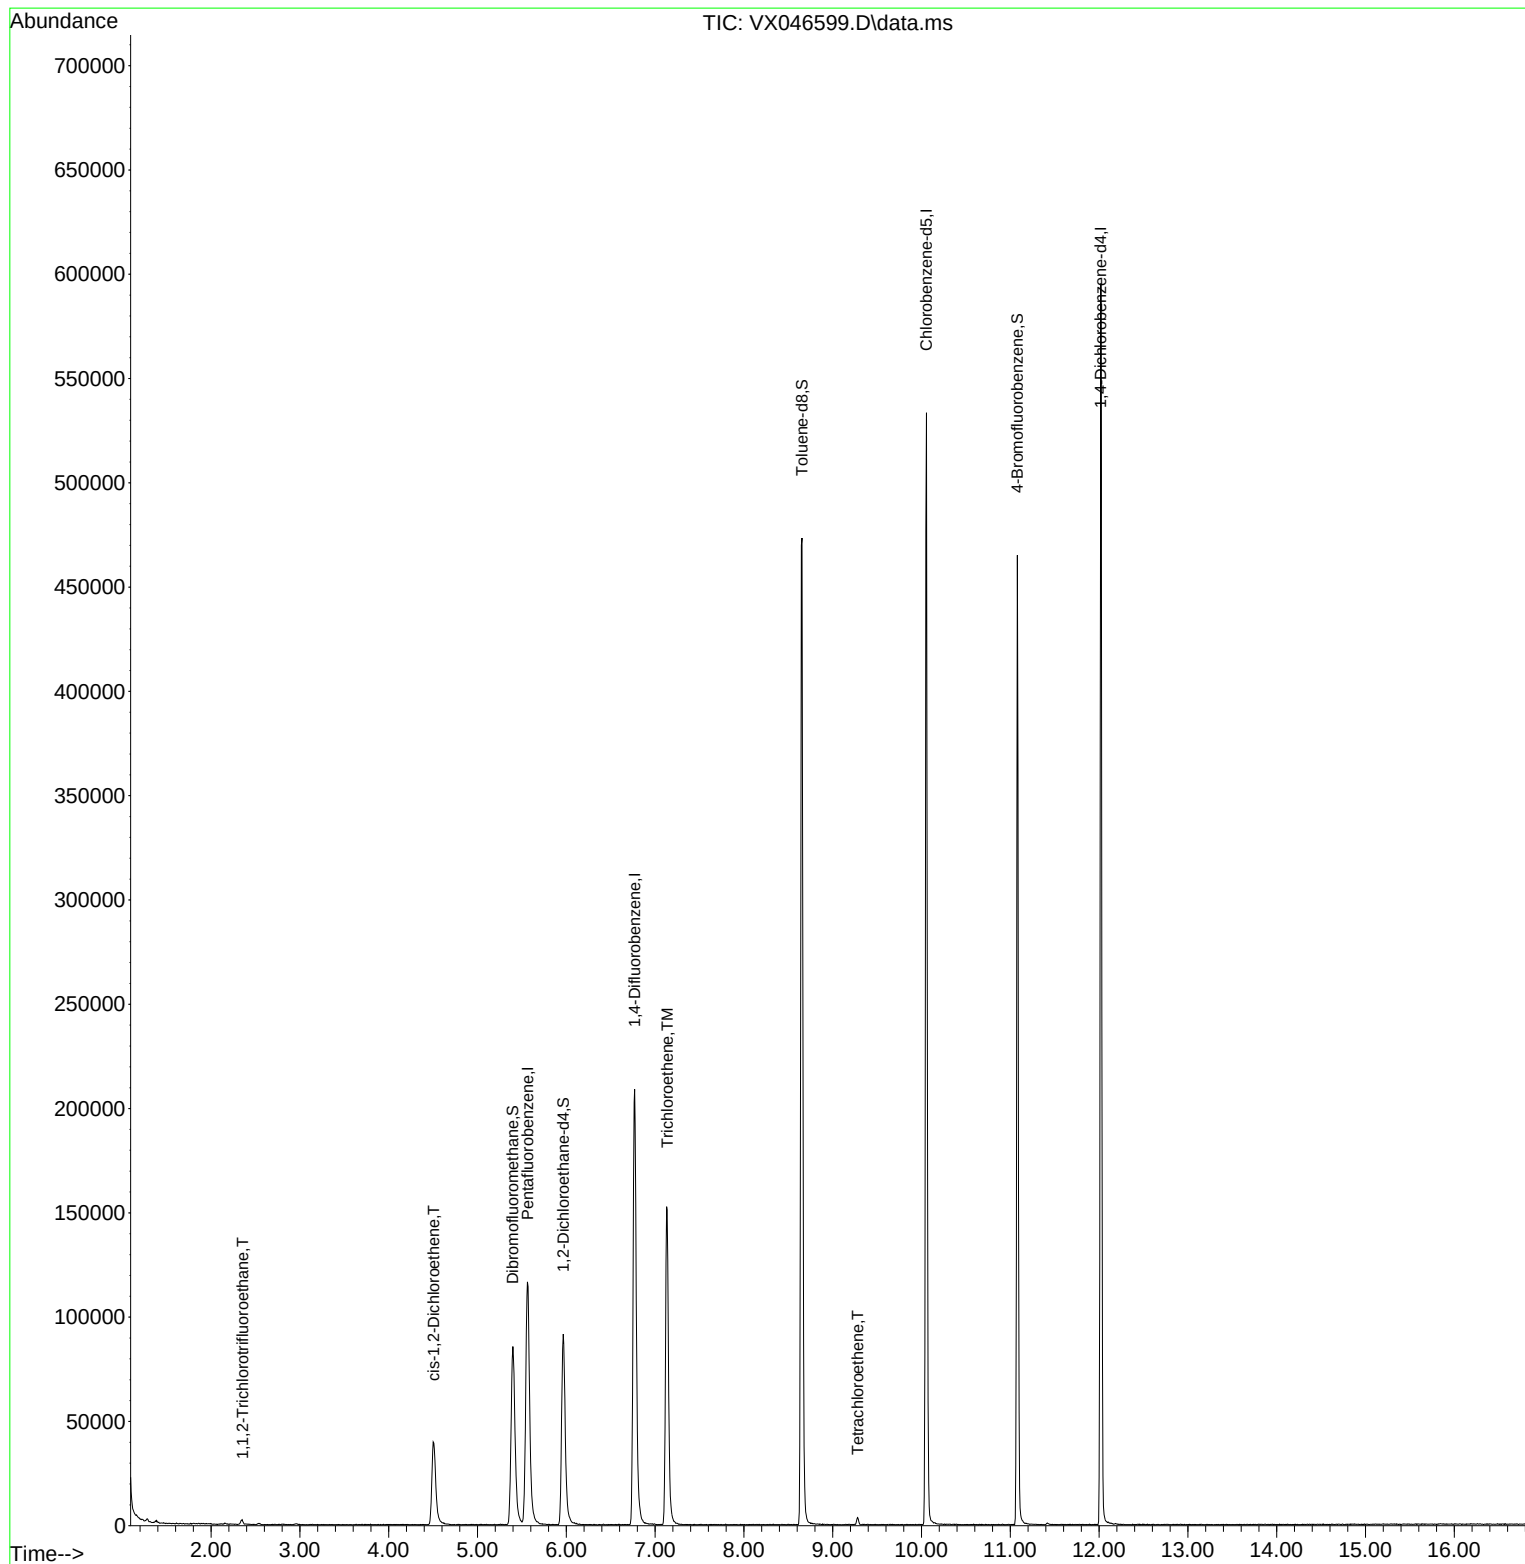



#1
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.562 min Scan# 71

Delta R.T. -0.006 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55

Instrument :

MSVOA_X

ClientSampleId :





MW-17B-55-060425DL

Tgt Ion:168 Resp: 110214

Ion Ratio Lower Upper

168 100

99 72.0 54.9 82.3

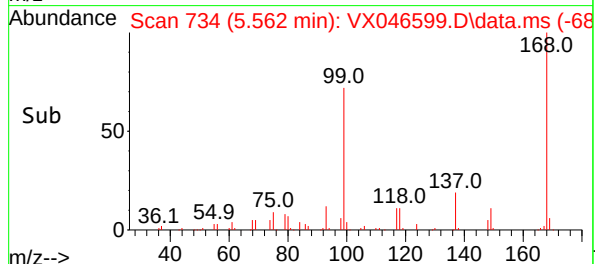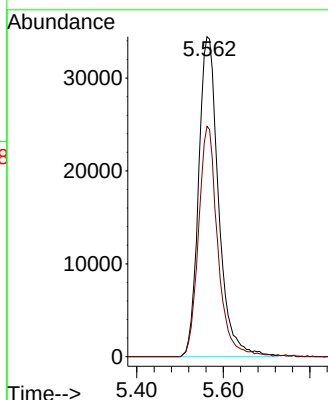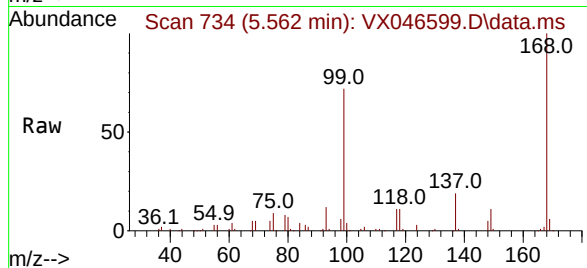

#9

1,1,2-Trichlorotrifluoroethane

Concen: 0.674 ug/l

RT: 2.355 min Scan# 208

Delta R.T. 0.006 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55




Tgt Ion:101 Resp: 976


Ion Ratio Lower Upper

101 100

85 41.3 38.6 58.0

151 65.7 55.2 82.8

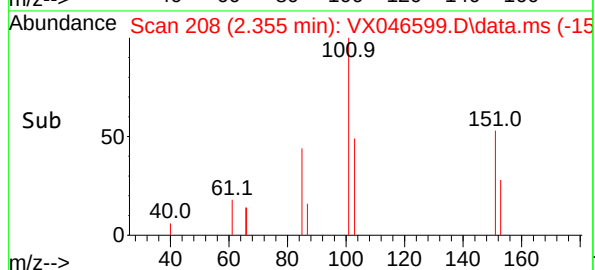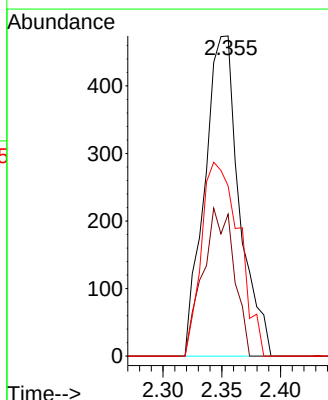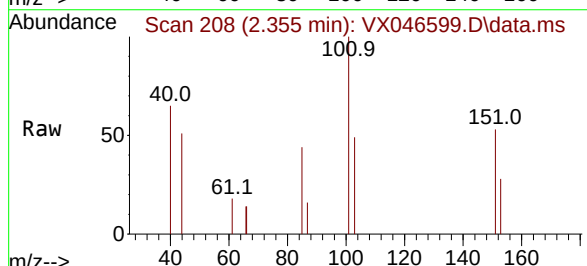



#27

cis-1,2-Dichloroethene

Concen: 16.322 ug/l

RT: 4.507 min Scan# 50

Delta R.T. 0.000 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55

Instrument :

MSVOA_X

ClientSampleId :

MW-17B-55-060425DL





Tgt Ion: 96 Resp: 27823

Ion Ratio Lower Upper

96 100

61 136.5 0.0 322.8

98 65.1 0.0 129.0

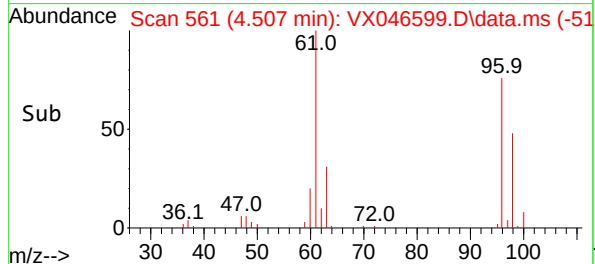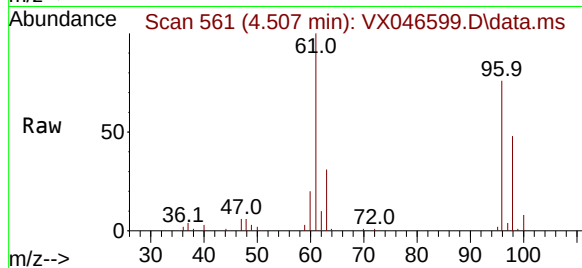

#33

1,2-Dichloroethane-d4

Concen: 50.422 ug/l

RT: 5.964 min Scan# 800

Delta R.T. -0.006 min

Lab File: VX046599.D




Acq: 10 Jun 2025 13:55


Tgt Ion: 65 Resp: 98868

Ion Ratio Lower Upper

65 100

67 50.1 0.0 99.0

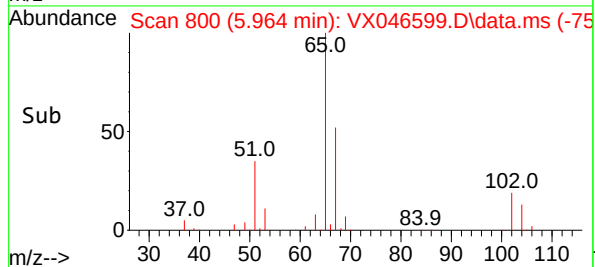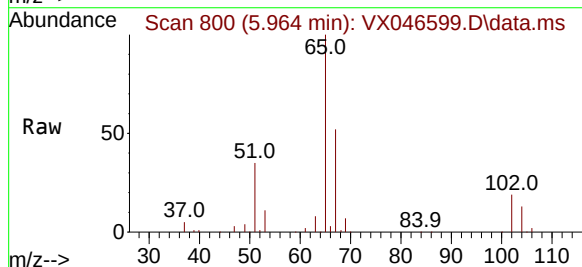



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 91

Delta R.T. -0.006 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55

Instrument :

MSVOA_X

ClientSampleId :

MW-17B-55-060425DL





Tgt Ion:114 Resp: 218656

Ion Ratio Lower Upper

114 100

63 22.4 0.0 49.2

88 16.7 0.0 33.6



#35

Dibromofluoromethane

Concen: 50.222 ug/l

RT: 5.397 min Scan# 707

Delta R.T. -0.006 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55




Tgt Ion:113 Resp: 80756


Ion Ratio Lower Upper

113 100

111 102.8 83.1 124.7

192 16.6 13.3 19.9

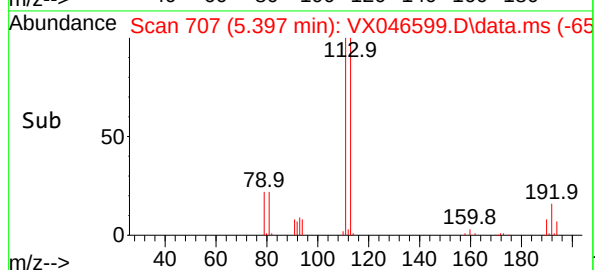



#44

Trichloroethene

Concen: 37.312 ug/l

RT: 7.135 min Scan# 99

Delta R.T. -0.000 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55

Instrument :

MSVOA_X

ClientSampleId :





MW-17B-55-060425DL

Tgt Ion:130 Resp: 61302

Ion Ratio Lower Upper

130 100

95 103.8 0.0 204.2

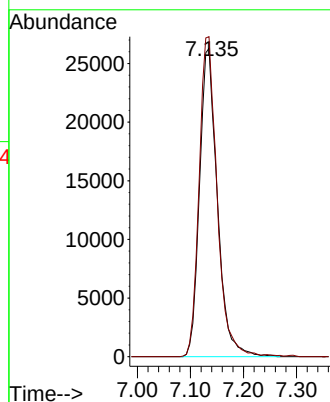

#50

Toluene-d8

Concen: 54.414 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX046599.D




Acq: 10 Jun 2025 13:55


Tgt Ion: 98 Resp: 288466

Ion Ratio Lower Upper

98 100

100 65.9 53.5 80.3

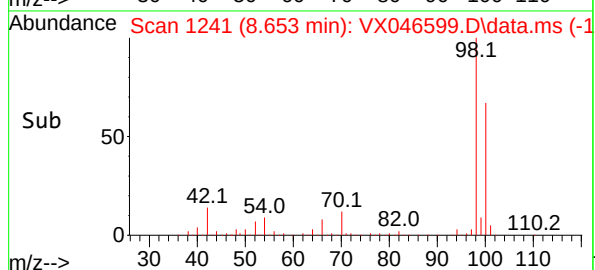



#62

4-Bromofluorobenzene

Concen: 54.744 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55

Instrument :

MSVOA_X

ClientSampleId :

MW-17B-55-060425DL





Tgt Ion: 95 Resp: 120075

Ion Ratio Lower Upper

95 100

174 68.5 0.0 135.8

176 66.9 0.0 131.4

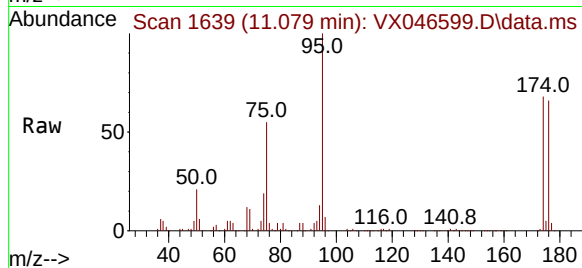

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55




Tgt Ion: 117 Resp: 224113


Ion Ratio Lower Upper

117 100

82 58.5 50.6 76.0

119 32.2 25.8 38.6

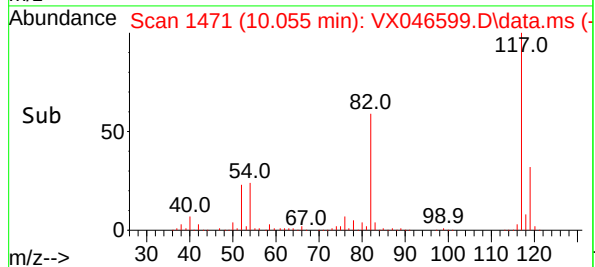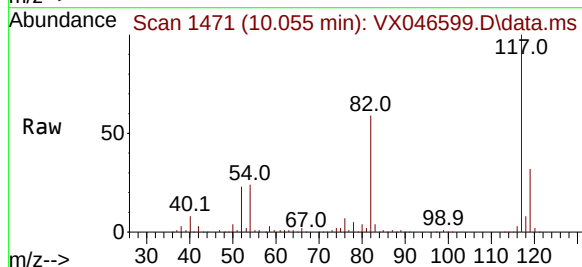



#64

Tetrachloroethene

Concen: 0.442 ug/l

RT: 9.281 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55

Instrument :

MSVOA_X

ClientSampleId :

MW-17B-55-060425DL

Tgt Ion:164 Resp: 662





Ion Ratio Lower Upper

164 100

166 108.9 105.0 157.6

129 82.7 83.5 125.3#

131 71.1 76.5 114.7#

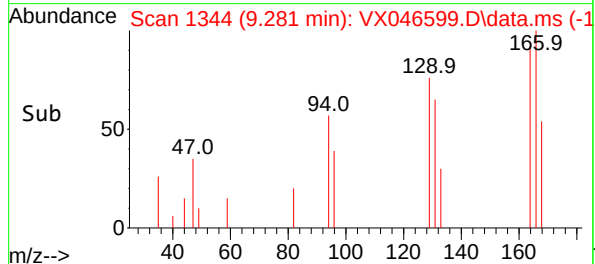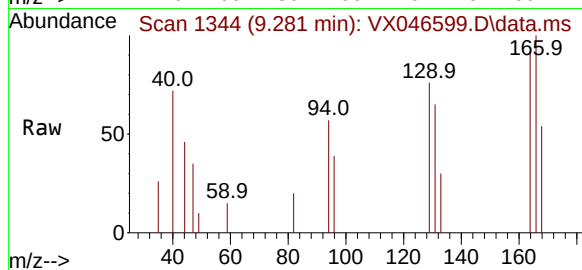

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX046599.D

Acq: 10 Jun 2025 13:55




Tgt Ion:152 Resp: 112148

Ion Ratio Lower Upper

152 100

115 64.2 46.9 140.7

150 157.5 0.0 351.0

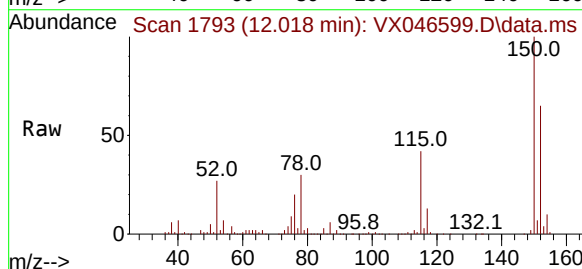



CALIBRATION SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: CHEMTECH Contract: JAC005
 Lab Code: CHEM Case No.: Q2234 SAS No.: Q2234 SDG No.: Q2234
 Instrument ID: MSVOA_X Calibration Date(s): 06/06/2025 06/06/2025
 Heated Purge: (Y/N) N Calibration Time(s): 09:42 12:57
 GC Column: DB-624UI ID: 0.18 (mm)

LAB FILE ID:		RRF005 = VX046518.D		RRF020 = VX046519.D		RRF050 = VX046520.D		
		RRF100 = VX046521.D		RRF150 = VX046522.D		RRF001 = VX046524.D		
COMPOUND	RRF005	RRF020	RRF050	RRF100	RRF150	RRF001	RRF	% RSD
Vinyl Chloride	0.697	0.593	0.596	0.591	0.622	0.679	0.630	7.5
1,1-Dichloroethene	0.663	0.550	0.567	0.561	0.585	0.635	0.594	7.6
1,1-Dichloroethane	1.349	1.266	1.259	1.234	1.297	1.281	1.281	3.1
cis-1,2-Dichloroethene	0.786	0.752	0.741	0.728	0.767	0.866	0.773	6.4
1,1,1-Trichloroethane	1.170	1.131	1.141	1.128	1.188	1.131	1.148	2.2
Benzene	1.597	1.503	1.427	1.380	1.442	1.522	1.479	5.3
1,2-Dichloroethane	0.646	0.641	0.610	0.586	0.602	0.606	0.615	3.8
Trichloroethene	0.385	0.356	0.351	0.332	0.354	0.476	0.376	13.8
1,1,2-Trichloroethane	0.375	0.389	0.366	0.356	0.372	0.331	0.365	5.4
Tetrachloroethene	0.347	0.324	0.310	0.301	0.314	0.410	0.334	12.1
1,2-Dichloroethane-d4	0.997	0.848	0.873	0.828	0.900		0.890	7.4
Dibromofluoromethane	0.392	0.353	0.368	0.347	0.379		0.368	5
Toluene-d8	1.362	1.159	1.188	1.132	1.220		1.212	7.4
4-Bromofluorobenzene	0.564	0.482	0.493	0.468	0.501		0.502	7.4

* Compounds with required minimum RRF and maximum %RSD values.
 All other compounds must meet a minimum RRF of 0.010.
 RRF of 1,4-Dioxane = Value should be divide by 1000.

Method Path : Z:\voasrv\HPCHEM1\MSVOA_X\Method\
 Method File : 82X060625W.M
 Title : SW846 8260
 Last Update : Fri Jun 06 16:56:12 2025
 Response Via : Initial Calibration

Calibration Files

1 =VX046524.D 5 =VX046518.D 20 =VX046519.D 50 =VX046520.D 100 =VX046521.D 150 =VX046522.D

Compound		1	5	20	50	100	150	Avg	%RSD

1) I	Pentafluorobenzene	-----ISTD-----							
2) T	Dichlorodifluo...	0.838	0.740	0.653	0.645	0.635	0.654	0.694	11.52
3) P	Chloromethane	0.713	0.737	0.586	0.573	0.568	0.614	0.632	11.76
4) C	Vinyl Chloride	0.679	0.697	0.593	0.596	0.591	0.622	0.630	7.46#
5) T	Bromomethane		0.592	0.429	0.398	0.256	0.237	0.382	37.77
6) T	Chloroethane	0.509	0.456	0.384	0.373	0.357	0.373	0.409	14.73
7) T	Trichlorofluor...	1.019	1.136	1.055	1.021	0.988	1.034	1.042	4.89
8) T	Diethyl Ether	0.412	0.368	0.355	0.356	0.349	0.368	0.368	6.23
9) T	1,1,2-Trichlor...	0.697	0.699	0.651	0.638	0.616	0.639	0.657	5.19
10) T	Methyl Iodide		0.653	0.664	0.716	0.744	0.782	0.712	7.65
11) T	Tert butyl alc...		0.087	0.090	0.098	0.104	0.114	0.099	10.94
12) CM	1,1-Dichloroet...	0.635	0.663	0.550	0.567	0.561	0.585	0.594	7.64#
13) T	Acrolein		0.040	0.110	0.112	0.117	0.135	0.103	35.72
14) T	Allyl chloride	1.283	1.198	1.115	1.130	1.138	1.131	1.166	5.52
15) T	Acrylonitrile	0.342	0.367	0.368	0.379	0.381	0.403	0.373	5.42
16) T	Acetone	0.566	0.347	0.334	0.340	0.341	0.360	0.381	23.86
17) T	Carbon Disulfide	2.313	1.618	1.229	1.218	1.220	1.288	1.481	29.41
18) T	Methyl Acetate	0.883	0.870	1.082	1.130	1.155	1.237	1.060	14.20
19) T	Methyl tert-bu...	1.873	2.038	2.050	2.115	2.131	2.256	2.077	6.11
20) T	Methylene Chlo...	0.868	0.752	0.676	0.662	0.646	0.678	0.714	11.77
21) T	trans-1,2-Dich...	0.785	0.661	0.580	0.582	0.567	0.594	0.628	13.34
22) T	Diisopropyl ether	2.017	2.338	2.344	2.343	2.319	2.429	2.298	6.22
23) T	Vinyl Acetate	1.639	1.727	1.682	1.828	1.831	1.940	1.775	6.31
24) P	1,1-Dichloroet...	1.281	1.349	1.266	1.259	1.234	1.297	1.281	3.09
25) T	2-Butanone	0.484	0.459	0.469	0.503	0.511	0.544	0.495	6.28
26) T	2,2-Dichloropr...	0.900	0.931	0.919	0.966	0.968	1.022	0.951	4.61
27) T	cis-1,2-Dichlo...	0.866	0.786	0.752	0.741	0.728	0.767	0.773	6.43
28) T	Bromochloromet...	0.650	0.652	0.592	0.590	0.594	0.589	0.611	5.04
29) T	Tetrahydrofuran	0.306	0.301	0.291	0.316	0.320	0.342	0.313	5.64
30) C	Chloroform	1.349	1.392	1.356	1.318	1.290	1.349	1.342	2.59#
31) T	Cyclohexane		1.172	1.012	0.995	0.974	1.018	1.034	7.64
32) T	1,1,1-Trichlor...	1.131	1.170	1.131	1.141	1.128	1.188	1.148	2.17
33) S	1,2-Dichloroet...		0.997	0.848	0.873	0.828	0.900	0.890	7.42
34) I	1,4-Difluorobenzene	-----ISTD-----							
35) S	Dibromofluorom...		0.392	0.353	0.368	0.347	0.379	0.368	5.01
36) T	1,1-Dichloropr...	0.660	0.554	0.506	0.485	0.461	0.485	0.525	13.89
37) T	Ethyl Acetate	0.355	0.483	0.522	0.554	0.566	0.596	0.513	16.84
38) T	Carbon Tetrach...	0.655	0.599	0.579	0.564	0.554	0.579	0.588	6.09
39) T	Methylcyclohexane	0.725	0.696	0.576	0.572	0.565	0.587	0.620	11.41
40) TM	Benzene	1.522	1.597	1.503	1.427	1.380	1.442	1.479	5.25
41) T	Methacrylonitrile	0.279	0.310	0.335	0.323	0.320	0.344	0.318	7.09
42) TM	1,2-Dichloroet...	0.606	0.646	0.641	0.610	0.586	0.602	0.615	3.80
43) T	Isopropyl Acetate	0.772	0.842	0.887	0.923	0.935	1.002	0.894	8.92
44) TM	Trichloroethene	0.476	0.385	0.356	0.351	0.332	0.354	0.376	13.85
45) C	1,2-Dichloropr...	0.359	0.393	0.396	0.381	0.370	0.390	0.382	3.84#
46) T	Dibromomethane	0.291	0.308	0.286	0.279	0.272	0.286	0.287	4.22
47) T	Bromodichlorom...	0.534	0.580	0.617	0.603	0.589	0.618	0.590	5.32
48) T	Methyl methacr...	0.395	0.423	0.454	0.481	0.490	0.517	0.460	9.79
49) T	1,4-Dioxane	0.004	0.006	0.007	0.006	0.007	0.007	0.006	14.38
50) S	Toluene-d8		1.362	1.159	1.188	1.132	1.220	1.212	7.42
51) T	4-Methyl-2-Pen...	0.492	0.548	0.583	0.593	0.582	0.609	0.568	7.47
52) CM	Toluene	0.938	0.980	0.911	0.884	0.849	0.888	0.908	5.04#
53) T	t-1,3-Dichloro...	0.480	0.469	0.524	0.542	0.559	0.601	0.529	9.38
54) T	cis-1,3-Dichlo...	0.567	0.567	0.580	0.590	0.595	0.633	0.589	4.15
55) T	1,1,2-Trichlor...	0.331	0.375	0.389	0.366	0.356	0.372	0.365	5.41
56) T	Ethyl methacry...	0.456	0.536	0.566	0.583	0.594	0.632	0.561	10.79


Method Path : Z:\voasrv\HPCHEM1\MSVOA_X\Method\
 Method File : 82X060625W.M

57)	T	1,3-Dichloropr...	0.653	0.664	0.666	0.636	0.612	0.637	0.644	3.15
58)	T	2-Chloroethyl ...	0.278	0.301	0.302	0.316	0.312	0.326	0.306	5.46
59)	T	2-Hexanone	0.368	0.376	0.416	0.426	0.419	0.438	0.407	6.99
60)	T	Dibromochlorom...	0.405	0.431	0.438	0.432	0.422	0.447	0.429	3.35
61)	T	1,2-Dibromoethane	0.420	0.367	0.380	0.370	0.365	0.378	0.380	5.37
62)	S	4-Bromofluorob...	0.564	0.482	0.493	0.468	0.501	0.502		7.36
63)	I	Chlorobenzene-d5	-----ISTD-----							
64)	T	Tetrachloroethene	0.410	0.347	0.324	0.310	0.301	0.314	0.334	12.07
65)	PM	Chlorobenzene	1.356	1.187	1.152	1.126	1.096	1.139	1.176	7.91
66)	T	1,1,1,2-Tetrac...	0.362	0.394	0.401	0.403	0.404	0.420	0.397	4.87
67)	C	Ethyl Benzene	2.166	2.093	2.029	2.018	1.971	2.041	2.053	3.30#
68)	T	m/p-Xylenes	0.773	0.756	0.750	0.737	0.714	0.738	0.745	2.67
69)	T	o-Xylene	0.719	0.728	0.731	0.716	0.703	0.724	0.720	1.42
70)	T	Styrene	1.209	1.205	1.257	1.257	1.213	1.257	1.233	2.15
71)	P	Bromoform	0.286	0.269	0.300	0.311	0.317	0.335	0.303	7.76
72)	I	1,4-Dichlorobenzen...	-----ISTD-----							
73)	T	Isopropylbenzene	3.896	3.936	3.949	3.909	3.828	4.064	3.930	1.98
74)	T	N-amyl acetate	1.424	1.613	1.673	1.803	1.854	2.019	1.731	11.98
75)	P	1,1,2,2-Tetrac...	1.148	1.294	1.294	1.257	1.249	1.306	1.258	4.65
76)	T	1,2,3-Trichlor...	1.091	1.022	1.076	1.049	1.025	1.092	1.059	2.97
77)	T	Bromobenzene	0.958	0.904	0.925	0.881	0.878	0.928	0.912	3.36
78)	T	n-propylbenzene	5.051	4.659	4.775	4.693	4.553	4.813	4.757	3.58
79)	T	2-Chlorotoluene	3.087	2.885	2.870	2.786	2.721	2.866	2.869	4.31
80)	T	1,3,5-Trimethy...	3.322	3.329	3.297	3.243	3.147	3.314	3.275	2.14
81)	T	trans-1,4-Dich...	0.274	0.352	0.370	0.398	0.442	0.367		16.86
82)	T	4-Chlorotoluene	3.872	3.390	3.342	3.293	3.177	3.329	3.400	7.12
83)	T	tert-Butylbenzene	3.284	3.341	3.364	3.287	3.248	3.482	3.334	2.50
84)	T	1,2,4-Trimethy...	3.406	3.309	3.360	3.256	3.194	3.356	3.313	2.34
85)	T	sec-Butylbenzene	4.458	4.350	4.296	4.172	4.096	4.334	4.284	3.04
86)	T	p-Isopropyltol...	3.910	3.509	3.554	3.484	3.397	3.575	3.572	4.96
87)	T	1,3-Dichlorobe...	2.105	1.745	1.714	1.684	1.642	1.740	1.772	9.46
88)	T	1,4-Dichlorobe...	2.421	1.804	1.736	1.675	1.627	1.752	1.836	15.98
89)	T	n-Butylbenzene	4.197	3.319	3.378	3.354	3.310	3.487	3.507	9.80
90)	T	Hexachloroethane	0.682	0.599	0.602	0.610	0.633	0.683	0.635	6.11
91)	T	1,2-Dichlorobe...	1.908	1.730	1.693	1.639	1.595	1.695	1.710	6.32
92)	T	1,2-Dibromo-3-...	0.238	0.250	0.272	0.285	0.309	0.337	0.282	13.06
93)	T	1,2,4-Trichlor...	1.513	1.038	1.085	1.077	1.093	1.194	1.167	15.22
94)	T	Hexachlorobuta...	0.695	0.526	0.508	0.501	0.497	0.525	0.542	14.01
95)	T	Naphthalene	3.783	3.138	3.527	3.726	3.816	4.205	3.699	9.53
96)	T	1,2,3-Trichlor...	1.500	1.042	1.078	1.092	1.108	1.198	1.170	14.55

(#) = Out of Range

Acrolein

Response Ratio

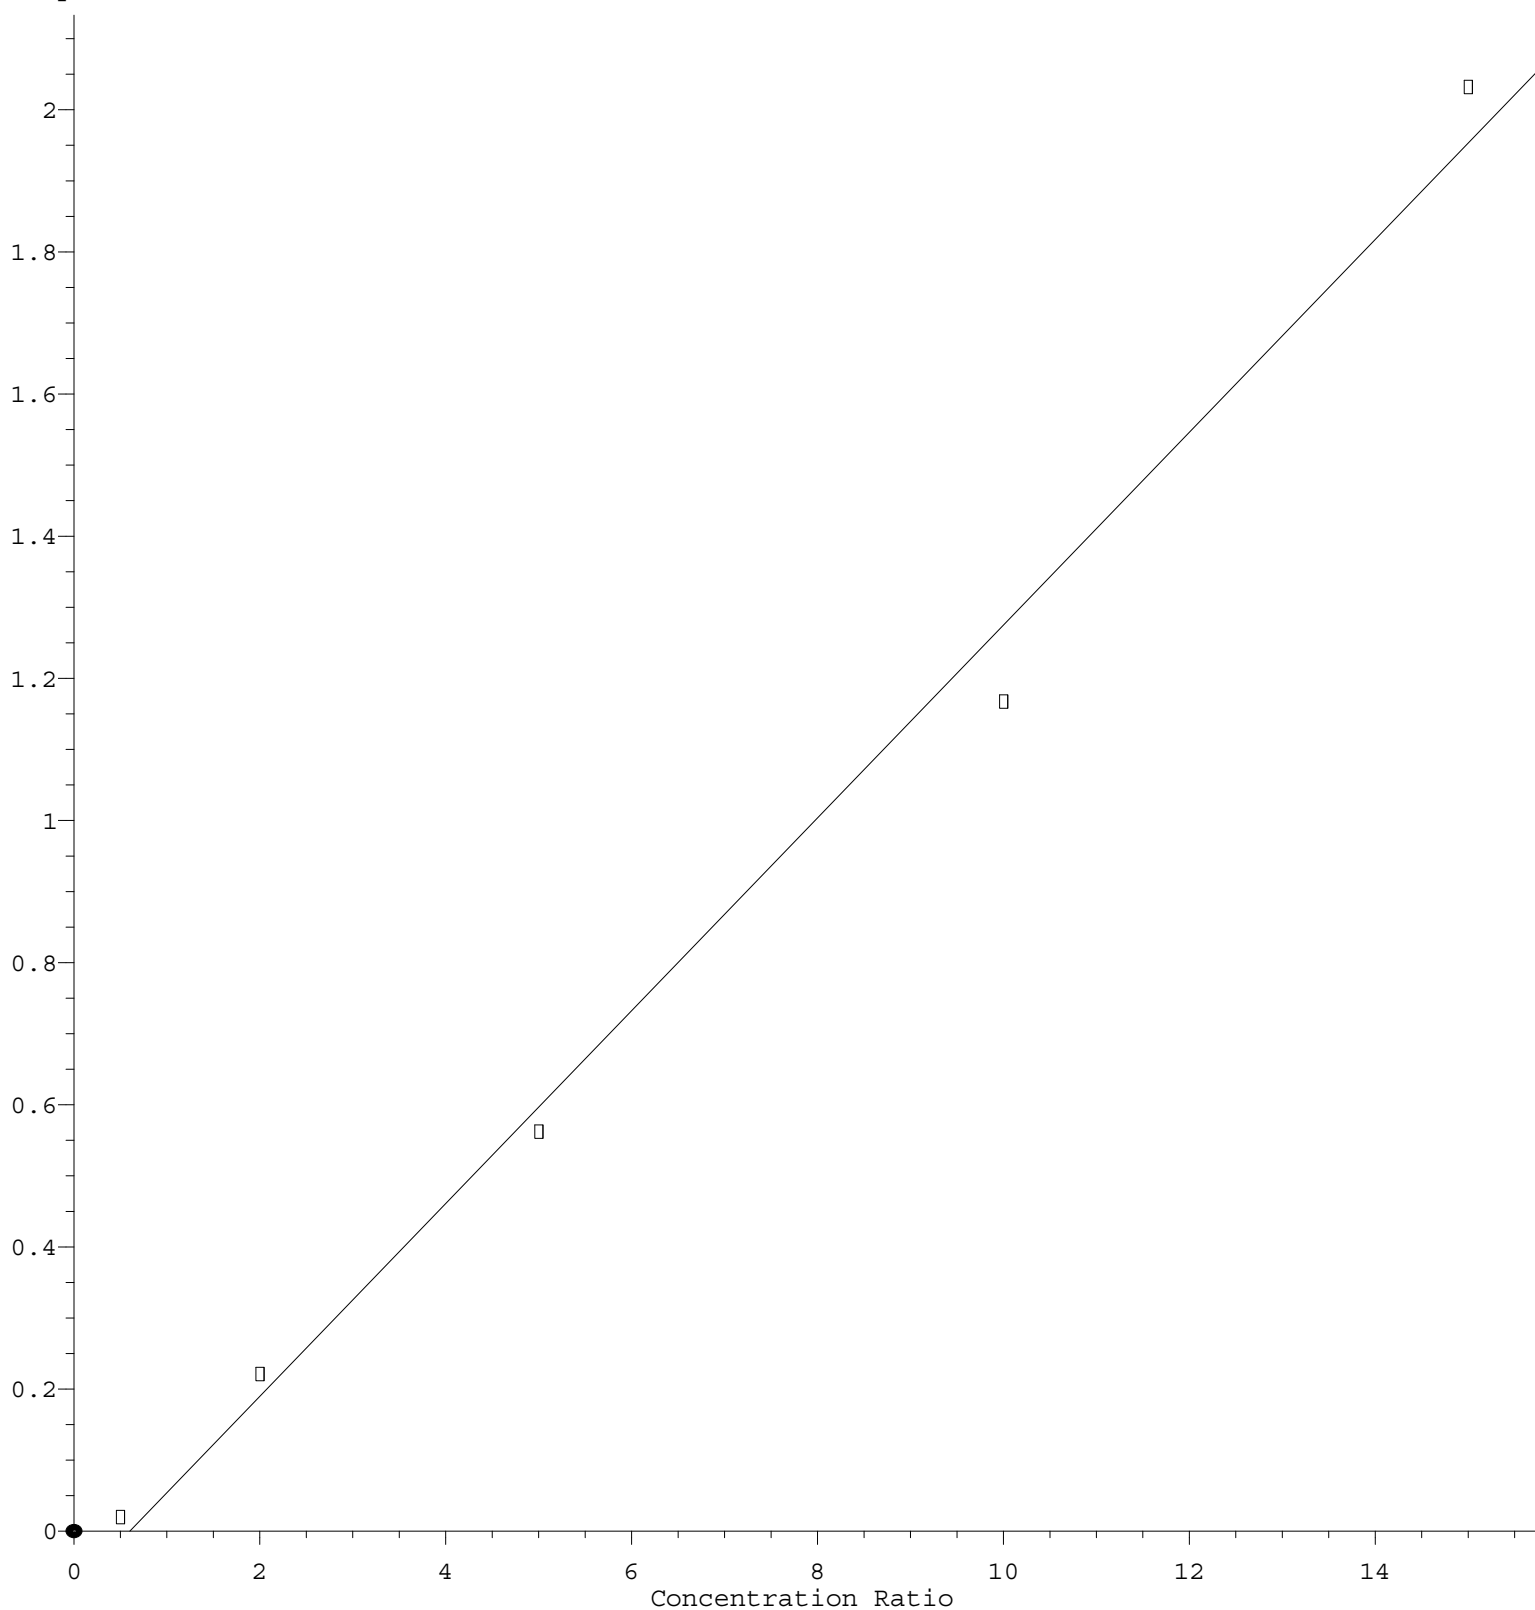

$$\text{Response} = 1.357\text{e-}001 * \text{Amt} - 8.141\text{e-}002$$


Coef of Det (r^2) = 0.992061 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060625W.M

Calibration Table Last Updated: Fri Jun 06 16:56:12 2025

Acetone


Response Ratio

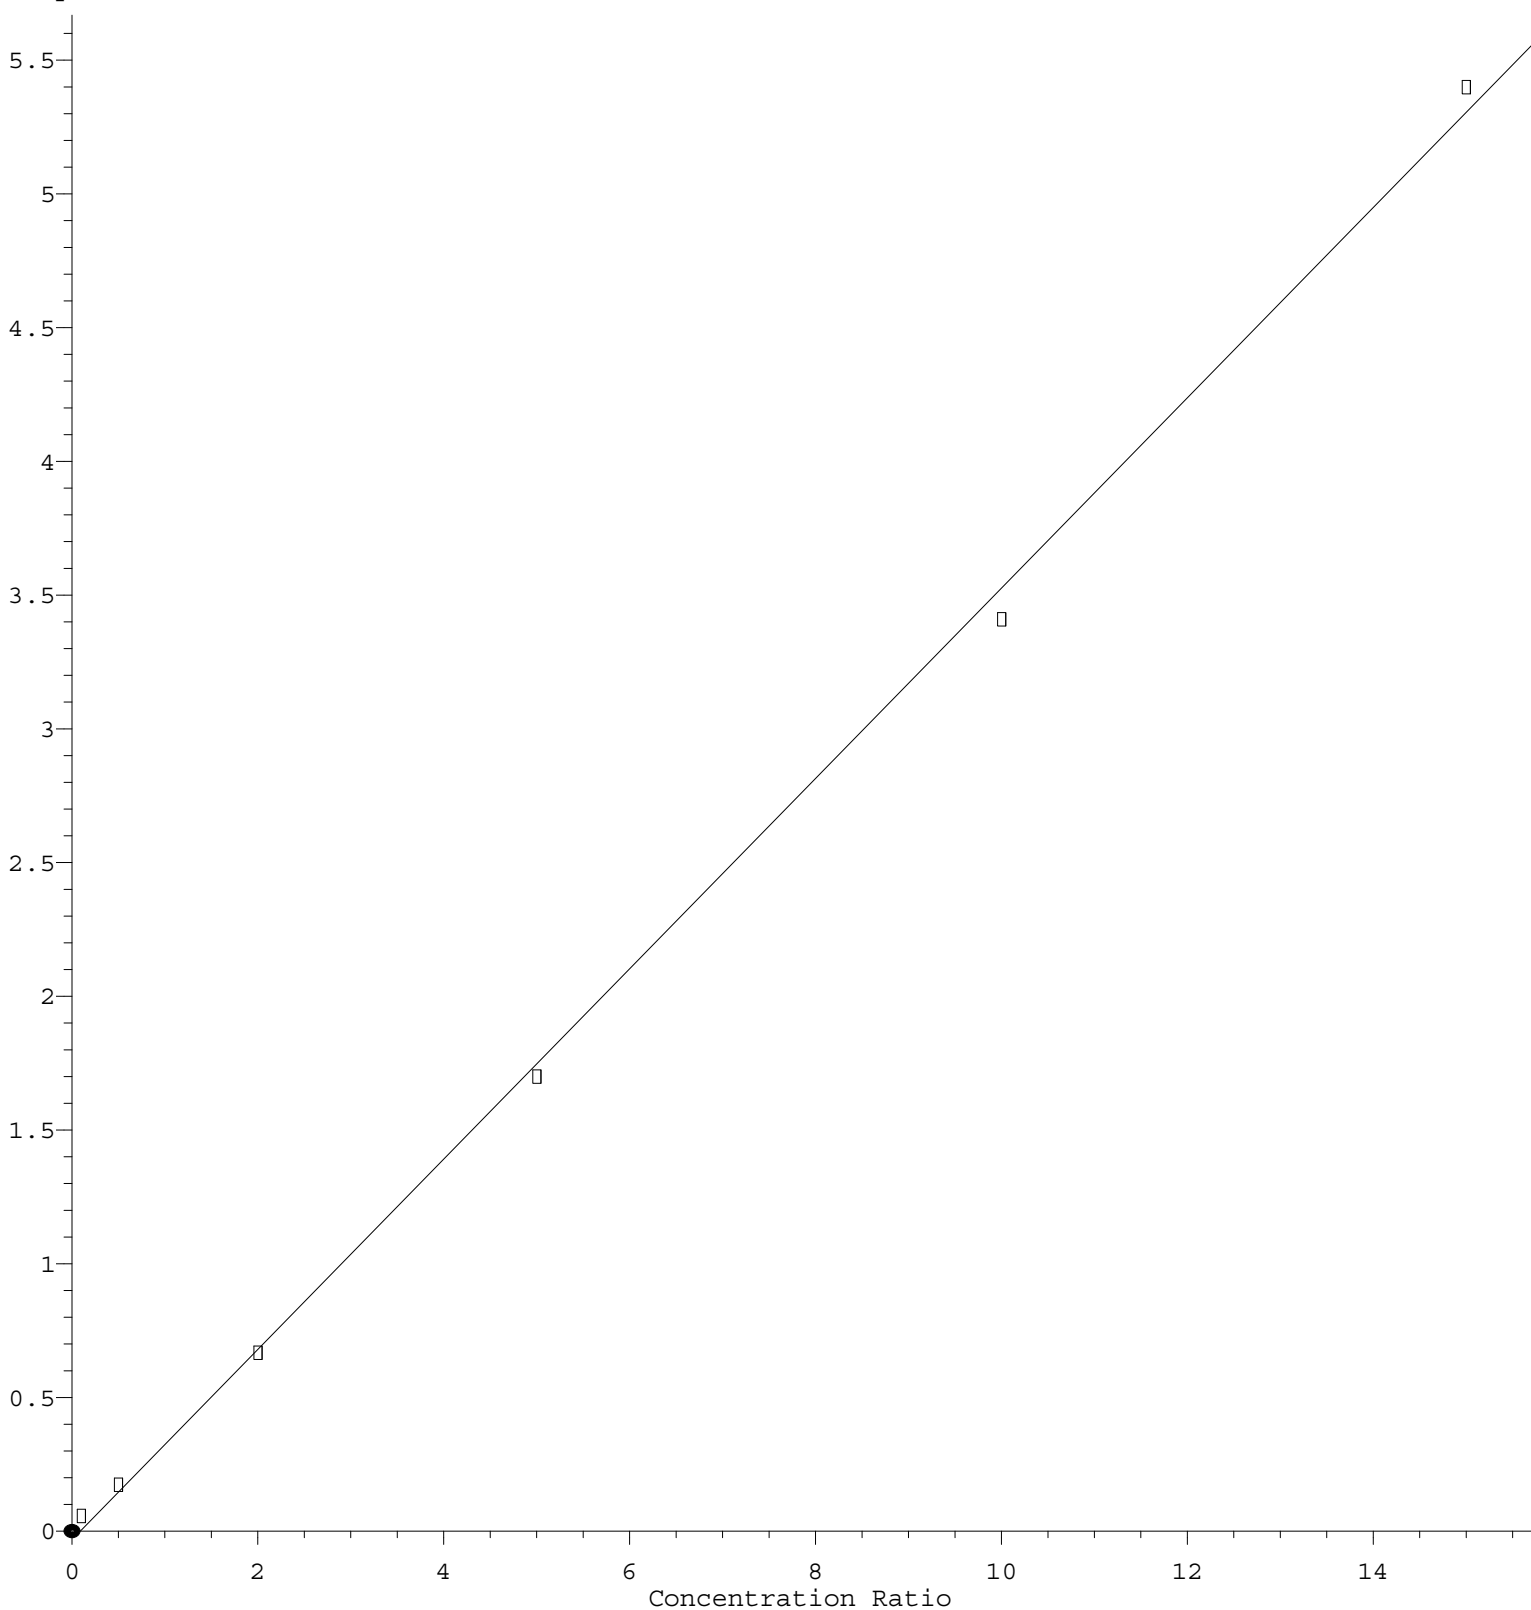

$\text{Response} = 3.559\text{e-}001 * \text{Amt} - 3.270\text{e-}002$
 Coef of Det (r^2) = 0.998736 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060625W.M
 Calibration Table Last Updated: Fri Jun 06 16:56:12 2025

Carbon Disulfide

Response Ratio

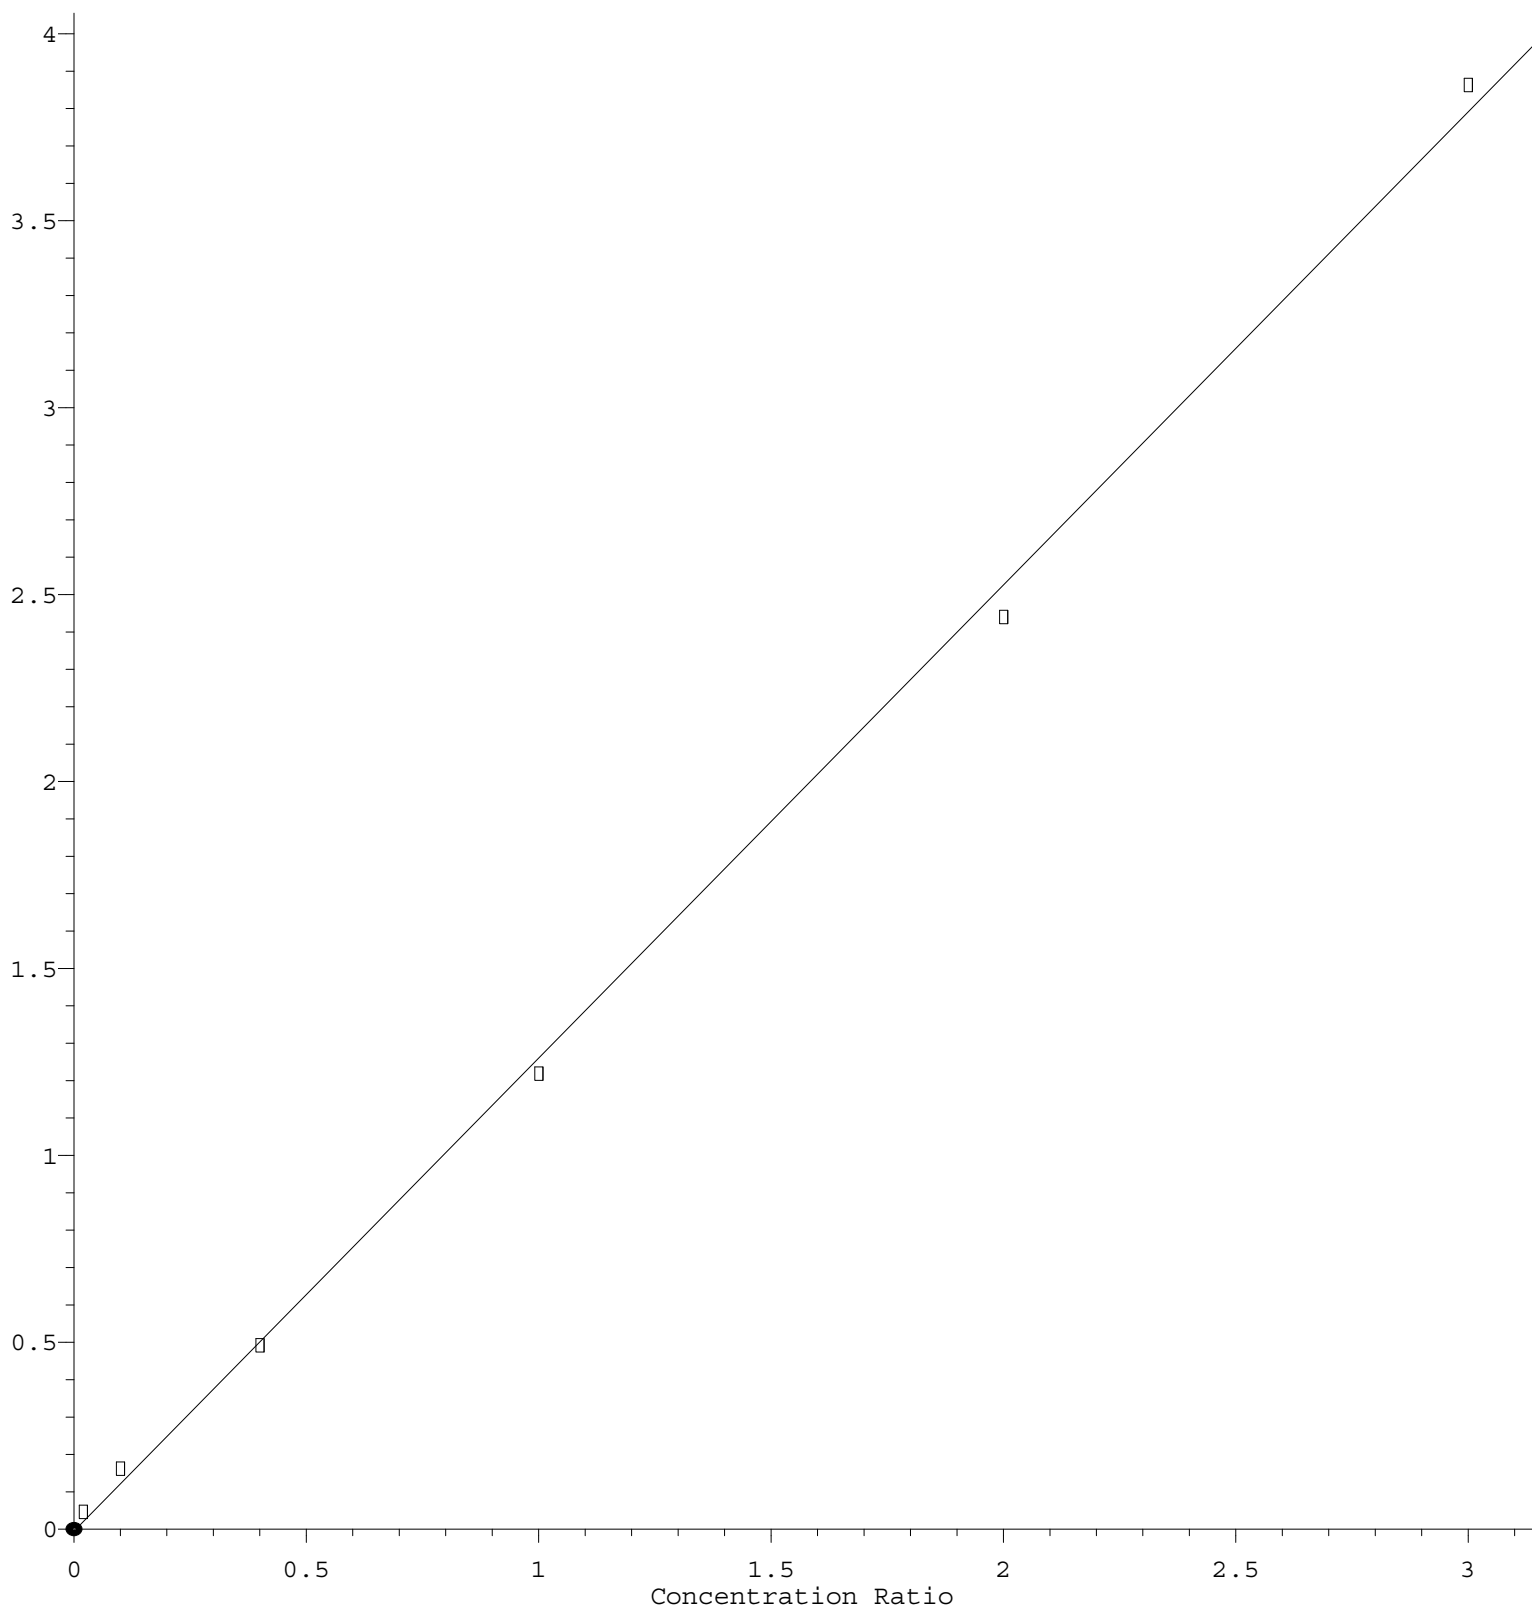

$$\text{Response} = 1.266\text{e}+000 * \text{Amt} - 5.124\text{e}-003$$

Coef of Det (r^2) = 0.998532 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X060625W.M

Calibration Table Last Updated: Fri Jun 06 16:56:12 2025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046518.D
 Acq On : 06 Jun 2025 09:42
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC005

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:40:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	104428	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	181356	50.000	ug/l	-0.01
63) Chlorobenzene-d5	10.055	117	164496	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	81515	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	10415	5.606	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	11.220%#		
35) Dibromofluoromethane	5.391	113	7110	5.331	ug/l	-0.01
Spiked Amount 50.000	Range 75 - 124		Recovery =	10.660%#		
50) Toluene-d8	8.653	98	24704	5.618	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	11.240%#		
62) 4-Bromofluorobenzene	11.079	95	10224	5.620	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	11.240%#		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.179	85	7726	5.329	ug/l	99
3) Chloromethane	1.307	50	7698	5.833	ug/l	99
4) Vinyl Chloride	1.386	62	7283	5.536	ug/l	92
5) Bromomethane	1.618	94	6181	7.740	ug/l	89
6) Chloroethane	1.697	64	4764	5.582	ug/l	98
7) Trichlorofluoromethane	1.904	101	11861	5.450	ug/l	97
8) Diethyl Ether	2.148	74	3843	4.997	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.349	101	7299	5.323	ug/l	98
10) Methyl Iodide	2.465	142	6815	4.585	ug/l	96
11) Tert butyl alcohol	2.971	59	4565	22.143	ug/l	97
12) 1,1-Dichloroethene	2.331	96	6923	5.584	ug/l	92
13) Acrolein	2.246	56	2067	37.301	ug/l	95
14) Allyl chloride	2.678	41	12513	5.139	ug/l	99
15) Acrylonitrile	3.075	53	19139	24.554	ug/l	100
16) Acetone	2.392	43	18117	28.970	ug/l	92
17) Carbon Disulfide	2.526	76	16895	6.594	ug/l	99
18) Methyl Acetate	2.715	43	9089	4.107	ug/l	98
19) Methyl tert-butyl Ether	3.130	73	21281	4.905	ug/l	100
20) Methylene Chloride	2.800	84	7851	5.267	ug/l	95
21) trans-1,2-Dichloroethene	3.105	96	6901	5.260	ug/l	87
22) Diisopropyl ether	3.770	45	24417	5.086	ug/l #	55
23) Vinyl Acetate	3.739	43	90187	24.333	ug/l	97
24) 1,1-Dichloroethane	3.617	63	14092	5.267	ug/l	98
25) 2-Butanone	4.581	43	23977	23.183	ug/l	98
26) 2,2-Dichloropropane	4.483	77	9718	4.893	ug/l	95
27) cis-1,2-Dichloroethene	4.495	96	8212	5.084	ug/l	97
28) Bromochloromethane	4.910	49	6807	5.334	ug/l #	99
29) Tetrahydrofuran	5.026	42	15713	24.057	ug/l	93
30) Chloroform	5.099	83	14532	5.184	ug/l	94
31) Cyclohexane	5.483	56	12241	5.667	ug/l	89
32) 1,1,1-Trichloroethane	5.391	97	12216	5.094	ug/l	97
36) 1,1-Dichloropropene	5.702	75	10048	5.274	ug/l	96
37) Ethyl Acetate	4.733	43	8766	4.716	ug/l #	89
38) Carbon Tetrachloride	5.690	117	10857	5.088	ug/l	98
39) Methylcyclohexane	7.385	83	12614	5.610	ug/l	97
40) Benzene	6.044	78	28961	5.400	ug/l	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046518.D
 Acq On : 06 Jun 2025 09:42
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC005

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:40:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.940	41	5621	4.868	ug/l #	90
42) 1,2-Dichloroethane	6.092	62	11718	5.252	ug/l	100
43) Isopropyl Acetate	6.349	43	15275	4.712	ug/l #	97
44) Trichloroethene	7.129	130	6978	5.121	ug/l	99
45) 1,2-Dichloropropane	7.434	63	7132	5.152	ug/l	97
46) Dibromomethane	7.586	93	5588	5.366	ug/l	97
47) Bromodichloromethane	7.824	83	10524	4.915	ug/l	97
48) Methyl methacrylate	7.708	41	7663	4.595	ug/l	97
49) 1,4-Dioxane	7.665	88	2221	99.585	ug/l	98
51) 4-Methyl-2-Pentanone	8.574	43	49709	24.133	ug/l	99
52) Toluene	8.720	92	17773	5.394	ug/l	99
53) t-1,3-Dichloropropene	8.982	75	8503	4.429	ug/l	100
54) cis-1,3-Dichloropropene	8.373	75	10282	4.817	ug/l	92
55) 1,1,2-Trichloroethane	9.153	97	6794	5.136	ug/l	97
56) Ethyl methacrylate	9.122	69	9723	4.777	ug/l	97
57) 1,3-Dichloropropane	9.311	76	12033	5.148	ug/l	98
58) 2-Chloroethyl Vinyl ether	8.245	63	27324	24.645	ug/l	97
59) 2-Hexanone	9.433	43	34128	23.102	ug/l	98
60) Dibromochloromethane	9.519	129	7808	5.018	ug/l	96
61) 1,2-Dibromoethane	9.610	107	6661	4.833	ug/l	94
64) Tetrachloroethene	9.275	164	5704	5.186	ug/l	90
65) Chlorobenzene	10.080	112	19529	5.048	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	6488	4.963	ug/l	98
67) Ethyl Benzene	10.195	91	34429	5.098	ug/l	98
68) m/p-Xylenes	10.299	106	24857	10.146	ug/l	99
69) o-Xylene	10.640	106	11976	5.054	ug/l	99
70) Styrene	10.659	104	19826	4.888	ug/l	98
71) Bromoform	10.799	173	4418	4.432	ug/l #	96
73) Isopropylbenzene	10.964	105	32087	5.007	ug/l	99
74) N-amyl acetate	10.848	43	13145	4.658	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.214	83	10551	5.144	ug/l	98
76) 1,2,3-Trichloropropane	11.238	75	8330m	4.746	ug/l	
77) Bromobenzene	11.195	156	7367	4.953	ug/l	98
78) n-propylbenzene	11.305	91	37974	4.896	ug/l	99
79) 2-Chlorotoluene	11.366	91	23514	5.028	ug/l	100
80) 1,3,5-Trimethylbenzene	11.451	105	27140	5.083	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	2236	3.736	ug/l #	77
82) 4-Chlorotoluene	11.457	91	27633	4.985	ug/l	97
83) tert-Butylbenzene	11.713	119	27238	5.011	ug/l	99
84) 1,2,4-Trimethylbenzene	11.750	105	26973	4.993	ug/l	97
85) sec-Butylbenzene	11.890	105	35458	5.077	ug/l	97
86) p-Isopropyltoluene	12.006	119	28606	4.913	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	14222	4.924	ug/l	99
88) 1,4-Dichlorobenzene	12.043	146	14704	4.913	ug/l	87
89) n-Butylbenzene	12.329	91	27055	4.731	ug/l	99
90) Hexachloroethane	12.536	117	4884	4.719	ug/l	93
91) 1,2-Dichlorobenzene	12.335	146	14100	5.058	ug/l	98
92) 1,2-Dibromo-3-Chloropr...	12.945	75	2035	4.431	ug/l	95
93) 1,2,4-Trichlorobenzene	13.585	180	8458	4.447	ug/l	99
94) Hexachlorobutadiene	13.725	225	4285	4.848	ug/l	97
95) Naphthalene	13.774	128	25583	4.242	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	8491	4.453	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046518.D
Acq On : 06 Jun 2025 09:42
Operator : JC/MD
Sample : VSTDICC005
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:40:47 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046518.D
 Acq On : 06 Jun 2025 09:42
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC005

Manual Integrations APPROVED

Reviewed By :John Carlone 06/06/2025
 Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:40:47 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

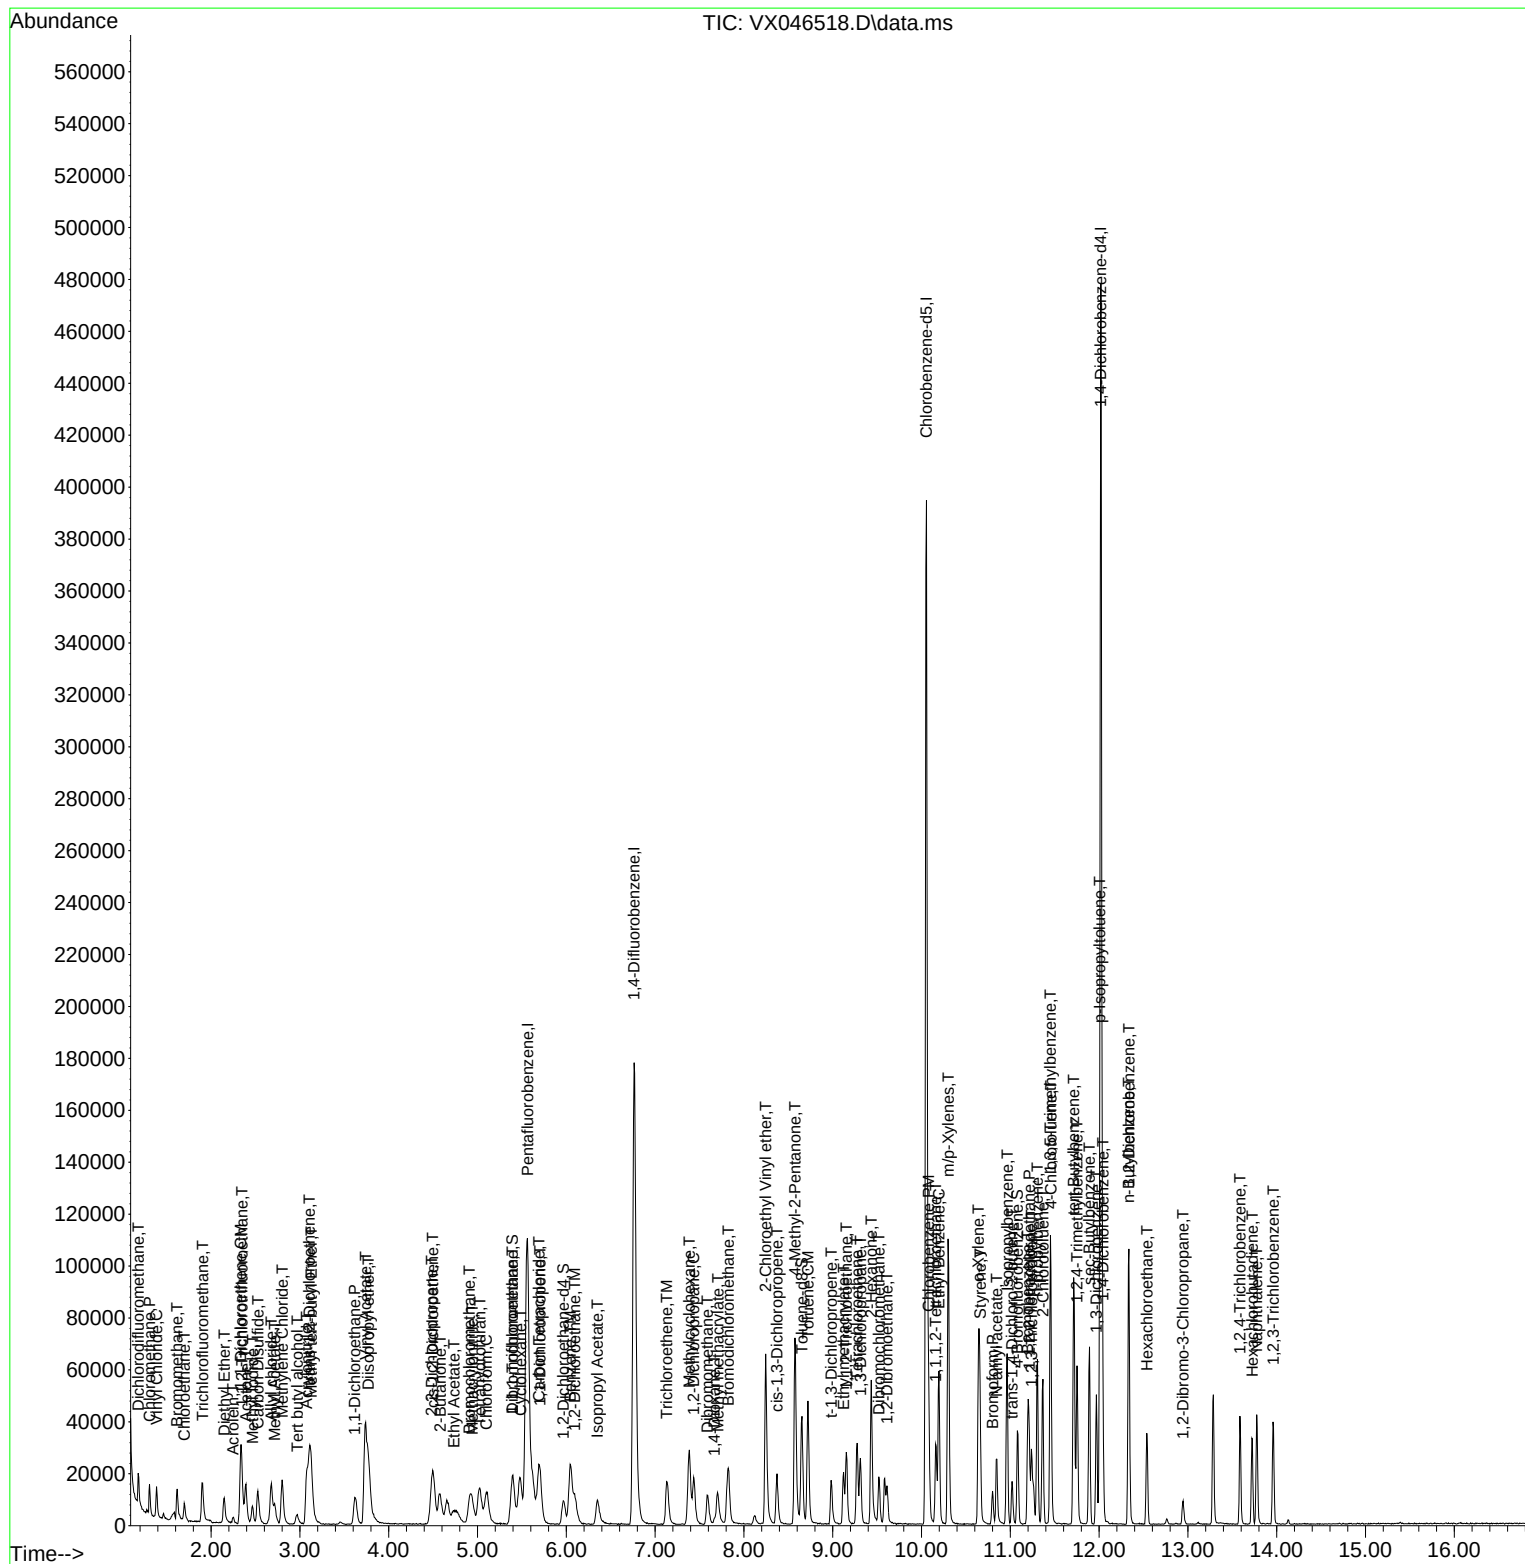

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046519.D
 Acq On : 06 Jun 2025 10:18
 Operator : JC/MD
 Sample : VSTDICC020
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC020

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	91899	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	155168	50.000	ug/l	-0.01
63) Chlorobenzene-d5	10.055	117	138173	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	69785	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	31177	19.069	ug/l	-0.01
Spiked Amount 50.000	Range 74 - 125		Recovery =	38.140%#		
35) Dibromofluoromethane	5.391	113	21913	19.203	ug/l	-0.01
Spiked Amount 50.000	Range 75 - 124		Recovery =	38.400%#		
50) Toluene-d8	8.647	98	71915	19.116	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	38.240%#		
62) 4-Bromofluorobenzene	11.079	95	29923	19.224	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	38.440%#		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.185	85	24011	18.820	ug/l	97
3) Chloromethane	1.307	50	21532	18.541	ug/l	97
4) Vinyl Chloride	1.386	62	21814	18.843	ug/l	99
5) Bromomethane	1.624	94	15765	22.432	ug/l	98
6) Chloroethane	1.703	64	14119	18.798	ug/l	97
7) Trichlorofluoromethane	1.904	101	38797	20.256	ug/l	95
8) Diethyl Ether	2.148	74	13057	19.294	ug/l	94
9) 1,1,2-Trichlorotrifluo...	2.343	101	23928	19.829	ug/l	98
10) Methyl Iodide	2.465	142	24399	18.652	ug/l	98
11) Tert butyl alcohol	2.965	59	16570	91.334	ug/l	98
12) 1,1-Dichloroethene	2.337	96	20232	18.543	ug/l	94
13) Acrolein	2.245	56	20307	111.446	ug/l	98
14) Allyl chloride	2.678	41	40999	19.133	ug/l	96
15) Acrylonitrile	3.075	53	67593	98.540	ug/l	99
16) Acetone	2.386	43	61298	98.314	ug/l	97
17) Carbon Disulfide	2.526	76	45190	19.630	ug/l	100
18) Methyl Acetate	2.715	43	39765	20.419	ug/l	100
19) Methyl tert-butyl Ether	3.123	73	75365	19.741	ug/l	99
20) Methylene Chloride	2.800	84	24863	18.955	ug/l	96
21) trans-1,2-Dichloroethene	3.105	96	21333	18.476	ug/l	93
22) Diisopropyl ether	3.770	45	86178	20.399	ug/l #	77
23) Vinyl Acetate	3.733	43	309124	94.776	ug/l	100
24) 1,1-Dichloroethane	3.623	63	46528	19.761	ug/l	99
25) 2-Butanone	4.562	43	86287	94.804	ug/l	99
26) 2,2-Dichloropropane	4.489	77	33782	19.327	ug/l	97
27) cis-1,2-Dichloroethene	4.501	96	27631	19.439	ug/l	97
28) Bromochloromethane	4.910	49	21754	19.371	ug/l	99
29) Tetrahydrofuran	5.013	42	53547	93.158	ug/l	100
30) Chloroform	5.105	83	49854	20.208	ug/l	92
31) Cyclohexane	5.483	56	37188	19.565	ug/l	90
32) 1,1,1-Trichloroethane	5.391	97	41583	19.705	ug/l	98
36) 1,1-Dichloropropene	5.702	75	31397	19.262	ug/l	99
37) Ethyl Acetate	4.733	43	32379	20.357	ug/l	98
38) Carbon Tetrachloride	5.684	117	35956	19.695	ug/l	98
39) Methylcyclohexane	7.379	83	35729	18.571	ug/l	96
40) Benzene	6.044	78	93317	20.336	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046519.D
 Acq On : 06 Jun 2025 10:18
 Operator : JC/MD
 Sample : VSTDIC020
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDIC020

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.928	41	20773	21.027	ug/l	96
42) 1,2-Dichloroethane	6.098	62	39768	20.832	ug/l	100
43) Isopropyl Acetate	6.342	43	55054	19.851	ug/l	99
44) Trichloroethene	7.129	130	22094	18.950	ug/l	97
45) 1,2-Dichloropropane	7.434	63	24588	20.760	ug/l	98
46) Dibromomethane	7.586	93	17753	19.924	ug/l	97
47) Bromodichloromethane	7.824	83	38325	20.919	ug/l	100
48) Methyl methacrylate	7.696	41	28189	19.755	ug/l	98
49) 1,4-Dioxane	7.665	88	8127	425.896	ug/l	99
51) 4-Methyl-2-Pentanone	8.574	43	180974	102.687	ug/l	99
52) Toluene	8.720	92	56537	20.055	ug/l	98
53) t-1,3-Dichloropropene	8.976	75	32552	19.817	ug/l	99
54) cis-1,3-Dichloropropene	8.372	75	36009	19.716	ug/l	89
55) 1,1,2-Trichloroethane	9.153	97	24130	21.322	ug/l	98
56) Ethyl methacrylate	9.116	69	35137	20.176	ug/l	97
57) 1,3-Dichloropropane	9.305	76	41306	20.653	ug/l	98
58) 2-Chloroethyl Vinyl ether	8.244	63	93580	98.650	ug/l	99
59) 2-Hexanone	9.427	43	128964	102.032	ug/l	99
60) Dibromochloromethane	9.519	129	27175	20.414	ug/l	99
61) 1,2-Dibromoethane	9.610	107	23582	19.996	ug/l	99
64) Tetrachloroethene	9.275	164	17890	19.362	ug/l	94
65) Chlorobenzene	10.079	112	63695	19.600	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.165	131	22188	20.205	ug/l	99
67) Ethyl Benzene	10.195	91	112127	19.765	ug/l	98
68) m/p-Xylenes	10.299	106	82876	40.272	ug/l	97
69) o-Xylene	10.640	106	40415	20.304	ug/l	99
70) Styrene	10.653	104	69469	20.388	ug/l	100
71) Bromoform	10.799	173	16593	19.817	ug/l #	97
73) Isopropylbenzene	10.963	105	110221	20.092	ug/l	100
74) N-amyl acetate	10.842	43	46707	19.334	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	36116	20.568	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	30039m	19.991	ug/l	
77) Bromobenzene	11.195	156	25827	20.283	ug/l	96
78) n-propylbenzene	11.305	91	133297	20.075	ug/l	100
79) 2-Chlorotoluene	11.360	91	80101	20.005	ug/l	98
80) 1,3,5-Trimethylbenzene	11.451	105	92024	20.131	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	9832	19.187	ug/l	99
82) 4-Chlorotoluene	11.451	91	93283	19.655	ug/l	98
83) tert-Butylbenzene	11.713	119	93897	20.178	ug/l	98
84) 1,2,4-Trimethylbenzene	11.750	105	93782	20.279	ug/l	98
85) sec-Butylbenzene	11.890	105	119909	20.054	ug/l	99
86) p-Isopropyltoluene	12.006	119	99196	19.900	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	47842	19.349	ug/l	99
88) 1,4-Dichlorobenzene	12.043	146	48453	18.912	ug/l	99
89) n-Butylbenzene	12.329	91	94297	19.263	ug/l	99
90) Hexachloroethane	12.536	117	16809	18.972	ug/l	97
91) 1,2-Dichlorobenzene	12.335	146	47259	19.801	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	7586	19.293	ug/l	98
93) 1,2,4-Trichlorobenzene	13.585	180	30280	18.598	ug/l	98
94) Hexachlorobutadiene	13.725	225	14184	18.746	ug/l	97
95) Naphthalene	13.774	128	98466	19.071	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	30099	18.437	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046519.D
Acq On : 06 Jun 2025 10:18
Operator : JC/MD
Sample : VSTDICC020
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046519.D
Acq On : 06 Jun 2025 10:18
Operator : JC/MD
Sample : VSTDICC020
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020

Manual Integrations APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration

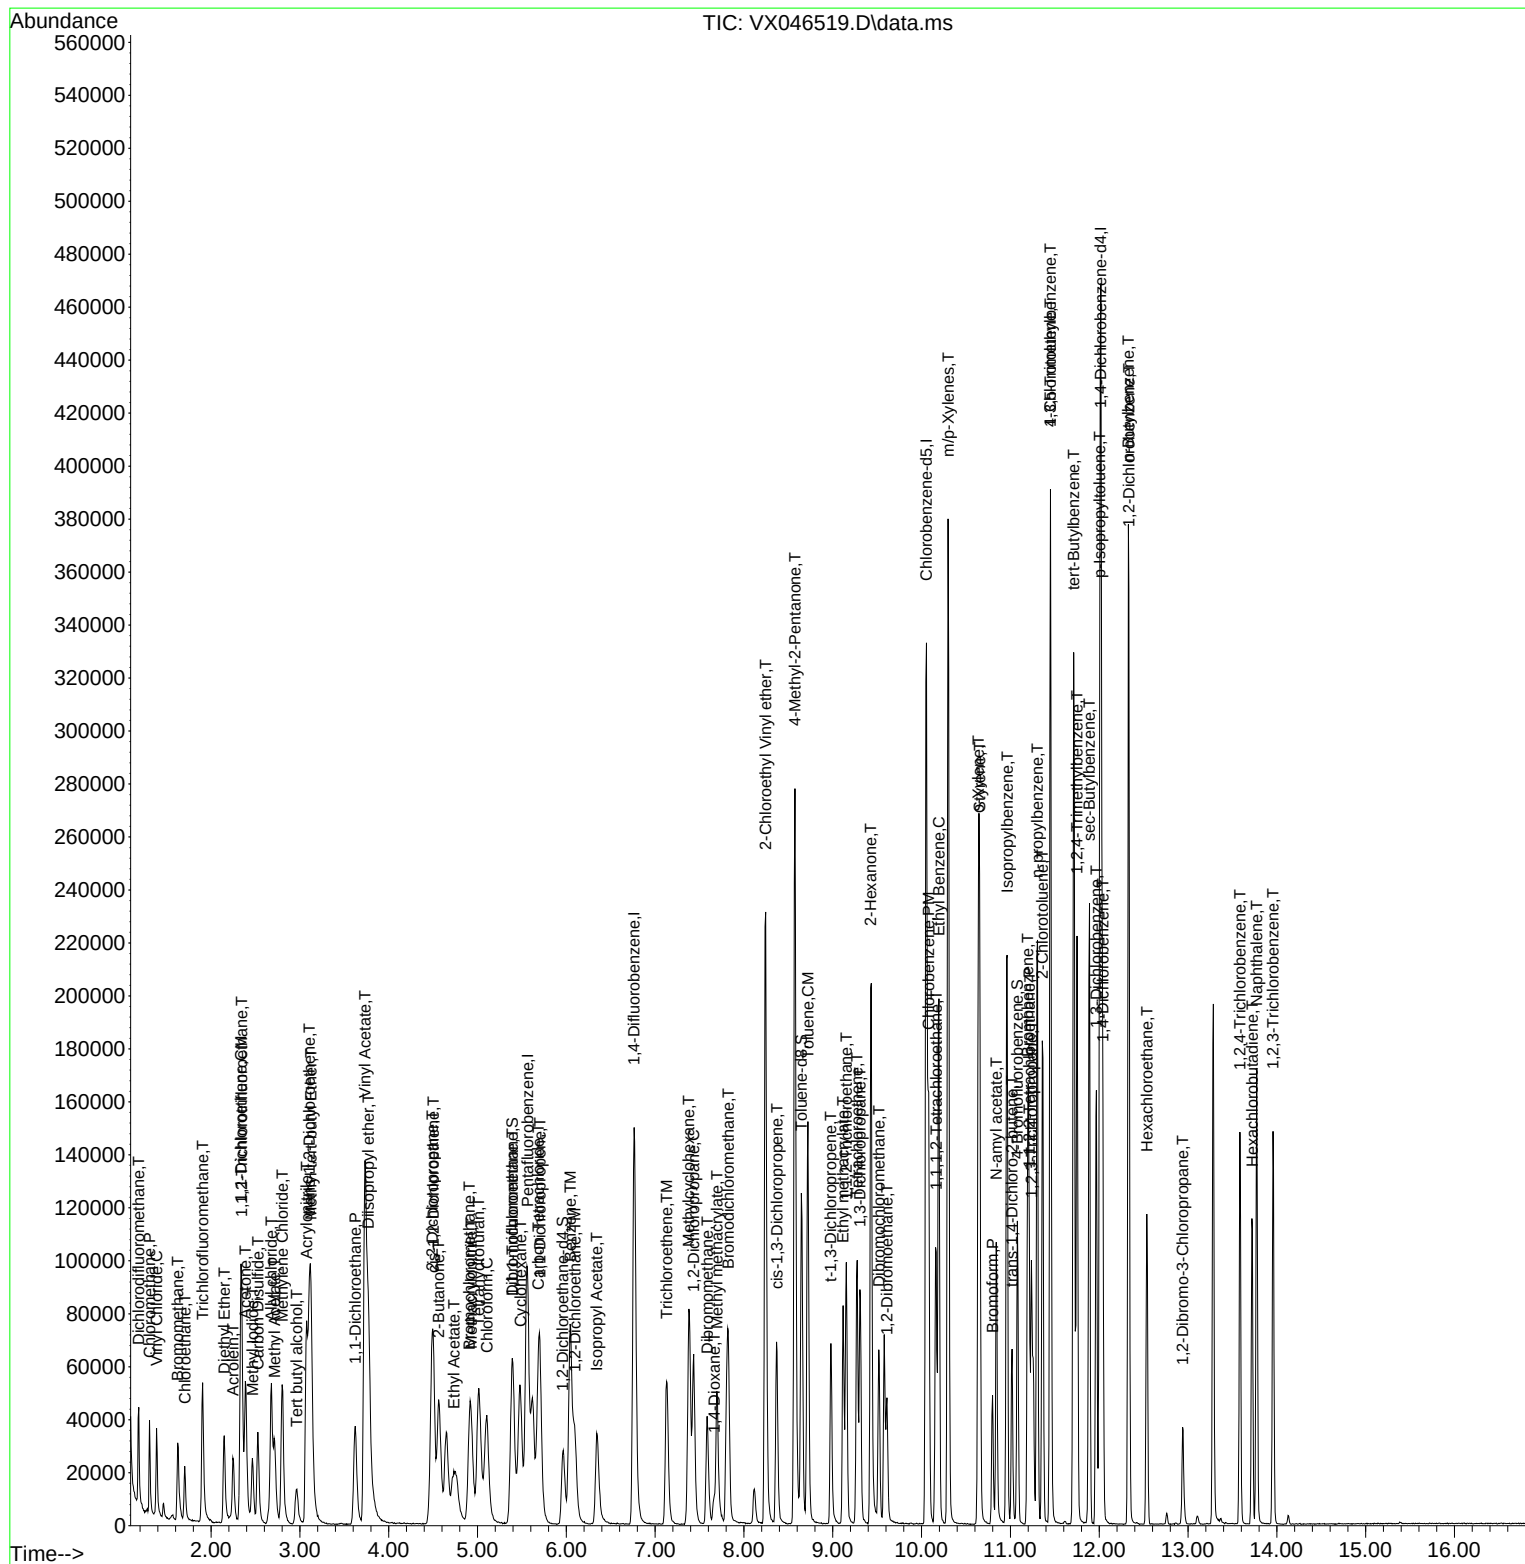

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046520.D
 Acq On : 06 Jun 2025 10:40
 Operator : JC/MD
 Sample : VSTDICCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICCC050

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	90114	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	156192	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	136564	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68831	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	78706	49.092	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	98.180%		
35) Dibromofluoromethane	5.403	113	57416	49.986	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.980%		
50) Toluene-d8	8.653	98	185557	49.000	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	98.000%		
62) 4-Bromofluorobenzene	11.079	95	76988	49.137	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	98.280%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.185	85	58145	46.477	ug/l	95
3) Chloromethane	1.307	50	51612	45.324	ug/l	96
4) Vinyl Chloride	1.386	62	53673	47.282	ug/l	100
5) Bromomethane	1.624	94	35883	52.070	ug/l	96
6) Chloroethane	1.703	64	33654	45.694	ug/l	96
7) Trichlorofluoromethane	1.904	101	92019	48.994	ug/l	95
8) Diethyl Ether	2.154	74	32101	48.374	ug/l	94
9) 1,1,2-Trichlorotrifluo...	2.349	101	57448	48.549	ug/l	98
10) Methyl Iodide	2.471	142	64524	50.302	ug/l	100
11) Tert butyl alcohol	2.971	59	44039	247.552	ug/l	100
12) 1,1-Dichloroethene	2.337	96	51110	47.772	ug/l	99
13) Acrolein	2.251	56	50652	237.168	ug/l	98
14) Allyl chloride	2.684	41	101836	48.466	ug/l	96
15) Acrylonitrile	3.081	53	170615	253.656	ug/l	99
16) Acetone	2.392	43	153142	243.373	ug/l	100
17) Carbon Disulfide	2.532	76	109794	48.339	ug/l	100
18) Methyl Acetate	2.721	43	101867	53.343	ug/l	100
19) Methyl tert-butyl Ether	3.135	73	190602	50.914	ug/l	99
20) Methylene Chloride	2.806	84	59622	46.355	ug/l	94
21) trans-1,2-Dichloroethene	3.111	96	52474	46.346	ug/l	95
22) Diisopropyl ether	3.782	45	211118	50.963	ug/l #	80
23) Vinyl Acetate	3.739	43	823688	257.541	ug/l	100
24) 1,1-Dichloroethane	3.629	63	113435	49.132	ug/l	97
25) 2-Butanone	4.574	43	226668	253.975	ug/l	98
26) 2,2-Dichloropropane	4.495	77	87040	50.783	ug/l	100
27) cis-1,2-Dichloroethene	4.507	96	66760	47.898	ug/l	99
28) Bromochloromethane	4.916	49	53158	48.273	ug/l	100
29) Tetrahydrofuran	5.019	42	142276	252.427	ug/l	99
30) Chloroform	5.111	83	118738	49.084	ug/l	99
31) Cyclohexane	5.489	56	89669	48.110	ug/l	99
32) 1,1,1-Trichloroethane	5.397	97	102837	49.696	ug/l	98
36) 1,1-Dichloropropene	5.714	75	75745	46.165	ug/l	99
37) Ethyl Acetate	4.733	43	86522	54.042	ug/l	98
38) Carbon Tetrachloride	5.696	117	88063	47.920	ug/l	99
39) Methylcyclohexane	7.391	83	89357	46.141	ug/l	97
40) Benzene	6.056	78	222898	48.257	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046520.D
 Acq On : 06 Jun 2025 10:40
 Operator : JC/MD
 Sample : VSTDICCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICCC050

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.934	41	50437	50.720	ug/l	96
42) 1,2-Dichloroethane	6.098	62	95292	49.590	ug/l	99
43) Isopropyl Acetate	6.354	43	144198	51.653	ug/l	99
44) Trichloroethene	7.135	130	54791	46.686	ug/l	98
45) 1,2-Dichloropropane	7.440	63	59497	49.904	ug/l	99
46) Dibromomethane	7.586	93	43598	48.609	ug/l	98
47) Bromodichloromethane	7.830	83	94149	51.052	ug/l	98
48) Methyl methacrylate	7.702	41	75100	52.285	ug/l	97
49) 1,4-Dioxane	7.671	88	19805	1031.079	ug/l	98
51) 4-Methyl-2-Pentanone	8.573	43	462924	260.948	ug/l	100
52) Toluene	8.720	92	138129	48.677	ug/l	99
53) t-1,3-Dichloropropene	8.982	75	84697	51.223	ug/l	100
54) cis-1,3-Dichloropropene	8.372	75	92087	50.089	ug/l	91
55) 1,1,2-Trichloroethane	9.153	97	57143	50.162	ug/l	97
56) Ethyl methacrylate	9.116	69	91058	51.943	ug/l	97
57) 1,3-Dichloropropane	9.311	76	99273	49.312	ug/l	98
58) 2-Chloroethyl Vinyl ether	8.244	63	246532	258.184	ug/l	100
59) 2-Hexanone	9.433	43	333019	261.746	ug/l	99
60) Dibromochloromethane	9.525	129	67410	50.307	ug/l	99
61) 1,2-Dibromoethane	9.610	107	57774	48.669	ug/l	98
64) Tetrachloroethene	9.275	164	42288	46.308	ug/l	96
65) Chlorobenzene	10.079	112	153710	47.857	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.165	131	54990	50.666	ug/l	99
67) Ethyl Benzene	10.195	91	275626	49.157	ug/l	100
68) m/p-Xylenes	10.299	106	201325	98.982	ug/l	99
69) o-Xylene	10.640	106	97769	49.696	ug/l	97
70) Styrene	10.658	104	171642	50.968	ug/l	99
71) Bromoform	10.799	173	42521	51.382	ug/l #	98
73) Isopropylbenzene	10.963	105	269074	49.729	ug/l	99
74) N-amyl acetate	10.841	43	124077	52.072	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	86539	49.967	ug/l	98
76) 1,2,3-Trichloropropane	11.238	75	72182m	48.702	ug/l	
77) Bromobenzene	11.195	156	60653	48.295	ug/l	100
78) n-propylbenzene	11.305	91	323032	49.325	ug/l	100
79) 2-Chlorotoluene	11.366	91	191732	48.549	ug/l	100
80) 1,3,5-Trimethylbenzene	11.451	105	223189	49.500	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	25456	50.367	ug/l	98
82) 4-Chlorotoluene	11.451	91	226629	48.414	ug/l	99
83) tert-Butylbenzene	11.713	119	226214	49.285	ug/l	98
84) 1,2,4-Trimethylbenzene	11.750	105	224100	49.131	ug/l	100
85) sec-Butylbenzene	11.890	105	287196	48.696	ug/l	99
86) p-Isopropyltoluene	12.006	119	239809	48.775	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	115889	47.520	ug/l	99
88) 1,4-Dichlorobenzene	12.042	146	115263	45.612	ug/l	99
89) n-Butylbenzene	12.329	91	230830	47.808	ug/l	99
90) Hexachloroethane	12.536	117	41969	48.027	ug/l	98
91) 1,2-Dichlorobenzene	12.335	146	112815	47.923	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	19603	50.545	ug/l	94
93) 1,2,4-Trichlorobenzene	13.585	180	74109	46.149	ug/l	99
94) Hexachlorobutadiene	13.725	225	34506	46.237	ug/l	98
95) Naphthalene	13.774	128	256456	50.359	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	75172	46.684	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046520.D
Acq On : 06 Jun 2025 10:40
Operator : JC/MD
Sample : VSTDICCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050

Manual Integrations

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

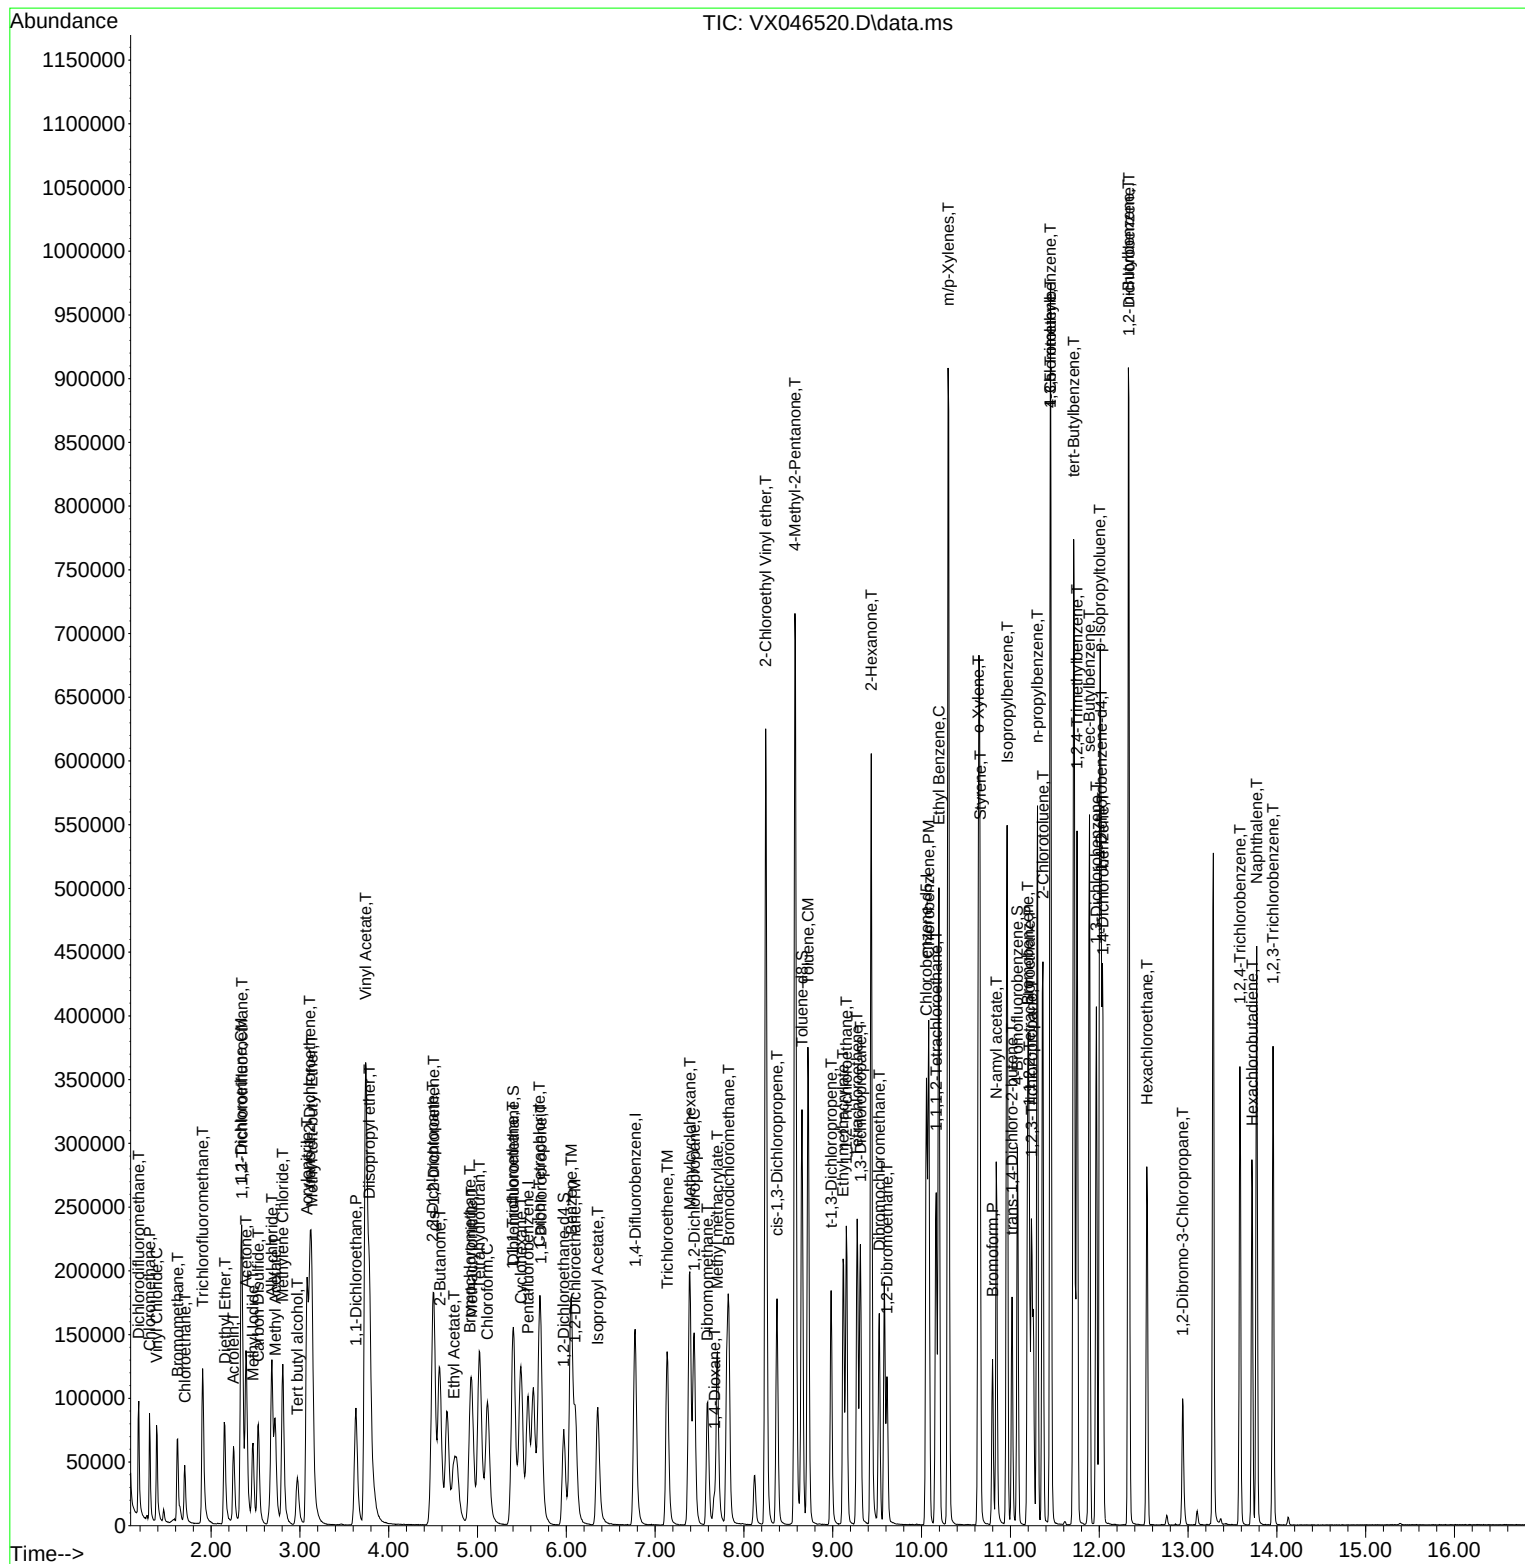

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046521.D
 Acq On : 06 Jun 2025 11:02
 Operator : JC/MD
 Sample : VSTDICC100
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC100

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	86761	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	151628	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	131925	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	65495	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	143754	93.131	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 186.260%#			
35) Dibromofluoromethane	5.403	113	105237	94.377	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 188.760%#			
50) Toluene-d8	8.653	98	343367	93.402	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 186.800%#			
62) 4-Bromofluorobenzene	11.079	95	141905	93.296	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 186.600%#			
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.185	85	110112	91.417	ug/l	98
3) Chloromethane	1.307	50	98615	89.947	ug/l	99
4) Vinyl Chloride	1.386	62	102609	93.885	ug/l	98
5) Bromomethane	1.617	94	44380	66.888	ug/l	98
6) Chloroethane	1.697	64	61909	87.305	ug/l	99
7) Trichlorofluoromethane	1.904	101	171395	94.783	ug/l	98
8) Diethyl Ether	2.154	74	60580	94.817	ug/l	97
9) 1,1,2-Trichlorotrifluo...	2.349	101	106901	93.832	ug/l	97
10) Methyl Iodide	2.471	142	129059	104.501	ug/l	100
11) Tert butyl alcohol	2.977	59	90368	527.609	ug/l	99
12) 1,1-Dichloroethene	2.337	96	97296	94.457	ug/l	95
13) Acrolein	2.252	56	101278	460.232	ug/l	100
14) Allyl chloride	2.684	41	197384	97.570	ug/l	94
15) Acrylonitrile	3.081	53	330844	510.880	ug/l	100
16) Acetone	2.398	43	295803	483.635	ug/l	99
17) Carbon Disulfide	2.532	76	211673	96.592	ug/l	98
18) Methyl Acetate	2.721	43	200390	108.991	ug/l	99
19) Methyl tert-butyl Ether	3.129	73	369725	102.579	ug/l	99
20) Methylene Chloride	2.806	84	112036	90.472	ug/l	94
21) trans-1,2-Dichloroethene	3.111	96	98333	90.207	ug/l	97
22) Diisopropyl ether	3.782	45	402386	100.889	ug/l #	81
23) Vinyl Acetate	3.739	43	1588475	515.860	ug/l	100
24) 1,1-Dichloroethane	3.629	63	214175	96.351	ug/l	98
25) 2-Butanone	4.574	43	443718	516.388	ug/l	100
26) 2,2-Dichloropropane	4.501	77	168003	101.809	ug/l	99
27) cis-1,2-Dichloroethene	4.507	96	126373	94.172	ug/l	99
28) Bromochloromethane	4.916	49	103145	97.287	ug/l	100
29) Tetrahydrofuran	5.019	42	277926	512.155	ug/l	98
30) Chloroform	5.117	83	223890	96.128	ug/l	96
31) Cyclohexane	5.489	56	168997	94.175	ug/l	96
32) 1,1,1-Trichloroethane	5.397	97	195664	98.210	ug/l	98
36) 1,1-Dichloropropene	5.708	75	139920	87.846	ug/l	99
37) Ethyl Acetate	4.733	43	171559	110.381	ug/l	98
38) Carbon Tetrachloride	5.696	117	168024	94.183	ug/l	100
39) Methylcyclohexane	7.391	83	171321	91.127	ug/l	98
40) Benzene	6.056	78	418566	93.347	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046521.D
 Acq On : 06 Jun 2025 11:02
 Operator : JC/MD
 Sample : VSTDICC100
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC100

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.940	41	96904	100.381	ug/l	96
42) 1,2-Dichloroethane	6.098	62	177798	95.311	ug/l	99
43) Isopropyl Acetate	6.354	43	283615	104.651	ug/l	100
44) Trichloroethene	7.135	130	100714	88.399	ug/l	97
45) 1,2-Dichloropropane	7.440	63	112349	97.071	ug/l	97
46) Dibromomethane	7.586	93	82614	94.883	ug/l	98
47) Bromodichloromethane	7.830	83	178755	99.847	ug/l	99
48) Methyl methacrylate	7.702	41	148448	106.461	ug/l	97
49) 1,4-Dioxane	7.671	88	39522	2119.509	ug/l	99
51) 4-Methyl-2-Pentanone	8.580	43	882926	512.682	ug/l	100
52) Toluene	8.720	92	257539	93.489	ug/l	99
53) t-1,3-Dichloropropene	8.982	75	169431	105.552	ug/l	100
54) cis-1,3-Dichloropropene	8.372	75	180299	101.023	ug/l	93
55) 1,1,2-Trichloroethane	9.153	97	107827	97.502	ug/l	99
56) Ethyl methacrylate	9.122	69	180282	105.935	ug/l	97
57) 1,3-Dichloropropane	9.311	76	185642	94.990	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.250	63	472343	509.557	ug/l	100
59) 2-Hexanone	9.433	43	635829	514.792	ug/l	99
60) Dibromochloromethane	9.525	129	128006	98.404	ug/l	100
61) 1,2-Dibromoethane	9.610	107	110603	95.976	ug/l	98
64) Tetrachloroethene	9.275	164	79545	90.169	ug/l	97
65) Chlorobenzene	10.079	112	289084	93.171	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.165	131	106634	101.705	ug/l	99
67) Ethyl Benzene	10.195	91	520064	96.013	ug/l	99
68) m/p-Xylenes	10.305	106	376918	191.829	ug/l	100
69) o-Xylene	10.640	106	185444	97.576	ug/l	100
70) Styrene	10.659	104	319998	98.362	ug/l	99
71) Bromoform	10.799	173	83574	104.541	ug/l #	97
73) Isopropylbenzene	10.963	105	501468	97.400	ug/l	100
74) N-amyl acetate	10.841	43	242879	107.123	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	163624	99.288	ug/l	100
76) 1,2,3-Trichloropropane	11.238	75	134330m	95.251	ug/l	
77) Bromobenzene	11.201	156	115005	96.236	ug/l	98
78) n-propylbenzene	11.305	91	596385	95.703	ug/l	99
79) 2-Chlorotoluene	11.366	91	356389	94.839	ug/l	99
80) 1,3,5-Trimethylbenzene	11.451	105	412251	96.089	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	52102	108.338	ug/l	94
82) 4-Chlorotoluene	11.457	91	416150	93.429	ug/l	98
83) tert-Butylbenzene	11.713	119	425478	97.420	ug/l	98
84) 1,2,4-Trimethylbenzene	11.750	105	418383	96.397	ug/l	100
85) sec-Butylbenzene	11.890	105	536486	95.599	ug/l	100
86) p-Isopropyltoluene	12.006	119	445024	95.124	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	215104	92.695	ug/l	100
88) 1,4-Dichlorobenzene	12.042	146	213122	88.632	ug/l	99
89) n-Butylbenzene	12.329	91	433603	94.378	ug/l	99
90) Hexachloroethane	12.536	117	82886	99.681	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	208931	93.273	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	40499	109.744	ug/l	98
93) 1,2,4-Trichlorobenzene	13.585	180	143150	93.683	ug/l	99
94) Hexachlorobutadiene	13.725	225	65134	91.723	ug/l	99
95) Naphthalene	13.774	128	499805	103.144	ug/l	99
96) 1,2,3-Trichlorobenzene	13.957	180	145123	94.716	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046521.D
Acq On : 06 Jun 2025 11:02
Operator : JC/MD
Sample : VSTDICC100
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046521.D
 Acq On : 06 Jun 2025 11:02
 Operator : JC/MD
 Sample : VSTDICC100
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC100

Manual Integrations APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:41:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

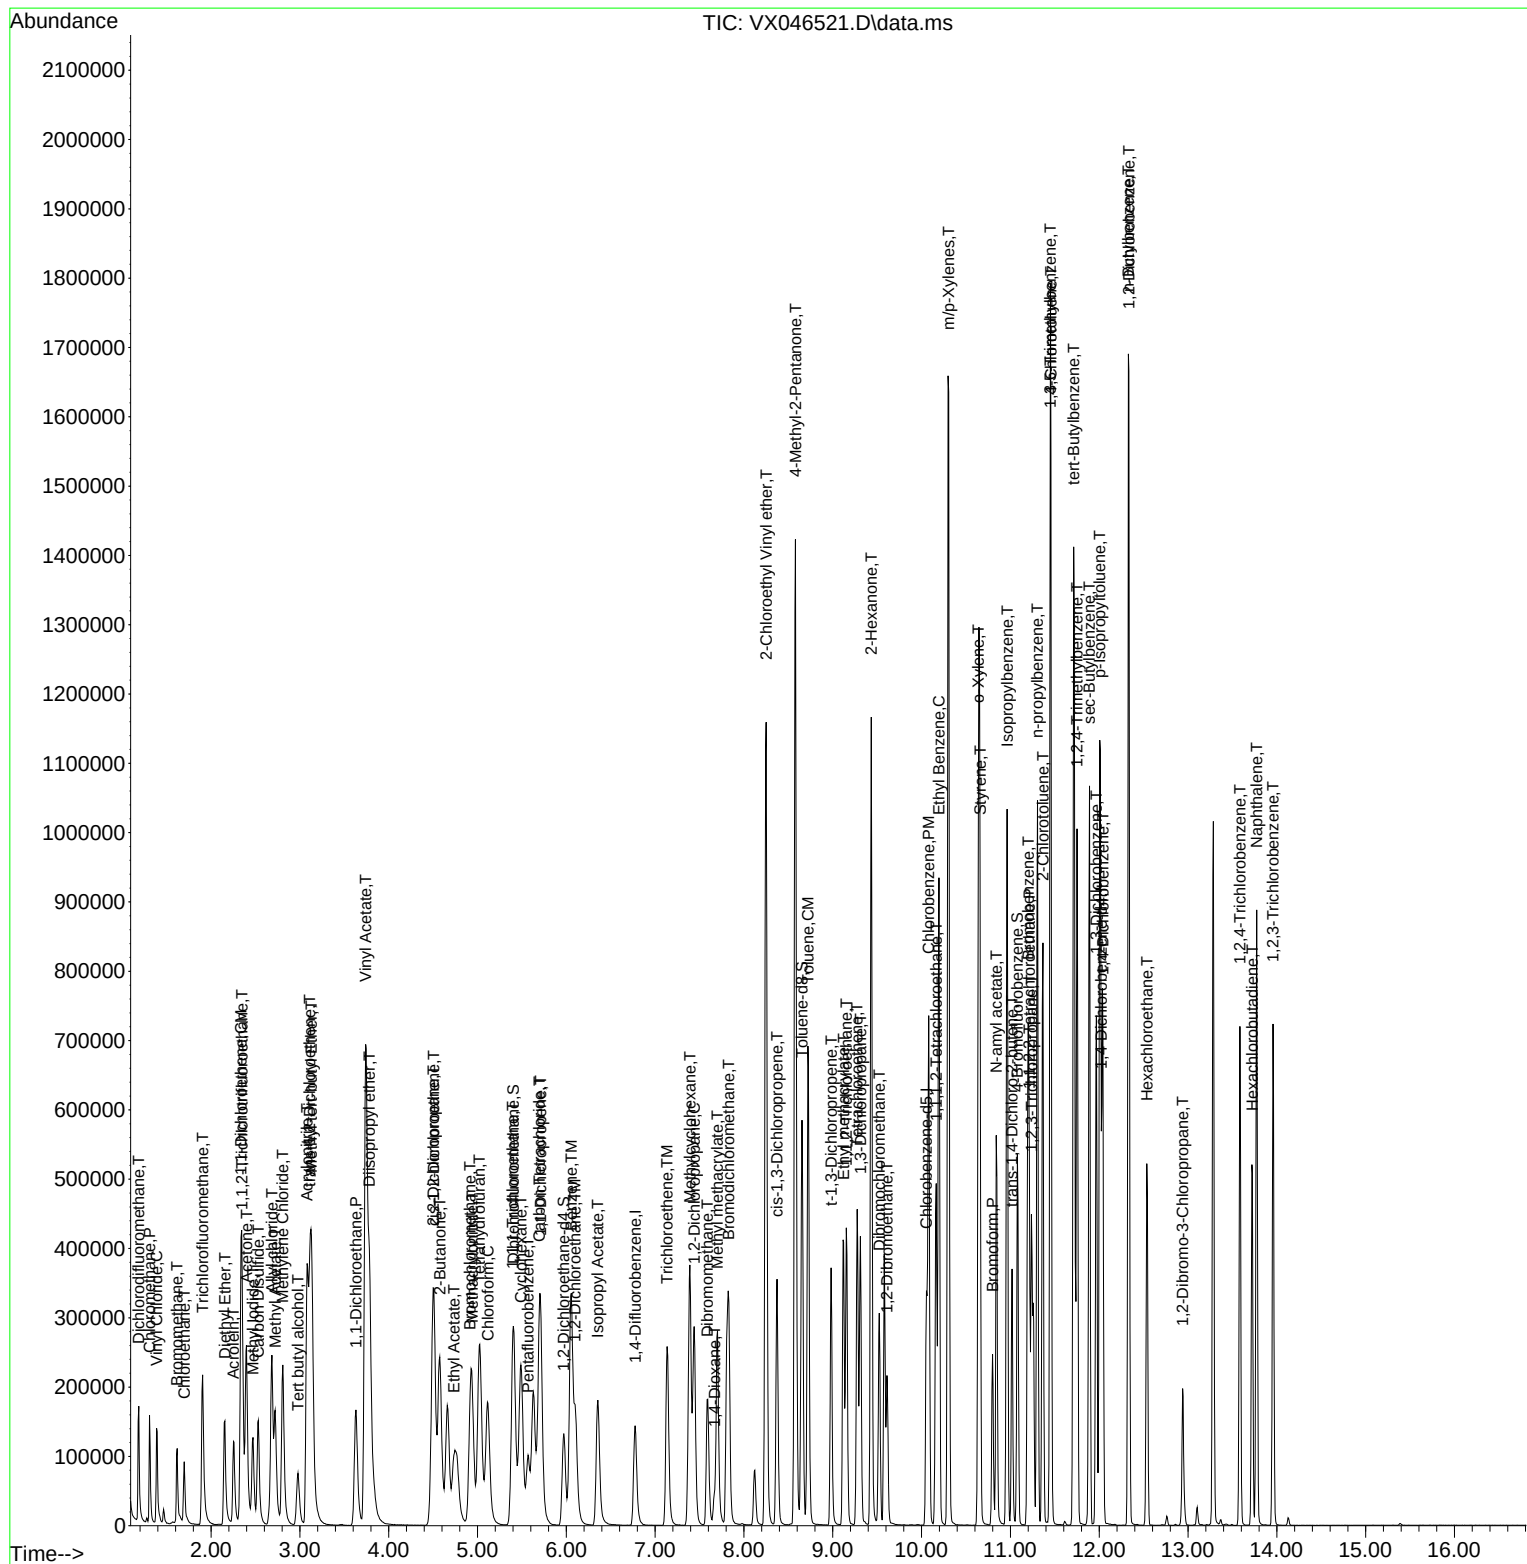

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046522.D
 Acq On : 06 Jun 2025 11:25
 Operator : JC/MD
 Sample : VSTDICC150
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC150

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:42:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	78828	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	138158	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	121245	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	58605	50.000	ug/l	# 0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.971	65	212938	151.835	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 303.660%#			
35) Dibromofluoromethane	5.404	113	156990	154.516	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 309.040%#			
50) Toluene-d8	8.653	98	505724	150.978	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 301.960%#			
62) 4-Bromofluorobenzene	11.079	95	207701	149.867	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 299.740%#			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.179	85	154709	141.368	ug/l	97
3) Chloromethane	1.307	50	145250	145.815	ug/l	98
4) Vinyl Chloride	1.386	62	147097	148.135	ug/l	98
5) Bromomethane	1.612	94	56077	93.023	ug/l	97
6) Chloroethane	1.691	64	88121	136.776	ug/l	98
7) Trichlorofluoromethane	1.898	101	244494	148.815	ug/l	98
8) Diethyl Ether	2.148	74	87079	150.009	ug/l	91
9) 1,1,2-Trichlorotrifluo...	2.343	101	151059	145.936	ug/l	98
10) Methyl Iodide	2.465	142	185045	164.913	ug/l	99
11) Tert butyl alcohol	2.983	59	134861	866.618	ug/l	100
12) 1,1-Dichloroethene	2.331	96	138358	147.838	ug/l	99
13) Acrolein	2.252	56	160165	778.853	ug/l	100
14) Allyl chloride	2.678	41	267359	145.460	ug/l	93
15) Acrylonitrile	3.081	53	476614	810.040	ug/l	99
16) Acetone	2.398	43	425579	763.161	ug/l	98
17) Carbon Disulfide	2.526	76	304498	152.815	ug/l	99
18) Methyl Acetate	2.721	43	292598	175.157	ug/l	98
19) Methyl tert-butyl Ether	3.130	73	533557	162.931	ug/l	99
20) Methylene Chloride	2.806	84	160400	142.563	ug/l	94
21) trans-1,2-Dichloroethene	3.111	96	140409	141.768	ug/l	98
22) Diisopropyl ether	3.782	45	574529	158.547	ug/l	# 84
23) Vinyl Acetate	3.739	43	2294131	820.000	ug/l	100
24) 1,1-Dichloroethane	3.629	63	306779	151.900	ug/l	99
25) 2-Butanone	4.574	43	643633	824.425	ug/l	99
26) 2,2-Dichloropropane	4.495	77	241718	161.222	ug/l	100
27) cis-1,2-Dichloroethene	4.507	96	181365	148.753	ug/l	98
28) Bromochloromethane	4.916	49	139177	144.483	ug/l	99
29) Tetrahydrofuran	5.019	42	404249	819.909	ug/l	99
30) Chloroform	5.111	83	319000	150.747	ug/l	96
31) Cyclohexane	5.489	56	240734	147.652	ug/l	98
32) 1,1,1-Trichloroethane	5.404	97	280921	155.193	ug/l	97
36) 1,1-Dichloropropene	5.708	75	201157	138.605	ug/l	99
37) Ethyl Acetate	4.733	43	247037	174.441	ug/l	100
38) Carbon Tetrachloride	5.696	117	240128	147.722	ug/l	100
39) Methylcyclohexane	7.391	83	243263	142.009	ug/l	96
40) Benzene	6.056	78	597704	146.294	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046522.D
 Acq On : 06 Jun 2025 11:25
 Operator : JC/MD
 Sample : VSTDICC150
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC150

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:42:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.934	41	142496	162.001	ug/l	97
42) 1,2-Dichloroethane	6.105	62	249510	146.794	ug/l	98
43) Isopropyl Acetate	6.355	43	415327	168.193	ug/l	99
44) Trichloroethene	7.135	130	146894	141.503	ug/l	98
45) 1,2-Dichloropropane	7.440	63	161815	153.441	ug/l	96
46) Dibromomethane	7.586	93	118718	149.642	ug/l	98
47) Bromodichloromethane	7.830	83	256187	157.050	ug/l	99
48) Methyl methacrylate	7.702	41	214089	168.505	ug/l	97
49) 1,4-Dioxane	7.671	88	57504	3384.526	ug/l	97
51) 4-Methyl-2-Pentanone	8.580	43	1262813	804.759	ug/l	99
52) Toluene	8.720	92	368137	146.666	ug/l	99
53) t-1,3-Dichloropropene	8.982	75	249298	170.450	ug/l	99
54) cis-1,3-Dichloropropene	8.373	75	262248	161.266	ug/l	93
55) 1,1,2-Trichloroethane	9.153	97	154220	153.049	ug/l	98
56) Ethyl methacrylate	9.122	69	261827	168.851	ug/l	97
57) 1,3-Dichloropropane	9.311	76	263879	148.186	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.251	63	676448	800.891	ug/l	100
59) 2-Hexanone	9.433	43	908142	806.953	ug/l	98
60) Dibromochloromethane	9.525	129	185185	156.239	ug/l	99
61) 1,2-Dibromoethane	9.610	107	156873	149.399	ug/l	97
64) Tetrachloroethene	9.275	164	114275	140.948	ug/l	96
65) Chlorobenzene	10.080	112	414361	145.311	ug/l	100
66) 1,1,1,2-Tetrachloroethane	10.165	131	152702	158.472	ug/l	99
67) Ethyl Benzene	10.195	91	742300	149.114	ug/l	100
68) m/p-Xylenes	10.305	106	537140	297.452	ug/l	99
69) o-Xylene	10.640	106	263508	150.865	ug/l	99
70) Styrene	10.653	104	457350	152.965	ug/l	99
71) Bromoform	10.799	173	121843	165.836	ug/l #	97
73) Isopropylbenzene	10.964	105	714594	155.114	ug/l	100
74) N-amyl acetate	10.842	43	354967	174.965	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	229605	155.706	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	191913m	152.081	ug/l	
77) Bromobenzene	11.195	156	163113	152.540	ug/l	99
78) n-propylbenzene	11.305	91	846247	151.764	ug/l	99
79) 2-Chlorotoluene	11.366	91	503830	149.837	ug/l	100
80) 1,3,5-Trimethylbenzene	11.451	105	582683	151.781	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	77638	180.416	ug/l	91
82) 4-Chlorotoluene	11.451	91	585232	146.836	ug/l	98
83) tert-Butylbenzene	11.713	119	612111	156.630	ug/l	96
84) 1,2,4-Trimethylbenzene	11.750	105	590035	151.929	ug/l	100
85) sec-Butylbenzene	11.890	105	761909	151.730	ug/l	100
86) p-Isopropyltoluene	12.006	119	628539	150.146	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	305990	147.362	ug/l	99
88) 1,4-Dichlorobenzene	12.043	146	308002	143.149	ug/l	99
89) n-Butylbenzene	12.329	91	613010	149.115	ug/l	99
90) Hexachloroethane	12.536	117	120040	161.336	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	298047	148.701	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	59166	179.177	ug/l	97
93) 1,2,4-Trichlorobenzene	13.585	180	209982	153.577	ug/l	99
94) Hexachlorobutadiene	13.725	225	92311	145.277	ug/l	98
95) Naphthalene	13.774	128	739300	170.506	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	210596	153.606	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046522.D
Acq On : 06 Jun 2025 11:25
Operator : JC/MD
Sample : VSTDICC150
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:42:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046522.D
Acq On : 06 Jun 2025 11:25
Operator : JC/MD
Sample : VSTDICC150
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

Manual Integrations

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:42:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration

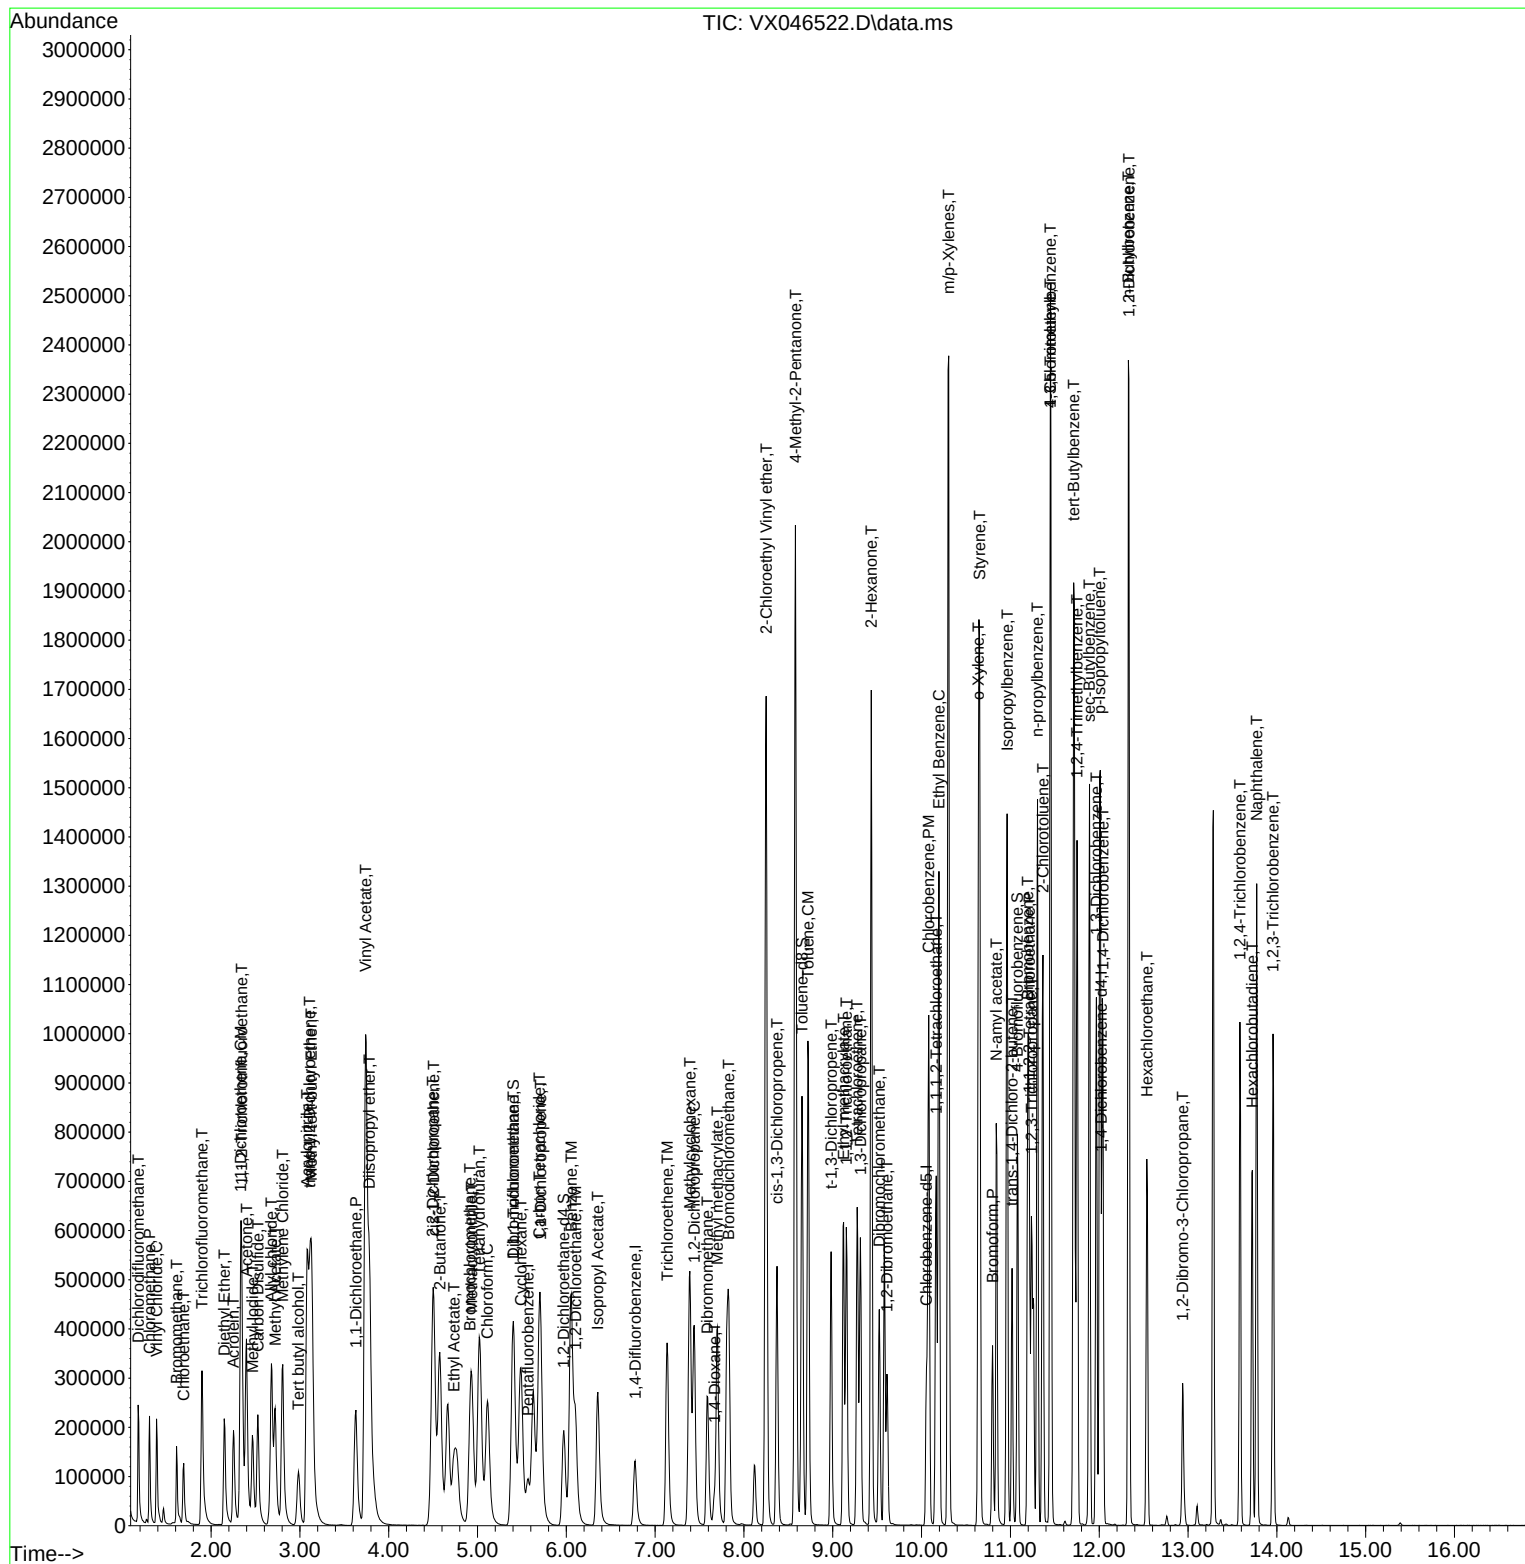

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046524.D
 Acq On : 06 Jun 2025 12:57
 Operator : JC/MD
 Sample : VSTDICC001
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/09/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:43:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	92377	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.763	114	161412	50.000	ug/l	-0.01
63) Chlorobenzene-d5	10.055	117	144029	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	72344	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	0.000	65	0d	0.000	ug/l	
Spiked Amount	50.000	Range	74 - 125	Recovery	=	0.000%#
35) Dibromofluoromethane	0.000	113	0d	0.000	ug/l	
Spiked Amount	50.000	Range	75 - 124	Recovery	=	0.000%#
50) Toluene-d8	0.000	98	0d	0.000	ug/l	
Spiked Amount	50.000	Range	86 - 113	Recovery	=	0.000%#
62) 4-Bromofluorobenzene	0.000	95	0d	0.000	ug/l	
Spiked Amount	50.000	Range	77 - 121	Recovery	=	0.000%#

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.184	85	1548	1.207	ug/l	89
3) Chloromethane	1.306	50	1317	1.128	ug/l	95
4) Vinyl Chloride	1.386	62	1255	1.078	ug/l #	83
6) Chloroethane	1.697	64	940	1.245	ug/l #	76
7) Trichlorofluoromethane	1.904	101	1882	0.977	ug/l	95
8) Diethyl Ether	2.136	74	762	1.120	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.349	101	1288	1.062	ug/l	95
12) 1,1-Dichloroethene	2.337	96	1174	1.070	ug/l	78
14) Allyl chloride	2.678	41	2371	1.101	ug/l	94
15) Acrylonitrile	3.080	53	3158	4.580	ug/l	90
16) Acetone	2.392	43	5228	12.546	ug/l	99
17) Carbon Disulfide	2.526	76	4273	2.030	ug/l	100
18) Methyl Acetate	2.721	43	1631	0.833	ug/l #	90
19) Methyl tert-butyl Ether	3.123	73	3460	0.902	ug/l	92
20) Methylene Chloride	2.806	84	1604	1.217	ug/l	93
21) trans-1,2-Dichloroethene	3.105	96	1451	1.250	ug/l	94
22) Diisopropyl ether	3.763	45	3727	0.878	ug/l #	1
23) Vinyl Acetate	3.739	43	15142	4.618	ug/l #	93
24) 1,1-Dichloroethane	3.617	63	2366	1.000	ug/l #	89
25) 2-Butanone	4.598	43	4468	4.884	ug/l #	87
26) 2,2-Dichloropropane	4.483	77	1663	0.947	ug/l	86
27) cis-1,2-Dichloroethene	4.507	96	1600	1.120	ug/l	94
28) Bromochloromethane	4.928	49	1200	1.063	ug/l #	89
29) Tetrahydrofuran	5.037	42	2828	4.895	ug/l	89
30) Chloroform	5.098	83	2492	1.005	ug/l	98
32) 1,1,1-Trichloroethane	5.391	97	2090	0.985	ug/l #	53
36) 1,1-Dichloropropene	5.702	75	2130	1.256	ug/l #	70
37) Ethyl Acetate	4.739	43	1146m	0.693	ug/l	
38) Carbon Tetrachloride	5.696	117	2113	1.113	ug/l #	65
39) Methylcyclohexane	7.391	83	2339	1.169	ug/l #	72
40) Benzene	6.043	78	4913	1.029	ug/l	99
41) Methacrylonitrile	4.952	41	901	0.877	ug/l #	43
42) 1,2-Dichloroethane	6.104	62	1955	0.984	ug/l	82
43) Isopropyl Acetate	6.348	43	2493	0.864	ug/l #	92
44) Trichloroethene	7.141	130	1537	1.267	ug/l	91
45) 1,2-Dichloropropane	7.433	63	1158	0.940	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046524.D
 Acq On : 06 Jun 2025 12:57
 Operator : JC/MD
 Sample : VSTDICC001
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/09/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:43:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:38:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) Dibromomethane	7.592	93	938	1.012	ug/l	92
47) Bromodichloromethane	7.830	83	1724	0.905	ug/l #	91
48) Methyl methacrylate	7.714	41	1276	0.860	ug/l	94
49) 1,4-Dioxane	7.677	88	286	14.408	ug/l #	79
51) 4-Methyl-2-Pentanone	8.573	43	7935	4.328	ug/l	98
52) Toluene	8.720	92	3027	1.032	ug/l	94
53) t-1,3-Dichloropropene	8.988	75	1550	0.907	ug/l	94
54) cis-1,3-Dichloropropene	8.378	75	1831	0.964	ug/l	91
55) 1,1,2-Trichloroethane	9.159	97	1069	0.908	ug/l #	82
56) Ethyl methacrylate	9.122	69	1471	0.812	ug/l	94
57) 1,3-Dichloropropane	9.317	76	2109	1.014	ug/l	95
58) 2-Chloroethyl Vinyl ether	8.250	63	4480	4.540	ug/l	97
59) 2-Hexanone	9.439	43	5937	4.515	ug/l	91
60) Dibromochloromethane	9.524	129	1307	0.944	ug/l	89
61) 1,2-Dibromoethane	9.616	107	1355	1.105	ug/l	89
64) Tetrachloroethene	9.274	164	1182	1.227	ug/l	90
65) Chlorobenzene	10.079	112	3905	1.153	ug/l	97
66) 1,1,1,2-Tetrachloroethane	10.165	131	1042	0.910	ug/l #	59
67) Ethyl Benzene	10.195	91	6238	1.055	ug/l #	89
68) m/p-Xylenes	10.305	106	4454	2.076	ug/l	94
69) o-Xylene	10.640	106	2072	0.999	ug/l	96
70) Styrene	10.658	104	3482	0.980	ug/l	95
71) Bromoform	10.805	173	824	0.944	ug/l #	95
73) Isopropylbenzene	10.963	105	5637	0.991	ug/l	99
74) N-amyl acetate	10.847	43	2060	0.823	ug/l	95
75) 1,1,2,2-Tetrachloroethane	11.213	83	1661	0.912	ug/l	86
76) 1,2,3-Trichloropropane	11.244	75	1578m	1.013	ug/l	
77) Bromobenzene	11.207	156	1386	1.050	ug/l	94
78) n-propylbenzene	11.305	91	7308	1.062	ug/l	92
79) 2-Chlorotoluene	11.366	91	4466	1.076	ug/l	98
80) 1,3,5-Trimethylbenzene	11.451	105	4806	1.014	ug/l	96
82) 4-Chlorotoluene	11.457	91	5603	1.139	ug/l	98
83) tert-Butylbenzene	11.713	119	4751	0.985	ug/l	97
84) 1,2,4-Trimethylbenzene	11.756	105	4928	1.028	ug/l	99
85) sec-Butylbenzene	11.890	105	6450	1.041	ug/l	99
86) p-Isopropyltoluene	12.012	119	5657	1.095	ug/l	96
87) 1,3-Dichlorobenzene	11.969	146	3045	1.188	ug/l	96
88) 1,4-Dichlorobenzene	12.036	146	3503m	1.319	ug/l	
89) n-Butylbenzene	12.335	91	6072	1.197	ug/l	97
90) Hexachloroethane	12.536	117	987	1.075	ug/l	88
91) 1,2-Dichlorobenzene	12.335	146	2761	1.116	ug/l	94
92) 1,2-Dibromo-3-Chloropr...	12.945	75	345	0.846	ug/l	84
93) 1,2,4-Trichlorobenzene	13.591	180	2189	1.297	ug/l	92
94) Hexachlorobutadiene	13.725	225	1006	1.283	ug/l	97
95) Naphthalene	13.780	128	5474	1.023	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	2171	1.283	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046524.D
Acq On : 06 Jun 2025 12:57
Operator : JC/MD
Sample : VSTDICC001
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

Quant Time: Jun 06 16:43:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:38:39 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/09/2025
Supervised By :Mahesh Dadoda 06/09/2025

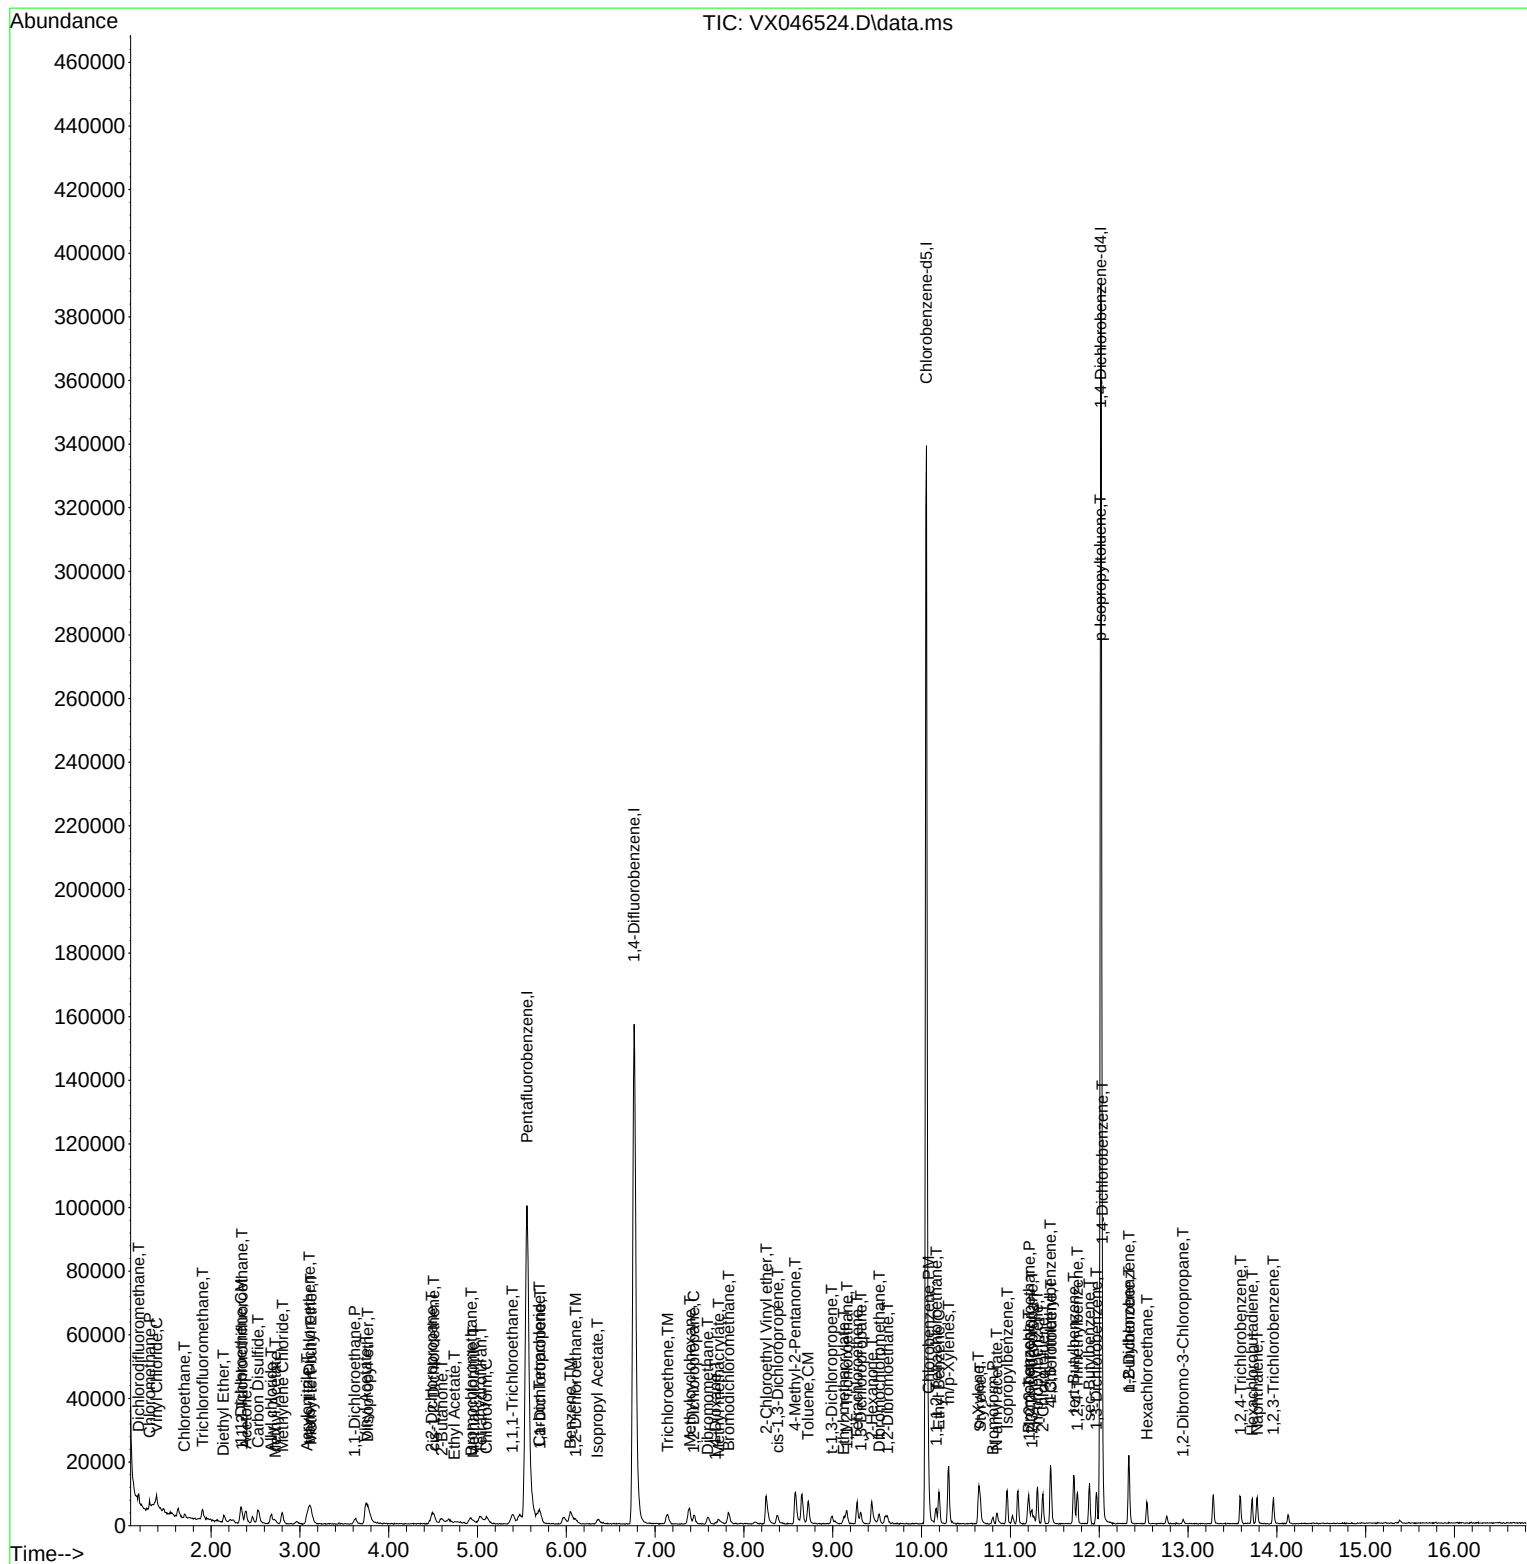

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046525.D
 Acq On : 06 Jun 2025 14:11
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX060625

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:57:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	87638	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	151058	50.000	ug/l	-0.01
63) Chlorobenzene-d5	10.055	117	132539	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	65454	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	78349	50.250	ug/l	-0.01
Spiked Amount 50.000	Range 74 - 125		Recovery = 100.500%			
35) Dibromofluoromethane	5.391	113	56698	51.039	ug/l	-0.01
Spiked Amount 50.000	Range 75 - 124		Recovery = 102.080%			
50) Toluene-d8	8.647	98	183212	50.025	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 100.040%			
62) 4-Bromofluorobenzene	11.079	95	75584	49.880	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 99.760%			
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.179	85	59758	49.116	ug/l	98
3) Chloromethane	1.307	50	53337	48.162	ug/l	98
4) Vinyl Chloride	1.386	62	54649	49.502	ug/l	99
5) Bromomethane	1.618	94	34113	50.900	ug/l	93
6) Chloroethane	1.697	64	33633	46.955	ug/l	93
7) Trichlorofluoromethane	1.898	101	90940	49.788	ug/l	100
8) Diethyl Ether	2.142	74	32152	49.819	ug/l	96
9) 1,1,2-Trichlorotrifluo...	2.343	101	57034	49.561	ug/l	97
10) Methyl Iodide	2.465	142	67786	54.338	ug/l	100
11) Tert butyl alcohol	2.965	59	47374	273.823	ug/l	99
12) 1,1-Dichloroethene	2.331	96	51107	49.119	ug/l	99
13) Acrolein	2.246	56	51802	247.857	ug/l	98
14) Allyl chloride	2.678	41	105373	51.566	ug/l	94
15) Acrylonitrile	3.069	53	174229	266.347	ug/l	98
16) Acetone	2.386	43	157823	257.624	ug/l	99
17) Carbon Disulfide	2.526	76	110616	50.069	ug/l	98
18) Methyl Acetate	2.715	43	106595	57.396	ug/l	99
19) Methyl tert-butyl Ether	3.123	73	195706	53.754	ug/l	98
20) Methylene Chloride	2.800	84	60058	48.013	ug/l	96
21) trans-1,2-Dichloroethene	3.099	96	52668	47.832	ug/l	96
22) Diisopropyl ether	3.770	45	212853	52.834	ug/l #	80
23) Vinyl Acetate	3.727	43	827531	266.053	ug/l	99
24) 1,1-Dichloroethane	3.617	63	115021	51.227	ug/l	98
25) 2-Butanone	4.562	43	232201	267.525	ug/l	99
26) 2,2-Dichloropropane	4.483	77	89180	53.502	ug/l	99
27) cis-1,2-Dichloroethene	4.501	96	66779	49.265	ug/l	99
28) Bromochloromethane	4.904	49	52893	49.390	ug/l	99
29) Tetrahydrofuran	5.013	42	146302	266.904	ug/l	98
30) Chloroform	5.099	83	119994	51.004	ug/l	95
31) Cyclohexane	5.477	56	88988	49.093	ug/l	99
32) 1,1,1-Trichloroethane	5.391	97	103945	51.651	ug/l	97
36) 1,1-Dichloropropene	5.696	75	75696	47.703	ug/l	99
37) Ethyl Acetate	4.721	43	90139	58.203	ug/l	99
38) Carbon Tetrachloride	5.684	117	87750	49.372	ug/l	96
39) Methylcyclohexane	7.385	83	89168	47.608	ug/l	99
40) Benzene	6.044	78	221890	49.672	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046525.D
 Acq On : 06 Jun 2025 14:11
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX060625

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/06/2025
 Supervised By : Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:57:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	54128	56.282	ug/l	97
42) 1,2-Dichloroethane	6.092	62	94588	50.897	ug/l	99
43) Isopropyl Acetate	6.342	43	146579	54.290	ug/l	100
44) Trichloroethene	7.129	130	54213	47.764	ug/l	96
45) 1,2-Dichloropropane	7.434	63	59286	51.417	ug/l	99
46) Dibromomethane	7.586	93	44071	50.807	ug/l	99
47) Bromodichloromethane	7.824	83	94362	52.906	ug/l	97
48) Methyl methacrylate	7.696	41	76134	54.806	ug/l	97
49) 1,4-Dioxane	7.659	88	20118	1082.971	ug/l	94
51) 4-Methyl-2-Pentanone	8.574	43	466259	271.760	ug/l	100
52) Toluene	8.714	92	136448	49.719	ug/l	99
53) t-1,3-Dichloropropene	8.976	75	85596	53.526	ug/l	99
54) cis-1,3-Dichloropropene	8.366	75	92273	51.896	ug/l	91
55) 1,1,2-Trichloroethane	9.153	97	57283	51.993	ug/l	98
56) Ethyl methacrylate	9.116	69	92299	54.440	ug/l	97
57) 1,3-Dichloropropane	9.305	76	98748	50.718	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.245	63	240616	260.553	ug/l	100
59) 2-Hexanone	9.427	43	337353	274.165	ug/l	99
60) Dibromochloromethane	9.519	129	68814	53.100	ug/l	97
61) 1,2-Dibromoethane	9.610	107	57046	49.689	ug/l	96
64) Tetrachloroethene	9.275	164	42310	47.739	ug/l	97
65) Chlorobenzene	10.080	112	154357	49.518	ug/l	100
66) 1,1,1,2-Tetrachloroethane	10.159	131	55536	52.723	ug/l	100
67) Ethyl Benzene	10.195	91	273659	50.288	ug/l	98
68) m/p-Xylenes	10.299	106	199258	100.941	ug/l	99
69) o-Xylene	10.640	106	97151	50.882	ug/l	99
70) Styrene	10.653	104	169628	51.899	ug/l	100
71) Bromoform	10.799	173	42728	53.200	ug/l #	99
73) Isopropylbenzene	10.957	105	266347	51.765	ug/l	100
74) N-amyl acetate	10.842	43	125656	55.456	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	86308	52.405	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	73842m	53.262	ug/l	
77) Bromobenzene	11.195	156	60607	50.748	ug/l	98
78) n-propylbenzene	11.305	91	316743	50.860	ug/l	100
79) 2-Chlorotoluene	11.360	91	191582	51.014	ug/l	99
80) 1,3,5-Trimethylbenzene	11.451	105	221291	51.612	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	26534	55.208	ug/l	97
82) 4-Chlorotoluene	11.451	91	224207	50.368	ug/l	99
83) tert-Butylbenzene	11.713	119	226613	51.919	ug/l	98
84) 1,2,4-Trimethylbenzene	11.750	105	223226	51.464	ug/l	99
85) sec-Butylbenzene	11.890	105	284027	50.644	ug/l	100
86) p-Isopropyltoluene	12.006	119	237583	50.815	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	114034	49.171	ug/l	99
88) 1,4-Dichlorobenzene	12.037	146	114838	47.788	ug/l	99
89) n-Butylbenzene	12.329	91	232333	50.601	ug/l	100
90) Hexachloroethane	12.536	117	42498	51.141	ug/l	99
91) 1,2-Dichlorobenzene	12.335	146	111587	49.847	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	20611	55.886	ug/l	98
93) 1,2,4-Trichlorobenzene	13.585	180	75169	49.224	ug/l	99
94) Hexachlorobutadiene	13.725	225	33512	47.222	ug/l	98
95) Naphthalene	13.774	128	257845	53.245	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	75157	49.082	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046525.D
Acq On : 06 Jun 2025 14:11
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX060625

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:57:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed



```
Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\  
Data File : VX046525.D  
Acq On    : 06 Jun 2025  14:11  
Operator  : JC/MD  
Sample    : VSTDICV050  
Misc      : 5.0mL/MSVOA_X/WATER  
ALS Vial  : 10   Sample Multiplier: 1
```

Instrument :
MSVOA_X
ClientSampleId :
ICVVX060625

Manual Integrations APPROVED

Reviewed By :John Carlone 06/06/2025
Supervised By :Mahesh Dadoda 06/09/2025

Quant Time: Jun 06 16:57:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

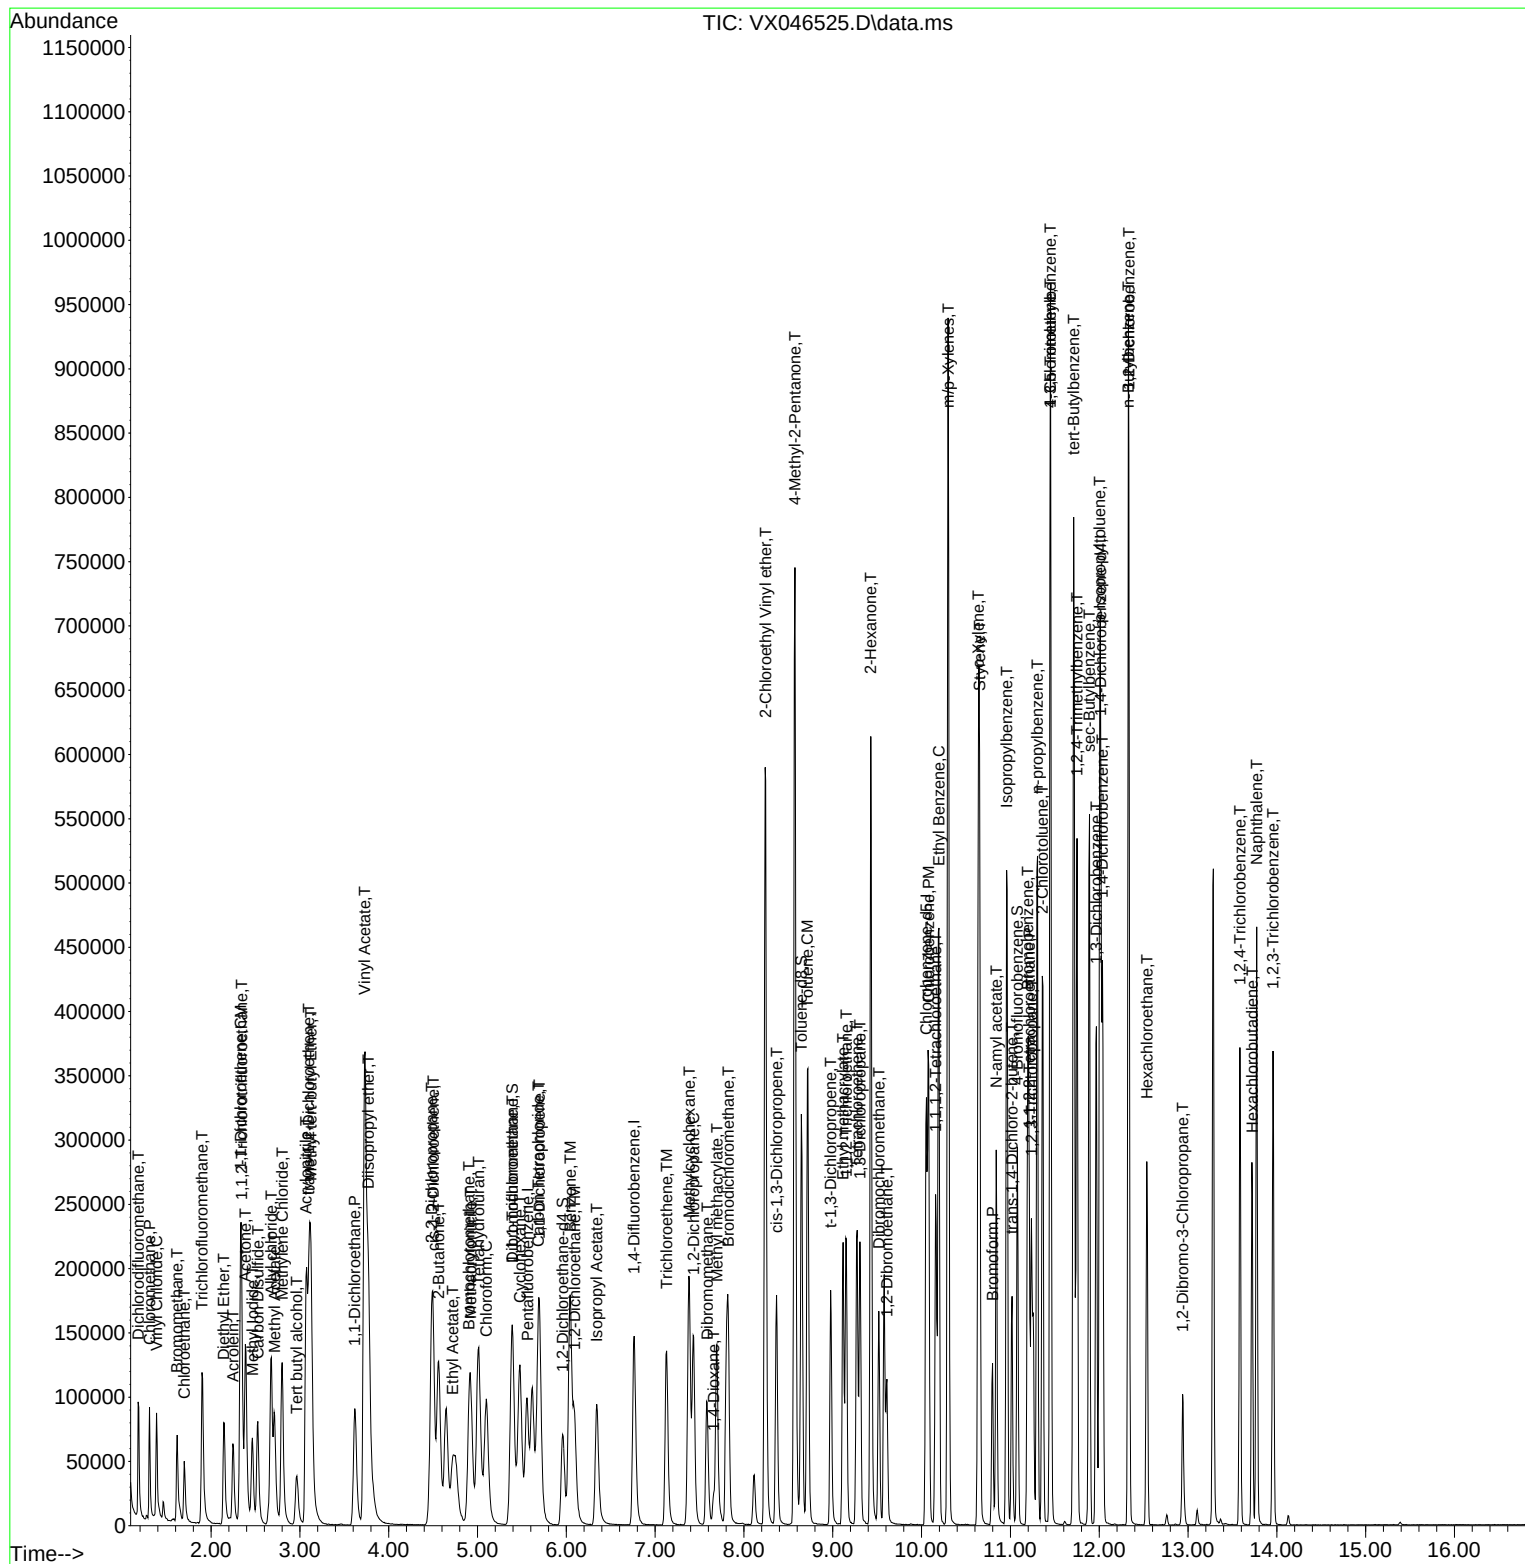

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046525.D
 Acq On : 06 Jun 2025 14:11
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX060625

Quant Time: Jun 06 16:57:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	97	0.00
2 T	Dichlorodifluoromethane	0.694	0.682	1.7	103	0.00
3 P	Chloromethane	0.632	0.609	3.6	103	0.00
4 C	Vinyl Chloride	0.630	0.624	1.0#	102	0.00
5 T	Bromomethane	0.382	0.389	-1.8	95	0.00
6 T	Chloroethane	0.409	0.384	6.1	100	0.00
7 T	Trichlorofluoromethane	1.042	1.038	0.4	99	0.00
8 T	Diethyl Ether	0.368	0.367	0.3	100	-0.01
9 T	1,1,2-Trichlorotrifluoroeth	0.657	0.651	0.9	99	0.00
10 T	Methyl Iodide	0.712	0.773	-8.6	105	0.00
11 T	Tert butyl alcohol	0.099	0.108	-9.1	108	0.00
12 CM	1,1-Dichloroethene	0.594	0.583	1.9#	100	0.00
13 T	Acrolein	0.103	0.118	-14.6	102	0.00
14 T	Allyl chloride	1.166	1.202	-3.1	103	0.00
15 T	Acrylonitrile	0.373	0.398	-6.7	102	-0.01
16 T	Acetone	0.381	0.360	5.5	103	0.00
17 T	Carbon Disulfide	1.481	1.262	14.8	101	0.00
18 T	Methyl Acetate	1.060	1.216	-14.7	105	0.00
19 T	Methyl tert-butyl Ether	2.077	2.233	-7.5	103	-0.01
20 T	Methylene Chloride	0.714	0.685	4.1	101	0.00
21 T	trans-1,2-Dichloroethene	0.628	0.601	4.3	100	-0.01
22 T	Diisopropyl ether	2.298	2.429	-5.7	101	-0.01
23 T	Vinyl Acetate	1.775	1.889	-6.4	100	-0.01
24 P	1,1-Dichloroethane	1.281	1.312	-2.4	101	-0.01
25 T	2-Butanone	0.495	0.530	-7.1	102	-0.01
26 T	2,2-Dichloropropane	0.951	1.018	-7.0	102	-0.01
27 T	cis-1,2-Dichloroethene	0.773	0.762	1.4	100	0.00
28 T	Bromochloromethane	0.611	0.604	1.1	100	-0.01
29 T	Tetrahydrofuran	0.313	0.334	-6.7	103	0.00
30 C	Chloroform	1.342	1.369	-2.0#	101	-0.01
31 T	Cyclohexane	1.034	1.015	1.8	99	-0.01
32 T	1,1,1-Trichloroethane	1.148	1.186	-3.3	101	0.00
33 S	1,2-Dichloroethane-d4	0.890	0.894	-0.4	100	-0.01
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	97	-0.01
35 S	Dibromofluoromethane	0.368	0.375	-1.9	99	-0.01
36 T	1,1-Dichloropropene	0.525	0.501	4.6	100	-0.02
37 T	Ethyl Acetate	0.513	0.597	-16.4	104	-0.01
38 T	Carbon Tetrachloride	0.588	0.581	1.2	100	-0.01
39 T	Methylcyclohexane	0.620	0.590	4.8	100	0.00
40 TM	Benzene	1.479	1.469	0.7	100	-0.01
41 T	Methacrylonitrile	0.318	0.358	-12.6	107	-0.01
42 TM	1,2-Dichloroethane	0.615	0.626	-1.8	99	0.00
43 T	Isopropyl Acetate	0.894	0.970	-8.5	102	-0.01
44 TM	Trichloroethene	0.376	0.359	4.5	99	0.00
45 C	1,2-Dichloropropane	0.382	0.392	-2.6#	100	0.00
46 T	Dibromomethane	0.287	0.292	-1.7	101	0.00
47 T	Bromodichloromethane	0.590	0.625	-5.9	100	0.00
48 T	Methyl methacrylate	0.460	0.504	-9.6	101	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046525.D
 Acq On : 06 Jun 2025 14:11
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ICSVVX060625

Quant Time: Jun 06 16:57:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.006	0.007	-16.7	102	-0.01
50 S	Toluene-d8	1.212	1.213	-0.1	99	0.00
51 T	4-Methyl-2-Pentanone	0.568	0.617	-8.6	101	0.00
52 CM	Toluene	0.908	0.903	0.6#	99	0.00
53 T	t-1,3-Dichloropropene	0.529	0.567	-7.2	101	0.00
54 T	cis-1,3-Dichloropropene	0.589	0.611	-3.7	100	0.00
55 T	1,1,2-Trichloroethane	0.365	0.379	-3.8	100	0.00
56 T	Ethyl methacrylate	0.561	0.611	-8.9	101	0.00
57 T	1,3-Dichloropropane	0.644	0.654	-1.6	99	0.00
58 T	2-Chloroethyl Vinyl ether	0.306	0.319	-4.2	98	0.00
59 T	2-Hexanone	0.407	0.447	-9.8	101	0.00
60 T	Dibromochloromethane	0.429	0.456	-6.3	102	0.00
61 T	1,2-Dibromoethane	0.380	0.378	0.5	99	0.00
62 S	4-Bromofluorobenzene	0.502	0.500	0.4	98	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	97	0.00
64 T	Tetrachloroethene	0.334	0.319	4.5	100	0.00
65 PM	Chlorobenzene	1.176	1.165	0.9	100	0.00
66 T	1,1,1,2-Tetrachloroethane	0.397	0.419	-5.5	101	0.00
67 C	Ethyl Benzene	2.053	2.065	-0.6#	99	0.00
68 T	m/p-Xylenes	0.745	0.752	-0.9	99	0.00
69 T	o-Xylene	0.720	0.733	-1.8	99	0.00
70 T	Styrene	1.233	1.280	-3.8	99	0.00
71 P	Bromoform	0.303	0.322	-6.3	100	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	95	0.00
73 T	Isopropylbenzene	3.930	4.069	-3.5	99	0.00
74 T	N-amyl acetate	1.731	1.920	-10.9	101	0.00
75 P	1,1,2,2-Tetrachloroethane	1.258	1.319	-4.8	100	0.00
76 T	1,2,3-Trichloropropane	1.059	1.128	-6.5	102	0.00
77 T	Bromobenzene	0.912	0.926	-1.5	100	0.00
78 T	n-propylbenzene	4.757	4.839	-1.7	98	0.00
79 T	2-Chlorotoluene	2.869	2.927	-2.0	100	0.00
80 T	1,3,5-Trimethylbenzene	3.275	3.381	-3.2	99	0.00
81 T	trans-1,4-Dichloro-2-butene	0.367	0.405	-10.4	104	0.00
82 T	4-Chlorotoluene	3.400	3.425	-0.7	99	0.00
83 T	tert-Butylbenzene	3.334	3.462	-3.8	100	0.00
84 T	1,2,4-Trimethylbenzene	3.313	3.410	-2.9	100	0.00
85 T	sec-Butylbenzene	4.284	4.339	-1.3	99	0.00
86 T	p-Isopropyltoluene	3.572	3.630	-1.6	99	0.00
87 T	1,3-Dichlorobenzene	1.772	1.742	1.7	98	0.00
88 T	1,4-Dichlorobenzene	1.836	1.754	4.5	100	0.00
89 T	n-Butylbenzene	3.507	3.550	-1.2	101	0.00
90 T	Hexachloroethane	0.635	0.649	-2.2	101	0.00
91 T	1,2-Dichlorobenzene	1.710	1.705	0.3	99	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.282	0.315	-11.7	105	0.00
93 T	1,2,4-Trichlorobenzene	1.167	1.148	1.6	101	0.00
94 T	Hexachlorobutadiene	0.542	0.512	5.5	97	0.00
95 T	Naphthalene	3.699	3.939	-6.5	101	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046525.D
Acq On : 06 Jun 2025 14:11
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX060625

Quant Time: Jun 06 16:57:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	1.170	1.148	1.9	100	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046525.D
 Acq On : 06 Jun 2025 14:11
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX060625

Quant Time: Jun 06 16:57:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	97	0.00
2 T	Dichlorodifluoromethane	50.000	49.116	1.8	103	0.00
3 P	Chloromethane	50.000	48.162	3.7	103	0.00
4 C	Vinyl Chloride	50.000	49.502	1.0#	102	0.00
5 T	Bromomethane	50.000	50.900	-1.8	95	0.00
6 T	Chloroethane	50.000	46.955	6.1	100	0.00
7 T	Trichlorofluoromethane	50.000	49.788	0.4	99	0.00
8 T	Diethyl Ether	50.000	49.819	0.4	100	-0.01
9 T	1,1,2-Trichlorotrifluoroeth	50.000	49.561	0.9	99	0.00
10 T	Methyl Iodide	50.000	54.338	-8.7	105	0.00
11 T	Tert butyl alcohol	250.000	273.823	-9.5	108	0.00
12 CM	1,1-Dichloroethene	50.000	49.119	1.8#	100	0.00
13 T	Acrolein	250.000	247.857	0.9	102	0.00
14 T	Allyl chloride	50.000	51.566	-3.1	103	0.00
15 T	Acrylonitrile	250.000	266.347	-6.5	102	-0.01
16 T	Acetone	250.000	257.624	-3.0	103	0.00
17 T	Carbon Disulfide	50.000	50.069	-0.1	101	0.00
18 T	Methyl Acetate	50.000	57.396	-14.8	105	0.00
19 T	Methyl tert-butyl Ether	50.000	53.754	-7.5	103	-0.01
20 T	Methylene Chloride	50.000	48.013	4.0	101	0.00
21 T	trans-1,2-Dichloroethene	50.000	47.832	4.3	100	-0.01
22 T	Diisopropyl ether	50.000	52.834	-5.7	101	-0.01
23 T	Vinyl Acetate	250.000	266.053	-6.4	100	-0.01
24 P	1,1-Dichloroethane	50.000	51.227	-2.5	101	-0.01
25 T	2-Butanone	250.000	267.525	-7.0	102	-0.01
26 T	2,2-Dichloropropane	50.000	53.502	-7.0	102	-0.01
27 T	cis-1,2-Dichloroethene	50.000	49.265	1.5	100	0.00
28 T	Bromochloromethane	50.000	49.390	1.2	100	-0.01
29 T	Tetrahydrofuran	250.000	266.904	-6.8	103	0.00
30 C	Chloroform	50.000	51.004	-2.0#	101	-0.01
31 T	Cyclohexane	50.000	49.093	1.8	99	-0.01
32 T	1,1,1-Trichloroethane	50.000	51.651	-3.3	101	0.00
33 S	1,2-Dichloroethane-d4	50.000	50.250	-0.5	100	-0.01
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	97	-0.01
35 S	Dibromofluoromethane	50.000	51.039	-2.1	99	-0.01
36 T	1,1-Dichloropropene	50.000	47.703	4.6	100	-0.02
37 T	Ethyl Acetate	50.000	58.203	-16.4	104	-0.01
38 T	Carbon Tetrachloride	50.000	49.372	1.3	100	-0.01
39 T	Methylcyclohexane	50.000	47.608	4.8	100	0.00
40 TM	Benzene	50.000	49.672	0.7	100	-0.01
41 T	Methacrylonitrile	50.000	56.282	-12.6	107	-0.01
42 TM	1,2-Dichloroethane	50.000	50.897	-1.8	99	0.00
43 T	Isopropyl Acetate	50.000	54.290	-8.6	102	-0.01
44 TM	Trichloroethene	50.000	47.764	4.5	99	0.00
45 C	1,2-Dichloropropane	50.000	51.417	-2.8#	100	0.00
46 T	Dibromomethane	50.000	50.807	-1.6	101	0.00
47 T	Bromodichloromethane	50.000	52.906	-5.8	100	0.00
48 T	Methyl methacrylate	50.000	54.806	-9.6	101	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
 Data File : VX046525.D
 Acq On : 06 Jun 2025 14:11
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX060625

Quant Time: Jun 06 16:57:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	1082.971	-8.3	102	-0.01
50 S	Toluene-d8	50.000	50.025	-0.0	99	0.00
51 T	4-Methyl-2-Pentanone	250.000	271.760	-8.7	101	0.00
52 CM	Toluene	50.000	49.719	0.6#	99	0.00
53 T	t-1,3-Dichloropropene	50.000	53.526	-7.1	101	0.00
54 T	cis-1,3-Dichloropropene	50.000	51.896	-3.8	100	0.00
55 T	1,1,2-Trichloroethane	50.000	51.993	-4.0	100	0.00
56 T	Ethyl methacrylate	50.000	54.440	-8.9	101	0.00
57 T	1,3-Dichloropropane	50.000	50.718	-1.4	99	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	260.553	-4.2	98	0.00
59 T	2-Hexanone	250.000	274.165	-9.7	101	0.00
60 T	Dibromochloromethane	50.000	53.100	-6.2	102	0.00
61 T	1,2-Dibromoethane	50.000	49.689	0.6	99	0.00
62 S	4-Bromofluorobenzene	50.000	49.880	0.2	98	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	97	0.00
64 T	Tetrachloroethene	50.000	47.739	4.5	100	0.00
65 PM	Chlorobenzene	50.000	49.518	1.0	100	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	52.723	-5.4	101	0.00
67 C	Ethyl Benzene	50.000	50.288	-0.6#	99	0.00
68 T	m/p-Xylenes	100.000	100.941	-0.9	99	0.00
69 T	o-Xylene	50.000	50.882	-1.8	99	0.00
70 T	Styrene	50.000	51.899	-3.8	99	0.00
71 P	Bromoform	50.000	53.200	-6.4	100	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	95	0.00
73 T	Isopropylbenzene	50.000	51.765	-3.5	99	0.00
74 T	N-amyl acetate	50.000	55.456	-10.9	101	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	52.405	-4.8	100	0.00
76 T	1,2,3-Trichloropropane	50.000	53.262	-6.5	102	0.00
77 T	Bromobenzene	50.000	50.748	-1.5	100	0.00
78 T	n-propylbenzene	50.000	50.860	-1.7	98	0.00
79 T	2-Chlorotoluene	50.000	51.014	-2.0	100	0.00
80 T	1,3,5-Trimethylbenzene	50.000	51.612	-3.2	99	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	55.208	-10.4	104	0.00
82 T	4-Chlorotoluene	50.000	50.368	-0.7	99	0.00
83 T	tert-Butylbenzene	50.000	51.919	-3.8	100	0.00
84 T	1,2,4-Trimethylbenzene	50.000	51.464	-2.9	100	0.00
85 T	sec-Butylbenzene	50.000	50.644	-1.3	99	0.00
86 T	p-Isopropyltoluene	50.000	50.815	-1.6	99	0.00
87 T	1,3-Dichlorobenzene	50.000	49.171	1.7	98	0.00
88 T	1,4-Dichlorobenzene	50.000	47.788	4.4	100	0.00
89 T	n-Butylbenzene	50.000	50.601	-1.2	101	0.00
90 T	Hexachloroethane	50.000	51.141	-2.3	101	0.00
91 T	1,2-Dichlorobenzene	50.000	49.847	0.3	99	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	55.886	-11.8	105	0.00
93 T	1,2,4-Trichlorobenzene	50.000	49.224	1.6	101	0.00
94 T	Hexachlorobutadiene	50.000	47.222	5.6	97	0.00
95 T	Naphthalene	50.000	53.245	-6.5	101	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046525.D
Acq On : 06 Jun 2025 14:11
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX060625

Quant Time: Jun 06 16:57:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	50.000	49.082	1.8	100	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: CHEMTECH Contract: JAC005
 Lab Code: CHEM Case No.: Q2234 SAS No.: Q2234 SDG No.: Q2234
 Instrument ID: MSVOA_X Calibration Date/Time: 06/10/2025 09:07
 Lab File ID: VX046586.D Init. Calib. Date(s): 06/06/2025 06/06/2025
 Heated Purge: (Y/N) N Init. Calib. Time(s): 09:42 12:57
 GC Column: DB-624UI ID: 0.18 (mm)

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Vinyl Chloride	0.630	0.640		1.59	20
1,1-Dichloroethene	0.594	0.603		1.51	20
1,1-Dichloroethane	1.281	1.282	0.1	0.08	20
cis-1,2-Dichloroethene	0.773	0.814		5.3	20
1,1,1-Trichloroethane	1.148	1.224		6.62	20
Benzene	1.479	1.615		9.19	20
1,2-Dichloroethane	0.615	0.657		6.83	20
Trichloroethene	0.376	0.395		5.05	20
1,1,2-Trichloroethane	0.365	0.402		10.14	20
Tetrachloroethene	0.334	0.336		0.6	20
1,2-Dichloroethane-d4	0.890	0.757		-14.94	20
Dibromofluoromethane	0.368	0.360		-2.17	20
Toluene-d8	1.212	1.152		-4.95	20
4-Bromofluorobenzene	0.502	0.468		-6.77	20

All other compounds must meet a minimum RRF of 0.010.
 RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046586.D
 Acq On : 10 Jun 2025 09:07
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050

Manual Integrations
 APPROVED

Reviewed By :John Carlone 06/11/2025
 Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:40:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	90758	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.763	114	150623	50.000	ug/l	-0.01
63) Chlorobenzene-d5	10.055	117	134767	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	66941	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	68670	42.529	ug/l	-0.01
Spiked Amount 50.000	Range 74 - 125		Recovery =	85.060%		
35) Dibromofluoromethane	5.385	113	54188	48.920	ug/l	-0.02
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.840%		
50) Toluene-d8	8.647	98	173470	47.502	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.000%		
62) 4-Bromofluorobenzene	11.079	95	70476	46.644	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	93.280%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.185	85	64016	50.806	ug/l	100
3) Chloromethane	1.307	50	56444	49.215	ug/l	99
4) Vinyl Chloride	1.386	62	58114	50.831	ug/l	98
5) Bromomethane	1.618	94	32498	46.823	ug/l	93
6) Chloroethane	1.703	64	32178	43.380	ug/l	97
7) Trichlorofluoromethane	1.904	101	90554	47.872	ug/l	96
8) Diethyl Ether	2.142	74	31717	47.456	ug/l	88
9) 1,1,2-Trichlorotrifluo...	2.343	101	60548	50.805	ug/l	94
10) Methyl Iodide	2.465	142	73653	57.012	ug/l	97
11) Tert butyl alcohol	2.959	59	31425	175.393	ug/l	100
12) 1,1-Dichloroethene	2.331	96	54724	50.787	ug/l	87
13) Acrolein	2.245	56	46336	218.171	ug/l	99
14) Allyl chloride	2.678	41	99768	47.145	ug/l	92
15) Acrylonitrile	3.068	53	154316	227.796	ug/l	99
16) Acetone	2.386	43	125573	198.999	ug/l	94
17) Carbon Disulfide	2.526	76	113942	49.803	ug/l	99
18) Methyl Acetate	2.709	43	88227	45.873	ug/l	96
19) Methyl tert-butyl Ether	3.123	73	190642	50.563	ug/l	98
20) Methylene Chloride	2.800	84	63269	48.842	ug/l	92
21) trans-1,2-Dichloroethene	3.105	96	56466	49.518	ug/l	94
22) Diisopropyl ether	3.763	45	218014	52.255	ug/l #	73
23) Vinyl Acetate	3.727	43	792157	245.925	ug/l	98
24) 1,1-Dichloroethane	3.623	63	116355	50.040	ug/l	99
25) 2-Butanone	4.556	43	191877	213.467	ug/l	99
26) 2,2-Dichloropropane	4.483	77	96821	56.089	ug/l	99
27) cis-1,2-Dichloroethene	4.495	96	73894	52.640	ug/l	96
28) Bromochloromethane	4.904	49	54238	48.905	ug/l	99
29) Tetrahydrofuran	5.007	42	122206	215.281	ug/l	99
30) Chloroform	5.099	83	130421	53.531	ug/l	96
31) Cyclohexane	5.477	56	95665	50.962	ug/l	98
32) 1,1,1-Trichloroethane	5.391	97	111065	53.292	ug/l	98
36) 1,1-Dichloropropene	5.696	75	80709	51.010	ug/l	98
37) Ethyl Acetate	4.721	43	78957	51.130	ug/l	99
38) Carbon Tetrachloride	5.684	117	95156	53.694	ug/l	95
39) Methylcyclohexane	7.379	83	94883	50.806	ug/l	99
40) Benzene	6.037	78	243205	54.601	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046586.D
 Acq On : 10 Jun 2025 09:07
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/11/2025
 Supervised By : Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:40:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	49327	51.438	ug/l	95
42) 1,2-Dichloroethane	6.086	62	98959	53.402	ug/l	99
43) Isopropyl Acetate	6.342	43	131206	48.737	ug/l	99
44) Trichloroethene	7.129	130	59456	52.534	ug/l	99
45) 1,2-Dichloropropane	7.427	63	63071	54.858	ug/l	99
46) Dibromomethane	7.580	93	45581	52.699	ug/l	96
47) Bromodichloromethane	7.824	83	101554	57.103	ug/l	97
48) Methyl methacrylate	7.690	41	68324	49.326	ug/l	95
49) 1,4-Dioxane	7.653	88	17651	952.914	ug/l	98
51) 4-Methyl-2-Pentanone	8.568	43	409850	239.572	ug/l	99
52) Toluene	8.714	92	149428	54.605	ug/l	99
53) t-1,3-Dichloropropene	8.976	75	91050	57.101	ug/l	98
54) cis-1,3-Dichloropropene	8.366	75	100606	56.746	ug/l	92
55) 1,1,2-Trichloroethane	9.147	97	60612	55.174	ug/l	97
56) Ethyl methacrylate	9.116	69	90648	53.621	ug/l	94
57) 1,3-Dichloropropane	9.305	76	104709	53.935	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.238	63	226143	245.588	ug/l	99
59) 2-Hexanone	9.427	43	281334	229.299	ug/l	98
60) Dibromochloromethane	9.519	129	73121	56.586	ug/l	99
61) 1,2-Dibromoethane	9.604	107	59442	51.925	ug/l	96
64) Tetrachloroethene	9.275	164	45245	50.206	ug/l	96
65) Chlorobenzene	10.079	112	166316	52.473	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	60360	56.356	ug/l	100
67) Ethyl Benzene	10.189	91	293712	53.081	ug/l	99
68) m/p-Xylenes	10.299	106	216146	107.686	ug/l	99
69) o-Xylene	10.640	106	104495	53.823	ug/l	100
70) Styrene	10.652	104	186521	56.124	ug/l	97
71) Bromoform	10.799	173	45425	55.623	ug/l #	97
73) Isopropylbenzene	10.957	105	284717	54.106	ug/l	100
74) N-amyl acetate	10.841	43	114046	49.214	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.207	83	85869	50.980	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	73742m	52.008	ug/l	
77) Bromobenzene	11.195	156	67715	55.440	ug/l	94
78) n-propylbenzene	11.299	91	339470	53.299	ug/l	99
79) 2-Chlorotoluene	11.360	91	202364	52.688	ug/l	99
80) 1,3,5-Trimethylbenzene	11.451	105	236032	53.827	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	25693	52.271	ug/l	90
82) 4-Chlorotoluene	11.451	91	239181	52.538	ug/l	98
83) tert-Butylbenzene	11.713	119	242094	54.234	ug/l	95
84) 1,2,4-Trimethylbenzene	11.750	105	234197	52.794	ug/l	98
85) sec-Butylbenzene	11.890	105	304462	53.081	ug/l	100
86) p-Isopropyltoluene	12.006	119	252631	52.834	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	124600	52.534	ug/l	99
88) 1,4-Dichlorobenzene	12.036	146	123785	50.367	ug/l	99
89) n-Butylbenzene	12.329	91	245852	52.356	ug/l	99
90) Hexachloroethane	12.536	117	45495	53.532	ug/l	96
91) 1,2-Dichlorobenzene	12.329	146	121670	53.144	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	17650	46.795	ug/l	94
93) 1,2,4-Trichlorobenzene	13.585	180	81781	52.365	ug/l	98
94) Hexachlorobutadiene	13.725	225	35940	49.518	ug/l	96
95) Naphthalene	13.774	128	251036	50.687	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	80018	51.096	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046586.D
Acq On : 10 Jun 2025 09:07
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:40:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046586.D
 Acq On : 10 Jun 2025 09:07
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050

Manual Integrations APPROVED

Reviewed By : John Carlone 06/11/2025
 Supervised By : Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:40:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

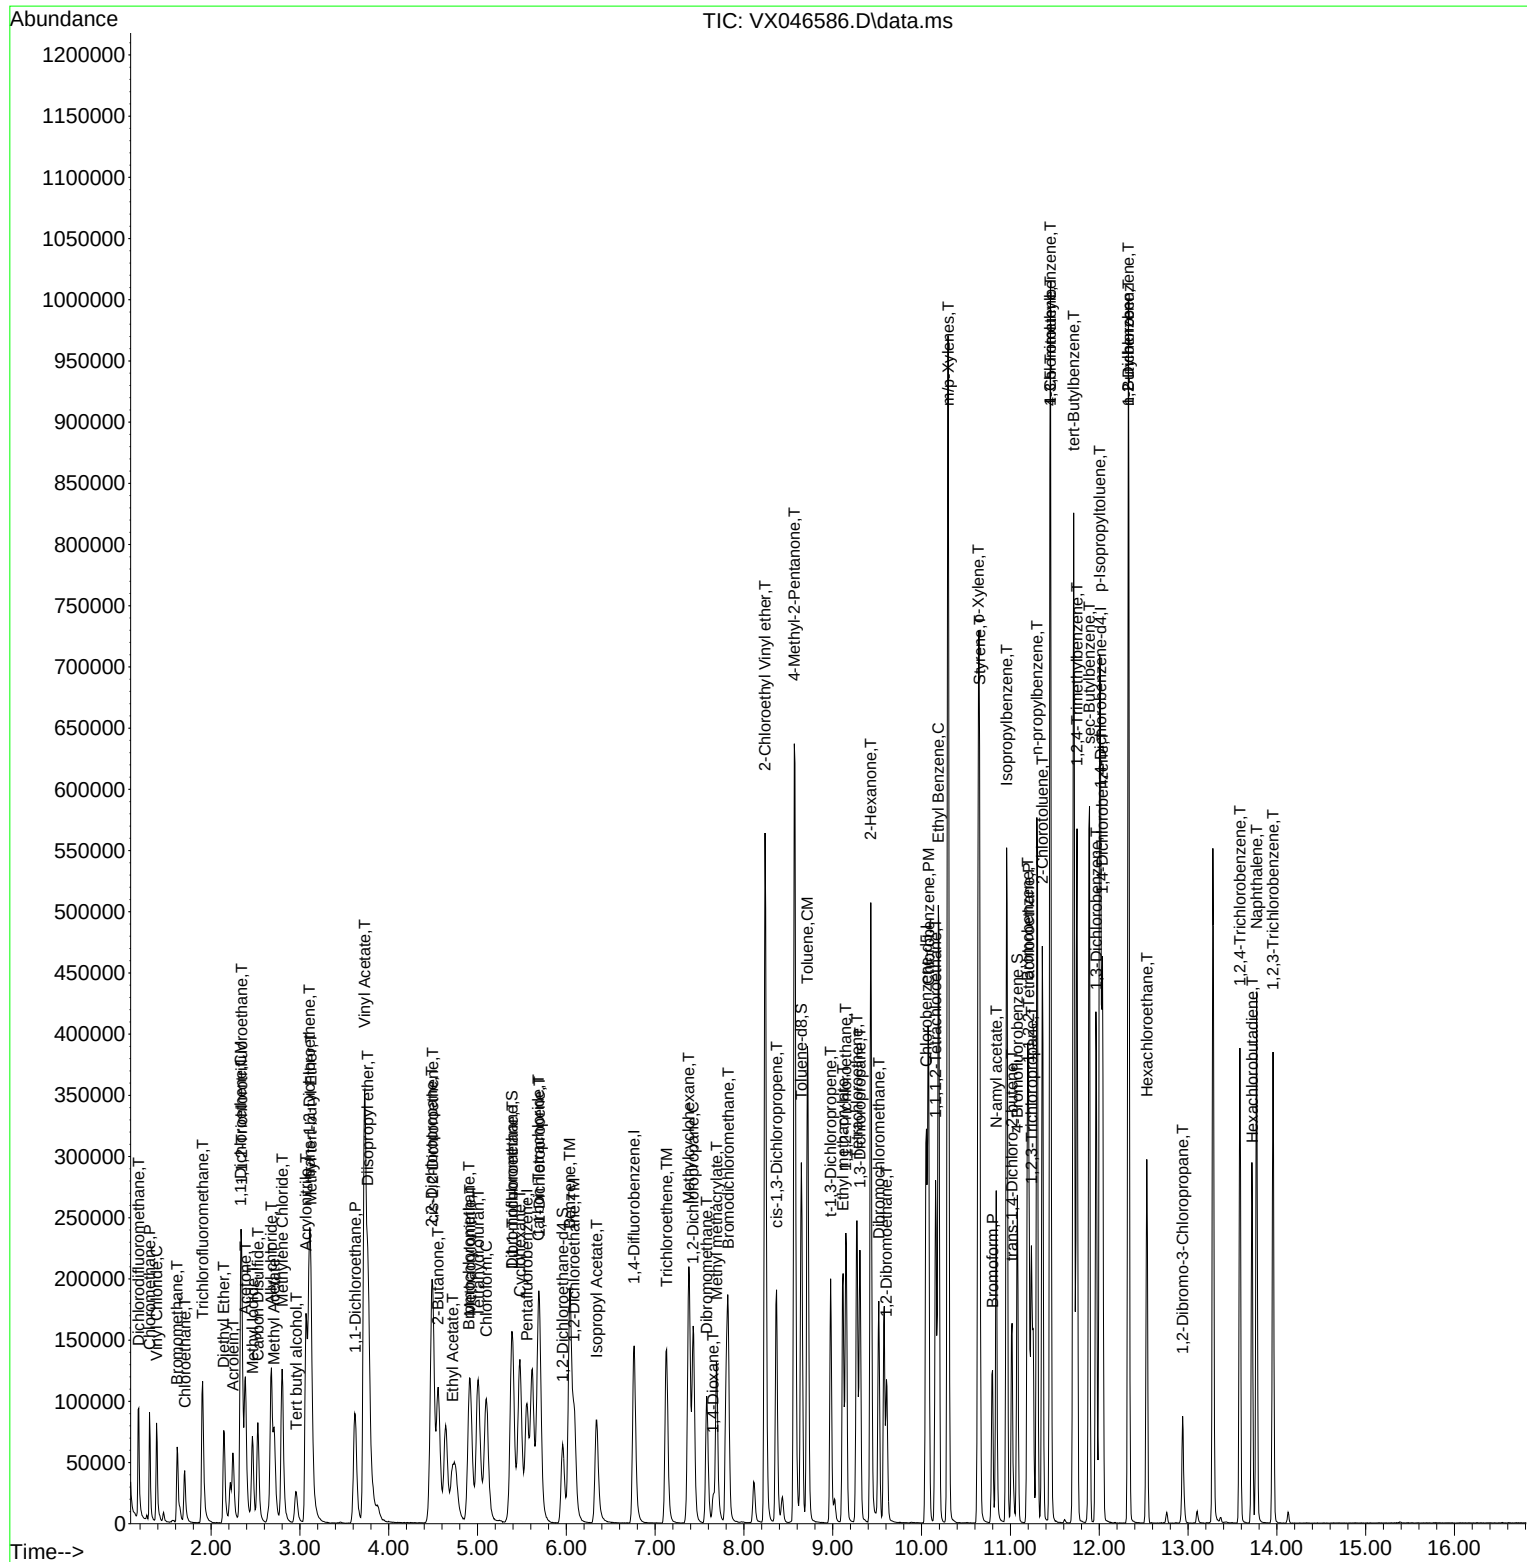

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046586.D
 Acq On : 10 Jun 2025 09:07
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDCCC050

Quant Time: Jun 11 01:40:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	101	-0.01
2 T	Dichlorodifluoromethane	0.694	0.705	-1.6	110	0.00
3 P	Chloromethane	0.632	0.622	1.6	109	0.00
4 C	Vinyl Chloride	0.630	0.640	-1.6#	108	0.00
5 T	Bromomethane	0.382	0.358	6.3	91	0.00
6 T	Chloroethane	0.409	0.355	13.2	96	0.00
7 T	Trichlorofluoromethane	1.042	0.998	4.2	98	0.00
8 T	Diethyl Ether	0.368	0.349	5.2	99	-0.01
9 T	1,1,2-Trichlorotrifluoroeth	0.657	0.667	-1.5	105	0.00
10 T	Methyl Iodide	0.712	0.812	-14.0	114	0.00
11 T	Tert butyl alcohol	0.099	0.069	30.3#	71	-0.01
12 CM	1,1-Dichloroethene	0.594	0.603	-1.5#	107	0.00
13 T	Acrolein	0.103	0.102	1.0	91	0.00
14 T	Allyl chloride	1.166	1.099	5.7	98	0.00
15 T	Acrylonitrile	0.373	0.340	8.8	90	-0.01
16 T	Acetone	0.381	0.277	27.3#	82	0.00
17 T	Carbon Disulfide	1.481	1.255	15.3	104	0.00
18 T	Methyl Acetate	1.060	0.972	8.3	87	-0.01
19 T	Methyl tert-butyl Ether	2.077	2.101	-1.2	100	-0.01
20 T	Methylene Chloride	0.714	0.697	2.4	106	0.00
21 T	trans-1,2-Dichloroethene	0.628	0.622	1.0	108	0.00
22 T	Diisopropyl ether	2.298	2.402	-4.5	103	-0.02
23 T	Vinyl Acetate	1.775	1.746	1.6	96	-0.01
24 P	1,1-Dichloroethane	1.281	1.282	-0.1	103	0.00
25 T	2-Butanone	0.495	0.423	14.5	85	-0.02
26 T	2,2-Dichloropropane	0.951	1.067	-12.2	111	-0.01
27 T	cis-1,2-Dichloroethene	0.773	0.814	-5.3	111	-0.01
28 T	Bromochloromethane	0.611	0.598	2.1	102	-0.01
29 T	Tetrahydrofuran	0.313	0.269	14.1	86	-0.01
30 C	Chloroform	1.342	1.437	-7.1#	110	-0.01
31 T	Cyclohexane	1.034	1.054	-1.9	107	-0.01
32 T	1,1,1-Trichloroethane	1.148	1.224	-6.6	108	0.00
33 S	1,2-Dichloroethane-d4	0.890	0.757	14.9	87	-0.01
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	96	-0.01
35 S	Dibromofluoromethane	0.368	0.360	2.2	94	-0.02
36 T	1,1-Dichloropropene	0.525	0.536	-2.1	107	-0.02
37 T	Ethyl Acetate	0.513	0.524	-2.1	91	-0.01
38 T	Carbon Tetrachloride	0.588	0.632	-7.5	108	-0.01
39 T	Methylcyclohexane	0.620	0.630	-1.6	106	-0.01
40 TM	Benzene	1.479	1.615	-9.2	109	-0.02
41 T	Methacrylonitrile	0.318	0.327	-2.8	98	-0.02
42 TM	1,2-Dichloroethane	0.615	0.657	-6.8	104	-0.01
43 T	Isopropyl Acetate	0.894	0.871	2.6	91	-0.01
44 TM	Trichloroethene	0.376	0.395	-5.1	109	0.00
45 C	1,2-Dichloropropane	0.382	0.419	-9.7#	106	-0.01
46 T	Dibromomethane	0.287	0.303	-5.6	105	0.00
47 T	Bromodichloromethane	0.590	0.674	-14.2	108	0.00
48 T	Methyl methacrylate	0.460	0.454	1.3	91	-0.01

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046586.D
 Acq On : 10 Jun 2025 09:07
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDCCC050

Quant Time: Jun 11 01:40:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.006	0.006	0.0	89	-0.02
50 S	Toluene-d8	1.212	1.152	5.0	93	0.00
51 T	4-Methyl-2-Pentanone	0.568	0.544	4.2	89	0.00
52 CM	Toluene	0.908	0.992	-9.3#	108	0.00
53 T	t-1,3-Dichloropropene	0.529	0.604	-14.2	108	0.00
54 T	cis-1,3-Dichloropropene	0.589	0.668	-13.4	109	0.00
55 T	1,1,2-Trichloroethane	0.365	0.402	-10.1	106	0.00
56 T	Ethyl methacrylate	0.561	0.602	-7.3	100	0.00
57 T	1,3-Dichloropropane	0.644	0.695	-7.9	105	0.00
58 T	2-Chloroethyl Vinyl ether	0.306	0.300	2.0	92	0.00
59 T	2-Hexanone	0.407	0.374	8.1	84	0.00
60 T	Dibromochloromethane	0.429	0.485	-13.1	108	0.00
61 T	1,2-Dibromoethane	0.380	0.395	-3.9	103	0.00
62 S	4-Bromofluorobenzene	0.502	0.468	6.8	92	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	99	0.00
64 T	Tetrachloroethene	0.334	0.336	-0.6	107	0.00
65 PM	Chlorobenzene	1.176	1.234	-4.9	108	0.00
66 T	1,1,1,2-Tetrachloroethane	0.397	0.448	-12.8	110	0.00
67 C	Ethyl Benzene	2.053	2.179	-6.1#	107	0.00
68 T	m/p-Xylenes	0.745	0.802	-7.7	107	0.00
69 T	o-Xylene	0.720	0.775	-7.6	107	0.00
70 T	Styrene	1.233	1.384	-12.2	109	0.00
71 P	Bromoform	0.303	0.337	-11.2	107	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	97	0.00
73 T	Isopropylbenzene	3.930	4.253	-8.2	106	0.00
74 T	N-amyl acetate	1.731	1.704	1.6	92	0.00
75 P	1,1,2,2-Tetrachloroethane	1.258	1.283	-2.0	99	0.00
76 T	1,2,3-Trichloropropane	1.059	1.102	-4.1	102	0.00
77 T	Bromobenzene	0.912	1.012	-11.0	112	0.00
78 T	n-propylbenzene	4.757	5.071	-6.6	105	0.00
79 T	2-Chlorotoluene	2.869	3.023	-5.4	106	0.00
80 T	1,3,5-Trimethylbenzene	3.275	3.526	-7.7	106	0.00
81 T	trans-1,4-Dichloro-2-butene	0.367	0.384	-4.6	101	0.00
82 T	4-Chlorotoluene	3.400	3.573	-5.1	106	0.00
83 T	tert-Butylbenzene	3.334	3.617	-8.5	107	0.00
84 T	1,2,4-Trimethylbenzene	3.313	3.499	-5.6	105	0.00
85 T	sec-Butylbenzene	4.284	4.548	-6.2	106	0.00
86 T	p-Isopropyltoluene	3.572	3.774	-5.7	105	0.00
87 T	1,3-Dichlorobenzene	1.772	1.861	-5.0	108	0.00
88 T	1,4-Dichlorobenzene	1.836	1.849	-0.7	107	0.00
89 T	n-Butylbenzene	3.507	3.673	-4.7	107	0.00
90 T	Hexachloroethane	0.635	0.680	-7.1	108	0.00
91 T	1,2-Dichlorobenzene	1.710	1.818	-6.3	108	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.282	0.264	6.4	90	0.00
93 T	1,2,4-Trichlorobenzene	1.167	1.222	-4.7	110	0.00
94 T	Hexachlorobutadiene	0.542	0.537	0.9	104	0.00
95 T	Naphthalene	3.699	3.750	-1.4	98	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046586.D
Acq On : 10 Jun 2025 09:07
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Jun 11 01:40:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	1.170	1.195	-2.1	106	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046586.D
 Acq On : 10 Jun 2025 09:07
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDCCC050

Quant Time: Jun 11 01:40:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	101	-0.01
2 T	Dichlorodifluoromethane	50.000	50.806	-1.6	110	0.00
3 P	Chloromethane	50.000	49.215	1.6	109	0.00
4 C	Vinyl Chloride	50.000	50.831	-1.7#	108	0.00
5 T	Bromomethane	50.000	46.823	6.4	91	0.00
6 T	Chloroethane	50.000	43.380	13.2	96	0.00
7 T	Trichlorofluoromethane	50.000	47.872	4.3	98	0.00
8 T	Diethyl Ether	50.000	47.456	5.1	99	-0.01
9 T	1,1,2-Trichlorotrifluoroeth	50.000	50.805	-1.6	105	0.00
10 T	Methyl Iodide	50.000	57.012	-14.0	114	0.00
11 T	Tert butyl alcohol	250.000	175.393	29.8#	71	-0.01
12 CM	1,1-Dichloroethene	50.000	50.787	-1.6#	107	0.00
13 T	Acrolein	250.000	218.171	12.7	91	0.00
14 T	Allyl chloride	50.000	47.145	5.7	98	0.00
15 T	Acrylonitrile	250.000	227.796	8.9	90	-0.01
16 T	Acetone	250.000	198.999	20.4	82	0.00
17 T	Carbon Disulfide	50.000	49.803	0.4	104	0.00
18 T	Methyl Acetate	50.000	45.873	8.3	87	-0.01
19 T	Methyl tert-butyl Ether	50.000	50.563	-1.1	100	-0.01
20 T	Methylene Chloride	50.000	48.842	2.3	106	0.00
21 T	trans-1,2-Dichloroethene	50.000	49.518	1.0	108	0.00
22 T	Diisopropyl ether	50.000	52.255	-4.5	103	-0.02
23 T	Vinyl Acetate	250.000	245.925	1.6	96	-0.01
24 P	1,1-Dichloroethane	50.000	50.040	-0.1	103	0.00
25 T	2-Butanone	250.000	213.467	14.6	85	-0.02
26 T	2,2-Dichloropropane	50.000	56.089	-12.2	111	-0.01
27 T	cis-1,2-Dichloroethene	50.000	52.640	-5.3	111	-0.01
28 T	Bromochloromethane	50.000	48.905	2.2	102	-0.01
29 T	Tetrahydrofuran	250.000	215.281	13.9	86	-0.01
30 C	Chloroform	50.000	53.531	-7.1#	110	-0.01
31 T	Cyclohexane	50.000	50.962	-1.9	107	-0.01
32 T	1,1,1-Trichloroethane	50.000	53.292	-6.6	108	0.00
33 S	1,2-Dichloroethane-d4	50.000	42.529	14.9	87	-0.01
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	96	-0.01
35 S	Dibromofluoromethane	50.000	48.920	2.2	94	-0.02
36 T	1,1-Dichloropropene	50.000	51.010	-2.0	107	-0.02
37 T	Ethyl Acetate	50.000	51.130	-2.3	91	-0.01
38 T	Carbon Tetrachloride	50.000	53.694	-7.4	108	-0.01
39 T	Methylcyclohexane	50.000	50.806	-1.6	106	-0.01
40 TM	Benzene	50.000	54.601	-9.2	109	-0.02
41 T	Methacrylonitrile	50.000	51.438	-2.9	98	-0.02
42 TM	1,2-Dichloroethane	50.000	53.402	-6.8	104	-0.01
43 T	Isopropyl Acetate	50.000	48.737	2.5	91	-0.01
44 TM	Trichloroethene	50.000	52.534	-5.1	109	0.00
45 C	1,2-Dichloropropane	50.000	54.858	-9.7#	106	-0.01
46 T	Dibromomethane	50.000	52.699	-5.4	105	0.00
47 T	Bromodichloromethane	50.000	57.103	-14.2	108	0.00
48 T	Methyl methacrylate	50.000	49.326	1.3	91	-0.01

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046586.D
 Acq On : 10 Jun 2025 09:07
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDCCC050

Quant Time: Jun 11 01:40:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	952.914	4.7	89	-0.02
50 S	Toluene-d8	50.000	47.502	5.0	93	0.00
51 T	4-Methyl-2-Pentanone	250.000	239.572	4.2	89	0.00
52 CM	Toluene	50.000	54.605	-9.2#	108	0.00
53 T	t-1,3-Dichloropropene	50.000	57.101	-14.2	108	0.00
54 T	cis-1,3-Dichloropropene	50.000	56.746	-13.5	109	0.00
55 T	1,1,2-Trichloroethane	50.000	55.174	-10.3	106	0.00
56 T	Ethyl methacrylate	50.000	53.621	-7.2	100	0.00
57 T	1,3-Dichloropropane	50.000	53.935	-7.9	105	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	245.588	1.8	92	0.00
59 T	2-Hexanone	250.000	229.299	8.3	84	0.00
60 T	Dibromochloromethane	50.000	56.586	-13.2	108	0.00
61 T	1,2-Dibromoethane	50.000	51.925	-3.8	103	0.00
62 S	4-Bromofluorobenzene	50.000	46.644	6.7	92	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	99	0.00
64 T	Tetrachloroethene	50.000	50.206	-0.4	107	0.00
65 PM	Chlorobenzene	50.000	52.473	-4.9	108	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	56.356	-12.7	110	0.00
67 C	Ethyl Benzene	50.000	53.081	-6.2#	107	0.00
68 T	m/p-Xylenes	100.000	107.686	-7.7	107	0.00
69 T	o-Xylene	50.000	53.823	-7.6	107	0.00
70 T	Styrene	50.000	56.124	-12.2	109	0.00
71 P	Bromoform	50.000	55.623	-11.2	107	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	97	0.00
73 T	Isopropylbenzene	50.000	54.106	-8.2	106	0.00
74 T	N-amyl acetate	50.000	49.214	1.6	92	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	50.980	-2.0	99	0.00
76 T	1,2,3-Trichloropropane	50.000	52.008	-4.0	102	0.00
77 T	Bromobenzene	50.000	55.440	-10.9	112	0.00
78 T	n-propylbenzene	50.000	53.299	-6.6	105	0.00
79 T	2-Chlorotoluene	50.000	52.688	-5.4	106	0.00
80 T	1,3,5-Trimethylbenzene	50.000	53.827	-7.7	106	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	52.271	-4.5	101	0.00
82 T	4-Chlorotoluene	50.000	52.538	-5.1	106	0.00
83 T	tert-Butylbenzene	50.000	54.234	-8.5	107	0.00
84 T	1,2,4-Trimethylbenzene	50.000	52.794	-5.6	105	0.00
85 T	sec-Butylbenzene	50.000	53.081	-6.2	106	0.00
86 T	p-Isopropyltoluene	50.000	52.834	-5.7	105	0.00
87 T	1,3-Dichlorobenzene	50.000	52.534	-5.1	108	0.00
88 T	1,4-Dichlorobenzene	50.000	50.367	-0.7	107	0.00
89 T	n-Butylbenzene	50.000	52.356	-4.7	107	0.00
90 T	Hexachloroethane	50.000	53.532	-7.1	108	0.00
91 T	1,2-Dichlorobenzene	50.000	53.144	-6.3	108	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	46.795	6.4	90	0.00
93 T	1,2,4-Trichlorobenzene	50.000	52.365	-4.7	110	0.00
94 T	Hexachlorobutadiene	50.000	49.518	1.0	104	0.00
95 T	Naphthalene	50.000	50.687	-1.4	98	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046586.D
Acq On : 10 Jun 2025 09:07
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Jun 11 01:40:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T	1,2,3-Trichlorobenzene	50.000	51.096	-2.2	106	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6




QC SAMPLE DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046516.D
Acq On : 06 Jun 2025 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Title : SW846 8260
Last Update : Fri Jun 06 16:56:12 2025

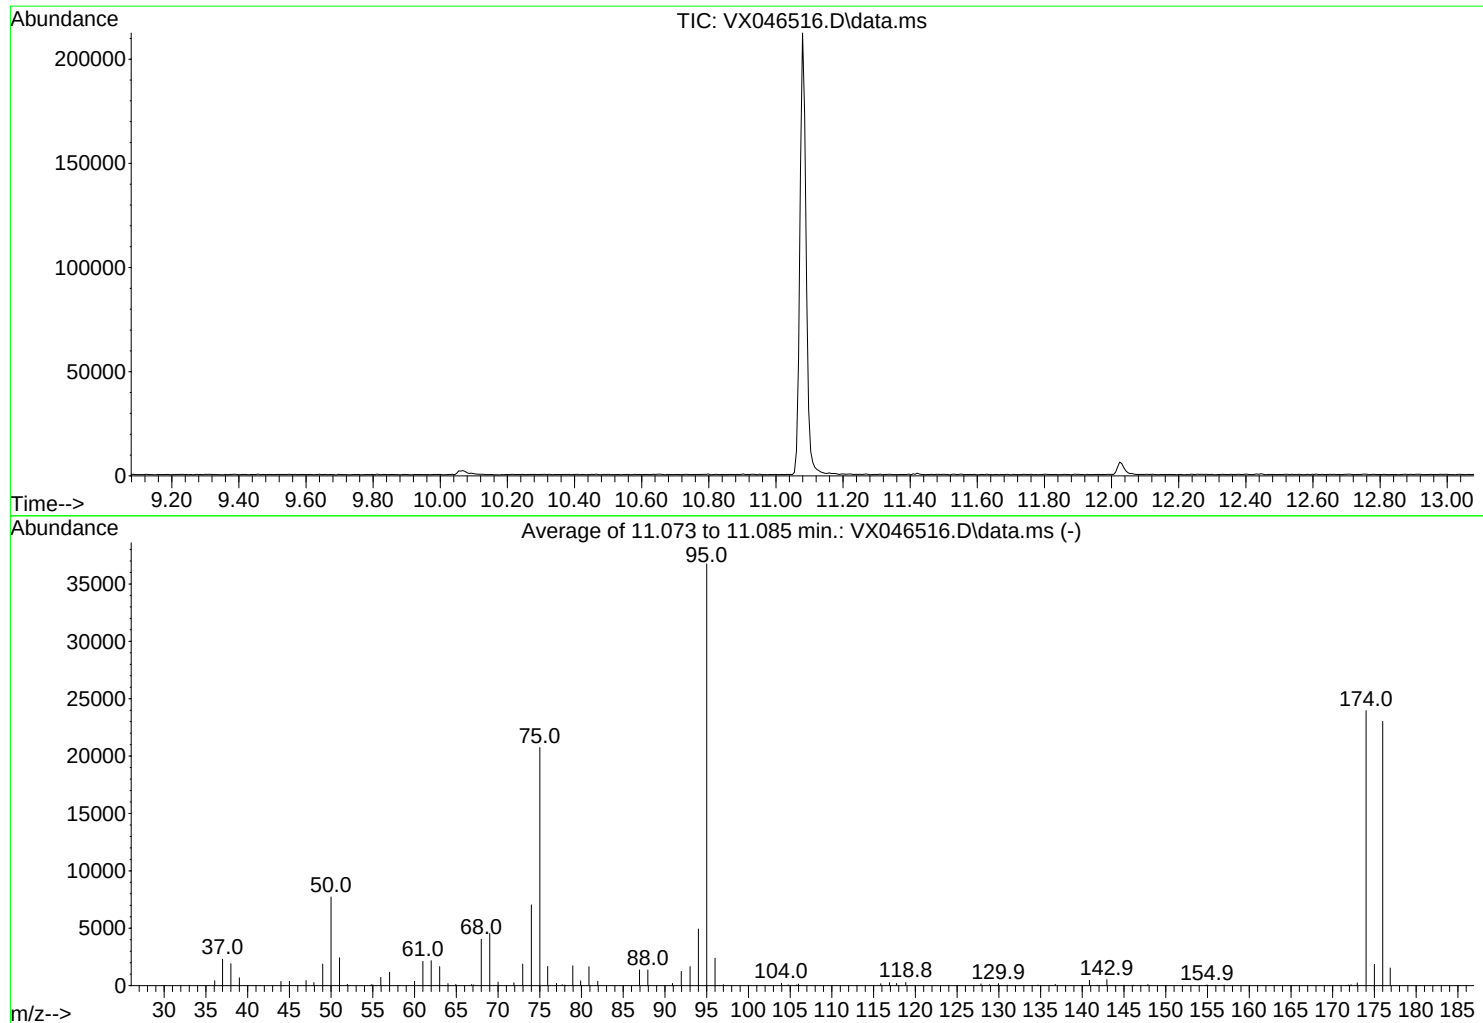

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632



Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	7727	PASS
75	95	30	60	56.5	20747	PASS
95	95	100	100	100.0	36752	PASS
96	95	5	9	6.5	2397	PASS
173	174	0.00	2	1.0	238	PASS
174	95	50	100	65.2	23963	PASS
175	174	5	9	7.7	1850	PASS
176	174	95	101	96.1	23028	PASS
177	176	5	9	6.6	1530	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046585.D
Acq On : 10 Jun 2025 08:36
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Title : SW846 8260
Last Update : Fri Jun 06 16:56:12 2025

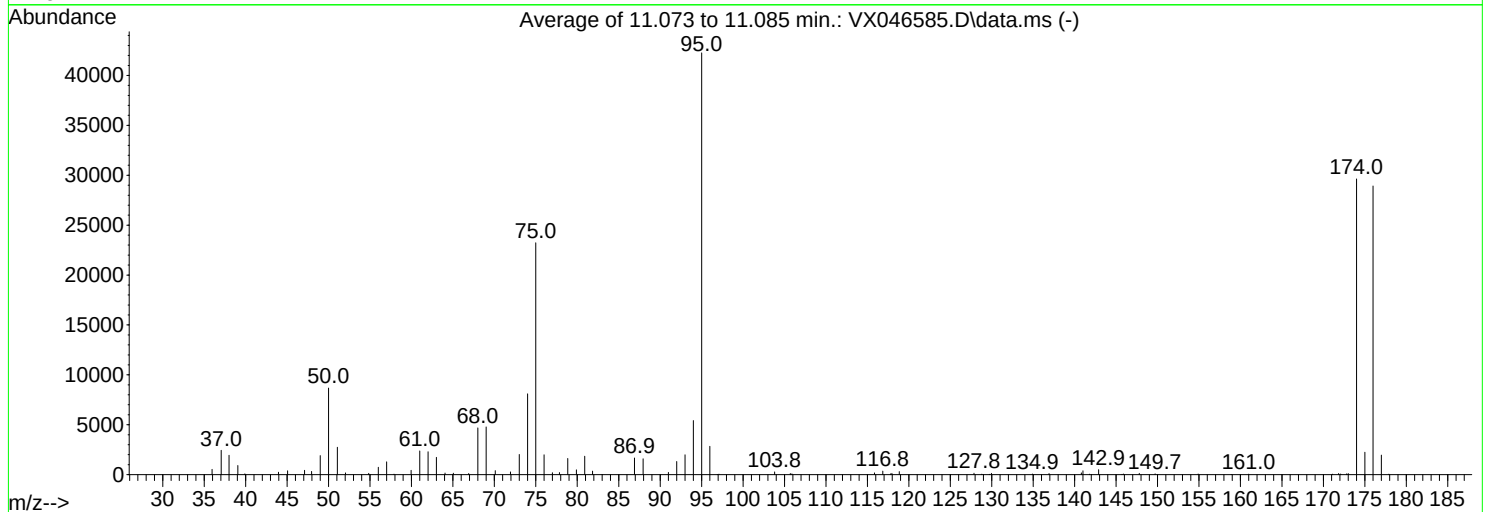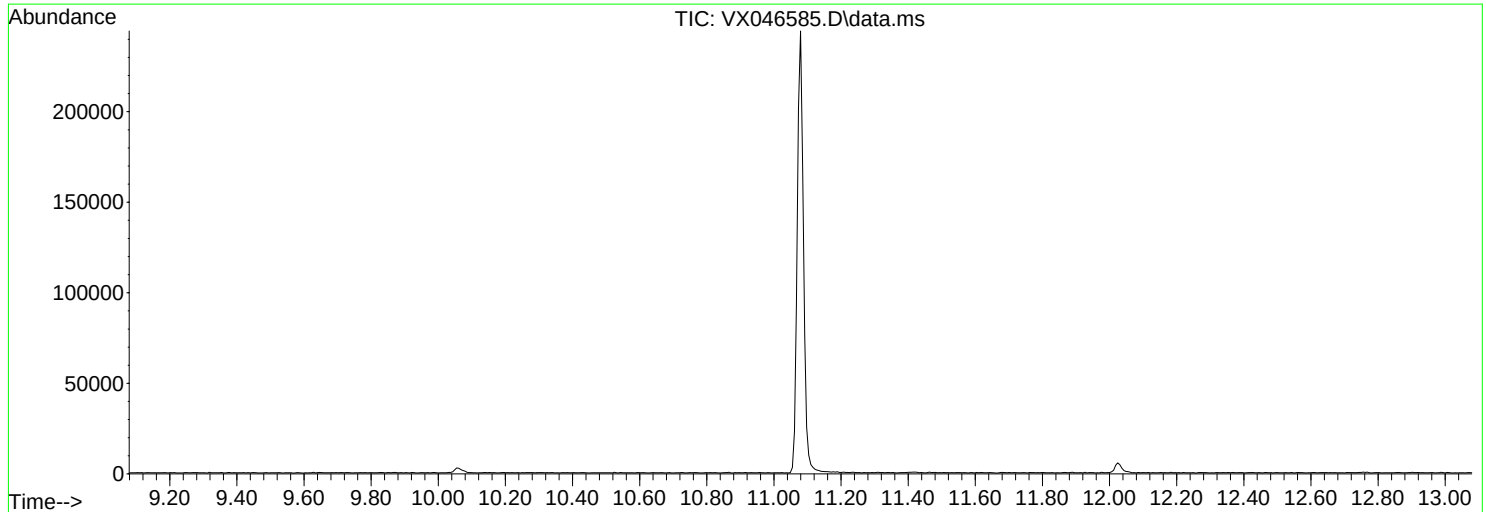

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	8668	PASS
75	95	30	60	55.0	23232	PASS
95	95	100	100	100.0	42264	PASS
96	95	5	9	6.7	2835	PASS
173	174	0.00	2	0.4	107	PASS
174	95	50	100	70.1	29635	PASS
175	174	5	9	7.6	2246	PASS
176	174	95	101	97.6	28920	PASS
177	176	5	9	6.8	1965	PASS

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	VX0610WBL01	SDG No.:	Q2234
Lab Sample ID:	VX0610WBL01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046588.D	1		06/10/25 09:57	VX061025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	50.1		70 (74) - 130 (125)	100%	SPK: 50
1868-53-7	Dibromofluoromethane	50.1		70 (75) - 130 (124)	100%	SPK: 50
2037-26-5	Toluene-d8	54.3		70 (86) - 130 (113)	109%	SPK: 50
460-00-4	4-Bromofluorobenzene	54.8		70 (77) - 130 (121)	110%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	106000	5.562			
540-36-3	1,4-Difluorobenzene	212000	6.769			
3114-55-4	Chlorobenzene-d5	217000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	104000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046588.D
Acq On : 10 Jun 2025 09:57
Operator : JC/MD
Sample : VX0610WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0610WBL01

Quant Time: Jun 11 01:42:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	106110	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	211553	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	217338	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	104374	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	94499	50.058	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	100.120%
35) Dibromofluoromethane	5.397	113	77970	50.117	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.240%
50) Toluene-d8	8.647	98	278481	54.294	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	108.580%
62) 4-Bromofluorobenzene	11.079	95	116202	54.757	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	109.520%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046588.D
Acq On : 10 Jun 2025 09:57
Operator : JC/MD
Sample : VX0610WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0610WBL01

Quant Time: Jun 11 01:42:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

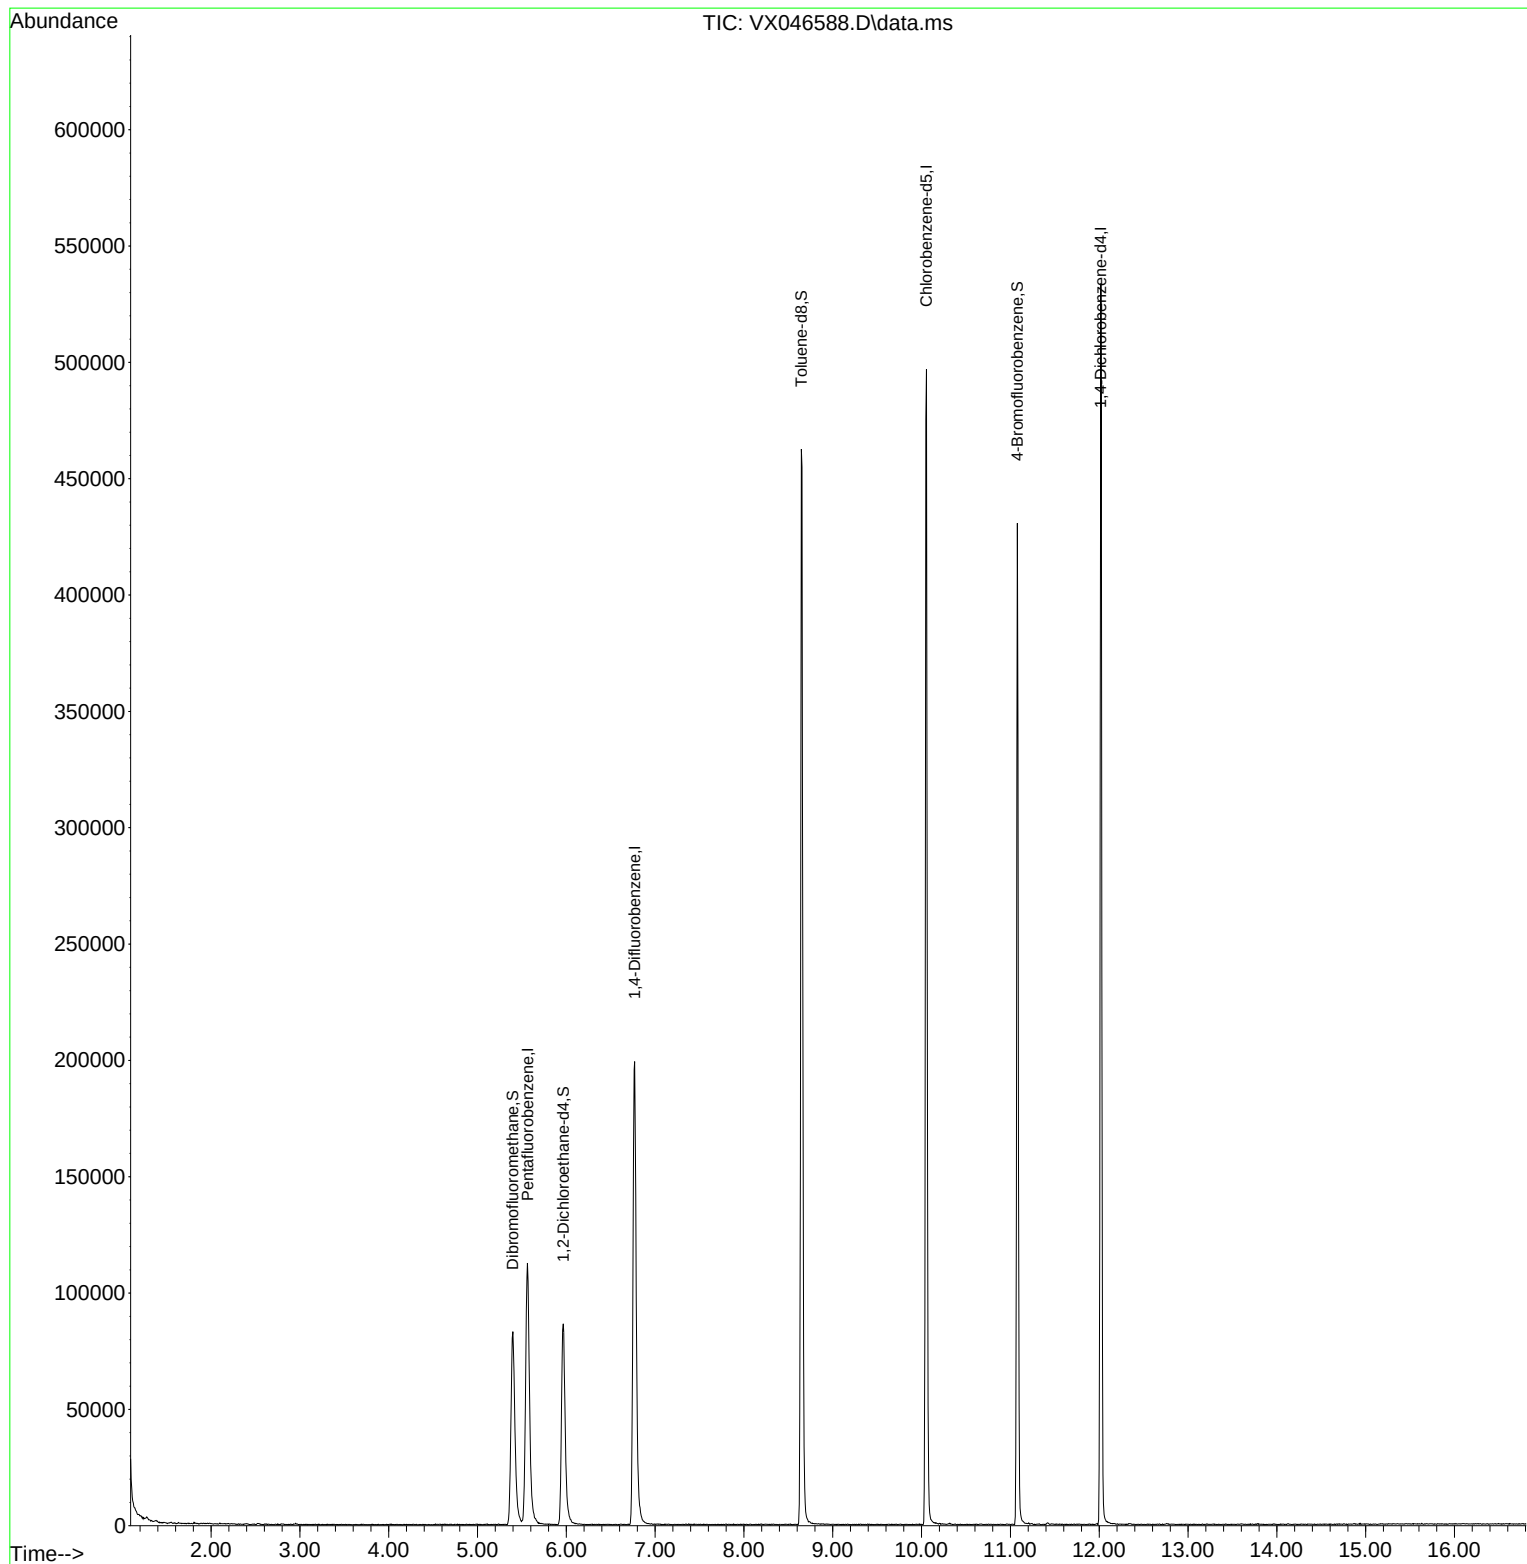

#1
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.562 min Scan# 71

Delta R.T. -0.006 min

Lab File: VX046588.D

Acq: 10 Jun 2025 09:57

Instrument :

MSVOA_X

ClientSampleId :





VX0610WBL01

Tgt Ion:168 Resp: 106110

Ion Ratio Lower Upper

168 100

99 71.7 54.9 82.3

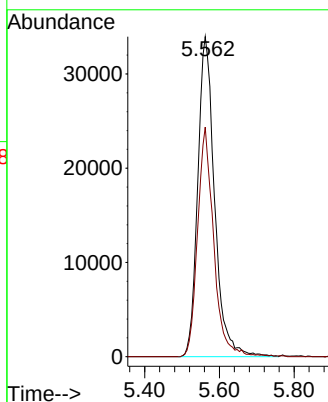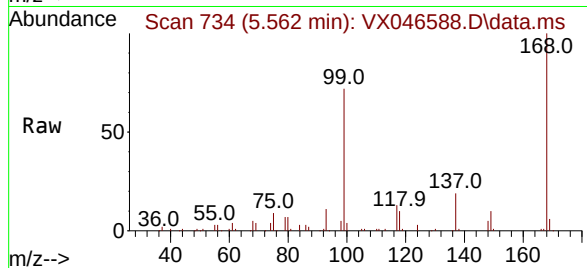

#33

1,2-Dichloroethane-d4

Concen: 50.058 ug/l

RT: 5.964 min Scan# 800

Delta R.T. -0.006 min

Lab File: VX046588.D




Acq: 10 Jun 2025 09:57


Tgt Ion: 65 Resp: 94499

Ion Ratio Lower Upper

65 100

67 51.0 0.0 99.0


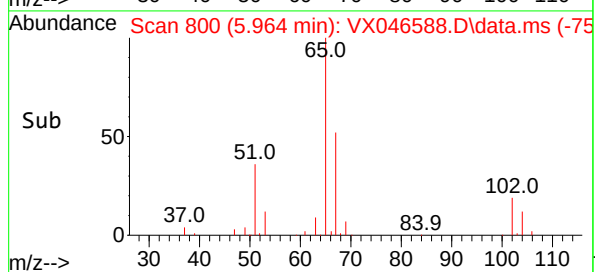
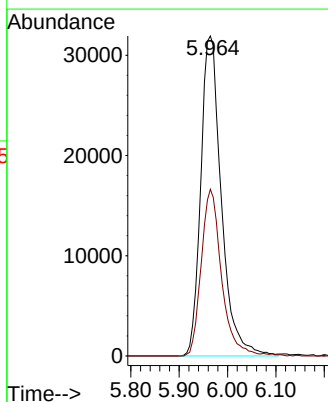
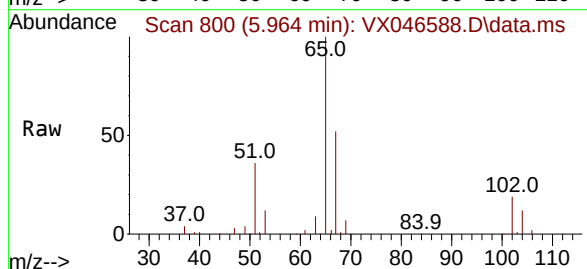


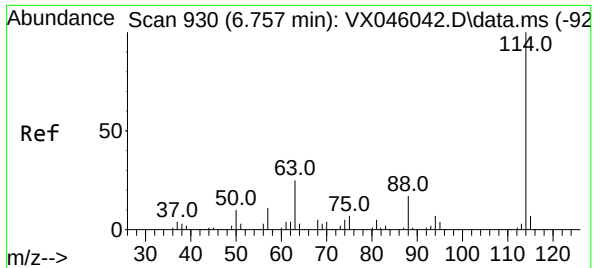

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX046588.D
Acq: 10 Jun 2025 09:57




Instrument :
MSVOA_X
ClientSampleId :
VX0610WBL01


Tgt Ion:114 Resp: 211553
Ion Ratio Lower Upper
114 100
63 23.0 0.0 49.2
88 17.1 0.0 33.6

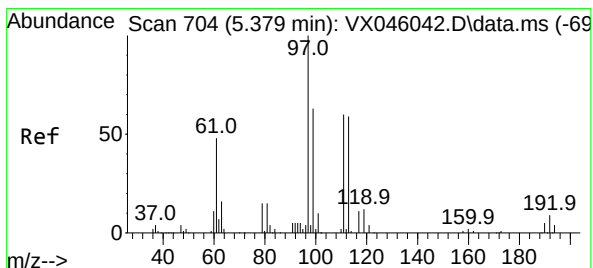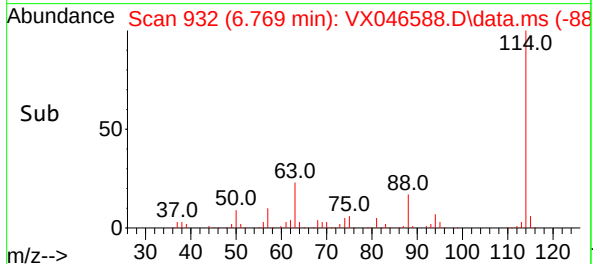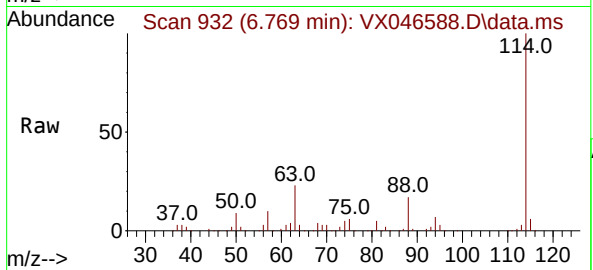

#35
Dibromofluoromethane
Concen: 50.117 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.006 min
Lab File: VX046588.D
Acq: 10 Jun 2025 09:57

Tgt Ion:113 Resp: 77970
Ion Ratio Lower Upper
113 100
111 103.7 83.1 124.7
192 17.6 13.3 19.9

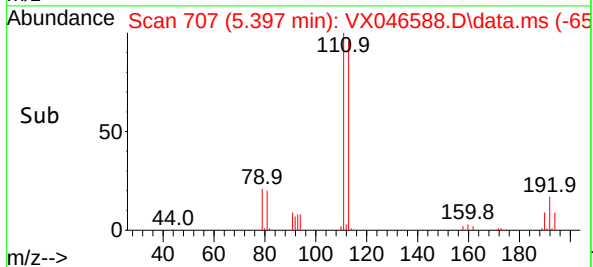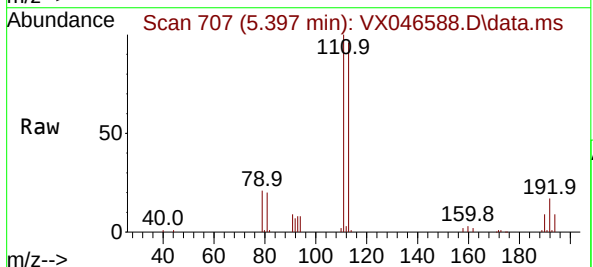



#50

Toluene-d8

Concen: 54.294 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX046588.D

Acq: 10 Jun 2025 09:57

Instrument :

MSVOA_X

ClientSampleId :





VX0610WBL01

Tgt Ion: 98 Resp: 278481

Ion Ratio Lower Upper

98 100

100 65.6 53.5 80.3

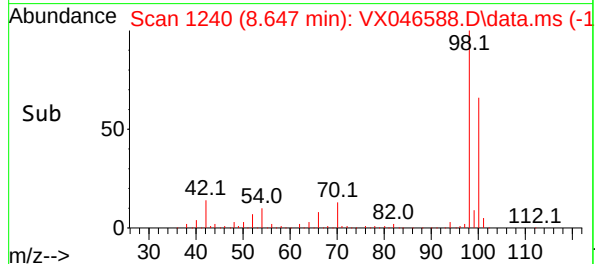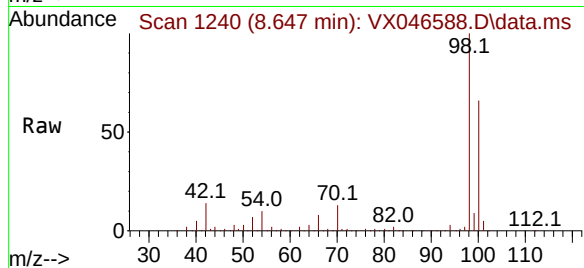

#62

4-Bromofluorobenzene

Concen: 54.757 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046588.D

Acq: 10 Jun 2025 09:57




Tgt Ion: 95 Resp: 116202


Ion Ratio Lower Upper

95 100

174 70.0 0.0 135.8

176 66.7 0.0 131.4

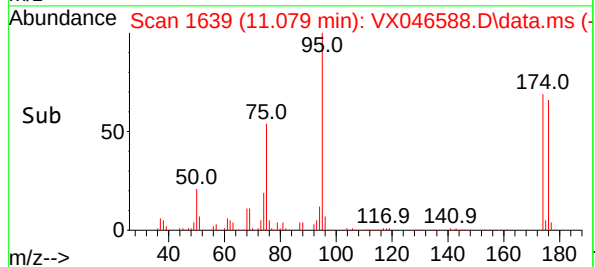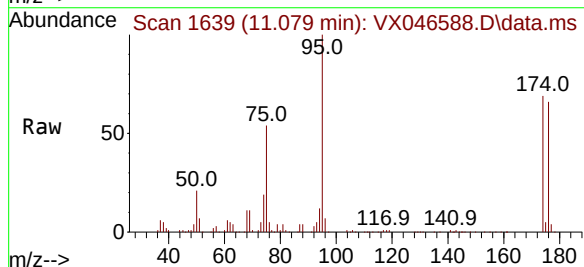



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX046588.D

Acq: 10 Jun 2025 09:57

Instrument :

MSVOA_X

ClientSampleId :

VX0610WBL01





Tgt Ion:117 Resp: 217338

Ion Ratio Lower Upper

117 100

82 57.1 50.6 76.0

119 32.8 25.8 38.6

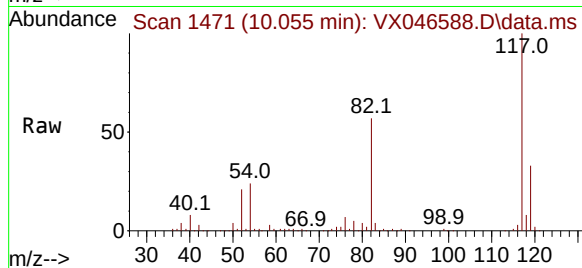

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX046588.D

Acq: 10 Jun 2025 09:57




Tgt Ion:152 Resp: 104374

Ion Ratio Lower Upper

152 100

115 65.3 46.9 140.7

150 157.8 0.0 351.0

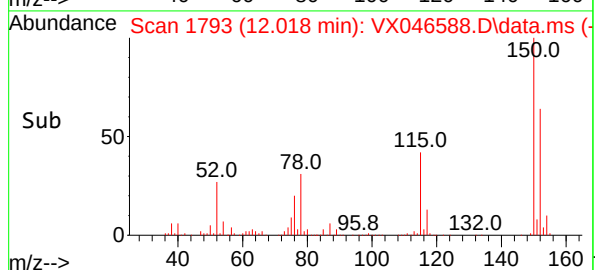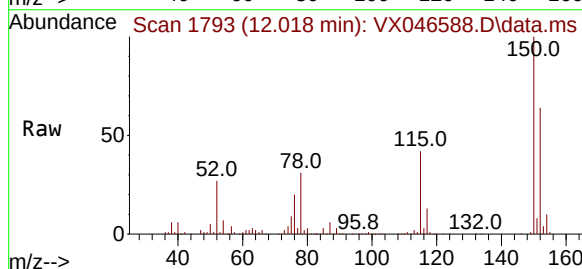

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	VX0610WBS01	SDG No.:	Q2234
Lab Sample ID:	VX0610WBS01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5	Units:	mL
Soil Aliquot Vol:			uL
GC Column:	DB-624UI	ID :	0.18
Prep Method :		Level :	LOW

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046589.D	1		06/10/25 10:18	VX061025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	18.7		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	19.2		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	20.4		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	20.6		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	20.6		0.20	1.00	ug/L
71-43-2	Benzene	21.0		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	20.8		0.22	1.00	ug/L
79-01-6	Trichloroethene	20.1		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	21.6		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	20.3		0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	47.4		70 (74) - 130 (125)	95%	SPK: 50
1868-53-7	Dibromofluoromethane	53.0		70 (75) - 130 (124)	106%	SPK: 50
2037-26-5	Toluene-d8	51.5		70 (86) - 130 (113)	103%	SPK: 50
460-00-4	4-Bromofluorobenzene	53.1		70 (77) - 130 (121)	106%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	84100	5.562			
540-36-3	1,4-Difluorobenzene	144000	6.769			
3114-55-4	Chlorobenzene-d5	131000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	68200	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046589.D
 Acq On : 10 Jun 2025 10:18
 Operator : JC/MD
 Sample : VX0610WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0610WBS01

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/11/2025
 Supervised By : Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:42:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	84052	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	143506	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	131426	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68222	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	70828	47.365	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 94.720%			
35) Dibromofluoromethane	5.397	113	55906	52.974	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 105.940%			
50) Toluene-d8	8.647	98	179208	51.507	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 103.020%			
62) 4-Bromofluorobenzene	11.079	95	76446	53.104	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 106.200%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.185	85	21364	18.308	ug/l	100
3) Chloromethane	1.307	50	19522	18.380	ug/l	96
4) Vinyl Chloride	1.386	62	19755	18.658	ug/l	95
5) Bromomethane	1.630	94	12259	19.072	ug/l	100
6) Chloroethane	1.703	64	11361	16.538	ug/l #	87
7) Trichlorofluoromethane	1.904	101	31526	17.996	ug/l	97
8) Diethyl Ether	2.148	74	10811	17.466	ug/l	92
9) 1,1,2-Trichlorotrifluo...	2.343	101	21056	19.078	ug/l	95
10) Methyl Iodide	2.465	142	24545	20.515	ug/l	96
11) Tert butyl alcohol	2.959	59	11873	71.554	ug/l	97
12) 1,1-Dichloroethene	2.337	96	19187	19.227	ug/l	85
13) Acrolein	2.251	56	15557	98.221	ug/l	100
14) Allyl chloride	2.684	41	34982	17.850	ug/l	93
15) Acrylonitrile	3.075	53	58538	93.306	ug/l	98
16) Acetone	2.392	43	44483	78.955	ug/l	93
17) Carbon Disulfide	2.526	76	39330	18.689	ug/l	99
18) Methyl Acetate	2.715	43	32974	18.512	ug/l	97
19) Methyl tert-butyl Ether	3.123	73	70651	20.234	ug/l	98
20) Methylene Chloride	2.806	84	22844	19.042	ug/l	92
21) trans-1,2-Dichloroethene	3.105	96	20405	19.322	ug/l	93
22) Diisopropyl ether	3.776	45	81863	21.187	ug/l #	82
23) Vinyl Acetate	3.733	43	295594	99.089	ug/l	100
24) 1,1-Dichloroethane	3.629	63	43840	20.358	ug/l	98
25) 2-Butanone	4.568	43	72292	86.843	ug/l	98
26) 2,2-Dichloropropane	4.489	77	32929	20.598	ug/l	98
27) cis-1,2-Dichloroethene	4.507	96	26773	20.594	ug/l	95
28) Bromochloromethane	4.916	49	20852	20.302	ug/l	99
29) Tetrahydrofuran	5.019	42	45988	87.477	ug/l	100
30) Chloroform	5.105	83	47450	21.029	ug/l	99
31) Cyclohexane	5.483	56	33142	19.064	ug/l	89
32) 1,1,1-Trichloroethane	5.397	97	39813	20.627	ug/l	97
36) 1,1-Dichloropropene	5.702	75	29838	19.793	ug/l	99
37) Ethyl Acetate	4.733	43	29233	19.869	ug/l	98
38) Carbon Tetrachloride	5.690	117	34504	20.435	ug/l	99
39) Methylcyclohexane	7.385	83	34288	19.270	ug/l	99
40) Benzene	6.050	78	88942	20.958	ug/l	95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046589.D
 Acq On : 10 Jun 2025 10:18
 Operator : JC/MD
 Sample : VX0610WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0610WBS01

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/11/2025
 Supervised By : Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:42:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.928	41	16637	18.209	ug/l	93
42) 1,2-Dichloroethane	6.098	62	36740	20.810	ug/l	99
43) Isopropyl Acetate	6.348	43	49580	19.330	ug/l	100
44) Trichloroethene	7.129	130	21670	20.097	ug/l	99
45) 1,2-Dichloropropane	7.433	63	23739	21.672	ug/l	99
46) Dibromomethane	7.586	93	17188	20.858	ug/l	98
47) Bromodichloromethane	7.824	83	37295	22.011	ug/l	95
48) Methyl methacrylate	7.696	41	25179	19.079	ug/l	95
49) 1,4-Dioxane	7.659	88	6473	366.785	ug/l #	90
51) 4-Methyl-2-Pentanone	8.573	43	160847	98.684	ug/l	100
52) Toluene	8.720	92	55219	21.179	ug/l	99
53) t-1,3-Dichloropropene	8.982	75	31694	20.862	ug/l	96
54) cis-1,3-Dichloropropene	8.366	75	35775	21.180	ug/l	92
55) 1,1,2-Trichloroethane	9.153	97	22559	21.553	ug/l	95
56) Ethyl methacrylate	9.116	69	32654	20.274	ug/l	95
57) 1,3-Dichloropropane	9.311	76	39081	21.129	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.244	63	81610	93.023	ug/l	98
59) 2-Hexanone	9.433	43	111008	94.963	ug/l	99
60) Dibromochloromethane	9.518	129	27795	22.577	ug/l	97
61) 1,2-Dibromoethane	9.610	107	22620	20.739	ug/l	98
64) Tetrachloroethene	9.275	164	17851	20.312	ug/l	94
65) Chlorobenzene	10.079	112	62603	20.253	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.159	131	22301	21.351	ug/l	99
67) Ethyl Benzene	10.195	91	109725	20.334	ug/l	98
68) m/p-Xylenes	10.299	106	81525	41.649	ug/l	98
69) o-Xylene	10.640	106	40019	21.137	ug/l	98
70) Styrene	10.652	104	69335	21.393	ug/l	99
71) Bromoform	10.799	173	16884	21.200	ug/l #	99
73) Isopropylbenzene	10.963	105	108394	20.212	ug/l	99
74) N-amyl acetate	10.841	43	43808	18.549	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.213	83	34119	19.876	ug/l	98
76) 1,2,3-Trichloropropane	11.238	75	27186m	18.813	ug/l	
77) Bromobenzene	11.195	156	26036	20.916	ug/l	96
78) n-propylbenzene	11.305	91	129891	20.011	ug/l	100
79) 2-Chlorotoluene	11.366	91	78249	19.991	ug/l	98
80) 1,3,5-Trimethylbenzene	11.451	105	91704	20.520	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.018	75	8748	17.463	ug/l	98
82) 4-Chlorotoluene	11.451	91	93212	20.090	ug/l	97
83) tert-Butylbenzene	11.713	119	92923	20.426	ug/l	98
84) 1,2,4-Trimethylbenzene	11.750	105	94205	20.838	ug/l	99
85) sec-Butylbenzene	11.890	105	119911	20.513	ug/l	100
86) p-Isopropyltoluene	12.006	119	98241	20.160	ug/l	98
87) 1,3-Dichlorobenzene	11.969	146	48297	19.981	ug/l	99
88) 1,4-Dichlorobenzene	12.036	146	49276	19.673	ug/l	98
89) n-Butylbenzene	12.329	91	95315	19.917	ug/l	99
90) Hexachloroethane	12.536	117	16834	19.436	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	48730	20.885	ug/l	98
92) 1,2-Dibromo-3-Chloropr...	12.939	75	6919	18.000	ug/l	95
93) 1,2,4-Trichlorobenzene	13.585	180	30939	19.438	ug/l	100
94) Hexachlorobutadiene	13.719	225	14378	19.438	ug/l	98
95) Naphthalene	13.774	128	98907	19.595	ug/l	99
96) 1,2,3-Trichlorobenzene	13.957	180	30702	19.237	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046589.D
Acq On : 10 Jun 2025 10:18
Operator : JC/MD
Sample : VX0610WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0610WBS01

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:42:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046589.D
Acq On : 10 Jun 2025 10:18
Operator : JC/MD
Sample : VX0610WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0610WBS01

Manual Integrations APPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:42:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

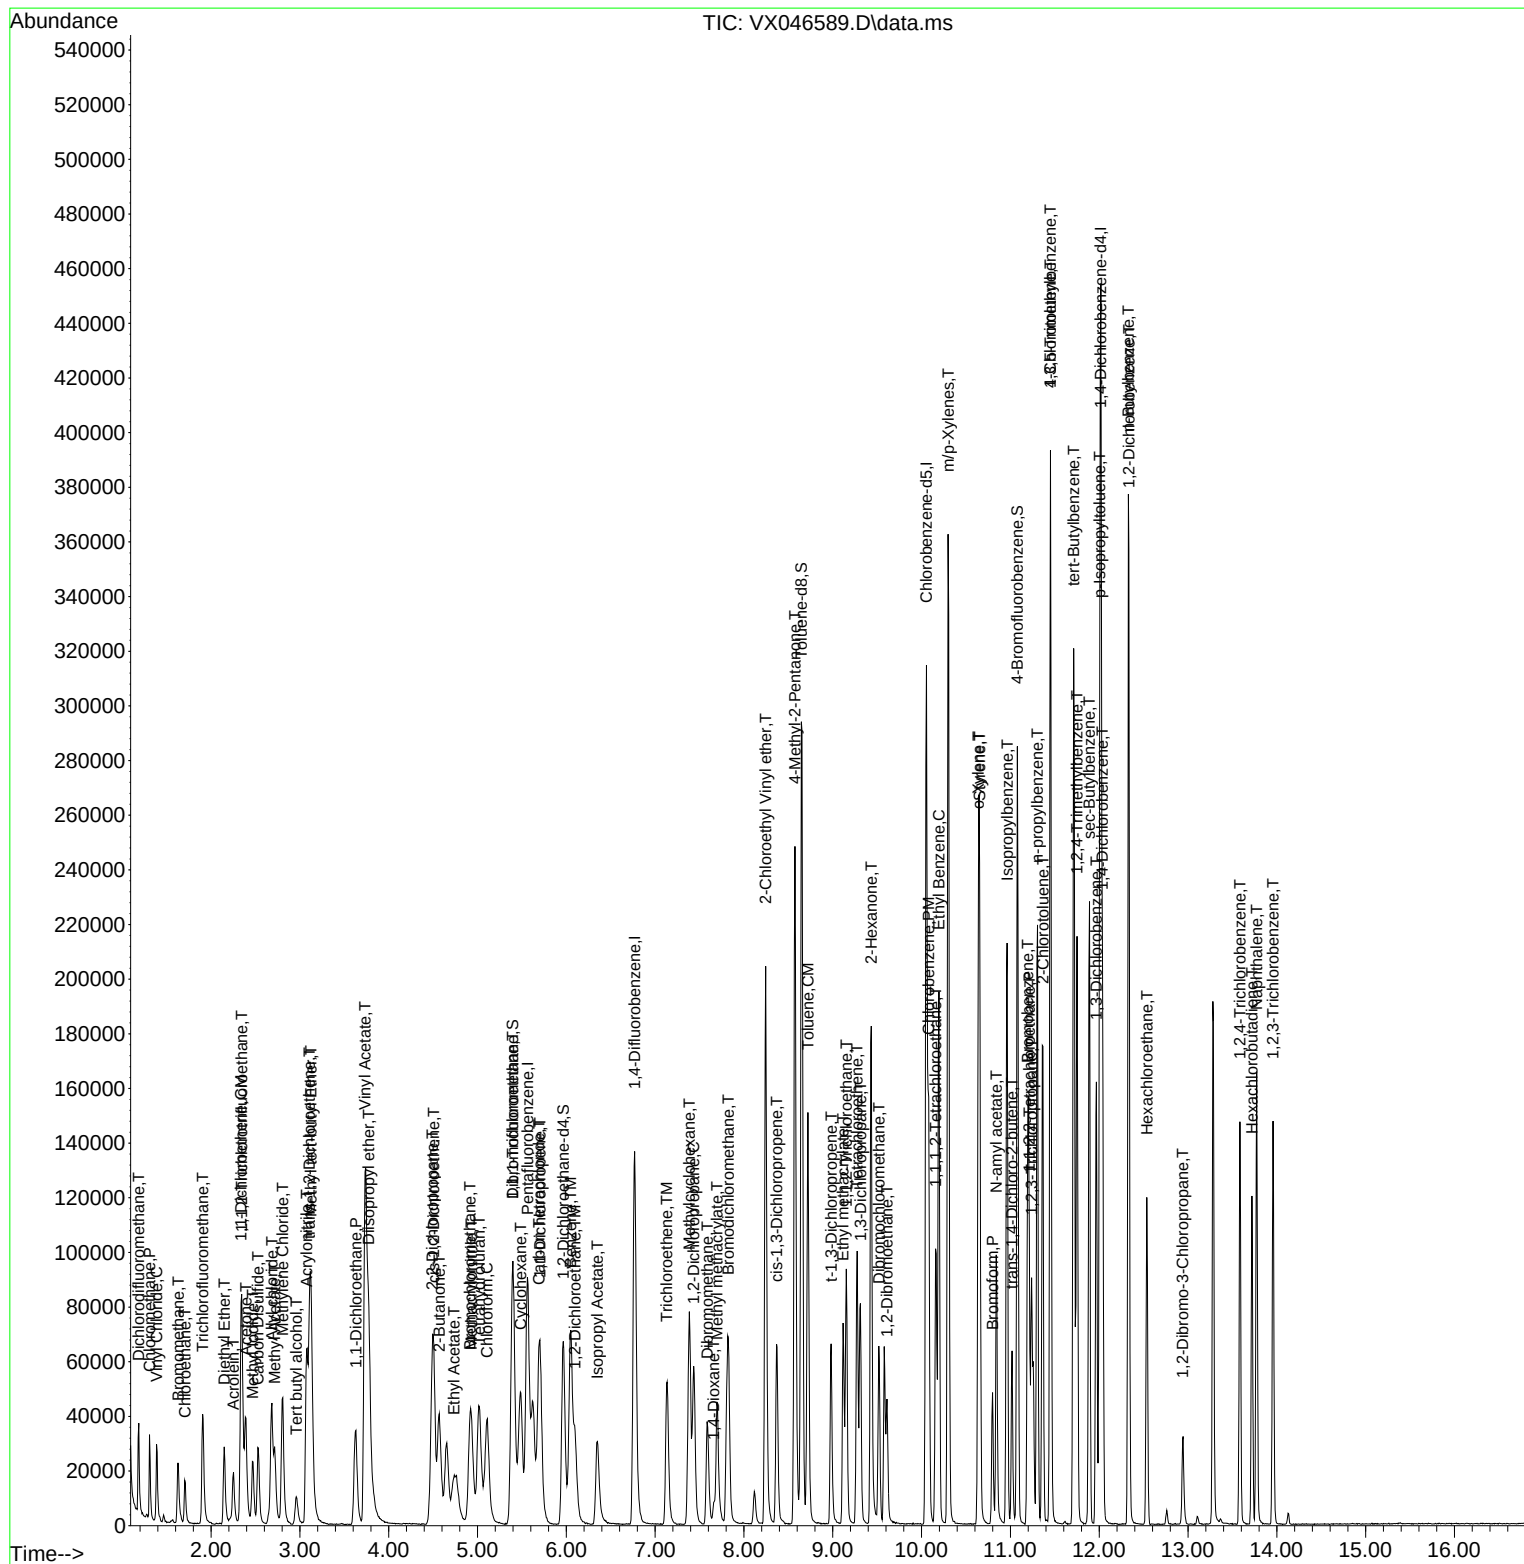

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	VX0610WBSD01	SDG No.:	Q2234
Lab Sample ID:	VX0610WBSD01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5	Units:	mL
Soil Aliquot Vol:			uL
GC Column:	DB-624UI	ID :	0.18
Prep Method :		Level :	LOW

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046590.D	1		06/10/25 10:44	VX061025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	19.1		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	19.8		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	20.7		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	20.5		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	20.9		0.20	1.00	ug/L
71-43-2	Benzene	20.6		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	20.6		0.22	1.00	ug/L
79-01-6	Trichloroethene	19.8		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	22.3		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	19.8		0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	49.3		70 (74) - 130 (125)	99%	SPK: 50
1868-53-7	Dibromofluoromethane	52.3		70 (75) - 130 (124)	105%	SPK: 50
2037-26-5	Toluene-d8	51.0		70 (86) - 130 (113)	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	52.3		70 (77) - 130 (121)	105%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	79700	5.562			
540-36-3	1,4-Difluorobenzene	139000	6.769			
3114-55-4	Chlorobenzene-d5	126000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	65300	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046590.D
 Acq On : 10 Jun 2025 10:44
 Operator : JC/MD
 Sample : VX0610WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0610WBSD01

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/11/2025
 Supervised By : Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:43:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	79698	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	139229	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	126313	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	65284	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	69863	49.272	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	98.540%		
35) Dibromofluoromethane	5.391	113	53548	52.299	ug/l	-0.01
Spiked Amount 50.000	Range 75 - 124		Recovery =	104.600%		
50) Toluene-d8	8.647	98	172301	51.043	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	102.080%		
62) 4-Bromofluorobenzene	11.079	95	73113	52.349	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	104.700%		
Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.184	85	19714	17.817	ug/l	97
3) Chloromethane	1.306	50	17982	17.855	ug/l	94
4) Vinyl Chloride	1.386	62	19173	19.098	ug/l	96
5) Bromomethane	1.623	94	12029	19.736	ug/l	95
6) Chloroethane	1.703	64	11655	17.893	ug/l	96
7) Trichlorofluoromethane	1.904	101	32041	19.289	ug/l	97
8) Diethyl Ether	2.148	74	11524	19.635	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.343	101	20490	19.579	ug/l	95
10) Methyl Iodide	2.465	142	24020	21.173	ug/l	100
11) Tert butyl alcohol	2.959	59	12773	81.183	ug/l	97
12) 1,1-Dichloroethene	2.337	96	18698	19.761	ug/l	90
13) Acrolein	2.251	56	18334	114.790	ug/l	99
14) Allyl chloride	2.678	41	36552	19.670	ug/l	94
15) Acrylonitrile	3.074	53	59520	100.054	ug/l	99
16) Acetone	2.385	43	49623	92.079	ug/l	94
17) Carbon Disulfide	2.526	76	38042	19.061	ug/l	96
18) Methyl Acetate	2.715	43	34953	20.695	ug/l	98
19) Methyl tert-butyl Ether	3.123	73	71303	21.536	ug/l	97
20) Methylene Chloride	2.800	84	22898	20.130	ug/l	100
21) trans-1,2-Dichloroethene	3.105	96	19750	19.723	ug/l	97
22) Diisopropyl ether	3.769	45	79532	21.708	ug/l #	68
23) Vinyl Acetate	3.733	43	295435	104.446	ug/l	100
24) 1,1-Dichloroethane	3.623	63	42302	20.717	ug/l	99
25) 2-Butanone	4.562	43	73687	93.355	ug/l	100
26) 2,2-Dichloropropane	4.495	77	31719	20.925	ug/l	100
27) cis-1,2-Dichloroethene	4.501	96	25251	20.484	ug/l	97
28) Bromochloromethane	4.903	49	20382	20.928	ug/l	100
29) Tetrahydrofuran	5.013	42	46579	93.442	ug/l	99
30) Chloroform	5.104	83	46110	21.552	ug/l	96
31) Cyclohexane	5.476	56	33496	20.320	ug/l	97
32) 1,1,1-Trichloroethane	5.391	97	38162	20.852	ug/l	97
36) 1,1-Dichloropropene	5.702	75	26610	18.194	ug/l	97
37) Ethyl Acetate	4.720	43	29636	20.762	ug/l	99
38) Carbon Tetrachloride	5.690	117	32421	19.791	ug/l	97
39) Methylcyclohexane	7.385	83	33599	19.463	ug/l	98
40) Benzene	6.049	78	84785	20.592	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
 Data File : VX046590.D
 Acq On : 10 Jun 2025 10:44
 Operator : JC/MD
 Sample : VX0610WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0610WBSD01

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/11/2025
 Supervised By : Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:43:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.934	41	17305	19.522	ug/l	94
42) 1,2-Dichloroethane	6.092	62	35332	20.627	ug/l	97
43) Isopropyl Acetate	6.342	43	49240	19.787	ug/l	99
44) Trichloroethene	7.128	130	20662	19.751	ug/l	97
45) 1,2-Dichloropropane	7.433	63	22717	21.376	ug/l	100
46) Dibromomethane	7.586	93	16680	20.863	ug/l	97
47) Bromodichloromethane	7.824	83	36402	22.144	ug/l	100
48) Methyl methacrylate	7.695	41	25589	19.986	ug/l	94
49) 1,4-Dioxane	7.659	88	6531	381.440	ug/l	98
51) 4-Methyl-2-Pentanone	8.573	43	160533	101.517	ug/l	100
52) Toluene	8.720	92	53830	21.281	ug/l	98
53) t-1,3-Dichloropropene	8.982	75	31270	21.215	ug/l	98
54) cis-1,3-Dichloropropene	8.366	75	35060	21.394	ug/l	92
55) 1,1,2-Trichloroethane	9.153	97	22637	22.292	ug/l	98
56) Ethyl methacrylate	9.116	69	33471	21.419	ug/l	95
57) 1,3-Dichloropropane	9.311	76	39409	21.961	ug/l	97
58) 2-Chloroethyl Vinyl ether	8.244	63	80781	94.906	ug/l	99
59) 2-Hexanone	9.427	43	109874	96.880	ug/l	98
60) Dibromochloromethane	9.518	129	26619	22.286	ug/l	97
61) 1,2-Dibromoethane	9.610	107	22947	21.686	ug/l	99
64) Tetrachloroethene	9.274	164	16706	19.779	ug/l	97
65) Chlorobenzene	10.079	112	60350	20.315	ug/l	98
66) 1,1,1,2-Tetrachloroethane	10.165	131	22060	21.975	ug/l	99
67) Ethyl Benzene	10.195	91	106184	20.474	ug/l	98
68) m/p-Xylenes	10.299	106	79852	42.445	ug/l	99
69) o-Xylene	10.640	106	38136	20.958	ug/l	100
70) Styrene	10.652	104	67308	21.609	ug/l	98
71) Bromoform	10.799	173	16667	21.775	ug/l #	96
73) Isopropylbenzene	10.963	105	105188	20.497	ug/l	99
74) N-amyl acetate	10.841	43	43899	19.424	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	33998	20.697	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	27348m	19.777	ug/l	
77) Bromobenzene	11.195	156	25071	21.047	ug/l	95
78) n-propylbenzene	11.305	91	123754	19.923	ug/l	99
79) 2-Chlorotoluene	11.359	91	75334	20.112	ug/l	100
80) 1,3,5-Trimethylbenzene	11.451	105	88592	20.716	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.018	75	9083	18.948	ug/l	96
82) 4-Chlorotoluene	11.451	91	88877	20.018	ug/l	98
83) tert-Butylbenzene	11.713	119	89858	20.641	ug/l	96
84) 1,2,4-Trimethylbenzene	11.750	105	88738	20.512	ug/l	99
85) sec-Butylbenzene	11.890	105	113499	20.290	ug/l	100
86) p-Isopropyltoluene	12.006	119	94330	20.228	ug/l	99
87) 1,3-Dichlorobenzene	11.969	146	47031	20.333	ug/l	99
88) 1,4-Dichlorobenzene	12.036	146	48118	20.076	ug/l	98
89) n-Butylbenzene	12.329	91	91794	20.045	ug/l	99
90) Hexachloroethane	12.536	117	16304	19.671	ug/l	99
91) 1,2-Dichlorobenzene	12.335	146	46557	20.852	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.938	75	6753	18.358	ug/l	90
93) 1,2,4-Trichlorobenzene	13.585	180	30842	20.249	ug/l	97
94) Hexachlorobutadiene	13.725	225	13499	19.071	ug/l	96
95) Naphthalene	13.774	128	95309	19.732	ug/l	100
96) 1,2,3-Trichlorobenzene	13.963	180	29998	19.642	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046590.D
Acq On : 10 Jun 2025 10:44
Operator : JC/MD
Sample : VX0610WBSD01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0610WBSD01

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:43:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061025\
Data File : VX046590.D
Acq On : 10 Jun 2025 10:44
Operator : JC/MD
Sample : VX0610WBSD01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0610WBSD01

Manual Integrations APPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 11 01:43:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

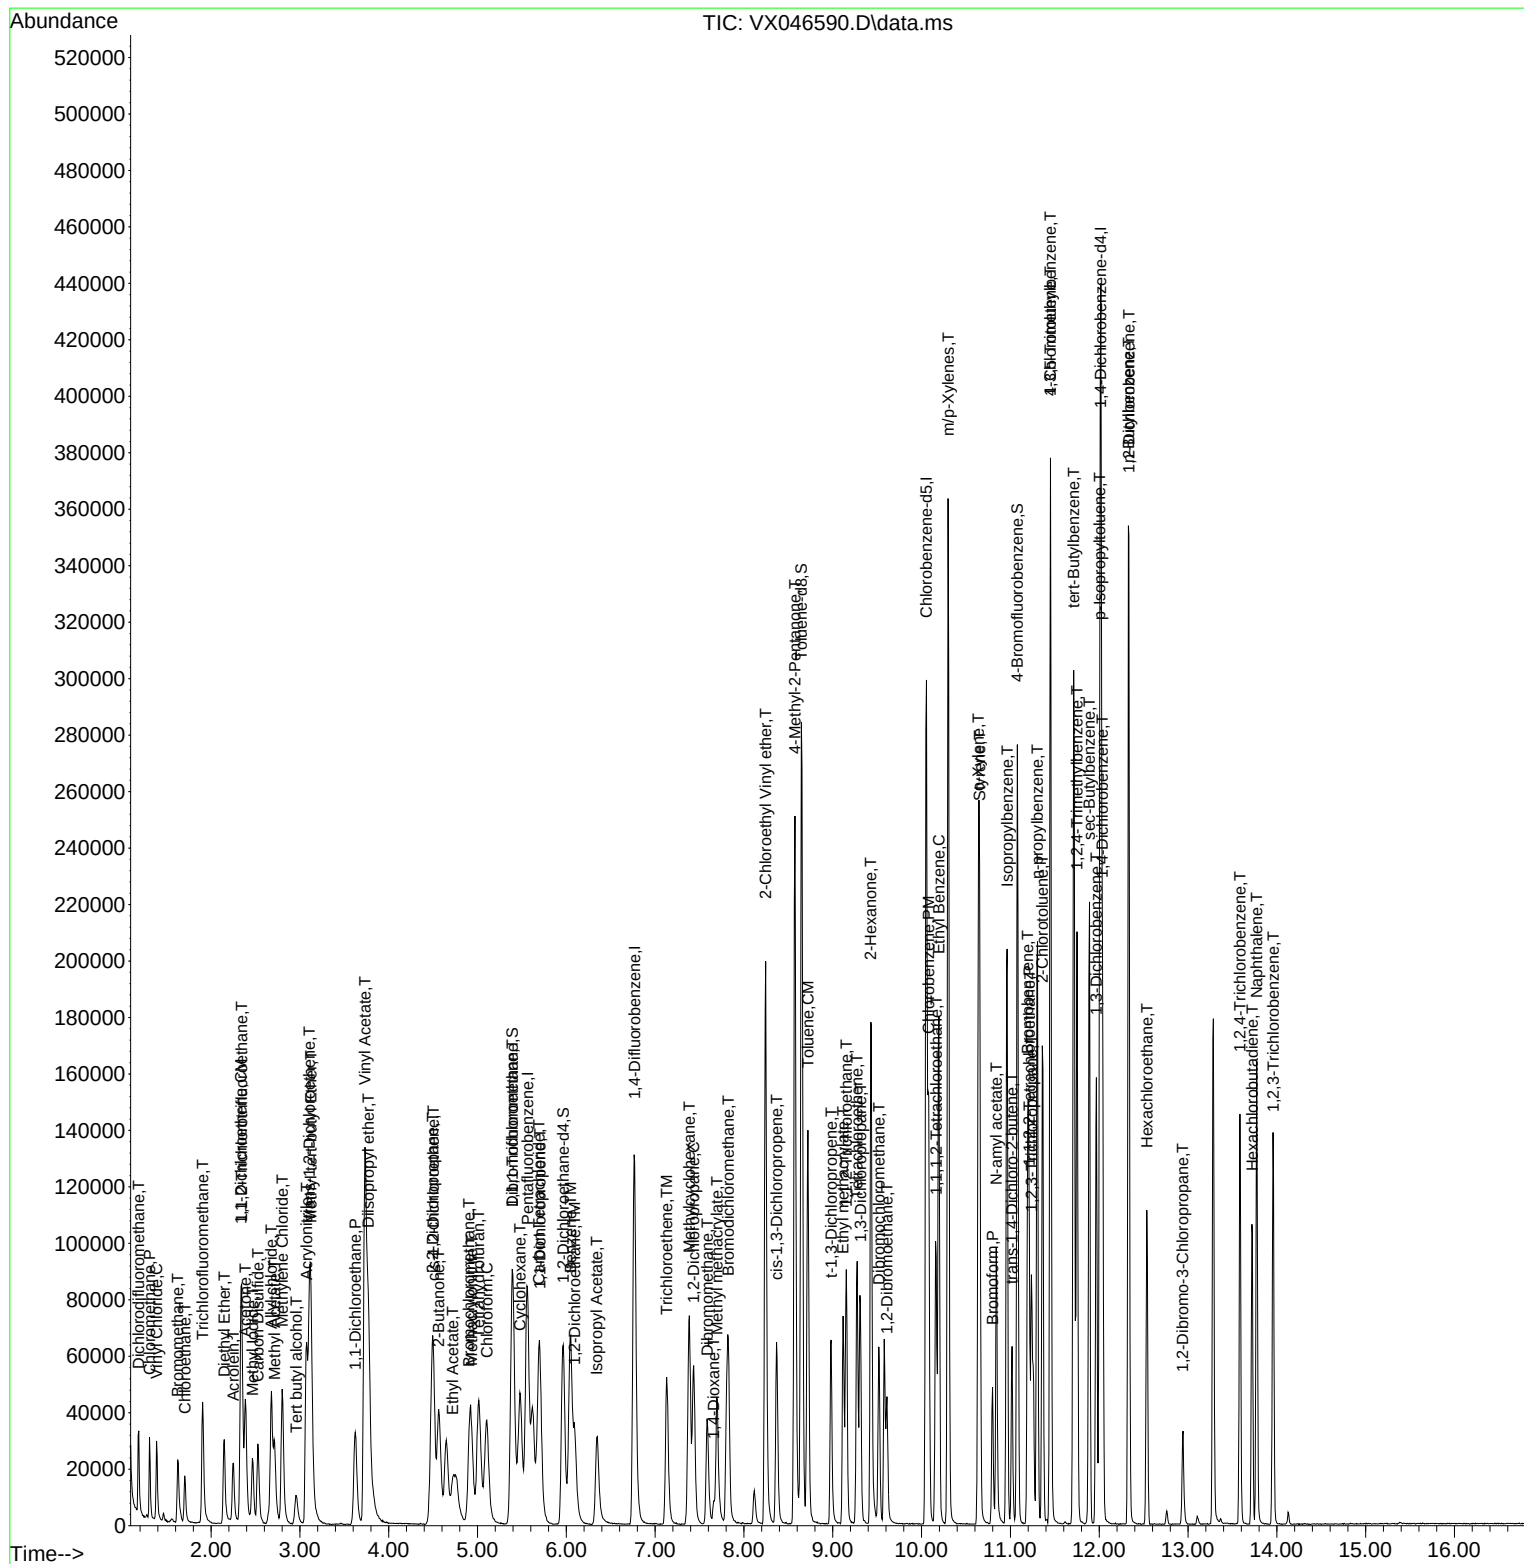

Manual Integration Report

Sequence:	VX060625	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDIC005	VX046518.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:36 PM	MMDadoda	6/9/2025 1:14:56 PM	Peak Integrated by Software
VSTDIC020	VX046519.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:40 PM	MMDadoda	6/9/2025 1:14:59 PM	Peak Integrated by Software
VSTDIC050	VX046520.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:44 PM	MMDadoda	6/9/2025 1:15:03 PM	Peak Integrated by Software
VSTDIC100	VX046521.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:48 PM	MMDadoda	6/9/2025 1:15:08 PM	Peak Integrated by Software
VSTDIC150	VX046522.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:52 PM	MMDadoda	6/9/2025 1:15:37 PM	Peak Integrated by Software
VSTDIC001	VX046524.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:08:38 AM	MMDadoda	6/9/2025 1:15:41 PM	Peak Integrated by Software
VSTDIC001	VX046524.D	1,4-Dichlorobenzene	JOHN	6/9/2025 8:08:38 AM	MMDadoda	6/9/2025 1:15:41 PM	Peak Integrated by Software
VSTDIC001	VX046524.D	Ethyl Acetate	JOHN	6/9/2025 8:08:38 AM	MMDadoda	6/9/2025 1:15:41 PM	Peak Integrated by Software
VSTDICV050	VX046525.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:26:01 PM	MMDadoda	6/9/2025 1:16:01 PM	Peak Integrated by Software
VSTDIC050	VX046544.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:10:18 AM	MMDadoda	6/9/2025 1:16:52 PM	Peak Integrated by Software
VSTDIC050	VX046546.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:10:22 AM	MMDadoda	6/9/2025 1:16:54 PM	Peak Integrated by Software
VSTDIC050	VX046565.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:12:06 AM	Sam	6/9/2025 1:18:52 PM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

VX060625

Instrument

MSVOA_x

Sample ID

File ID

Parameter

Review By

Review On

Supervised
By

Supervised On

Reason

Manual Integration Report

Sequence:	vx061025	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VX046586.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:01:36 AM	MMDadoda	6/11/2025 11:13:23 AM	Peak Integrated by Software
VX0610WBS01	VX046589.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:01:43 AM	MMDadoda	6/11/2025 11:13:26 AM	Peak Integrated by Software
VX0610WBSD0 1	VX046590.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:01:48 AM	MMDadoda	6/11/2025 11:13:29 AM	Peak Integrated by Software
VSTDCCC050	VX046612.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:02:50 AM	MMDadoda	6/11/2025 11:13:46 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	1,1,1-Trichloroethane	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	1,1-Dichloropropene	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	1,2-Dibromoethane	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	1,2-Dichloropropane	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	Acrolein	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	Diethyl Ether	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICC005	VX046614.D	Methyl methacrylate	JOHN	6/11/2025 10:02:54 AM	MMDadoda	6/11/2025 11:13:49 AM	Peak Integrated by Software
VSTDICCC020	VX046615.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:02:58 AM	MMDadoda	6/11/2025 11:13:51 AM	Peak Integrated by Software

Manual Integration Report

Sequence:	vx061025	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICCC020	VX046615.D	Ethyl Acetate	JOHN	6/11/2025 10:02:58 AM	MMDadoda	6/11/2025 11:13:51 AM	Peak Integrated by Software
VSTDICCC050	VX046616.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:03:09 AM	MMDadoda	6/11/2025 11:13:53 AM	Peak Integrated by Software
VSTDICCC100	VX046617.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:03:14 AM	MMDadoda	6/11/2025 11:13:55 AM	Peak Integrated by Software
VSTDICCC100	VX046617.D	Ethyl Acetate	JOHN	6/11/2025 10:03:14 AM	MMDadoda	6/11/2025 11:13:55 AM	Peak Integrated by Software
VSTDICCC150	VX046618.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:03:18 AM	MMDadoda	6/11/2025 11:13:57 AM	Peak Integrated by Software
VSTDICCC150	VX046618.D	Ethyl Acetate	JOHN	6/11/2025 10:03:18 AM	MMDadoda	6/11/2025 11:13:57 AM	Peak Integrated by Software
VSTDICV020	VX046620.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:03:22 AM	MMDadoda	6/11/2025 11:13:59 AM	Peak Integrated by Software
VSTDICV020	VX046620.D	tert-Butyl Alcohol	JOHN	6/11/2025 10:03:22 AM	MMDadoda	6/11/2025 11:13:59 AM	Peak Integrated by Software
VSTDCCC020	VX046626.D	1,2,3-Trichloropropane	JOHN	6/11/2025 10:03:50 AM	MMDadoda	6/11/2025 11:14:07 AM	Peak Integrated by Software
VSTDCCC020	VX046626.D	Ethyl Acetate	JOHN	6/11/2025 10:03:50 AM	MMDadoda	6/11/2025 11:14:07 AM	Peak Integrated by Software

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Mahesh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX046516.D	06 Jun 2025 08:47	JC/MD	Ok
2	VSTDIC001	VX046517.D	06 Jun 2025 09:13	JC/MD	Not Ok
3	VSTDIC005	VX046518.D	06 Jun 2025 09:42	JC/MD	Ok,M
4	VSTDIC020	VX046519.D	06 Jun 2025 10:18	JC/MD	Ok,M
5	VSTDIC050	VX046520.D	06 Jun 2025 10:40	JC/MD	Ok,M
6	VSTDIC100	VX046521.D	06 Jun 2025 11:02	JC/MD	Ok,M
7	VSTDIC150	VX046522.D	06 Jun 2025 11:25	JC/MD	Ok,M
8	IBLK	VX046523.D	06 Jun 2025 11:47	JC/MD	Ok
9	VSTDIC001	VX046524.D	06 Jun 2025 12:57	JC/MD	Ok,M
10	VSTDICV050	VX046525.D	06 Jun 2025 14:11	JC/MD	Ok,M
11	VX0606MBL01	VX046526.D	06 Jun 2025 14:39	JC/MD	Ok
12	VX0606WBL01	VX046527.D	06 Jun 2025 15:02	JC/MD	Ok
13	VX0606WBS01	VX046528.D	06 Jun 2025 15:25	JC/MD	Ok,M
14	VX0606MBS01	VX046529.D	06 Jun 2025 15:51	JC/MD	Ok,M
15	Q2168-11MEDL	VX046530.D	06 Jun 2025 16:13	JC/MD	Ok
16	VX0606WBSD01	VX046531.D	06 Jun 2025 16:36	JC/MD	Ok,M
17	Q2194-02	VX046532.D	06 Jun 2025 16:58	JC/MD	Ok
18	Q2194-04	VX046533.D	06 Jun 2025 17:21	JC/MD	Ok
19	Q2207-09	VX046534.D	06 Jun 2025 17:43	JC/MD	Ok,M
20	Q2207-18	VX046535.D	06 Jun 2025 18:06	JC/MD	Ok,M
21	Q2207-27	VX046536.D	06 Jun 2025 18:28	JC/MD	Ok,M

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Maresh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	Q2207-36	VX046537.D	06 Jun 2025 18:51	JC/MD	Ok,M
23	Q2207-45	VX046538.D	06 Jun 2025 19:13	JC/MD	Ok,M
24	Q2208-09	VX046539.D	06 Jun 2025 19:35	JC/MD	Ok,M
25	Q2208-18	VX046540.D	06 Jun 2025 19:58	JC/MD	Ok,M
26	Q2208-27	VX046541.D	06 Jun 2025 20:20	JC/MD	Ok,M
27	Q2208-36	VX046542.D	06 Jun 2025 20:42	JC/MD	Ok,M
28	Q2236-01	VX046543.D	06 Jun 2025 21:04	JC/MD	Not Ok
29	VSTDCCC050	VX046544.D	06 Jun 2025 21:26	JC/MD	Not Ok
30	BFB	VX046545.D	06 Jun 2025 23:59	JC/MD	Ok
31	VSTDCCC050	VX046546.D	07 Jun 2025 00:34	JC/MD	Ok,M
32	VX0606WBL02	VX046547.D	07 Jun 2025 01:17	JC/MD	Ok
33	VX0606WBS02	VX046548.D	07 Jun 2025 02:00	JC/MD	Ok,M
34	VX0606WBSD02	VX046549.D	07 Jun 2025 02:22	JC/MD	Ok,M
35	PB168312TB	VX046550.D	07 Jun 2025 02:43	JC/MD	Ok,M
36	PB168272TB	VX046551.D	07 Jun 2025 03:05	JC/MD	Ok,M
37	Q2236-05	VX046552.D	07 Jun 2025 03:26	JC/MD	ReRun
38	Q2236-09	VX046553.D	07 Jun 2025 03:48	JC/MD	ReRun
39	Q2236-13	VX046554.D	07 Jun 2025 04:09	JC/MD	Ok
40	Q2236-17	VX046555.D	07 Jun 2025 04:31	JC/MD	ReRun
41	Q2227-04	VX046556.D	07 Jun 2025 04:52	JC/MD	Ok,M
42	Q2228-04	VX046557.D	07 Jun 2025 05:14	JC/MD	ReRun
43	Q2235-01	VX046558.D	07 Jun 2025 05:36	JC/MD	ReRun
44	Q2240-04	VX046559.D	07 Jun 2025 05:57	JC/MD	ReRun

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Mahesh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	Q2240-08	VX046560.D	07 Jun 2025 06:18	JC/MD	ReRun
46	Q2240-12	VX046561.D	07 Jun 2025 06:40	JC/MD	ReRun
47	Q2241-04	VX046562.D	07 Jun 2025 07:01	JC/MD	ReRun
48	Q2241-08	VX046563.D	07 Jun 2025 07:23	JC/MD	ReRun
49	Q2226-04	VX046564.D	07 Jun 2025 07:44	JC/MD	ReRun
50	VSTDCCC050	VX046565.D	07 Jun 2025 08:06	JC/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QC Batch ID # VX061025

Review By	John Carlone	Review On	6/11/2025 10:17:47 AM
Supervise By	Maresh Dadoda	Supervise On	6/11/2025 11:14:33 AM
SubDirectory	VX061025	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134200		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134201,VP134202		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX046585.D	10 Jun 2025 08:36	JC/MD	Ok
2	VSTDCCC050	VX046586.D	10 Jun 2025 09:07	JC/MD	Ok,M
3	VX0610MBL01	VX046587.D	10 Jun 2025 09:36	JC/MD	Ok
4	VX0610WBL01	VX046588.D	10 Jun 2025 09:57	JC/MD	Ok
5	VX0610WBS01	VX046589.D	10 Jun 2025 10:18	JC/MD	Ok,M
6	VX0610WBSD01	VX046590.D	10 Jun 2025 10:44	JC/MD	Ok,M
7	Q2262-02	VX046591.D	10 Jun 2025 11:05	JC/MD	Ok
8	Q2262-04	VX046592.D	10 Jun 2025 11:27	JC/MD	Ok
9	IBLK	VX046593.D	10 Jun 2025 11:48	JC/MD	Ok
10	Q2230-01	VX046594.D	10 Jun 2025 12:09	JC/MD	Ok
11	Q2230-06	VX046595.D	10 Jun 2025 12:30	JC/MD	Ok
12	Q2233-01DL	VX046596.D	10 Jun 2025 12:51	JC/MD	Ok
13	Q2233-03DL	VX046597.D	10 Jun 2025 13:13	JC/MD	Ok
14	Q2233-04DL	VX046598.D	10 Jun 2025 13:34	JC/MD	Ok
15	Q2234-01DL	VX046599.D	10 Jun 2025 13:55	JC/MD	Ok
16	IBLK	VX046600.D	10 Jun 2025 14:16	JC/MD	Ok
17	Q2230-05	VX046601.D	10 Jun 2025 14:38	JC/MD	Ok,M
18	Q2230-02	VX046602.D	10 Jun 2025 14:59	JC/MD	Ok,M
19	Q2230-03MS	VX046603.D	10 Jun 2025 15:20	JC/MD	Not Ok
20	Q2230-04MSD	VX046604.D	10 Jun 2025 15:42	JC/MD	Not Ok
21	IBLK	VX046605.D	10 Jun 2025 16:03	JC/MD	Ok

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QC Batch ID # VX061025

Review By	John Carlone	Review On	6/11/2025 10:17:47 AM
Supervise By	Maresh Dadoda	Supervise On	6/11/2025 11:14:33 AM
SubDirectory	VX061025	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134200		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134201,VP134202		

22	Q2249-01	VX046606.D	10 Jun 2025 16:24	JC/MD	Not Ok
23	IBLK	VX046607.D	10 Jun 2025 16:46	JC/MD	Ok
24	Q2233-01	VX046608.D	10 Jun 2025 17:07	JC/MD	Dilution
25	Q2233-03	VX046609.D	10 Jun 2025 17:28	JC/MD	Dilution
26	Q2233-04	VX046610.D	10 Jun 2025 17:50	JC/MD	Dilution
27	Q2234-01	VX046611.D	10 Jun 2025 18:11	JC/MD	Dilution
28	VSTDCCC050	VX046612.D	10 Jun 2025 18:53	JC/MD	Ok,M
29	BFB	VX046613.D	10 Jun 2025 19:57	JC/MD	Ok
30	VSTDICC005	VX046614.D	10 Jun 2025 20:19	JC/MD	Ok,M
31	VSTDICCC020	VX046615.D	10 Jun 2025 20:40	JC/MD	Ok,M
32	VSTDICC050	VX046616.D	10 Jun 2025 21:01	JC/MD	Ok,M
33	VSTDICC100	VX046617.D	10 Jun 2025 21:22	JC/MD	Ok,M
34	VSTDICC150	VX046618.D	10 Jun 2025 21:44	JC/MD	Ok,M
35	IBLK	VX046619.D	10 Jun 2025 22:05	JC/MD	Ok
36	VSTDICV020	VX046620.D	10 Jun 2025 22:26	JC/MD	Ok,M
37	VX0610WBS02	VX046621.D	10 Jun 2025 23:09	JC/MD	Ok,M
38	VX0610WBSD02	VX046622.D	10 Jun 2025 23:30	JC/MD	Ok,M
39	VX0610WBL02	VX046623.D	11 Jun 2025 00:12	JC/MD	Ok
40	Q2203-01	VX046624.D	11 Jun 2025 00:33	JC/MD	Dilution
41	Q2203-04	VX046625.D	11 Jun 2025 00:54	JC/MD	Dilution
42	VSTDCCC020	VX046626.D	11 Jun 2025 01:16	JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Mahesh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M

STD. NAME	STD REF.#
Tune/Reschk	VP134153
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240
CCC	VP134154
Internal Standard/PEM	
ICV/I.BLK	VP134241
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX046516.D	06 Jun 2025 08:47		JC/MD	Ok
2	VSTDIC001	VSTDIC001	VX046517.D	06 Jun 2025 09:13		JC/MD	Not Ok
3	VSTDIC005	VSTDIC005	VX046518.D	06 Jun 2025 09:42	for TCLP	JC/MD	Ok,M
4	VSTDIC020	VSTDIC020	VX046519.D	06 Jun 2025 10:18	Comp #05 fail	JC/MD	Ok,M
5	VSTDIC050	VSTDIC050	VX046520.D	06 Jun 2025 10:40	LR-13,16,17	JC/MD	Ok,M
6	VSTDIC100	VSTDIC100	VX046521.D	06 Jun 2025 11:02		JC/MD	Ok,M
7	VSTDIC150	VSTDIC150	VX046522.D	06 Jun 2025 11:25		JC/MD	Ok,M
8	IBLK	IBLK	VX046523.D	06 Jun 2025 11:47		JC/MD	Ok
9	VSTDIC001	VSTDIC001	VX046524.D	06 Jun 2025 12:57		JC/MD	Ok,M
10	VSTDICV050	ICV VX060625	VX046525.D	06 Jun 2025 14:11		JC/MD	Ok,M
11	VX0606MBL01	VX0606MBL01	VX046526.D	06 Jun 2025 14:39		JC/MD	Ok
12	VX0606WBL01	VX0606WBL01	VX046527.D	06 Jun 2025 15:02		JC/MD	Ok
13	VX0606WBS01	VX0606WBS01	VX046528.D	06 Jun 2025 15:25		JC/MD	Ok,M
14	VX0606MBS01	VX0606MBS01	VX046529.D	06 Jun 2025 15:51		JC/MD	Ok,M
15	Q2168-11MEDL	C2MEDL	VX046530.D	06 Jun 2025 16:13		JC/MD	Ok
16	VX0606WBSD01	VX0606WBSD01	VX046531.D	06 Jun 2025 16:36		JC/MD	Ok,M
17	Q2194-02	COMP-12	VX046532.D	06 Jun 2025 16:58	vial A pH#5.0	JC/MD	Ok
18	Q2194-04	COMP-13	VX046533.D	06 Jun 2025 17:21	vial A pH#5.0	JC/MD	Ok

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Maresh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134153 VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC Internal Standard/PEM	VP134154		
ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134241		

19	Q2207-09	BU-703-COMP-01	VX046534.D	06 Jun 2025 17:43	vial A pH#5.0	JC/MD	Ok,M
20	Q2207-18	BU-703-COMP-02	VX046535.D	06 Jun 2025 18:06	vial A pH#5.0	JC/MD	Ok,M
21	Q2207-27	BU-703-COMP-03	VX046536.D	06 Jun 2025 18:28	vial A pH#5.0	JC/MD	Ok,M
22	Q2207-36	BU-703-COMP-04	VX046537.D	06 Jun 2025 18:51	vial A pH#5.0	JC/MD	Ok,M
23	Q2207-45	BU-703-COMP-05	VX046538.D	06 Jun 2025 19:13	vial A pH#5.0	JC/MD	Ok,M
24	Q2208-09	BU-703-COMP-06	VX046539.D	06 Jun 2025 19:35	vial A pH#5.0	JC/MD	Ok,M
25	Q2208-18	BU-703-COMP-07	VX046540.D	06 Jun 2025 19:58	vial A pH#5.0	JC/MD	Ok,M
26	Q2208-27	BU-703-COMP-08	VX046541.D	06 Jun 2025 20:20	vial A pH#5.0	JC/MD	Ok,M
27	Q2208-36	BU-703-COMP-09	VX046542.D	06 Jun 2025 20:42	vial A pH#5.0	JC/MD	Ok,M
28	Q2236-01	WC-A4-05A-G	VX046543.D	06 Jun 2025 21:04	vial A pH#5.0 Out of tune	JC/MD	Not Ok
29	VSTDCCC050	VSTDCCC050EC	VX046544.D	06 Jun 2025 21:26	Out of tune	JC/MD	Not Ok
30	BFB	BFB	VX046545.D	06 Jun 2025 23:59		JC/MD	Ok
31	VSTDCCC050	VSTDCCC050	VX046546.D	07 Jun 2025 00:34		JC/MD	Ok,M
32	VX0606WBL02	VX0606WBL02	VX046547.D	07 Jun 2025 01:17		JC/MD	Ok
33	VX0606WBS02	VX0606WBS02	VX046548.D	07 Jun 2025 02:00		JC/MD	Ok,M
34	VX0606WBSD02	VX0606WBSD02	VX046549.D	07 Jun 2025 02:22		JC/MD	Ok,M
35	PB168312TB	PB168312TB	VX046550.D	07 Jun 2025 02:43		JC/MD	Ok,M
36	PB168272TB	PB168272TB	VX046551.D	07 Jun 2025 03:05		JC/MD	Ok,M
37	Q2236-05	WC-A2-04-G	VX046552.D	07 Jun 2025 03:26	Surrogate Fail	JC/MD	ReRun

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Maresh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134153 VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC Internal Standard/PEM	VP134154		
ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134241		

38	Q2236-09	WC-A2-05-G	VX046553.D	07 Jun 2025 03:48	Internal Standard Fail	JC/MD	ReRun
39	Q2236-13	WC-A2-06-G	VX046554.D	07 Jun 2025 04:09	vial A pH#5.0	JC/MD	Ok
40	Q2236-17	WC-A2-07-G	VX046555.D	07 Jun 2025 04:31	Internal Standard Fail; Surrogate fail	JC/MD	ReRun
41	Q2227-04	TP07-MHH-WC	VX046556.D	07 Jun 2025 04:52		JC/MD	Ok,M
42	Q2228-04	TP08-MHI-WC	VX046557.D	07 Jun 2025 05:14	Internal Standard Fail	JC/MD	ReRun
43	Q2235-01	WC-A2-08-G	VX046558.D	07 Jun 2025 05:36	Internal Standard Fail	JC/MD	ReRun
44	Q2240-04	TP-3	VX046559.D	07 Jun 2025 05:57	Internal Standard Fail	JC/MD	ReRun
45	Q2240-08	TP-2	VX046560.D	07 Jun 2025 06:18	Internal Standard Fail	JC/MD	ReRun
46	Q2240-12	TP-1	VX046561.D	07 Jun 2025 06:40	Internal Standard Fail	JC/MD	ReRun
47	Q2241-04	TP-N	VX046562.D	07 Jun 2025 07:01	Internal Standard Fail	JC/MD	ReRun
48	Q2241-08	TP-S	VX046563.D	07 Jun 2025 07:23	Internal Standard Fail	JC/MD	ReRun
49	Q2226-04	TP06-MHI-WC	VX046564.D	07 Jun 2025 07:44	Internal Standard Fail	JC/MD	ReRun
50	VSTDCCC050	VSTDCCC050EC	VX046565.D	07 Jun 2025 08:06		JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX061025

Review By	John Carlone	Review On	6/11/2025 10:17:47 AM
Supervise By	Maresh Dadoda	Supervise On	6/11/2025 11:14:33 AM
SubDirectory	VX061025	HP Acquire Method	HP Processing Method 82X060625W.M

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds	VP134200
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134201,VP134202

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX046585.D	10 Jun 2025 08:36		JC/MD	Ok
2	VSTDCCC050	VSTDCCC050	VX046586.D	10 Jun 2025 09:07	pH#Lot#V12668	JC/MD	Ok,M
3	VX0610MBL01	VX0610MBL01	VX046587.D	10 Jun 2025 09:36		JC/MD	Ok
4	VX0610WBL01	VX0610WBL01	VX046588.D	10 Jun 2025 09:57		JC/MD	Ok
5	VX0610WBS01	VX0610WBS01	VX046589.D	10 Jun 2025 10:18		JC/MD	Ok,M
6	VX0610WBSD01	VX0610WBSD01	VX046590.D	10 Jun 2025 10:44		JC/MD	Ok,M
7	Q2262-02	ARS20-0032	VX046591.D	10 Jun 2025 11:05	vial B pH#5.0	JC/MD	Ok
8	Q2262-04	ARS20-0001	VX046592.D	10 Jun 2025 11:27	vial B pH#5.0	JC/MD	Ok
9	IBLK	IBLK	VX046593.D	10 Jun 2025 11:48		JC/MD	Ok
10	Q2230-01	FB-060425	VX046594.D	10 Jun 2025 12:09	vial A pH<2 FB	JC/MD	Ok
11	Q2230-06	TB060425	VX046595.D	10 Jun 2025 12:30	vial A pH<2 TB	JC/MD	Ok
12	Q2233-01DL	MW-18B-56-060425DL	VX046596.D	10 Jun 2025 12:51	vial B pH<2	JC/MD	Ok
13	Q2233-03DL	MW-18B-56-060425-FD	VX046597.D	10 Jun 2025 13:13	vial B pH<2	JC/MD	Ok
14	Q2233-04DL	MW-19B-72-060425DL	VX046598.D	10 Jun 2025 13:34	vial B pH<2	JC/MD	Ok
15	Q2234-01DL	MW-17B-55-060425DL	VX046599.D	10 Jun 2025 13:55	vial B pH<2	JC/MD	Ok
16	IBLK	IBLK	VX046600.D	10 Jun 2025 14:16		JC/MD	Ok
17	Q2230-05	GW-MW901-060425	VX046601.D	10 Jun 2025 14:38	vial A pH<2	JC/MD	Ok,M
18	Q2230-02	GW-MW01-060425	VX046602.D	10 Jun 2025 14:59	vial A pH<2	JC/MD	Ok,M

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX061025

Review By	John Carlone	Review On	6/11/2025 10:17:47 AM
Supervise By	Maresh Dadoda	Supervise On	6/11/2025 11:14:33 AM
SubDirectory	VX061025	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134200		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134201,VP134202		

19	Q2230-03MS	GW-MW01-060425MS	VX046603.D	10 Jun 2025 15:20	Internal Standard Fail; Surrogate Fail; Spike not added	JC/MD	Not Ok
20	Q2230-04MSD	GW-MW01-060425MS	VX046604.D	10 Jun 2025 15:42	Internal Standard Fail; Surrogate Fail; Spike not added	JC/MD	Not Ok
21	IBLK	IBLK	VX046605.D	10 Jun 2025 16:03		JC/MD	Ok
22	Q2249-01	MW-06-6.5-060525	VX046606.D	10 Jun 2025 16:24	Run @ lower dilution	JC/MD	Not Ok
23	IBLK	IBLK	VX046607.D	10 Jun 2025 16:46		JC/MD	Ok
24	Q2233-01	MW-18B-56-060425	VX046608.D	10 Jun 2025 17:07	vial A pH<2 Need 10X	JC/MD	Dilution
25	Q2233-03	MW-18B-56-060425-FD	VX046609.D	10 Jun 2025 17:28	vial A pH<2 Need 10X	JC/MD	Dilution
26	Q2233-04	MW-19B-72-060425	VX046610.D	10 Jun 2025 17:50	vial A pH<2 Need 100X	JC/MD	Dilution
27	Q2234-01	MW-17B-55-060425	VX046611.D	10 Jun 2025 18:11	vial A pH<2 Need 100X	JC/MD	Dilution
28	VSTDCCC050	VSTDCCC050EC	VX046612.D	10 Jun 2025 18:53		JC/MD	Ok,M
29	BFB	BFB	VX046613.D	10 Jun 2025 19:57		JC/MD	Ok
30	VSTDICC005	VSTDICC005	VX046614.D	10 Jun 2025 20:19		JC/MD	Ok,M
31	VSTDICCC020	VSTDICCC020	VX046615.D	10 Jun 2025 20:40		JC/MD	Ok,M
32	VSTDICC050	VSTDICC050	VX046616.D	10 Jun 2025 21:01		JC/MD	Ok,M
33	VSTDICC100	VSTDICC100	VX046617.D	10 Jun 2025 21:22		JC/MD	Ok,M
34	VSTDICC150	VSTDICC150	VX046618.D	10 Jun 2025 21:44		JC/MD	Ok,M
35	IBLK	IBLK	VX046619.D	10 Jun 2025 22:05		JC/MD	Ok
36	VSTDICV020	ICVVX061025	VX046620.D	10 Jun 2025 22:26		JC/MD	Ok,M
37	VX0610WBS02	VX0610WBS02	VX046621.D	10 Jun 2025 23:09		JC/MD	Ok,M

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX061025

Review By	John Carlone	Review On	6/11/2025 10:17:47 AM
Supervise By	Maresh Dadoda	Supervise On	6/11/2025 11:14:33 AM
SubDirectory	VX061025	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134200		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134201,VP134202		

38	VX0610WBSD02	VX0610WBSD02	VX046622.D	10 Jun 2025 23:30		JC/MD	Ok,M
39	VX0610WBL02	VX0610WBL02	VX046623.D	11 Jun 2025 00:12		JC/MD	Ok
40	Q2203-01	001-WILLETS-PT-BLVD	VX046624.D	11 Jun 2025 00:33	vial A pH<2 Need 5X	JC/MD	Dilution
41	Q2203-04	002-35TH-AVE(JUNE)	VX046625.D	11 Jun 2025 00:54	vial A pH<2 Need 5X	JC/MD	Dilution
42	VSTDCCC020	VSTDCCC020EC	VX046626.D	11 Jun 2025 01:16		JC/MD	Ok,M

M : Manual Integration

Prep Standard - Chemical Standard Summary

Order ID : Q2234

Test : VOCMS Group3

Prepbatch ID :

Sequence ID/Qc Batch ID: vx061025,

Standard ID :

VP133174,VP133887,VP133935,VP133953,VP133991,VP134142,VP134149,VP134200,VP134201,VP134202,

Chemical ID :

V13391,V13706,V14290,V14432,V14435,V14503,V14504,V14525,V14526,V14613,V14620,V14626,V14636,V14637,V14638,V14639,V14668,V14671,V14673,V14675,V14711,V14717,V14718,V14721,V14749,V14750,V14811,V14812,V14843,V14921,V14929,V14944,V14945,V14946,V14947,W3112,

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
617	8260 Surrogate, 400PPM	VP133174	02/27/2025	08/27/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								03/04/2025

FROM 0.40000ml of V13706 + 24.60000ml of V14613 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
257	8260 Calibration Working STD Mix-First source, 160PPM	VP133887	05/12/2025	06/23/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								05/14/2025

FROM 0.40000ml of V14843 + 1.00000ml of V14432 + 1.00000ml of V14435 + 1.00000ml of V14503 + 1.00000ml of V14504 + 1.00000ml of V14525 + 1.00000ml of V14526 + 1.00000ml of V14711 + 1.00000ml of V14717 + 1.00000ml of V14718 + 1.00000ml of V14721 + 1.00000ml of V14749 + 1.00000ml of V14750 + 1.00000ml of V14811 + 1.00000ml of V14812 + 10.60000ml of V14921 = Final Quantity: 25.000 ml

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
247	8260 Internal Standard, 250PPM	VP133935	05/16/2025	11/12/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								05/21/2025

FROM 0.25000ml of V14290 + 24.75000ml of V14921 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
218	BFB, 25PPM	VP133953	05/19/2025	11/09/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								05/21/2025

FROM 0.25000ml of V13391 + 24.75000ml of V14626 = Final Quantity: 25.000 ml

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
51	8260 Working STD (Acrolein) -first source, 800PPM	VP133991	05/22/2025	06/19/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								05/24/2025

FROM 1.00000ml of V14944 + 1.00000ml of V14945 + 1.00000ml of V14946 + 1.00000ml of V14947 + 21.00000ml of V14620 = Final
Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
719	8260 Working STD (BCM)-First source, 400PPM	VP134142	06/06/2025	12/06/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								06/10/2025

FROM 1.00000ml of V14668 + 1.00000ml of V14671 + 1.00000ml of V14673 + 1.00000ml of V14675 + 16.00000ml of V14929 = Final
Quantity: 20.000 ml

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1810	8260 Working Std(2-CVE)-800ppm	VP134149	06/06/2025	12/06/2025	Semsettin Yesilyurt	None	None	Maresh Dadoda
								06/10/2025

FROM 1.00000ml of V14636 + 1.00000ml of V14637 + 1.00000ml of V14638 + 1.00000ml of V14639 + 46.00000ml of V14929 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
589	BFB TUNE CHECK	VP134200	06/10/2025	06/11/2025	John Carlone	None	None	Maresh Dadoda
								06/10/2025

FROM 39.98400ml of W3112 + 0.01600ml of VP133953 = Final Quantity: 40.000 ml

[illegible]

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	VP134202	06/10/2025	06/11/2025	John Carlone	None	None	Mahesh Dadoda 06/10/2025
<u>FROM</u> 39.94450ml of W3112 + 0.00500ml of VP133174 + 0.00500ml of VP134142 + 0.00800ml of VP133935 + 0.01250ml of VP133887 + 0.01250ml of VP133991 + 0.01250ml of VP134149 = Final Quantity: 40.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30067 / BFB tuneing solution	A0191805	11/22/2025	11/22/2024 / SAM	01/13/2023 / SAM	V13391

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555582 / Custom Mixture, 8260 A/B Surrogate Mix [CS 5179-2]	A0196865	02/27/2026	02/27/2025 / SAM	04/12/2023 / SAM	V13706

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555581 / Custom Standard, 8260 Internal Std [CS 5179-1]	A0210184	12/12/2025	12/12/2024 / SAM	04/15/2024 / SAM	V14290

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	09/30/2025	05/12/2025 / SAM	08/15/2024 / SAM	V14432

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	09/20/2025	03/20/2025 / SAM	08/15/2024 / SAM	V14435

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	11/12/2025	05/12/2025 / SAM	09/17/2024 / SAM	V14503

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	11/12/2025	05/12/2025 / SAM	09/17/2024 / SAM	V14504

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	11/12/2025	05/12/2025 / SAM	09/18/2024 / SAM	V14525

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	11/12/2025	05/12/2025 / SAM	09/18/2024 / SAM	V14526

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	08/27/2025	02/27/2025 / SAM	11/26/2024 / SAM	V14613

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	10/25/2025	05/09/2025 / SAM	11/26/2024 / SAM	V14620

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	23I0762004	11/09/2025	05/09/2025 / SAM	11/26/2024 / SAM	V14626

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14636

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14637

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14638

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	12/06/2025	06/06/2025 / SAM	12/06/2024 / SAM	V14639

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0214960	12/06/2025	06/06/2025 / SAM	12/09/2024 / SAM	V14668

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0214960	12/06/2025	06/06/2025 / SAM	12/09/2024 / SAM	V14671

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0214960	12/06/2025	06/06/2025 / SAM	12/09/2024 / SAM	V14673

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0214960	12/06/2025	06/06/2025 / SAM	12/09/2024 / SAM	V14675

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14711

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14717

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14718

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000uq/ml, PTM, 1ml	A02110618	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14721

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	11/13/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14749

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	11/12/2025	05/12/2025 / SAM	12/17/2024 / SAM	V14750

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE	A0220471	11/12/2025	05/12/2025 / SAM	01/08/2025 / SAM	V14811

LOTS

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE	A0220471	06/30/2026	05/12/2025 / SAM	01/08/2025 / SAM	V14812

LOTS

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30470 / VOA Stock Solution, tert-butanol std, 1mL, P&TM	A0217535	11/12/2025	05/12/2025 / SAM	01/21/2025 / SAM	V14843

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	24G0262002	11/12/2025	05/12/2025 / SAM	05/09/2025 / SAM	V14921

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	24G0262002	12/06/2025	06/06/2025 / SAM	05/09/2025 / SAM	V14929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14944

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14945

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14946

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	051925	06/19/2025	05/22/2025 / SAM	05/21/2025 / SAM	V14947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 23I0762004
Manufactured Date: 2023-08-11
Expiration Date: 2026-08-10
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.5 ppm
Titration Acid (μeq/g)	≤ 0.3	0.2
Titration Base (μeq/g)	≤ 0.10	0.01
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Ken Koehnlein
Sr. Manager, Quality Assurance

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

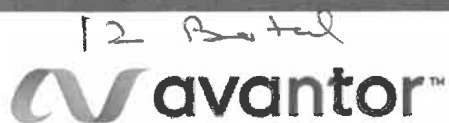

Material No.: 9077-02
Batch No.: 22L0562016
Manufactured Date: 2022-10-26
Expiration Date: 2025-10-25
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid (μeq/g)	≤ 0.3	0.2
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier
Vice President Global Quality

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

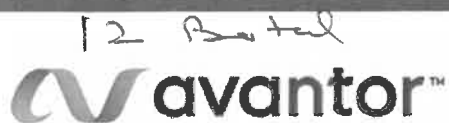


Material No.: 9077-02
Batch No.: 22L0562016
Manufactured Date: 2022-10-26
Expiration Date: 2025-10-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid (μeq/g)	≤ 0.3	0.2
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

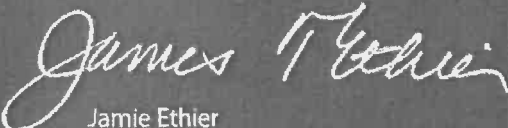
Jamie Ethier
Vice President Global Quality



Ree 03117/24

CERTIFIED WEIGHT REPORT

Part Number: 95317

Lot Number: 021624

Description: Universal VOA Megamix

69 components

Expiration Date: 021627

Recommended Storage: Freezer (0 °C)

Nominal Concentration (µg/mL): 2000

NIST Test ID#: BUTB

Solvent(s): Lot#
Methanol EG359-USQ12Weight(s) shown below were combined and diluted to (mL): 100.0 0.021 Balance Uncertainty
Flask Uncertainty

Formulated By:	Prashant Chauhan	021624
Reviewed By:	Pedro L. Renteria	021624
DATE		


Compound	(KMe)	Lot	Dir.	Initial	Initial	Nominal	Purity	Purity	Uncertainty	Target	Actual	Actual	Expanded	SDS Information			
	Part Number	Number	Factor	Vol. (mL)	Conc.(µg/mL)	Conc (µg/mL)	(%)	Uncertainty	Pipette (mL)	Weight(g)	Weight(g)	Conc (µg/mL)	Uncertainty	(+/-) (µg/mL)	CASE	OSHA PEL (TWA)	LD50
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m3/8H)	or-rat 2450mg/kg	
2. Allyl chloride (3-Chloropropene)	(0325)	102396	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m3/8H)	or-rat 700mg/kg	
3. Carbon disulfide	(0060)	MKCR8561	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.6	8.1	75-15-0	4 ppm (12mg/m3) (skin)	or-rat 1200mg/kg	
4. cis-1,4-Dichloro-2-butene	(1196)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21056	0.21069	2001.1	8.5	1478-11-5	N/A	N/A	
5. trans-1,4-Dichloro-2-butene	(0486)	MKBP9041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20746	2001.7	8.4	110-57-6	N/A	N/A	
6. Diethyl ether	(0153)	IK18CAS000C	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	N/A	N/A	
7. Ethyl methacrylate	(0381)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	N/A	or-rat 14800mg/kg	
8. Iodomethane	(0489)	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20121	2001.5	8.2	74-88-4	5 ppm(28mg/m3/8H)(skin)	or-rat 75mg/kg	
9. 2-Methyl-1-propanol	(0445)	15241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m3/8H)	or-rat 2460mg/kg	
10. Methacrylonitrile	(0442)	00427ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	128-98-7	1 ppm (3mg/m3/8H)(skin)	or-rat 120mg/kg	
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm(35mg/m3/8H)(skin)	or-rat 277mg/kg	
12. Methyl methacrylate	(0404)	MKGW6137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-62-6	100 ppm (410mg/m3/8H)	or-rat 7872mg/kg	
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-95-3	1 ppm (5mg/m3/8H)(skin)	or-rat 780mg/kg	
14. 2-Nitropropane	(0461)	14002JX	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	78-46-9	10 ppm (35mg/m3/8H)	or-rat 720mg/kg	
15. Perchloroethane	(0460)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	N/A	N/A	
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18930	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1	1000 ppm (7600mg/m3/8H)	or-rat 43g/kg	
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-27-4	N/A	or-rat 915mg/kg	
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	N/A	or-rat 848mg/kg	
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	N/A	N/A	
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.4	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	N/A	N/A	
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2	500 ppm	or-rat 1235mg/kg	
22. 1,1-Dichloroethane	32261	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m3/8H)	or-rat 200mg/kg	
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	78-25-2	0.5 ppm (5mg/m3) (skin)	or-rat 933mg/kg	
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	2 ppm (12.6mg/m3/8H)	or-rat 2350mg/kg	
25. Chloroform	95321	020724	0.10	10.00	20004.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	67-68-3	60 ppm (240mg/m3) (CL)	or-rat 908mg/kg	
26. Dibromomethane	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-95-3	N/A	or-rat 106mg/kg	
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7	N/A	N/A	
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-34-3	100 ppm	or-rat 725mg/kg	
29. Trichloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	2019.8	20.8	127-18-4	25 ppm (170mg/m3/8H)(final)	or-rat 2629mg/kg	
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m3/8H)	or-rat 10300mg/kg	
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40016.5	2000	NA	NA	0.017	NA	NA	2000.3	22.9	96-12-8	0.001 ppm	or-rat 170mg/kg	
32. 1,2-Dibromoethane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-93-4	20 ppm (8H)	or-rat 108mg/kg	
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (8H)	or-rat 670mg/kg	
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5	75 ppm (350mg/m3/8H)	or-rat 1947mg/kg	
35. 1,3-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-28-9	N/A	or-rat 3600mg/kg	
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	2000.1	28.7	563-58-6	N/A	N/A	
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10061-01-5	N/A	N/A	
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.4	23.0	10061-02-6	N/A	N/A	
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-68-3	0.02 ppm (0.24mg/m3/8H)	or-rat 82mg/kg	
40. 1,1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	N/A	or-rat 670mg/kg	
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	79-34-5	5 ppm (35mg/m3/8H)(skin)	or-rat 800mg/kg	
42. 1,1,2-Trichloroethane	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.8	23.0	79-00-5	10 ppm (45mg/m3/8H)(skin)	or-rat 936mg/kg	
43. Trichloroethene	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	2000.9	22.9	79-01-6	50 ppm (270mg/m3/8H)	or-mus 2402mg/kg	
44. 1,2,3-Trichloropropane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	96-18-4	10 ppm (60mg/m3/8H)	or-rat 149.8mg/kg	
45. Benzene	35162	050823	0.05	5.00	40006.0	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm	or-rat 4894mg/kg	
46. Bromobenzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	104-51-8	N/A	or-rat 2699mg/kg	
47. n-Butyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m3/8H)	or-rat >2000mg/kg	
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	99-87-6	N/A	or-rat 4750mg/kg	
49. p-Isopropyl toluene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m3/8H)	or-rat 490mg/kg	
50. Naphthalene	35162	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm	or-rat 5000mg/kg	
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-98-3	200 ppm (435mg/m3/8H)	or-rat 5000mg/kg	
52. Toluene	35162	050823	0.05	5.00	40008.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	87-81-6	N/A	or-rat 1390mg/kg	
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m3)	or-rat 756mg/kg	
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	95-63-6	N/A	or-rat 5g/kg	
55. 1,2,4-Trimethylbenzene	35162	050823	0.05	5.00	40001.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-87-6	N/A	or-rat 5000mg/kg	
56. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3	100 ppm (435mg/m3/8H)	or-rat 5g/kg	
57. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	96-06-6	N/A	N/A	
58. tert-Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	135-98-6	N/A	or-rat 2240mg/kg	
59. sec-Butyl benzene	35163	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-90-7	75 ppm (350mg/m3/8H)	or-rat 2290mg/kg	
60. Chlorobenzene	35163	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	95-49-8	50 ppm (250mg/m3/8H)	or-rat 3900mg/kg	
61. 2-Chlorotoluene	35163	101923	0.05	5.00	40003.3	2000	NA	NA	0.017	NA	NA	1999.7	22.9	106-43-4	N/A	or-rat 2100mg/kg	
62. 4-Chlorotoluene	35163	101923	0.05	5.00	40003.3	2000	NA	NA	0.017	NA	NA	1999.7	22.9	95-50-1	50 ppm (300mg/m3) (CL)	or-rat 500mg/kg	
63. 1,2-Dichlorobenzene	35163	101923	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	23.2				



Run 16, "P95317 L021624 (2000µg/mL in MeOH)"

Run Length: 60.00 min, 35998 points at 10 points/second.
Created: Sat, Feb 17, 2024 at 8:56:46 AM.
Sampled: Sequence "021624-GC5M1", Method "GC5-M1".
Analyzed using Method "GC5-M1".

Comments
GC5-M1 Analysis by Candice Warren
Column ID SPB-Vocol 105 meter X 0.53mm X 3.0µm film thickness
Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,
Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.
Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.),
Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.
FID Signal = Edaq Channel 1
Standard injection = 0.5µL, Range=3

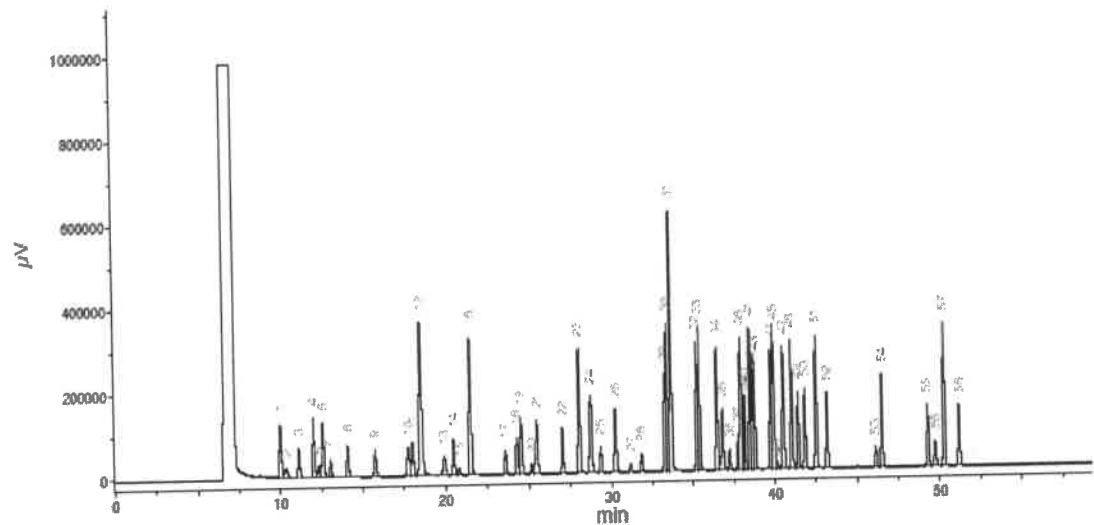

Peak #	Name	FID RT (min.)
1	Ether	9.97
2	1,1,2-Trichloro-1,2,2-trifluoroethane	10.53
3	1,1-Dichloroethane	11.10
4	Acetonitrile	12.60
5	Iodomethane	12.91
6	Allyl chloride	12.96
7	Carbon disulfide/Methylene chloride	13.04
8	trans-1,2-Dichloroethene	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,2-Dichloroethene	18.00
12	Methoxyvinylbenzene/Methyl acrylate/Chloroform	18.49
13	Isobutene/1,1,1-Trichloroethane	18.91
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethene	23.88
18	1,2-Dichloropropane	24.52
19	Methyl methacrylate	25.13
20	Bromochloropropane	25.46
21	Dibromomethane/2-Pentene	27.07
22	cis-1,2-Dichloroethene	28.03
23	Toluene	28.73
24	Ethyl methacrylate/Trans-1,2-Dichloroethene	29.34
25	1,1,2-Trichloroethane	30.34
26	Tetrachloroethane/1,2-Dichloropropane	31.16
27	Dibromochloromethane	31.84
28	1,2-Dibromomethane	33.06
29	Chlorobenzene	33.40
30	Ethylbenzene/1,1,1,2-Tetrachloroethane	33.85
31	m-Xylene/p-Xylene	35.33
32	o-Xylene	35.70
33	Styrene	35.70
34	Isopropylbenzene/Bromofarm	36.48
35	cis-1,4-Dichloro-3-butene	36.80
36	1,1,2-Trichloropropane	37.23
37	n-Propylbenzene	37.77
38	trans-1,4-Dichloro-3-butene	37.92
39	Bromobenzene	38.05
40	1,3,5-Trimethylbenzene	38.14
41	1,3,5-Trimethylbenzene	38.50
42	Chlorobenzene	38.63
43	4-Chlorobenzene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	39.91
46	Pentachloroethane	40.17
47	sec-Butylbenzene	40.52
48	p-Isopropylbenzene	41.02
49	1,3-Trichlorobenzene	41.42
50	1,4-Dichlorobenzene	41.83
51	n-Butylbenzene	42.52
52	1,2-Dichlorobenzene	42.58
53	1,2-Dibromo-3-chloropropane	46.12
54	Nitrobenzene	46.40
55	1,2,4-Trifluorobenzene	49.26
56	Hexachlorocyclopentadiene	49.72
57	Naphthalene	50.56
58	1,2,3-Trichlorobenzene	51.16

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225 H370 P271 P302,332	Highly Flammable Liquid and Vapor Cause damage to organs Use in ventilated area If on skin, wash with soap and water	H301, 311, 331 H351 P280 P305,351,338	Toxic if swallowed, skin contact, inhaled Suspected of causing cancer Use gloves, eye protection/face shield If in eyes, remove contacts, rinse with water
----------------------------------	---	--	---



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))	CAS#	% (optional)
Methanol METHYL ALCOHOL	67-56-1	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.
Storage Conditions	Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1 TWA 200 ppm
Skin notation	TWA 200 ppm
Potential for skin absorption	ingestion and inhalation.
Personal protective equipment	Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing.	Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)
UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol

IATA
UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Ree 03117/24

CERTIFIED WEIGHT REPORT

Part Number: 95317

Lot Number: 021624

Description: Universal VOA Megamix

69 components

Expiration Date: 021627

Recommended Storage: Freezer (0 °C)

Nominal Concentration (µg/mL): 2000

NIST Test ID#: BUTB

Solvent(s): Lot#
Methanol EG359-USQ12Weight(s) shown below were combined and diluted to (mL): 100.0 0.021 Balance Uncertainty
Flask Uncertainty

Formulated By:	Prashant Chauhan	021624
Reviewed By:	Pedro L. Renteria	021624
DATE		

Compound	(KMe) Part Number	Lot Number	Dir. Factor	Initial Vol. (mL)	Initial Conc. (µg/mL)	Nominal Conc. (µg/mL)	Purity (%)	Purity Uncertainty	Uncertainty Pipette (mL)	Target Weight(g)	Actual Weight(g)	Actual Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
														CAS#	OSHA PEL (TWA)	LD50
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8	40 ppm (70mg/m3/8H)	or-rat 2400mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102366	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1	1 ppm (3mg/m3/8H)	or-rat 700mg/kg
3. Carbon disulfide	(0060)	MKCR8561	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.6	8.1	75-15-0	4 ppm (12mg/m3) (skin)	or-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1196)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21056	0.21069	2001.1	8.5	1478-11-6	N/A	N/A
5. trans-1,4-Dichloro-2-butene	(0486)	MKBP9041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20746	2001.7	8.4	110-57-6	N/A	N/A
6. Diethyl ether	(0153)	IK18CAS000C	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7	N/A	N/A
7. Ethyl methacrylate	(0381)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2	N/A	N/A
8. Iodomethane	(0489)	SHBF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20121	2001.5	8.2	74-88-4	5 ppm (28mg/m3/8H) (skin)	or-rat 14800mg/kg
9. 2-Methyl-1-propanol	(0445)	15241EB	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20120	2001.4	8.1	78-83-1	50 ppm (150mg/m3/8H)	or-rat 3460mg/kg
10. Methacrylonitrile	(0442)	00427ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	128-98-7	1 ppm (3mg/m3/8H) (skin)	or-rat 120mg/kg
11. Methyl acrylate	(0755)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3	10 ppm (35mg/m3/8H) (skin)	or-rat 277mg/kg
12. Methyl methacrylate	(0404)	MKGW6137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	80-62-6	100 ppm (410mg/m3/8H)	or-rat 7872mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	98-95-3	1 ppm (5mg/m3/8H) (skin)	or-rat 780mg/kg
14. 2-Nitropropane	(0461)	HG002JK	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	78-46-9	10 ppm (35mg/m3/8H)	or-rat 720mg/kg
15. Pentachloroethane	(0460)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.6	8.3	78-01-7	N/A	N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18990	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	78-13-1	1000 ppm (7600mg/m3/8H)	or-rat 43g/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-27-4	NA	or-rat 915mg/kg
18. Dibromochloromethane	35171	101623	0.05	5.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1	N/A	or-rat 848mg/kg
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	156-59-2	N/A	N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.4	2000	NA	NA	0.017	NA	NA	1999.6	23.0	156-60-5	N/A	or-rat 1235mg/kg
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2	500 ppm	or-rat 820mg/kg
22. 1,1-Dichloroethane	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.7	20.4	75-35-4	1 ppm (4mg/m3/8H)	or-rat 200mg/kg
23. Bromoform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2	0.5 ppm (5mg/m3) (skin)	or-rat 930mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	56-23-5	2 ppm (12.6mg/m3/8H)	or-rat 2350mg/kg
25. Chloroform	95321	020724	0.10	10.00	20004.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	67-68-3	60 ppm (240mg/m3) (CL)	or-rat 908mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.9	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-95-3	N/A	or-rat 106mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7	N/A	N/A
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7	N/A	N/A
29. Trichloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	2019.8	20.8	127-18-4	25 ppm (170mg/m3/8H) (final)	or-rat 2629mg/kg
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	71-55-6	350 ppm (1900mg/m3/8H)	or-rat 10000mg/kg
31. 1,2-Dibromo-3-chloropropane	35161	112322	0.05	5.00	40016.5	2000	NA	NA	0.017	NA	NA	2000.3	22.9	96-12-8	0.001 ppm	or-rat 170mg/kg
32. 1,2-Dibromoethane	35161	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-93-4	20 ppm (8H)	or-rat 108mg/kg
33. 1,2-Dichloroethane	35161	112322	0.05	5.00	40018.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-06-2	50 ppm (8H)	or-rat 670mg/kg
34. 1,2-Dichloropropane	35161	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5	75 ppm (350mg/m3/8H)	or-rat 1847mg/kg
35. 1,3-Dichloropropane	35161	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	1999.8	22.9	142-28-9	N/A	or-rat 3600mg/kg
36. 1,1-Dichloropropene	35161	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	2000.1	28.7	563-58-6	N/A	N/A
37. cis-1,3-Dichloropropene	35161	112322	0.05	5.00	40010.0	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10061-01-5	N/A	N/A
38. trans-1,3-Dichloropropene	35161	112322	0.05	5.00	40017.6	2000	NA	NA	0.017	NA	NA	2000.4	23.0	10061-02-6	N/A	N/A
39. Hexachloro-1,3-butadiene	35161	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-68-3	0.02 ppm (0.24mg/m3/8H)	or-rat 82mg/kg
40. 1,1,1,2-Tetrachloroethane	35161	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.1	22.9	830-20-6	N/A	or-rat 670mg/kg
41. 1,1,2,2-Tetrachloroethane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	79-34-5	5 ppm (35mg/m3/8H) (skin)	or-rat 800mg/kg
42. 1,1,2-Trichloroethane	35161	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.8	23.0	79-00-5	10 ppm (45mg/m3/8H) (skin)	or-rat 936mg/kg
43. Trichloroethene	35161	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	2000.9	22.9	79-01-6	50 ppm (270mg/m3/8H)	or-mus 2402mg/kg
44. 1,2,3-Trichloropropane	35161	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	96-18-4	10 ppm (60mg/m3/8H)	or-rat 149.8mg/kg
45. Benzene	35162	050823	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2	1 ppm	or-rat 4894mg/kg
46. Bromobenzene	35162	050823	0.05	5.00	40006.0	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8	N/A	N/A
47. n-Butyl benzene	35162	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4	100 ppm (435mg/m3/8H)	or-rat >2000mg/kg
48. Ethyl benzene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	99-87-6	N/A	or-rat 4750mg/kg
49. p-Isopropyl toluene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3	10 ppm (50mg/m3/8H)	or-rat 490mg/kg
50. Naphthalene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5	100 ppm	or-rat 5000mg/kg
51. Styrene	35162	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-98-3	200 ppm	or-rat 5000mg/kg
52. Toluene	35162	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.7	22.9	87-81-6	N/A	or-rat 1390mg/kg
53. 1,2,3-Trichlorobenzene	35162	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1	5 ppm (CL) (40mg/m3)	or-rat 756mg/kg
54. 1,2,4-Trichlorobenzene	35162	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	23.0	95-63-6	N/A	or-rat 5g/kg
55. 1,2,4-Trimethylbenzene	35162	050823	0.05	5.00	40001.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-87-6	N/A	or-rat 5000mg/kg
56. 1,3,5-Trimethylbenzene	35162	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3	100 ppm (435mg/m3/8H)	or-rat 5g/kg
57. m-Xylene	35162	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	96-06-6	N/A	N/A
58. tert-Butyl benzene	35163	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	135-98-6	N/A	or-rat 2240mg/kg
59. sec-Butyl benzene	35163	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.7	22.9	108-90-7	75 ppm (350mg/m3/8H)	or-rat 2290mg/kg
60. Chlorobenzene	35163	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.5	22.9	95-49-8	50 ppm (250mg/m3/8H)	or-rat 3900mg/kg
61. 2-Chlorotoluene	35163	101923	0.05	5.00	40003.3	2000	NA	NA	0.017	NA	NA	1999.7	22.9	106-43-4	N/A	or-rat 2100mg/kg
62. 4-Chlorotoluene	35163	101923	0.05	5.00	40003.3	2000	NA	NA	0.017	NA	NA	1999.7	22.9	95-50-1	50 ppm (300mg/m3) (CL)	or-rat 500mg/kg
63. 1,2-Dichlorobenzene	35163	101923	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	23.0	541-73-1	N/A	or-mus 1060mg/kg
64. 1,3-Dichlorobenzene	35163	101923	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1999.6	22.9	108-46-7	75 ppm (450mg/m3/8H)	or-rat




Run 16, "P95317 L021624 (2000µg/mL in MeOH)"

Run Length: 60.00 min, 35998 points at 10 points/second.
Created: Sat, Feb 17, 2024 at 8:56:46 AM.
Sampled: Sequence "021624-GC5M1", Method "GC5-M1".
Analyzed using Method "GC5-M1".

Comments

GC5-M1 Analysis by Candice Warren
Column ID SPB-Vocol 105 meter X 0.53mm X 3.0µm film thickness
Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,
Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.
Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.),
Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.
FID Signal = Edaq Channel 1
Standard injection = 0.5µL, Range=3

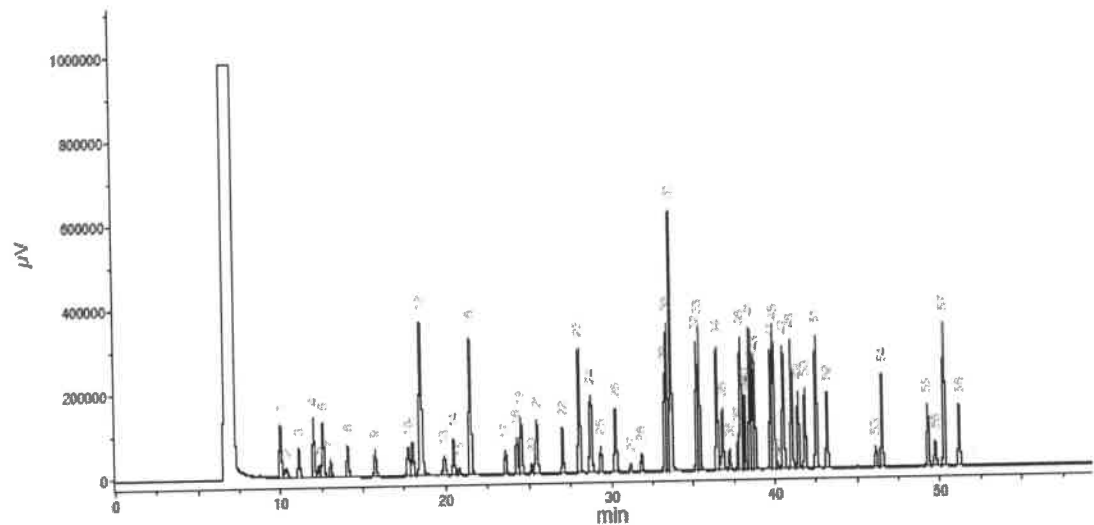

Peak #	Name	FID RT (min.)
1	Ether	9.97
2	1,1,2-Trichloro-1,2,2-trifluoroethane	10.53
3	1,1-Dichloroethane	11.10
4	Acetone	12.00
5	Isodimethane	12.21
6	Allyl chloride	12.56
7	Carbon disulfide/Methylene chloride	13.04
8	trans-1,2-Dichloroethane	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,2-Dichloroethane	18.00
12	Methyl methacrylate/Methyl acrylate/Chloroform	18.49
13	Isobutene/1,1,1-Trichloroethane	18.91
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.48
17	Trichloroethane	23.88
18	1,2-Dichloropropane	24.52
19	Methyl methacrylate	25.13
20	Bromochloropropane	25.46
21	Dibromomethane/2,2-Dichloropropane	27.07
22	cis-1,2-Dichloroethane	28.03
23	Toluene	28.73
24	Ethyl methacrylate/Trans-1,2-Dichloropropane	29.34
25	1,1,2-Trichloroethane	30.34
26	Tetrachloroethane/1,2-Dichloropropane	31.16
27	Dibromochloromethane	31.84
28	1,2-Dibromomethane	33.06
29	Chlorobenzene	33.40
30	Ethylbenzene/1,1,1,2-Tetrachloroethane	33.85
31	m-Xylene/p-Xylene	35.33
32	o-Xylene	35.70
33	Styrene	35.70
34	Isopropylbenzene/Bromofarm	36.48
35	cis-1,4-Dichloro-3-butene	36.80
36	1,1,2-Trichloropropane	37.23
37	n-Propylbenzene	37.77
38	trans-1,4-Dichloro-3-butene	37.92
39	Bromobenzene	38.05
40	1,3,5-Trimethylbenzene	38.14
41	1,3,5-Trimethylbenzene	38.50
42	Chlorobenzene	38.63
43	4-Chlorobenzene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	39.91
46	Pentachloroethane	40.17
47	sec-Butylbenzene	40.52
48	p-Isopropylbenzene	41.02
49	1,3-Trichlorobenzene	41.42
50	1,4-Dichlorobenzene	41.83
51	n-Butylbenzene	42.52
52	1,2-Dichlorobenzene	42.18
53	1,2-Dibromo-3-chloropropane	46.12
54	Nitrobenzene	46.40
55	1,2,4-Trifluorobenzene	49.28
56	Hexachlorobutadiene	49.72
57	Naphthalene	50.56
58	1,2,3-Trichlorobenzene	51.16

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225 H370 P271 P302,332	Highly Flammable Liquid and Vapor Cause damage to organs Use in ventilated area If on skin, wash with soap and water	H301, 311, 331 H351 P280 P305,351,338	Toxic if swallowed, skin contact, inhaled Suspected of causing cancer Use gloves, eye protection/face shield If in eyes, remove contacts, rinse with water
----------------------------------	---	--	---



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))	CAS#	% (optional)
Methanol METHYL ALCOHOL	67-56-1	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.
Storage Conditions	Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1 TWA 200 ppm
Skin notation	TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.	
Personal protective equipment	Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.	

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Certified Reference Material CRM



Dec 09/17/24

CERTIFIED WEIGHT REPORT

Part Number:

91980

Lot Number:

091424

Description:

Acrolein

Solvent(s):

Water

Lot#

072324Q

Expiration Date:

101424

Recommended Storage:

Refrigerate (4 °C)

Nominal Concentration (µg/mL):

5000

NIST Test ID#:

6UTB

5E-05 Balance Uncertainty

0.001 Flask Uncertainty

10.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	-------------	------------------	------------------	---------------------	------------------------------------	--	------	----------------	------

1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg
-------------	---	------------	------	----	-----	---------	---------	--------	------	----------	---------	-----------------

Method: GC/MSD-1, Detector: Mass Selective Detector (Scan mode). Columns: Vocol (60m X 0.25mm ID X 1.5µm film thickness), Oven Profile: Temp. 1 = 35°C (Time 1 = 0min.), Temp. 2 = 200°C (Time 2 = 8.75 min.), Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas, NOTE: Due to the instability of acrolein in solution, all solutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

TIC: [BSB2]79005.D

Scan 232 (8.927 min): [BSB2]79005.D

Abundance

27

250000

8.93

200000

C=CC=O

50000

56

150000

40000

30000

20000

50000

10000

37

Time-->

10.00 15.00 20.00 25.00 30.00 35.00 40.00 45.00 50.00 55.00 60.00

m/z-->

0

20 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170

44 65 75 85 119 158 169

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM



Dec 09/17/24

CERTIFIED WEIGHT REPORT

Part Number:

91980

Lot Number:

091424

Description:

Acrolein

Solvent(s):

Water

Lot#

072324Q

Expiration Date:

101424

Recommended Storage:

Refrigerate (4 °C)

Nominal Concentration (µg/mL):

5000

NIST Test ID#:

6UTB

5E-05 Balance Uncertainty

0.001 Flask Uncertainty

10.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	-------------	------------------	------------------	---------------------	------------------------------------	--	------	----------------	------

1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg
-------------	---	------------	------	----	-----	---------	---------	--------	------	----------	---------	-----------------

Method: GC/MSD-1, Detector: Mass Selective Detector (Scan mode). Columns: Vocol (60m X 0.25mm ID X 1.5µm film thickness), Oven Profile: Temp. 1 = 35°C (Time 1 = 0min.), Temp. 2 = 200°C (Time 2 = 8.75 min.), Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas, NOTE: Due to the instability of acrolein in solution, all solutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

TIC: [BSB2]79005.D

Scan 232 (8.927 min): [BSB2]79005.D

Abundance

27

250000

8.93

200000

C=CC=O

50000

56

150000

40000

30000

20000

50000

10000

37

Time-->

10.00 15.00 20.00 25.00 30.00 35.00 40.00 45.00 50.00 55.00 60.00

m/z-->

0

20 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170

44 65 75 85 119 158 169

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
 * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
 * All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
 * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Rec 1216124
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB


✓ 14630 to
✓ 14649

Weight(s) shown below were combined and diluted to (mL):

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8 N/A or-rat 250mg/kg

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp = 220°C. Analyst: Candice Warren.

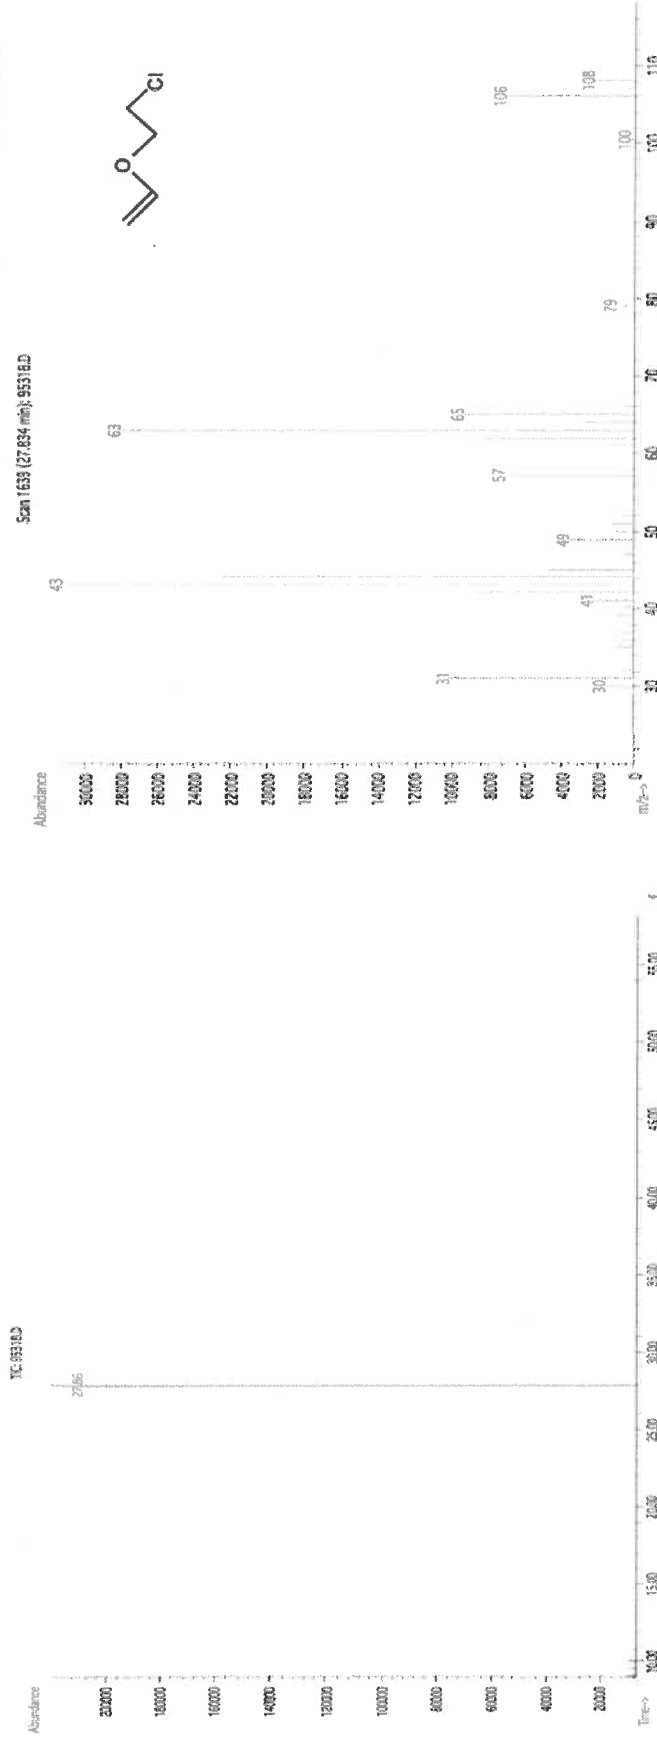

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr.	Emergency Telephone International	1-352-323-3500
	Hamden CT, 06514	Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))		% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1	67-56-1	TWA 200 ppm
Skin notation			TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.			
Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use.	Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.			

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Dec 12/6/24
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB


✓ 14630 to
✓ 14649

Weight(s) shown below were combined and diluted to (mL):

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8 N/A or-rat 250mg/kg

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp = 220°C. Analyst: Candice Warren.

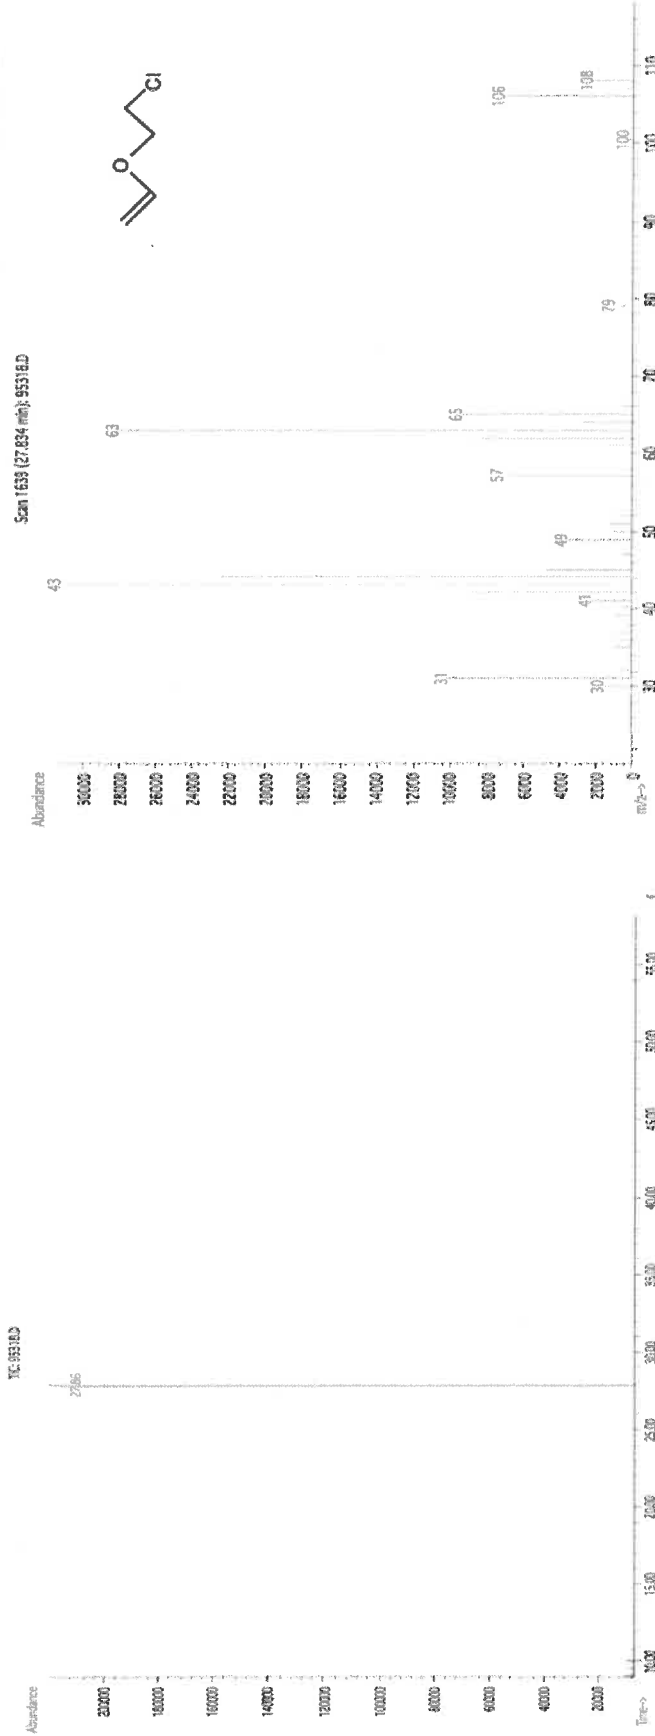

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr.	Emergency Telephone International	1-352-323-3500
	Hamden CT, 06514	Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))		% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1	67-56-1	TWA 200 ppm
Skin notation			TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.			
Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use.	Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.			

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Dec 12/16/24
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB

✓ 14630 to
✓ 14649

Weight(s) shown below were combined and diluted to (mL):


5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Expanded Uncertainty (Solvent Safety Info. On Attached pg.)
Uncertainty (±) (µg/mL) CAS# OSHA PEL (TWA) LDSO

SDS Information

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LDSO
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	or-rat 250mg/kg

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

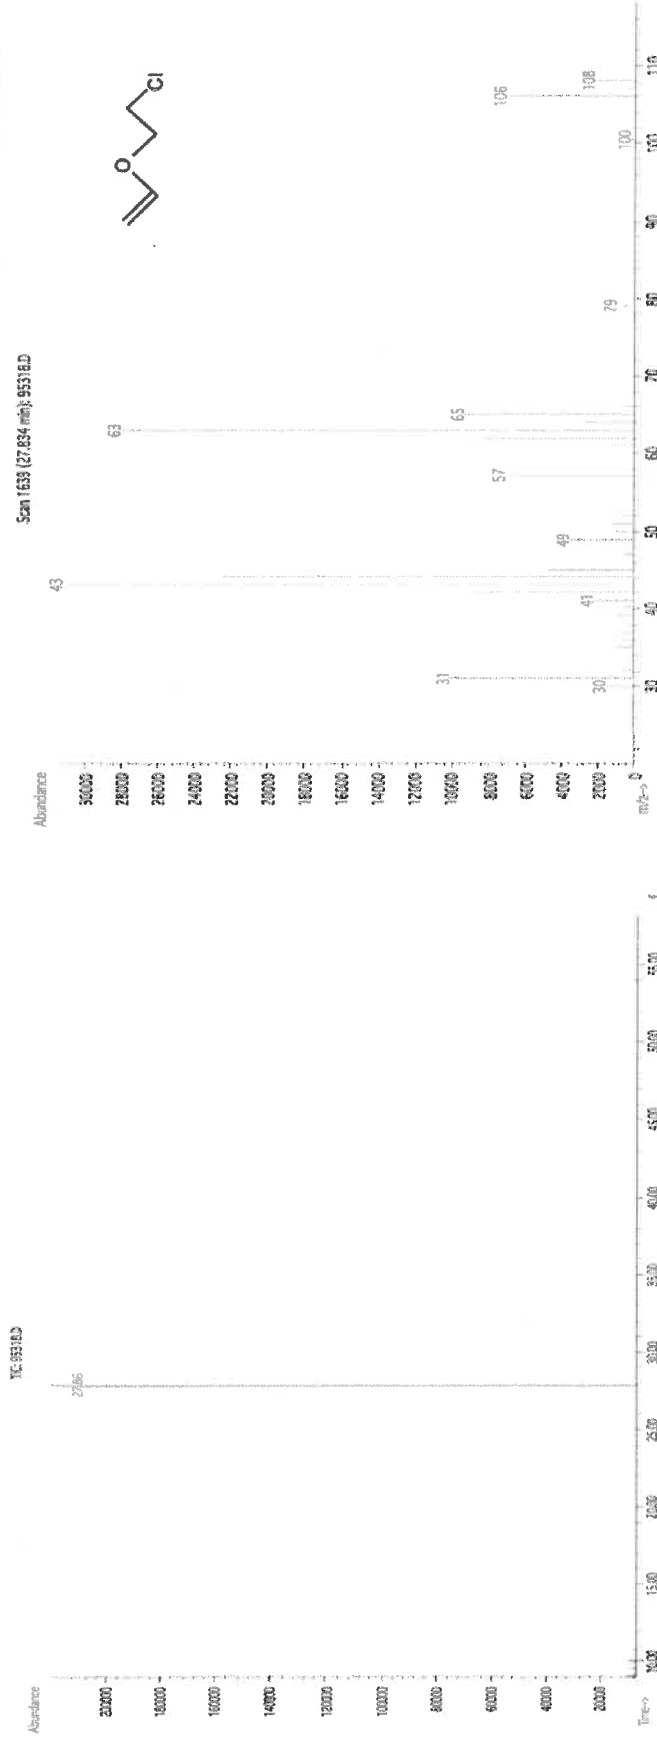

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rosotto Dr. Hamden CT. 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302, 332	If on skin, wash with soap and water	P305, 351, 338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))	CAS#	% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1 TWA 200 ppm		
Skin notation	TWA 200 ppm		
Potential for skin absorption, ingestion and inhalation.			
Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use.	Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.			

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



See 1216124
20 vial

CERTIFIED WEIGHT REPORT

Part Number: 95318
Lot Number: 120524
Description: 2-Chloroethyl vinyl ether

Solvent(s): Lot#
Methanol EJ143-US

Expiration Date: 120527
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 10000
NIST Test ID#: 6UTB

Weight(s) shown below were combined and diluted to (mL):


5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Formulated By: Prashant Chauhan 120524
Reviewed By: Pedro L. Rentas 120524

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information	
										(Solvent Safety Info. On Attached pg.)	LD50

1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	or-rat 250mg/kg
------------------------------	----	----------	-------	----	-----	---------	---------	---------	------	----------	-----	-----------------

Method: GC6MSD-1.M. Detector: MSD. Column: (60m X 0.25mm X 1.5 µm). Oven Profile: Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp = 200°C, Detector B Temp. = 220°C. Analyst: Candice Warren.

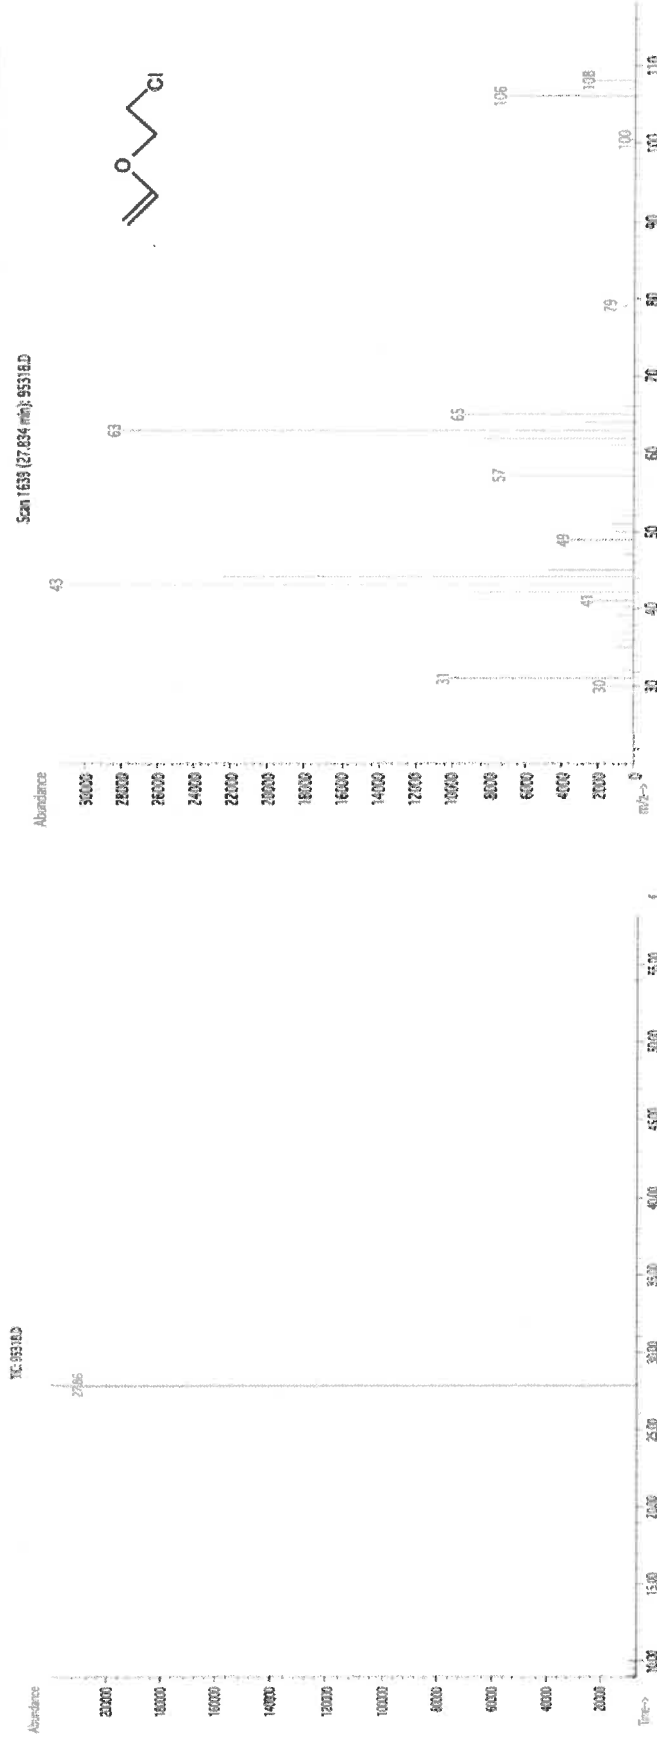

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr.	Emergency Telephone International	1-352-323-3500
	Hamden CT, 06514	Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))		% (optional)
Methanol	METHYL ALCOHOL	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability	Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol	67-56-1	67-56-1	TWA 200 ppm
Skin notation			TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.			
Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use.	Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.			

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	Vapours may form explosive mixture with air.
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
Hazardous decomposition products formed under fire conditions.	- Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
LC50 Inhalation - rat - 4 h - 64000 ppm
LD50 Dermal - rabbit - 15,800 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
EC50 24,500.00 mg/l - 48 h
EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)	IATA
UN number: 1230 Class: 3 Packing group: II	UN number: 1230 Class: 3 Packing group: II
Proper shipping name: Methanol	Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30067 **Lot No.:** A0191805

Description : 4-Bromofluorobenzene Standard

4-Bromofluorobenzene Standard 2,500µg/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2027 **Storage:** 0°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	2,483.9 µg/mL	+/- 139.5488

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:


40 ml/min

Inj. Vol

1µl

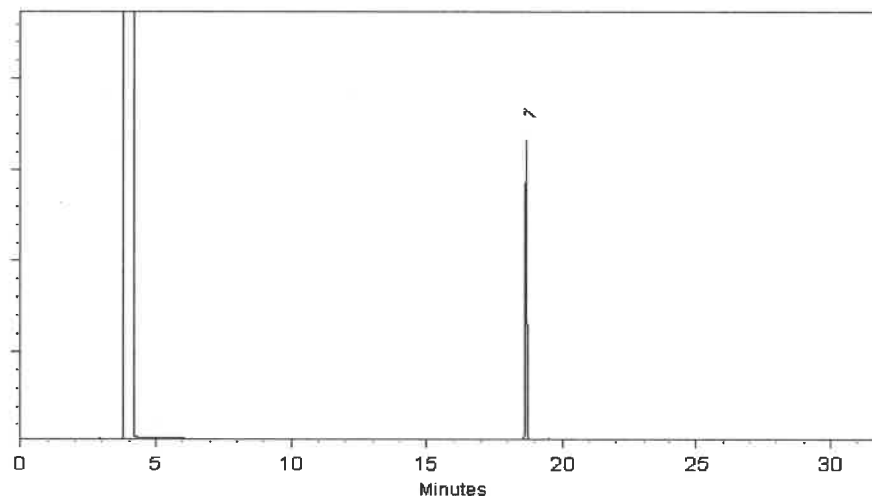

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Alicia Leathers - Operation Technician I

Date Mixed: 17-Nov-2022

Balance Serial # B251644995


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Nov-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555582 **Lot No.:** A0196865

Description : Custom 8260A/B Surrogate Mix
Custom 8260A/B Surrogate Mix 25,000µg/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2026 **Storage:** 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2-Dichloroethane-d4	17060-07-0	PR-32845	99%	25,036.0 µg/mL	+/- 1,417.9179
2	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	25,132.0 µg/mL	+/- 1,423.3549
3	Dibromofluoromethane	1868-53-7	022013	99%	25,040.0 µg/mL	+/- 1,418.1445
4	Toluene-d8	2037-26-5	PR-33397	99%	25,028.0 µg/mL	+/- 1,417.4648

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Russ Bookhamer - Operations Technician I

Date Mixed: 11-Apr-2023

Balance: 1127510105

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30489 **Lot No.:** A0209618

Description : 8260B Acetates Mix
8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2025 **Storage:** -20°C or colder

Handling: This product is photosensitive. **Ship:** On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

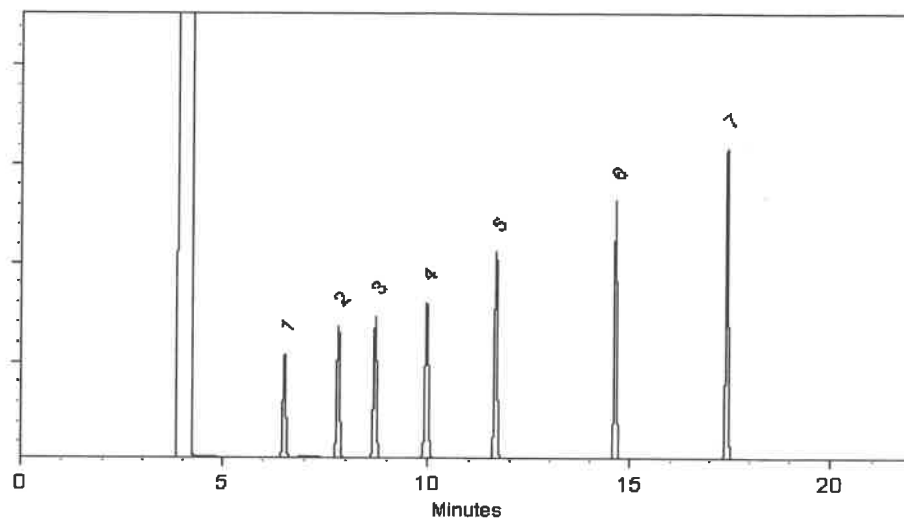

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 28-Mar-2024

Balance Serial # B707717271

Dillon Murphy
Dillon Murphy - Operations Technician I

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30489 **Lot No.:** A0209618

Description : 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : September 30, 2025 **Storage:** -20°C or colder

Handling: This product is photosensitive. **Ship:** On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

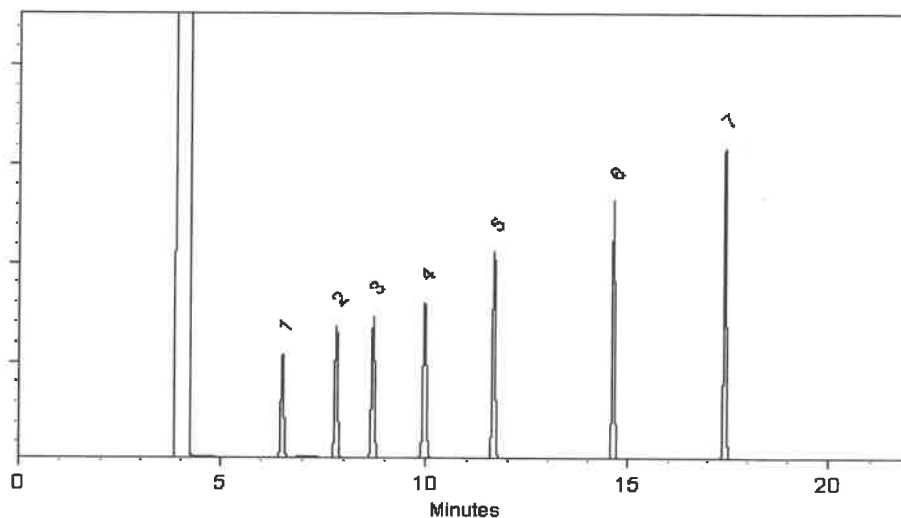

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 28-Mar-2024

Balance Serial # B707717271

Dillon Murphy
Dillon Murphy - Operations Technician I

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

gravimetric



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555581 Lot No.: A0210184

Description: Custom 8260 Internal Standard Mix

Custom 8260 Internal Standard Mix
25,000µg/mL, P&T Methanol,
1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: April 30, 2027 Storage: 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	25,212.0 µg/mL	+/- 1,427.8857
2	1,4-Difluorobenzene	540-36-3	MKCS8657	99%	25,220.0 µg/mL	+/- 1,428.3388
3	Chlorobenzene-d5	3114-55-4	PR-31132	99%	25,116.0 µg/mL	+/- 1,422.4487
4	Pentafluorobenzene	363-72-4	MKCR9383	99%	25,180.0 µg/mL	+/- 1,426.0734

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

John Friedline - Operations Technician I

Date Mixed: 11-Apr-2024 Balance: 1127510105



Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Dec 12/17/24
30 v. 4
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus

V14697-to-14726



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006 **Lot No.:** A0210618

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000µg/mL, P&T Methanol/Water(90:10), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2027 **Storage:** 0°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 µg/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 µg/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 µg/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 µg/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)
CAS # 67-56-1/7732-18-5
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

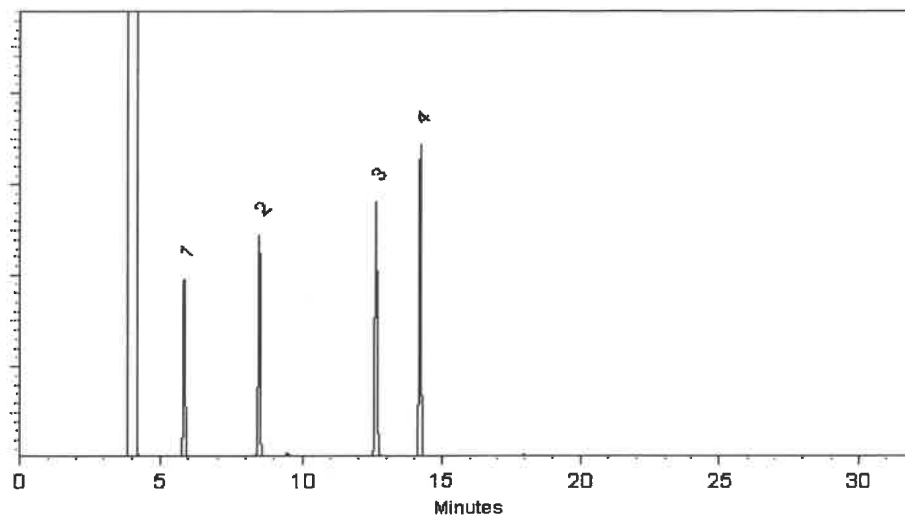


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B707717271


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Dec 12/17/24
30 v. 4
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus
V14697-to-14726



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006 **Lot No.:** A0210618
Description : VOA Calibration Mix #1
VOA Calibration Mix #1 5,000µg/mL, P&T Methanol/Water(90:10), 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : July 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 µg/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 µg/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 µg/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 µg/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)
CAS # 67-56-1/7732-18-5
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

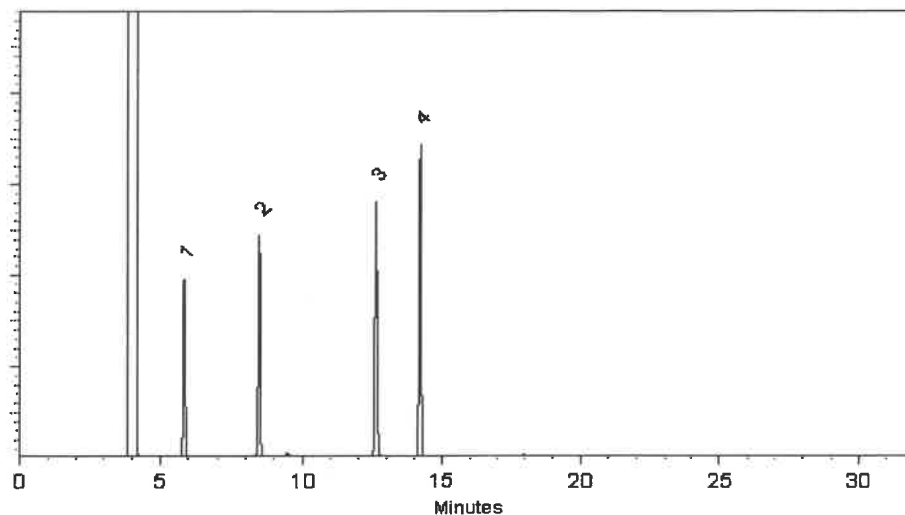


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B707717271


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Dec 12/17/24
30 v. 4
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus
V14697-to-14726



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006 **Lot No.:** A0210618
Description : VOA Calibration Mix #1
VOA Calibration Mix #1 5,000µg/mL, P&T Methanol/Water(90:10), 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : July 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 µg/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 µg/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 µg/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 µg/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)
CAS # 67-56-1/7732-18-5
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

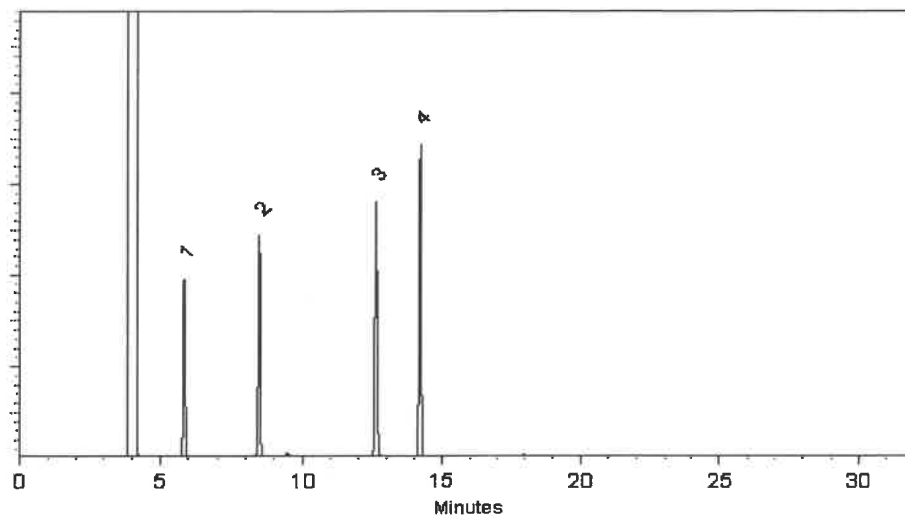


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B707717271


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Dec 12/17/24
30 v. 4
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus
V14697-to-14726



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006 **Lot No.:** A0210618
Description : VOA Calibration Mix #1
VOA Calibration Mix #1 5,000µg/mL, P&T Methanol/Water(90:10), 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : July 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 µg/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 µg/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 µg/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 µg/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)
CAS # 67-56-1/7732-18-5
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

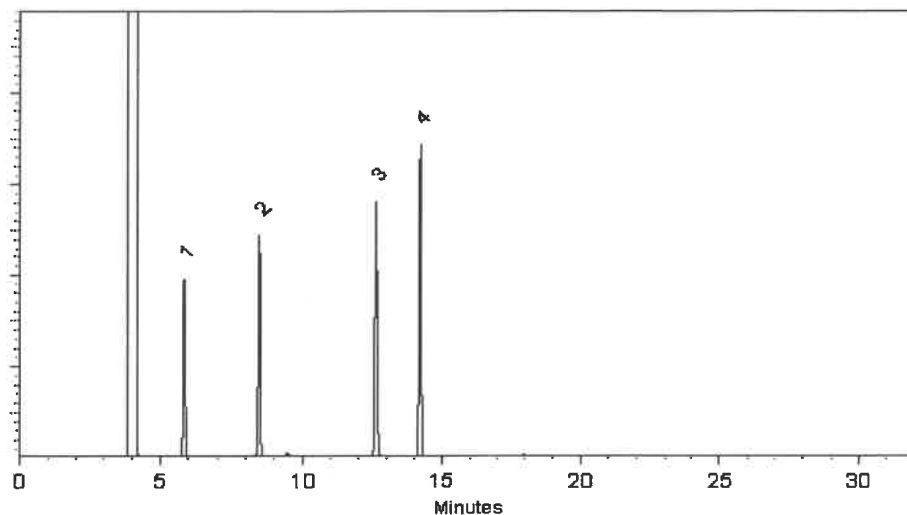


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B707717271


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

10 vial.
Dec: 12/09/24
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus
V14667-5
V14676



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30225 **Lot No.:** A0214960
Description : Bromochloromethane Standard
Bromochloromethane 2000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : August 31, 2029 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	SYN240416CTH	99%	2,012.0 µg/mL	+/- 113.0519

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

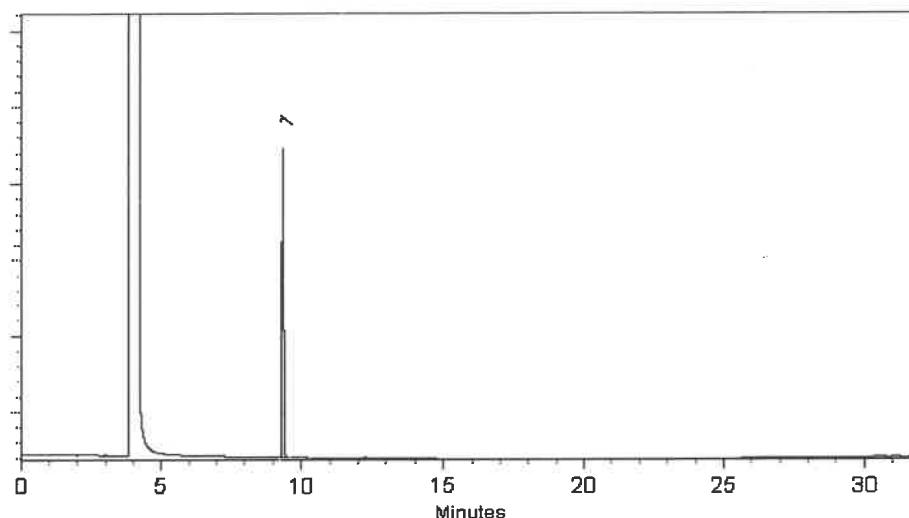

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 08-Aug-2024

Balance Serial # 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

10 vial.
Dec: 12/09/24
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus
V14667
V14676



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30225 **Lot No.:** A0214960
Description : Bromochloromethane Standard
Bromochloromethane 2000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : August 31, 2029 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	SYN240416CTH	99%	2,012.0 µg/mL	+/- 113.0519

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

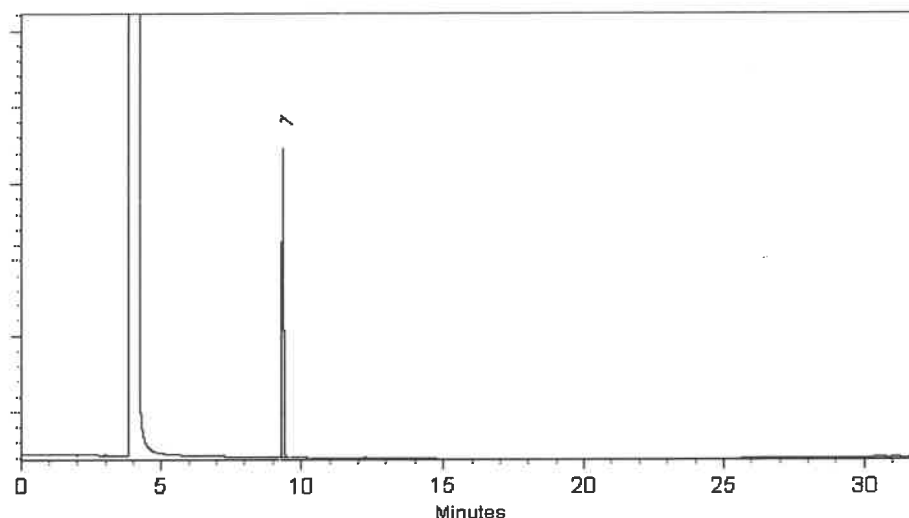

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 08-Aug-2024

Balance Serial # 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

10 vial.
CERTIFIED REFERENCE MATERIAL

Dec: 12/09/24

Certificate of Analysis

chromatographic plus

V14667-5

V14676



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30225 **Lot No.:** A0214960
Description : Bromochloromethane Standard
Bromochloromethane 2000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : August 31, 2029 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	SYN240416CTH	99%	2,012.0 µg/mL	+/- 113.0519

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

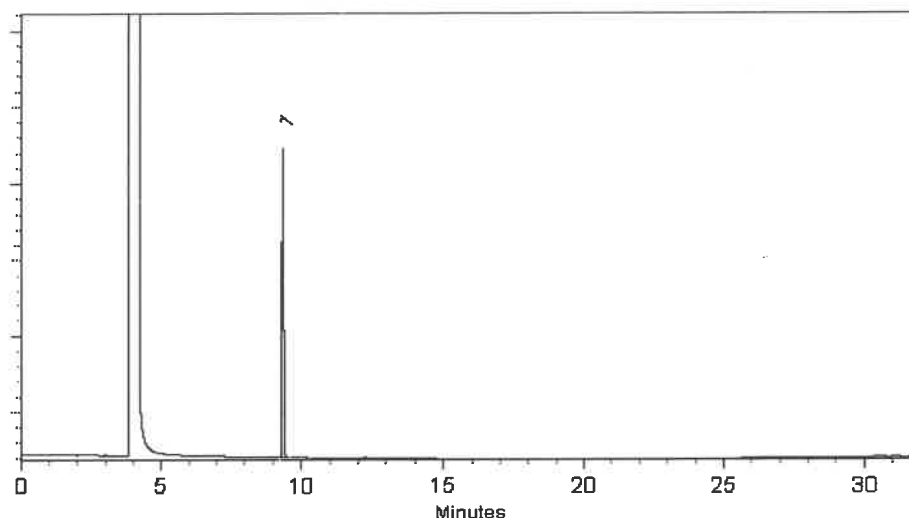

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 08-Aug-2024

Balance Serial # 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

10 vial.
Dec: 12/09/24
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus

V14667-5
V14676



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30225 **Lot No.:** A0214960
Description : Bromochloromethane Standard
Bromochloromethane 2000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : August 31, 2029 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	SYN240416CTH	99%	2,012.0 µg/mL	+/- 113.0519

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

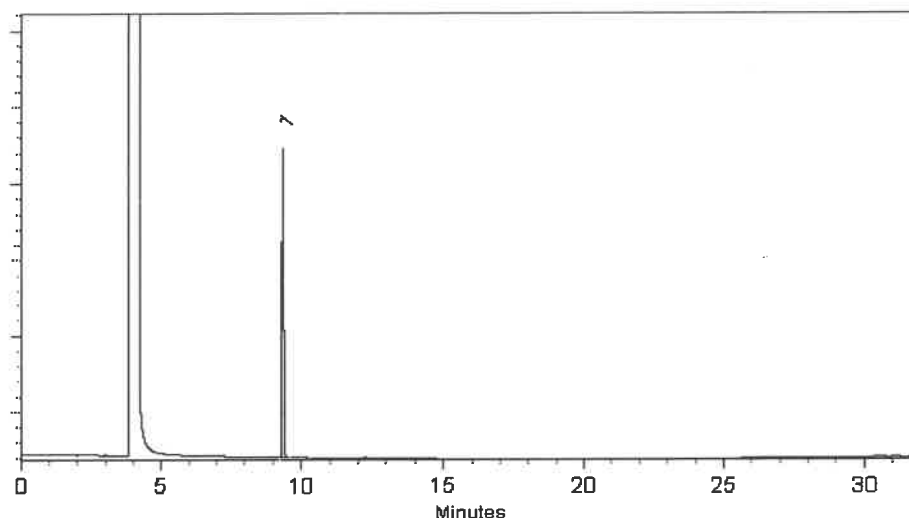

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Stacey Wanner - Operations Technician I

Date Mixed: 08-Aug-2024

Balance Serial # 1127510105

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 14-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Rec 12/17/24
CERTIFIED REFERENCE MATERIAL

30 ml
Certificate of Analysis
chromatographic plus

V14727 to
V14756



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30042 **Lot No.:** A0216826
Description : 502.2 Calibration Mix #1
502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : May 31, 2031 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4µm
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant flow 2.0 mL/min.

Temp. Program:

40°C (hold 6 min.) to 100°C
@ 6°C/min.

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

Split ratio 10:1

Inj. Vol

1µl

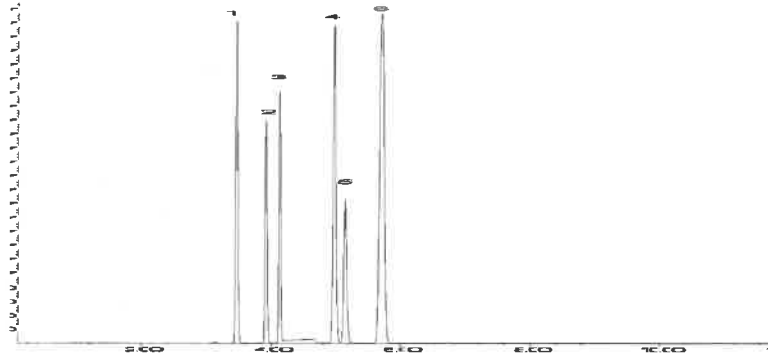

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.



Tom Suckal - Mix Technician

Date Mixed: 23-Sep-2024

Balance Serial # B707717271



Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Rec 12/17/24
30 ml
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus

V14727 to
V14756



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30042 **Lot No.:** A0216826
Description : 502.2 Calibration Mix #1
502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : May 31, 2031 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4µm
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant flow 2.0 mL/min.

Temp. Program:

40°C (hold 6 min.) to 100°C
@ 6°C/min.

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

Split ratio 10:1

Inj. Vol

1µl

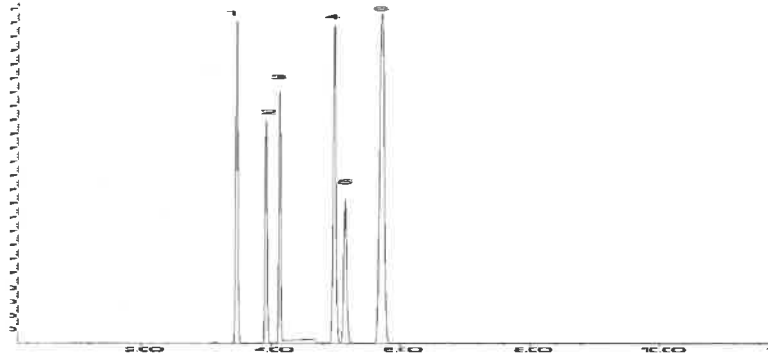

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckal - Mix Technician

Date Mixed: 23-Sep-2024

Balance Serial # B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus

✓ 14842 to 14846



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30470 **Lot No.:** A0217535
Description : tert-Butanol Standard
tert-Butanol Std 50,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : October 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	tert-Butanol (TBA)	75-65-0	SHBQ8002-1	99%	50,007.5 µg/mL	+/- 717.6137

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

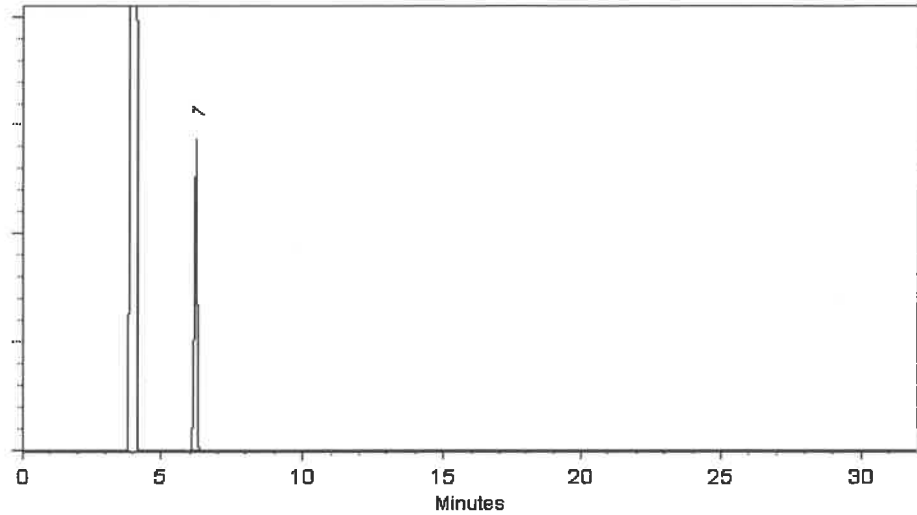

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. E.
Aaron Enyart - Operations Tech I

Date Mixed: 07-Oct-2024

Balance Serial # B251644995

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 09-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

2014 Dec 01/08/21
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic

V14803 - V14822



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555408-SL **Lot No.:** A0220471
Description : Custom Vinyl Acetate Standard
Custom Vinyl Acetate Standard 8,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : June 30, 2026 **Storage:** -20°C or colder
Handling: This product is photosensitive. **Ship:** On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 µg/mL	+/- 278.7979

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

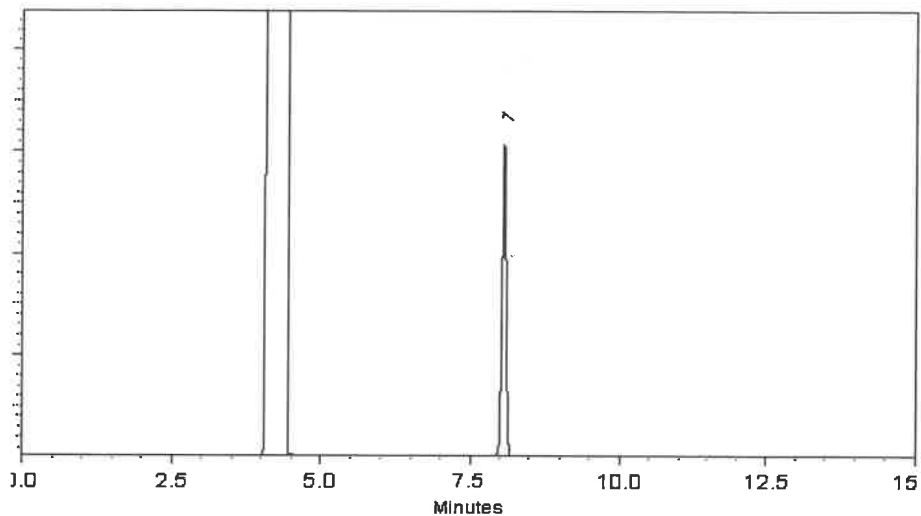

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024

Balance Serial # 1127510105

Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED
By Jennifer Pollock at 7:12 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

2014 Dec 01/08/21
CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic

V14803 - V14822



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555408-SL **Lot No.:** A0220471
Description : Custom Vinyl Acetate Standard
Custom Vinyl Acetate Standard 8,000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : June 30, 2026 **Storage:** -20°C or colder
Handling: This product is photosensitive. **Ship:** On Ice

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 µg/mL	+/- 278.7979

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1µl

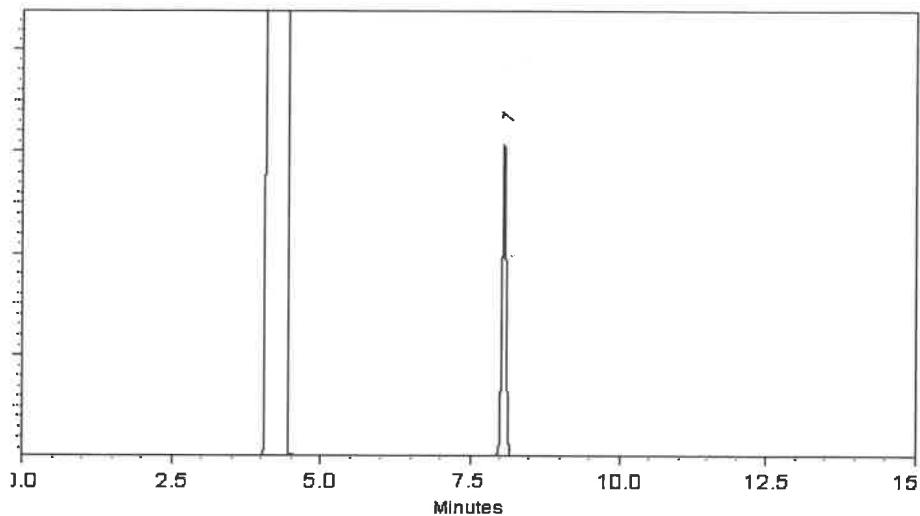

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024

Balance Serial # 1127510105

Dillan Murphy - Operations Technician I

Date Passed: 02-Jan-2025

REVIEWED
By Jennifer Pollock at 7:12 am, Jan 05, 2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

Rec 05/09/25
Avantor™



*V14921 to
V14938*

Material No.: 9077-02
Batch No.: 24G0262002
Manufactured Date: 2024-05-14
Expiration Date: 2027-05-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Titration Acid (μeq/g)	≤ 0.3	0.3
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis - Below EPA 82608 CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Mark
Jamie Croak
Director Quality Operations, Bioscience Production

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



V14921 to
V14938

Material No.: 9077-02
Batch No.: 24G0262002
Manufactured Date: 2024-05-14
Expiration Date: 2027-05-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Titration Acid (μeq/g)	≤ 0.3	0.3
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis - Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Mark
Jamie Croak
Director Quality Operations, Bioscience Production



Certified Reference Material CRM

see 05/21/25



CERTIFIED WEIGHT REPORT

Part Number: **91980**
Lot Number: **051925**
Description: **Acrolein**

Solvent(s):
Water Lot# 041725Q

5.019

114944-114948

		051925
Formulated By:	Lawrence Barry	DATE
		051925
Reviewed By:	Pedro L. Rentas	DATE



Expiration Date: 061925
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 5000
NIST Test ID#: 6UTB

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5µm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

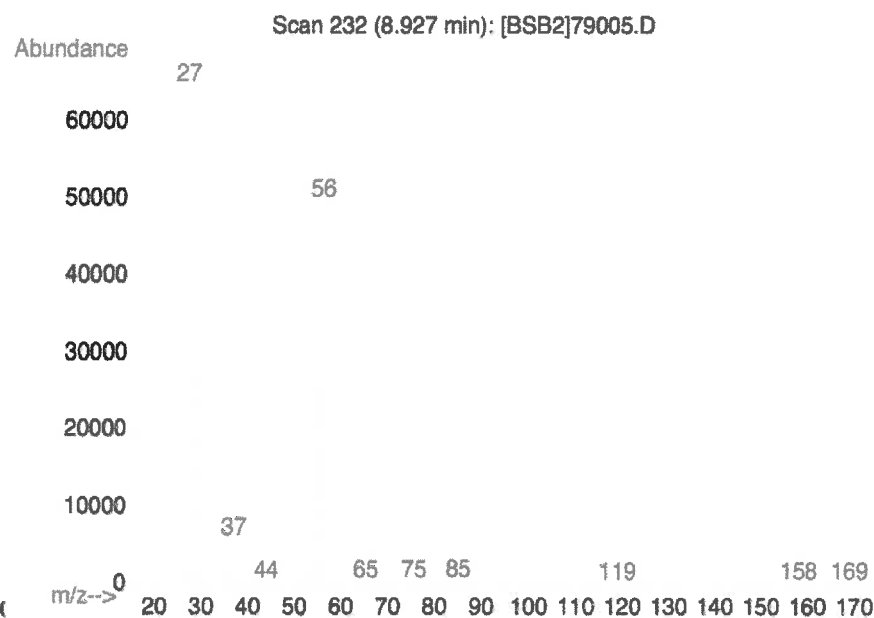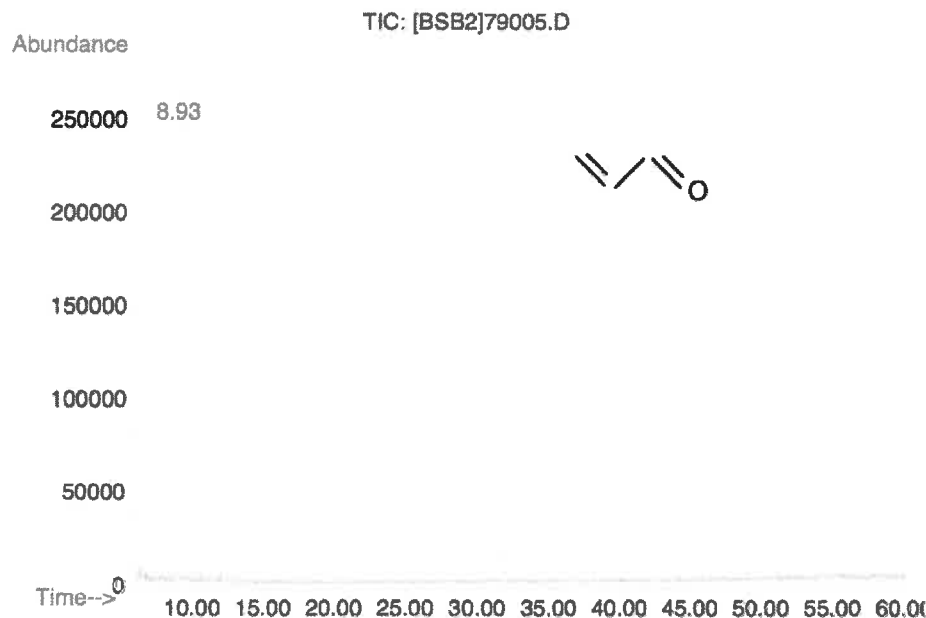

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
 - Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
 - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
 - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
- Rev 1.0, 2/25/2025



Certified Reference Material CRM

see 05/21/25



CERTIFIED WEIGHT REPORT

Part Number: **91980**
Lot Number: **051925**
Description: **Acrolein**

Solvent(s):
Water Lot# 041725Q

5.019

114944-114948

		051925
Formulated By:	Lawrence Barry	DATE
		051925
Reviewed By:	Pedro L. Rentas	DATE



Expiration Date: 061925
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 5000
NIST Test ID#: 6UTB

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5µm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

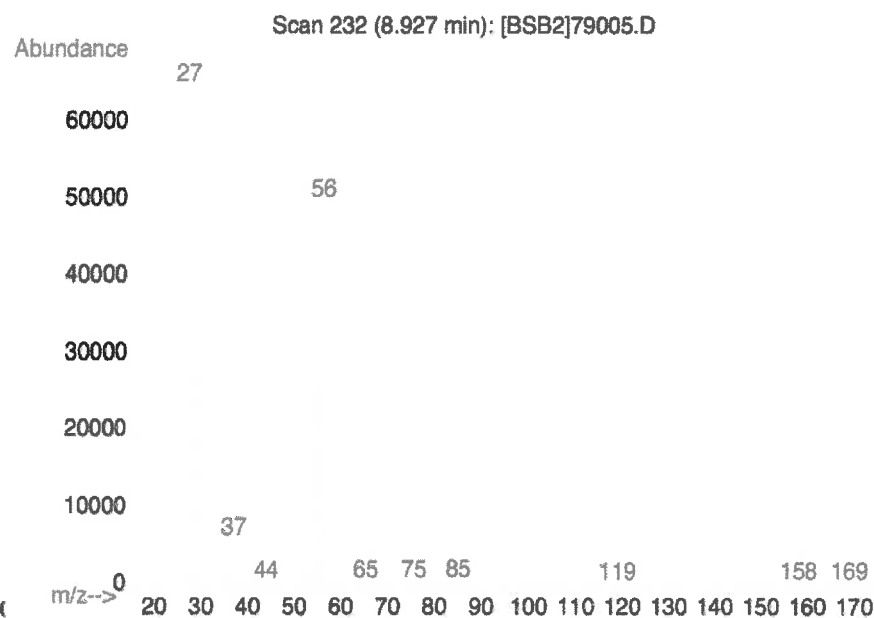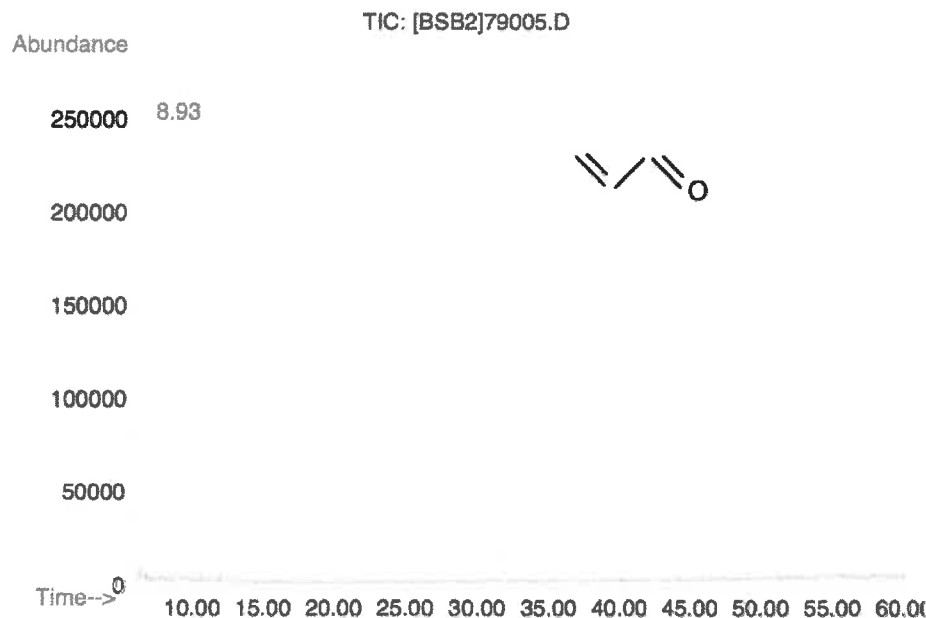

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
 - Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
 - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
 - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
- Rev 1.0, 2/25/2025



Certified Reference Material CRM

see 05/21/25



CERTIFIED WEIGHT REPORT

Part Number: **91980**
Lot Number: **051925**
Description: **Acrolein**

Solvent(s):
Water Lot# 041725Q

5.019

114944-114948

		051925
Formulated By:	Lawrence Barry	DATE
		051925
Reviewed By:	Pedro L. Rentas	DATE



Expiration Date: 061925
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 5000
NIST Test ID#: 6UTB

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5µm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

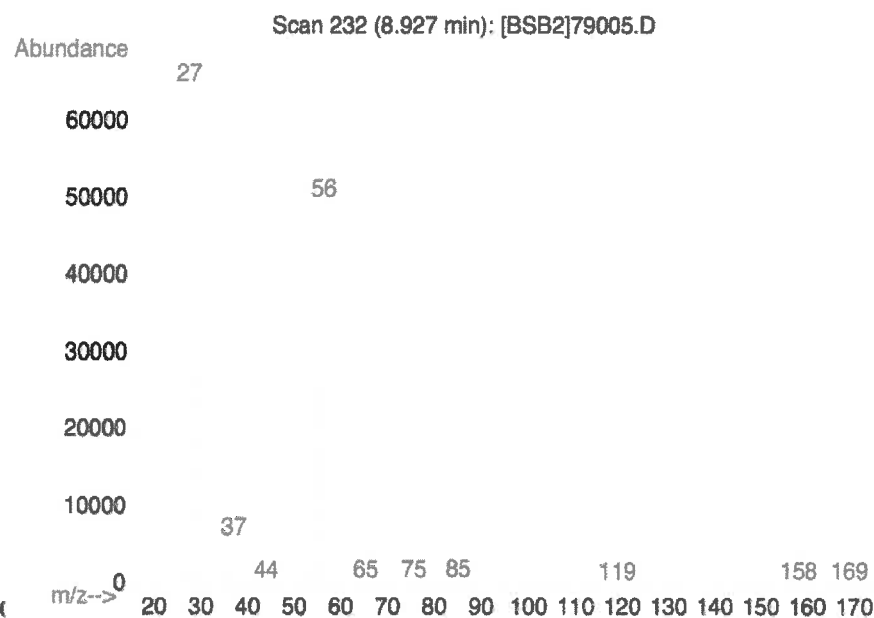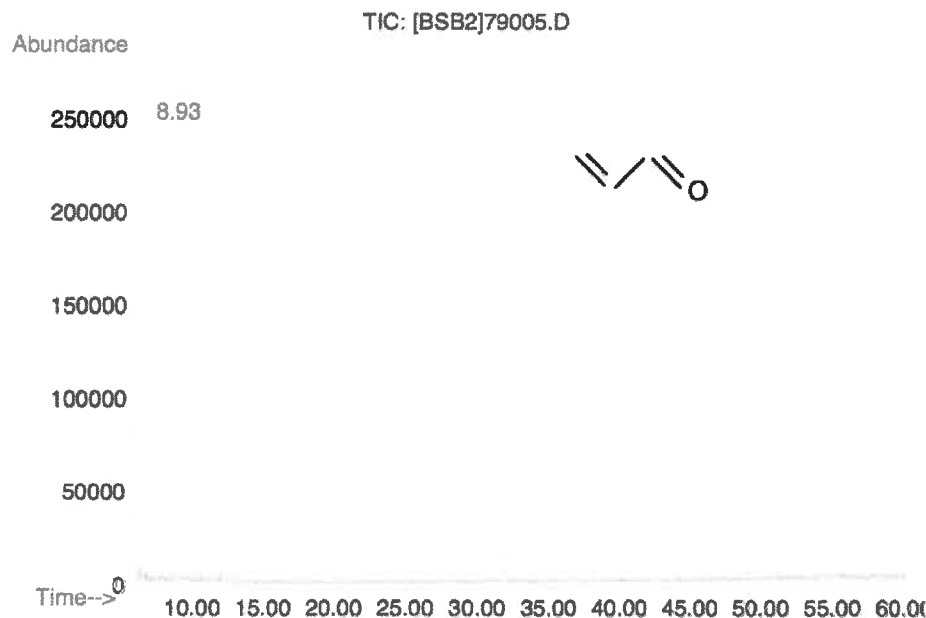

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
 - Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
 - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
 - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
- Rev 1.0, 2/25/2025



Certified Reference Material CRM

see 05/21/25



CERTIFIED WEIGHT REPORT

Part Number: 91980
Lot Number: 051925
Description: Acrolein

Solvent(s): Water
Lot#: 041725Q

5.019

114944-114948

		051925
Formulated By:	Lawrence Barry	DATE
		051925
Reviewed By:	Pedro L. Rentas	DATE



Expiration Date: 061925
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 5000
NIST Test ID#: 6UTB

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05170	5004.1	52.5	107-02-8	0.1 ppm	ori-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5µm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately. Long term storage is not recommended. Please contact our technical department if further information is required.

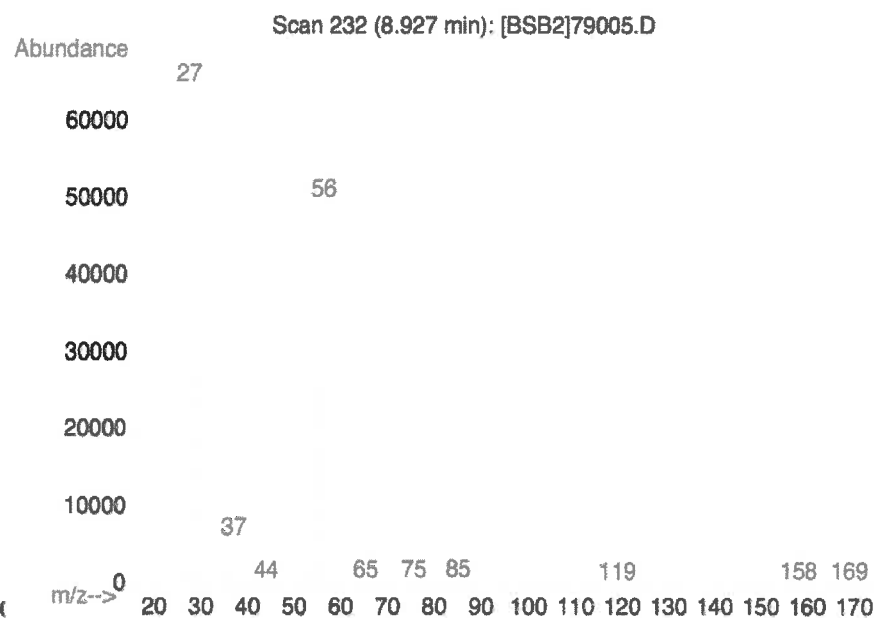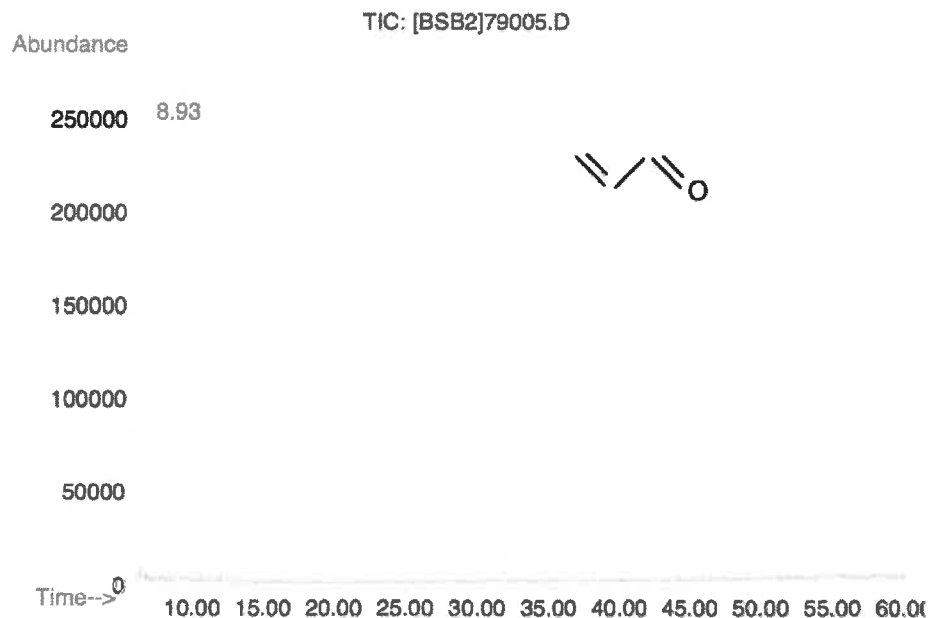

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 - Standards are prepared gravimetrically using balances that are calibrated by an ISO 17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
 - Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
 - All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
 - Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).
- Rev 1.0, 2/25/2025



SHIPPING DOCUMENTS

CLIENT INFORMATION

CLIENT PROJECT INFORMATION

CLIENT BILLING INFORMATION

REPORT TO BE SENT TO:
COMPANY: Jacobs
ADDRESS: 412 Mt. Kemble Ave., Suite 100
CITY: Morrisstown STATE: NJ ZIP: 07960
ATTENTION: John Vinfante, John.Vinfante@Jacobs.com
PHONE: _____ FAX: _____

PROJECT NAME: StC Princeton
PROJECT NO.: D3868221 LOCATION: Princeton Junction
PROJECT MANAGER: Mary Murphy
e-mail: Mary.Murphy@Jacobs.com
PHONE: _____ FAX: _____

BILL TO: Mary Murphy PO#: _____
ADDRESS: _____
CITY: _____ STATE: _____ ZIP: _____
ATTENTION: _____ PHONE: _____

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) Standard TAT DAYS*
HARDCOPY (DATA PACKAGE): _____ DAYS*
EDD: _____ DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP
☒ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other _____
☐ EDD FORMAT

1. Site Specific VOCs (52605-1000)
2. 114-Dioxane (182705-500)
3. Total Metals (166705-500)
4. Dissolved Iron (166705-500)
5. Alkalinity (15m 420B)
6. TDS (5m 2540C)
7. Anions (9066)
8. Trace VOCs (5FAMOL-1-500)
9.

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS	
			COMP	GRAB	DATE	TIME		A/E	E	B/E	B/E	E	E	E	A/E			← Specify Preservatives A-HCl D-NaOH B-HNO3 E-ICE C-H2SO4 F-OTHER
								1	2	3	4	5	6	7	8	9		
1.	MW-17B-55-060425	GW		X	6/4/25	1140	20	X	X	X	X	X	X	X			MS/MSD*	
2.	MW-17B-55-060425-SIM	GW		X	6/4/25	1145	3								X			
3.	MW-18B-56-060425	GW		X	6/4/25	1230	7		X	X	X	X	X	X				
4.	MW-18B-56-060425-FD	GW		X	6/4/25	1250	7		X	X	X	X	X	X				
5.	MW-19B-72-060425	GW		X	6/4/25	1550	7		X	X	X	X	X	X				
6.																		
7.																		
8.																		
9.																		
10.																		

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: _____ DATE/TIME: _____ RECEIVED BY: 6-5-25
1. [Signature] 6/4/25 1830 1. [Signature] 0700
RELINQUISHED BY SAMPLER: _____ DATE/TIME: _____ RECEIVED BY: _____
2. _____ 2. _____
RELINQUISHED BY SAMPLER: _____ DATE/TIME: _____ RECEIVED BY: _____
3. _____ 3. _____

Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 1.8°C

Comments: See work order for list of site specific VOCs

*MW-17B MS/MSD is for total metals, dissolved iron, alkalinity, TDS, and anions only
- Dissolved iron is field filtered
- PO# 148064311; 3 sample coolers

Page 1 of 2 CLIENT: ☐ Hand Delivered ☐ Other

Shipment Complete

☐ YES ☐ NO

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q2234	JACO05	Order Date : 6/5/2025 10:52:00 AM	Project Mgr :
Client Name : JACOBS Engineering Grou		Project Name : Former Schlumberger STC	Report Type : Level 3
Client Contact : John Ynfante		Receive DateTime : 6/5/2025 7:00:00 AM	EDD Type : CH2MHILL
Invoice Name : JACOBS Engineering Grou		Purchase Order :	Hard Copy Date :
Invoice Contact : John Ynfante			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q2234-01	MW-17B-55-060425	Water	06/04/2025	11:40					
					VOCMS Group3		8260-Low	10 Bus. Days	
Q2234-04	MW-17B-55-060425-SIM	Water	06/04/2025	11:40					
				11:45	VOC-TRACE-SFAM		SFAM_Trace	10 Bus. Days	

Relinquished By :

Date / Time :

Received By :

Date / Time :

Storage Area : VOA Refridgerator Room