

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060625\
 Data File : P0111523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2025 14:30
 Operator : YP/AJ
 Sample : Q2236-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 WC-A2-07-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/09/2025
 Supervised By :mohammad ahmed 06/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 16:52:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.679	3.675	107.0E6	92899738	18.182m	17.041m
2) SA Decachlor...	8.718	8.667	84570658	30579984	16.381	16.528

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060625\
Data File : PO111523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2025 14:30
Operator : YP/AJ
Sample : Q2236-18
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-A2-07-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2025
Supervised By :mohammad ahmed 06/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 16:52:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

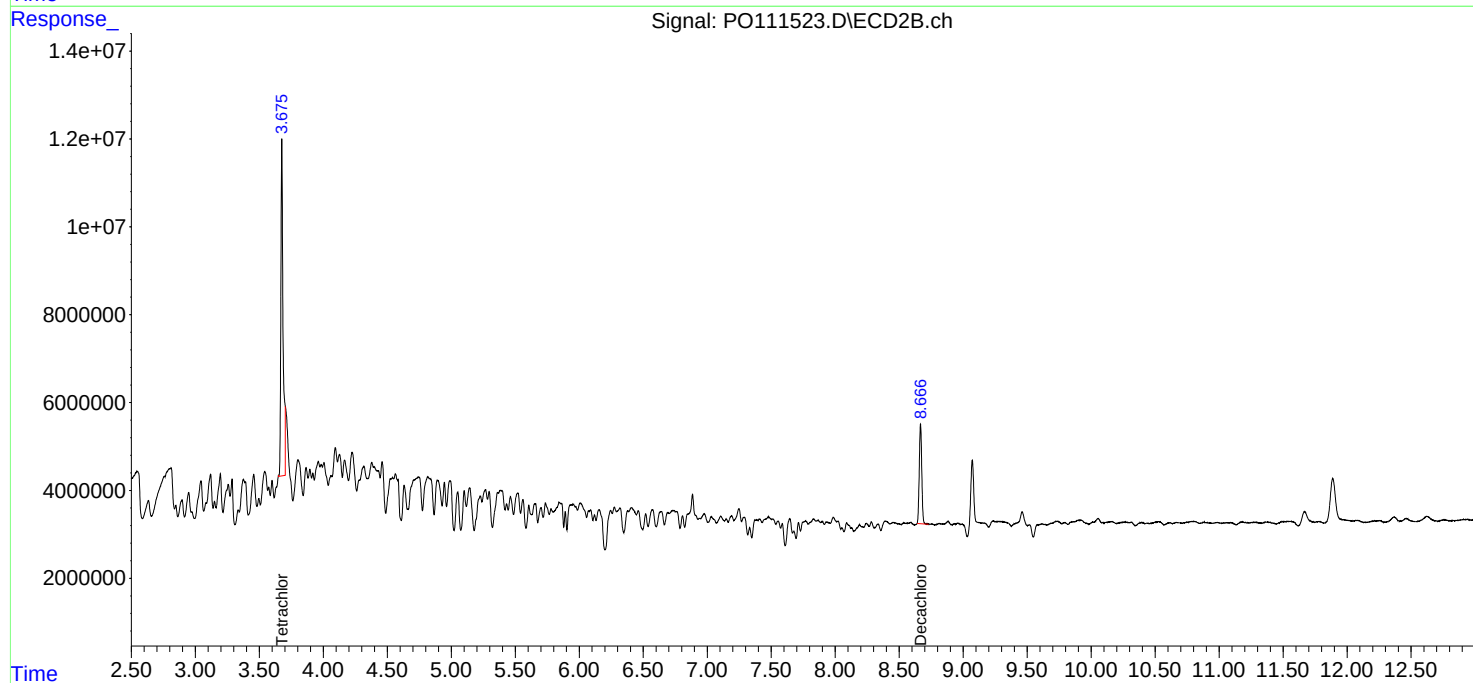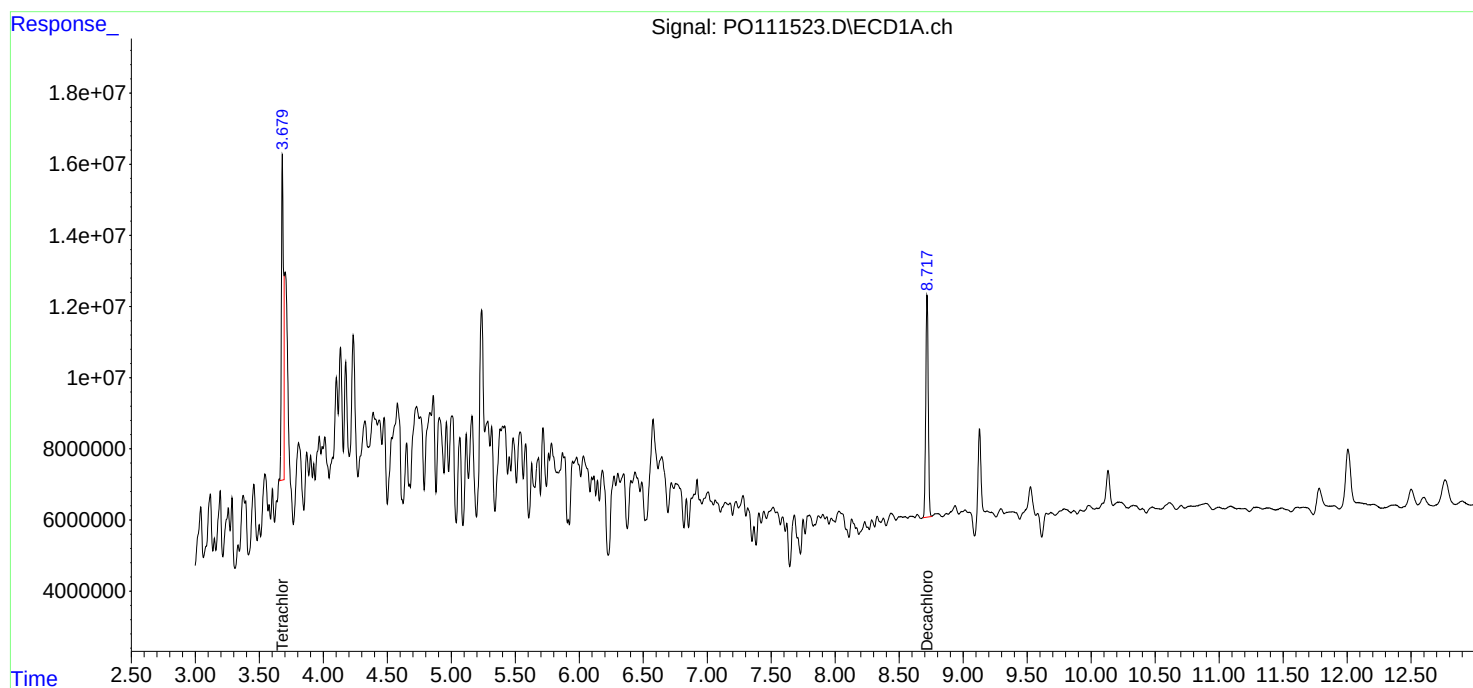

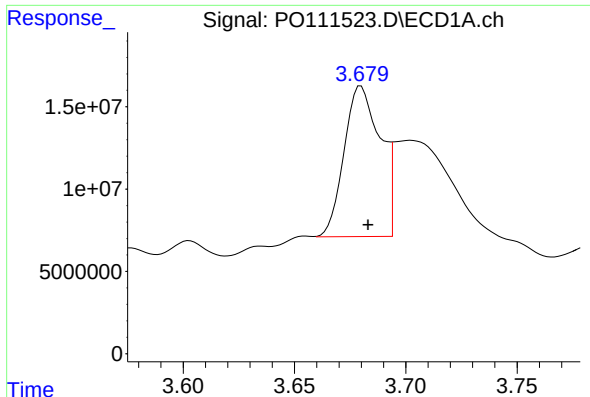


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: -0.004 min
Response: 106967205
Conc: 18.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-A2-07-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2025
Supervised By :mohammad ahmed 06/10/2025

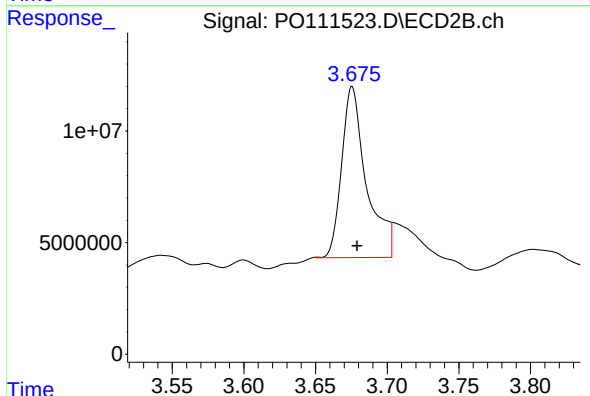


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.004 min
Response: 92899738
Conc: 17.04 ng/ml m

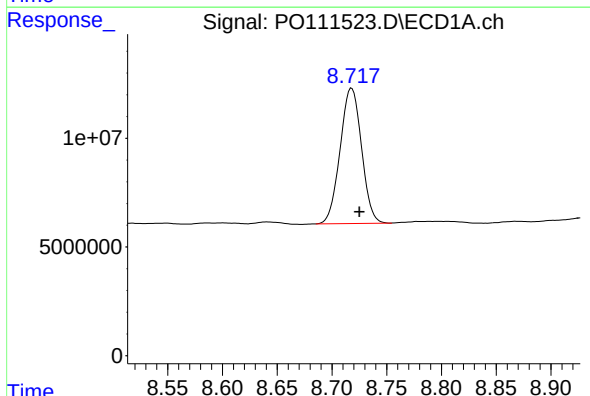

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: -0.007 min
Response: 84570658
Conc: 16.38 ng/ml

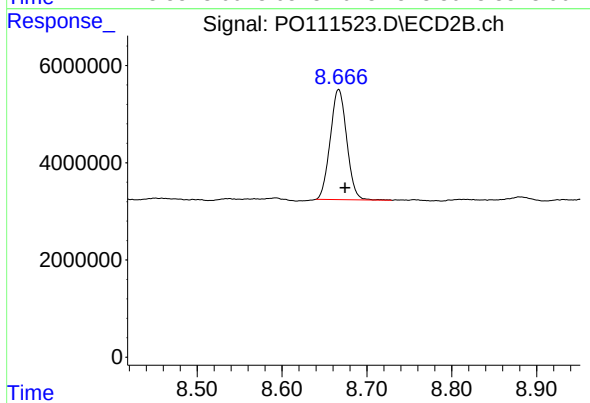

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.007 min
Response: 30579984
Conc: 16.53 ng/ml