


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050193.D
Acq On : 05 Jun 2025 08:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 05 16:20:25 2025

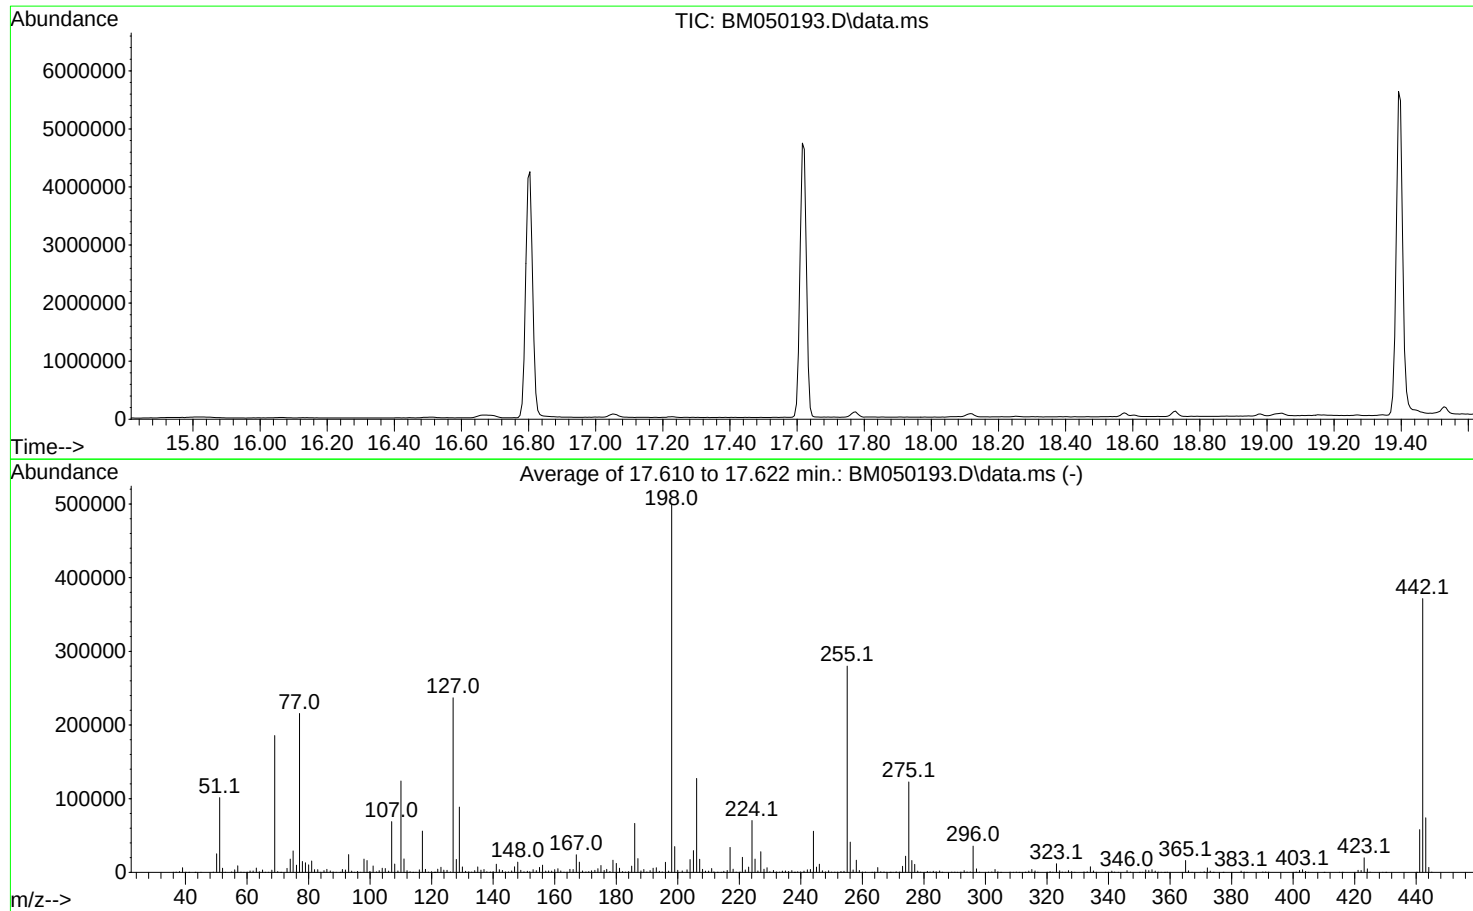




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.3	101444	PASS
68	69	0.00	2	1.6	2964	PASS
69	198	0.00	100	37.2	185664	PASS
70	69	0.00	2	0.6	1032	PASS
127	198	10	80	47.5	237035	PASS
197	198	0.00	2	0.4	1811	PASS
198	198	100	100	100.0	499264	PASS
199	198	5	9	7.0	34904	PASS
275	198	10	60	24.6	122771	PASS
365	198	1	100	3.2	16128	PASS
441	198	0.01	100	11.6	57920	PASS
442	442	50	100	100.0	371584	PASS
443	442	15	24	19.9	74069	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050193.D
Acq On : 05 Jun 2025 08:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 05 16:27:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

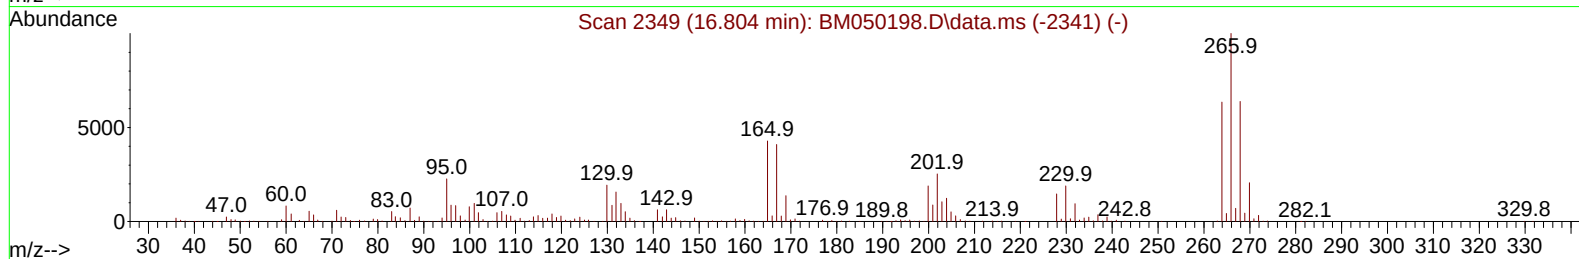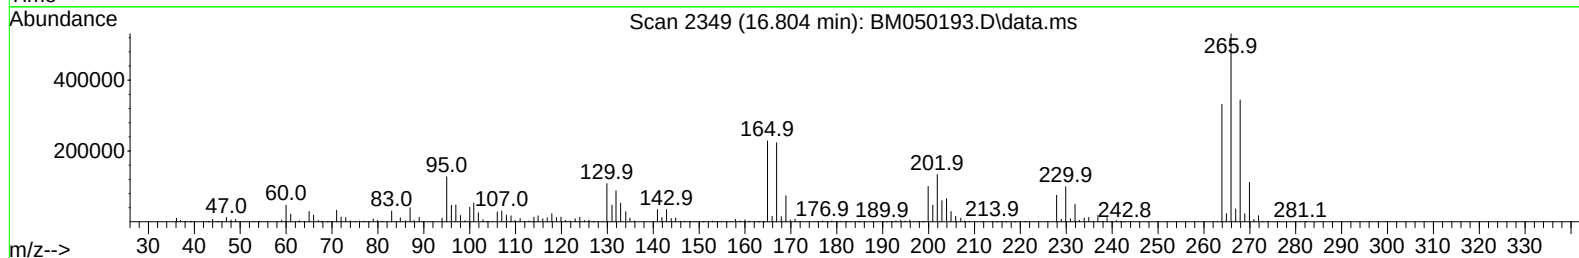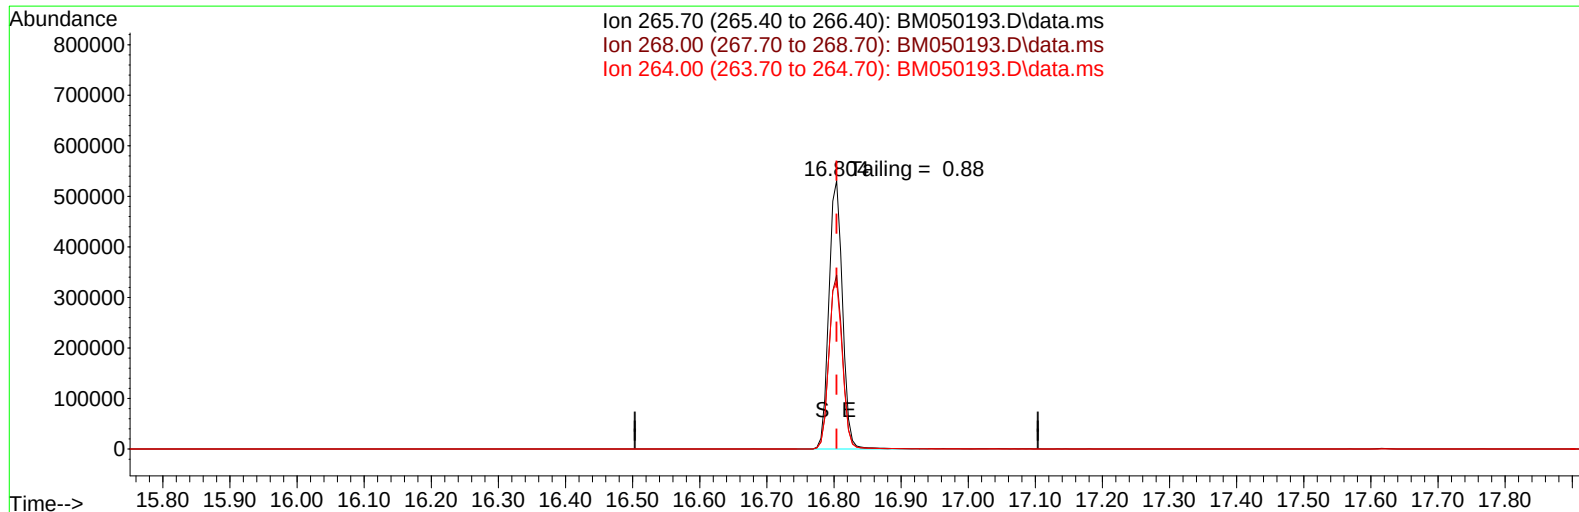

TIC: BM050193.D\data.ms

(70) Pentachlorophenol (C)

16.804min (+ 0.000) 1708888.69 ng




response 747502

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.80
264.00	63.50	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060525\
Data File : BM050193.D
Acq On : 05 Jun 2025 08:40
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 05 16:27:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 05 16:20:25 2025
Response via : Initial Calibration

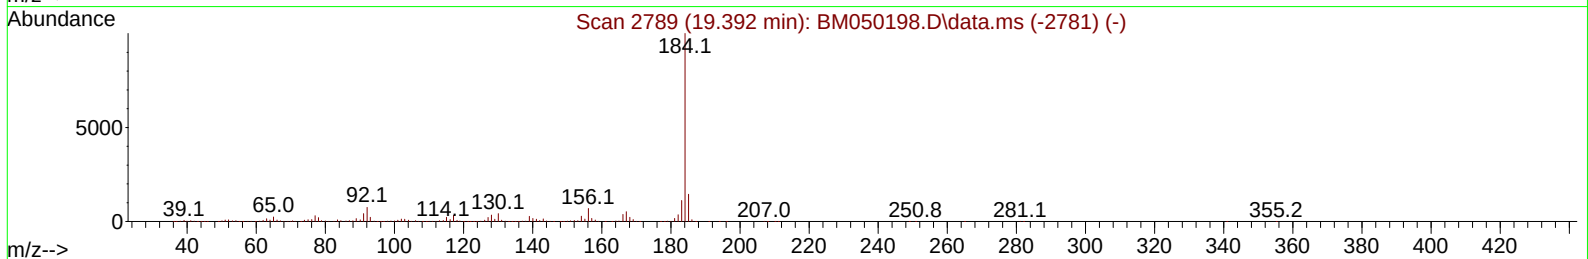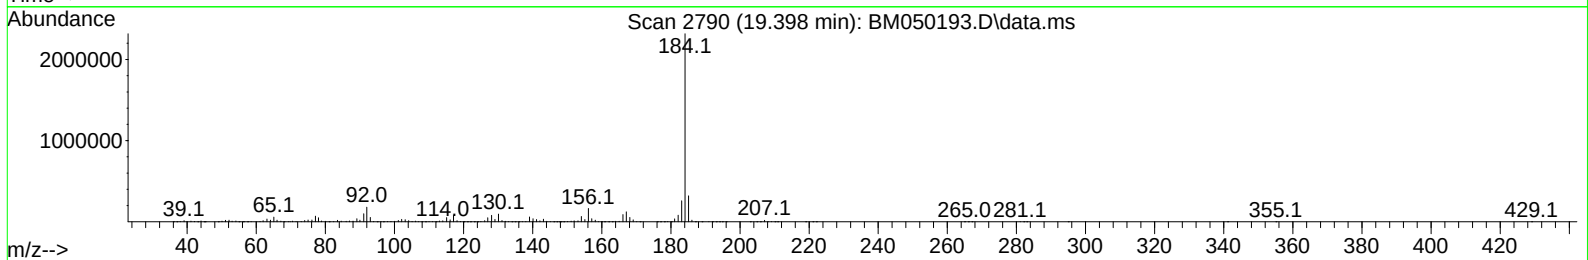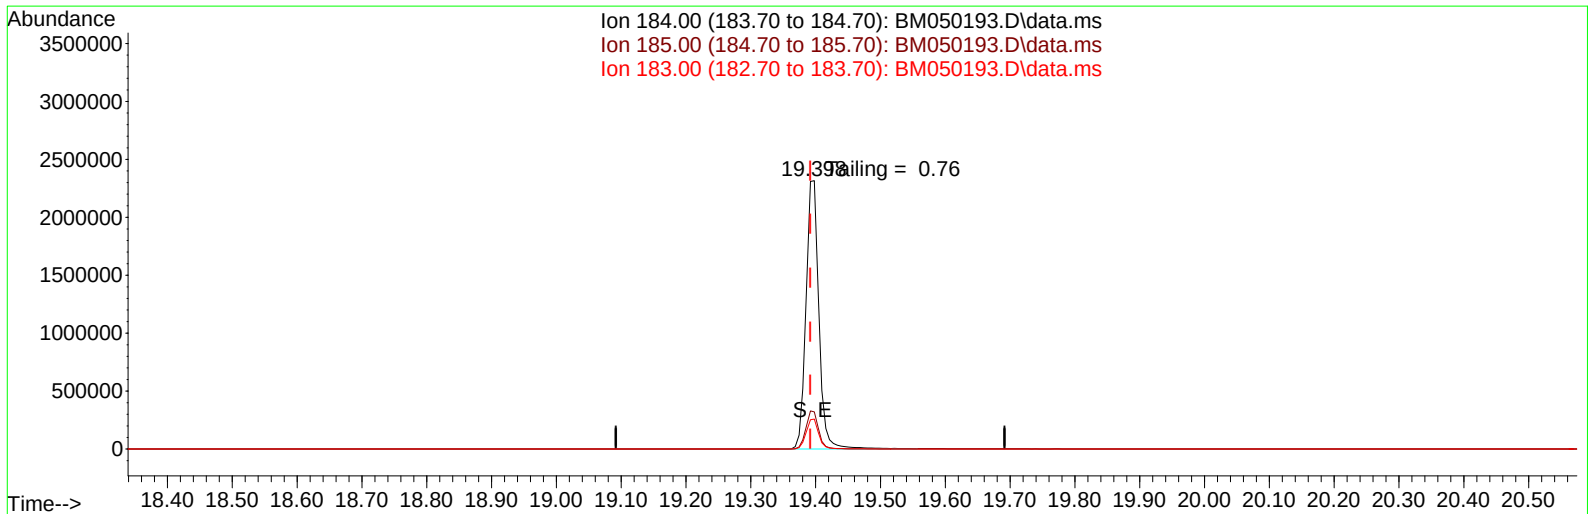

TIC: BM050193.D\data.ms

(77) Benzidine

19.398min (+ 0.006) 33233.28 ng

response 3215775

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.84
183.00	11.20	11.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/5/2025	BNA_M	<u>BM050193.D</u>
Compound Name	Response	Retention Time
DDT	1539212	20.645
DDD	20154	20.257
DDE	1832	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21986	1561198	1.41

Instrument :
BNA_M
ClientSampleId :
DFTPP