


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050244.D
Acq On : 09 Jun 2025 16:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 11:54:38 2025

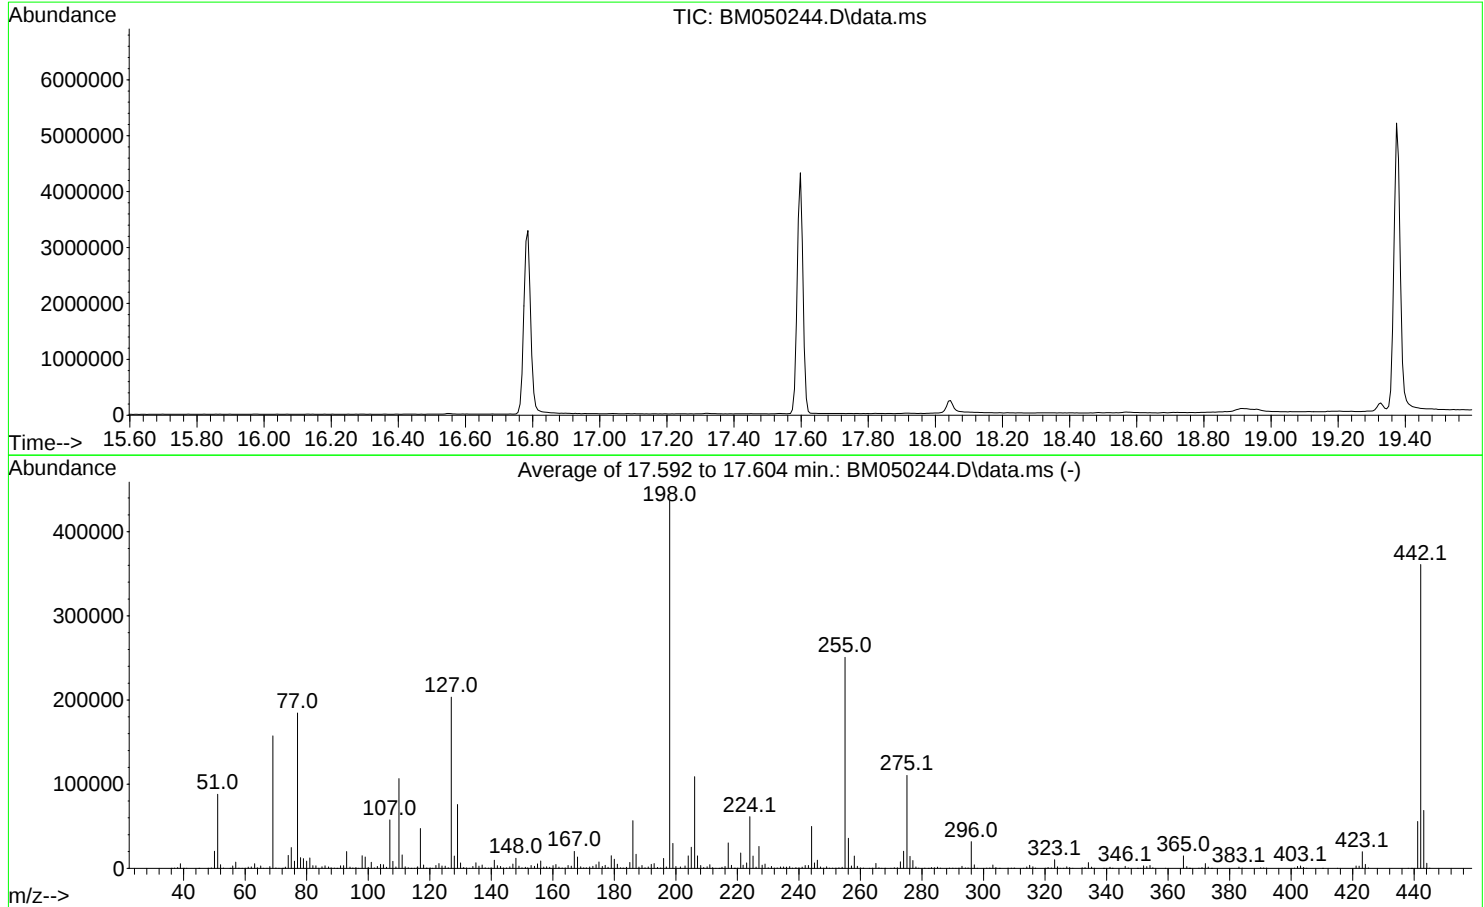




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.2	88096	PASS
68	69	0.00	2	1.4	2134	PASS
69	198	0.00	100	36.0	157327	PASS
70	69	0.00	2	0.3	522	PASS
127	198	10	80	46.5	203328	PASS
197	198	0.00	2	0.4	1683	PASS
198	198	100	100	100.0	437035	PASS
199	198	5	9	6.8	29595	PASS
275	198	10	60	25.3	110448	PASS
365	198	1	100	3.4	14806	PASS
441	198	0.01	100	12.7	55720	PASS
442	442	50	100	100.0	360981	PASS
443	442	15	24	19.1	68901	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050244.D
Acq On : 09 Jun 2025 16:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 09 17:38:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

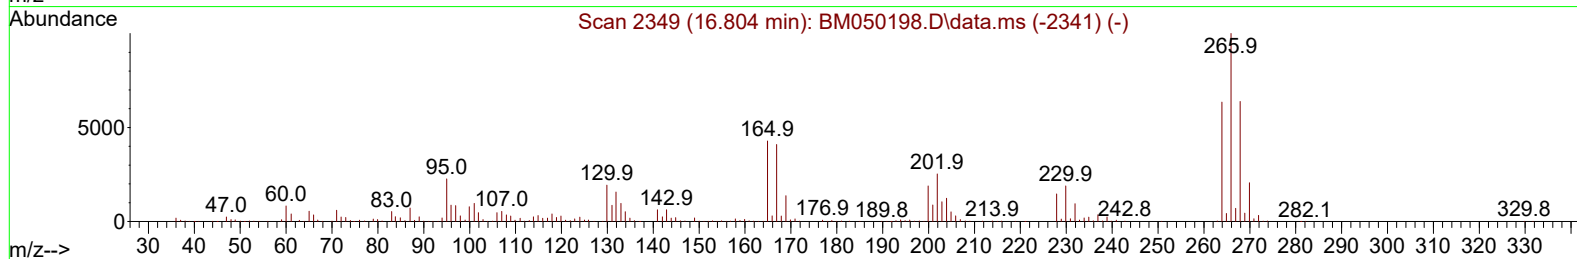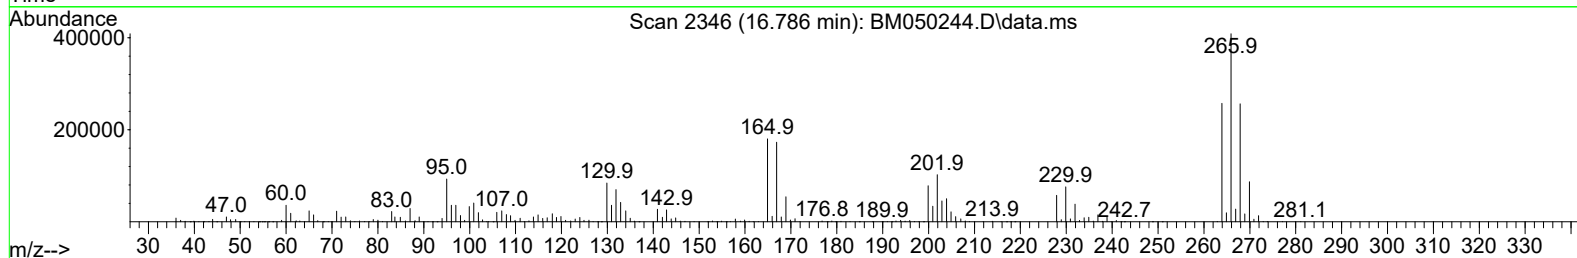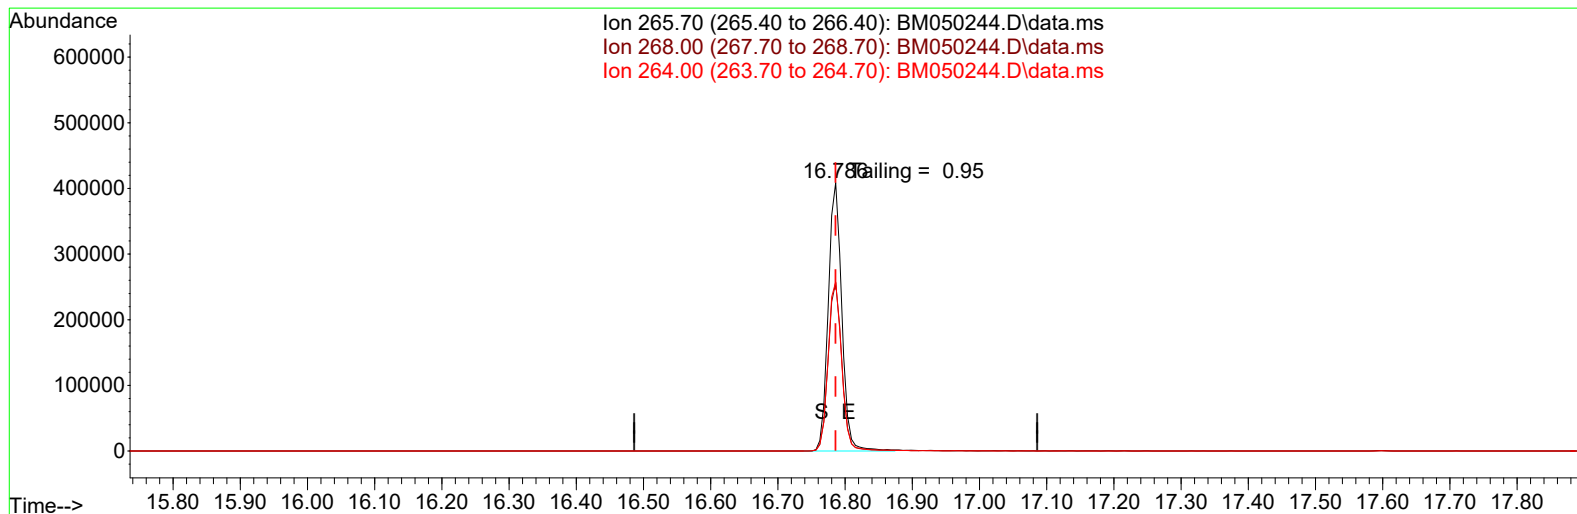

TIC: BM050244.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.000) 282541.19 ng




response 572172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.74
264.00	63.50	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050244.D
Acq On : 09 Jun 2025 16:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 09 17:38:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

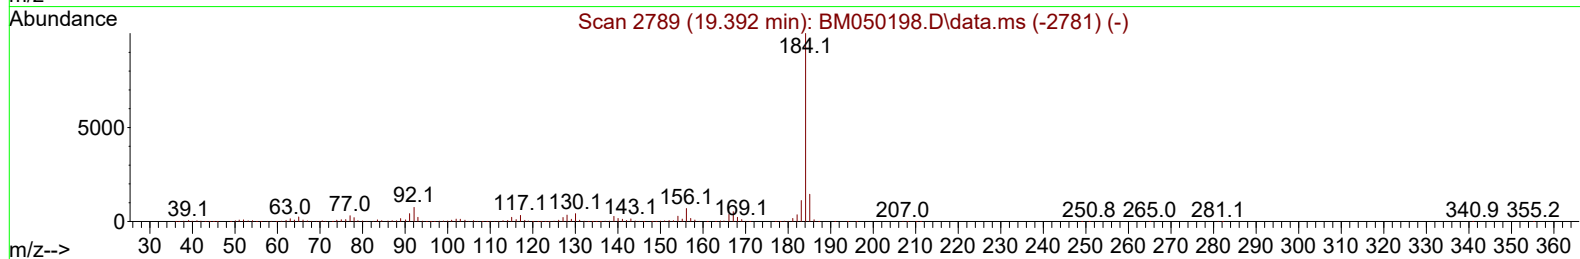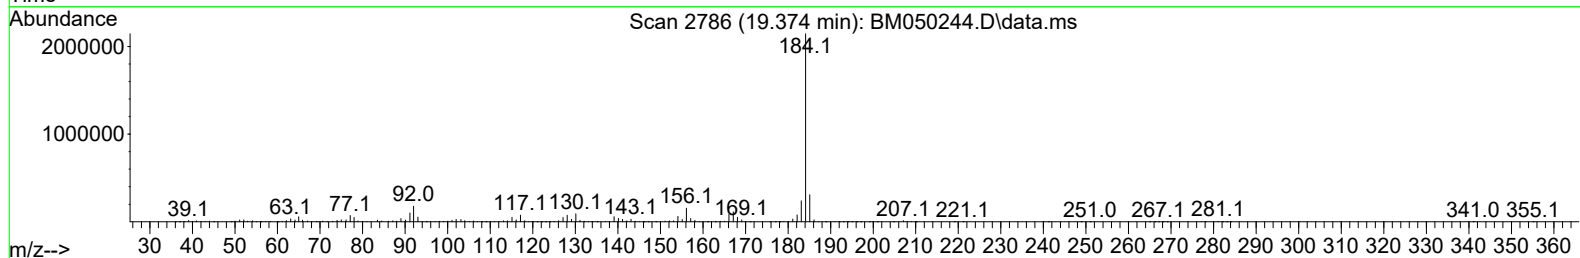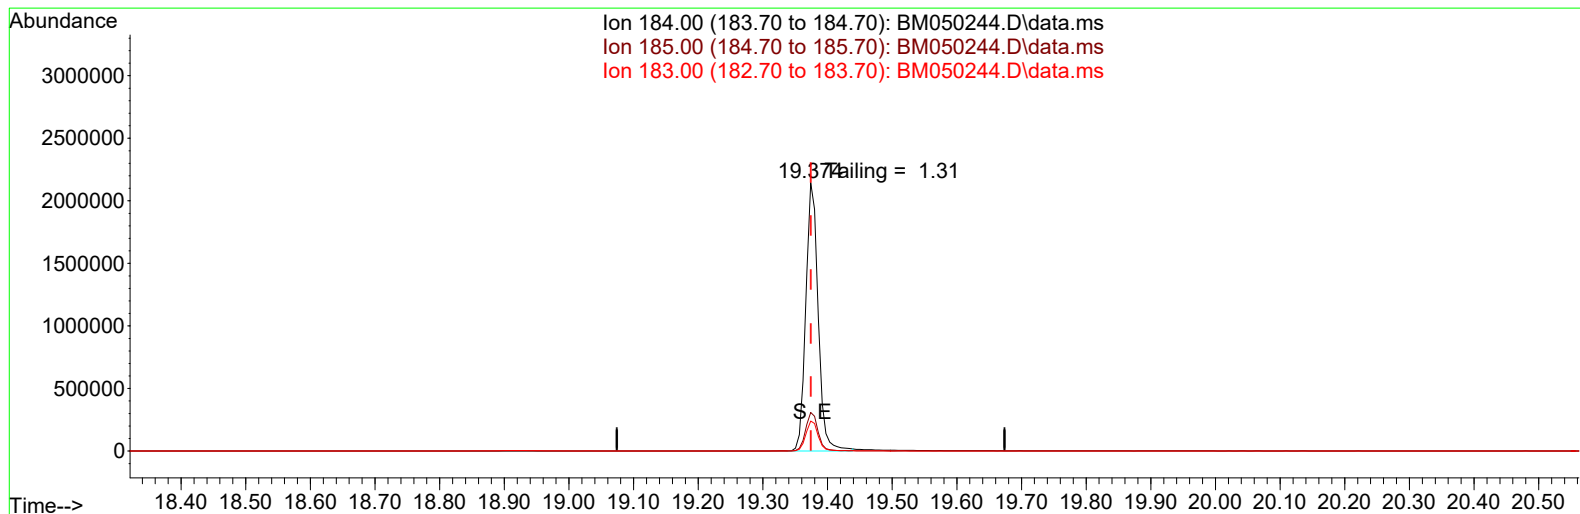

TIC: BM050244.D\data.ms

(77) Benzidine

19.374min (-0.000) 185831.97 ng

response 2889837

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.40
183.00	11.20	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2025	BNA_M	<u>BM050244.D</u>
Compound Name	Response	Retention Time
DDT	1441801	20.621
DDD	16704	20.233
DDE	1198	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17902	1459703	1.23

Instrument :
BNA_M
ClientSampleId :
DFTPP