


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050261.D
Acq On : 10 Jun 2025 04:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 11:54:38 2025

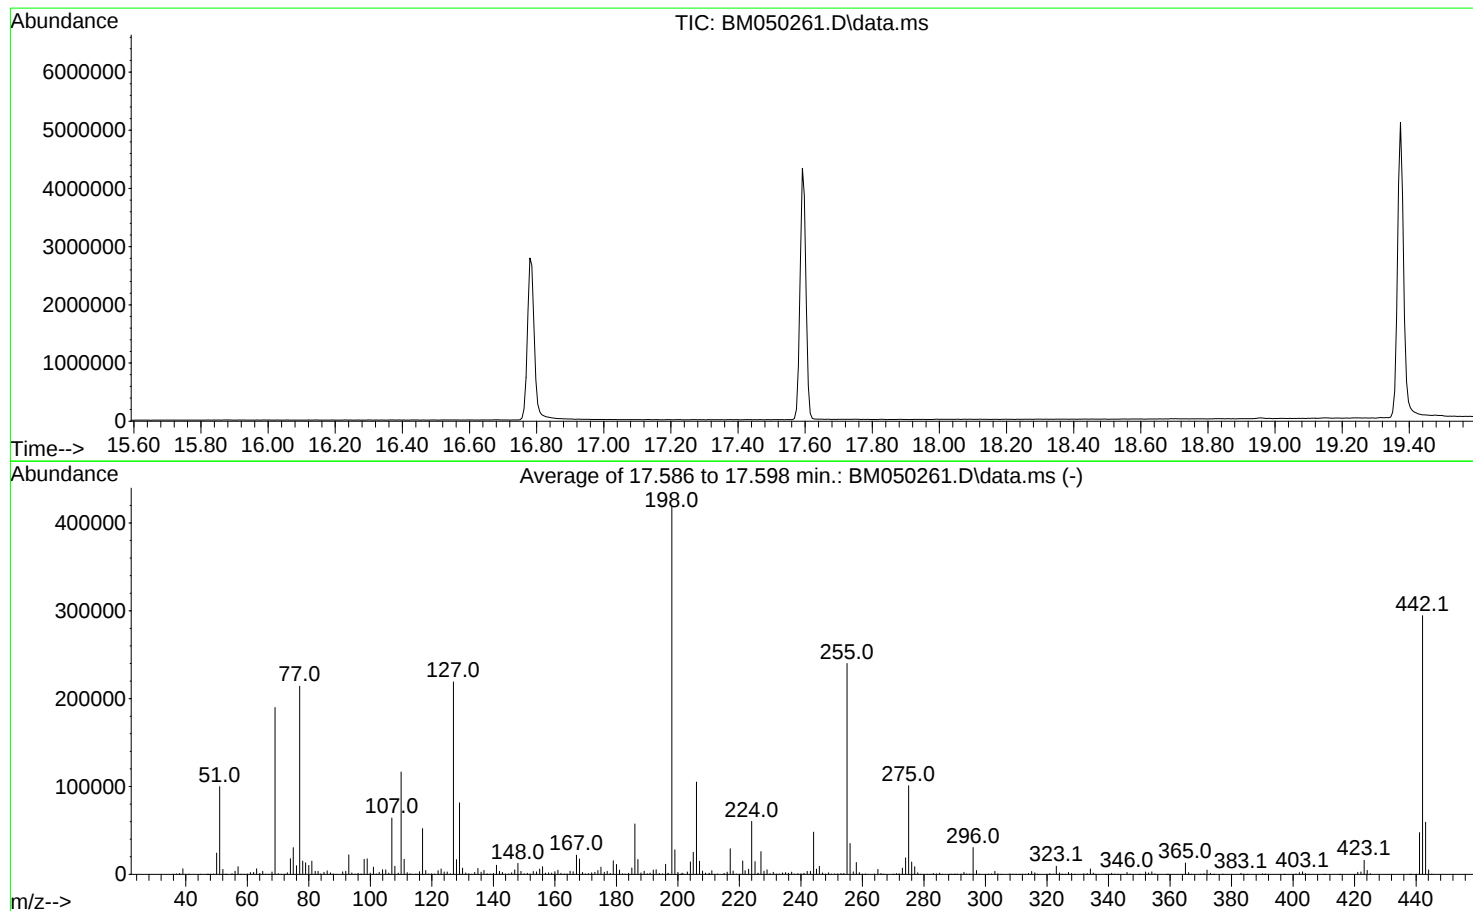




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	99808	PASS
68	69	0.00	2	1.5	2792	PASS
69	198	0.00	100	45.4	189995	PASS
70	69	0.00	2	0.5	984	PASS
127	198	10	80	52.3	219093	PASS
197	198	0.00	2	0.3	1212	PASS
198	198	100	100	100.0	418709	PASS
199	198	5	9	6.6	27819	PASS
275	198	10	60	24.1	100909	PASS
365	198	1	100	3.1	12955	PASS
441	198	0.01	100	11.3	47504	PASS
442	442	50	100	100.0	294400	PASS
443	442	15	24	20.2	59373	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050261.D
Acq On : 10 Jun 2025 04:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 10 05:34:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

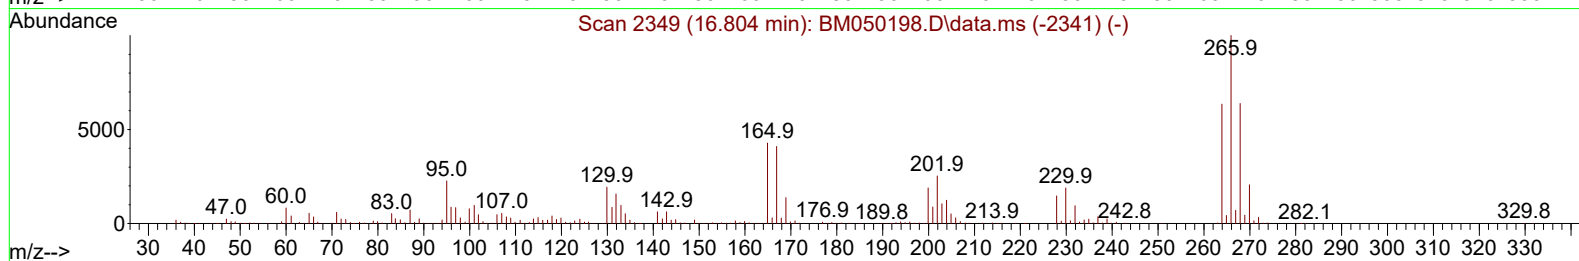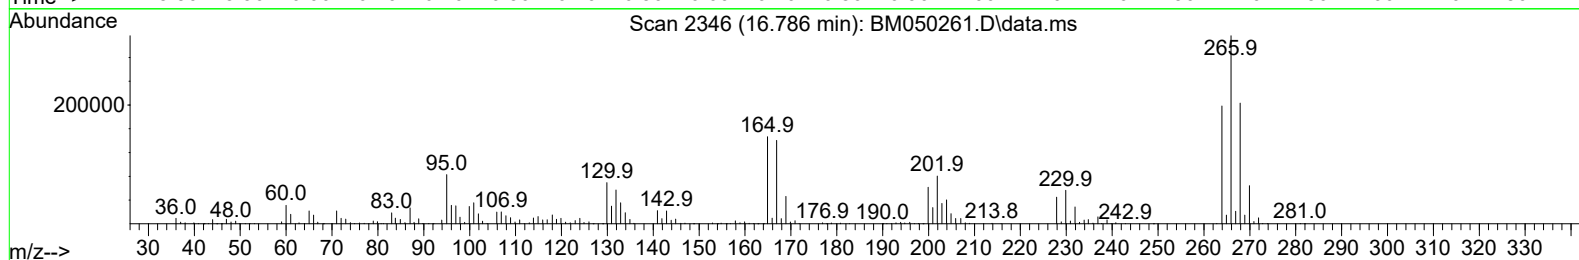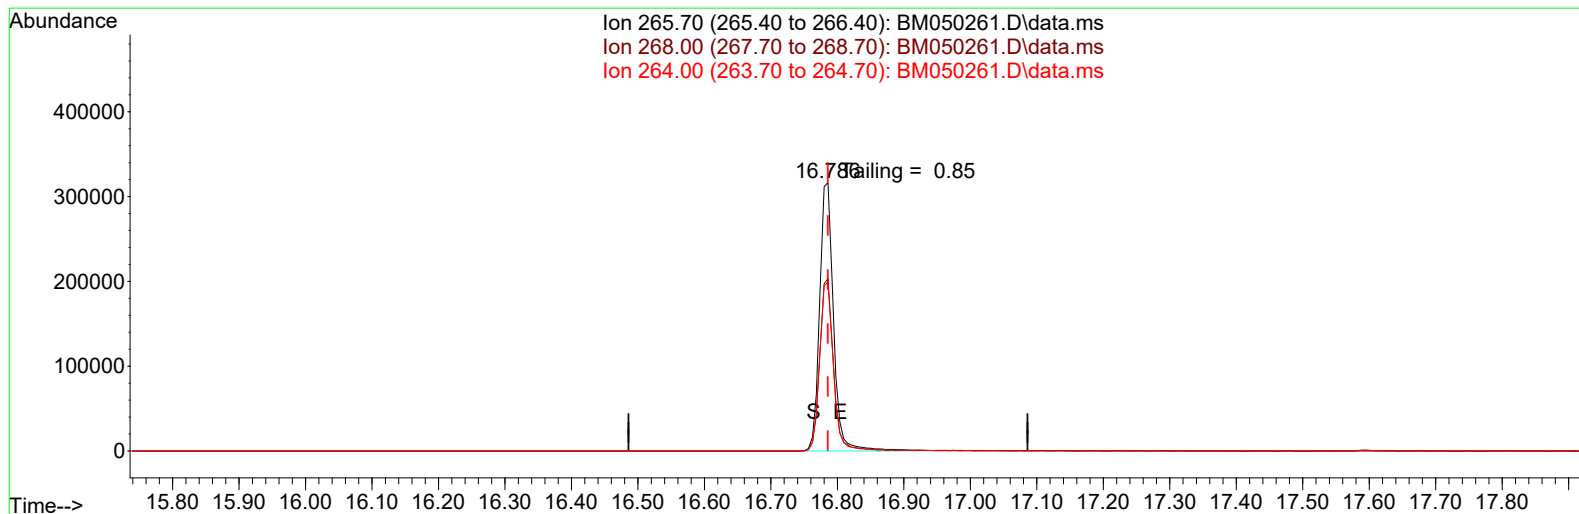

TIC: BM050261.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.000) 158695.78 ng




response 460207

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.15
264.00	63.50	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060925\
Data File : BM050261.D
Acq On : 10 Jun 2025 04:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 10 05:34:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

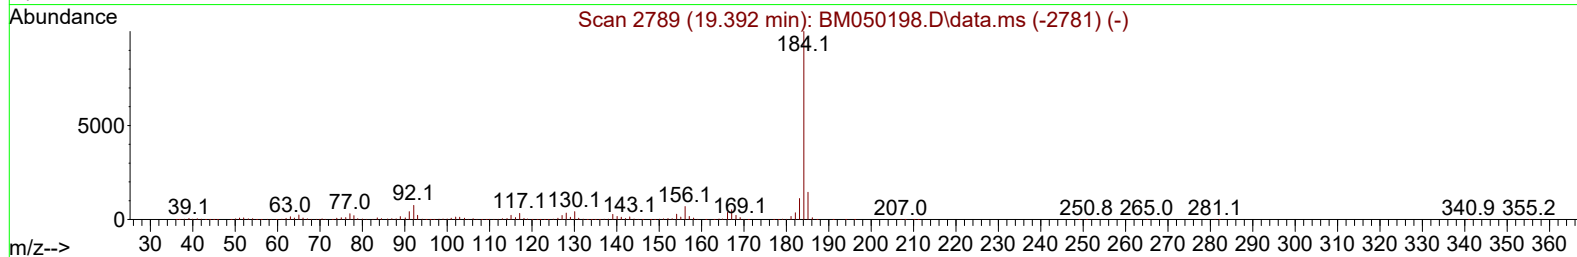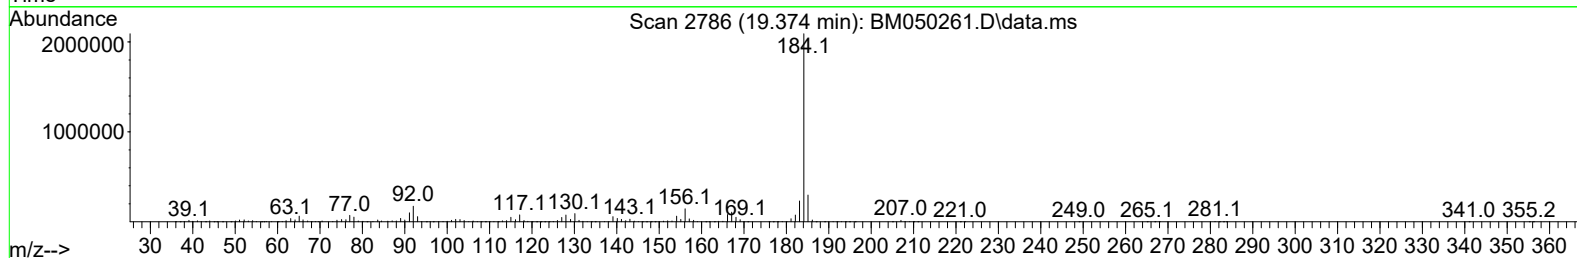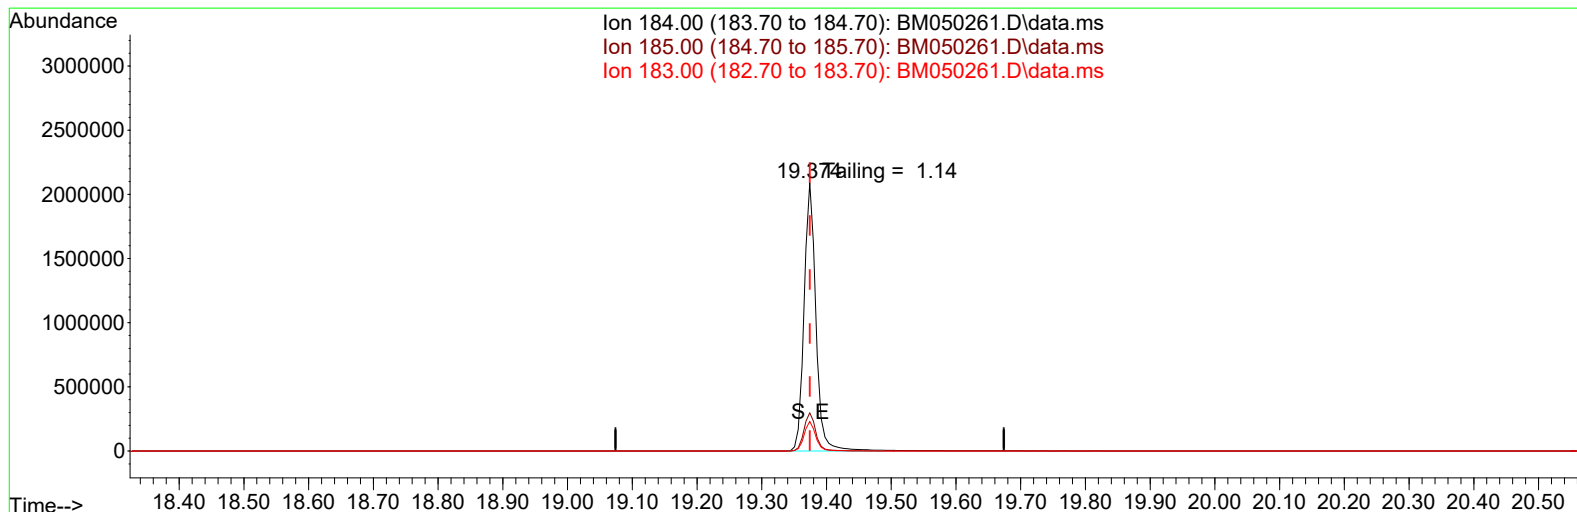

TIC: BM050261.D\data.ms

(77) Benzidine

19.374min (-0.000) 99825.69 ng

response 2680856

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.26
183.00	11.20	11.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2025	BNA_M	<u>BM050261.D</u>
Compound Name	Response	Retention Time
DDT	1335236	20.615
DDD	14959	20.233
DDE	1895	19.668
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16854	1352090	1.25

Instrument :
BNA_M
ClientSampleId :
DFTPP