

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060625\
 Data File : PP072722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2025 00:41
 Operator : YP\AJ
 Sample : Q2237-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TW-WTS-10

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/09/2025
 Supervised By :mohammad ahmed 06/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 03:16:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.498	3.796	38710653	36866489	19.251m	23.065
2) SA Decachlor...	10.199	8.809	11883647	9889096	7.294	9.342 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060625\
Data File : PP072722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2025 00:41
Operator : YP\AJ
Sample : Q2237-02
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
TW-WTS-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2025
Supervised By :mohammad ahmed 06/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 03:16:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

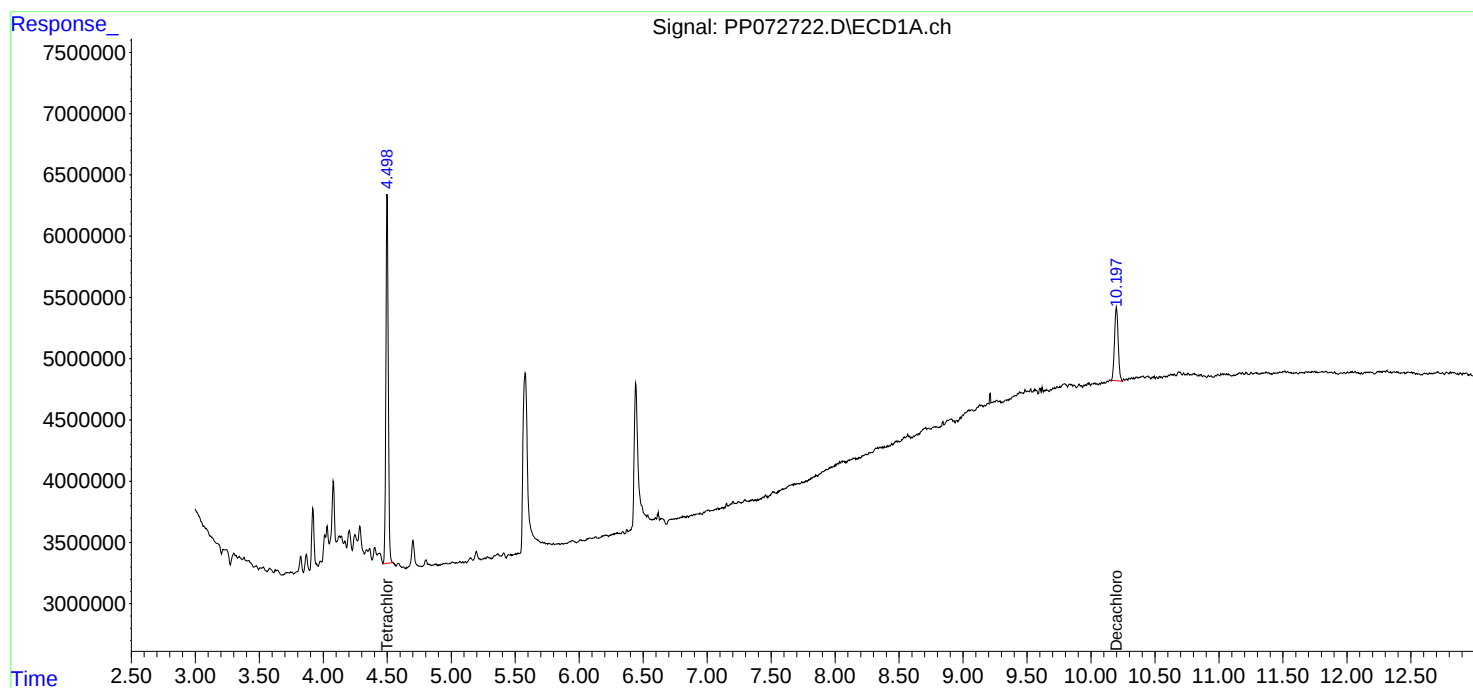

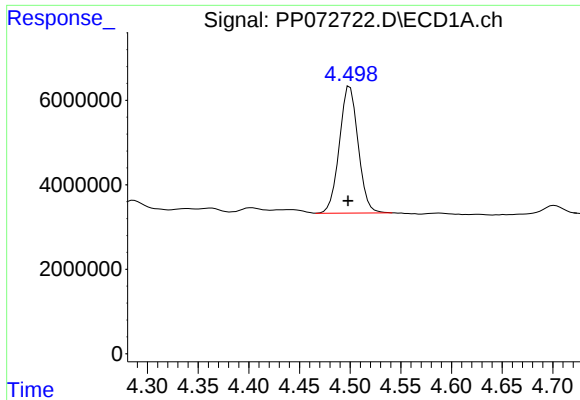


#1 Tetrachloro-m-xylene

R.T.: 4.498 min
Delta R.T.: 0.000 min
Response: 38710653
Conc: 19.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
TW-WTS-10


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/09/2025
Supervised By :mohammad ahmed 06/10/2025

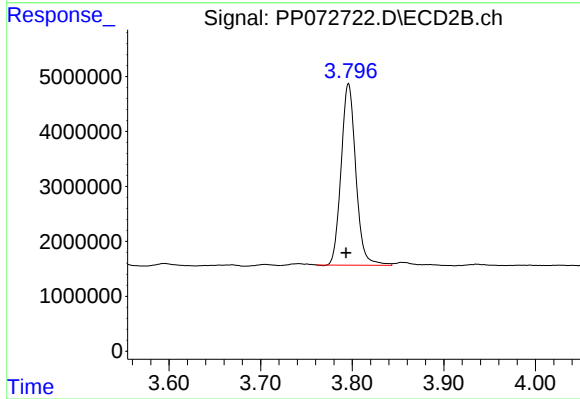


#1 Tetrachloro-m-xylene

R.T.: 3.796 min
Delta R.T.: 0.003 min
Response: 36866489
Conc: 23.07 ng/ml

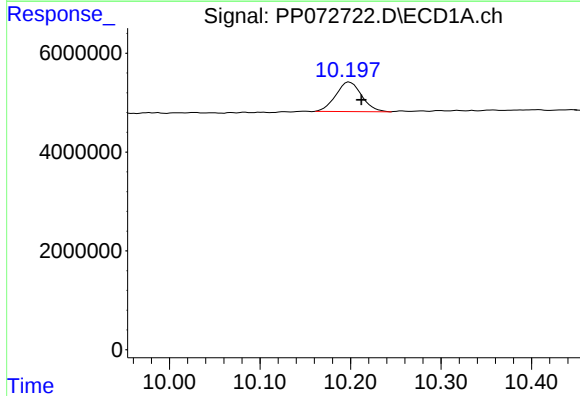

#2 Decachlorobiphenyl

R.T.: 10.199 min
Delta R.T.: -0.013 min
Response: 11883647
Conc: 7.29 ng/ml

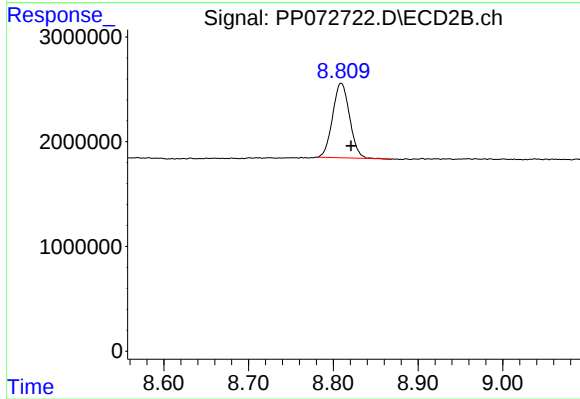

#2 Decachlorobiphenyl

R.T.: 8.809 min
Delta R.T.: -0.012 min
Response: 9889096
Conc: 9.34 ng/ml