

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060925\
 Data File : PP072755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jun 2025 17:12
 Operator : YP\AJ
 Sample : Q2259-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OU4-PCS-TC-36-060525

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/10/2025
 Supervised By :mohammad ahmed 06/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 02:31:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 24 03:32:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.499	3.793	44370194	39462397	22.066	24.689
2) SA Decachlor...	10.196	8.807	35676885	26025711	21.899m	24.585m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP060925\
Data File : PP072755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jun 2025 17:12
Operator : YP\AJ
Sample : Q2259-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OU4-PCS-TC-36-060525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2025
Supervised By :mohammad ahmed 06/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 02:31:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 24 03:32:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

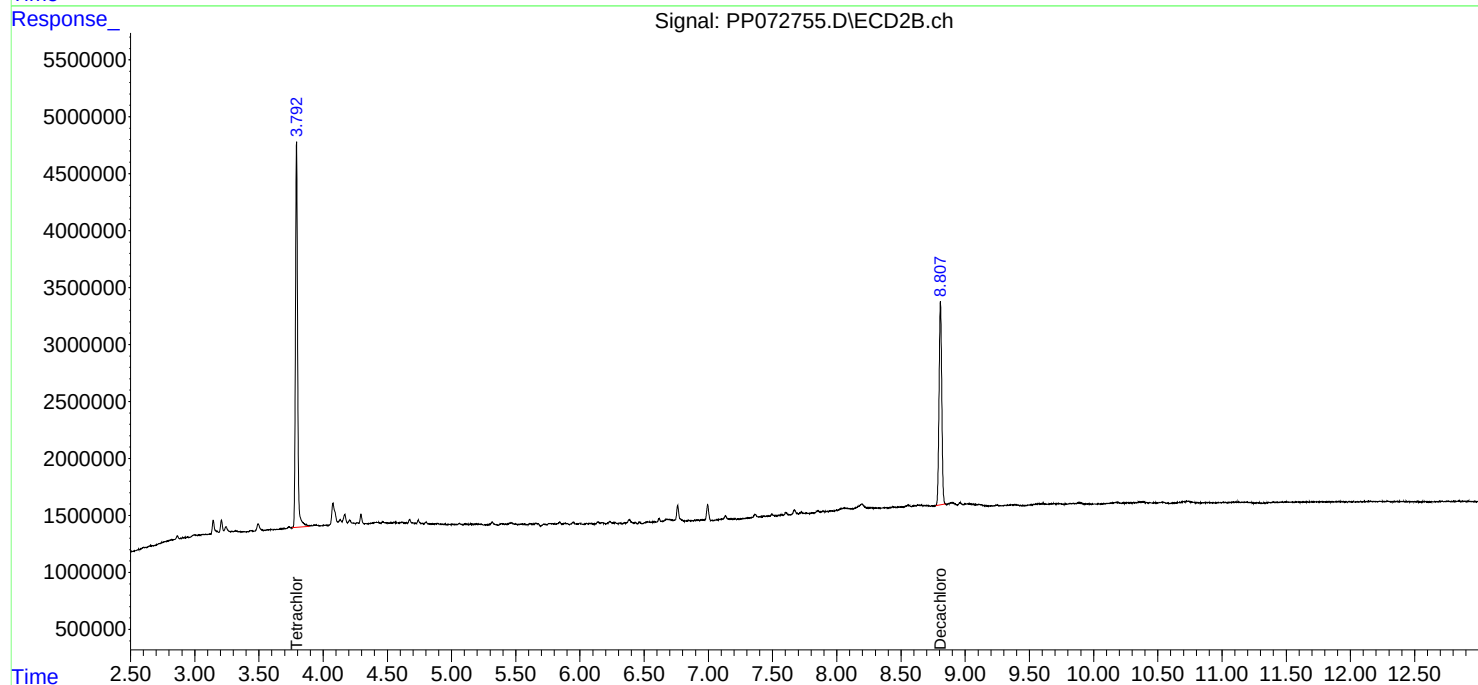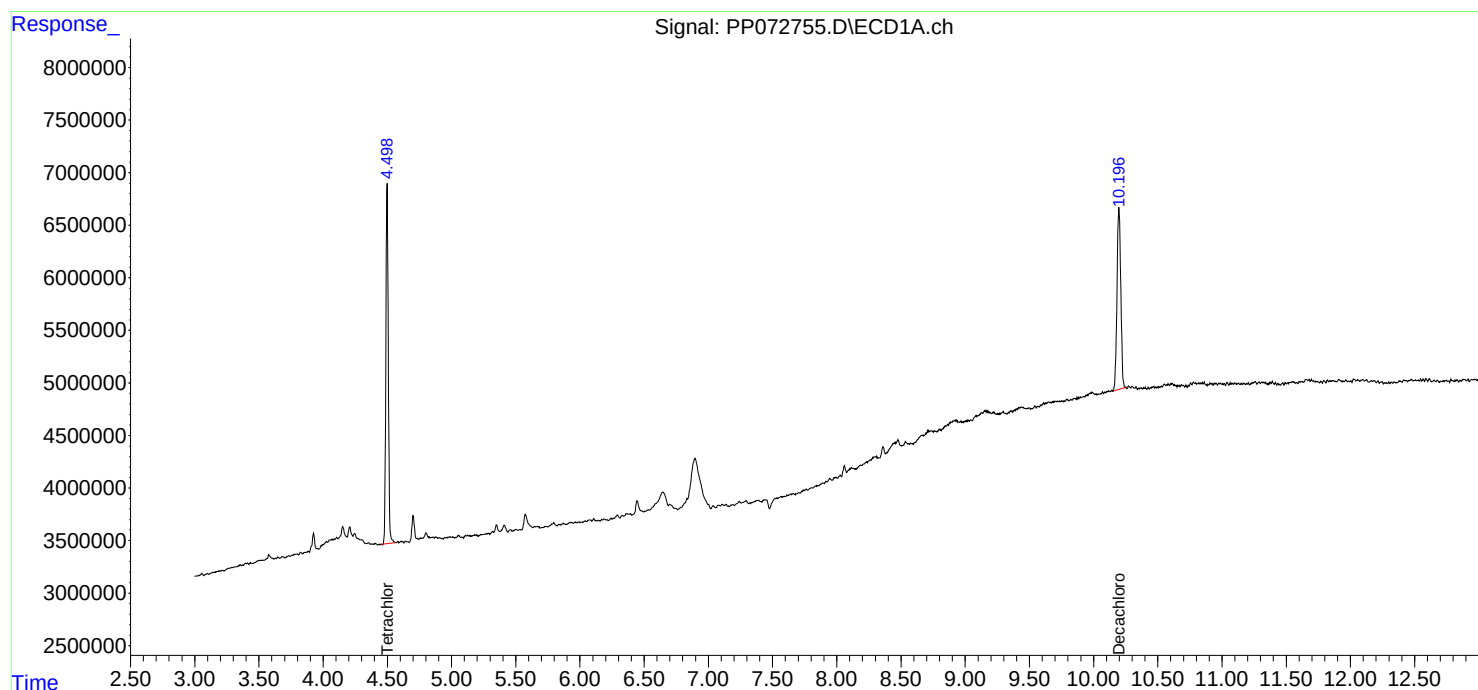

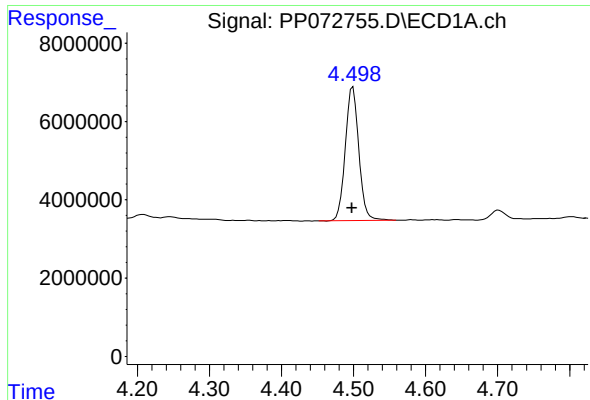


#1 Tetrachloro-m-xylene

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 44370194
Conc: 22.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
OU4-PCS-TC-36-060525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2025
Supervised By :mohammad ahmed 06/11/2025

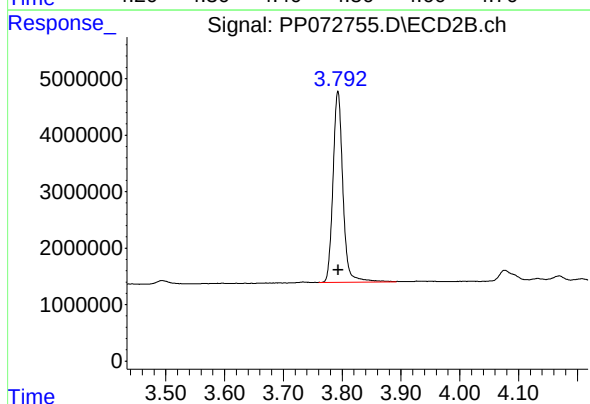


#1 Tetrachloro-m-xylene

R.T.: 3.793 min
Delta R.T.: 0.000 min
Response: 39462397
Conc: 24.69 ng/ml

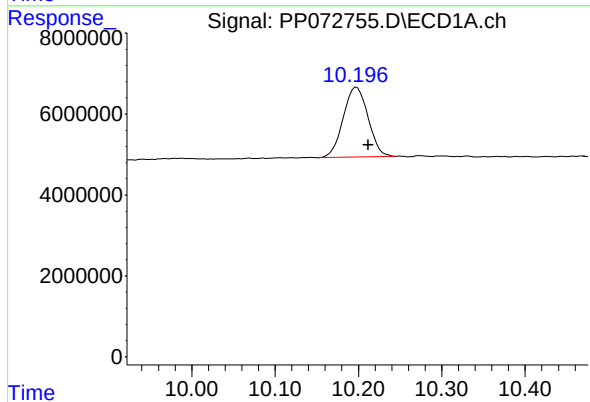

#2 Decachlorobiphenyl

R.T.: 10.196 min
Delta R.T.: -0.016 min
Response: 35676885
Conc: 21.90 ng/ml m

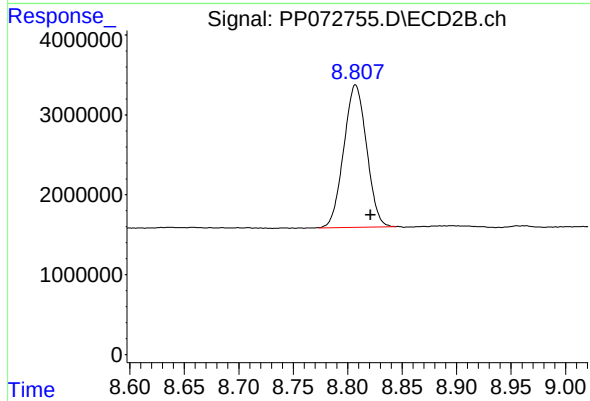

#2 Decachlorobiphenyl

R.T.: 8.807 min
Delta R.T.: -0.014 min
Response: 26025711
Conc: 24.58 ng/ml m