
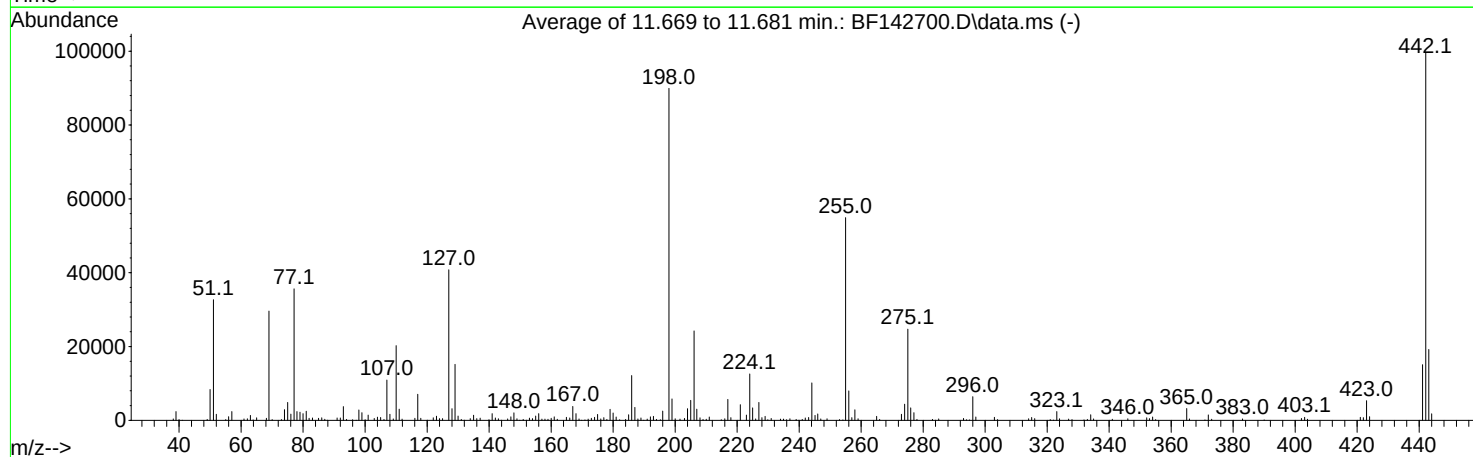


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142700.D
Acq On : 10 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 18:21:22 2025

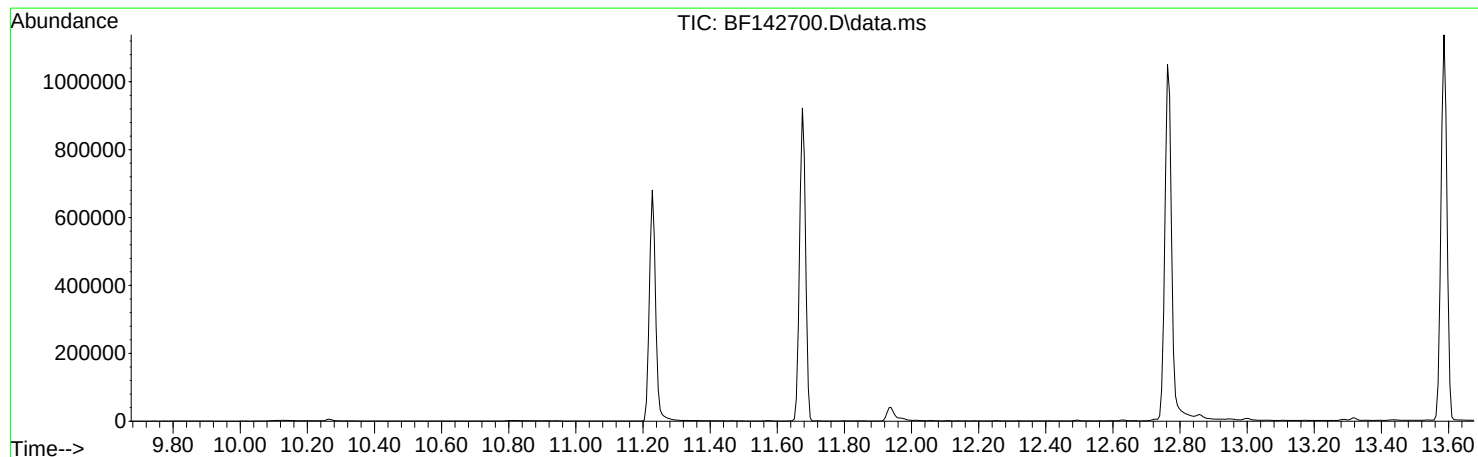

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	32669	PASS
68	69	0.00	2	1.9	566	PASS
69	198	0.00	100	32.9	29592	PASS
70	69	0.00	2	0.7	209	PASS
127	198	10	80	45.4	40784	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89928	PASS
199	198	5	9	6.5	5809	PASS
275	198	10	60	27.5	24696	PASS
365	198	1	100	3.6	3225	PASS
441	198	0.01	100	16.8	15085	PASS
442	442	50	100	100.0	99645	PASS
443	442	15	24	19.3	19186	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/10/2025	BNA_F	<u>BF142700.D</u>
Compound Name	Response	Retention Time
DDT	292880	13.586
DDD	4351	13.316
DDE	963	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5314	298194	1.78

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142700.D
Acq On : 10 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:16:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 18:21:22 2025
Response via : Initial Calibration

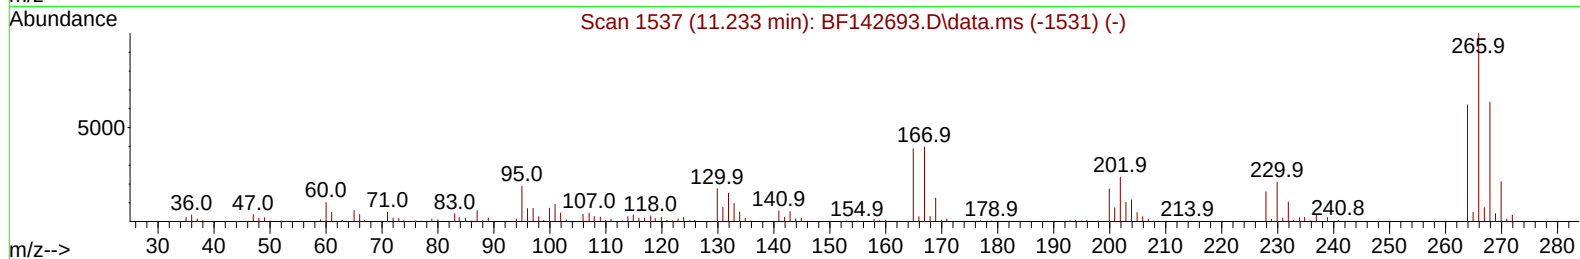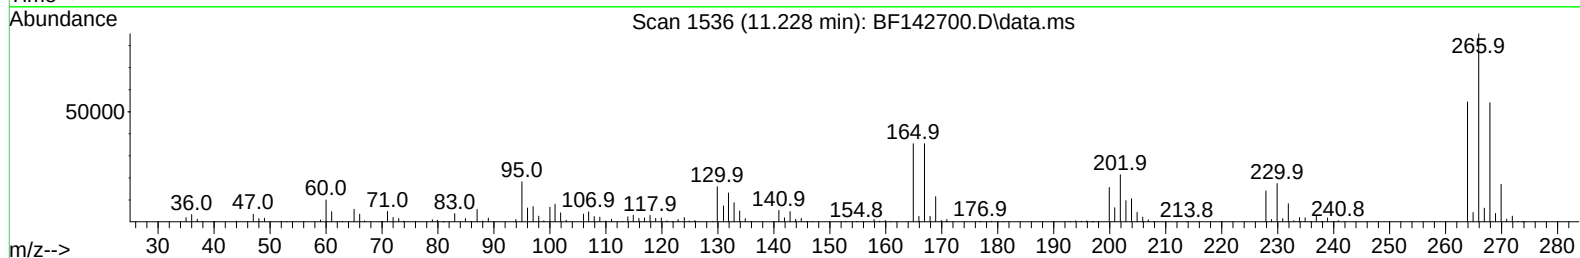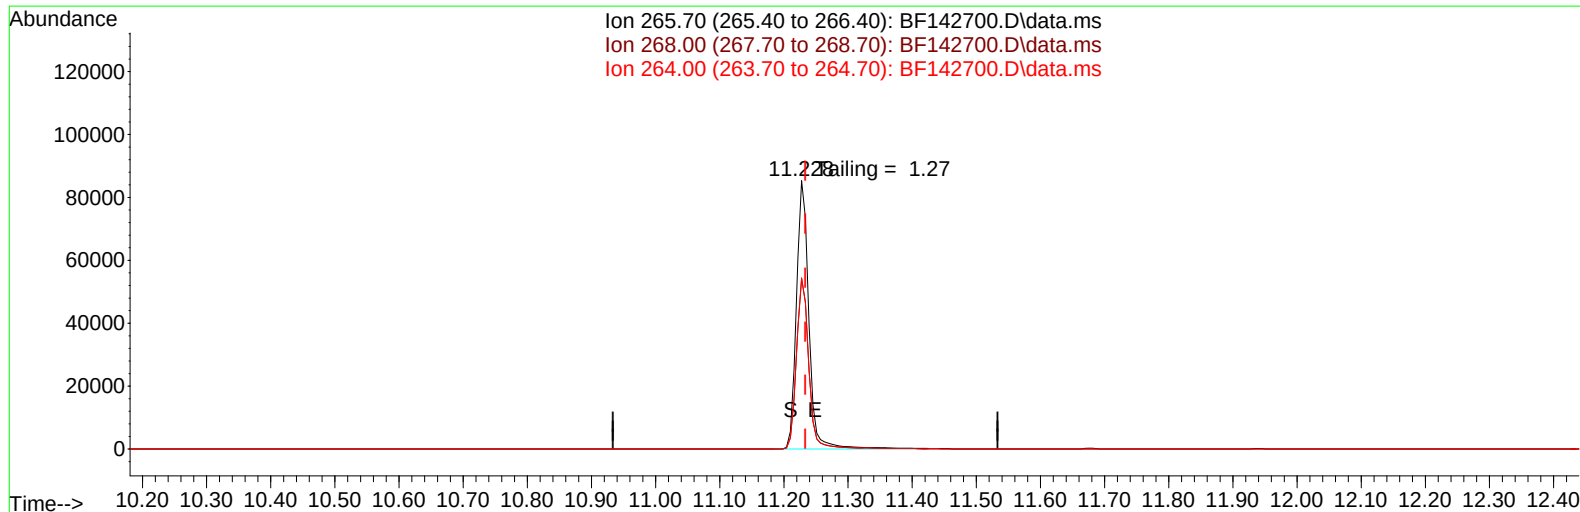

TIC: BF142700.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.006) 58811.37 ng




response 116657

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.43
264.00	62.10	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061025\
Data File : BF142700.D
Acq On : 10 Jun 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 10 11:16:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 18:21:22 2025
Response via : Initial Calibration

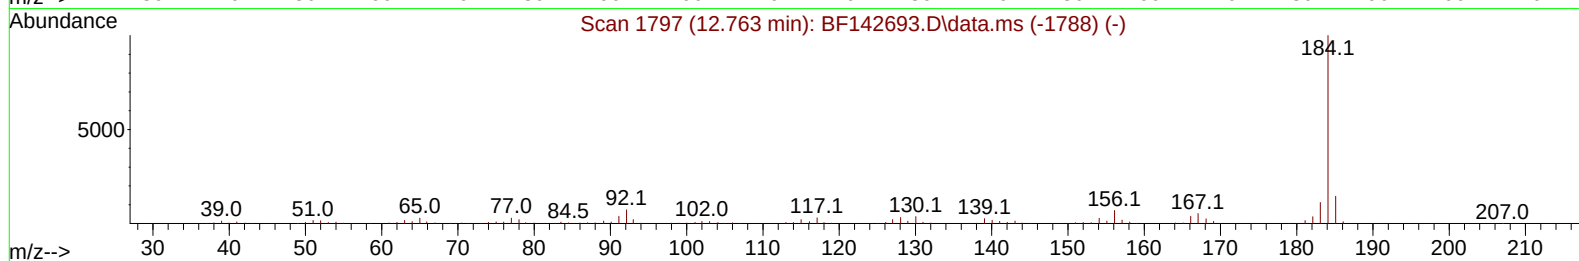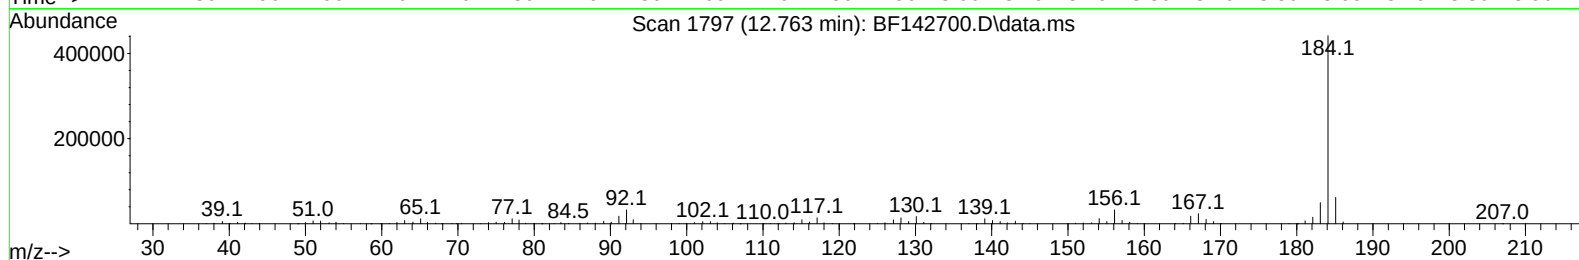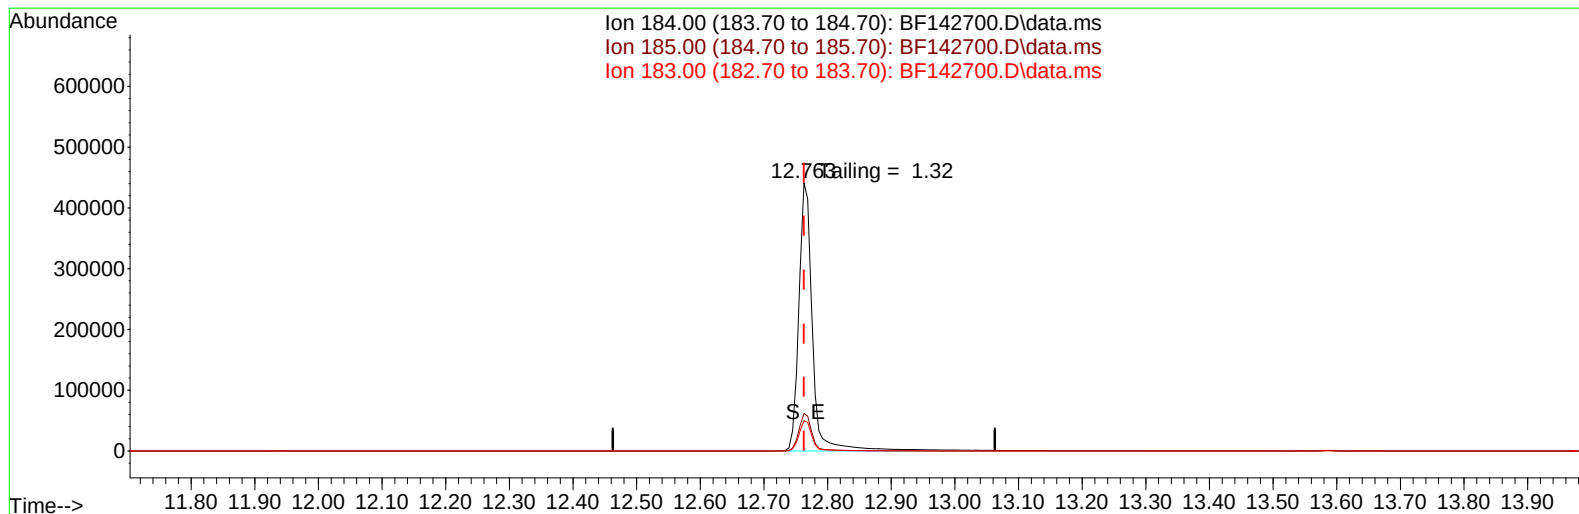

TIC: BF142700.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 44952.78 ng

response 659366

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.00
183.00	11.10	11.27
0.00	0.00	0.00