


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037223.D
Acq On : 13 Jun 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 13 18:43:34 2025

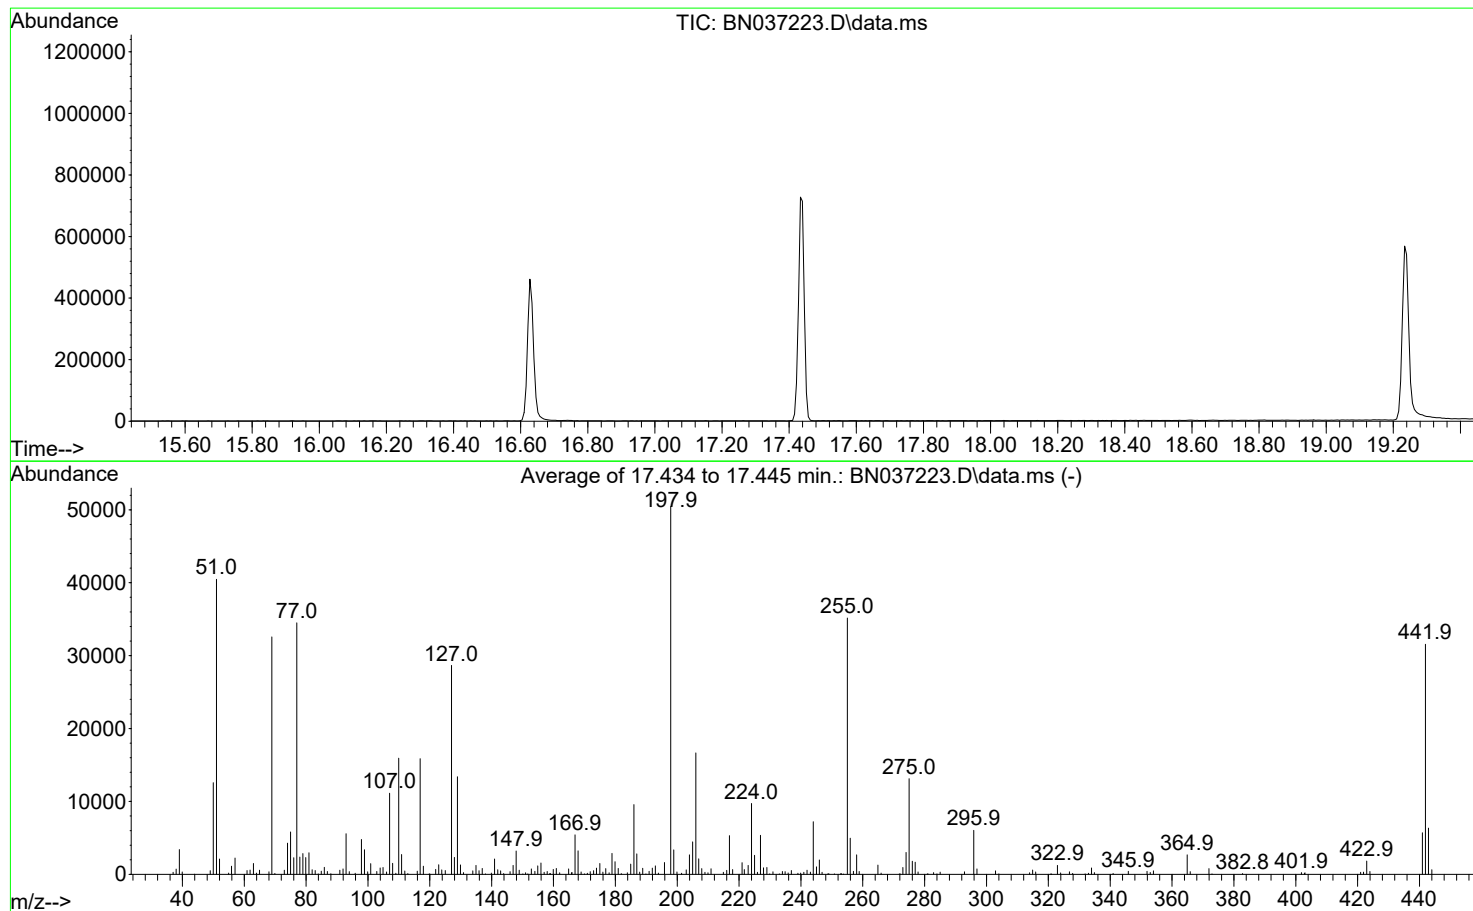




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	80.2	40477	FAIL*
68	69	0.00	2	1.1	362	PASS
69	198	0.00	100	64.6	32573	PASS
70	69	0.00	2	0.4	132	PASS
127	198	10	80	56.8	28661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50453	PASS
199	198	5	9	6.7	3367	PASS
275	198	10	60	26.0	13127	PASS
365	198	1	100	5.3	2675	PASS
441	198	0.01	100	11.3	5714	PASS
442	442	50	100	100.0	31557	PASS
443	442	15	24	20.1	6344	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037223.D
Acq On : 13 Jun 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 13 18:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 10 06:01:37 2025
Response via : Initial Calibration

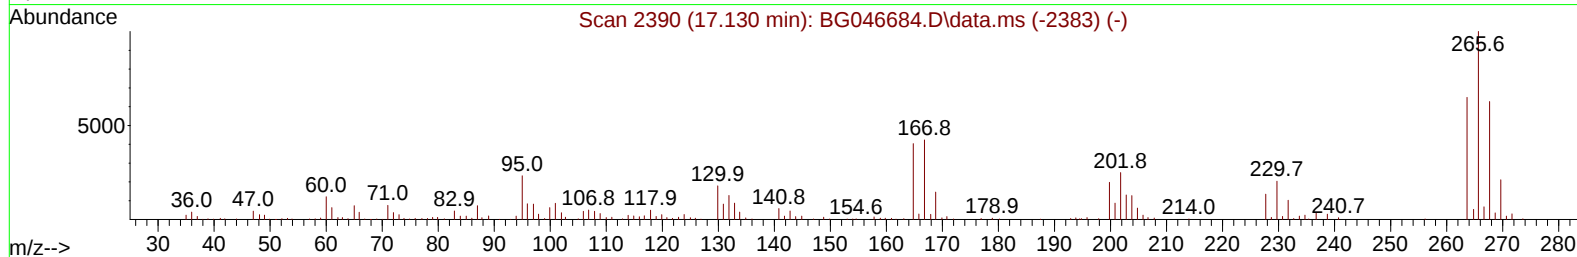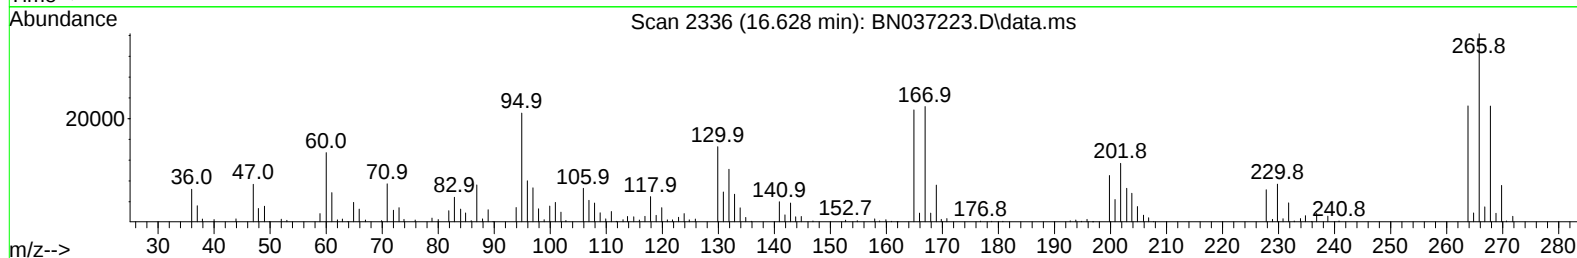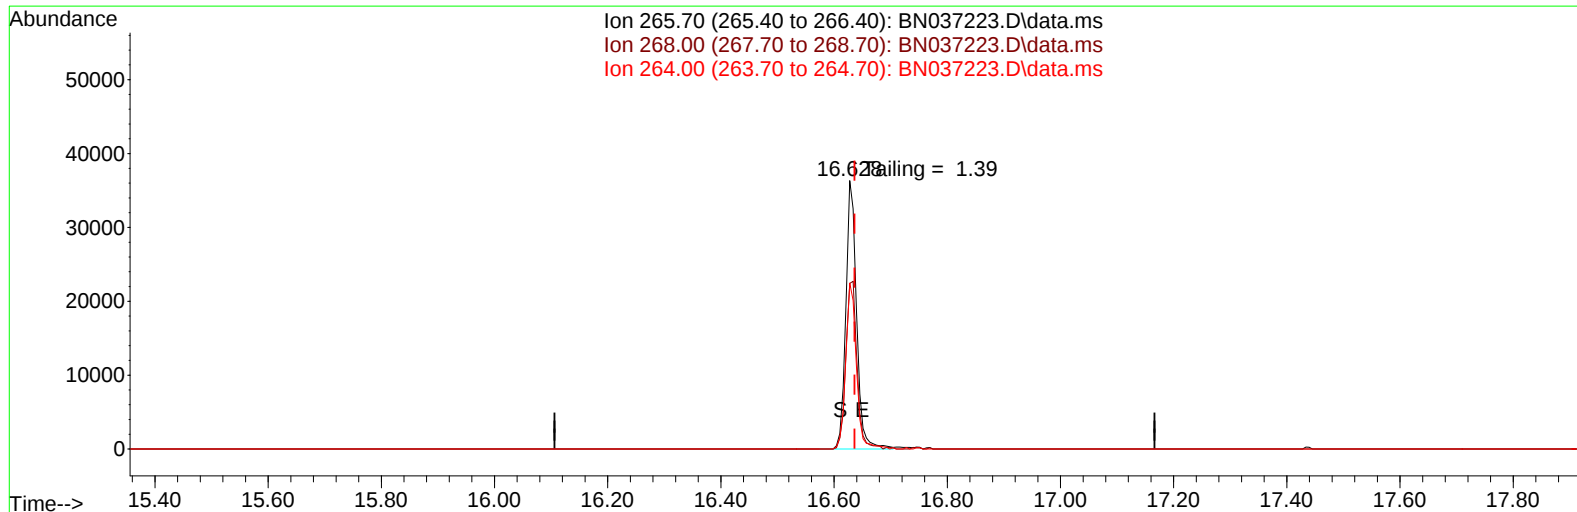

TIC: BN037223.D\data.ms

(70) Pentachlorophenol (C)

16.628min (-0.008) 13765.31 ng




response 48504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.73
264.00	61.60	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037223.D
Acq On : 13 Jun 2025 11:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 13 18:35:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 10 06:01:37 2025
Response via : Initial Calibration

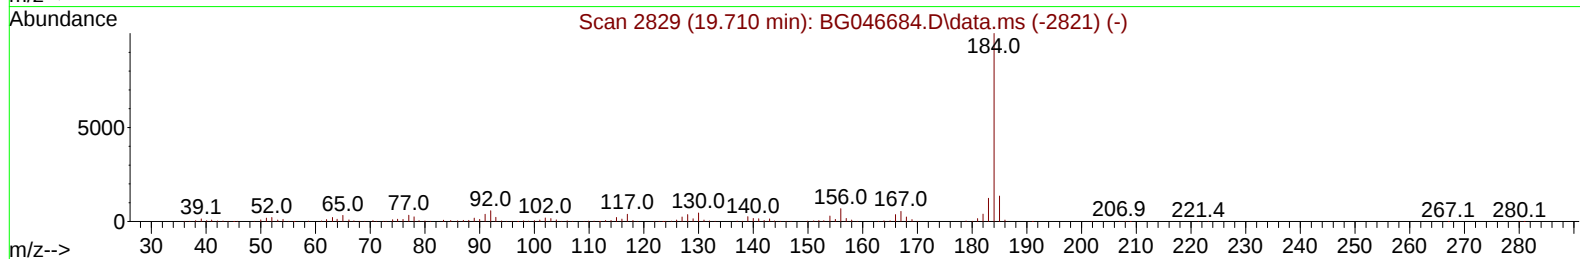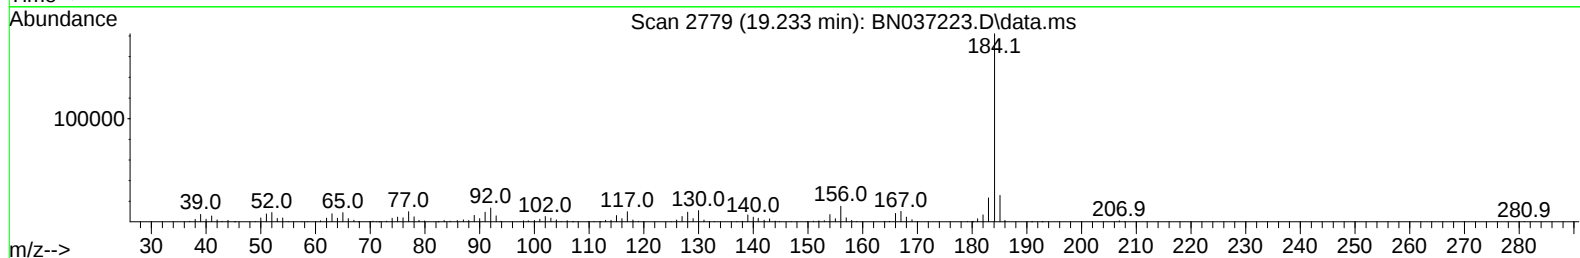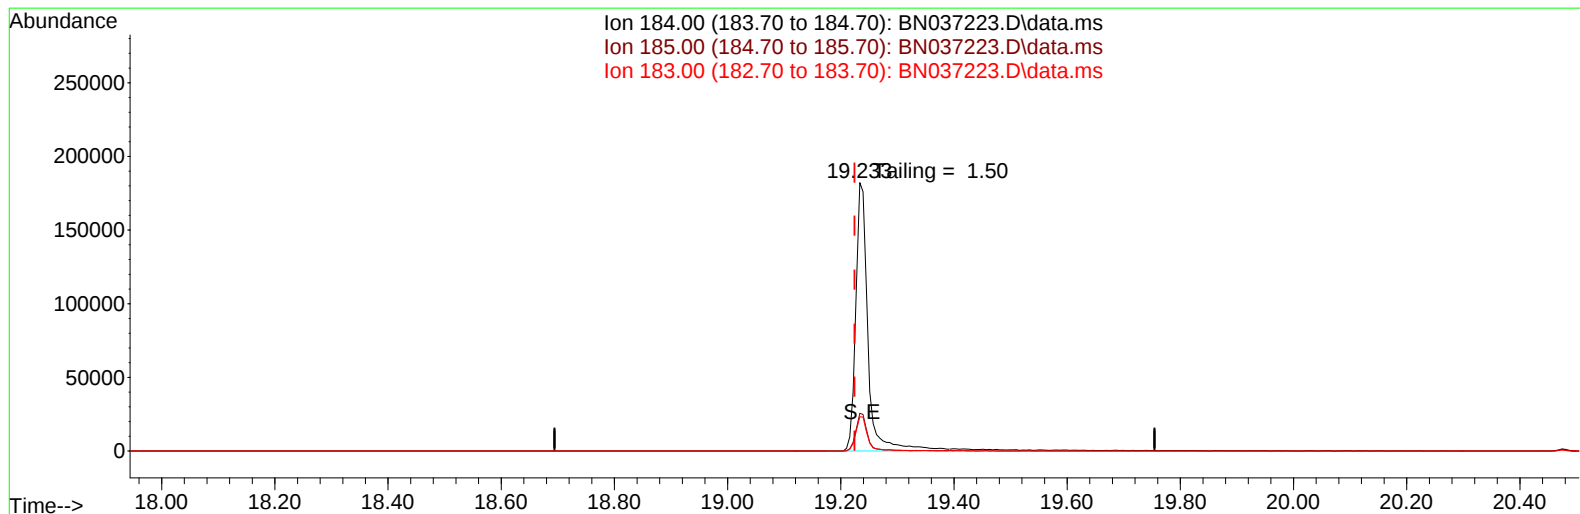

TIC: BN037223.D\data.ms

(77) Benzidine

19.233min (+ 0.009) 0.00 ng

response 272616

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	12.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_N	<u>BN037223.D</u>
Compound Name	Response	Retention Time
DDT	179828	20.475
DDD	1789	20.086
DDE	62	19.528
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1851	181679	1.02

Instrument :
BNA_N
ClientSampleId :
DFTPP