
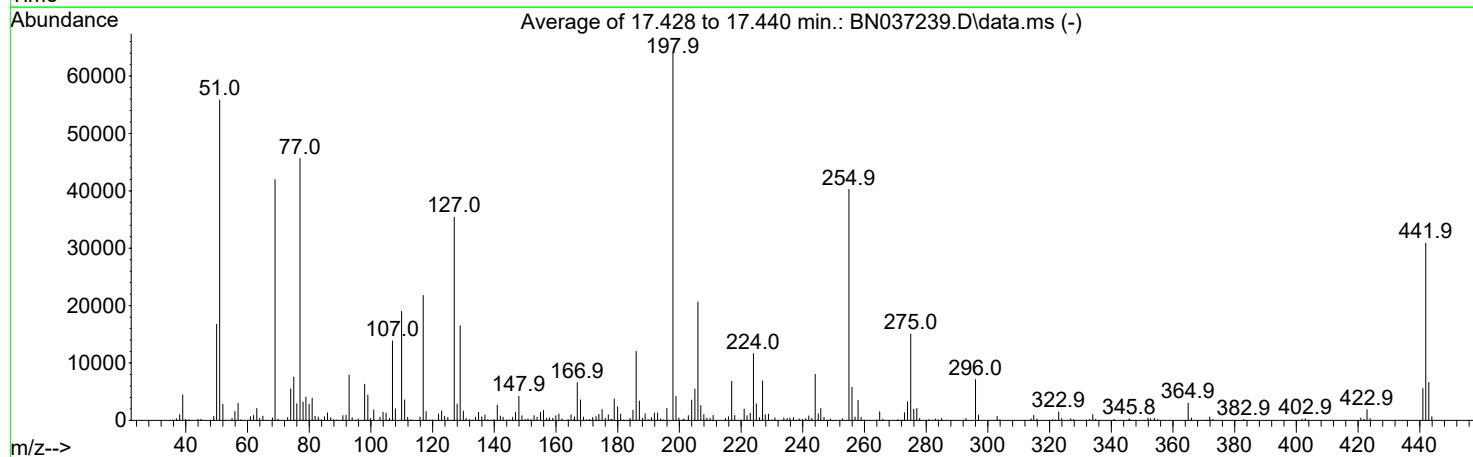


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037239.D
Acq On : 13 Jun 2025 23:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN061325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 13 18:43:34 2025

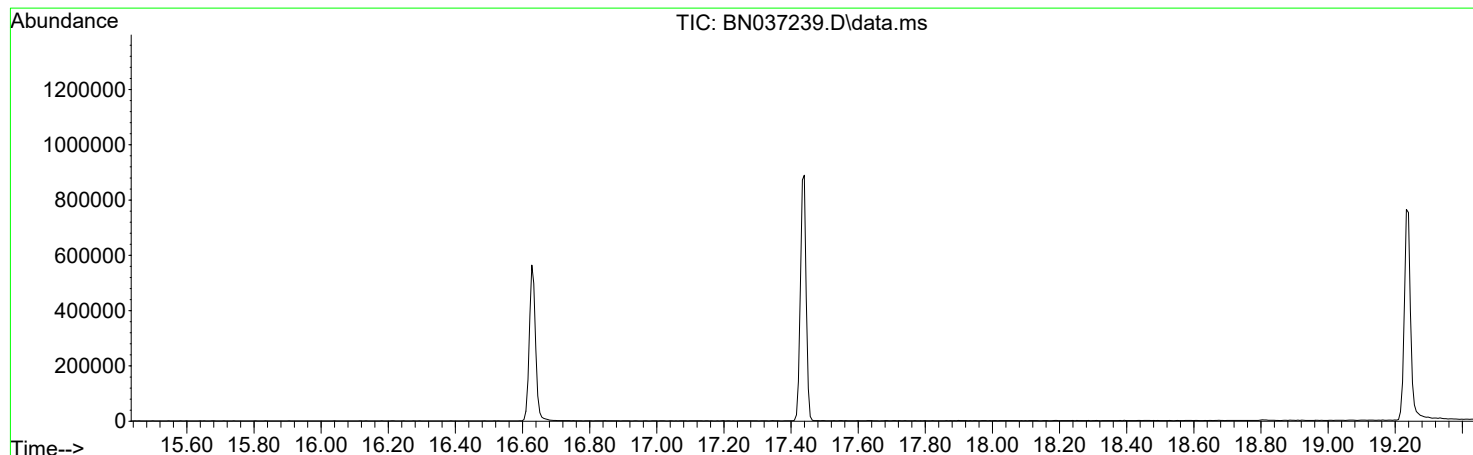

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	87.1	55816	FAIL*
68	69	0.00	2	1.0	417	PASS
69	198	0.00	100	65.4	41957	PASS
70	69	0.00	2	0.6	239	PASS
127	198	10	80	55.2	35408	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64112	PASS
199	198	5	9	6.5	4172	PASS
275	198	10	60	23.4	15028	PASS
365	198	1	100	4.7	3005	PASS
441	198	0.01	100	8.7	5553	PASS
442	442	50	100	100.0	30862	PASS
443	442	15	24	21.5	6621	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_N	<u>BN037239.D</u>
Compound Name	Response	Retention Time
DDT	204788	20.475
DDD	3055	20.039
DDE	55	19.528
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3110	207898	1.50

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037239.D
Acq On : 13 Jun 2025 23:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 14 03:28:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 14 03:28:35 2025
Response via : Initial Calibration

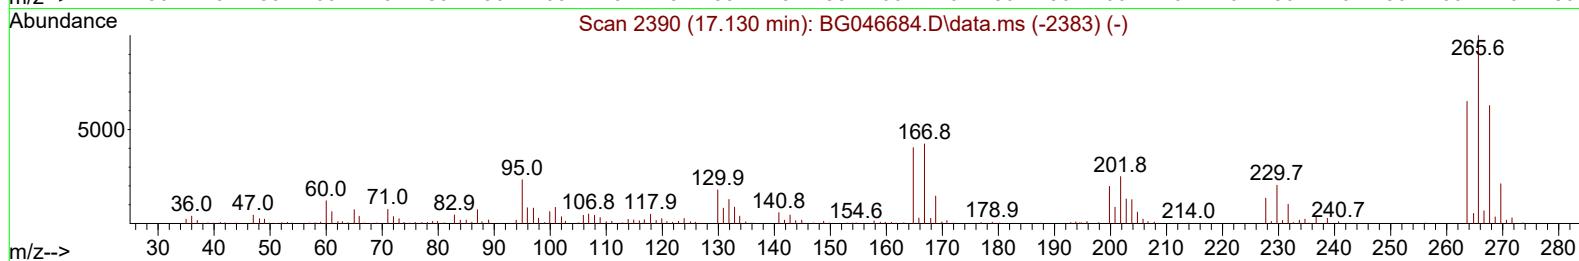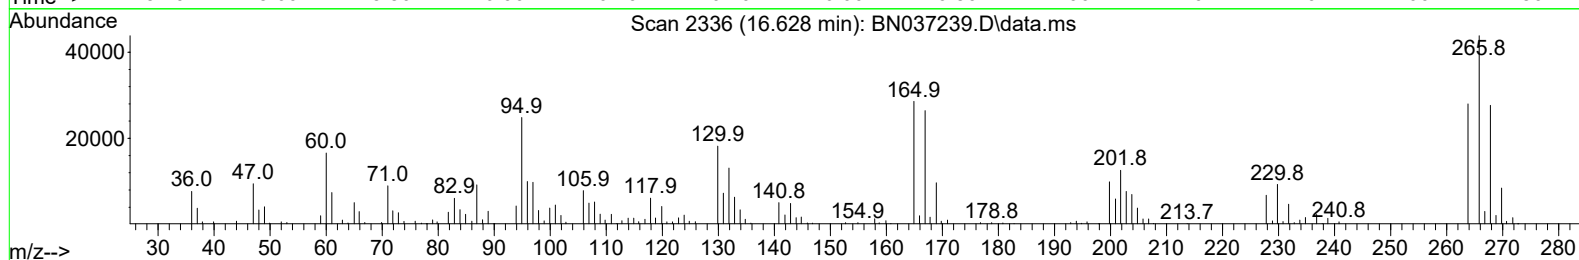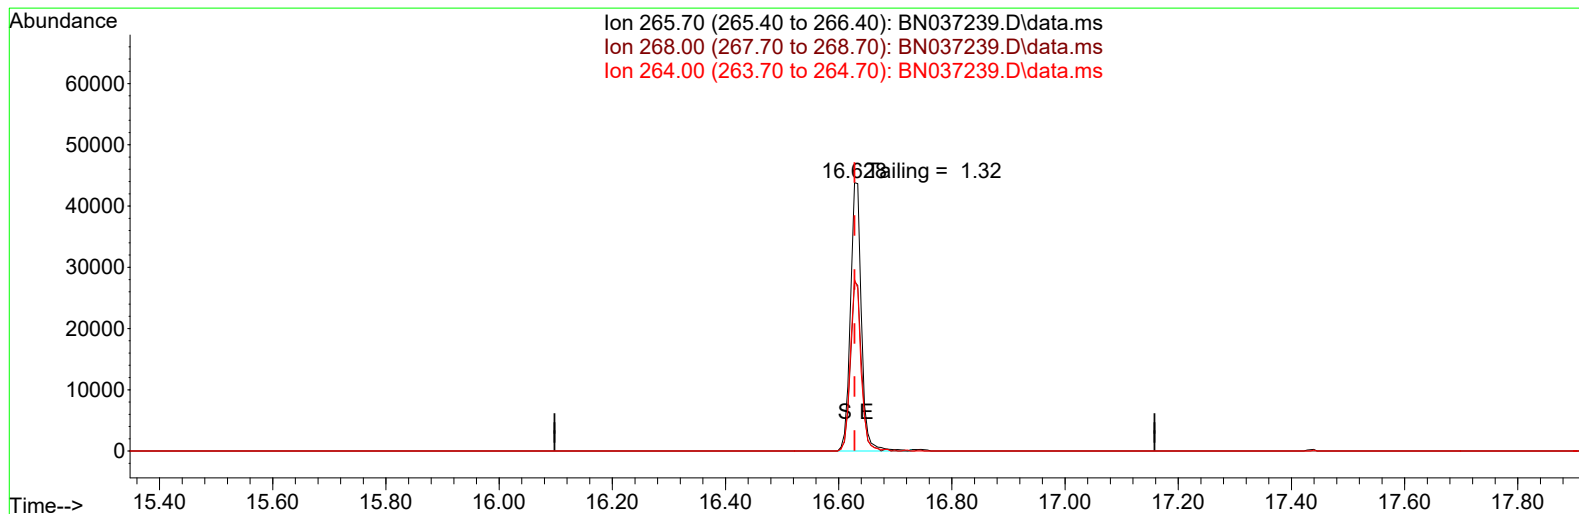

TIC: BN037239.D\data.ms

(70) Pentachlorophenol (C)

16.628min (0.000) 18785.64 ng




response 58970

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.13
264.00	61.60	63.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037239.D
Acq On : 13 Jun 2025 23:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 14 03:28:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 14 03:28:35 2025
Response via : Initial Calibration

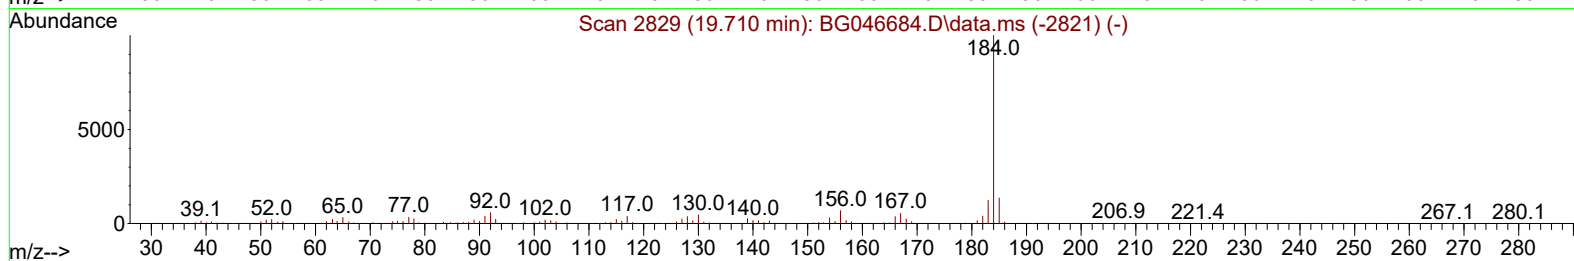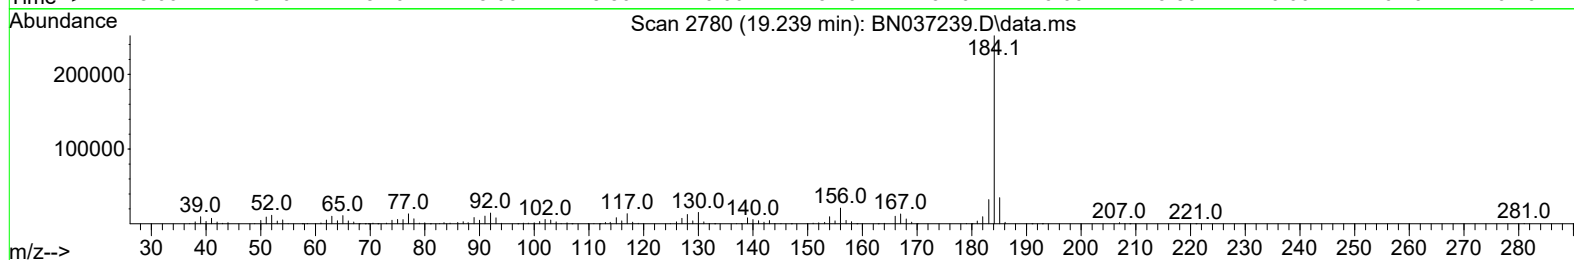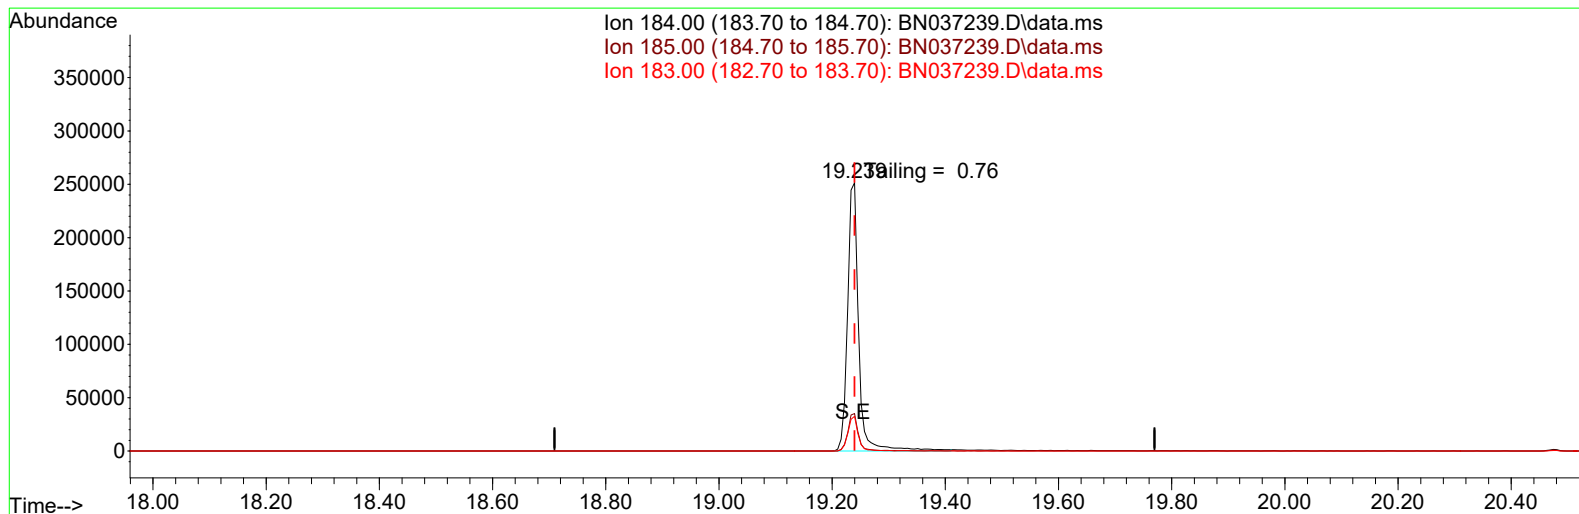

TIC: BN037239.D\data.ms

(77) Benzidine

19.239min (0.000) 0.00 ng

response 344668

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	12.95
0.00	0.00	0.00