

Cover Page

Order ID : Q2267

Project ID : Con Ed Non MGP – Atlantic Ave 453957.600024.05

Client : PARSONS Engineering of New York, Inc.

Lab Sample Number

Q2267-01

Client Sample Number

WC-20250605

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 6/14/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q2267

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Custody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: KETAN PATEL

Date: 06/14/2025



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

LAB CHRONICLE

OrderID:	Q2267	OrderDate:	6/6/2025 2:17:00 PM
Client:	PARSONS Engineering of New York, Inc.	Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05
Contact:	Stephen Liberatore	Location:	D41

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2267-01	WC-20250605	WATER	PCB	8082A	06/05/25	06/10/25	06/10/25	06/06/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q2267

Order ID: Q2267

Client: PARSONS Engineering of New York, Inc.

Project ID: Con Ed Non MGP – Atlantic Ave 4539

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: Q2267

Client: PARSONS Engineering of New York, Inc.

Analytical Method: 8082A

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO111057.D	PIBLK-PO111057.D	Tetrachloro-m-xylene	1	20	16.4	82		60	140
		Decachlorobiphenyl	1	20	17.5	87		60	140
		Tetrachloro-m-xylene	2	20	15.4	77		60	140
		Decachlorobiphenyl	2	20	17.9	90		60	140
I.BLK-PO111573.D	PIBLK-PO111573.D	Tetrachloro-m-xylene	1	20	21.8	109		60	140
		Decachlorobiphenyl	1	20	20.7	104		60	140
		Tetrachloro-m-xylene	2	20	20.0	100		60	140
		Decachlorobiphenyl	2	20	19.4	97		60	140
PB168377BL	PB168377BL	Tetrachloro-m-xylene	1	20	23.5	118		30	173
		Decachlorobiphenyl	1	20	22.1	111		10	173
		Tetrachloro-m-xylene	2	20	21.4	107		30	173
		Decachlorobiphenyl	2	20	20.6	103		10	173
PB168377BS	PB168377BS	Tetrachloro-m-xylene	1	20	21.8	109		30	173
		Decachlorobiphenyl	1	20	22.1	111		10	173
		Tetrachloro-m-xylene	2	20	20.0	100		30	173
		Decachlorobiphenyl	2	20	20.6	103		10	173
PB168377BSD	PB168377BSD	Tetrachloro-m-xylene	1	20	21.2	106		30	173
		Decachlorobiphenyl	1	20	22.0	110		10	173
		Tetrachloro-m-xylene	2	20	20.0	100		30	173
		Decachlorobiphenyl	2	20	20.7	104		10	173
Q2267-01	WC-20250605	Tetrachloro-m-xylene	1	20	20.3	101		30	173
		Decachlorobiphenyl	1	20	4.19	21		10	173
		Tetrachloro-m-xylene	2	20	18.4	92		30	173
		Decachlorobiphenyl	2	20	3.98	20		10	173
I.BLK-PO111584.D	PIBLK-PO111584.D	Tetrachloro-m-xylene	1	20	21.6	108		60	140
		Decachlorobiphenyl	1	20	20.3	101		60	140
		Tetrachloro-m-xylene	2	20	19.9	100		60	140
		Decachlorobiphenyl	2	20	19.2	96		60	140



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q2267</u>	Analytical Method:	<u>8082A</u>
Client:	<u>PARSONS Engineering of New York, Inc</u>	Datafile :	<u>PO111575.D</u>

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Low	Limits	RPD
								Qual		High	
PB168377BS (Column 1)	AR1016	5	4.70	ug/L	94				77	107	
	AR1260	5	5.00	ug/L	100				66	113	
PB168377BS (Column 2)	AR1016	5	4.20	ug/L	84				77	107	
	AR1260	5	4.00	ug/L	80				66	113	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2267

Analytical Method: 8082A

Client: PARSONS Engineering of New York, Inc

Datafile : PO111576.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD	Limits		RPD
								Qual	Low	High	
PB168377BSD (Column 1)	AR1016	5	4.90	ug/L	98	4			77	107	20
	AR1260	5	5.10	ug/L	102	2			66	113	20
PB168377BSD (Column 2)	AR1016	5	4.30	ug/L	86	2			77	107	20
	AR1260	5	4.10	ug/L	82	2			66	113	20

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB168377BL

Lab Name: CHEMTECH

Contract: PARS02

Lab Code: CHEM Case No.: Q2267

SAS No.: Q2267 SDG NO.: Q2267

Lab Sample ID: PB168377BL

Lab File ID: PO111574.D

Matrix: (soil/water) WATER

Extraction: (Type) SEPF

Sulfur Cleanup: (Y/N) N

Date Extracted: 06/10/2025

Date Analyzed (1): 06/10/2025

Date Analyzed (2): 06/10/2025

Time Analyzed (1): 14:28

Time Analyzed (2): 14:28

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB168377BS	PB168377BS	PO111575.D	06/10/2025	06/10/2025
PB168377BSD	PB168377BSD	PO111576.D	06/10/2025	06/10/2025
WC-20250605	Q2267-01	PO111579.D	06/10/2025	06/10/2025

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	PARSONS Engineering of New York, Inc.		Date Collected:	06/05/25	
Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05		Date Received:	06/06/25	
Client Sample ID:	WC-20250605		SDG No.:	Q2267	
Lab Sample ID:	Q2267-01		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	980	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO111579.D	1	06/10/25 09:00	06/10/25 16:00	PB168377

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.099	U	0.099	0.51	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.51	ug/L
11141-16-5	Aroclor-1232	0.098	U	0.098	0.51	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.51	ug/L
12672-29-6	Aroclor-1248	0.072	U	0.072	0.51	ug/L
11097-69-1	Aroclor-1254	0.096	U	0.096	0.51	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.51	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.51	ug/L
11096-82-5	Aroclor-1260	0.083	U	0.083	0.51	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.3		30 - 173	101%	SPK: 20
2051-24-3	Decachlorobiphenyl	4.19		10 - 173	21%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
 Data File : PO111579.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 16:00
 Operator : YP/AJ
 Sample : Q2267-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-20250605

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
 Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:28:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.679	3.675	119.3E6	100.3E6	20.282	18.408m
2) SA Decachlor...	8.714	8.664	21634537	7358945	4.190	3.977m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 16:00
Operator : YP/AJ
Sample : Q2267-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

WC-20250605

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 06/11/2025

Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:28:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

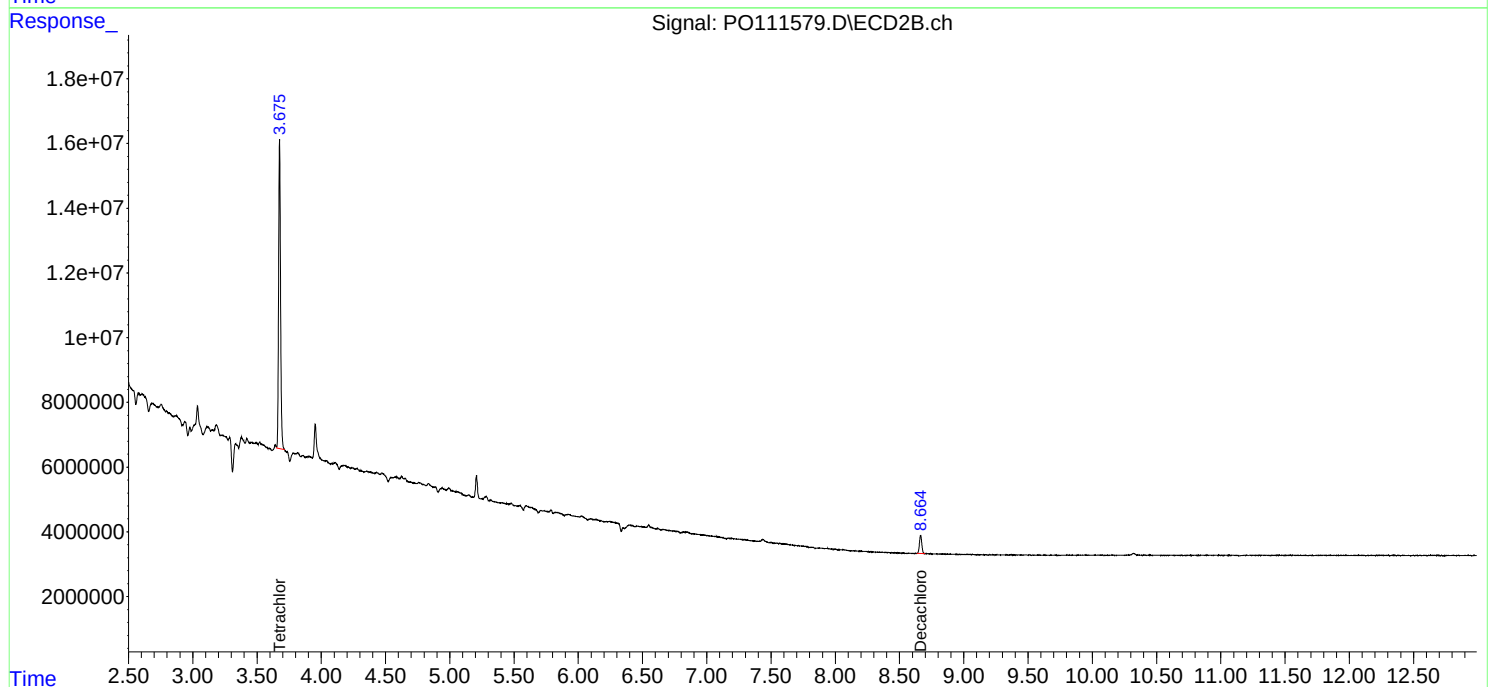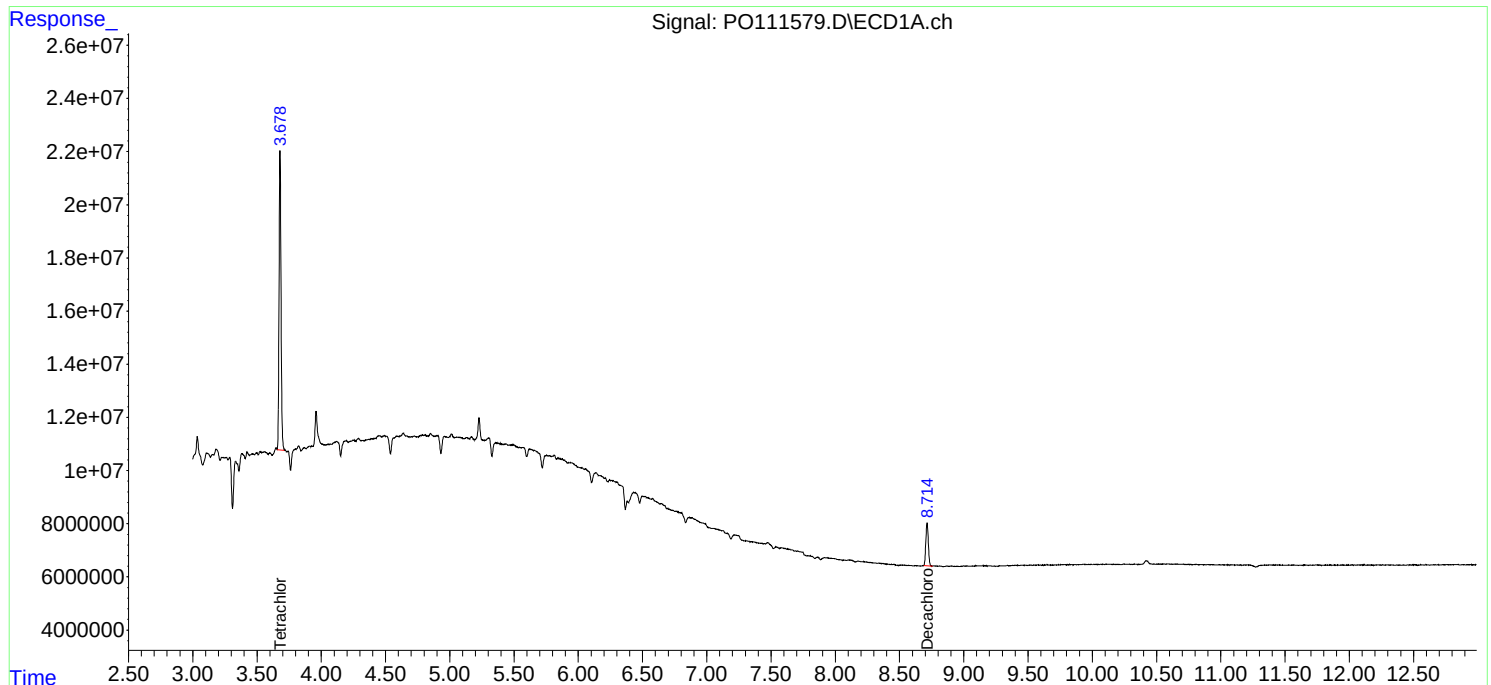

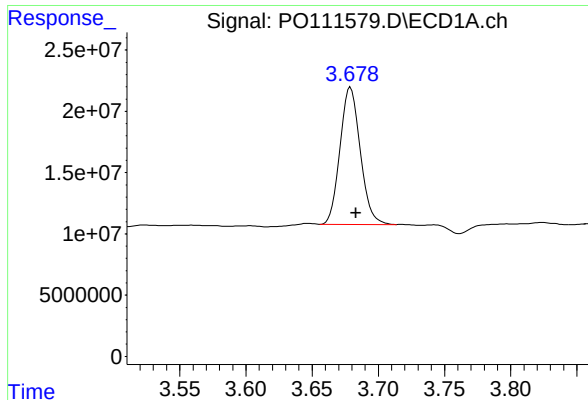


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: -0.004 min
Response: 119322412
Conc: 20.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-20250605


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

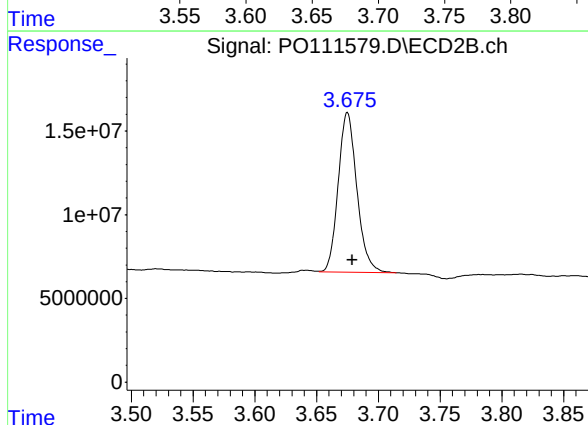


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.004 min
Response: 100348791
Conc: 18.41 ng/ml

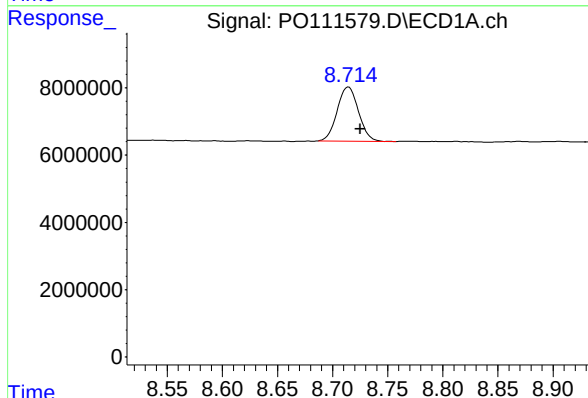

#2 Decachlorobiphenyl

R.T.: 8.714 min
Delta R.T.: -0.011 min
Response: 21634537
Conc: 4.19 ng/ml

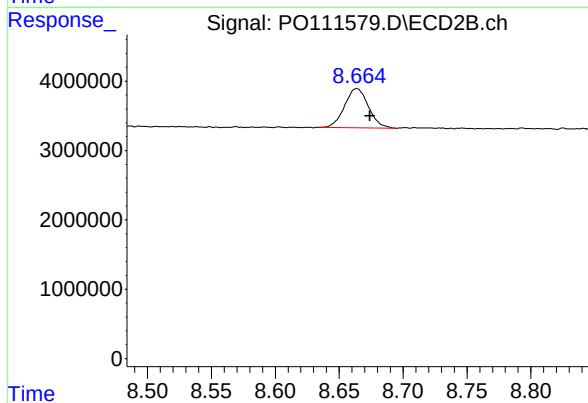

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: -0.011 min
Response: 7358945
Conc: 3.98 ng/ml



CALIBRATION SUMMARY

RETENTION TIMES OF INITIAL CALIBRATION

Contract: PARS02
Lab Code: CHEM **Case No.:** Q2267 **SAS No.:** Q2267 **SDG NO.:** Q2267
Instrument ID: ECD_O **Calibration Date(s):** 05/14/2025 05/15/2025
Calibration Times: 17:19 01:31

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 = <u>PO111058.D</u>	RT 750 = <u>PO111059.D</u>
RT 500 = <u>PO111060.D</u>	RT 250 = <u>PO111061.D</u>	RT 050 = <u>PO111062.D</u>

COMPOUND		RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW	
								FROM	TO
Aroclor-1016-1	(1)	4.77	4.77	4.77	4.77	4.77	4.77	4.67	4.87
Aroclor-1016-2	(2)	4.79	4.79	4.79	4.79	4.79	4.79	4.69	4.89
Aroclor-1016-3	(3)	4.85	4.85	4.85	4.85	4.85	4.85	4.75	4.95
Aroclor-1016-4	(4)	4.97	4.97	4.97	4.97	4.97	4.97	4.87	5.07
Aroclor-1016-5	(5)	5.23	5.23	5.23	5.23	5.23	5.23	5.13	5.33
Aroclor-1260-1	(1)	6.27	6.27	6.27	6.27	6.27	6.27	6.17	6.37
Aroclor-1260-2	(2)	6.46	6.46	6.46	6.46	6.45	6.46	6.36	6.56
Aroclor-1260-3	(3)	6.82	6.82	6.82	6.82	6.82	6.82	6.72	6.92
Aroclor-1260-4	(4)	7.08	7.08	7.08	7.08	7.08	7.08	6.98	7.18
Aroclor-1260-5	(5)	7.33	7.33	7.33	7.32	7.32	7.33	7.23	7.43
Decachlorobiphenyl		8.73	8.73	8.72	8.72	8.72	8.72	8.62	8.82
Tetrachloro-m-xylene		3.68	3.68	3.68	3.68	3.68	3.68	3.58	3.78
Aroclor-1242-1	(1)	4.77	4.77	4.77	4.77	4.77	4.77	4.67	4.87
Aroclor-1242-2	(2)	4.79	4.79	4.79	4.79	4.79	4.79	4.69	4.89
Aroclor-1242-3	(3)	4.85	4.85	4.85	4.85	4.85	4.85	4.75	4.95
Aroclor-1242-4	(4)	4.97	4.97	4.97	4.97	4.97	4.97	4.87	5.07
Aroclor-1242-5	(5)	5.62	5.62	5.62	5.62	5.62	5.62	5.52	5.72
Decachlorobiphenyl		8.72	8.72	8.73	8.72	8.72	8.72	8.62	8.82
Tetrachloro-m-xylene		3.68	3.68	3.68	3.68	3.68	3.68	3.58	3.78
Aroclor-1248-1	(1)	4.77	4.77	4.77	4.77	4.77	4.77	4.67	4.87
Aroclor-1248-2	(2)	5.01	5.01	5.01	5.01	5.01	5.01	4.91	5.11
Aroclor-1248-3	(3)	5.23	5.23	5.23	5.22	5.23	5.23	5.13	5.33
Aroclor-1248-4	(4)	5.58	5.58	5.58	5.58	5.58	5.58	5.48	5.68
Aroclor-1248-5	(5)	5.62	5.62	5.62	5.62	5.62	5.62	5.52	5.72
Decachlorobiphenyl		8.72	8.72	8.72	8.72	8.72	8.72	8.62	8.82
Tetrachloro-m-xylene		3.68	3.68	3.68	3.68	3.68	3.68	3.58	3.78
Aroclor-1254-1	(1)	5.58	5.58	5.58	5.58	5.58	5.58	5.48	5.68
Aroclor-1254-2	(2)	5.73	5.73	5.73	5.73	5.73	5.73	5.63	5.83
Aroclor-1254-3	(3)	6.13	6.13	6.13	6.13	6.13	6.13	6.03	6.23
Aroclor-1254-4	(4)	6.36	6.36	6.36	6.36	6.36	6.36	6.26	6.46
Aroclor-1254-5	(5)	6.78	6.78	6.78	6.78	6.78	6.78	6.68	6.88
Decachlorobiphenyl		8.73	8.73	8.72	8.72	8.72	8.72	8.62	8.82
Tetrachloro-m-xylene		3.68	3.68	3.68	3.68	3.68	3.68	3.58	3.78
Aroclor-1268-1	(1)	7.61	7.61	7.61	7.61	7.61	7.61	7.51	7.71
Aroclor-1268-2	(2)	7.67	7.67	7.67	7.67	7.67	7.67	7.57	7.77
Aroclor-1268-3	(3)	7.88	7.88	7.88	7.88	7.88	7.88	7.78	7.98
Aroclor-1268-4	(4)	8.17	8.17	8.17	8.17	8.17	8.17	8.07	8.27
Aroclor-1268-5	(5)	8.46	8.47	8.47	8.46	8.46	8.46	8.36	8.56

[illegible]

RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>PARS02</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q2267</u>	SAS No.:	<u>Q2267</u>	SDG NO.:	<u>Q2267</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):		<u>05/14/2025</u>	<u>05/15/2025</u>		
		Calibration Times:		<u>17:19</u>	<u>01:31</u>		

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID: RT 1000 = PO111058.D RT 750 = PO111059.D
RT 500 = PO111060.D RT 250 = PO111061.D RT 050 = PO111062.D

[illegible]

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: PARS02
Lab Code: CHEM **Case No.:** Q2267 **SAS No.:** Q2267 **SDG NO.:** Q2267
Instrument ID: ECD_O
Calibration Date(s): 05/14/2025 05/15/2025
Calibration Times: 17:19 01:31
GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO111058.D</u>		CF 750 = <u>PO111059.D</u>			
CF 500 = <u>PO111060.D</u>		CF 250 = <u>PO111061.D</u>		CF 050 = <u>PO111062.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	205952128	213833112	226414102	241684928	237394280	225055710 7
Aroclor-1016-2	(2)	293931044	310127113	321220528	340419712	328971000	318933879 6
Aroclor-1016-3	(3)	200116672	210641735	220217832	233629012	221015000	217124050 6
Aroclor-1016-4	(4)	160298181	168708089	176290662	187854588	177589060	174148116 6
Aroclor-1016-5	(5)	161898024	175820952	178167232	187226608	176844020	175991367 5
Aroclor-1260-1	(1)	277561674	293756041	305741896	331877740	315901980	304967866 7
Aroclor-1260-2	(2)	349775279	367746601	383860622	411536992	401831460	382950191 7
Aroclor-1260-3	(3)	317018248	333963835	348833732	373392584	369733400	348588360 7
Aroclor-1260-4	(4)	251785051	267674384	282392668	305806136	292149520	279961552 8
Aroclor-1260-5	(5)	680936092	706872008	727490352	760116820	724090440	719901142 4
Decachlorobiphenyl		4789049460	4988917347	5187039280	5515117840	5334237200	5162872225 6
Tetrachloro-m-xylene		5665666390	5873534533	6010307880	6167763840	5698750600	5883204649 4
Aroclor-1242-1	(1)	176697919	185695675	196416184	207079416	190109540	191199747 6
Aroclor-1242-2	(2)	257720398	267748761	279433570	293144628	262025820	272014635 5
Aroclor-1242-3	(3)	175187474	182923969	192610042	201232700	177980140	185986865 6
Aroclor-1242-4	(4)	140203851	146287348	153093646	159943472	139472860	147800235 6
Aroclor-1242-5	(5)	145186142	152022244	159321518	169027516	152152160	155541916 6
Decachlorobiphenyl		4774382260	4985278507	5225823760	5476782920	5013508400	5095155169 5
Tetrachloro-m-xylene		5680960800	5831614707	6040672820	6174416800	5348804000	5815293825 6
Aroclor-1248-1	(1)	138162515	145942143	153069466	163443424	165211980	153165906 8
Aroclor-1248-2	(2)	182760569	190399631	201027290	214399212	214001160	200517572 7
Aroclor-1248-3	(3)	227450486	238283761	250971210	267719672	295599780	256004982 10
Aroclor-1248-4	(4)	324783137	336810133	356284496	381846900	411181480	362181229 10
Aroclor-1248-5	(5)	233936098	243272008	257408728	275769428	299891040	262055460 10
Decachlorobiphenyl		4861959910	5031694707	5278313240	5604075320	5730172600	5301243155 7
Tetrachloro-m-xylene		5864549650	6045437613	6209272300	6477502560	6275643200	6174481065 4
Aroclor-1254-1	(1)	338668376	359337472	379562628	402119132	418187300	379574982 8
Aroclor-1254-2	(2)	291859728	310115756	327944084	347727744	356229960	326775454 8
Aroclor-1254-3	(3)	475332844	499809000	523764968	549245752	582561520	526142817 8
Aroclor-1254-4	(4)	302105681	318736953	335883014	351987900	371678540	336078418 8
Aroclor-1254-5	(5)	429218631	452008725	475302254	500931908	514812140	474454732 7
Decachlorobiphenyl		4923933440	5141137400	5443620080	5700682920	5862774600	5414429688 7
Tetrachloro-m-xylene		5948877150	6190104627	6408412200	6583454240	6338928400	6293955323 4
Aroclor-1268-1	(1)	930869745	936595251	978341018	1015935428	986319920	969612272 4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	856384474	860524951	901691384	934576100	909379560	892511294	4
Aroclor-1268-3	(3)	718671507	725558572	764699306	799960100	785246420	758827181	5
Aroclor-1268-4	(4)	311213814	313193287	331181486	347305704	329997080	326578274	5
Aroclor-1268-5	(5)	2117705977	2107339941	2194587578	2235031552	2137458100	2158424630	3
Decachlorobiphenyl		8888535700	9012836760	9503909100	9956674120	9729229000	9418236936	5
Tetrachloro-m-xylene		6171599970	6168104493	6441282720	6673989440	6170217200	6325038765	4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Instrument ID: ECD_O

Calibration Date(s): 05/14/2025 05/15/2025

Calibration Times: 17:19 01:31

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO111058.D</u>		CF 750 = <u>PO111059.D</u>			
CF 500 = <u>PO111060.D</u>		CF 250 = <u>PO111061.D</u>		CF 050 = <u>PO111062.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	175951340	184131151	190391494	201135208	203027340	190927307
Aroclor-1016-2	(2)	259304006	268965180	279695444	293662868	283996940	277124888
Aroclor-1016-3	(3)	136562816	142759844	148101780	155422472	147528240	146075030
Aroclor-1016-4	(4)	108537077	112835540	120886250	129636068	128548860	120088759
Aroclor-1016-5	(5)	141286439	151385859	154206636	161907480	163215520	154400387
Aroclor-1260-1	(1)	230380518	239225432	248869338	264781264	266186040	249888518
Aroclor-1260-2	(2)	272772980	284661173	294194664	310691584	309118120	294287704
Aroclor-1260-3	(3)	260160385	271476124	281551496	303268832	317136960	286718759
Aroclor-1260-4	(4)	184546577	192670083	200645580	215256196	210698140	200763315
Aroclor-1260-5	(5)	441090120	451615468	461646416	479352764	464333260	459607606
Decachlorobiphenyl		1699216120	1787921307	1869222220	1982547480	1911821600	1850145745
Tetrachloro-m-xylene		5406429520	5548905467	5601909540	5641328400	5058606000	5451435785
Aroclor-1242-1	(1)	150759764	157292616	165241112	172974524	159265900	161106783
Aroclor-1242-2	(2)	223621907	231686419	240612100	250441092	226668900	234606084
Aroclor-1242-3	(3)	118098683	122379071	128101210	133446692	116067680	123618667
Aroclor-1242-4	(4)	114724574	119985329	127001834	134027396	122337120	123615251
Aroclor-1242-5	(5)	142391198	148226844	155505330	163277824	150532140	151986667
Decachlorobiphenyl		1649752350	1732528187	1806674400	1933059040	1771454800	1778693755
Tetrachloro-m-xylene		5396035140	5504454880	5603860600	5606837360	4728358600	5367909316
Aroclor-1248-1	(1)	116677575	122377953	128716756	138512244	142355880	129728082
Aroclor-1248-2	(2)	159784658	166591041	175162942	187618608	190301260	175891702
Aroclor-1248-3	(3)	169685896	176680541	185649606	199757956	206297360	187614272
Aroclor-1248-4	(4)	198935902	206440528	216987222	226820008	250016460	219840024
Aroclor-1248-5	(5)	198293592	205844156	215149564	228236984	244101860	218325231
Decachlorobiphenyl		1675757640	1739961147	1894631500	1998157320	2119618200	1885625161
Tetrachloro-m-xylene		5392118780	5499156400	5577007680	5634478280	5189850400	5458522308
Aroclor-1254-1	(1)	294845056	308276565	323607480	339068536	354395480	324038623
Aroclor-1254-2	(2)	254192198	266619067	281454614	297953104	316004460	283244689
Aroclor-1254-3	(3)	400479051	415178477	433542960	448248844	459811580	431452182
Aroclor-1254-4	(4)	228881544	238106540	250287146	259634416	259809520	247343833
Aroclor-1254-5	(5)	318351803	329524227	344594700	358702264	378528780	345940355
Decachlorobiphenyl		1730307610	1804634267	1900572880	2018627520	2049052800	1900639015
Tetrachloro-m-xylene		5453750800	5591916973	5732062480	5726435600	5385705600	5577974291
Aroclor-1268-1	(1)	505658591	508360996	529570342	550274560	556601860	530093270



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	460495321	464888113	483851588	503248308	499197120	482336090	4
Aroclor-1268-3	(3)	328655790	333834055	349506788	366413796	363835440	348449174	5
Aroclor-1268-4	(4)	119697414	122740856	130580600	138639360	124687920	127269230	6
Aroclor-1268-5	(5)	727936615	731233425	757715258	780322444	766884820	752818512	3
Decachlorobiphenyl		3022618140	3077226480	3258756880	3437439920	3301382200	3219484724	5
Tetrachloro-m-xylene		5636439670	5594566640	5754942040	5800136080	5153076200	5587832126	5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Instrument ID: ECD_O Date(s) Analyzed: 05/14/2025 05/15/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.90	3.80	4.00	87106400
		2	3.98	3.88	4.08	63703800
		3	4.06	3.96	4.16	192327000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.06	3.96	4.16	153174000
		2	4.55	4.45	4.65	81946400
		3	4.79	4.69	4.89	152927000
		4	4.97	4.87	5.07	82251400
		5	5.01	4.91	5.11	54259200
Aroclor-1262	500	1	6.82	6.72	6.92	486664000
		2	7.33	7.23	7.43	808494000
		3	7.61	7.51	7.71	338264000
		4	7.67	7.57	7.77	590414000
		5	8.17	8.07	8.27	285216000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Instrument ID: ECD_O Date(s) Analyzed: 05/14/2025 05/15/2025

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.89	3.79	3.99	73843000
		2	3.98	3.88	4.08	54414200
		3	4.05	3.95	4.15	167101000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.05	3.95	4.15	130595000
		2	4.78	4.68	4.88	131160000
		3	4.95	4.85	5.05	68071600
		4	5.04	4.94	5.14	61676400
		5	5.21	5.11	5.31	65732600
Aroclor-1262	500	1	6.79	6.69	6.89	340780000
		2	7.29	7.19	7.39	502862000
		3	7.57	7.47	7.67	187635000
		4	7.64	7.54	7.74	330230000
		5	8.13	8.03	8.23	112306000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 17:19
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 18:08:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 14 18:04:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	566.6E6	540.6E6	97.048	98.224
2) SA Decachlor...	8.725	8.674	478.9E6	169.9E6	96.011	95.236
Target Compounds						
3) L1 AR-1016-1	4.774	4.758	206.0E6	176.0E6	952.674	960.583
4) L1 AR-1016-2	4.792	4.777	293.9E6	259.3E6	955.638	962.168
5) L1 AR-1016-3	4.849	4.952	200.1E6	136.6E6	952.178	959.465
6) L1 AR-1016-4	4.969	4.995	160.3E6	108.5E6	952.487	946.173
7) L1 AR-1016-5	5.226	5.207	161.9E6	141.3E6	952.159	956.276
31) L7 AR-1260-1	6.265	6.238	277.6E6	230.4E6	951.689	961.421
32) L7 AR-1260-2	6.456	6.426	349.8E6	272.8E6	953.539	962.217
33) L7 AR-1260-3	6.822	6.579	317.0E6	260.2E6	952.218	960.512
34) L7 AR-1260-4	7.083	7.049	251.8E6	184.5E6	942.701	958.205
35) L7 AR-1260-5	7.325	7.290	680.9E6	441.1E6	966.946	977.229



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 17:19
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 18:08:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 14 18:04:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

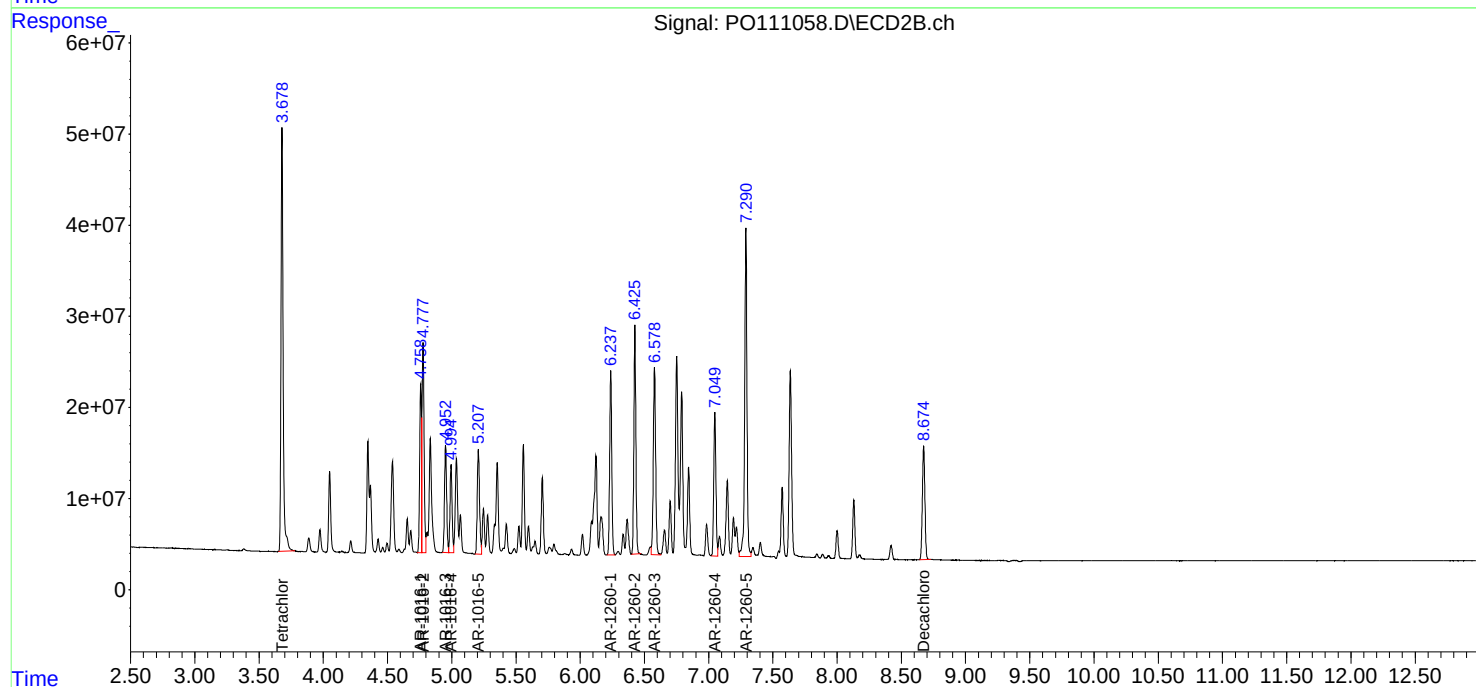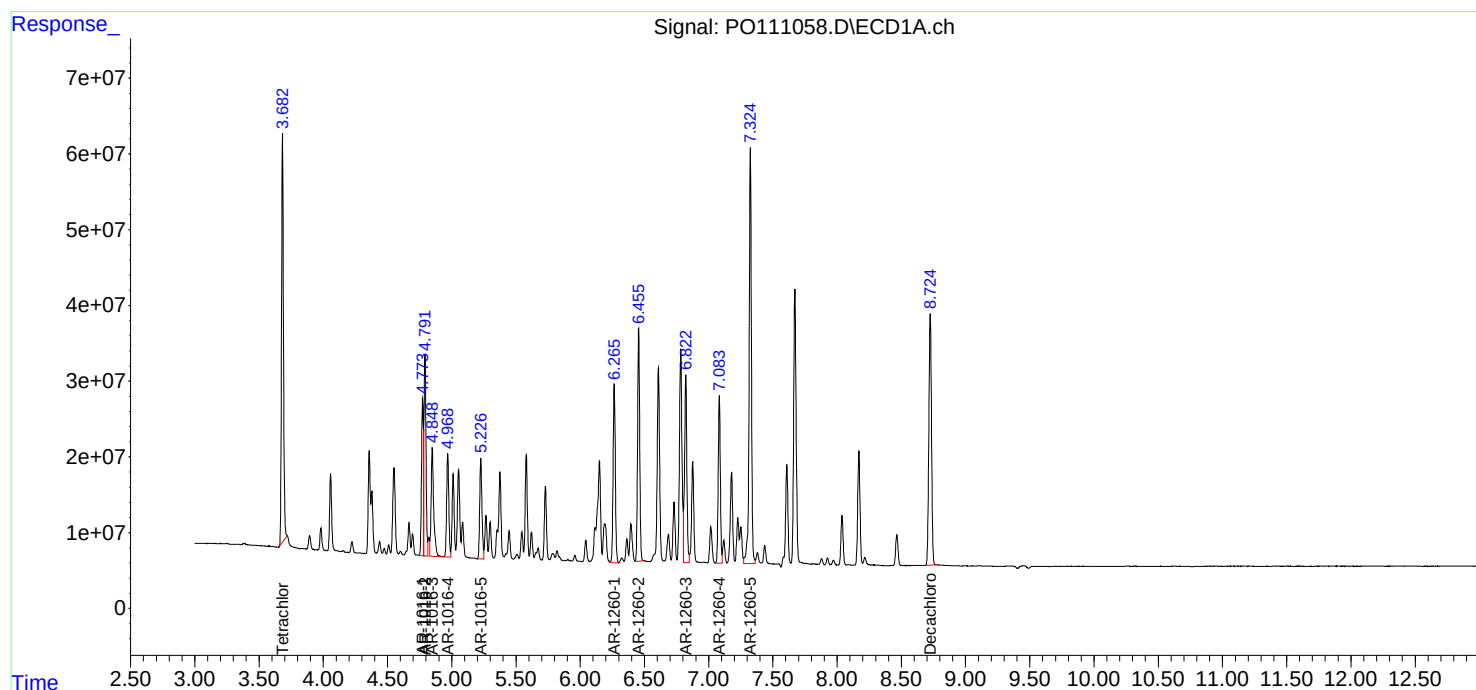

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 17:38
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/15/2025
 Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 18:11:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 14 18:04:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.679	440.5E6	416.2E6	75.304	75.405
2) SA Decachlor...	8.725	8.674	374.2E6	134.1E6	75.009	75.104
Target Compounds						
3) L1 AR-1016-1	4.773	4.759	160.4E6	138.1E6	744.545	752.615
4) L1 AR-1016-2	4.792	4.777	232.6E6	201.7E6	754.136	749.008
5) L1 AR-1016-3	4.848	4.953	158.0E6	107.1E6	751.128	751.500
6) L1 AR-1016-4	4.968	4.995	126.5E6	84626655	751.228	741.778
7) L1 AR-1016-5	5.226	5.208	131.9E6	113.5E6	766.830	762.216
31) L7 AR-1260-1	6.266	6.238	220.3E6	179.4E6	753.599	749.166
32) L7 AR-1260-2	6.455	6.427	275.8E6	213.5E6	751.265	752.074
33) L7 AR-1260-3	6.822	6.578	250.5E6	203.6E6	751.557	751.527m
34) L7 AR-1260-4	7.083	7.050	200.8E6	144.5E6	751.095	750.192
35) L7 AR-1260-5	7.325	7.291	530.2E6	338.7E6	751.885	750.274

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 17:38
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/15/2025
Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 18:11:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 14 18:04:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

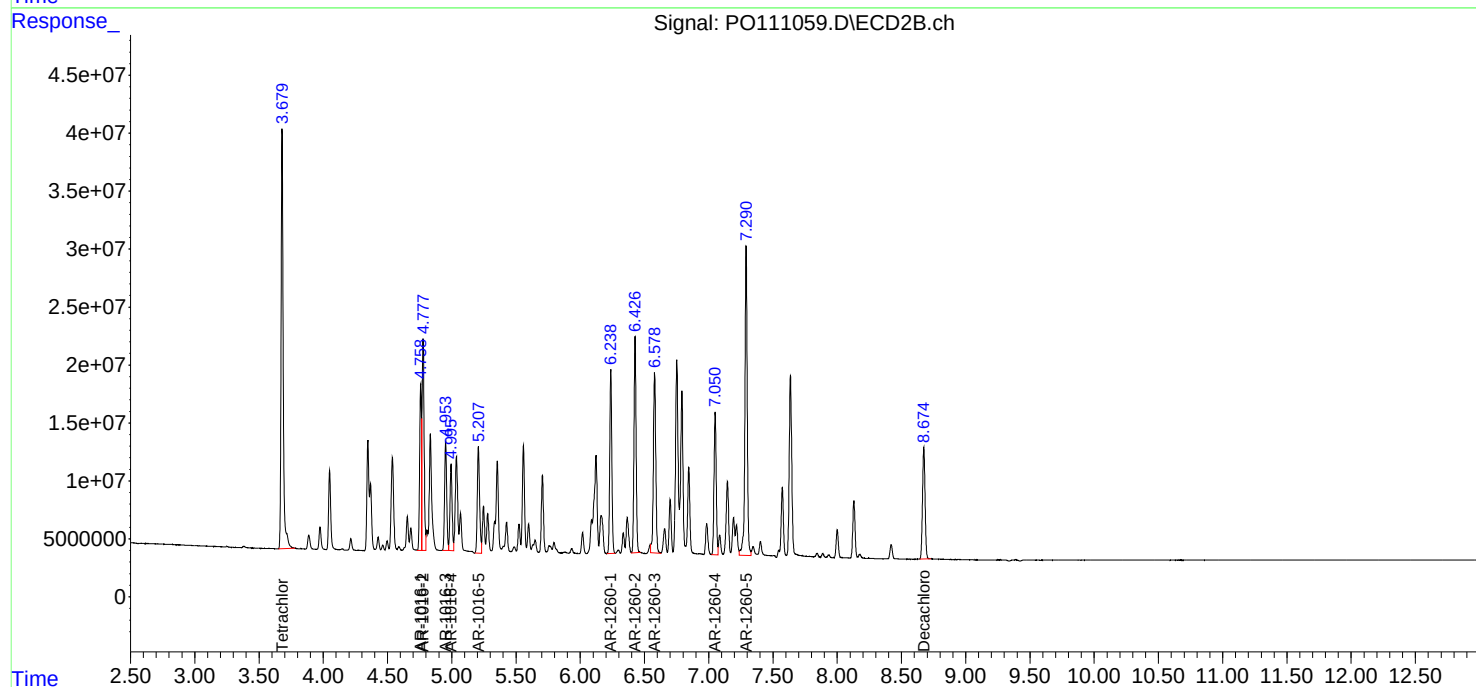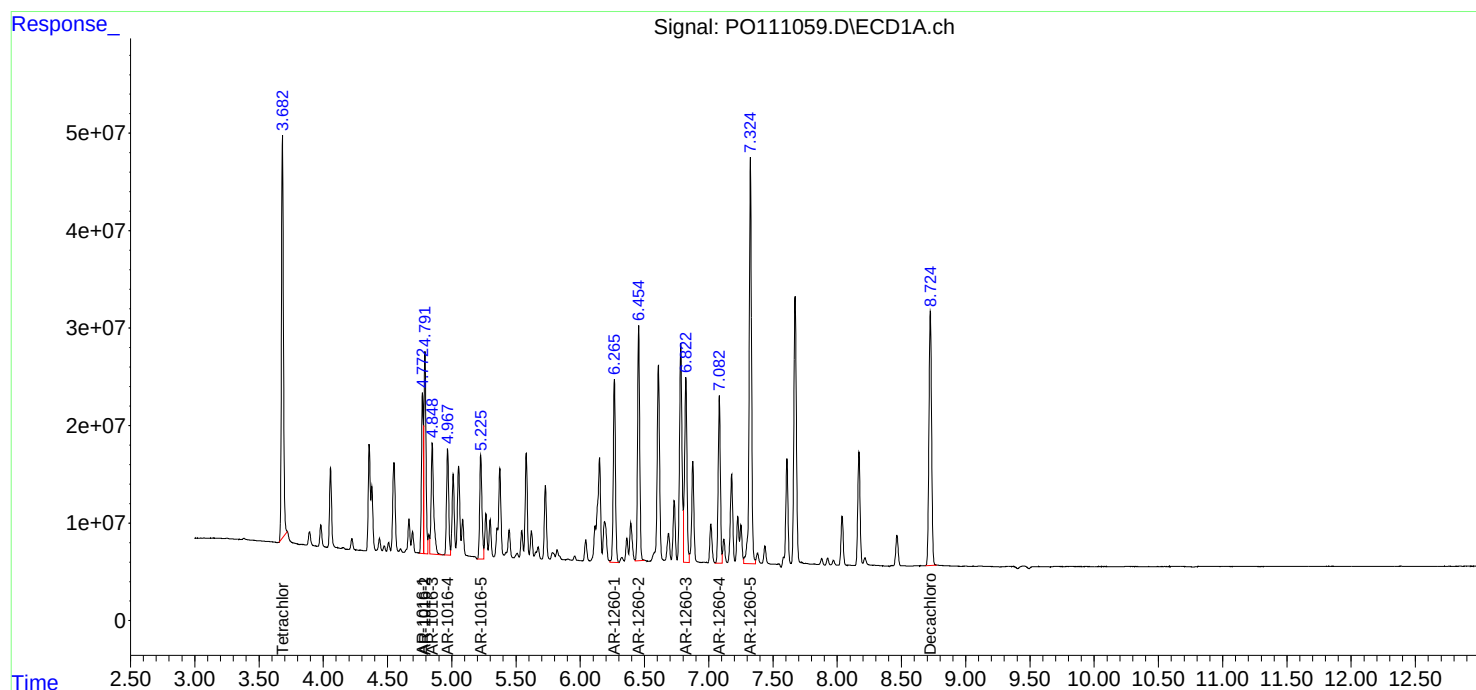

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 17:56
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 18:04:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 14 18:04:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.679	300.5E6	280.1E6	50.000	50.000
2) SA Decachlor...	8.724	8.674	259.4E6	93461111	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	4.773	4.758	113.2E6	95195747	500.000	500.000
4) L1 AR-1016-2	4.792	4.777	160.6E6	139.8E6	500.000	500.000
5) L1 AR-1016-3	4.849	4.952	110.1E6	74050890	500.000	500.000
6) L1 AR-1016-4	4.969	4.994	88145331	60443125	500.000	500.000
7) L1 AR-1016-5	5.226	5.207	89083616	77103318	500.000	500.000
31) L7 AR-1260-1	6.266	6.238	152.9E6	124.4E6	500.000	500.000
32) L7 AR-1260-2	6.455	6.426	191.9E6	147.1E6	500.000	500.000
33) L7 AR-1260-3	6.822	6.579	174.4E6	140.8E6	500.000	500.000
34) L7 AR-1260-4	7.083	7.049	141.2E6	100.3E6	500.000	500.000
35) L7 AR-1260-5	7.325	7.291	363.7E6	230.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 17:56
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 18:04:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 14 18:04:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

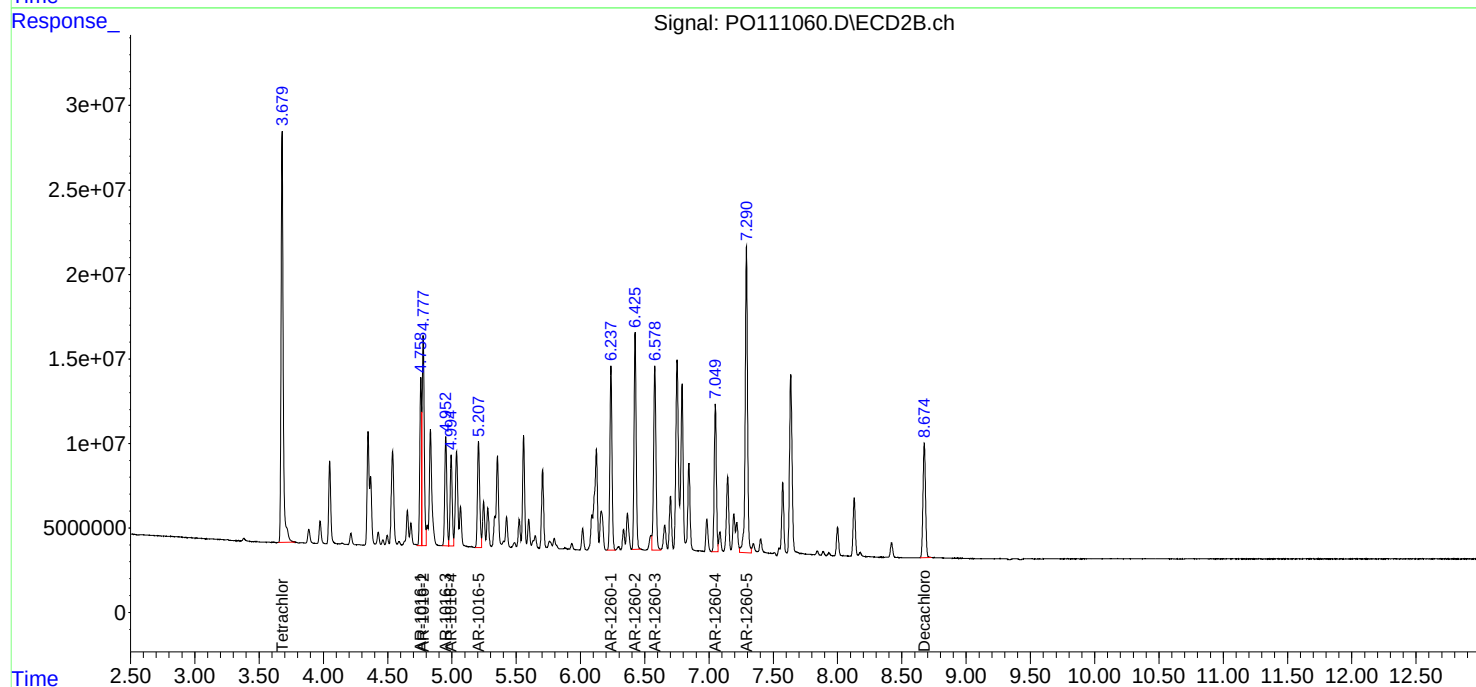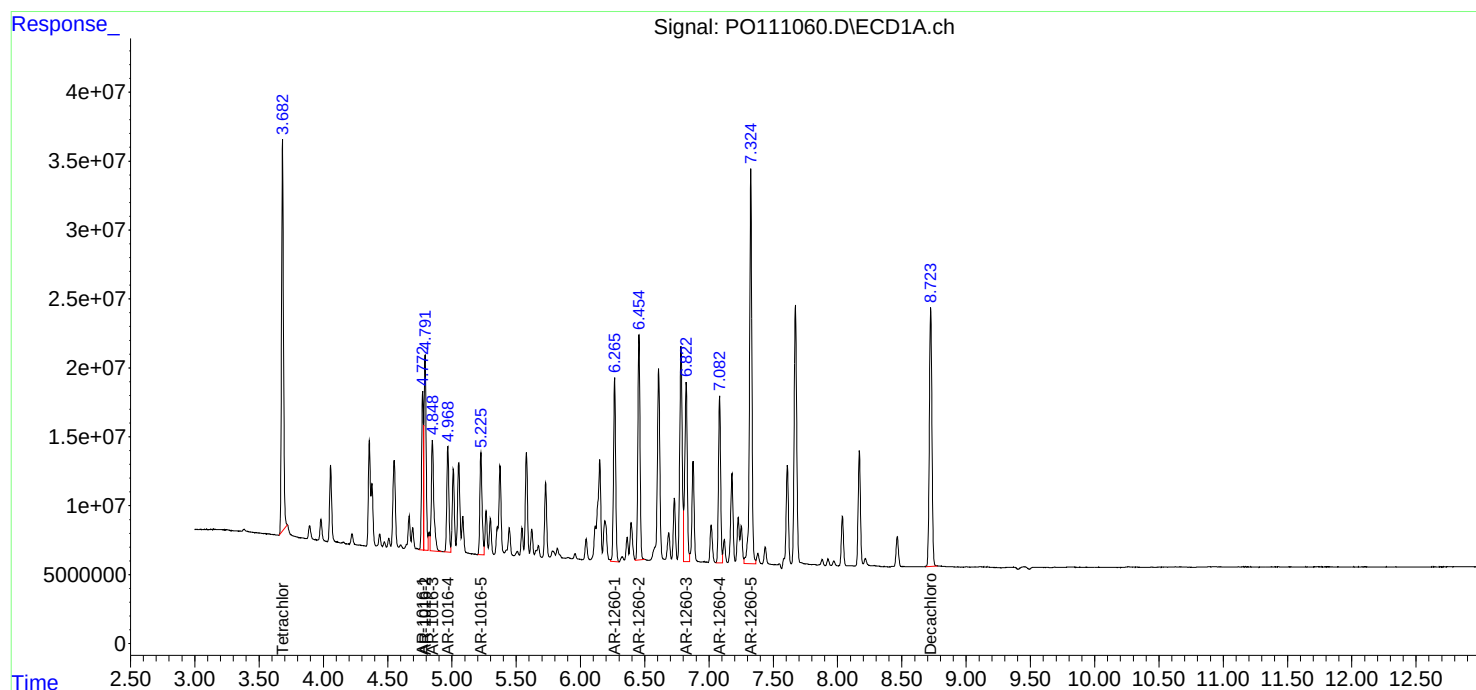

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 18:15
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/15/2025
 Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 18:23:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 14 18:22:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.679	154.2E6	141.0E6	26.005	25.413
2) SA Decachlor...	8.724	8.675	137.9E6	49563687	26.929	27.014
Target Compounds						
3) L1 AR-1016-1	4.772	4.758	60421232	50283802	272.203	267.606
4) L1 AR-1016-2	4.791	4.777	85104928	73415717	268.958	266.572
5) L1 AR-1016-3	4.847	4.952	58407253	38855618	271.623m	266.661
6) L1 AR-1016-4	4.968	4.994	46963647	32409017	271.015	274.714
7) L1 AR-1016-5	5.226	5.207	46806652	40476870	266.282	265.951
31) L7 AR-1260-1	6.265	6.237	82969435	66195316	274.520	269.290
32) L7 AR-1260-2	6.455	6.426	102.9E6	77672896	272.015	267.303
33) L7 AR-1260-3	6.822	6.578	93348146	75817208	271.913	271.635
34) L7 AR-1260-4	7.082	7.049	76451534	53814049	276.083	271.405
35) L7 AR-1260-5	7.324	7.290	190.0E6	119.8E6	264.350	261.412

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 18:15
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/15/2025
Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 18:23:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 14 18:22:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

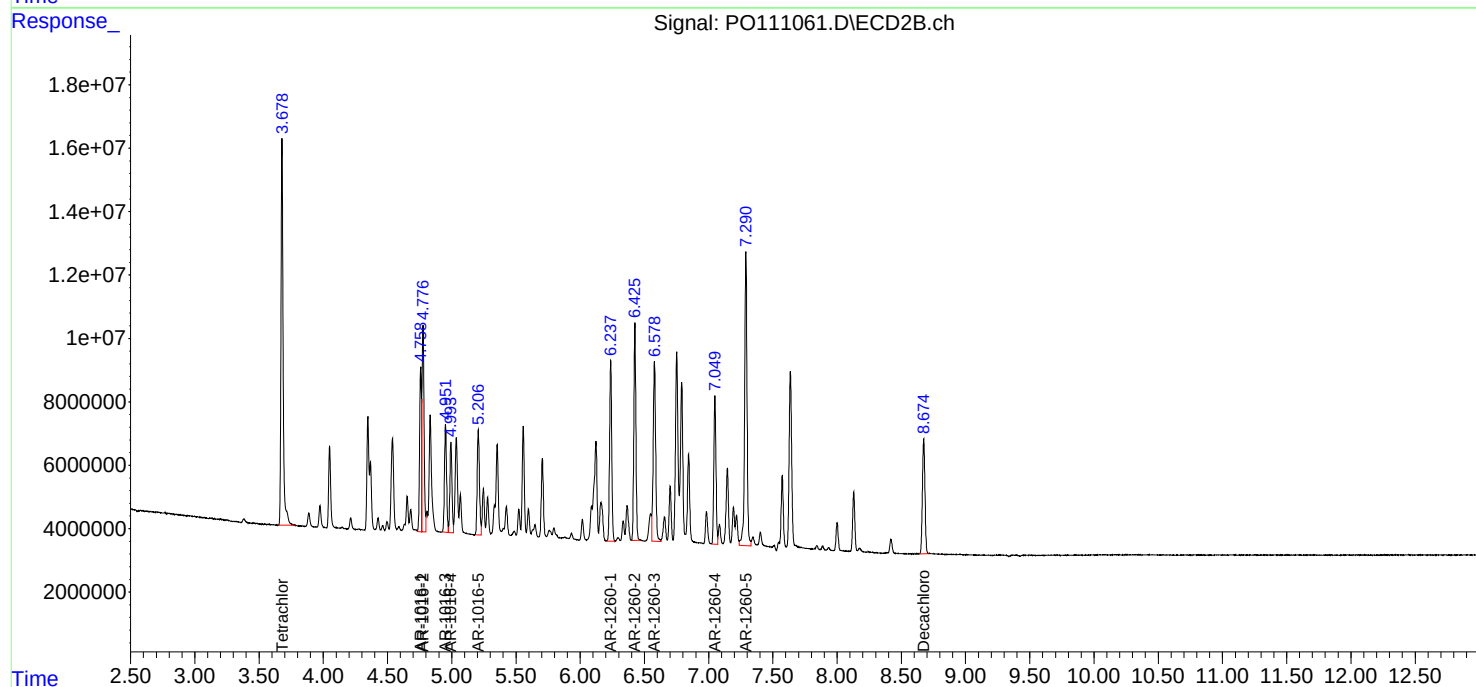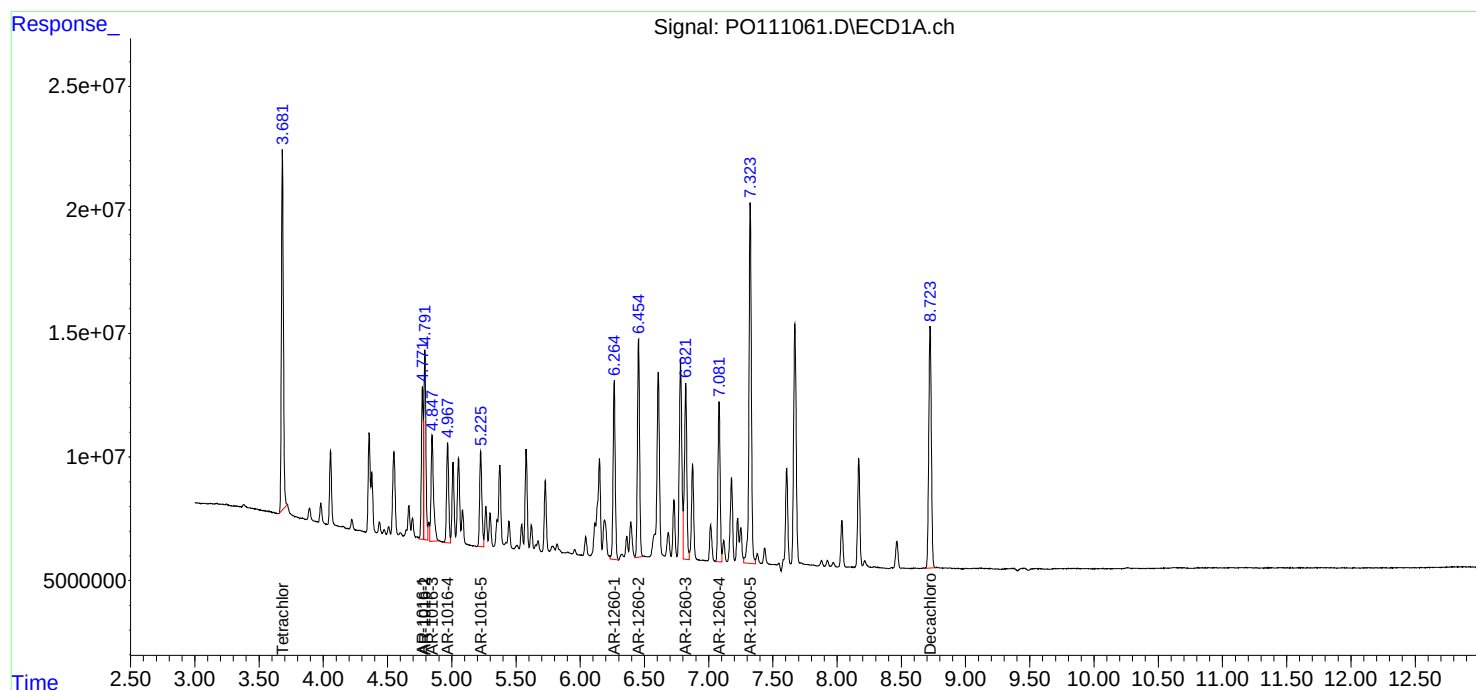

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 18:33
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/15/2025
 Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 18:42:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 14 18:42:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	28493753	25293030	4.843	4.640
2) SA Decachlor...	8.723	8.673	26671186	9559108	5.166	5.167
Target Compounds						
3) L1 AR-1016-1	4.773	4.758	11869714	10151367	52.741	53.169
4) L1 AR-1016-2	4.792	4.777	16448550	14199847	51.574	51.240
5) L1 AR-1016-3	4.849	4.953	11050750	7376412	50.896	50.497
6) L1 AR-1016-4	4.969	4.995	8879453	6427443	50.988	53.522
7) L1 AR-1016-5	5.226	5.207	8842201	8160776	50.242	52.855
31) L7 AR-1260-1	6.265	6.238	15795099	13309302	51.824m	53.261
32) L7 AR-1260-2	6.454	6.426	20091573	15455906	52.473m	52.520
33) L7 AR-1260-3	6.822	6.577	18486670	15856848	53.033	54.622m
34) L7 AR-1260-4	7.081	7.049	14607476	10534907	52.177	52.474
35) L7 AR-1260-5	7.324	7.290	36204522	23216663	50.291	50.514

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 18:33
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/15/2025
Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 18:42:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 14 18:42:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

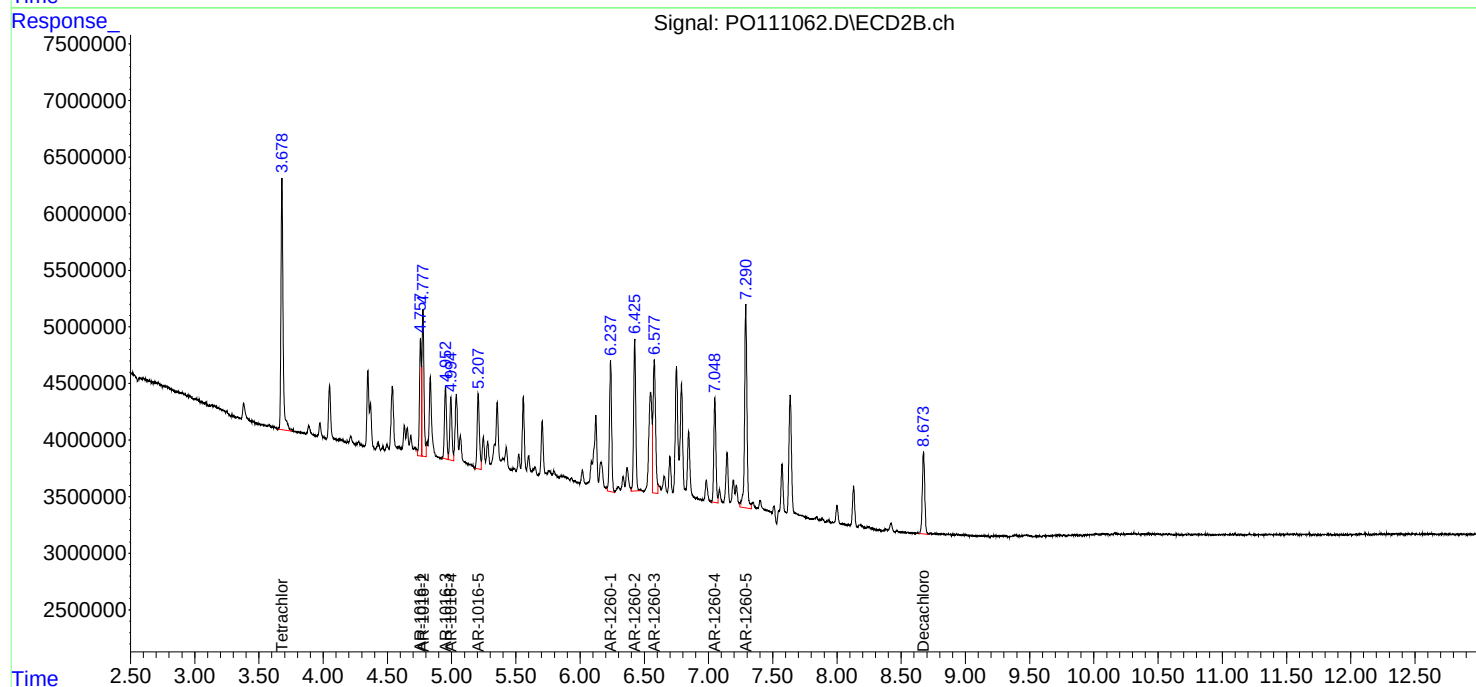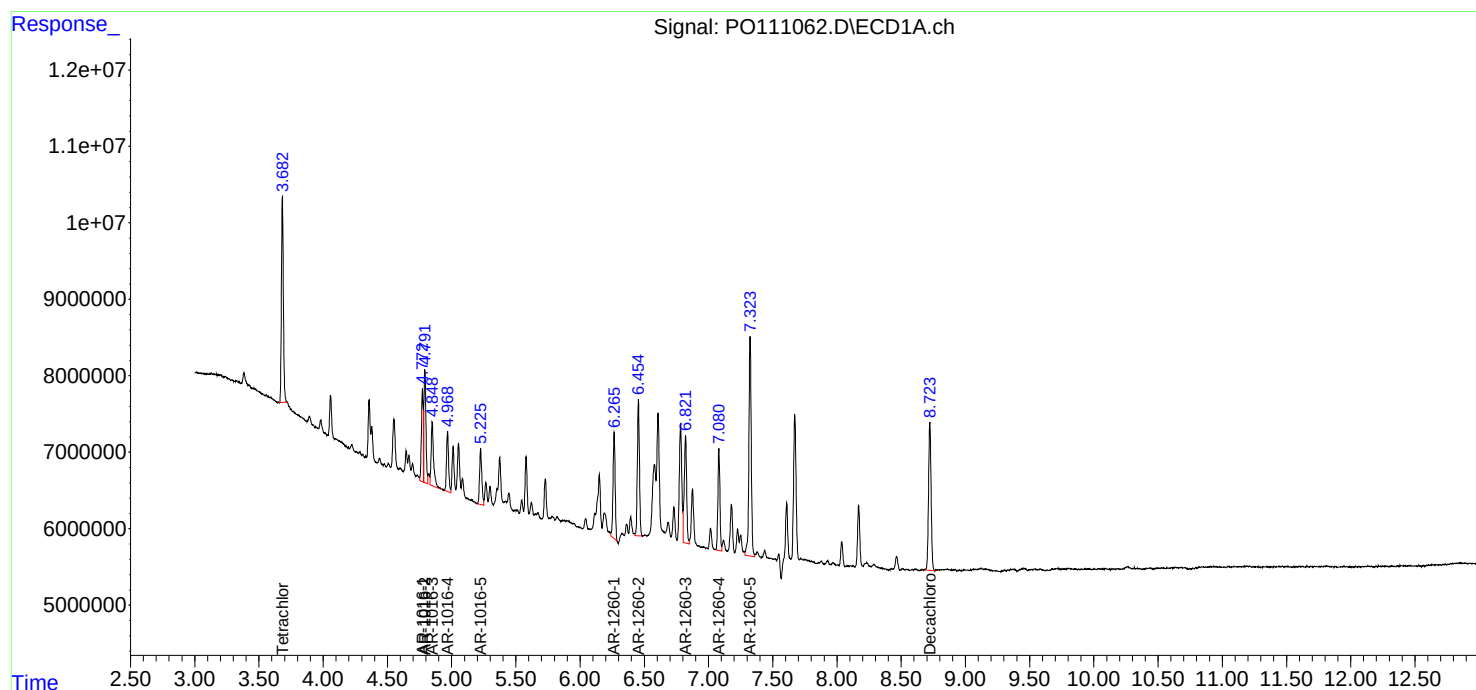

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 18:51
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 04:12:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 04:09:37 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	288.5E6	284.4E6	50.000	50.000
2) SA Decachlor...	8.724	8.674	258.5E6	91931505	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	3.895	3.890	43553173	36921483	500.000	500.000
9) L2 AR-1221-2	3.981	3.975	31851907	27207063	500.000	500.000
10) L2 AR-1221-3	4.057	4.050	96163744	83550323	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 18:51
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 04:12:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 04:09:37 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

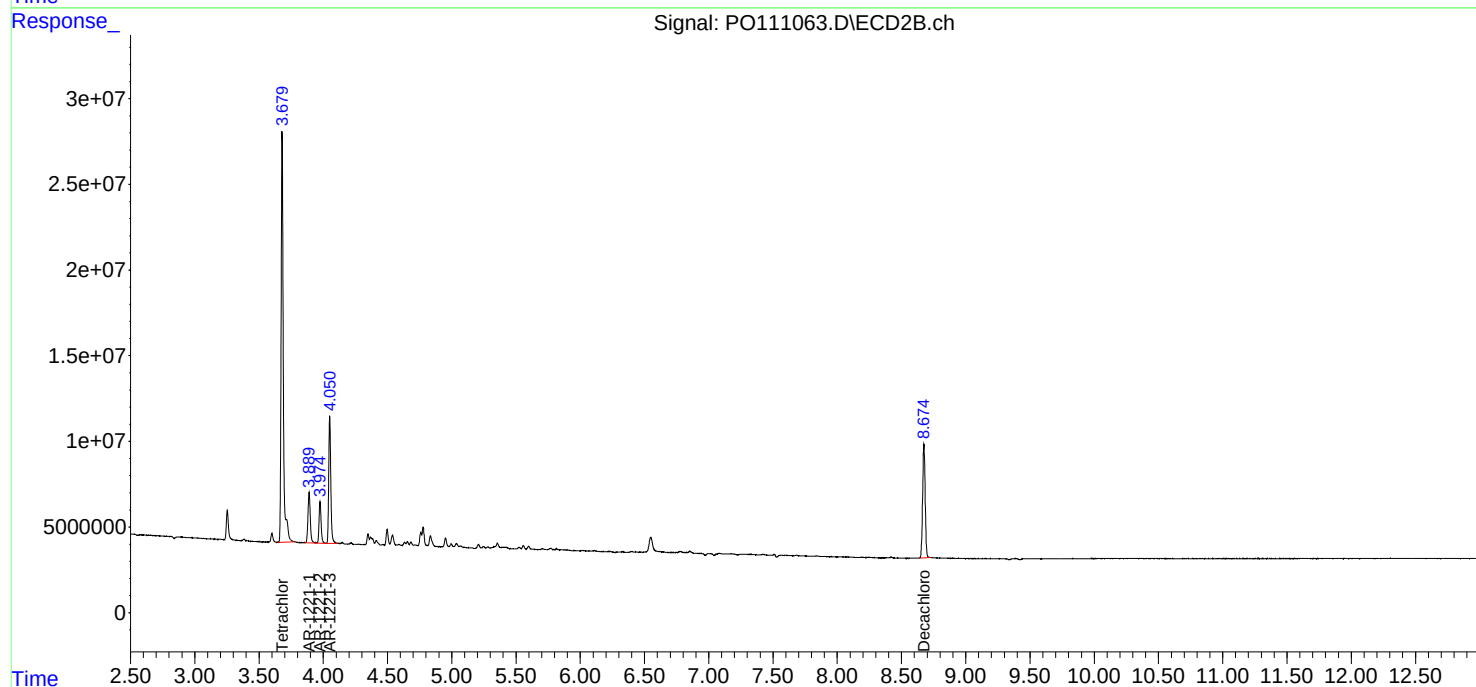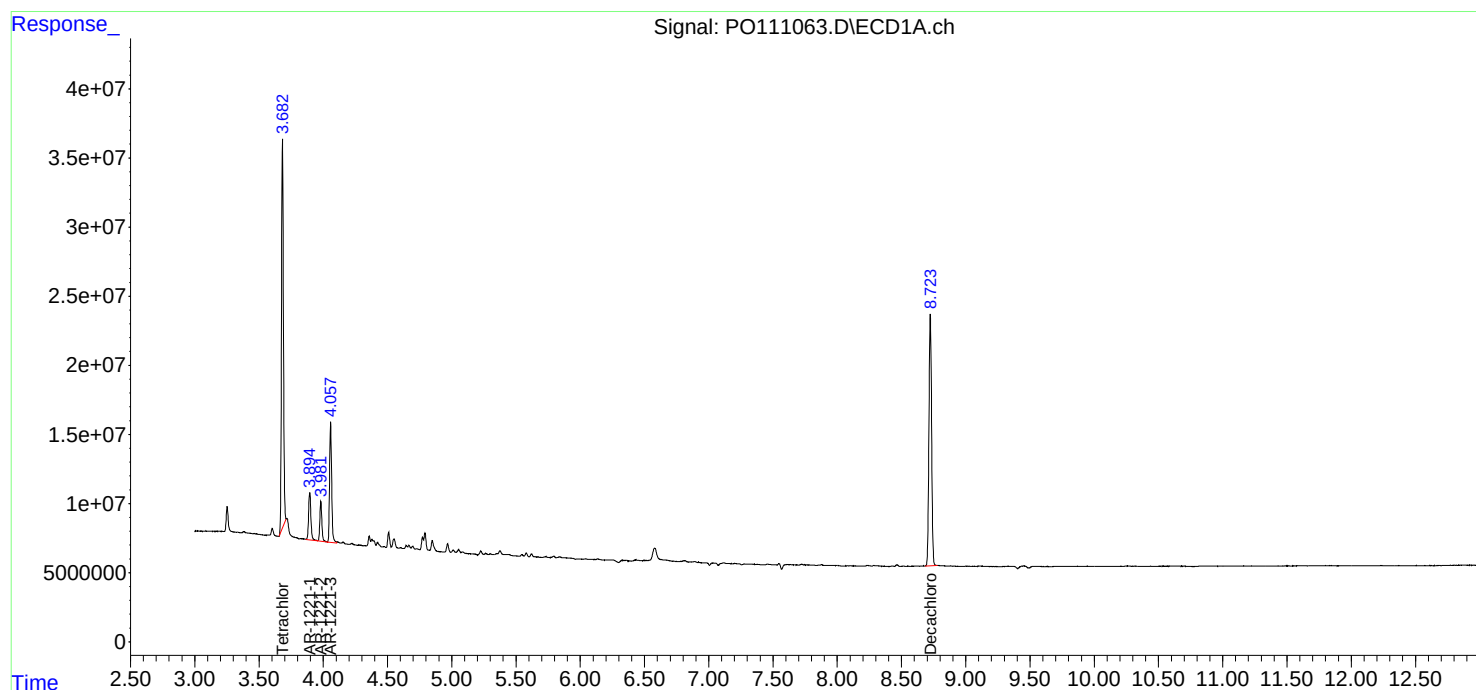

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 19:10
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 04:17:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 04:17:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	289.7E6	276.3E6	50.000	50.000
2) SA Decachlor...	8.724	8.675	254.0E6	89356624	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.057	4.050	76586849	65297499	500.000	500.000
12) L3 AR-1232-2	4.551	4.777	40973235	65580176	500.000	500.000
13) L3 AR-1232-3	4.792	4.952	76463454	34035848	500.000	500.000
14) L3 AR-1232-4	4.968	5.037	41125705	30838173	500.000	500.000
15) L3 AR-1232-5	5.012	5.207	27129649	32866275	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 19:10
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 04:17:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 04:17:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

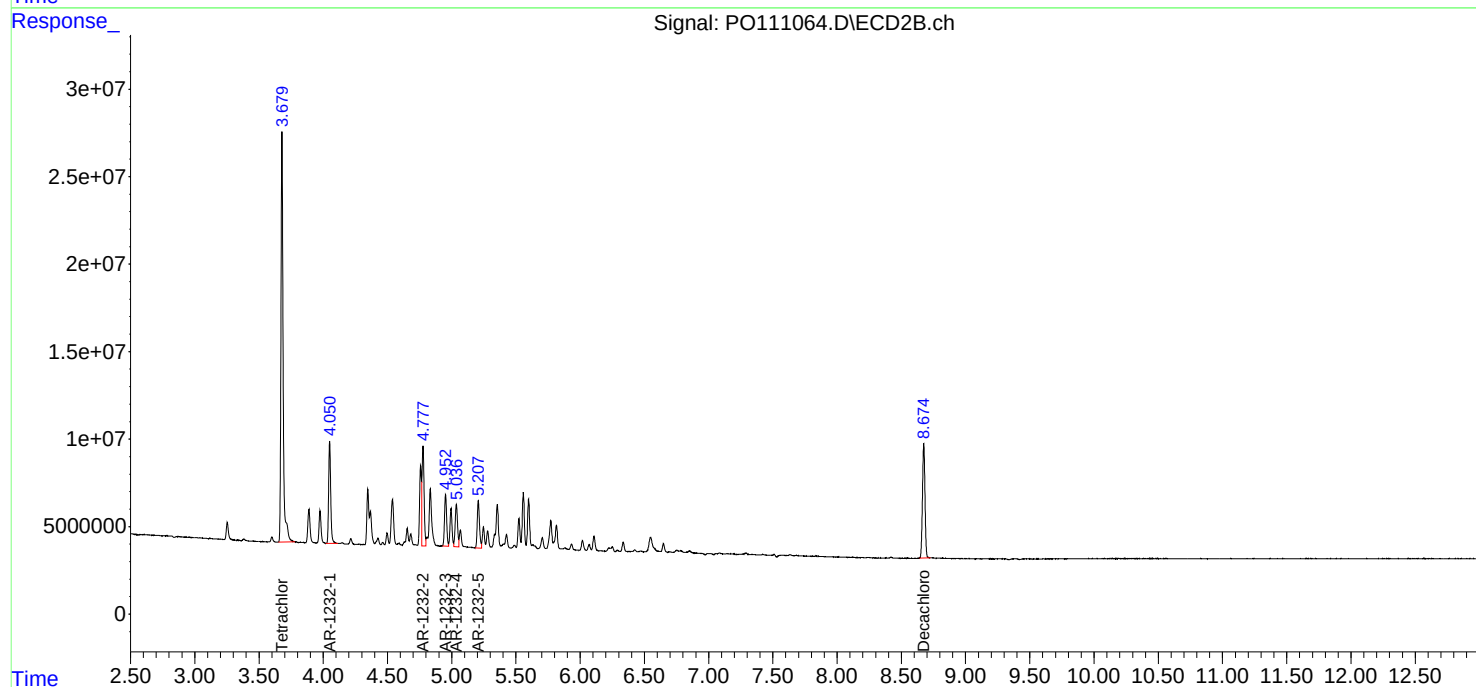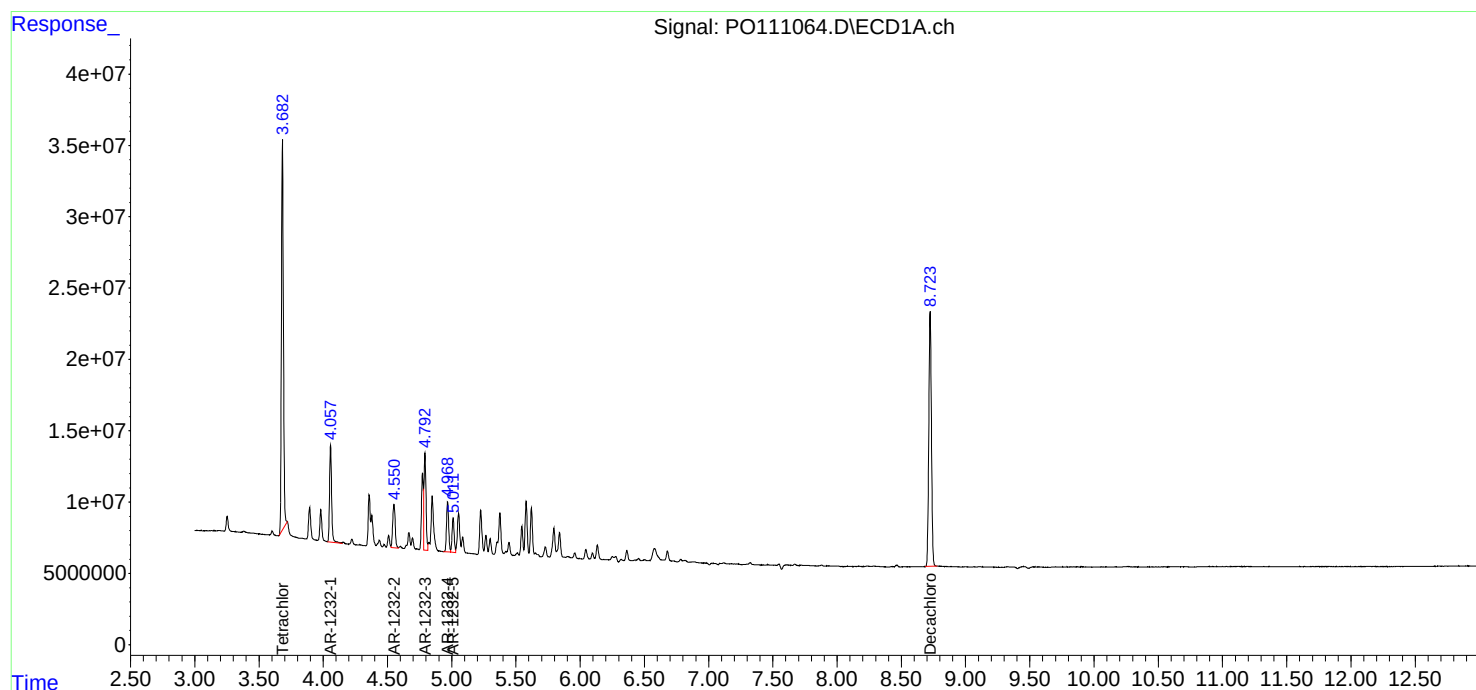

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 19:28
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 04:23:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 04:23:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.679	568.1E6	539.6E6	94.045	96.291
2) SA Decachlor...	8.724	8.673	477.4E6	165.0E6	91.361	91.314
Target Compounds						
16) L4 AR-1242-1	4.772	4.758	176.7E6	150.8E6	899.610	912.362
17) L4 AR-1242-2	4.791	4.777	257.7E6	223.6E6	922.296	929.388
18) L4 AR-1242-3	4.848	4.952	175.2E6	118.1E6	909.545	921.917
19) L4 AR-1242-4	4.967	5.036	140.2E6	114.7E6	915.805	903.330
20) L4 AR-1242-5	5.620	5.557	145.2E6	142.4E6	911.278	915.668



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 19:28
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 04:23:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 04:23:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

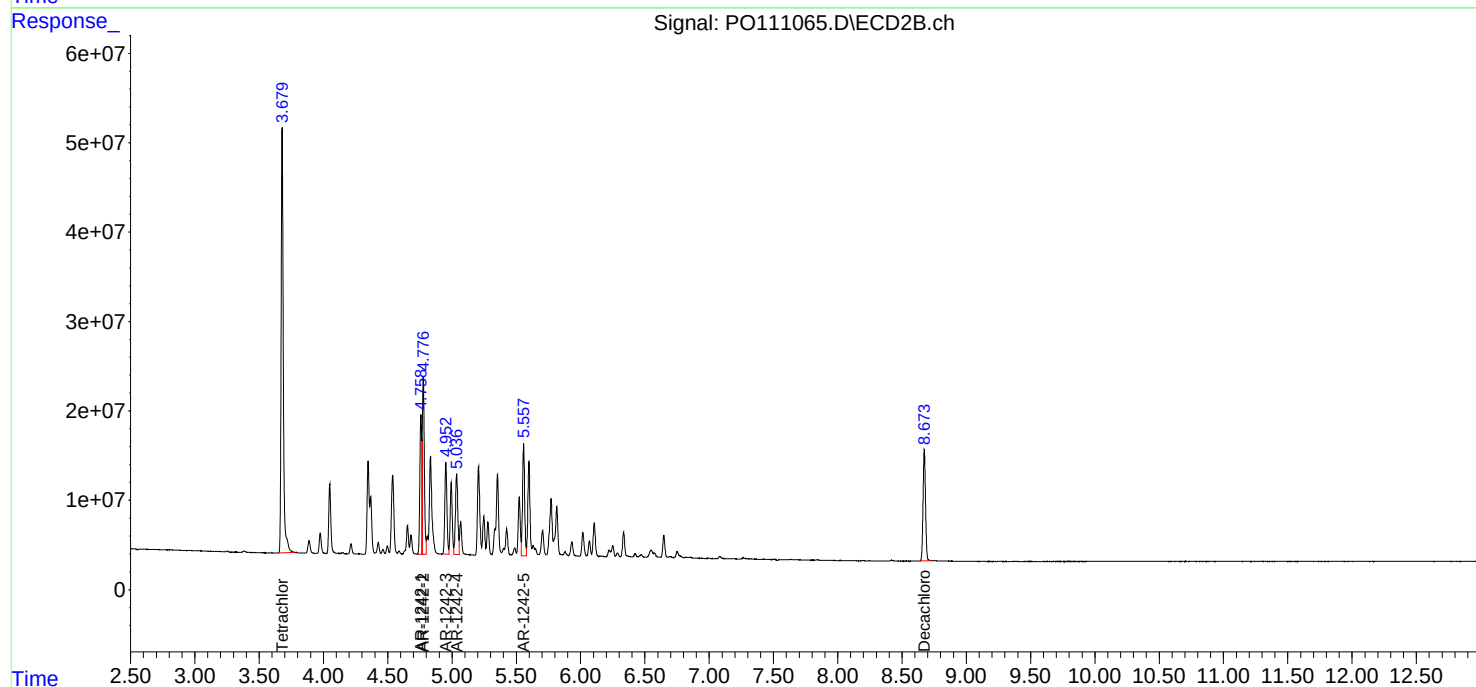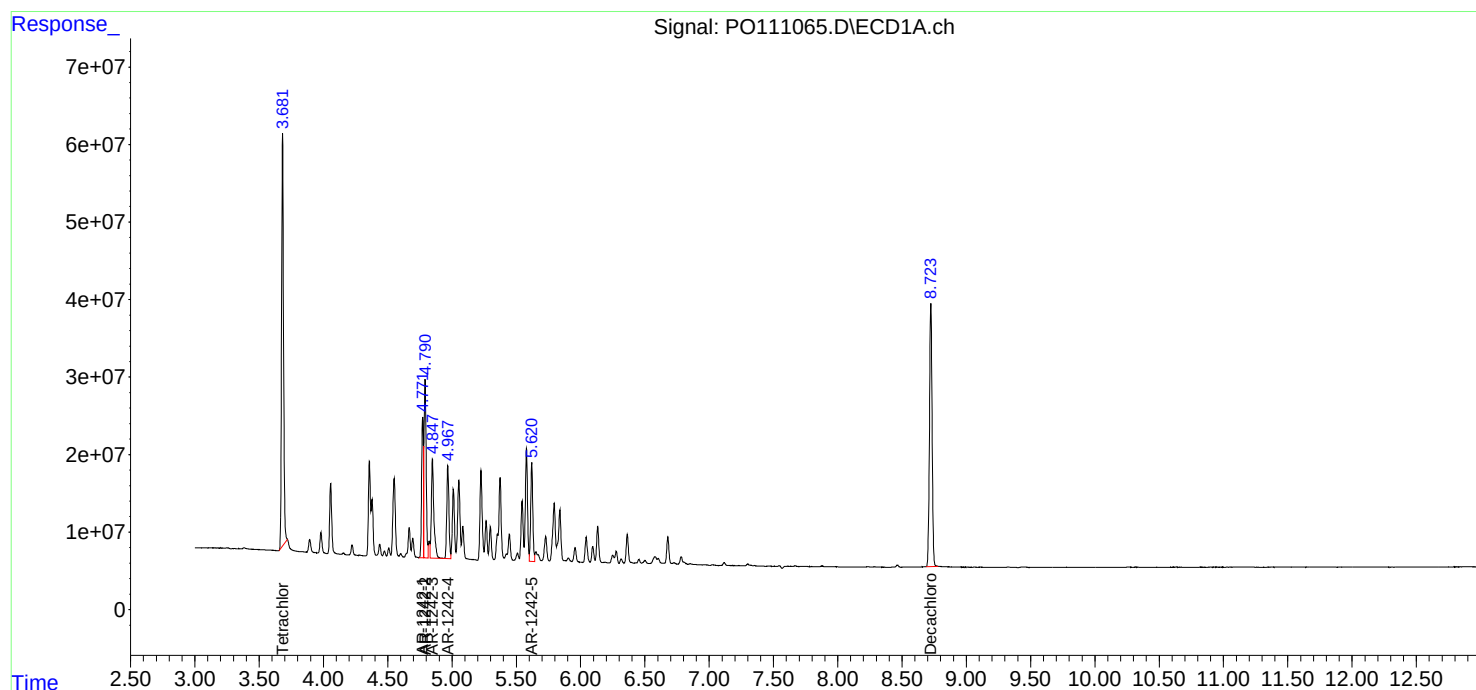

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 19:46
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 04:24:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 04:23:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	437.4E6	412.8E6	72.404	73.670
2) SA Decachlor...	8.724	8.674	373.9E6	129.9E6	71.548	71.922
Target Compounds						
16) L4 AR-1242-1	4.773	4.759	139.3E6	118.0E6	709.065	713.923
17) L4 AR-1242-2	4.792	4.777	200.8E6	173.8E6	718.638	722.178
18) L4 AR-1242-3	4.849	4.953	137.2E6	91784303	712.284	716.498
19) L4 AR-1242-4	4.969	5.037	109.7E6	89988997	716.656	708.565
20) L4 AR-1242-5	5.622	5.558	114.0E6	111.2E6	715.639	714.896



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 19:46
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 04:24:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 04:23:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

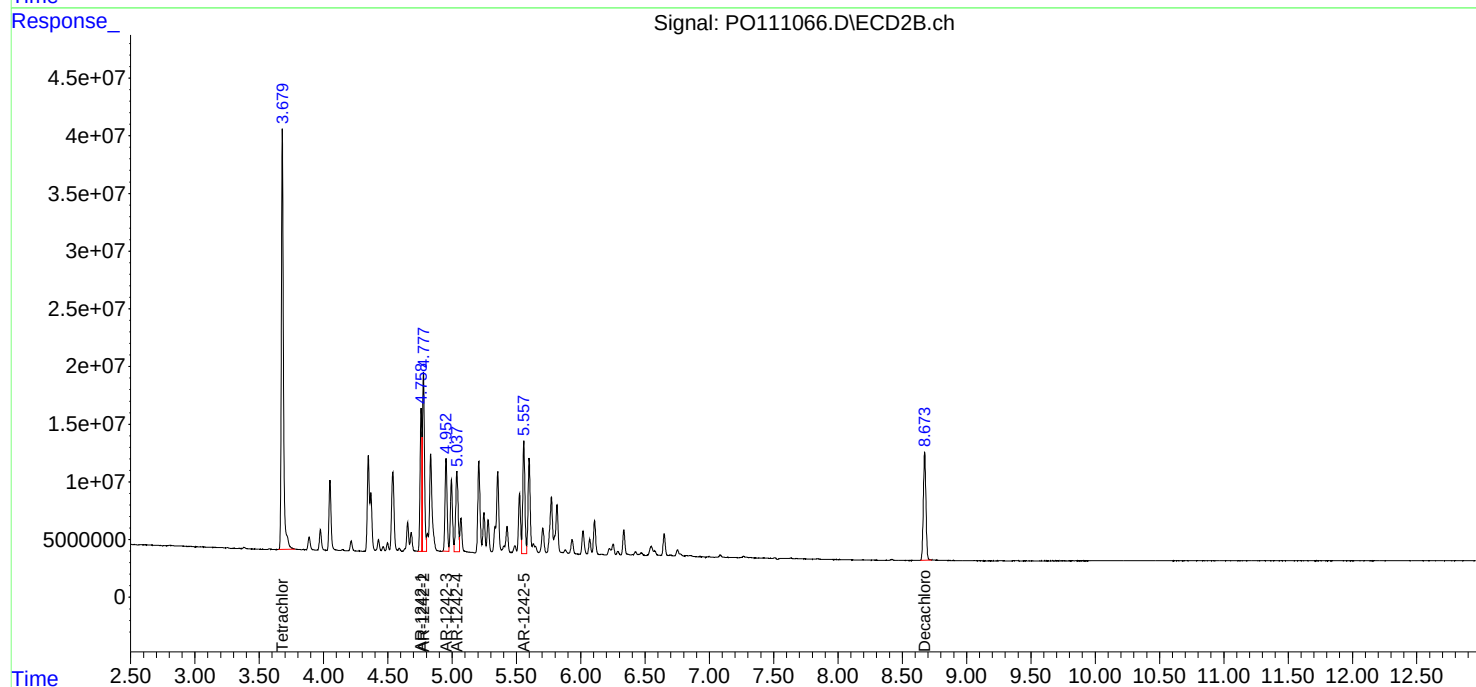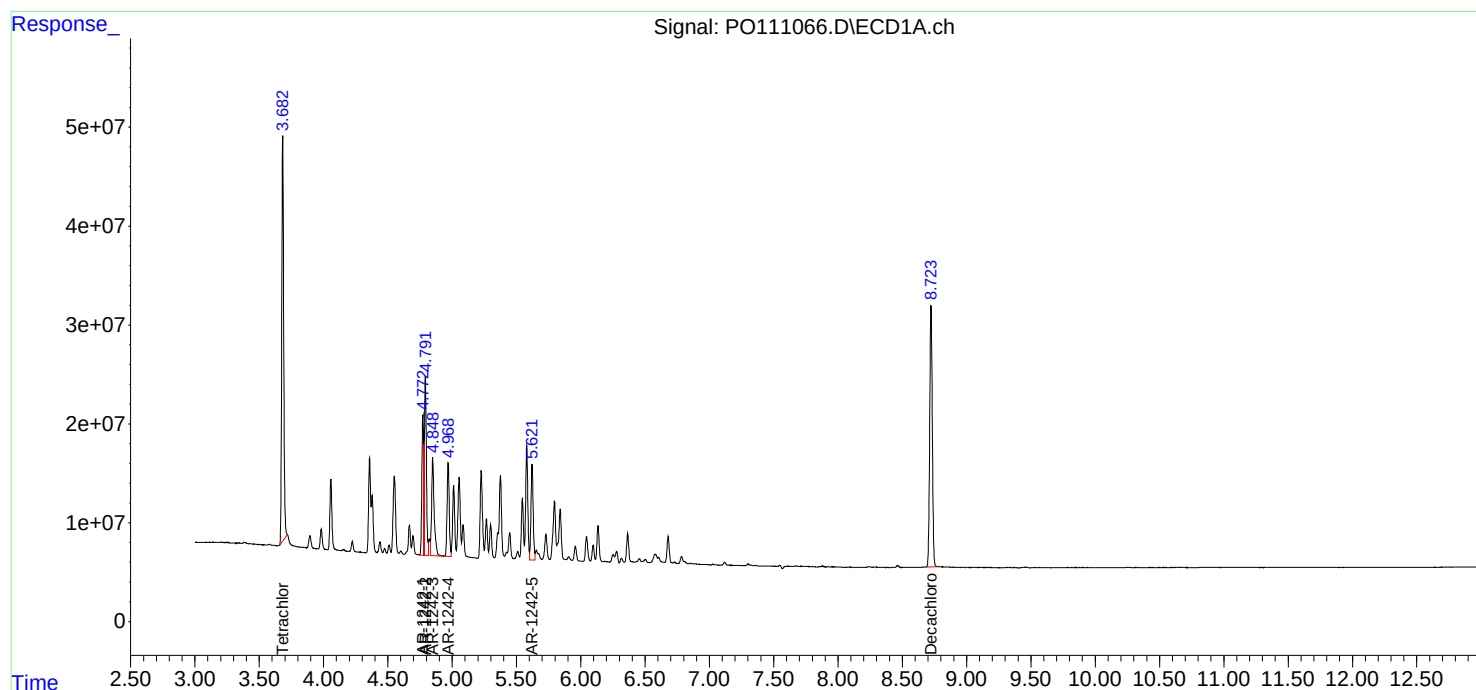

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 20:05
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 04:24:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 04:23:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	302.0E6	280.2E6	50.000	50.000
2) SA Decachlor...	8.725	8.674	261.3E6	90333720	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	4.773	4.759	98208092	82620556	500.000	500.000
17) L4 AR-1242-2	4.792	4.778	139.7E6	120.3E6	500.000	500.000
18) L4 AR-1242-3	4.848	4.953	96305021	64050605	500.000	500.000
19) L4 AR-1242-4	4.969	5.037	76546823	63500917	500.000	500.000
20) L4 AR-1242-5	5.621	5.558	79660759	77752665	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 20:05
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 04:24:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 04:23:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

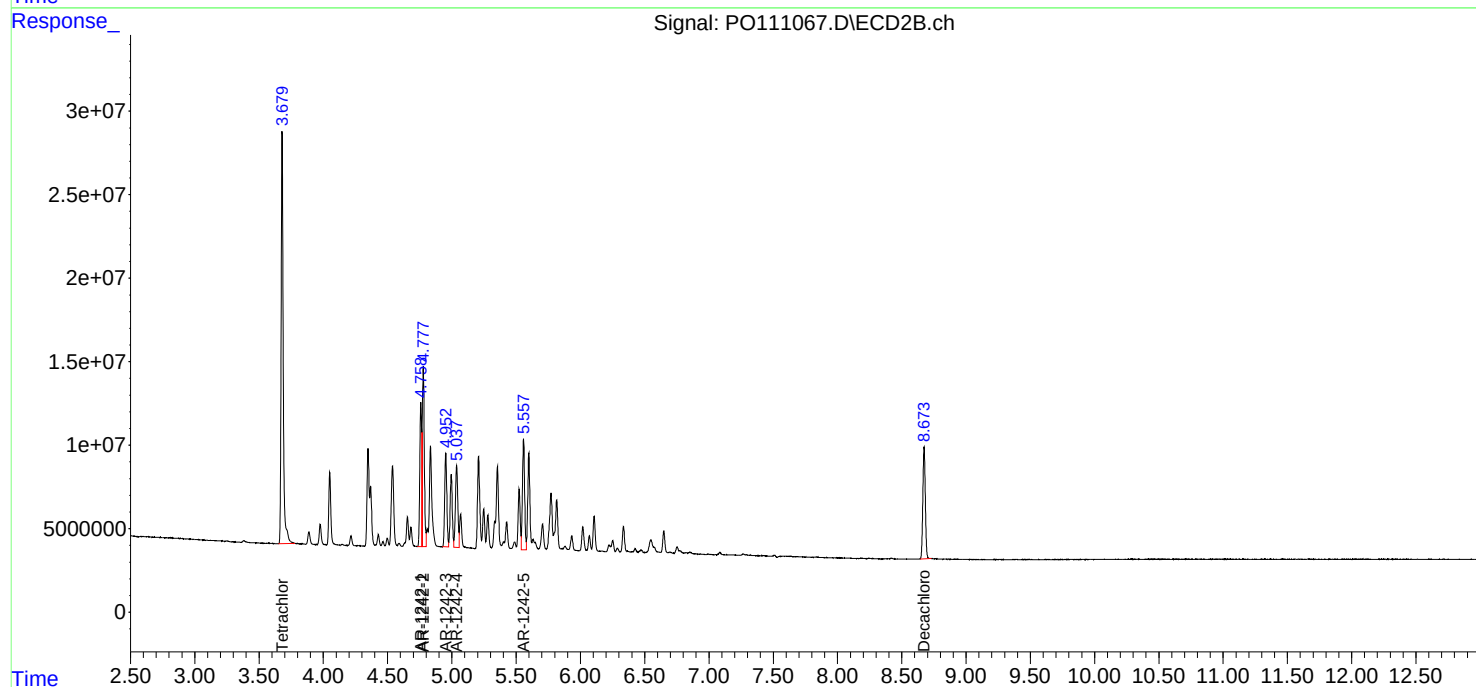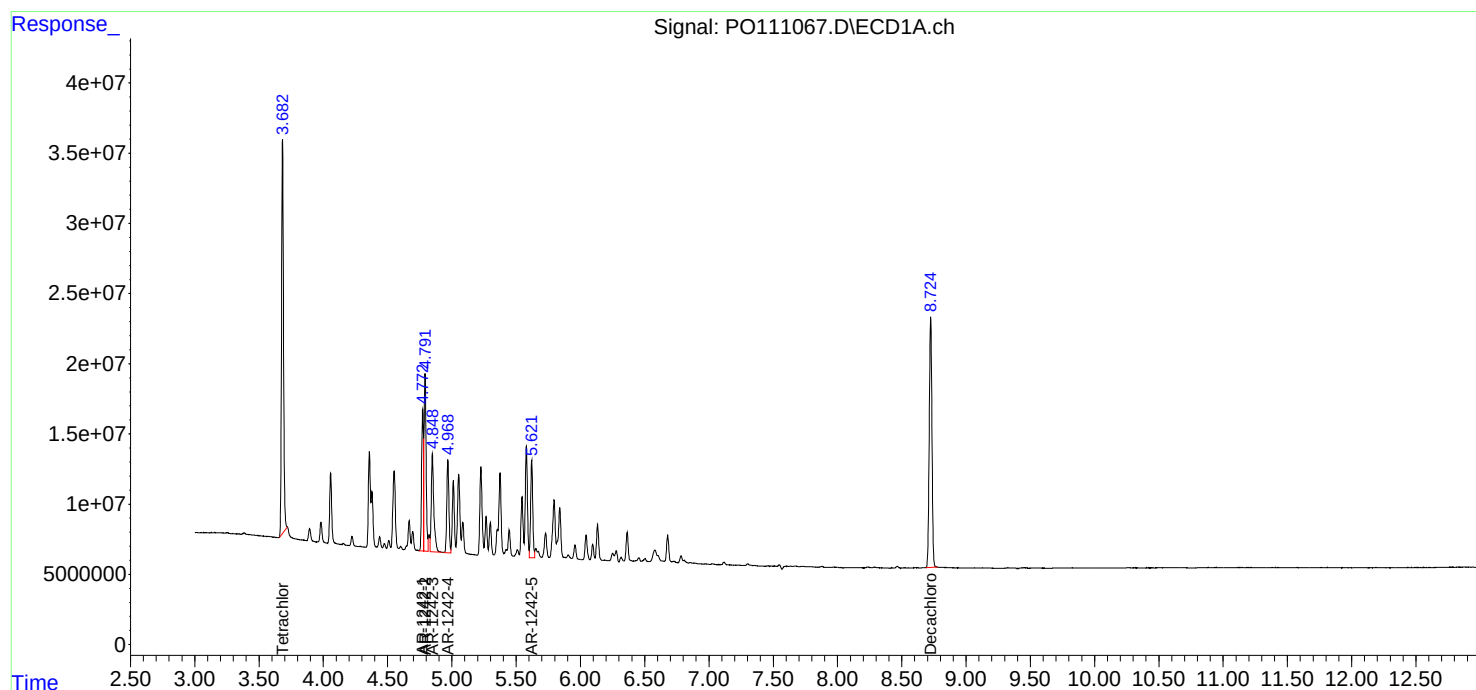

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 20:23
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 04:24:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 04:23:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.679	154.4E6	140.2E6	25.554	25.013
2) SA Decachlor...	8.724	8.674	136.9E6	48326476	26.201	26.749
Target Compounds						
16) L4 AR-1242-1	4.773	4.758	51769854	43243631	263.572	261.700
17) L4 AR-1242-2	4.791	4.777	73286157	62610273	262.267	260.212
18) L4 AR-1242-3	4.848	4.952	50308175	33361673	261.192	260.432
19) L4 AR-1242-4	4.968	5.037	39985868	33506849	261.186	263.830
20) L4 AR-1242-5	5.620	5.557	42256879	40819456	265.230	262.496



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 20:23
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 04:24:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 04:23:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

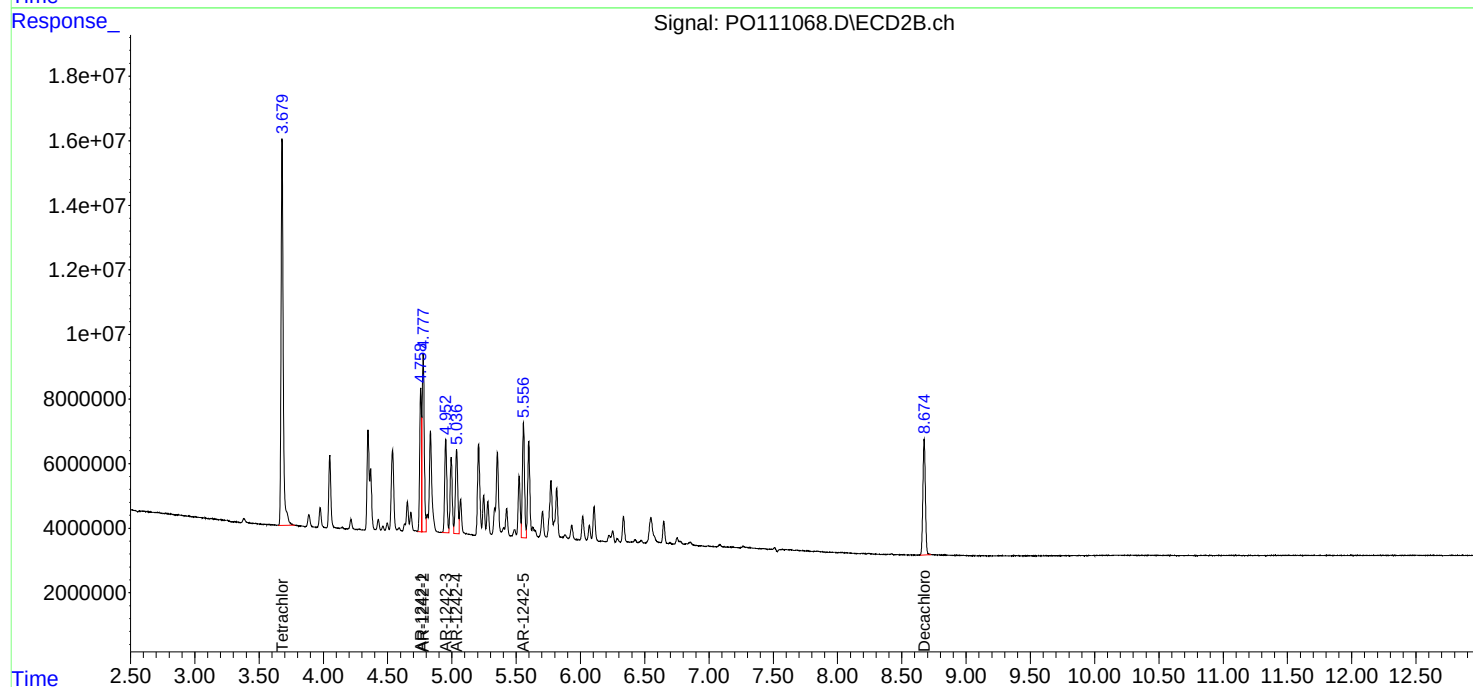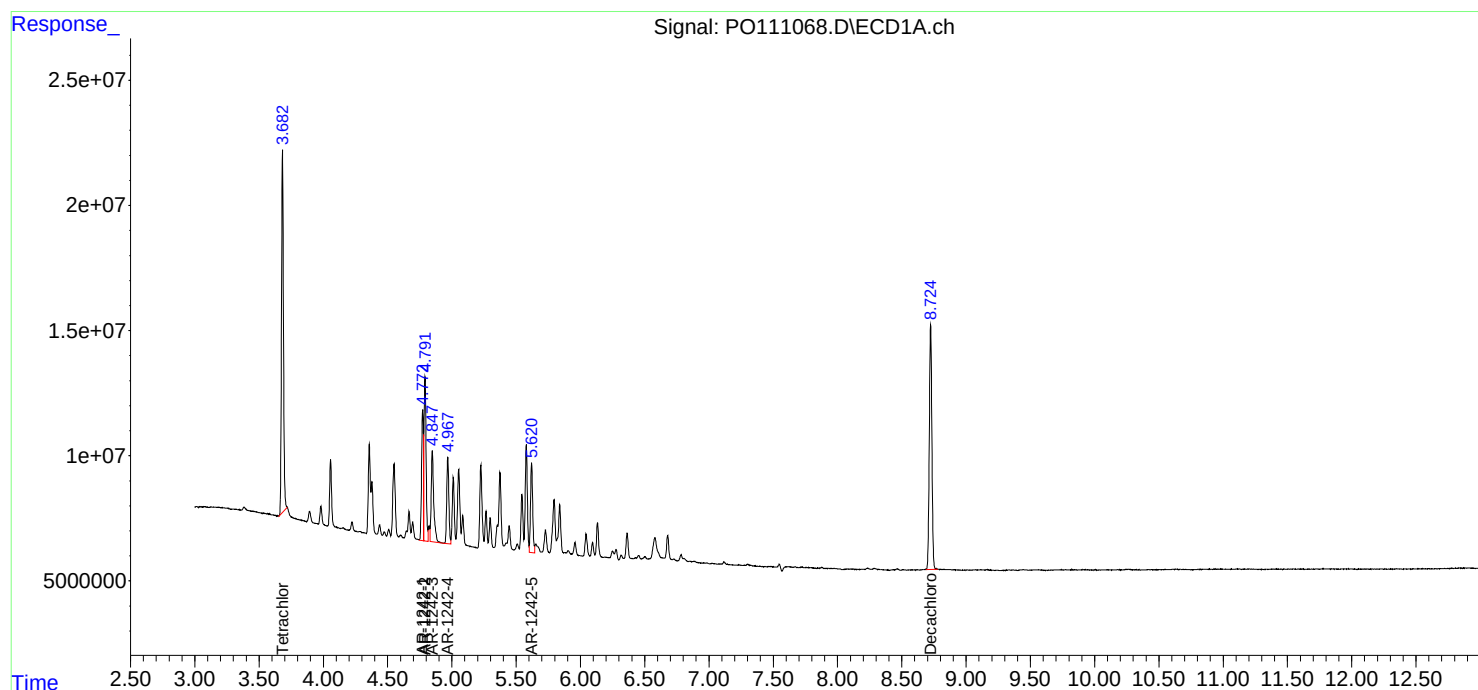

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 20:41
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 04:25:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 04:23:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.678	26744020	23641793	4.427	4.219
2) SA Decachlor...	8.723	8.672	25067542	8857274	4.797	4.903
Target Compounds						
16) L4 AR-1242-1	4.772	4.758	9505477	7963295	48.395	48.192
17) L4 AR-1242-2	4.791	4.776	13101291	11333445	46.885	47.103
18) L4 AR-1242-3	4.848	4.951	8899007	5803384	46.202	45.303
19) L4 AR-1242-4	4.968	5.036	6973643	6116856	45.551	48.164
20) L4 AR-1242-5	5.621	5.556	7607608	7526607	47.750	48.401



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 20:41
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 04:25:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 04:23:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

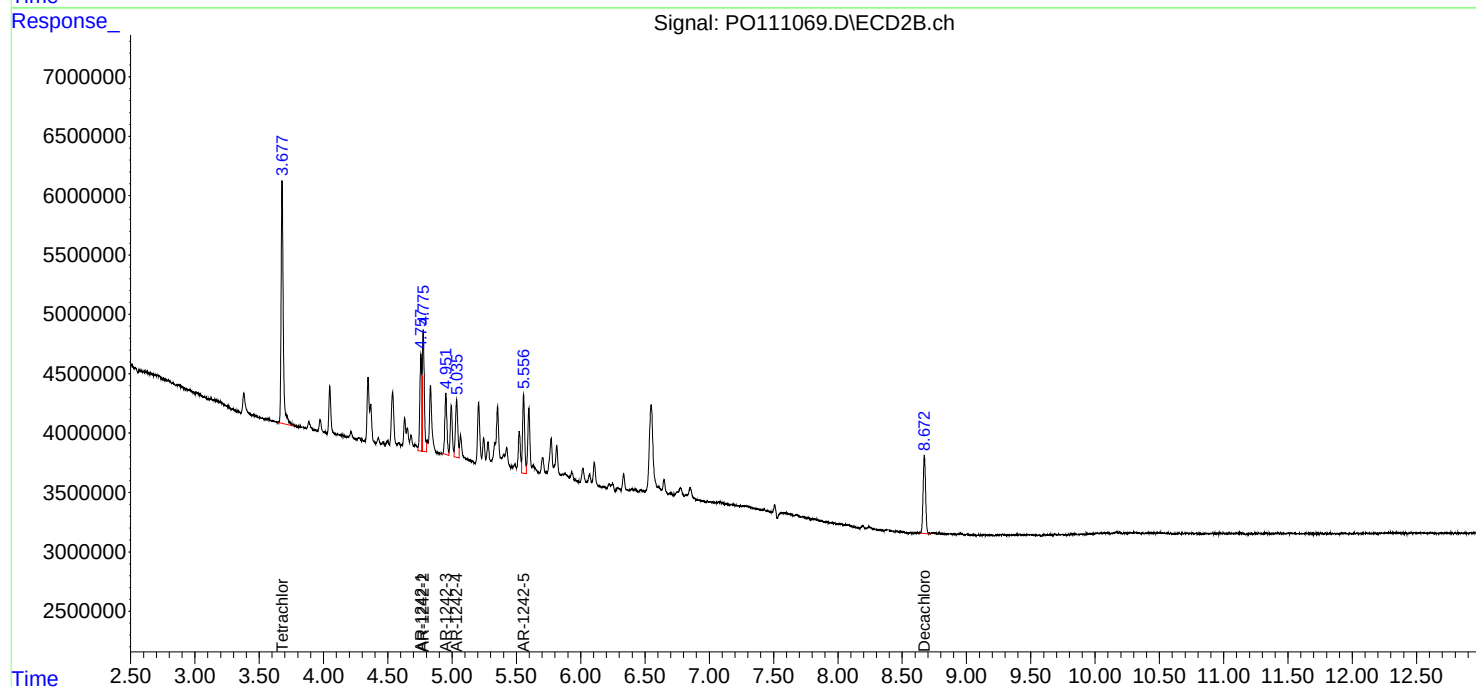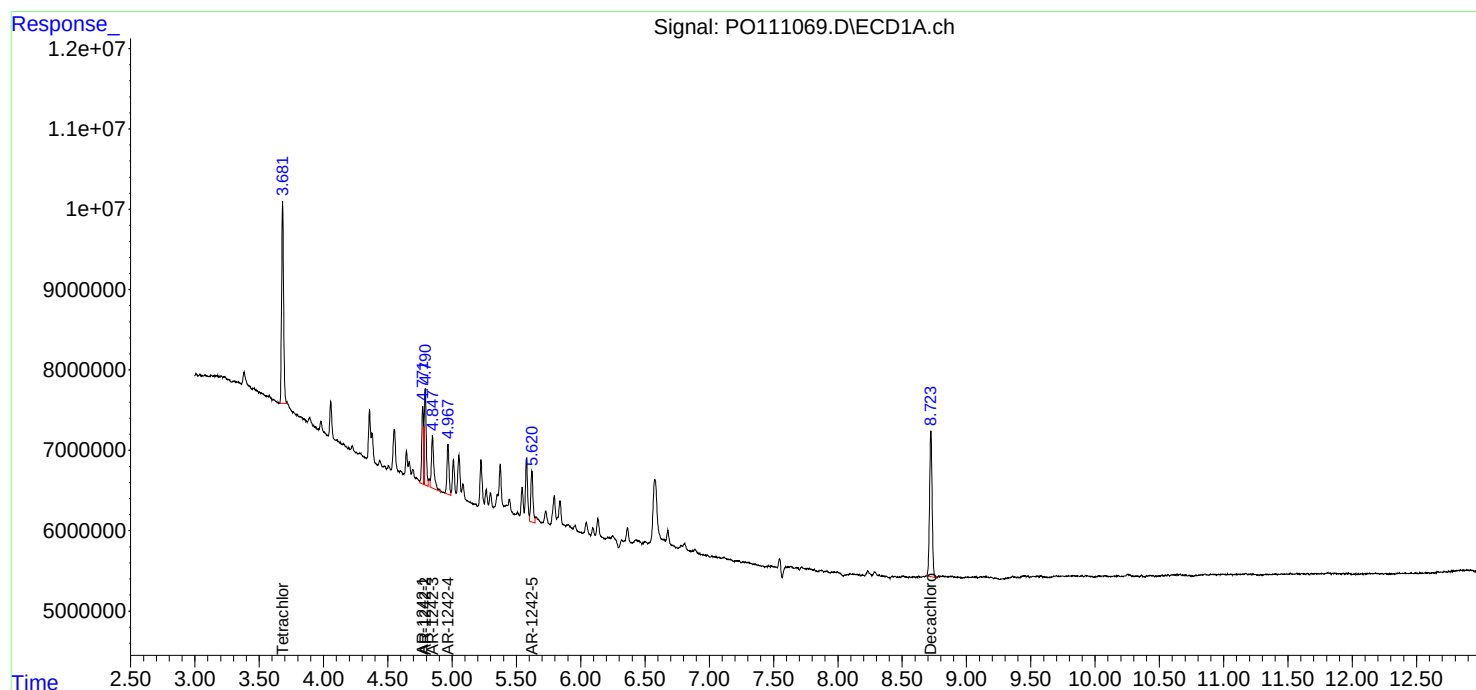

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 21:00
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:27:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:26:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	586.5E6	539.2E6	94.448	96.685
2) SA Decachlor...	8.723	8.674	486.2E6	167.6E6	92.112	88.448
Target Compounds						
21) L5 AR-1248-1	4.774	4.759	138.2E6	116.7E6	902.613	906.468
22) L5 AR-1248-2	5.012	4.995	182.8E6	159.8E6	909.133	912.206
23) L5 AR-1248-3	5.226	5.037	227.5E6	169.7E6	906.281	914.012
24) L5 AR-1248-4	5.580	5.208	324.8E6	198.9E6	911.584	916.809
25) L5 AR-1248-5	5.622	5.599	233.9E6	198.3E6	908.812	921.655



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 21:00
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:27:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:26:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

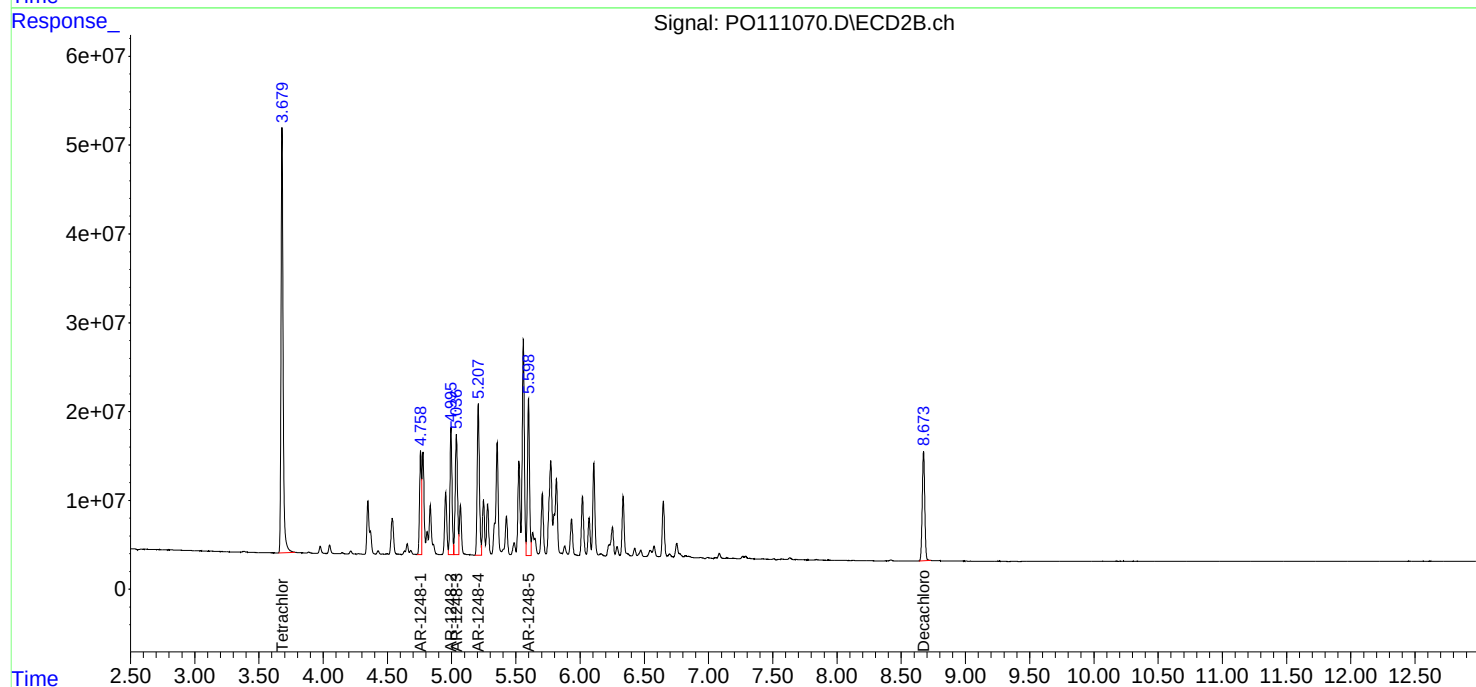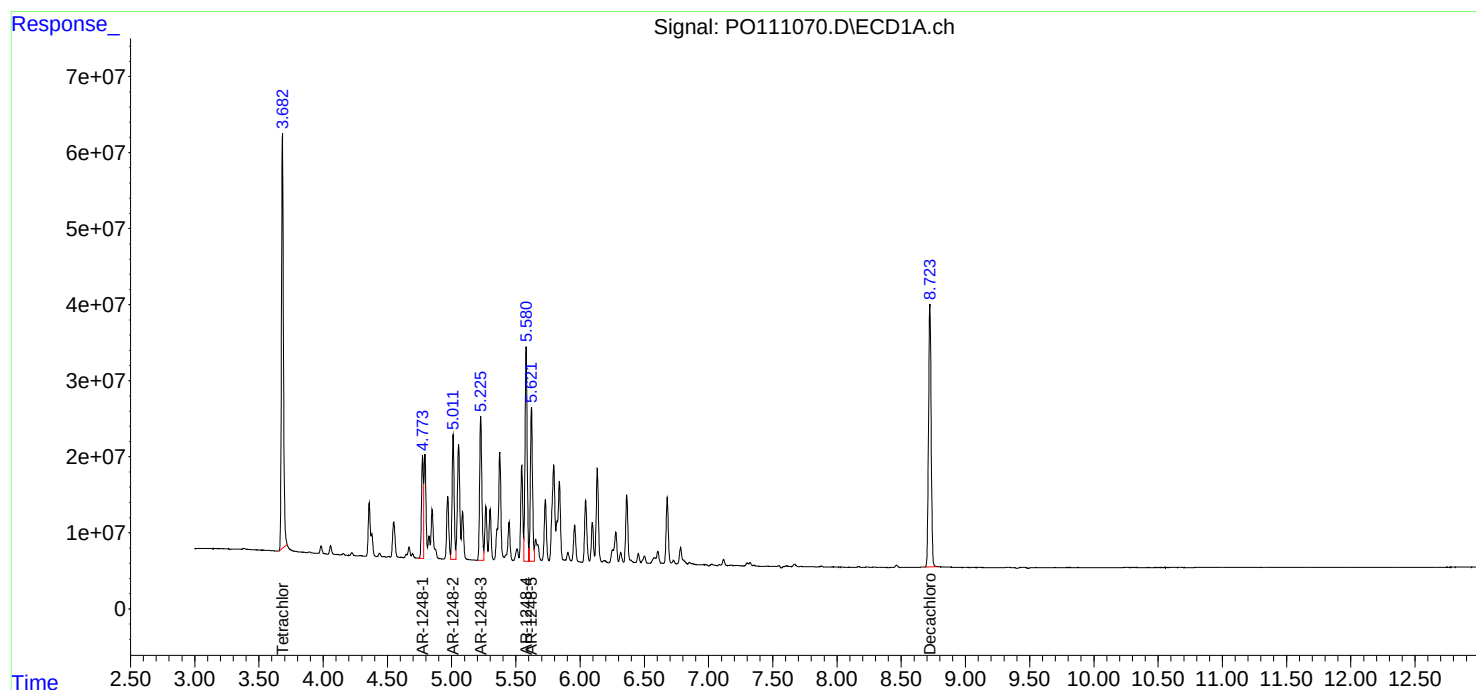

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 21:18
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:27:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:26:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	453.4E6	412.4E6	73.021	73.953
2) SA Decachlor...	8.724	8.674	377.4E6	130.5E6	71.496	68.877
Target Compounds						
21) L5 AR-1248-1	4.772	4.758	109.5E6	91783465	715.078	713.065
22) L5 AR-1248-2	5.011	4.995	142.8E6	124.9E6	710.350	713.297
23) L5 AR-1248-3	5.225	5.037	178.7E6	132.5E6	712.085	713.766
24) L5 AR-1248-4	5.580	5.207	252.6E6	154.8E6	709.005	713.546
25) L5 AR-1248-5	5.621	5.598	182.5E6	154.4E6	708.810	717.562



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 21:18
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:27:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:26:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

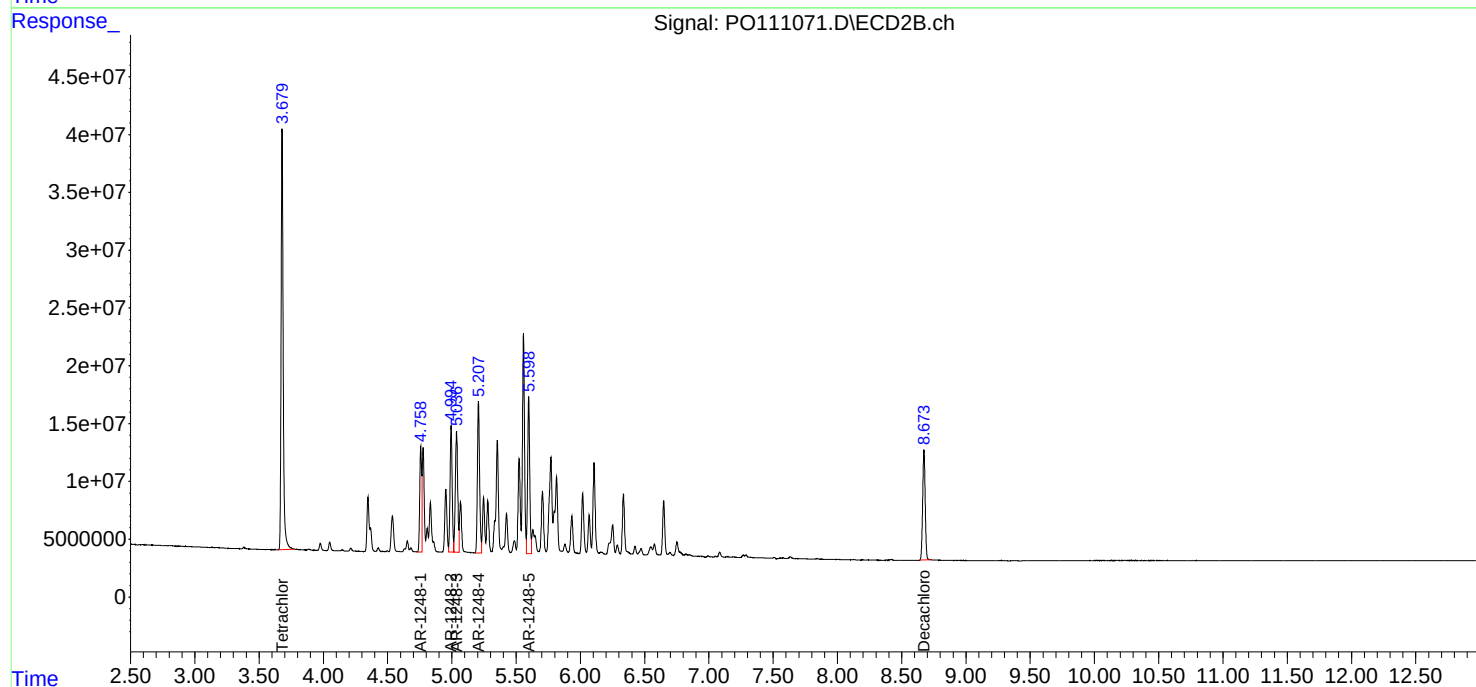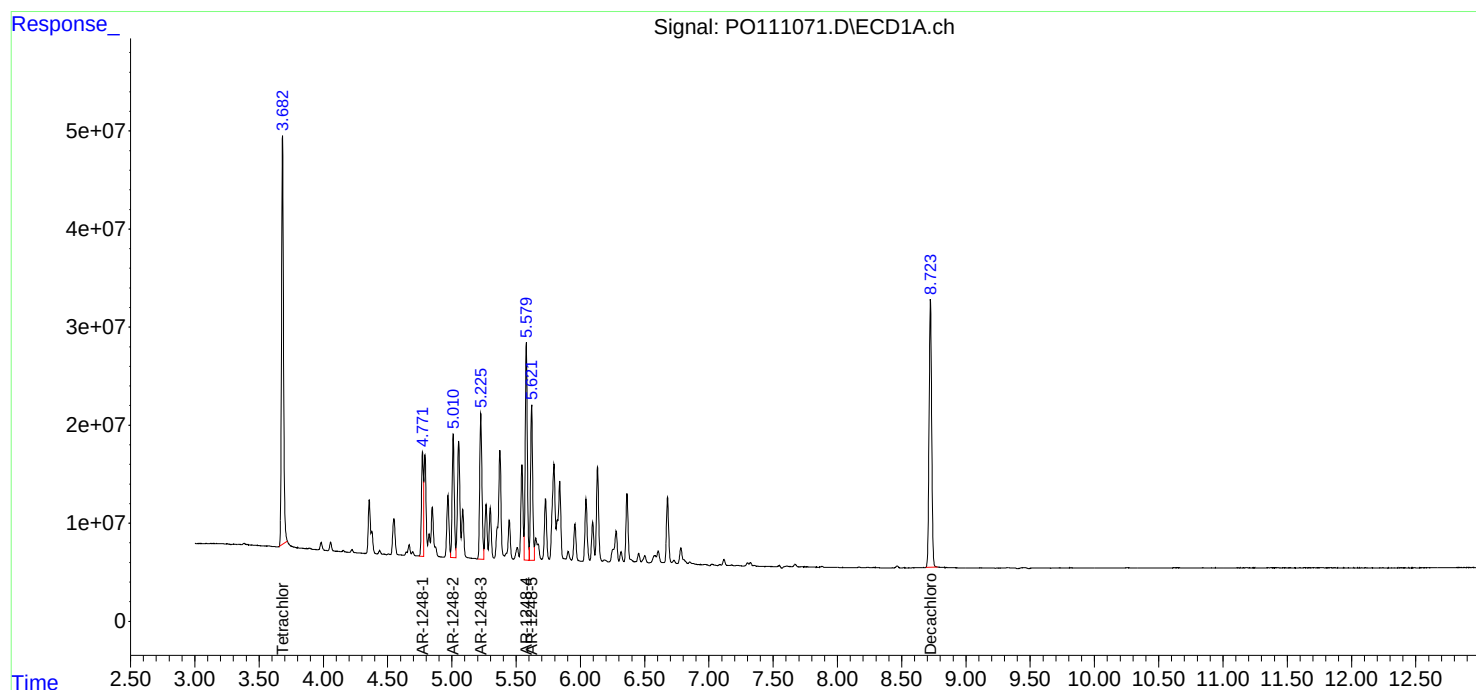

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 21:37
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:27:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:26:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	310.5E6	278.9E6	50.000	50.000
2) SA Decachlor...	8.724	8.675	263.9E6	94731575	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	4.772	4.758	76534733	64358378	500.000	500.000
22) L5 AR-1248-2	5.011	4.995	100.5E6	87581471	500.000	500.000
23) L5 AR-1248-3	5.226	5.037	125.5E6	92824803	500.000	500.000
24) L5 AR-1248-4	5.580	5.207	178.1E6	108.5E6	500.000	500.000
25) L5 AR-1248-5	5.621	5.599	128.7E6	107.6E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 21:37
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:27:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:26:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

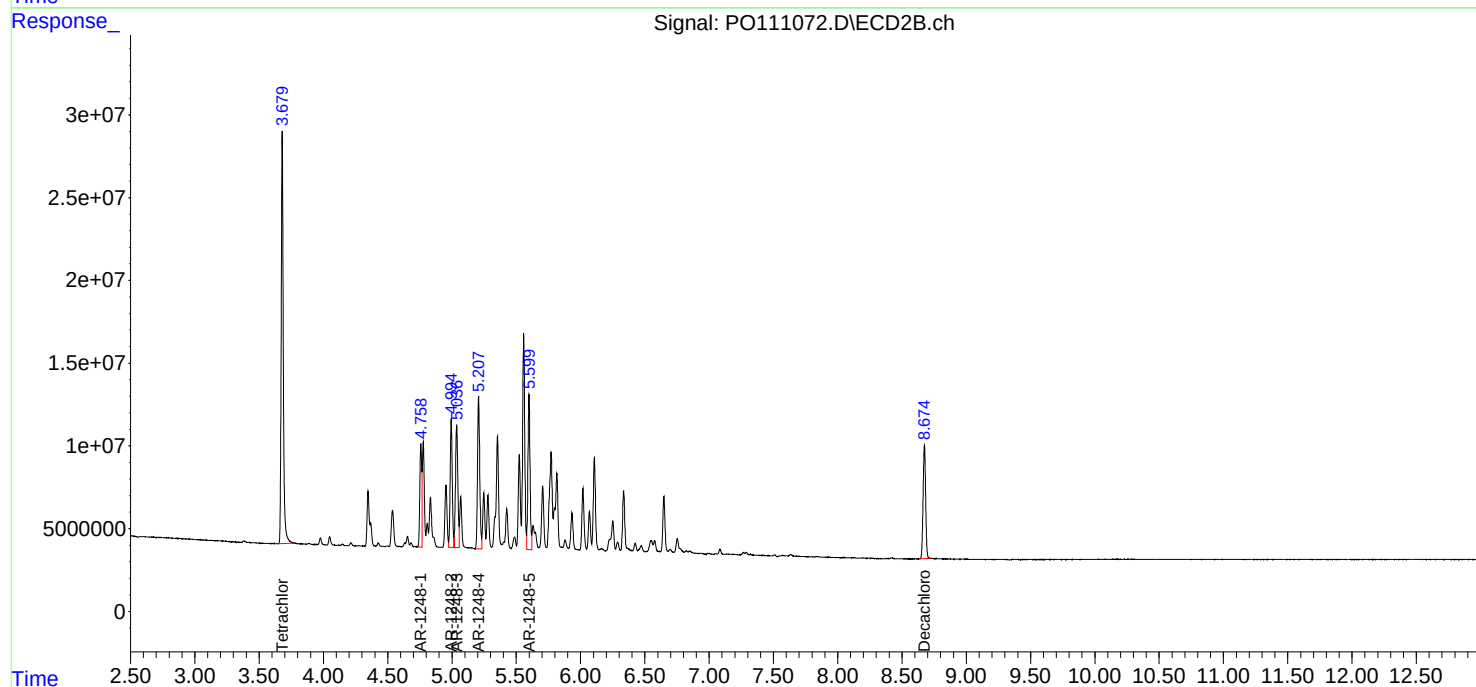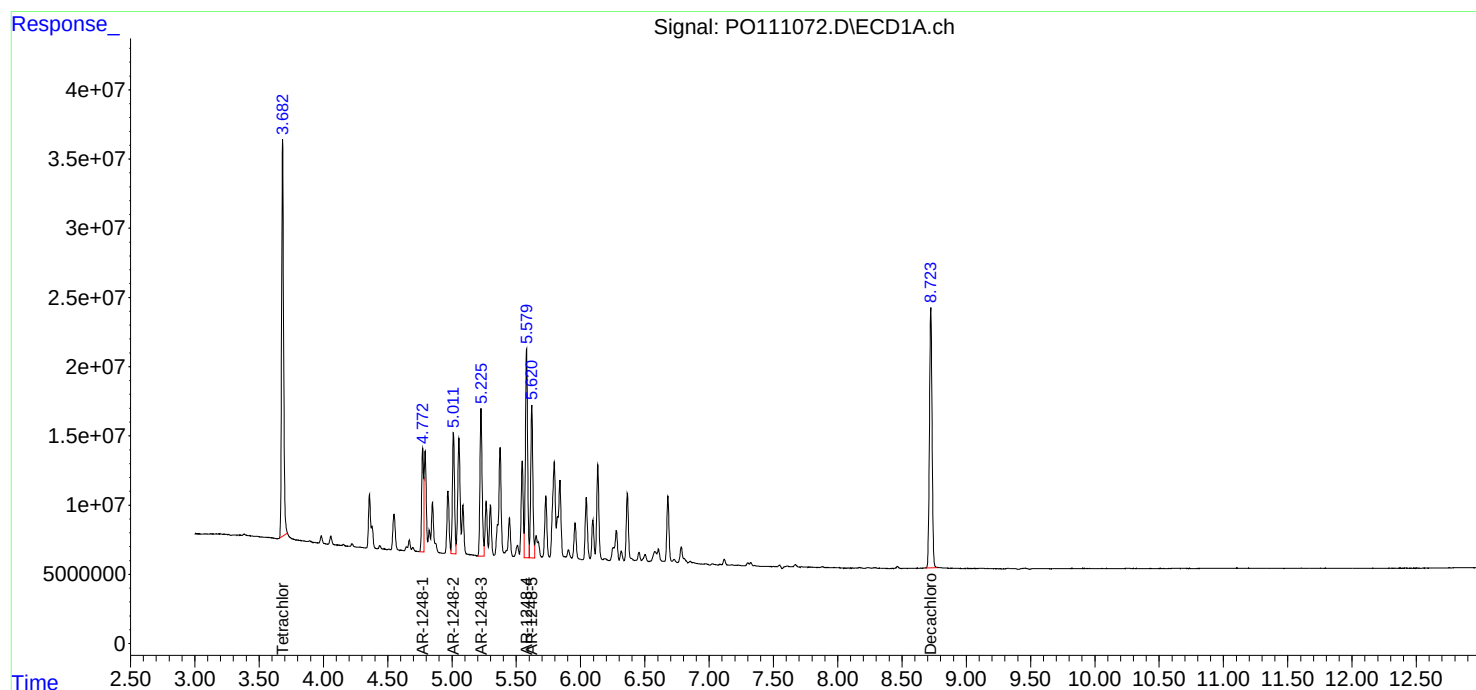

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 21:54
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:28:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:26:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.681	3.693	161.9E6	140.9E6	26.080	25.258
2) SA Decachlor...	8.722	8.687	140.1E6	49953933	26.543	26.366
Target Compounds						
21) L5 AR-1248-1	4.770	4.772	40860856	34628061	266.943	269.025
22) L5 AR-1248-2	5.009	5.008	53599803	46904652	266.629	267.777
23) L5 AR-1248-3	5.223	5.050	66929918	49939489	266.684	268.999
24) L5 AR-1248-4	5.577	5.221	95461725	56705002	267.937	261.329
25) L5 AR-1248-5	5.619	5.612	68942357	57059246	267.832	265.207



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 21:54
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:28:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:26:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

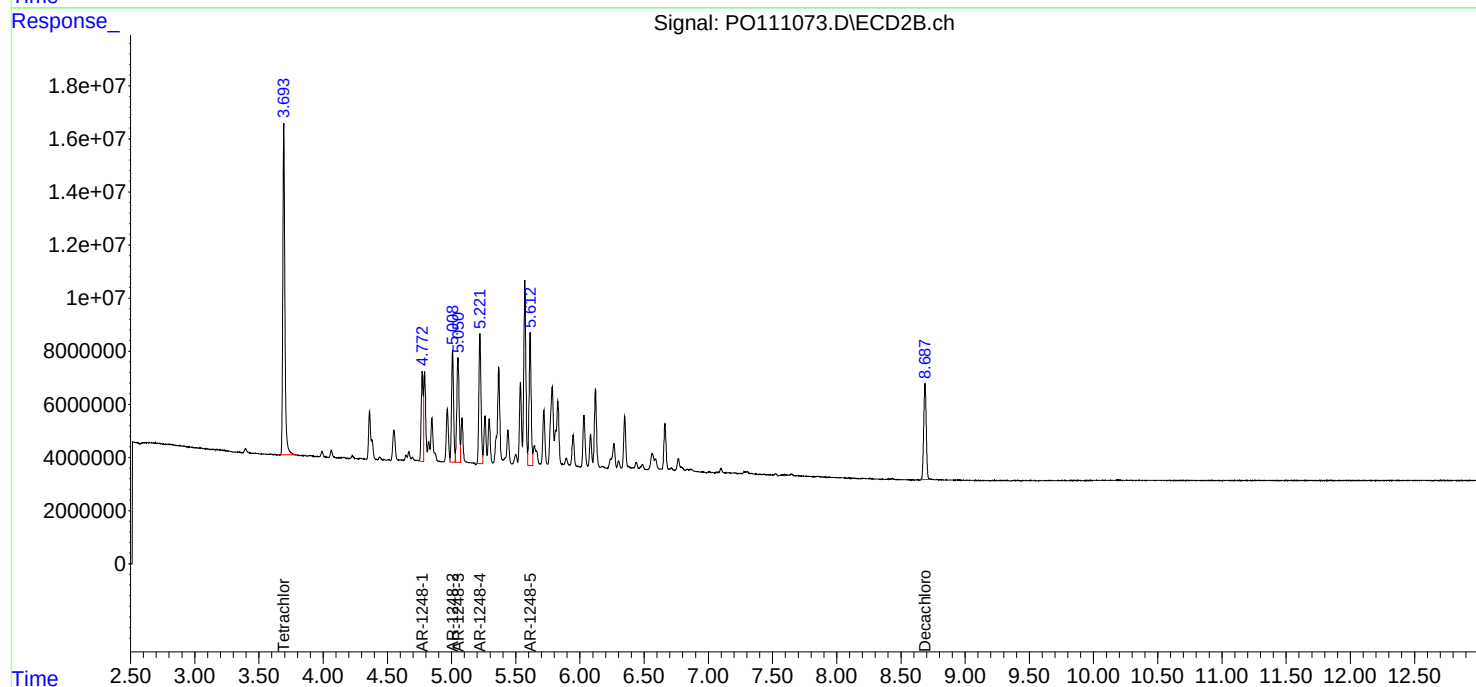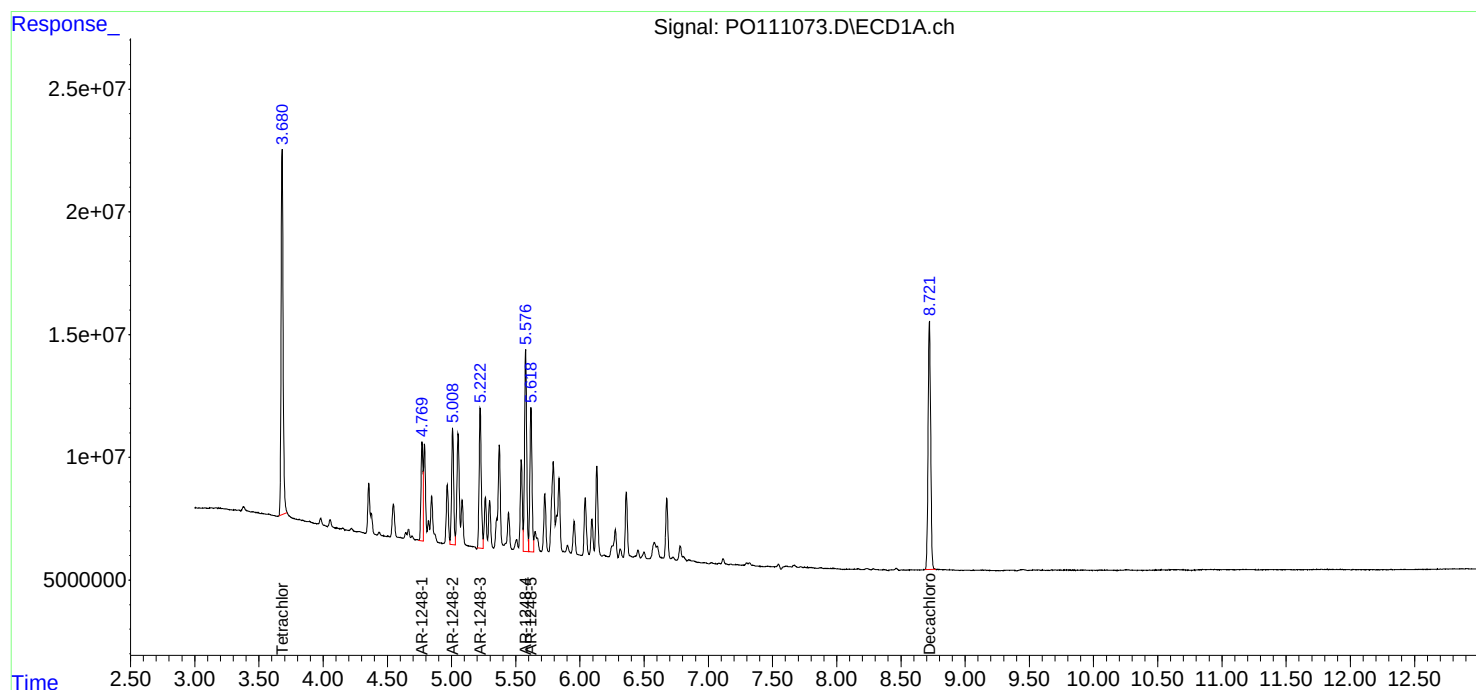

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 22:12
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:28:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:26:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	31378216	25949252	5.053	4.653
2) SA Decachlor...	8.724	8.673	28650863	10598091	5.428	5.594
Target Compounds						
21) L5 AR-1248-1	4.773	4.758	8260599	7117794	53.966	55.298
22) L5 AR-1248-2	5.012	4.995	10700058	9515063	53.227	54.321
23) L5 AR-1248-3	5.226	5.036	14779989	10314868	58.891	55.561
24) L5 AR-1248-4	5.580	5.207	20559074	12500823	57.704	57.611
25) L5 AR-1248-5	5.621	5.598	14994552	12205093	58.252	56.728



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 22:12
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:28:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:26:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

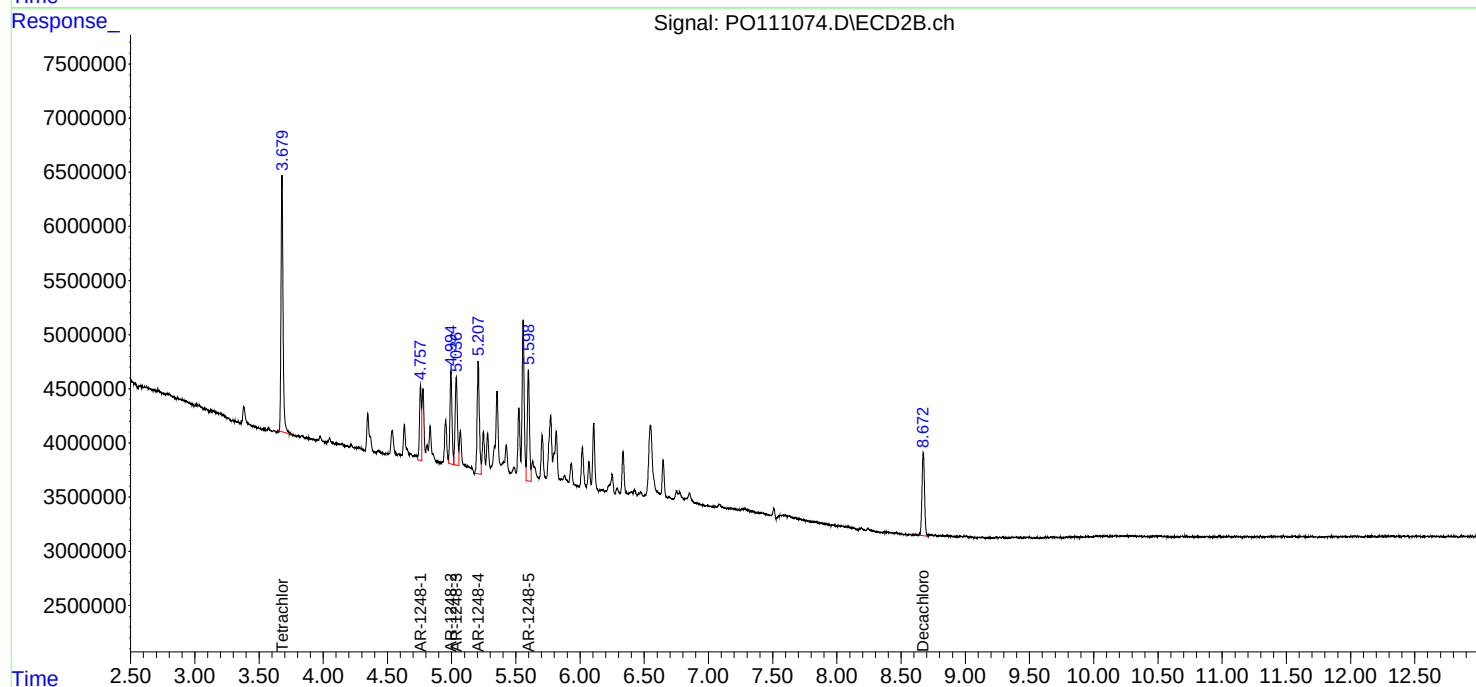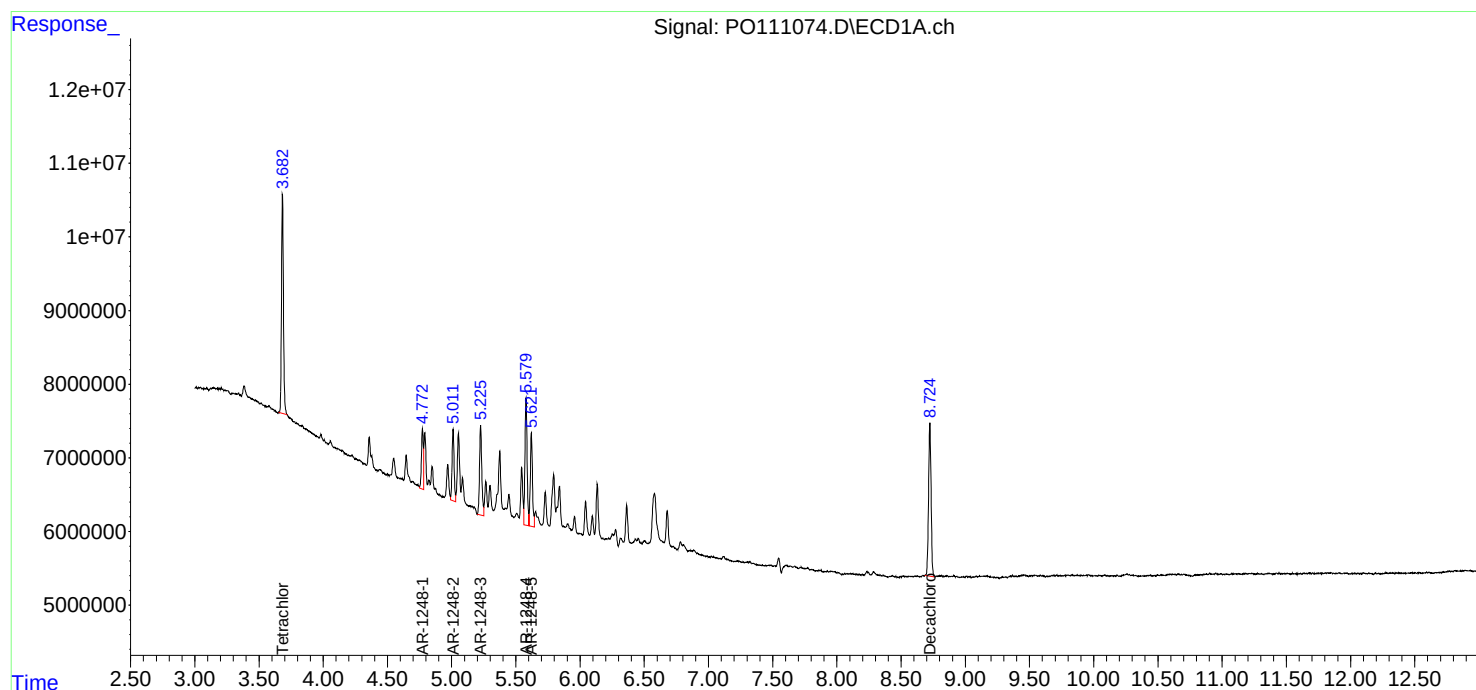

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 22:31
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:44:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:44:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	594.9E6	545.4E6	92.829	95.145
2) SA Decachlor...	8.725	8.674	492.4E6	173.0E6	90.453	91.041
Target Compounds						
26) L6 AR-1254-1	5.581	5.558	338.7E6	294.8E6	892.260	911.119
27) L6 AR-1254-2	5.730	5.706	291.9E6	254.2E6	889.968	903.137
28) L6 AR-1254-3	6.134	6.107	475.3E6	400.5E6	907.531	923.736
29) L6 AR-1254-4	6.364	6.336	302.1E6	228.9E6	899.437	914.476
30) L6 AR-1254-5	6.784	6.752	429.2E6	318.4E6	903.044	923.844



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 22:31
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:44:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:44:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

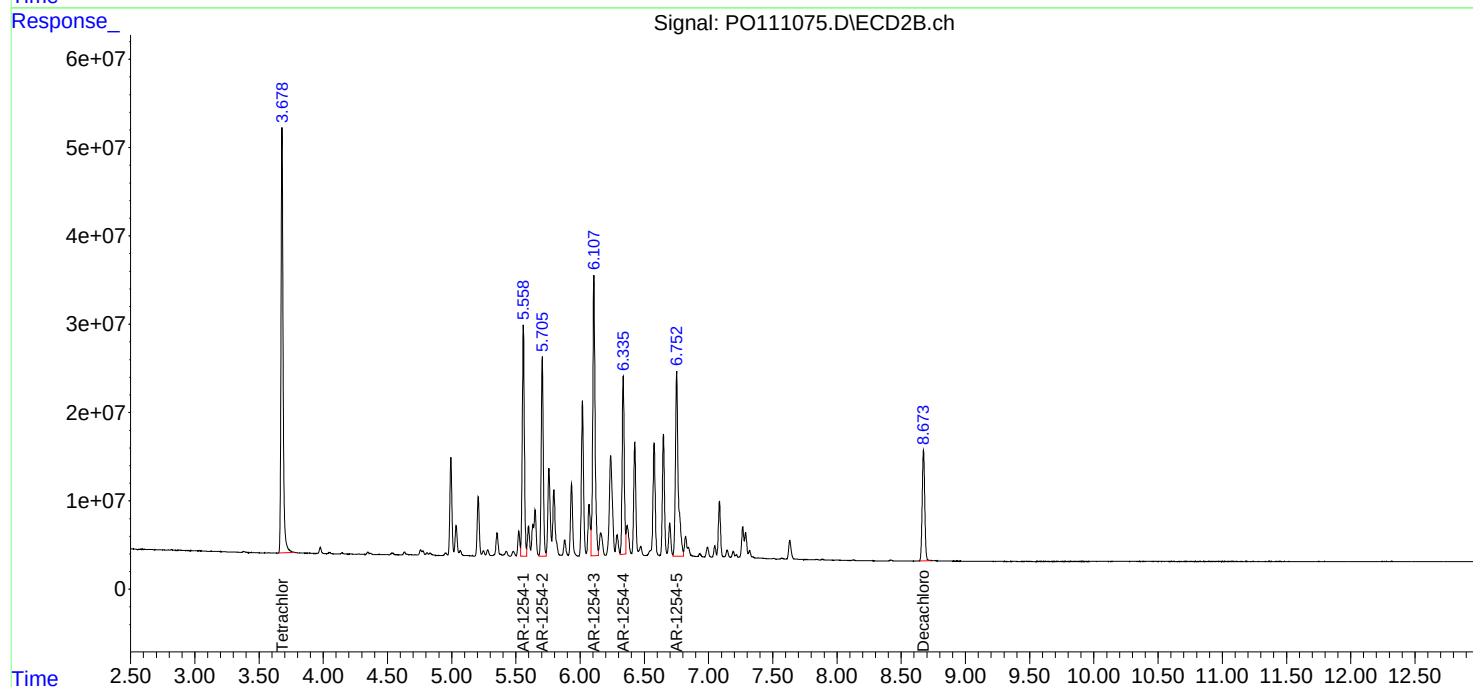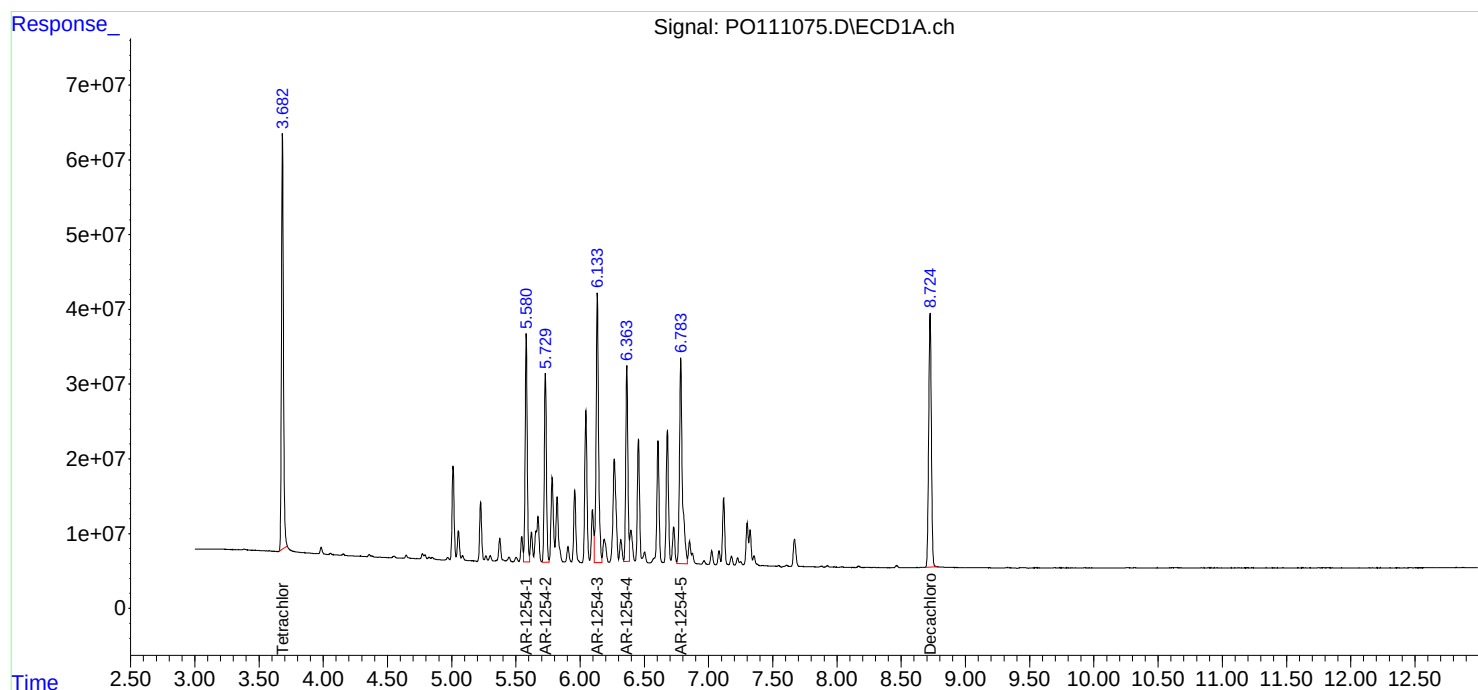

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 22:49
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:45:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:44:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	464.3E6	419.4E6	72.445	73.166
2) SA Decachlor...	8.725	8.674	385.6E6	135.3E6	70.833	71.214
Target Compounds						
26) L6 AR-1254-1	5.580	5.558	269.5E6	231.2E6	710.036	714.469
27) L6 AR-1254-2	5.730	5.706	232.6E6	200.0E6	709.227	710.467
28) L6 AR-1254-3	6.134	6.108	374.9E6	311.4E6	715.696	718.231
29) L6 AR-1254-4	6.363	6.336	239.1E6	178.6E6	711.714	713.500
30) L6 AR-1254-5	6.784	6.753	339.0E6	247.1E6	713.244	717.200



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 22:49
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:45:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:44:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

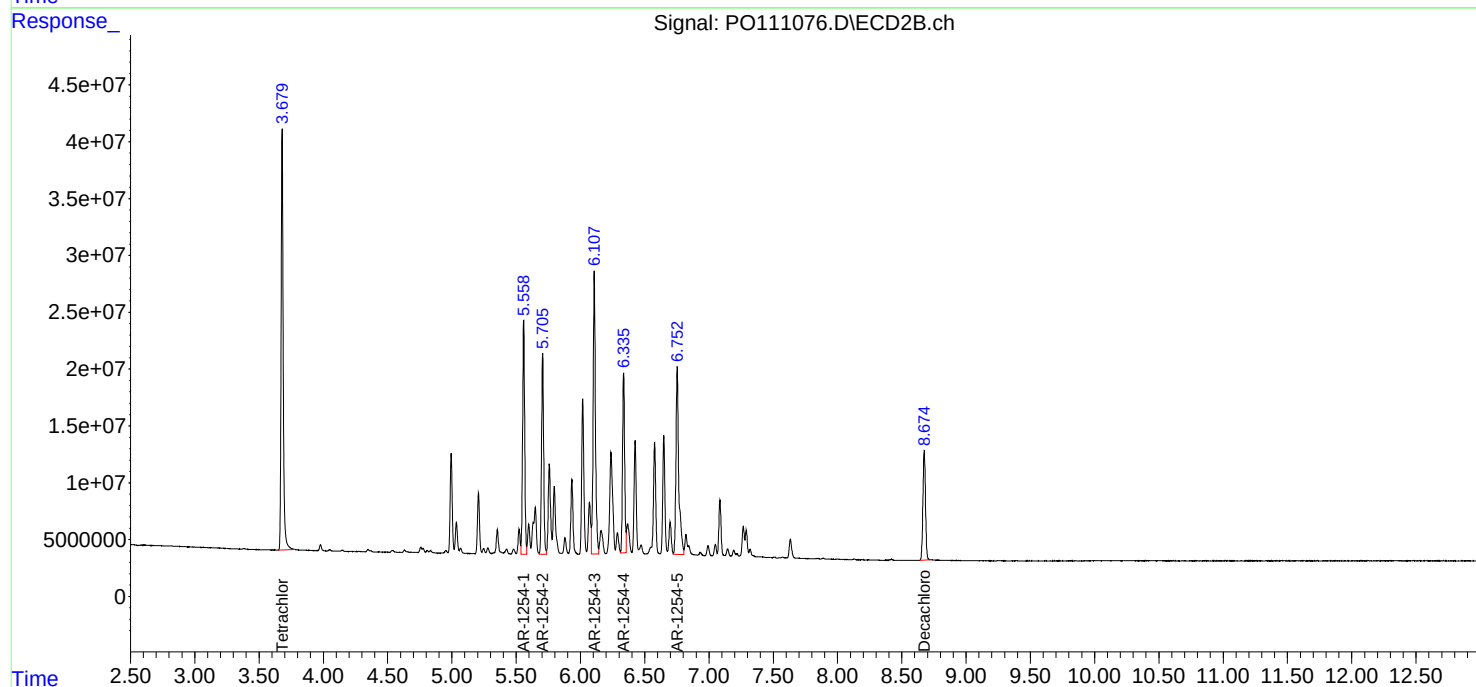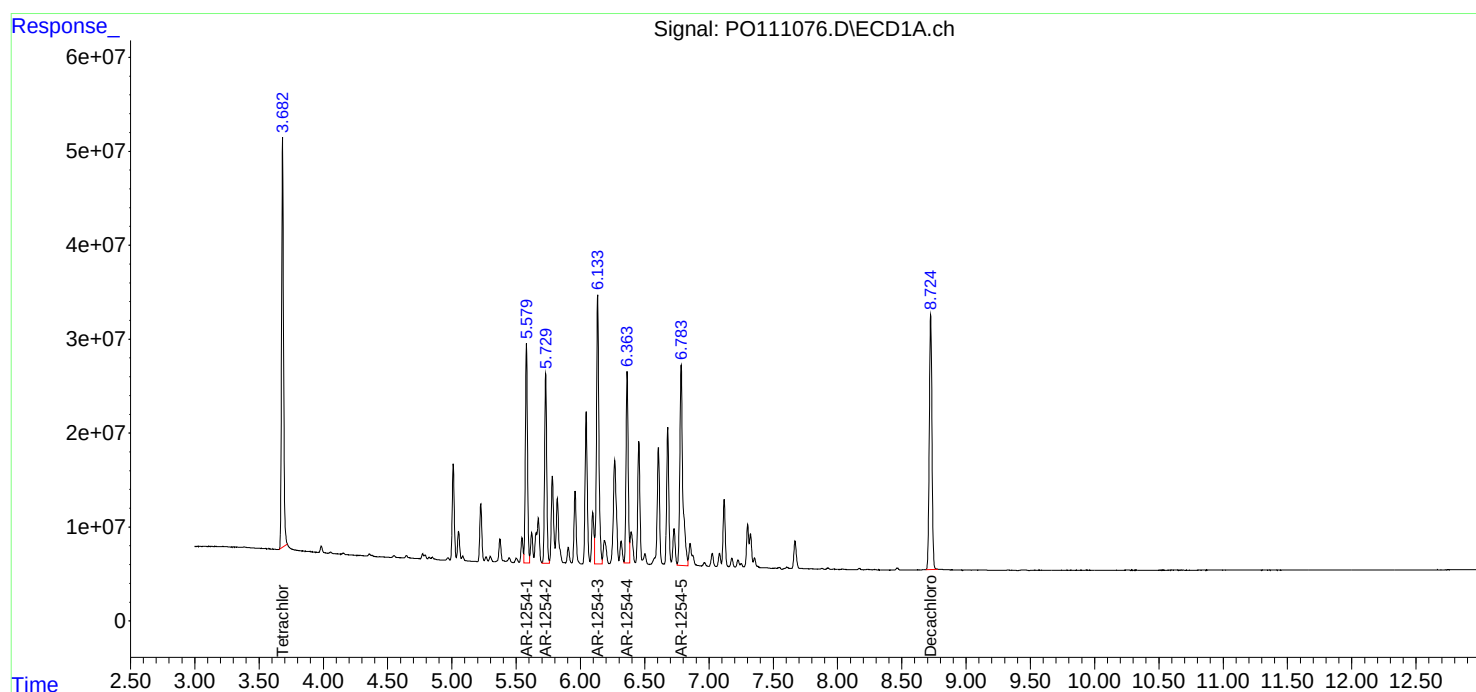

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 23:06
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:45:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:44:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.681	3.679	320.4E6	286.6E6	50.000	50.000
2) SA Decachlor...	8.722	8.673	272.2E6	95028644	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	5.578	5.557	189.8E6	161.8E6	500.000	500.000
27) L6 AR-1254-2	5.727	5.705	164.0E6	140.7E6	500.000	500.000
28) L6 AR-1254-3	6.132	6.107	261.9E6	216.8E6	500.000	500.000
29) L6 AR-1254-4	6.361	6.335	167.9E6	125.1E6	500.000	500.000
30) L6 AR-1254-5	6.781	6.751	237.7E6	172.3E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 23:06
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:45:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:44:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

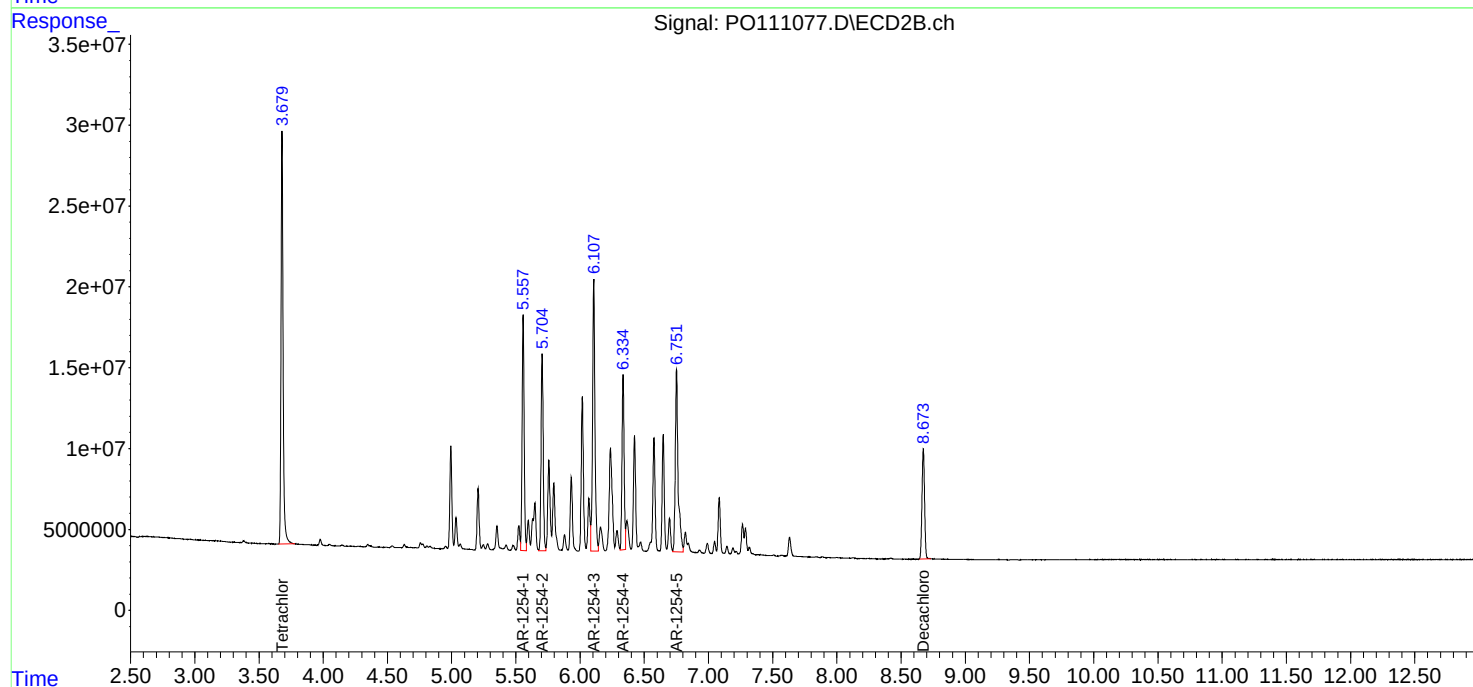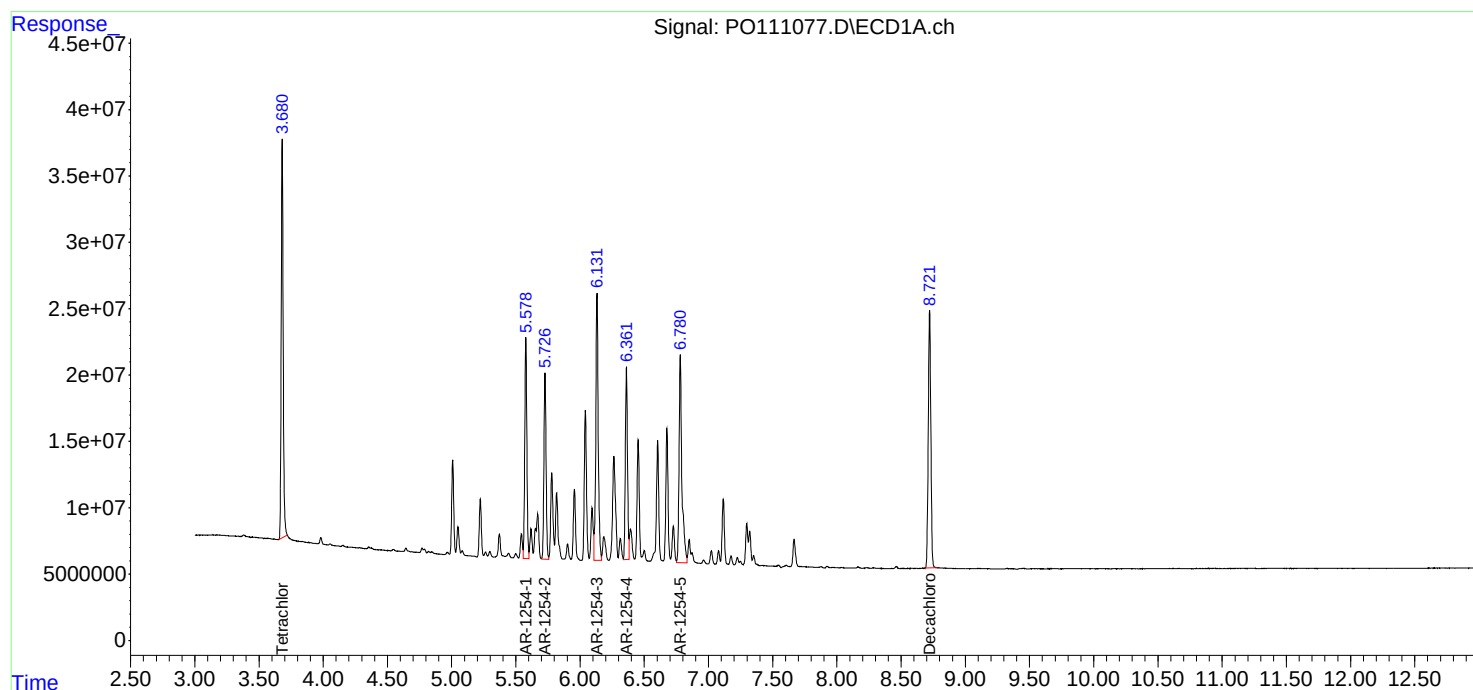

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 23:25
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:45:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:44:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	164.6E6	143.2E6	25.683	24.975
2) SA Decachlor...	8.723	8.674	142.5E6	50465688	26.181	26.553
Target Compounds						
26) L6 AR-1254-1	5.581	5.558	100.5E6	84767134	264.857	261.944
27) L6 AR-1254-2	5.730	5.706	86931936	74488276	265.082	264.655
28) L6 AR-1254-3	6.134	6.108	137.3E6	112.1E6	262.162	258.480
29) L6 AR-1254-4	6.364	6.336	87996975	64908604	261.987	259.337
30) L6 AR-1254-5	6.783	6.752	125.2E6	89675566	263.481	260.235



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 23:25
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:45:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:44:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

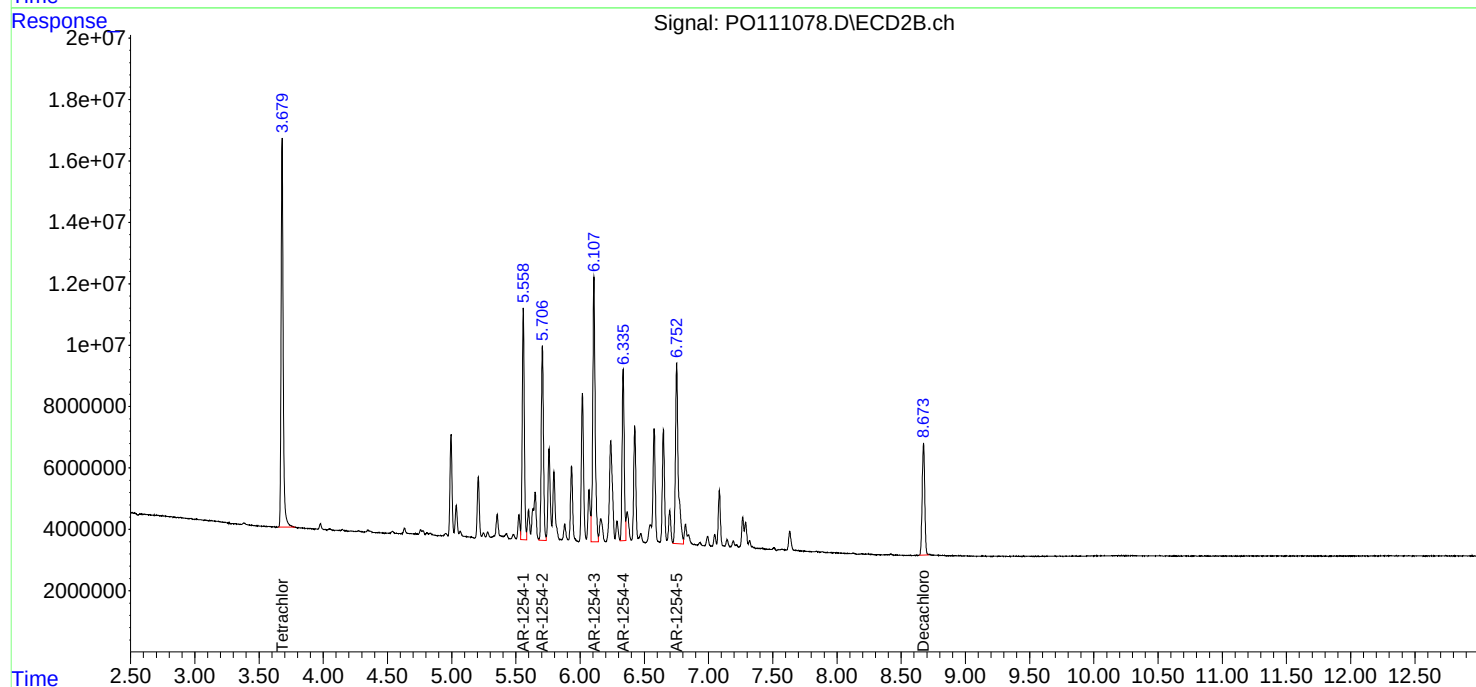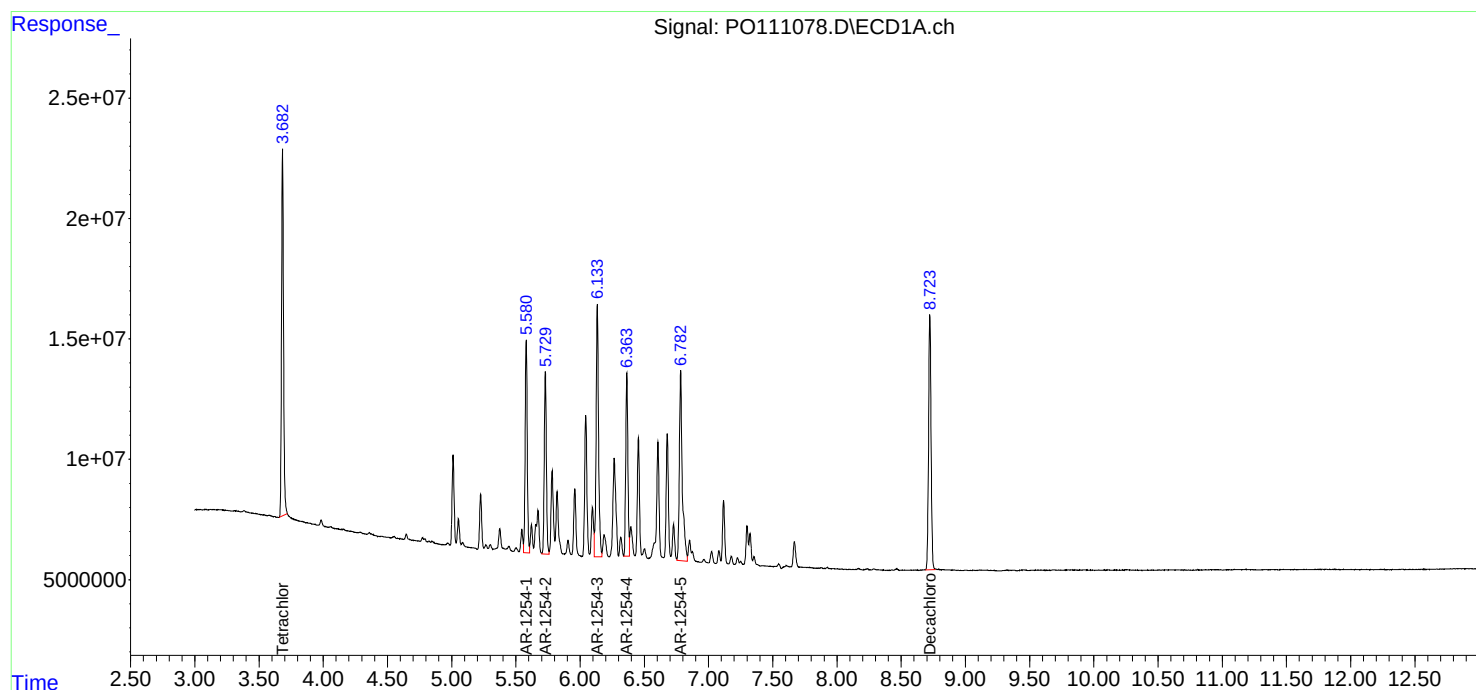

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 23:43
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:46:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:44:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.682	3.679	31694642	26928528	4.946	4.698
2) SA Decachlor...	8.724	8.674	29313873	10245264	5.385	5.391
Target Compounds						
26) L6 AR-1254-1	5.580	5.558	20909365	17719774	55.088	54.757
27) L6 AR-1254-2	5.729	5.706	17811498	15800223	54.313	56.138
28) L6 AR-1254-3	6.134	6.107	29128076	22990579	55.613	53.030
29) L6 AR-1254-4	6.364	6.335	18583927	12990476	55.329	51.902
30) L6 AR-1254-5	6.783	6.752	25740607	18926439	54.156	54.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 23:43
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:46:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:44:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

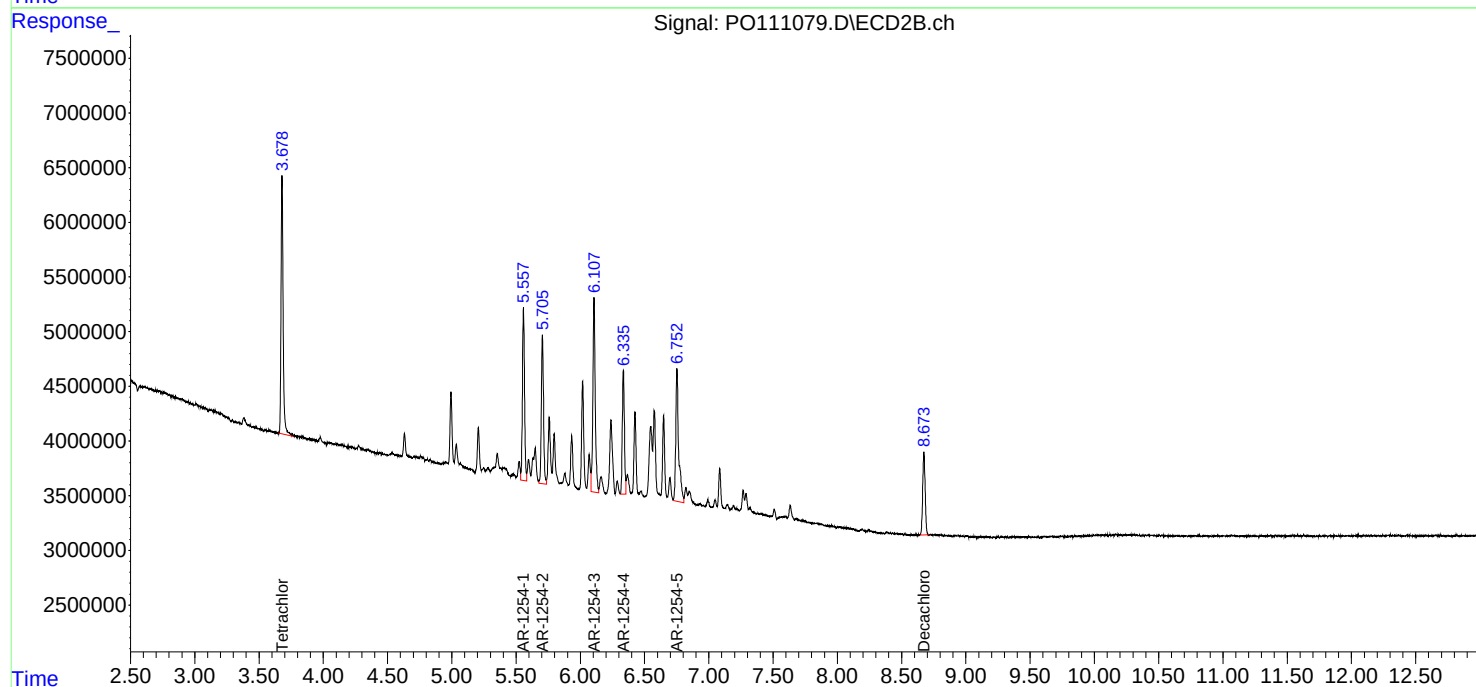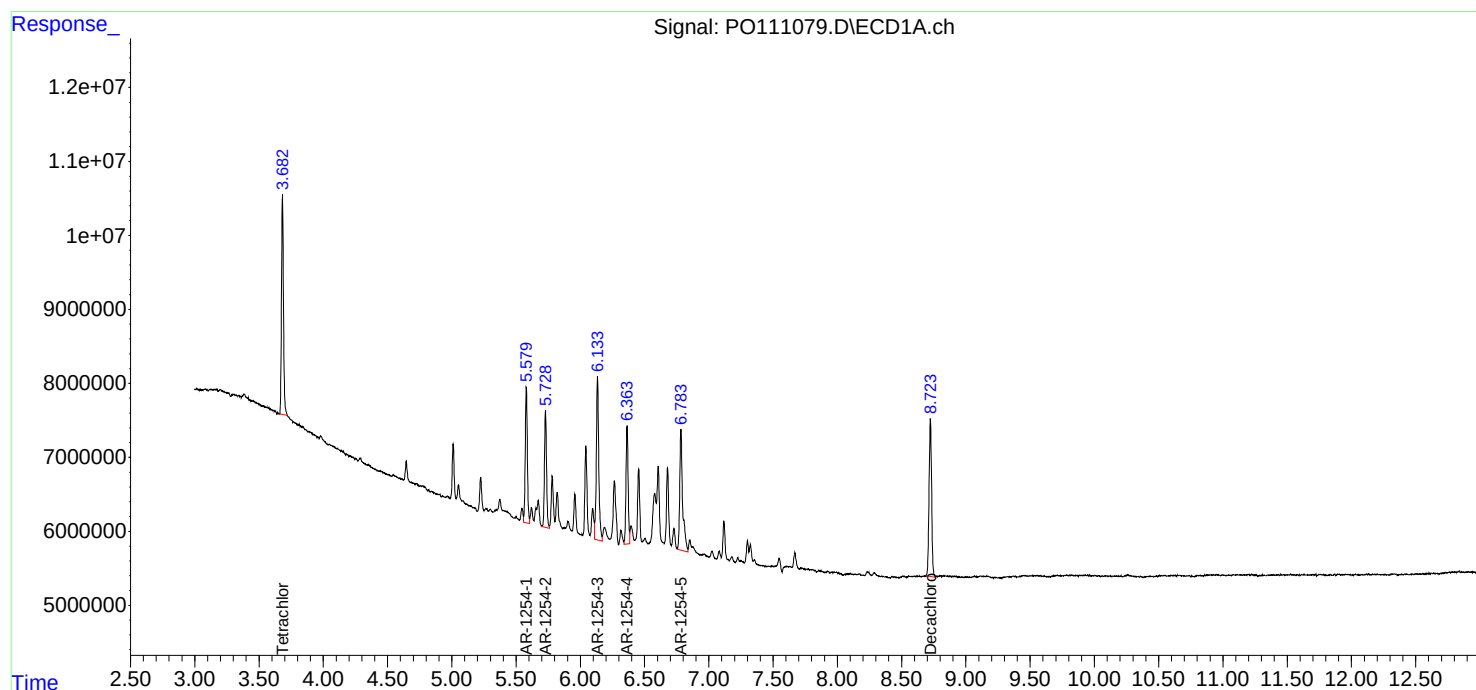

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 00:01
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 05:59:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 05:58:56 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	303.0E6	269.7E6	50.000	50.000
2) SA Decachlor...	8.725	8.674	257.1E6	90216078	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	6.823	6.792	243.3E6	170.4E6	500.000	500.000
37) L8 AR-1262-2	7.325	7.291	404.2E6	251.4E6	500.000	500.000
38) L8 AR-1262-3	7.609	7.573	169.1E6	93817526	500.000	500.000
39) L8 AR-1262-4	7.674	7.637	295.2E6	165.1E6	500.000	500.000
40) L8 AR-1262-5	8.170	8.129	142.6E6	56152869	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 00:01
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 05:59:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 05:58:56 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

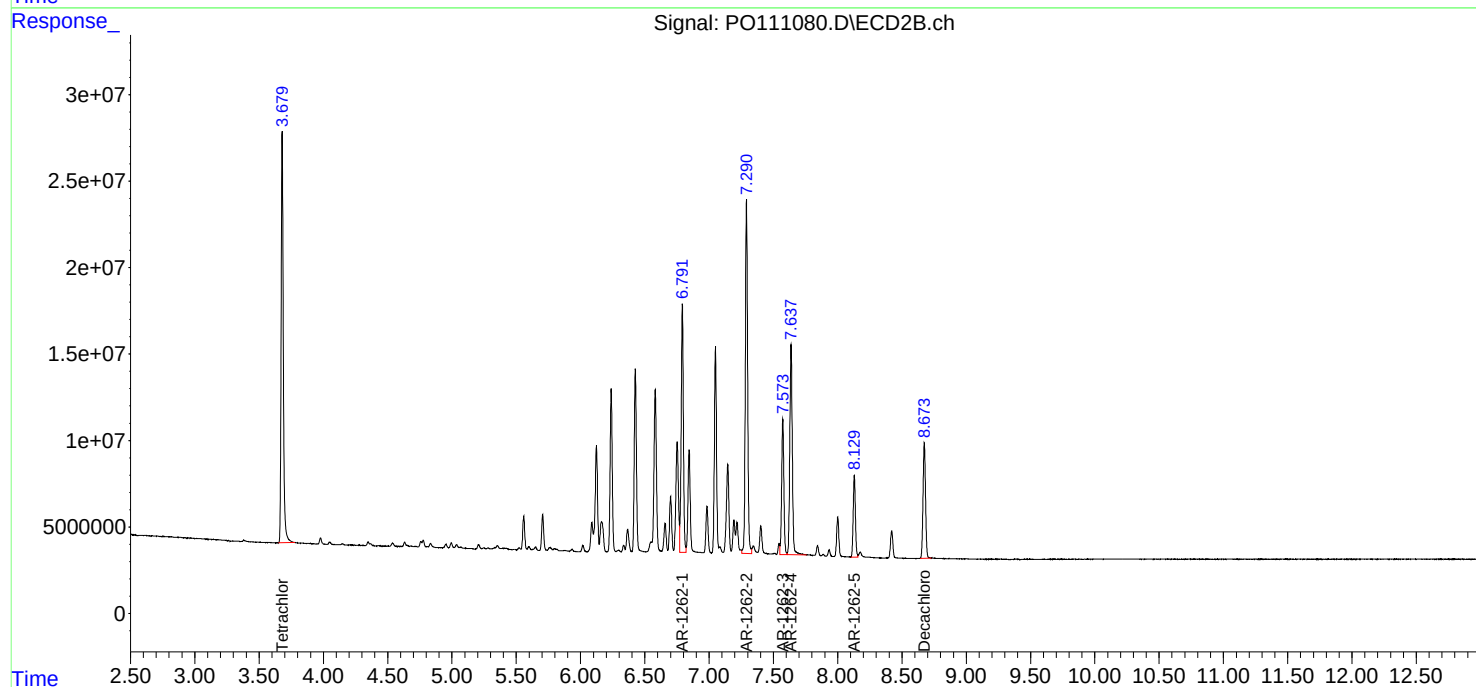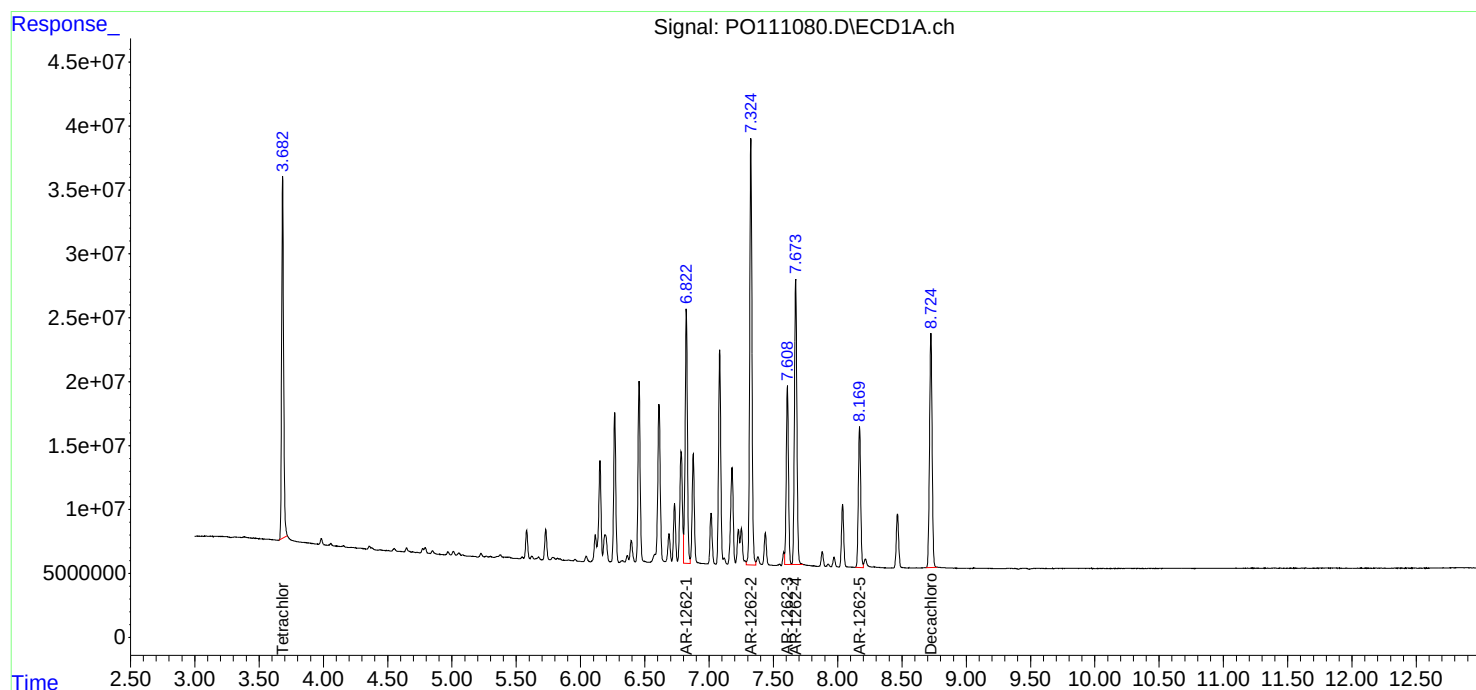

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 00:19
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:14:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:12:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.681	3.679	617.2E6	563.6E6	95.813	97.941
2) SA Decachlor...	8.722	8.673	888.9E6	302.3E6	93.525	92.754
Target Compounds						
41) L9 AR-1268-1	7.607	7.572	930.9E6	505.7E6	951.478	954.847
42) L9 AR-1268-2	7.672	7.636	856.4E6	460.5E6	949.753	951.728
43) L9 AR-1268-3	7.879	7.843	718.7E6	328.7E6	939.809	940.342
44) L9 AR-1268-4	8.168	8.129	311.2E6	119.7E6	939.708	916.655
45) L9 AR-1268-5	8.463	8.419	2117.7E6	727.9E6	964.968	960.699



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 00:19
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:14:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

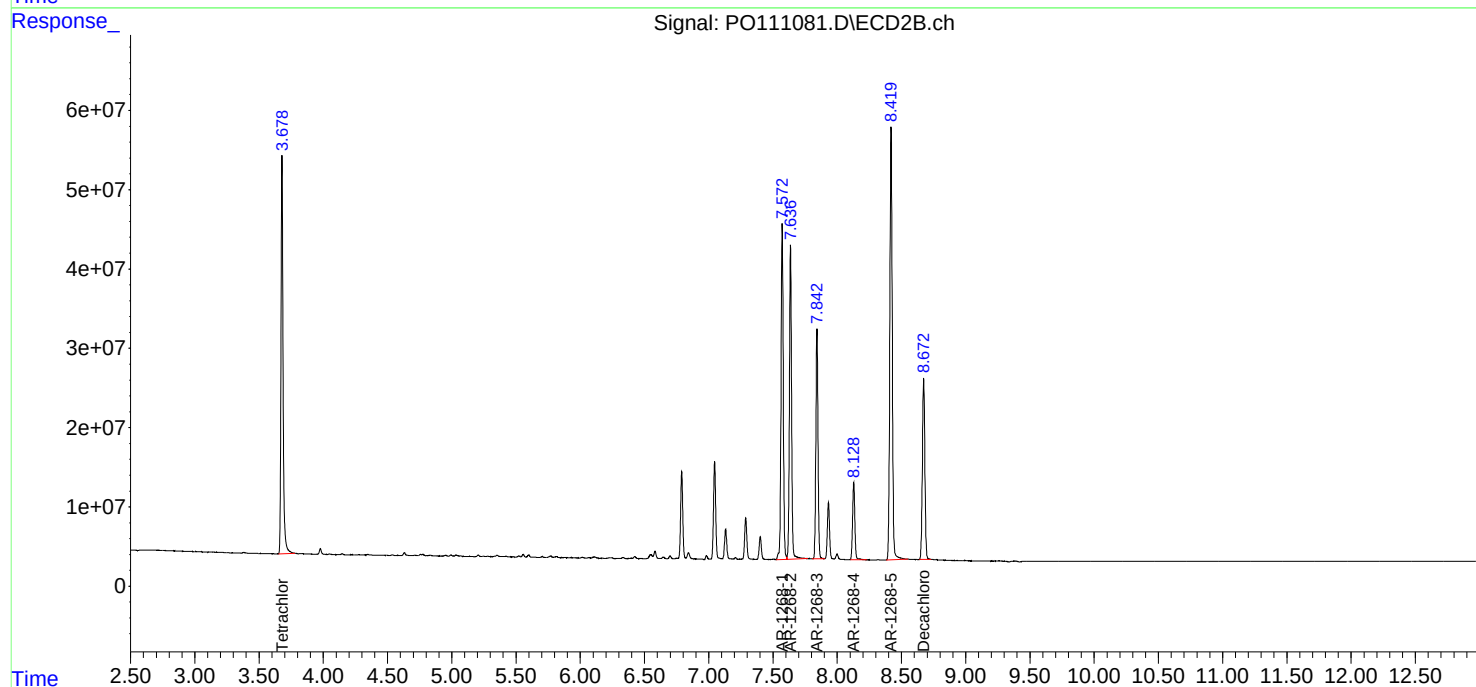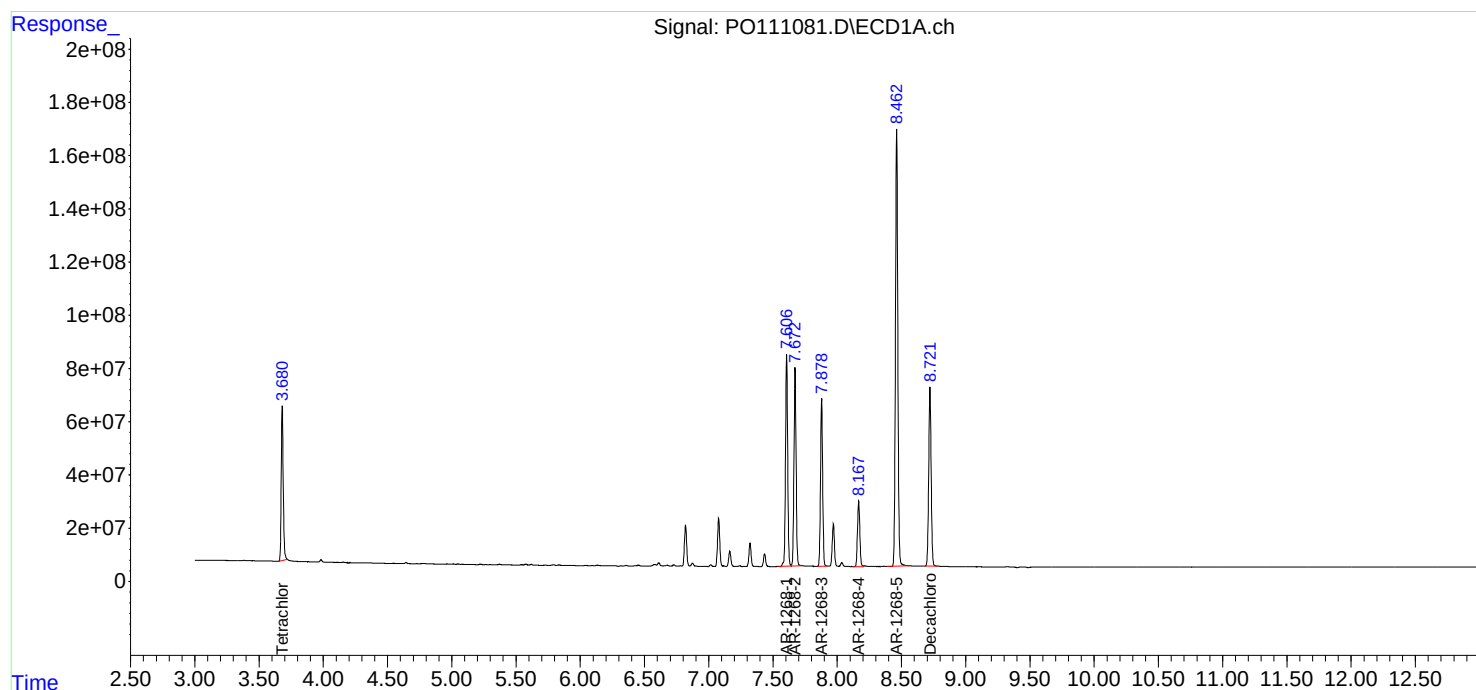

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 00:37
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:14:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:12:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	462.6E6	419.6E6	71.819	72.910
2) SA Decachlor...	8.723	8.673	676.0E6	230.8E6	71.125	70.822
Target Compounds						
41) L9 AR-1268-1	7.608	7.572	702.4E6	381.3E6	717.998	719.962
42) L9 AR-1268-2	7.673	7.637	645.4E6	348.7E6	715.759	720.605
43) L9 AR-1268-3	7.880	7.843	544.2E6	250.4E6	711.612	716.368
44) L9 AR-1268-4	8.169	8.129	234.9E6	92055642	709.264	704.972
45) L9 AR-1268-5	8.465	8.420	1580.5E6	548.4E6	720.183	723.788



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 00:37
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:14:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

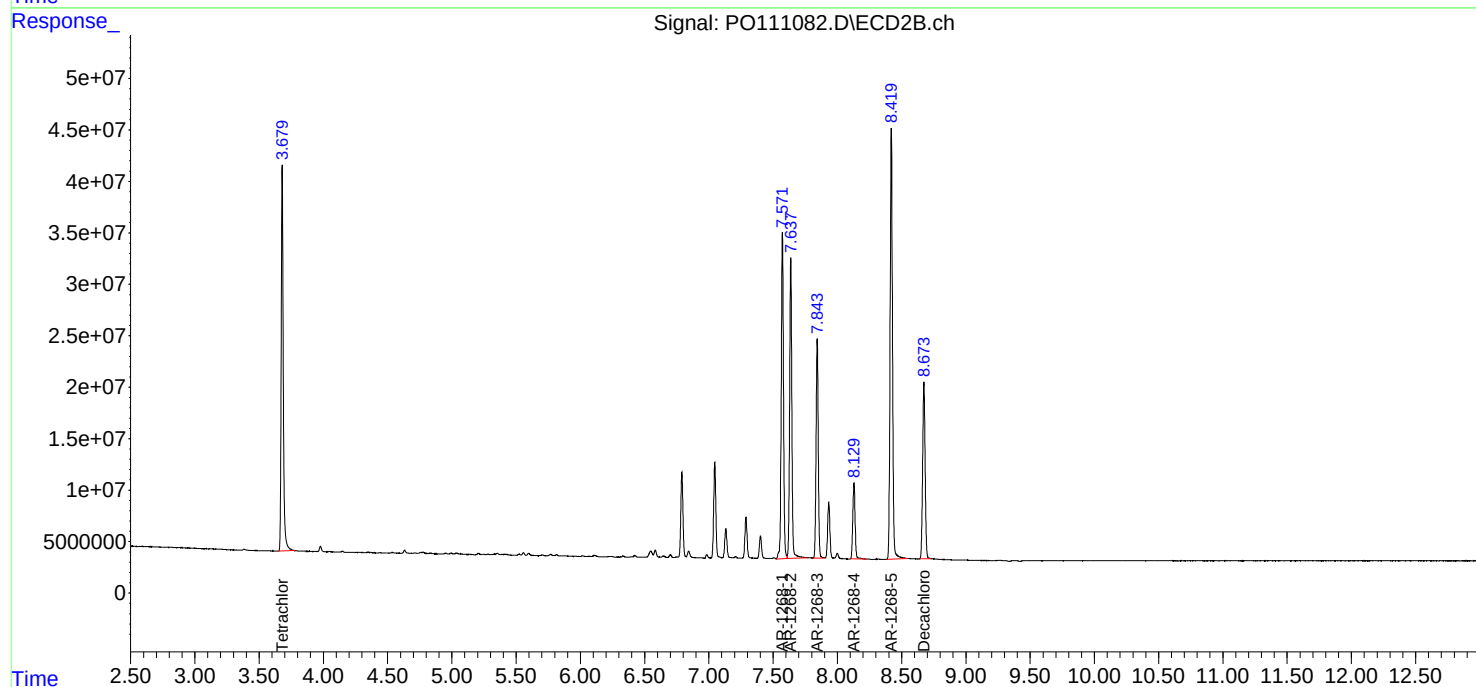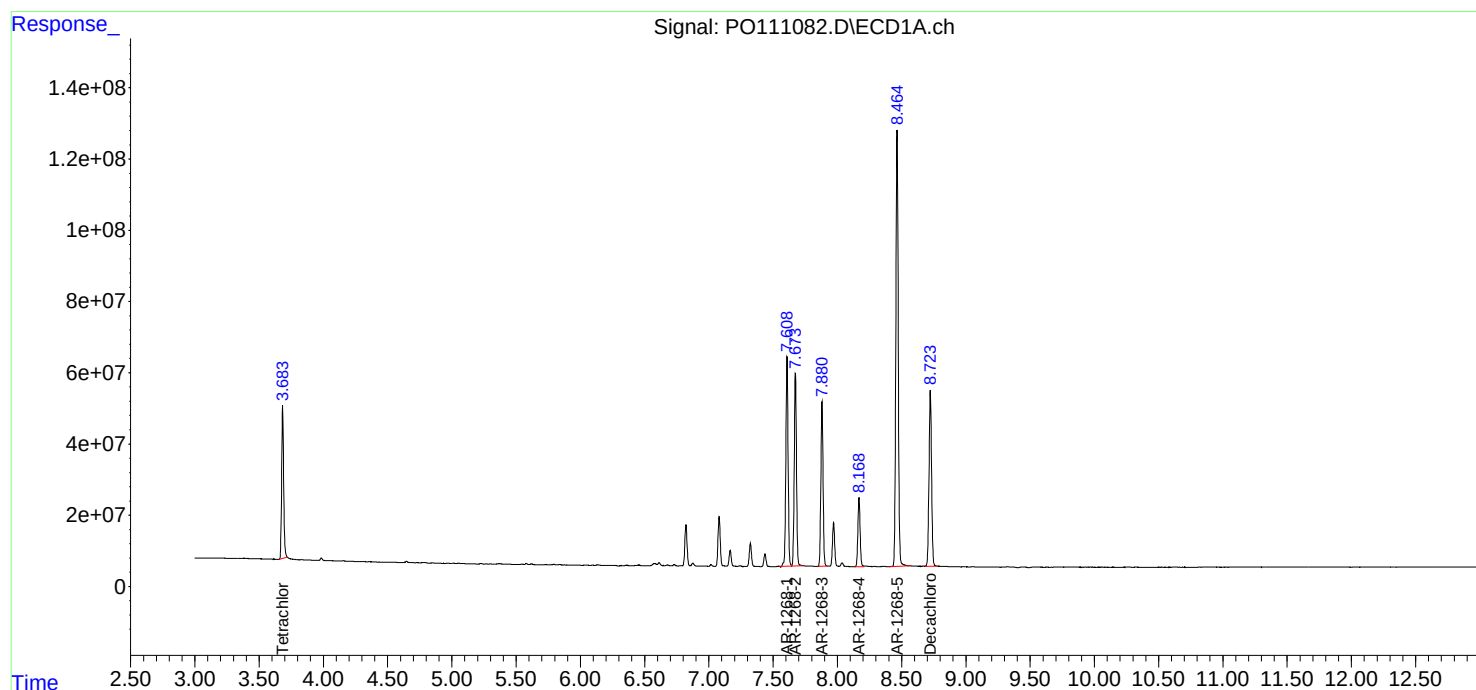

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 00:56
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:16:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:12:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	322.1E6	287.7E6	50.000	50.000
2) SA Decachlor...	8.725	8.674	475.2E6	162.9E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	7.609	7.573	489.2E6	264.8E6	500.000	500.000
42) L9 AR-1268-2	7.674	7.638	450.8E6	241.9E6	500.000	500.000
43) L9 AR-1268-3	7.881	7.843	382.3E6	174.8E6	500.000	500.000
44) L9 AR-1268-4	8.169	8.130	165.6E6	65290300	500.000	500.000
45) L9 AR-1268-5	8.466	8.421	1097.3E6	378.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 00:56
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:16:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

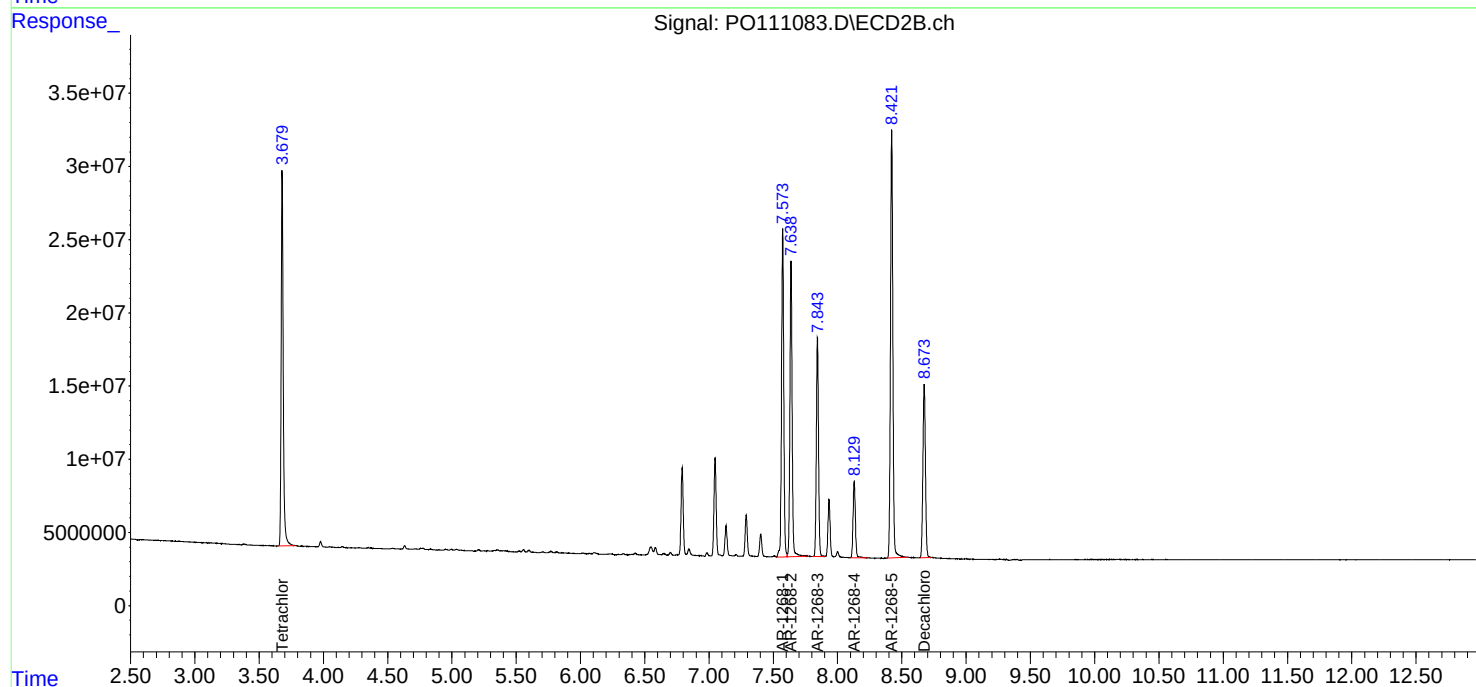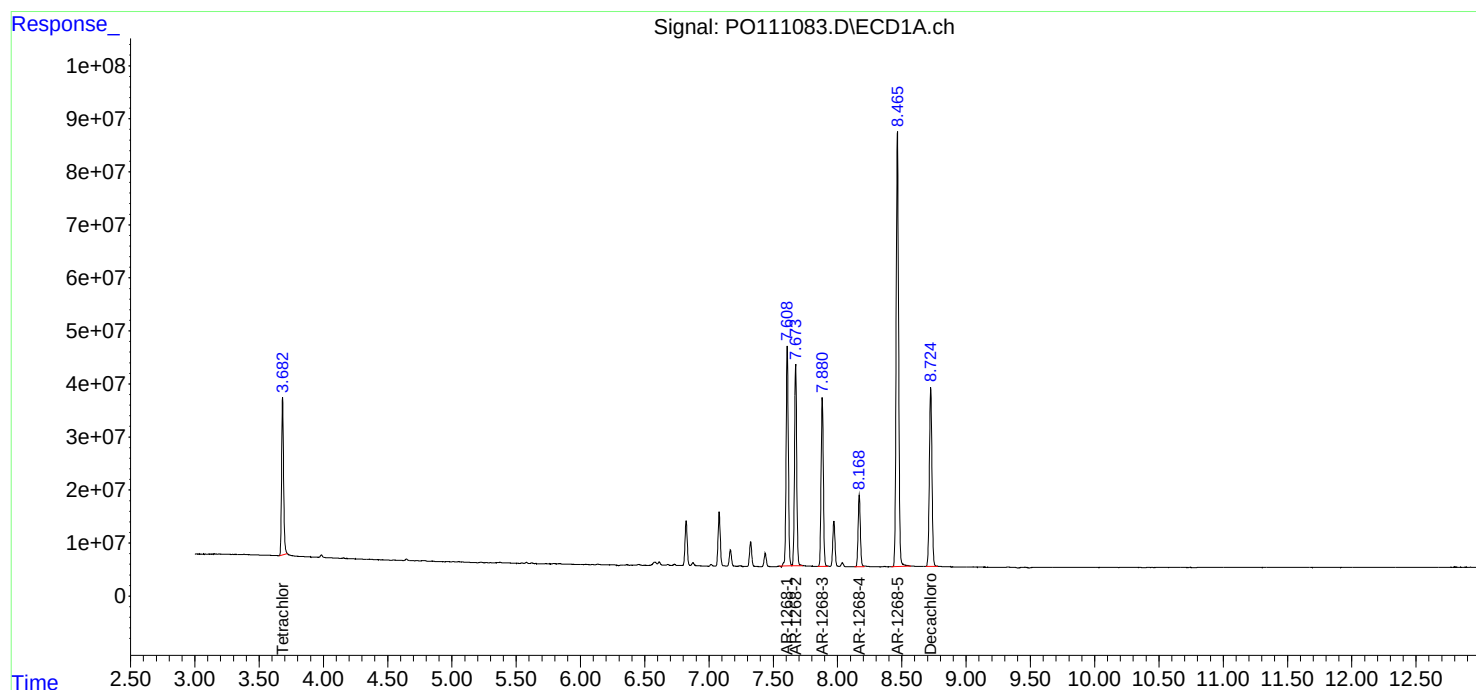

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 01:14
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:17:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:12:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	166.8E6	145.0E6	25.903	25.196
2) SA Decachlor...	8.723	8.673	248.9E6	85935998	26.191	26.371
Target Compounds						
41) L9 AR-1268-1	7.609	7.573	254.0E6	137.6E6	259.607	259.774
42) L9 AR-1268-2	7.673	7.638	233.6E6	125.8E6	259.118	260.022
43) L9 AR-1268-3	7.880	7.842	200.0E6	91603449	261.528	262.093
44) L9 AR-1268-4	8.168	8.129	86826426	34659840	262.172	265.429
45) L9 AR-1268-5	8.464	8.421	558.8E6	195.1E6	254.607	257.459



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 01:14
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:17:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

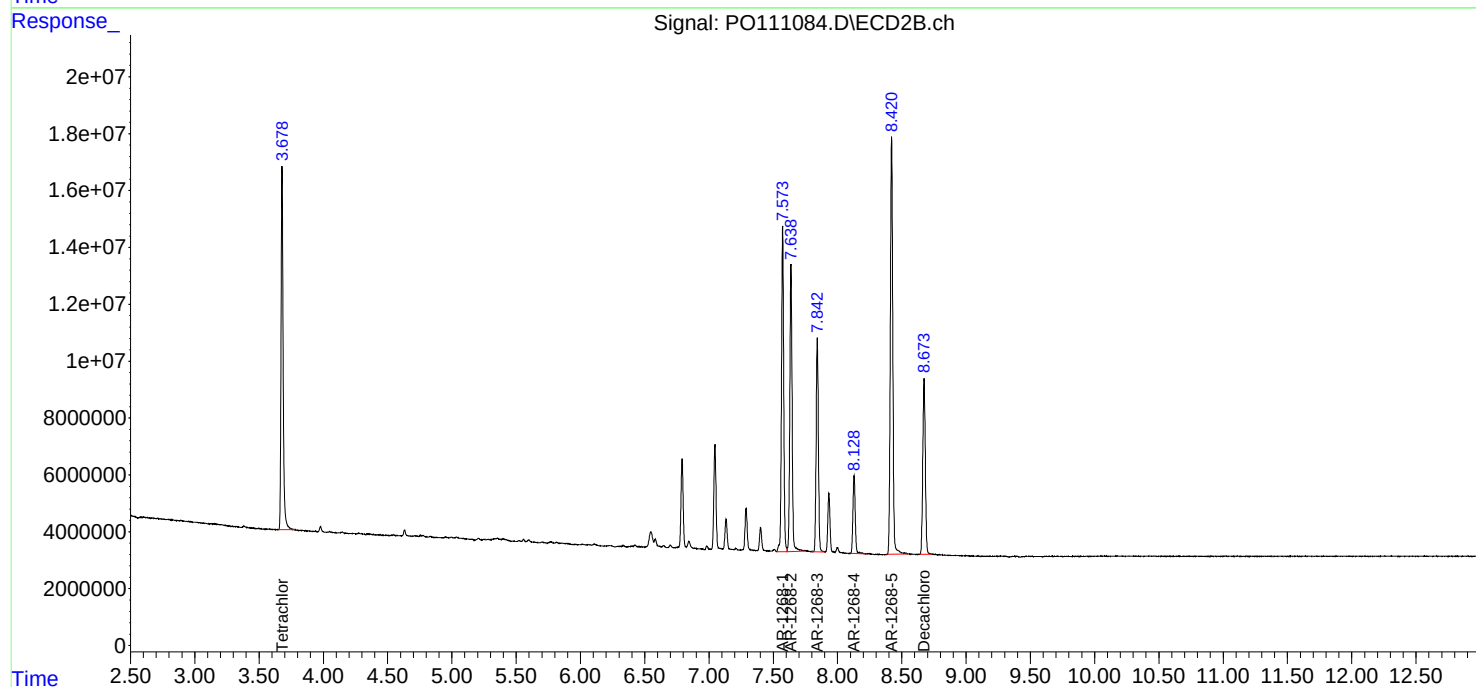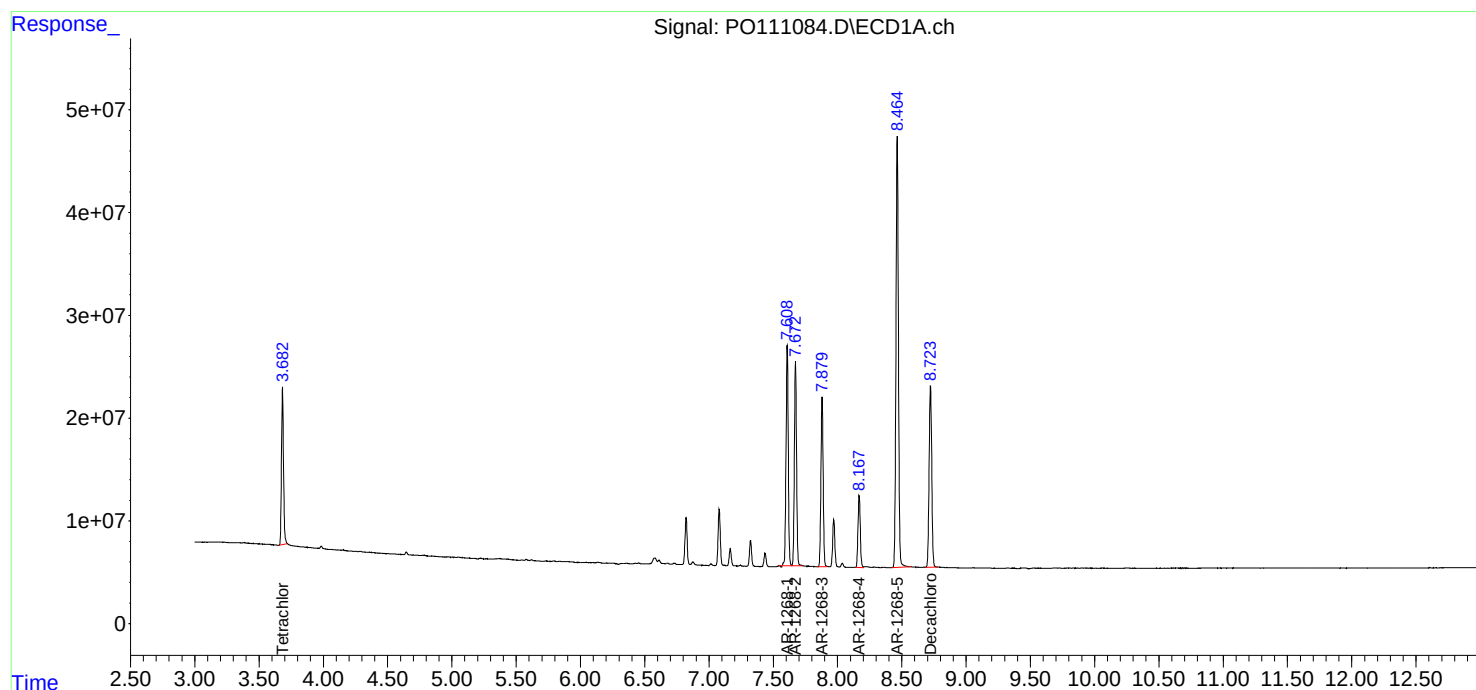

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 01:31
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:17:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:12:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.681	3.679	30851086	25765381	4.790	4.477
2) SA Decachlor...	8.721	8.673	48646145	16506911	5.119	5.065
Target Compounds						
41) L9 AR-1268-1	7.607	7.572	49315996	27830093	50.408	52.552
42) L9 AR-1268-2	7.671	7.637	45468978	24959856	50.426	51.586
43) L9 AR-1268-3	7.879	7.842	39262321	18191772	51.343	52.050
44) L9 AR-1268-4	8.167	8.128	16499854	6234396	49.821	47.744
45) L9 AR-1268-5	8.463	8.420	106.9E6	38344241	48.698	50.605



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 01:31
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:17:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:12:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

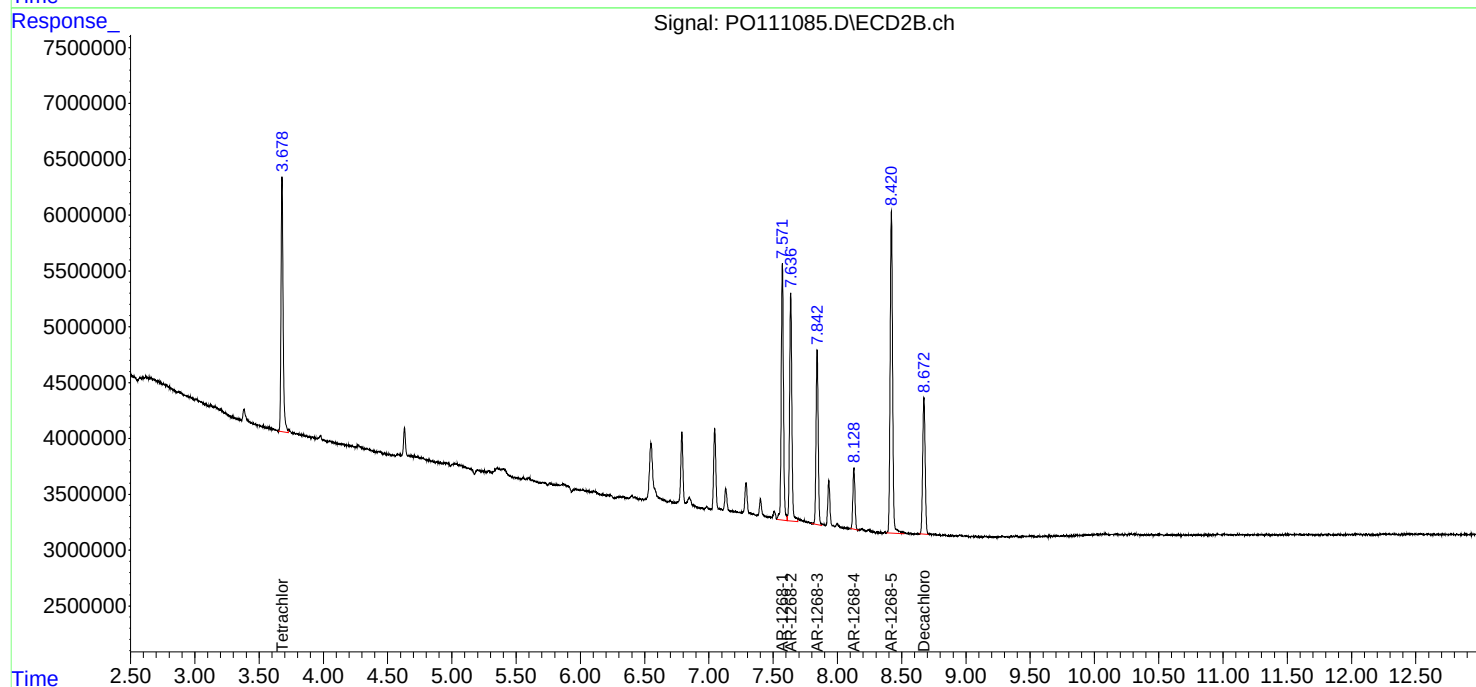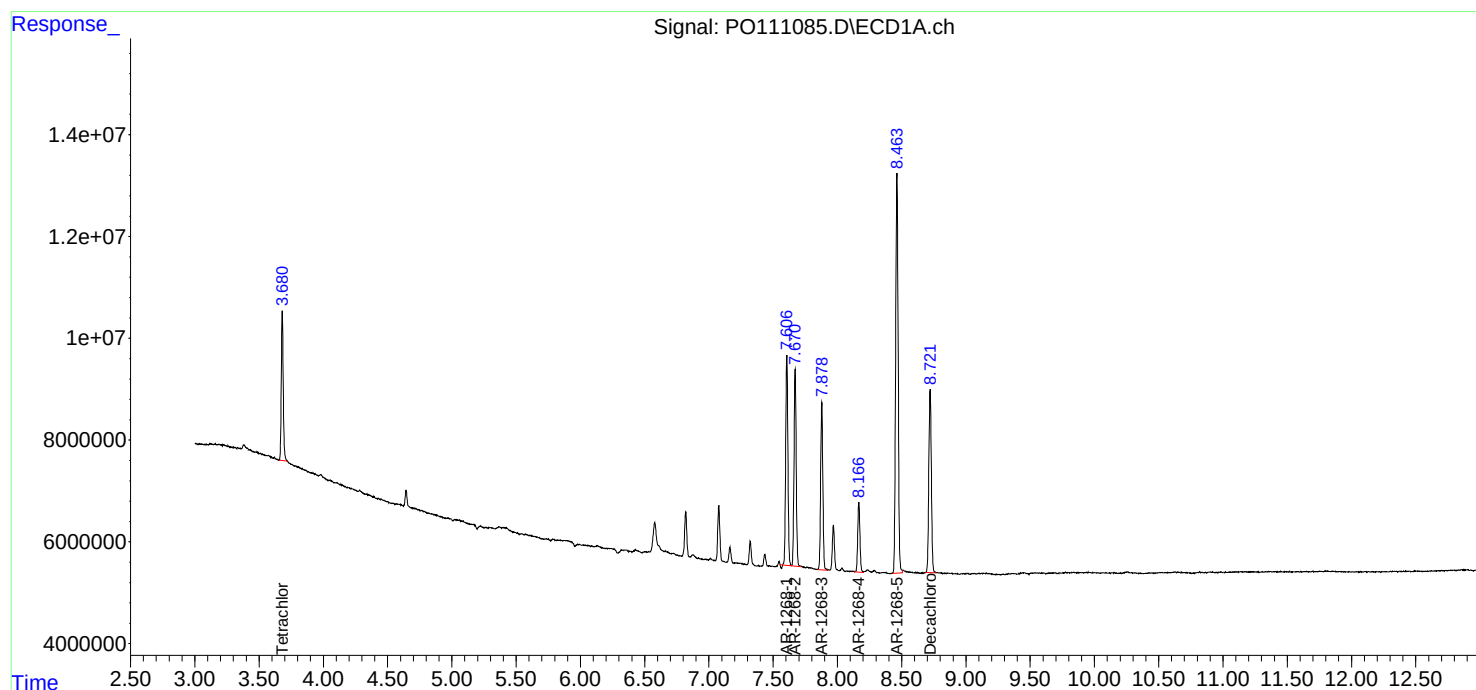

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 01:50
 Operator : YP/AJ
 Sample : P0051525ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO051525

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:39:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:36:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	299.9E6	278.2E6	50.977	51.032
2) SA Decachlor...	8.724	8.674	257.8E6	95007008	49.937	51.351
Target Compounds						
3) L1 AR-1016-1	4.774	4.759	114.2E6	95398004	507.589	499.656
4) L1 AR-1016-2	4.793	4.778	161.4E6	137.6E6	506.205	496.569
5) L1 AR-1016-3	4.849	4.953	112.3E6	73817070	517.291	505.337
6) L1 AR-1016-4	4.969	4.995	88734333	60529384	509.534	504.039
7) L1 AR-1016-5	5.226	5.208	90702842	77413957	515.382	501.384
31) L7 AR-1260-1	6.266	6.238	155.3E6	125.8E6	509.245	503.619
32) L7 AR-1260-2	6.455	6.426	192.1E6	147.5E6	501.513	501.050
33) L7 AR-1260-3	6.822	6.578	175.9E6	139.3E6	504.478	485.852
34) L7 AR-1260-4	7.082	7.049	141.0E6	101.6E6	503.768	506.176
35) L7 AR-1260-5	7.324	7.290	361.0E6	232.3E6	501.501	505.512



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 01:50
Operator : YP/AJ
Sample : PO051525ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO051525

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:39:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:36:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

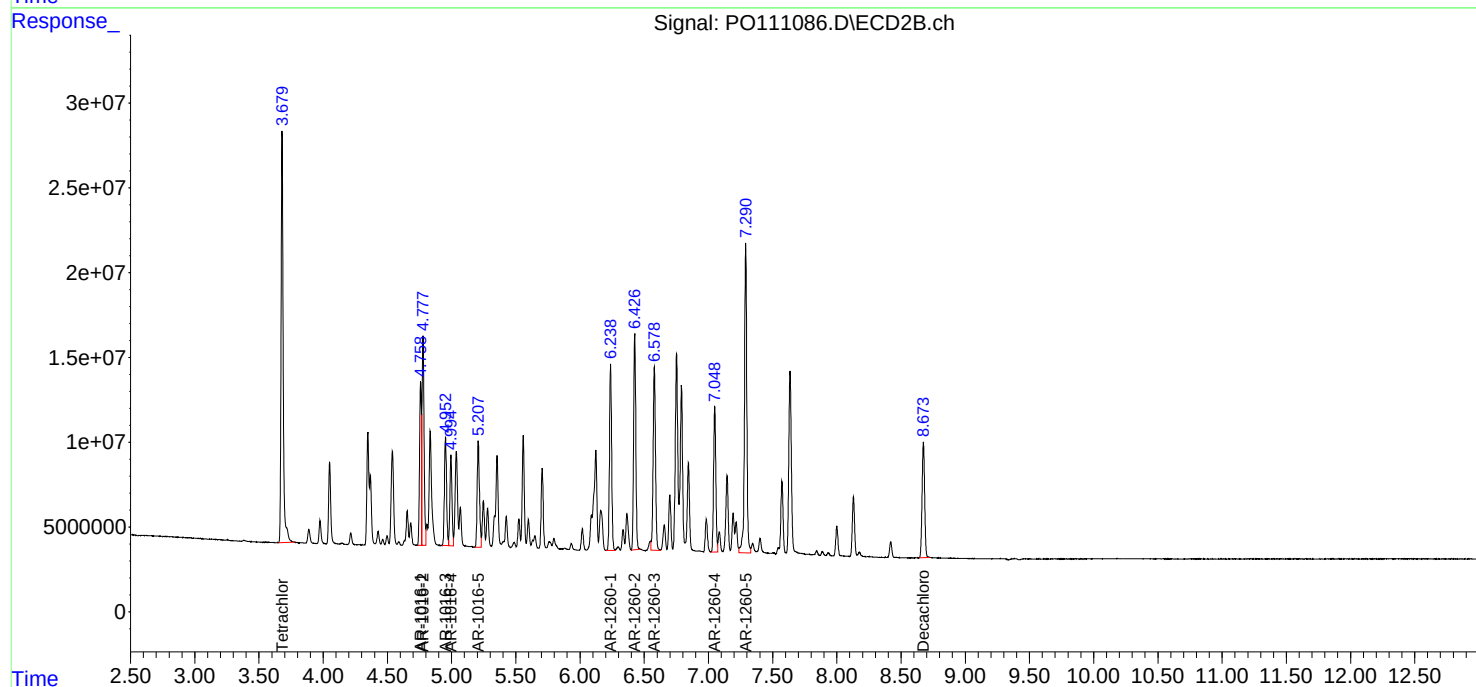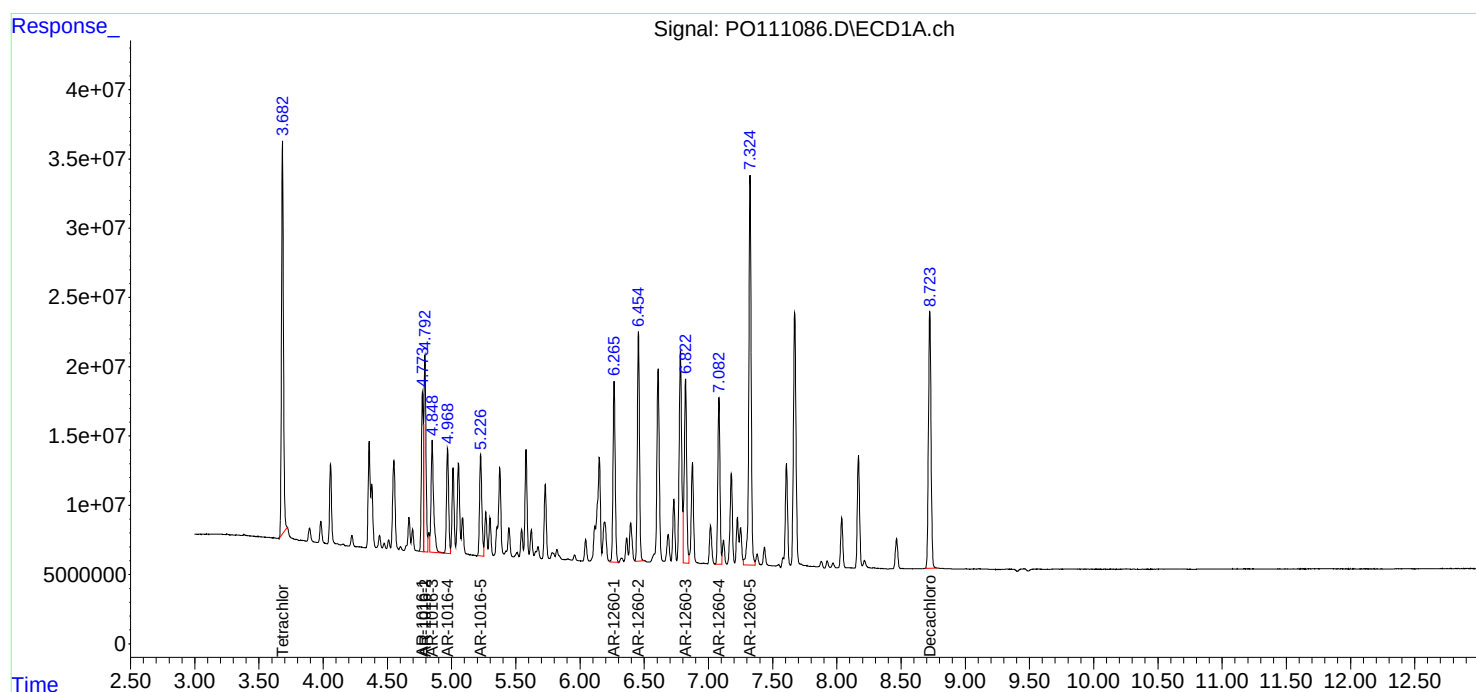

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 02:26
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO051525AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:40:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:36:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	305.8E6	280.9E6	51.973	51.528
2) SA Decachlor...	8.725	8.674	260.0E6	94073353	50.364	50.846
Target Compounds						
16) L4 AR-1242-1	4.773	4.759	100.1E6	82733417	523.282	513.532
17) L4 AR-1242-2	4.792	4.778	140.8E6	120.8E6	517.536	514.803
18) L4 AR-1242-3	4.849	4.953	98004292	64351170	526.942	520.562
19) L4 AR-1242-4	4.969	5.037	77694741	63517417	525.674	513.832
20) L4 AR-1242-5	5.621	5.558	81076986	78206793	521.255	514.564



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 02:26
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO051525AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:40:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:36:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

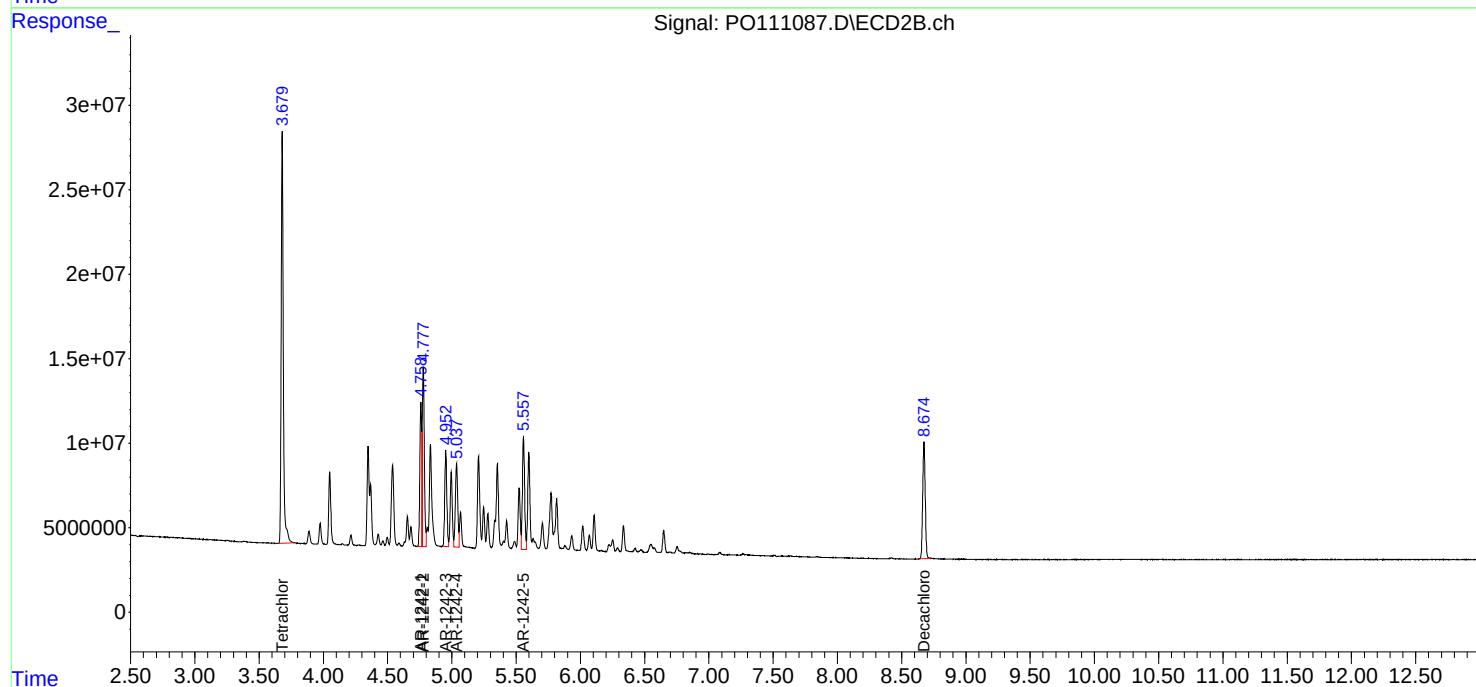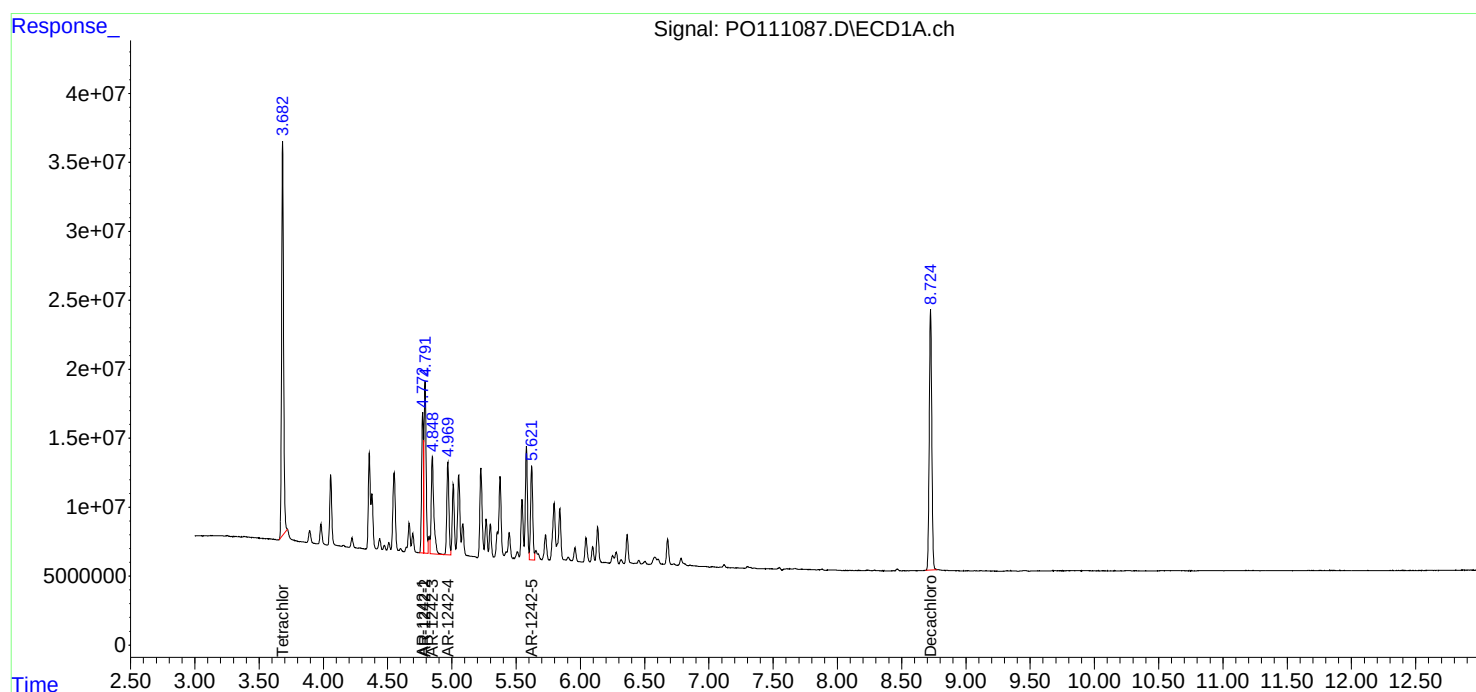

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 03:03
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO051525AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:40:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:36:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.680	302.3E6	269.4E6	51.383	49.416
2) SA Decachlor...	8.725	8.674	257.8E6	92861317	49.936	50.191
Target Compounds						
21) L5 AR-1248-1	4.773	4.758	75013440	61783121	489.753	476.251
22) L5 AR-1248-2	5.012	4.994	98705358	84886979	492.253	482.609
23) L5 AR-1248-3	5.226	5.037	123.6E6	90239307	482.709	480.983
24) L5 AR-1248-4	5.580	5.207	175.1E6	105.4E6	483.415	479.447
25) L5 AR-1248-5	5.622	5.598	126.5E6	105.1E6	482.660	481.511



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 03:03
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO051525AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:40:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:36:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

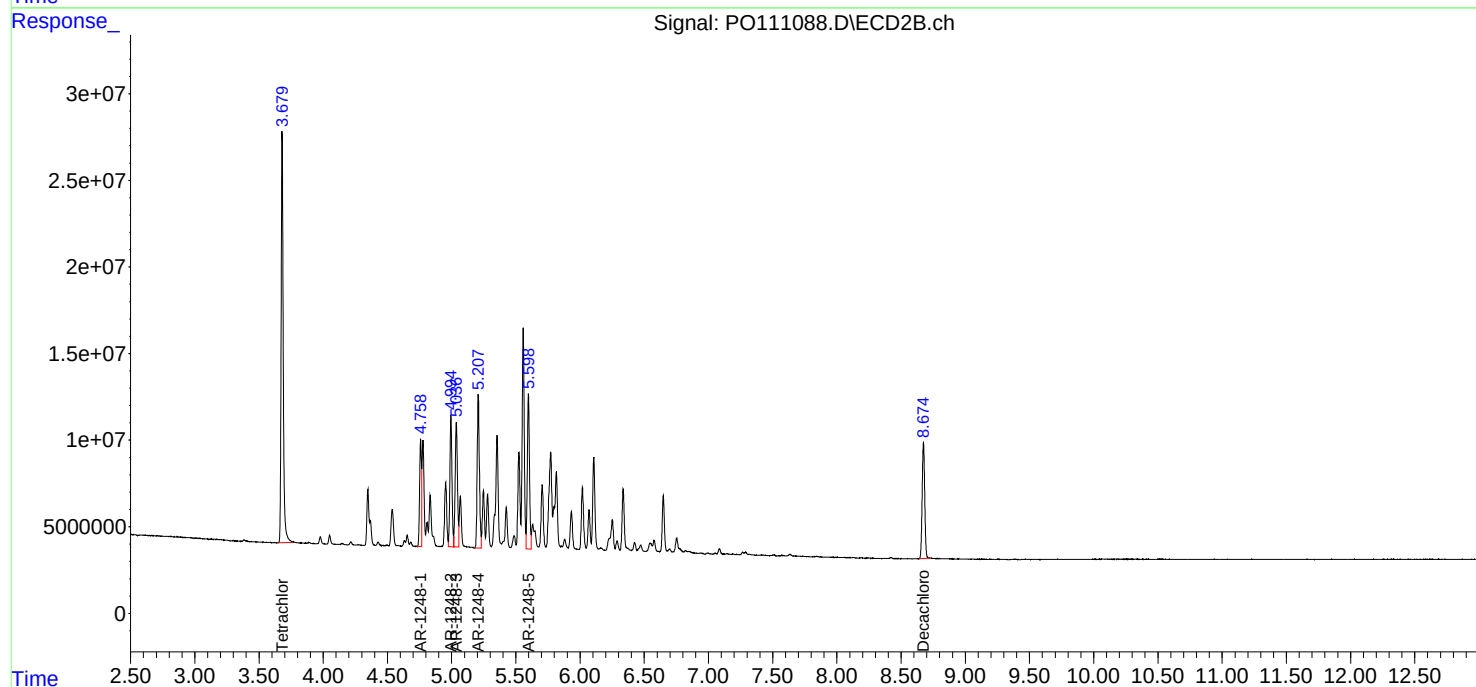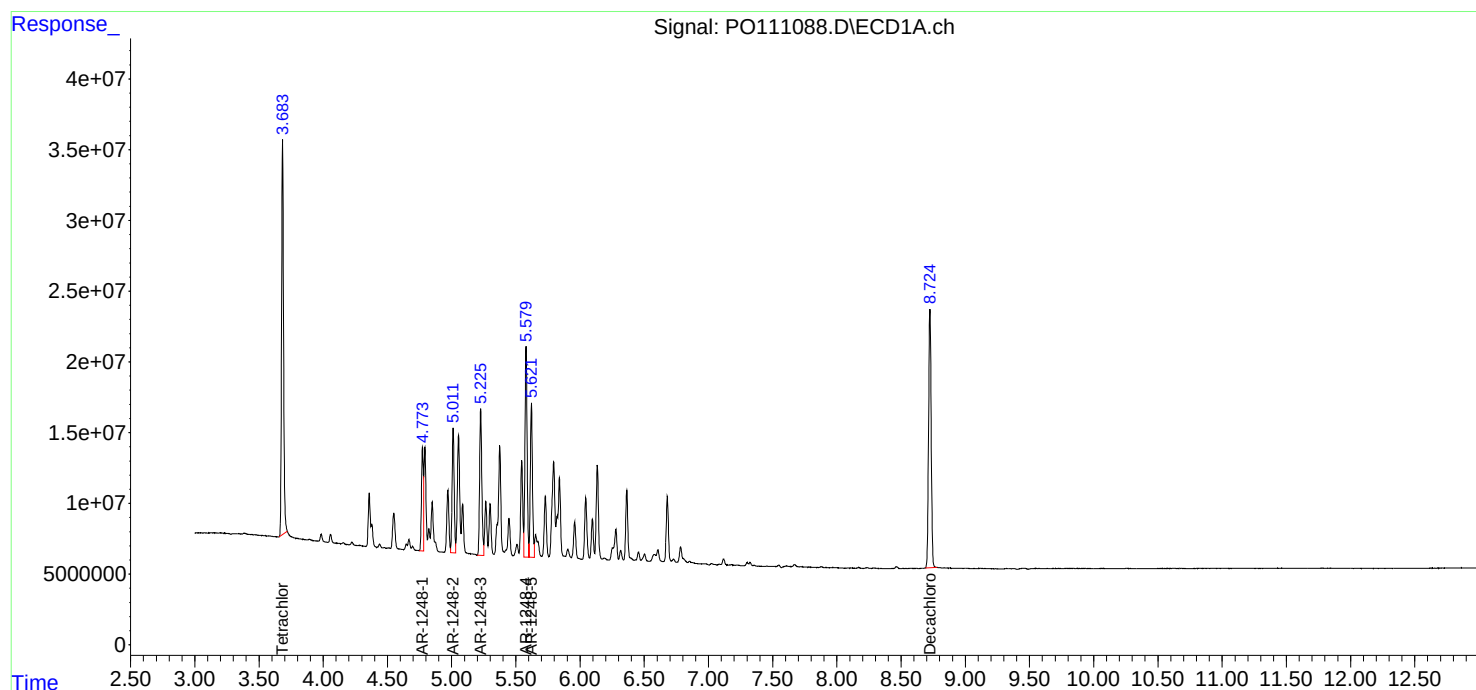

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 03:40
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO051525AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:41:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:36:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	308.9E6	272.7E6	52.510	50.016
2) SA Decachlor...	8.725	8.674	260.1E6	92401602	50.379	49.943
Target Compounds						
26) L6 AR-1254-1	5.581	5.558	183.2E6	154.4E6	482.546	476.507
27) L6 AR-1254-2	5.730	5.706	158.3E6	134.3E6	484.442	474.276
28) L6 AR-1254-3	6.135	6.107	251.9E6	206.7E6	478.753	479.126
29) L6 AR-1254-4	6.365	6.336	160.6E6	118.8E6	477.996	480.225
30) L6 AR-1254-5	6.784	6.753	228.7E6	165.0E6	482.108	477.039



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 03:40
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO051525AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:41:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:36:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

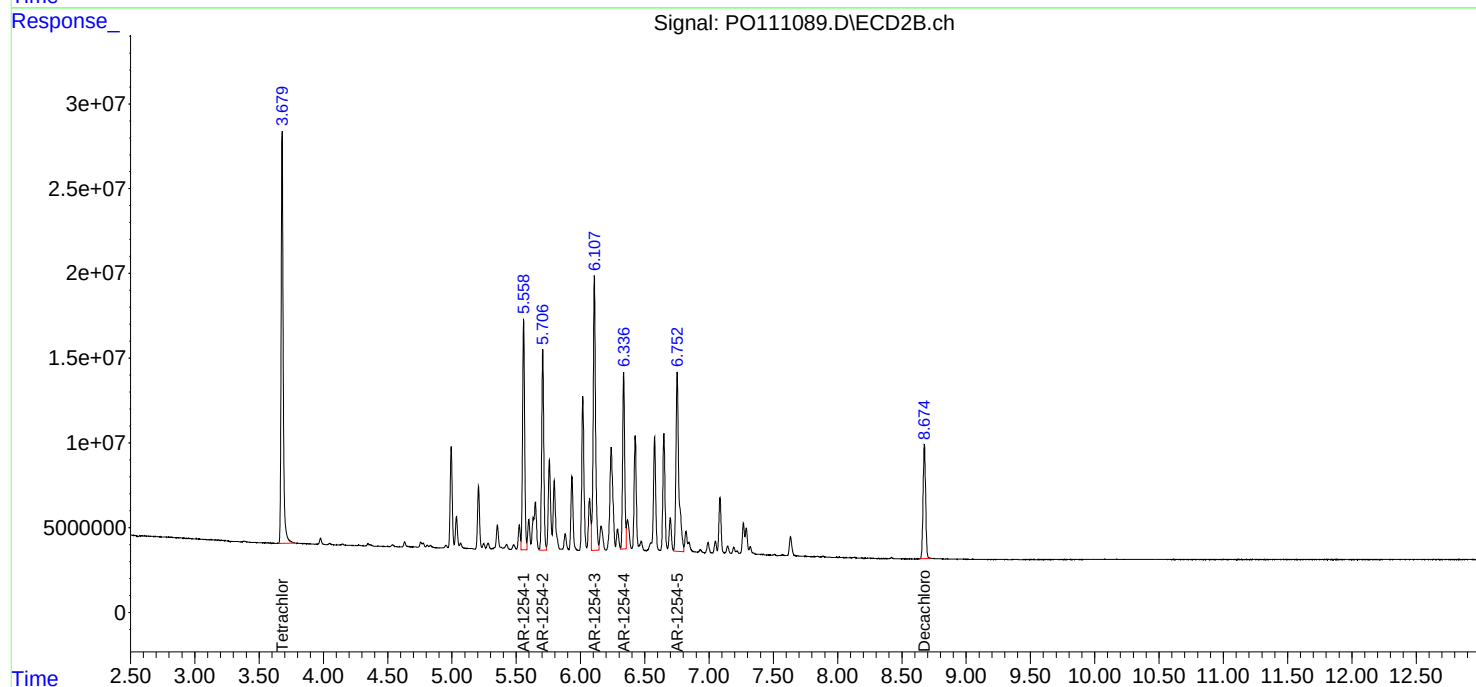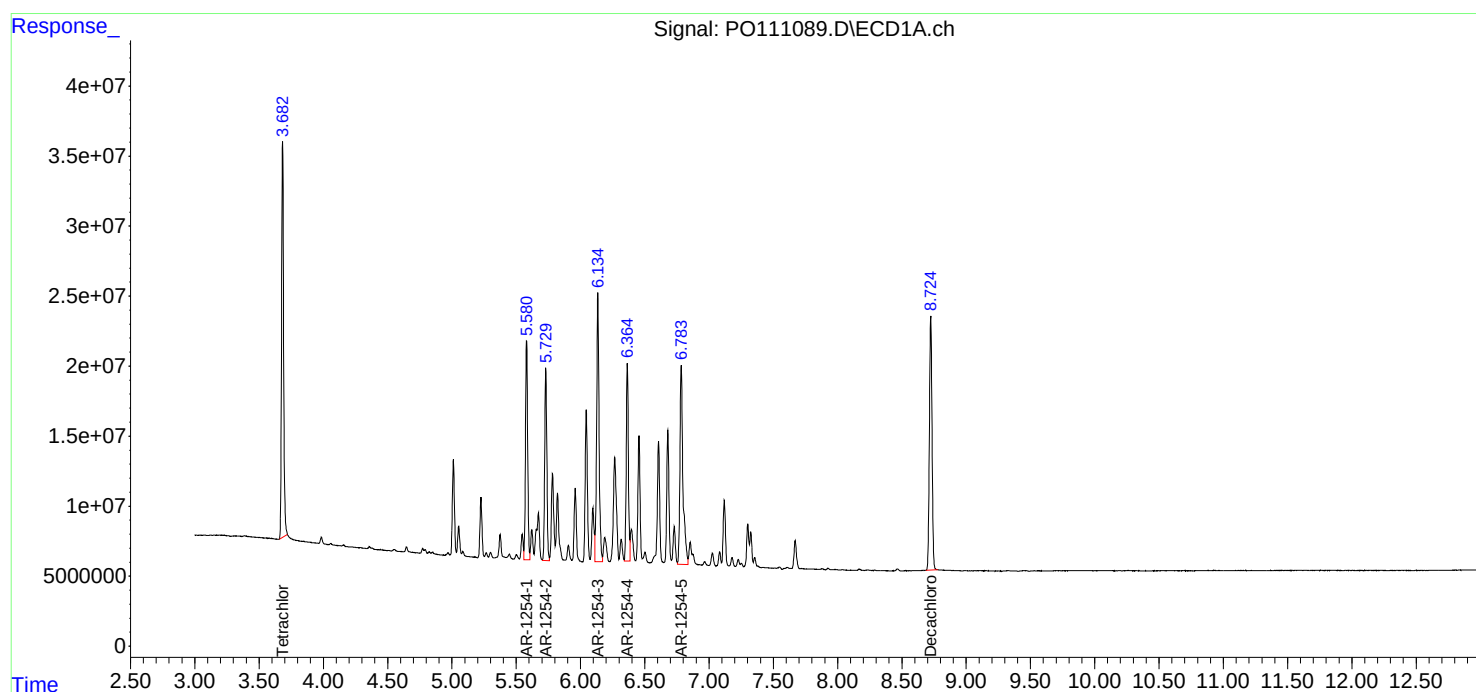

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051525\
 Data File : P0111090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 04:17
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO051525AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 07:05:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:04:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	316.0E6	278.9E6	49.967	49.915
2) SA Decachlor...	8.725	8.674	463.0E6	161.9E6	49.157	50.297
Target Compounds						
41) L9 AR-1268-1	7.610	7.573	483.9E6	268.5E6	499.094	506.477
42) L9 AR-1268-2	7.674	7.638	441.4E6	247.6E6	494.559	513.322
43) L9 AR-1268-3	7.881	7.844	371.8E6	178.9E6	489.927	513.498
44) L9 AR-1268-4	8.170	8.129	162.1E6	67162410	496.415	527.719
45) L9 AR-1268-5	8.466	8.421	1064.0E6	381.5E6	492.966	506.818



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 04:17
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO051525AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 07:05:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:04:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

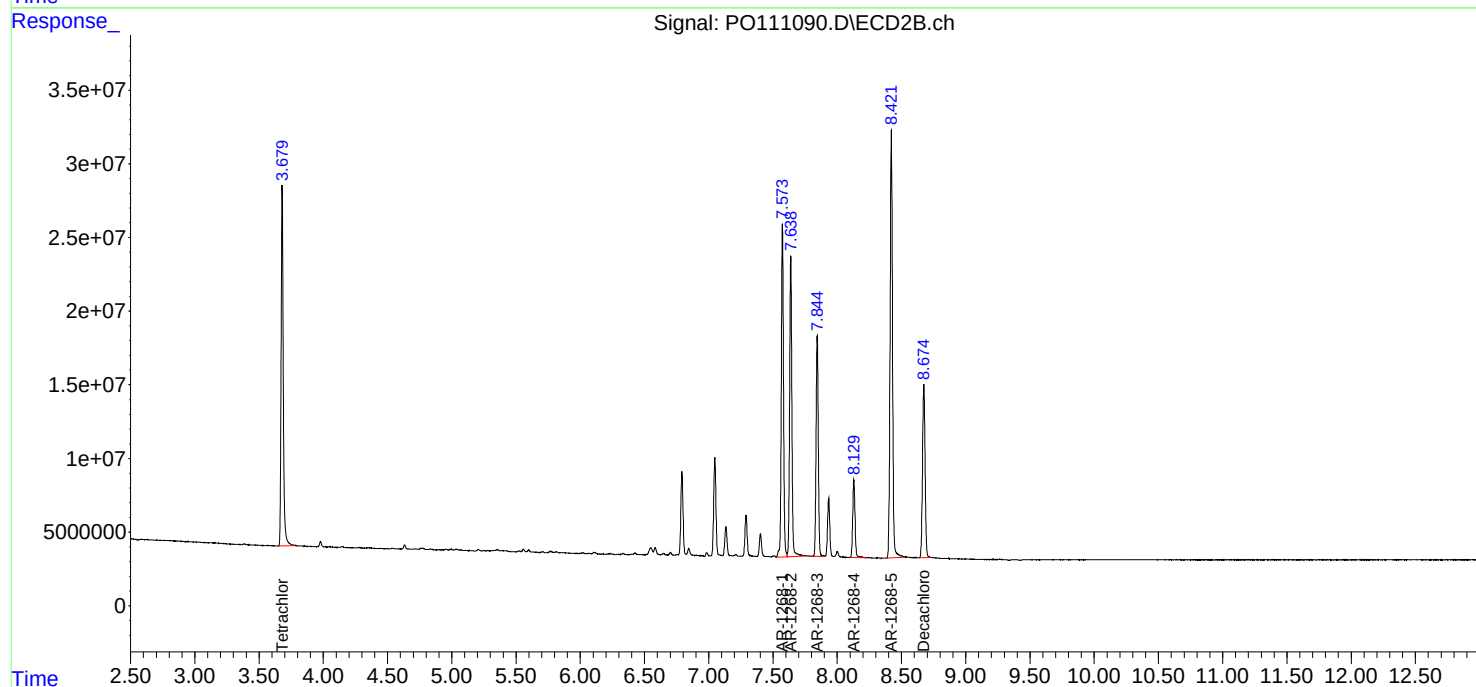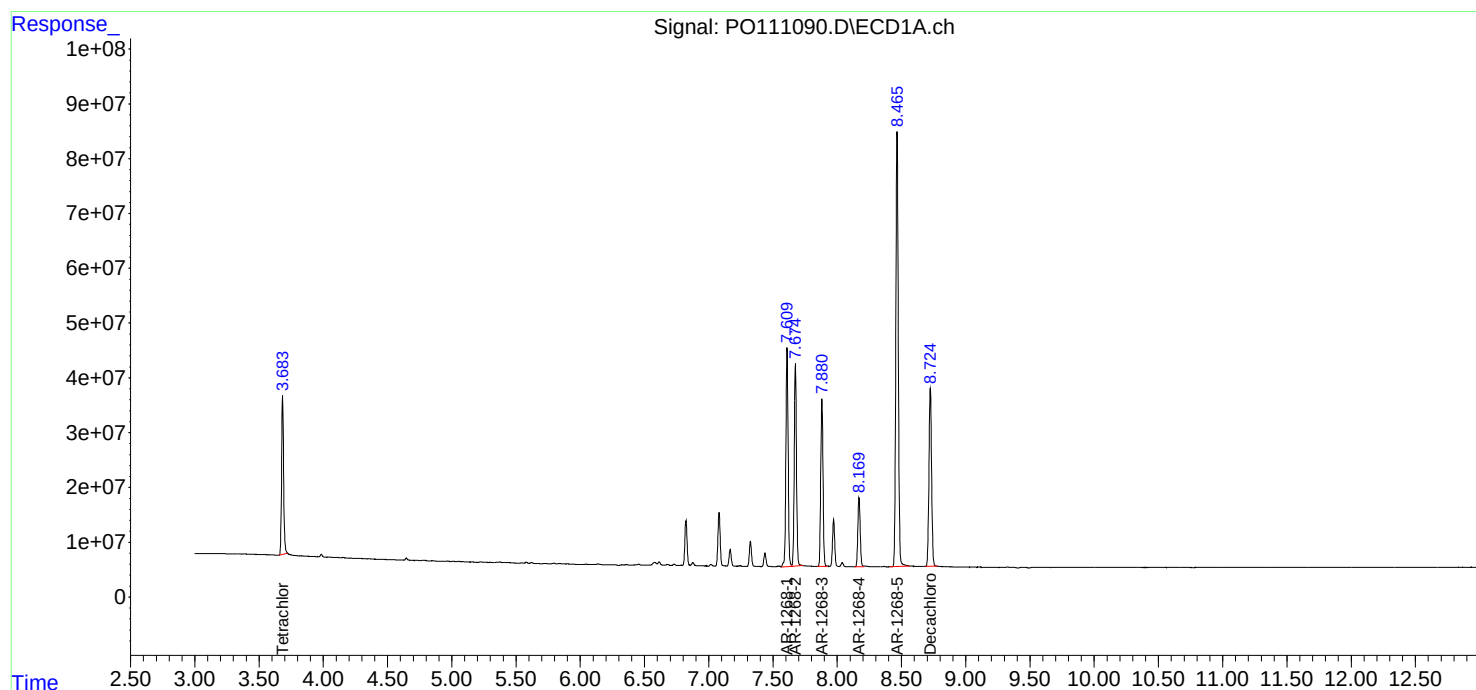



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Continuing Calib Date: 06/10/2025 Initial Calibration Date(s): 05/14/2025 05/15/2025

Continuing Calib Time: 10:26 Initial Calibration Time(s): 17:19 01:31

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.77	4.77	4.67	4.87	0.00
Aroclor-1016-2	(2)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-3	(3)	4.85	4.85	4.75	4.95	0.00
Aroclor-1016-4	(4)	4.97	4.97	4.87	5.07	0.00
Aroclor-1016-5	(5)	5.23	5.23	5.13	5.33	0.00
Aroclor-1260-1	(1)	6.27	6.27	6.17	6.37	0.01
Aroclor-1260-2	(2)	6.46	6.46	6.36	6.56	0.01
Aroclor-1260-3	(3)	6.82	6.82	6.72	6.92	0.00
Aroclor-1260-4	(4)	7.08	7.08	6.98	7.18	0.00
Aroclor-1260-5	(5)	7.33	7.33	7.23	7.43	0.01
Tetrachloro-m-xylene		3.68	3.68	3.58	3.78	0.00
Decachlorobiphenyl		8.72	8.72	8.62	8.82	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Continuing Calib Date: 06/10/2025 Initial Calibration Date(s): 05/14/2025 05/15/2025

Continuing Calib Time: 10:26 Initial Calibration Time(s): 17:19 01:31

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.75	4.76	4.66	4.86	0.01
Aroclor-1016-2	(2)	4.77	4.78	4.68	4.88	0.01
Aroclor-1016-3	(3)	4.95	4.95	4.85	5.05	0.00
Aroclor-1016-4	(4)	4.99	4.99	4.89	5.09	0.00
Aroclor-1016-5	(5)	5.20	5.21	5.11	5.31	0.01
Aroclor-1260-1	(1)	6.23	6.24	6.14	6.34	0.01
Aroclor-1260-2	(2)	6.42	6.43	6.33	6.53	0.01
Aroclor-1260-3	(3)	6.57	6.58	6.48	6.68	0.01
Aroclor-1260-4	(4)	7.04	7.05	6.95	7.15	0.01
Aroclor-1260-5	(5)	7.29	7.29	7.19	7.39	0.01
Tetrachloro-m-xylene		3.68	3.68	3.58	3.78	0.01
Decachlorobiphenyl		8.67	8.67	8.57	8.77	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 05/14/2025 05/14/2025

Client Sample No.: CCAL01 Date Analyzed: 06/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO111569.D Time Analyzed: 10:26

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.773	4.673	4.873	543.730	500.000	8.7
Aroclor-1016-2	4.792	4.692	4.892	544.840	500.000	9.0
Aroclor-1016-3	4.849	4.749	4.949	556.420	500.000	11.3
Aroclor-1016-4	4.968	4.869	5.069	554.460	500.000	10.9
Aroclor-1016-5	5.227	5.126	5.326	561.910	500.000	12.4
Aroclor-1260-1	6.265	6.166	6.366	579.850	500.000	16.0
Aroclor-1260-2	6.455	6.355	6.555	612.830	500.000	22.6
Aroclor-1260-3	6.822	6.722	6.922	607.480	500.000	21.5
Aroclor-1260-4	7.082	6.983	7.183	553.840	500.000	10.8
Aroclor-1260-5	7.325	7.225	7.425	555.070	500.000	11.0
Decachlorobiphenyl	8.724	8.624	8.824	47.480	50.000	-5.0
Tetrachloro-m-xylene	3.684	3.582	3.782	51.920	50.000	3.8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 05/14/2025 05/14/2025

Client Sample No.: CCAL01 Date Analyzed: 06/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO111569.D Time Analyzed: 10:26

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.754	4.658	4.858	486.180	500.000	-2.8
Aroclor-1016-2	4.772	4.677	4.877	497.080	500.000	-0.6
Aroclor-1016-3	4.948	4.852	5.052	496.220	500.000	-0.8
Aroclor-1016-4	4.990	4.894	5.094	492.820	500.000	-1.4
Aroclor-1016-5	5.202	5.107	5.307	489.370	500.000	-2.1
Aroclor-1260-1	6.233	6.138	6.338	492.100	500.000	-1.6
Aroclor-1260-2	6.421	6.326	6.526	493.500	500.000	-1.3
Aroclor-1260-3	6.573	6.479	6.679	456.330	500.000	-8.7
Aroclor-1260-4	7.044	6.949	7.149	473.200	500.000	-5.4
Aroclor-1260-5	7.285	7.191	7.391	468.180	500.000	-6.4
Decachlorobiphenyl	8.668	8.574	8.774	44.690	50.000	-10.6
Tetrachloro-m-xylene	3.675	3.579	3.779	50.650	50.000	1.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
 Data File : PO111569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 10:26
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:25:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.684	3.675	305.5E6	276.1E6	51.921	50.648
2) SA Decachlor...	8.724	8.668	245.1E6	82690658	47.481	44.694
Target Compounds						
3) L1 AR-1016-1	4.773	4.754	122.4E6	92824944	543.725	486.180
4) L1 AR-1016-2	4.792	4.772	173.8E6	137.8E6	544.837	497.080
5) L1 AR-1016-3	4.849	4.948	120.8E6	72485784	556.423	496.223
6) L1 AR-1016-4	4.968	4.990	96558857	59182238	554.464	492.821
7) L1 AR-1016-5	5.227	5.202	98892152	75559314	561.915	489.373
31) L7 AR-1260-1	6.265	6.233	176.8E6	123.0E6	579.855	492.097
32) L7 AR-1260-2	6.455	6.421	234.7E6	145.2E6	612.833	493.501
33) L7 AR-1260-3	6.822	6.573	211.8E6	130.8E6	607.482	456.330
34) L7 AR-1260-4	7.082	7.044	155.1E6	95002105	553.843	473.204
35) L7 AR-1260-5	7.325	7.285	399.6E6	215.2E6	555.068	468.180



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 10:26
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:25:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

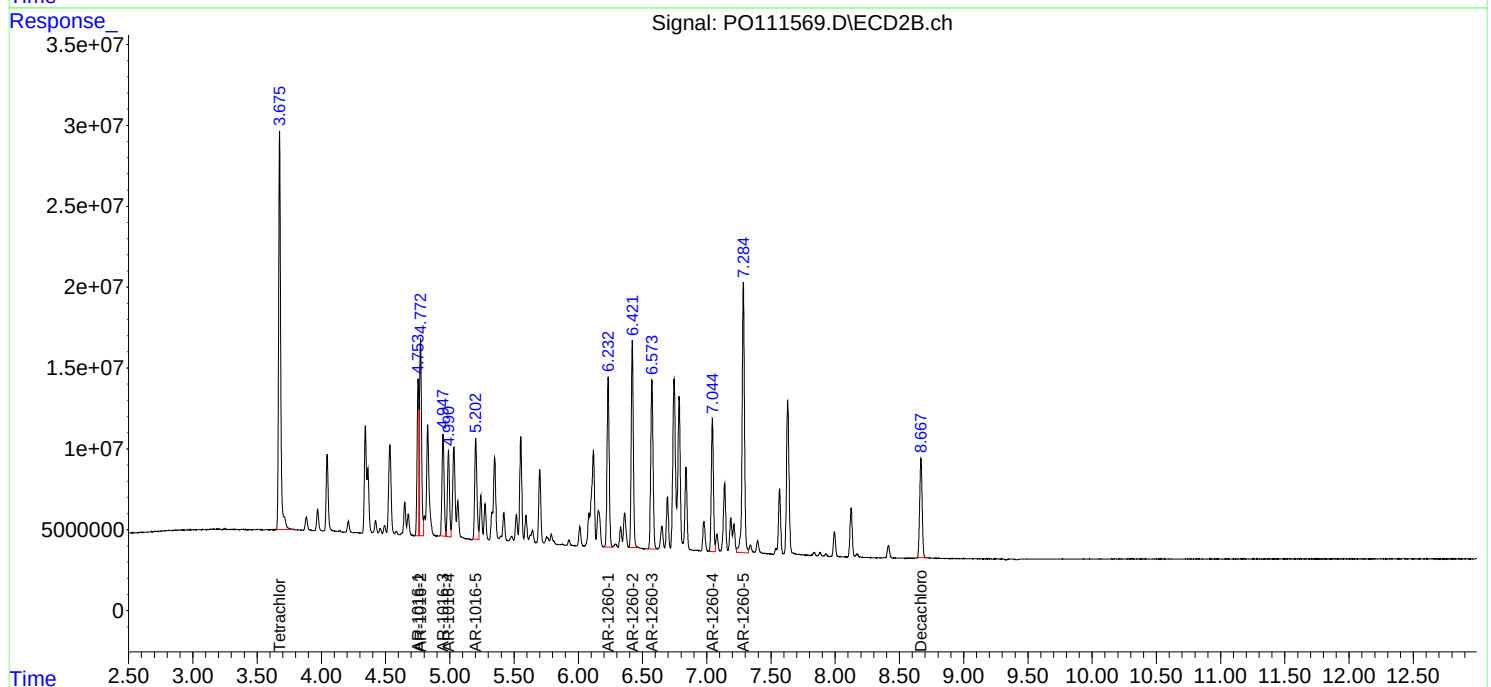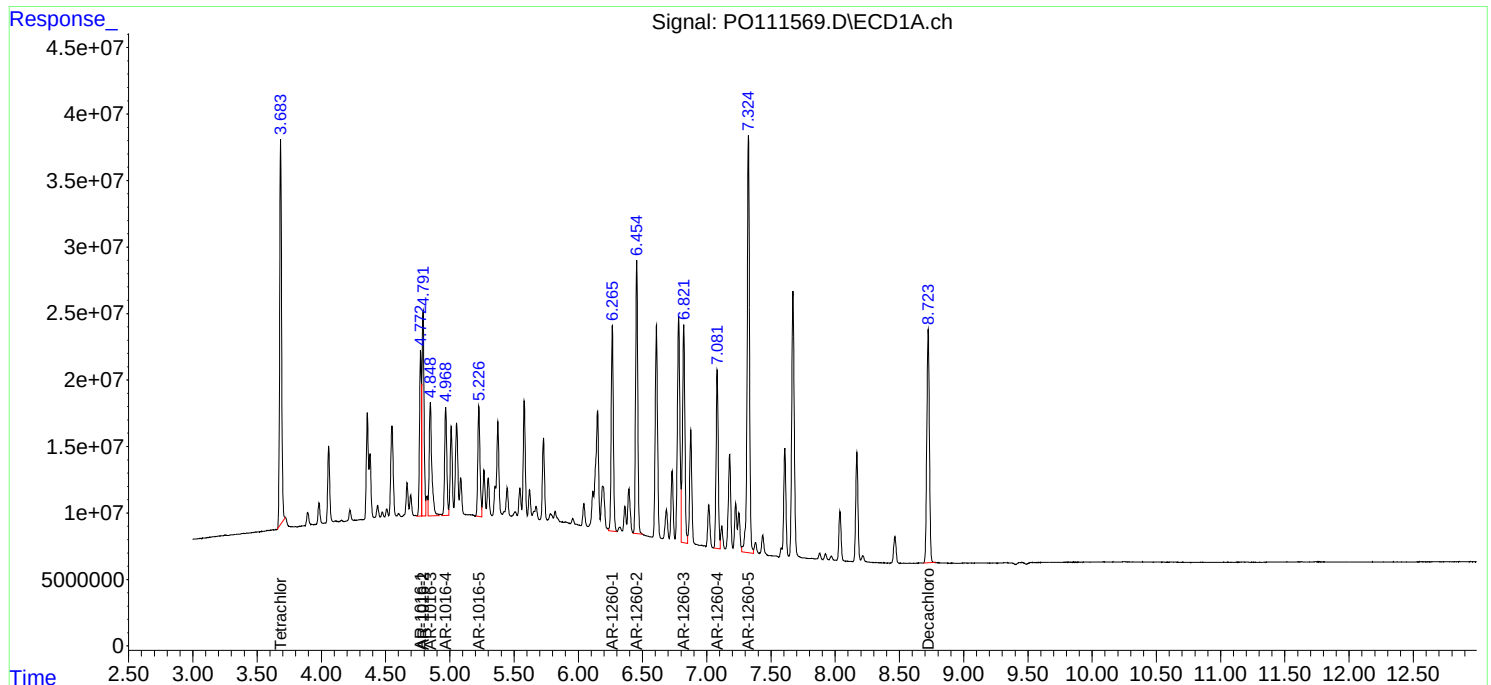



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Continuing Calib Date: 06/10/2025 Initial Calibration Date(s): 05/14/2025 05/15/2025

Continuing Calib Time: 17:04 Initial Calibration Time(s): 17:19 01:31

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.77	4.77	4.67	4.87	0.01
Aroclor-1016-2	(2)	4.78	4.79	4.69	4.89	0.01
Aroclor-1016-3	(3)	4.84	4.85	4.75	4.95	0.01
Aroclor-1016-4	(4)	4.96	4.97	4.87	5.07	0.01
Aroclor-1016-5	(5)	5.22	5.23	5.13	5.33	0.01
Aroclor-1260-1	(1)	6.26	6.27	6.17	6.37	0.01
Aroclor-1260-2	(2)	6.45	6.46	6.36	6.56	0.01
Aroclor-1260-3	(3)	6.81	6.82	6.72	6.92	0.01
Aroclor-1260-4	(4)	7.07	7.08	6.98	7.18	0.01
Aroclor-1260-5	(5)	7.32	7.33	7.23	7.43	0.01
Tetrachloro-m-xylene		3.68	3.68	3.58	3.78	0.00
Decachlorobiphenyl		8.71	8.72	8.62	8.82	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Continuing Calib Date: 06/10/2025 Initial Calibration Date(s): 05/14/2025 05/15/2025

Continuing Calib Time: 17:04 Initial Calibration Time(s): 17:19 01:31

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.75	4.76	4.66	4.86	0.01
Aroclor-1016-2	(2)	4.77	4.78	4.68	4.88	0.01
Aroclor-1016-3	(3)	4.95	4.95	4.85	5.05	0.00
Aroclor-1016-4	(4)	4.99	4.99	4.89	5.09	0.00
Aroclor-1016-5	(5)	5.20	5.21	5.11	5.31	0.01
Aroclor-1260-1	(1)	6.23	6.24	6.14	6.34	0.01
Aroclor-1260-2	(2)	6.42	6.43	6.33	6.53	0.01
Aroclor-1260-3	(3)	6.57	6.58	6.48	6.68	0.01
Aroclor-1260-4	(4)	7.04	7.05	6.95	7.15	0.01
Aroclor-1260-5	(5)	7.28	7.29	7.19	7.39	0.01
Tetrachloro-m-xylene		3.68	3.68	3.58	3.78	0.01
Decachlorobiphenyl		8.66	8.67	8.57	8.77	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 05/14/2025 05/14/2025

Client Sample No.: CCAL02 Date Analyzed: 06/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO111580.D Time Analyzed: 17:04

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.765	4.673	4.873	533.610	500.000	6.7
Aroclor-1016-2	4.784	4.692	4.892	537.930	500.000	7.6
Aroclor-1016-3	4.841	4.749	4.949	542.340	500.000	8.5
Aroclor-1016-4	4.960	4.869	5.069	545.430	500.000	9.1
Aroclor-1016-5	5.217	5.126	5.326	567.340	500.000	13.5
Aroclor-1260-1	6.256	6.166	6.366	588.500	500.000	17.7
Aroclor-1260-2	6.446	6.355	6.555	611.860	500.000	22.4
Aroclor-1260-3	6.813	6.722	6.922	603.330	500.000	20.7
Aroclor-1260-4	7.072	6.983	7.183	552.320	500.000	10.5
Aroclor-1260-5	7.315	7.225	7.425	559.270	500.000	11.9
Decachlorobiphenyl	8.712	8.624	8.824	47.210	50.000	-5.6
Tetrachloro-m-xylene	3.677	3.582	3.782	50.760	50.000	1.5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 05/14/2025 05/14/2025

Client Sample No.: CCAL02 Date Analyzed: 06/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO111580.D Time Analyzed: 17:04

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.753	4.658	4.858	499.890	500.000	0.0
Aroclor-1016-2	4.771	4.677	4.877	501.590	500.000	0.3
Aroclor-1016-3	4.946	4.852	5.052	495.710	500.000	-0.9
Aroclor-1016-4	4.989	4.894	5.094	459.850	500.000	-8.0
Aroclor-1016-5	5.201	5.107	5.307	501.140	500.000	0.2
Aroclor-1260-1	6.230	6.138	6.338	491.800	500.000	-1.6
Aroclor-1260-2	6.419	6.326	6.526	491.220	500.000	-1.8
Aroclor-1260-3	6.570	6.479	6.679	452.850	500.000	-9.4
Aroclor-1260-4	7.041	6.949	7.149	459.980	500.000	-8.0
Aroclor-1260-5	7.282	7.191	7.391	449.980	500.000	-10.0
Decachlorobiphenyl	8.663	8.574	8.774	44.710	50.000	-10.6
Tetrachloro-m-xylene	3.675	3.579	3.779	51.630	50.000	3.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
 Data File : PO111580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 17:04
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/11/2025
 Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:28:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.677	3.675	298.7E6	281.5E6	50.765	51.634
2) SA Decachlor...	8.712	8.663	243.7E6	82720318	47.207m	44.710m
Target Compounds						
3) L1 AR-1016-1	4.765	4.753	120.1E6	95443410	533.614	499.894
4) L1 AR-1016-2	4.784	4.771	171.6E6	139.0E6	537.931	501.591
5) L1 AR-1016-3	4.841	4.946	117.8E6	72410641	542.341	495.709
6) L1 AR-1016-4	4.960	4.989	94985053	55222320	545.427	459.846
7) L1 AR-1016-5	5.217	5.201	99847287	77375955	567.342m	501.138
31) L7 AR-1260-1	6.256	6.230	179.5E6	122.9E6	588.499	491.798
32) L7 AR-1260-2	6.446	6.419	234.3E6	144.6E6	611.860	491.220
33) L7 AR-1260-3	6.813	6.570	210.3E6	129.8E6	603.333	452.854
34) L7 AR-1260-4	7.072	7.041	154.6E6	92347349	552.324	459.981
35) L7 AR-1260-5	7.315	7.282	402.6E6	206.8E6	559.272	449.978

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 17:04
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

AR1660CCC500

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 06/11/2025

Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:28:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

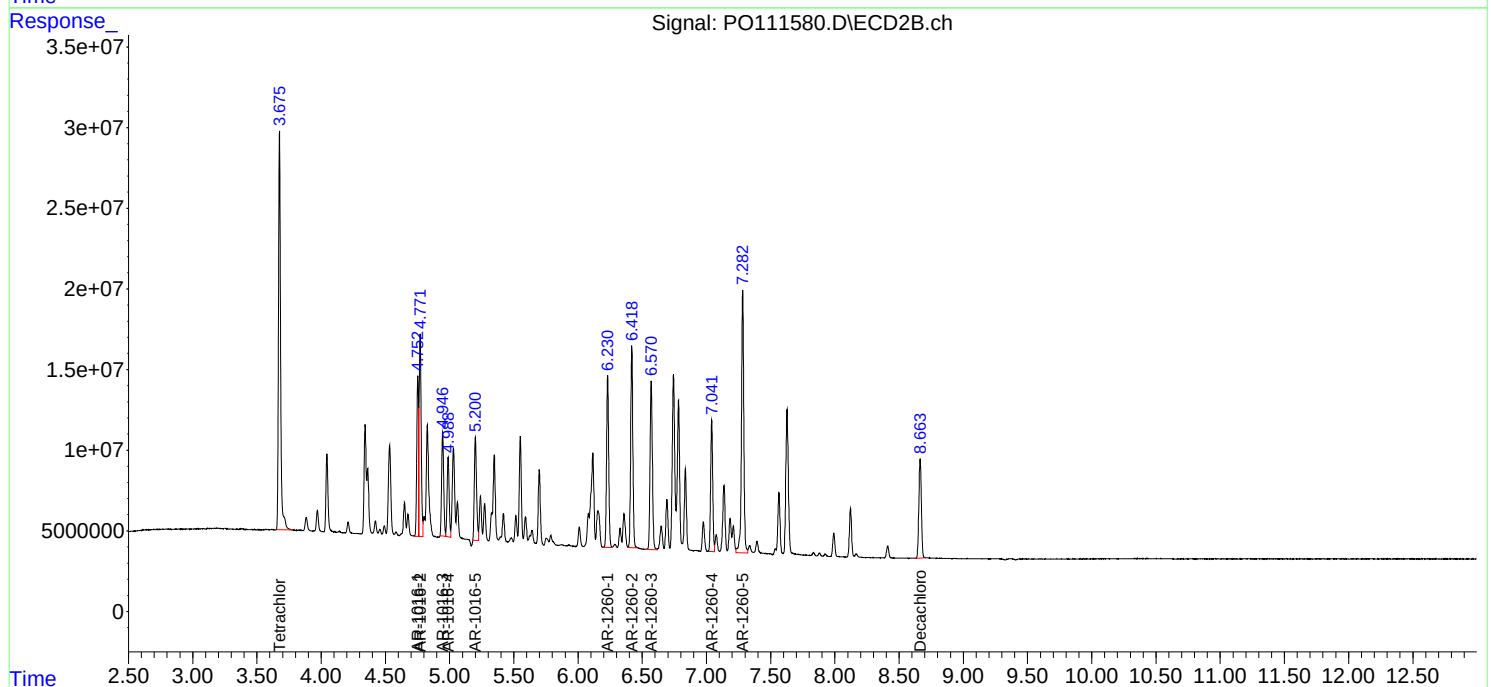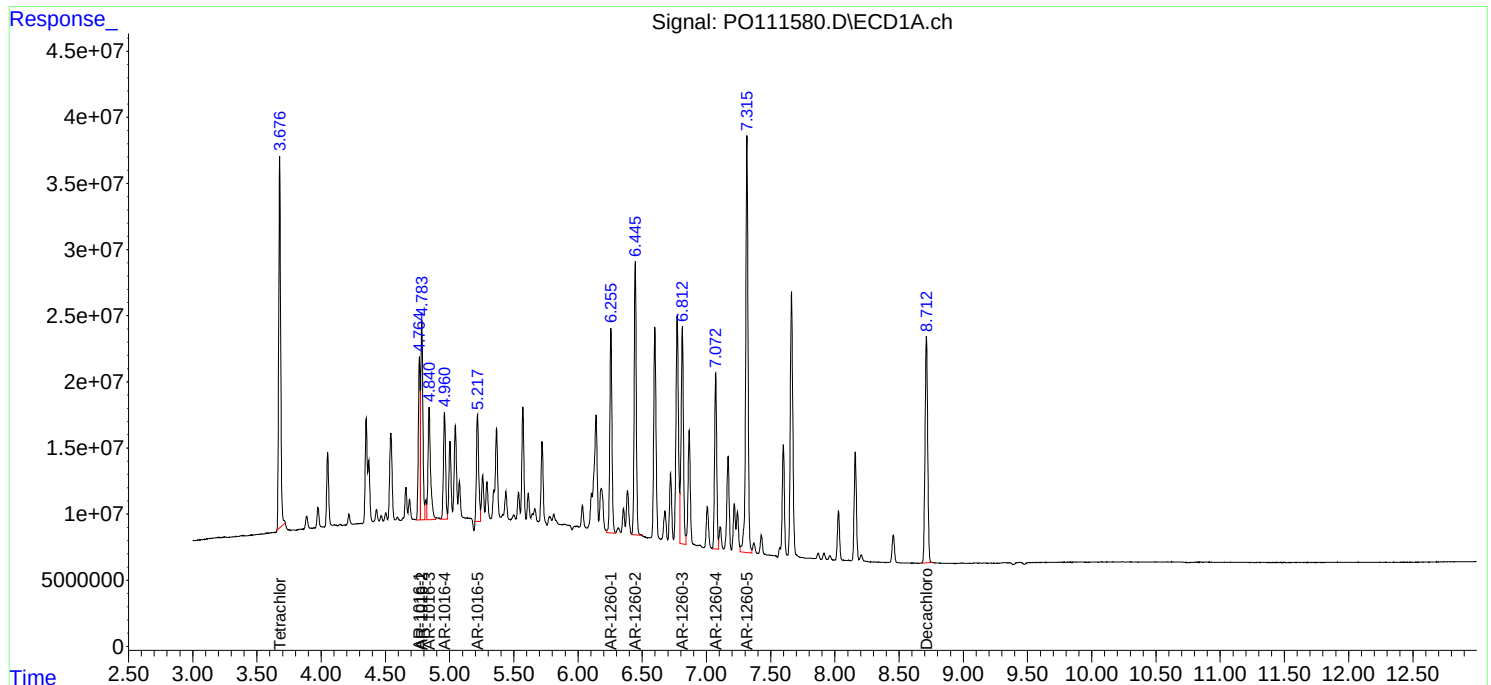

Analytical Sequence

Client: PARSONS Engineering of New York, Inc.	SDG No.: Q2267
Project: Con Ed Non MGP – Atlantic Ave 453957.600	Instrument ID: ECD_O
GC Column: ZB-MR1	ID: 0.32 (mm) Inst. Calib. Date(s): 05/14/2025 05/14/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	05/14/2025	17:01	PO111057.D	8.72	3.68
AR1660ICC1000	AR1660ICC1000	05/14/2025	17:19	PO111058.D	8.73	3.68
AR1660ICC750	AR1660ICC750	05/14/2025	17:38	PO111059.D	8.73	3.68
AR1660ICC500	AR1660ICC500	05/14/2025	17:56	PO111060.D	8.72	3.68
AR1660ICC250	AR1660ICC250	05/14/2025	18:15	PO111061.D	8.72	3.68
AR1660ICC050	AR1660ICC050	05/14/2025	18:33	PO111062.D	8.72	3.68
AR1221ICC500	AR1221ICC500	05/14/2025	18:51	PO111063.D	8.72	3.68
AR1232ICC500	AR1232ICC500	05/14/2025	19:10	PO111064.D	8.72	3.68
AR1242ICC1000	AR1242ICC1000	05/14/2025	19:28	PO111065.D	8.72	3.68
AR1242ICC750	AR1242ICC750	05/14/2025	19:46	PO111066.D	8.72	3.68
AR1242ICC500	AR1242ICC500	05/14/2025	20:05	PO111067.D	8.73	3.68
AR1242ICC250	AR1242ICC250	05/14/2025	20:23	PO111068.D	8.72	3.68
AR1242ICC050	AR1242ICC050	05/14/2025	20:41	PO111069.D	8.72	3.68
AR1248ICC1000	AR1248ICC1000	05/14/2025	21:00	PO111070.D	8.72	3.68
AR1248ICC750	AR1248ICC750	05/14/2025	21:18	PO111071.D	8.72	3.68
AR1248ICC500	AR1248ICC500	05/14/2025	21:37	PO111072.D	8.72	3.68
AR1248ICC250	AR1248ICC250	05/14/2025	21:54	PO111073.D	8.72	3.68
AR1248ICC050	AR1248ICC050	05/14/2025	22:12	PO111074.D	8.72	3.68
AR1254ICC1000	AR1254ICC1000	05/14/2025	22:31	PO111075.D	8.73	3.68
AR1254ICC750	AR1254ICC750	05/14/2025	22:49	PO111076.D	8.73	3.68
AR1254ICC500	AR1254ICC500	05/14/2025	23:06	PO111077.D	8.72	3.68
AR1254ICC250	AR1254ICC250	05/14/2025	23:25	PO111078.D	8.72	3.68
AR1254ICC050	AR1254ICC050	05/14/2025	23:43	PO111079.D	8.72	3.68
AR1262ICC500	AR1262ICC500	05/15/2025	00:01	PO111080.D	8.73	3.68
AR1268ICC1000	AR1268ICC1000	05/15/2025	00:19	PO111081.D	8.72	3.68
AR1268ICC750	AR1268ICC750	05/15/2025	00:37	PO111082.D	8.72	3.68
AR1268ICC500	AR1268ICC500	05/15/2025	00:56	PO111083.D	8.73	3.68
AR1268ICC250	AR1268ICC250	05/15/2025	01:14	PO111084.D	8.72	3.68
AR1268ICC050	AR1268ICC050	05/15/2025	01:31	PO111085.D	8.72	3.68
AR1660CCC500	AR1660CCC500	06/10/2025	10:26	PO111569.D	8.72	3.68
IBLK	IBLK	06/10/2025	11:39	PO111573.D	8.72	3.68
PB168377BL	PB168377BL	06/10/2025	14:28	PO111574.D	8.72	3.68
PB168377BS	PB168377BS	06/10/2025	14:47	PO111575.D	8.72	3.68
PB168377BSD	PB168377BSD	06/10/2025	15:05	PO111576.D	8.72	3.68
WC-20250605	Q2267-01	06/10/2025	16:00	PO111579.D	8.71	3.68
AR1660CCC500	AR1660CCC500	06/10/2025	17:04	PO111580.D	8.71	3.68
IBLK	IBLK	06/10/2025	18:32	PO111584.D	8.71	3.68

Analytical Sequence

Client: PARSONS Engineering of New York, Inc.	SDG No.: Q2267
Project: Con Ed Non MGP – Atlantic Ave 453957.600	Instrument ID: ECD_O
GC Column: ZB-MR2	ID: 0.32 (mm) Inst. Calib. Date(s): 05/14/2025 05/14/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	05/14/2025	17:01	PO111057.D	8.67	3.68
AR1660ICC1000	AR1660ICC1000	05/14/2025	17:19	PO111058.D	8.67	3.68
AR1660ICC750	AR1660ICC750	05/14/2025	17:38	PO111059.D	8.67	3.68
AR1660ICC500	AR1660ICC500	05/14/2025	17:56	PO111060.D	8.67	3.68
AR1660ICC250	AR1660ICC250	05/14/2025	18:15	PO111061.D	8.68	3.68
AR1660ICC050	AR1660ICC050	05/14/2025	18:33	PO111062.D	8.67	3.68
AR1221ICC500	AR1221ICC500	05/14/2025	18:51	PO111063.D	8.67	3.68
AR1232ICC500	AR1232ICC500	05/14/2025	19:10	PO111064.D	8.68	3.68
AR1242ICC1000	AR1242ICC1000	05/14/2025	19:28	PO111065.D	8.67	3.68
AR1242ICC750	AR1242ICC750	05/14/2025	19:46	PO111066.D	8.67	3.68
AR1242ICC500	AR1242ICC500	05/14/2025	20:05	PO111067.D	8.67	3.68
AR1242ICC250	AR1242ICC250	05/14/2025	20:23	PO111068.D	8.67	3.68
AR1242ICC050	AR1242ICC050	05/14/2025	20:41	PO111069.D	8.67	3.68
AR1248ICC1000	AR1248ICC1000	05/14/2025	21:00	PO111070.D	8.67	3.68
AR1248ICC750	AR1248ICC750	05/14/2025	21:18	PO111071.D	8.67	3.68
AR1248ICC500	AR1248ICC500	05/14/2025	21:37	PO111072.D	8.68	3.68
AR1248ICC250	AR1248ICC250	05/14/2025	21:54	PO111073.D	8.69	3.69
AR1248ICC050	AR1248ICC050	05/14/2025	22:12	PO111074.D	8.67	3.68
AR1254ICC1000	AR1254ICC1000	05/14/2025	22:31	PO111075.D	8.67	3.68
AR1254ICC750	AR1254ICC750	05/14/2025	22:49	PO111076.D	8.67	3.68
AR1254ICC500	AR1254ICC500	05/14/2025	23:06	PO111077.D	8.67	3.68
AR1254ICC250	AR1254ICC250	05/14/2025	23:25	PO111078.D	8.67	3.68
AR1254ICC050	AR1254ICC050	05/14/2025	23:43	PO111079.D	8.67	3.68
AR1262ICC500	AR1262ICC500	05/15/2025	00:01	PO111080.D	8.67	3.68
AR1268ICC1000	AR1268ICC1000	05/15/2025	00:19	PO111081.D	8.67	3.68
AR1268ICC750	AR1268ICC750	05/15/2025	00:37	PO111082.D	8.67	3.68
AR1268ICC500	AR1268ICC500	05/15/2025	00:56	PO111083.D	8.67	3.68
AR1268ICC250	AR1268ICC250	05/15/2025	01:14	PO111084.D	8.67	3.68
AR1268ICC050	AR1268ICC050	05/15/2025	01:31	PO111085.D	8.67	3.68
AR1660CCC500	AR1660CCC500	06/10/2025	10:26	PO111569.D	8.67	3.68
IBLK	IBLK	06/10/2025	11:39	PO111573.D	8.67	3.68
PB168377BL	PB168377BL	06/10/2025	14:28	PO111574.D	8.66	3.67
PB168377BS	PB168377BS	06/10/2025	14:47	PO111575.D	8.66	3.68
PB168377BSD	PB168377BSD	06/10/2025	15:05	PO111576.D	8.67	3.68
WC-20250605	Q2267-01	06/10/2025	16:00	PO111579.D	8.66	3.68
AR1660CCC500	AR1660CCC500	06/10/2025	17:04	PO111580.D	8.66	3.68
IBLK	IBLK	06/10/2025	18:32	PO111584.D	8.67	3.68

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB168377BS

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Lab Sample ID: PB168377BS Date(s) Analyzed: 06/10/2025 06/10/2025

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO111575.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.767	4.717	4.817	4.72	4.70	11.24
COLUMN 1	2	4.786	4.736	4.836	4.78		
	3	4.843	4.793	4.893	4.74		
	4	4.963	4.913	5.013	4.76		
	5	5.22	5.17	5.27	4.60		
	1	4.753	4.703	4.803	4.20		
COLUMN 2	2	4.771	4.721	4.821	4.24	4.20	
	3	4.946	4.896	4.996	4.18		
	4	4.988	4.938	5.038	4.20		
	5	5.201	5.151	5.251	4.08		
Aroclor-1260	1	6.259	6.209	6.309	5.45	5.00	22.22
COLUMN 1	2	6.449	6.399	6.499	5.67		
	3	6.816	6.766	6.866	4.76		
	4	7.076	7.026	7.126	4.61		
	5	7.319	7.269	7.369	4.50		
	1	6.231	6.181	6.281	4.41		
COLUMN 2	2	6.419	6.369	6.469	4.38	4.00	
	3	6.571	6.521	6.621	4.08		
	4	7.041	6.991	7.091	3.71		
	5	7.283	7.233	7.333	3.58		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB168377BSD

Contract: PARS02

Lab Code: CHEM Case No.: Q2267 SAS No.: Q2267 SDG NO.: Q2267

Lab Sample ID: PB168377BSD Date(s) Analyzed: 06/10/2025 06/10/2025

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO111576.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD	
			FROM	TO				
Aroclor-1016	1	4.768	4.718	4.818	4.88	4.90		
	2	4.787	4.737	4.837	4.89			
	3	4.843	4.793	4.893	4.97			
	4	4.964	4.914	5.014	4.94			
	5	5.22	5.17	5.27	4.67			
COLUMN 1								
	1	4.753	4.703	4.803	4.30	4.30		
	2	4.771	4.721	4.821	4.36			
	3	4.946	4.896	4.996	4.27			
	4	4.989	4.939	5.039	4.29			
5	5.201	5.151	5.251	4.16				
COLUMN 2							13.04	
Aroclor-1260	1	6.26	6.21	6.31	5.52	5.10		
	2	6.449	6.399	6.499	5.70			
	3	6.816	6.766	6.866	4.79			
	4	7.076	7.026	7.126	4.65			
	5	7.319	7.269	7.369	4.58			
COLUMN 1								
	1	6.231	6.181	6.281	4.51	4.10		
	2	6.42	6.37	6.47	4.47			
	3	6.572	6.522	6.622	4.14			
	4	7.042	6.992	7.092	3.81			
5	7.283	7.233	7.333	3.64				
COLUMN 2							21.74	



QC SAMPLE DATA

Report of Analysis

Client:	PARSONS Engineering of New York, Inc.		Date Collected:		
Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05		Date Received:		
Client Sample ID:	PB168377BL		SDG No.:	Q2267	
Lab Sample ID:	PB168377BL		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO111574.D	1	06/10/25 09:00	06/10/25 14:28	PB168377

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	23.5		30 - 173	118%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.1		10 - 173	111%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
 Data File : PO111574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 14:28
 Operator : YP/AJ
 Sample : PB168377BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB168377BL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
 Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:26:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.678	3.674	138.4E6	116.4E6	23.532	21.353
2) SA Decachlor...	8.716	8.664	114.3E6	38185151	22.143	20.639m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 14:28
Operator : YP/AJ
Sample : PB168377BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB168377BL

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 06/11/2025

Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:26:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

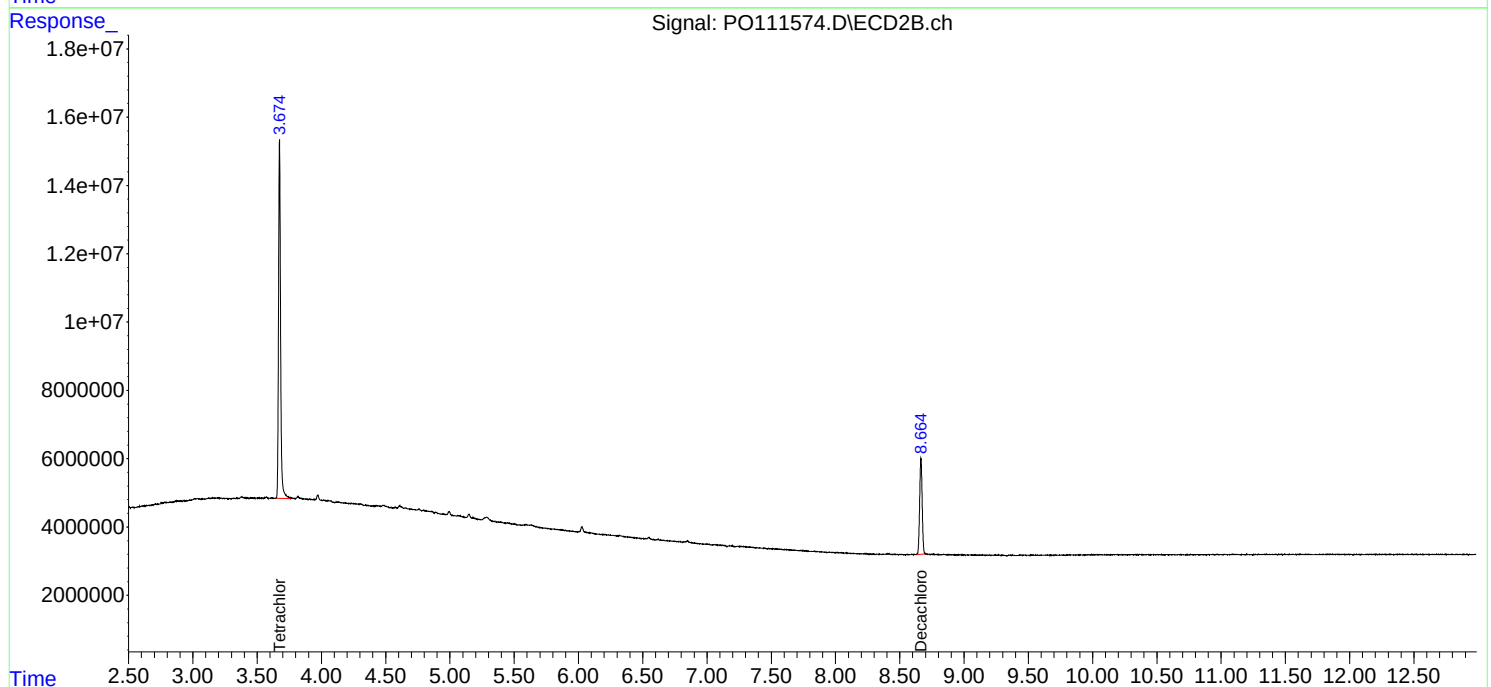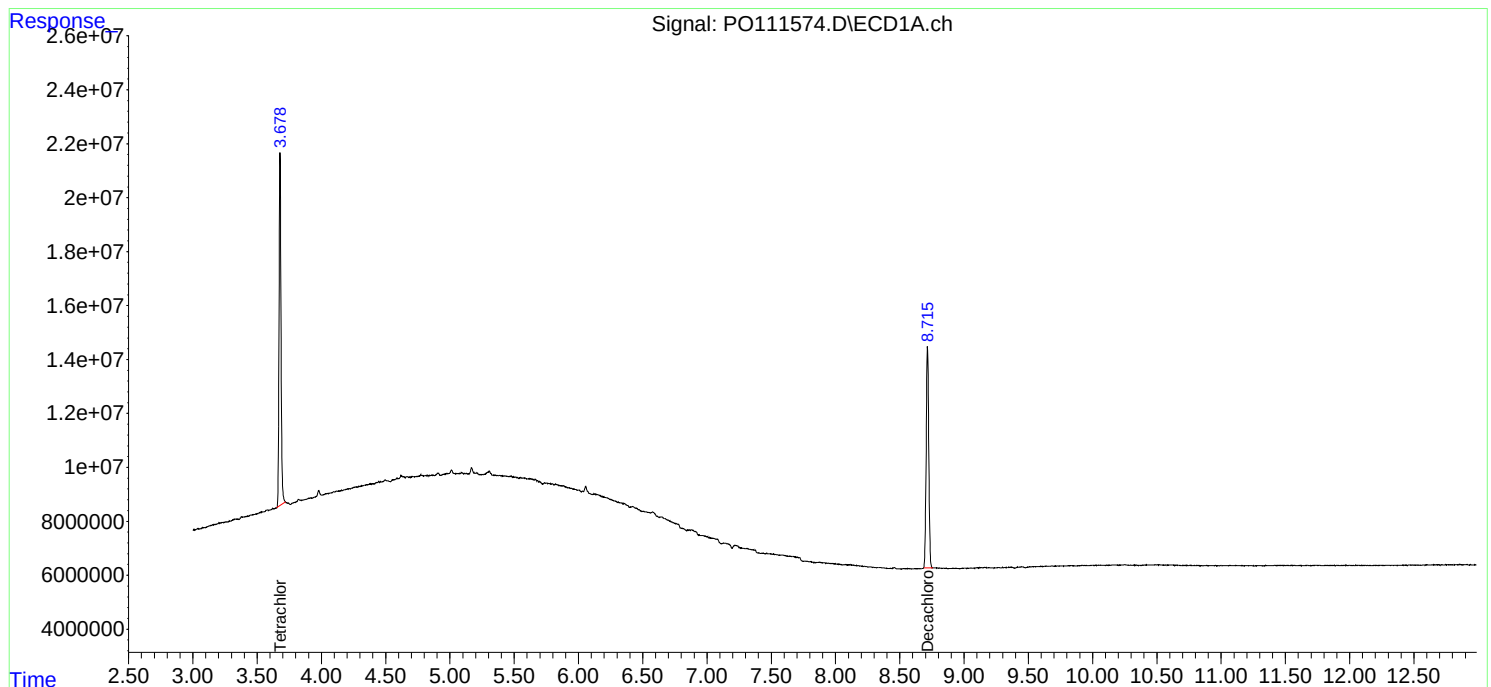

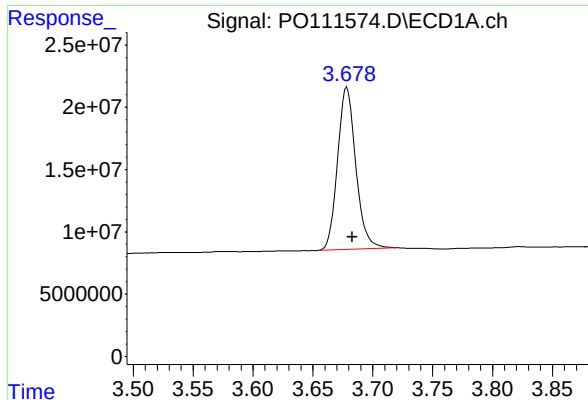


#1 Tetrachloro-m-xylene

R.T.: 3.678 min
Delta R.T.: -0.005 min
Response: 138444811
Conc: 23.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB168377BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

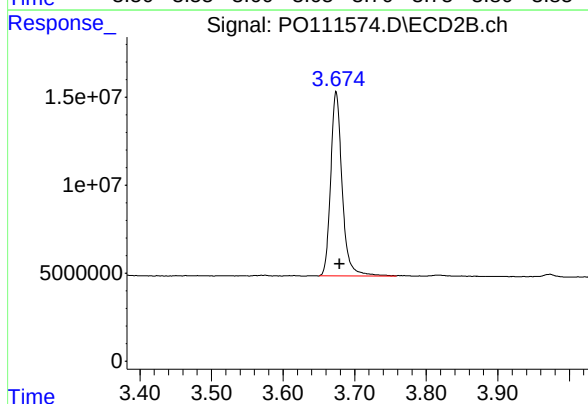


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: -0.005 min
Response: 116403245
Conc: 21.35 ng/ml

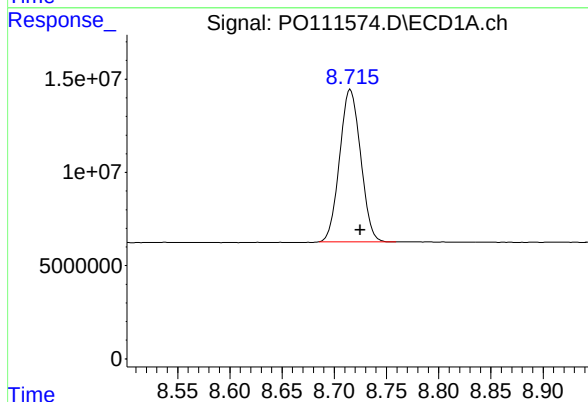

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: -0.010 min
Response: 114321644
Conc: 22.14 ng/ml

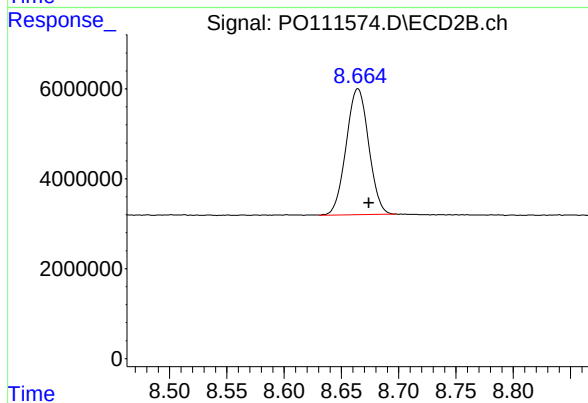

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: -0.010 min
Response: 38185151
Conc: 20.64 ng/ml m

Report of Analysis

Client:	PARSONS Engineering of New York, Inc.	Date Collected:	05/14/25
Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05	Date Received:	05/14/25
Client Sample ID:	PIBLK-PO111057.D	SDG No.:	Q2267
Lab Sample ID:	I.BLK-PO111057.D	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO111057.D	1		05/14/25	PO051525

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	15.4		60 - 140	77%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.5		60 - 140	87%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
 Data File : PO111057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2025 17:01
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 06:39:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 06:36:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	96561347	84147358	16.413	15.436
2) SA Decachlor...	8.723	8.674	90198524	33203686	17.471	17.947

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051525\
Data File : PO111057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2025 17:01
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 06:39:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 06:36:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

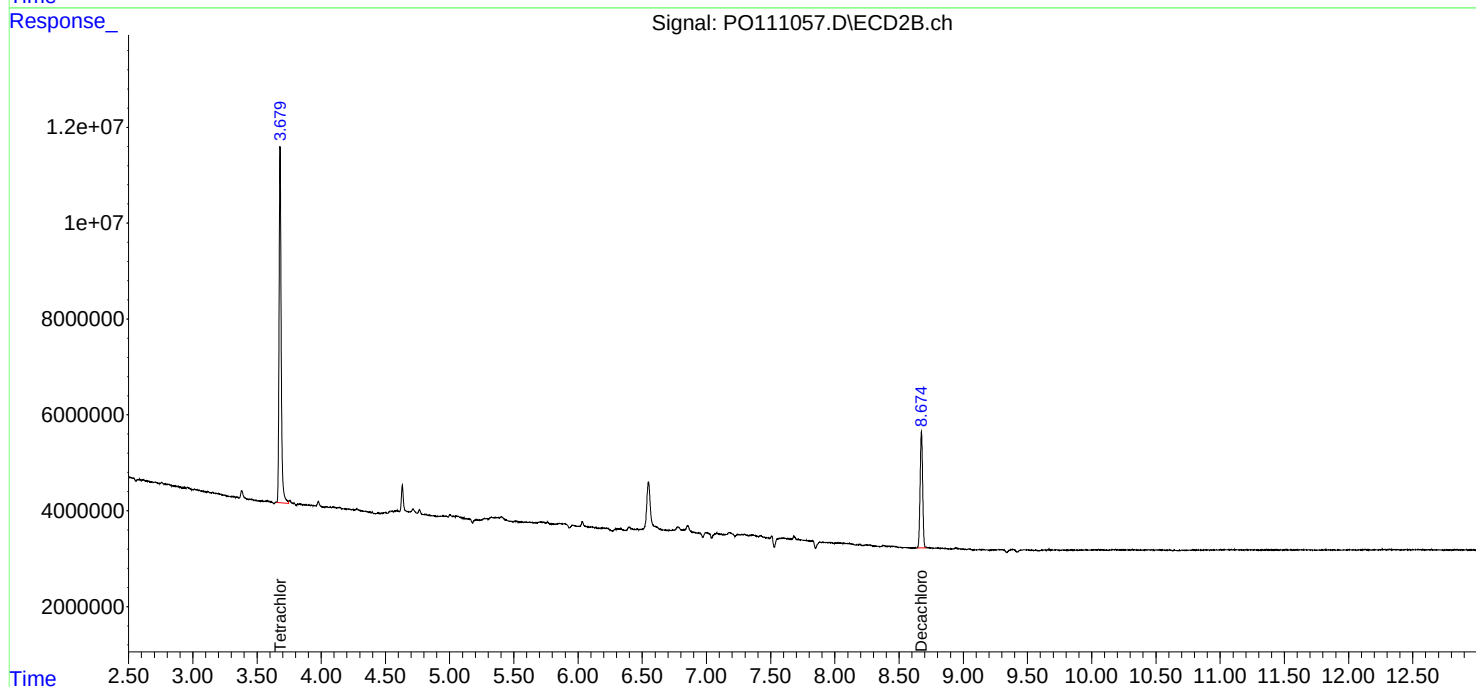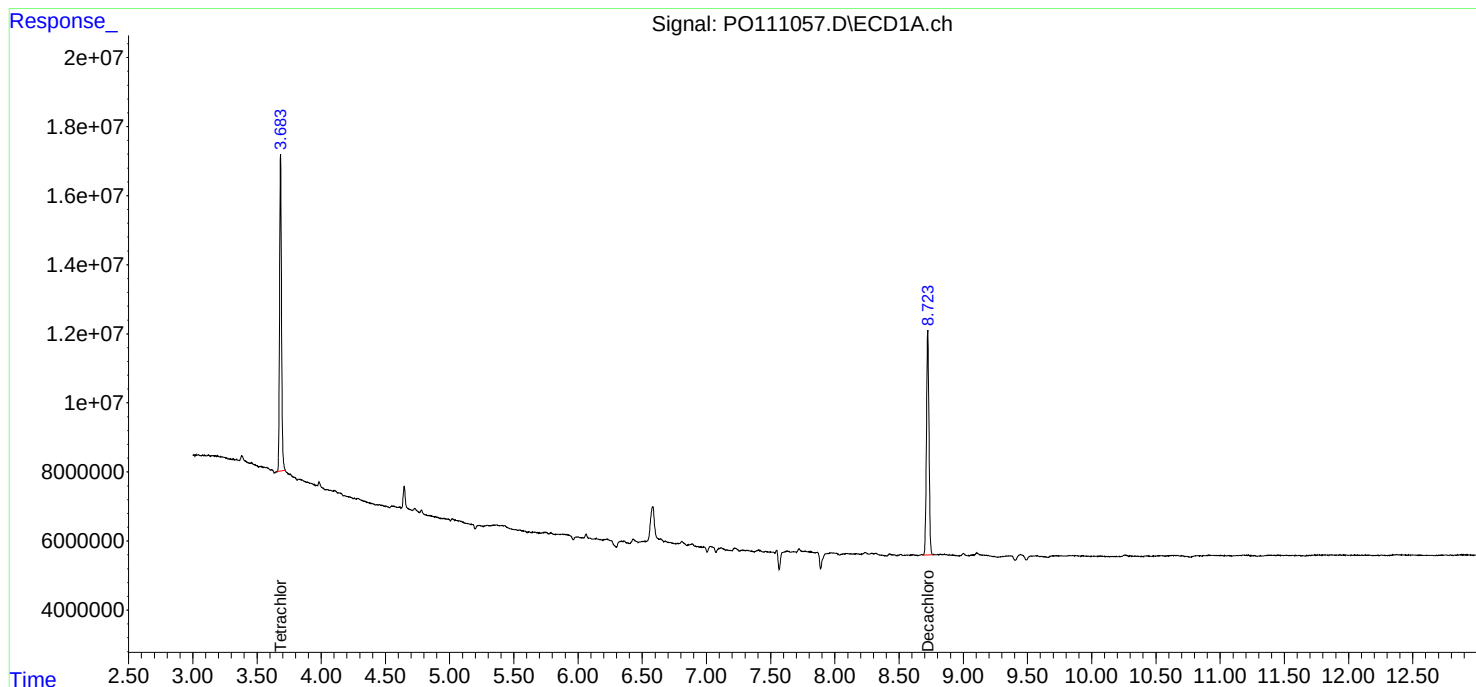


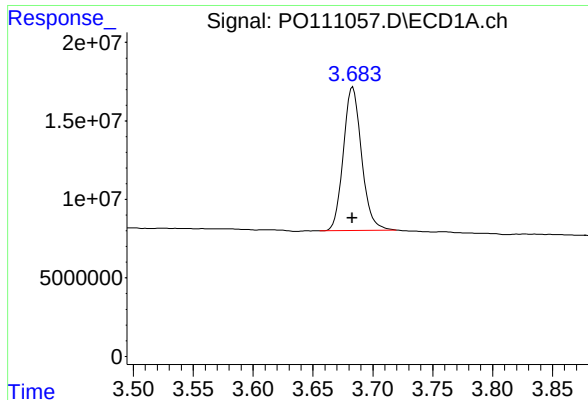

#1 Tetrachloro-m-xylene


R.T.: 3.683 min
Delta R.T.: 0.000 min
Response: 96561347
Conc: 16.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

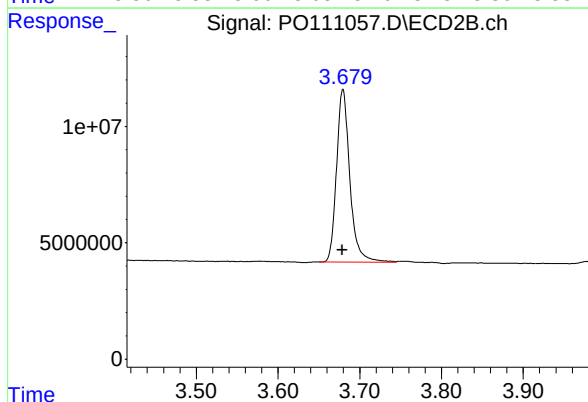


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: 0.000 min
Response: 84147358
Conc: 15.44 ng/ml

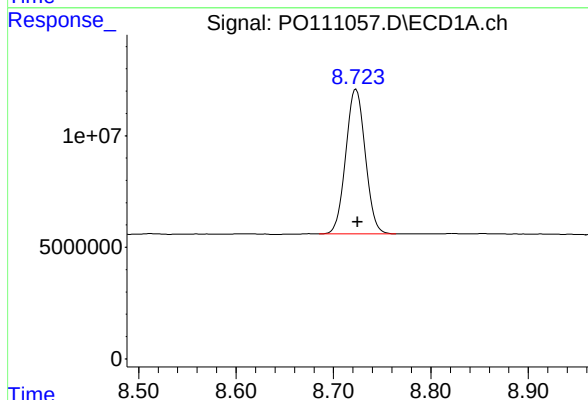

#2 Decachlorobiphenyl

R.T.: 8.723 min
Delta R.T.: -0.002 min
Response: 90198524
Conc: 17.47 ng/ml

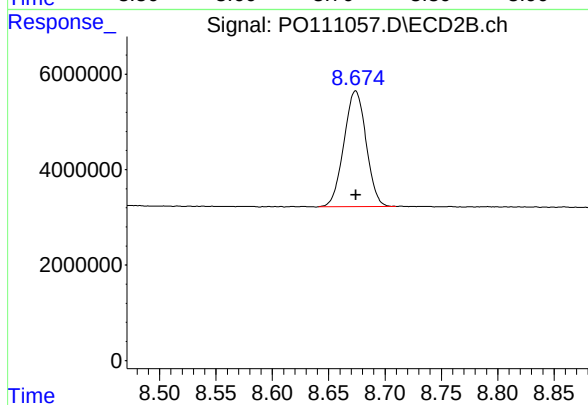

#2 Decachlorobiphenyl

R.T.: 8.674 min
Delta R.T.: 0.000 min
Response: 33203686
Conc: 17.95 ng/ml

Report of Analysis

Client:	PARSONS Engineering of New York, Inc.	Date Collected:	06/10/25
Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05	Date Received:	06/10/25
Client Sample ID:	PIBLK-PO111573.D	SDG No.:	Q2267
Lab Sample ID:	I.BLK-PO111573.D	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO111573.D	1		06/10/25	po061025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.0		60 - 140	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.4		60 - 140	97%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
 Data File : PO111573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 11:39
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
 Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:26:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.679	3.676	128.1E6	109.0E6	21.779	19.998
2) SA Decachlor...	8.716	8.665	106.8E6	35875209	20.695	19.390m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 11:39
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:26:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

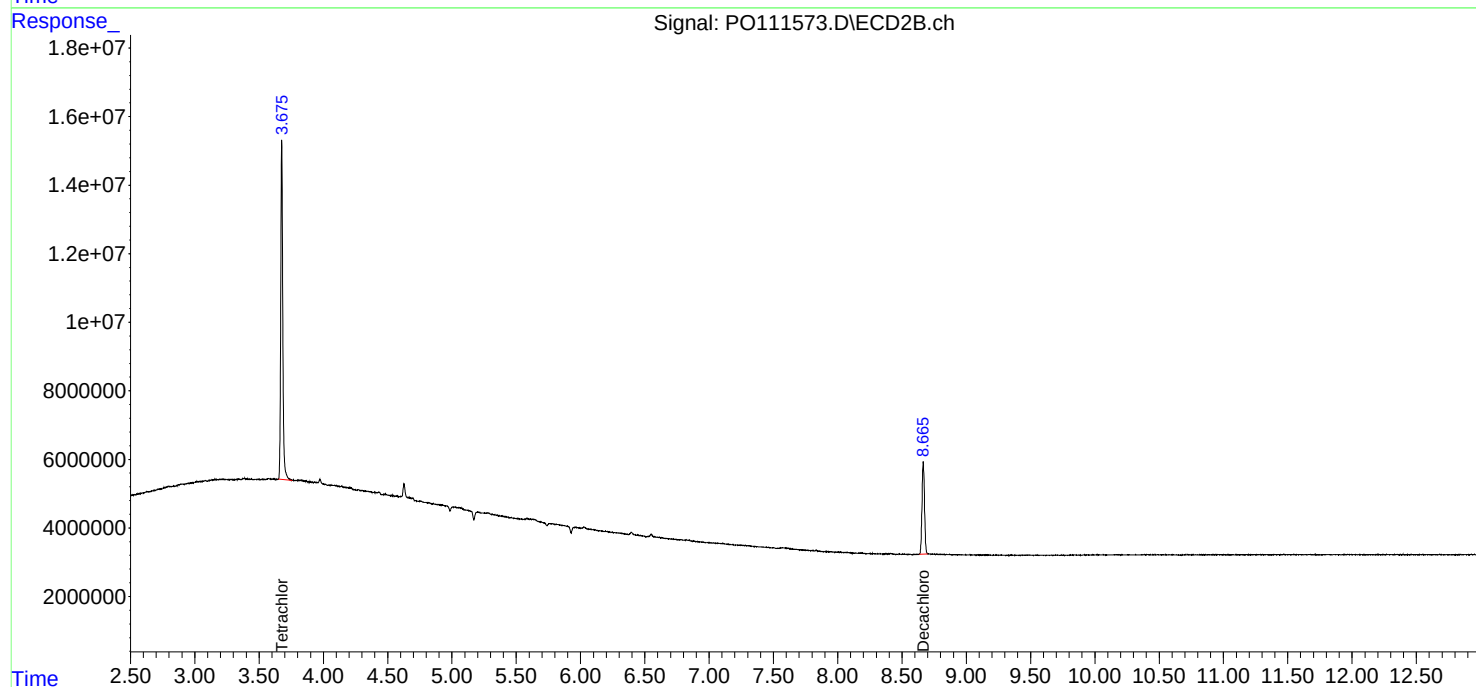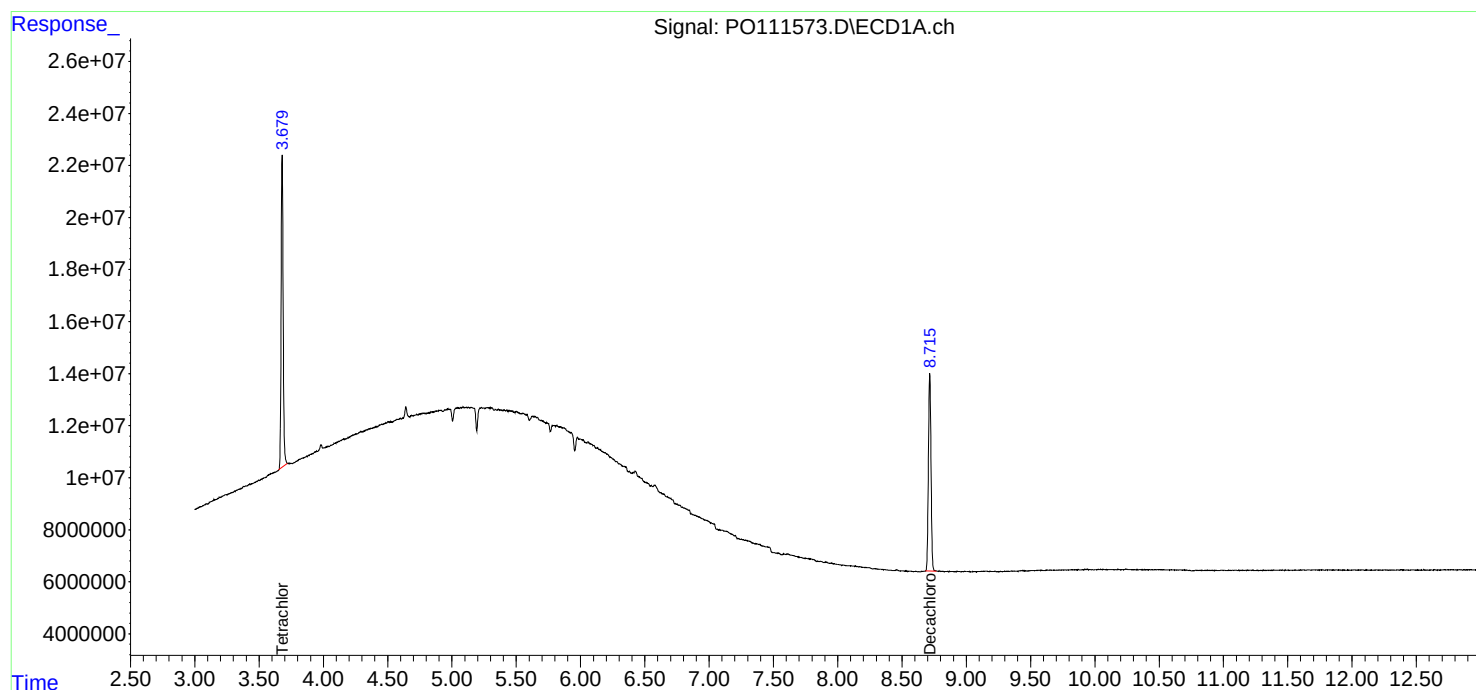

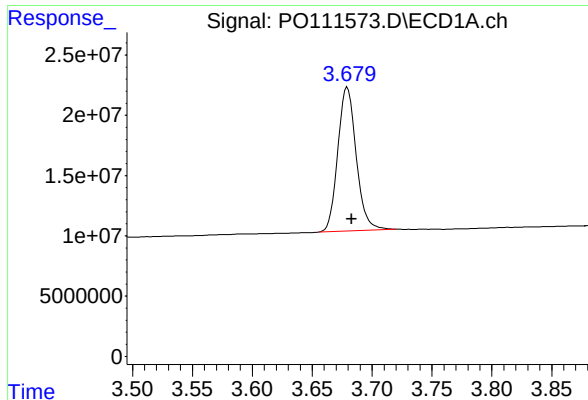


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: -0.004 min
Response: 128129567
Conc: 21.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

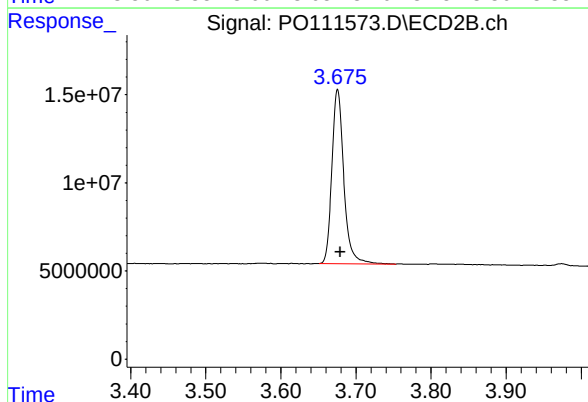


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: -0.003 min
Response: 109017858
Conc: 20.00 ng/ml

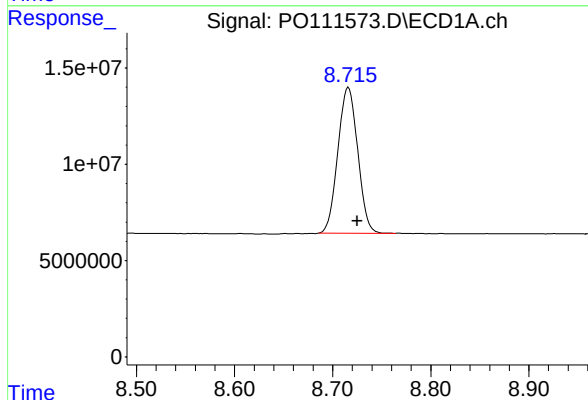

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: -0.009 min
Response: 106848048
Conc: 20.70 ng/ml

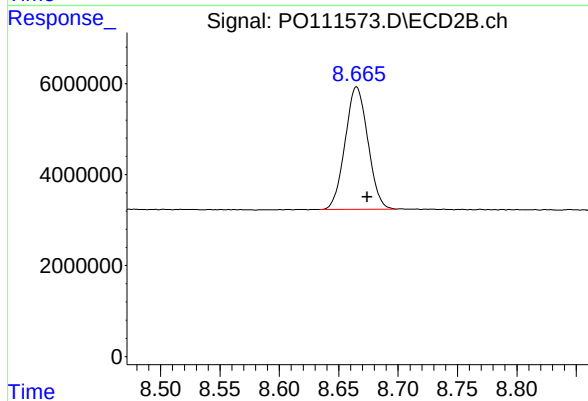

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.009 min
Response: 35875209
Conc: 19.39 ng/ml m

Report of Analysis

Client:	PARSONS Engineering of New York, Inc.	Date Collected:	06/10/25
Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05	Date Received:	06/10/25
Client Sample ID:	PIBLK-PO111584.D	SDG No.:	Q2267
Lab Sample ID:	I.BLK-PO111584.D	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO111584.D	1		06/10/25	po061025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.9		60 - 140	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.2		60 - 140	96%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
 Data File : PO111584.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 18:32
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
 Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:29:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.678	3.676	126.9E6	108.6E6	21.577	19.928
2) SA Decachlor...	8.714	8.665	104.6E6	35521240	20.262	19.199m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111584.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 18:32
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:29:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

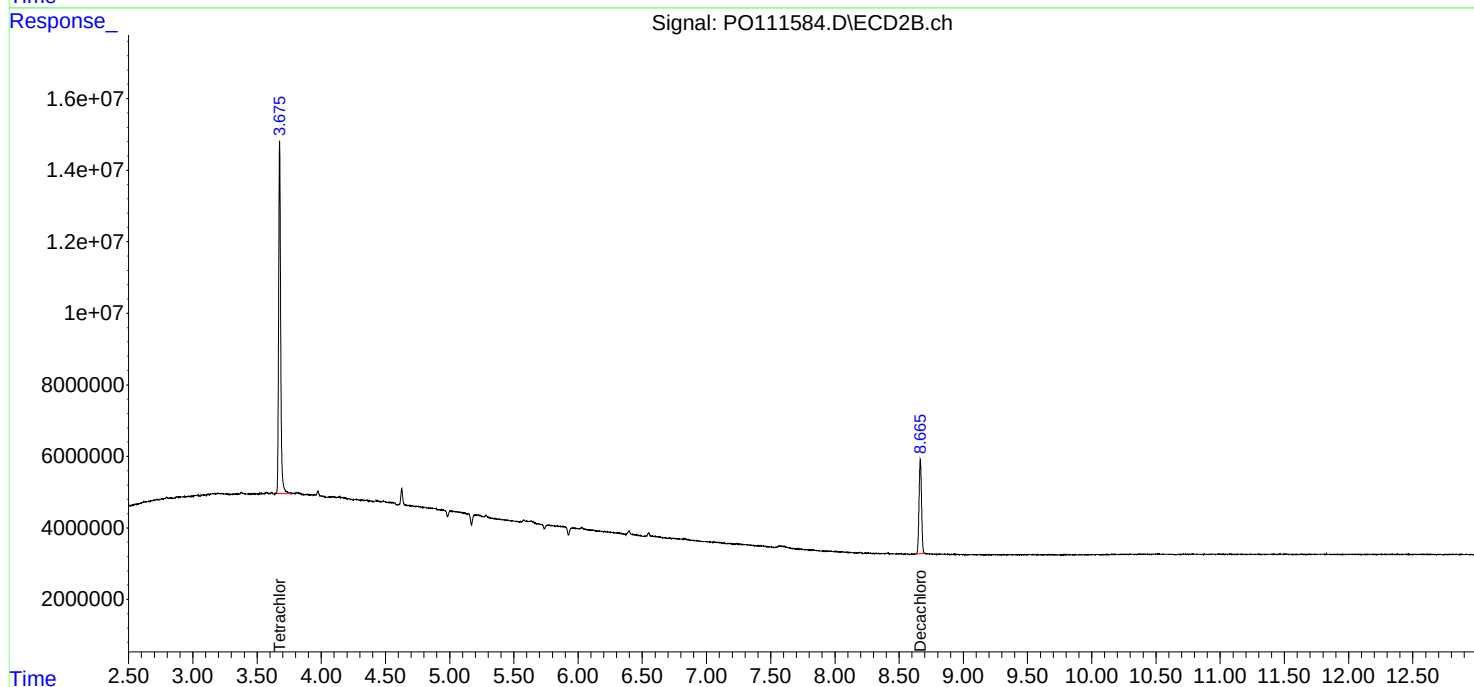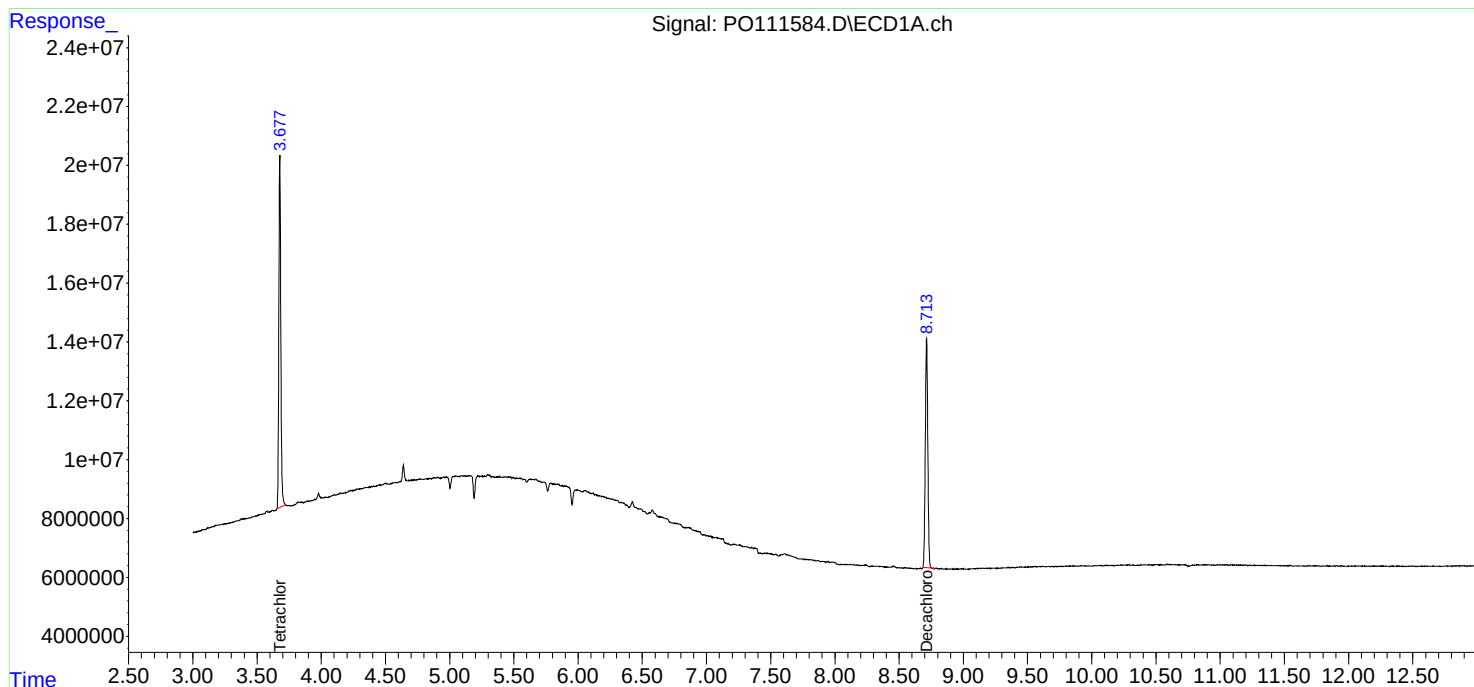

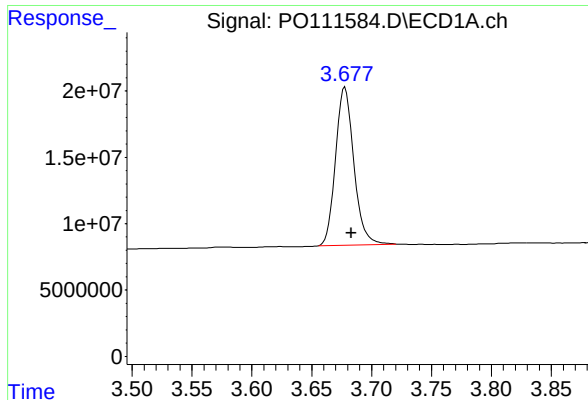


#1 Tetrachloro-m-xylene

R.T.: 3.678 min
Delta R.T.: -0.005 min
Response: 126940997
Conc: 21.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/11/2025
Supervised By :mohammad ahmed 06/12/2025

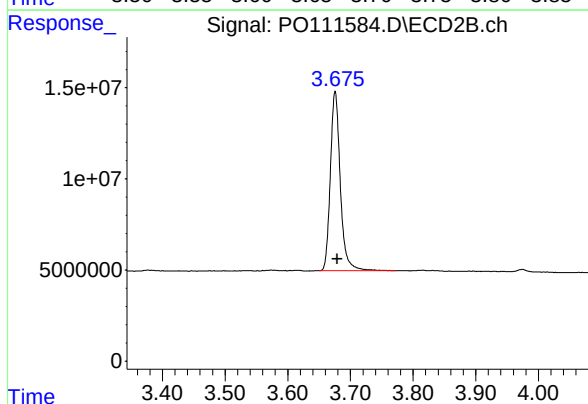


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: -0.003 min
Response: 108638341
Conc: 19.93 ng/ml

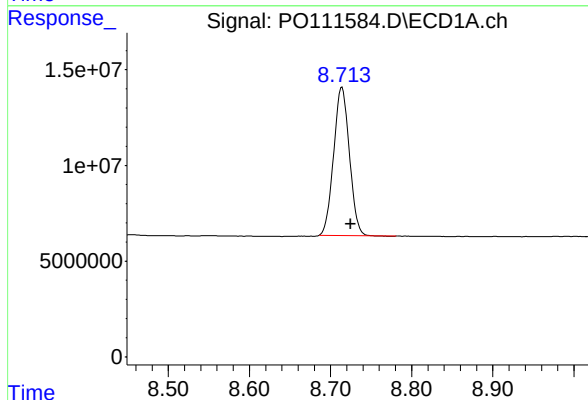

#2 Decachlorobiphenyl

R.T.: 8.714 min
Delta R.T.: -0.011 min
Response: 104607741
Conc: 20.26 ng/ml

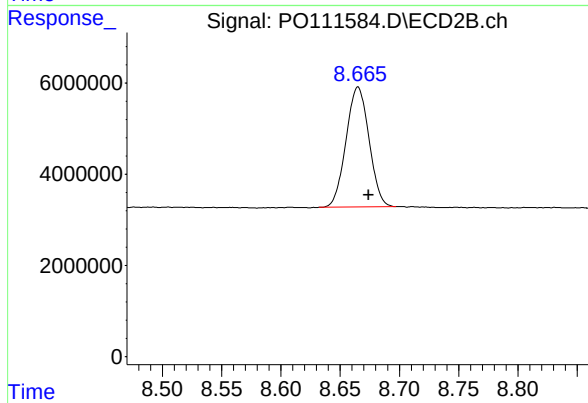

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.009 min
Response: 35521240
Conc: 19.20 ng/ml m

Report of Analysis

Client:	PARSONS Engineering of New York, Inc.	Date Collected:	
Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05	Date Received:	
Client Sample ID:	PB168377BS	SDG No.:	Q2267
Lab Sample ID:	PB168377BS	Matrix:	WATER
Analytical Method:	8082A	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO111575.D	1	06/10/25 09:00	06/10/25 14:47	PB168377

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	4.70		0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	5.00		0.081	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.8		30 - 173	109%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.1		10 - 173	111%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
 Data File : PO111575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 14:47
 Operator : YP/AJ
 Sample : PB168377BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB168377BS

Manual Integrations**APPROVED**

Reviewed By :Yogesh Patel 06/11/2025

Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:26:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.679	3.675	128.0E6	109.0E6	21.758	19.990
2) SA Decachlor...	8.716	8.664	114.2E6	38039060	22.117	20.560m
Target Compounds						
3) L1 AR-1016-1	4.767	4.753	106.2E6	80150460	471.678	419.796
4) L1 AR-1016-2	4.786	4.771	152.4E6	117.4E6	477.937	423.635
5) L1 AR-1016-3	4.843	4.946	103.0E6	61069939	474.431	418.072
6) L1 AR-1016-4	4.963	4.988	82843510	50467906	475.707	420.255
7) L1 AR-1016-5	5.220	5.201	81013188	63044328	460.325m	408.317m
31) L7 AR-1260-1	6.259	6.231	166.4E6	110.1E6	545.492	440.577
32) L7 AR-1260-2	6.449	6.419	217.3E6	128.9E6	567.471	438.063
33) L7 AR-1260-3	6.816	6.571	165.9E6	117.0E6	475.824	407.956
34) L7 AR-1260-4	7.076	7.041	129.0E6	74432103	460.853	370.746
35) L7 AR-1260-5	7.319	7.283	324.1E6	164.3E6	450.217	357.549

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 14:47
Operator : YP/AJ
Sample : PB168377BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB168377BS

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 06/11/2025

Supervised By :mohammad ahmed 06/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:26:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

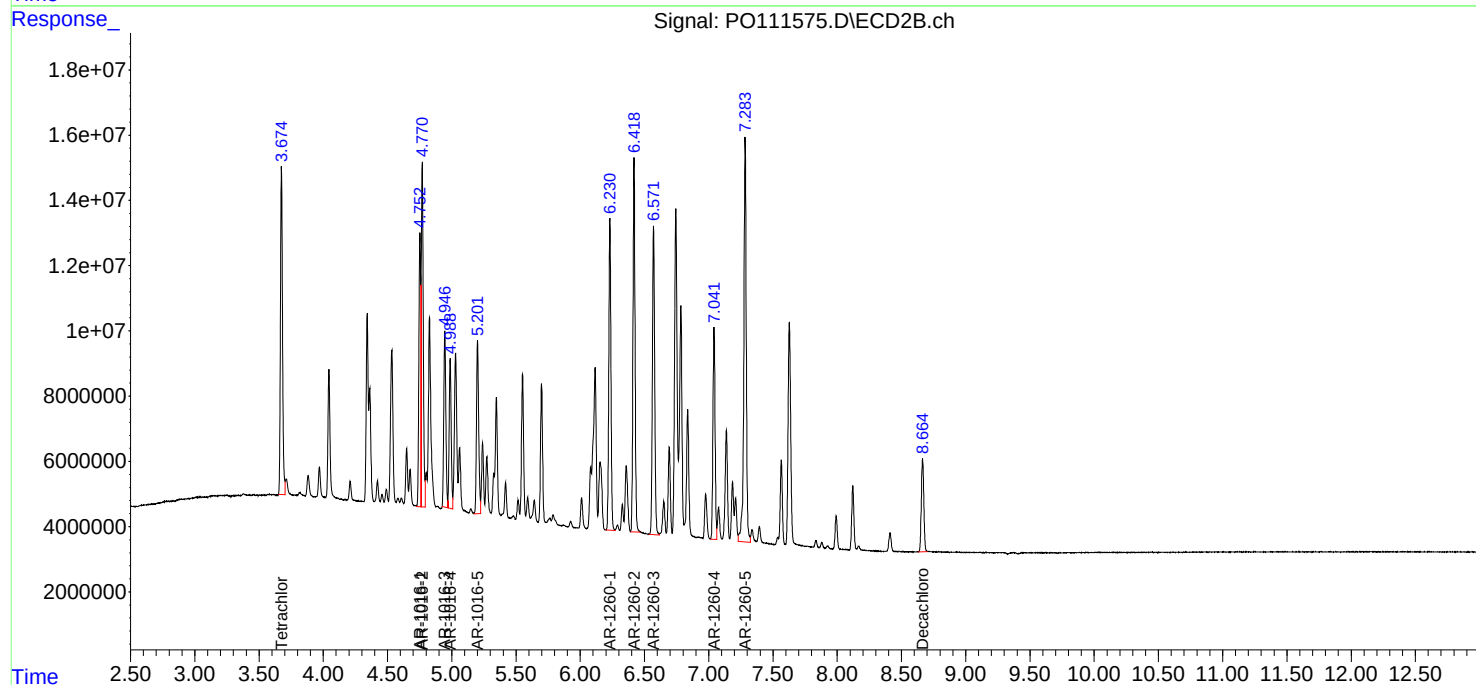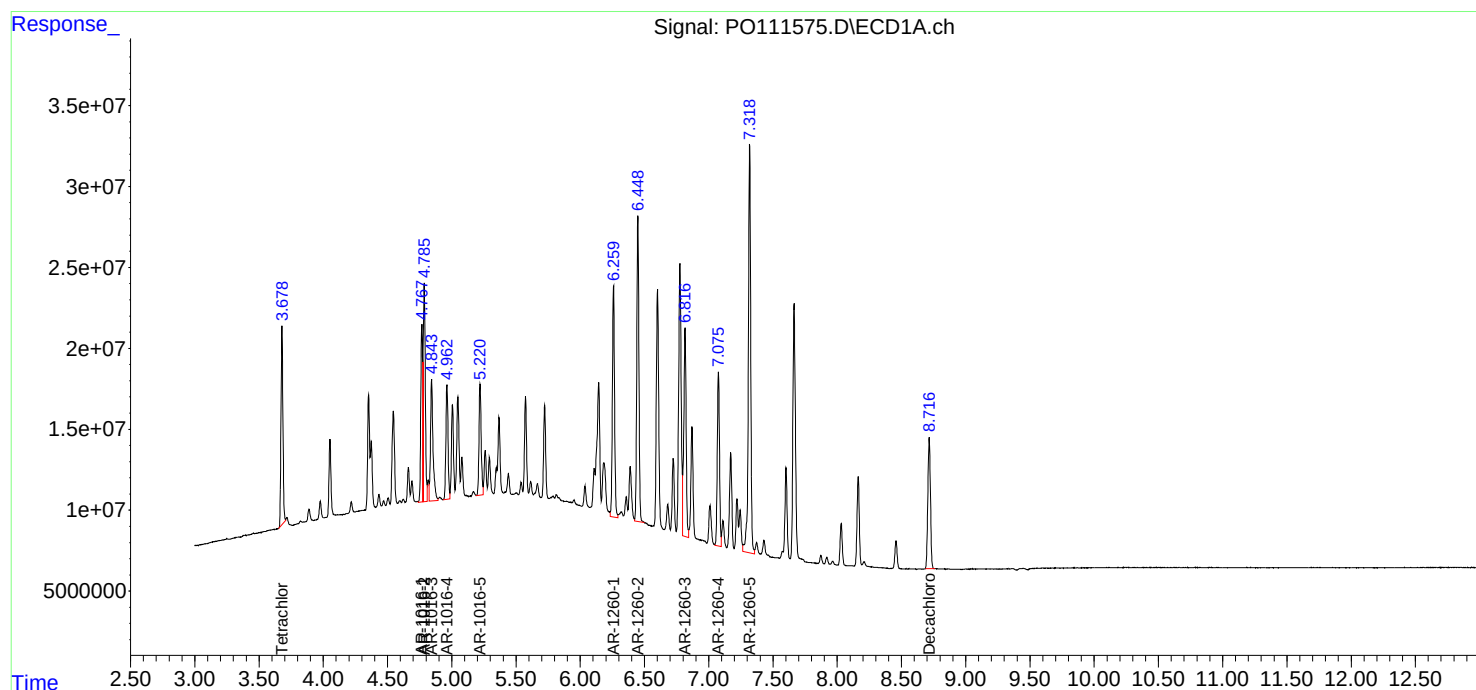

Report of Analysis

Client:	PARSONS Engineering of New York, Inc.		Date Collected:		
Project:	Con Ed Non MGP – Atlantic Ave 453957.600024.05		Date Received:		
Client Sample ID:	PB168377BSD		SDG No.:	Q2267	
Lab Sample ID:	PB168377BSD		Matrix:	WATER	
Analytical Method:	8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	3510C				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO111576.D	1	06/10/25 09:00	06/10/25 15:05	PB168377

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	4.90		0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	5.10		0.081	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.2		30 - 173	106%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.0		10 - 173	110%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061025\
 Data File : P0111576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2025 15:05
 Operator : YP/AJ
 Sample : PB168377BSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB168377BSD

Manual Integrations
APPROVED

Reviewed By :Yogesh
 Patel

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:27:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

06/11/2025
 Supervised By :mohammad
 ahmed

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	06/12/2025

System Monitoring Compounds							
1) SA Tetrachlo...	3.679	3.675	124.9E6	108.9E6	21.238	19.972	
2) SA Decachlor...	8.716	8.665	113.6E6	38356990	22.006	20.732m	
Target Compounds							
3) L1 AR-1016-1	4.768	4.753	109.8E6	82086452	488.018	429.936	
4) L1 AR-1016-2	4.787	4.771	155.9E6	120.7E6	488.796	435.544	
5) L1 AR-1016-3	4.843	4.946	107.9E6	62344910	496.860	426.801	
6) L1 AR-1016-4	4.964	4.989	85993947	51534109	493.798	429.133	
7) L1 AR-1016-5	5.220	5.201	82135119	64173306	466.700m	415.629m	
31) L7 AR-1260-1	6.260	6.231	168.4E6	112.7E6	552.350	451.098	
32) L7 AR-1260-2	6.449	6.420	218.4E6	131.4E6	570.388	446.644	
33) L7 AR-1260-3	6.816	6.572	167.0E6	118.6E6	479.093	413.772	
34) L7 AR-1260-4	7.076	7.042	130.3E6	76585363	465.437	381.471	
35) L7 AR-1260-5	7.319	7.283	329.6E6	167.3E6	457.794	363.973	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061025\
Data File : PO111576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2025 15:05
Operator : YP/AJ
Sample : PB168377BSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB168377BSD



Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:27:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

06/11/2025
Supervised By :mohammad
ahmed

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

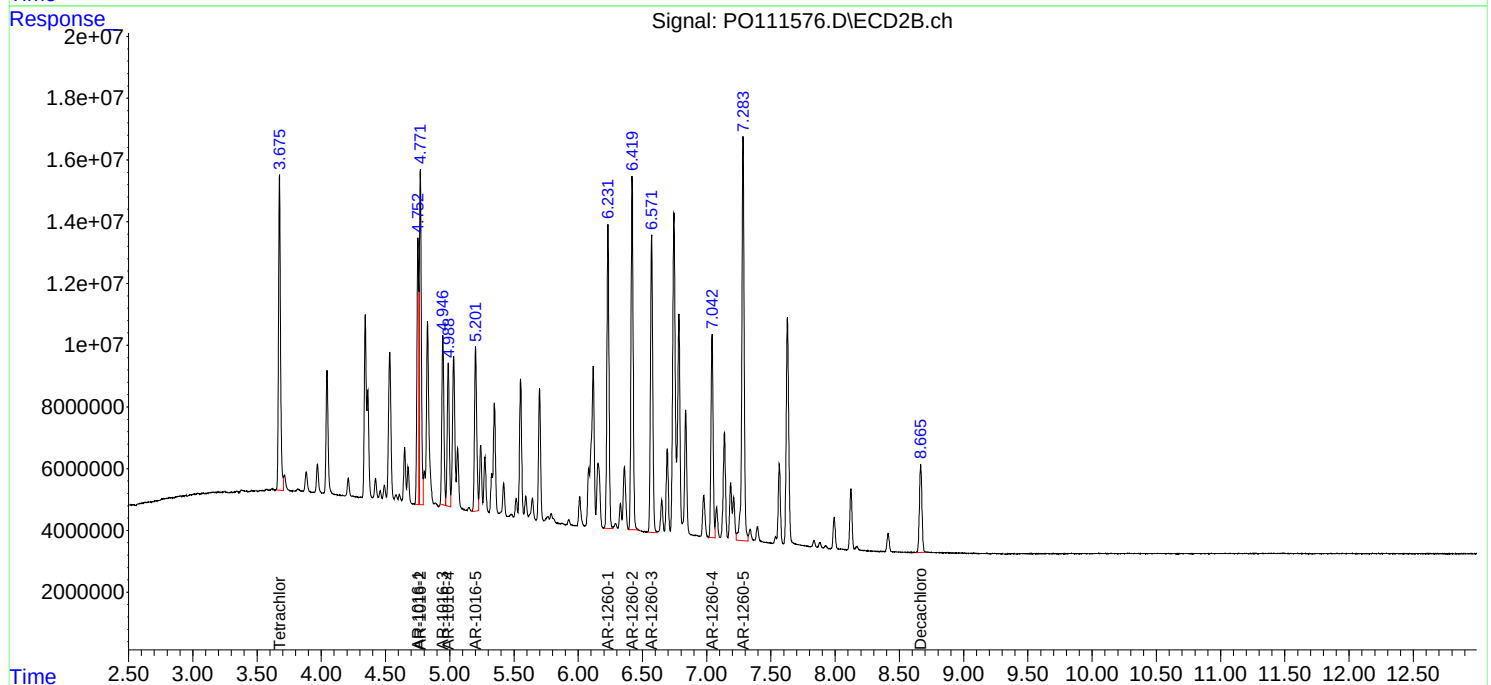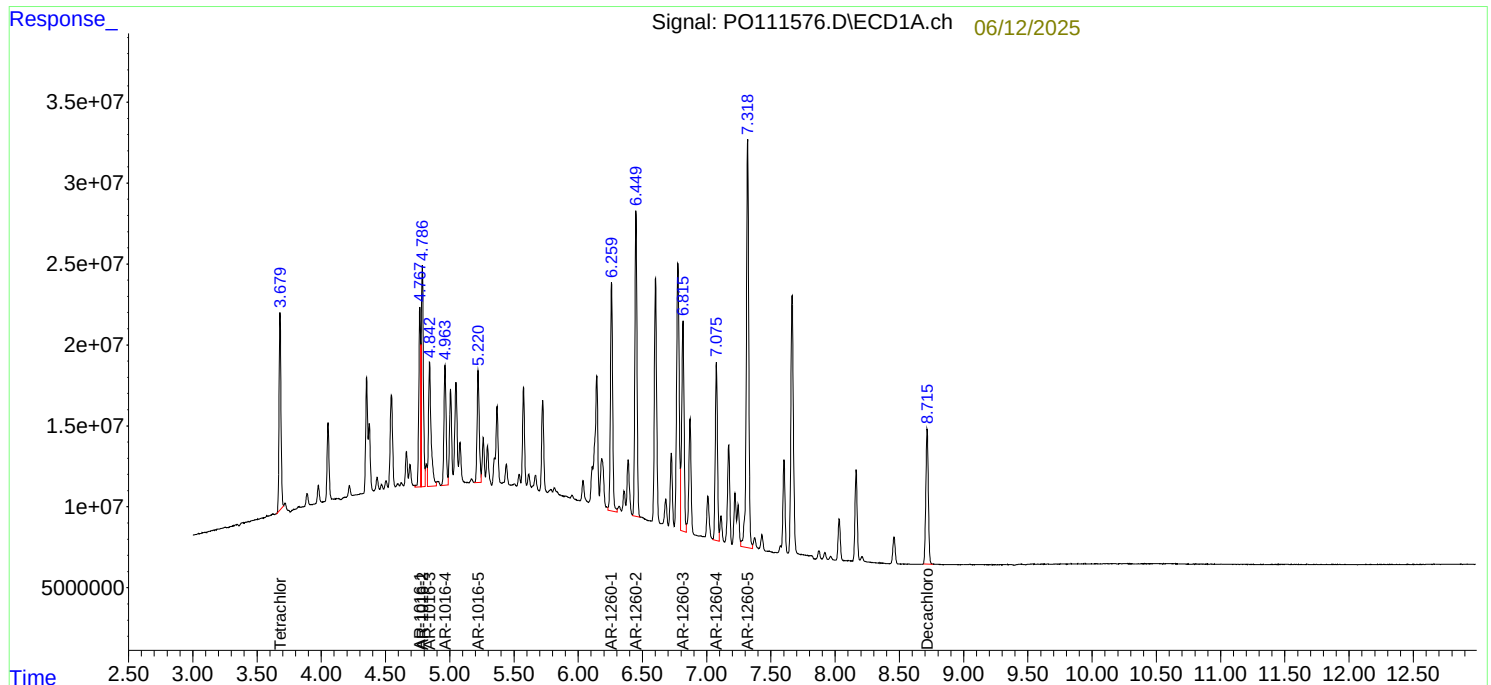

Manual Integration Report

Sequence:

PO051525

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC750	PO111059.D	AR-1260-3 #2	yogesh	5/15/2025 7:37:11 AM	mohammad	5/16/2025 1:55:32	Peak Integrated by Software
AR1660ICC250	PO111061.D	AR-1016-3	yogesh	5/15/2025 7:37:15 AM	mohammad	5/16/2025 1:55:32	Peak Integrated by Software
AR1660ICC050	PO111062.D	AR-1260-1	yogesh	5/15/2025 7:37:17 AM	mohammad	5/16/2025 1:55:32	Peak Integrated by Software
AR1660ICC050	PO111062.D	AR-1260-2	yogesh	5/15/2025 7:37:17 AM	mohammad	5/16/2025 1:55:32	Peak Integrated by Software
AR1660ICC050	PO111062.D	AR-1260-3 #2	yogesh	5/15/2025 7:37:17 AM	mohammad	5/16/2025 1:55:32	Peak Integrated by Software

Manual Integration Report

Sequence:	po061025	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1242CCC500	PO111570.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:13 AM	 	 	Peak Integrated by Software
AR1248CCC500	PO111571.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:15 AM	 	 	Peak Integrated by Software
AR1254CCC500	PO111572.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:16 AM	 	 	Peak Integrated by Software
I.BLK	PO111573.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:18 AM	 	 	Peak Integrated by Software
PB168377BL	PO111574.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:19 AM	 	 	Peak Integrated by Software
PB168377BS	PO111575.D	AR-1016-5	yogesh	6/11/2025 11:27:21 AM	 	 	Peak Integrated by Software
PB168377BS	PO111575.D	AR-1016-5 #2	yogesh	6/11/2025 11:27:21 AM	 	 	Peak Integrated by Software
PB168377BS	PO111575.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:21 AM	 	 	Peak Integrated by Software
PB168377BSD	PO111576.D	AR-1016-5	yogesh	6/11/2025 11:27:23 AM	 	 	Peak Integrated by Software
PB168377BSD	PO111576.D	AR-1016-5 #2	yogesh	6/11/2025 11:27:23 AM	 	 	Peak Integrated by Software
PB168377BSD	PO111576.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:23 AM	 	 	Peak Integrated by Software
Q2267-01	PO111579.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:28 AM	 	 	Peak Integrated by Software
Q2267-01	PO111579.D	Tetrachloro-m-xylene #2	yogesh	6/11/2025 11:27:28 AM	 	 	Peak Integrated by Software

Manual Integration Report

Sequence:

po061025

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO111580.D	AR-1016-5	yogesh	6/11/2025 11:27:30 AM	 	 	Peak Integrated by Software
AR1660CCC500	PO111580.D	Decachlorobiphenyl	yogesh	6/11/2025 11:27:30 AM	 	 	Peak Integrated by Software
AR1660CCC500	PO111580.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:30 AM	 	 	Peak Integrated by Software
AR1242CCC500	PO111581.D	AR-1242-5	yogesh	6/11/2025 11:27:32 AM	 	 	Peak Integrated by Software
AR1242CCC500	PO111581.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:32 AM	 	 	Peak Integrated by Software
AR1248CCC500	PO111582.D	AR-1248-3	yogesh	6/11/2025 11:27:34 AM	 	 	Peak Integrated by Software
AR1248CCC500	PO111582.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:34 AM	 	 	Peak Integrated by Software
AR1254CCC500	PO111583.D	Decachlorobiphenyl	yogesh	6/11/2025 11:27:35 AM	 	 	Peak Integrated by Software
AR1254CCC500	PO111583.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:35 AM	 	 	Peak Integrated by Software
I.BLK	PO111584.D	Decachlorobiphenyl #2	yogesh	6/11/2025 11:27:37 AM	 	 	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO051525

Review By	yogesh	Review On	5/14/2025 3:39:03 PM
Supervise By	mohammad	Supervise On	5/16/2025 1:55:32 AM
SubDirectory	PO051525	HP Acquire Method	HP Processing Method PO051525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344, PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359, PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		

Sr#	Sampleld	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO111056.D	14 May 2025 16:43	YP/AJ	Ok
2	I.BLK	PO111057.D	14 May 2025 17:01	YP/AJ	Ok
3	AR1660ICC1000	PO111058.D	14 May 2025 17:19	YP/AJ	Ok
4	AR1660ICC750	PO111059.D	14 May 2025 17:38	YP/AJ	Ok,M
5	AR1660ICC500	PO111060.D	14 May 2025 17:56	YP/AJ	Ok
6	AR1660ICC250	PO111061.D	14 May 2025 18:15	YP/AJ	Ok,M
7	AR1660ICC050	PO111062.D	14 May 2025 18:33	YP/AJ	Ok,M
8	AR1221ICC500	PO111063.D	14 May 2025 18:51	YP/AJ	Ok
9	AR1232ICC500	PO111064.D	14 May 2025 19:10	YP/AJ	Ok
10	AR1242ICC1000	PO111065.D	14 May 2025 19:28	YP/AJ	Ok
11	AR1242ICC750	PO111066.D	14 May 2025 19:46	YP/AJ	Ok
12	AR1242ICC500	PO111067.D	14 May 2025 20:05	YP/AJ	Ok
13	AR1242ICC250	PO111068.D	14 May 2025 20:23	YP/AJ	Ok
14	AR1242ICC050	PO111069.D	14 May 2025 20:41	YP/AJ	Ok
15	AR1248ICC1000	PO111070.D	14 May 2025 21:00	YP/AJ	Ok
16	AR1248ICC750	PO111071.D	14 May 2025 21:18	YP/AJ	Ok
17	AR1248ICC500	PO111072.D	14 May 2025 21:37	YP/AJ	Ok
18	AR1248ICC250	PO111073.D	14 May 2025 21:54	YP/AJ	Ok
19	AR1248ICC050	PO111074.D	14 May 2025 22:12	YP/AJ	Ok
20	AR1254ICC1000	PO111075.D	14 May 2025 22:31	YP/AJ	Ok
21	AR1254ICC750	PO111076.D	14 May 2025 22:49	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO051525

Review By	yogesh	Review On	5/14/2025 3:39:03 PM
Supervise By	mohammad	Supervise On	5/16/2025 1:55:32 AM
SubDirectory	PO051525	HP Acquire Method	HP Processing Method PO051525
STD. NAME	STD REF.#		
Tune/Reschk	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
LCS Standard			

22	AR1254ICC500	PO111077.D	14 May 2025 23:06	YP/AJ	Ok
23	AR1254ICC250	PO111078.D	14 May 2025 23:25	YP/AJ	Ok
24	AR1254ICC050	PO111079.D	14 May 2025 23:43	YP/AJ	Ok
25	AR1262ICC500	PO111080.D	15 May 2025 00:01	YP/AJ	Ok
26	AR1268ICC1000	PO111081.D	15 May 2025 00:19	YP/AJ	Ok
27	AR1268ICC750	PO111082.D	15 May 2025 00:37	YP/AJ	Ok
28	AR1268ICC500	PO111083.D	15 May 2025 00:56	YP/AJ	Ok
29	AR1268ICC250	PO111084.D	15 May 2025 01:14	YP/AJ	Ok
30	AR1268ICC050	PO111085.D	15 May 2025 01:31	YP/AJ	Ok
31	PO051525ICV500	PO111086.D	15 May 2025 01:50	YP/AJ	Ok
32	AR1242ICV500	PO111087.D	15 May 2025 02:26	YP/AJ	Ok
33	AR1248ICV500	PO111088.D	15 May 2025 03:03	YP/AJ	Ok
34	AR1254ICV500	PO111089.D	15 May 2025 03:40	YP/AJ	Ok
35	AR1268ICV500	PO111090.D	15 May 2025 04:17	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO061025

Review By	yogesh	Review On	6/10/2025 1:00:18 PM
Supervise By		Supervise On	
SubDirectory	PO061025	HP Acquire Method	HP Processing Method PO051525
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369		
CCC	PP24332,PP24347,PP24352,PP24357		
Internal Standard/PEM			
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO111568.D	10 Jun 2025 09:42	YP/AJ	Ok
2	AR1660CCC500	PO111569.D	10 Jun 2025 10:26	YP/AJ	Ok
3	AR1242CCC500	PO111570.D	10 Jun 2025 10:44	YP/AJ	Ok,NS
4	AR1248CCC500	PO111571.D	10 Jun 2025 11:03	YP/AJ	Ok,NS
5	AR1254CCC500	PO111572.D	10 Jun 2025 11:21	YP/AJ	Ok,NS
6	I.BLK	PO111573.D	10 Jun 2025 11:39	YP/AJ	Ok,NS
7	PB168377BL	PO111574.D	10 Jun 2025 14:28	YP/AJ	Ok,NS
8	PB168377BS	PO111575.D	10 Jun 2025 14:47	YP/AJ	Ok,NS
9	PB168377BSD	PO111576.D	10 Jun 2025 15:05	YP/AJ	Ok,NS
10	Q2245-01	PO111577.D	10 Jun 2025 15:24	YP/AJ	Ok,NS
11	Q2245-02	PO111578.D	10 Jun 2025 15:42	YP/AJ	Ok,NS
12	Q2267-01	PO111579.D	10 Jun 2025 16:00	YP/AJ	Ok,NS
13	AR1660CCC500	PO111580.D	10 Jun 2025 17:04	YP/AJ	Ok,NS
14	AR1242CCC500	PO111581.D	10 Jun 2025 17:40	YP/AJ	Ok,NS
15	AR1248CCC500	PO111582.D	10 Jun 2025 17:57	YP/AJ	Ok,NS
16	AR1254CCC500	PO111583.D	10 Jun 2025 18:15	YP/AJ	Ok,NS
17	I.BLK	PO111584.D	10 Jun 2025 18:32	YP/AJ	Ok,NS

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO051525

Review By	yogesh	Review On	5/14/2025 3:39:03 PM
Supervise By	mohammad	Supervise On	5/16/2025 1:55:32 AM
SubDirectory	PO051525	HP Acquire Method	HP Processing Method PO051525

STD. NAME	STD REF.#
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,P P24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP 24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO111056.D	14 May 2025 16:43		YP/AJ	Ok
2	I.BLK	I.BLK	PO111057.D	14 May 2025 17:01		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO111058.D	14 May 2025 17:19		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO111059.D	14 May 2025 17:38		YP/AJ	Ok,M
5	AR1660ICC500	AR1660ICC500	PO111060.D	14 May 2025 17:56		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO111061.D	14 May 2025 18:15		YP/AJ	Ok,M
7	AR1660ICC050	AR1660ICC050	PO111062.D	14 May 2025 18:33		YP/AJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PO111063.D	14 May 2025 18:51		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO111064.D	14 May 2025 19:10		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO111065.D	14 May 2025 19:28		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO111066.D	14 May 2025 19:46		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO111067.D	14 May 2025 20:05		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO111068.D	14 May 2025 20:23		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO111069.D	14 May 2025 20:41		YP/AJ	Ok
15	AR1248ICC1000	AR1248ICC1000	PO111070.D	14 May 2025 21:00		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO111071.D	14 May 2025 21:18		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO111072.D	14 May 2025 21:37		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO111073.D	14 May 2025 21:54		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO051525

Review By	yogesh	Review On	5/14/2025 3:39:03 PM
Supervise By	mohammad	Supervise On	5/16/2025 1:55:32 AM
SubDirectory	PO051525	HP Acquire Method	HP Processing Method PO051525
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,P P24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP 24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387		

19	AR1248ICC050	AR1248ICC050	PO111074.D	14 May 2025 22:12		YP/AJ	Ok
20	AR1254ICC1000	AR1254ICC1000	PO111075.D	14 May 2025 22:31		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO111076.D	14 May 2025 22:49		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO111077.D	14 May 2025 23:06		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO111078.D	14 May 2025 23:25		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO111079.D	14 May 2025 23:43		YP/AJ	Ok
25	AR1262ICC500	AR1262ICC500	PO111080.D	15 May 2025 00:01		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO111081.D	15 May 2025 00:19		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO111082.D	15 May 2025 00:37		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO111083.D	15 May 2025 00:56		YP/AJ	Ok
29	AR1268ICC250	AR1268ICC250	PO111084.D	15 May 2025 01:14		YP/AJ	Ok
30	AR1268ICC050	AR1268ICC050	PO111085.D	15 May 2025 01:31		YP/AJ	Ok
31	PO051525ICV500	ICVPO051525	PO111086.D	15 May 2025 01:50		YP/AJ	Ok
32	AR1242ICV500	ICVPO051525AR1242	PO111087.D	15 May 2025 02:26		YP/AJ	Ok
33	AR1248ICV500	ICVPO051525AR1248	PO111088.D	15 May 2025 03:03		YP/AJ	Ok
34	AR1254ICV500	ICVPO051525AR1254	PO111089.D	15 May 2025 03:40		YP/AJ	Ok
35	AR1268ICV500	ICVPO051525AR1268	PO111090.D	15 May 2025 04:17		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO061025

Review By	yogesh	Review On	6/10/2025 1:00:18 PM
Supervise By		Supervise On	
SubDirectory	PO061025	HP Acquire Method	HP Processing Method PO051525

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,P P24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP 24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369
CCC	PP24332,PP24347,PP24352,PP24357
Internal Standard/PEM	
ICV/I.BLK	PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO111568.D	10 Jun 2025 09:42		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO111569.D	10 Jun 2025 10:26	AR1260 - 2,3 High in 1st column	YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO111570.D	10 Jun 2025 10:44	AR1242 - 5 high in 1st column	YP/AJ	Ok,NS
4	AR1248CCC500	AR1248CCC500	PO111571.D	10 Jun 2025 11:03		YP/AJ	Ok,NS
5	AR1254CCC500	AR1254CCC500	PO111572.D	10 Jun 2025 11:21	AR1254 - 2 high in 1st column	YP/AJ	Ok,NS
6	I.BLK	I.BLK	PO111573.D	10 Jun 2025 11:39		YP/AJ	Ok,NS
7	PB168377BL	PB168377BL	PO111574.D	10 Jun 2025 14:28		YP/AJ	Ok,NS
8	PB168377BS	PB168377BS	PO111575.D	10 Jun 2025 14:47		YP/AJ	Ok,NS
9	PB168377BSD	PB168377BSD	PO111576.D	10 Jun 2025 15:05		YP/AJ	Ok,NS
10	Q2245-01	AUD-25-0090	PO111577.D	10 Jun 2025 15:24		YP/AJ	Ok,NS
11	Q2245-02	AUD-25-0091	PO111578.D	10 Jun 2025 15:42		YP/AJ	Ok,NS
12	Q2267-01	WC-20250605	PO111579.D	10 Jun 2025 16:00		YP/AJ	Ok,NS
13	AR1660CCC500	AR1660CCC500	PO111580.D	10 Jun 2025 17:04	AR1260 - 2,3 High in 1st column	YP/AJ	Ok,NS
14	AR1242CCC500	AR1242CCC500	PO111581.D	10 Jun 2025 17:40		YP/AJ	Ok,NS
15	AR1248CCC500	AR1248CCC500	PO111582.D	10 Jun 2025 17:57		YP/AJ	Ok,NS
16	AR1254CCC500	AR1254CCC500	PO111583.D	10 Jun 2025 18:15		YP/AJ	Ok,NS
17	I.BLK	I.BLK	PO111584.D	10 Jun 2025 18:32		YP/AJ	Ok,NS

M : Manual Integration

SOP ID: M3510C,3580A-Extraction PCB-14

Clean Up SOP #: Acid Cleanup

Matrix : Water

Weigh By: N/A

Balance check: N/A

Balance ID: N/A

pH Strip Lot#: E3880

Extraction By: RS

Filter By: RS

pH Meter ID: N/A

Hood ID: 4,5,6,7

Extraction Start Date : 06/10/2025

Extraction Start Time : 09:00

Extraction End Date : 06/10/2025

Extraction End Time : 13:40

Concentration By: EH

Supervisor By : RUPESH

Extraction Method: ☒ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☐ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24461
Surrogate	1.0ML	200 PPB	PP24597
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3939
Baked Na2SO4	N/A	EP2620
Hexane	N/A	E3938
H2SO4 1:1	N/A	EP2610
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40BTS723,

KD Bath ID: WATER BATH-1,2

KD Bath Temperature: 60 °C

Envap ID: NEVAP-02

Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
06/10/25	RP (Ext-204)	Y-P POSTIP CB
13:45	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction PCB-14

Concentration Date: 06/10/2025

Sample ID	Client Sample ID	Test	g / <u>mL</u>	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB168377BL	ABLK377	PCB	1000	6	RUPESH	ritesh	10			SEP-01
PB168377BS	ALCS377	PCB	1000	6	RUPESH	ritesh	10			2
PB168377BS D	ALCSD377	PCB	1000	6	RUPESH	ritesh	10			3
Q2245-01	AU-25-0090	PCB	990	6	RUPESH	ritesh	10	B		4
Q2245-02	AU-25-0091	PCB	990	6	RUPESH	ritesh	10	B		5
Q2267-01	WC-20250605	PCB	980	6	RUPESH	ritesh	10	G		6

* Extracts relinquished on the same date as received.

8/6/10/25

WORKLIST(Hardcopy Internal Chain)

168377
Q:00

Worklist Name : Q2267

Worklist ID : 190062

Department : Extraction

Date : 06-10-2025 08:07:03

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2245-01	AU-25-0090	Water	PCB	Cool 4 deg C	PSEG03	D11	06/05/2025	8082A
Q2245-02	AU-25-0091	Water	PCB	Cool 4 deg C	PSEG03	D11	06/05/2025	8082A
Q2267-01	WC-20250605	Water	PCB	Cool 4 deg C	PARS02	D41	06/06/2025	8082A

Date/Time

06/10/25 5:55

Raw Sample Received by:

PL (Sot 164)

Raw Sample Relinquished by:

CPG

Date/Time

06/10/25

9:15

Raw Sample Received by:

PL (Sot 164)

Raw Sample Relinquished by:

PL (Sot 164)

Prep Standard - Chemical Standard Summary

Order ID : Q2267

Test : PCB

Prepbatch ID : PB168377,

Sequence ID/Qc Batch ID: po061025,

Standard ID :

EP2610,EP2620,PP24329,PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369,PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387,PP24461,PP24597,

Chemical ID :

E3551,E3804,E3877,E3917,E3932,E3938,E3939,M6157,P11522,P12699,P12702,P12931,P12936,P12949,P12955,P12957,P13356,P13357,P13373,P13381,P13589,P13591,P13697,P13702,P13830,P13878,P13883,W3112,W3177,



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2610	05/07/2025	11/07/2025	RUPESHKUMAR SHAH	Extraction_SCALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/07/2025
<u>FROM</u>	1000.00000ml of M6157 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2620	05/30/2025	07/01/2025	RUPESHKUMAR SHAH	Extraction_SCALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/30/2025
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24329	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP24330	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13697 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP24331	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP24332	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP24333	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24330 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP24334	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24332 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP24335	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13702 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP24336	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24335 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP24337	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24335 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP24338	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24335 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP24339	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24337 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP24340	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13878 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP24341	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24340 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP24342	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24340 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP24343	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24340 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP24344	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24342 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP24345	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P12931 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP24346	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.75000ml of PP24345 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP24347	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24345 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP24348	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24345 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP24349	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24347 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP24350	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P12936 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP24351	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24350 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP24352	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24350 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP24353	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24350 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP24354	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24352 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP24355	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13830 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP24356	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24355 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP24357	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24355 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP24358	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24355 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP24359	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24357 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP24360	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13883 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP24361	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24360 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP24362	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24360 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP24363	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24360 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP24364	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24362 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP24365	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.10000ml of P13381 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP24366	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.25000ml of W3177 + 0.75000ml of PP24365 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP24367	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24365 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP24368	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.75000ml of W3177 + 0.25000ml of PP24365 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP24369	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.90000ml of W3177 + 0.10000ml of PP24367 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP24370	03/18/2025	09/18/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12949 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP24371	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 98.50000ml of W3177 + 0.50000ml of PP24329 + 1.00000ml of PP24370 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP24372	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24371 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP24373	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13373 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1886	AR1221 500 PPB ICV	PP24374	03/18/2025	08/12/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of E3877 + 0.50000ml of W3177 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP24375	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12699 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP24376	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24375 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP24377	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13589 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP24378	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24377 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP24379	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P13591 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP24380	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24379 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP24381	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 1.00000ml of P12957 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP24382	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza 04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24381 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP24384	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P12702 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP24385	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24384 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP24386	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P11522 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP24387	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 0.50000ml of W3177 + 0.50000ml of PP24386 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP24461	04/11/2025	10/03/2025	Abdul Mirza	None	None	Yogesh Patel
								04/16/2025

FROM 0.50000ml of P12955 + 99.50000ml of E3917 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24597	05/20/2025	11/05/2025	Abdul Mirza	None	None	Yogesh Patel
								05/22/2025

FROM 1.00000ml of P13357 + 999.00000ml of E3932 = Final Quantity: 1000.000 ml

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	12/04/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	08/12/2025	02/12/2025 / Rajesh	02/12/2025 / Rajesh	E3877

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	10/03/2025	04/03/2025 / Rajesh	03/31/2025 / Rajesh	E3917

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	11/05/2025	05/05/2025 / RUPESH	04/23/2025 / RUPESH	E3932

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	/	05/14/2025 / RUPESH	E3938

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A2862010	11/22/2025	05/22/2025 / RUPESH	02/28/2025 / RUPESH	E3939

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	24i1262013	11/07/2025	05/07/2025 / RUPESH	02/18/2025 / Mohan	M6157

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	09/18/2025	03/18/2025 / yogesh	02/21/2022 / Ankita	P11522

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards,Inc	91867 / Aroclor 1232 100 ug/mL	020823	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12699

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards,Inc	x9166 / Aroclor 1262 100 ug/mL	060523	09/18/2025	03/18/2025 / yogesh	08/07/2023 / Ankita	P12702

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12931

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	09/18/2025	03/18/2025 / yogesh	12/07/2023 / Ankita	P12936

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	09/18/2025	03/18/2025 / yogesh	12/20/2023 / Yogesh	P12949

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	10/11/2025	04/11/2025 / Abdul	12/20/2023 / Yogesh	P12955

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/18/2025	03/18/2025 / yogesh	04/22/2024 / Abdul	P13356

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	11/20/2025	05/20/2025 / Abdul	04/22/2024 / Abdul	P13357

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	09/18/2025	03/18/2025 / yogesh	05/02/2024 / Ankita	P13373

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0207475	09/18/2025	03/18/2025 / yogesh	05/03/2024 / Abdul	P13381

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13589

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006726317	09/18/2025	03/18/2025 / yogesh	10/14/2024 / Ankita	P13591

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0210629	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13697

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0215270	09/18/2025	03/18/2025 / yogesh	10/17/2024 / yogesh	P13702

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0217391	09/18/2025	03/18/2025 / yogesh	12/09/2024 / Ankita	P13830

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0219655	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13878

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0220950	09/18/2025	03/18/2025 / yogesh	01/23/2025 / Ankita	P13883

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantorsTM**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd. by RP on 2/12/25

 E3877

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 03/31/25

E3917

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

RS

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3932

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3938

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 25A2862010
Manufactured Date: 2024-12-18
Expiration Date: 2026-03-19
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
Assay (CH ₂ Cl ₂) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	99.9 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Titration Acid (μ eq/g)	≤ 0.3	<0.1
Chloride (Cl)	≤ 10 ppm	<5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	<0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E3939

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium

avantor™



M6157
MS

Material No.: 9673-33

Batch No.: 24I1262013

Manufactured Date: 2024-08-07

Retest Date: 2029-08-06

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.2 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	<1 ppm
ACS – Substances Reducing Permanganate(as SO ₂)	<= 2 ppm	<2 ppm
Ammonium (NH ₄)	<= 1 ppm	<1 ppm
Chloride (Cl)	<= 0.1 ppm	<0.1 ppm
Nitrate (NO ₃)	<= 0.2 ppm	0.1 ppm
Phosphate (PO ₄)	<= 0.5 ppm	<0.1 ppm
Trace Impurities – Aluminum (Al)	<= 30.0 ppb	<5.0 ppb
Arsenic & Antimony (as As)	<= 4.0 ppb	<2.0 ppb
Trace Impurities – Boron (B)	<= 10.0 ppb	<5.0 ppb
Trace Impurities – Cadmium (Cd)	<= 2.0 ppb	<1.0 ppb
Trace Impurities – Chromium (Cr)	<= 6.0 ppb	<1.0 ppb
Trace Impurities – Cobalt (Co)	<= 0.5 ppb	<0.3 ppb
Trace Impurities – Copper (Cu)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Gold (Au)	<= 10.0 ppb	<5.0 ppb
Heavy Metals (as Pb)	<= 500.0 ppb	<100.0 ppb
Trace Impurities – Iron (Fe)	<= 50.0 ppb	<1.0 ppb
Trace Impurities – Lead (Pb)	<= 0.5 ppb	<0.5 ppb
Trace Impurities – Magnesium (Mg)	<= 7.0 ppb	<1.0 ppb
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	<0.1 ppb
Trace Impurities – Nickel (Ni)	<= 2.0 ppb	<0.3 ppb
Trace Impurities – Potassium (K)	<= 500.0 ppb	<10.0 ppb
Trace Impurities – Selenium (Se)	<= 50.0 ppb	7.2 ppb
Trace Impurities – Silicon (Si)	<= 100.0 ppb	12.8 ppb
Trace Impurities – Silver (Ag)	<= 1.0 ppb	<1.0 ppb

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

 **avantors**™



Material No.: 9673-33

Batch No.: 2411262013

Test	Specification	Result
Trace Impurities – Sodium (Na)	≤ 500.0 ppb	< 5.0 ppb
Trace Impurities – Strontium (Sr)	≤ 5.0 ppb	< 1.0 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	1.1 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	< 1.0 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration (µg/mL): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5µL, Range=3

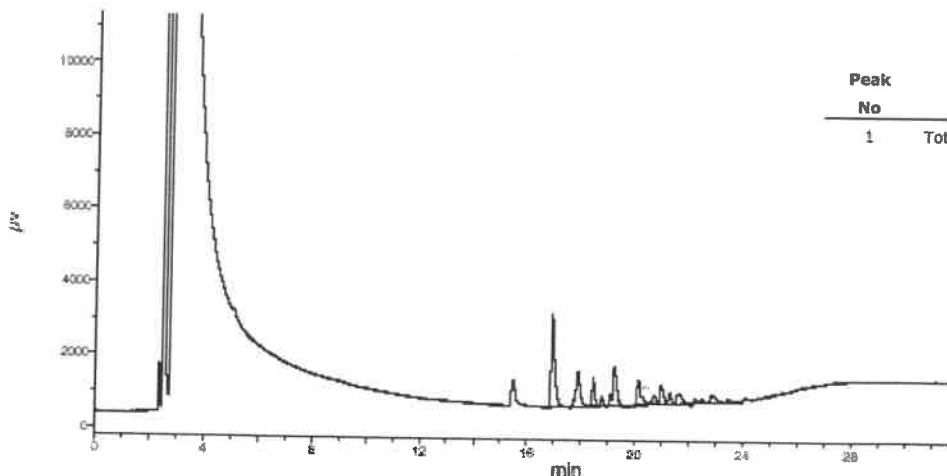




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

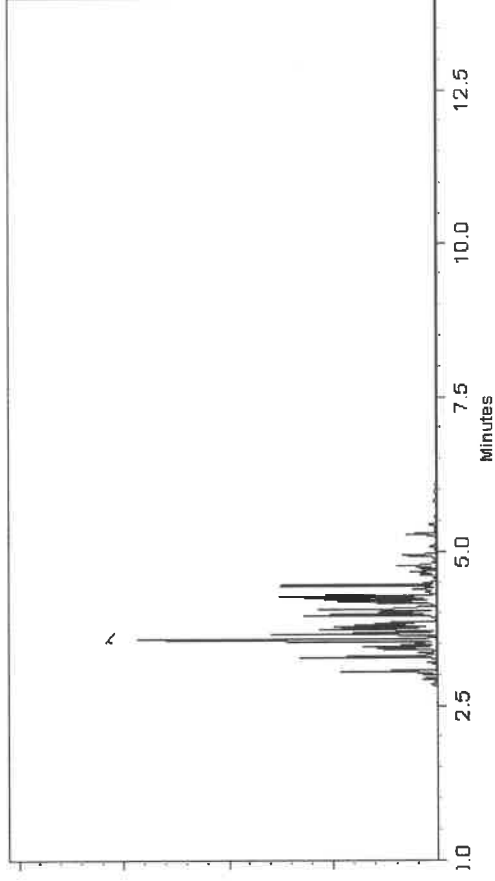

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023

Balance Serial #

B442140311

Jennifer Polino

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1219697
P1219697
A1
12104123

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

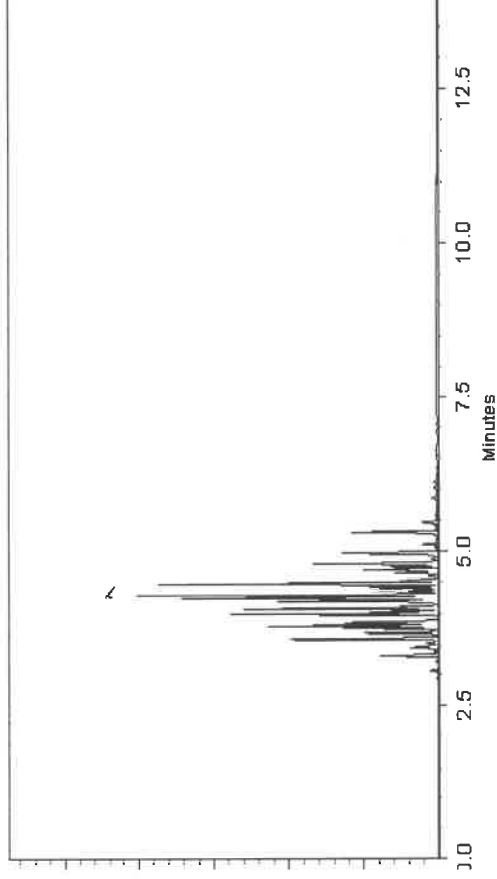

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#:
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE:
022023

DATE:
022023

Weight(s) shown below were combined and diluted to (mL):
200.0

Balance Uncertainty:
0.010

Flask Uncertainty:
0.010

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#:
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE:
022023

DATE:
022023

Weight(s) shown below were combined and diluted to (mL):
200.0


Balance Uncertainty:
0.010

Flask Uncertainty:
0.010

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

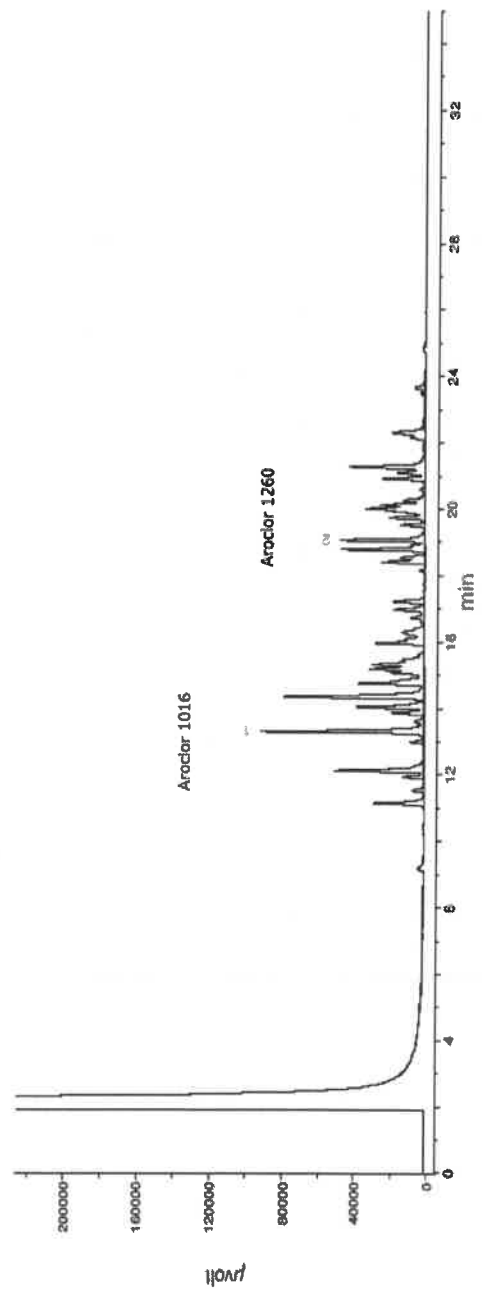



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Solvent(s):
Hexane

Lot#
273615

Lot Number:
022023

Formulated By:
Benson Chan

DATE
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Reviewed By:
Pedro L. Rentas

DATE
022023

Expiration Date:
022033

Expanded
Uncertainty
(+/-) (µg/mL)

4.0

Recommended Storage:
Ambient (20 °C)

Actual
Conc (µg/mL)

1002.8

Nominal Concentration (µg/mL):
1000

Actual
Weight(g)

0.20060

NIST Test ID#:
6UTB

Target
Weight(g)

0.20004

Weight(s) shown below were combined and diluted to (mL.):
200.0

Purity
(%)

100

5E-05 Balance Uncertainty

Balance Uncertainty

0.010

Flask Uncertainty

Flask Uncertainty


0.010

PR2946 718
↓
12/20/23
P12955

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

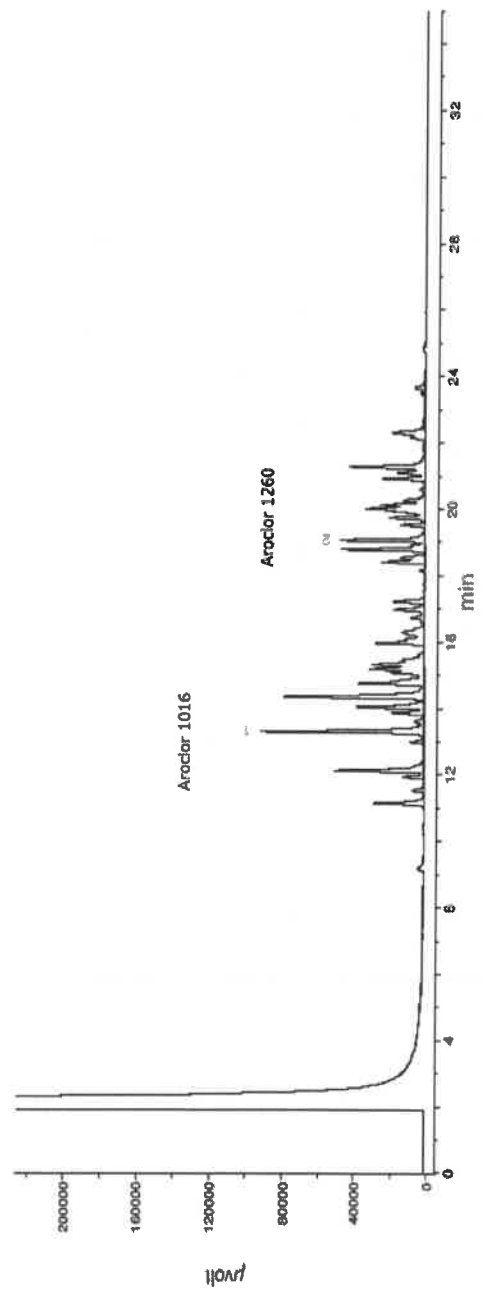



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Solvent(s): Iso-octane

Lot# 82227

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

5E-05 Balance Uncertainty
0.003 Flask Uncertainty

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE


P12956 / Y.P.
P12957 / 12/18/23

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
											(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA) LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	1003.3	100.1	1.8	11097-69-1	0.5mg/m3 (skin)	or-rat 1295mg/kg		

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 250 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = EDAQ Channel 1
Standard Injection = 1.5µL, Range = 3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

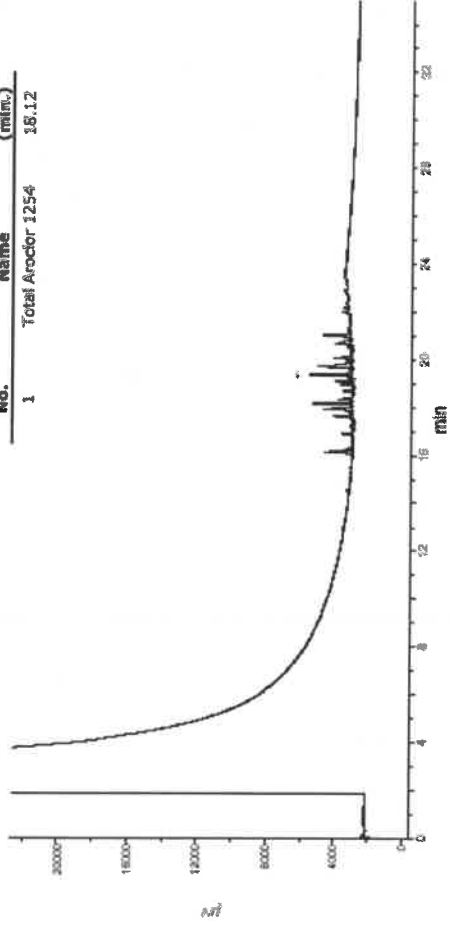



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

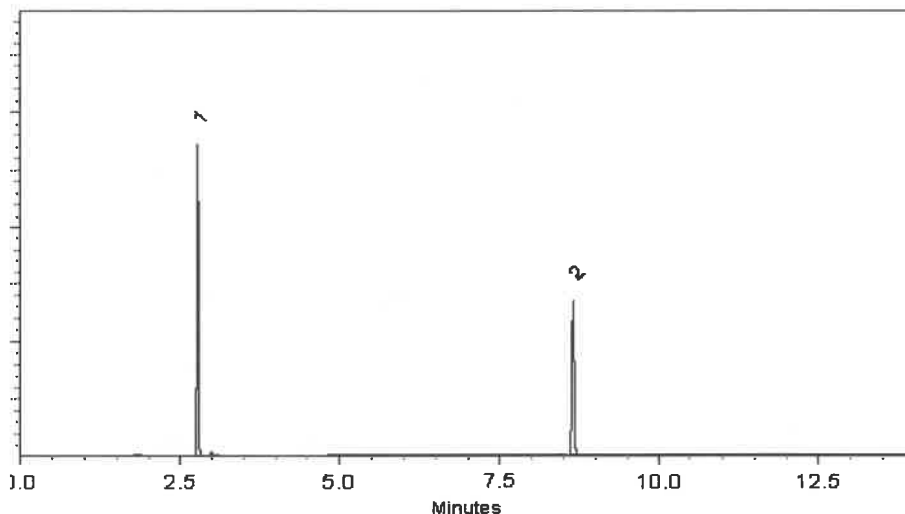


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

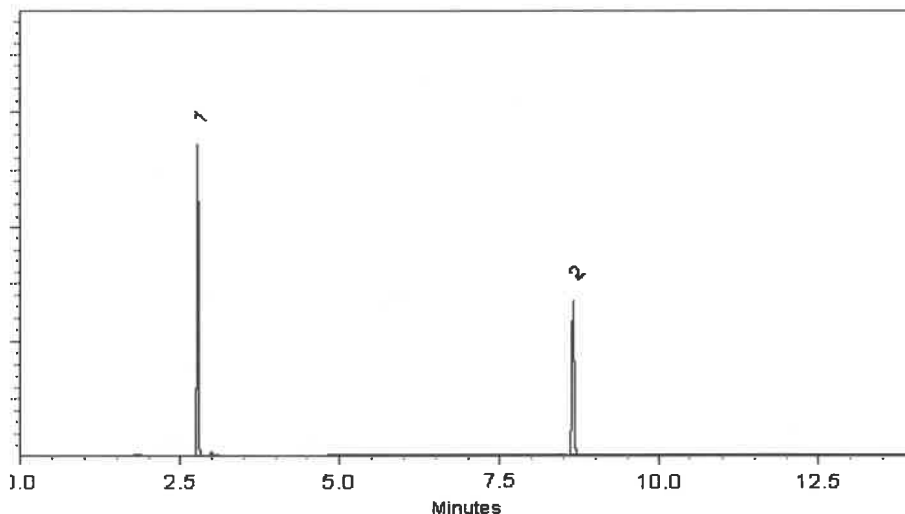


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
SAUF
04/25/2025



ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality


ISO 17025
Cert No. AT-1937



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 **Lot No.:** A0207475

Description : Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1268	11100-14-4	10947000	---%	1,000.0 µg/mL	+/- 55.4925

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 13380
↓
P 13381
↓
SAZU
05/6/2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

Split ratio 500:1

Inj. Vol

0.2µl

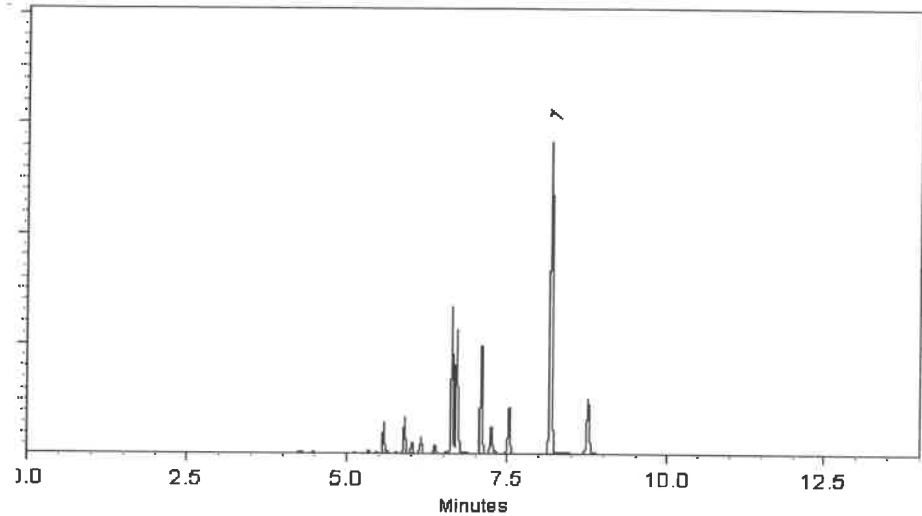

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 06-Feb-2024

Balance Serial # B442140311

Dylan Murphy
Dylan Murphy - Operations Technician I


Date Passed: 09-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13380 } ②
↓
P13381
1

[Signature]
05/6/2024

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1242	100.4	± 0.5 µg/mL	053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13589
↓
P13590AJ
10/14/24

ISO 17034



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

Reference Material Certificate
Product Information Sheet

Product Name: Aroclor 1248 Standard

Lot Number: 0006726317

Product Number: PP-342-1

Lot Issue Date: 27-Jan-2023

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 28-Feb-2031

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1248	100.3 ±	0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material (RM) standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above. Purity values are taken from approved vendor raw material certificates.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference (RM) standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference (RM) standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard (RM) is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13591
↓
P13592

AS
10/14/2024

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
QMS Representative



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 **Lot No.:** A0210629

Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13697
↓
P13701 } Y.P.
10/19/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1016	12674-11-2	07	----%	1,005.3 µg/mL	+/- 55.7809
2	Aroclor 1260	11096-82-5	1320657	----%	1,000.0 µg/mL	+/- 55.4850

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

0.2µl

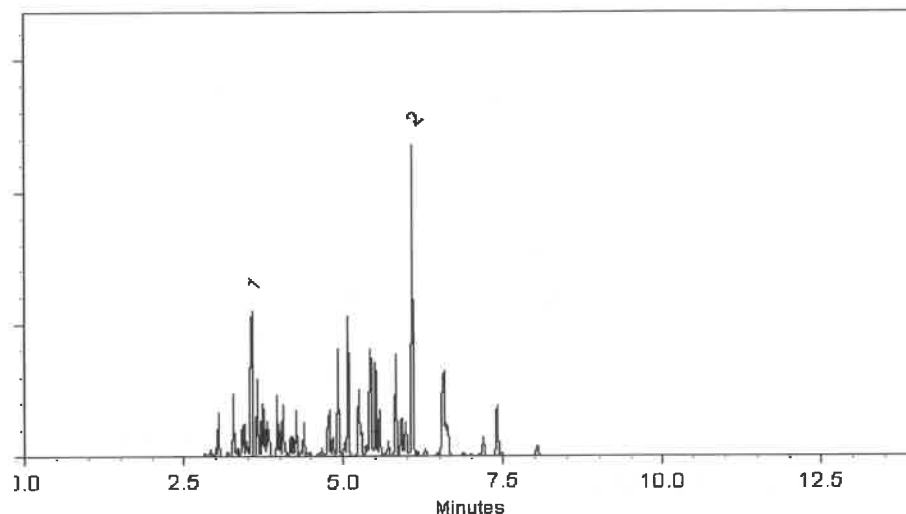


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Apr-2024

Balance Serial # B442140311


Dillan Murphy - Operations Technician I

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 **Lot No.:** A0215270

Description : Aroclor® 1221 Standard

Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P13902
P13703 } Y.P.
10/17/24

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1221	11104-28-2	14969200	----%	1,005.0 µg/mL	+/- 55.7700

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

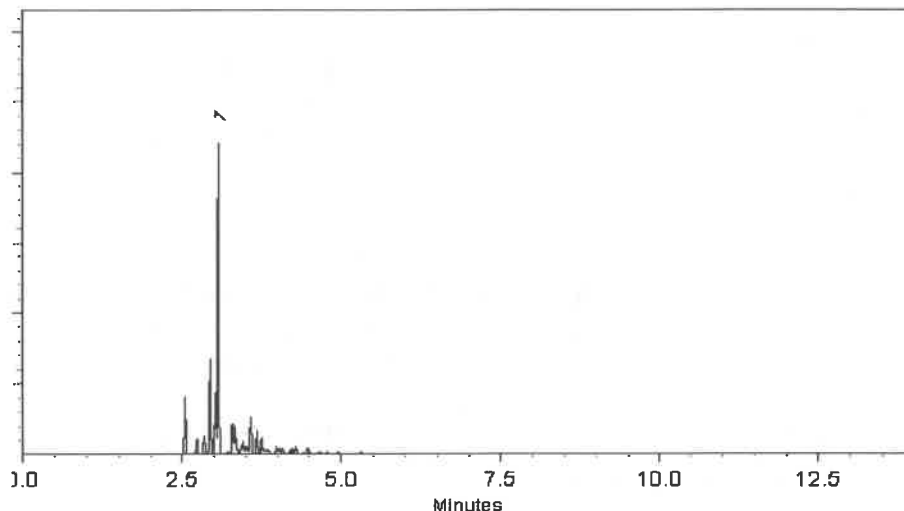

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 16-Aug-2024

Balance Serial # 1128360905

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 **Lot No.:** A0217391

Description : Aroclor® 1254 Standard

Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2031 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1254	11097-69-1	124-191-B	----%	1,004.7 µg/mL	+/- 55.7515

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P13830
↓
P13832
AJ
12/09/24

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

1µl

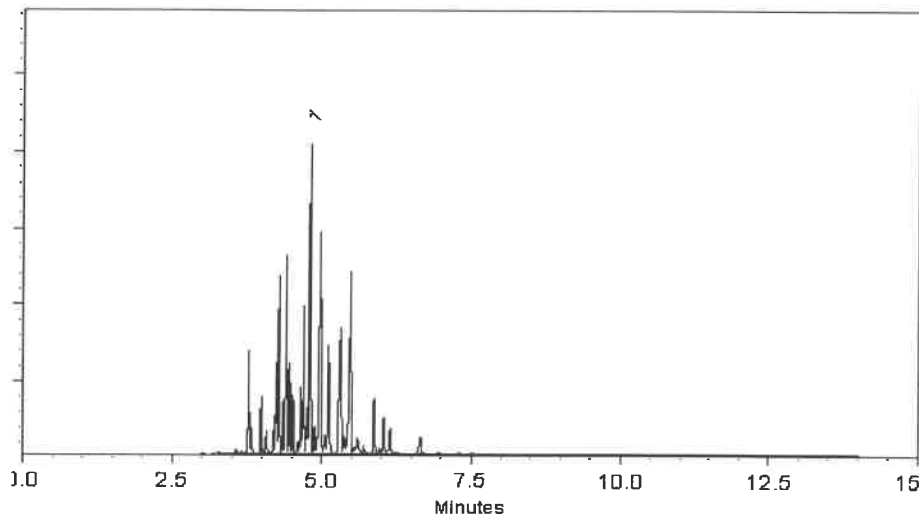

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Oct-2024

Balance Serial # C322230531

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 07-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008

Lot No.: A0219655

Description : Aroclor® 1232 Standard

Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : March 31, 2031

Storage: 25°C nominal

Handling:

This product contains PCBs.

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1232	11141-16-5	15665-01	---%	1,007.0 µg/mL	+/- 55.8810

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

P13878



AJ
01/28/25

P13880

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

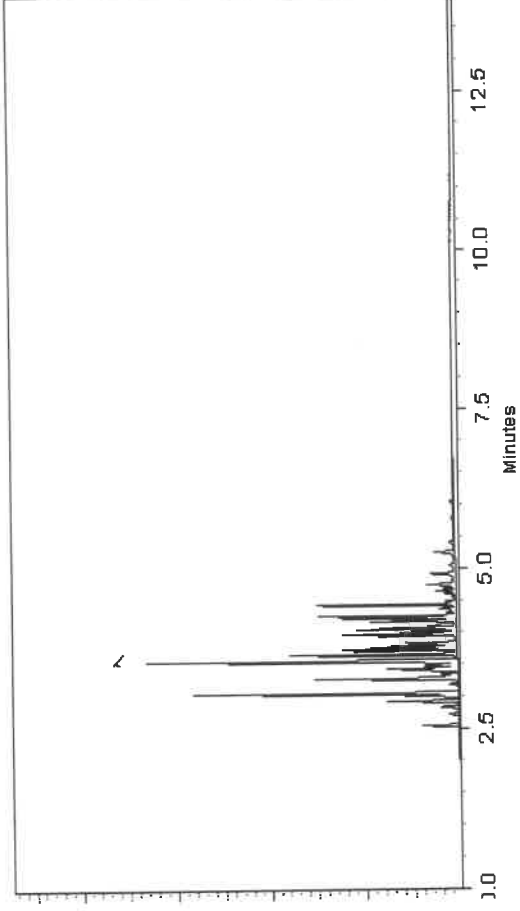

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Michael Maye
Michael Maye - Operations Tech I

Date Mixed: 02-Dec-2024

Balance Serial #

C322230531

Brittany Federhik
Brittany Federhiko - Operations Tech I

Date Passed: 05-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus

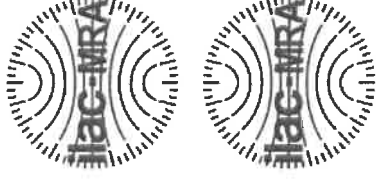

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32409 **Lot No.:** A0220950

Description: Aroclor® 1262 Standard

Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: April 30, 2031 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1262	37324-23-5	10849100	----%	1,002.0 µg/mL	+/- 55.6035

Solvent: Hexane

CAS # 110-54-3
Purity 99%

P13882

↓

AJ
01/28/25

P13883

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

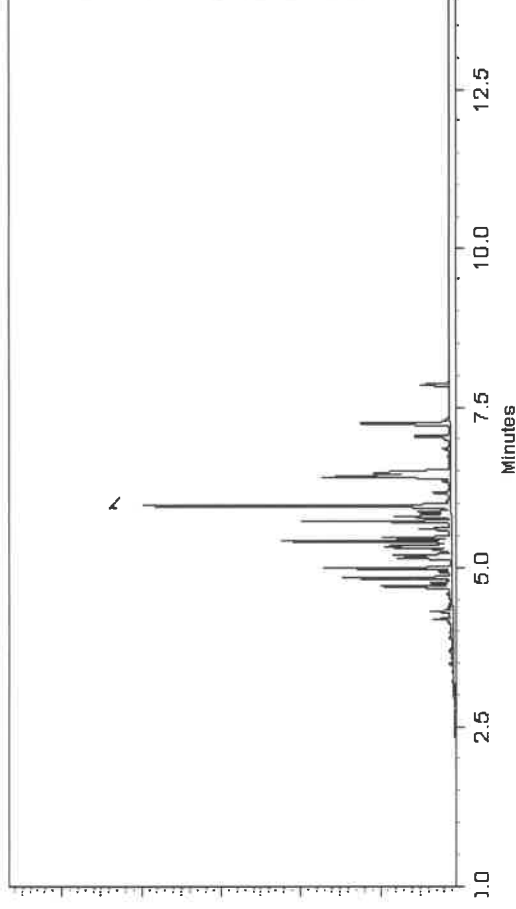

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckal - Mix Technician

Date Mixed: 09-Jan-2025 Balance Serial # C322230531



Britiany Federinko - Operations Tech I

Date Passed: 14-Jan-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production



SHIPPING DOCUMENTS

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Parsons

ADDRESS: 301 Plainfield Rd

CITY Syracuse

STATE: NY

ZIP: 13212

ATTENTION: Stephen Liberatore

PHONE: 315-418-8767

FAX: NA

CLIENT PROJECT INFORMATION

PROJECT NAME: Con Ed Atlantic Ave

PROJECT NO.: 453957-01000 LOCATION: Brooklyn, NY

PROJECT MANAGER: Stephen Liberatore

e-mail: Stephen.Liberatore@parsons.com

PHONE: 315-418-8767 FAX: NA

CLIENT BILLING INFORMATION

BILL TO: Parsons

PO#:

ADDRESS: 301 Plainfield Rd

CITY Syracuse

STATE: NY

ZIP: 13212

ATTENTION: Stephen Liberatore PHONE: 315-418-8767

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) 5 Day TAT DAYS*

HARDCOPY (DATA PACKAGE): DAYS*

EDD: DAYS*

*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)

☒ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP

☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B

+ Raw Data) ☐ Other

☐ EDD FORMAT

TCLP VOCs
TCLP SVOCs
PCB
Flash point
TCLP Extraction
TCLP metals/mercury
PH reactive solids
reactive solids

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES							COMMENTS	
			COMP	GRAB	DATE	TIME		E	E	E	E	E	E	E	← Specify Preservatives A-HCl D-NaOH B-HNO3 E-ICE C-H2SO4 F-OTHER	
1.	WC-20250605	W		X	6/5/25	1520	8	X	X	X	X	X	X	X		
2.																
3.																
4.																
5.																
6.																
7.																
8.																
9.																
10.																

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP
1. <u>Ym M</u>	<u>6-5-25/1330</u>	<u>[Signature]</u> <u>1330</u>	<u>3.0</u> °C
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	Comments: <u>Please CC kirsten.valentini@parsons.com</u>
2. <u>[Signature]</u>		<u>[Signature]</u>	
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	
3. <u>[Signature]</u>	<u>6-6-25</u>	<u>[Signature]</u>	

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488