


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050276.D
Acq On : 11 Jun 2025 15:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 11:54:38 2025

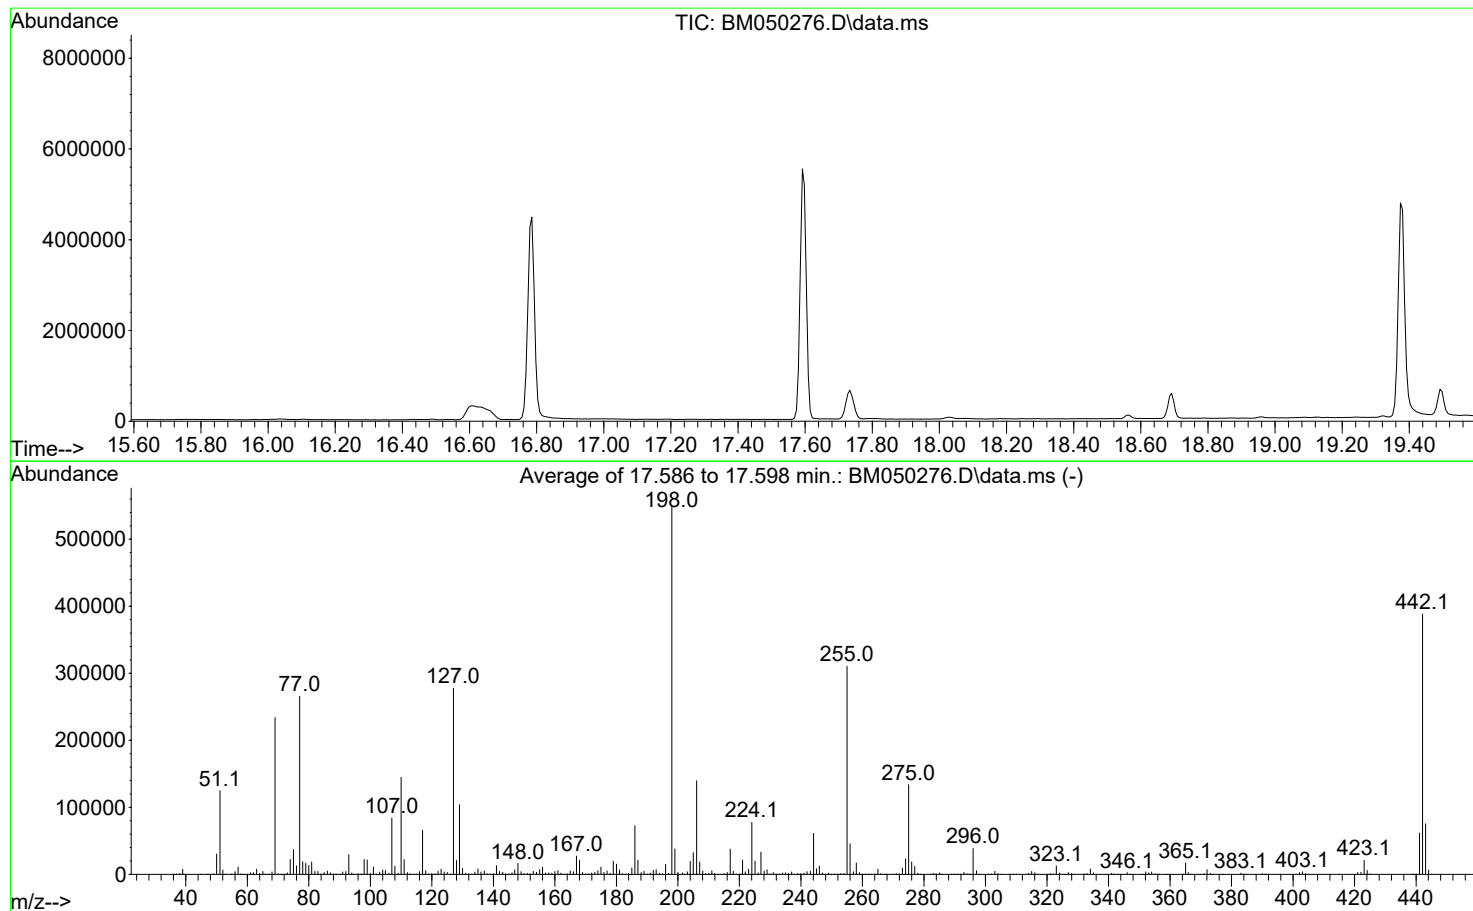

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	124833	PASS
68	69	0.00	2	1.5	3603	PASS
69	198	0.00	100	42.6	233985	PASS
70	69	0.00	2	0.4	1012	PASS
127	198	10	80	50.6	277675	PASS
197	198	0.00	2	0.3	1432	PASS
198	198	100	100	100.0	548821	PASS
199	198	5	9	6.9	37939	PASS
275	198	10	60	24.4	133920	PASS
365	198	1	100	3.1	16999	PASS
441	198	0.01	100	11.2	61619	PASS
442	442	50	100	100.0	388501	PASS
443	442	15	24	19.4	75376	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/11/2025	BNA_M	<u>BM050276.D</u>
Compound Name	Response	Retention Time
DDT	1741494	20.621
DDD	20318	20.233
DDE	2850	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23168	1764662	1.31

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050276.D
Acq On : 11 Jun 2025 15:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 11 18:44:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

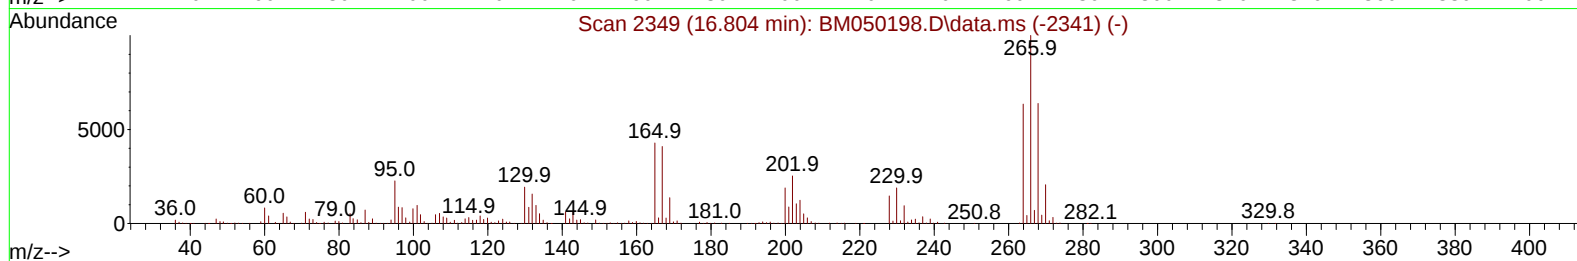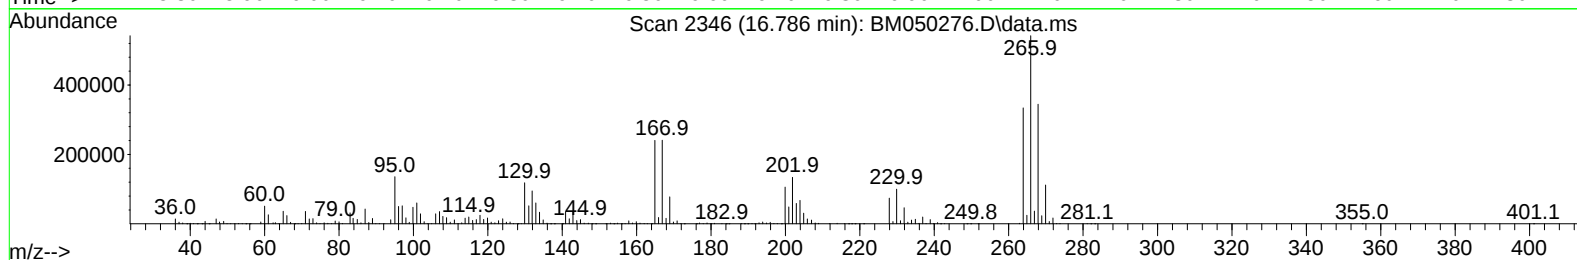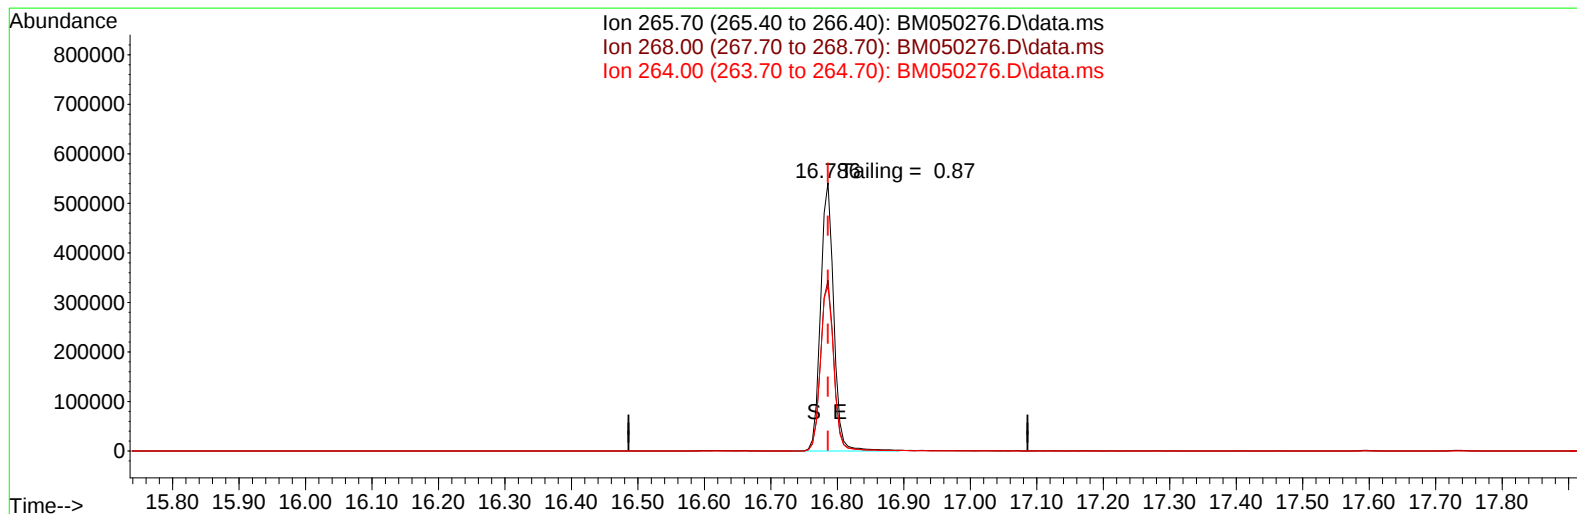

TIC: BM050276.D\data.ms

(70) Pentachlorophenol (C)

16.786min (-0.000) 1703653.44 ng




response 745212

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.56
264.00	63.50	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050276.D
Acq On : 11 Jun 2025 15:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 11 18:44:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

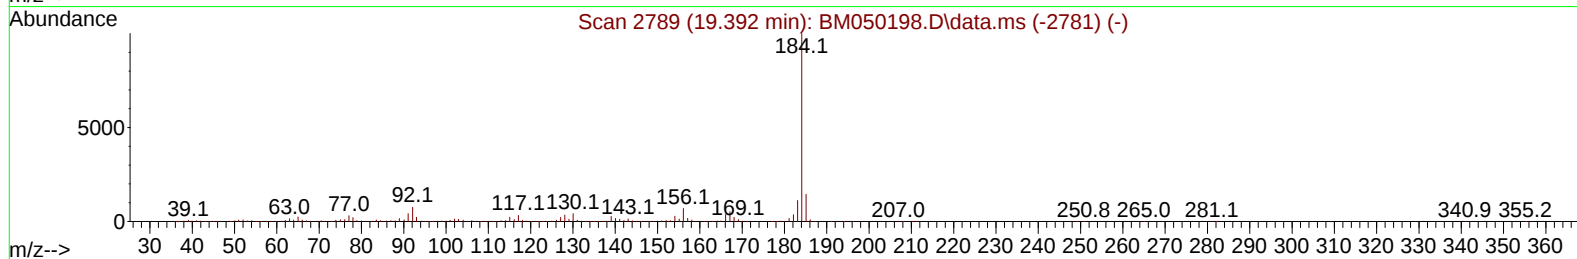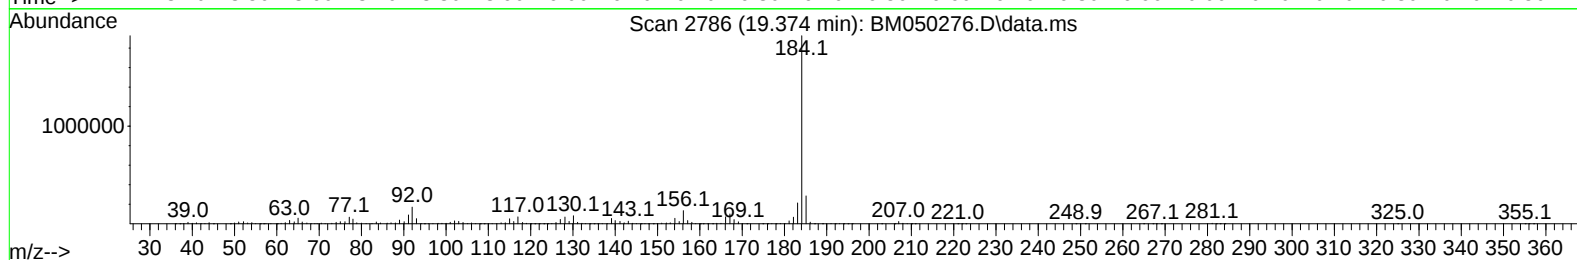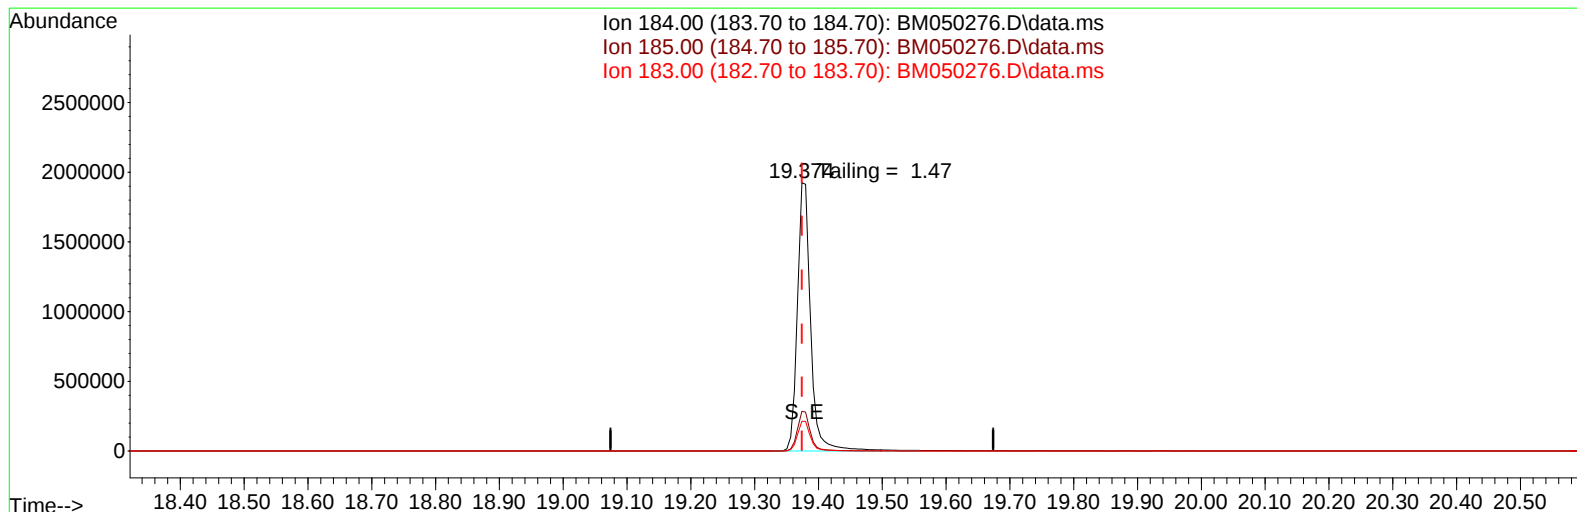

TIC: BM050276.D\data.ms

(77) Benzidine

19.374min (-0.000) 2147.98 ng

response 2793632

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.78
183.00	11.20	11.11
0.00	0.00	0.00