


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050293.D
Acq On : 12 Jun 2025 03:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 09 11:54:38 2025

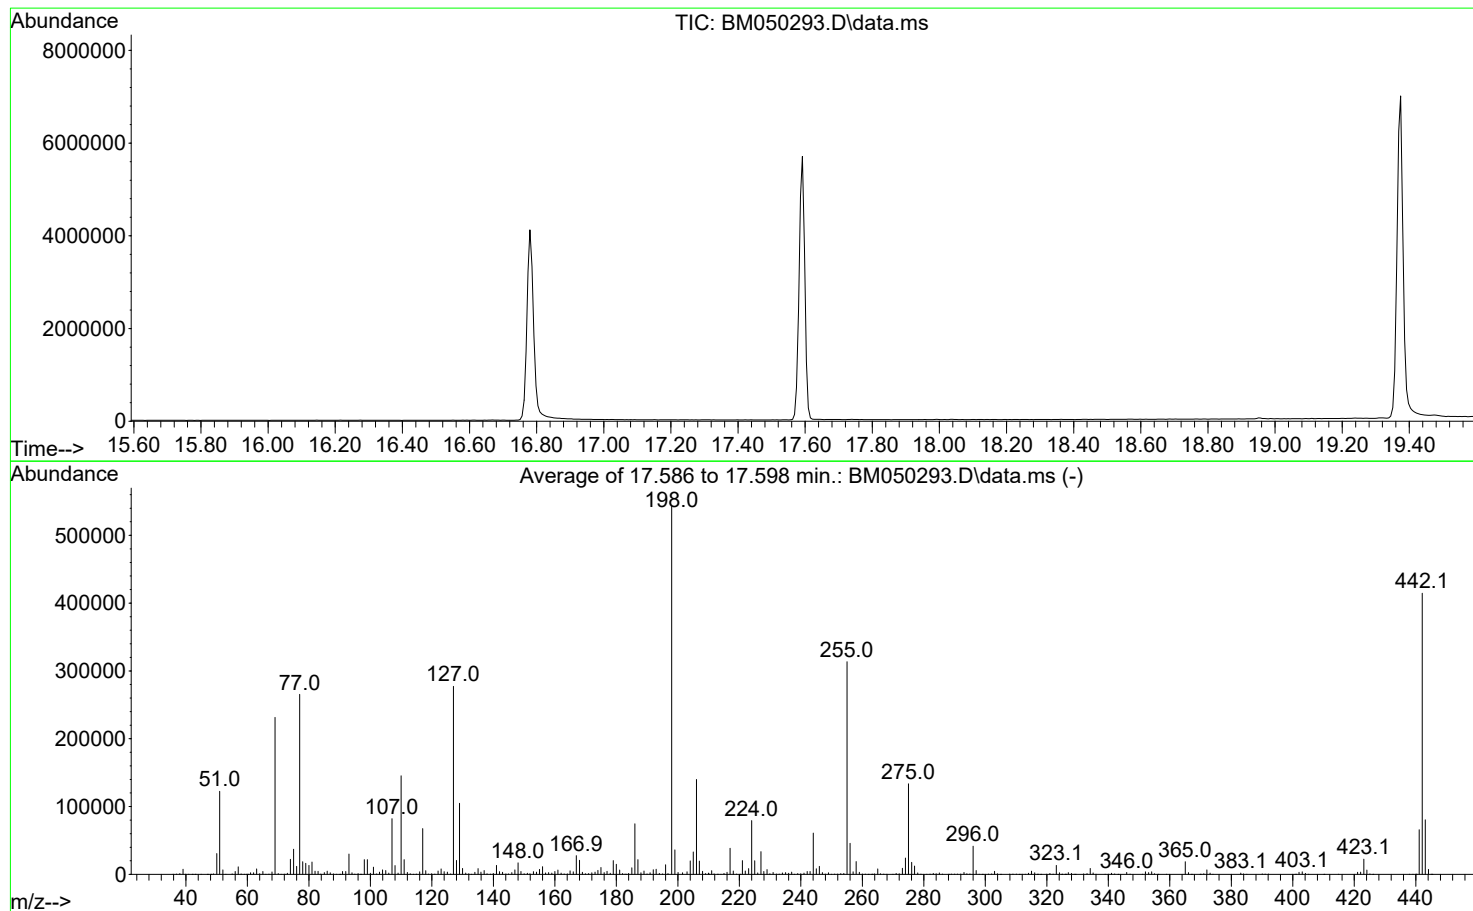

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	22.6	122571	PASS
68	69	0.00	2	1.5	3537	PASS
69	198	0.00	100	42.7	231531	PASS
70	69	0.00	2	0.5	1188	PASS
127	198	10	80	51.1	277333	PASS
197	198	0.00	2	0.2	1296	PASS
198	198	100	100	100.0	542507	PASS
199	198	5	9	6.7	36229	PASS
275	198	10	60	24.6	133573	PASS
365	198	1	100	3.4	18647	PASS
441	198	0.01	100	12.2	65955	PASS
442	442	50	100	100.0	414592	PASS
443	442	15	24	19.4	80435	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/11/2025	BNA_M	<u>BM050293.D</u>
Compound Name	Response	Retention Time
DDT	1783815	20.615
DDD	17796	20.227
DDE	2037	19.668
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19833	1803648	1.10

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050293.D
Acq On : 12 Jun 2025 03:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 12 05:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

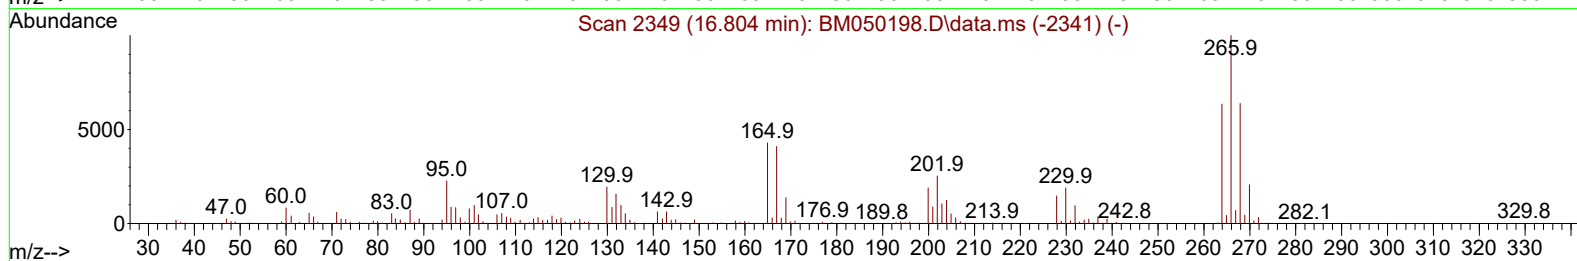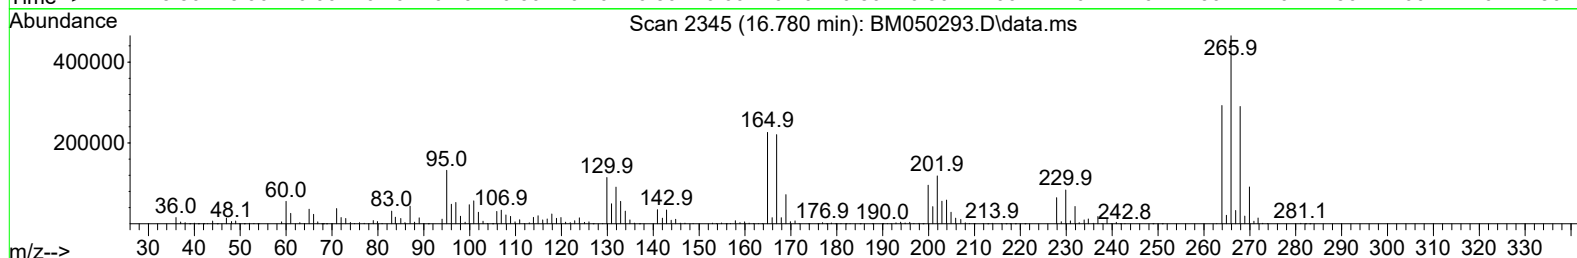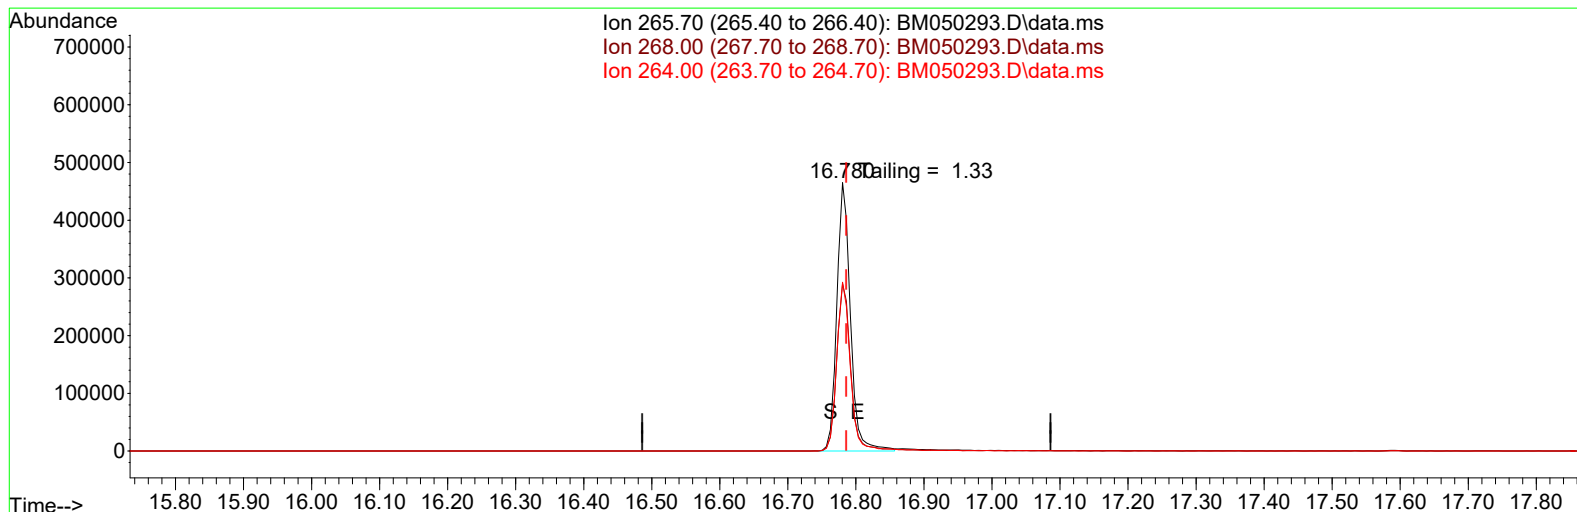

TIC: BM050293.D\data.ms

(70) Pentachlorophenol (C)

16.780min (-0.006) 258016.11 ng




response 647908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.36
264.00	63.50	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061125\
Data File : BM050293.D
Acq On : 12 Jun 2025 03:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 12 05:28:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 09 11:54:38 2025
Response via : Initial Calibration

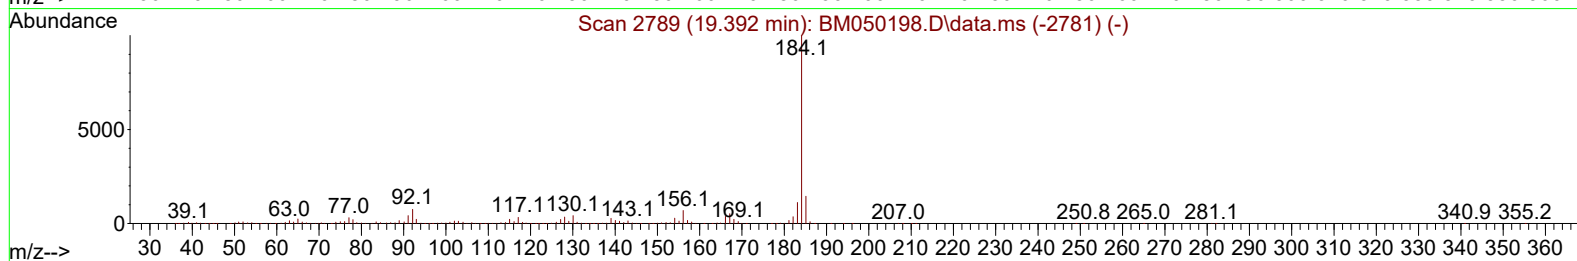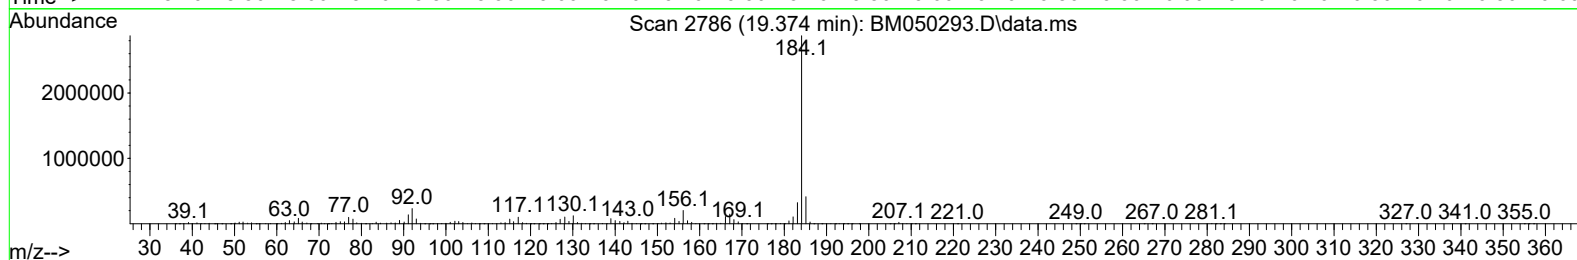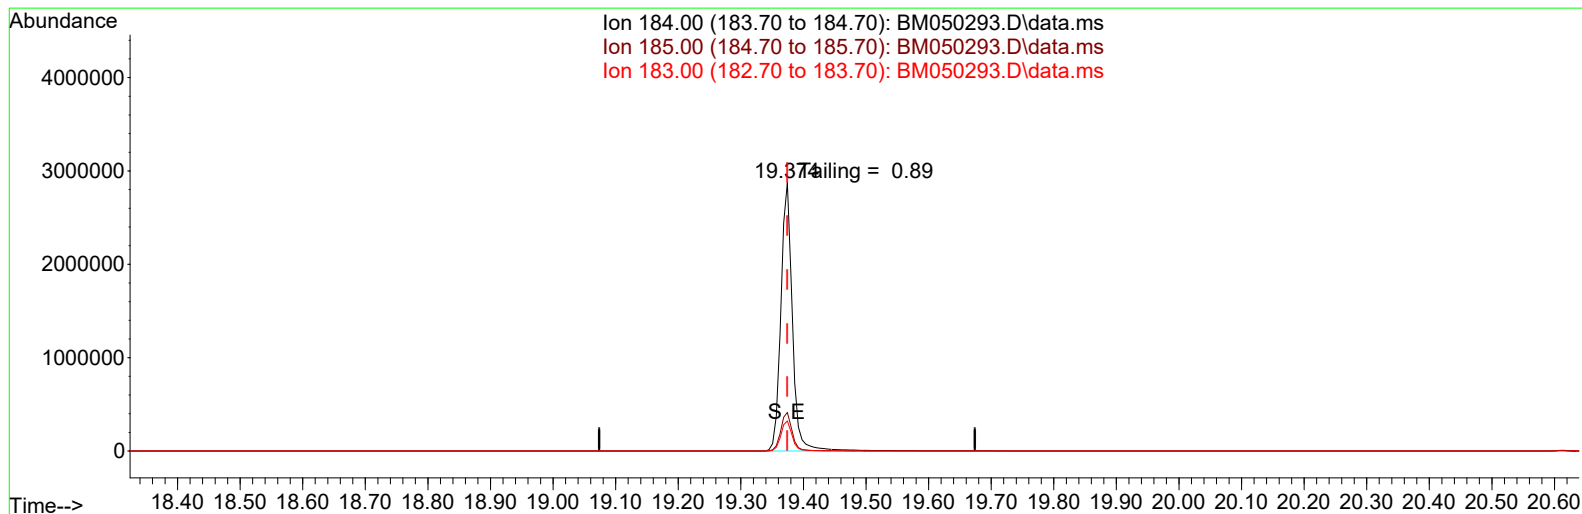

TIC: BM050293.D\data.ms

(77) Benzidine

19.374min (+ 0.000) 81131.91 ng

response 3702866

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.37
183.00	11.20	11.22
0.00	0.00	0.00