


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060625\
Data File : VX046516.D
Acq On : 06 Jun 2025 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Title : SW846 8260
Last Update : Fri Jun 06 16:56:12 2025

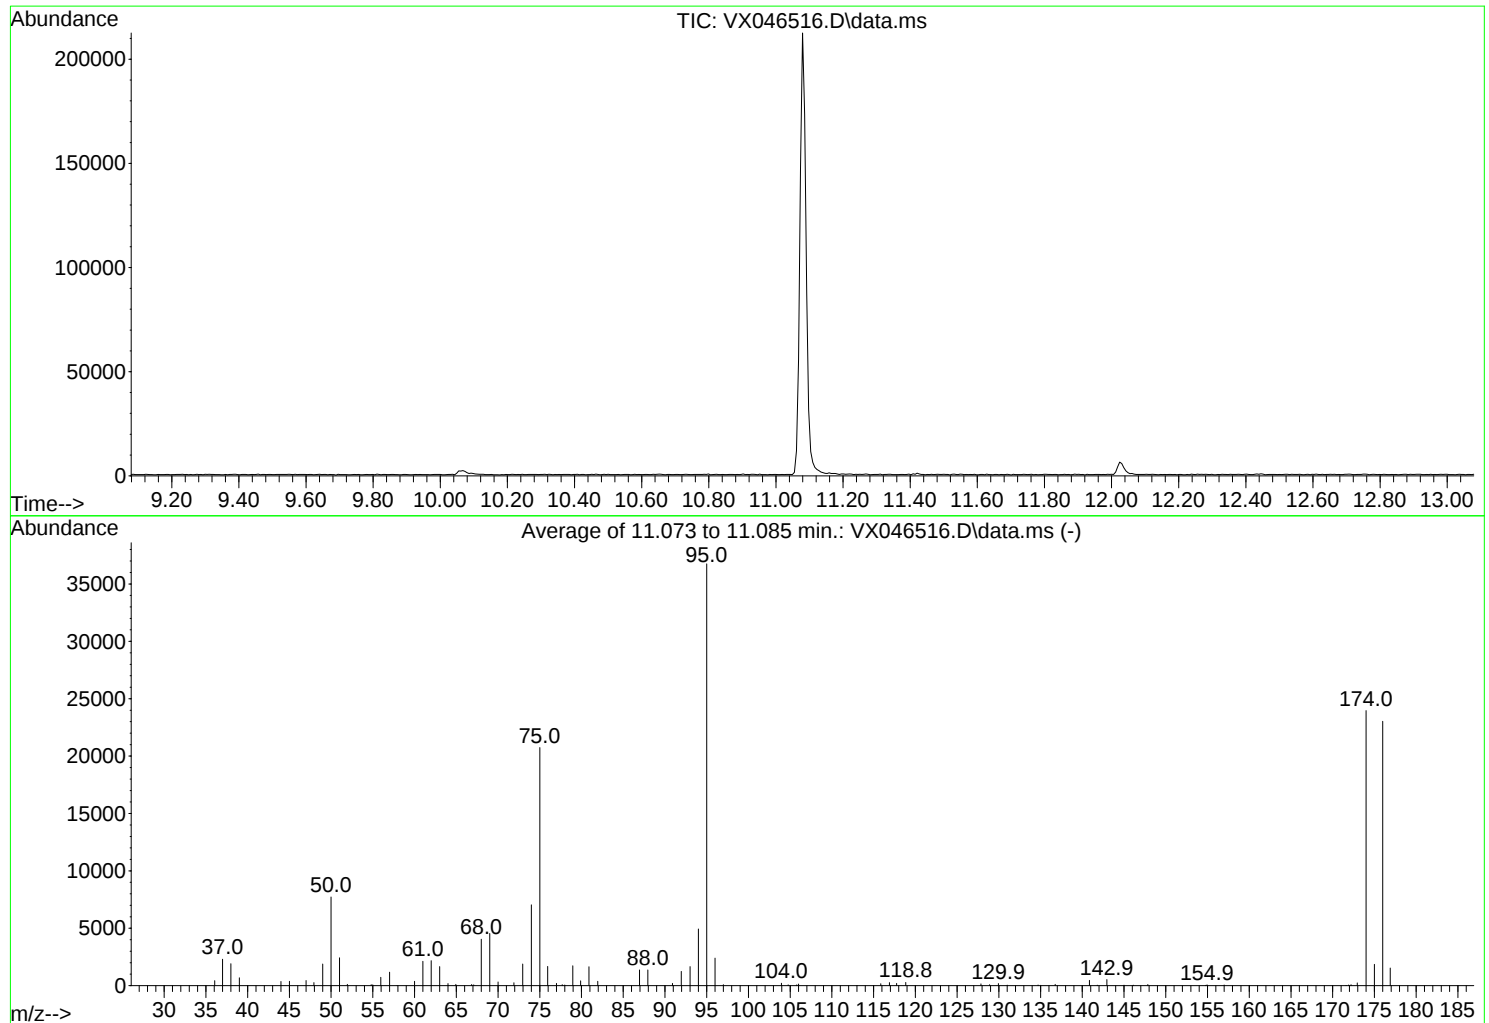

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	7727	PASS
75	95	30	60	56.5	20747	PASS
95	95	100	100	100.0	36752	PASS
96	95	5	9	6.5	2397	PASS
173	174	0.00	2	1.0	238	PASS
174	95	50	100	65.2	23963	PASS
175	174	5	9	7.7	1850	PASS
176	174	95	101	96.1	23028	PASS
177	176	5	9	6.6	1530	PASS