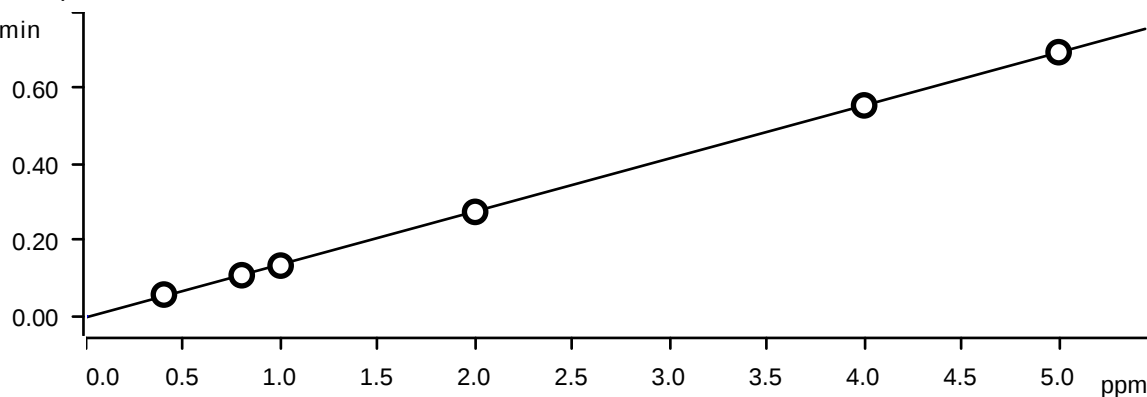


Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-052225	10 NF/IZ
STD2	0.4300	0.6400	0.6490	2.1290	0.5430	1.0980	3.2870	IC1-052225	10 NF/IZ
STD3	0.7950	1.2070	1.2050	4.0180	1.0040	1.8670	6.0690	IC1-052225	10 NF/IZ
STD4	0.9770	1.4800	1.4790	4.9290	1.2290	2.4770	7.4150	IC1-052225	10 NF/IZ
STD5	1.9910	2.9680	2.9600	9.9160	2.4670	5.1100	14.6210	IC1-052225	10 NF/IZ
STD6	4.0010	5.9670	5.9590	19.8680	4.9660	9.8700	29.8480	IC1-052225	10 NF/IZ
STD7	5.0060	7.5390	7.5480	25.1400	6.2900	12.5780	37.2600	IC1-052225	10 NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		5/22/2025 11:09
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		5/22/2025 11:30
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		5/22/2025 11:52
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		5/22/2025 12:13
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		5/22/2025 12:35
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		5/22/2025 12:56
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		5/22/2025 13:17
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1	7.5000	6.6667	8.1667	6.4500	8.6000	9.8000	9.5667		
STD2	-0.6250	0.5833	0.4167	0.4500	0.4000	-6.6500	1.1500		
STD3	-2.3000	-1.3333	-1.4000	-1.4200	-1.6800	-0.9200	-1.1333		
STD4	-0.4500	-1.0667	-1.3333	-0.8400	-1.3200	2.2000	-2.5267		
STD5	0.0250	-0.5500	-0.6833	-0.6600	-0.6800	-1.3000	-0.5067		
STD6	0.1200	0.5200	0.6400	0.5600	0.6400	0.6240	0.7027		

Fluoride (Anions)


 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -2.82659E-3 + 0.0139492 \times Q$

Relative standard deviation 0.920519 %

Correlation coefficient 0.999955

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.108	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.133	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.275	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.555	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.695	STD7	2025-05-22 13:17:57 UTC-4	used

Chloride (Anions)

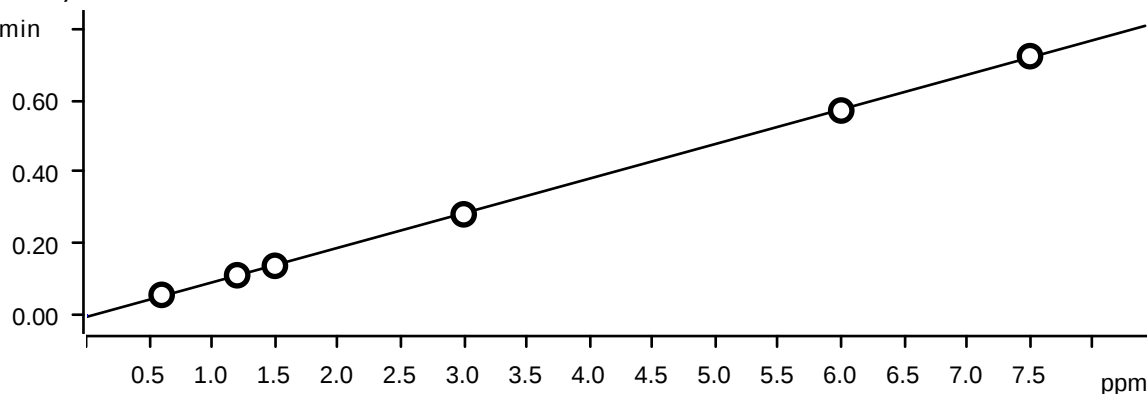 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -4.33057E-3 + 9.64673E-3 \times Q$


Relative standard deviation 1.154335 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.138	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.282	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.571	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.723	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

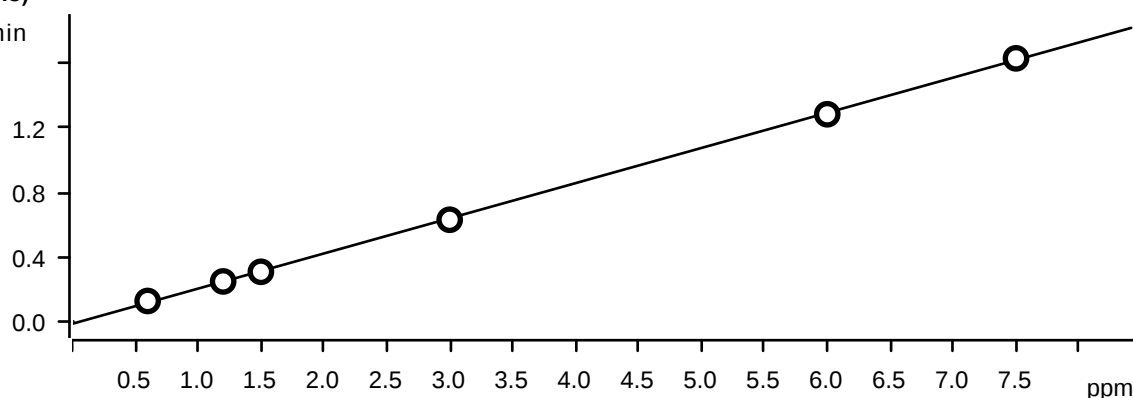Function: $A = -0.0150155 + 0.0217890 \times Q$


Relative standard deviation 1.428639 %

Correlation coefficient 0.999893

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.307	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.630	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.283	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.630	STD7	2025-05-22 13:17:57 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

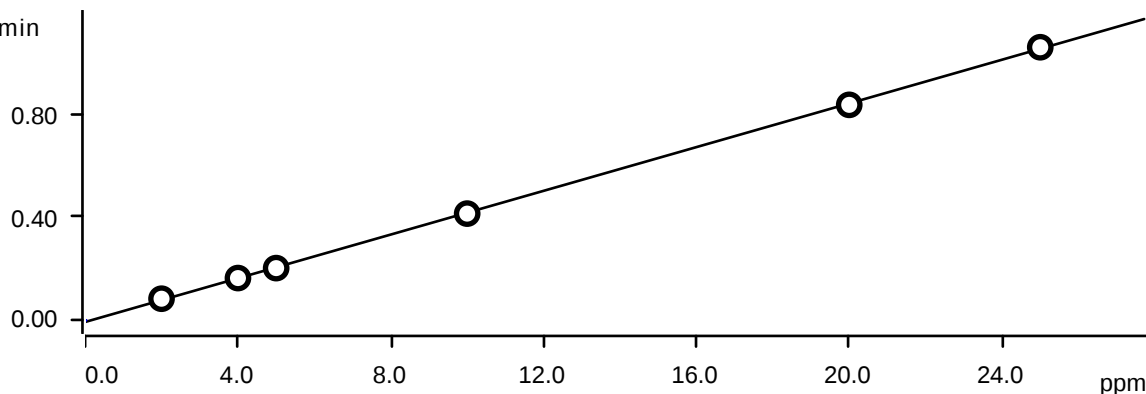

Function: $A = -6.27114E-3 + 4.23162E-3 \times Q$


Relative standard deviation: 1.185575 %

Correlation coefficient: 0.999925

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.164	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.202	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.413	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.834	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.058	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

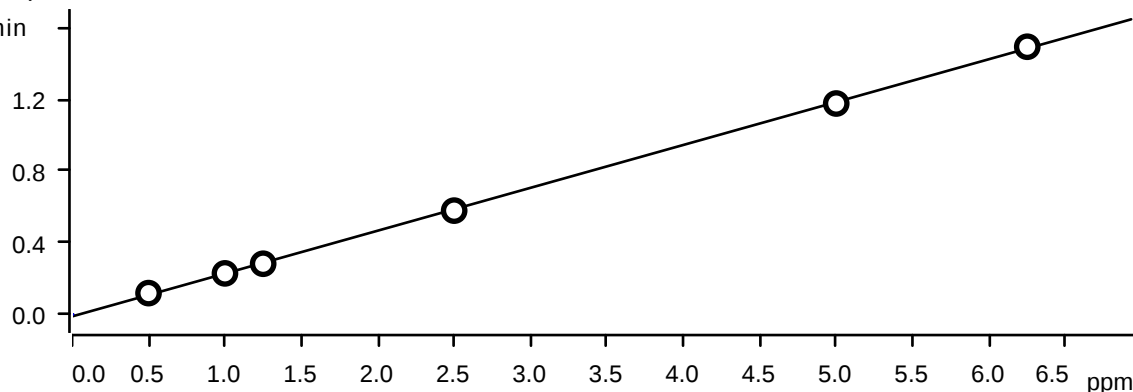


Function: $A = -0.0109593 + 0.0239055 \times Q$

Relative standard deviation: 1.451672 %

Correlation coefficient 0.999889

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.119	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.283	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.176	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.493	STD7	2025-05-22 13:17:57 UTC-4	used

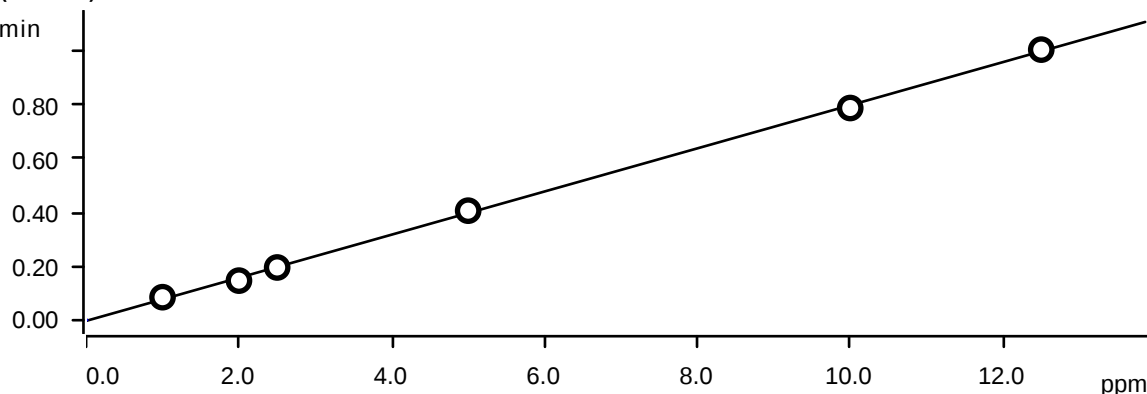
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.02035E-3 + 8.01761E-3 \times Q$

Relative standard deviation 2.297726 %

Correlation coefficient 0.999716

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.085	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.147	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.196	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.407	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.788	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.005	STD7	2025-05-22 13:17:57 UTC-4	used

Sulfate (Anions)

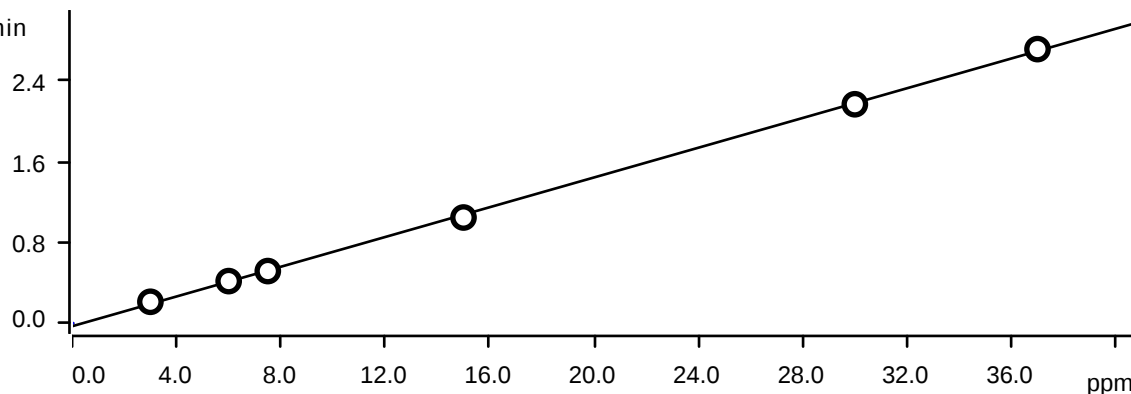 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0303663 + 7.37295E-3 \times Q$

Relative standard deviation 1.792871 %

Correlation coefficient 0.999832


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.417	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.516	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.048	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.170	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.717	STD7	2025-05-22 13:17:57 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-05-22 11:09:38 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

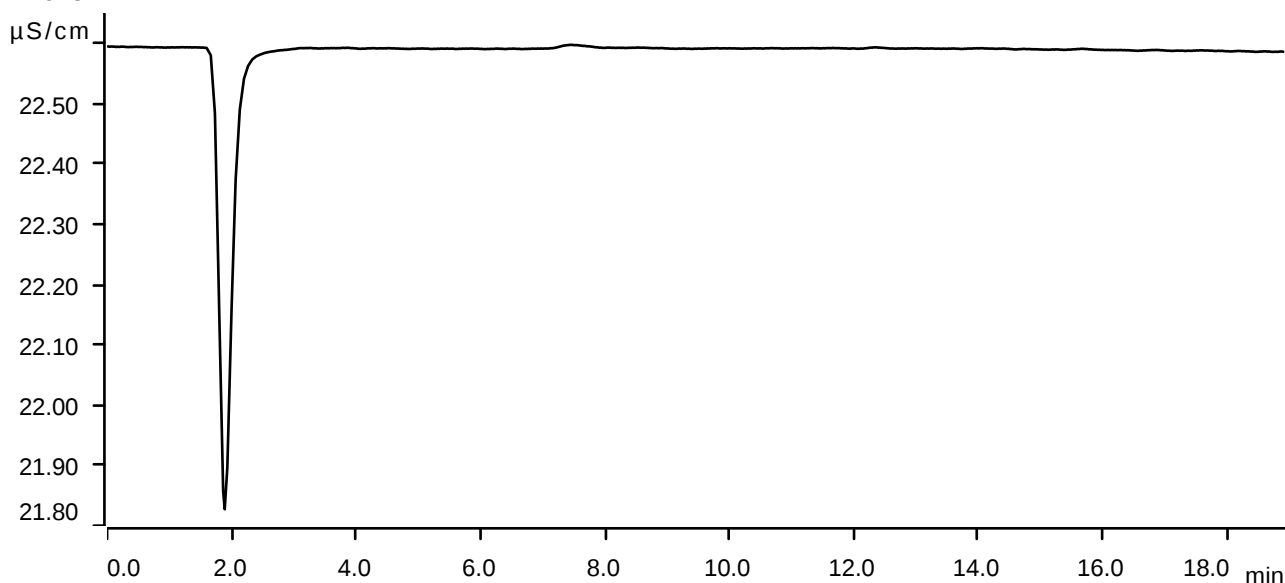Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-05-22 11:30:53 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

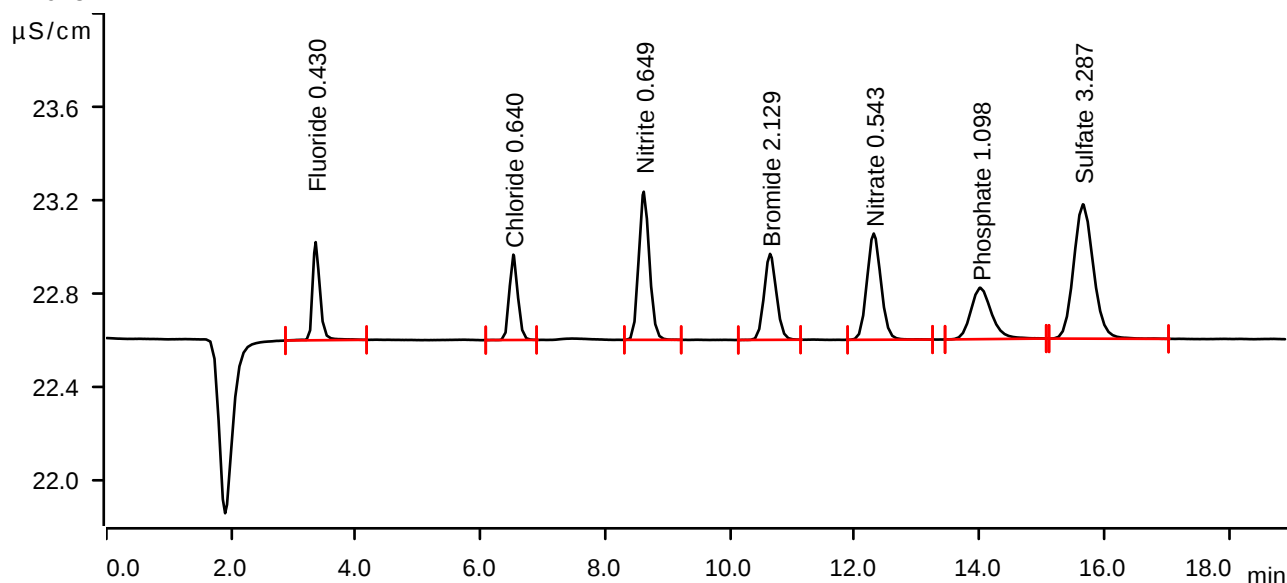

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0572	0.421	0.430	Fluoride
2	6.525	0.0574	0.366	0.640	Chloride
3	8.617	0.1264	0.636	0.649	Nitrite
4	10.642	0.0838	0.369	2.129	Bromide
5	12.303	0.1190	0.456	0.543	Nitrate
6	14.013	0.0850	0.221	1.098	Phosphate
7	15.657	0.2120	0.577	3.287	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-05-22 11:52:16 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

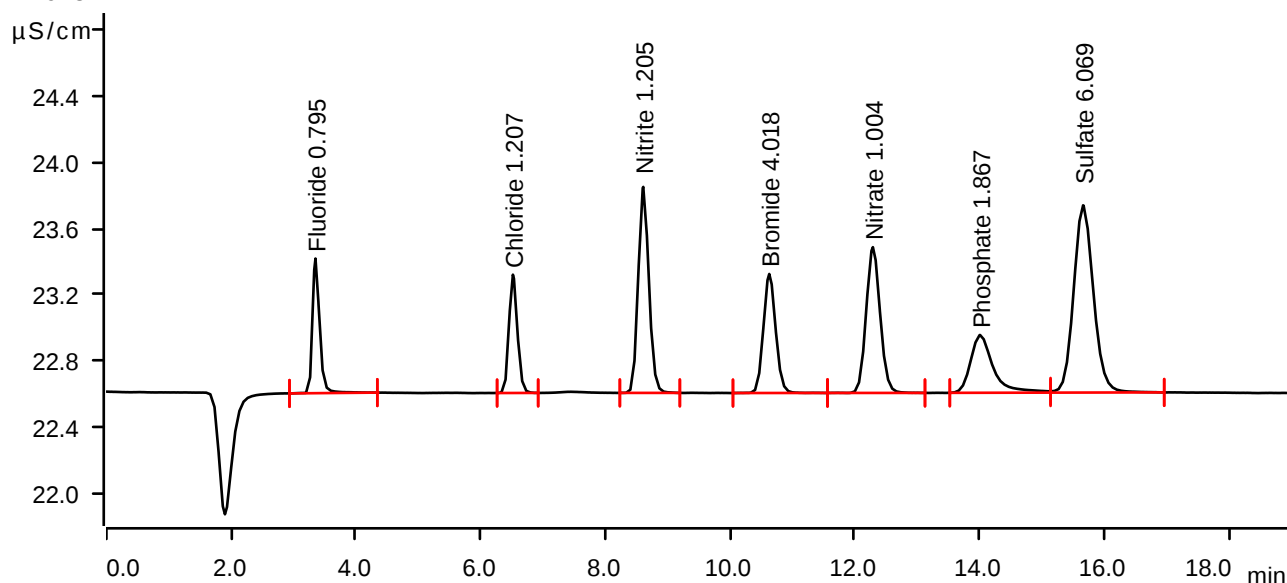

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1081	0.814	0.795	Fluoride
2	6.518	0.1121	0.716	1.207	Chloride
3	8.608	0.2475	1.247	1.205	Nitrite
4	10.628	0.1637	0.720	4.018	Bromide
5	12.290	0.2290	0.882	1.004	Nitrate
6	14.008	0.1467	0.350	1.867	Phosphate
7	15.660	0.4171	1.133	6.069	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-05-22 12:13:41 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

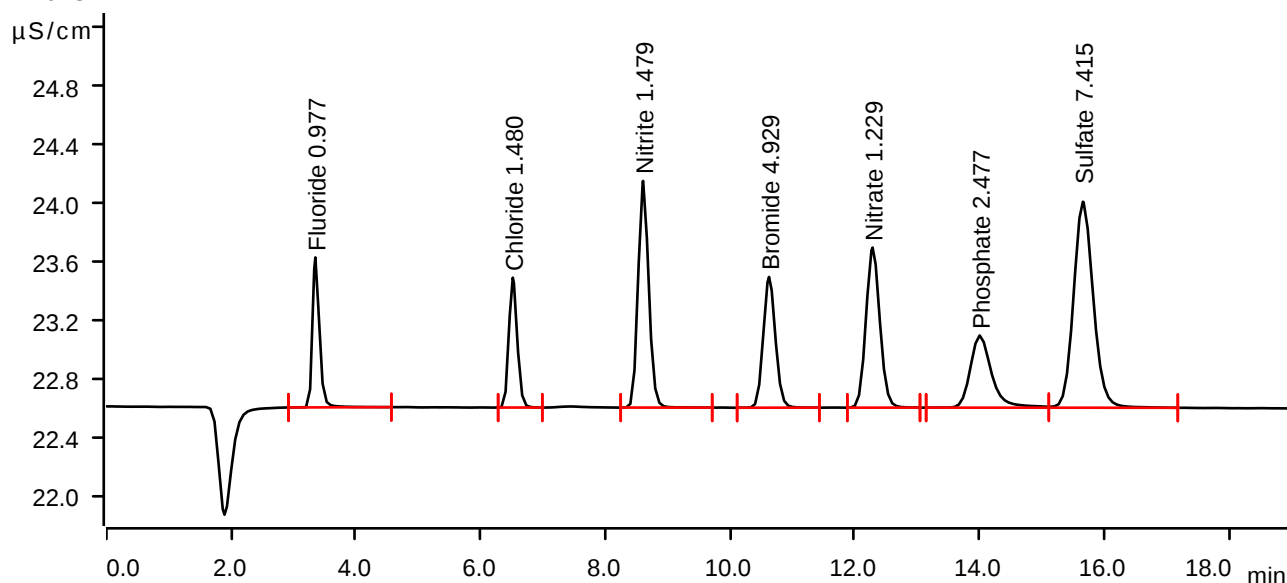

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.1334	1.024	0.977	Fluoride
2	6.517	0.1384	0.888	1.480	Chloride
3	8.607	0.3073	1.549	1.479	Nitrite
4	10.625	0.2023	0.894	4.929	Bromide
5	12.285	0.2828	1.094	1.229	Nitrate
6	14.003	0.1955	0.493	2.477	Phosphate
7	15.657	0.5164	1.408	7.415	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-05-22 12:35:06 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

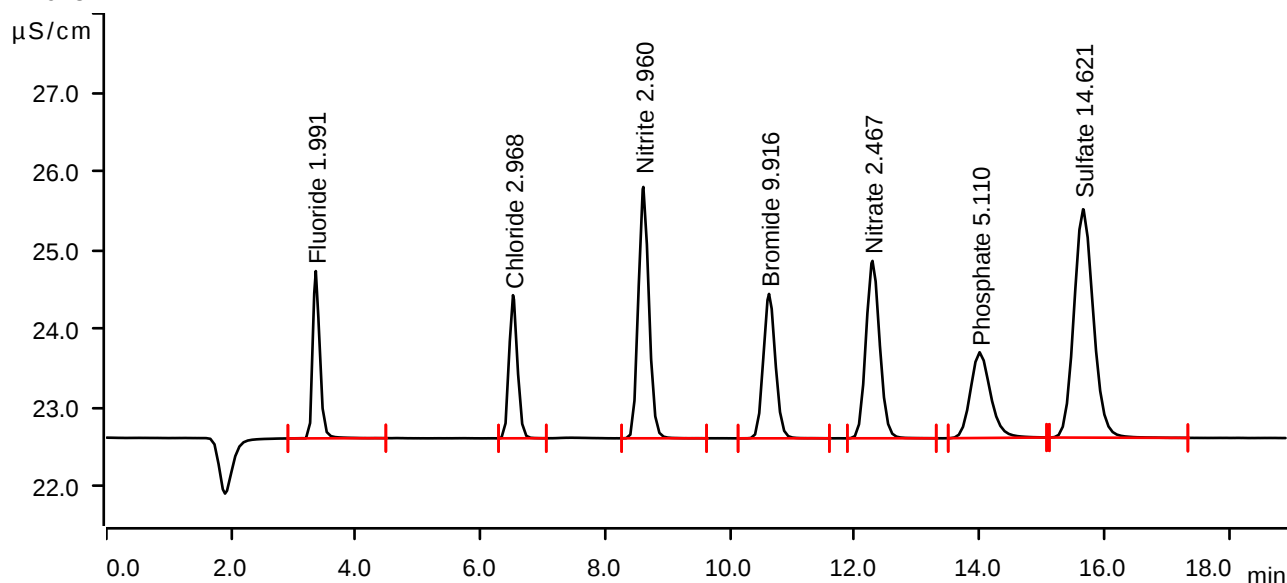

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2749	2.123	1.991	Fluoride
2	6.520	0.2820	1.816	2.968	Chloride
3	8.610	0.6298	3.190	2.960	Nitrite
4	10.625	0.4133	1.833	9.916	Bromide
5	12.283	0.5789	2.251	2.467	Nitrate
6	14.002	0.4067	1.087	5.110	Phosphate
7	15.660	1.0476	2.898	14.621	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-05-22 12:56:31 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

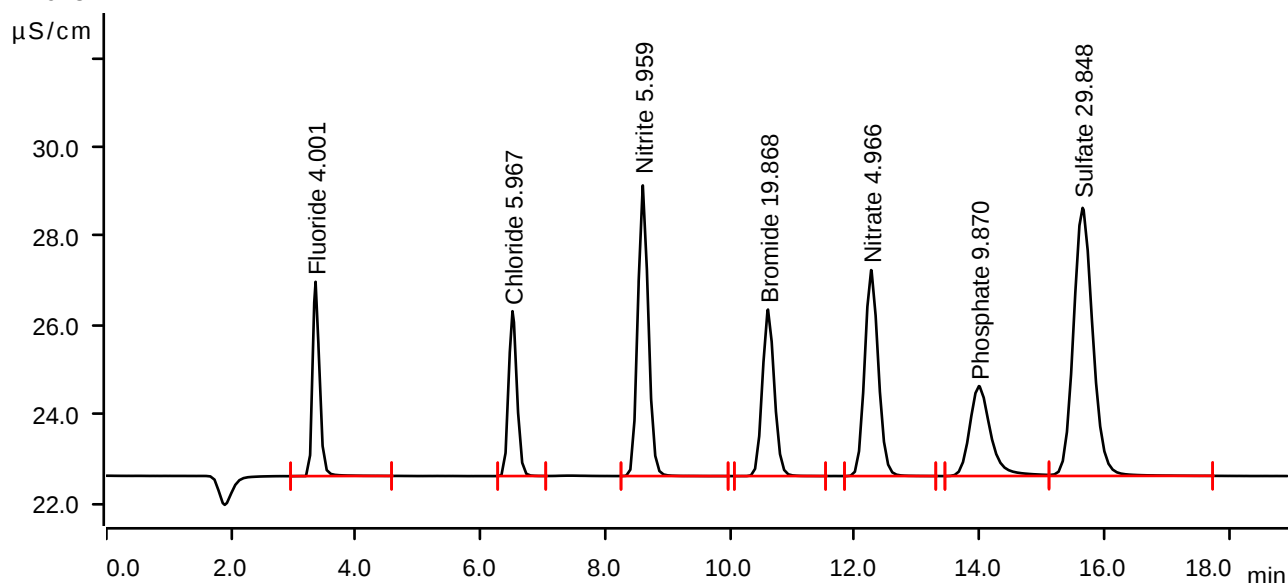

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.5553	4.361	4.001	Fluoride
2	6.512	0.5713	3.701	5.967	Chloride
3	8.602	1.2834	6.525	5.959	Nitrite
4	10.608	0.8345	3.739	19.868	Bromide
5	12.262	1.1762	4.624	4.966	Nitrate
6	13.990	0.7883	2.019	9.870	Phosphate
7	15.652	2.1703	6.019	29.848	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-05-22 13:17:57 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

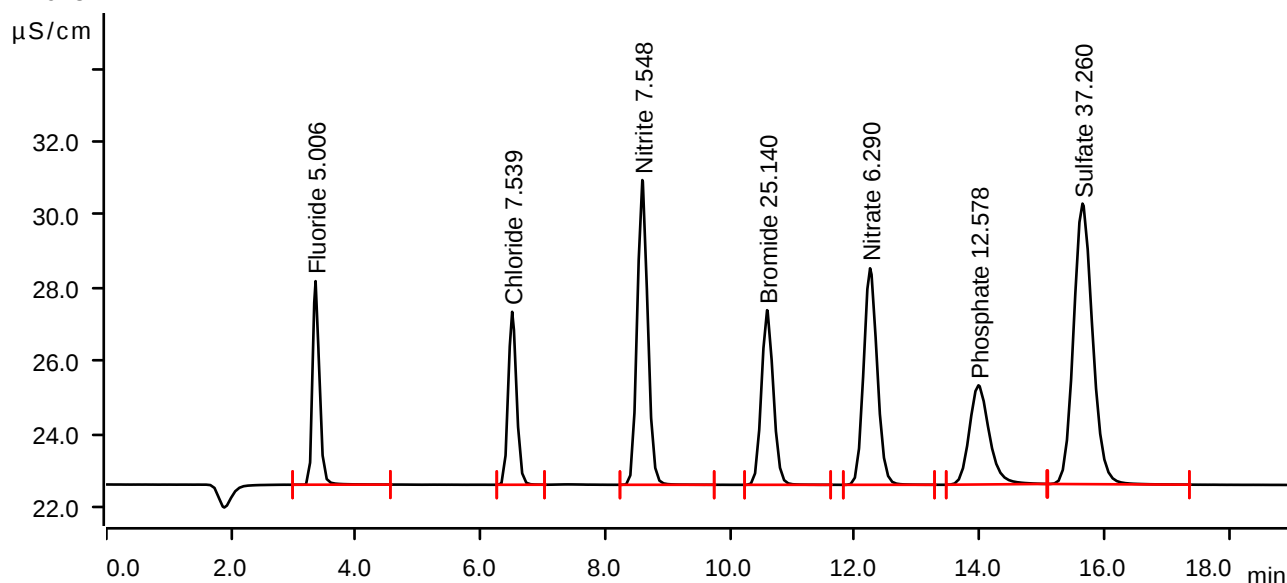

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.6954	5.562	5.006	Fluoride
2	6.507	0.7229	4.726	7.539	Chloride
3	8.593	1.6297	8.328	7.548	Nitrite
4	10.593	1.0576	4.774	25.140	Bromide
5	12.245	1.4927	5.918	6.290	Nitrate
6	13.982	1.0054	2.711	12.578	Phosphate
7	15.650	2.7168	7.668	37.260	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-05-22 13:39:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

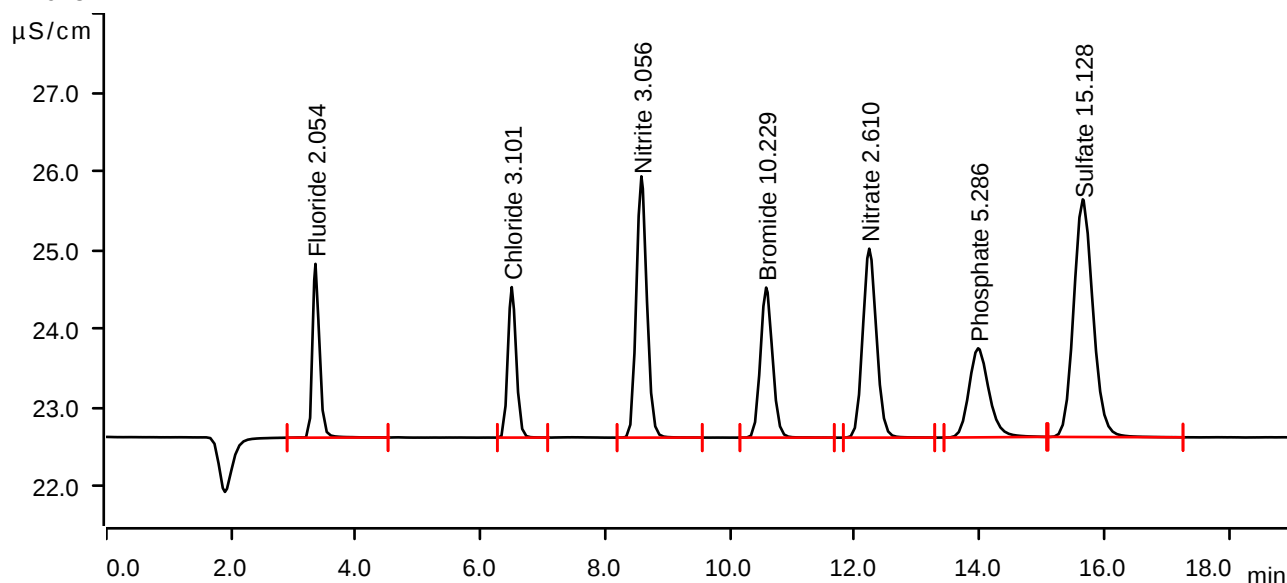


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2837	2.205	2.054	Fluoride
2	6.500	0.2948	1.910	3.101	Chloride
3	8.578	0.6509	3.316	3.056	Nitrite
4	10.578	0.4266	1.904	10.229	Bromide
5	12.232	0.6129	2.398	2.610	Nitrate
6	13.977	0.4208	1.130	5.286	Phosphate
7	15.655	1.0850	3.016	15.128	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-05-22 14:22:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

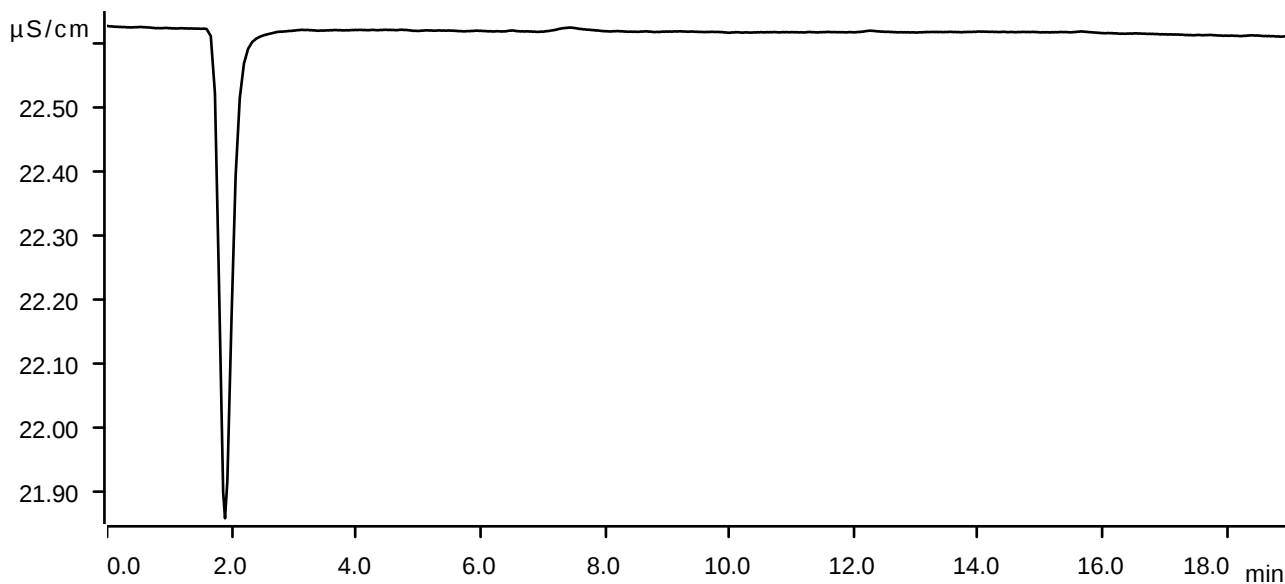Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-09 09:25:13 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

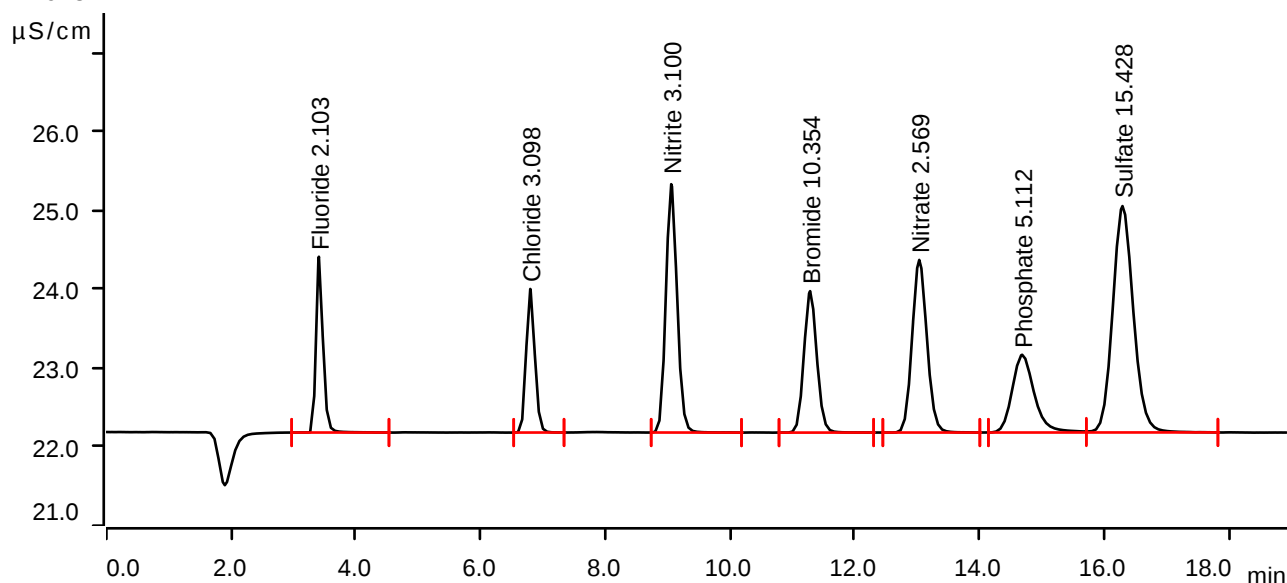

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.408	0.2905	2.230	2.103	Fluoride
2	6.797	0.2945	1.822	3.098	Chloride
3	9.057	0.6605	3.151	3.100	Nitrite
4	11.283	0.4319	1.795	10.354	Bromide
5	13.033	0.6032	2.191	2.569	Nitrate
6	14.683	0.4068	0.987	5.112	Phosphate
7	16.292	1.1071	2.873	15.428	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-09 09:46:43 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

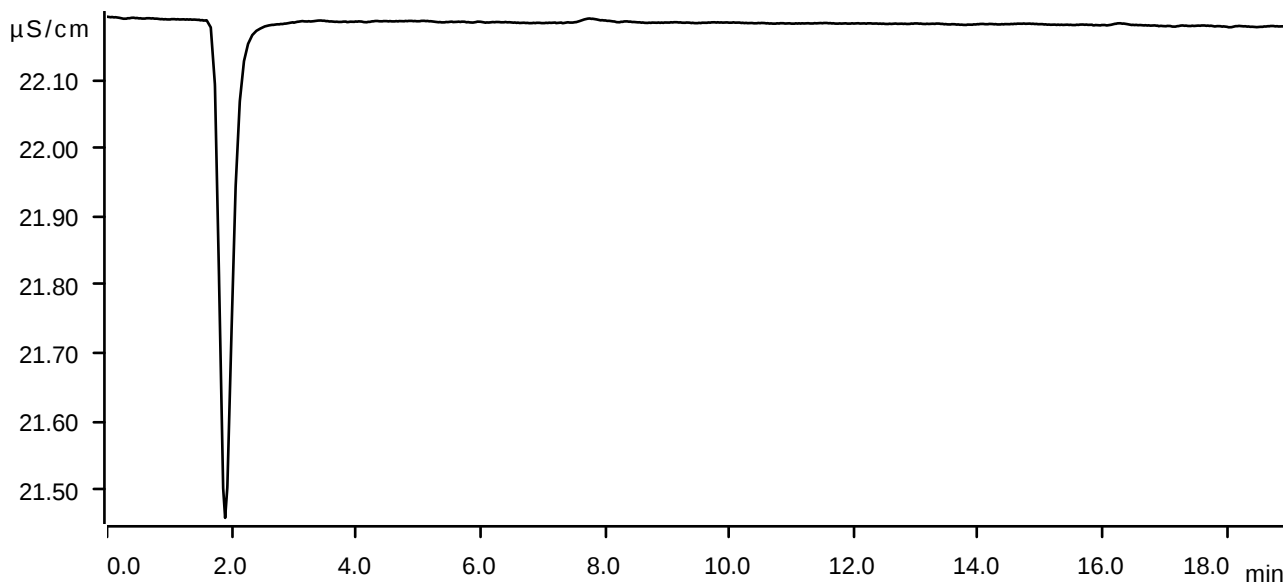


Sample data

Ident LB136070BLW
Sample type Sample
Determination start 2025-06-09 10:08:14 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.95 MPa
Maximum pressure monitored yes
Temperature ---- °C

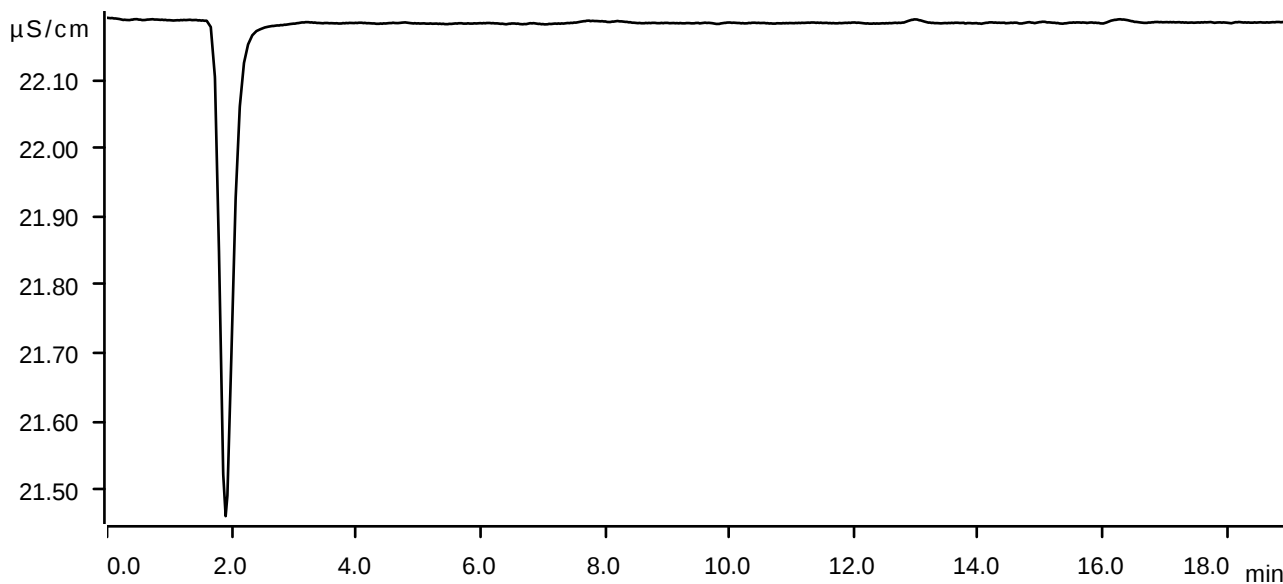Anions


Sample data

Ident LB136070BSW
Sample type Check standard 1
Determination start 2025-06-09 10:29:45 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

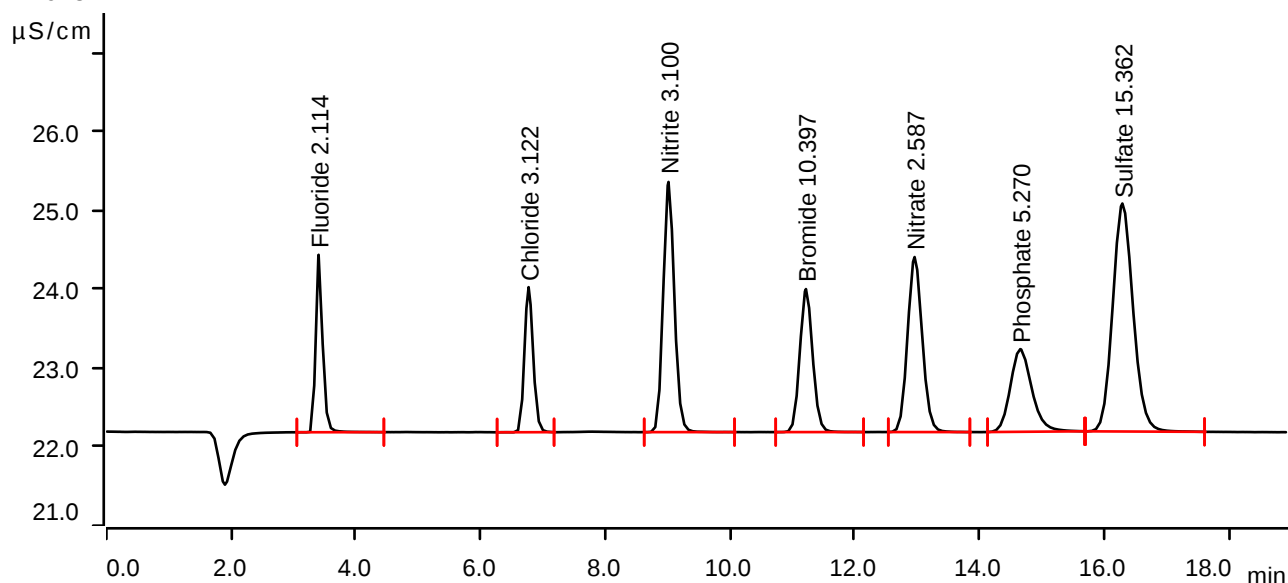

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.403	0.2921	2.251	2.114	Fluoride
2	6.770	0.2968	1.841	3.122	Chloride
3	9.013	0.6604	3.175	3.100	Nitrite
4	11.217	0.4337	1.815	10.397	Bromide
5	12.958	0.6075	2.221	2.587	Nitrate
6	14.653	0.4195	1.049	5.270	Phosphate
7	16.290	1.1023	2.893	15.362	Sulfate


Sample data

Ident Q2268-01
Sample type Sample
Determination start 2025-06-09 10:51:18 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

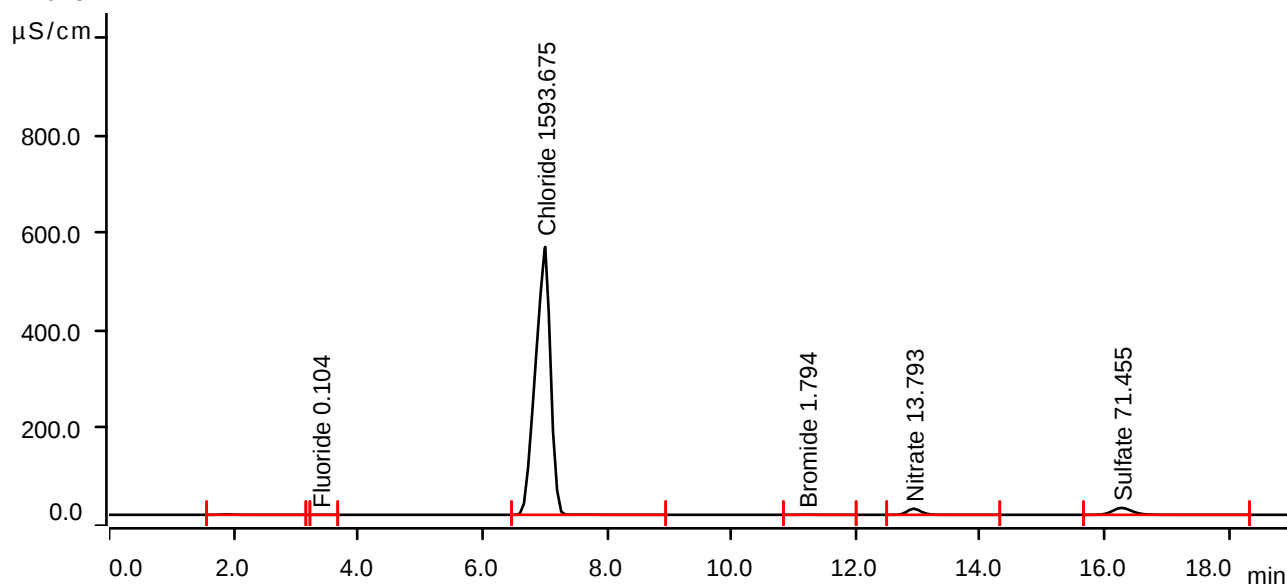

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.858	0.2293	0.837	invalid	
2	3.392	0.0117	0.087	0.104	Fluoride
3	7.010	153.7331	549.083	1593.675	Chloride
4	11.215	0.0696	0.290	1.794	Bromide
5	12.928	3.2863	12.585	13.793	Nitrate
6	16.270	5.2380	14.278	71.455	Sulfate


Sample data

Ident Q2268-02
Sample type Sample
Determination start 2025-06-09 11:12:51 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

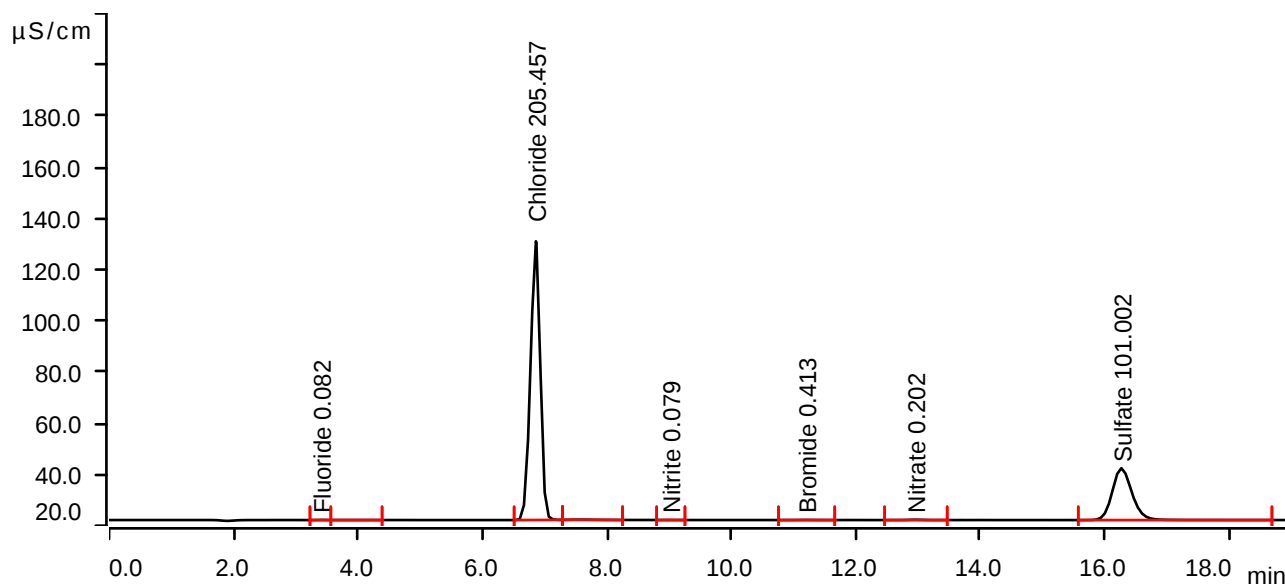

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.402	0.0085	0.062	0.082	Fluoride
2	3.623	0.0030	0.012	invalid	
3	6.860	19.8156	108.820	205.457	Chloride
4	7.560	0.0429	0.097	invalid	
5	9.015	0.0022	0.012	0.079	Nitrite
6	11.203	0.0112	0.046	0.413	Bromide
7	12.953	0.0374	0.137	0.202	Nitrate
8	16.267	7.4165	20.254	101.002	Sulfate


Sample data

Ident Q2268-03
Sample type Sample
Determination start 2025-06-09 11:34:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

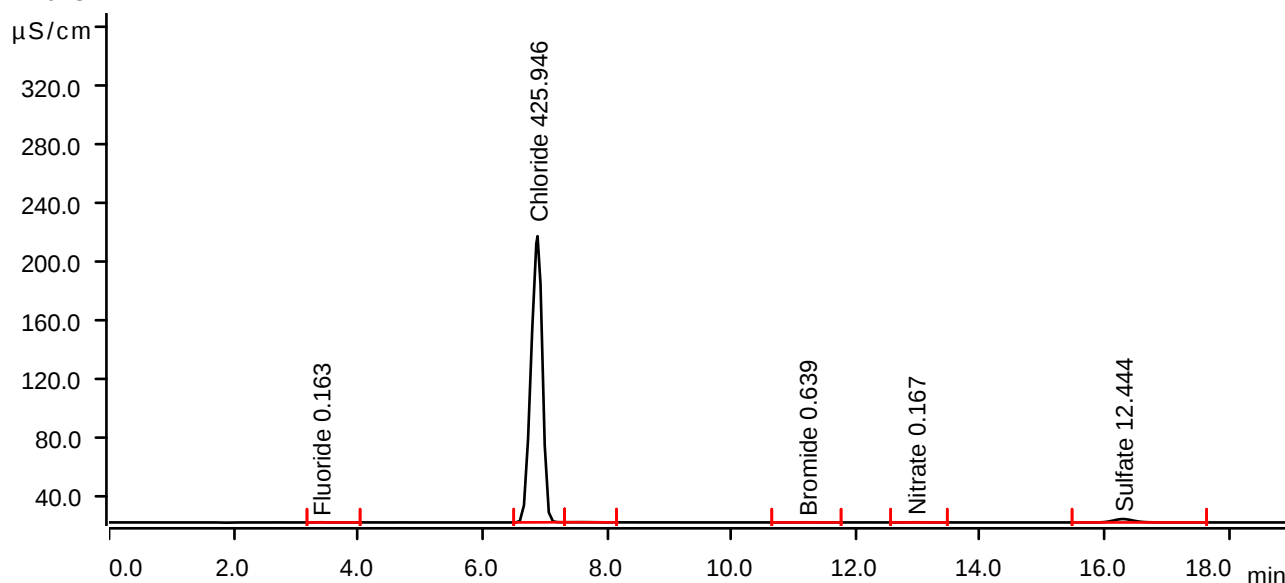

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.0199	0.132	0.163	Fluoride
2	6.887	41.0855	195.556	425.946	Chloride
3	7.535	0.0332	0.082	invalid	
4	11.213	0.0208	0.084	0.639	Bromide
5	12.957	0.0291	0.104	0.167	Nitrate
6	16.292	0.8871	2.327	12.444	Sulfate


Sample data

Ident Q2268-04MS
Sample type Sample
Determination start 2025-06-09 11:56:01 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.95 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

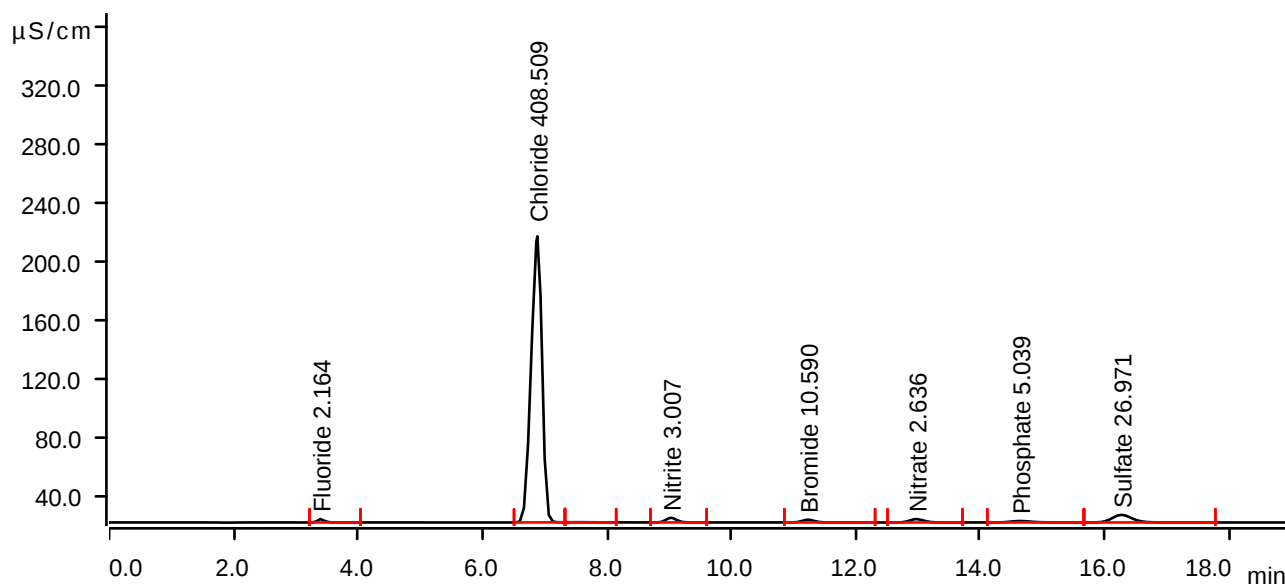

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.2991	2.298	2.164	Fluoride
2	6.883	39.4035	195.464	408.509	Chloride
3	7.558	0.0315	0.079	invalid	
4	9.030	0.6402	3.148	3.007	Nitrite
5	11.232	0.4419	1.866	10.590	Bromide
6	12.973	0.6192	2.280	2.636	Nitrate
7	14.640	0.4010	0.990	5.039	Phosphate
8	16.270	1.9582	5.213	26.971	Sulfate


Sample data

Ident Q2268-05MSD
Sample type Sample
Determination start 2025-06-09 12:17:37 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

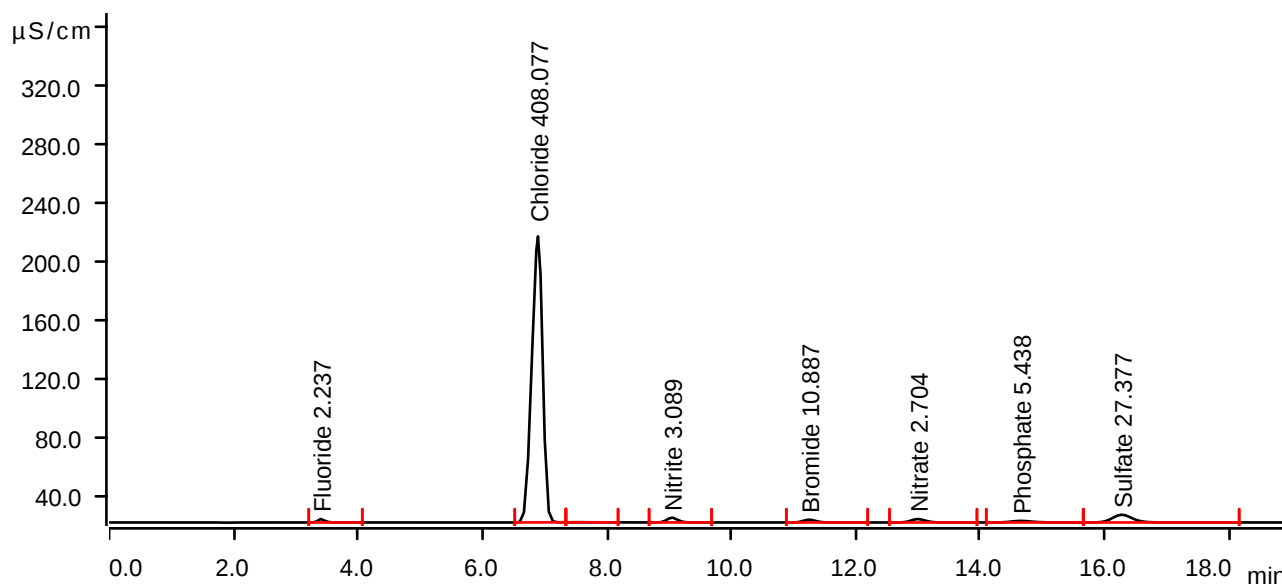

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.403	0.3092	2.348	2.237	Fluoride
2	6.893	39.3617	195.485	408.077	Chloride
3	7.585	0.0319	0.077	invalid	
4	9.047	0.6581	3.222	3.089	Nitrite
5	11.252	0.4544	1.909	10.887	Bromide
6	12.997	0.6355	2.333	2.704	Nitrate
7	14.650	0.4330	1.073	5.438	Phosphate
8	16.273	1.9881	5.278	27.377	Sulfate


Sample data

Ident Q2268-06
Sample type Sample
Determination start 2025-06-09 12:39:12 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.06 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

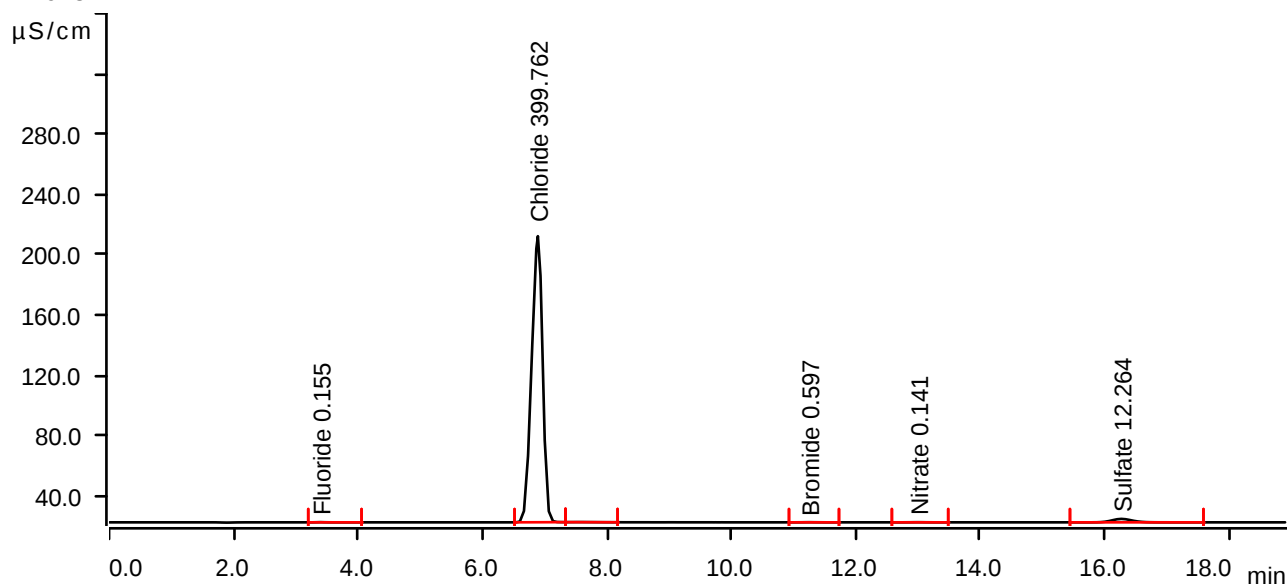

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.397	0.0188	0.126	0.155	Fluoride
2	6.892	38.5596	189.903	399.762	Chloride
3	7.557	0.0320	0.078	invalid	
4	11.248	0.0190	0.079	0.597	Bromide
5	13.000	0.0227	0.083	0.141	Nitrate
6	16.268	0.8738	2.290	12.264	Sulfate


Sample data

Ident Q2268-07
Sample type Sample
Determination start 2025-06-09 13:00:46 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.95 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

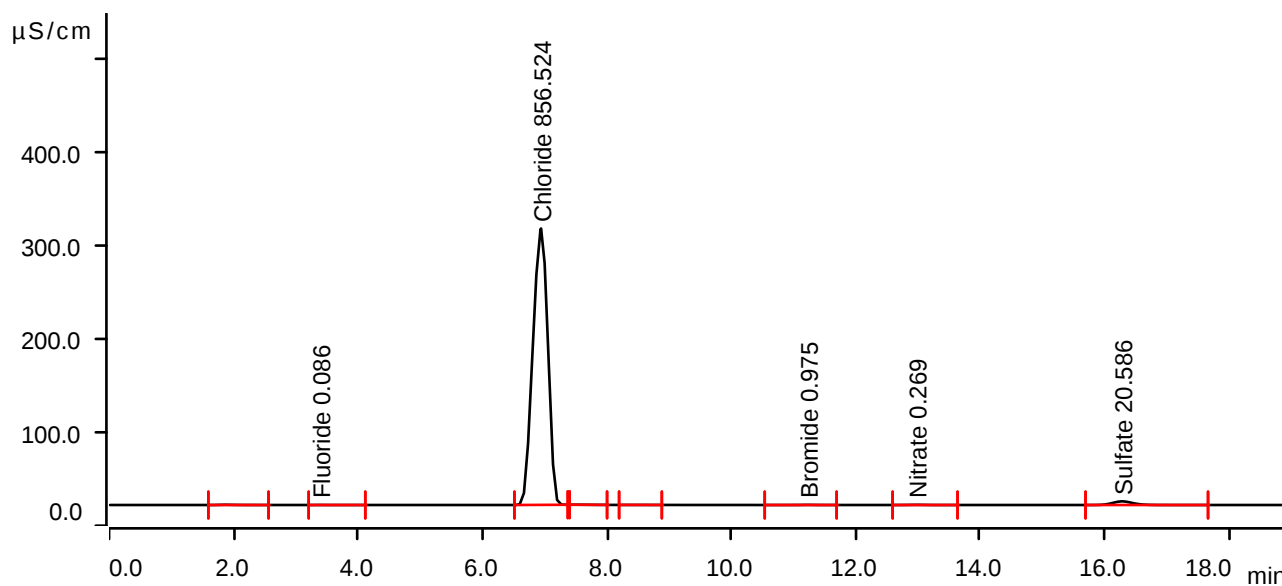

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	1.865	0.0761	0.275	invalid	
2	3.395	0.0092	0.056	0.086	Fluoride
3	6.943	82.6222	296.798	856.524	Chloride
4	7.497	0.0178	0.054	invalid	
5	8.402	0.0067	0.021	invalid	
6	11.232	0.0350	0.144	0.975	Bromide
7	12.973	0.0533	0.195	0.269	Nitrate
8	16.278	1.4875	3.944	20.586	Sulfate


Sample data

Ident Q2268-08
Sample type Sample
Determination start 2025-06-09 13:22:20 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

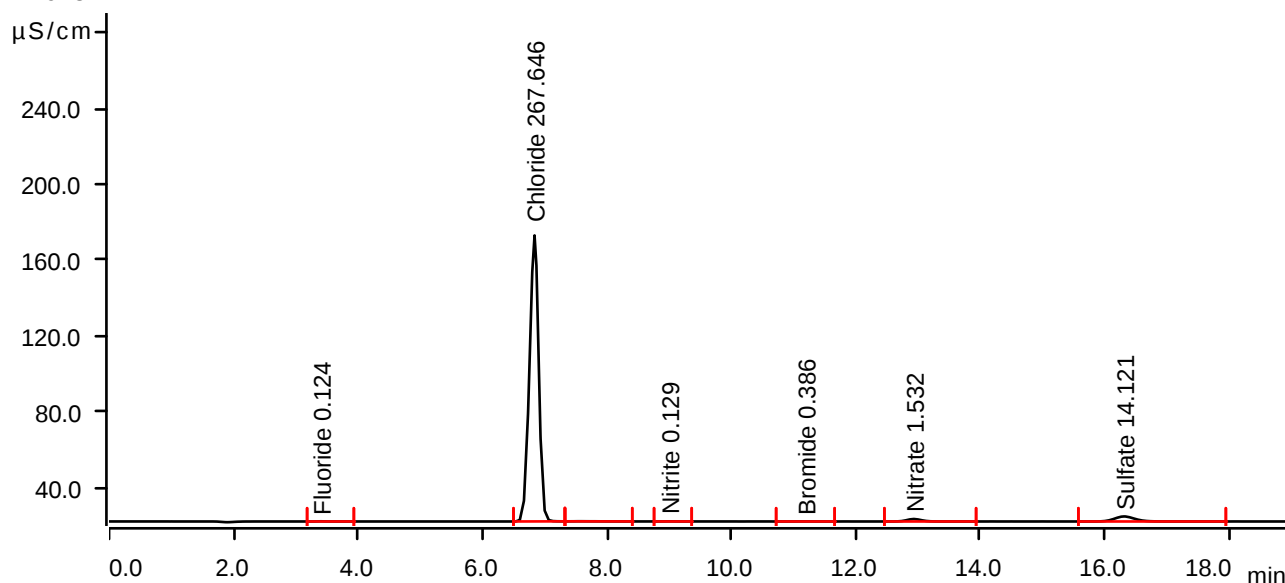

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.405	0.0145	0.102	0.124	Fluoride
2	6.838	25.8147	150.755	267.646	Chloride
3	7.580	0.0270	0.063	invalid	
4	9.002	0.0131	0.064	0.129	Nitrite
5	11.190	0.0101	0.039	0.386	Bromide
6	12.932	0.3553	1.301	1.532	Nitrate
7	16.312	1.0107	2.656	14.121	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-09 13:43:55 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

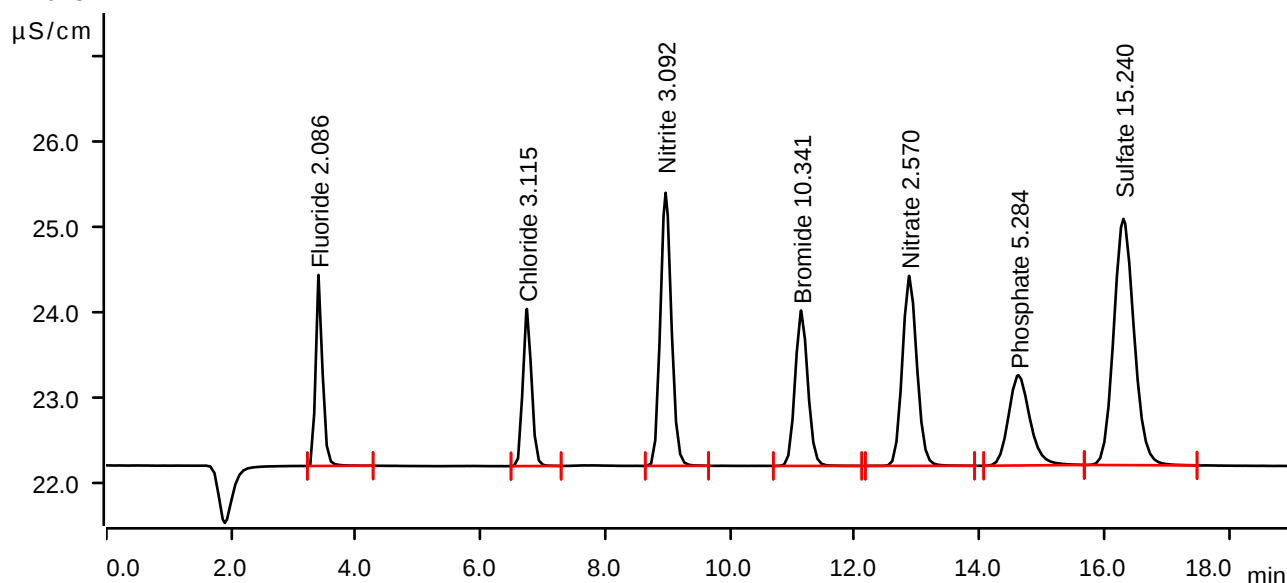

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.402	0.2882	2.237	2.086	Fluoride
2	6.743	0.2961	1.841	3.115	Chloride
3	8.967	0.6588	3.199	3.092	Nitrite
4	11.140	0.4313	1.821	10.341	Bromide
5	12.873	0.6034	2.225	2.570	Nitrate
6	14.622	0.4207	1.058	5.284	Phosphate
7	16.307	1.0933	2.884	15.240	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-09 14:05:22 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

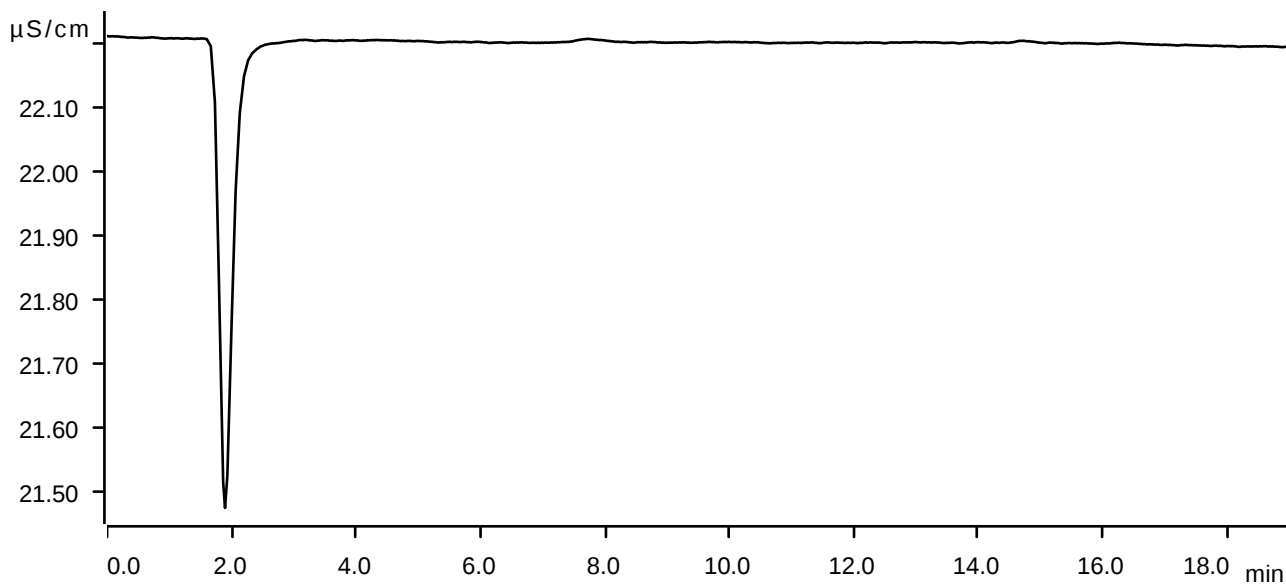


Sample data

Ident Q2268-10
Sample type Sample
Determination start 2025-06-09 14:26:53 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

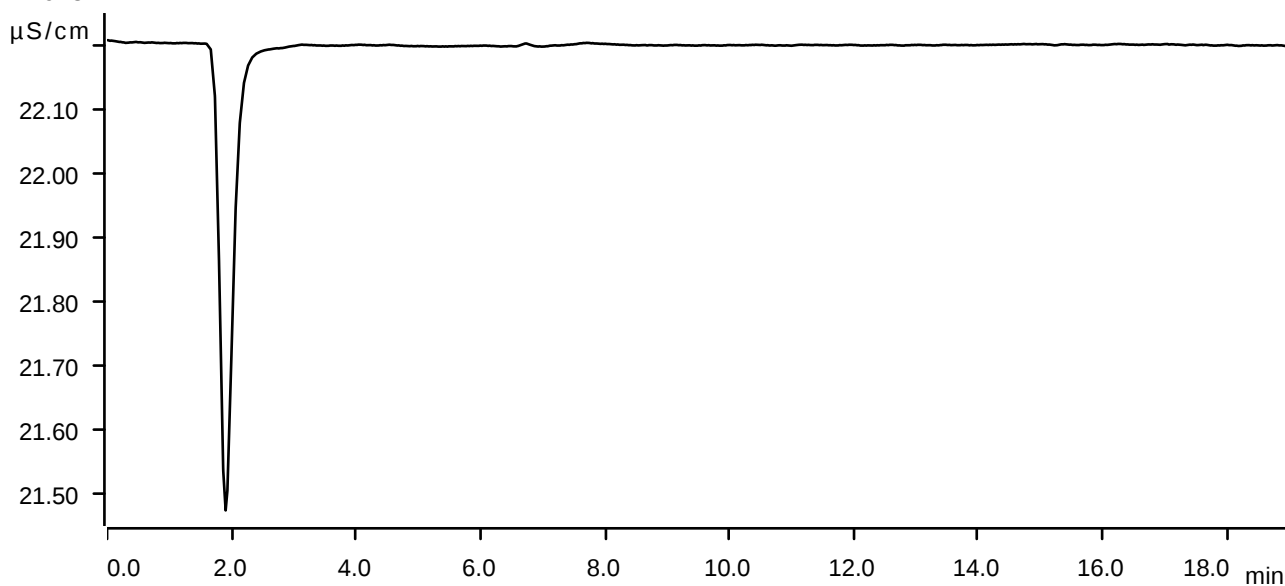


Sample data

Ident Q2268-01DLX5
Sample type Sample
Determination start 2025-06-09 14:48:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

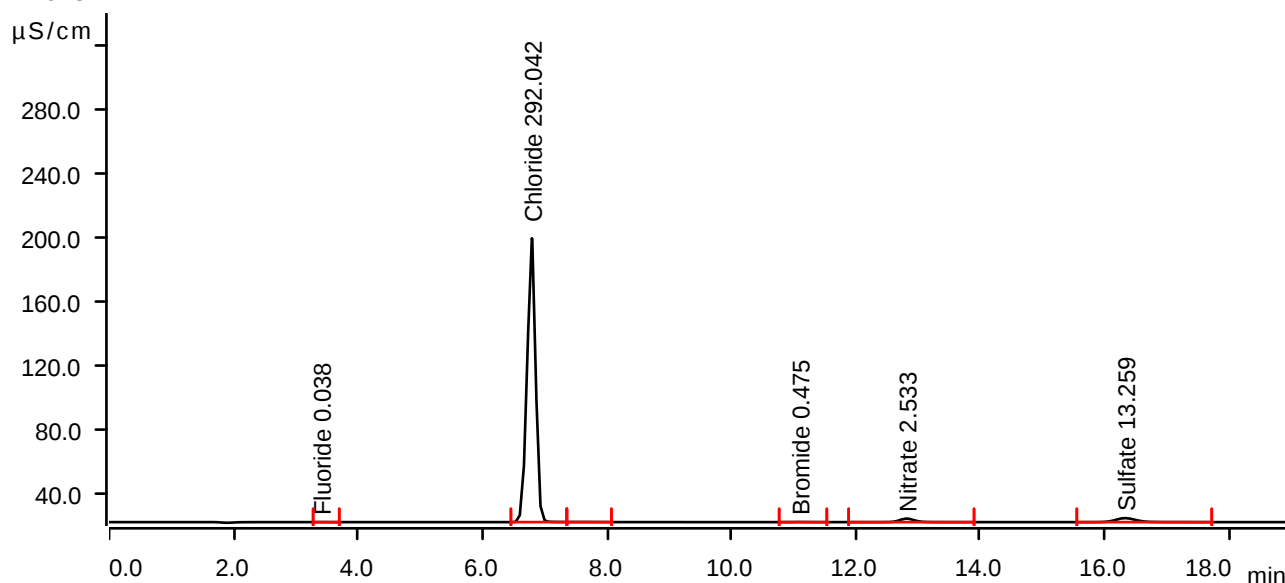

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.403	0.0025	0.018	0.038	Fluoride
2	6.795	28.1682	177.310	292.042	Chloride
3	7.555	0.0091	0.024	invalid	
4	11.095	0.0138	0.057	0.475	Bromide
5	12.817	0.5947	2.211	2.533	Nitrate
6	16.328	0.9472	2.500	13.259	Sulfate


Sample data

Ident Q2268-02DLX10
Sample type Sample
Determination start 2025-06-09 15:09:56 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

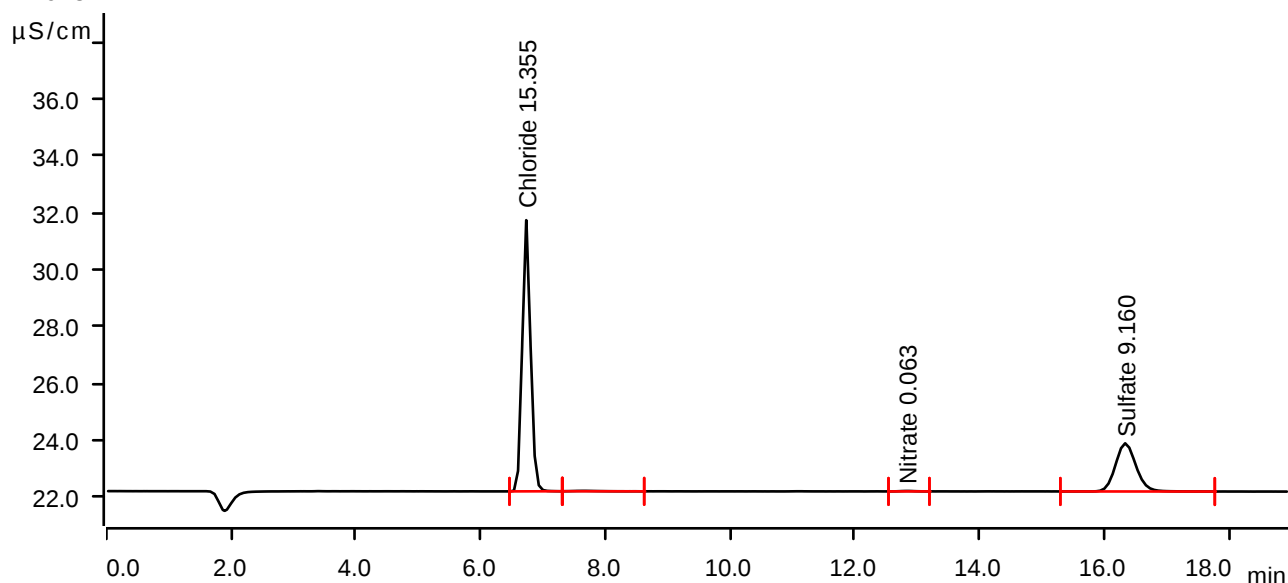

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.732	1.4769	9.529	15.355	Chloride
2	7.640	0.0067	0.014	invalid	
3	12.830	0.0041	0.016	0.063	Nitrate
4	16.335	0.6450	1.692	9.160	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-06-09 15:31:26 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

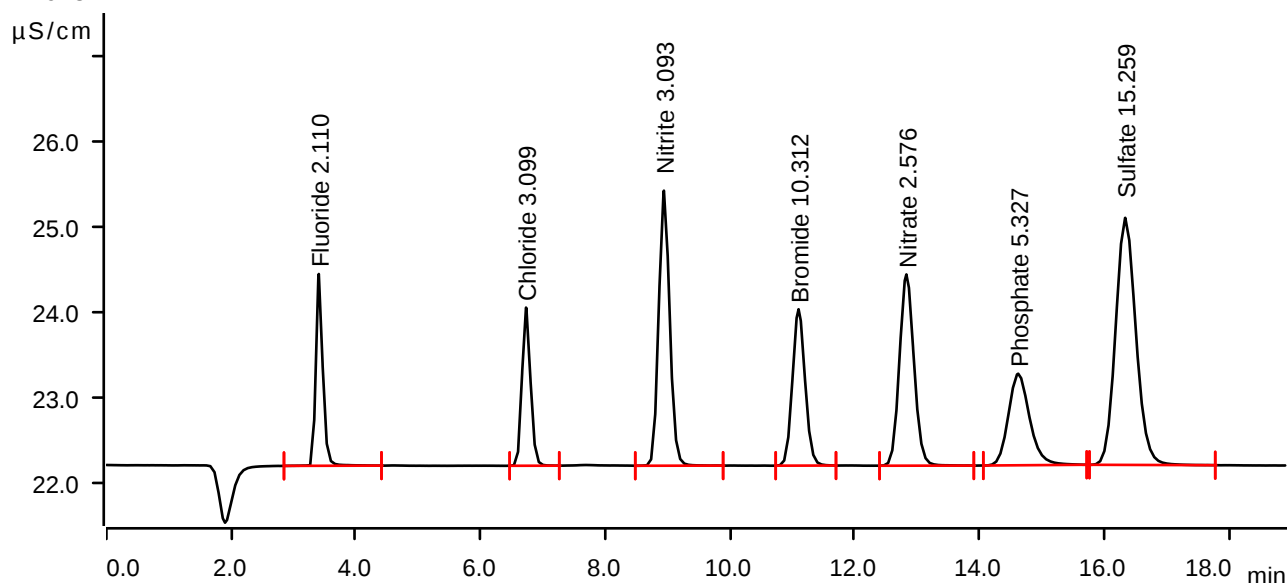

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.407	0.2916	2.246	2.110	Fluoride
2	6.728	0.2946	1.852	3.099	Chloride
3	8.940	0.6590	3.222	3.093	Nitrite
4	11.098	0.4301	1.832	10.312	Bromide
5	12.827	0.6048	2.241	2.576	Nitrate
6	14.620	0.4241	1.073	5.327	Phosphate
7	16.337	1.0947	2.894	15.259	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-09 15:52:56 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

