



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q2275
Client: JACOBS Engineering Group, Inc.

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
Client ID:				0				
Total Voc :								
Total Concentration:								



SAMPLE DATA

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	06/08/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	06/10/25
Client Sample ID:	OW-08B-72.5-060925	SDG No.:	Q2275
Lab Sample ID:	Q2275-01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046665.D	1		06/12/25 15:46	VX061225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	50.4		70 (74) - 130 (125)	101%	SPK: 50
1868-53-7	Dibromofluoromethane	53.9		70 (75) - 130 (124)	108%	SPK: 50
2037-26-5	Toluene-d8	52.1		70 (86) - 130 (113)	104%	SPK: 50
460-00-4	4-Bromofluorobenzene	53.4		70 (77) - 130 (121)	107%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	75900	5.568			
540-36-3	1,4-Difluorobenzene	134000	6.775			
3114-55-4	Chlorobenzene-d5	120000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	61900	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	06/08/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	06/10/25
Client Sample ID:	EB01-060925	SDG No.:	Q2275
Lab Sample ID:	Q2275-03	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046667.D	1		06/12/25 16:32	VX061225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	55.3		70 (74) - 130 (125)	111%	SPK: 50
1868-53-7	Dibromofluoromethane	56.6		70 (75) - 130 (124)	113%	SPK: 50
2037-26-5	Toluene-d8	54.4		70 (86) - 130 (113)	109%	SPK: 50
460-00-4	4-Bromofluorobenzene	55.2		70 (77) - 130 (121)	110%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	68400	5.574			
540-36-3	1,4-Difluorobenzene	128000	6.775			
3114-55-4	Chlorobenzene-d5	115000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	59200	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	06/08/25
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	06/10/25
Client Sample ID:	TB01-060925	SDG No.:	Q2275
Lab Sample ID:	Q2275-05	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046668.D	1		06/12/25 16:55	VX061225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	41.9		70 (74) - 130 (125)	84%	SPK: 50
1868-53-7	Dibromofluoromethane	47.6		70 (75) - 130 (124)	95%	SPK: 50
2037-26-5	Toluene-d8	46.0		70 (86) - 130 (113)	92%	SPK: 50
460-00-4	4-Bromofluorobenzene	46.1		70 (77) - 130 (121)	92%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	87100	5.574			
540-36-3	1,4-Difluorobenzene	148000	6.775			
3114-55-4	Chlorobenzene-d5	136000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	70800	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products



QC SUMMARY

Surrogate Summary

SDG No.: Q2275

Client: JACOBS Engineering Group, Inc.

Analytical Method: SW8260-Low

Lab Sample ID	Client ID	Parameter	Spike	Result	RecoveryQual	Limits	
						Low	High
Q2275-01	OW-08B-72.5-060925	1,2-Dichloroethane-d4	50	50.4	101	70 (74)	130 (125)
		Dibromofluoromethane	50	53.9	108	70 (75)	130 (124)
		Toluene-d8	50	52.1	104	70 (86)	130 (113)
		4-Bromofluorobenzene	50	53.4	107	70 (77)	130 (121)
Q2275-03	EB01-060925	1,2-Dichloroethane-d4	50	55.3	111	70 (74)	130 (125)
		Dibromofluoromethane	50	56.6	113	70 (75)	130 (124)
		Toluene-d8	50	54.4	109	70 (86)	130 (113)
		4-Bromofluorobenzene	50	55.2	110	70 (77)	130 (121)
Q2275-05	TB01-060925	1,2-Dichloroethane-d4	50	41.9	84	70 (74)	130 (125)
		Dibromofluoromethane	50	47.6	95	70 (75)	130 (124)
		Toluene-d8	50	46.0	92	70 (86)	130 (113)
		4-Bromofluorobenzene	50	46.1	92	70 (77)	130 (121)
VX0612WBL01	VX0612WBL01	1,2-Dichloroethane-d4	50	46.2	92	70 (74)	130 (125)
		Dibromofluoromethane	50	48.5	97	70 (75)	130 (124)
		Toluene-d8	50	52.4	105	70 (86)	130 (113)
		4-Bromofluorobenzene	50	54.6	109	70 (77)	130 (121)
VX0612WBS01	VX0612WBS01	1,2-Dichloroethane-d4	50	41.5	83	70 (74)	130 (125)
		Dibromofluoromethane	50	48.0	96	70 (75)	130 (124)
		Toluene-d8	50	47.8	96	70 (86)	130 (113)
		4-Bromofluorobenzene	50	48.1	96	70 (77)	130 (121)
VX0612WBSD01	VX0612WBSD01	1,2-Dichloroethane-d4	50	44.8	90	70 (74)	130 (125)
		Dibromofluoromethane	50	49.7	99	70 (75)	130 (124)
		Toluene-d8	50	48.3	97	70 (86)	130 (113)
		4-Bromofluorobenzene	50	50.5	101	70 (77)	130 (121)

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2275

Client: JACOBS Engineering Group, Inc.

Analytical Method: SW8260-Low

Datafile : VX046660.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VX0612WBS01	Vinyl chloride	20	15.1	ug/L	76			70 (65)	130 (117)	
	1,1-Dichloroethene	20	17.3	ug/L	86			70 (74)	130 (110)	
	1,1-Dichloroethane	20	17.8	ug/L	89			70 (78)	130 (112)	
	cis-1,2-Dichloroethene	20	18.1	ug/L	91			70 (77)	130 (110)	
	1,1,1-Trichloroethane	20	17.8	ug/L	89			70 (80)	130 (108)	
	Benzene	20	18.7	ug/L	94			70 (82)	130 (109)	
	1,2-Dichloroethane	20	17.6	ug/L	88			70 (80)	130 (115)	
	Trichloroethene	20	18.5	ug/L	93			70 (77)	130 (113)	
	1,1,2-Trichloroethane	20	20.6	ug/L	103			70 (83)	130 (112)	
	Tetrachloroethene	20	18.9	ug/L	95			70 (67)	130 (123)	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2275

Client: JACOBS Engineering Group, Inc.

Analytical Method: SW8260-Low

Datafile : VX046662.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Low	Limits High	RPD
VX0612WBSD01	Vinyl chloride	20	15.3	ug/L	77	1		70 (65)	130 (117)	20 (19)
	1,1-Dichloroethene	20	17.2	ug/L	86	0		70 (74)	130 (110)	20 (20)
	1,1-Dichloroethane	20	18.4	ug/L	92	3		70 (78)	130 (112)	20 (20)
	cis-1,2-Dichloroethene	20	19.0	ug/L	95	4		70 (77)	130 (110)	20 (20)
	1,1,1-Trichloroethane	20	18.4	ug/L	92	3		70 (80)	130 (108)	20 (20)
	Benzene	20	19.0	ug/L	95	1		70 (82)	130 (109)	20 (15)
	1,2-Dichloroethane	20	19.1	ug/L	96	9		70 (80)	130 (115)	20 (20)
	Trichloroethene	20	18.9	ug/L	95	2		70 (77)	130 (113)	20 (15)
	1,1,2-Trichloroethane	20	22.1	ug/L	111	7		70 (83)	130 (112)	20 (20)
	Tetrachloroethene	20	18.5	ug/L	93	2		70 (67)	130 (123)	20 (15)

VOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

VX0612WBL01

Lab Name: CHEMTECH

Contract: JAC005

Lab Code: CHEM Case No.: Q2275

SAS No.: Q2275 SDG NO.: Q2275

Lab File ID: VX046659.D

Lab Sample ID: VX0612WBL01

Date Analyzed: 06/12/2025

Time Analyzed: 13:10

GC Column: DB-624UI ID: 0.18 (mm)

Heated Purge: (Y/N) N

Instrument ID: MSVOA_X

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
VX0612WBS01	VX0612WBS01	VX046660.D	06/12/2025
VX0612WBSD01	VX0612WBSD01	VX046662.D	06/12/2025
OW-08B-72.5-060925	Q2275-01	VX046665.D	06/12/2025
EB01-060925	Q2275-03	VX046667.D	06/12/2025
TB01-060925	Q2275-05	VX046668.D	06/12/2025

COMMENTS: _____

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: CHEMTECH Contract: JACO05
Lab Code: CHEM Case No.: Q2275 SAS No.: Q2275 SDG NO.: Q2275
Lab File ID: VX046516.D BFB Injection Date: 06/06/2025
Instrument ID: MSVOA_X BFB Injection Time: 08:47
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	21
75	30.0 - 60.0% of mass 95	56.5
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.5
173	Less than 2.0% of mass 174	0.6 (1) 1
174	50.0 - 100.0% of mass 95	65.2
175	5.0 - 9.0% of mass 174	5 (7.7) 1
176	95.0 - 101.0% of mass 174	62.7 (96.1) 1
177	5.0 - 9.0% of mass 176	4.2 (6.6) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDIC005	VSTDIC005	VX046518.D	06/06/2025	09:42
VSTDIC020	VSTDIC020	VX046519.D	06/06/2025	10:18
VSTDIC050	VSTDIC050	VX046520.D	06/06/2025	10:40
VSTDIC100	VSTDIC100	VX046521.D	06/06/2025	11:02
VSTDIC150	VSTDIC150	VX046522.D	06/06/2025	11:25
VSTDIC001	VSTDIC001	VX046524.D	06/06/2025	12:57

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: CHEMTECH Contract: JACO05
Lab Code: CHEM Case No.: Q2275 SAS No.: Q2275 SDG NO.: Q2275
Lab File ID: VX046656.D BFB Injection Date: 06/12/2025
Instrument ID: MSVOA_X BFB Injection Time: 09:44
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	19.2
75	30.0 - 60.0% of mass 95	51
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.6
173	Less than 2.0% of mass 174	0.6 (0.8) 1
174	50.0 - 100.0% of mass 95	73.3
175	5.0 - 9.0% of mass 174	5.9 (8.1) 1
176	95.0 - 101.0% of mass 174	72.3 (98.6) 1
177	5.0 - 9.0% of mass 176	4.6 (6.3) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VX046657.D	06/12/2025	10:11
VX0612WBL01	VX0612WBL01	VX046659.D	06/12/2025	13:10
VX0612WBS01	VX0612WBS01	VX046660.D	06/12/2025	13:38
VX0612WBSD01	VX0612WBSD01	VX046662.D	06/12/2025	14:26
OW-08B-72.5-060925	Q2275-01	VX046665.D	06/12/2025	15:46
EB01-060925	Q2275-03	VX046667.D	06/12/2025	16:32
TB01-060925	Q2275-05	VX046668.D	06/12/2025	16:55

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: JACO05
Lab Code: CHEM Case No.: Q2275 SAS No.: Q2275 SDG NO.: Q2275
Lab File ID: VX046657.D Date Analyzed: 06/12/2025
Instrument ID: MSVOA_X Time Analyzed: 10:11
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	82603	5.56	125406	6.77	118101	10.06
UPPER LIMIT	165206	6.056	250812	7.269	236202	10.555
LOWER LIMIT	41301.5	5.056	62703	6.269	59050.5	9.555
EPA SAMPLE NO.						
OW-08B-72.5-060925	75942	5.57	133627	6.78	120396	10.06
EB01-060925	68445	5.57	127742	6.78	114769	10.06
TB01-060925	87075	5.57	148474	6.78	135692	10.06
VX0612WBL01	92224	5.57	180952	6.78	188641	10.06
VX0612WBS01	85578	5.56	144622	6.77	130715	10.06
VX0612WBSD01	77335	5.57	133427	6.78	124864	10.06

IS1 = Pentafluorobenzene
IS2 = 1,4-Difluorobenzene
IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area
AREA LOWER LIMIT = -50% of internal standard area
RT UPPER LIMIT = +0.50 minutes of internal standard RT
RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
* Values outside of QC limits.

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: JACO05
 Lab Code: CHEM Case No.: Q2275 SAS No.: Q2275 SDG NO.: Q2275
 Lab File ID: VX046657.D Date Analyzed: 06/12/2025
 Instrument ID: MSVOA_X Time Analyzed: 10:11
 GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS4 AREA #	RT #				
12 HOUR STD	60636	12.018				
UPPER LIMIT	121272	12.518				
LOWER LIMIT	30318	11.518				
EPA SAMPLE NO.						
OW-08B-72.5-060925	61889	12.02				
EB01-060925	59204	12.02				
TB01-060925	70754	12.02				
VX0612WBL01	95358	12.02				
VX0612WBS01	69016	12.02				
VX0612WBSD01	65393	12.02				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



QC SAMPLE DATA

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	VX0612WBL01	SDG No.:	Q2275
Lab Sample ID:	VX0612WBL01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046659.D	1		06/12/25 13:10	VX061225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	0.26	U	0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.23	U	0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.19	U	0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.20	U	0.20	1.00	ug/L
71-43-2	Benzene	0.15	U	0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.22	U	0.22	1.00	ug/L
79-01-6	Trichloroethene	0.090	U	0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
127-18-4	Tetrachloroethene	0.23	U	0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	46.2		70 (74) - 130 (125)	92%	SPK: 50
1868-53-7	Dibromofluoromethane	48.5		70 (75) - 130 (124)	97%	SPK: 50
2037-26-5	Toluene-d8	52.4		70 (86) - 130 (113)	105%	SPK: 50
460-00-4	4-Bromofluorobenzene	54.6		70 (77) - 130 (121)	109%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	92200	5.568			
540-36-3	1,4-Difluorobenzene	181000	6.775			
3114-55-4	Chlorobenzene-d5	189000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	95400	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	VX0612WBS01	SDG No.:	Q2275
Lab Sample ID:	VX0612WBS01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046660.D	1		06/12/25 13:38	VX061225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	15.1		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	17.3		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	17.8		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	18.1		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	17.8		0.20	1.00	ug/L
71-43-2	Benzene	18.7		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	17.6		0.22	1.00	ug/L
79-01-6	Trichloroethene	18.5		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	20.6		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	18.9		0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	41.5		70 (74) - 130 (125)	83%	SPK: 50
1868-53-7	Dibromofluoromethane	48.0		70 (75) - 130 (124)	96%	SPK: 50
2037-26-5	Toluene-d8	47.8		70 (86) - 130 (113)	96%	SPK: 50
460-00-4	4-Bromofluorobenzene	48.1		70 (77) - 130 (121)	96%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	85600	5.556			
540-36-3	1,4-Difluorobenzene	145000	6.769			
3114-55-4	Chlorobenzene-d5	131000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	69000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Report of Analysis

Client:	JACOBS Engineering Group, Inc.	Date Collected:	
Project:	Former Schlumberger STC PTC Site D3868221	Date Received:	
Client Sample ID:	VX0612WBSD01	SDG No.:	Q2275
Lab Sample ID:	VX0612WBSD01	Matrix:	Water
Analytical Method:	8260D	% Solid:	0
Sample Wt/Vol:	5 Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:	uL	Test:	VOCMS Group3
GC Column:	DB-624UI ID : 0.18	Level :	LOW
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX046662.D	1		06/12/25 14:26	VX061225

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-01-4	Vinyl Chloride	15.3		0.26	1.00	ug/L
75-35-4	1,1-Dichloroethene	17.2		0.23	1.00	ug/L
75-34-3	1,1-Dichloroethane	18.4		0.23	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	19.0		0.19	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	18.4		0.20	1.00	ug/L
71-43-2	Benzene	19.0		0.15	1.00	ug/L
107-06-2	1,2-Dichloroethane	19.1		0.22	1.00	ug/L
79-01-6	Trichloroethene	18.9		0.090	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	22.1		0.21	1.00	ug/L
127-18-4	Tetrachloroethene	18.5		0.23	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	44.8		70 (74) - 130 (125)	90%	SPK: 50
1868-53-7	Dibromofluoromethane	49.7		70 (75) - 130 (124)	99%	SPK: 50
2037-26-5	Toluene-d8	48.3		70 (86) - 130 (113)	97%	SPK: 50
460-00-4	4-Bromofluorobenzene	50.5		70 (77) - 130 (121)	101%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	77300	5.568			
540-36-3	1,4-Difluorobenzene	133000	6.775			
3114-55-4	Chlorobenzene-d5	125000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	65400	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products



CALIBRATION SUMMARY

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name: CHEMTECH Contract: JAC005
 Lab Code: CHEM Case No.: Q2275 SAS No.: Q2275 SDG No.: Q2275
 Instrument ID: MSVOA_X Calibration Date(s): 06/06/2025 06/06/2025
 Heated Purge: (Y/N) N Calibration Time(s): 09:42 12:57
 GC Column: DB-624UI ID: 0.18 (mm)

LAB FILE ID:		RRF005 = VX046518.D		RRF020 = VX046519.D		RRF050 = VX046520.D			
		RRF100 = VX046521.D		RRF150 = VX046522.D		RRF001 = VX046524.D			
COMPOUND	RRF005	RRF020	RRF050	RRF100	RRF150	RRF001	RRF	% RSD	
Vinyl Chloride	0.697	0.593	0.596	0.591	0.622	0.679	0.630	7.5	
1,1-Dichloroethene	0.663	0.550	0.567	0.561	0.585	0.635	0.594	7.6	
1,1-Dichloroethane	1.349	1.266	1.259	1.234	1.297	1.281	1.281	3.1	
cis-1,2-Dichloroethene	0.786	0.752	0.741	0.728	0.767	0.866	0.773	6.4	
1,1,1-Trichloroethane	1.170	1.131	1.141	1.128	1.188	1.131	1.148	2.2	
Benzene	1.597	1.503	1.427	1.380	1.442	1.522	1.479	5.3	
1,2-Dichloroethane	0.646	0.641	0.610	0.586	0.602	0.606	0.615	3.8	
Trichloroethene	0.385	0.356	0.351	0.332	0.354	0.476	0.376	13.8	
1,1,2-Trichloroethane	0.375	0.389	0.366	0.356	0.372	0.331	0.365	5.4	
Tetrachloroethene	0.347	0.324	0.310	0.301	0.314	0.410	0.334	12.1	
1,2-Dichloroethane-d4	0.997	0.848	0.873	0.828	0.900		0.890	7.4	
Dibromofluoromethane	0.392	0.353	0.368	0.347	0.379		0.368	5	
Toluene-d8	1.362	1.159	1.188	1.132	1.220		1.212	7.4	
4-Bromofluorobenzene	0.564	0.482	0.493	0.468	0.501		0.502	7.4	

* Compounds with required minimum RRF and maximum %RSD values.
 All other compounds must meet a minimum RRF of 0.010.
 RRF of 1,4-Dioxane = Value should be divide by 1000.

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name: CHEMTECH Contract: JAC005

Lab Code: CHEM Case No.: Q2275 SAS No.: Q2275 SDG No.: Q2275

Instrument ID: MSVOA_X Calibration Date/Time: 06/12/2025 10:11

Lab File ID: VX046657.D Init. Calib. Date(s): 06/06/2025 06/06/2025

Heated Purge: (Y/N) N Init. Calib. Time(s): 09:42 12:57

GC Column: DB-624UI ID: 0.18 (mm)

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Vinyl Chloride	0.630	0.498		-20.95	20
1,1-Dichloroethene	0.594	0.579		-2.53	20
1,1-Dichloroethane	1.281	1.183	0.1	-7.65	20
cis-1,2-Dichloroethene	0.773	0.764		-1.16	20
1,1,1-Trichloroethane	1.148	1.075		-6.36	20
Benzene	1.479	1.498		1.28	20
1,2-Dichloroethane	0.615	0.566		-7.97	20
Trichloroethene	0.376	0.394		4.79	20
1,1,2-Trichloroethane	0.365	0.423		15.89	20
Tetrachloroethene	0.334	0.342		2.39	20
1,2-Dichloroethane-d4	0.890	0.711		-20.11	20
Dibromofluoromethane	0.368	0.434		17.93	20
Toluene-d8	1.212	1.368		12.87	20
4-Bromofluorobenzene	0.502	0.561		11.75	20

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.



SAMPLE RAW DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046665.D
 Acq On : 12 Jun 2025 15:46
 Operator : JC/MD
 Sample : Q2275-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OW-08B-72.5-060925

Quant Time: Jun 13 01:45:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.568	168	75942	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	133627	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	120396	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	61889	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	68098	50.402	ug/l	0.00
Spiked Amount	50.000	Range 74 - 125	Recovery	= 100.800%		
35) Dibromofluoromethane	5.403	113	52947	53.880	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 107.760%		
50) Toluene-d8	8.653	98	168786	52.098	ug/l	0.00
Spiked Amount	50.000	Range 86 - 113	Recovery	= 104.200%		
62) 4-Bromofluorobenzene	11.079	95	71637	53.442	ug/l	0.00
Spiked Amount	50.000	Range 77 - 121	Recovery	= 106.880%		
Target Compounds						
16) Acetone	2.398	43	1798	7.921	ug/l	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
Data File : VX046665.D
Acq On : 12 Jun 2025 15:46
Operator : JC/MD
Sample : Q2275-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OW-08B-72.5-060925

Quant Time: Jun 13 01:45:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

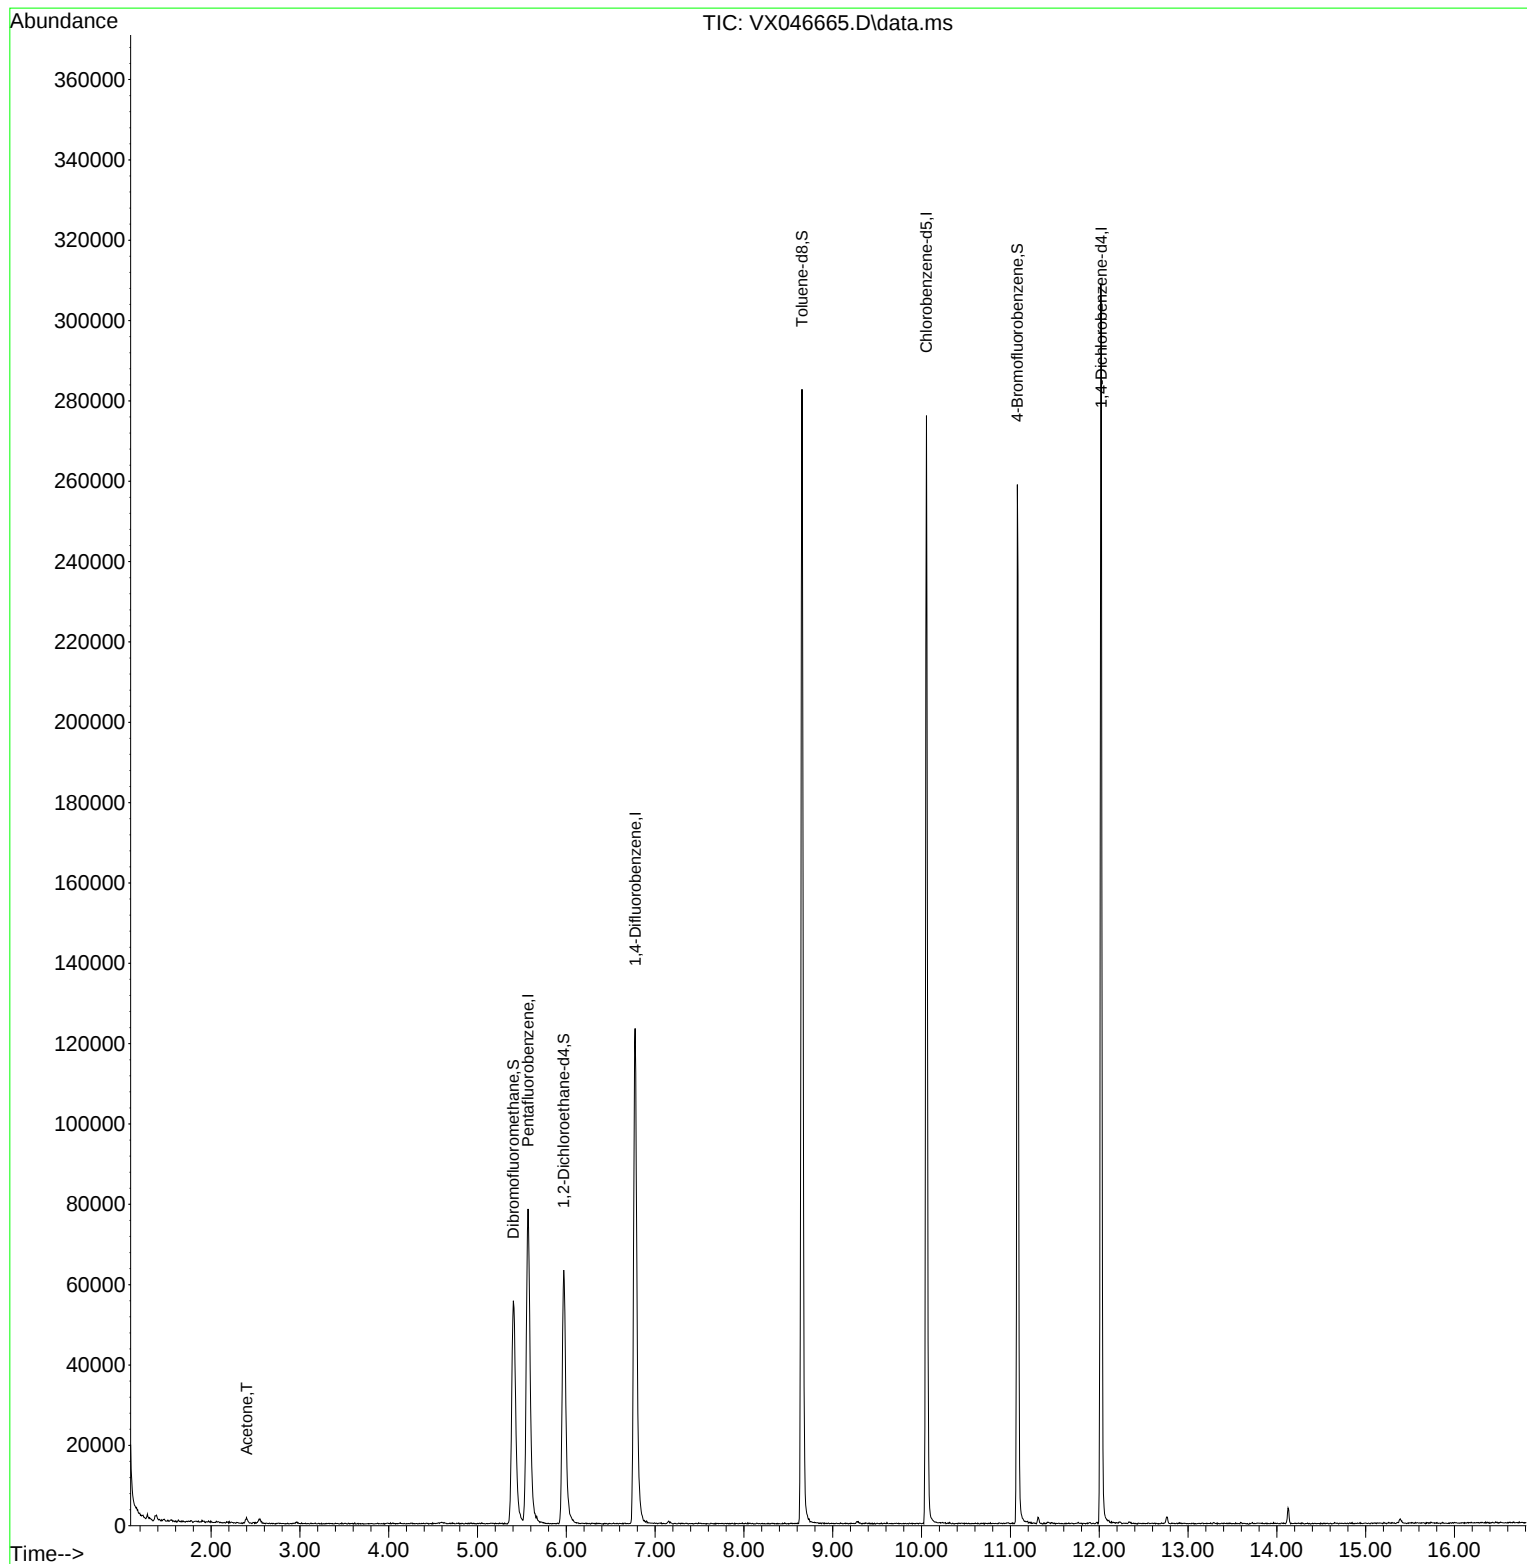

#1
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.568 min Scan# 71

Delta R.T. 0.000 min

Lab File: VX046665.D

Acq: 12 Jun 2025 15:46

Instrument :

MSVOA_X

ClientSampleId :





OW-08B-72.5-060925

Tgt Ion:168 Resp: 75942

Ion Ratio Lower Upper

168 100

99 63.3 54.9 82.3

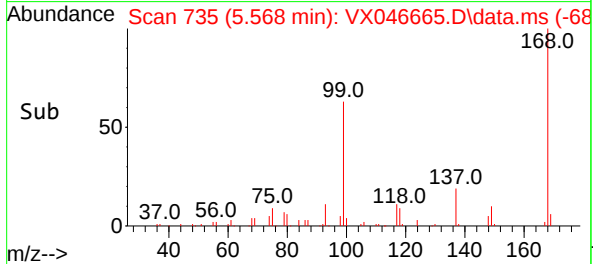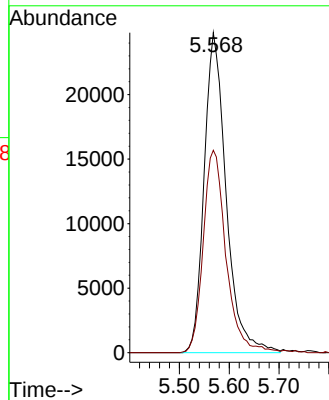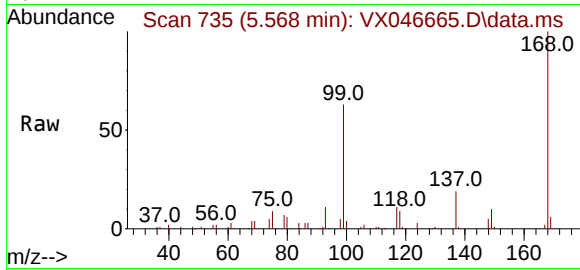

#16

Acetone

Concen: 7.921 ug/l

RT: 2.398 min Scan# 215

Delta R.T. 0.006 min

Lab File: VX046665.D




Acq: 12 Jun 2025 15:46


Tgt Ion: 43 Resp: 1798

Ion Ratio Lower Upper

43 100

58 33.7 21.2 31.8#

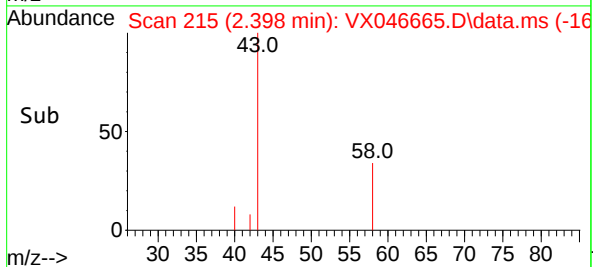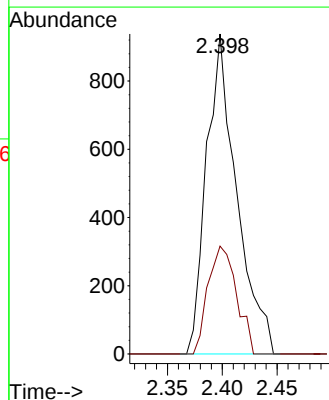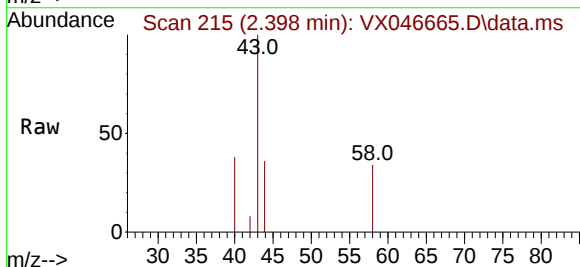



#33

1,2-Dichloroethane-d4

Concen: 50.402 ug/l

RT: 5.970 min Scan# 801

Delta R.T. 0.000 min

Lab File: VX046665.D

Acq: 12 Jun 2025 15:46

Instrument :

MSVOA_X

ClientSampleId :





OW-08B-72.5-060925

Tgt Ion: 65 Resp: 68098

Ion Ratio Lower Upper

65 100

67 50.2 0.0 99.0

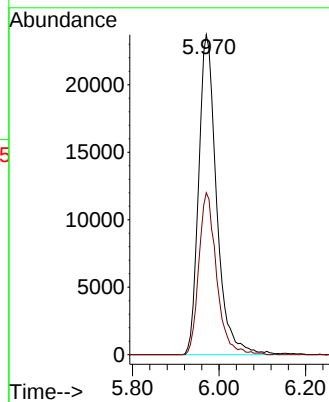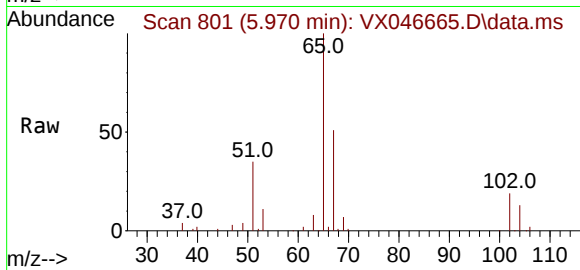

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.775 min Scan# 933

Delta R.T. 0.000 min

Lab File: VX046665.D

Acq: 12 Jun 2025 15:46




Tgt Ion: 114 Resp: 133627


Ion Ratio Lower Upper

114 100

63 21.3 0.0 49.2

88 16.1 0.0 33.6

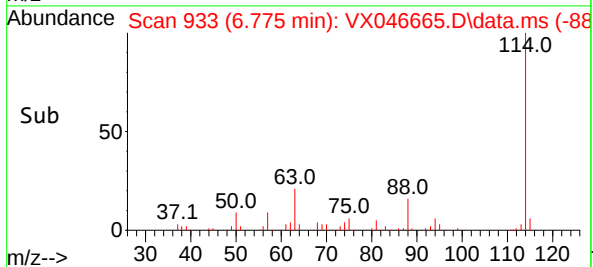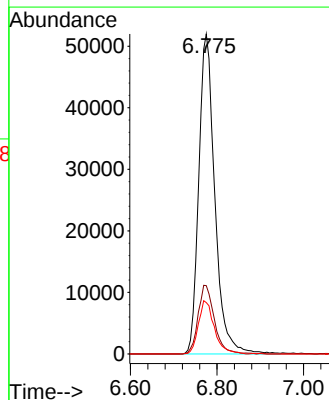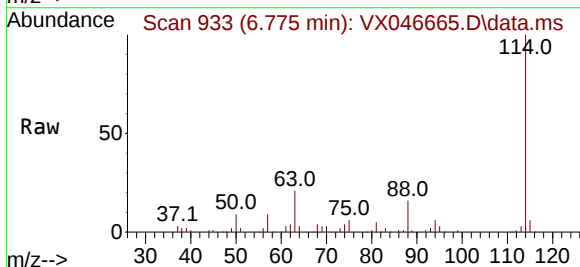



#35

Dibromofluoromethane

Concen: 53.880 ug/l

RT: 5.403 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX046665.D


Acq: 12 Jun 2025 15:46

Instrument :

MSVOA_X

ClientSampleId :

OW-08B-72.5-060925

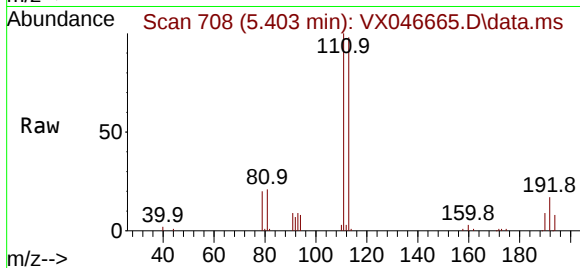




Tgt Ion:113 Resp: 52947

Ion Ratio Lower Upper

113 100

111 102.2 83.1 124.7

192 18.3 13.3 19.9

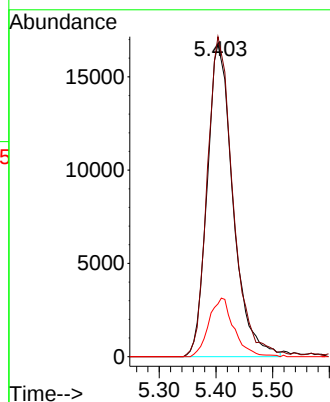

#50

Toluene-d8

Concen: 52.098 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX046665.D




Acq: 12 Jun 2025 15:46


Tgt Ion: 98 Resp: 168786

Ion Ratio Lower Upper

98 100

100 66.6 53.5 80.3

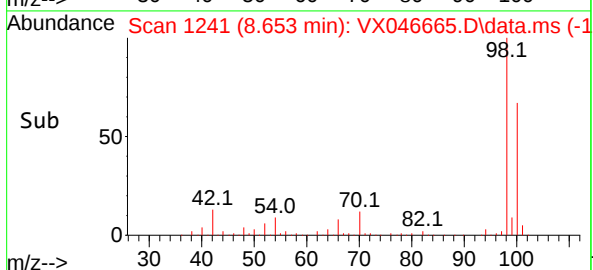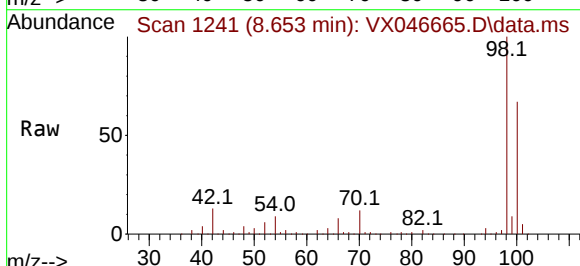



#62

4-Bromofluorobenzene

Concen: 53.442 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX046665.D

Acq: 12 Jun 2025 15:46

Instrument :

MSVOA_X

ClientSampleId :

OW-08B-72.5-060925





Tgt Ion: 95 Resp: 71637

Ion Ratio Lower Upper

95 100

174 71.4 0.0 135.8

176 68.9 0.0 131.4

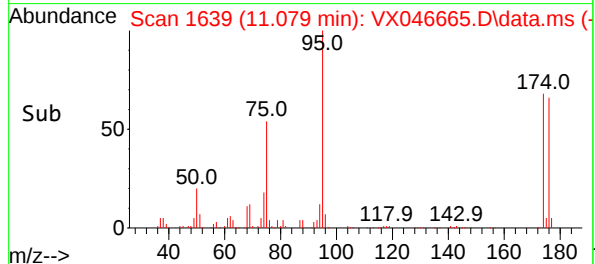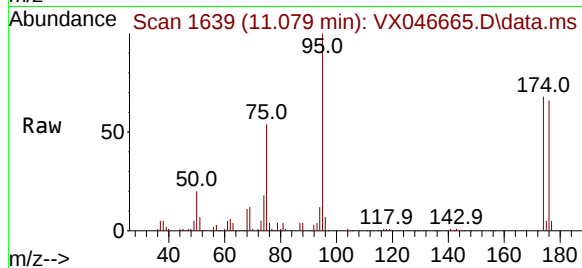

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX046665.D

Acq: 12 Jun 2025 15:46




Tgt Ion: 117 Resp: 120396


Ion Ratio Lower Upper

117 100

82 56.6 50.6 76.0

119 32.9 25.8 38.6

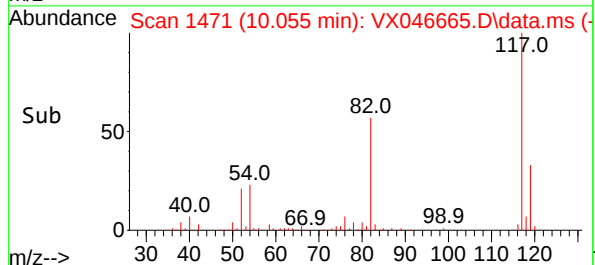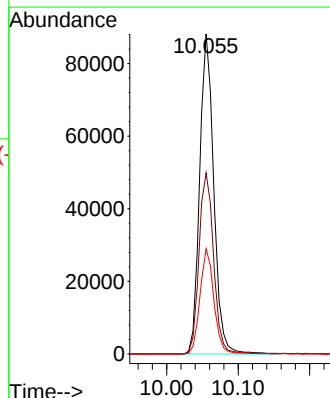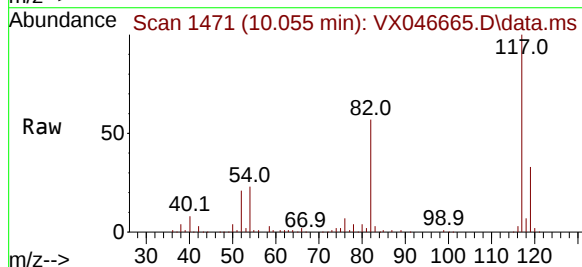



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX046665.D


Acq: 12 Jun 2025 15:46

Instrument :

MSVOA_X

ClientSampleId :

OW-08B-72.5-060925

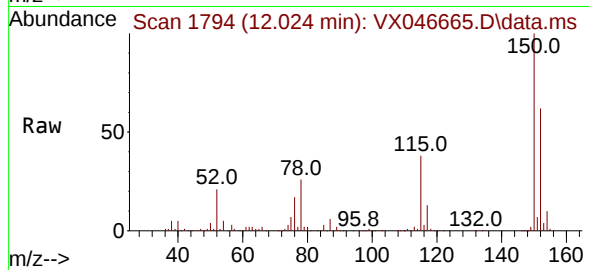



Tgt Ion:152 Resp: 61889

Ion Ratio Lower Upper

152 100

115 63.9 46.9 140.7

150 161.2 0.0 351.0

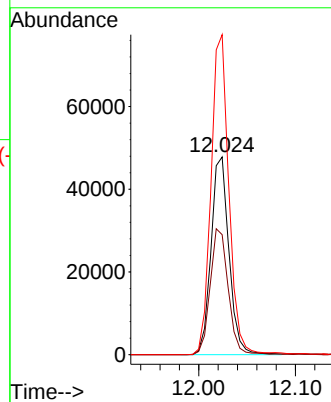

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046667.D
 Acq On : 12 Jun 2025 16:32
 Operator : JC/MD
 Sample : Q2275-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB01-060925

Quant Time: Jun 13 01:46:03 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.574	168	68445	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	127742	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	114769	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	59204	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	67313	55.279	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	110.560%
35) Dibromofluoromethane	5.403	113	53151	56.579	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	113.160%
50) Toluene-d8	8.653	98	168357	54.359	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	108.720%
62) 4-Bromofluorobenzene	11.079	95	70746	55.209	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	110.420%
Target Compounds						
16) Acetone	2.398	43	4909	14.672	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
Data File : VX046667.D
Acq On : 12 Jun 2025 16:32
Operator : JC/MD
Sample : Q2275-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB01-060925

Quant Time: Jun 13 01:46:03 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration




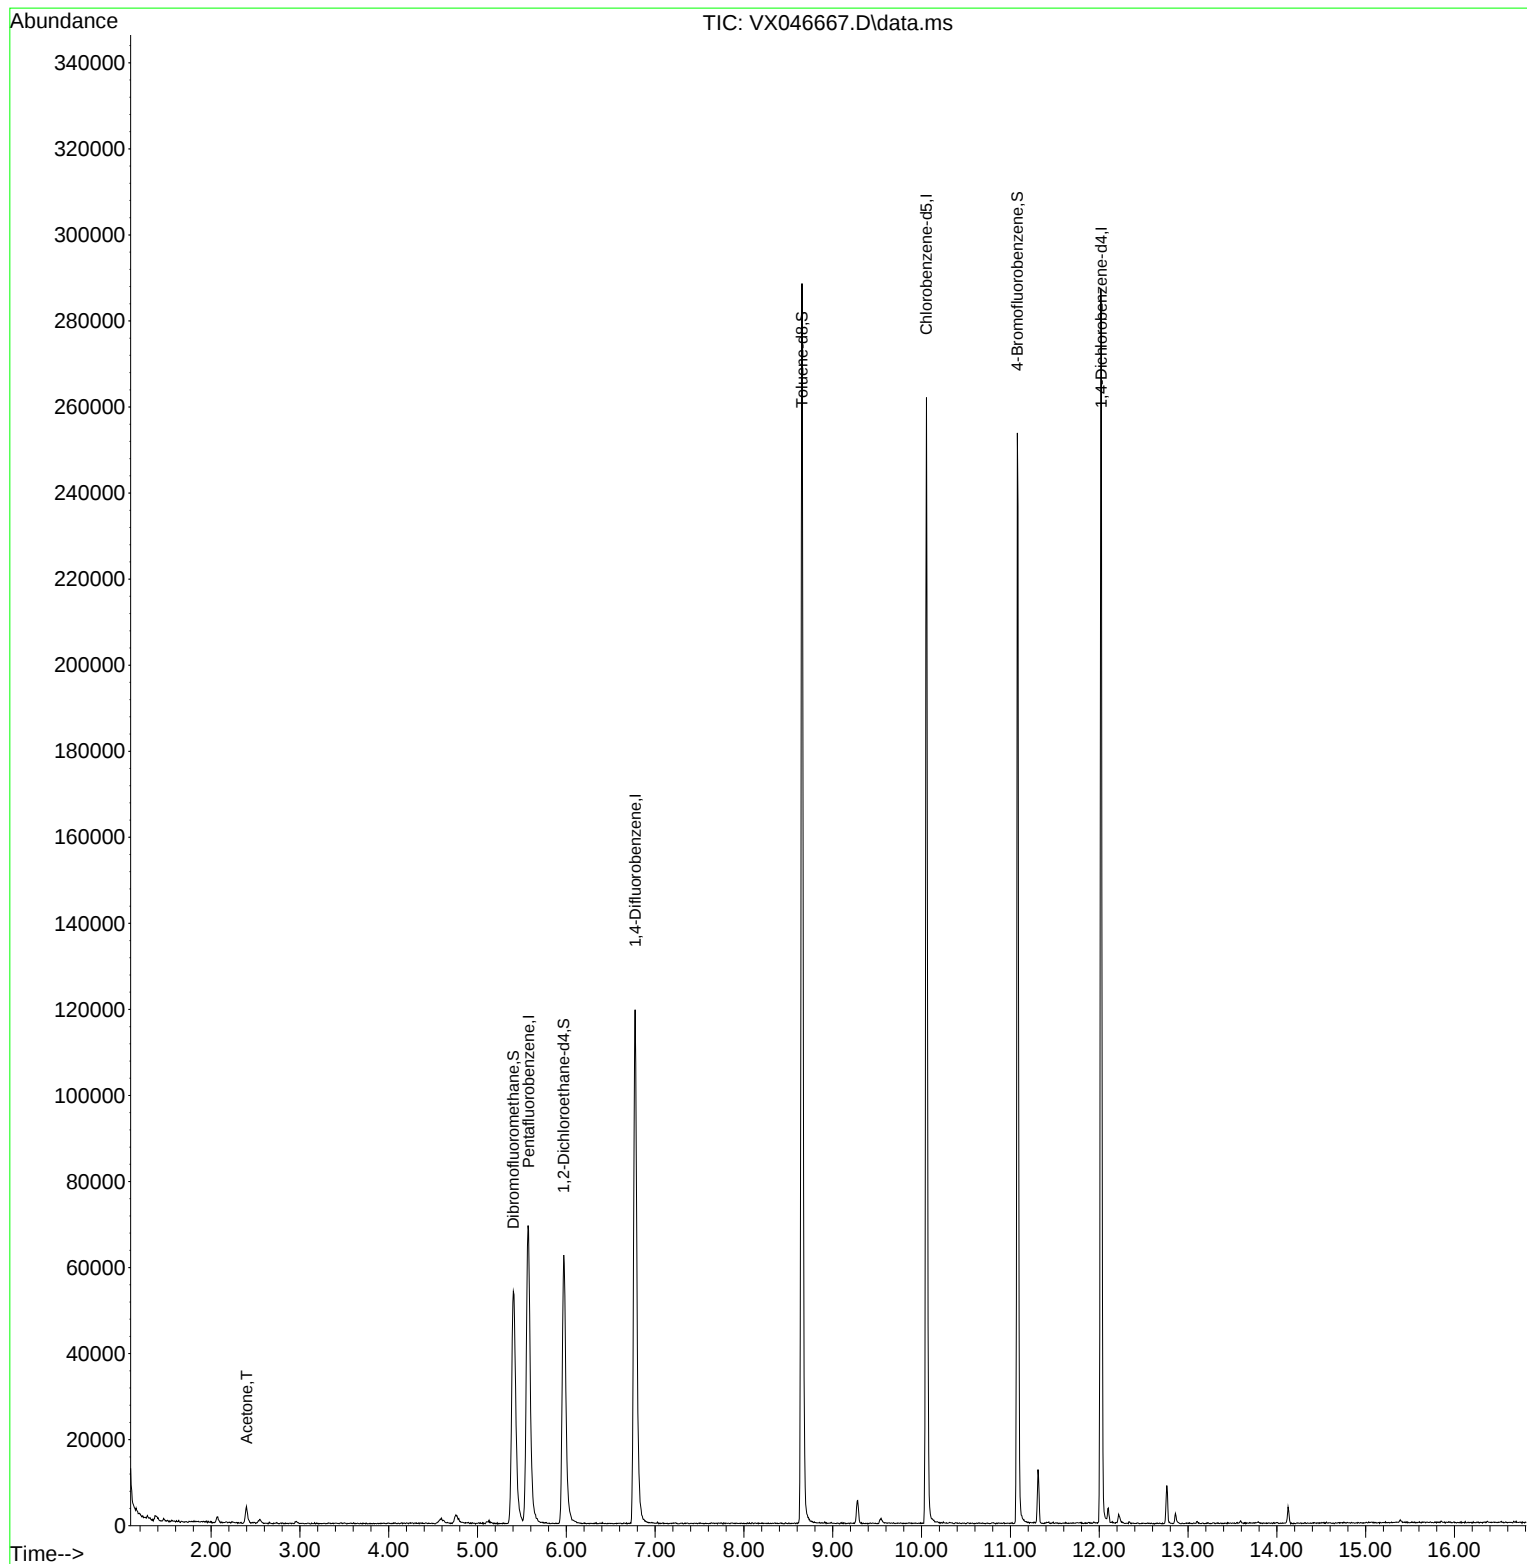




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.574 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX046667.D
Acq: 12 Jun 2025 16:32




Instrument :
MSVOA_X
ClientSampleId :
EB01-060925


Tgt Ion:168 Resp: 68445
Ion Ratio Lower Upper
168 100
99 60.3 54.9 82.3



#16
Acetone
Concen: 14.672 ug/l
RT: 2.398 min Scan# 215
Delta R.T. 0.006 min
Lab File: VX046667.D
Acq: 12 Jun 2025 16:32

Tgt Ion: 43 Resp: 4909
Ion Ratio Lower Upper
43 100
58 28.0 21.2 31.8

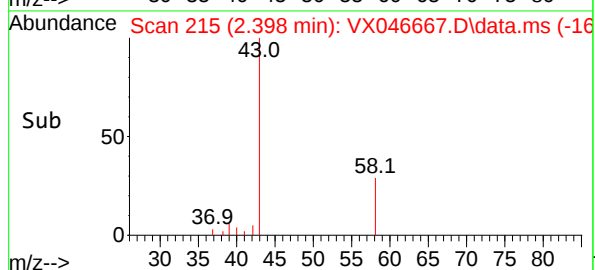



#33

1,2-Dichloroethane-d4

Concen: 55.279 ug/l

RT: 5.970 min Scan# 801

Delta R.T. 0.000 min

Lab File: VX046667.D

Acq: 12 Jun 2025 16:32

Instrument :

MSVOA_X

ClientSampleId :





EB01-060925

Tgt Ion: 65 Resp: 67313

Ion Ratio Lower Upper

65 100

67 51.0 0.0 99.0

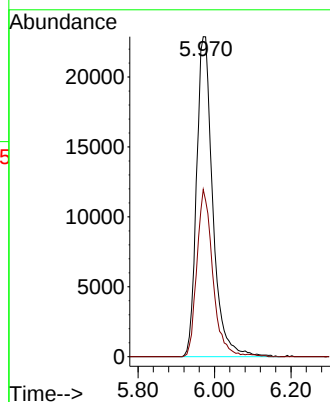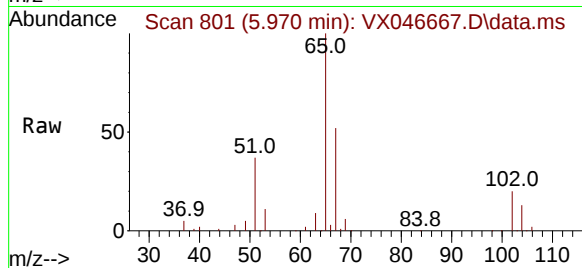

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.775 min Scan# 933

Delta R.T. 0.000 min

Lab File: VX046667.D

Acq: 12 Jun 2025 16:32




Tgt Ion: 114 Resp: 127742


Ion Ratio Lower Upper

114 100

63 20.7 0.0 49.2

88 16.7 0.0 33.6

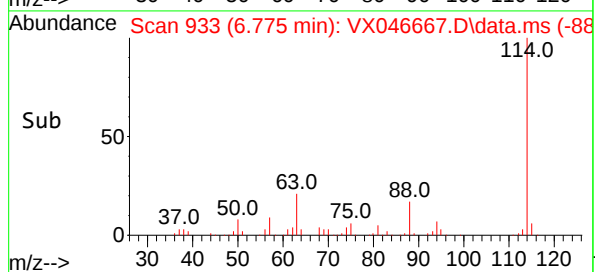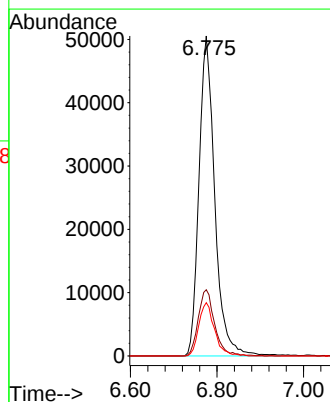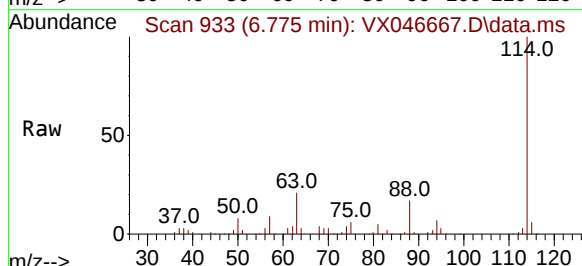



#35

Dibromofluoromethane

Concen: 56.579 ug/l

RT: 5.403 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX046667.D

Acq: 12 Jun 2025 16:32

Instrument :

MSVOA_X

ClientSampleId :

EB01-060925





Tgt Ion:113 Resp: 53151

Ion Ratio Lower Upper

113 100

111 103.4 83.1 124.7

192 17.8 13.3 19.9

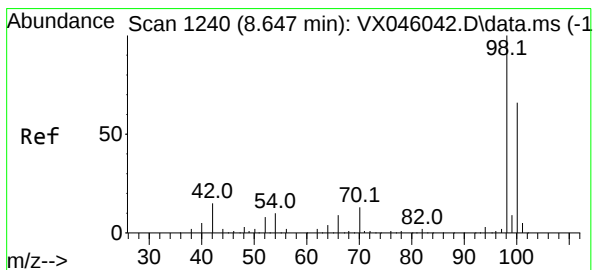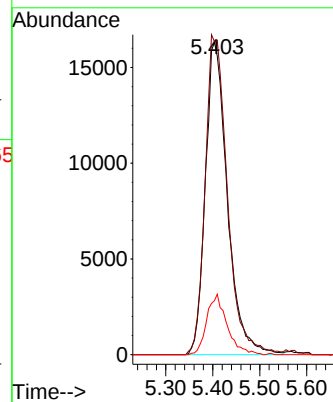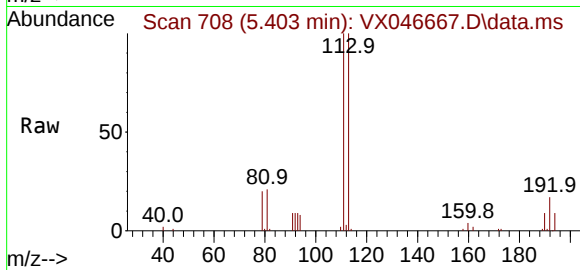

#50

Toluene-d8

Concen: 54.359 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX046667.D




Acq: 12 Jun 2025 16:32


Tgt Ion: 98 Resp: 168357

Ion Ratio Lower Upper

98 100

100 66.8 53.5 80.3


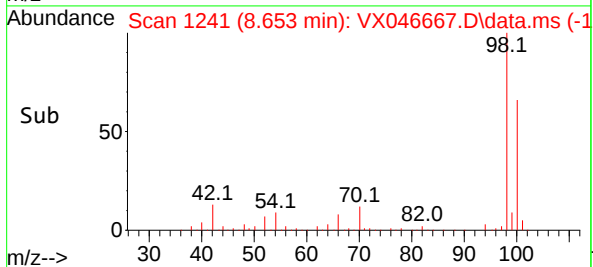
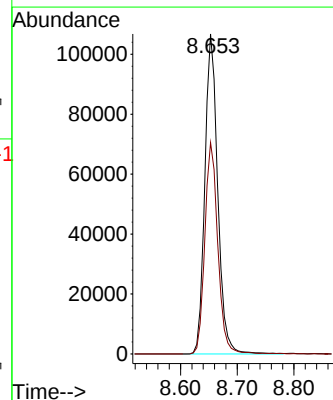
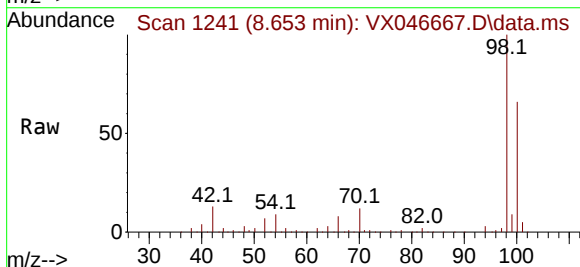




#62
4-Bromofluorobenzene
Concen: 55.209 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX046667.D
Acq: 12 Jun 2025 16:32




Instrument :
MSVOA_X
ClientSampleId :
EB01-060925


Tgt Ion: 95 Resp: 70746
Ion Ratio Lower Upper
95 100
174 71.4 0.0 135.8
176 67.8 0.0 131.4

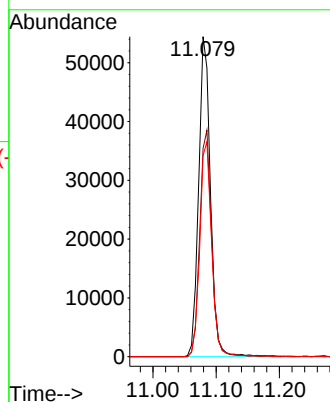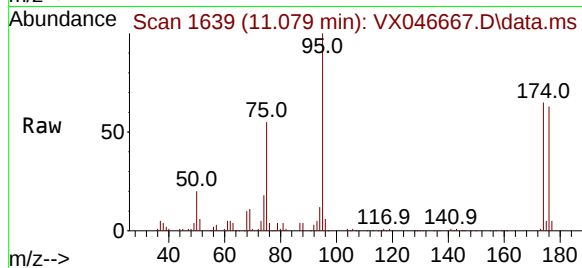

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX046667.D
Acq: 12 Jun 2025 16:32

Tgt Ion: 117 Resp: 114769
Ion Ratio Lower Upper
117 100
82 59.1 50.6 76.0
119 33.5 25.8 38.6

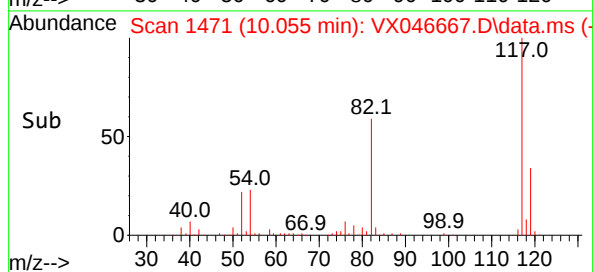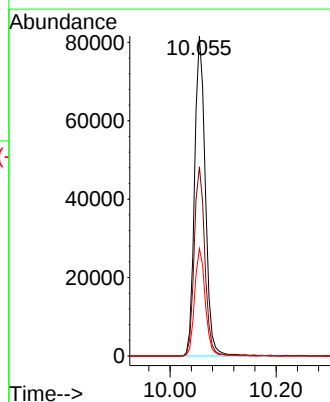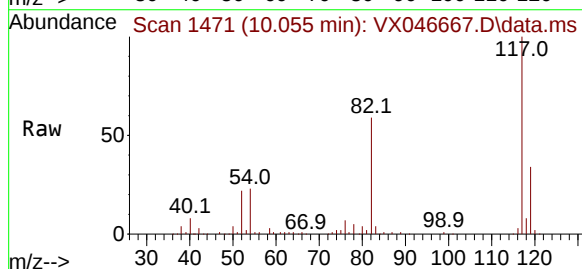



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX046667.D


Acq: 12 Jun 2025 16:32

Instrument :

MSVOA_X

ClientSampleId :

EB01-060925

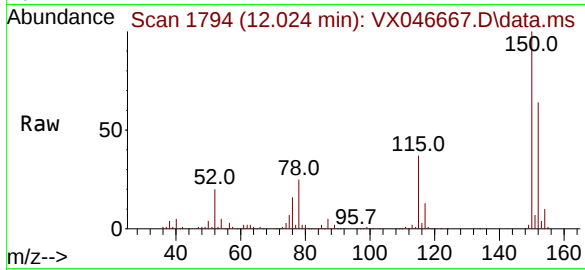



Tgt Ion:152 Resp: 59204

Ion Ratio Lower Upper

152 100

115 61.1 46.9 140.7

150 157.1 0.0 351.0

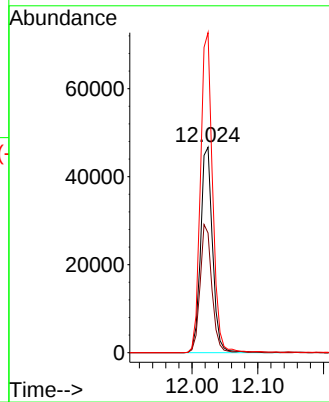

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046668.D
 Acq On : 12 Jun 2025 16:55
 Operator : JC/MD
 Sample : Q2275-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB01-060925

Quant Time: Jun 13 01:46:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.574	168	87075	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	148474	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	135692	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	70754	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	64851	41.862	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	83.720%
35) Dibromofluoromethane	5.403	113	51974	47.601	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.200%
50) Toluene-d8	8.653	98	165485	45.971	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.940%
62) 4-Bromofluorobenzene	11.079	95	68623	46.075	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	92.140%
Target Compounds						
16) Acetone	2.392	43	999	6.206	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
Data File : VX046668.D
Acq On : 12 Jun 2025 16:55
Operator : JC/MD
Sample : Q2275-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-060925

Quant Time: Jun 13 01:46:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

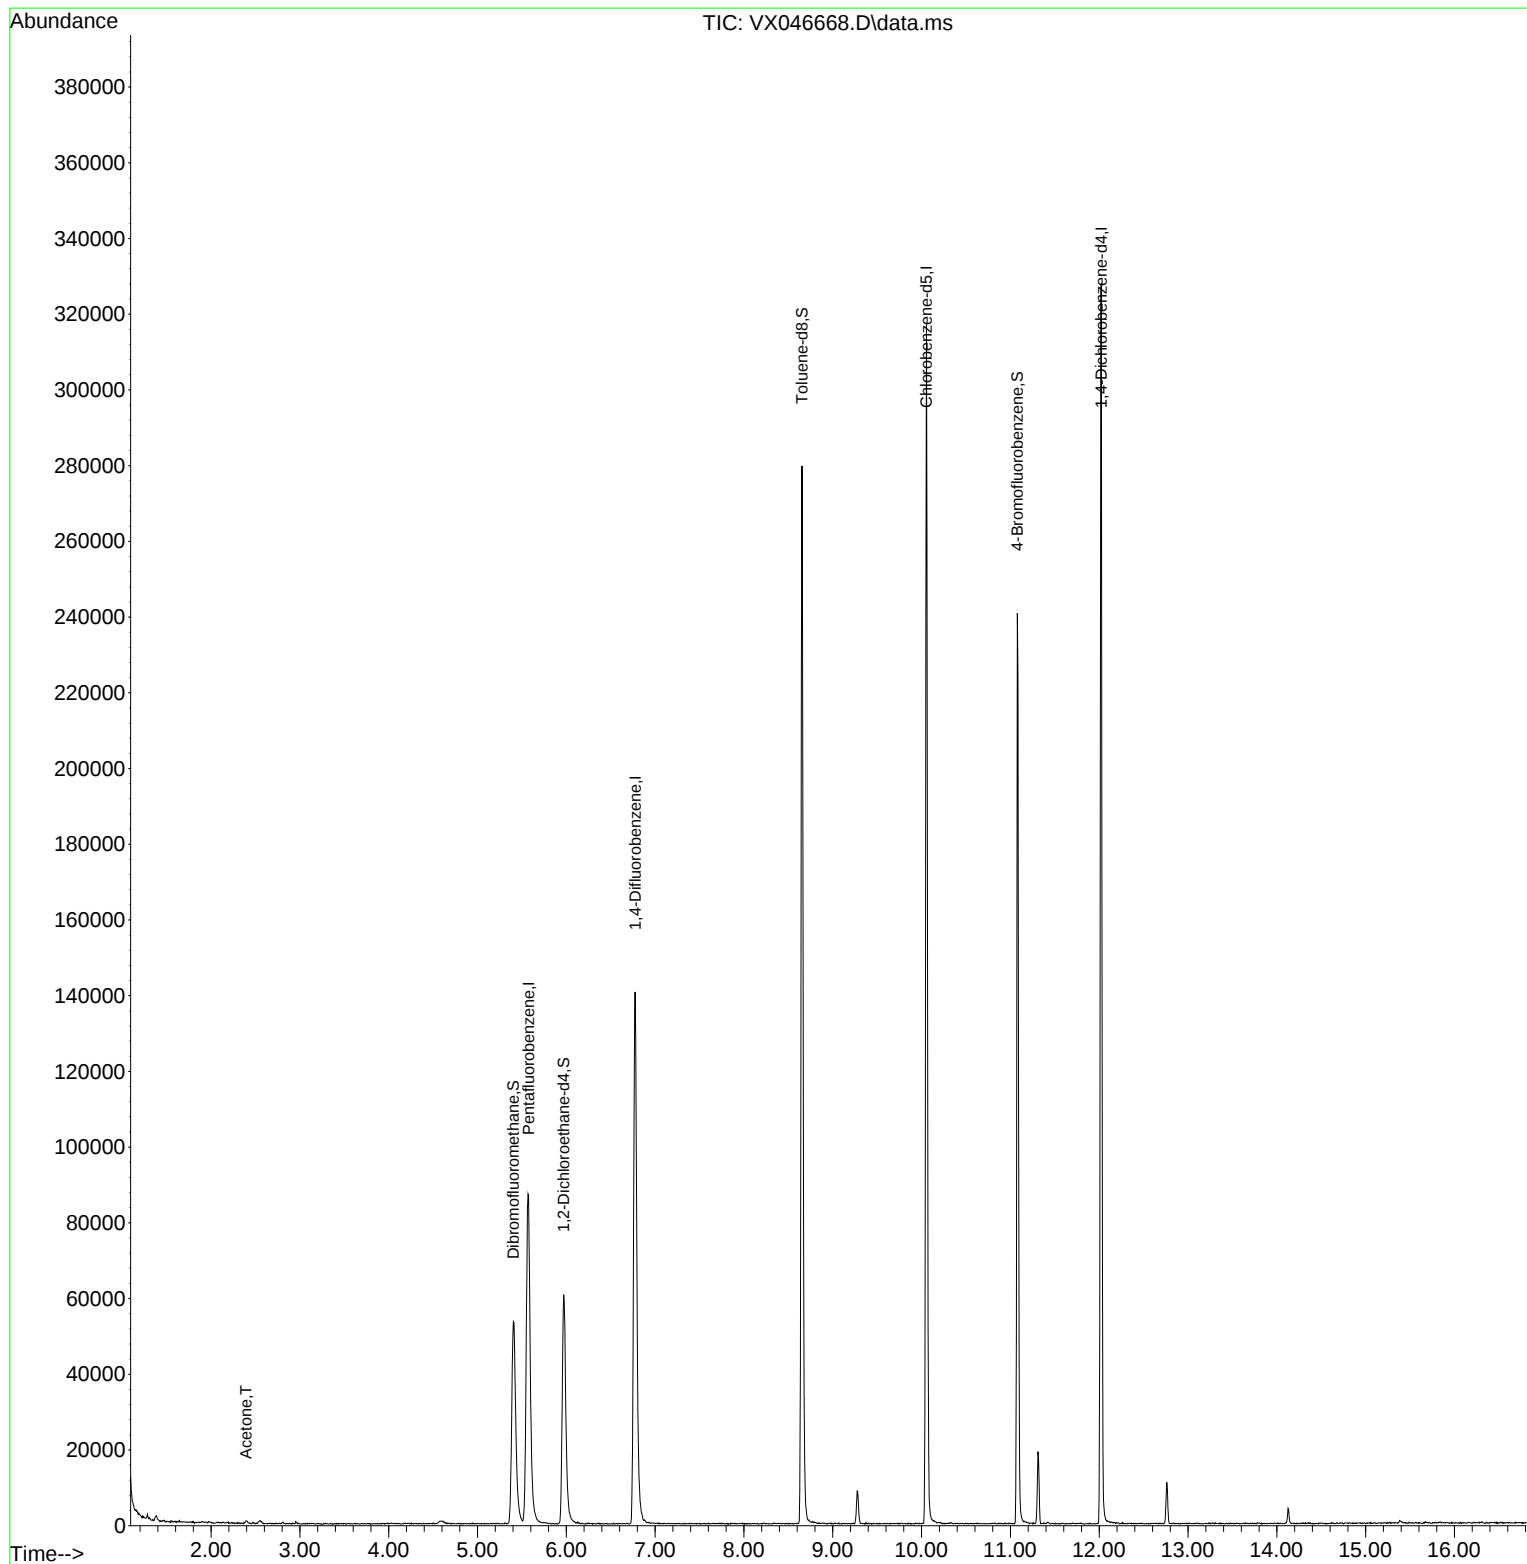

#1
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.574 min Scan# 71

Delta R.T. 0.006 min

Lab File: VX046668.D

Acq: 12 Jun 2025 16:55

Instrument :

MSVOA_X

ClientSampleId :





TB01-060925

Tgt Ion:168 Resp: 87075

Ion Ratio Lower Upper

168 100

99 63.1 54.9 82.3

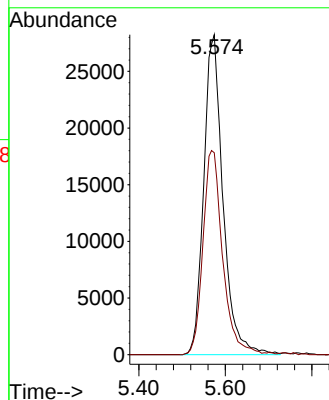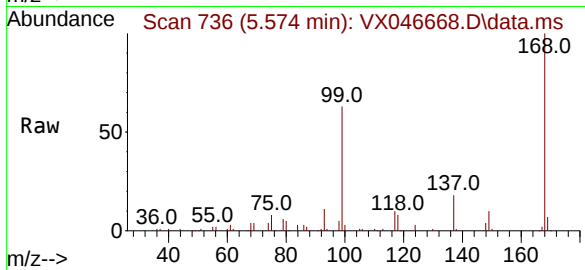

#16

Acetone

Concen: 6.206 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX046668.D




Acq: 12 Jun 2025 16:55


Tgt Ion: 43 Resp: 999

Ion Ratio Lower Upper

43 100

58 21.5 21.2 31.8

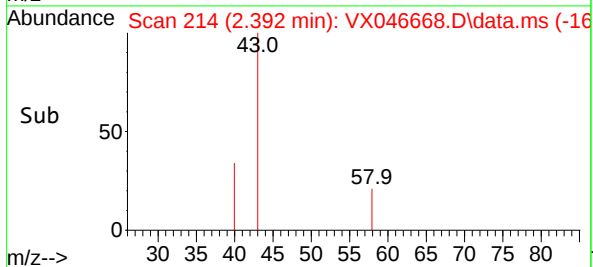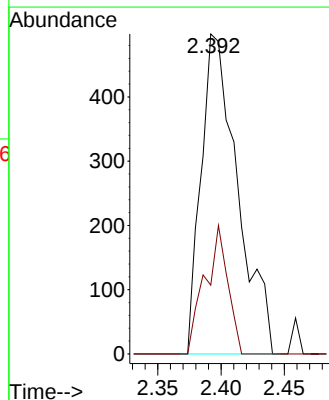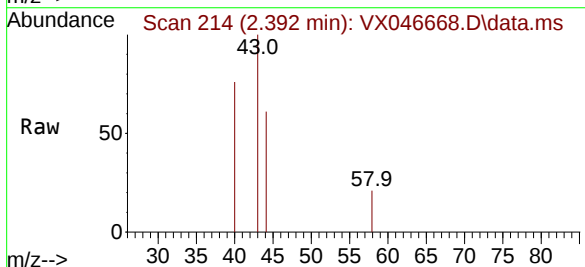



#33

1,2-Dichloroethane-d4

Concen: 41.862 ug/l

RT: 5.970 min Scan# 801

Delta R.T. 0.000 min

Lab File: VX046668.D

Acq: 12 Jun 2025 16:55

Instrument :

MSVOA_X

ClientSampleId :





TB01-060925

Tgt Ion: 65 Resp: 64851

Ion Ratio Lower Upper

65 100

67 51.0 0.0 99.0

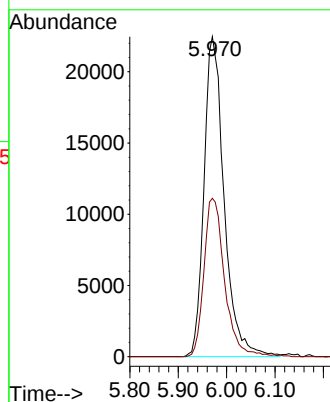

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.775 min Scan# 933

Delta R.T. 0.000 min

Lab File: VX046668.D

Acq: 12 Jun 2025 16:55




Tgt Ion: 114 Resp: 148474


Ion Ratio Lower Upper

114 100

63 21.3 0.0 49.2

88 16.1 0.0 33.6

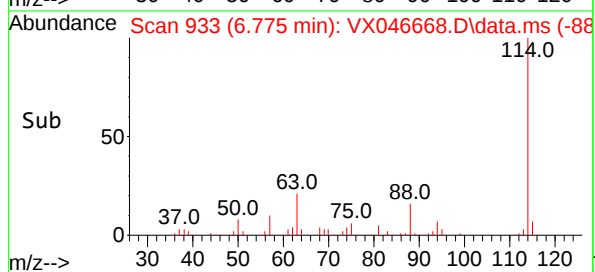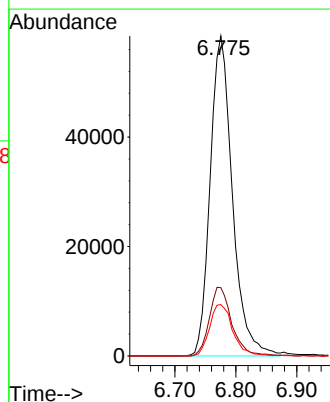



#35

Dibromofluoromethane

Concen: 47.601 ug/l

RT: 5.403 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX046668.D


Acq: 12 Jun 2025 16:55

Instrument :

MSVOA_X

ClientSampleId :

TB01-060925

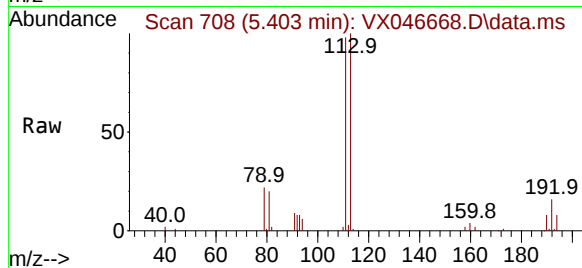




Tgt Ion:113 Resp: 51974

Ion Ratio Lower Upper

113 100

111 102.0 83.1 124.7

192 17.6 13.3 19.9



#50

Toluene-d8

Concen: 45.971 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX046668.D




Acq: 12 Jun 2025 16:55


Tgt Ion: 98 Resp: 165485

Ion Ratio Lower Upper

98 100

100 66.2 53.5 80.3



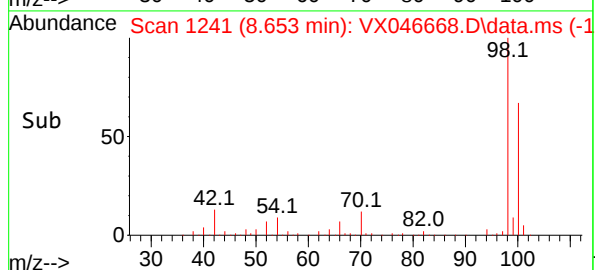
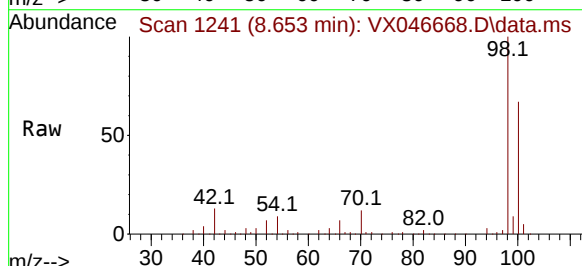




#62
4-Bromofluorobenzene
Concen: 46.075 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX046668.D
Acq: 12 Jun 2025 16:55




Instrument :
MSVOA_X
ClientSampleId :
TB01-060925


Tgt Ion: 95 Resp: 68623
Ion Ratio Lower Upper
95 100
174 71.9 0.0 135.8
176 69.2 0.0 131.4

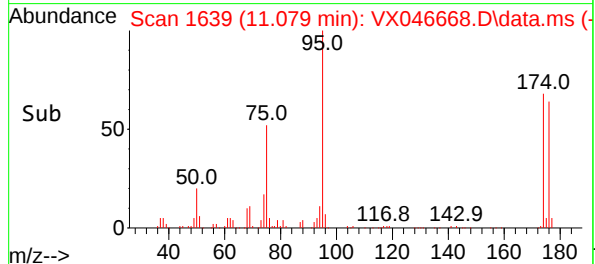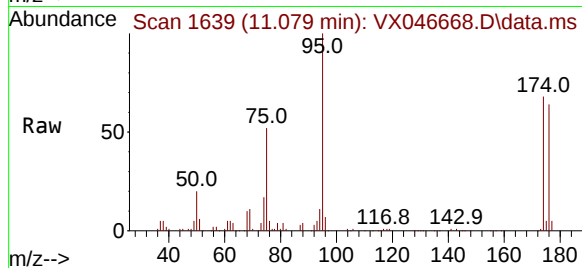

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX046668.D
Acq: 12 Jun 2025 16:55

Tgt Ion: 117 Resp: 135692
Ion Ratio Lower Upper
117 100
82 57.3 50.6 76.0
119 32.0 25.8 38.6

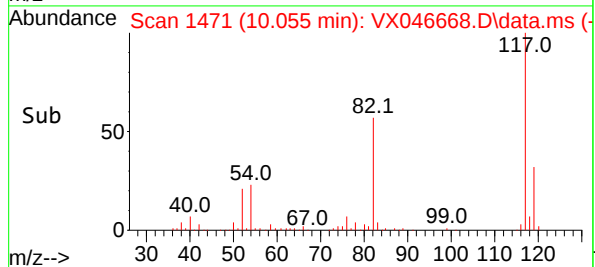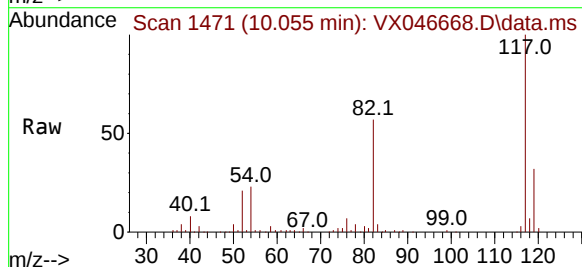



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX046668.D


Acq: 12 Jun 2025 16:55

Instrument :

MSVOA_X

ClientSampleId :

TB01-060925

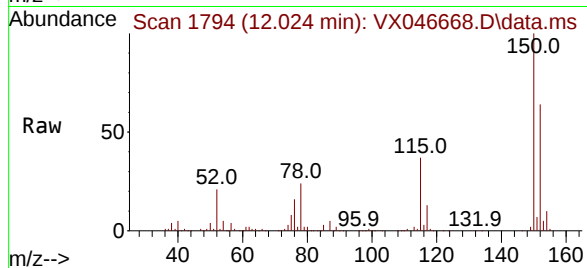



Tgt Ion:152 Resp: 70754

Ion Ratio Lower Upper

152 100

115 60.8 46.9 140.7

150 156.1 0.0 351.0

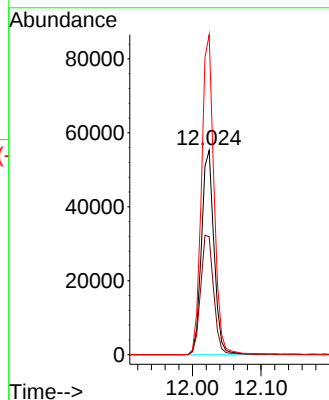

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046659.D
 Acq On : 12 Jun 2025 13:10
 Operator : JC/MD
 Sample : VX0612WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0612WBL01

A
B
C
D
E
F
G
H
I
J

Quant Time: Jun 13 01:42:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	92224	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	180952	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	188641	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	95358	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.971	65	75758	46.173	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.340%
35) Dibromofluoromethane	5.404	113	64522	48.487	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.980%
50) Toluene-d8	8.653	98	229993	52.424	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	104.840%
62) 4-Bromofluorobenzene	11.079	95	99118	54.605	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	109.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
Data File : VX046659.D
Acq On : 12 Jun 2025 13:10
Operator : JC/MD
Sample : VX0612WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0612WBL01

Quant Time: Jun 13 01:42:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration




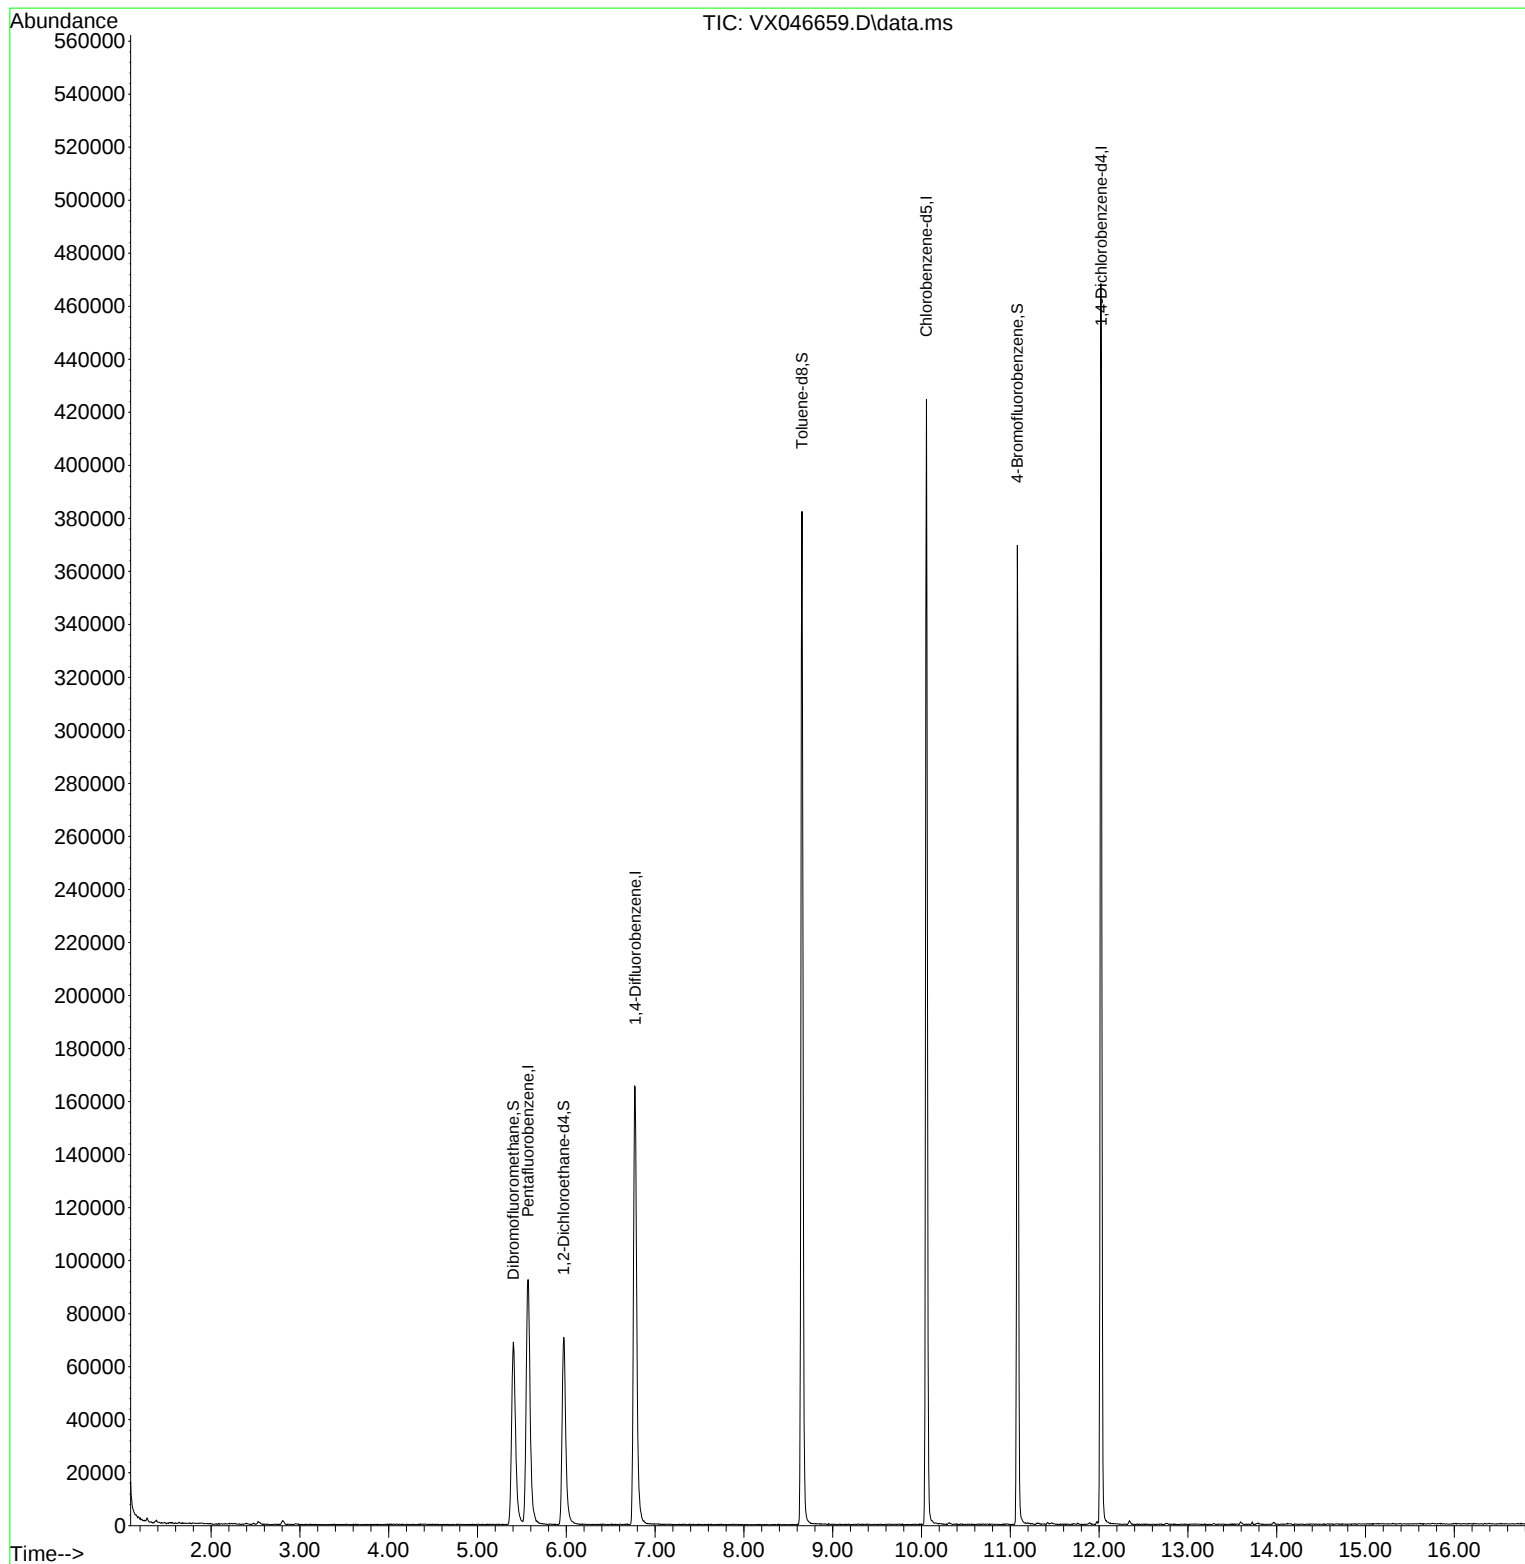




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.568 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX046659.D
Acq: 12 Jun 2025 13:10




Instrument :
MSVOA_X
ClientSampleId :
VX0612WBL01


Tgt Ion:168 Resp: 92224
Ion Ratio Lower Upper
168 100
99 63.0 54.9 82.3

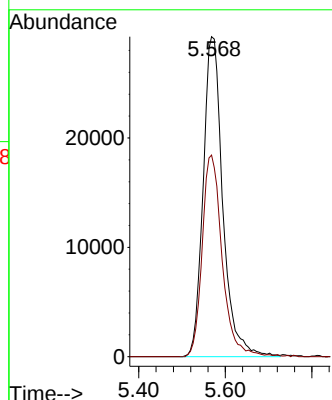

#33
1,2-Dichloroethane-d4
Concen: 46.173 ug/l
RT: 5.971 min Scan# 801
Delta R.T. 0.001 min
Lab File: VX046659.D
Acq: 12 Jun 2025 13:10

Tgt Ion: 65 Resp: 75758
Ion Ratio Lower Upper
65 100
67 50.0 0.0 99.0


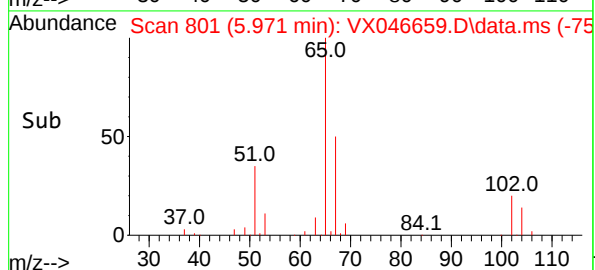
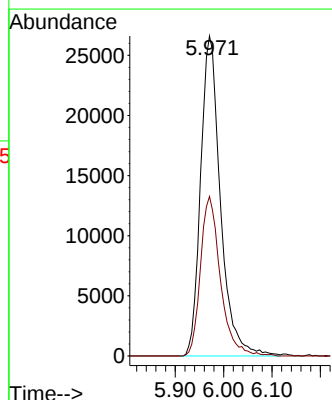
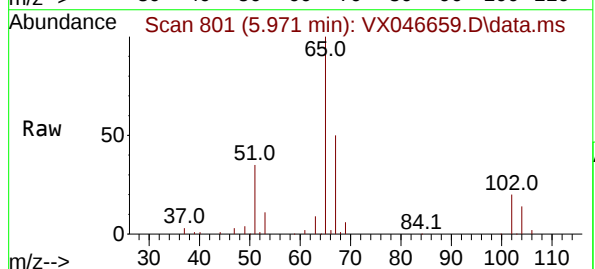




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.775 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX046659.D
Acq: 12 Jun 2025 13:10




Instrument :
MSVOA_X
ClientSampleId :
VX0612WBL01


Tgt Ion:114 Resp: 180952
Ion Ratio Lower Upper
114 100
63 21.2 0.0 49.2
88 16.7 0.0 33.6

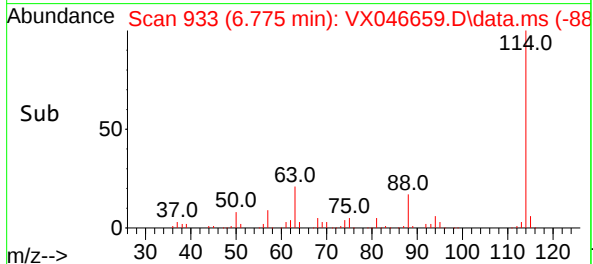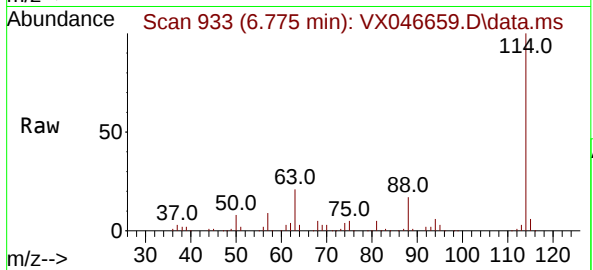

#35
Dibromofluoromethane
Concen: 48.487 ug/l
RT: 5.404 min Scan# 708
Delta R.T. 0.001 min
Lab File: VX046659.D
Acq: 12 Jun 2025 13:10

Tgt Ion:113 Resp: 64522
Ion Ratio Lower Upper
113 100
111 103.6 83.1 124.7
192 18.1 13.3 19.9

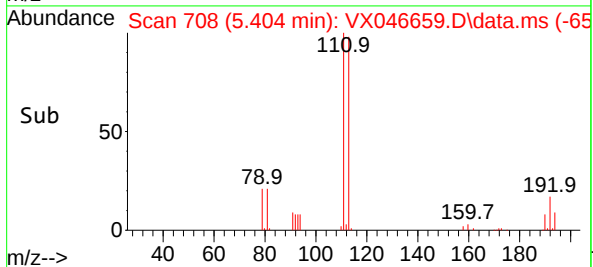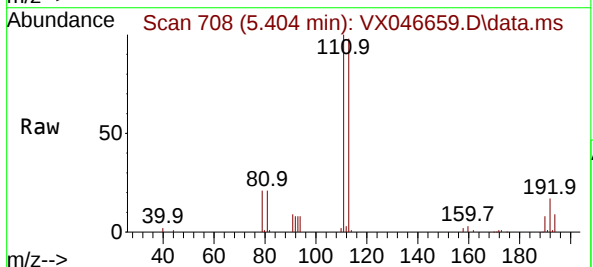



#50

Toluene-d8

Concen: 52.424 ug/l

RT: 8.653 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046659.D

Acq: 12 Jun 2025 13:10

Instrument :

MSVOA_X

ClientSampleId :





VX0612WBL01

Tgt Ion: 98 Resp: 229993

Ion Ratio Lower Upper

98 100

100 66.6 53.5 80.3

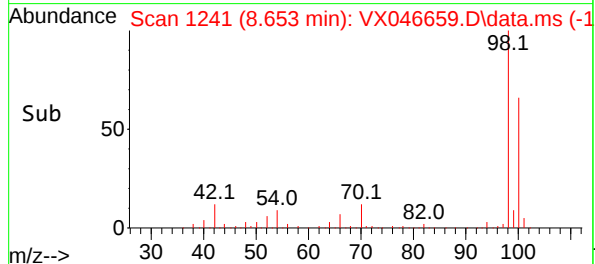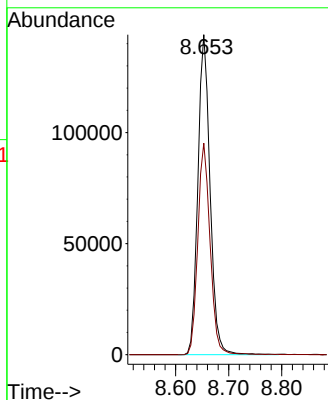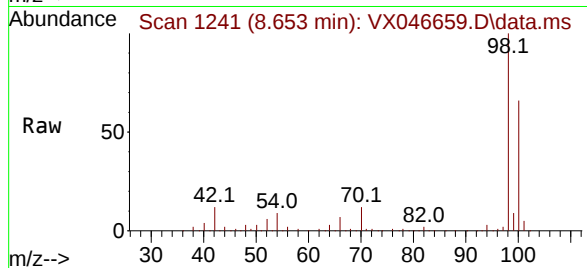

#62

4-Bromofluorobenzene

Concen: 54.605 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX046659.D

Acq: 12 Jun 2025 13:10




Tgt Ion: 95 Resp: 99118


Ion Ratio Lower Upper

95 100

174 73.2 0.0 135.8

176 70.9 0.0 131.4

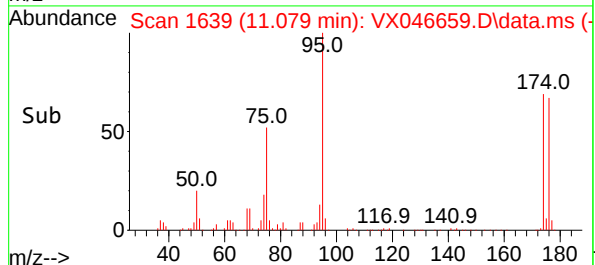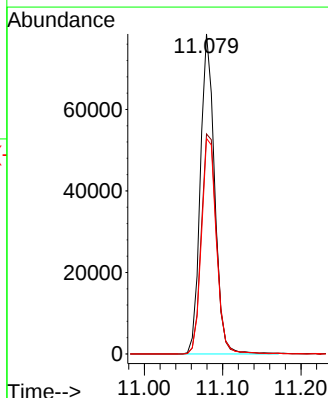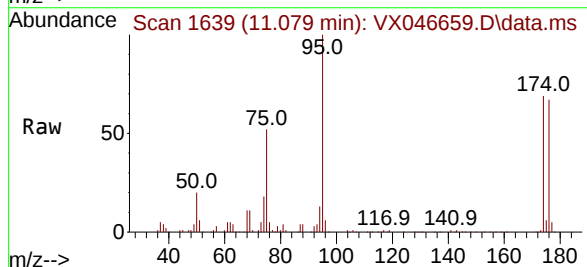



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX046659.D

Acq: 12 Jun 2025 13:10

Instrument :

MSVOA_X

ClientSampleId :

VX0612WBL01





Tgt Ion:117 Resp: 188641

Ion Ratio Lower Upper

117 100

82 56.0 50.6 76.0

119 32.4 25.8 38.6

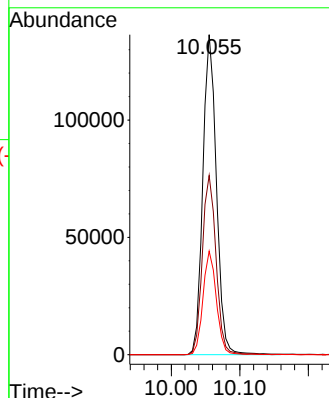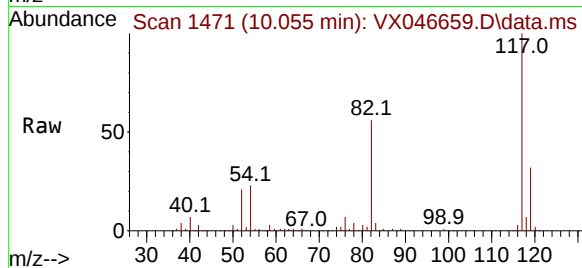

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX046659.D

Acq: 12 Jun 2025 13:10




Tgt Ion:152 Resp: 95358

Ion Ratio Lower Upper

152 100

115 63.2 46.9 140.7

150 156.4 0.0 351.0

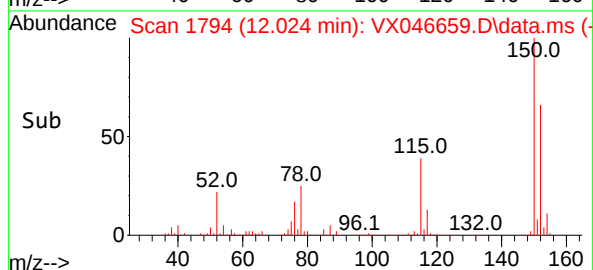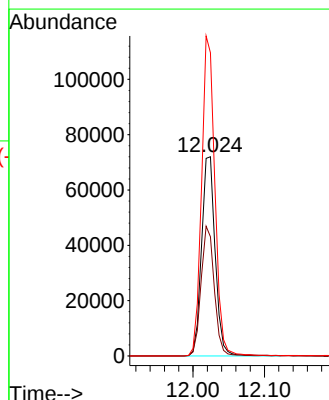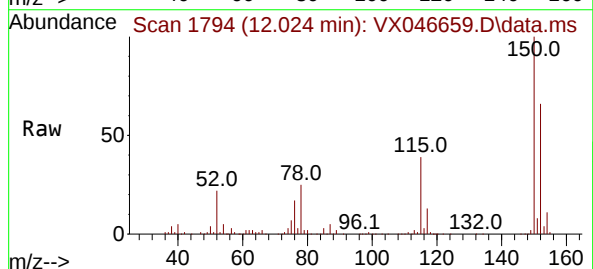

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046660.D
 Acq On : 12 Jun 2025 13:38
 Operator : JC/MD
 Sample : VX0612WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0612WBS01

Quant Time: Jun 13 01:42:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 06/13/2025
 Supervised By : Mahesh Dadoda 06/13/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	85578	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.769	114	144622	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	130715	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	69016	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	63210	41.517	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	83.040%		
35) Dibromofluoromethane	5.397	113	51021	47.973	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.940%		
50) Toluene-d8	8.647	98	167446	47.755	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.500%		
62) 4-Bromofluorobenzene	11.079	95	69758	48.084	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	96.160%		
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.185	85	17232	14.504	ug/l	100
3) Chloromethane	1.306	50	15679	14.498	ug/l	97
4) Vinyl Chloride	1.386	62	16285	15.106	ug/l	100
5) Bromomethane	1.623	94	10482	16.017	ug/l	99
6) Chloroethane	1.703	64	10352	14.800	ug/l	95
7) Trichlorofluoromethane	1.904	101	27911	15.648	ug/l	92
8) Diethyl Ether	2.148	74	10221	16.219	ug/l	87
9) 1,1,2-Trichlorotrifluo...	2.343	101	19140	17.032	ug/l	95
10) Methyl Iodide	2.465	142	17822	14.630	ug/l	95
11) Tert butyl alcohol	2.965	59	14604	86.443	ug/l	99
12) 1,1-Dichloroethene	2.331	96	17566	17.289	ug/l	84
13) Acrolein	2.251	56	9994	73.047	ug/l	100
14) Allyl chloride	2.678	41	33622	16.850	ug/l	93
15) Acrylonitrile	3.074	53	58711	91.913	ug/l	99
16) Acetone	2.392	43	52132	90.187	ug/l	92
17) Carbon Disulfide	2.526	76	33805	15.809	ug/l	100
18) Methyl Acetate	2.715	43	35232	19.427	ug/l	95
19) Methyl tert-butyl Ether	3.129	73	66811	18.793	ug/l	98
20) Methylene Chloride	2.800	84	21926	17.951	ug/l	92
21) trans-1,2-Dichloroethene	3.105	96	18523	17.227	ug/l	97
22) Diisopropyl ether	3.769	45	72754	18.494	ug/l #	65
23) Vinyl Acetate	3.733	43	272827	89.826	ug/l	99
24) 1,1-Dichloroethane	3.623	63	38925	17.753	ug/l	99
25) 2-Butanone	4.568	43	74592	88.008	ug/l	96
26) 2,2-Dichloropropane	4.483	77	29645	18.213	ug/l	97
27) cis-1,2-Dichloroethene	4.501	96	23891	18.050	ug/l	95
28) Bromochloromethane	4.909	49	26095	24.953	ug/l	92
29) Tetrahydrofuran	5.013	42	45745	85.463	ug/l	96
30) Chloroform	5.105	83	41974	18.271	ug/l	97
31) Cyclohexane	5.476	56	29749	16.807	ug/l	99
32) 1,1,1-Trichloroethane	5.391	97	35020	17.821	ug/l	97
36) 1,1-Dichloropropene	5.702	75	25822	16.997	ug/l	97
37) Ethyl Acetate	4.727	43	29586	19.954	ug/l	99
38) Carbon Tetrachloride	5.690	117	29642	17.420	ug/l	99
39) Methylcyclohexane	7.385	83	29365	16.376	ug/l	95
40) Benzene	6.049	78	79810	18.661	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046660.D
 Acq On : 12 Jun 2025 13:38
 Operator : JC/MD
 Sample : VX0612WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0612WBS01

Quant Time: Jun 13 01:42:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 06/13/2025
 Supervised By : Mahesh Dadoda 06/13/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.940	41	16120	17.507	ug/l #	92
42) 1,2-Dichloroethane	6.098	62	31253	17.565	ug/l	97
43) Isopropyl Acetate	6.348	43	46852	18.125	ug/l	96
44) Trichloroethene	7.129	130	20132	18.526	ug/l	97
45) 1,2-Dichloropropane	7.433	63	21411	19.396	ug/l	96
46) Dibromomethane	7.586	93	15723	18.933	ug/l	94
47) Bromodichloromethane	7.824	83	33506	19.622	ug/l	98
48) Methyl methacrylate	7.696	41	24360	18.316	ug/l	92
49) 1,4-Dioxane	7.659	88	6794	382.003	ug/l	99
51) 4-Methyl-2-Pentanone	8.573	43	158516	96.503	ug/l	97
52) Toluene	8.720	92	52013	19.796	ug/l	98
53) t-1,3-Dichloropropene	8.982	75	29385	19.193	ug/l	98
54) cis-1,3-Dichloropropene	8.372	75	32617	19.161	ug/l #	85
55) 1,1,2-Trichloroethane	9.153	97	21748	20.618	ug/l	99
56) Ethyl methacrylate	9.116	69	32307	19.903	ug/l	92
57) 1,3-Dichloropropane	9.311	76	35837	19.225	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.244	63	87671	99.160	ug/l	97
59) 2-Hexanone	9.433	43	113348	96.217	ug/l	95
60) Dibromochloromethane	9.518	129	25395	20.468	ug/l	98
61) 1,2-Dibromoethane	9.610	107	21756	19.793	ug/l	98
64) Tetrachloroethene	9.275	164	16534	18.916	ug/l	98
65) Chlorobenzene	10.079	112	59264	19.277	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.165	131	21995	21.172	ug/l	98
67) Ethyl Benzene	10.195	91	99830	18.601	ug/l	97
68) m/p-Xylenes	10.299	106	77489	39.802	ug/l	94
69) o-Xylene	10.640	106	37114	19.709	ug/l	98
70) Styrene	10.652	104	66406	20.601	ug/l	96
71) Bromoform	10.799	173	16330	20.616	ug/l #	99
73) Isopropylbenzene	10.963	105	101339	18.679	ug/l	99
74) N-amyl acetate	10.841	43	42555	17.811	ug/l	97
75) 1,1,2,2-Tetrachloroethane	11.213	83	33322	19.188	ug/l	98
76) 1,2,3-Trichloropropane	11.238	75	26882m	18.389	ug/l	
77) Bromobenzene	11.195	156	24285	19.285	ug/l	93
78) n-propylbenzene	11.305	91	118689	18.075	ug/l	98
79) 2-Chlorotoluene	11.366	91	72123	18.214	ug/l	98
80) 1,3,5-Trimethylbenzene	11.451	105	85488	18.909	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.018	75	9208	18.170	ug/l	91
82) 4-Chlorotoluene	11.451	91	86099	18.344	ug/l	97
83) tert-Butylbenzene	11.713	119	84512	18.363	ug/l	95
84) 1,2,4-Trimethylbenzene	11.750	105	85107	18.609	ug/l	98
85) sec-Butylbenzene	11.890	105	106791	18.059	ug/l	99
86) p-Isopropyltoluene	12.006	119	92930	18.850	ug/l	98
87) 1,3-Dichlorobenzene	11.969	146	47662	19.491	ug/l	98
88) 1,4-Dichlorobenzene	12.036	146	48120	18.991	ug/l	99
89) n-Butylbenzene	12.329	91	85715	17.705	ug/l	99
90) Hexachloroethane	12.536	117	15279	17.437	ug/l	91
91) 1,2-Dichlorobenzene	12.335	146	45679	19.352	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.945	75	6541	16.820	ug/l	80
93) 1,2,4-Trichlorobenzene	13.585	180	31308	19.444	ug/l	97
94) Hexachlorobutadiene	13.725	225	13715	18.328	ug/l	99
95) Naphthalene	13.774	128	101037	19.787	ug/l	99
96) 1,2,3-Trichlorobenzene	13.957	180	30574	18.936	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
Data File : VX046660.D
Acq On : 12 Jun 2025 13:38
Operator : JC/MD
Sample : VX0612WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 13 01:42:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Instrument :
MSVOA_X
ClientSampleId :
VX0612WBS01

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_X
ClientSampleId :
VX0612WBS01

Manual Integrations APPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

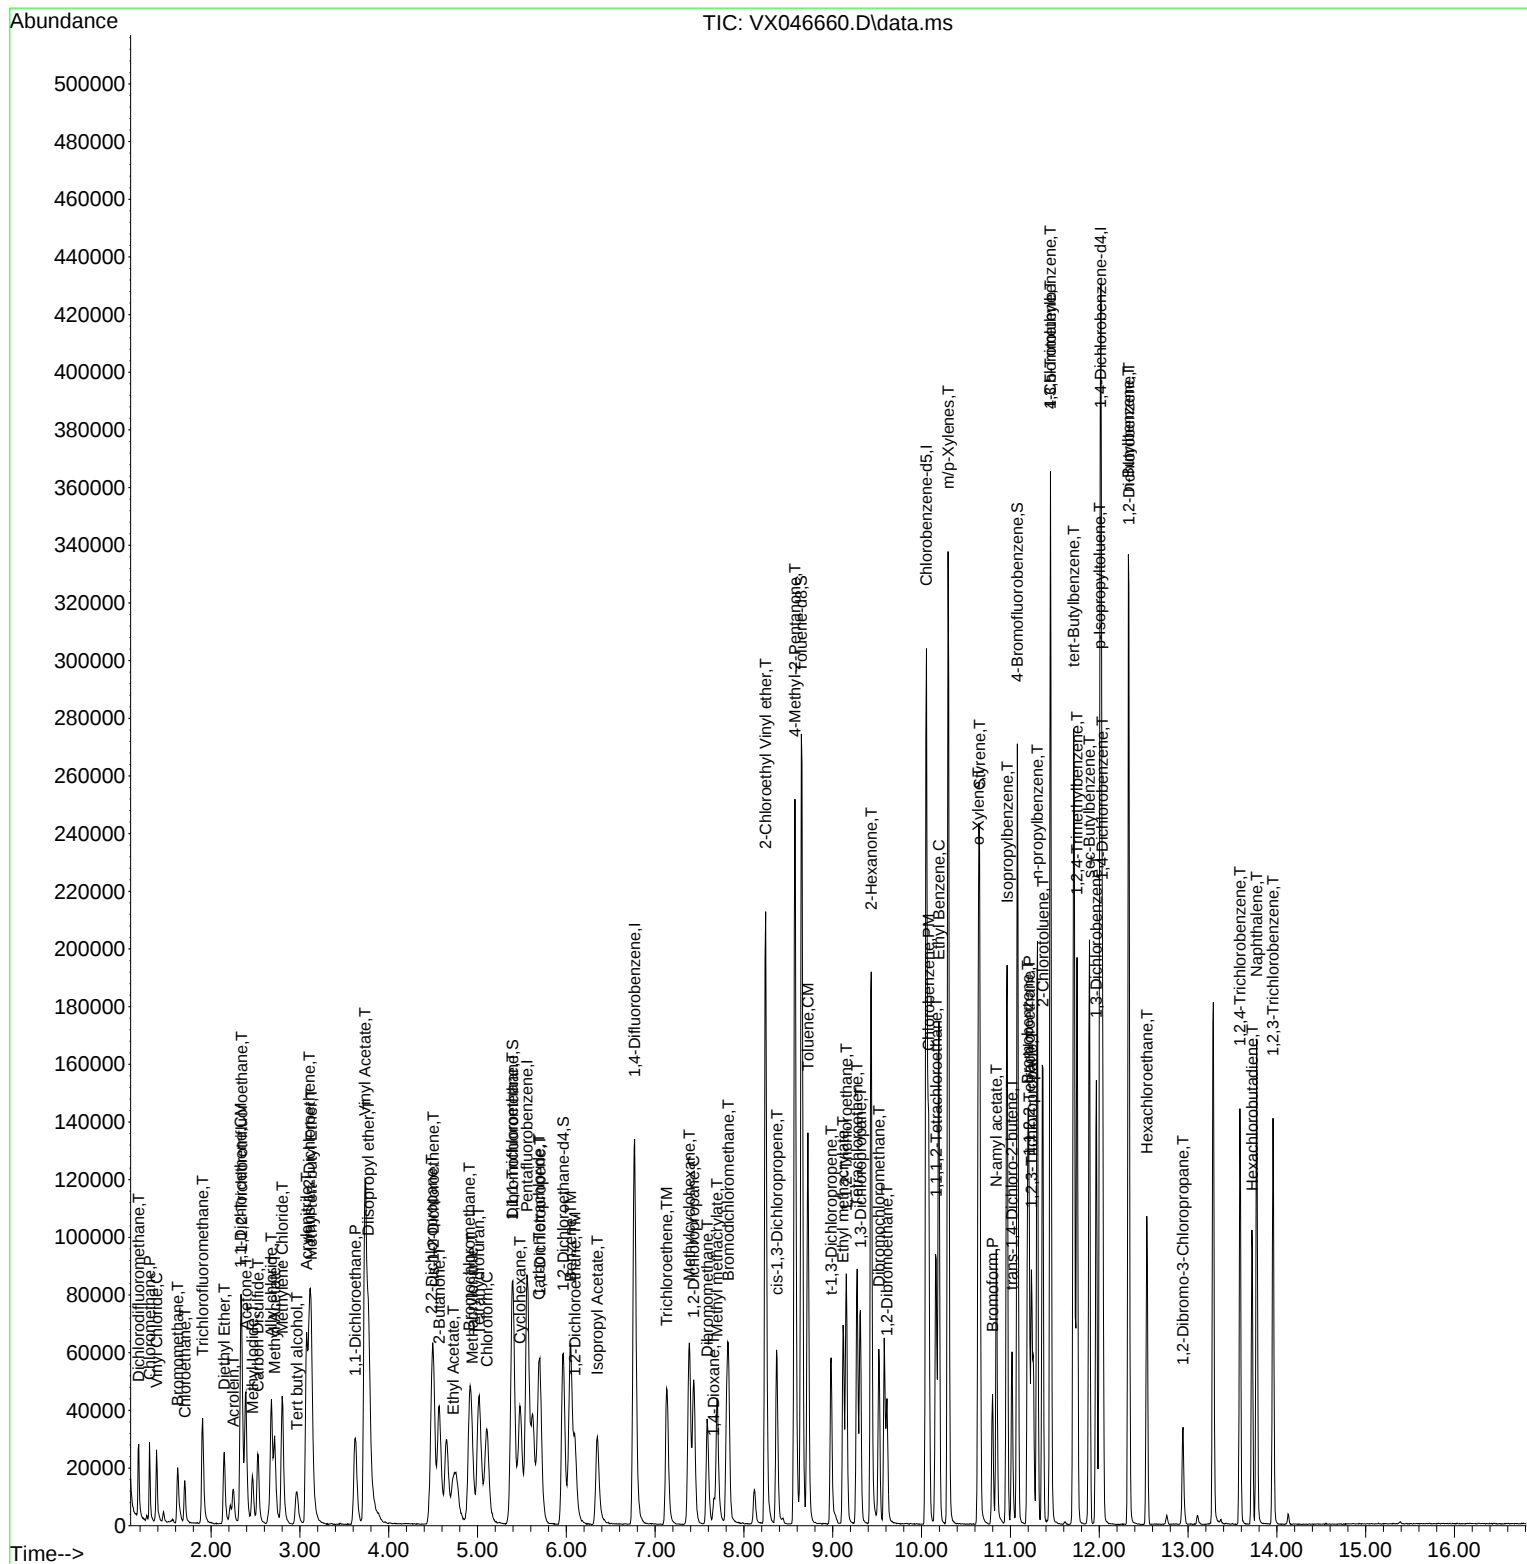

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046662.D
 Acq On : 12 Jun 2025 14:26
 Operator : JC/MD
 Sample : VX0612WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0612WBSD01

Manual Integrations APPROVED

Reviewed By : John Carlone 06/13/2025
 Supervised By : Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 01:43:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.568	168	77335	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.775	114	133427	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	124864	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	65393	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	61672	44.824	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	89.640%		
35) Dibromofluoromethane	5.409	113	48780	49.714	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.420%		
50) Toluene-d8	8.653	98	156263	48.305	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	96.600%		
62) 4-Bromofluorobenzene	11.079	95	67540	50.462	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	100.920%		
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.185	85	15159	14.119	ug/l	96
3) Chloromethane	1.307	50	14237	14.568	ug/l	97
4) Vinyl Chloride	1.386	62	14877	15.271	ug/l	96
5) Bromomethane	1.624	94	10127	17.124	ug/l	98
6) Chloroethane	1.709	64	10193	16.126	ug/l	96
7) Trichlorofluoromethane	1.904	101	25875	16.053	ug/l	97
8) Diethyl Ether	2.148	74	9926	17.429	ug/l	91
9) 1,1,2-Trichlorotrifluo...	2.349	101	17146	16.884	ug/l	94
10) Methyl Iodide	2.471	142	16573	15.055	ug/l	97
11) Tert butyl alcohol	2.971	59	15766	103.268	ug/l	99
12) 1,1-Dichloroethene	2.337	96	15836	17.248	ug/l	90
13) Acrolein	2.252	56	10925	82.071	ug/l	97
14) Allyl chloride	2.684	41	31675	17.566	ug/l	92
15) Acrylonitrile	3.081	53	62440	108.170	ug/l	99
16) Acetone	2.398	43	52285	99.588	ug/l	95
17) Carbon Disulfide	2.532	76	30557	15.813	ug/l	99
18) Methyl Acetate	2.721	43	37422	22.834	ug/l	98
19) Methyl tert-butyl Ether	3.129	73	65699	20.450	ug/l	99
20) Methylene Chloride	2.806	84	20169	18.272	ug/l	96
21) trans-1,2-Dichloroethene	3.111	96	16904	17.397	ug/l	96
22) Diisopropyl ether	3.782	45	69021	19.415	ug/l #	77
23) Vinyl Acetate	3.739	43	275263	100.288	ug/l	98
24) 1,1-Dichloroethane	3.629	63	36498	18.421	ug/l	98
25) 2-Butanone	4.574	43	81745	106.728	ug/l	96
26) 2,2-Dichloropropane	4.501	77	26479	18.002	ug/l	99
27) cis-1,2-Dichloroethene	4.513	96	22731	19.004	ug/l	94
28) Bromochloromethane	4.916	49	24813	26.256	ug/l	94
29) Tetrahydrofuran	5.025	42	51560	106.594	ug/l	97
30) Chloroform	5.117	83	40022	19.278	ug/l	98
31) Cyclohexane	5.489	56	26131	16.337	ug/l	98
32) 1,1,1-Trichloroethane	5.403	97	32623	18.370	ug/l	96
36) 1,1-Dichloropropene	5.708	75	23651	16.874	ug/l	97
37) Ethyl Acetate	4.739	43	31194m	22.803	ug/l	
38) Carbon Tetrachloride	5.696	117	27030	17.218	ug/l	95
39) Methylcyclohexane	7.391	83	27000	16.321	ug/l	96
40) Benzene	6.056	78	75001	19.008	ug/l	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046662.D
 Acq On : 12 Jun 2025 14:26
 Operator : JC/MD
 Sample : VX0612WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0612WBSD01

Manual Integrations
 APPROVED

Reviewed By :John Carlone 06/13/2025
 Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 01:43:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.946	41	17391	20.473	ug/l	92
42) 1,2-Dichloroethane	6.104	62	31275	19.052	ug/l	97
43) Isopropyl Acetate	6.354	43	48318	20.261	ug/l	98
44) Trichloroethene	7.135	130	18936	18.888	ug/l	99
45) 1,2-Dichloropropane	7.446	63	20974	20.594	ug/l	99
46) Dibromomethane	7.586	93	15538	20.280	ug/l	97
47) Bromodichloromethane	7.830	83	31910	20.255	ug/l	100
48) Methyl methacrylate	7.702	41	24860	20.261	ug/l	93
49) 1,4-Dioxane	7.671	88	7152	435.873	ug/l	99
51) 4-Methyl-2-Pentanone	8.580	43	169429	111.801	ug/l	98
52) Toluene	8.726	92	47973	19.790	ug/l	99
53) t-1,3-Dichloropropene	8.982	75	28068	19.871	ug/l	94
54) cis-1,3-Dichloropropene	8.372	75	31374	19.977	ug/l #	86
55) 1,1,2-Trichloroethane	9.159	97	21487	22.080	ug/l	97
56) Ethyl methacrylate	9.122	69	33081	22.090	ug/l	91
57) 1,3-Dichloropropane	9.311	76	34906	20.297	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.244	63	88144	108.060	ug/l	97
59) 2-Hexanone	9.433	43	122560	112.765	ug/l	95
60) Dibromochloromethane	9.525	129	24681	21.562	ug/l	97
61) 1,2-Dibromoethane	9.610	107	21425	21.128	ug/l	98
64) Tetrachloroethene	9.275	164	15466	18.523	ug/l	92
65) Chlorobenzene	10.079	112	55650	18.950	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.165	131	20124	20.279	ug/l	98
67) Ethyl Benzene	10.195	91	93152	18.170	ug/l	99
68) m/p-Xylenes	10.305	106	71271	38.324	ug/l	95
69) o-Xylene	10.640	106	34941	19.425	ug/l	97
70) Styrene	10.659	104	62281	20.227	ug/l	96
71) Bromoform	10.799	173	16530	21.846	ug/l #	100
73) Isopropylbenzene	10.963	105	94452	18.374	ug/l	99
74) N-amyl acetate	10.841	43	43589	19.255	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.213	83	34369	20.888	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	27152m	19.603	ug/l	
77) Bromobenzene	11.201	156	23326	19.550	ug/l	93
78) n-propylbenzene	11.305	91	111370	17.900	ug/l	98
79) 2-Chlorotoluene	11.366	91	67642	18.028	ug/l	97
80) 1,3,5-Trimethylbenzene	11.451	105	79297	18.512	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.018	75	9232	19.227	ug/l	93
82) 4-Chlorotoluene	11.457	91	80597	18.123	ug/l	95
83) tert-Butylbenzene	11.713	119	83097	19.056	ug/l	94
84) 1,2,4-Trimethylbenzene	11.750	105	80595	18.598	ug/l	99
85) sec-Butylbenzene	11.890	105	102518	18.297	ug/l	100
86) p-Isopropyltoluene	12.012	119	86541	18.527	ug/l	98
87) 1,3-Dichlorobenzene	11.969	146	44009	18.994	ug/l	98
88) 1,4-Dichlorobenzene	12.042	146	44978	18.734	ug/l	98
89) n-Butylbenzene	12.329	91	81561	17.780	ug/l	99
90) Hexachloroethane	12.536	117	14475	17.435	ug/l	93
91) 1,2-Dichlorobenzene	12.335	146	44738	20.004	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	7269	19.728	ug/l	82
93) 1,2,4-Trichlorobenzene	13.585	180	28666	18.789	ug/l	98
94) Hexachlorobutadiene	13.725	225	12471	17.589	ug/l	99
95) Naphthalene	13.774	128	100632	20.800	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	29289	19.145	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
Data File : VX046662.D
Acq On : 12 Jun 2025 14:26
Operator : JC/MD
Sample : VX0612WBSD01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Jun 13 01:43:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 06 16:56:12 2025
Response via : Initial Calibration

Instrument :
MSVOA_X
ClientSampleId :
VX0612WBSD01

Manual Integrations
APPROVED

Reviewed By :John Carlone 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061225\
 Data File : VX046662.D
 Acq On : 12 Jun 2025 14:26
 Operator : JC/MD
 Sample : VX0612WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0612WBSD01

Manual Integrations
 APPROVED

Reviewed By : John Carlone 06/13/2025
 Supervised By : Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 01:43:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060625W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 06 16:56:12 2025
 Response via : Initial Calibration

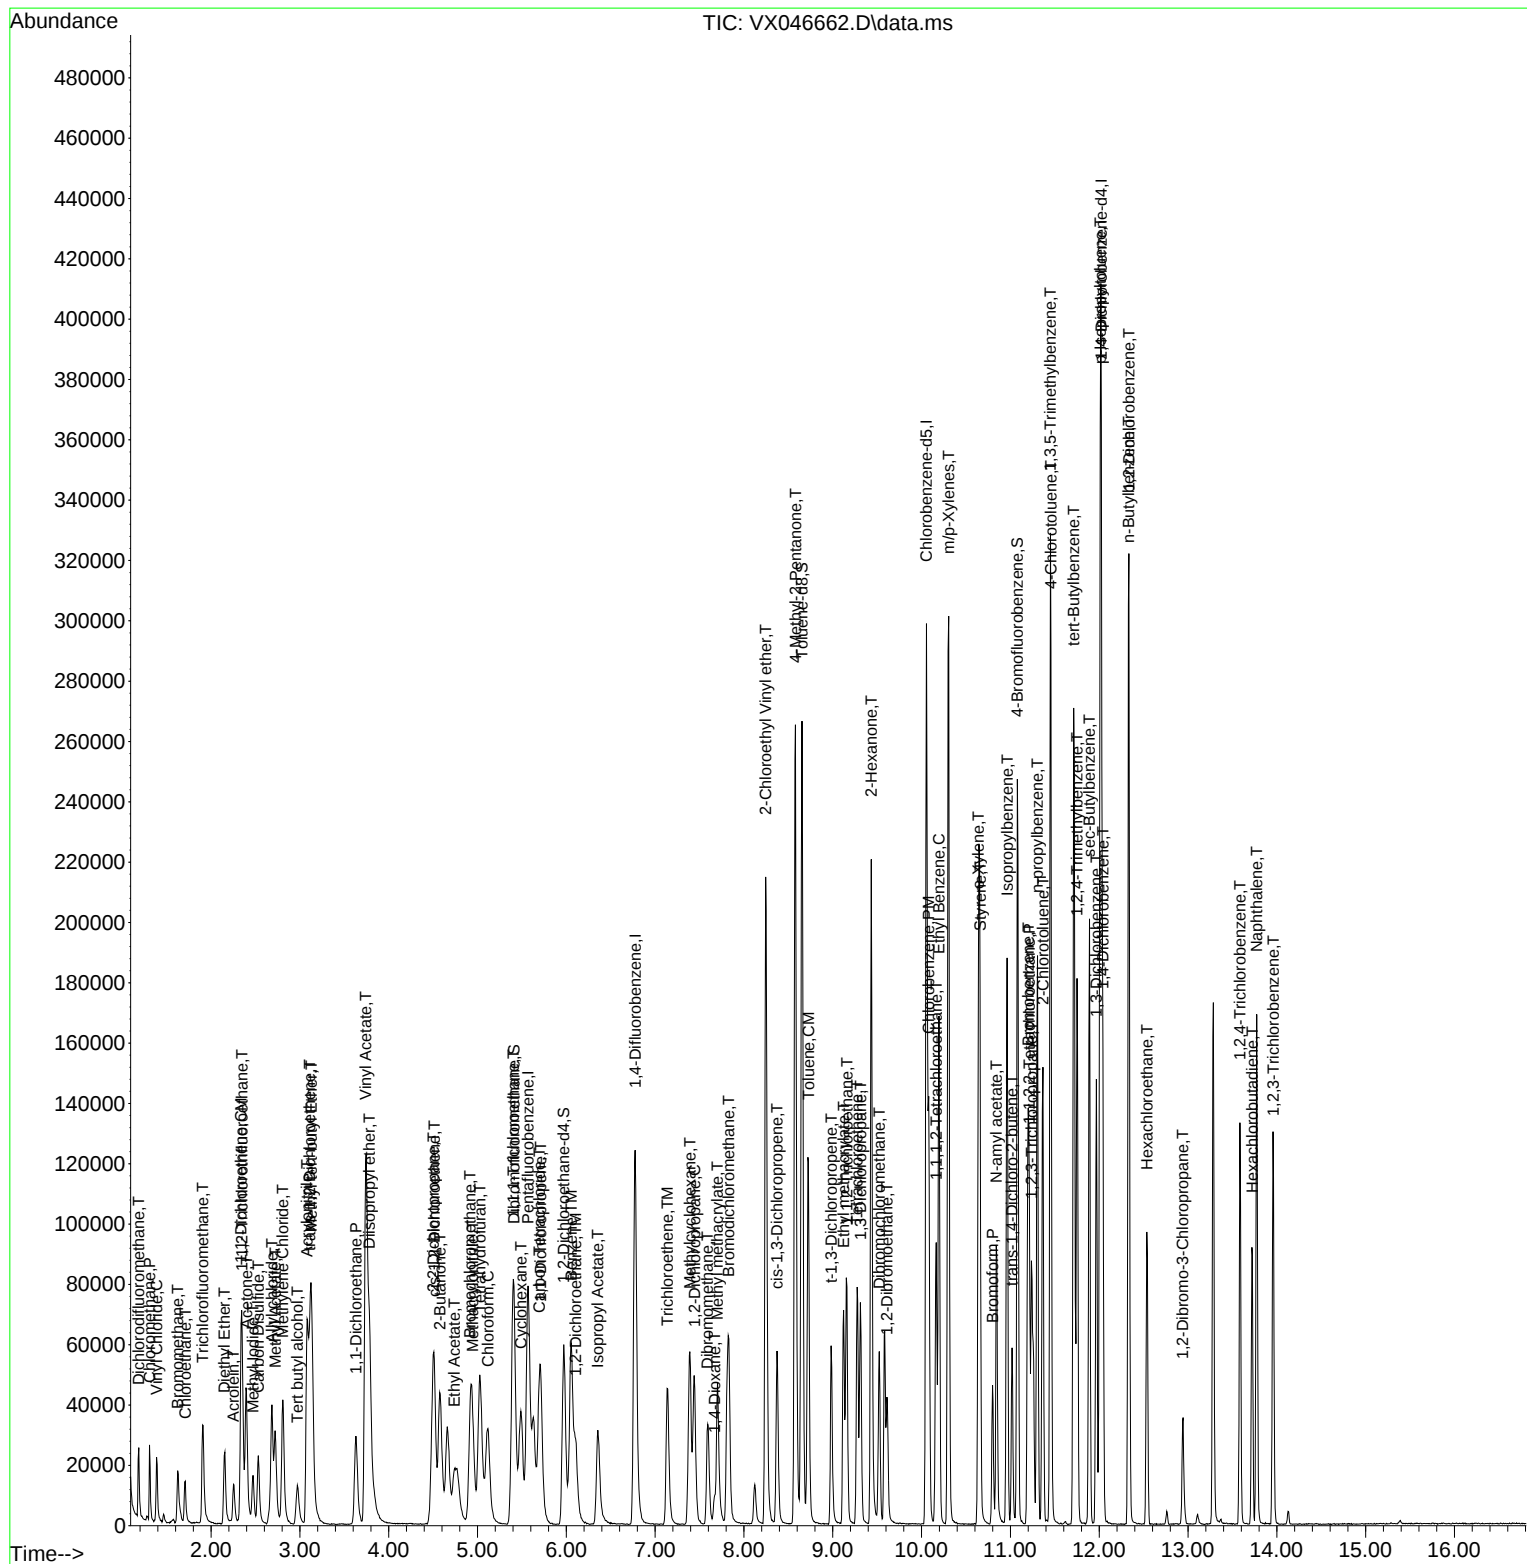

Manual Integration Report

Sequence:	VX060625	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDIC005	VX046518.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:36 PM	MMDadoda	6/9/2025 1:14:56 PM	Peak Integrated by Software
VSTDIC020	VX046519.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:40 PM	MMDadoda	6/9/2025 1:14:59 PM	Peak Integrated by Software
VSTDIC050	VX046520.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:44 PM	MMDadoda	6/9/2025 1:15:03 PM	Peak Integrated by Software
VSTDIC100	VX046521.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:48 PM	MMDadoda	6/9/2025 1:15:08 PM	Peak Integrated by Software
VSTDIC150	VX046522.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:25:52 PM	MMDadoda	6/9/2025 1:15:37 PM	Peak Integrated by Software
VSTDIC001	VX046524.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:08:38 AM	MMDadoda	6/9/2025 1:15:41 PM	Peak Integrated by Software
VSTDIC001	VX046524.D	1,4-Dichlorobenzene	JOHN	6/9/2025 8:08:38 AM	MMDadoda	6/9/2025 1:15:41 PM	Peak Integrated by Software
VSTDIC001	VX046524.D	Ethyl Acetate	JOHN	6/9/2025 8:08:38 AM	MMDadoda	6/9/2025 1:15:41 PM	Peak Integrated by Software
VSTDICV050	VX046525.D	1,2,3-Trichloropropane	JOHN	6/6/2025 5:26:01 PM	MMDadoda	6/9/2025 1:16:01 PM	Peak Integrated by Software
VSTDIC050	VX046544.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:10:18 AM	MMDadoda	6/9/2025 1:16:52 PM	Peak Integrated by Software
VSTDIC050	VX046546.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:10:22 AM	MMDadoda	6/9/2025 1:16:54 PM	Peak Integrated by Software
VSTDIC050	VX046565.D	1,2,3-Trichloropropane	JOHN	6/9/2025 8:12:06 AM	Sam	6/9/2025 1:18:52 PM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VX060625	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
-----------	---------	-----------	-----------	-----------	---------------	---------------	--------

A

C

D

E

F

G

H

I

J

Manual Integration Report

Sequence:

vx061225

Instrument

MSVOA_x

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VX046657.D	1,2,3-Trichloropropane	JOHN	6/13/2025 10:02:14 AM	MMDadoda	6/13/2025 10:58:05 AM	Peak Integrated by Software
VX0612WBS01	VX046660.D	1,2,3-Trichloropropane	JOHN	6/13/2025 10:02:18 AM	MMDadoda	6/13/2025 10:58:06 AM	Peak Integrated by Software
VX0612WBSD0 1	VX046662.D	1,2,3-Trichloropropane	JOHN	6/13/2025 10:02:22 AM	MMDadoda	6/13/2025 10:58:07 AM	Peak Integrated by Software
VX0612WBSD0 1	VX046662.D	Ethyl Acetate	JOHN	6/13/2025 10:02:22 AM	MMDadoda	6/13/2025 10:58:07 AM	Peak Integrated by Software
VSTDCCC050	VX046673.D	1,2,3-Trichloropropane	JOHN	6/13/2025 10:02:43 AM	MMDadoda	6/13/2025 10:58:16 AM	Peak Integrated by Software

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QCBatch ID # VX060625

Review By	Mahesh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX046516.D	06 Jun 2025 08:47	JC/MD	Ok
2	VSTDICC001	VX046517.D	06 Jun 2025 09:13	JC/MD	Not Ok
3	VSTDICC005	VX046518.D	06 Jun 2025 09:42	JC/MD	Ok,M
4	VSTDICC020	VX046519.D	06 Jun 2025 10:18	JC/MD	Ok,M
5	VSTDICCC050	VX046520.D	06 Jun 2025 10:40	JC/MD	Ok,M
6	VSTDICC100	VX046521.D	06 Jun 2025 11:02	JC/MD	Ok,M
7	VSTDICC150	VX046522.D	06 Jun 2025 11:25	JC/MD	Ok,M
8	IBLK	VX046523.D	06 Jun 2025 11:47	JC/MD	Ok
9	VSTDICC001	VX046524.D	06 Jun 2025 12:57	JC/MD	Ok,M
10	VSTDICV050	VX046525.D	06 Jun 2025 14:11	JC/MD	Ok,M
11	VX0606MBL01	VX046526.D	06 Jun 2025 14:39	JC/MD	Ok
12	VX0606WBL01	VX046527.D	06 Jun 2025 15:02	JC/MD	Ok
13	VX0606WBS01	VX046528.D	06 Jun 2025 15:25	JC/MD	Ok,M
14	VX0606MBS01	VX046529.D	06 Jun 2025 15:51	JC/MD	Ok,M
15	Q2168-11MEDL	VX046530.D	06 Jun 2025 16:13	JC/MD	Ok
16	VX0606WBSD01	VX046531.D	06 Jun 2025 16:36	JC/MD	Ok,M
17	Q2194-02	VX046532.D	06 Jun 2025 16:58	JC/MD	Ok
18	Q2194-04	VX046533.D	06 Jun 2025 17:21	JC/MD	Ok
19	Q2207-09	VX046534.D	06 Jun 2025 17:43	JC/MD	Ok,M
20	Q2207-18	VX046535.D	06 Jun 2025 18:06	JC/MD	Ok,M
21	Q2207-27	VX046536.D	06 Jun 2025 18:28	JC/MD	Ok,M

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Maresh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	Q2207-36	VX046537.D	06 Jun 2025 18:51	JC/MD	Ok,M
23	Q2207-45	VX046538.D	06 Jun 2025 19:13	JC/MD	Ok,M
24	Q2208-09	VX046539.D	06 Jun 2025 19:35	JC/MD	Ok,M
25	Q2208-18	VX046540.D	06 Jun 2025 19:58	JC/MD	Ok,M
26	Q2208-27	VX046541.D	06 Jun 2025 20:20	JC/MD	Ok,M
27	Q2208-36	VX046542.D	06 Jun 2025 20:42	JC/MD	Ok,M
28	Q2236-01	VX046543.D	06 Jun 2025 21:04	JC/MD	Not Ok
29	VSTDCCC050	VX046544.D	06 Jun 2025 21:26	JC/MD	Not Ok
30	BFB	VX046545.D	06 Jun 2025 23:59	JC/MD	Ok
31	VSTDCCC050	VX046546.D	07 Jun 2025 00:34	JC/MD	Ok,M
32	VX0606WBL02	VX046547.D	07 Jun 2025 01:17	JC/MD	Ok
33	VX0606WBS02	VX046548.D	07 Jun 2025 02:00	JC/MD	Ok,M
34	VX0606WBSD02	VX046549.D	07 Jun 2025 02:22	JC/MD	Ok,M
35	PB168312TB	VX046550.D	07 Jun 2025 02:43	JC/MD	Ok,M
36	PB168272TB	VX046551.D	07 Jun 2025 03:05	JC/MD	Ok,M
37	Q2236-05	VX046552.D	07 Jun 2025 03:26	JC/MD	ReRun
38	Q2236-09	VX046553.D	07 Jun 2025 03:48	JC/MD	ReRun
39	Q2236-13	VX046554.D	07 Jun 2025 04:09	JC/MD	Ok
40	Q2236-17	VX046555.D	07 Jun 2025 04:31	JC/MD	ReRun
41	Q2227-04	VX046556.D	07 Jun 2025 04:52	JC/MD	Ok,M
42	Q2228-04	VX046557.D	07 Jun 2025 05:14	JC/MD	ReRun
43	Q2235-01	VX046558.D	07 Jun 2025 05:36	JC/MD	ReRun
44	Q2240-04	VX046559.D	07 Jun 2025 05:57	JC/MD	ReRun

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QCBatch ID # VX060625

Review By	Maresh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	Q2240-08	VX046560.D	07 Jun 2025 06:18	JC/MD	ReRun
46	Q2240-12	VX046561.D	07 Jun 2025 06:40	JC/MD	ReRun
47	Q2241-04	VX046562.D	07 Jun 2025 07:01	JC/MD	ReRun
48	Q2241-08	VX046563.D	07 Jun 2025 07:23	JC/MD	ReRun
49	Q2226-04	VX046564.D	07 Jun 2025 07:44	JC/MD	ReRun
50	VSTDCCC050	VX046565.D	07 Jun 2025 08:06	JC/MD	Ok,M

M : Manual Integration

Instrument ID: **MSVOA_X**

Daily Analysis Runlog For Sequence/QC Batch ID # VX061225

Review By	John Carlone	Review On	6/13/2025 10:05:11 AM
Supervise By	Maresh Dadoda	Supervise On	6/13/2025 10:58:22 AM
SubDirectory	VX061225	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134305		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134306,VP134307		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX046656.D	12 Jun 2025 09:44	JC/MD	Ok
2	VSTDCCC050	VX046657.D	12 Jun 2025 10:11	JC/MD	Ok,M
3	VX0612MBL01	VX046658.D	12 Jun 2025 12:48	JC/MD	Ok
4	VX0612WBL01	VX046659.D	12 Jun 2025 13:10	JC/MD	Ok
5	VX0612WBS01	VX046660.D	12 Jun 2025 13:38	JC/MD	Ok,M
6	Q2249-01RE	VX046661.D	12 Jun 2025 14:04	JC/MD	Confirms
7	VX0612WBSD01	VX046662.D	12 Jun 2025 14:26	JC/MD	Ok,M
8	Q2249-01	VX046663.D	12 Jun 2025 14:53	JC/MD	Not Ok
9	Q2249-01	VX046664.D	12 Jun 2025 15:24	JC/MD	Not Ok
10	Q2275-01	VX046665.D	12 Jun 2025 15:46	JC/MD	Ok
11	Q2275-05	VX046666.D	12 Jun 2025 16:10	JC/MD	ReRun
12	Q2275-03	VX046667.D	12 Jun 2025 16:32	JC/MD	Ok
13	Q2275-05	VX046668.D	12 Jun 2025 16:55	JC/MD	Ok
14	Q2267-01	VX046669.D	12 Jun 2025 17:17	JC/MD	Ok,M
15	Q2278-04	VX046670.D	12 Jun 2025 17:40	JC/MD	Ok,M
16	Q2285-05	VX046671.D	12 Jun 2025 18:02	JC/MD	Ok,M
17	PB168448TB	VX046672.D	12 Jun 2025 18:24	JC/MD	Ok,M
18	VSTDCCC050	VX046673.D	12 Jun 2025 18:47	JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Mahesh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	Sampleld	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX046516.D	06 Jun 2025 08:47		JC/MD	Ok
2	VSTDIC001	VSTDIC001	VX046517.D	06 Jun 2025 09:13		JC/MD	Not Ok
3	VSTDIC005	VSTDIC005	VX046518.D	06 Jun 2025 09:42	for TCLP	JC/MD	Ok,M
4	VSTDIC020	VSTDIC020	VX046519.D	06 Jun 2025 10:18	Comp #05 fail	JC/MD	Ok,M
5	VSTDIC050	VSTDIC050	VX046520.D	06 Jun 2025 10:40	LR-13,16,17	JC/MD	Ok,M
6	VSTDIC100	VSTDIC100	VX046521.D	06 Jun 2025 11:02		JC/MD	Ok,M
7	VSTDIC150	VSTDIC150	VX046522.D	06 Jun 2025 11:25		JC/MD	Ok,M
8	IBLK	IBLK	VX046523.D	06 Jun 2025 11:47		JC/MD	Ok
9	VSTDIC001	VSTDIC001	VX046524.D	06 Jun 2025 12:57		JC/MD	Ok,M
10	VSTDICV050	ICV VX060625	VX046525.D	06 Jun 2025 14:11		JC/MD	Ok,M
11	VX0606MBL01	VX0606MBL01	VX046526.D	06 Jun 2025 14:39		JC/MD	Ok
12	VX0606WBL01	VX0606WBL01	VX046527.D	06 Jun 2025 15:02		JC/MD	Ok
13	VX0606WBS01	VX0606WBS01	VX046528.D	06 Jun 2025 15:25		JC/MD	Ok,M
14	VX0606MBS01	VX0606MBS01	VX046529.D	06 Jun 2025 15:51		JC/MD	Ok,M
15	Q2168-11MEDL	C2MEDL	VX046530.D	06 Jun 2025 16:13		JC/MD	Ok
16	VX0606WBSD01	VX0606WBSD01	VX046531.D	06 Jun 2025 16:36		JC/MD	Ok,M
17	Q2194-02	COMP-12	VX046532.D	06 Jun 2025 16:58	vial A pH#5.0	JC/MD	Ok
18	Q2194-04	COMP-13	VX046533.D	06 Jun 2025 17:21	vial A pH#5.0	JC/MD	Ok

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Maresh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	Q2207-09	BU-703-COMP-01	VX046534.D	06 Jun 2025 17:43	vial A pH#5.0	JC/MD	Ok,M
20	Q2207-18	BU-703-COMP-02	VX046535.D	06 Jun 2025 18:06	vial A pH#5.0	JC/MD	Ok,M
21	Q2207-27	BU-703-COMP-03	VX046536.D	06 Jun 2025 18:28	vial A pH#5.0	JC/MD	Ok,M
22	Q2207-36	BU-703-COMP-04	VX046537.D	06 Jun 2025 18:51	vial A pH#5.0	JC/MD	Ok,M
23	Q2207-45	BU-703-COMP-05	VX046538.D	06 Jun 2025 19:13	vial A pH#5.0	JC/MD	Ok,M
24	Q2208-09	BU-703-COMP-06	VX046539.D	06 Jun 2025 19:35	vial A pH#5.0	JC/MD	Ok,M
25	Q2208-18	BU-703-COMP-07	VX046540.D	06 Jun 2025 19:58	vial A pH#5.0	JC/MD	Ok,M
26	Q2208-27	BU-703-COMP-08	VX046541.D	06 Jun 2025 20:20	vial A pH#5.0	JC/MD	Ok,M
27	Q2208-36	BU-703-COMP-09	VX046542.D	06 Jun 2025 20:42	vial A pH#5.0	JC/MD	Ok,M
28	Q2236-01	WC-A4-05A-G	VX046543.D	06 Jun 2025 21:04	vial A pH#5.0 Out of tune	JC/MD	Not Ok
29	VSTDCCC050	VSTDCCC050EC	VX046544.D	06 Jun 2025 21:26	Out of tune	JC/MD	Not Ok
30	BFB	BFB	VX046545.D	06 Jun 2025 23:59		JC/MD	Ok
31	VSTDCCC050	VSTDCCC050	VX046546.D	07 Jun 2025 00:34		JC/MD	Ok,M
32	VX0606WBL02	VX0606WBL02	VX046547.D	07 Jun 2025 01:17		JC/MD	Ok
33	VX0606WBS02	VX0606WBS02	VX046548.D	07 Jun 2025 02:00		JC/MD	Ok,M
34	VX0606WBSD02	VX0606WBSD02	VX046549.D	07 Jun 2025 02:22		JC/MD	Ok,M
35	PB168312TB	PB168312TB	VX046550.D	07 Jun 2025 02:43		JC/MD	Ok,M
36	PB168272TB	PB168272TB	VX046551.D	07 Jun 2025 03:05		JC/MD	Ok,M
37	Q2236-05	WC-A2-04-G	VX046552.D	07 Jun 2025 03:26	Surrogate Fail	JC/MD	ReRun

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX060625

Review By	Maresh Dadoda	Review On	6/9/2025 1:15:21 PM
Supervise By	Semsettin Yesilyurt	Supervise On	6/9/2025 1:19:58 PM
SubDirectory	VX060625	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP134153		
Initial Calibration Stds	VP134235,VP134236,VP134237,VP134238,VP134239,VP134240		
CCC	VP134154		
Internal Standard/PEM			
ICV/I.BLK	VP134241		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	Q2236-09	WC-A2-05-G	VX046553.D	07 Jun 2025 03:48	Internal Standard Fail	JC/MD	ReRun
39	Q2236-13	WC-A2-06-G	VX046554.D	07 Jun 2025 04:09	vial A pH#5.0	JC/MD	Ok
40	Q2236-17	WC-A2-07-G	VX046555.D	07 Jun 2025 04:31	Internal Standard Fail; Surrogate fail	JC/MD	ReRun
41	Q2227-04	TP07-MHH-WC	VX046556.D	07 Jun 2025 04:52		JC/MD	Ok,M
42	Q2228-04	TP08-MHI-WC	VX046557.D	07 Jun 2025 05:14	Internal Standard Fail	JC/MD	ReRun
43	Q2235-01	WC-A2-08-G	VX046558.D	07 Jun 2025 05:36	Internal Standard Fail	JC/MD	ReRun
44	Q2240-04	TP-3	VX046559.D	07 Jun 2025 05:57	Internal Standard Fail	JC/MD	ReRun
45	Q2240-08	TP-2	VX046560.D	07 Jun 2025 06:18	Internal Standard Fail	JC/MD	ReRun
46	Q2240-12	TP-1	VX046561.D	07 Jun 2025 06:40	Internal Standard Fail	JC/MD	ReRun
47	Q2241-04	TP-N	VX046562.D	07 Jun 2025 07:01	Internal Standard Fail	JC/MD	ReRun
48	Q2241-08	TP-S	VX046563.D	07 Jun 2025 07:23	Internal Standard Fail	JC/MD	ReRun
49	Q2226-04	TP06-MHI-WC	VX046564.D	07 Jun 2025 07:44	Internal Standard Fail	JC/MD	ReRun
50	VSTDCCC050	VSTDCCC050EC	VX046565.D	07 Jun 2025 08:06		JC/MD	Ok,M

M : Manual Integration

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX061225

Review By	John Carlone	Review On	6/13/2025 10:05:11 AM
Supervise By	Maresh Dadoda	Supervise On	6/13/2025 10:58:22 AM
SubDirectory	VX061225	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134305		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134306,VP134307		

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX046656.D	12 Jun 2025 09:44		JC/MD	Ok
2	VSTDCCC050	VSTDCCC050	VX046657.D	12 Jun 2025 10:11		JC/MD	Ok,M
3	VX0612MBL01	VX0612MBL01	VX046658.D	12 Jun 2025 12:48		JC/MD	Ok
4	VX0612WBL01	VX0612WBL01	VX046659.D	12 Jun 2025 13:10		JC/MD	Ok
5	VX0612WBS01	VX0612WBS01	VX046660.D	12 Jun 2025 13:38		JC/MD	Ok,M
6	Q2249-01RE	MW-06-6.5-060525RE	VX046661.D	12 Jun 2025 14:04	vial B pH<2 ISTD Fail	JC/MD	Confirms
7	VX0612WBSD01	VX0612WBSD01	VX046662.D	12 Jun 2025 14:26		JC/MD	Ok,M
8	Q2249-01	MW-06-6.5-060525	VX046663.D	12 Jun 2025 14:53	Not req	JC/MD	Not Ok
9	Q2249-01	MW-06-6.5-060525	VX046664.D	12 Jun 2025 15:24	Not req	JC/MD	Not Ok
10	Q2275-01	OW-08B-72.5-060925	VX046665.D	12 Jun 2025 15:46	vial A pH<2	JC/MD	Ok
11	Q2275-05	TB01-060925	VX046666.D	12 Jun 2025 16:10	vial A pH<2 TB; Surrogate Fail	JC/MD	ReRun
12	Q2275-03	EB01-060925	VX046667.D	12 Jun 2025 16:32	vial A pH<2 EB	JC/MD	Ok
13	Q2275-05	TB01-060925	VX046668.D	12 Jun 2025 16:55	vial B pH<2 TB	JC/MD	Ok
14	Q2267-01	WC-20250605	VX046669.D	12 Jun 2025 17:17	vial A pH#5.0	JC/MD	Ok,M
15	Q2278-04	TP-2	VX046670.D	12 Jun 2025 17:40	vial B pH#5.0	JC/MD	Ok,M
16	Q2285-05	HAM-CONCRETE	VX046671.D	12 Jun 2025 18:02	vial B pH#5.0	JC/MD	Ok,M
17	PB168448TB	PB168448TB	VX046672.D	12 Jun 2025 18:24		JC/MD	Ok,M
18	VSTDCCC050	VSTDCCC050EC	VX046673.D	12 Jun 2025 18:47		JC/MD	Ok,M

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QC Batch ID # VX061225

Review By	John Carlone	Review On	6/13/2025 10:05:11 AM
Supervise By	Mahesh Dadoda	Supervise On	6/13/2025 10:58:22 AM
SubDirectory	VX061225	HP Acquire Method	HP Processing Method 82X060625W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP134305		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP134306,VP134307		

M : Manual Integration

A
B
C
D
E
F
G
H
I
J

LAB CHRONICLE

OrderID:	Q2275	OrderDate:	6/10/2025 11:03:00 AM
Client:	JACOBS Engineering Group, Inc.	Project:	Former Schlumberger STC PTC Site D3868221
Contact:	John Ynfante	Location:	D31,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2275-01	OW-08B-72.5-060925	Water	VOCMS Group3	8260-Low	06/08/25		06/12/25	06/10/25
Q2275-03	EB01-060925	Water	VOCMS Group3	8260-Low	06/08/25		06/12/25	06/10/25
Q2275-05	TB01-060925	Water	VOCMS Group3	8260-Low	06/08/25		06/12/25	06/10/25