
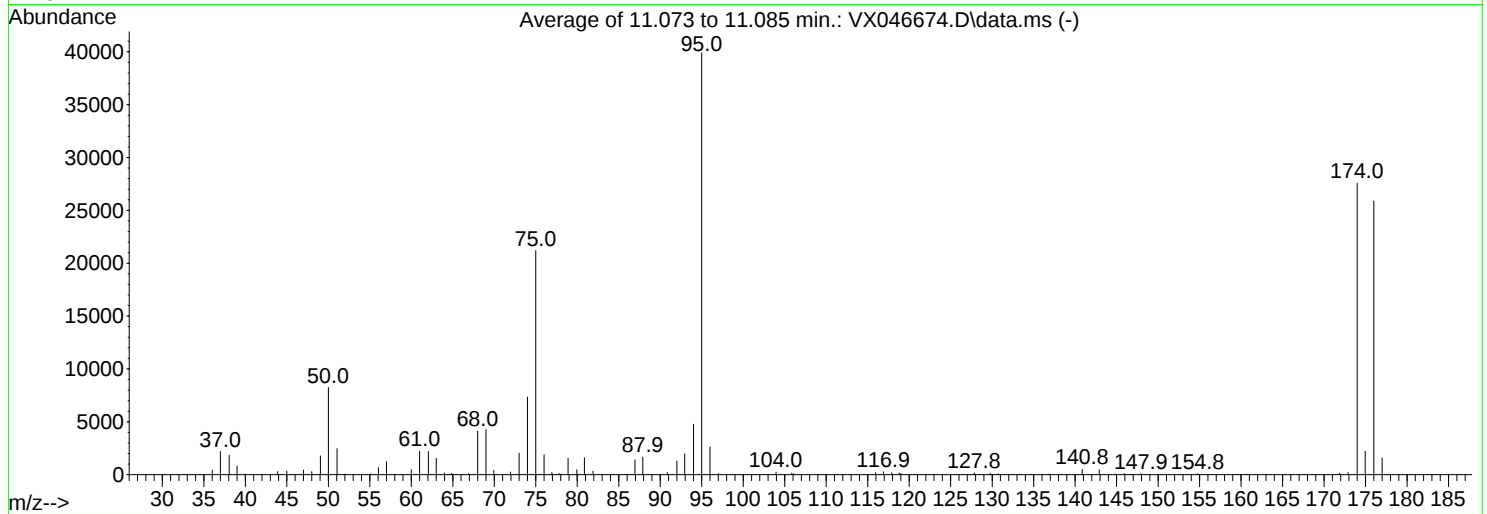


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061325\
Data File : VX046674.D
Acq On : 13 Jun 2025 08:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X061025W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Jun 11 06:20:28 2025

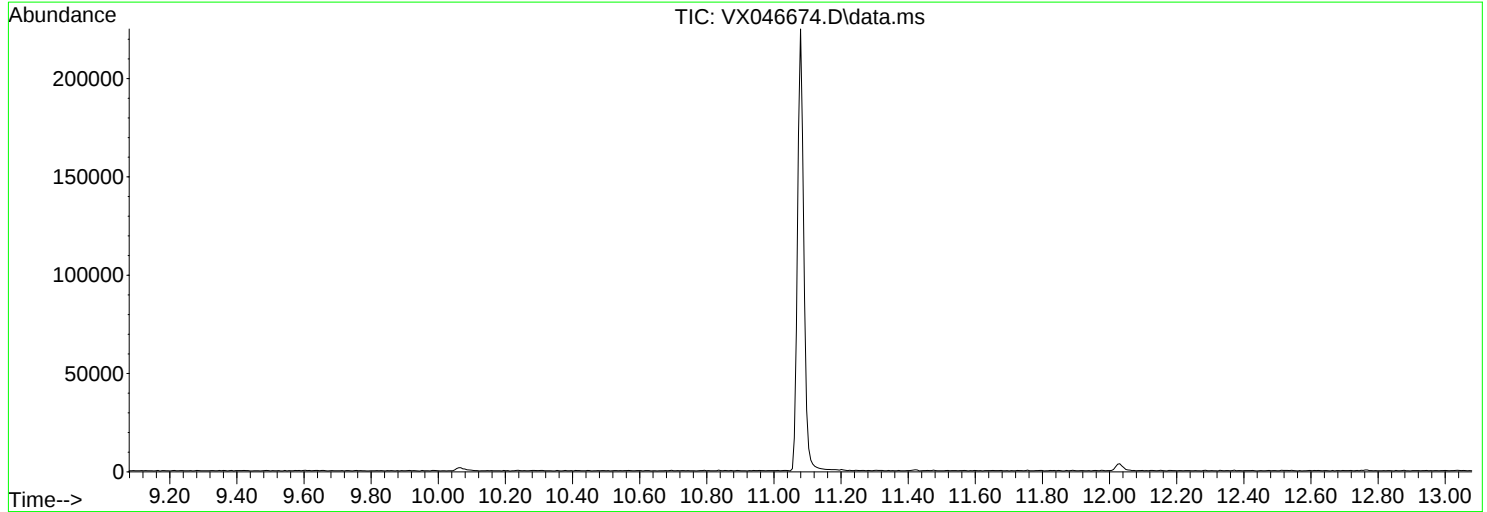

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	8238	PASS
75	95	30	60	53.1	21195	PASS
95	95	100	100	100.0	39904	PASS
96	95	5	9	6.6	2631	PASS
173	174	0.00	2	0.7	200	PASS
174	95	50	100	69.1	27584	PASS
175	174	5	9	8.0	2209	PASS
176	174	95	101	93.8	25883	FAIL*
177	176	5	9	6.1	1580	PASS