


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037272.D
Acq On : 14 Jun 2025 21:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 19 02:50:12 2025

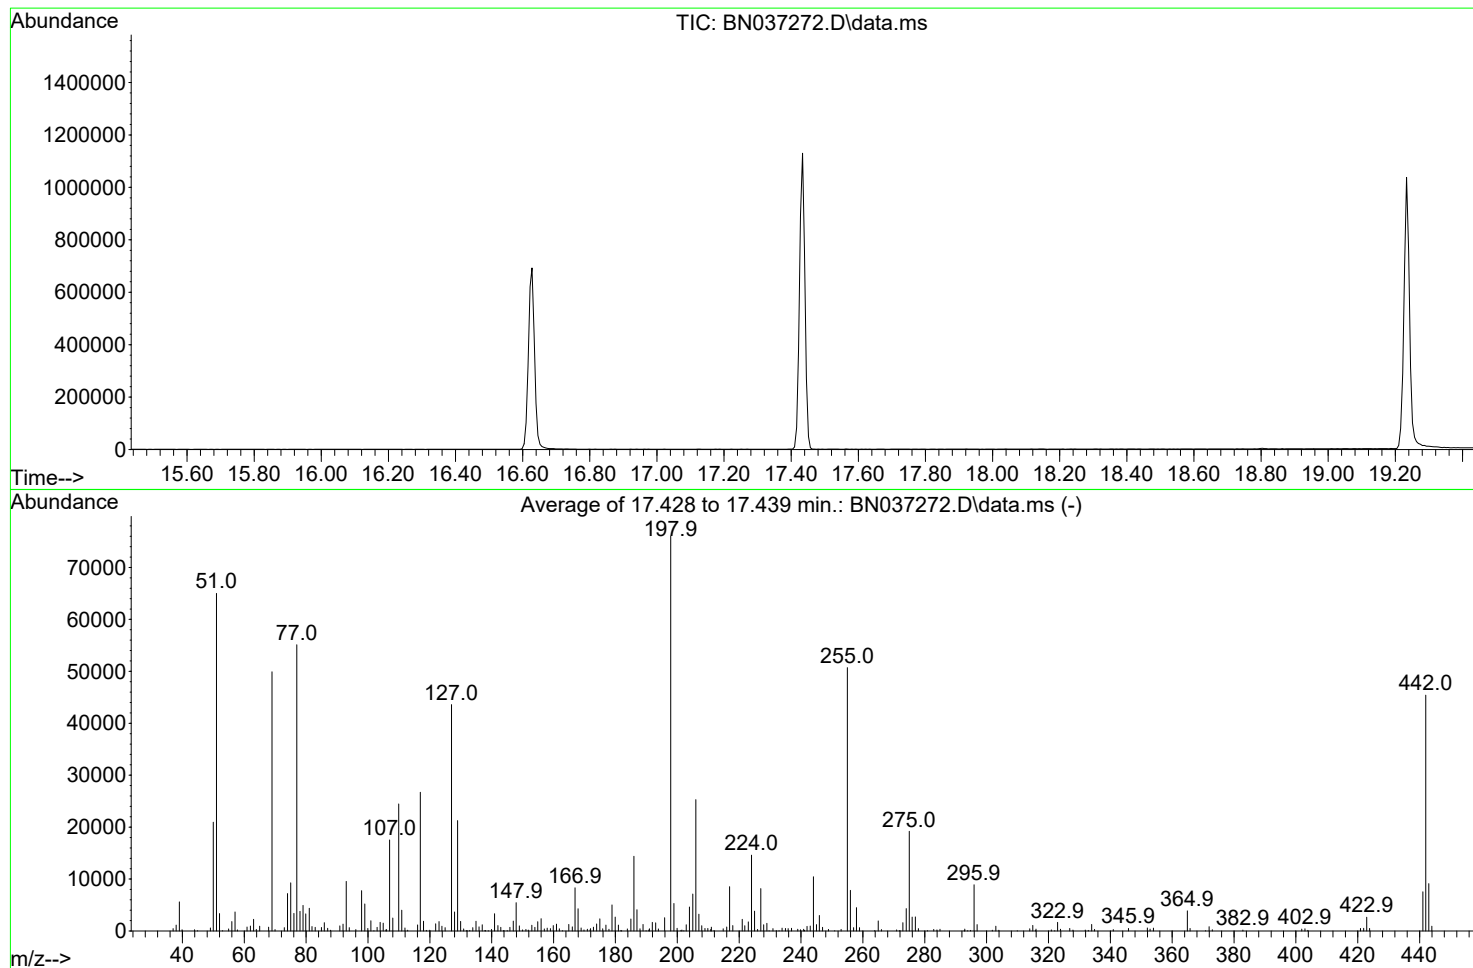

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	741	PASS
69	69	100	100	100.0	49899	PASS
70	69	0.00	2	0.6	291	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76024	PASS
199	198	5	9	7.0	5292	PASS
365	198	1	100	5.1	3876	PASS
441	443	0.01	150	82.8	7543	PASS
442	442	100	100	100.0	45411	PASS
443	442	15	24	20.1	9108	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/13/2025	BNA_N	<u>BN037258.D</u>
Compound Name	Response	Retention Time
DDT	228732	20.475
DDD	3511	20.033
DDE	0	0
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3511	232243	1.51

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037272.D
Acq On : 14 Jun 2025 21:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 03:00:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

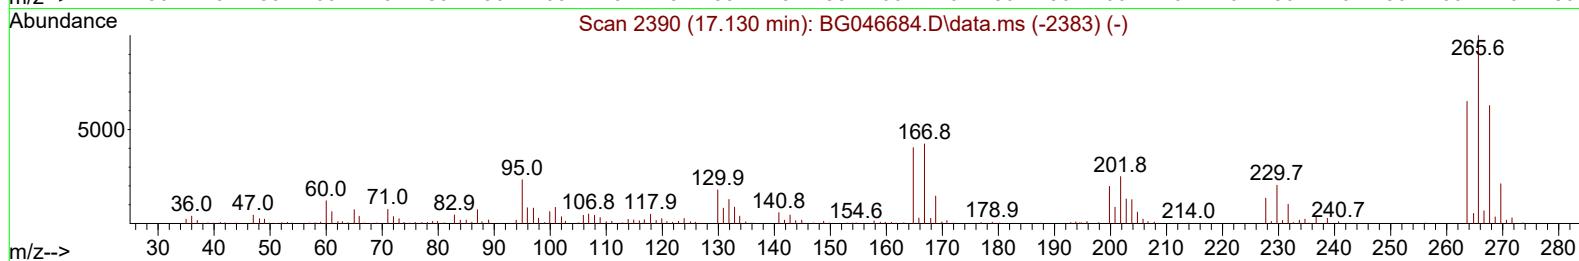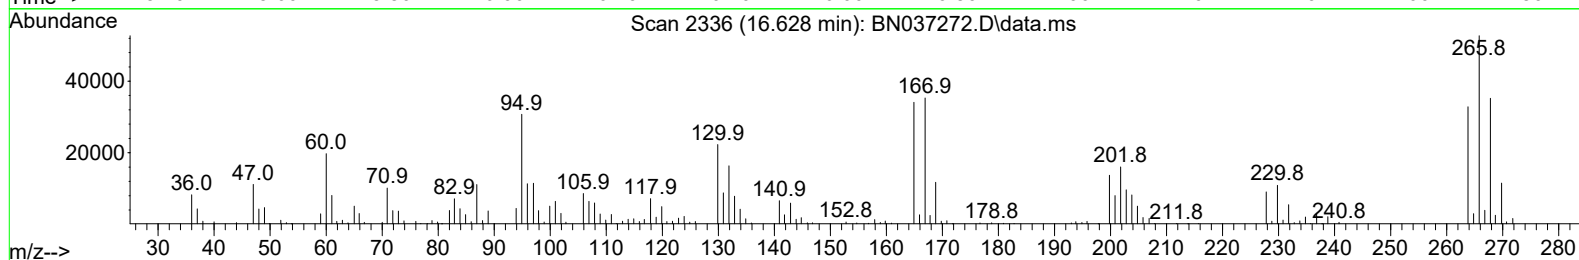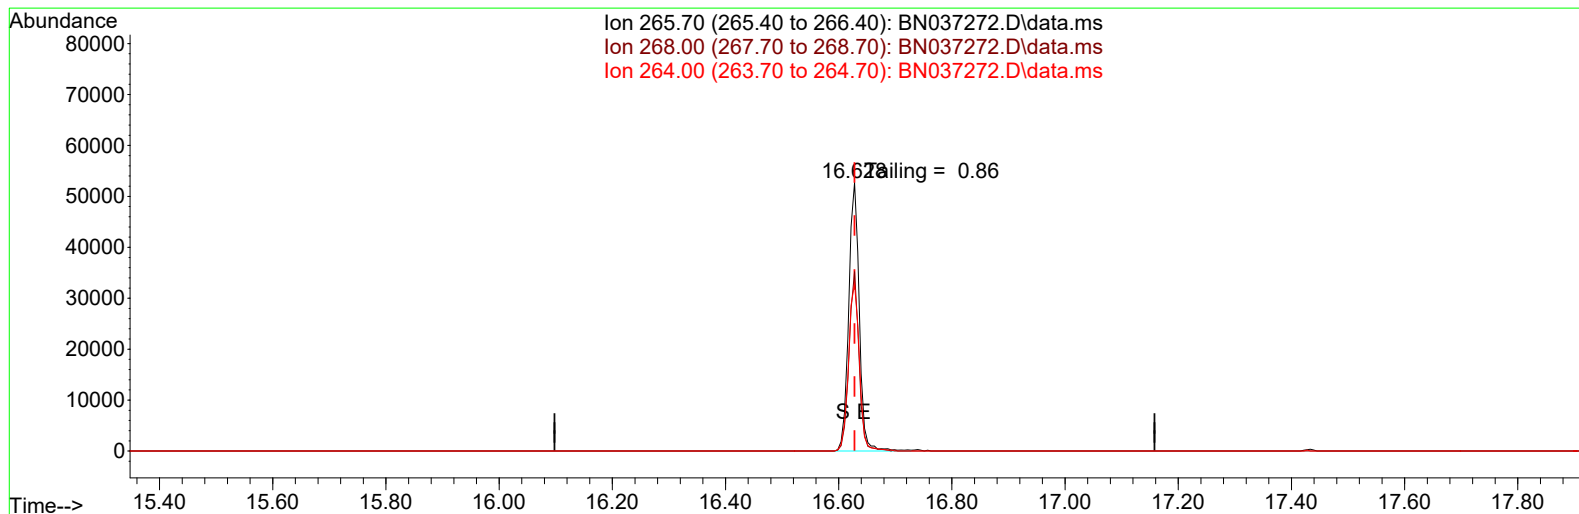

TIC: BN037272.D\data.ms

(70) Pentachlorophenol (C)

16.628min (0.000) 15244.65 ng




response 68073

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.57
264.00	61.60	62.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061325\
Data File : BN037272.D
Acq On : 14 Jun 2025 21:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 16 03:00:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 16 03:00:26 2025
Response via : Initial Calibration

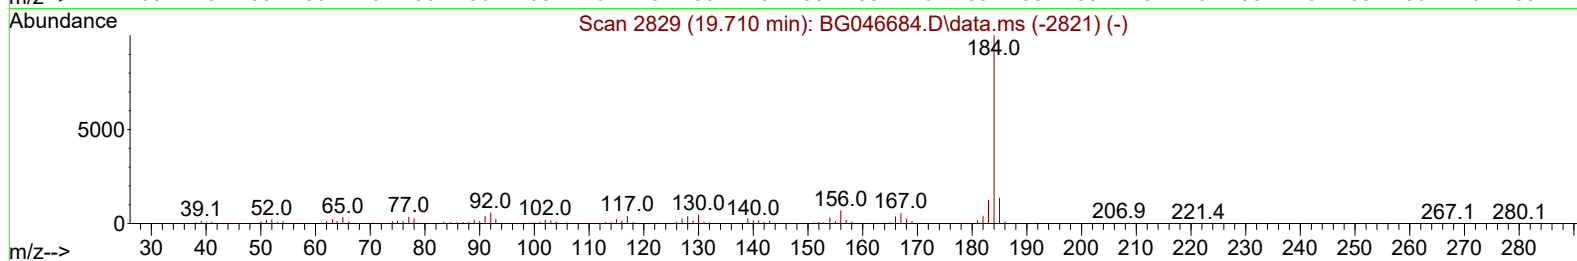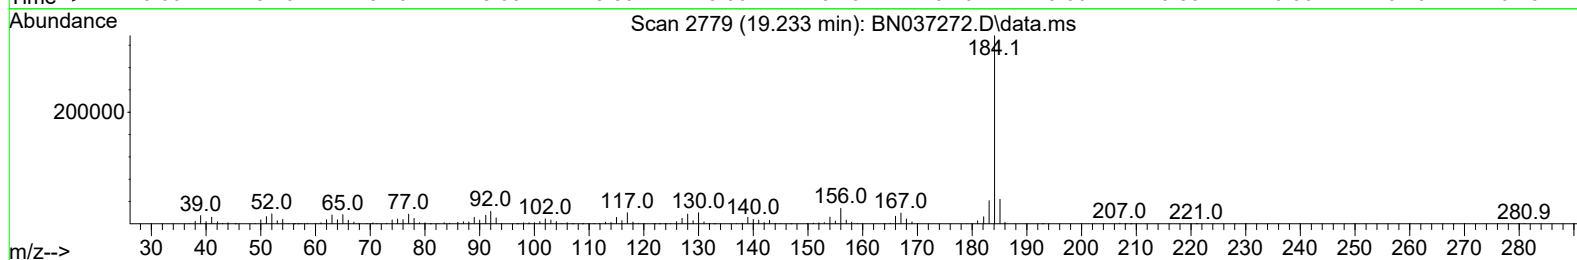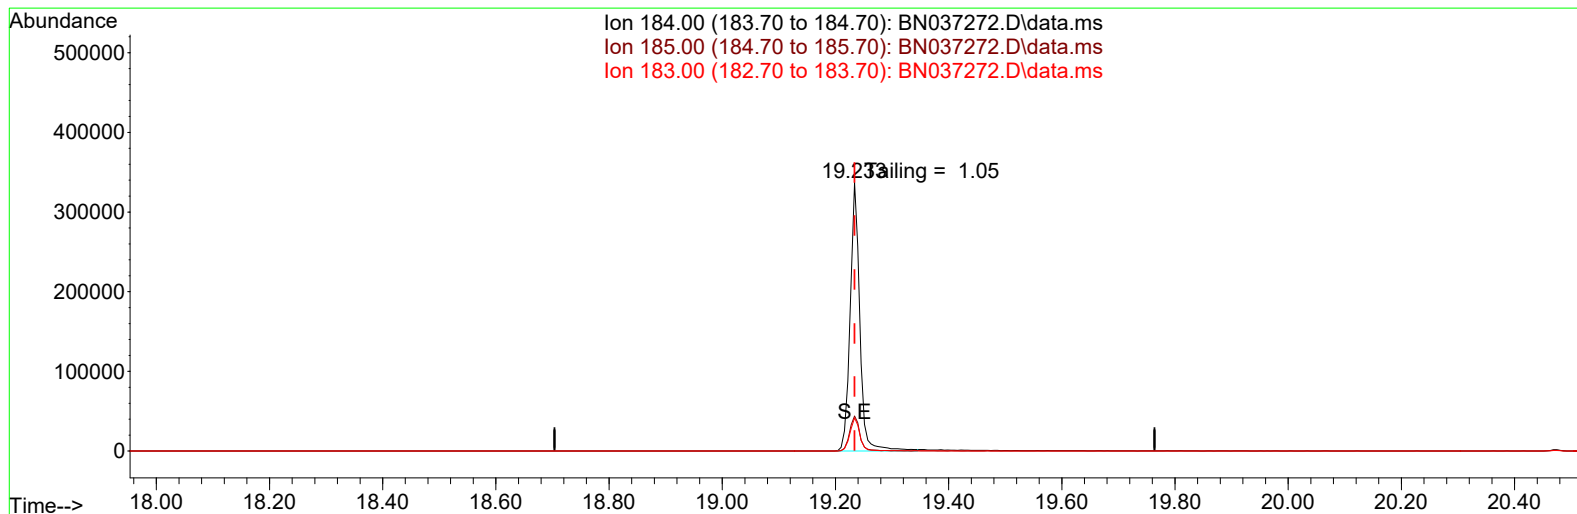

TIC: BN037272.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 404622

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.08
183.00	13.20	12.35
0.00	0.00	0.00