
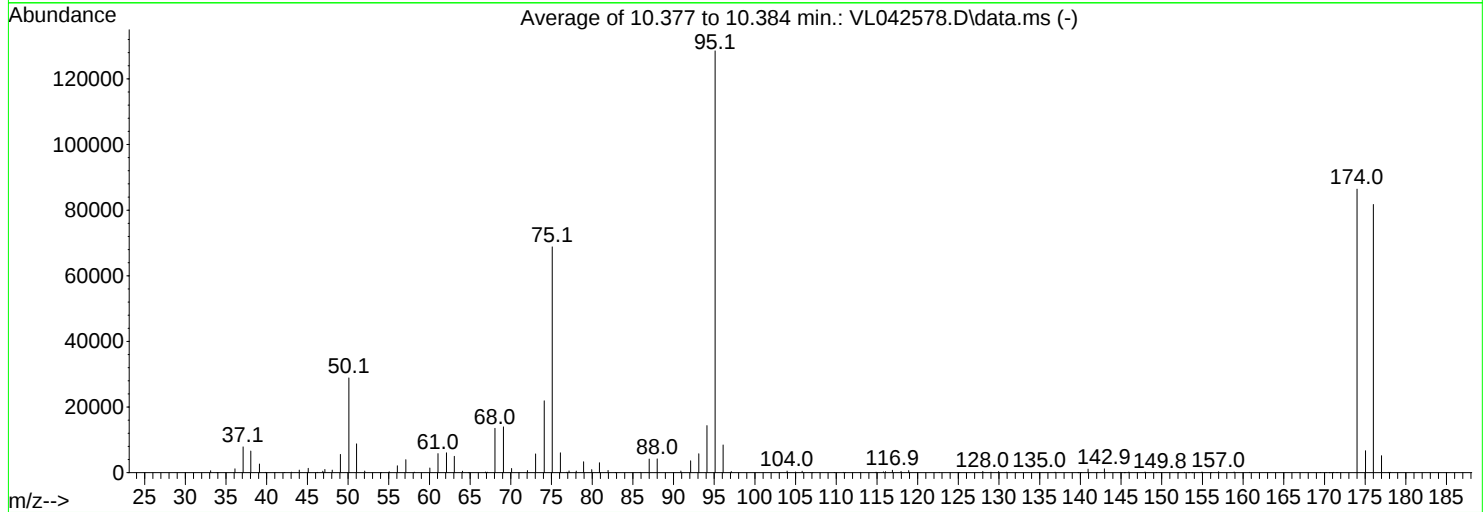


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL052925\
Data File : VL042578.D
Acq On : 29 May 2025 08:05
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052025AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Wed May 21 00:21:29 2025

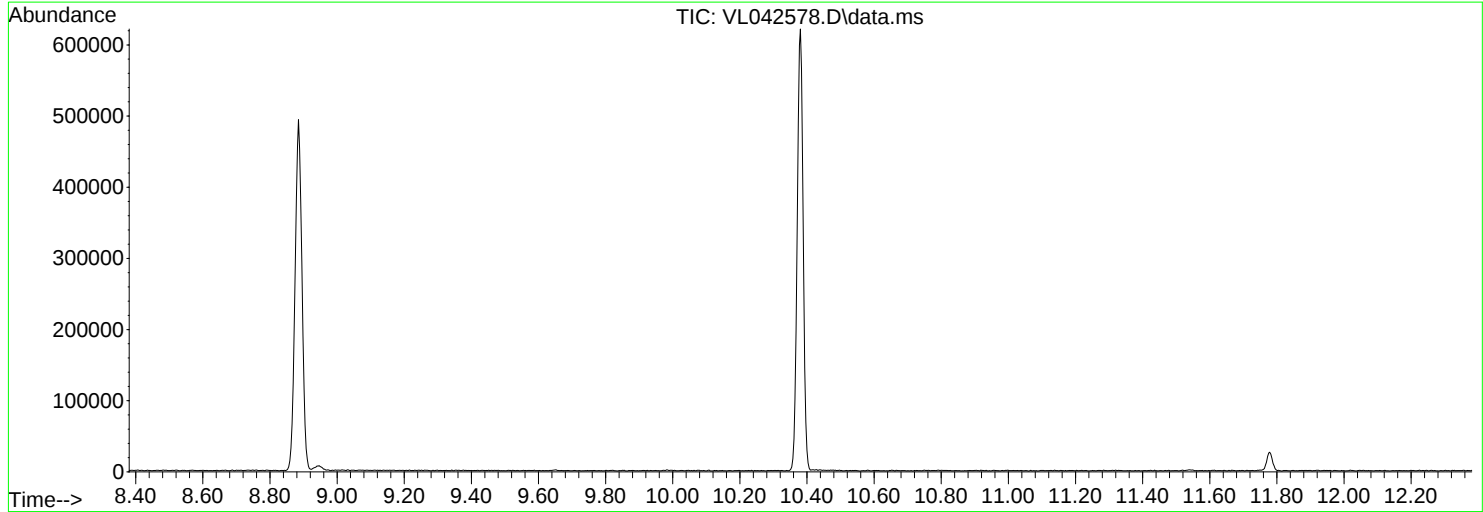

AutoFind: Scans 3179, 3180, 3181; Background Corrected with Scan 3165

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.4	28861	PASS
75	95	30	66	53.5	68792	PASS
95	95	100	100	100.0	128557	PASS
96	95	5	9	6.6	8426	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.2	86397	PASS
175	174	4	9	7.7	6664	PASS
176	174	93	101	94.6	81744	PASS
177	176	5	9	6.3	5154	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	604	45.10	1310	56.05	2107	68.05	1349
33.90	20	46.20	82	57.10	3938	69.10	1396
36.10	1179	46.90	454	58.15	159	70.10	125
37.10	7865	47.15	999	60.05	1394	71.00	7
38.05	6599	48.05	784	61.05	5793	72.05	616
39.10	2657	49.05	5570	62.10	6048	73.05	5702
39.90	81	50.10	28861	63.05	4979	74.10	21883
41.00	66	51.05	8796	64.05	430	75.10	68792
42.20	45	52.05	485	64.80	28	76.10	6072
43.05	164	54.00	17	66.90	188	76.90	143
44.00	762	55.05	314	67.10	147	77.15	541

Average of 10.377 to 10.384 min.: VL042578.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.05	512	93.10	5769	110.85	127	128.00	371
78.95	3322	94.10	14351	111.10	39	129.00	147
79.95	936	95.10	128557	112.95	118	129.95	325
80.90	3038	96.10	8426	114.90	160	130.95	149
81.95	666	97.10	324	115.80	234	132.10	57
82.85	69	103.95	507	116.05	275	134.80	45
85.90	102	105.00	185	116.90	719	135.00	127
87.00	4138	105.80	434	117.95	400	136.90	144
88.00	4195	106.80	76	118.90	638	139.70	25
90.90	504	107.00	24	122.65	40	140.10	50
92.10	3594	109.75	56	125.00	20	140.95	1056

Average of 10.377 to 10.384 min.: VL042578.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.05	103	152.80	86	170.90	53		
142.95	1152	153.30	25	171.10	116		
144.90	93	153.70	29	171.50	43		
145.10	33	154.95	214	171.65	64		
145.40	18	156.00	20	172.00	56		
145.95	182	157.00	303	174.00	86397		
147.00	65	158.90	220	175.05	6664		
147.95	210	160.80	92	176.00	81744		
149.35	45	169.50	60	177.00	5154		
149.80	42	170.20	51	177.90	98		
152.00	19	170.60	17	178.10	81		

Instrument :

MSVOA_L

ClientSampleId :

BFB