
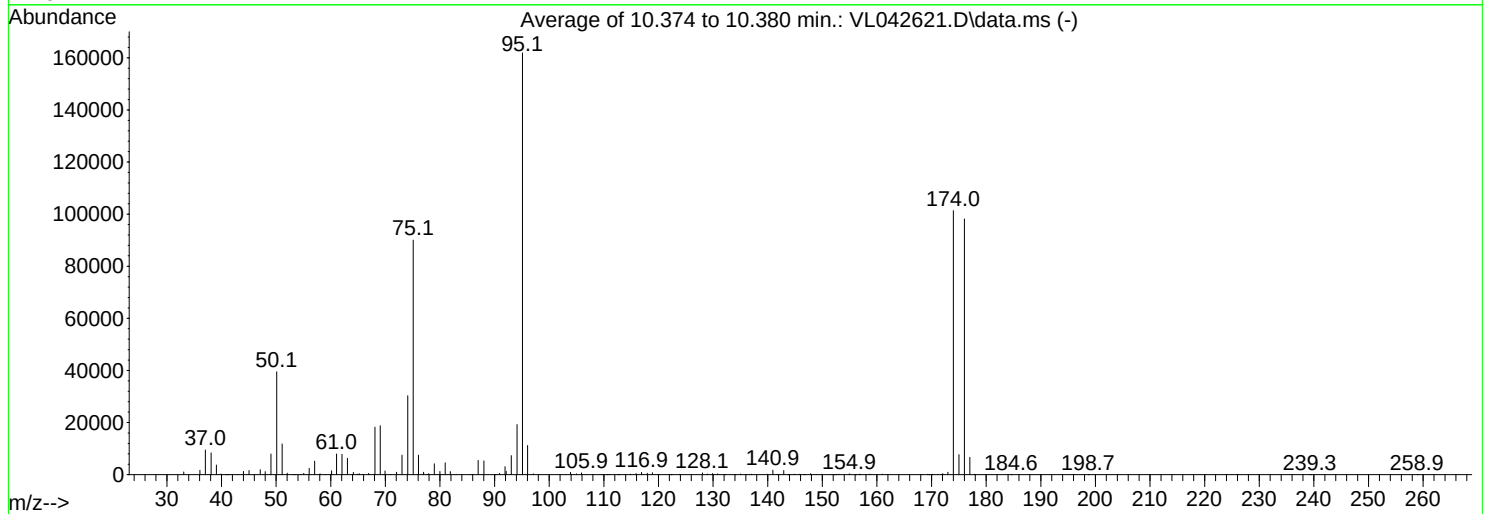


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061625\
Data File : VL042621.D
Acq On : 16 Jun 2025 08:07
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 30 02:01:56 2025

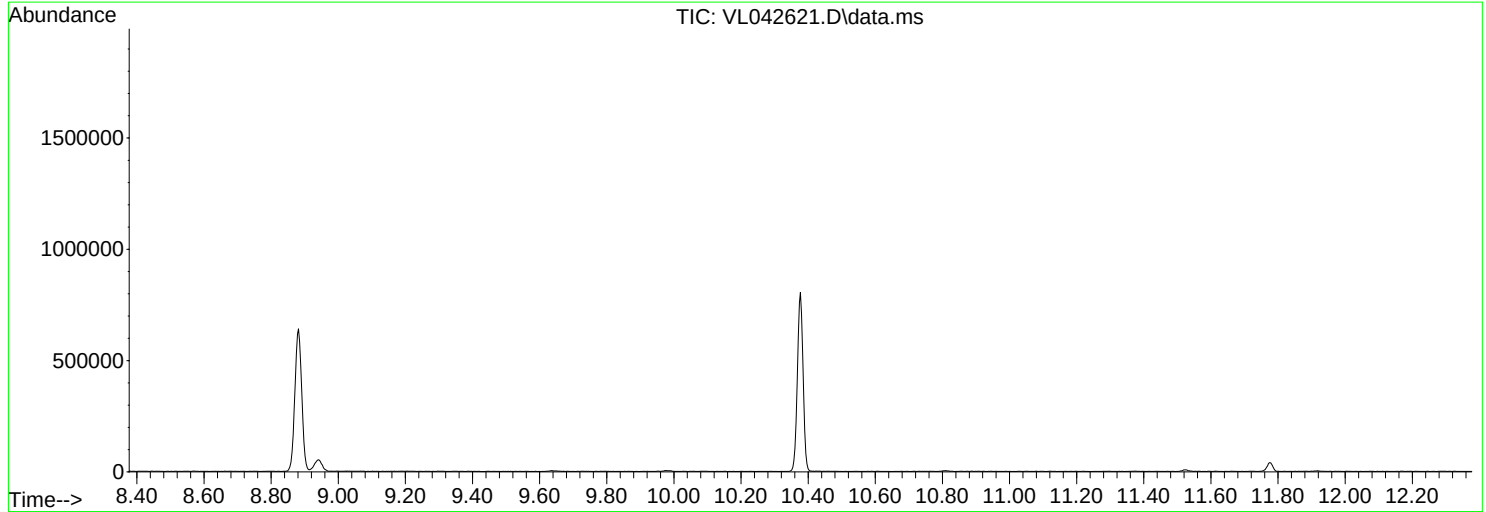

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	39483	PASS
75	95	30	66	55.6	90024	PASS
95	95	100	100	100.0	161920	PASS
96	95	5	9	6.9	11160	PASS
173	174	0.00	2	0.9	953	PASS
174	95	50	120	62.6	101357	PASS
175	174	4	9	7.6	7688	PASS
176	174	93	101	96.9	98187	PASS
177	176	5	9	6.7	6621	PASS

Average of 10.374 to 10.380 min.: VL042621.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1048	45.95	69	56.05	2408	65.85	41
36.05	1689	47.10	1941	57.05	5184	66.95	48
37.05	9469	48.00	1162	58.05	307	68.10	1822
38.10	8338	49.05	7955	59.10	62	69.05	1882
39.05	3716	50.10	39483	60.15	1458	69.95	1411
39.90	260	51.10	11792	61.05	7956	71.00	79
40.80	36	52.05	538	62.05	7825	72.05	953
41.20	18	53.10	86	63.05	6241	73.05	7523
43.00	57	53.30	28	64.15	874	74.10	30277
44.00	1219	54.40	58	65.00	232	75.10	90024
45.05	1593	55.05	477	65.25	284	76.05	7513

Average of 10.374 to 10.380 min.: VL042621.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	948	88.05	5293	103.90	854	114.90	208
77.70	151	90.10	28	105.00	313	115.90	450
77.95	359	90.90	485	105.90	654	116.90	885
78.95	4153	91.90	3082	106.80	54	117.95	552
80.00	1205	92.10	1326	109.70	79	118.90	733
80.95	4522	93.05	7319	109.90	32	119.90	17
81.90	1197	94.10	19213	110.60	21	122.30	18
82.95	150	95.10	161920	111.00	152	123.90	99
85.65	83	96.05	11160	112.00	73	126.00	100
86.00	59	97.10	337	112.50	54	128.05	652
87.00	5470	103.05	80	112.70	20	128.95	232

Average of 10.374 to 10.380 min.: VL042621.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.90	413	142.05	115	151.75	92	161.05	195
130.85	330	142.95	1620	152.10	36	168.25	70
132.10	21	143.70	37	152.50	33	169.20	111
134.00	23	144.05	80	153.05	185	169.50	37
135.05	242	144.80	186	154.00	98	170.00	37
136.15	48	145.10	67	154.95	325	170.25	91
136.70	47	145.90	201	156.10	29	171.15	93
137.05	200	146.70	28	156.80	171	171.80	96
139.95	216	147.85	389	157.00	54	172.05	384
140.95	1747	148.85	48	158.70	167	173.00	953
141.75	116	149.95	210	158.90	63	174.00	101357

Average of 10.374 to 10.380 min.: VL042621.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.00	7688						
176.00	98187						
177.00	6621						
177.85	146						
178.10	46						
184.60	22						
198.70	17						
239.30	17						
258.90	17						

Instrument :

MSVOA_L

ClientSampleId :

BFB