


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061725\
Data File : VN087044.D
Acq On : 17 Jun 2025 08:51
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

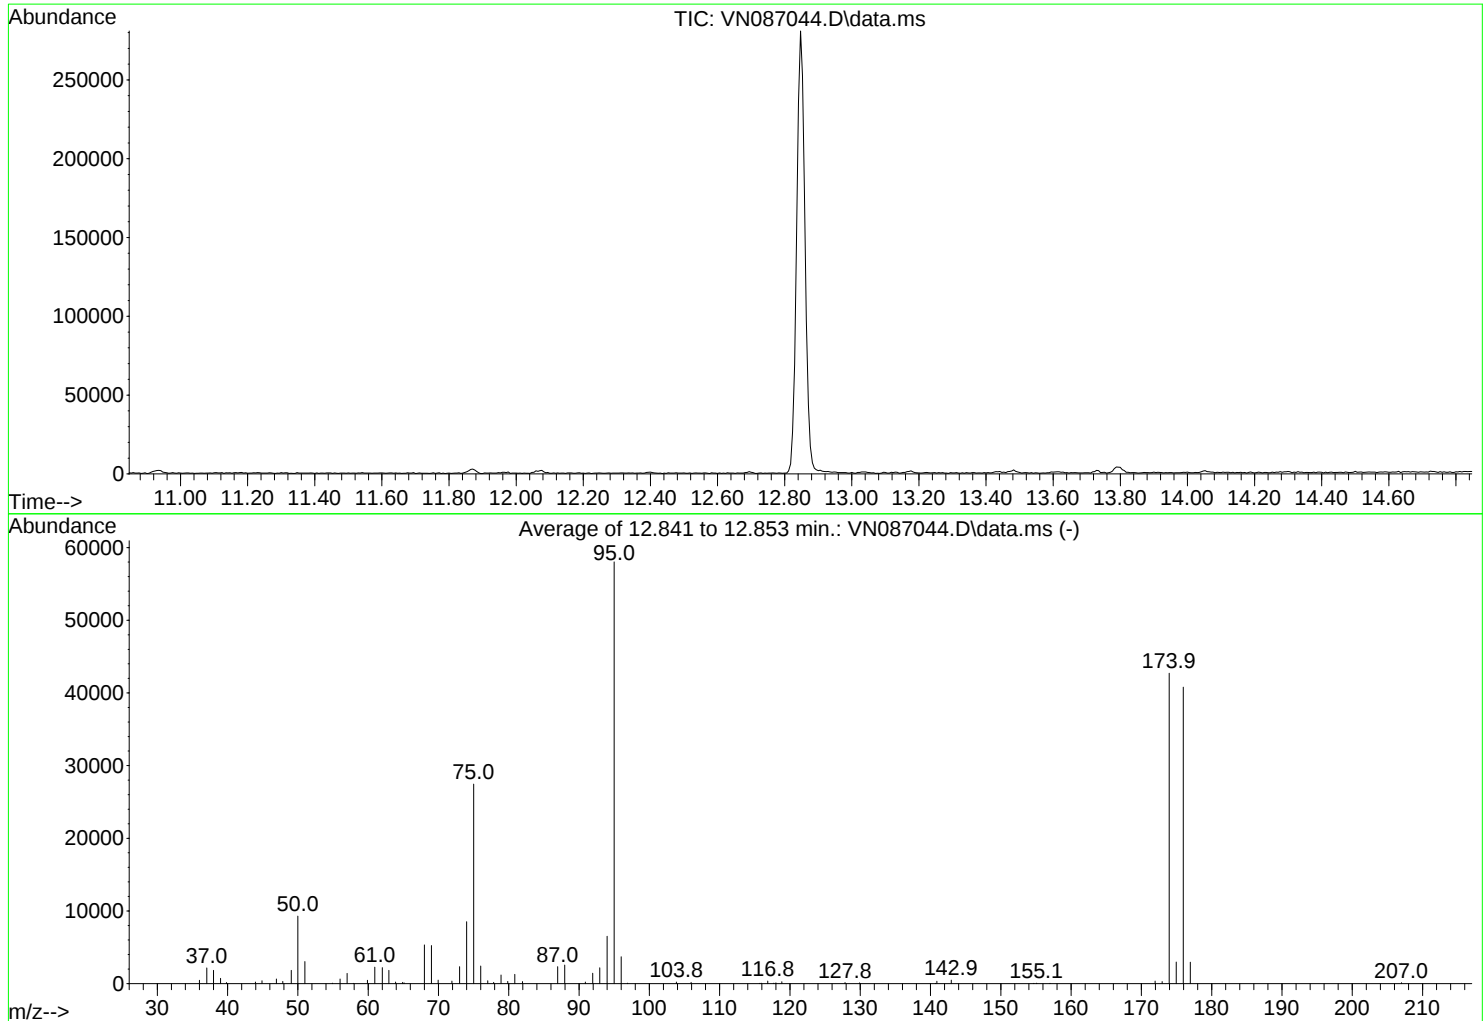

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	9291	PASS
75	95	30	60	47.3	27451	PASS
95	95	100	100	100.0	58037	PASS
96	95	5	9	6.4	3705	PASS
173	174	0.00	2	0.7	297	PASS
174	95	50	100	73.6	42712	PASS
175	174	5	9	7.0	2969	PASS
176	174	95	101	95.5	40787	PASS
177	176	5	9	7.2	2942	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	454	51.00	3033	65.10	105	78.90	119
37.05	2152	54.90	63	68.00	5318	79.85	31
38.00	1824	56.00	647	69.00	5238	80.85	127
39.00	739	57.00	1412	69.95	491	81.95	29
39.85	146	57.90	51	71.90	346	86.95	2337
43.95	228	59.90	475	73.00	2344	87.95	2560
44.90	406	60.95	2266	74.00	8531	90.90	213
46.95	647	62.00	2192	75.00	27451	91.95	1435
47.85	313	62.95	1819	76.00	2419	92.95	2174
49.05	1827	63.90	223	77.00	390	94.00	6515
50.00	9291	64.90	168	77.85	178	95.00	58037

Average of 12.841 to 12.853 min.: VN087044.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.00	3705	129.90	104	175.95	40787		
96.90	62	140.70	51	176.95	2942		
103.85	227	140.90	341	207.00	131		
105.95	187	142.95	487				
115.70	54	154.70	51				
115.90	68	155.10	57				
116.85	343	157.00	53				
117.70	63	171.95	343				
118.00	115	172.95	297				
118.85	259	173.95	42712				
127.85	153	174.95	2969				