


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061825\
Data File : BP024986.D
Acq On : 18 Jun 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 06 16:20:27 2025

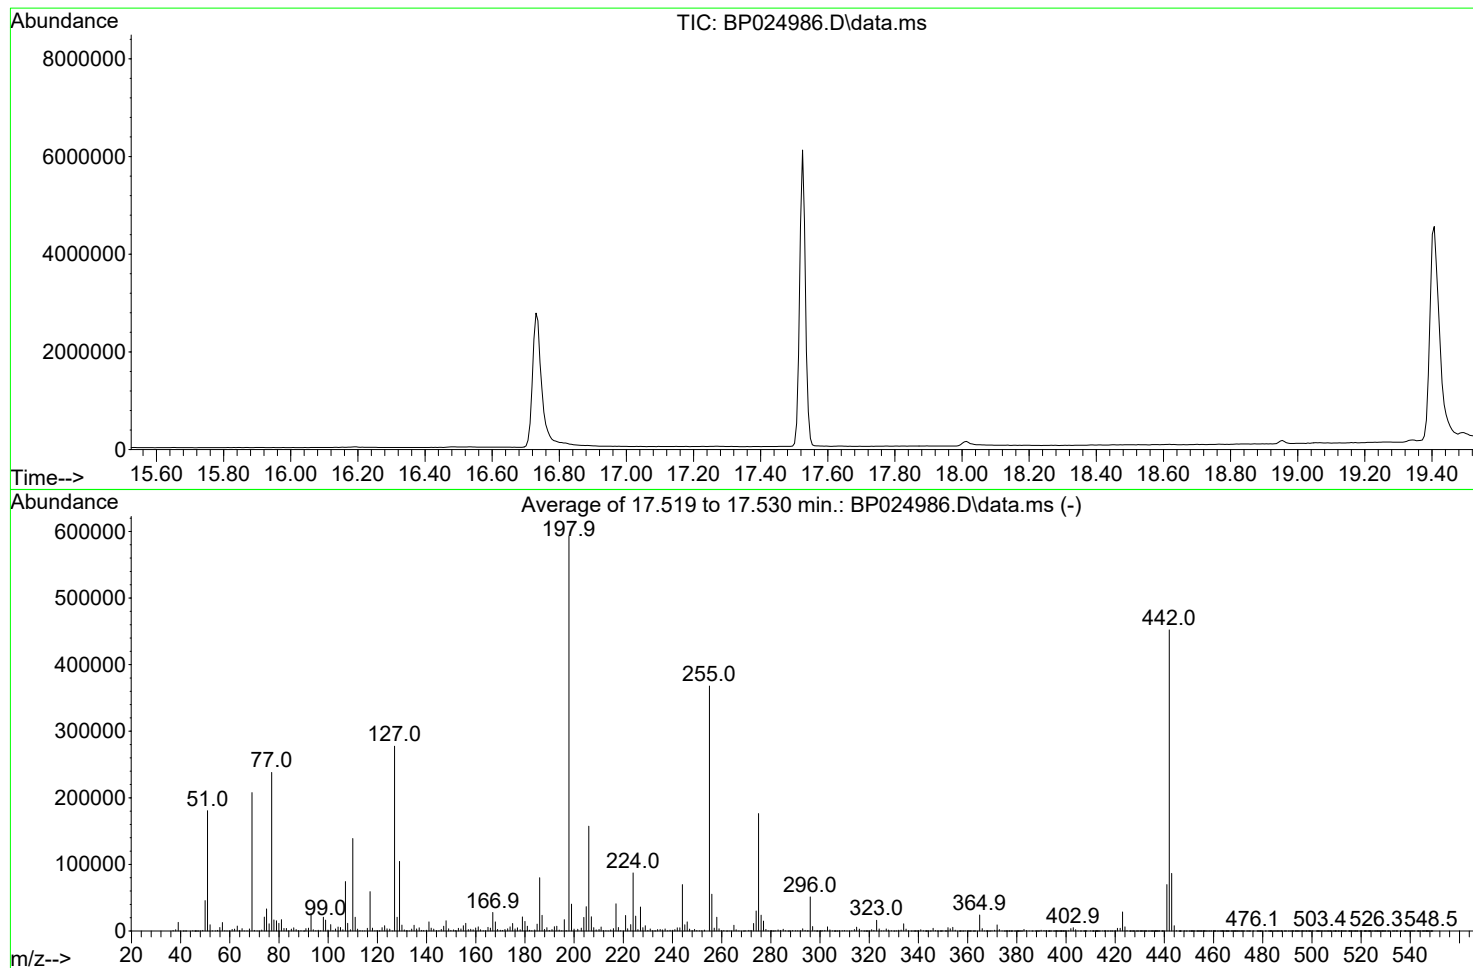

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	3188	PASS
69	69	100	100	100.0	207869	PASS
70	69	0.00	2	0.5	1028	PASS
197	198	0.00	2	0.1	776	PASS
198	198	100	100	100.0	592942	PASS
199	198	5	9	6.8	40483	PASS
365	198	1	100	4.1	24073	PASS
441	443	0.01	150	80.7	69821	PASS
442	442	100	100	100.0	452245	PASS
443	442	15	24	19.1	86555	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/18/2025	BNA_P	<u>BP024386.D</u>
Compound Name	Response	Retention Time
DDT	1976784	20.683
DDD	62779	20.224
DDE	5557	19.695
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68336	2045120	3.34

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061825\
Data File : BP024986.D
Acq On : 18 Jun 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 18 11:34:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

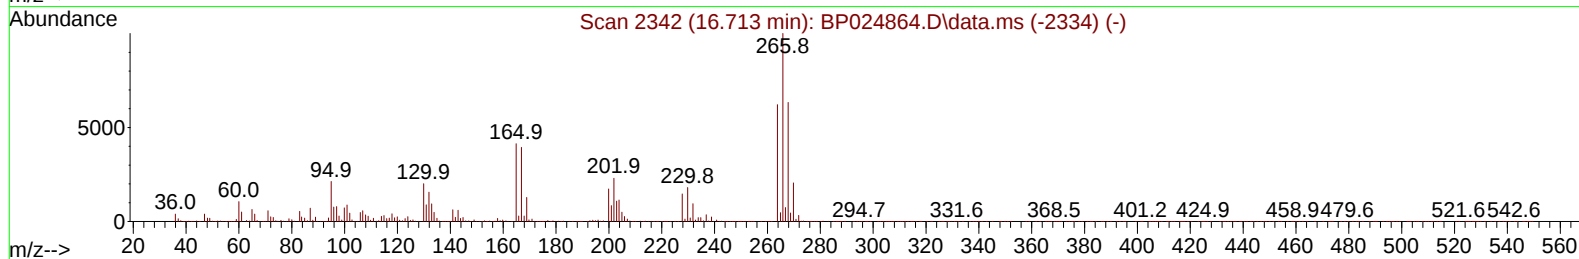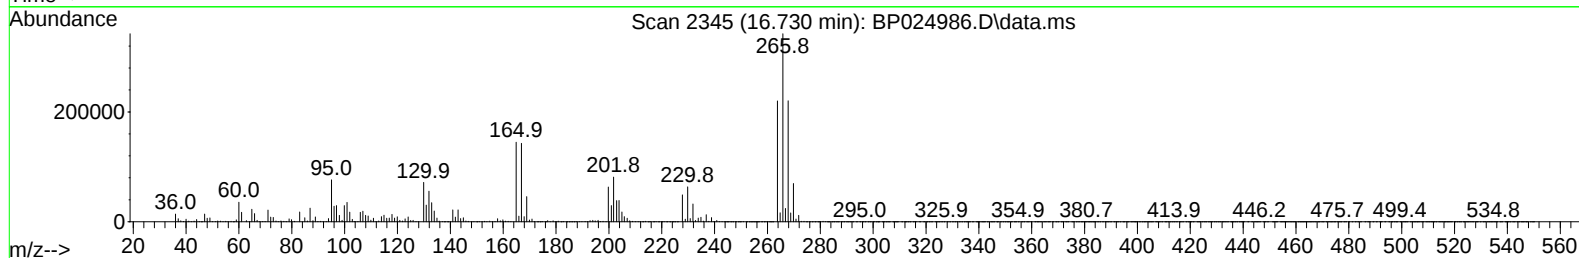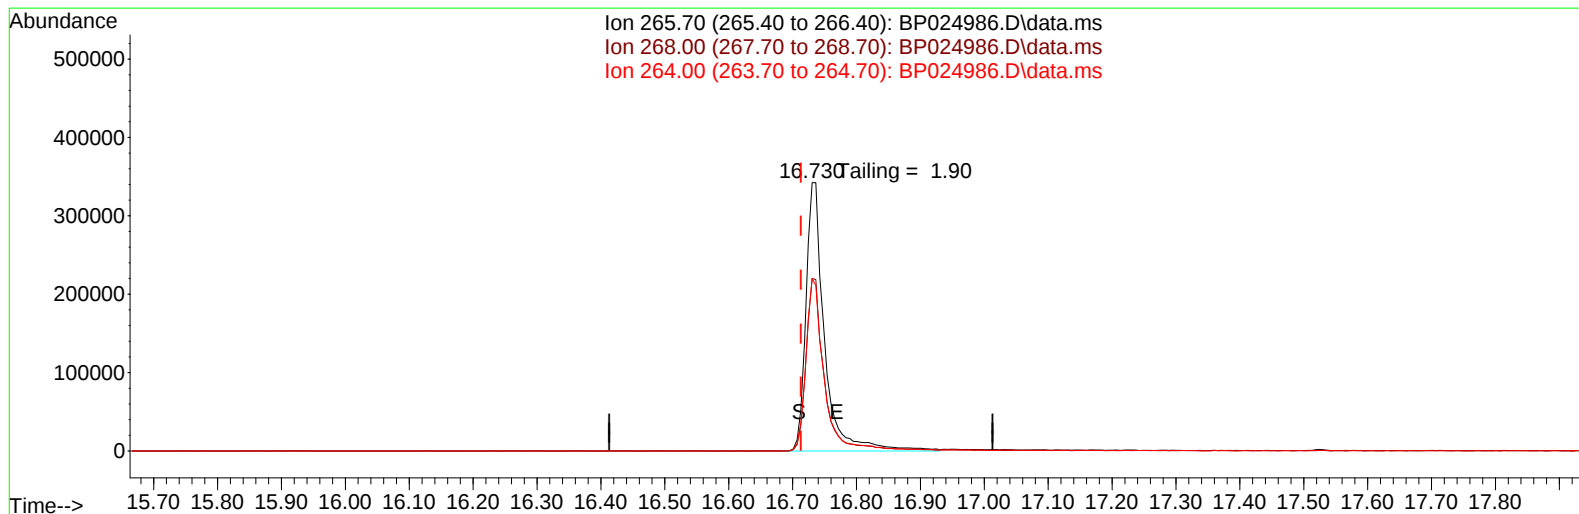

TIC: BP024986.D\data.ms

(70) Pentachlorophenol (C)

16.730min (+ 0.017) 2136417.31 ng




response 695724

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.34
264.00	62.10	64.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP061825\
Data File : BP024986.D
Acq On : 18 Jun 2025 09:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 18 11:34:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP060625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 06 16:20:27 2025
Response via : Initial Calibration

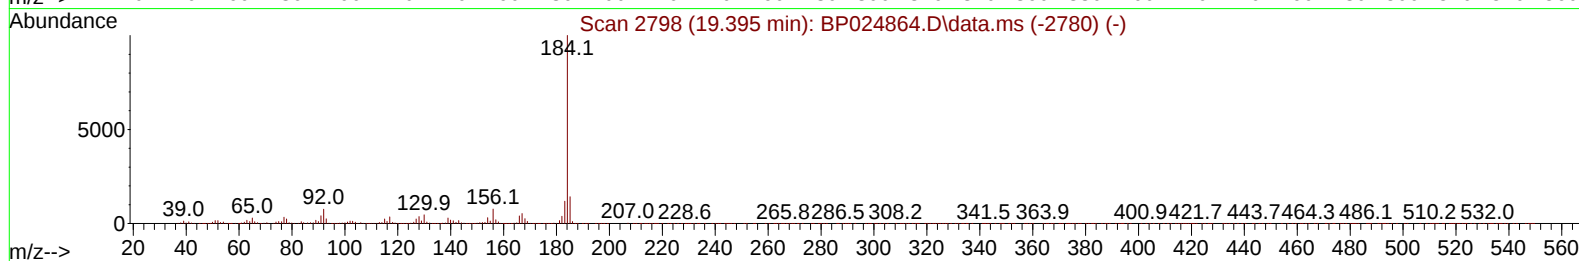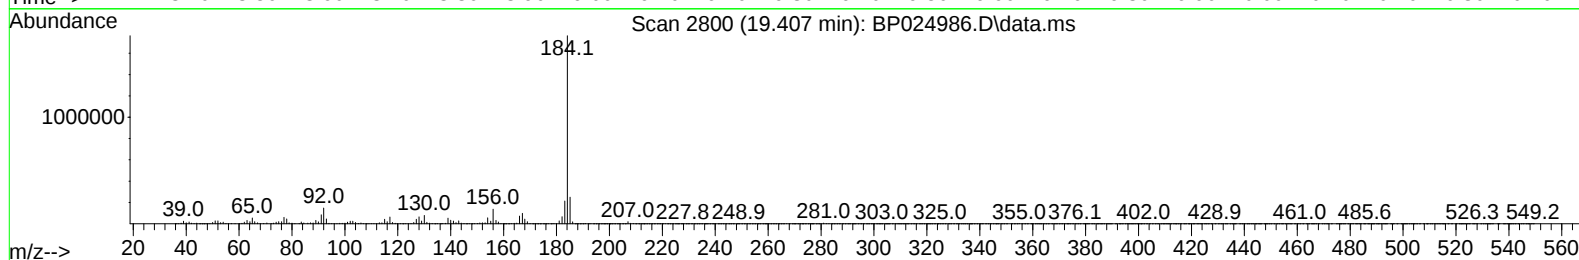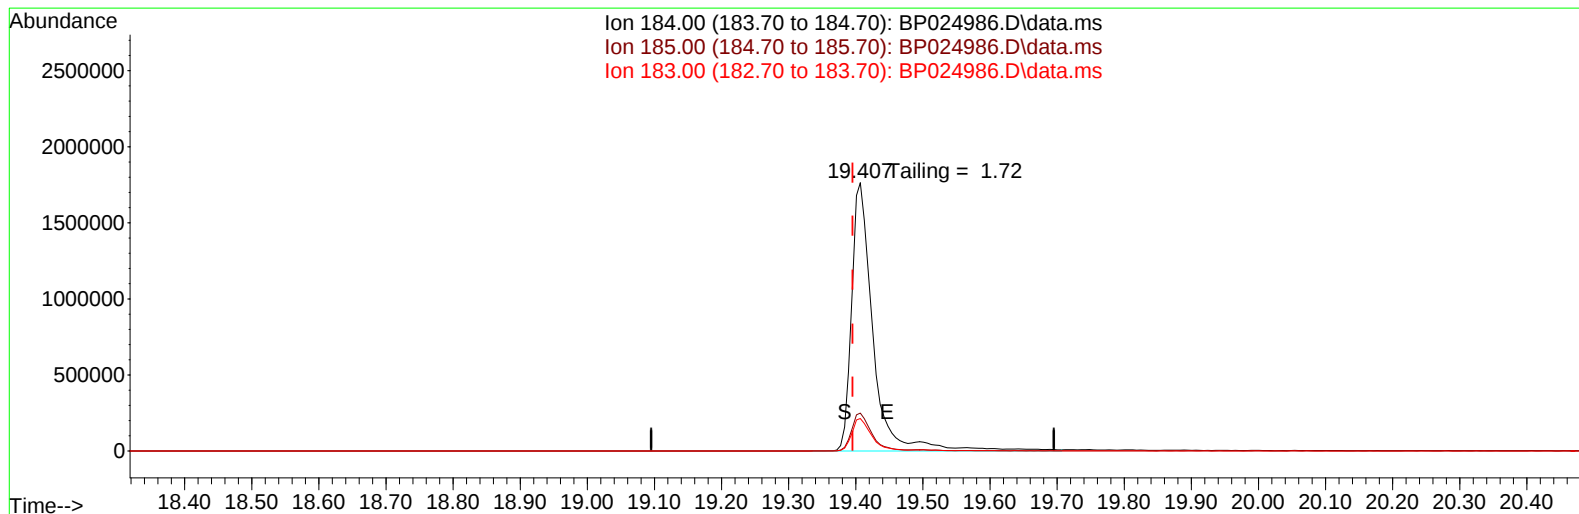

TIC: BP024986.D\data.ms

(77) Benzidine

19.407min (+ 0.012) 430098.83 ng

response 3649895

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.16
183.00	11.90	12.09
0.00	0.00	0.00