


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061925\
Data File : VX046757.D
Acq On : 19 Jun 2025 08:42
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
Title : SW846 8260
Last Update : Wed Jun 18 03:09:16 2025

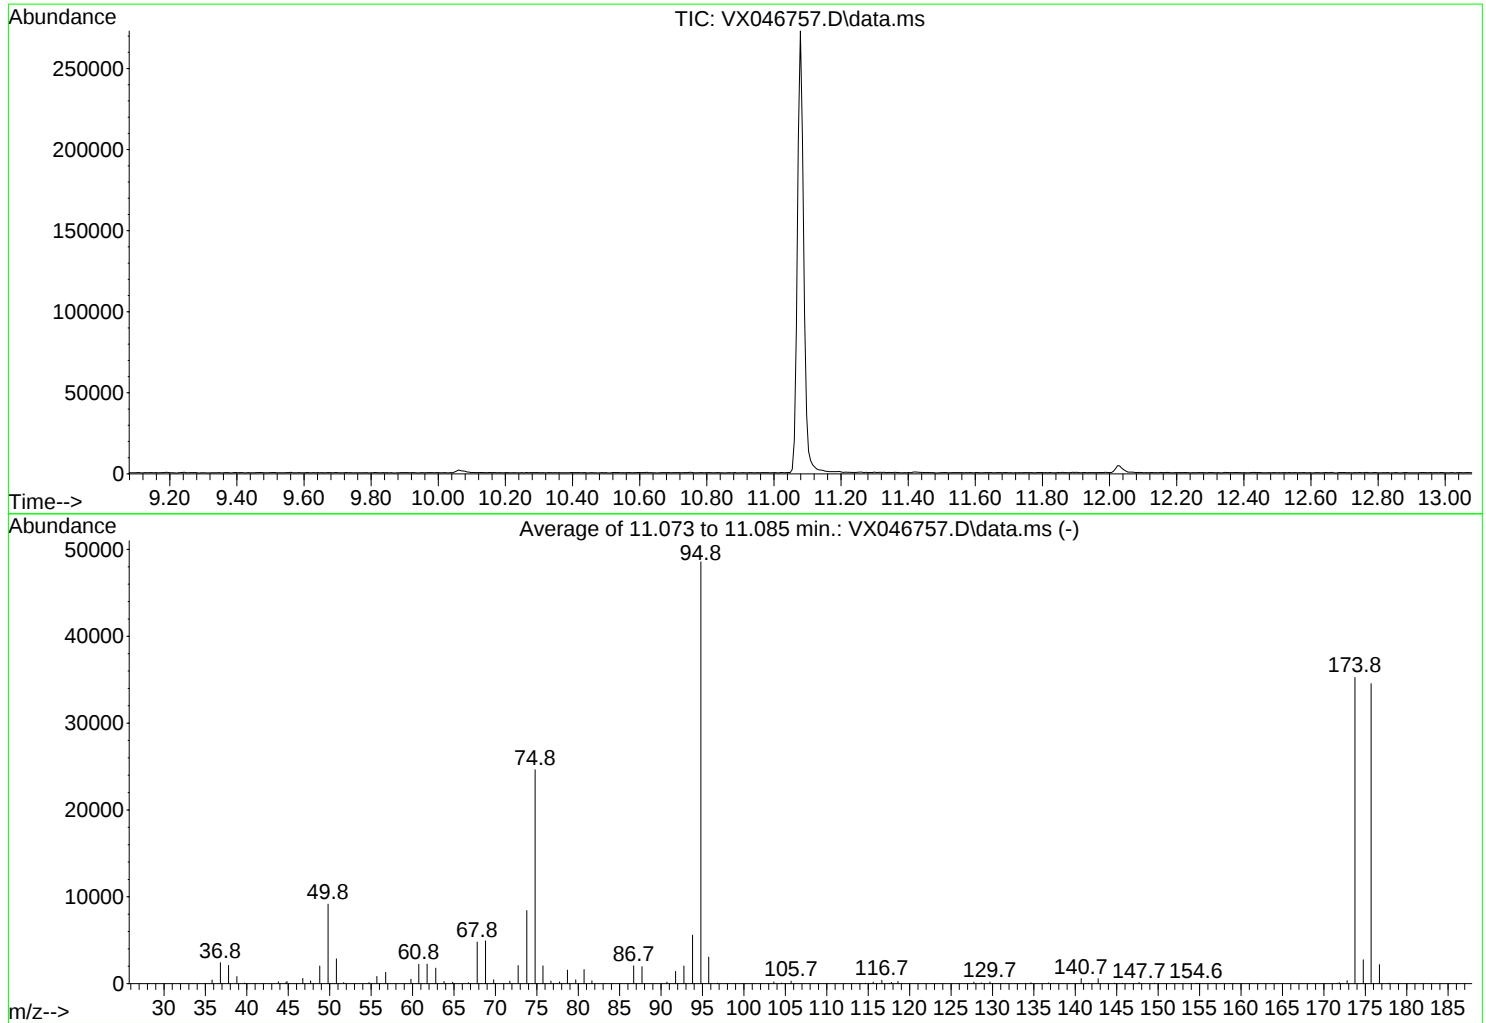

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	9154	PASS
75	95	30	60	50.7	24627	PASS
95	95	100	100	100.0	48571	PASS
96	95	5	9	6.3	3061	PASS
173	174	0.00	2	1.0	352	PASS
174	95	50	100	72.6	35267	PASS
175	174	5	9	7.8	2745	PASS
176	174	95	101	97.9	34539	PASS
177	176	5	9	6.3	2186	PASS