


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062125\
Data File : BN037351.D
Acq On : 20 Jun 2025 15:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 20 23:41:54 2025

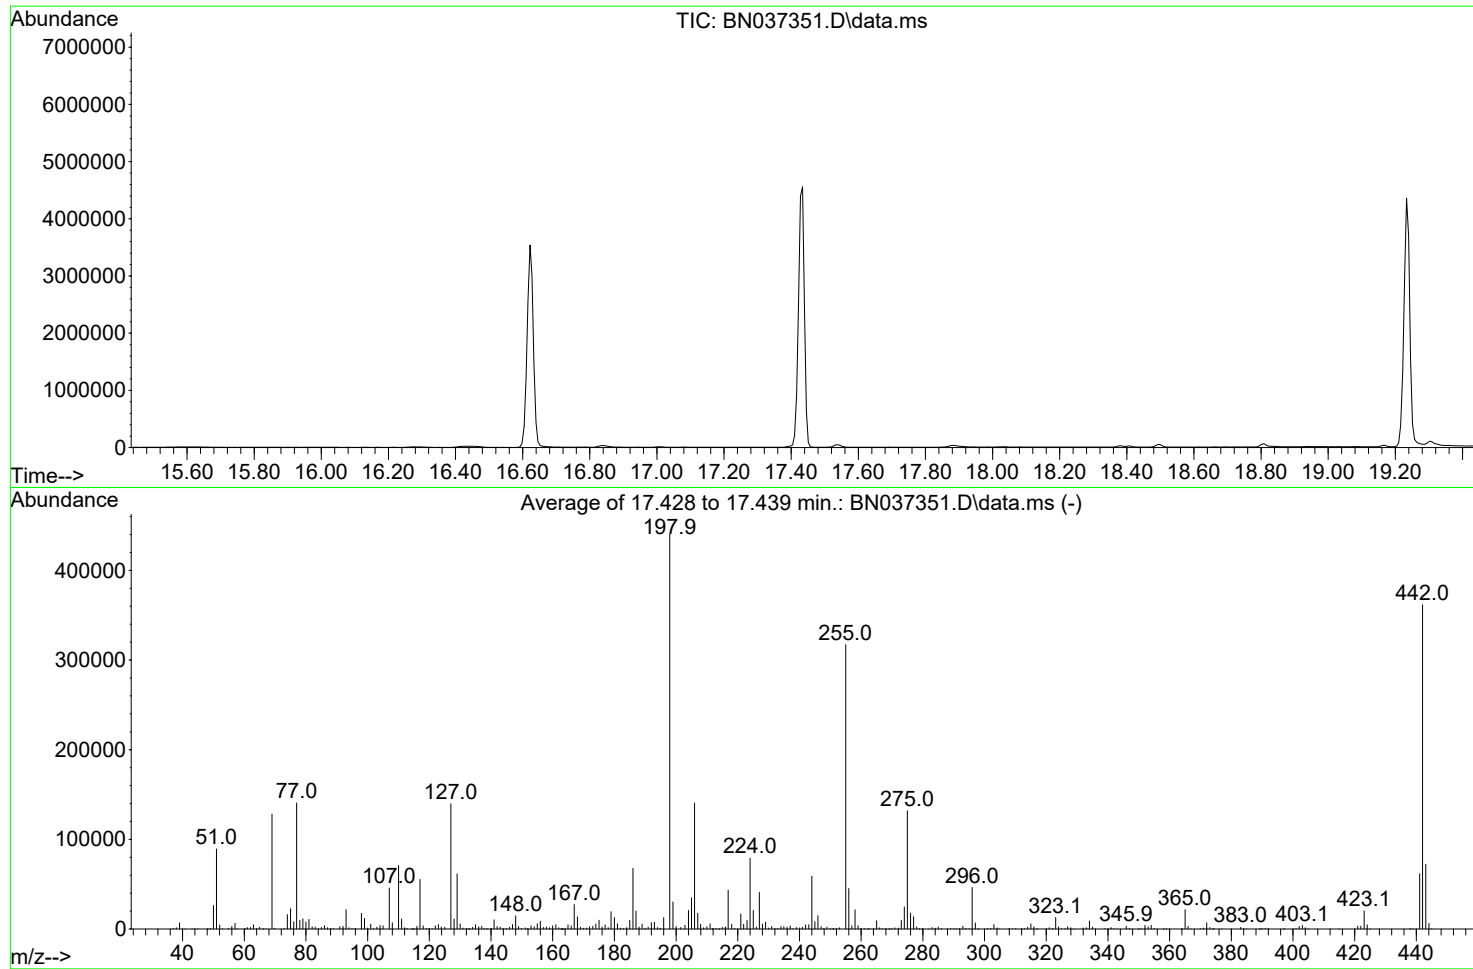

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	128141	PASS
70	69	0.00	2	0.7	882	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	440469	PASS
199	198	5	9	6.8	30163	PASS
365	198	1	100	4.9	21610	PASS
441	443	0.01	150	85.2	61520	PASS
442	442	100	100	100.0	361557	PASS
443	442	15	24	20.0	72213	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/21/2025	BNA_N	<u>BN037351.D</u>
Compound Name	Response	Retention Time
DDT	1600198	20.475
DDD	22591	20.257
DDE	1214	19.522
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23805	1624003	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062125\
Data File : BN037351.D
Acq On : 20 Jun 2025 15:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 21 02:21:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

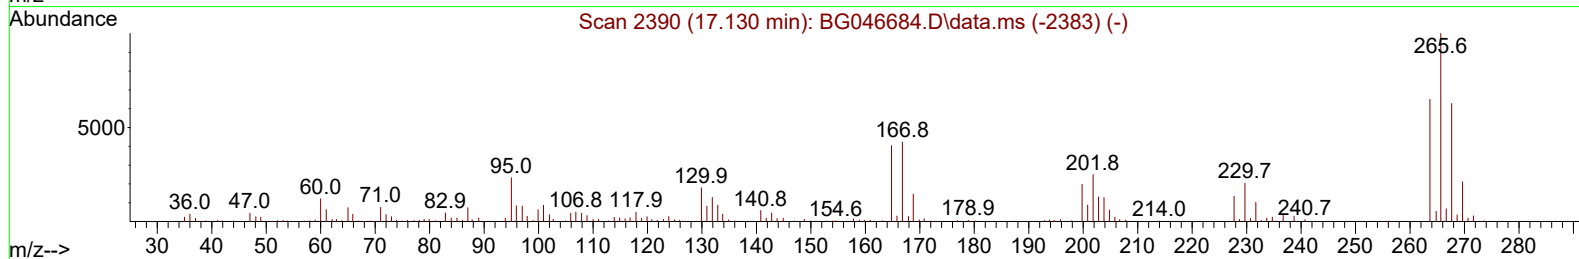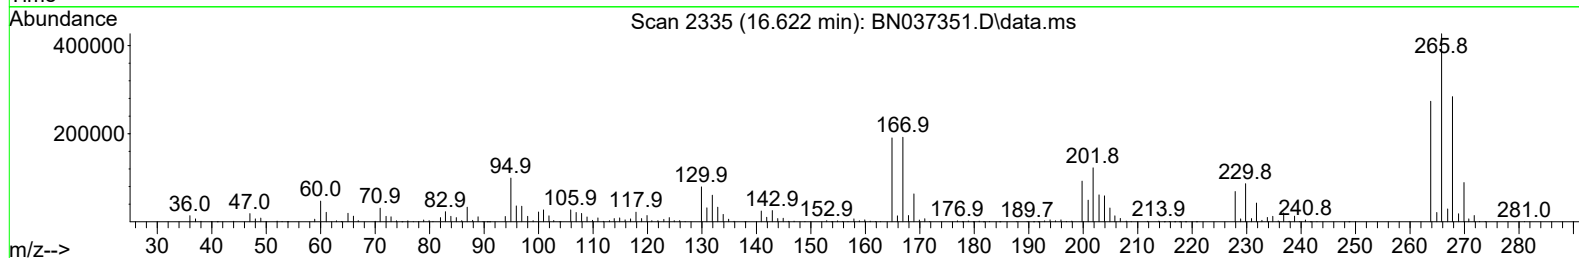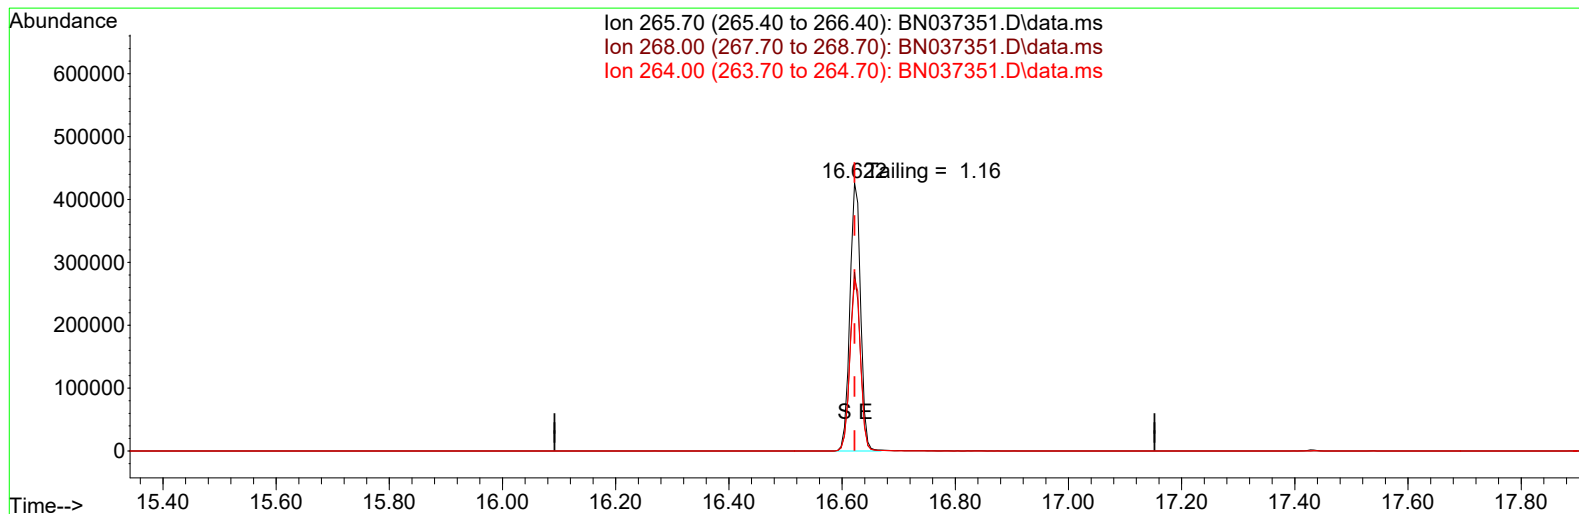

TIC: BN037351.D\data.ms

(70) Pentachlorophenol (C)

16.622min (0.000) 21508.69 ng




response 561749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.53
264.00	61.60	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062125\
Data File : BN037351.D
Acq On : 20 Jun 2025 15:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 21 02:21:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

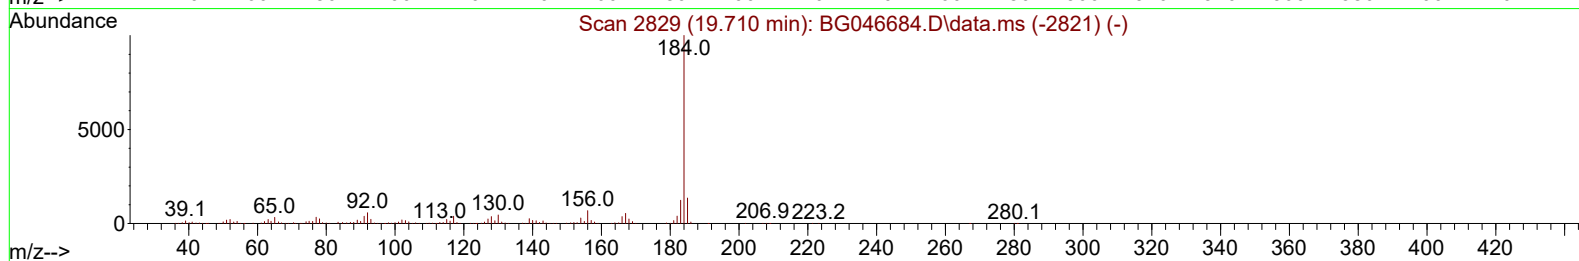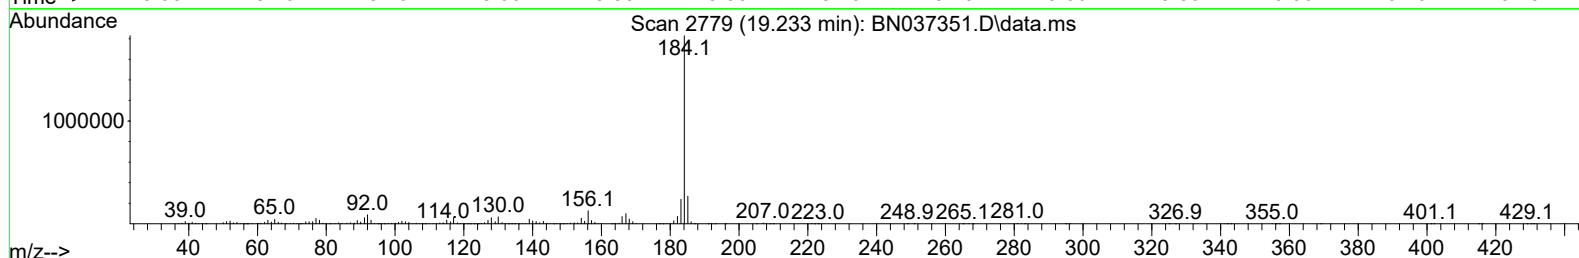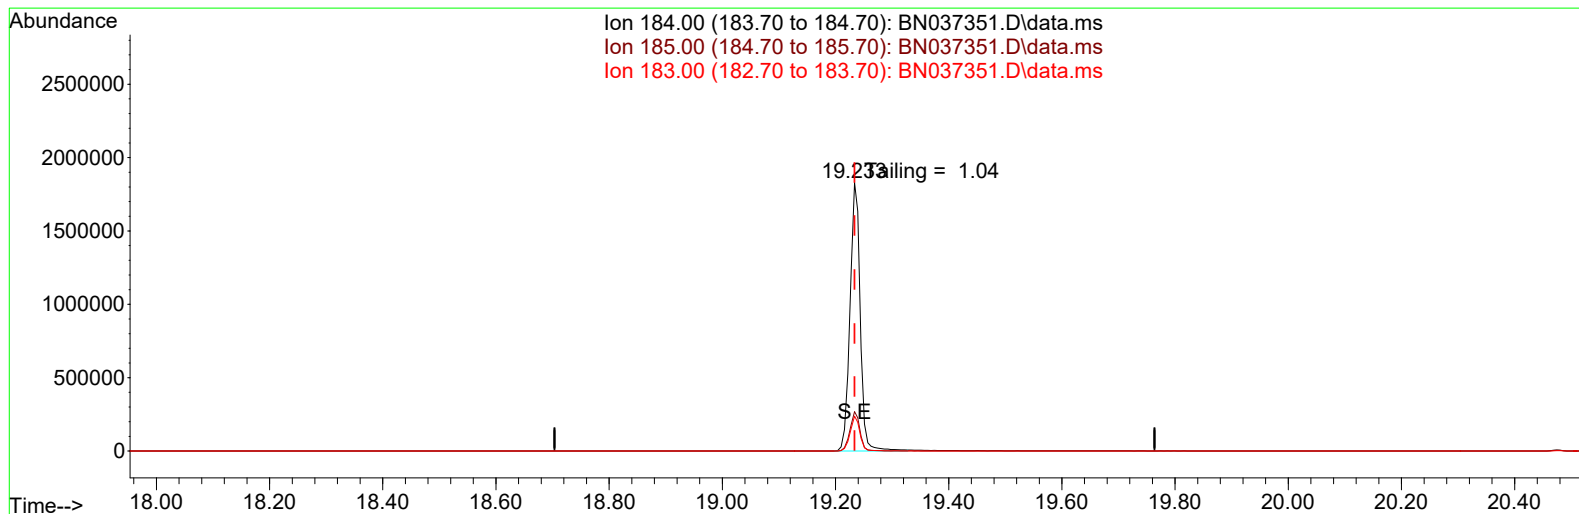

TIC: BN037351.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 2309913

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	13.00
0.00	0.00	0.00