


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062725\
Data File : BN037416.D
Acq On : 27 Jun 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 27 04:09:23 2025

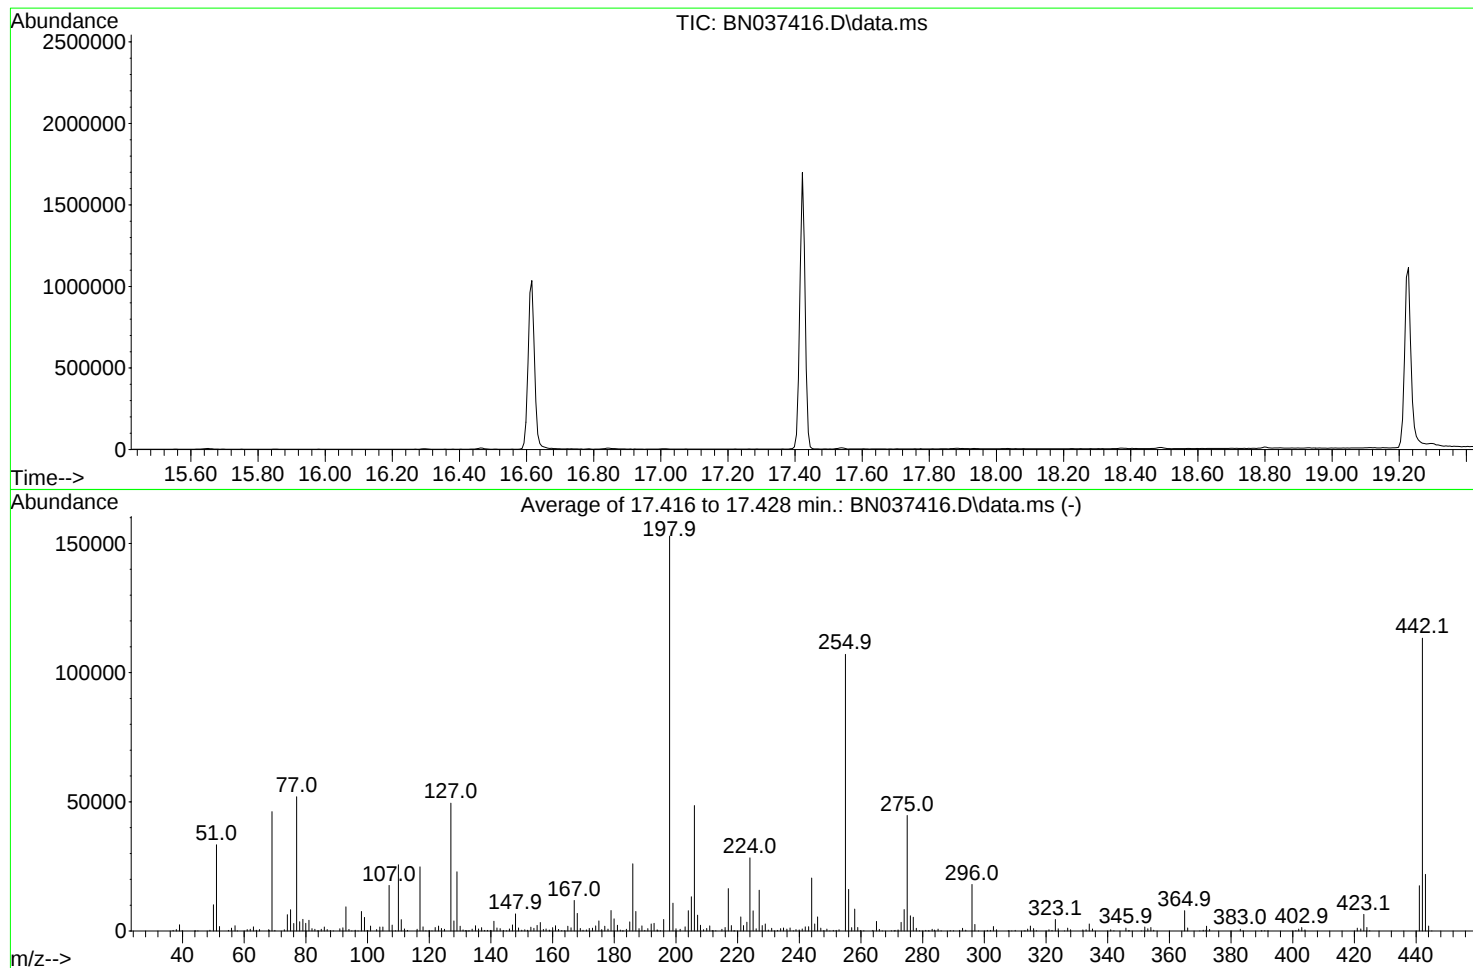




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.1	485	PASS
69	69	100	100	100.0	46181	PASS
70	69	0.00	2	0.6	273	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	152824	PASS
199	198	5	9	7.1	10807	PASS
365	198	1	100	5.1	7868	PASS
441	443	0.01	150	79.9	17524	PASS
442	442	100	100	100.0	113360	PASS
443	442	15	24	19.3	21933	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062725\
Data File : BN037416.D
Acq On : 27 Jun 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 15:30:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

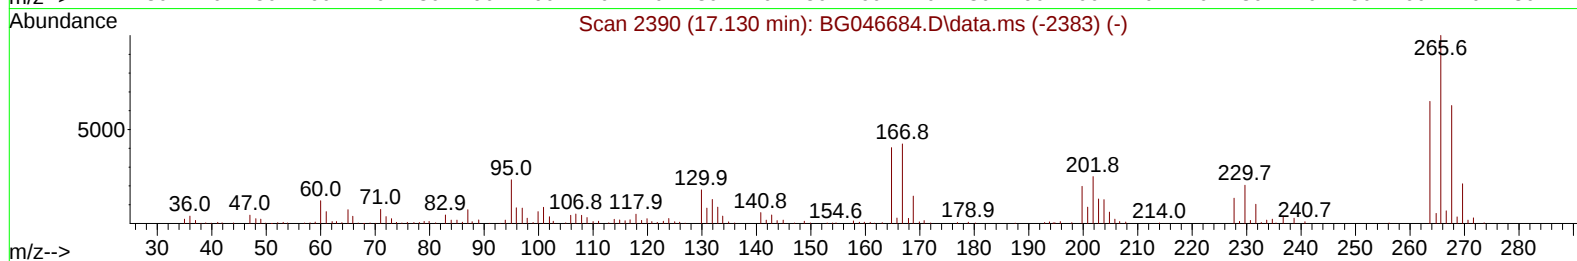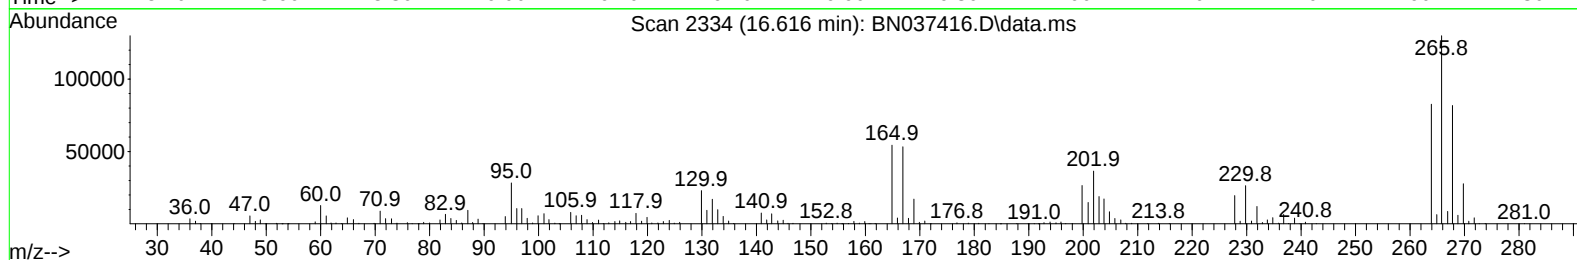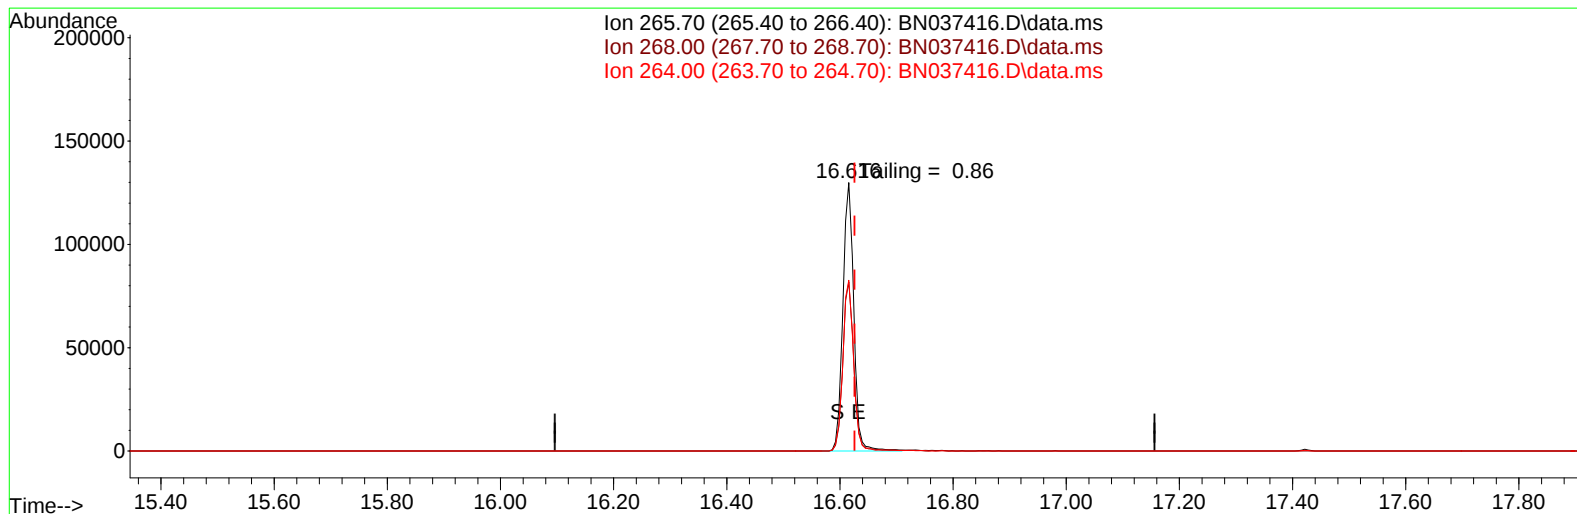

TIC: BN037416.D\data.ms

(70) Pentachlorophenol (C)

16.616min (-0.010) 18836.45 ng




response 173545

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.94
264.00	61.60	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062725\
Data File : BN037416.D
Acq On : 27 Jun 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 15:30:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

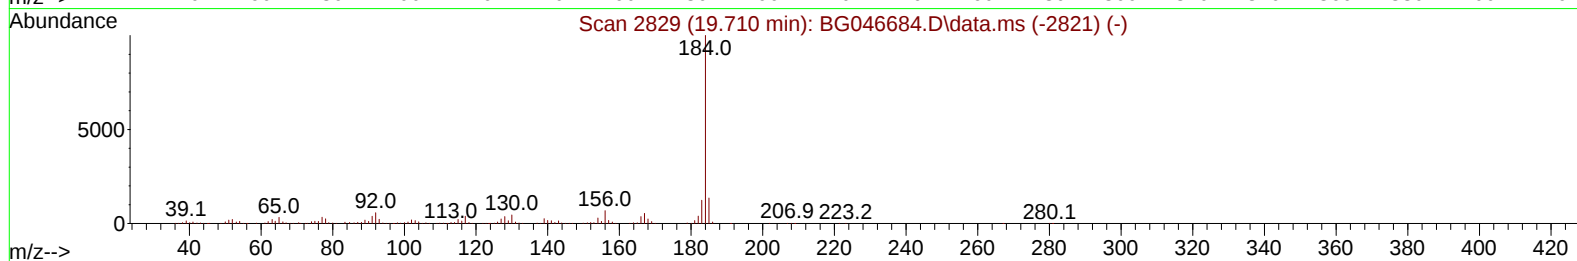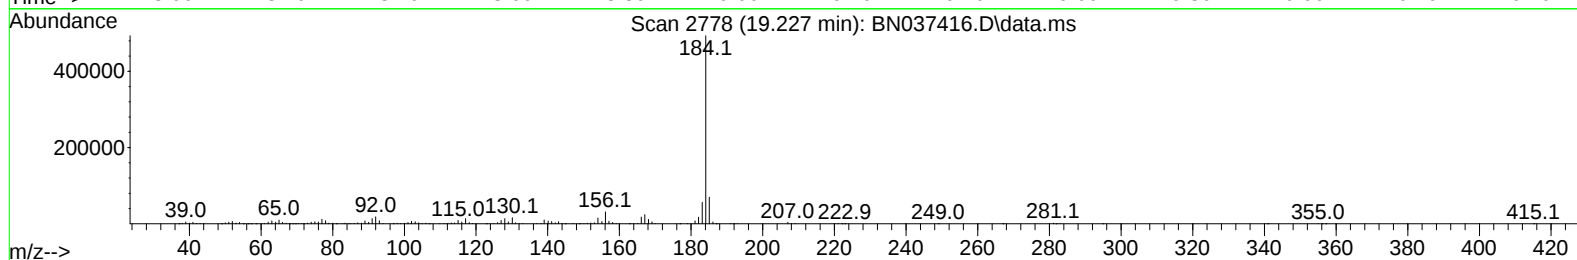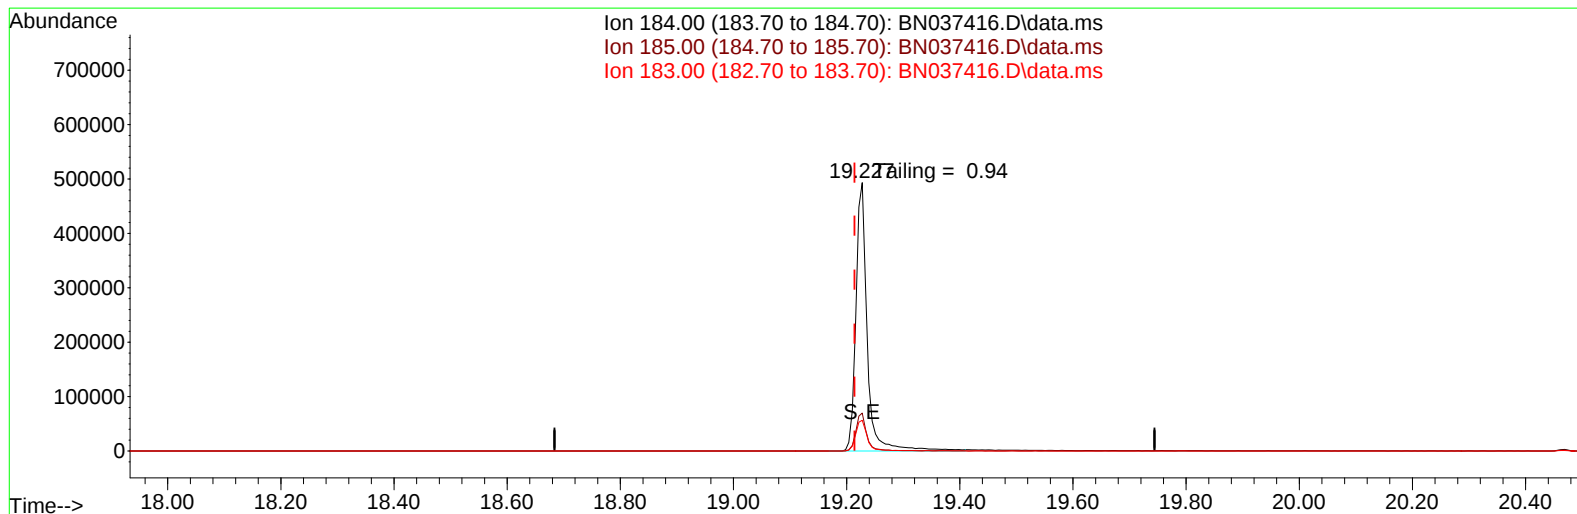

TIC: BN037416.D\data.ms

(77) Benzidine

19.227min (+ 0.013) 0.00 ng

response 690171

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/27/2025	BNA_N	<u>BN037416.D</u>
Compound Name	Response	Retention Time
DDT	549318	20.469
DDD	13683	20.027
DDE	2707	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16390	565708	2.90

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP