
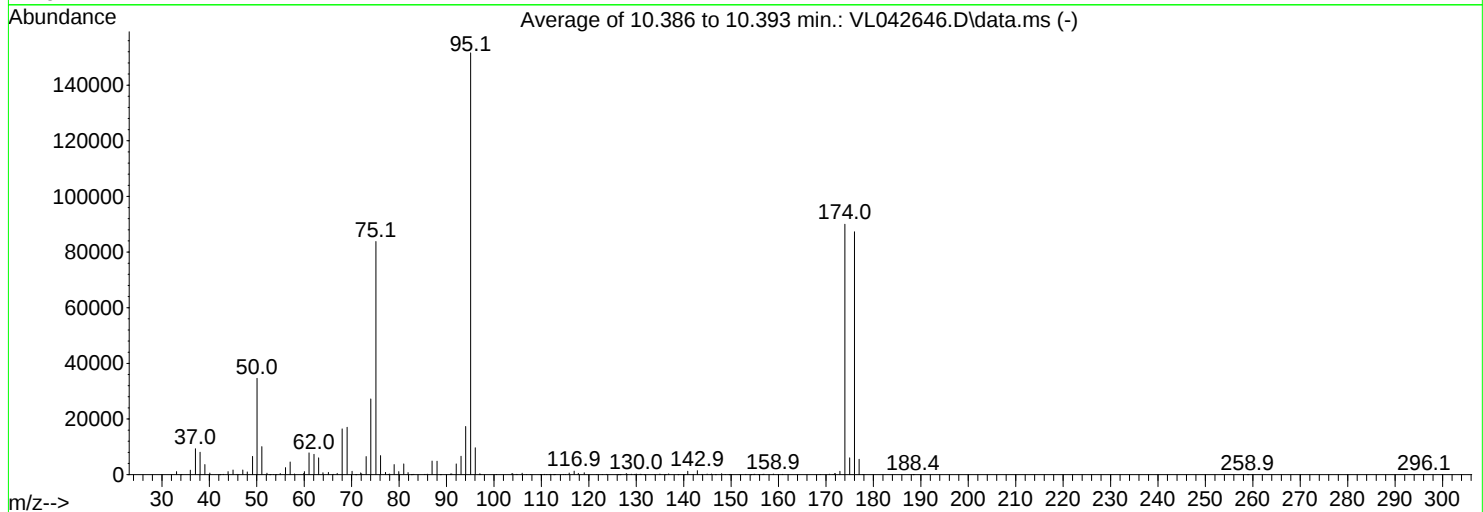


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL061925\
Data File : VL042646.D
Acq On : 19 Jun 2025 08:10
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL052925AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri May 30 02:01:56 2025

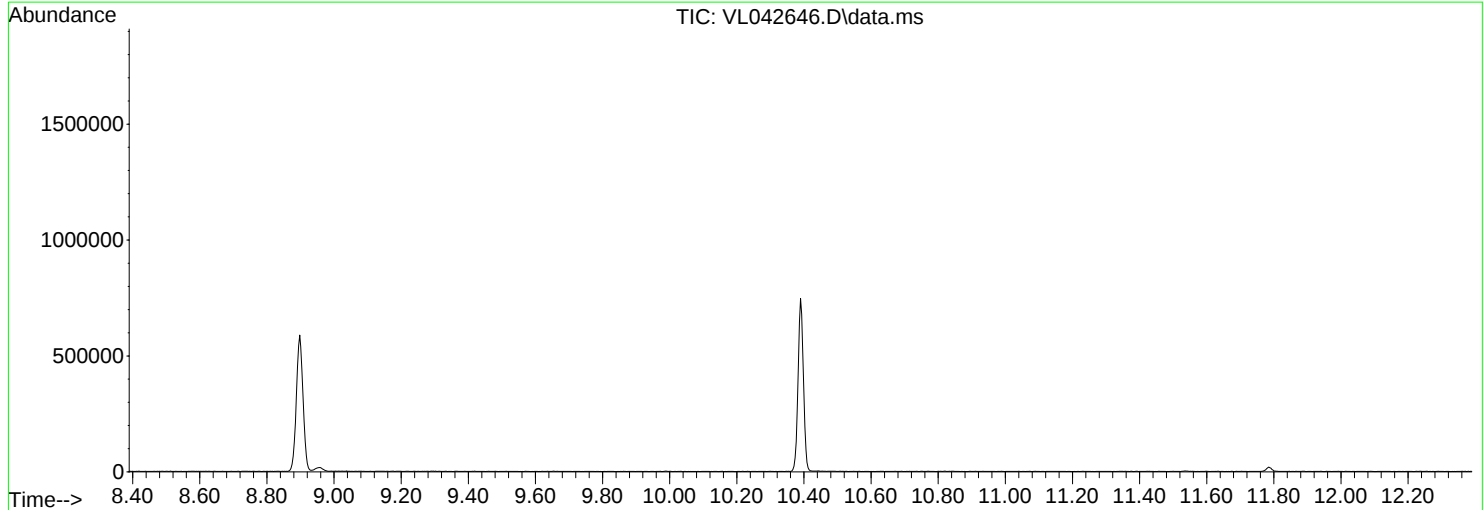

AutoFind: Scans 3182, 3183, 3184; Background Corrected with Scan 3159

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	22.8	34621	PASS
75	95	30	66	55.3	83795	PASS
95	95	100	100	100.0	151616	PASS
96	95	5	9	6.4	9668	PASS
173	174	0.00	2	1.3	1201	PASS
174	95	50	120	59.4	90011	PASS
175	174	4	9	6.7	6045	PASS
176	174	93	101	97.0	87299	PASS
177	176	5	9	6.3	5534	PASS

Average of 10.386 to 10.393 min.: VL042646.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1122	45.85	98	54.00	17	65.10	80
34.00	29	46.20	72	54.95	378	66.10	11
36.00	1599	47.05	1666	56.05	2524	66.95	48
37.05	9321	48.00	962	57.05	4546	68.00	1645
38.05	8036	49.10	6571	57.95	233	69.05	17042
39.05	3601	50.05	34621	59.90	418	70.10	1196
40.10	553	51.05	10079	60.05	1094	70.85	25
42.20	30	52.15	530	61.00	7816	71.90	611
42.95	104	52.70	25	62.05	7313	72.10	311
43.95	1103	53.00	82	63.05	6070	73.05	6496
45.00	1671	53.55	46	63.95	709	74.05	27232

Average of 10.386 to 10.393 min.: VL042646.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	83795	85.45	121	96.05	9668	109.80	18
76.10	6864	85.95	199	97.00	279	110.65	137
77.15	818	86.95	4911	97.20	155	111.15	70
77.70	112	88.00	4830	100.50	52	111.80	56
78.00	243	88.70	31	103.80	345	111.95	106
78.95	3634	90.85	249	103.95	335	112.60	28
79.95	1101	91.10	297	104.70	119	112.95	80
81.00	3837	92.05	3843	104.90	81	114.65	60
81.90	769	93.05	6644	105.95	517	115.05	81
82.60	22	94.05	17330	106.90	66	115.85	598
83.10	102	95.10	151616	107.70	63	116.90	1262

Average of 10.386 to 10.393 min.: VL042646.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.80	448	130.00	228	142.00	117	150.10	41
119.05	699	130.85	175	142.90	1460	151.90	82
121.70	49	131.05	128	143.85	122	153.10	112
122.85	57	131.70	17	144.95	213	154.20	18
123.80	127	133.90	58	145.60	67	154.80	136
126.20	30	135.00	249	145.90	259	155.00	195
126.60	22	136.10	21	146.70	23	155.80	17
127.90	416	136.85	280	148.00	327	156.70	106
128.10	102	138.80	18	148.75	94	156.90	178
128.95	198	140.10	28	149.60	25	158.90	229
129.70	148	140.85	1236	149.80	134	160.85	120

Average of 10.386 to 10.393 min.: VL042646.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
168.80	63	177.95	80				
170.70	185	188.40	19				
171.50	58	258.90	18				
171.80	321	296.15	48				
172.00	366						
172.95	1201						
174.00	90011						
175.00	6045						
176.00	87299						
177.00	5534						
177.80	79						