


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN062025\
Data File : VN087121.D
Acq On : 20 Jun 2025 08:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

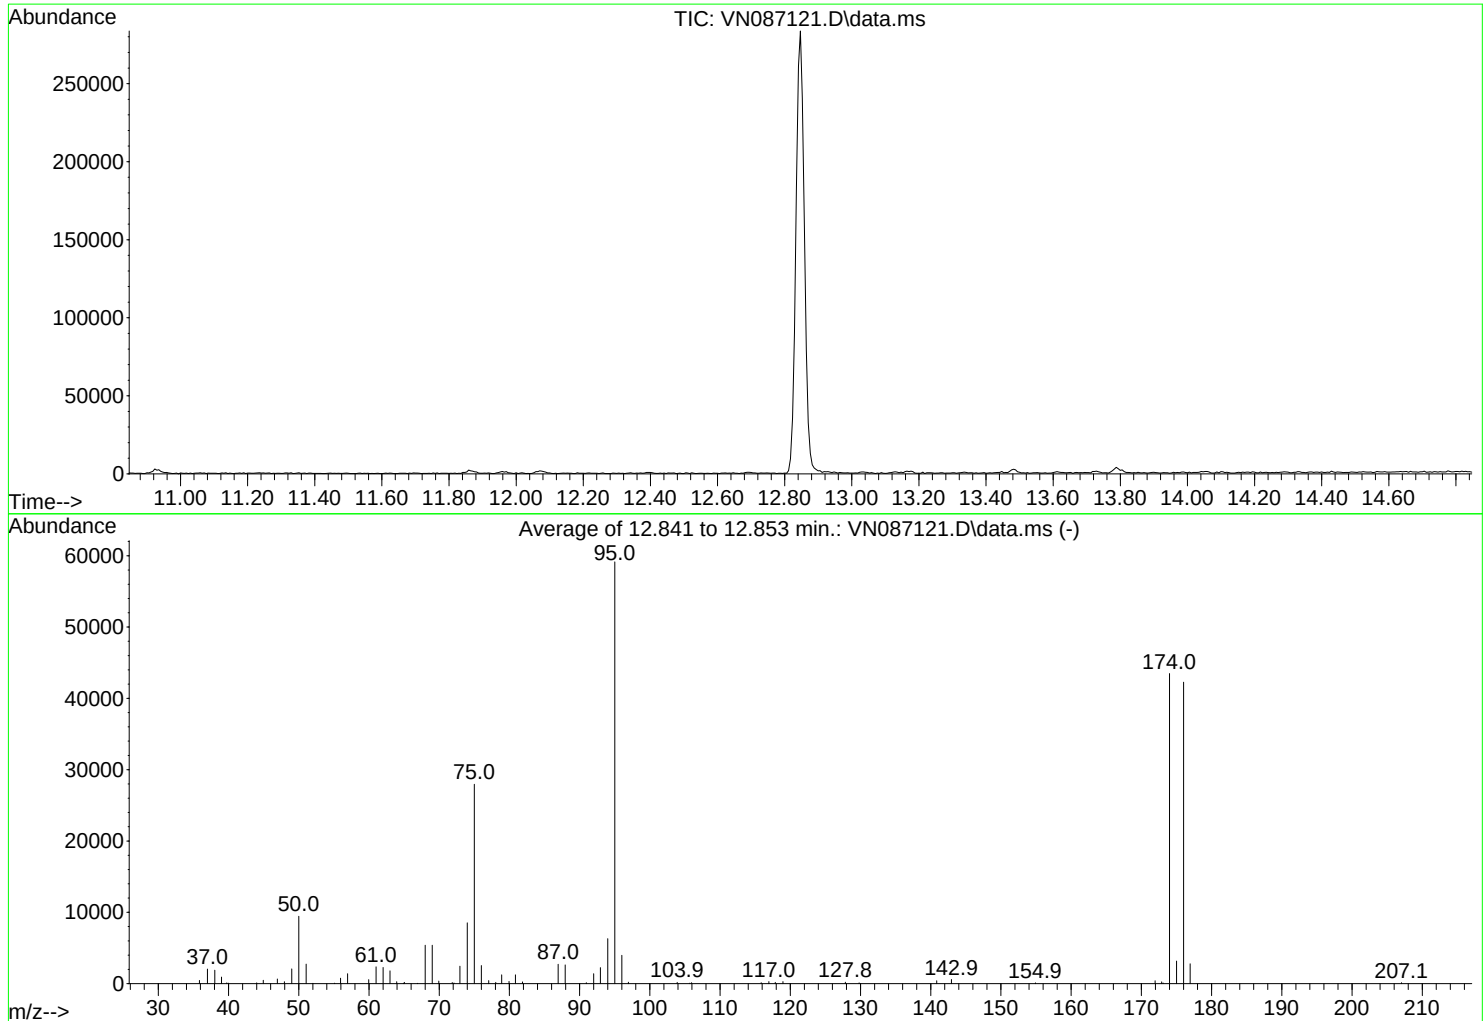

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	9438	PASS
75	95	30	60	47.3	27960	PASS
95	95	100	100	100.0	59141	PASS
96	95	5	9	6.7	3965	PASS
173	174	0.00	2	0.5	238	PASS
174	95	50	100	73.5	43488	PASS
175	174	5	9	7.3	3167	PASS
176	174	95	101	97.2	42269	PASS
177	176	5	9	6.6	2789	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	450	50.00	9438	64.90	64	76.00	253
37.00	2045	51.05	2741	65.05	184	77.05	41
38.05	1874	52.00	54	66.90	51	78.05	18
39.00	912	55.10	61	68.00	5395	78.90	122
39.75	120	55.95	755	69.00	5381	79.95	323
40.00	68	56.95	1392	69.95	358	80.85	1225
44.00	118	59.95	554	71.85	160	81.85	239
44.95	468	61.00	2362	72.10	87	86.95	2709
46.95	662	62.00	2266	72.95	2455	87.95	2619
47.95	268	63.00	1786	74.00	8525	90.95	137
49.00	2057	63.95	270	75.00	27960	92.00	1398

Average of 12.841 to 12.853 min.: VN087121.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	2246	118.95	283	176.00	42269		
94.00	6313	127.85	197	176.95	2789		
95.00	59141	129.80	111	207.05	135		
96.00	3965	140.85	400				
96.95	204	142.95	586				
103.90	180	154.90	108				
105.70	72	171.95	407				
105.95	127	172.90	238				
115.85	137	173.10	95				
116.95	286	174.00	43488				
117.85	171	175.00	3167				

Instrument :

MSVOA_N

ClientSampleId :

BFB