

SOP ID: M3510C,3580A-Extraction SVOC-21

Clean Up SOP #: N/A

Matrix : Water

Welgh By: N/A **Extraction By:** RS

Balance check: N/A **Filter By:** RJ

Balance ID: N/A **pH Meter ID:** N/A

pH Strlp Lot#: E3880 **Hood ID:** 4,6,7

Extraction Method: ☒ Seperatory Funnel ☐ Continious Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☐ Soxhlet

Extraction Start Date : 06/24/2025

Extraction Start Time : 08:39

Extraction End Date : 06/24/2025

Extraction End Time : 13:35

Concentration By: EH

Supervisor By : RUPESH

Standared Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	50/100 PPM	SP6794
Surrogate	1.0ML	100/150 PPM	SP6754
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3943
Baked Na2SO4	N/A	EP2622
H2SO4 1:1	N/A	EP2610
10N NaoH	N/A	EP2609
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

pH Adjusted to < 2 with 1:1 H2SO4 & >12 with 10N NaOH , 1.5ML Vial Lot # 2210443.

KD Bath ID: WATER BATH-1,2 **Envap ID:** NE VAP-02


KD Bath Temperature: 60 °C **Envap Temperature:** 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
6/24/25	RS (Ext Lab)	RLSVOC
13:40	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction SVOC-21

Concentration Date: 06/24/2025

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB168592BL	SBLK592	SVOC-TCL BNA -20	1000	6	RUPESH	ritesh	1			SEP-1
PB168592BS	SLCS592	SVOC-TCL BNA -20	1000	6	RUPESH	ritesh	1			2
PB168592BS D	SLCSD592	SVOC-TCL BNA -20	1000	6	RUPESH	ritesh	1			3
Q2372-01	GAV1W	SVOCMS Group2	980	6	RUPESH	ritesh	1	D		4
Q2385-01	A5311	SVOC-TCL BNA -20	1000	6	RUPESH	ritesh	1	N		5

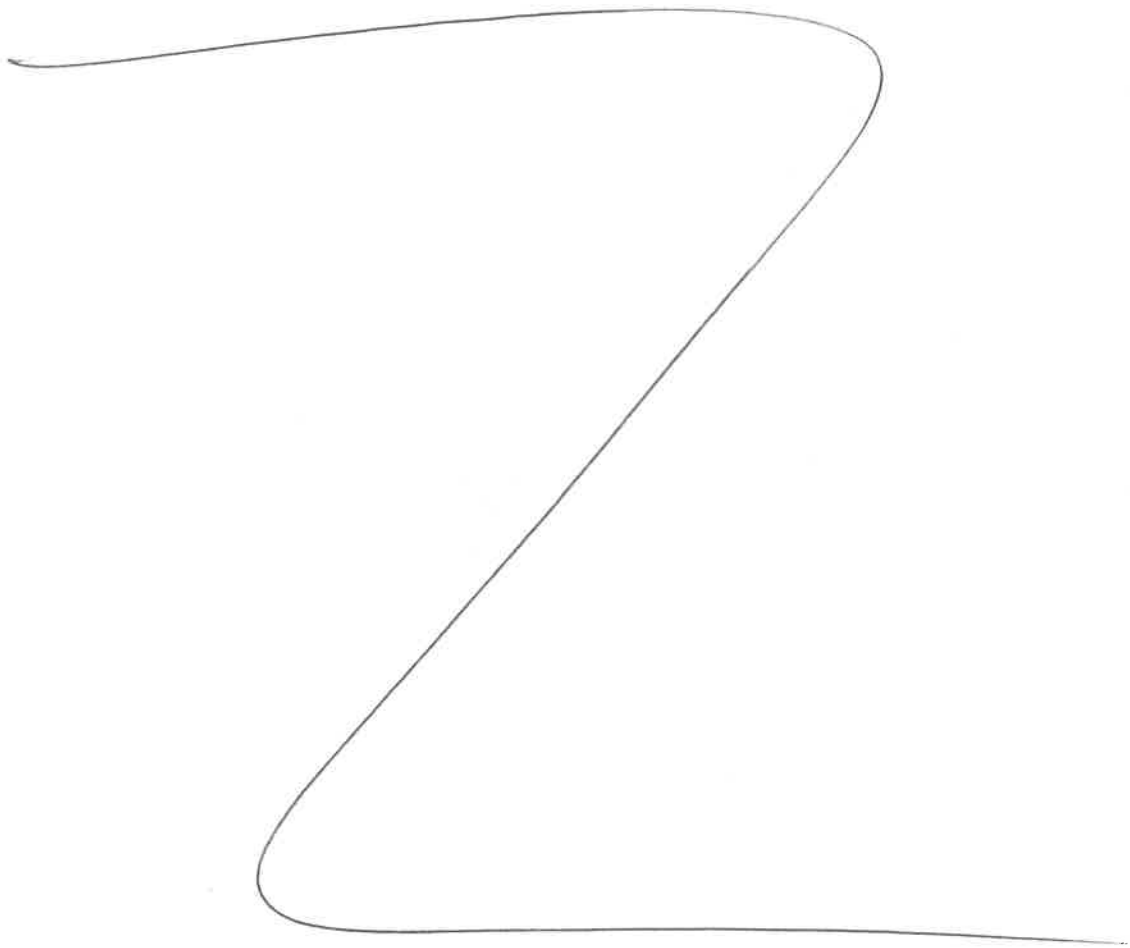

RS
6/24