


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037402.D
Acq On : 26 Jun 2025 20:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 26 16:06:33 2025

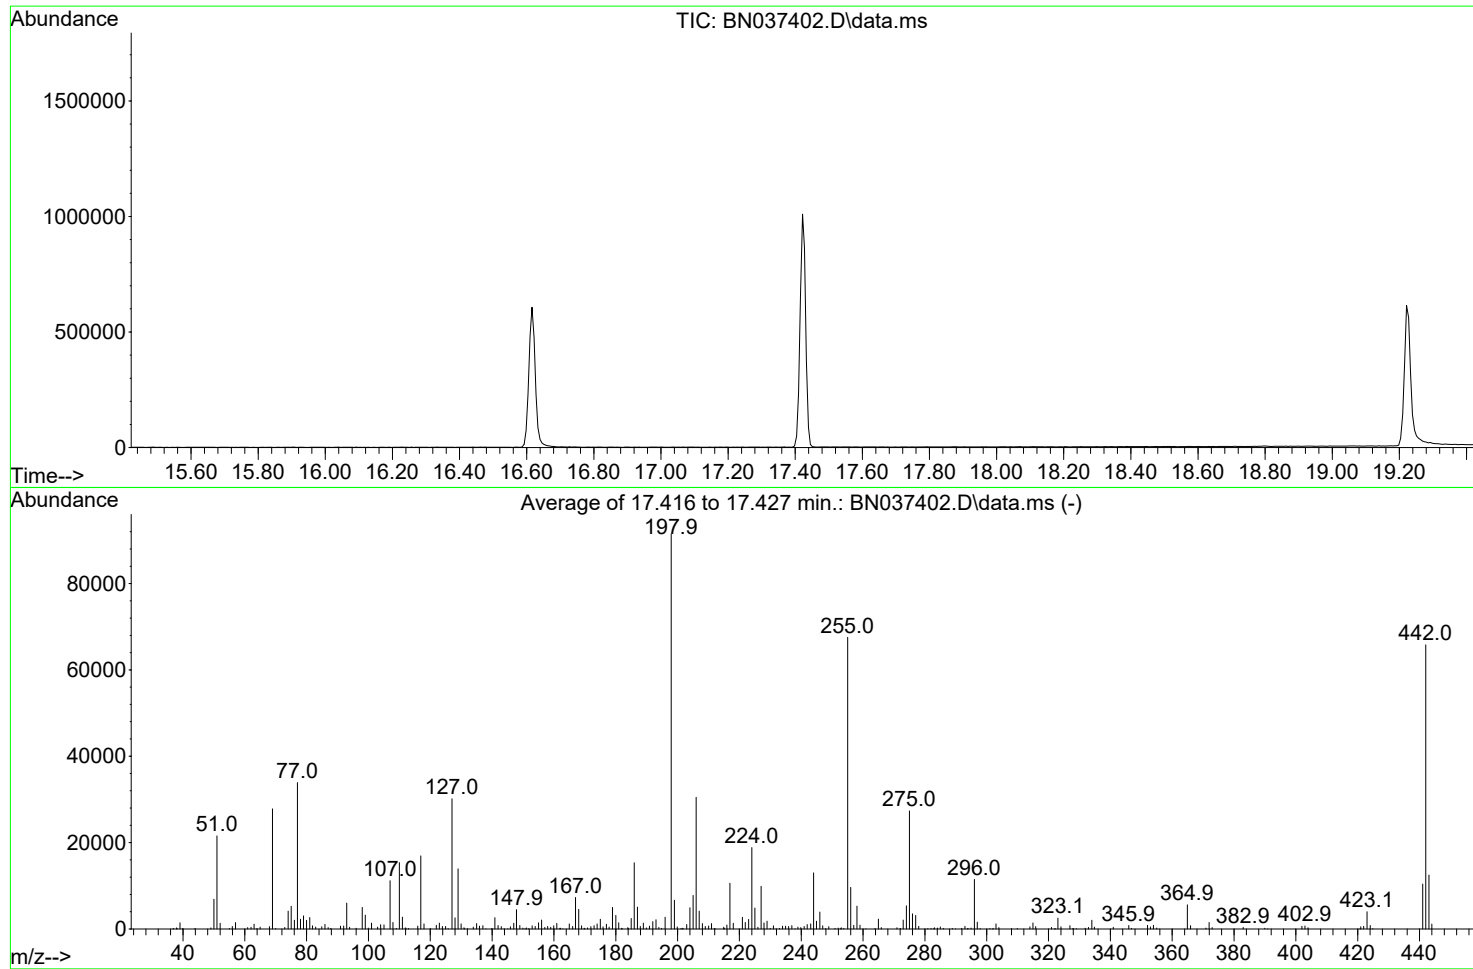

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	567	PASS
69	69	100	100	100.0	27835	PASS
70	69	0.00	2	0.5	131	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91421	PASS
199	198	5	9	7.3	6679	PASS
365	198	1	100	6.1	5585	PASS
441	443	0.01	150	83.2	10396	PASS
442	442	100	100	100.0	65797	PASS
443	442	15	24	19.0	12501	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/26/2025	BNA_N	<u>BN037402.D</u>
Compound Name	Response	Retention Time
DDT	341583	20.463
DDD	4324	20.074
DDE	90	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4414	345997	1.28

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037402.D
Acq On : 26 Jun 2025 20:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 04:09:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

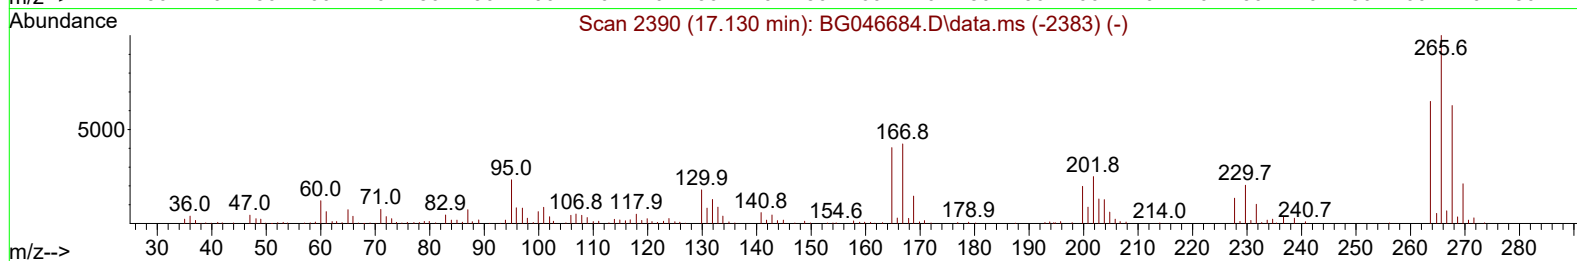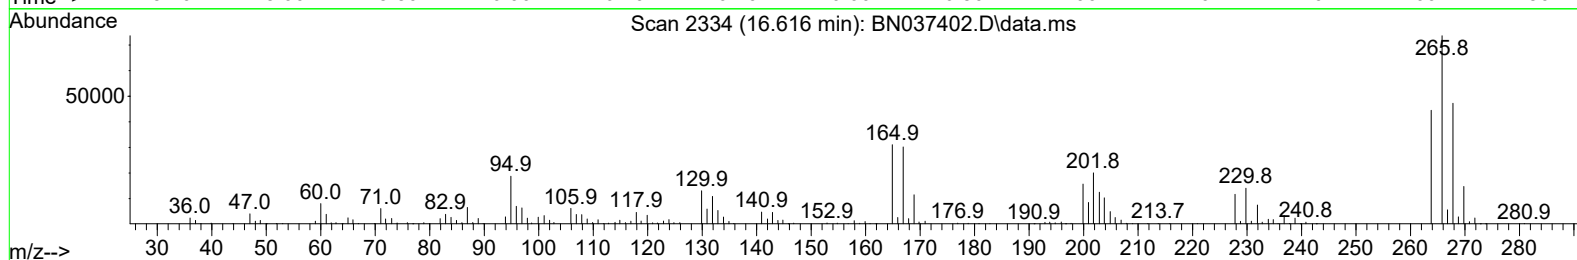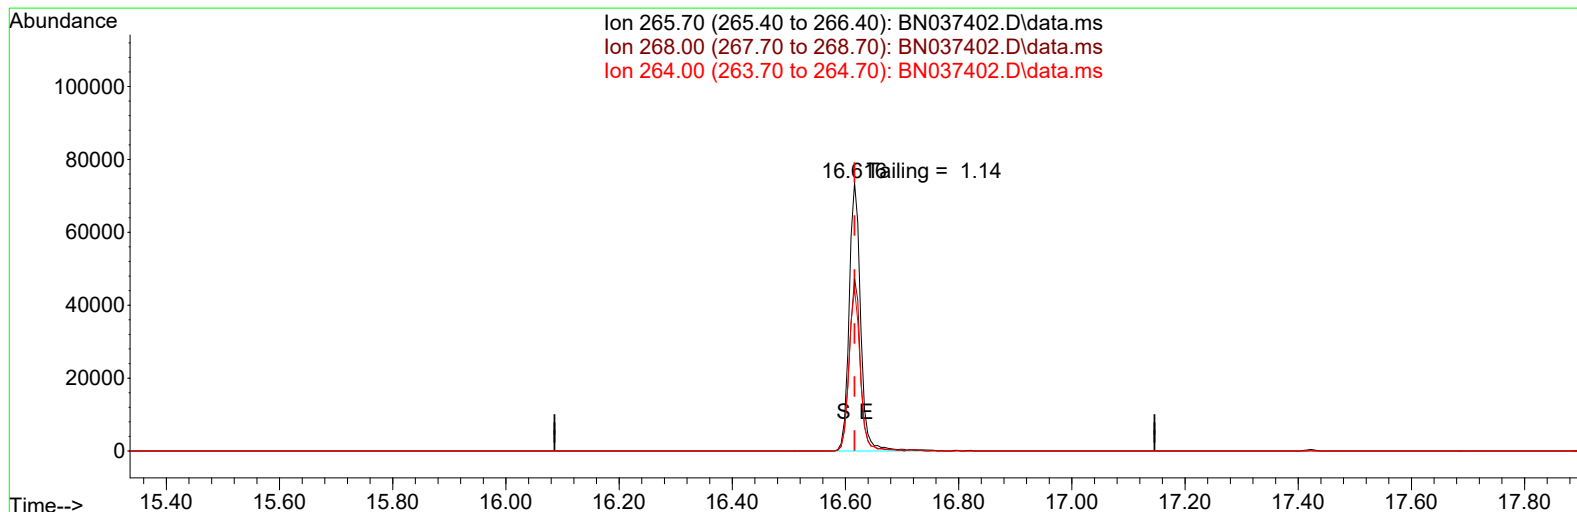

TIC: BN037402.D\data.ms

(70) Pentachlorophenol (C)

16.616min (0.000) 18260.25 ng




response 103034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	60.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037402.D
Acq On : 26 Jun 2025 20:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 04:09:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

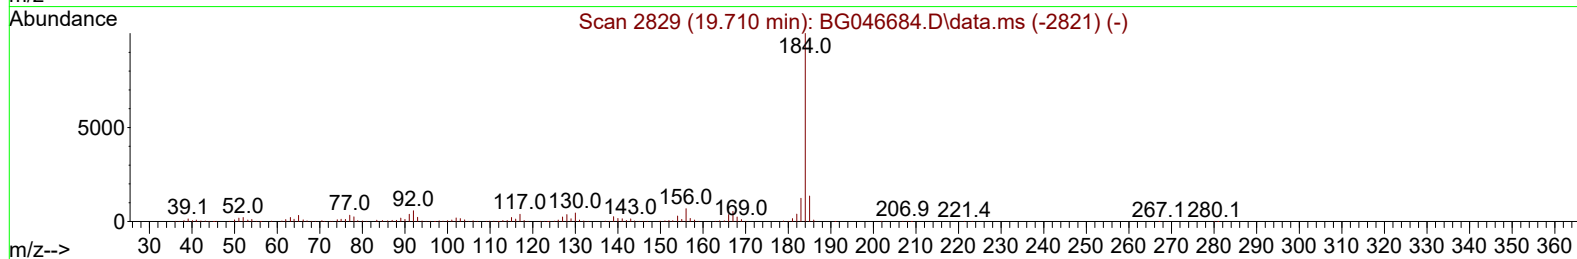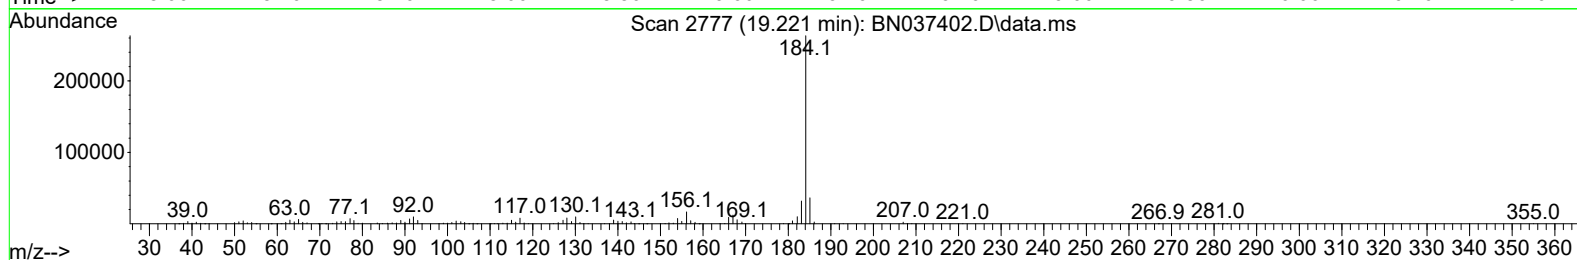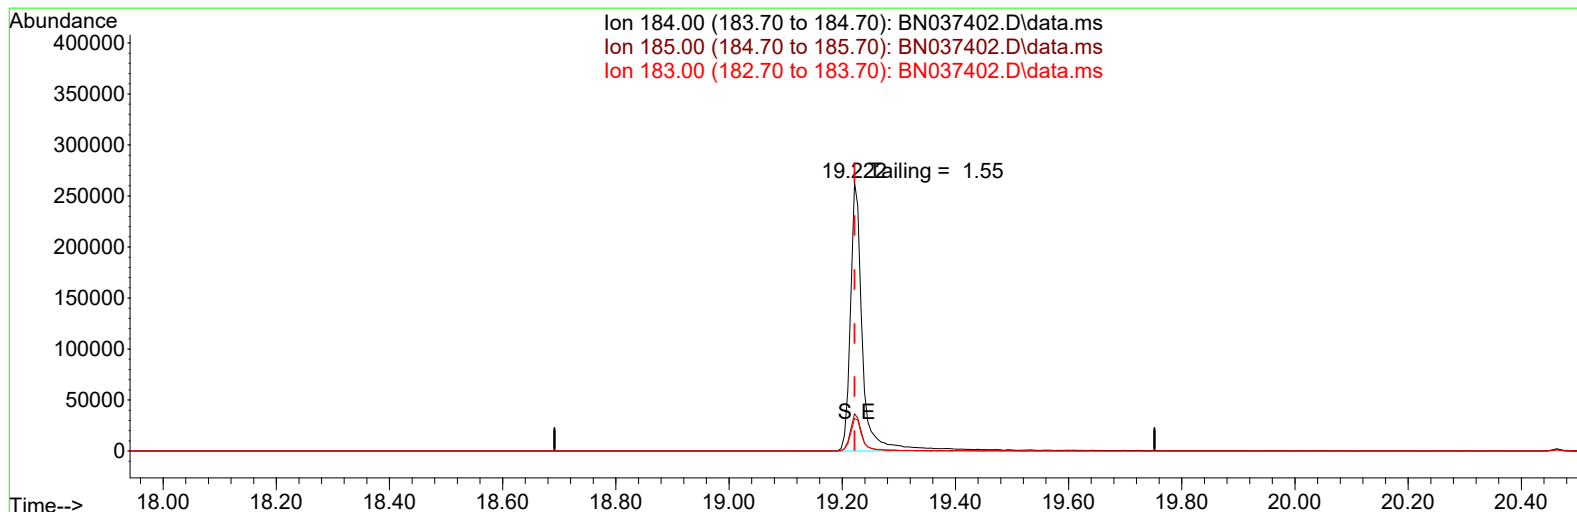

TIC: BN037402.D\data.ms

(77) Benzidine

19.221min (0.000) 0.00 ng

response 385080

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	12.12
0.00	0.00	0.00