

**DATA PACKAGE  
SEMI-VOLATILE ORGANICS**

**PROJECT NAME : NWIRP BETHPAGE 112G08005-WE13**

**TETRA TECH NUS, INC.  
661 Andersen Drive  
Suite 200  
Pittsburgh, PA - 15220-2745  
Phone No: 412-921-7090**

**ORDER ID : Q2375  
ATTENTION : Ernie Wu**



**Laboratory Certification ID # 20012**

<b>1) SEMI-VOLATILE DATA</b>	<b>2</b>
<b>2) Signature Page</b>	<b>4</b>
<b>3) Case Narrative</b>	<b>5</b>
<b>4) Qualifier Page</b>	<b>7</b>
<b>5) Conformance/Non Conformance</b>	<b>8</b>
<b>6) QA Checklist</b>	<b>10</b>
<b>7) Chronicle</b>	<b>11</b>
<b>8) Hit Summary</b>	<b>12</b>
<b>9) QC Data Summary For SVOC-SIMGroup1</b>	<b>13</b>
<b>9.1) Deuterated Monitoring Compound Summary</b>	<b>14</b>
<b>9.2) LCS/LCSD Summary</b>	<b>15</b>
<b>9.3) Method Blank Summary</b>	<b>17</b>
<b>9.4) GS/MS Tune Summary</b>	<b>18</b>
<b>9.5) Internal Standard Area and RT Summary</b>	<b>21</b>
<b>10) Sample Data</b>	<b>25</b>
<b>10.1) RW8-SP100-20250619</b>	<b>26</b>
<b>10.2) RW8-SP303-20250619</b>	<b>37</b>
<b>11) Calibration Data Summary</b>	<b>48</b>
<b>11.1) Initial Calibration Data</b>	<b>3</b>
<b>11.1.1) BN062125</b>	<b>49</b>
<b>11.1.2) BN062625</b>	<b>234</b>
<b>11.2) Continued Calibration Data</b>	<b>419</b>
<b>11.2.1) BN037365.D</b>	<b>419</b>
<b>11.2.2) BN037403.D</b>	<b>445</b>
<b>11.2.3) BN037415.D</b>	<b>471</b>
<b>12) QC Sample Data</b>	<b>497</b>
<b>12.1) Tune Raw Data</b>	<b>498</b>
<b>12.2) Method Blank Data</b>	<b>510</b>
<b>12.3) LCS Data</b>	<b>520</b>
<b>12.4) LCSD Data</b>	<b>544</b>
<b>13) Manual Integration</b>	<b>568</b>
<b>14) Analytical Runlogs</b>	<b>570</b>
<b>15) Extraction Logs</b>	<b>576</b>
<b>15.1) PB168563.pdf</b>	<b>576</b>
<b>15.2) PB168563IC.pdf</b>	<b>578</b>

## Table Of Contents for Q2375

<b>16) Standard Prep Logs</b>	580	1
<b>17) Shipping Document</b>	650	2
<b>17.1) Chain Of Custody</b>	651	3
<b>17.2) Lab Certificate</b>	652	4
<b>18) Not Reviewed Data</b>	653	5
		6
		7
		8
		9
		10
		11
		12
		13
		14
		15
		16
		17
		18

## Cover Page

**Order ID :** Q2375

**Project ID :** NWIRP Bethpage 112G08005-WE13

**Client :** Tetra Tech NUS, Inc.

**Lab Sample Number**

Q2375-01  
Q2375-02

**Client Sample Number**

RW8-SP100-20250619  
RW8-SP303-20250619

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : \_\_\_\_\_

Date: 6/30/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

## CASE NARRATIVE

**Tetra Tech NUS, Inc.**

**Project Name:** NWIRP Bethpage 112G08005-WE13

**Project Manager #** Ernie Wu

**Order ID #** Q2375

**Test Name:** SVOC-SIMGroup1

**A. Number of Samples and Date of Receipt:**

2 Water samples were received on 06/19/2025.

**B. Parameters**

According to the Chain of Custody document, the following analyses were requested:  
Metals Group4, SVOC-SIMGroup1, TDS and TSS. This data package contains results for  
SVOC-SIMGroup1.

**C. Analytical Techniques:**

The samples were analyzed on instrument BNA\_N using GC Column ZB-SemiVolatiles  
Guardian which is 30 meters, 0.25 mm ID, 0.5 um df, Catalog # 7HG-G027-17-GGAThe  
analysis of SVOC-SIMGroup1 was based on method 8270-Modified and extraction was  
done based on method 3510.

**D. QA/ QC Samples:**

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria.

The Internal Standards Areas met the acceptable requirements.

The Retention Times were acceptable for all samples.

The RPD met criteria .

The Blank Spike met requirements for all samples .

The Blank Spike Duplicate met requirements for all samples .

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements .

The Continuous Calibration File ID BN037403.D met the requirements except for 2,4,6-Tribromophenol ,The Failure Surrogate is not Associated with DOD Parameter list,Therefore no Corrective Action was taken.

The Tuning criteria met requirements.

**E. Additional Comments:**

The laboratory certifies that the all-electronic diskette deliverable exactly match the data summary forms (i.e. Form Is)."

The Form 6 is not included in the data package because the Initial Calibration was performed using 7 points.

The Sample #RW8-SP100-20250619 have the concentration of target compound below Method detection limits, therefore it is not reported as Hit in Form1.



284 Sheffield Street, Mountainside, NJ 07092  
Phone: 908 789 8900 Fax: 908 789 8922

The not QT review data is reported in the Miscellaneous.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

**F. Manual Integration Comments:**

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

---

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature \_\_\_\_\_

**DATA REPORTING QUALIFIERS- ORGANIC**

For reporting results, the following "Results Qualifiers" are used:

- Value** If the result is a value greater than or equal to the detection limit, report the value
- U** Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
- ND** Indicates the analyte was analyzed for, but not detected
- J** Indicates an estimated value. This flag is used:  
(1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.)  
(2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
- B** Indicates the analyte was found in the blank as well as the sample report as "12 B".
- E** Indicates the analyte's concentration exceeds the calibrated range of the instrument for that specific analysis.
- D** This flag identifies all compounds identified in an analysis at a secondary dilution factor.
- P** This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
- N** This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
- A** This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
- Q** Indicates the LCS did not meet the control limits requirements

# **ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092**

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

## **GC/MS SEMI-VOLATILE ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY**

ORDER ID: Q2375

MATRIX: Water

METHOD: 8270-Modified/3510

	NA	NO	YES
1. Chromatograms Labeled/Compounds Identified. (Field samples and Method Blanks)			✓
2. GC/MS Tuning Specifications. DFTPP Meet Criteria. (NOTE THAT THERE ARE DIFFERENT CRITERIA FOR NY ASP CLP, CLP AND NJ)			✓
3. GC/MS Tuning Frequency - Performed every 24 hours for 600 series and 12 hours for 8000 Series.			✓
4. GC/MS Calibration - Initial Calibration performed within 30 days before sample analysis and continuing calibration performed within 24 hours of sample analysis for 600 series and 12 hours for 8000 series.			✓
5. GC/MS Calibration Requirements.			✓

The Initial Calibration met the requirements .

The Continuous Calibration File ID BN037403.D met the requirements except for 2,4,6-Tribromophenol ,The Failure Surrogate is not Associated with DOD Parameter list,Therefore no Corrective Action was taken.

6. Blank Contamination - If yes, list compounds and concentrations in each blank:	✓
7. Surrogate Recoveries Meet Criteria	✓

If not met, list those compounds and their recoveries which fall outside the acceptable ranges.

8. Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria	✓
If not met, list those compounds and their recoveries which fall outside the acceptable range.	

The Blank Spike met requirements for all samples .

The Blank Spike Duplicate met requirements for all samples .

9. Internal Standard Area/Retention Time Shift Meet Criteria	✓
Comments:	

10. Extraction Holding Time Met	✓
If not met, list number of days exceeded for each sample:	

**ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092**

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

**GC/MS SEMI-VOLATILE ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY****(CONTINUED)**

NA      NO      YES

11. Analysis Holding Time Met
- ✓

If not met, list number of days exceeded for each sample:

**ADDITIONAL COMMENTS:**

The laboratory certifies that the all-electronic diskette deliverable exactly match the data summary forms (i.e. Form Is.) The Form 6 is not included in the data package because the Initial Calibration was performed using 7 points. The Sample #RW8-SP100-20250619 have the concentration of target compound below Method detection limits, therefore it is not reported as Hit in Form1.

The not QT review data is reported in the Miscellaneous.

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the % RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

---

QA REVIEW

---

Date

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18

## APPENDIX A

### QA REVIEW GENERAL DOCUMENTATION

Project #: Q2375

Completed

For thorough review, the report must have the following:

#### GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page) ✓

Check chain-of-custody for proper relinquish/return of samples ✓

Is the chain of custody signed and complete ✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts ✓

Collect information for each project id from server. Were all requirements followed ✓

#### COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page ✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody ✓

#### CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results ✓

Do requested analyses on Chain of Custody agree with the log-in page ✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody ✓

Were the samples received within hold time ✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle ✓

#### ANALYTICAL:

Was method requirement followed? ✓

Was client requirement followed? ✓

Does the case narrative summarize all QC failure? ✓

All runlogs and manual integration are reviewed for requirements ✓

All manual calculations and /or hand notations verified ✓

QA Review Signature: MOHAMMAD AHMED

Date: 06/30/2025

## LAB CHRONICLE

<b>OrderID:</b>	Q2375	<b>OrderDate:</b>	6/19/2025 3:57:00 PM					
<b>Client:</b>	Tetra Tech NUS, Inc.	<b>Project:</b>	NWIRP Bethpage 112G08005-WE13					
<b>Contact:</b>	Ernie Wu	<b>Location:</b>	D51					
<hr/>								
LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2375-01	RW8-SP100-2025061 9	Water			<b>06/19/25</b>			<b>06/19/25</b>
			SVOC-SIMGroup1	8270-Modified		06/20/25	06/27/25	
Q2375-02	RW8-SP303-2025061 9	Water			<b>06/19/25</b>			<b>06/19/25</b>
			SVOC-SIMGroup1	8270-Modified		06/20/25	06/27/25	

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

**Hit Summary Sheet**  
**SW-846**

**SDG No.:** Q2375  
**Client:** Tetra Tech NUS, Inc.

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	LOD	RDL	Units
Client ID :				0.000					
			Total Svoc :	0.00					
			Total Concentration:	0.00					



# QC SUMMARY

### Surrogate Summary

SW-846

SDG No.: Q2375

Client: Tetra Tech NUS, Inc.

Analytical Method: 8270-Modified

Lab Sample ID	Client ID	Parameter	Spike (PPM)	Result (PPM)	Recovery (%)	Qual	Limits (%)	
							Low	High
PB168563BL	PB168563BL	2-Methylnaphthalene-d10	0.4	0.32	81		30	150
		Fluoranthene-d10	0.4	0.37	93		30	150
		Nitrobenzene-d5	0.4	0.30	75		55	111
		2-Fluorobiphenyl	0.4	0.33	81		53	106
		Terphenyl-d14	0.4	0.37	93		58	132
PB168563BS	PB168563BS	2-Methylnaphthalene-d10	0.4	0.49	123		30	150
		Fluoranthene-d10	0.4	0.35	86		30	150
		Nitrobenzene-d5	0.4	0.37	92		55	111
		2-Fluorobiphenyl	0.4	0.39	97		53	106
		Terphenyl-d14	0.4	0.39	98		58	132
PB168563BSD	PB168563BSD	2-Methylnaphthalene-d10	0.4	0.39	97		30	150
		Fluoranthene-d10	0.4	0.35	86		30	150
		Nitrobenzene-d5	0.4	0.39	97		55	111
		2-Fluorobiphenyl	0.4	0.40	99		53	106
		Terphenyl-d14	0.4	0.38	94		58	132
Q2375-01	RW8-SP100-20250619	2-Methylnaphthalene-d10	0.4	0.32	81		30	150
		Fluoranthene-d10	0.4	0.40	100		30	150
		Nitrobenzene-d5	0.4	0.28	69		55	111
		2-Fluorobiphenyl	0.4	0.33	81		53	106
		Terphenyl-d14	0.4	0.45	112		58	132
Q2375-02	RW8-SP303-20250619	2-Methylnaphthalene-d10	0.4	0.35	88		30	150
		Fluoranthene-d10	0.4	0.39	98		30	150
		Nitrobenzene-d5	0.4	0.28	71		55	111
		2-Fluorobiphenyl	0.4	0.35	88		53	106
		Terphenyl-d14	0.4	0.46	116		58	132

### Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2375

Client: Tetra Tech NUS, Inc.

Analytical Method: 8270-Modified DataFile: BN037363.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Qual	Limits		RPD
									Low	High	
PB168563BS	1,4-Dioxane	0.4	0.32	ug/L	80				70	130	

### Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2375

Client: Tetra Tech NUS, Inc.

Analytical Method: 8270-Modified DataFile: BN037364.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Qual	Limits		RPD
									Low	High	
PB168563BSD	1,4-Dioxane	0.4	0.30	ug/L	75	6			70	130	20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

4B

SEMIVOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB168563BL

Lab Name: CHEMTECH

Contract: TETR06

Lab Code: CHEM Case No.: Q2375

SAS No.: Q2375 SDG NO.: Q2375

Lab File ID: BN037361.D

Lab Sample ID: PB168563BL

Instrument ID: BNA\_N

Date Extracted: 06/20/2025

Matrix: (soil/water) Water

Date Analyzed: 06/20/2025

Level: (low/med) LOW

Time Analyzed: 22:16

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
PB168563BS	PB168563BS	BN037363.D	06/20/2025
PB168563BSD	PB168563BSD	BN037364.D	06/21/2025
RW8-SP100-20250619	Q2375-01	BN037413.D	06/27/2025
RW8-SP303-20250619	Q2375-02	BN037414.D	06/27/2025

COMMENTS:



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

5B

SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: CHEMTECHContract: TETR06Lab Code: CHEMSAS No.: Q2375 SDG No.: Q2375Lab File ID: BN037351.DDFTPP Injection Date: 06/20/2025Instrument ID: BNA\_NDFTPP Injection Time: 15:00

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
68	Less than 2.0% of mass 69	0.0 ( 0.0 ) 1
69	Mass 69 relative abundance	100
70	Less than 2.0% of mass 69	0.2 ( 0.7 ) 1
197	Less than 2.0% of mass 198	0.0
198	Base Peak, 100% relative abundance	100
199	5.0 to 9.0% of mass 198	6.8
365	Greater than 1% of mass 198	4.9
441	Present, but less than mass 443	85.2
442	Greater than 50% of mass 198	100
443	15.0 - 24.0% of mass 442	16.4 ( 20 ) 2

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
SSTDICC0.1	SSTDICC0.1	BN037353.D	06/20/2025	16:51
SSTDICC0.2	SSTDICC0.2	BN037354.D	06/20/2025	17:27
SSTDICCC0.4	SSTDICCC0.4	BN037355.D	06/20/2025	18:03
SSTDICC0.8	SSTDICC0.8	BN037356.D	06/20/2025	18:39
SSTDICC1.6	SSTDICC1.6	BN037357.D	06/20/2025	19:15
SSTDICC3.2	SSTDICC3.2	BN037358.D	06/20/2025	19:51
SSTDICC5.0	SSTDICC5.0	BN037359.D	06/20/2025	20:27
PB168563BL	PB168563BL	BN037361.D	06/20/2025	22:16
PB168563BS	PB168563BS	BN037363.D	06/20/2025	23:28
PB168563BSD	PB168563BSD	BN037364.D	06/21/2025	00:04
SSTDCCC0.4EC	SSTDCCC0.4	BN037365.D	06/21/2025	01:17



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

5B

SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: CHEMTECH

Contract: TETR06

Lab Code: CHEM

SAS No.: Q2375 SDG NO.: Q2375

Lab File ID: BN037385.D

DFTPP Injection Date: 06/26/2025

Instrument ID: BNA\_N

DFTPP Injection Time: 10:01

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
68	Less than 2.0% of mass 69	0.3 ( 0.9 ) 1
69	Mass 69 relative abundance	100
70	Less than 2.0% of mass 69	0.2 ( 0.6 ) 1
197	Less than 2.0% of mass 198	0.0
198	Base Peak, 100% relative abundance	100
199	5.0 to 9.0% of mass 198	7.1
365	Greater than 1% of mass 198	4.9
441	Present, but less than mass 443	78.0
442	Greater than 50% of mass 198	100
443	15.0 - 24.0% of mass 442	14.1 (18.8) 2

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
SSTDICC0.1	SSTDICC0.1	BN037386.D	06/26/2025	10:41
SSTDICC0.2	SSTDICC0.2	BN037387.D	06/26/2025	11:17
SSTDICCC0.4	SSTDICCC0.4	BN037388.D	06/26/2025	11:53
SSTDICC0.8	SSTDICC0.8	BN037389.D	06/26/2025	12:29
SSTDICC1.6	SSTDICC1.6	BN037390.D	06/26/2025	13:05
SSTDICC3.2	SSTDICC3.2	BN037391.D	06/26/2025	13:41
SSTDICC5.0	SSTDICC5.0	BN037392.D	06/26/2025	14:17



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

5B

SEMIVOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK  
DECAFLUOROTRIPHENYLPHOSPHINE (DFTPP)

Lab Name: CHEMTECH

Contract: TETR06

Lab Code: CHEM

SAS No.: Q2375 SDG NO.: Q2375

Lab File ID: BN037402.D

DFTPP Injection Date: 06/26/2025

Instrument ID: BNA\_N

DFTPP Injection Time: 20:19

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
68	Less than 2.0% of mass 69	0.6 ( 2 ) 1
69	Mass 69 relative abundance	100
70	Less than 2.0% of mass 69	0.1 ( 0.5 ) 1
197	Less than 2.0% of mass 198	0.0
198	Base Peak, 100% relative abundance	100
199	5.0 to 9.0% of mass 198	7.3
365	Greater than 1% of mass 198	6.1
441	Present, but less than mass 443	83.2
442	Greater than 50% of mass 198	100
443	15.0 - 24.0% of mass 442	13.7 ( 19 ) 2

1-Value is % mass 69

2-Value is % mass 442

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
SSTDCCC0.4	SSTDCCC0.4	BN037403.D	06/26/2025	21:38
RW8-SP100-20250619	Q2375-01	BN037413.D	06/27/2025	03:41
RW8-SP303-20250619	Q2375-02	BN037414.D	06/27/2025	04:18
SSTDCCC0.4EC	SSTDCCC0.4	BN037415.D	06/27/2025	04:54



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

8B

SEMOVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH  
Lab Code: CHEM Case No.: Q2375 SAS No.: Q2375 SDG No.: Q2375  
EPA Sample No.: SSTDICCC0.4 Date Analyzed: 06/20/2025  
Lab File ID: BN037355.D Time Analyzed: 18:03  
Instrument ID: BNA\_N GC Column: ZB-GR ID: 0.25 (mm)

	IS1 (DCB) AREA #	RT #	IS2 (NPT) AREA #	RT #	IS3 (ANT) AREA #	RT #
12 HOUR STD	1912	7.568	4157	10.34	2811	14.21
	3824	8.068	8314	10.84	5622	14.713
	956	7.068	2078.5	9.84	1405.5	13.713
EPA SAMPLE NO.						
01 PB168563BL	1968	7.57	4045	10.35	2736	14.22
02 PB168563BS	1960	7.57	4204	10.34	2586	14.21
03 PB168563BSD	1885	7.57	4095	10.34	2623	14.21

IS1 (DCB) = 1,4-Dichlorobenzene-d4

IS2 (NPT) = Naphthalene-d8

IS3 (ANT) = Acenaphthene-d10

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.

8C

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name:	CHEMTECH						
Lab Code:	CHEM	Case No.:	Q2375	SAS No.:	Q2375	SDG NO.:	Q2375
EPA Sample No.:	SSTDICCC0.4		Date Analyzed:	06/20/2025			
Lab File ID:	BN037355.D		Time Analyzed:	18:03			
Instrument ID:	BNA_N		GC Column:	ZB-GR	ID:	0.25 (mm)	

	IS4 (PHN) AREA #	RT #	IS5 (CRY) AREA #	RT #	IS6 (PRY) AREA #	RT #
12 HOUR STD	5776	16.971	4813	21.171	4943	23.354
	11552	17.471	9626	21.671	9886	23.854
	2888	16.471	2406.5	20.671	2471.5	22.854
EPA SAMPLE NO.						
01 PB168563BL	4864	16.98	4288	21.17	3457	23.36
02 PB168563BS	4830	16.97	3875	21.17	2749	23.35
03 PB168563BSD	5035	16.97	4193	21.16	4470	23.35

IS4 (PHN) = Phenanthrene-d10

IS5 (CRY) = Chrysene-d12

IS6 (PRY) = Perylene-d12

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

8B

SEMOVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH  
Lab Code: CHEM Case No.: Q2375 SAS No.: Q2375 SDG NO.: Q2375  
EPA Sample No.: SSTDCCC0.4 Date Analyzed: 06/26/2025  
Lab File ID: BN037403.D Time Analyzed: 21:38  
Instrument ID: BNA\_N GC Column: ZB-GR ID: 0.25 (mm)

	IS1 (DCB) AREA #	RT #	IS2 (NPT) AREA #	RT #	IS3 (ANT) AREA #	RT #
12 HOUR STD	1253	7.56	2741	10.34	1842	14.21
UPPER LIMIT	2506	8.06	5482	10.84	3684	14.713
LOWER LIMIT	626.5	7.06	1370.5	9.84	921	13.713
EPA SAMPLE NO.						
01 RW8-SP100-20250619	1845	7.57	4080	10.34	2805	14.21
02 RW8-SP303-20250619	1773	7.57	3842	10.34	2717	14.21

IS1 (DCB) = 1,4-Dichlorobenzene-d4

IS2 (NPT) = Naphthalene-d8

IS3 (ANT) = Acenaphthene-d10

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.

8C

SEMIVOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name:	CHEMTECH						
Lab Code:	CHEM	Case No.:	Q2375	SAS No.:	Q2375	SDG NO.:	Q2375
EPA Sample No.:	SSTDCCCC0.4		Date Analyzed:	06/26/2025			
Lab File ID:	BN037403.D		Time Analyzed:	21:38			
Instrument ID:	BNA_N		GC Column:	ZB-GR	ID:	0.25 (mm)	

	IS4 (PHN) AREA #	RT #	IS5 (CRY) AREA #	RT #	IS6 (PRY) AREA #	RT #
12 HOUR STD	3978	16.959	3956	21.162	4281	23.342
	7956	17.459	7912	21.662	8562	23.842
	1989	16.459	1978	20.662	2140.5	22.842
EPA SAMPLE NO.						
01 RW8-SP100-20250619	5405	16.97	5167	21.16	5486	23.35
02 RW8-SP303-20250619	5443	16.97	5375	21.16	5619	23.35

IS4 (PHN) = Phenanthrene-d10

IS5 (CRY) = Chrysene-d12

IS6 (PRY) = Perylene-d12

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.

\* Values outside of QC limits.



# SAMPLE

# DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Tetra Tech NUS, Inc.	Date Collected:	06/19/25
Project:	NWIRP Bethpage 112G08005-WE13	Date Received:	06/19/25
Client Sample ID:	RW8-SP100-20250619	SDG No.:	Q2375
Lab Sample ID:	Q2375-01	Matrix:	Water
Analytical Method:	SW8270ESIM	% Solid:	0
Sample Wt/Vol:	990	Units: mL	Final Vol: 1000 uL
Soil Aliquot Vol:		uL	Test: SVOC-SIMGroup1
Extraction Type :		Decanted : N	Level : LOW
Injection Volume :		GPC Factor : 1.0	GPC Cleanup : N PH :
Prep Method :			

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN037413.D	1	06/20/25 12:03	06/27/25 03:41	PB168563

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
123-91-1	1,4-Dioxane	0.20	U	0.070	0.20	0.20	ug/L
<b>SURROGATES</b>							
7297-45-2	2-Methylnaphthalene-d10	0.32		30 - 150		81%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.40		30 - 150		100%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.28		55 - 111		69%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.33		53 - 106		81%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.45		58 - 132		112%	SPK: 0.4
<b>INTERNAL STANDARDS</b>							
3855-82-1	1,4-Dichlorobenzene-d4	1850	7.567				
1146-65-2	Naphthalene-d8	4080	10.34				
15067-26-2	Acenaphthene-d10	2810	14.213				
1517-22-2	Phenanthrene-d10	5410	16.971				
1719-03-5	Chrysene-d12	5170	21.161				
1520-96-3	Perylene-d12	5490	23.345				

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037413.D  
 Acq On : 27 Jun 2025 03:41  
 Operator : RC/JU  
 Sample : Q2375-01  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**RW8-SP100-20250619**

Quant Time: Jun 27 04:38:21 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.567	152	1845	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4080	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2805	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5405	0.400	ng	0.01
29) Chrysene-d12	21.161	240	5167	0.400	ng	# 0.00
35) Perylene-d12	23.345	264	5486	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.162	112	520	0.146	ng	0.00
5) Phenol-d6	6.766	99	237	0.064	ng	0.02
8) Nitrobenzene-d5	8.728	82	909	0.278	ng	0.01
11) 2-Methylnaphthalene-d10	11.945	152	2032	0.322	ng	0.00
14) 2,4,6-Tribromophenol	15.717	330	511	0.311	ng	0.00
15) 2-Fluorobiphenyl	12.832	172	3946	0.326	ng	0.00
27) Fluoranthene-d10	19.003	212	6216	0.401	ng	0.00
31) Terphenyl-d14	19.611	244	4924	0.447	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	90	0.051	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.090	149	730	0.114	ng	# 95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037413.D  
 Acq On : 27 Jun 2025 03:41  
 Operator : RC/JU  
 Sample : Q2375-01  
 Misc :  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 RW8-SP100-20250619

Quant Time: Jun 27 04:38:21 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration




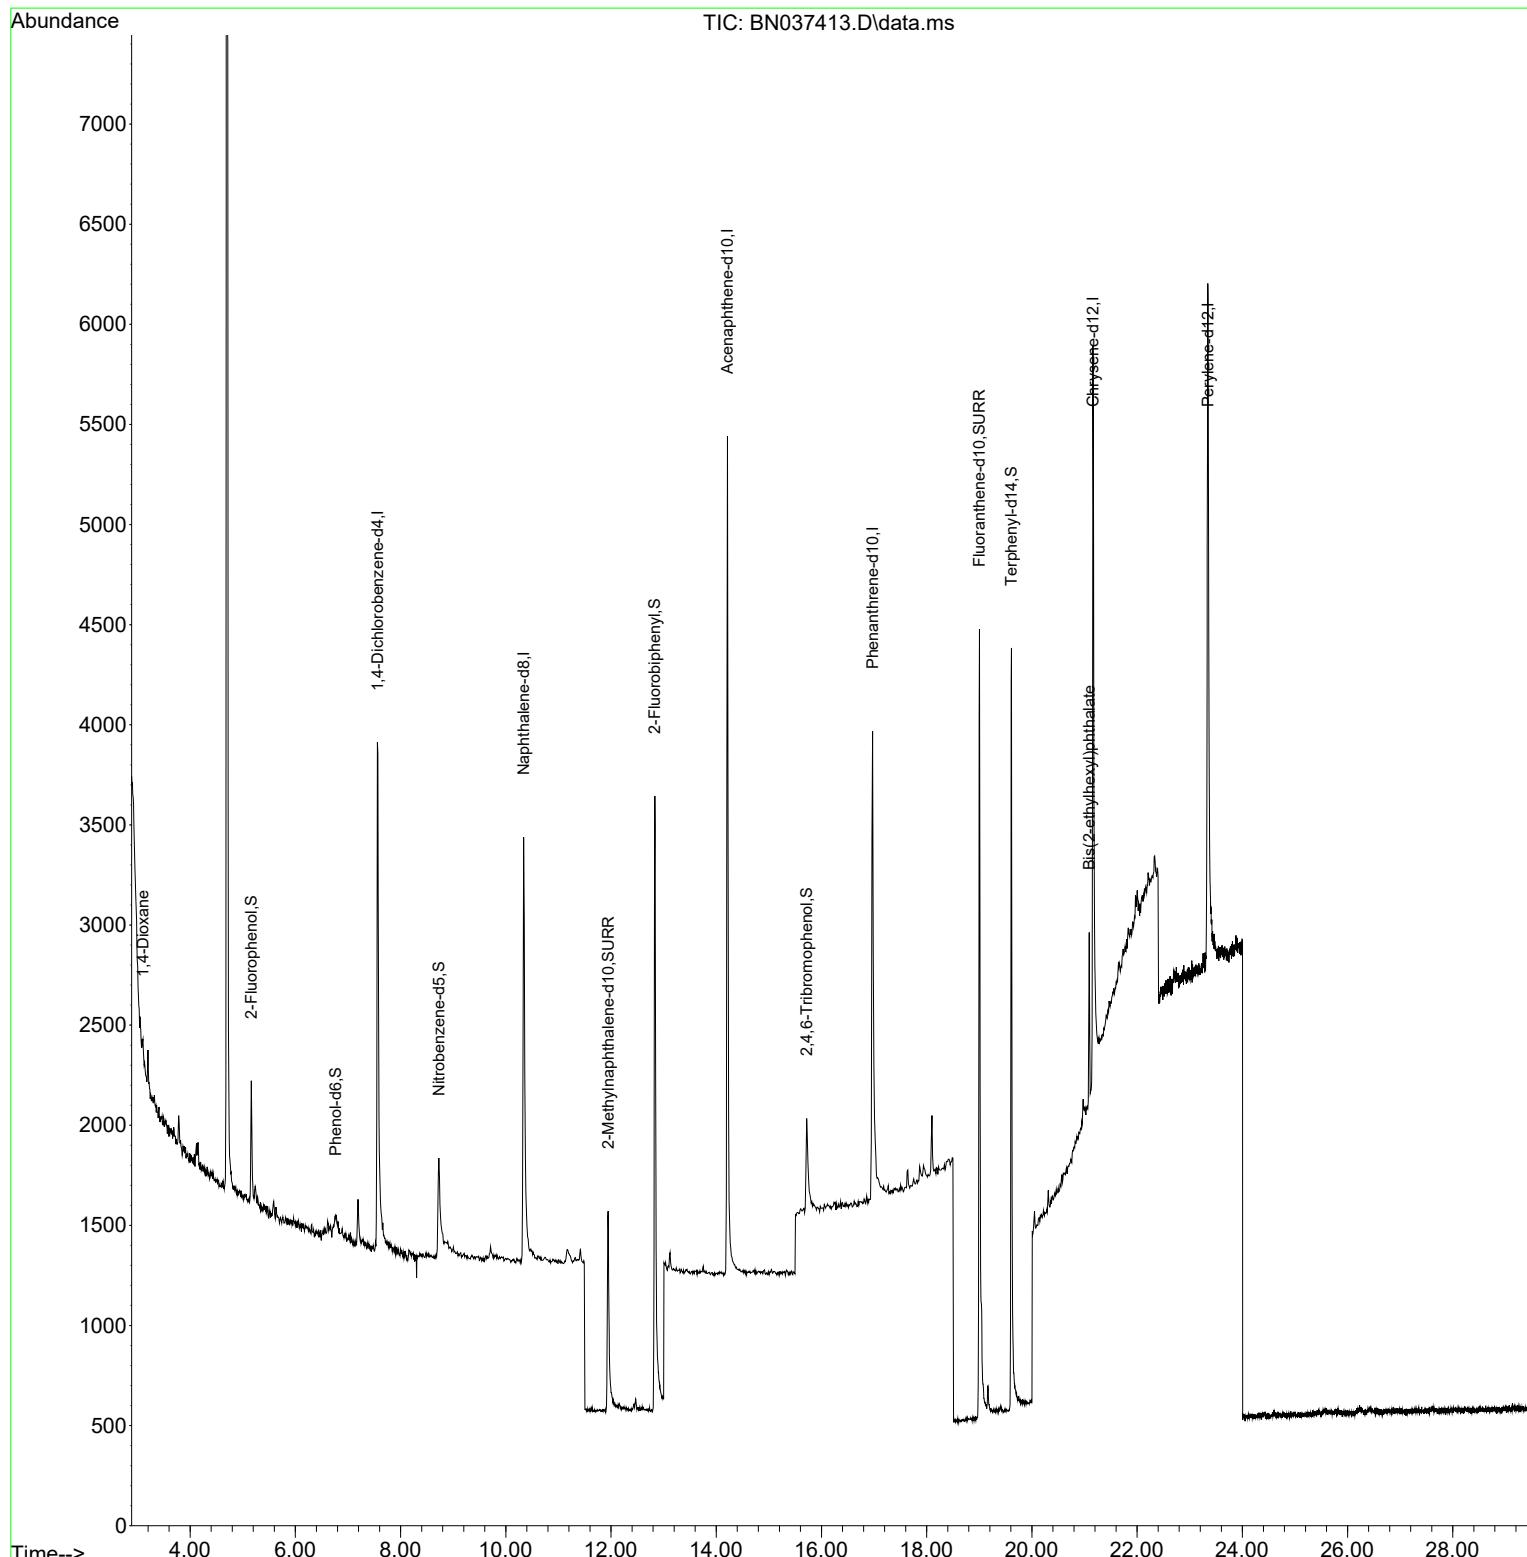




#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.567 min Scan# 6  
Delta R.T. -0.001 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41


Instrument : BNA\_N  
ClientSampleId : RW8-SP100-20250619




Tgt Ion:152 Resp: 1845  
Ion Ratio Lower Upper  
152 100  
150 145.2 116.2 174.2  
115 56.6 42.9 64.3

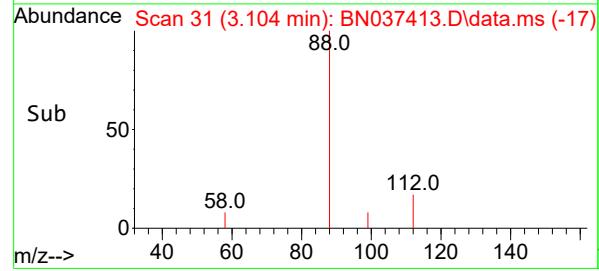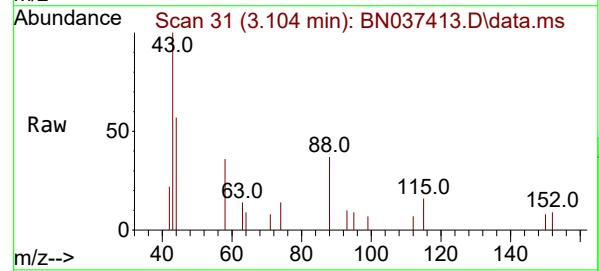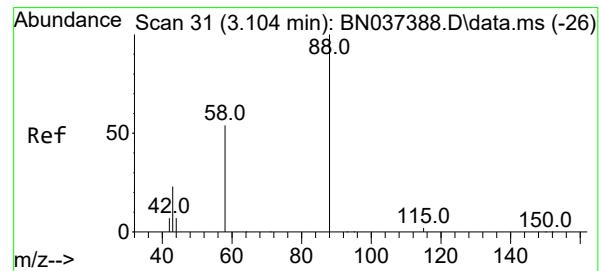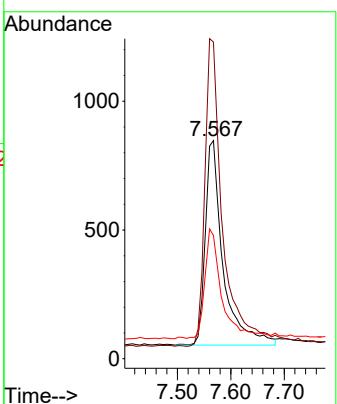

#2  
1,4-Dioxane  
Concen: 0.051 ng  
RT: 3.104 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41

Tgt Ion: 88 Resp: 90  
Ion Ratio Lower Upper  
88 100  
43 181.1 21.6 32.4#  
58 71.1 45.9 68.9#




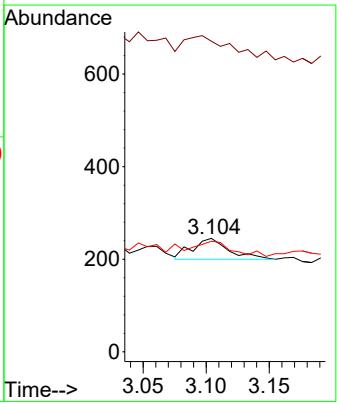


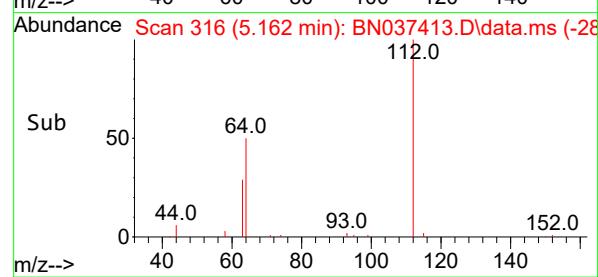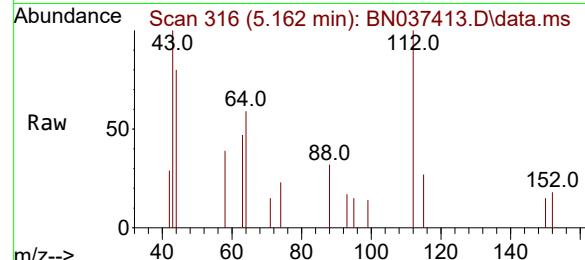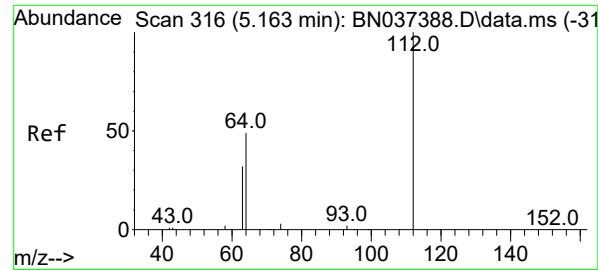

#4  
2-Fluorophenol  
Concen: 0.146 ng  
RT: 5.162 min Scan# 3  
Delta R.T. -0.000 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41


Instrument : BNA\_N  
ClientSampleId : RW8-SP100-20250619




Tgt Ion:112 Resp: 520  
Ion Ratio Lower Upper  
112 100  
64 49.4 40.3 60.5  
63 30.6 26.1 39.1

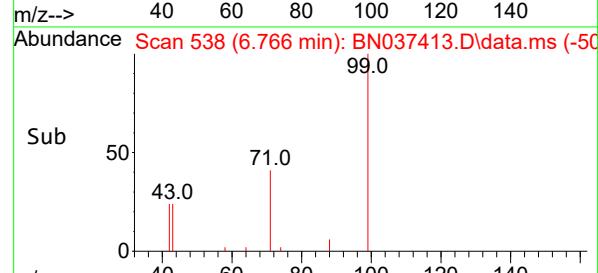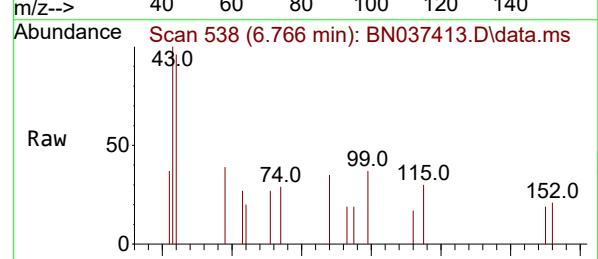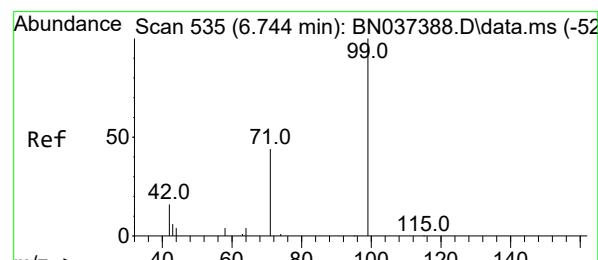

#5  
Phenol-d6  
Concen: 0.064 ng  
RT: 6.766 min Scan# 538  
Delta R.T. 0.021 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41

Tgt Ion: 99 Resp: 237  
Ion Ratio Lower Upper  
99 100  
42 8.9 15.6 23.4#  
71 42.6 35.8 53.8

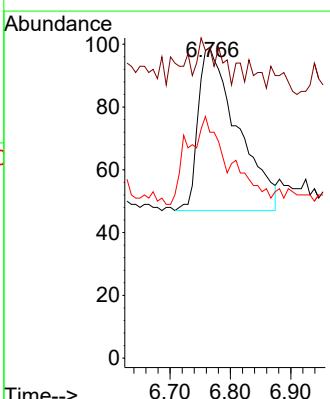







#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037413.D  
 Acq: 27 Jun 2025 03:41

Instrument : BNA\_N  
 ClientSampleId : RW8-SP100-20250619

Tgt Ion:136 Resp: 4080


Ion	Ratio	Lower	Upper
136	100		
137	12.8	10.4	15.6
54	8.7	5.6	8.4#
68	7.3	4.6	6.8#



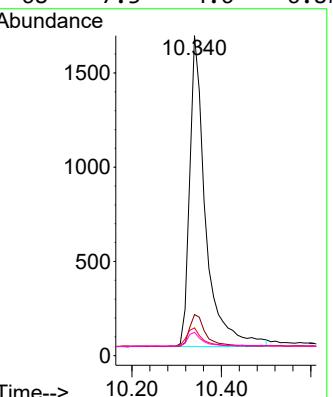


#8  
 Nitrobenzene-d5  
 Concen: 0.278 ng  
 RT: 8.728 min Scan# 791  
 Delta R.T. 0.010 min  
 Lab File: BN037413.D  
 Acq: 27 Jun 2025 03:41

Tgt Ion: 82 Resp: 909





Ion	Ratio	Lower	Upper
82	100		
128	47.5	34.0	51.0
54	47.9	37.7	56.5

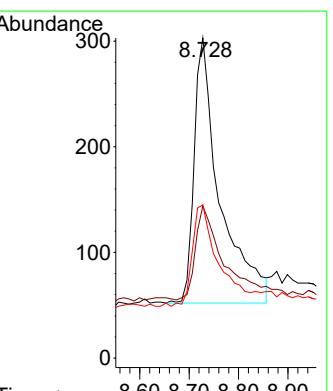

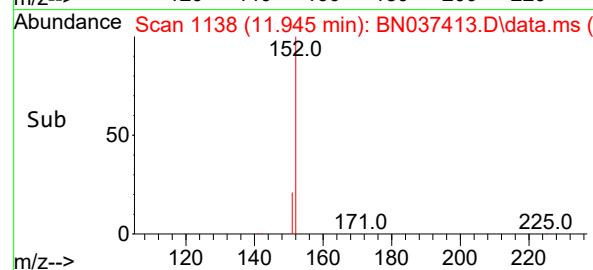


#11  
2-Methylnaphthalene-d10  
Concen: 0.322 ng  
RT: 11.945 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.005 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41 ClientSampleId : RW8-SP100-20250619


Tgt Ion:152 Resp: 2032  
Ion Ratio Lower Upper  
152 100  
151 20.6 18.4 27.6



#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1460  
Delta R.T. -0.000 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41

Tgt Ion:164 Resp: 2805  
Ion Ratio Lower Upper  
164 100  
162 100.6 82.6 123.8  
160 52.2 42.2 63.2


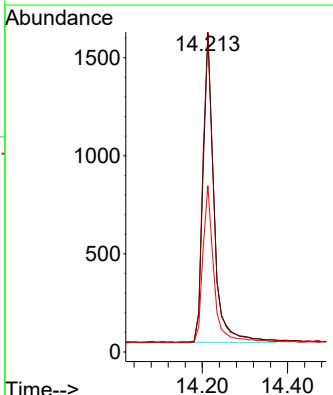


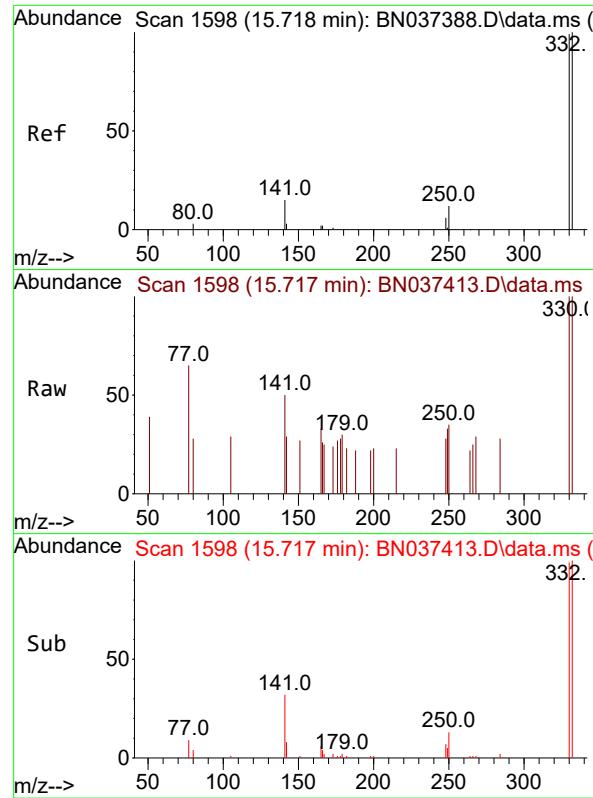

#14  
2,4,6-Tribromophenol  
Concen: 0.311 ng  
RT: 15.717 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41


Instrument : BNA\_N  
ClientSampleId : RW8-SP100-20250619




Tgt Ion:330 Resp: 511  
Ion Ratio Lower Upper  
330 100  
332 97.3 77.8 116.8  
141 33.3 24.0 36.0

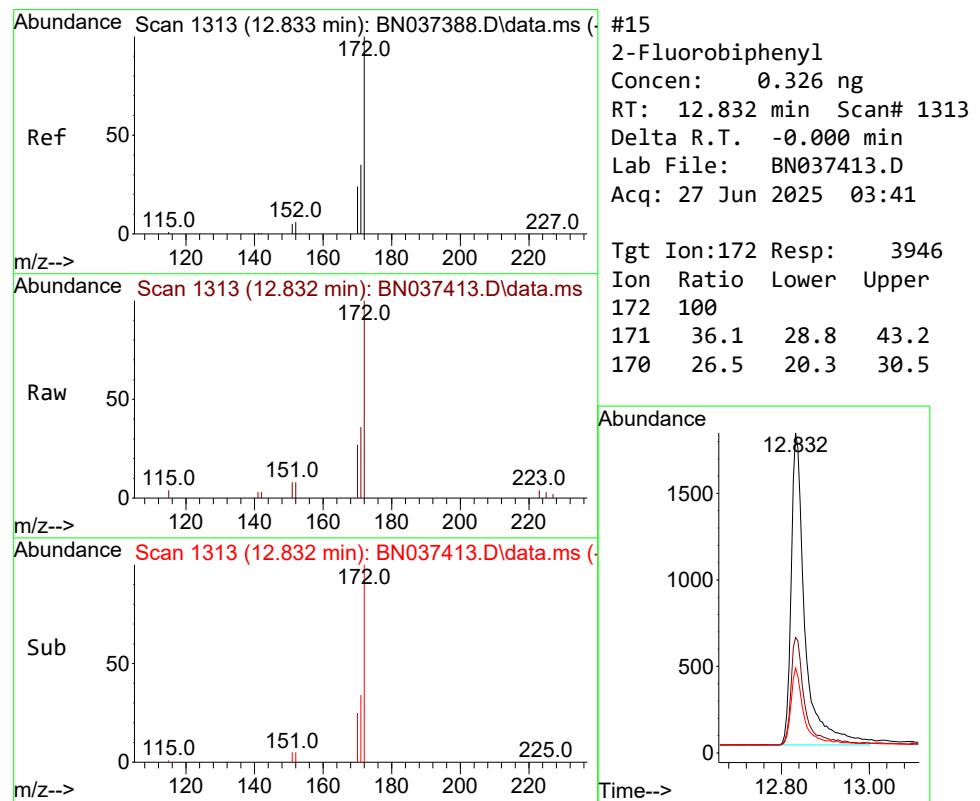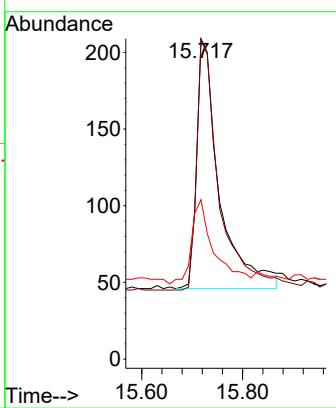

#15  
2-Fluorobiphenyl  
Concen: 0.326 ng  
RT: 12.832 min Scan# 1313  
Delta R.T. -0.000 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41

Tgt Ion:172 Resp: 3946  
Ion Ratio Lower Upper  
172 100  
171 36.1 28.8 43.2  
170 26.5 20.3 30.5

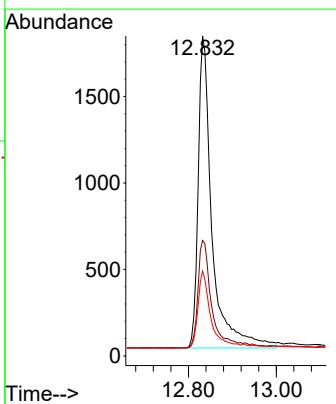



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. 0.012 min

Lab File: BN037413.D ClientSampleId :

Acq: 27 Jun 2025 03:41 RW8-SP100-20250619

Instrument :

BNA\_N





Tgt Ion:188 Resp: 5405

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 7.0 6.2 9.4

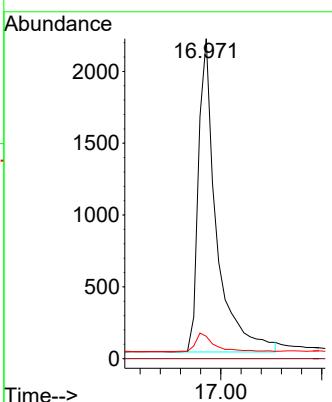

#27

Fluoranthene-d10

Concen: 0.401 ng

RT: 19.003 min Scan# 1929

Delta R.T. -0.000 min

Lab File: BN037413.D

Acq: 27 Jun 2025 03:41


Tgt Ion:212 Resp: 6216


Ion Ratio Lower Upper

212 100

106 5.9 4.5 6.7

104 3.3 2.7 4.1





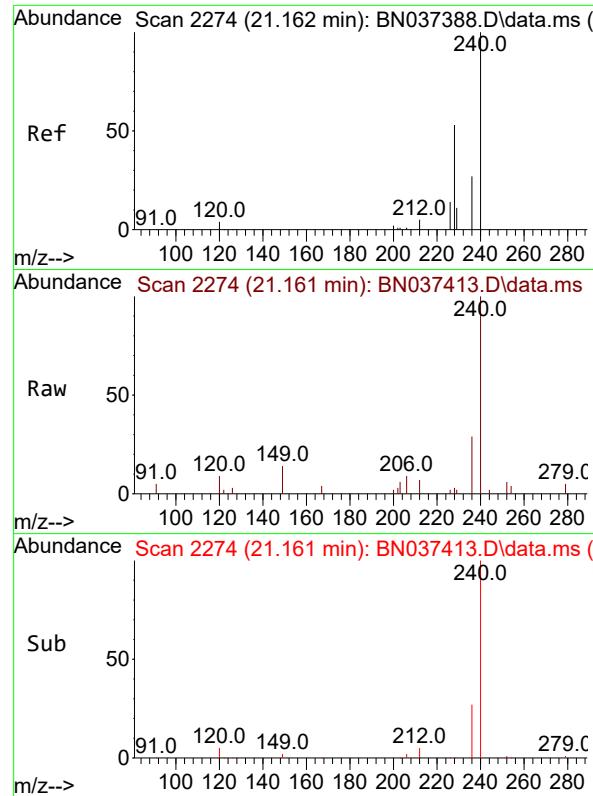

#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.161 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41


Instrument : BNA\_N  
ClientSampleId : RW8-SP100-20250619




Tgt Ion:240 Resp: 5167  
Ion Ratio Lower Upper  
240 100  
120 8.8 5.3 7.9#  
236 29.3 22.7 34.1

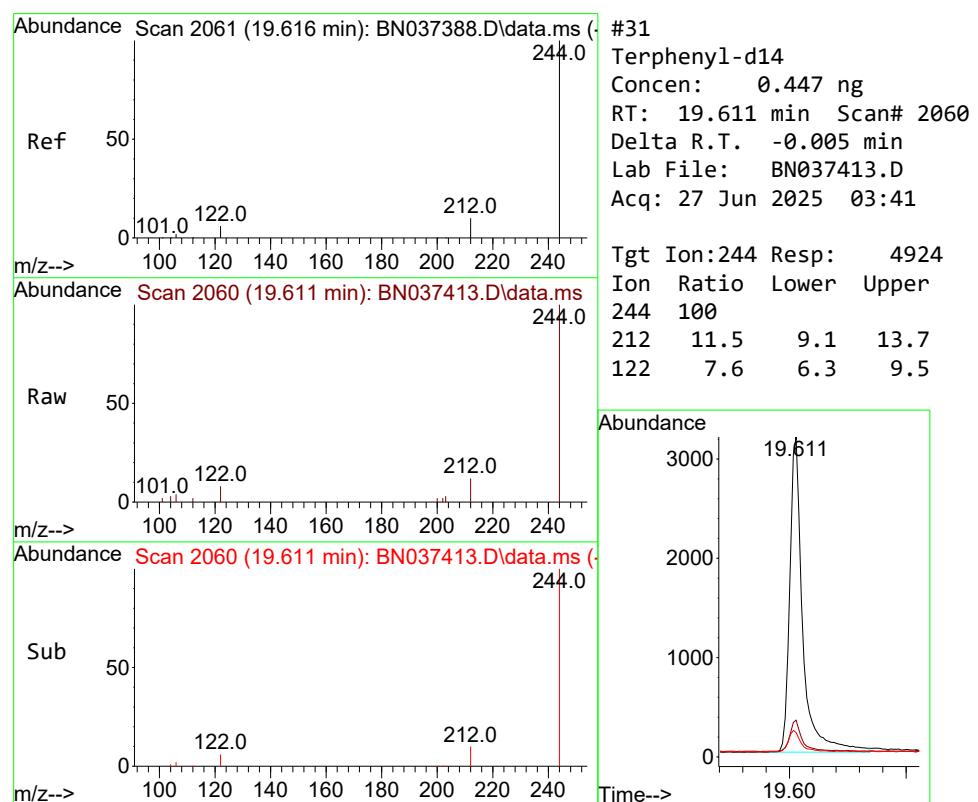

#31  
Terphenyl-d14  
Concen: 0.447 ng  
RT: 19.611 min Scan# 2060  
Delta R.T. -0.005 min  
Lab File: BN037413.D  
Acq: 27 Jun 2025 03:41

Tgt Ion:244 Resp: 4924  
Ion Ratio Lower Upper  
244 100  
212 11.5 9.1 13.7  
122 7.6 6.3 9.5



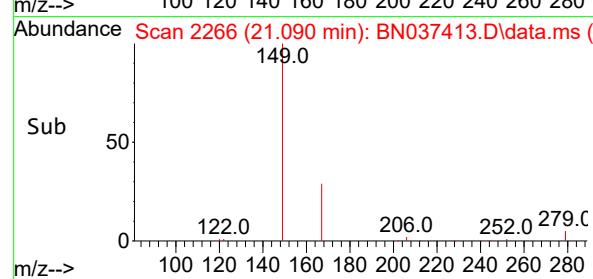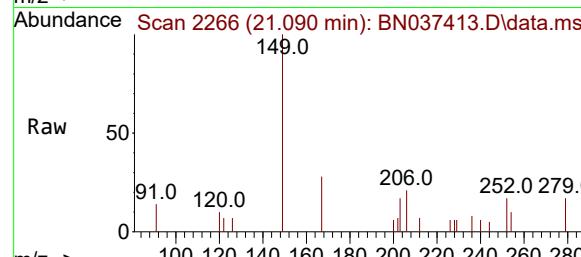

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.114 ng

RT: 21.090 min Scan# 2

Delta R.T. -0.000 min

Lab File: BN037413.D

Acq: 27 Jun 2025 03:41

Instrument :

BNA\_N

ClientSampleId :

RW8-SP100-20250619





Tgt Ion:149 Resp: 730

Ion Ratio Lower Upper

149 100

167 28.9 24.8 37.2

279 9.3 5.0 7.6#

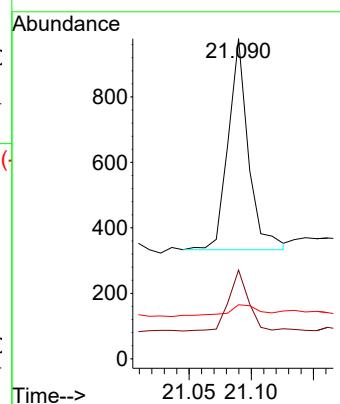

#35

Perylene-d<sub>12</sub>

Concen: 0.400 ng

RT: 23.345 min Scan# 2734

Delta R.T. -0.000 min

Lab File: BN037413.D

Acq: 27 Jun 2025 03:41


Tgt Ion:264 Resp: 5486

Ion Ratio Lower Upper

264 100

260 26.8 21.4 32.0

265 92.8 56.2 84.4#

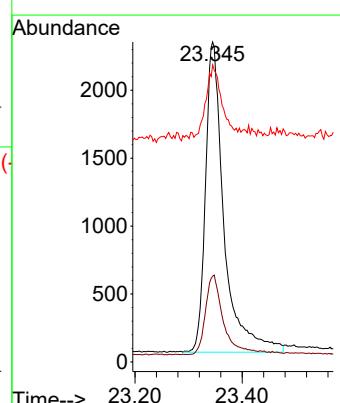



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Tetra Tech NUS, Inc.			Date Collected:	06/19/25	
Project:	NWIRP Bethpage 112G08005-WE13			Date Received:	06/19/25	
Client Sample ID:	RW8-SP303-20250619			SDG No.:	Q2375	
Lab Sample ID:	Q2375-02			Matrix:	Water	
Analytical Method:	SW8270ESIM			% Solid:	0	
Sample Wt/Vol:	990	Units:	mL	Final Vol:	1000	uL
Soil Aliquot Vol:	uL			Test:	SVOC-SIMGroup1	
Extraction Type :	Decanted : N			Level :	LOW	
Injection Volume :	GPC Factor : 1.0			GPC Cleanup :	N	PH :
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN037414.D	1	06/20/25 12:03	06/27/25 04:18	PB168563

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
123-91-1	1,4-Dioxane	0.20	U	0.070	0.20	0.20	ug/L
<b>SURROGATES</b>							
7297-45-2	2-Methylnaphthalene-d10	0.35		30 - 150		88%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.39		30 - 150		98%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.28		55 - 111		71%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.35		53 - 106		88%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.46		58 - 132		116%	SPK: 0.4
<b>INTERNAL STANDARDS</b>							
3855-82-1	1,4-Dichlorobenzene-d4	1770		7.568			
1146-65-2	Naphthalene-d8	3840		10.34			
15067-26-2	Acenaphthene-d10	2720		14.213			
1517-22-2	Phenanthrene-d10	5440		16.971			
1719-03-5	Chrysene-d12	5380		21.162			
1520-96-3	Perylene-d12	5620		23.345			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037414.D  
 Acq On : 27 Jun 2025 04:18  
 Operator : RC/JU  
 Sample : Q2375-02  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 RW8-SP303-20250619

Quant Time: Jun 27 05:26:29 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1773	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	3842	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2717	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5443	0.400	ng	0.01
29) Chrysene-d12	21.162	240	5375	0.400	ng	# 0.00
35) Perylene-d12	23.345	264	5619	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	514	0.150	ng	0.00
5) Phenol-d6	6.766	99	219	0.062	ng	0.02
8) Nitrobenzene-d5	8.728	82	872	0.283	ng	0.01
11) 2-Methylnaphthalene-d10	11.940	152	2100	0.353	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	582	0.365	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	4145	0.353	ng	0.00
27) Fluoranthene-d10	19.003	212	6108	0.392	ng	0.00
31) Terphenyl-d14	19.607	244	5311	0.463	ng	0.00
<b>Target Compounds</b>						
34) Bis(2-ethylhexyl)phtha...	21.090	149	1863	0.279	ng	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037414.D  
 Acq On : 27 Jun 2025 04:18  
 Operator : RC/JU  
 Sample : Q2375-02  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 RW8-SP303-20250619

Quant Time: Jun 27 05:26:29 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration



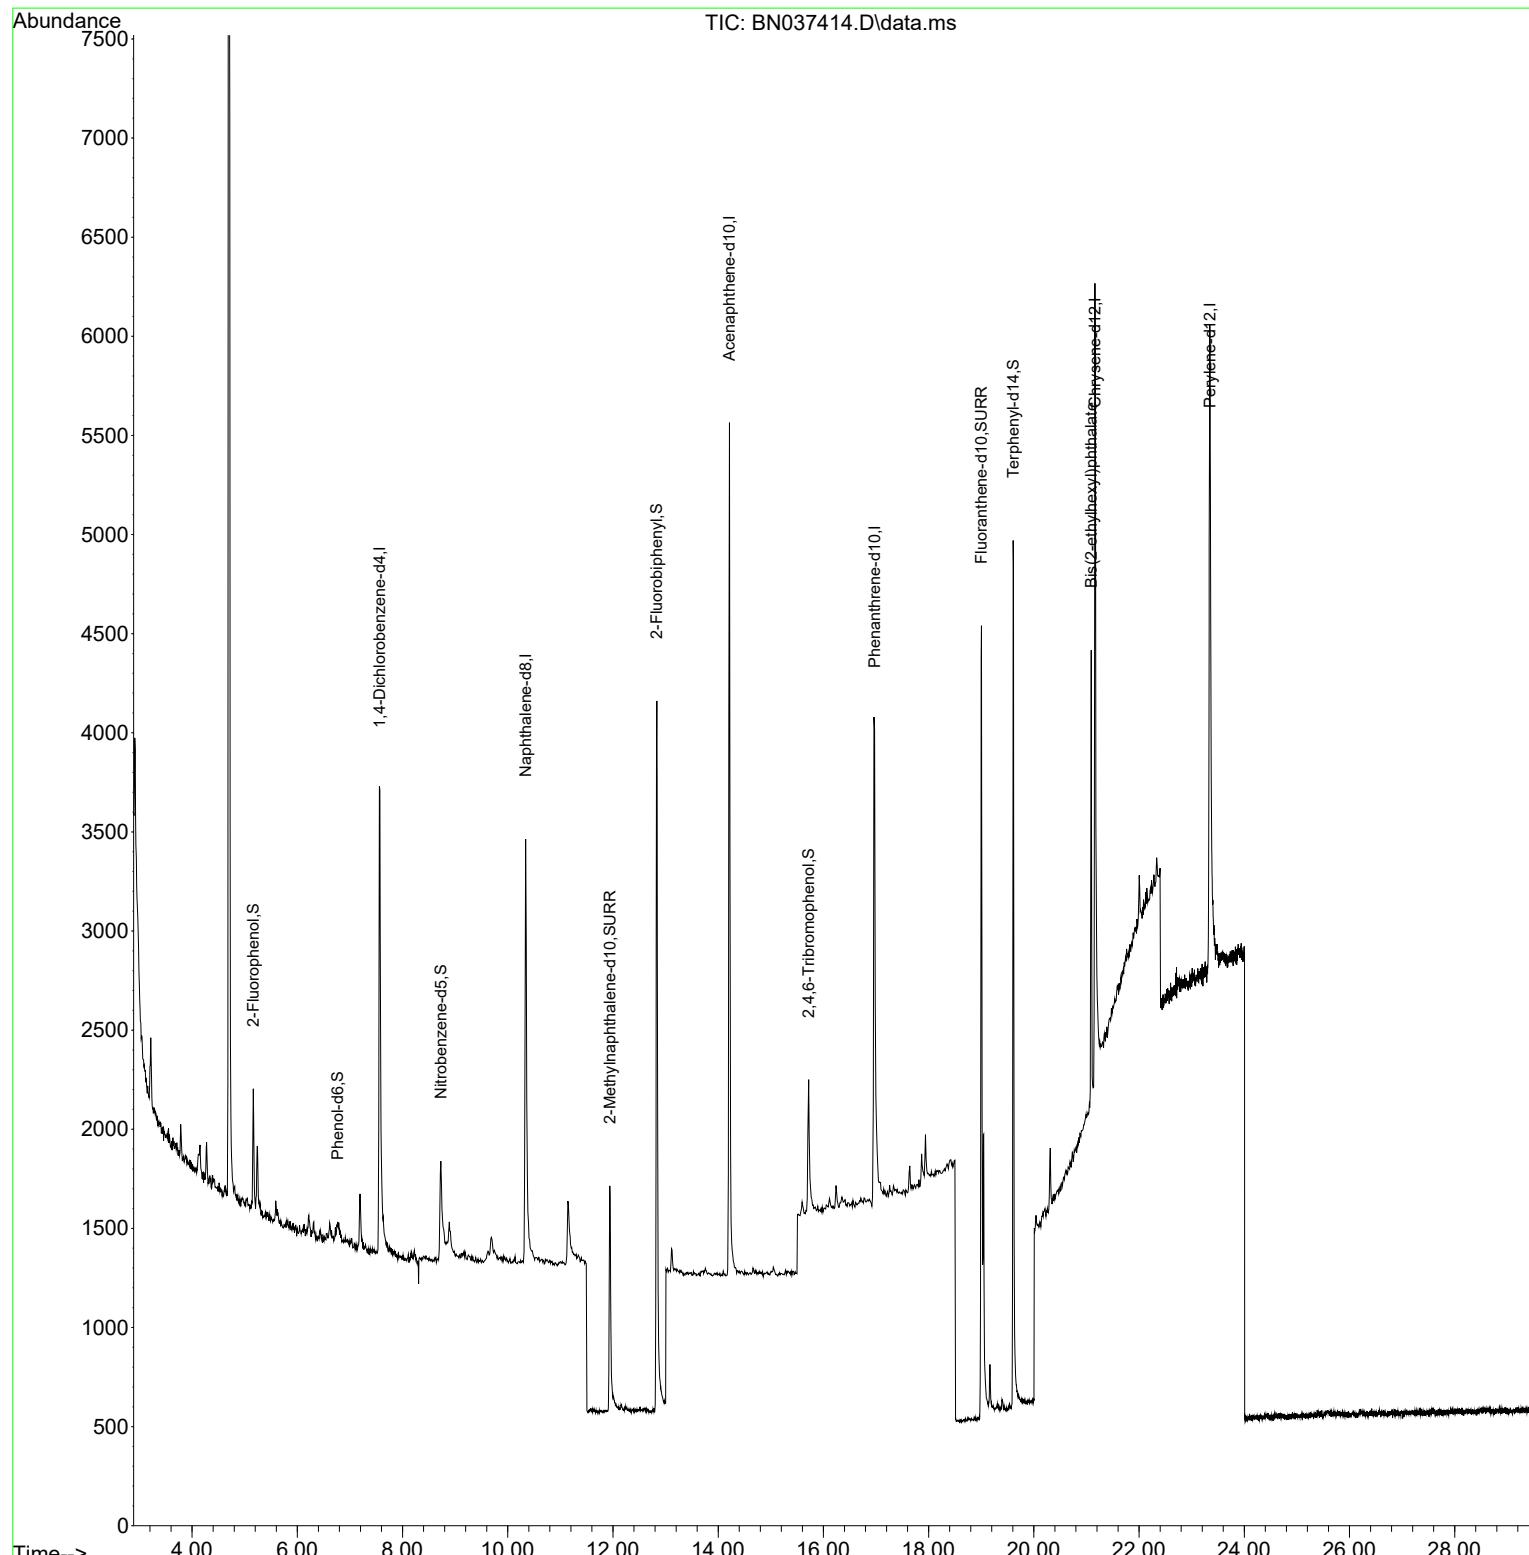


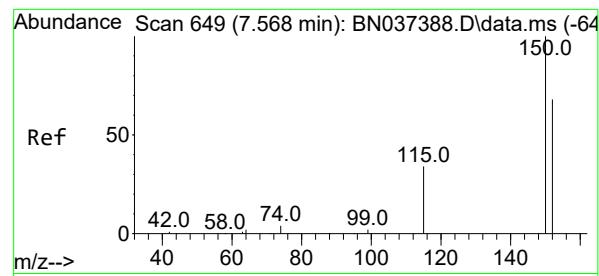

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037414.D  
Acq: 27 Jun 2025 04:18



Instrument : BNA\_N  
ClientSampleId : RW8-SP303-20250619




Tgt Ion:152 Resp: 1773  
Ion Ratio Lower Upper  
152 100  
150 148.1 116.2 174.2  
115 54.5 42.9 64.3

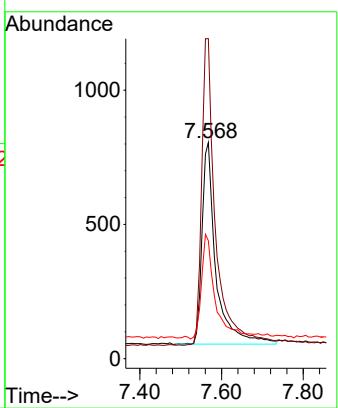

#4  
2-Fluorophenol  
Concen: 0.150 ng  
RT: 5.163 min Scan# 316  
Delta R.T. -0.000 min  
Lab File: BN037414.D  
Acq: 27 Jun 2025 04:18

Tgt Ion:112 Resp: 514  
Ion Ratio Lower Upper  
112 100  
64 48.8 40.3 60.5  
63 30.0 26.1 39.1



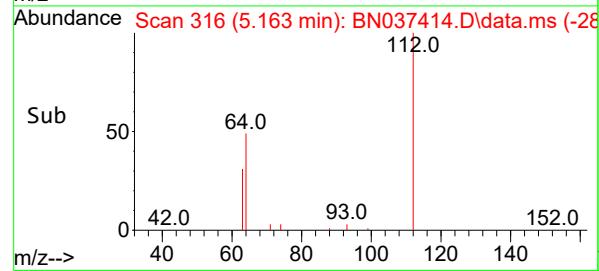
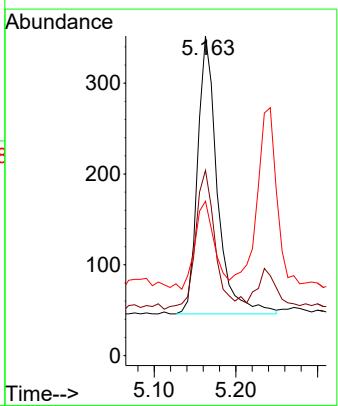


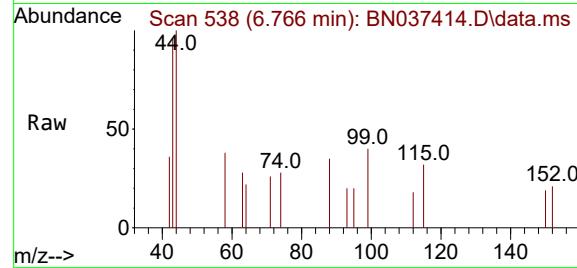

#5  
 Phenol-d6  
 Concen: 0.062 ng  
 RT: 6.766 min Scan# 5  
 Delta R.T. 0.022 min  
 Lab File: BN037414.D  
 Acq: 27 Jun 2025 04:18


Instrument : BNA\_N  
 ClientSampleId : RW8-SP303-20250619




Tgt Ion: 99 Resp: 219  
 Ion Ratio Lower Upper  
 99 100  
 42 10.5 15.6 23.4#  
 71 0.0 35.8 53.8#

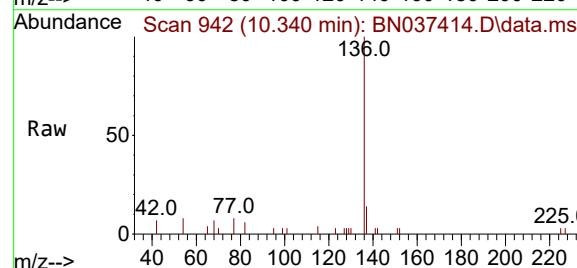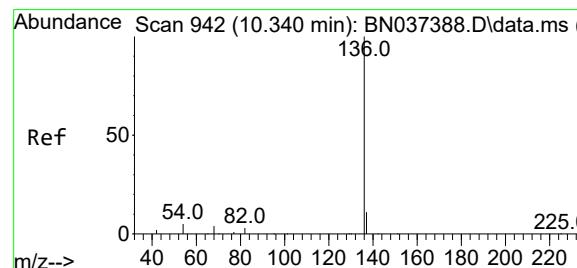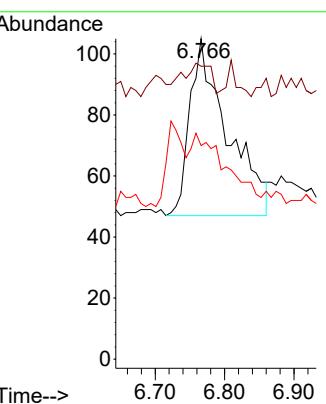

#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 942  
 Delta R.T. -0.000 min  
 Lab File: BN037414.D  
 Acq: 27 Jun 2025 04:18

Tgt Ion:136 Resp: 3842  
 Ion Ratio Lower Upper  
 136 100  
 137 13.9 10.4 15.6  
 54 8.3 5.6 8.4  
 68 7.3 4.6 6.8#

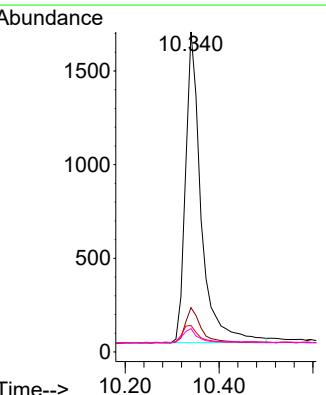

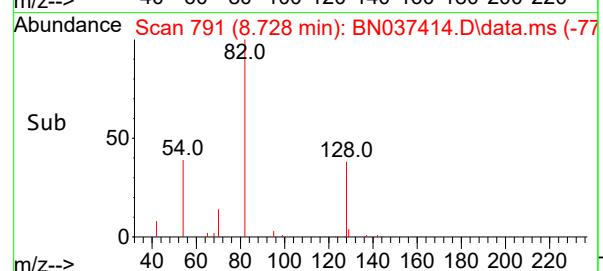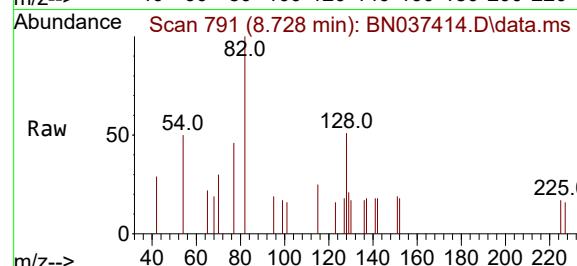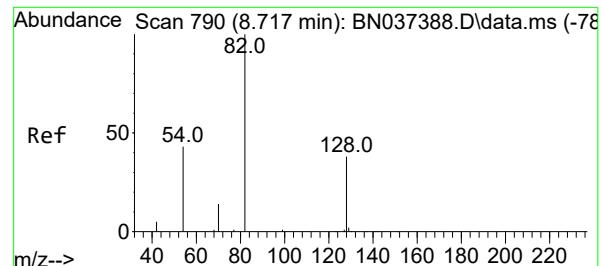

#8

Nitrobenzene-d5

Concen: 0.283 ng

RT: 8.728 min Scan# 7

Delta R.T. 0.011 min

Lab File: BN037414.D

Acq: 27 Jun 2025 04:18

Instrument :

BNA\_N

ClientSampleId :

RW8-SP303-20250619

Tgt Ion: 82 Resp: 872

Ion Ratio Lower Upper





82 100

128 51.0 34.0 51.0#

54 49.7 37.7 56.5

Abundance

8.728

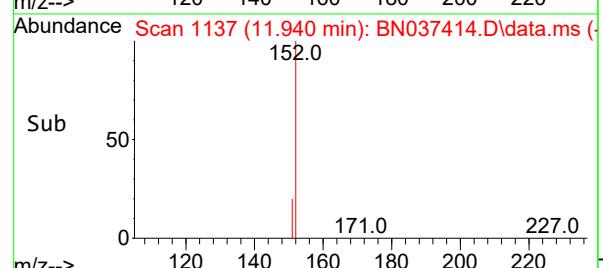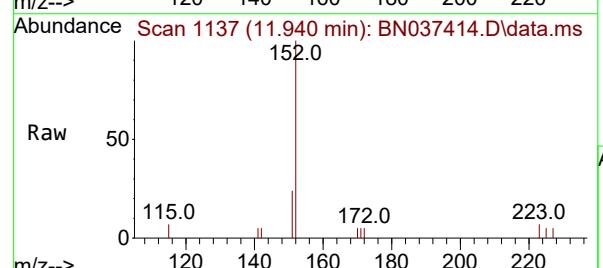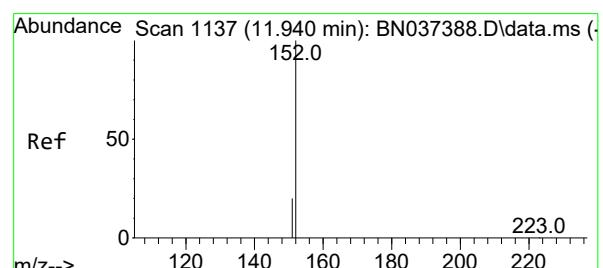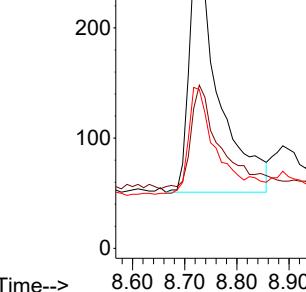

#11

2-Methylnaphthalene-d10

Concen: 0.353 ng

RT: 11.940 min Scan# 1137

Delta R.T. -0.000 min

Lab File: BN037414.D

Acq: 27 Jun 2025 04:18

Tgt Ion: 152 Resp: 2100


Ion Ratio Lower Upper


152 100

151 20.3 18.4 27.6

Abundance

11.940

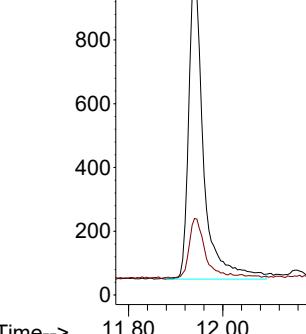

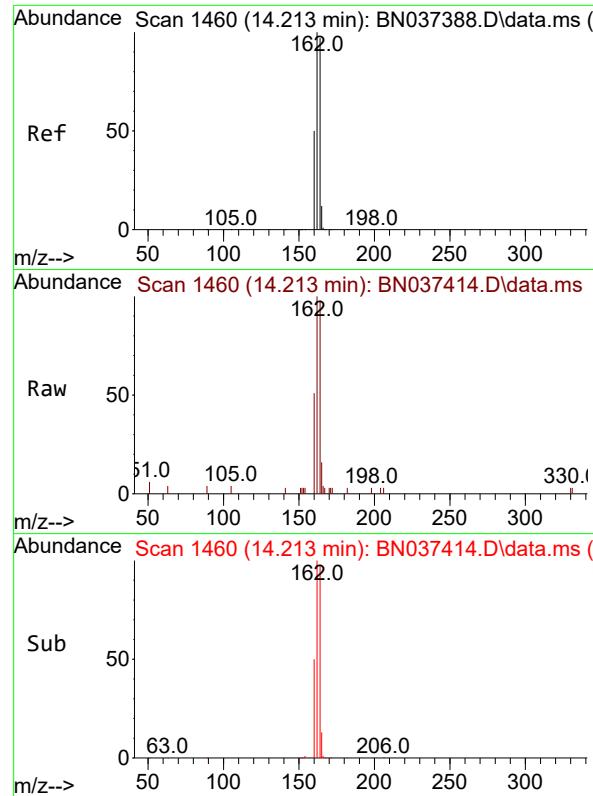

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037414.D

Acq: 27 Jun 2025 04:18

Instrument :  
BNA\_N  
ClientSampleId :  
RW8-SP303-20250619



Tgt Ion:164 Resp: 2717

Ion Ratio Lower Upper

164 100

162 101.8 82.6 123.8

160 52.2 42.2 63.2

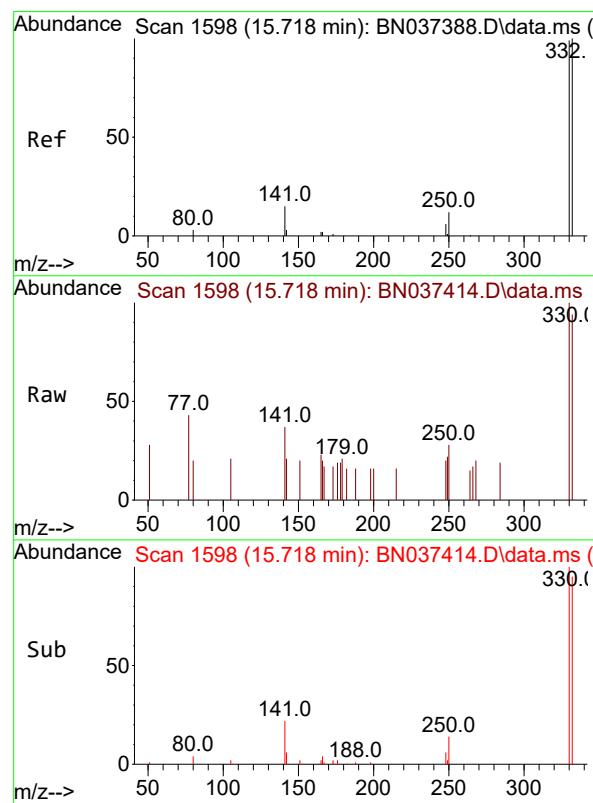

#14

2,4,6-Tribromophenol

Concen: 0.365 ng

RT: 15.718 min Scan# 1598

Delta R.T. -0.000 min

Lab File: BN037414.D

Acq: 27 Jun 2025 04:18


Tgt Ion:330 Resp: 582




Ion Ratio Lower Upper

330 100

332 93.1 77.8 116.8





141 33.2 24.0 36.0






#15  
2-Fluorobiphenyl  
Concen: 0.353 ng  
RT: 12.833 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037414.D  
Acq: 27 Jun 2025 04:18  
ClientSampleId : RW8-SP303-20250619


Tgt Ion:172 Resp: 4145  
Ion Ratio Lower Upper  
172 100  
171 37.1 28.8 43.2  
170 25.9 20.3 30.5

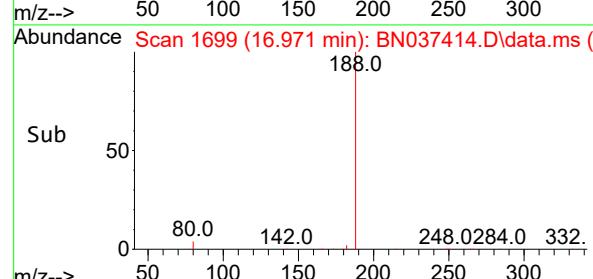

#19  
Phenanthrene-d10  
Concen: 0.400 ng  
RT: 16.971 min Scan# 1699  
Delta R.T. 0.012 min  
Lab File: BN037414.D  
Acq: 27 Jun 2025 04:18

Tgt Ion:188 Resp: 5443  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 6.6 6.2 9.4


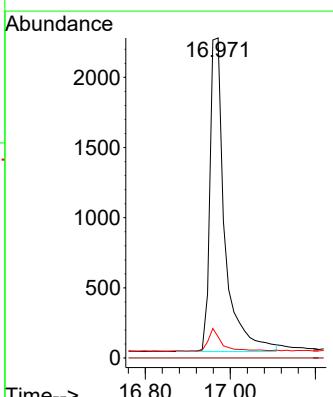


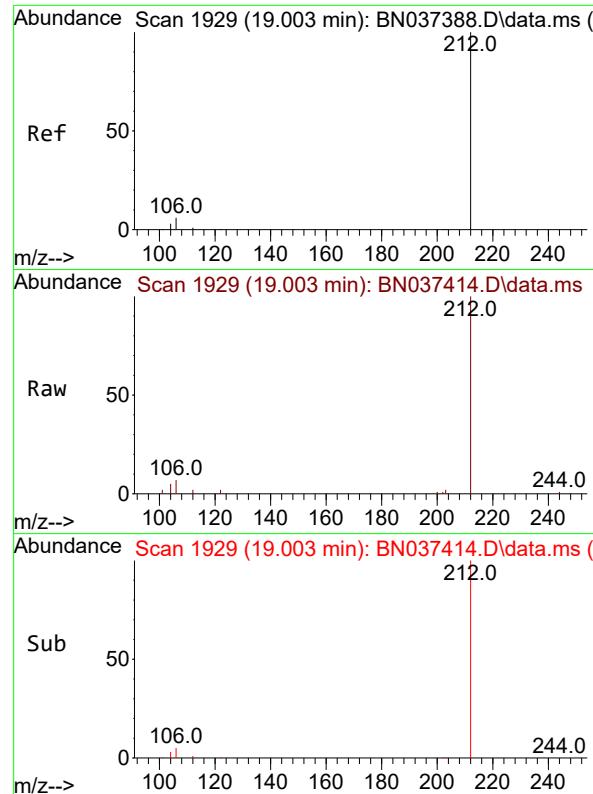

#27  
 Fluoranthene-d10  
 Concen: 0.392 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037414.D  
 Acq: 27 Jun 2025 04:18


Instrument : BNA\_N  
 ClientSampleId : RW8-SP303-20250619


Tgt Ion:212 Resp: 6108  
 Ion Ratio Lower Upper  
 212 100  
 106 5.4 4.5 6.7  
 104 3.4 2.7 4.1

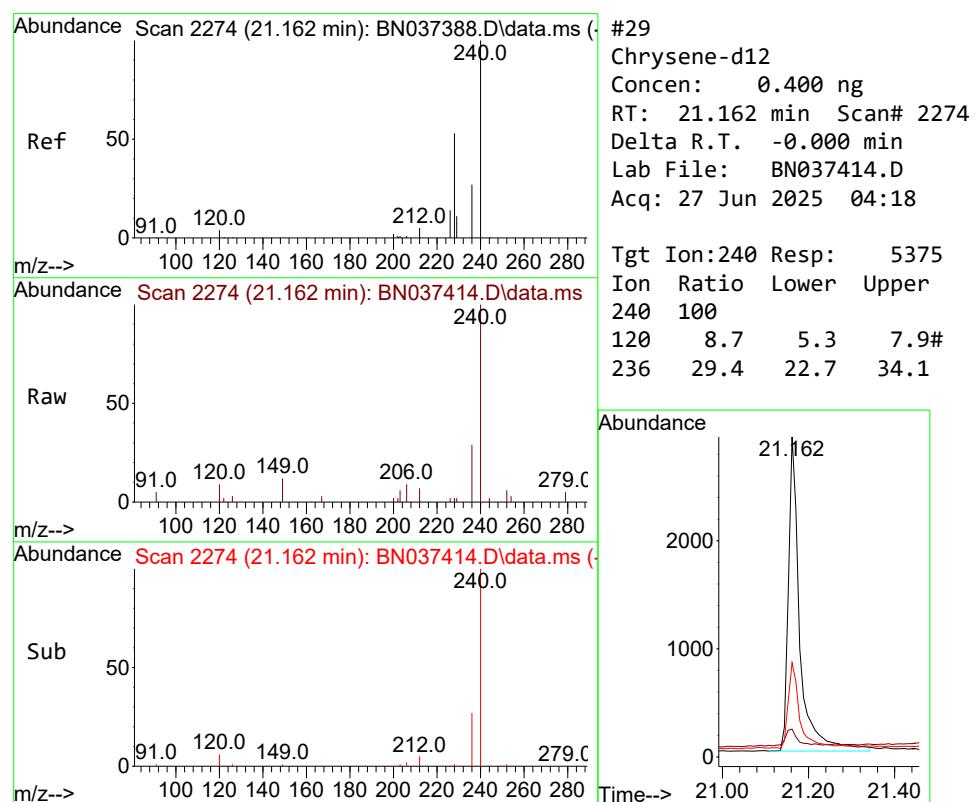

#29  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.162 min Scan# 2274  
 Delta R.T. -0.000 min  
 Lab File: BN037414.D  
 Acq: 27 Jun 2025 04:18

Tgt Ion:240 Resp: 5375  
 Ion Ratio Lower Upper  
 240 100  
 120 8.7 5.3 7.9#  
 236 29.4 22.7 34.1





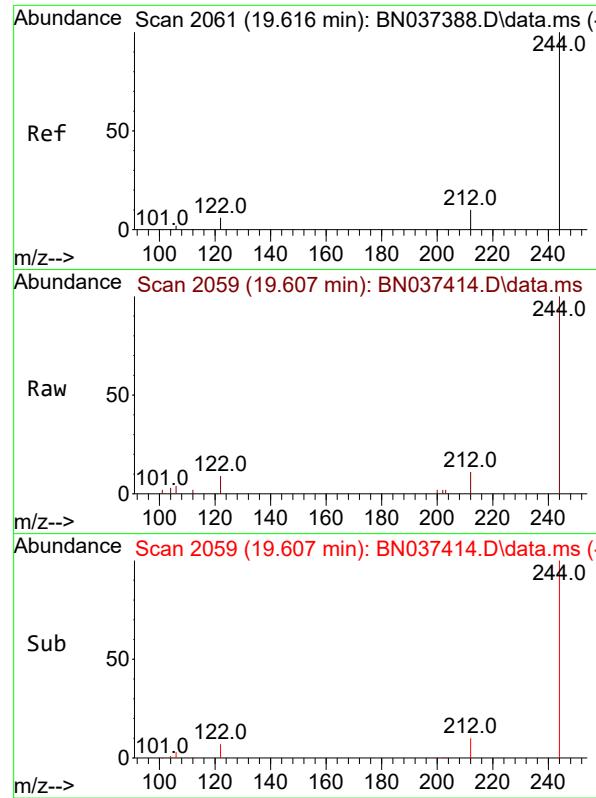

#31  
Terphenyl-d14  
Concen: 0.463 ng  
RT: 19.607 min Scan# 2  
Delta R.T. -0.009 min  
Lab File: BN037414.D  
Acq: 27 Jun 2025 04:18


Instrument : BNA\_N  
ClientSampleId : RW8-SP303-20250619


Tgt Ion:244 Resp: 5311  
Ion Ratio Lower Upper  
244 100  
212 11.2 9.1 13.7  
122 8.6 6.3 9.5

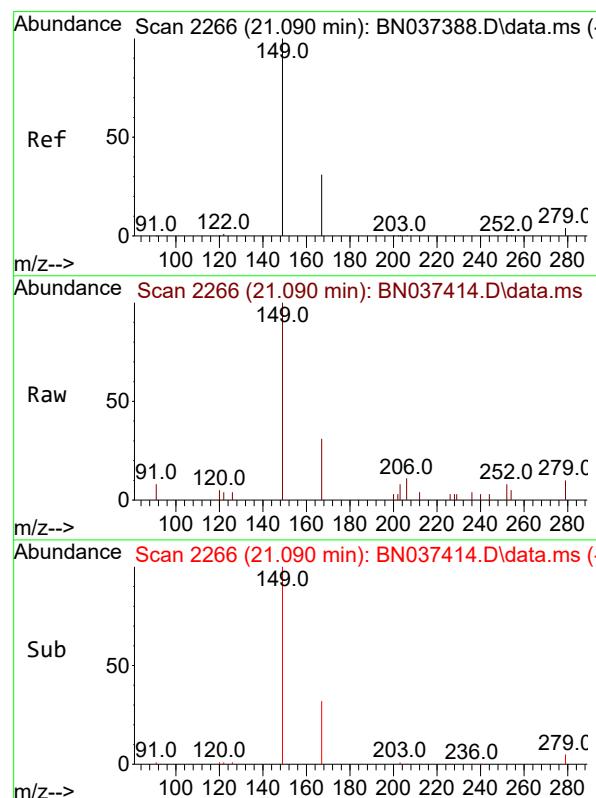

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.279 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. -0.000 min  
Lab File: BN037414.D  
Acq: 27 Jun 2025 04:18

Tgt Ion:149 Resp: 1863  
Ion Ratio Lower Upper  
149 100  
167 30.8 24.8 37.2  
279 6.3 5.0 7.6

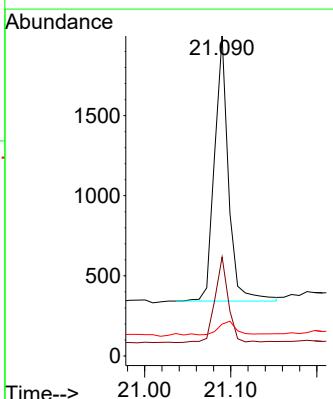

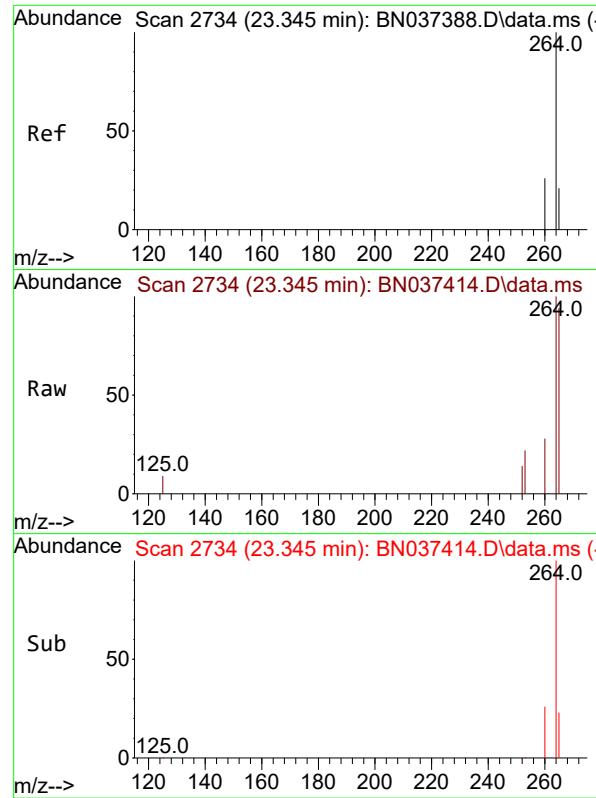

#35

Perylene-d<sub>12</sub>

Concen: 0.400 ng

RT: 23.345 min Scan# 2

Delta R.T. -0.000 min

Lab File: BN037414.D

Acq: 27 Jun 2025 04:18

Instrument :

BNA\_N

ClientSampleId :

RW8-SP303-20250619


Tgt Ion:264 Resp: 5619

Ion Ratio Lower Upper

264 100

260 27.5 21.4 32.0

265 93.9 56.2 84.4#

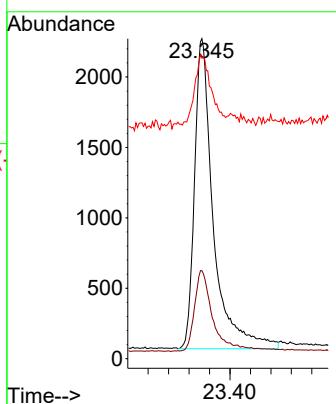



# CALIBRATION

# SUMMARY

Method Path : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\  
 Method File : 8270-SIM-BN062125.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jun 20 23:41:54 2025  
 Response Via : Initial Calibration

## Calibration Files

0.1 =BN037353.D 0.2 =BN037354.D 0.4 =BN037355.D 0.8 =BN037356.D 1.6 =BN037357.D 3.2 =BN037358.D 5 =BN037359.D

Compound	0.1	0.2	0.4	0.8	1.6	3.2	5	Avg	%RSD
----------	-----	-----	-----	-----	-----	-----	---	-----	------

1) I	1,4-Dichlorobenzene	-----	ISTD-----						
2)	1,4-Dioxane	0.506	0.390	0.412	0.417	0.370	0.346	0.407	13.63
3)	n-Nitrosodimethylamine	0.392	0.394	0.367	0.391	0.354	0.338	0.373	6.37
4) S	2-Fluorophenol	0.854	0.818	0.751	0.781	0.834	0.786	0.771	0.799
5) S	Phenol-d6	0.781	0.766	0.766	0.785	0.891	0.878	0.896	0.823
6)	bis(2-Chloroethyl)ether	0.719	0.546	0.707	0.738	0.826	0.786	0.791	0.730
7) I	Naphthalene-d8	-----	ISTD-----						
8) S	Nitrobenzene-d5	0.254	0.292	0.319	0.318	0.363	0.354	0.361	0.323
9)	Naphthalene	1.056	1.056	1.046	1.014	1.105	1.052	1.063	1.056
10)	Hexachlorobutane	0.452	0.434	0.441	0.407	0.424	0.384	0.376	0.417
11)	SURR2-Methylnaphthalene	0.619	0.638	0.666	0.610	0.666	0.664	0.675	0.648
12)	2-Methylnaphthalene	0.703	0.692	0.711	0.704	0.777	0.778	0.787	0.736
13) I	Acenaphthene-d10	-----	ISTD-----						
14) S	2,4,6-Tribromoethane	0.219	0.226	0.230	0.231	0.253	0.238	0.246	0.235
15) S	2-Fluorobiphenyl	1.705	1.675	1.777	1.714	1.897	1.752	1.778	1.757
16)	Acenaphthylene	1.646	1.636	1.597	1.595	1.797	1.717	1.786	1.682
17)	Acenaphthene	1.108	1.070	1.061	1.051	1.174	1.123	1.160	1.107
18)	Fluorene	1.499	1.470	1.506	1.490	1.660	1.605	1.660	1.556
19) I	Phenanthrene-d10	-----	ISTD-----						
20)	4,6-Dinitro-2-phenol	0.070	0.079	0.097	0.110	0.107	0.114	0.096	18.63
21)	4-Bromophenylmethanol	0.264	0.267	0.279	0.284	0.305	0.295	0.299	0.285
22)	Hexachlorobenzene	0.322	0.319	0.314	0.304	0.324	0.296	0.292	0.310
23)	Atrazine	0.221	0.215	0.218	0.220	0.239	0.239	0.238	0.227
24)	Pentachlorophenol	0.131	0.137	0.157	0.169	0.161	0.170	0.154	10.69
25)	Phenanthrene	1.108	1.075	1.104	1.139	1.242	1.221	1.222	1.158
26)	Anthracene	0.993	0.984	0.990	1.054	1.150	1.137	1.171	1.068
27)	SURRFluoranthene-d10	1.097	1.070	1.161	1.166	1.235	1.151	1.158	1.148
28)	Fluoranthene	1.412	1.343	1.367	1.492	1.605	1.512	1.518	1.464
29) I	Chrysene-d12	-----	ISTD-----						
30)	Pyrene	1.726	1.690	1.660	1.444	1.572	1.642	1.643	1.625
31) S	Terphenyl-d14	0.949	0.911	0.925	0.829	0.909	0.935	0.921	0.912
32)	Benzo(a)anthracene	1.309	1.168	1.216	1.278	1.431	1.372	1.429	1.315
33)	Chrysene	1.752	1.706	1.611	1.481	1.586	1.528	1.495	1.594
34)	Bis(2-ethylhexyl)phthalate	0.606	0.541	0.487	0.520	0.531	0.554	0.540	7.34
35) I	Perylene-d12	-----	ISTD-----						

Method Path : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\  
Method File : 8270-SIM-BN062125.M

36)	Indeno(1,2,3-c... 37)	Benzo(b)fluora... 38)	Benzo(k)fluora... 39) C	Benzo(a)pyrene 40)	Dibenzo(a,h)an... 41)	1.741 1.715 1.695 1.761 1.974 1.819 1.856 1.794 1.428 1.380 1.444 1.392 1.541 1.532 1.587 1.472 1.576 1.593 1.569 1.466 1.671 1.617 1.686 1.597 1.320 1.249 1.274 1.247 1.399 1.348 1.395 1.319 1.179 1.185 1.236 1.355 1.561 1.446 1.478 1.348 1.620 1.554 1.589 1.560 1.720 1.577 1.598 1.603	5.42 5.50 4.59 4.90 11.32 3.53
-----	--------------------------	--------------------------	----------------------------	-----------------------	--------------------------	--	---

(#) = Out of Range

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037353.D  
 Acq On : 20 Jun 2025 16:51  
 Operator : RC/JU  
 Sample : SSTDICCO.1  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

**Instrument :**  
BNA\_N  
**ClientSampleId :**  
SSTDICCO.1

Quant Time: Jun 20 23:26:13 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2463	0.400	ng	0.00
7) Naphthalene-d8	10.351	136	5110	0.400	ng	# 0.01
13) Acenaphthene-d10	14.213	164	3596	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	7299	0.400	ng	0.00
29) Chrysene-d12	21.171	240	6135	0.400	ng	0.00
35) Perylene-d12	23.357	264	6598	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.170	112	526	0.117	ng	0.00
5) Phenol-d6	6.752	99	481	0.108	ng	0.00
8) Nitrobenzene-d5	8.728	82	325	0.077	ng	0.01
11) 2-Methylnaphthalene-d10	11.955	152	791	0.096	ng	0.01
14) 2,4,6-Tribromophenol	15.730	330	197	0.077	ng	0.01
15) 2-Fluorobiphenyl	12.848	172	1533	0.097	ng	0.01
27) Fluoranthene-d10	19.012	212	2001	0.088	ng	0.00
31) Terphenyl-d14	19.625	244	1456	0.104	ng	0.00
<b>Target Compounds</b>						
				<b>Qvalue</b>		
6) bis(2-Chloroethyl)ether	7.004	93	443	0.114	ng	98
9) Naphthalene	10.394	128	1349	0.102	ng	98
10) Hexachlorobutadiene	10.682	225	578	0.089	ng	# 99
12) 2-Methylnaphthalene	12.026	142	898	0.096	ng	96
16) Acenaphthylene	13.935	152	1480	0.098	ng	98
17) Acenaphthene	14.277	154	996	0.100	ng	99
18) Fluorene	15.282	166	1348	0.095	ng	99
21) 4-Bromophenyl-phenylether	16.177	248	482	0.081	ng	# 95
22) Hexachlorobenzene	16.276	284	588	0.095	ng	98
23) Atrazine	16.450	200	404	0.087	ng	92
25) Phenanthrene	17.009	178	2021	0.098	ng	99
26) Anthracene	17.108	178	1812	0.094	ng	98
28) Fluoranthene	19.045	202	2576	0.091	ng	# 99
30) Pyrene	19.407	202	2647	0.113	ng	99
32) Benzo(a)anthracene	21.162	228	2007	0.101	ng	98
33) Chrysene	21.206	228	2687	0.107	ng	98
36) Indeno(1,2,3-cd)pyrene	25.550	276	2871	0.103	ng	# 98
37) Benzo(b)fluoranthene	22.708	252	2355	0.101	ng	# 75
38) Benzo(k)fluoranthene	22.749	252	2600	0.102	ng	# 79
39) Benzo(a)pyrene	23.263	252	2178	0.102	ng	# 60
40) Dibenzo(a,h)anthracene	25.567	278	1944	0.087	ng	# 78
41) Benzo(g,h,i)perylene	26.213	276	2673	0.104	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037353.D  
 Acq On : 20 Jun 2025 16:51  
 Operator : RC/JU  
 Sample : SSTDICCO.1  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCO.1

Quant Time: Jun 20 23:26:13 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


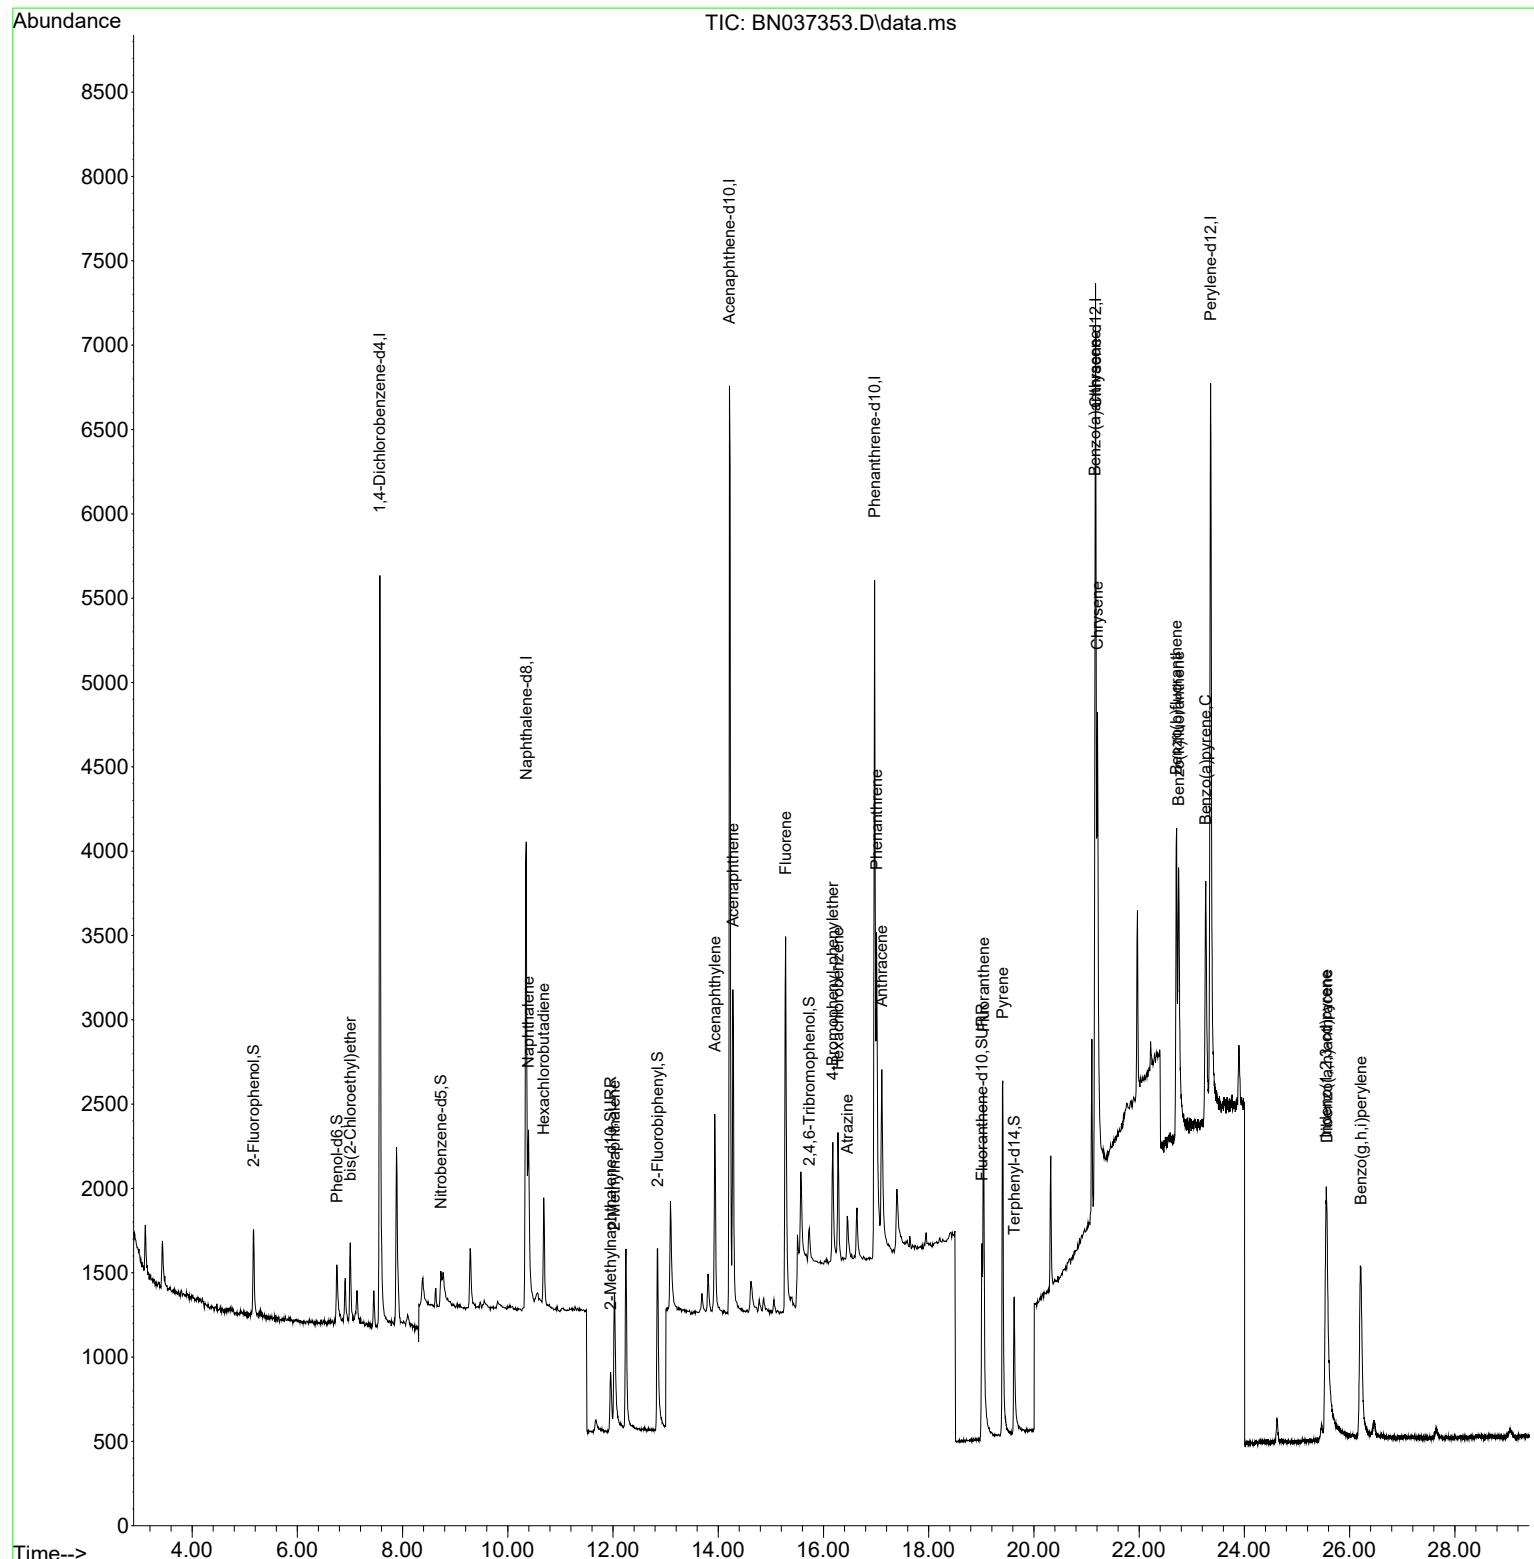


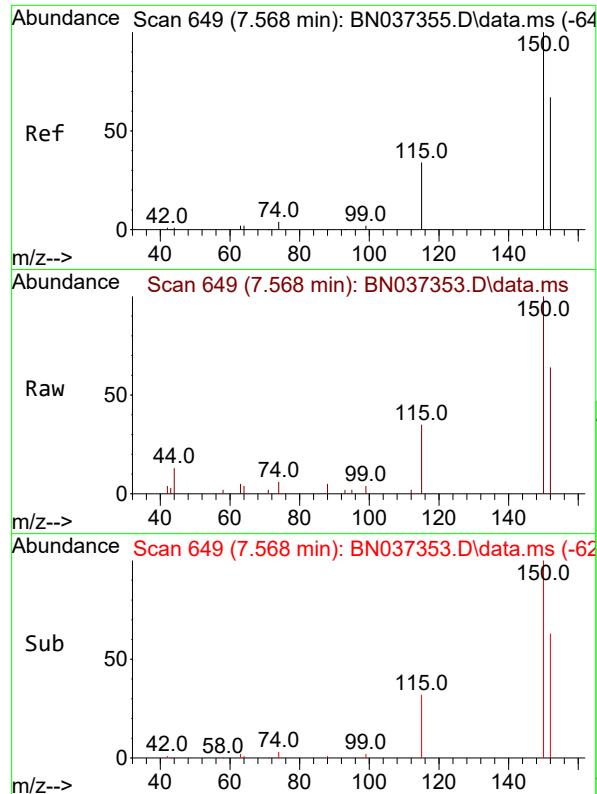

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


Tgt Ion:152 Resp: 2463  
Ion Ratio Lower Upper  
152 100  
150 155.8 112.7 169.1  
115 54.4 45.9 68.9

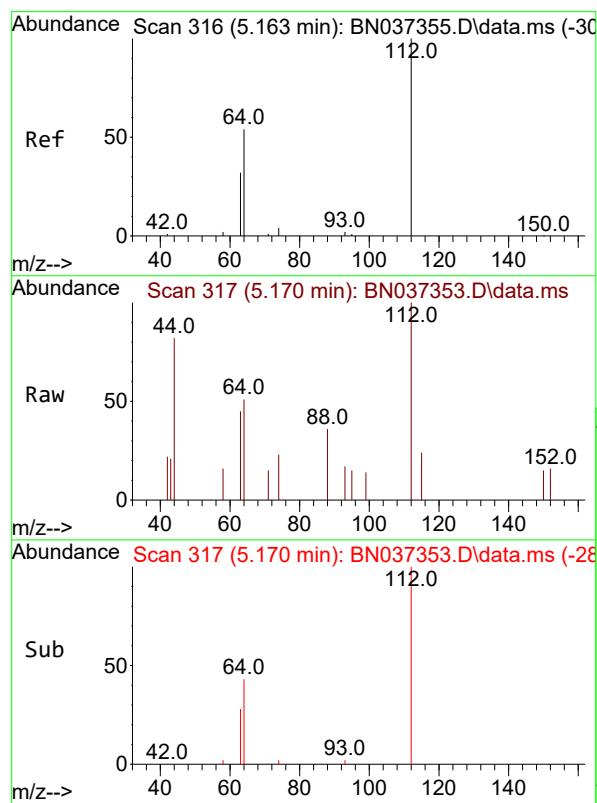

#4  
2-Fluorophenol  
Concen: 0.117 ng  
RT: 5.170 min Scan# 317  
Delta R.T. 0.007 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51

Tgt Ion:112 Resp: 526  
Ion Ratio Lower Upper  
112 100  
64 51.3 38.7 58.1  
63 37.1 26.4 39.6



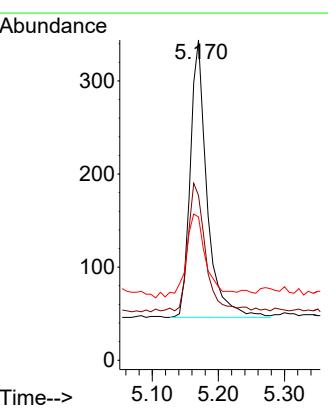


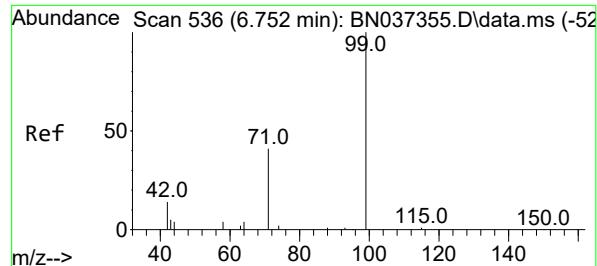

#5  
 Phenol-d6  
 Concen: 0.108 ng  
 RT: 6.752 min Scan# 5  
 Delta R.T. -0.000 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51




Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1




Tgt Ion: 99 Resp: 481  
 Ion Ratio Lower Upper  
 99 100  
 42 22.0 19.8 29.8  
 71 41.6 42.6 64.0#



#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.114 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. -0.000 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion: 93 Resp: 443  
 Ion Ratio Lower Upper  
 93 100  
 63 68.4 53.2 79.8  
 95 34.5 27.3 40.9

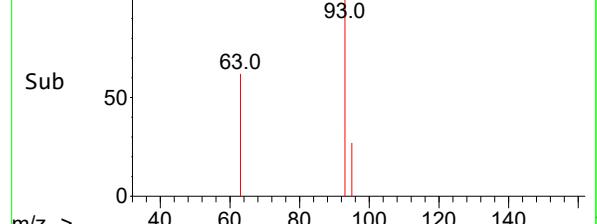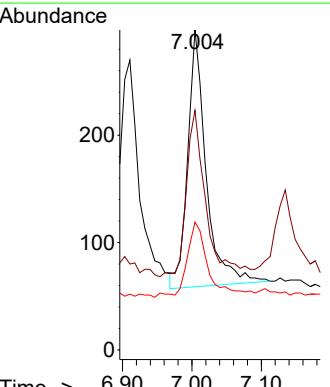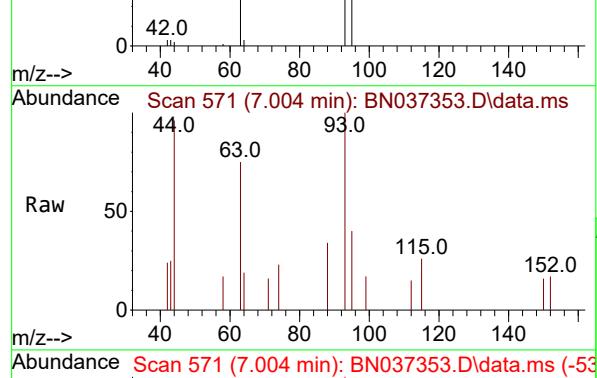







#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.351 min Scan# 9  
 Delta R.T. 0.011 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1

Tgt Ion:136 Resp: 5110

Ion Ratio Lower Upper

136	100		
137	13.2	12.2	18.2
54	6.6	8.8	13.2#
68	5.2	7.0	10.4#

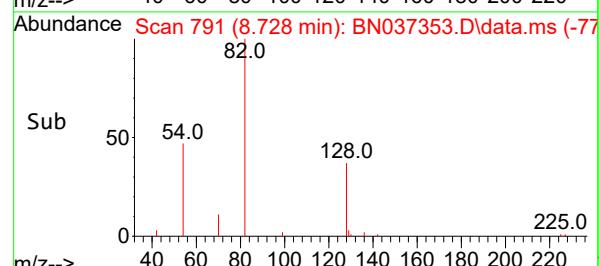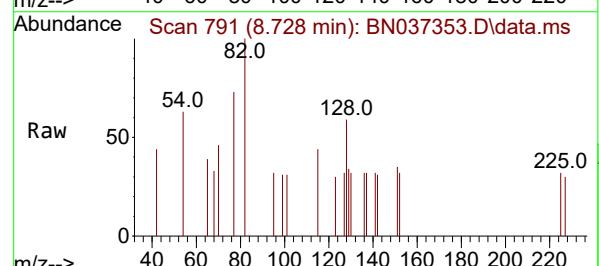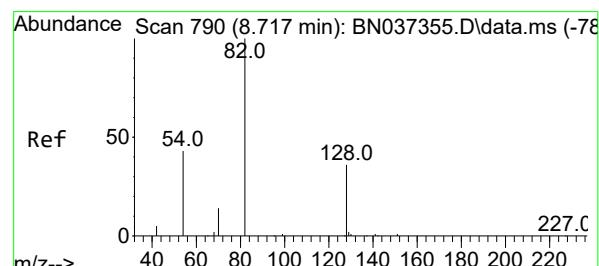





#8  
 Nitrobenzene-d5  
 Concen: 0.077 ng  
 RT: 8.728 min Scan# 791  
 Delta R.T. 0.011 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion: 82 Resp: 325

Ion Ratio Lower Upper

82	100		
128	58.7	42.5	63.7
54	62.6	43.2	64.8



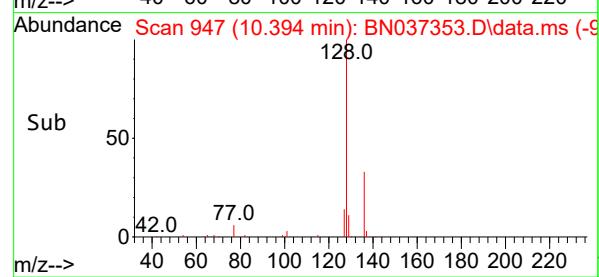

#9

Naphthalene

Concen: 0.102 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037353.D

Acq: 20 Jun 2025 16:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.1





Tgt Ion:128 Resp: 1349

Ion Ratio Lower Upper

128 100

129 18.2 14.0 21.0

127 20.6 15.8 23.8

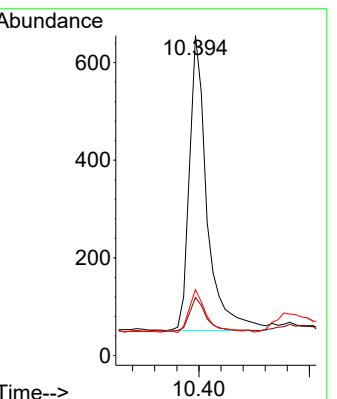

#10

Hexachlorobutadiene

Concen: 0.089 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037353.D

Acq: 20 Jun 2025 16:51


Tgt Ion:225 Resp: 578




Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 62.1 50.3 75.5

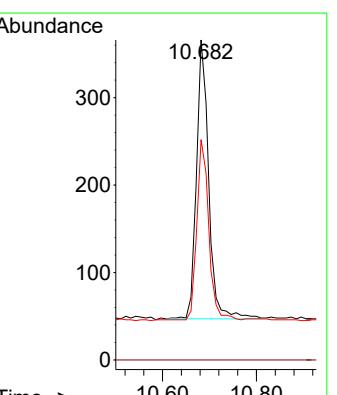



#11

2-Methylnaphthalene-d10

Concen: 0.096 ng

RT: 11.955 min Scan# 1

Delta R.T. 0.010 min

Lab File: BN037353.D




Acq: 20 Jun 2025 16:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICC0.1



#12

2-Methylnaphthalene

Concen: 0.096 ng

RT: 12.026 min Scan# 1154

Delta R.T. 0.005 min

Lab File: BN037353.D

Acq: 20 Jun 2025 16:51




Tgt Ion:142 Resp: 898


Ion Ratio Lower Upper

142 100

141 90.9 70.2 105.2

115 50.1 43.0 64.4

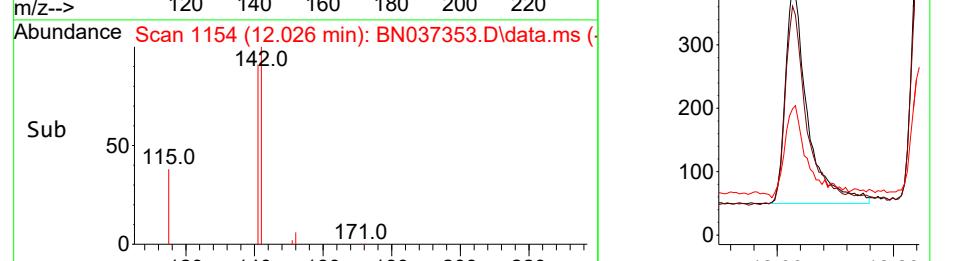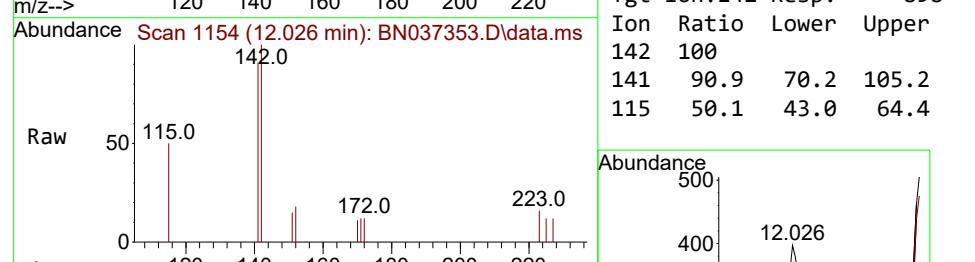
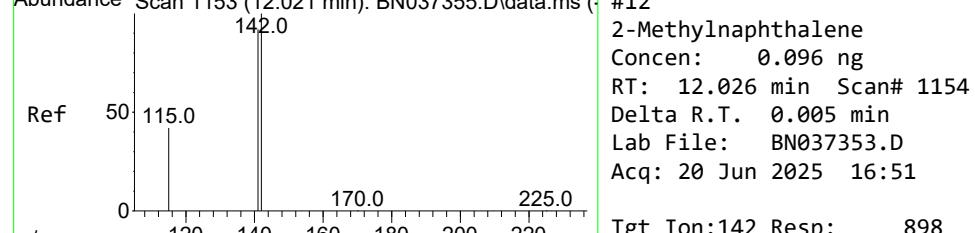


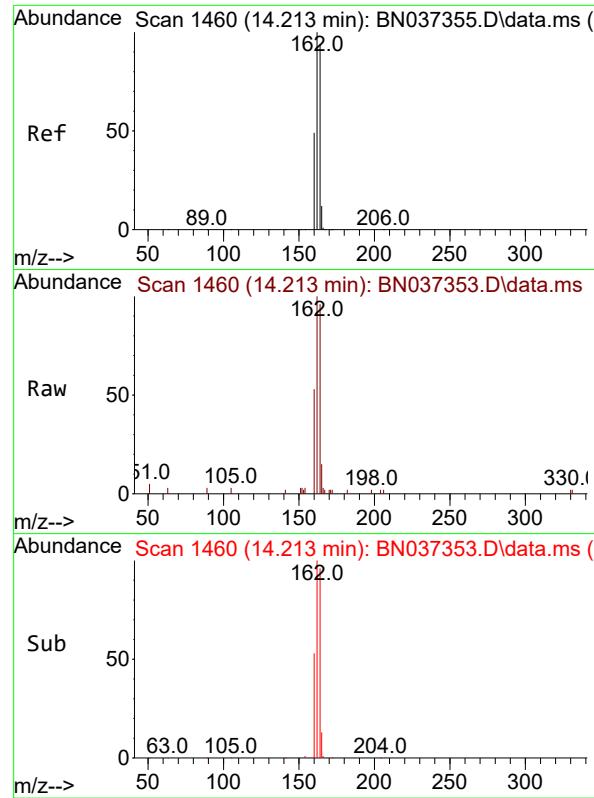

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


Tgt Ion:164 Resp: 3596  
Ion Ratio Lower Upper  
164 100  
162 104.3 81.5 122.3  
160 55.8 43.0 64.4

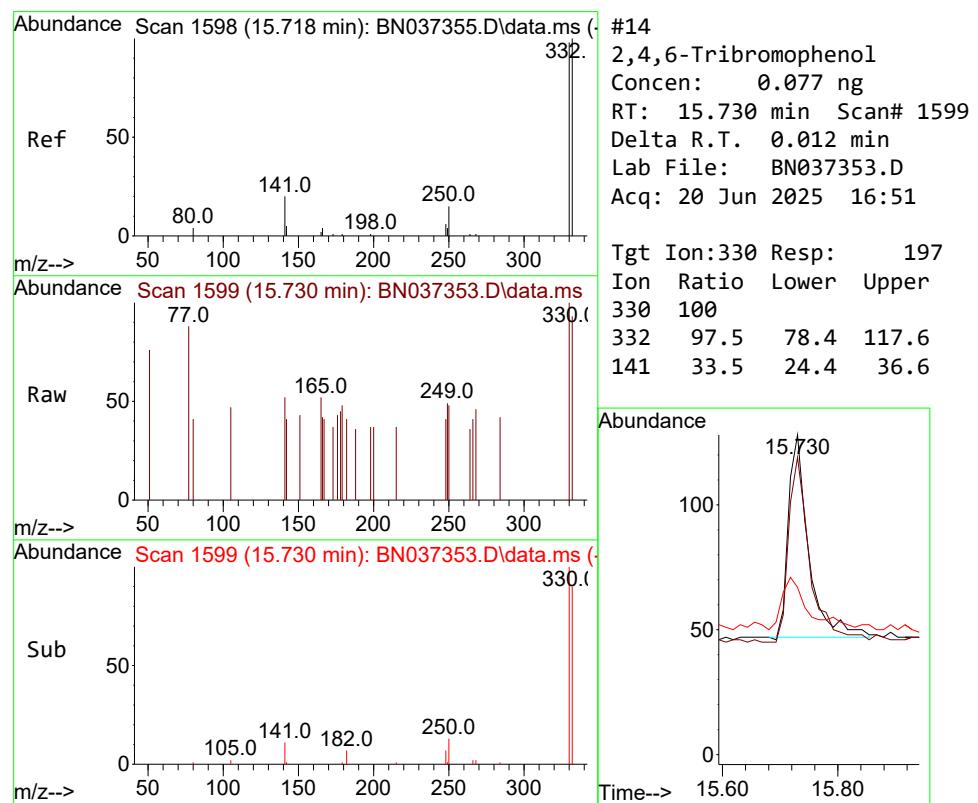

#14  
2,4,6-Tribromophenol  
Concen: 0.077 ng  
RT: 15.730 min Scan# 1599  
Delta R.T. 0.012 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51



Tgt Ion:330 Resp: 197  
Ion Ratio Lower Upper  
330 100  
332 97.5 78.4 117.6  
141 33.5 24.4 36.6

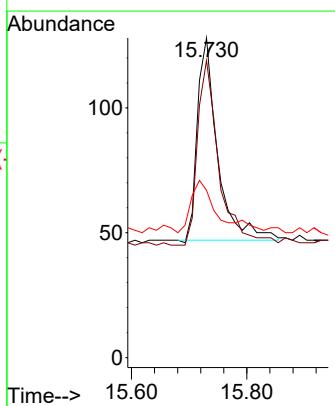

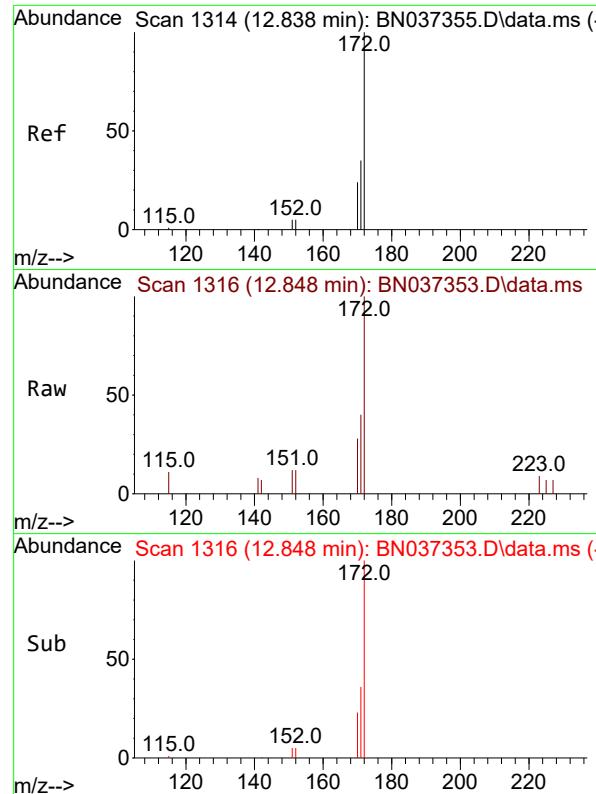


#15  
2-Fluorobiphenyl  
Concen: 0.097 ng  
RT: 12.848 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.010 min  
Lab File: BN037353.D ClientSampleId : SSTDICCO.1  
Acq: 20 Jun 2025 16:51




Tgt Ion:172 Resp: 1533  
Ion Ratio Lower Upper  
172 100  
171 40.1 30.8 46.2  
170 28.2 21.9 32.9

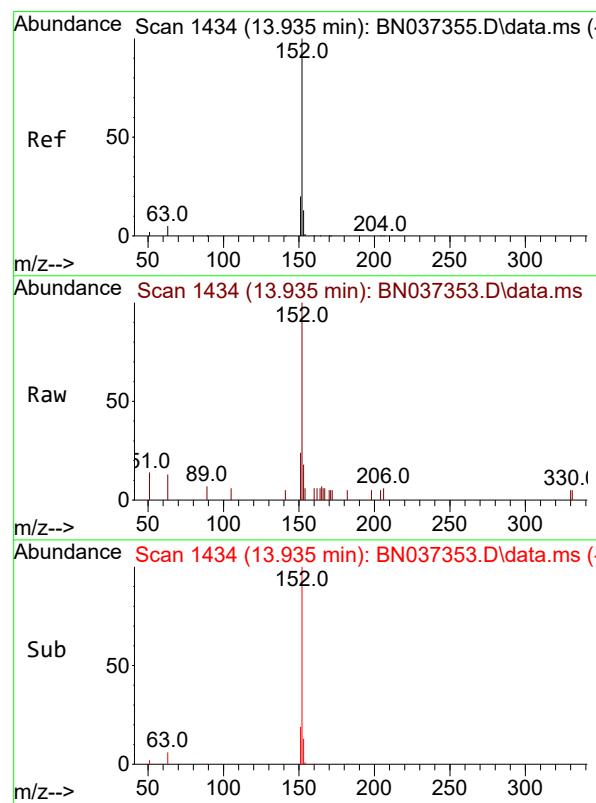

#16  
Acenaphthylene  
Concen: 0.098 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51

Tgt Ion:152 Resp: 1480  
Ion Ratio Lower Upper  
152 100  
151 19.5 16.6 24.8  
153 13.2 10.2 15.2



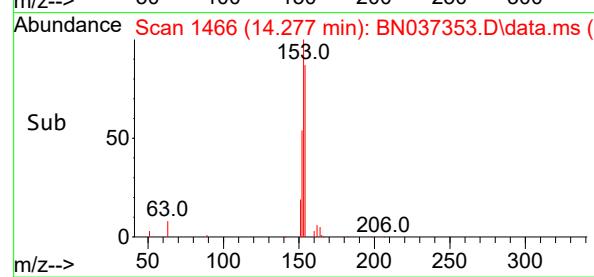

#17

Acenaphthene

Concen: 0.100 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037353.D

Acq: 20 Jun 2025 16:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.1





Tgt Ion:154 Resp: 996

Ion Ratio Lower Upper

154 100

153 116.2 93.1 139.7

152 62.9 48.6 73.0

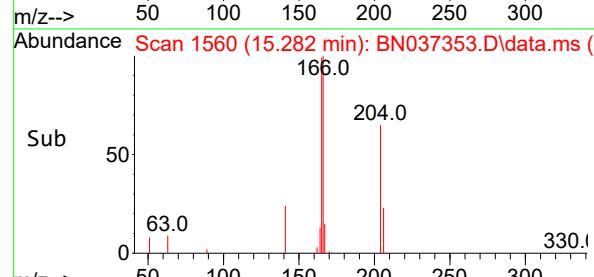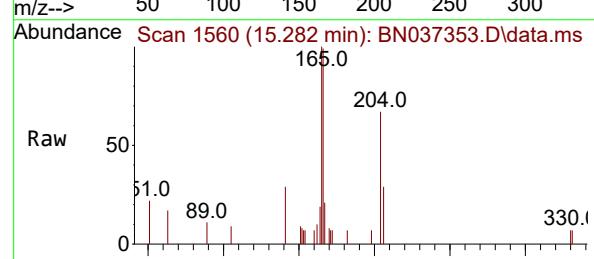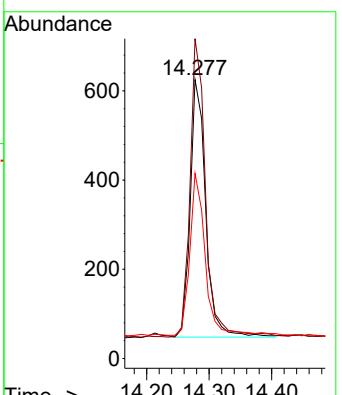

#18

Fluorene

Concen: 0.095 ng

RT: 15.282 min Scan# 1560

Delta R.T. 0.011 min

Lab File: BN037353.D

Acq: 20 Jun 2025 16:51


Tgt Ion:166 Resp: 1348


Ion Ratio Lower Upper

166 100

165 99.0 79.5 119.3

167 15.1 10.7 16.1


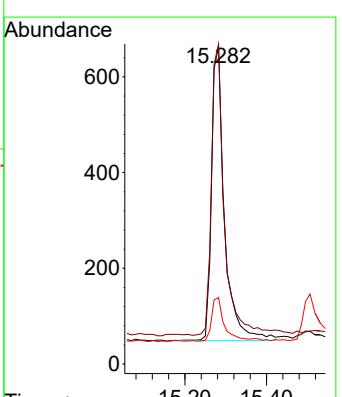


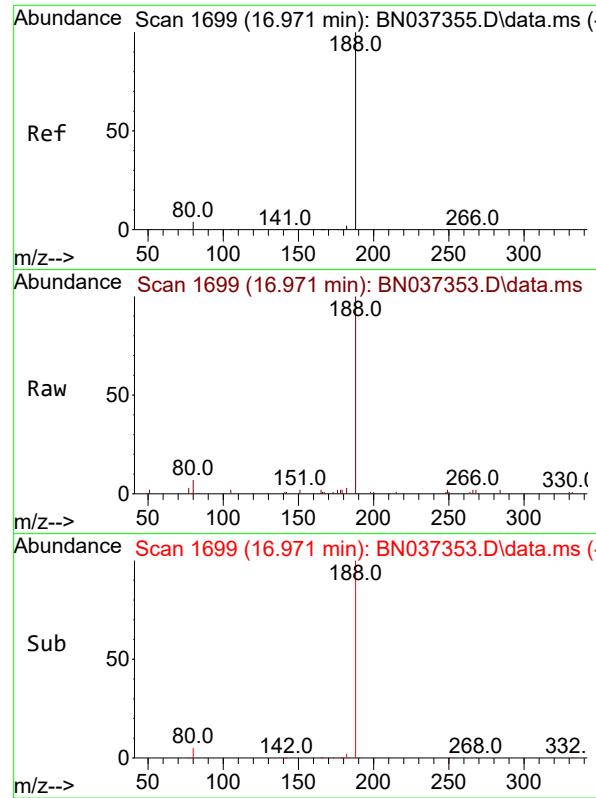

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1



Tgt Ion:188 Resp: 7299  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 6.5 6.2 9.2

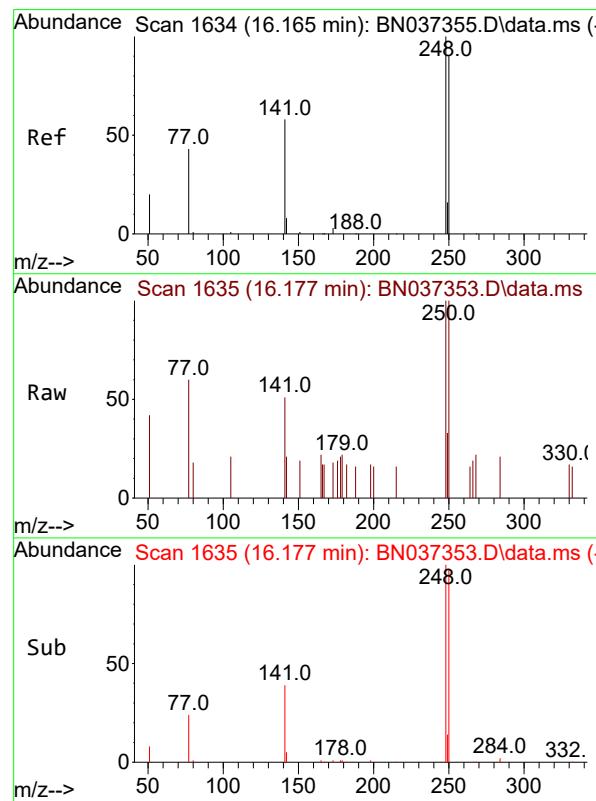

#21  
 4-Bromophenyl-phenylether  
 Concen: 0.081 ng  
 RT: 16.177 min Scan# 1635  
 Delta R.T. 0.012 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion:248 Resp: 482  
 Ion Ratio Lower Upper  
 248 100  
 250 99.7 80.4 120.6  
 141 50.5 33.3 49.9#

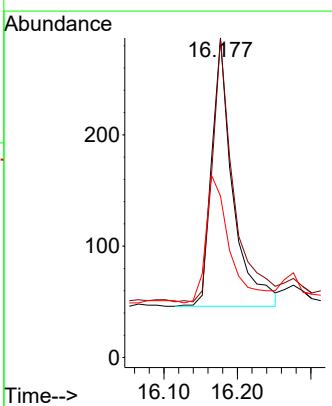

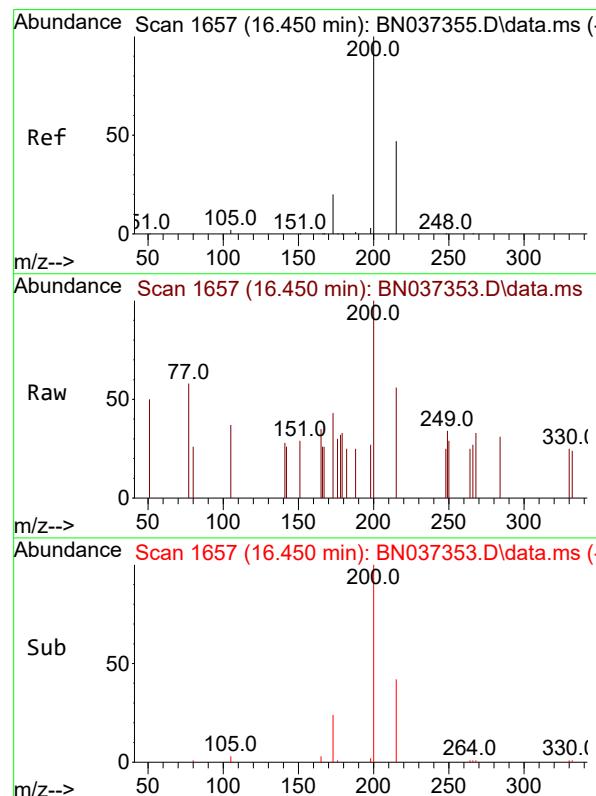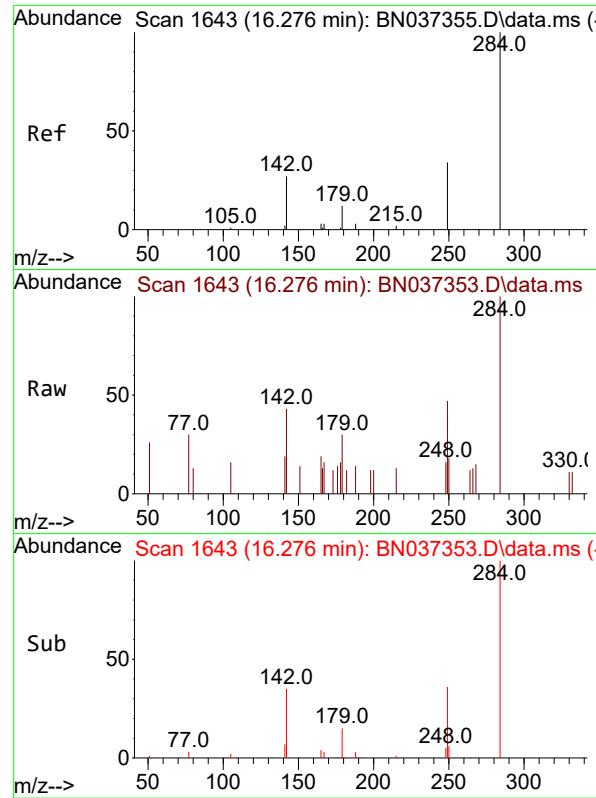


Instrument : BNA\_N

ClientSampleId : SSTDICCO.1

Tgt Ion:284 Resp: 588

Ion	Ratio	Lower	Upper
284	100		
142	35.9	27.0	40.6
249	36.7	28.8	43.2



#23

Atrazine

Concen: 0.087 ng

RT: 16.450 min Scan# 1657


Delta R.T. -0.000 min


Lab File: BN037353.D

Acq: 20 Jun 2025 16:51

Tgt Ion:200 Resp: 404

Ion	Ratio	Lower	Upper
200	100		
173	42.6	29.2	43.8
215	56.3	48.8	73.2


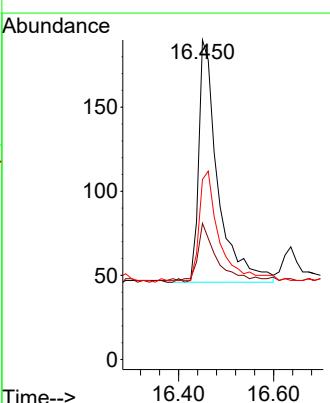


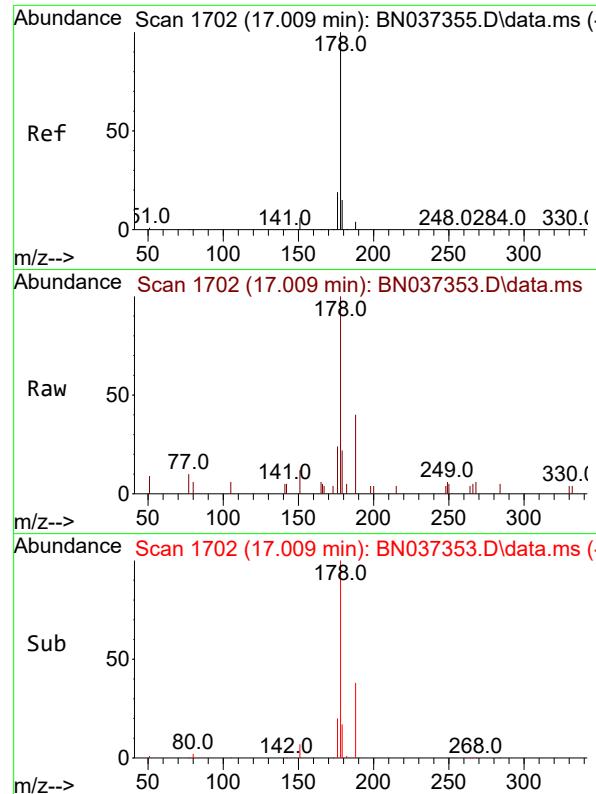

#25  
 Phenanthrene  
 Concen: 0.098 ng  
 RT: 17.009 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:178 Resp: 2021  
 Ion Ratio Lower Upper  
 178 100  
 176 19.4 15.2 22.8  
 179 16.8 12.9 19.3

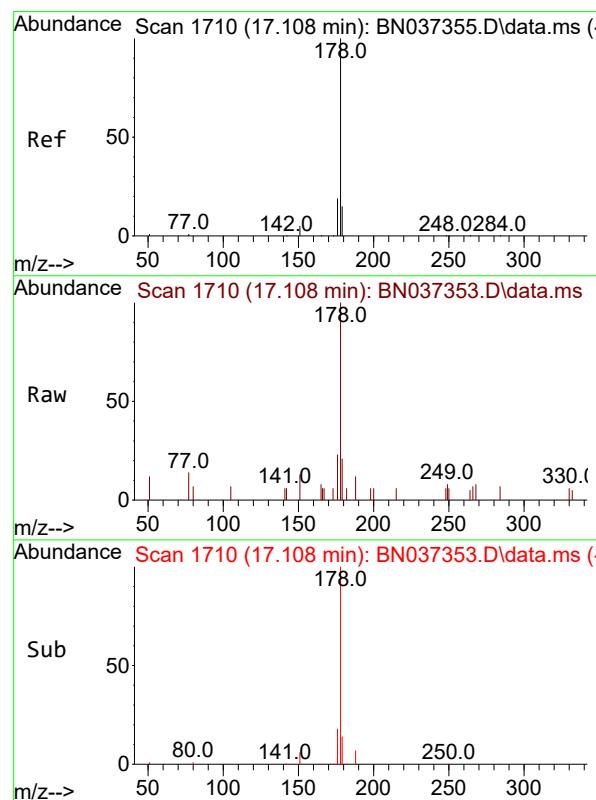

#26  
 Anthracene  
 Concen: 0.094 ng  
 RT: 17.108 min Scan# 1710  
 Delta R.T. -0.000 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion:178 Resp: 1812  
 Ion Ratio Lower Upper  
 178 100  
 176 18.8 14.7 22.1  
 179 14.8 13.0 19.6





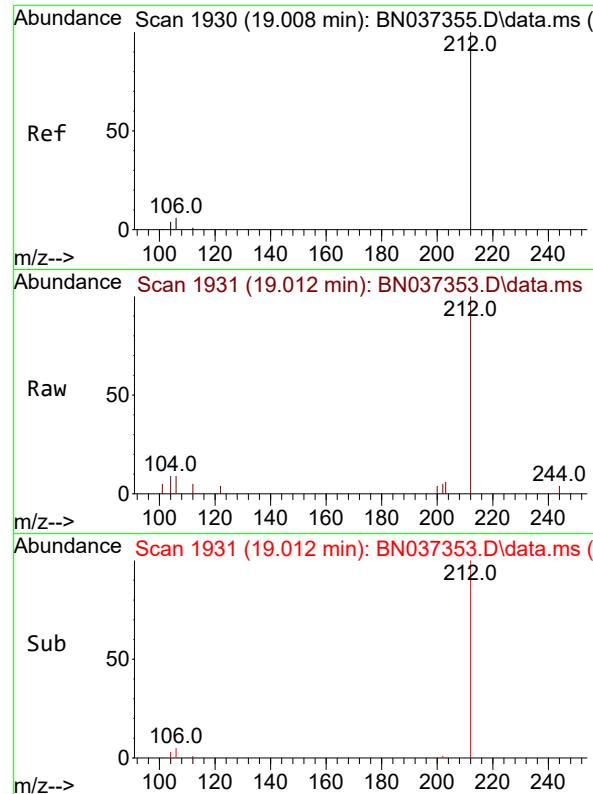

#27  
 Fluoranthene-d10  
 Concen: 0.088 ng  
 RT: 19.012 min Scan# 1  
 Delta R.T. 0.005 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:212 Resp: 2001  
 Ion Ratio Lower Upper  
 212 100  
 106 5.8 3.0 4.4#  
 104 4.1 2.0 3.0#

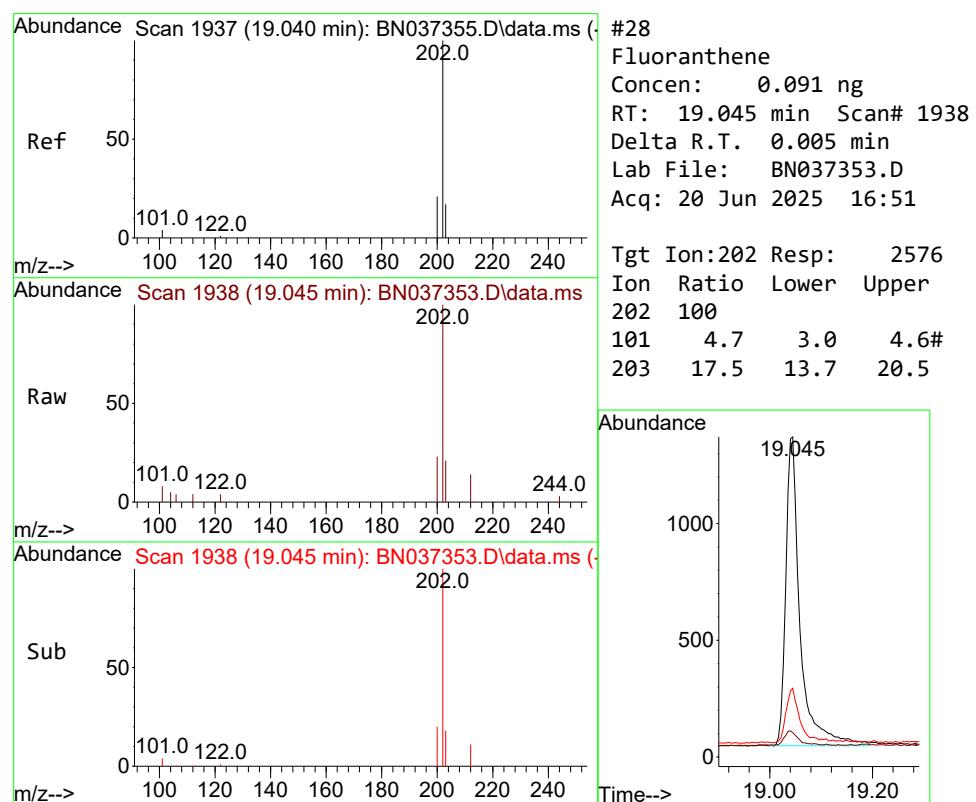

#28  
 Fluoranthene  
 Concen: 0.091 ng  
 RT: 19.045 min Scan# 1938  
 Delta R.T. 0.005 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion:202 Resp: 2576  
 Ion Ratio Lower Upper  
 202 100  
 101 4.7 3.0 4.6#  
 203 17.5 13.7 20.5


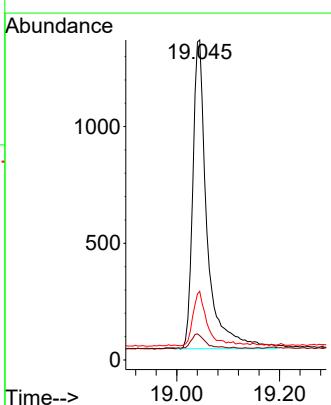


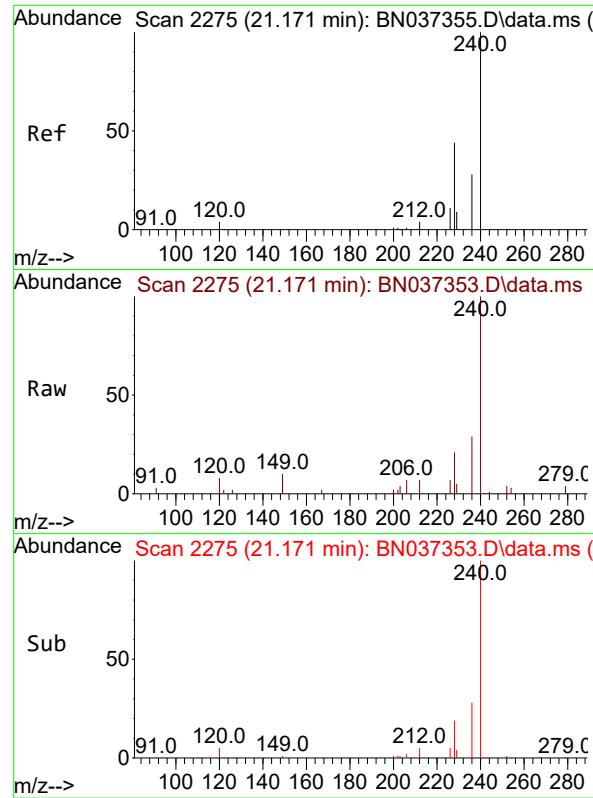

#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.171 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


Tgt Ion:240 Resp: 6135  
Ion Ratio Lower Upper  
240 100  
120 7.9 7.5 11.3  
236 29.3 24.9 37.3

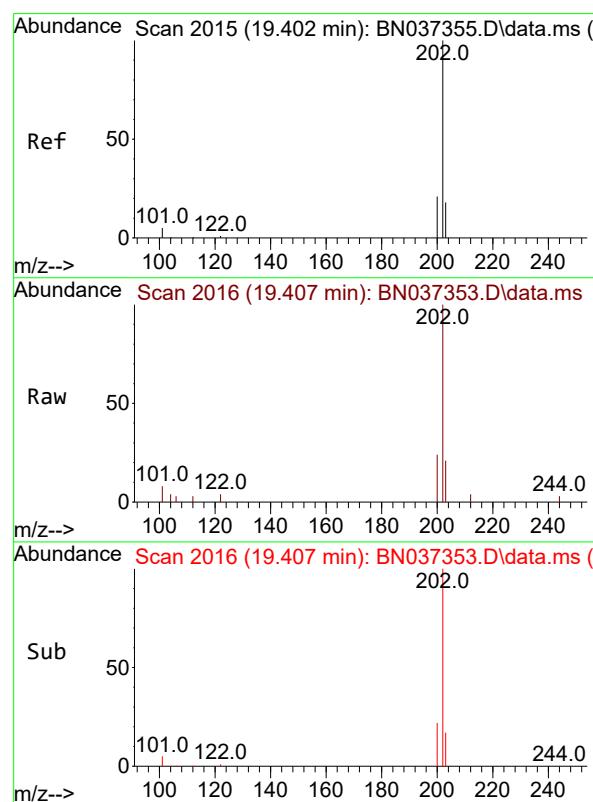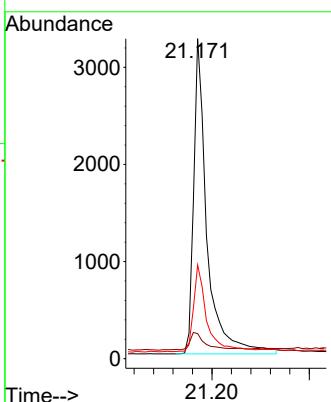

#30  
Pyrene  
Concen: 0.113 ng  
RT: 19.407 min Scan# 2016  
Delta R.T. 0.005 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51

Tgt Ion:202 Resp: 2647  
Ion Ratio Lower Upper  
202 100  
200 21.1 16.8 25.2  
203 17.4 14.5 21.7





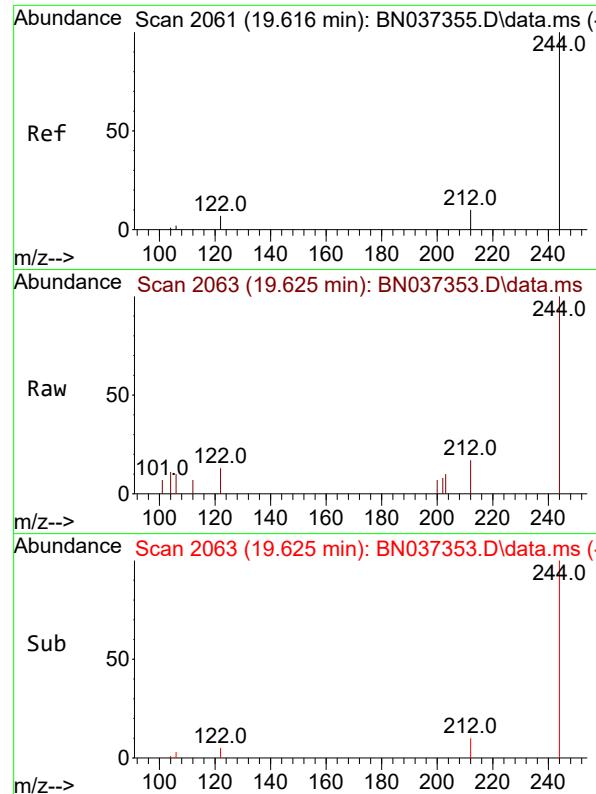

#31  
 Terphenyl-d14  
 Concen: 0.104 ng  
 RT: 19.625 min Scan# 2  
 Delta R.T. 0.009 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:244 Resp: 1456  
 Ion Ratio Lower Upper  
 244 100  
 212 16.7 11.1 16.7#  
 122 12.7 7.2 10.8#

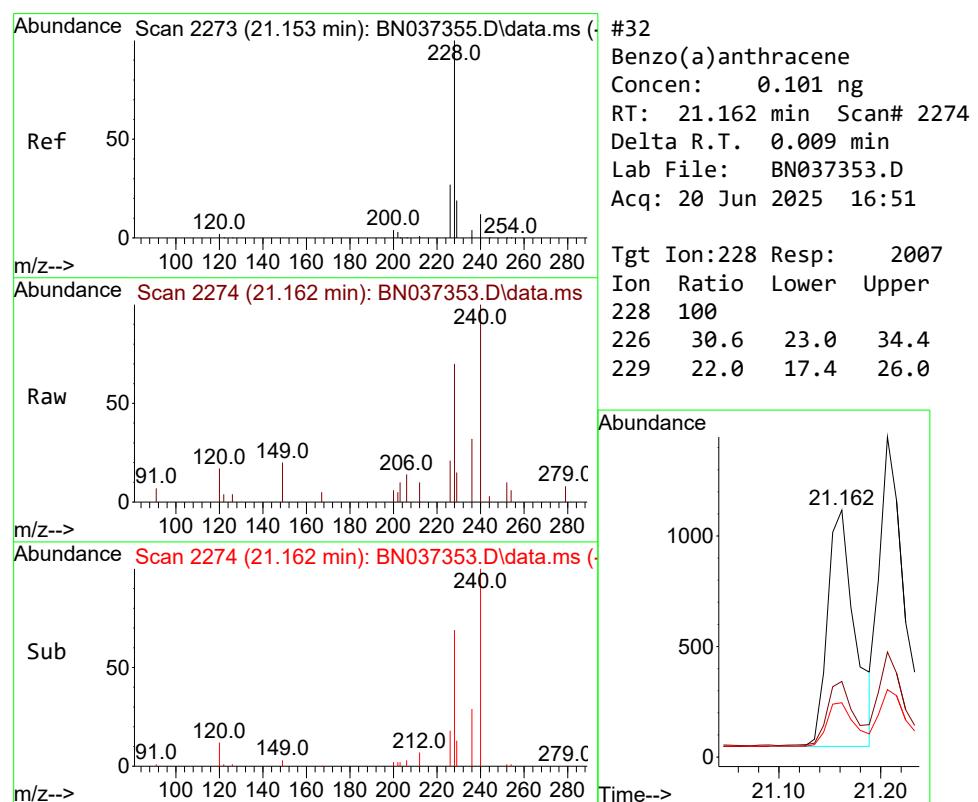

#32  
 Benzo(a)anthracene  
 Concen: 0.101 ng  
 RT: 21.162 min Scan# 2274  
 Delta R.T. 0.009 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion:228 Resp: 2007  
 Ion Ratio Lower Upper  
 228 100  
 226 30.6 23.0 34.4  
 229 22.0 17.4 26.0





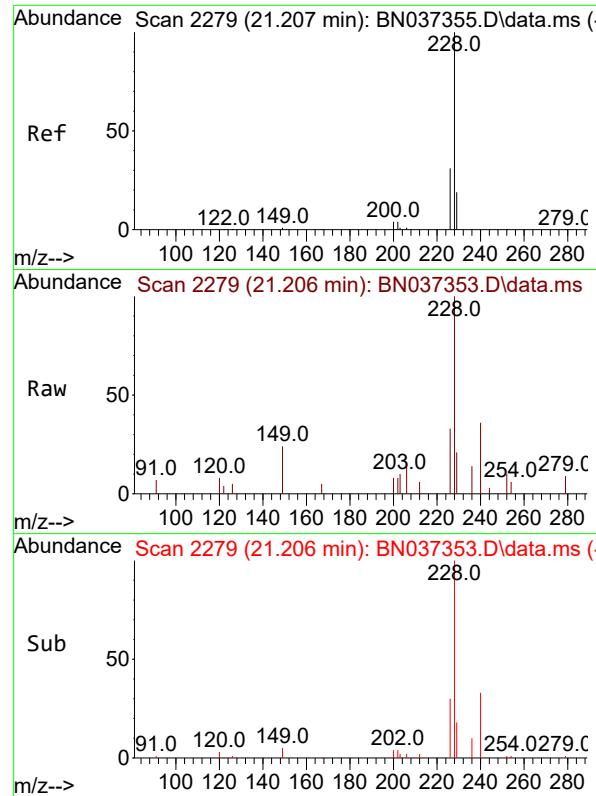

#33  
 Chrysene  
 Concen: 0.107 ng  
 RT: 21.206 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:228 Resp: 2687  
 Ion Ratio Lower Upper  
 228 100  
 226 32.8 25.4 38.2  
 229 21.1 17.3 25.9

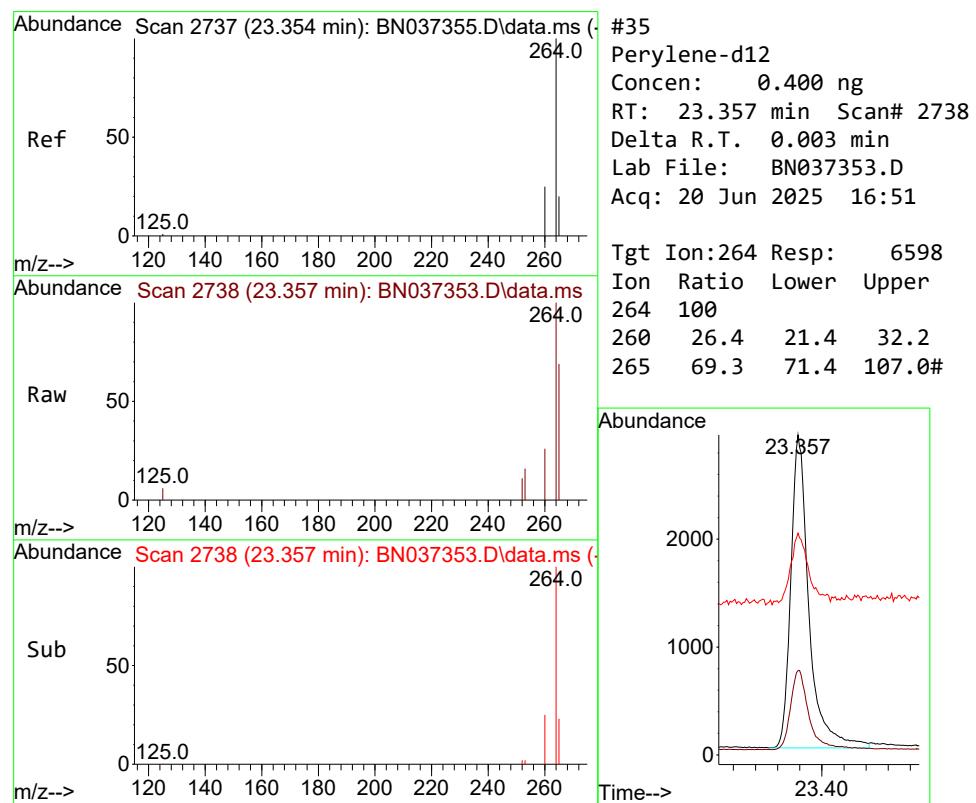

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.357 min Scan# 2738  
 Delta R.T. 0.003 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion:264 Resp: 6598  
 Ion Ratio Lower Upper  
 264 100  
 260 26.4 21.4 32.2  
 265 69.3 71.4 107.0#





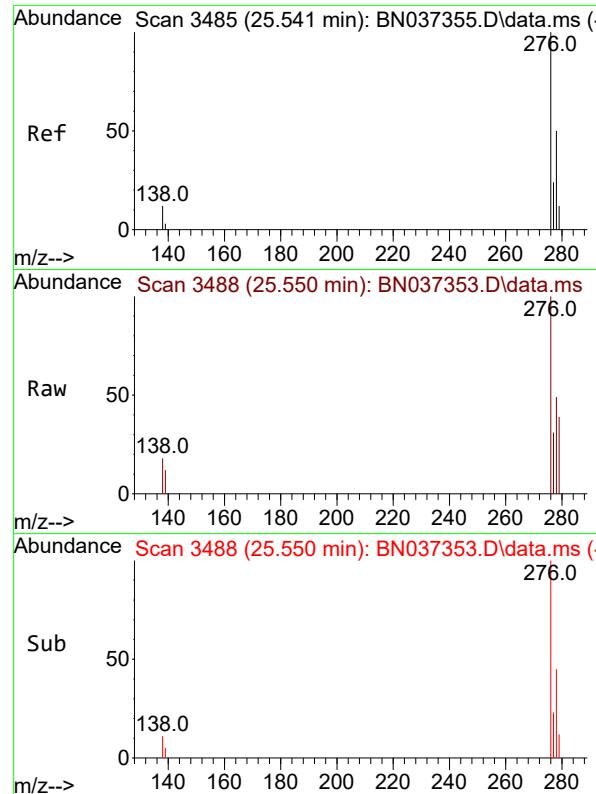

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.103 ng  
RT: 25.550 min Scan# 34  
Delta R.T. 0.009 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


Tgt Ion:276 Resp: 2871  
Ion Ratio Lower Upper  
276 100  
138 4.2 2.2 3.2#  
277 22.3 17.1 25.7

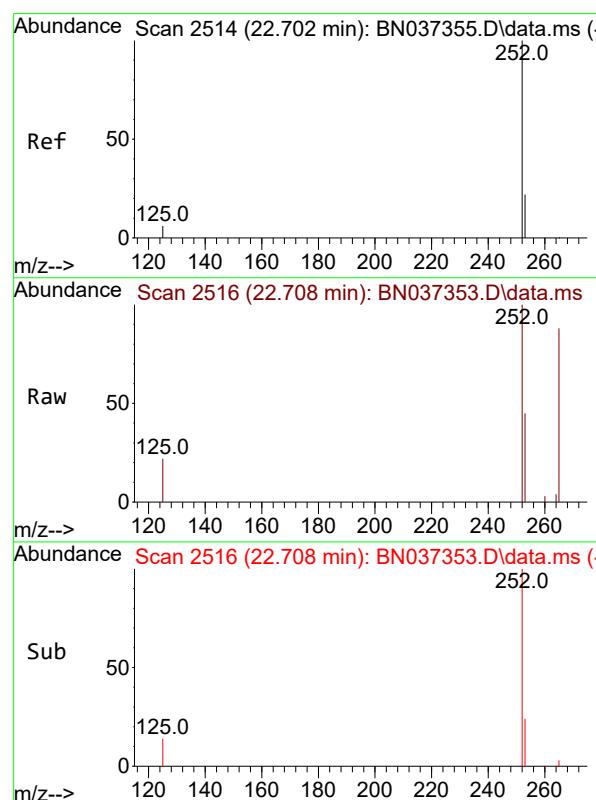

#37  
Benzo(b)fluoranthene  
Concen: 0.101 ng  
RT: 22.708 min Scan# 2516  
Delta R.T. 0.006 min  
Lab File: BN037353.D  
Acq: 20 Jun 2025 16:51

Tgt Ion:252 Resp: 2355  
Ion Ratio Lower Upper  
252 100  
253 45.5 26.6 40.0#  
125 22.4 6.1 9.1#



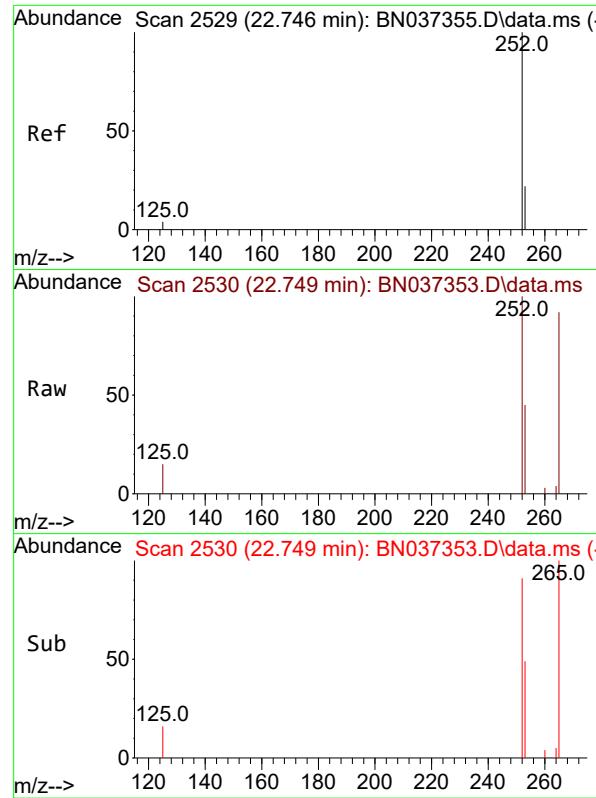

#38

Benzo(k)fluoranthene

Concen: 0.102 ng

RT: 22.749 min Scan# 2

Delta R.T. 0.003 min

Lab File: BN037353.D

Acq: 20 Jun 2025 16:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.1


Tgt Ion:252 Resp: 2600

Ion Ratio Lower Upper

252 100

253 45.5 26.7 40.1#

125 15.1 6.5 9.7#



#39

Benzo(a)pyrene

Concen: 0.102 ng

RT: 23.263 min Scan# 2706

Delta R.T. 0.006 min

Lab File: BN037353.D

Acq: 20 Jun 2025 16:51



Tgt Ion:252 Resp: 2178


Ion Ratio Lower Upper

252 100

253 58.7 31.6 47.4#

125 37.6 8.4 12.6#

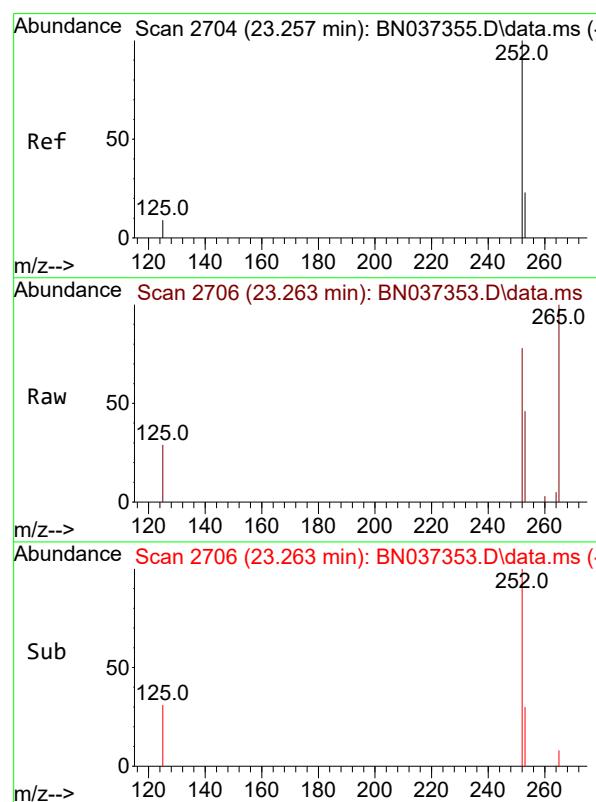



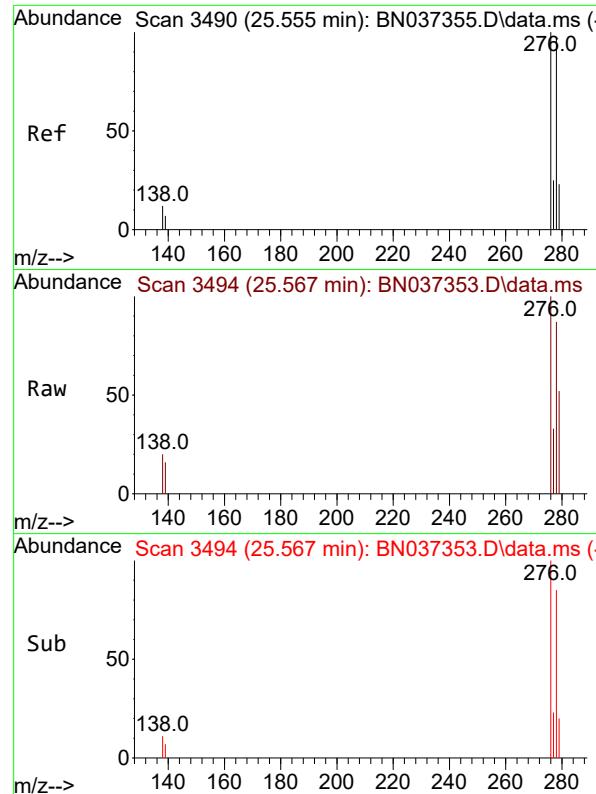

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.087 ng  
 RT: 25.567 min Scan# 3490  
 Delta R.T. 0.012 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1

Tgt Ion:278 Resp: 1944  
 Ion Ratio Lower Upper  
 278 100  
 139 18.8 10.2 15.4#  
 279 60.3 35.6 53.4#

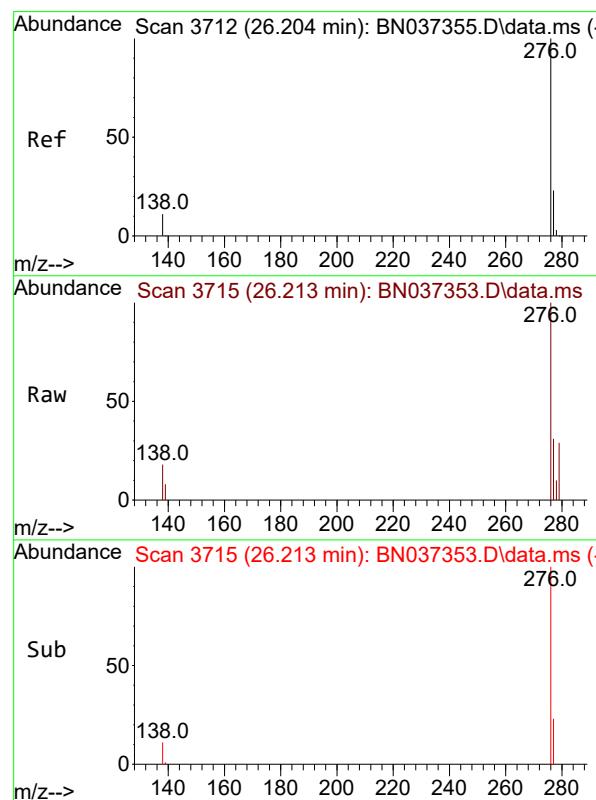

#41  
 Benzo(g,h,i)perylene  
 Concen: 0.104 ng  
 RT: 26.213 min Scan# 3715  
 Delta R.T. 0.009 min  
 Lab File: BN037353.D  
 Acq: 20 Jun 2025 16:51

Tgt Ion:276 Resp: 2673  
 Ion Ratio Lower Upper  
 276 100  
 277 30.6 22.7 34.1  
 138 18.2 9.4 14.2#

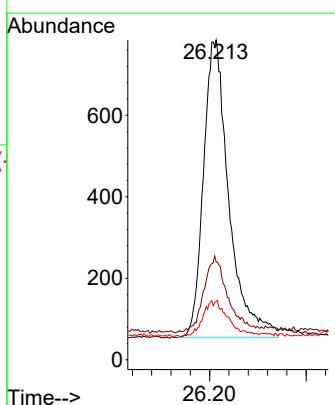

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037354.D  
 Acq On : 20 Jun 2025 17:27  
 Operator : RC/JU  
 Sample : SSTDICCO.2  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCO.2

Quant Time: Jun 20 23:26:34 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1865	0.400	ng	0.00
7) Naphthalene-d8	10.351	136	3983	0.400	ng	# 0.01
13) Acenaphthene-d10	14.213	164	2790	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5628	0.400	ng	0.00
29) Chrysene-d12	21.171	240	4640	0.400	ng	0.00
35) Perylene-d12	23.354	264	4914	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.170	112	763	0.224	ng	0.00
5) Phenol-d6	6.752	99	714	0.212	ng	0.00
8) Nitrobenzene-d5	8.728	82	582	0.176	ng	0.01
11) 2-Methylnaphthalene-d10	11.950	152	1271	0.197	ng	0.00
14) 2,4,6-Tribromophenol	15.730	330	315	0.158	ng	0.01
15) 2-Fluorobiphenyl	12.843	172	2337	0.191	ng	0.00
27) Fluoranthene-d10	19.008	212	3010	0.172	ng	0.00
31) Terphenyl-d14	19.621	244	2114	0.200	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	472	0.287	ng	98
3) n-Nitrosodimethylamine	3.422	42	366	0.191	ng	# 79
6) bis(2-Chloroethyl)ether	7.012	93	509	0.172	ng	95
9) Naphthalene	10.394	128	2104	0.204	ng	94
10) Hexachlorobutadiene	10.682	225	864	0.171	ng	# 99
12) 2-Methylnaphthalene	12.026	142	1379	0.190	ng	93
16) Acenaphthylene	13.935	152	2282	0.195	ng	97
17) Acenaphthene	14.277	154	1492	0.192	ng	99
18) Fluorene	15.282	166	2051	0.186	ng	100
20) 4,6-Dinitro-2-methylph...	15.378	198	196	0.115	ng	# 68
21) 4-Bromophenyl-phenylether	16.177	248	750	0.163	ng	96
22) Hexachlorobenzene	16.276	284	898	0.187	ng	98
23) Atrazine	16.450	200	604	0.168	ng	96
24) Pentachlorophenol	16.636	266	369	0.140	ng	97
25) Phenanthrene	17.009	178	3024	0.190	ng	98
26) Anthracene	17.108	178	2769	0.186	ng	97
28) Fluoranthene	19.040	202	3780	0.174	ng	# 98
30) Pyrene	19.402	202	3921	0.221	ng	99
32) Benzo(a)anthracene	21.153	228	2710	0.181	ng	98
33) Chrysene	21.206	228	3959	0.208	ng	99
34) Bis(2-ethylhexyl)phtha...	21.099	149	1406	0.229	ng	98
36) Indeno(1,2,3-cd)pyrene	25.547	276	4213	0.202	ng	# 95
37) Benzo(b)fluoranthene	22.702	252	3390	0.195	ng	# 90
38) Benzo(k)fluoranthene	22.746	252	3913	0.207	ng	# 90
39) Benzo(a)pyrene	23.260	252	3070	0.193	ng	# 79
40) Dibenzo(a,h)anthracene	25.564	278	2911	0.175	ng	# 93
41) Benzo(g,h,i)perylene	26.207	276	3819	0.200	ng	# 96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037354.D  
 Acq On : 20 Jun 2025 17:27  
 Operator : RC/JU  
 Sample : SSTDICCO.2  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCO.2

Quant Time: Jun 20 23:26:34 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration



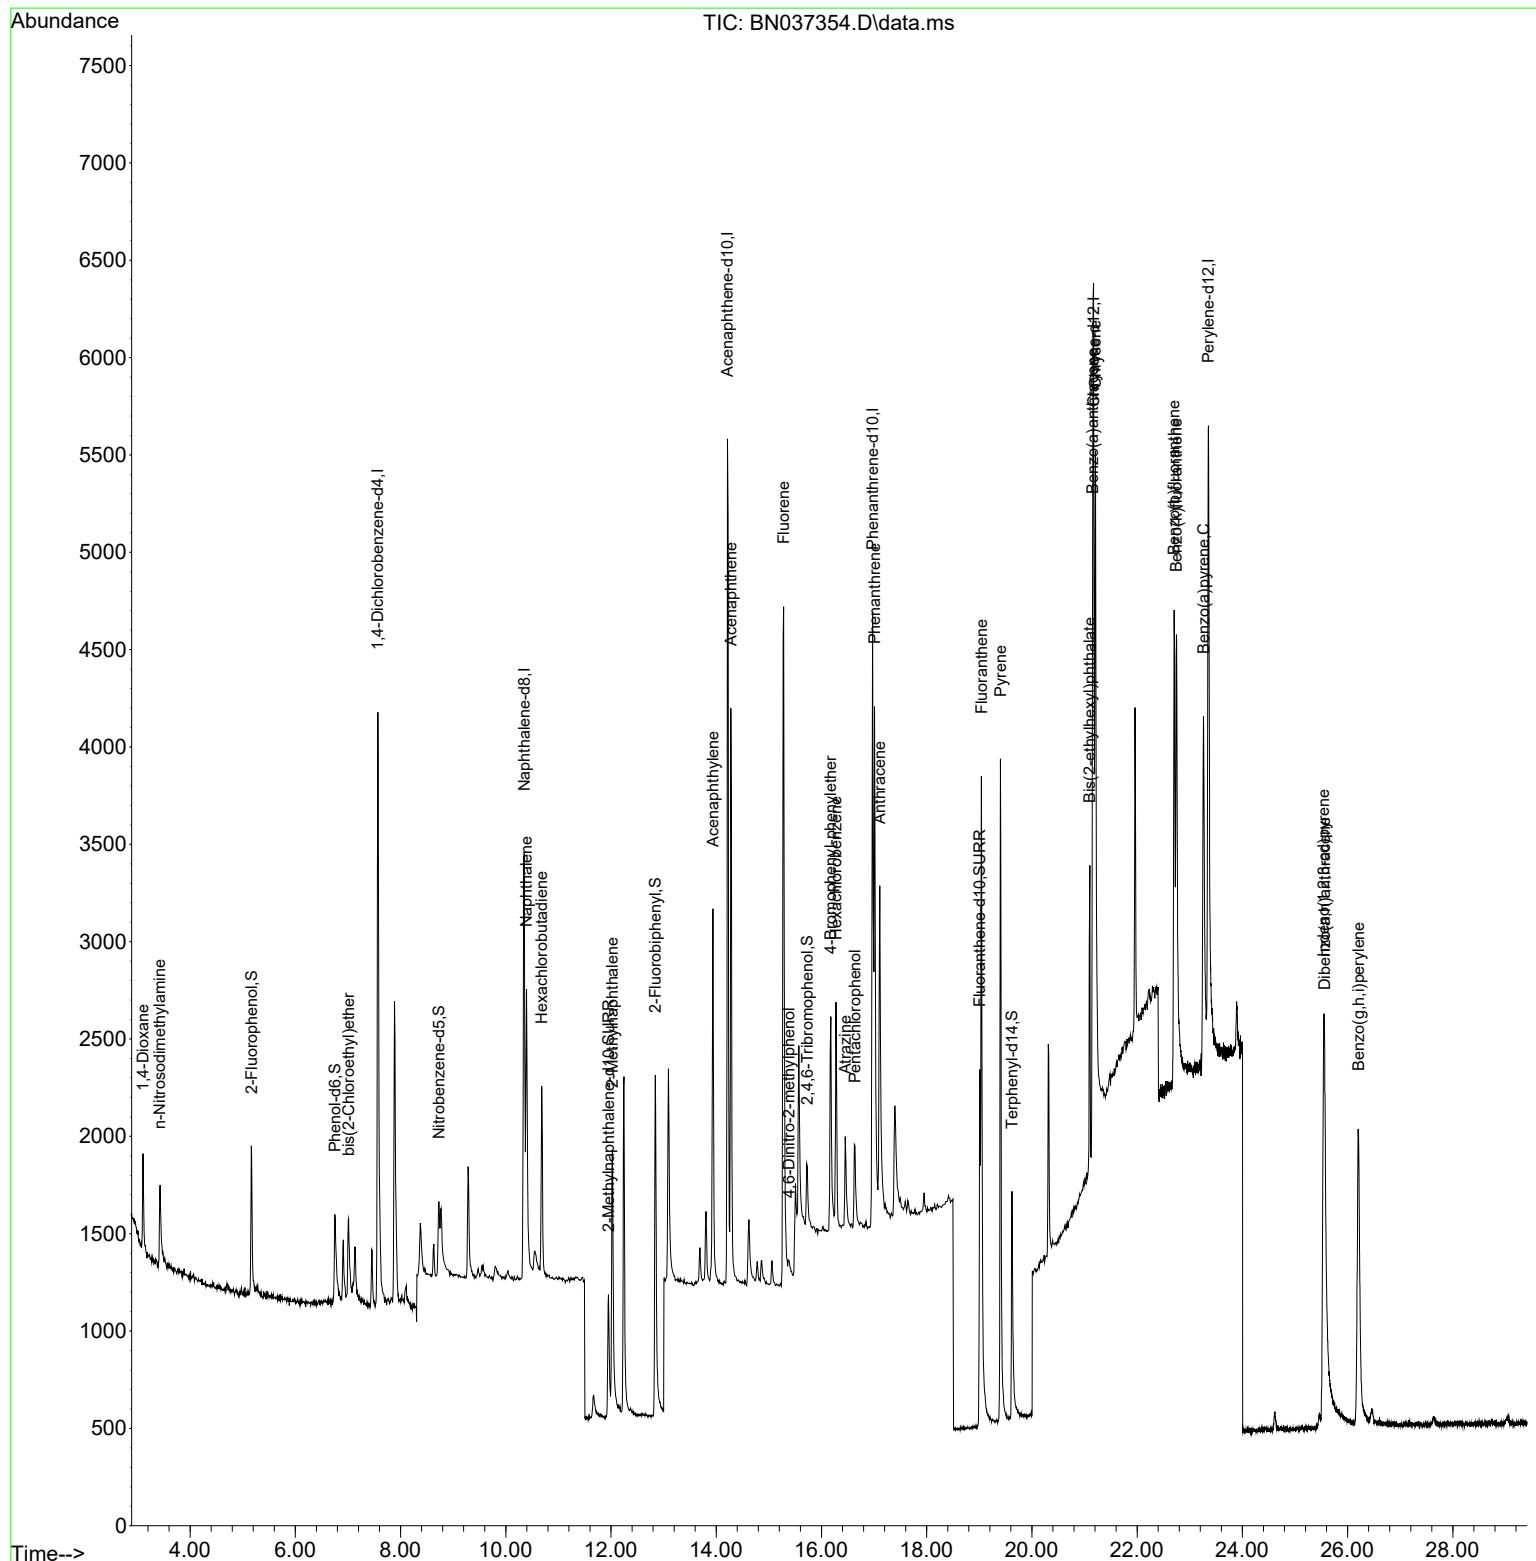


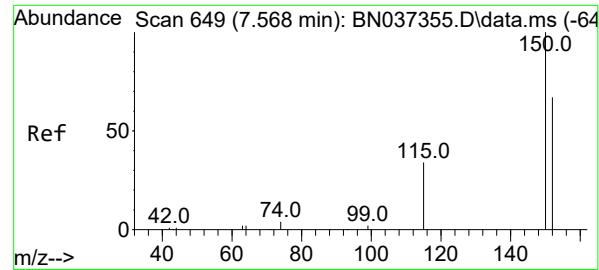

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27



Instrument :  
BNA\_N  
ClientSampleId :  
SSTDICCO.2


Tgt Ion:152 Resp: 1865  
Ion Ratio Lower Upper  
152 100  
150 153.3 112.7 169.1  
115 56.9 45.9 68.9

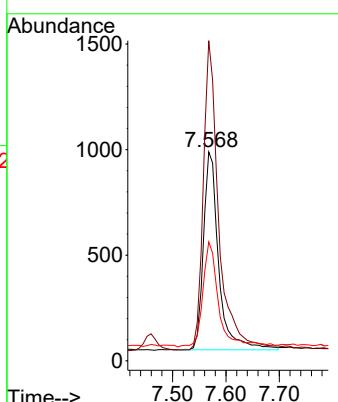

#2  
1,4-Dioxane  
Concen: 0.287 ng  
RT: 3.104 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27



Tgt Ion: 88 Resp: 472  
Ion Ratio Lower Upper  
88 100  
43 23.9 21.0 31.6  
58 46.8 38.0 57.0

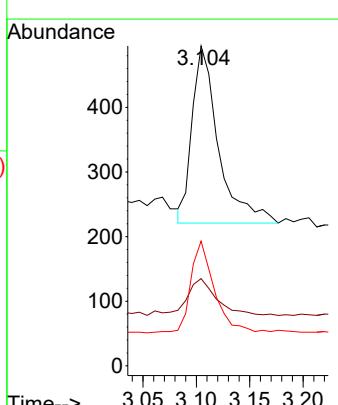

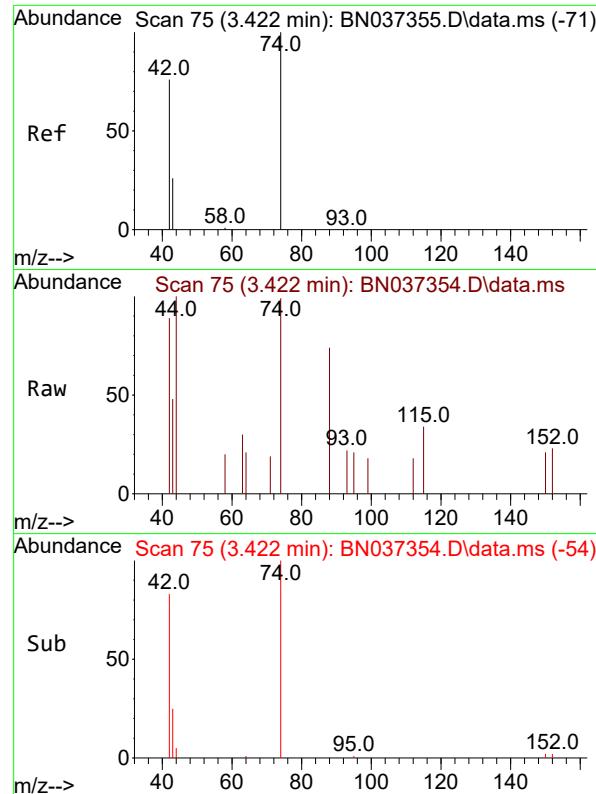


#3  
n-Nitrosodimethylamine  
Concen: 0.191 ng  
RT: 3.422 min Scan# 7  
Instrument: BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27  
ClientSampleId : SSTDICCO.2


Tgt Ion: 42 Resp: 366  
Ion Ratio Lower Upper  
42 100  
74 128.1 84.3 126.5#  
44 2.5 5.0 7.4#

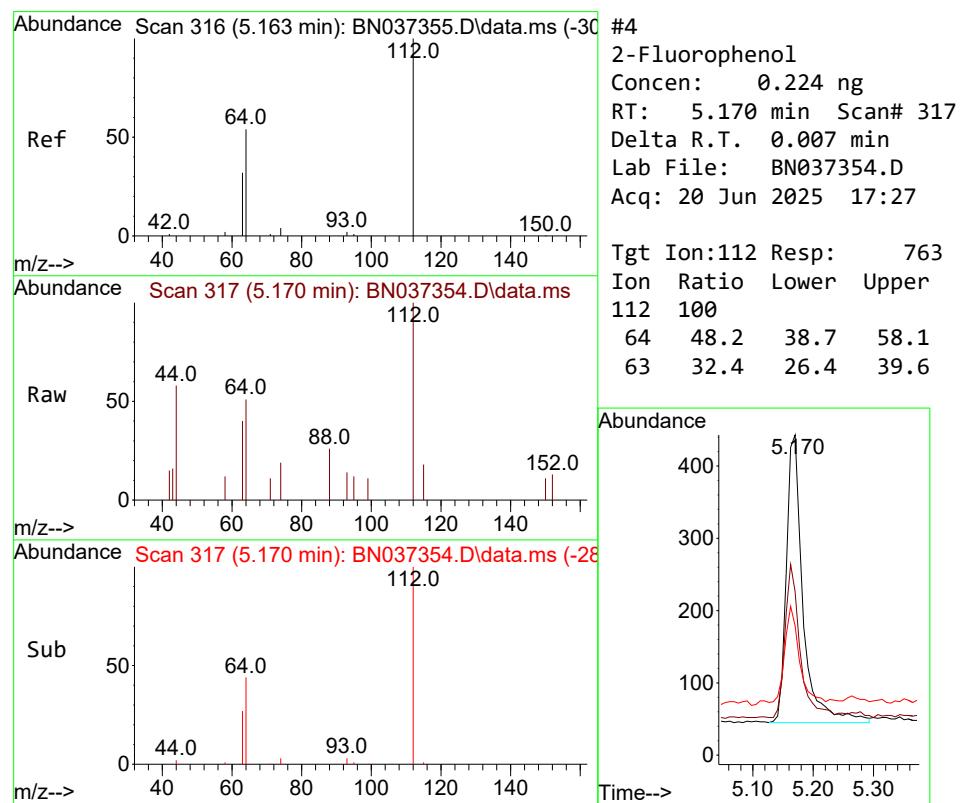

#4  
2-Fluorophenol  
Concen: 0.224 ng  
RT: 5.170 min Scan# 317  
Delta R.T. 0.007 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Tgt Ion: 112 Resp: 763  
Ion Ratio Lower Upper  
112 100  
64 48.2 38.7 58.1  
63 32.4 26.4 39.6


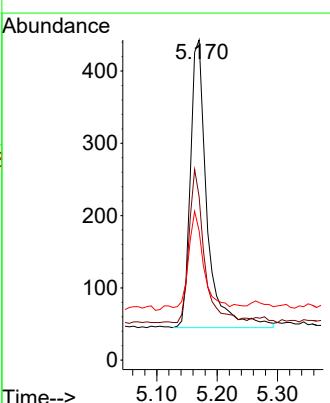


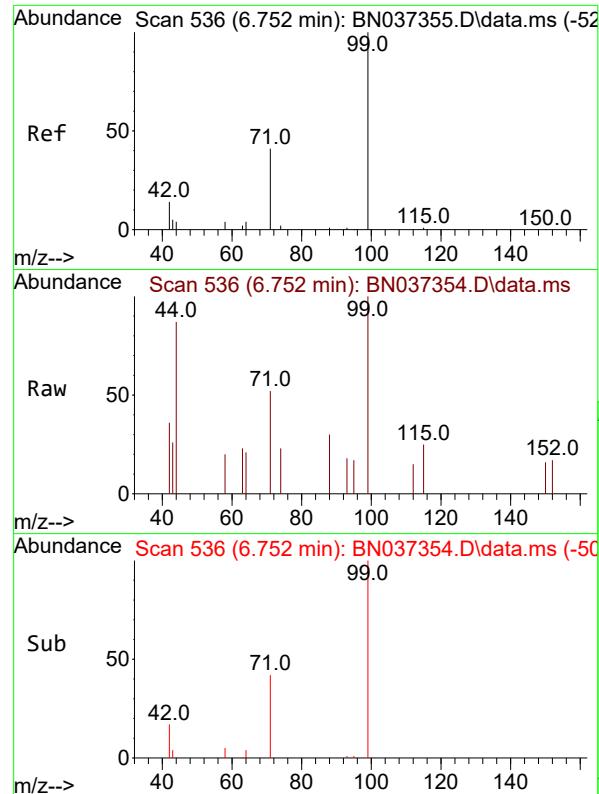

#5  
 Phenol-d6  
 Concen: 0.212 ng  
 RT: 6.752 min Scan# 5  
 Delta R.T. -0.000 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2




Tgt Ion: 99 Resp: 714  
 Ion Ratio Lower Upper  
 99 100  
 42 16.2 19.8 29.8#  
 71 44.0 42.6 64.0

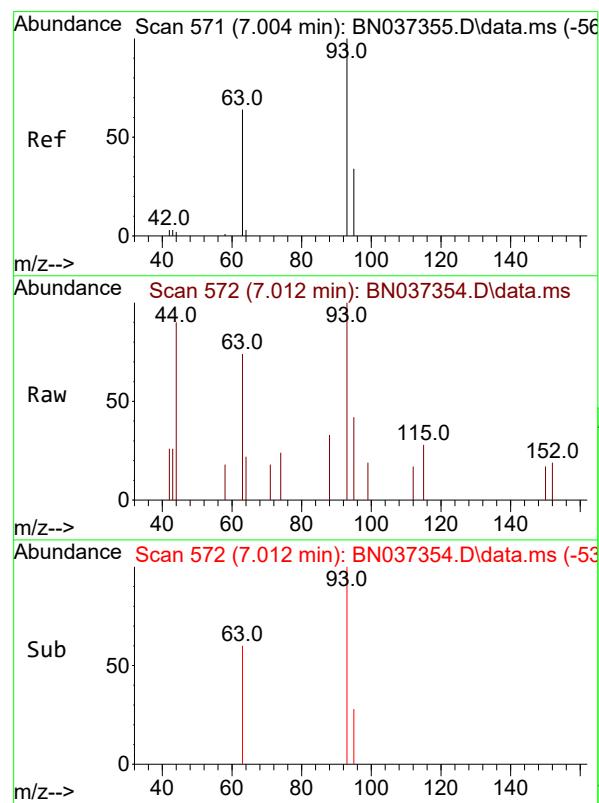

#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.172 ng  
 RT: 7.012 min Scan# 572  
 Delta R.T. 0.007 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27

Tgt Ion: 93 Resp: 509  
 Ion Ratio Lower Upper  
 93 100  
 63 69.4 53.2 79.8  
 95 38.3 27.3 40.9





#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.351 min Scan# 9  
 Delta R.T. 0.011 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27





Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2

Tgt Ion:136 Resp: 3983

Ion Ratio Lower Upper

136	100
137	12.9
54	7.0
68	5.8
	12.2
	8.8
	7.0
	18.2
	13.2#
	10.4#

Abundance

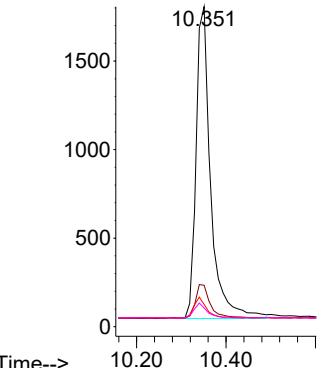





#8  
 Nitrobenzene-d5  
 Concen: 0.176 ng  
 RT: 8.728 min Scan# 791  
 Delta R.T. 0.011 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27

Tgt Ion: 82 Resp: 582

Ion Ratio Lower Upper

82	100
128	52.7
54	52.7
	42.5
	43.2
	63.7
	64.8

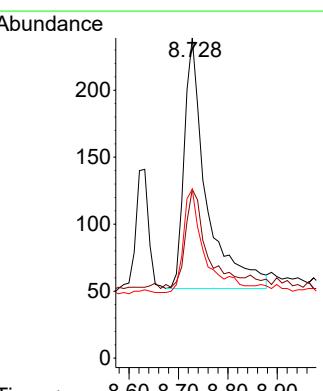

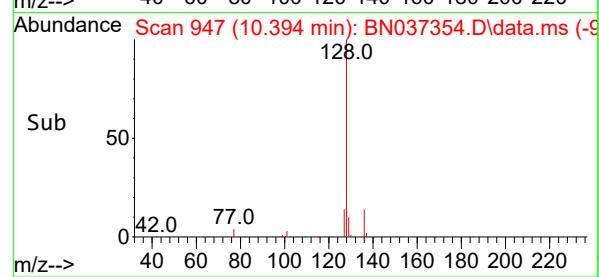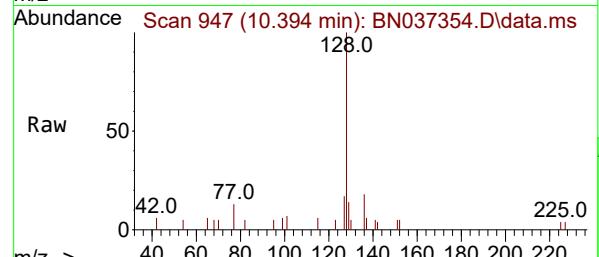

#9

Naphthalene

Concen: 0.204 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.2

Tgt Ion:128 Resp: 2104

Ion Ratio Lower Upper

128 100

129 14.4 14.0 21.0





127 17.4 15.8 23.8

Abundance

1000  
800  
600  
400  
200  
0

10.394

Time--&gt;

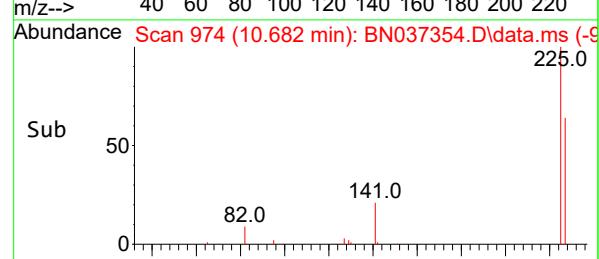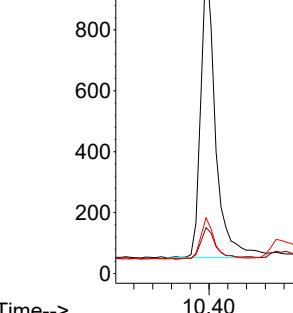

#10

Hexachlorobutadiene

Concen: 0.171 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Tgt Ion:225 Resp: 864

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0


227 63.9 50.3 75.5




Abundance

500  
400  
300  
200  
100  
0

10.682

Time--&gt;

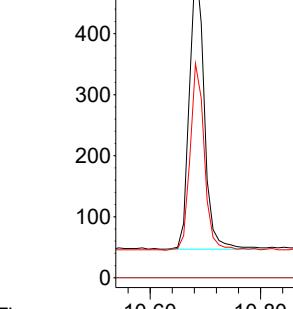

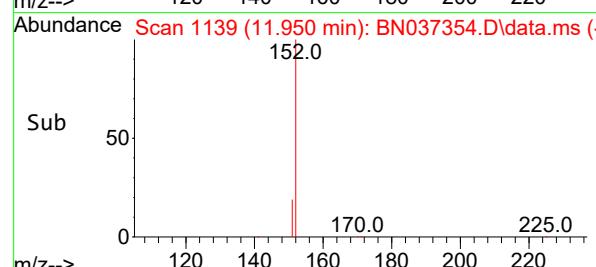

#11

2-Methylnaphthalene-d10

Concen: 0.197 ng

RT: 11.950 min Scan# 1139

Delta R.T. 0.005 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Instrument :

BNA\_N

ClientSampleId :




SSTDICCO.2

Tgt Ion:152 Resp: 1271

Ion Ratio Lower Upper

152 100

151 20.8 17.4 26.0

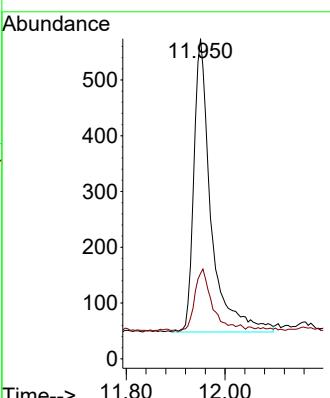

#12

2-Methylnaphthalene

Concen: 0.190 ng

RT: 12.026 min Scan# 1154

Delta R.T. 0.005 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27



Tgt Ion:142 Resp: 1379


Ion Ratio Lower Upper

142 100

141 92.8 70.2 105.2

115 47.0 43.0 64.4


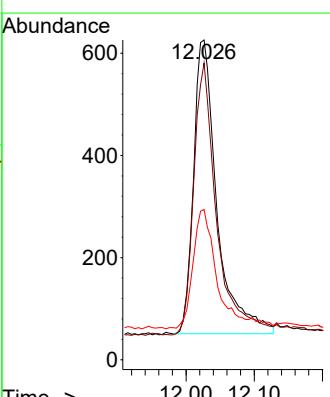


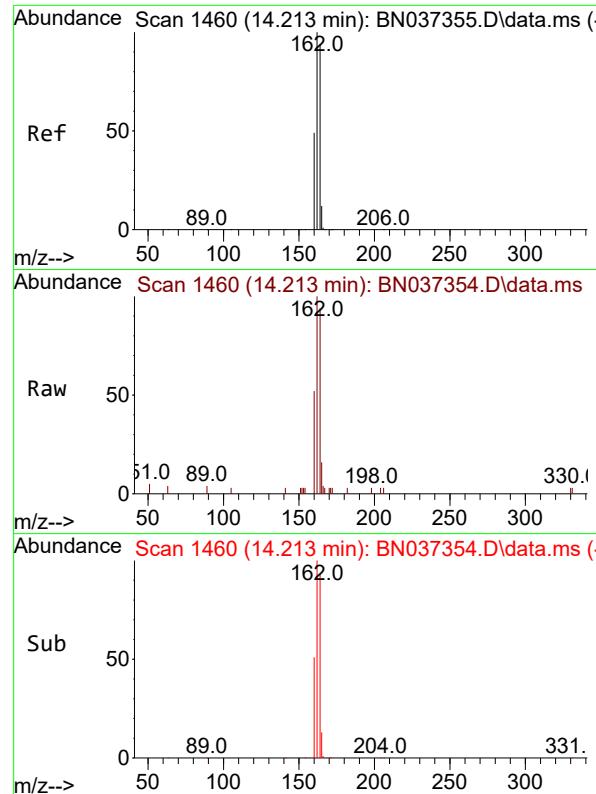

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2


Tgt Ion:164 Resp: 2790  
Ion Ratio Lower Upper  
164 100  
162 106.9 81.5 122.3  
160 55.5 43.0 64.4

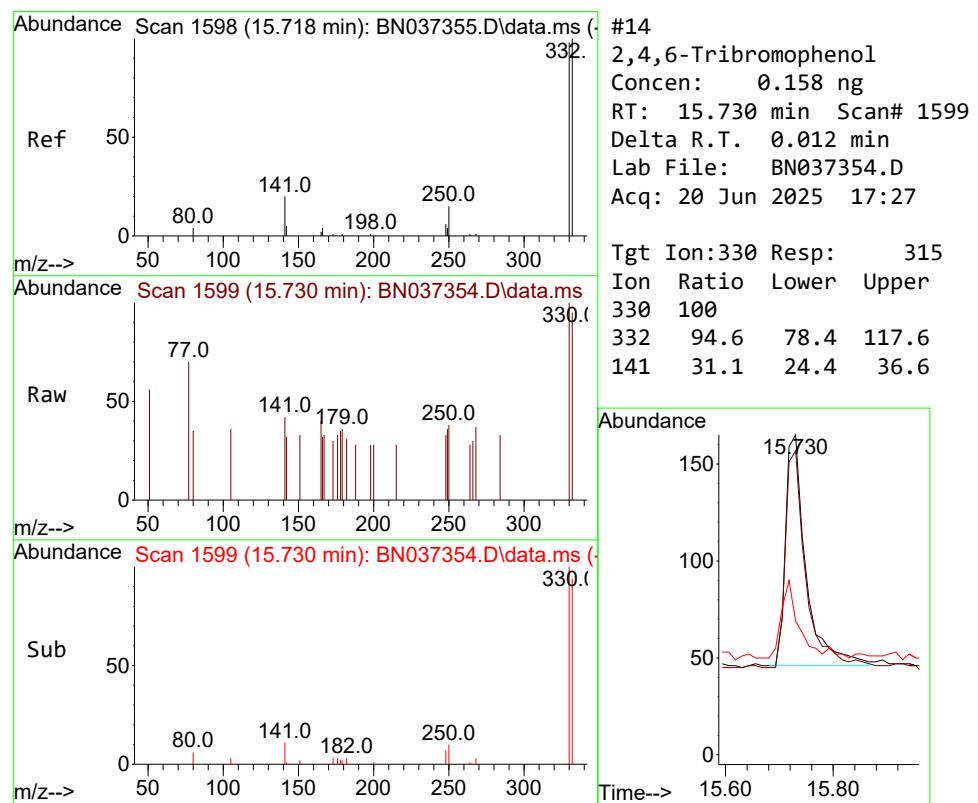

#14  
2,4,6-Tribromophenol  
Concen: 0.158 ng  
RT: 15.730 min Scan# 1599  
Delta R.T. 0.012 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27



Tgt Ion:330 Resp: 315  
Ion Ratio Lower Upper  
330 100  
332 94.6 78.4 117.6  
141 31.1 24.4 36.6



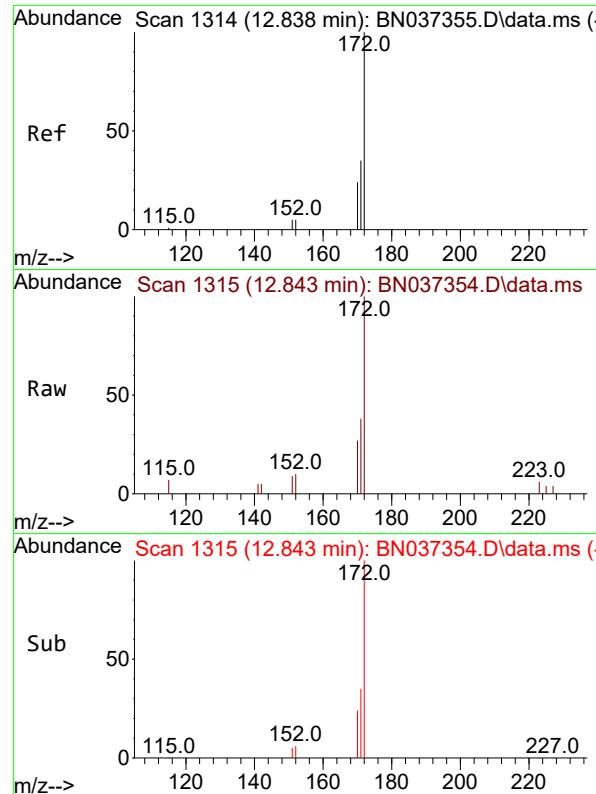


#15  
2-Fluorobiphenyl  
Concen: 0.191 ng  
RT: 12.843 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.005 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27  
ClientSampleId : SSTDICCO.2




Tgt Ion:172 Resp: 2337  
Ion Ratio Lower Upper  
172 100  
171 38.1 30.8 46.2  
170 27.1 21.9 32.9

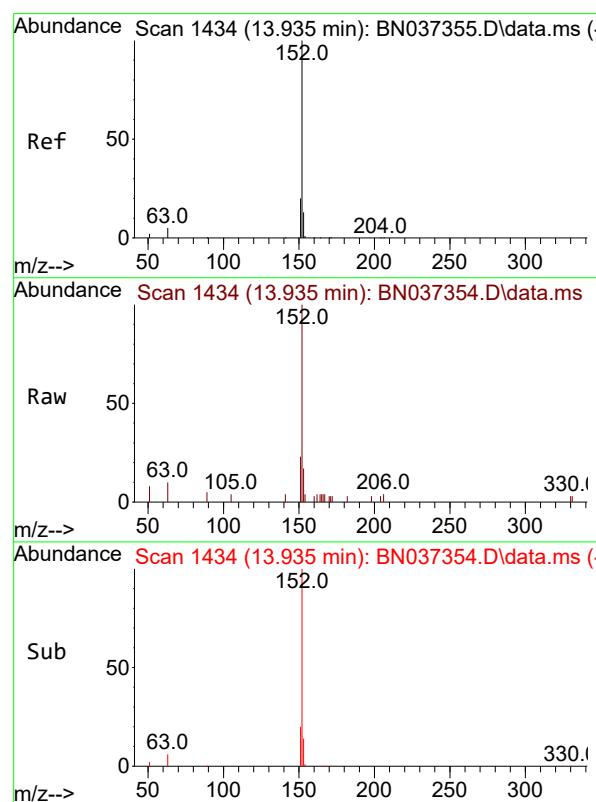

#16  
Acenaphthylene  
Concen: 0.195 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Tgt Ion:152 Resp: 2282  
Ion Ratio Lower Upper  
152 100  
151 19.8 16.6 24.8  
153 14.1 10.2 15.2



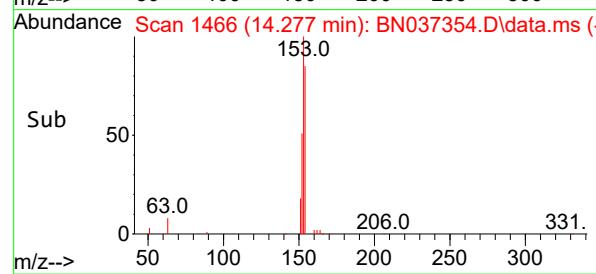

#17

Acenaphthene

Concen: 0.192 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.2

Tgt Ion:154 Resp: 1492

Ion Ratio Lower Upper

154 100

153 118.3 93.1 139.7

152 60.7 48.6 73.0

Abundance

1000

800

600




400

200

0

14.20 14.277 14.40

Time--&gt;



#18

Fluorene

Concen: 0.186 ng

RT: 15.282 min Scan# 1560

Delta R.T. 0.011 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Tgt Ion:166 Resp: 2051

Ion Ratio Lower Upper

166 100

165 99.9 79.5 119.3

167 13.3 10.7 16.1

Abundance

1000

800

600


400

200

0

15.20 15.282 15.40

Time--&gt;

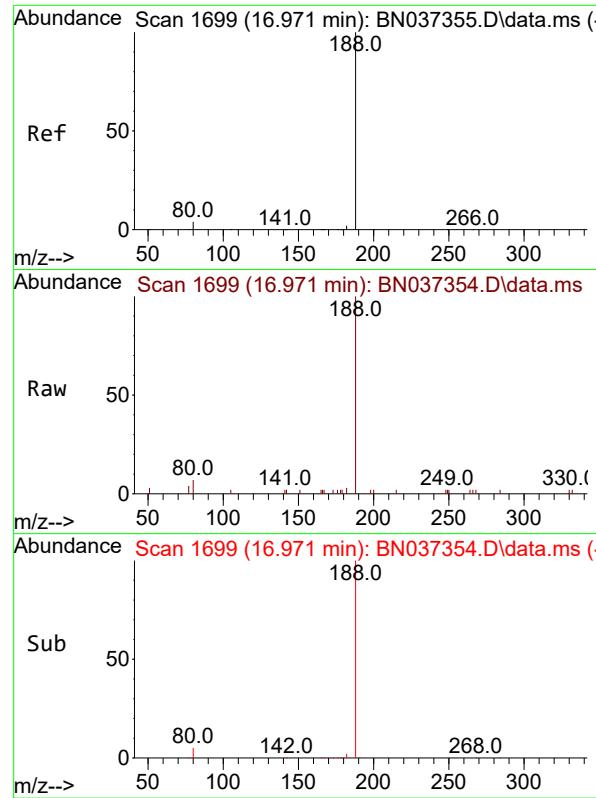

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Instrument:

BNA\_N

ClientSampleId :

SSTDICCO.2

Tgt Ion:188 Resp: 5628

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 6.5 6.2 9.2

Abundance


16.971

2000

1000

0

Time--&gt; 16.80 17.00

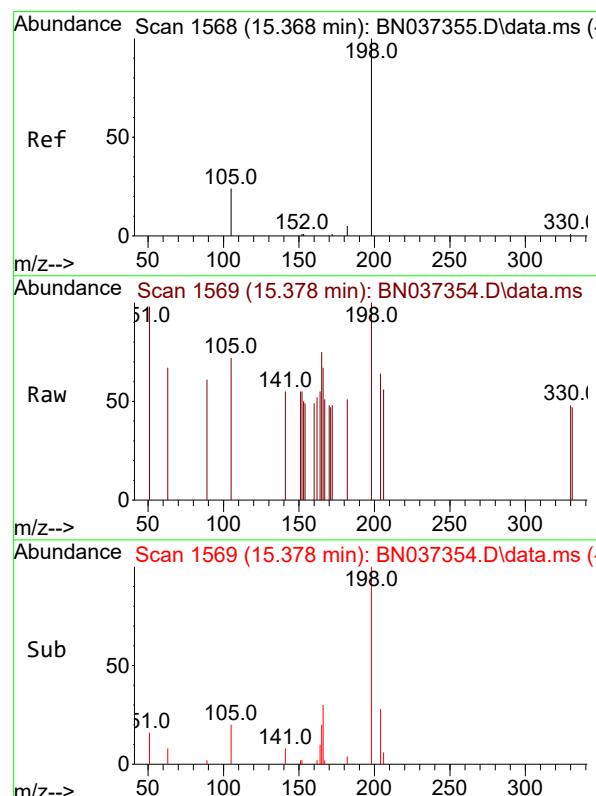

#20

4,6-Dinitro-2-methylphenol

Concen: 0.115 ng

RT: 15.378 min Scan# 1569

Delta R.T. 0.011 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Tgt Ion:198 Resp: 196

Ion Ratio Lower Upper

198 100

51 97.9 51.4 77.0#

105 71.9 45.5 68.3#

Abundance

15.378

200


150

100

50



0

Time--&gt; 15.40

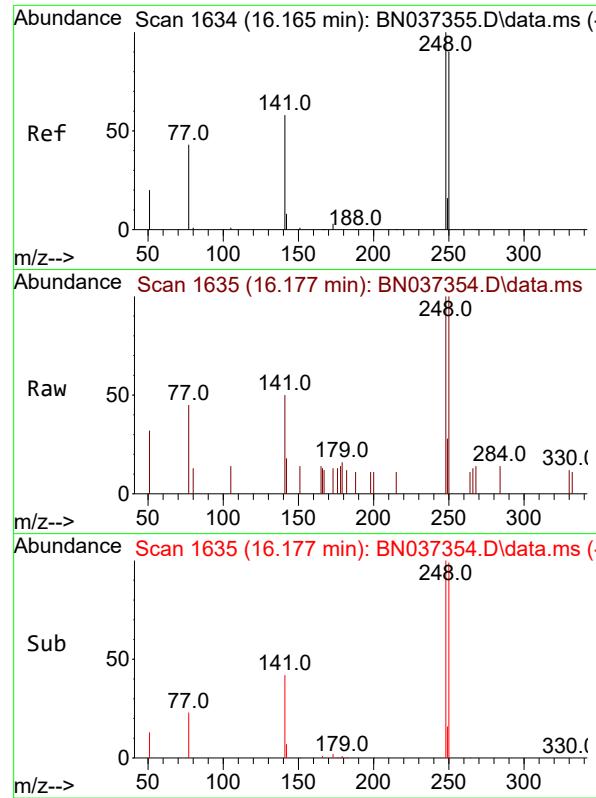


#21  
4-Bromophenyl-phenylether  
Concen: 0.163 ng  
RT: 16.177 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.012 min  
Lab File: BN037354.D  
ClientSampleId : SSTDICCO.2  
Acq: 20 Jun 2025 17:27


Tgt Ion:248 Resp: 750  
Ion Ratio Lower Upper  
248 100  
250 100.0 80.4 120.6  
141 49.8 33.3 49.9

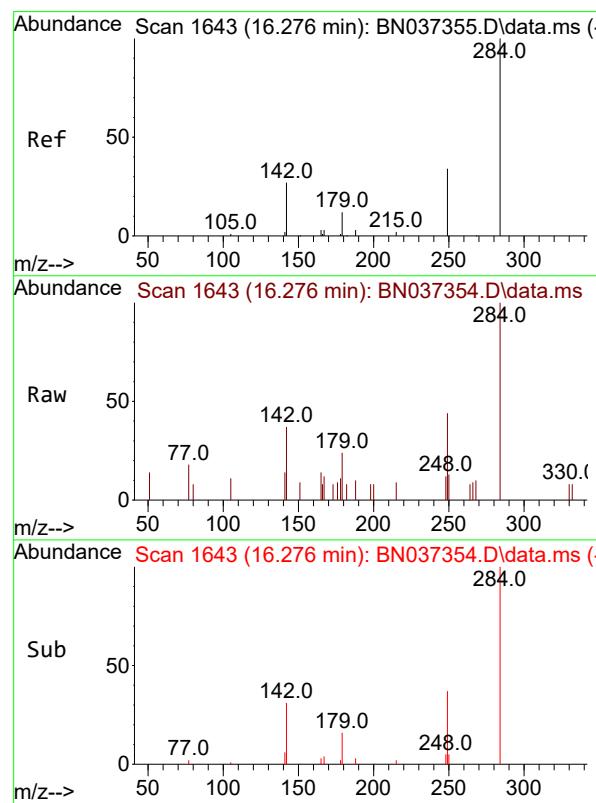

#22  
Hexachlorobenzene  
Concen: 0.187 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Tgt Ion:284 Resp: 898  
Ion Ratio Lower Upper  
284 100  
142 33.4 27.0 40.6  
249 37.8 28.8 43.2


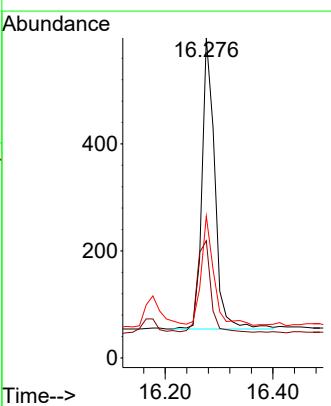


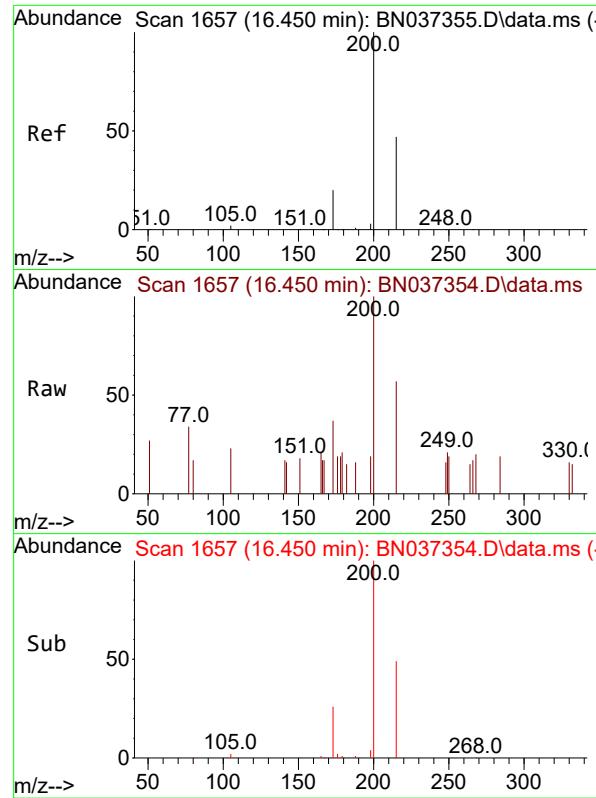

#23  
Atrazine  
Concen: 0.168 ng  
RT: 16.450 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2




Tgt Ion:200 Resp: 604  
Ion Ratio Lower Upper  
200 100  
173 37.2 29.2 43.8  
215 56.8 48.8 73.2

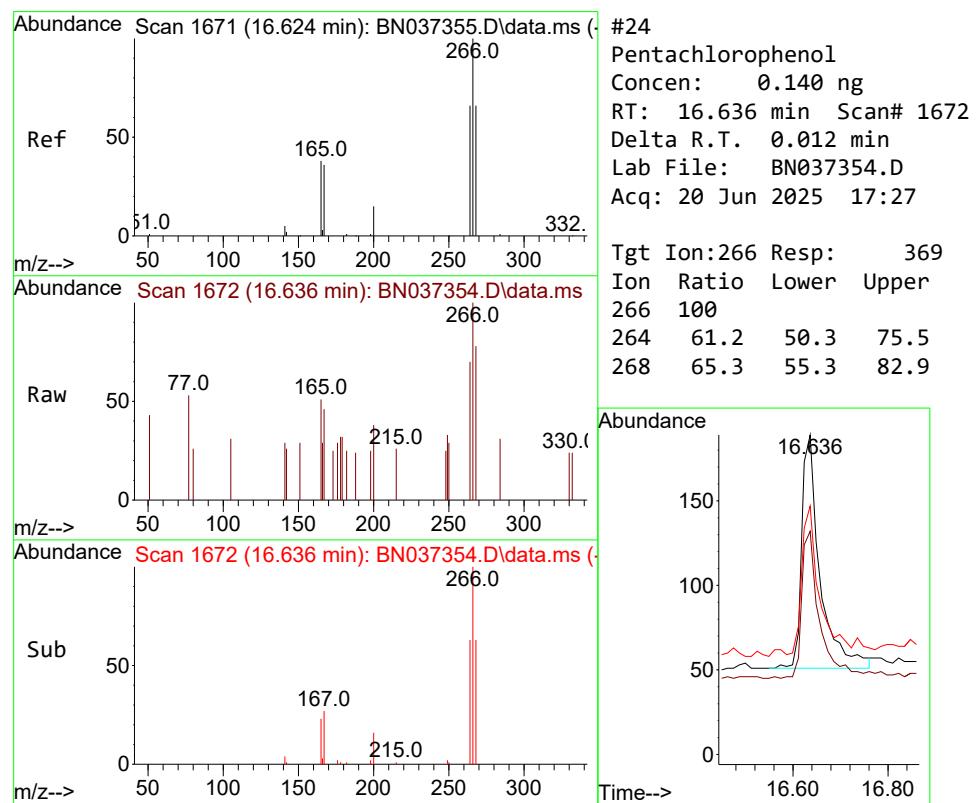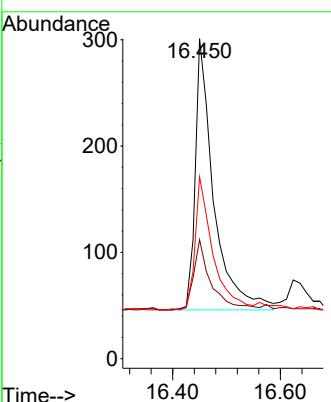

#24  
Pentachlorophenol  
Concen: 0.140 ng  
RT: 16.636 min Scan# 1672  
Delta R.T. 0.012 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Tgt Ion:266 Resp: 369  
Ion Ratio Lower Upper  
266 100  
264 61.2 50.3 75.5  
268 65.3 55.3 82.9





#25

Phenanthrene

Concen: 0.190 ng

RT: 17.009 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27

Instrument:

BNA\_N

ClientSampleId :

SSTDICCO.2





Tgt Ion:178 Resp: 3024

Ion Ratio Lower Upper

178 100

176 19.6 15.2 22.8

179 15.3 12.9 19.3

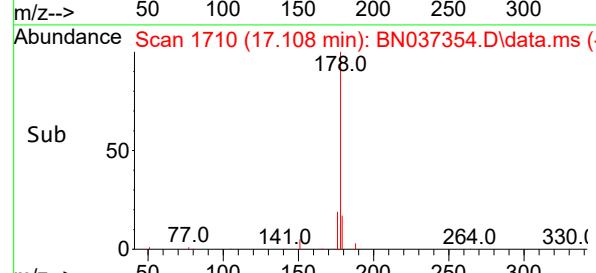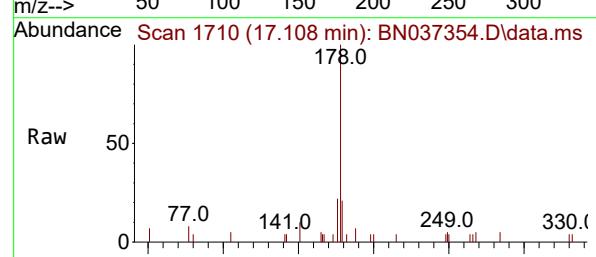

#26

Anthracene

Concen: 0.186 ng

RT: 17.108 min Scan# 1710

Delta R.T. -0.000 min

Lab File: BN037354.D

Acq: 20 Jun 2025 17:27


Tgt Ion:178 Resp: 2769


Ion Ratio Lower Upper

178 100

176 19.7 14.7 22.1

179 15.0 13.0 19.6


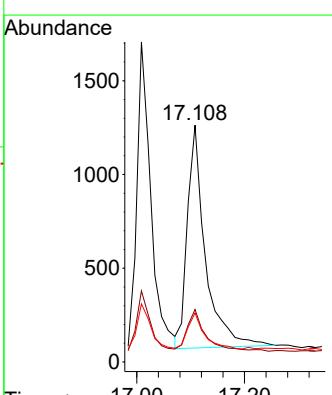


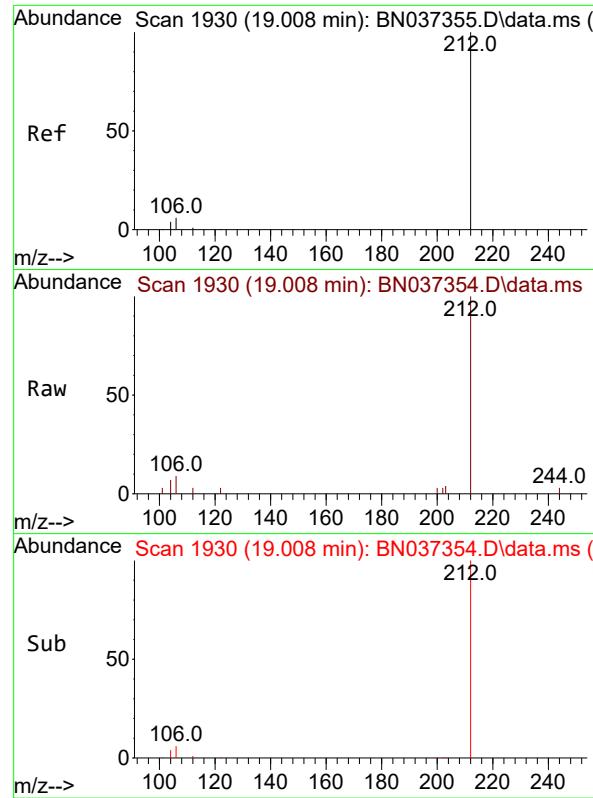

#27  
Fluoranthene-d10  
Concen: 0.172 ng  
RT: 19.008 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2


Tgt Ion:212 Resp: 3010  
Ion Ratio Lower Upper  
212 100  
106 6.0 3.0 4.4#  
104 3.2 2.0 3.0#

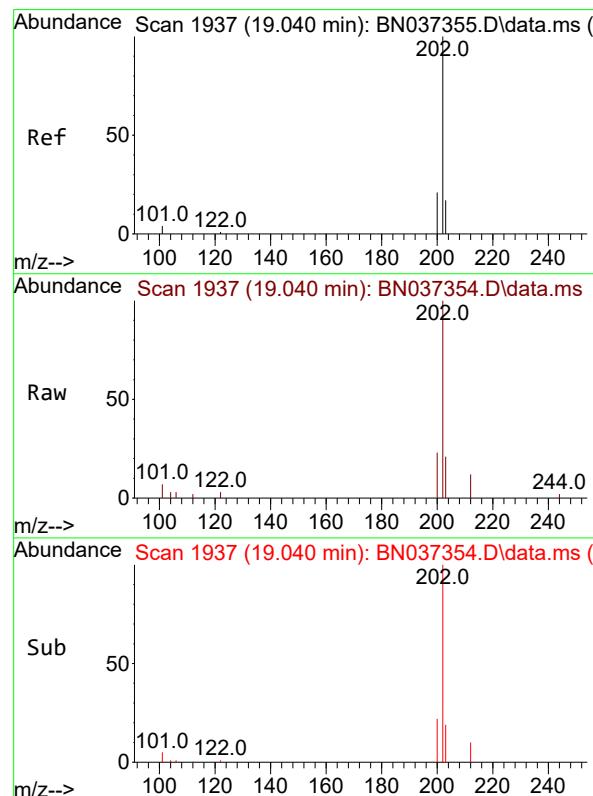

#28  
Fluoranthene  
Concen: 0.174 ng  
RT: 19.040 min Scan# 1937  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Tgt Ion:202 Resp: 3780  
Ion Ratio Lower Upper  
202 100  
101 4.7 3.0 4.6#  
203 17.8 13.7 20.5





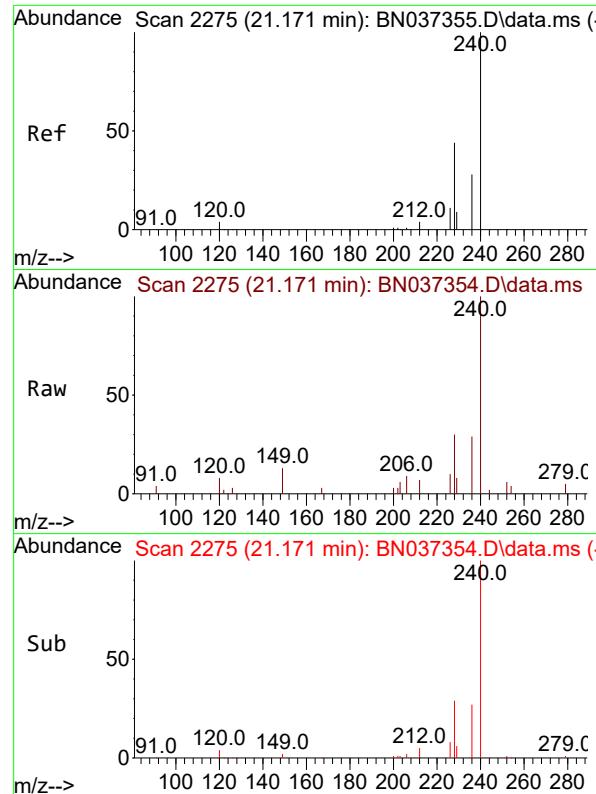

#29  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.171 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2


Tgt Ion:240 Resp: 4640  
 Ion Ratio Lower Upper  
 240 100  
 120 7.5 7.5 11.3  
 236 28.7 24.9 37.3

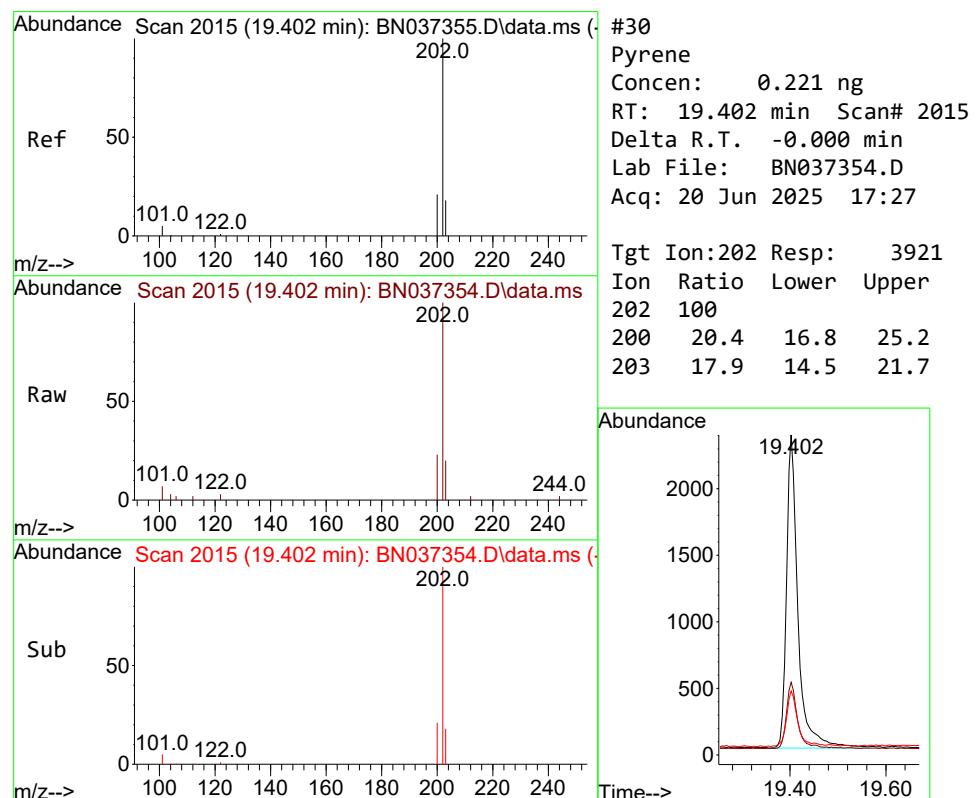

#30  
 Pyrene  
 Concen: 0.221 ng  
 RT: 19.402 min Scan# 2015  
 Delta R.T. -0.000 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27

Tgt Ion:202 Resp: 3921  
 Ion Ratio Lower Upper  
 202 100  
 200 20.4 16.8 25.2  
 203 17.9 14.5 21.7


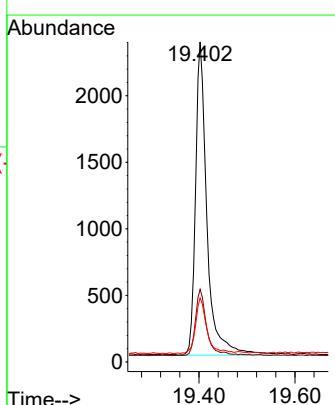


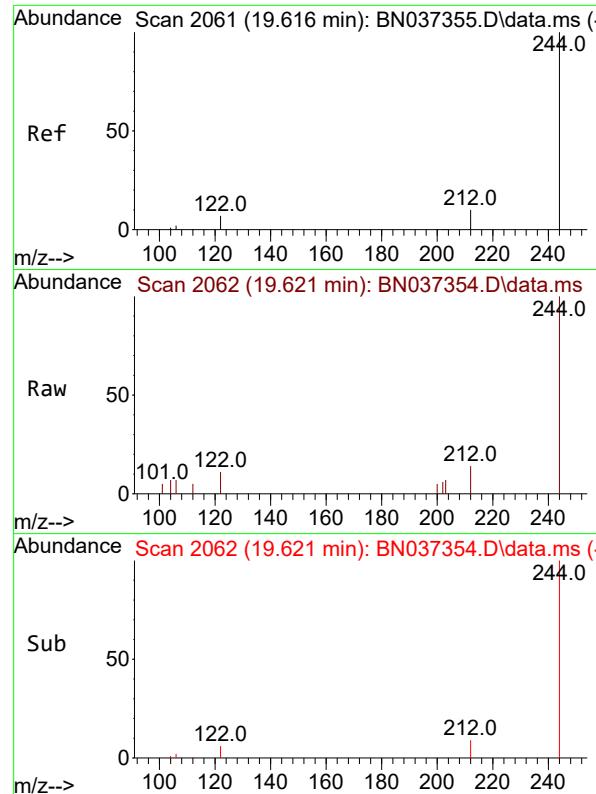

#31  
Terphenyl-d14  
Concen: 0.200 ng  
RT: 19.621 min Scan# 2114  
Delta R.T. 0.005 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2




Tgt Ion:244 Resp: 2114  
Ion Ratio Lower Upper  
244 100  
212 13.9 11.1 16.7  
122 11.1 7.2 10.8#

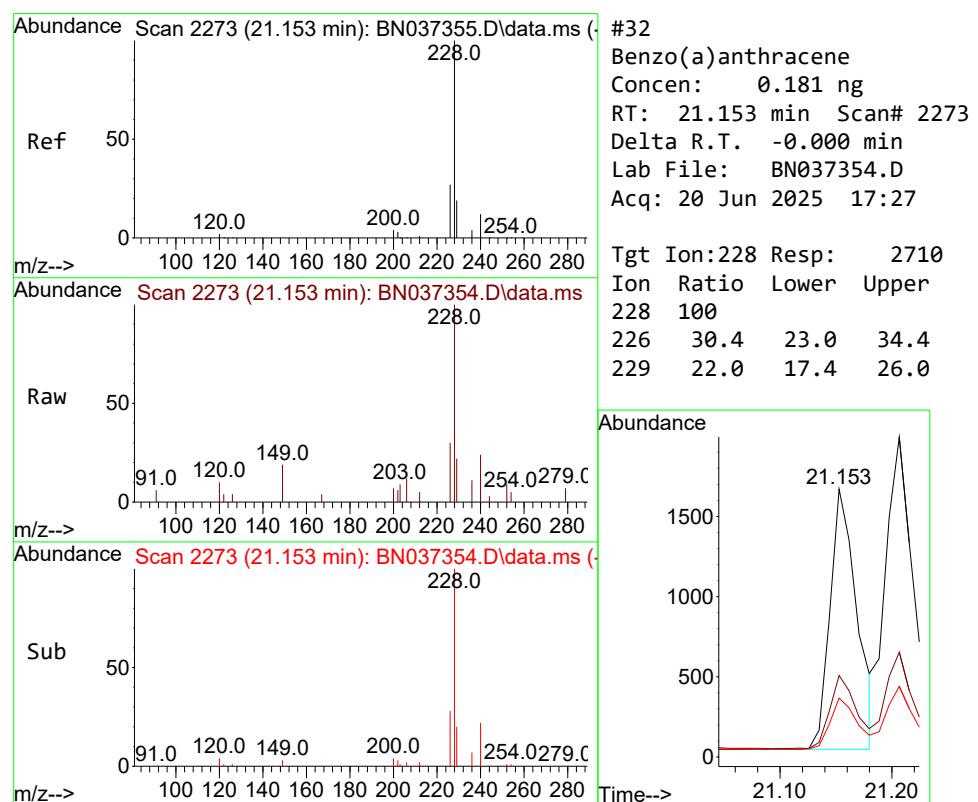

#32  
Benzo(a)anthracene  
Concen: 0.181 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27





Tgt Ion:228 Resp: 2710  
Ion Ratio Lower Upper  
228 100  
226 30.4 23.0 34.4  
229 22.0 17.4 26.0






#33  
Chrysene  
Concen: 0.208 ng  
RT: 21.206 min Scan# 2  
Instrument: BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27  
ClientSampleId : SSTDICCO.2


Tgt Ion:228 Resp: 3959  
Ion Ratio Lower Upper  
228 100  
226 32.8 25.4 38.2  
229 22.0 17.3 25.9

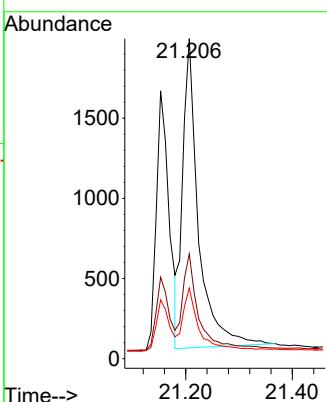

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.229 ng  
RT: 21.099 min Scan# 2267  
Delta R.T. -0.000 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Tgt Ion:149 Resp: 1406  
Ion Ratio Lower Upper  
149 100  
167 31.8 24.6 37.0  
279 7.7 6.5 9.7





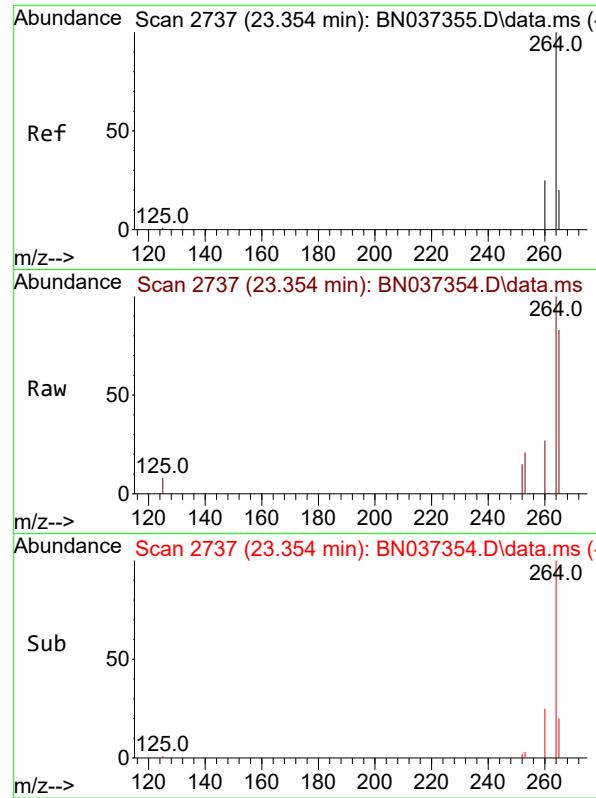

#35  
 Perylene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 23.354 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2


Tgt Ion:264 Resp: 4914  
 Ion Ratio Lower Upper  
 264 100  
 260 26.9 21.4 32.2  
 265 82.7 71.4 107.0

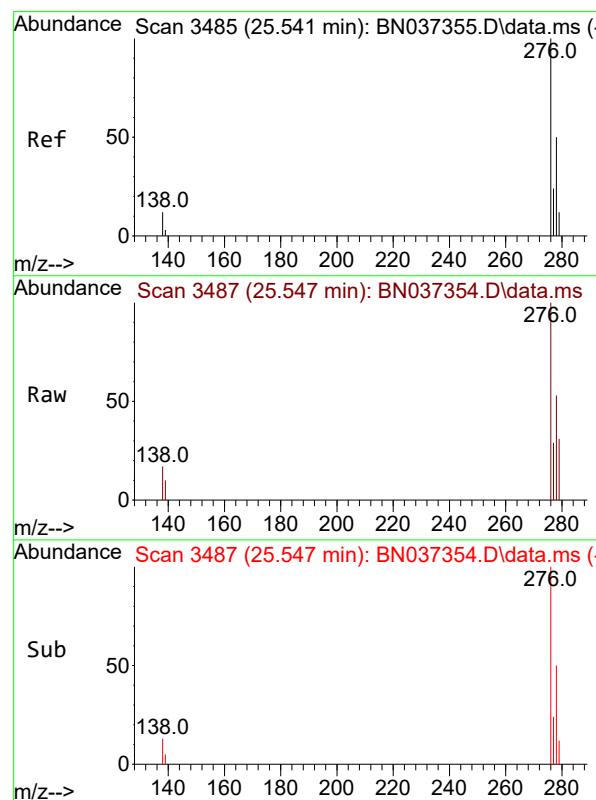

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.202 ng  
 RT: 25.547 min Scan# 3487  
 Delta R.T. 0.006 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27

Tgt Ion:276 Resp: 4213  
 Ion Ratio Lower Upper  
 276 100  
 138 9.1 2.2 3.2#  
 277 22.8 17.1 25.7





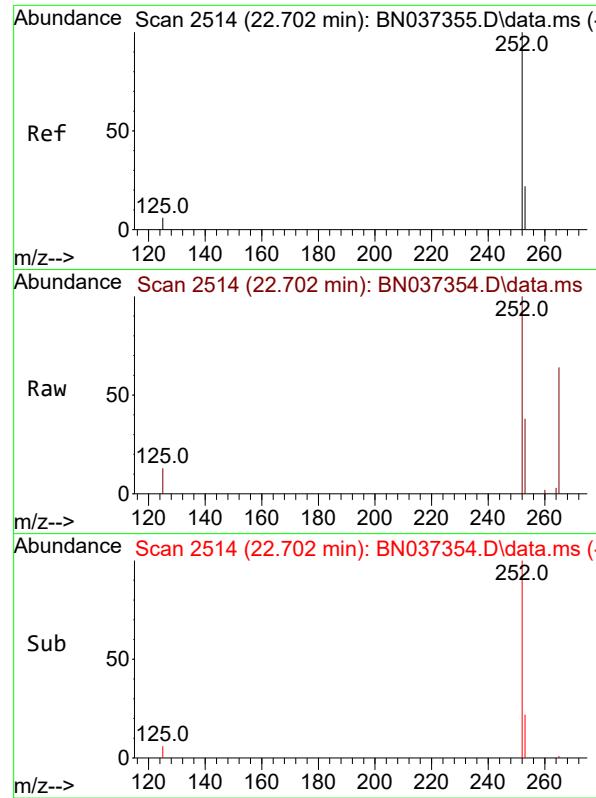

#37  
 Benzo(b)fluoranthene  
 Concen: 0.195 ng  
 RT: 22.702 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2


Tgt Ion:252 Resp: 3390  
 Ion Ratio Lower Upper  
 252 100  
 253 38.1 26.6 40.0  
 125 13.4 6.1 9.1#

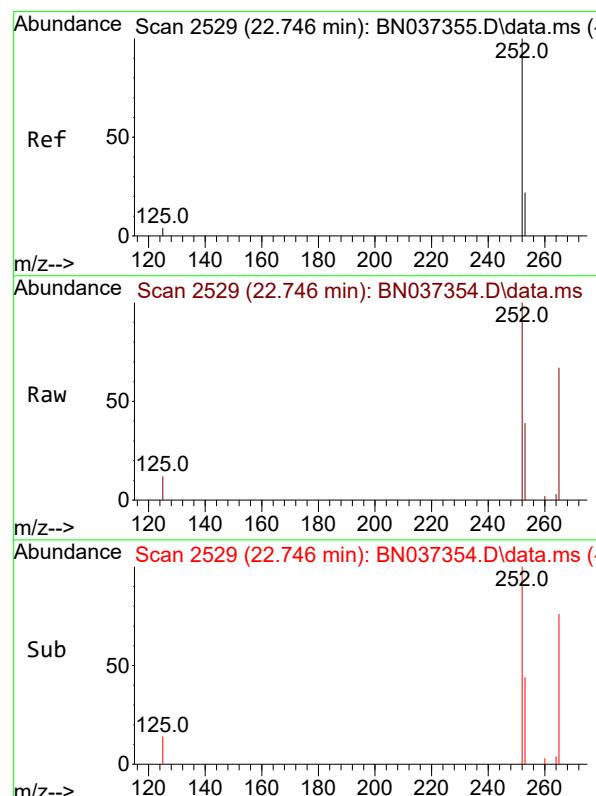

#38  
 Benzo(k)fluoranthene  
 Concen: 0.207 ng  
 RT: 22.746 min Scan# 2529  
 Delta R.T. -0.000 min  
 Lab File: BN037354.D  
 Acq: 20 Jun 2025 17:27



Tgt Ion:252 Resp: 3913  
 Ion Ratio Lower Upper  
 252 100  
 253 38.5 26.7 40.1  
 125 12.3 6.5 9.7#



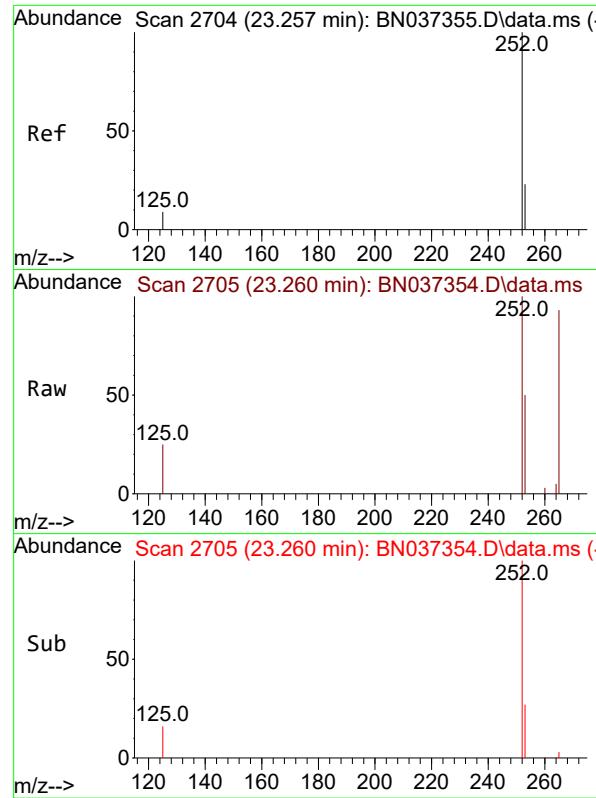


#39  
Benzo(a)pyrene  
Concen: 0.193 ng  
RT: 23.260 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.003 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27  
ClientSampleId : SSTDICCO.2


Tgt Ion:252 Resp: 3070  
Ion Ratio Lower Upper  
252 100  
253 49.8 31.6 47.4#  
125 24.8 8.4 12.6#

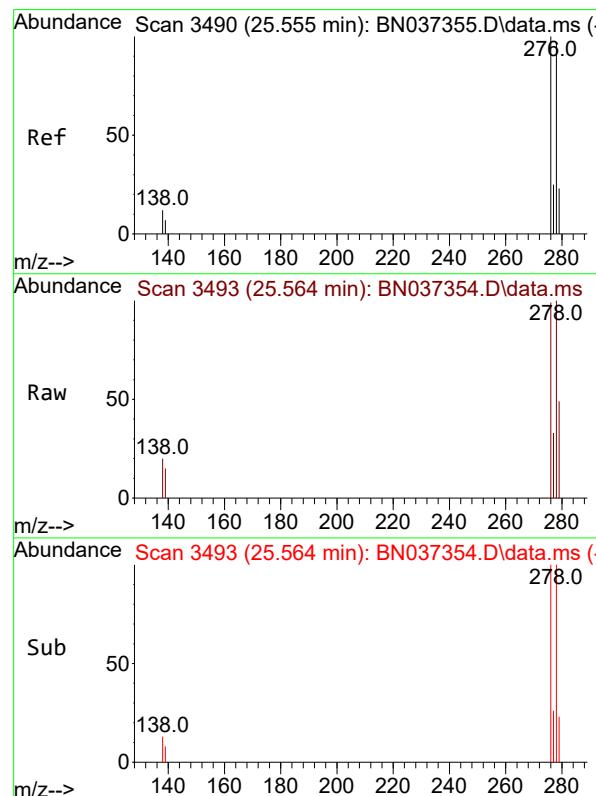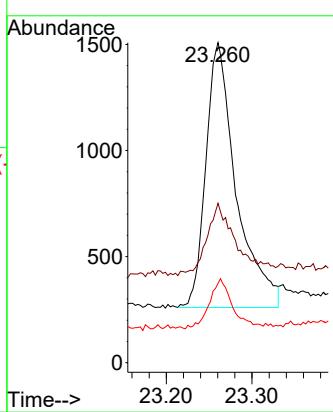

#40  
Dibenzo(a,h)anthracene  
Concen: 0.175 ng  
RT: 25.564 min Scan# 3493  
Delta R.T. 0.009 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Tgt Ion:278 Resp: 2911  
Ion Ratio Lower Upper  
278 100  
139 15.4 10.2 15.4#  
279 49.3 35.6 53.4




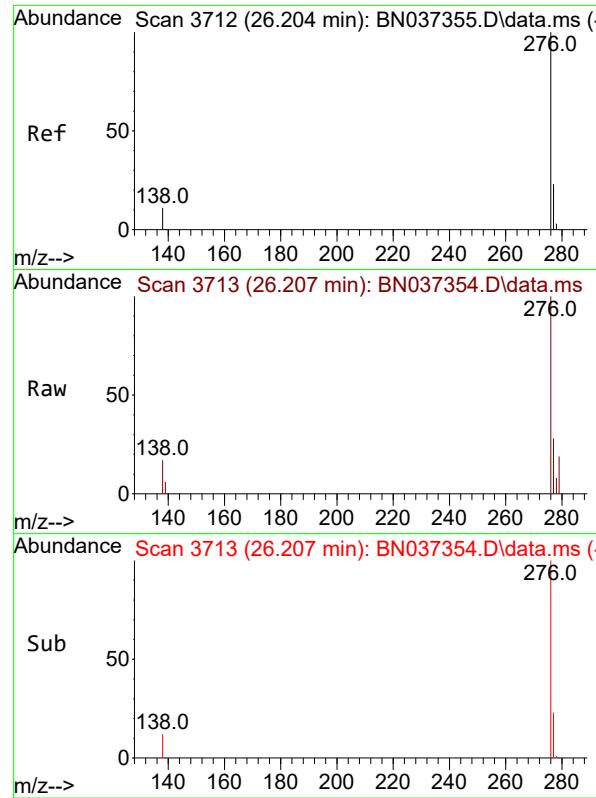

#41  
Benzo(g,h,i)perylene  
Concen: 0.200 ng  
RT: 26.207 min Scan# 3  
Delta R.T. 0.003 min  
Lab File: BN037354.D  
Acq: 20 Jun 2025 17:27

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2

Tgt Ion:276 Resp: 3819  
Ion Ratio Lower Upper  
276 100  
277 28.1 22.7 34.1  
138 16.6 9.4 14.2#

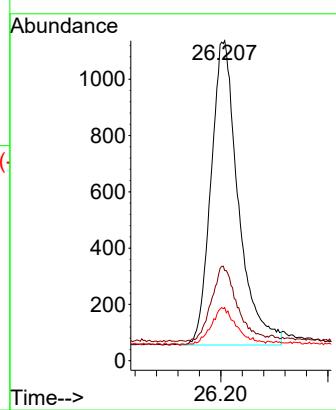

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037355.D  
 Acq On : 20 Jun 2025 18:03  
 Operator : RC/JU  
 Sample : SSTDICCC0.4  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCC0.4

Quant Time: Jun 20 23:26:55 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1912	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4157	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2811	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5776	0.400	ng	# 0.00
29) Chrysene-d12	21.171	240	4813	0.400	ng	# 0.00
35) Perylene-d12	23.354	264	4943	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1436	0.411	ng	0.00
5) Phenol-d6	6.752	99	1465	0.424	ng	0.00
8) Nitrobenzene-d5	8.717	82	1327	0.385	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	2768	0.411	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	646	0.321	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	4996	0.405	ng	0.00
27) Fluoranthene-d10	19.008	212	6705	0.373	ng	0.00
31) Terphenyl-d14	19.616	244	4452	0.405	ng	0.00
<b>Target Compounds</b>						
					Qvalue	
2) 1,4-Dioxane	3.104	88	745	0.441	ng	94
3) n-Nitrosodimethylamine	3.422	42	754	0.383	ng	81
6) bis(2-Chloroethyl)ether	7.004	93	1351	0.446	ng	94
9) Naphthalene	10.394	128	4347	0.403	ng	# 89
10) Hexachlorobutadiene	10.682	225	1832	0.348	ng	# 99
12) 2-Methylnaphthalene	12.021	142	2957	0.390	ng	92
16) Acenaphthylene	13.935	152	4490	0.381	ng	99
17) Acenaphthene	14.277	154	2983	0.381	ng	98
18) Fluorene	15.272	166	4232	0.382	ng	100
20) 4,6-Dinitro-2-methylph...	15.368	198	459	0.263	ng	89
21) 4-Bromophenyl-phenylether	16.165	248	1611	0.342	ng	# 85
22) Hexachlorobenzene	16.276	284	1814	0.369	ng	98
23) Atrazine	16.450	200	1262	0.342	ng	# 85
24) Pentachlorophenol	16.624	266	792	0.293	ng	98
25) Phenanthrene	17.009	178	6374	0.391	ng	99
26) Anthracene	17.108	178	5717	0.375	ng	98
28) Fluoranthene	19.040	202	7896	0.354	ng	# 98
30) Pyrene	19.402	202	7990	0.434	ng	100
32) Benzo(a)anthracene	21.153	228	5851	0.377	ng	98
33) Chrysene	21.207	228	7754	0.394	ng	98
34) Bis(2-ethylhexyl)phtha...	21.099	149	2603	0.409	ng	98
36) Indeno(1,2,3-cd)pyrene	25.541	276	8379	0.400	ng	# 93
37) Benzo(b)fluoranthene	22.702	252	7138m	0.407	ng	
38) Benzo(k)fluoranthene	22.746	252	7755	0.407	ng	95
39) Benzo(a)pyrene	23.257	252	6298	0.393	ng	# 92
40) Dibenzo(a,h)anthracene	25.555	278	6108	0.366	ng	# 88
41) Benzo(g,h,i)perylene	26.204	276	7852	0.408	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037355.D  
 Acq On : 20 Jun 2025 18:03  
 Operator : RC/JU  
 Sample : SSTDICCC0.4  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1


Quant Time: Jun 20 23:26:55 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCC0.4

**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

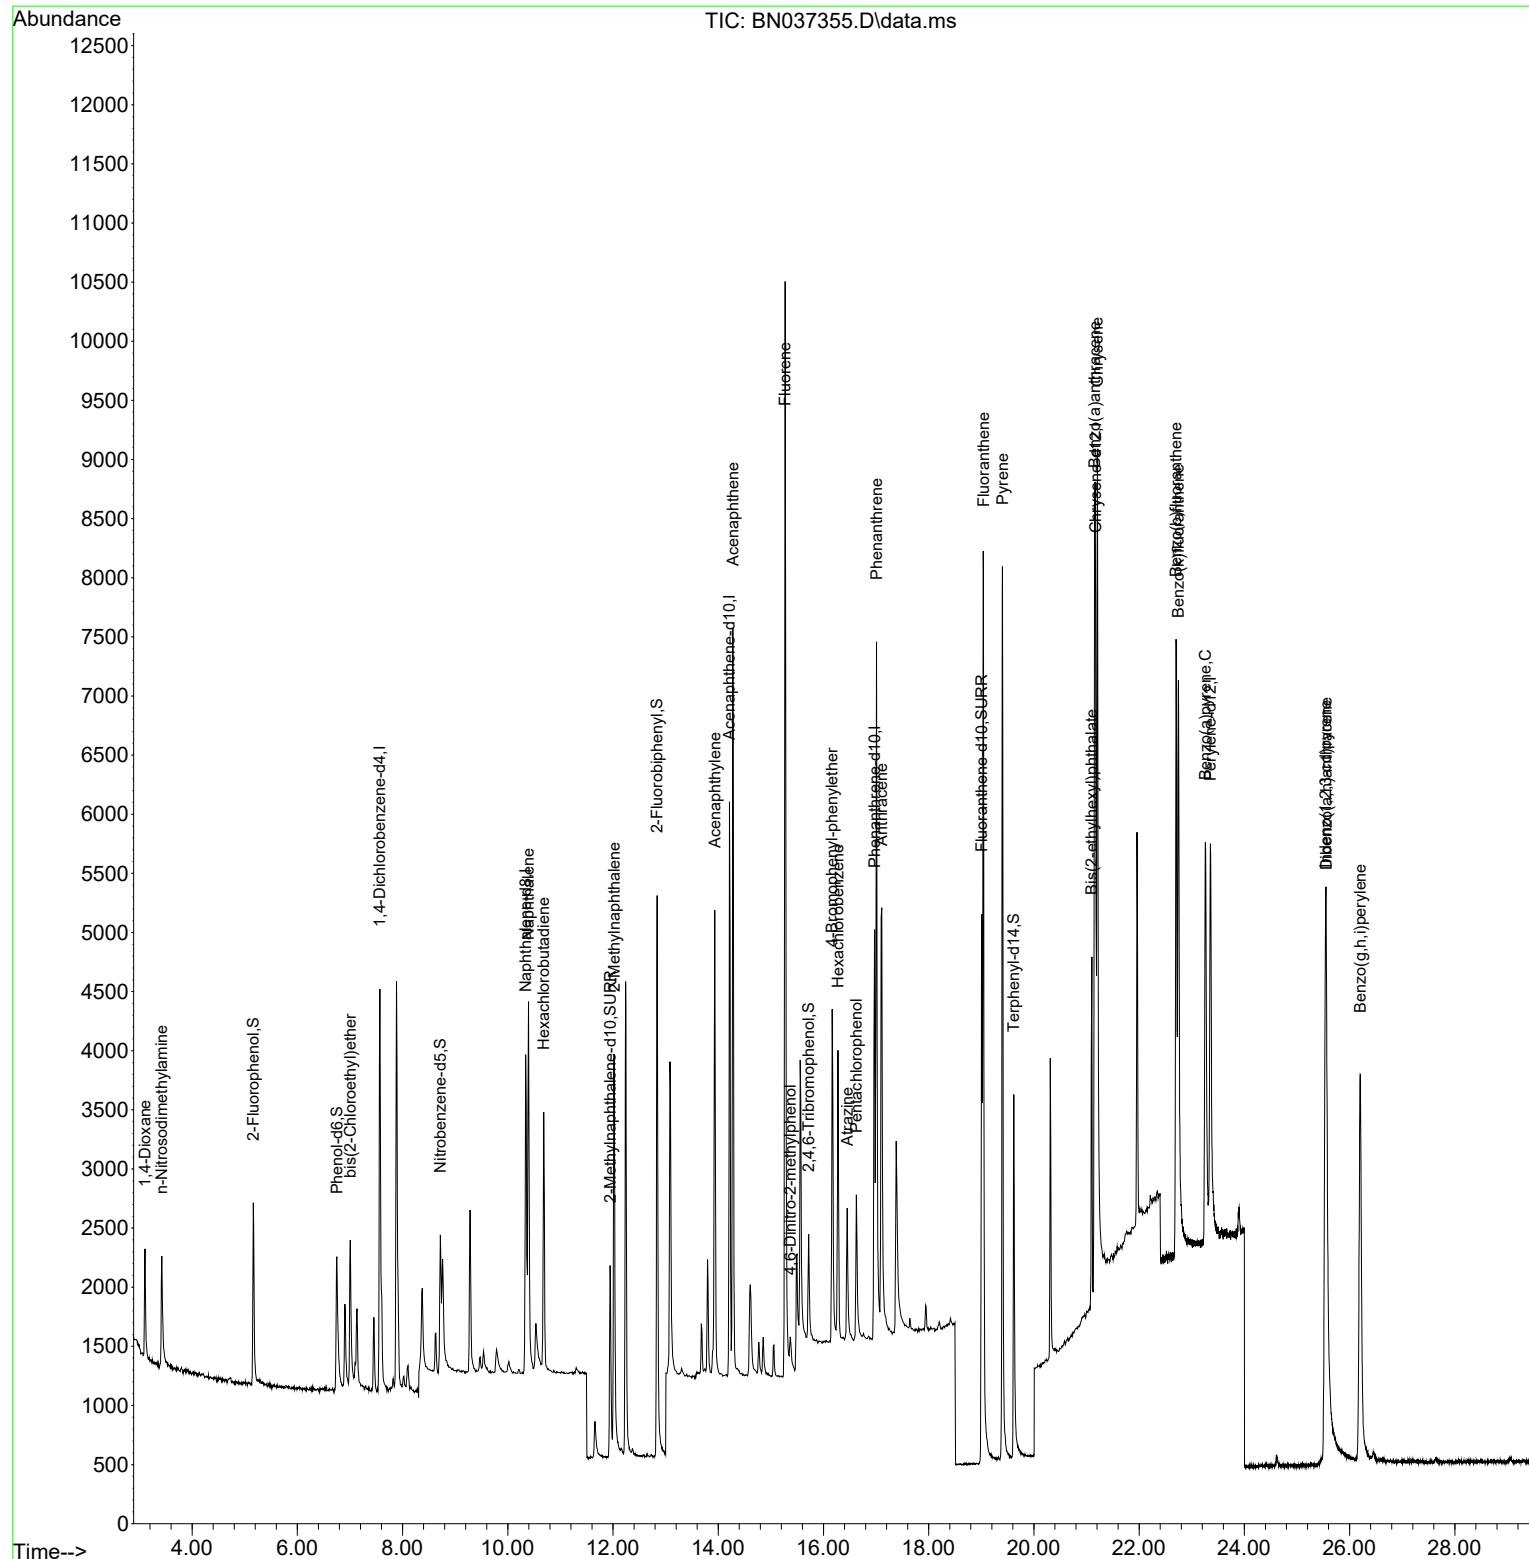



#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03




Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4




Tgt Ion:152 Resp: 191:  
Ion Ratio Lower Upper  
152 100  
150 147.0 112.7 169.1  
115 53.9 45.9 68.9

### Manual Integrations APPROVED



Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025









#2  
1,4-Dioxane  
Concen: 0.441 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03



Tgt Ion: 88 Resp: 745  
Ion Ratio Lower Upper  
88 100  
43 26.3 21.0 31.6  
58 54.1 38.0 57.0

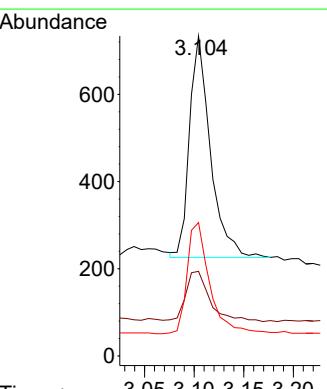



#3

n-Nitrosodimethylamine

Concen: 0.383 ng

RT: 3.422 min Scan# 7

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N


ClientSampleId :

SSTDICCC0.4

### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

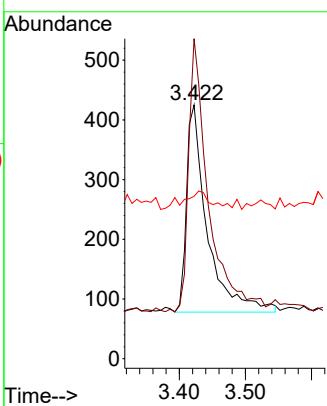

#4

2-Fluorophenol

Concen: 0.411 ng

RT: 5.163 min Scan# 316

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03


Tgt Ion:112 Resp: 1436


Ion Ratio Lower Upper

112 100

64 49.6 38.7 58.1


63 31.1 26.4 39.6



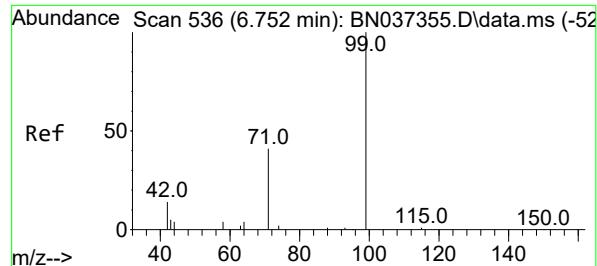

#5  
 Phenol-d6  
 Concen: 0.424 ng  
 RT: 6.752 min Scan# 51  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03




Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4

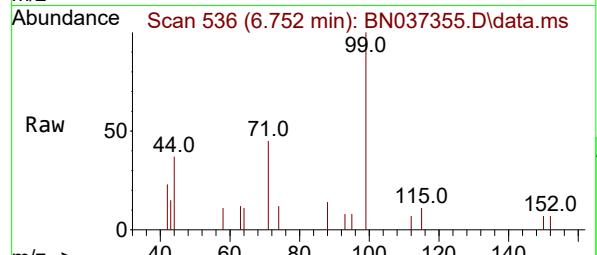




Tgt Ion: 99 Resp: 1469  
 Ion Ratio Lower Upper  
 99 100  
 42 17.0 19.8 29.8  
 71 43.2 42.6 64.0


### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

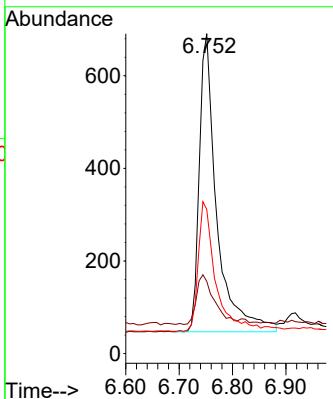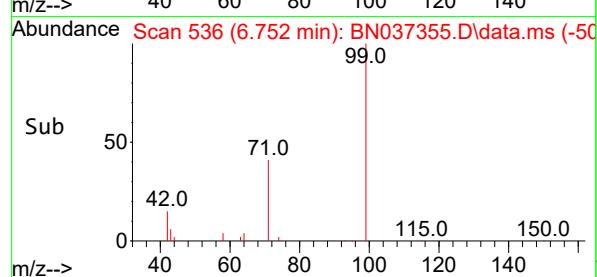


#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.446 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

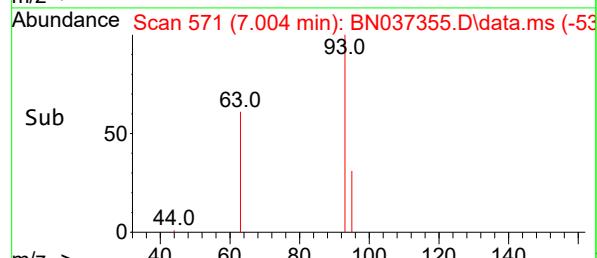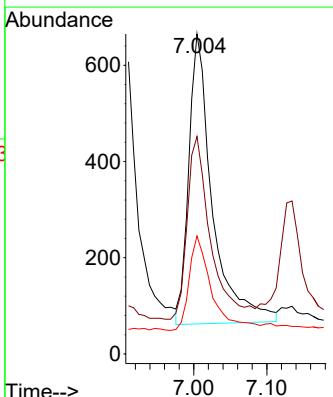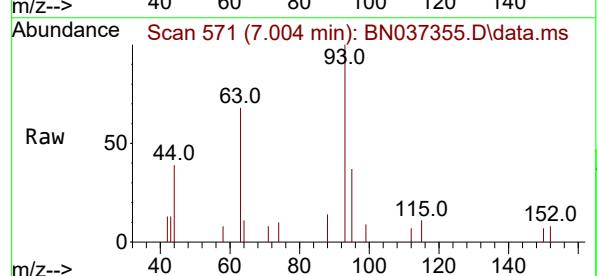



#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.340 min Scan# 9  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03




Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4

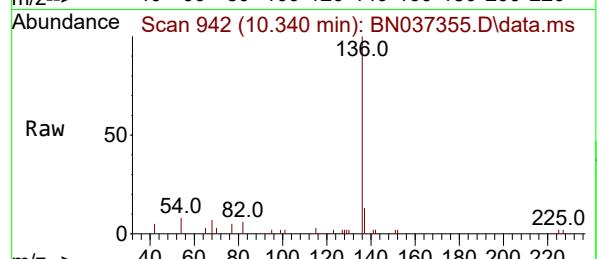


Tgt Ion:136 Resp: 4151  
Ion Ratio Lower Upper  
136 100  
137 12.9 12.2 18.2  
54 8.1 8.8 13.2  
68 6.6 7.0 10.4#

Manual Integrations  
APPROVED



Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

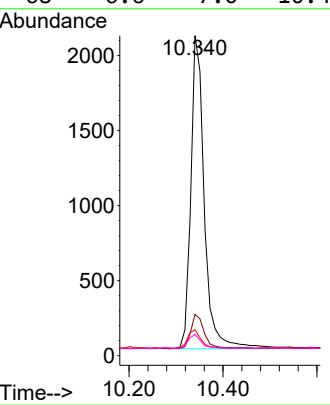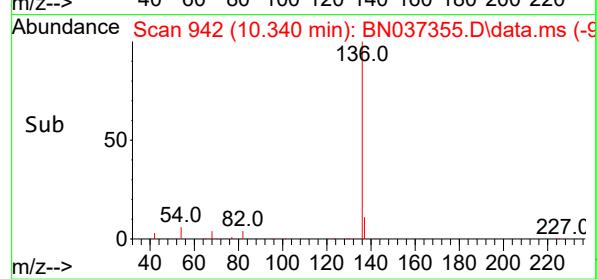


#8  
Nitrobenzene-d5  
Concen: 0.385 ng  
RT: 8.717 min Scan# 790  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03



Tgt Ion: 82 Resp: 1327  
Ion Ratio Lower Upper  
82 100  
128 41.8 42.5 63.7#  
54 47.4 43.2 64.8

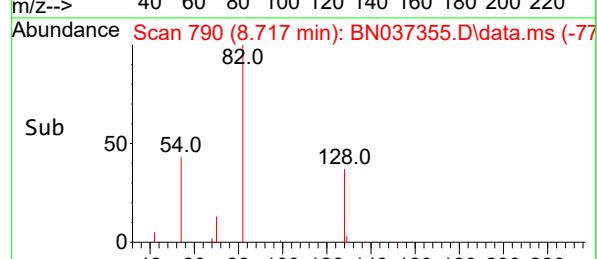



#9

Naphthalene

Concen: 0.403 ng

RT: 10.394 min Scan# 9

Delta R.T. 0.000 min

Lab File: BN037355.D


Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N

ClientSampleId :

SSTDICCC0.4

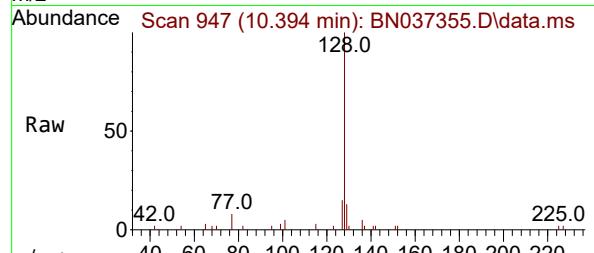

Tgt Ion:128 Resp: 4341

Ion Ratio Lower Upper

128 100




129 12.5 14.0 21.0

127 14.9 15.8 23.8

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

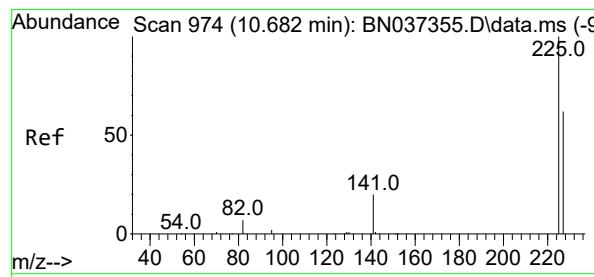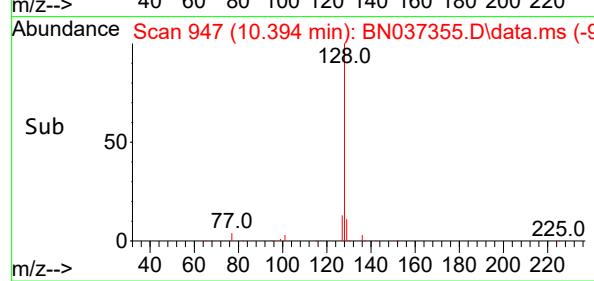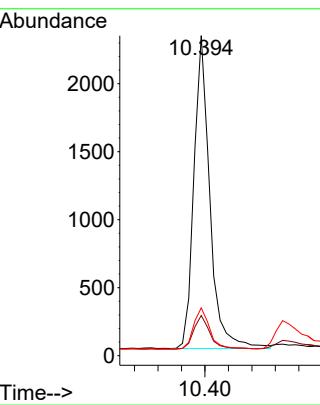

#10

Hexachlorobutadiene

Concen: 0.348 ng

RT: 10.682 min Scan# 974

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03



Tgt Ion:225 Resp: 1832




Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 62.4 50.3 75.5

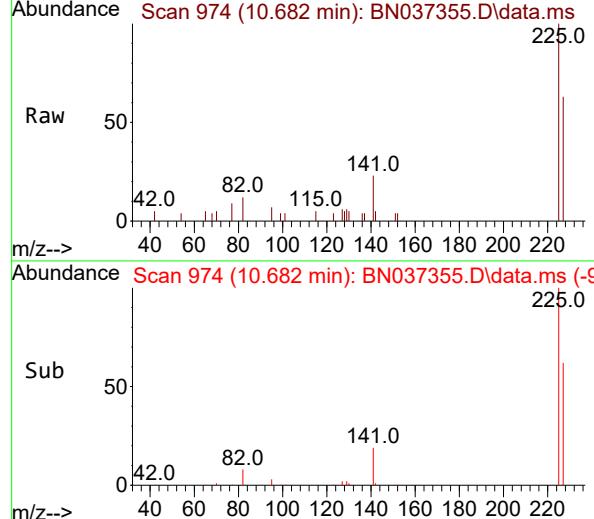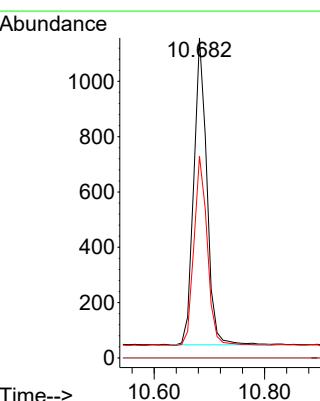


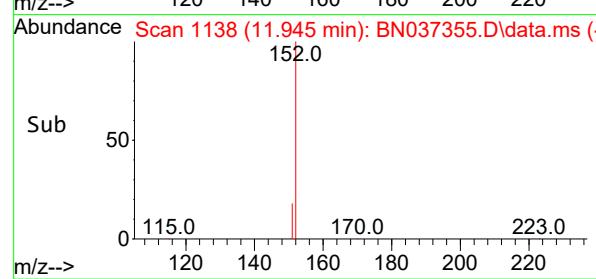




#11  
2-Methylnaphthalene-d10  
Concen: 0.411 ng  
RT: 11.945 min Scan# 1138  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4


### Manual Integrations APPROVED


Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

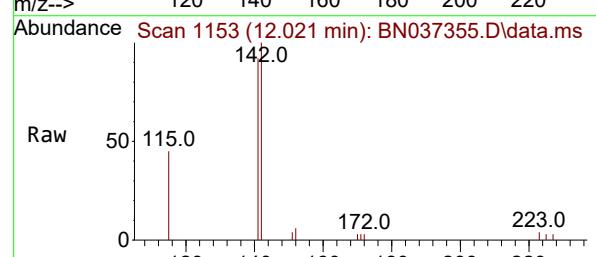



#12  
2-Methylnaphthalene  
Concen: 0.390 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:142 Resp: 2957  
Ion Ratio Lower Upper  
142 100  
141 91.8 70.2 105.2  
115 44.5 43.0 64.4

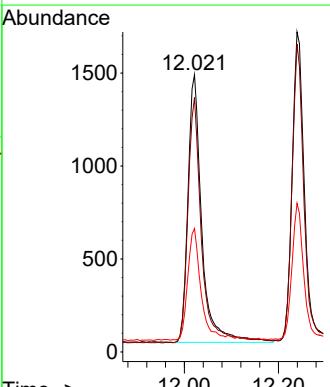


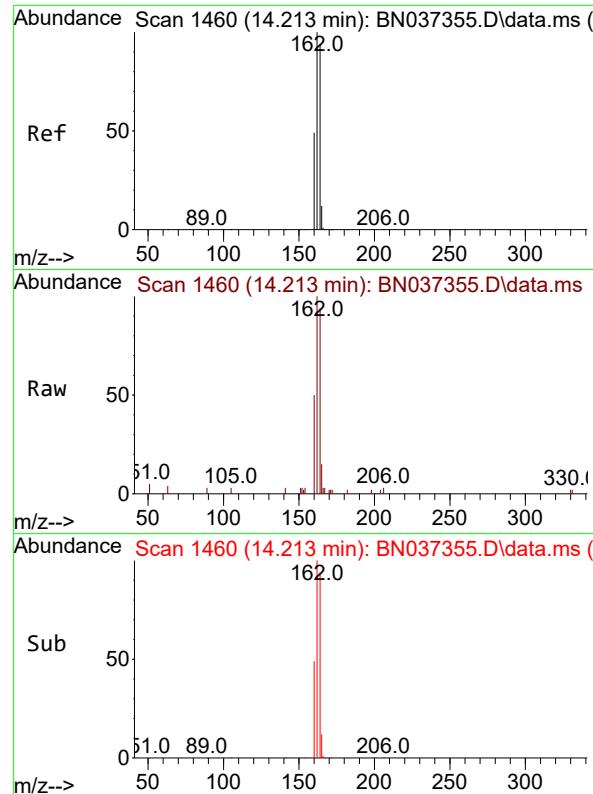


#13

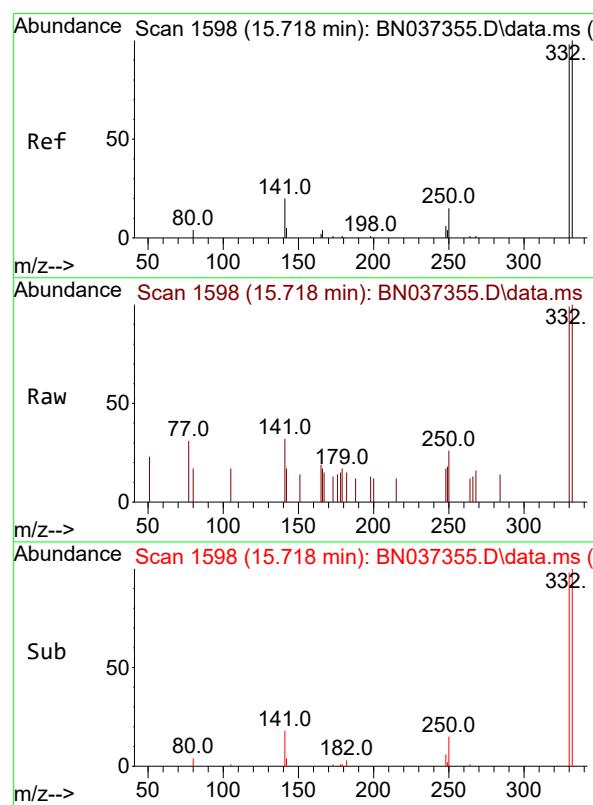Acenaphthene-d10  
Concen: 0.400 ngRT: 14.213 min Scan# 1460  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4**Manual Integrations  
APPROVED**Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

#14

2,4,6-Tribromophenol  
Concen: 0.321 ng  
RT: 15.718 min Scan# 1598  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03Tgt Ion:330 Resp: 646  
Ion Ratio Lower Upper  
330 100  
332 96.3 78.4 117.6  
141 29.6 24.4 36.6

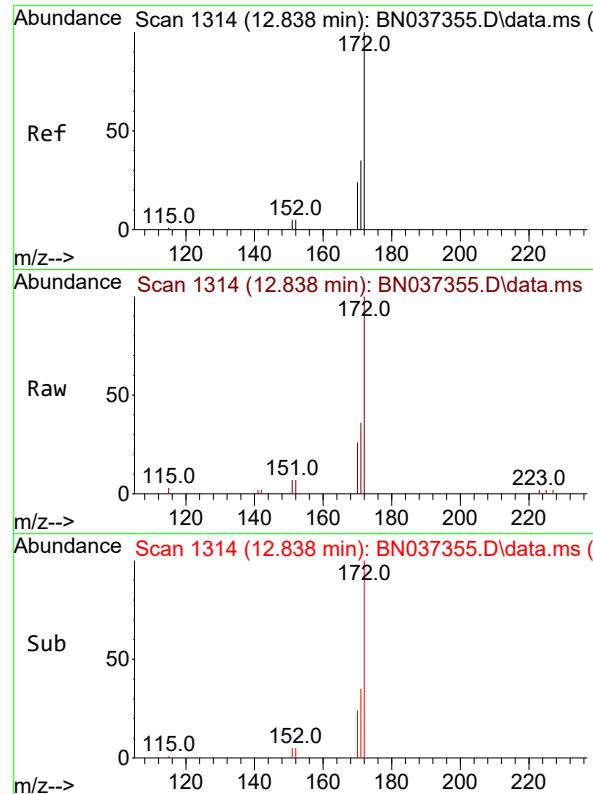



#15  
2-Fluorobiphenyl  
Concen: 0.405 ng  
RT: 12.838 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4

Tgt Ion:172 Resp: 4990  
Ion Ratio Lower Upper  
172 100  
171 36.2 30.8 46.2  
170 25.6 21.9 32.9


### Manual Integrations APPROVED




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

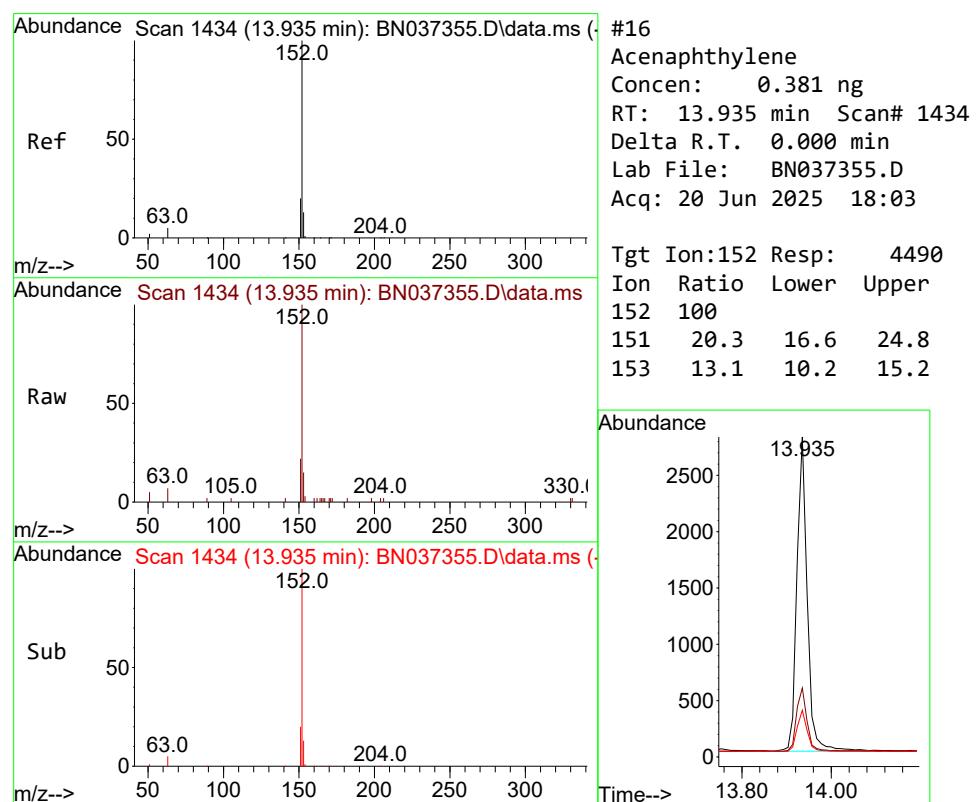

#16  
Acenaphthylene  
Concen: 0.381 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:152 Resp: 4490  
Ion Ratio Lower Upper  
152 100  
151 20.3 16.6 24.8  
153 13.1 10.2 15.2





#17

Acenaphthene

Concen: 0.381 ng

RT: 14.277 min Scan# 1466

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N





ClientSampleId :

SSTDICCC0.4

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

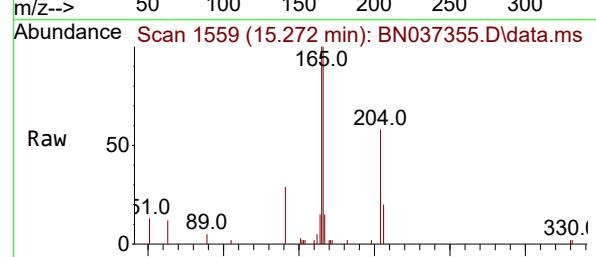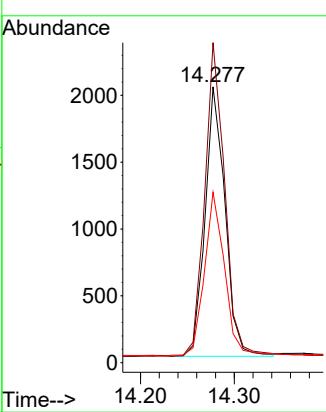

#18

Fluorene

Concen: 0.382 ng


RT: 15.272 min Scan# 1559


Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Tgt	Ion:166	Resp:	4232
Ion	Ratio	Lower	Upper
166	100		
165	99.8	79.5	119.3
167	13.6	10.7	16.1

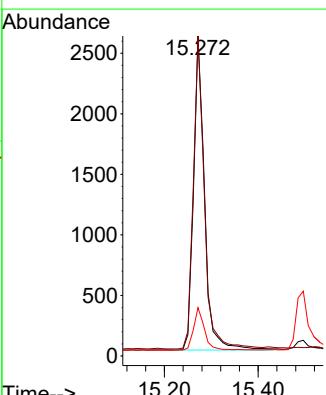

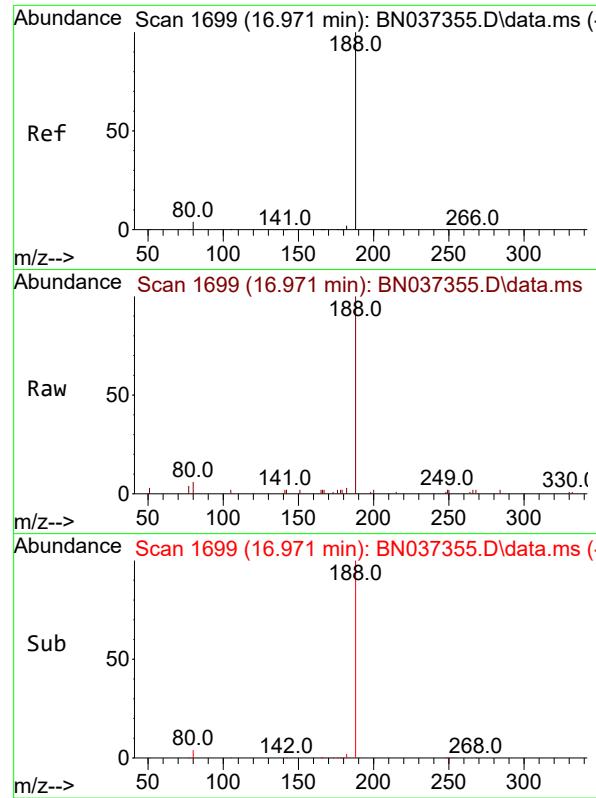

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N



ClientSampleId :

SSTDICCC0.4

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

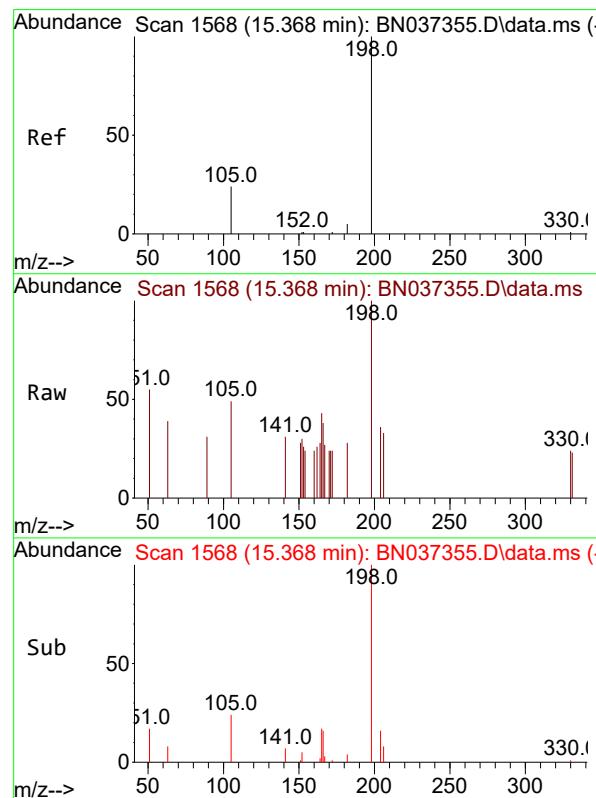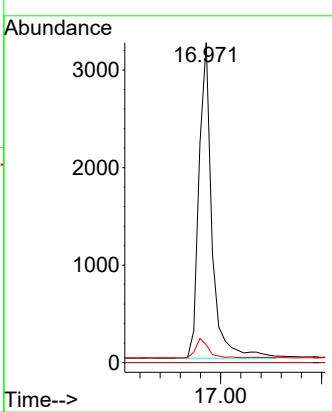

#20

4,6-Dinitro-2-methylphenol

Concen: 0.263 ng


RT: 15.368 min Scan# 1568


Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Tgt	Ion:198	Resp:	459
Ion	Ratio	Lower	Upper
198	100		
51	55.4	51.4	77.0
105	49.2	45.5	68.3




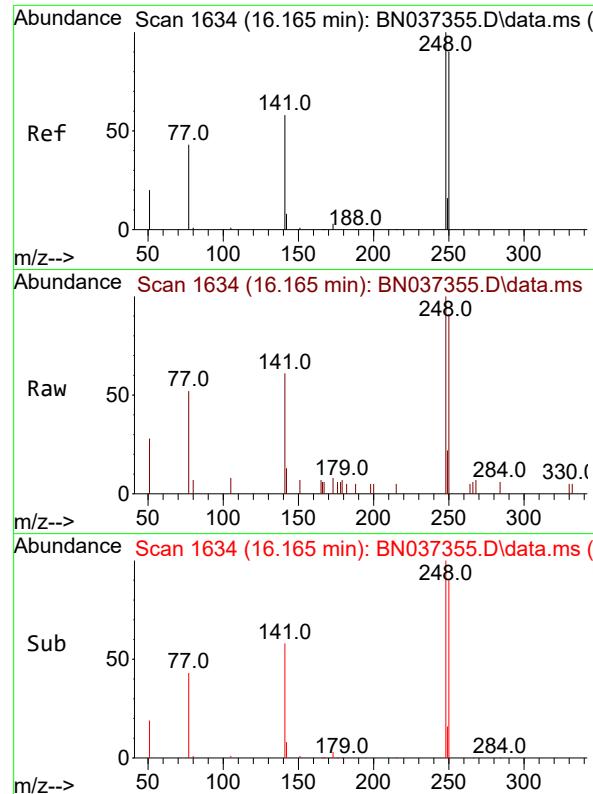


#21  
4-Bromophenyl-phenylether  
Concen: 0.342 ng  
RT: 16.165 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

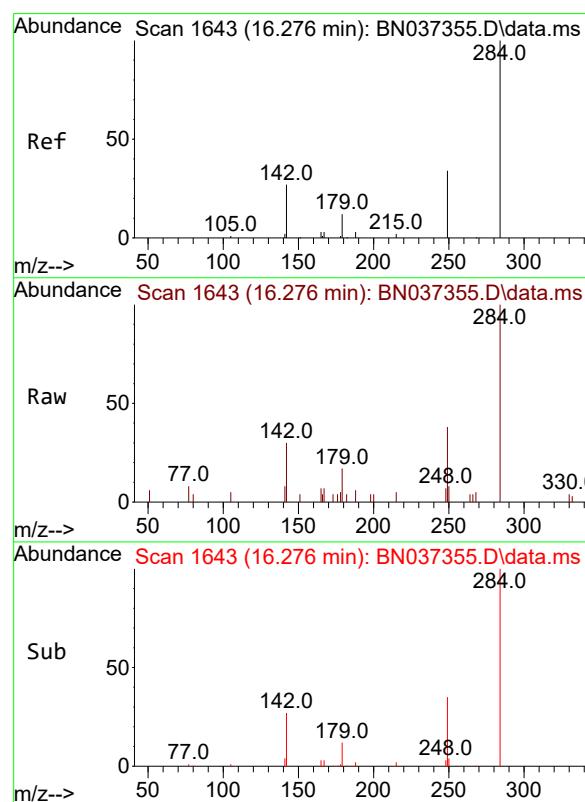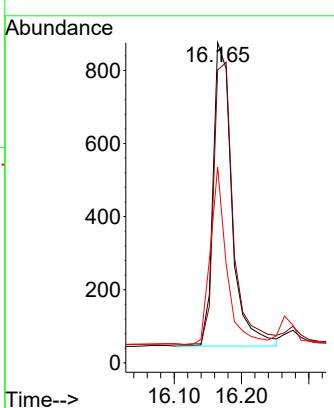

#22  
Hexachlorobenzene  
Concen: 0.369 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:284 Resp: 1814  
Ion Ratio Lower Upper  
284 100  
142 34.2 27.0 40.6  
249 34.2 28.8 43.2

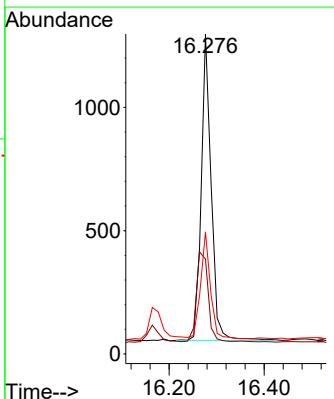

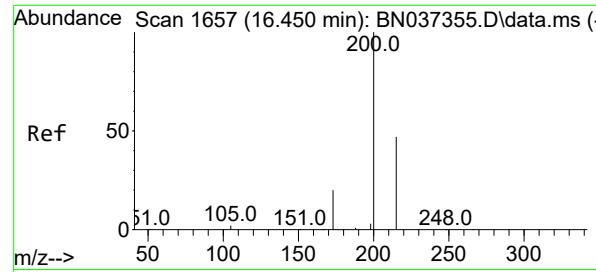

#23

Atrazine

Concen: 0.342 ng

RT: 16.450 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N





ClientSampleId :

SSTDICCC0.4

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#24

Pentachlorophenol

Concen: 0.293 ng

RT: 16.624 min Scan# 1671


Delta R.T. 0.000 min




Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Tgt Ion:266 Resp: 792

Ion	Ratio	Lower	Upper
266	100		
264	64.3	50.3	75.5
268	67.4	55.3	82.9

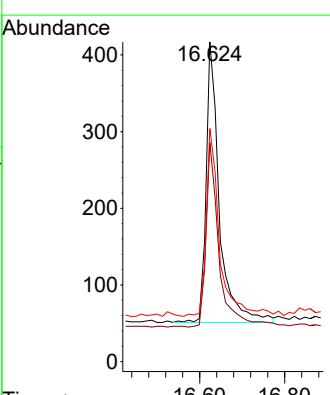

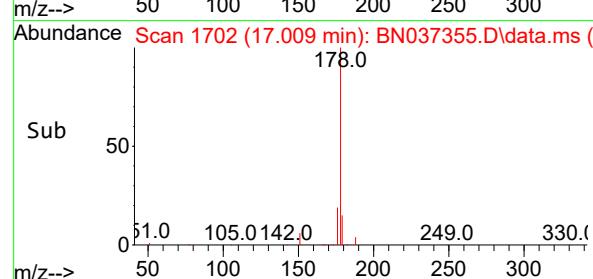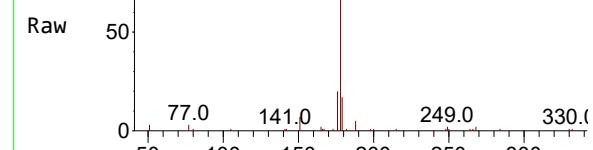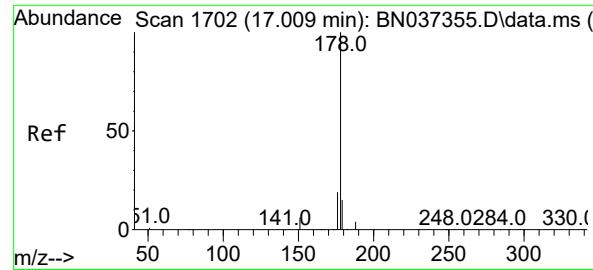

#25

Phenanthrene

Concen: 0.391 ng

RT: 17.009 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N




ClientSampleId :

SSTDICCC0.4

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

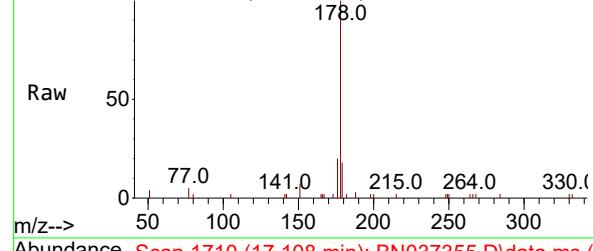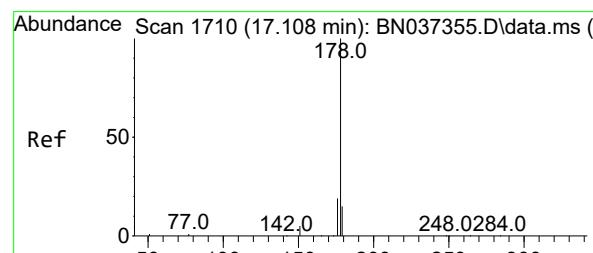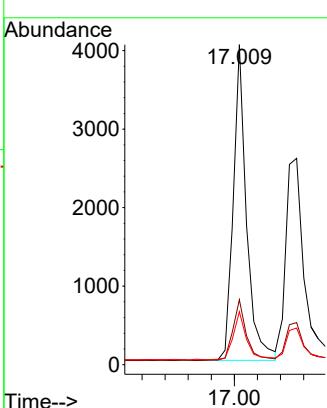

#26

Anthracene

Concen: 0.375 ng


RT: 17.108 min Scan# 1710


Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Tgt	Ion:178	Resp:	5717
Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.7	22.1
179	15.2	13.0	19.6




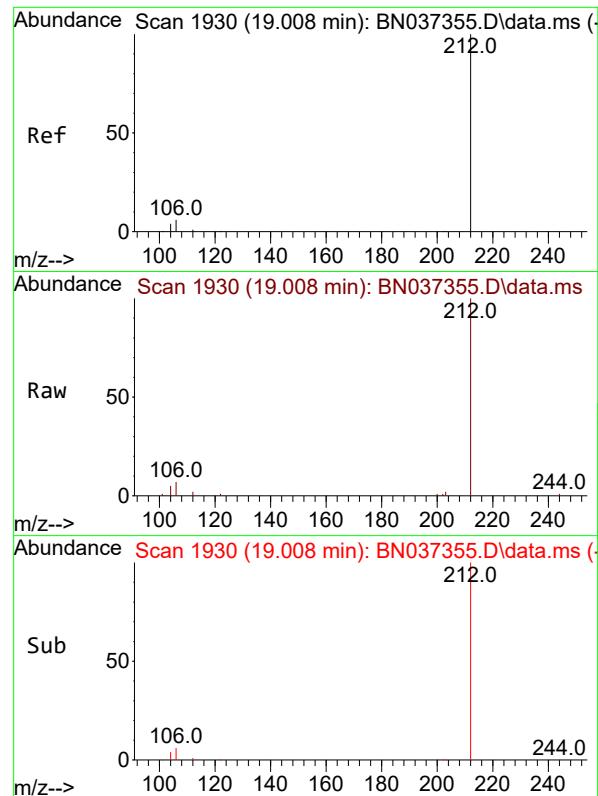


#27  
**Fluoranthene-d10**  
Concen: 0.373 ng  
RT: 19.008 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4


1 Manual Integrations  
2 APPROVED




3 Reviewed By :Rahul Chavli 06/23/2025  
4 Supervised By :Jagrut Upadhyay 06/24/2025

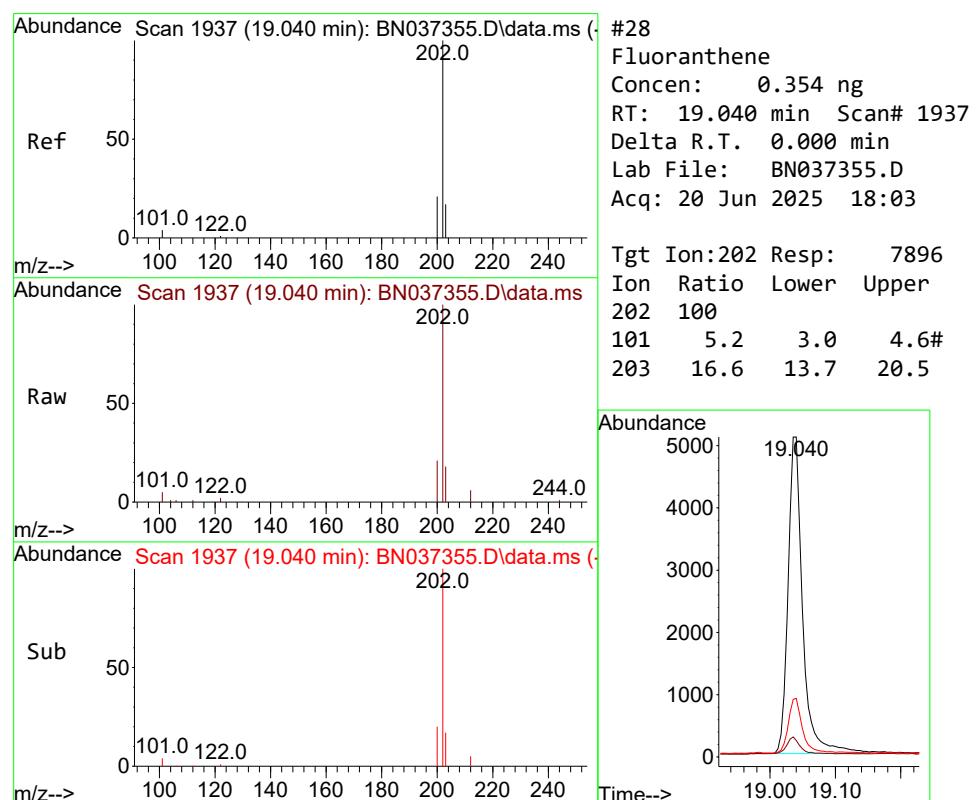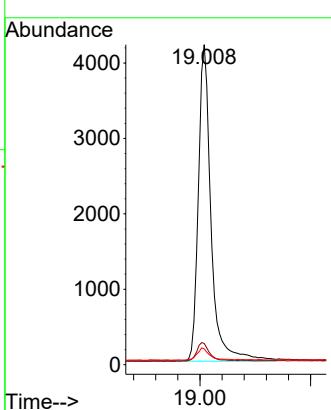

#28  
**Fluoranthene**  
Concen: 0.354 ng  
RT: 19.040 min Scan# 1937  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:202 Resp: 7896  
Ion Ratio Lower Upper  
202 100  
101 5.2 3.0 4.6#  
203 16.6 13.7 20.5

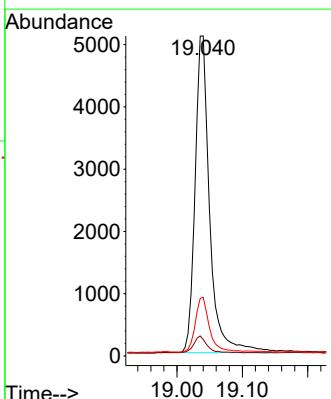



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.171 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N




ClientSampleId :

SSTDICCC0.4

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#30

Pyrene

Concen: 0.434 ng

RT: 19.402 min Scan# 2015

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03


Tgt Ion:202 Resp: 7990


Ion Ratio Lower Upper

202 100

200 21.1 16.8 25.2

203 18.0 14.5 21.7

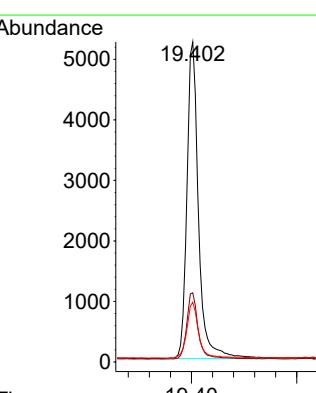


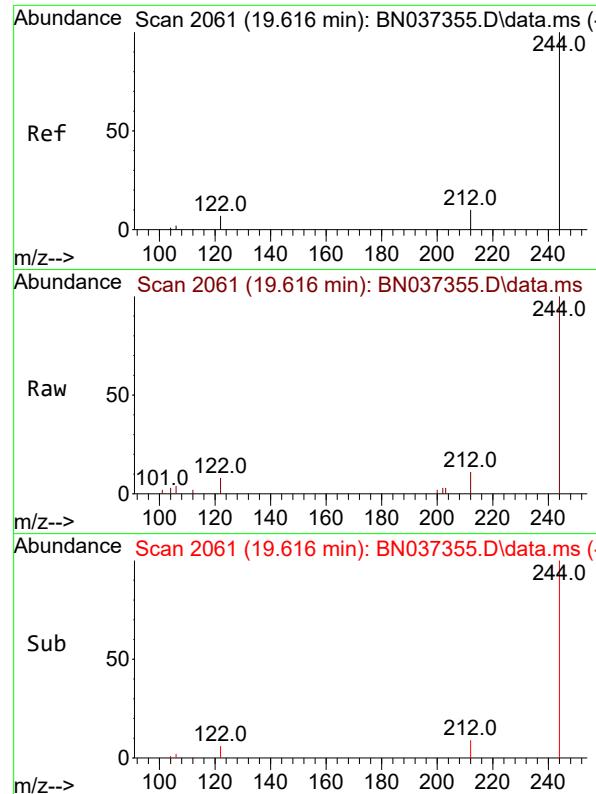


#31  
Terphenyl-d14  
Concen: 0.405 ng  
RT: 19.616 min Scan# 2  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

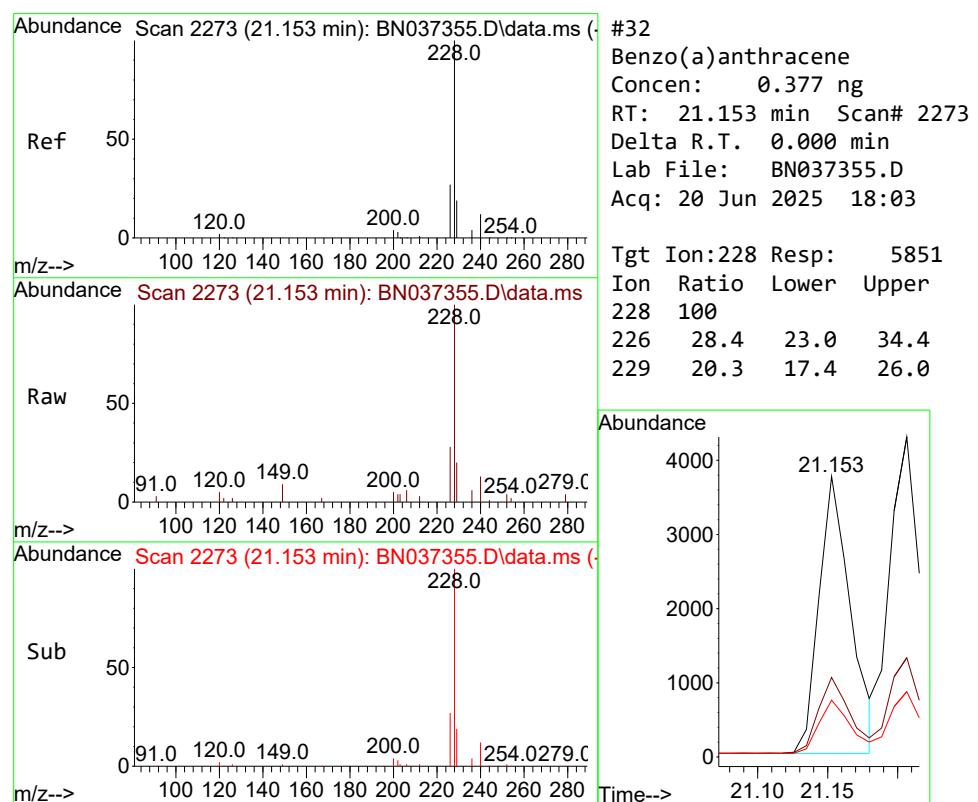

#32  
Benzo(a)anthracene  
Concen: 0.377 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:228 Resp: 5851  
Ion Ratio Lower Upper  
228 100  
226 28.4 23.0 34.4  
229 20.3 17.4 26.0



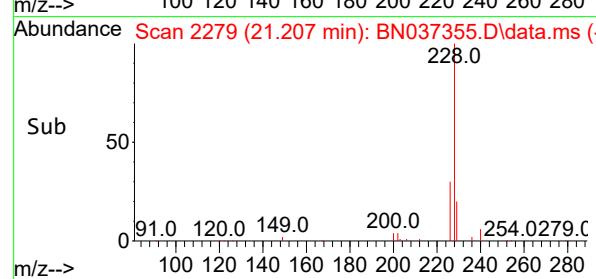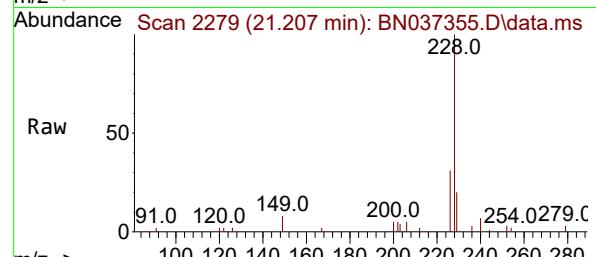

#33

Chrysene

Concen: 0.394 ng

RT: 21.207 min Scan# 2

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N





ClientSampleId :

SSTDICCC0.4

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

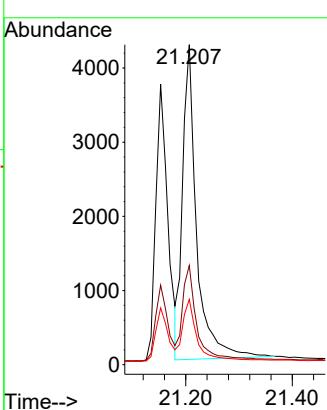

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.409 ng

RT: 21.099 min Scan# 2267

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03


Tgt Ion:149 Resp: 2603


Ion Ratio Lower Upper

149 100

167 31.9 24.6 37.0

279 7.2 6.5 9.7

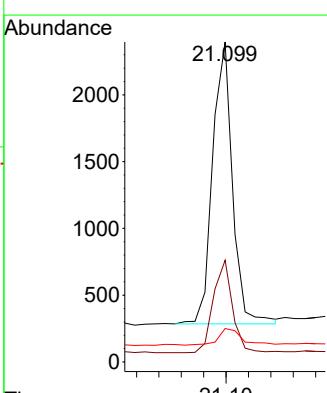


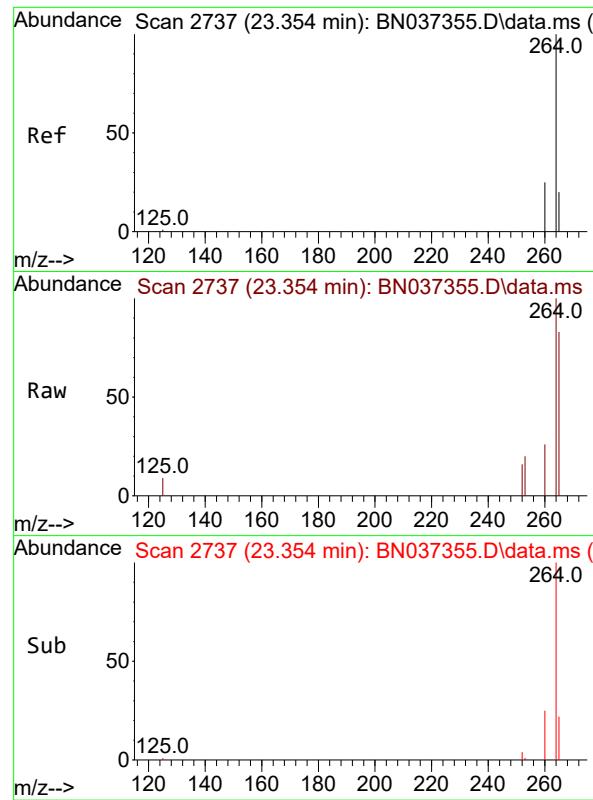


#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.354 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

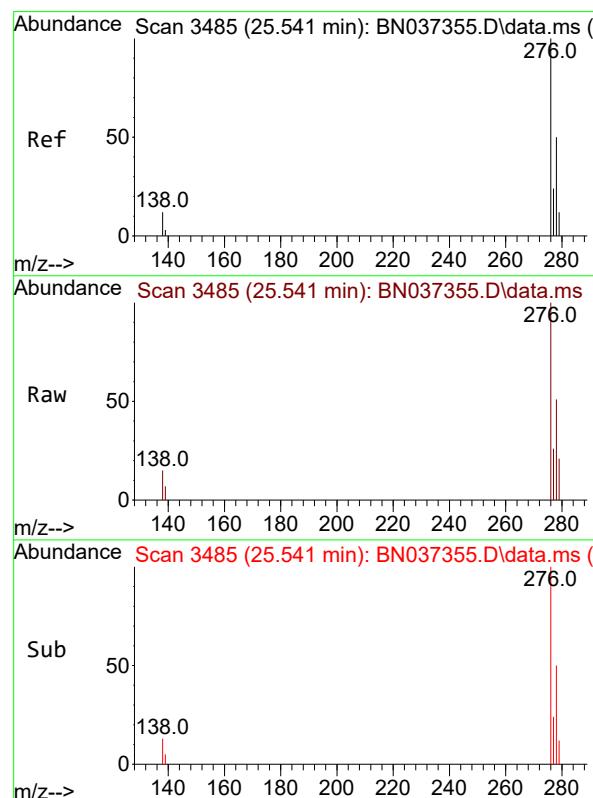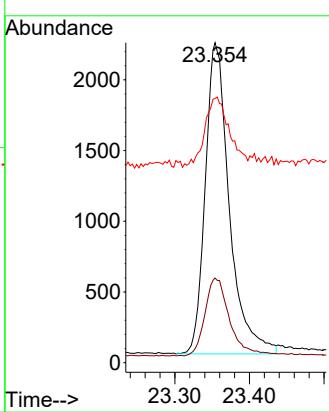

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.400 ng  
 RT: 25.541 min Scan# 3485  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

Tgt Ion:276 Resp: 8379  
 Ion Ratio Lower Upper  
 276 100  
 138 11.3 2.2 3.2#  
 277 23.4 17.1 25.7

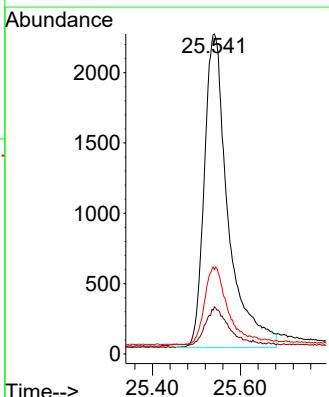

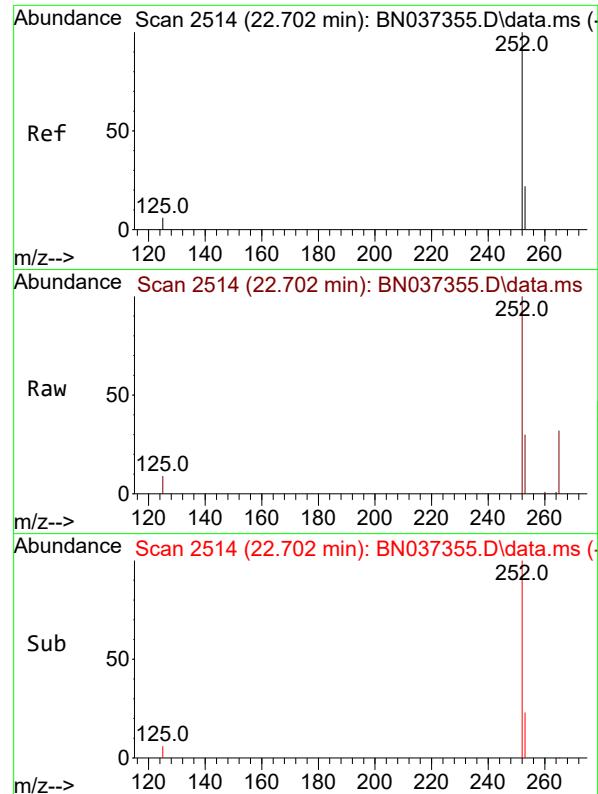

#37

Benzo(b)fluoranthene

Concen: 0.407 ng m

RT: 22.702 min Scan# 2

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N



ClientSampleId :

SSTDICCC0.4

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

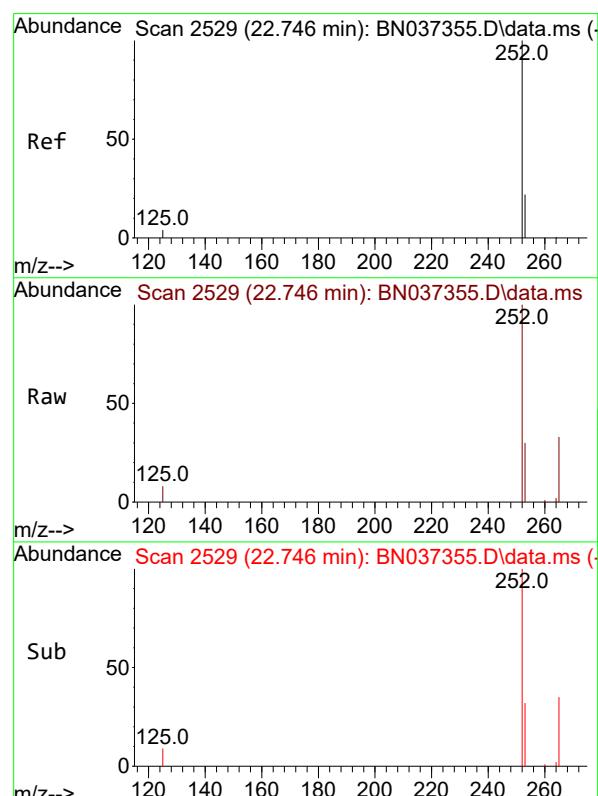

#38

Benzo(k)fluoranthene

Concen: 0.407 ng

RT: 22.746 min Scan# 2529


Delta R.T. 0.000 min


Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Tgt Ion:252 Resp: 7755

Ion	Ratio	Lower	Upper
252	100		
253	30.3	26.7	40.1
125	8.5	6.5	9.7

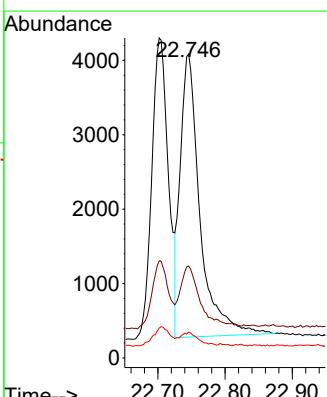

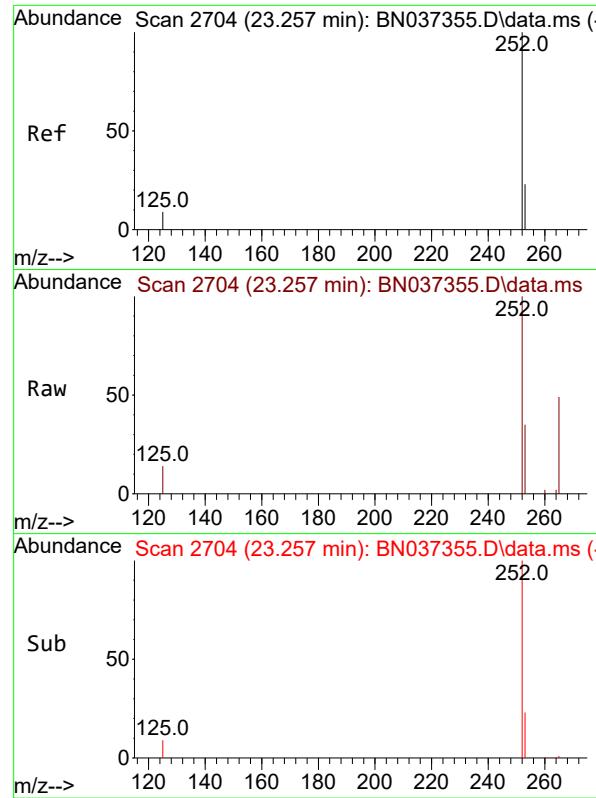

#39

Benzo(a)pyrene

Concen: 0.393 ng

RT: 23.257 min Scan# 2

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N

ClientSampleId :

SSTDICCC0.4



**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

Abundance

23.257

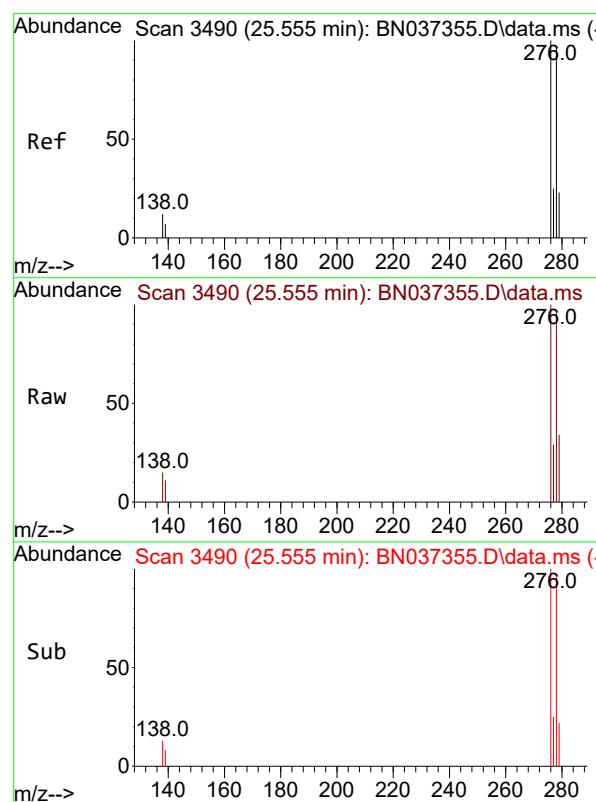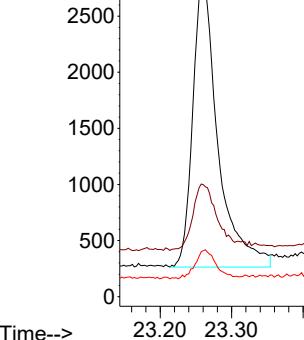

#40

Dibenzo(a,h)anthracene

Concen: 0.366 ng

RT: 25.555 min Scan# 3490

Delta R.T. 0.000 min


Lab File: BN037355.D


Acq: 20 Jun 2025 18:03

Tgt	Ion:278	Resp:	6108
Ion	Ratio	Lower	Upper
278	100		
139	11.3	10.2	15.4
279	35.1	35.6	53.4

Abundance

25.555

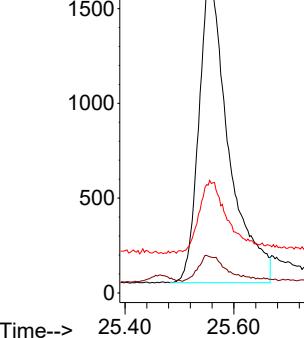

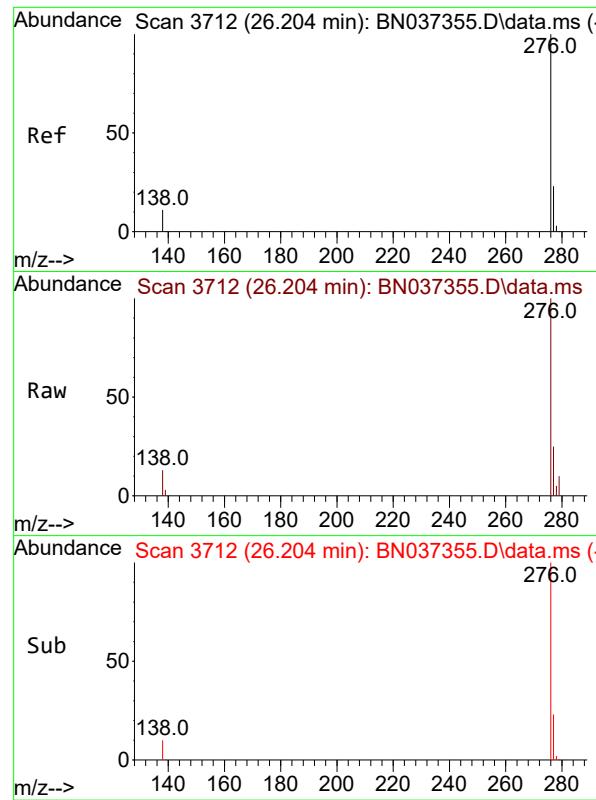


#41  
Benzo(g,h,i)perylene  
Concen: 0.408 ng  
RT: 26.204 min Scan# 3  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

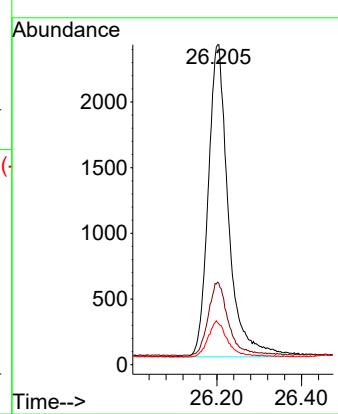

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037356.D  
 Acq On : 20 Jun 2025 18:39  
 Operator : RC/JU  
 Sample : SSTDICCO.8  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCO.8

Quant Time: Jun 20 23:27:16 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2011	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4268	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2836	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5716	0.400	ng	# 0.00
29) Chrysene-d12	21.162	240	5944	0.400	ng	0.00
35) Perylene-d12	23.351	264	6423	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	3141	0.854	ng	0.00
5) Phenol-d6	6.744	99	3157	0.868	ng	0.00
8) Nitrobenzene-d5	8.717	82	2717	0.767	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	5209	0.754	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	1310	0.646	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	9720	0.781	ng	0.00
27) Fluoranthene-d10	19.003	212	13334	0.749	ng	0.00
31) Terphenyl-d14	19.616	244	9859	0.726	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	1657	0.933	ng	93
3) n-Nitrosodimethylamine	3.415	42	1478	0.715	ng	# 74
6) bis(2-Chloroethyl)ether	7.004	93	2967	0.932	ng	96
9) Naphthalene	10.394	128	8659	0.783	ng	# 87
10) Hexachlorobutadiene	10.682	225	3472	0.642	ng	# 99
12) 2-Methylnaphthalene	12.016	142	6007	0.772	ng	93
16) Acenaphthylene	13.935	152	9047	0.760	ng	99
17) Acenaphthene	14.277	154	5960	0.755	ng	100
18) Fluorene	15.272	166	8453	0.756	ng	100
20) 4,6-Dinitro-2-methylph...	15.368	198	1108	0.641	ng	# 55
21) 4-Bromophenyl-phenylether	16.165	248	3252	0.697	ng	# 89
22) Hexachlorobenzene	16.276	284	3471	0.713	ng	98
23) Atrazine	16.450	200	2516	0.689	ng	# 82
24) Pentachlorophenol	16.624	266	1797	0.673	ng	96
25) Phenanthrene	17.009	178	13016	0.806	ng	99
26) Anthracene	17.096	178	12050	0.799	ng	99
28) Fluoranthene	19.035	202	17056	0.772	ng	# 99
30) Pyrene	19.398	202	17163	0.754	ng	100
32) Benzo(a)anthracene	21.153	228	15193	0.792	ng	97
33) Chrysene	21.198	228	17610	0.724	ng	98
34) Bis(2-ethylhexyl)phtha...	21.099	149	5787	0.736	ng	# 97
36) Indeno(1,2,3-cd)pyrene	25.535	276	22625	0.831	ng	# 91
37) Benzo(b)fluoranthene	22.696	252	17878	0.785	ng	# 87
38) Benzo(k)fluoranthene	22.740	252	18833	0.761	ng	# 86
39) Benzo(a)pyrene	23.257	252	16022	0.769	ng	# 84
40) Dibenzo(a,h)anthracene	25.547	278	17405	0.803	ng	# 77
41) Benzo(g,h,i)perylene	26.202	276	20041	0.801	ng	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037356.D  
 Acq On : 20 Jun 2025 18:39  
 Operator : RC/JU  
 Sample : SSTDICC0.8  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC0.8


Quant Time: Jun 20 23:27:16 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration

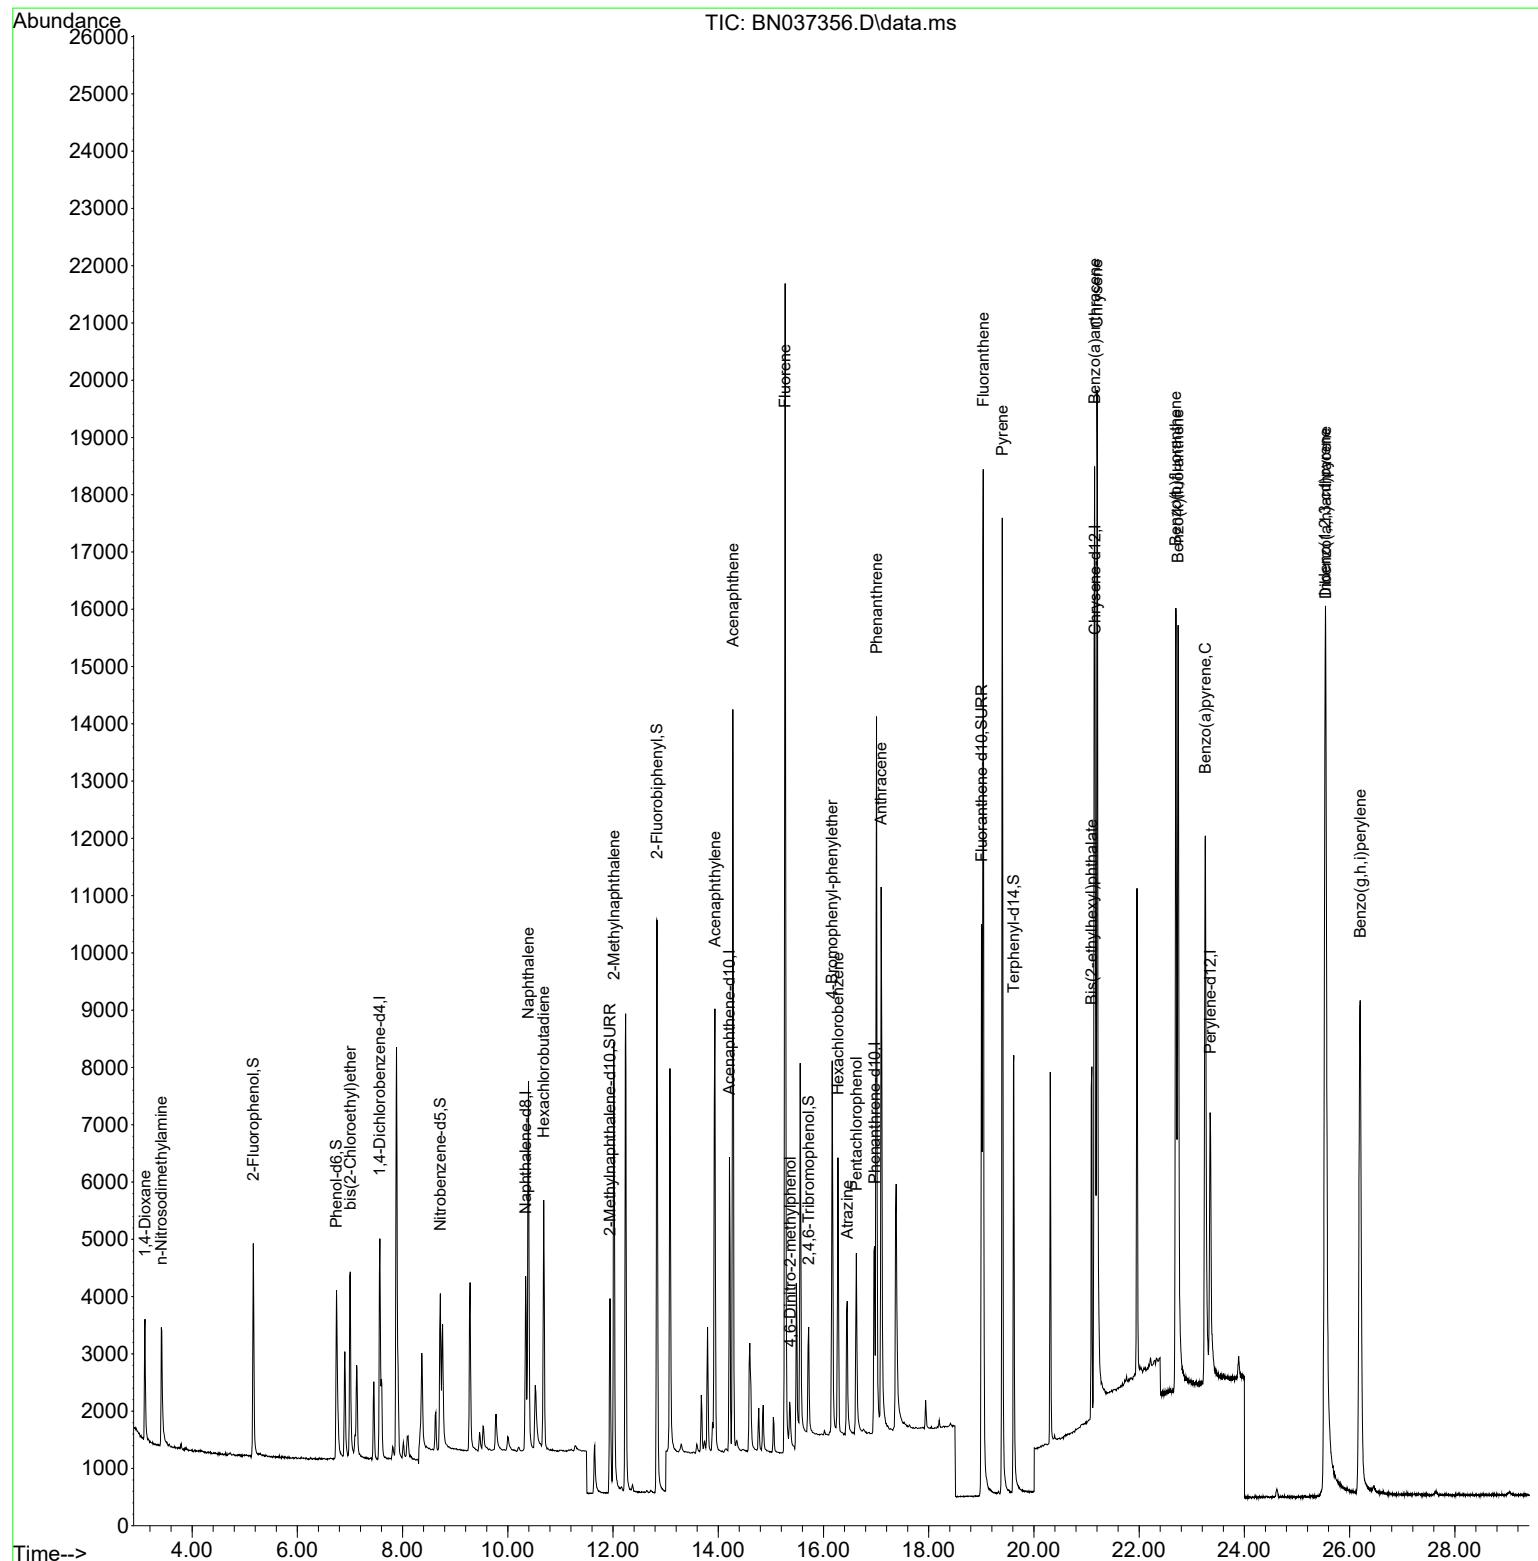






#1  
 1,4-Dichlorobenzene-d4  
 Concen: 0.400 ng  
 RT: 7.568 min Scan# 6  
 Delta R.T. -0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8





Tgt Ion:152 Resp: 2011  
 Ion Ratio Lower Upper  
 152 100  
 150 148.2 112.7 169.1  
 115 55.2 45.9 68.9

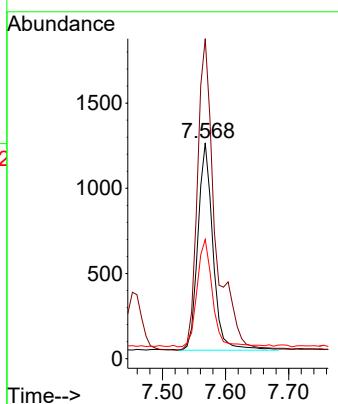




#2  
 1,4-Dioxane  
 Concen: 0.933 ng  
 RT: 3.104 min Scan# 31  
 Delta R.T. -0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39



Tgt Ion: 88 Resp: 1657  
 Ion Ratio Lower Upper  
 88 100  
 43 23.4 21.0 31.6  
 58 52.7 38.0 57.0

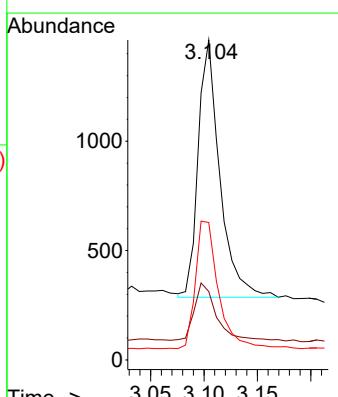

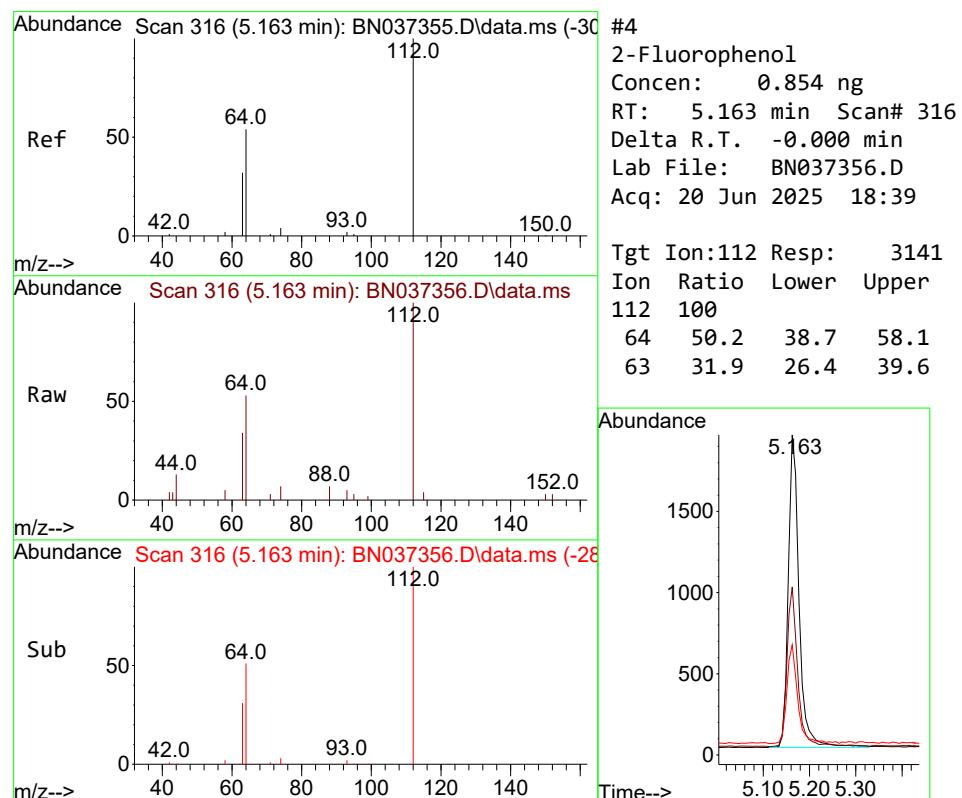
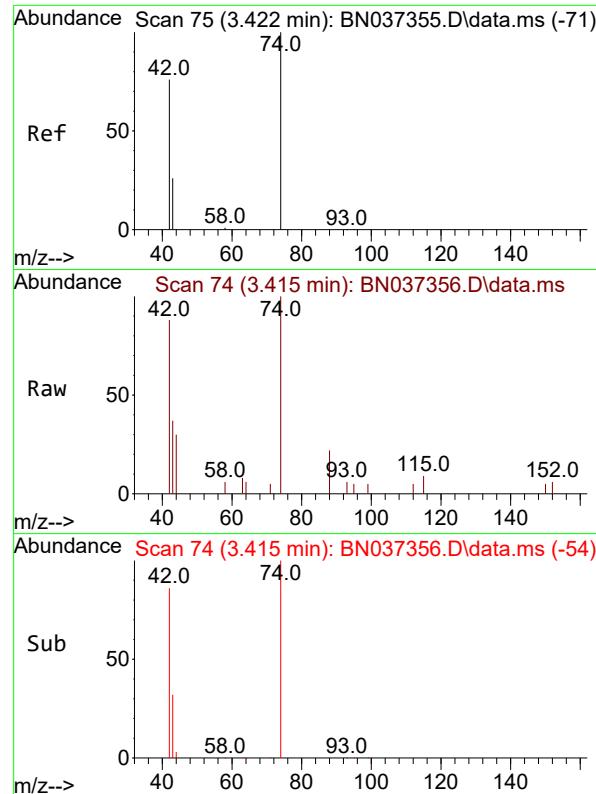


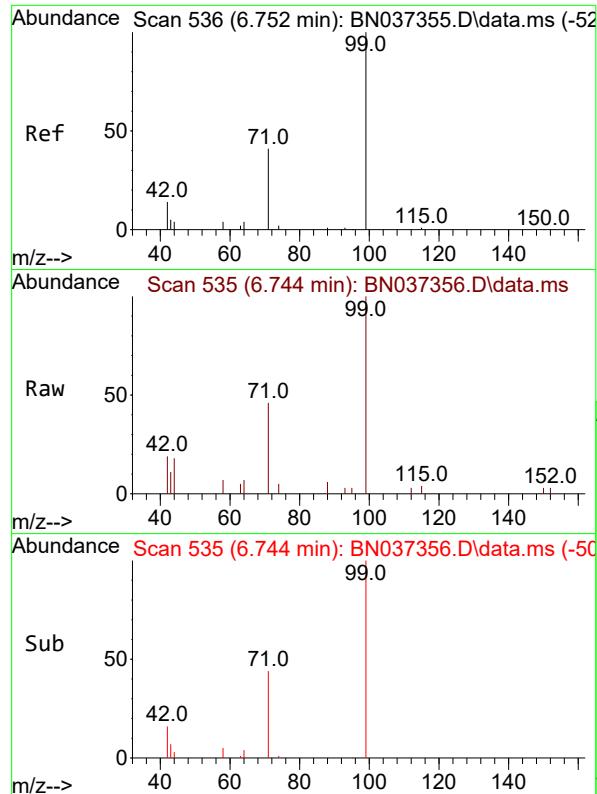

#5  
 Phenol-d6  
 Concen: 0.868 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. -0.007 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion: 99 Resp: 3157  
 Ion Ratio Lower Upper  
 99 100  
 42 17.5 19.8 29.8#  
 71 43.4 42.6 64.0

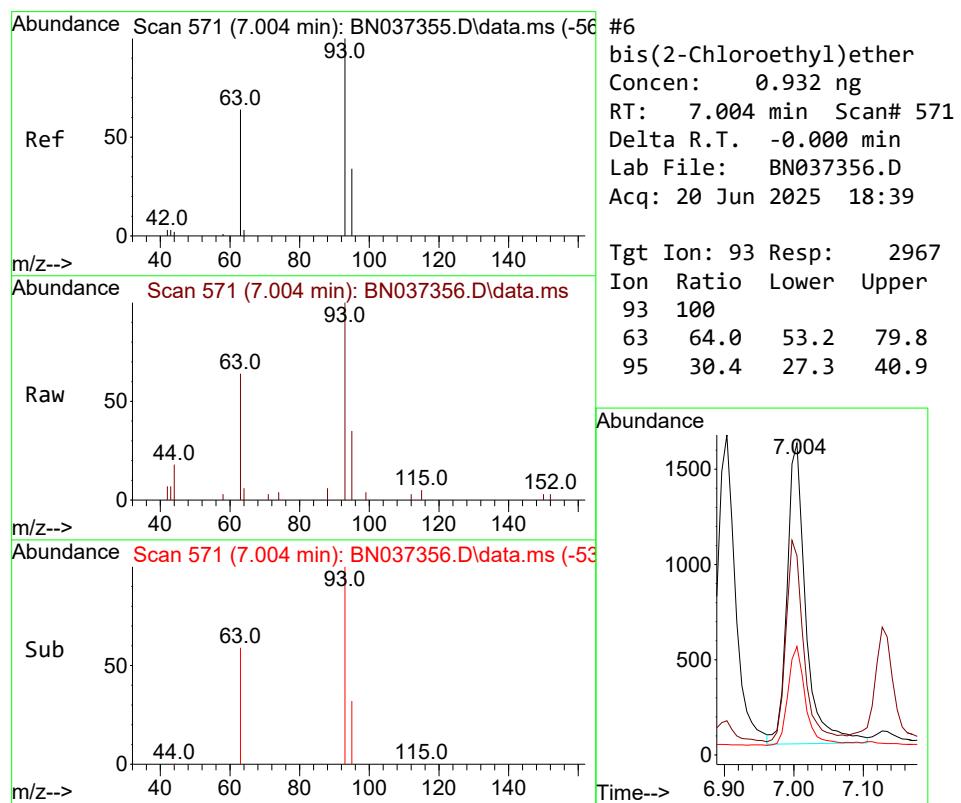

#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.932 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. -0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39

Tgt Ion: 93 Resp: 2967  
 Ion Ratio Lower Upper  
 93 100  
 63 64.0 53.2 79.8  
 95 30.4 27.3 40.9


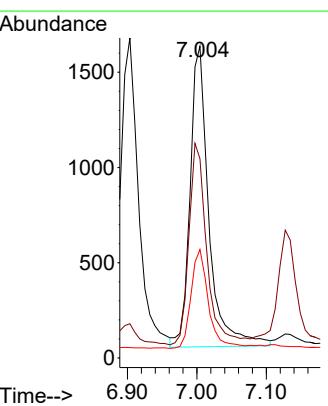


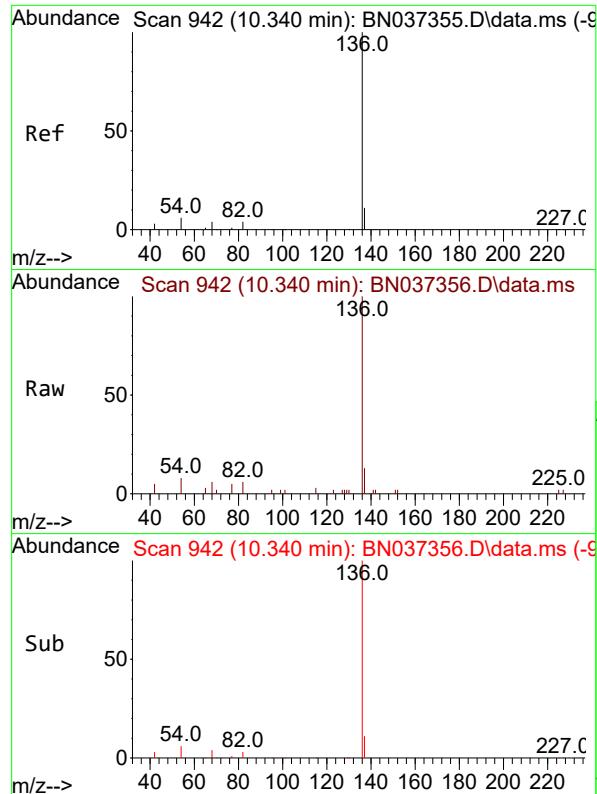

#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:136 Resp: 4268  
 Ion Ratio Lower Upper  
 136 100  
 137 12.5 12.2 18.2  
 54 8.0 8.8 13.2#  
 68 6.3 7.0 10.4#

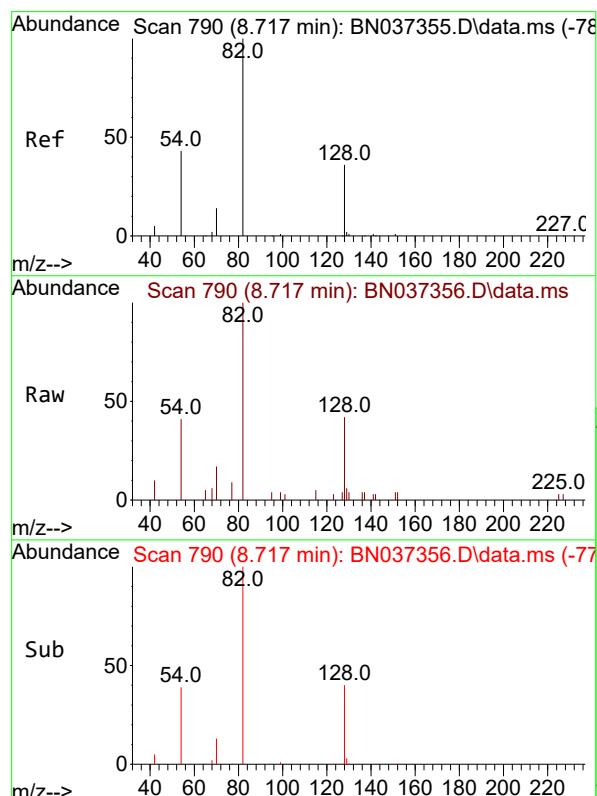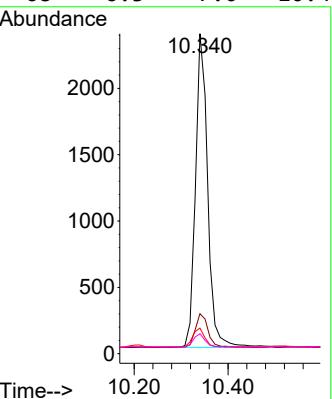


#8  
 Nitrobenzene-d5  
 Concen: 0.767 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. -0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39

Tgt Ion: 82 Resp: 2717  
 Ion Ratio Lower Upper  
 82 100  
 128 42.2 42.5 63.7#  
 54 41.4 43.2 64.8#


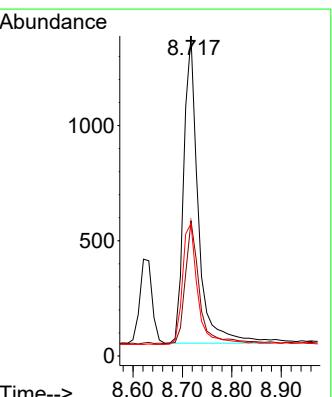


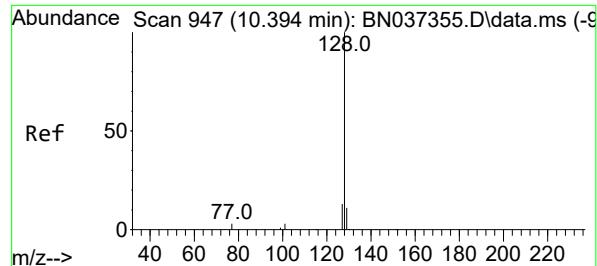


#9  
Naphthalene  
Concen: 0.783 ng  
RT: 10.394 min Scan# 9  
Instrument :  
Delta R.T. -0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39  
ClientSampleId : SSTDICCO.8





Tgt Ion:128 Resp: 8659  
Ion Ratio Lower Upper  
128 100  
129 11.7 14.0 21.0#  
127 14.3 15.8 23.8#

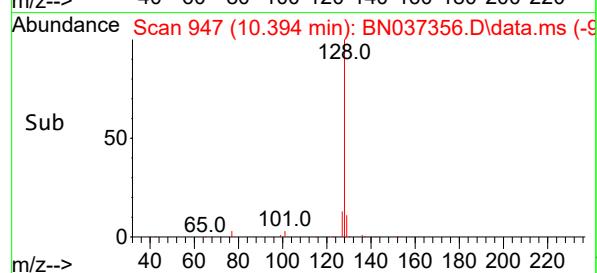


#10  
Hexachlorobutadiene  
Concen: 0.642 ng  
RT: 10.682 min Scan# 974  
Delta R.T. -0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39


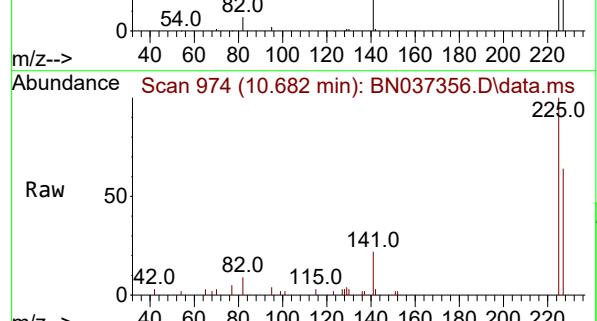


Tgt Ion:225 Resp: 3472  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 63.6 50.3 75.5






Abundance Scan 1137 (11.940 min): BN037356.D\data.ms (-)

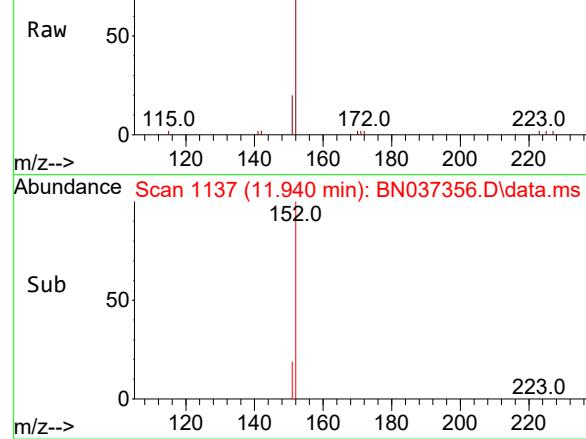

Abundance Scan 1152 (12.016 min): BN037356.D\data.ms (-)

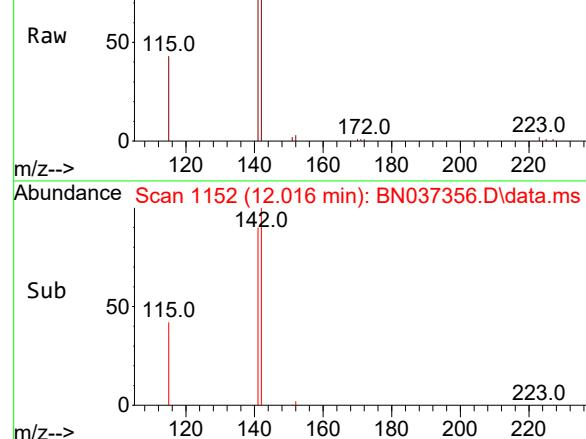

#11

2-Methylnaphthalene-d10

Concen: 0.754 ng

RT: 11.940 min Scan# 1

Delta R.T. -0.005 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39

Instrument :

BNA\_N

ClientSampleId :

SSTDICC0.8

Tgt Ion:152 Resp: 5209


Ion Ratio Lower Upper

152 100

151 21.4 17.4 26.0

Abundance

11.940

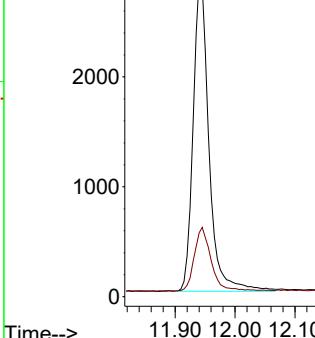

#12

2-Methylnaphthalene

Concen: 0.772 ng

RT: 12.016 min Scan# 1152

Delta R.T. -0.005 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39

Tgt Ion:142 Resp: 6007

Ion Ratio Lower Upper


142 100


141 89.7 70.2 105.2

115 43.4 43.0 64.4

Abundance

12.016

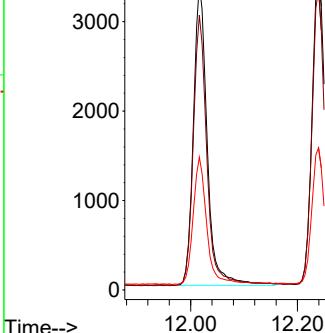

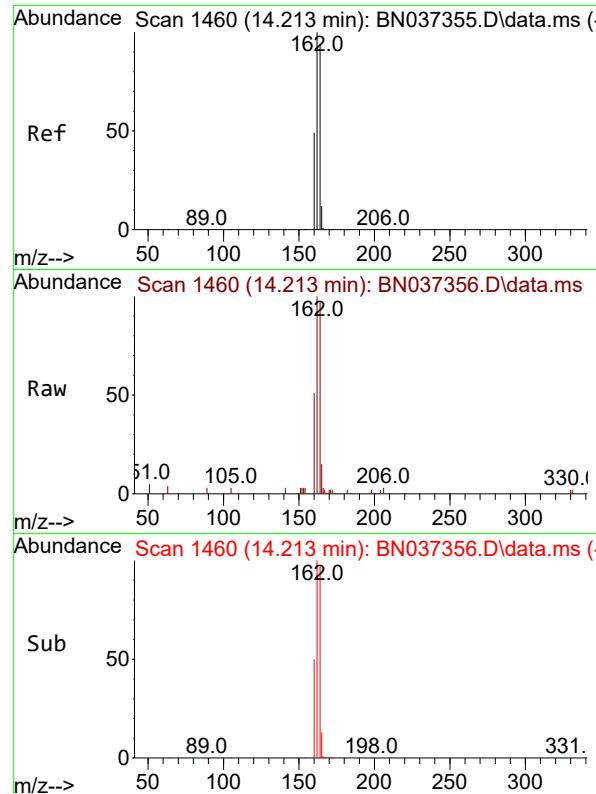

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39

Instrument :

BNA\_N

ClientSampleId :

SSTDICC0.8



Tgt Ion:164 Resp: 2836

Ion Ratio Lower Upper

164 100

162 103.4 81.5 122.3

160 52.7 43.0 64.4

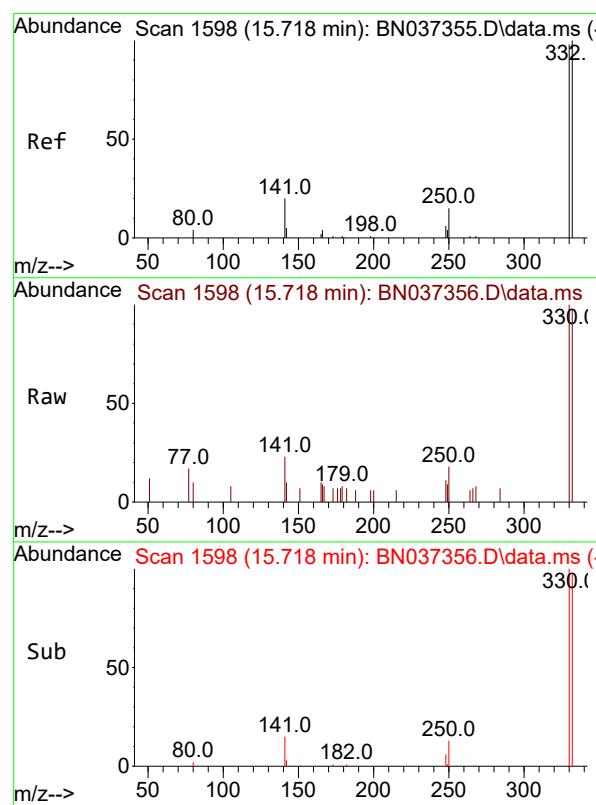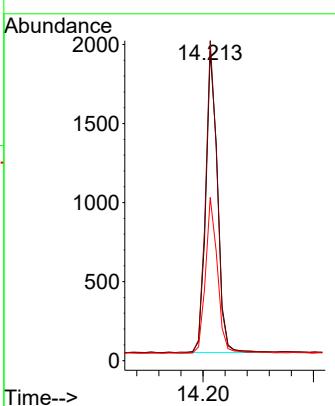

#14

2,4,6-Tribromophenol

Concen: 0.646 ng

RT: 15.718 min Scan# 1598

Delta R.T. -0.000 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39


Tgt Ion:330 Resp: 1310


Ion Ratio Lower Upper

330 100

332 96.3 78.4 117.6



141 32.2 24.4 36.6

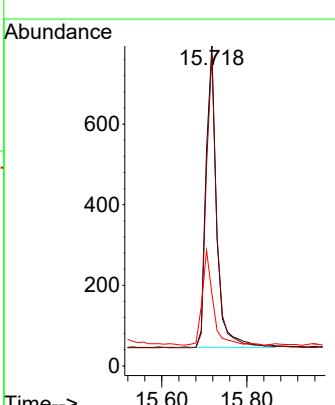

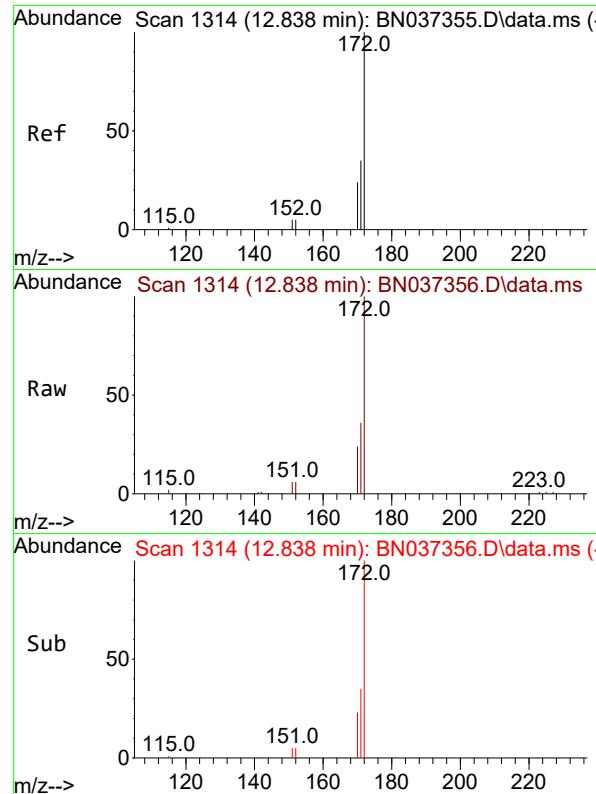


#15  
2-Fluorobiphenyl  
Concen: 0.781 ng  
RT: 12.838 min Scan# 1  
Instrument: BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39  
ClientSampleId : SSTDICCO.8




Tgt Ion:172 Resp: 9720  
Ion Ratio Lower Upper  
172 100  
171 35.5 30.8 46.2  
170 23.9 21.9 32.9

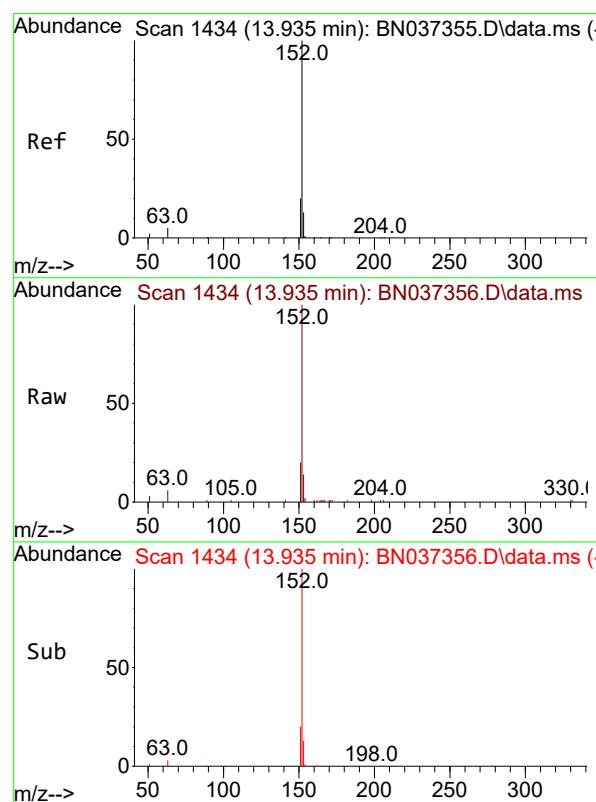

#16  
Acenaphthylene  
Concen: 0.760 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39

Tgt Ion:152 Resp: 9047  
Ion Ratio Lower Upper  
152 100  
151 20.1 16.6 24.8  
153 13.4 10.2 15.2



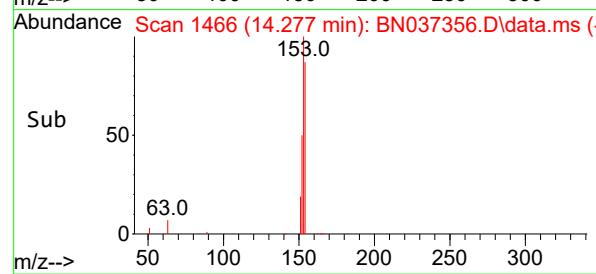

#17

Acenaphthene

Concen: 0.755 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39

Instrument :

BNA\_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:154 Resp: 5960

Ion Ratio Lower Upper

154 100

153 116.3 93.1 139.7

152 60.6 48.6 73.0

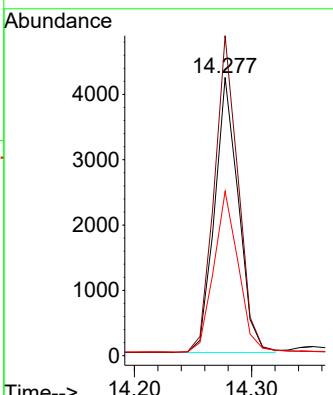

#18

Fluorene

Concen: 0.756 ng

RT: 15.272 min Scan# 1559

Delta R.T. 0.000 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39


Tgt Ion:166 Resp: 8453


Ion Ratio Lower Upper

166 100

165 99.0 79.5 119.3

167 13.3 10.7 16.1


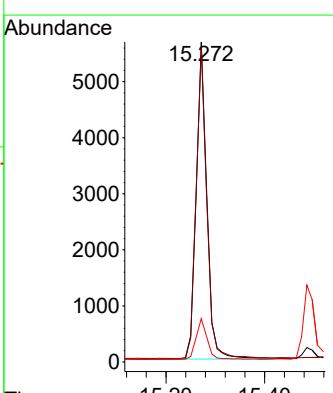


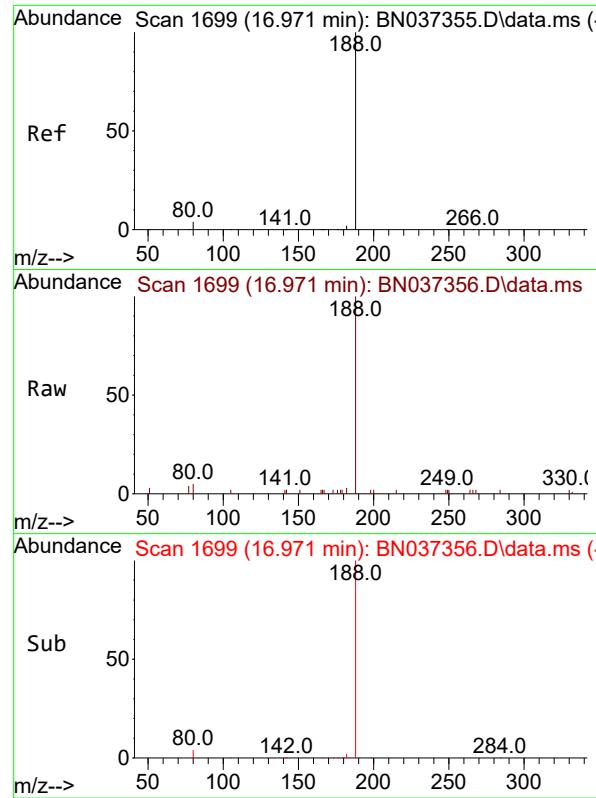

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:188 Resp: 5716  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 5.5 6.2 9.2#

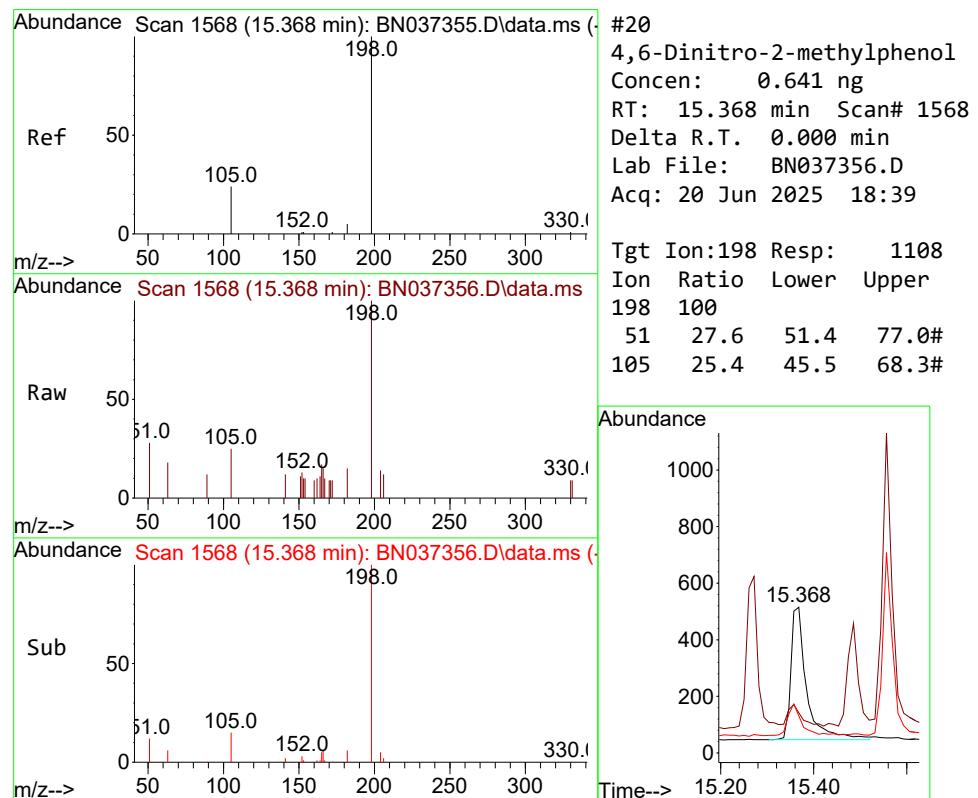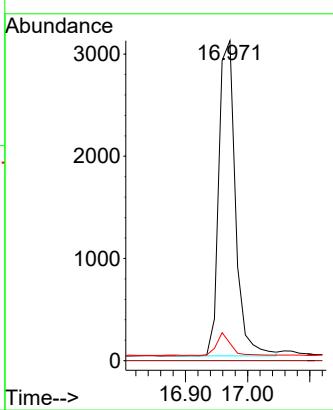

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.641 ng  
 RT: 15.368 min Scan# 1568  
 Delta R.T. 0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39



Tgt Ion:198 Resp: 1108  
 Ion Ratio Lower Upper  
 198 100  
 51 27.6 51.4 77.0#  
 105 25.4 45.5 68.3#



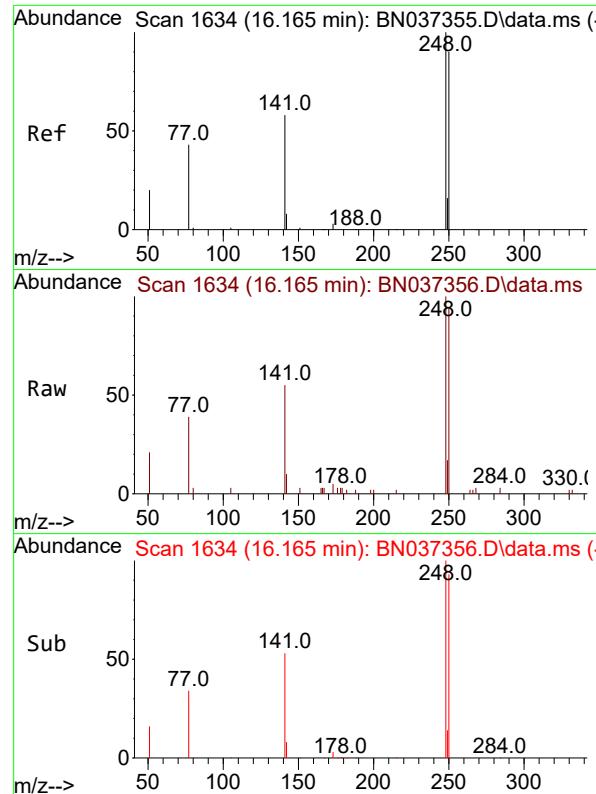


#21  
 4-Bromophenyl-phenylether  
 Concen: 0.697 ng  
 RT: 16.165 min Scan# 1  
 Delta R.T. 0.000 min BNA\_N  
 Lab File: BN037356.D ClientSampleId :  
 Acq: 20 Jun 2025 18:39 SSTDICCO.8


Tgt Ion:248 Resp: 3252  
 Ion Ratio Lower Upper  
 248 100  
 250 93.9 80.4 120.6  
 141 54.6 33.3 49.9#

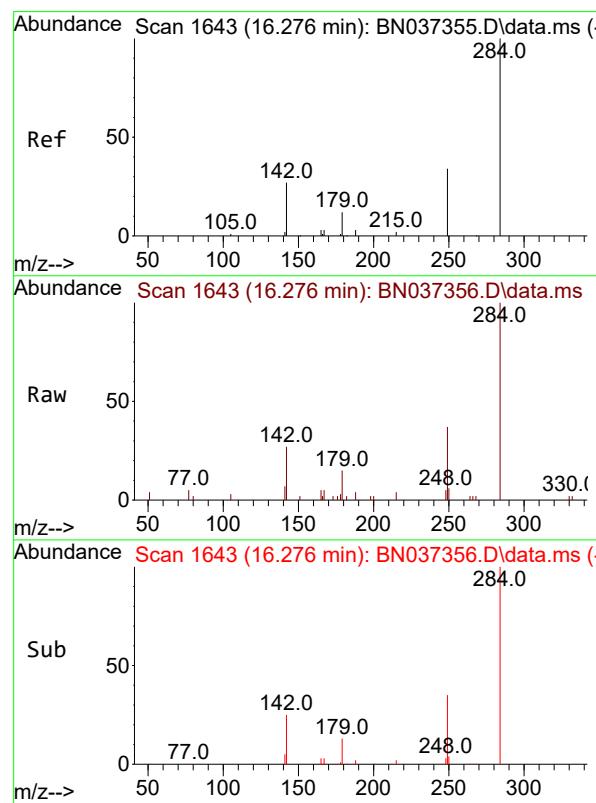

#22  
 Hexachlorobenzene  
 Concen: 0.713 ng  
 RT: 16.276 min Scan# 1643  
 Delta R.T. -0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39

Tgt Ion:284 Resp: 3471  
 Ion Ratio Lower Upper  
 284 100  
 142 33.9 27.0 40.6  
 249 34.1 28.8 43.2





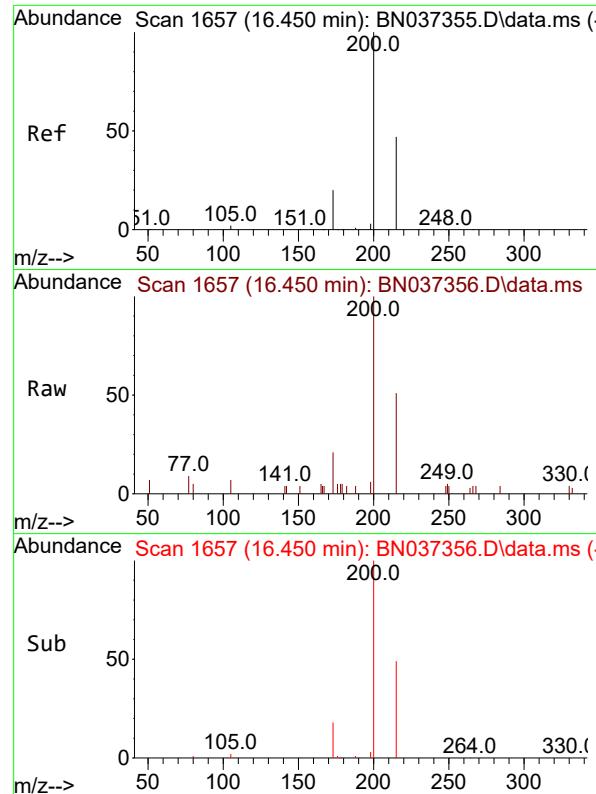

#23  
Atrazine  
Concen: 0.689 ng  
RT: 16.450 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8


Tgt Ion:200 Resp: 2516  
Ion Ratio Lower Upper  
200 100  
173 21.1 29.2 43.8#  
215 50.6 48.8 73.2

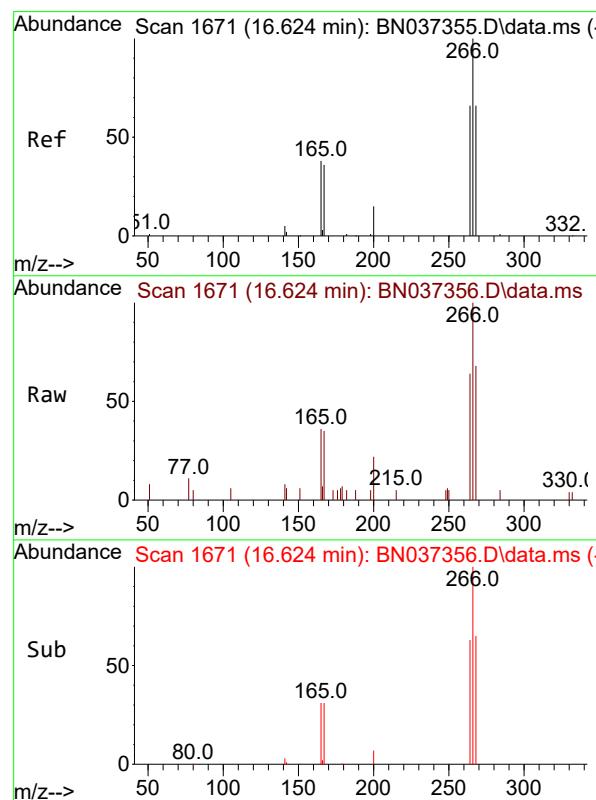

#24  
Pentachlorophenol  
Concen: 0.673 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39

Tgt Ion:266 Resp: 1797  
Ion Ratio Lower Upper  
266 100  
264 61.8 50.3 75.5  
268 63.2 55.3 82.9


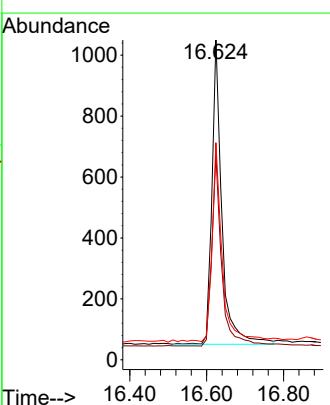


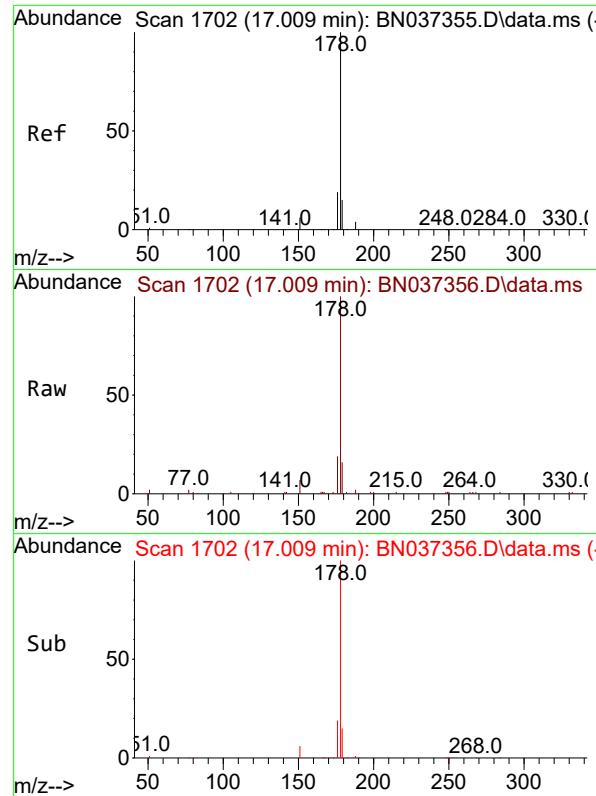

#25  
Phenanthrene  
Concen: 0.806 ng  
RT: 17.009 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8


Tgt Ion:178 Resp: 13016  
Ion Ratio Lower Upper  
178 100  
176 19.1 15.2 22.8  
179 15.2 12.9 19.3

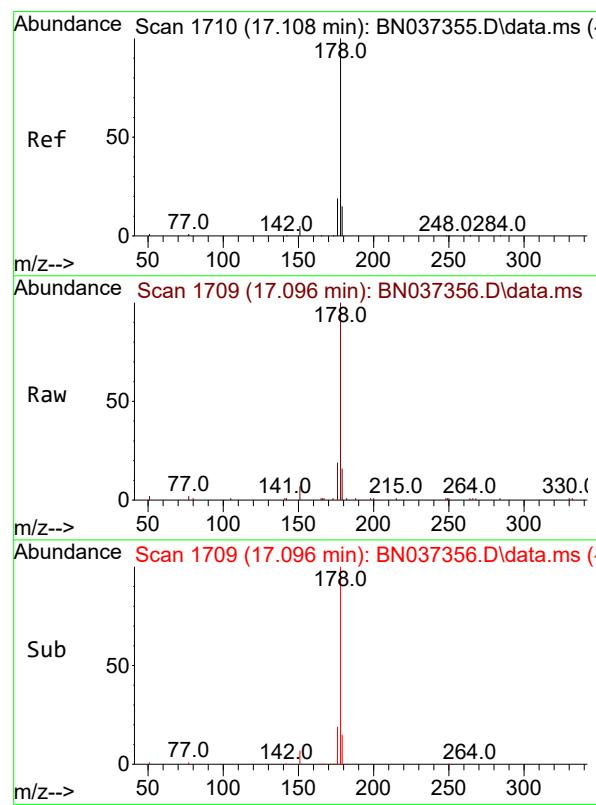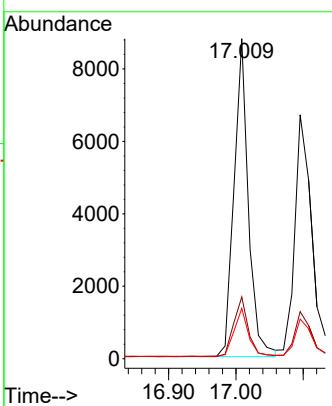

#26  
Anthracene  
Concen: 0.799 ng  
RT: 17.096 min Scan# 1709  
Delta R.T. -0.012 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39

Tgt Ion:178 Resp: 12050  
Ion Ratio Lower Upper  
178 100  
176 18.6 14.7 22.1  
179 15.6 13.0 19.6





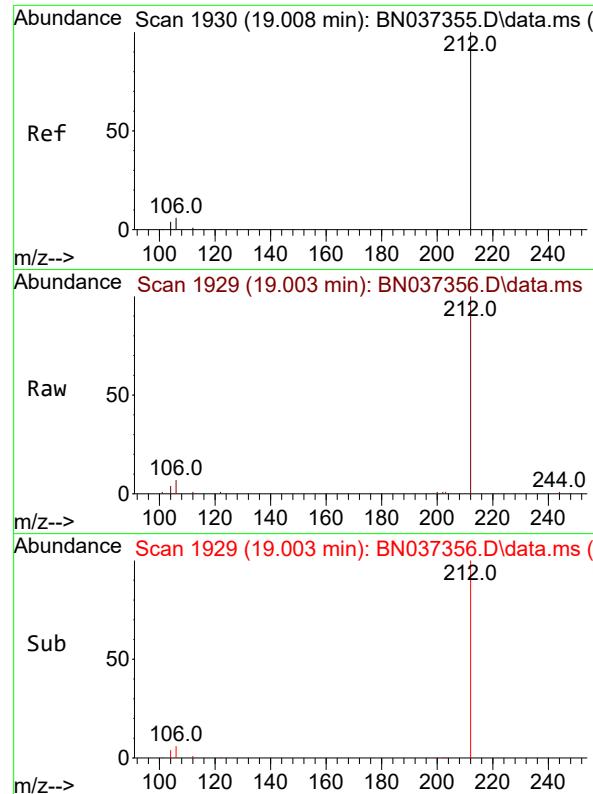

#27  
 Fluoranthene-d10  
 Concen: 0.749 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. -0.005 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:212 Resp: 13334  
 Ion Ratio Lower Upper  
 212 100  
 106 5.9 3.0 4.4#  
 104 3.6 2.0 3.0#

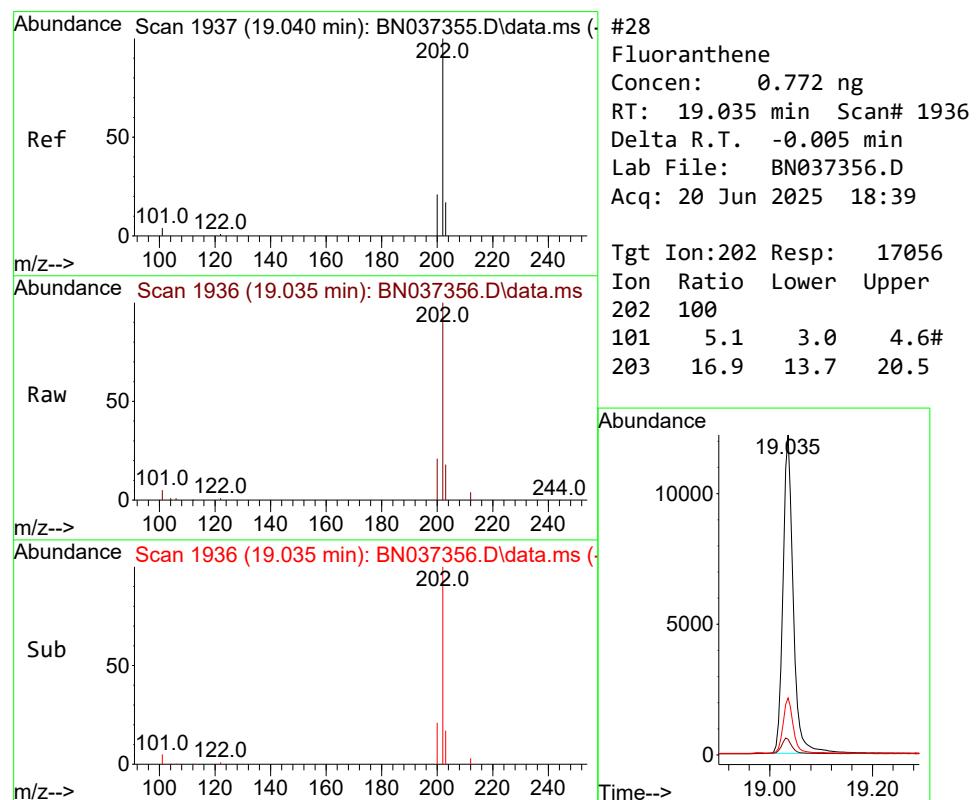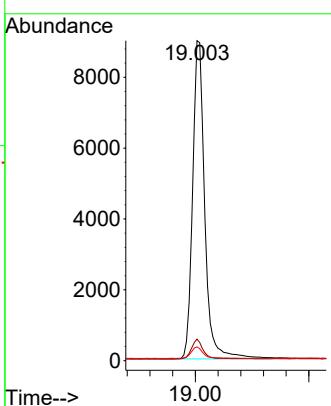

#28  
 Fluoranthene  
 Concen: 0.772 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39

Tgt Ion:202 Resp: 17056  
 Ion Ratio Lower Upper  
 202 100  
 101 5.1 3.0 4.6#  
 203 16.9 13.7 20.5


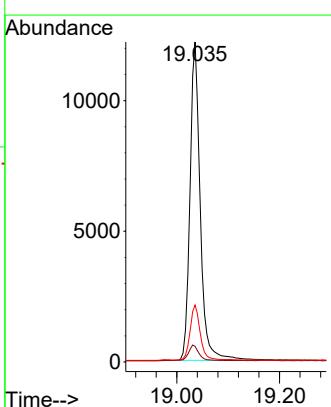


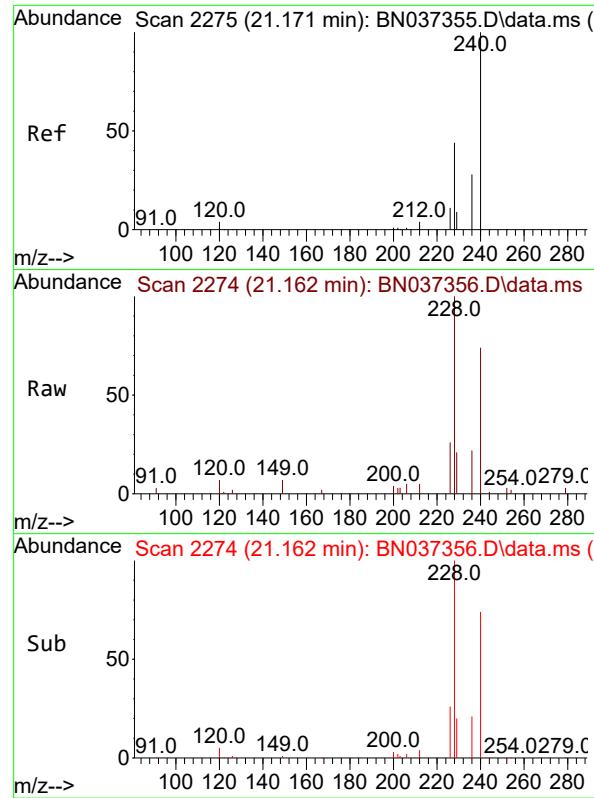

#29  
 Chrysene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 21.162 min Scan# 2  
 Delta R.T. -0.009 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:240 Resp: 5944  
 Ion Ratio Lower Upper  
 240 100  
 120 8.8 7.5 11.3  
 236 29.7 24.9 37.3

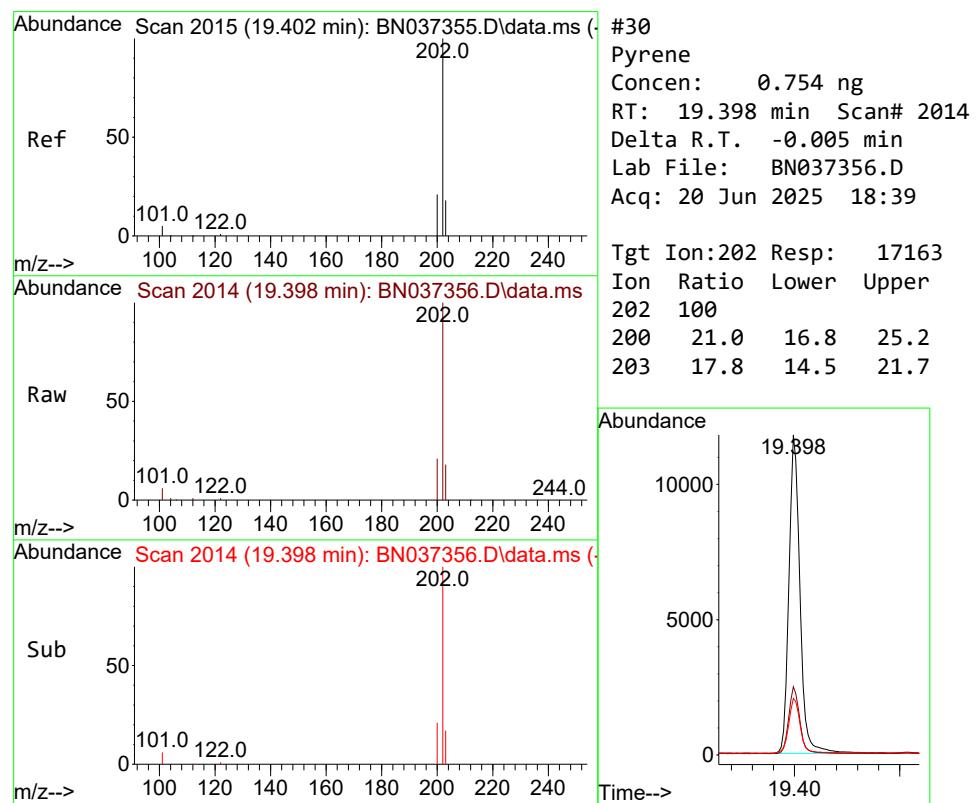

#30  
 Pyrene  
 Concen: 0.754 ng  
 RT: 19.398 min Scan# 2014  
 Delta R.T. -0.005 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39



Tgt Ion:202 Resp: 17163  
 Ion Ratio Lower Upper  
 202 100  
 200 21.0 16.8 25.2  
 203 17.8 14.5 21.7



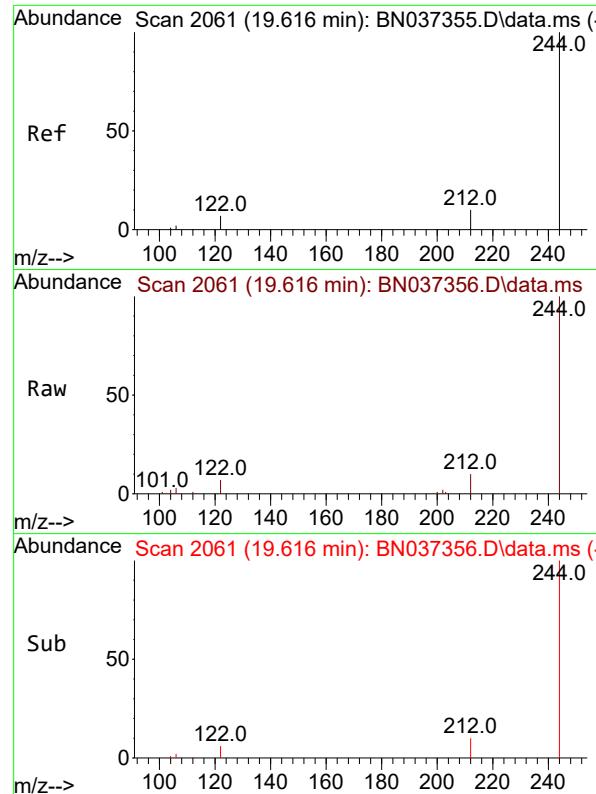


#31  
Terphenyl-d14  
Concen: 0.726 ng  
RT: 19.616 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39  
ClientSampleId : SSTDICCO.8


Tgt Ion:244 Resp: 9859  
Ion Ratio Lower Upper  
244 100  
212 10.4 11.1 16.7#  
122 6.9 7.2 10.8#

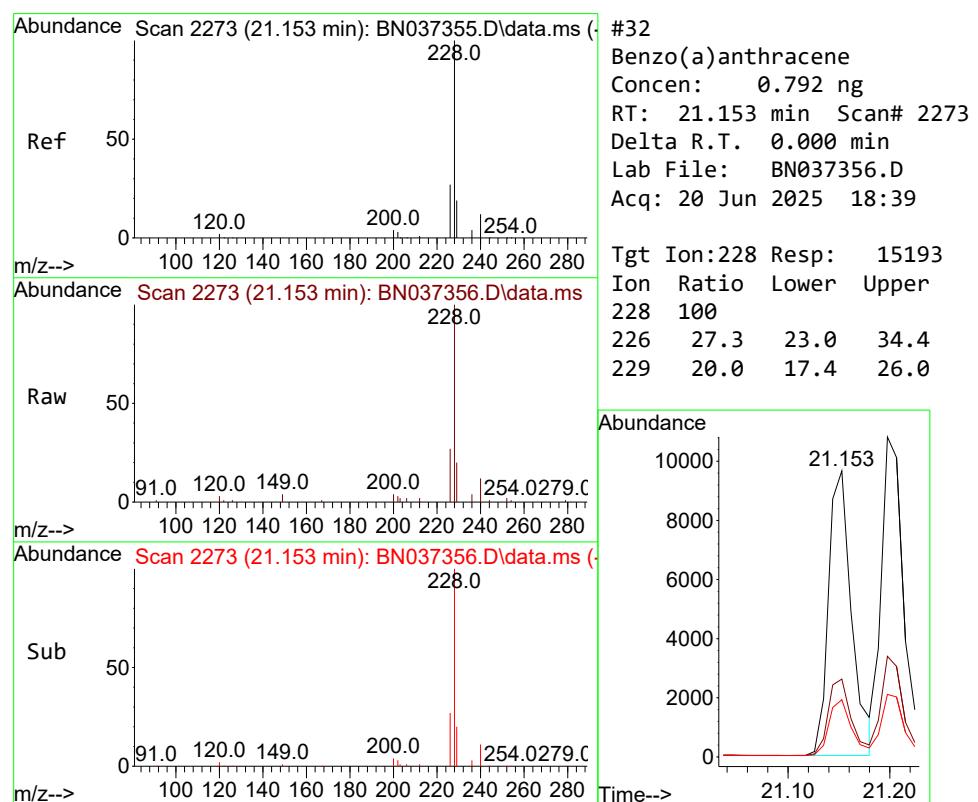

#32  
Benzo(a)anthracene  
Concen: 0.792 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39



Tgt Ion:228 Resp: 15193  
Ion Ratio Lower Upper  
228 100  
226 27.3 23.0 34.4  
229 20.0 17.4 26.0

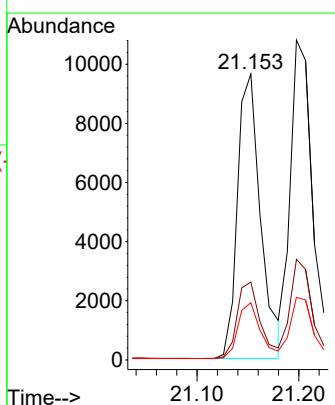

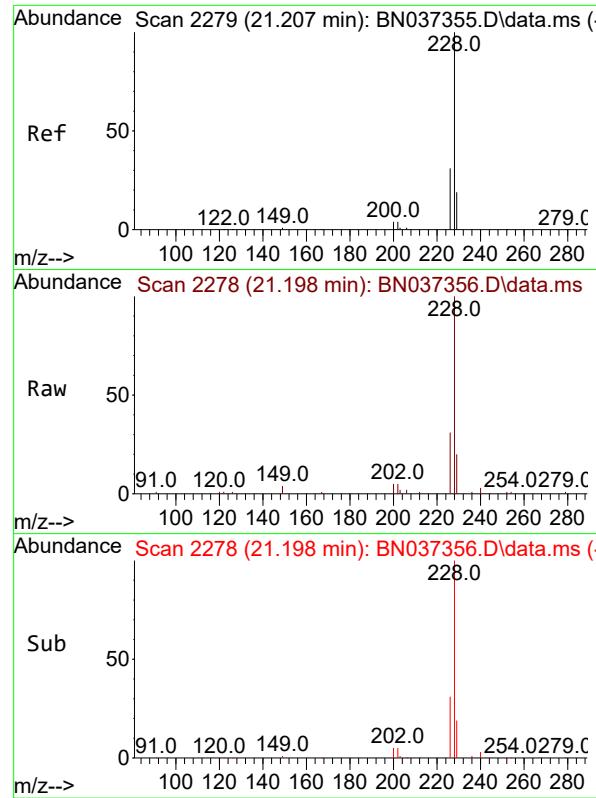


#33  
Chrysene  
Concen: 0.724 ng  
RT: 21.198 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.009 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39  
ClientSampleId : SSTDICCO.8


Tgt Ion:228 Resp: 17610  
Ion Ratio Lower Upper  
228 100  
226 31.4 25.4 38.2  
229 19.5 17.3 25.9

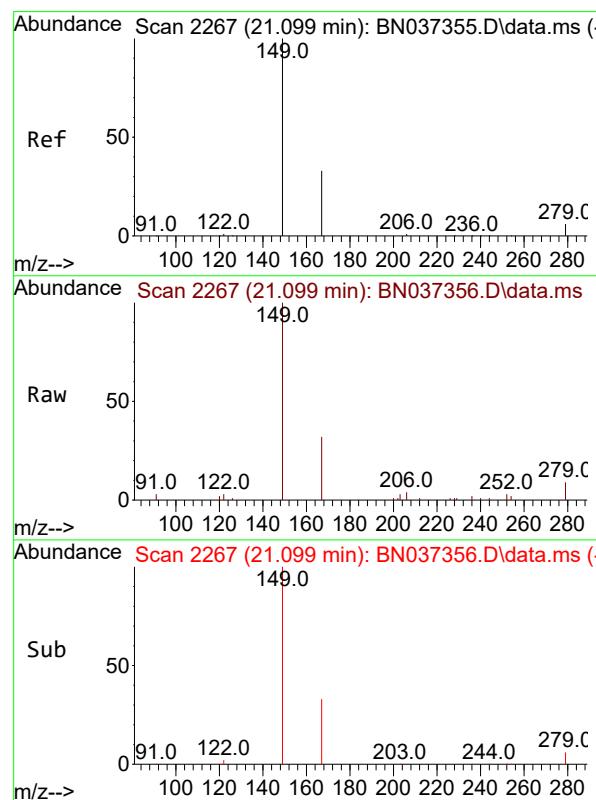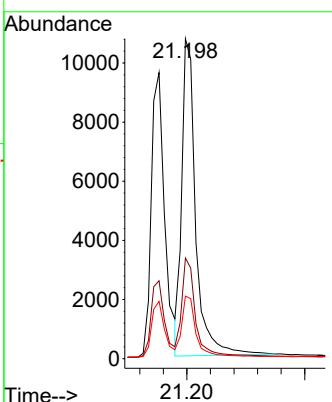

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.736 ng  
RT: 21.099 min Scan# 2267  
Delta R.T. 0.000 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39

Tgt Ion:149 Resp: 5787  
Ion Ratio Lower Upper  
149 100  
167 31.8 24.6 37.0  
279 6.2 6.5 9.7#





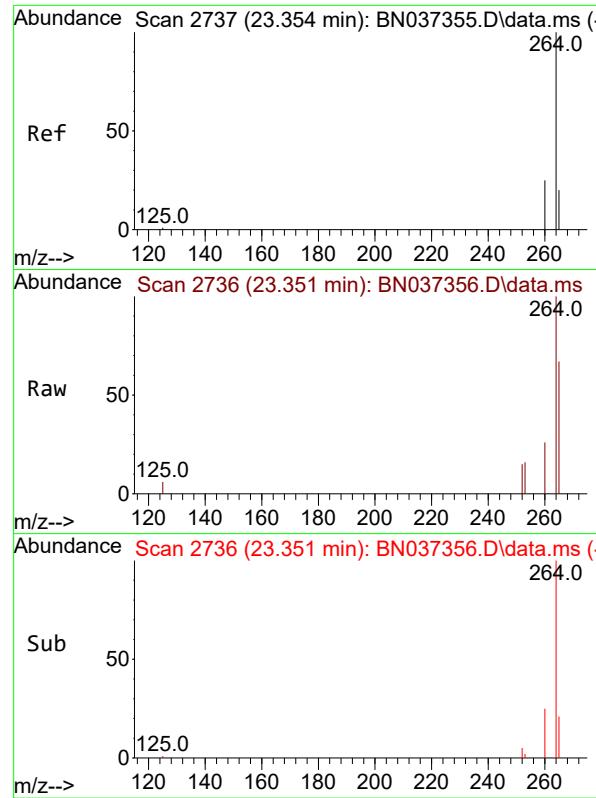

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.351 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:264 Resp: 6423  
 Ion Ratio Lower Upper  
 264 100  
 260 25.7 21.4 32.2  
 265 66.8 71.4 107.0#

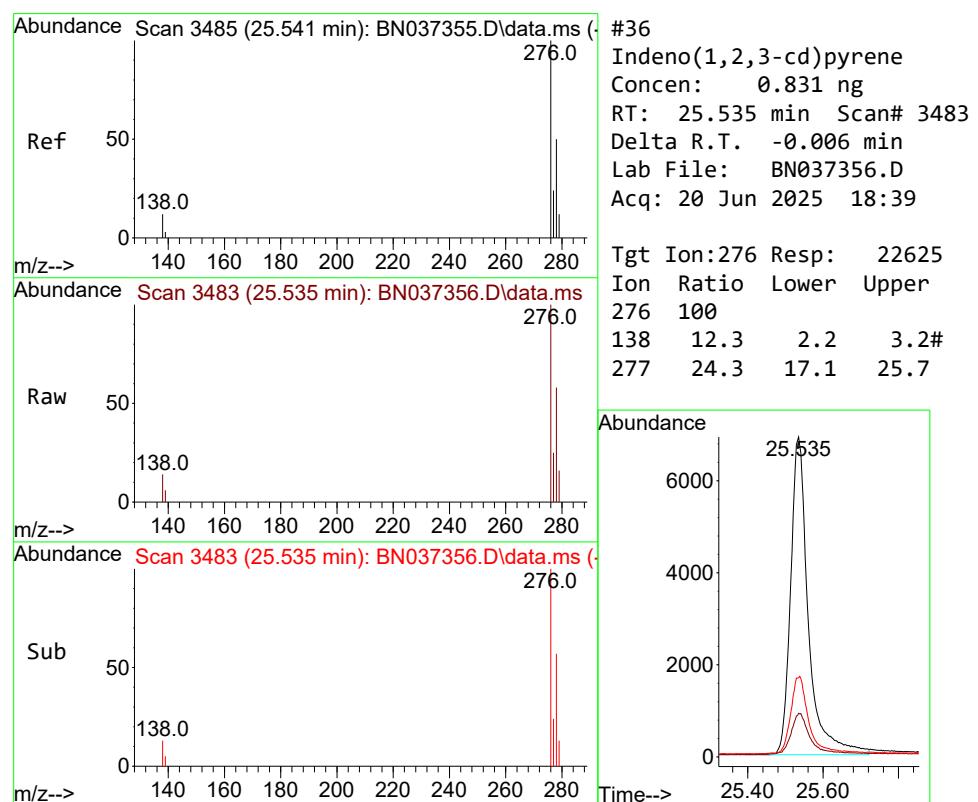

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.831 ng  
 RT: 25.535 min Scan# 3483  
 Delta R.T. -0.006 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39

Tgt Ion:276 Resp: 22625  
 Ion Ratio Lower Upper  
 276 100  
 138 12.3 2.2 3.2#  
 277 24.3 17.1 25.7



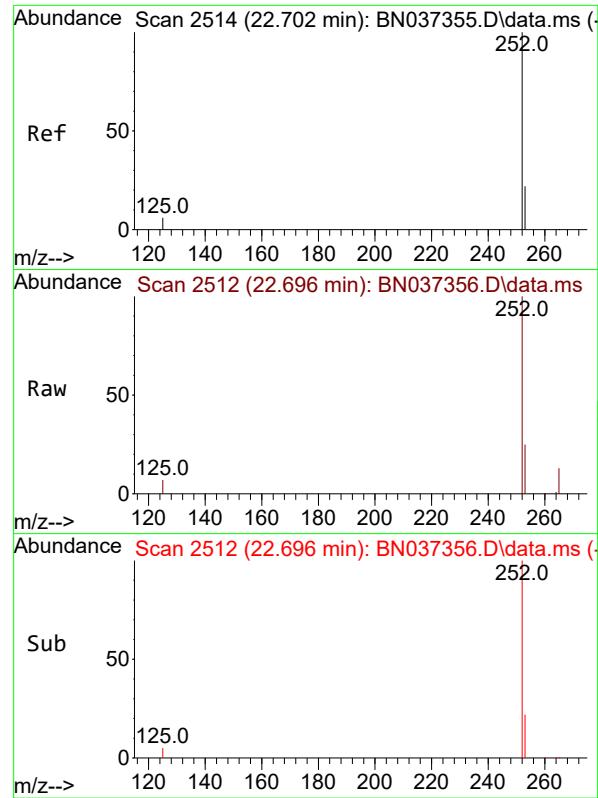

#37

Benzo(b)fluoranthene

Concen: 0.785 ng

RT: 22.696 min Scan# 2

Instrument :

BNA\_N

Delta R.T. -0.006 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39

ClientSampleId :

SSTDICC0.8


Tgt Ion:252 Resp: 17878

Ion Ratio Lower Upper

252 100

253 24.8 26.6 40.0#

125 6.7 6.1 9.1



#38

Benzo(k)fluoranthene

Concen: 0.761 ng

RT: 22.740 min Scan# 2527

Delta R.T. -0.006 min

Lab File: BN037356.D

Acq: 20 Jun 2025 18:39



Tgt Ion:252 Resp: 18833


Ion Ratio Lower Upper

252 100

253 24.4 26.7 40.1#

125 6.3 6.5 9.7#

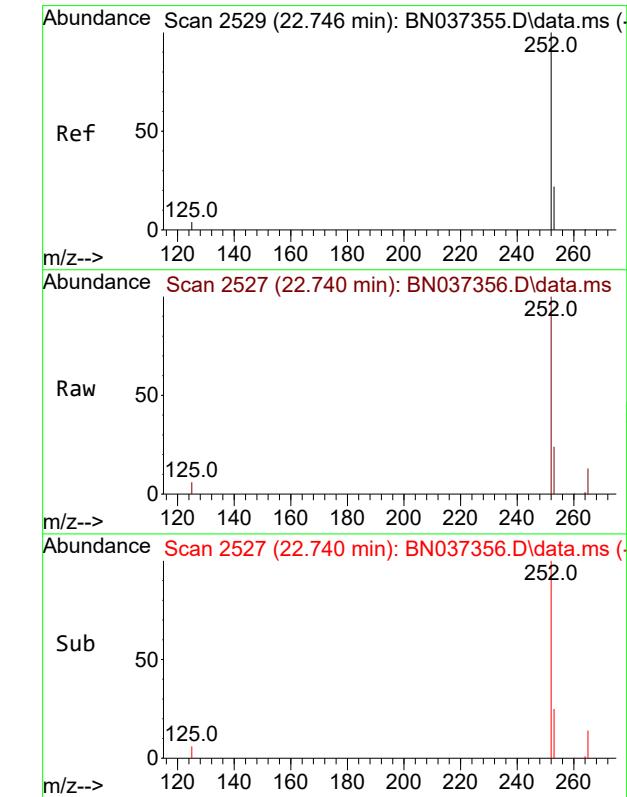



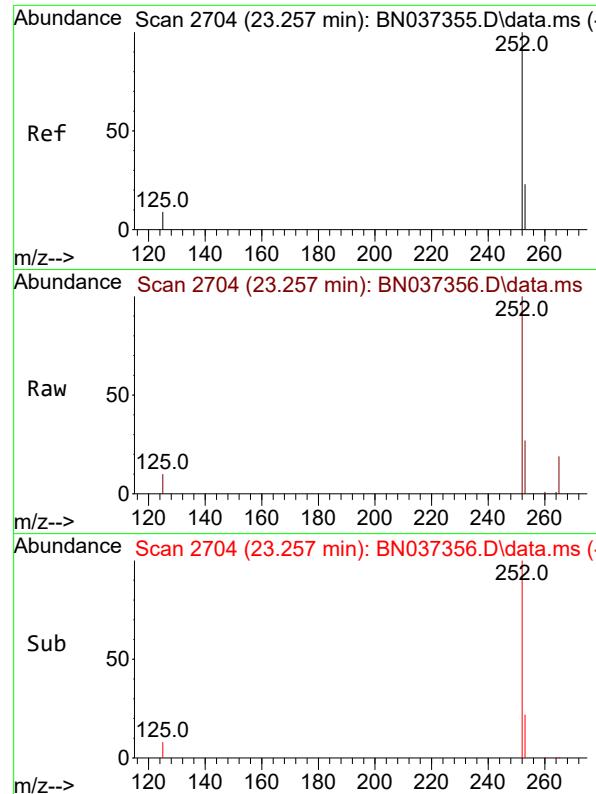

#39  
 Benzo(a)pyrene  
 Concen: 0.769 ng  
 RT: 23.257 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:252 Resp: 16022  
 Ion Ratio Lower Upper  
 252 100  
 253 27.1 31.6 47.4#  
 125 9.9 8.4 12.6

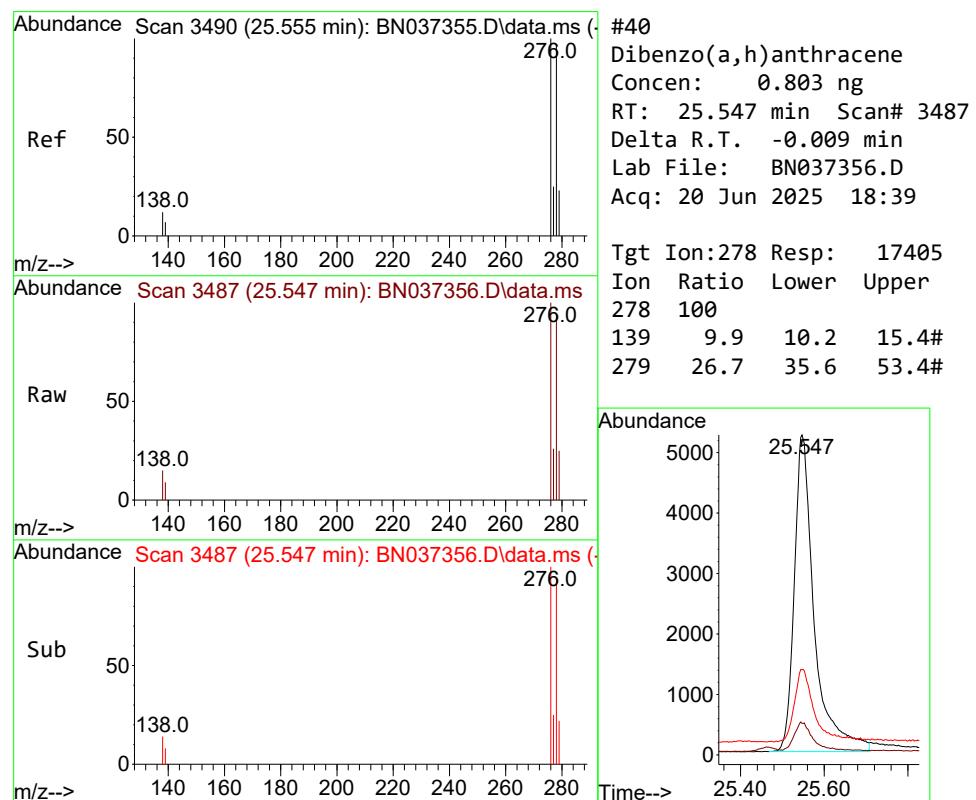

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.803 ng  
 RT: 25.547 min Scan# 3487  
 Delta R.T. -0.009 min  
 Lab File: BN037356.D  
 Acq: 20 Jun 2025 18:39

Tgt Ion:278 Resp: 17405  
 Ion Ratio Lower Upper  
 278 100  
 139 9.9 10.2 15.4#  
 279 26.7 35.6 53.4#

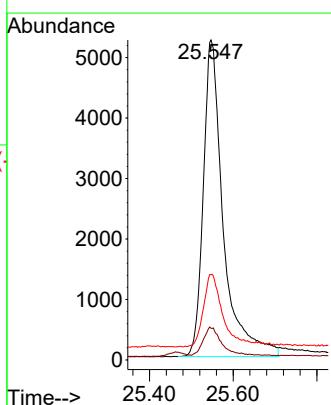


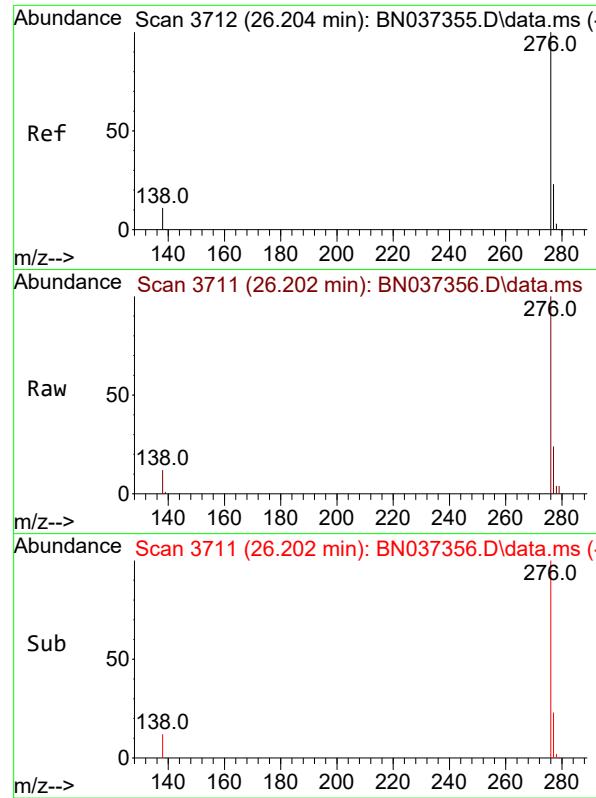

#41  
Benzo(g,h,i)perylene  
Concen: 0.801 ng  
RT: 26.202 min Scan# 3  
Delta R.T. -0.003 min  
Lab File: BN037356.D  
Acq: 20 Jun 2025 18:39

Instrument :  
BNA\_N  
ClientSampleId :  
SSTDICC0.8

Tgt Ion:276 Resp: 20041  
Ion Ratio Lower Upper  
276 100  
277 24.4 22.7 34.1  
138 12.5 9.4 14.2

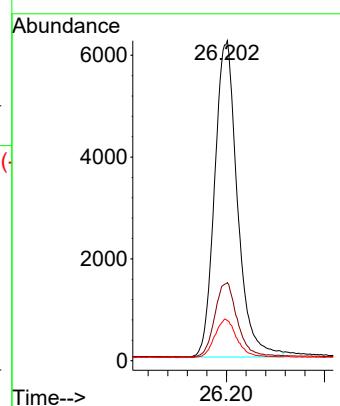

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037357.D  
 Acq On : 20 Jun 2025 19:15  
 Operator : RC/JU  
 Sample : SSTDICC1.6  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC1.6

Quant Time: Jun 20 23:27:39 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2270	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4835	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	3136	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	6455	0.400	ng	-0.01
29) Chrysene-d12	21.162	240	6604	0.400	ng	0.00
35) Perylene-d12	23.351	264	7013	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	7577	1.826	ng	0.00
5) Phenol-d6	6.744	99	8087	1.969	ng	0.00
8) Nitrobenzene-d5	8.717	82	7020	1.749	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	12882	1.647	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	3170	1.413	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	23802	1.730	ng	0.00
27) Fluoranthene-d10	19.003	212	31876	1.586	ng	0.00
31) Terphenyl-d14	19.612	244	24025	1.593	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	3788	1.889	ng	92
3) n-Nitrosodimethylamine	3.415	42	3553	1.522	ng	# 73
6) bis(2-Chloroethyl)ether	6.997	93	7504	2.088	ng	96
9) Naphthalene	10.394	128	21372	1.705	ng	# 86
10) Hexachlorobutadiene	10.682	225	8200	1.339	ng	# 99
12) 2-Methylnaphthalene	12.016	142	15021	1.704	ng	# 92
16) Acenaphthylene	13.935	152	22546	1.713	ng	98
17) Acenaphthene	14.277	154	14727	1.688	ng	99
18) Fluorene	15.272	166	20827	1.684	ng	100
20) 4,6-Dinitro-2-methylph...	15.357	198	2836	1.453	ng	# 49
21) 4-Bromophenyl-phenylether	16.165	248	7869	1.493	ng	# 91
22) Hexachlorobenzene	16.276	284	8354	1.519	ng	97
23) Atrazine	16.438	200	6166	1.495	ng	# 83
24) Pentachlorophenol	16.624	266	4361	1.445	ng	96
25) Phenanthrene	17.009	178	32059	1.758	ng	99
26) Anthracene	17.096	178	29693	1.743	ng	99
28) Fluoranthene	19.035	202	41430	1.660	ng	# 99
30) Pyrene	19.398	202	41513	1.642	ng	100
32) Benzo(a)anthracene	21.153	228	37793	1.773	ng	97
33) Chrysene	21.207	228	41889	1.550	ng	96
34) Bis(2-ethylhexyl)phtha...	21.099	149	13738	1.573	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.535	276	55371	1.863	ng	# 91
37) Benzo(b)fluoranthene	22.699	252	43215	1.738	ng	# 85
38) Benzo(k)fluoranthene	22.740	252	46879	1.736	ng	# 85
39) Benzo(a)pyrene	23.255	252	39242	1.724	ng	# 78
40) Dibenzo(a,h)anthracene	25.547	278	43786	1.849	ng	# 74
41) Benzo(g,h,i)perylene	26.199	276	48259	1.767	ng	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037357.D  
 Acq On : 20 Jun 2025 19:15  
 Operator : RC/JU  
 Sample : SSTDICC1.6  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC1.6


Quant Time: Jun 20 23:27:39 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration

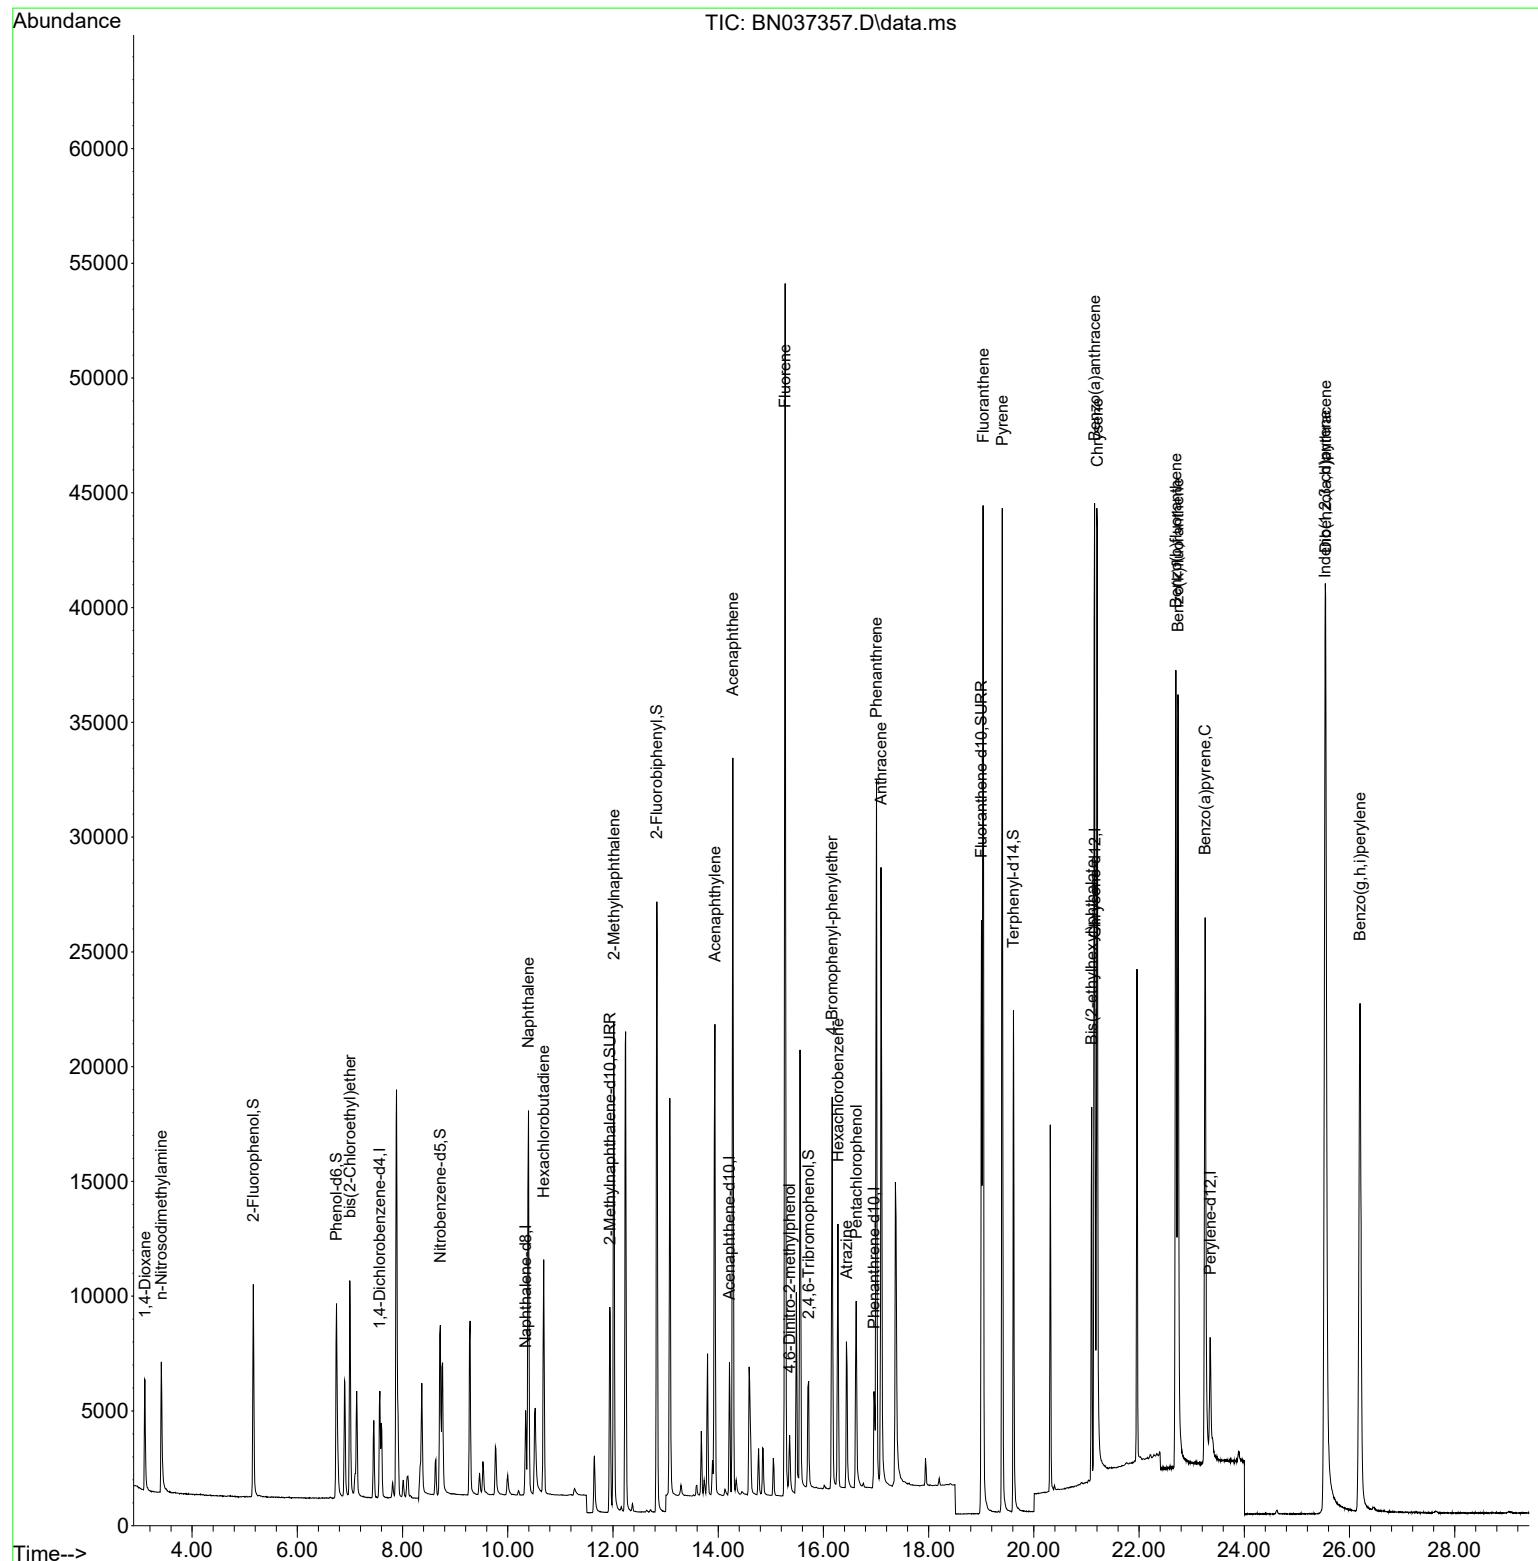






#1  
 1,4-Dichlorobenzene-d4  
 Concen: 0.400 ng  
 RT: 7.568 min Scan# 6  
 Delta R.T. -0.000 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6





Tgt Ion:152 Resp: 2270  
 Ion Ratio Lower Upper  
 152 100  
 150 152.7 112.7 169.1  
 115 52.5 45.9 68.9

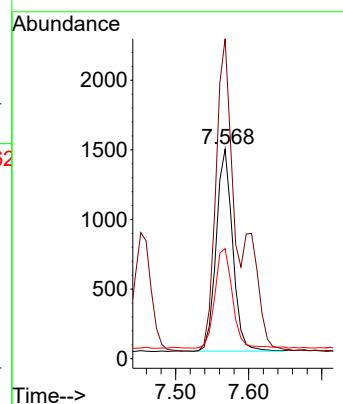






#2  
 1,4-Dioxane  
 Concen: 1.889 ng  
 RT: 3.104 min Scan# 31  
 Delta R.T. -0.000 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15



Tgt Ion: 88 Resp: 3788  
 Ion Ratio Lower Upper  
 88 100  
 43 22.8 21.0 31.6  
 58 53.7 38.0 57.0

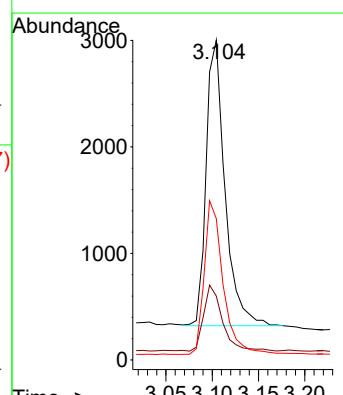



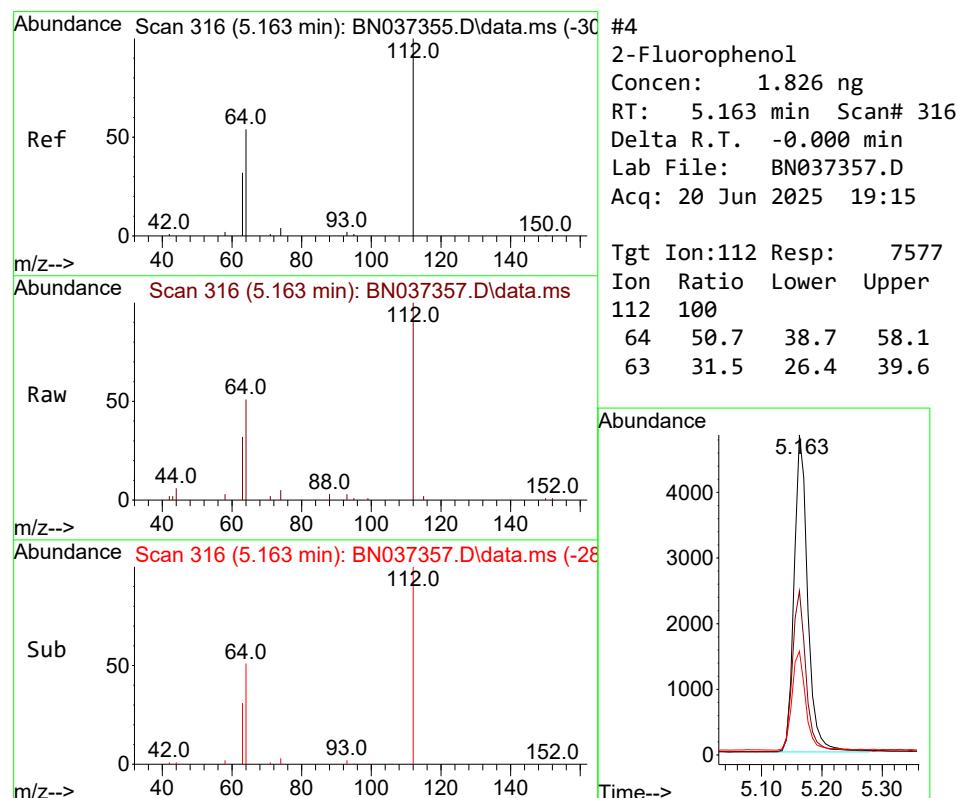
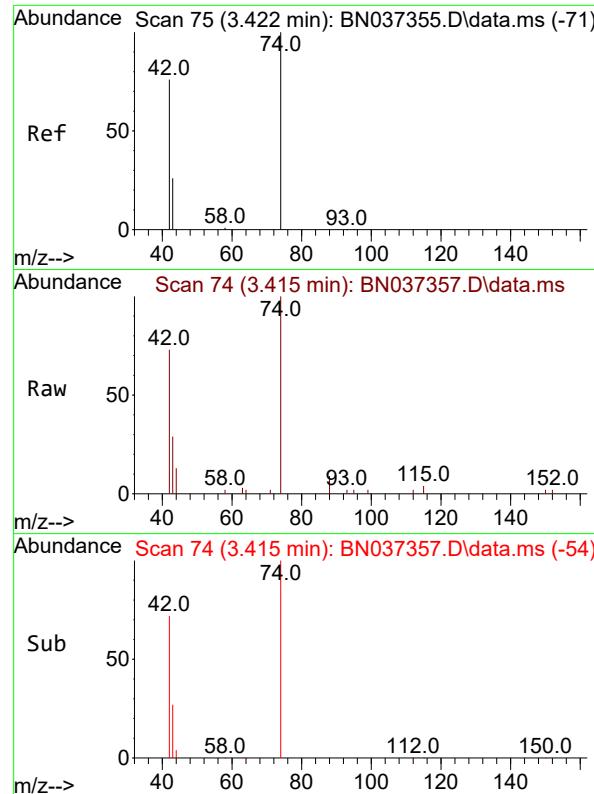


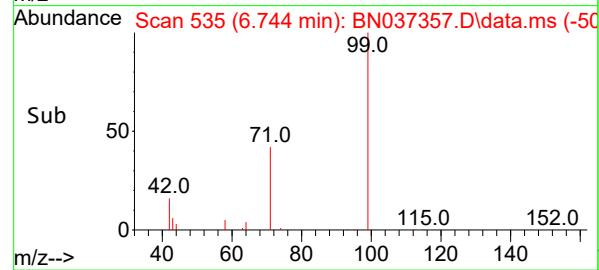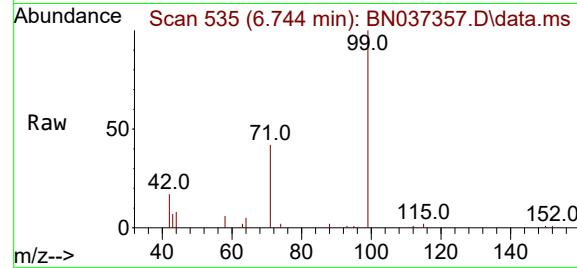

#5  
 Phenol-d6  
 Concen: 1.969 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. -0.007 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion: 99 Resp: 8087  
 Ion Ratio Lower Upper  
 99 100  
 42 18.1 19.8 29.8#  
 71 44.2 42.6 64.0

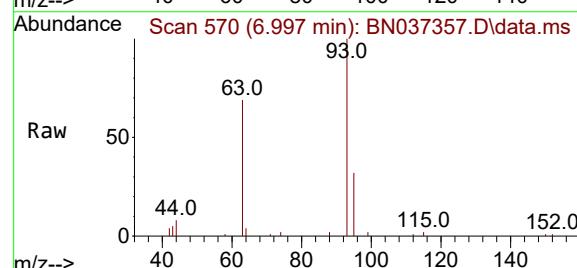

#6  
 bis(2-Chloroethyl)ether  
 Concen: 2.088 ng  
 RT: 6.997 min Scan# 570  
 Delta R.T. -0.007 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Tgt Ion: 93 Resp: 7504  
 Ion Ratio Lower Upper  
 93 100  
 63 64.1 53.2 79.8  
 95 31.5 27.3 40.9








#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6





Tgt Ion:136 Resp: 4835  
 Ion Ratio Lower Upper  
 136 100  
 137 12.3 12.2 18.2  
 54 7.0 8.8 13.2#  
 68 5.8 7.0 10.4#






#8  
 Nitrobenzene-d5  
 Concen: 1.749 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. -0.000 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15



Tgt Ion: 82 Resp: 7020  
 Ion Ratio Lower Upper  
 82 100  
 128 43.6 42.5 63.7  
 54 38.7 43.2 64.8#





#9

Naphthalene

Concen: 1.705 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037357.D

Acq: 20 Jun 2025 19:15

Instrument :

BNA\_N

ClientSampleId :

SSTDICC1.6

Tgt Ion:128 Resp: 21372





Ion Ratio Lower Upper

128 100

129 11.3 14.0 21.0#

127 13.6 15.8 23.8#

Abundance

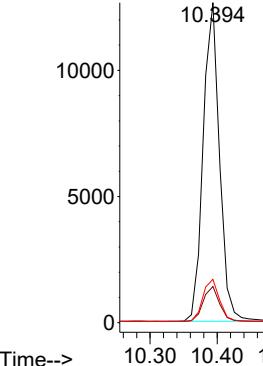

#10

Hexachlorobutadiene

Concen: 1.339 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037357.D

Acq: 20 Jun 2025 19:15

Tgt Ion:225 Resp: 8200


Ion Ratio Lower Upper


225 100

223 0.0 0.0 0.0

227 63.5 50.3 75.5



Abundance

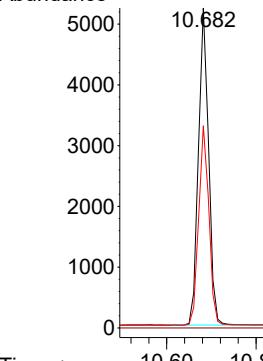

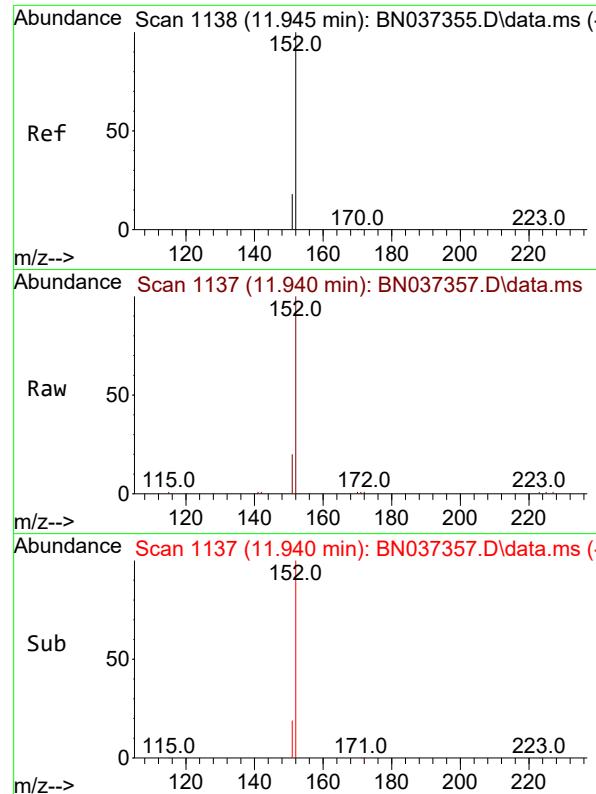


#11  
2-Methylnaphthalene-d10  
Concen: 1.647 ng  
RT: 11.940 min Scan# 1:Instrument :  
Delta R.T. -0.005 min BNA\_N  
Lab File: BN037357.D ClientSampleId :  
Acq: 20 Jun 2025 19:15 SSTDICC1.6


Tgt Ion:152 Resp: 12882  
Ion Ratio Lower Upper  
152 100  
151 21.8 17.4 26.0

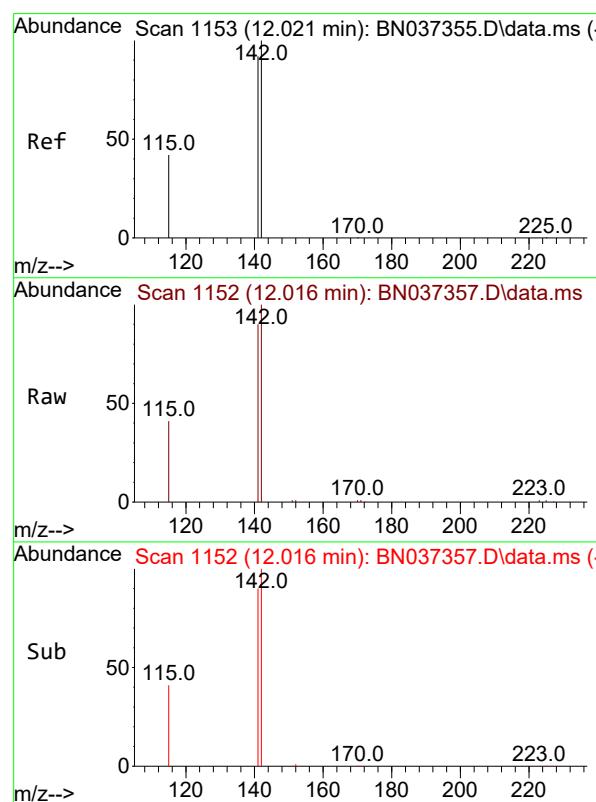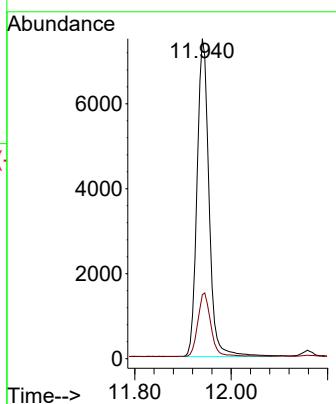

#12  
2-Methylnaphthalene  
Concen: 1.704 ng  
RT: 12.016 min Scan# 1152  
Delta R.T. -0.005 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15

Tgt Ion:142 Resp: 15021  
Ion Ratio Lower Upper  
142 100  
141 89.5 70.2 105.2  
115 41.2 43.0 64.4#


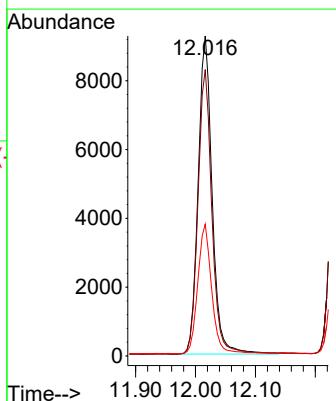


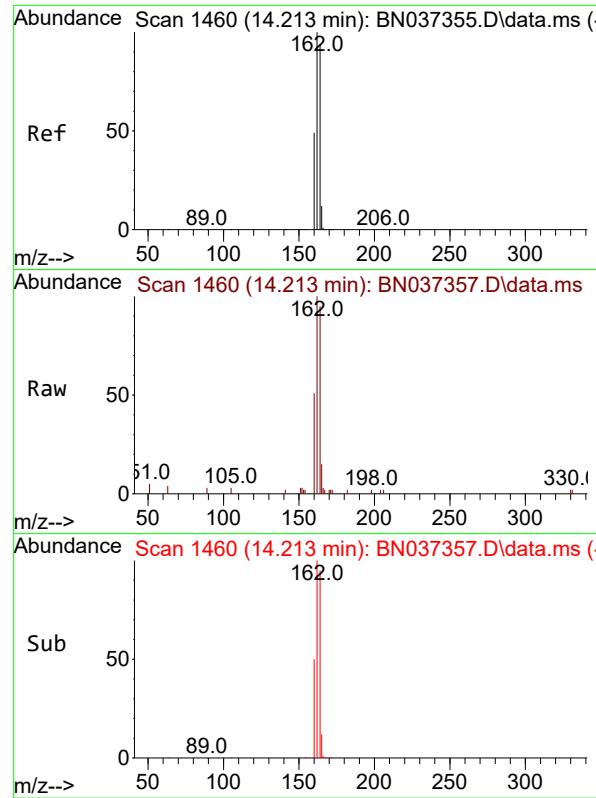

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6


Tgt Ion:164 Resp: 3136  
Ion Ratio Lower Upper  
164 100  
162 105.0 81.5 122.3  
160 53.1 43.0 64.4

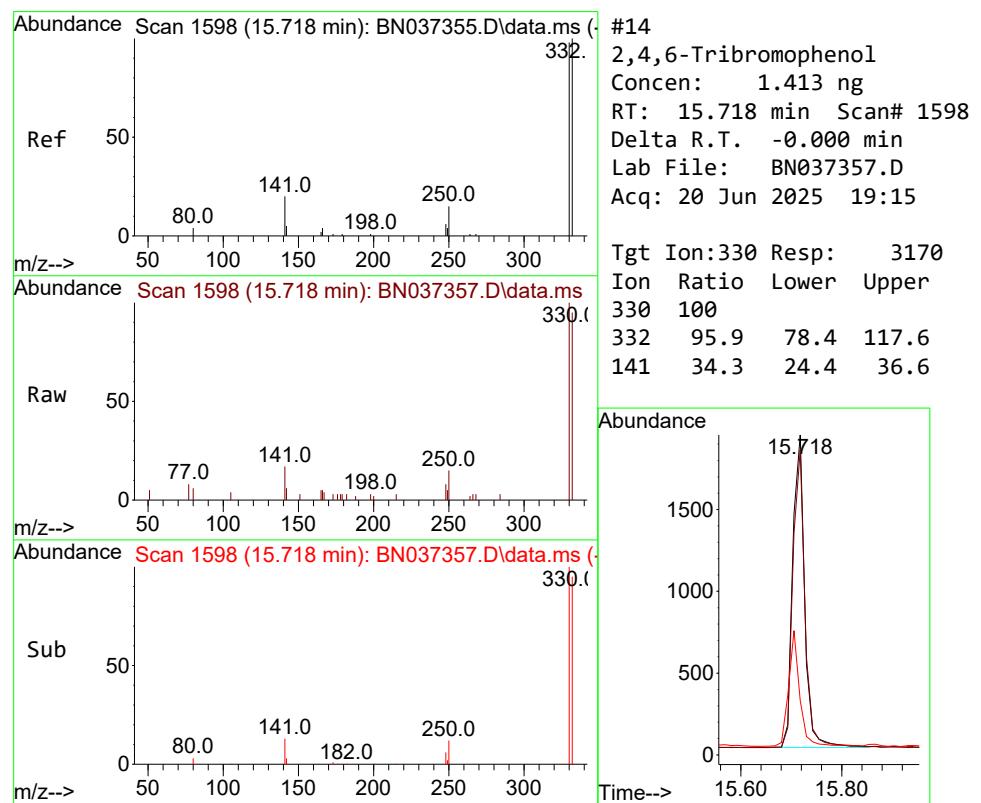

#14  
2,4,6-Tribromophenol  
Concen: 1.413 ng  
RT: 15.718 min Scan# 1598  
Delta R.T. -0.000 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15



Tgt Ion:330 Resp: 3170  
Ion Ratio Lower Upper  
330 100  
332 95.9 78.4 117.6  
141 34.3 24.4 36.6



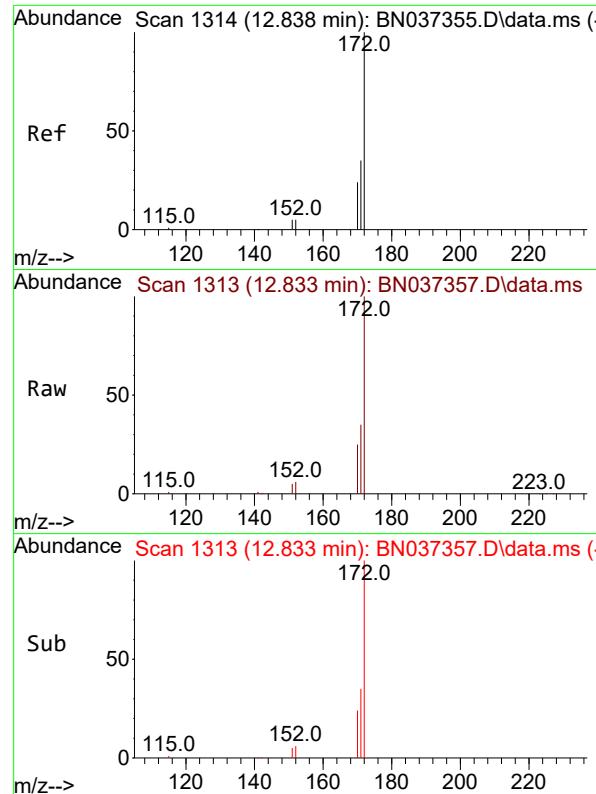


#15  
2-Fluorobiphenyl  
Concen: 1.730 ng  
RT: 12.833 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. -0.005 min  
Lab File: BN037357.D  
ClientSampleId : SSTDICC1.6  
Acq: 20 Jun 2025 19:15




Tgt Ion:172 Resp: 23802  
Ion Ratio Lower Upper  
172 100  
171 35.5 30.8 46.2  
170 24.7 21.9 32.9

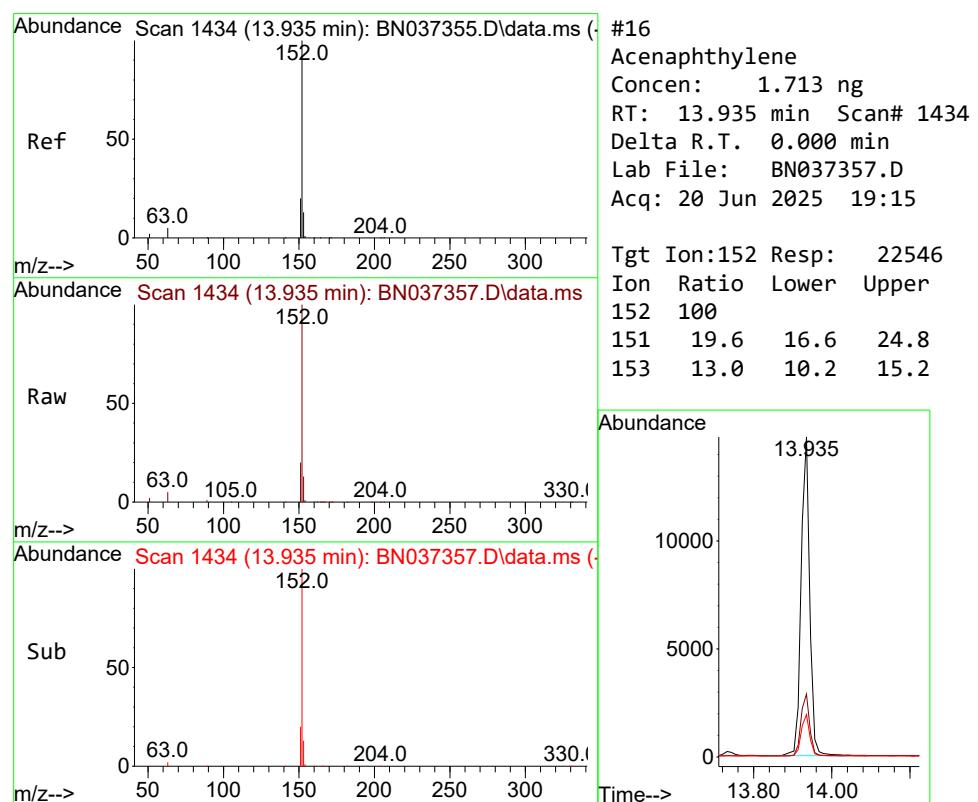

#16  
Acenaphthylene  
Concen: 1.713 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15

Tgt Ion:152 Resp: 22546  
Ion Ratio Lower Upper  
152 100  
151 19.6 16.6 24.8  
153 13.0 10.2 15.2

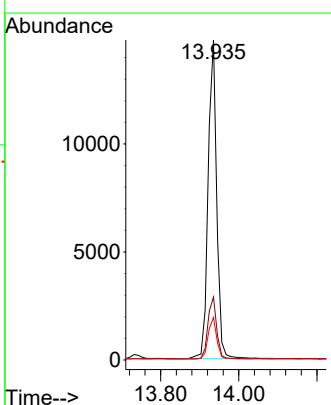

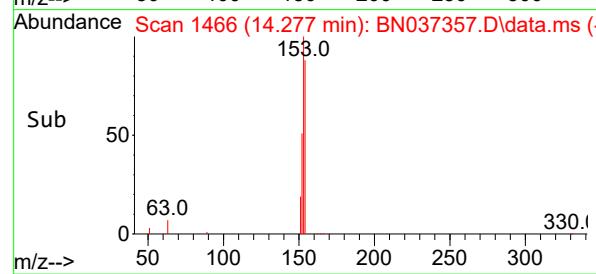

#17

Acenaphthene

Concen: 1.688 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037357.D

Acq: 20 Jun 2025 19:15

Instrument :

BNA\_N

ClientSampleId :

SSTDICC1.6

Tgt Ion:154 Resp: 14727

Ion Ratio Lower Upper

154 100




153 115.0 93.1 139.7

152 60.4 48.6 73.0

Abundance

14.277

Time--&gt;

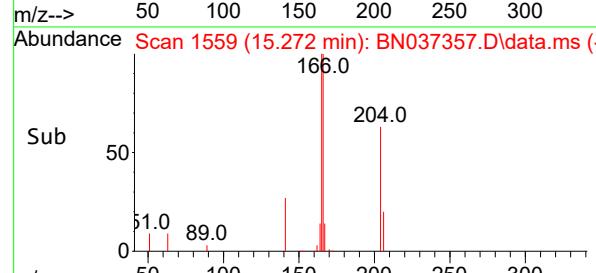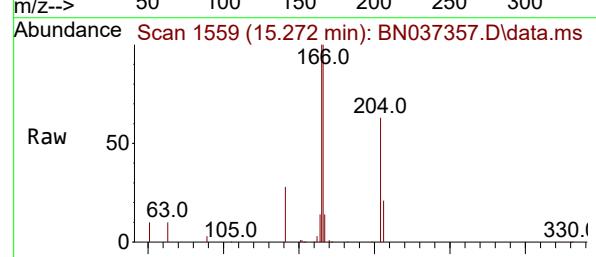

#18

Fluorene

Concen: 1.684 ng

RT: 15.272 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037357.D

Acq: 20 Jun 2025 19:15

Tgt Ion:166 Resp: 20827

Ion Ratio Lower Upper

166 100


165 99.5 79.5 119.3

167 13.8 10.7 16.1

Abundance

15.272



Time--&gt;

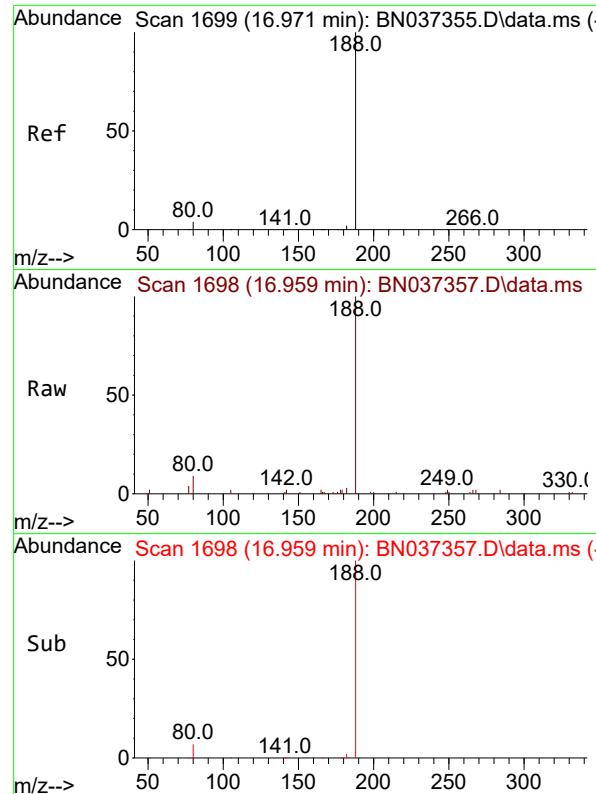

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.959 min Scan# 1  
 Delta R.T. -0.012 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:188 Resp: 6455  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 8.6 6.2 9.2

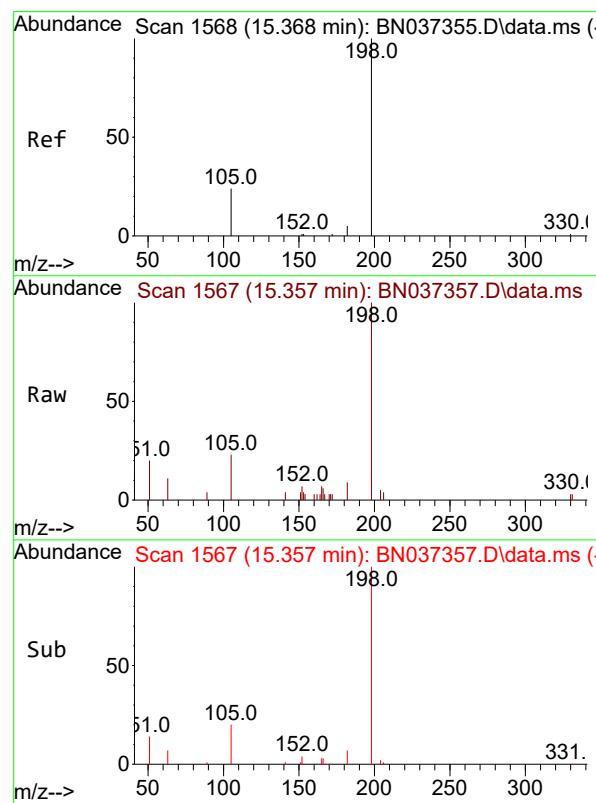

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 1.453 ng  
 RT: 15.357 min Scan# 1567  
 Delta R.T. -0.011 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Tgt Ion:198 Resp: 2836  
 Ion Ratio Lower Upper  
 198 100  
 51 19.9 51.4 77.0#  
 105 23.3 45.5 68.3#





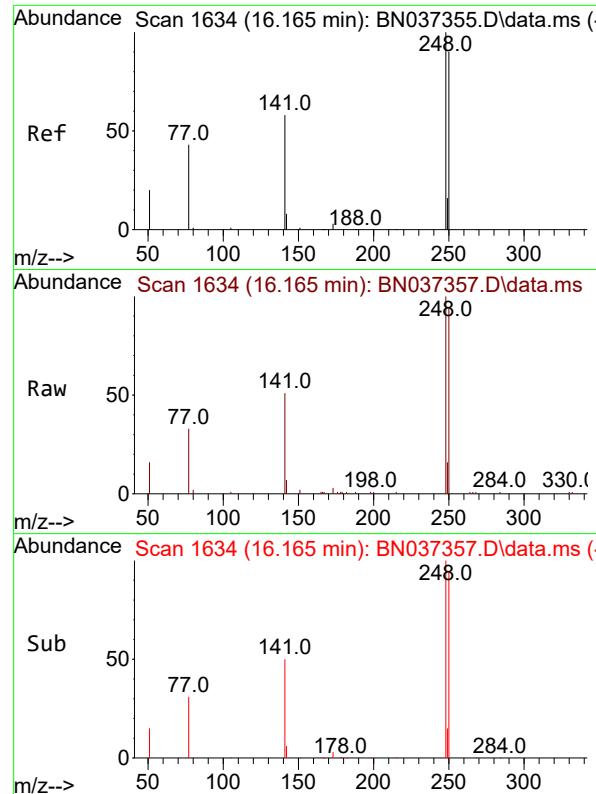

#21  
 4-Bromophenyl-phenylether  
 Concen: 1.493 ng  
 RT: 16.165 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:248 Resp: 7869  
 Ion Ratio Lower Upper  
 248 100  
 250 94.1 80.4 120.6  
 141 50.7 33.3 49.9#

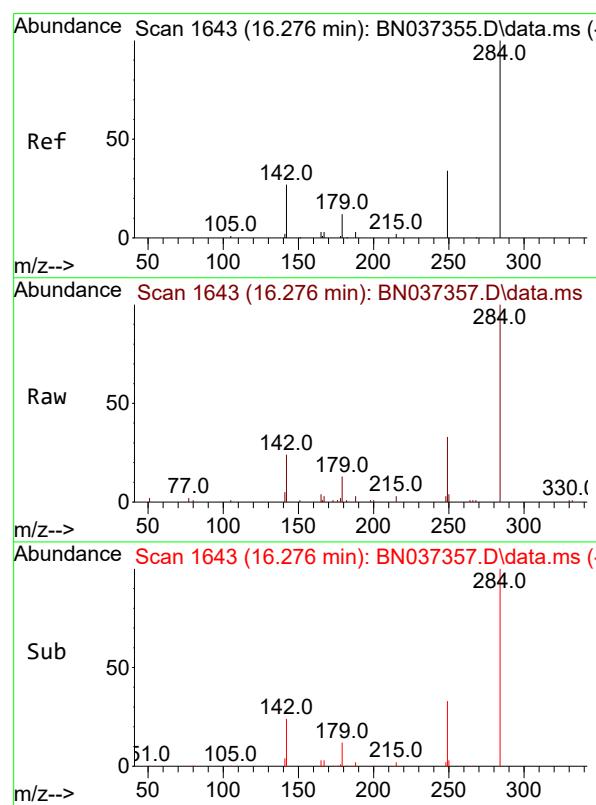

#22  
 Hexachlorobenzene  
 Concen: 1.519 ng  
 RT: 16.276 min Scan# 1643  
 Delta R.T. -0.000 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Tgt Ion:284 Resp: 8354  
 Ion Ratio Lower Upper  
 284 100  
 142 33.8 27.0 40.6  
 249 32.9 28.8 43.2


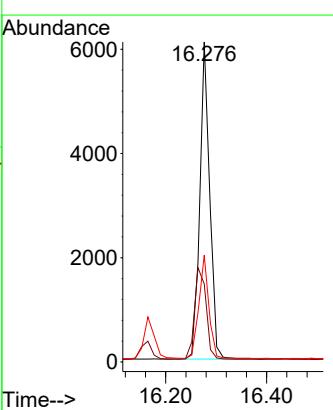


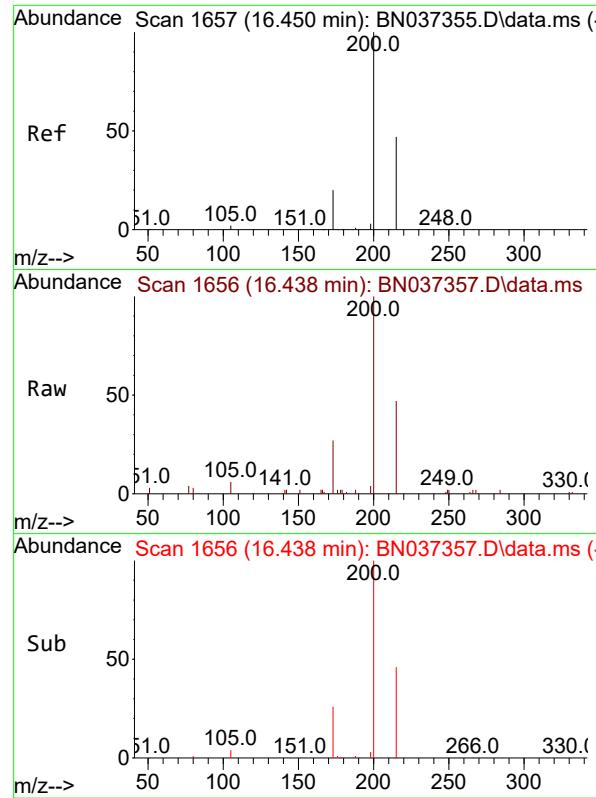

#23  
Atrazine  
Concen: 1.495 ng  
RT: 16.438 min Scan# 1  
Delta R.T. -0.012 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6


Tgt Ion:200 Resp: 6166  
Ion Ratio Lower Upper  
200 100  
173 26.9 29.2 43.8#  
215 47.2 48.8 73.2#

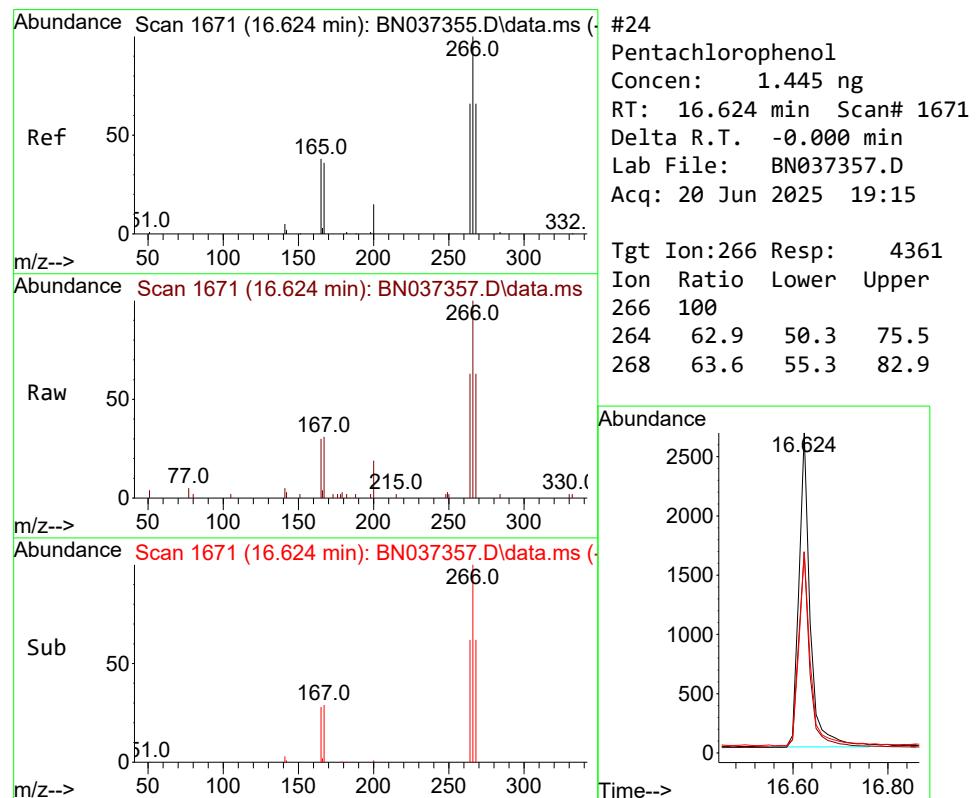

#24  
Pentachlorophenol  
Concen: 1.445 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15

Tgt Ion:266 Resp: 4361  
Ion Ratio Lower Upper  
266 100  
264 62.9 50.3 75.5  
268 63.6 55.3 82.9





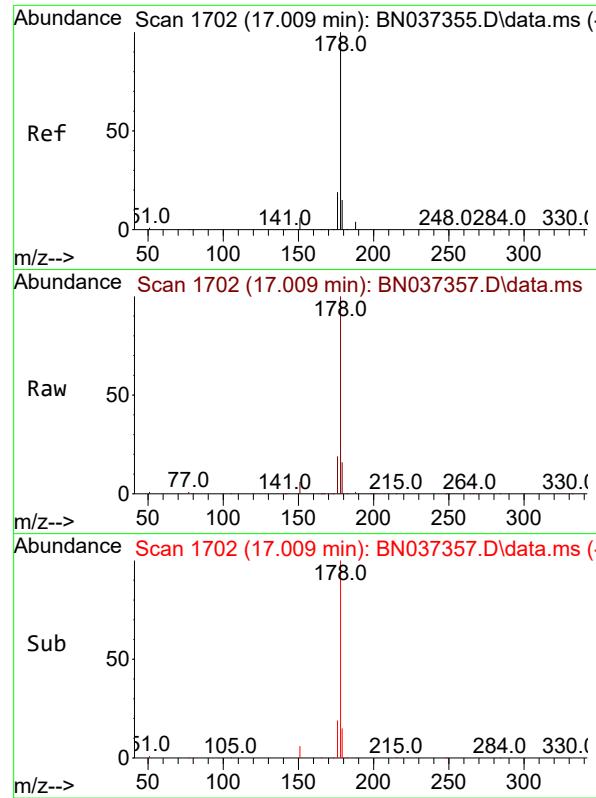

#25  
 Phenanthrene  
 Concen: 1.758 ng  
 RT: 17.009 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:178 Resp: 32059  
 Ion Ratio Lower Upper  
 178 100  
 176 19.2 15.2 22.8  
 179 15.4 12.9 19.3

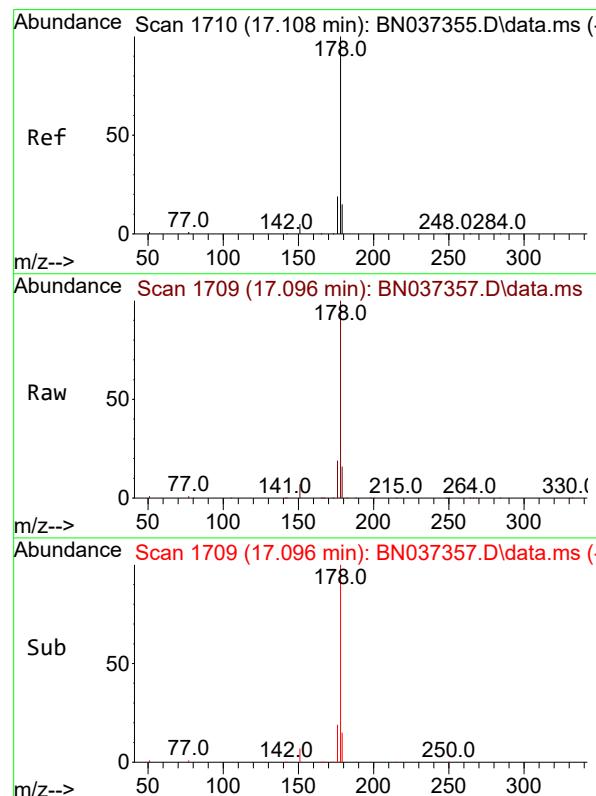

#26  
 Anthracene  
 Concen: 1.743 ng  
 RT: 17.096 min Scan# 1709  
 Delta R.T. -0.012 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Tgt Ion:178 Resp: 29693  
 Ion Ratio Lower Upper  
 178 100  
 176 18.7 14.7 22.1  
 179 15.5 13.0 19.6





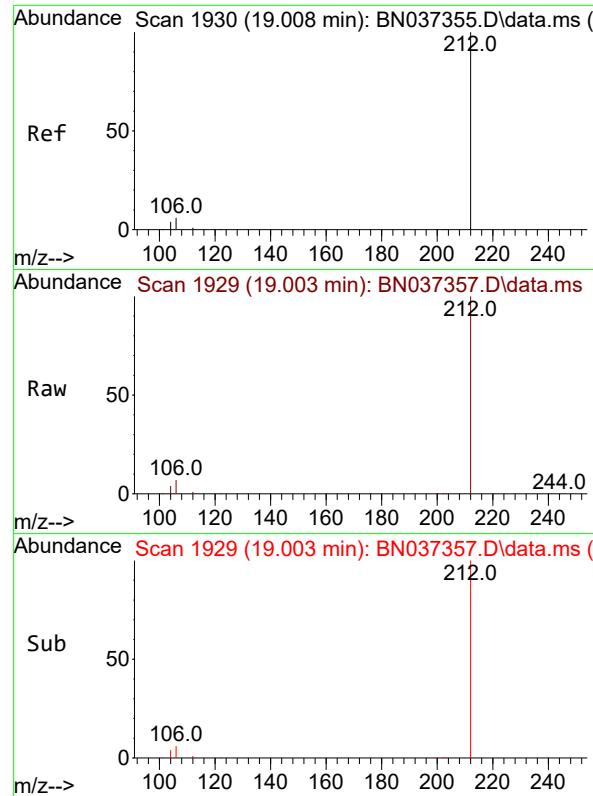

#27  
 Fluoranthene-d10  
 Concen: 1.586 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. -0.005 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:212 Resp: 31876  
 Ion Ratio Lower Upper  
 212 100  
 106 6.3 3.0 4.4#  
 104 3.8 2.0 3.0#

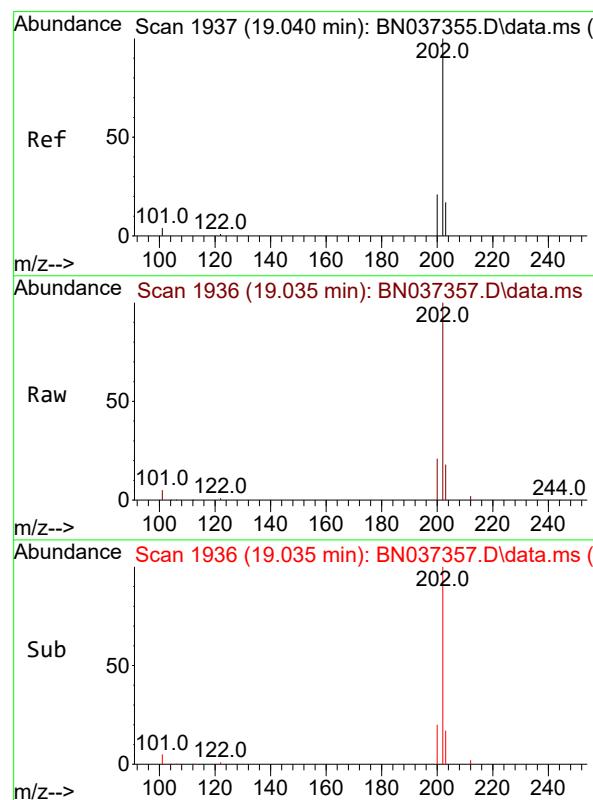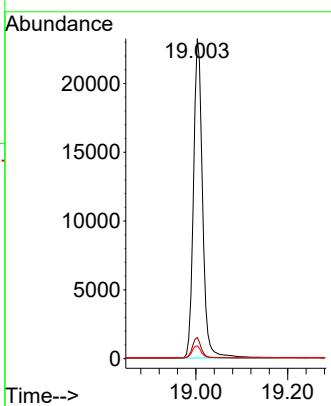

#28  
 Fluoranthene  
 Concen: 1.660 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Tgt Ion:202 Resp: 41430  
 Ion Ratio Lower Upper  
 202 100  
 101 5.4 3.0 4.6#  
 203 17.3 13.7 20.5


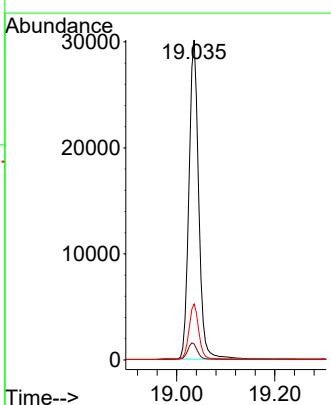


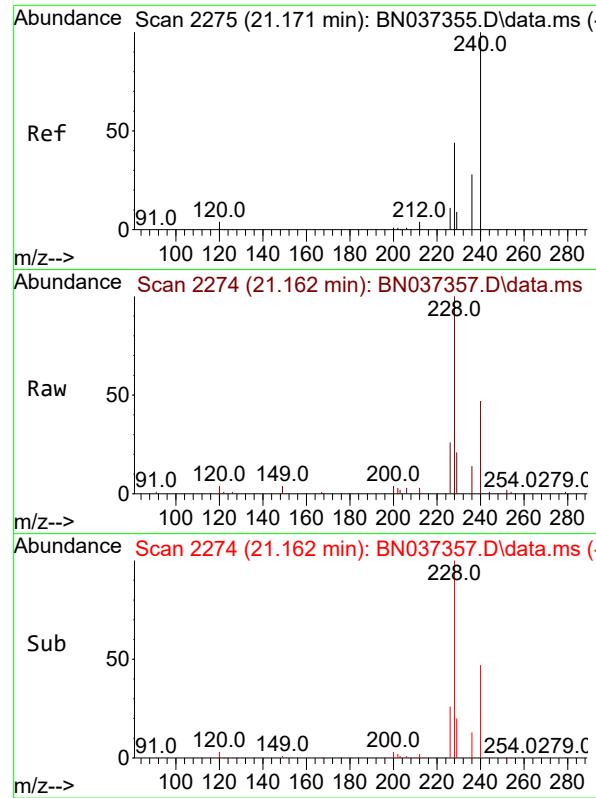

#29  
 Chrysene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 21.162 min Scan# 2  
 Delta R.T. -0.009 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:240 Resp: 6604  
 Ion Ratio Lower Upper  
 240 100  
 120 8.3 7.5 11.3  
 236 28.9 24.9 37.3

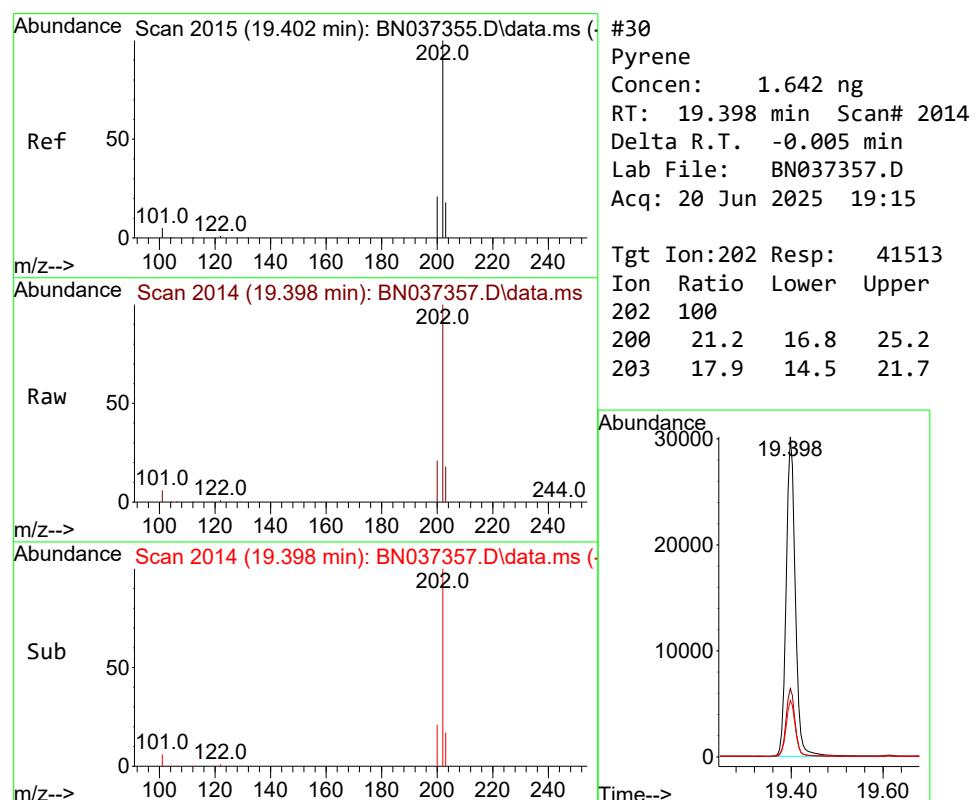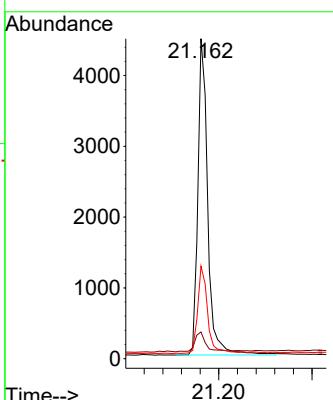

#30  
 Pyrene  
 Concen: 1.642 ng  
 RT: 19.398 min Scan# 2014  
 Delta R.T. -0.005 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Tgt Ion:202 Resp: 41513  
 Ion Ratio Lower Upper  
 202 100  
 200 21.2 16.8 25.2  
 203 17.9 14.5 21.7


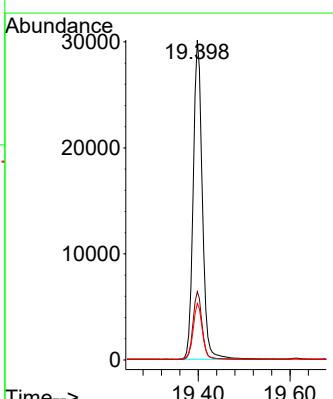


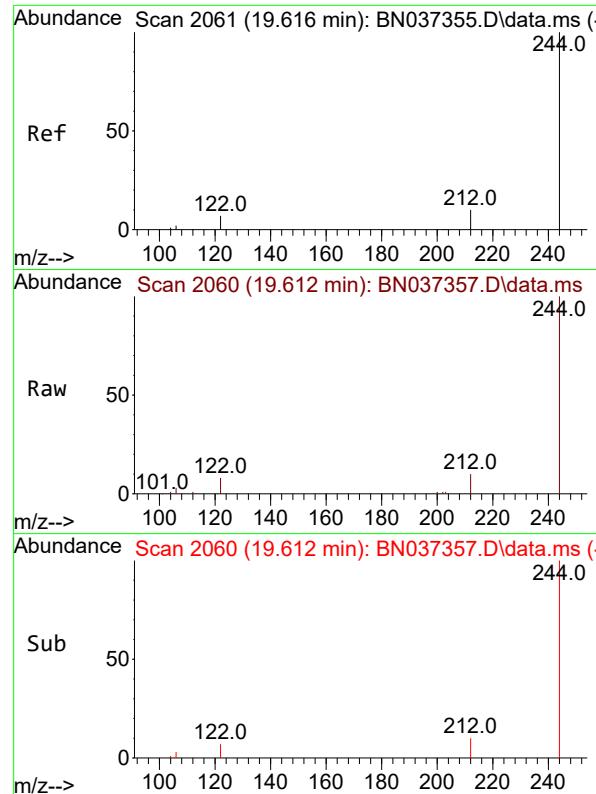

#31  
**Terphenyl-d14**  
Concen: 1.593 ng  
RT: 19.612 min Scan# 2  
Delta R.T. -0.005 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6


Tgt Ion:244 Resp: 24025  
Ion Ratio Lower Upper  
244 100  
212 10.3 11.1 16.7#  
122 7.7 7.2 10.8

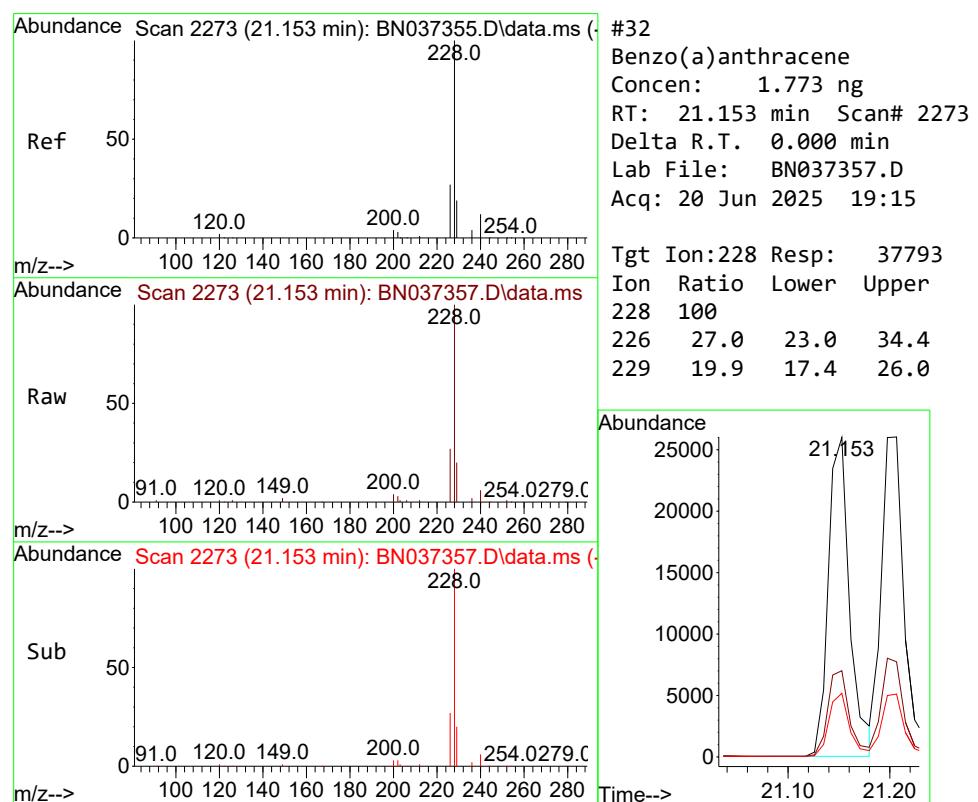

#32  
**Benzo(a)anthracene**  
Concen: 1.773 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.000 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15



Tgt Ion:228 Resp: 37793  
Ion Ratio Lower Upper  
228 100  
226 27.0 23.0 34.4  
229 19.9 17.4 26.0



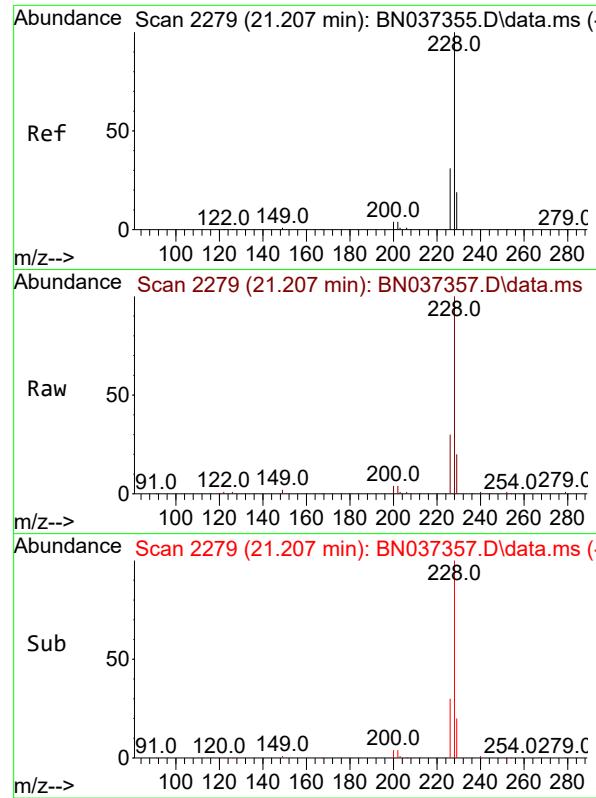


#33  
Chrysene  
Concen: 1.550 ng  
RT: 21.207 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15  
ClientSampleId : SSTDICC1.6


Tgt Ion:228 Resp: 41889  
Ion Ratio Lower Upper  
228 100  
226 29.8 25.4 38.2  
229 19.7 17.3 25.9

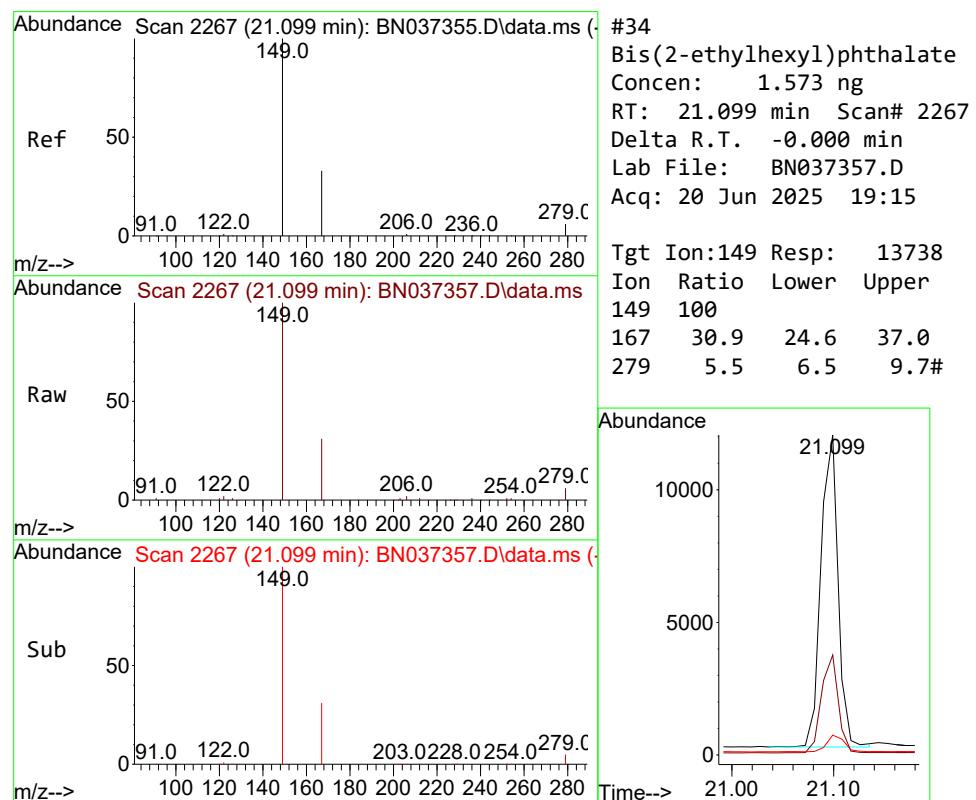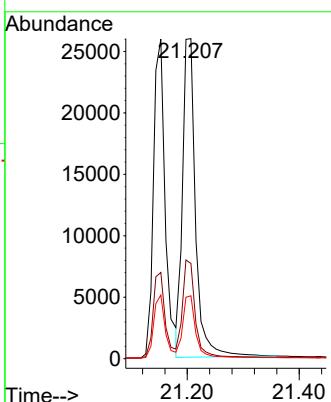

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 1.573 ng  
RT: 21.099 min Scan# 2267  
Delta R.T. -0.000 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15

Tgt Ion:149 Resp: 13738  
Ion Ratio Lower Upper  
149 100  
167 30.9 24.6 37.0  
279 5.5 6.5 9.7#





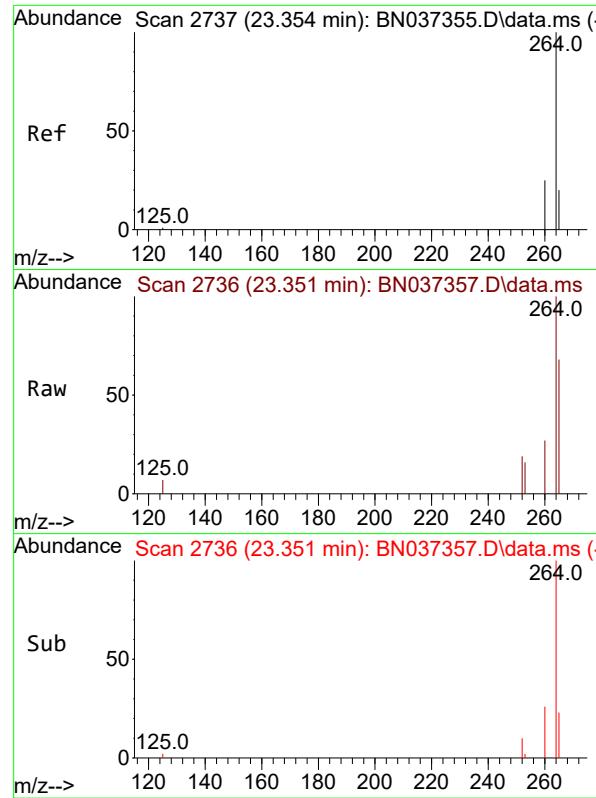

#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.351 min Scan# 2  
Delta R.T. -0.003 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6


Tgt Ion:264 Resp: 7013  
Ion Ratio Lower Upper  
264 100  
260 26.9 21.4 32.2  
265 68.4 71.4 107.0#

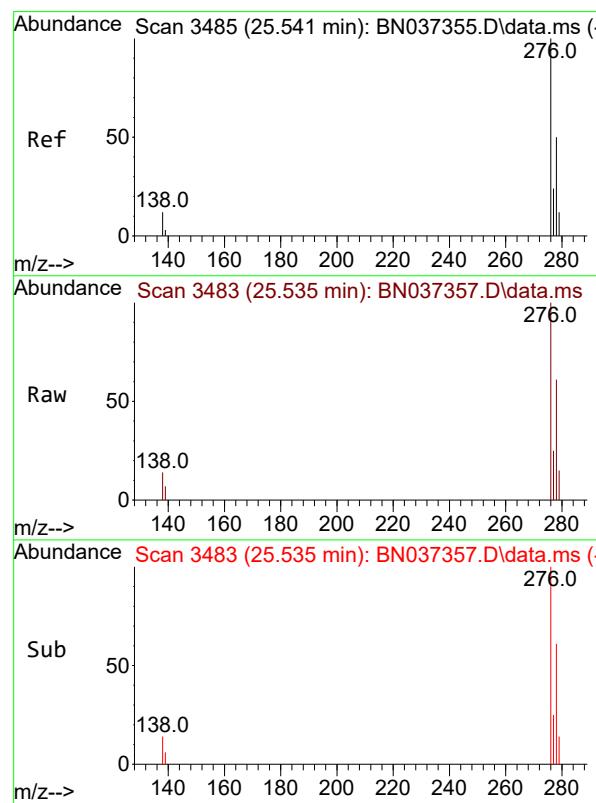

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 1.863 ng  
RT: 25.535 min Scan# 3483  
Delta R.T. -0.006 min  
Lab File: BN037357.D  
Acq: 20 Jun 2025 19:15

Tgt Ion:276 Resp: 55371  
Ion Ratio Lower Upper  
276 100  
138 14.3 2.2 3.2#  
277 24.2 17.1 25.7





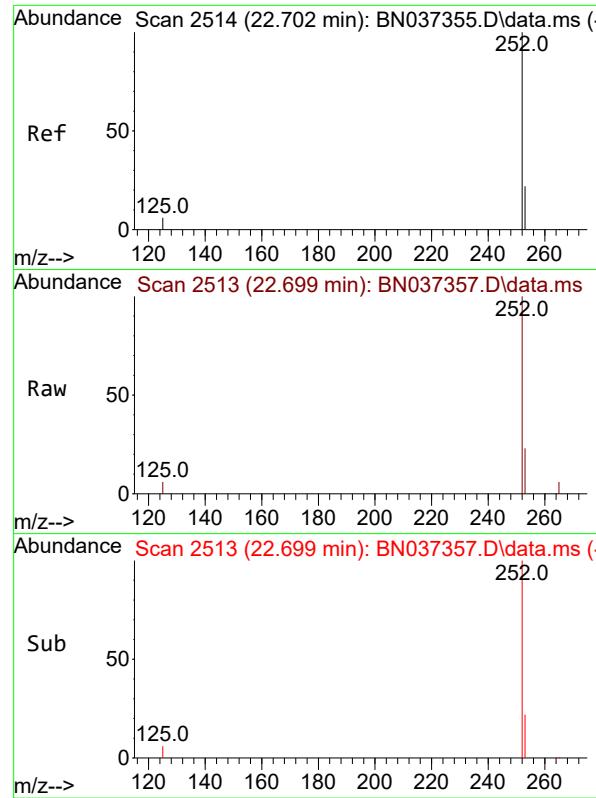

#37  
 Benzo(b)fluoranthene  
 Concen: 1.738 ng  
 RT: 22.699 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:252 Resp: 43215  
 Ion Ratio Lower Upper  
 252 100  
 253 23.1 26.6 40.0#  
 125 6.1 6.1 9.1

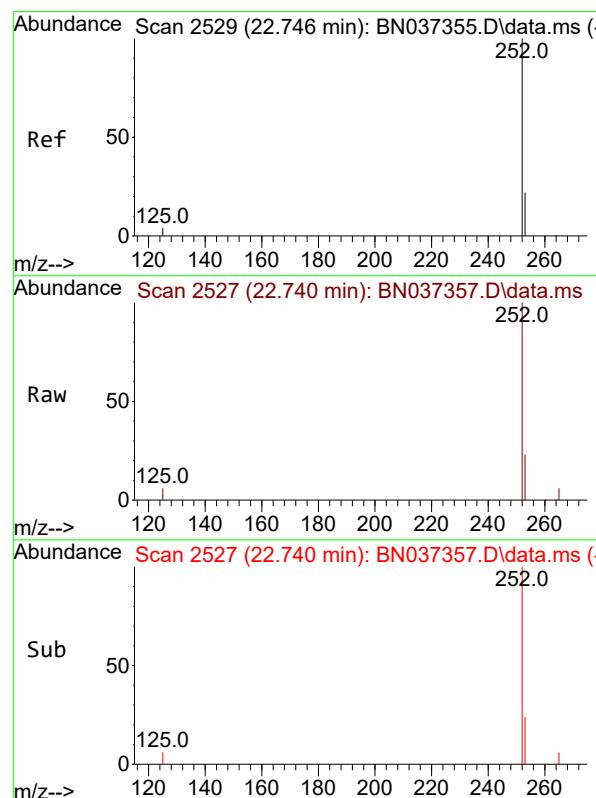

#38  
 Benzo(k)fluoranthene  
 Concen: 1.736 ng  
 RT: 22.740 min Scan# 2527  
 Delta R.T. -0.006 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Tgt Ion:252 Resp: 46879  
 Ion Ratio Lower Upper  
 252 100  
 253 23.4 26.7 40.1#  
 125 6.0 6.5 9.7#





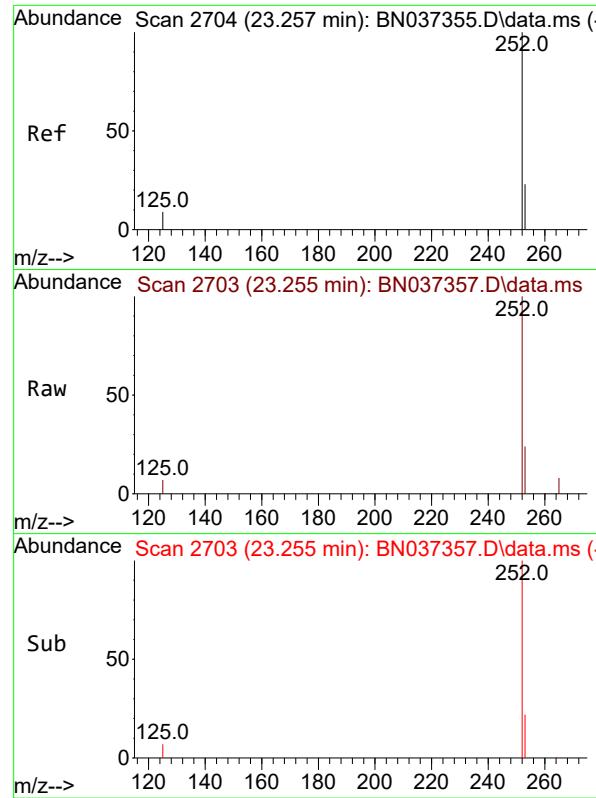

#39  
 Benzo(a)pyrene  
 Concen: 1.724 ng  
 RT: 23.255 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:252 Resp: 39242  
 Ion Ratio Lower Upper  
 252 100  
 253 24.1 31.6 47.4#  
 125 7.5 8.4 12.6#

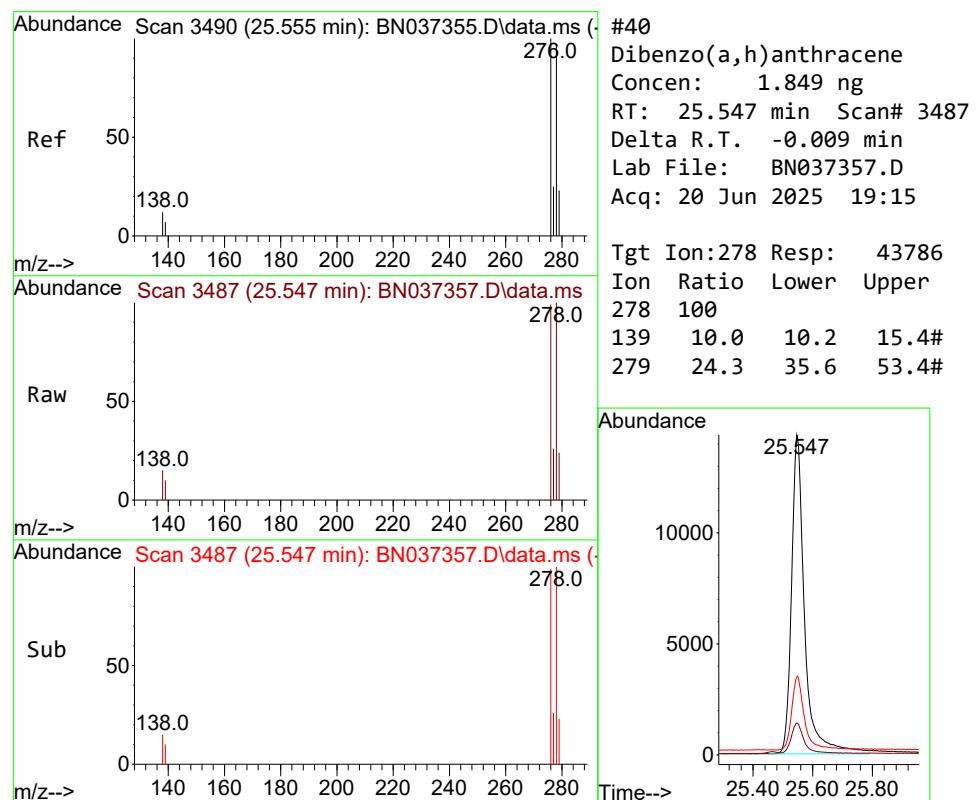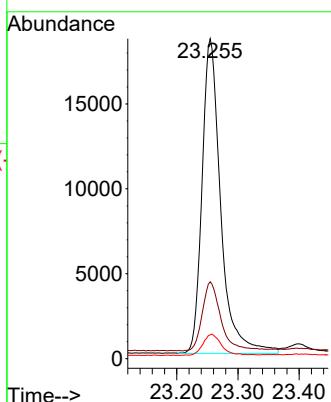

#40  
 Dibenzo(a,h)anthracene  
 Concen: 1.849 ng  
 RT: 25.547 min Scan# 3487  
 Delta R.T. -0.009 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Tgt Ion:278 Resp: 43786  
 Ion Ratio Lower Upper  
 278 100  
 139 10.0 10.2 15.4#  
 279 24.3 35.6 53.4#




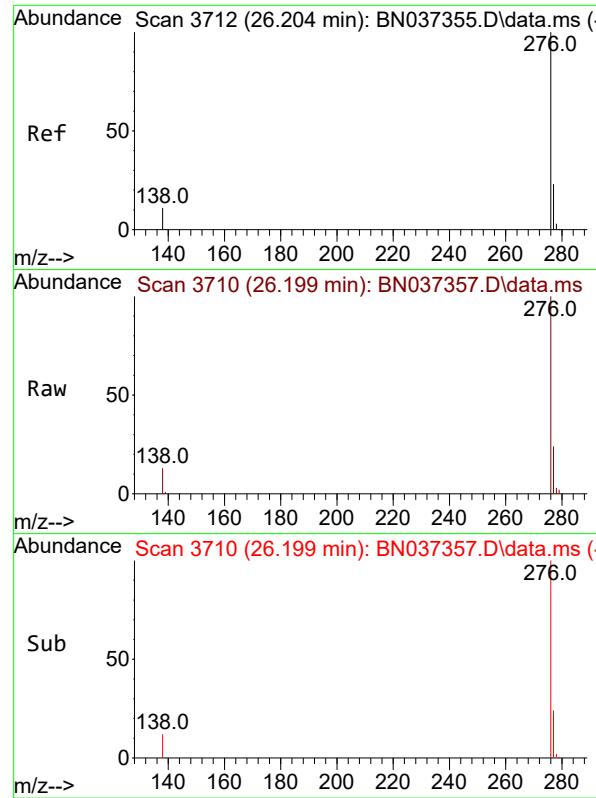

#41  
 Benzo(g,h,i)perylene  
 Concen: 1.767 ng  
 RT: 26.199 min Scan# 3  
 Delta R.T. -0.006 min  
 Lab File: BN037357.D  
 Acq: 20 Jun 2025 19:15

Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6

Tgt Ion:276 Resp: 48259  
 Ion Ratio Lower Upper  
 276 100  
 277 24.2 22.7 34.1  
 138 12.9 9.4 14.2

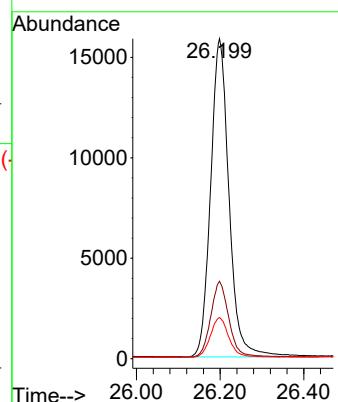

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037358.D  
 Acq On : 20 Jun 2025 19:51  
 Operator : RC/JU  
 Sample : SSTDICC3.2  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC3.2

Quant Time: Jun 20 23:28:00 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2553	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	5431	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	3830	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	7833	0.400	ng	#-0.01
29) Chrysene-d12	21.162	240	7155	0.400	ng	0.00
35) Perylene-d12	23.348	264	6736	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	16051	3.439	ng	0.00
5) Phenol-d6	6.744	99	17930	3.882	ng	0.00
8) Nitrobenzene-d5	8.707	82	15387	3.413	ng	-0.01
11) 2-Methylnaphthalene-d10	11.940	152	28839	3.282	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	7296	2.664	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	53666	3.194	ng	0.00
27) Fluoranthene-d10	19.003	212	72122	2.957	ng	0.00
31) Terphenyl-d14	19.611	244	53536	3.277	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.097	88	7556	3.351	ng	91
3) n-Nitrosodimethylamine	3.408	42	7228	2.753	ng	# 72
6) bis(2-Chloroethyl)ether	6.997	93	16052	3.972	ng	97
9) Naphthalene	10.394	128	45711	3.247	ng	# 86
10) Hexachlorobutadiene	10.682	225	16687	2.426	ng	# 99
12) 2-Methylnaphthalene	12.016	142	33783	3.412	ng	# 92
16) Acenaphthylene	13.935	152	52599	3.272	ng	98
17) Acenaphthene	14.277	154	34413	3.229	ng	98
18) Fluorene	15.271	166	49180	3.256	ng	100
20) 4,6-Dinitro-2-methylph...	15.357	198	6721	2.838	ng	# 44
21) 4-Bromophenyl-phenylether	16.165	248	18488	2.891	ng	96
22) Hexachlorobenzene	16.276	284	18573	2.784	ng	98
23) Atrazine	16.438	200	14961	2.988	ng	# 81
24) Pentachlorophenol	16.624	266	10110	2.761	ng	97
25) Phenanthrene	17.009	178	76487	3.455	ng	99
26) Anthracene	17.095	178	71218	3.446	ng	98
28) Fluoranthene	19.035	202	94745	3.129	ng	# 99
30) Pyrene	19.398	202	93984	3.430	ng	99
32) Benzo(a)anthracene	21.144	228	78532	3.401	ng	97
33) Chrysene	21.197	228	87474	2.987	ng	97
34) Bis(2-ethylhexyl)phtha...	21.090	149	30412	3.214	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.529	276	98025	3.433	ng	# 90
37) Benzo(b)fluoranthene	22.696	252	82568	3.456	ng	# 84
38) Benzo(k)fluoranthene	22.737	252	87144	3.359	ng	# 83
39) Benzo(a)pyrene	23.254	252	72643	3.323	ng	# 76
40) Dibenzo(a,h)anthracene	25.547	278	77899	3.426	ng	# 74
41) Benzo(g,h,i)perylene	26.199	276	84957	3.239	ng	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037358.D  
 Acq On : 20 Jun 2025 19:51  
 Operator : RC/JU  
 Sample : SSTDICC3.2  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC3.2


Quant Time: Jun 20 23:28:00 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration

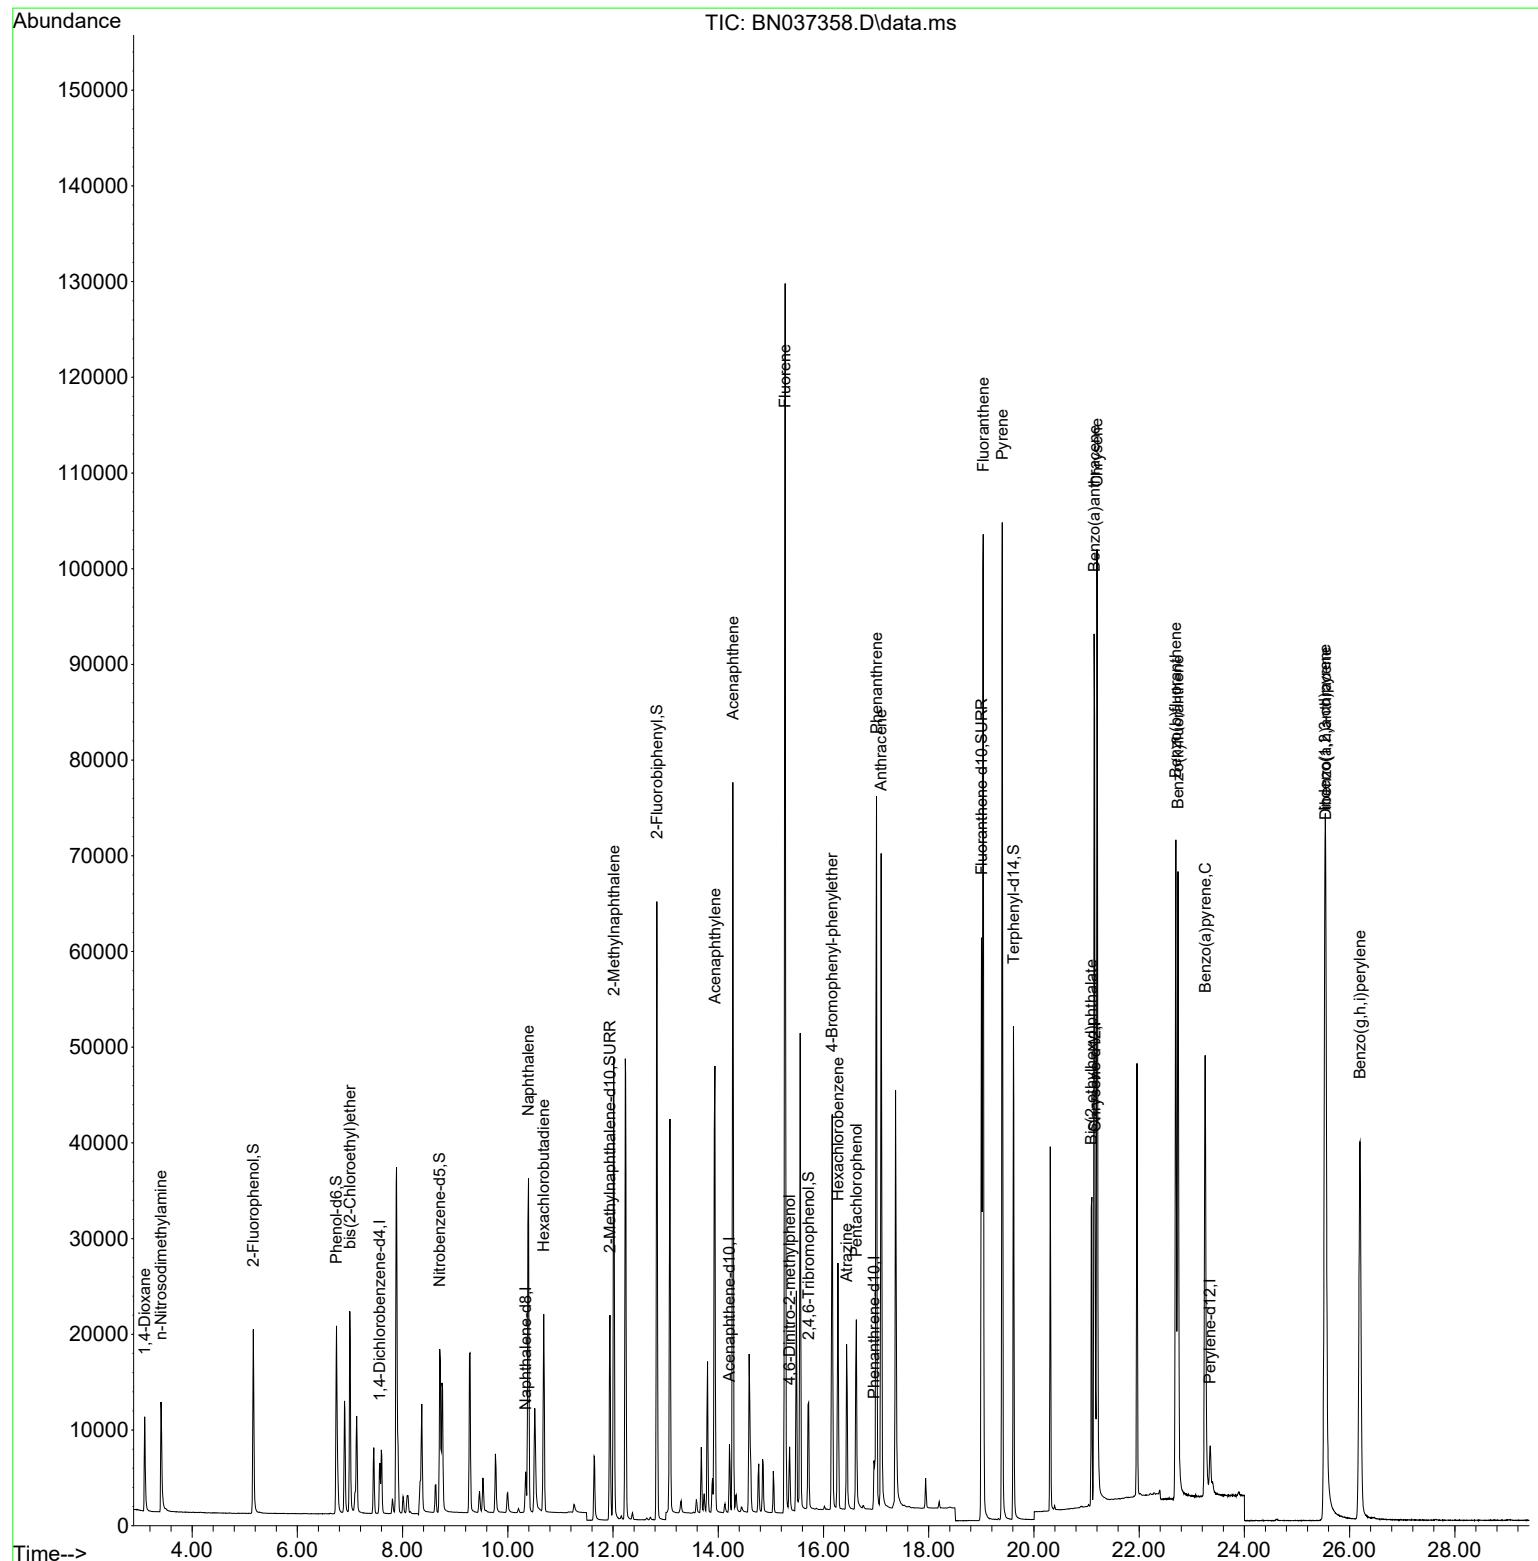






#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2





Tgt Ion:152 Resp: 2553  
Ion Ratio Lower Upper  
152 100  
150 151.3 112.7 169.1  
115 53.5 45.9 68.9

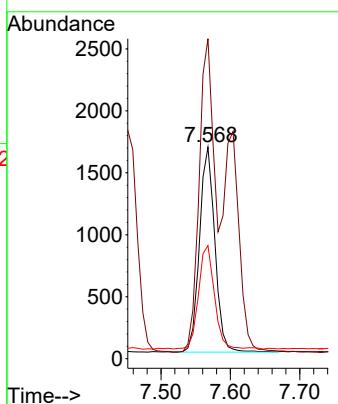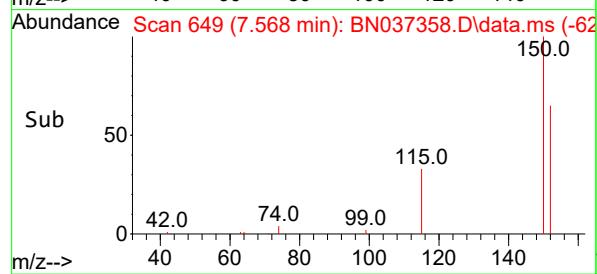


#2  
1,4-Dioxane  
Concen: 3.351 ng  
RT: 3.097 min Scan# 30  
Delta R.T. -0.007 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51





Tgt Ion: 88 Resp: 7556  
Ion Ratio Lower Upper  
88 100  
43 22.5 21.0 31.6  
58 54.2 38.0 57.0

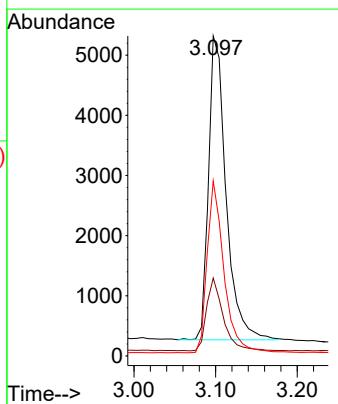

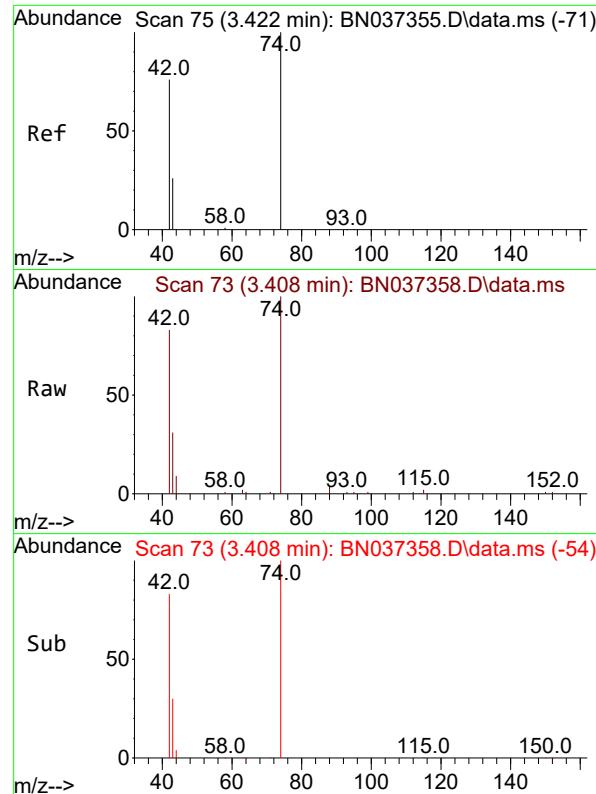


#3  
n-Nitrosodimethylamine  
Concen: 2.753 ng  
RT: 3.408 min Scan# 7  
Instrument : BNA\_N  
Delta R.T. -0.015 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51  
ClientSampleId : SSTDICC3.2


Tgt Ion: 42 Resp: 7228  
Ion Ratio Lower Upper  
42 100  
74 135.8 84.3 126.5#  
44 5.2 5.0 7.4

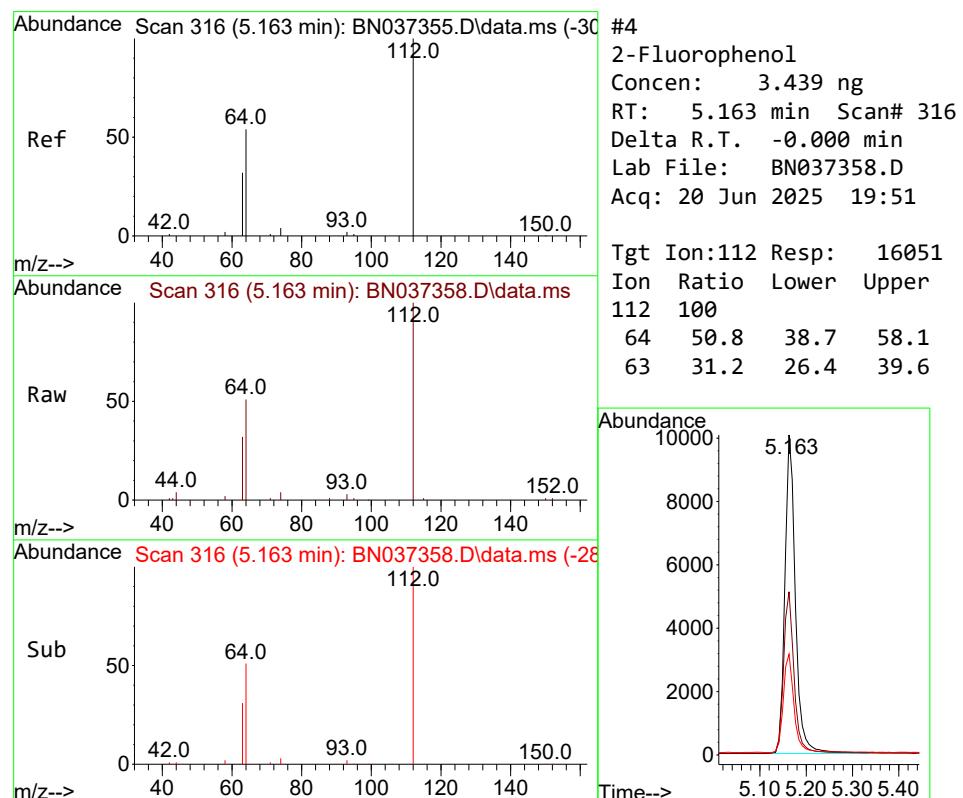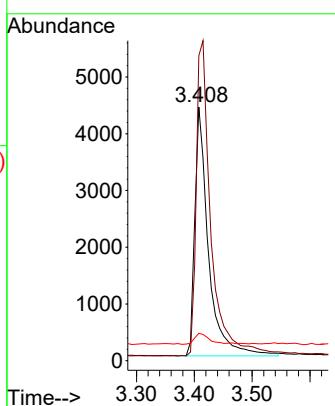

#4  
2-Fluorophenol  
Concen: 3.439 ng  
RT: 5.163 min Scan# 316  
Delta R.T. -0.000 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51

Tgt Ion: 112 Resp: 16051  
Ion Ratio Lower Upper  
112 100  
64 50.8 38.7 58.1  
63 31.2 26.4 39.6





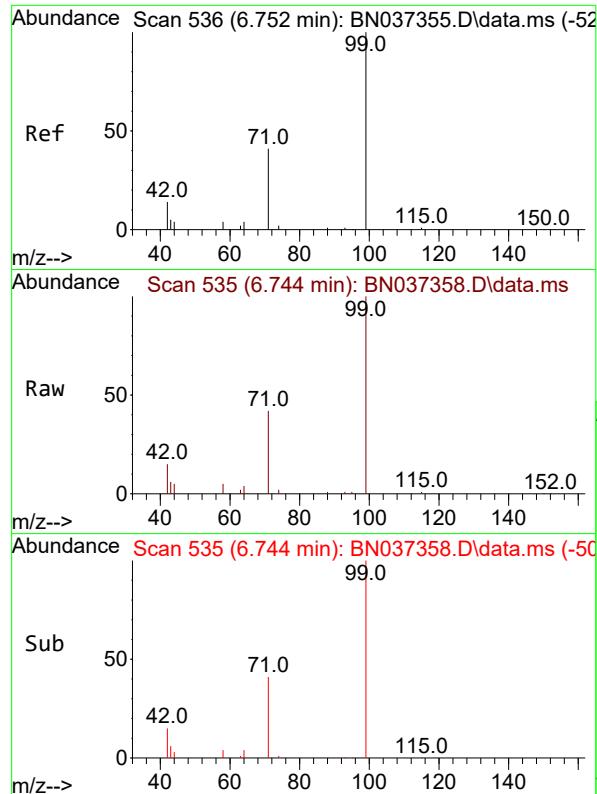

#5  
 Phenol-d6  
 Concen: 3.882 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. -0.007 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2




Tgt Ion: 99 Resp: 17930  
 Ion Ratio Lower Upper  
 99 100  
 42 17.7 19.8 29.8#  
 71 42.9 42.6 64.0

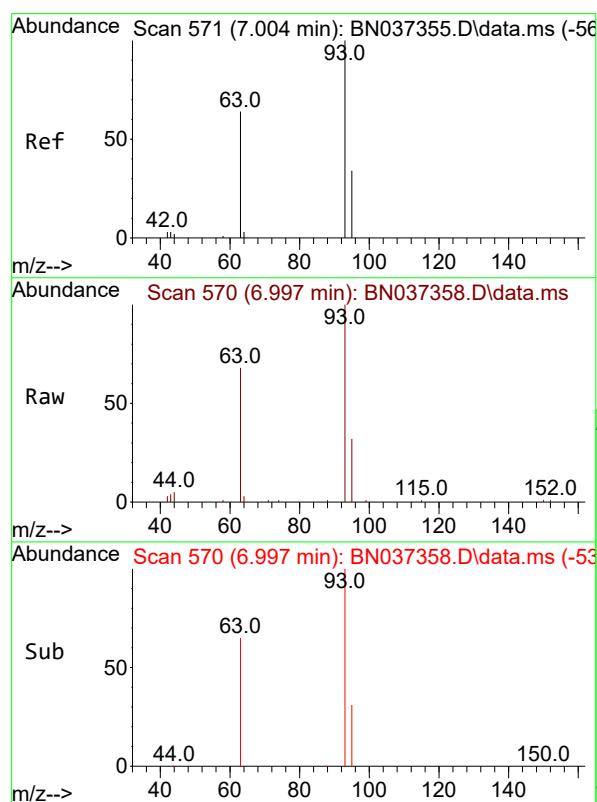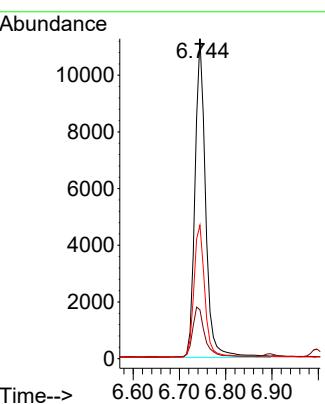

#6  
 bis(2-Chloroethyl)ether  
 Concen: 3.972 ng  
 RT: 6.997 min Scan# 570  
 Delta R.T. -0.007 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion: 93 Resp: 16052  
 Ion Ratio Lower Upper  
 93 100  
 63 64.4 53.2 79.8  
 95 31.6 27.3 40.9

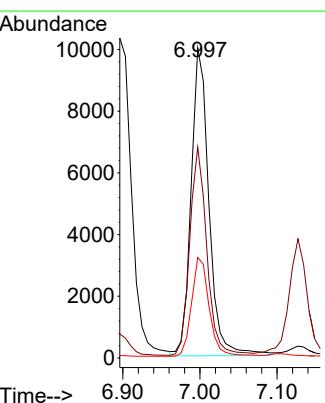



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.340 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2

Tgt Ion:136 Resp: 5431

Ion Ratio Lower Upper

136 100





137 12.4 12.2 18.2

54 6.7 8.8 13.2#

68 5.6 7.0 10.4#

Abundance

10.340

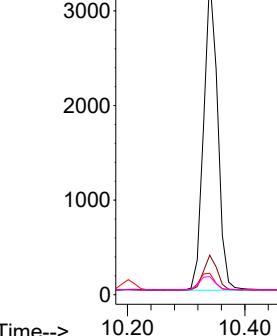

#8

Nitrobenzene-d5

Concen: 3.413 ng

RT: 8.707 min Scan# 789

Delta R.T. -0.011 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Tgt Ion: 82 Resp: 15387

Ion Ratio Lower Upper


82 100




128 33.6 42.5 63.7#

54 43.9 43.2 64.8

Abundance

8.707

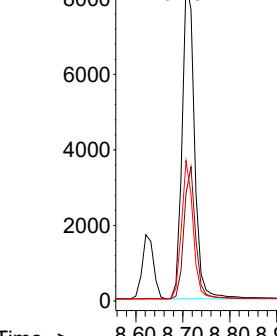

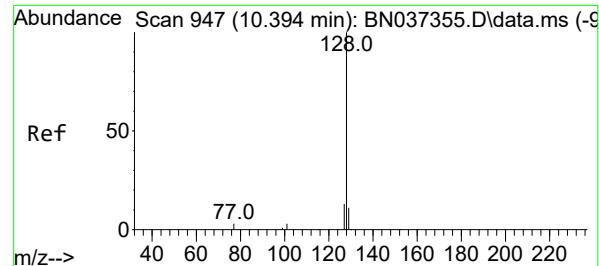

#9

Naphthalene

Concen: 3.247 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2

Tgt Ion:128 Resp: 45711

Ion Ratio Lower Upper

128 100

129 11.1 14.0 21.0#

127 13.5 15.8 23.8#

Abundance

25000

20000





15000

10000

5000

0

10.394

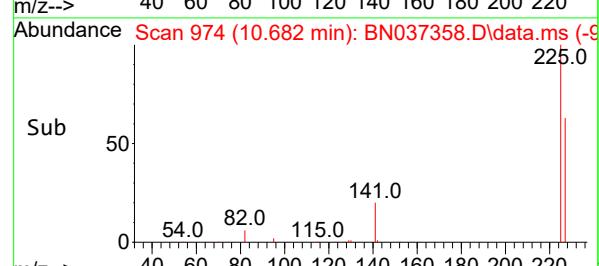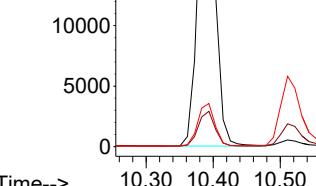

#10

Hexachlorobutadiene

Concen: 2.426 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Tgt Ion:225 Resp: 16687

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.8 50.3 75.5

Abundance

10000

8000


6000


4000

2000


0

10.682

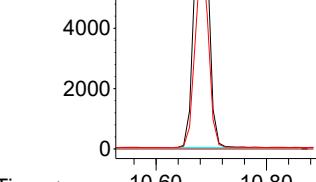



Abundance Scan 1137 (11.940 min): BN037358.D\data.ms (-)

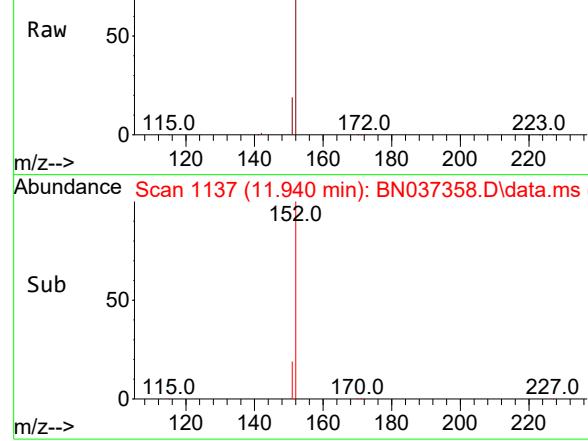

#11

2-Methylnaphthalene-d10

Concen: 3.282 ng

RT: 11.940 min Scan# 1137

Delta R.T. -0.005 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Instrument : BNA\_N



ClientSampleId : SSTDICC3.2

Tgt Ion:152 Resp: 28839


Ion Ratio Lower Upper

152 100

151 21.3 17.4 26.0

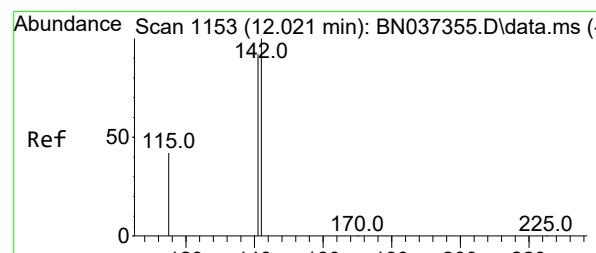

Abundance Scan 1152 (12.016 min): BN037358.D\data.ms (-)

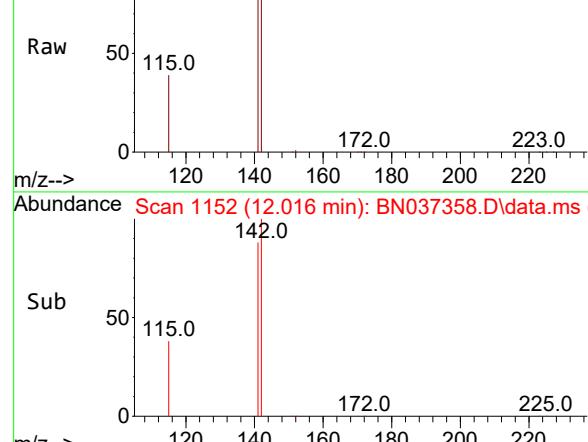

#12

2-Methylnaphthalene

Concen: 3.412 ng

RT: 12.016 min Scan# 1152

Delta R.T. -0.005 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51


Tgt Ion:142 Resp: 33783


Ion Ratio Lower Upper

142 100

141 88.4 70.2 105.2

115 38.7 43.0 64.4#



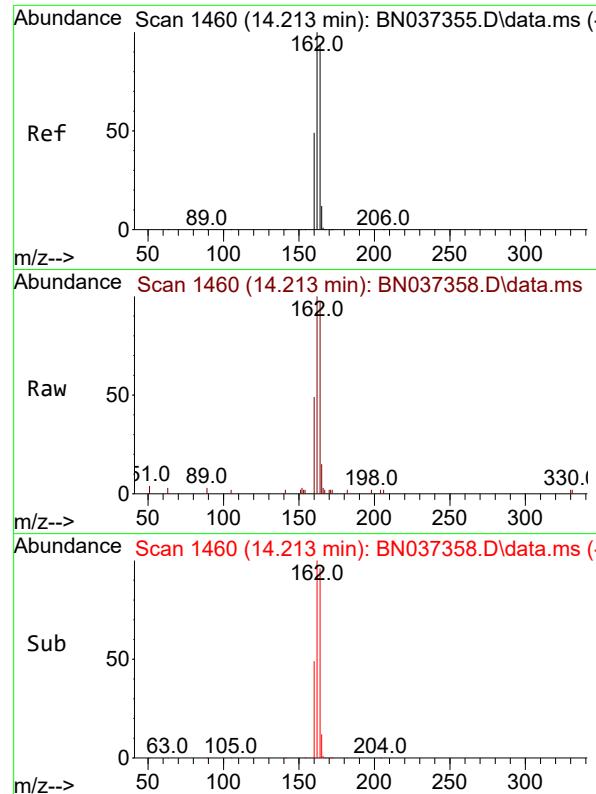

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2



Tgt Ion:164 Resp: 3830

Ion Ratio Lower Upper

164 100

162 103.5 81.5 122.3

160 51.1 43.0 64.4

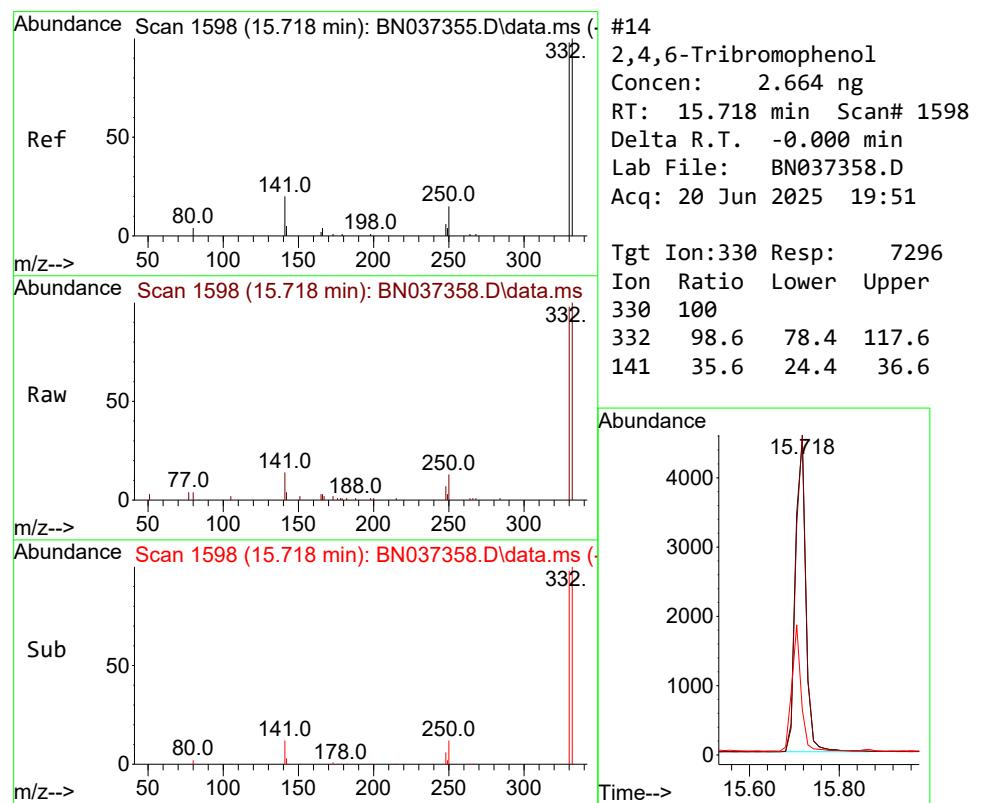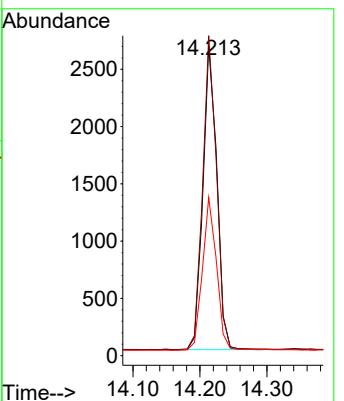

#14

2,4,6-Tribromophenol

Concen: 2.664 ng

RT: 15.718 min Scan# 1598

Delta R.T. -0.000 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51


Tgt Ion:330 Resp: 7296


Ion Ratio Lower Upper

330 100

332 98.6 78.4 117.6

141 35.6 24.4 36.6


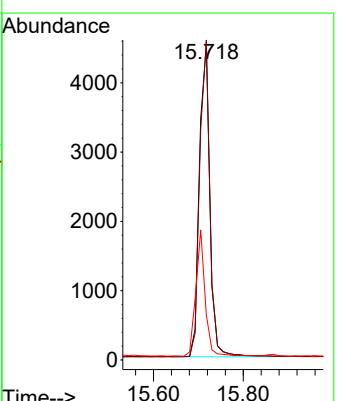


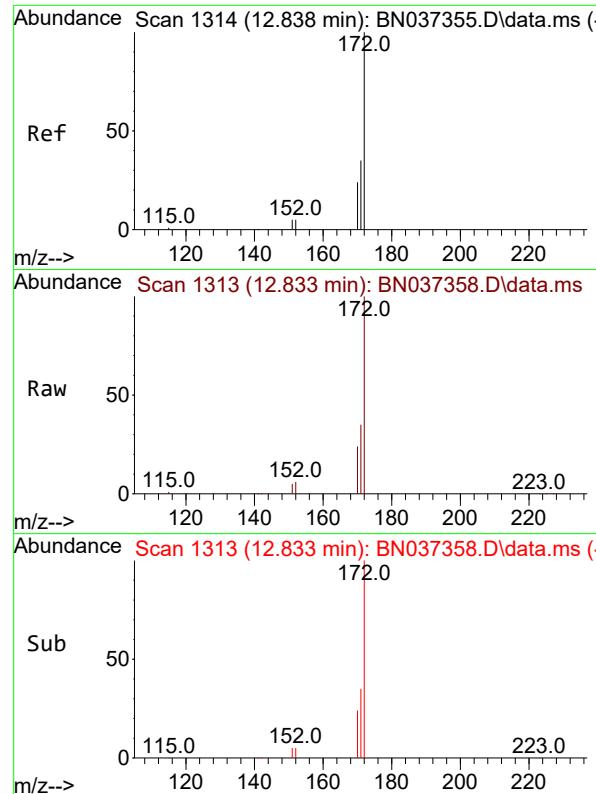

#15  
2-Fluorobiphenyl  
Concen: 3.194 ng  
RT: 12.833 min Scan# 1  
Delta R.T. -0.005 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2




Tgt Ion:172 Resp: 53666  
Ion Ratio Lower Upper  
172 100  
171 35.5 30.8 46.2  
170 23.9 21.9 32.9

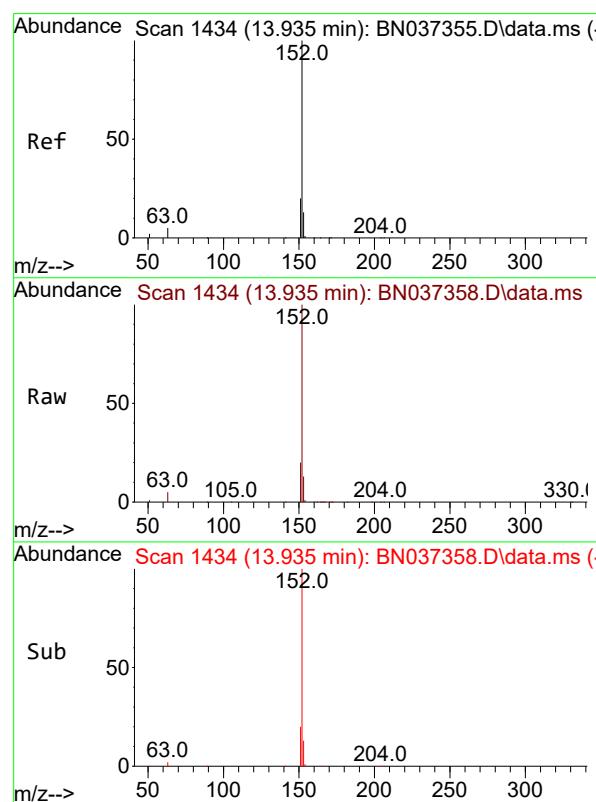

#16  
Acenaphthylene  
Concen: 3.272 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51

Tgt Ion:152 Resp: 52599  
Ion Ratio Lower Upper  
152 100  
151 19.8 16.6 24.8  
153 13.1 10.2 15.2



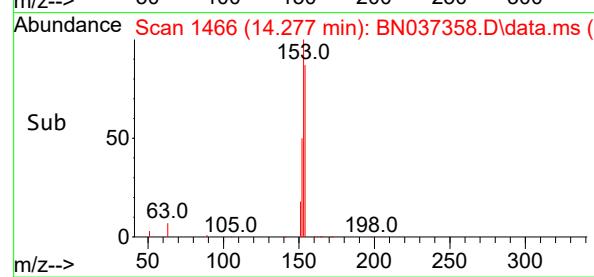

#17

Acenaphthene

Concen: 3.229 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2

Tgt Ion:154 Resp: 34413

Ion Ratio Lower Upper

154 100

153 114.5 93.1 139.7

152 58.7 48.6 73.0

Abundance

25000

20000

15000




10000

5000

0

14.277

Time--&gt; 14.10 14.20 14.30

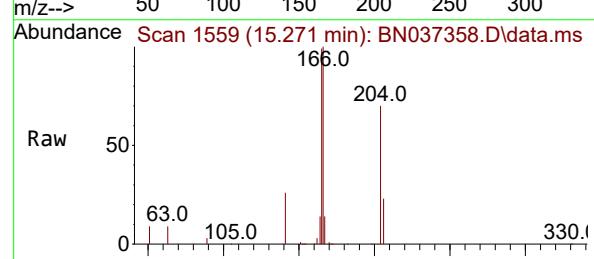

#18

Fluorene

Concen: 3.256 ng

RT: 15.271 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

Tgt Ion:166 Resp: 49180

Ion Ratio Lower Upper

166 100

165 99.3 79.5 119.3

167 13.5 10.7 16.1

Abundance

30000


20000

10000

0

15.271



Time--&gt; 15.20 15.30 15.40

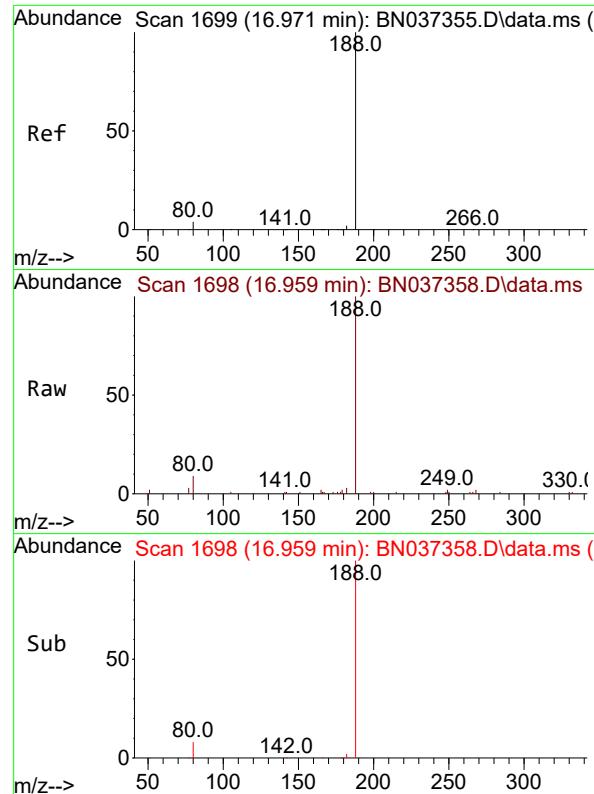

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.959 min Scan# 1  
 Delta R.T. -0.012 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:188 Resp: 7833  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 9.4 6.2 9.2#

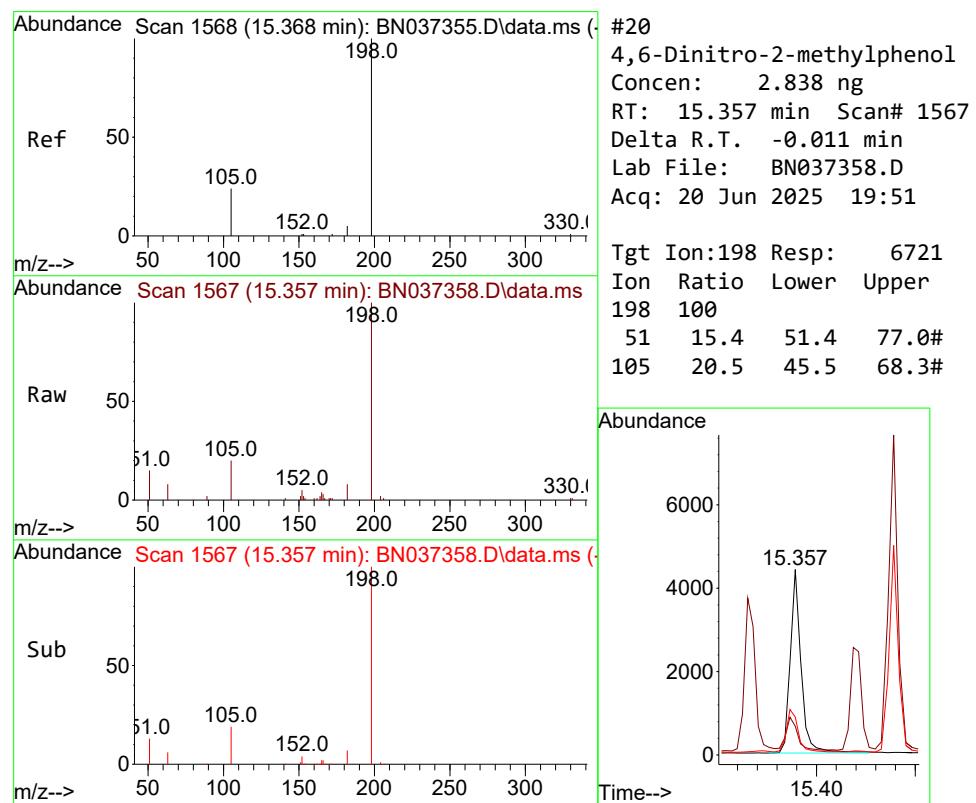

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 2.838 ng  
 RT: 15.357 min Scan# 1567  
 Delta R.T. -0.011 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion:198 Resp: 6721  
 Ion Ratio Lower Upper  
 198 100  
 51 15.4 51.4 77.0#  
 105 20.5 45.5 68.3#


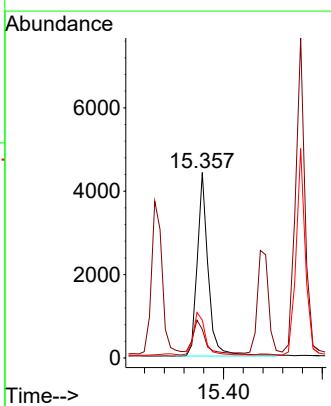


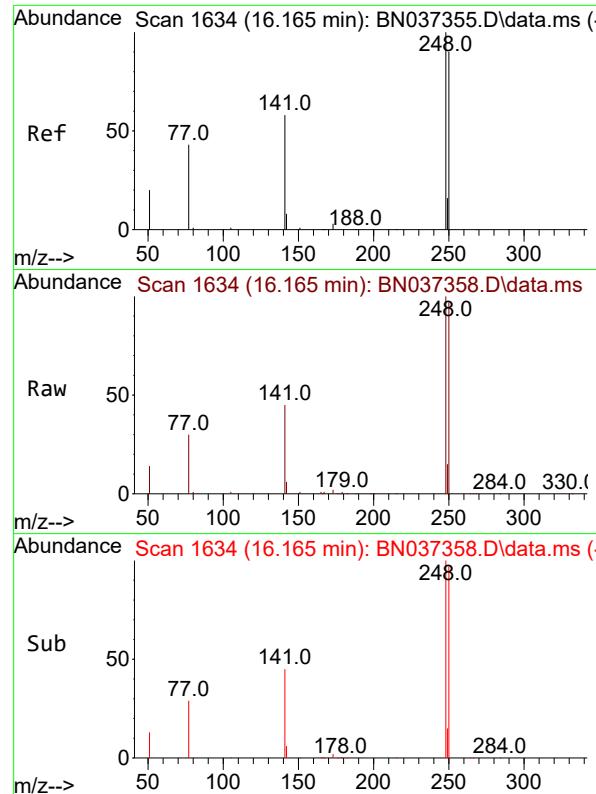

#21  
 4-Bromophenyl-phenylether  
 Concen: 2.891 ng  
 RT: 16.165 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:248 Resp: 18488  
 Ion Ratio Lower Upper  
 248 100  
 250 96.9 80.4 120.6  
 141 45.2 33.3 49.9

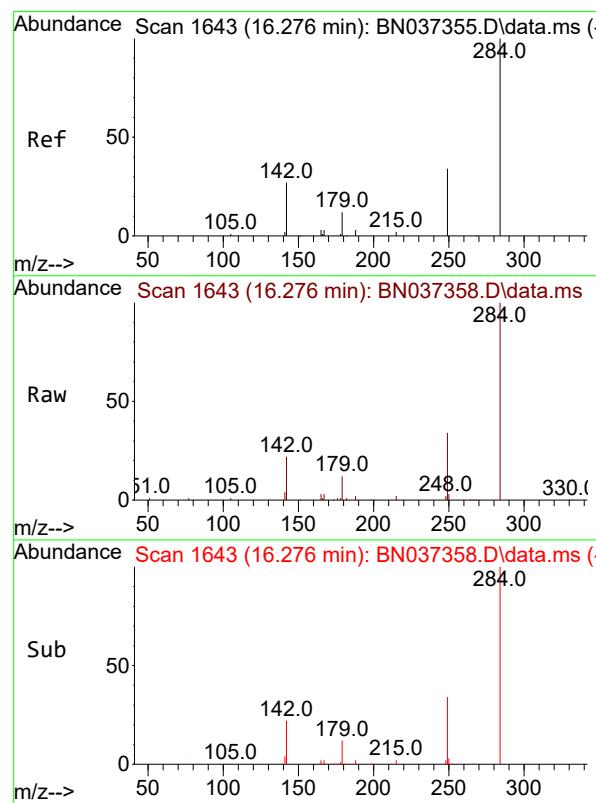

#22  
 Hexachlorobenzene  
 Concen: 2.784 ng  
 RT: 16.276 min Scan# 1643  
 Delta R.T. -0.000 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion:284 Resp: 18573  
 Ion Ratio Lower Upper  
 284 100  
 142 34.8 27.0 40.6  
 249 34.5 28.8 43.2




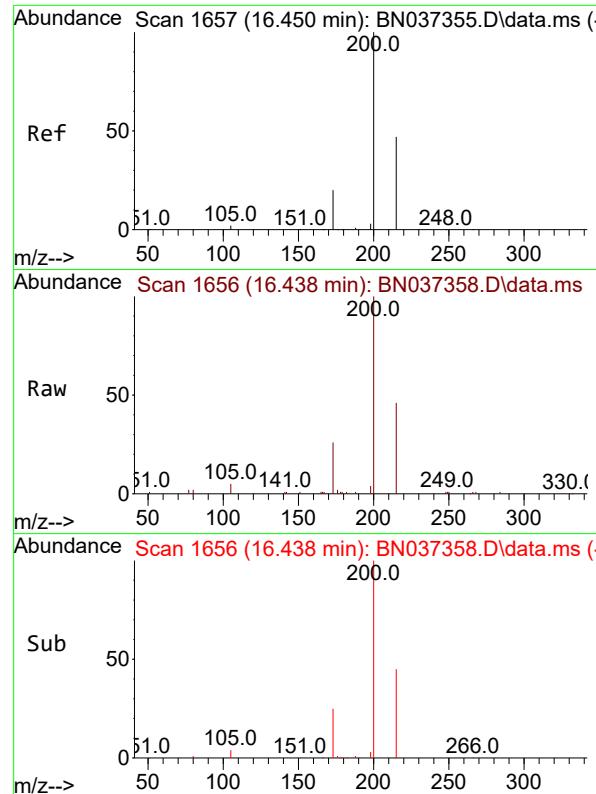

#23  
Atrazine  
Concen: 2.988 ng  
RT: 16.438 min Scan# 1  
Delta R.T. -0.012 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51

Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:200 Resp: 14961  
Ion Ratio Lower Upper  
200 100  
173 25.8 29.2 43.8#  
215 45.7 48.8 73.2#

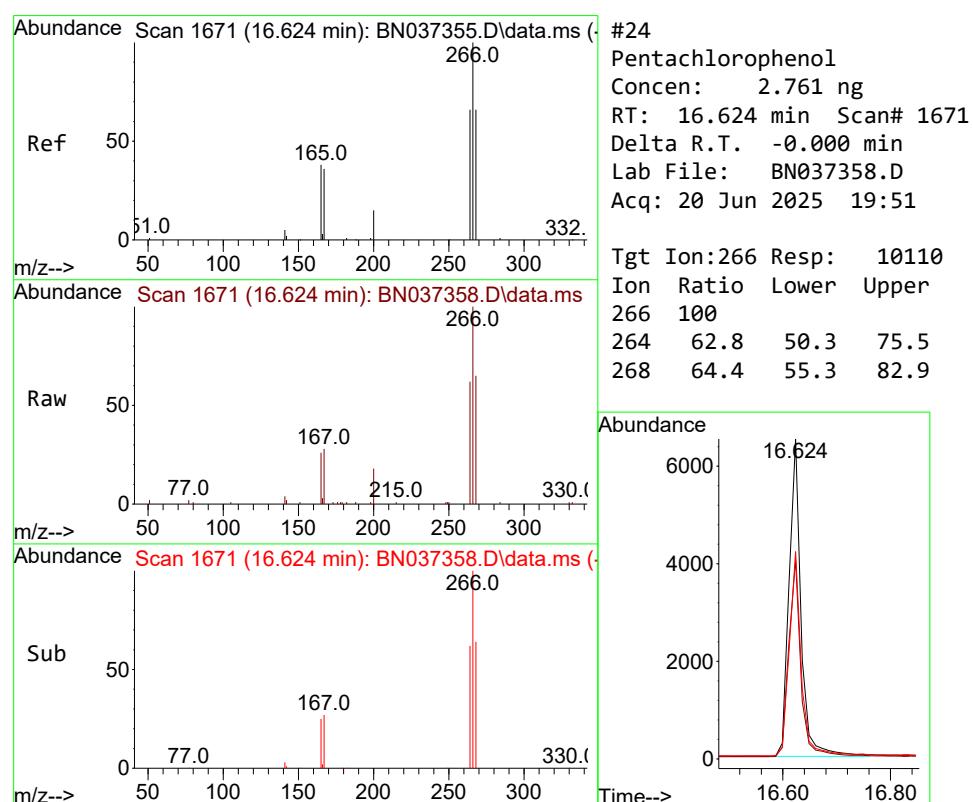

#24  
Pentachlorophenol  
Concen: 2.761 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51

Tgt Ion:266 Resp: 10110  
Ion Ratio Lower Upper  
266 100  
264 62.8 50.3 75.5  
268 64.4 55.3 82.9



1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18

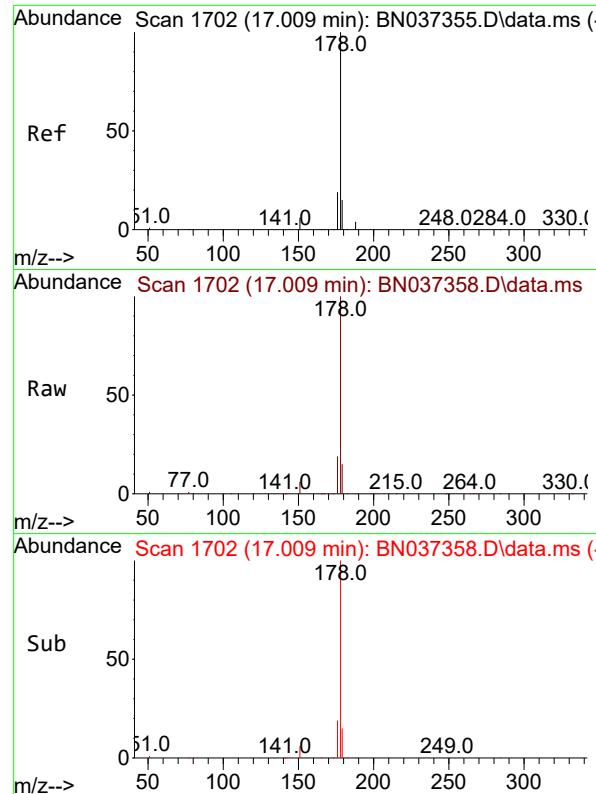

#25  
 Phenanthrene  
 Concen: 3.455 ng  
 RT: 17.009 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:178 Resp: 76487  
 Ion Ratio Lower Upper  
 178 100  
 176 19.4 15.2 22.8  
 179 15.2 12.9 19.3

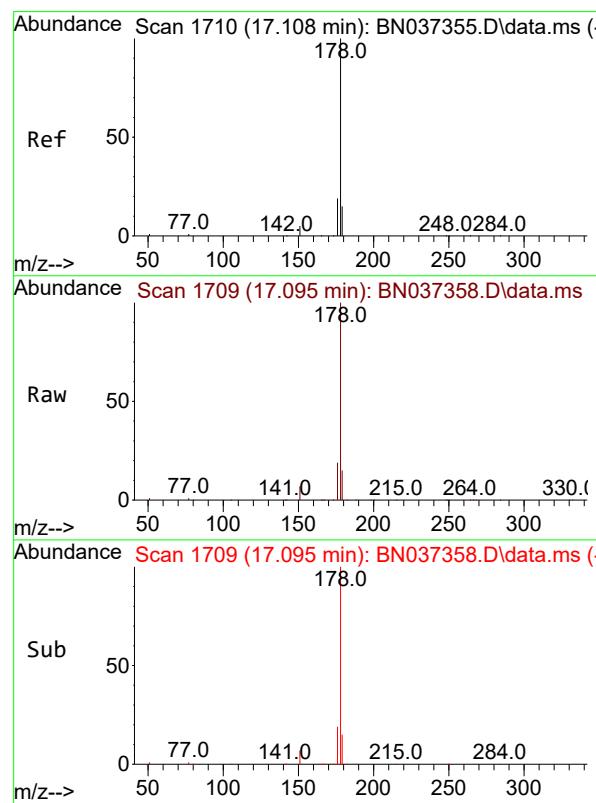

#26  
 Anthracene  
 Concen: 3.446 ng  
 RT: 17.095 min Scan# 1709  
 Delta R.T. -0.012 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion:178 Resp: 71218  
 Ion Ratio Lower Upper  
 178 100  
 176 18.8 14.7 22.1  
 179 15.3 13.0 19.6


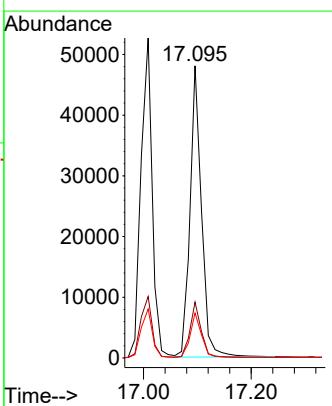


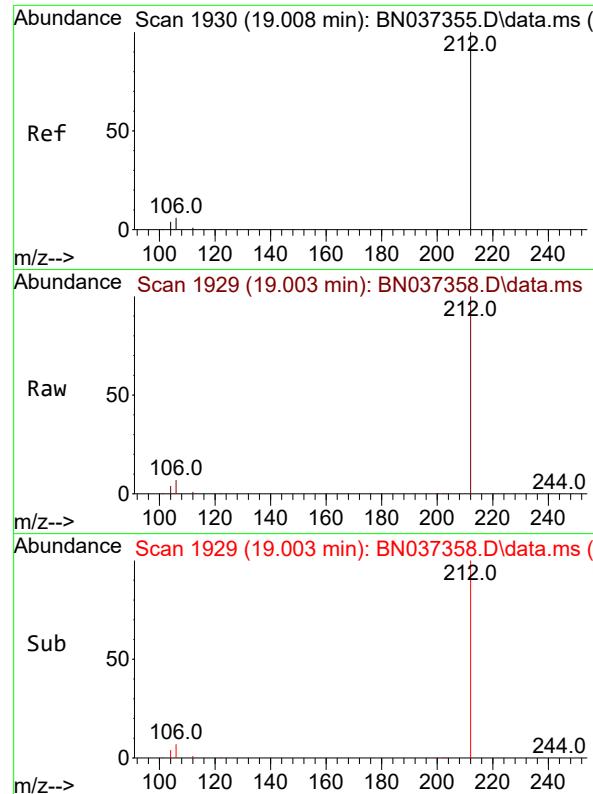

#27  
 Fluoranthene-d10  
 Concen: 2.957 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. -0.005 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:212 Resp: 72122  
 Ion Ratio Lower Upper  
 212 100  
 106 6.8 3.0 4.4#  
 104 4.1 2.0 3.0#

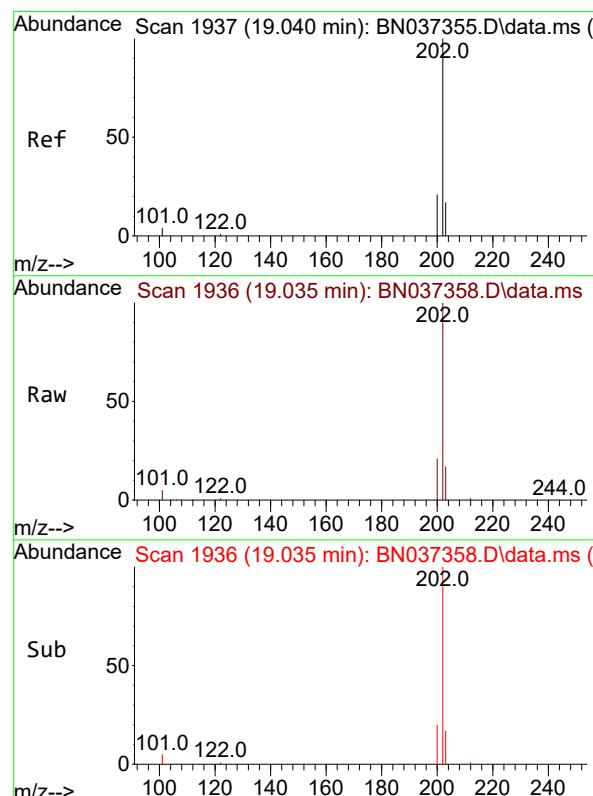

#28  
 Fluoranthene  
 Concen: 3.129 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion:202 Resp: 94745  
 Ion Ratio Lower Upper  
 202 100  
 101 5.9 3.0 4.6#  
 203 17.0 13.7 20.5





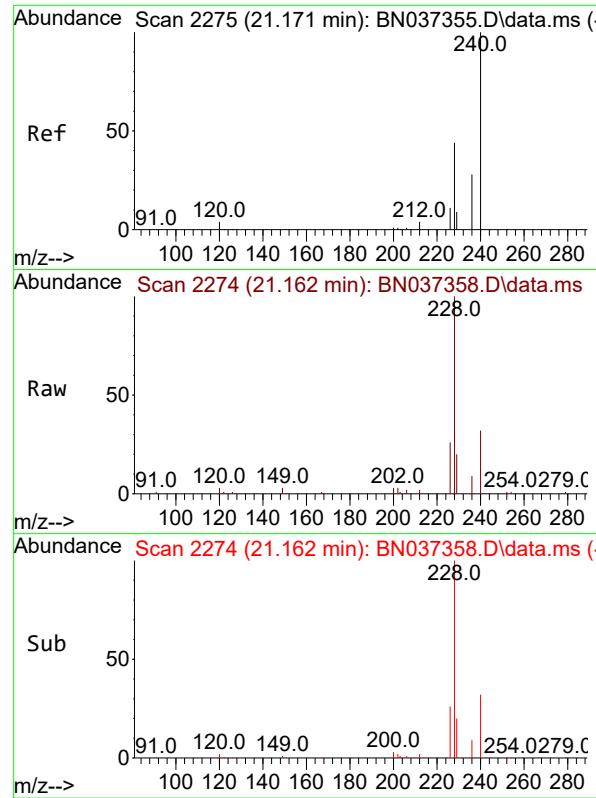

#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.162 min Scan# 2  
Delta R.T. -0.009 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:240 Resp: 7155  
Ion Ratio Lower Upper  
240 100  
120 8.3 7.5 11.3  
236 29.3 24.9 37.3

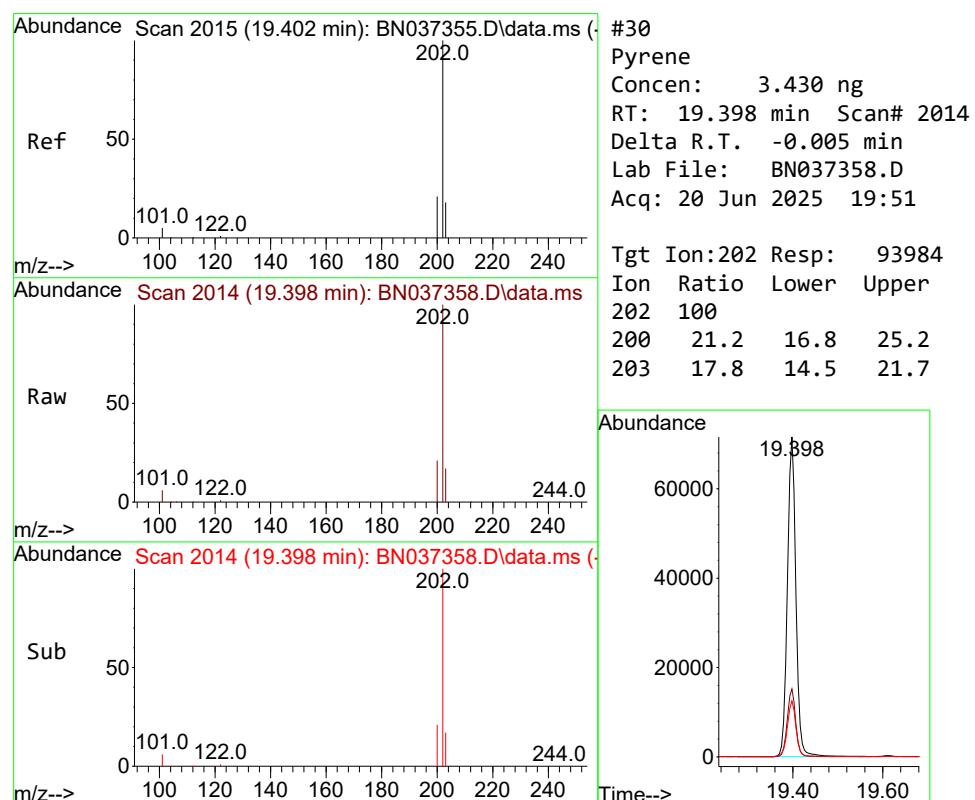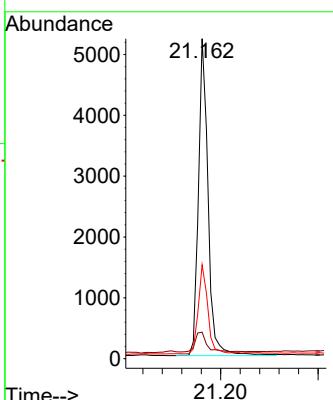

#30  
Pyrene  
Concen: 3.430 ng  
RT: 19.398 min Scan# 2014  
Delta R.T. -0.005 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51

Tgt Ion:202 Resp: 93984  
Ion Ratio Lower Upper  
202 100  
200 21.2 16.8 25.2  
203 17.8 14.5 21.7





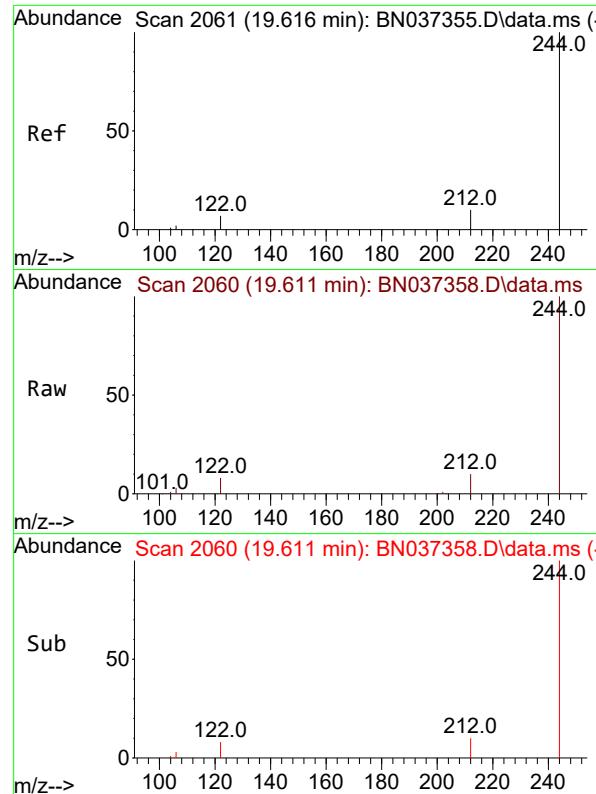

#31  
 Terphenyl-d14  
 Concen: 3.277 ng  
 RT: 19.611 min Scan# 2  
 Delta R.T. -0.005 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:244 Resp: 53536  
 Ion Ratio Lower Upper  
 244 100  
 212 10.0 11.1 16.7#  
 122 7.7 7.2 10.8

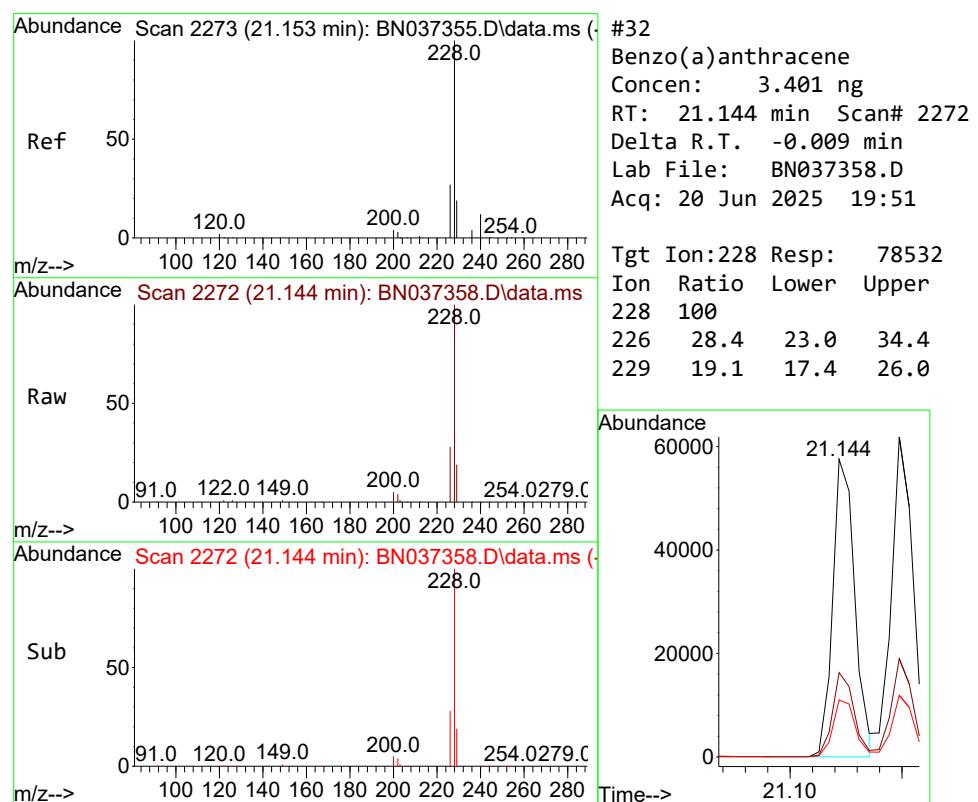

#32  
 Benzo(a)anthracene  
 Concen: 3.401 ng  
 RT: 21.144 min Scan# 2272  
 Delta R.T. -0.009 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion:228 Resp: 78532  
 Ion Ratio Lower Upper  
 228 100  
 226 28.4 23.0 34.4  
 229 19.1 17.4 26.0





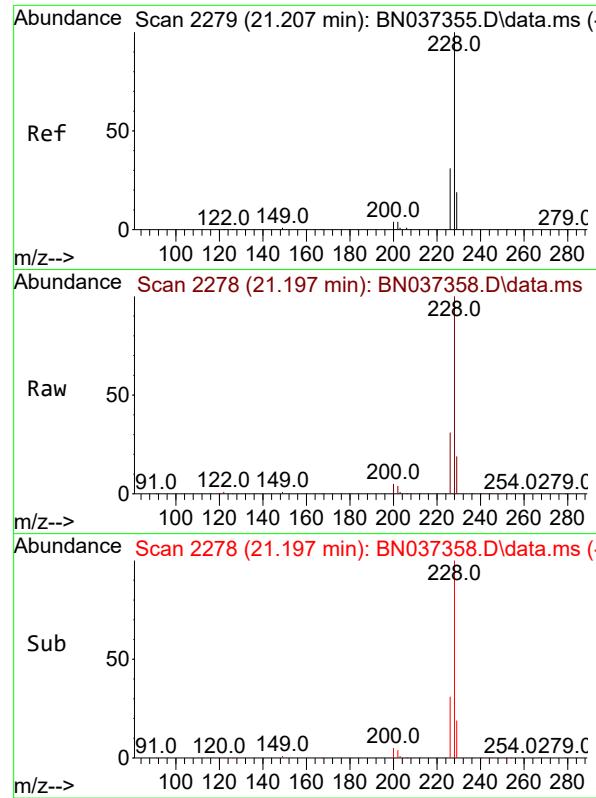

#33  
 Chrysene  
 Concen: 2.987 ng  
 RT: 21.197 min Scan# 2  
 Delta R.T. -0.009 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:228 Resp: 87474  
 Ion Ratio Lower Upper  
 228 100  
 226 30.7 25.4 38.2  
 229 19.3 17.3 25.9

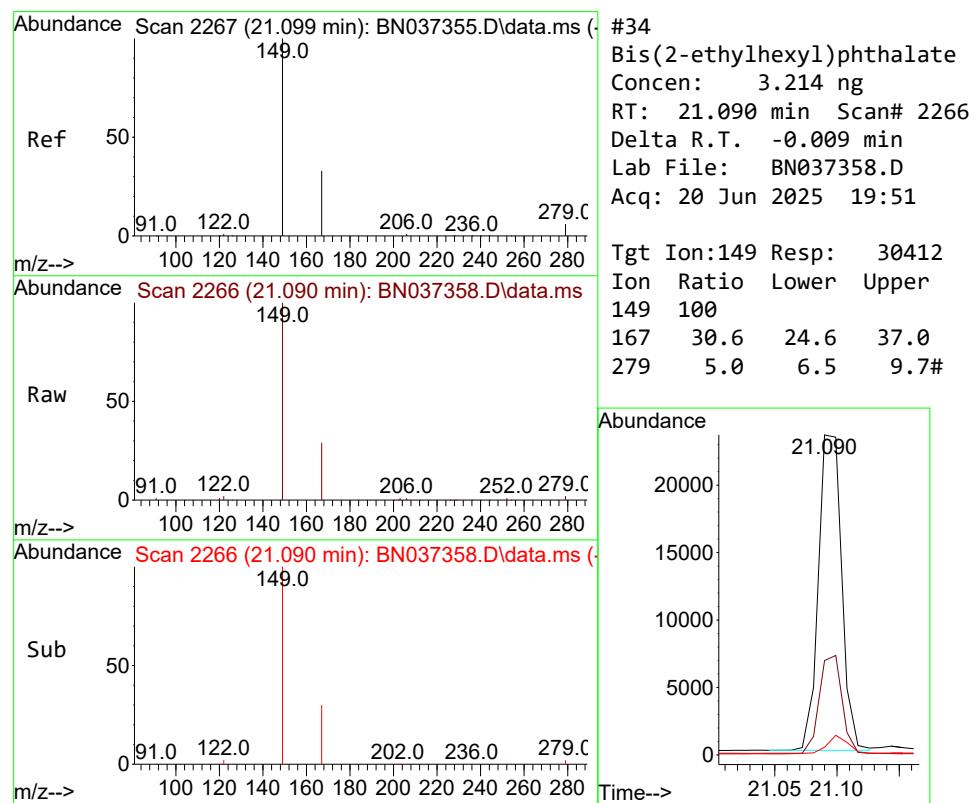

#34  
 Bis(2-ethylhexyl)phthalate  
 Concen: 3.214 ng  
 RT: 21.090 min Scan# 2266  
 Delta R.T. -0.009 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion:149 Resp: 30412  
 Ion Ratio Lower Upper  
 149 100  
 167 30.6 24.6 37.0  
 279 5.0 6.5 9.7#





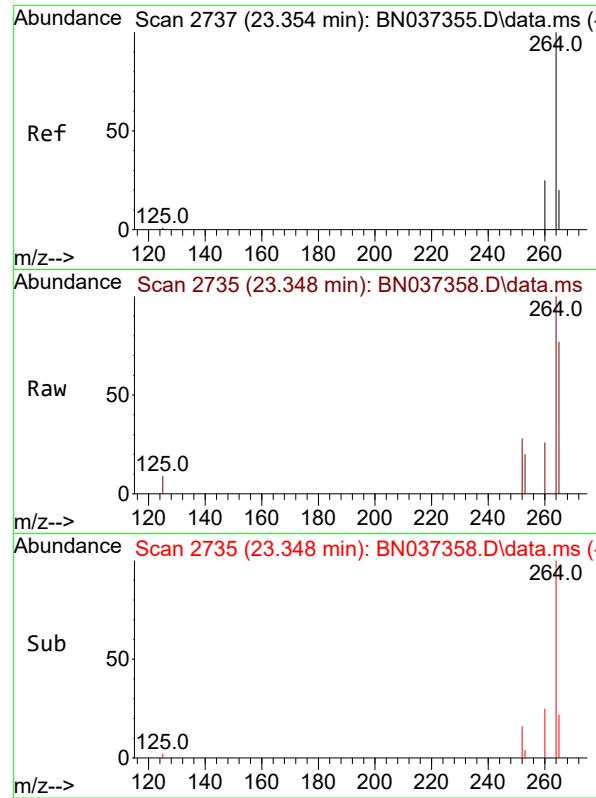

#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.348 min Scan# 2  
Delta R.T. -0.006 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:264 Resp: 6736  
Ion Ratio Lower Upper  
264 100  
260 26.2 21.4 32.2  
265 77.3 71.4 107.0

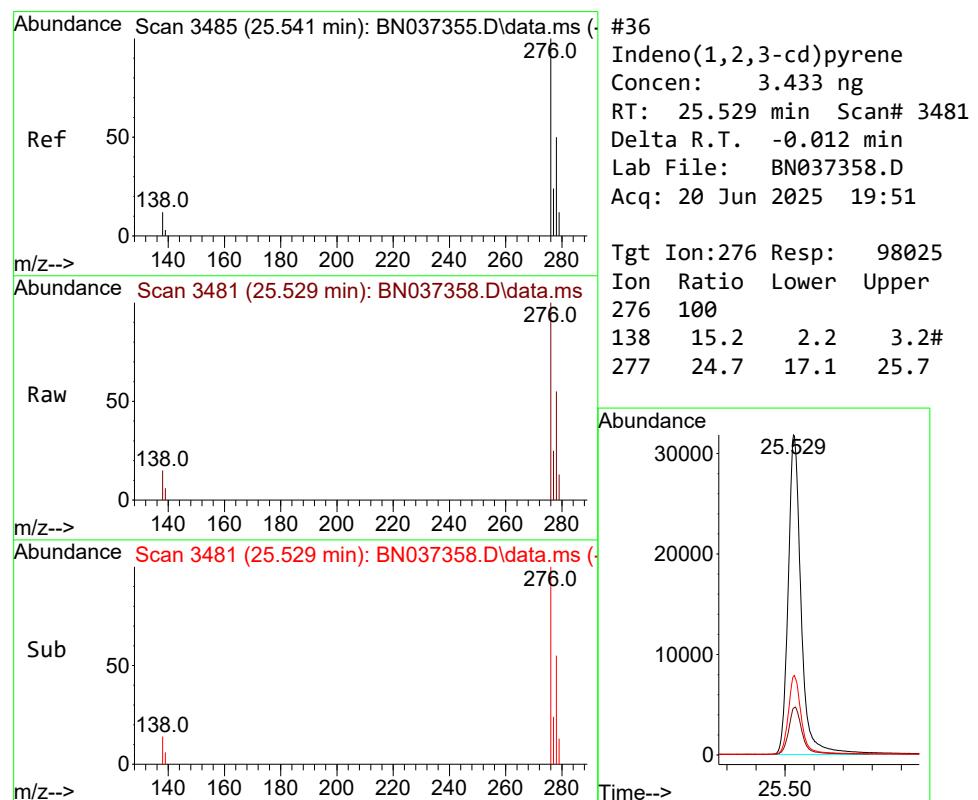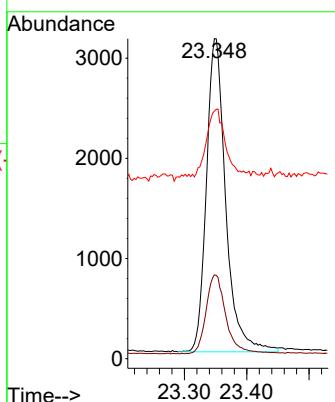

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 3.433 ng  
RT: 25.529 min Scan# 3481  
Delta R.T. -0.012 min  
Lab File: BN037358.D  
Acq: 20 Jun 2025 19:51

Tgt Ion:276 Resp: 98025  
Ion Ratio Lower Upper  
276 100  
138 15.2 2.2 3.2#  
277 24.7 17.1 25.7



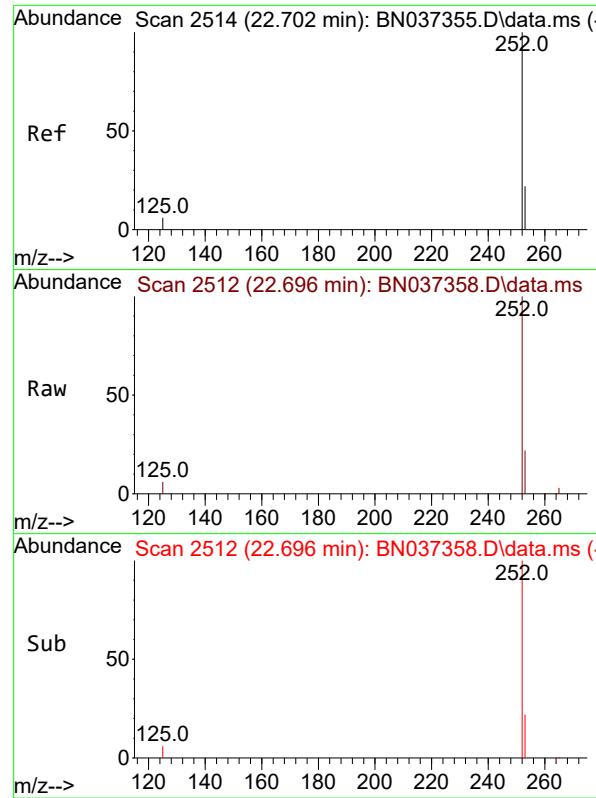

#37

Benzo(b)fluoranthene

Concen: 3.456 ng

RT: 22.696 min Scan# 2

Instrument :

BNA\_N

Delta R.T. -0.006 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51

ClientSampleId :

SSTDICC3.2


Tgt Ion:252 Resp: 82568

Ion Ratio Lower Upper

252 100

253 22.4 26.6 40.0#

125 6.1 6.1 9.1

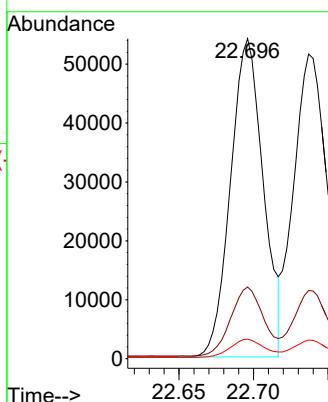

#38

Benzo(k)fluoranthene

Concen: 3.359 ng

RT: 22.737 min Scan# 2526

Delta R.T. -0.009 min

Lab File: BN037358.D

Acq: 20 Jun 2025 19:51


Tgt Ion:252 Resp: 87144


Ion Ratio Lower Upper

252 100

253 22.4 26.7 40.1#

125 6.1 6.5 9.7#


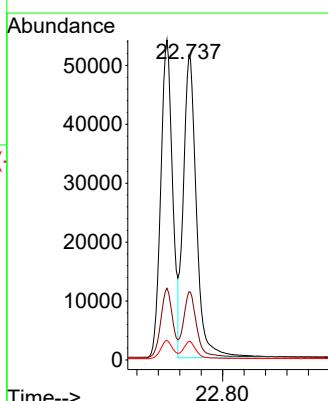


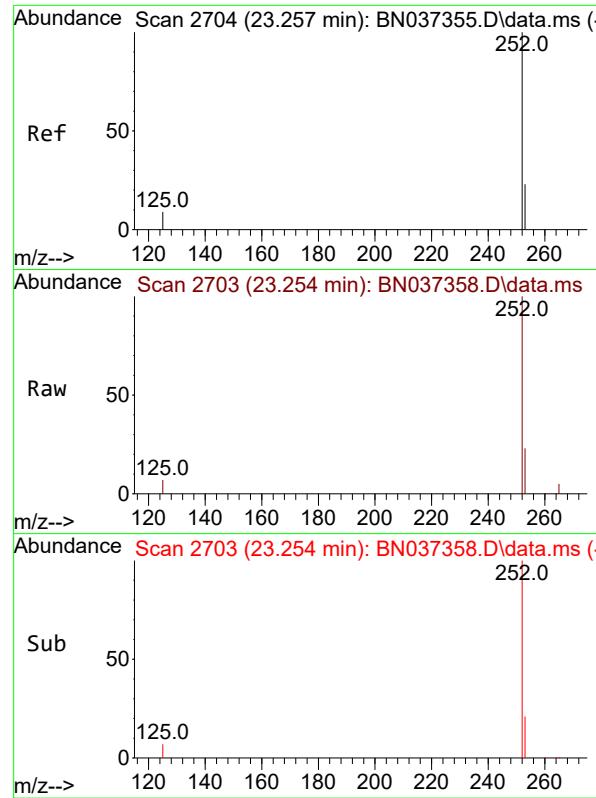

#39  
 Benzo(a)pyrene  
 Concen: 3.323 ng  
 RT: 23.254 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:252 Resp: 72643  
 Ion Ratio Lower Upper  
 252 100  
 253 22.7 31.6 47.4#  
 125 7.2 8.4 12.6#

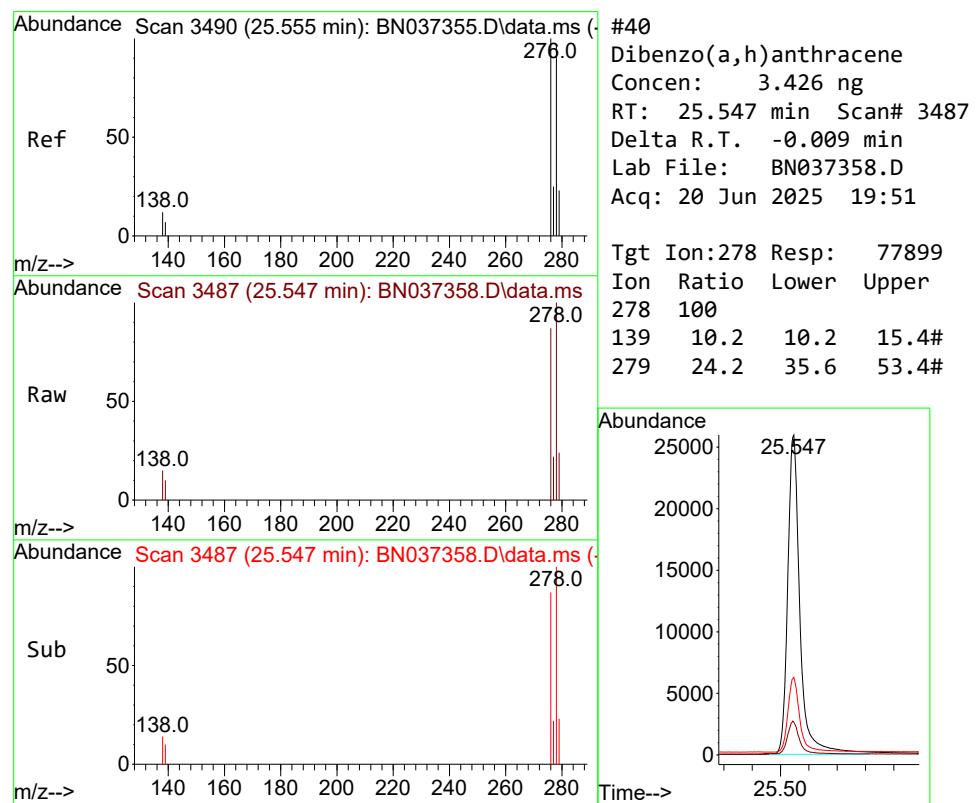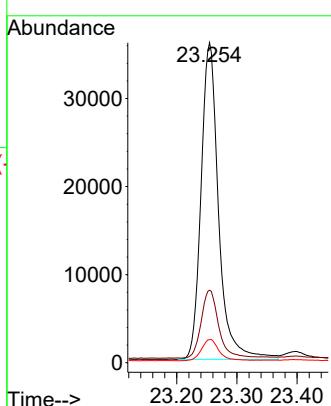

#40  
 Dibenzo(a,h)anthracene  
 Concen: 3.426 ng  
 RT: 25.547 min Scan# 3487  
 Delta R.T. -0.009 min  
 Lab File: BN037358.D  
 Acq: 20 Jun 2025 19:51

Tgt Ion:278 Resp: 77899  
 Ion Ratio Lower Upper  
 278 100  
 139 10.2 10.2 15.4#  
 279 24.2 35.6 53.4#

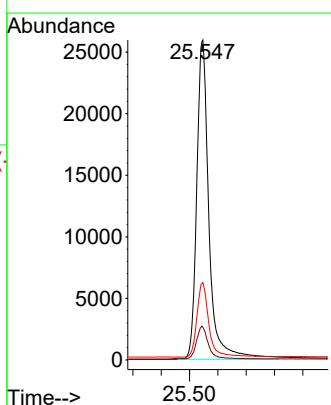

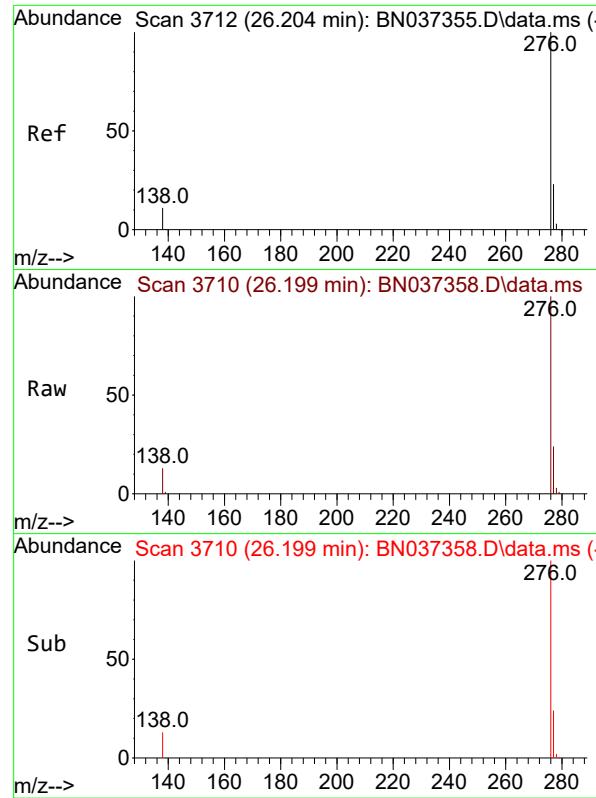

#41

Benzo(g,h,i)perylene

Concen: 3.239 ng

RT: 26.199 min Scan# 3

Instrument :

BNA\_N

Delta R.T. -0.006 min

Lab File: BN037358.D

ClientSampleId :

Acq: 20 Jun 2025 19:51

SSTDICC3.2


Tgt Ion:276 Resp: 84957

Ion Ratio Lower Upper

276 100

277 23.8 22.7 34.1

138 13.3 9.4 14.2



Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037359.D  
 Acq On : 20 Jun 2025 20:27  
 Operator : RC/JU  
 Sample : SSTDICC5.0  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC5.0

Quant Time: Jun 20 23:28:21 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	3043	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	6418	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	4465	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	9254	0.400	ng	#-0.01
29) Chrysene-d12	21.162	240	8543	0.400	ng	0.00
35) Perylene-d12	23.354	264	7704	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	29312	5.270	ng	0.00
5) Phenol-d6	6.744	99	34073	6.190	ng	0.00
8) Nitrobenzene-d5	8.707	82	28934	5.432	ng	-0.01
11) 2-Methylnaphthalene-d10	11.940	152	54112	5.210	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	13707	4.292	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	99254	5.067	ng	0.00
27) Fluoranthene-d10	19.003	212	133941	4.649	ng	0.00
31) Terphenyl-d14	19.611	244	98354	5.042	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.097	88	13159	4.896	ng	90
3) n-Nitrosodimethylamine	3.408	42	12840	4.103	ng	# 68
6) bis(2-Chloroethyl)ether	6.997	93	30083	6.246	ng	97
9) Naphthalene	10.394	128	85311	5.128	ng	# 86
10) Hexachlorobutadiene	10.682	225	30147	3.708	ng	# 99
12) 2-Methylnaphthalene	12.011	142	63177	5.400	ng	# 91
16) Acenaphthylene	13.935	152	99681	5.319	ng	98
17) Acenaphthene	14.277	154	64734	5.211	ng	98
18) Fluorene	15.271	166	92629	5.260	ng	99
20) 4,6-Dinitro-2-methylph...	15.357	198	13168	4.707	ng	# 44
21) 4-Bromophenyl-phenylether	16.165	248	34583	4.578	ng	94
22) Hexachlorobenzene	16.276	284	33797	4.288	ng	98
23) Atrazine	16.438	200	27492	4.648	ng	# 81
24) Pentachlorophenol	16.624	266	19702	4.555	ng	97
25) Phenanthrene	17.009	178	141308	5.404	ng	99
26) Anthracene	17.095	178	135503	5.549	ng	99
28) Fluoranthene	19.035	202	175639	4.910	ng	# 98
30) Pyrene	19.398	202	175487	5.364	ng	99
32) Benzo(a)anthracene	21.153	228	152551	5.534	ng	97
33) Chrysene	21.206	228	159633	4.566	ng	96
34) Bis(2-ethylhexyl)phtha...	21.099	149	59151	5.235	ng	# 97
36) Indeno(1,2,3-cd)pyrene	25.535	276	178739	5.473	ng	# 89
37) Benzo(b)fluoranthene	22.699	252	152855	5.595	ng	# 83
38) Benzo(k)fluoranthene	22.740	252	162397	5.473	ng	# 83
39) Benzo(a)pyrene	23.254	252	134379	5.375	ng	# 76
40) Dibenzo(a,h)anthracene	25.549	278	142364	5.474	ng	# 74
41) Benzo(g,h,i)perylene	26.199	276	153920	5.131	ng	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037359.D  
 Acq On : 20 Jun 2025 20:27  
 Operator : RC/JU  
 Sample : SSTDICC5.0  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC5.0


Quant Time: Jun 20 23:28:21 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration

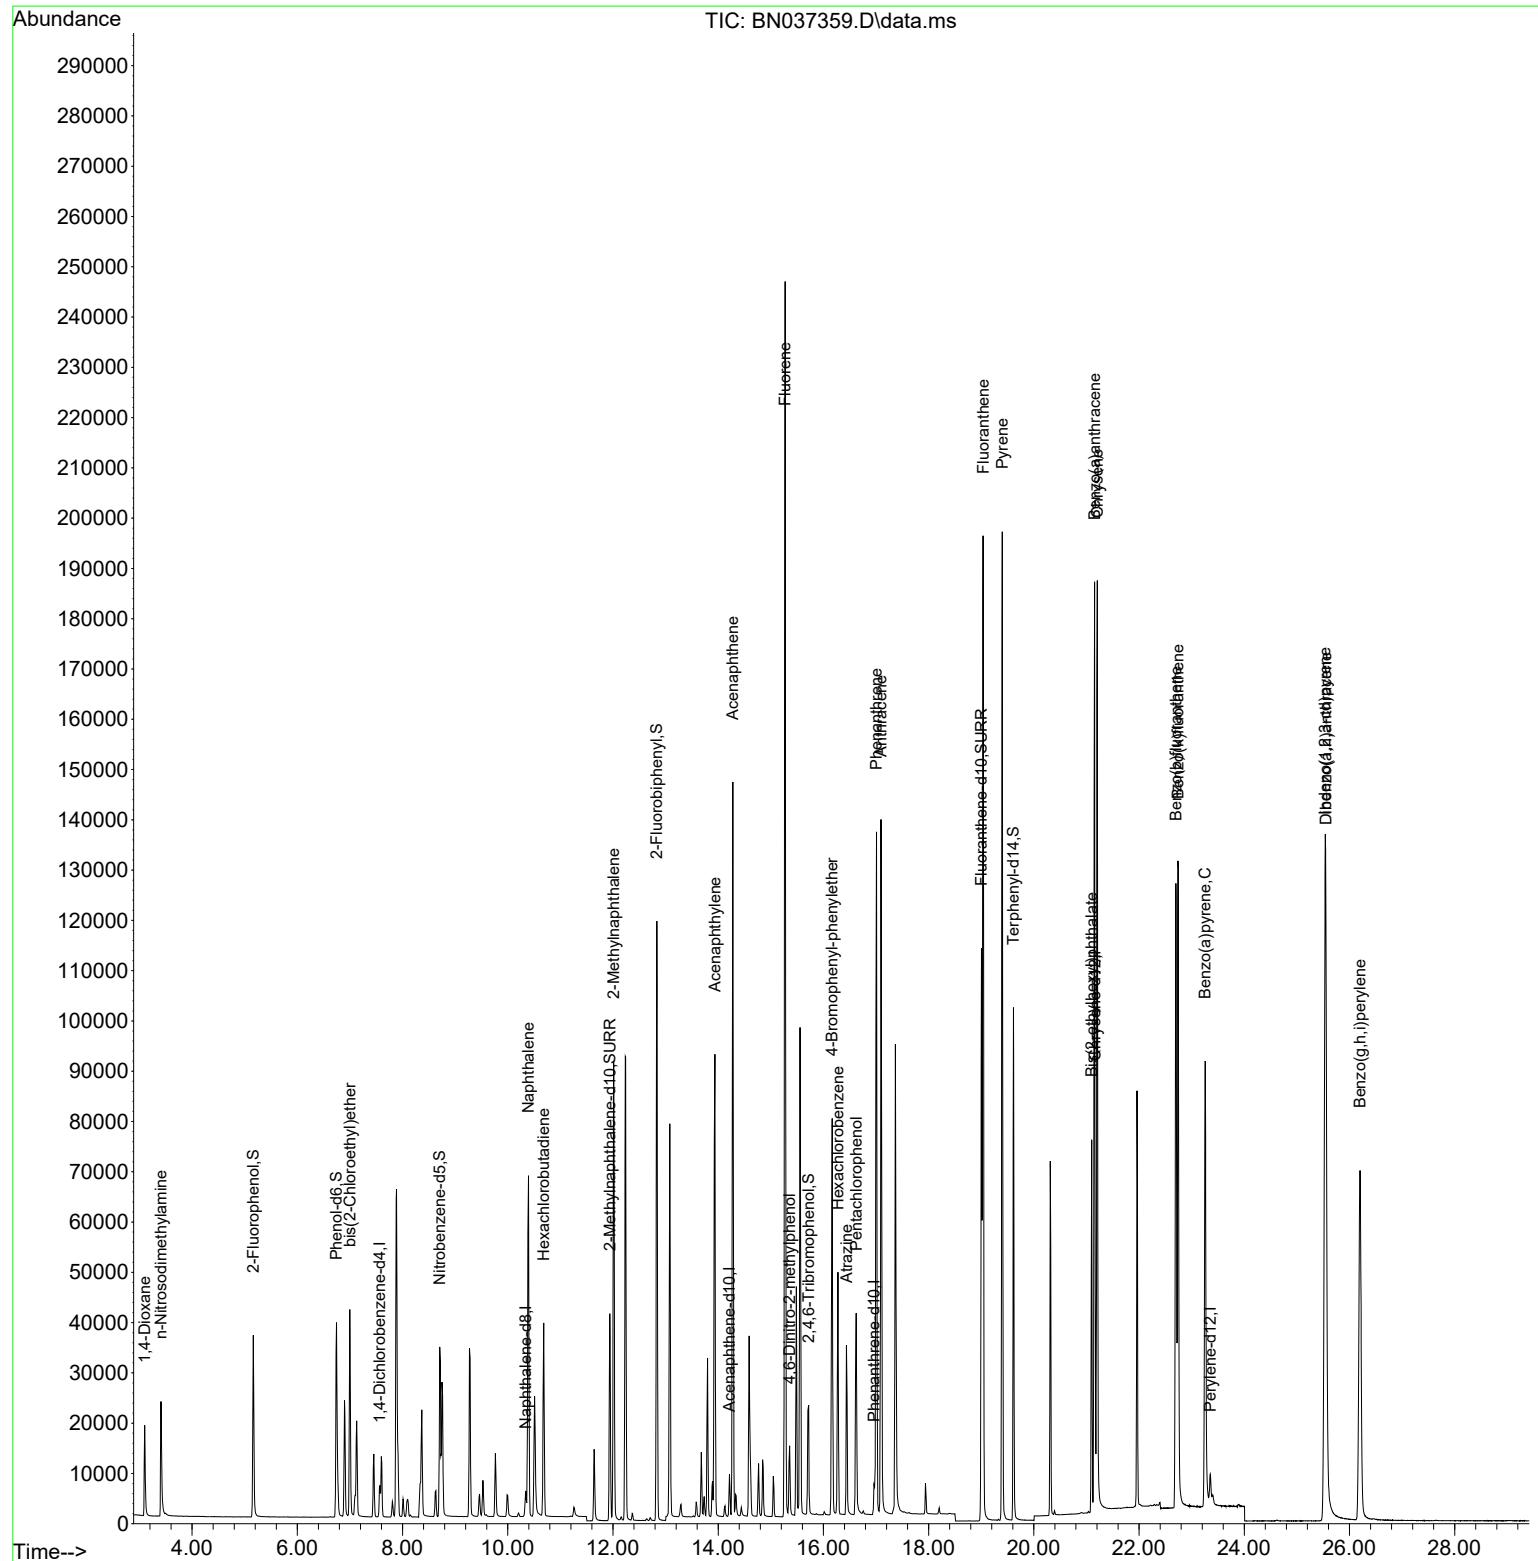






#1  
 1,4-Dichlorobenzene-d4  
 Concen: 0.400 ng  
 RT: 7.568 min Scan# 6  
 Delta R.T. -0.000 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0





Tgt Ion:152 Resp: 3043  
 Ion Ratio Lower Upper  
 152 100  
 150 149.8 112.7 169.1  
 115 53.3 45.9 68.9

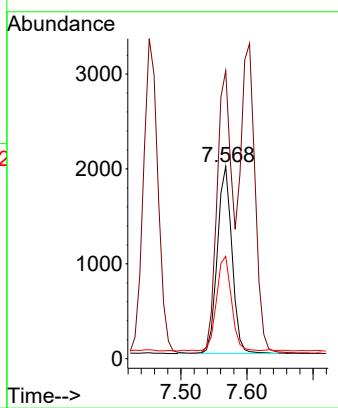
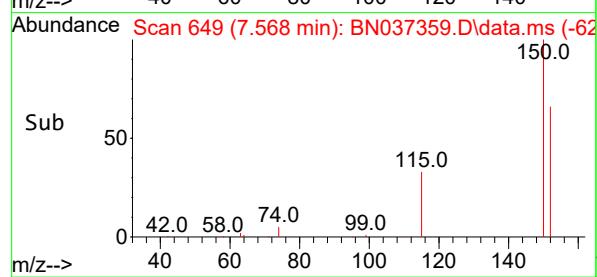




#2  
 1,4-Dioxane  
 Concen: 4.896 ng  
 RT: 3.097 min Scan# 30  
 Delta R.T. -0.007 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27



Tgt Ion: 88 Resp: 13159  
 Ion Ratio Lower Upper  
 88 100  
 43 22.8 21.0 31.6  
 58 55.2 38.0 57.0

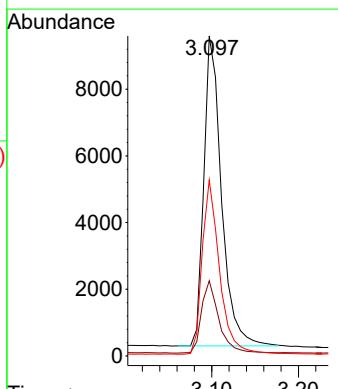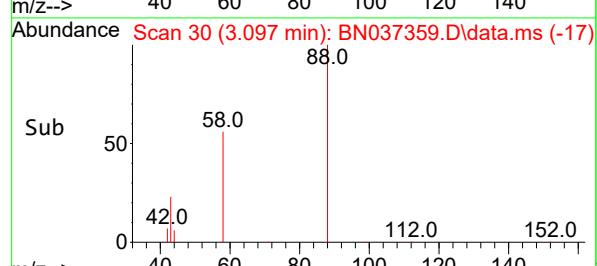

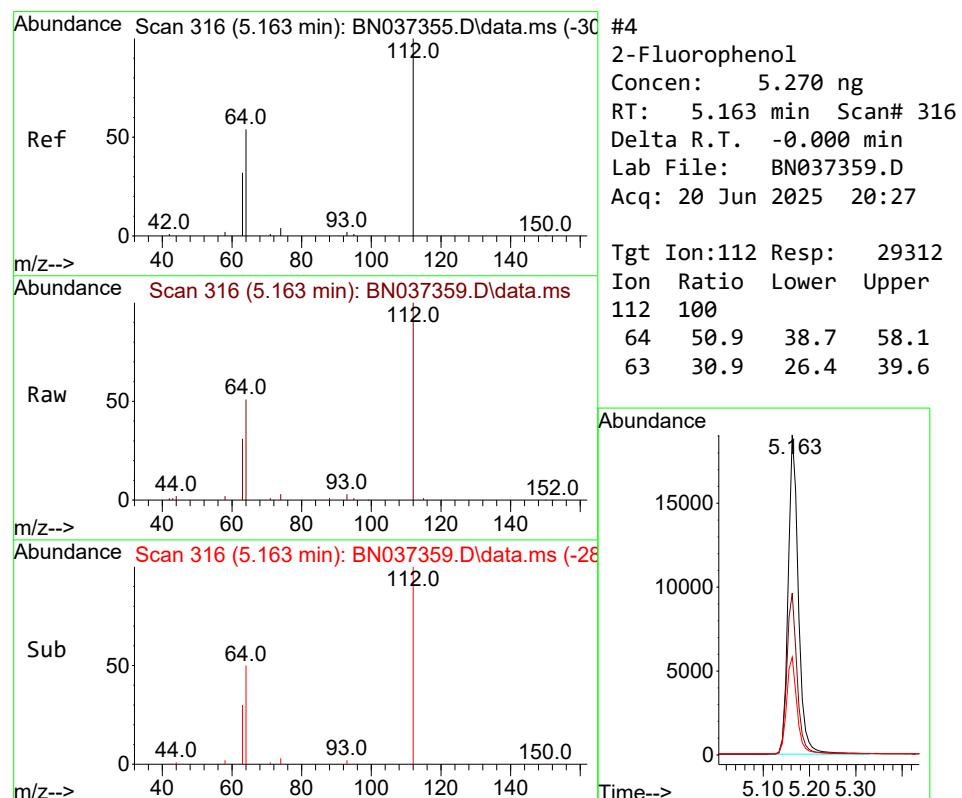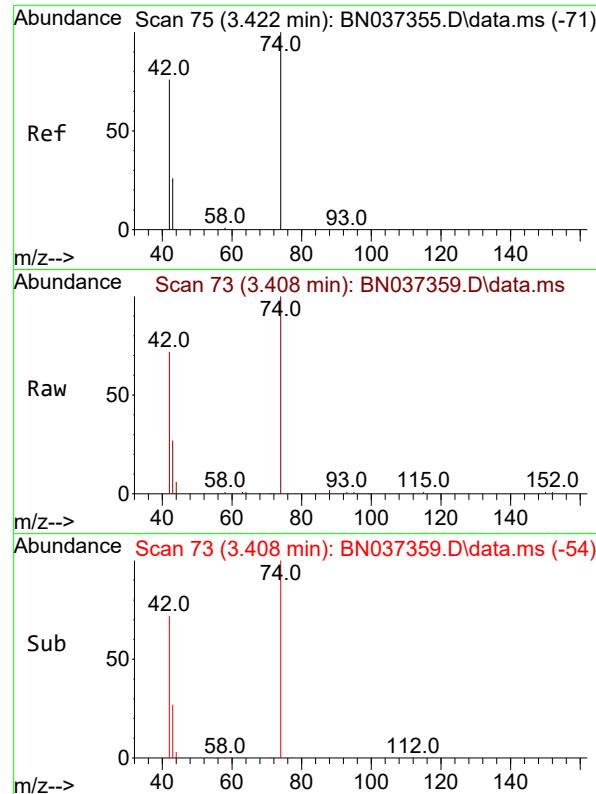


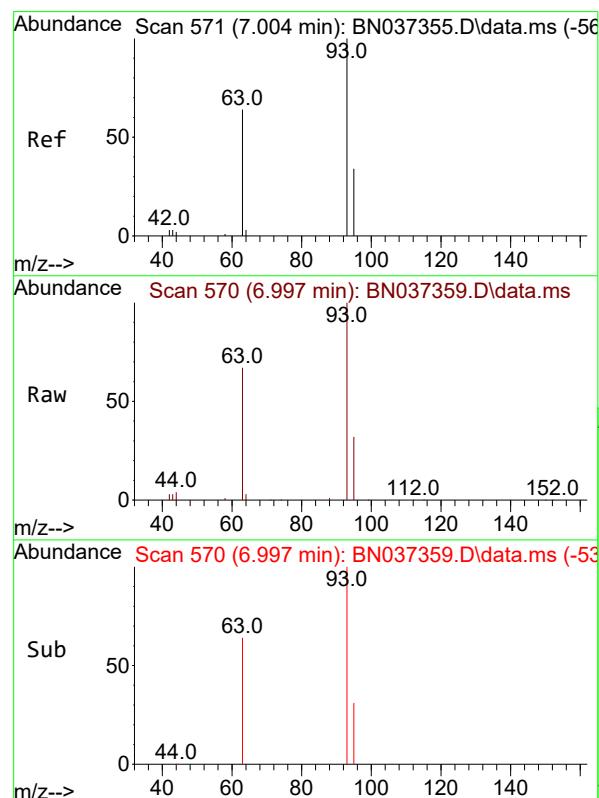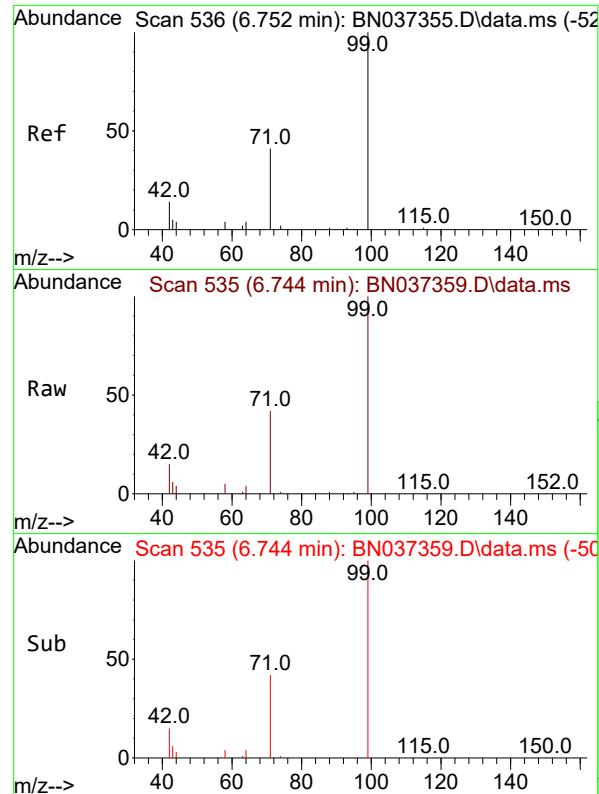

#5  
Phenol-d6  
Concen: 6.190 ng  
RT: 6.744 min Scan# 5  
Delta R.T. -0.007 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0


Tgt Ion: 99 Resp: 34073  
Ion Ratio Lower Upper  
99 100  
42 17.4 19.8 29.8#  
71 42.6 42.6 64.0#



#6  
bis(2-Chloroethyl)ether  
Concen: 6.246 ng  
RT: 6.997 min Scan# 570  
Delta R.T. -0.007 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Tgt Ion: 93 Resp: 30083  
Ion Ratio Lower Upper  
93 100  
63 64.8 53.2 79.8  
95 31.7 27.3 40.9







#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0

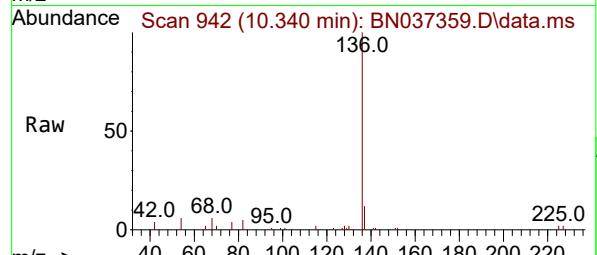



Tgt Ion:136 Resp: 6418  
 Ion Ratio Lower Upper  
 136 100  
 137 12.3 12.2 18.2  
 54 6.5 8.8 13.2#  
 68 5.7 7.0 10.4#


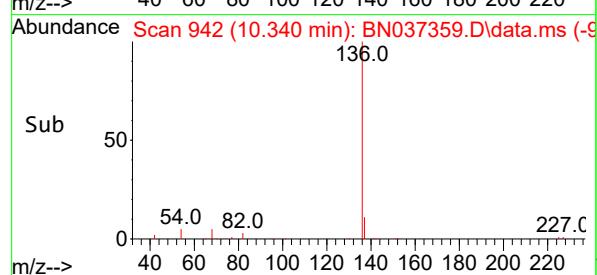
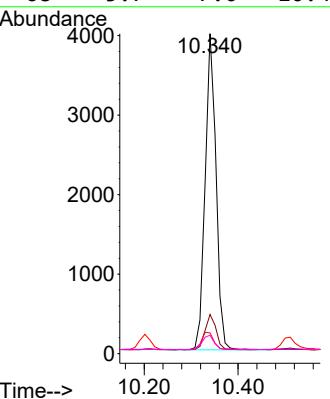


#8  
 Nitrobenzene-d5  
 Concen: 5.432 ng  
 RT: 8.707 min Scan# 789  
 Delta R.T. -0.011 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27

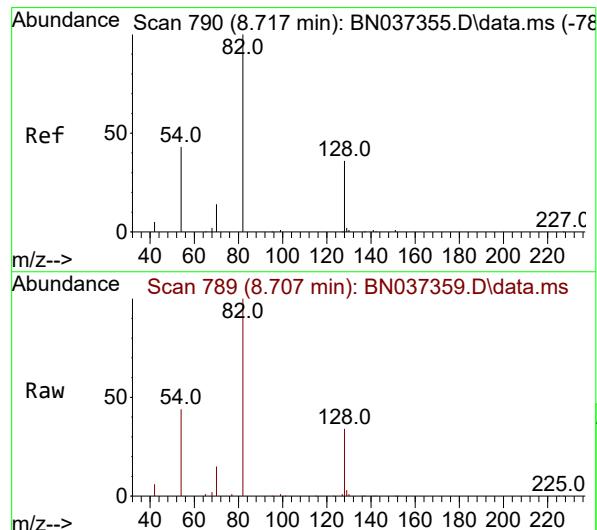

Tgt Ion: 82 Resp: 28934  
 Ion Ratio Lower Upper  
 82 100  
 128 34.1 42.5 63.7#  
 54 44.3 43.2 64.8

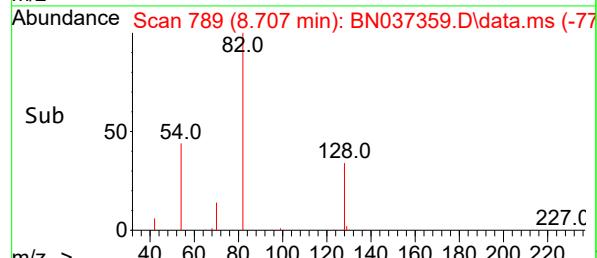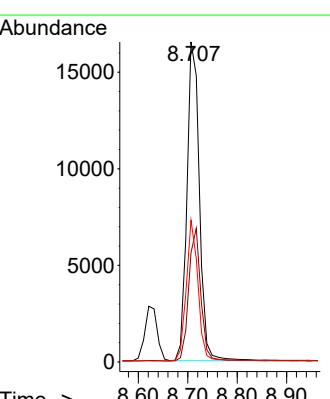



#9

Naphthalene

Concen: 5.128 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:128 Resp: 85311

Ion Ratio Lower Upper

128 100

129 11.0 14.0 21.0#

127 13.5 15.8 23.8#

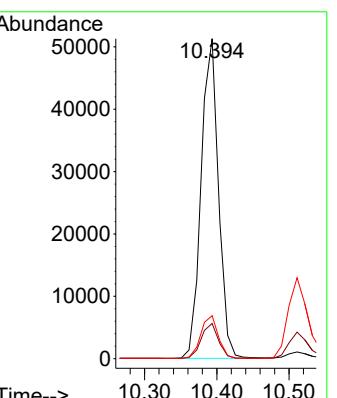

#10

Hexachlorobutadiene

Concen: 3.708 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27


Tgt Ion:225 Resp: 30147




Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0





227 63.4 50.3 75.5

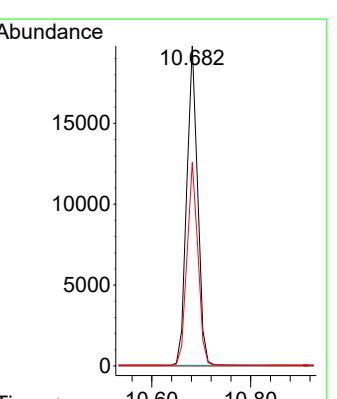




#11  
2-Methylnaphthalene-d10  
Concen: 5.210 ng  
RT: 11.940 min Scan# 1:Instrument :  
Delta R.T. -0.005 min BNA\_N  
Lab File: BN037359.D ClientSampleId :  
Acq: 20 Jun 2025 20:27 SSTDICC5.0


Tgt Ion:152 Resp: 54112  
Ion Ratio Lower Upper  
152 100  
151 21.2 17.4 26.0

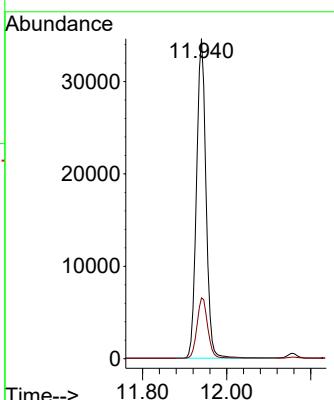

#12  
2-Methylnaphthalene  
Concen: 5.400 ng  
RT: 12.011 min Scan# 1151  
Delta R.T. -0.010 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27

Tgt Ion:142 Resp: 63177  
Ion Ratio Lower Upper  
142 100  
141 90.4 70.2 105.2  
115 40.0 43.0 64.4#

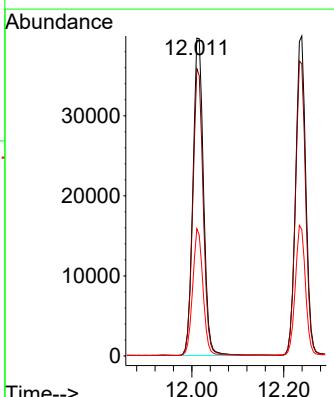

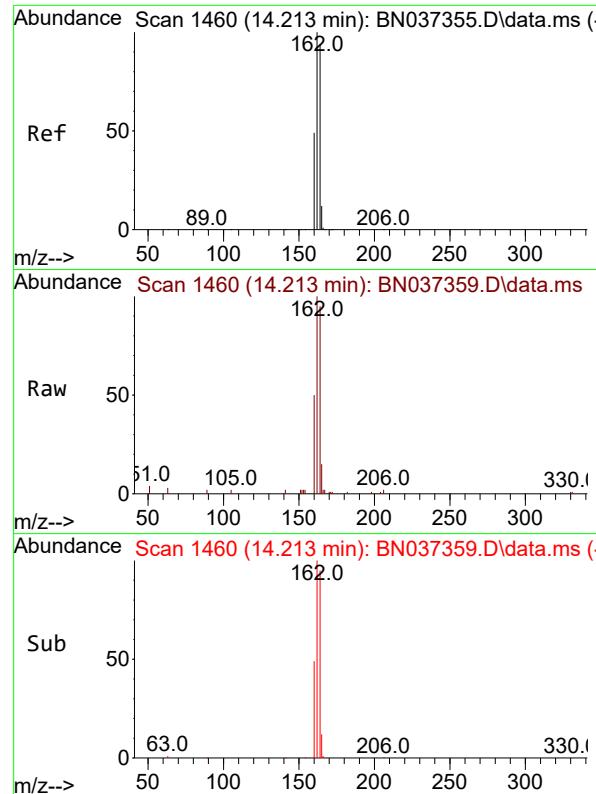

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1460

Delta R.T. -0.000 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0



Tgt Ion:164 Resp: 4465

Ion Ratio Lower Upper

164 100

162 105.2 81.5 122.3

160 52.3 43.0 64.4

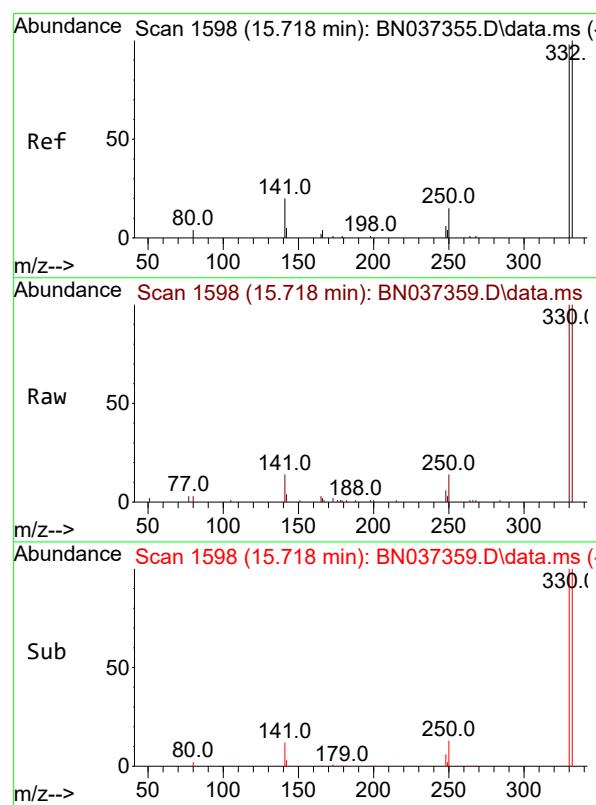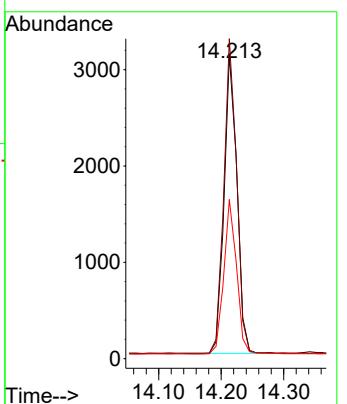

#14

2,4,6-Tribromophenol

Concen: 4.292 ng

RT: 15.718 min Scan# 1598

Delta R.T. -0.000 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27


Tgt Ion:330 Resp: 13707


Ion Ratio Lower Upper

330 100

332 96.8 78.4 117.6

141 36.8 24.4 36.6#


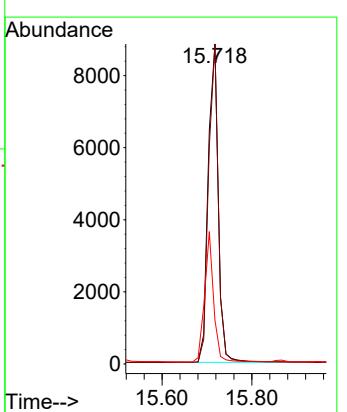


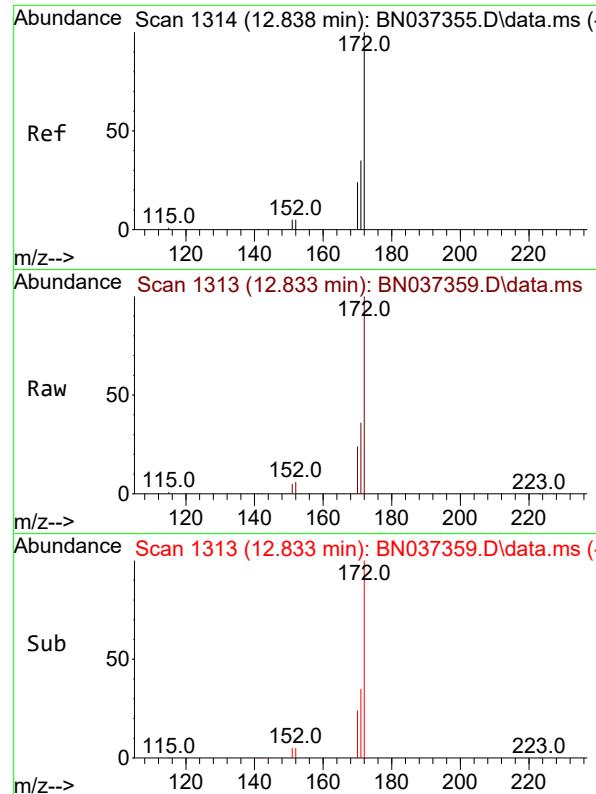

#15  
2-Fluorobiphenyl  
Concen: 5.067 ng  
RT: 12.833 min Scan# 1  
Delta R.T. -0.005 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0




Tgt Ion:172 Resp: 99254  
Ion Ratio Lower Upper  
172 100  
171 35.7 30.8 46.2  
170 23.6 21.9 32.9

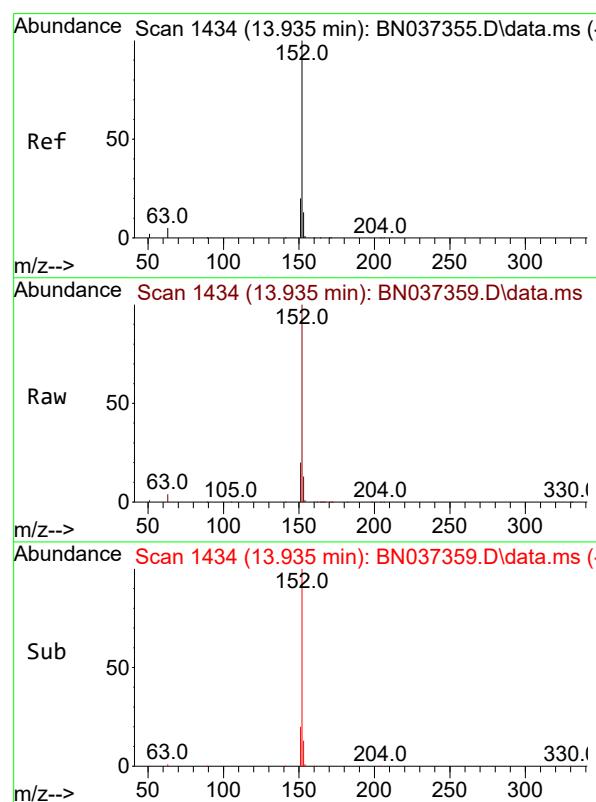

#16  
Acenaphthylene  
Concen: 5.319 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27

Tgt Ion:152 Resp: 99681  
Ion Ratio Lower Upper  
152 100  
151 19.8 16.6 24.8  
153 13.1 10.2 15.2

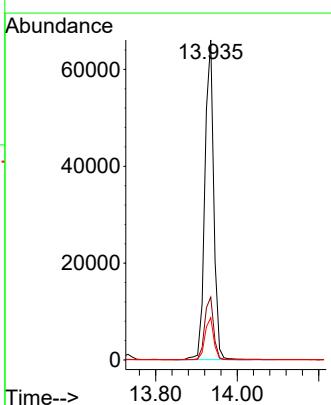



#17

Acenaphthene

Concen: 5.211 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:154 Resp: 64734

Ion Ratio Lower Upper

154 100

153 115.1 93.1 139.7

152 58.2 48.6 73.0



#18

Fluorene

Concen: 5.260 ng

RT: 15.271 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27


Tgt Ion:166 Resp: 92629


Ion Ratio Lower Upper

166 100

165 98.8 79.5 119.3

167 13.4 10.7 16.1

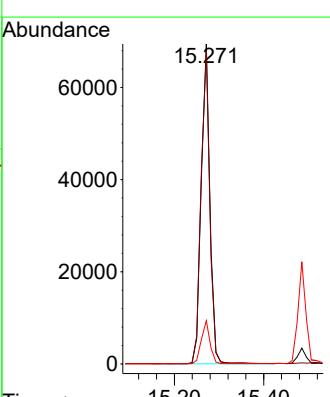

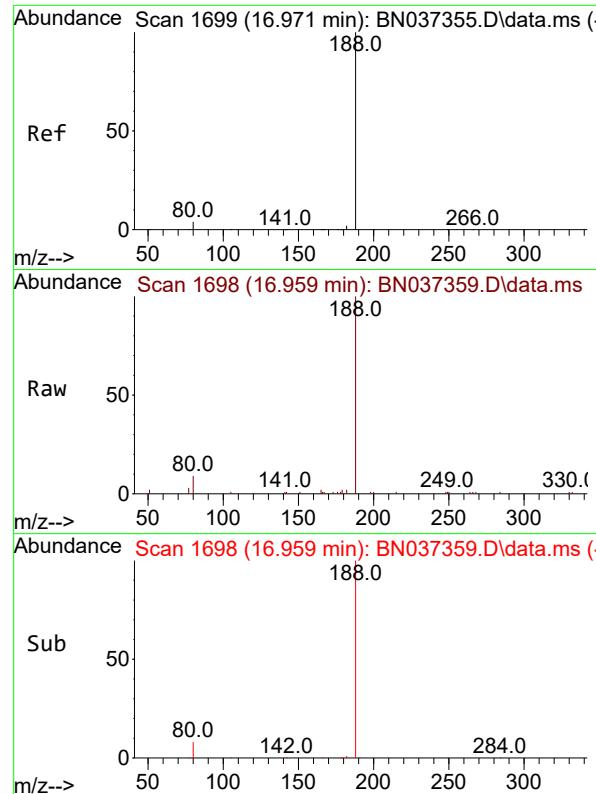

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.959 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0

Tgt Ion:188 Resp: 9254

Ion Ratio Lower Upper



188 100

94 0.0 0.0 0.0

80 9.3 6.2 9.2#

Abundance

16.959

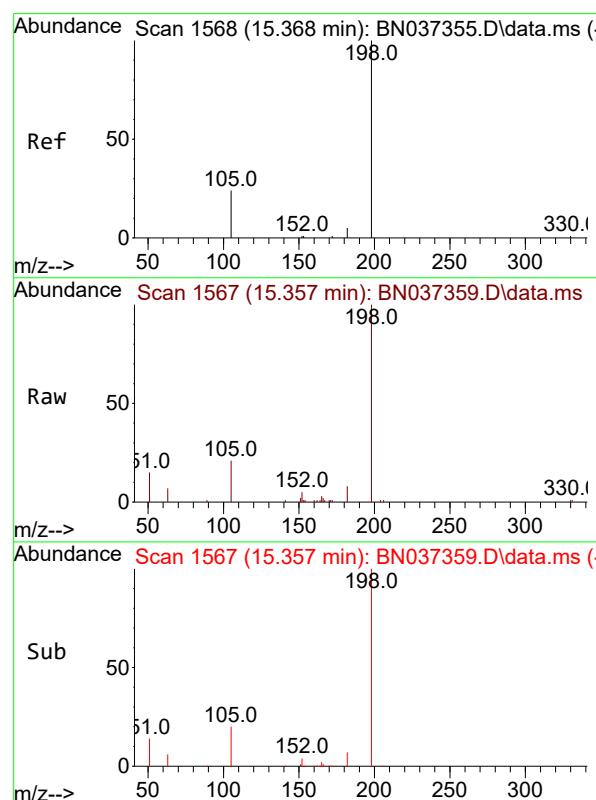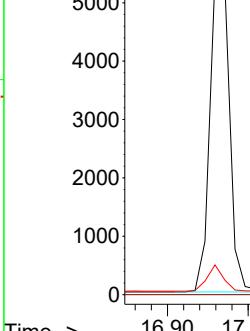

#20

4,6-Dinitro-2-methylphenol

Concen: 4.707 ng

RT: 15.357 min Scan# 1567

Delta R.T. -0.011 min

Lab File: BN037359.D

Acq: 20 Jun 2025 20:27

Tgt Ion:198 Resp: 13168


Ion Ratio Lower Upper


198 100

51 15.1 51.4 77.0#

105 20.6 45.5 68.3#

Abundance


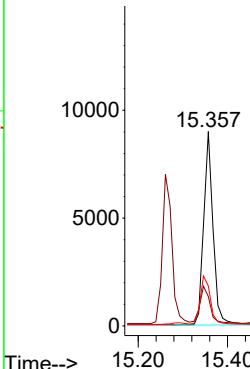


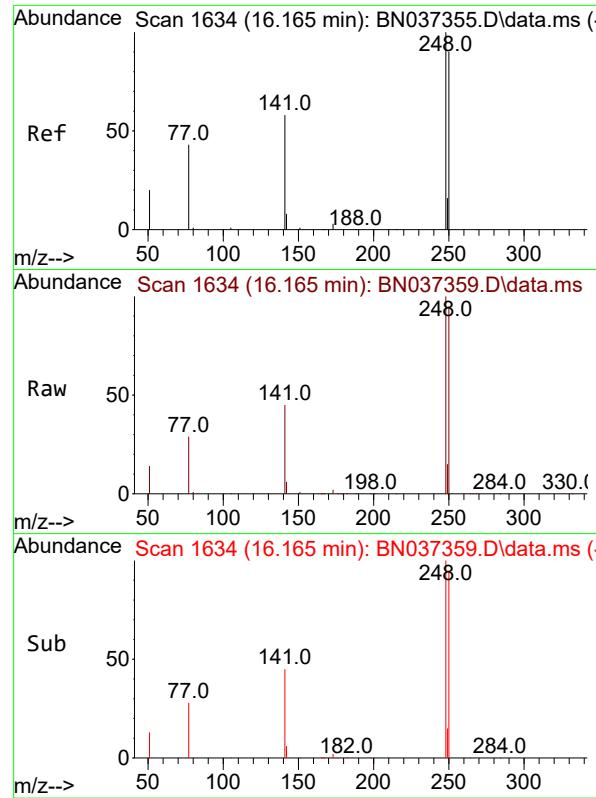

#21  
4-Bromophenyl-phenylether  
Concen: 4.578 ng  
RT: 16.165 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0


Tgt Ion:248 Resp: 34583  
Ion Ratio Lower Upper  
248 100  
250 94.8 80.4 120.6  
141 45.4 33.3 49.9

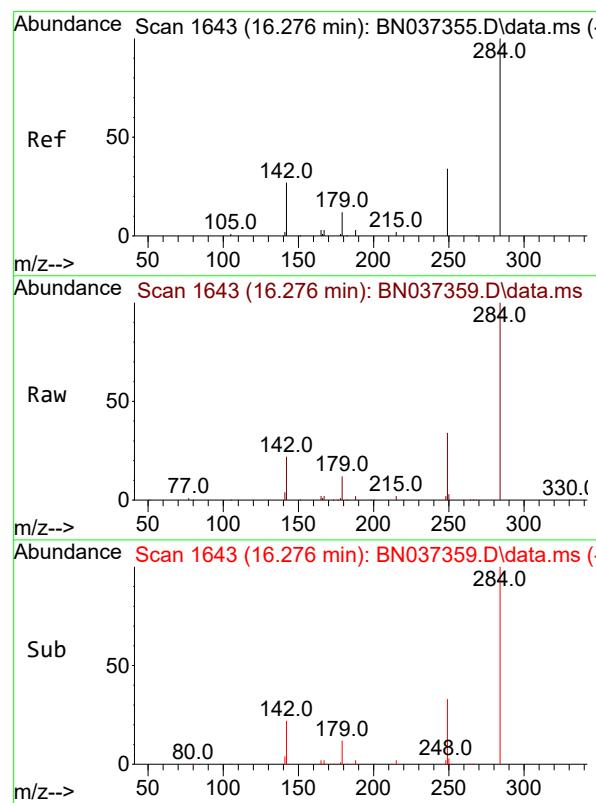

#22  
Hexachlorobenzene  
Concen: 4.288 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27

Tgt Ion:284 Resp: 33797  
Ion Ratio Lower Upper  
284 100  
142 34.2 27.0 40.6  
249 34.0 28.8 43.2





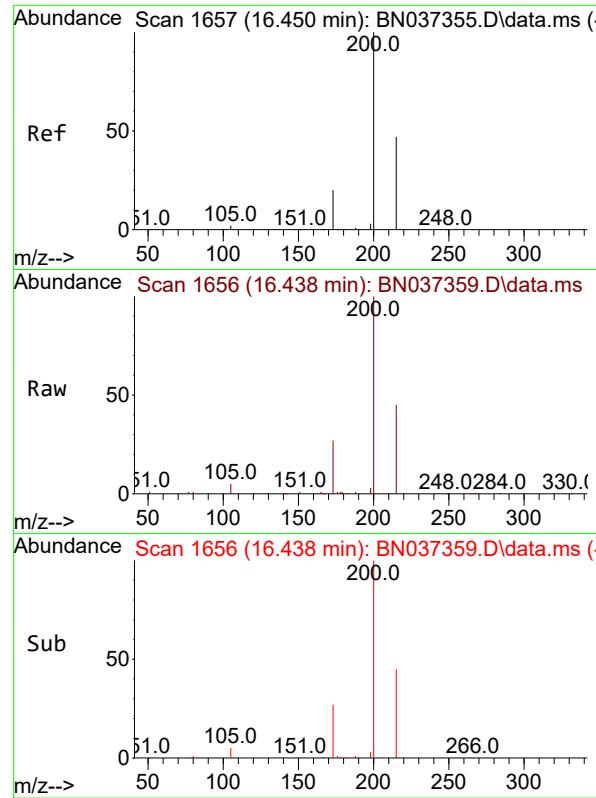

#23  
Atrazine  
Concen: 4.648 ng  
RT: 16.438 min Scan# 1  
Delta R.T. -0.012 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0



Tgt Ion:200 Resp: 27492  
Ion Ratio Lower Upper  
200 100  
173 27.4 29.2 43.8#  
215 45.1 48.8 73.2#

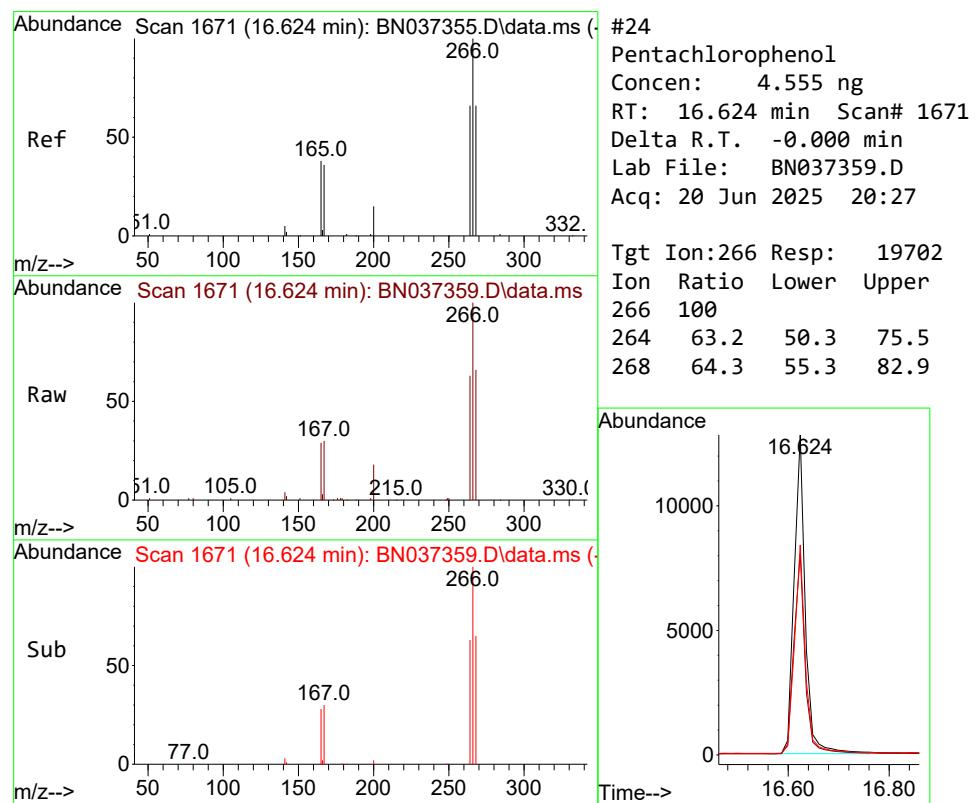

#24  
Pentachlorophenol  
Concen: 4.555 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Tgt Ion:266 Resp: 19702  
Ion Ratio Lower Upper  
266 100  
264 63.2 50.3 75.5  
268 64.3 55.3 82.9

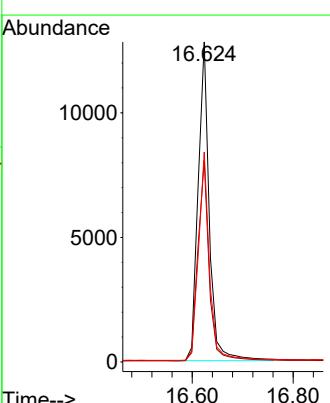

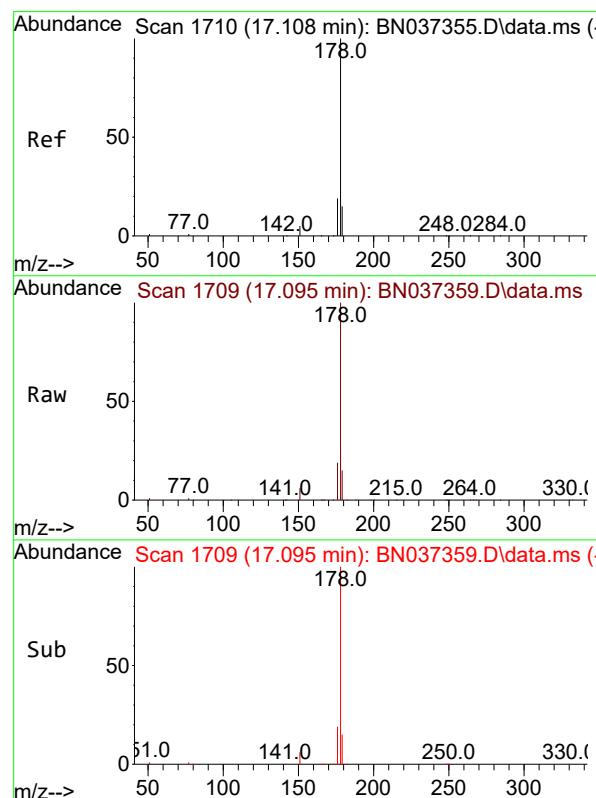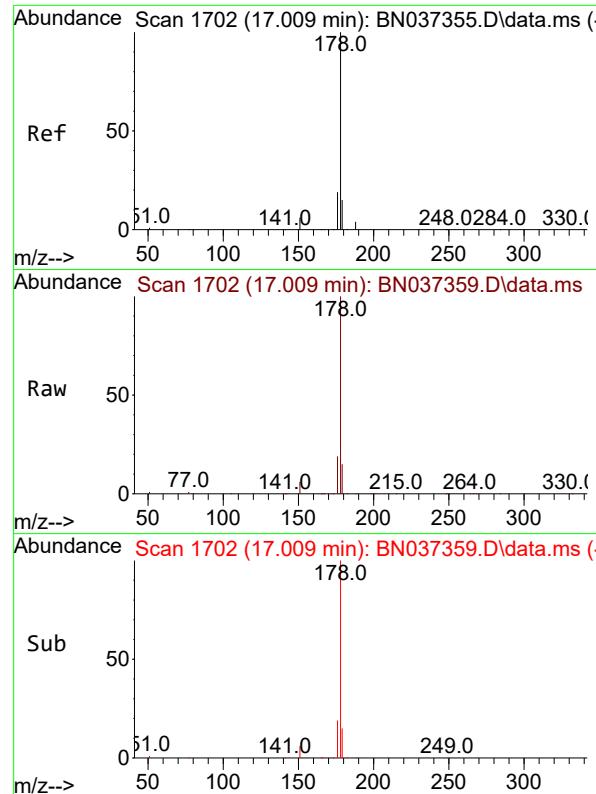


#25  
Phenanthrene  
Concen: 5.404 ng  
RT: 17.009 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27  
ClientSampleId : SSTDICC5.0


Tgt Ion:178 Resp: 141308  
Ion Ratio Lower Upper  
178 100  
176 19.2 15.2 22.8  
179 15.2 12.9 19.3



#26  
Anthracene  
Concen: 5.549 ng  
RT: 17.095 min Scan# 1709  
Delta R.T. -0.013 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27

Tgt Ion:178 Resp: 135503  
Ion Ratio Lower Upper  
178 100  
176 18.6 14.7 22.1  
179 15.4 13.0 19.6





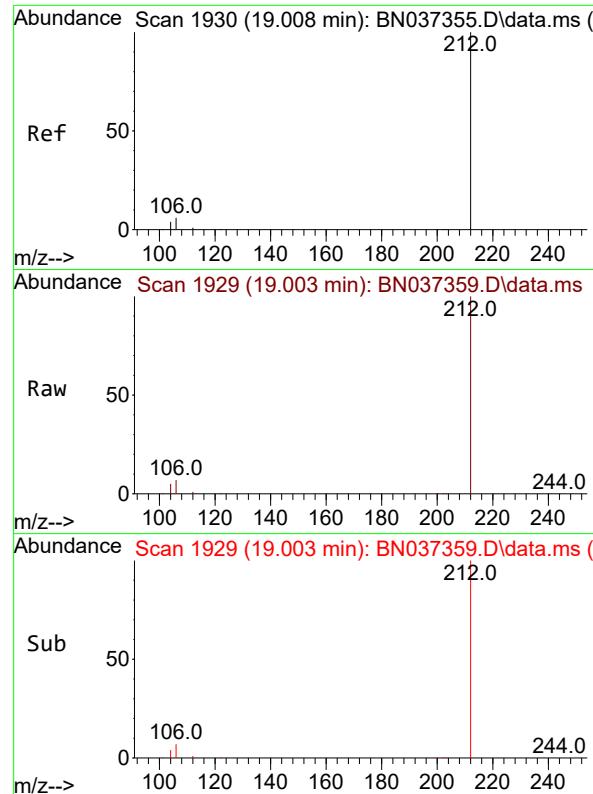

#27  
 Fluoranthene-d10  
 Concen: 4.649 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. -0.005 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0


Tgt Ion:212 Resp: 133941  
 Ion Ratio Lower Upper  
 212 100  
 106 7.3 3.0 4.4#  
 104 4.3 2.0 3.0#

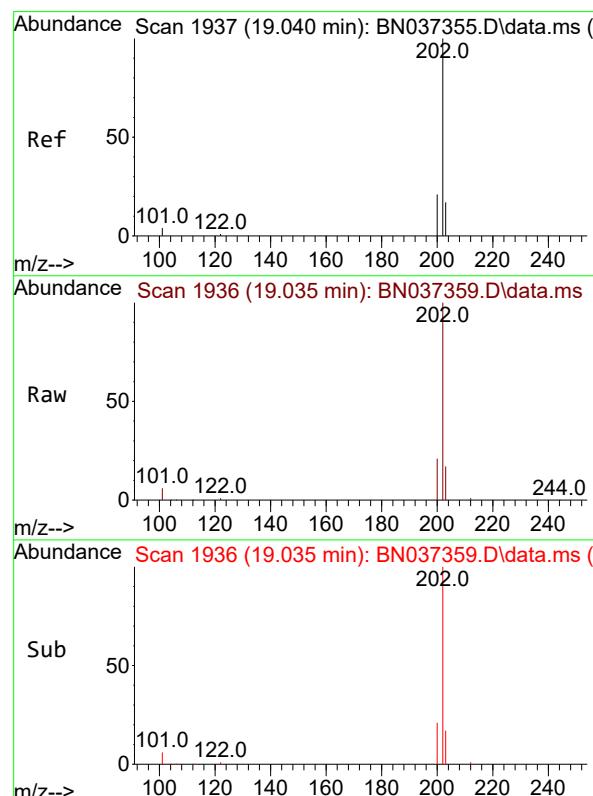

#28  
 Fluoranthene  
 Concen: 4.910 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27

Tgt Ion:202 Resp: 175639  
 Ion Ratio Lower Upper  
 202 100  
 101 6.2 3.0 4.6#  
 203 17.3 13.7 20.5


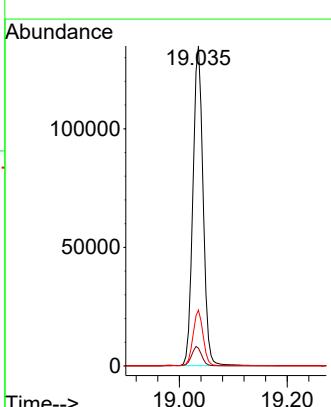


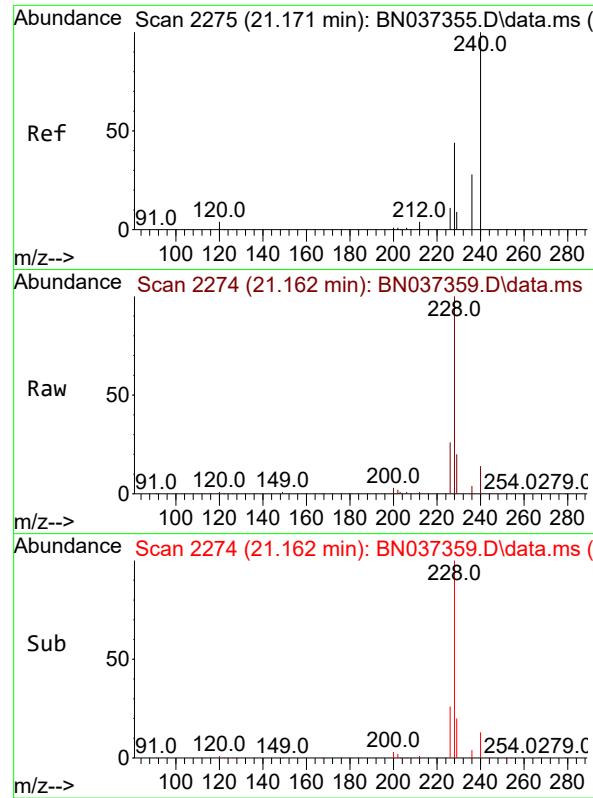

#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.162 min Scan# 2  
Delta R.T. -0.009 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0


Tgt Ion:240 Resp: 8543  
Ion Ratio Lower Upper  
240 100  
120 9.8 7.5 11.3  
236 29.1 24.9 37.3

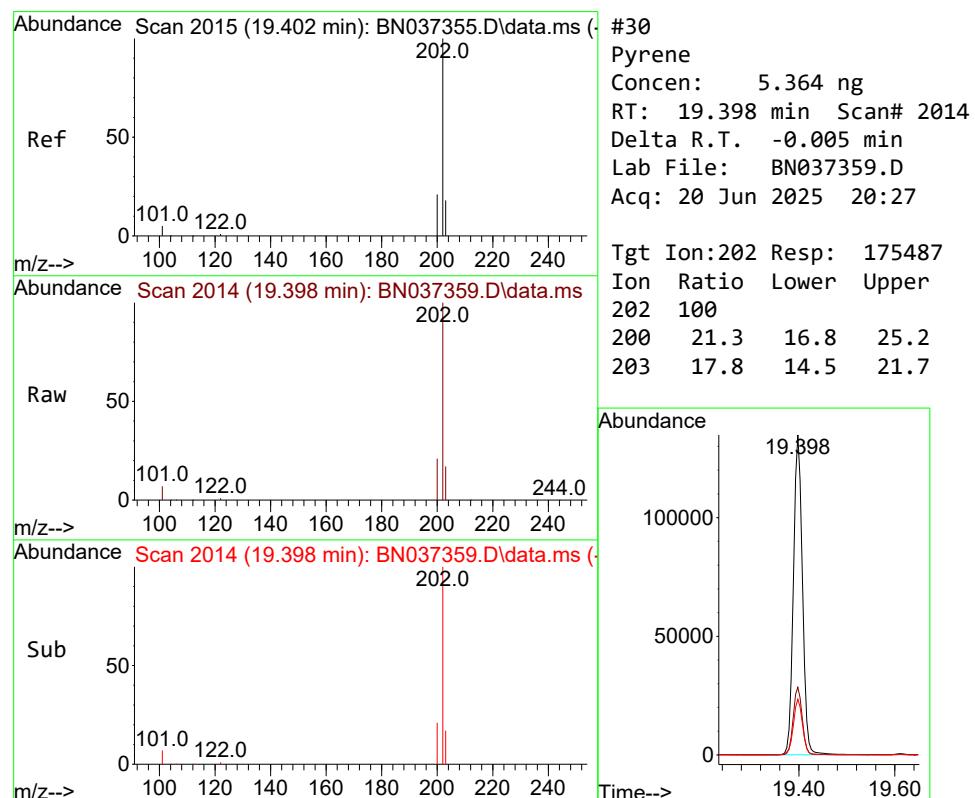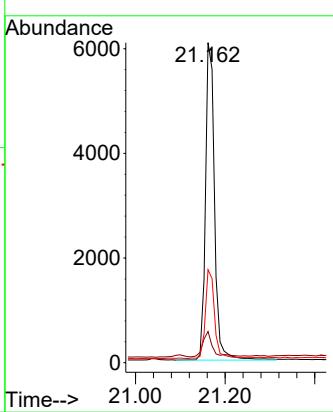

#30  
Pyrene  
Concen: 5.364 ng  
RT: 19.398 min Scan# 2014  
Delta R.T. -0.005 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27

Tgt Ion:202 Resp: 175487  
Ion Ratio Lower Upper  
202 100  
200 21.3 16.8 25.2  
203 17.8 14.5 21.7


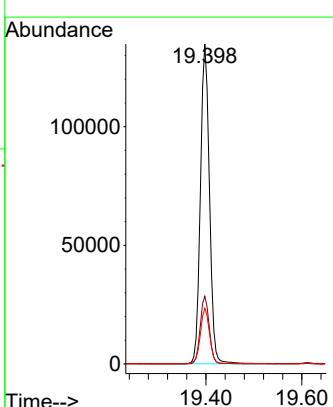


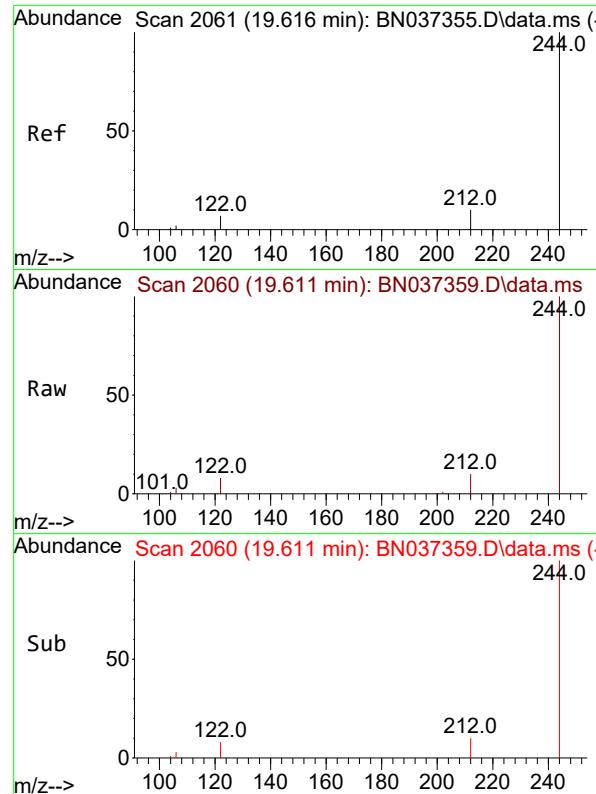

#31  
**Terphenyl-d14**  
Concen: 5.042 ng  
RT: 19.611 min Scan# 2  
Delta R.T. -0.005 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0


Tgt Ion:244 Resp: 98354  
Ion Ratio Lower Upper  
244 100  
212 10.2 11.1 16.7#  
122 8.4 7.2 10.8

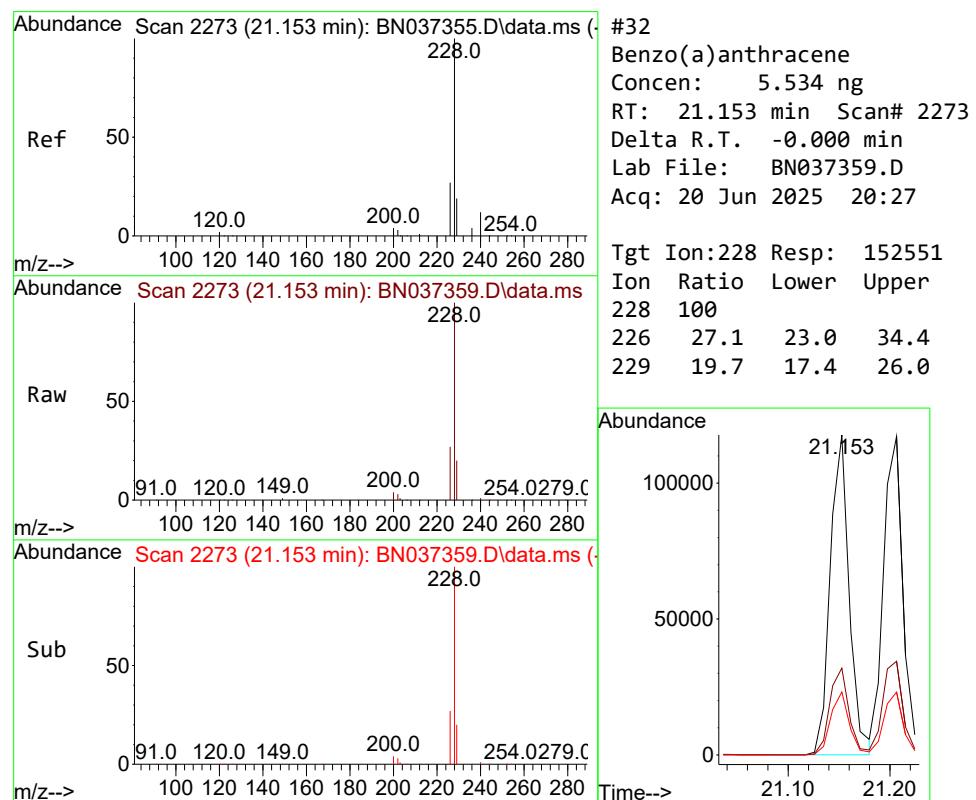

#32  
**Benzo(a)anthracene**  
Concen: 5.534 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27



Tgt Ion:228 Resp: 152551  
Ion Ratio Lower Upper  
228 100  
226 27.1 23.0 34.4  
229 19.7 17.4 26.0

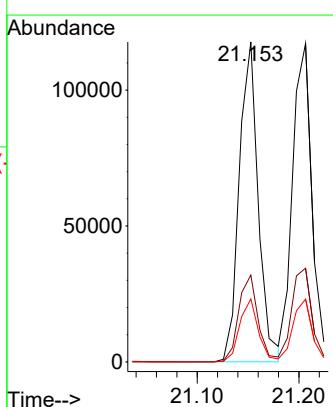

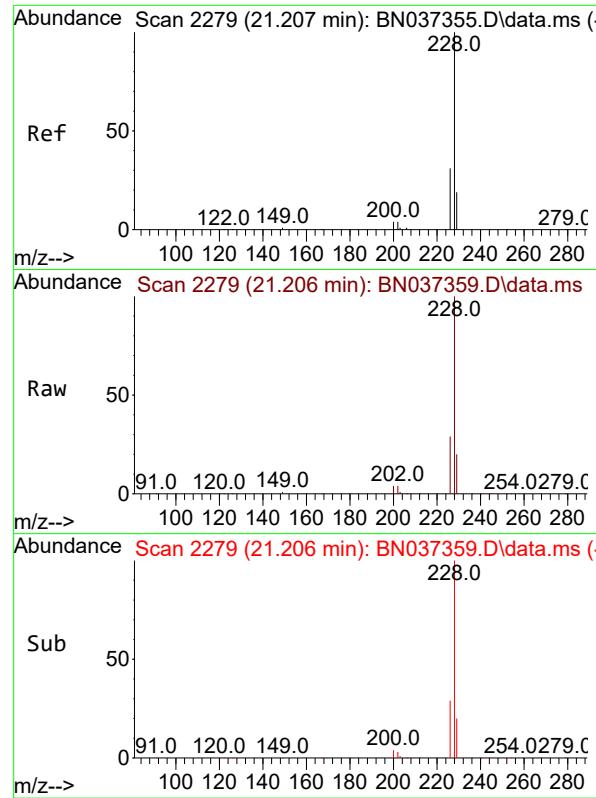


#33  
Chrysene  
Concen: 4.566 ng  
RT: 21.206 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27  
ClientSampleId : SSTDICC5.0


Tgt Ion:228 Resp: 159633  
Ion Ratio Lower Upper  
228 100  
226 29.5 25.4 38.2  
229 19.7 17.3 25.9

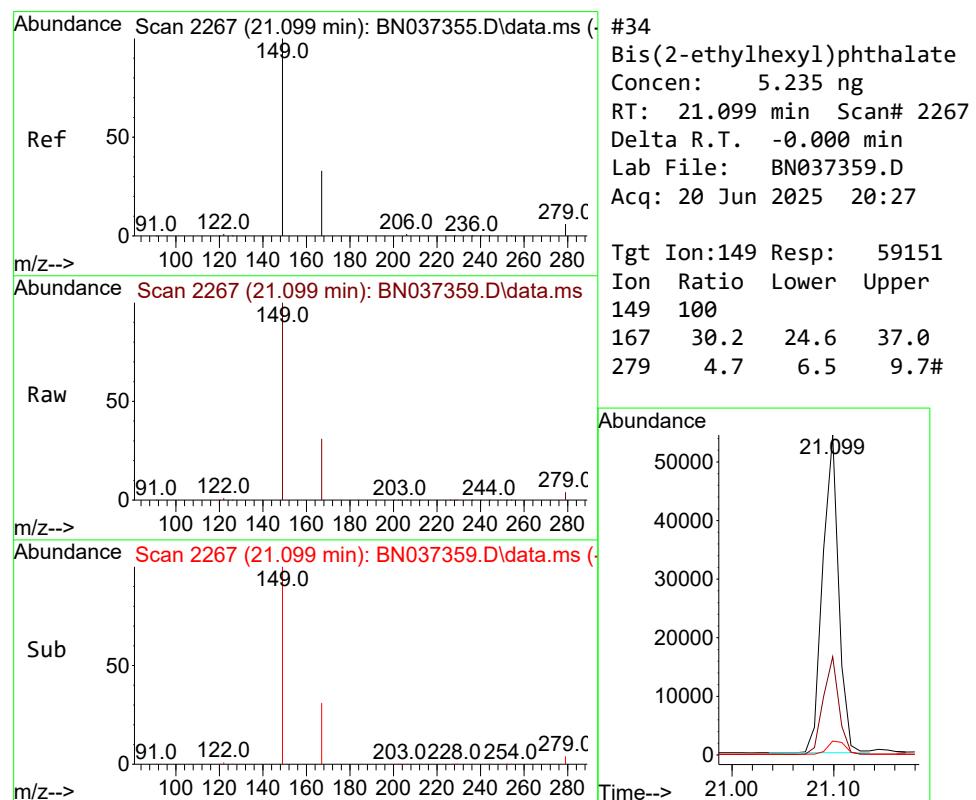

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 5.235 ng  
RT: 21.099 min Scan# 2267  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27



Tgt Ion:149 Resp: 59151  
Ion Ratio Lower Upper  
149 100  
167 30.2 24.6 37.0  
279 4.7 6.5 9.7#



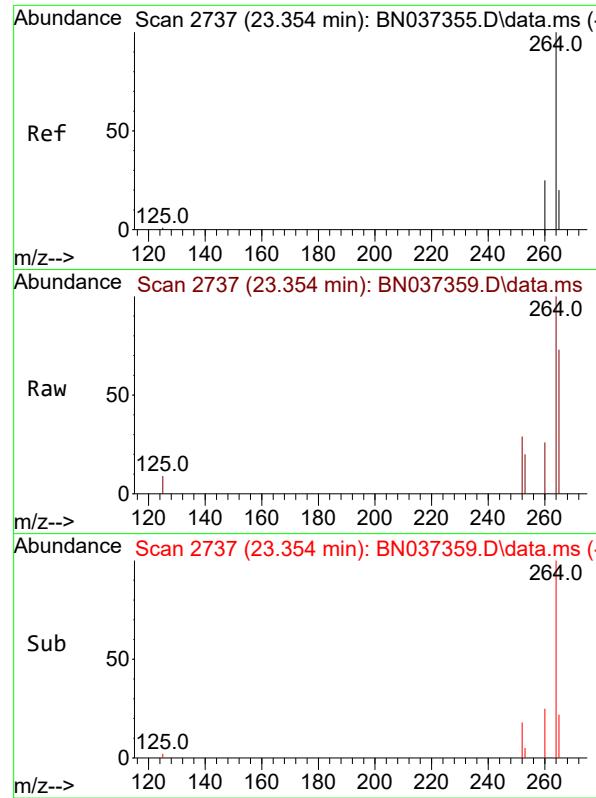


#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.354 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27  
ClientSampleId : SSTDICC5.0


Tgt Ion:264 Resp: 7704  
Ion Ratio Lower Upper  
264 100  
260 26.2 21.4 32.2  
265 73.1 71.4 107.0

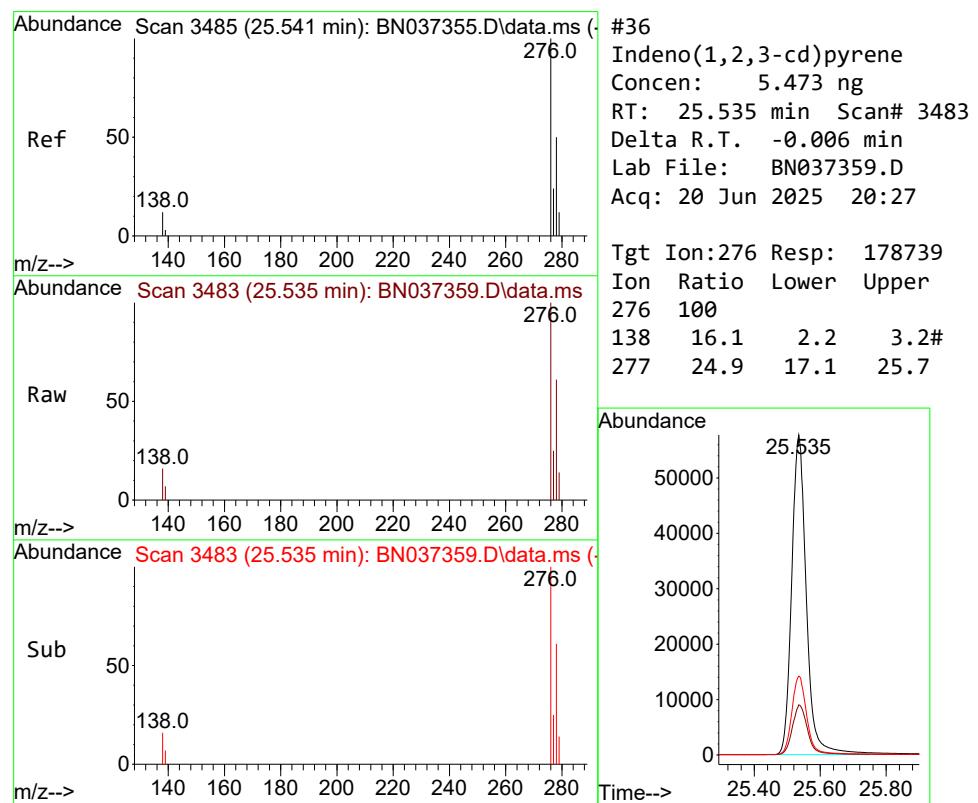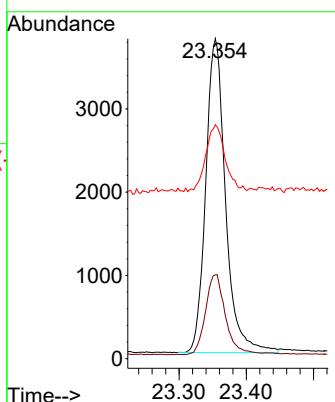

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 5.473 ng  
RT: 25.535 min Scan# 3483  
Delta R.T. -0.006 min  
Lab File: BN037359.D  
Acq: 20 Jun 2025 20:27

Tgt Ion:276 Resp: 178739  
Ion Ratio Lower Upper  
276 100  
138 16.1 2.2 3.2#  
277 24.9 17.1 25.7





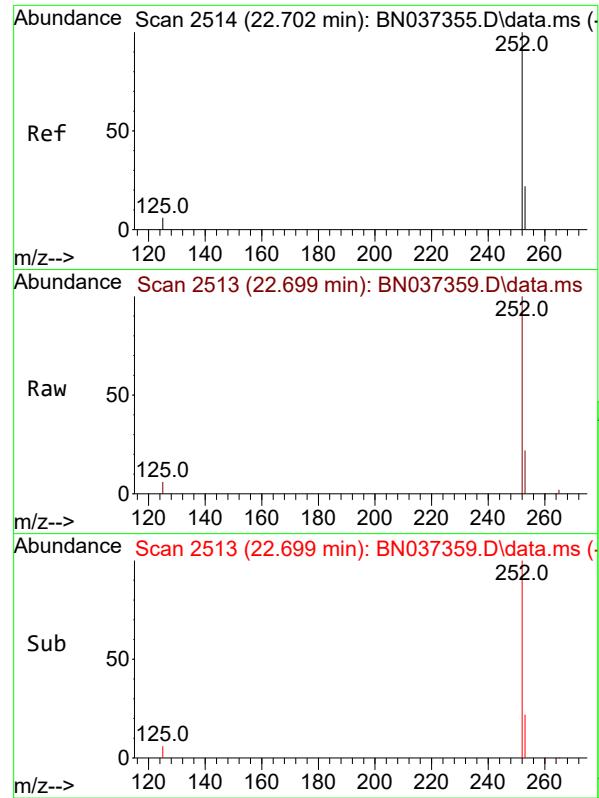

#37  
 Benzo(b)fluoranthene  
 Concen: 5.595 ng  
 RT: 22.699 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0


Tgt Ion:252 Resp: 152855  
 Ion Ratio Lower Upper  
 252 100  
 253 22.1 26.6 40.0#  
 125 6.3 6.1 9.1

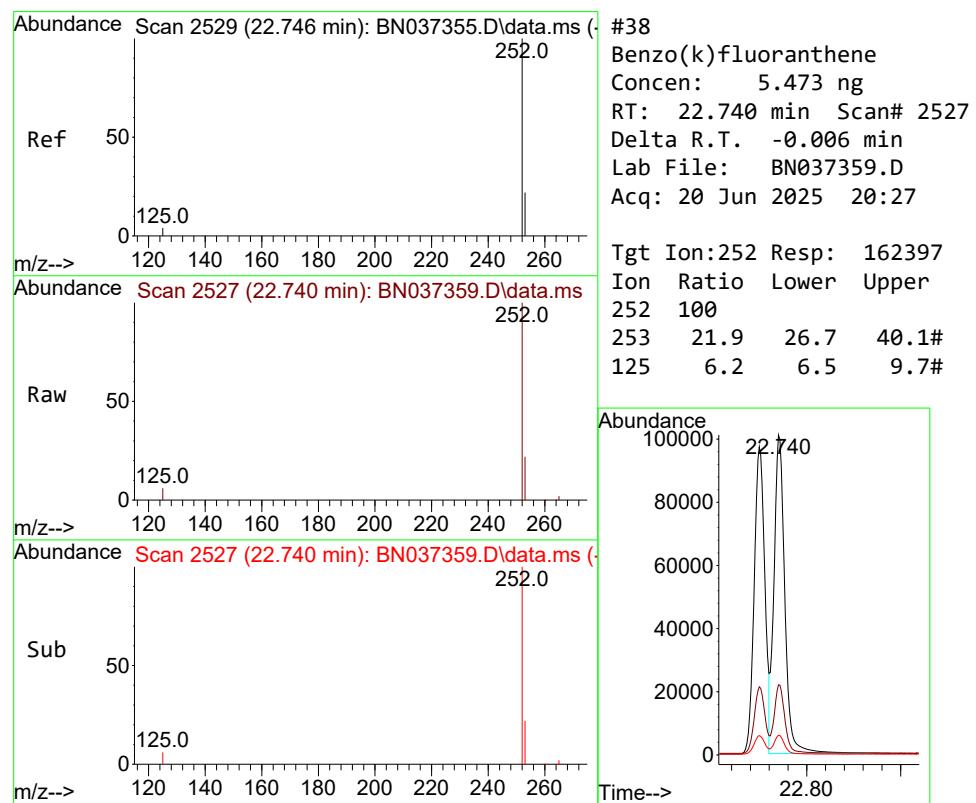

#38  
 Benzo(k)fluoranthene  
 Concen: 5.473 ng  
 RT: 22.740 min Scan# 2527  
 Delta R.T. -0.006 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27

Tgt Ion:252 Resp: 162397  
 Ion Ratio Lower Upper  
 252 100  
 253 21.9 26.7 40.1#  
 125 6.2 6.5 9.7#





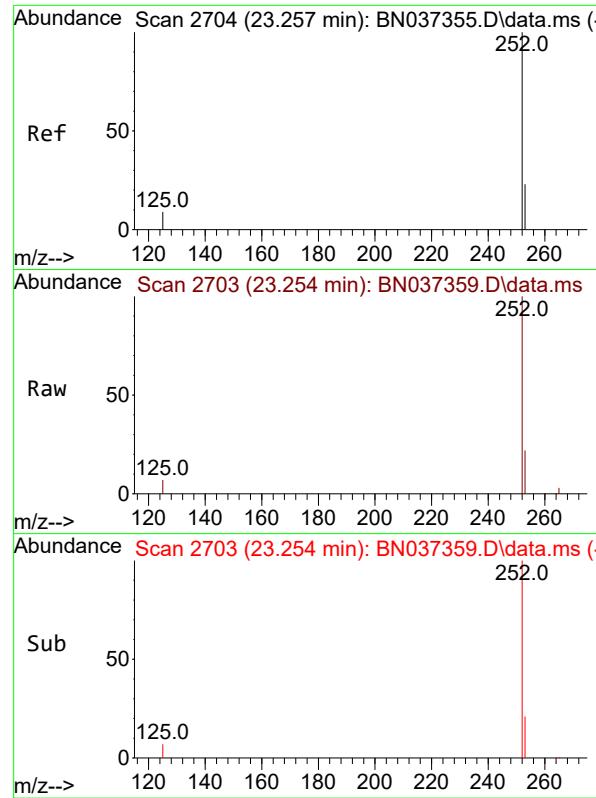

#39  
 Benzo(a)pyrene  
 Concen: 5.375 ng  
 RT: 23.254 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0


Tgt Ion:252 Resp: 134379  
 Ion Ratio Lower Upper  
 252 100  
 253 22.0 31.6 47.4#  
 125 7.0 8.4 12.6#

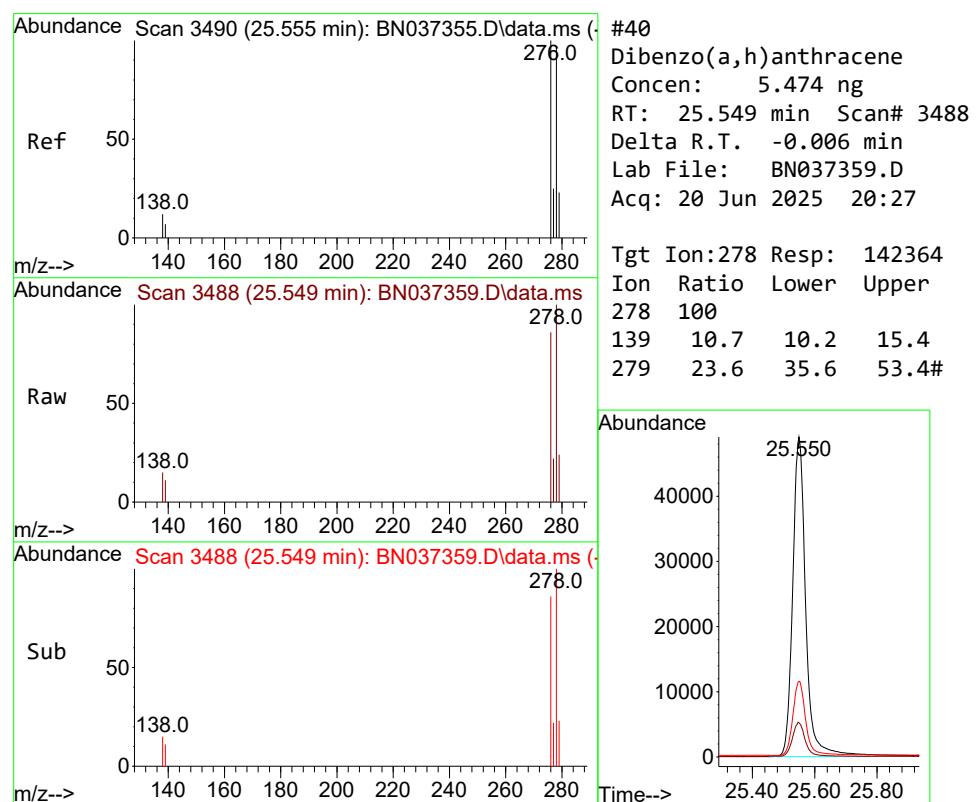

#40  
 Dibenzo(a,h)anthracene  
 Concen: 5.474 ng  
 RT: 25.549 min Scan# 3488  
 Delta R.T. -0.006 min  
 Lab File: BN037359.D  
 Acq: 20 Jun 2025 20:27

Tgt Ion:278 Resp: 142364  
 Ion Ratio Lower Upper  
 278 100  
 139 10.7 10.2 15.4  
 279 23.6 35.6 53.4#



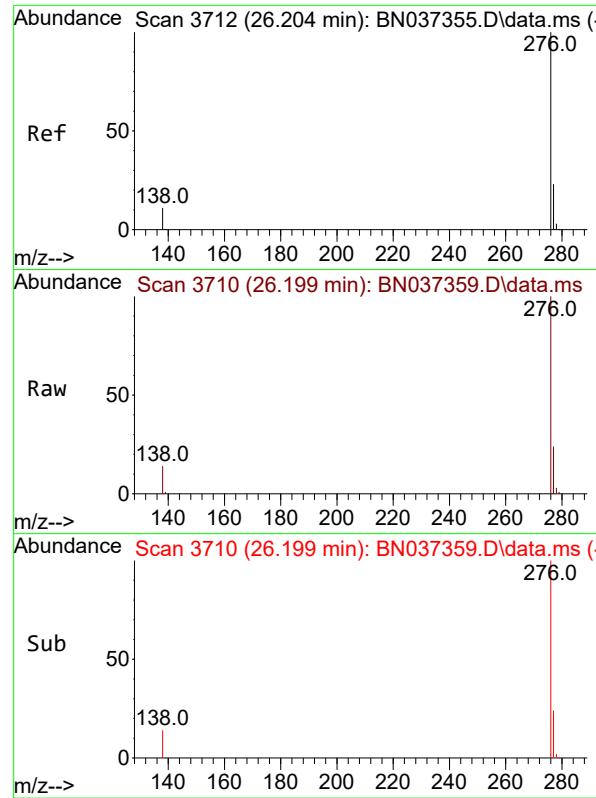

#41

Benzo(g,h,i)perylene

Concen: 5.131 ng

RT: 26.199 min Scan# 3

Instrument :

BNA\_N

Delta R.T. -0.006 min

Lab File: BN037359.D

ClientSampleId :

Acq: 20 Jun 2025 20:27

SSTDICC5.0


Tgt Ion:276 Resp: 153920

Ion Ratio Lower Upper

276 100

277 23.8 22.7 34.1

138 13.8 9.4 14.2



Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037360.D  
 Acq On : 20 Jun 2025 21:39  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 ICVBN062125

Quant Time: Jun 20 23:48:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2309	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	5064	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	3457	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	7065	0.400	ng	# 0.00
29) Chrysene-d12	21.171	240	5560	0.400	ng	# 0.00
35) Perylene-d12	23.354	264	5756	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1841	0.399	ng	0.00
5) Phenol-d6	6.752	99	1797	0.378	ng	0.00
8) Nitrobenzene-d5	8.717	82	1658	0.405	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	3394	0.414	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	756	0.373	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	6049	0.398	ng	0.00
27) Fluoranthene-d10	19.008	212	7940	0.392	ng	0.00
31) Terphenyl-d14	19.616	244	5266	0.416	ng	0.00
<b>Target Compounds</b>						
					Qvalue	
2) 1,4-Dioxane	3.104	88	942	0.401	ng	91
3) n-Nitrosodimethylamine	3.422	42	845	0.393	ng	# 70
6) bis(2-Chloroethyl)ether	7.004	93	1718	0.407	ng	93
9) Naphthalene	10.394	128	5338	0.399	ng	# 89
10) Hexachlorobutadiene	10.682	225	2157	0.409	ng	# 99
12) 2-Methylnaphthalene	12.021	142	3620	0.388	ng	# 91
16) Acenaphthylene	13.935	152	5463	0.376	ng	98
17) Acenaphthene	14.277	154	3720	0.389	ng	99
18) Fluorene	15.272	166	5193	0.386	ng	99
20) 4,6-Dinitro-2-methylph...	15.368	198	491	0.289	ng	92
21) 4-Bromophenyl-phenylether	16.165	248	1905	0.379	ng	# 84
22) Hexachlorobenzene	16.276	284	2222	0.406	ng	98
23) Atrazine	16.450	200	1453	0.362	ng	# 84
24) Pentachlorophenol	16.624	266	881	0.323	ng	97
25) Phenanthrene	17.009	178	7743	0.378	ng	99
26) Anthracene	17.108	178	6739	0.357	ng	99
28) Fluoranthene	19.036	202	9535	0.369	ng	# 99
30) Pyrene	19.398	202	9570	0.424	ng	100
32) Benzo(a)anthracene	21.153	228	6805	0.372	ng	99
33) Chrysene	21.207	228	9119	0.412	ng	98
34) Bis(2-ethylhexyl)phtha...	21.099	149	3022	0.403	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.541	276	9492	0.368	ng	# 92
37) Benzo(b)fluoranthene	22.702	252	8083m	0.382	ng	
38) Benzo(k)fluoranthene	22.746	252	9472	0.412	ng	95
39) Benzo(a)pyrene	23.260	252	7258	0.382	ng	# 89
40) Dibenzo(a,h)anthracene	25.553	278	7116	0.367	ng	# 87
41) Benzo(g,h,i)perylene	26.199	276	8707	0.378	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037360.D  
 Acq On : 20 Jun 2025 21:39  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1


Quant Time: Jun 20 23:48:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

Instrument :  
 BNA\_N  
 ClientSampleId :  
 ICVBN062125

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

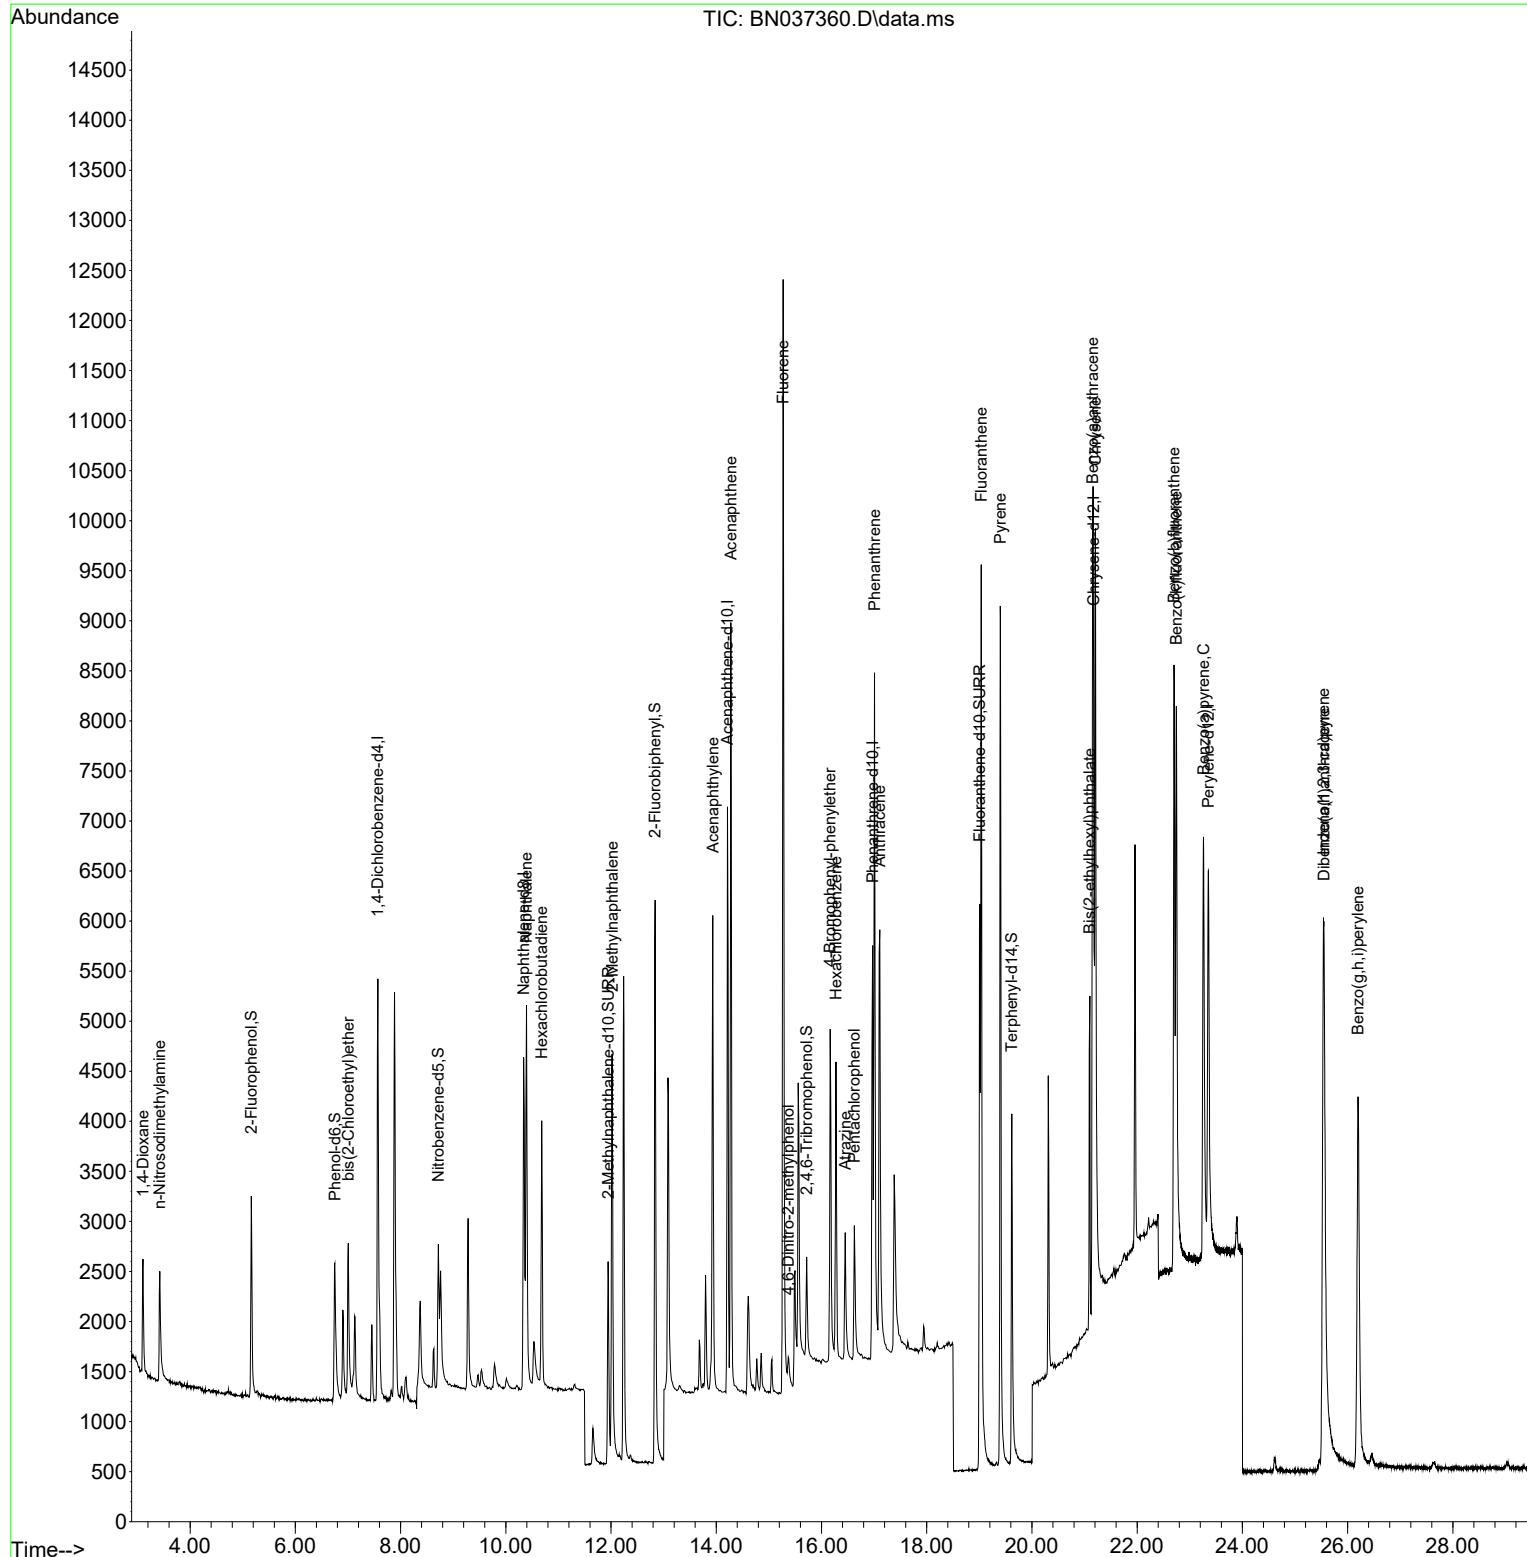


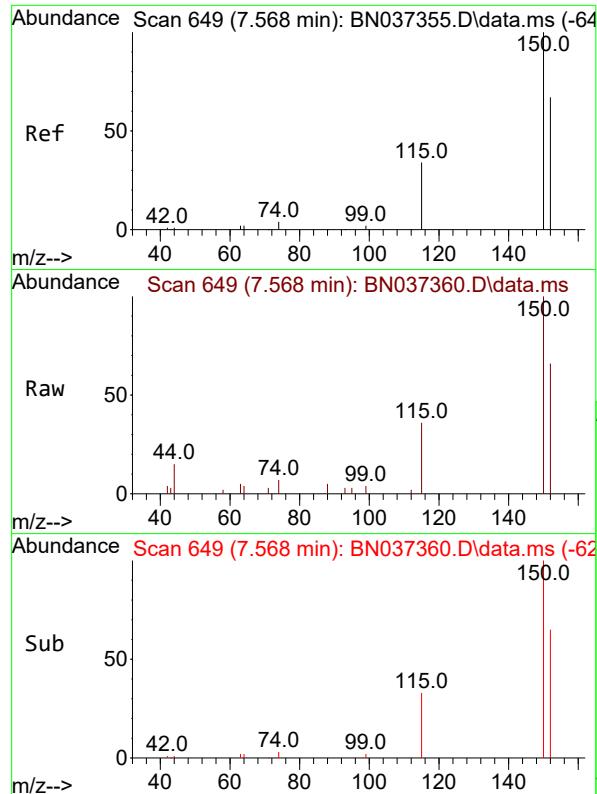


#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
ClientSampleId : ICVBN062125


**Manual Integrations**  
**APPROVED**



Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

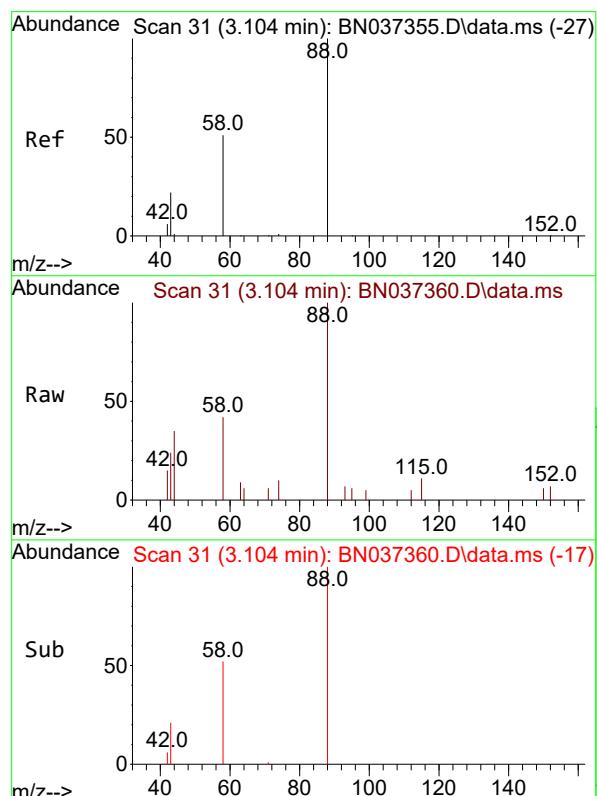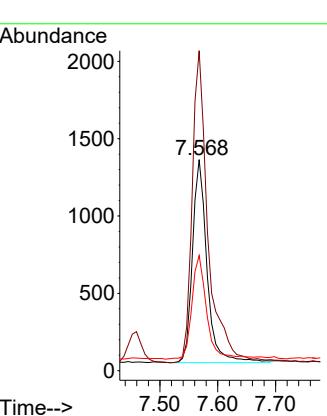

#2  
1,4-Dioxane  
Concen: 0.401 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Tgt Ion: 88 Resp: 942  
Ion Ratio Lower Upper  
88 100  
43 24.5 21.0 31.6  
58 55.4 38.0 57.0

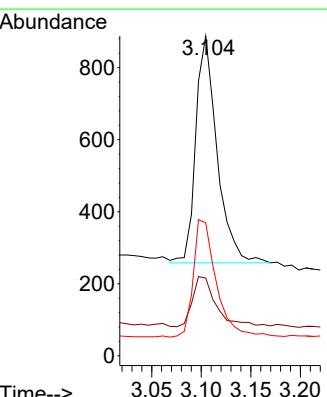

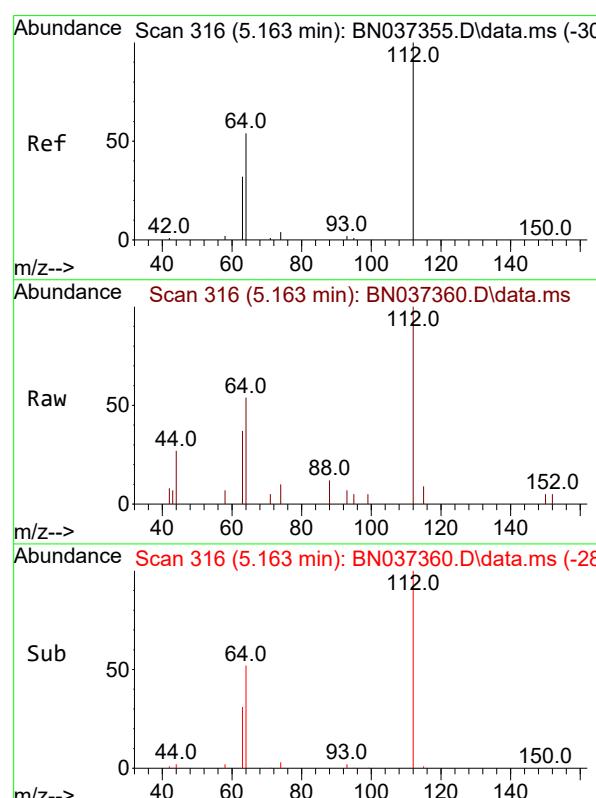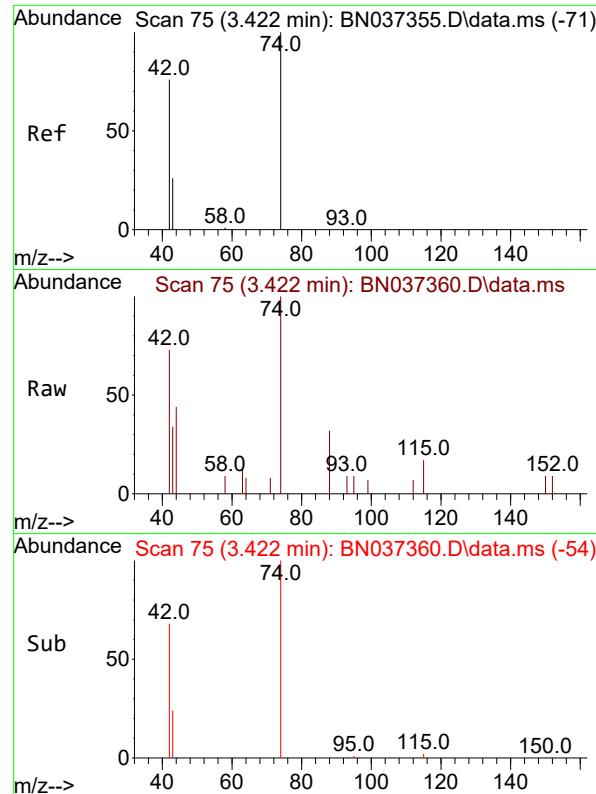

#3

n-Nitrosodimethylamine

Concen: 0.393 ng

RT: 3.422 min Scan# 7

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N


ClientSampleId :

ICVBN062125

### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#4

2-Fluorophenol

Concen: 0.399 ng

RT: 5.163 min Scan# 316

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39


Tgt Ion:112 Resp: 1841


Ion Ratio Lower Upper

112 100

64 50.3 38.7 58.1

63 31.9 26.4 39.6

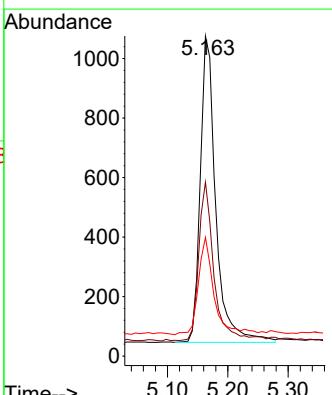


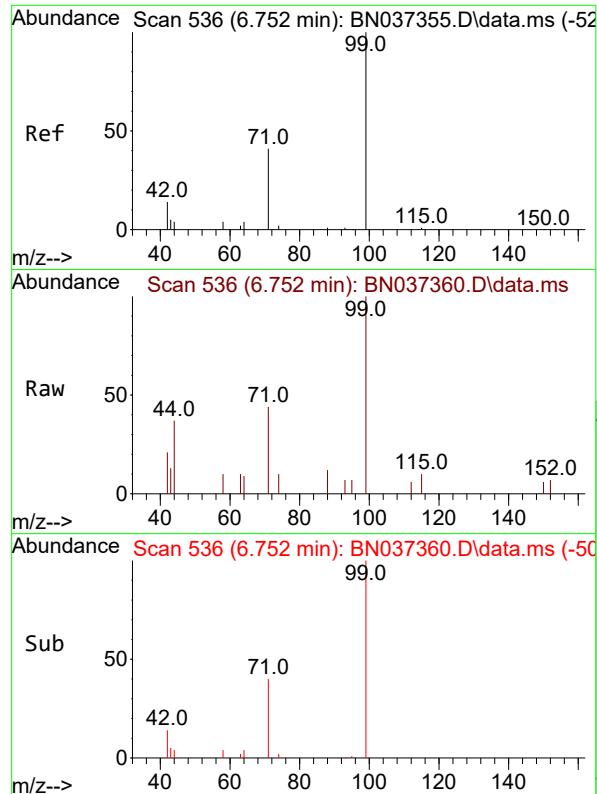


#5  
 Phenol-d6  
 Concen: 0.378 ng  
 RT: 6.752 min Scan# 51  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
 ClientSampleId : ICVBN062125


**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

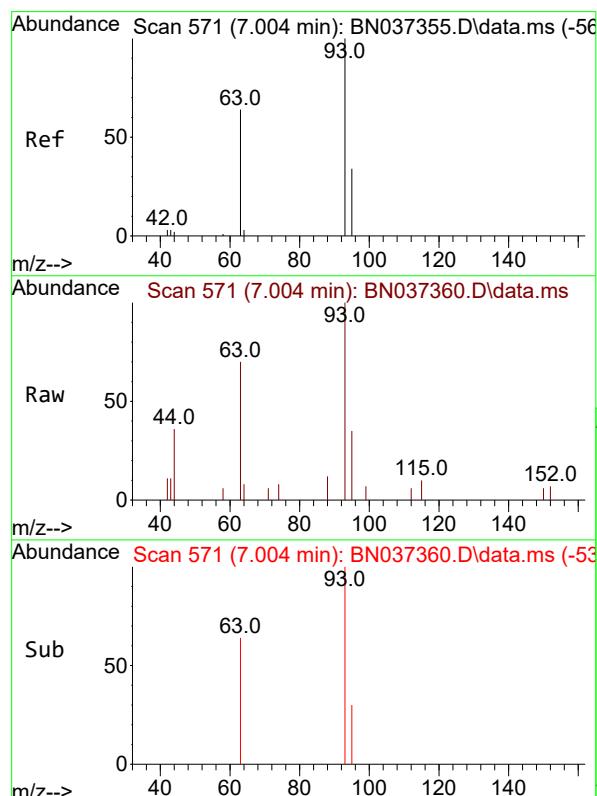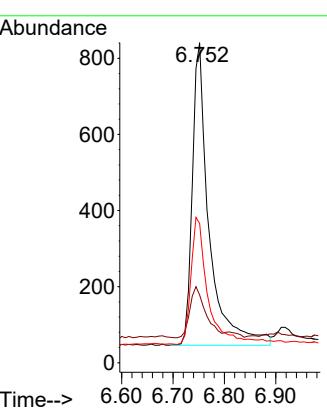

#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.407 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Tgt Ion: 93 Resp: 1718  
 Ion Ratio Lower Upper  
 93 100  
 63 61.8 53.2 79.8  
 95 29.5 27.3 40.9

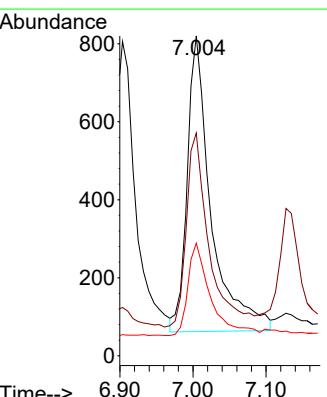



#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.340 min Scan# 9  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39




Instrument : BNA\_N  
ClientSampleId : ICVBN062125

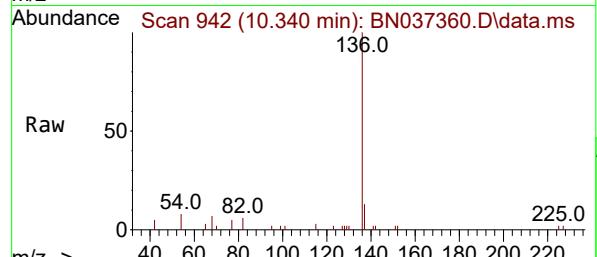


Tgt Ion:136 Resp: 5064  
Ion Ratio Lower Upper  
136 100  
137 12.7 12.2 18.2  
54 7.6 8.8 13.2  
68 6.7 7.0 10.4#

### Manual Integrations APPROVED



Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

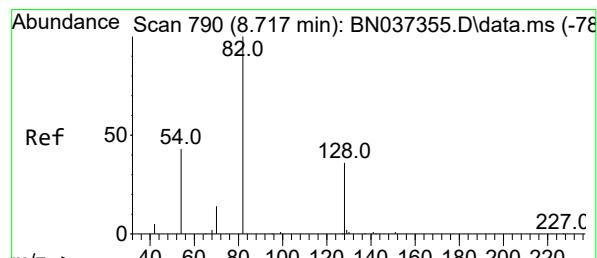

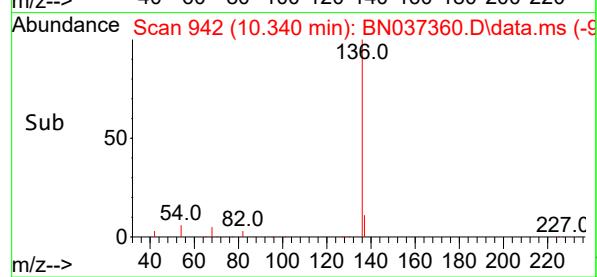


#8  
Nitrobenzene-d5  
Concen: 0.405 ng  
RT: 8.717 min Scan# 790  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

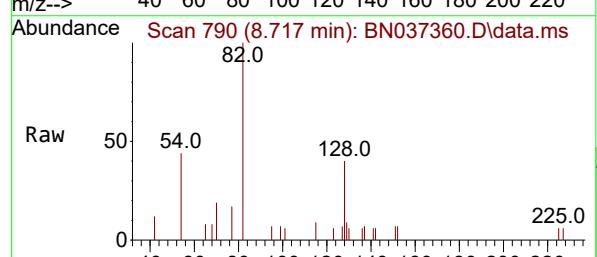

Tgt Ion: 82 Resp: 1658  
Ion Ratio Lower Upper  
82 100  
128 39.6 42.5 63.7#  
54 43.9 43.2 64.8

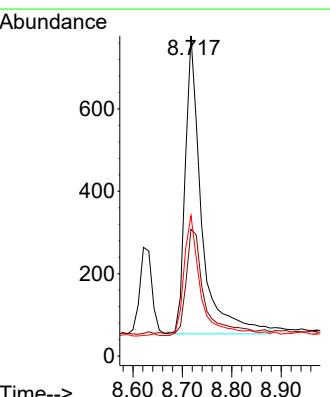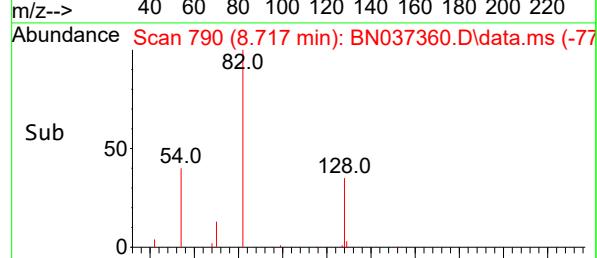



#9

Naphthalene

Concen: 0.399 ng

RT: 10.394 min Scan# 9

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N





ClientSampleId :

ICVBN062125

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

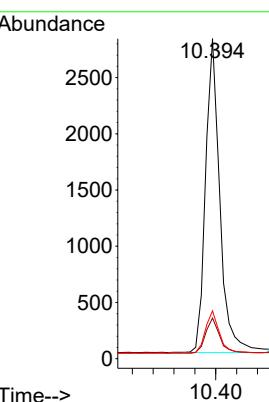

#10

Hexachlorobutadiene

Concen: 0.409 ng


RT: 10.682 min Scan# 974




Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Tgt	Ion:225	Resp:	2157
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.3	50.3	75.5

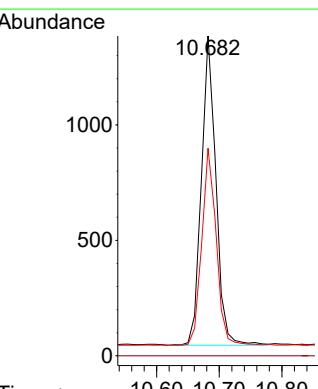


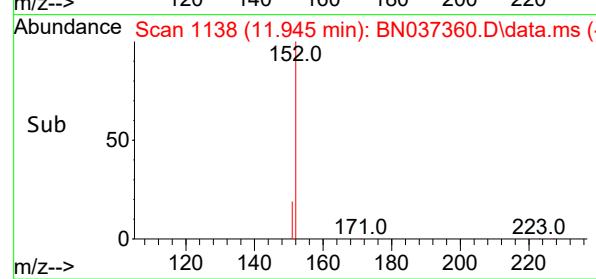




#11  
2-Methylnaphthalene-d10  
Concen: 0.414 ng  
RT: 11.945 min Scan# 1138  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
ClientSampleId : ICVBN062125


**Manual Integrations**  
**APPROVED**







Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

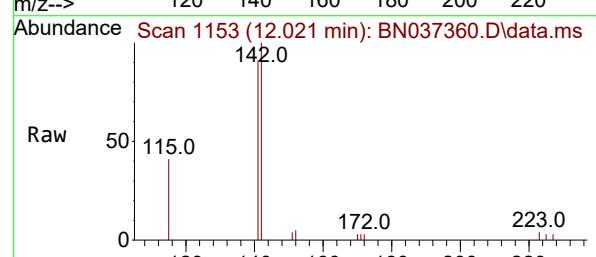


#12  
2-Methylnaphthalene  
Concen: 0.388 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Tgt Ion:142 Resp: 3620  
Ion Ratio Lower Upper  
142 100  
141 90.6 70.2 105.2  
115 41.2 43.0 64.4#

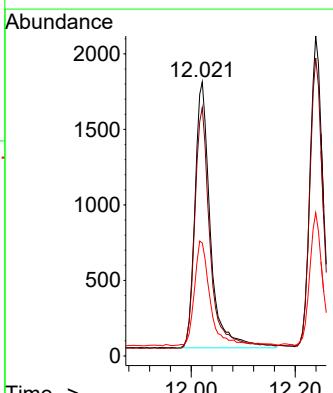


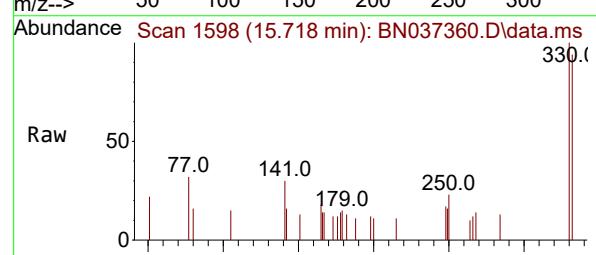
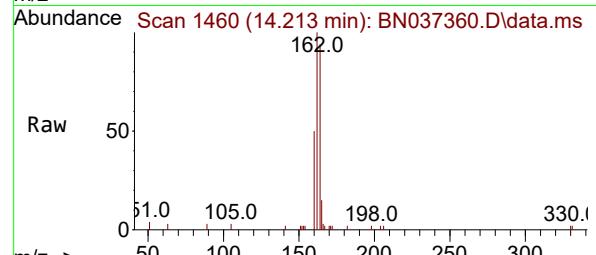



#13

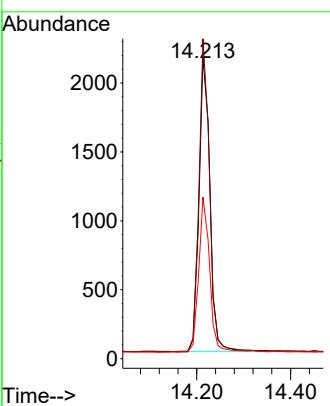Acenaphthene-d10  
Concen: 0.400 ngRT: 14.213 min Scan# 1460  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39Instrument : BNA\_N  
ClientSampleId : ICVBN062125**Manual Integrations  
APPROVED**Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

#14

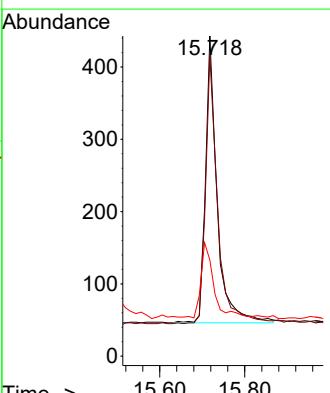2,4,6-Tribromophenol  
Concen: 0.373 ng  
RT: 15.718 min Scan# 1598  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39Tgt Ion:330 Resp: 756  
Ion Ratio Lower Upper  
330 100  
332 96.7 78.4 117.6  
141 28.0 24.4 36.6

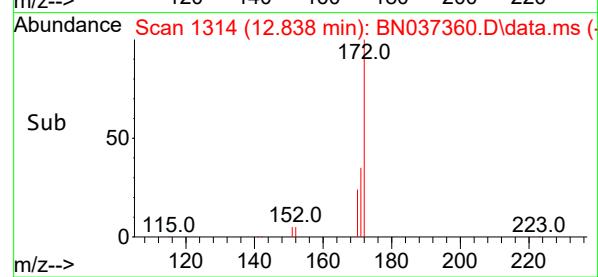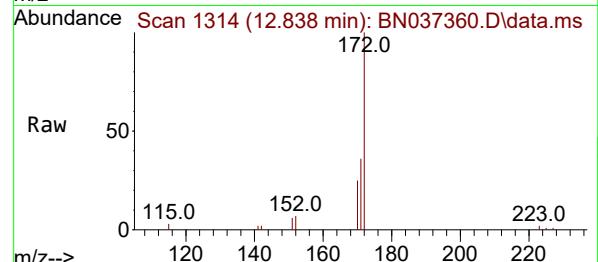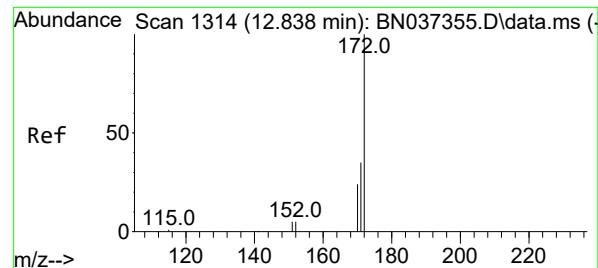

#15

2-Fluorobiphenyl

Concen: 0.398 ng

RT: 12.838 min Scan# 1314

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39





Instrument : BNA\_N

ClientSampleId : ICVBN062125

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

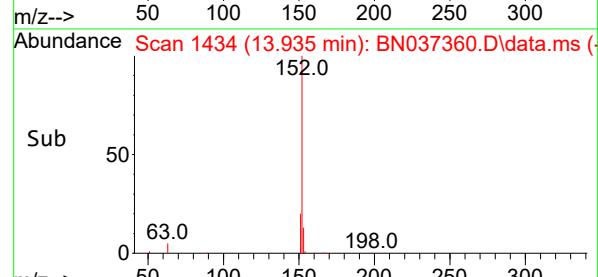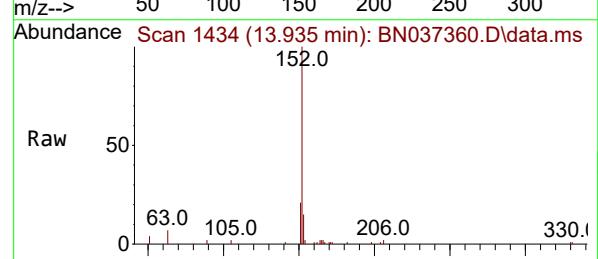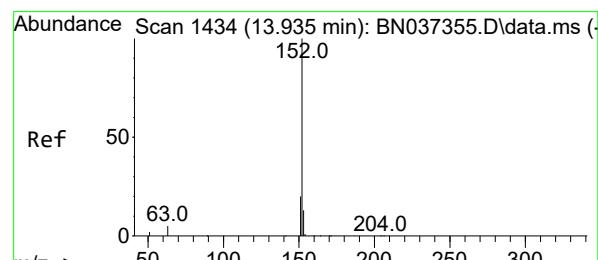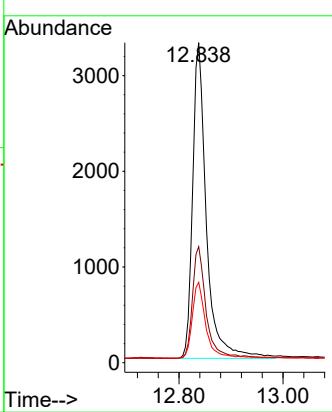

#16

Acenaphthylene

Concen: 0.376 ng


RT: 13.935 min Scan# 1434




Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Tgt	Ion:152	Resp:	5463
Ion	Ratio	Lower	Upper
152	100		
151	19.8	16.6	24.8
153	13.3	10.2	15.2

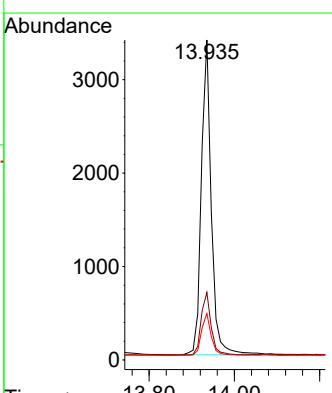



#17

Acenaphthene

Concen: 0.389 ng

RT: 14.277 min Scan# 1466

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N




ClientSampleId :

ICVBN062125

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#18

Fluorene

Concen: 0.386 ng


RT: 15.272 min Scan# 1559


Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Tgt	Ion:166	Resp:	5193
Ion	Ratio	Lower	Upper
166	100		
165	98.8	79.5	119.3
167	13.4	10.7	16.1

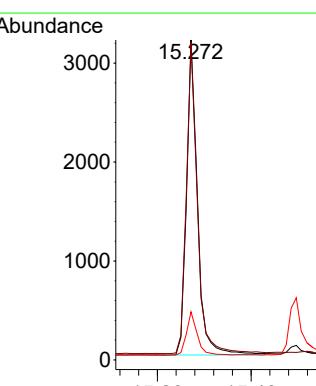

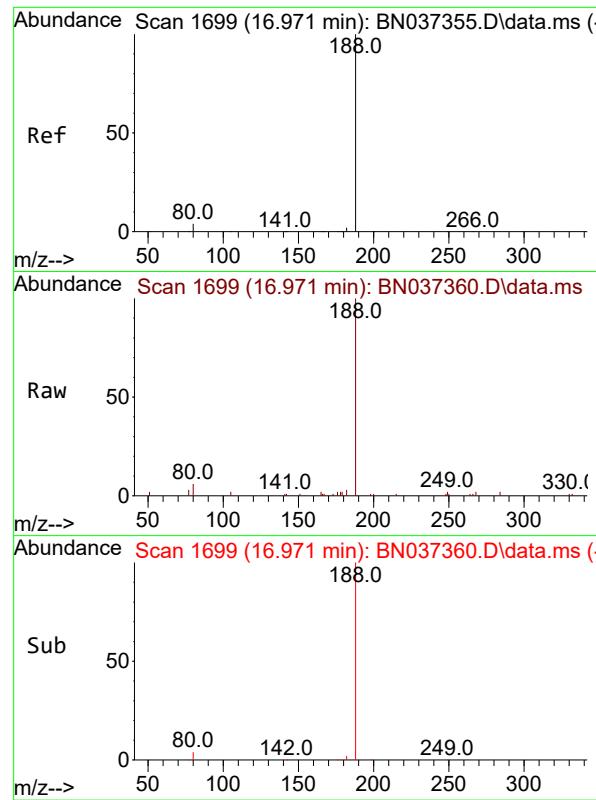

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N



ClientSampleId :

ICVBN062125

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

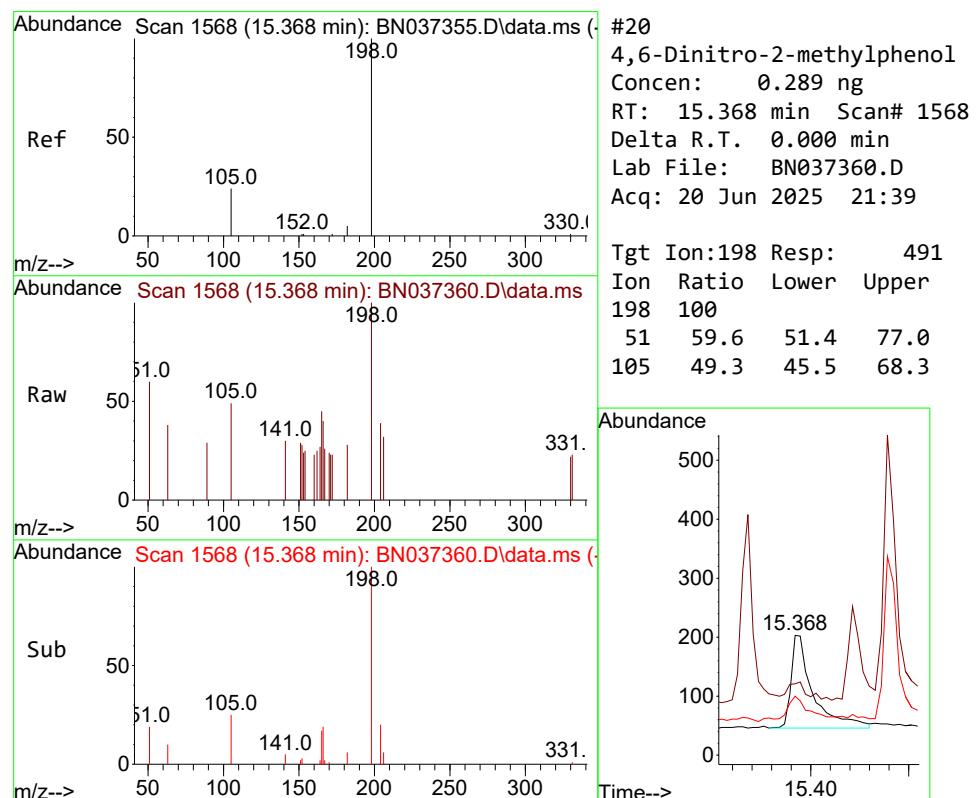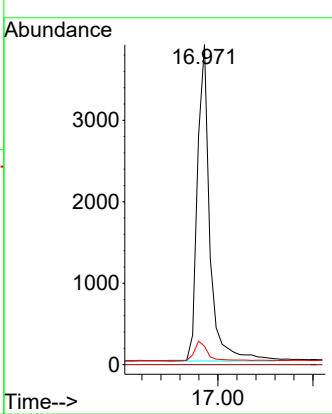

#20

4,6-Dinitro-2-methylphenol

Concen: 0.289 ng

RT: 15.368 min Scan# 1568

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39


Tgt Ion:198 Resp: 491


Ion Ratio Lower Upper

198 100

51 59.6 51.4 77.0

105 49.3 45.5 68.3

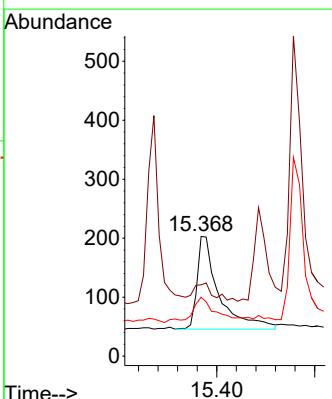


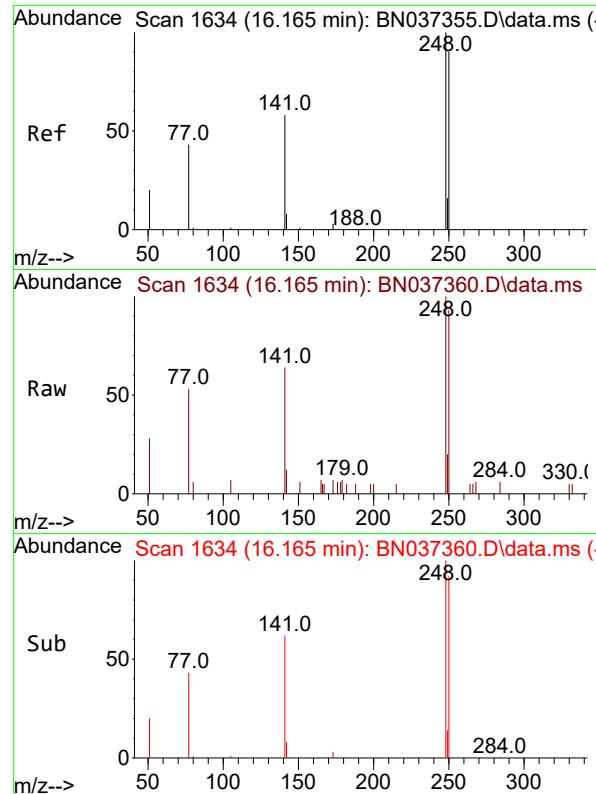


#21  
4-Bromophenyl-phenylether  
Concen: 0.379 ng  
RT: 16.165 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
ClientSampleId : ICVBN062125


**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

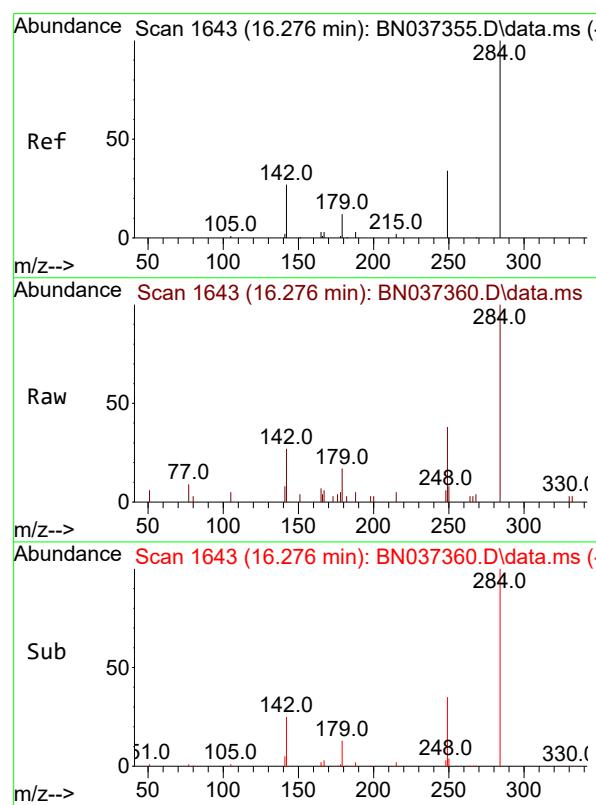


#22  
Hexachlorobenzene  
Concen: 0.406 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Tgt Ion:284 Resp: 2222  
Ion Ratio Lower Upper  
284 100  
142 33.0 27.0 40.6  
249 35.0 28.8 43.2






Abundance Scan 1657 (16.450 min): BN037360.D\data.ms (-)

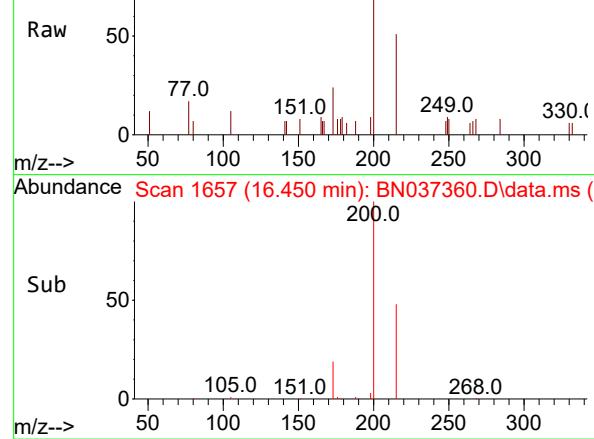

Abundance Scan 1657 (16.450 min): BN037360.D\data.ms (-)

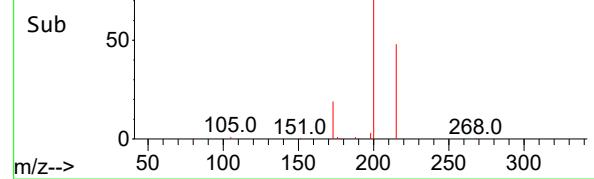

#23

Atrazine

Concen: 0.362 ng

RT: 16.450 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N


ClientSampleId :

ICVBN062125


**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025


Supervised By :Jagrut Upadhyay 06/24/2025

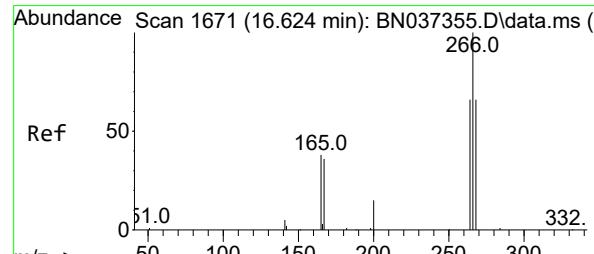

Abundance Scan 1671 (16.624 min): BN037360.D\data.ms (-)

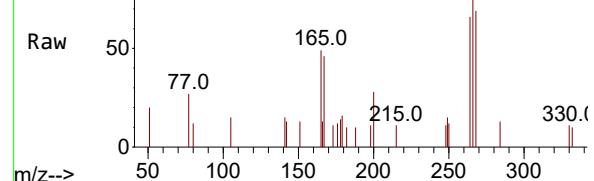

Abundance Scan 1671 (16.624 min): BN037360.D\data.ms (-)

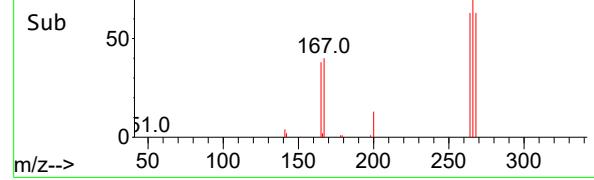

#24

Pentachlorophenol

Concen: 0.323 ng

RT: 16.624 min Scan# 1671

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Tgt Ion:266 Resp: 881

Ion Ratio Lower Upper

266 100



264 63.5 50.3 75.5

268 65.0 55.3 82.9

Abundance

16.624

Time--&gt;

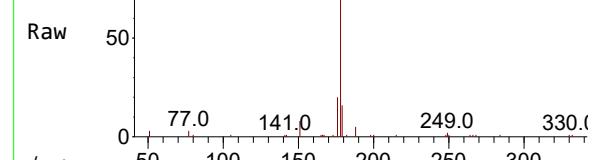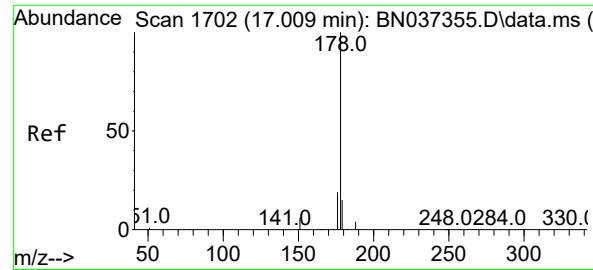

#25

Phenanthrene

Concen: 0.378 ng

RT: 17.009 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N



ClientSampleId :

ICVBN062125

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

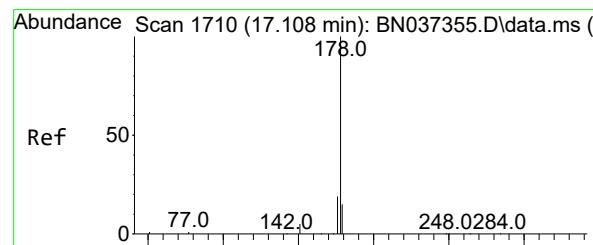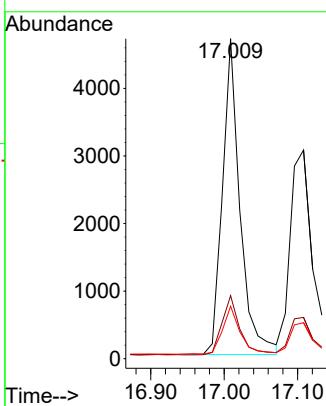

#26

Anthracene

Concen: 0.357 ng

RT: 17.108 min Scan# 1710

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39


Tgt Ion:178 Resp: 6739


Ion Ratio Lower Upper

178 100

176 19.0 14.7 22.1

179 15.7 13.0 19.6

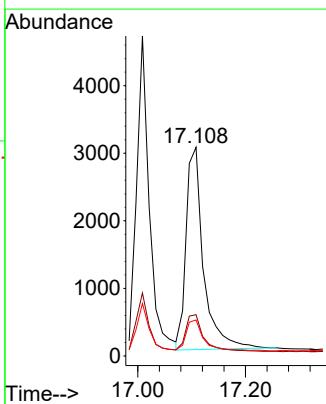

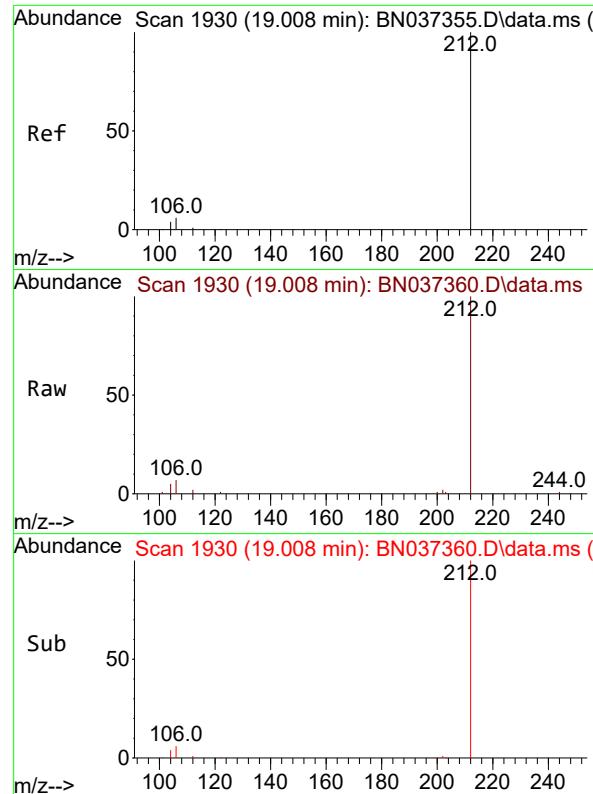

#27

Fluoranthene-d10

Concen: 0.392 ng

RT: 19.008 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N



ClientSampleId :

ICVBN062125

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

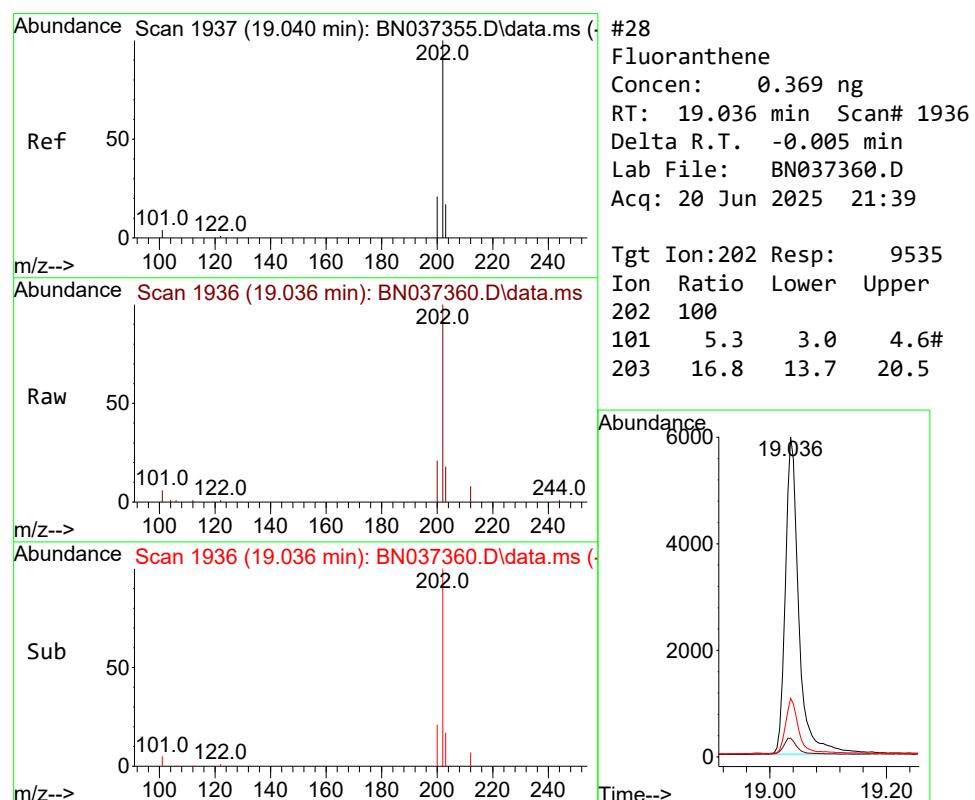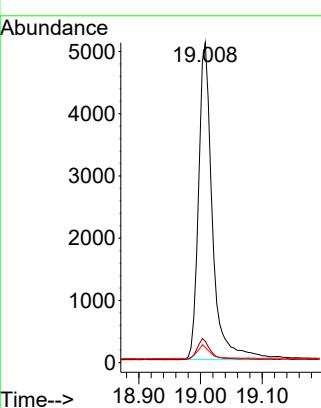

#28

Fluoranthene

Concen: 0.369 ng

RT: 19.036 min Scan# 1936


Delta R.T. -0.005 min




Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Tgt Ion:202 Resp: 9535

Ion	Ratio	Lower	Upper
202	100		
101	5.3	3.0	4.6
203	16.8	13.7	20.5

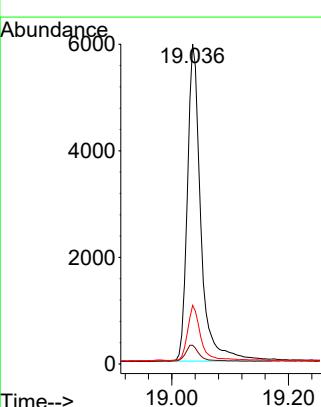

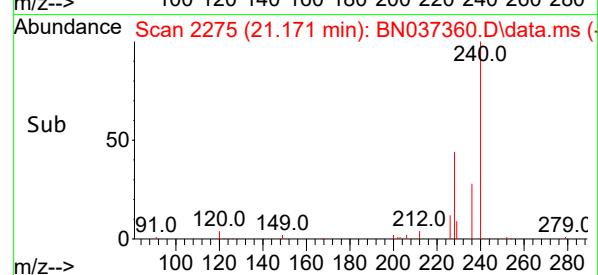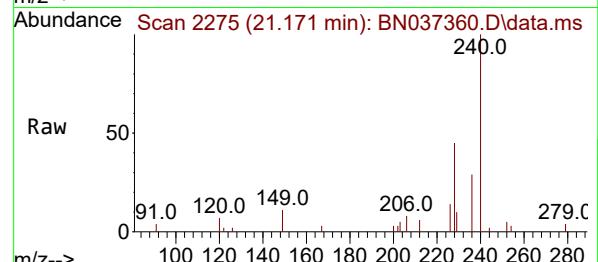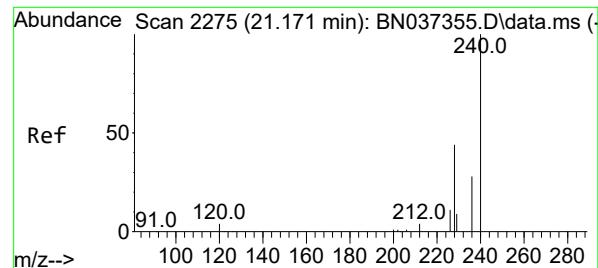

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.171 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N





ClientSampleId :

ICVBN062125

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

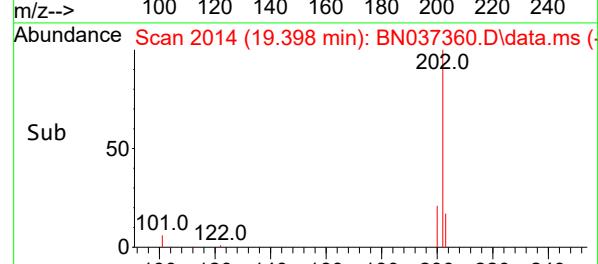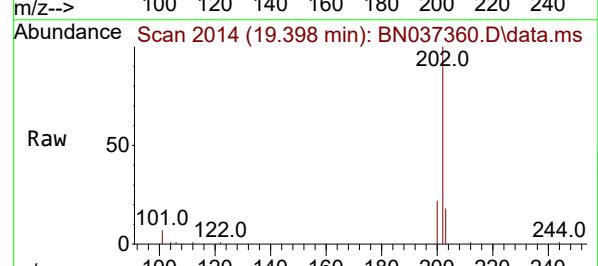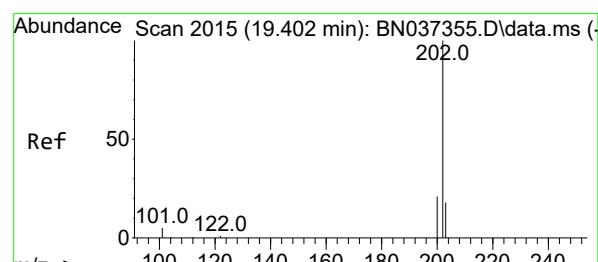

#30

Pyrene

Concen: 0.424 ng

RT: 19.398 min Scan# 2014

Delta R.T. -0.005 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39


Tgt Ion:202 Resp: 9570


Ion Ratio Lower Upper

202 100

200 20.7 16.8 25.2

203 18.0 14.5 21.7

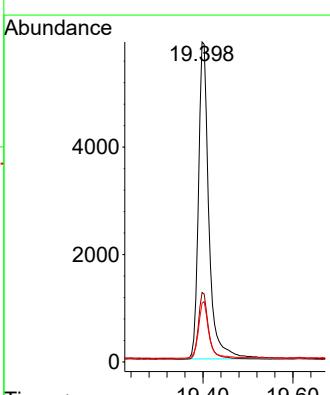


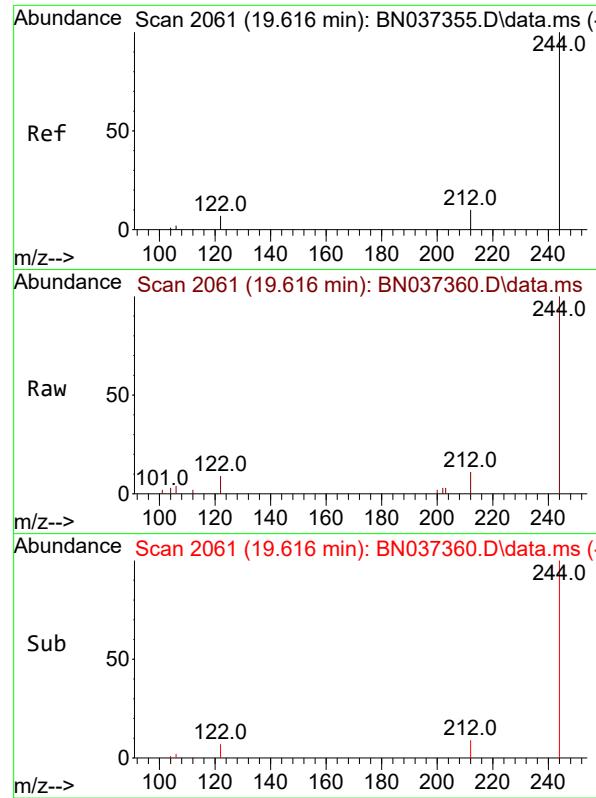


#31  
Terphenyl-d14  
Concen: 0.416 ng  
RT: 19.616 min Scan# 2  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
ClientSampleId : ICBN062125


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

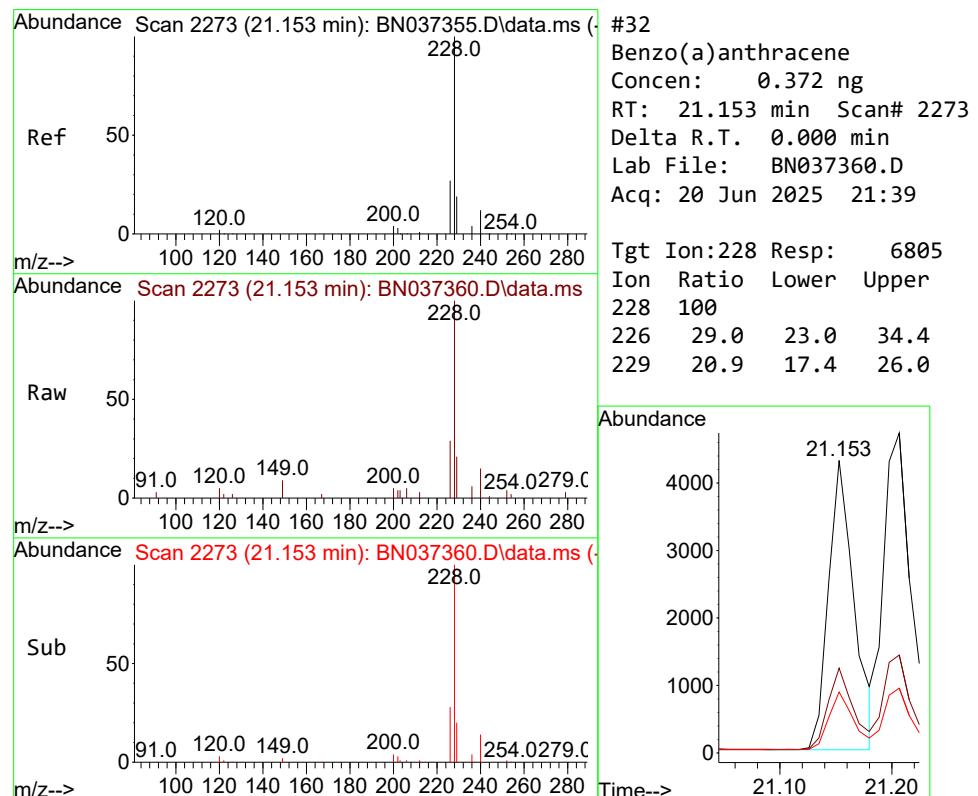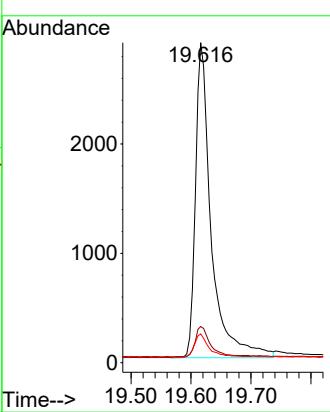

#32  
Benzo(a)anthracene  
Concen: 0.372 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Tgt Ion:228 Resp: 6805  
Ion Ratio Lower Upper  
228 100  
226 29.0 23.0 34.4  
229 20.9 17.4 26.0

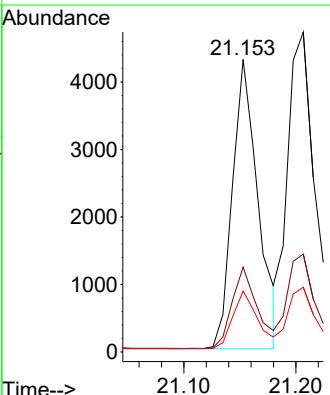

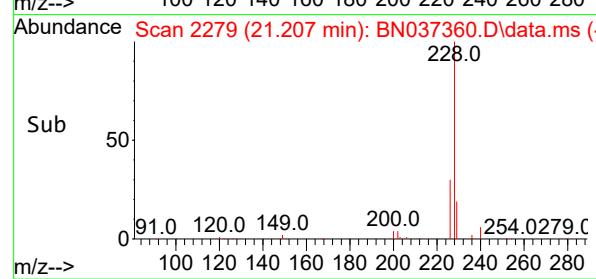

#33

Chrysene

Concen: 0.412 ng

RT: 21.207 min Scan# 2279

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N





ClientSampleId :

ICVBN062125

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

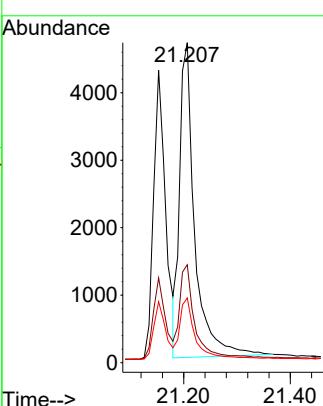

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.403 ng

RT: 21.099 min Scan# 2267

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39


Tgt Ion:149 Resp: 3022

Ion Ratio Lower Upper

149 100

167 31.4 24.6 37.0

279 5.6 6.5 9.7#

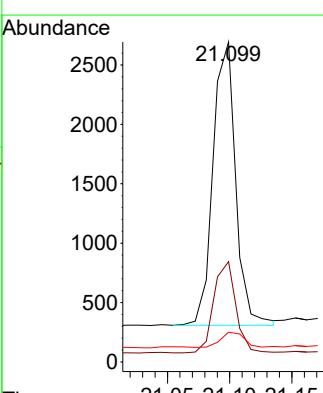

#35

Perylene-d<sub>12</sub>

Concen: 0.400 ng

RT: 23.354 min Scan# 2

Delta R.T. 0.000 min

Lab File: BN037360.D


Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N

ClientSampleId :



ICVBN062125

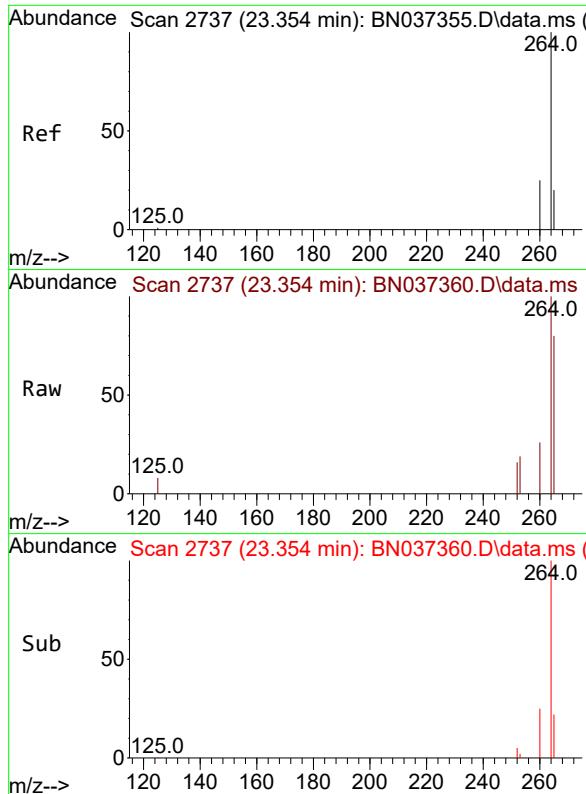


Tgt	Ion:264	Resp:	5750
Ion	Ratio	Lower	Upper
264	100		
260	26.4	21.4	32.2
265	80.4	71.4	107.0

### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

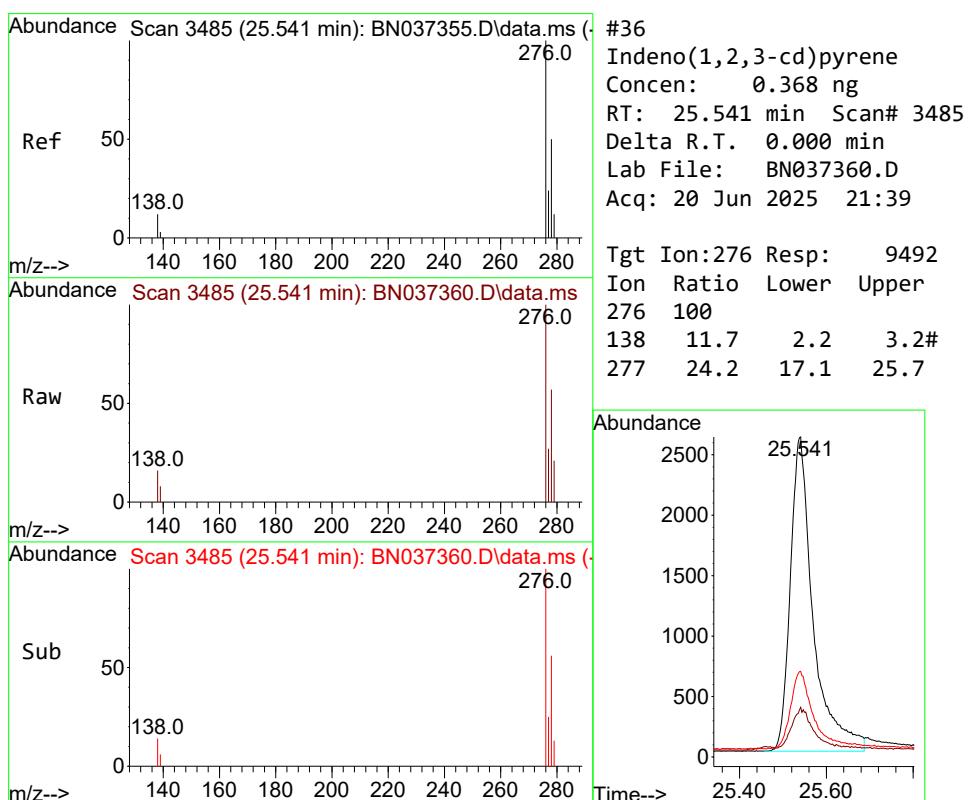

Tgt	Ion:276	Resp:	9492
Ion	Ratio	Lower	Upper
276	100		
138	11.7	2.2	3.2#
277	24.2	17.1	25.7

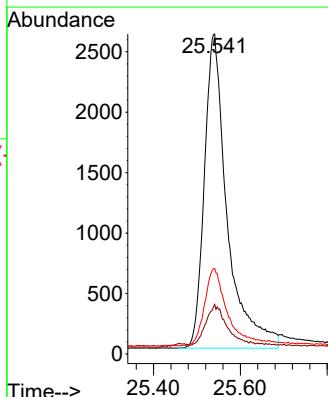

#37

Benzo(b)fluoranthene

Concen: 0.382 ng m

RT: 22.702 min Scan# 2

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N

ClientSampleId :

ICVBN062125

Tgt Ion:252 Resp: 8083

Ion Ratio Lower Upper

252 100

253 29.6 26.6 40.0


125 10.7 6.1 9.1

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

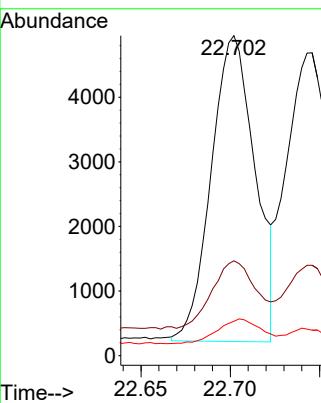

#38

Benzo(k)fluoranthene

Concen: 0.412 ng

RT: 22.746 min Scan# 2529

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39



Tgt Ion:252 Resp: 9472


Ion Ratio Lower Upper

252 100

253 29.9 26.7 40.1

125 8.4 6.5 9.7

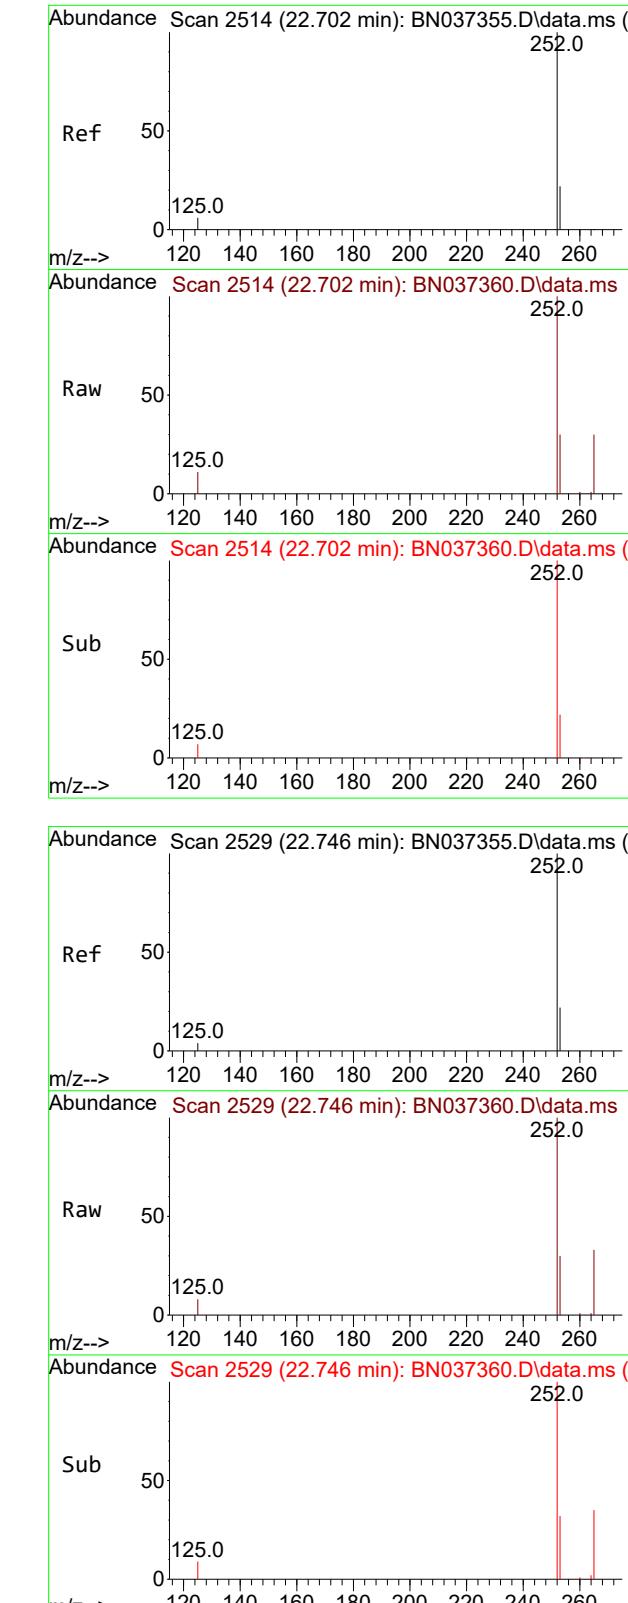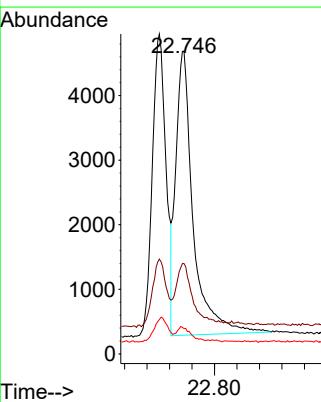


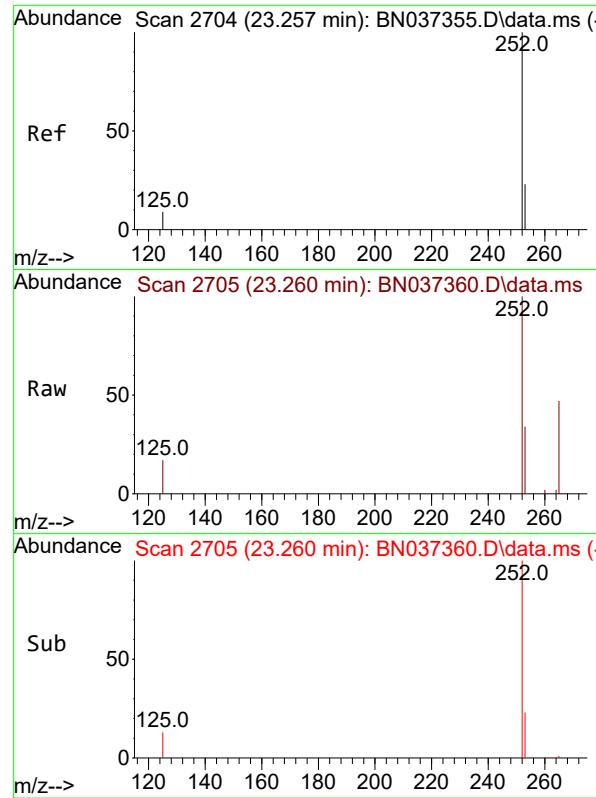


#39  
Benzo(a)pyrene  
Concen: 0.382 ng  
RT: 23.260 min Scan# 2  
Delta R.T. 0.003 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
ClientSampleId : ICVBN062125


**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

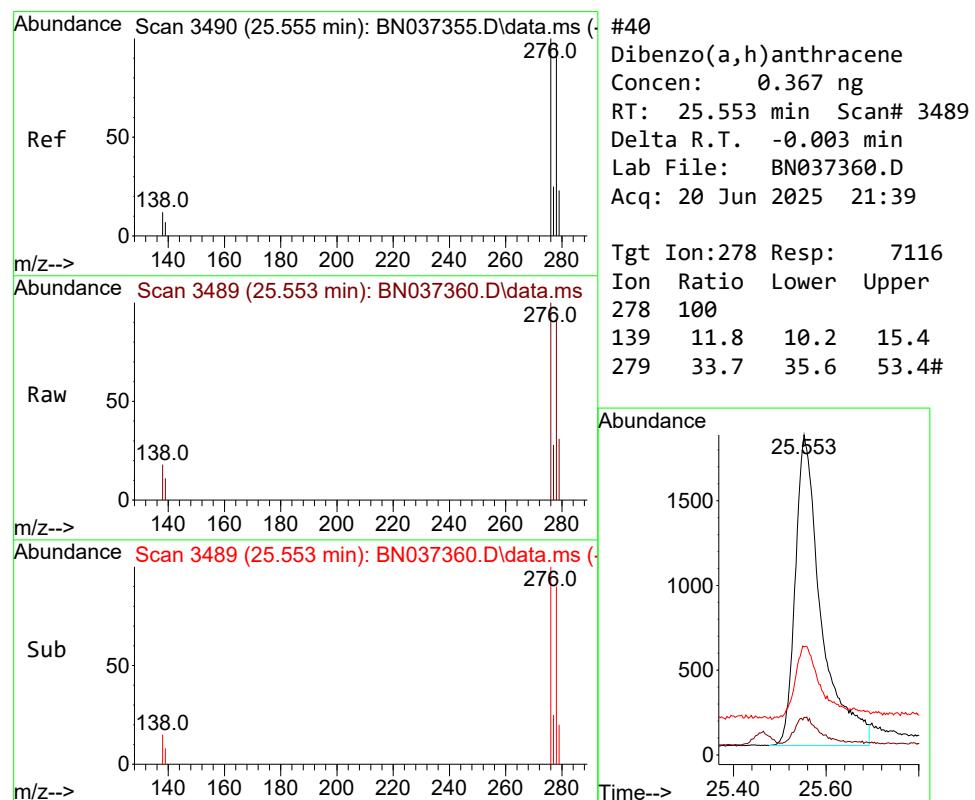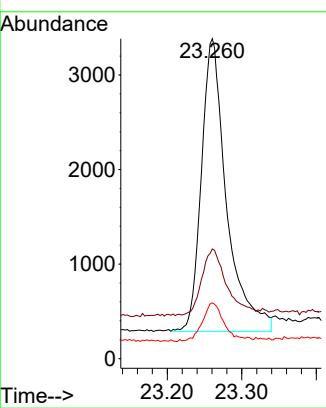

#40  
Dibenzo(a,h)anthracene  
Concen: 0.367 ng  
RT: 25.553 min Scan# 3489  
Delta R.T. -0.003 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Tgt Ion:278 Resp: 7116  
Ion Ratio Lower Upper  
278 100  
139 11.8 10.2 15.4  
279 33.7 35.6 53.4#

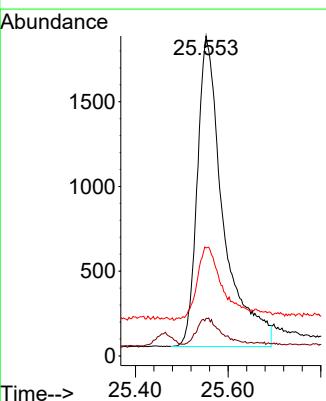

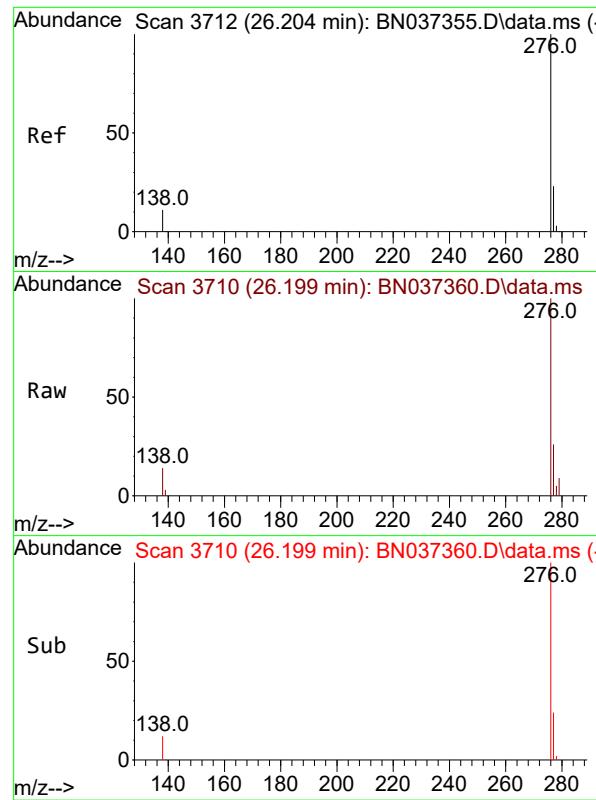

#41

Benzo(g,h,i)perylene

Concen: 0.378 ng

RT: 26.199 min Scan# 3

Delta R.T. -0.006 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N


ClientSampleId :

ICVBN062125

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

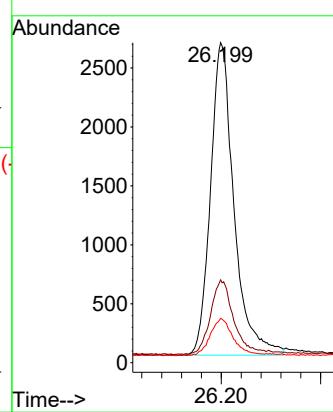

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037360.D  
 Acq On : 20 Jun 2025 21:39  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**ICVBN062125**

Quant Time: Jun 20 23:48:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	121	0.00
2	1,4-Dioxane	0.407	0.408	-0.2	126	0.00
3	n-Nitrosodimethylamine	0.373	0.366	1.9	112	0.00
4 S	2-Fluorophenol	0.799	0.797	0.3	128	0.00
5 S	Phenol-d6	0.823	0.778	5.5	123	0.00
6	bis(2-Chloroethyl)ether	0.730	0.744	-1.9	127	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	122	0.00
8 S	Nitrobenzene-d5	0.323	0.327	-1.2	125	0.00
9	Naphthalene	1.056	1.054	0.2	123	0.00
10	Hexachlorobutadiene	0.417	0.426	-2.2	118	0.00
11 SURR	2-Methylnaphthalene-d10	0.648	0.670	-3.4	123	0.00
12	2-Methylnaphthalene	0.736	0.715	2.9	122	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	123	0.00
14 S	2,4,6-Tribromophenol	0.235	0.219	6.8	117	0.00
15 S	2-Fluorobiphenyl	1.757	1.750	0.4	121	0.00
16	Acenaphthylene	1.682	1.580	6.1	122	0.00
17	Acenaphthene	1.107	1.076	2.8	125	0.00
18	Fluorene	1.556	1.502	3.5	123	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	122	0.00
20	4,6-Dinitro-2-methylphenol	0.096	0.069	28.1#	107	0.00
21	4-Bromophenyl-phenylether	0.285	0.270	5.3	118	0.00
22	Hexachlorobenzene	0.310	0.315	-1.6	122	0.00
23	Atrazine	0.227	0.206	9.3	115	0.00
24	Pentachlorophenol	0.154	0.125	18.8	111	0.00
25	Phenanthrene	1.158	1.096	5.4	121	0.00
26	Anthracene	1.068	0.954	10.7	118	0.00
27 SURR	Fluoranthene-d10	1.148	1.124	2.1	118	0.00
28	Fluoranthene	1.464	1.350	7.8	121	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	116	0.00
30	Pyrene	1.625	1.721	-5.9	120	0.00
31 S	Terphenyl-d14	0.912	0.947	-3.8	118	0.00
32	Benzo(a)anthracene	1.315	1.224	6.9	116	0.00
33	Chrysene	1.594	1.640	-2.9	118	0.00
34	Bis(2-ethylhexyl)phthalate	0.540	0.544	-0.7	116	0.00
35 I	Perylene-d12	1.000	1.000	0.0	116	0.00
36	Indeno(1,2,3-cd)pyrene	1.794	1.649	8.1	113	0.00
37	Benzo(b)fluoranthene	1.472	1.404	4.6	113	0.00
38	Benzo(k)fluoranthene	1.597	1.646	-3.1	122	0.00
39 C	Benzo(a)pyrene	1.319	1.261	4.4	115	0.00
40	Dibenzo(a,h)anthracene	1.348	1.236	8.3	117	0.00
41	Benzo(g,h,i)perylene	1.603	1.513	5.6	111	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037360.D  
 Acq On : 20 Jun 2025 21:39  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**ICVBN062125**

Quant Time: Jun 20 23:48:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	121	0.00
2	1,4-Dioxane	0.400	0.401	-0.3	126	0.00
3	n-Nitrosodimethylamine	0.400	0.393	1.8	112	0.00
4 S	2-Fluorophenol	0.400	0.399	0.3	128	0.00
5 S	Phenol-d6	0.400	0.378	5.5	123	0.00
6	bis(2-Chloroethyl)ether	0.400	0.407	-1.7	127	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	122	0.00
8 S	Nitrobenzene-d5	0.400	0.405	-1.3	125	0.00
9	Naphthalene	0.400	0.399	0.3	123	0.00
10	Hexachlorobutadiene	0.400	0.409	-2.2	118	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.414	-3.5	123	0.00
12	2-Methylnaphthalene	0.400	0.388	3.0	122	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	123	0.00
14 S	2,4,6-Tribromophenol	0.400	0.373	6.8	117	0.00
15 S	2-Fluorobiphenyl	0.400	0.398	0.5	121	0.00
16	Acenaphthylene	0.400	0.376	6.0	122	0.00
17	Acenaphthene	0.400	0.389	2.8	125	0.00
18	Fluorene	0.400	0.386	3.5	123	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	122	0.00
20	4,6-Dinitro-2-methylphenol	0.400	0.289	27.8#	107	0.00
21	4-Bromophenyl-phenylether	0.400	0.379	5.3	118	0.00
22	Hexachlorobenzene	0.400	0.406	-1.5	122	0.00
23	Atrazine	0.400	0.362	9.5	115	0.00
24	Pentachlorophenol	0.400	0.323	19.3	111	0.00
25	Phenanthrene	0.400	0.378	5.5	121	0.00
26	Anthracene	0.400	0.357	10.8	118	0.00
27 SURR	Fluoranthene-d10	0.400	0.392	2.0	118	0.00
28	Fluoranthene	0.400	0.369	7.8	121	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	116	0.00
30	Pyrene	0.400	0.424	-6.0	120	0.00
31 S	Terphenyl-d14	0.400	0.416	-4.0	118	0.00
32	Benzo(a)anthracene	0.400	0.372	7.0	116	0.00
33	Chrysene	0.400	0.412	-3.0	118	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.403	-0.8	116	0.00
35 I	Perylene-d12	0.400	0.400	0.0	116	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.368	8.0	113	0.00
37	Benzo(b)fluoranthene	0.400	0.382	4.5	113	0.00
38	Benzo(k)fluoranthene	0.400	0.412	-3.0	122	0.00
39 C	Benzo(a)pyrene	0.400	0.382	4.5	115	0.00
40	Dibenzo(a,h)anthracene	0.400	0.367	8.3	117	0.00
41	Benzo(g,h,i)perylene	0.400	0.378	5.5	111	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Method Path : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\  
 Method File : 8270-SIM-BN062625.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jun 26 16:06:33 2025  
 Response Via : Initial Calibration

## Calibration Files

0.1 =BN037386.D 0.2 =BN037387.D 0.4 =BN037388.D 0.8 =BN037389.D 1.6 =BN037390.D 3.2 =BN037391.D 5 =BN037392.D

Compound	0.1	0.2	0.4	0.8	1.6	3.2	5	Avg	%RSD
----------	-----	-----	-----	-----	-----	-----	---	-----	------

1) I	1,4-Dichlorobenzene	-----	ISTD-----						
2)	1,4-Dioxane	0.470	0.369	0.366	0.377	0.363	0.331	0.379	12.38
3)	n-Nitrosodimethylamine	0.377	0.374	0.366	0.385	0.374	0.371	0.375	1.73
4) S	2-Fluorophenol	0.771	0.778	0.804	0.697	0.754	0.773	0.818	0.771
5) S	Phenol-d6	0.663	0.706	0.812	0.737	0.839	0.886	0.951	0.799
6)	bis(2-Chloroethyl)ether	0.574	0.661	0.718	0.694	0.765	0.775	0.790	0.711
7) I	Naphthalene-d8	-----	ISTD-----						
8) S	Nitrobenzene-d5	0.270	0.281	0.311	0.296	0.345	0.353	0.389	0.321
9)	Naphthalene	1.042	1.001	0.999	0.972	1.048	1.050	1.096	1.030
10)	Hexachlorobutane	0.407	0.410	0.413	0.400	0.422	0.404	0.405	0.409
11)	SURR2-Methylnaphthalene	0.532	0.567	0.576	0.568	0.628	0.656	0.807	0.619
12)	2-Methylnaphthalene	0.635	0.665	0.684	0.662	0.746	0.767	0.803	0.709
13) I	Acenaphthene-d10	-----	ISTD-----						
14) S	2,4,6-Tribromoethane	0.194	0.207	0.239	0.225	0.251	0.256	0.271	0.235
15) S	2-Fluorobiphenyl	1.548	1.656	1.723	1.652	1.798	1.801	1.910	1.727
16)	Acenaphthylene	1.585	1.600	1.576	1.538	1.714	1.741	1.858	1.659
17)	Acenaphthene	1.030	1.027	1.045	1.009	1.123	1.147	1.203	1.083
18)	Fluorene	1.444	1.417	1.476	1.420	1.603	1.643	1.706	1.530
19) I	Phenanthrene-d10	-----	ISTD-----						
20)	4,6-Dinitro-2-phenol	0.084	0.085	0.087	0.113	0.119	0.128	0.103	19.13
21)	4-Bromophenylmethanol	0.264	0.253	0.270	0.269	0.303	0.302	0.316	0.282
22)	Hexachlorobenzene	0.310	0.299	0.302	0.291	0.311	0.301	0.311	0.303
23)	Atrazine	0.200	0.208	0.213	0.204	0.232	0.242	0.266	0.224
24)	Pentachlorophenol	0.164	0.155	0.148	0.165	0.168	0.183	0.164	7.30
25)	Phenanthrene	1.056	1.067	1.080	1.038	1.172	1.190	1.287	1.127
26)	Anthracene	0.935	0.972	0.969	0.959	1.076	1.120	1.222	1.036
27)	SURRFluoranthene-d10	1.073	1.137	1.063	1.028	1.121	1.154	1.447	1.146
28)	Fluoranthene	1.377	1.398	1.362	1.320	1.487	1.507	1.624	1.439
29) I	Chrysene-d12	-----	ISTD-----						
30)	Pyrene	1.459	1.449	1.534	1.431	1.561	1.550	1.612	1.514
31) S	Terphenyl-d14	0.800	0.794	0.868	0.796	0.878	0.892	0.943	0.853
32)	Benzo(a)anthracene	1.149	1.202	1.167	1.152	1.318	1.364	1.446	1.257
33)	Chrysene	1.630	1.573	1.583	1.491	1.554	1.510	1.551	1.556
34)	Bis(2-ethylhexyl)phthalate	0.509	0.504	0.466	0.481	0.488	0.537	0.498	5.00
35) I	Perylene-d12	-----	ISTD-----						

Method Path : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\  
Method File : 8270-SIM-BN062625.M  
36) Indeno(1,2,3-c...) 1.487 1.515 1.577 1.620 1.786 1.853 1.967 1.686 10.88  
37) Benzo(b)fluora... 1.329 1.305 1.318 1.320 1.464 1.504 1.632 1.410 8.93  
38) Benzo(k)fluora... 1.408 1.389 1.462 1.430 1.552 1.613 1.697 1.507 7.73  
39) C Benzo(a)pyrene 1.211 1.160 1.183 1.174 1.286 1.341 1.426 1.254 8.01  
40) Dibenzo(a,h)an... 1.050 1.138 1.211 1.229 1.394 1.485 1.561 1.296 14.53  
41) Benzo(g,h,i)pe... 1.425 1.473 1.477 1.462 1.617 1.658 1.725 1.548 7.51

---

(#) = Out of Range

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037386.D  
 Acq On : 26 Jun 2025 10:41  
 Operator : RC/JU  
 Sample : SSTDICCO.1  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCO.1

Quant Time: Jun 26 16:03:56 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:02:41 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/27/2025  
 Supervised By :Jagrut Upadhyay 06/27/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.560	152	2183	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4628	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	2945	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5811	0.400	ng	0.01
29) Chrysene-d12	21.171	240	5498	0.400	ng	0.00
35) Perylene-d12	23.348	264	5798	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	421	0.100	ng	0.00
5) Phenol-d6	6.744	99	362	0.083	ng	0.00
8) Nitrobenzene-d5	8.728	82	312m	0.085	ng	0.01
11) 2-Methylnaphthalene-d10	11.955	152	615	0.086	ng	0.02
14) 2,4,6-Tribromophenol	15.730	330	143	0.083	ng	0.01
15) 2-Fluorobiphenyl	12.843	172	1140	0.090	ng	0.01
27) Fluoranthene-d10	19.008	212	1559	0.094	ng	0.00
31) Terphenyl-d14	19.625	244	1099	0.094	ng	0.00
<b>Target Compounds</b>						
6) bis(2-Chloroethyl)ether	7.004	93	313	0.081	ng	# 85
9) Naphthalene	10.394	128	1206	0.101	ng	# 86
10) Hexachlorobutadiene	10.682	225	471	0.100	ng	# 98
12) 2-Methylnaphthalene	12.026	142	735	0.090	ng	96
16) Acenaphthylene	13.935	152	1167	0.096	ng	97
17) Acenaphthene	14.277	154	758	0.095	ng	98
18) Fluorene	15.272	166	1063	0.094	ng	100
21) 4-Bromophenyl-phenylether	16.177	248	383	0.093	ng	# 93
22) Hexachlorobenzene	16.276	284	450	0.102	ng	98
23) Atrazine	16.462	200	291	0.090	ng	# 73
25) Phenanthrene	17.009	178	1534	0.094	ng	97
26) Anthracene	17.108	178	1358	0.090	ng	100
28) Fluoranthene	19.040	202	2001	0.096	ng	99
30) Pyrene	19.402	202	2006	0.096	ng	99
32) Benzo(a)anthracene	21.153	228	1579	0.091	ng	92
33) Chrysene	21.198	228	2241	0.105	ng	94
36) Indeno(1,2,3-cd)pyrene	25.535	276	2156	0.088	ng	# 90
37) Benzo(b)fluoranthene	22.699	252	1927	0.094	ng	# 66
38) Benzo(k)fluoranthene	22.740	252	2041	0.093	ng	# 61
39) Benzo(a)pyrene	23.254	252	1755	0.097	ng	# 52
40) Dibenzo(a,h)anthracene	25.567	278	1522	0.081	ng	# 41
41) Benzo(g,h,i)perylene	26.193	276	2066	0.092	ng	# 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037386.D  
 Acq On : 26 Jun 2025 10:41  
 Operator : RC/JU  
 Sample : SSTDICC0.1  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1


Quant Time: Jun 26 16:03:56 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:02:41 2025  
 Response via : Initial Calibration

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC0.1

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/27/2025  
 Supervised By :Jagrut Upadhyay 06/27/2025

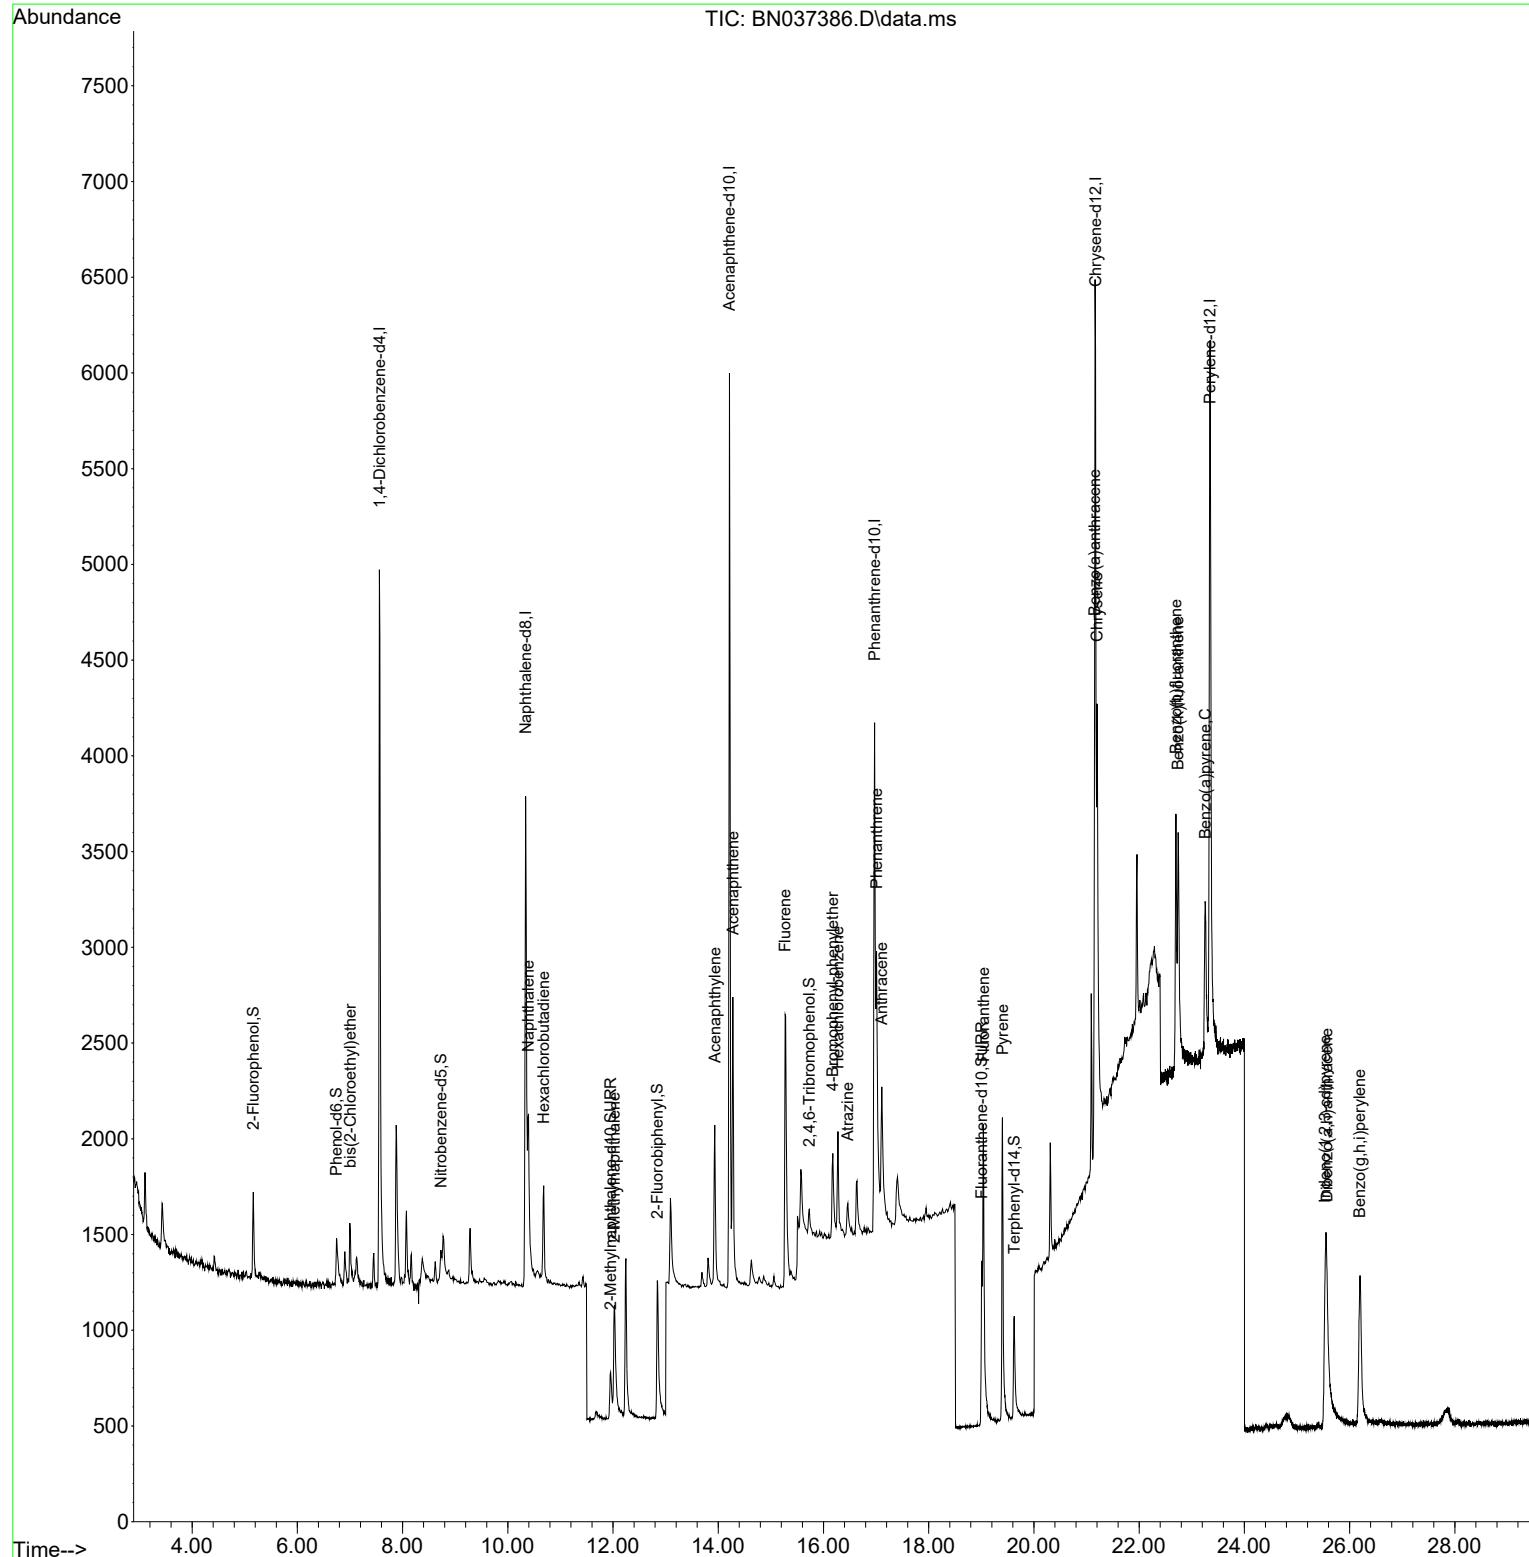


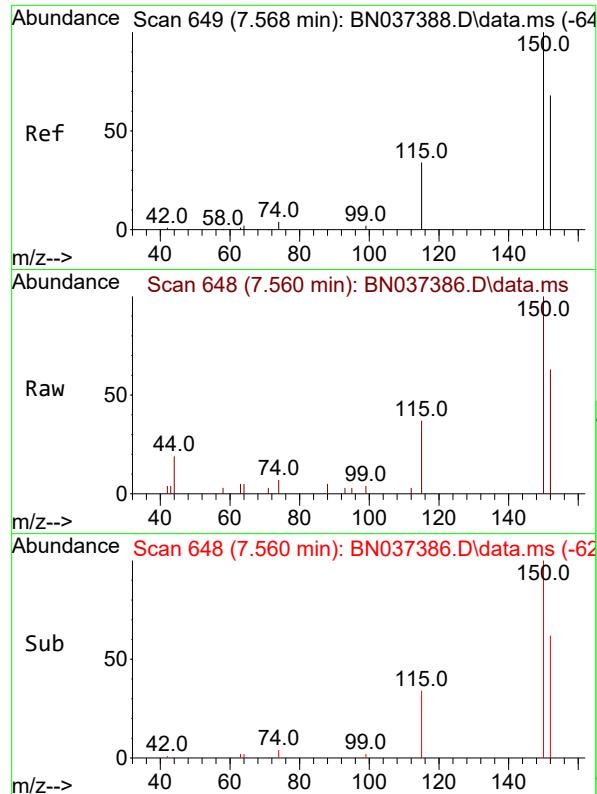


#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.560 min Scan# 6  
Delta R.T. -0.008 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025

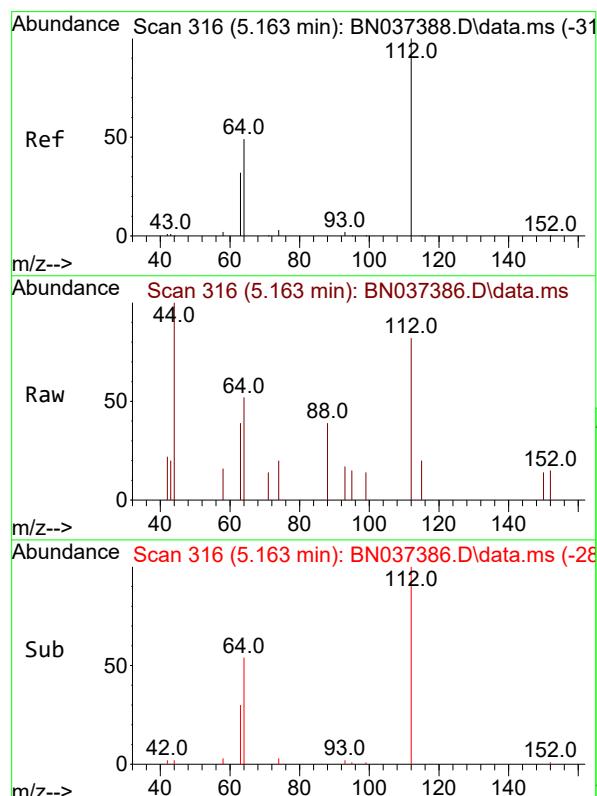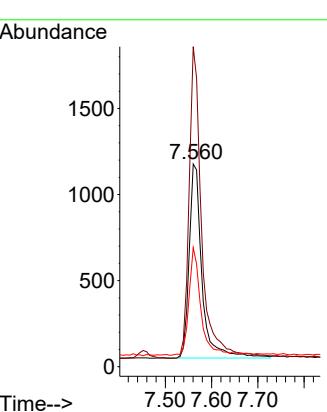

#4  
2-Fluorophenol  
Concen: 0.100 ng  
RT: 5.163 min Scan# 316  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt Ion:112 Resp: 421  
Ion Ratio Lower Upper  
112 100  
64 50.6 40.3 60.5  
63 34.0 26.1 39.1

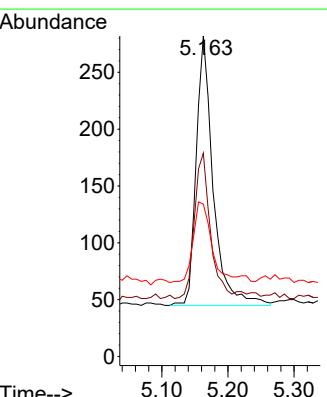







#5  
Phenol-d6  
Concen: 0.083 ng  
RT: 6.744 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1

Tgt	Ion:	99	Resp:	362
Ion	Ratio	Lower	Upper	
99	100			
42	19.6	15.6	23.4	
71	43.6	35.8	53.8	




### Manual Integrations APPROVED


Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025

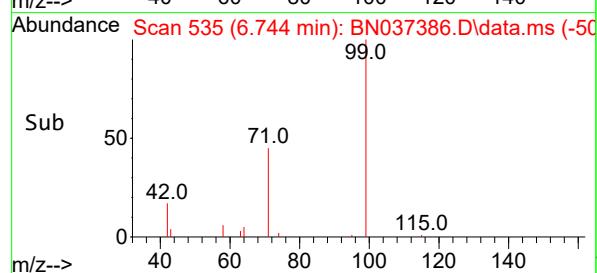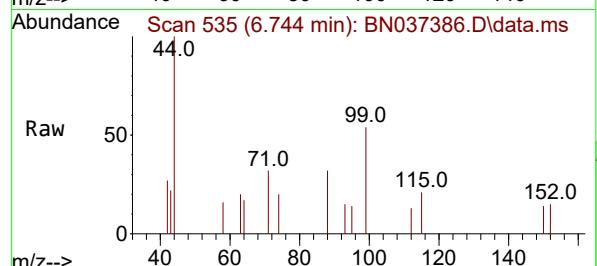

#6  
bis(2-Chloroethyl)ether  
Concen: 0.081 ng  
RT: 7.004 min Scan# 571  
Delta R.T. 0.007 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41



Tgt	Ion:	93	Resp:	313
Ion	Ratio	Lower	Upper	
93	100			
63	75.1	49.6	74.4	#
95	35.5	23.9	35.9	






#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.340 min Scan# 9  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1




Tgt Ion:136 Resp: 4623

	Ion Ratio	Lower	Upper
136	100		
137	12.8	10.4	15.6
54	8.0	5.6	8.4
68	6.4	4.6	6.8

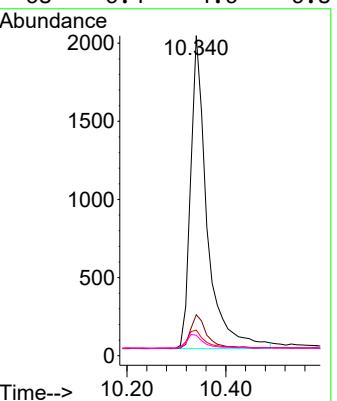


Manual Integrations  
APPROVED



Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025




#8  
Nitrobenzene-d5  
Concen: 0.085 ng m  
RT: 8.728 min Scan# 791  
Delta R.T. 0.011 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41



Tgt Ion: 82 Resp: 312  
Ion Ratio Lower Upper  
82 100  
128 65.4 34.0 51.0#  
54 65.4 37.7 56.5#

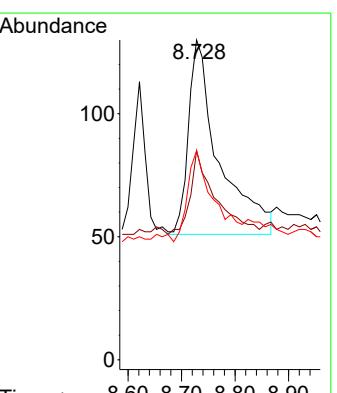



#9

Naphthalene

Concen: 0.101 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037386.D


Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N

ClientSampleId :



SSTDICCO.1

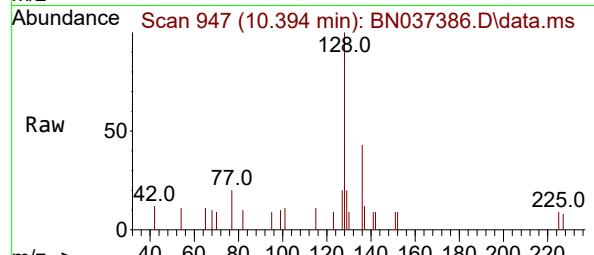

Tgt	Ion:128	Resp:	1200
Ion Ratio	Lower	Upper	
128	100		
129	19.9	10.4	15.6
127	20.3	12.2	18.4



### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025

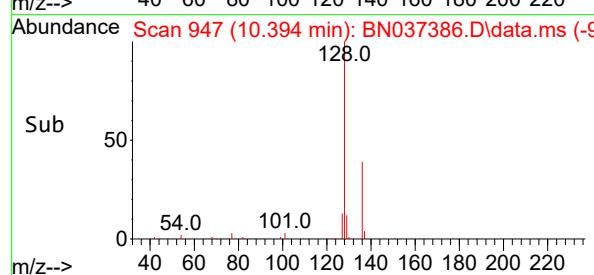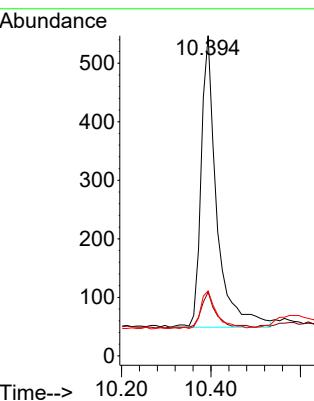







#10  
Hexachlorobutadiene  
Concen: 0.100 ng  
RT: 10.682 min Scan# 974  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt	Ion:225	Resp:	471
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	60.7	49.9	74.9

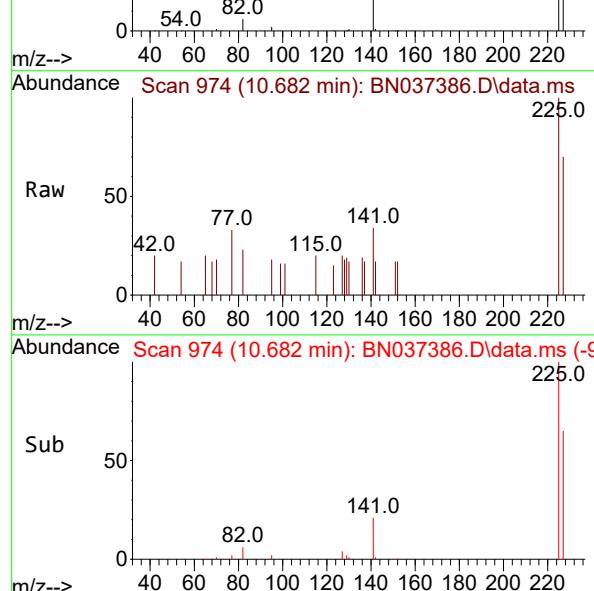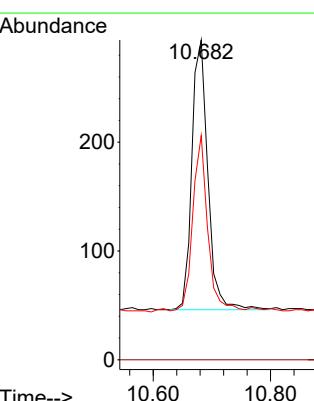

Sub 50

225.0  
82.0  
141.0

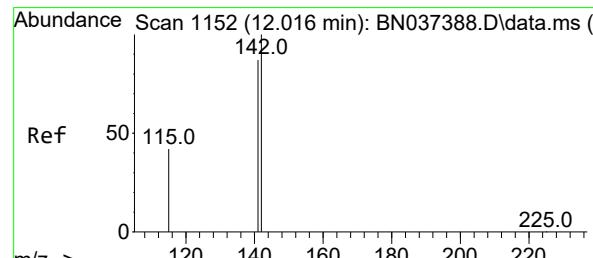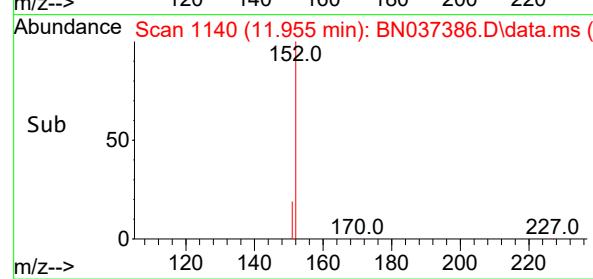

#11

2-Methylnaphthalene-d10  
Concen: 0.086 ng

RT: 11.955 min Scan# 1137

Delta R.T. 0.015 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41


Instrument : BNA\_N

ClientSampleId : SSTDICCO.1

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/27/2025


Supervised By :Jagrut Upadhyay 06/27/2025

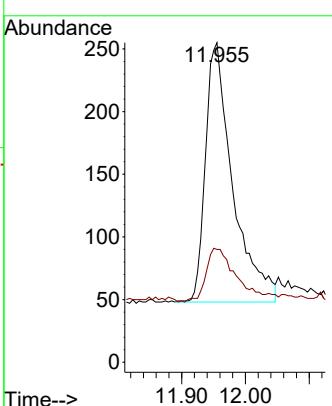


#12



2-Methylnaphthalene  
Concen: 0.090 ng  
RT: 12.026 min Scan# 1154  
Delta R.T. 0.010 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt Ion:142 Resp: 735  
Ion Ratio Lower Upper  
142 100  
141 85.4 70.1 105.1  
115 49.2 35.8 53.6

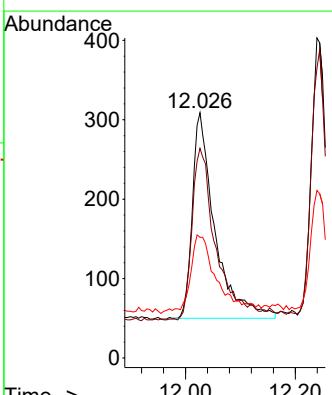







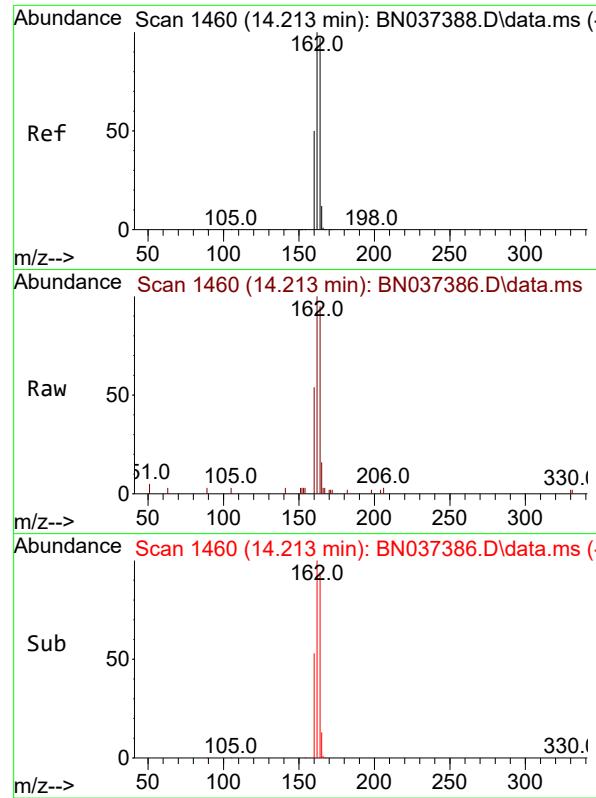


#13

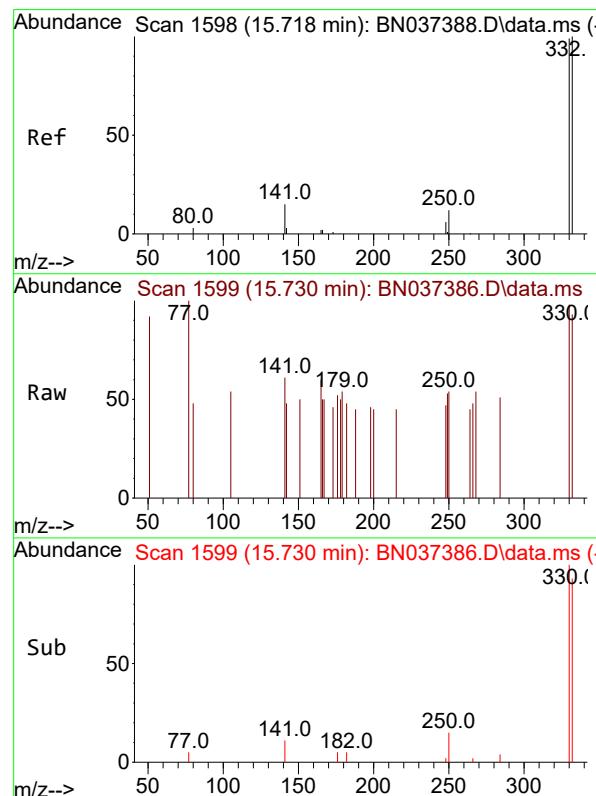Acenaphthene-d10  
Concen: 0.400 ngRT: 14.213 min Scan# 1460  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1**Manual Integrations  
APPROVED**Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025

#14

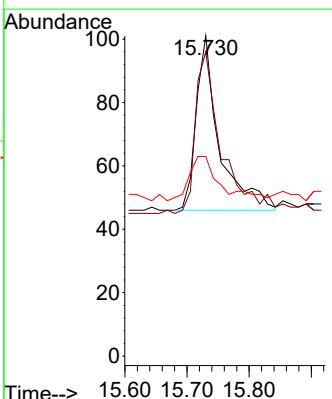2,4,6-Tribromophenol  
Concen: 0.083 ng  
RT: 15.730 min Scan# 1599  
Delta R.T. 0.012 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41Tgt Ion:330 Resp: 143  
Ion Ratio Lower Upper  
330 100  
332 107.7 77.8 116.8  
141 33.6 24.0 36.0



#15

2-Fluorobiphenyl

Concen: 0.090 ng

RT: 12.843 min Scan# 1313

Delta R.T. 0.010 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.1

Tgt Ion:172 Resp: 1140

Ion Ratio Lower Upper

172 100

171 40.4 28.8 43.2


170 30.3 20.3 30.5

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/27/2025

Supervised By :Jagrut Upadhyay 06/27/2025



#16  
Acenaphthylene  
Concen: 0.096 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41


Tgt Ion:152 Resp: 1167




Ion Ratio Lower Upper

152 100

151 21.9 15.8 23.6

153 13.1 10.3 15.5



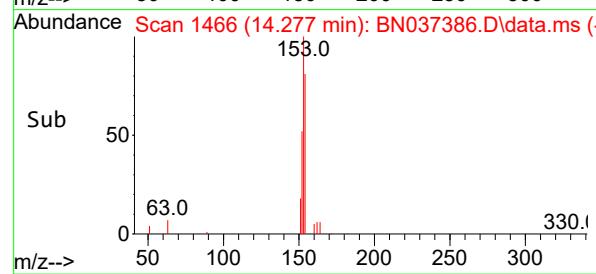

#17

Acenaphthene

Concen: 0.095 ng

RT: 14.277 min Scan# 1466

Delta R.T. -0.000 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N




ClientSampleId :

SSTDICCO.1

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/27/2025

Supervised By :Jagrut Upadhyay 06/27/2025

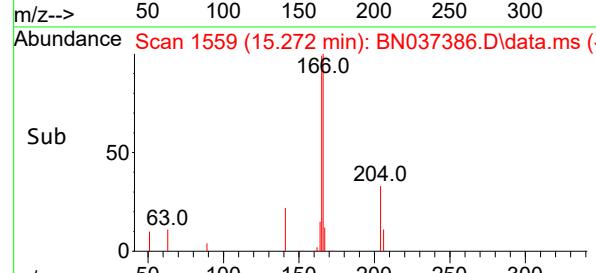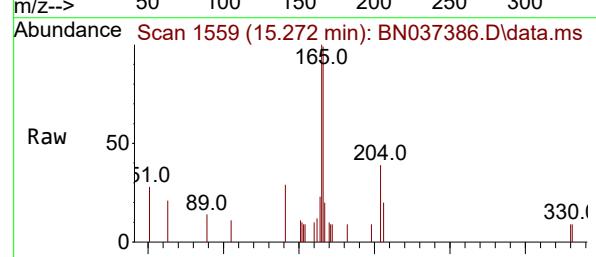

#18

Fluorene

Concen: 0.094 ng

RT: 15.272 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41


Tgt Ion:166 Resp: 1063


Ion Ratio Lower Upper

166 100

165 99.1 79.4 119.2

167 12.2 10.6 15.8

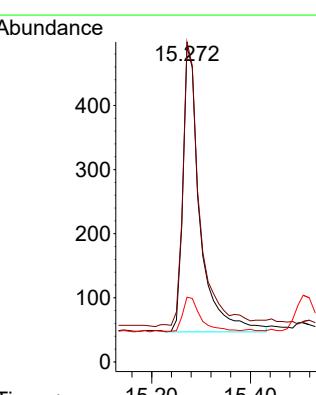

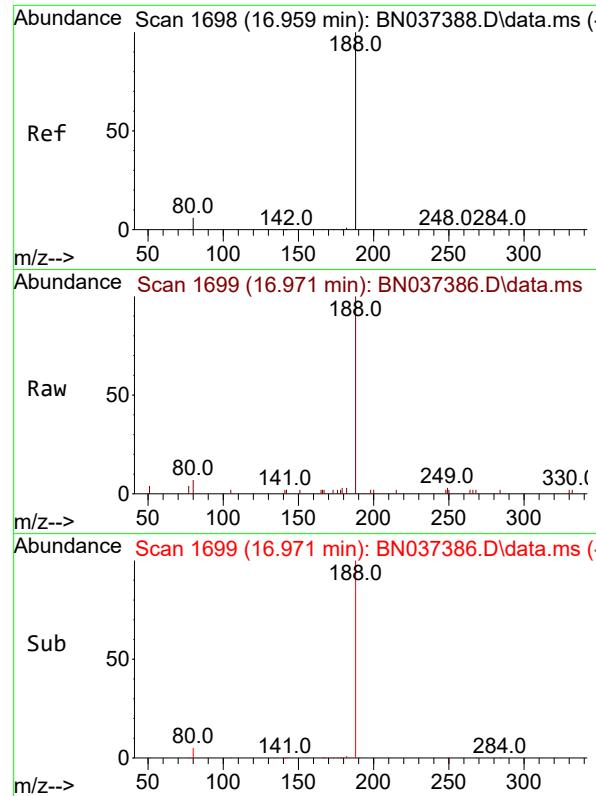

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. 0.012 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N



ClientSampleId :

SSTDICCO.1

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/27/2025

Supervised By :Jagrut Upadhyay 06/27/2025

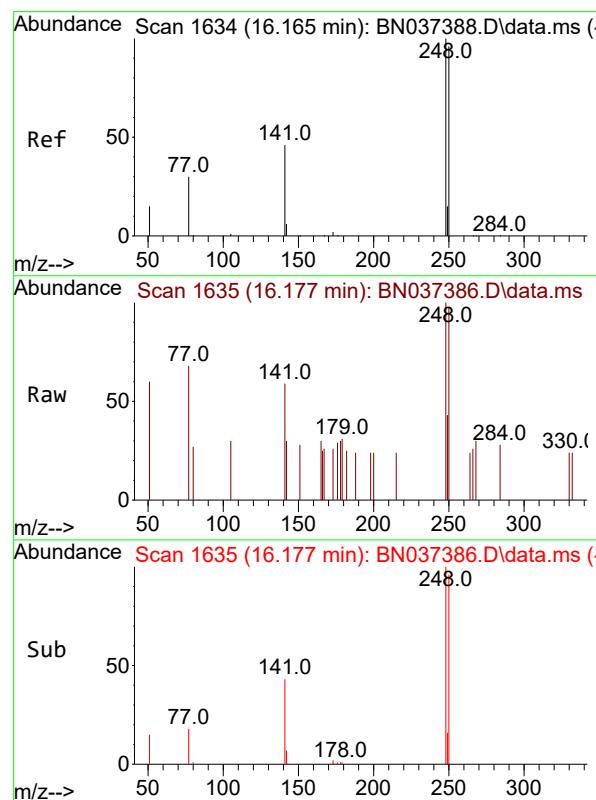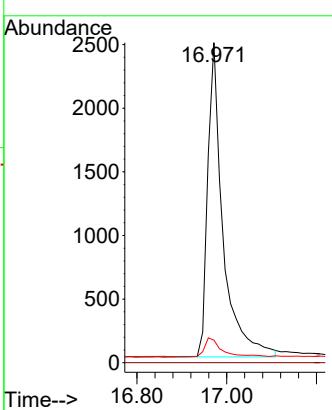

#21

4-Bromophenyl-phenylether

Concen: 0.093 ng

RT: 16.177 min Scan# 1635

Delta R.T. 0.012 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41


Tgt Ion:248 Resp: 383


Ion Ratio Lower Upper

248 100

250 98.4 77.0 115.4

141 58.7 38.7 58.1#



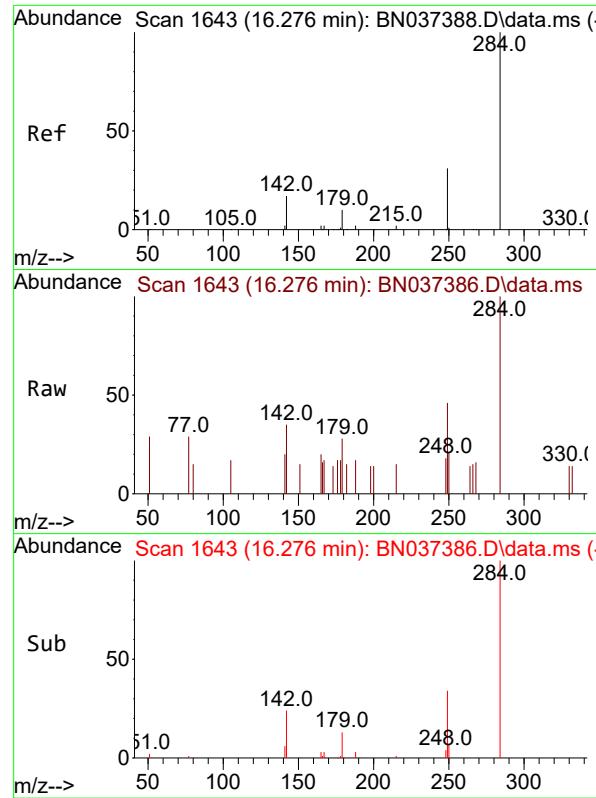

#22

Hexachlorobenzene

Concen: 0.102 ng

RT: 16.276 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N


ClientSampleId :

SSTDICC0.1

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/27/2025

Supervised By :Jagrut Upadhyay 06/27/2025

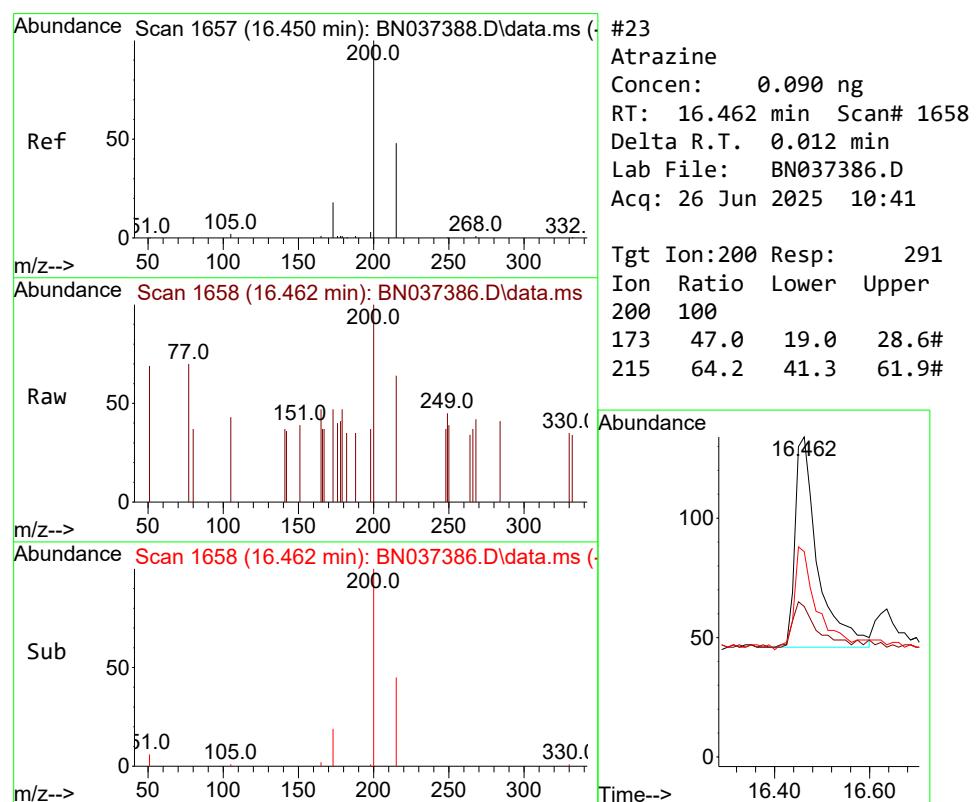

#23

Atrazine

Concen: 0.090 ng

RT: 16.462 min Scan# 1658

Delta R.T. 0.012 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41


Tgt Ion:200 Resp: 291




Ion Ratio Lower Upper

200 100

173 47.0 19.0 28.6#

215 64.2 41.3 61.9#

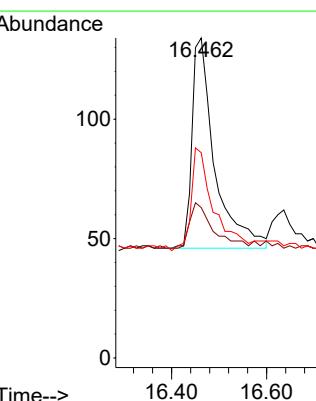

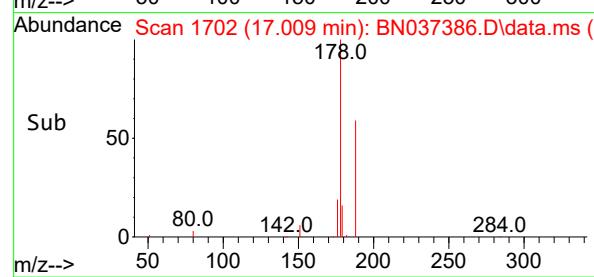

#25

Phenanthrene

Concen: 0.094 ng

RT: 17.009 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N





ClientSampleId :

SSTDICCO.1

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/27/2025

Supervised By :Jagrut Upadhyay 06/27/2025

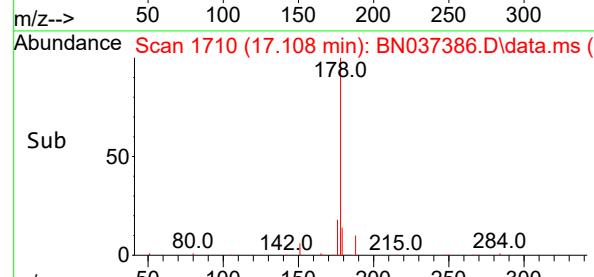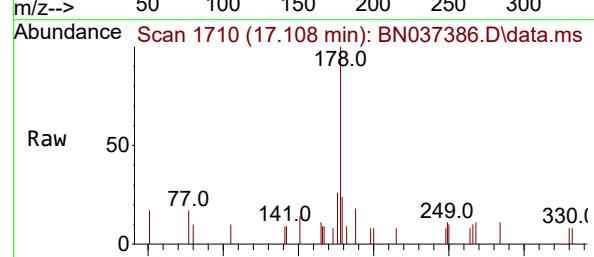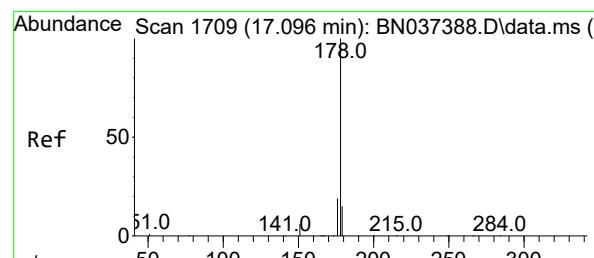

#26

Anthracene

Concen: 0.090 ng


RT: 17.108 min Scan# 1710


Delta R.T. 0.012 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Tgt	Ion:178	Resp:	1358
Ion	Ratio	Lower	Upper
178	100		
176	18.6	14.9	22.3
179	15.2	12.4	18.6

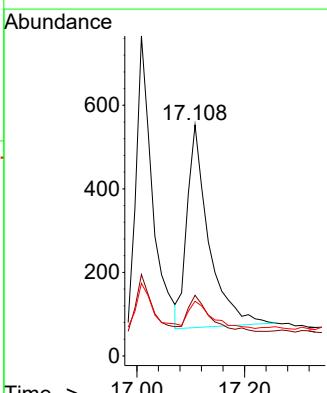


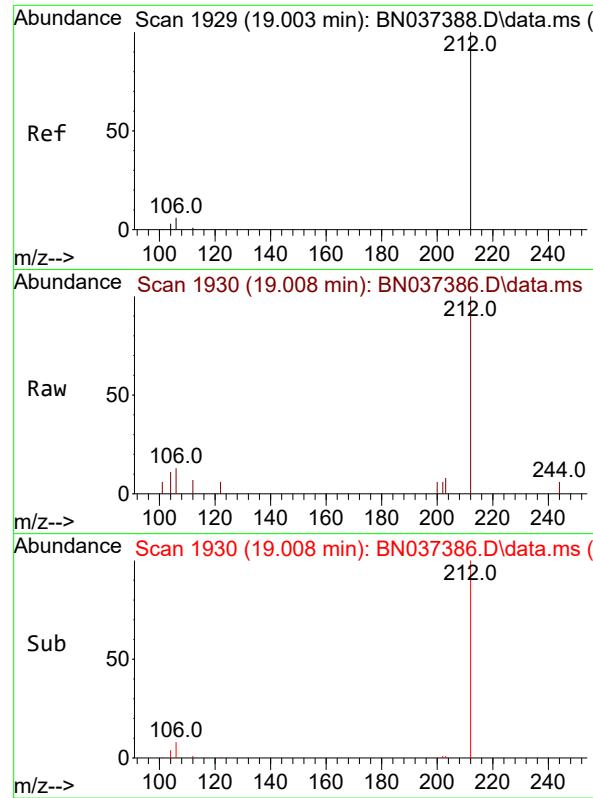


#27  
**Fluoranthene-d10**  
Concen: 0.094 ng  
RT: 19.008 min Scan# 1  
Delta R.T. 0.005 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


1 Manual Integrations  
2 APPROVED




3 Reviewed By :Rahul Chavli 06/27/2025  
4 Supervised By :Jagrut Upadhyay 06/27/2025

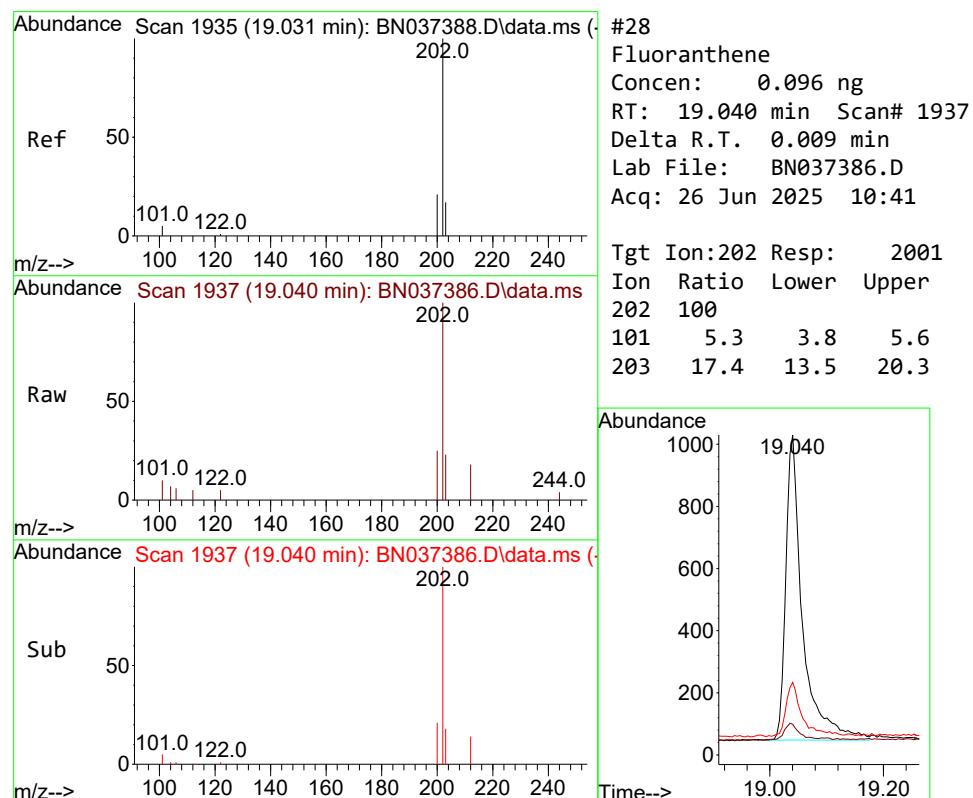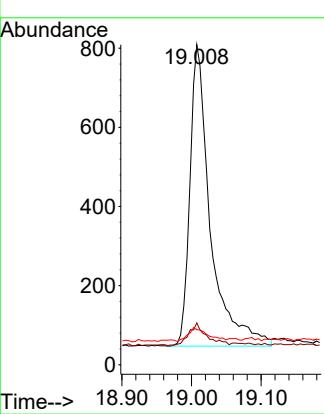

#28  
**Fluoranthene**  
Concen: 0.096 ng  
RT: 19.040 min Scan# 1937  
Delta R.T. 0.009 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt Ion:202 Resp: 2001  
Ion Ratio Lower Upper  
202 100  
101 5.3 3.8 5.6  
203 17.4 13.5 20.3

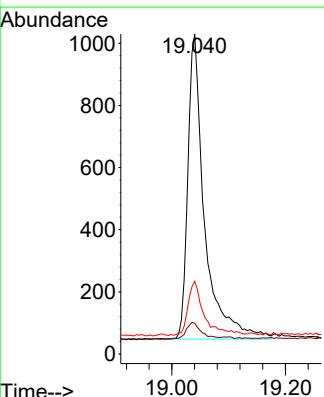



#29

Chrysene-d<sub>12</sub>

Concen: 0.400 ng

RT: 21.171 min Scan# 2

Delta R.T. 0.009 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N





ClientSampleId :

SSTDICCO.1

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/27/2025

Supervised By :Jagrut Upadhyay 06/27/2025

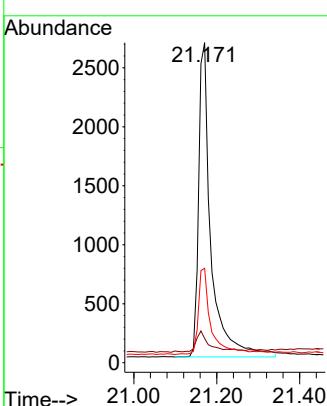

#30

Pyrene

Concen: 0.096 ng


RT: 19.402 min Scan# 2015


Delta R.T. 0.005 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Tgt	Ion:202	Resp:	2006
Ion	Ratio	Lower	Upper
202	100		
200	21.0	16.5	24.7
203	18.0	14.2	21.2

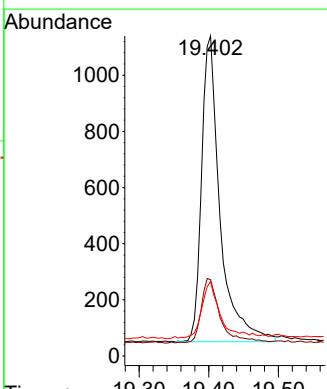


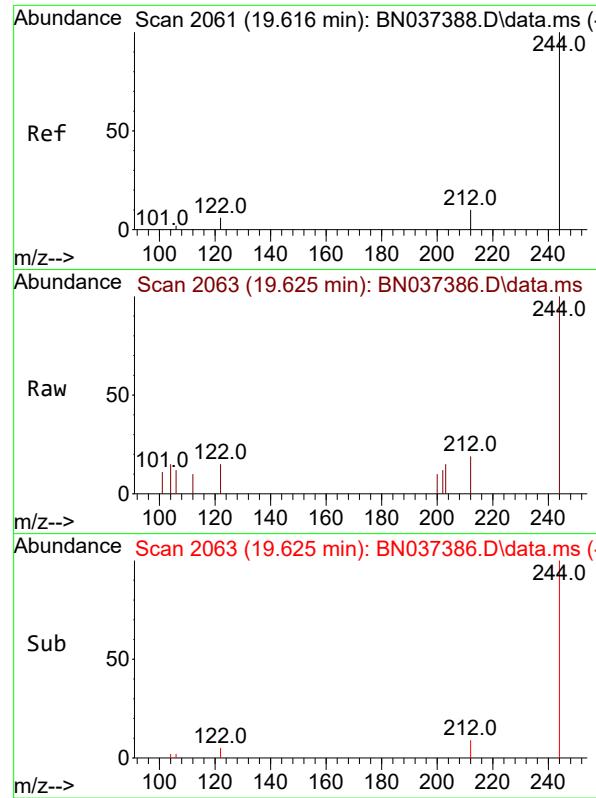


Terphenyl-d14  
Concen: 0.094 ng  
RT: 19.625 min Scan# 21099  
Delta R.T. 0.009 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025

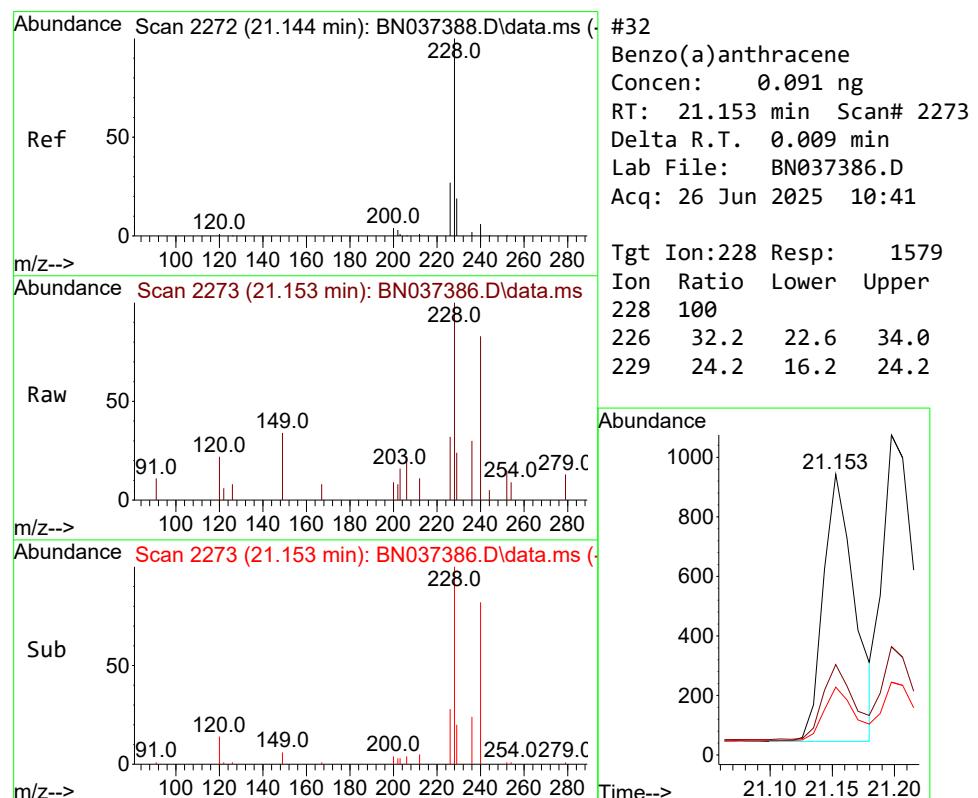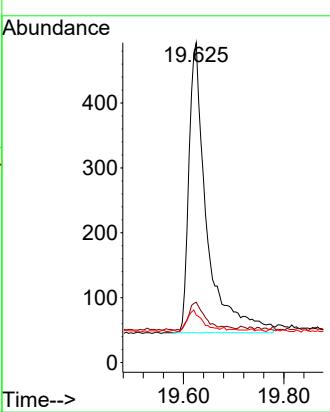

Benzo(a)anthracene  
Concen: 0.091 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.009 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt Ion:228 Resp: 1579  
Ion Ratio Lower Upper  
228 100  
226 32.2 22.6 34.0  
229 24.2 16.2 24.2

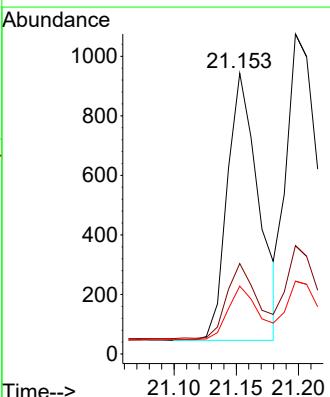



#33

Chrysene

Concen: 0.105 ng

RT: 21.198 min Scan# 2

Delta R.T. -0.000 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41

Instrument :

BNA\_N




ClientSampleId :

SSTDICCO.1

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/27/2025

Supervised By :Jagrut Upadhyay 06/27/2025



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.348 min Scan# 2735

Delta R.T. 0.003 min

Lab File: BN037386.D

Acq: 26 Jun 2025 10:41


Tgt Ion:264 Resp: 5798


Ion Ratio Lower Upper

264 100

260 26.9 21.4 32.0

265 77.1 56.2 84.4

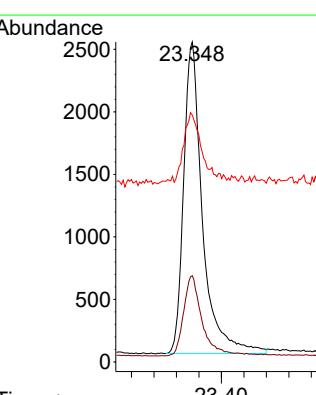


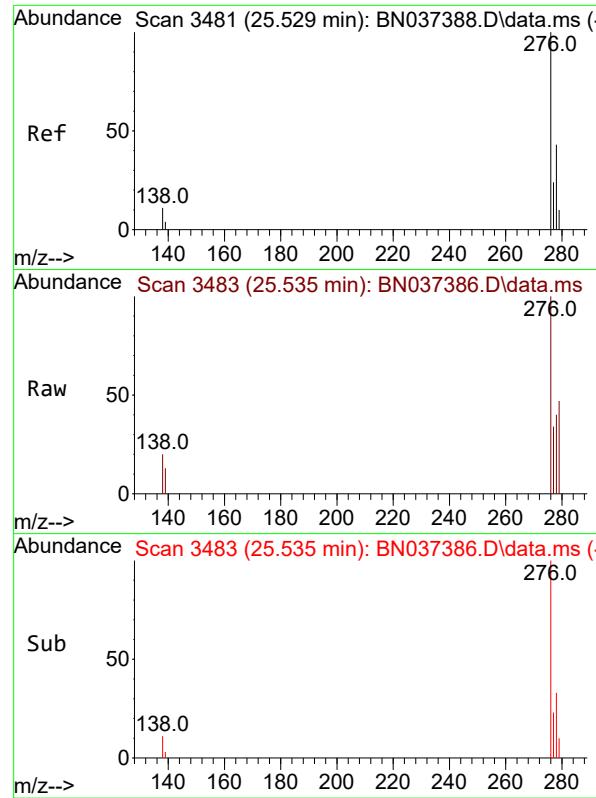


#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.088 ng  
RT: 25.535 min Scan# 3481  
Delta R.T. 0.006 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025

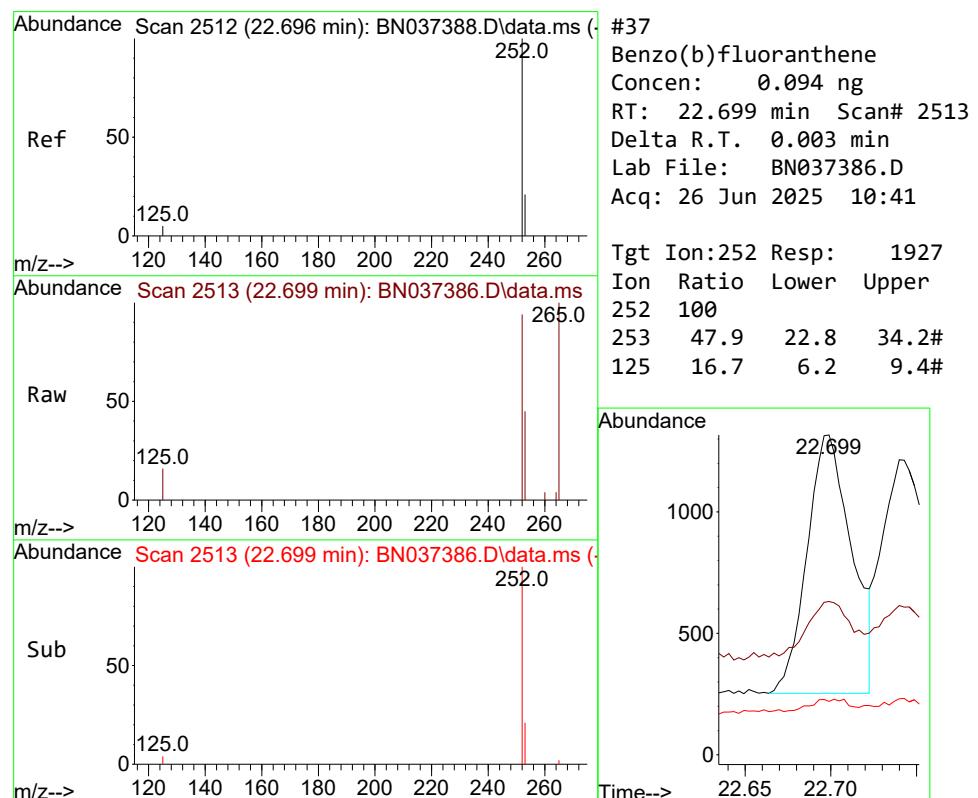

#37  
Benzo(b)fluoranthene  
Concen: 0.094 ng  
RT: 22.699 min Scan# 2513  
Delta R.T. 0.003 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt Ion:252 Resp: 1927  
Ion Ratio Lower Upper  
252 100  
253 47.9 22.8 34.2#  
125 16.7 6.2 9.4#

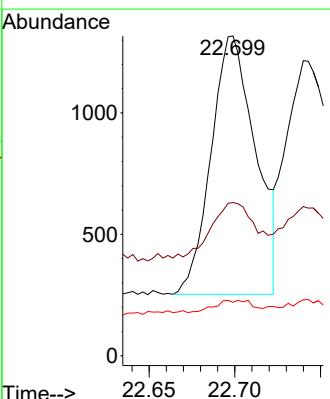


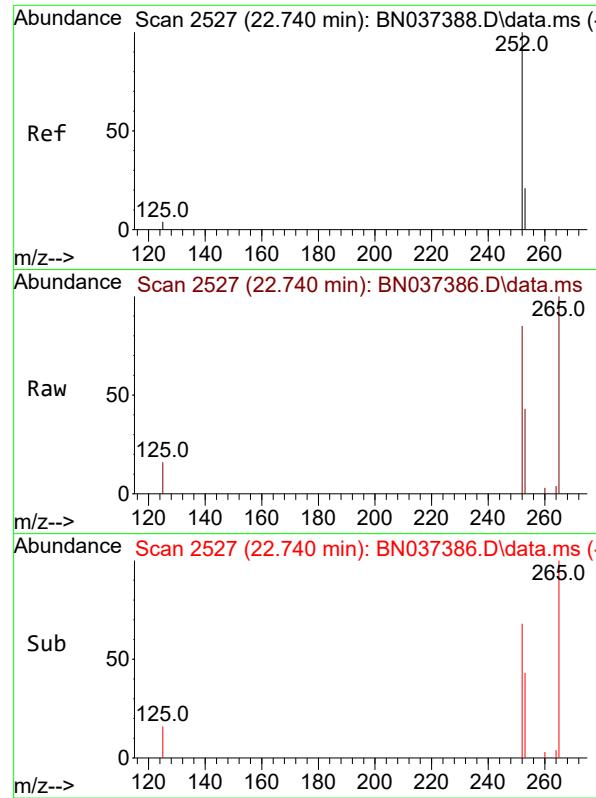


#38  
 Benzo(k)fluoranthene  
 Concen: 0.093 ng  
 RT: 22.740 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/27/2025  
 Supervised By :Jagrut Upadhyay 06/27/2025

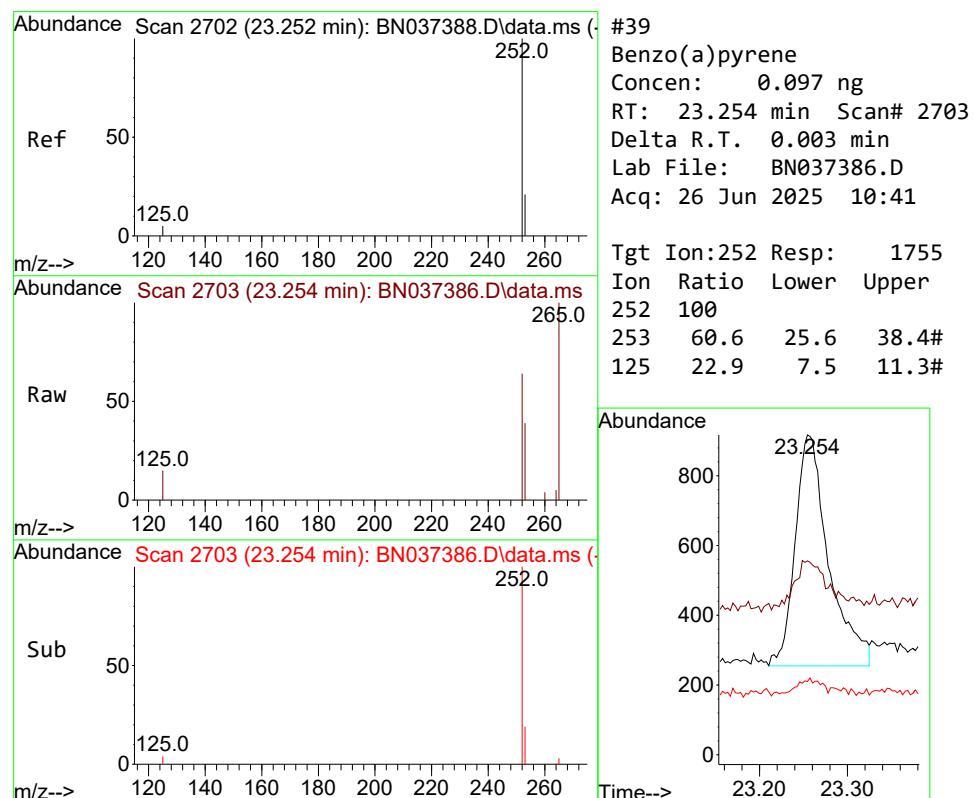

#39  
 Benzo(a)pyrene  
 Concen: 0.097 ng  
 RT: 23.254 min Scan# 2703  
 Delta R.T. 0.003 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Tgt Ion:252 Resp: 1755  
 Ion Ratio Lower Upper  
 252 100  
 253 60.6 25.6 38.4#  
 125 22.9 7.5 11.3#

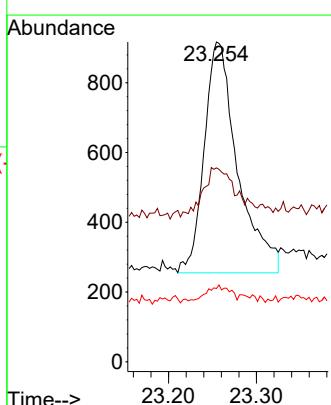


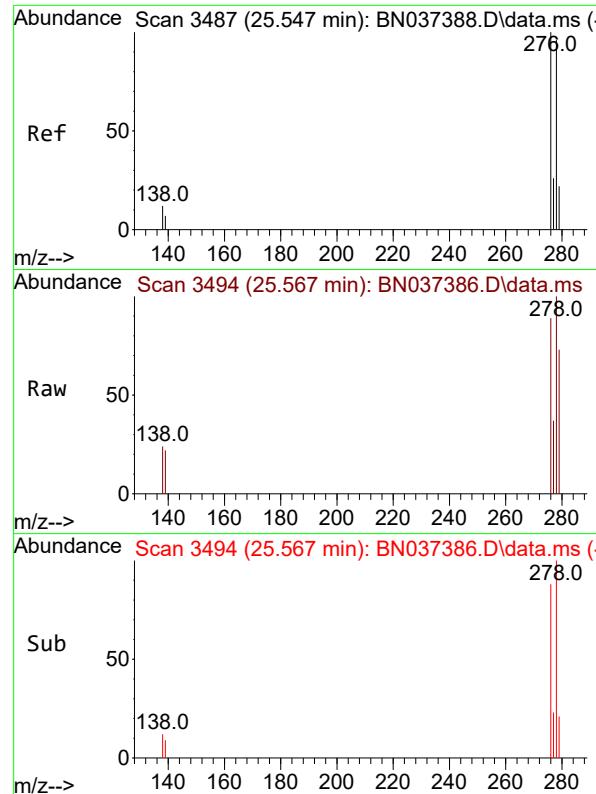


#40  
Dibenzo(a,h)anthracene  
Concen: 0.081 ng  
RT: 25.567 min Scan# 3  
Delta R.T. 0.020 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1


**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/27/2025  
Supervised By :Jagrut Upadhyay 06/27/2025

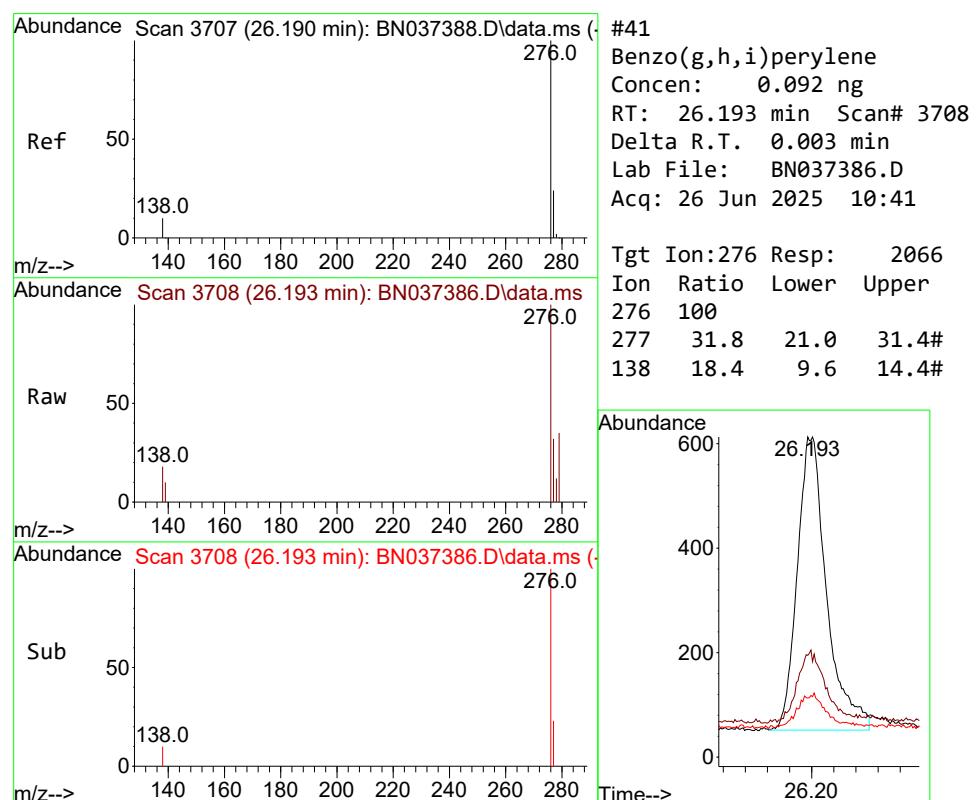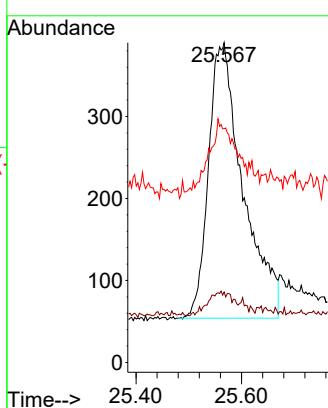

#41  
Benzo(g,h,i)perylene  
Concen: 0.092 ng  
RT: 26.193 min Scan# 3708  
Delta R.T. 0.003 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt Ion:276 Resp: 2066  
Ion Ratio Lower Upper  
276 100  
277 31.8 21.0 31.4#  
138 18.4 9.6 14.4#

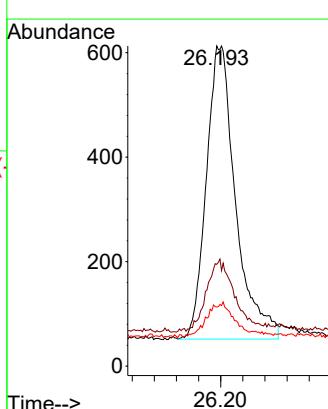

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037387.D  
 Acq On : 26 Jun 2025 11:17  
 Operator : RC/JU  
 Sample : SSTDICCO.2  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCO.2

Quant Time: Jun 26 16:05:20 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:05:06 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.561	152	1946	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4021	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2635	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5416	0.400	ng	# 0.01
29) Chrysene-d12	21.162	240	5370	0.400	ng	# 0.00
35) Perylene-d12	23.345	264	5780	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	757	0.202	ng	0.00
5) Phenol-d6	6.744	99	687	0.177	ng	0.00
8) Nitrobenzene-d5	8.717	82	565	0.175	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	1139	0.183	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	273	0.177	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	2182	0.192	ng	0.00
27) Fluoranthene-d10	19.008	212	3080	0.198	ng	0.00
31) Terphenyl-d14	19.616	244	2132	0.186	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	457	0.248	ng	# 88
3) n-Nitrosodimethylamine	3.422	42	367	0.201	ng	99
6) bis(2-Chloroethyl)ether	7.004	93	643	0.186	ng	98
9) Naphthalene	10.394	128	2012	0.194	ng	94
10) Hexachlorobutadiene	10.682	225	824	0.201	ng	# 98
12) 2-Methylnaphthalene	12.016	142	1337	0.188	ng	98
16) Acenaphthylene	13.935	152	2108	0.193	ng	99
17) Acenaphthene	14.277	154	1353	0.190	ng	99
18) Fluorene	15.272	166	1867	0.185	ng	98
20) 4,6-Dinitro-2-methylph...	15.378	198	228	0.164	ng	# 46
21) 4-Bromophenyl-phenylether	16.165	248	684	0.179	ng	# 92
22) Hexachlorobenzene	16.276	284	809	0.197	ng	98
23) Atrazine	16.450	200	563	0.186	ng	# 89
24) Pentachlorophenol	16.624	266	445	0.201	ng	94
25) Phenanthrene	17.009	178	2890	0.189	ng	99
26) Anthracene	17.096	178	2632	0.188	ng	98
28) Fluoranthene	19.035	202	3786	0.194	ng	99
30) Pyrene	19.398	202	3891	0.191	ng	99
32) Benzo(a)anthracene	21.153	228	3228	0.191	ng	99
33) Chrysene	21.198	228	4224	0.202	ng	97
34) Bis(2-ethylhexyl)phtha...	21.090	149	1366	0.204	ng	# 99
36) Indeno(1,2,3-cd)pyrene	25.532	276	4378	0.180	ng	# 95
37) Benzo(b)fluoranthene	22.696	252	3772	0.185	ng	# 88
38) Benzo(k)fluoranthene	22.740	252	4013	0.184	ng	# 87
39) Benzo(a)pyrene	23.254	252	3352	0.185	ng	# 84
40) Dibenzo(a,h)anthracene	25.555	278	3290	0.176	ng	# 82
41) Benzo(g,h,i)perylene	26.193	276	4258	0.190	ng	# 95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037387.D  
 Acq On : 26 Jun 2025 11:17  
 Operator : RC/JU  
 Sample : SSTDICCO.2  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCO.2

Quant Time: Jun 26 16:05:20 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:05:06 2025  
 Response via : Initial Calibration



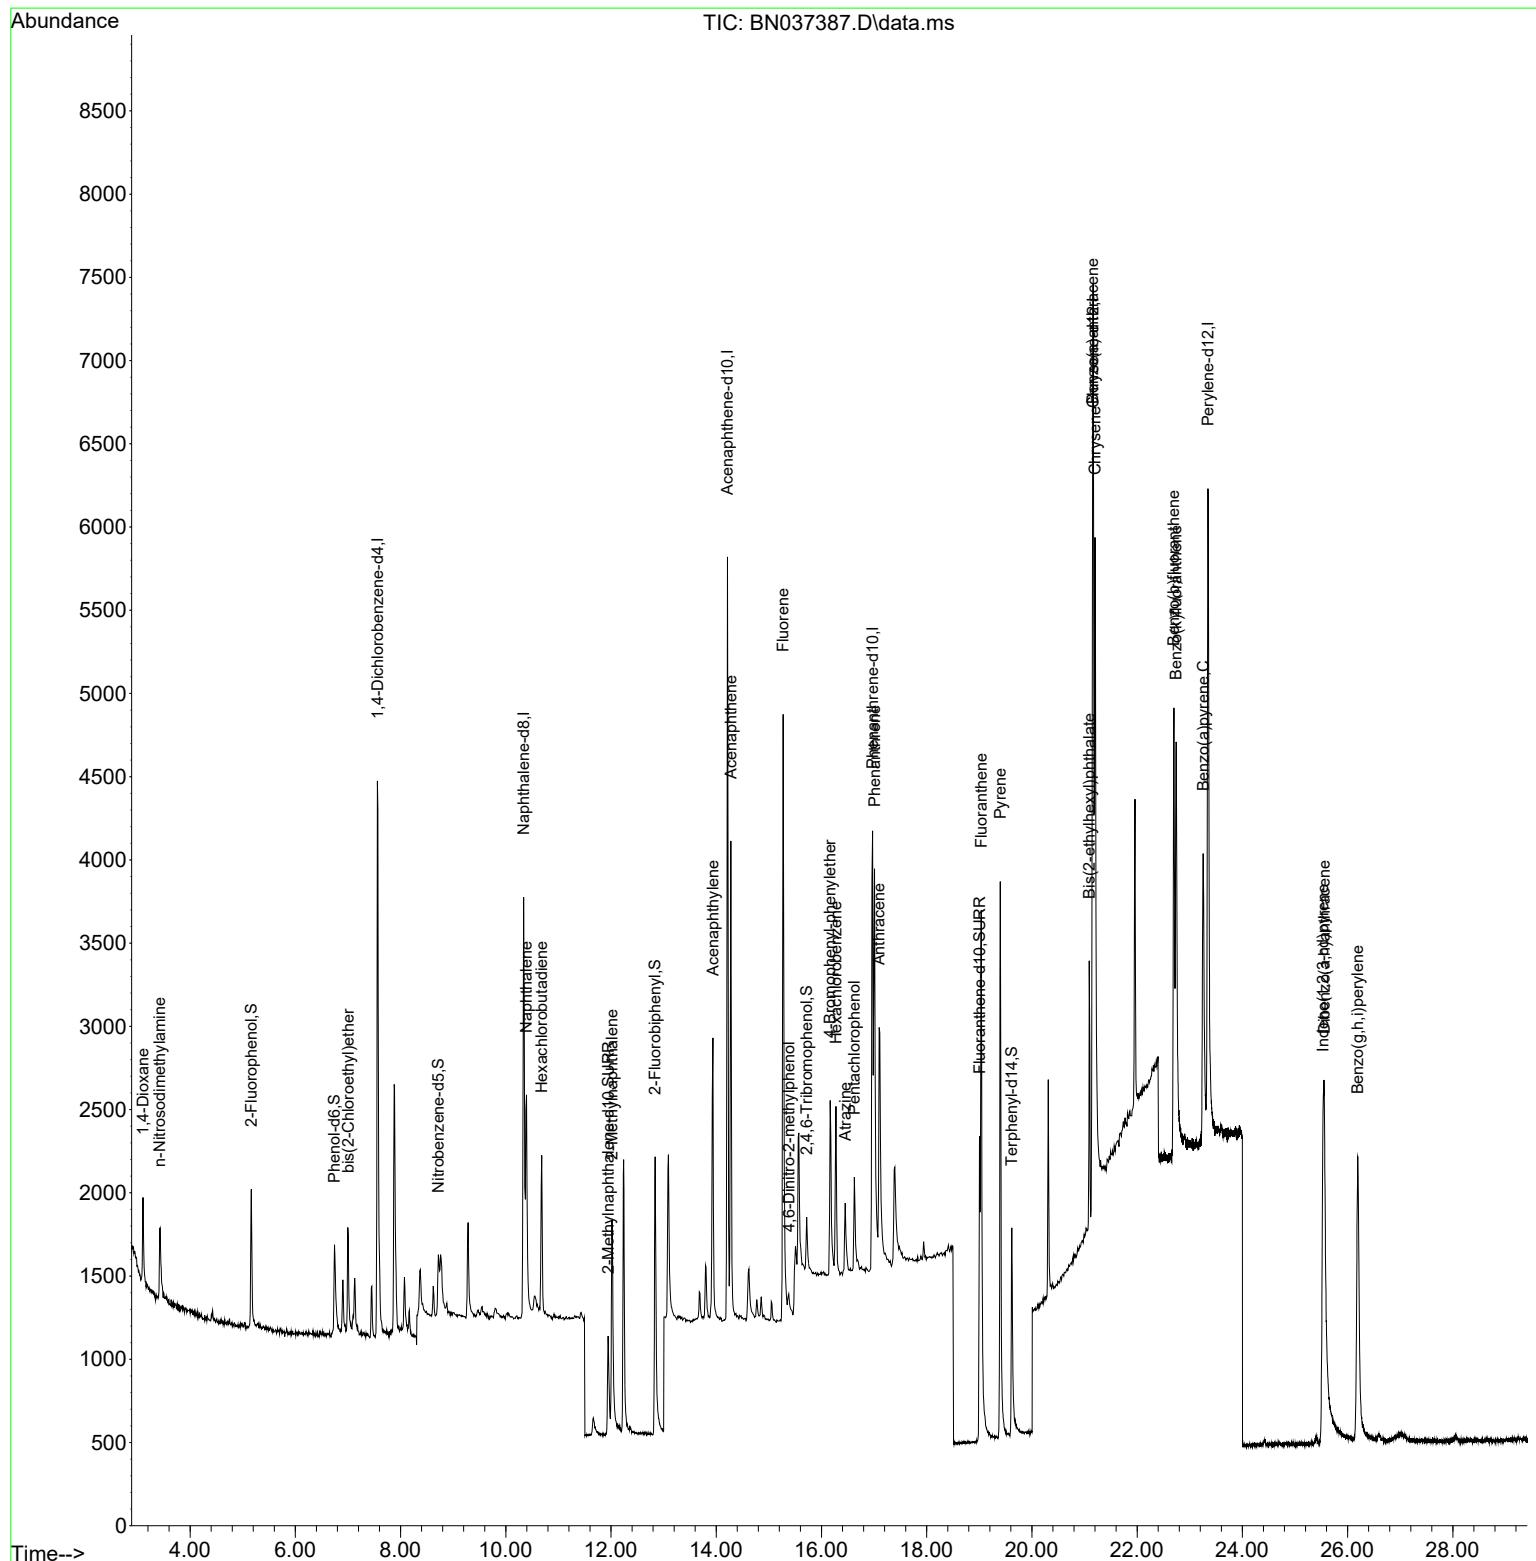


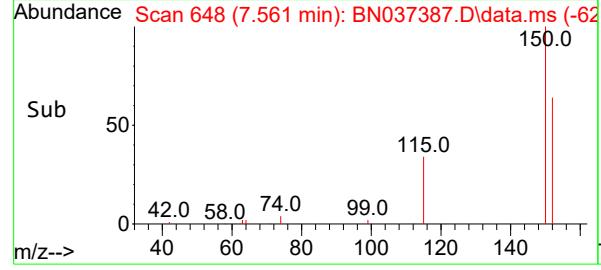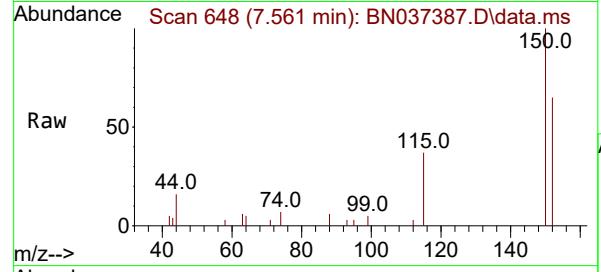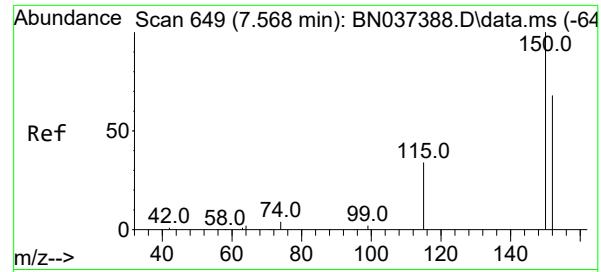

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.561 min Scan# 6  
Delta R.T. -0.007 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17



Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2




Tgt Ion:152 Resp: 1946  
Ion Ratio Lower Upper  
152 100  
150 153.3 116.2 174.2  
115 56.6 42.9 64.3

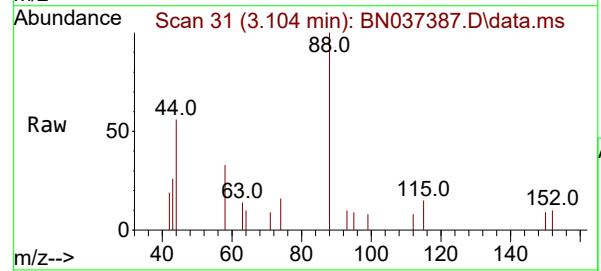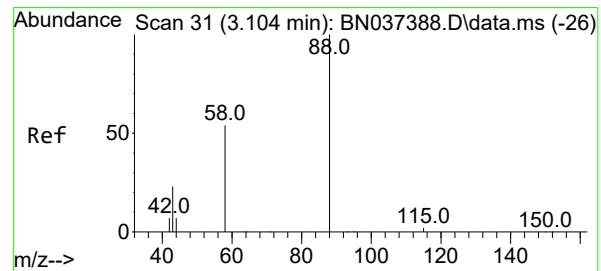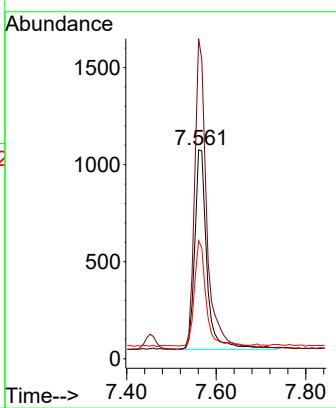

#2  
1,4-Dioxane  
Concen: 0.248 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17

Tgt Ion: 88 Resp: 457  
Ion Ratio Lower Upper  
88 100  
43 24.9 21.6 32.4  
58 45.5 45.9 68.9#

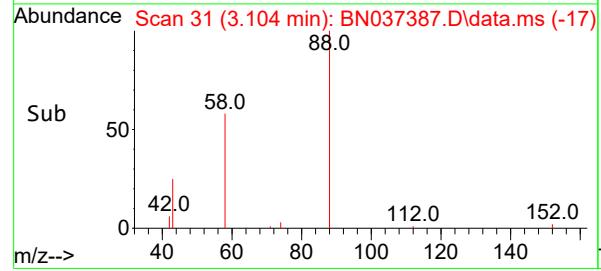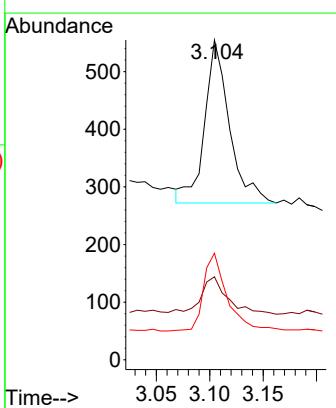

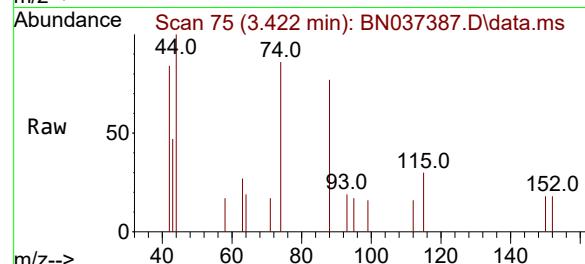

#3

n-Nitrosodimethylamine

Concen: 0.201 ng

RT: 3.422 min Scan# 7

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.2





Tgt Ion: 42 Resp: 367

Ion Ratio Lower Upper

42 100

74 123.2 97.8 146.8

44 11.4 8.7 13.1

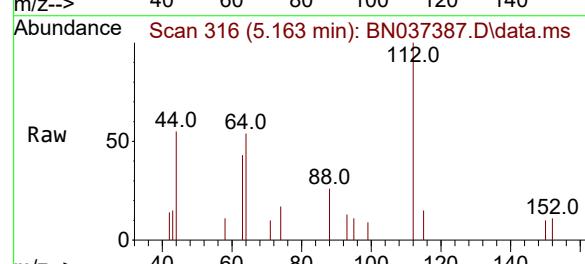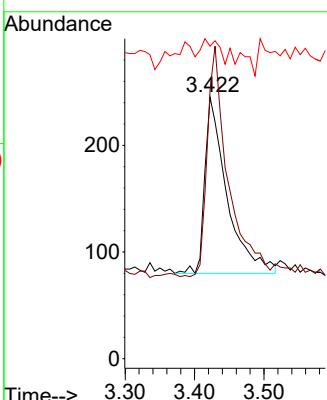

#4

2-Fluorophenol

Concen: 0.202 ng

RT: 5.163 min Scan# 316

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17


Tgt Ion: 112 Resp: 757


Ion Ratio Lower Upper

112 100

64 51.0 40.3 60.5


63 35.1 26.1 39.1





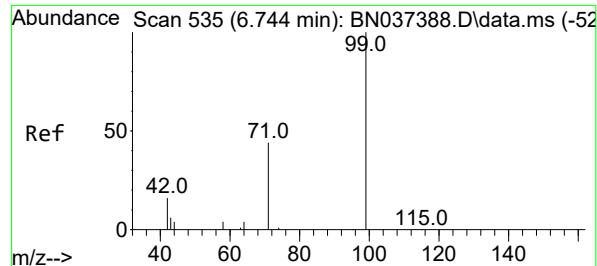


#5  
Phenol-d6  
Concen: 0.177 ng  
RT: 6.744 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2

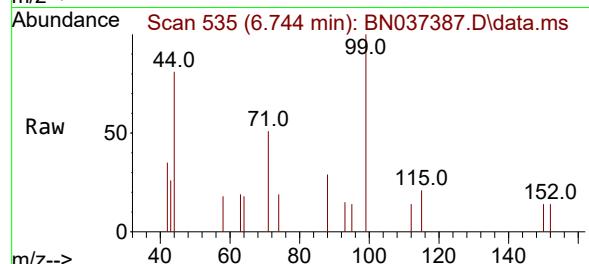



Tgt Ion: 99 Resp: 687  
Ion Ratio Lower Upper  
99 100  
42 23.0 15.6 23.4  
71 44.1 35.8 53.8




#6  
bis(2-Chloroethyl)ether  
Concen: 0.186 ng  
RT: 7.004 min Scan# 571  
Delta R.T. 0.007 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17




Tgt Ion: 93 Resp: 643  
Ion Ratio Lower Upper  
93 100  
63 63.9 49.6 74.4  
95 30.2 23.9 35.9





#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. 0.000 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17



Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2




Tgt Ion:136 Resp: 4021

Ion	Ratio	Lower	Upper
136	100		
137	13.7	10.4	15.6
54	8.7	5.6	8.4#
68	6.7	4.6	6.8

Abundance

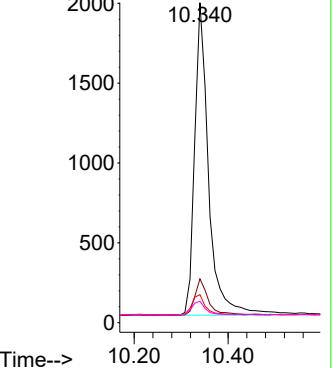



#8  
 Nitrobenzene-d5  
 Concen: 0.175 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. 0.000 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17



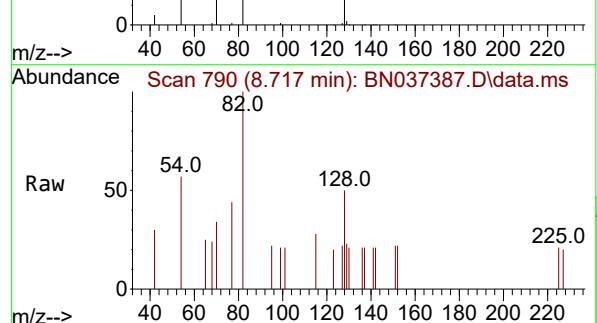


Tgt Ion: 82 Resp: 565

Ion	Ratio	Lower	Upper
82	100		
128	50.4	34.0	51.0
54	57.5	37.7	56.5#

Abundance

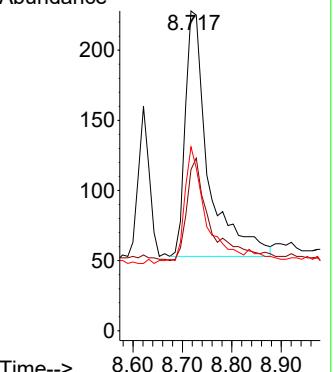

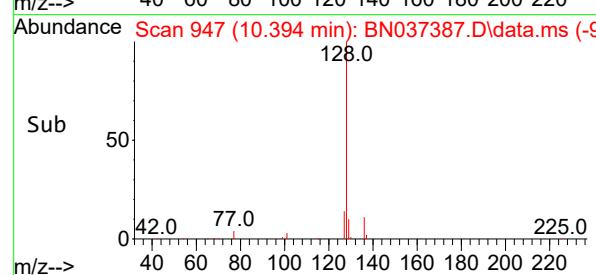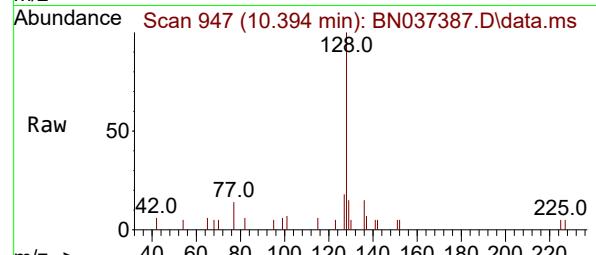

#9

Naphthalene

Concen: 0.194 ng

RT: 10.394 min Scan# 9

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.2

Tgt Ion:128 Resp: 2012

Ion Ratio Lower Upper





128 100

129 15.0 10.4 15.6

127 17.9 12.2 18.4

Abundance

10.394

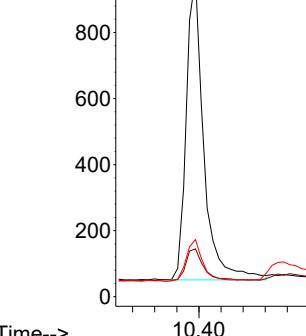

#10

Hexachlorobutadiene

Concen: 0.201 ng

RT: 10.682 min Scan# 974

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Tgt Ion:225 Resp: 824

Ion Ratio Lower Upper


225 100




223 0.0 0.0 0.0

227 63.6 49.9 74.9

Abundance

10.682

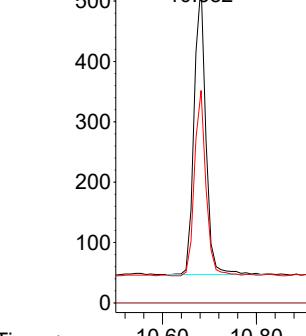



#11

2-Methylnaphthalene-d10

Concen: 0.183 ng

RT: 11.945 min Scan# 1139

Delta R.T. 0.005 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Instrument :

BNA\_N

ClientSampleId :





SSTDICCO.2

Tgt Ion:152 Resp: 1139

Ion Ratio Lower Upper

152 100

151 23.1 18.4 27.6

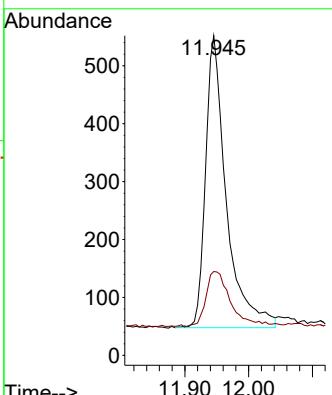

#12

2-Methylnaphthalene

Concen: 0.188 ng

RT: 12.016 min Scan# 1152

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17


Tgt Ion:142 Resp: 1337


Ion Ratio Lower Upper

142 100

141 88.9 70.1 105.1

115 47.7 35.8 53.6

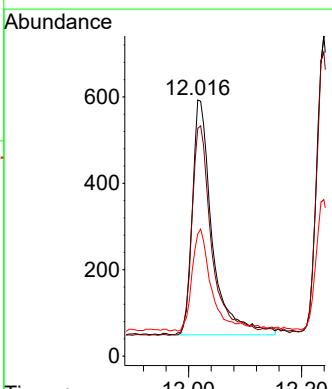

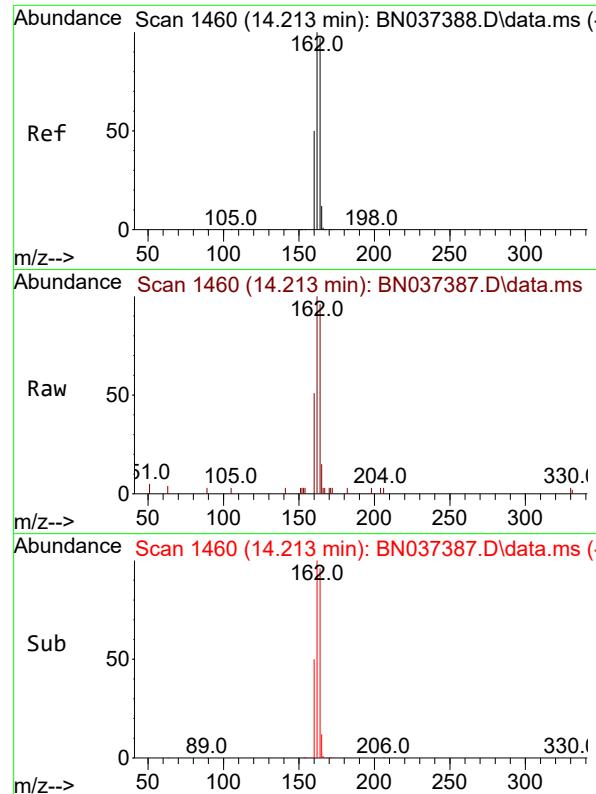

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1460

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Instrument : BNA\_N

ClientSampleId : SSTDICCO.2



Tgt Ion:164 Resp: 2635

Ion Ratio Lower Upper

164 100

162 104.4 82.6 123.8

160 53.6 42.2 63.2

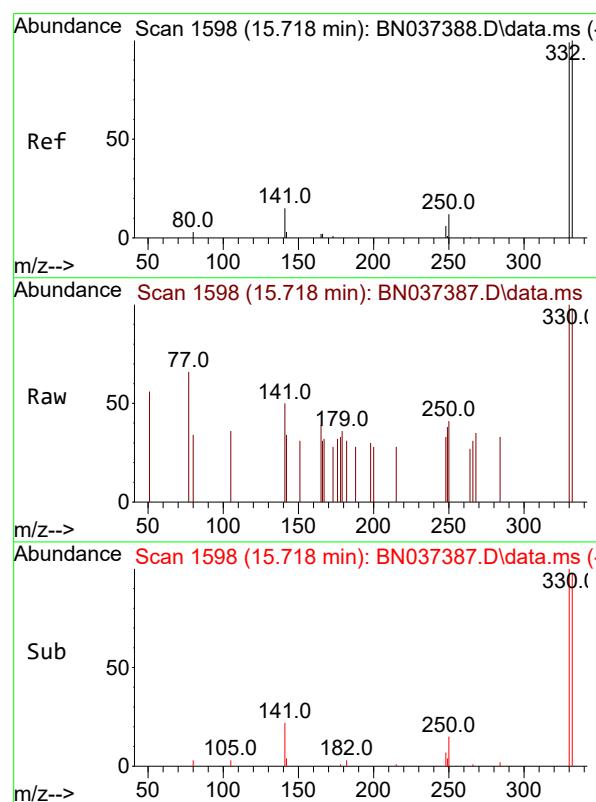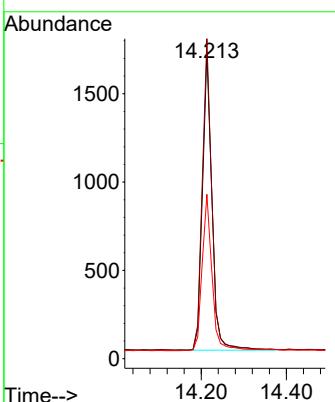

#14

2,4,6-Tribromophenol

Concen: 0.177 ng

RT: 15.718 min Scan# 1598

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17


Tgt Ion:330 Resp: 273


Ion Ratio Lower Upper

330 100

332 101.8 77.8 116.8



141 35.2 24.0 36.0



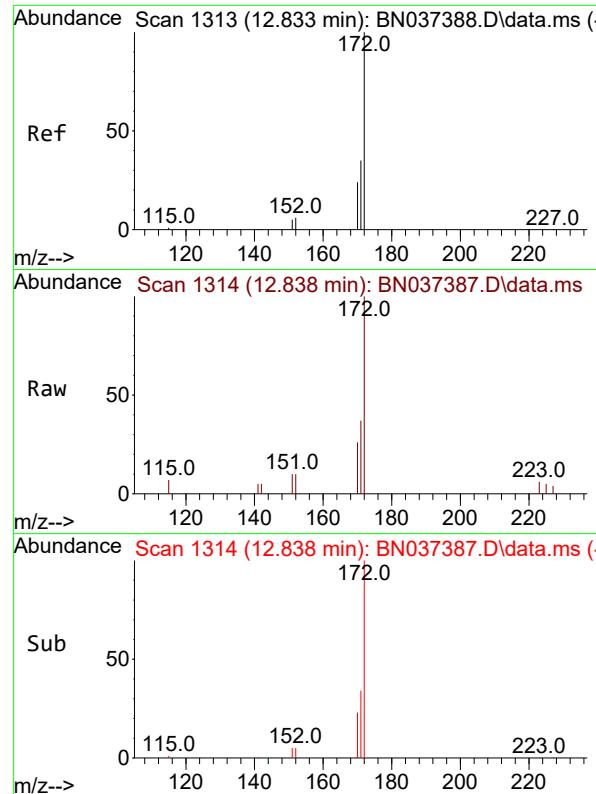


#15  
2-Fluorobiphenyl  
Concen: 0.192 ng  
RT: 12.838 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.005 min  
Lab File: BN037387.D ClientSampleId : SSTDICCO.2  
Acq: 26 Jun 2025 11:17




Tgt Ion:172 Resp: 2182  
Ion Ratio Lower Upper  
172 100  
171 37.1 28.8 43.2  
170 26.4 20.3 30.5

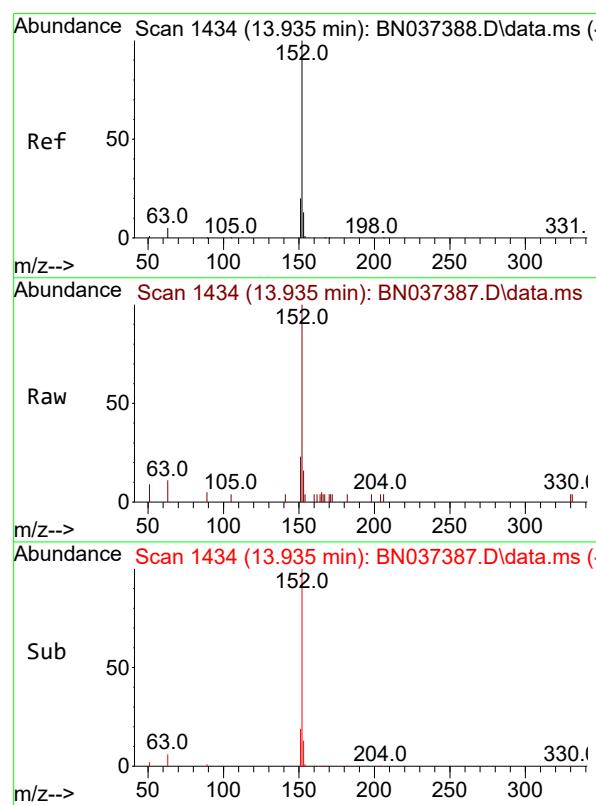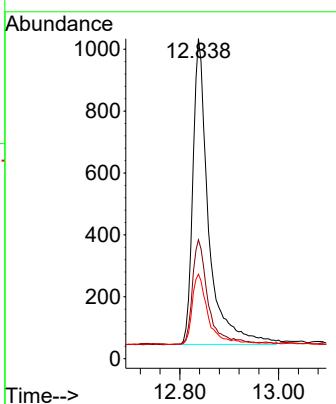

#16  
Acenaphthylene  
Concen: 0.193 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17

Tgt Ion:152 Resp: 2108  
Ion Ratio Lower Upper  
152 100  
151 20.2 15.8 23.6  
153 12.8 10.3 15.5

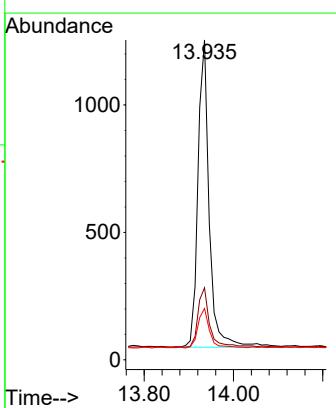

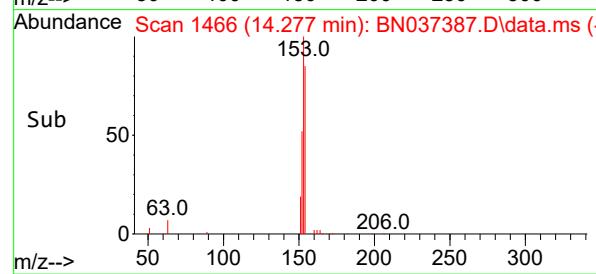

#17

Acenaphthene

Concen: 0.190 ng

RT: 14.277 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.2

Tgt Ion:154 Resp: 1353

Ion Ratio Lower Upper

154 100





153 118.8 94.6 141.8

152 63.5 50.2 75.2

Abundance

1000  
800  
600  
400  
200  
0

14.277

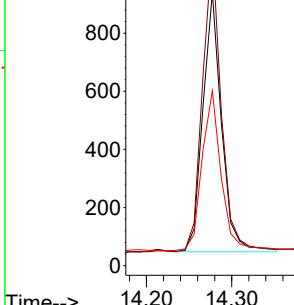

#18

Fluorene

Concen: 0.185 ng

RT: 15.272 min Scan# 1559

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Tgt Ion:166 Resp: 1867

Ion Ratio Lower Upper

166 100


165 101.4 79.4 119.2


167 14.0 10.6 15.8

Abundance

1000  
800  
600  
400  
200  
0

15.272


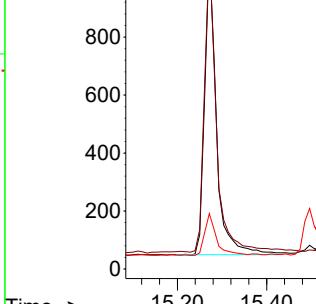


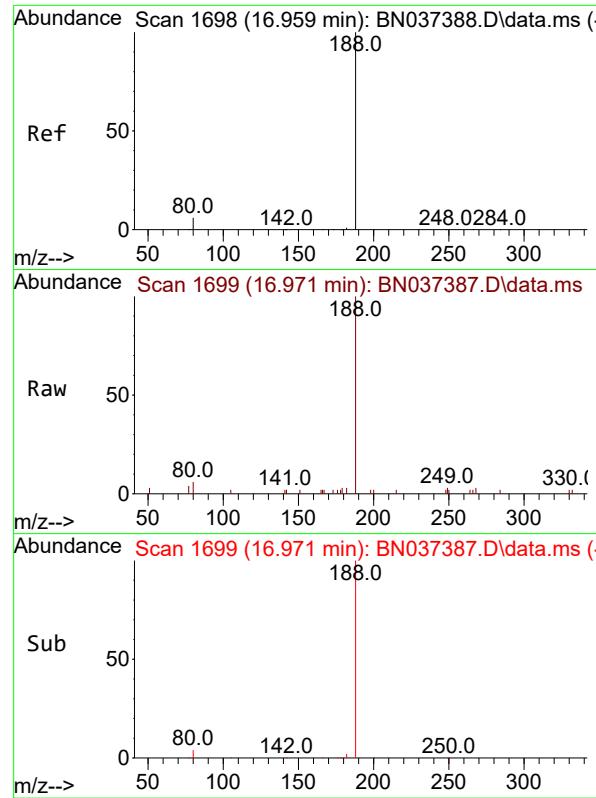

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. 0.012 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2


Tgt Ion:188 Resp: 5416  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 5.8 6.2 9.4#

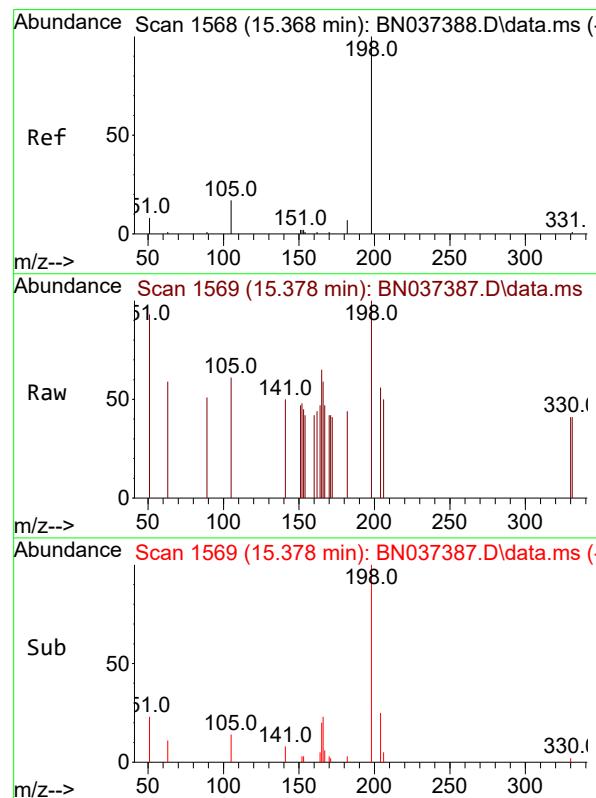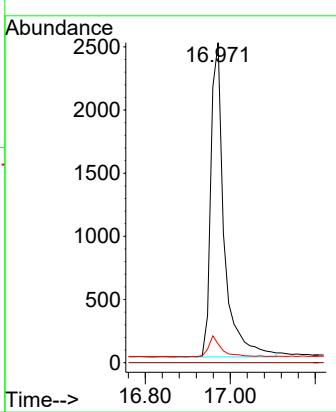

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.164 ng  
 RT: 15.378 min Scan# 1569  
 Delta R.T. 0.011 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17



Tgt Ion:198 Resp: 228  
 Ion Ratio Lower Upper  
 198 100  
 51 92.8 38.8 58.2#  
 105 61.3 29.8 44.6#

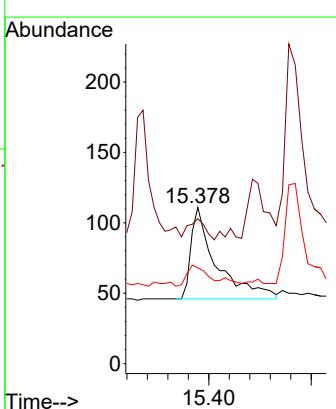

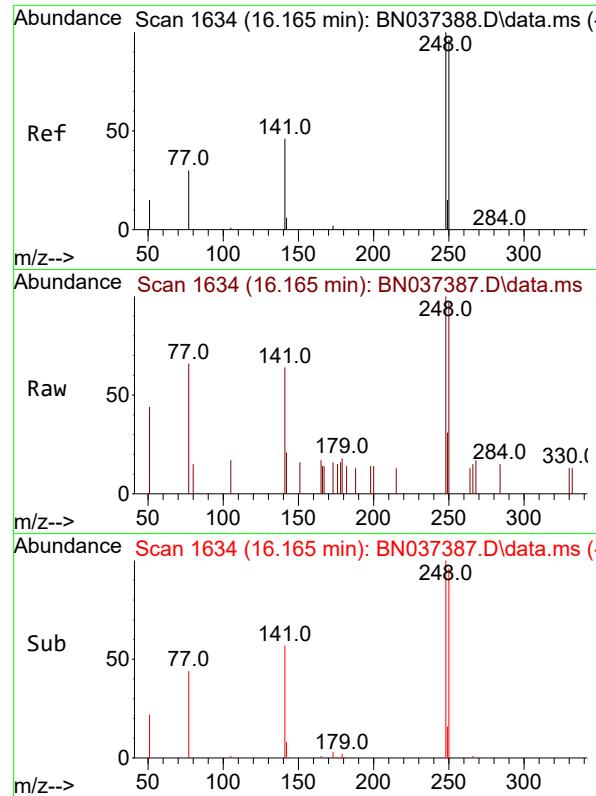


#21  
4-Bromophenyl-phenylether  
Concen: 0.179 ng  
RT: 16.165 min Scan# 1  
Instrument: BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037387.D  
ClientSampleId : SSTDICCO.2  
Acq: 26 Jun 2025 11:17


Tgt Ion:248 Resp: 684  
Ion Ratio Lower Upper  
248 100  
250 97.1 77.0 115.4  
141 64.3 38.7 58.1#

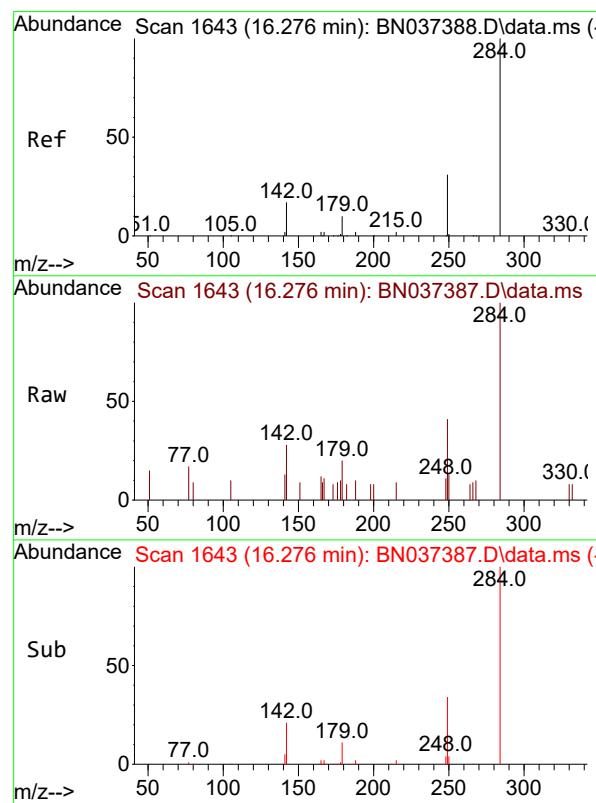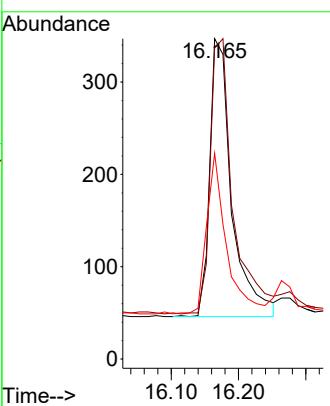

#22  
Hexachlorobenzene  
Concen: 0.197 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17

Tgt Ion:284 Resp: 809  
Ion Ratio Lower Upper  
284 100  
142 35.0 27.2 40.8  
249 35.1 26.7 40.1



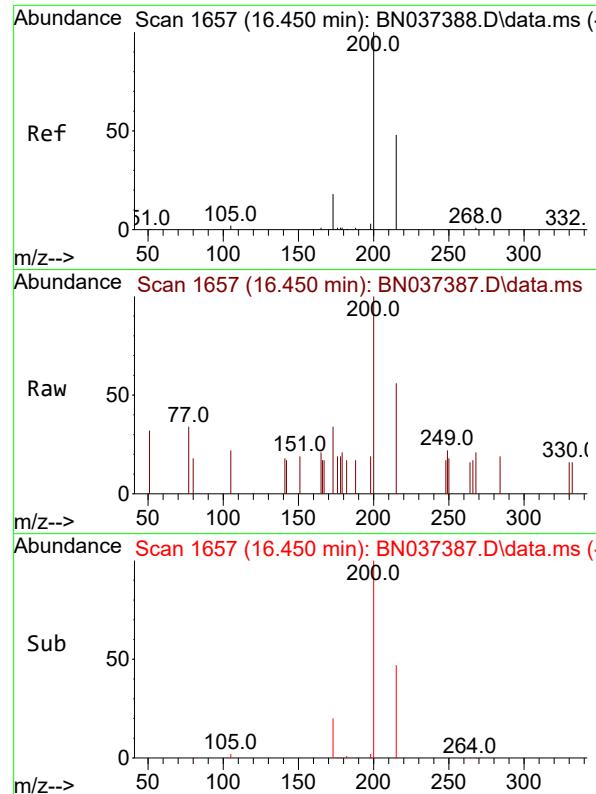

#23

Atrazine

Concen: 0.186 ng

RT: 16.450 min Scan# 1

Instrument:

BNA\_N

Delta R.T. 0.000 min

Lab File: BN037387.D

ClientSampleId :

Acq: 26 Jun 2025 11:17

SSTDICCO.2

Tgt Ion:200 Resp: 563

Ion Ratio Lower Upper



200 100

173 33.6 19.0 28.6#

215 56.3 41.3 61.9

Abundance

16.450

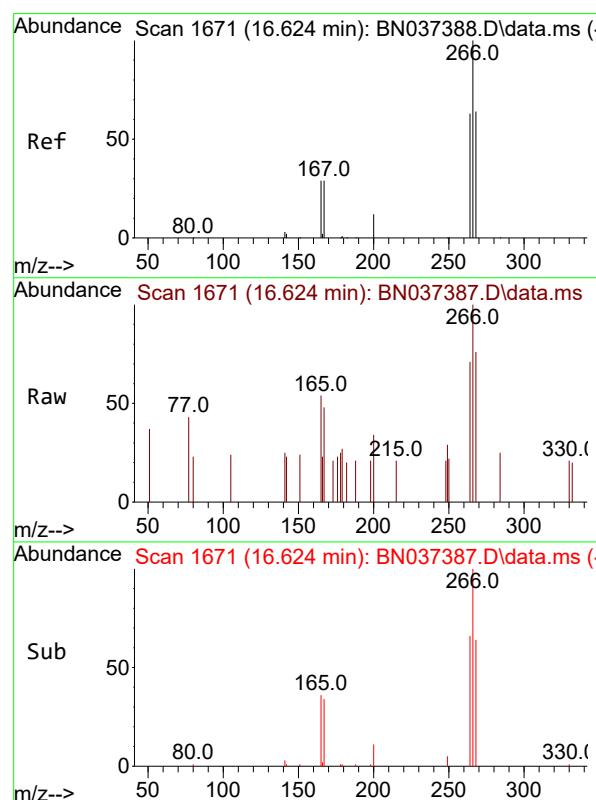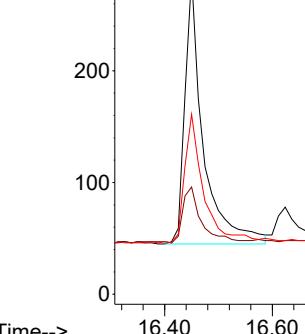

#24

Pentachlorophenol

Concen: 0.201 ng

RT: 16.624 min Scan# 1671

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Tgt Ion:266 Resp: 445


Ion Ratio Lower Upper




266 100

264 61.6 49.2 73.8

268 59.1 54.2 81.4

Abundance

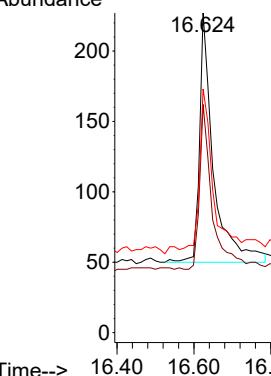

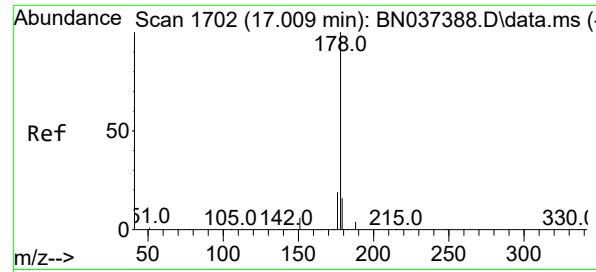

#25

Phenanthrene

Concen: 0.189 ng

RT: 17.009 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.2





Tgt Ion:178 Resp: 2890

Ion Ratio Lower Upper

178 100

176 19.3 15.6 23.4

179 15.7 12.8 19.2

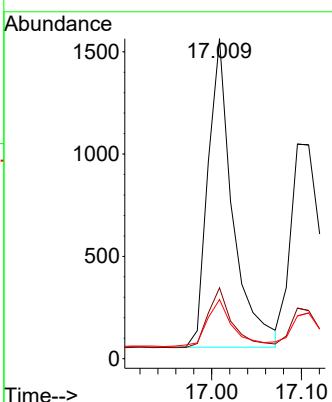

#26

Anthracene

Concen: 0.188 ng

RT: 17.096 min Scan# 1709

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17


Tgt Ion:178 Resp: 2632


Ion Ratio Lower Upper

178 100

176 17.3 14.9 22.3

179 15.5 12.4 18.6





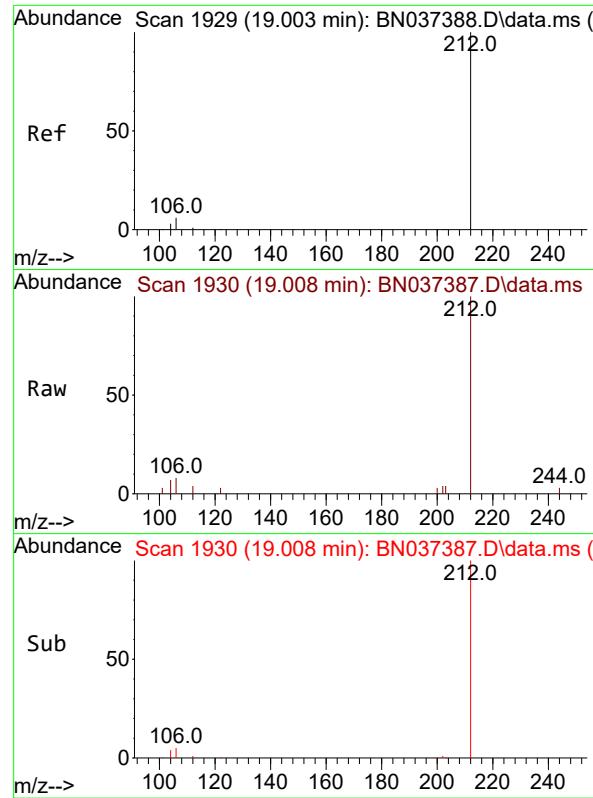

#27  
 Fluoranthene-d10  
 Concen: 0.198 ng  
 RT: 19.008 min Scan# 1  
 Delta R.T. 0.005 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2




Tgt Ion:212 Resp: 3080  
 Ion Ratio Lower Upper  
 212 100  
 106 5.6 4.5 6.7  
 104 3.8 2.7 4.1

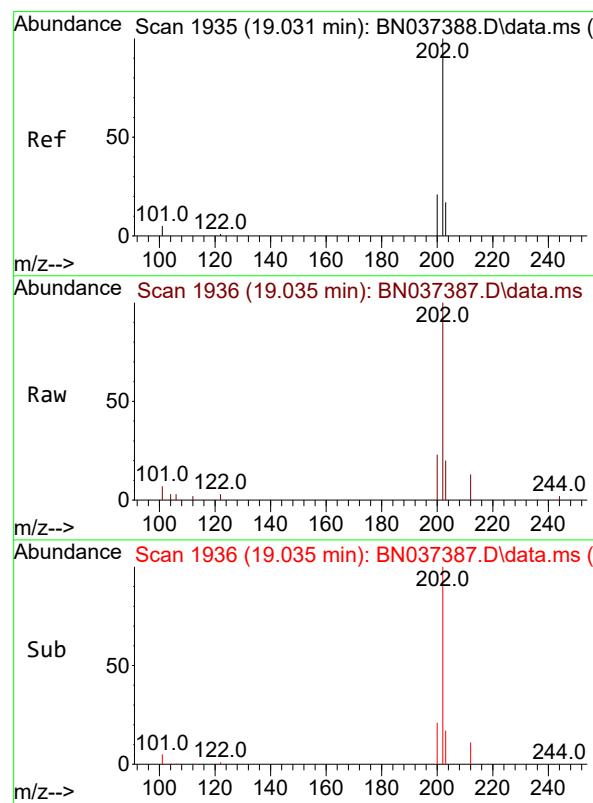

#28  
 Fluoranthene  
 Concen: 0.194 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. 0.005 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17

Tgt Ion:202 Resp: 3786  
 Ion Ratio Lower Upper  
 202 100  
 101 4.8 3.8 5.6  
 203 17.2 13.5 20.3





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.162 min Scan# 2

Instrument : BNA\_N

Delta R.T. 0.000 min

Lab File: BN037387.D

ClientSampleId : SSTDICCO.2

Acq: 26 Jun 2025 11:17





Tgt Ion:240 Resp: 5370

Ion Ratio Lower Upper

240 100

120 8.8 5.3 7.9#

236 30.5 22.7 34.1

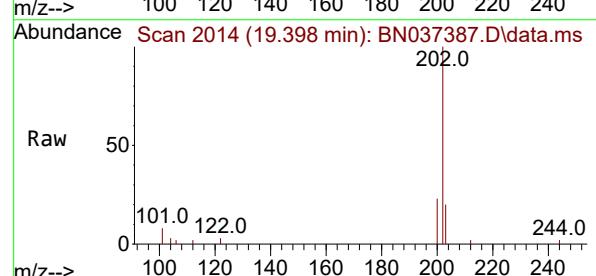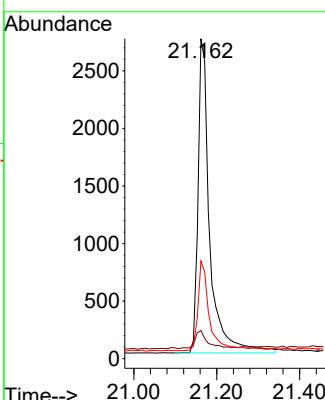

#30

Pyrene

Concen: 0.191 ng

RT: 19.398 min Scan# 2014

Delta R.T. 0.000 min

Lab File: BN037387.D

Acq: 26 Jun 2025 11:17


Tgt Ion:202 Resp: 3891


Ion Ratio Lower Upper

202 100

200 20.8 16.5 24.7

203 18.6 14.2 21.2


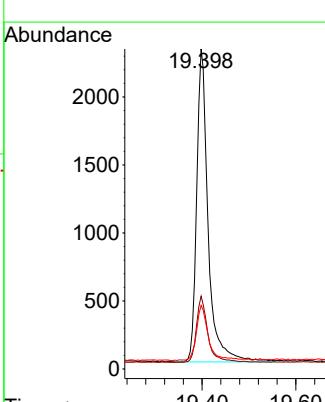


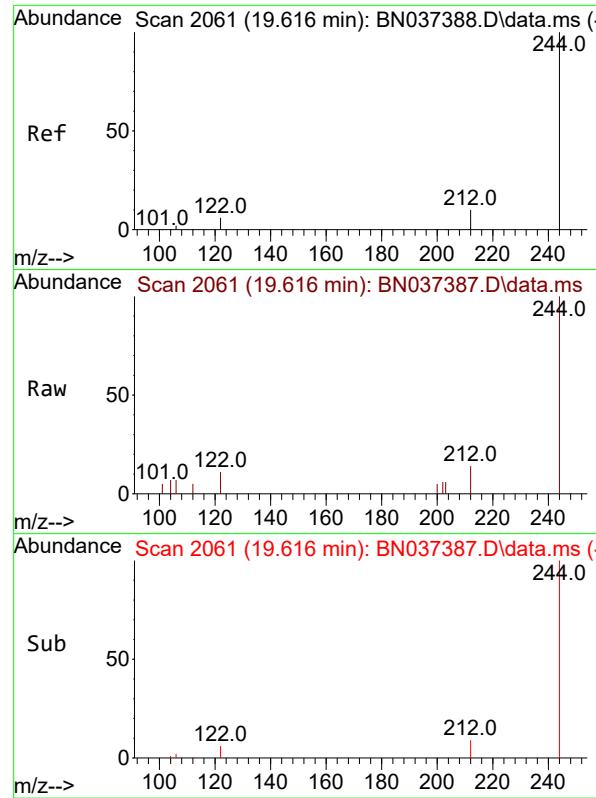

#31  
Terphenyl-d14  
Concen: 0.186 ng  
RT: 19.616 min Scan# 2132  
Delta R.T. 0.000 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2


Tgt Ion:244 Resp: 2132  
Ion Ratio Lower Upper  
244 100  
212 13.8 9.1 13.7#  
122 10.9 6.3 9.5#

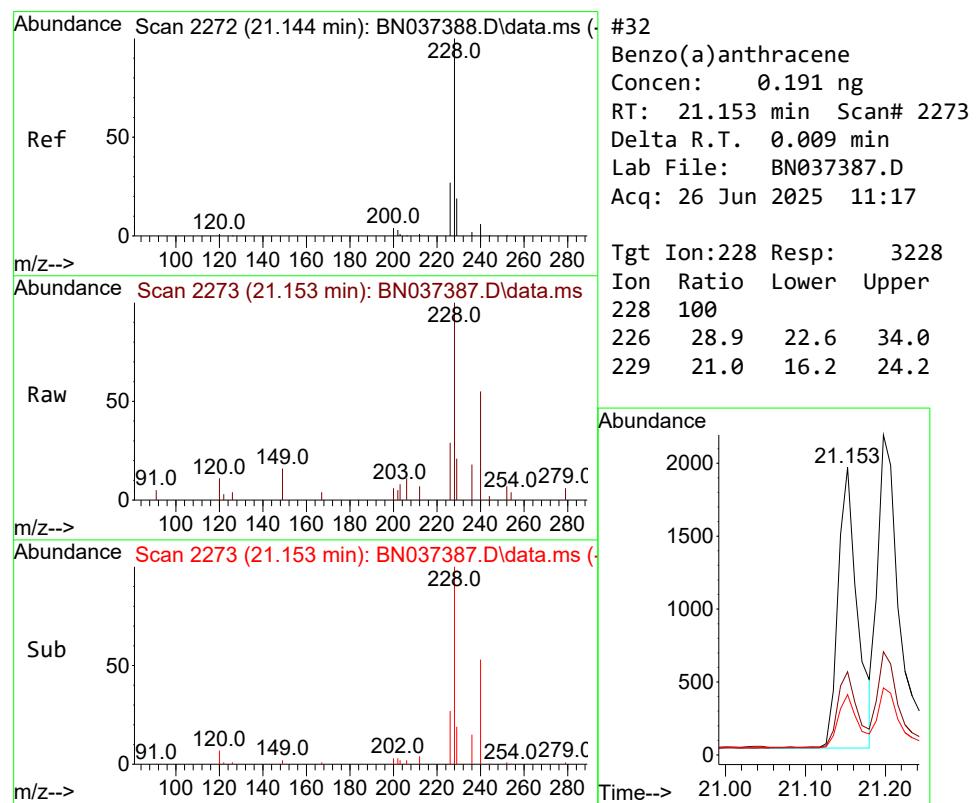

#32  
Benzo(a)anthracene  
Concen: 0.191 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.009 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17



Tgt Ion:228 Resp: 3228  
Ion Ratio Lower Upper  
228 100  
226 28.9 22.6 34.0  
229 21.0 16.2 24.2



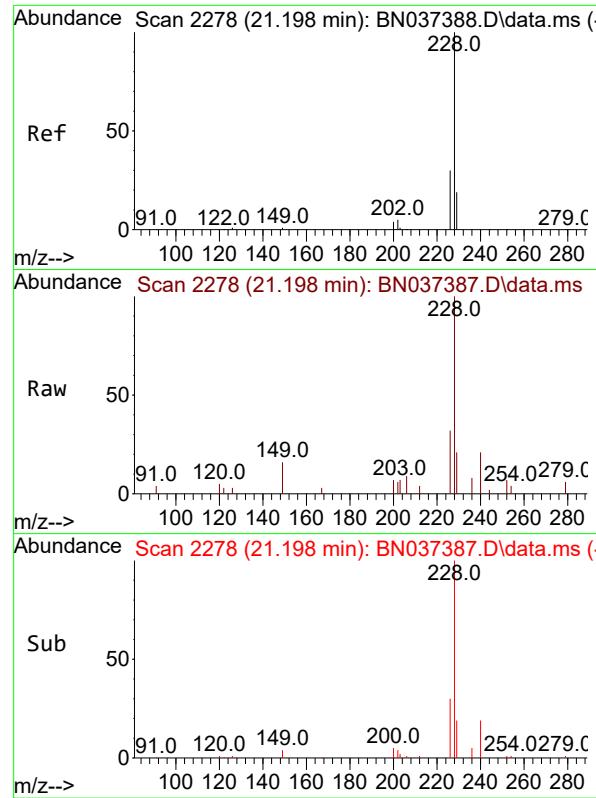


#33  
Chrysene  
Concen: 0.202 ng  
RT: 21.198 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037387.D ClientSampleId : SSTDICCO.2  
Acq: 26 Jun 2025 11:17


Tgt Ion:228 Resp: 4224  
Ion Ratio Lower Upper  
228 100  
226 32.3 24.5 36.7  
229 20.9 16.1 24.1

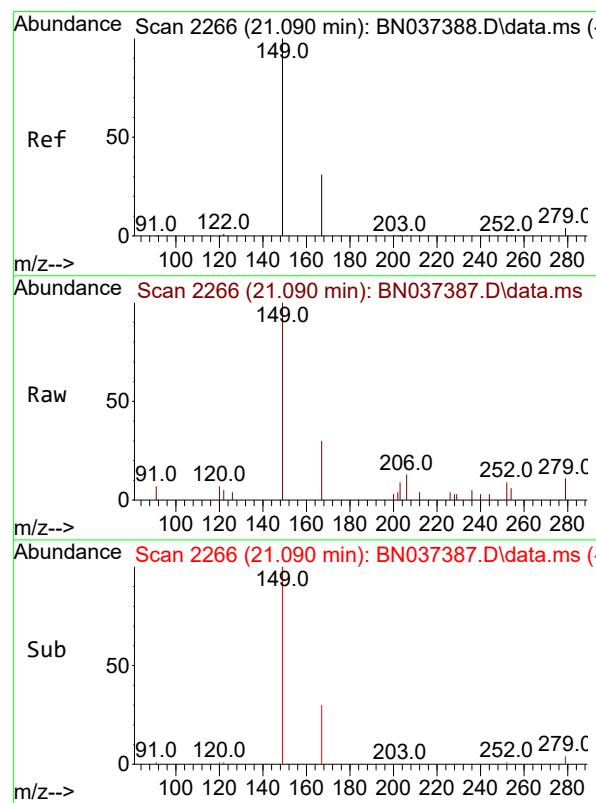

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.204 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. 0.000 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17

Tgt Ion:149 Resp: 1366  
Ion Ratio Lower Upper  
149 100  
167 30.9 24.8 37.2  
279 7.6 5.0 7.6#





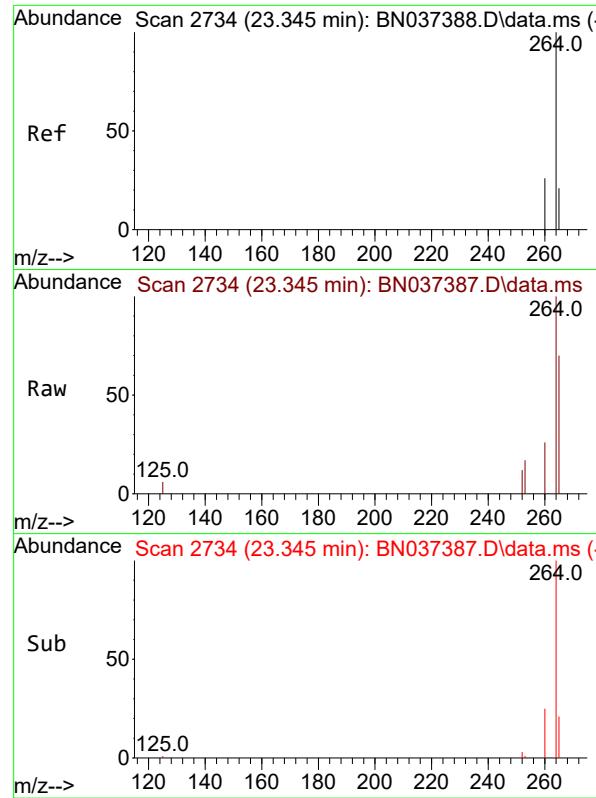

#35  
 Perylene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 23.345 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2


Tgt Ion:264 Resp: 5780  
 Ion Ratio Lower Upper  
 264 100  
 260 25.9 21.4 32.0  
 265 69.6 56.2 84.4

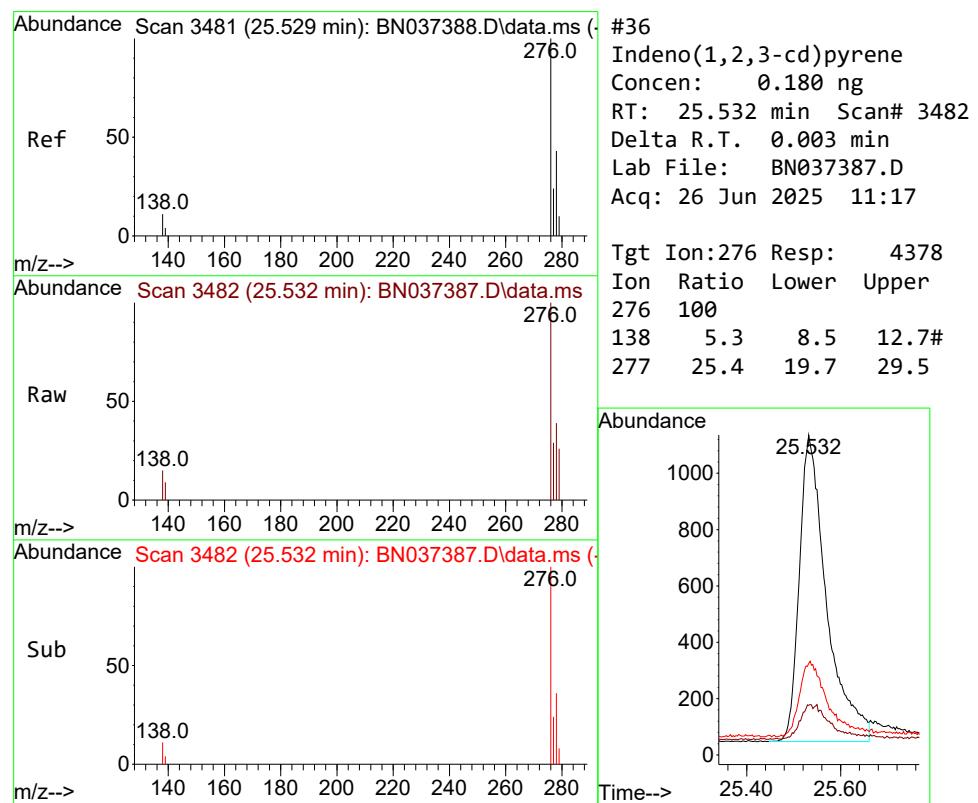

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.180 ng  
 RT: 25.532 min Scan# 3482  
 Delta R.T. 0.003 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17

Tgt Ion:276 Resp: 4378  
 Ion Ratio Lower Upper  
 276 100  
 138 5.3 8.5 12.7#  
 277 25.4 19.7 29.5





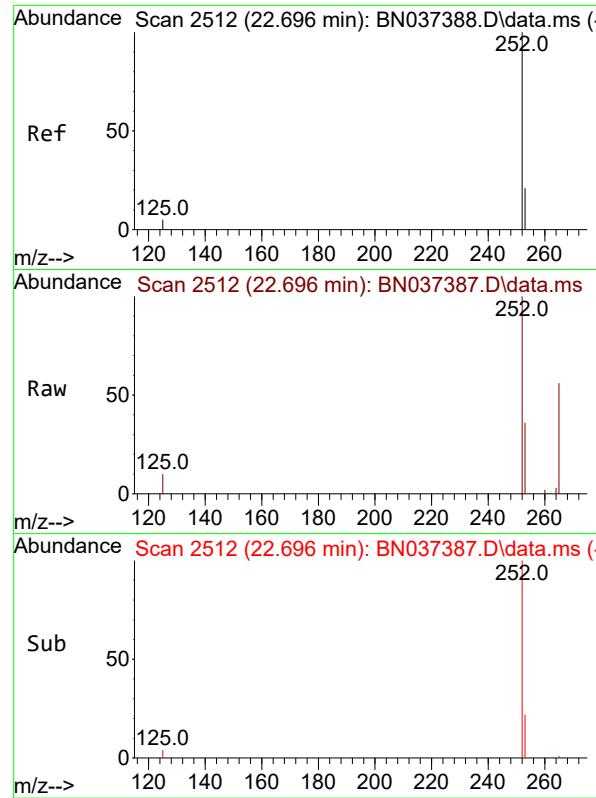

#37  
 Benzo(b)fluoranthene  
 Concen: 0.185 ng  
 RT: 22.696 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2


Tgt Ion:252 Resp: 3772  
 Ion Ratio Lower Upper  
 252 100  
 253 35.5 22.8 34.2#  
 125 10.2 6.2 9.4#

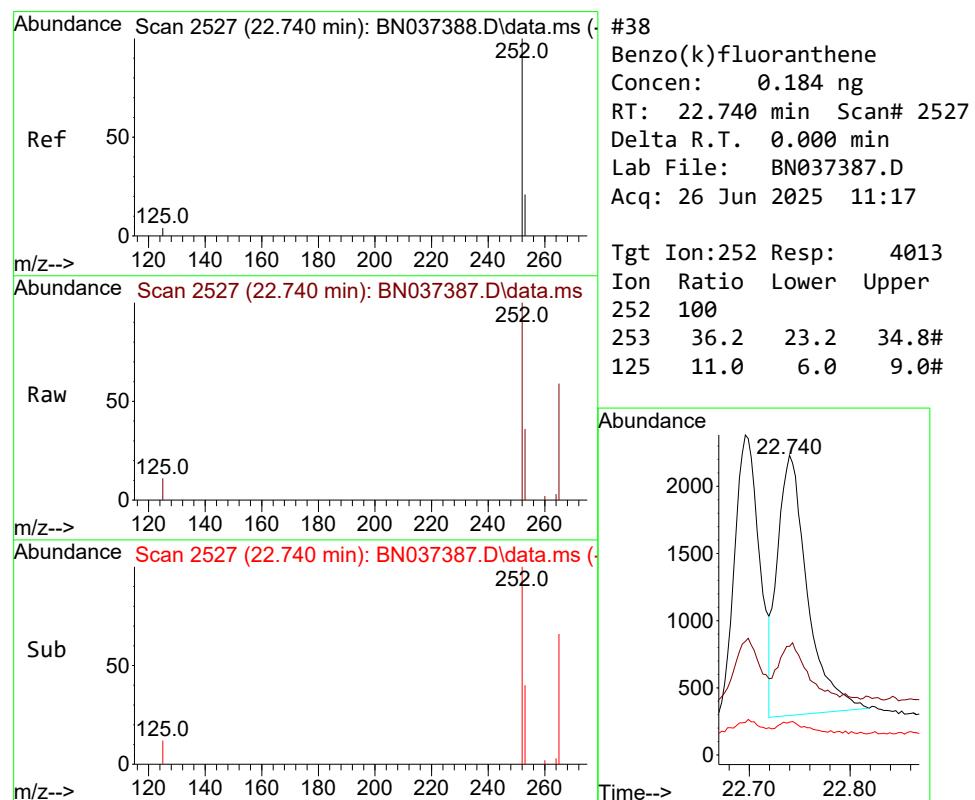

#38  
 Benzo(k)fluoranthene  
 Concen: 0.184 ng  
 RT: 22.740 min Scan# 2527  
 Delta R.T. 0.000 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17

Tgt Ion:252 Resp: 4013  
 Ion Ratio Lower Upper  
 252 100  
 253 36.2 23.2 34.8#  
 125 11.0 6.0 9.0#


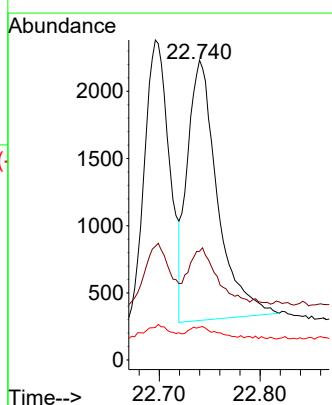


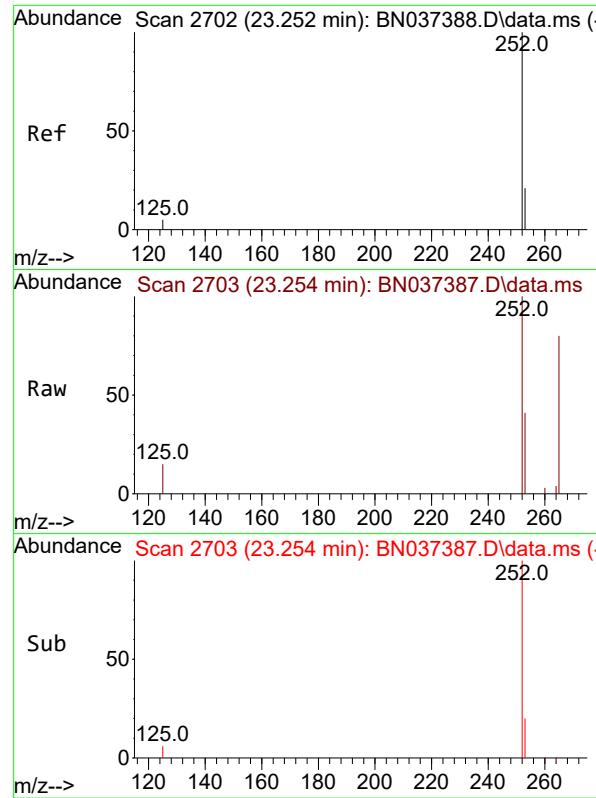

#39  
 Benzo(a)pyrene  
 Concen: 0.185 ng  
 RT: 23.254 min Scan# 2  
 Delta R.T. 0.003 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.2


Tgt Ion:252 Resp: 3352  
 Ion Ratio Lower Upper  
 252 100  
 253 41.5 25.6 38.4#  
 125 14.7 7.5 11.3#

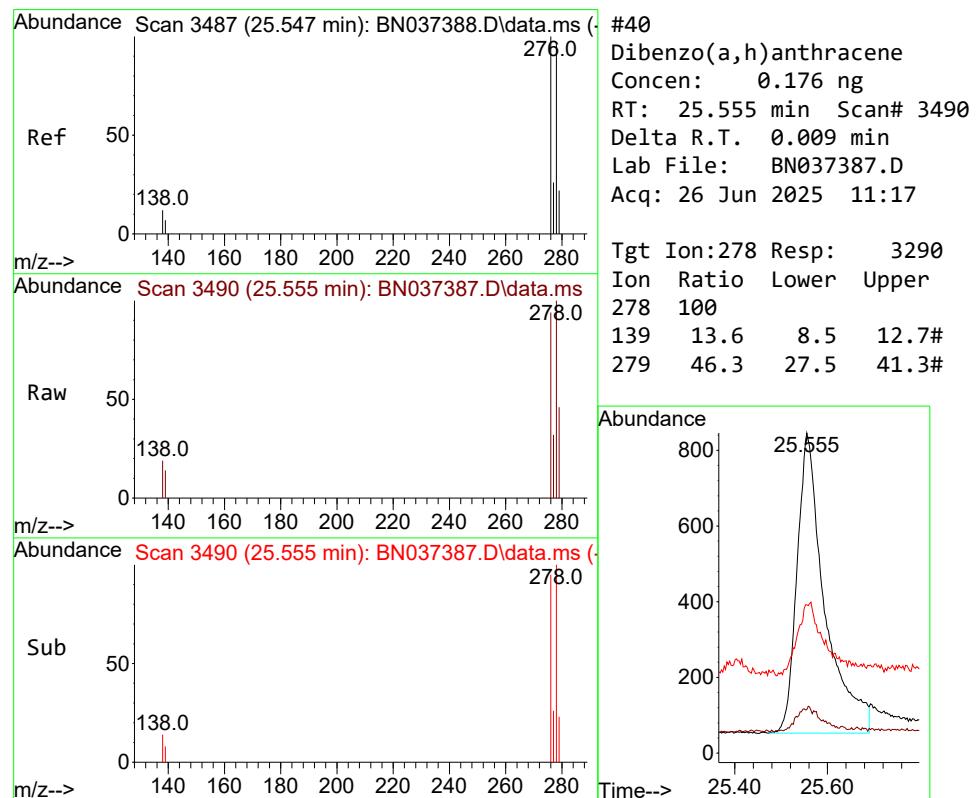

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.176 ng  
 RT: 25.555 min Scan# 3490  
 Delta R.T. 0.009 min  
 Lab File: BN037387.D  
 Acq: 26 Jun 2025 11:17

Tgt Ion:278 Resp: 3290  
 Ion Ratio Lower Upper  
 278 100  
 139 13.6 8.5 12.7#  
 279 46.3 27.5 41.3#




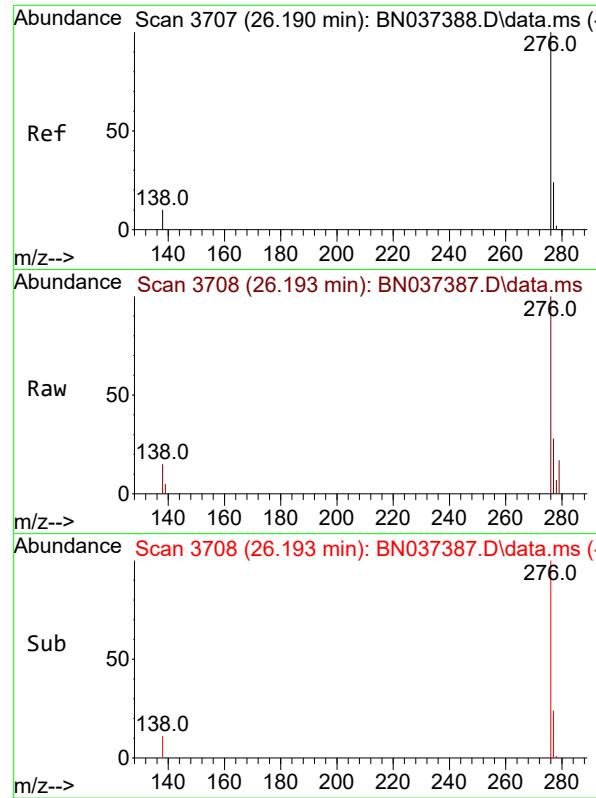

#41  
Benzo(g,h,i)perylene  
Concen: 0.190 ng  
RT: 26.193 min Scan# 3  
Delta R.T. 0.003 min  
Lab File: BN037387.D  
Acq: 26 Jun 2025 11:17

Instrument : BNA\_N  
ClientSampleId : SSTDICCO.2

Tgt Ion:276 Resp: 4258  
Ion Ratio Lower Upper  
276 100  
277 27.8 21.0 31.4  
138 15.3 9.6 14.4#



Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037388.D  
 Acq On : 26 Jun 2025 11:53  
 Operator : RC/JU  
 Sample : SSTDICCC0.4  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCC0.4

Quant Time: Jun 26 14:43:58 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2117	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4565	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	3048	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	6284	0.400	ng	0.00
29) Chrysene-d12	21.162	240	5612	0.400	ng	0.00
35) Perylene-d12	23.345	264	5950	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1703	0.417	ng	0.00
5) Phenol-d6	6.744	99	1720	0.407	ng	0.00
8) Nitrobenzene-d5	8.717	82	1419	0.386	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	2629	0.372	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	729	0.408	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	5253	0.399	ng	0.00
27) Fluoranthene-d10	19.003	212	6680	0.371	ng	0.00
31) Terphenyl-d14	19.616	244	4873	0.407	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	781	0.412	ng	100
3) n-Nitrosodimethylamine	3.422	42	792	0.399	ng	100
6) bis(2-Chloroethyl)ether	6.997	93	1521	0.404	ng	100
9) Naphthalene	10.394	128	4559	0.388	ng	100
10) Hexachlorobutadiene	10.682	225	1887	0.405	ng	# 100
12) 2-Methylnaphthalene	12.016	142	3122	0.386	ng	100
16) Acenaphthylene	13.935	152	4804	0.380	ng	100
17) Acenaphthene	14.277	154	3185	0.386	ng	100
18) Fluorene	15.272	166	4498	0.386	ng	100
20) 4,6-Dinitro-2-methylph...	15.368	198	535	0.331	ng	100
21) 4-Bromophenyl-phenylether	16.165	248	1694	0.382	ng	100
22) Hexachlorobenzene	16.276	284	1899	0.398	ng	100
23) Atrazine	16.450	200	1336	0.380	ng	100
24) Pentachlorophenol	16.624	266	973	0.378	ng	99
25) Phenanthrene	17.009	178	6787	0.383	ng	100
26) Anthracene	17.096	178	6087	0.374	ng	100
28) Fluoranthene	19.031	202	8557	0.378	ng	100
30) Pyrene	19.398	202	8607	0.405	ng	100
32) Benzo(a)anthracene	21.144	228	6549	0.371	ng	100
33) Chrysene	21.198	228	8883	0.407	ng	100
34) Bis(2-ethylhexyl)phtha...	21.090	149	2830	0.405	ng	100
36) Indeno(1,2,3-cd)pyrene	25.529	276	9382	0.374	ng	100
37) Benzo(b)fluoranthene	22.696	252	7840	0.374	ng	100
38) Benzo(k)fluoranthene	22.740	252	8696	0.388	ng	100
39) Benzo(a)pyrene	23.252	252	7038	0.377	ng	100
40) Dibenzo(a,h)anthracene	25.547	278	7205	0.374	ng	100
41) Benzo(g,h,i)perylene	26.190	276	8788	0.382	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
Data File : BN037388.D  
Acq On : 26 Jun 2025 11:53  
Operator : RC/JU  
Sample : SSTDICCC0.4  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

**Instrument :**  
BNA\_N  
**ClientSampleId :**  
SSTDICCC0.4

Quant Time: Jun 26 14:43:58 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 26 14:40:13 2025  
Response via : Initial Calibration


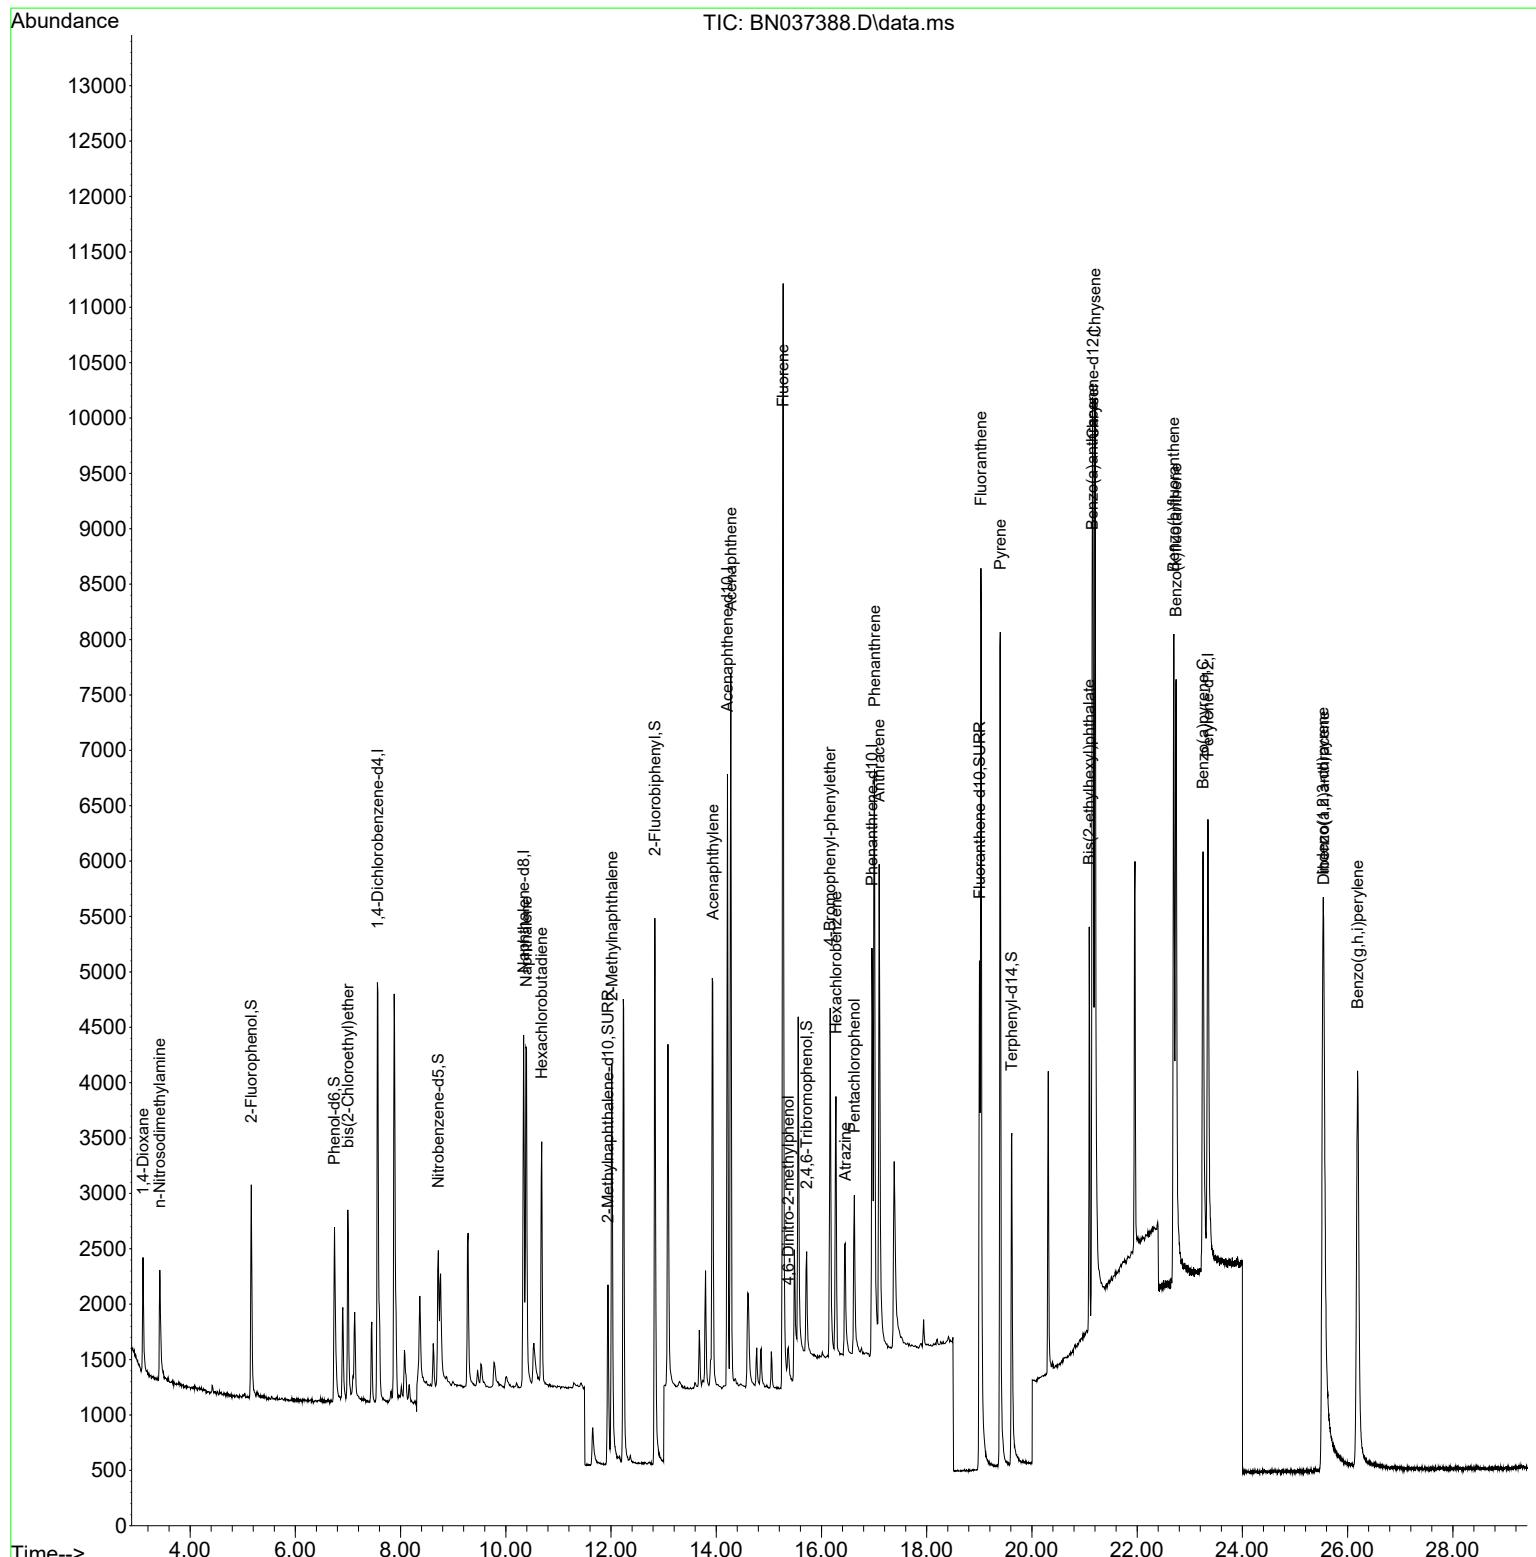


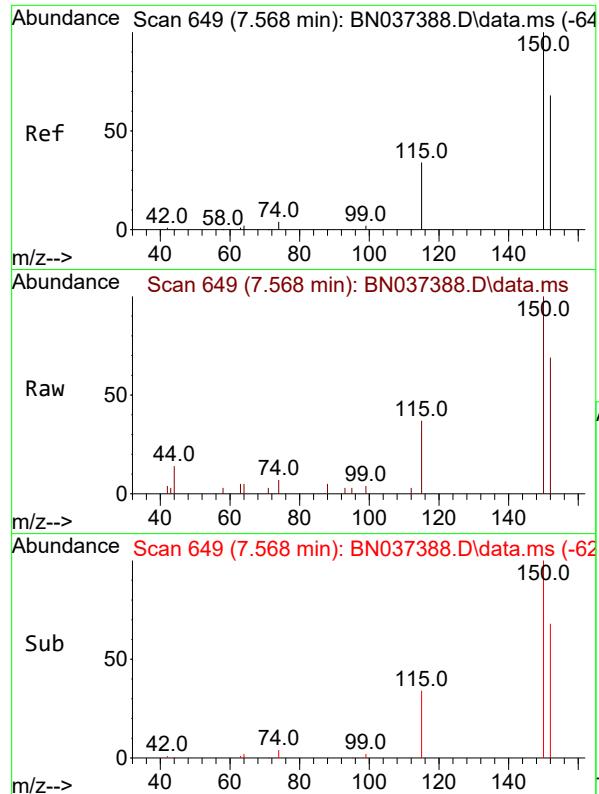

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4




Tgt Ion:152 Resp: 2117  
Ion Ratio Lower Upper  
152 100  
150 145.2 116.2 174.2  
115 53.6 42.9 64.3

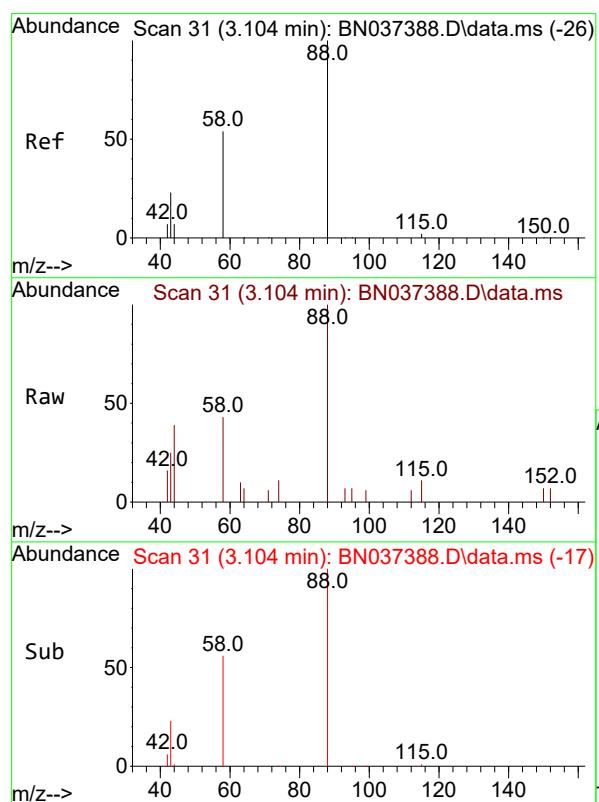

#2  
1,4-Dioxane  
Concen: 0.412 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53

Tgt Ion: 88 Resp: 781  
Ion Ratio Lower Upper  
88 100  
43 27.0 21.6 32.4  
58 57.4 45.9 68.9

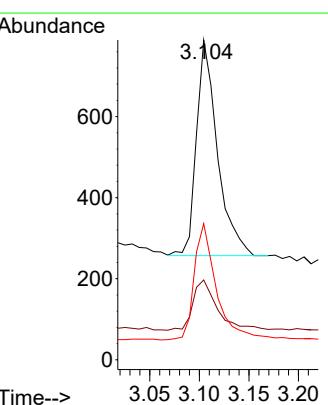



#3

n-Nitrosodimethylamine

Concen: 0.399 ng

RT: 3.422 min Scan# 7

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

Instrument :

BNA\_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion: 42 Resp: 792

Ion Ratio Lower Upper

42 100

74 122.3 97.8 146.8

44 10.9 8.7 13.1

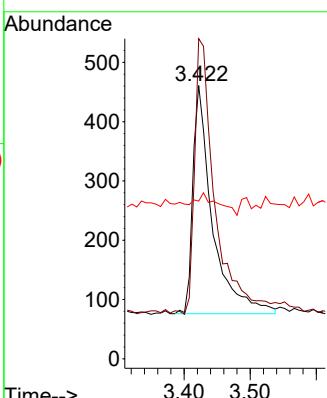

#4

2-Fluorophenol

Concen: 0.417 ng

RT: 5.163 min Scan# 316

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53


Tgt Ion: 112 Resp: 1703


Ion Ratio Lower Upper

112 100

64 50.4 40.3 60.5

63 32.6 26.1 39.1


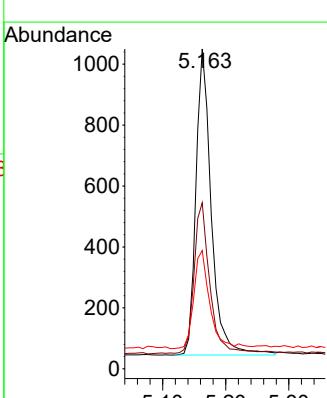


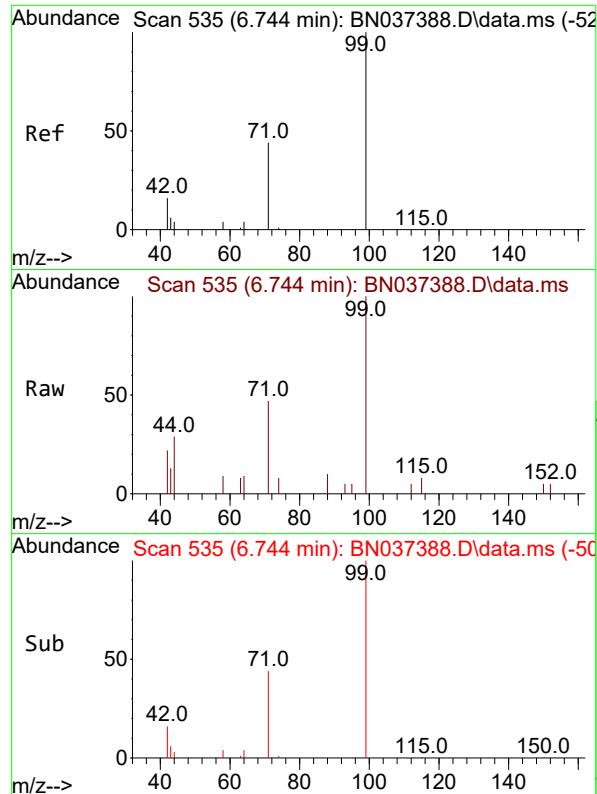

#5  
 Phenol-d6  
 Concen: 0.407 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion: 99 Resp: 1720  
 Ion Ratio Lower Upper  
 99 100  
 42 19.2 15.6 23.4  
 71 44.8 35.8 53.8

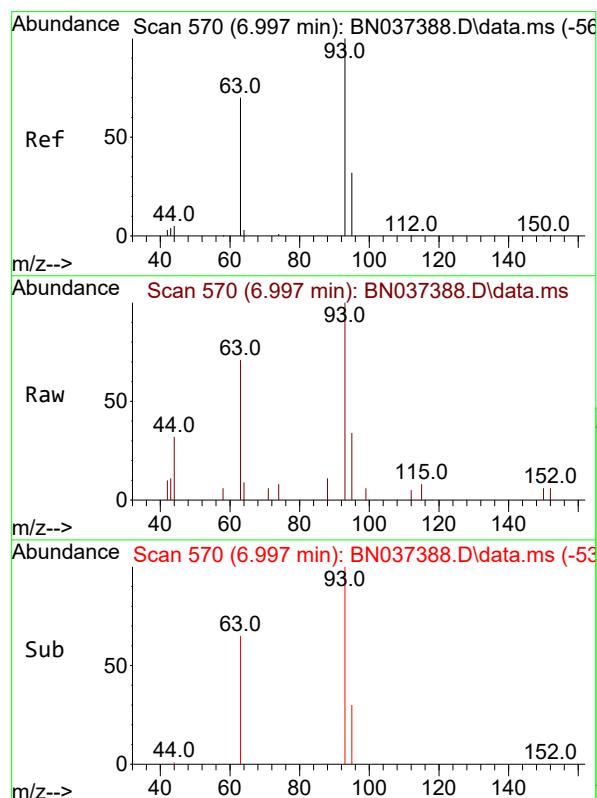

#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.404 ng  
 RT: 6.997 min Scan# 570  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53


Tgt Ion: 93 Resp: 1521  
 Ion Ratio Lower Upper  
 93 100  
 63 62.3 49.6 74.4  
 95 30.0 23.9 35.9







#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53

Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4




Tgt Ion:136 Resp: 4565



Ion	Ratio	Lower	Upper
136	100		
137	13.0	10.4	15.6
54	7.0	5.6	8.4
68	5.7	4.6	6.8

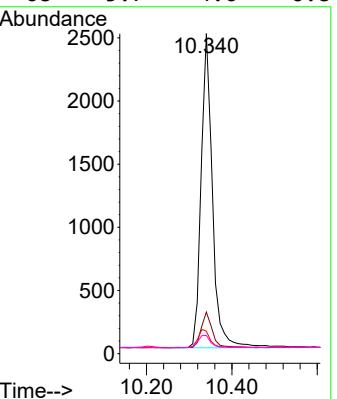


#8  
 Nitrobenzene-d5  
 Concen: 0.386 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53






Tgt Ion: 82 Resp: 1419  
 Ion Ratio Lower Upper  
 82 100  
 128 42.5 34.0 51.0  
 54 47.1 37.7 56.5

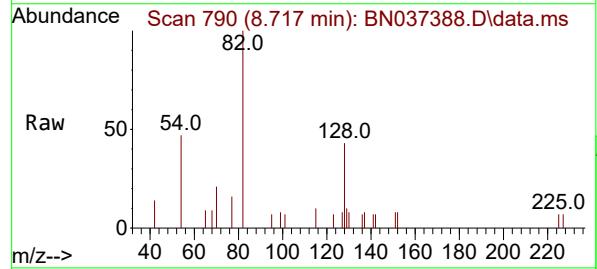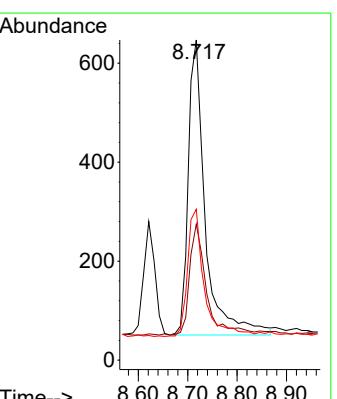

Abundance Scan 790 (8.717 min): BN037388.D\data.ms (-77)

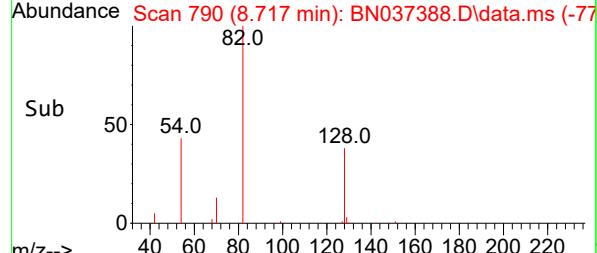



#9

Naphthalene

Concen: 0.388 ng

RT: 10.394 min Scan# 9

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

Instrument :

BNA\_N

ClientSampleId :

SSTDICCC0.4

Tgt Ion:128 Resp: 4559





Ion Ratio Lower Upper

128 100

129 13.0 10.4 15.6

127 15.3 12.2 18.4

Abundance

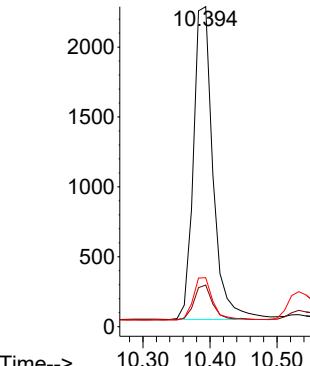

#10

Hexachlorobutadiene

Concen: 0.405 ng

RT: 10.682 min Scan# 974

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

Tgt Ion:225 Resp: 1887


Ion Ratio Lower Upper




225 100

223 0.0 0.0 0.0

227 62.4 49.9 74.9

Abundance




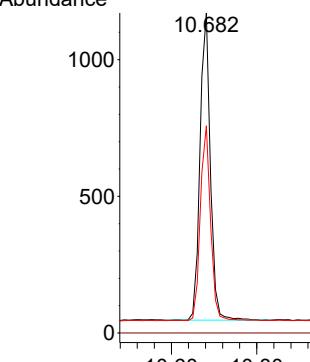




#11  
2-Methylnaphthalene-d10  
Concen: 0.372 ng  
RT: 11.940 min Scan# 1137  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4


Tgt Ion:152 Resp: 2629  
Ion Ratio Lower Upper  
152 100  
151 23.0 18.4 27.6

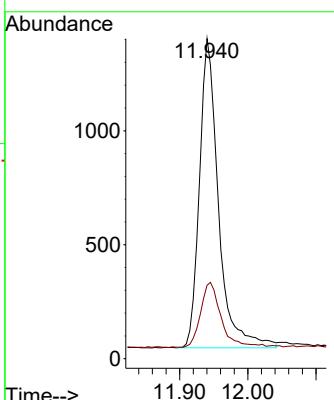

#12  
2-Methylnaphthalene  
Concen: 0.386 ng  
RT: 12.016 min Scan# 1152  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53

Tgt Ion:142 Resp: 3122  
Ion Ratio Lower Upper  
142 100  
141 87.6 70.1 105.1  
115 44.7 35.8 53.6


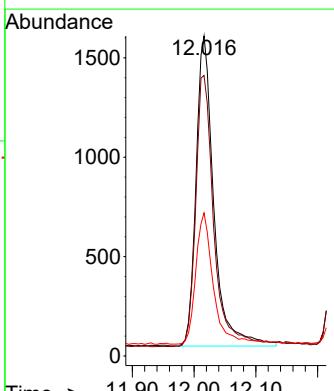


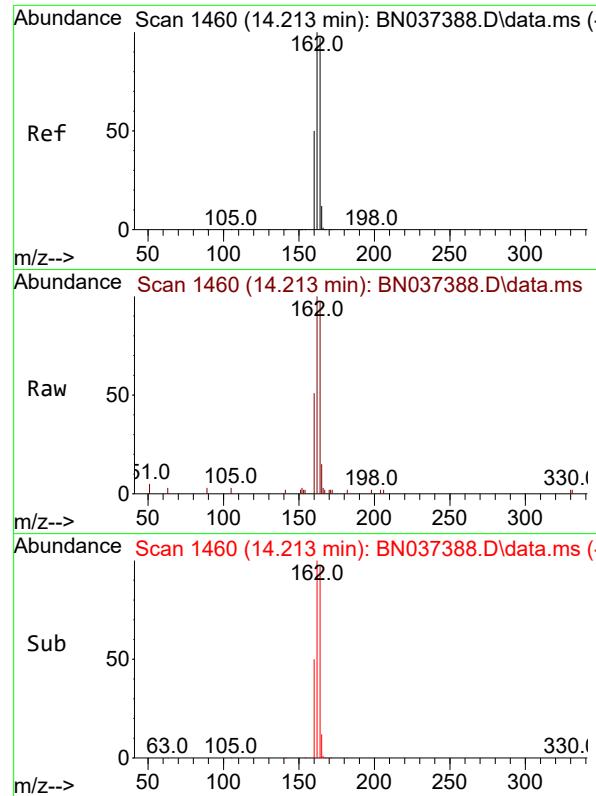


#13


Acenaphthene-d10  
Concen: 0.400 ngRT: 14.213 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53Instrument :  
BNA\_N  
ClientSampleId :  
SSTDICCC0.4

Tgt Ion:164 Resp: 3048

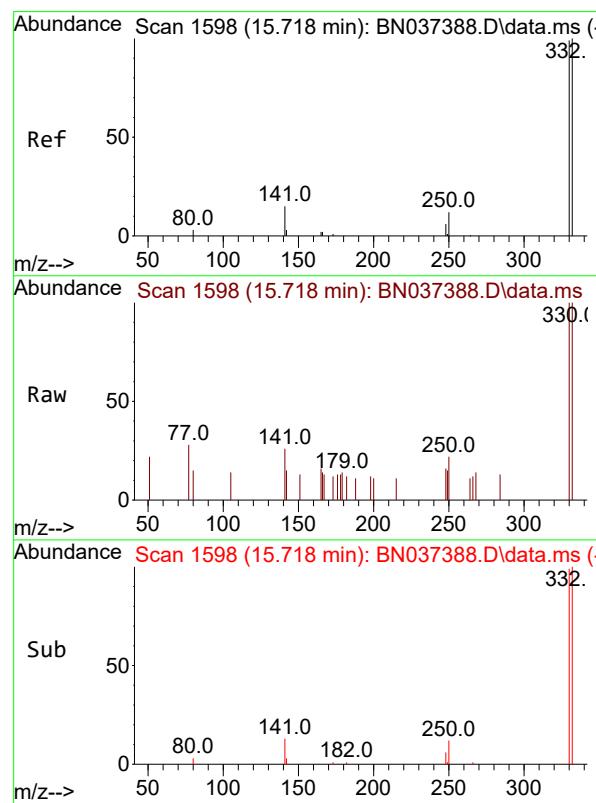Ion Ratio Lower Upper  
164 100  
162 103.2 82.6 123.8  
160 52.7 42.2 63.2



#14

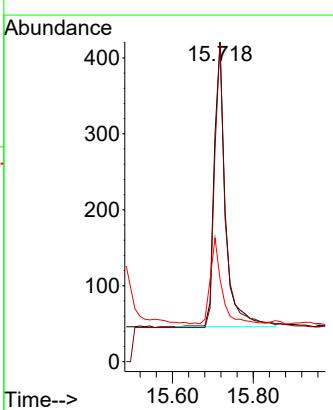2,4,6-Tribromophenol  
Concen: 0.408 ng  
RT: 15.718 min Scan# 1598  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53Tgt Ion:330 Resp: 729  
Ion Ratio Lower Upper  
330 100  
332 97.3 77.8 116.8  
141 30.0 24.0 36.0

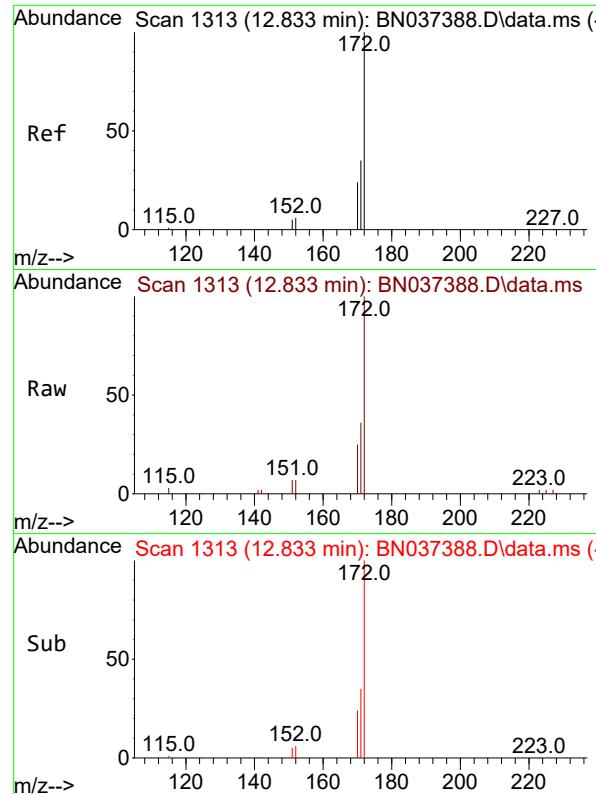


#15  
2-Fluorobiphenyl  
Concen: 0.399 ng  
RT: 12.833 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53  
ClientSampleId : SSTDICCC0.4




Tgt Ion:172 Resp: 5253  
Ion Ratio Lower Upper  
172 100  
171 36.0 28.8 43.2  
170 25.4 20.3 30.5

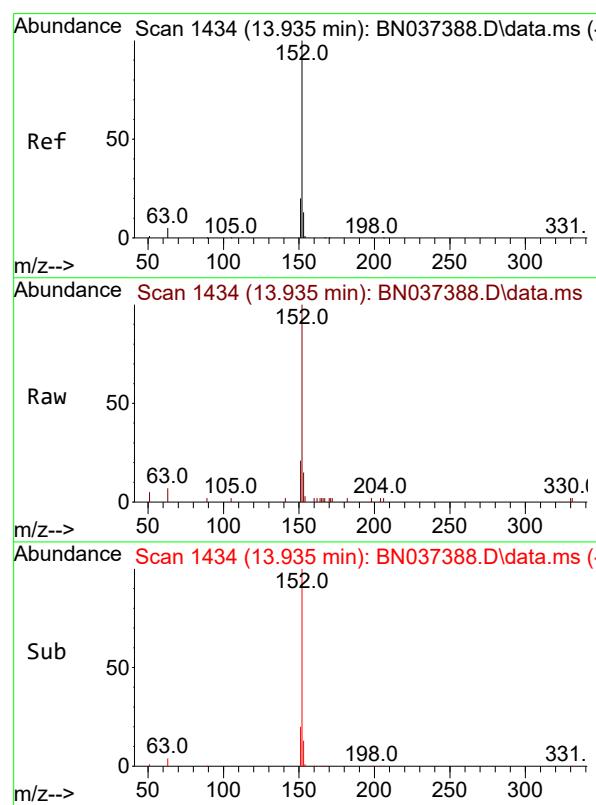

#16  
Acenaphthylene  
Concen: 0.380 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53

Tgt Ion:152 Resp: 4804  
Ion Ratio Lower Upper  
152 100  
151 19.7 15.8 23.6  
153 12.9 10.3 15.5





#17

Acenaphthene

Concen: 0.386 ng

RT: 14.277 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

Instrument :

BNA\_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:154 Resp: 3185

Ion Ratio Lower Upper

154 100

153 118.2 94.6 141.8

152 62.7 50.2 75.2

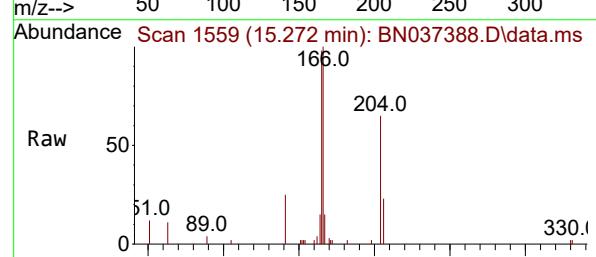

#18

Fluorene

Concen: 0.386 ng

RT: 15.272 min Scan# 1559

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53


Tgt Ion:166 Resp: 4498


Ion Ratio Lower Upper

166 100

165 99.3 79.4 119.2

167 13.2 10.6 15.8



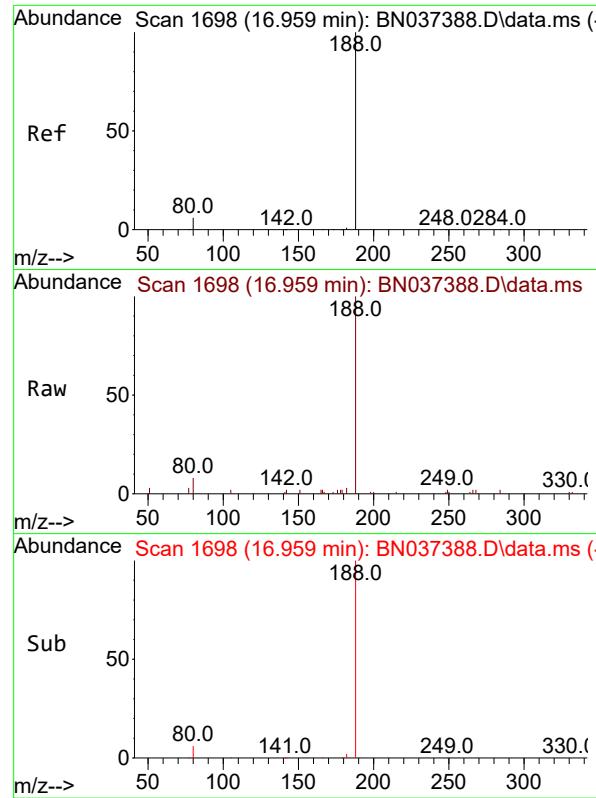

#19

Phenanthrene-d10  
Concen: 0.400 ng

RT: 16.959 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

Instrument:

BNA\_N

ClientSampleId :

SSTDICCC0.4

Tgt Ion:188 Resp: 6284

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 7.8 6.2 9.4

Abundance

16.959


3000

2000

1000

0

Time--&gt; 16.80 17.00

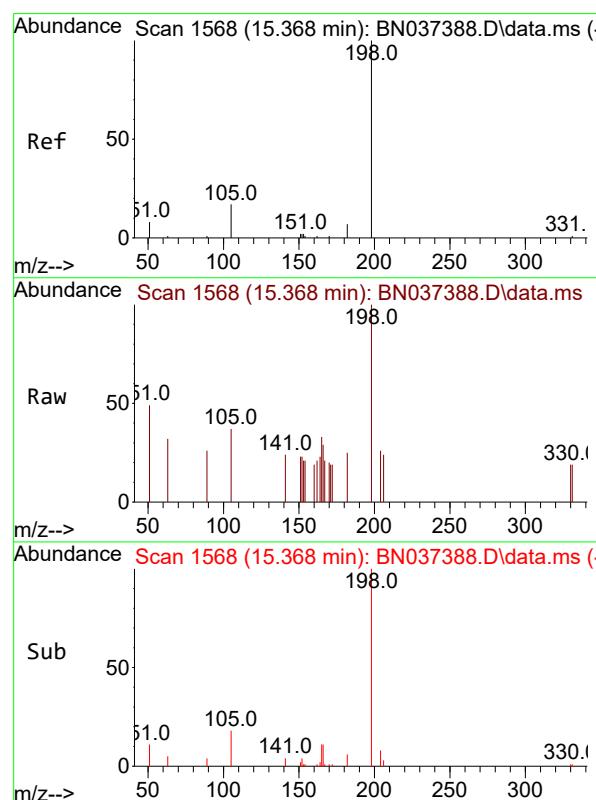

#20

4,6-Dinitro-2-methylphenol

Concen: 0.331 ng

RT: 15.368 min Scan# 1568

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

Tgt Ion:198 Resp: 535

Ion Ratio Lower Upper

198 100

51 48.5 38.8 58.2

105 37.2 29.8 44.6

Abundance

15.368

500

400


300

200

100



0

Time--&gt; 15.40

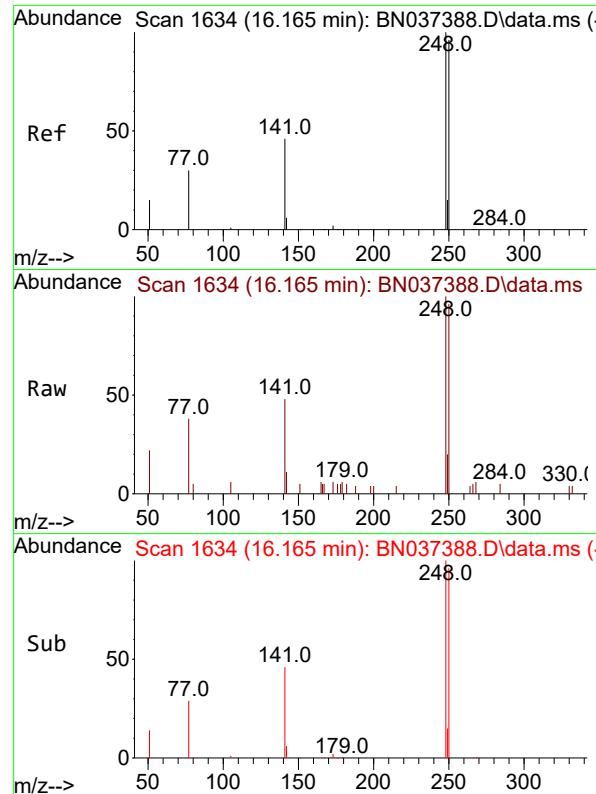


#21  
4-Bromophenyl-phenylether  
Concen: 0.382 ng  
RT: 16.165 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037388.D ClientSampleId : SSTDICCC0.4  
Acq: 26 Jun 2025 11:53




Tgt Ion:248 Resp: 1694  
Ion Ratio Lower Upper  
248 100  
250 96.2 77.0 115.4  
141 48.4 38.7 58.1

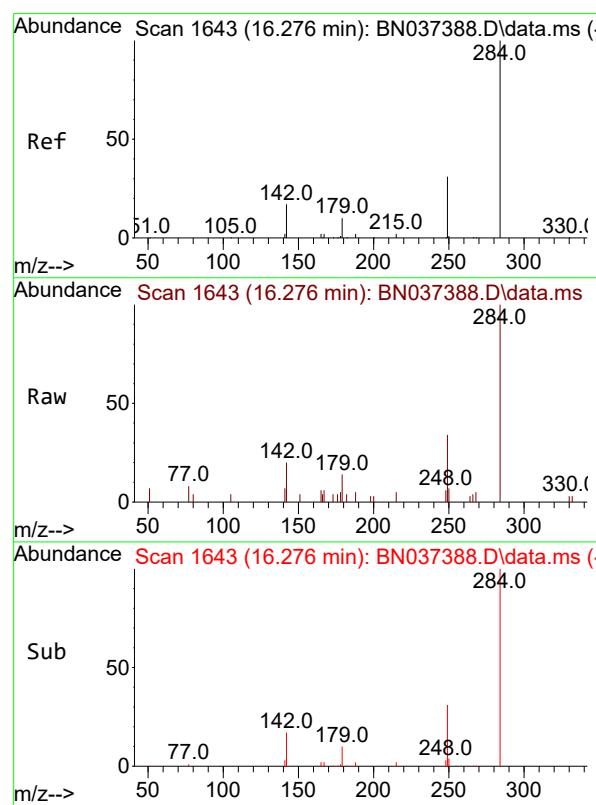

#22  
Hexachlorobenzene  
Concen: 0.398 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53

Tgt Ion:284 Resp: 1899  
Ion Ratio Lower Upper  
284 100  
142 34.0 27.2 40.8  
249 33.4 26.7 40.1

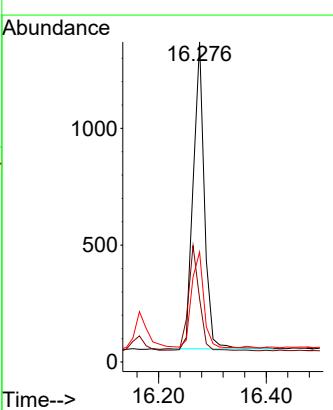

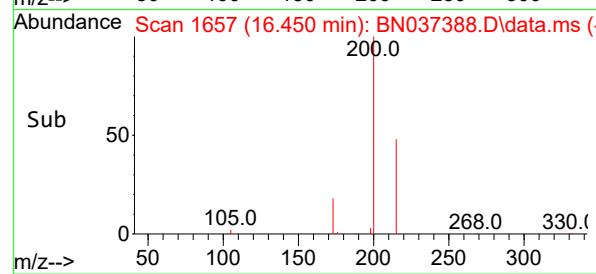

#23

Atrazine

Concen: 0.380 ng

RT: 16.450 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

Instrument:

BNA\_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:200 Resp: 1336

Ion Ratio Lower Upper

200 100

173 23.8 19.0 28.6

215 51.6 41.3 61.9

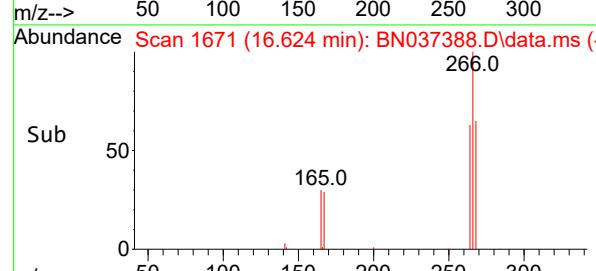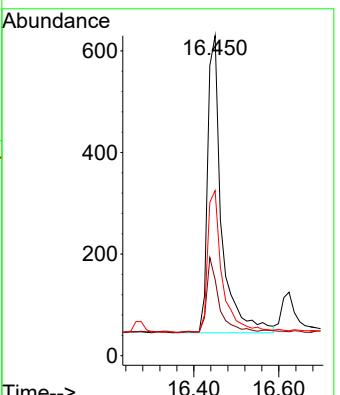

#24

Pentachlorophenol

Concen: 0.378 ng

RT: 16.624 min Scan# 1671

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53


Tgt Ion:266 Resp: 973


Ion Ratio Lower Upper

266 100

264 60.4 49.2 73.8

268 67.3 54.2 81.4


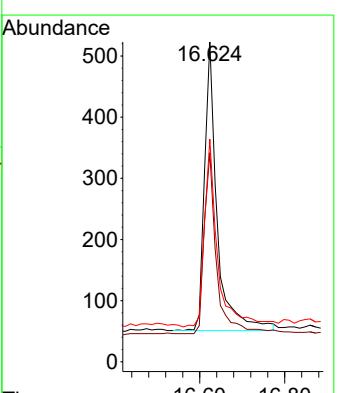


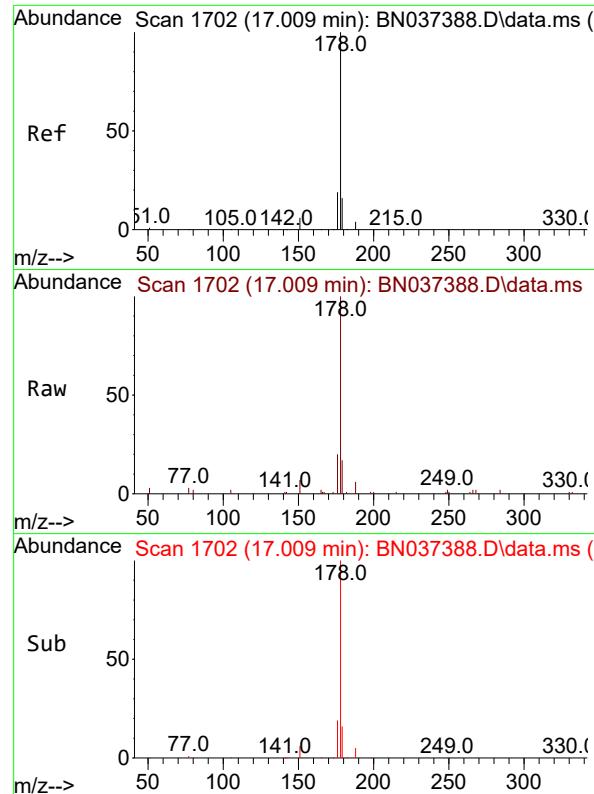

#25  
Phenanthrene  
Concen: 0.383 ng  
RT: 17.009 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4


Tgt Ion:178 Resp: 6787  
Ion Ratio Lower Upper  
178 100  
176 19.5 15.6 23.4  
179 16.0 12.8 19.2

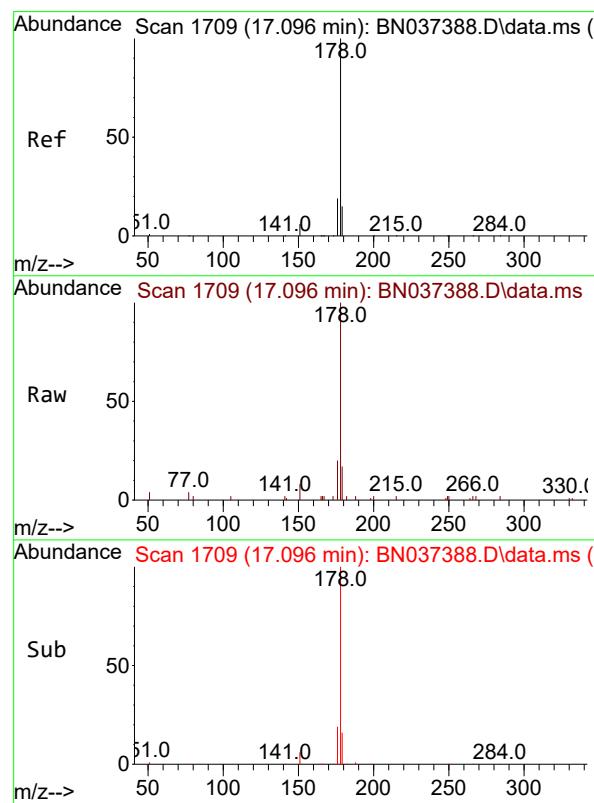

#26  
Anthracene  
Concen: 0.374 ng  
RT: 17.096 min Scan# 1709  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53

Tgt Ion:178 Resp: 6087  
Ion Ratio Lower Upper  
178 100  
176 18.6 14.9 22.3  
179 15.5 12.4 18.6





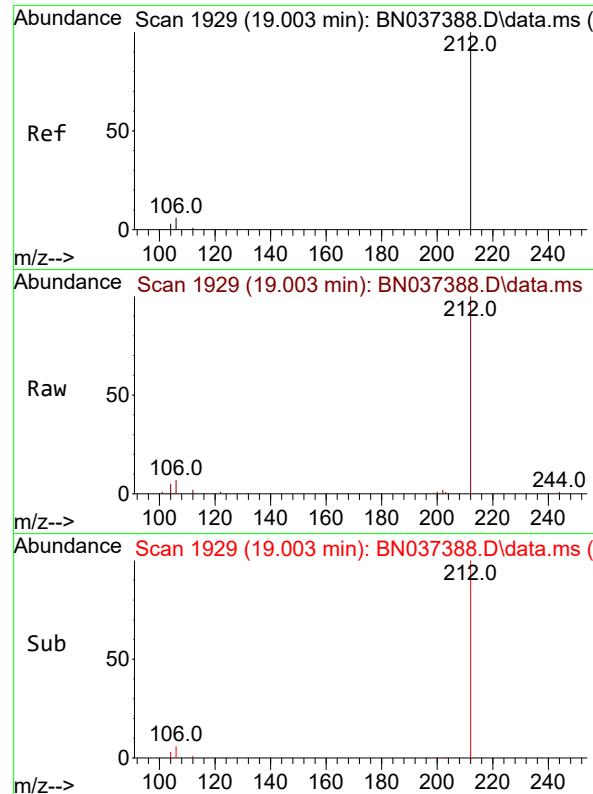

#27  
 Fluoranthene-d10  
 Concen: 0.371 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:212 Resp: 6680  
 Ion Ratio Lower Upper  
 212 100  
 106 5.6 4.5 6.7  
 104 3.4 2.7 4.1

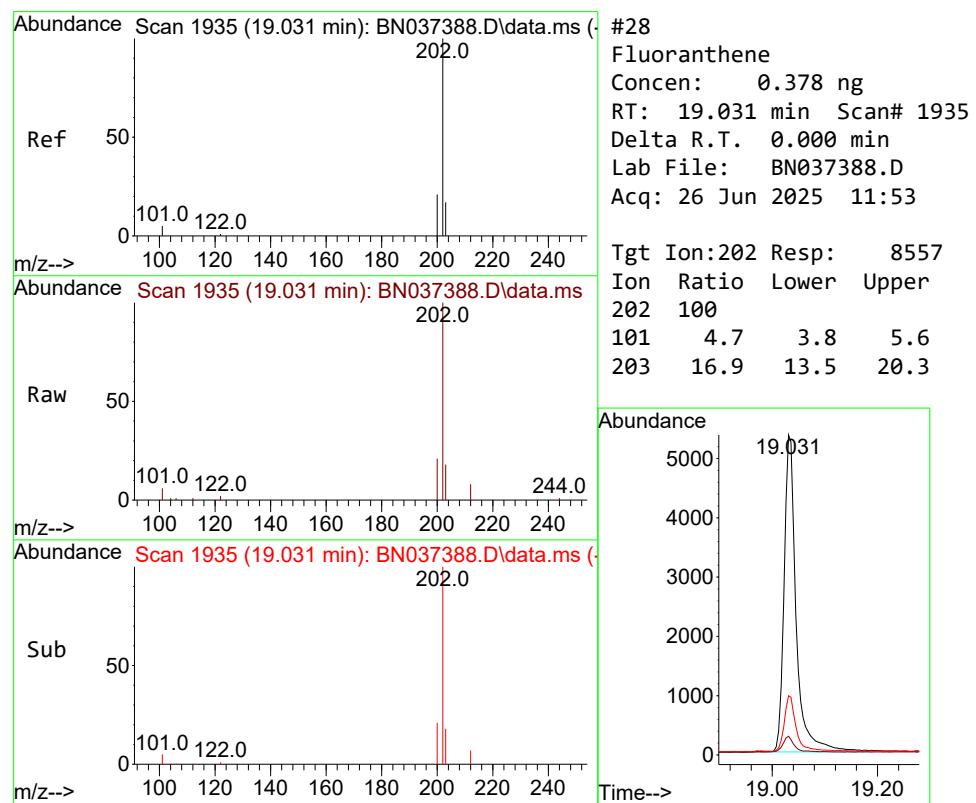

#28  
 Fluoranthene  
 Concen: 0.378 ng  
 RT: 19.031 min Scan# 1935  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53

Tgt Ion:202 Resp: 8557  
 Ion Ratio Lower Upper  
 202 100  
 101 4.7 3.8 5.6  
 203 16.9 13.5 20.3





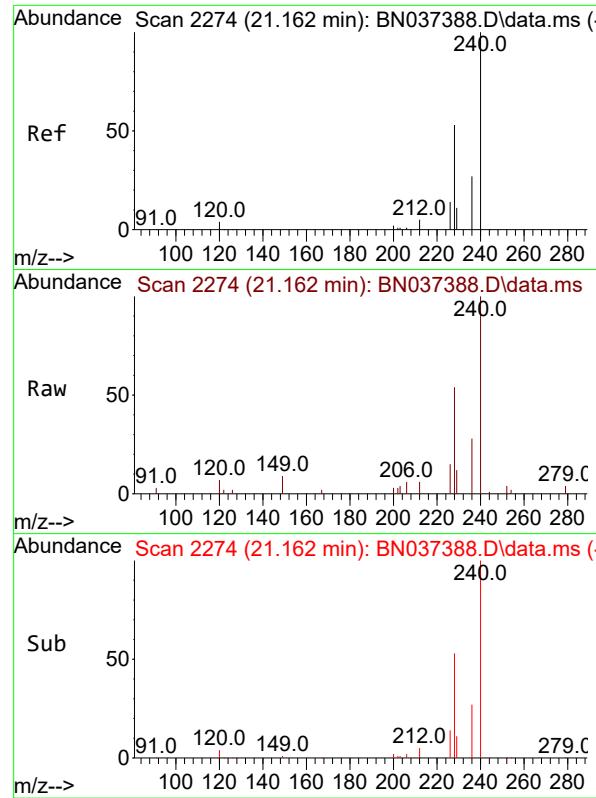

#29  
 Chrysene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 21.162 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:240 Resp: 5612  
 Ion Ratio Lower Upper  
 240 100  
 120 6.6 5.3 7.9  
 236 28.4 22.7 34.1

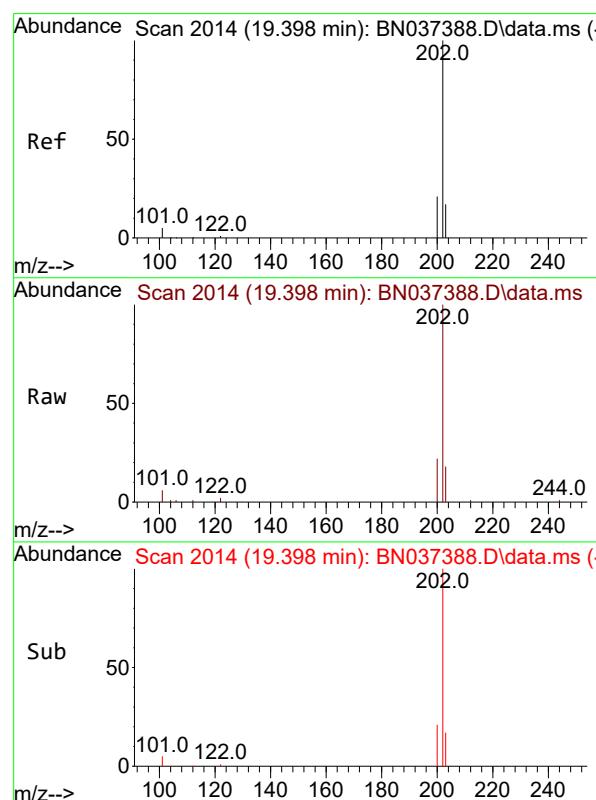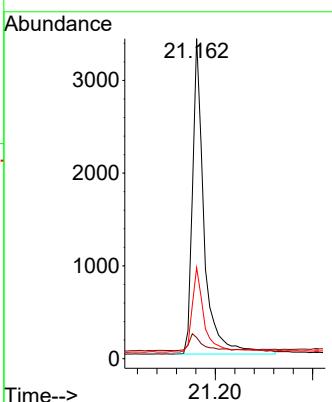

#30  
 Pyrene  
 Concen: 0.405 ng  
 RT: 19.398 min Scan# 2014  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53



Tgt Ion:202 Resp: 8607  
 Ion Ratio Lower Upper  
 202 100  
 200 20.6 16.5 24.7  
 203 17.7 14.2 21.2



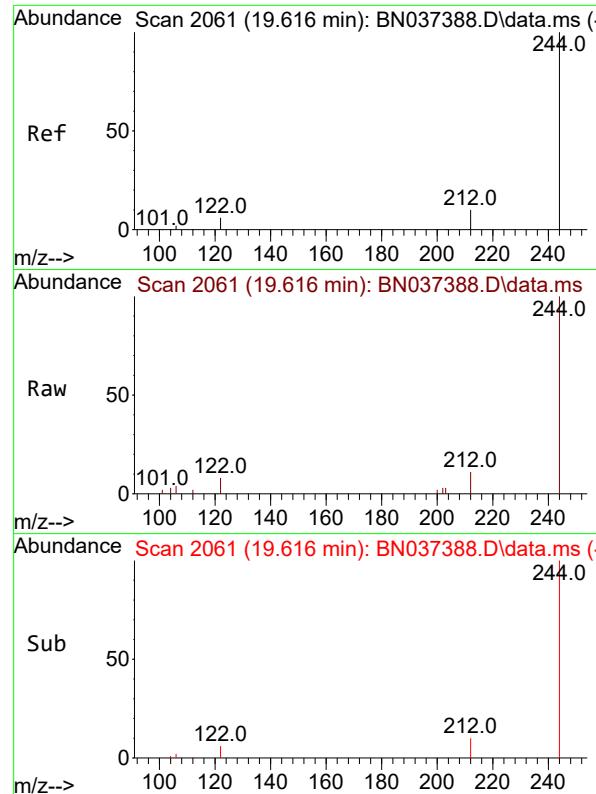


#31  
Terphenyl-d14  
Concen: 0.407 ng  
RT: 19.616 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53 ClientSampleId : SSTDICCC0.4


Tgt Ion:244 Resp: 4873  
Ion Ratio Lower Upper  
244 100  
212 11.4 9.1 13.7  
122 7.9 6.3 9.5

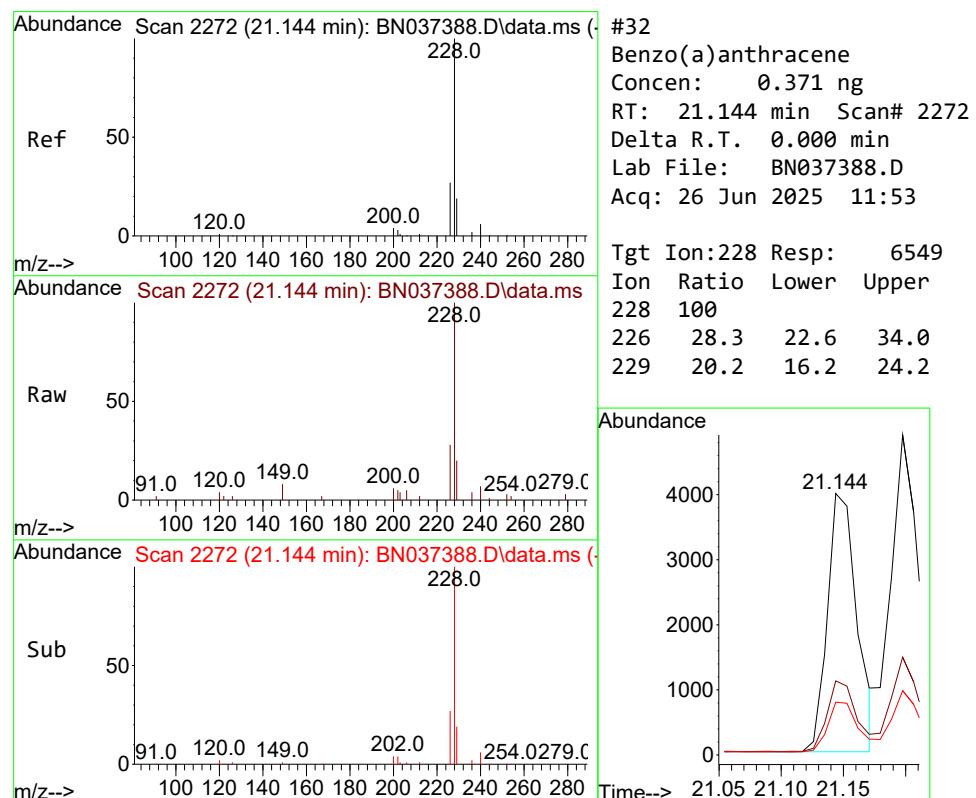

#32  
Benzo(a)anthracene  
Concen: 0.371 ng  
RT: 21.144 min Scan# 2272  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53



Tgt Ion:228 Resp: 6549  
Ion Ratio Lower Upper  
228 100  
226 28.3 22.6 34.0  
229 20.2 16.2 24.2



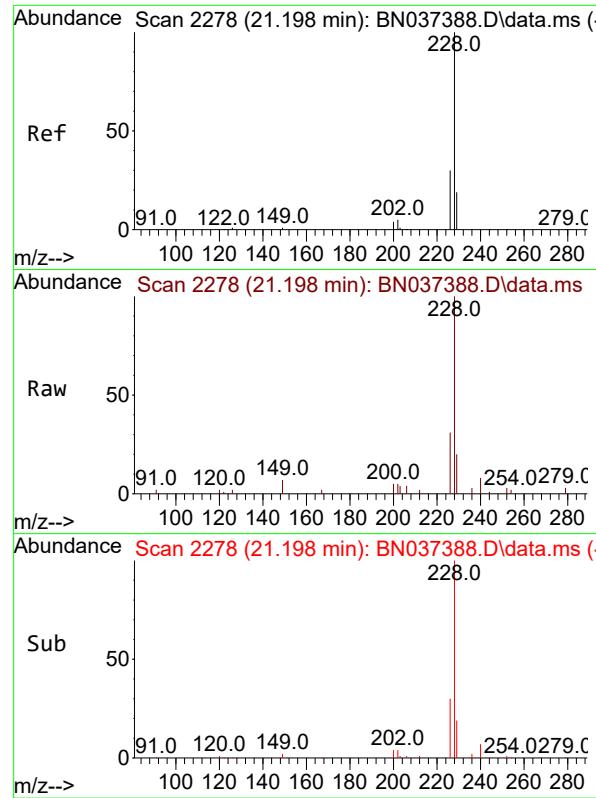


#33  
Chrysene  
Concen: 0.407 ng  
RT: 21.198 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53 ClientSampleId : SSTDICCC0.4


Tgt Ion:228 Resp: 8883  
Ion Ratio Lower Upper  
228 100  
226 30.6 24.5 36.7  
229 20.1 16.1 24.1

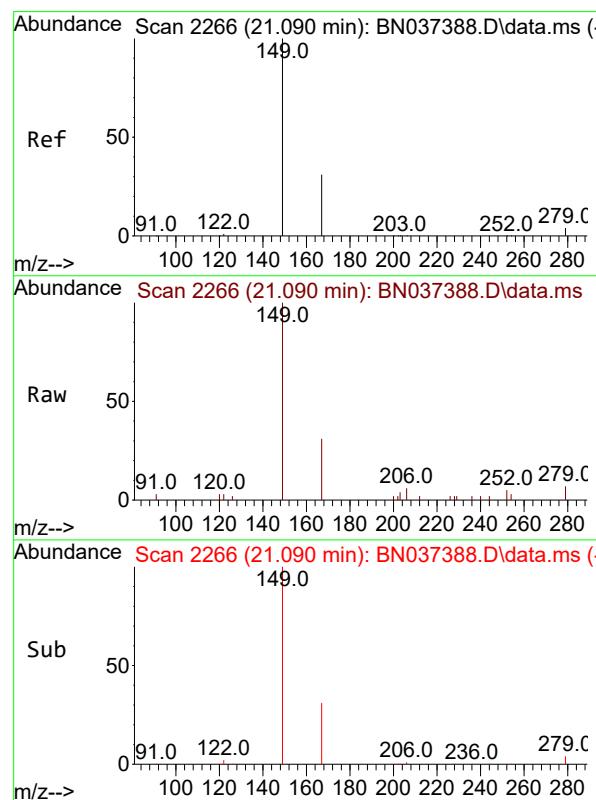

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.405 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. 0.000 min  
Lab File: BN037388.D  
Acq: 26 Jun 2025 11:53

Tgt Ion:149 Resp: 2830  
Ion Ratio Lower Upper  
149 100  
167 31.0 24.8 37.2  
279 6.3 5.0 7.6





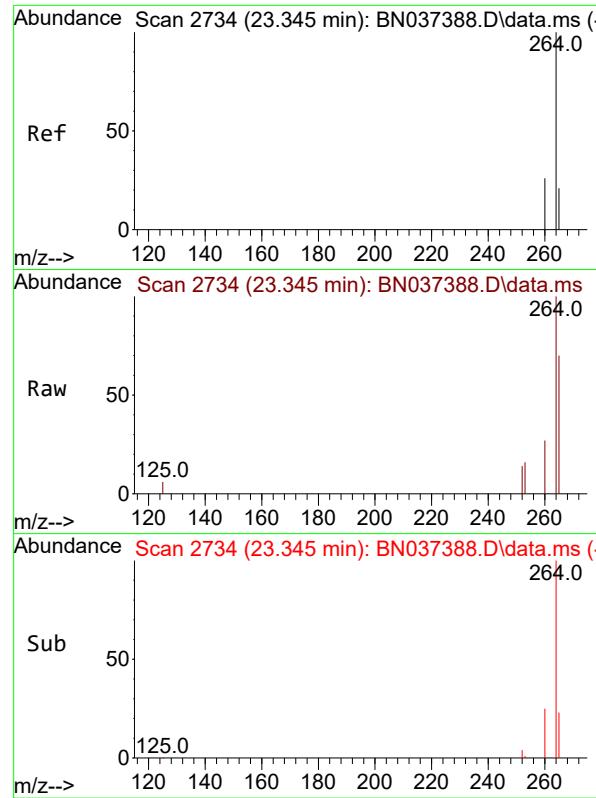

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.345 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:264 Resp: 5950  
 Ion Ratio Lower Upper  
 264 100  
 260 26.7 21.4 32.0  
 265 70.3 56.2 84.4

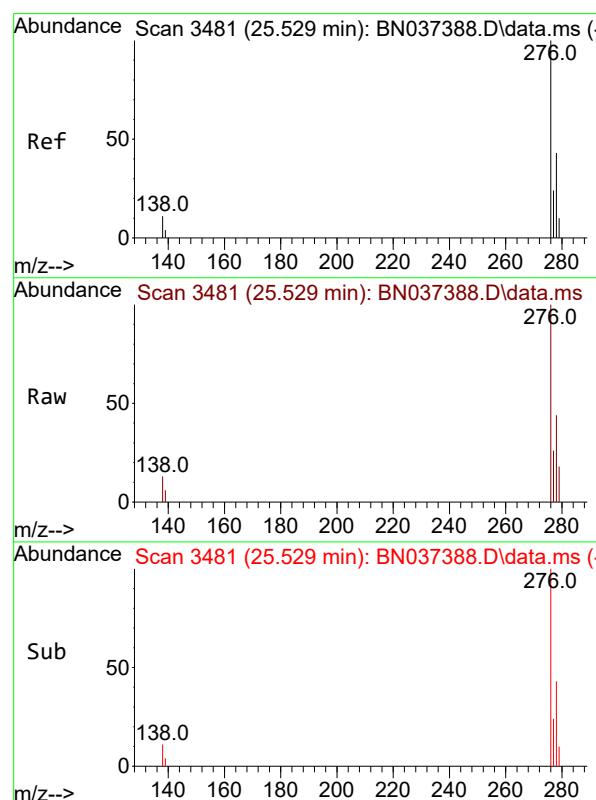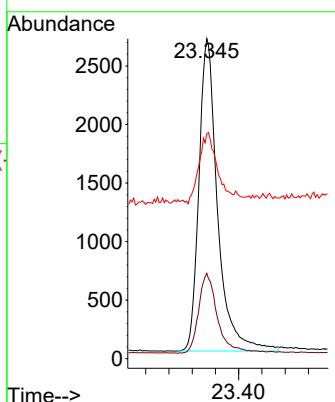

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.374 ng  
 RT: 25.529 min Scan# 3481  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53

Tgt Ion:276 Resp: 9382  
 Ion Ratio Lower Upper  
 276 100  
 138 10.6 8.5 12.7  
 277 24.6 19.7 29.5



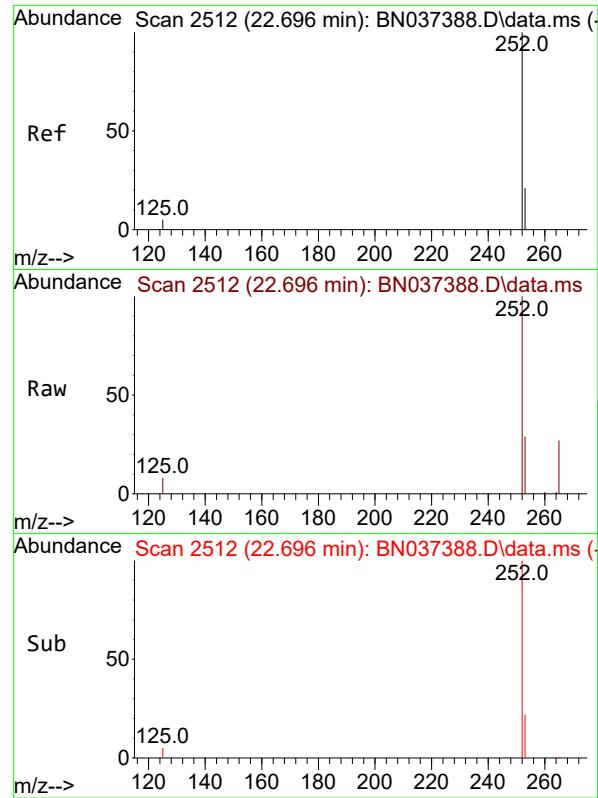

#37

Benzo(b)fluoranthene

Concen: 0.374 ng

RT: 22.696 min Scan# 2

Instrument :

BNA\_N

Delta R.T. 0.000 min

Lab File: BN037388.D

ClientSampleId :

Acq: 26 Jun 2025 11:53

SSTDICCC0.4


Tgt Ion:252 Resp: 7840

Ion Ratio Lower Upper

252 100

253 28.5 22.8 34.2

125 7.8 6.2 9.4



#38

Benzo(k)fluoranthene

Concen: 0.388 ng

RT: 22.740 min Scan# 2527

Delta R.T. 0.000 min

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53



Tgt Ion:252 Resp: 8696


Ion Ratio Lower Upper

252 100

253 29.0 23.2 34.8

125 7.5 6.0 9.0

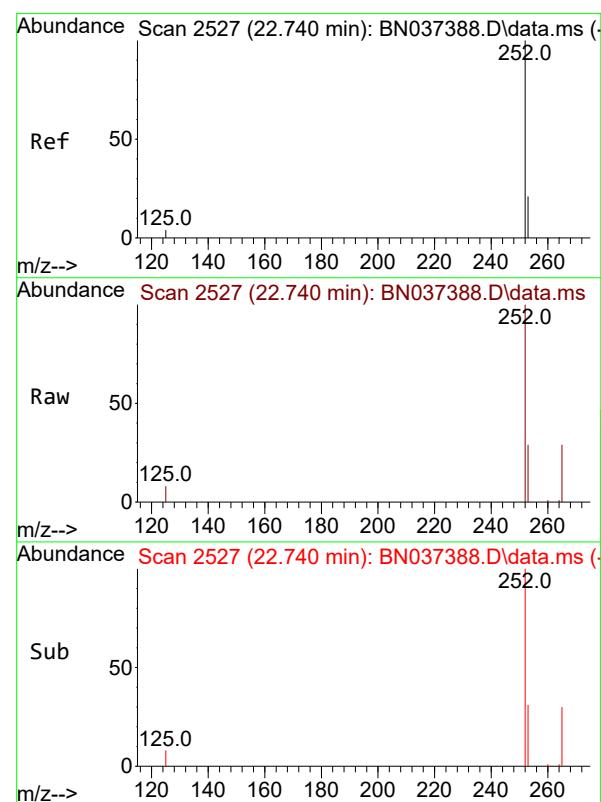



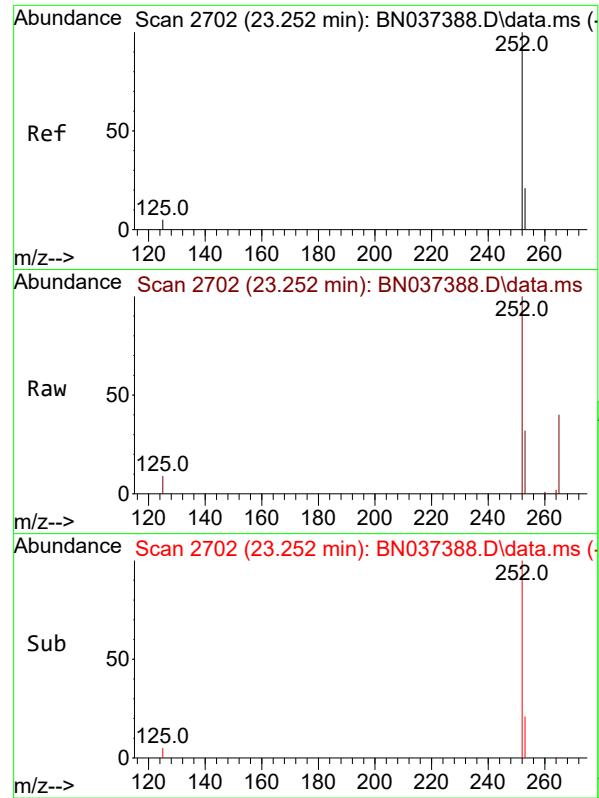

#39  
 Benzo(a)pyrene  
 Concen: 0.377 ng  
 RT: 23.252 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:252 Resp: 7038  
 Ion Ratio Lower Upper  
 252 100  
 253 32.0 25.6 38.4  
 125 9.4 7.5 11.3

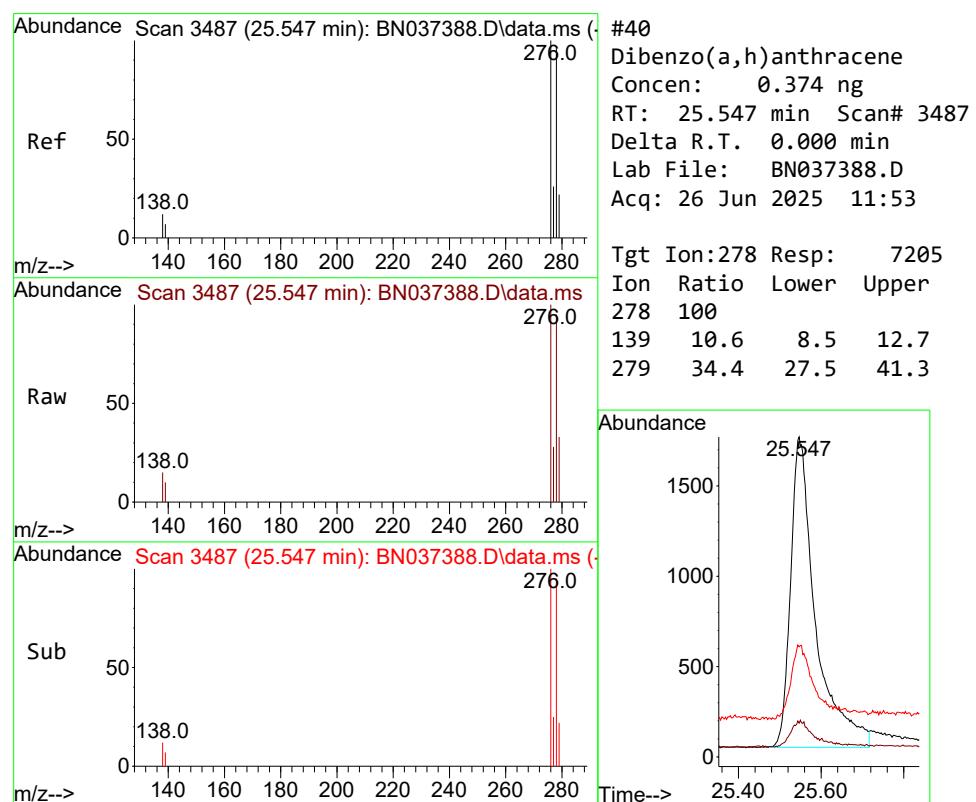

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.374 ng  
 RT: 25.547 min Scan# 3487  
 Delta R.T. 0.000 min  
 Lab File: BN037388.D  
 Acq: 26 Jun 2025 11:53

Tgt Ion:278 Resp: 7205  
 Ion Ratio Lower Upper  
 278 100  
 139 10.6 8.5 12.7  
 279 34.4 27.5 41.3



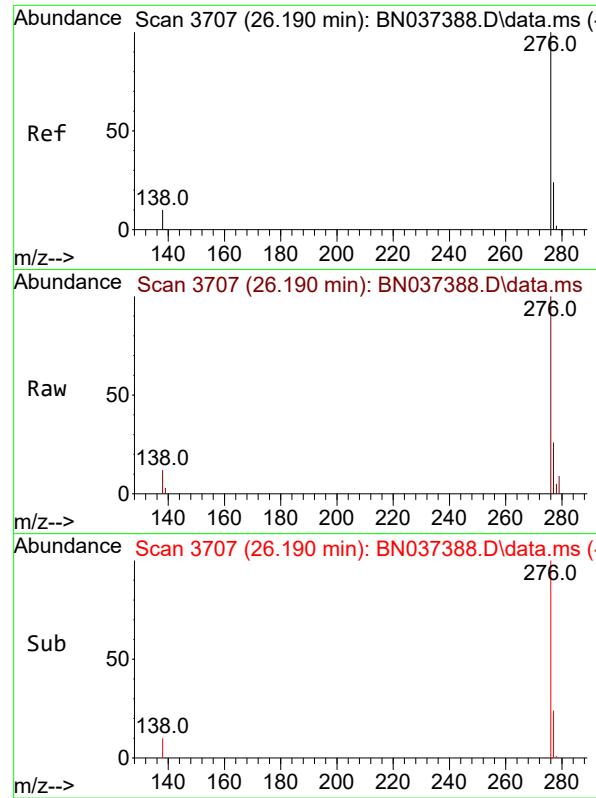

#41

Benzo(g,h,i)perylene

Concen: 0.382 ng

RT: 26.190 min Scan# 3

Instrument :

BNA\_N

Delta R.T. 0.000 min

ClientSampleId :

Lab File: BN037388.D

Acq: 26 Jun 2025 11:53

SSTDICCC0.4


Tgt Ion:276 Resp: 8788

Ion Ratio Lower Upper

276 100

277 26.2 21.0 31.4

138 12.0 9.6 14.4

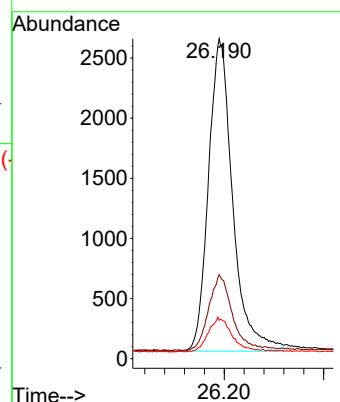

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037389.D  
 Acq On : 26 Jun 2025 12:29  
 Operator : RC/JU  
 Sample : SSTDICCO.8  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
BNA\_N  
**ClientSampleId :**  
SSTDICCO.8

Quant Time: Jun 26 14:44:25 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1666	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	3597	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	2328	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	4756	0.400	ng	0.00
29) Chrysene-d12	21.162	240	4408	0.400	ng	0.00
35) Perylene-d12	23.345	264	4628	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	2321	0.723	ng	0.00
5) Phenol-d6	6.744	99	2457	0.738	ng	0.00
8) Nitrobenzene-d5	8.717	82	2126	0.735	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	4083	0.734	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	1046	0.766	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	7691	0.765	ng	0.00
27) Fluoranthene-d10	19.003	212	9775	0.717	ng	0.00
31) Terphenyl-d14	19.612	244	7017	0.747	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	1220	0.817	ng	97
3) n-Nitrosodimethylamine	3.415	42	1219	0.781	ng	# 98
6) bis(2-Chloroethyl)ether	6.997	93	2313	0.781	ng	99
9) Naphthalene	10.383	128	6991	0.755	ng	98
10) Hexachlorobutadiene	10.682	225	2877	0.783	ng	# 99
12) 2-Methylnaphthalene	12.011	142	4762	0.747	ng	97
16) Acenaphthylene	13.925	152	7160	0.742	ng	99
17) Acenaphthene	14.277	154	4696	0.745	ng	100
18) Fluorene	15.272	166	6613	0.743	ng	99
20) 4,6-Dinitro-2-methylph...	15.368	198	826	0.676	ng	# 79
21) 4-Bromophenyl-phenylether	16.165	248	2555	0.762	ng	96
22) Hexachlorobenzene	16.276	284	2768	0.767	ng	99
23) Atrazine	16.438	200	1939	0.730	ng	97
24) Pentachlorophenol	16.624	266	1406	0.722	ng	96
25) Phenanthrene	17.009	178	9870	0.737	ng	99
26) Anthracene	17.096	178	9124	0.741	ng	99
28) Fluoranthene	19.031	202	12556	0.734	ng	100
30) Pyrene	19.398	202	12616	0.756	ng	100
32) Benzo(a)anthracene	21.144	228	10155	0.733	ng	100
33) Chrysene	21.198	228	13144	0.767	ng	100
34) Bis(2-ethylhexyl)phtha...	21.090	149	4107	0.749	ng	99
36) Indeno(1,2,3-cd)pyrene	25.529	276	14993	0.768	ng	98
37) Benzo(b)fluoranthene	22.693	252	12221	0.749	ng	96
38) Benzo(k)fluoranthene	22.737	252	13232	0.759	ng	96
39) Benzo(a)pyrene	23.252	252	10863	0.748	ng	95
40) Dibenzo(a,h)anthracene	25.547	278	11379	0.759	ng	94
41) Benzo(g,h,i)perylene	26.187	276	13535	0.756	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037389.D  
 Acq On : 26 Jun 2025 12:29  
 Operator : RC/JU  
 Sample : SSTDICC0.8  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC0.8


Quant Time: Jun 26 14:44:25 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration

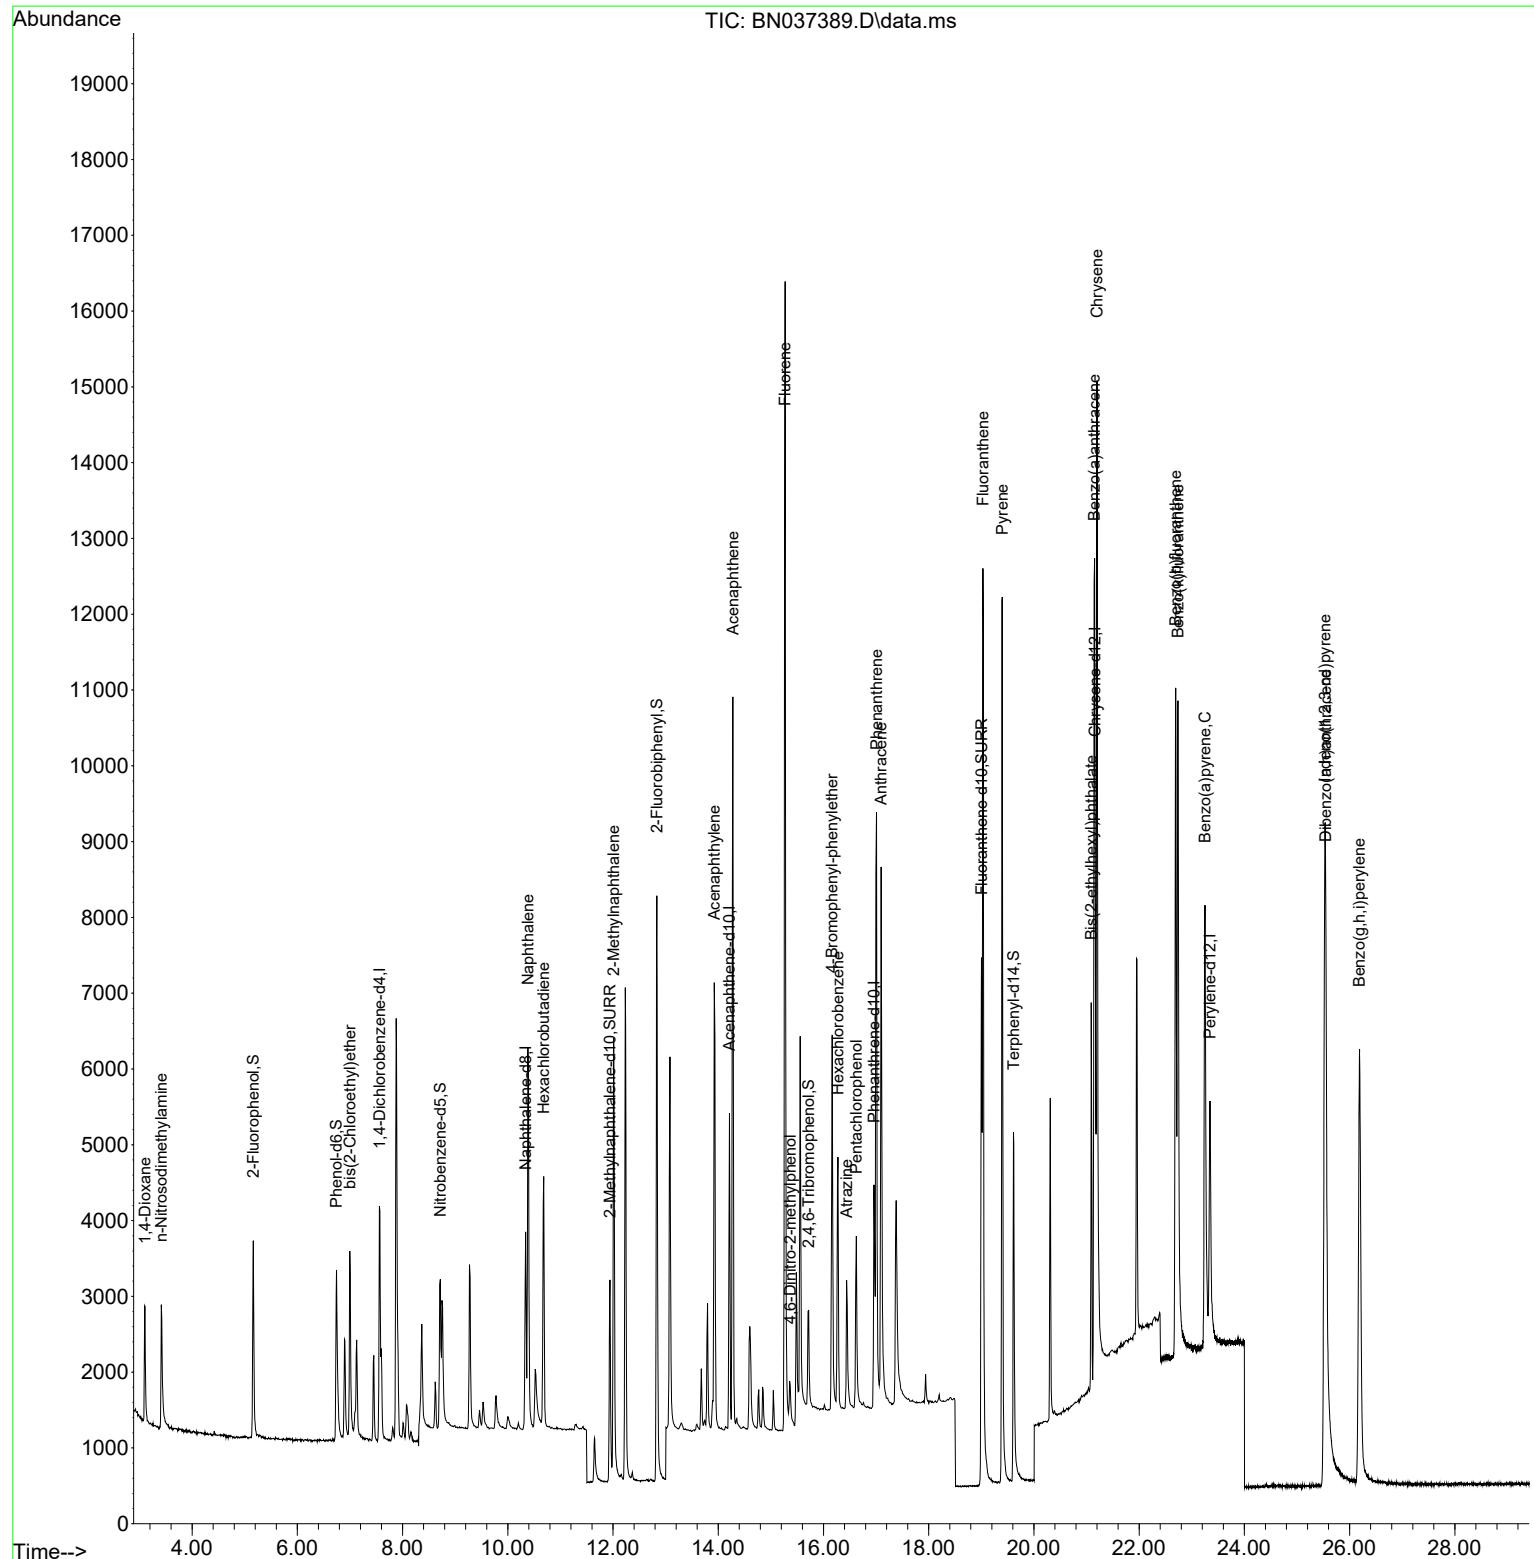






#1  
 1,4-Dichlorobenzene-d4  
 Concen: 0.400 ng  
 RT: 7.568 min Scan# 6  
 Delta R.T. -0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29




Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


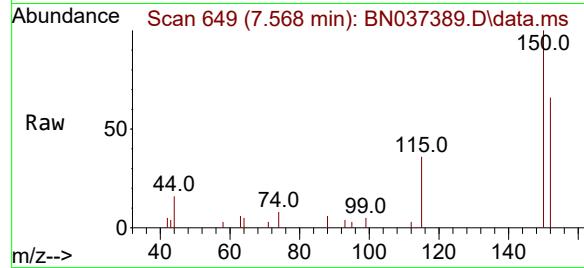



Tgt Ion:152 Resp: 1666  
 Ion Ratio Lower Upper  
 152 100  
 150 150.7 116.2 174.2  
 115 54.9 42.9 64.3

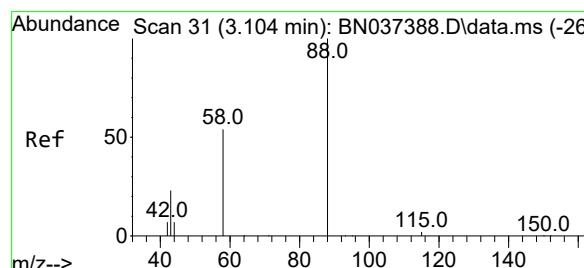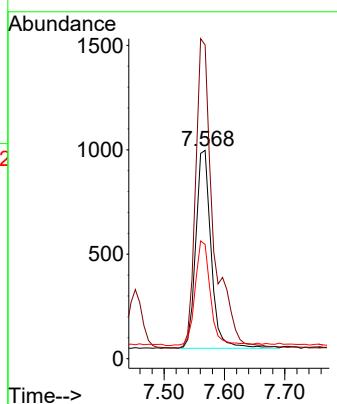

#2  
 1,4-Dioxane  
 Concen: 0.817 ng  
 RT: 3.104 min Scan# 31  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29

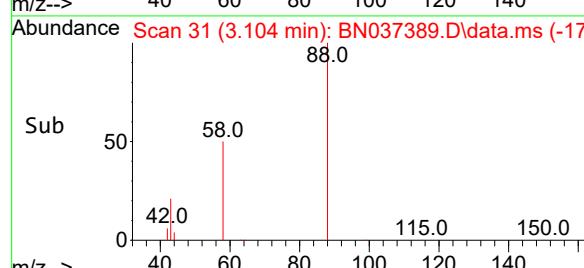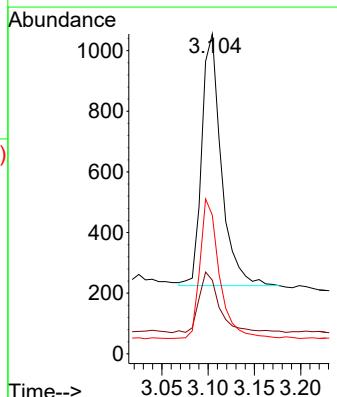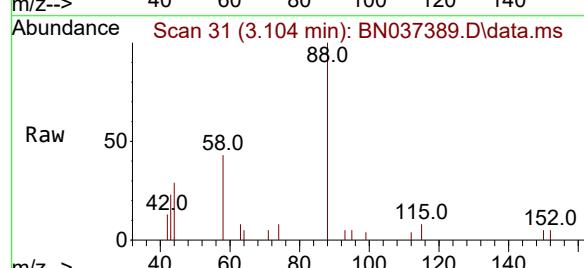


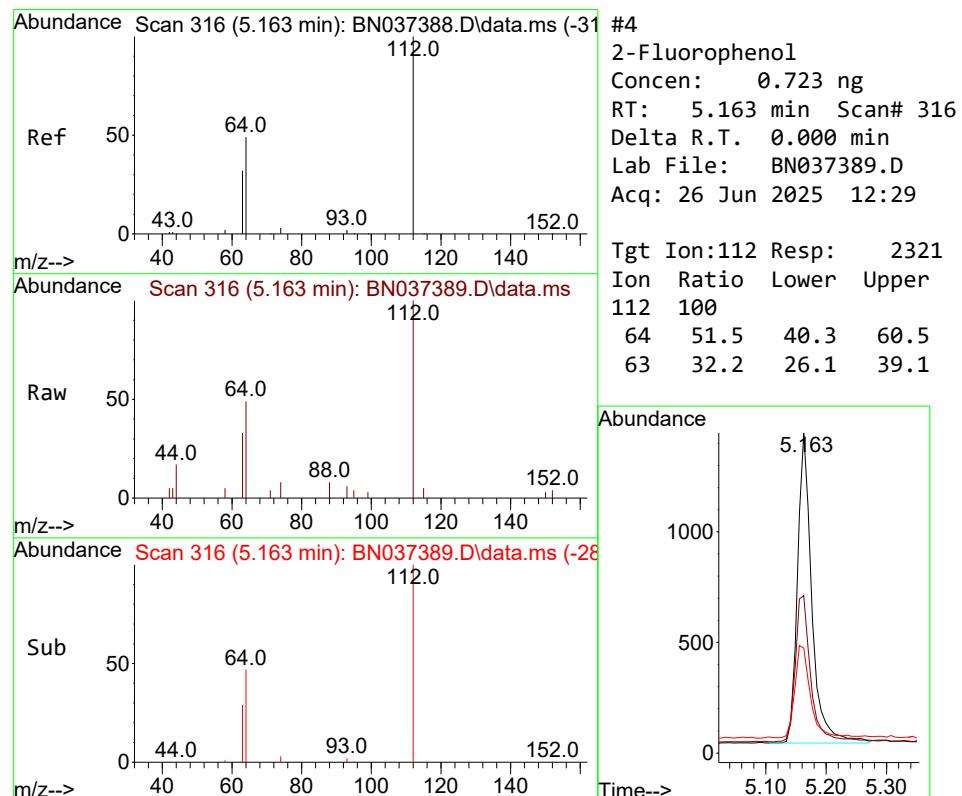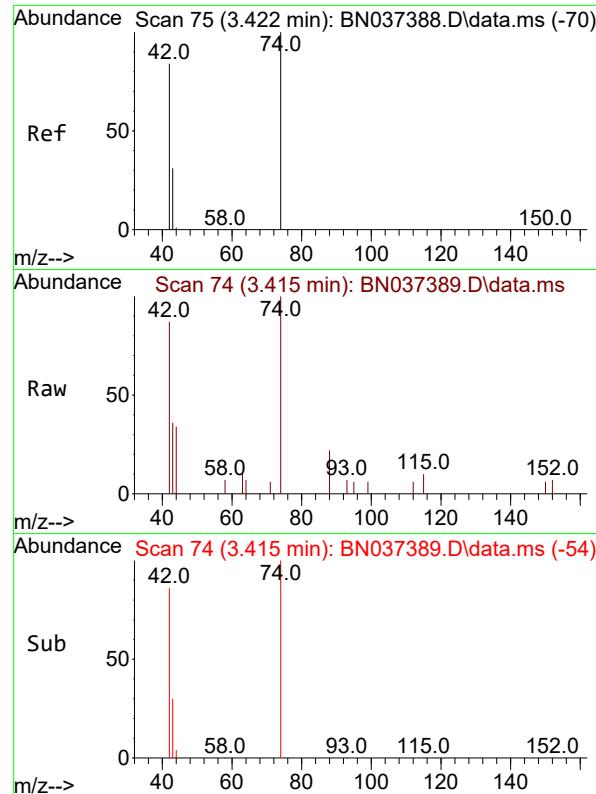





#5  
Phenol-d6  
Concen: 0.738 ng  
RT: 6.744 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8





Tgt Ion: 99 Resp: 2457  
Ion Ratio Lower Upper  
99 100  
42 18.7 15.6 23.4  
71 43.0 35.8 53.8

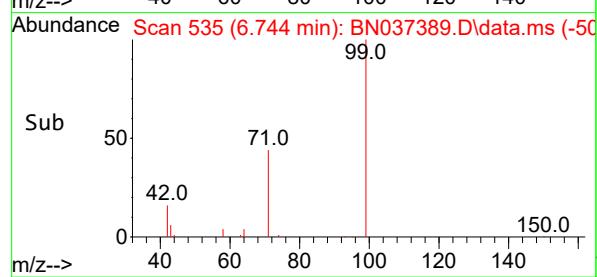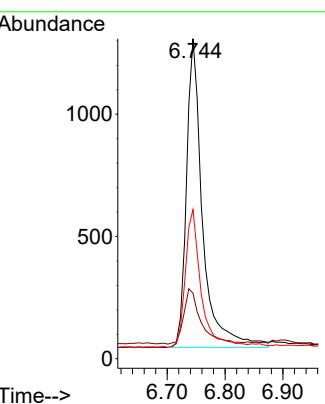


#6  
bis(2-Chloroethyl)ether  
Concen: 0.781 ng  
RT: 6.997 min Scan# 570  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29

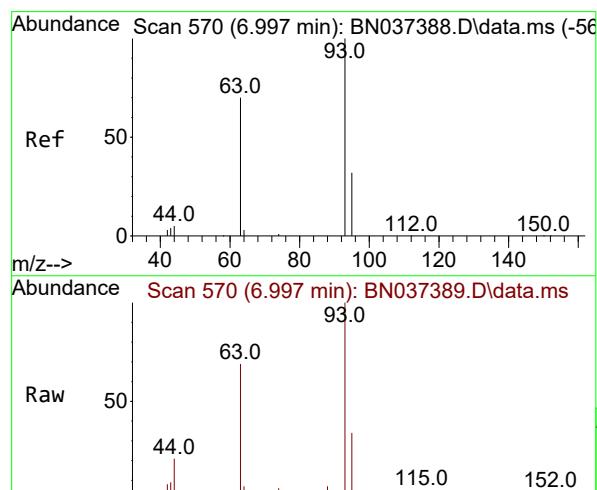


Tgt Ion: 93 Resp: 2313  
Ion Ratio Lower Upper  
93 100  
63 62.6 49.6 74.4  
95 31.1 23.9 35.9

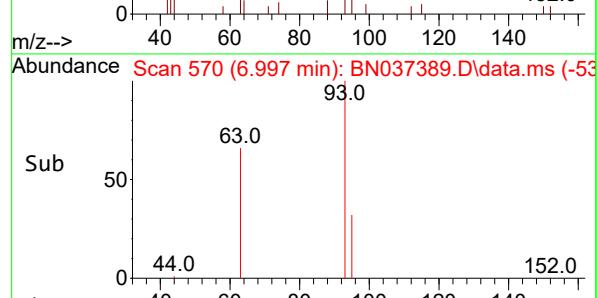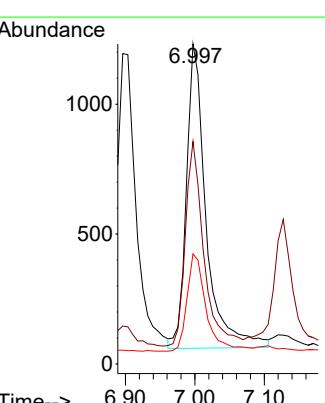



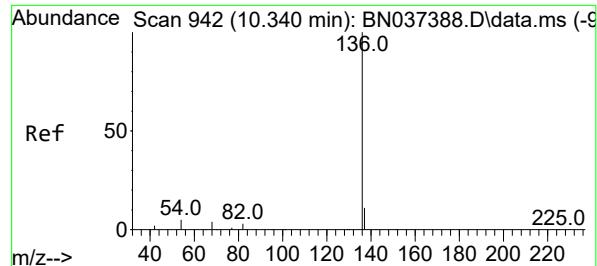


#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8





Tgt Ion:136 Resp: 3597  
 Ion Ratio Lower Upper  
 136 100  
 137 12.9 10.4 15.6  
 54 7.0 5.6 8.4  
 68 5.3 4.6 6.8


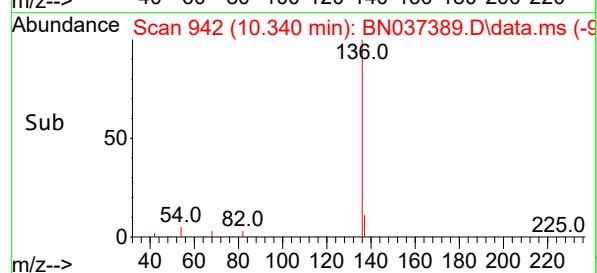



#8  
 Nitrobenzene-d5  
 Concen: 0.735 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29







Tgt Ion: 82 Resp: 2126  
 Ion Ratio Lower Upper  
 82 100  
 128 46.1 34.0 51.0  
 54 42.5 37.7 56.5

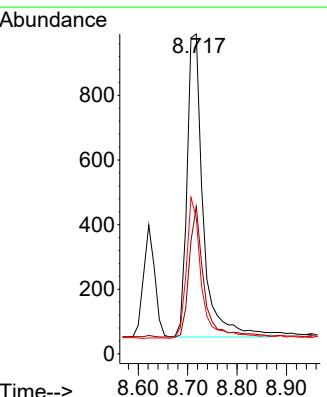

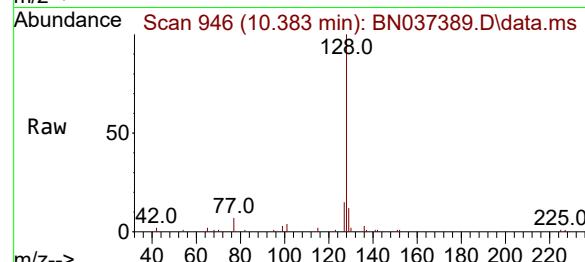


#9  
Naphthalene  
Concen: 0.755 ng  
RT: 10.383 min Scan# 9  
Instrument : BNA\_N  
Delta R.T. -0.011 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29  
ClientSampleId : SSTDICCO.8




Tgt Ion:128 Resp: 6991  
Ion Ratio Lower Upper  
128 100  
129 12.2 10.4 15.6  
127 14.8 12.2 18.4

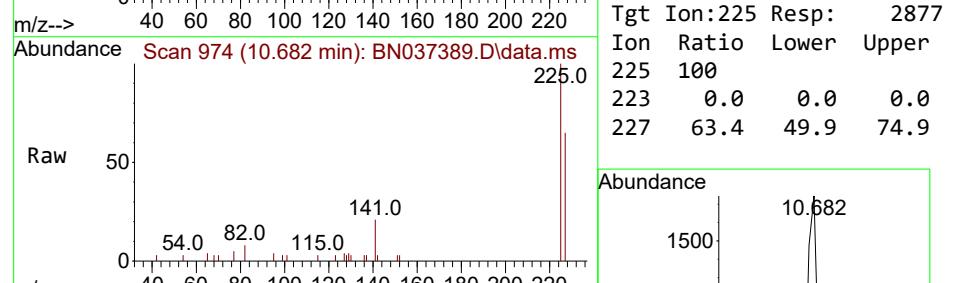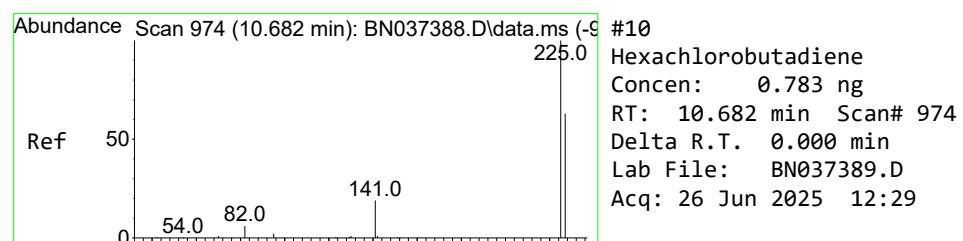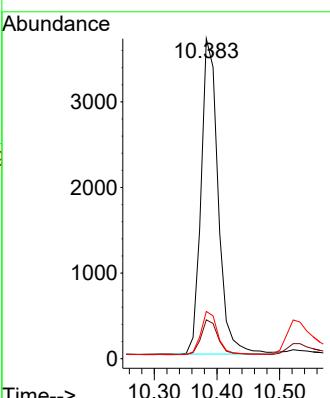

#10  
Hexachlorobutadiene  
Concen: 0.783 ng  
RT: 10.682 min Scan# 974  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29

Tgt Ion:225 Resp: 2877  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 63.4 49.9 74.9




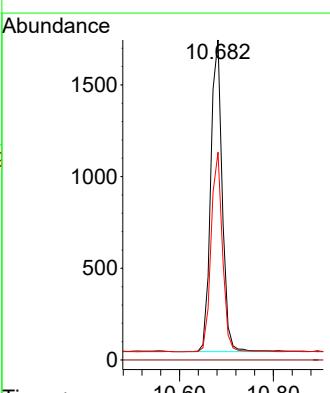


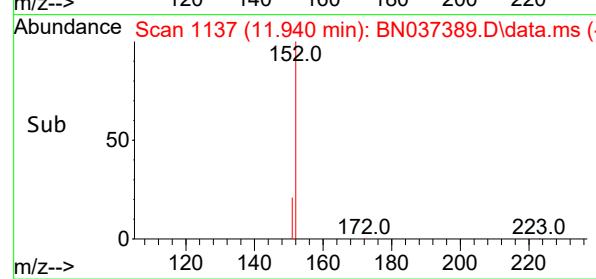

#11  
2-Methylnaphthalene-d10  
Concen: 0.734 ng  
RT: 11.940 min Scan# 1137  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8


Tgt Ion:152 Resp: 4083  
Ion Ratio Lower Upper  
152 100  
151 21.6 18.4 27.6

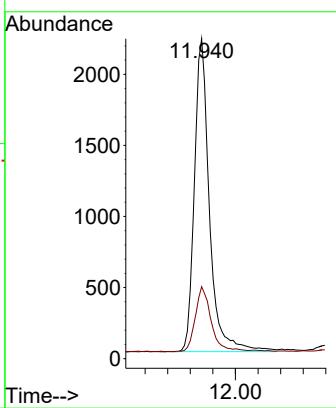

#12  
2-Methylnaphthalene  
Concen: 0.747 ng  
RT: 12.011 min Scan# 1151  
Delta R.T. -0.005 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29

Tgt Ion:142 Resp: 4762  
Ion Ratio Lower Upper  
142 100  
141 90.9 70.1 105.1  
115 44.3 35.8 53.6


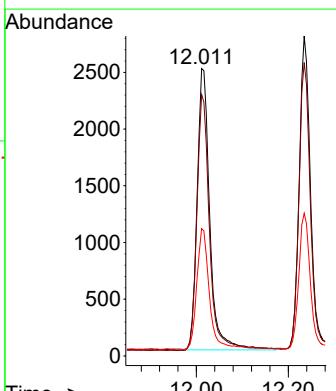


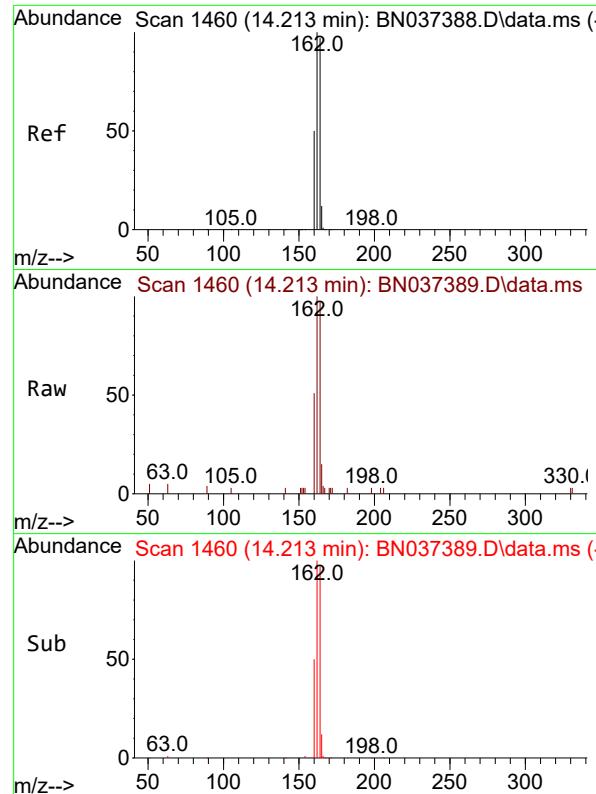

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1460  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8


Tgt Ion:164 Resp: 2328  
Ion Ratio Lower Upper  
164 100  
162 103.1 82.6 123.8  
160 53.1 42.2 63.2

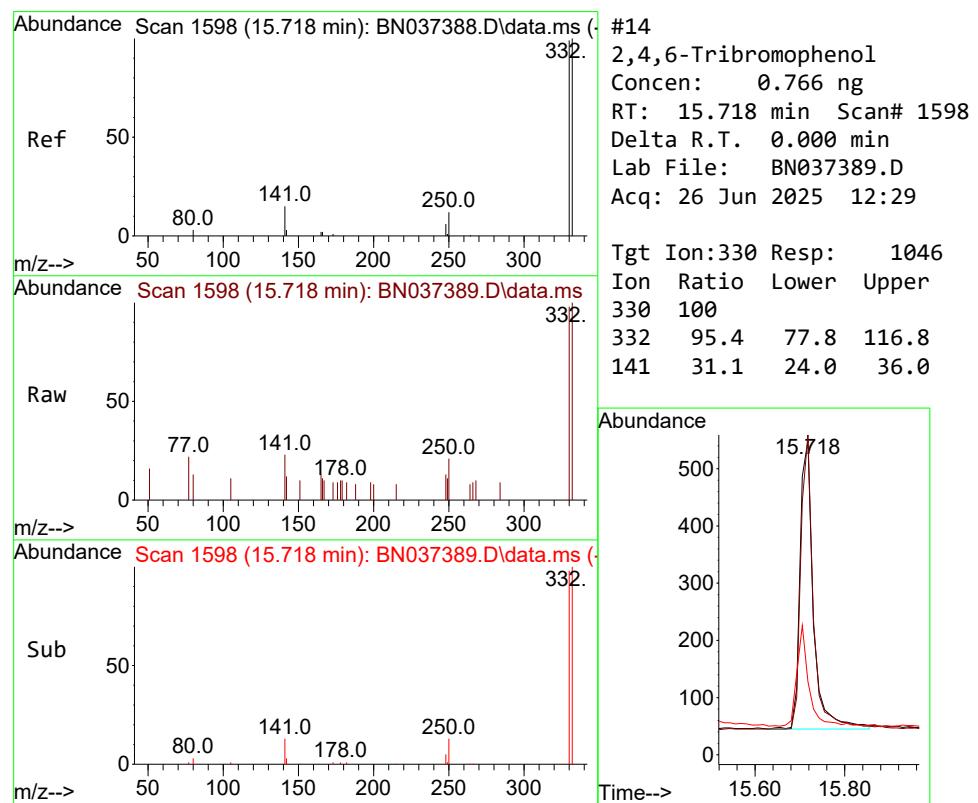

#14  
2,4,6-Tribromophenol  
Concen: 0.766 ng  
RT: 15.718 min Scan# 1598  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29



Tgt Ion:330 Resp: 1046  
Ion Ratio Lower Upper  
330 100  
332 95.4 77.8 116.8  
141 31.1 24.0 36.0



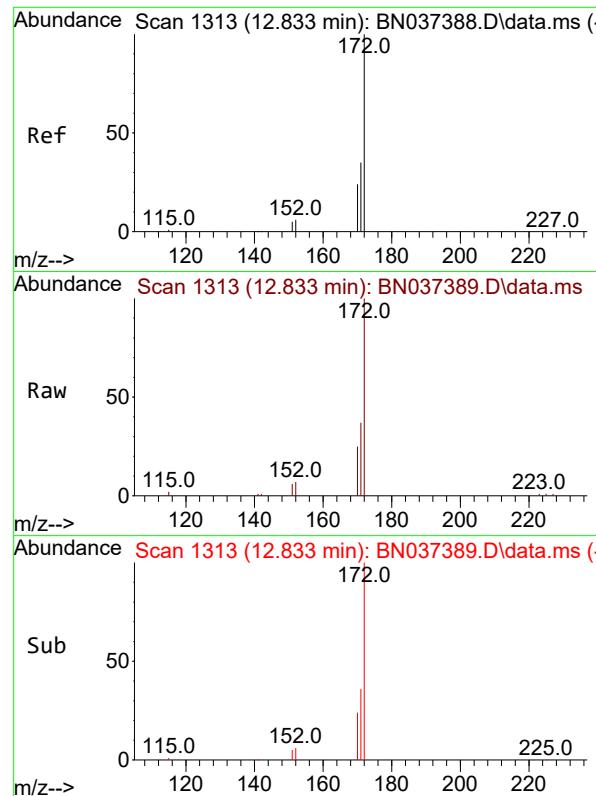


#15  
2-Fluorobiphenyl  
Concen: 0.765 ng  
RT: 12.833 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
ClientSampleId : SSTDICCO.8  
Acq: 26 Jun 2025 12:29




Tgt Ion:172 Resp: 7691  
Ion Ratio Lower Upper  
172 100  
171 36.7 28.8 43.2  
170 24.5 20.3 30.5

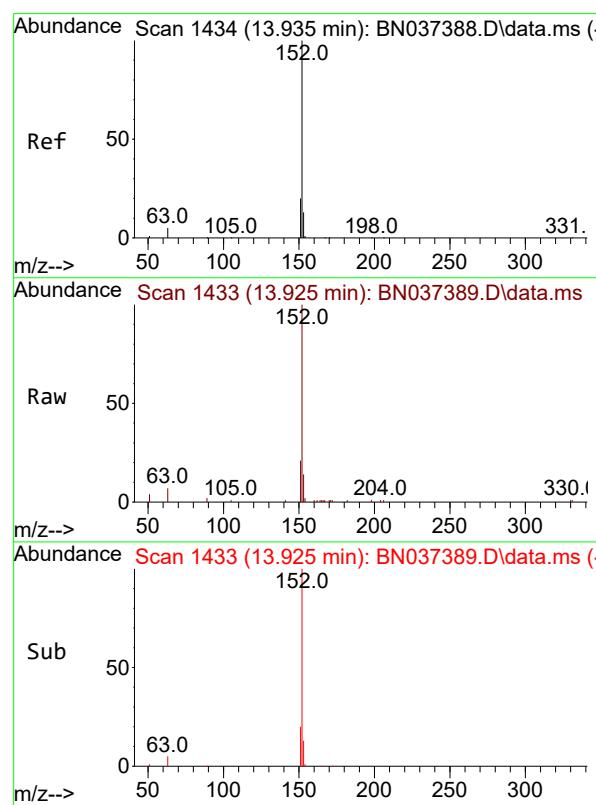

#16  
Acenaphthylene  
Concen: 0.742 ng  
RT: 13.925 min Scan# 1433  
Delta R.T. -0.011 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29

Tgt Ion:152 Resp: 7160  
Ion Ratio Lower Upper  
152 100  
151 19.9 15.8 23.6  
153 13.3 10.3 15.5





#17

Acenaphthene

Concen: 0.745 ng

RT: 14.277 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.8





Tgt Ion:154 Resp: 4696

Ion Ratio Lower Upper

154 100

153 117.8 94.6 141.8

152 62.8 50.2 75.2

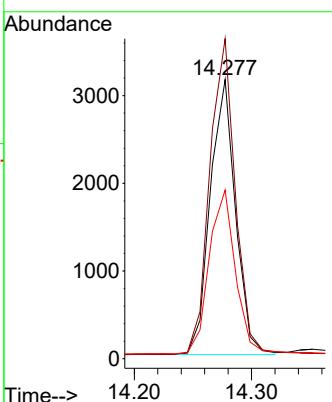

#18

Fluorene

Concen: 0.743 ng

RT: 15.272 min Scan# 1559

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29


Tgt Ion:166 Resp: 6613




Ion Ratio Lower Upper

166 100

165 100.0 79.4 119.2

167 13.7 10.6 15.8



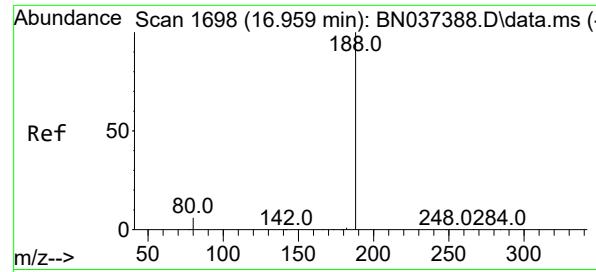

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.959 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29

Instrument :

BNA\_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:188 Resp: 4756

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 8.2 6.2 9.4



#20

4,6-Dinitro-2-methylphenol

Concen: 0.676 ng

RT: 15.368 min Scan# 1568

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29


Tgt Ion:198 Resp: 826


Ion Ratio Lower Upper

198 100

51 30.6 38.8 58.2#

105 28.3 29.8 44.6#



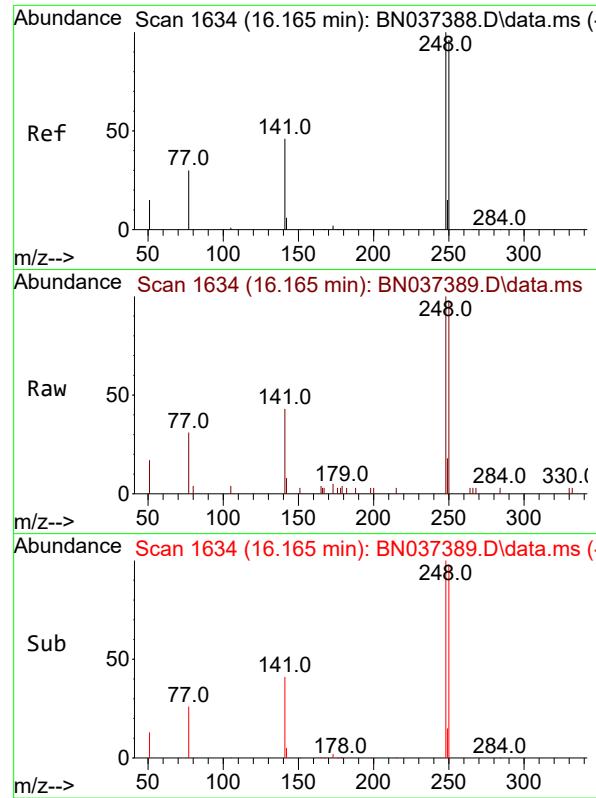

#21

4-Bromophenyl-phenylether

Concen: 0.762 ng

RT: 16.165 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29

Instrument :

BNA\_N

ClientSampleId :

SSTDICCO.8



Tgt Ion:248 Resp: 2555

Ion Ratio Lower Upper

248 100

250 97.7 77.0 115.4

141 43.2 38.7 58.1

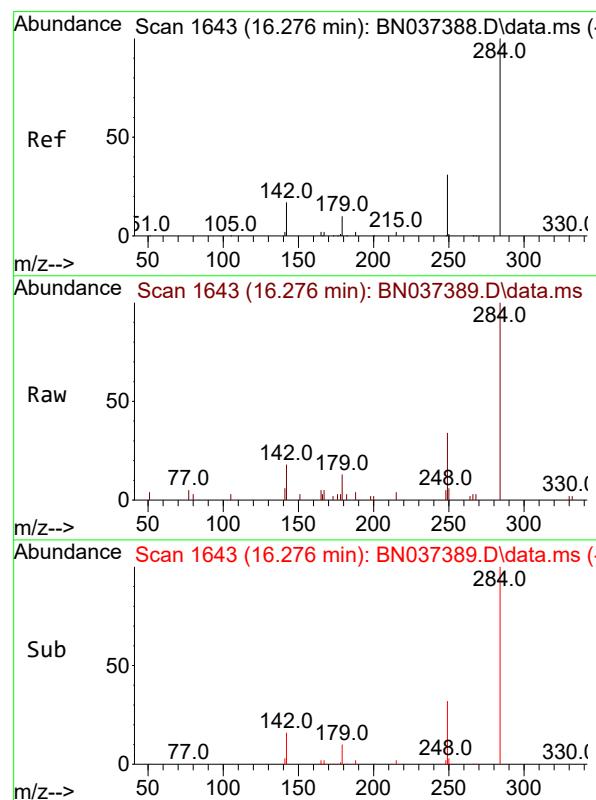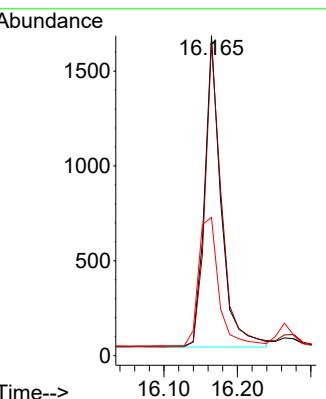

#22

Hexachlorobenzene

Concen: 0.767 ng

RT: 16.276 min Scan# 1643

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29


Tgt Ion:284 Resp: 2768


Ion Ratio Lower Upper

284 100

142 34.0 27.2 40.8

249 34.2 26.7 40.1


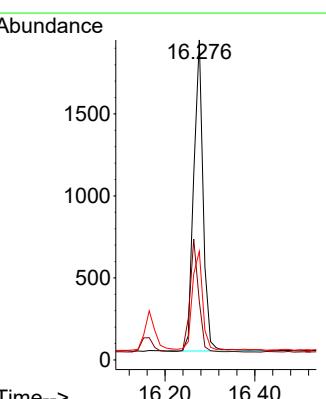


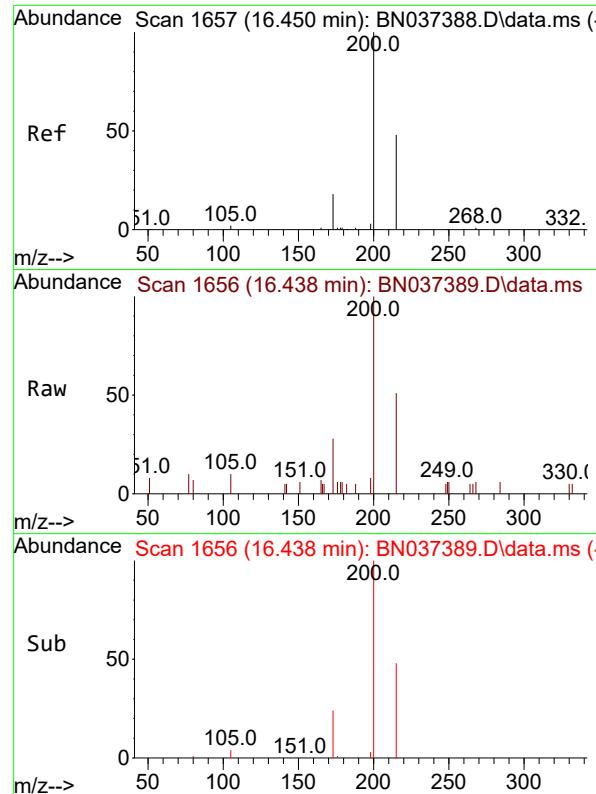

#23  
Atrazine  
Concen: 0.730 ng  
RT: 16.438 min Scan# 1  
Delta R.T. -0.012 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8




Tgt Ion:200 Resp: 1939  
Ion Ratio Lower Upper  
200 100  
173 27.7 19.0 28.6  
215 50.9 41.3 61.9

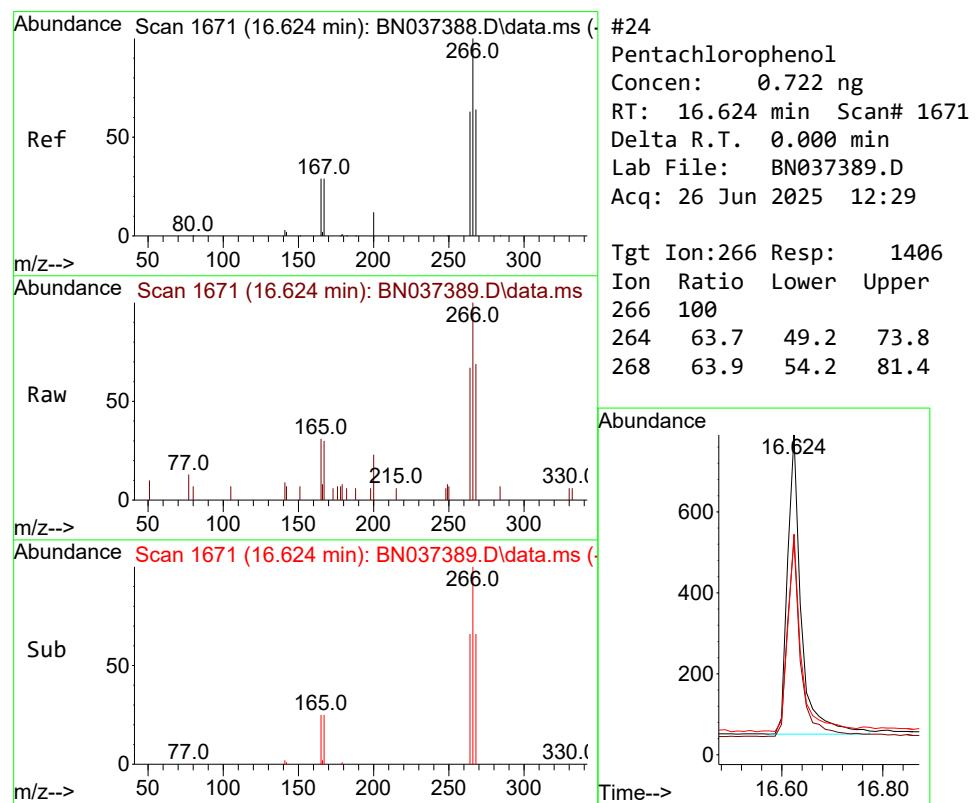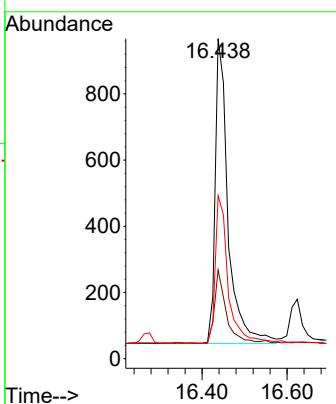

#24  
Pentachlorophenol  
Concen: 0.722 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29

Tgt Ion:266 Resp: 1406  
Ion Ratio Lower Upper  
266 100  
264 63.7 49.2 73.8  
268 63.9 54.2 81.4

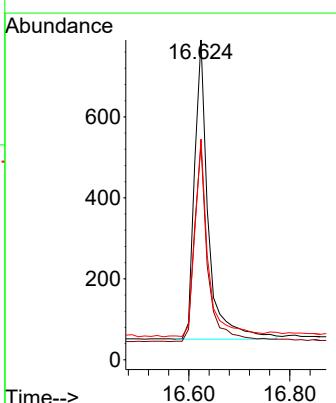

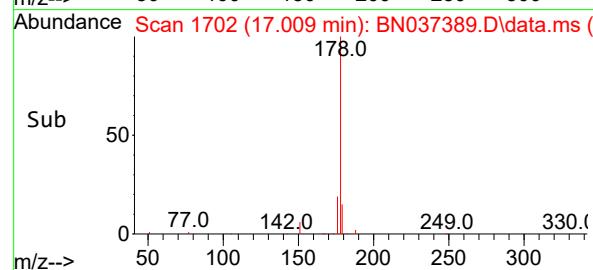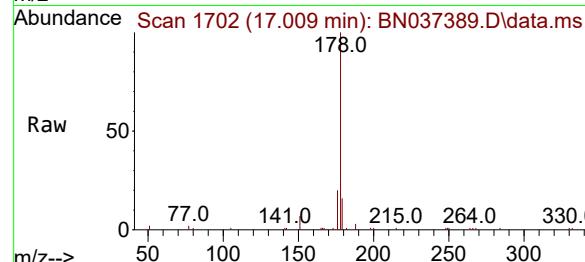

#25

Phenanthrene

Concen: 0.737 ng

RT: 17.009 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29

Instrument :

BNA\_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:178 Resp: 9870

Ion Ratio Lower Upper

178 100

176 19.6 15.6 23.4

179 15.3 12.8 19.2

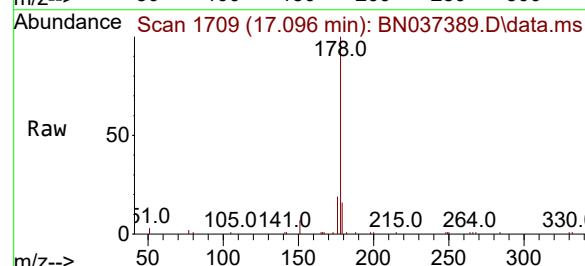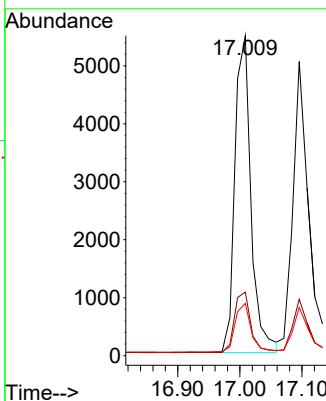

#26

Anthracene

Concen: 0.741 ng

RT: 17.096 min Scan# 1709

Delta R.T. 0.000 min

Lab File: BN037389.D

Acq: 26 Jun 2025 12:29


Tgt Ion:178 Resp: 9124


Ion Ratio Lower Upper

178 100

176 18.0 14.9 22.3

179 15.4 12.4 18.6


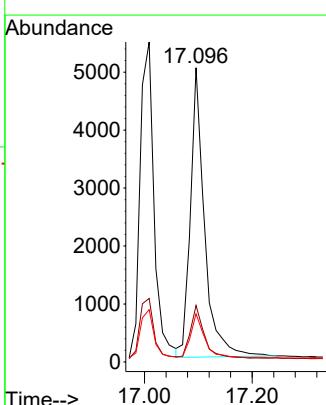


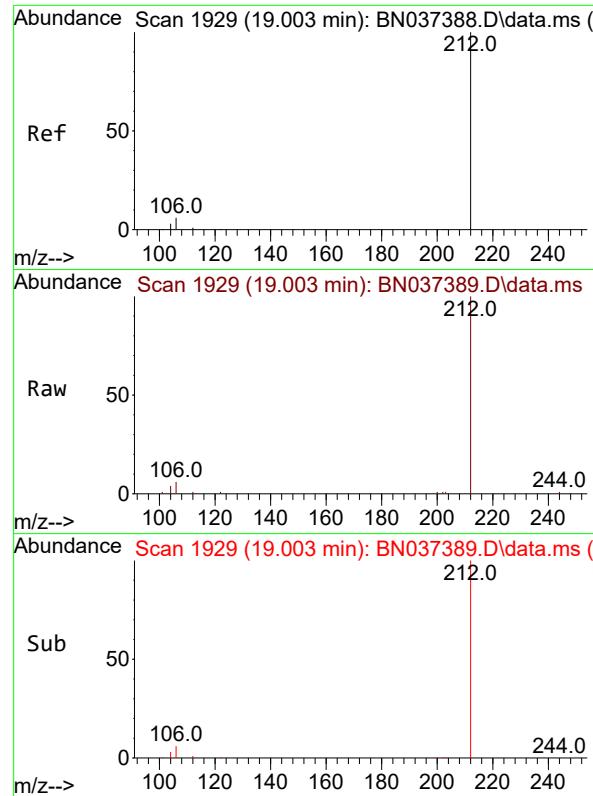

#27  
 Fluoranthene-d10  
 Concen: 0.717 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:212 Resp: 9775  
 Ion Ratio Lower Upper  
 212 100  
 106 5.7 4.5 6.7  
 104 3.3 2.7 4.1

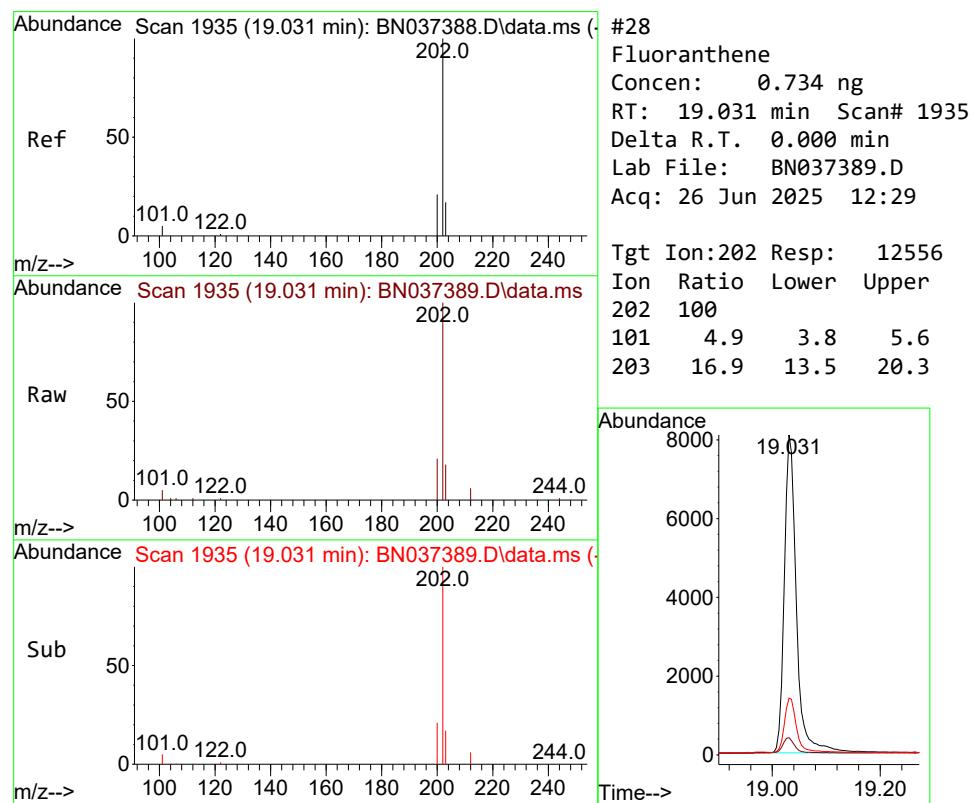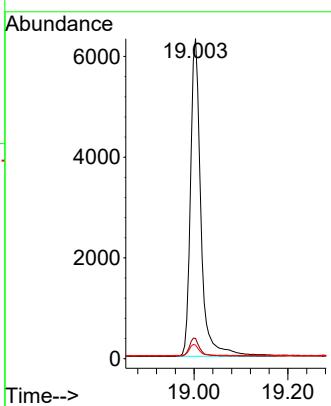

#28  
 Fluoranthene  
 Concen: 0.734 ng  
 RT: 19.031 min Scan# 1935  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29

Tgt Ion:202 Resp: 12556  
 Ion Ratio Lower Upper  
 202 100  
 101 4.9 3.8 5.6  
 203 16.9 13.5 20.3





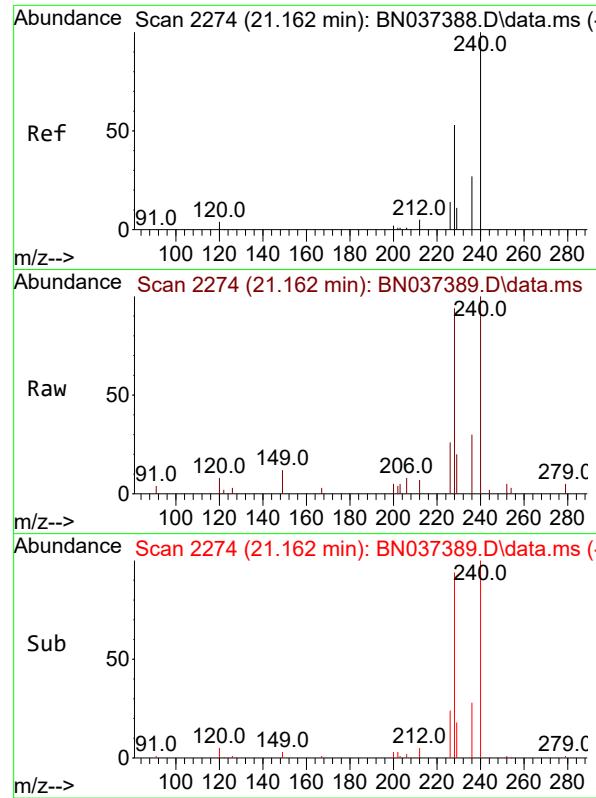

#29  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.162 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:240 Resp: 4408  
 Ion Ratio Lower Upper  
 240 100  
 120 7.9 5.3 7.9  
 236 29.6 22.7 34.1

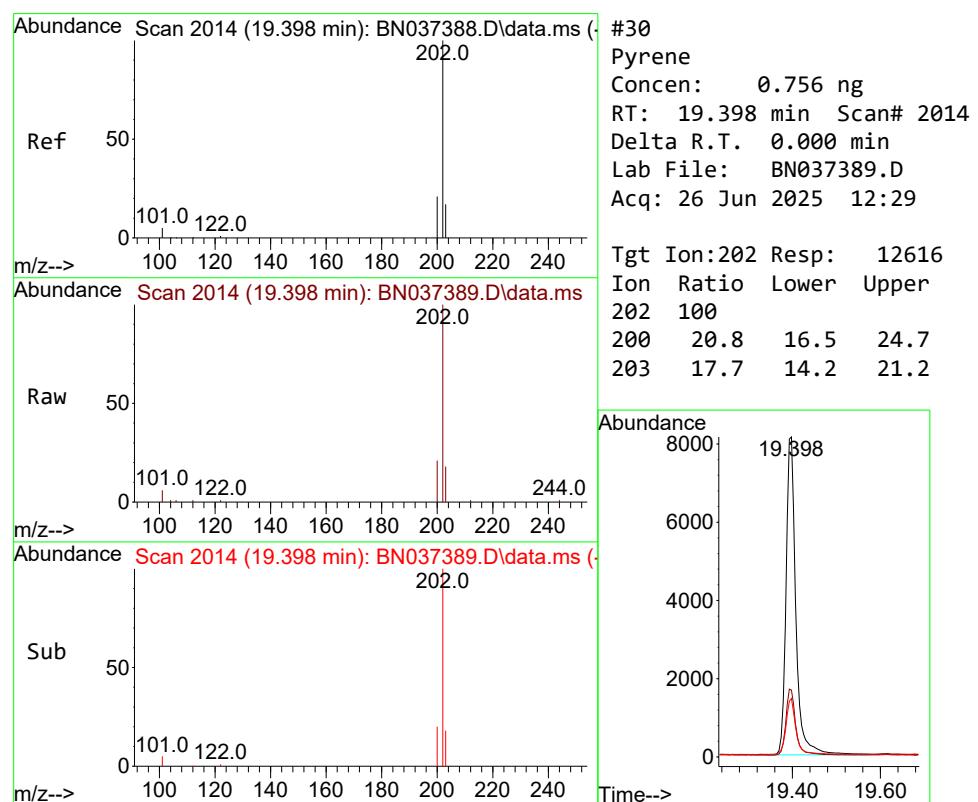

#30  
 Pyrene  
 Concen: 0.756 ng  
 RT: 19.398 min Scan# 2014  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29

Tgt Ion:202 Resp: 12616  
 Ion Ratio Lower Upper  
 202 100  
 200 20.8 16.5 24.7  
 203 17.7 14.2 21.2





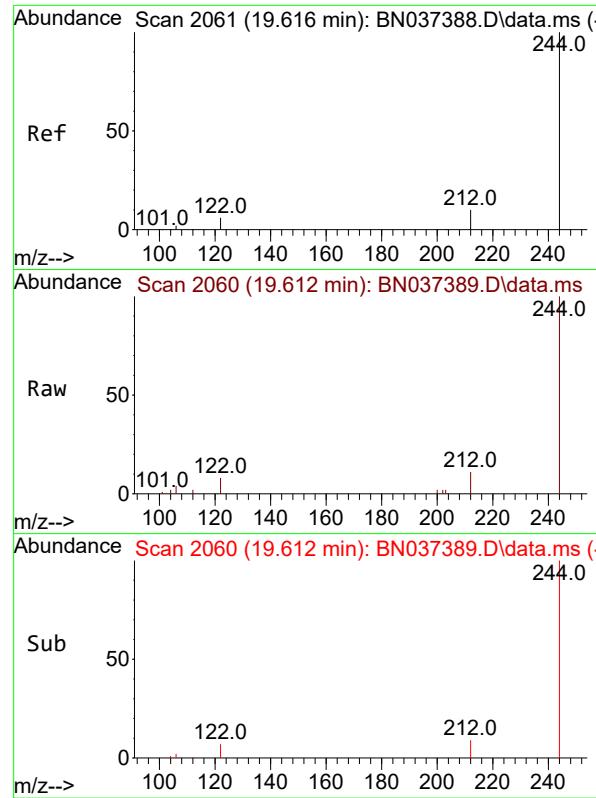

#31  
**Terphenyl-d14**  
Concen: 0.747 ng  
RT: 19.612 min Scan# 2  
Delta R.T. -0.005 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8




Tgt Ion:244 Resp: 7017  
Ion Ratio Lower Upper  
244 100  
212 10.7 9.1 13.7  
122 8.1 6.3 9.5

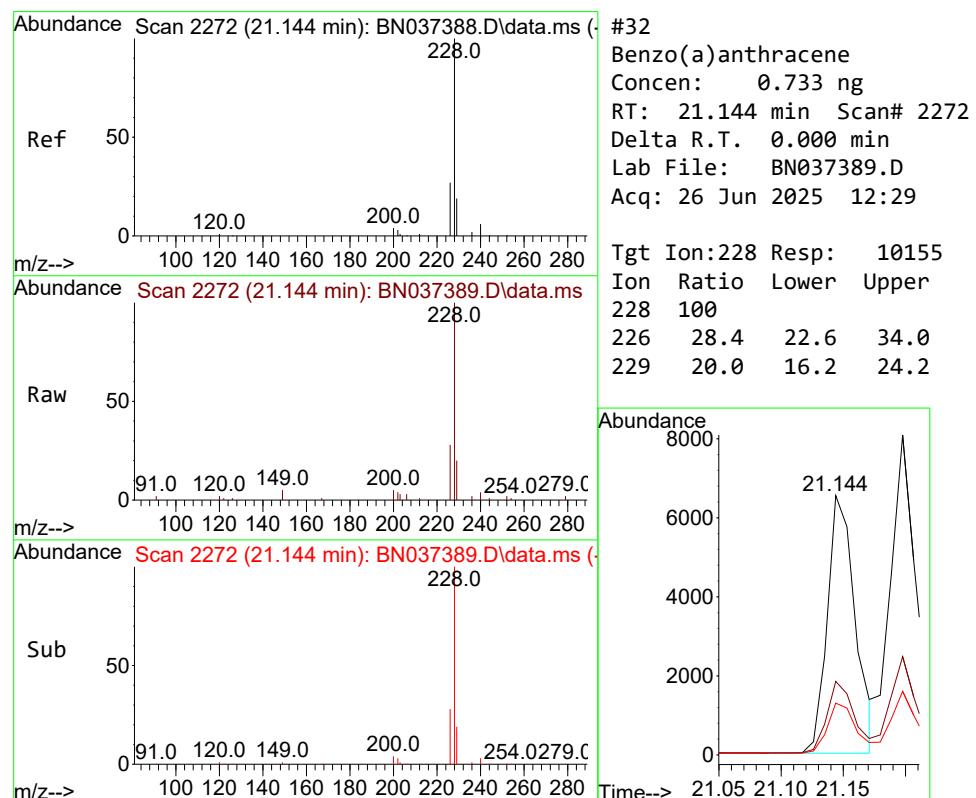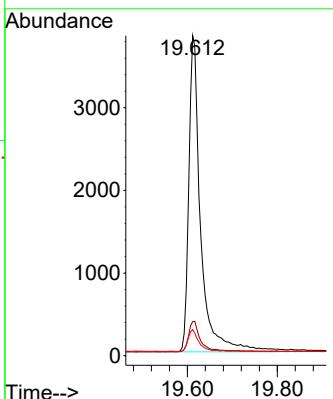

#32  
**Benzo(a)anthracene**  
Concen: 0.733 ng  
RT: 21.144 min Scan# 2272  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29

Tgt Ion:228 Resp: 10155  
Ion Ratio Lower Upper  
228 100  
226 28.4 22.6 34.0  
229 20.0 16.2 24.2




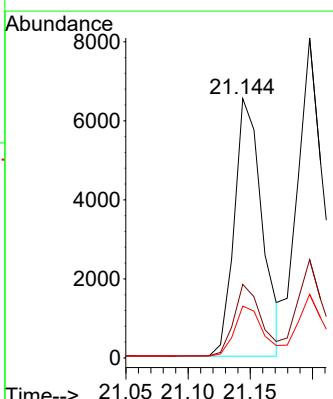


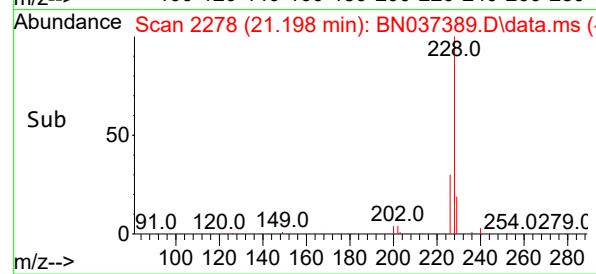

#33  
 Chrysene  
 Concen: 0.767 ng  
 RT: 21.198 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:228 Resp: 13144  
 Ion Ratio Lower Upper  
 228 100  
 226 30.7 24.5 36.7  
 229 19.9 16.1 24.1

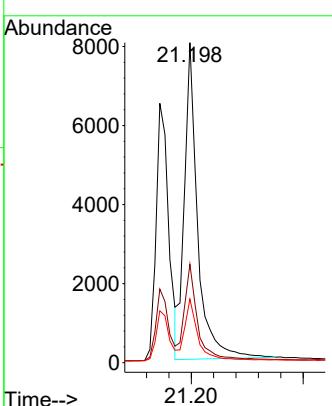

#34  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.749 ng  
 RT: 21.090 min Scan# 2266  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29

Tgt Ion:149 Resp: 4107  
 Ion Ratio Lower Upper  
 149 100  
 167 31.9 24.8 37.2  
 279 6.4 5.0 7.6





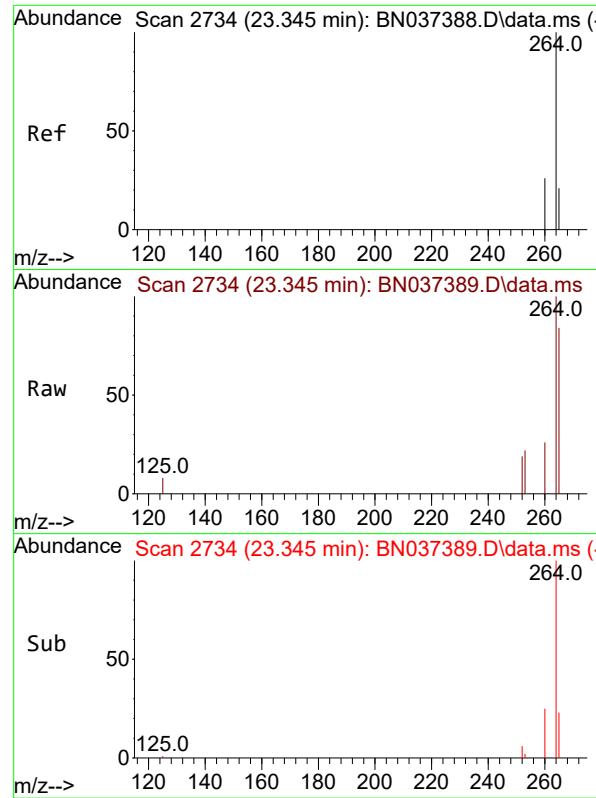

#35  
Perylene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 23.345 min Scan# 2  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.8


Tgt Ion:264 Resp: 4628  
Ion Ratio Lower Upper  
264 100  
260 26.3 21.4 32.0  
265 84.2 56.2 84.4

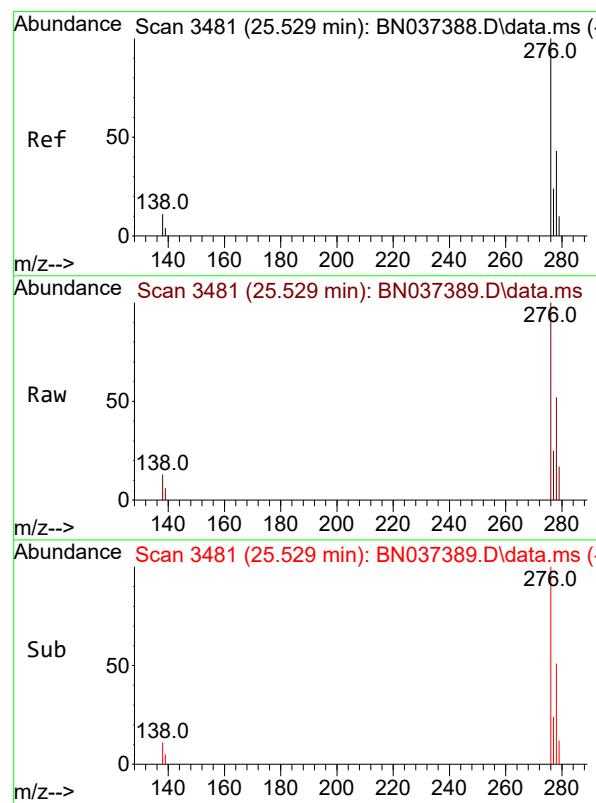

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.768 ng  
RT: 25.529 min Scan# 3481  
Delta R.T. 0.000 min  
Lab File: BN037389.D  
Acq: 26 Jun 2025 12:29

Tgt Ion:276 Resp: 14993  
Ion Ratio Lower Upper  
276 100  
138 11.6 8.5 12.7  
277 23.8 19.7 29.5





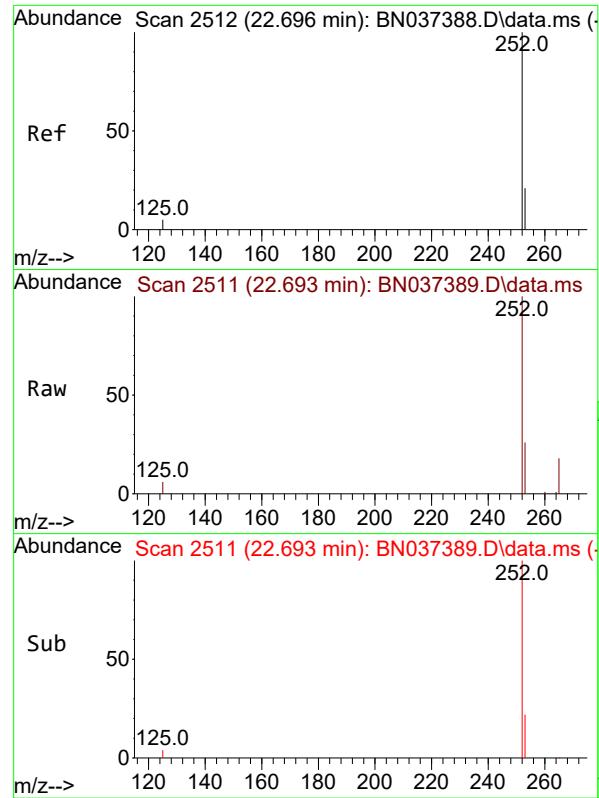

#37  
 Benzo(b)fluoranthene  
 Concen: 0.749 ng  
 RT: 22.693 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:252 Resp: 12221  
 Ion Ratio Lower Upper  
 252 100  
 253 26.4 22.8 34.2  
 125 6.4 6.2 9.4

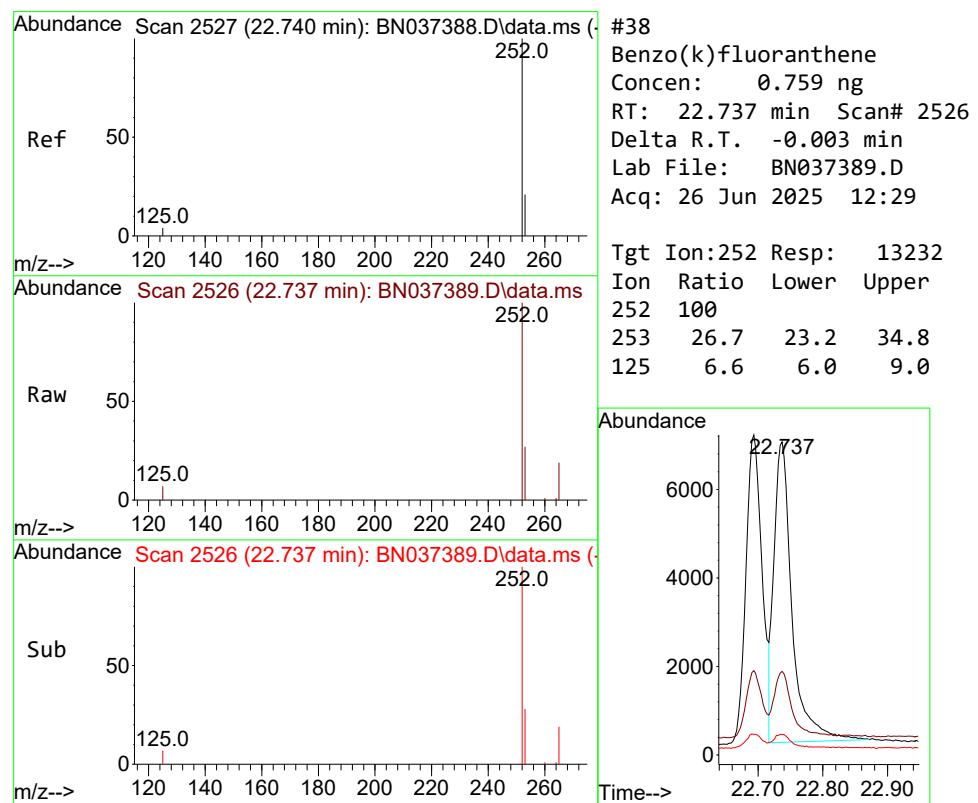

#38  
 Benzo(k)fluoranthene  
 Concen: 0.759 ng  
 RT: 22.737 min Scan# 2526  
 Delta R.T. -0.003 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29

Tgt Ion:252 Resp: 13232  
 Ion Ratio Lower Upper  
 252 100  
 253 26.7 23.2 34.8  
 125 6.6 6.0 9.0





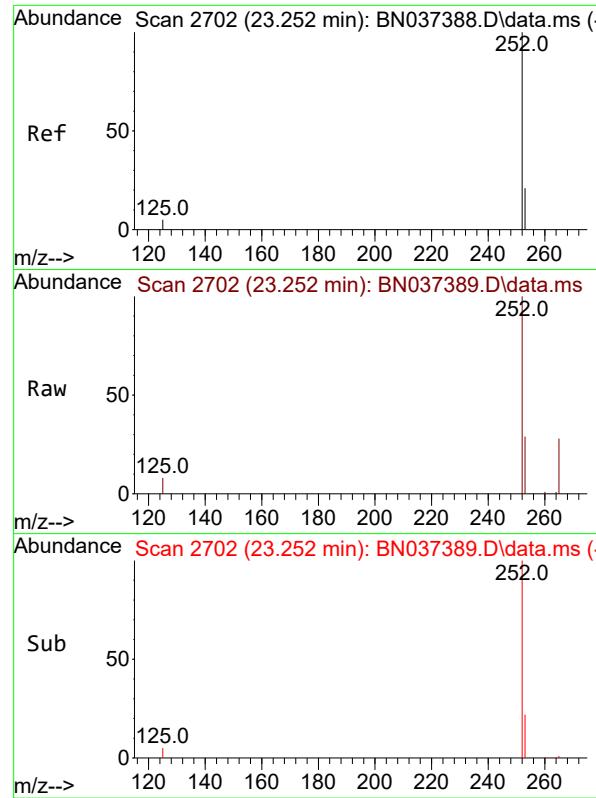

#39  
 Benzo(a)pyrene  
 Concen: 0.748 ng  
 RT: 23.252 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.8


Tgt Ion:252 Resp: 10863  
 Ion Ratio Lower Upper  
 252 100  
 253 29.0 25.6 38.4  
 125 8.0 7.5 11.3

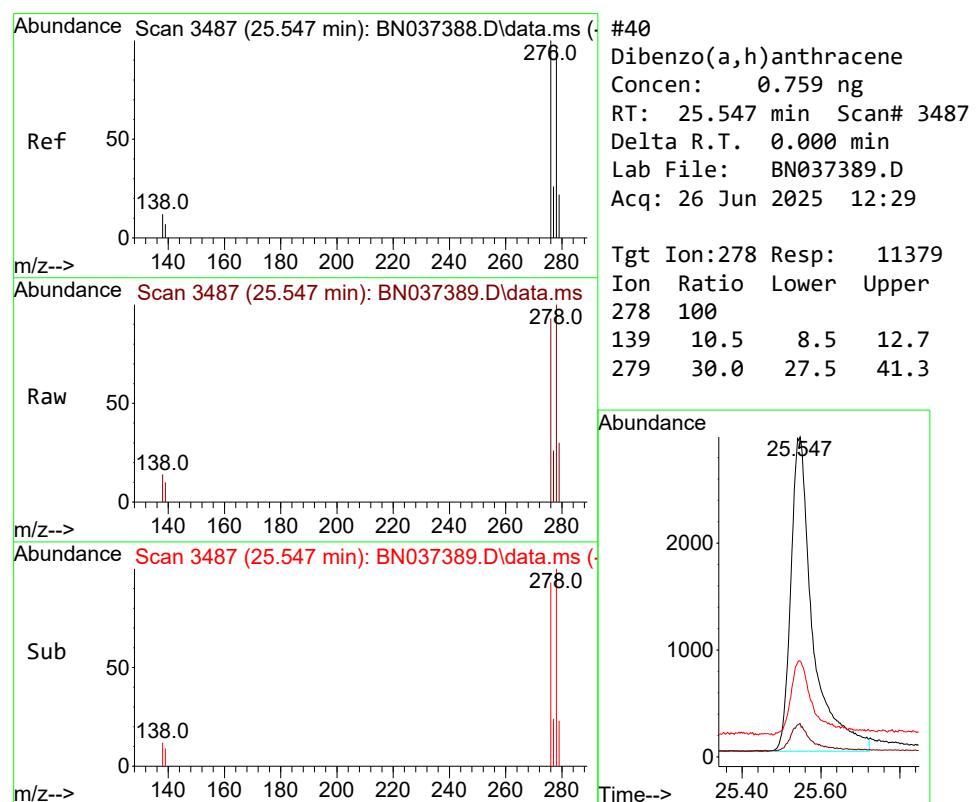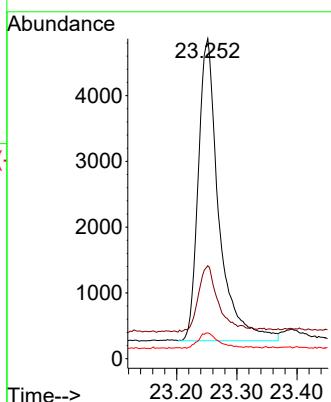

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.759 ng  
 RT: 25.547 min Scan# 3487  
 Delta R.T. 0.000 min  
 Lab File: BN037389.D  
 Acq: 26 Jun 2025 12:29

Tgt Ion:278 Resp: 11379  
 Ion Ratio Lower Upper  
 278 100  
 139 10.5 8.5 12.7  
 279 30.0 27.5 41.3



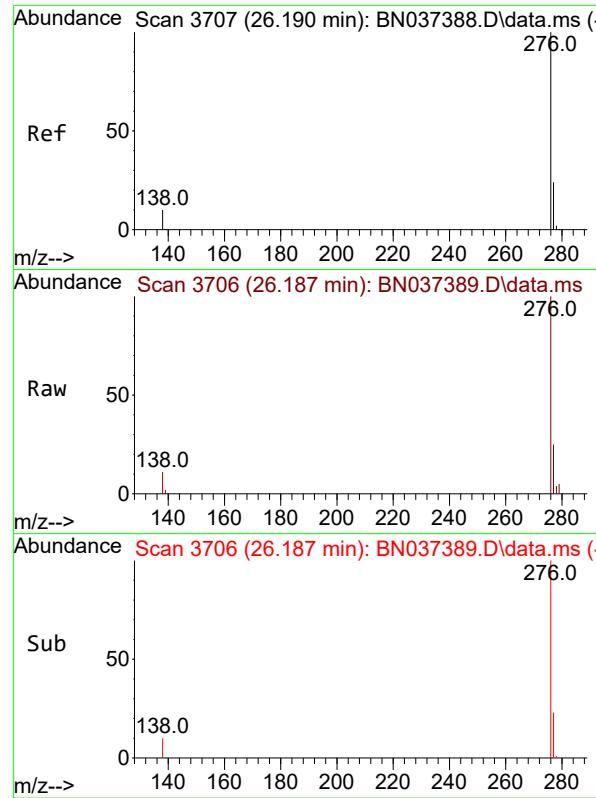

#41

Benzo(g,h,i)perylene

Concen: 0.756 ng

RT: 26.187 min Scan# 3

Instrument :

BNA\_N

Delta R.T. -0.003 min

Lab File: BN037389.D

ClientSampleId :

SSTDICC0.8

Acq: 26 Jun 2025 12:29


Tgt Ion:276 Resp: 13535

Ion Ratio Lower Upper

276 100

277 24.8 21.0 31.4

138 11.4 9.6 14.4



Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037390.D  
 Acq On : 26 Jun 2025 13:05  
 Operator : RC/JU  
 Sample : SSTDICC1.6  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC1.6

Quant Time: Jun 26 14:44:50 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.561	152	1757	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	3755	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	2497	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	5134	0.400	ng	0.00
29) Chrysene-d12	21.162	240	4846	0.400	ng	0.00
35) Perylene-d12	23.345	264	4921	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	5301	1.566	ng	0.00
5) Phenol-d6	6.745	99	5895	1.679	ng	0.00
8) Nitrobenzene-d5	8.707	82	5183	1.716	ng	-0.01
11) 2-Methylnaphthalene-d10	11.935	152	9434	1.624	ng	0.00
14) 2,4,6-Tribromophenol	15.705	330	2504	1.710	ng	-0.01
15) 2-Fluorobiphenyl	12.833	172	17962	1.666	ng	0.00
27) Fluoranthene-d10	18.998	212	23030	1.565	ng	0.00
31) Terphenyl-d14	19.612	244	17013	1.647	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.097	88	2649	1.682	ng	96
3) n-Nitrosodimethylamine	3.408	42	2708	1.646	ng	# 97
6) bis(2-Chloroethyl)ether	6.997	93	5373	1.721	ng	97
9) Naphthalene	10.383	128	15743	1.629	ng	97
10) Hexachlorobutadiene	10.682	225	6333	1.651	ng	# 98
12) 2-Methylnaphthalene	12.011	142	11211	1.685	ng	97
16) Acenaphthylene	13.925	152	17120	1.653	ng	100
17) Acenaphthene	14.277	154	11218	1.659	ng	98
18) Fluorene	15.272	166	16008	1.676	ng	100
20) 4,6-Dinitro-2-methylph...	15.357	198	2324	1.762	ng	# 63
21) 4-Bromophenyl-phenylether	16.165	248	6221	1.718	ng	# 92
22) Hexachlorobenzene	16.276	284	6380	1.638	ng	98
23) Atrazine	16.438	200	4771	1.663	ng	98
24) Pentachlorophenol	16.624	266	3391	1.612	ng	96
25) Phenanthrene	16.996	178	24063	1.663	ng	99
26) Anthracene	17.096	178	22103	1.662	ng	100
28) Fluoranthene	19.031	202	30535	1.653	ng	99
30) Pyrene	19.393	202	30249	1.650	ng	100
32) Benzo(a)anthracene	21.144	228	25546	1.678	ng	99
33) Chrysene	21.198	228	30118	1.598	ng	99
34) Bis(2-ethylhexyl)phtha...	21.090	149	9332	1.548	ng	99
36) Indeno(1,2,3-cd)pyrene	25.529	276	35151	1.694	ng	98
37) Benzo(b)fluoranthene	22.690	252	28814	1.661	ng	# 91
38) Benzo(k)fluoranthene	22.737	252	30557	1.648	ng	# 91
39) Benzo(a)pyrene	23.249	252	25315	1.640	ng	# 88
40) Dibenzo(a,h)anthracene	25.538	278	27440	1.722	ng	# 87
41) Benzo(g,h,i)perylene	26.187	276	31821	1.671	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037390.D  
 Acq On : 26 Jun 2025 13:05  
 Operator : RC/JU  
 Sample : SSTDICC1.6  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC1.6

Quant Time: Jun 26 14:44:50 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration


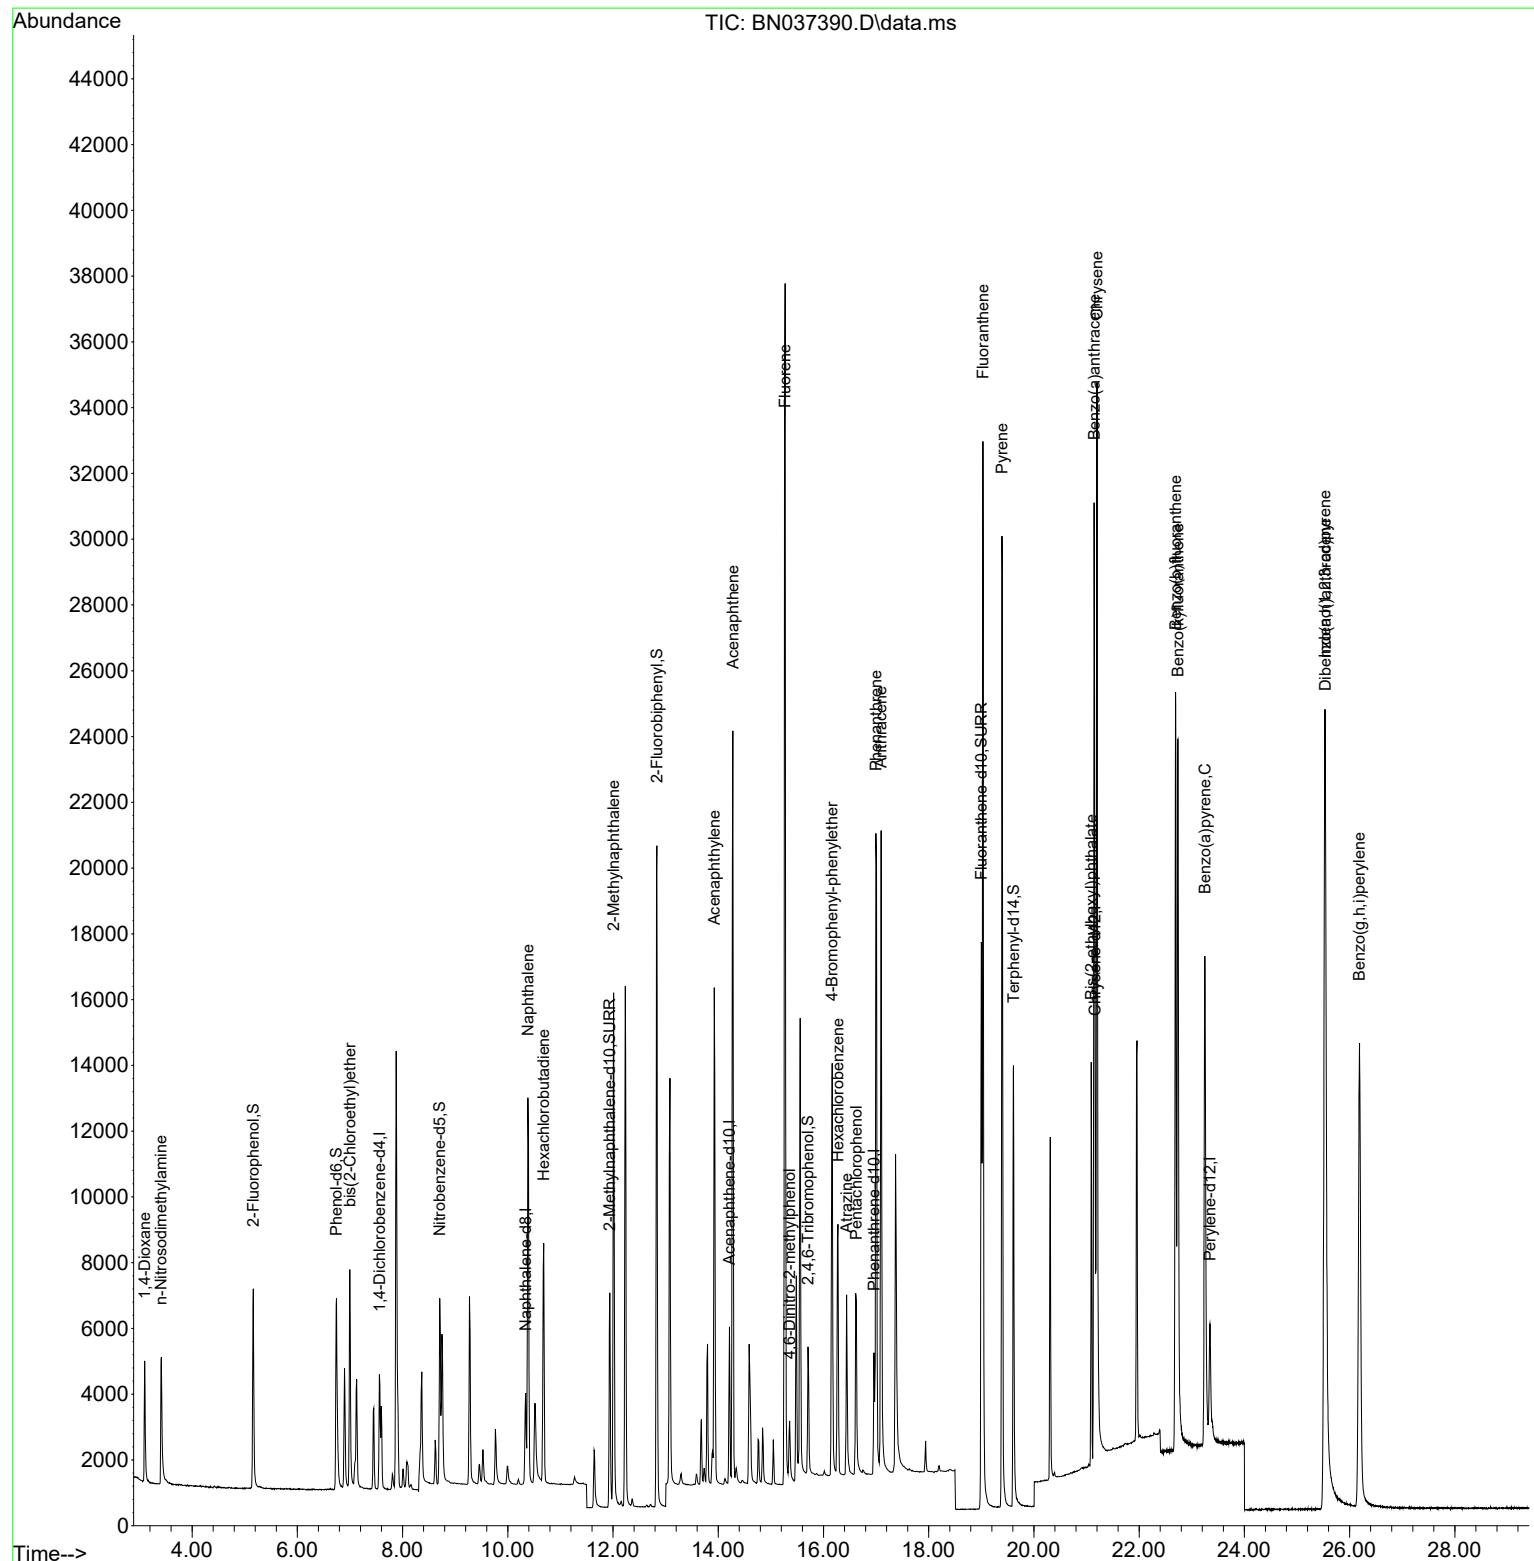


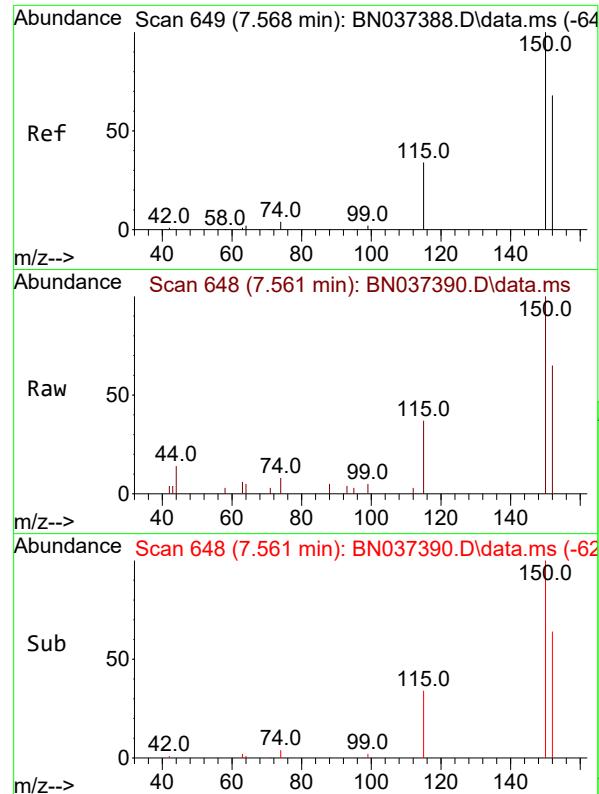

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.561 min Scan# 6  
Delta R.T. -0.007 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6


Tgt Ion:152 Resp: 1757  
Ion Ratio Lower Upper  
152 100  
150 153.6 116.2 174.2  
115 56.4 42.9 64.3

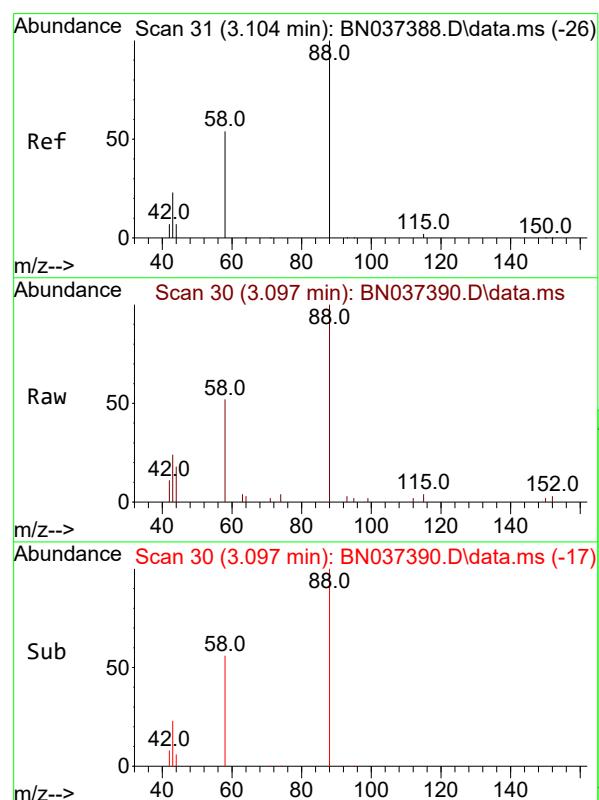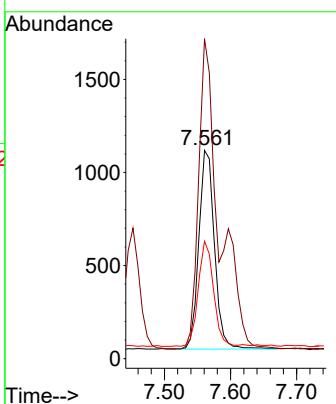

#2  
1,4-Dioxane  
Concen: 1.682 ng  
RT: 3.097 min Scan# 30  
Delta R.T. -0.007 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05



Tgt Ion: 88 Resp: 2649  
Ion Ratio Lower Upper  
88 100  
43 23.8 21.6 32.4  
58 55.3 45.9 68.9

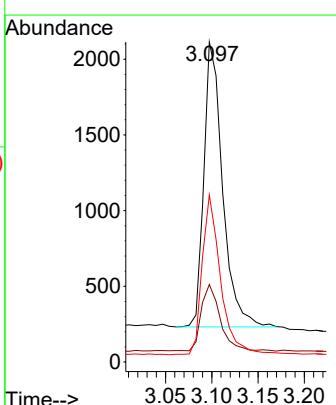

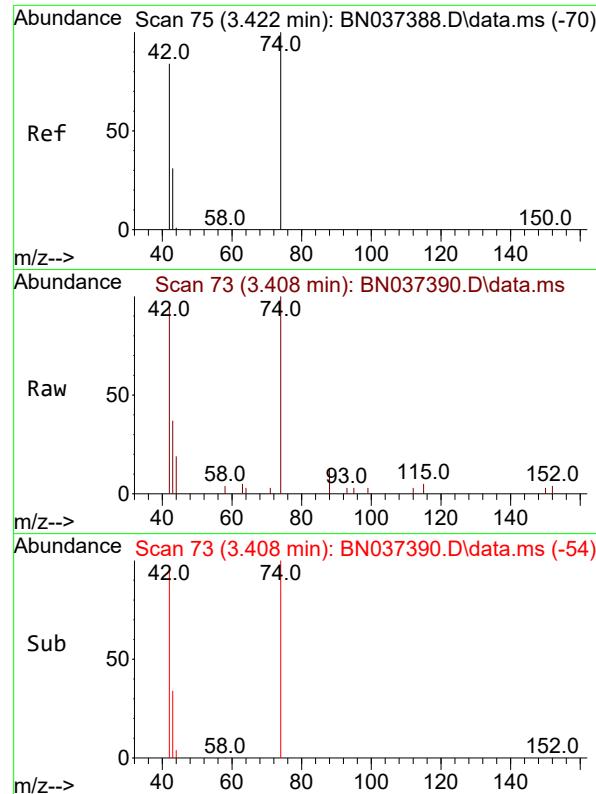


#3  
n-Nitrosodimethylamine  
Concen: 1.646 ng  
RT: 3.408 min Scan# 7  
Instrument : BNA\_N  
Delta R.T. -0.014 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05  
ClientSampleId : SSTDICC1.6


Tgt Ion: 42 Resp: 2708  
Ion Ratio Lower Upper  
42 100  
74 125.6 97.8 146.8  
44 7.3 8.7 13.1#

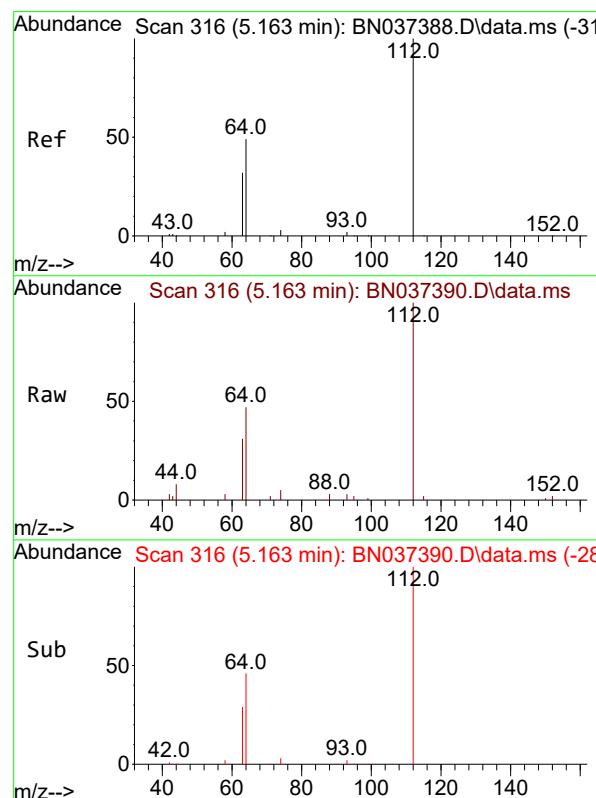

#4  
2-Fluorophenol  
Concen: 1.566 ng  
RT: 5.163 min Scan# 316  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05


Tgt Ion:112 Resp: 5301  
Ion Ratio Lower Upper  
112 100  
64 50.2 40.3 60.5  
63 32.2 26.1 39.1







#5  
Phenol-d6  
Concen: 1.679 ng  
RT: 6.745 min Scan# 5  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6






Tgt Ion: 99 Resp: 5895  
Ion Ratio Lower Upper  
99 100  
42 18.4 15.6 23.4  
71 44.7 35.8 53.8




#6  
bis(2-Chloroethyl)ether  
Concen: 1.721 ng  
RT: 6.997 min Scan# 570  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

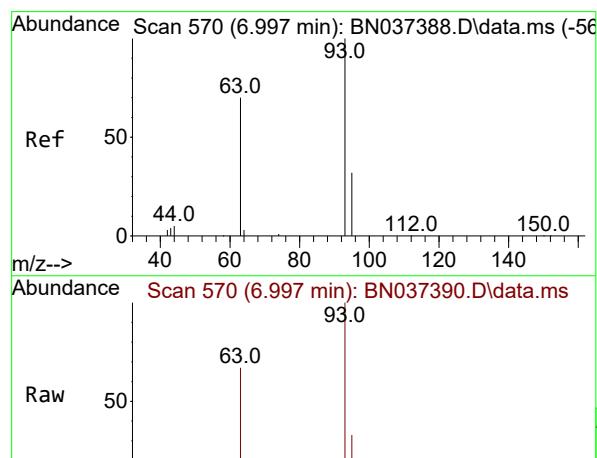

Tgt Ion: 93 Resp: 5373  
Ion Ratio Lower Upper  
93 100  
63 64.6 49.6 74.4  
95 31.7 23.9 35.9

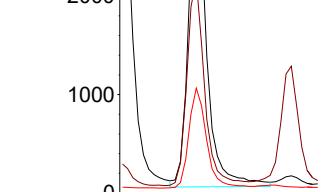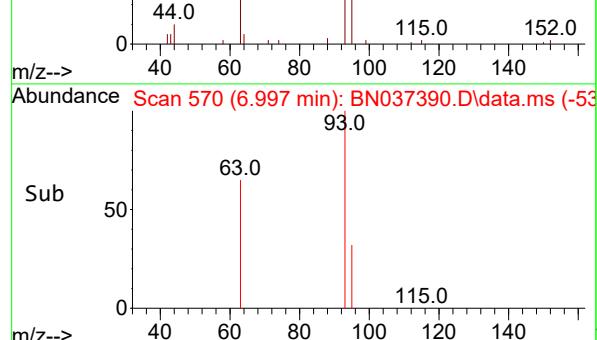

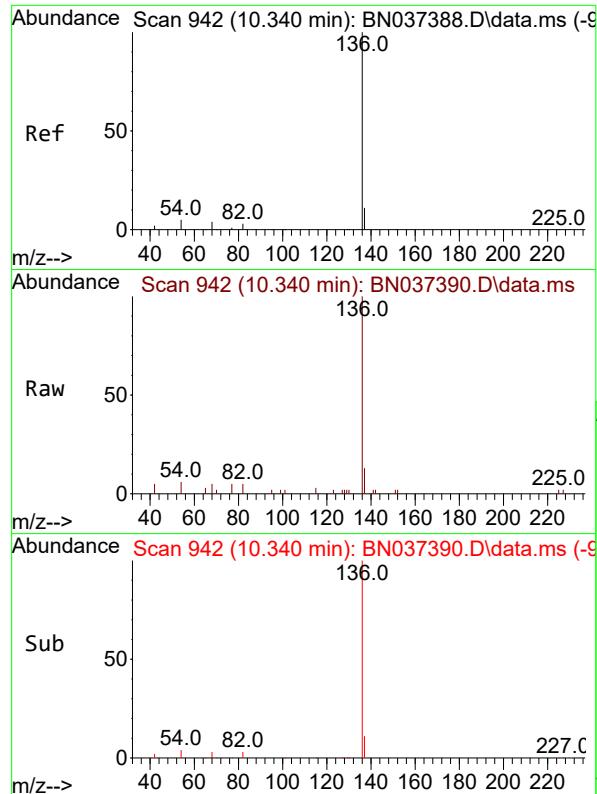



#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. 0.000 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05

Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6

Tgt Ion:136 Resp: 3755

	Ion Ratio	Lower	Upper
136	100		
137	12.5	10.4	15.6
54	6.3	5.6	8.4
68	5.2	4.6	6.8


Abundance


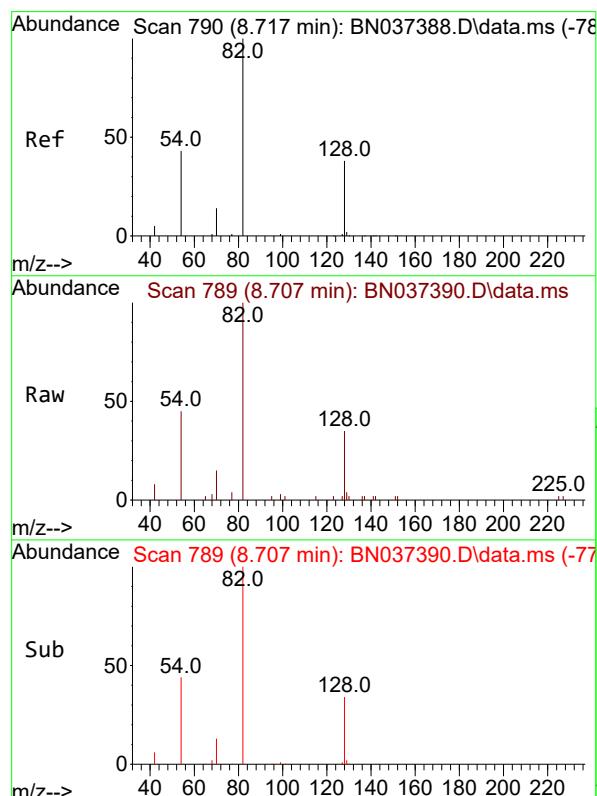
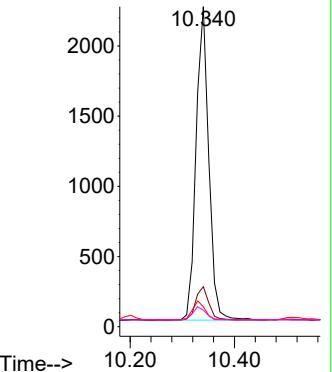


#8  
 Nitrobenzene-d5  
 Concen: 1.716 ng  
 RT: 8.707 min Scan# 789  
 Delta R.T. -0.011 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05

Tgt Ion: 82 Resp: 5183




	Ion Ratio	Lower	Upper
82	100		
128	35.3	34.0	51.0
54	45.2	37.7	56.5

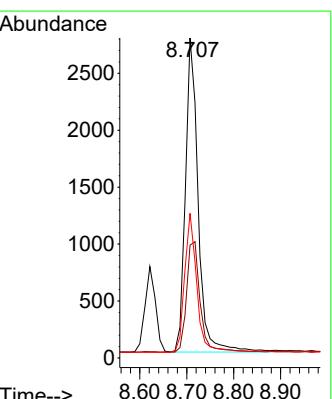

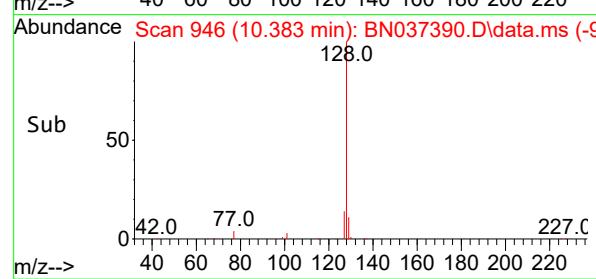



#9  
Naphthalene  
Concen: 1.629 ng  
RT: 10.383 min Scan# 9  
Instrument : BNA\_N  
Delta R.T. -0.011 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05  
ClientSampleId : SSTDICC1.6


Tgt Ion:128 Resp: 15743  
Ion Ratio Lower Upper  
128 100  
129 11.4 10.4 15.6  
127 14.4 12.2 18.4



#10  
Hexachlorobutadiene  
Concen: 1.651 ng  
RT: 10.682 min Scan# 974  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05



Tgt Ion:225 Resp: 6333  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 63.9 49.9 74.9



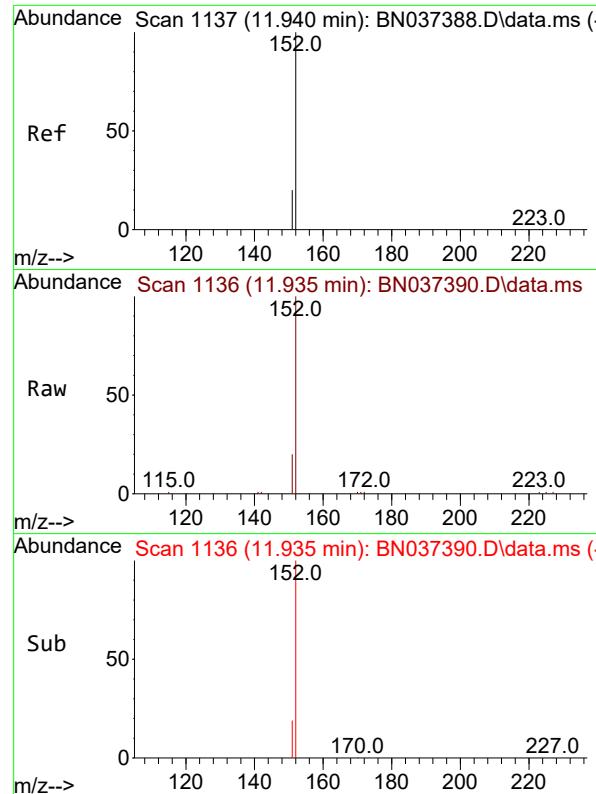


#11  
2-Methylnaphthalene-d10  
Concen: 1.624 ng  
RT: 11.935 min Scan# 1:Instrument :  
Delta R.T. -0.005 min BNA\_N  
Lab File: BN037390.D ClientSampleId :  
Acq: 26 Jun 2025 13:05 SSTDICC1.6


Tgt Ion:152 Resp: 9434  
Ion Ratio Lower Upper  
152 100  
151 21.5 18.4 27.6

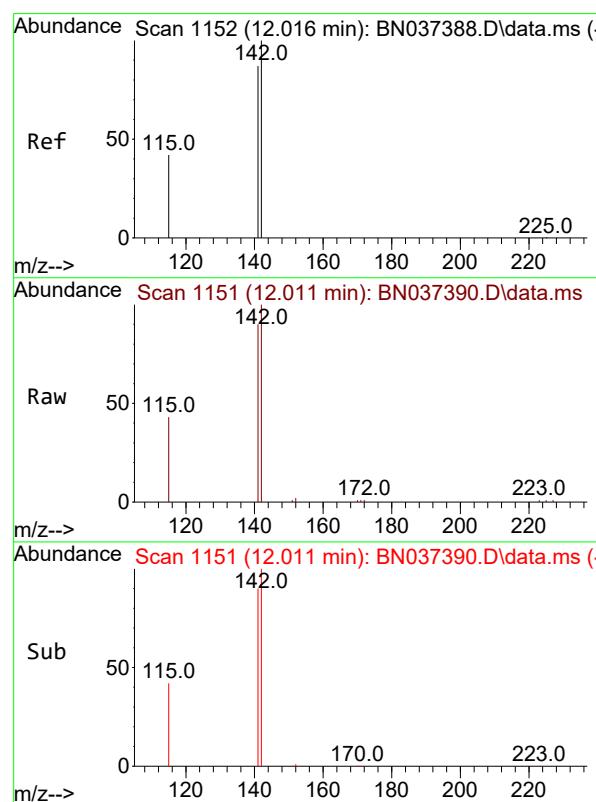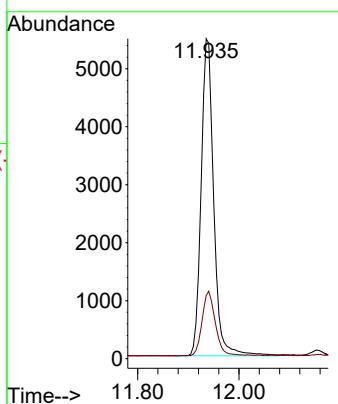

#12  
2-Methylnaphthalene  
Concen: 1.685 ng  
RT: 12.011 min Scan# 1151  
Delta R.T. -0.005 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

Tgt Ion:142 Resp: 11211  
Ion Ratio Lower Upper  
142 100  
141 90.4 70.1 105.1  
115 42.7 35.8 53.6


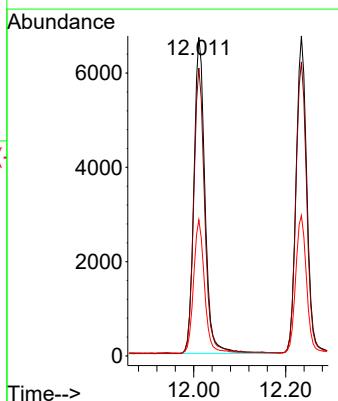


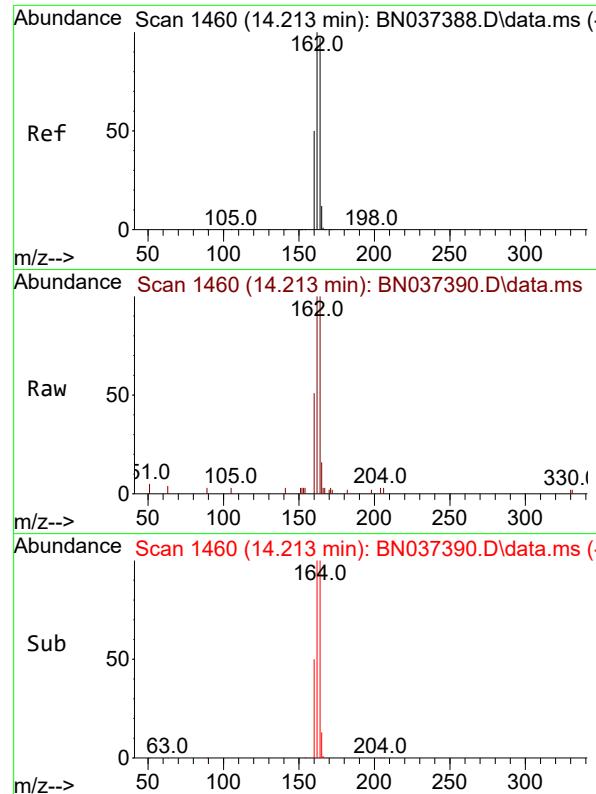

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1460  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6




Tgt Ion:164 Resp: 2497  
Ion Ratio Lower Upper  
164 100  
162 99.8 82.6 123.8  
160 51.0 42.2 63.2

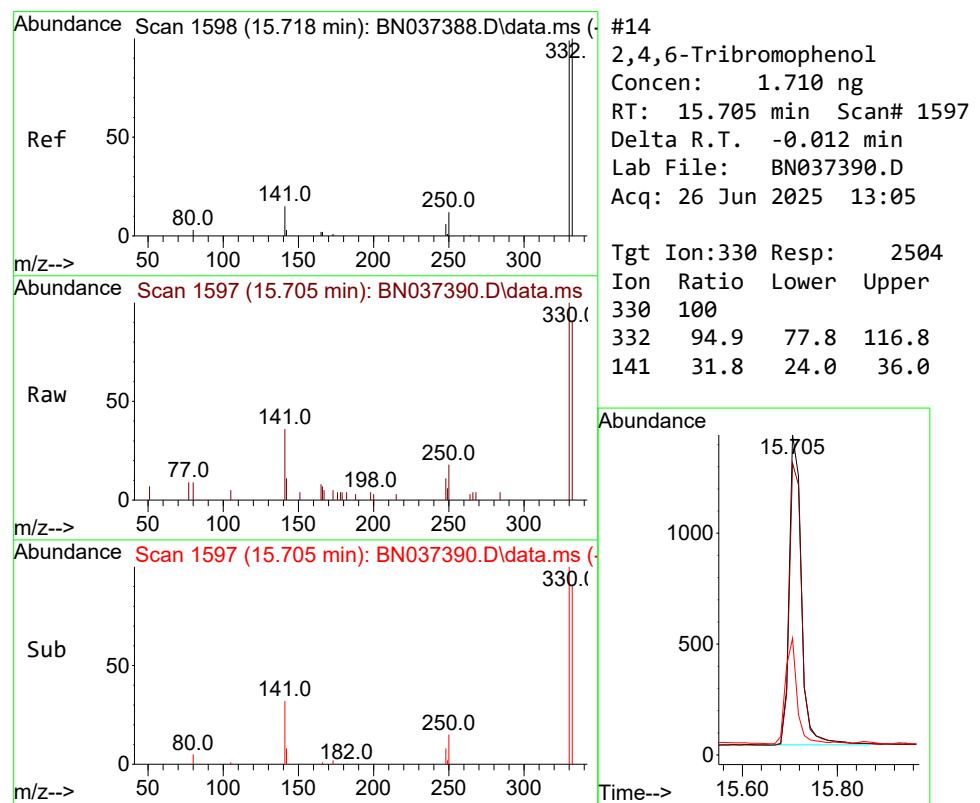

#14  
2,4,6-Tribromophenol  
Concen: 1.710 ng  
RT: 15.705 min Scan# 1597  
Delta R.T. -0.012 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05





Tgt Ion:330 Resp: 2504  
Ion Ratio Lower Upper  
330 100  
332 94.9 77.8 116.8  
141 31.8 24.0 36.0






#15  
2-Fluorobiphenyl  
Concen: 1.666 ng  
RT: 12.833 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05  
ClientSampleId : SSTDICC1.6




Tgt Ion:172 Resp: 17962  
Ion Ratio Lower Upper  
172 100  
171 35.3 28.8 43.2  
170 23.7 20.3 30.5

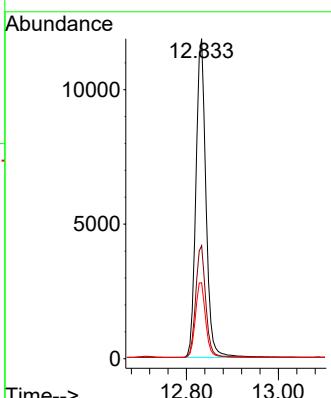

#16  
Acenaphthylene  
Concen: 1.653 ng  
RT: 13.925 min Scan# 1433  
Delta R.T. -0.011 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

Tgt Ion:152 Resp: 17120  
Ion Ratio Lower Upper  
152 100  
151 19.9 15.8 23.6  
153 13.1 10.3 15.5

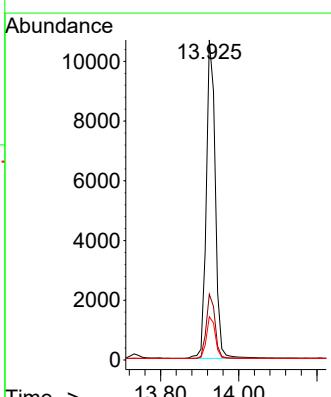

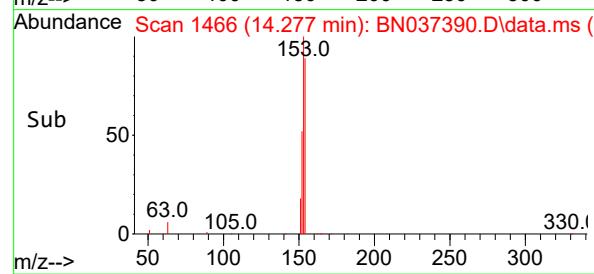

#17

Acenaphthene

Concen: 1.659 ng

RT: 14.277 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037390.D

Acq: 26 Jun 2025 13:05

Instrument :

BNA\_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:154 Resp: 11218

Ion Ratio Lower Upper

154 100

153 115.8 94.6 141.8

152 61.2 50.2 75.2

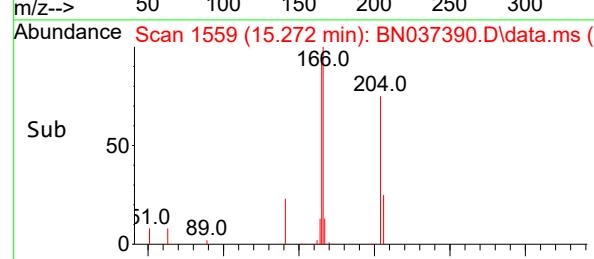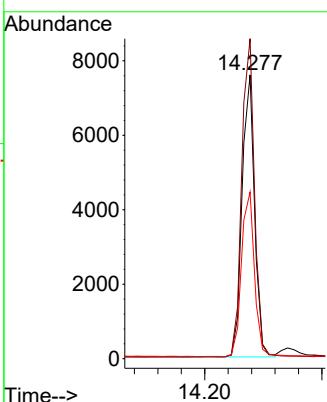

#18

Fluorene

Concen: 1.676 ng

RT: 15.272 min Scan# 1559

Delta R.T. 0.000 min

Lab File: BN037390.D

Acq: 26 Jun 2025 13:05


Tgt Ion:166 Resp: 16008


Ion Ratio Lower Upper

166 100

165 99.2 79.4 119.2

167 13.5 10.6 15.8


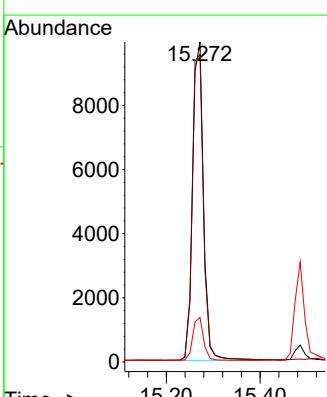


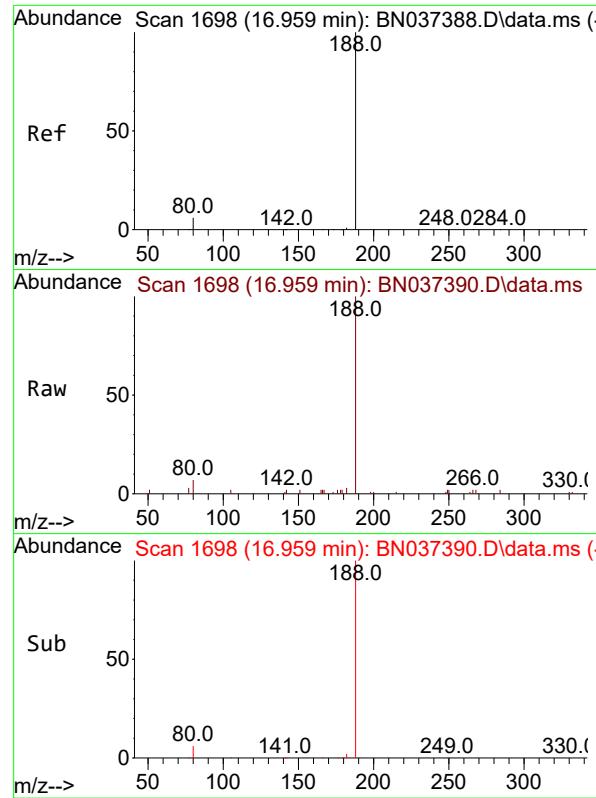

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.959 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:188 Resp: 5134  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 7.4 6.2 9.4

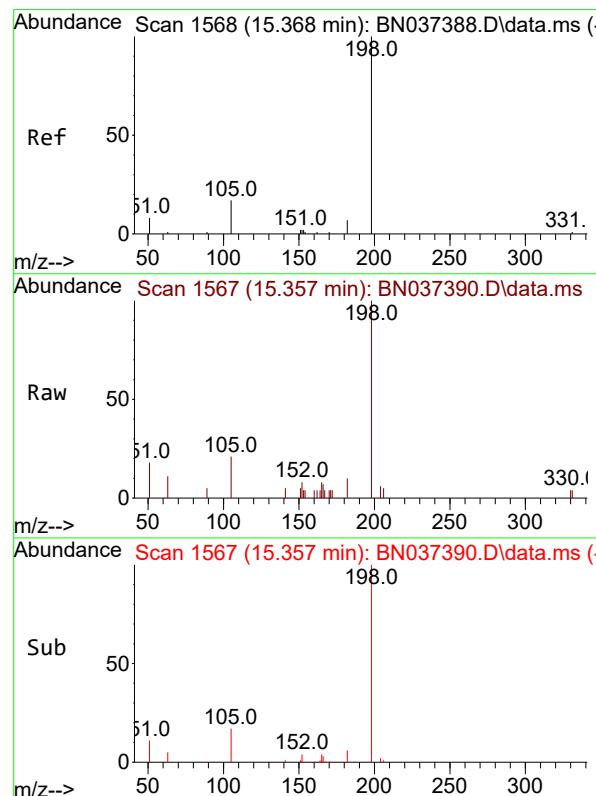

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 1.762 ng  
 RT: 15.357 min Scan# 1567  
 Delta R.T. -0.011 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05



Tgt Ion:198 Resp: 2324  
 Ion Ratio Lower Upper  
 198 100  
 51 18.0 38.8 58.2#  
 105 21.3 29.8 44.6#



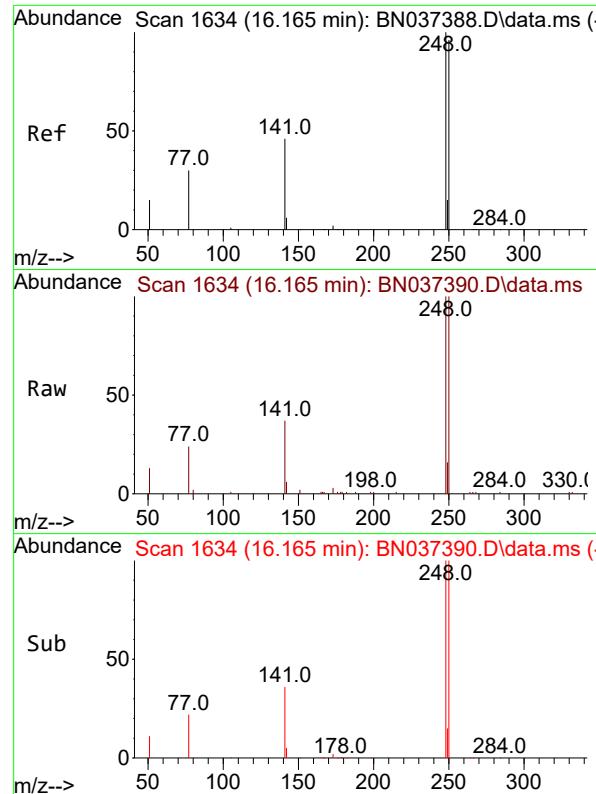


#21  
4-Bromophenyl-phenylether  
Concen: 1.718 ng  
RT: 16.165 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
ClientSampleId : SSTDICC1.6  
Acq: 26 Jun 2025 13:05


Tgt Ion:248 Resp: 6221  
Ion Ratio Lower Upper  
248 100  
250 99.7 77.0 115.4  
141 37.2 38.7 58.1#

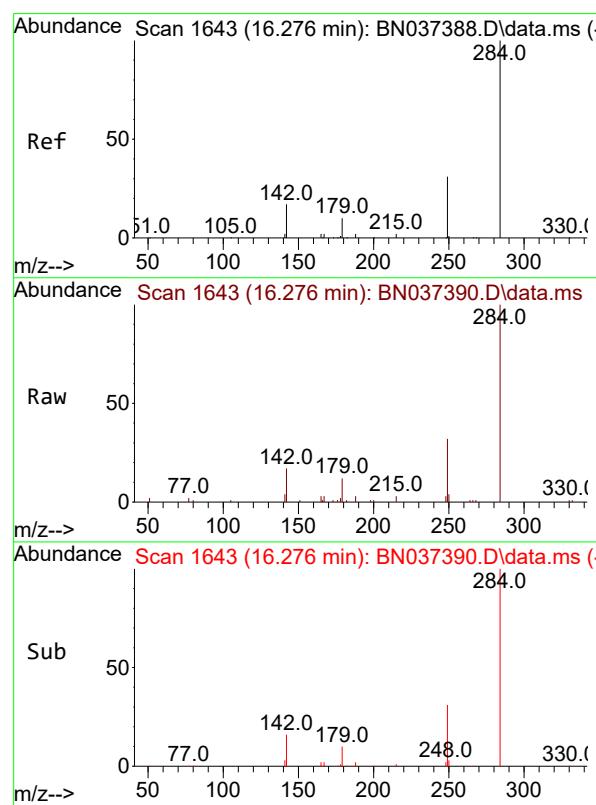

#22  
Hexachlorobenzene  
Concen: 1.638 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

Tgt Ion:284 Resp: 6380  
Ion Ratio Lower Upper  
284 100  
142 34.9 27.2 40.8  
249 34.5 26.7 40.1





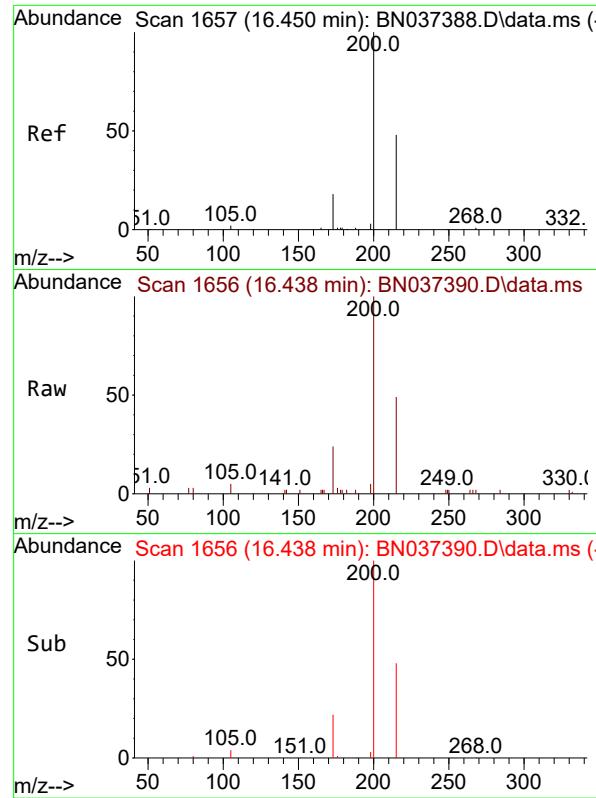

#23  
Atrazine  
Concen: 1.663 ng  
RT: 16.438 min Scan# 1  
Delta R.T. -0.012 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6



Tgt Ion:200 Resp: 4771  
Ion Ratio Lower Upper  
200 100  
173 23.6 19.0 28.6  
215 49.4 41.3 61.9

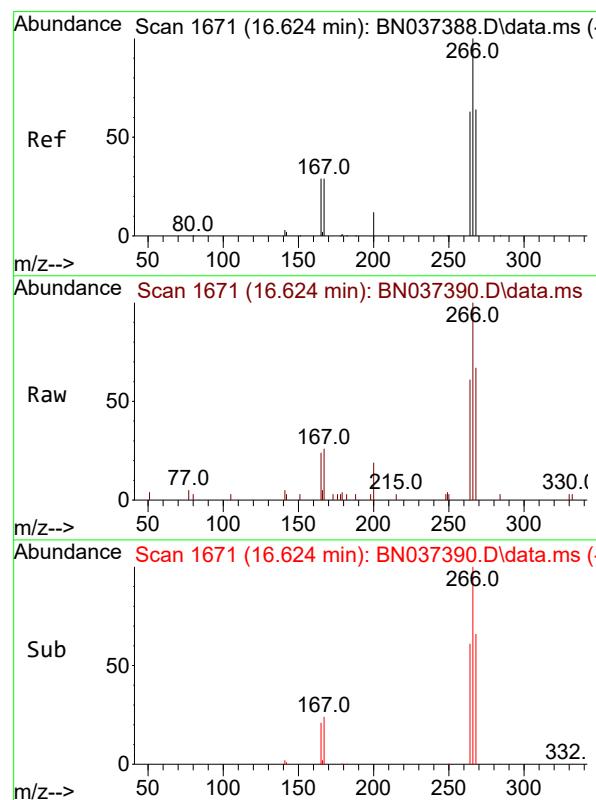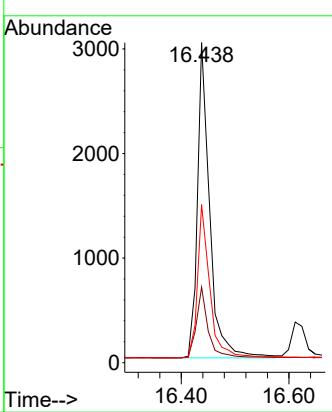

#24  
Pentachlorophenol  
Concen: 1.612 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

Tgt Ion:266 Resp: 3391  
Ion Ratio Lower Upper  
266 100  
264 63.2 49.2 73.8  
268 63.9 54.2 81.4

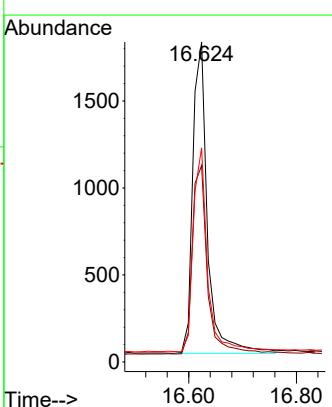

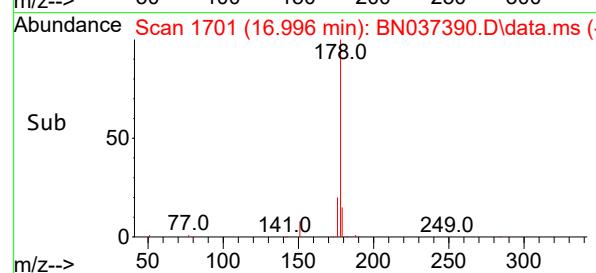

#25

Phenanthrene

Concen: 1.663 ng

RT: 16.996 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN037390.D

Acq: 26 Jun 2025 13:05

Instrument:

BNA\_N

ClientSampleId :

SSTDICC1.6




Tgt Ion:178 Resp: 24063

Ion Ratio Lower Upper

178 100

176 19.3 15.6 23.4

179 15.2 12.8 19.2

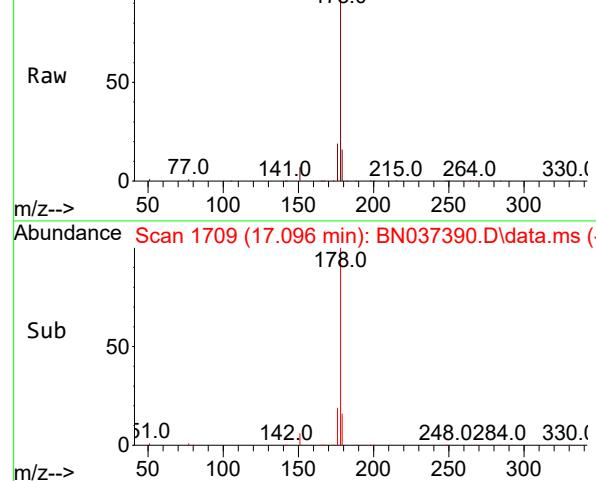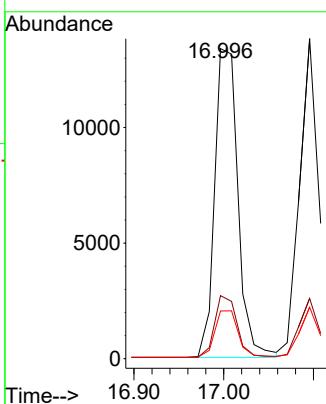

#26

Anthracene

Concen: 1.662 ng

RT: 17.096 min Scan# 1709

Delta R.T. 0.000 min

Lab File: BN037390.D

Acq: 26 Jun 2025 13:05


Tgt Ion:178 Resp: 22103


Ion Ratio Lower Upper

178 100

176 18.7 14.9 22.3

179 15.7 12.4 18.6


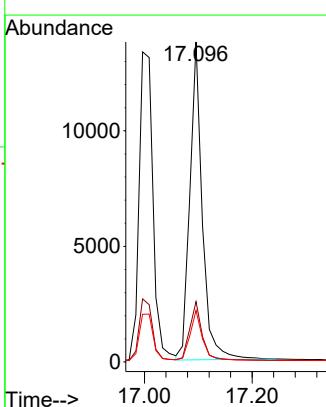


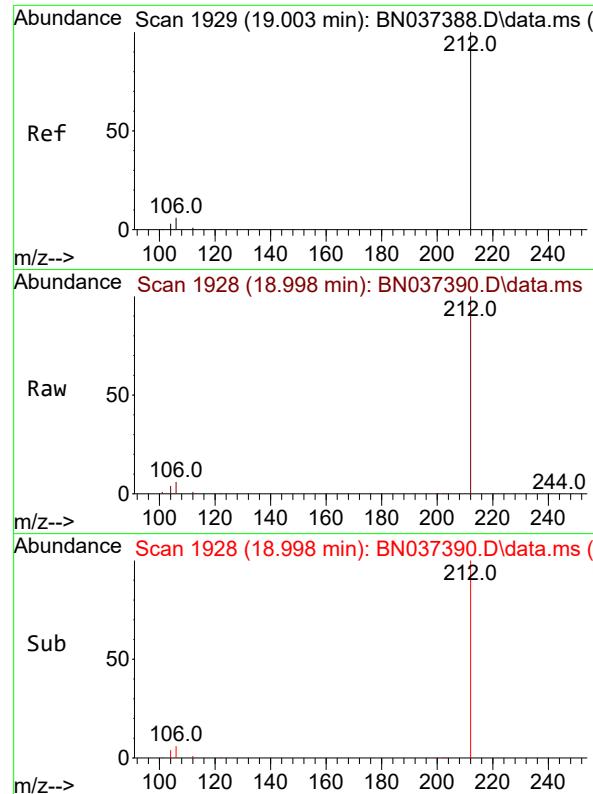

#27  
 Fluoranthene-d10  
 Concen: 1.565 ng  
 RT: 18.998 min Scan# 1  
 Delta R.T. -0.005 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:212 Resp: 23030  
 Ion Ratio Lower Upper  
 212 100  
 106 5.8 4.5 6.7  
 104 3.6 2.7 4.1

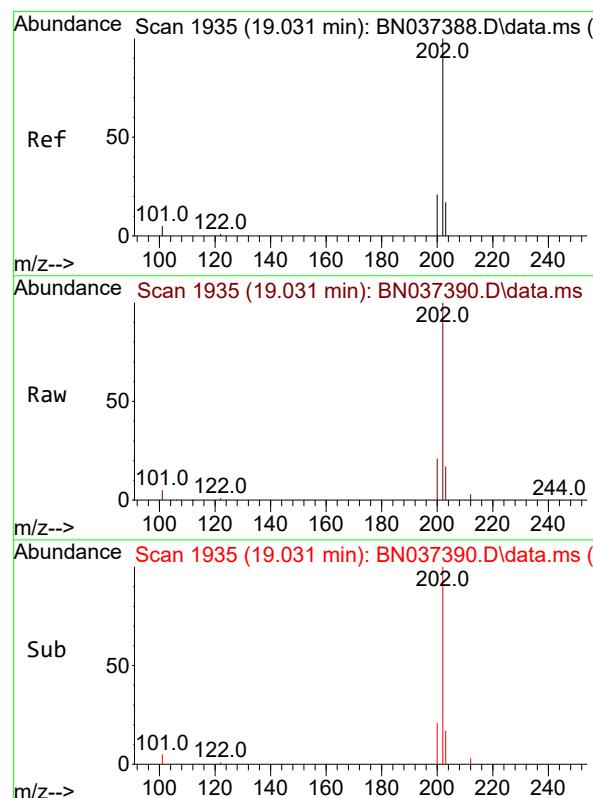

#28  
 Fluoranthene  
 Concen: 1.653 ng  
 RT: 19.031 min Scan# 1935  
 Delta R.T. 0.000 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05

Tgt Ion:202 Resp: 30535  
 Ion Ratio Lower Upper  
 202 100  
 101 5.1 3.8 5.6  
 203 17.1 13.5 20.3





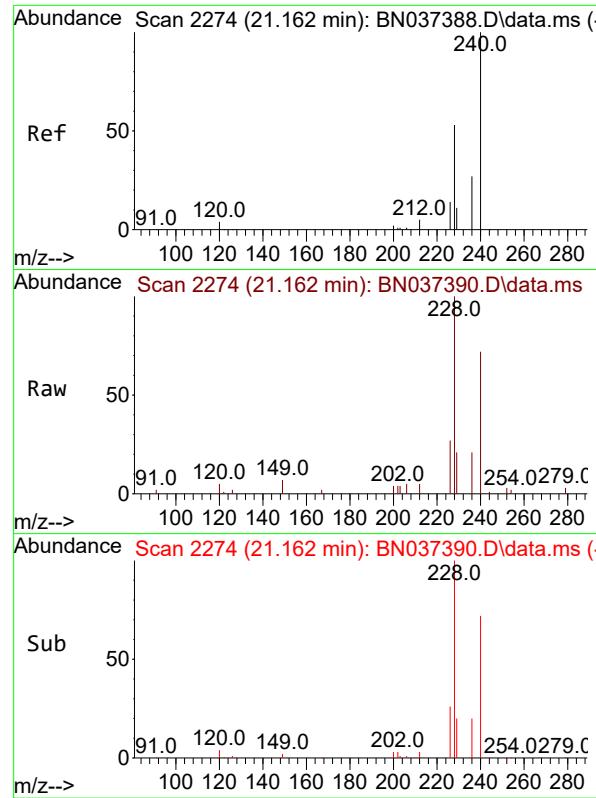

#29  
Chrysene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 21.162 min Scan# 2  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6


Tgt Ion:240 Resp: 4846  
Ion Ratio Lower Upper  
240 100  
120 7.4 5.3 7.9  
236 29.4 22.7 34.1

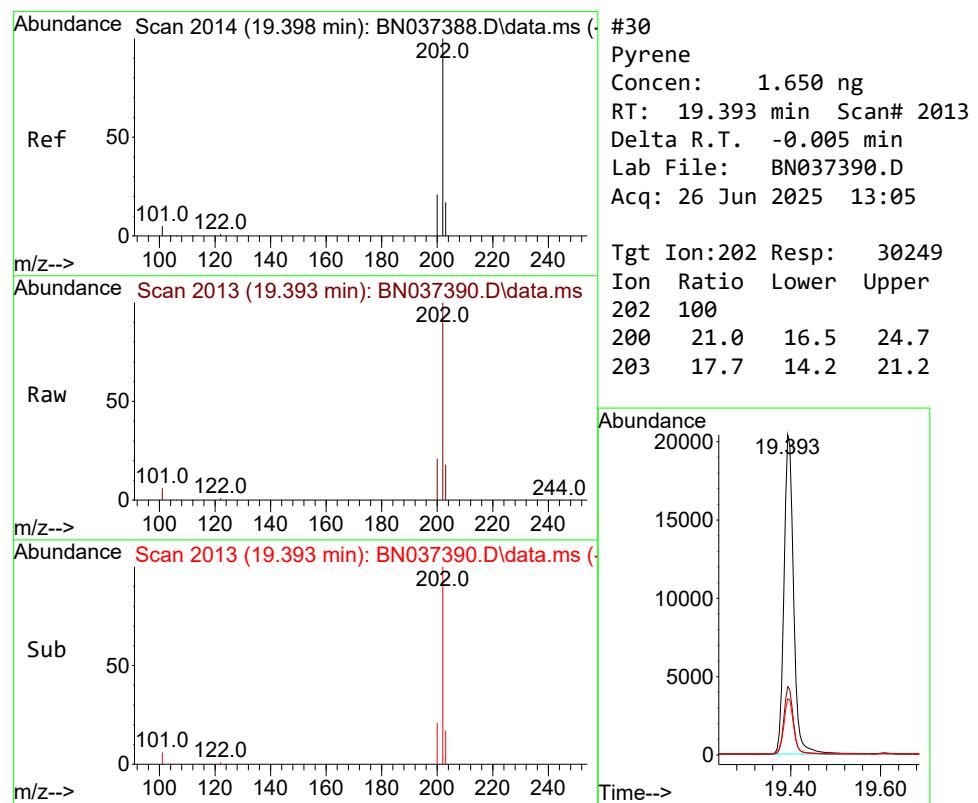

#30  
Pyrene  
Concen: 1.650 ng  
RT: 19.393 min Scan# 2013  
Delta R.T. -0.005 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

Tgt Ion:202 Resp: 30249  
Ion Ratio Lower Upper  
202 100  
200 21.0 16.5 24.7  
203 17.7 14.2 21.2





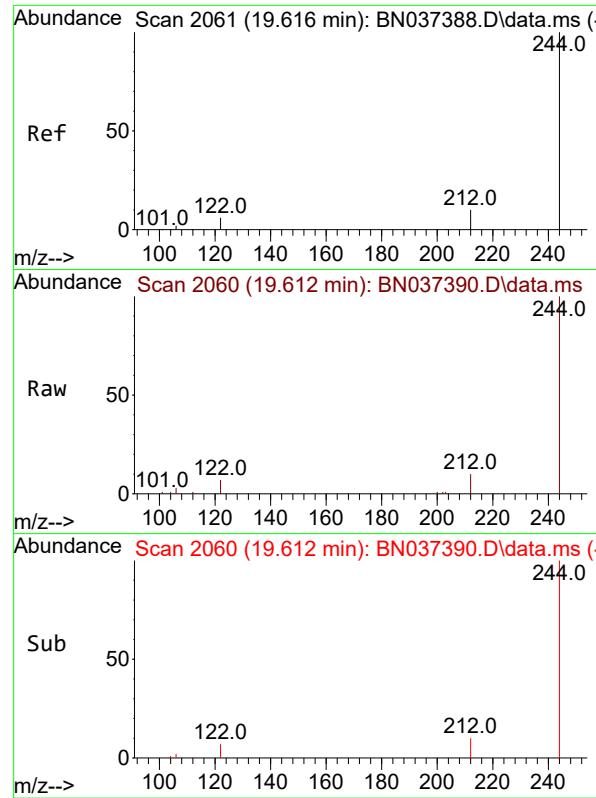

#31  
**Terphenyl-d14**  
Concen: 1.647 ng  
RT: 19.612 min Scan# 2  
Delta R.T. -0.005 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
ClientSampleId : SSTDICC1.6




Tgt Ion:244 Resp: 17013  
Ion Ratio Lower Upper  
244 100  
212 10.2 9.1 13.7  
122 7.1 6.3 9.5

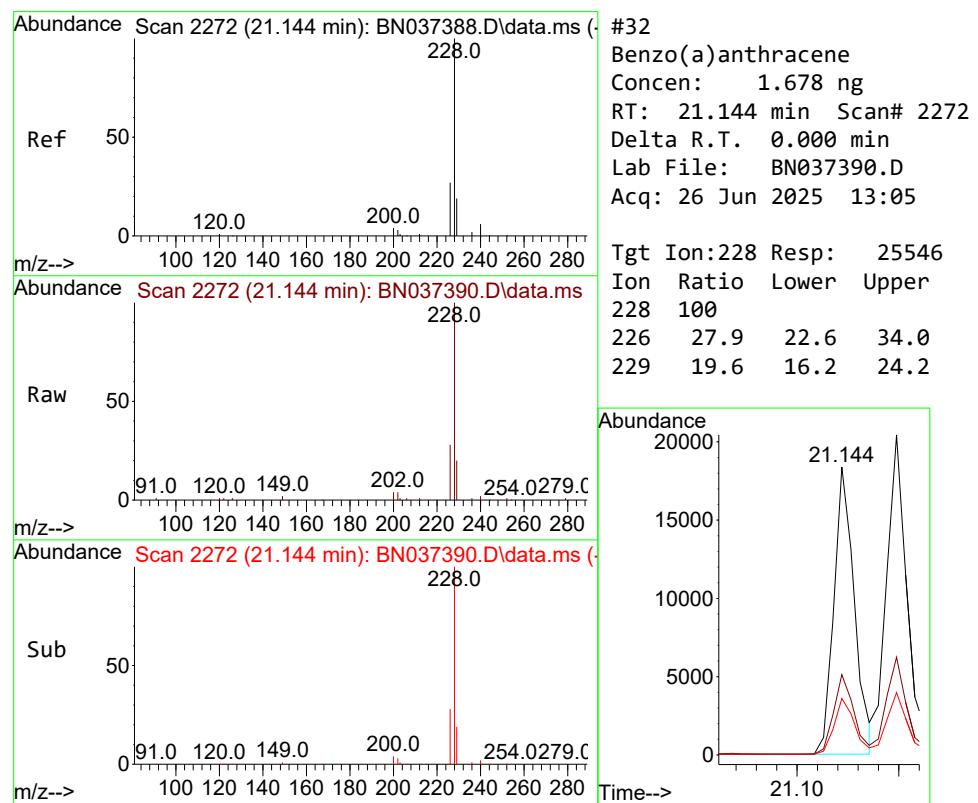

#32  
**Benzo(a)anthracene**  
Concen: 1.678 ng  
RT: 21.144 min Scan# 2272  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05





Tgt Ion:228 Resp: 25546  
Ion Ratio Lower Upper  
228 100  
226 27.9 22.6 34.0  
229 19.6 16.2 24.2



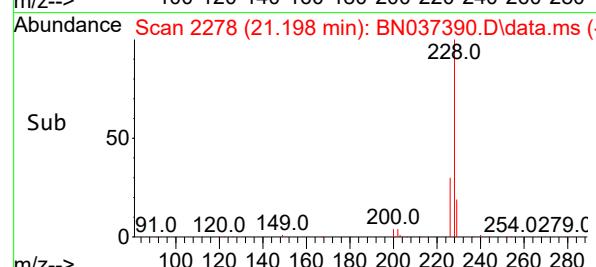


#33  
Chrysene  
Concen: 1.598 ng  
RT: 21.198 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05  
ClientSampleId : SSTDICC1.6


Tgt Ion:228 Resp: 30118  
Ion Ratio Lower Upper  
228 100  
226 30.5 24.5 36.7  
229 19.5 16.1 24.1

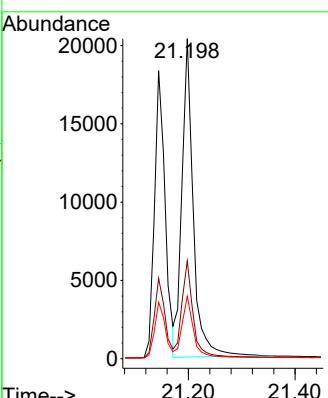

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 1.548 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. 0.000 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

Tgt Ion:149 Resp: 9332  
Ion Ratio Lower Upper  
149 100  
167 31.7 24.8 37.2  
279 6.3 5.0 7.6


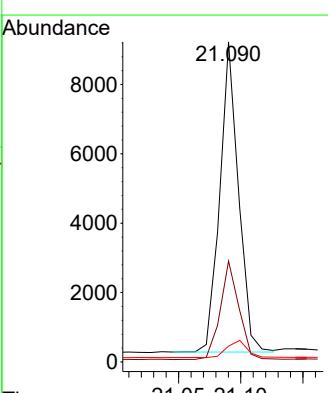


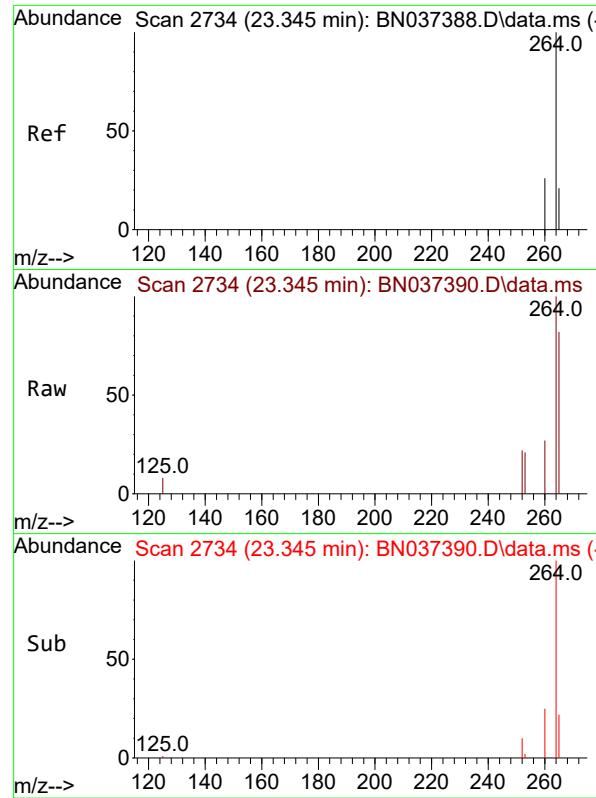

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.345 min Scan# 2  
 Delta R.T. 0.000 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:264 Resp: 4921  
 Ion Ratio Lower Upper  
 264 100  
 260 26.9 21.4 32.0  
 265 82.2 56.2 84.4

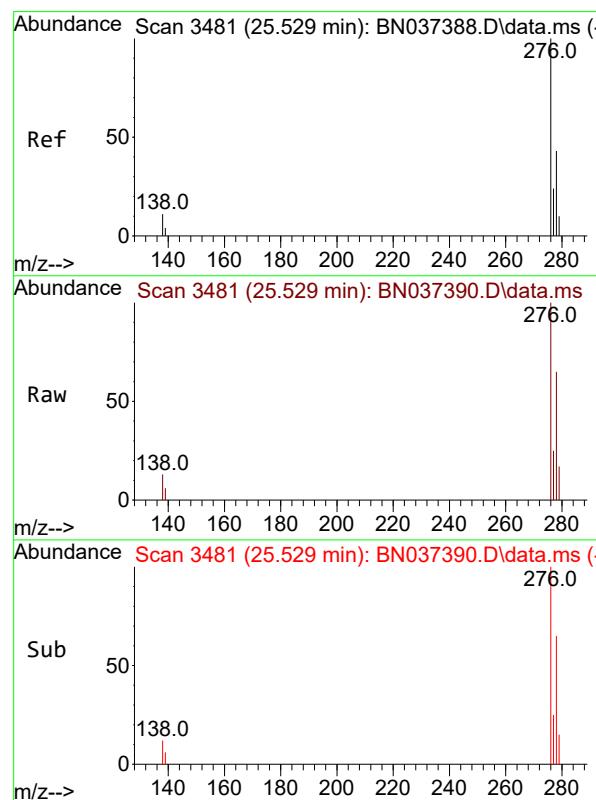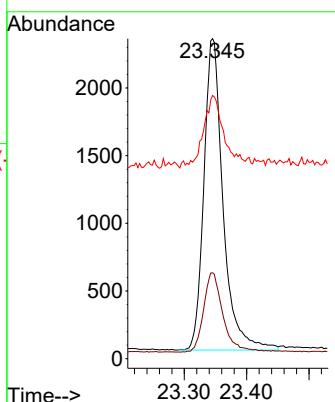

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 1.694 ng  
 RT: 25.529 min Scan# 3481  
 Delta R.T. 0.000 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05

Tgt Ion:276 Resp: 35151  
 Ion Ratio Lower Upper  
 276 100  
 138 12.7 8.5 12.7  
 277 24.5 19.7 29.5





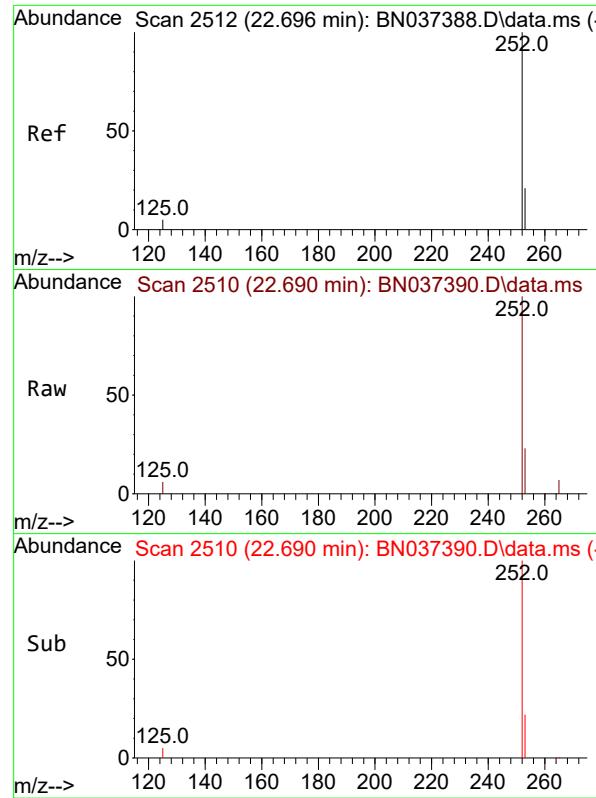

#37  
 Benzo(b)fluoranthene  
 Concen: 1.661 ng  
 RT: 22.690 min Scan# 2  
 Delta R.T. -0.006 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:252 Resp: 28814  
 Ion Ratio Lower Upper  
 252 100  
 253 23.4 22.8 34.2  
 125 5.5 6.2 9.4#

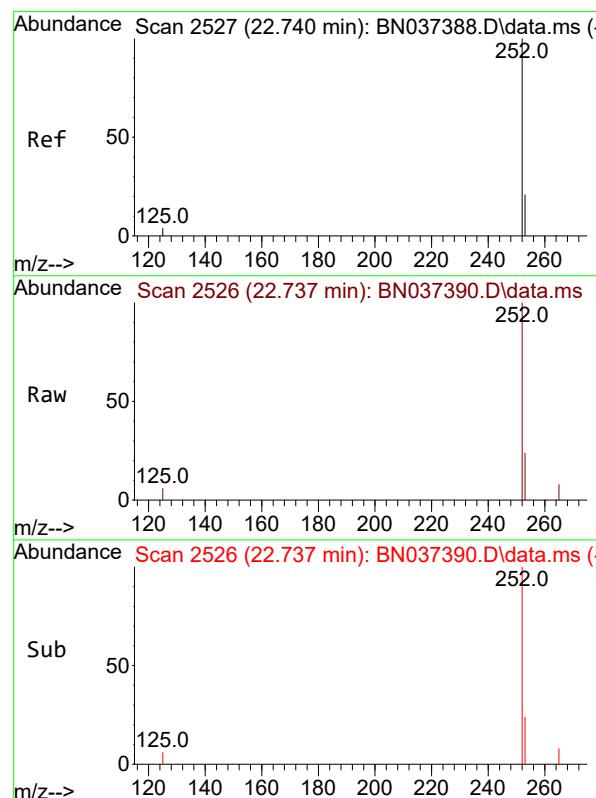

#38  
 Benzo(k)fluoranthene  
 Concen: 1.648 ng  
 RT: 22.737 min Scan# 2526  
 Delta R.T. -0.003 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05

Tgt Ion:252 Resp: 30557  
 Ion Ratio Lower Upper  
 252 100  
 253 23.8 23.2 34.8  
 125 5.7 6.0 9.0#





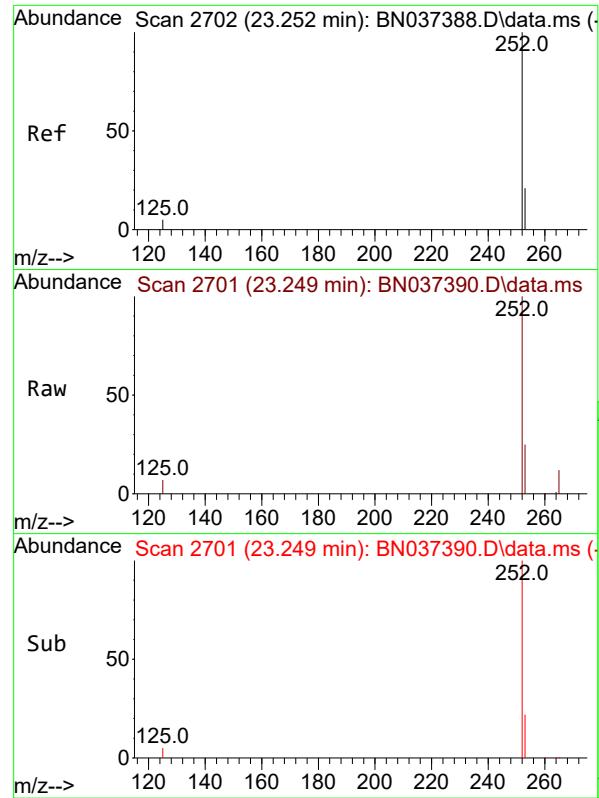

#39  
 Benzo(a)pyrene  
 Concen: 1.640 ng  
 RT: 23.249 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05


Instrument : BNA\_N  
 ClientSampleId : SSTDICC1.6


Tgt Ion:252 Resp: 25315  
 Ion Ratio Lower Upper  
 252 100  
 253 24.9 25.6 38.4#  
 125 6.6 7.5 11.3#

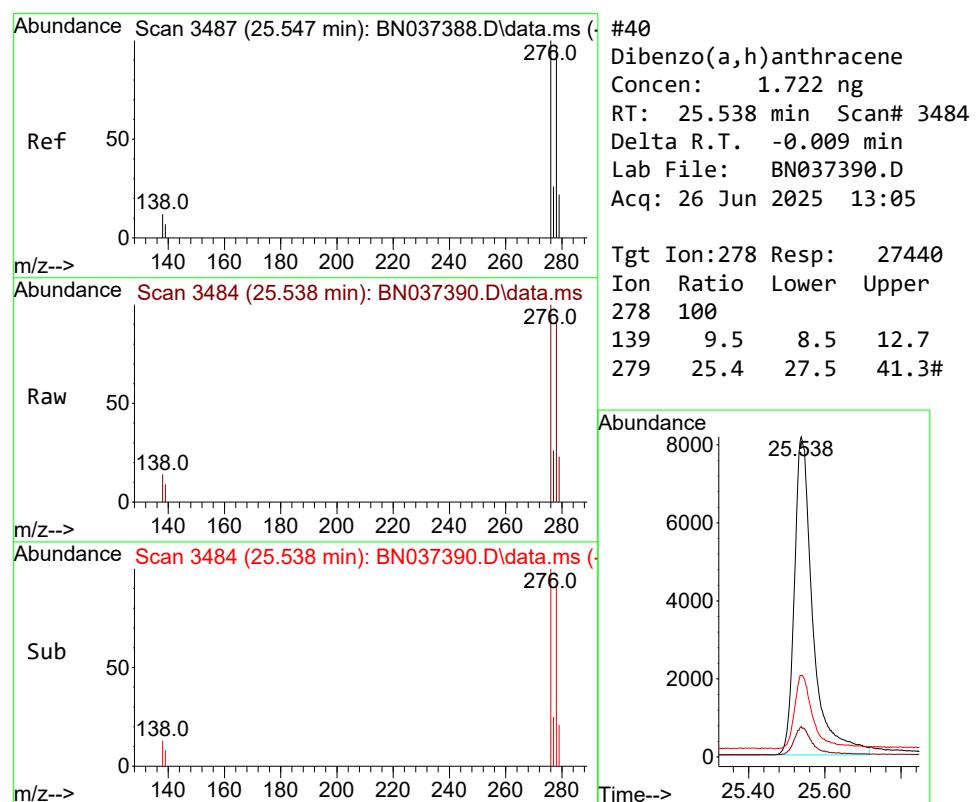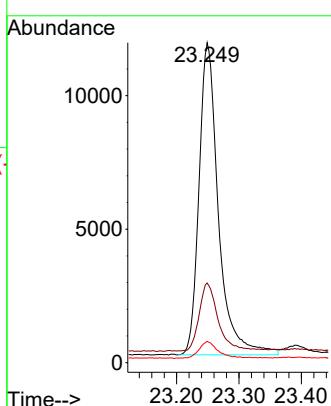

#40  
 Dibenzo(a,h)anthracene  
 Concen: 1.722 ng  
 RT: 25.538 min Scan# 3484  
 Delta R.T. -0.009 min  
 Lab File: BN037390.D  
 Acq: 26 Jun 2025 13:05

Tgt Ion:278 Resp: 27440  
 Ion Ratio Lower Upper  
 278 100  
 139 9.5 8.5 12.7  
 279 25.4 27.5 41.3#

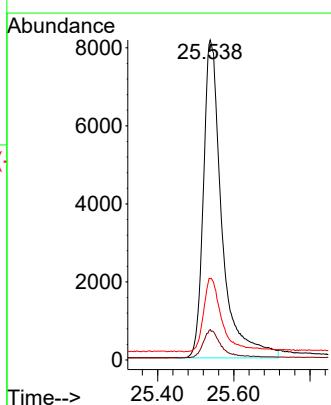


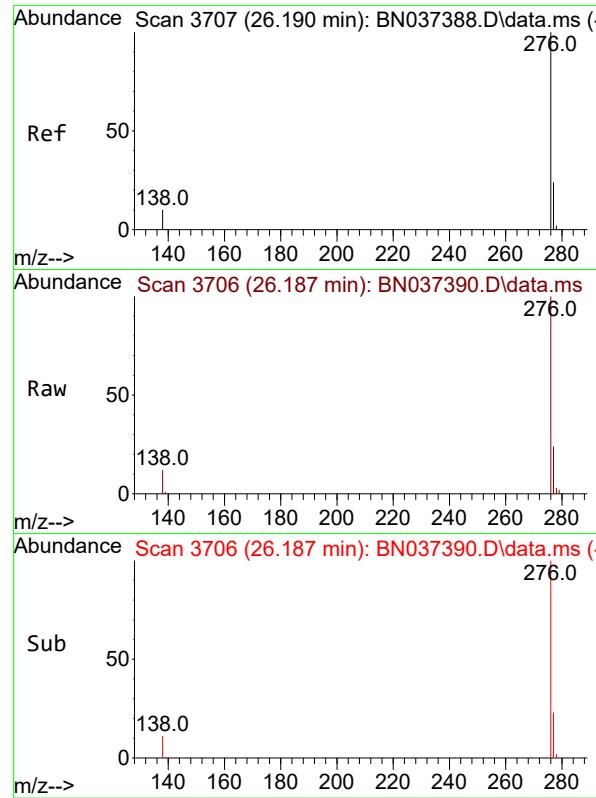

#41  
Benzo(g,h,i)perylene  
Concen: 1.671 ng  
RT: 26.187 min Scan# 3  
Delta R.T. -0.003 min  
Lab File: BN037390.D  
Acq: 26 Jun 2025 13:05

Instrument :  
BNA\_N  
ClientSampleId :  
SSTDICC1.6

Tgt Ion:276 Resp: 31821  
Ion Ratio Lower Upper  
276 100  
277 23.9 21.0 31.4  
138 11.8 9.6 14.4

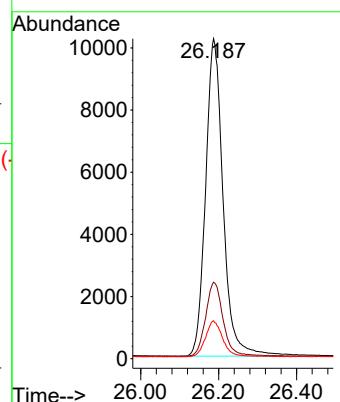

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037391.D  
 Acq On : 26 Jun 2025 13:41  
 Operator : RC/JU  
 Sample : SSTDICC3.2  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC3.2

Quant Time: Jun 26 14:45:16 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.560	152	1913	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4102	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	2755	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	5771	0.400	ng	0.00
29) Chrysene-d12	21.162	240	5566	0.400	ng	0.00
35) Perylene-d12	23.348	264	5442	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	11831	3.209	ng	0.00
5) Phenol-d6	6.744	99	13561	3.547	ng	0.00
8) Nitrobenzene-d5	8.707	82	11574	3.508	ng	-0.01
11) 2-Methylnaphthalene-d10	11.935	152	21511	3.390	ng	0.00
14) 2,4,6-Tribromophenol	15.705	330	5638	3.489	ng	-0.01
15) 2-Fluorobiphenyl	12.833	172	39687	3.337	ng	0.00
27) Fluoranthene-d10	18.998	212	53268	3.221	ng	0.00
31) Terphenyl-d14	19.607	244	39701	3.345	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.097	88	5559	3.243	ng	96
3) n-Nitrosodimethylamine	3.408	42	5726	3.196	ng	# 93
6) bis(2-Chloroethyl)ether	6.997	93	11865	3.490	ng	96
9) Naphthalene	10.383	128	34450	3.263	ng	96
10) Hexachlorobutadiene	10.682	225	13273	3.167	ng	# 98
12) 2-Methylnaphthalene	12.011	142	25164	3.461	ng	97
16) Acenaphthylene	13.924	152	38375	3.359	ng	100
17) Acenaphthene	14.277	154	25275	3.388	ng	97
18) Fluorene	15.271	166	36211	3.437	ng	100
20) 4,6-Dinitro-2-methylph...	15.357	198	5478	3.696	ng	# 55
21) 4-Bromophenyl-phenylether	16.165	248	13953	3.427	ng	# 91
22) Hexachlorobenzene	16.276	284	13881	3.171	ng	98
23) Atrazine	16.438	200	11170	3.463	ng	96
24) Pentachlorophenol	16.624	266	7774	3.288	ng	97
25) Phenanthrene	16.996	178	54938	3.379	ng	99
26) Anthracene	17.095	178	51719	3.460	ng	100
28) Fluoranthene	19.031	202	69575	3.351	ng	99
30) Pyrene	19.393	202	69001	3.276	ng	99
32) Benzo(a)anthracene	21.144	228	60725	3.472	ng	98
33) Chrysene	21.198	228	67241	3.106	ng	99
34) Bis(2-ethylhexyl)phtha...	21.090	149	21735	3.139	ng	100
36) Indeno(1,2,3-cd)pyrene	25.526	276	80692	3.517	ng	# 97
37) Benzo(b)fluoranthene	22.693	252	65471	3.412	ng	# 90
38) Benzo(k)fluoranthene	22.734	252	70234	3.425	ng	# 89
39) Benzo(a)pyrene	23.252	252	58393	3.422	ng	# 86
40) Dibenzo(a,h)anthracene	25.541	278	64655	3.668	ng	# 86
41) Benzo(g,h,i)perylene	26.187	276	72186	3.427	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037391.D  
 Acq On : 26 Jun 2025 13:41  
 Operator : RC/JU  
 Sample : SSTDICC3.2  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC3.2


Quant Time: Jun 26 14:45:16 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration

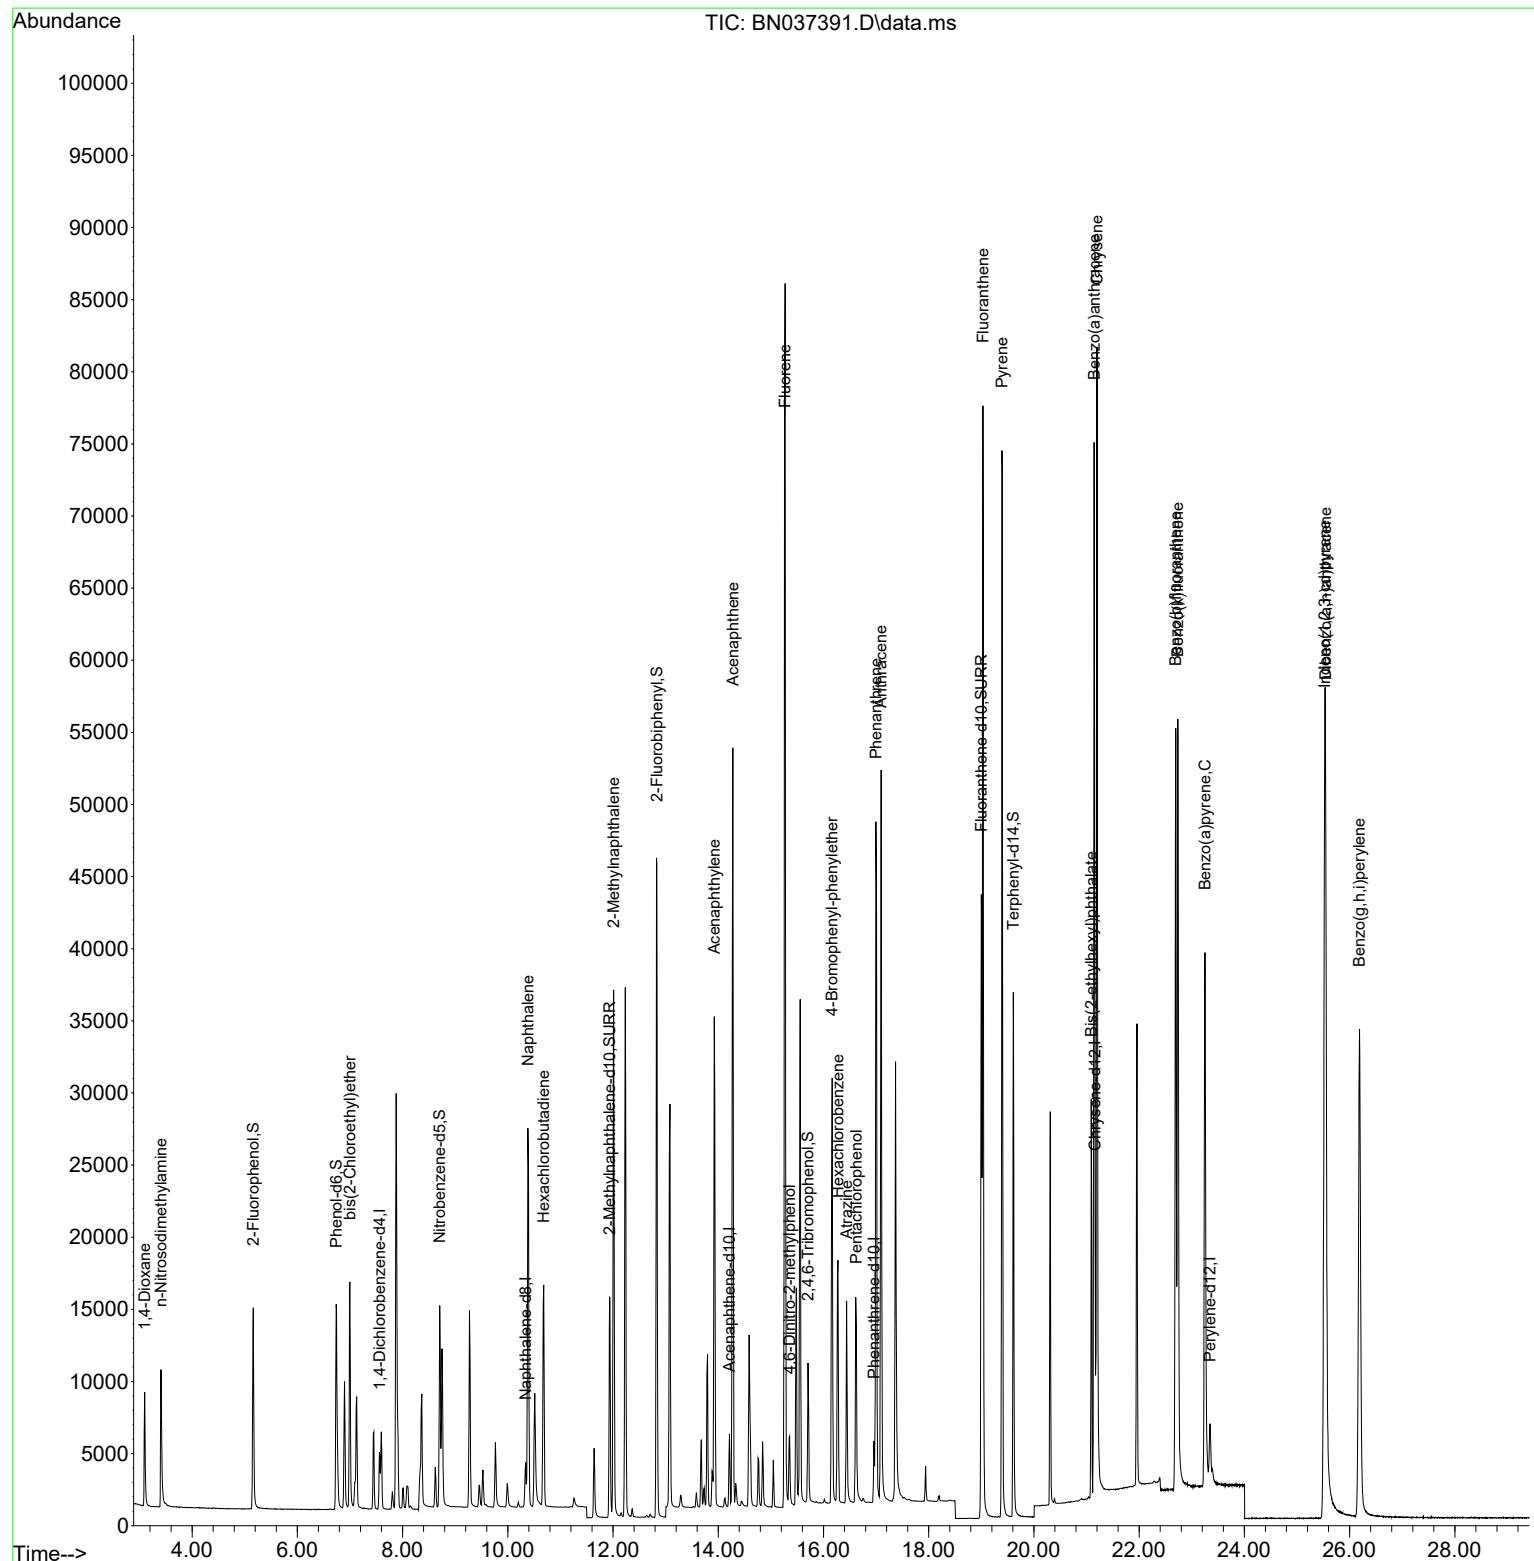






#1  
 1,4-Dichlorobenzene-d4  
 Concen: 0.400 ng  
 RT: 7.560 min Scan# 6  
 Delta R.T. -0.008 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2

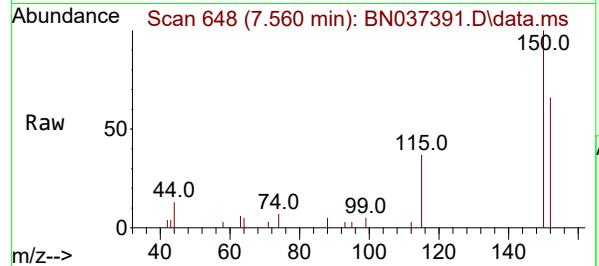



Tgt Ion:152 Resp: 1913  
 Ion Ratio Lower Upper  
 152 100  
 150 150.9 116.2 174.2  
 115 56.4 42.9 64.3

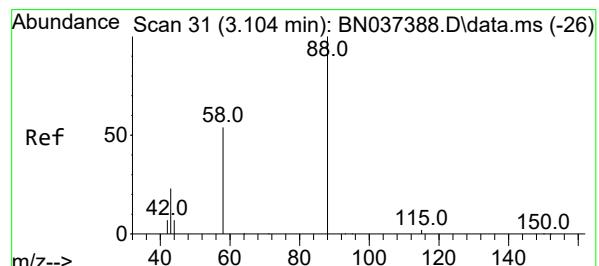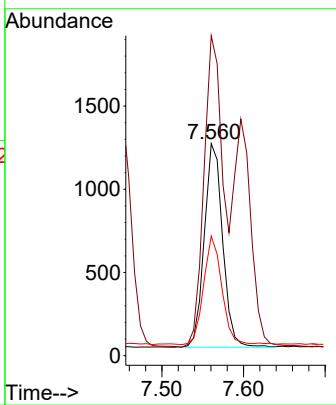
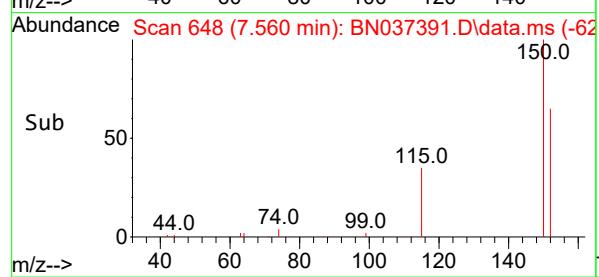


#2  
 1,4-Dioxane  
 Concen: 3.243 ng  
 RT: 3.097 min Scan# 30  
 Delta R.T. -0.007 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41

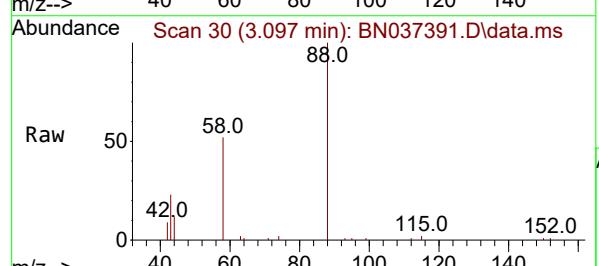

Tgt Ion: 88 Resp: 5559  
 Ion Ratio Lower Upper  
 88 100  
 43 24.1 21.6 32.4  
 58 54.5 45.9 68.9

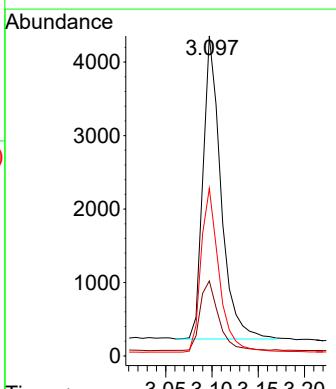

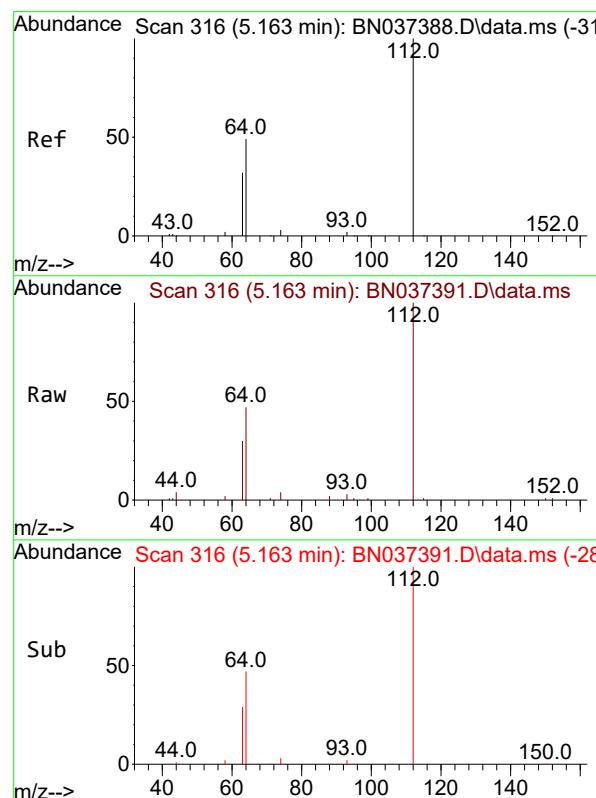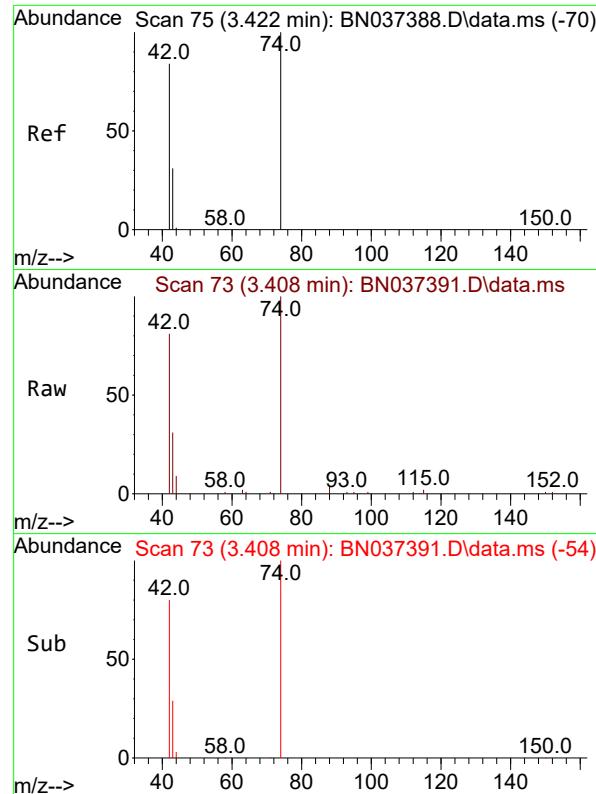

#3

n-Nitrosodimethylamine

Concen: 3.196 ng

RT: 3.408 min Scan# 7

Delta R.T. -0.014 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41

Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2


Tgt Ion: 42 Resp: 5726

Ion Ratio Lower Upper

42 100

74 129.6 97.8 146.8

44 5.2 8.7 13.1#



#4

2-Fluorophenol

Concen: 3.209 ng

RT: 5.163 min Scan# 316

Delta R.T. -0.000 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41


Tgt Ion: 112 Resp: 11831


Ion Ratio Lower Upper

112 100

64 50.5 40.3 60.5

63 31.8 26.1 39.1


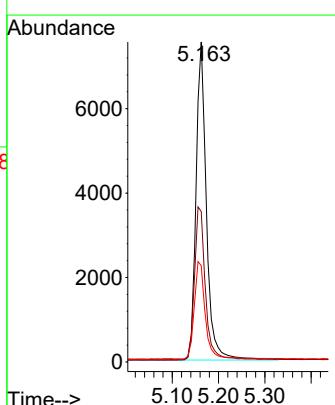


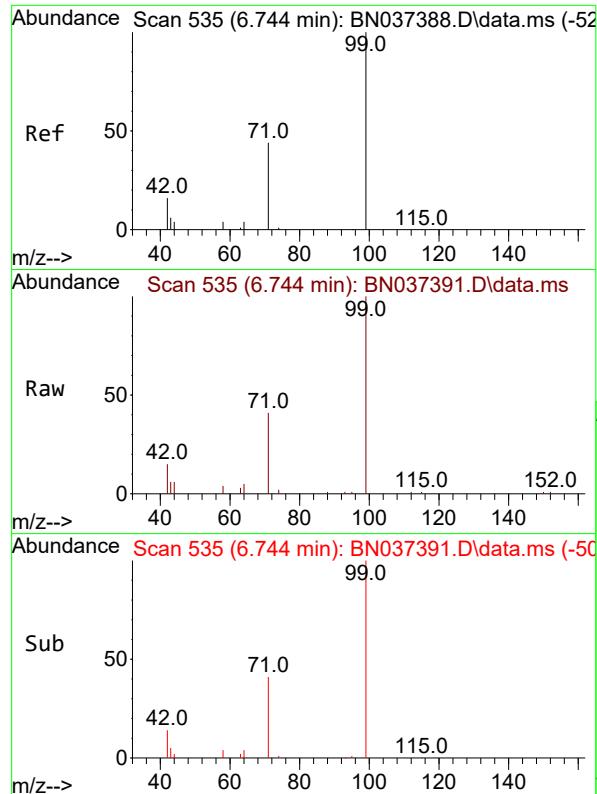

#5  
 Phenol-d6  
 Concen: 3.547 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. -0.000 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion: 99 Resp: 13561  
 Ion Ratio Lower Upper  
 99 100  
 42 18.5 15.6 23.4  
 71 44.5 35.8 53.8

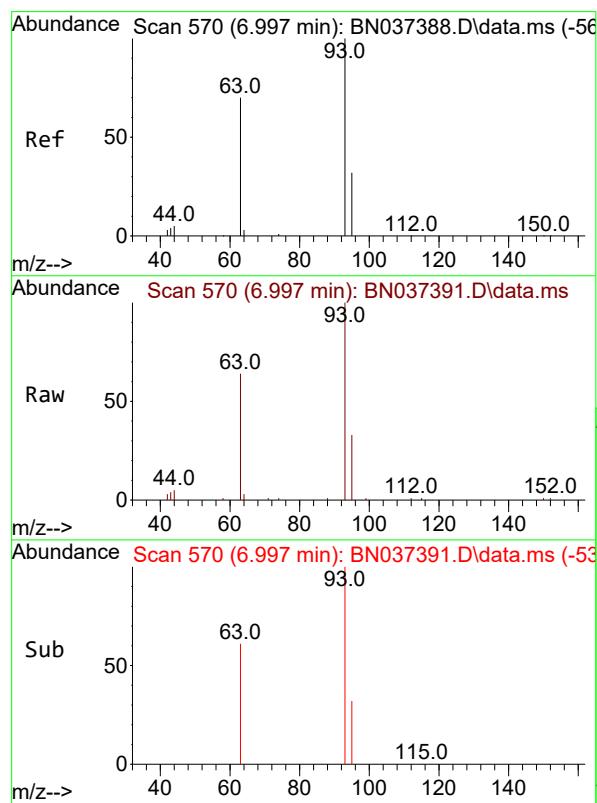

#6  
 bis(2-Chloroethyl)ether  
 Concen: 3.490 ng  
 RT: 6.997 min Scan# 570  
 Delta R.T. -0.000 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41


Tgt Ion: 93 Resp: 11865  
 Ion Ratio Lower Upper  
 93 100  
 63 65.4 49.6 74.4  
 95 31.9 23.9 35.9



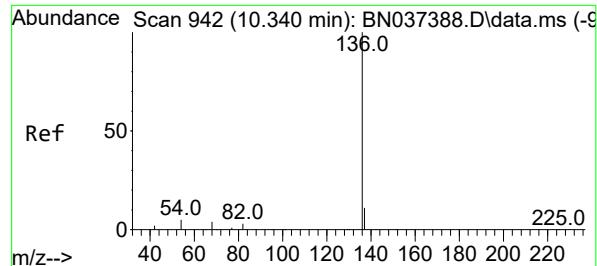

#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41



Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2




Tgt Ion:136 Resp: 4102

Ion Ratio Lower Upper

136	100
137	12.6
54	6.4
68	5.5
	10.4 15.6
	5.6 8.4
	4.6 6.8

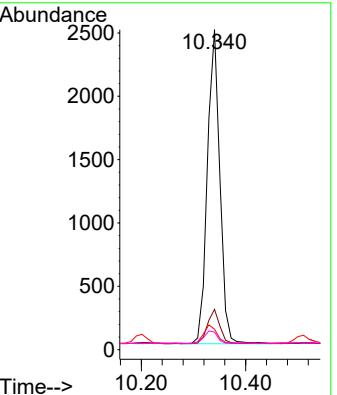



#8  
 Nitrobenzene-d5  
 Concen: 3.508 ng  
 RT: 8.707 min Scan# 789  
 Delta R.T. -0.011 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41






Tgt Ion: 82 Resp: 11574

Ion Ratio Lower Upper





82	100
128	36.3
54	43.4
	34.0 51.0
	37.7 56.5

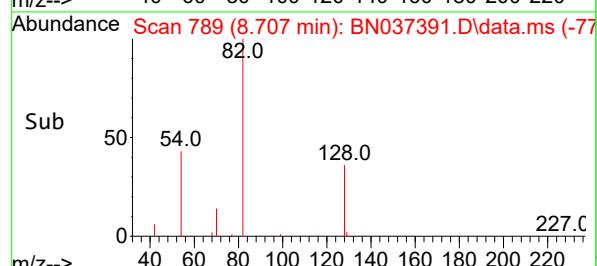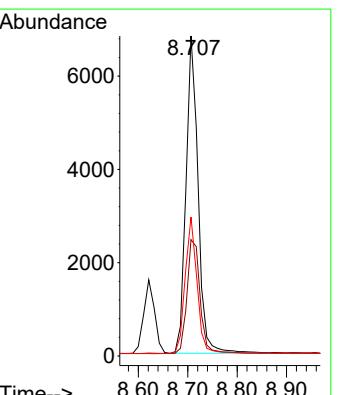

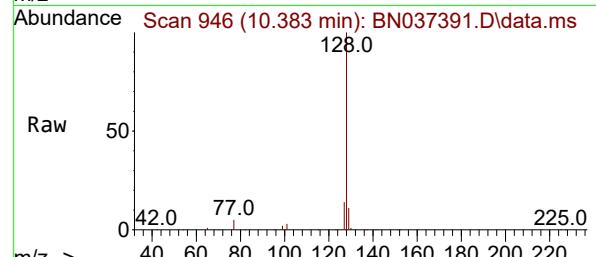


#9  
Naphthalene  
Concen: 3.263 ng  
RT: 10.383 min Scan# 9  
Instrument : BNA\_N  
Delta R.T. -0.011 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41  
ClientSampleId : SSTDICC3.2


Tgt Ion:128 Resp: 34450  
Ion Ratio Lower Upper  
128 100  
129 11.2 10.4 15.6  
127 14.0 12.2 18.4





#10  
Hexachlorobutadiene  
Concen: 3.167 ng  
RT: 10.682 min Scan# 974  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:225 Resp: 13273  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 63.7 49.9 74.9

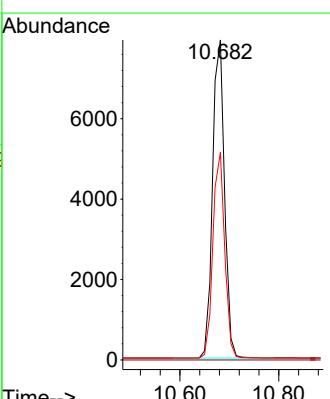




Abundance Scan 1136 (11.935 min): BN037391.D\data.ms (-)

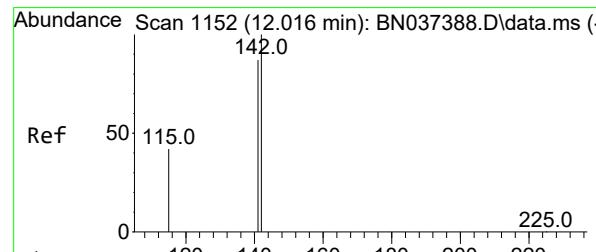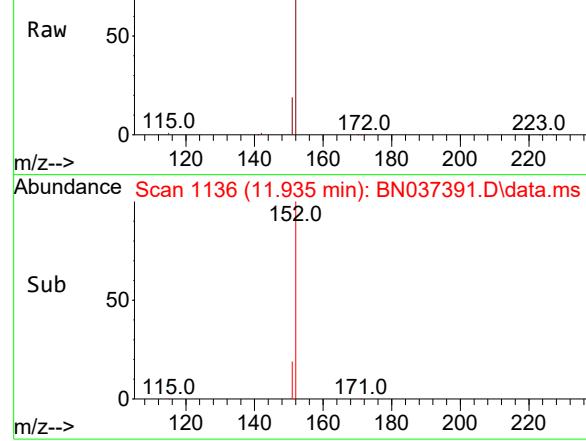

Abundance Scan 1151 (12.011 min): BN037391.D\data.ms (-)

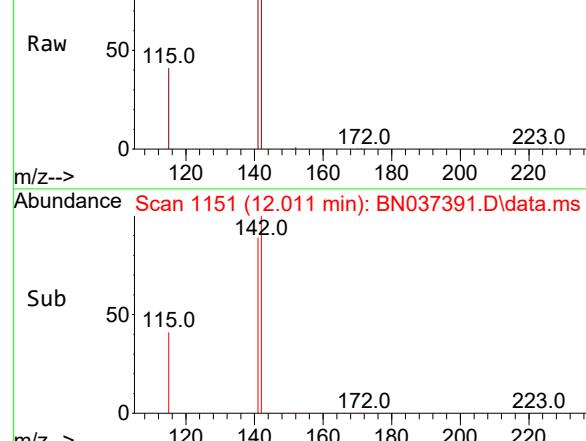

#11

2-Methylnaphthalene-d10

Concen: 3.390 ng

RT: 11.935 min Scan# 1

Delta R.T. -0.005 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41

Instrument :

BNA\_N

ClientSampleId :


SSTDICC3.2

Tgt Ion:152 Resp: 21511

Ion Ratio Lower Upper

152 100

151 21.6 18.4 27.6



#12

2-Methylnaphthalene

Concen: 3.461 ng

RT: 12.011 min Scan# 1151

Delta R.T. -0.005 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41


Tgt Ion:142 Resp: 25164


Ion Ratio Lower Upper

142 100

141 89.0 70.1 105.1

115 41.4 35.8 53.6





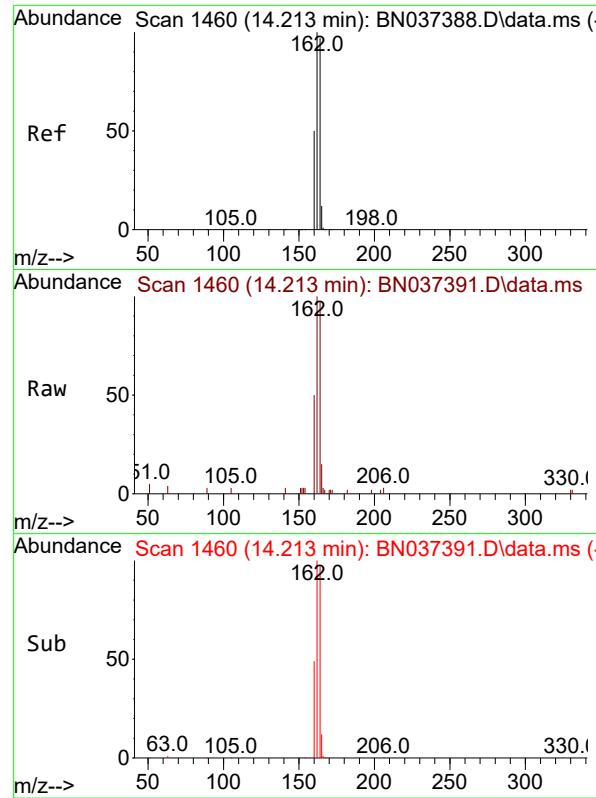

#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1460  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:164 Resp: 2755  
Ion Ratio Lower Upper  
164 100  
162 103.5 82.6 123.8  
160 51.3 42.2 63.2

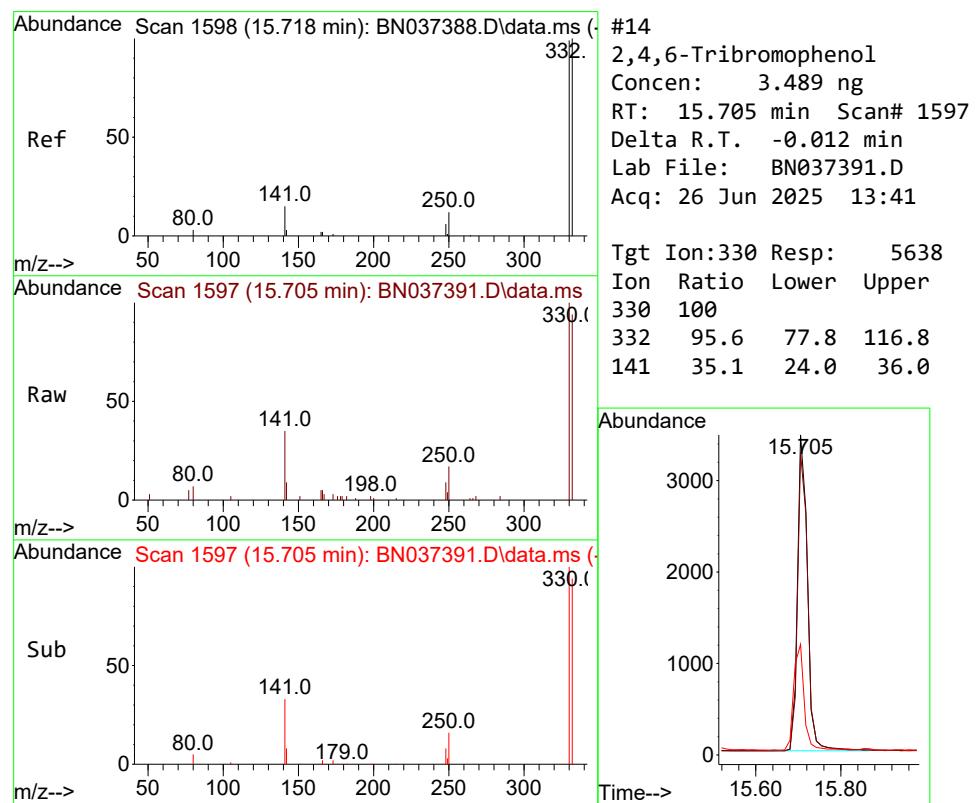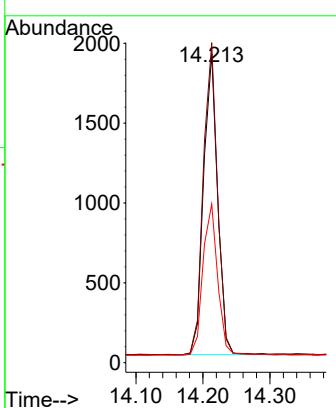

#14  
2,4,6-Tribromophenol  
Concen: 3.489 ng  
RT: 15.705 min Scan# 1597  
Delta R.T. -0.012 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:330 Resp: 5638  
Ion Ratio Lower Upper  
330 100  
332 95.6 77.8 116.8  
141 35.1 24.0 36.0


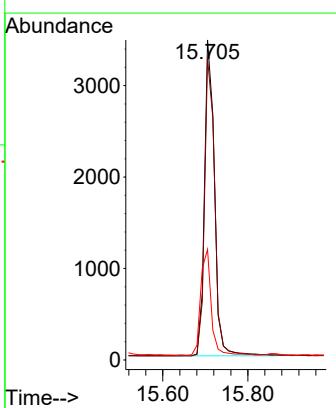


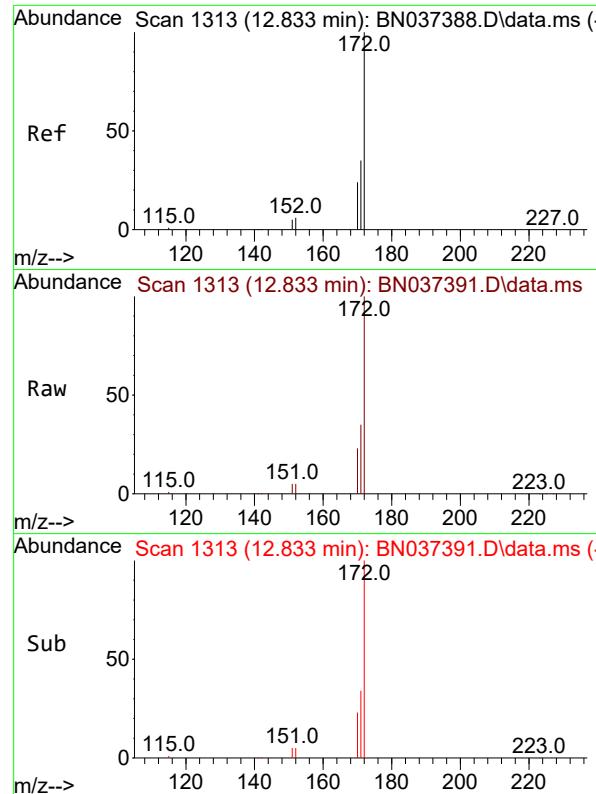

#15  
2-Fluorobiphenyl  
Concen: 3.337 ng  
RT: 12.833 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2




Tgt Ion:172 Resp: 39687  
Ion Ratio Lower Upper  
172 100  
171 34.7 28.8 43.2  
170 23.1 20.3 30.5

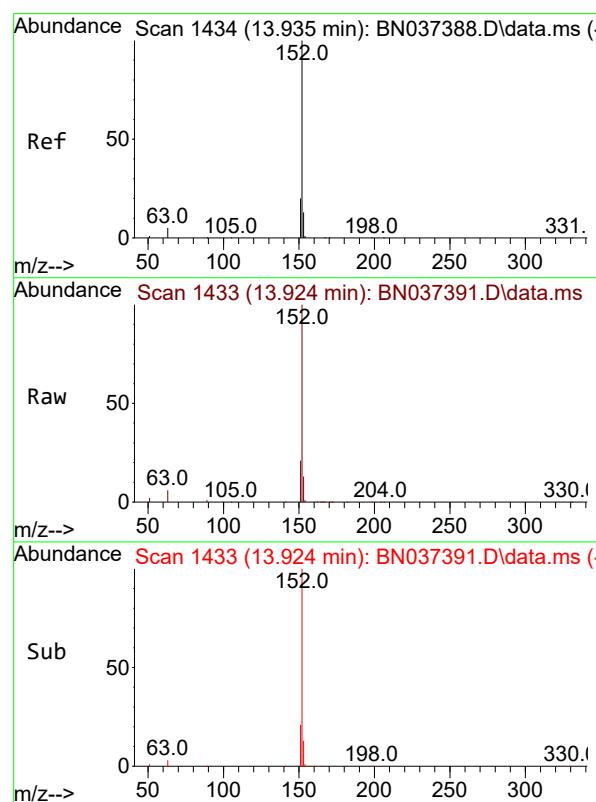

#16  
Acenaphthylene  
Concen: 3.359 ng  
RT: 13.924 min Scan# 1433  
Delta R.T. -0.011 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:152 Resp: 38375  
Ion Ratio Lower Upper  
152 100  
151 19.8 15.8 23.6  
153 13.1 10.3 15.5





#17

Acenaphthene

Concen: 3.388 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41

Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2





Tgt Ion:154 Resp: 25275

Ion Ratio Lower Upper

154 100

153 115.2 94.6 141.8

152 59.7 50.2 75.2

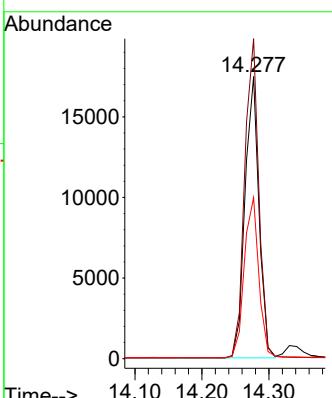

#18

Fluorene

Concen: 3.437 ng

RT: 15.271 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41


Tgt Ion:166 Resp: 36211


Ion Ratio Lower Upper

166 100

165 98.9 79.4 119.2

167 13.5 10.6 15.8

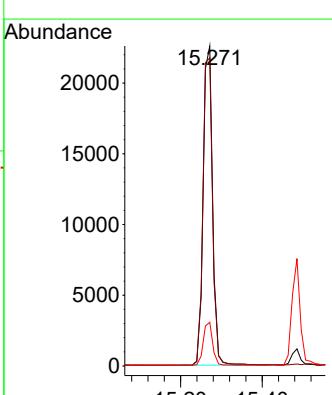

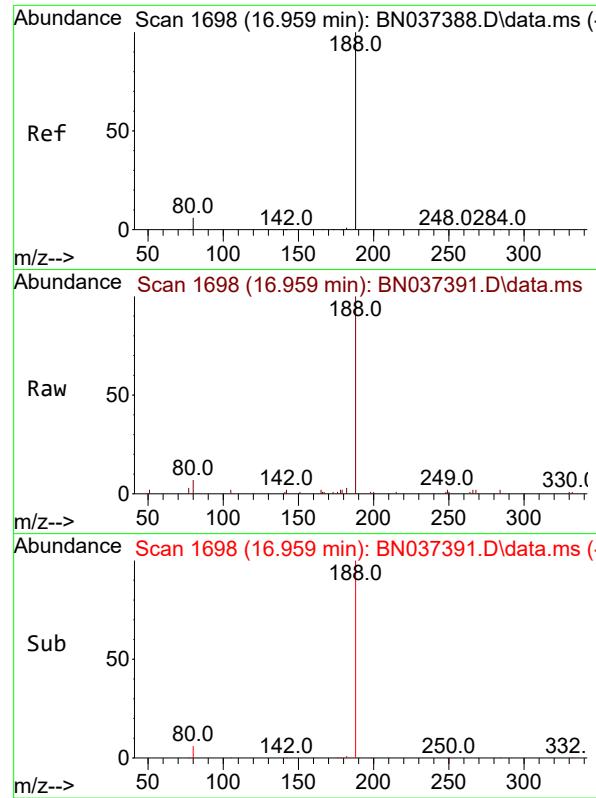

#19

Phenanthrene-d10  
Concen: 0.400 ng  
RT: 16.959 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41



Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2


Tgt Ion:188 Resp: 5771  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 7.4 6.2 9.4

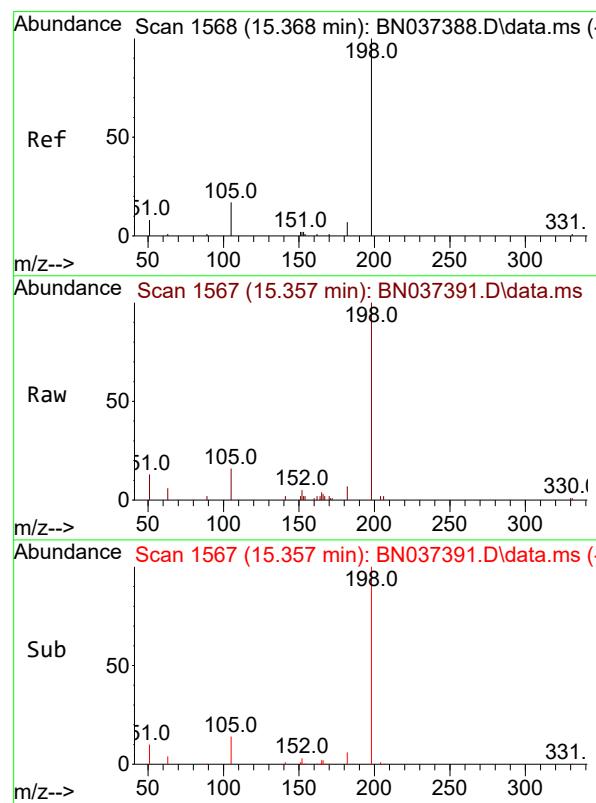


#20

4,6-Dinitro-2-methylphenol  
Concen: 3.696 ng  
RT: 15.357 min Scan# 1567  
Delta R.T. -0.011 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:198 Resp: 5478  
Ion Ratio Lower Upper  
198 100  
51 12.7 38.8 58.2#  
105 15.9 29.8 44.6#



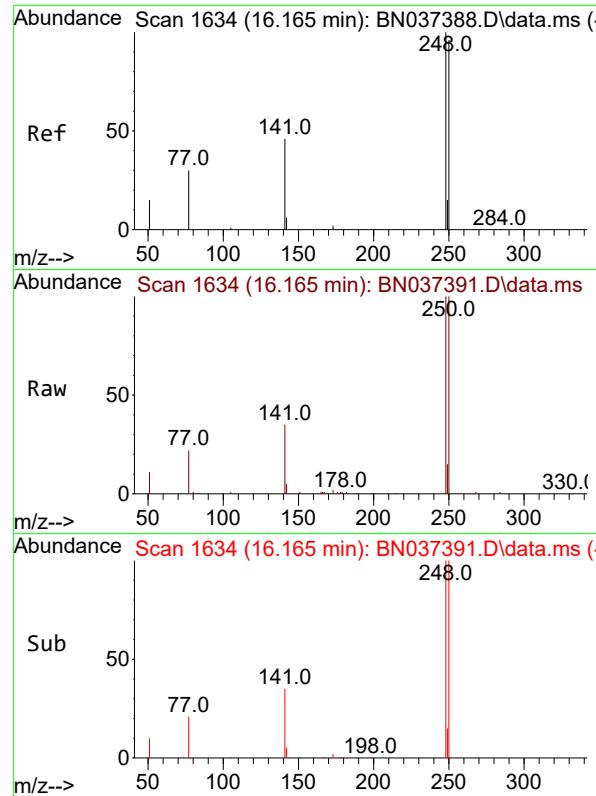

#21

4-Bromophenyl-phenylether

Concen: 3.427 ng

RT: 16.165 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41

Instrument:

BNA\_N

ClientSampleId :

SSTDICC3.2



Tgt Ion:248 Resp: 13953

Ion Ratio Lower Upper

248 100

250 99.6 77.0 115.4

141 35.0 38.7 58.1#

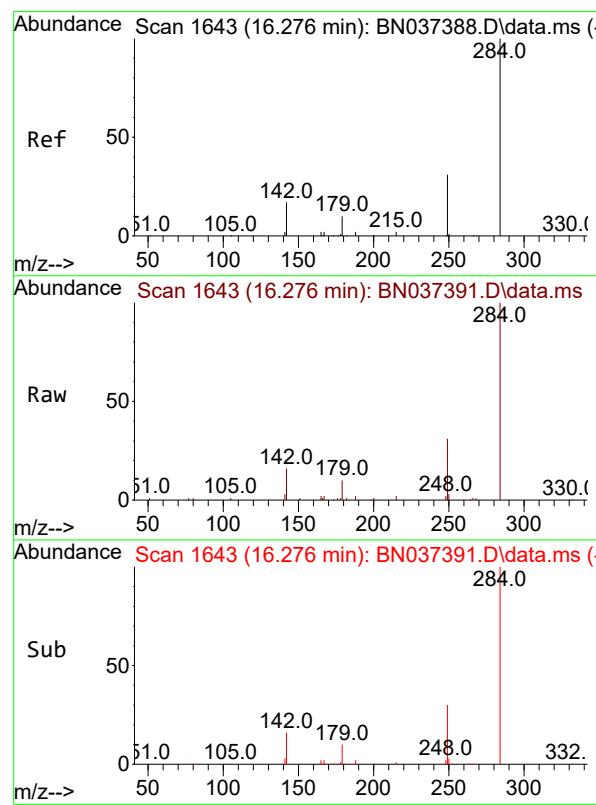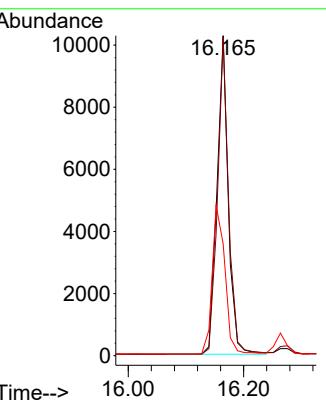

#22

Hexachlorobenzene

Concen: 3.171 ng

RT: 16.276 min Scan# 1643

Delta R.T. -0.000 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41


Tgt Ion:284 Resp: 13881


Ion Ratio Lower Upper

284 100

142 35.4 27.2 40.8

249 33.9 26.7 40.1


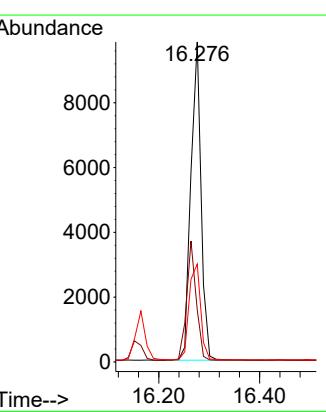


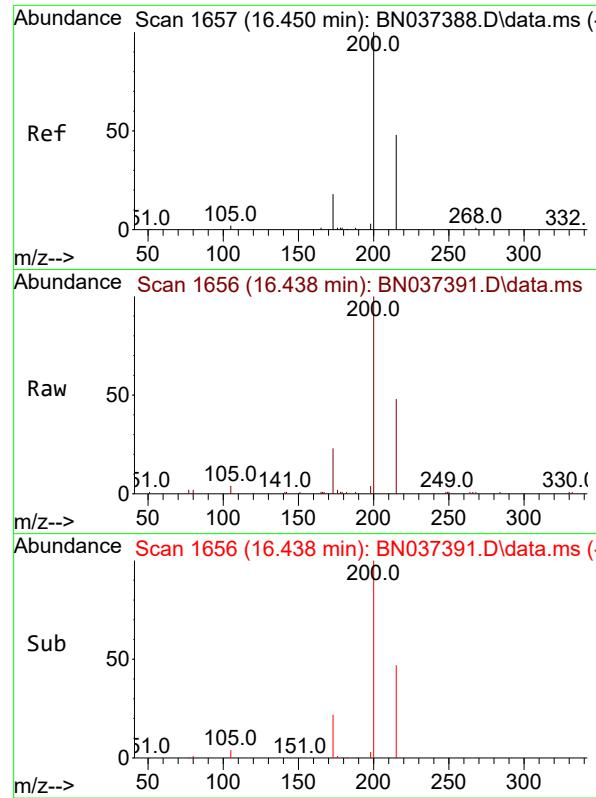

#23  
 Atrazine  
 Concen: 3.463 ng  
 RT: 16.438 min Scan# 1  
 Delta R.T. -0.012 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:200 Resp: 11170  
 Ion Ratio Lower Upper  
 200 100  
 173 22.8 19.0 28.6  
 215 48.1 41.3 61.9

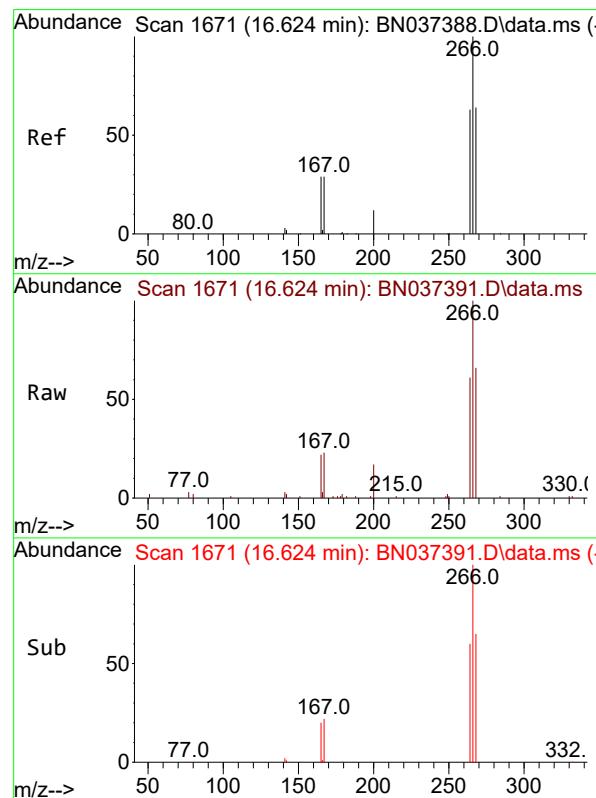

#24  
 Pentachlorophenol  
 Concen: 3.288 ng  
 RT: 16.624 min Scan# 1671  
 Delta R.T. -0.000 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41

Tgt Ion:266 Resp: 7774  
 Ion Ratio Lower Upper  
 266 100  
 264 62.4 49.2 73.8  
 268 63.6 54.2 81.4





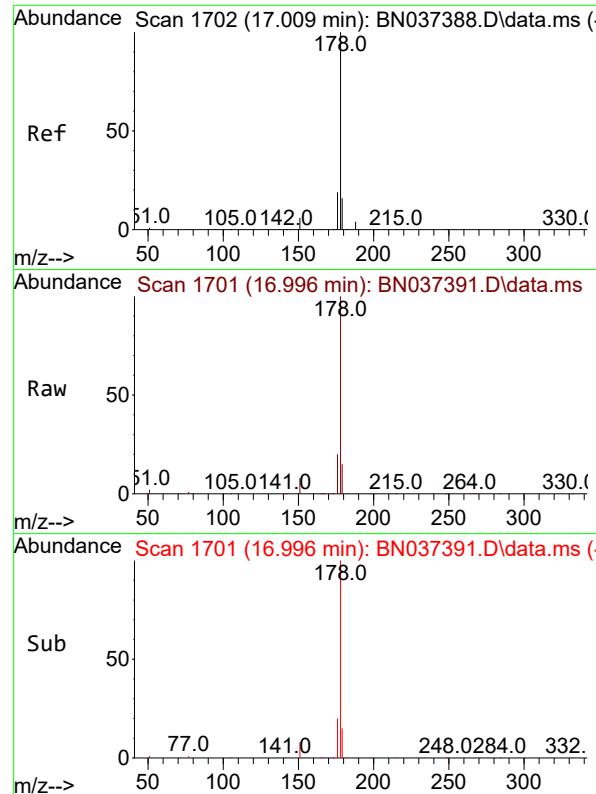

#25  
Phenanthrene  
Concen: 3.379 ng  
RT: 16.996 min Scan# 1  
Delta R.T. -0.012 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:178 Resp: 54938  
Ion Ratio Lower Upper  
178 100  
176 19.3 15.6 23.4  
179 15.3 12.8 19.2

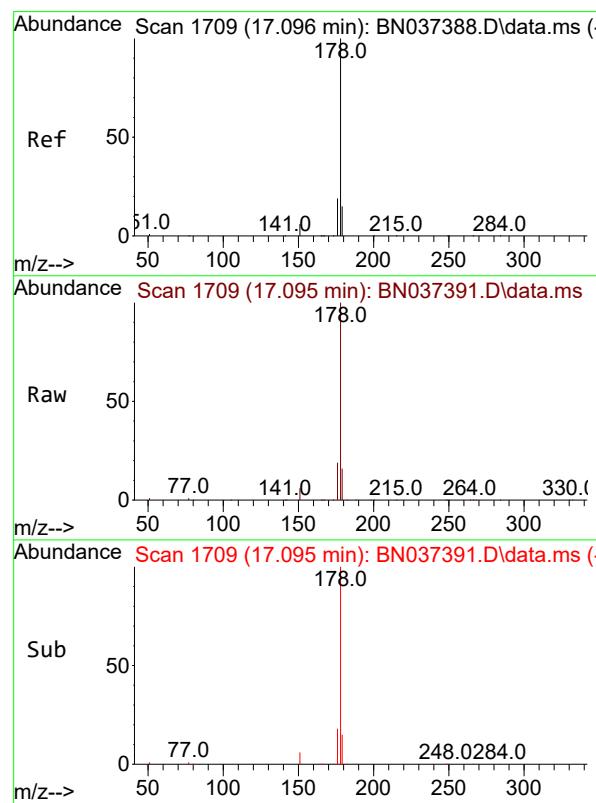

#26  
Anthracene  
Concen: 3.460 ng  
RT: 17.095 min Scan# 1709  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:178 Resp: 51719  
Ion Ratio Lower Upper  
178 100  
176 18.6 14.9 22.3  
179 15.3 12.4 18.6


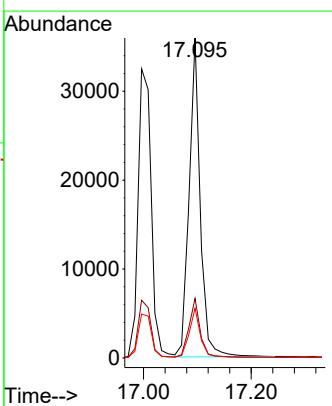


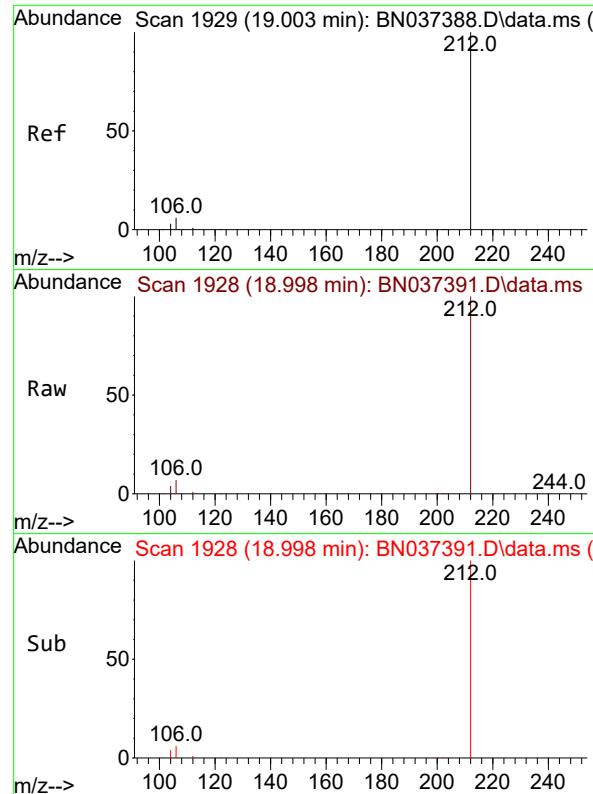

#27  
 Fluoranthene-d10  
 Concen: 3.221 ng  
 RT: 18.998 min Scan# 1  
 Delta R.T. -0.005 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:212 Resp: 53268  
 Ion Ratio Lower Upper  
 212 100  
 106 6.2 4.5 6.7  
 104 3.8 2.7 4.1

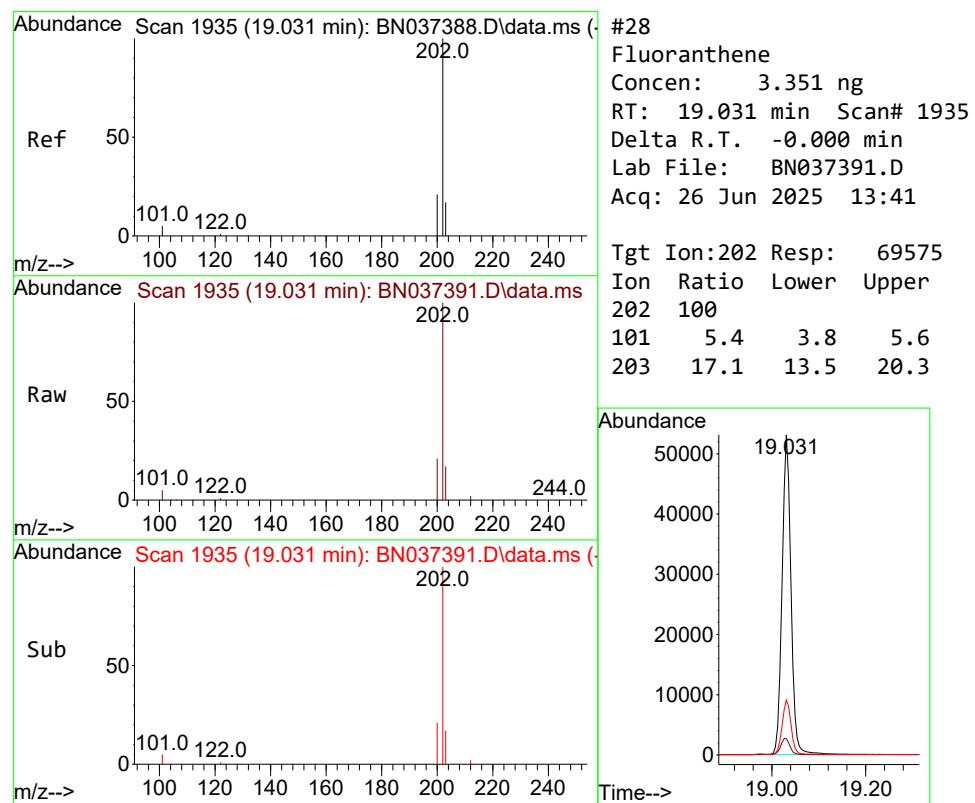

#28  
 Fluoranthene  
 Concen: 3.351 ng  
 RT: 19.031 min Scan# 1935  
 Delta R.T. -0.000 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41

Tgt Ion:202 Resp: 69575  
 Ion Ratio Lower Upper  
 202 100  
 101 5.4 3.8 5.6  
 203 17.1 13.5 20.3





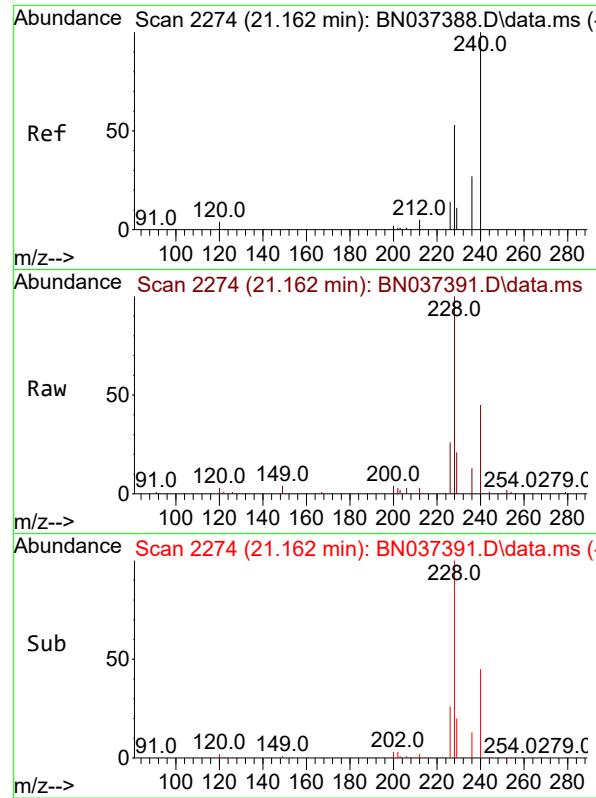

#29  
Chrysene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 21.162 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:240 Resp: 5566  
Ion Ratio Lower Upper  
240 100  
120 7.7 5.3 7.9  
236 29.4 22.7 34.1

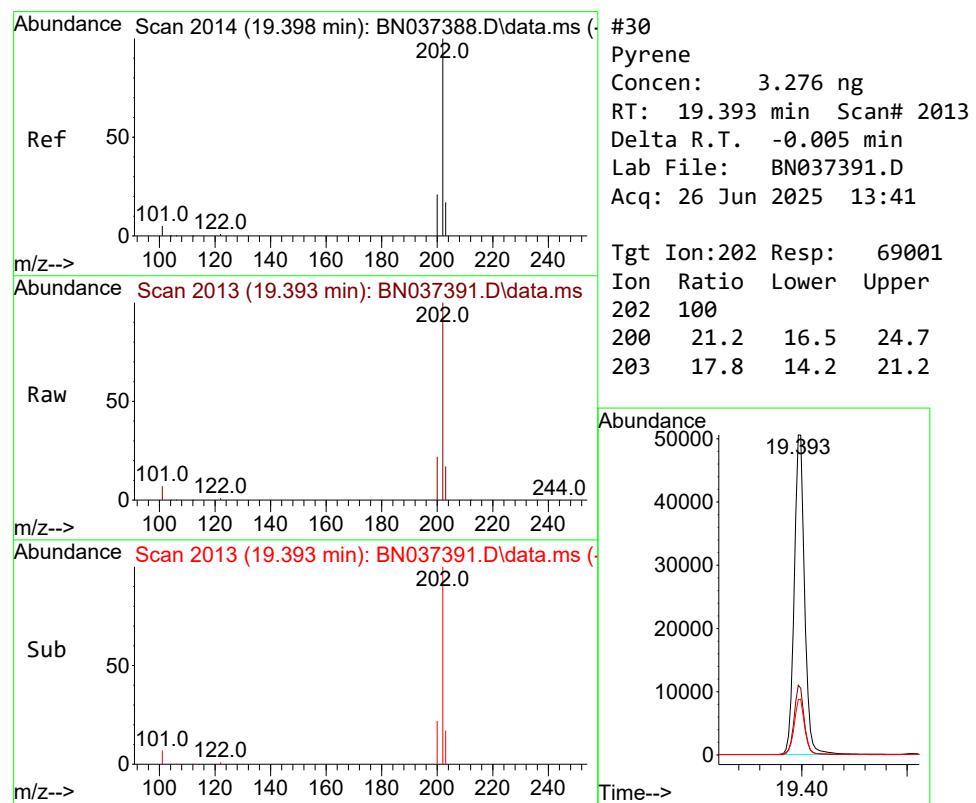

#30  
Pyrene  
Concen: 3.276 ng  
RT: 19.393 min Scan# 2013  
Delta R.T. -0.005 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:202 Resp: 69001  
Ion Ratio Lower Upper  
202 100  
200 21.2 16.5 24.7  
203 17.8 14.2 21.2





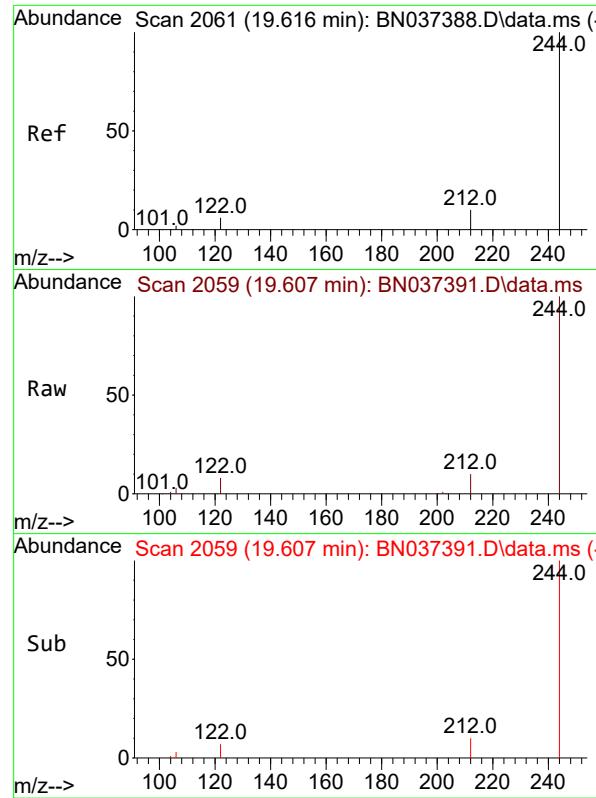

#31  
**Terphenyl-d14**  
Concen: 3.345 ng  
RT: 19.607 min Scan# 2  
Delta R.T. -0.009 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:244 Resp: 39701  
Ion Ratio Lower Upper  
244 100  
212 10.1 9.1 13.7  
122 7.7 6.3 9.5

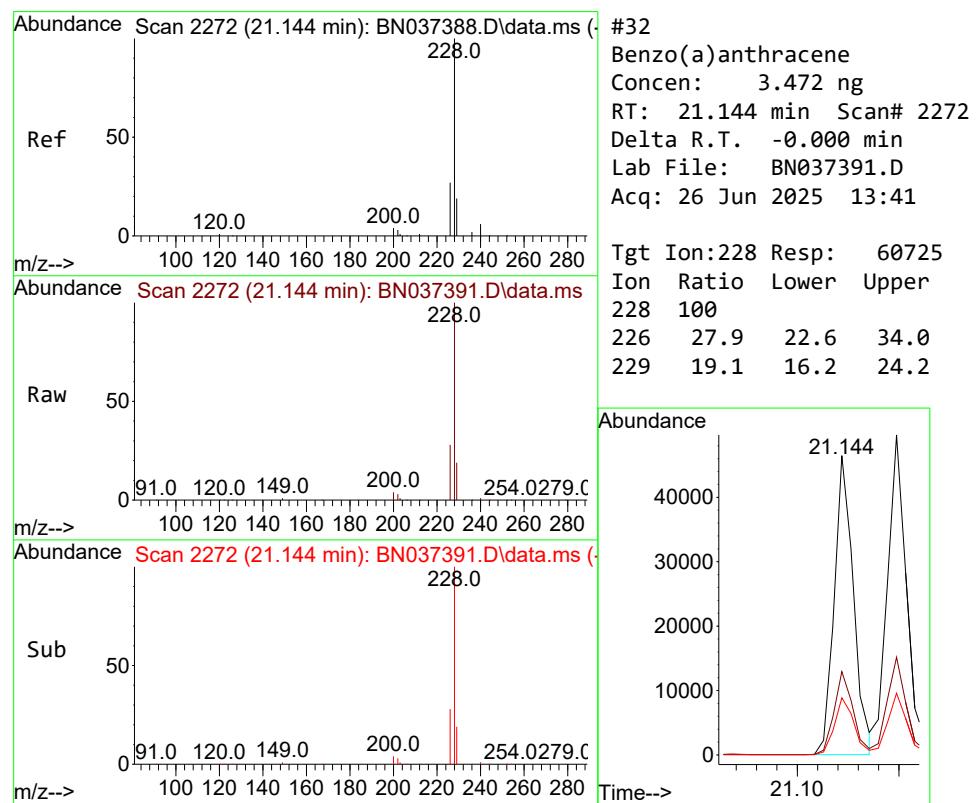

#32  
**Benzo(a)anthracene**  
Concen: 3.472 ng  
RT: 21.144 min Scan# 2272  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:228 Resp: 60725  
Ion Ratio Lower Upper  
228 100  
226 27.9 22.6 34.0  
229 19.1 16.2 24.2





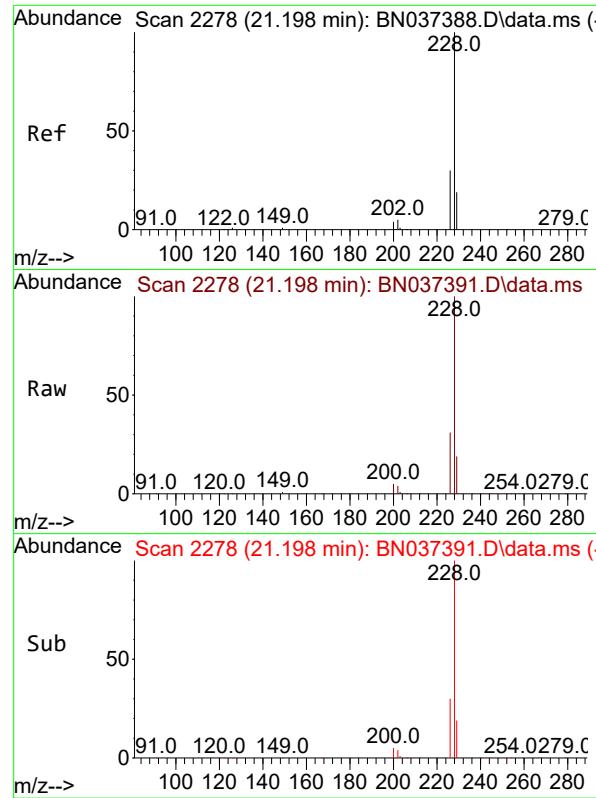

#33  
Chrysene  
Concen: 3.106 ng  
RT: 21.198 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
ClientSampleId : SSTDICC3.2


Tgt Ion:228 Resp: 67241  
Ion Ratio Lower Upper  
228 100  
226 30.5 24.5 36.7  
229 19.3 16.1 24.1

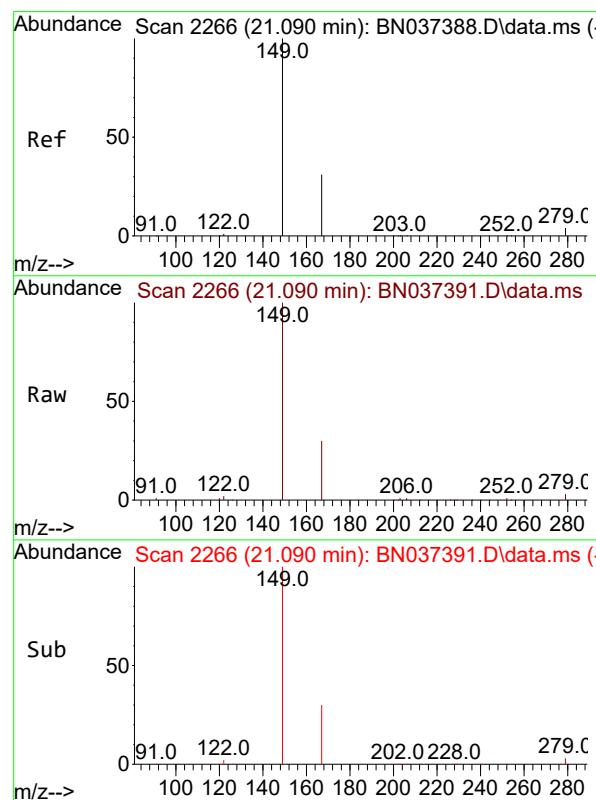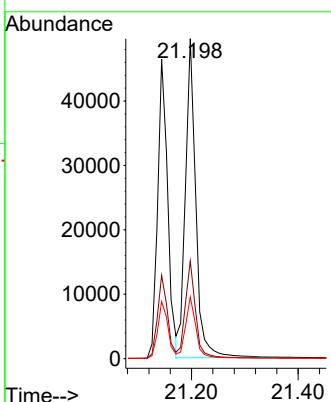

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 3.139 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. -0.000 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Tgt Ion:149 Resp: 21735  
Ion Ratio Lower Upper  
149 100  
167 31.0 24.8 37.2  
279 5.5 5.0 7.6





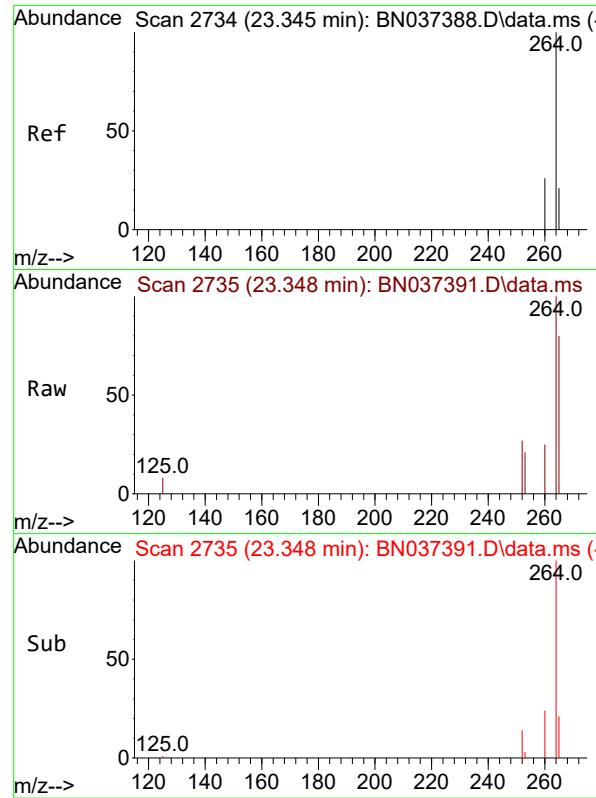

#35  
 Perylene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 23.348 min Scan# 2  
 Delta R.T. 0.003 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:264 Resp: 5442  
 Ion Ratio Lower Upper  
 264 100  
 260 25.2 21.4 32.0  
 265 79.8 56.2 84.4

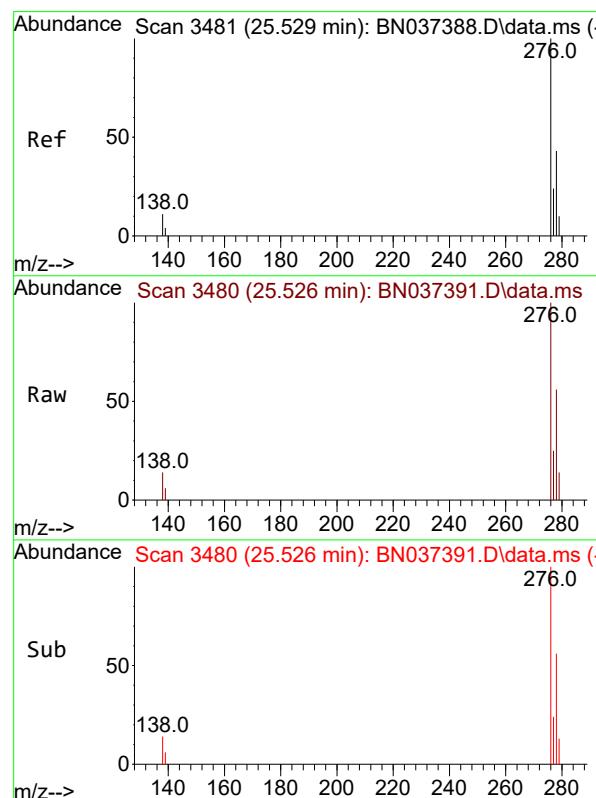

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 3.517 ng  
 RT: 25.526 min Scan# 3480  
 Delta R.T. -0.003 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41

Tgt Ion:276 Resp: 80692  
 Ion Ratio Lower Upper  
 276 100  
 138 14.3 8.5 12.7#  
 277 24.7 19.7 29.5



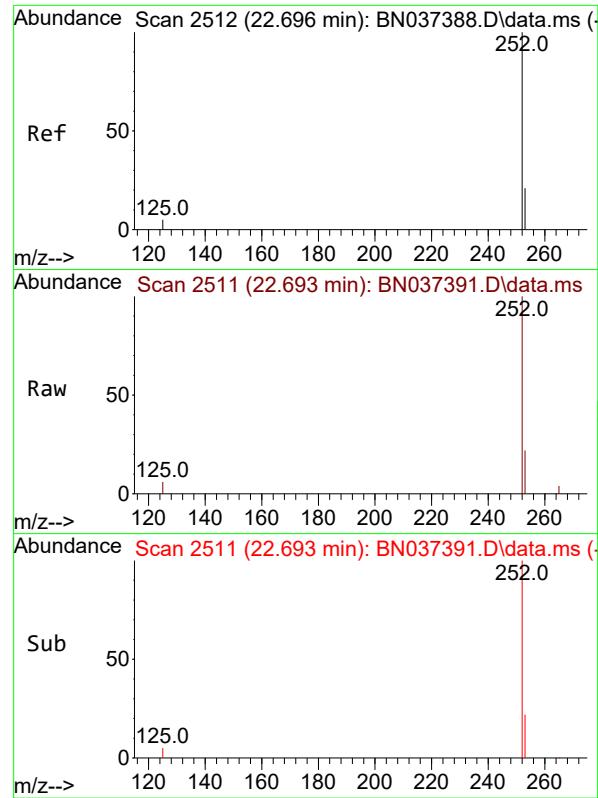

#37

Benzo(b)fluoranthene

Concen: 3.412 ng

RT: 22.693 min Scan# 2

Delta R.T. -0.003 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41

Instrument :

BNA\_N

ClientSampleId :

SSTDICC3.2



Tgt Ion:252 Resp: 65471

Ion Ratio Lower Upper

252 100

253 22.4 22.8 34.2#

125 5.6 6.2 9.4#

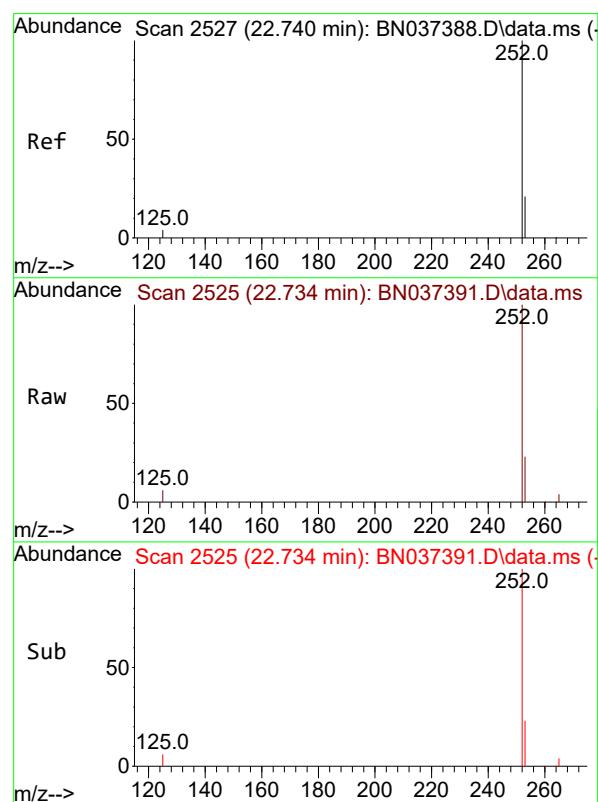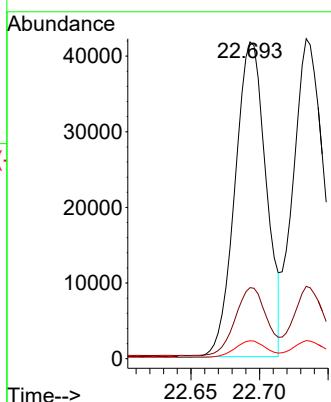

#38

Benzo(k)fluoranthene

Concen: 3.425 ng

RT: 22.734 min Scan# 2525

Delta R.T. -0.006 min

Lab File: BN037391.D

Acq: 26 Jun 2025 13:41


Tgt Ion:252 Resp: 70234


Ion Ratio Lower Upper

252 100

253 22.6 23.2 34.8#

125 5.6 6.0 9.0#





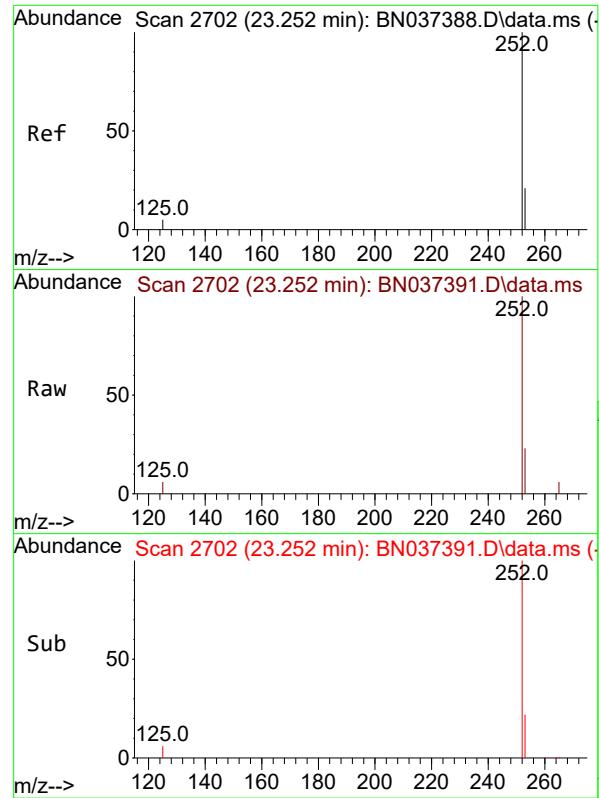

#39  
 Benzo(a)pyrene  
 Concen: 3.422 ng  
 RT: 23.252 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICC3.2


Tgt Ion:252 Resp: 58393  
 Ion Ratio Lower Upper  
 252 100  
 253 23.1 25.6 38.4#  
 125 6.3 7.5 11.3#

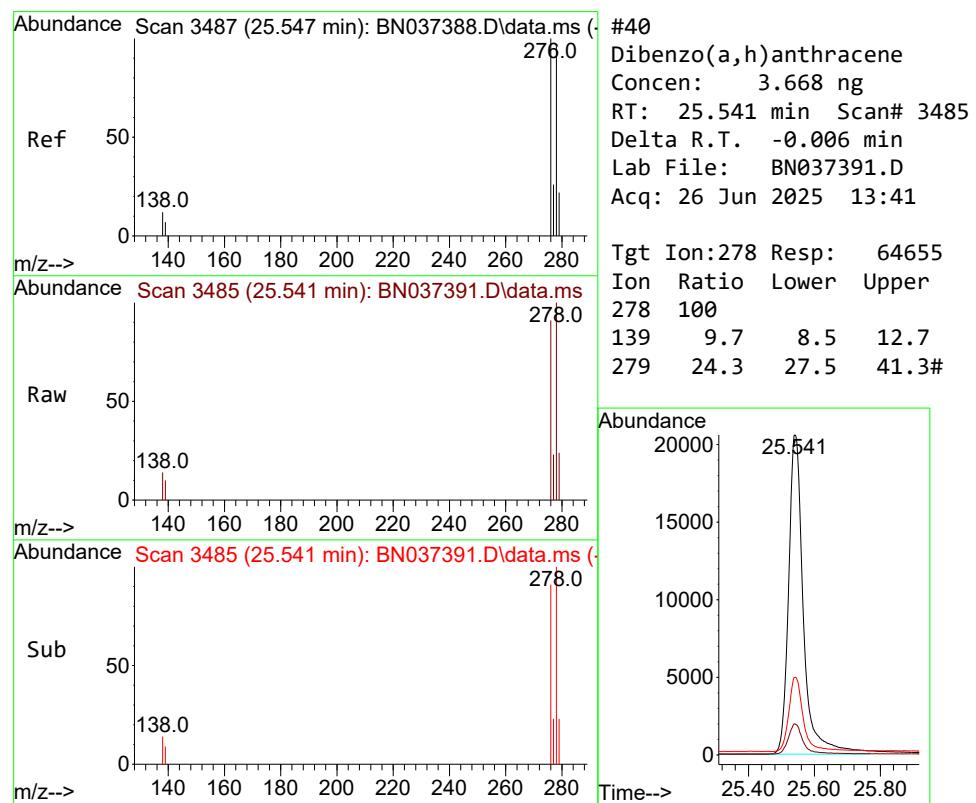

#40  
 Dibenzo(a,h)anthracene  
 Concen: 3.668 ng  
 RT: 25.541 min Scan# 3485  
 Delta R.T. -0.006 min  
 Lab File: BN037391.D  
 Acq: 26 Jun 2025 13:41

Tgt Ion:278 Resp: 64655  
 Ion Ratio Lower Upper  
 278 100  
 139 9.7 8.5 12.7  
 279 24.3 27.5 41.3#




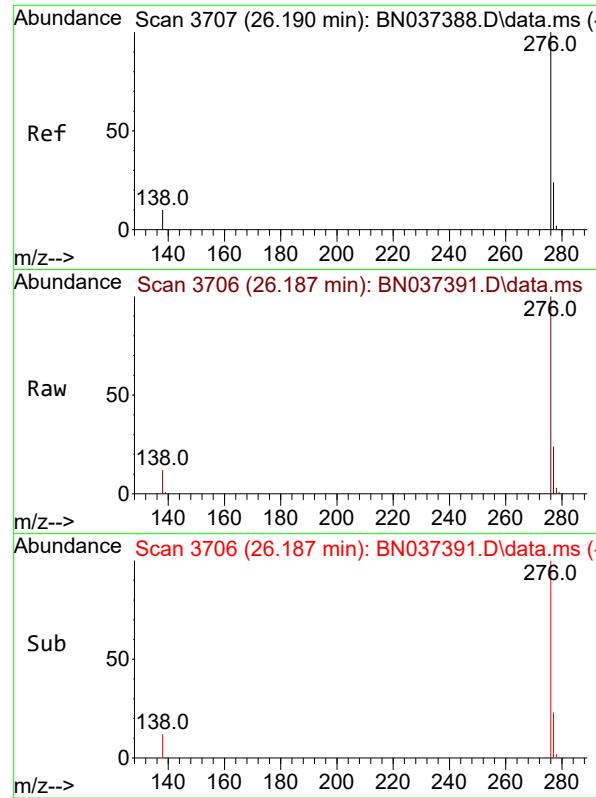

#41  
Benzo(g,h,i)perylene  
Concen: 3.427 ng  
RT: 26.187 min Scan# 3  
Delta R.T. -0.003 min  
Lab File: BN037391.D  
Acq: 26 Jun 2025 13:41

Instrument :  
BNA\_N  
ClientSampleId :  
SSTDICC3.2

Tgt Ion:276 Resp: 72186  
Ion Ratio Lower Upper  
276 100  
277 23.6 21.0 31.4  
138 12.4 9.6 14.4



Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037392.D  
 Acq On : 26 Jun 2025 14:17  
 Operator : RC/JU  
 Sample : SSTDICC5.0  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC5.0

Quant Time: Jun 26 14:45:42 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.560	152	2311	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4753	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	3216	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	6554	0.400	ng	0.00
29) Chrysene-d12	21.162	240	6601	0.400	ng	0.00
35) Perylene-d12	23.345	264	6264	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	23643	5.308	ng	0.00
5) Phenol-d6	6.744	99	27480	5.950	ng	0.00
8) Nitrobenzene-d5	8.706	82	23095	6.041	ng	-0.01
11) 2-Methylnaphthalene-d10	11.935	152	47934	6.519	ng	0.00
14) 2,4,6-Tribromophenol	15.705	330	10881	5.768	ng	-0.01
15) 2-Fluorobiphenyl	12.833	172	76771	5.529	ng	0.00
27) Fluoranthene-d10	19.003	212	118571	6.313	ng	0.00
31) Terphenyl-d14	19.607	244	77795	5.527	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.097	88	9566	4.619	ng	95
3) n-Nitrosodimethylamine	3.408	42	10726	4.955	ng	# 90
6) bis(2-Chloroethyl)ether	6.997	93	22819	5.555	ng	96
9) Naphthalene	10.383	128	65119	5.322	ng	96
10) Hexachlorobutadiene	10.682	225	24052	4.952	ng	# 99
12) 2-Methylnaphthalene	12.011	142	47716	5.664	ng	96
16) Acenaphthylene	13.924	152	74682	5.600	ng	99
17) Acenaphthene	14.277	154	48364	5.553	ng	96
18) Fluorene	15.271	166	68578	5.576	ng	99
20) 4,6-Dinitro-2-methylph...	15.357	198	10525	6.252	ng	# 54
21) 4-Bromophenyl-phenylether	16.164	248	25866	5.594	ng	# 93
22) Hexachlorobenzene	16.276	284	25453	5.120	ng	98
23) Atrazine	16.437	200	21783	5.947	ng	95
24) Pentachlorophenol	16.624	266	14964	5.574	ng	96
25) Phenanthrene	16.996	178	105409	5.708	ng	99
26) Anthracene	17.095	178	100113	5.897	ng	100
28) Fluoranthene	19.031	202	133030	5.641	ng	# 99
30) Pyrene	19.393	202	132986	5.324	ng	99
32) Benzo(a)anthracene	21.144	228	119334	5.754	ng	99
33) Chrysene	21.197	228	127936	4.982	ng	99
34) Bis(2-ethylhexyl)phtha...	21.090	149	44321	5.397	ng	# 99
36) Indeno(1,2,3-cd)pyrene	25.523	276	154039	5.833	ng	# 96
37) Benzo(b)fluoranthene	22.693	252	127810	5.787	ng	# 90
38) Benzo(k)fluoranthene	22.737	252	132887	5.630	ng	# 89
39) Benzo(a)pyrene	23.248	252	111691	5.686	ng	# 85
40) Dibenzo(a,h)anthracene	25.538	278	122232	6.025	ng	# 86
41) Benzo(g,h,i)perylene	26.190	276	135052	5.570	ng	95


(#) = qualifier out of range (#) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037392.D  
 Acq On : 26 Jun 2025 14:17  
 Operator : RC/JU  
 Sample : SSTDICC5.0  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC5.0

Quant Time: Jun 26 14:45:42 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 14:40:13 2025  
 Response via : Initial Calibration


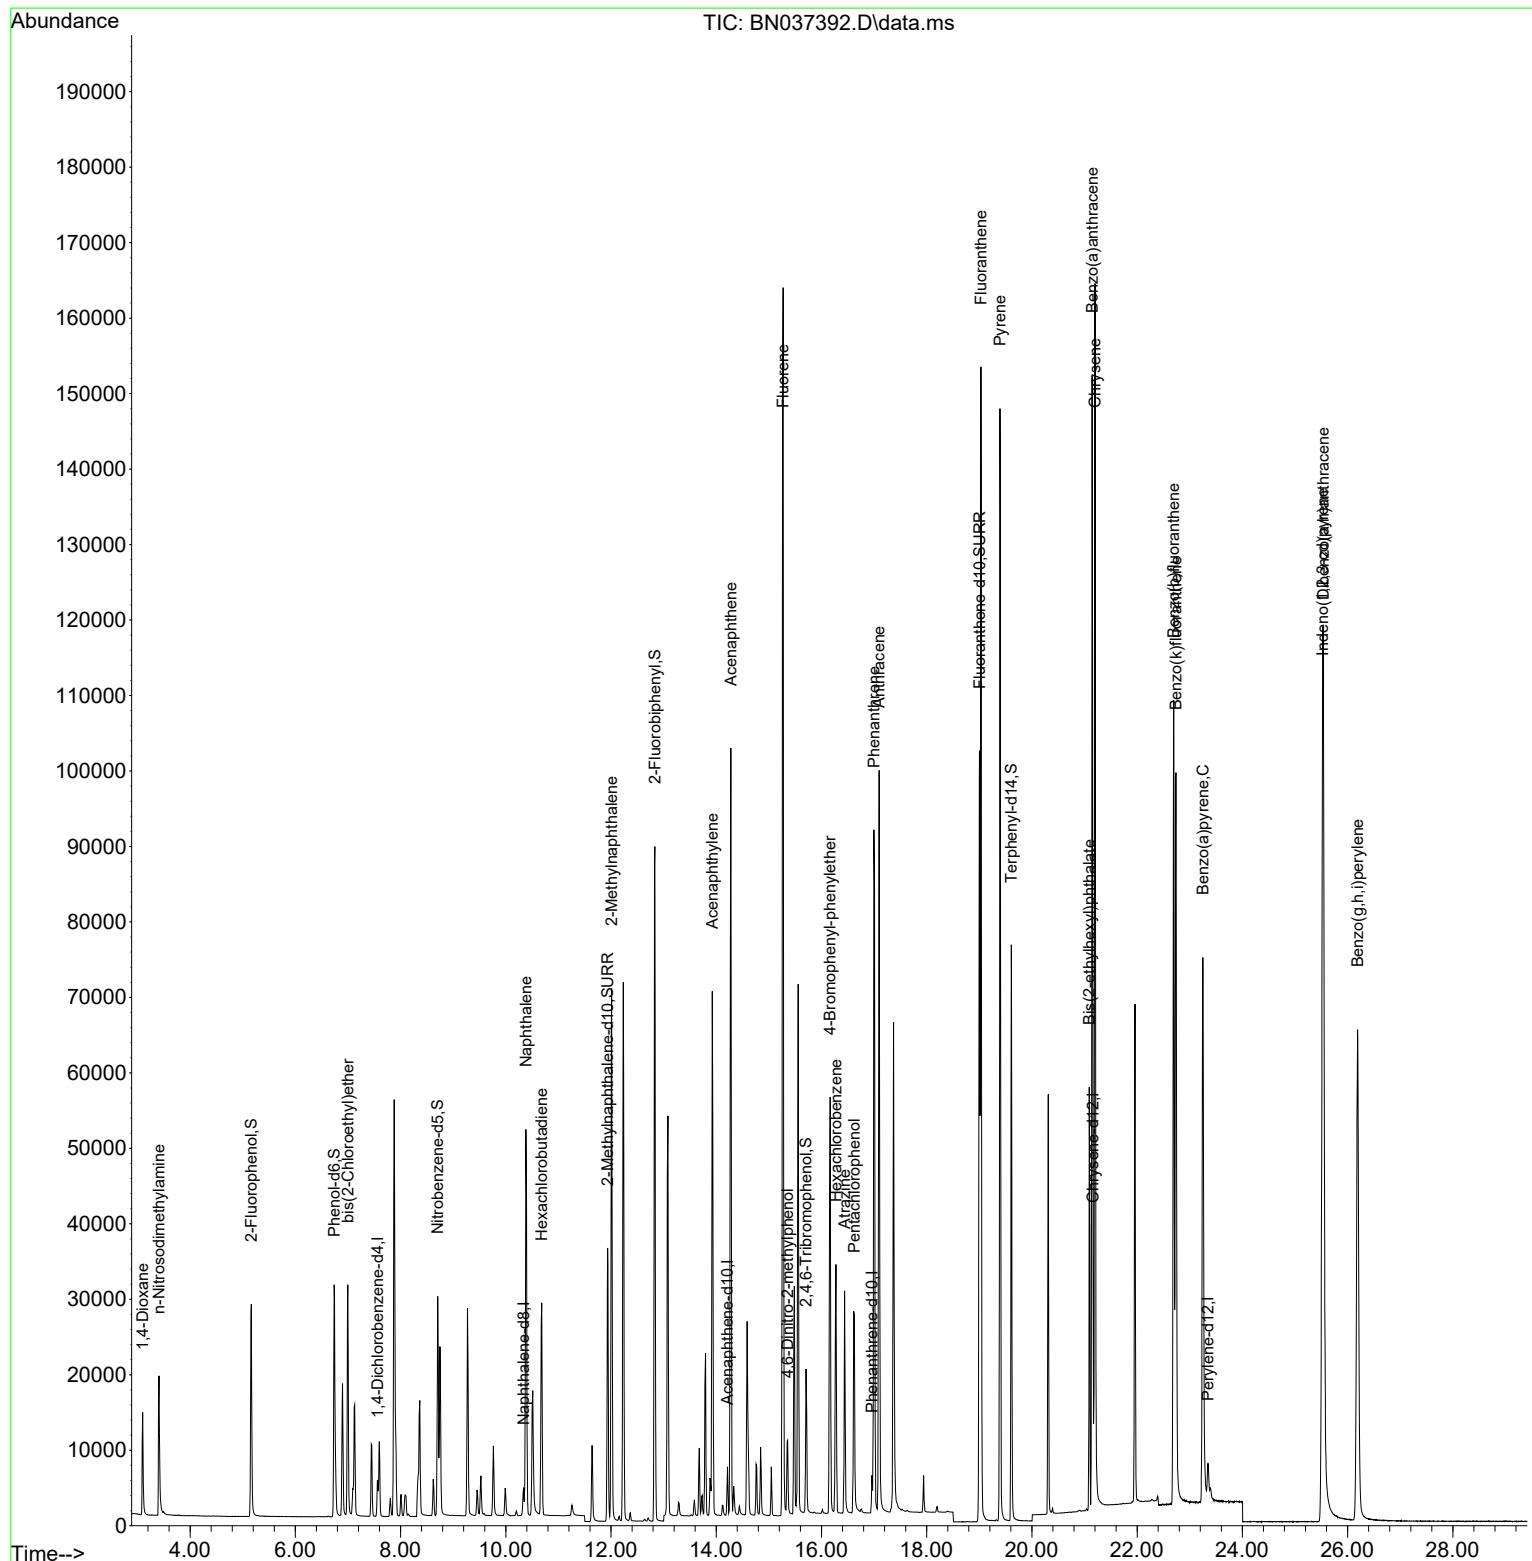


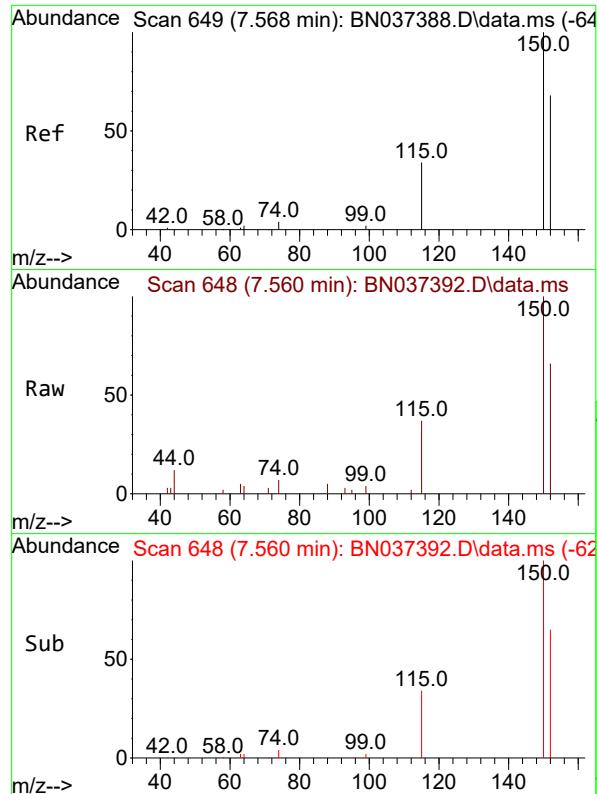

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.560 min Scan# 6  
Delta R.T. -0.008 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0


Tgt Ion:152 Resp: 2311  
Ion Ratio Lower Upper  
152 100  
150 152.5 116.2 174.2  
115 56.0 42.9 64.3

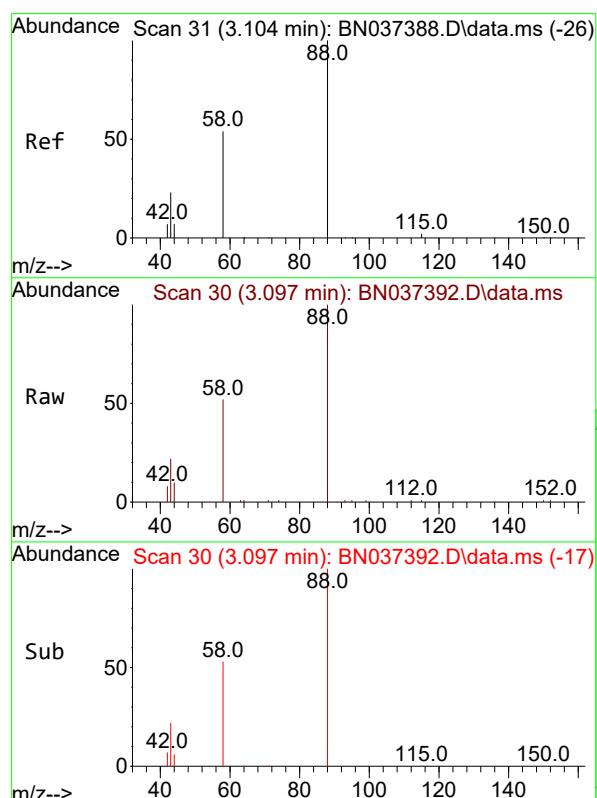

#2  
1,4-Dioxane  
Concen: 4.619 ng  
RT: 3.097 min Scan# 30  
Delta R.T. -0.007 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17



Tgt Ion: 88 Resp: 9566  
Ion Ratio Lower Upper  
88 100  
43 23.1 21.6 32.4  
58 54.1 45.9 68.9



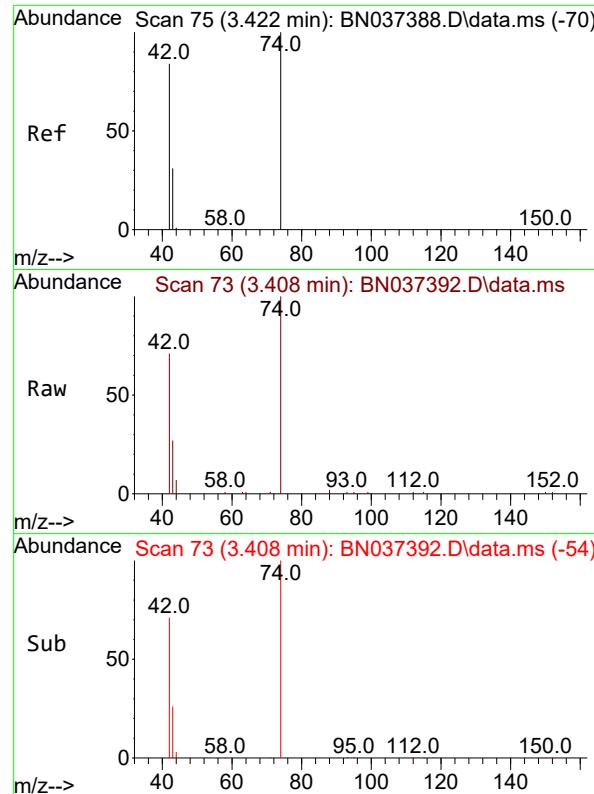


#3  
n-Nitrosodimethylamine  
Concen: 4.955 ng  
RT: 3.408 min Scan# 7  
Instrument : BNA\_N  
Delta R.T. -0.015 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17  
ClientSampleId : SSTDICC5.0


Tgt Ion: 42 Resp: 10726  
Ion Ratio Lower Upper  
42 100  
74 133.1 97.8 146.8  
44 4.5 8.7 13.1#

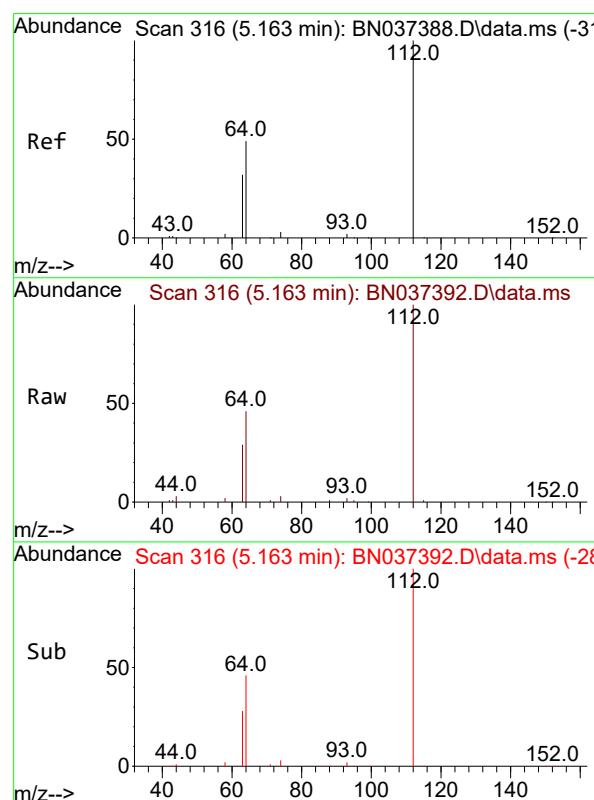

#4  
2-Fluorophenol  
Concen: 5.308 ng  
RT: 5.163 min Scan# 316  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17


Tgt Ion:112 Resp: 23643  
Ion Ratio Lower Upper  
112 100  
64 50.8 40.3 60.5  
63 31.8 26.1 39.1

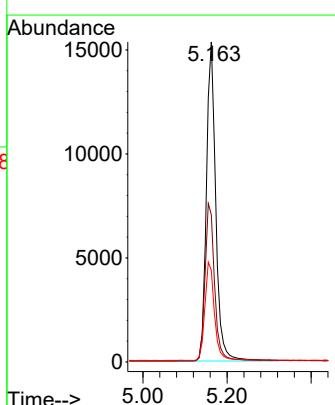





#5  
Phenol-d6  
Concen: 5.950 ng  
RT: 6.744 min Scan# 5  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0





Tgt Ion: 99 Resp: 27480  
Ion Ratio Lower Upper  
99 100  
42 18.2 15.6 23.4  
71 44.1 35.8 53.8

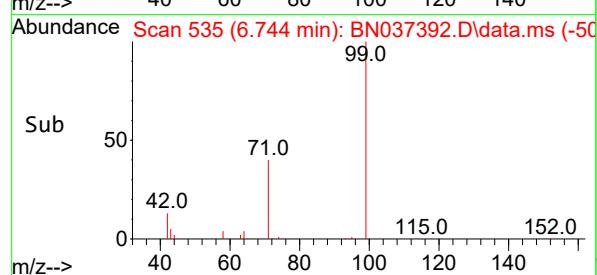


#6  
bis(2-Chloroethyl)ether  
Concen: 5.555 ng  
RT: 6.997 min Scan# 570  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17

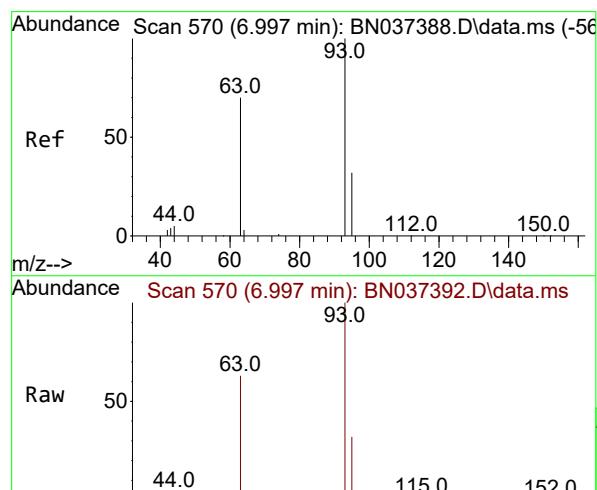


Tgt Ion: 93 Resp: 22819  
Ion Ratio Lower Upper  
93 100  
63 65.3 49.6 74.4  
95 31.7 23.9 35.9

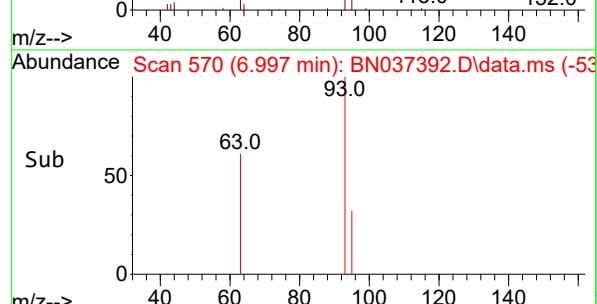





#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0






Tgt Ion:136 Resp: 4753  
 Ion Ratio Lower Upper  
 136 100  
 137 12.1 10.4 15.6  
 54 6.3 5.6 8.4  
 68 5.3 4.6 6.8



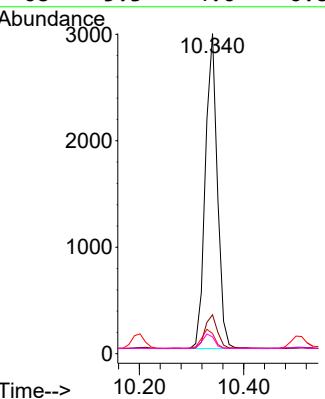


#8  
 Nitrobenzene-d5  
 Concen: 6.041 ng  
 RT: 8.706 min Scan# 789  
 Delta R.T. -0.011 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17



Tgt Ion: 82 Resp: 23095  
 Ion Ratio Lower Upper  
 82 100  
 128 35.9 34.0 51.0  
 54 41.9 37.7 56.5

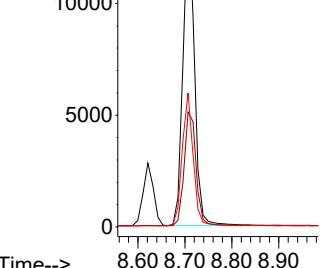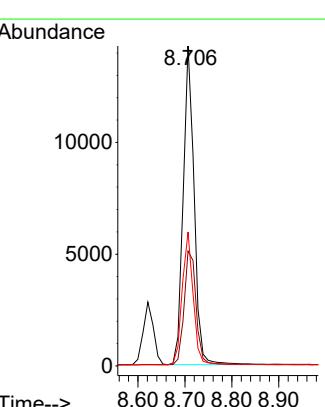



#9

Naphthalene

Concen: 5.322 ng

RT: 10.383 min Scan# 9

Delta R.T. -0.011 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0

Tgt Ion:128 Resp: 65119

Ion Ratio Lower Upper

128 100

129 10.8 10.4 15.6

127 13.8 12.2 18.4

Abundance

10.383

30000




20000

10000

0

Time--&gt;

10.30 10.40 10.50

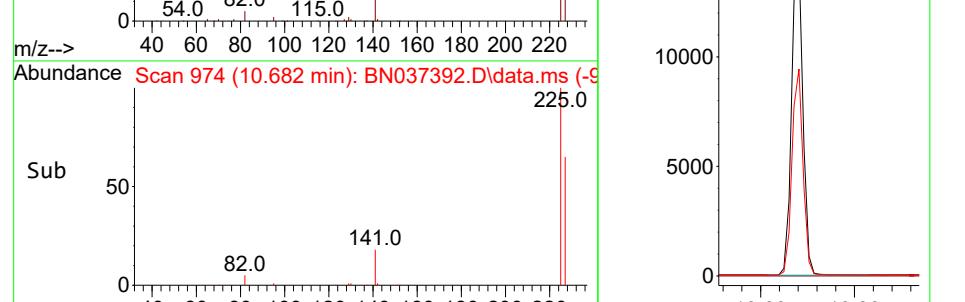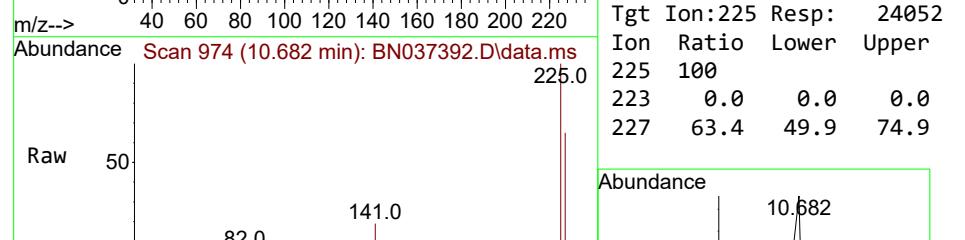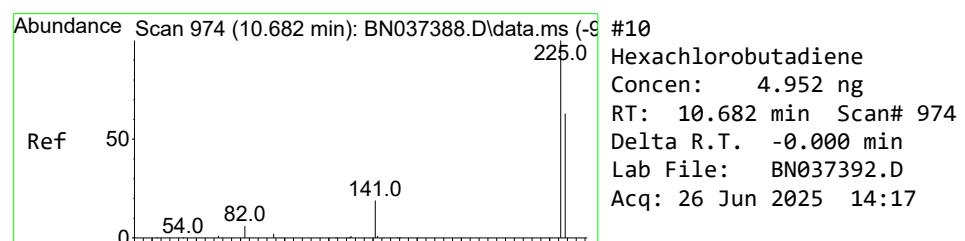

#10

Hexachlorobutadiene

Concen: 4.952 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Tgt Ion:225 Resp: 24052

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.4 49.9 74.9

Abundance

10.682


10000

5000


0

Time--&gt;

10.60 10.70 10.80



Abundance Scan 1136 (11.935 min): BN037392.D\data.ms (-)

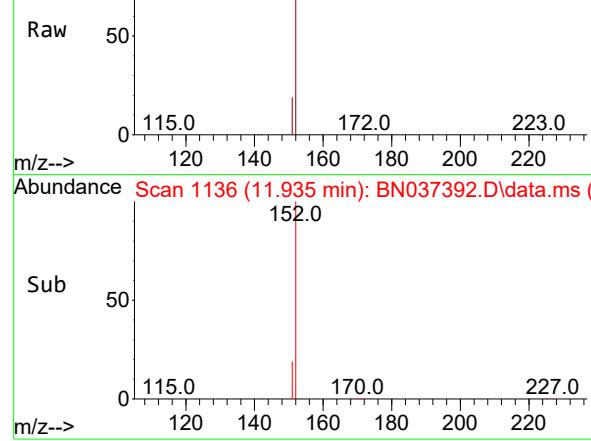

#11

2-Methylnaphthalene-d10

Concen: 6.519 ng

RT: 11.935 min Scan# 1136

Delta R.T. -0.005 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0

Tgt Ion:152 Resp: 47934



Ion Ratio Lower Upper

152 100


151 21.4 18.4 27.6

Abundance 30000  
20000  
10000  
0

11.935

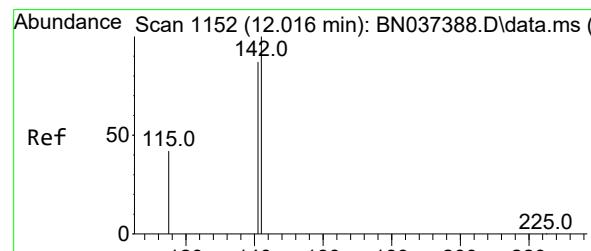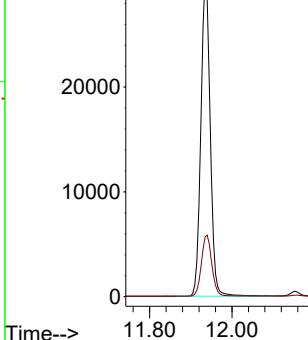

Abundance Scan 1151 (12.011 min): BN037392.D\data.ms (-)

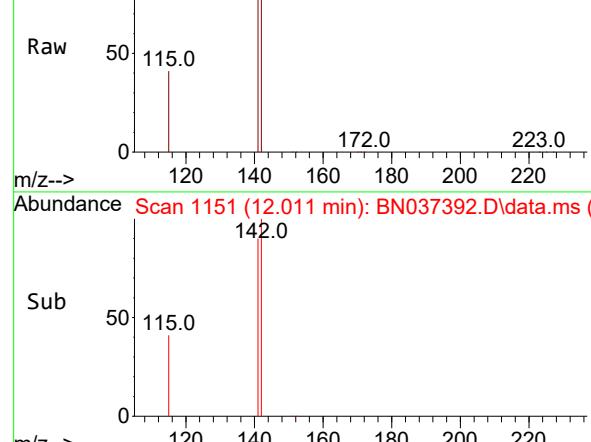

#12

2-Methylnaphthalene

Concen: 5.664 ng

RT: 12.011 min Scan# 1151

Delta R.T. -0.005 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Tgt Ion:142 Resp: 47716

Ion Ratio Lower Upper


142 100


141 89.7 70.1 105.1

115 40.7 35.8 53.6

Abundance 30000  
20000  
10000  
0

12.011


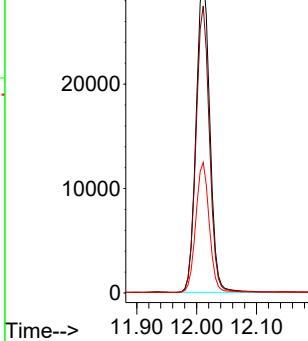


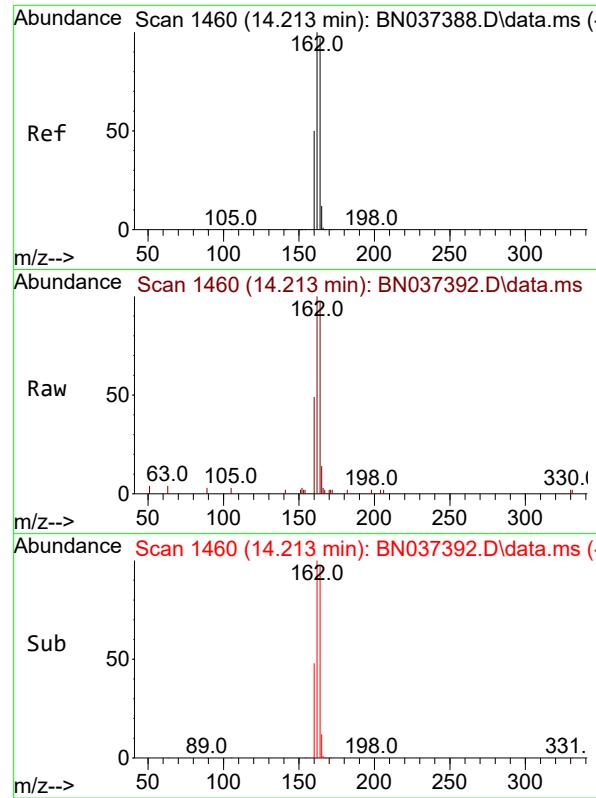

#13

Acenaphthene-d10  
Concen: 0.400 ngRT: 14.213 min Scan# 14  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17Instrument :  
BNA\_N  
ClientSampleId :  
SSTDICC5.0


Tgt Ion:164 Resp: 3216

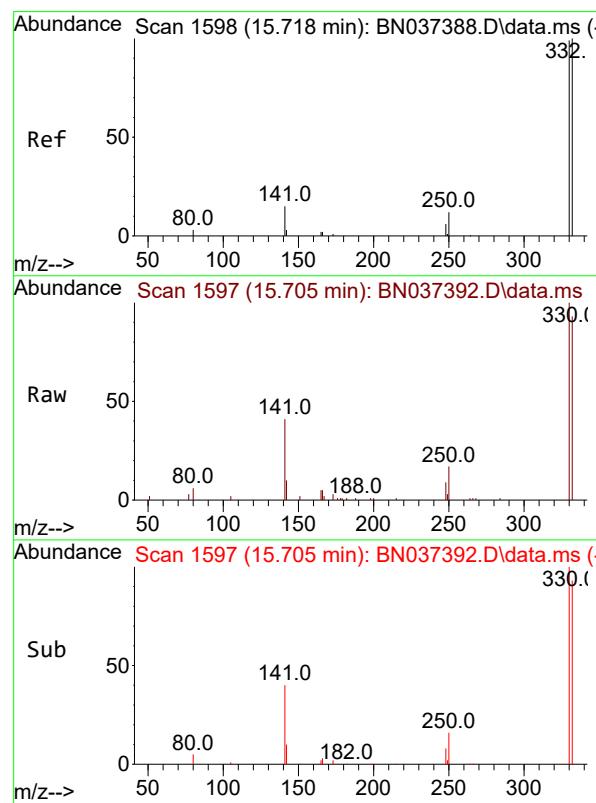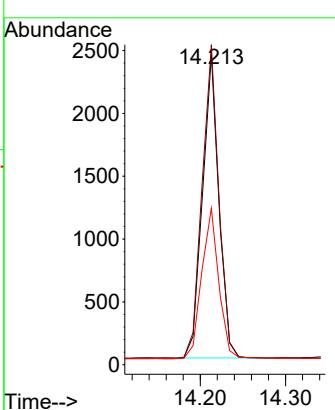
Ion Ratio Lower Upper  
164 100  
162 103.1 82.6 123.8  
160 50.4 42.2 63.2

#14

2,4,6-Tribromophenol  
Concen: 5.768 ng  
RT: 15.705 min Scan# 1597  
Delta R.T. -0.013 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17

Tgt Ion:330 Resp: 10881


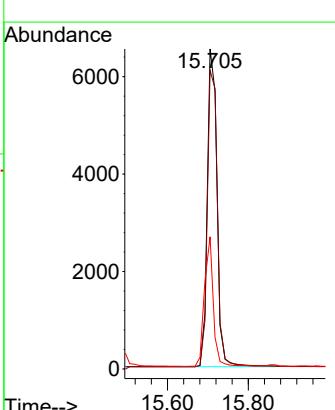
Ion Ratio Lower Upper  
330 100  
332 96.8 77.8 116.8  
141 37.2 24.0 36.0#

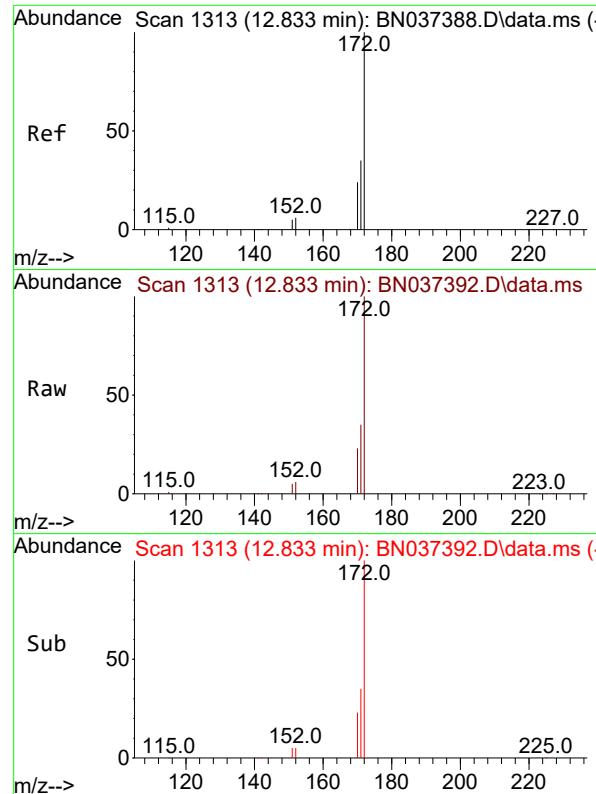

#15  
2-Fluorobiphenyl  
Concen: 5.529 ng  
RT: 12.833 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0




Tgt Ion:172 Resp: 76771  
Ion Ratio Lower Upper  
172 100  
171 35.3 28.8 43.2  
170 23.2 20.3 30.5

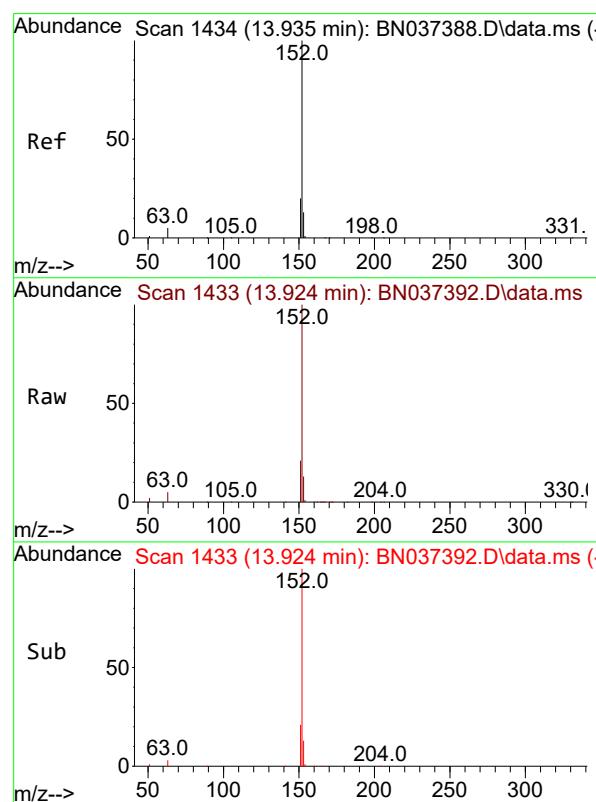

#16  
Acenaphthylene  
Concen: 5.600 ng  
RT: 13.924 min Scan# 1433  
Delta R.T. -0.011 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17

Tgt Ion:152 Resp: 74682  
Ion Ratio Lower Upper  
152 100  
151 19.9 15.8 23.6  
153 13.1 10.3 15.5





#17

Acenaphthene

Concen: 5.553 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:154 Resp: 48364

Ion Ratio Lower Upper

154 100

153 115.1 94.6 141.8

152 58.6 50.2 75.2

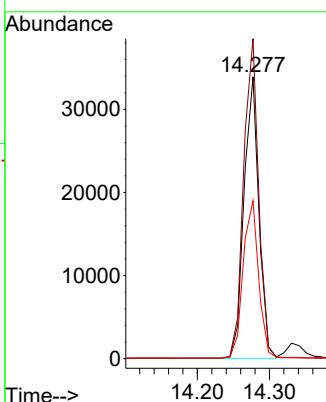

#18

Fluorene

Concen: 5.576 ng

RT: 15.271 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17


Tgt Ion:166 Resp: 68578


Ion Ratio Lower Upper

166 100



165 98.3 79.4 119.2

167 13.4 10.6 15.8

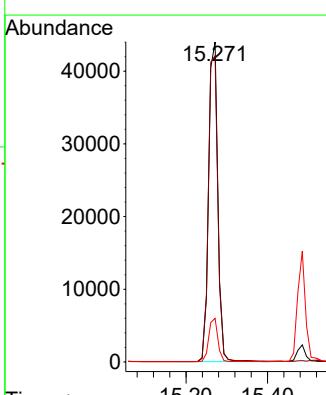


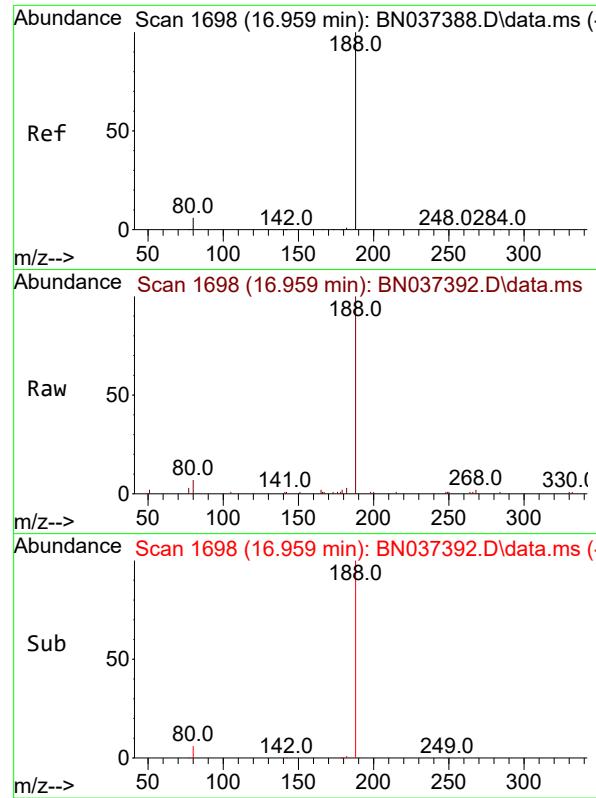


#19

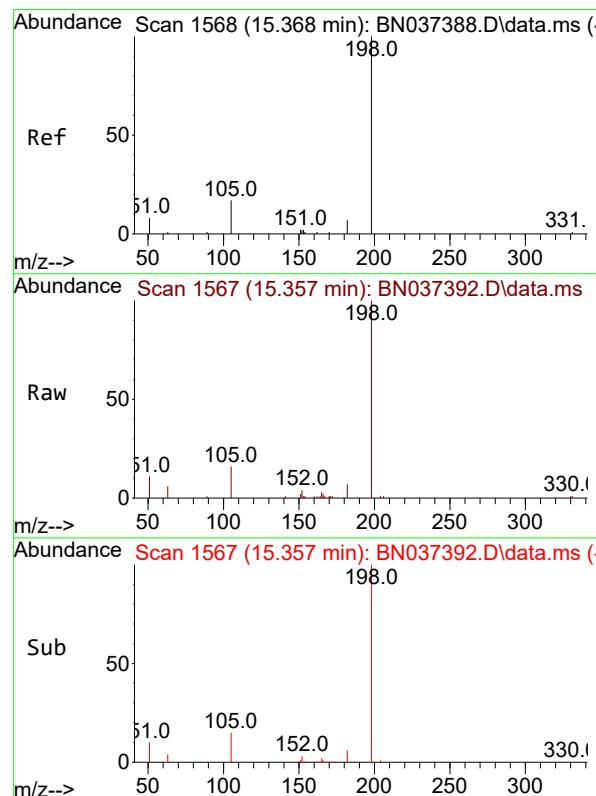Phenanthrene-d10  
Concen: 0.400 ngRT: 16.959 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17Instrument :  
BNA\_N  
ClientSampleId :  
SSTDICC5.0Tgt Ion:188 Resp: 6554  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 7.4 6.2 9.4

#20

4,6-Dinitro-2-methylphenol  
Concen: 6.252 ng  
RT: 15.357 min Scan# 1567  
Delta R.T. -0.011 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17Tgt Ion:198 Resp: 10525  
Ion Ratio Lower Upper  
198 100  
51 11.4 38.8 58.2#  
105 15.8 29.8 44.6#

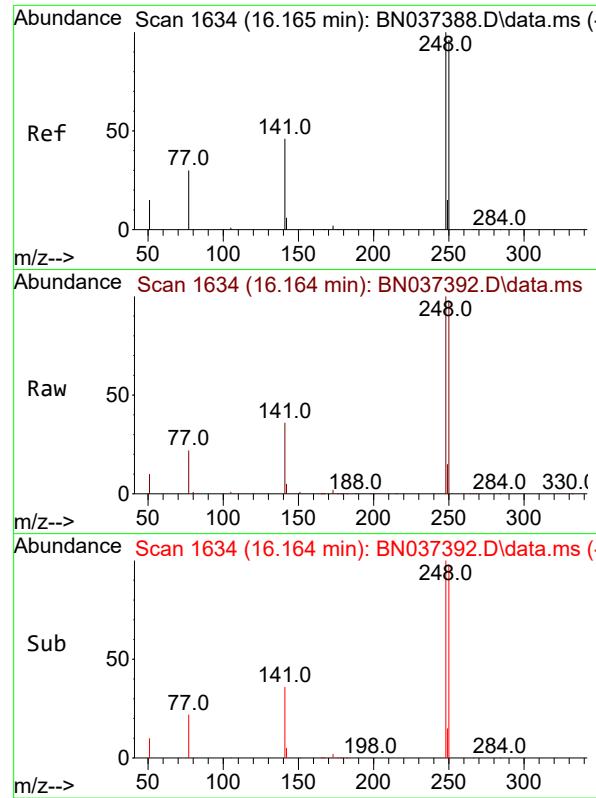

#21

4-Bromophenyl-phenylether

Concen: 5.594 ng

RT: 16.164 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Instrument:

BNA\_N

ClientSampleId :

SSTDICC5.0

Tgt Ion:248 Resp: 25866

Ion Ratio Lower Upper



248 100

250 98.4 77.0 115.4

141 36.3 38.7 58.1#

Abundance

Scan 1634 (16.164 min): BN037392.D\data.ms (-)

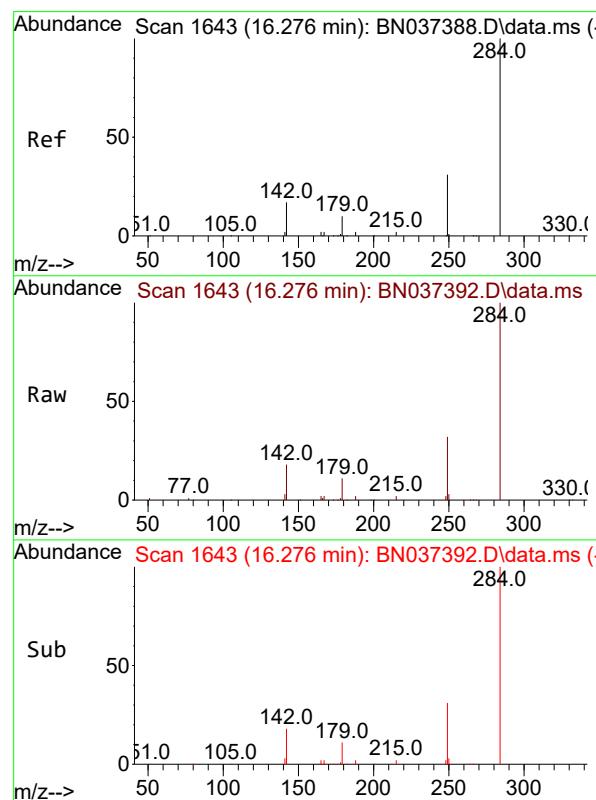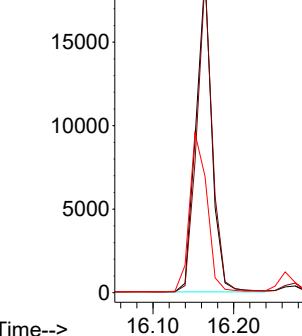

#22

Hexachlorobenzene

Concen: 5.120 ng

RT: 16.276 min Scan# 1643

Delta R.T. -0.000 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Tgt Ion:284 Resp: 25453


Ion Ratio Lower Upper


284 100

142 35.3 27.2 40.8

249 34.4 26.7 40.1

Abundance


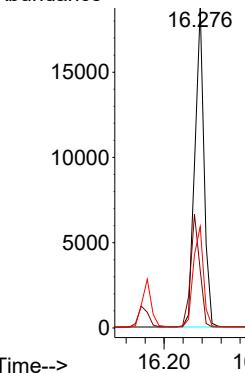


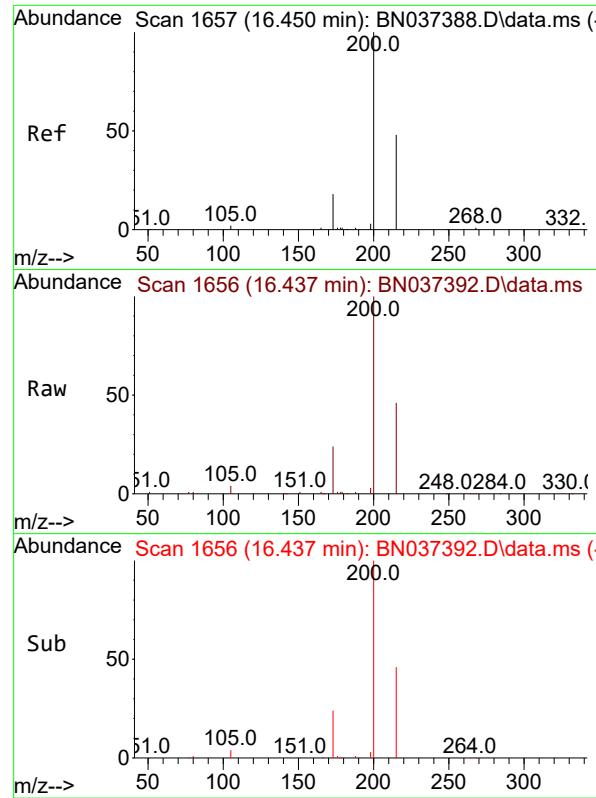

#23  
Atrazine  
Concen: 5.947 ng  
RT: 16.437 min Scan# 1  
Delta R.T. -0.013 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0



Tgt Ion:200 Resp: 21783  
Ion Ratio Lower Upper  
200 100  
173 23.9 19.0 28.6  
215 46.3 41.3 61.9

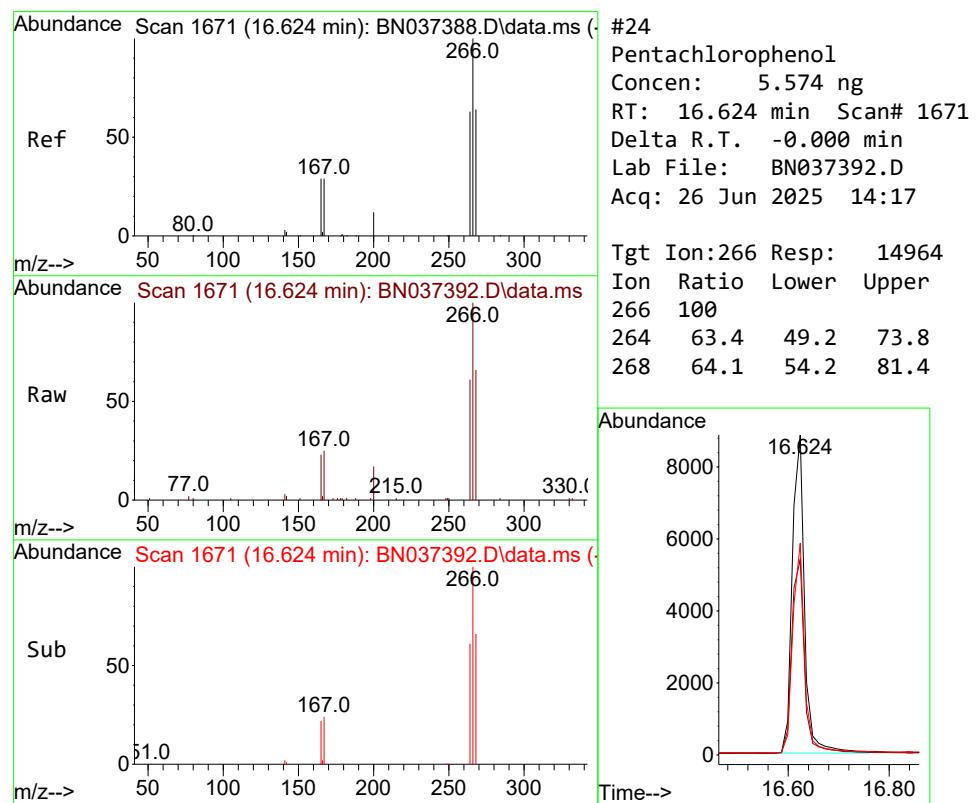

#24  
Pentachlorophenol  
Concen: 5.574 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17

Tgt Ion:266 Resp: 14964  
Ion Ratio Lower Upper  
266 100  
264 63.4 49.2 73.8  
268 64.1 54.2 81.4





#25

Phenanthrene

Concen: 5.708 ng

RT: 16.996 min Scan# 1

Delta R.T. -0.013 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17

Instrument :

BNA\_N

ClientSampleId :

SSTDICC5.0




Tgt Ion:178 Resp: 105409

Ion Ratio Lower Upper

178 100

176 19.3 15.6 23.4

179 15.2 12.8 19.2

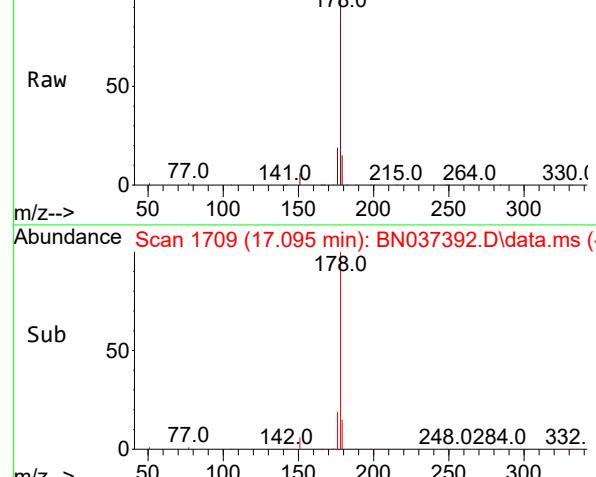

#26

Anthracene

Concen: 5.897 ng

RT: 17.095 min Scan# 1709

Delta R.T. -0.000 min

Lab File: BN037392.D

Acq: 26 Jun 2025 14:17


Tgt Ion:178 Resp: 100113


Ion Ratio Lower Upper

178 100

176 18.6 14.9 22.3

179 15.3 12.4 18.6





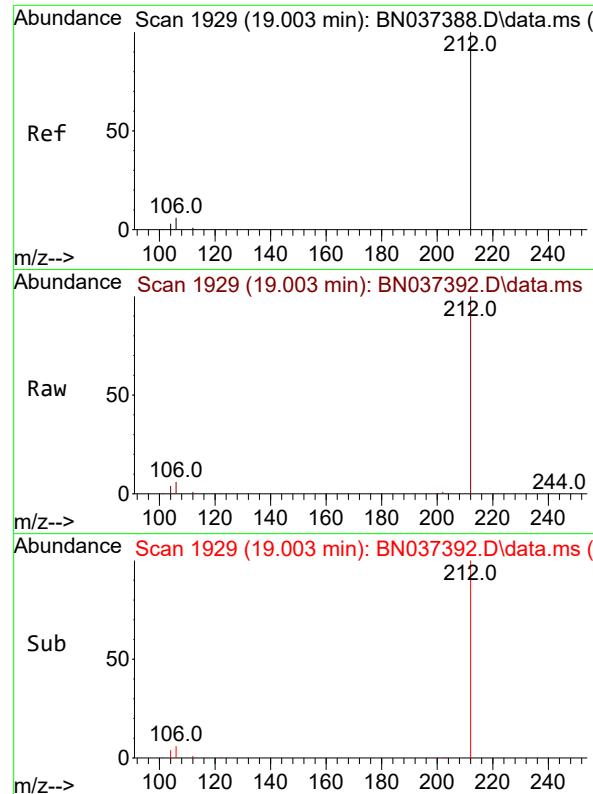

#27  
 Fluoranthene-d10  
 Concen: 6.313 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0


Tgt Ion:212 Resp: 118571  
 Ion Ratio Lower Upper  
 212 100  
 106 6.8 4.5 6.7#  
 104 4.1 2.7 4.1#

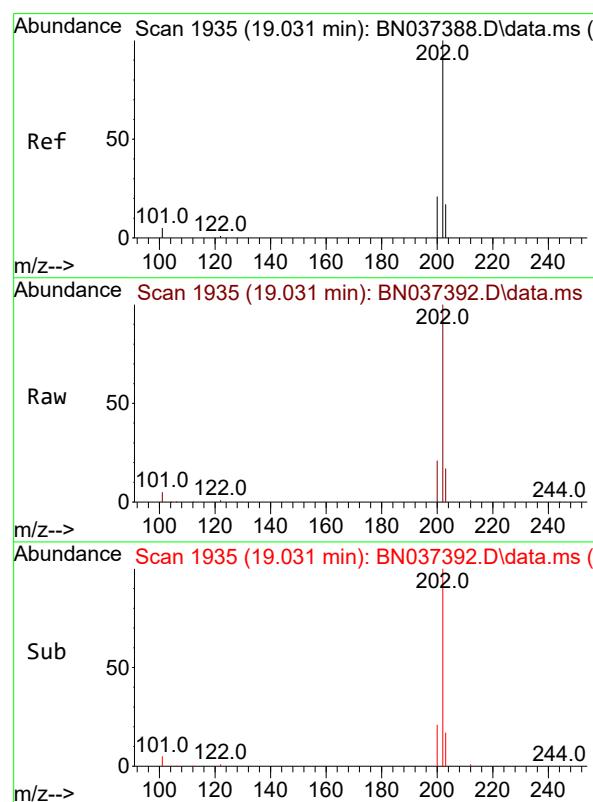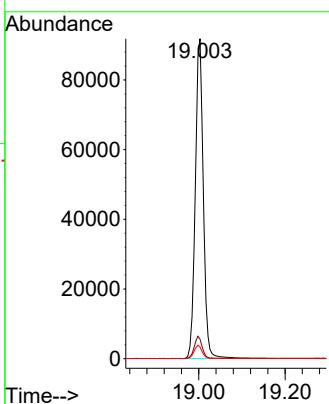

#28  
 Fluoranthene  
 Concen: 5.641 ng  
 RT: 19.031 min Scan# 1935  
 Delta R.T. -0.000 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17

Tgt Ion:202 Resp: 133030  
 Ion Ratio Lower Upper  
 202 100  
 101 5.8 3.8 5.6#  
 203 17.3 13.5 20.3


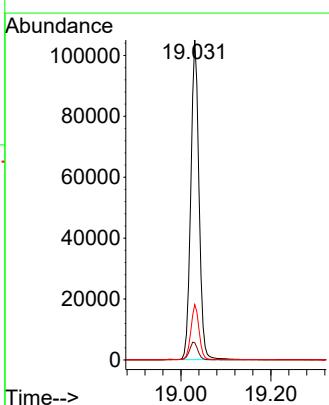


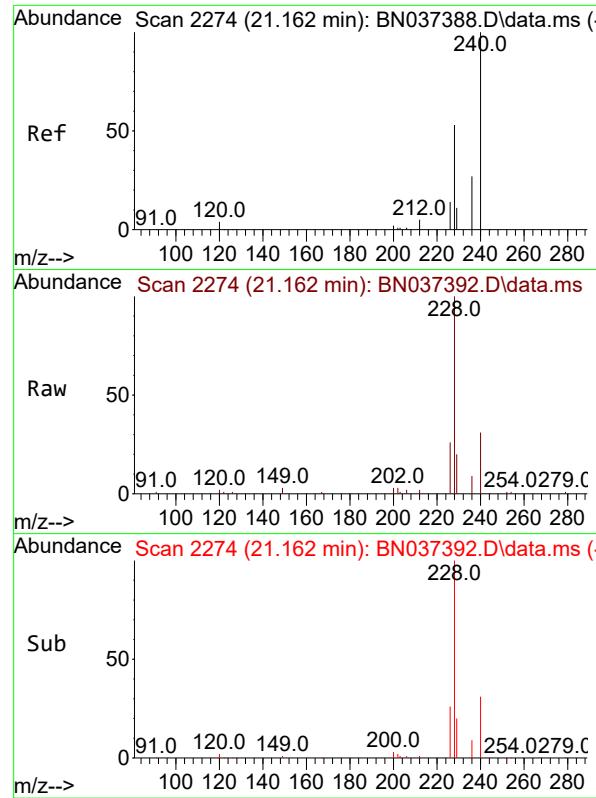

#29  
Chrysene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 21.162 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0


Tgt Ion:240 Resp: 6601  
Ion Ratio Lower Upper  
240 100  
120 7.3 5.3 7.9  
236 28.7 22.7 34.1

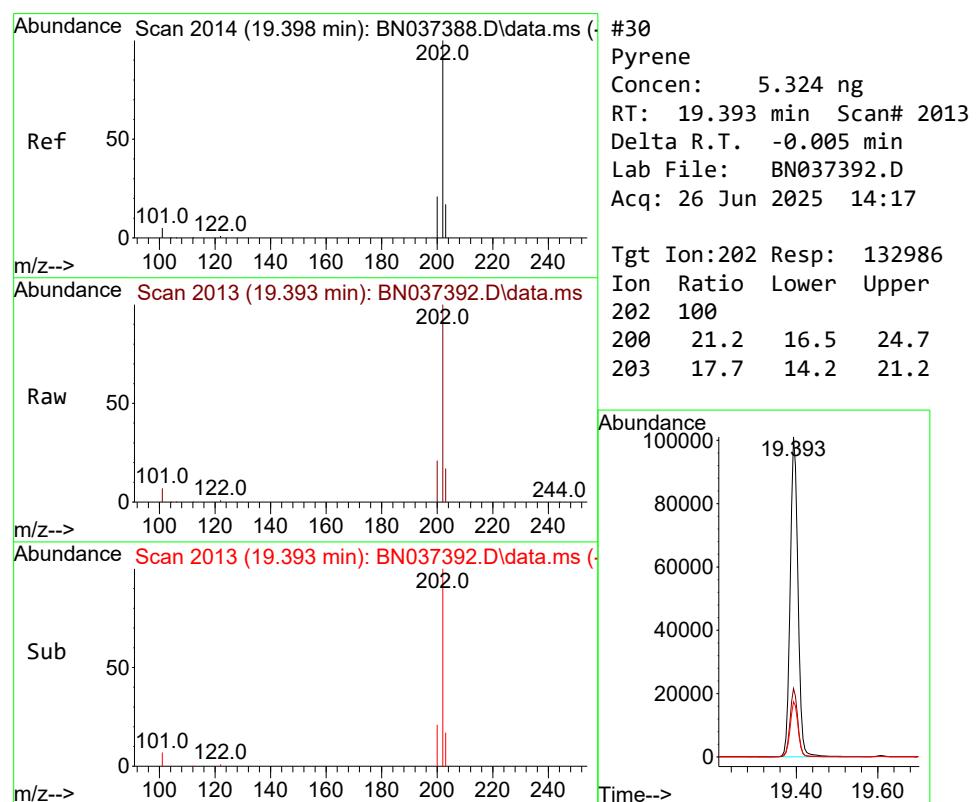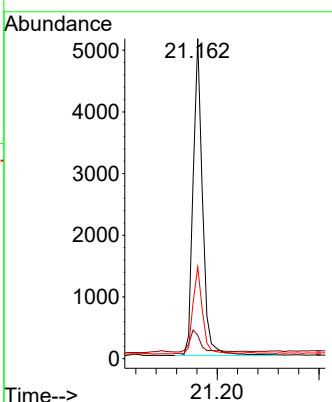

#30  
Pyrene  
Concen: 5.324 ng  
RT: 19.393 min Scan# 2013  
Delta R.T. -0.005 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17

Tgt Ion:202 Resp: 132986  
Ion Ratio Lower Upper  
202 100  
200 21.2 16.5 24.7  
203 17.7 14.2 21.2





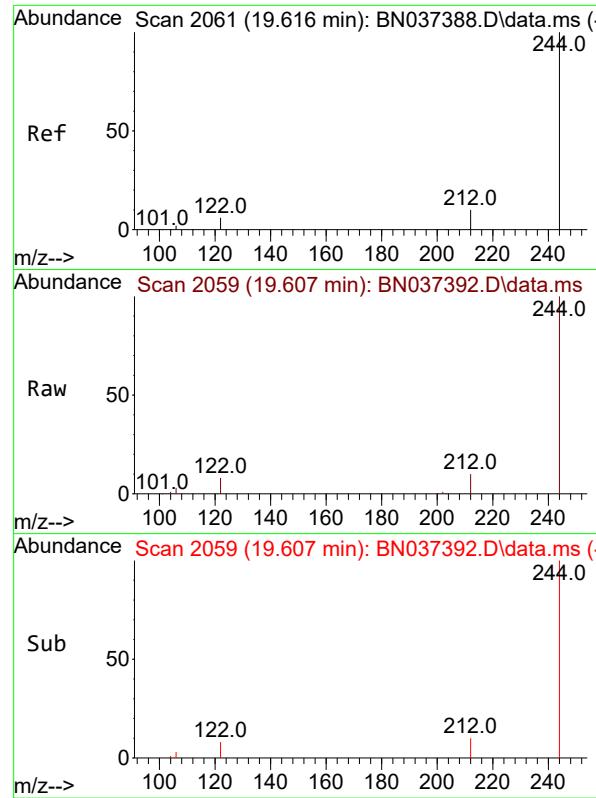

#31  
**Terphenyl-d14**  
Concen: 5.527 ng  
RT: 19.607 min Scan# 2  
Delta R.T. -0.009 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
ClientSampleId : SSTDICC5.0


Tgt Ion:244 Resp: 77795  
Ion Ratio Lower Upper  
244 100  
212 10.2 9.1 13.7  
122 8.3 6.3 9.5

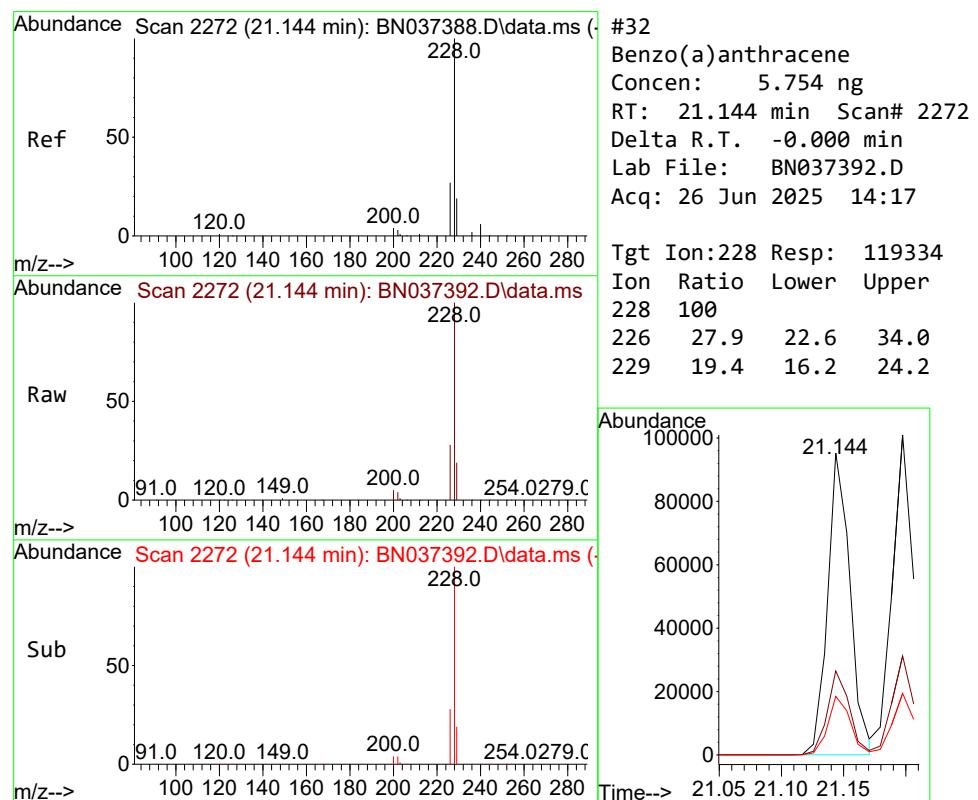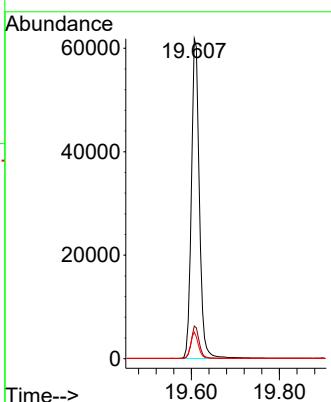

#32  
**Benzo(a)anthracene**  
Concen: 5.754 ng  
RT: 21.144 min Scan# 2272  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17



Tgt Ion:228 Resp: 119334  
Ion Ratio Lower Upper  
228 100  
226 27.9 22.6 34.0  
229 19.4 16.2 24.2



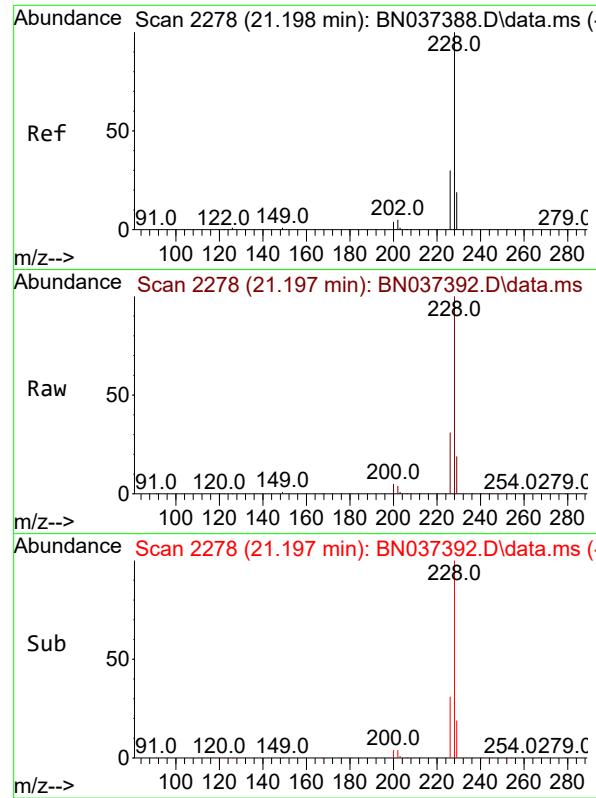


#33  
Chrysene  
Concen: 4.982 ng  
RT: 21.197 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17  
ClientSampleId : SSTDICC5.0


Tgt Ion:228 Resp: 127936  
Ion Ratio Lower Upper  
228 100  
226 30.9 24.5 36.7  
229 19.3 16.1 24.1

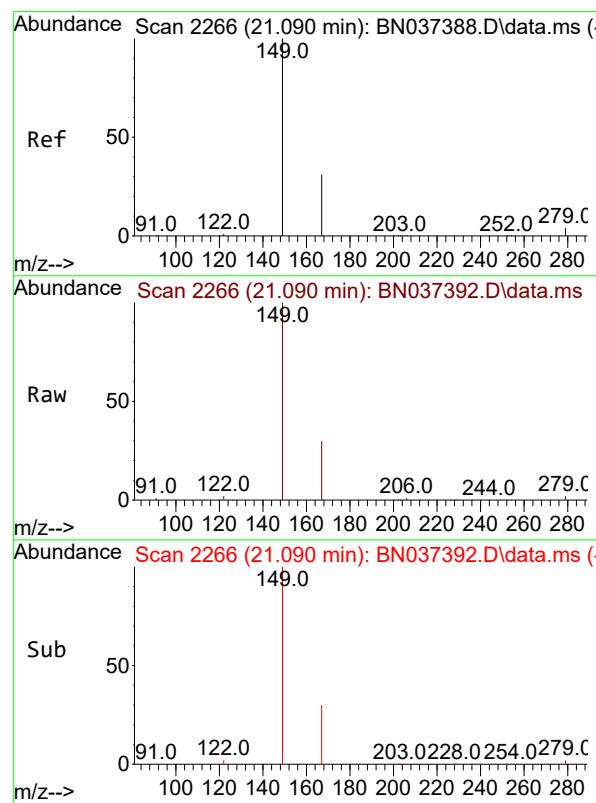

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 5.397 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. -0.000 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17

Tgt Ion:149 Resp: 44321  
Ion Ratio Lower Upper  
149 100  
167 30.9 24.8 37.2  
279 5.0 5.0 7.6#





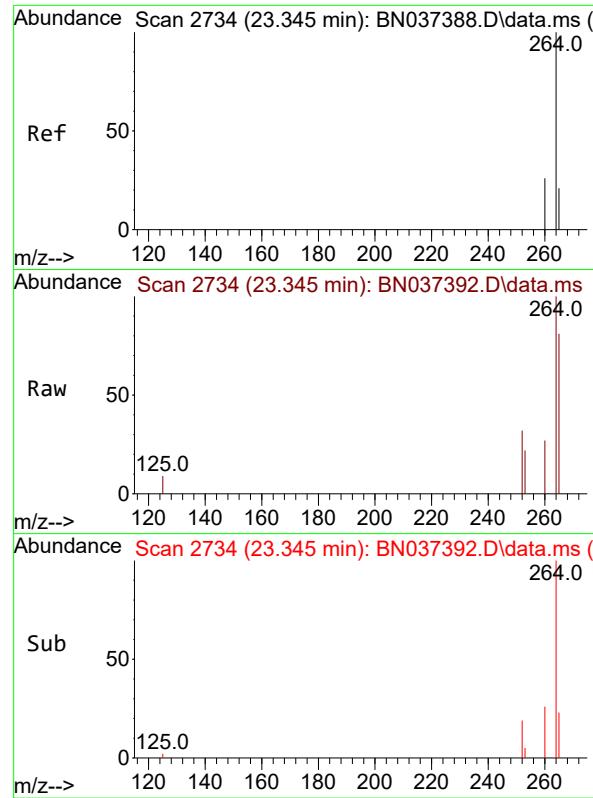

#35  
 Perylene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 23.345 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0


Tgt Ion:264 Resp: 6264  
 Ion Ratio Lower Upper  
 264 100  
 260 27.3 21.4 32.0  
 265 81.1 56.2 84.4

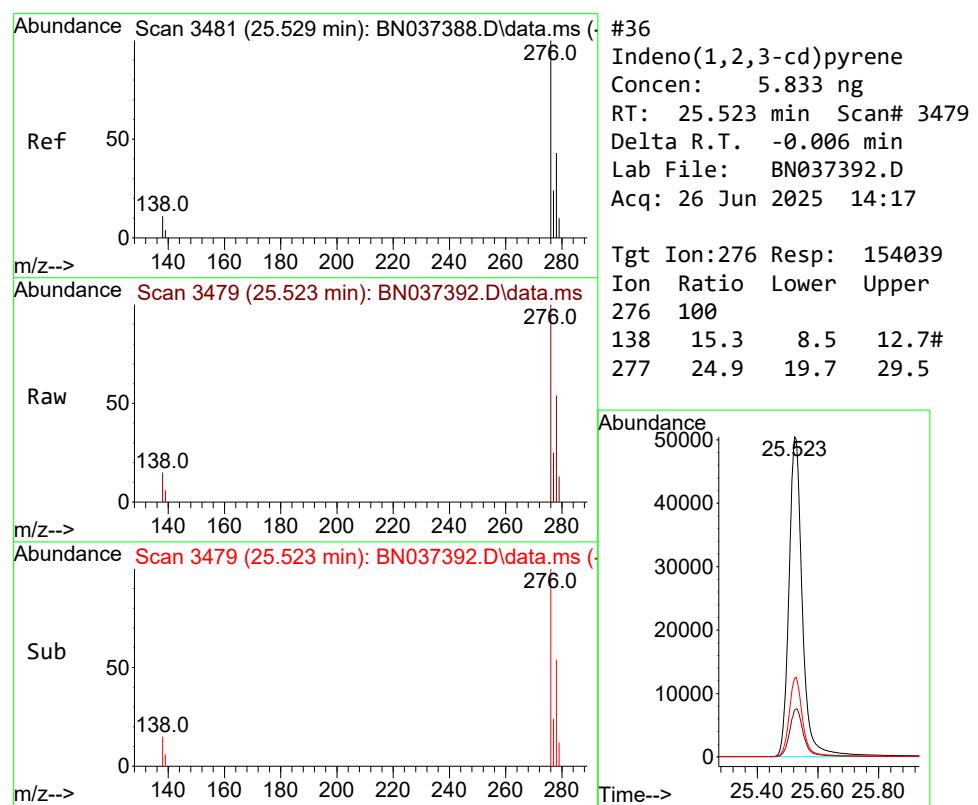

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 5.833 ng  
 RT: 25.523 min Scan# 3479  
 Delta R.T. -0.006 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17



Tgt Ion:276 Resp: 154039  
 Ion Ratio Lower Upper  
 276 100  
 138 15.3 8.5 12.7#  
 277 24.9 19.7 29.5



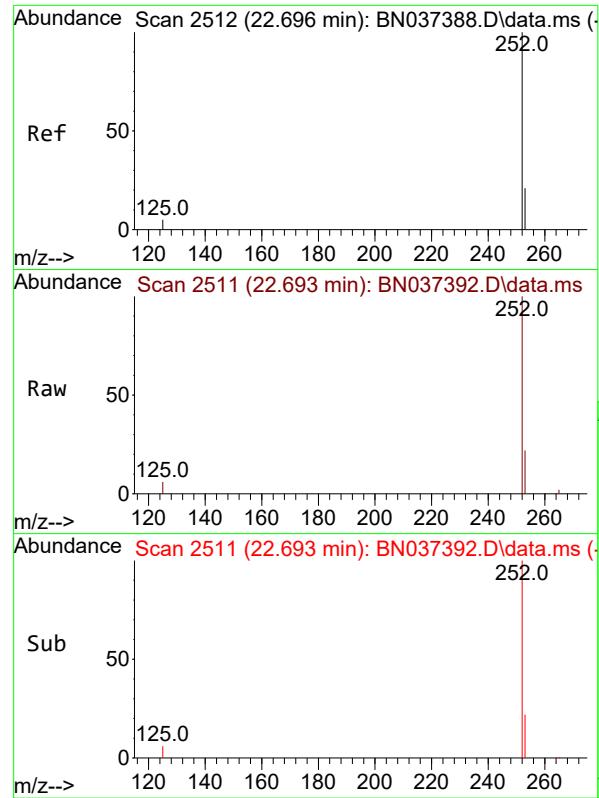


#37  
Benzo(b)fluoranthene  
Concen: 5.787 ng  
RT: 22.693 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.003 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17  
ClientSampleId : SSTDICC5.0


Tgt Ion:252 Resp: 127810  
Ion Ratio Lower Upper  
252 100  
253 22.2 22.8 34.2#  
125 6.0 6.2 9.4#

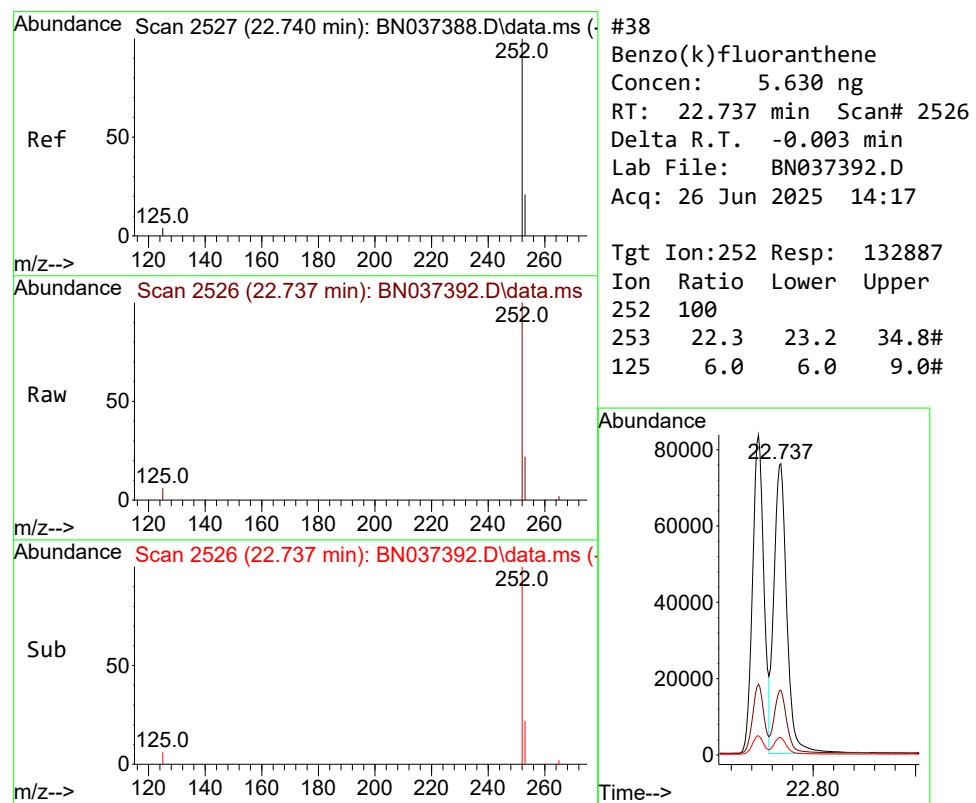

#38  
Benzo(k)fluoranthene  
Concen: 5.630 ng  
RT: 22.737 min Scan# 2526  
Delta R.T. -0.003 min  
Lab File: BN037392.D  
Acq: 26 Jun 2025 14:17

Tgt Ion:252 Resp: 132887  
Ion Ratio Lower Upper  
252 100  
253 22.3 23.2 34.8#  
125 6.0 6.0 9.0#





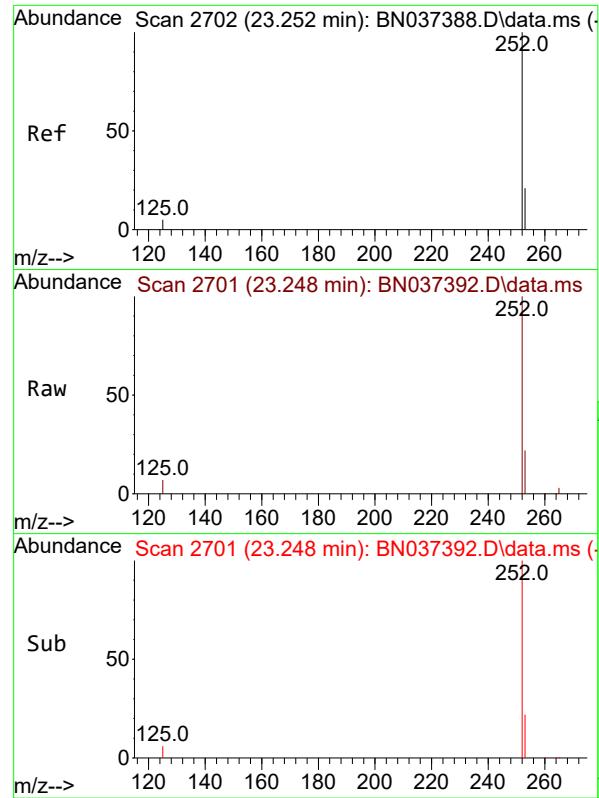

#39  
 Benzo(a)pyrene  
 Concen: 5.686 ng  
 RT: 23.248 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17


Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0


Tgt Ion:252 Resp: 111691  
 Ion Ratio Lower Upper  
 252 100  
 253 22.3 25.6 38.4#  
 125 6.6 7.5 11.3#

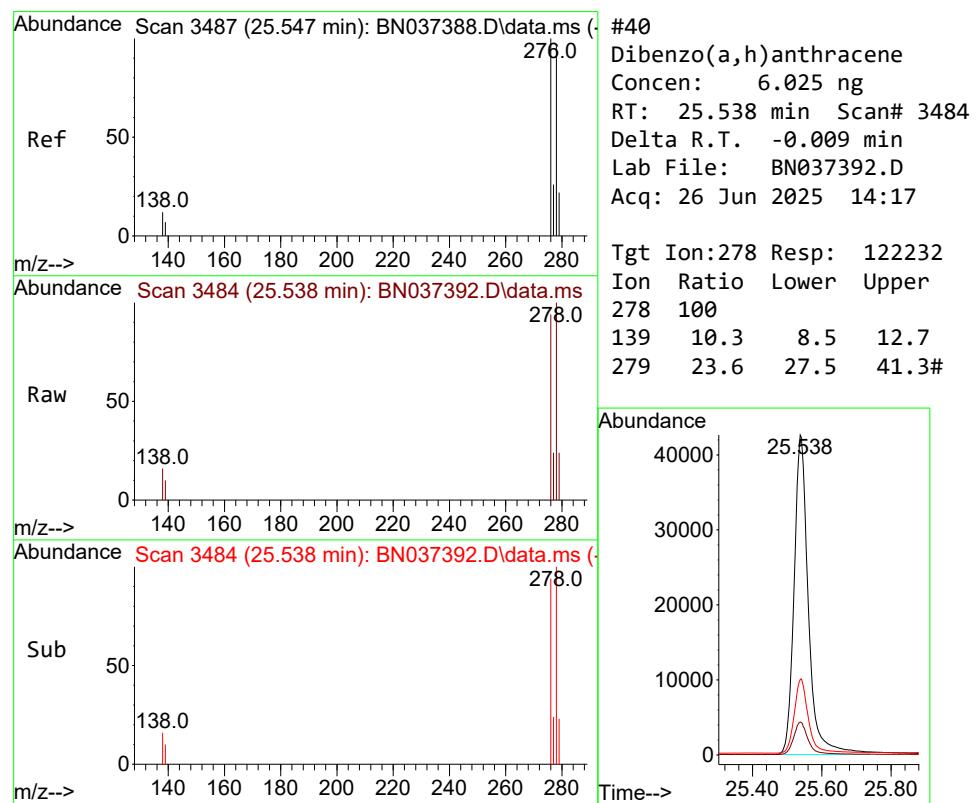

#40  
 Dibenzo(a,h)anthracene  
 Concen: 6.025 ng  
 RT: 25.538 min Scan# 3484  
 Delta R.T. -0.009 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17

Tgt Ion:278 Resp: 122232  
 Ion Ratio Lower Upper  
 278 100  
 139 10.3 8.5 12.7  
 279 23.6 27.5 41.3#




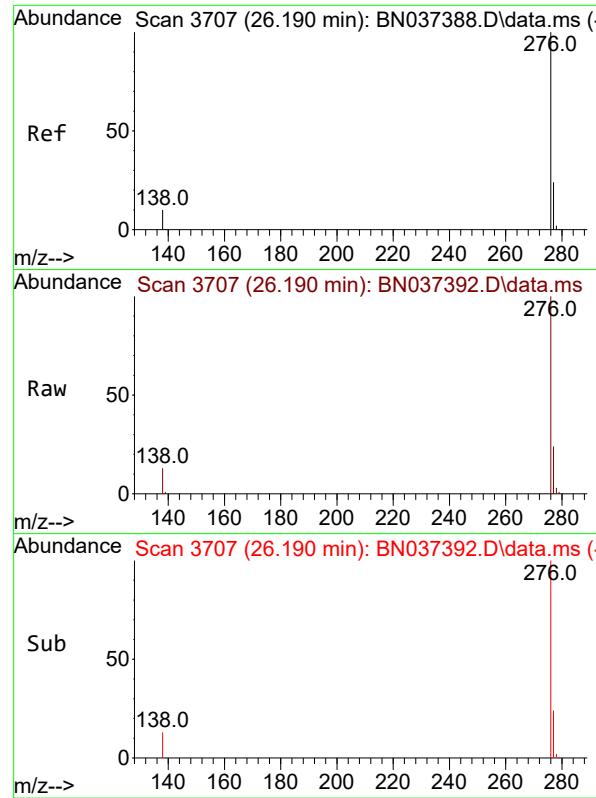

#41  
 Benzo(g,h,i)perylene  
 Concen: 5.570 ng  
 RT: 26.190 min Scan# 3  
 Delta R.T. -0.000 min  
 Lab File: BN037392.D  
 Acq: 26 Jun 2025 14:17

Instrument : BNA\_N  
 ClientSampleId : SSTDICC5.0

Tgt Ion:276 Resp: 135052  
 Ion Ratio Lower Upper  
 276 100  
 277 23.6 21.0 31.4  
 138 13.4 9.6 14.4

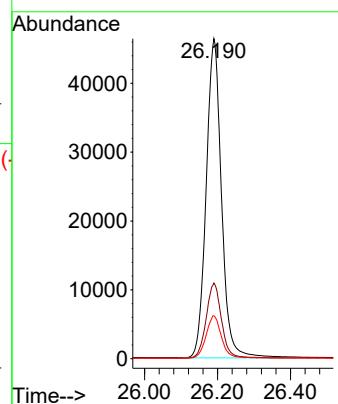

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037393.D  
 Acq On : 26 Jun 2025 14:54  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 ICVBN062625

Quant Time: Jun 26 16:06:51 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2171	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4836	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	3065	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	6127	0.400	ng	# 0.01
29) Chrysene-d12	21.162	240	5019	0.400	ng	# 0.00
35) Perylene-d12	23.348	264	4884	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1574	0.376	ng	0.00
5) Phenol-d6	6.744	99	1620	0.373	ng	0.00
8) Nitrobenzene-d5	8.717	82	1646	0.425	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	3153	0.421	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	623	0.347	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	6004	0.454	ng	0.00
27) Fluoranthene-d10	19.003	212	6867	0.391	ng	0.00
31) Terphenyl-d14	19.616	244	4960	0.464	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	1015	0.493	ng	94
3) n-Nitrosodimethylamine	3.422	42	847	0.417	ng	# 88
6) bis(2-Chloroethyl)ether	7.004	93	1776	0.460	ng	99
9) Naphthalene	10.394	128	5176	0.416	ng	99
10) Hexachlorobutadiene	10.682	225	2038	0.412	ng	# 99
12) 2-Methylnaphthalene	12.016	142	3148	0.367	ng	98
16) Acenaphthylene	13.935	152	5693	0.448	ng	99
17) Acenaphthene	14.277	154	3435	0.414	ng	99
18) Fluorene	15.272	166	4775	0.407	ng	100
20) 4,6-Dinitro-2-methylph...	15.378	198	497	0.316	ng	# 86
21) 4-Bromophenyl-phenylether	16.165	248	1722	0.398	ng	# 93
22) Hexachlorobenzene	16.276	284	1984	0.427	ng	97
23) Atrazine	16.450	200	1384	0.404	ng	97
24) Pentachlorophenol	16.624	266	775	0.309	ng	98
25) Phenanthrene	17.009	178	7070	0.410	ng	99
26) Anthracene	17.095	178	6496	0.409	ng	99
28) Fluoranthene	19.035	202	8423	0.382	ng	99
30) Pyrene	19.398	202	8354	0.440	ng	99
32) Benzo(a)anthracene	21.153	228	6494	0.412	ng	99
33) Chrysene	21.198	228	7943	0.407	ng	99
34) Bis(2-ethylhexyl)phtha...	21.090	149	2775	0.444	ng	99
36) Indeno(1,2,3-cd)pyrene	25.532	276	8543	0.415	ng	96
37) Benzo(b)fluoranthene	22.699	252	6764	0.393	ng	96
38) Benzo(k)fluoranthene	22.743	252	8109	0.441	ng	# 96
39) Benzo(a)pyrene	23.254	252	6621	0.432	ng	# 94
40) Dibenzo(a,h)anthracene	25.552	278	6443	0.407	ng	96
41) Benzo(g,h,i)perylene	26.193	276	7497	0.397	ng	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037393.D  
 Acq On : 26 Jun 2025 14:54  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 ICVBN062625

Quant Time: Jun 26 16:06:51 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

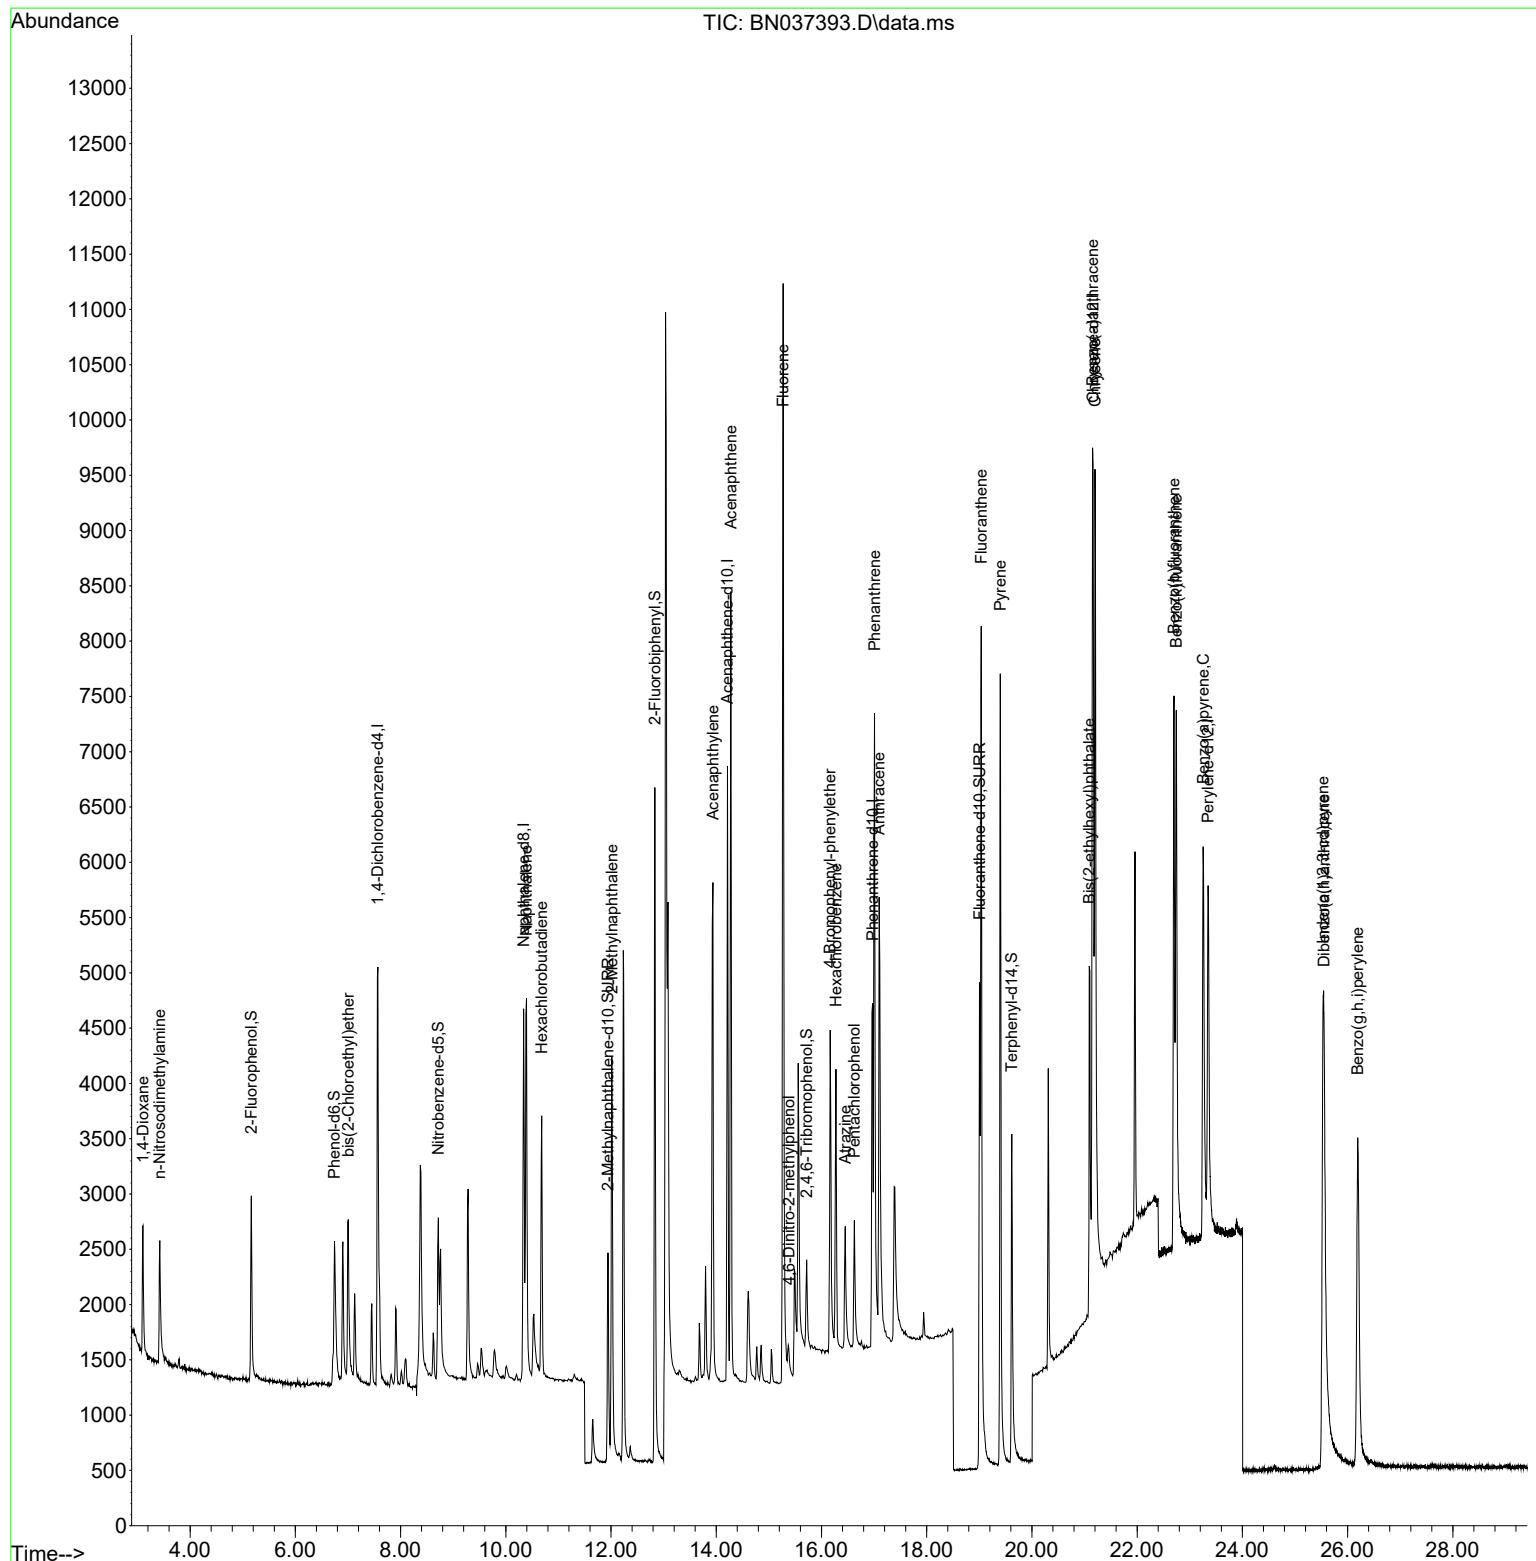

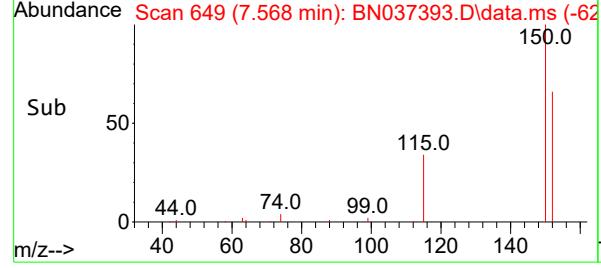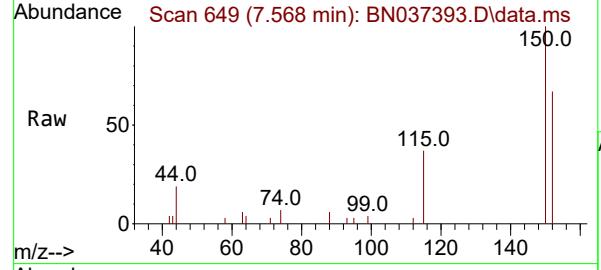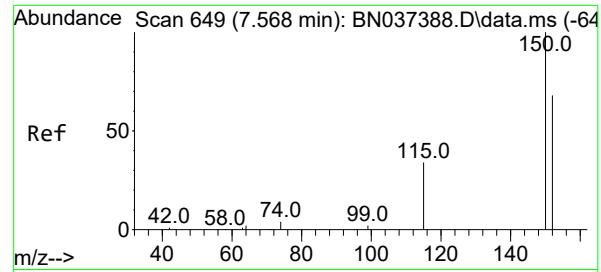

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.568 min Scan# 6

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54

Instrument :

BNA\_N

ClientSampleId :

ICVBN062625




Tgt Ion:152 Resp: 2171

Ion Ratio Lower Upper

152 100

150 148.2 116.2 174.2

115 55.1 42.9 64.3

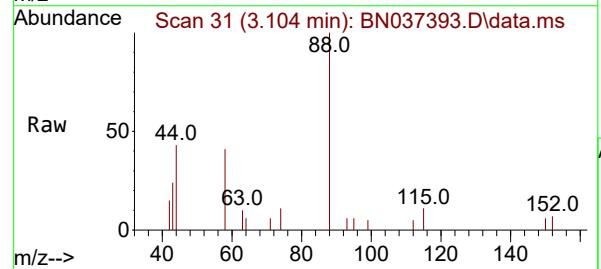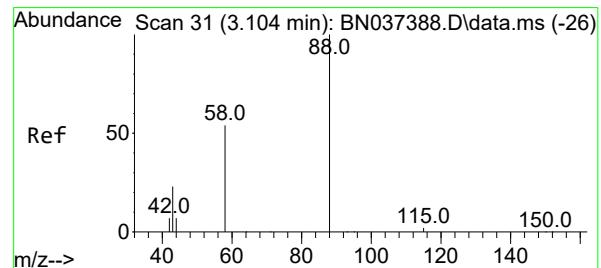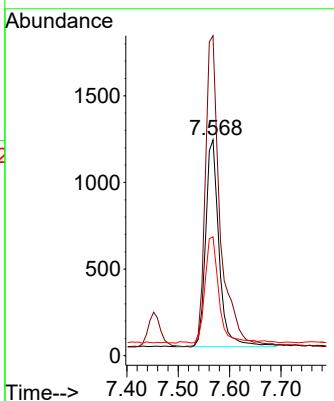

#2

1,4-Dioxane

Concen: 0.493 ng

RT: 3.104 min Scan# 31

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54



Tgt Ion: 88 Resp: 1015

Ion Ratio Lower Upper

88 100


43 23.0 21.6 32.4

58 53.6 45.9 68.9

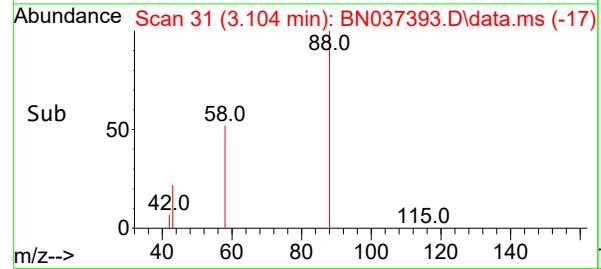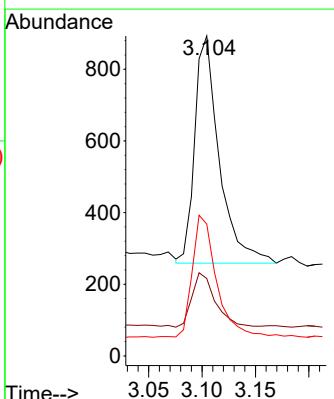



Sub

m/z--&gt;

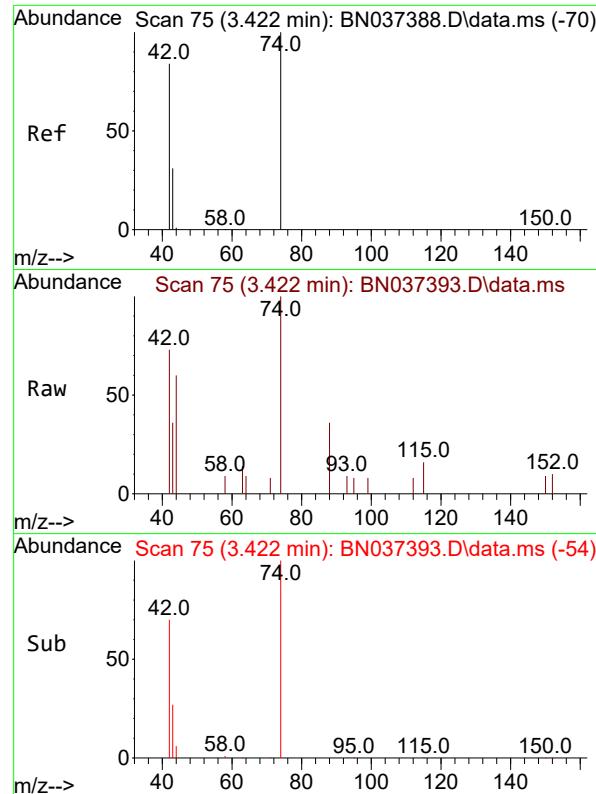


#3  
n-Nitrosodimethylamine  
Concen: 0.417 ng  
RT: 3.422 min Scan# 7  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54  
ClientSampleId : ICVBN062625




Tgt Ion: 42 Resp: 847  
Ion Ratio Lower Upper  
42 100  
74 136.5 97.8 146.8  
44 7.3 8.7 13.1#

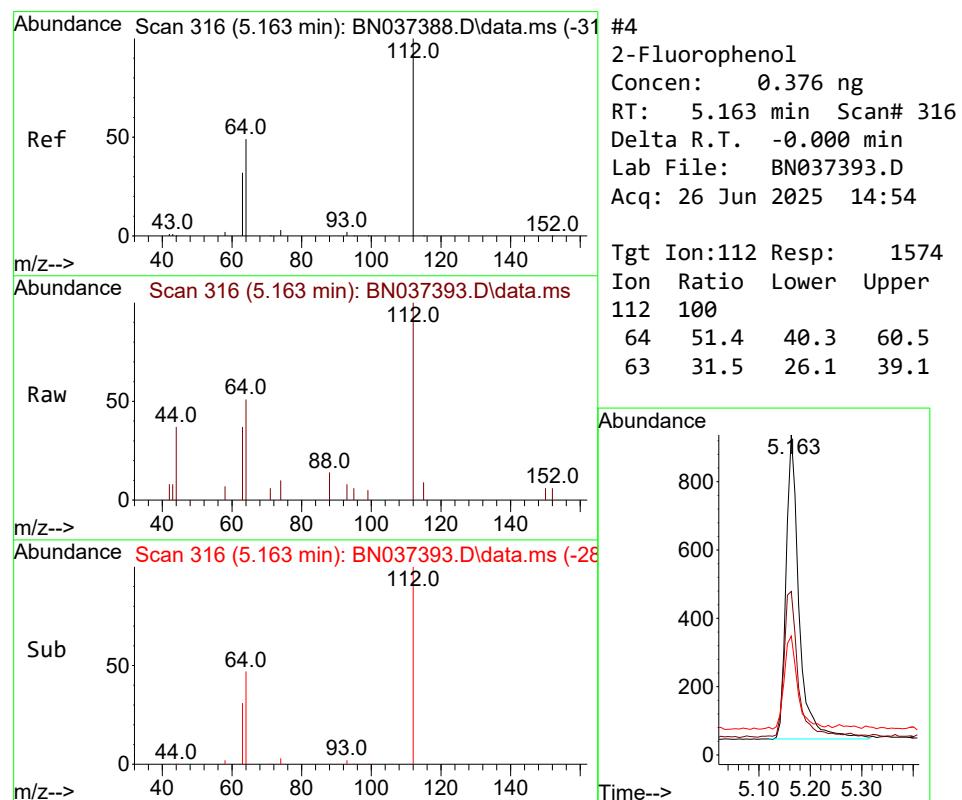

#4  
2-Fluorophenol  
Concen: 0.376 ng  
RT: 5.163 min Scan# 316  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54

Tgt Ion: 112 Resp: 1574  
Ion Ratio Lower Upper  
112 100  
64 51.4 40.3 60.5  
63 31.5 26.1 39.1






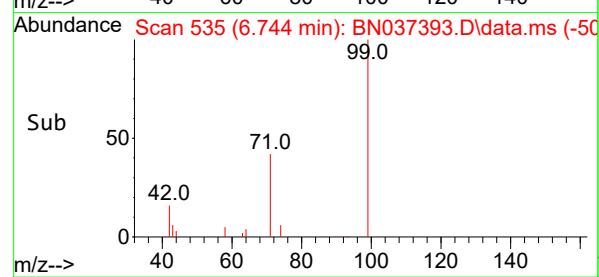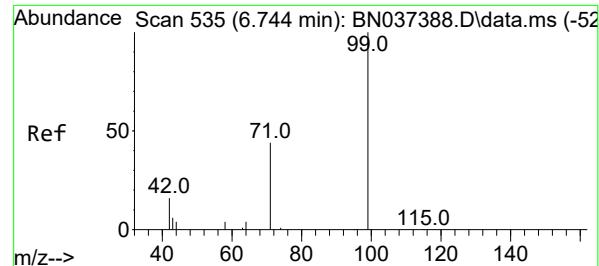

#5  
 Phenol-d6  
 Concen: 0.373 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. -0.000 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54



Instrument : BNA\_N  
 ClientSampleId : ICVBN062625


Tgt Ion: 99 Resp: 1620  
 Ion Ratio Lower Upper  
 99 100  
 42 18.6 15.6 23.4  
 71 42.7 35.8 53.8

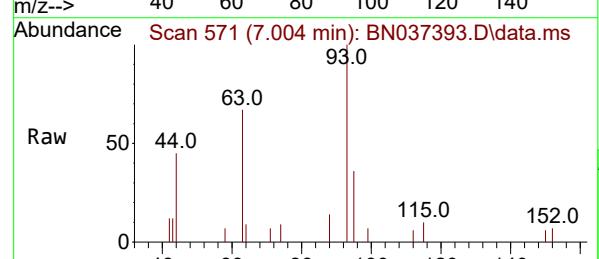

#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.460 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. 0.007 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54


Tgt Ion: 93 Resp: 1776  
 Ion Ratio Lower Upper  
 93 100  
 63 60.8 49.6 74.4  
 95 30.5 23.9 35.9







#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54

Instrument : BNA\_N  
 ClientSampleId : ICVBN062625




Tgt Ion:136 Resp: 4836



Ion	Ratio	Lower	Upper
136	100		
137	12.9	10.4	15.6
54	7.1	5.6	8.4
68	5.9	4.6	6.8



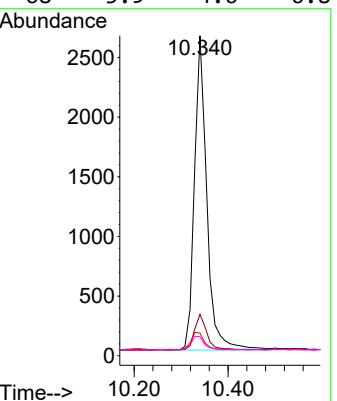


#8  
 Nitrobenzene-d5  
 Concen: 0.425 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. -0.000 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54



Tgt Ion: 82 Resp: 1646  
 Ion Ratio Lower Upper  
 82 100  
 128 44.2 34.0 51.0  
 54 42.2 37.7 56.5

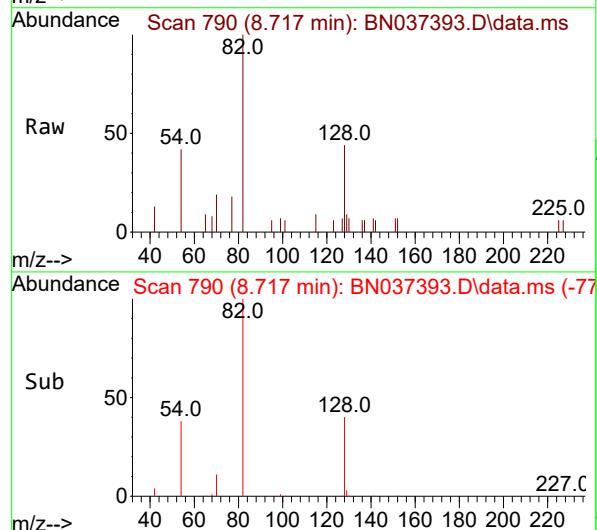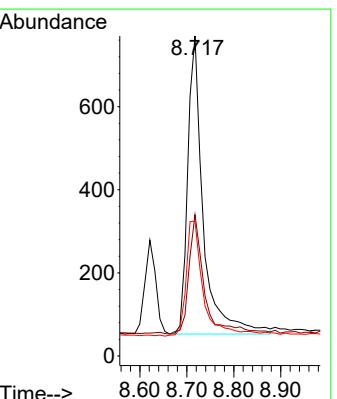



#9

Naphthalene

Concen: 0.416 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54

Instrument :

BNA\_N

ClientSampleId :

ICVBN062625

Tgt Ion:128 Resp: 5176

Ion Ratio Lower Upper

128 100

129 12.4 10.4 15.6

127 14.9 12.2 18.4

Abundance

2500 10.394





2000

1500

1000

500

0

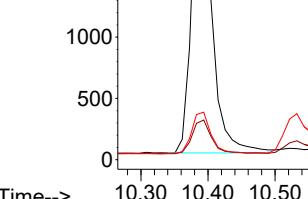

#10

Hexachlorobutadiene

Concen: 0.412 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54

Tgt Ion:225 Resp: 2038

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0


227 62.9 49.9 74.9




Abundance

1000 10.682

500





0

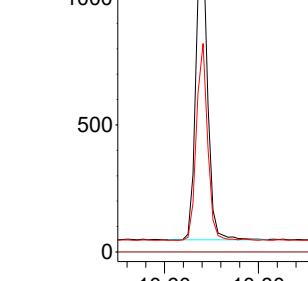




#11  
2-Methylnaphthalene-d10  
Concen: 0.421 ng  
RT: 11.940 min Scan# 1:Instrument :  
Delta R.T. -0.000 min BNA\_N  
Lab File: BN037393.D ClientSampleId :  
Acq: 26 Jun 2025 14:54 ICBVN062625


Tgt Ion:152 Resp: 3153  
Ion Ratio Lower Upper  
152 100  
151 21.6 18.4 27.6

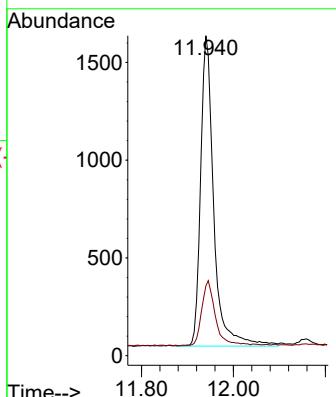

#12  
2-Methylnaphthalene  
Concen: 0.367 ng  
RT: 12.016 min Scan# 1152  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54

Tgt Ion:142 Resp: 3148  
Ion Ratio Lower Upper  
142 100  
141 88.9 70.1 105.1  
115 43.1 35.8 53.6


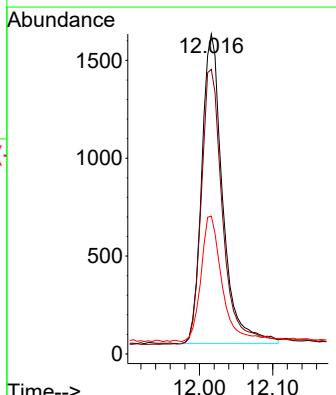


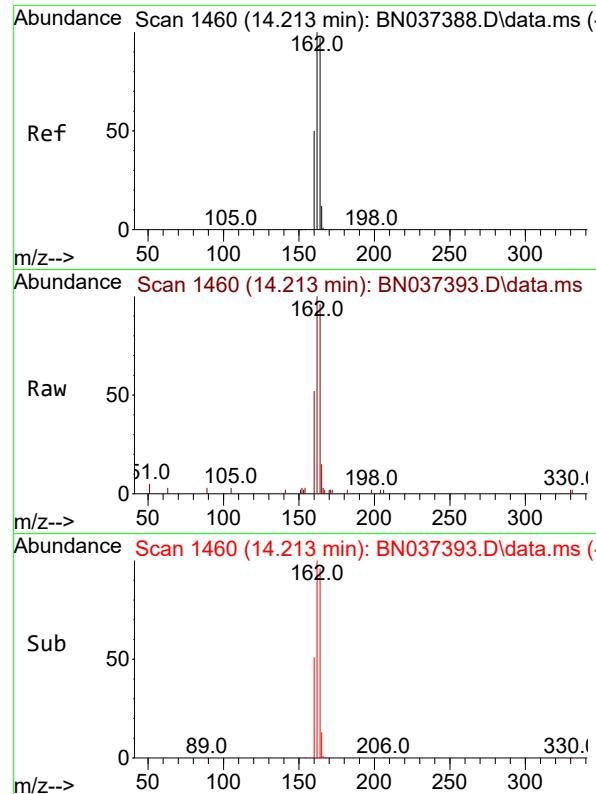


#13


Acenaphthene-d10  
Concen: 0.400 ngRT: 14.213 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54Instrument :  
BNA\_N  
ClientSampleId :  
ICVBN062625

Tgt Ion:164 Resp: 3065

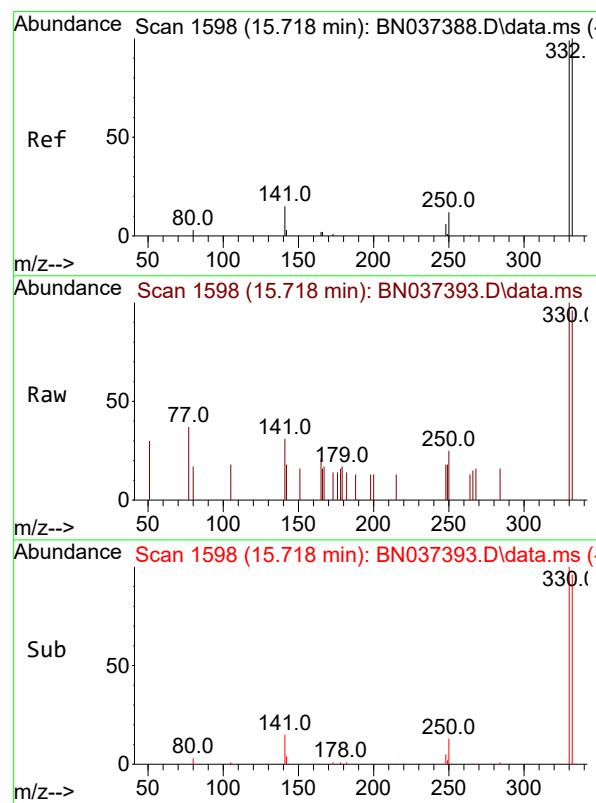Ion Ratio Lower Upper  
164 100  
162 104.4 82.6 123.8  
160 54.1 42.2 63.2



#14

2,4,6-Tribromophenol  
Concen: 0.347 ng  
RT: 15.718 min Scan# 1598  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54Tgt Ion:330 Resp: 623  
Ion Ratio Lower Upper  
330 100  
332 97.3 77.8 116.8  
141 26.8 24.0 36.0

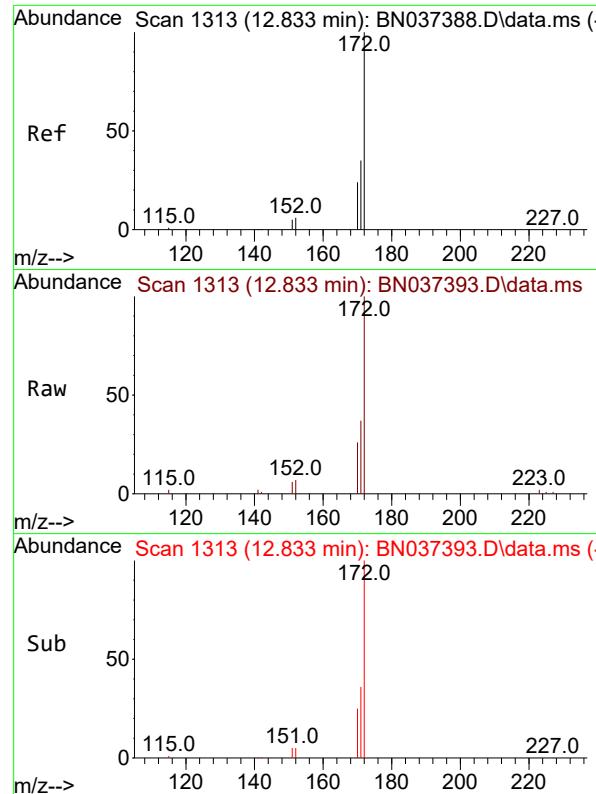


#15  
2-Fluorobiphenyl  
Concen: 0.454 ng  
RT: 12.833 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54  
ClientSampleId : ICVBN062625




Tgt Ion:172 Resp: 6004  
Ion Ratio Lower Upper  
172 100  
171 36.6 28.8 43.2  
170 25.6 20.3 30.5

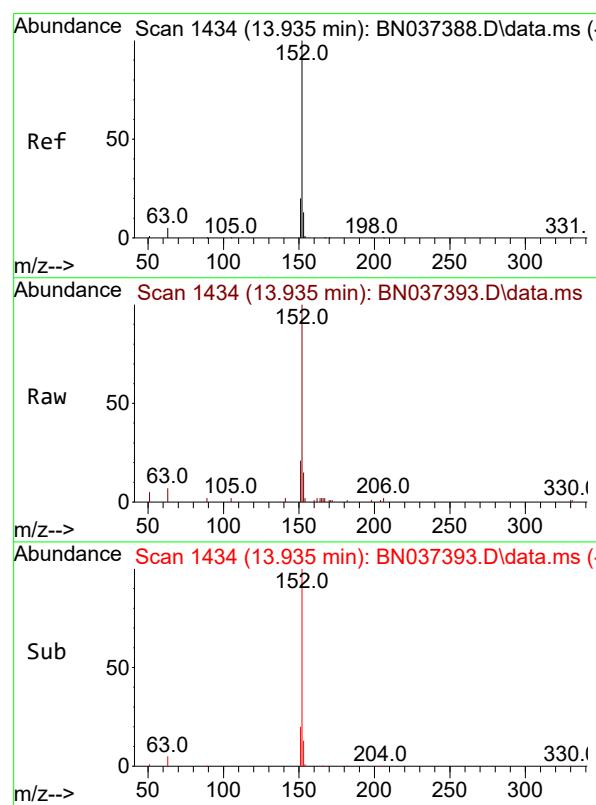

#16  
Acenaphthylene  
Concen: 0.448 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54

Tgt Ion:152 Resp: 5693  
Ion Ratio Lower Upper  
152 100  
151 20.1 15.8 23.6  
153 12.9 10.3 15.5





#17

Acenaphthene

Concen: 0.414 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54

Instrument :

BNA\_N

ClientSampleId :

ICVBN062625





Tgt Ion:154 Resp: 3435

Ion Ratio Lower Upper

154 100

153 116.4 94.6 141.8

152 63.6 50.2 75.2

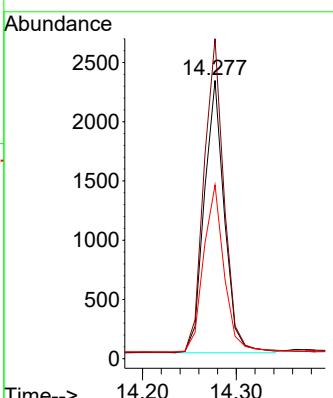

#18

Fluorene

Concen: 0.407 ng

RT: 15.272 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54


Tgt Ion:166 Resp: 4775


Ion Ratio Lower Upper

166 100

165 99.5 79.4 119.2

167 14.0 10.6 15.8


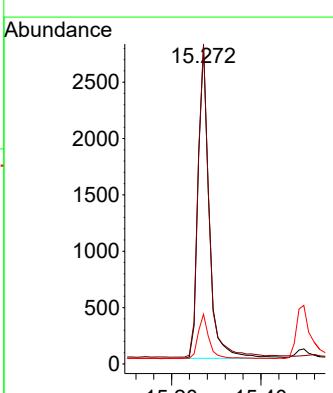


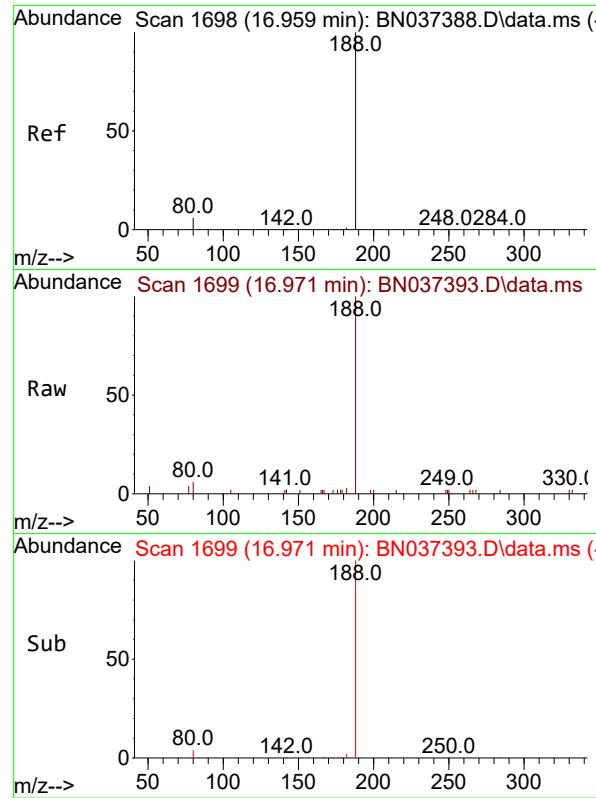

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. 0.012 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54


Instrument : BNA\_N  
 ClientSampleId : ICVBN062625



Tgt Ion:188 Resp: 6127  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 5.8 6.2 9.4#

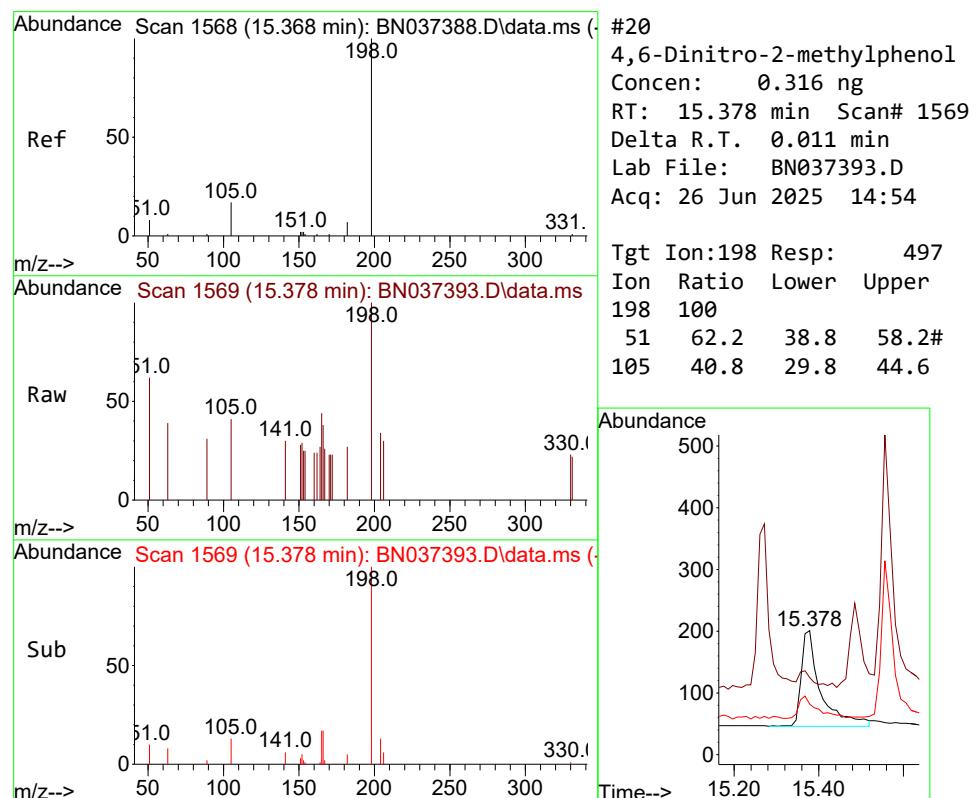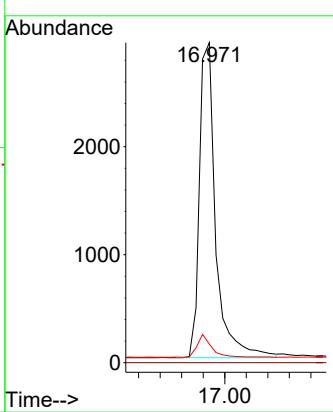

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.316 ng  
 RT: 15.378 min Scan# 1569  
 Delta R.T. 0.011 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54

Tgt Ion:198 Resp: 497  
 Ion Ratio Lower Upper  
 198 100  
 51 62.2 38.8 58.2#  
 105 40.8 29.8 44.6

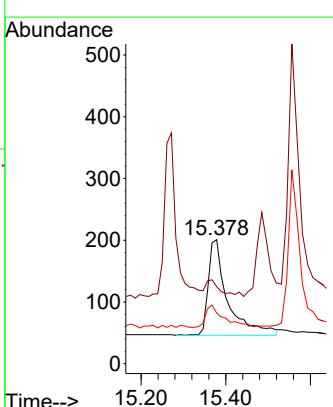

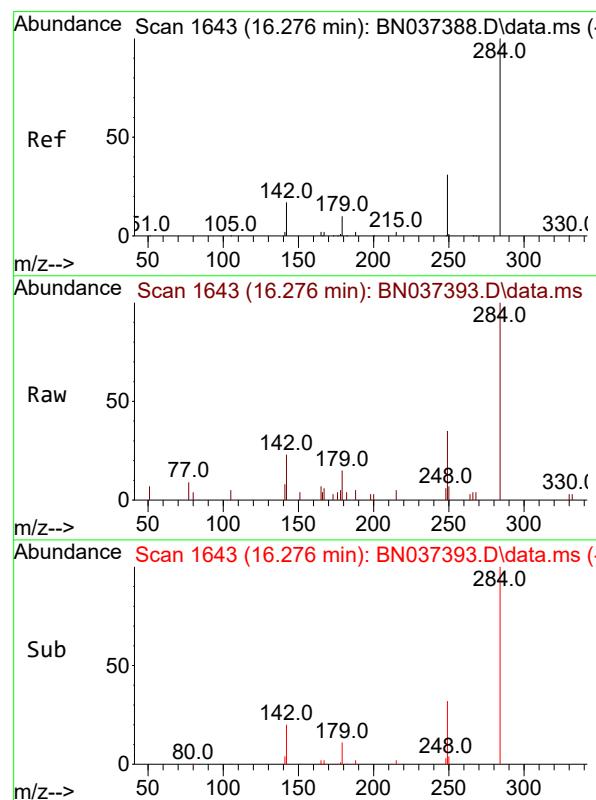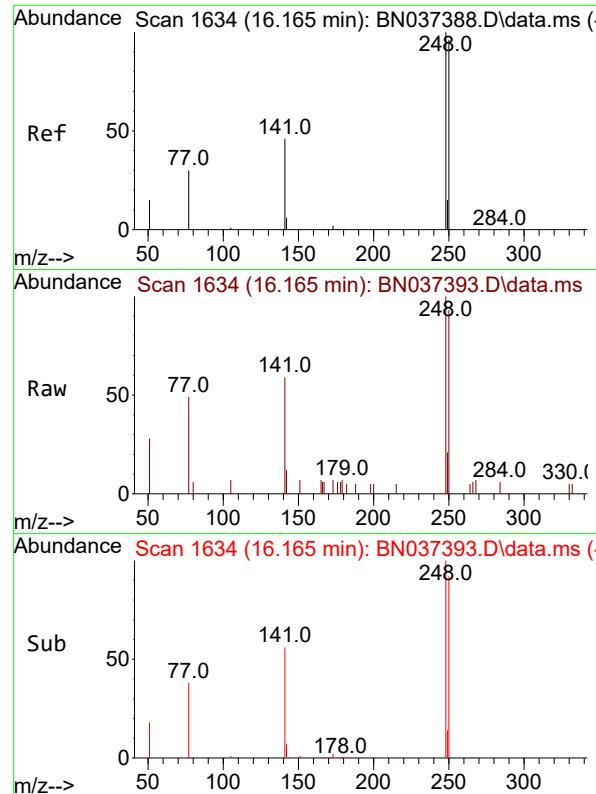

#22

Hexachlorobenzene

Concen: 0.427 ng

RT: 16.276 min Scan# 1643


Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54

Tgt Ion:284 Resp: 1984

Ion	Ratio	Lower	Upper
284	100		
142	34.2	27.2	40.8
249	36.5	26.7	40.1

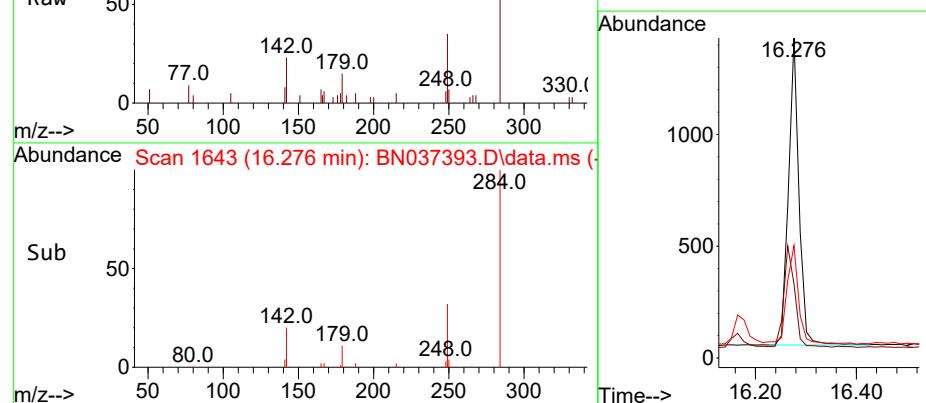

#22

Hexachlorobenzene




Concen: 0.427 ng

RT: 16.276 min Scan# 1643

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54

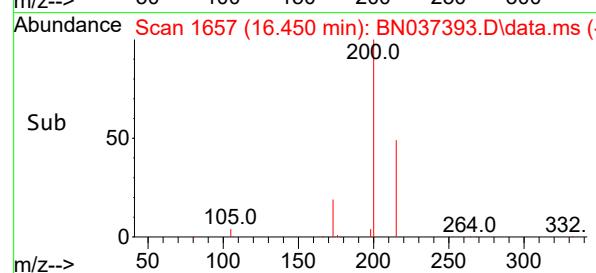





#23

Atrazine  
Concen: 0.404 ng  
RT: 16.450 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54

Instrument :  
BNA\_N  
ClientSampleId :  
ICVBN062625

Tgt Ion:200 Resp: 1384

Ion	Ratio	Lower	Upper
200	100		
173	25.2	19.0	28.6
215	53.3	41.3	61.9

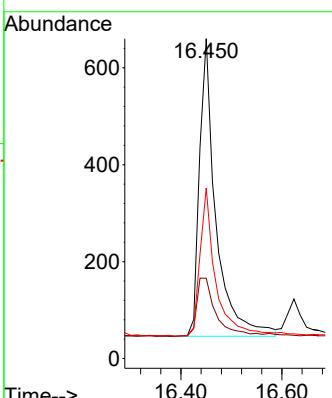





#24

Pentachlorophenol  
Concen: 0.309 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54

Tgt Ion:266 Resp: 775

Ion	Ratio	Lower	Upper
266	100		
264	64.0	49.2	73.8
268	68.8	54.2	81.4

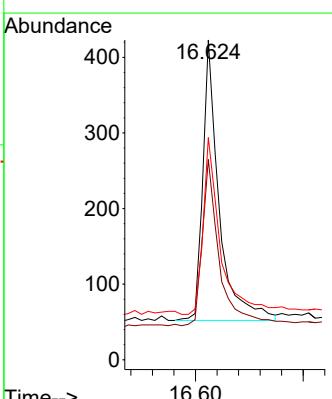



#25

Phenanthrene

Concen: 0.410 ng

RT: 17.009 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54

Instrument :

BNA\_N

ClientSampleId :

ICVBN062625





Tgt Ion:178 Resp: 7070

Ion Ratio Lower Upper

178 100

176 19.1 15.6 23.4

179 15.4 12.8 19.2

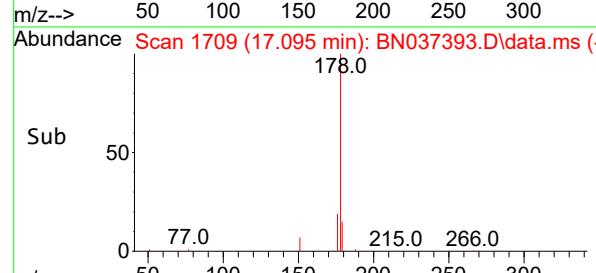

#26

Anthracene

Concen: 0.409 ng

RT: 17.095 min Scan# 1709

Delta R.T. -0.000 min

Lab File: BN037393.D

Acq: 26 Jun 2025 14:54


Tgt Ion:178 Resp: 6496


Ion Ratio Lower Upper

178 100

176 18.1 14.9 22.3

179 14.8 12.4 18.6





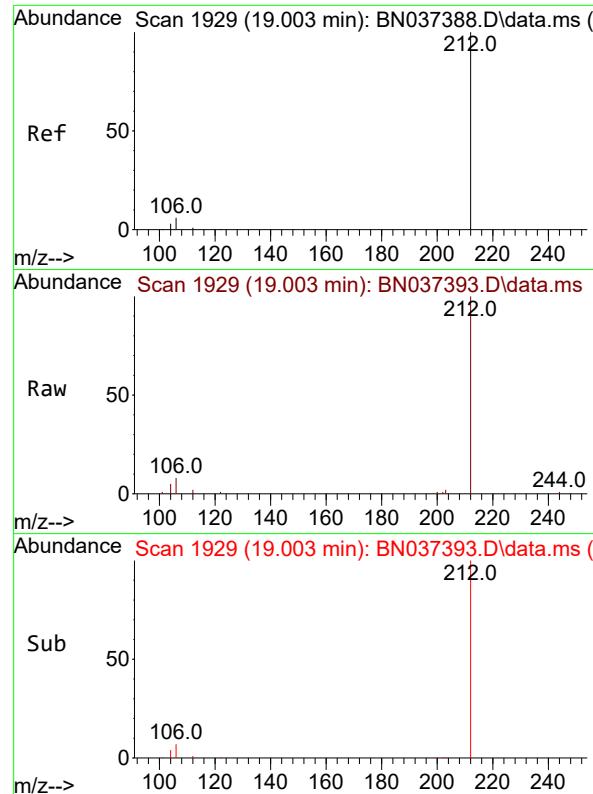

#27  
 Fluoranthene-d10  
 Concen: 0.391 ng  
 RT: 19.003 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54


Instrument : BNA\_N  
 ClientSampleId : ICVBN062625


Tgt Ion:212 Resp: 6867  
 Ion Ratio Lower Upper  
 212 100  
 106 6.5 4.5 6.7  
 104 3.9 2.7 4.1

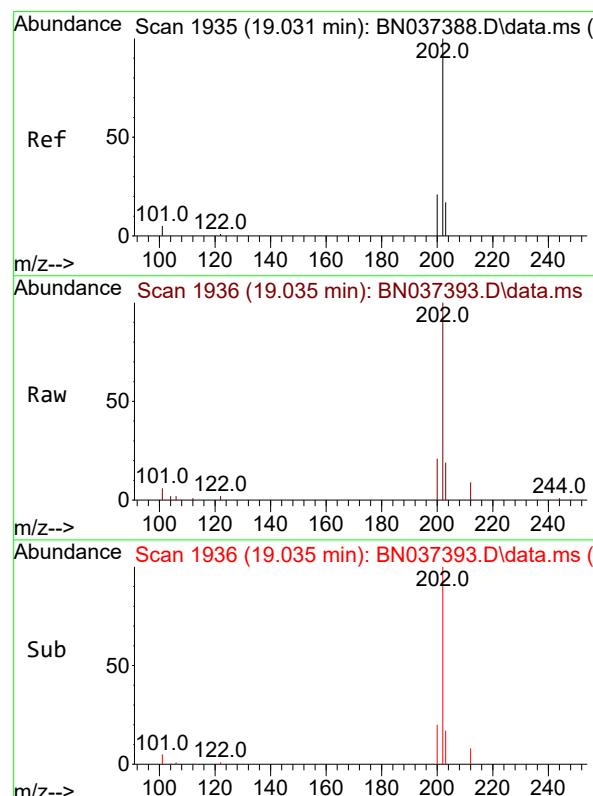

#28  
 Fluoranthene  
 Concen: 0.382 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. 0.005 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54

Tgt Ion:202 Resp: 8423  
 Ion Ratio Lower Upper  
 202 100  
 101 5.1 3.8 5.6  
 203 17.3 13.5 20.3


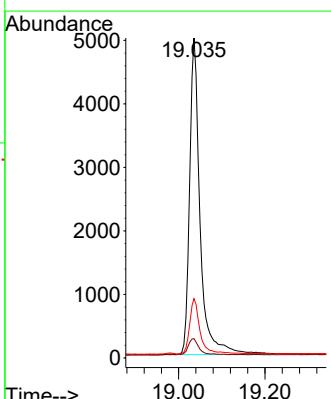


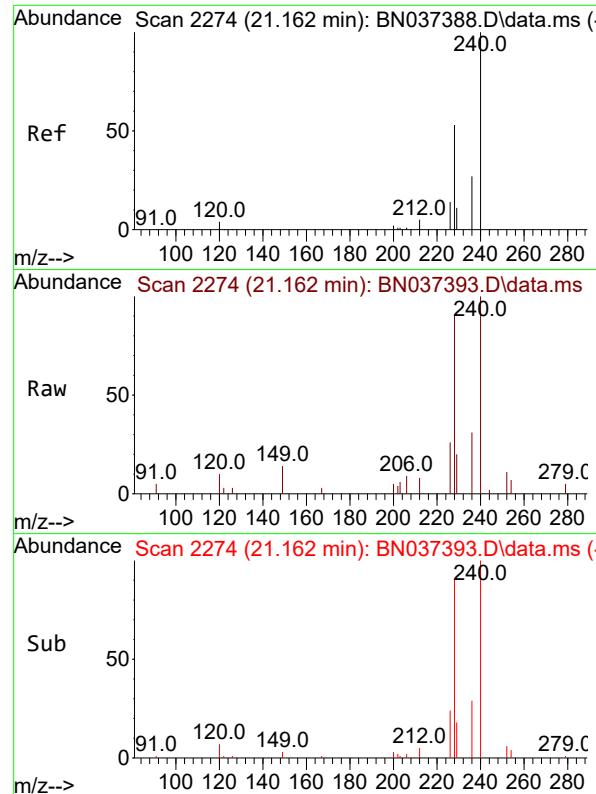

#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.162 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54


Instrument : BNA\_N  
ClientSampleId : ICVBN062625


Tgt Ion:240 Resp: 5019  
Ion Ratio Lower Upper  
240 100  
120 10.1 5.3 7.9#  
236 30.8 22.7 34.1

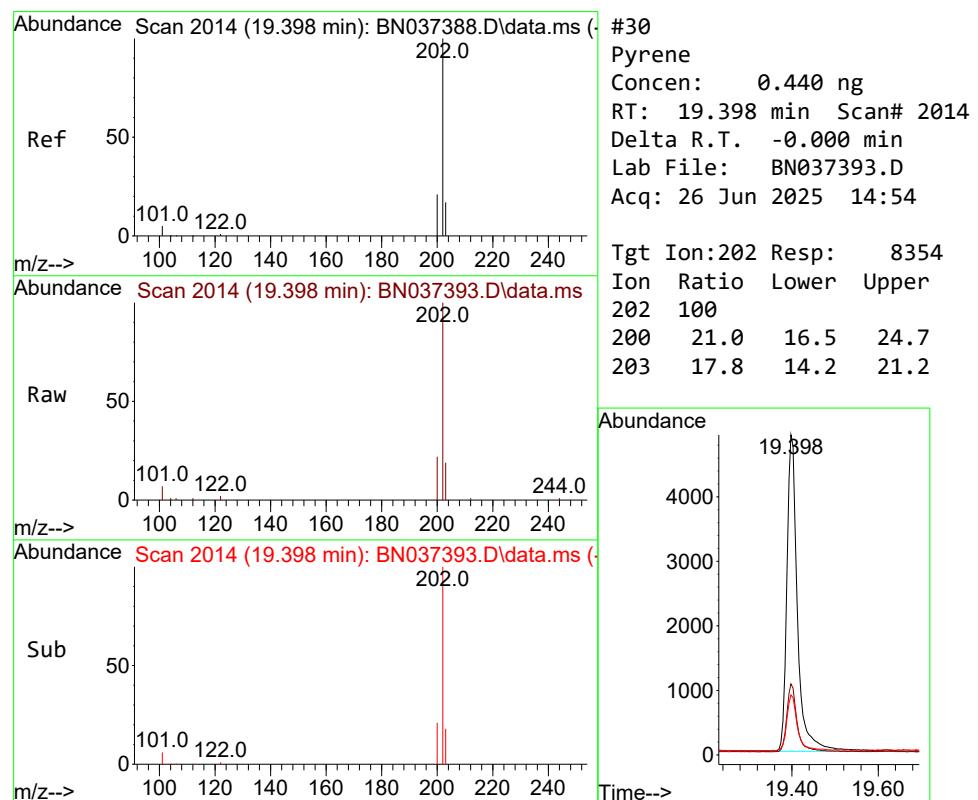

#30  
Pyrene  
Concen: 0.440 ng  
RT: 19.398 min Scan# 2014  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54



Tgt Ion:202 Resp: 8354  
Ion Ratio Lower Upper  
202 100  
200 21.0 16.5 24.7  
203 17.8 14.2 21.2

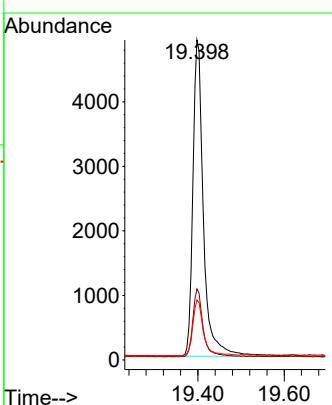

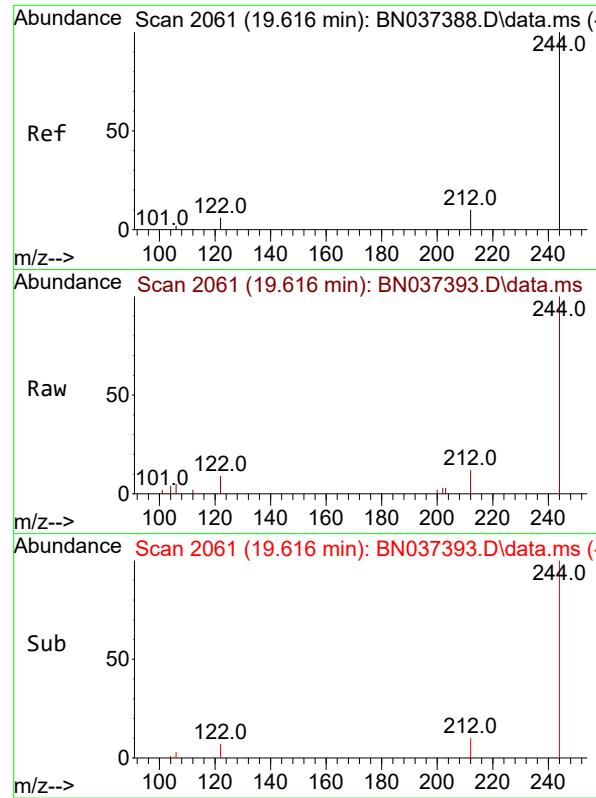


#31  
Terphenyl-d14  
Concen: 0.464 ng  
RT: 19.616 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54  
ClientSampleId : ICVBN062625


Tgt Ion:244 Resp: 4960  
Ion Ratio Lower Upper  
244 100  
212 11.6 9.1 13.7  
122 9.0 6.3 9.5

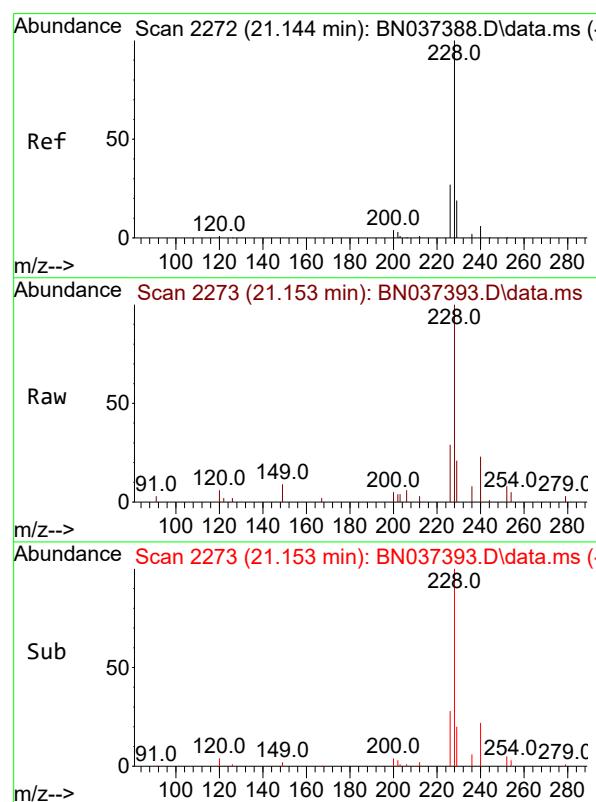

#32  
Benzo(a)anthracene  
Concen: 0.412 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.009 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54



Tgt Ion:228 Resp: 6494  
Ion Ratio Lower Upper  
228 100  
226 28.7 22.6 34.0  
229 21.0 16.2 24.2



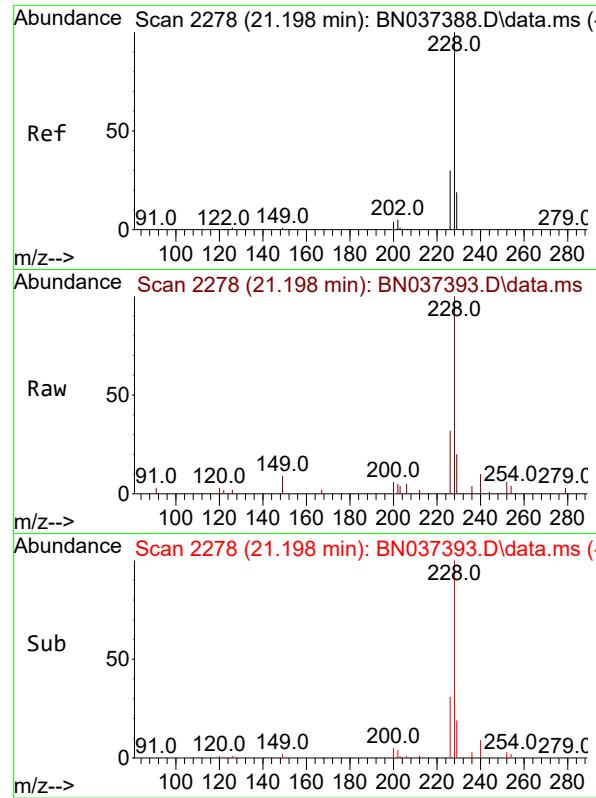


#33  
Chrysene  
Concen: 0.407 ng  
RT: 21.198 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54  
ClientSampleId : ICBN062625


Tgt Ion:228 Resp: 7943  
Ion Ratio Lower Upper  
228 100  
226 31.8 24.5 36.7  
229 20.1 16.1 24.1

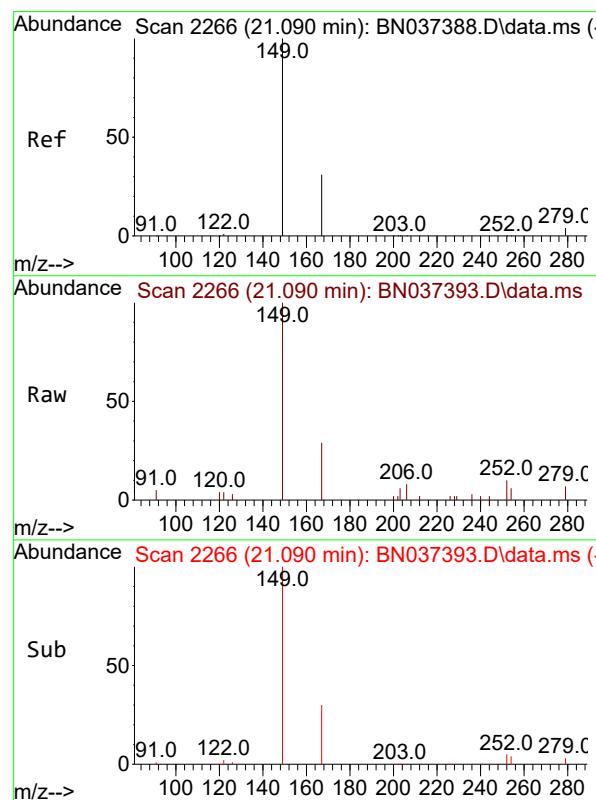

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.444 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. -0.000 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54

Tgt Ion:149 Resp: 2775  
Ion Ratio Lower Upper  
149 100  
167 30.4 24.8 37.2  
279 6.2 5.0 7.6





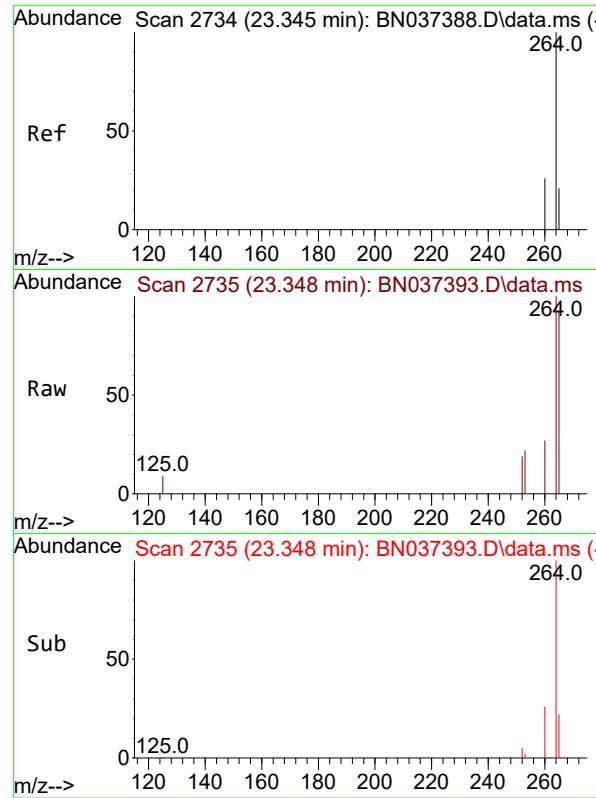

#35  
Perylene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 23.348 min Scan# 2  
Delta R.T. 0.003 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54


Instrument : BNA\_N  
ClientSampleId : ICVBN062625


Tgt Ion:264 Resp: 4884  
Ion Ratio Lower Upper  
264 100  
260 27.2 21.4 32.0  
265 91.7 56.2 84.4#

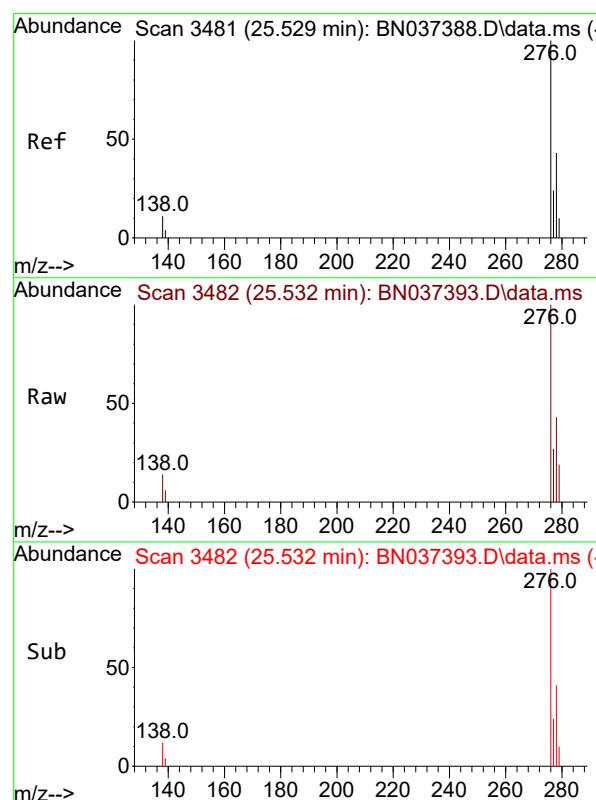

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.415 ng  
RT: 25.532 min Scan# 3482  
Delta R.T. 0.003 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54



Tgt Ion:276 Resp: 8543  
Ion Ratio Lower Upper  
276 100  
138 11.6 8.5 12.7  
277 22.6 19.7 29.5



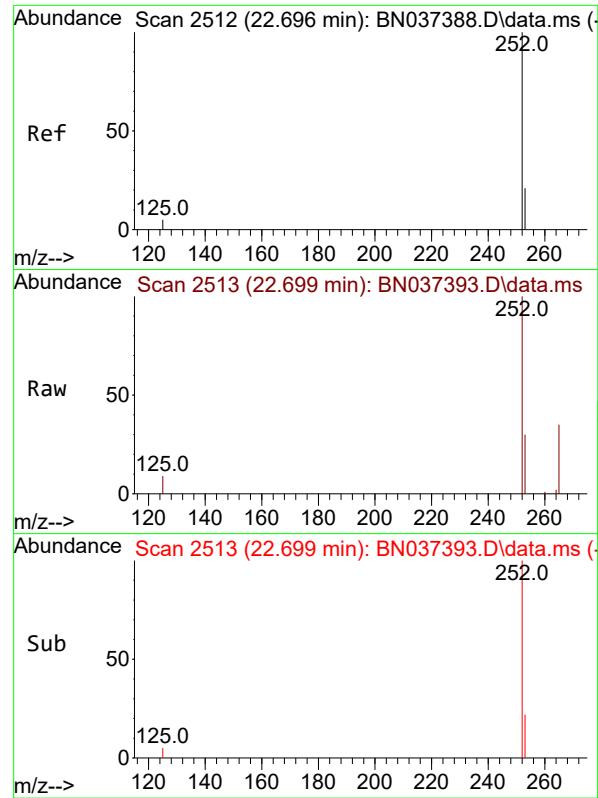


#37  
Benzo(b)fluoranthene  
Concen: 0.393 ng  
RT: 22.699 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.003 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54 ClientSampleId : ICVBN062625


Tgt Ion:252 Resp: 6764  
Ion Ratio Lower Upper  
252 100  
253 30.4 22.8 34.2  
125 9.3 6.2 9.4

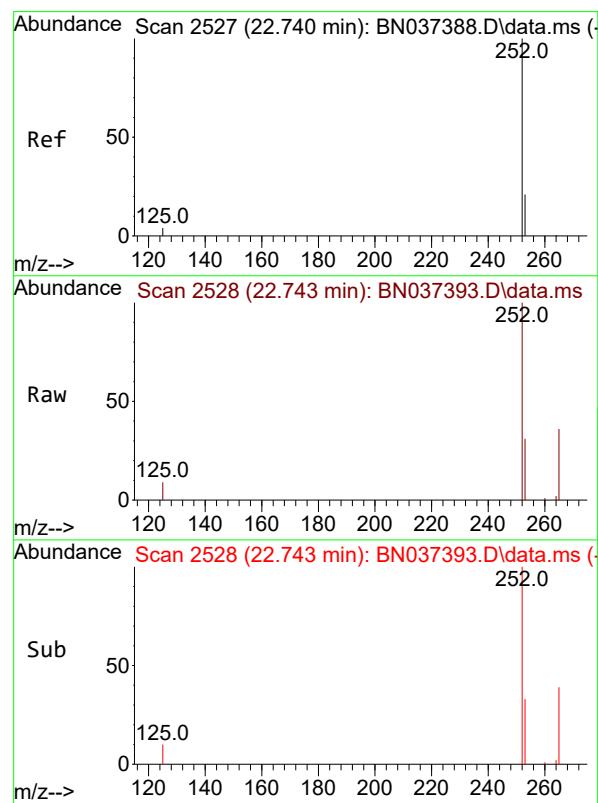

#38  
Benzo(k)fluoranthene  
Concen: 0.441 ng  
RT: 22.743 min Scan# 2528  
Delta R.T. 0.003 min  
Lab File: BN037393.D  
Acq: 26 Jun 2025 14:54

Tgt Ion:252 Resp: 8109  
Ion Ratio Lower Upper  
252 100  
253 30.8 23.2 34.8  
125 9.1 6.0 9.0#





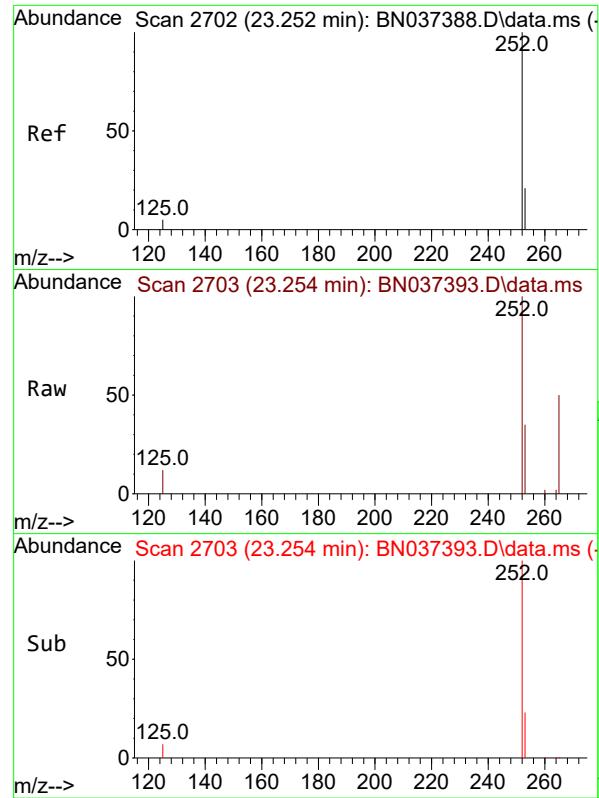

#39  
 Benzo(a)pyrene  
 Concen: 0.432 ng  
 RT: 23.254 min Scan# 2  
 Delta R.T. 0.003 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54


Instrument : BNA\_N  
 ClientSampleId : ICVBN062625


Tgt Ion:252 Resp: 6621  
 Ion Ratio Lower Upper  
 252 100  
 253 35.1 25.6 38.4  
 125 12.2 7.5 11.3#

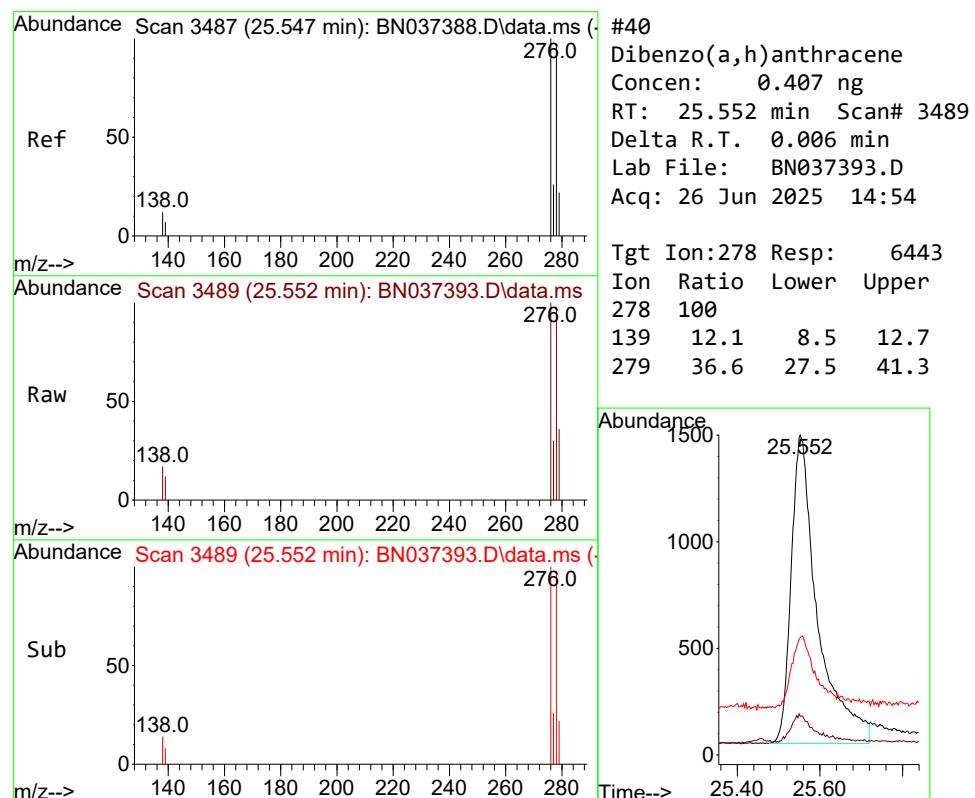

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.407 ng  
 RT: 25.552 min Scan# 3489  
 Delta R.T. 0.006 min  
 Lab File: BN037393.D  
 Acq: 26 Jun 2025 14:54

Tgt Ion:278 Resp: 6443  
 Ion Ratio Lower Upper  
 278 100  
 139 12.1 8.5 12.7  
 279 36.6 27.5 41.3



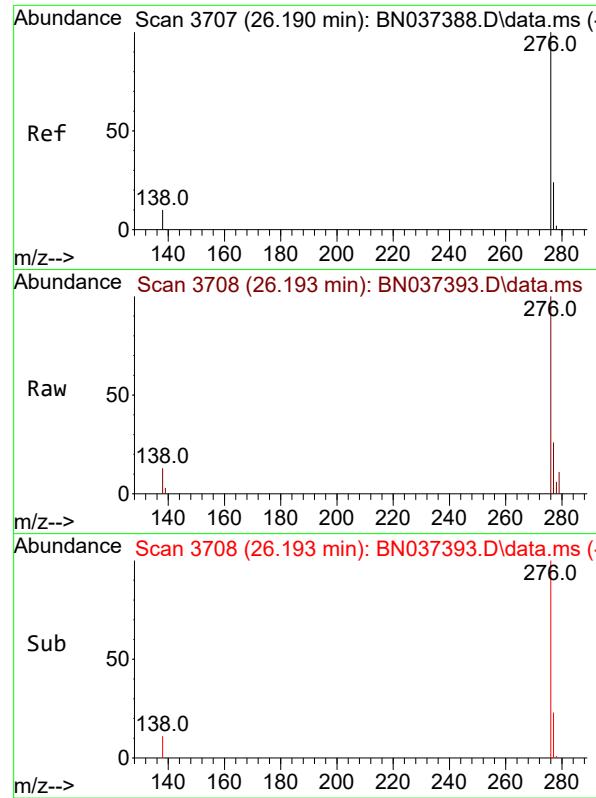

#41

Benzo(g,h,i)perylene

Concen: 0.397 ng

RT: 26.193 min Scan# 3

Instrument :

Delta R.T. 0.003 min

BNA\_N

Lab File: BN037393.D

ClientSampleId :

Acq: 26 Jun 2025 14:54

ICVBN062625


Tgt Ion:276 Resp: 7497

Ion Ratio Lower Upper

276 100

277 25.9 21.0 31.4

138 13.0 9.6 14.4

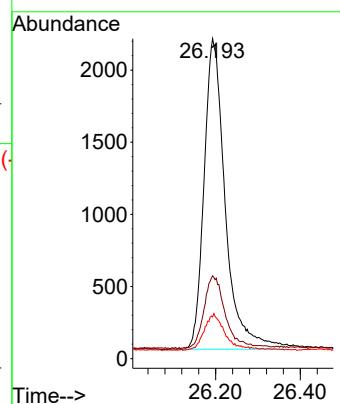

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037393.D  
 Acq On : 26 Jun 2025 14:54  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**ICVBN062625**

Quant Time: Jun 26 16:06:51 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	103	0.00
2	1,4-Dioxane	0.379	0.468	-23.5	130	0.00
3	n-Nitrosodimethylamine	0.375	0.390	-4.0	107	0.00
4 S	2-Fluorophenol	0.771	0.725	6.0	92	0.00
5 S	Phenol-d6	0.799	0.746	6.6	94	0.00
6	bis(2-Chloroethyl)ether	0.711	0.818	-15.0	117	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	106	0.00
8 S	Nitrobenzene-d5	0.321	0.340	-5.9	116	0.00
9	Naphthalene	1.030	1.070	-3.9	114	0.00
10	Hexachlorobutadiene	0.409	0.421	-2.9	108	0.00
11 SURR	2-Methylnaphthalene-d10	0.619	0.652	-5.3	120	0.00
12	2-Methylnaphthalene	0.709	0.651	8.2	101	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	101	0.00
14 S	2,4,6-Tribromophenol	0.235	0.203	13.6	85	0.00
15 S	2-Fluorobiphenyl	1.727	1.959	-13.4	114	0.00
16	Acenaphthylene	1.659	1.857	-11.9	119	0.00
17	Acenaphthene	1.083	1.121	-3.5	108	0.00
18	Fluorene	1.530	1.558	-1.8	106	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	98	0.01
20	4,6-Dinitro-2-methylphenol	0.103	0.081	21.4	93	0.01
21	4-Bromophenyl-phenylether	0.282	0.281	0.4	102	0.00
22	Hexachlorobenzene	0.303	0.324	-6.9	104	0.00
23	Atrazine	0.224	0.226	-0.9	104	0.00
24	Pentachlorophenol	0.164	0.126	23.2	80	0.00
25	Phenanthrene	1.127	1.154	-2.4	104	0.00
26	Anthracene	1.036	1.060	-2.3	107	0.00
27 SURR	Fluoranthene-d10	1.146	1.121	2.2	103	0.00
28	Fluoranthene	1.439	1.375	4.4	98	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	89	0.00
30	Pyrene	1.514	1.664	-9.9	97	0.00
31 S	Terphenyl-d14	0.853	0.988	-15.8	102	0.00
32	Benzo(a)anthracene	1.257	1.294	-2.9	99	0.00
33	Chrysene	1.556	1.583	-1.7	89	0.00
34	Bis(2-ethylhexyl)phthalate	0.498	0.553	-11.0	98	0.00
35 I	Perylene-d12	1.000	1.000	0.0	82	0.00
36	Indeno(1,2,3-cd)pyrene	1.686	1.749	-3.7	91	0.00
37	Benzo(b)fluoranthene	1.410	1.385	1.8	86	0.00
38	Benzo(k)fluoranthene	1.507	1.660	-10.2	93	0.00
39 C	Benzo(a)pyrene	1.254	1.356	-8.1	94	0.00
40	Dibenzo(a,h)anthracene	1.296	1.319	-1.8	89	0.00
41	Benzo(g,h,i)perylene	1.548	1.535	0.8	85	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037393.D  
 Acq On : 26 Jun 2025 14:54  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**ICVBN062625**

Quant Time: Jun 26 16:06:51 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	103	0.00
2	1,4-Dioxane	0.400	0.493	-23.2	130	0.00
3	n-Nitrosodimethylamine	0.400	0.417	-4.2	107	0.00
4 S	2-Fluorophenol	0.400	0.376	6.0	92	0.00
5 S	Phenol-d6	0.400	0.373	6.8	94	0.00
6	bis(2-Chloroethyl)ether	0.400	0.460	-15.0	117	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	106	0.00
8 S	Nitrobenzene-d5	0.400	0.425	-6.2	116	0.00
9	Naphthalene	0.400	0.416	-4.0	114	0.00
10	Hexachlorobutadiene	0.400	0.412	-3.0	108	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.421	-5.2	120	0.00
12	2-Methylnaphthalene	0.400	0.367	8.3	101	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	101	0.00
14 S	2,4,6-Tribromophenol	0.400	0.347	13.3	85	0.00
15 S	2-Fluorobiphenyl	0.400	0.454	-13.5	114	0.00
16	Acenaphthylene	0.400	0.448	-12.0	119	0.00
17	Acenaphthene	0.400	0.414	-3.5	108	0.00
18	Fluorene	0.400	0.407	-1.7	106	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	98	0.01
20	4,6-Dinitro-2-methylphenol	0.400	0.316	21.0	93	0.01
21	4-Bromophenyl-phenylether	0.400	0.398	0.5	102	0.00
22	Hexachlorobenzene	0.400	0.427	-6.7	104	0.00
23	Atrazine	0.400	0.404	-1.0	104	0.00
24	Pentachlorophenol	0.400	0.309	22.8	80	0.00
25	Phenanthrene	0.400	0.410	-2.5	104	0.00
26	Anthracene	0.400	0.409	-2.2	107	0.00
27 SURR	Fluoranthene-d10	0.400	0.391	2.3	103	0.00
28	Fluoranthene	0.400	0.382	4.5	98	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	89	0.00
30	Pyrene	0.400	0.440	-10.0	97	0.00
31 S	Terphenyl-d14	0.400	0.464	-16.0	102	0.00
32	Benzo(a)anthracene	0.400	0.412	-3.0	99	0.00
33	Chrysene	0.400	0.407	-1.7	89	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.444	-11.0	98	0.00
35 I	Perylene-d12	0.400	0.400	0.0	82	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.415	-3.7	91	0.00
37	Benzo(b)fluoranthene	0.400	0.393	1.8	86	0.00
38	Benzo(k)fluoranthene	0.400	0.441	-10.2	93	0.00
39 C	Benzo(a)pyrene	0.400	0.432	-8.0	94	0.00
40	Dibenzo(a,h)anthracene	0.400	0.407	-1.7	89	0.00
41	Benzo(g,h,i)perylene	0.400	0.397	0.8	85	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

7C

## SEMIVOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>CHEMTECH</u>		Contract:	<u>TETR06</u>	
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q2375</u>	SAS No.:	<u>Q2375</u>
Instrument ID:	<u>BNA_N</u>		Calibration Date/Time:	<u>06/21/2025</u>	<u>01:17</u>
Lab File ID:	<u>BN037365.D</u>		Init. Calib. Date(s):	<u>06/20/2025</u>	<u>06/20/2025</u>
EPA Sample No.:	<u>SSTDCCC0.4EC</u>		Init. Calib. Time(s):	<u>16:51</u>	<u>20:27</u>
GC Column:	<u>ZB-GR</u>	ID: <u>0.25</u>	(mm)		

COMPOUND	RRF	RRF0.4	MIN RRF	%D	MAX%D
2-Methylnaphthalene-d10	0.648	0.670		3.4	50.0
Fluoranthene-d10	1.148	1.189		3.6	50.0
2-Fluorophenol	0.799	0.740		-7.4	50.0
Phenol-d6	0.823	0.753		-8.5	50.0
Nitrobenzene-d5	0.323	0.318		-1.5	50.0
2-Fluorobiphenyl	1.757	1.777		1.1	50.0
2,4,6-Tribromophenol	0.235	0.218		-7.2	50.0
Terphenyl-d14	0.912	0.903		-1.0	50.0
1,4-Dioxane	0.407	0.399		-2.0	50.0

All other compounds must meet a minimum RRF of 0.010.

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037365.D  
 Acq On : 21 Jun 2025 01:17  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4EC

Quant Time: Jun 21 01:41:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1894	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4150	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2786	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5748	0.400	ng	# 0.00
29) Chrysene-d12	21.162	240	5140	0.400	ng	0.00
35) Perylene-d12	23.351	264	5682	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1402	0.370	ng	0.00
5) Phenol-d6	6.752	99	1426	0.366	ng	0.00
8) Nitrobenzene-d5	8.717	82	1321	0.394	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	2780	0.413	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	608	0.372	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	4951	0.405	ng	0.00
27) Fluoranthene-d10	19.008	212	6836	0.414	ng	0.00
31) Terphenyl-d14	19.616	244	4639	0.396	ng	0.00
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) 1,4-Dioxane	3.104	88	755	0.392	ng	95
3) n-Nitrosodimethylamine	3.422	42	701	0.397	ng	# 78
6) bis(2-Chloroethyl)ether	7.004	93	1274	0.368	ng	100
9) Naphthalene	10.394	128	4308	0.393	ng	# 90
10) Hexachlorobutadiene	10.682	225	1876	0.434	ng	# 100
12) 2-Methylnaphthalene	12.021	142	2941	0.385	ng	93
16) Acenaphthylene	13.935	152	4498	0.384	ng	98
17) Acenaphthene	14.277	154	2949	0.383	ng	98
18) Fluorene	15.272	166	4167	0.385	ng	99
20) 4,6-Dinitro-2-methylph...	15.379	198	483	0.350	ng	85
21) 4-Bromophenyl-phenylether	16.177	248	1621	0.396	ng	# 94
22) Hexachlorobenzene	16.276	284	1819	0.408	ng	99
23) Atrazine	16.450	200	1187	0.364	ng	# 87
24) Pentachlorophenol	16.624	266	805	0.363	ng	96
25) Phenanthrene	17.009	178	6282	0.377	ng	99
26) Anthracene	17.108	178	5522	0.360	ng	99
28) Fluoranthene	19.036	202	8102	0.385	ng	98
30) Pyrene	19.403	202	8105	0.388	ng	100
32) Benzo(a)anthracene	21.153	228	6359	0.376	ng	98
33) Chrysene	21.198	228	8015	0.391	ng	98
34) Bis(2-ethylhexyl)phtha...	21.090	149	2672	0.385	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.535	276	9725	0.382	ng	# 92
37) Benzo(b)fluoranthene	22.696	252	7592m	0.363	ng	
38) Benzo(k)fluoranthene	22.740	252	9018	0.398	ng	94
39) Benzo(a)pyrene	23.255	252	7122	0.380	ng	# 90
40) Dibenzo(a,h)anthracene	25.553	278	7424	0.388	ng	# 85
41) Benzo(g,h,i)perylene	26.199	276	8859	0.389	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037365.D  
 Acq On : 21 Jun 2025 01:17  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1


Quant Time: Jun 21 01:41:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4EC

### Manual Integrations APPROVED


Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

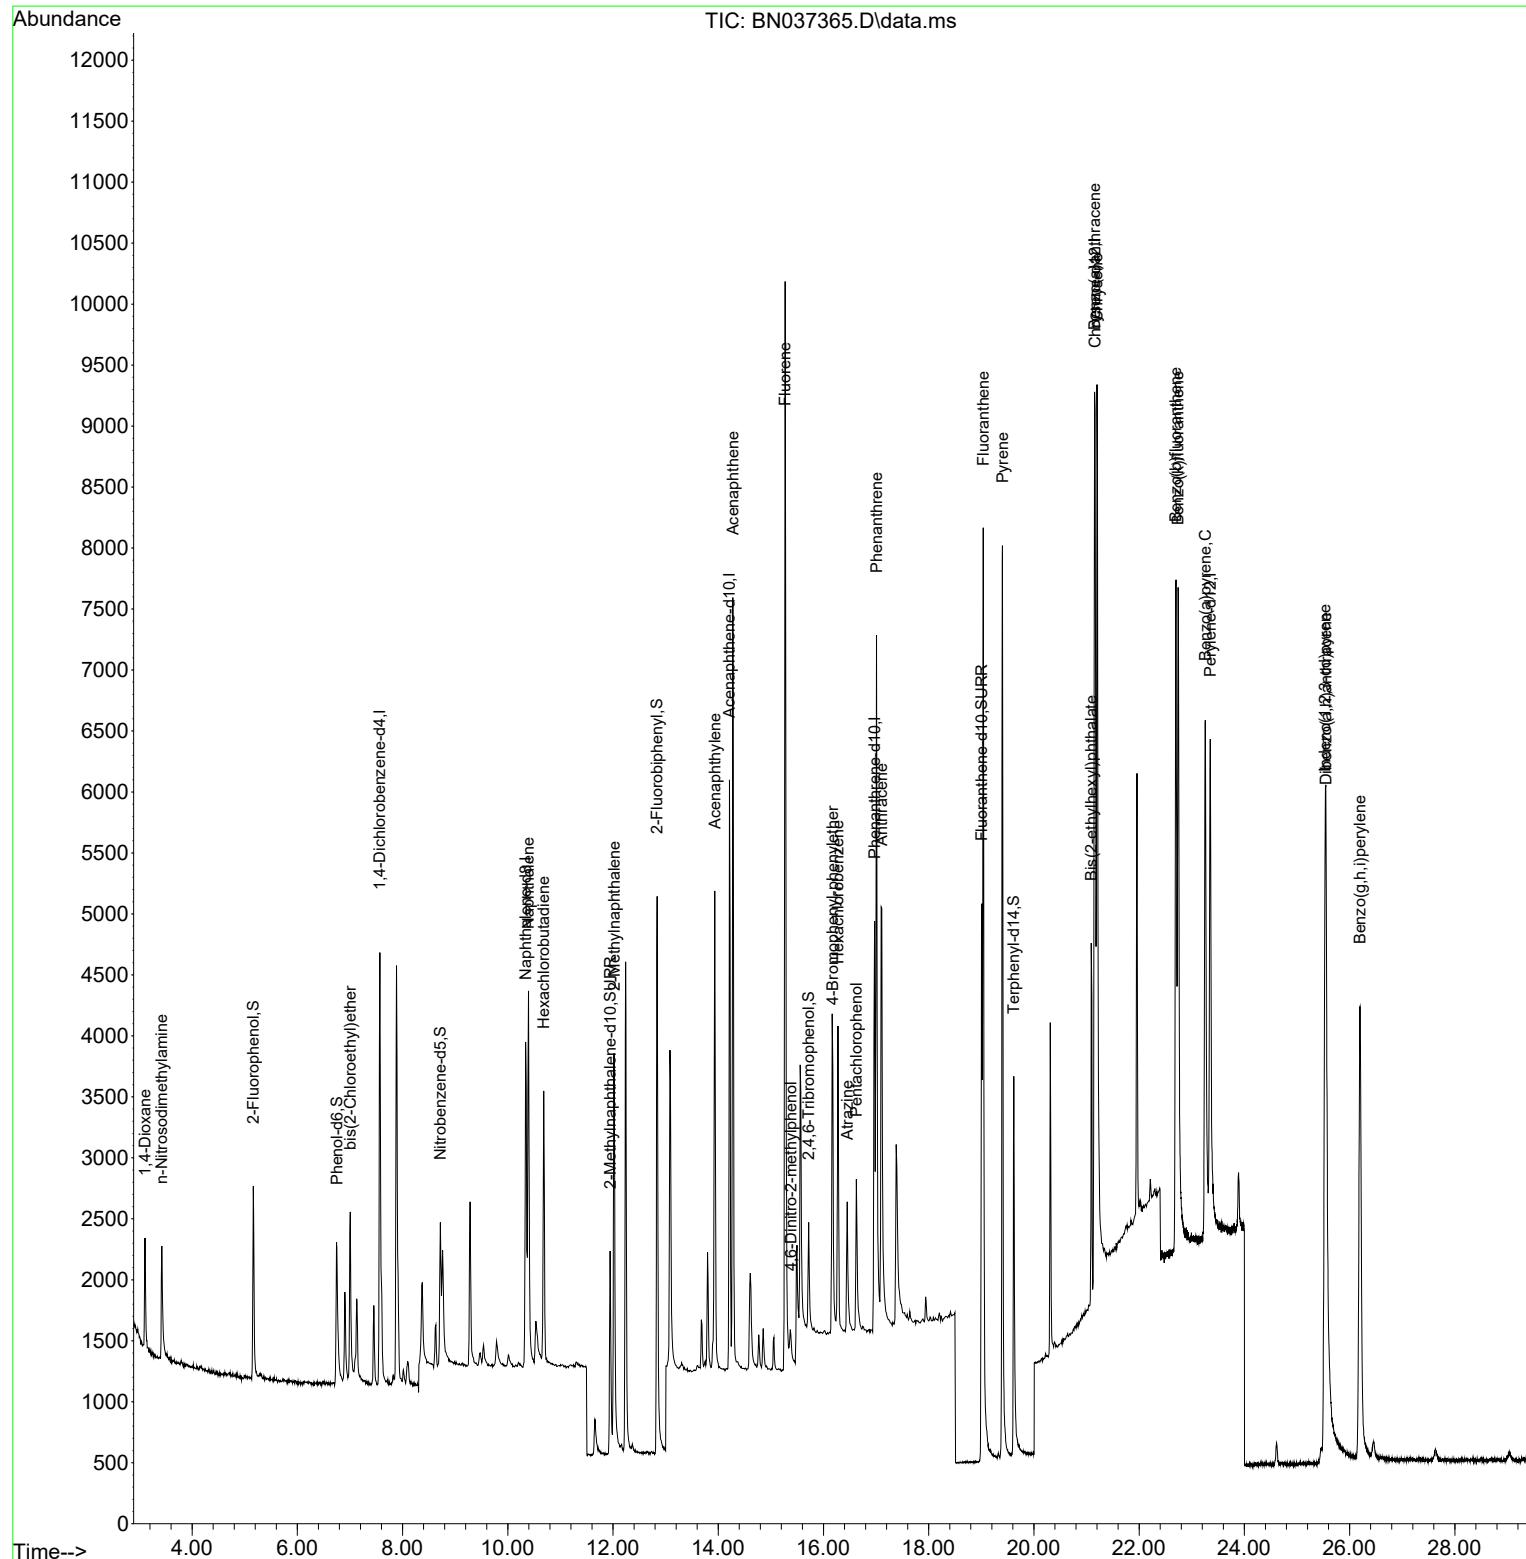

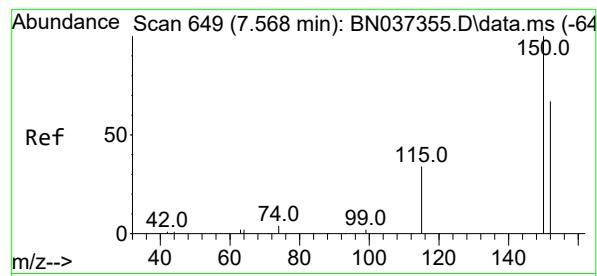

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17




Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC




Tgt Ion:152 Resp: 189.4  
Ion Ratio Lower Upper  
152 100  
150 149.8 112.7 169.1  
115 55.5 45.9 68.9

Manual Integrations APPROVED



Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025


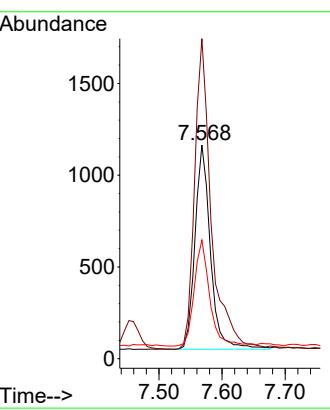
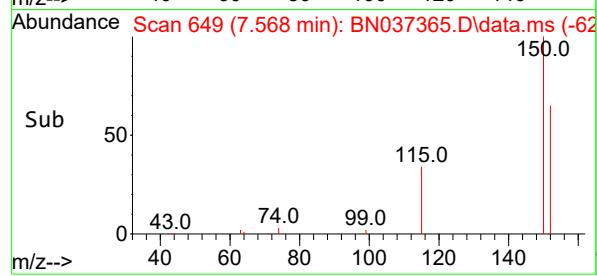


#2  
1,4-Dioxane  
Concen: 0.392 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17



Tgt Ion: 88 Resp: 755  
Ion Ratio Lower Upper  
88 100  
43 22.8 21.0 31.6  
58 49.9 38.0 57.0

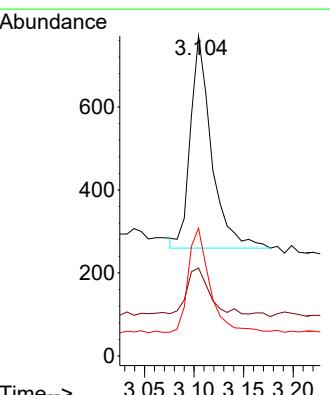

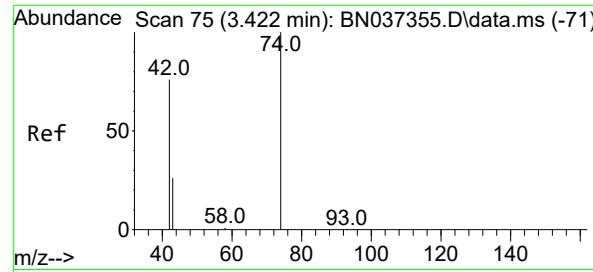

#3

n-Nitrosodimethylamine

Concen: 0.397 ng

RT: 3.422 min Scan# 7

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N




ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#4

2-Fluorophenol

Concen: 0.370 ng

RT: 5.163 min Scan# 316

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Tgt Ion:112 Resp: 1402

Ion Ratio Lower Upper



112 100







64 52.2 38.7 58.1

63 31.0 26.4 39.6

Time--&gt; 3.30 3.40 3.50

Time--&gt; 5.10 5.20 5.30

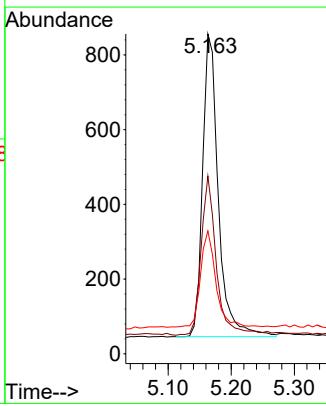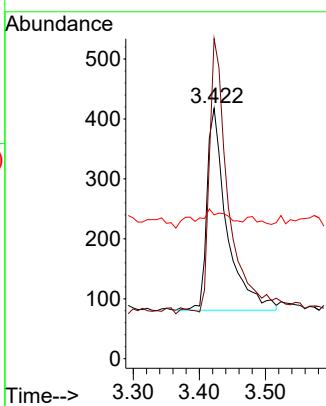



#5

Phenol-d6

Concen: 0.366 ng

RT: 6.752 min Scan# 5

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N


ClientSampleId :

SSTDCCC0.4EC

### Manual Integrations APPROVED


Reviewed By :Rahul Chavli 06/23/2025




Supervised By :Jagrut Upadhyay 06/24/2025

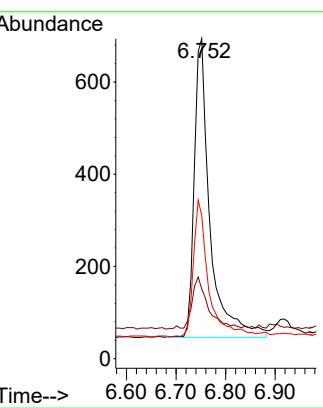

#6  
bis(2-Chloroethyl)ether  
Concen: 0.368 ng  
RT: 7.004 min Scan# 571  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion: 93 Resp: 1274  
Ion Ratio Lower Upper  
93 100  
63 66.6 53.2 79.8  
95 33.8 27.3 40.9

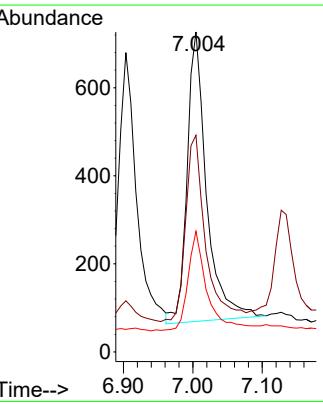


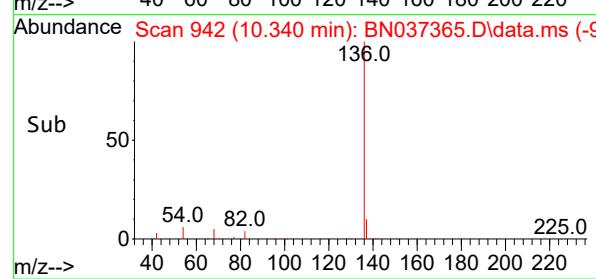




#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.340 min Scan# 9  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC


### Manual Integrations APPROVED


Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

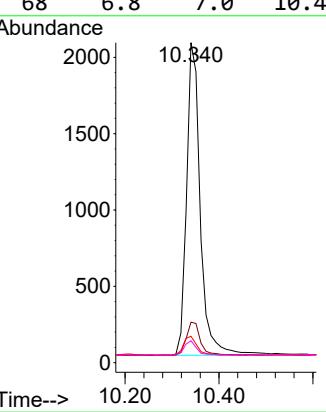

#8  
Nitrobenzene-d5  
Concen: 0.394 ng  
RT: 8.717 min Scan# 790  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion: 82 Resp: 1321  
Ion Ratio Lower Upper  
82 100  
128 41.4 42.5 63.7#  
54 44.6 43.2 64.8

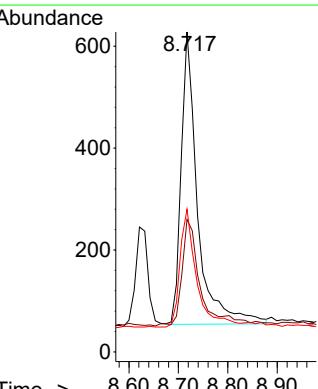

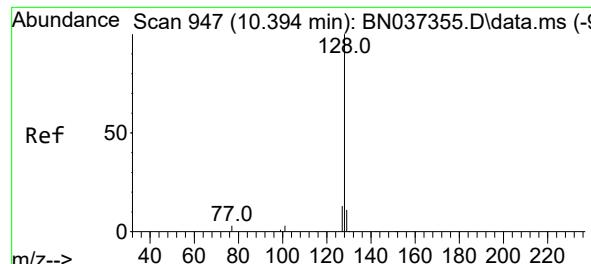

#9

Naphthalene

Concen: 0.393 ng

RT: 10.394 min Scan# 9

Delta R.T. 0.000 min

Lab File: BN037365.D


Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC

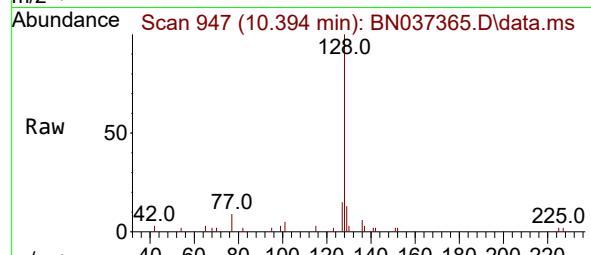

Tgt Ion:128 Resp: 4308

Ion Ratio Lower Upper

128 100

129 12.7 14.0 21.0




127 15.2 15.8 23.8

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

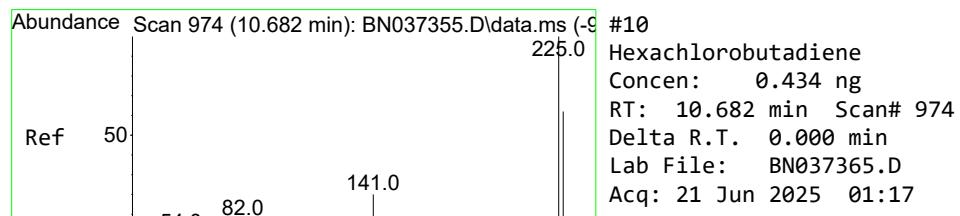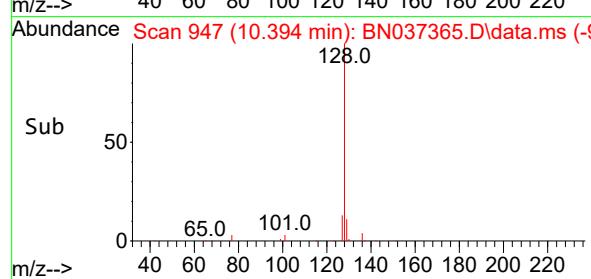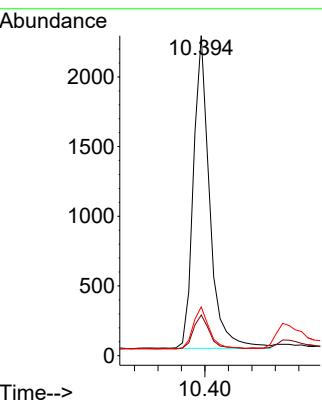

#10

Hexachlorobutadiene

Concen: 0.434 ng

RT: 10.682 min Scan# 974

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17



Tgt Ion:225 Resp: 1876

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 62.9 50.3 75.5


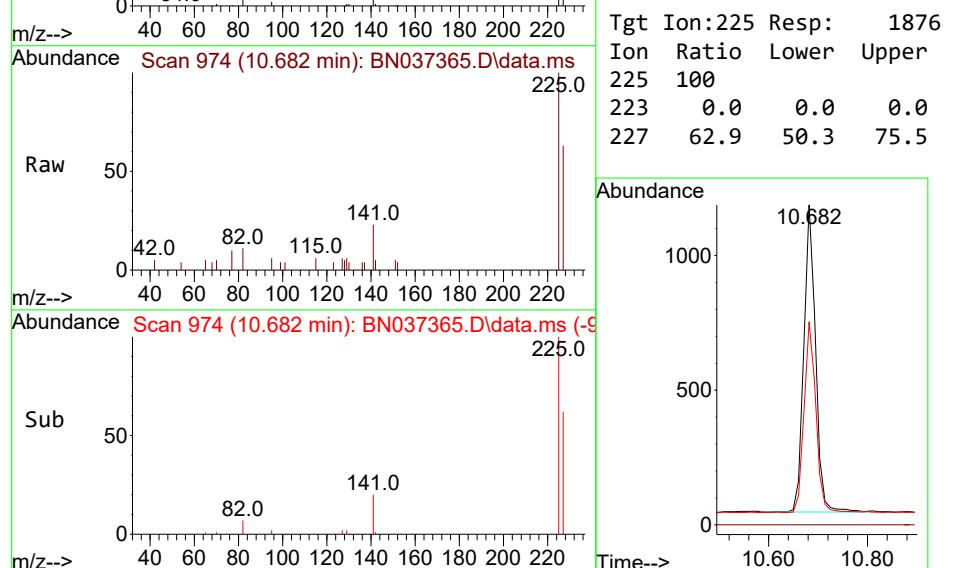
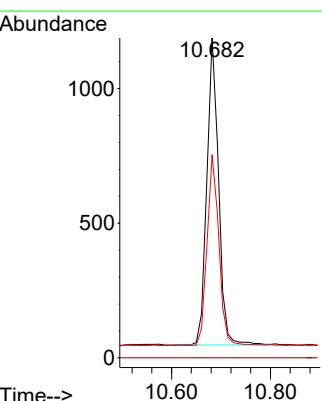


Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC

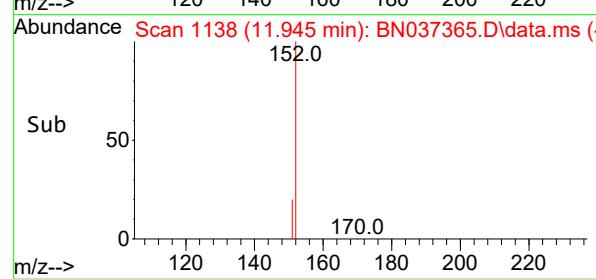




#11  
2-Methylnaphthalene-d10  
Concen: 0.413 ng  
RT: 11.945 min Scan# 1138  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025



#12  
2-Methylnaphthalene  
Concen: 0.385 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion:142 Resp: 2941  
Ion Ratio Lower Upper  
142 100  
141 90.9 70.2 105.2  
115 43.9 43.0 64.4

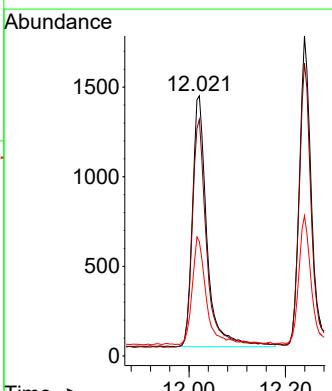

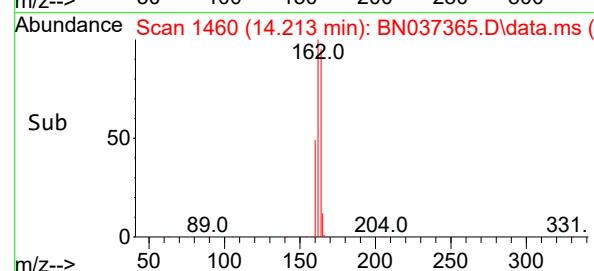

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1460

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N


ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#14

2,4,6-Tribromophenol

Concen: 0.372 ng

RT: 15.718 min Scan# 1598

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17





Tgt Ion:330 Resp: 608




Ion Ratio Lower Upper

330 100

332 102.3 78.4 117.6

141 35.9 24.4 36.6

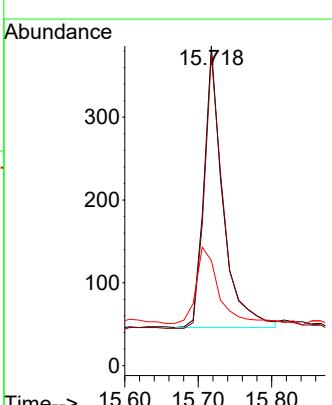



#15

2-Fluorobiphenyl

Concen: 0.405 ng

RT: 12.838 min Scan# 1314

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17





Instrument : BNA\_N

ClientSampleId : SSTDCCC0.4EC

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

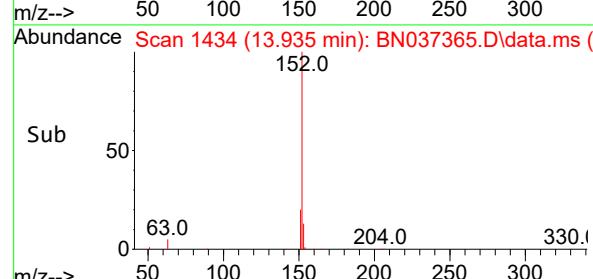

#16

Acenaphthylene

Concen: 0.384 ng


RT: 13.935 min Scan# 1434




Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Tgt	Ion:152	Resp:	4498
Ion	Ratio	Lower	Upper
152	100		
151	19.8	16.6	24.8
153	13.1	10.2	15.2

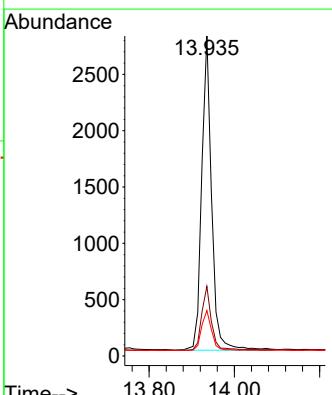



#17

Acenaphthene

Concen: 0.383 ng

RT: 14.277 min Scan# 1466

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17





Instrument : BNA\_N

ClientSampleId : SSTDCCC0.4EC

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

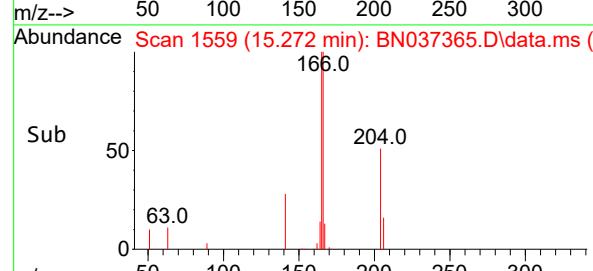

#18

Fluorene

Concen: 0.385 ng


RT: 15.272 min Scan# 1559


Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Tgt	Ion:166	Resp:	4167
Ion	Ratio	Lower	Upper
166	100		
165	100.6	79.5	119.3
167	13.8	10.7	16.1

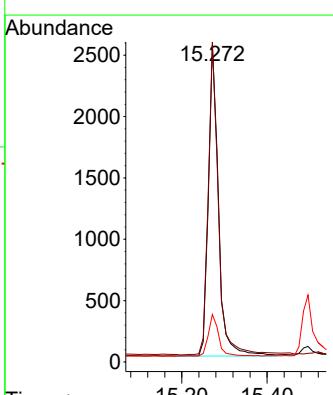

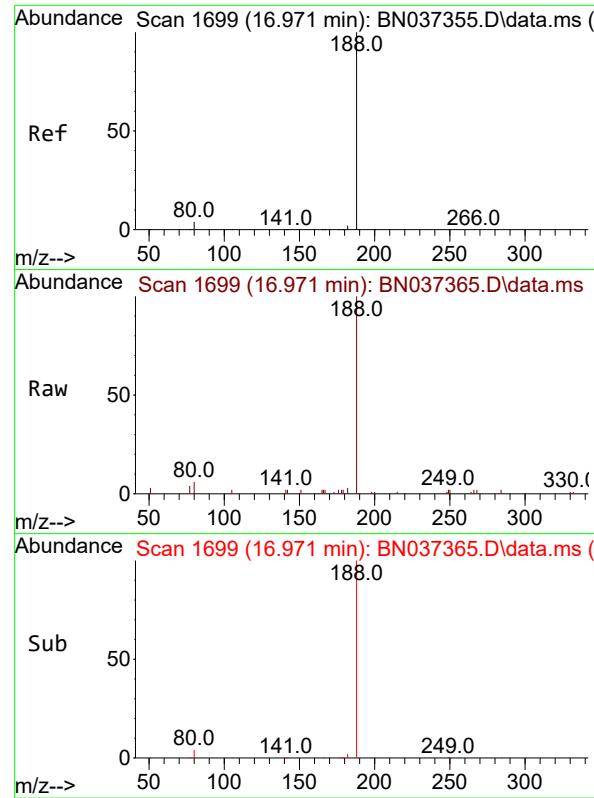

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N


ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

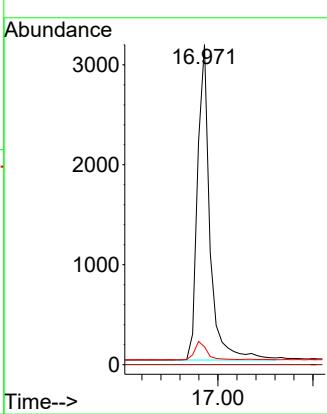

#20

4,6-Dinitro-2-methylphenol

Concen: 0.350 ng

RT: 15.379 min Scan# 1569

Delta R.T. 0.011 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17


Tgt Ion:198 Resp: 483


Ion Ratio Lower Upper

198 100

51 52.1 51.4 77.0

105 45.9 45.5 68.3




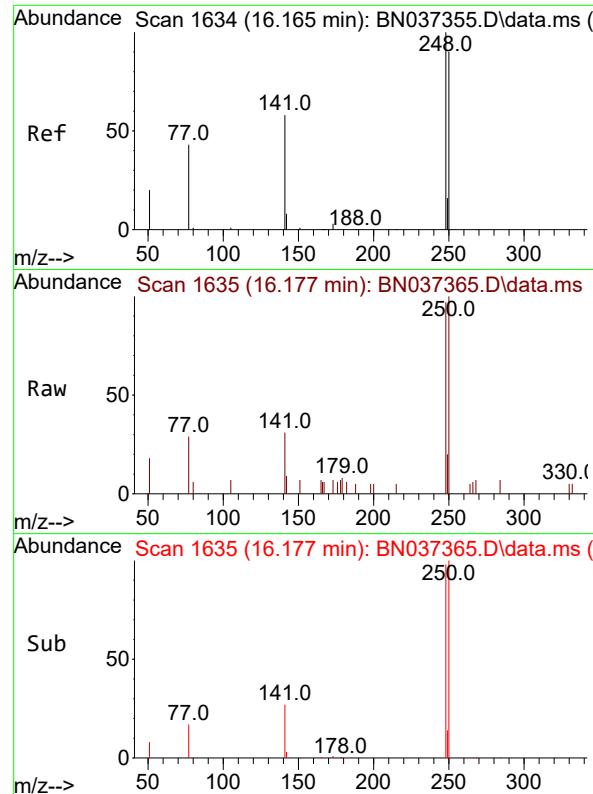


#21  
4-Bromophenyl-phenylether  
Concen: 0.396 ng  
RT: 16.177 min Scan# 1  
Delta R.T. 0.012 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

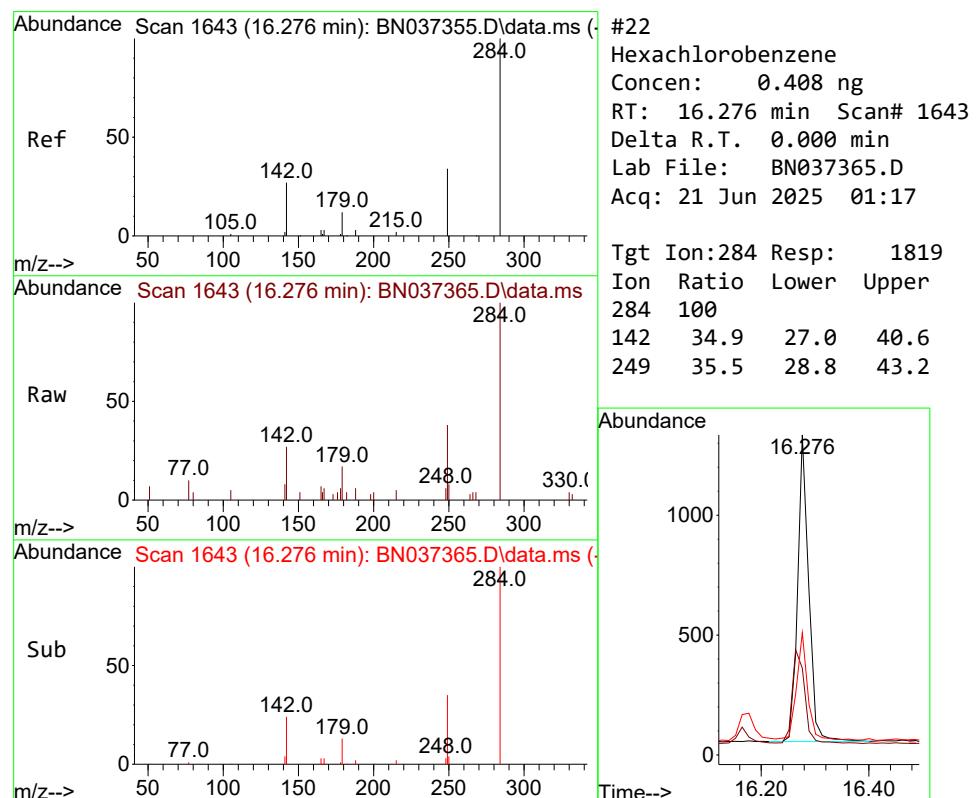

#22  
Hexachlorobenzene  
Concen: 0.408 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion:284 Resp: 1819  
Ion Ratio Lower Upper  
284 100  
142 34.9 27.0 40.6  
249 35.5 28.8 43.2









#23

Atrazine  
Concen: 0.364 ng  
RT: 16.450 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Instrument :  
BNA\_N  
ClientSampleId :  
SSTDCCC0.4EC

### Manual Integrations APPROVED


Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

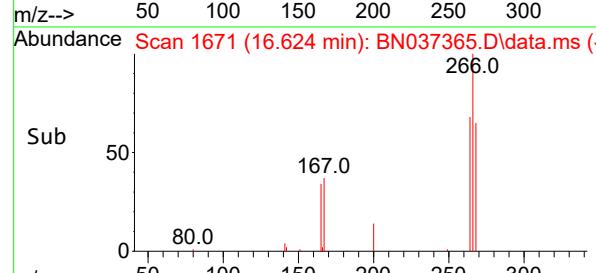




#24

Pentachlorophenol  
Concen: 0.363 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion:266 Resp: 805  
Ion Ratio Lower Upper  
266 100  
264 65.6 50.3 75.5  
268 66.2 55.3 82.9

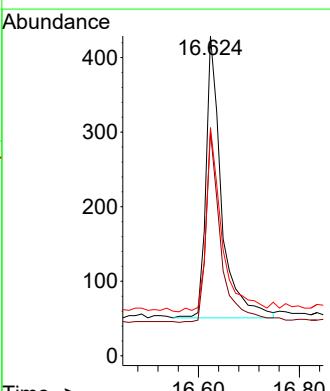

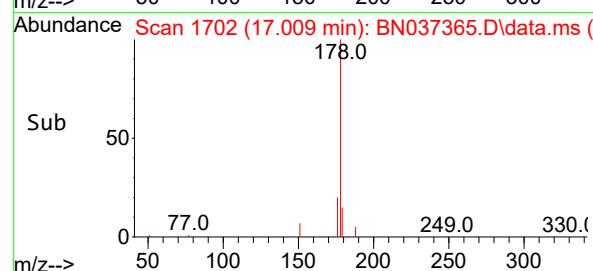

#25

Phenanthrene

Concen: 0.377 ng

RT: 17.009 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N





ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

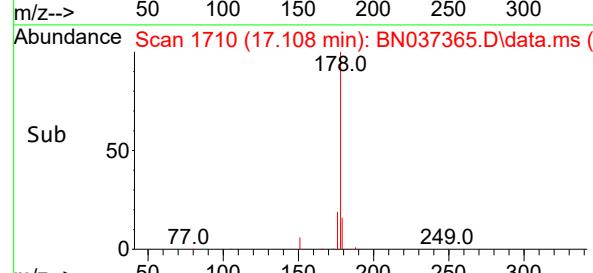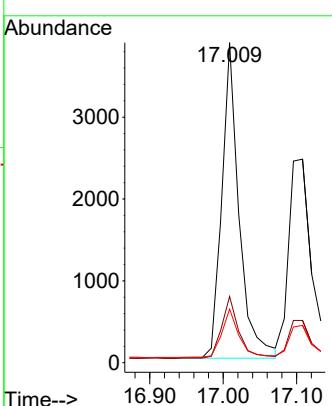

#26

Anthracene

Concen: 0.360 ng

RT: 17.108 min Scan# 1710

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17


Tgt Ion:178 Resp: 5522


Ion Ratio Lower Upper

178 100

176 19.0 14.7 22.1

179 16.2 13.0 19.6

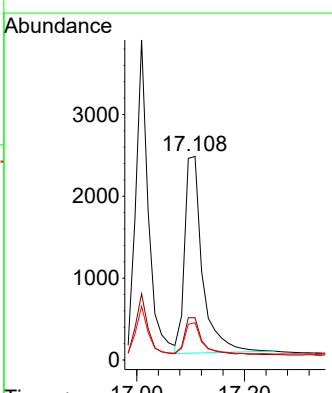

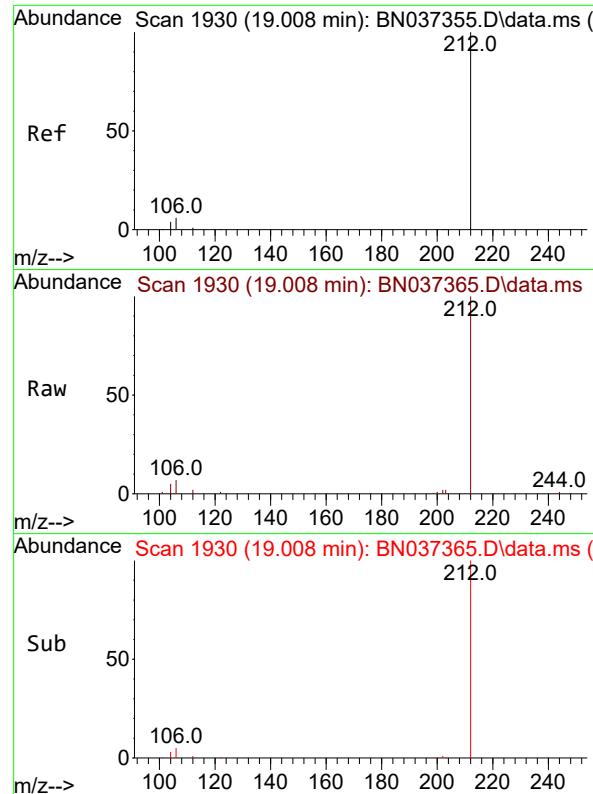

#27

Fluoranthene-d10

Concen: 0.414 ng

RT: 19.008 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:212 Resp: 6830

Ion Ratio Lower Upper

212 100

106 5.5 3.0 4.4


104 3.4 2.0 3.0

Manual Integrations

APPROVED

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#28

Fluoranthene

Concen: 0.385 ng

RT: 19.036 min Scan# 1936

Delta R.T. -0.005 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17



Tgt Ion:202 Resp: 8102




Ion Ratio Lower Upper

202 100

101 4.5 3.0 4.6

203 16.4 13.7 20.5

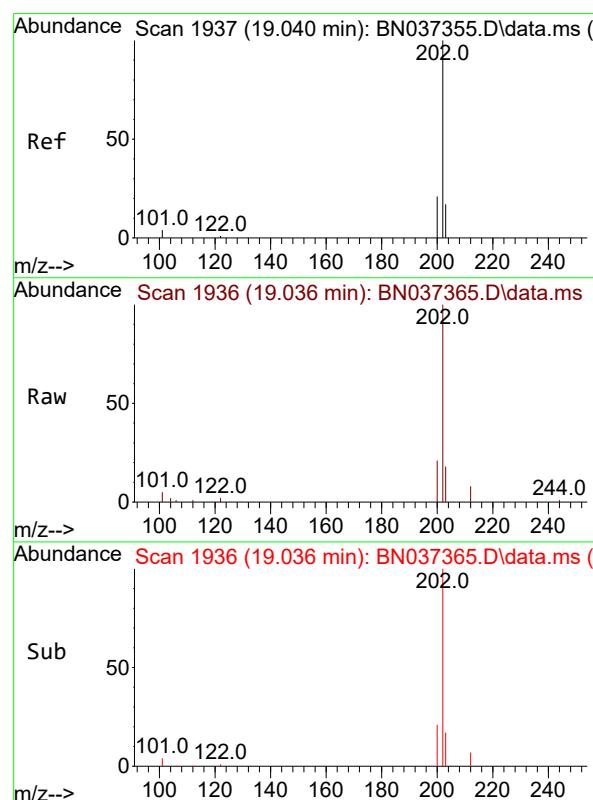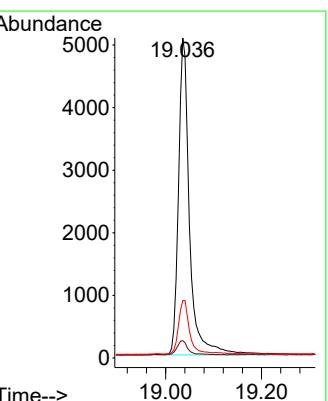

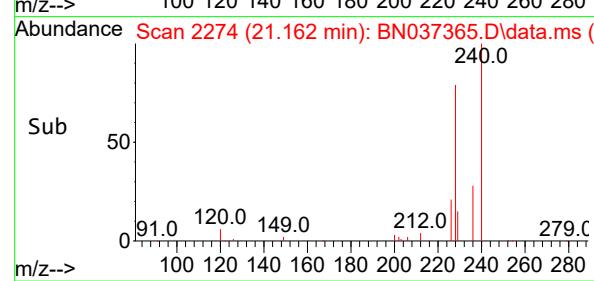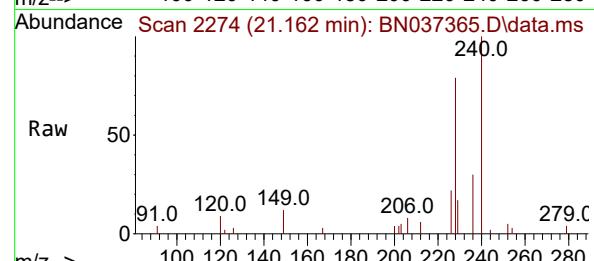

#29

Chrysene-d<sub>12</sub>

Concen: 0.400 ng

RT: 21.162 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N





ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

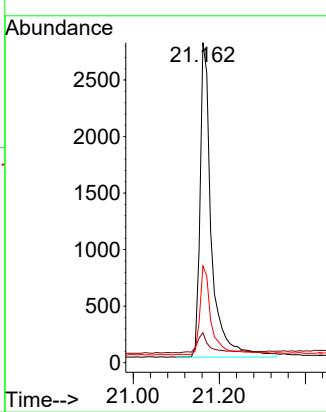

#30

Pyrene

Concen: 0.388 ng


RT: 19.403 min Scan# 2015


Delta R.T. 0.000 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Tgt	Ion:202	Resp:	8105
Ion	Ratio	Lower	Upper
202	100		
200	21.0	16.8	25.2
203	17.7	14.5	21.7

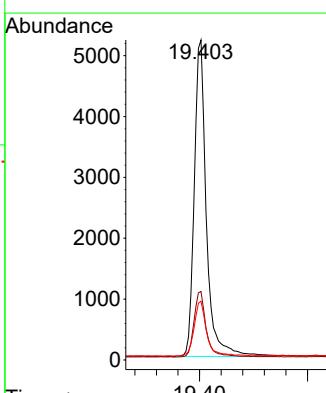


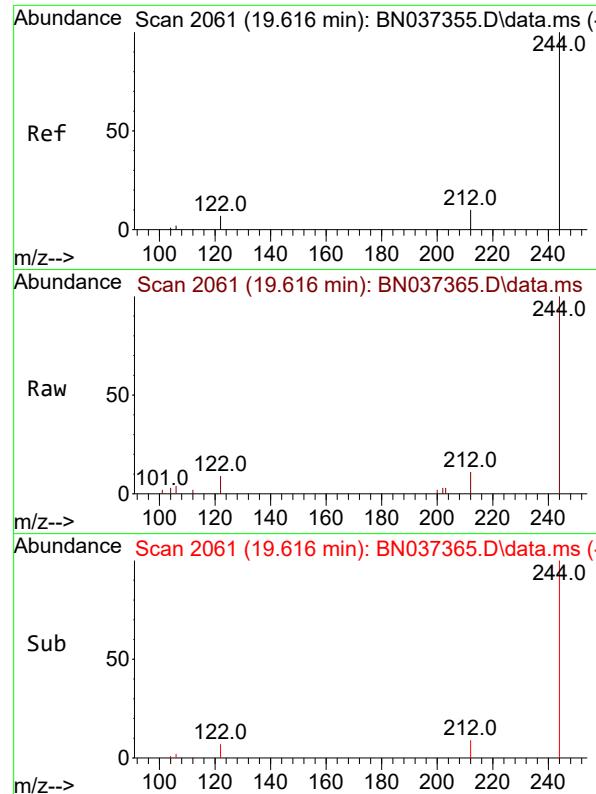


#31  
Terphenyl-d14  
Concen: 0.396 ng  
RT: 19.616 min Scan# 2  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Instrument :  
BNA\_N  
ClientSampleId :  
SSTDCCC0.4EC


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

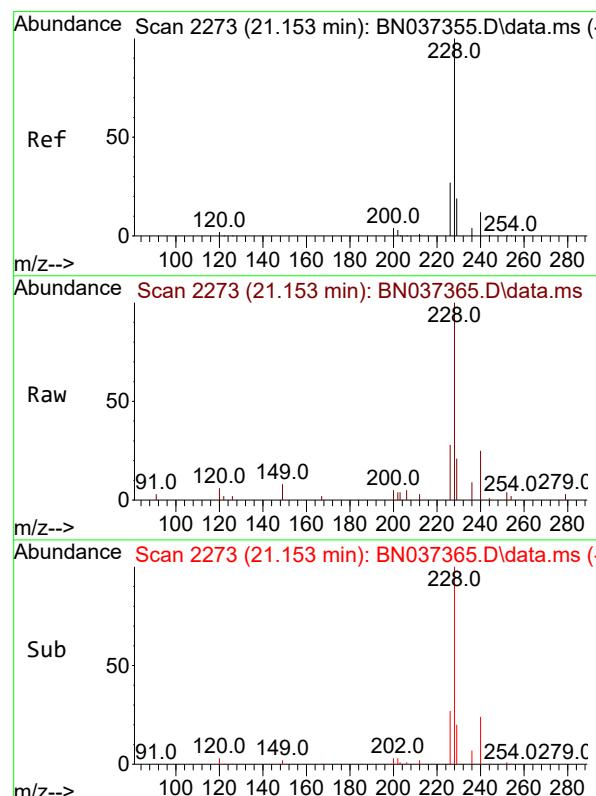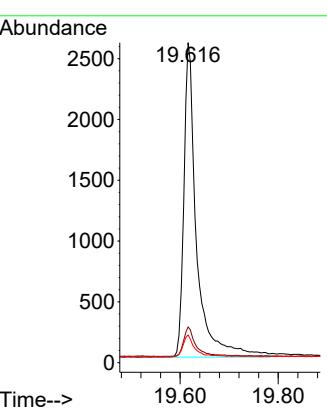

#32  
Benzo(a)anthracene  
Concen: 0.376 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion:228 Resp: 6359  
Ion Ratio Lower Upper  
228 100  
226 27.5 23.0 34.4  
229 20.7 17.4 26.0

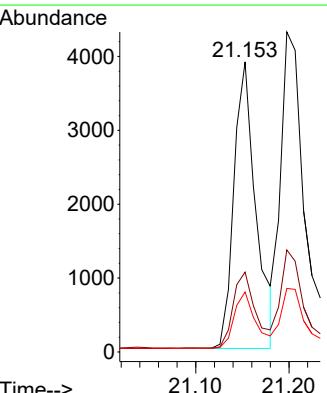

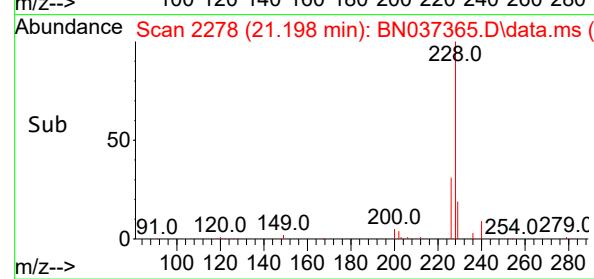

#33

Chrysene

Concen: 0.391 ng

RT: 21.198 min Scan# 2

Delta R.T. -0.009 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N





ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

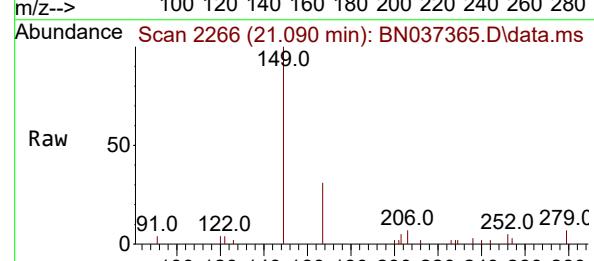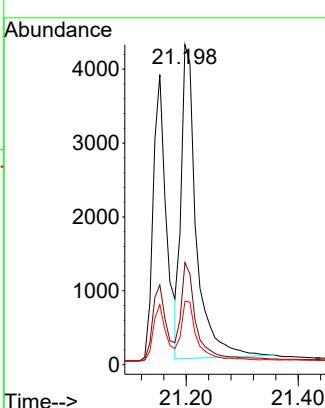

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.385 ng

RT: 21.090 min Scan# 2266

Delta R.T. -0.009 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17


Tgt Ion:149 Resp: 2672


Ion Ratio Lower Upper

149 100

167 31.7 24.6 37.0

279 6.5 6.5 9.7#

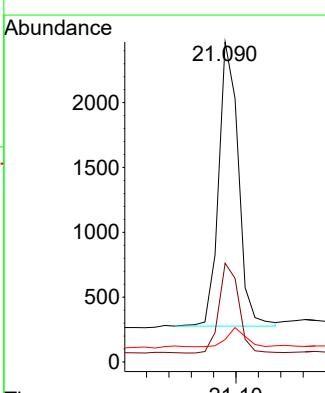

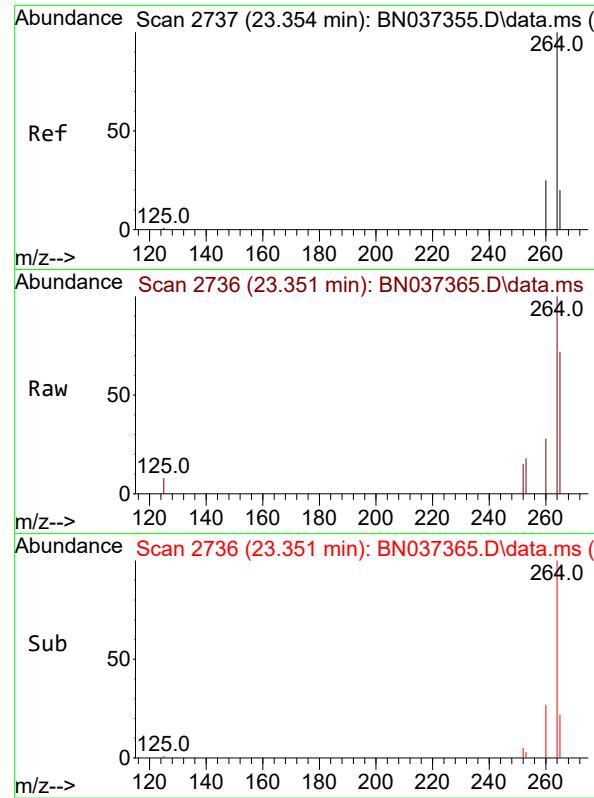


#35  
Perylene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 23.351 min Scan# 2  
Delta R.T. -0.003 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC



1 Manual Integrations  
2 APPROVED


3 Reviewed By :Rahul Chavli 06/23/2025  
4 Supervised By :Jagrut Upadhyay 06/24/2025

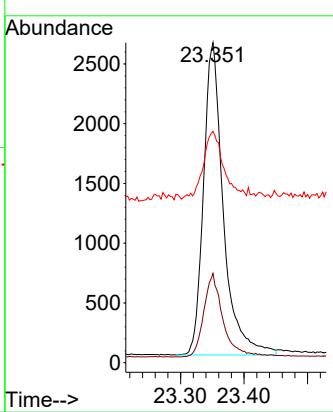

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.382 ng  
RT: 25.535 min Scan# 3483  
Delta R.T. -0.006 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion:276 Resp: 9725  
Ion Ratio Lower Upper  
276 100  
138 11.2 2.2 3.2#  
277 24.1 17.1 25.7

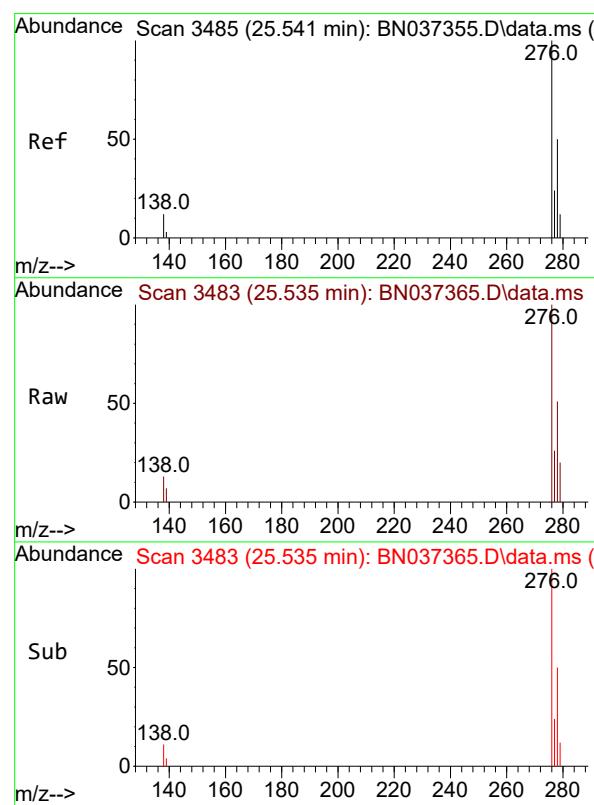

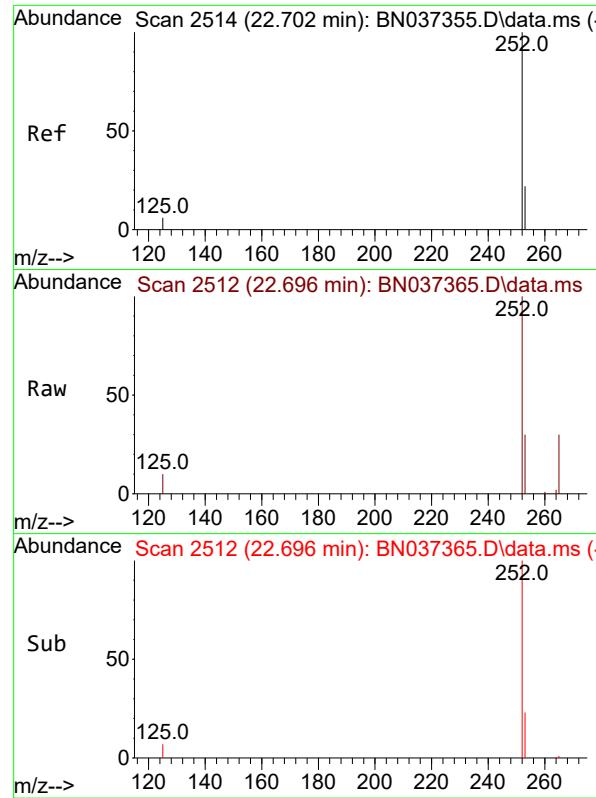

#37

Benzo(b)fluoranthene

Concen: 0.363 ng m

RT: 22.696 min Scan# 2

Delta R.T. -0.006 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N



ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

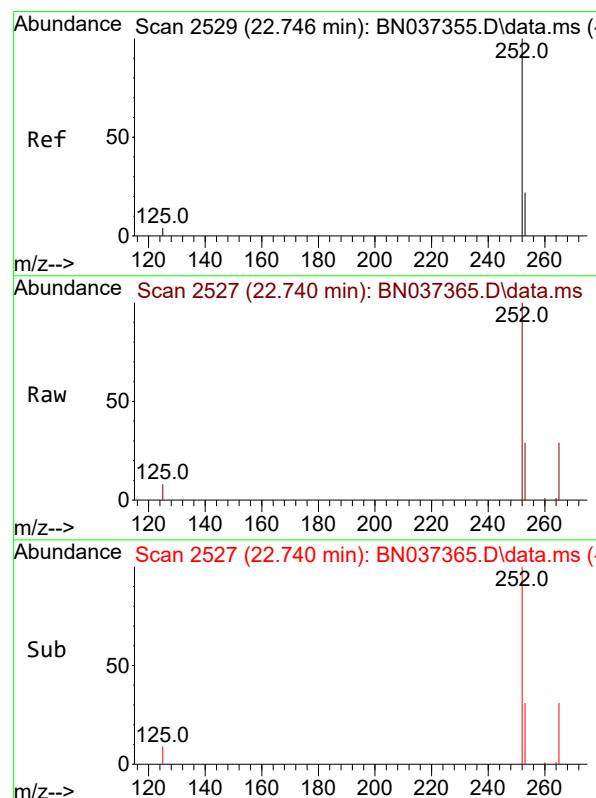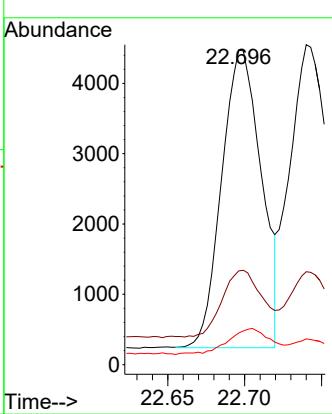

#38

Benzo(k)fluoranthene

Concen: 0.398 ng

RT: 22.740 min Scan# 2527


Delta R.T. -0.006 min




Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Tgt Ion:252 Resp: 9018

Ion	Ratio	Lower	Upper
252	100		
253	29.0	26.7	40.1
125	8.1	6.5	9.7

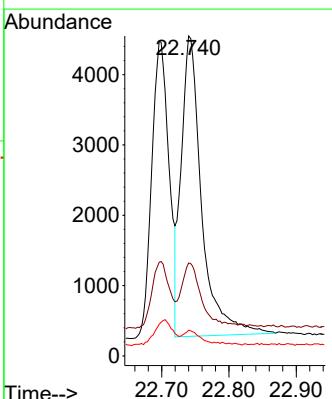



#39

Benzo(a)pyrene

Concen: 0.380 ng

RT: 23.255 min Scan# 2

Delta R.T. -0.003 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Instrument :

BNA\_N





ClientSampleId :

SSTDCCC0.4EC

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

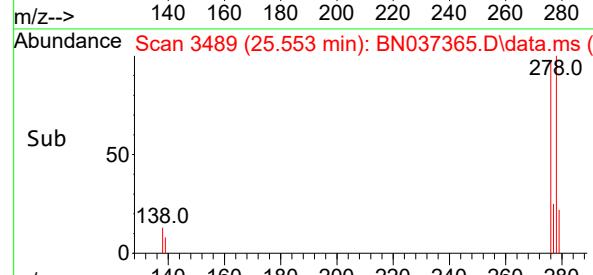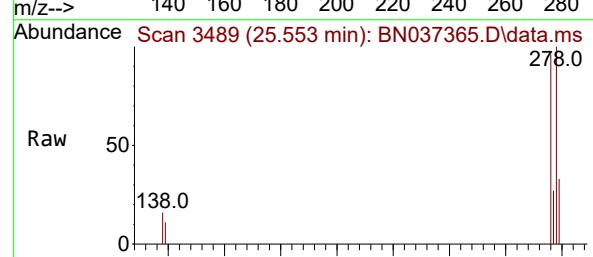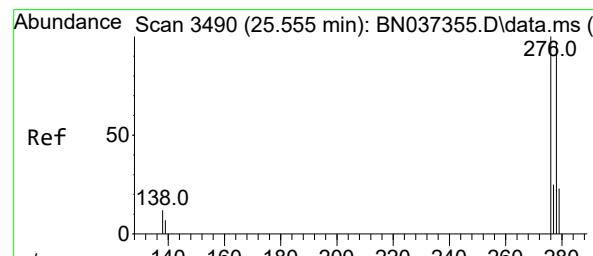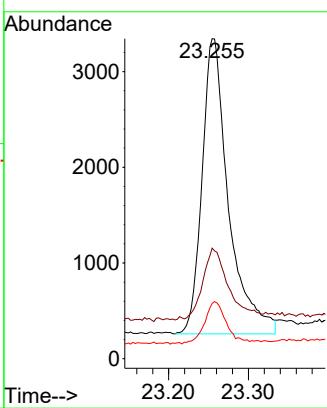

#40

Dibenzo(a,h)anthracene

Concen: 0.388 ng


RT: 25.553 min Scan# 3489


Delta R.T. -0.003 min

Lab File: BN037365.D

Acq: 21 Jun 2025 01:17

Tgt	Ion:278	Resp:	7424
Ion	Ratio	Lower	Upper
278	100		
139	11.0	10.2	15.4
279	33.0	35.6	53.4

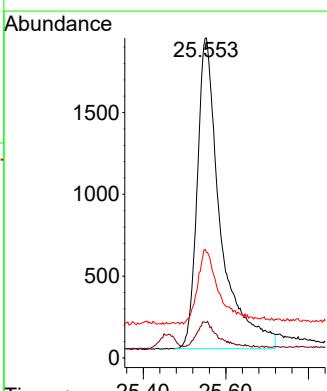

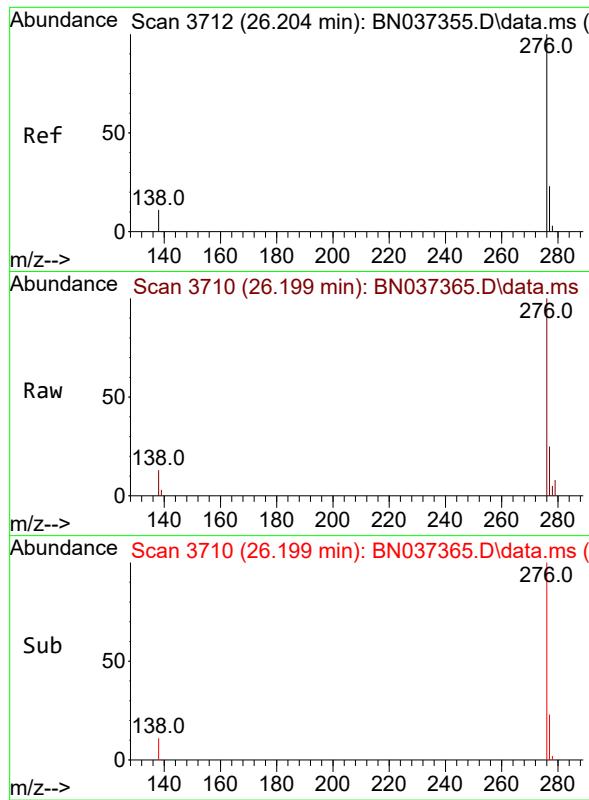


#41  
Benzo(g,h,i)perylene  
Concen: 0.389 ng  
RT: 26.199 min Scan# 3  
Delta R.T. -0.006 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Instrument :  
BNA\_N  
ClientSampleId :  
SSTDCCC0.4EC

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

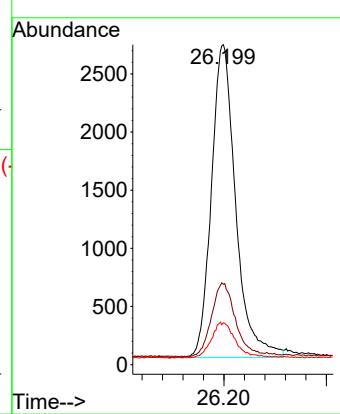

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037365.D  
 Acq On : 21 Jun 2025 01:17  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 LabSampleId :  
 SSTDCCC0.4

Quant Time: Jun 21 01:41:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	99	0.00
2	1,4-Dioxane	0.407	0.399	2.0	101	0.00
3	n-Nitrosodimethylamine	0.373	0.370	0.8	93	0.00
4 S	2-Fluorophenol	0.799	0.740	7.4	98	0.00
5 S	Phenol-d6	0.823	0.753	8.5	97	0.00
6	bis(2-Chloroethyl)ether	0.730	0.673	7.8	94	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	100	0.00
8 S	Nitrobenzene-d5	0.323	0.318	1.5	100	0.00
9	Naphthalene	1.056	1.038	1.7	99	0.00
10	Hexachlorobutadiene	0.417	0.452	-8.4	102	0.00
11 SURR	2-Methylnaphthalene-d10	0.648	0.670	-3.4	100	0.00
12	2-Methylnaphthalene	0.736	0.709	3.7	99	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	99	0.00
14 S	2,4,6-Tribromophenol	0.235	0.218	7.2	94	0.00
15 S	2-Fluorobiphenyl	1.757	1.777	-1.1	99	0.00
16	Acenaphthylene	1.682	1.615	4.0	100	0.00
17	Acenaphthene	1.107	1.059	4.3	99	0.00
18	Fluorene	1.556	1.496	3.9	98	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	100	0.00
20	4,6-Dinitro-2-methylphenol	0.096	0.084	12.5	105	0.01
21	4-Bromophenyl-phenylether	0.285	0.282	1.1	101	0.01
22	Hexachlorobenzene	0.310	0.316	-1.9	100	0.00
23	Atrazine	0.227	0.207	8.8	94	0.00
24	Pentachlorophenol	0.154	0.140	9.1	102	0.00
25	Phenanthrene	1.158	1.093	5.6	99	0.00
26	Anthracene	1.068	0.961	10.0	97	0.00
27 SURR	Fluoranthene-d10	1.148	1.189	-3.6	102	0.00
28	Fluoranthene	1.464	1.410	3.7	103	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	107	0.00
30	Pyrene	1.625	1.577	3.0	101	0.00
31 S	Terphenyl-d14	0.912	0.903	1.0	104	0.00
32	Benzo(a)anthracene	1.315	1.237	5.9	109	0.00
33	Chrysene	1.594	1.559	2.2	103	0.00
34	Bis(2-ethylhexyl)phthalate	0.540	0.520	3.7	103	0.00
35 I	Perylene-d12	1.000	1.000	0.0	115	0.00
36	Indeno(1,2,3-cd)pyrene	1.794	1.712	4.6	116	0.00
37	Benzo(b)fluoranthene	1.472	1.336	9.2	106	0.00
38	Benzo(k)fluoranthene	1.597	1.587	0.6	116	0.00
39 C	Benzo(a)pyrene	1.319	1.253	5.0	113	0.00
40	Dibenzo(a,h)anthracene	1.348	1.307	3.0	122	0.00
41	Benzo(g,h,i)perylene	1.603	1.559	2.7	113	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037365.D  
 Acq On : 21 Jun 2025 01:17  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 LabSampleId :  
 SSTDCCC0.4

Quant Time: Jun 21 01:41:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	99	0.00
2	1,4-Dioxane	0.400	0.392	2.0	101	0.00
3	n-Nitrosodimethylamine	0.400	0.397	0.8	93	0.00
4 S	2-Fluorophenol	0.400	0.370	7.5	98	0.00
5 S	Phenol-d6	0.400	0.366	8.5	97	0.00
6	bis(2-Chloroethyl)ether	0.400	0.368	8.0	94	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	100	0.00
8 S	Nitrobenzene-d5	0.400	0.394	1.5	100	0.00
9	Naphthalene	0.400	0.393	1.8	99	0.00
10	Hexachlorobutadiene	0.400	0.434	-8.5	102	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.413	-3.2	100	0.00
12	2-Methylnaphthalene	0.400	0.385	3.8	99	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	99	0.00
14 S	2,4,6-Tribromophenol	0.400	0.372	7.0	94	0.00
15 S	2-Fluorobiphenyl	0.400	0.405	-1.3	99	0.00
16	Acenaphthylene	0.400	0.384	4.0	100	0.00
17	Acenaphthene	0.400	0.383	4.3	99	0.00
18	Fluorene	0.400	0.385	3.8	98	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	100	0.00
20	4,6-Dinitro-2-methylphenol	0.400	0.350	12.5	105	0.01
21	4-Bromophenyl-phenylether	0.400	0.396	1.0	101	0.01
22	Hexachlorobenzene	0.400	0.408	-2.0	100	0.00
23	Atrazine	0.400	0.364	9.0	94	0.00
24	Pentachlorophenol	0.400	0.363	9.3	102	0.00
25	Phenanthrene	0.400	0.377	5.8	99	0.00
26	Anthracene	0.400	0.360	10.0	97	0.00
27 SURR	Fluoranthene-d10	0.400	0.414	-3.5	102	0.00
28	Fluoranthene	0.400	0.385	3.8	103	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	107	0.00
30	Pyrene	0.400	0.388	3.0	101	0.00
31 S	Terphenyl-d14	0.400	0.396	1.0	104	0.00
32	Benzo(a)anthracene	0.400	0.376	6.0	109	0.00
33	Chrysene	0.400	0.391	2.3	103	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.385	3.8	103	0.00
35 I	Perylene-d12	0.400	0.400	0.0	115	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.382	4.5	116	0.00
37	Benzo(b)fluoranthene	0.400	0.363	9.3	106	0.00
38	Benzo(k)fluoranthene	0.400	0.398	0.5	116	0.00
39 C	Benzo(a)pyrene	0.400	0.380	5.0	113	0.00
40	Dibenzo(a,h)anthracene	0.400	0.388	3.0	122	0.00
41	Benzo(g,h,i)perylene	0.400	0.389	2.8	113	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

7C

## SEMIVOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>CHEMTECH</u>		Contract:	<u>TETR06</u>	
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q2375</u>	SAS No.:	<u>Q2375</u>
Instrument ID:	<u>BNA_N</u>		Calibration Date/Time:	<u>06/26/2025</u>	<u>21:38</u>
Lab File ID:	<u>BN037403.D</u>		Init. Calib. Date(s):	<u>06/26/2025</u>	<u>06/26/2025</u>
EPA Sample No.:	<u>SSTDCCC0.4</u>		Init. Calib. Time(s):	<u>10:41</u>	<u>14:17</u>
GC Column:	<u>ZB-GR</u>	ID: <u>0.25</u>	(mm)		

COMPOUND	RRF	RRF0.4	MIN RRF	%D	MAX%D
2-Methylnaphthalene-d10	0.619	0.590		-4.7	20.0
Fluoranthene-d10	1.146	1.145		-0.1	20.0
2-Fluorophenol	0.771	0.749		-2.9	20.0
Phenol-d6	0.799	0.782		-2.1	20.0
Nitrobenzene-d5	0.321	0.301		-6.2	20.0
2-Fluorobiphenyl	1.727	1.728		0.1	20.0
2,4,6-Tribromophenol	0.235	0.289		23.0	20.0
Terphenyl-d14	0.853	0.867		1.6	20.0
1,4-Dioxane	0.379	0.373		-1.6	20.0

All other compounds must meet a minimum RRF of 0.010.

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037403.D  
 Acq On : 26 Jun 2025 21:38  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4

Quant Time: Jun 27 03:00:38 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.560	152	1253	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	2741	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	1842	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	3978	0.400	ng	0.00
29) Chrysene-d12	21.162	240	3956	0.400	ng	0.00
35) Perylene-d12	23.342	264	4281	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	939	0.389	ng	0.00
5) Phenol-d6	6.744	99	980	0.391	ng	0.00
8) Nitrobenzene-d5	8.717	82	824	0.375	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	1618	0.382	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	532	0.492	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	3183	0.400	ng	0.00
27) Fluoranthene-d10	19.003	212	4555	0.400	ng	0.00
31) Terphenyl-d14	19.611	244	3431	0.407	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.097	88	467	0.393	ng	96
3) n-Nitrosodimethylamine	3.415	42	469	0.400	ng	# 90
6) bis(2-Chloroethyl)ether	6.997	93	828	0.372	ng	95
9) Naphthalene	10.383	128	2760	0.391	ng	97
10) Hexachlorobutadiene	10.682	225	1242	0.443	ng	# 99
12) 2-Methylnaphthalene	12.011	142	1868	0.385	ng	95
16) Acenaphthylene	13.924	152	2920	0.382	ng	99
17) Acenaphthene	14.277	154	1878	0.376	ng	99
18) Fluorene	15.271	166	2778	0.394	ng	99
20) 4,6-Dinitro-2-methylph...	15.368	198	435	0.426	ng	97
21) 4-Bromophenyl-phenylether	16.165	248	1143	0.407	ng	99
22) Hexachlorobenzene	16.276	284	1236	0.410	ng	97
23) Atrazine	16.438	200	901	0.405	ng	# 92
24) Pentachlorophenol	16.624	266	737	0.452	ng	94
25) Phenanthrene	17.009	178	4265	0.381	ng	100
26) Anthracene	17.095	178	3988	0.387	ng	99
28) Fluoranthene	19.031	202	5729	0.400	ng	99
30) Pyrene	19.398	202	5716	0.382	ng	100
32) Benzo(a)anthracene	21.144	228	4770	0.384	ng	99
33) Chrysene	21.197	228	6302	0.410	ng	99
34) Bis(2-ethylhexyl)phtha...	21.090	149	2069	0.420	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.520	276	7185	0.398	ng	97
37) Benzo(b)fluoranthene	22.690	252	5748	0.381	ng	99
38) Benzo(k)fluoranthene	22.734	252	6484	0.402	ng	99
39) Benzo(a)pyrene	23.249	252	5244	0.391	ng	96
40) Dibenzo(a,h)anthracene	25.541	278	5585	0.403	ng	98
41) Benzo(g,h,i)perylene	26.184	276	6411	0.387	ng	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037403.D  
 Acq On : 26 Jun 2025 21:38  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4

Quant Time: Jun 27 03:00:38 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration




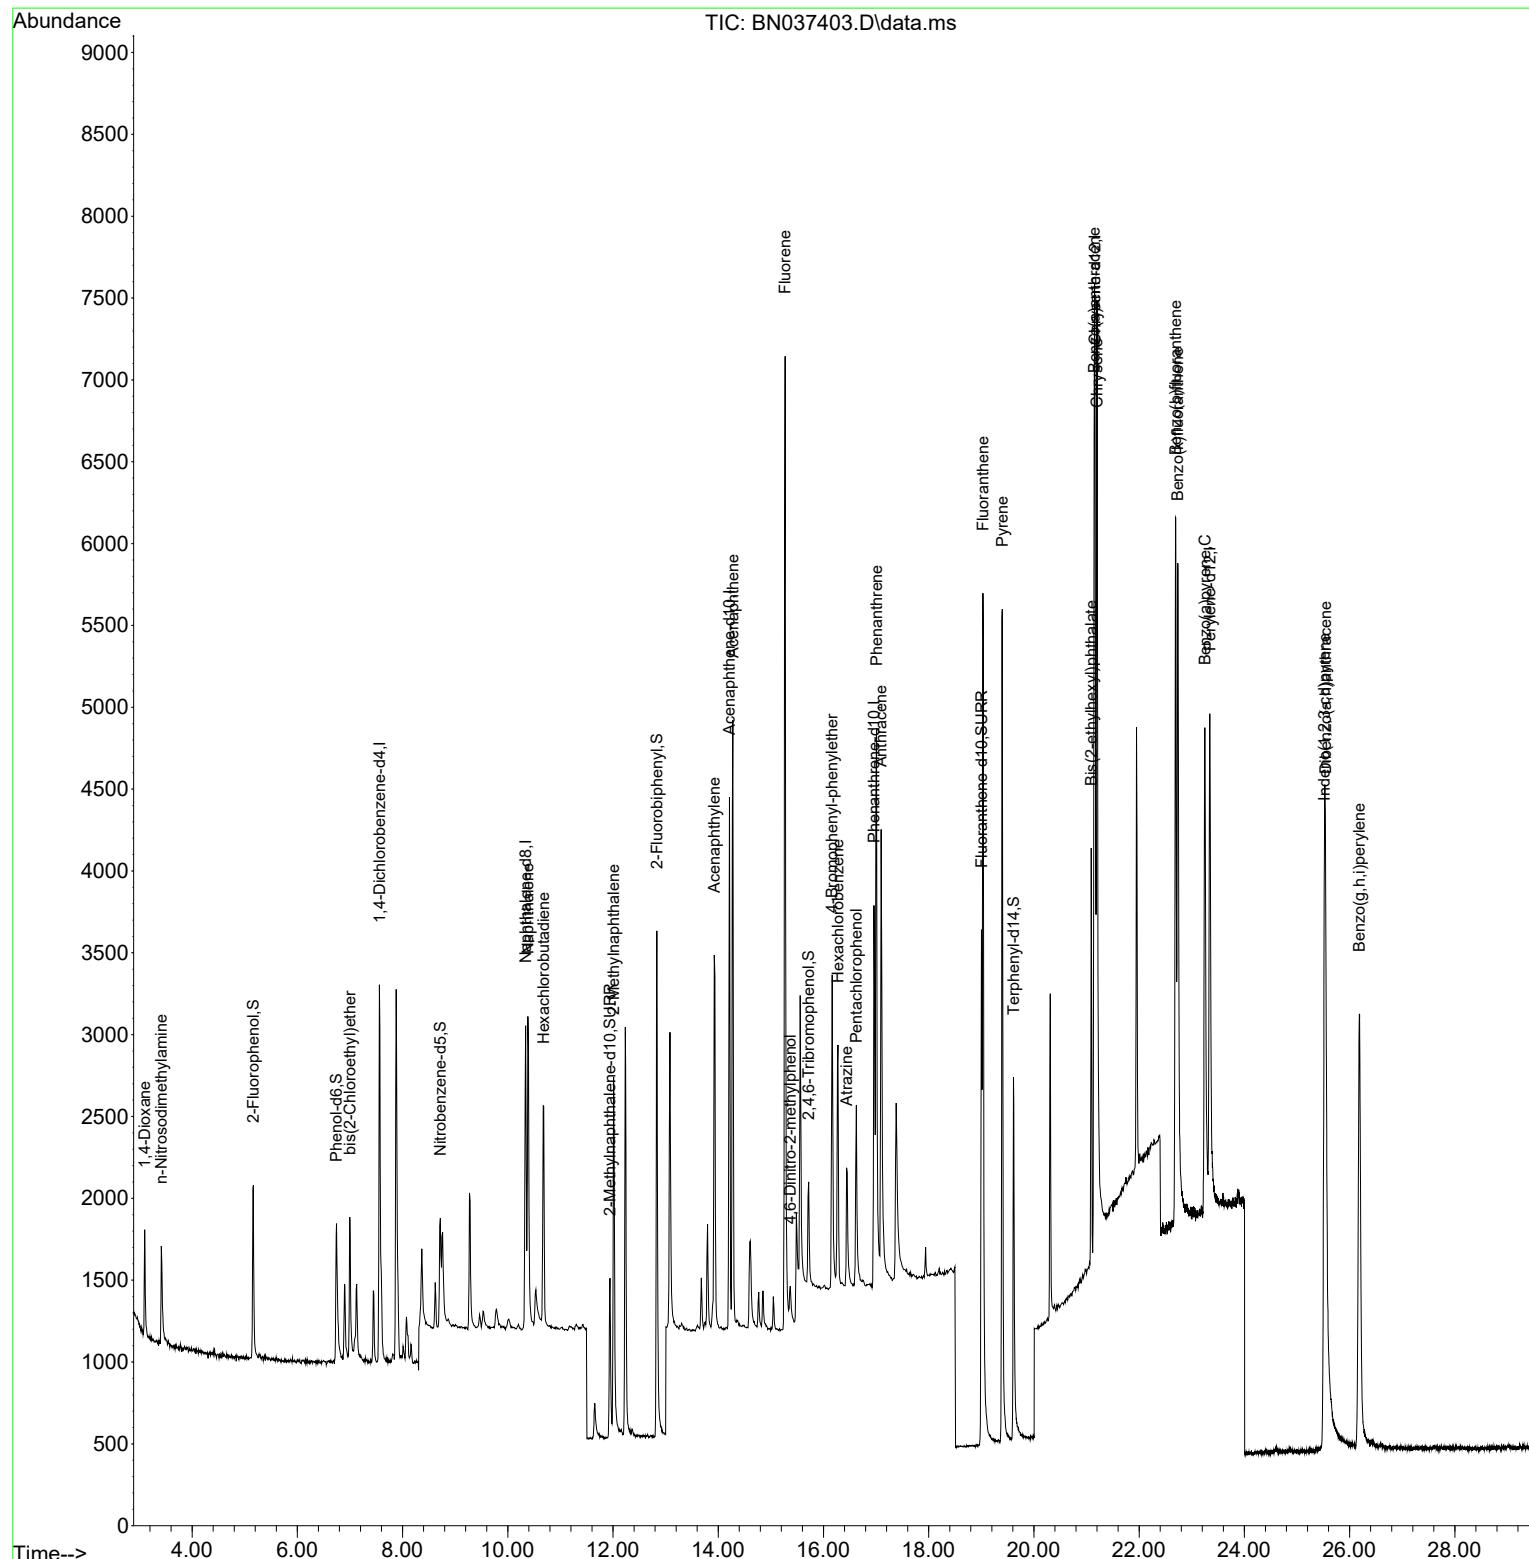




#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.560 min Scan# 6  
Delta R.T. -0.008 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38


Instrument :  
BNA\_N  
ClientSampleId :  
SSTDCCC0.4




Tgt Ion:152 Resp: 1253  
Ion Ratio Lower Upper  
152 100  
150 149.5 116.2 174.2  
115 57.6 42.9 64.3



#2  
1,4-Dioxane  
Concen: 0.393 ng  
RT: 3.097 min Scan# 30  
Delta R.T. -0.007 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion: 88 Resp: 467  
Ion Ratio Lower Upper  
88 100  
43 29.6 21.6 32.4  
58 54.8 45.9 68.9







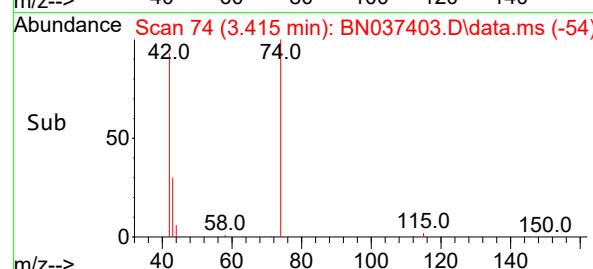

#3  
n-Nitrosodimethylamine  
Concen: 0.400 ng  
RT: 3.415 min Scan# 7  
Delta R.T. -0.007 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4




Tgt Ion: 42 Resp: 469  
Ion Ratio Lower Upper  
42 100  
74 112.4 97.8 146.8  
44 4.3 8.7 13.1#

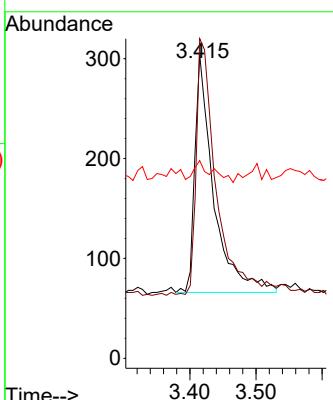

#4  
2-Fluorophenol  
Concen: 0.389 ng  
RT: 5.163 min Scan# 316  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion: 112 Resp: 939  
Ion Ratio Lower Upper  
112 100  
64 52.6 40.3 60.5  
63 33.5 26.1 39.1




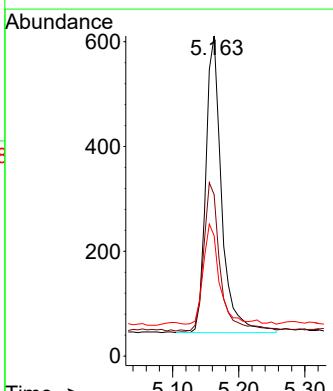


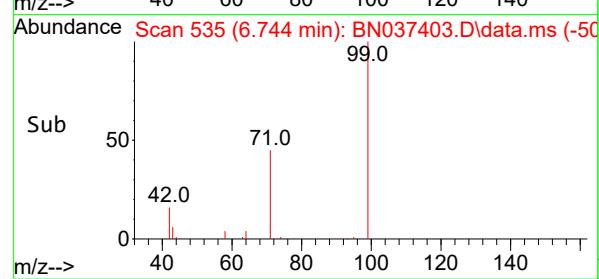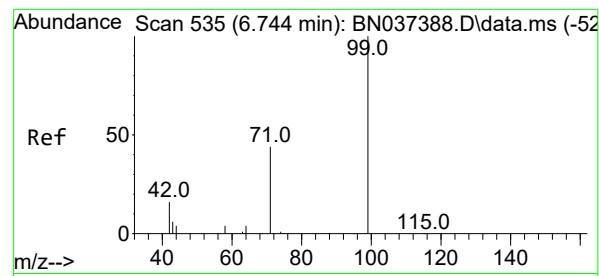

#5  
 Phenol-d6  
 Concen: 0.391 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. -0.000 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38


Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCCC0.4




Tgt Ion: 99 Resp: 980  
 Ion Ratio Lower Upper  
 99 100  
 42 21.3 15.6 23.4  
 71 46.0 35.8 53.8

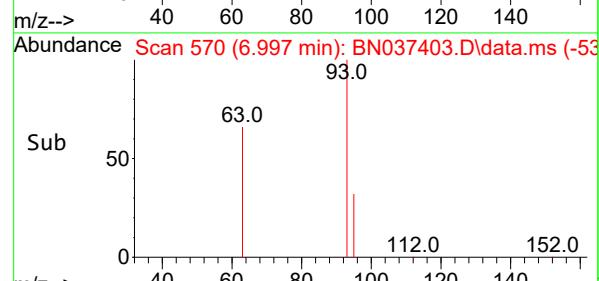

#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.372 ng  
 RT: 6.997 min Scan# 570  
 Delta R.T. -0.000 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38

Tgt Ion: 93 Resp: 828  
 Ion Ratio Lower Upper  
 93 100  
 63 65.8 49.6 74.4  
 95 31.9 23.9 35.9

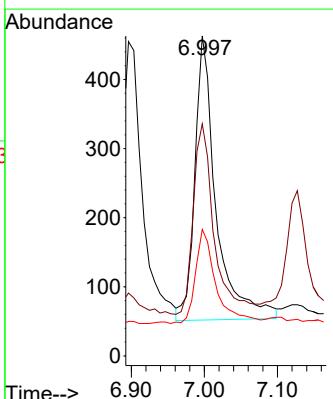


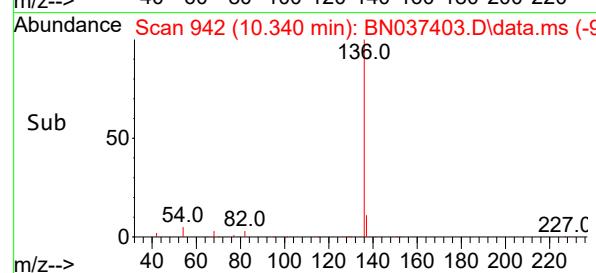




#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4


Tgt Ion:136 Resp: 2741




Ion	Ratio	Lower	Upper
136	100		
137	14.3	10.4	15.6
54	8.3	5.6	8.4
68	6.2	4.6	6.8

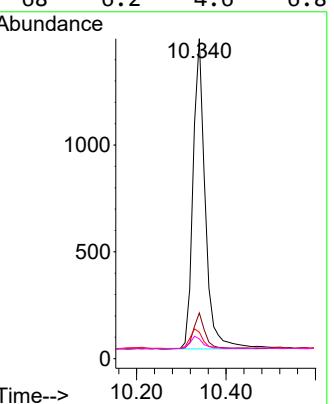

#8  
 Nitrobenzene-d5  
 Concen: 0.375 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. -0.000 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38

Tgt Ion: 82 Resp: 824  
 Ion Ratio Lower Upper  
 82 100  
 128 45.9 34.0 51.0  
 54 49.3 37.7 56.5

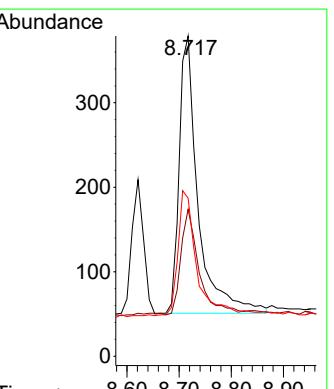

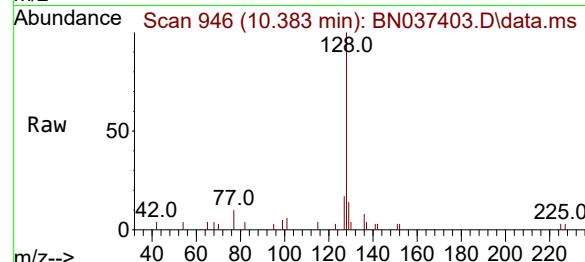

#9

Naphthalene

Concen: 0.391 ng

RT: 10.383 min Scan# 9

Delta R.T. -0.011 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4

Tgt Ion:128 Resp: 2760

Ion Ratio Lower Upper





128 100

129 13.8 10.4 15.6

127 17.0 12.2 18.4

Abundance

10.383

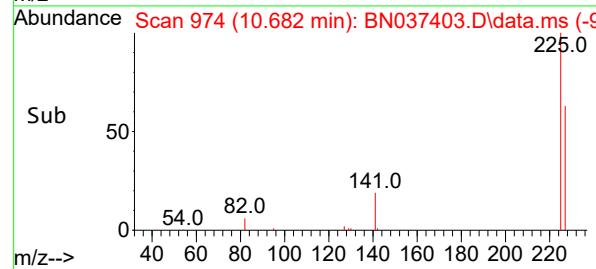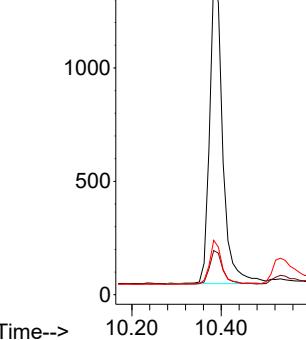

#10

Hexachlorobutadiene

Concen: 0.443 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Tgt Ion:225 Resp: 1242

Ion Ratio Lower Upper


225 100




223 0.0 0.0 0.0

227 63.4 49.9 74.9

Abundance

10.682




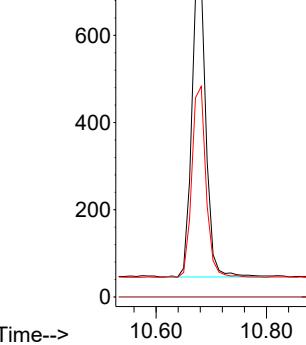




#11  
2-Methylnaphthalene-d10  
Concen: 0.382 ng  
RT: 11.940 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38


Instrument :  
BNA\_N  
ClientSampleId :  
SSTDCCC0.4

Tgt Ion:152 Resp: 1618  
Ion Ratio Lower Upper  
152 100  
151 21.3 18.4 27.6

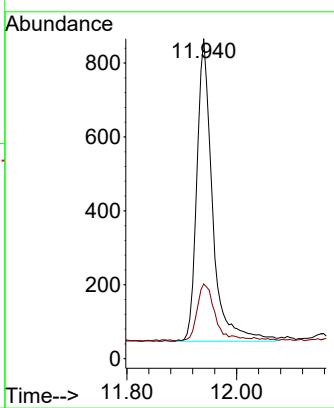

#12  
2-Methylnaphthalene  
Concen: 0.385 ng  
RT: 12.011 min Scan# 1151  
Delta R.T. -0.005 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion:142 Resp: 1868  
Ion Ratio Lower Upper  
142 100  
141 92.5 70.1 105.1  
115 47.9 35.8 53.6

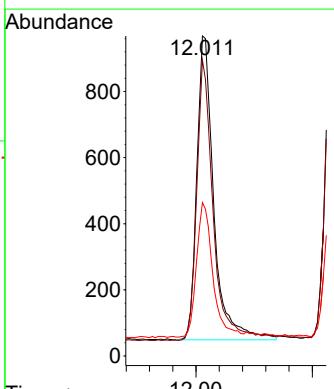

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037403.D




Acq: 26 Jun 2025 21:38

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4

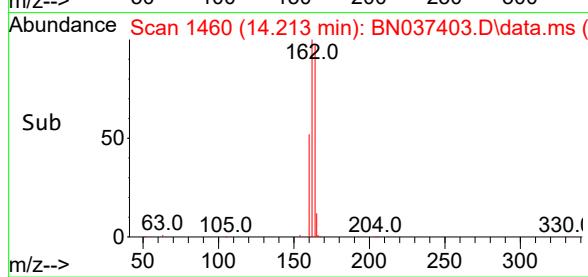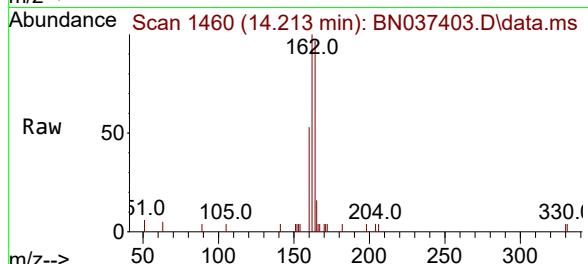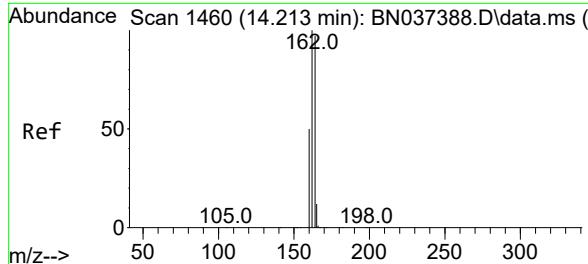





Tgt Ion:164 Resp: 1842

Ion Ratio Lower Upper

164 100

162 102.8 82.6 123.8

160 54.8 42.2 63.2

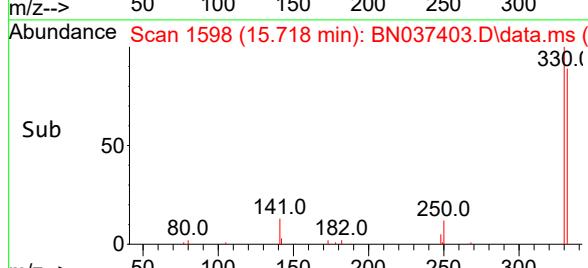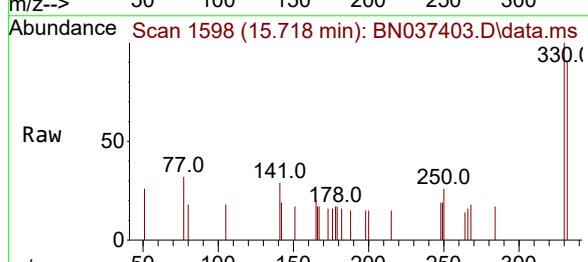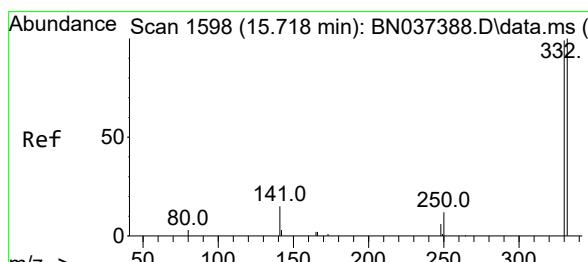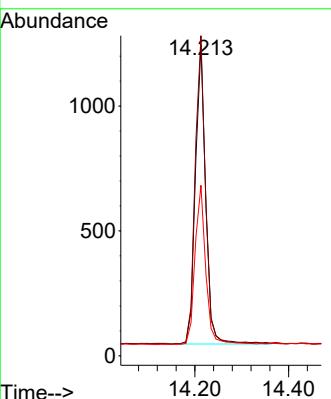

#14

2,4,6-Tribromophenol

Concen: 0.492 ng

RT: 15.718 min Scan# 1598

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38


Tgt Ion:330 Resp: 532




Ion Ratio Lower Upper

330 100

332 91.0 77.8 116.8

141 27.8 24.0 36.0



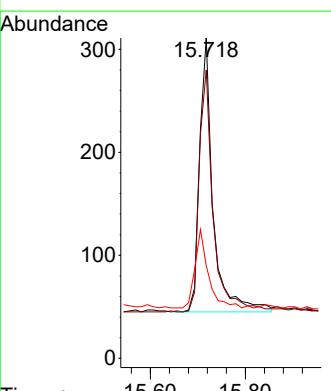




#15  
2-Fluorobiphenyl  
Concen: 0.400 ng  
RT: 12.833 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38



Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4




Tgt Ion:172 Resp: 3183  
Ion Ratio Lower Upper  
172 100  
171 37.9 28.8 43.2  
170 26.2 20.3 30.5

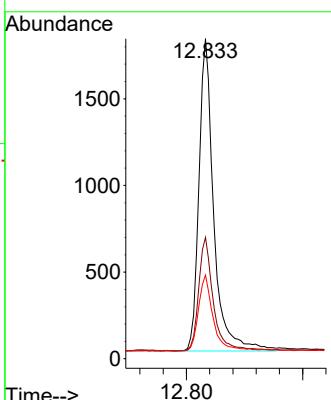

#16  
Acenaphthylene  
Concen: 0.382 ng  
RT: 13.924 min Scan# 1433  
Delta R.T. -0.011 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion:152 Resp: 2920  
Ion Ratio Lower Upper  
152 100  
151 19.6 15.8 23.6  
153 13.5 10.3 15.5

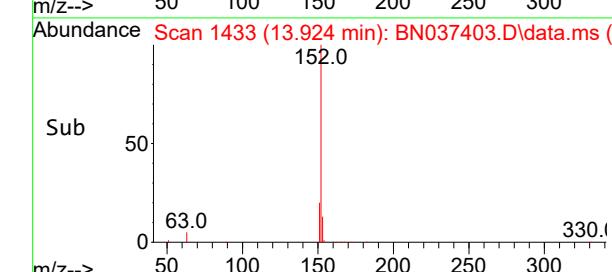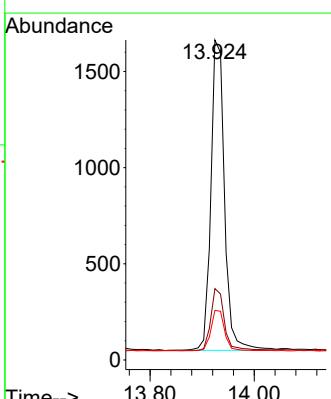



#17

Acenaphthene

Concen: 0.376 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Instrument:

BNA\_N

ClientSampleId :

SSTDCCC0.4

Tgt Ion:154 Resp: 1878

Ion Ratio Lower Upper

154 100

153 118.1 94.6 141.8

152 64.9 50.2 75.2

Abundance


Time--&gt; 14.20 14.277 14.30

1000

500

0

14.20 14.277 14.30

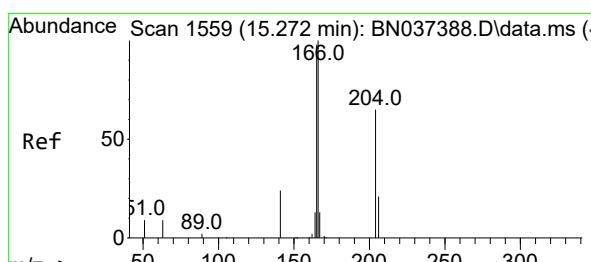

#18

Fluorene

Concen: 0.394 ng

RT: 15.271 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Tgt Ion:166 Resp: 2778

Ion Ratio Lower Upper

166 100

165 98.1 79.4 119.2

167 13.4 10.6 15.8

Abundance

Time--&gt; 15.20 15.271 15.40



1500




1000

500

0

15.20 15.271 15.40



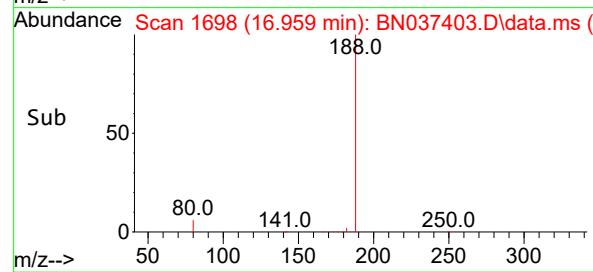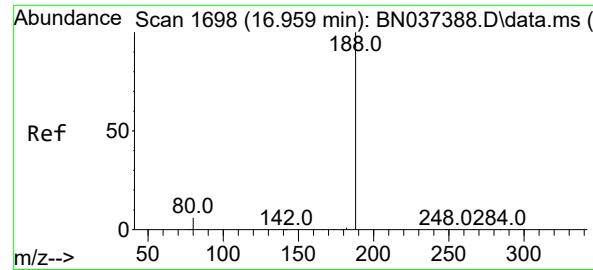

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.959 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Instrument: 1

BNA\_N

ClientSampleId : SSTDCCC0.4





Tgt Ion:188 Resp: 3978

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 7.6 6.2 9.4

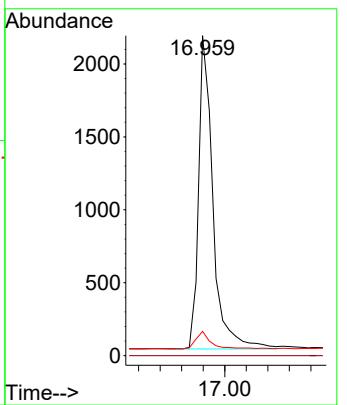

#20

4,6-Dinitro-2-methylphenol

Concen: 0.426 ng

RT: 15.368 min Scan# 1568

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38


Tgt Ion:198 Resp: 435


Ion Ratio Lower Upper

198 100

51 47.4 38.8 58.2

105 39.7 29.8 44.6


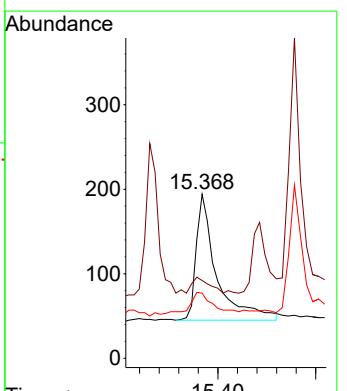


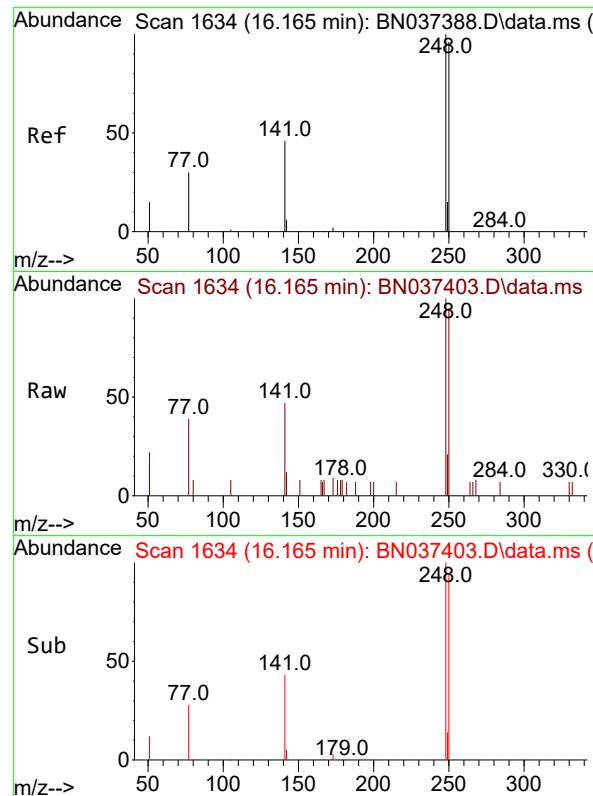

#21  
4-Bromophenyl-phenylether  
Concen: 0.407 ng  
RT: 16.165 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4




Tgt Ion:248 Resp: 1143  
Ion Ratio Lower Upper  
248 100  
250 95.2 77.0 115.4  
141 47.0 38.7 58.1

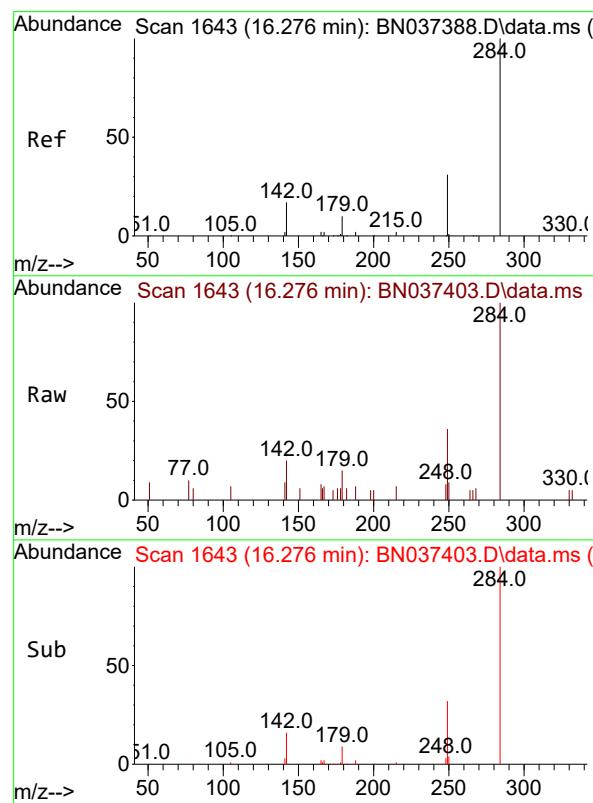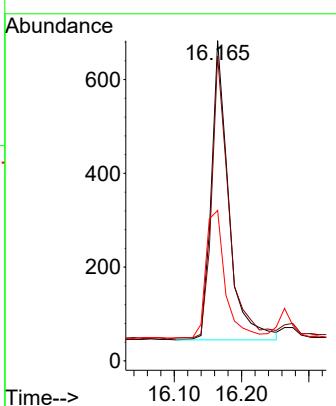

#22  
Hexachlorobenzene  
Concen: 0.410 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion:284 Resp: 1236  
Ion Ratio Lower Upper  
284 100  
142 33.3 27.2 40.8  
249 36.0 26.7 40.1

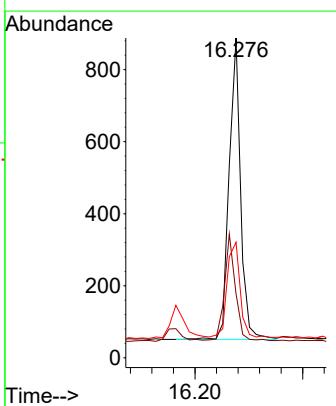



#23

Atrazine

Concen: 0.405 ng

RT: 16.438 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Instrument:

BNA\_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:200 Resp: 901

Ion Ratio Lower Upper

200 100

173 32.3 19.0 28.6#

215 54.1 41.3 61.9

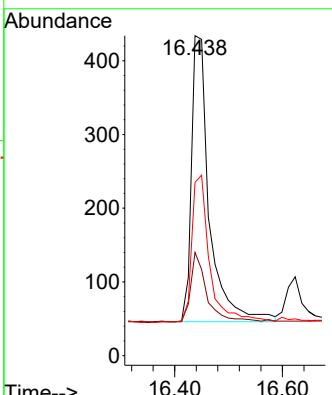

#24

Pentachlorophenol

Concen: 0.452 ng

RT: 16.624 min Scan# 1671

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38


Tgt Ion:266 Resp: 737




Ion Ratio Lower Upper

266 100

264 56.2 49.2 73.8

268 64.0 54.2 81.4

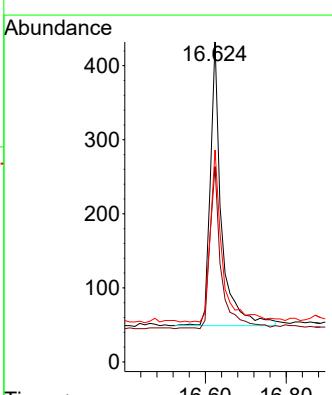

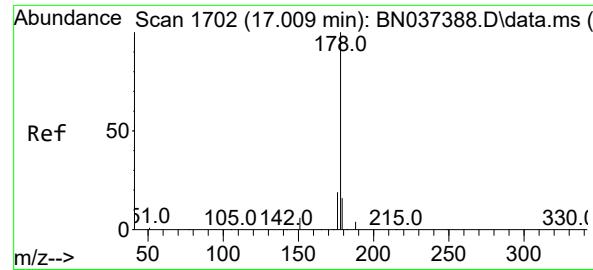

#25

Phenanthrene

Concen: 0.381 ng

RT: 17.009 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Instrument:

BNA\_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:178 Resp: 4265

Ion Ratio Lower Upper

178 100

176 19.7 15.6 23.4

179 15.8 12.8 19.2

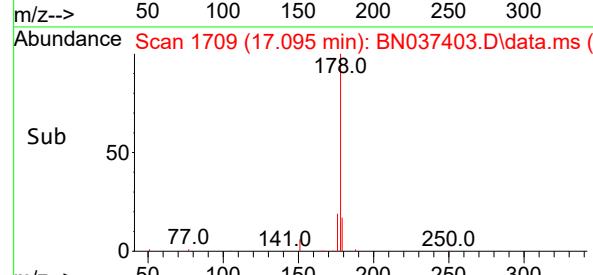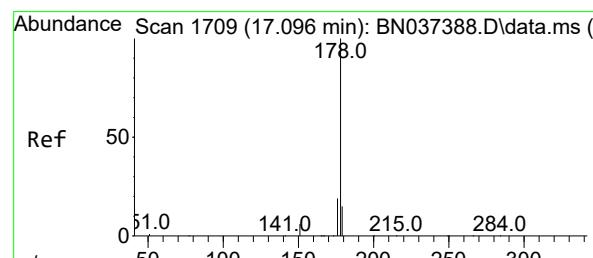

#26

Anthracene

Concen: 0.387 ng

RT: 17.095 min Scan# 1709

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38


Tgt Ion:178 Resp: 3988


Ion Ratio Lower Upper

178 100

176 18.0 14.9 22.3

179 15.5 12.4 18.6





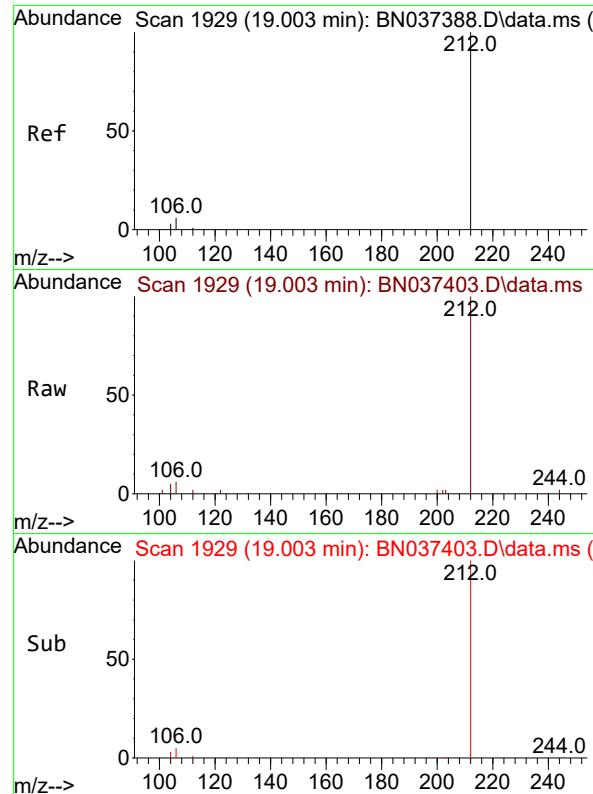

#27  
Fluoranthene-d10  
Concen: 0.400 ng  
RT: 19.003 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4




Tgt Ion:212 Resp: 4555  
Ion Ratio Lower Upper  
212 100  
106 5.1 4.5 6.7  
104 3.0 2.7 4.1

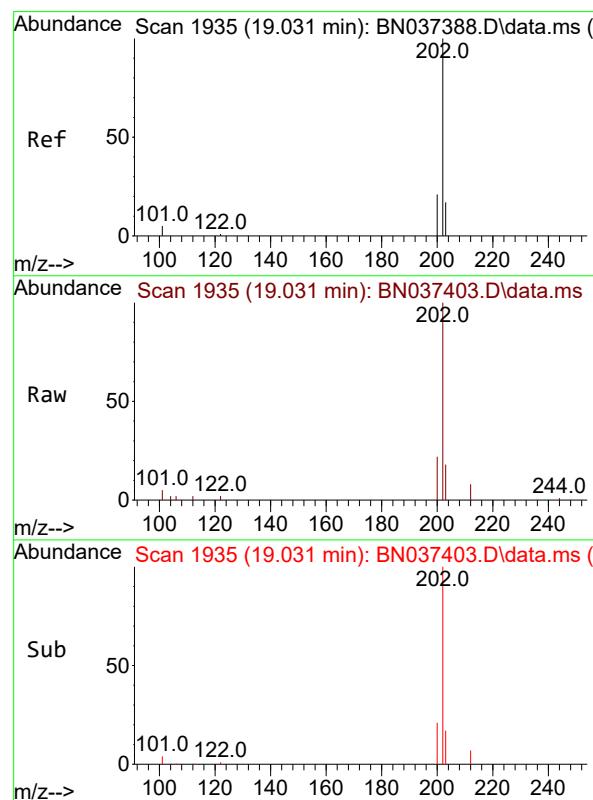

#28  
Fluoranthene  
Concen: 0.400 ng  
RT: 19.031 min Scan# 1935  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion:202 Resp: 5729  
Ion Ratio Lower Upper  
202 100  
101 4.3 3.8 5.6  
203 17.4 13.5 20.3





#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.162 min Scan# 2

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:240 Resp: 3956

Ion Ratio Lower Upper

240 100

120 7.3 5.3 7.9

236 29.7 22.7 34.1

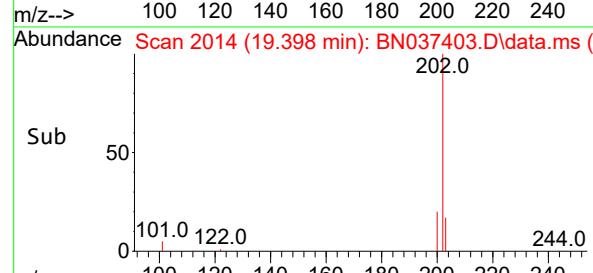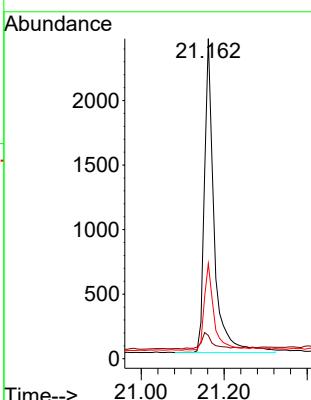

#30

Pyrene

Concen: 0.382 ng

RT: 19.398 min Scan# 2014

Delta R.T. -0.000 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38


Tgt Ion:202 Resp: 5716


Ion Ratio Lower Upper

202 100

200 20.6 16.5 24.7

203 17.8 14.2 21.2





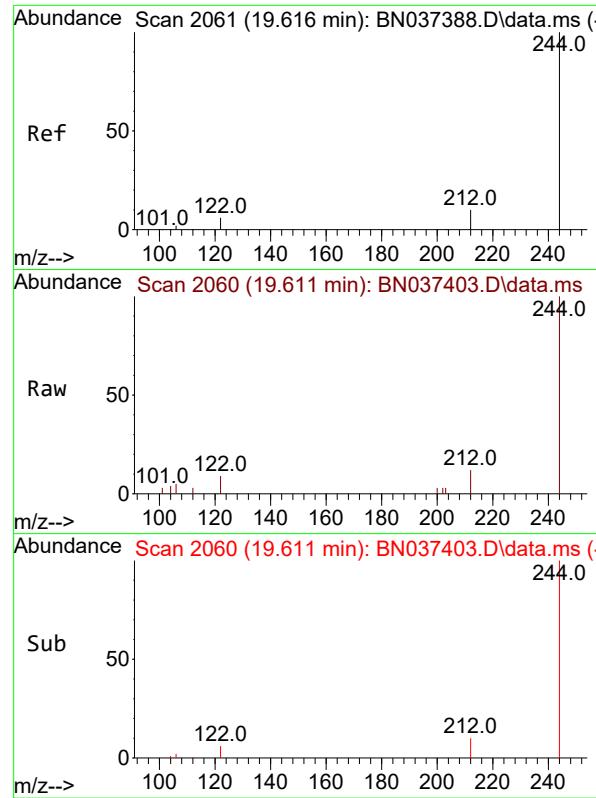

#31  
 Terphenyl-d14  
 Concen: 0.407 ng  
 RT: 19.611 min Scan# 2  
 Delta R.T. -0.005 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4




Tgt Ion:244 Resp: 3431  
 Ion Ratio Lower Upper  
 244 100  
 212 12.1 9.1 13.7  
 122 8.8 6.3 9.5

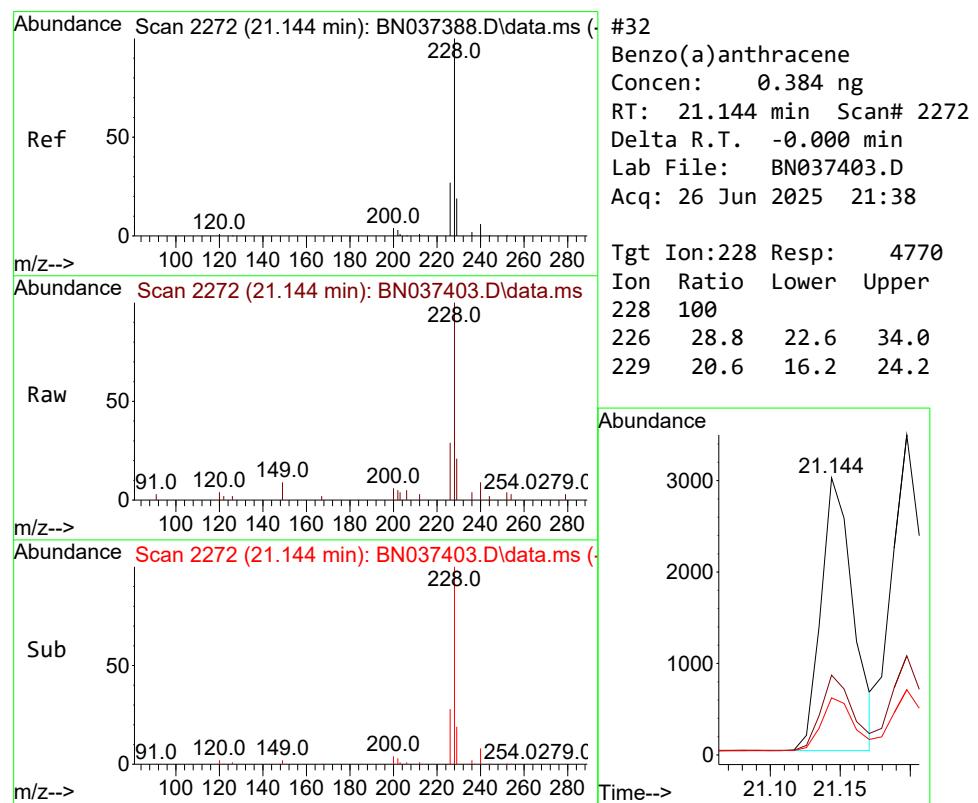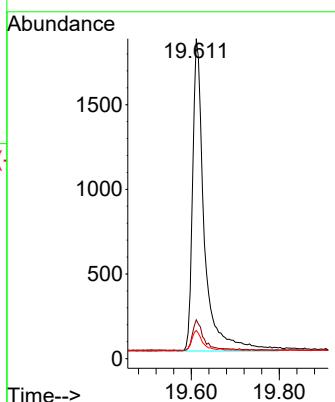

#32  
 Benzo(a)anthracene  
 Concen: 0.384 ng  
 RT: 21.144 min Scan# 2272  
 Delta R.T. -0.000 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38





Tgt Ion:228 Resp: 4770  
 Ion Ratio Lower Upper  
 228 100  
 226 28.8 22.6 34.0  
 229 20.6 16.2 24.2






#33  
Chrysene  
Concen: 0.410 ng  
RT: 21.197 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38  
ClientSampleId : SSTDCCC0.4


Tgt Ion:228 Resp: 6302  
Ion Ratio Lower Upper  
228 100  
226 31.0 24.5 36.7  
229 20.4 16.1 24.1

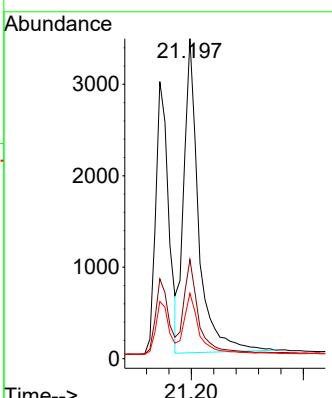

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.420 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. -0.000 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion:149 Resp: 2069  
Ion Ratio Lower Upper  
149 100  
167 32.0 24.8 37.2  
279 7.6 5.0 7.6#


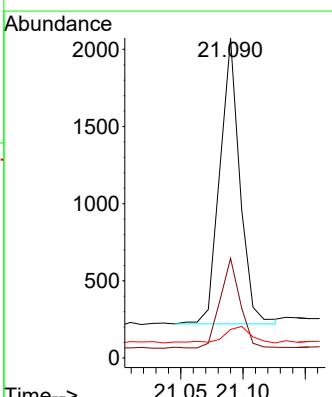


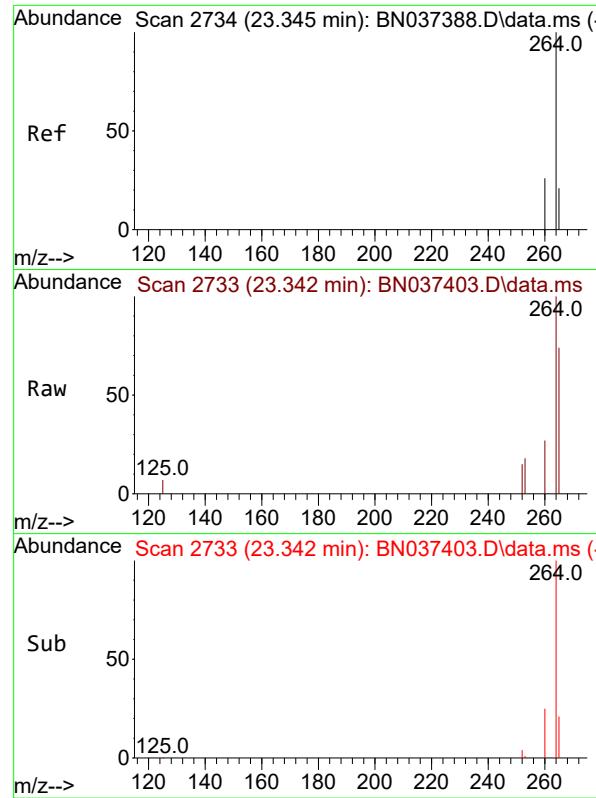

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.342 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4


Tgt Ion:264 Resp: 4281  
 Ion Ratio Lower Upper  
 264 100  
 260 27.2 21.4 32.0  
 265 73.6 56.2 84.4

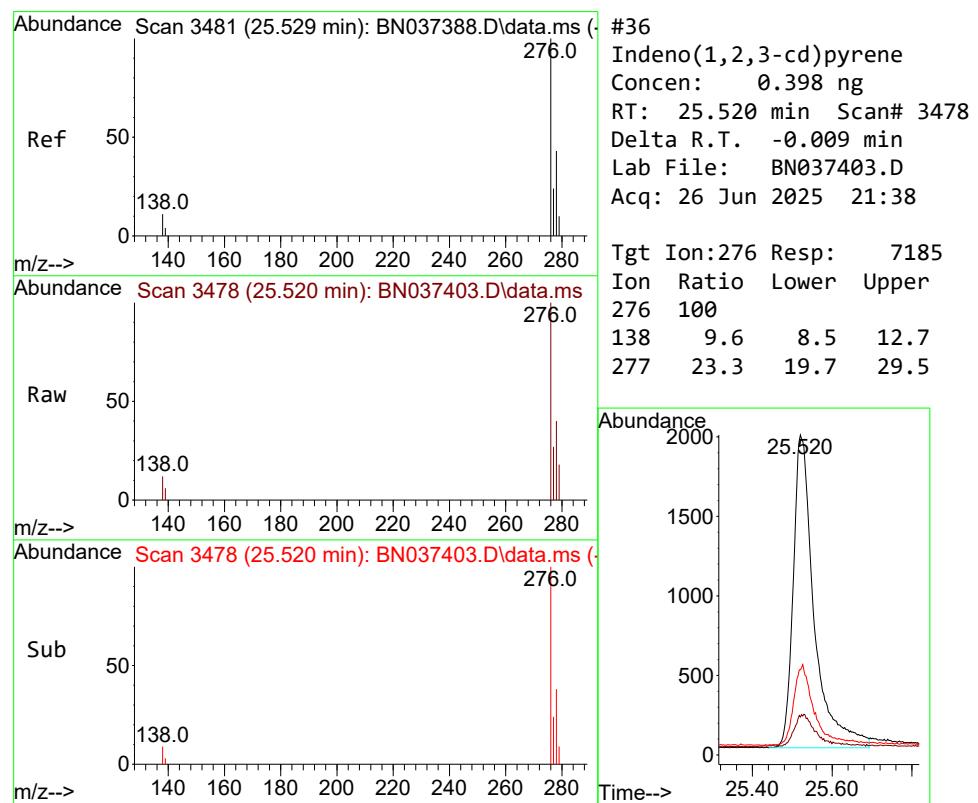

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.398 ng  
 RT: 25.520 min Scan# 3478  
 Delta R.T. -0.009 min  
 Lab File: BN037403.D  
 Acq: 26 Jun 2025 21:38

Tgt Ion:276 Resp: 7185  
 Ion Ratio Lower Upper  
 276 100  
 138 9.6 8.5 12.7  
 277 23.3 19.7 29.5



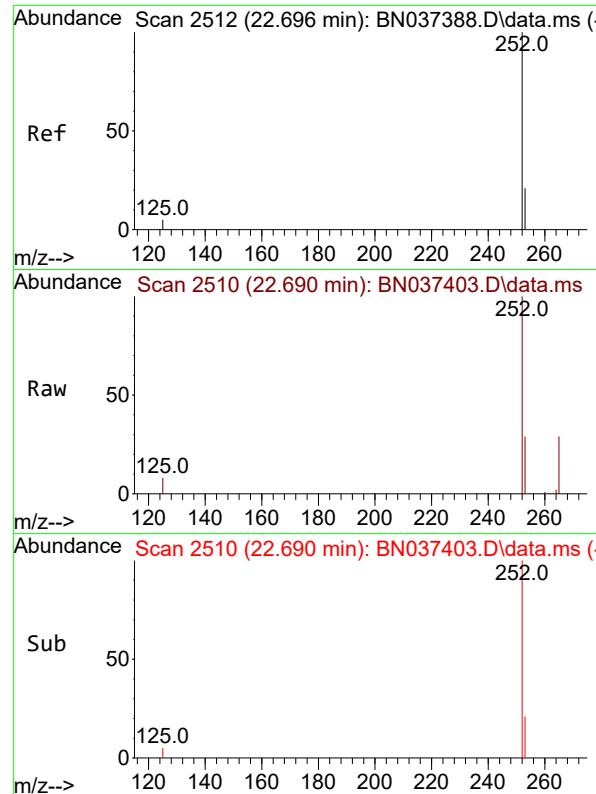

#37

Benzo(b)fluoranthene

Concen: 0.381 ng

RT: 22.690 min Scan# 2

Delta R.T. -0.006 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4



Tgt Ion:252 Resp: 5748

Ion Ratio Lower Upper

252 100

253 29.2 22.8 34.2

125 8.0 6.2 9.4

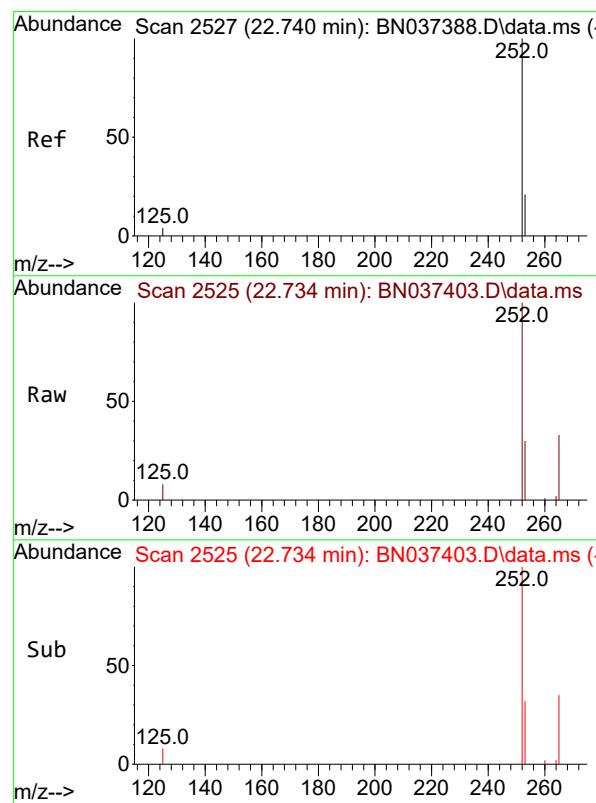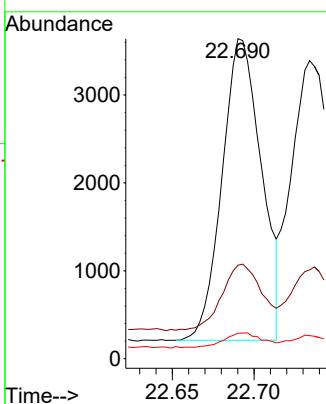

#38

Benzo(k)fluoranthene

Concen: 0.402 ng

RT: 22.734 min Scan# 2525

Delta R.T. -0.006 min

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38


Tgt Ion:252 Resp: 6484


Ion Ratio Lower Upper

252 100

253 29.8 23.2 34.8



125 7.7 6.0 9.0

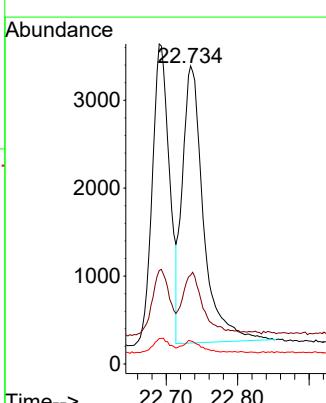

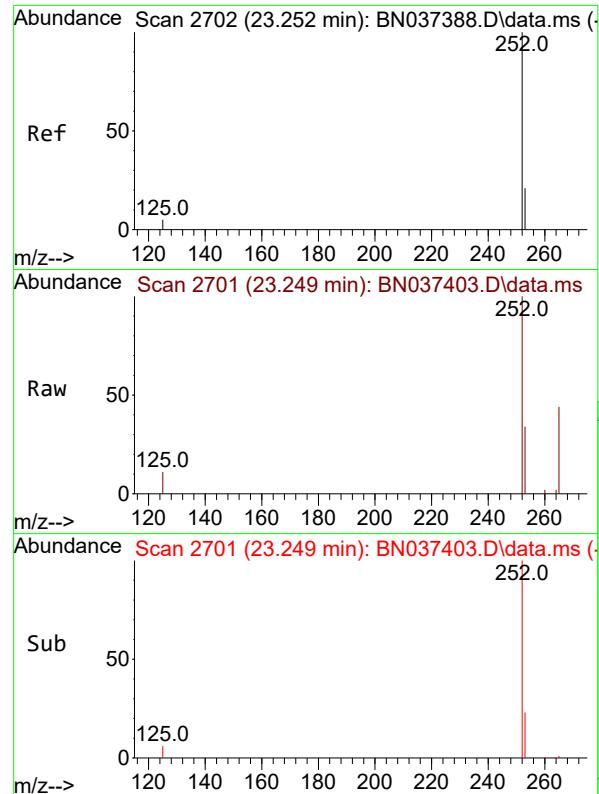


#39  
Benzo(a)pyrene  
Concen: 0.391 ng  
RT: 23.249 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.003 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38  
ClientSampleId : SSTDCCCC0.4


Tgt Ion:252 Resp: 5244  
Ion Ratio Lower Upper  
252 100  
253 34.2 25.6 38.4  
125 10.6 7.5 11.3

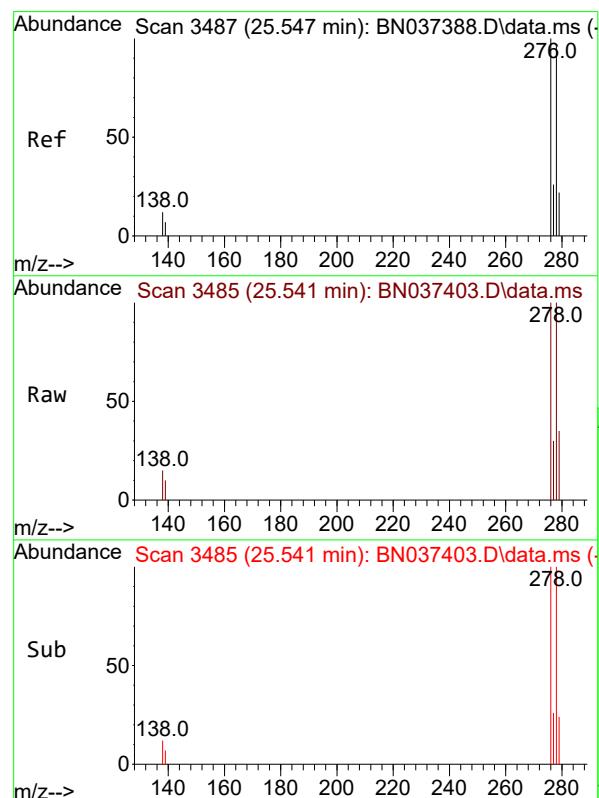

#40  
Dibenzo(a,h)anthracene  
Concen: 0.403 ng  
RT: 25.541 min Scan# 3485  
Delta R.T. -0.006 min  
Lab File: BN037403.D  
Acq: 26 Jun 2025 21:38

Tgt Ion:278 Resp: 5585  
Ion Ratio Lower Upper  
278 100  
139 10.5 8.5 12.7  
279 35.6 27.5 41.3

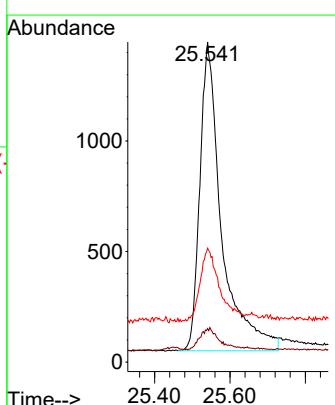

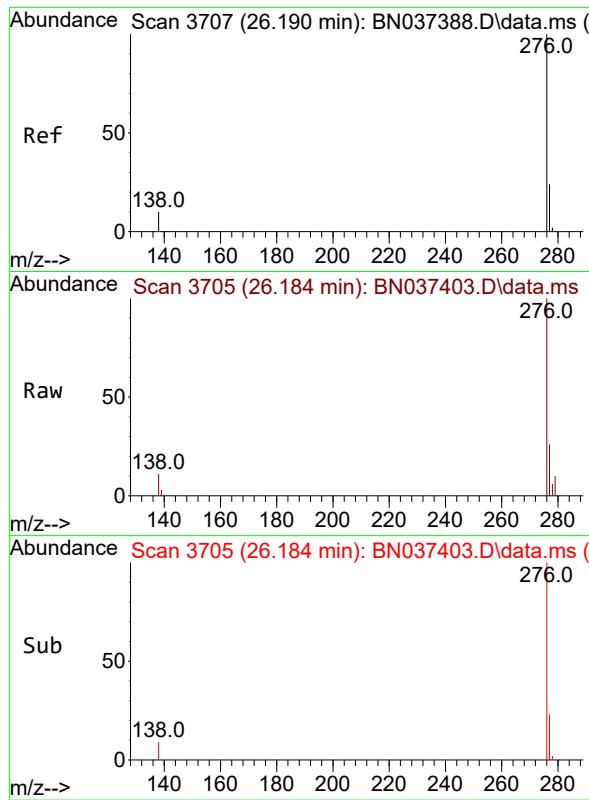

#41

Benzo(g,h,i)perylene

Concen: 0.387 ng

RT: 26.184 min Scan# 3

Instrument :

BNA\_N

Delta R.T. -0.006 min

ClientSampleId :

Lab File: BN037403.D

Acq: 26 Jun 2025 21:38

SSTDCCC0.4


Tgt Ion:276 Resp: 6411

Ion Ratio Lower Upper

276 100

277 25.7 21.0 31.4

138 11.4 9.6 14.4

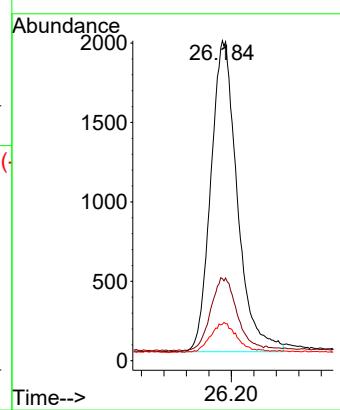

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037403.D  
 Acq On : 26 Jun 2025 21:38  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 LabSampleId :  
 SSTDCCC0.4

Quant Time: Jun 27 03:00:38 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	59	0.00
2	1,4-Dioxane	0.379	0.373	1.6	60	0.00
3	n-Nitrosodimethylamine	0.375	0.374	0.3	59	0.00
4 S	2-Fluorophenol	0.771	0.749	2.9	55	0.00
5 S	Phenol-d6	0.799	0.782	2.1	57	0.00
6	bis(2-Chloroethyl)ether	0.711	0.661	7.0	54	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	60	0.00
8 S	Nitrobenzene-d5	0.321	0.301	6.2	58	0.00
9	Naphthalene	1.030	1.007	2.2	61	-0.01
10	Hexachlorobutadiene	0.409	0.453	-10.8	66	0.00
11 SURR	2-Methylnaphthalene-d10	0.619	0.590	4.7	62	0.00
12	2-Methylnaphthalene	0.709	0.682	3.8	60	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	60	0.00
14 S	2,4,6-Tribromophenol	0.235	0.289	-23.0	73	0.00
15 S	2-Fluorobiphenyl	1.727	1.728	-0.1	61	0.00
16	Acenaphthylene	1.659	1.585	4.5	61	-0.01
17	Acenaphthene	1.083	1.020	5.8	59	0.00
18	Fluorene	1.530	1.508	1.4	62	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	63	0.00
20	4,6-Dinitro-2-methylphenol	0.103	0.109	-5.8	81	0.00
21	4-Bromophenyl-phenylether	0.282	0.287	-1.8	67	0.00
22	Hexachlorobenzene	0.303	0.311	-2.6	65	0.00
23	Atrazine	0.224	0.226	-0.9	67	-0.01
24	Pentachlorophenol	0.164	0.185	-12.8	76	0.00
25	Phenanthrene	1.127	1.072	4.9	63	0.00
26	Anthracene	1.036	1.003	3.2	66	0.00
27 SURR	Fluoranthene-d10	1.146	1.145	0.1	68	0.00
28	Fluoranthene	1.439	1.440	-0.1	67	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	70	0.00
30	Pyrene	1.514	1.445	4.6	66	0.00
31 S	Terphenyl-d14	0.853	0.867	-1.6	70	0.00
32	Benzo(a)anthracene	1.257	1.206	4.1	73	0.00
33	Chrysene	1.556	1.593	-2.4	71	0.00
34	Bis(2-ethylhexyl)phthalate	0.498	0.523	-5.0	73	0.00
35 I	Perylene-d12	1.000	1.000	0.0	72	0.00
36	Indeno(1,2,3-cd)pyrene	1.686	1.678	0.5	77	0.00
37	Benzo(b)fluoranthene	1.410	1.343	4.8	73	0.00
38	Benzo(k)fluoranthene	1.507	1.515	-0.5	75	0.00
39 C	Benzo(a)pyrene	1.254	1.225	2.3	75	0.00
40	Dibenzo(a,h)anthracene	1.296	1.305	-0.7	78	0.00
41	Benzo(g,h,i)perylene	1.548	1.498	3.2	73	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037403.D  
 Acq On : 26 Jun 2025 21:38  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 LabSampleId :  
 SSTDCCC0.4

Quant Time: Jun 27 03:00:38 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	59	0.00
2	1,4-Dioxane	0.400	0.393	1.8	60	0.00
3	n-Nitrosodimethylamine	0.400	0.400	0.0	59	0.00
4 S	2-Fluorophenol	0.400	0.389	2.8	55	0.00
5 S	Phenol-d6	0.400	0.391	2.3	57	0.00
6	bis(2-Chloroethyl)ether	0.400	0.372	7.0	54	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	60	0.00
8 S	Nitrobenzene-d5	0.400	0.375	6.3	58	0.00
9	Naphthalene	0.400	0.391	2.3	61	-0.01
10	Hexachlorobutadiene	0.400	0.443	-10.7	66	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.382	4.5	62	0.00
12	2-Methylnaphthalene	0.400	0.385	3.8	60	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	60	0.00
14 S	2,4,6-Tribromophenol	0.400	0.492	-23.0	73	0.00
15 S	2-Fluorobiphenyl	0.400	0.400	0.0	61	0.00
16	Acenaphthylene	0.400	0.382	4.5	61	-0.01
17	Acenaphthene	0.400	0.376	6.0	59	0.00
18	Fluorene	0.400	0.394	1.5	62	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	63	0.00
20	4,6-Dinitro-2-methylphenol	0.400	0.426	-6.5	81	0.00
21	4-Bromophenyl-phenylether	0.400	0.407	-1.7	67	0.00
22	Hexachlorobenzene	0.400	0.410	-2.5	65	0.00
23	Atrazine	0.400	0.405	-1.3	67	-0.01
24	Pentachlorophenol	0.400	0.452	-13.0	76	0.00
25	Phenanthrene	0.400	0.381	4.8	63	0.00
26	Anthracene	0.400	0.387	3.3	66	0.00
27 SURR	Fluoranthene-d10	0.400	0.400	0.0	68	0.00
28	Fluoranthene	0.400	0.400	0.0	67	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	70	0.00
30	Pyrene	0.400	0.382	4.5	66	0.00
31 S	Terphenyl-d14	0.400	0.407	-1.7	70	0.00
32	Benzo(a)anthracene	0.400	0.384	4.0	73	0.00
33	Chrysene	0.400	0.410	-2.5	71	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.420	-5.0	73	0.00
35 I	Perylene-d12	0.400	0.400	0.0	72	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.398	0.5	77	0.00
37	Benzo(b)fluoranthene	0.400	0.381	4.8	73	0.00
38	Benzo(k)fluoranthene	0.400	0.402	-0.5	75	0.00
39 C	Benzo(a)pyrene	0.400	0.391	2.3	75	0.00
40	Dibenzo(a,h)anthracene	0.400	0.403	-0.8	78	0.00
41	Benzo(g,h,i)perylene	0.400	0.387	3.3	73	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

7C

## SEMIVOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	<u>CHEMTECH</u>		Contract:	<u>TETR06</u>	
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q2375</u>	SAS No.:	<u>Q2375</u>
Instrument ID:	<u>BNA_N</u>		Calibration Date/Time:	<u>06/27/2025</u>	<u>04:54</u>
Lab File ID:	<u>BN037415.D</u>		Init. Calib. Date(s):	<u>06/26/2025</u>	<u>06/26/2025</u>
EPA Sample No.:	<u>SSTDCCC0.4EC</u>		Init. Calib. Time(s):	<u>10:41</u>	<u>14:17</u>
GC Column:	<u>ZB-GR</u>	ID: <u>0.25</u>	(mm)		

COMPOUND	RRF	RRF0.4	MIN RRF	%D	MAX%D
2-Methylnaphthalene-d10	0.619	0.582		-6.0	50.0
Fluoranthene-d10	1.146	1.097		-4.3	50.0
2-Fluorophenol	0.771	0.782		1.4	50.0
Phenol-d6	0.799	0.787		-1.5	50.0
Nitrobenzene-d5	0.321	0.289		-10.0	50.0
2-Fluorobiphenyl	1.727	1.699		-1.6	50.0
2,4,6-Tribromophenol	0.235	0.235		0.0	50.0
Terphenyl-d14	0.853	0.849		-0.5	50.0
1,4-Dioxane	0.379	0.394		4.0	50.0

All other compounds must meet a minimum RRF of 0.010.

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037415.D  
 Acq On : 27 Jun 2025 04:54  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4EC

Quant Time: Jun 27 05:26:40 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.560	152	1911	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4152	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	2803	0.400	ng	0.00
19) Phenanthrene-d10	16.959	188	5832	0.400	ng	0.00
29) Chrysene-d12	21.162	240	5618	0.400	ng	0.00
35) Perylene-d12	23.342	264	5931	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1495	0.406	ng	0.00
5) Phenol-d6	6.744	99	1504	0.394	ng	0.00
8) Nitrobenzene-d5	8.717	82	1198	0.360	ng	0.00
11) 2-Methylnaphthalene-d10	11.940	152	2415	0.376	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	658	0.400	ng	0.00
15) 2-Fluorobiphenyl	12.833	172	4761	0.393	ng	0.00
27) Fluoranthene-d10	19.003	212	6400	0.383	ng	0.00
31) Terphenyl-d14	19.611	244	4769	0.398	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.097	88	752	0.415	ng	92
3) n-Nitrosodimethylamine	3.415	42	652	0.364	ng	83
6) bis(2-Chloroethyl)ether	6.997	93	1118	0.329	ng	90
9) Naphthalene	10.383	128	4123	0.386	ng	98
10) Hexachlorobutadiene	10.682	225	1736	0.409	ng	# 97
12) 2-Methylnaphthalene	12.016	142	2789	0.379	ng	99
16) Acenaphthylene	13.924	152	4361	0.375	ng	98
17) Acenaphthene	14.277	154	2865	0.377	ng	99
18) Fluorene	15.271	166	4105	0.383	ng	100
20) 4,6-Dinitro-2-methylph...	15.368	198	405	0.270	ng	# 83
21) 4-Bromophenyl-phenylether	16.164	248	1533	0.373	ng	98
22) Hexachlorobenzene	16.276	284	1783	0.403	ng	98
23) Atrazine	16.450	200	1260	0.387	ng	98
24) Pentachlorophenol	16.624	266	828	0.347	ng	98
25) Phenanthrene	17.008	178	6159	0.375	ng	99
26) Anthracene	17.095	178	5663	0.375	ng	99
28) Fluoranthene	19.031	202	8012	0.382	ng	100
30) Pyrene	19.393	202	8391	0.395	ng	100
32) Benzo(a)anthracene	21.144	228	6423	0.364	ng	99
33) Chrysene	21.197	228	9016	0.413	ng	100
34) Bis(2-ethylhexyl)phtha...	21.090	149	2930	0.419	ng	98
36) Indeno(1,2,3-cd)pyrene	25.523	276	9870	0.395	ng	97
37) Benzo(b)fluoranthene	22.693	252	7809	0.373	ng	98
38) Benzo(k)fluoranthene	22.737	252	8852	0.396	ng	97
39) Benzo(a)pyrene	23.249	252	7434	0.400	ng	# 96
40) Dibenzo(a,h)anthracene	25.544	278	7351	0.383	ng	99
41) Benzo(g,h,i)perylene	26.184	276	8948	0.390	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037415.D  
 Acq On : 27 Jun 2025 04:54  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4EC


Quant Time: Jun 27 05:26:40 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

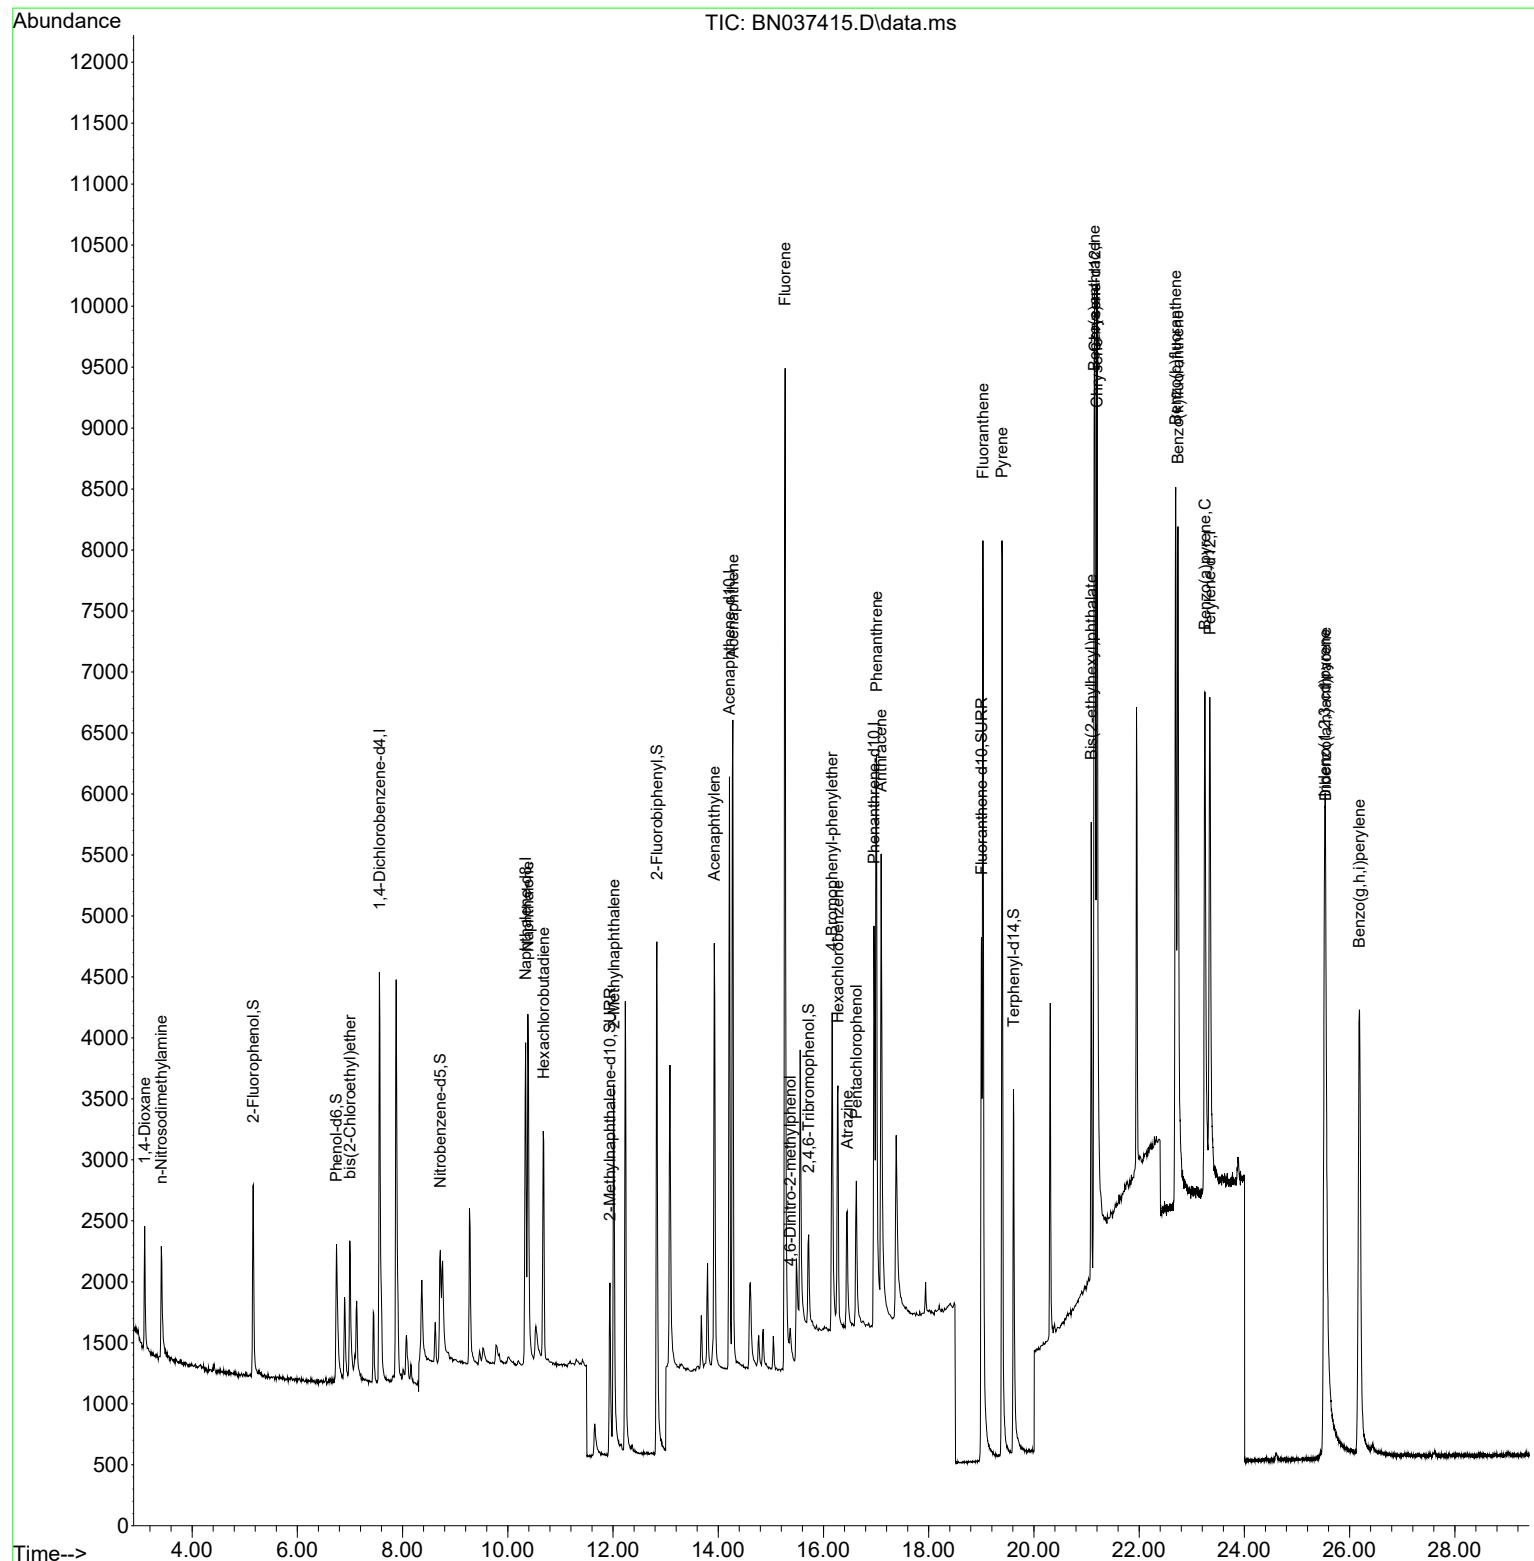






#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.560 min Scan# 6  
Delta R.T. -0.008 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC





Tgt Ion:152 Resp: 1911  
Ion Ratio Lower Upper  
152 100  
150 150.8 116.2 174.2  
115 55.1 42.9 64.3


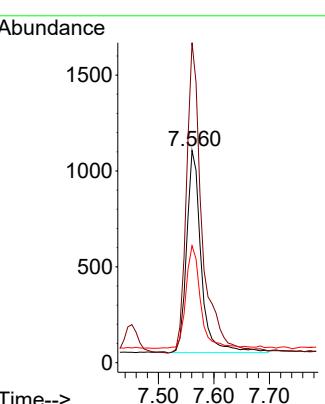
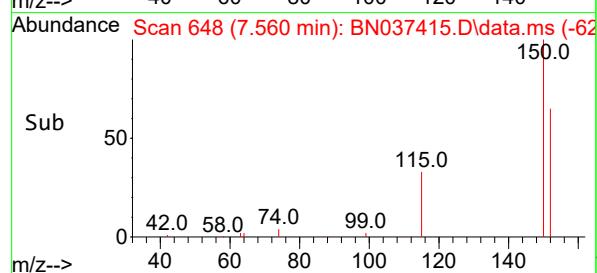


#2  
1,4-Dioxane  
Concen: 0.415 ng  
RT: 3.097 min Scan# 30  
Delta R.T. -0.007 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54



Tgt Ion: 88 Resp: 752  
Ion Ratio Lower Upper  
88 100  
43 23.9 21.6 32.4  
58 51.1 45.9 68.9

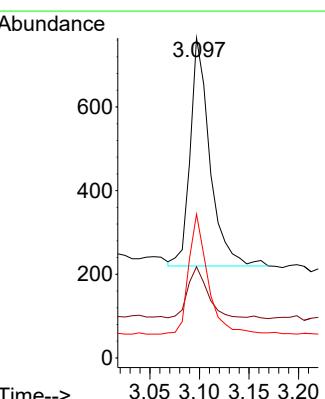

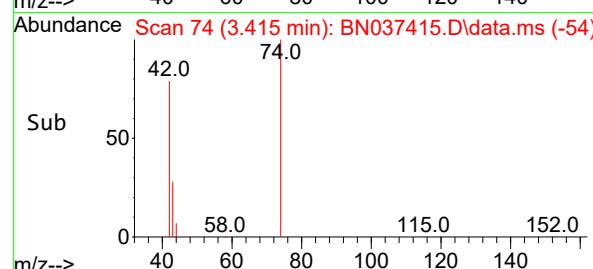

#3

n-Nitrosodimethylamine

Concen: 0.364 ng

RT: 3.415 min Scan# 7

Delta R.T. -0.007 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion: 42 Resp: 652

Ion Ratio Lower Upper

42 100

74 142.6 97.8 146.8

44 9.2 8.7 13.1

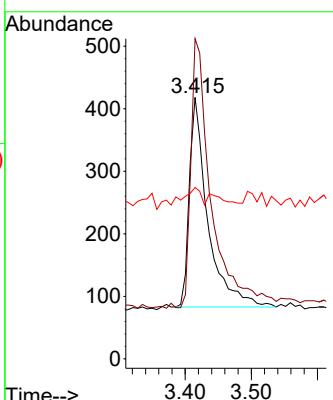

#4

2-Fluorophenol

Concen: 0.406 ng

RT: 5.163 min Scan# 316

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54


Tgt Ion: 112 Resp: 1495




Ion Ratio Lower Upper

112 100

64 49.6 40.3 60.5

63 32.4 26.1 39.1




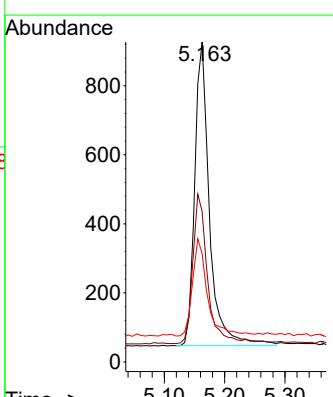


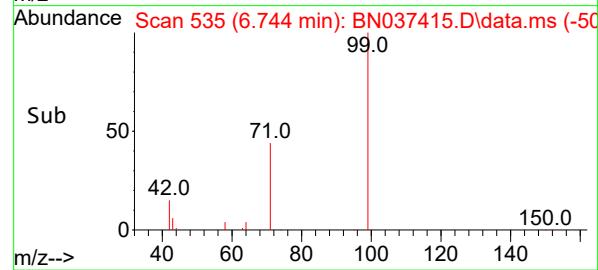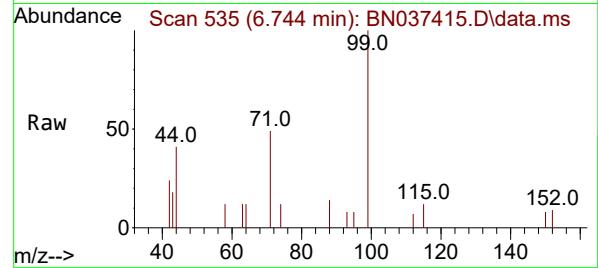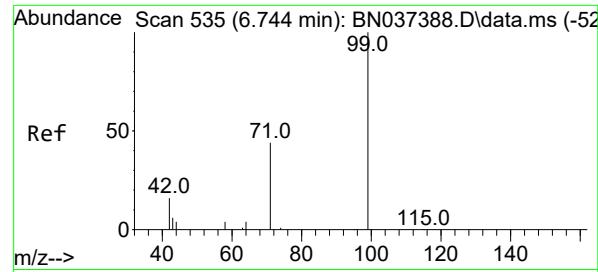

#5  
Phenol-d6  
Concen: 0.394 ng  
RT: 6.744 min Scan# 5  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC




Tgt Ion: 99 Resp: 1504  
Ion Ratio Lower Upper  
99 100  
42 16.6 15.6 23.4  
71 43.2 35.8 53.8

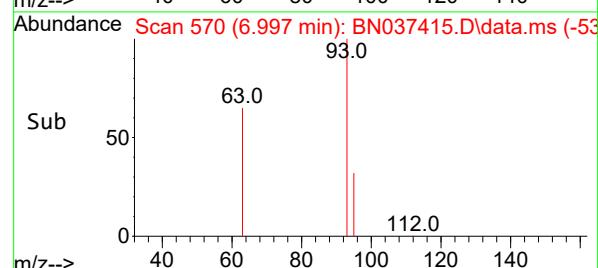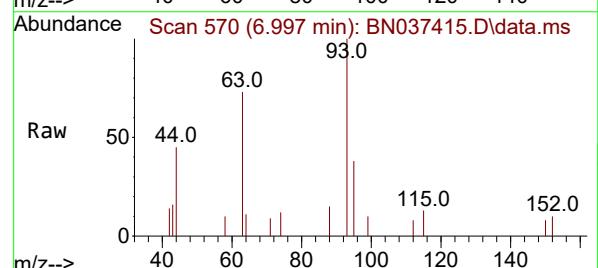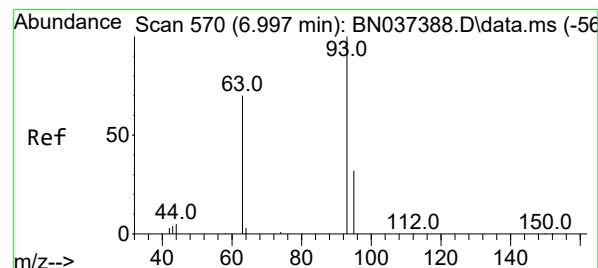

#6  
bis(2-Chloroethyl)ether  
Concen: 0.329 ng  
RT: 6.997 min Scan# 570  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion: 93 Resp: 1118  
Ion Ratio Lower Upper  
93 100  
63 69.5 49.6 74.4  
95 35.8 23.9 35.9




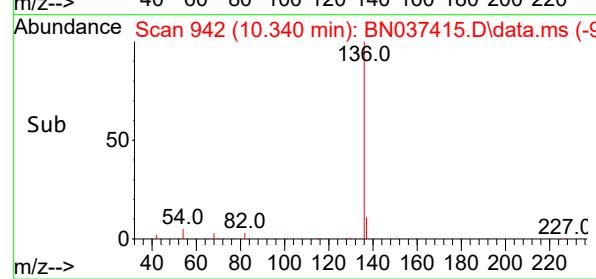




#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037415.D  
 Acq: 27 Jun 2025 04:54

Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC

Tgt Ion:136 Resp: 4152


	Ion Ratio	Lower	Upper
136	100		
137	13.1	10.4	15.6
54	6.8	5.6	8.4
68	5.8	4.6	6.8






#8  
 Nitrobenzene-d5  
 Concen: 0.360 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. -0.000 min  
 Lab File: BN037415.D  
 Acq: 27 Jun 2025 04:54

Tgt Ion: 82 Resp: 1198

	Ion Ratio	Lower	Upper
82	100		
128	47.3	34.0	51.0
54	44.1	37.7	56.5

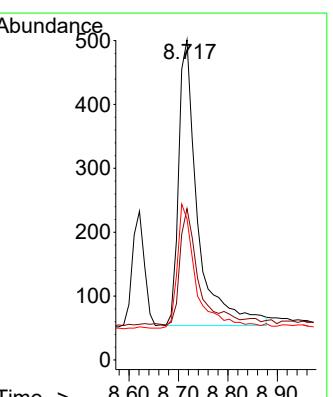

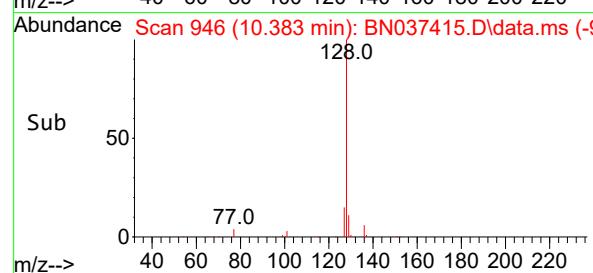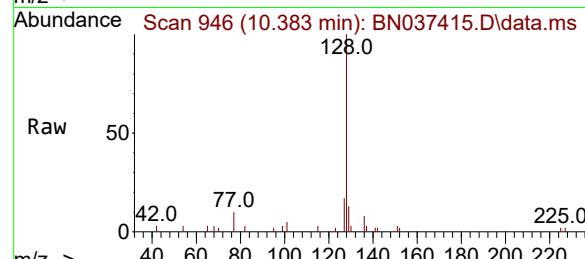

#9

Naphthalene

Concen: 0.386 ng

RT: 10.383 min Scan# 9

Delta R.T. -0.011 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:128 Resp: 4123

Ion Ratio Lower Upper

128 100

129 13.1 10.4 15.6

127 16.5 12.2 18.4

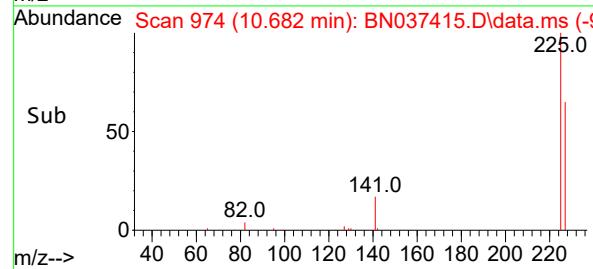

#10

Hexachlorobutadiene

Concen: 0.409 ng

RT: 10.682 min Scan# 974

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54


Tgt Ion:225 Resp: 1736




Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 64.6 49.9 74.9




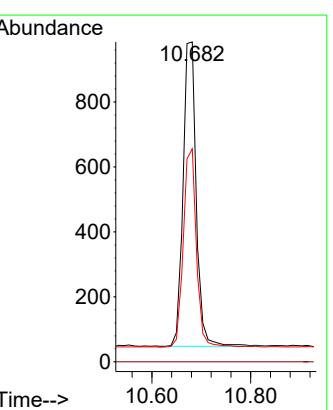


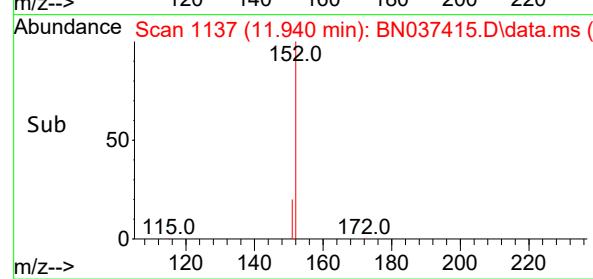

#11  
2-Methylnaphthalene-d10  
Concen: 0.376 ng  
RT: 11.940 min Scan# 1137  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC


Tgt Ion:152 Resp: 2415  
Ion Ratio Lower Upper  
152 100  
151 22.1 18.4 27.6



#12  
2-Methylnaphthalene  
Concen: 0.379 ng  
RT: 12.016 min Scan# 1152  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion:142 Resp: 2789  
Ion Ratio Lower Upper  
142 100  
141 88.5 70.1 105.1  
115 43.4 35.8 53.6

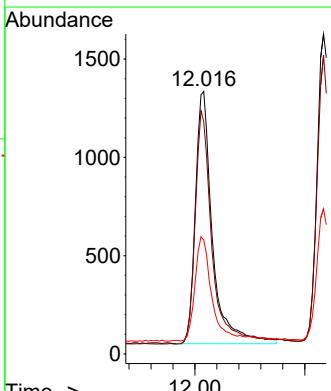

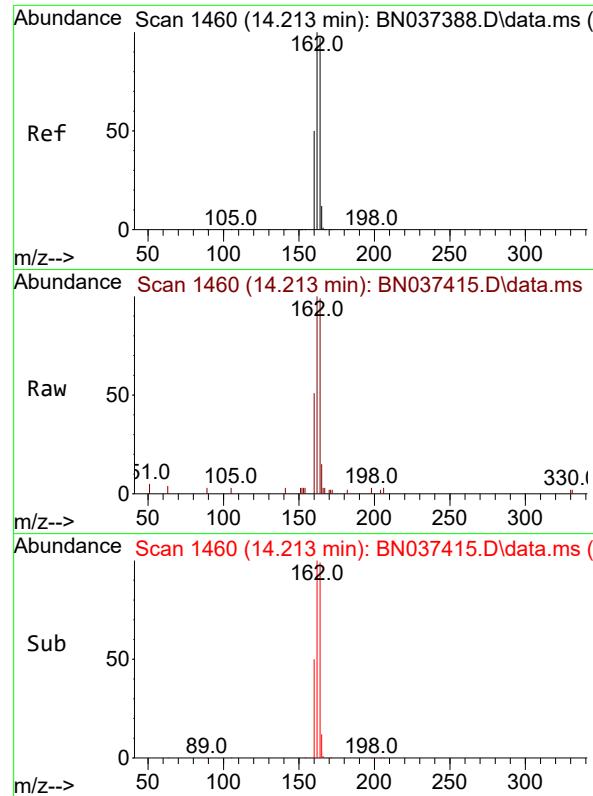

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.213 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:164 Resp: 2803

Ion Ratio Lower Upper



164 100

162 100.9 82.6 123.8

160 51.1 42.2 63.2

Abundance

14.213

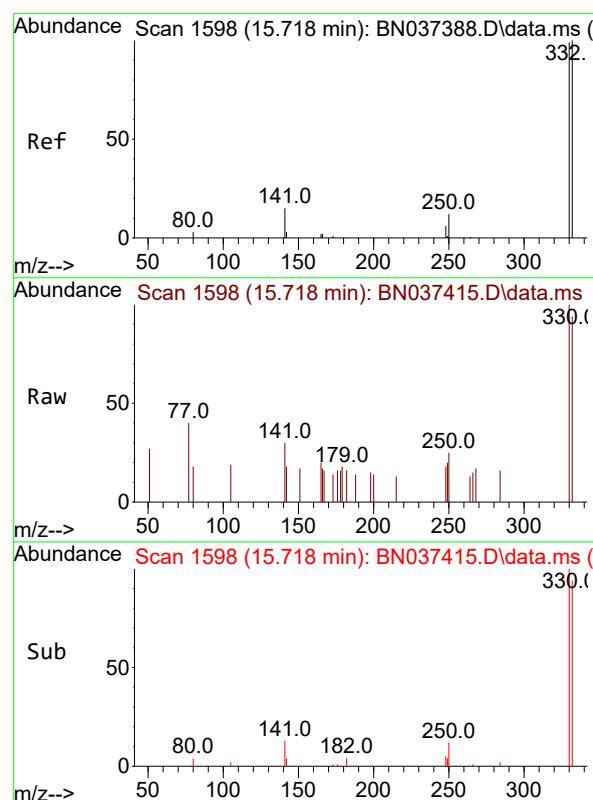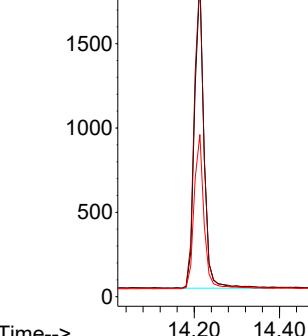

#14

2,4,6-Tribromophenol

Concen: 0.400 ng

RT: 15.718 min Scan# 1598

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Tgt Ion:330 Resp: 658

Ion Ratio Lower Upper


330 100




332 97.0 77.8 116.8

141 28.6 24.0 36.0

Abundance

15.718




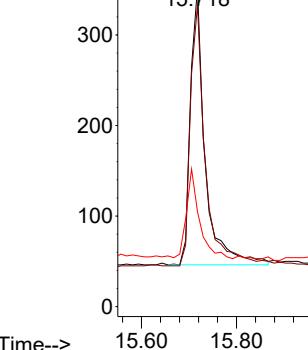


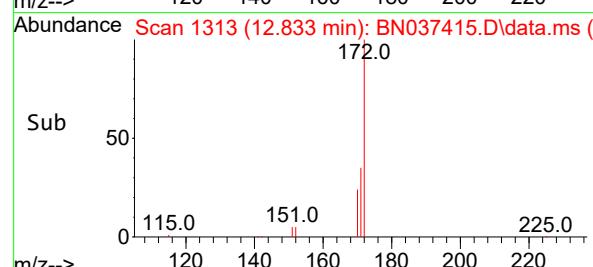

#15  
2-Fluorobiphenyl  
Concen: 0.393 ng  
RT: 12.833 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC




Tgt Ion:172 Resp: 4761  
Ion Ratio Lower Upper  
172 100  
171 36.5 28.8 43.2  
170 25.2 20.3 30.5



#16  
Acenaphthylene  
Concen: 0.375 ng  
RT: 13.924 min Scan# 1433  
Delta R.T. -0.011 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion:152 Resp: 4361  
Ion Ratio Lower Upper  
152 100  
151 20.6 15.8 23.6  
153 13.5 10.3 15.5

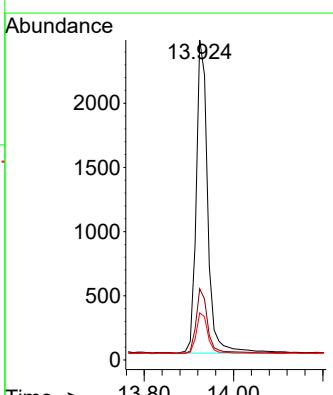



#17

Acenaphthene

Concen: 0.377 ng

RT: 14.277 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC




Tgt Ion:154 Resp: 2865

Ion Ratio Lower Upper

154 100

153 118.2 94.6 141.8

152 61.0 50.2 75.2



#18

Fluorene

Concen: 0.383 ng

RT: 15.271 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54


Tgt Ion:166 Resp: 4105

Ion Ratio Lower Upper

166 100

165 99.5 79.4 119.2

167 13.5 10.6 15.8



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.959 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037415.D




Acq: 27 Jun 2025 04:54

Instrument:

BNA\_N

ClientSampleId :

SSTDCCC0.4EC

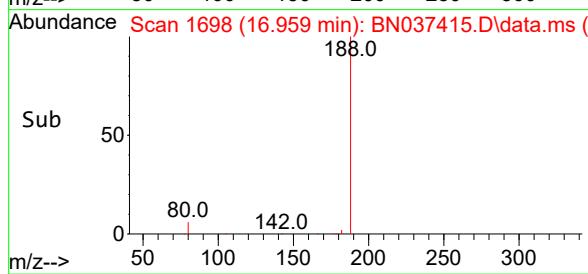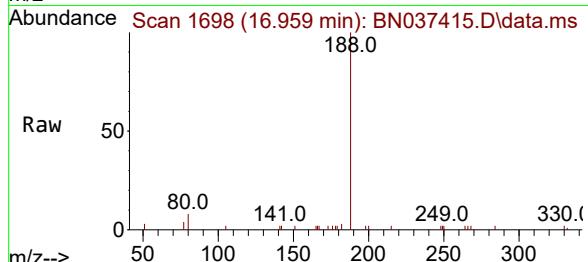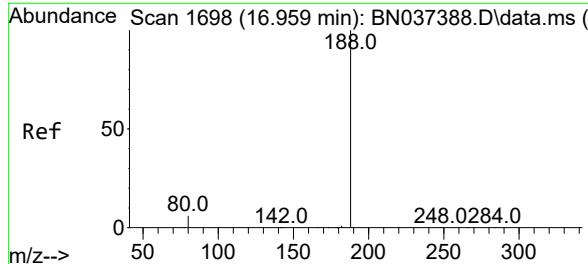





Tgt Ion:188 Resp: 5832

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 8.0 6.2 9.4

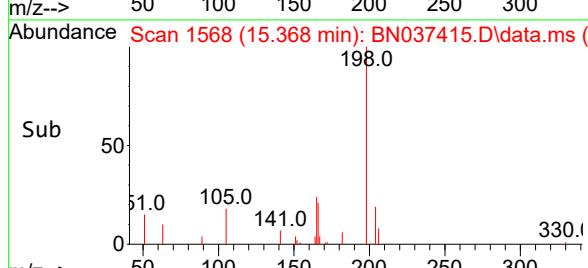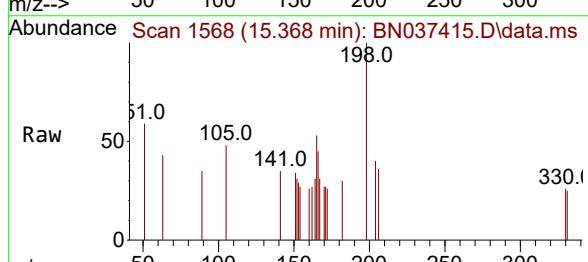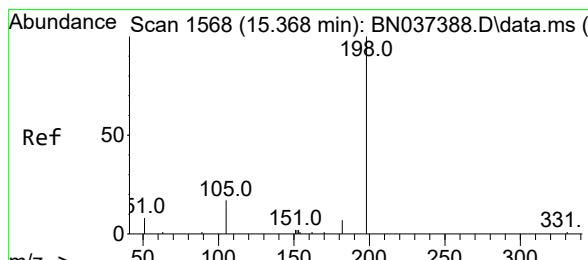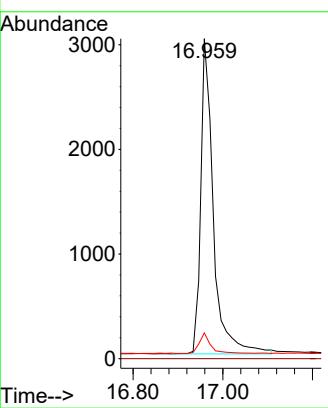

#20

4,6-Dinitro-2-methylphenol

Concen: 0.270 ng

RT: 15.368 min Scan# 1568

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54


Tgt Ion:198 Resp: 405


Ion Ratio Lower Upper

198 100

51 59.3 38.8 58.2#

105 48.4 29.8 44.6#


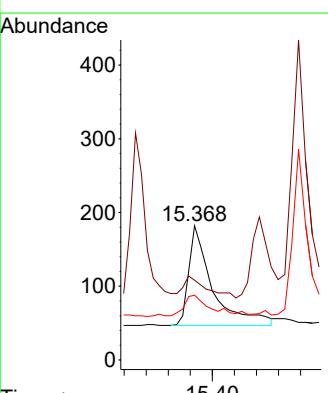


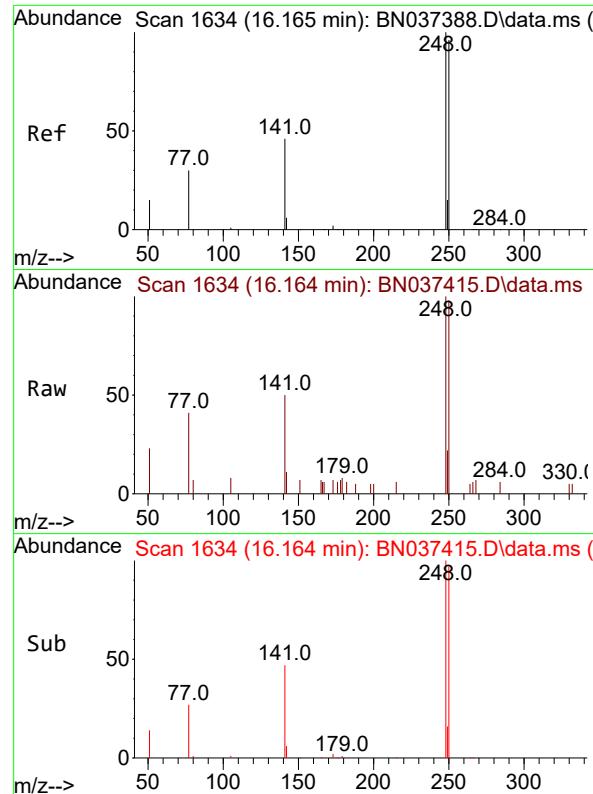

#21  
4-Bromophenyl-phenylether  
Concen: 0.373 ng  
RT: 16.164 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC




Tgt Ion:248 Resp: 1533  
Ion Ratio Lower Upper  
248 100  
250 97.6 77.0 115.4  
141 50.0 38.7 58.1

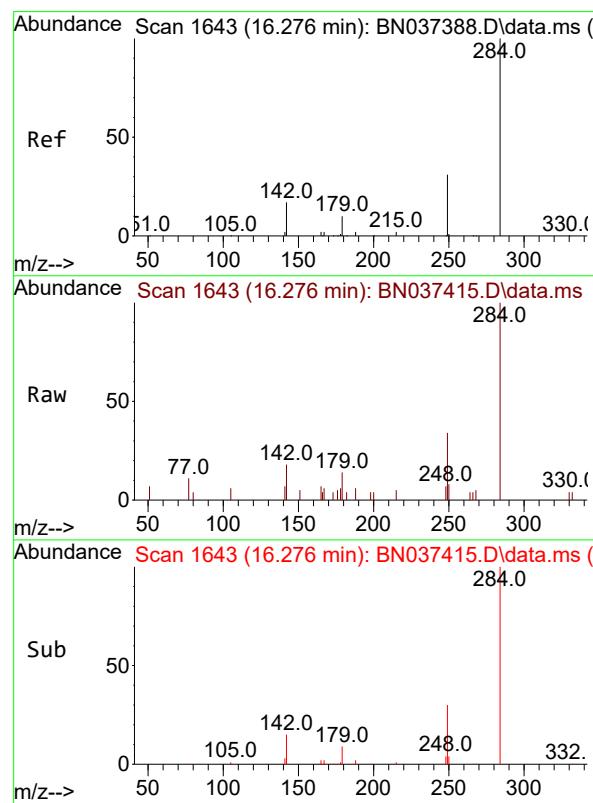

#22  
Hexachlorobenzene  
Concen: 0.403 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion:284 Resp: 1783  
Ion Ratio Lower Upper  
284 100  
142 33.3 27.2 40.8  
249 34.9 26.7 40.1



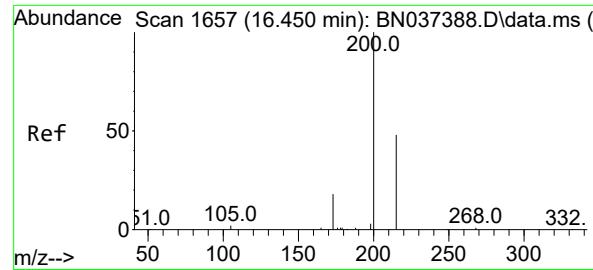

#23

Atrazine

Concen: 0.387 ng

RT: 16.450 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:200 Resp: 1260

Ion Ratio Lower Upper

200 100

173 23.5 19.0 28.6

215 53.2 41.3 61.9



#24

Pentachlorophenol

Concen: 0.347 ng

RT: 16.624 min Scan# 1671

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54


Tgt Ion:266 Resp: 828




Ion Ratio Lower Upper

266 100

264 64.0 49.2 73.8

268 66.7 54.2 81.4





#25

Phenanthrene

Concen: 0.375 ng

RT: 17.008 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument:

BNA\_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:178 Resp: 6159

Ion Ratio Lower Upper

178 100

176 20.1 15.6 23.4

179 15.9 12.8 19.2



#26

Anthracene

Concen: 0.375 ng

RT: 17.095 min Scan# 1709

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54


Tgt Ion:178 Resp: 5663




Ion Ratio Lower Upper

178 100

176 19.1 14.9 22.3

179 15.9 12.4 18.6




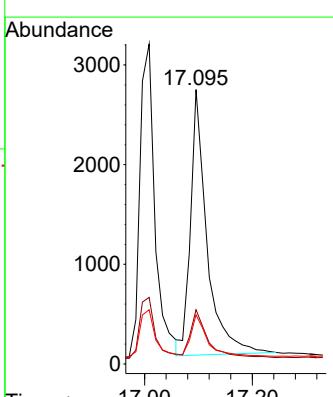




#27  
Fluoranthene-d10  
Concen: 0.383 ng  
RT: 19.003 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC




Tgt Ion:212 Resp: 6400  
Ion Ratio Lower Upper  
212 100  
106 5.7 4.5 6.7  
104 3.7 2.7 4.1



#28  
Fluoranthene  
Concen: 0.382 ng  
RT: 19.031 min Scan# 1935  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion:202 Resp: 8012  
Ion Ratio Lower Upper  
202 100  
101 4.9 3.8 5.6  
203 17.0 13.5 20.3

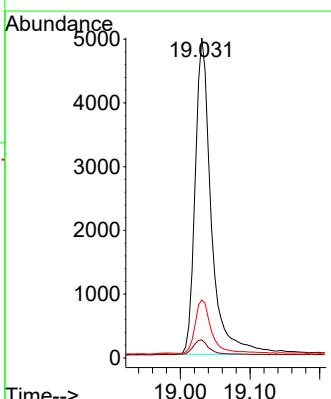



#29

Chrysene-d<sub>12</sub>

Concen: 0.400 ng

RT: 21.162 min Scan# 2

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:240 Resp: 5618

Ion Ratio Lower Upper

240 100

120 7.5





236 28.8

5.3

22.7

7.9

34.1

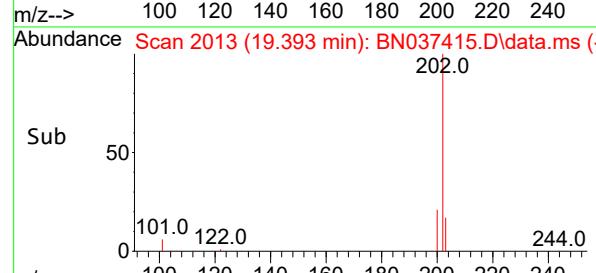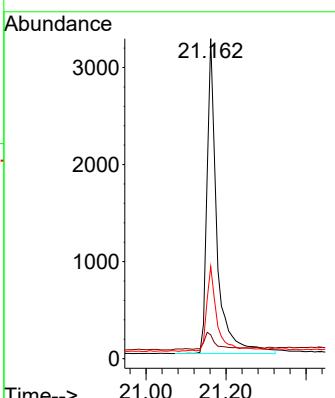

#30

Pyrene

Concen: 0.395 ng

RT: 19.393 min Scan# 2013

Delta R.T. -0.005 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Tgt Ion:202 Resp: 8391

Ion Ratio Lower Upper

202 100

200 20.6


203 17.7


16.5

24.7

14.2

21.2


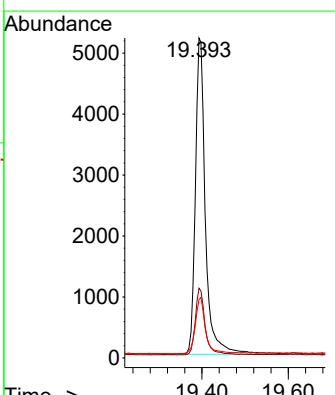


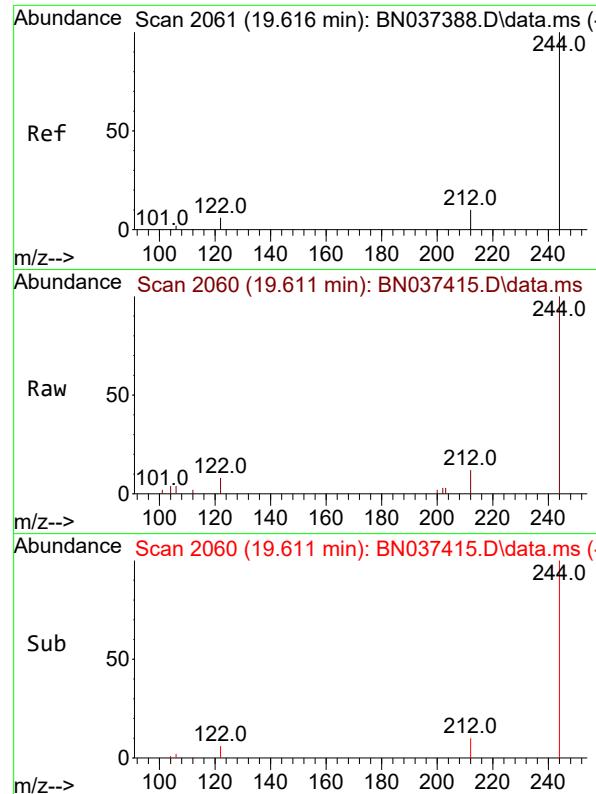

#31  
Terphenyl-d14  
Concen: 0.398 ng  
RT: 19.611 min Scan# 2  
Delta R.T. -0.005 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC




Tgt Ion:244 Resp: 4769  
Ion Ratio Lower Upper  
244 100  
212 11.6 9.1 13.7  
122 8.2 6.3 9.5

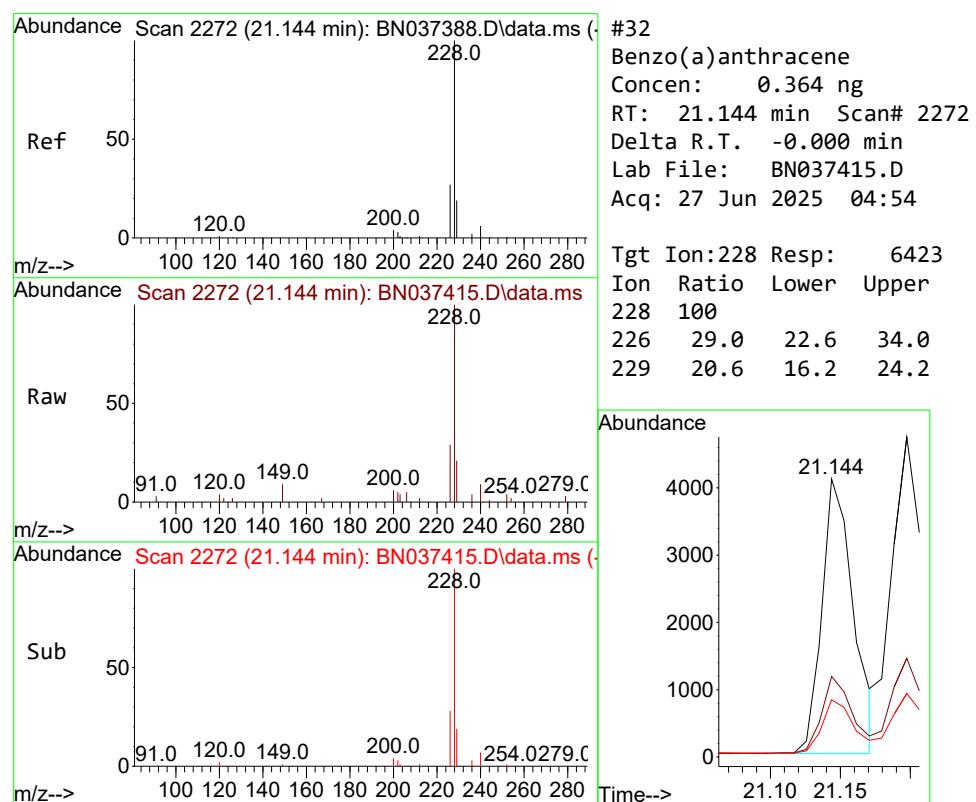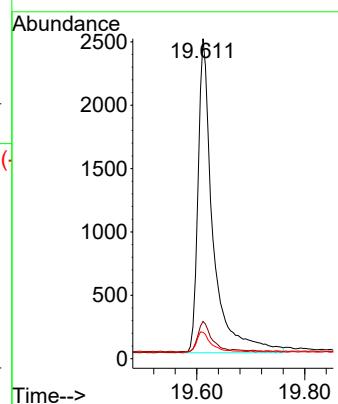

#32  
Benzo(a)anthracene  
Concen: 0.364 ng  
RT: 21.144 min Scan# 2272  
Delta R.T. -0.000 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion:228 Resp: 6423  
Ion Ratio Lower Upper  
228 100  
226 29.0 22.6 34.0  
229 20.6 16.2 24.2

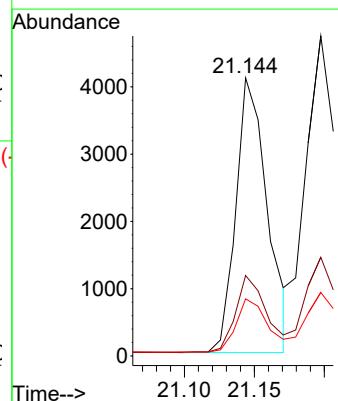

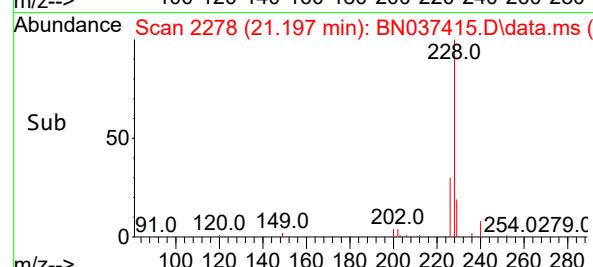

#33

Chrysene

Concen: 0.413 ng

RT: 21.197 min Scan# 2

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54

Instrument :

BNA\_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:228 Resp: 9016

Ion Ratio Lower Upper

228 100

226 30.9 24.5 36.7

229 19.9 16.1 24.1

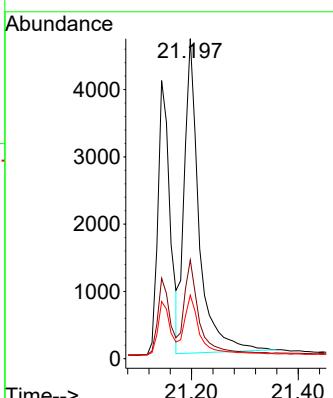

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.419 ng

RT: 21.090 min Scan# 2266

Delta R.T. -0.000 min

Lab File: BN037415.D

Acq: 27 Jun 2025 04:54


Tgt Ion:149 Resp: 2930


Ion Ratio Lower Upper

149 100

167 31.9 24.8 37.2

279 7.5 5.0 7.6


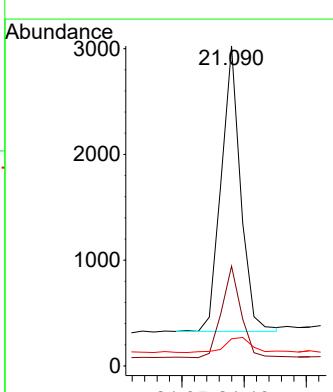


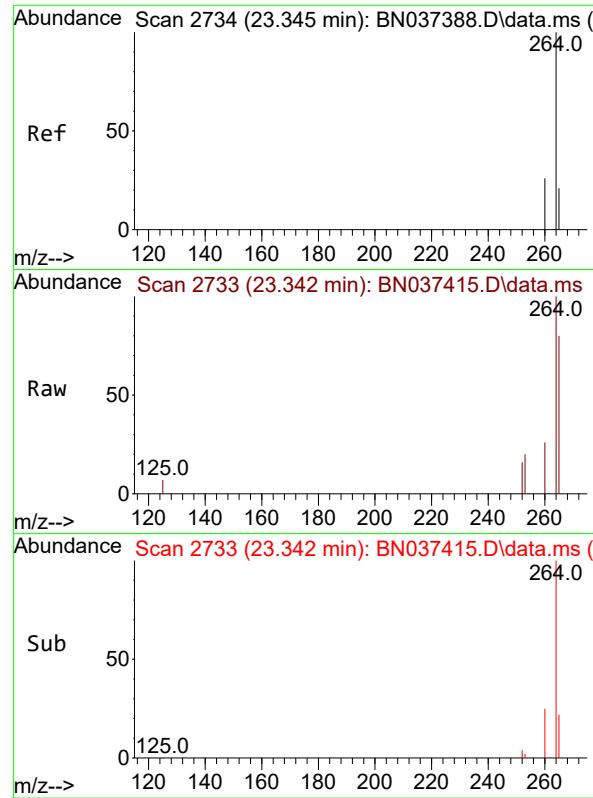

#35  
Perylene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 23.342 min Scan# 2  
Delta R.T. -0.003 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC


Tgt Ion:264 Resp: 5931  
Ion Ratio Lower Upper  
264 100  
260 26.2 21.4 32.0  
265 80.2 56.2 84.4

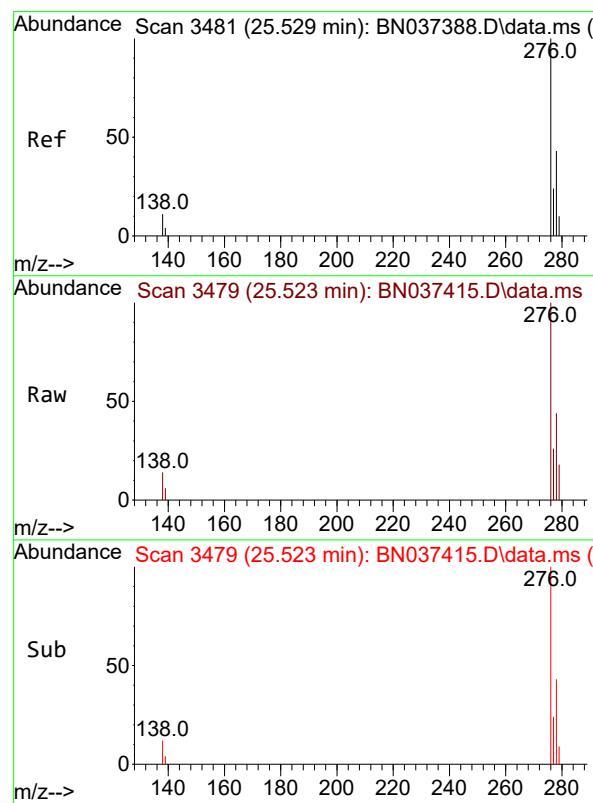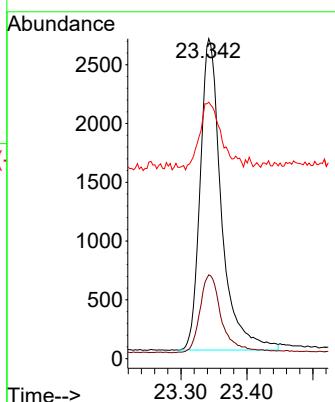

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.395 ng  
RT: 25.523 min Scan# 3479  
Delta R.T. -0.006 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion:276 Resp: 9870  
Ion Ratio Lower Upper  
276 100  
138 11.3 8.5 12.7  
277 22.8 19.7 29.5





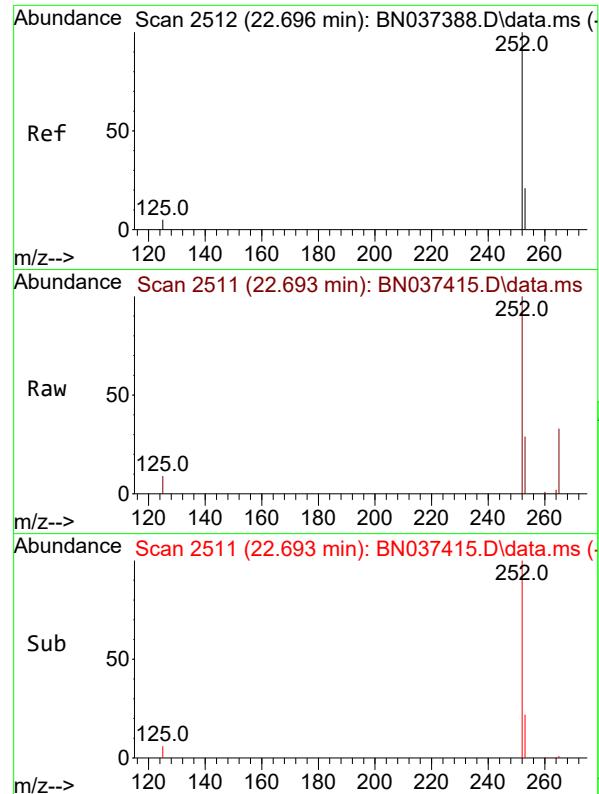

#37  
Benzo(b)fluoranthene  
Concen: 0.373 ng  
RT: 22.693 min Scan# 2  
Delta R.T. -0.003 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC


Tgt Ion:252 Resp: 7809  
Ion Ratio Lower Upper  
252 100  
253 29.5 22.8 34.2  
125 9.3 6.2 9.4

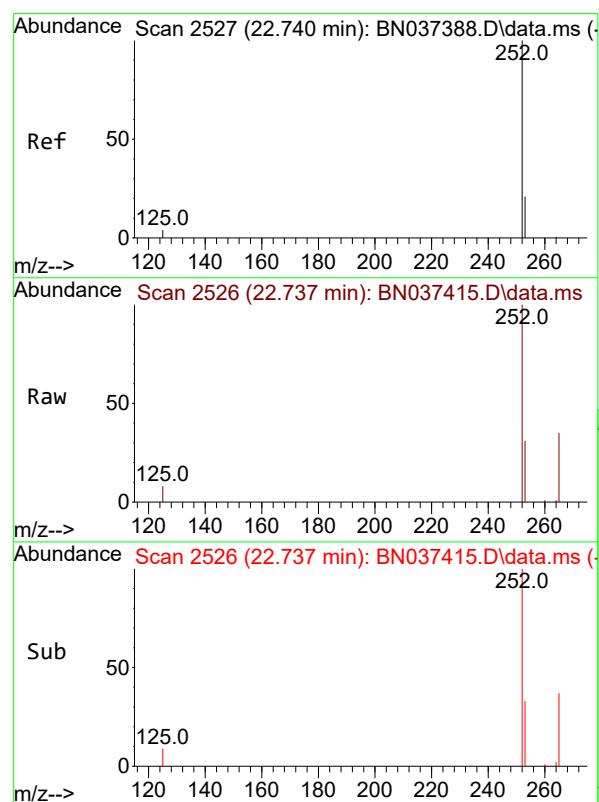

#38  
Benzo(k)fluoranthene  
Concen: 0.396 ng  
RT: 22.737 min Scan# 2526  
Delta R.T. -0.003 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54



Tgt Ion:252 Resp: 8852  
Ion Ratio Lower Upper  
252 100  
253 30.6 23.2 34.8  
125 8.1 6.0 9.0



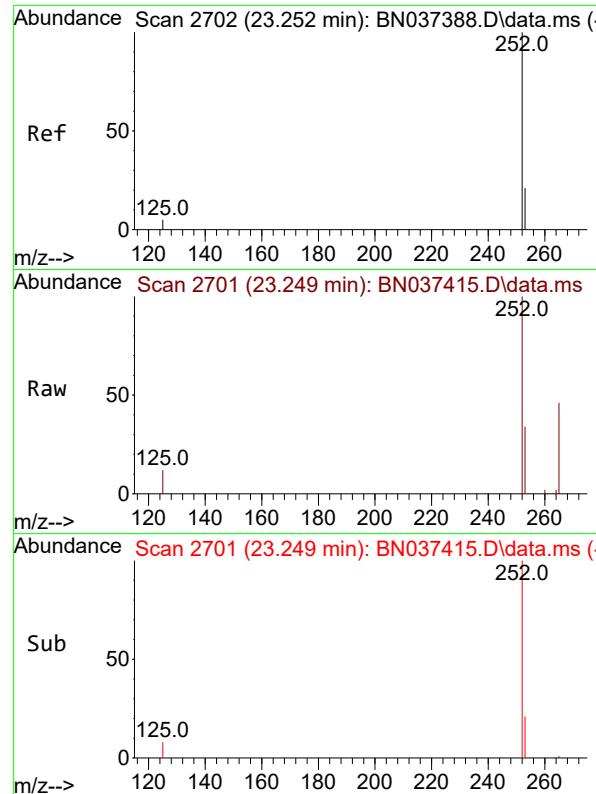


#39  
Benzo(a)pyrene  
Concen: 0.400 ng  
RT: 23.249 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.003 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54  
ClientSampleId : SSTDCCC0.4EC


Tgt Ion:252 Resp: 7434  
Ion Ratio Lower Upper  
252 100  
253 33.6 25.6 38.4  
125 12.3 7.5 11.3#

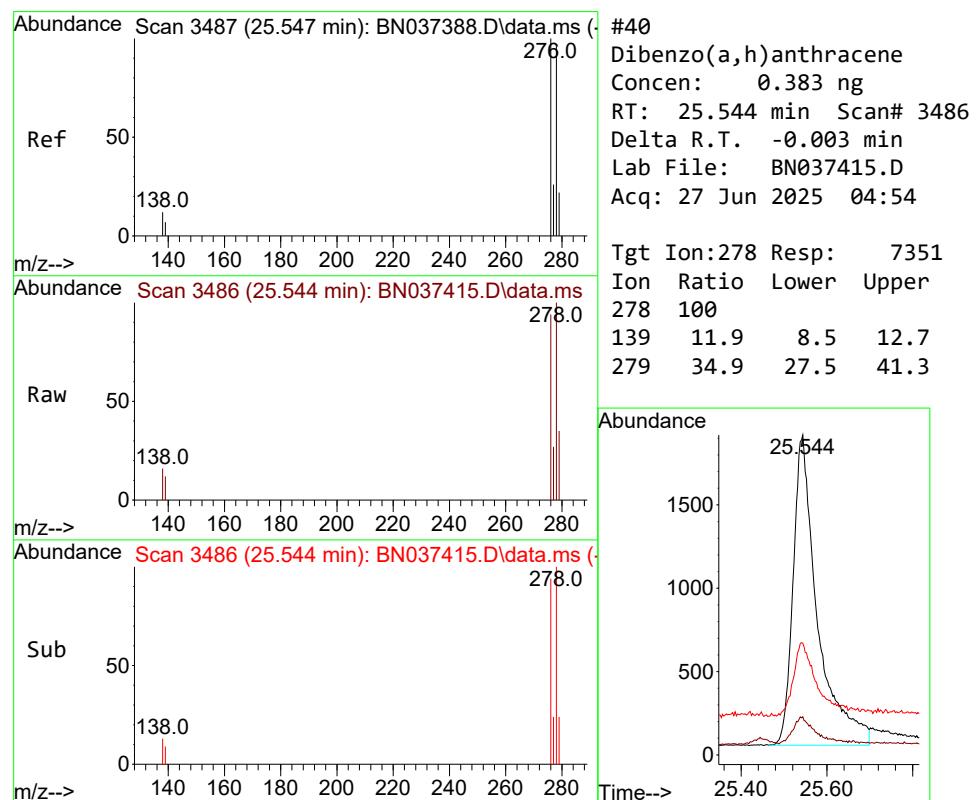

#40  
Dibenzo(a,h)anthracene  
Concen: 0.383 ng  
RT: 25.544 min Scan# 3486  
Delta R.T. -0.003 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Tgt Ion:278 Resp: 7351  
Ion Ratio Lower Upper  
278 100  
139 11.9 8.5 12.7  
279 34.9 27.5 41.3




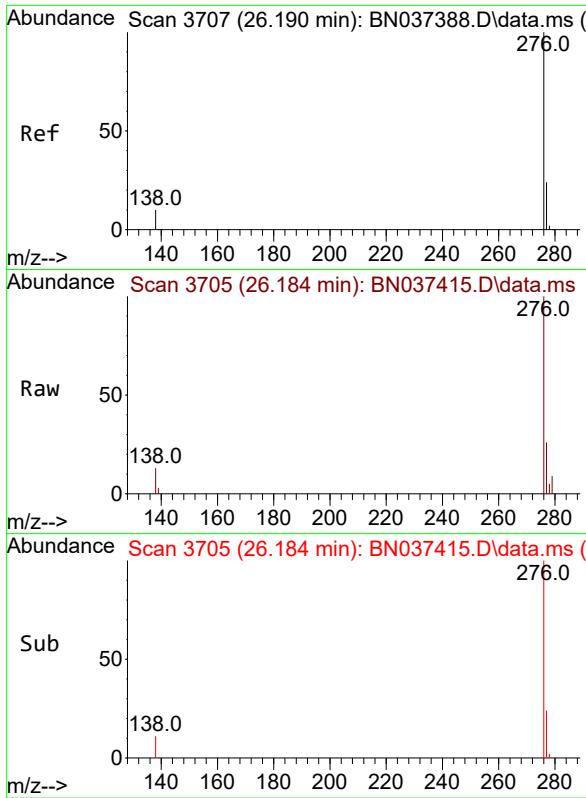

#41  
Benzo(g,h,i)perylene  
Concen: 0.390 ng  
RT: 26.184 min Scan# 3  
Delta R.T. -0.006 min  
Lab File: BN037415.D  
Acq: 27 Jun 2025 04:54

Instrument :  
BNA\_N  
ClientSampleId :  
SSTDCCC0.4EC

Tgt Ion:276 Resp: 8948  
Ion Ratio Lower Upper  
276 100  
277 25.9 21.0 31.4  
138 12.6 9.6 14.4

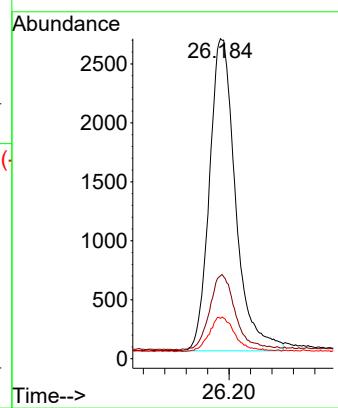

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037415.D  
 Acq On : 27 Jun 2025 04:54  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 LabSampleId :  
 SSTDCCC0.4

Quant Time: Jun 27 05:26:40 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	90	0.00
2	1,4-Dioxane	0.379	0.394	-4.0	96	0.00
3	n-Nitrosodimethylamine	0.375	0.341	9.1	82	0.00
4 S	2-Fluorophenol	0.771	0.782	-1.4	88	0.00
5 S	Phenol-d6	0.799	0.787	1.5	87	0.00
6	bis(2-Chloroethyl)ether	0.711	0.585	17.7	74	0.00
7 I	Naphthalene-d8	1.000	1.000	0.0	91	0.00
8 S	Nitrobenzene-d5	0.321	0.289	10.0	84	0.00
9	Naphthalene	1.030	0.993	3.6	90	-0.01
10	Hexachlorobutadiene	0.409	0.418	-2.2	92	0.00
11 SURR	2-Methylnaphthalene-d10	0.619	0.582	6.0	92	0.00
12	2-Methylnaphthalene	0.709	0.672	5.2	89	0.00
13 I	Acenaphthene-d10	1.000	1.000	0.0	92	0.00
14 S	2,4,6-Tribromophenol	0.235	0.235	0.0	90	0.00
15 S	2-Fluorobiphenyl	1.727	1.699	1.6	91	0.00
16	Acenaphthylene	1.659	1.556	6.2	91	-0.01
17	Acenaphthene	1.083	1.022	5.6	90	0.00
18	Fluorene	1.530	1.465	4.2	91	0.00
19 I	Phenanthrene-d10	1.000	1.000	0.0	93	0.00
20	4,6-Dinitro-2-methylphenol	0.103	0.069	33.0#	76	0.00
21	4-Bromophenyl-phenylether	0.282	0.263	6.7	90	0.00
22	Hexachlorobenzene	0.303	0.306	-1.0	94	0.00
23	Atrazine	0.224	0.216	3.6	94	0.00
24	Pentachlorophenol	0.164	0.142	13.4	85	0.00
25	Phenanthrene	1.127	1.056	6.3	91	0.00
26	Anthracene	1.036	0.971	6.3	93	0.00
27 SURR	Fluoranthene-d10	1.146	1.097	4.3	96	0.00
28	Fluoranthene	1.439	1.374	4.5	94	0.00
29 I	Chrysene-d12	1.000	1.000	0.0	100	0.00
30	Pyrene	1.514	1.494	1.3	97	0.00
31 S	Terphenyl-d14	0.853	0.849	0.5	98	0.00
32	Benzo(a)anthracene	1.257	1.143	9.1	98	0.00
33	Chrysene	1.556	1.605	-3.1	101	0.00
34	Bis(2-ethylhexyl)phthalate	0.498	0.522	-4.8	104	0.00
35 I	Perylene-d12	1.000	1.000	0.0	100	0.00
36	Indeno(1,2,3-cd)pyrene	1.686	1.664	1.3	105	0.00
37	Benzo(b)fluoranthene	1.410	1.317	6.6	100	0.00
38	Benzo(k)fluoranthene	1.507	1.492	1.0	102	0.00
39 C	Benzo(a)pyrene	1.254	1.253	0.1	106	0.00
40	Dibenzo(a,h)anthracene	1.296	1.239	4.4	102	0.00
41	Benzo(g,h,i)perylene	1.548	1.509	2.5	102	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037415.D  
 Acq On : 27 Jun 2025 04:54  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 LabSampleId :  
 SSTDCCC0.4

Quant Time: Jun 27 05:26:40 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:06:33 2025  
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min  
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	1,4-Dichlorobenzene-d4	0.400	0.400	0.0	90	0.00
2	1,4-Dioxane	0.400	0.415	-3.7	96	0.00
3	n-Nitrosodimethylamine	0.400	0.364	9.0	82	0.00
4 S	2-Fluorophenol	0.400	0.406	-1.5	88	0.00
5 S	Phenol-d6	0.400	0.394	1.5	87	0.00
6	bis(2-Chloroethyl)ether	0.400	0.329	17.8	74	0.00
7 I	Naphthalene-d8	0.400	0.400	0.0	91	0.00
8 S	Nitrobenzene-d5	0.400	0.360	10.0	84	0.00
9	Naphthalene	0.400	0.386	3.5	90	-0.01
10	Hexachlorobutadiene	0.400	0.409	-2.2	92	0.00
11 SURR	2-Methylnaphthalene-d10	0.400	0.376	6.0	92	0.00
12	2-Methylnaphthalene	0.400	0.379	5.3	89	0.00
13 I	Acenaphthene-d10	0.400	0.400	0.0	92	0.00
14 S	2,4,6-Tribromophenol	0.400	0.400	0.0	90	0.00
15 S	2-Fluorobiphenyl	0.400	0.393	1.8	91	0.00
16	Acenaphthylene	0.400	0.375	6.3	91	-0.01
17	Acenaphthene	0.400	0.377	5.8	90	0.00
18	Fluorene	0.400	0.383	4.3	91	0.00
19 I	Phenanthrene-d10	0.400	0.400	0.0	93	0.00
20	4,6-Dinitro-2-methylphenol	0.400	0.270	32.5#	76	0.00
21	4-Bromophenyl-phenylether	0.400	0.373	6.8	90	0.00
22	Hexachlorobenzene	0.400	0.403	-0.8	94	0.00
23	Atrazine	0.400	0.387	3.3	94	0.00
24	Pentachlorophenol	0.400	0.347	13.3	85	0.00
25	Phenanthrene	0.400	0.375	6.3	91	0.00
26	Anthracene	0.400	0.375	6.3	93	0.00
27 SURR	Fluoranthene-d10	0.400	0.383	4.3	96	0.00
28	Fluoranthene	0.400	0.382	4.5	94	0.00
29 I	Chrysene-d12	0.400	0.400	0.0	100	0.00
30	Pyrene	0.400	0.395	1.3	97	0.00
31 S	Terphenyl-d14	0.400	0.398	0.5	98	0.00
32	Benzo(a)anthracene	0.400	0.364	9.0	98	0.00
33	Chrysene	0.400	0.413	-3.2	101	0.00
34	Bis(2-ethylhexyl)phthalate	0.400	0.419	-4.7	104	0.00
35 I	Perylene-d12	0.400	0.400	0.0	100	0.00
36	Indeno(1,2,3-cd)pyrene	0.400	0.395	1.3	105	0.00
37	Benzo(b)fluoranthene	0.400	0.373	6.8	100	0.00
38	Benzo(k)fluoranthene	0.400	0.396	1.0	102	0.00
39 C	Benzo(a)pyrene	0.400	0.400	0.0	106	0.00
40	Dibenzo(a,h)anthracene	0.400	0.383	4.3	102	0.00
41	Benzo(g,h,i)perylene	0.400	0.390	2.5	102	0.00

(#) = Out of Range

SPCC's out = 0 CCC's out = 0



# QC SAMPLE


# DATA

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037351.D  
 Acq On : 20 Jun 2025 15:00  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jun 20 23:41:54 2025

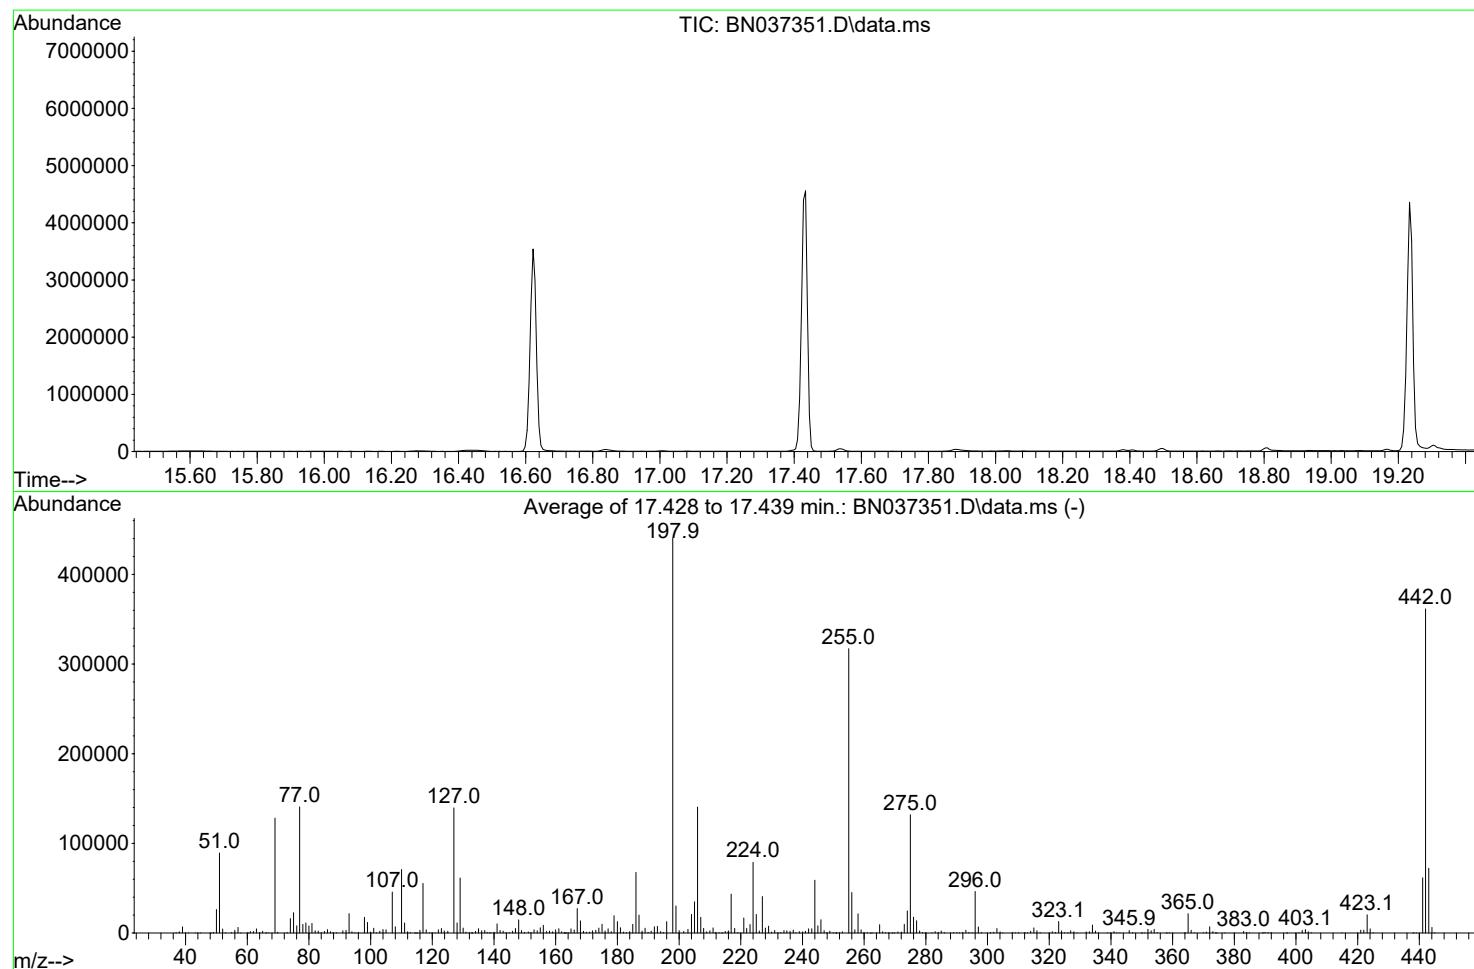




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	128141	PASS
70	69	0.00	2	0.7	882	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	440469	PASS
199	198	5	9	6.8	30163	PASS
365	198	1	100	4.9	21610	PASS
441	443	0.01	150	85.2	61520	PASS
442	442	100	100	100.0	361557	PASS
443	442	15	24	20.0	72213	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037351.D  
 Acq On : 20 Jun 2025 15:00  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 21 02:21:15 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Jun 21 02:21:08 2025  
 Response via : Initial Calibration

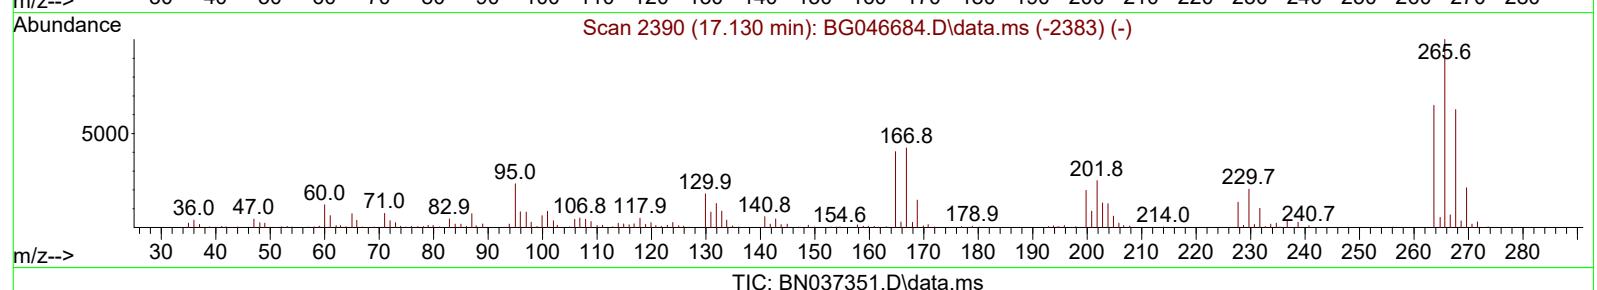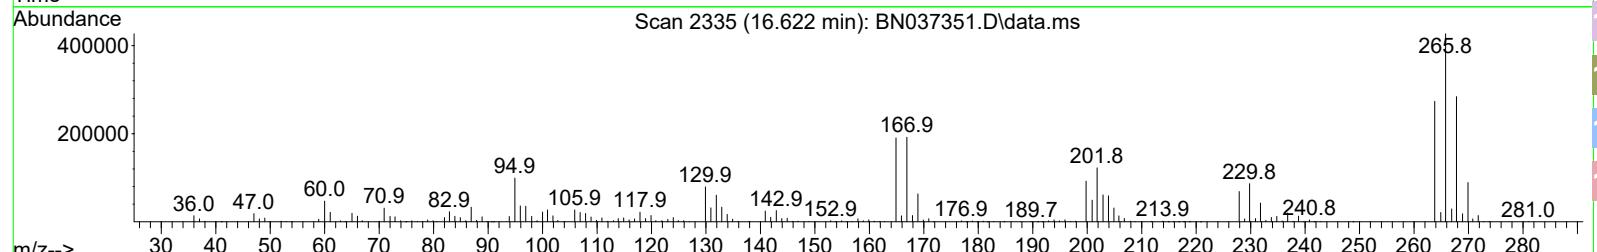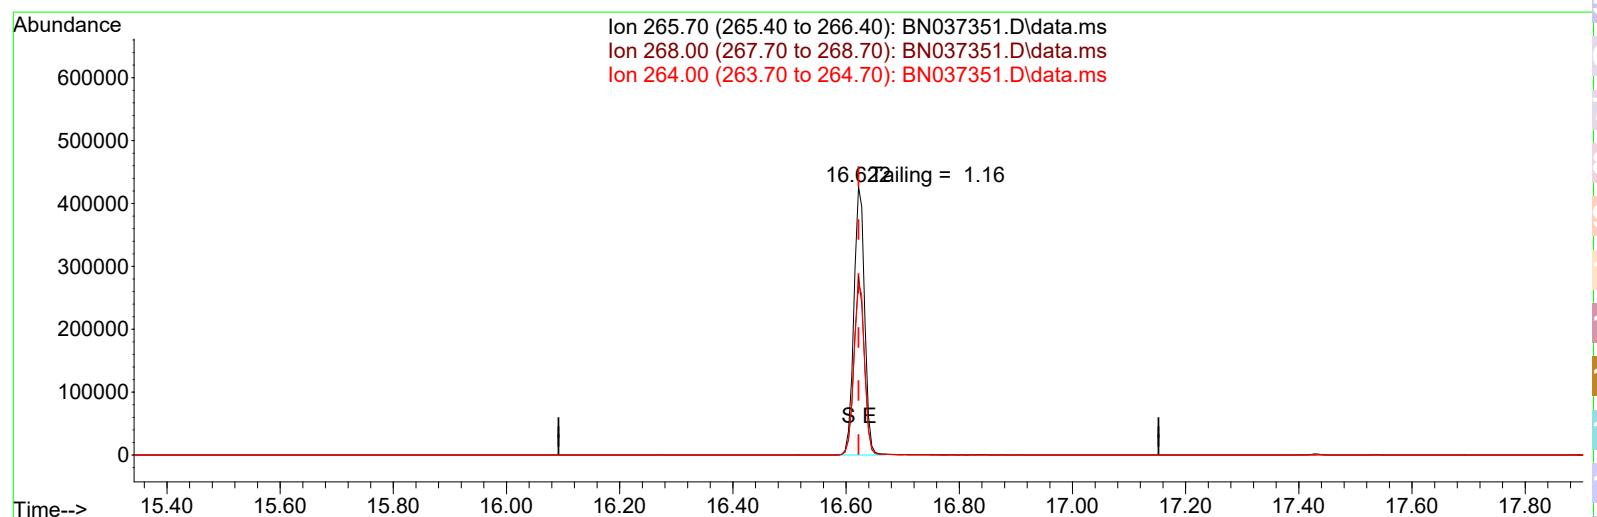

TIC: BN037351.D\data.ms

(70) Pentachlorophenol (C)  
 16.622min ( 0.000) 21508.69 ng


response 561749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.53
264.00	61.60	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037351.D  
 Acq On : 20 Jun 2025 15:00  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 21 02:21:15 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Jun 21 02:21:08 2025  
 Response via : Initial Calibration

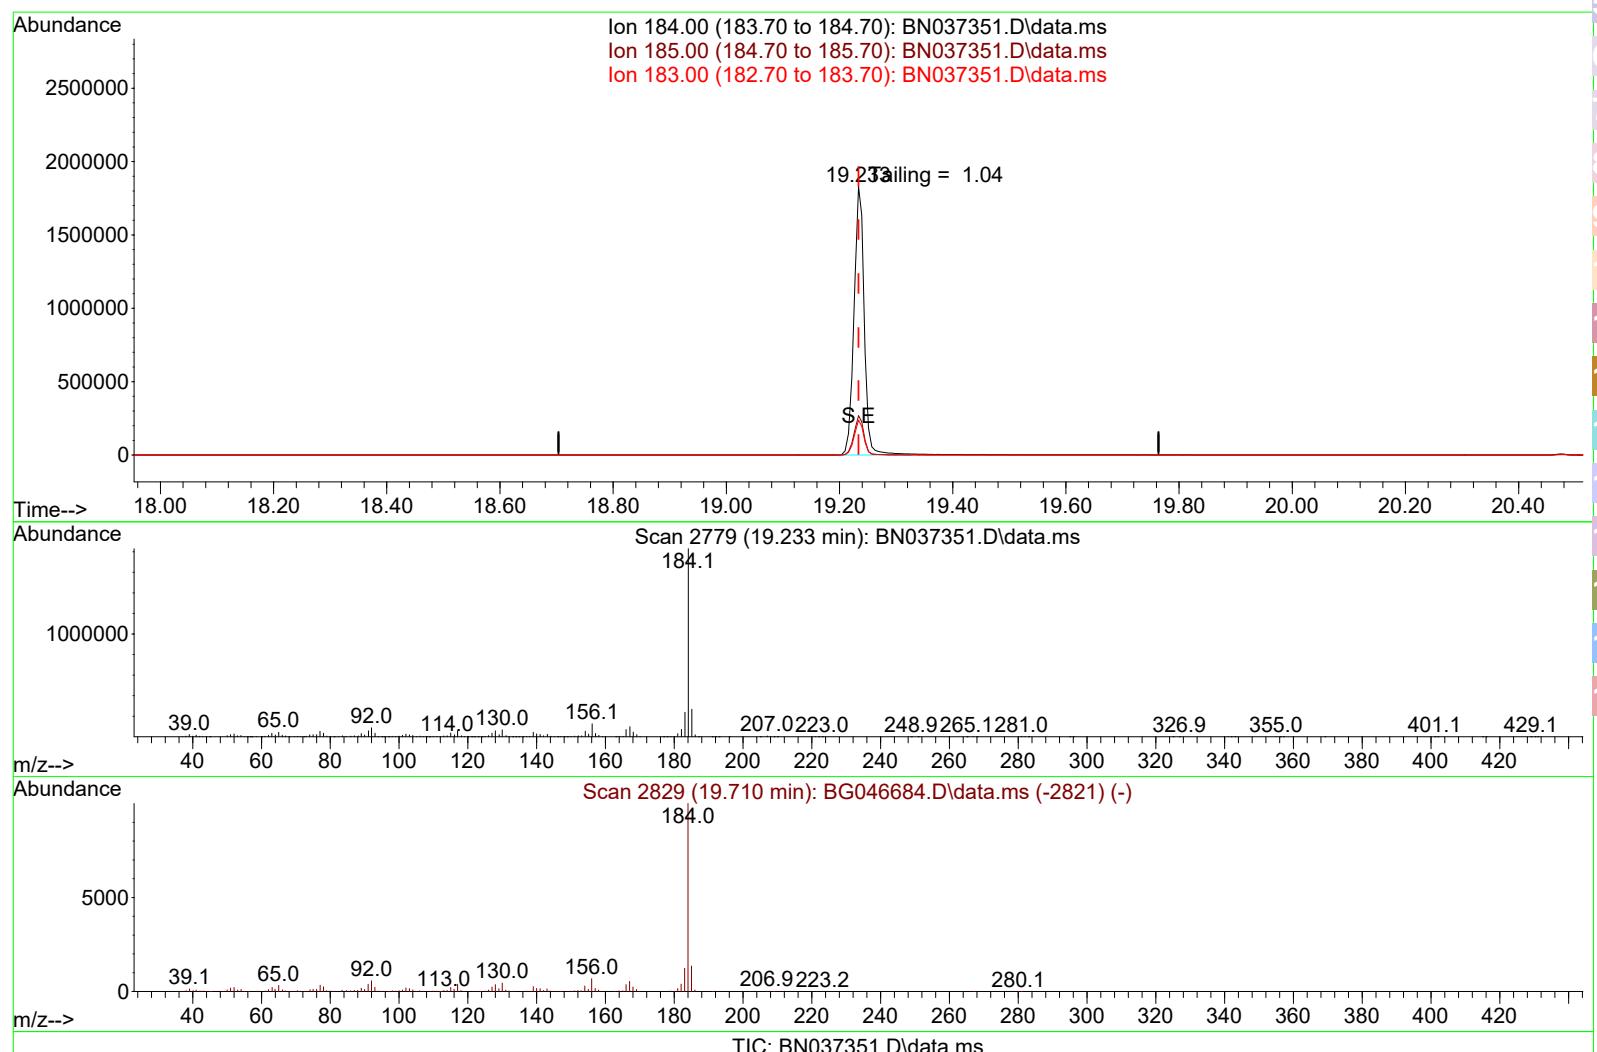

## (77) Benzidine

19.233min ( 0.000) 0.00 ng

response 2309913

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	13.00
0.00	0.00	0.00

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

### DDT Breakdown


Date	Instrument Name	DFTPP Data File
6/21/2025	BNA_N	BN037351.D
Compound Name	Response	Retention Time
DDT	1600198	20.475
DDD	22591	20.257
DDE	1214	19.522
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23805	1624003	1.47

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037385.D  
 Acq On : 26 Jun 2025 10:01  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jun 26 16:06:33 2025

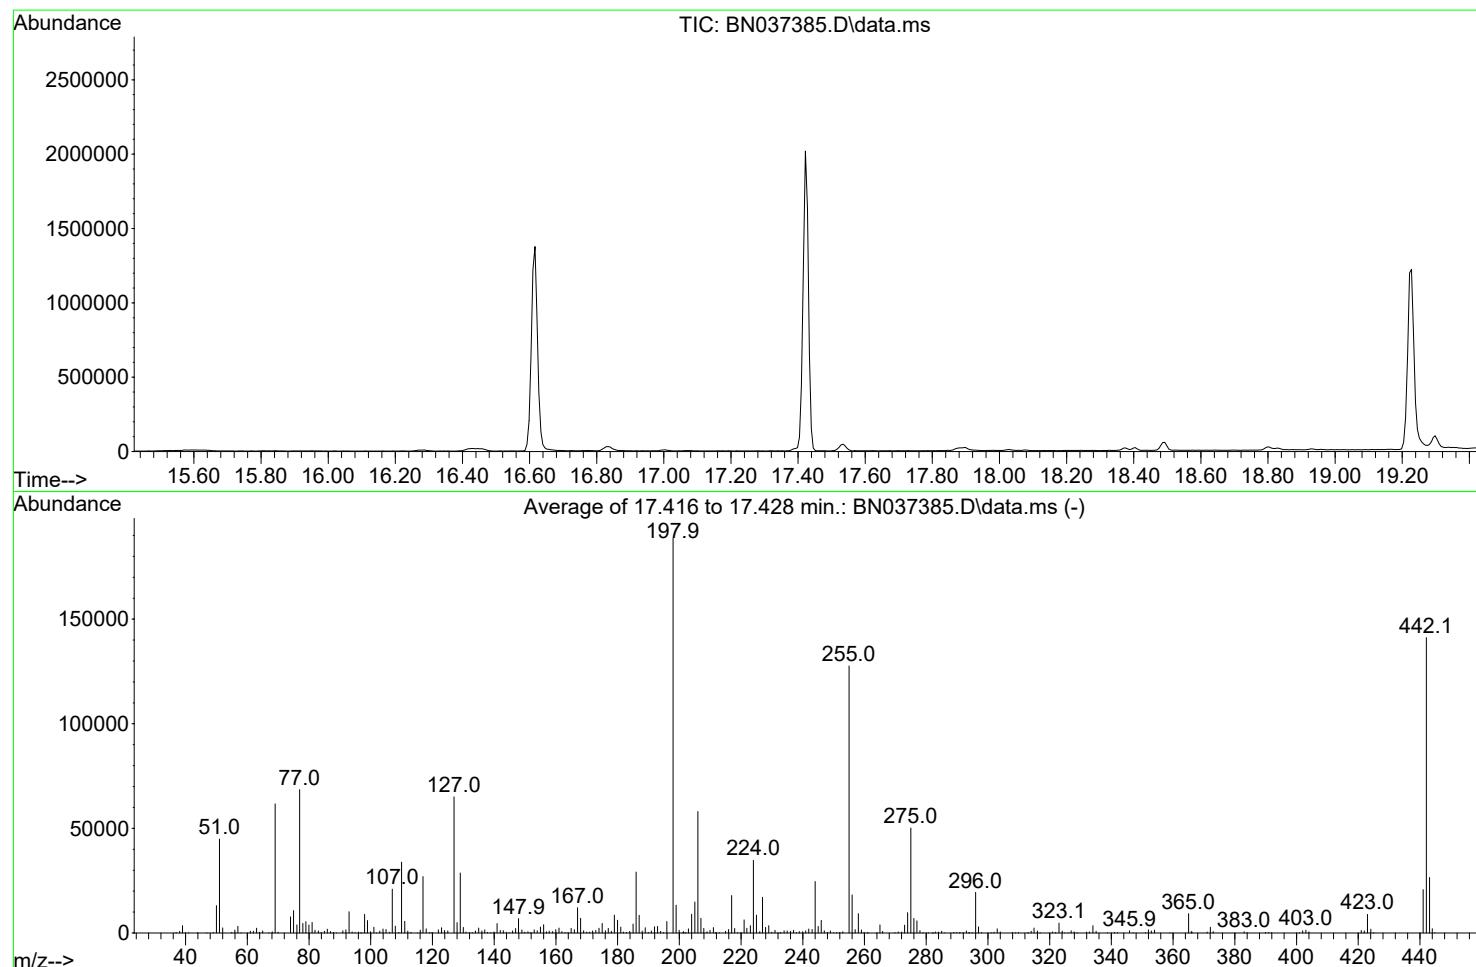




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.9	565	PASS
69	69	100	100	100.0	61709	PASS
70	69	0.00	2	0.6	395	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	188693	PASS
199	198	5	9	7.1	13336	PASS
365	198	1	100	4.9	9289	PASS
441	443	0.01	150	78.0	20689	PASS
442	442	100	100	100.0	141205	PASS
443	442	15	24	18.8	26534	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037385.D  
 Acq On : 26 Jun 2025 10:01  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 26 17:27:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Jun 21 02:21:08 2025  
 Response via : Initial Calibration

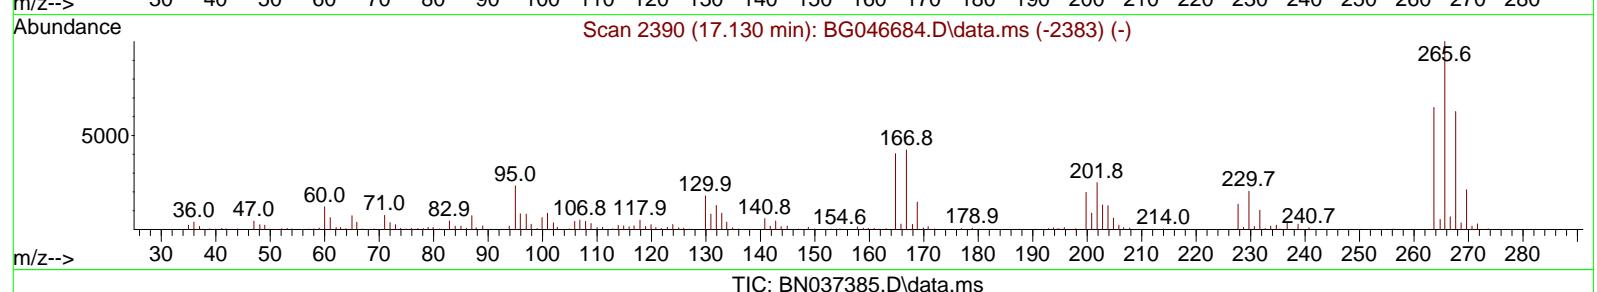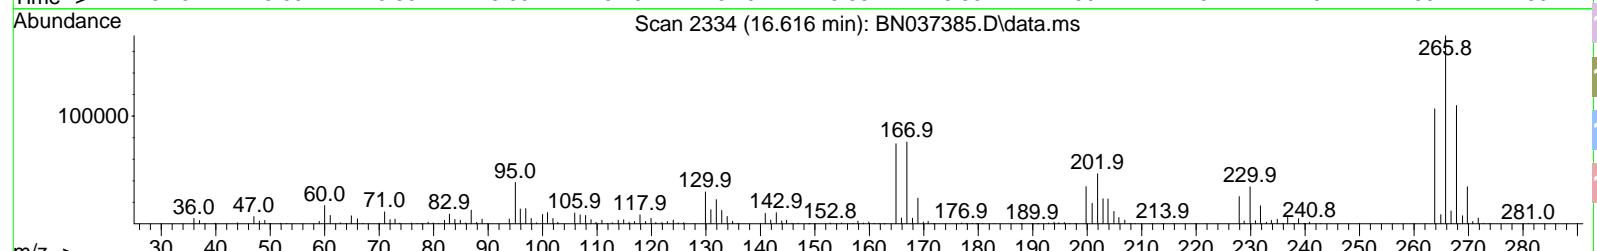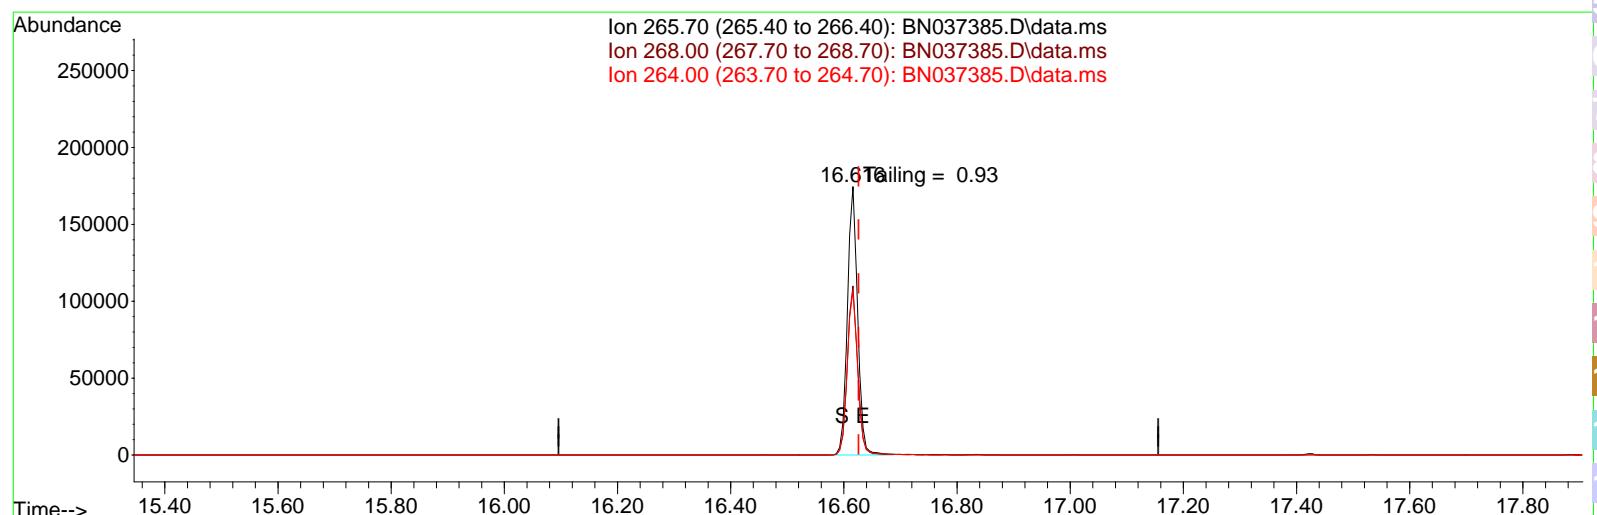

TIC: BN037385.D\data.ms

(70) Pentachlorophenol (C)  
 16.616min (-0.010) 22827.65 ng




response 218916

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.95
264.00	61.60	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037385.D  
 Acq On : 26 Jun 2025 10:01  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 26 17:27:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat Jun 21 02:21:08 2025  
 Response via : Initial Calibration

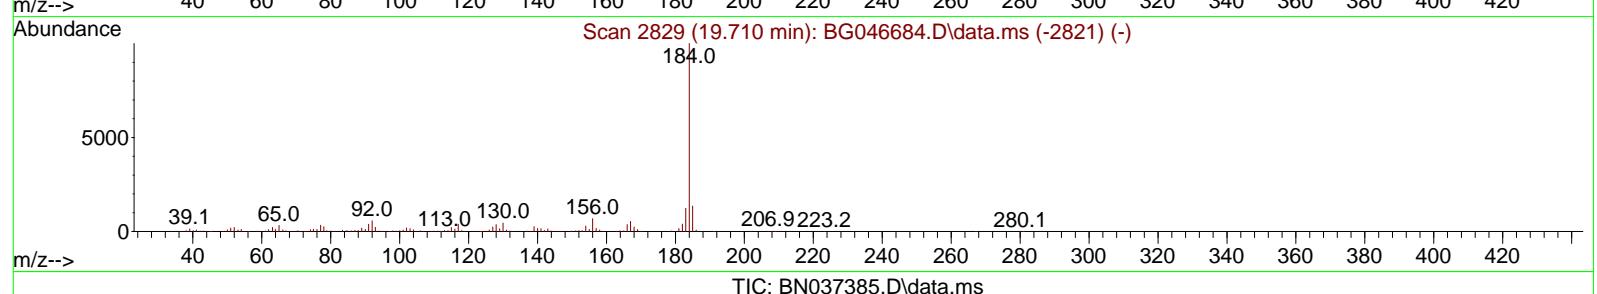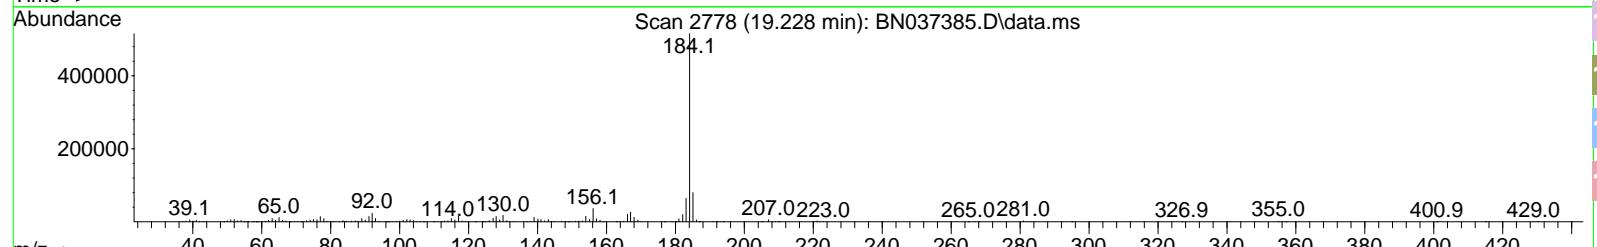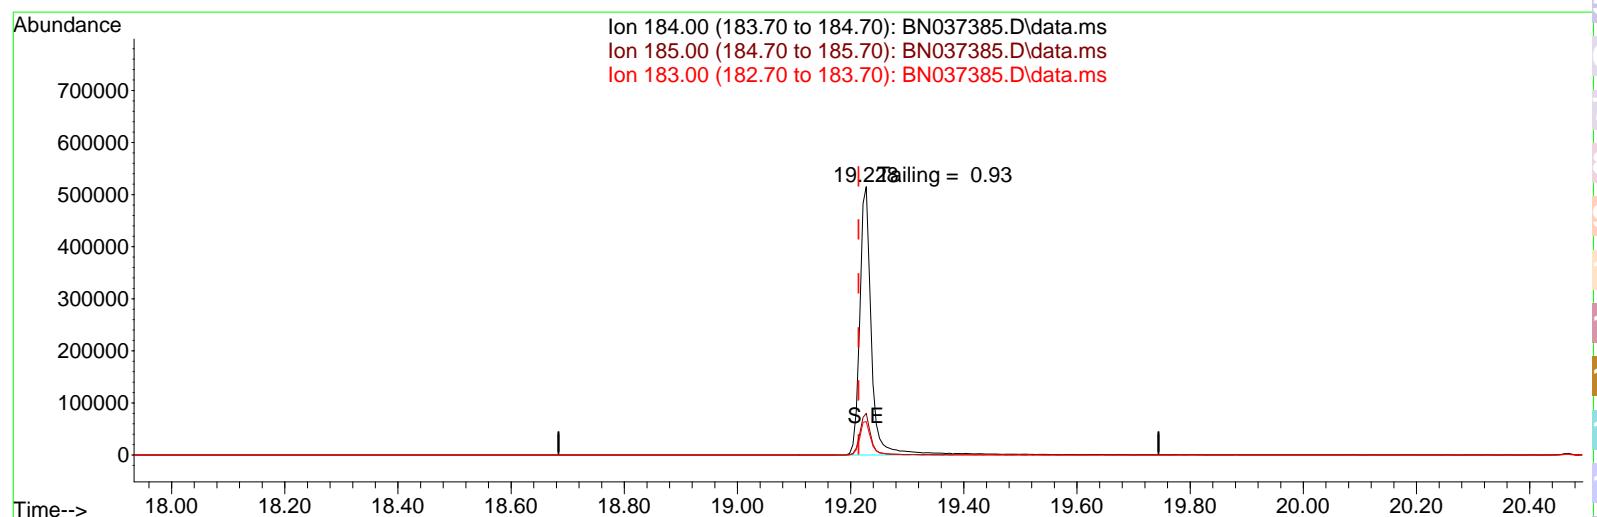

TIC: BN037385.D\data.ms

(77) Benzidine

19.228min (+ 0.014) 0.00 ng

response 733495

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.54
183.00	13.20	12.50
0.00	0.00	0.00

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

DDT Breakdown


Date	Instrument Name	DFTPP Data File
6/26/2025	BNA_N	BN037385.D
Compound Name	Response	Retention Time
DDT	575237	20.469
DDD	9375	20.028
DDE	1379	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10754	585991	1.84

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037402.D  
 Acq On : 26 Jun 2025 20:19  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jun 26 16:06:33 2025

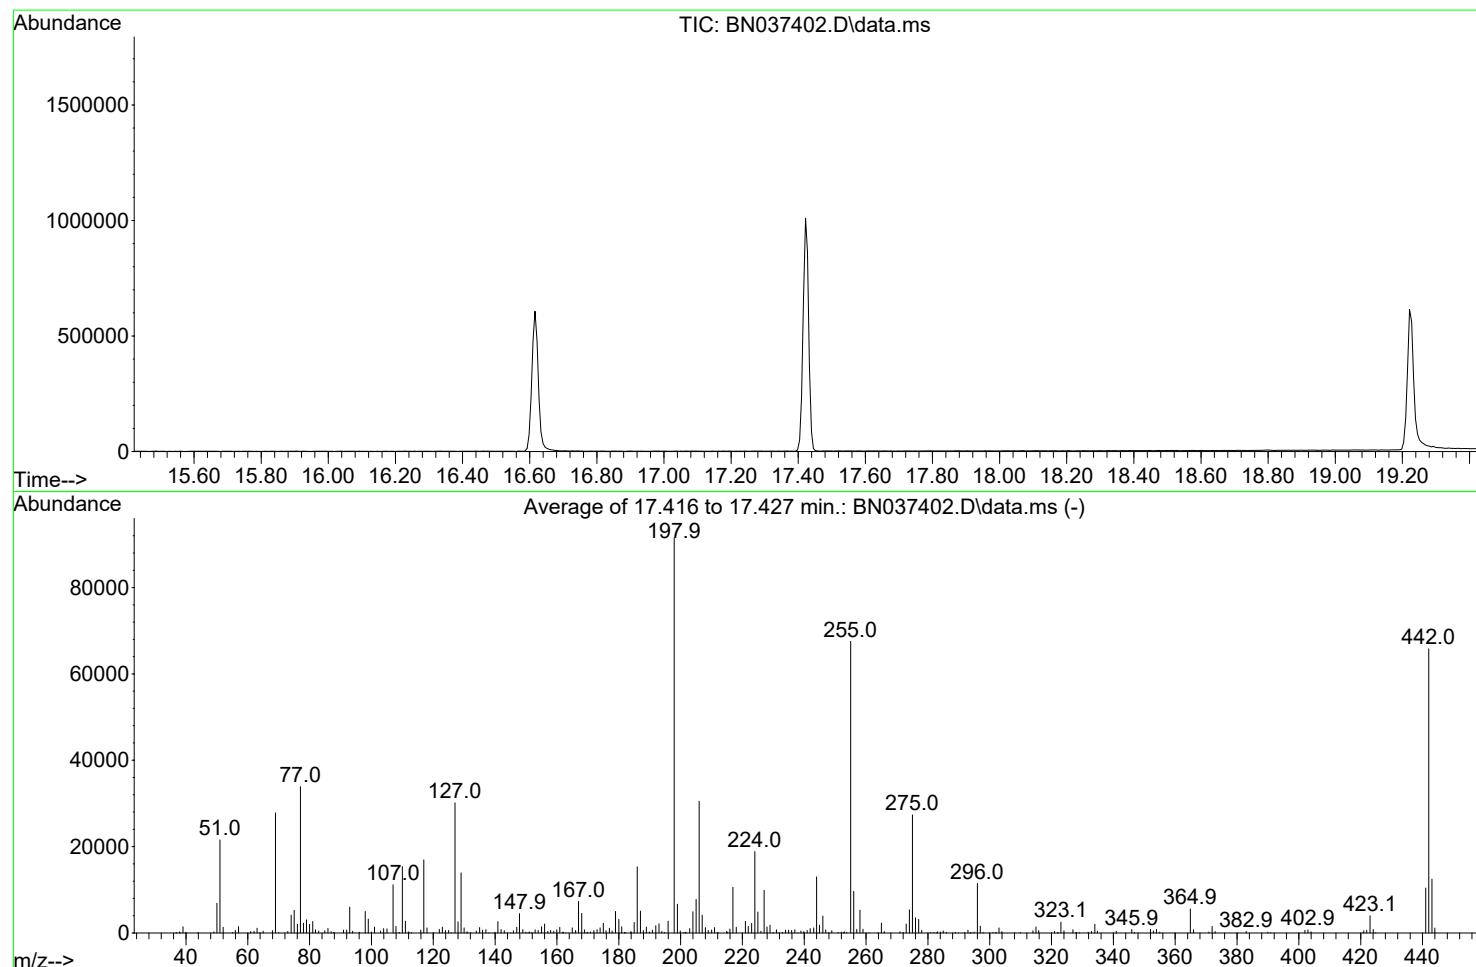




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	567	PASS
69	69	100	100	100.0	27835	PASS
70	69	0.00	2	0.5	131	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91421	PASS
199	198	5	9	7.3	6679	PASS
365	198	1	100	6.1	5585	PASS
441	443	0.01	150	83.2	10396	PASS
442	442	100	100	100.0	65797	PASS
443	442	15	24	19.0	12501	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037402.D  
 Acq On : 26 Jun 2025 20:19  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 27 04:09:41 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 27 04:09:23 2025  
 Response via : Initial Calibration

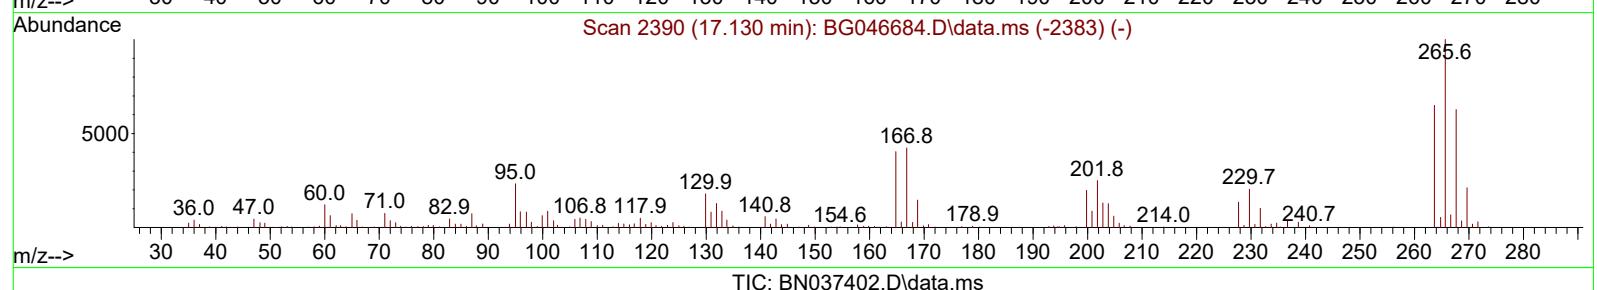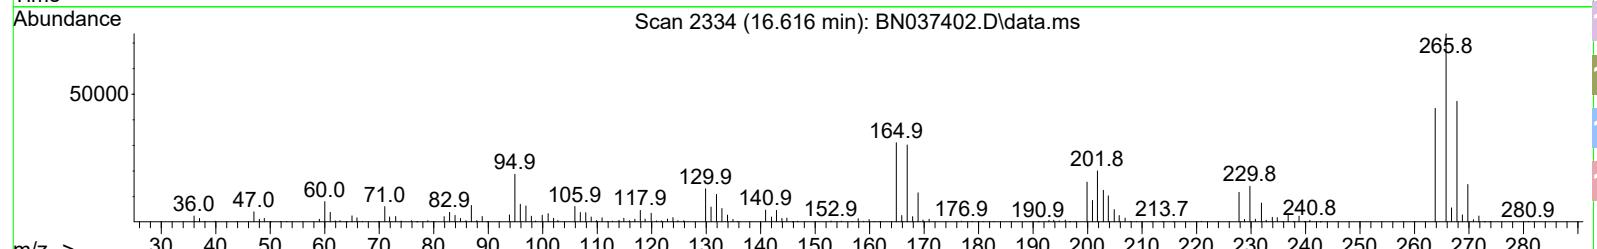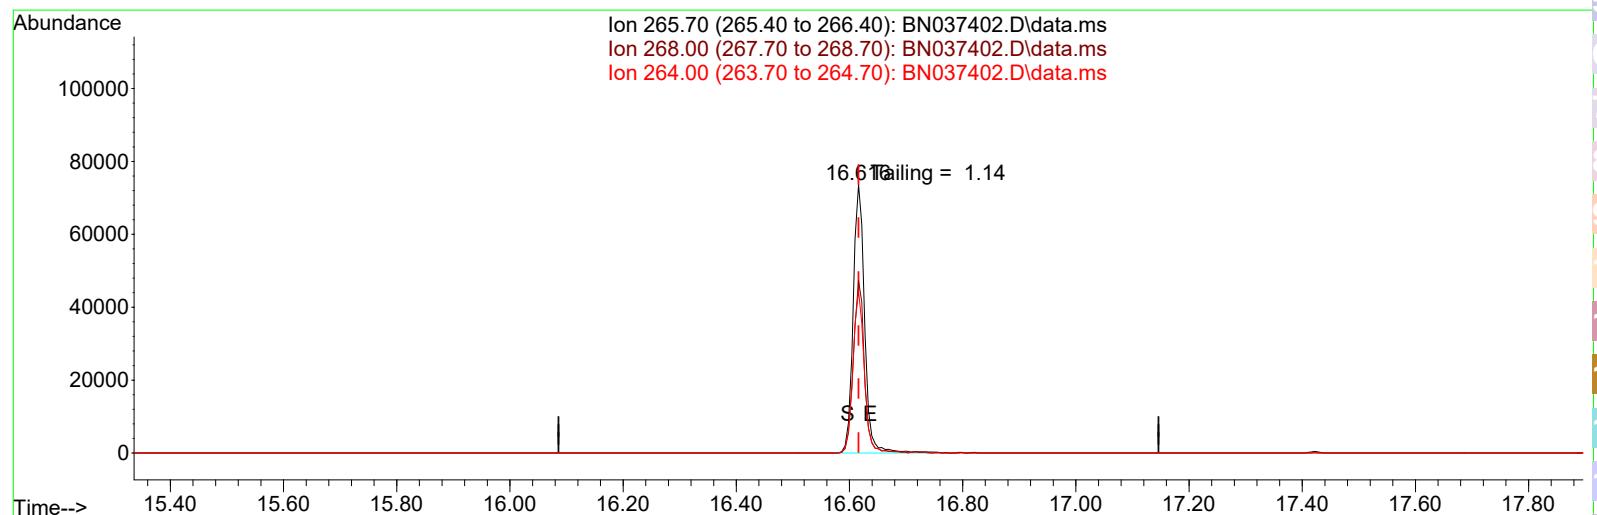

TIC: BN037402.D\data.ms

(70) Pentachlorophenol (C)

16.616min ( 0.000) 18260.25 ng




response 103034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.20
264.00	61.60	60.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037402.D  
 Acq On : 26 Jun 2025 20:19  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jun 27 04:09:41 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 27 04:09:23 2025  
 Response via : Initial Calibration

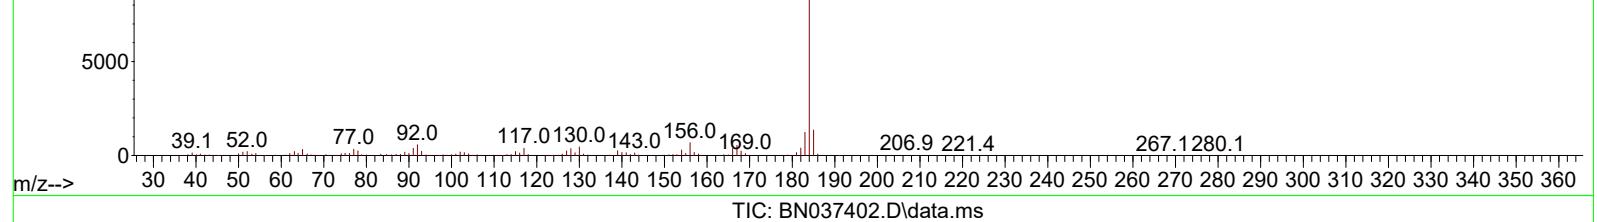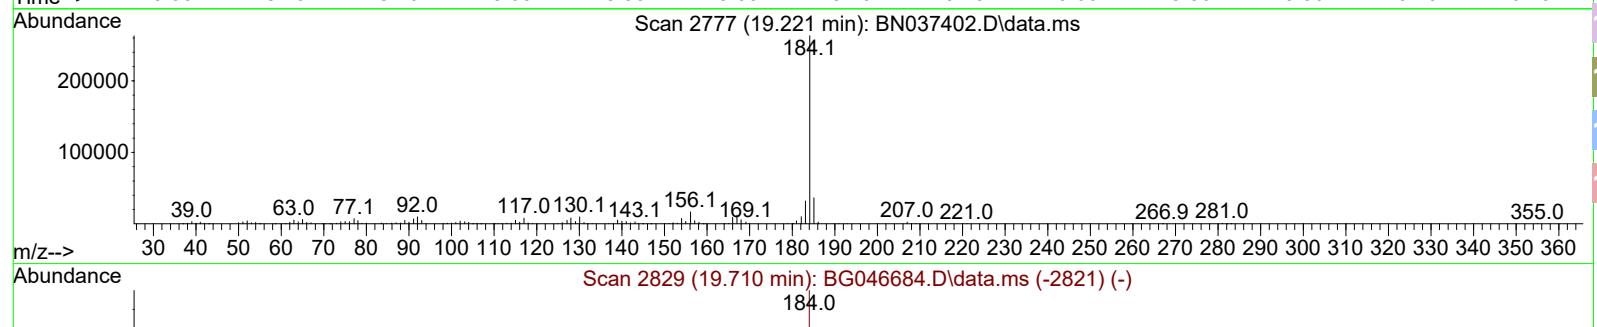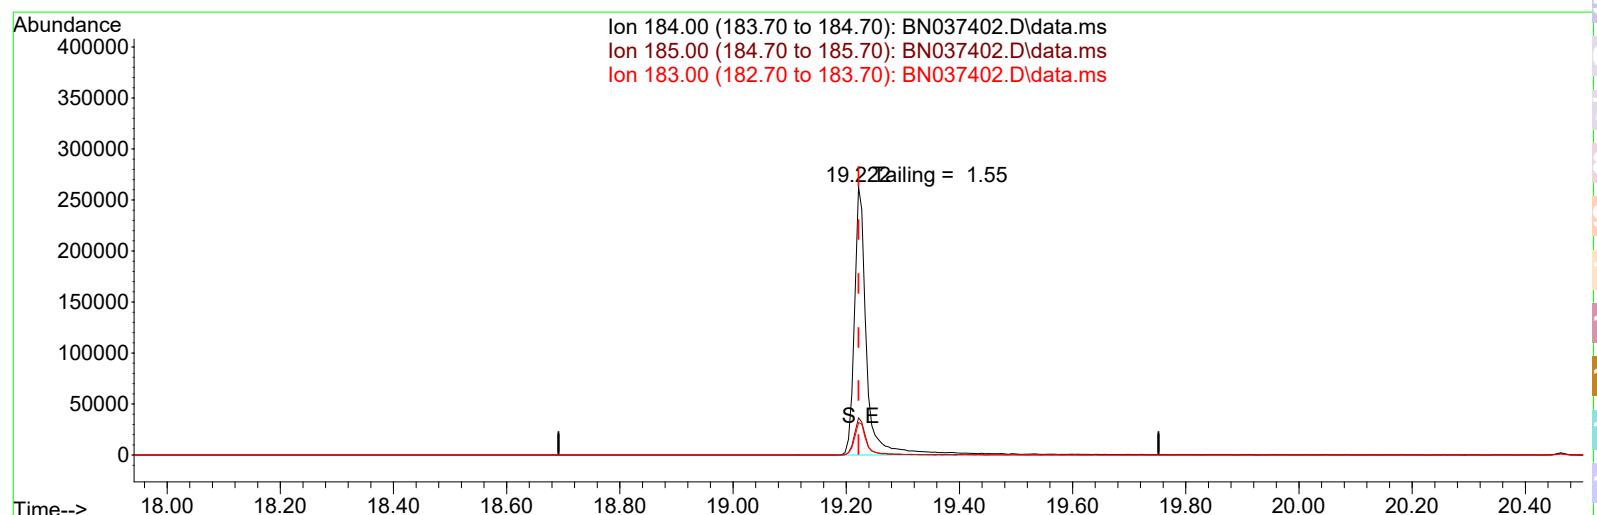

TIC: BN037402.D\data.ms

(77) Benzidine

19.221min ( 0.000) 0.00 ng

response 385080

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.50	13.89
--------	-------	-------

183.00	13.20	12.12
--------	-------	-------

0.00	0.00	0.00
------	------	------

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/26/2025	BNA_N	BN037402.D
Compound Name	Response	Retention Time
DDT	341583	20.463
DDD	4324	20.074
DDE	90	19.516
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4414	345997	1.28



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Tetra Tech NUS, Inc.			Date Collected:	
Project:	NWIRP Bethpage 112G08005-WE13			Date Received:	
Client Sample ID:	PB168563BL			SDG No.:	Q2375
Lab Sample ID:	PB168563BL			Matrix:	Water
Analytical Method:	SW8270ESIM			% Solid:	0
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	1000 uL
Soil Aliquot Vol:			uL	Test:	SVOC-SIMGroup1
Extraction Type :		Decanted :	N	Level :	LOW
Injection Volume :		GPC Factor :	1.0	GPC Cleanup :	N PH :
Prep Method :					

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN037361.D	1	06/20/25 12:03	06/20/25 22:16	PB168563

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
123-91-1	1,4-Dioxane	0.20	U	0.070	0.20	0.20	ug/L
<b>SURROGATES</b>							
7297-45-2	2-Methylnaphthalene-d10	0.32		30 - 150		81%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.37		30 - 150		93%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.30		55 - 111		75%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.33		53 - 106		81%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.37		58 - 132		93%	SPK: 0.4
<b>INTERNAL STANDARDS</b>							
3855-82-1	1,4-Dichlorobenzene-d4	1970		7.568			
1146-65-2	Naphthalene-d8	4050		10.351			
15067-26-2	Acenaphthene-d10	2740		14.224			
1517-22-2	Phenanthrene-d10	4860		16.984			
1719-03-5	Chrysene-d12	4290		21.171			
1520-96-3	Perylene-d12	3460		23.357			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037361.D  
 Acq On : 20 Jun 2025 22:16  
 Operator : RC/JU  
 Sample : PB168563BL  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BL

Quant Time: Jun 20 23:51:33 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1968	0.400	ng	0.00
7) Naphthalene-d8	10.351	136	4045	0.400	ng	0.01
13) Acenaphthene-d10	14.224	164	2736	0.400	ng	0.01
19) Phenanthrene-d10	16.984	188	4864	0.400	ng	0.01
29) Chrysene-d12	21.171	240	4288	0.400	ng	# 0.00
35) Perylene-d12	23.357	264	3457	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.170	112	1419	0.361	ng	0.00
5) Phenol-d6	6.759	99	1185	0.293	ng	0.00
8) Nitrobenzene-d5	8.739	82	978	0.299	ng	0.02
11) 2-Methylnaphthalene-d10	11.960	152	2116	0.323	ng	0.02
14) 2,4,6-Tribromophenol	15.742	330	469	0.292	ng	0.02
15) 2-Fluorobiphenyl	12.853	172	3920	0.326	ng	0.02
27) Fluoranthene-d10	19.012	212	5207	0.373	ng	0.00
31) Terphenyl-d14	19.621	244	3648	0.373	ng	0.00




Target Compounds	Qvalue
(#= qualifier out of range (m) = manual integration (+) = signals summed	

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037361.D  
 Acq On : 20 Jun 2025 22:16  
 Operator : RC/JU  
 Sample : PB168563BL  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BL




Quant Time: Jun 20 23:51:33 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

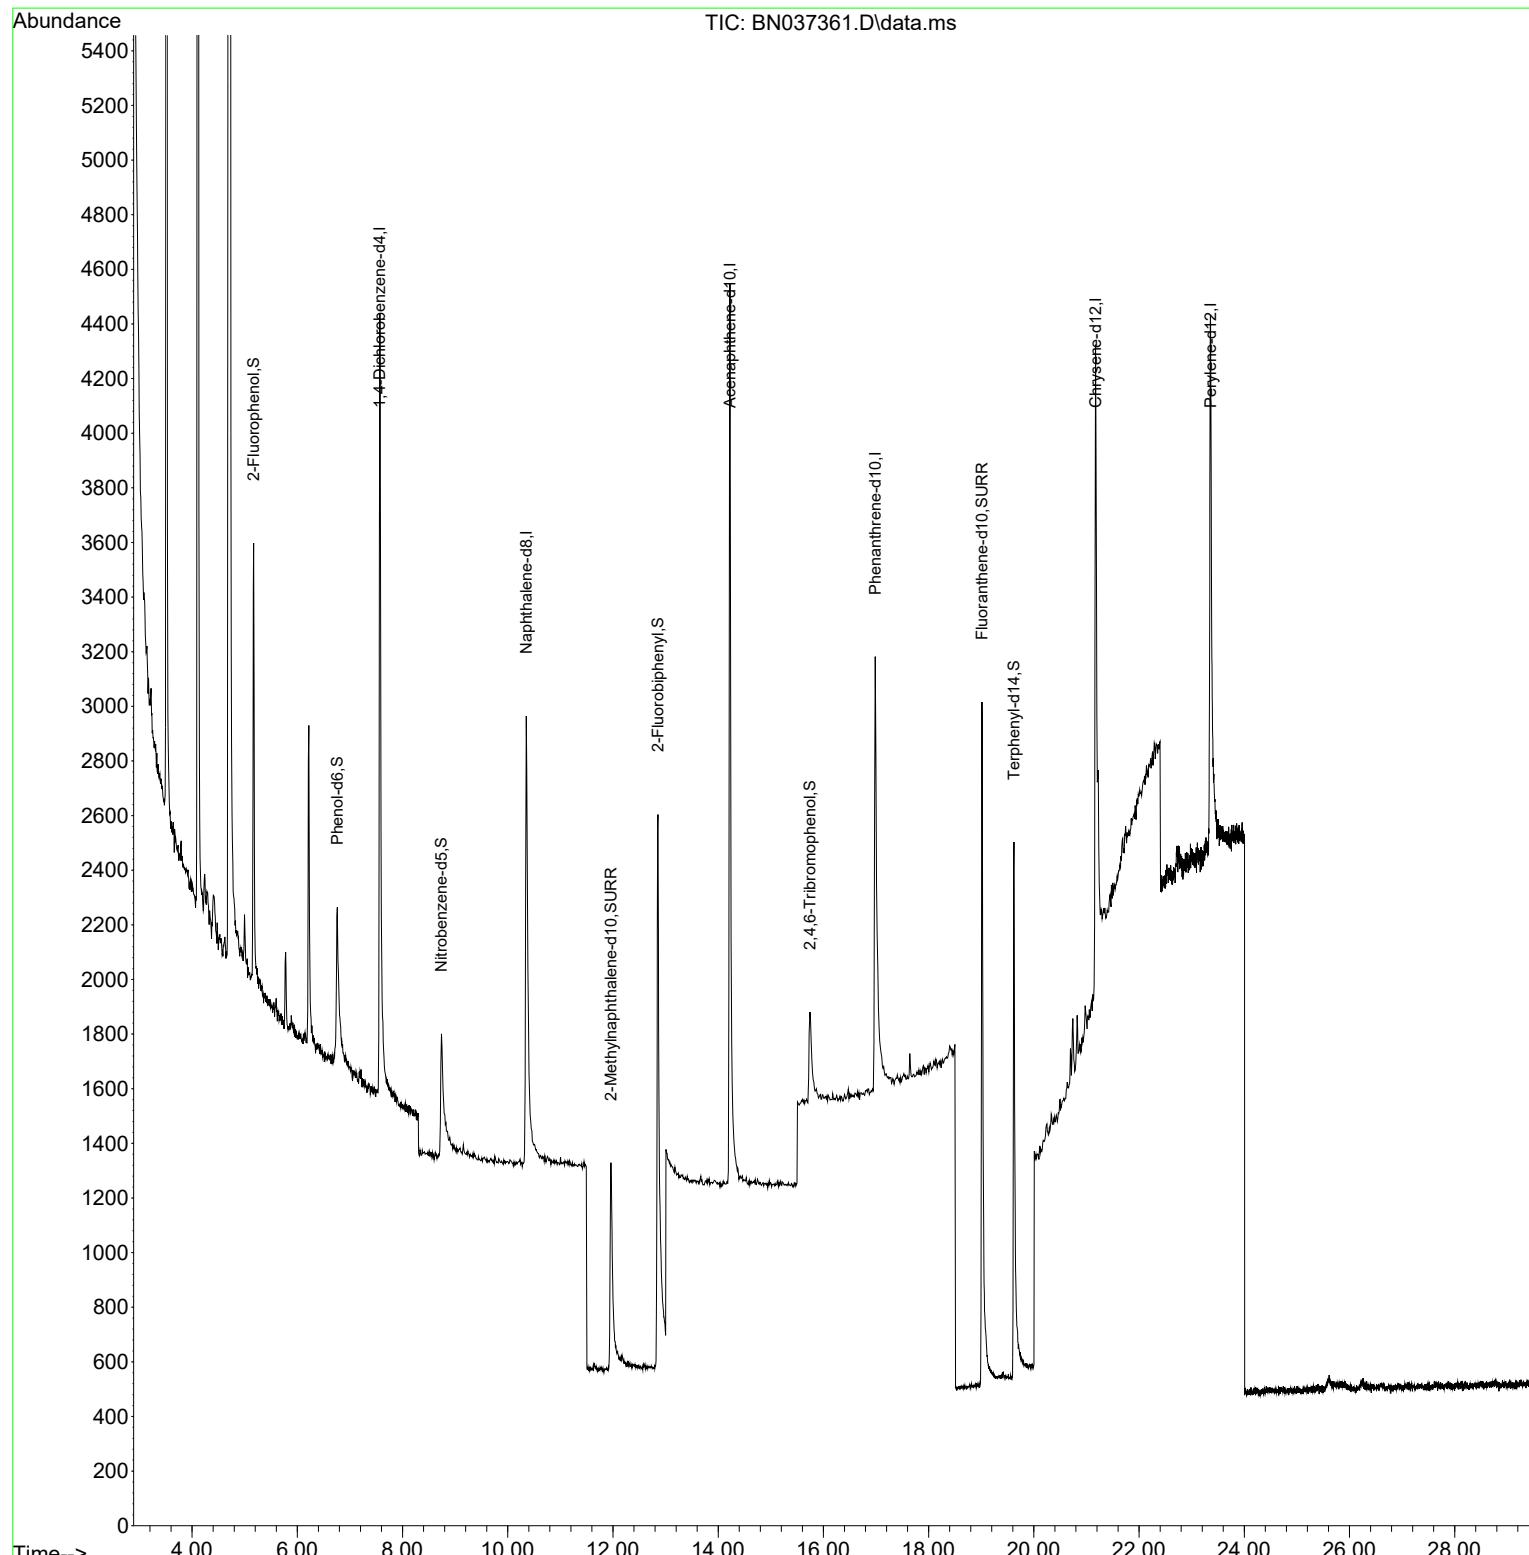





#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037361.D  
ClientSampleId : PB168563BL  
Acq: 20 Jun 2025 22:16




Tgt Ion:152 Resp: 1968  
Ion Ratio Lower Upper  
152 100  
150 146.8 112.7 169.1  
115 58.6 45.9 68.9



#4  
2-Fluorophenol  
Concen: 0.361 ng  
RT: 5.170 min Scan# 317  
Delta R.T. 0.007 min  
Lab File: BN037361.D  
Acq: 20 Jun 2025 22:16

Tgt Ion:112 Resp: 1419  
Ion Ratio Lower Upper  
112 100  
64 50.4 38.7 58.1  
63 30.7 26.4 39.6






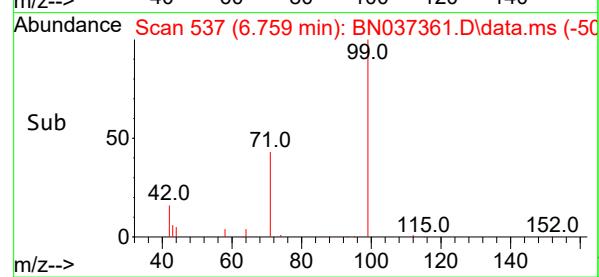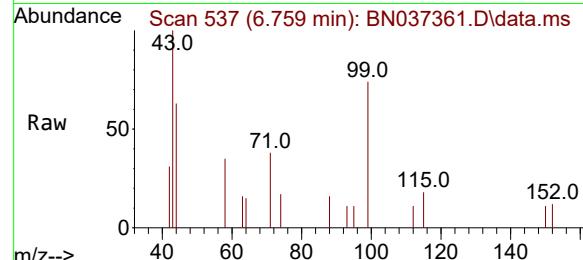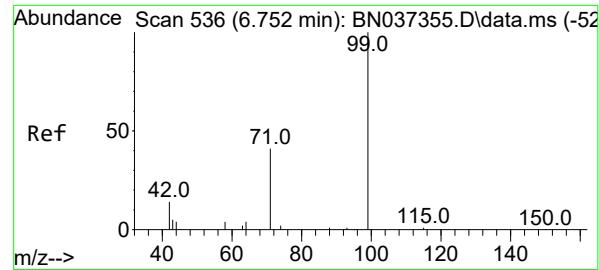

#5  
 Phenol-d6  
 Concen: 0.293 ng  
 RT: 6.759 min Scan# 5  
 Delta R.T. 0.007 min  
 Lab File: BN037361.D  
 Acq: 20 Jun 2025 22:16



Instrument : BNA\_N  
 ClientSampleId : PB168563BL




Tgt Ion: 99 Resp: 1185  
 Ion Ratio Lower Upper  
 99 100  
 42 19.7 19.8 29.8#  
 71 40.8 42.6 64.0#

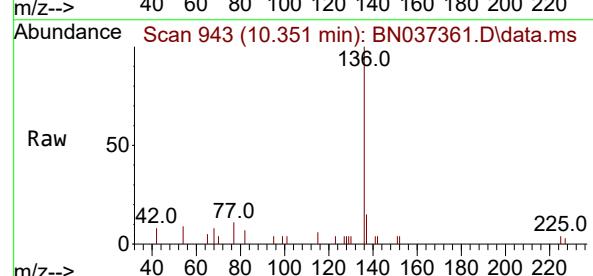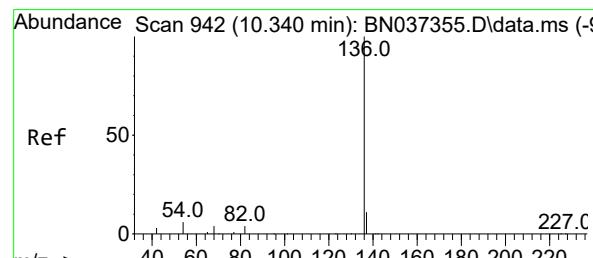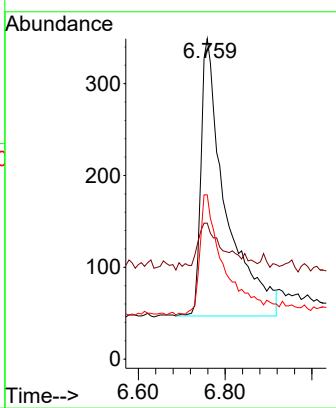

#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.351 min Scan# 943  
 Delta R.T. 0.010 min  
 Lab File: BN037361.D  
 Acq: 20 Jun 2025 22:16

Tgt Ion:136 Resp: 4045  
 Ion Ratio Lower Upper  
 136 100  
 137 14.9 12.2 18.2  
 54 9.0 8.8 13.2  
 68 8.0 7.0 10.4

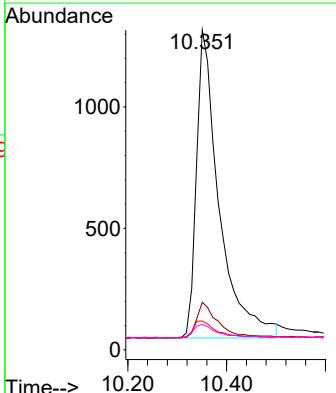

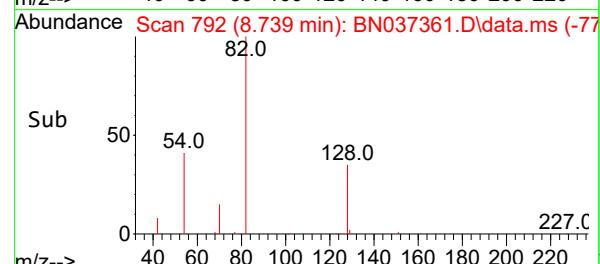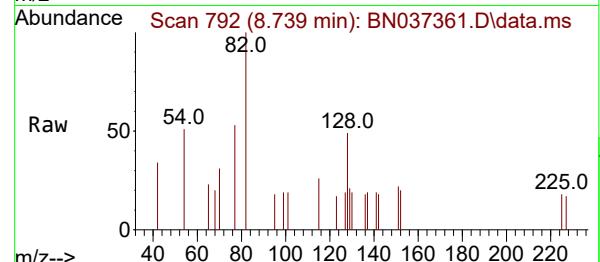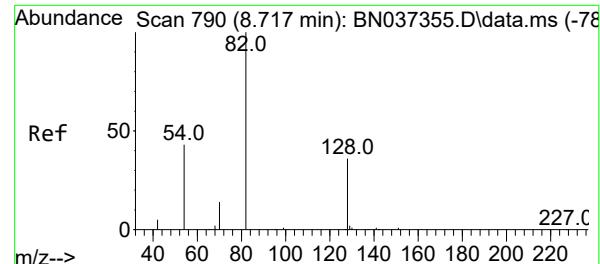

#8

Nitrobenzene-d5

Concen: 0.299 ng

RT: 8.739 min Scan# 7

Delta R.T. 0.021 min

Lab File: BN037361.D

Acq: 20 Jun 2025 22:16

Instrument :

BNA\_N

ClientSampleId :

PB168563BL





Tgt Ion: 82 Resp: 978

Ion Ratio Lower Upper

82 100

128 48.5 42.5 63.7

54 50.7 43.2 64.8

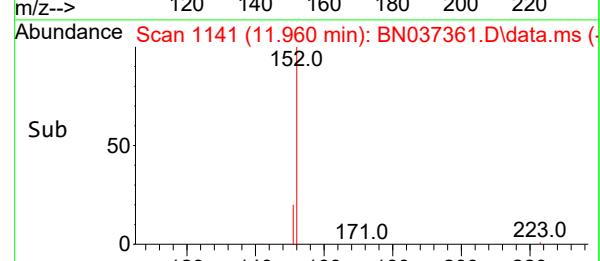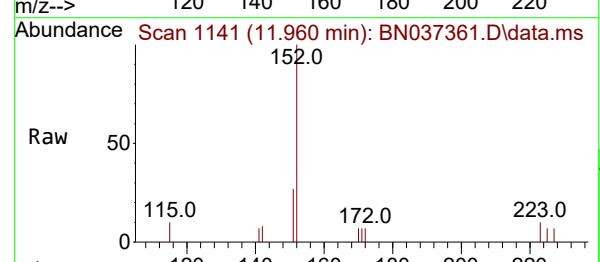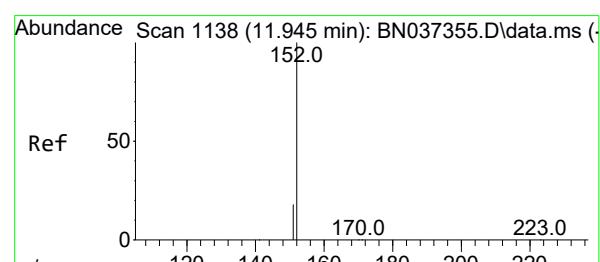

#11

2-Methylnaphthalene-d10

Concen: 0.323 ng

RT: 11.960 min Scan# 1141

Delta R.T. 0.015 min

Lab File: BN037361.D


Acq: 20 Jun 2025 22:16




Tgt Ion:152 Resp: 2116

Ion Ratio Lower Upper

152 100

151 23.0 17.4 26.0





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.224 min Scan# 1

Delta R.T. 0.011 min

Lab File: BN037361.D

Acq: 20 Jun 2025 22:16

Instrument :

BNA\_N

ClientSampleId :

PB168563BL





Tgt Ion:164 Resp: 2736

Ion Ratio Lower Upper

164 100

162 102.7 81.5 122.3

160 52.5 43.0 64.4



#14

2,4,6-Tribromophenol

Concen: 0.292 ng

RT: 15.742 min Scan# 1600

Delta R.T. 0.025 min

Lab File: BN037361.D

Acq: 20 Jun 2025 22:16


Tgt Ion:330 Resp: 469


Ion Ratio Lower Upper

330 100

332 95.1 78.4 117.6

141 31.3 24.4 36.6





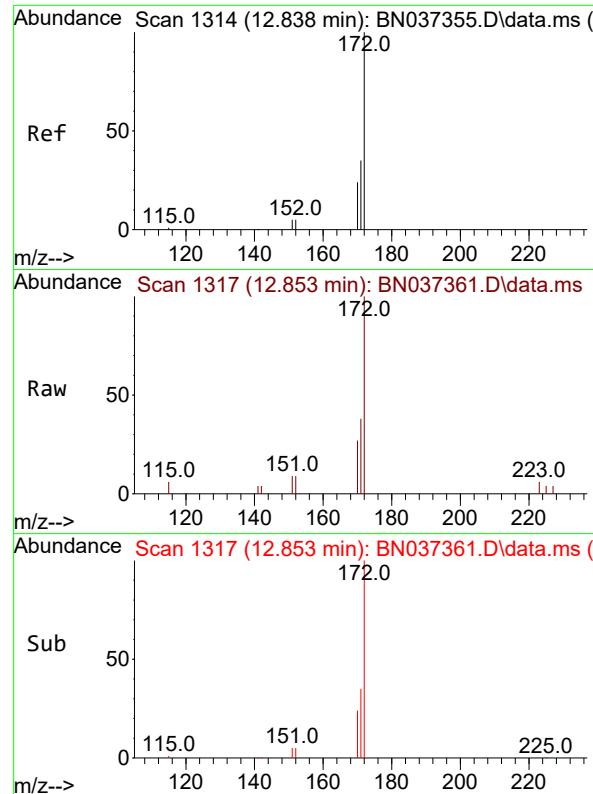

#15  
2-Fluorobiphenyl  
Concen: 0.326 ng  
RT: 12.853 min Scan# 1  
Delta R.T. 0.015 min  
Lab File: BN037361.D  
Acq: 20 Jun 2025 22:16


Instrument : BNA\_N  
ClientSampleId : PB168563BL


Tgt Ion:172 Resp: 3920  
Ion Ratio Lower Upper  
172 100  
171 37.8 30.8 46.2  
170 26.6 21.9 32.9

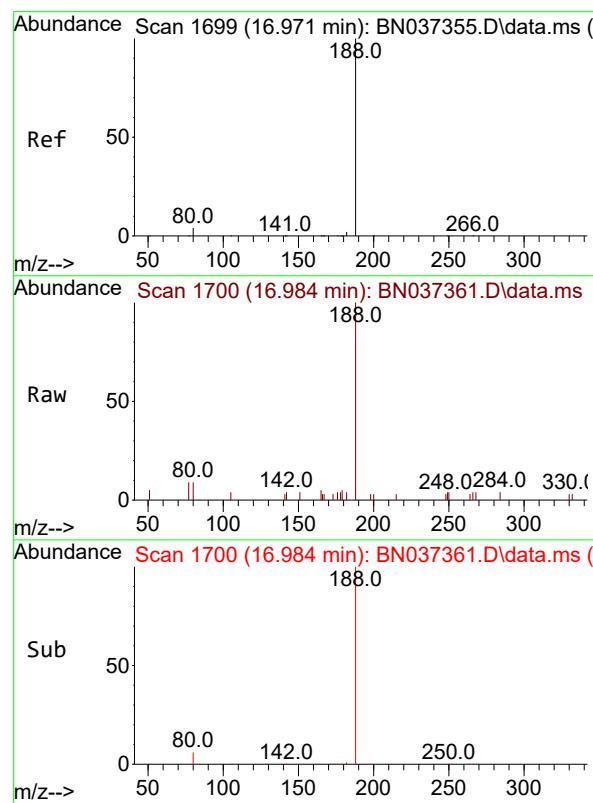

#19  
Phenanthrene-d10  
Concen: 0.400 ng  
RT: 16.984 min Scan# 1700  
Delta R.T. 0.012 min  
Lab File: BN037361.D  
Acq: 20 Jun 2025 22:16

Tgt Ion:188 Resp: 4864  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 8.9 6.2 9.2





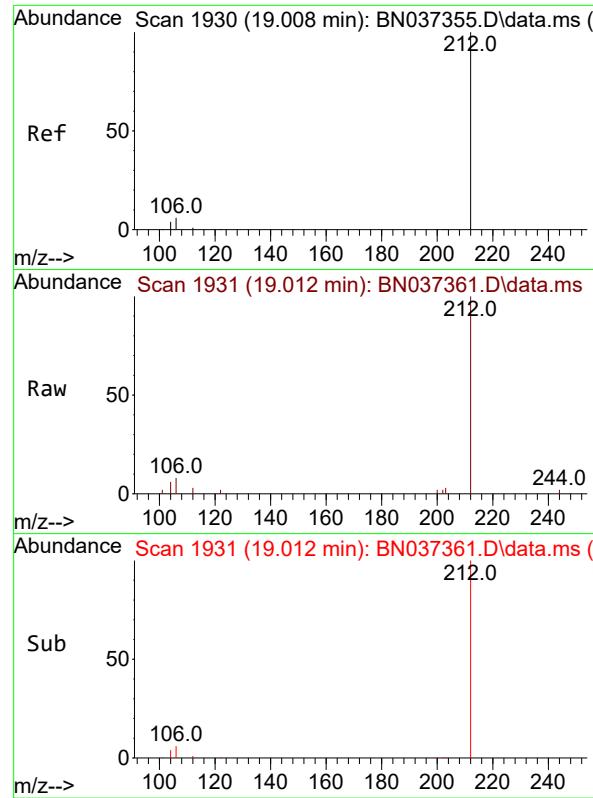

#27  
Fluoranthene-d10  
Concen: 0.373 ng  
RT: 19.012 min Scan# 1  
Delta R.T. 0.004 min  
Lab File: BN037361.D  
Acq: 20 Jun 2025 22:16


Instrument : BNA\_N  
ClientSampleId : PB168563BL


Tgt Ion:212 Resp: 5207  
Ion Ratio Lower Upper  
212 100  
106 5.8 3.0 4.4#  
104 3.4 2.0 3.0#

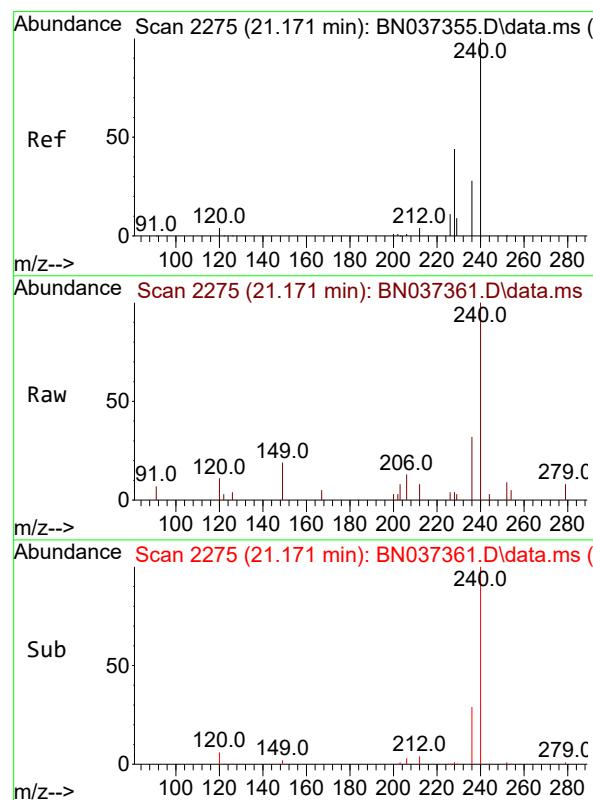

#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.171 min Scan# 2275  
Delta R.T. -0.000 min  
Lab File: BN037361.D  
Acq: 20 Jun 2025 22:16



Tgt Ion:240 Resp: 4288  
Ion Ratio Lower Upper  
240 100  
120 11.3 7.5 11.3#  
236 32.4 24.9 37.3



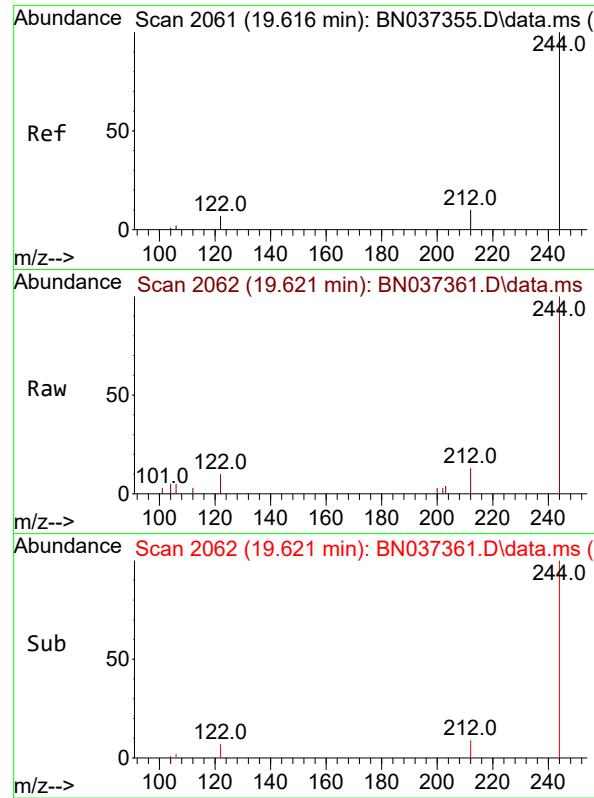


#31  
Terphenyl-d14  
Concen: 0.373 ng  
RT: 19.621 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.004 min  
Lab File: BN037361.D ClientSampleId :  
Acq: 20 Jun 2025 22:16 PB168563BL

Tgt Ion:244 Resp: 3648  
Ion Ratio Lower Upper  
244 100  
212 12.5 11.1 16.7  
122 9.7 7.2 10.8

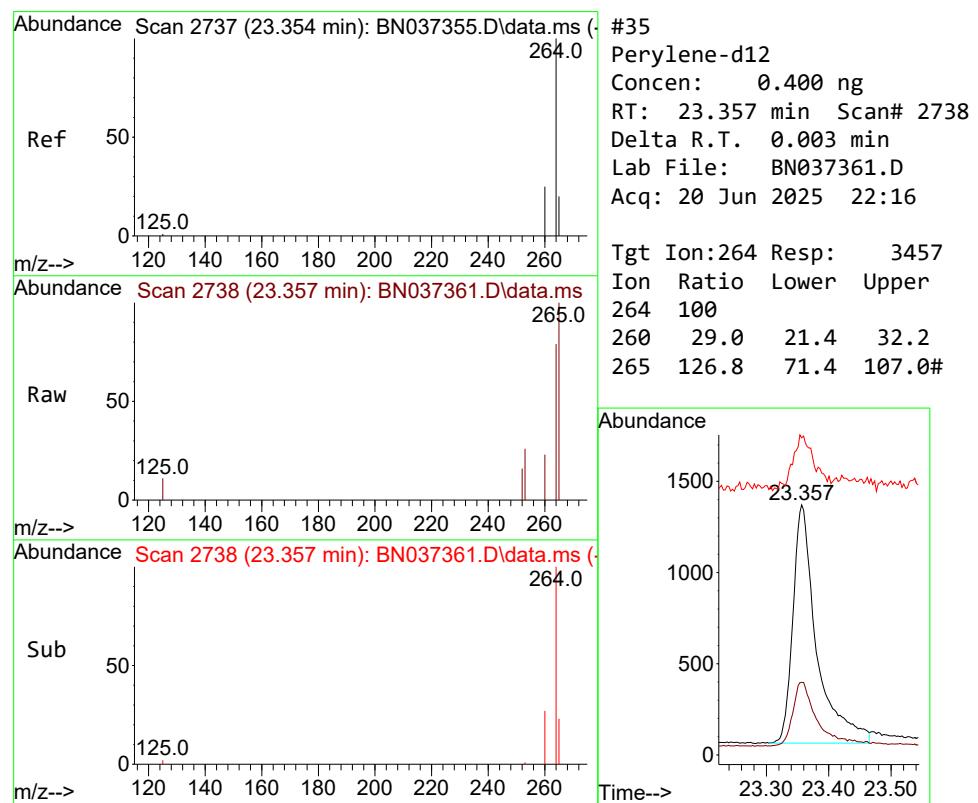

#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.357 min Scan# 2738  
Delta R.T. 0.003 min  
Lab File: BN037361.D  
Acq: 20 Jun 2025 22:16

Tgt Ion:264 Resp: 3457  
Ion Ratio Lower Upper  
264 100  
260 29.0 21.4 32.2  
265 126.8 71.4 107.0#





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Tetra Tech NUS, Inc.			Date Collected:	
Project:	NWIRP Bethpage 112G08005-WE13			Date Received:	
Client Sample ID:	PB168563BS			SDG No.:	Q2375
Lab Sample ID:	PB168563BS			Matrix:	Water
Analytical Method:	SW8270ESIM			% Solid:	0
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	1000 uL
Soil Aliquot Vol:			uL	Test:	SVOC-SIMGroup1
Extraction Type :		Decanted :	N	Level :	LOW
Injection Volume :		GPC Factor :	1.0	GPC Cleanup :	N
Prep Method :				PH :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN037363.D	1	06/20/25 12:03	06/20/25 23:28	PB168563

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
123-91-1	1,4-Dioxane	0.32		0.070	0.20	0.20	ug/L
<b>SURROGATES</b>							
7297-45-2	2-Methylnaphthalene-d10	0.49		30 - 150		123%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.35		30 - 150		86%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.37		55 - 111		92%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.39		53 - 106		97%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.39		58 - 132		98%	SPK: 0.4
<b>INTERNAL STANDARDS</b>							
3855-82-1	1,4-Dichlorobenzene-d4	1960		7.568			
1146-65-2	Naphthalene-d8	4200		10.34			
15067-26-2	Acenaphthene-d10	2590		14.213			
1517-22-2	Phenanthrene-d10	4830		16.971			
1719-03-5	Chrysene-d12	3880		21.171			
1520-96-3	Perylene-d12	2750		23.351			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037363.D  
 Acq On : 20 Jun 2025 23:28  
 Operator : RC/JU  
 Sample : PB168563BS  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BS

Quant Time: Jun 20 23:54:04 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1960	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4204	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2586	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	4830	0.400	ng	0.00
29) Chrysene-d12	21.171	240	3875	0.400	ng	0.00
35) Perylene-d12	23.351	264	2749	0.400	ng	# 0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.170	112	1356	0.346	ng	0.00
5) Phenol-d6	6.752	99	1369	0.339	ng	0.00
8) Nitrobenzene-d5	8.717	82	1246	0.367	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	3338	0.490	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	509	0.336	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	4401	0.387	ng	0.00
27) Fluoranthene-d10	19.007	212	4783	0.345	ng	0.00
31) Terphenyl-d14	19.616	244	3479	0.394	ng	0.00
<b>Target Compounds</b>						
				Qvalue		
2) 1,4-Dioxane	3.104	88	631	0.317	ng	# 32
3) n-Nitrosodimethylamine	3.415	42	717	0.392	ng	# 82
6) bis(2-Chloroethyl)ether	7.004	93	1334	0.373	ng	97
9) Naphthalene	10.394	128	4124	0.372	ng	# 90
10) Hexachlorobutadiene	10.682	225	1728	0.394	ng	# 99
12) 2-Methylnaphthalene	12.021	142	2530	0.327	ng	94
16) Acenaphthylene	13.935	152	4145	0.381	ng	98
17) Acenaphthene	14.277	154	2614	0.365	ng	99
18) Fluorene	15.271	166	3566	0.355	ng	99
20) 4,6-Dinitro-2-methylph...	15.378	198	387	0.333	ng	89
21) 4-Bromophenyl-phenylether	16.177	248	1258	0.366	ng	98
22) Hexachlorobenzene	16.276	284	1521	0.406	ng	99
23) Atrazine	16.462	200	89	0.032	ng	# 63
24) Pentachlorophenol	16.624	266	1322	0.709	ng	95
25) Phenanthrene	17.009	178	5063	0.362	ng	99
26) Anthracene	17.108	178	4541	0.352	ng	98
28) Fluoranthene	19.035	202	6071	0.343	ng	# 99
30) Pyrene	19.402	202	5679	0.361	ng	99
32) Benzo(a)anthracene	21.153	228	4660	0.366	ng	99
33) Chrysene	21.206	228	6398	0.414	ng	98
34) Bis(2-ethylhexyl)phtha...	21.090	149	1970	0.377	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.541	276	6014	0.488	ng	# 92
37) Benzo(b)fluoranthene	22.699	252	5246	0.519	ng	# 98
38) Benzo(k)fluoranthene	22.743	252	5910	0.539	ng	99
39) Benzo(a)pyrene	23.254	252	4418	0.487	ng	# 96
40) Dibenzo(a,h)anthracene	25.555	278	4975	0.537	ng	95
41) Benzo(g,h,i)perylene	26.201	276	5107	0.464	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037363.D  
 Acq On : 20 Jun 2025 23:28  
 Operator : RC/JU  
 Sample : PB168563BS  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BS


Quant Time: Jun 20 23:54:04 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

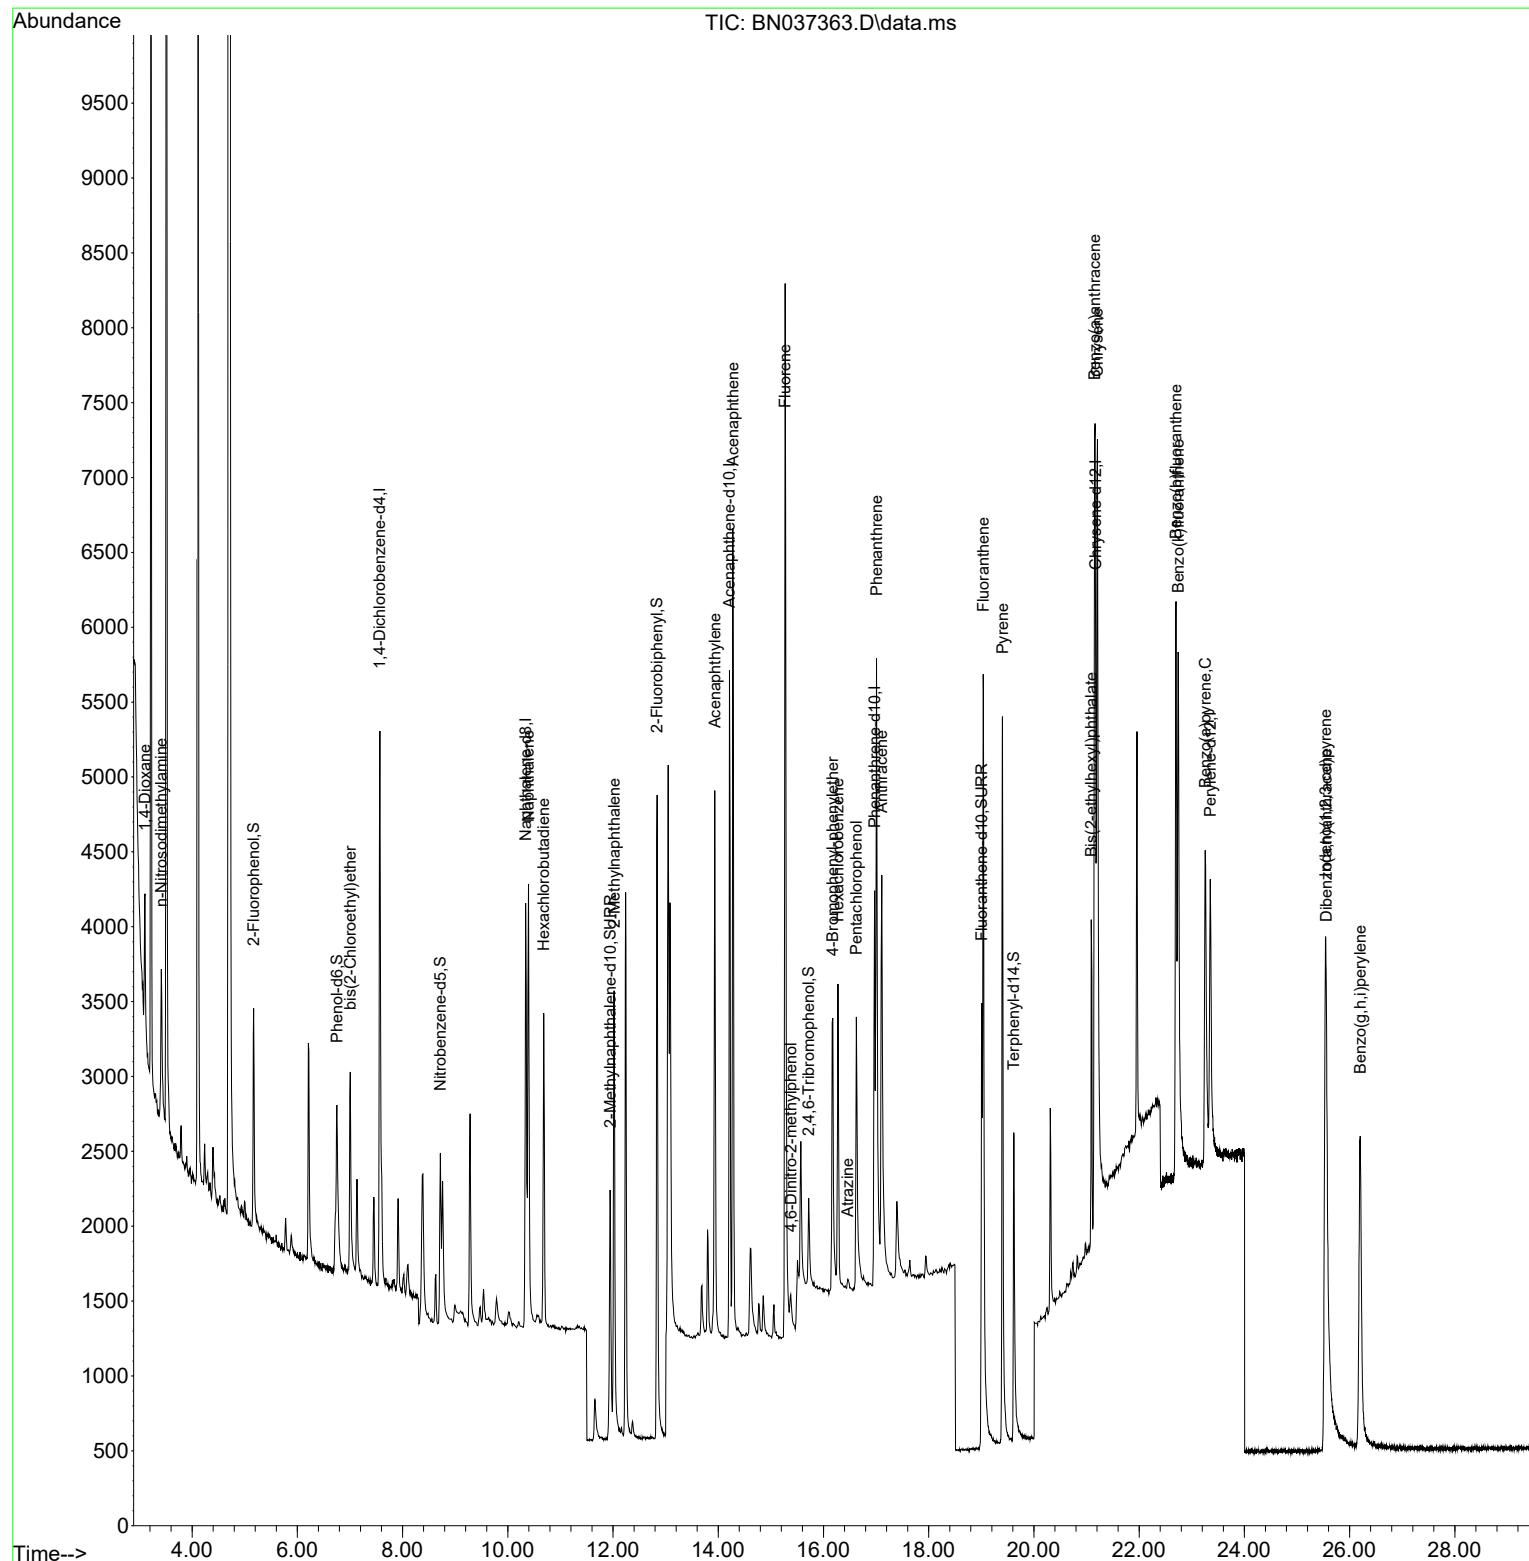



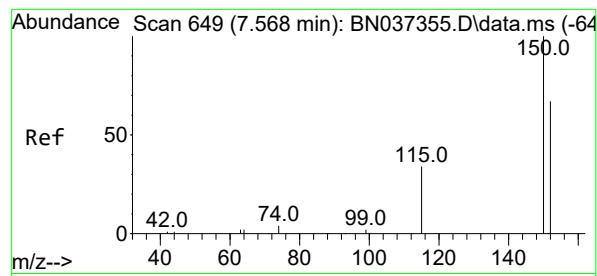


#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
ClientSampleId : PB168563BS





Tgt Ion:152 Resp: 1960  
Ion Ratio Lower Upper  
152 100  
150 152.8 112.7 169.1  
115 55.2 45.9 68.9





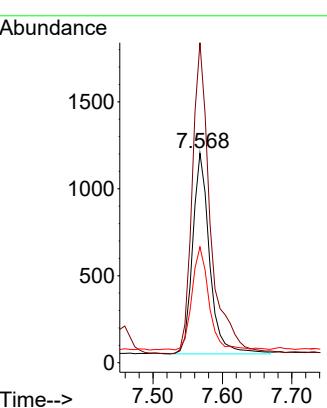



#2  
1,4-Dioxane  
Concen: 0.317 ng  
RT: 3.104 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28



Tgt Ion: 88 Resp: 631  
Ion Ratio Lower Upper  
88 100  
43 96.4 21.0 31.6#  
58 68.0 38.0 57.0#



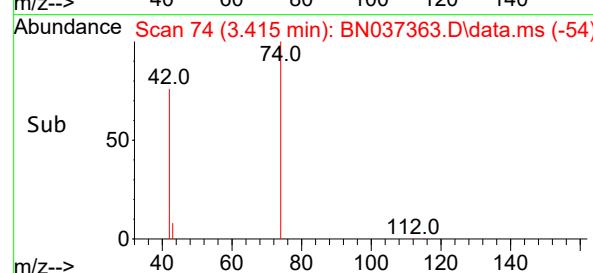

#3

n-Nitrosodimethylamine

Concen: 0.392 ng

RT: 3.415 min Scan# 7

Delta R.T. -0.007 min

Lab File: BN037363.D

Acq: 20 Jun 2025 23:28

Instrument :

BNA\_N

ClientSampleId :

PB168563BS


Tgt Ion: 42 Resp: 717

Ion Ratio Lower Upper

42 100

74 124.4 84.3 126.5

44 3.2 5.0 7.4#

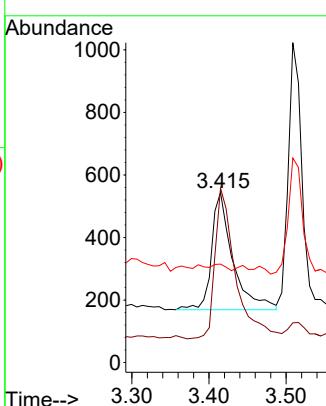

#4

2-Fluorophenol

Concen: 0.346 ng

RT: 5.170 min Scan# 317

Delta R.T. 0.007 min

Lab File: BN037363.D

Acq: 20 Jun 2025 23:28


Tgt Ion: 112 Resp: 1356




Ion Ratio Lower Upper

112 100

64 51.6 38.7 58.1

63 30.4 26.4 39.6




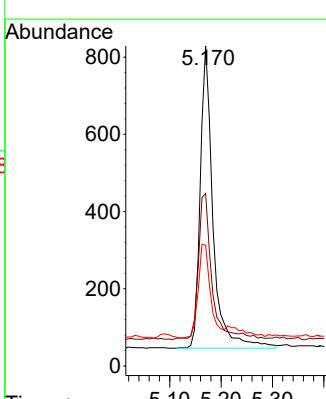


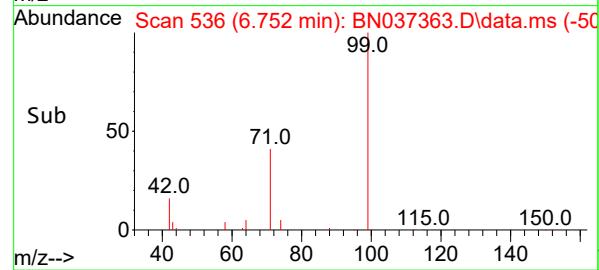

#5  
 Phenol-d6  
 Concen: 0.339 ng  
 RT: 6.752 min Scan# 5  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
 ClientSampleId : PB168563BS




Tgt Ion: 99 Resp: 1369  
 Ion Ratio Lower Upper  
 99 100  
 42 19.0 19.8 29.8#  
 71 44.8 42.6 64.0



#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.373 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28

Tgt Ion: 93 Resp: 1334  
 Ion Ratio Lower Upper  
 93 100  
 63 63.3 53.2 79.8  
 95 34.0 27.3 40.9




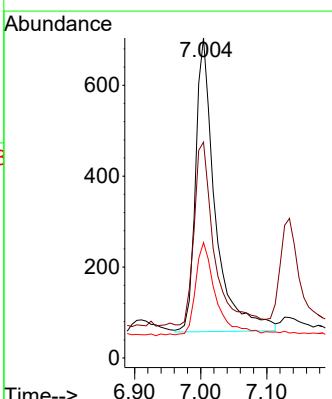




#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28


Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BS




Tgt Ion:136 Resp: 4204  
 Ion Ratio Lower Upper  
 136 100  
 137 13.2 12.2 18.2  
 54 8.4 8.8 13.2#  
 68 6.7 7.0 10.4#

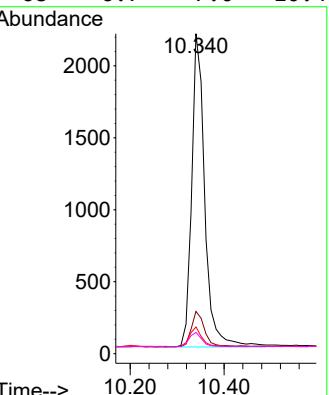

#8  
 Nitrobenzene-d5  
 Concen: 0.367 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28





Tgt Ion: 82 Resp: 1246  
 Ion Ratio Lower Upper  
 82 100  
 128 43.7 42.5 63.7  
 54 44.2 43.2 64.8

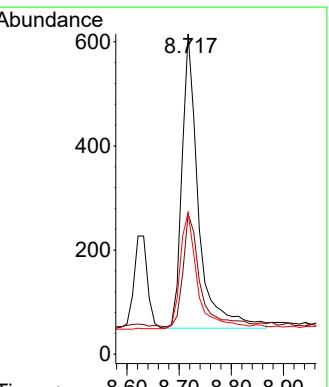




#9  
Naphthalene  
Concen: 0.372 ng  
RT: 10.394 min Scan# 9  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28  
ClientSampleId : PB168563BS




Tgt Ion:128 Resp: 4124  
Ion Ratio Lower Upper  
128 100  
129 13.3 14.0 21.0#  
127 15.1 15.8 23.8#



#10  
Hexachlorobutadiene  
Concen: 0.394 ng  
RT: 10.682 min Scan# 974  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:225 Resp: 1728  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 63.7 50.3 75.5



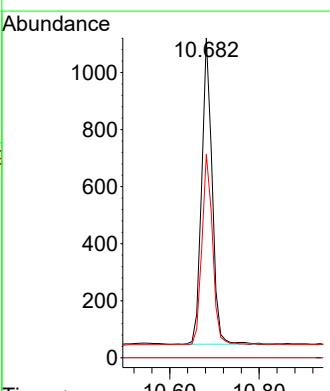




#11  
2-Methylnaphthalene-d10  
Concen: 0.490 ng  
RT: 11.945 min Scan# 1138  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
ClientSampleId : PB168563BS


Tgt Ion:152 Resp: 3338  
Ion Ratio Lower Upper  
152 100  
151 15.7 17.4 26.0#

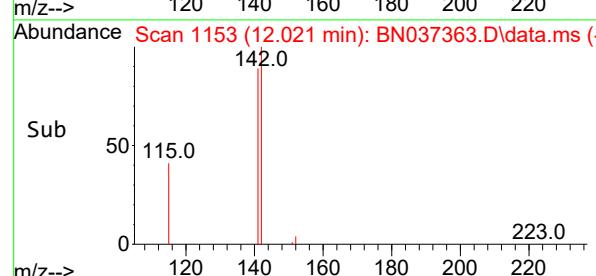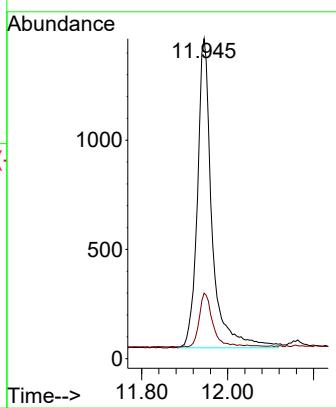

#12  
2-Methylnaphthalene  
Concen: 0.327 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:142 Resp: 2530  
Ion Ratio Lower Upper  
142 100  
141 88.8 70.2 105.2  
115 44.3 43.0 64.4

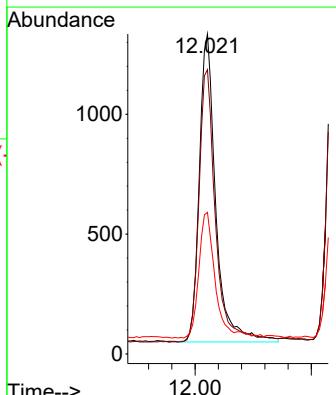

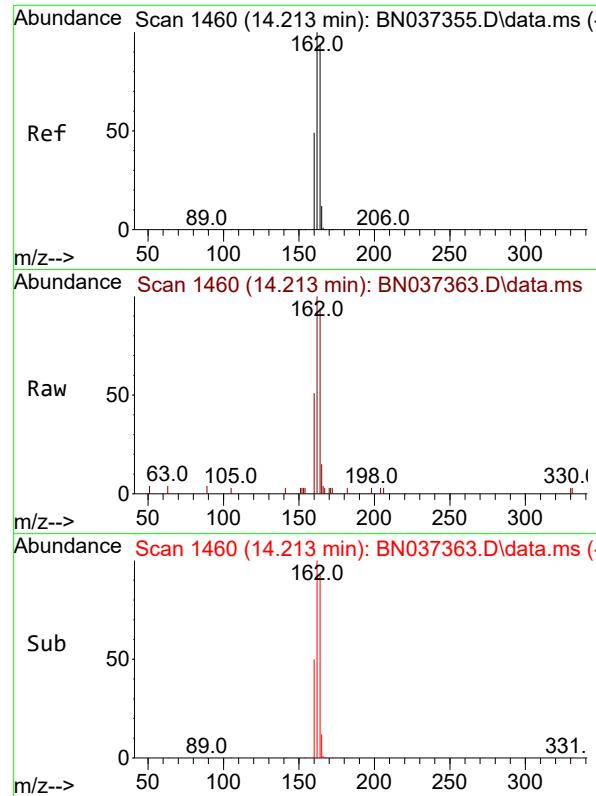

#13

Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Instrument :

BNA\_N

ClientSampleId :



PB168563BS

Tgt Ion:164 Resp: 2586

Ion	Ratio	Lower	Upper
164	100		
162	106.7	81.5	122.3
160	54.8	43.0	64.4

Abundance

14.213

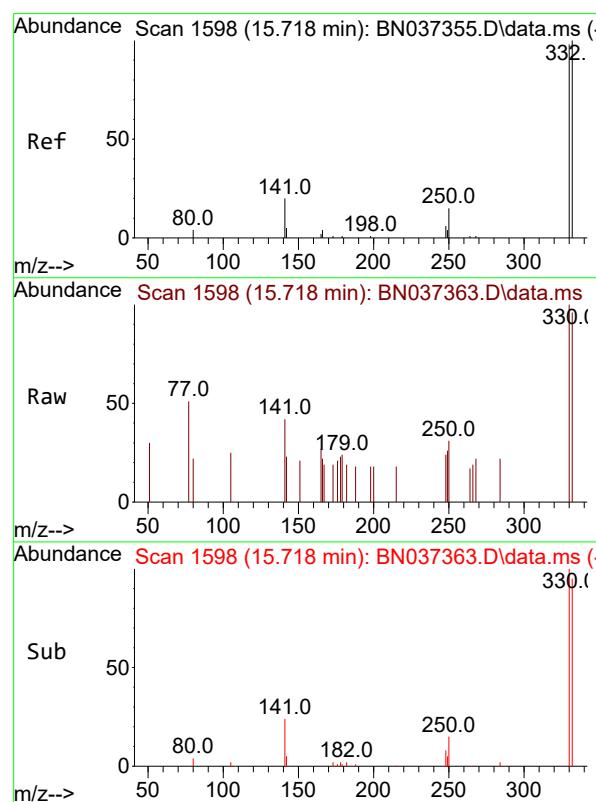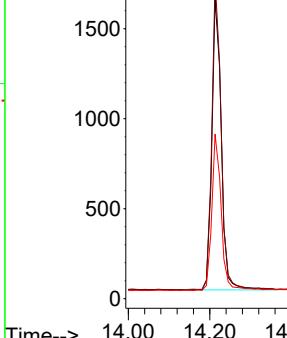

#14


2,4,6-Tribromophenol  
Concen: 0.336 ng  
RT: 15.718 min Scan# 1598  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28




Tgt Ion:330 Resp: 509

Ion	Ratio	Lower	Upper
330	100		
332	94.9	78.4	117.6
141	30.1	24.4	36.6

Abundance

15.718




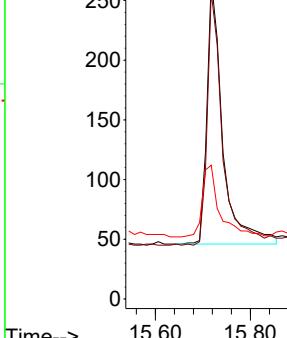




#15  
2-Fluorobiphenyl  
Concen: 0.387 ng  
RT: 12.838 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
ClientSampleId : PB168563BS




Tgt Ion:172 Resp: 4401  
Ion Ratio Lower Upper  
172 100  
171 36.9 30.8 46.2  
170 24.9 21.9 32.9



#16  
Acenaphthylene  
Concen: 0.381 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:152 Resp: 4145  
Ion Ratio Lower Upper  
152 100  
151 20.0 16.6 24.8  
153 13.4 10.2 15.2








#17  
Acenaphthene  
Concen: 0.365 ng  
RT: 14.277 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
ClientSampleId : PB168563BS

Tgt Ion:154 Resp: 2614  
Ion Ratio Lower Upper  
154 100  
153 116.8 93.1 139.7  
152 62.5 48.6 73.0

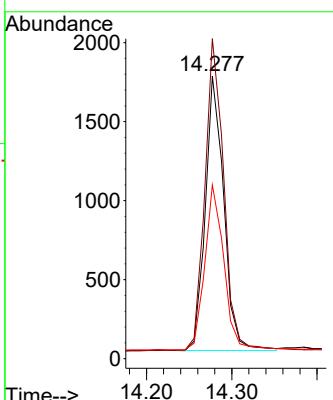

#18  
Fluorene  
Concen: 0.355 ng  
RT: 15.271 min Scan# 1559  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:166 Resp: 3566  
Ion Ratio Lower Upper  
166 100  
165 100.6 79.5 119.3  
167 14.3 10.7 16.1

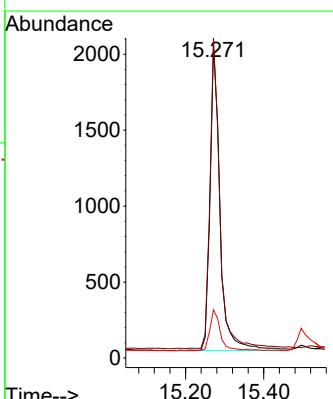

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037363.D




Acq: 20 Jun 2025 23:28

Instrument:

BNA\_N

ClientSampleId :

PB168563BS

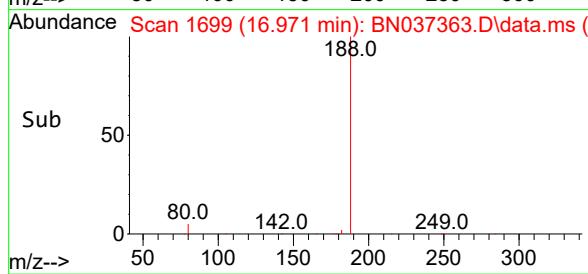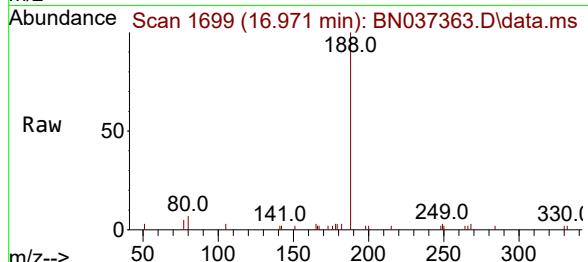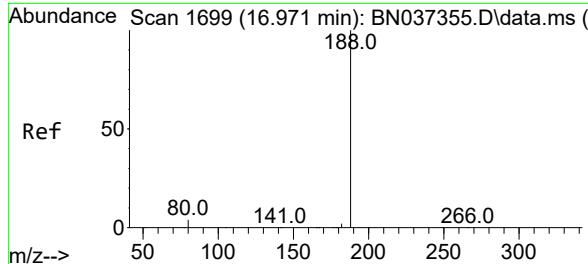





Tgt Ion:188 Resp: 4830

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 6.9 6.2 9.2

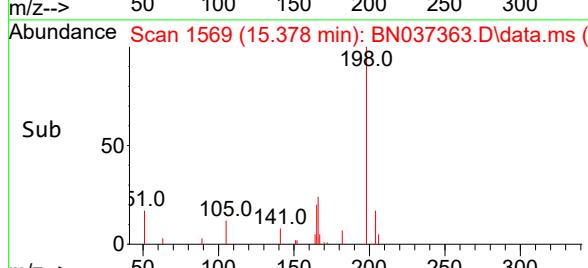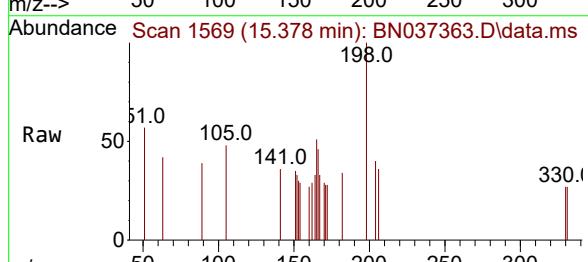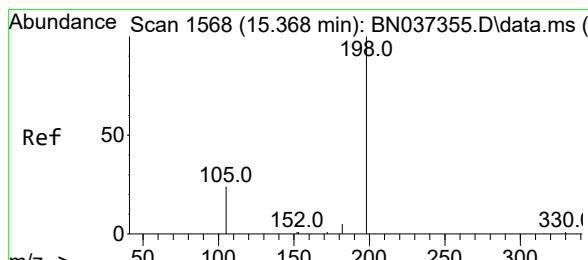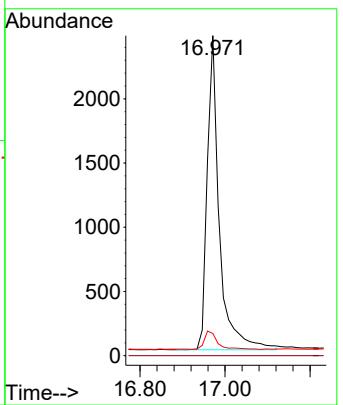

#20

4,6-Dinitro-2-methylphenol

Concen: 0.333 ng

RT: 15.378 min Scan# 1569

Delta R.T. 0.011 min

Lab File: BN037363.D

Acq: 20 Jun 2025 23:28


Tgt Ion:198 Resp: 387


Ion Ratio Lower Upper

198 100

51 56.5 51.4 77.0

105 48.2 45.5 68.3


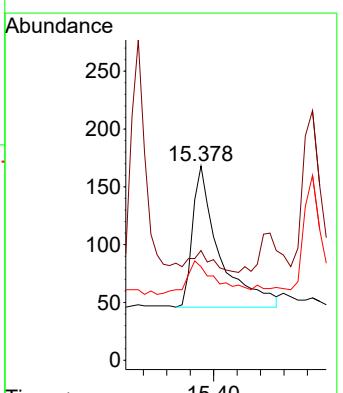


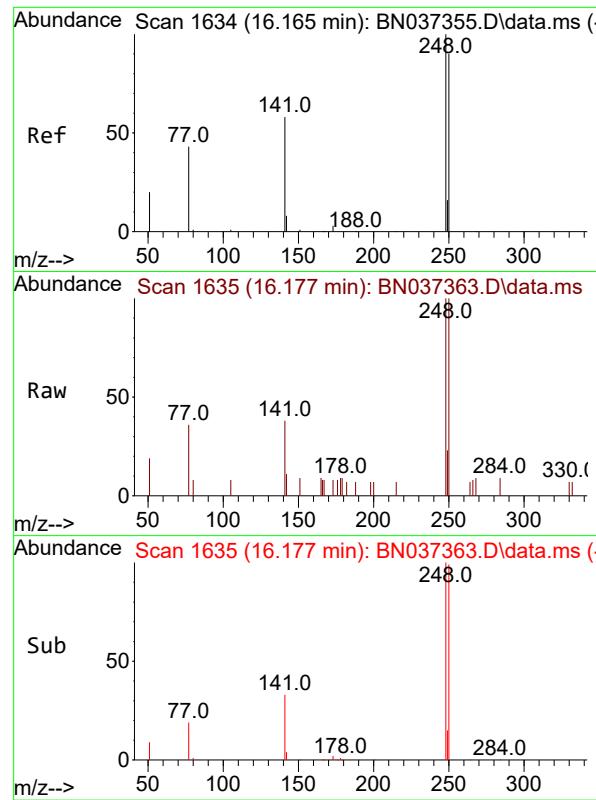

#21  
4-Bromophenyl-phenylether  
Concen: 0.366 ng  
RT: 16.177 min Scan# 1  
Delta R.T. 0.012 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28


Instrument :  
BNA\_N  
ClientSampleId :  
PB168563BS




Tgt Ion:248 Resp: 1258  
Ion Ratio Lower Upper  
248 100  
250 100.0 80.4 120.6  
141 38.3 33.3 49.9

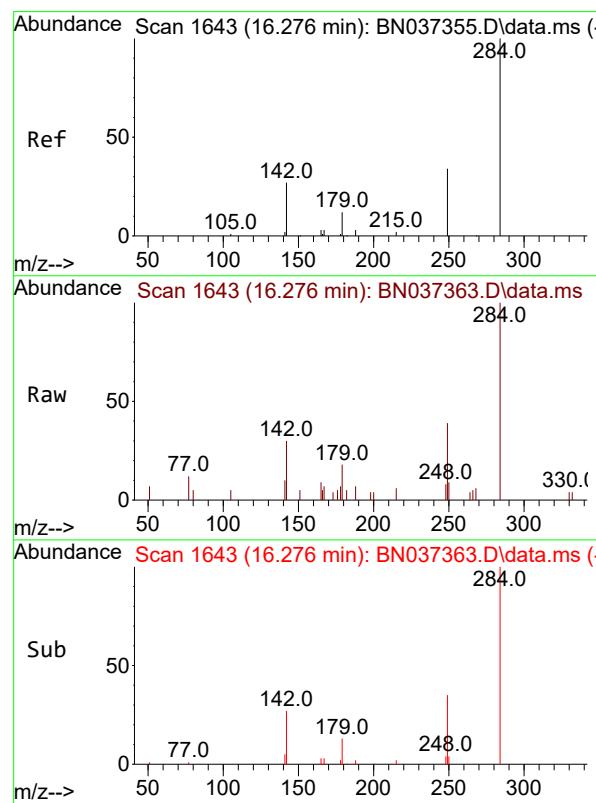

#22  
Hexachlorobenzene  
Concen: 0.406 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:284 Resp: 1521  
Ion Ratio Lower Upper  
284 100  
142 34.2 27.0 40.6  
249 34.9 28.8 43.2








#23

Atrazine  
Concen: 0.032 ng  
RT: 16.462 min Scan# 1  
Delta R.T. 0.012 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28


Instrument :  
BNA\_N  
ClientSampleId :  
PB168563BS




Tgt Ion:200 Resp: 89  
Ion Ratio Lower Upper  
200 100  
173 69.6 29.2 43.8#  
215 81.0 48.8 73.2#

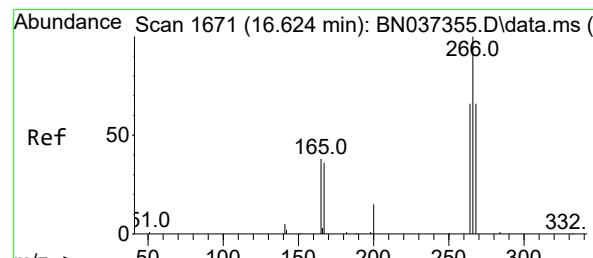

#24  
Pentachlorophenol  
Concen: 0.709 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:266 Resp: 1322  
Ion Ratio Lower Upper  
266 100  
264 62.1 50.3 75.5  
268 62.8 55.3 82.9





#25

Phenanthrene

Concen: 0.362 ng

RT: 17.009 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037363.D

Acq: 20 Jun 2025 23:28

Instrument:

BNA\_N

ClientSampleId :

PB168563BS

Tgt Ion:178 Resp: 5063





Ion Ratio Lower Upper

178 100

176 19.5 15.2 22.8

179 15.4 12.9 19.3

Abundance

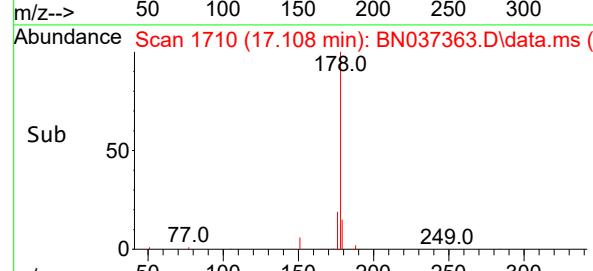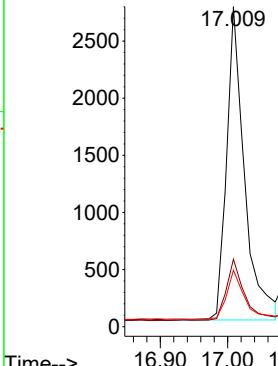

#26

Anthracene

Concen: 0.352 ng

RT: 17.108 min Scan# 1710

Delta R.T. -0.000 min

Lab File: BN037363.D

Acq: 20 Jun 2025 23:28

Tgt Ion:178 Resp: 4541


Ion Ratio Lower Upper


178 100

176 19.5 14.7 22.1

179 15.4 13.0 19.6

Abundance


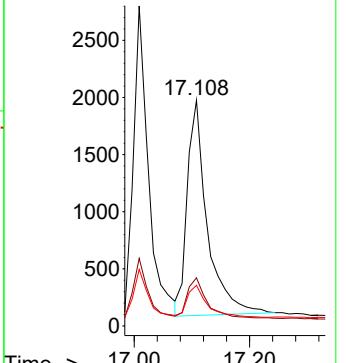


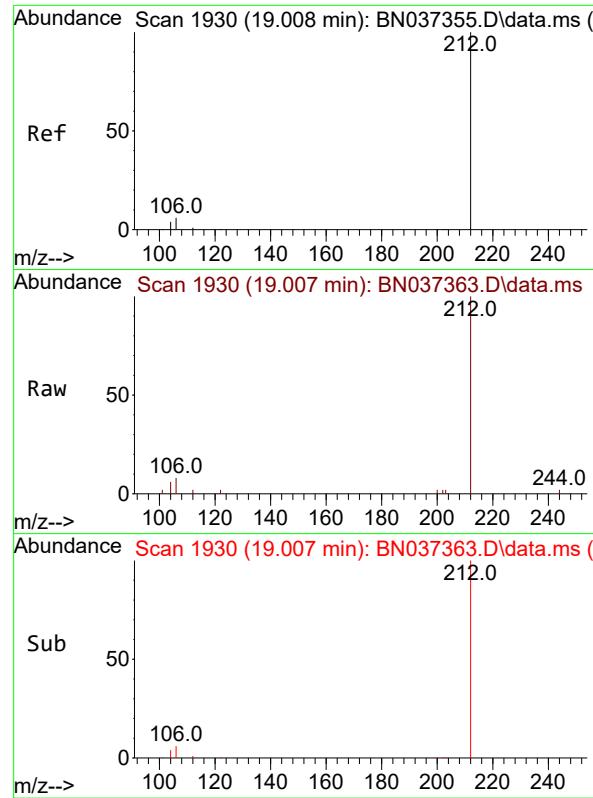

#27  
 Fluoranthene-d10  
 Concen: 0.345 ng  
 RT: 19.007 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
 ClientSampleId : PB168563BS




Tgt Ion:212 Resp: 4783  
 Ion Ratio Lower Upper  
 212 100  
 106 5.9 3.0 4.4#  
 104 3.7 2.0 3.0#

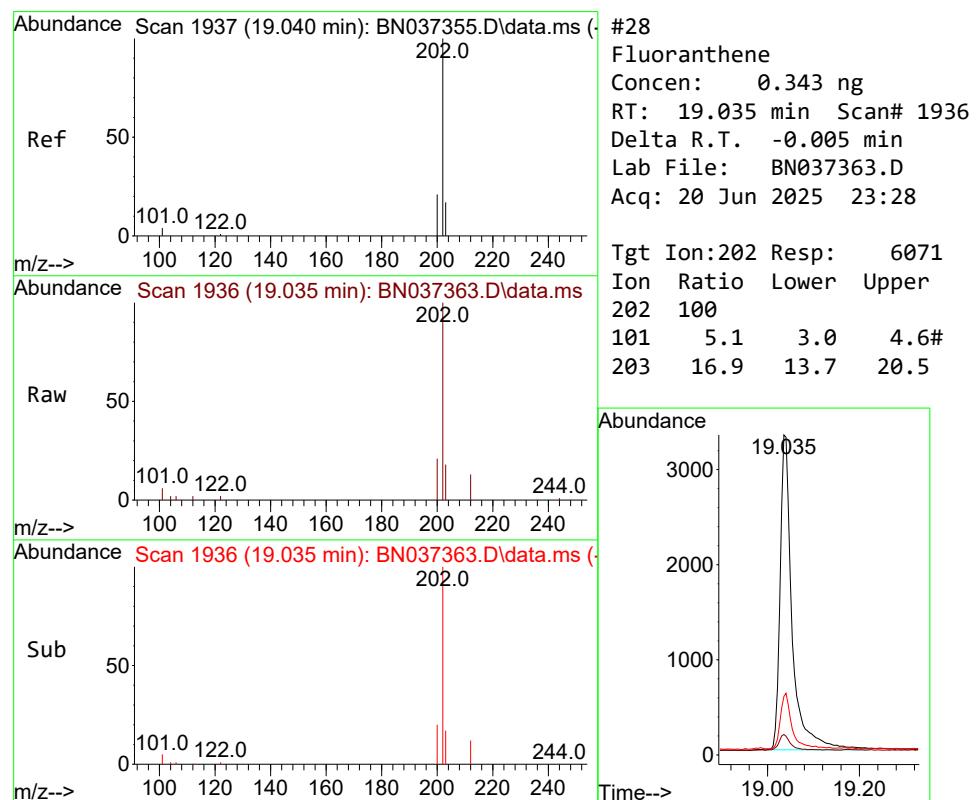

#28  
 Fluoranthene  
 Concen: 0.343 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28




Tgt Ion:202 Resp: 6071  
 Ion Ratio Lower Upper  
 202 100  
 101 5.1 3.0 4.6#  
 203 16.9 13.7 20.5







#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.171 min Scan# 2  
Instrument: BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28  
ClientSampleId : PB168563BS


Tgt Ion:240 Resp: 3875  
Ion Ratio Lower Upper  
240 100  
120 8.3 7.5 11.3  
236 29.7 24.9 37.3

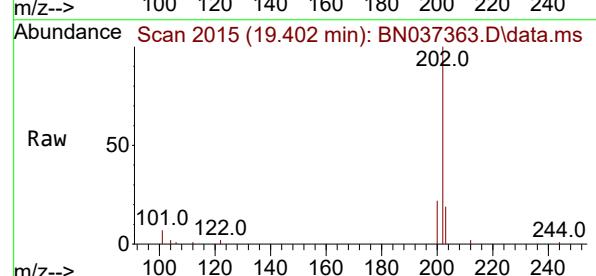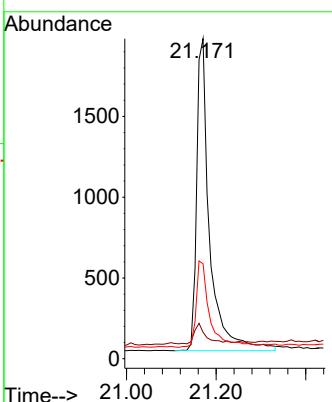

#30  
Pyrene  
Concen: 0.361 ng  
RT: 19.402 min Scan# 2015  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:202 Resp: 5679  
Ion Ratio Lower Upper  
202 100  
200 20.8 16.8 25.2  
203 17.2 14.5 21.7





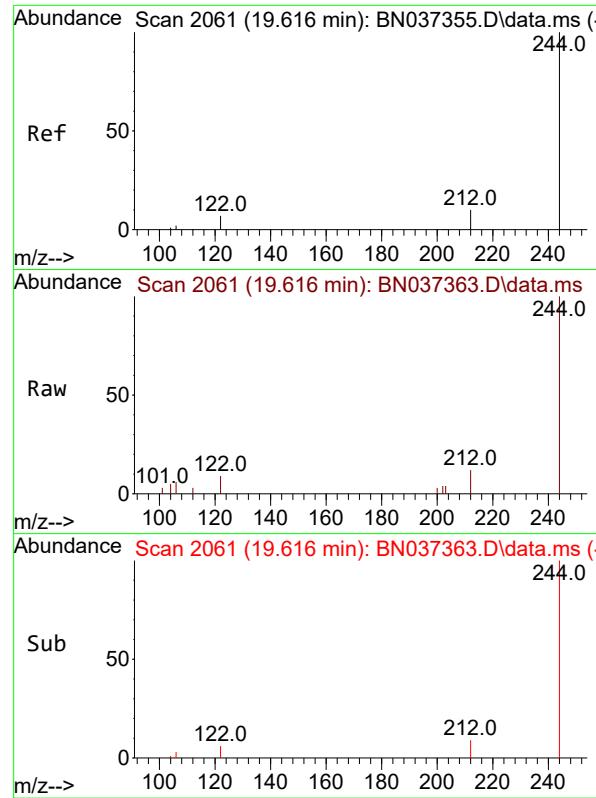

#31  
 Terphenyl-d14  
 Concen: 0.394 ng  
 RT: 19.616 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
 ClientSampleId : PB168563BS




Tgt Ion:244 Resp: 3479  
 Ion Ratio Lower Upper  
 244 100  
 212 12.1 11.1 16.7  
 122 9.0 7.2 10.8

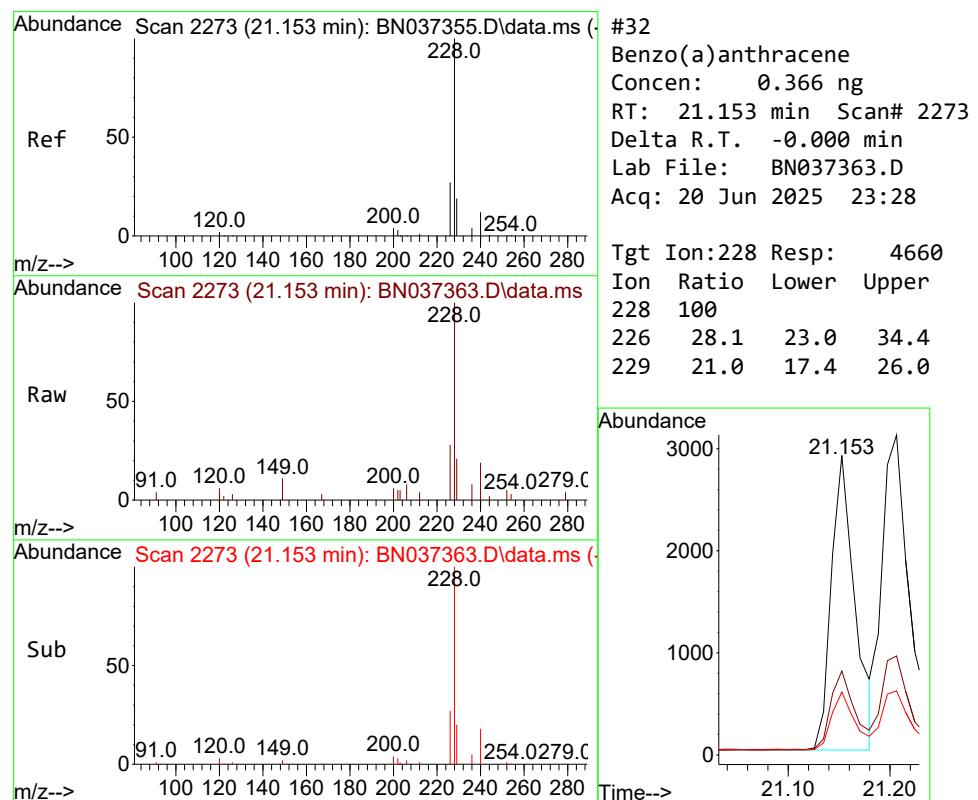

#32  
 Benzo(a)anthracene  
 Concen: 0.366 ng  
 RT: 21.153 min Scan# 2273  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28





Tgt Ion:228 Resp: 4660  
 Ion Ratio Lower Upper  
 228 100  
 226 28.1 23.0 34.4  
 229 21.0 17.4 26.0



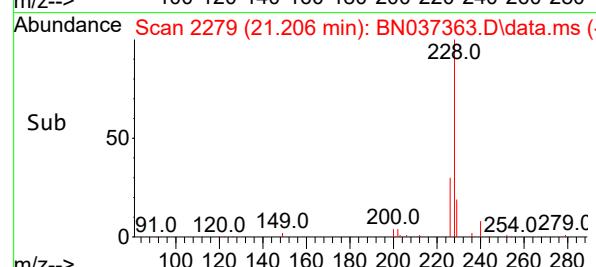


#33  
Chrysene  
Concen: 0.414 ng  
RT: 21.206 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28  
ClientSampleId : PB168563BS


Tgt Ion:228 Resp: 6398  
Ion Ratio Lower Upper  
228 100  
226 31.0 25.4 38.2  
229 20.1 17.3 25.9

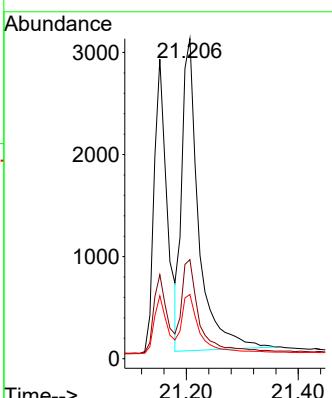

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.377 ng  
RT: 21.090 min Scan# 2266  
Delta R.T. -0.009 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:149 Resp: 1970  
Ion Ratio Lower Upper  
149 100  
167 31.2 24.6 37.0  
279 6.2 6.5 9.7#


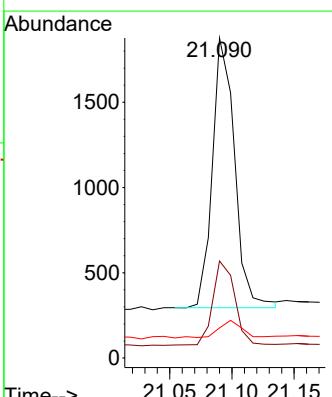


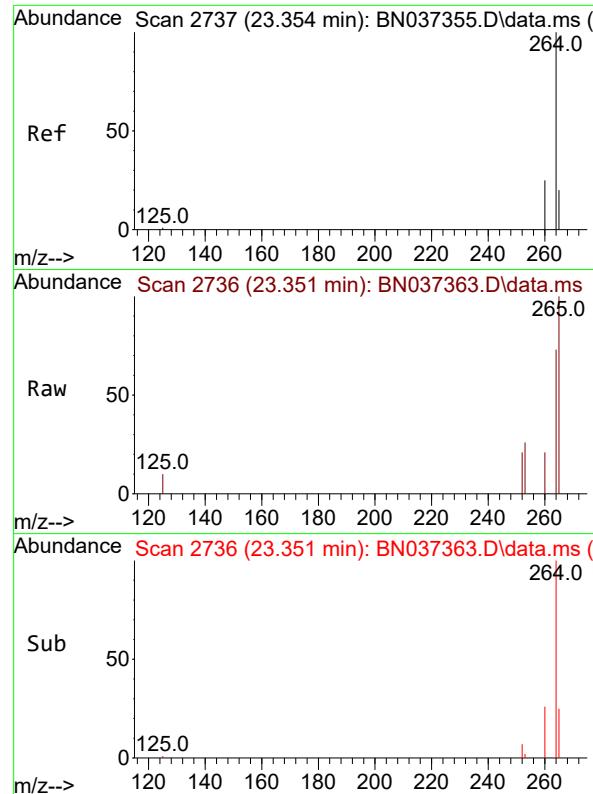

#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.351 min Scan# 2  
Delta R.T. -0.003 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
ClientSampleId : PB168563BS


Tgt Ion:264 Resp: 2749  
Ion Ratio Lower Upper  
264 100  
260 28.5 21.4 32.2  
265 137.6 71.4 107.0#

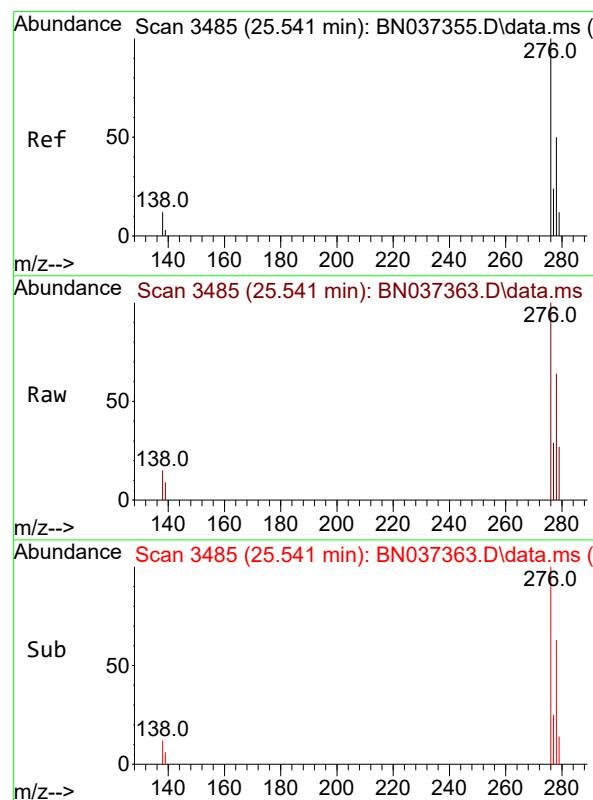

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.488 ng  
RT: 25.541 min Scan# 3485  
Delta R.T. -0.000 min  
Lab File: BN037363.D  
Acq: 20 Jun 2025 23:28

Tgt Ion:276 Resp: 6014  
Ion Ratio Lower Upper  
276 100  
138 11.2 2.2 3.2#  
277 24.2 17.1 25.7





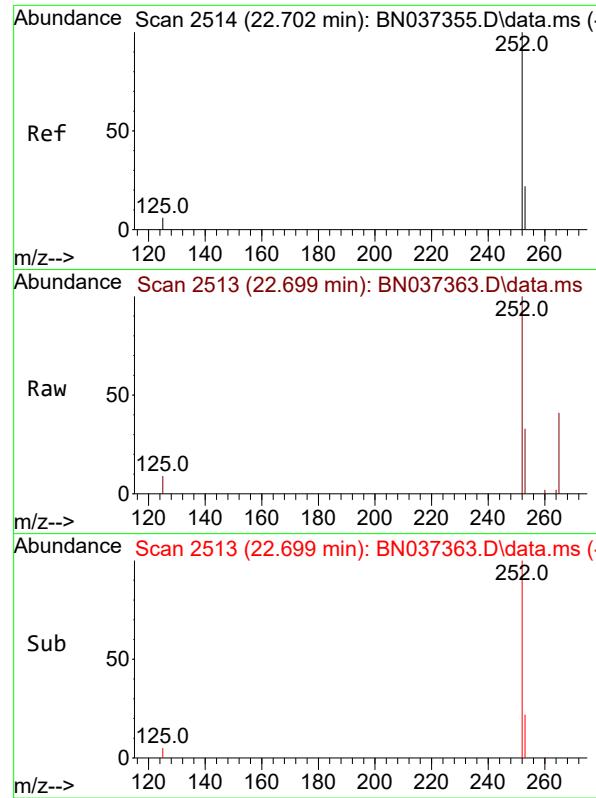

#37  
 Benzo(b)fluoranthene  
 Concen: 0.519 ng  
 RT: 22.699 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
 ClientSampleId : PB168563BS


Tgt Ion:252 Resp: 5246  
 Ion Ratio Lower Upper  
 252 100  
 253 32.6 26.6 40.0  
 125 9.5 6.1 9.1#

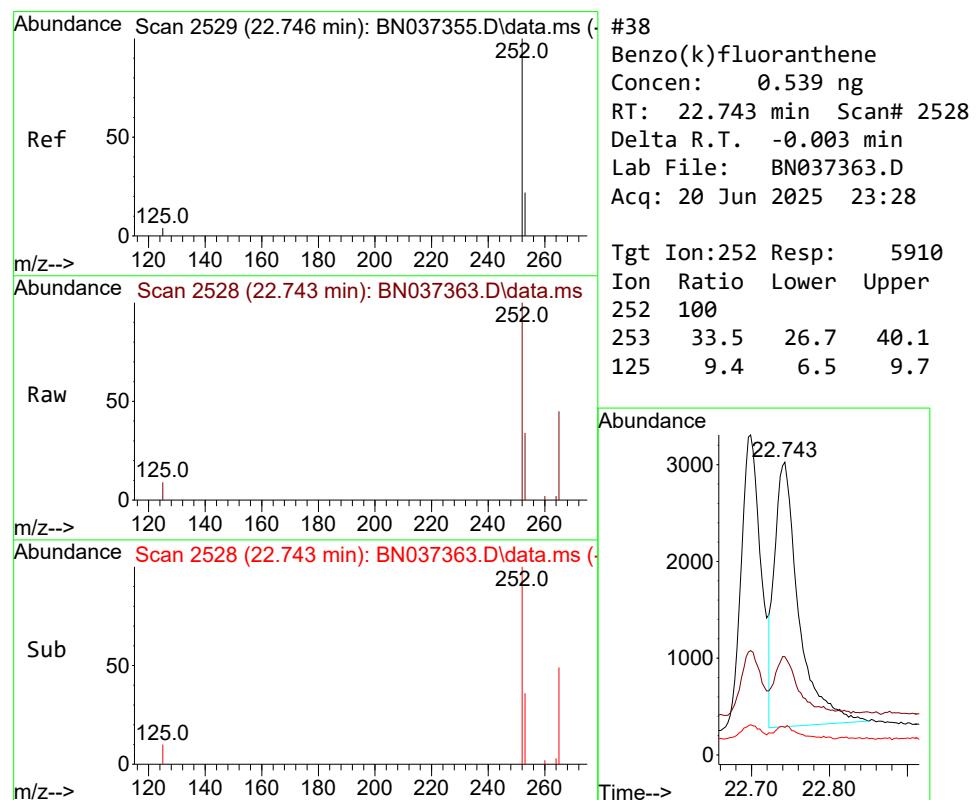

#38  
 Benzo(k)fluoranthene  
 Concen: 0.539 ng  
 RT: 22.743 min Scan# 2528  
 Delta R.T. -0.003 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28

Tgt Ion:252 Resp: 5910  
 Ion Ratio Lower Upper  
 252 100  
 253 33.5 26.7 40.1  
 125 9.4 6.5 9.7





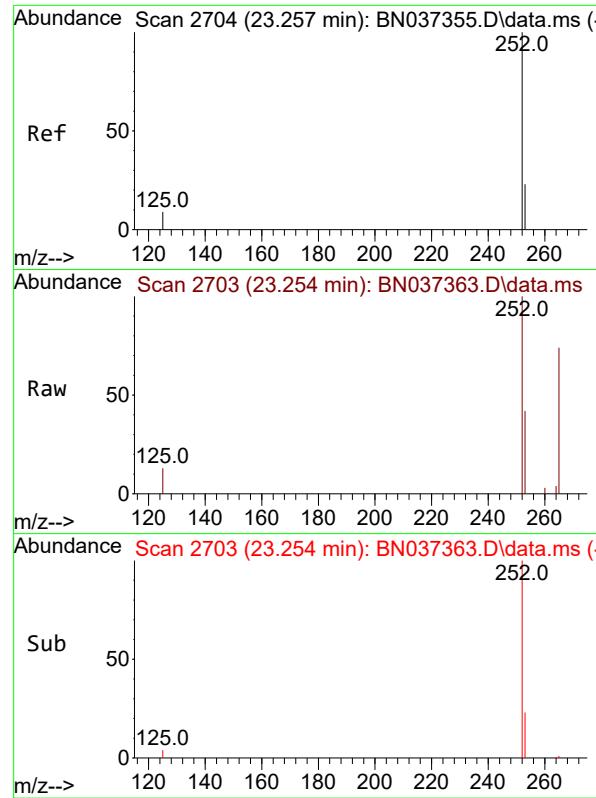

#39  
 Benzo(a)pyrene  
 Concen: 0.487 ng  
 RT: 23.254 min Scan# 2  
 Delta R.T. -0.003 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28


Instrument : BNA\_N  
 ClientSampleId : PB168563BS


Tgt Ion:252 Resp: 4418  
 Ion Ratio Lower Upper  
 252 100  
 253 41.9 31.6 47.4  
 125 12.8 8.4 12.6#

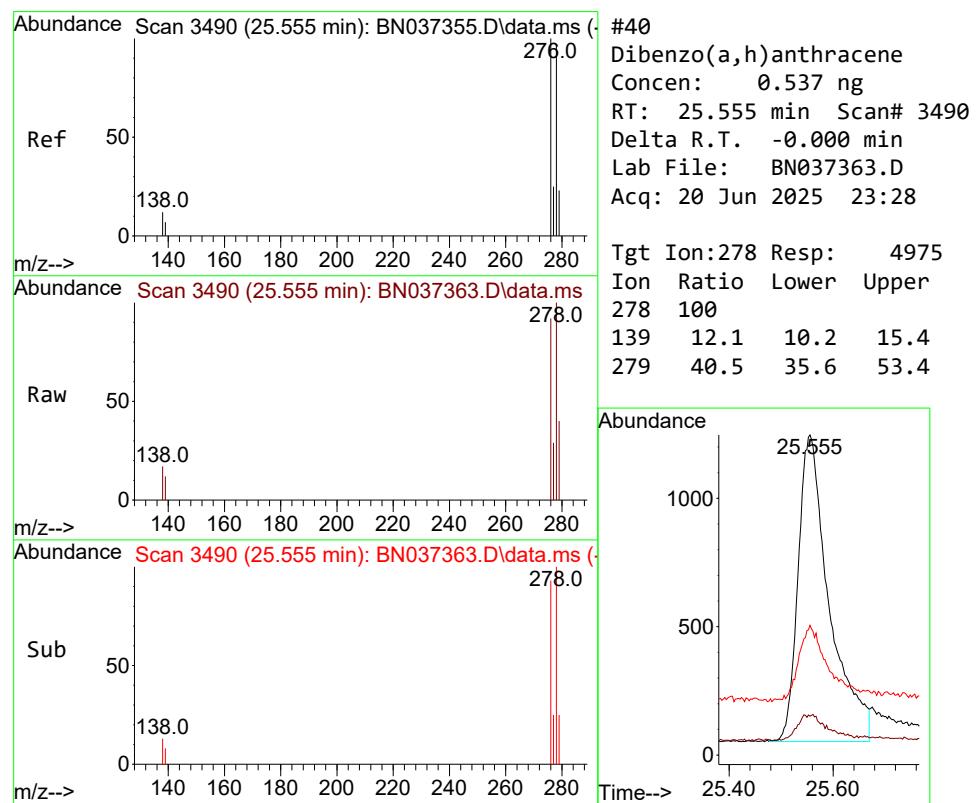

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.537 ng  
 RT: 25.555 min Scan# 3490  
 Delta R.T. -0.000 min  
 Lab File: BN037363.D  
 Acq: 20 Jun 2025 23:28

Tgt Ion:278 Resp: 4975  
 Ion Ratio Lower Upper  
 278 100  
 139 12.1 10.2 15.4  
 279 40.5 35.6 53.4



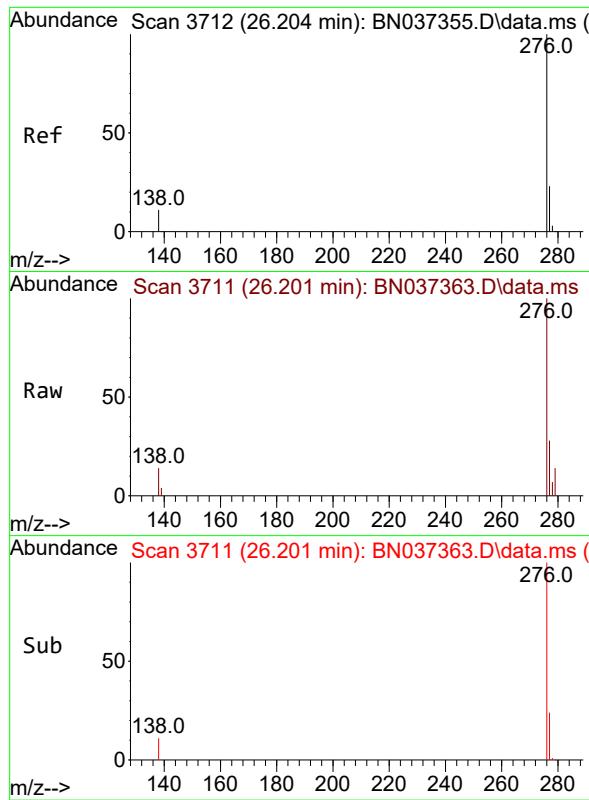

#41

Benzo(g,h,i)perylene

Concen: 0.464 ng

RT: 26.201 min Scan# 3

Instrument :

BNA\_N

Delta R.T. -0.003 min

Lab File: BN037363.D

ClientSampleId :

Acq: 20 Jun 2025 23:28

PB168563BS


Tgt Ion:276 Resp: 5107

Ion Ratio Lower Upper

276 100

277 27.9 22.7 34.1

138 14.2 9.4 14.2#

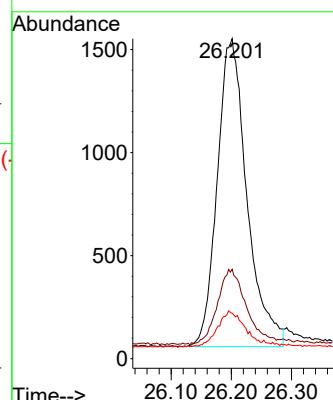



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,  
Fax : 908 789 8922

## Report of Analysis

Client:	Tetra Tech NUS, Inc.			Date Collected:	
Project:	NWIRP Bethpage 112G08005-WE13			Date Received:	
Client Sample ID:	PB168563BSD			SDG No.:	Q2375
Lab Sample ID:	PB168563BSD			Matrix:	Water
Analytical Method:	SW8270ESIM			% Solid:	0
Sample Wt/Vol:	1000	Units:	mL	Final Vol:	1000 uL
Soil Aliquot Vol:			uL	Test:	SVOC-SIMGroup1
Extraction Type :		Decanted :	N	Level :	LOW
Injection Volume :		GPC Factor :	1.0	GPC Cleanup :	N
Prep Method :				PH :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
BN037364.D	1	06/20/25 12:03	06/21/25 00:04	PB168563

CAS Number	Parameter	Conc.	Qualifier	MDL	LOD	LOQ / CRQL	Units
<b>TARGETS</b>							
123-91-1	1,4-Dioxane	0.30		0.070	0.20	0.20	ug/L
<b>SURROGATES</b>							
7297-45-2	2-Methylnaphthalene-d10	0.39		30 - 150		97%	SPK: 0.4
93951-69-0	Fluoranthene-d10	0.35		30 - 150		86%	SPK: 0.4
4165-60-0	Nitrobenzene-d5	0.39		55 - 111		97%	SPK: 0.4
321-60-8	2-Fluorobiphenyl	0.40		53 - 106		99%	SPK: 0.4
1718-51-0	Terphenyl-d14	0.38		58 - 132		94%	SPK: 0.4
<b>INTERNAL STANDARDS</b>							
3855-82-1	1,4-Dichlorobenzene-d4	1890		7.568			
1146-65-2	Naphthalene-d8	4100		10.34			
15067-26-2	Acenaphthene-d10	2620		14.213			
1517-22-2	Phenanthrene-d10	5040		16.971			
1719-03-5	Chrysene-d12	4190		21.162			
1520-96-3	Perylene-d12	4470		23.354			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

\* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037364.D  
 Acq On : 21 Jun 2025 00:04  
 Operator : RC/JU  
 Sample : PB168563BSD  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BSD

Quant Time: Jun 21 00:33:22 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1885	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4095	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2623	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5035	0.400	ng	# 0.00
29) Chrysene-d12	21.162	240	4193	0.400	ng	0.00
35) Perylene-d12	23.354	264	4470	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.170	112	1274	0.338	ng	0.00
5) Phenol-d6	6.752	99	1342	0.346	ng	0.00
8) Nitrobenzene-d5	8.717	82	1284	0.388	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	2563m	0.386	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	522	0.339	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	4574	0.397	ng	0.00
27) Fluoranthene-d10	19.007	212	5003	0.346	ng	0.00
31) Terphenyl-d14	19.616	244	3587	0.375	ng	0.00
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) 1,4-Dioxane	3.104	88	583	0.304	ng	# 36
3) n-Nitrosodimethylamine	3.415	42	653	0.372	ng	# 70
6) bis(2-Chloroethyl)ether	7.004	93	1260	0.366	ng	99
9) Naphthalene	10.394	128	4026	0.372	ng	# 89
10) Hexachlorobutadiene	10.682	225	1748	0.410	ng	# 100
12) 2-Methylnaphthalene	12.021	142	2474	0.328	ng	93
16) Acenaphthylene	13.935	152	4445	0.403	ng	98
17) Acenaphthene	14.277	154	2642	0.364	ng	98
18) Fluorene	15.271	166	3709	0.364	ng	99
20) 4,6-Dinitro-2-methylph...	15.378	198	419	0.346	ng	# 81
21) 4-Bromophenyl-phenylether	16.177	248	1344	0.375	ng	96
22) Hexachlorobenzene	16.276	284	1596	0.409	ng	99
23) Atrazine	16.450	200	1011	0.354	ng	# 88
24) Pentachlorophenol	16.624	266	1337	0.688	ng	97
25) Phenanthrene	17.009	178	5370	0.368	ng	99
26) Anthracene	17.108	178	4862	0.362	ng	99
28) Fluoranthene	19.035	202	6244	0.339	ng	# 99
30) Pyrene	19.402	202	6351	0.373	ng	99
32) Benzo(a)anthracene	21.153	228	5141	0.373	ng	99
33) Chrysene	21.206	228	6472	0.387	ng	97
34) Bis(2-ethylhexyl)phtha...	21.090	149	2023	0.358	ng	96
36) Indeno(1,2,3-cd)pyrene	25.538	276	7744	0.386	ng	# 92
37) Benzo(b)fluoranthene	22.696	252	5838	0.355	ng	95
38) Benzo(k)fluoranthene	22.740	252	6945	0.389	ng	96
39) Benzo(a)pyrene	23.254	252	5888	0.399	ng	95
40) Dibenzo(a,h)anthracene	25.552	278	5912	0.392	ng	89
41) Benzo(g,h,i)perylene	26.199	276	7039	0.393	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037364.D  
 Acq On : 21 Jun 2025 00:04  
 Operator : RC/JU  
 Sample : PB168563BSD  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1


Quant Time: Jun 21 00:33:22 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BSD

**Manual Integrations**  
**APPROVED**


Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

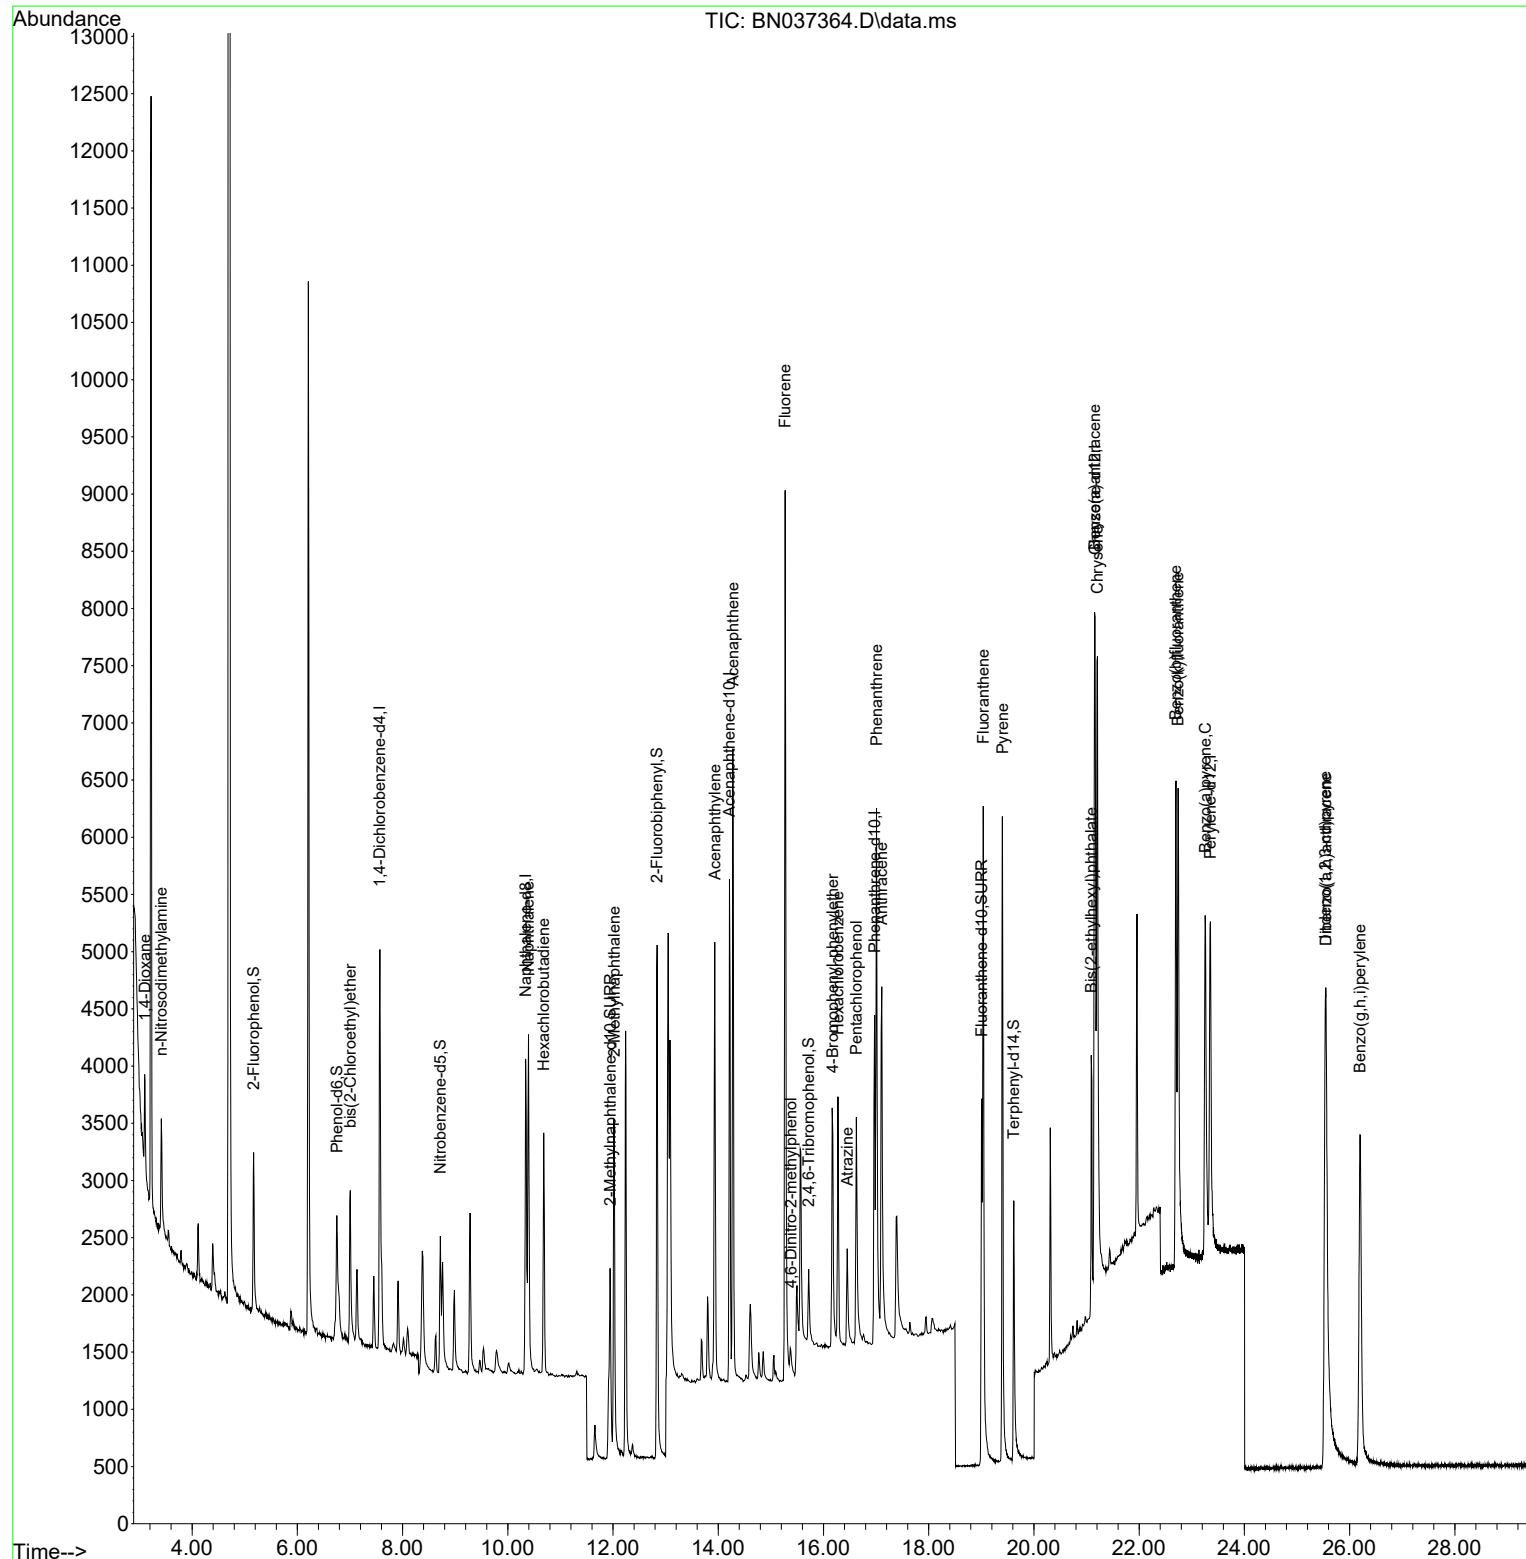

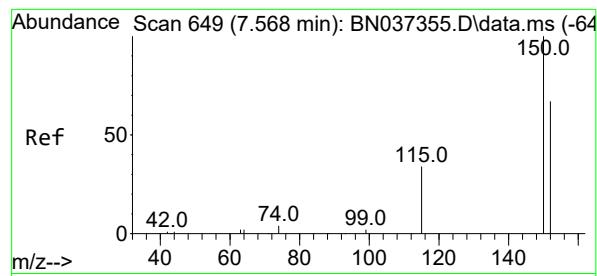

#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 6  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04




Instrument : BNA\_N  
ClientSampleId : PB168563BSD

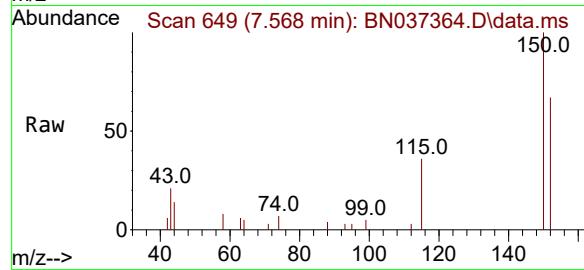


Tgt Ion:152 Resp: 1889  
Ion Ratio Lower Upper  
152 100  
150 149.8 112.7 169.1  
115 54.4 45.9 68.9

### Manual Integrations APPROVED



Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025




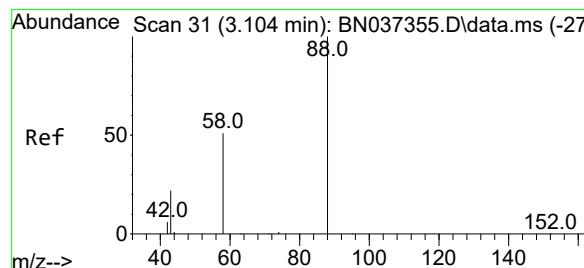
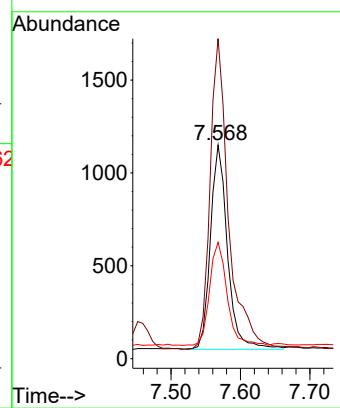
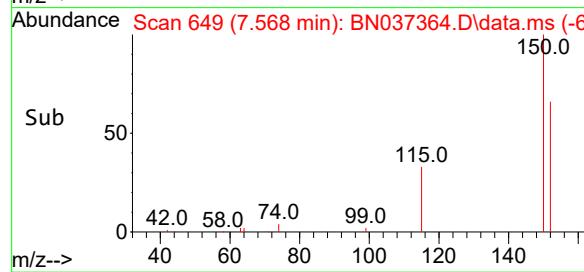


#2  
1,4-Dioxane  
Concen: 0.304 ng  
RT: 3.104 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

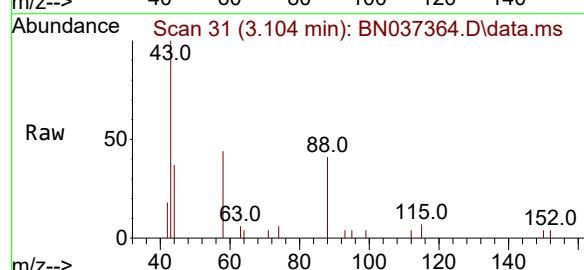

Tgt Ion: 88 Resp: 583  
Ion Ratio Lower Upper  
88 100  
43 101.0 21.0 31.6#  
58 59.7 38.0 57.0#

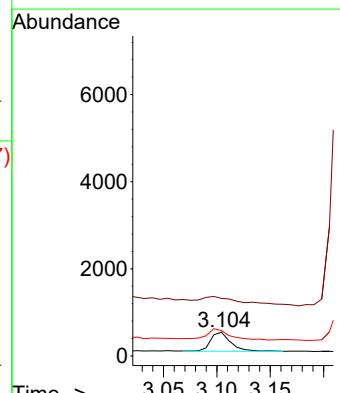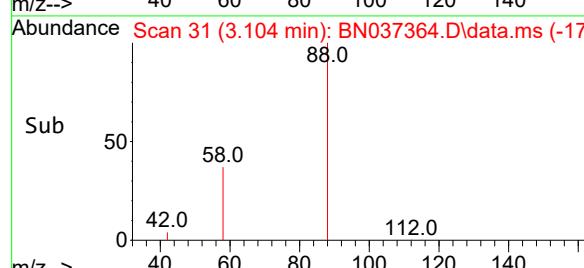



#3

n-Nitrosodimethylamine

Concen: 0.372 ng

RT: 3.415 min Scan# 7

Delta R.T. -0.007 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N


ClientSampleId :

PB168563BSD

### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

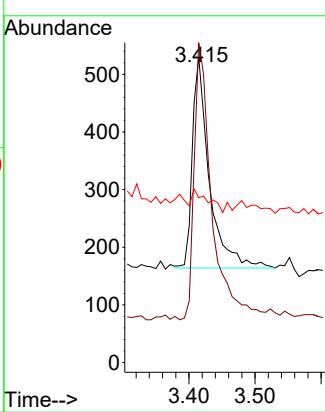

#4

2-Fluorophenol

Concen: 0.338 ng

RT: 5.170 min Scan# 317

Delta R.T. 0.007 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04


Tgt Ion:112 Resp: 1274







Ion Ratio Lower Upper

112 100

64 50.5 38.7 58.1

63 33.0 26.4 39.6

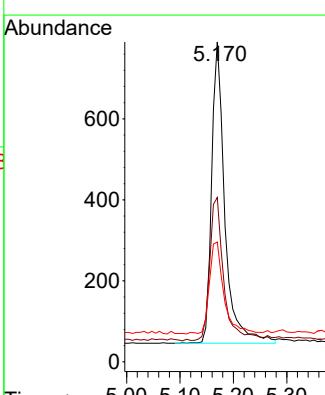


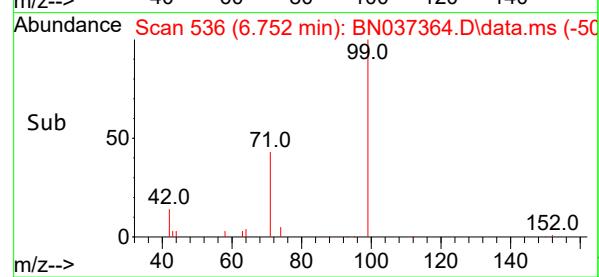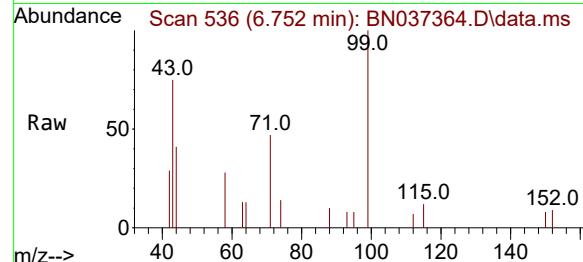

#5


Phenol-d6  
Concen: 0.346 ngRT: 6.752 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04Instrument :  
BNA\_N  
ClientSampleId :  
PB168563BSD




Tgt	Ion: 99	Resp:	1342
Ion Ratio	100	Lower	Upper
99	100		
42	21.1	19.8	29.8
71	42.0	42.6	64.0

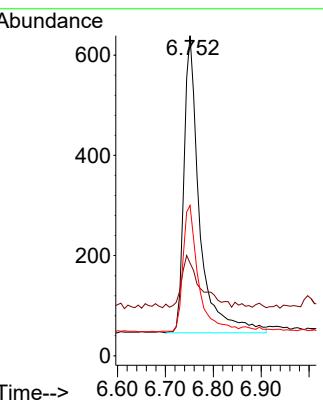**Manual Integrations  
APPROVED**Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

#6  
bis(2-Chloroethyl)ether  
Concen: 0.366 ng  
RT: 7.004 min Scan# 571  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt	Ion: 93	Resp:	1260
Ion Ratio	100	Lower	Upper
93	100		
63	66.8	53.2	79.8
95	32.7	27.3	40.9

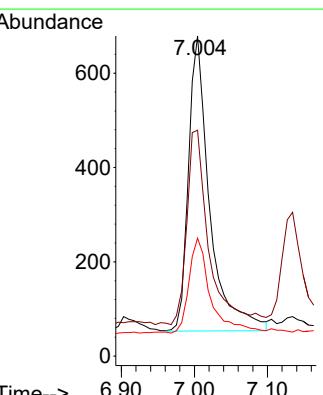



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.340 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N





ClientSampleId :

PB168563BSD

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#8

Nitrobenzene-d5

Concen: 0.388 ng


RT: 8.717 min Scan# 790




Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Tgt	Ion:	82	Resp:	1284
Ion	Ratio	Lower	Upper	
82	100			
128	42.9	42.5	63.7	#
54	41.7	43.2	64.8	#

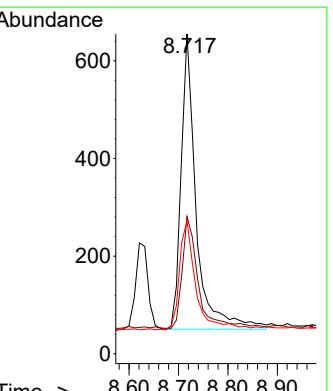



#9

Naphthalene

Concen: 0.372 ng

RT: 10.394 min Scan# 9

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N





ClientSampleId :

PB168563BSD

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

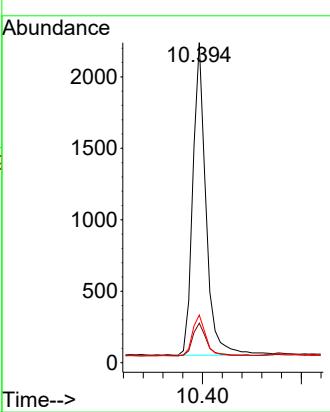

#10

Hexachlorobutadiene

Concen: 0.410 ng


RT: 10.682 min Scan# 974







Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Tgt	Ion:225	Resp:	1748
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	62.6	50.3	75.5

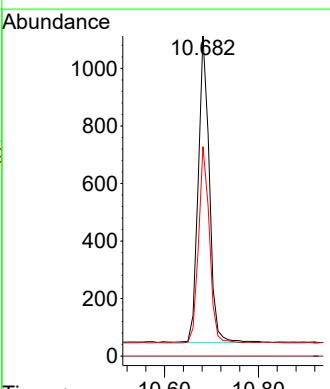



#11

2-Methylnaphthalene-d10  
Concen: 0.386 ng m

RT: 11.945 min Scan# 1138

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N


ClientSampleId :

PB168563BSD


**Manual Integrations  
APPROVED**




Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

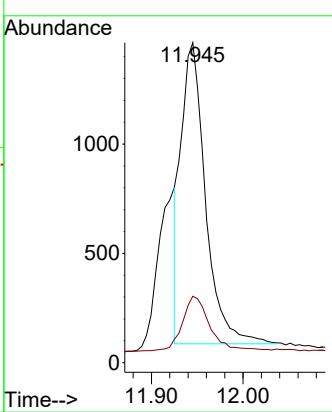

#12

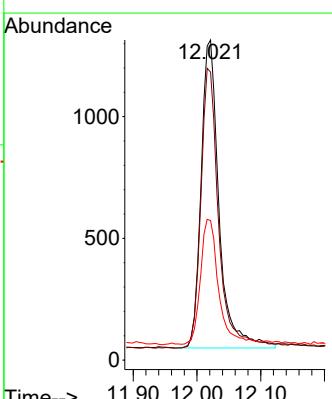2-Methylnaphthalene  
Concen: 0.328 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04Tgt Ion:142 Resp: 2474  
Ion Ratio Lower Upper  
142 100  
141 90.0 70.2 105.2  
115 43.6 43.0 64.4







#13  
 Acenaphthene-d10  
 Concen: 0.400 ng  
 RT: 14.213 min Scan# 1460  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


**Manual Integrations**  
**APPROVED**




Reviewed By :Rahul Chavli 06/23/2025  
 Supervised By :Jagrut Upadhyay 06/24/2025

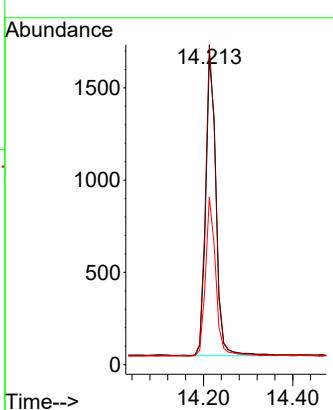

#14  
 2,4,6-Tribromophenol  
 Concen: 0.339 ng  
 RT: 15.718 min Scan# 1598  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Tgt Ion:330 Resp: 522  
 Ion Ratio Lower Upper  
 330 100  
 332 95.8 78.4 117.6  
 141 30.7 24.4 36.6









#15  
2-Fluorobiphenyl  
Concen: 0.397 ng  
RT: 12.838 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
ClientSampleId : PB168563BSD


1 Manual Integrations  
2 APPROVED







3 Reviewed By :Rahul Chavli 06/23/2025  
4 Supervised By :Jagrut Upadhyay 06/24/2025



#16  
Acenaphthylene  
Concen: 0.403 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:152 Resp: 4445  
Ion Ratio Lower Upper  
152 100  
151 19.4 16.6 24.8  
153 13.3 10.2 15.2

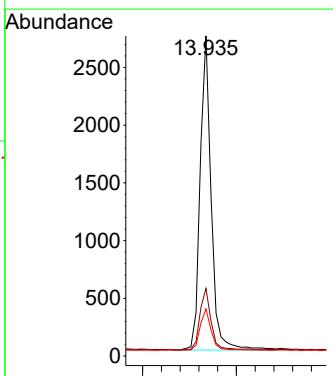

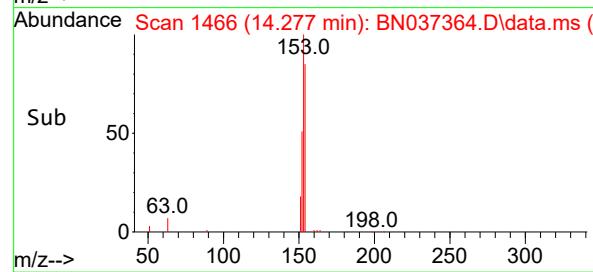

#17

Acenaphthene

Concen: 0.364 ng

RT: 14.277 min Scan# 1466

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N


ClientSampleId :

PB168563BSD

### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#18

Fluorene

Concen: 0.364 ng

RT: 15.271 min Scan# 1559

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04


Tgt Ion:166 Resp: 3709




Ion Ratio Lower Upper

166 100

165 100.1 79.5 119.3

167 13.8 10.7 16.1

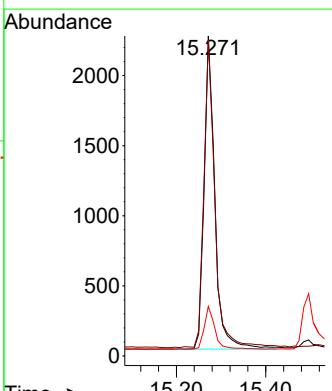



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.971 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N





ClientSampleId :

PB168563BSD

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

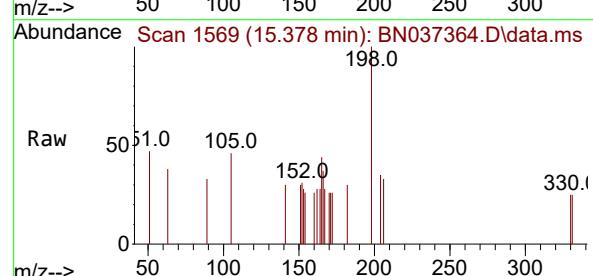

#20

4,6-Dinitro-2-methylphenol

Concen: 0.346 ng

RT: 15.378 min Scan# 1569

Delta R.T. 0.011 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04


Tgt Ion:198 Resp: 419


Ion Ratio Lower Upper

198 100

51 46.7 51.4 77.0#

105 46.2 45.5 68.3

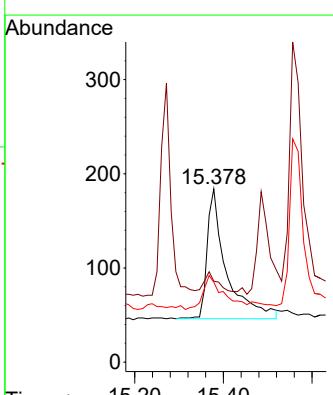


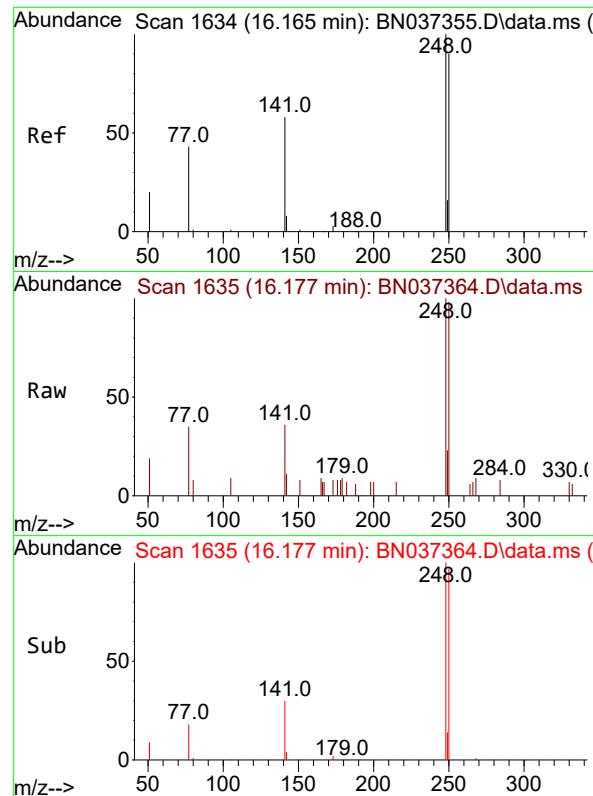


#21  
4-Bromophenyl-phenylether  
Concen: 0.375 ng  
RT: 16.177 min Scan# 1  
Delta R.T. 0.012 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
ClientSampleId : PB168563BSD


### Manual Integrations APPROVED




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

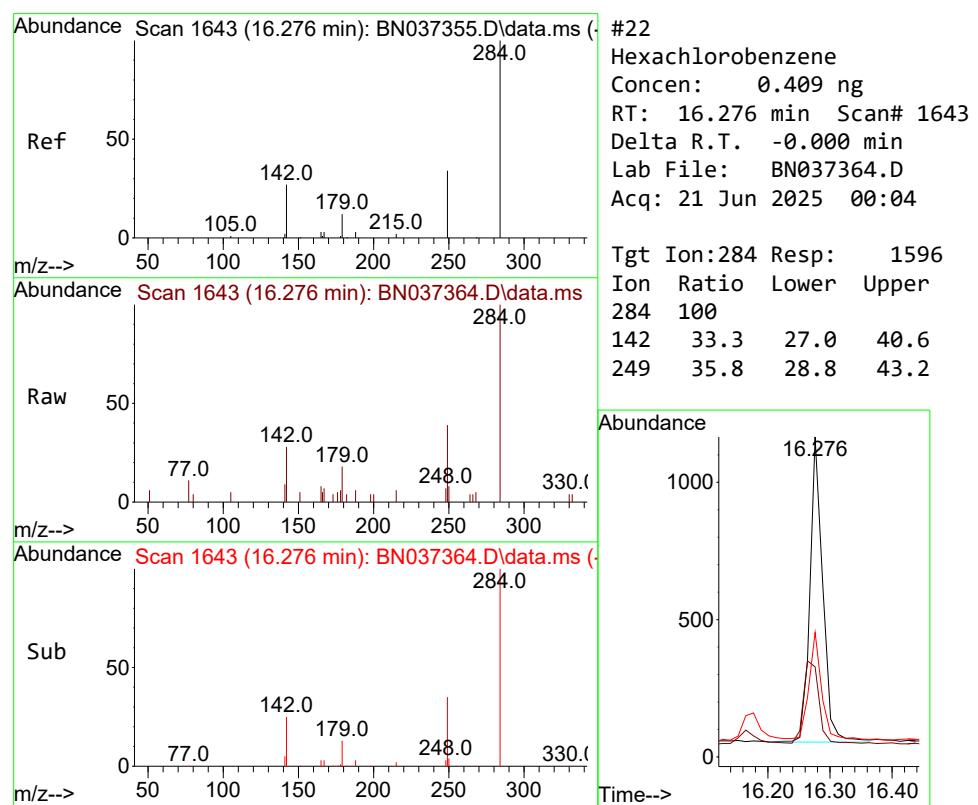

#22  
Hexachlorobenzene  
Concen: 0.409 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:284 Resp: 1596  
Ion Ratio Lower Upper  
284 100  
142 33.3 27.0 40.6  
249 35.8 28.8 43.2



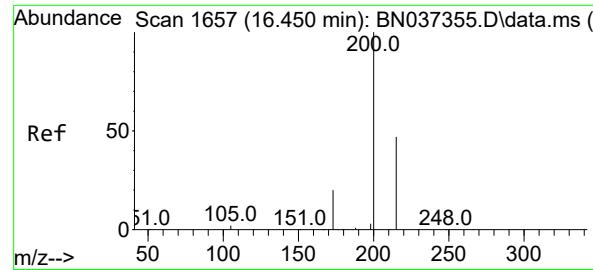

#23

Atrazine

Concen: 0.354 ng

RT: 16.450 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N




ClientSampleId :

PB168563BSD

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#24

Pentachlorophenol

Concen: 0.688 ng

RT: 16.624 min Scan# 1671

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04


Tgt Ion:266 Resp: 1337




Ion Ratio Lower Upper

266 100

264 62.5 50.3 75.5

268 65.4 55.3 82.9

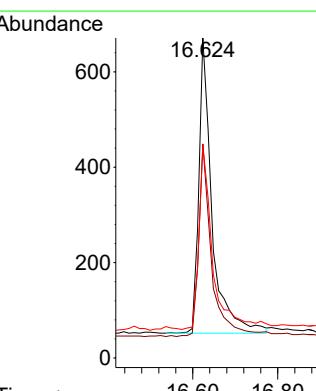



#25

Phenanthrene

Concen: 0.368 ng

RT: 17.009 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N





ClientSampleId :

PB168563BSD

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025



#26

Anthracene

Concen: 0.362 ng

RT: 17.108 min Scan# 1710

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04


Tgt Ion:178 Resp: 4862




Ion Ratio Lower Upper

178 100

176 18.5 14.7 22.1

179 15.5 13.0 19.6









#27  
Fluoranthene-d10  
Concen: 0.346 ng  
RT: 19.007 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Instrument :  
BNA\_N  
ClientSampleId :  
PB168563BSD


Manual Integrations  
**APPROVED**







Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025




#28  
Fluoranthene  
Concen: 0.339 ng  
RT: 19.035 min Scan# 1936  
Delta R.T. -0.005 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:202 Resp: 6244  
Ion Ratio Lower Upper  
202 100  
101 4.9 3.0 4.6#  
203 16.9 13.7 20.5

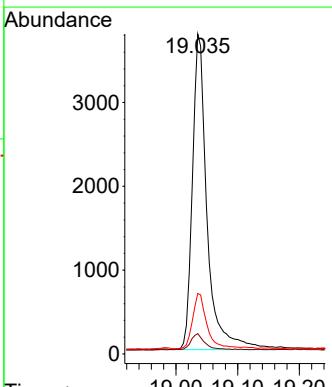







#29

Chrysene-d12  
Concen: 0.400 ngRT: 21.162 min Scan# 2  
Delta R.T. -0.009 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04Instrument :  
BNA\_N  
ClientSampleId :  
PB168563BSD**Manual Integrations  
APPROVED**Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

#30

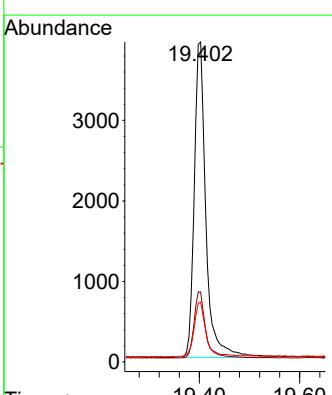Pyrene  
Concen: 0.373 ng  
RT: 19.402 min Scan# 2015  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04Tgt Ion:202 Resp: 6351  
Ion Ratio Lower Upper  
202 100  
200 20.7 16.8 25.2  
203 18.4 14.5 21.7







#31  
Terphenyl-d14  
Concen: 0.375 ng  
RT: 19.616 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
ClientSampleId : PB168563BSD


**Manual Integrations**  
**APPROVED**



Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

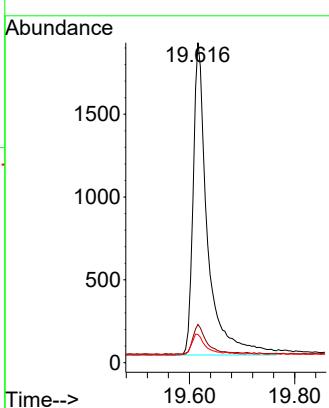

#32  
Benzo(a)anthracene  
Concen: 0.373 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:228 Resp: 5141  
Ion Ratio Lower Upper  
228 100  
226 28.4 23.0 34.4  
229 21.1 17.4 26.0

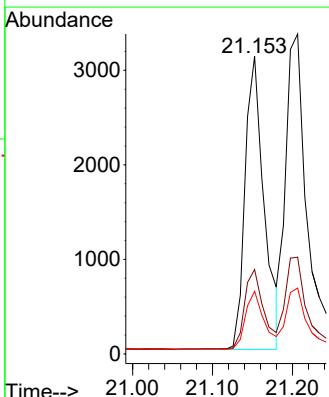

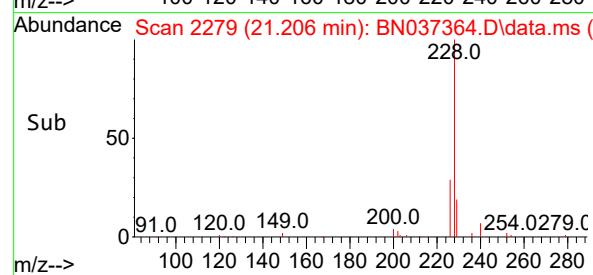

#33

Chrysene

Concen: 0.387 ng

RT: 21.206 min Scan# 2

Delta R.T. -0.000 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N





ClientSampleId :

PB168563BSD

**Manual Integrations  
APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

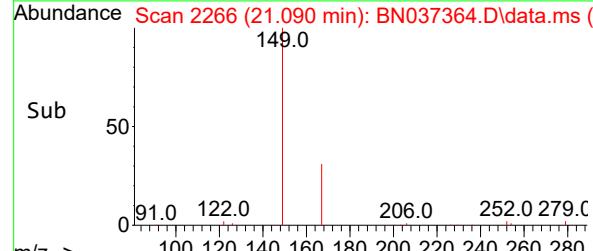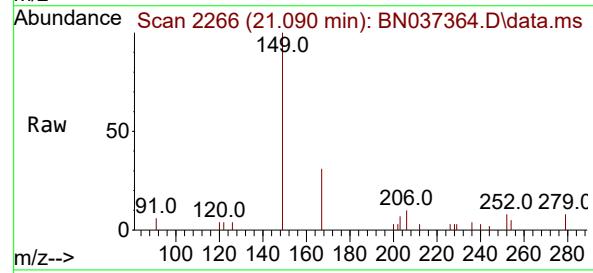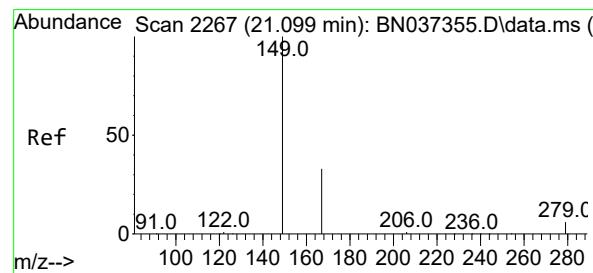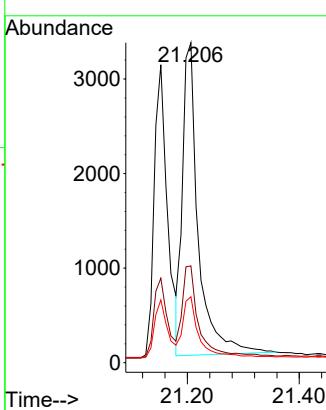

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.358 ng

RT: 21.090 min Scan# 2266

Delta R.T. -0.009 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04


Tgt Ion:149 Resp: 2023


Ion Ratio Lower Upper

149 100

167 32.9 24.6 37.0

279 9.0 6.5 9.7

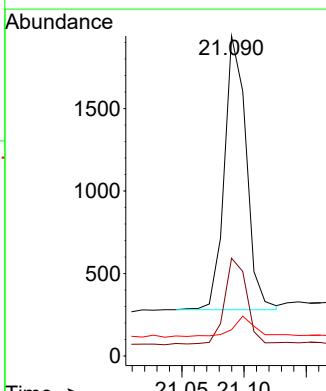


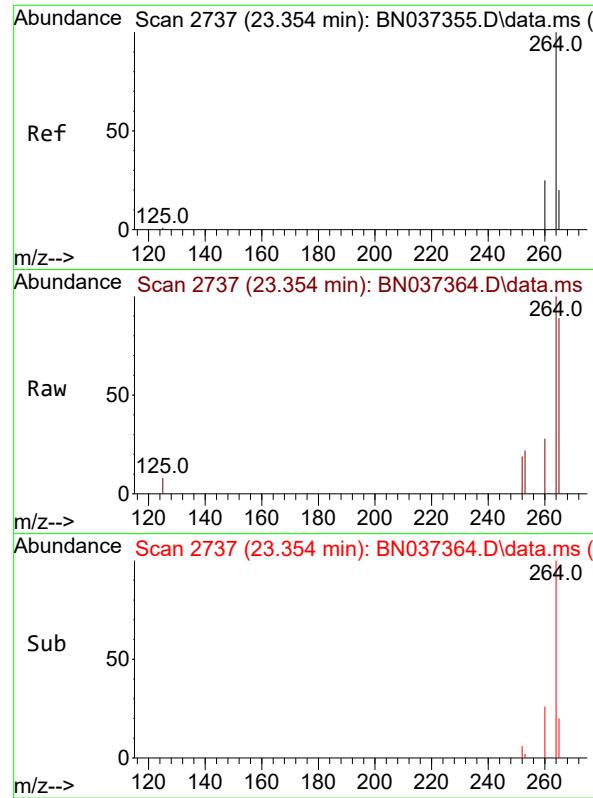


#35  
Perylene-d<sub>12</sub>  
Concen: 0.400 ng  
RT: 23.354 min Scan# 2  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
ClientSampleId : PB168563BSD


Manual Integrations  
APPROVED


Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

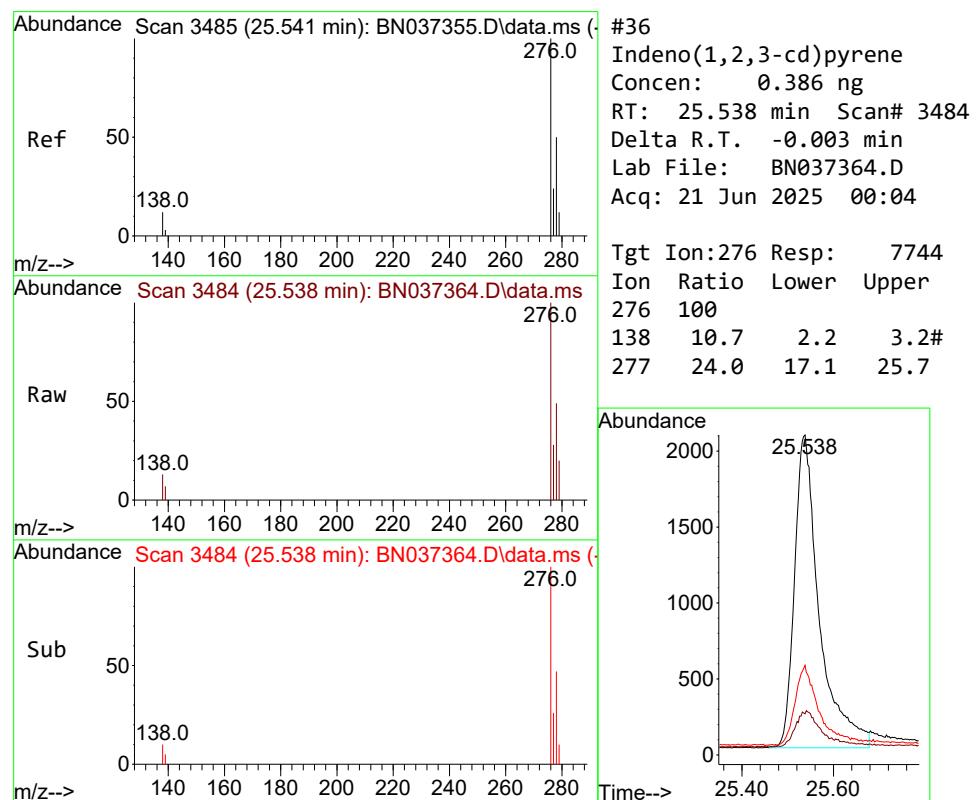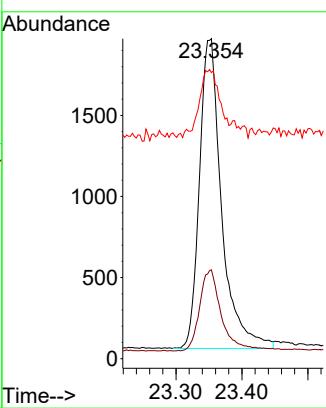

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.386 ng  
RT: 25.538 min Scan# 3484  
Delta R.T. -0.003 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:276 Resp: 7744  
Ion Ratio Lower Upper  
276 100  
138 10.7 2.2 3.2#  
277 24.0 17.1 25.7

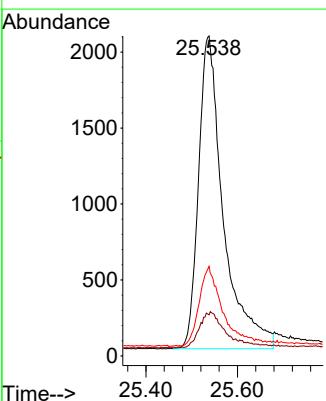


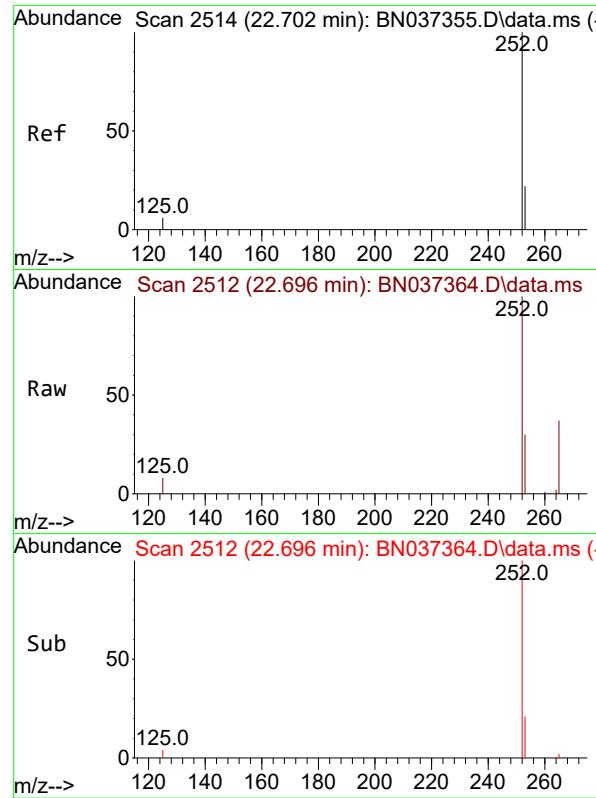


#37  
Benzo(b)fluoranthene  
Concen: 0.355 ng  
RT: 22.696 min Scan# 2  
Delta R.T. -0.006 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
ClientSampleId : PB168563BSD


### Manual Integrations APPROVED




Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

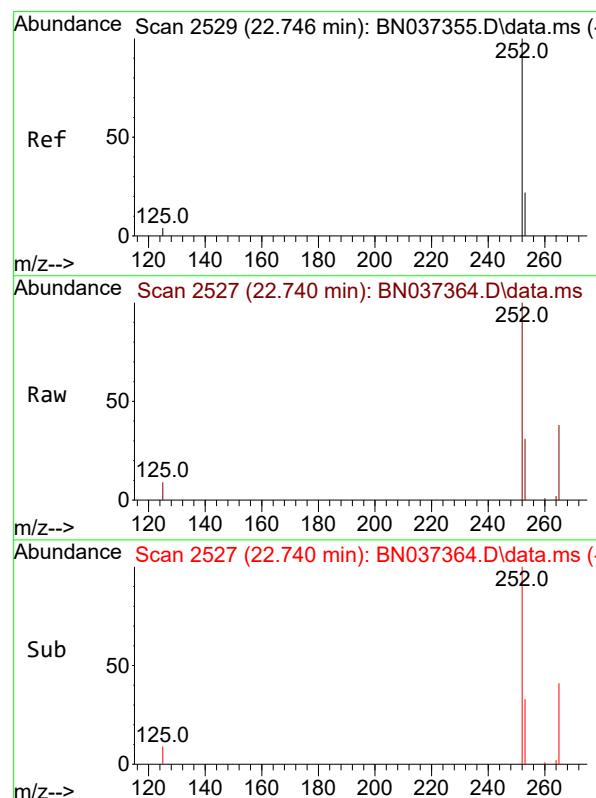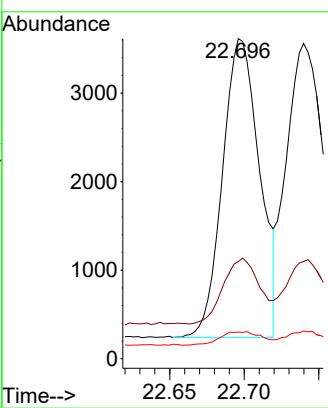

#38  
Benzo(k)fluoranthene  
Concen: 0.389 ng  
RT: 22.740 min Scan# 2527  
Delta R.T. -0.006 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:252 Resp: 6945  
Ion Ratio Lower Upper  
252 100  
253 30.8 26.7 40.1  
125 8.8 6.5 9.7

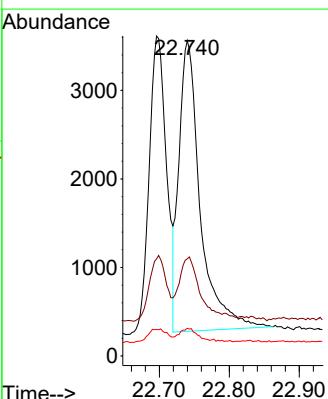

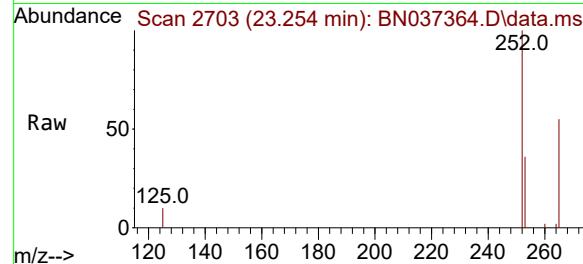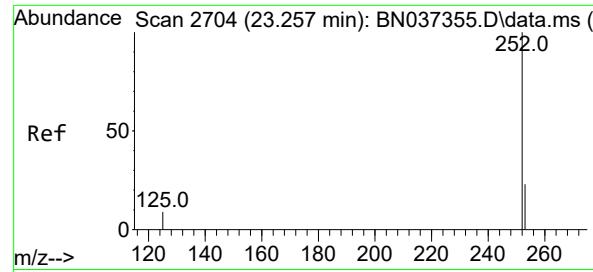

#39

Benzo(a)pyrene

Concen: 0.399 ng

RT: 23.254 min Scan# 2

Delta R.T. -0.003 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N




ClientSampleId :

PB168563BSD

**Manual Integrations**  
**APPROVED**

Reviewed By :Rahul Chavli 06/23/2025

Supervised By :Jagrut Upadhyay 06/24/2025

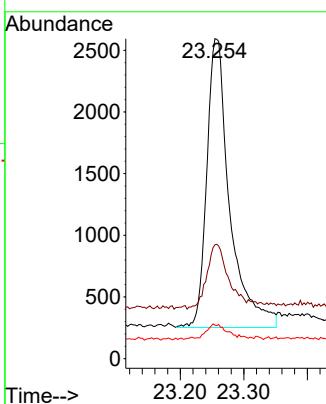

#40

Dibenzo(a,h)anthracene

Concen: 0.392 ng

RT: 25.552 min Scan# 3489


Delta R.T. -0.003 min


Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Tgt Ion:278 Resp: 5912

Ion	Ratio	Lower	Upper
278	100		
139	11.3	10.2	15.4
279	36.2	35.6	53.4

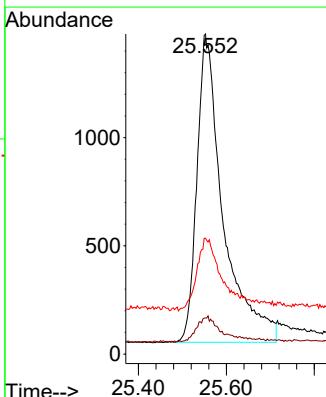

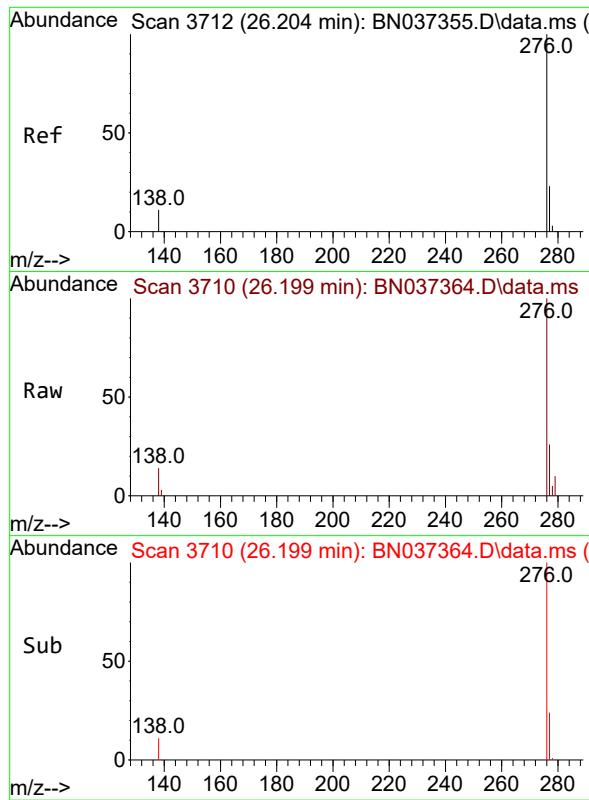


#41  
Benzo(g,h,i)perylene  
Concen: 0.393 ng  
RT: 26.199 min Scan# 3  
Delta R.T. -0.006 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
ClientSampleId : PB168563BSD

Tgt Ion:276 Resp: 7039  
Ion Ratio Lower Upper  
276 100  
277 26.4 22.7 34.1  
138 13.5 9.4 14.2

### Manual Integrations APPROVED

Reviewed By :Rahul Chavli 06/23/2025  
Supervised By :Jagrut Upadhyay 06/24/2025

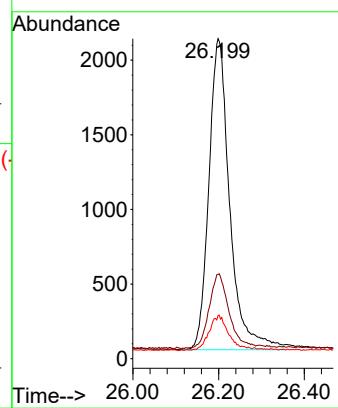

### Manual Integration Report

Sequence:	BN062125	Instrument	BNA_n
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
SSTDICCC0.4	BN037355.D	Benzo(b)fluoranthene	Rahul	6/23/2025 4:45:50 PM	Jagrut	6/24/2025 3:19:09 PM	Peak Integrated by Software
SSTDICV0.4	BN037360.D	Benzo(b)fluoranthene	Rahul	6/23/2025 4:45:53 PM	Jagrut	6/24/2025 3:19:11 PM	Peak Integrated by Software
PB168563BSD	BN037364.D	2-Methylnaphthalene-d10	Rahul	6/23/2025 4:45:56 PM	Jagrut	6/24/2025 3:19:14 PM	Peak Integrated by Software
SSTDCCC0.4	BN037365.D	Benzo(b)fluoranthene	Rahul	6/23/2025 4:45:59 PM	Jagrut	6/24/2025 3:19:16 PM	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

## Manual Integration Report

Sequence:	BN062625	Instrument	BNA_n
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
SSTDICC0.1	BN037386.D	Nitrobenzene-d5	Rahul	6/27/2025 12:01:52 PM	Jagrut	6/27/2025 12:02:28 PM	Peak Integrated by Software

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18

Instrument ID: BNA\_N

**Daily Analysis Runlog For Sequence/QCBatch ID # BN062125**

Review By	Rahul	Review On	6/24/2025 9:00:26 AM
Supervise By	Jagrut	Supervise On	6/24/2025 3:20:40 PM
SubDirectory	BN062125	HP Acquire Method	BNA_N, 8270_SIM HP Processing Method bn062125
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	SP6757 SP6781,SP6780,SP6779,SP6778,SP6777,SP6776,SP6775		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	SP6779 SP6740,1ul/100ul sample SP6768		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	DFTPP	BN037351.D	20 Jun 2025 15:00	RC/JU	Ok
2	SSTDCCC0.4	BN037352.D	20 Jun 2025 16:15	RC/JU	Not Ok
3	SSTDICC0.1	BN037353.D	20 Jun 2025 16:51	RC/JU	Ok
4	SSTDICC0.2	BN037354.D	20 Jun 2025 17:27	RC/JU	Ok
5	SSTDICCC0.4	BN037355.D	20 Jun 2025 18:03	RC/JU	Ok,M
6	SSTDICC0.8	BN037356.D	20 Jun 2025 18:39	RC/JU	Ok
7	SSTDICC1.6	BN037357.D	20 Jun 2025 19:15	RC/JU	Ok
8	SSTDICC3.2	BN037358.D	20 Jun 2025 19:51	RC/JU	Ok
9	SSTDICC5.0	BN037359.D	20 Jun 2025 20:27	RC/JU	Ok
10	SSTDICV0.4	BN037360.D	20 Jun 2025 21:39	RC/JU	Ok,M
11	PB168563BL	BN037361.D	20 Jun 2025 22:16	RC/JU	Ok
12	Q2377-01	BN037362.D	20 Jun 2025 22:52	RC/JU	Ok
13	PB168563BS	BN037363.D	20 Jun 2025 23:28	RC/JU	Ok
14	PB168563BSD	BN037364.D	21 Jun 2025 00:04	RC/JU	Ok,M
15	SSTDCCC0.4	BN037365.D	21 Jun 2025 01:17	RC/JU	Ok,M

M : Manual Integration

Instrument ID: BNA\_N

**Daily Analysis Runlog For Sequence/QCBatch ID # BN062625**

Review By	Rahul	Review On	6/27/2025 12:02:17 PM
Supervise By	Jagrut	Supervise On	6/27/2025 12:02:52 PM
SubDirectory	BN062625	HP Acquire Method	BNA_N, 8270_SIM HP Processing Method bn062625
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	SP6757 SP6842,SP6843,SP6844,SP6845,SP6846,SP6847,SP6848		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	SP6846 SP6740,1ul/100ul sample SP6768		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	DFTPP	BN037385.D	26 Jun 2025 10:01	RC/JU	Ok
2	SSTDICC0.1	BN037386.D	26 Jun 2025 10:41	RC/JU	Ok,M
3	SSTDICC0.2	BN037387.D	26 Jun 2025 11:17	RC/JU	Ok
4	SSTDICCC0.4	BN037388.D	26 Jun 2025 11:53	RC/JU	Ok
5	SSTDICC0.8	BN037389.D	26 Jun 2025 12:29	RC/JU	Ok
6	SSTDICC1.6	BN037390.D	26 Jun 2025 13:05	RC/JU	Ok
7	SSTDICC3.2	BN037391.D	26 Jun 2025 13:41	RC/JU	Ok
8	SSTDICC5.0	BN037392.D	26 Jun 2025 14:17	RC/JU	Ok
9	SSTDICV0.4	BN037393.D	26 Jun 2025 14:54	RC/JU	Ok
10	PB168563BL	BN037394.D	26 Jun 2025 15:30	RC/JU	Not Ok
11	Q2345-01	BN037395.D	26 Jun 2025 16:06	RC/JU	Ok,M
12	Q2345-13	BN037396.D	26 Jun 2025 16:42	RC/JU	Dilution
13	Q2345-14	BN037397.D	26 Jun 2025 17:18	RC/JU	Ok
14	Q2345-15	BN037398.D	26 Jun 2025 17:54	RC/JU	Ok
15	Q2345-16	BN037399.D	26 Jun 2025 18:30	RC/JU	Ok
16	Q2361-01	BN037400.D	26 Jun 2025 19:06	RC/JU	Ok
17	SSTDCCC0.4	BN037401.D	26 Jun 2025 19:42	RC/JU	Ok
18	DFTPP	BN037402.D	26 Jun 2025 20:19	RC/JU	Ok
19	SSTDCCC0.4	BN037403.D	26 Jun 2025 21:38	RC/JU	Ok
20	PB167430BL	BN037404.D	26 Jun 2025 22:14	RC/JU	Ok
21	Q2372-01	BN037405.D	26 Jun 2025 22:50	RC/JU	ReRun

Instrument ID: BNA\_N

**Daily Analysis Runlog For Sequence/QCBatch ID # BN062625**

Review By	Rahul	Review On	6/27/2025 12:02:17 PM
Supervise By	Jagrut	Supervise On	6/27/2025 12:02:52 PM
SubDirectory	BN062625	HP Acquire Method	BNA_N, 8270_SIM HP Processing Method bn062625
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	SP6757 SP6842,SP6843,SP6844,SP6845,SP6846,SP6847,SP6848		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	SP6846 SP6740,1ul/100ul sample SP6768		

22	Q2373-01	BN037406.D	26 Jun 2025 23:27	RC/JU	Not Ok
23	Q2373-02	BN037407.D	27 Jun 2025 00:03	RC/JU	Ok
24	Q2373-03	BN037408.D	27 Jun 2025 00:40	RC/JU	Ok
25	Q2374-01	BN037409.D	27 Jun 2025 01:16	RC/JU	Ok
26	Q2374-02	BN037410.D	27 Jun 2025 01:52	RC/JU	Ok
27	Q2374-03	BN037411.D	27 Jun 2025 02:29	RC/JU	Ok
28	Q2374-04	BN037412.D	27 Jun 2025 03:05	RC/JU	Ok
29	Q2375-01	BN037413.D	27 Jun 2025 03:41	RC/JU	Ok
30	Q2375-02	BN037414.D	27 Jun 2025 04:18	RC/JU	Ok
31	SSTDCCC0.4	BN037415.D	27 Jun 2025 04:54	RC/JU	Ok

M : Manual Integration

Instrument ID: BNA\_N

### Daily Analysis Runlog For Sequence/QCBatch ID # BN062125

Review By	Rahul	Review On	6/24/2025 9:00:26 AM	
Supervise By	Jagrut	Supervise On	6/24/2025 3:20:40 PM	
SubDirectory	BN062125	HP Acquire Method	BNA_N, 8270_HP Processing Method	bn062125
STD. NAME	STD REF.#			
Tune/Reschk Initial Calibration Stds	SP6757 SP6781,SP6780,SP6779,SP6778,SP6777,SP6776,SP6775			
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	SP6779 SP6740,1ul/100ul sample SP6768			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	DFTPP	DFTPP	BN037351.D	20 Jun 2025 15:00		RC/JU	Ok
2	SSTDCCC0.4	SSTDCCC0.4	BN037352.D	20 Jun 2025 16:15	A Fresh Calibration is required.	RC/JU	Not Ok
3	SSTDICC0.1	SSTDICC0.1	BN037353.D	20 Jun 2025 16:51		RC/JU	Ok
4	SSTDICC0.2	SSTDICC0.2	BN037354.D	20 Jun 2025 17:27		RC/JU	Ok
5	SSTDICCC0.4	SSTDICCC0.4	BN037355.D	20 Jun 2025 18:03	Calibration is good for DOD and nondod	RC/JU	Ok,M
6	SSTDICC0.8	SSTDICC0.8	BN037356.D	20 Jun 2025 18:39		RC/JU	Ok
7	SSTDICC1.6	SSTDICC1.6	BN037357.D	20 Jun 2025 19:15		RC/JU	Ok
8	SSTDICC3.2	SSTDICC3.2	BN037358.D	20 Jun 2025 19:51		RC/JU	Ok
9	SSTDICC5.0	SSTDICC5.0	BN037359.D	20 Jun 2025 20:27		RC/JU	Ok
10	SSTDICV0.4	ICVBN062125	BN037360.D	20 Jun 2025 21:39		RC/JU	Ok,M
11	PB168563BL	PB168563BL	BN037361.D	20 Jun 2025 22:16		RC/JU	Ok
12	Q2377-01	PW-B6-L66-061925	BN037362.D	20 Jun 2025 22:52		RC/JU	Ok
13	PB168563BS	PB168563BS	BN037363.D	20 Jun 2025 23:28	.	RC/JU	Ok
14	PB168563BSD	PB168563BSD	BN037364.D	21 Jun 2025 00:04		RC/JU	Ok,M
15	SSTDCCC0.4	SSTDCCC0.4EC	BN037365.D	21 Jun 2025 01:17		RC/JU	Ok,M

M : Manual Integration

Instrument ID: BNA\_N

### Daily Analysis Runlog For Sequence/QCBatch ID # BN062625

Review By	Rahul	Review On	6/27/2025 12:02:17 PM
Supervise By	Jagrut	Supervise On	6/27/2025 12:02:52 PM
SubDirectory	BN062625	HP Acquire Method	BNA_N, 8270_HP Processing Method bn062625
STD. NAME	STD REF.#		
Tune/Reschk	SP6757		
Initial Calibration Stds	SP6842,SP6843,SP6844,SP6845,SP6846,SP6847,SP6848		
CCC	SP6846		
Internal Standard/PEM	SP6740,1ul/100ul sample		
ICV/I.BLK	SP6768		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	DFTPP	DFTPP	BN037385.D	26 Jun 2025 10:01		RC/JU	Ok
2	SSTDICC0.1	SSTDICC0.1	BN037386.D	26 Jun 2025 10:41		RC/JU	Ok,M
3	SSTDICC0.2	SSTDICC0.2	BN037387.D	26 Jun 2025 11:17		RC/JU	Ok
4	SSTDICCC0.4	SSTDICCC0.4	BN037388.D	26 Jun 2025 11:53		RC/JU	Ok
5	SSTDICC0.8	SSTDICC0.8	BN037389.D	26 Jun 2025 12:29		RC/JU	Ok
6	SSTDICC1.6	SSTDICC1.6	BN037390.D	26 Jun 2025 13:05		RC/JU	Ok
7	SSTDICC3.2	SSTDICC3.2	BN037391.D	26 Jun 2025 13:41		RC/JU	Ok
8	SSTDICC5.0	SSTDICC5.0	BN037392.D	26 Jun 2025 14:17		RC/JU	Ok
9	SSTDICV0.4	ICVBN062625	BN037393.D	26 Jun 2025 14:54		RC/JU	Ok
10	PB168563BL	PB168563BL	BN037394.D	26 Jun 2025 15:30	Not Used	RC/JU	Not Ok
11	Q2345-01	EB02-20250616	BN037395.D	26 Jun 2025 16:06		RC/JU	Ok,M
12	Q2345-13	TT189D2-20250617	BN037396.D	26 Jun 2025 16:42	Need 2X dilution	RC/JU	Dilution
13	Q2345-14	TT150S1-20250617	BN037397.D	26 Jun 2025 17:18		RC/JU	Ok
14	Q2345-15	RW8-MW01D1-202506	BN037398.D	26 Jun 2025 17:54		RC/JU	Ok
15	Q2345-16	TT192D2-20250617	BN037399.D	26 Jun 2025 18:30		RC/JU	Ok
16	Q2361-01	TT205S1-20250617	BN037400.D	26 Jun 2025 19:06		RC/JU	Ok
17	SSTDCCC0.4	SSTDCCC0.4EC	BN037401.D	26 Jun 2025 19:42		RC/JU	Ok
18	DFTPP	DFTPP	BN037402.D	26 Jun 2025 20:19		RC/JU	Ok

Instrument ID: BNA\_N

### Daily Analysis Runlog For Sequence/QCBatch ID # BN062625

Review By	Rahul	Review On	6/27/2025 12:02:17 PM
Supervise By	Jagrut	Supervise On	6/27/2025 12:02:52 PM
SubDirectory	BN062625	HP Acquire Method	BNA_N, 8270_HP Processing Method bn062625
STD. NAME	STD REF.#		
Tune/Reschk	SP6757		
Initial Calibration Stds	SP6842,SP6843,SP6844,SP6845,SP6846,SP6847,SP6848		
CCC	SP6846		
Internal Standard/PEM	SP6740,1ul/100ul sample		
ICV/I.BLK	SP6768		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	SSTDCCC0.4	SSTDCCC0.4	BN037403.D	26 Jun 2025 21:38		RC/JU	Ok
20	PB167430BL	PB167430BL	BN037404.D	26 Jun 2025 22:14	Analyzed for contamination check	RC/JU	Ok
21	Q2372-01	GAV1W	BN037405.D	26 Jun 2025 22:50	Internal standard fail	RC/JU	ReRun
22	Q2373-01	RW5-SP100-20250619	BN037406.D	26 Jun 2025 23:27	Internal standard fail & Need 2X Dilution	RC/JU	Not Ok
23	Q2373-02	RW5-SP201-20250619	BN037407.D	27 Jun 2025 00:03		RC/JU	Ok
24	Q2373-03	RW5-SP303-20250619	BN037408.D	27 Jun 2025 00:40		RC/JU	Ok
25	Q2374-01	RW7-SP100-20250619	BN037409.D	27 Jun 2025 01:16		RC/JU	Ok
26	Q2374-02	RW7-SP201-20250619	BN037410.D	27 Jun 2025 01:52		RC/JU	Ok
27	Q2374-03	RW7-SP302-20250619	BN037411.D	27 Jun 2025 02:29		RC/JU	Ok
28	Q2374-04	RW7-SP303-20250619	BN037412.D	27 Jun 2025 03:05		RC/JU	Ok
29	Q2375-01	RW8-SP100-20250619	BN037413.D	27 Jun 2025 03:41		RC/JU	Ok
30	Q2375-02	RW8-SP303-20250619	BN037414.D	27 Jun 2025 04:18		RC/JU	Ok
31	SSTDCCC0.4	SSTDCCC0.4EC	BN037415.D	27 Jun 2025 04:54		RC/JU	Ok

M : Manual Integration

SOP ID:	M3510C,3580A-Extraction SVOC-21		
Clean Up SOP #:	N/A	Extraction Start Date :	06/20/2025
Matrix :	Water	Extraction Start Time :	09:32
Weigh By:	N/A	Extraction End Date :	06/20/2025
Balance check:	N/A	Extraction End Time :	16:30
Balance ID:	N/A	pH Meter ID:	N/A
pH Strip Lot#:	E3880	Hood ID:	4,5,6,7
Extraction Method:	<input checked="" type="checkbox"/> Separatory Funnel <input type="checkbox"/> Continous Liquid/Liquid <input type="checkbox"/> Sonication <input type="checkbox"/> Waste Dilution <input type="checkbox"/> Soxhlet		

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	0.4 PPM	SP6756
Surrogate	1.0ML	0.4 PPM	SP6831
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3943
Baked Na2SO4	N/A	EP2622
10N NaOH	N/A	EP2609
H2SO4 1:1	N/A	EP2610
N/A	N/A	N/A

**Extraction Conformance/Non-Conformance Comments:**

1.5 ML Vial lot# 2210443. pH Adjusted<2 with 1:1 H2SO4 &>11 with 10 N NaOH. Q2373,Q2374,Q2375 & Q2377 all samples added at 12:03 P.M.


KD Bath ID: WATER BATH-1,2 Envap ID: NEVAP-02  
 KD Bath Temperature: 60 °C Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
6/20/25	RS (BLT lab)	RCS/voC
16:35	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction SVOC-21

Concentration Date: 06/20/2025

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB168563BL	SBLK563	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			SEP-1
PB168563BS	SLCS563	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			2
PB168563BS D	SLCSD563	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			3
Q2345-01	EB02-20250616	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1	C		4
Q2345-13	TT189D2-2050617	SVOC-SIMGrou p1	990	6	RUPESH	ritesh	1	C		5
Q2345-14	TT150S1-2050617	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1	C		6
Q2345-15	RW8-MW01D1-20250617	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1	C		7
Q2345-16	TT192D2-2050617	SVOC-SIMGrou p1	990	6	RUPESH	ritesh	1	C		8
Q2361-01	TT205S1-20250617	SVOC-SIMGrou p1	990	6	RUPESH	ritesh	1	C		9
Q2372-01	GAV1W	SVOC-SIMGrou p1	970	6	RUPESH	ritesh	1	E		10
Q2373-01	RW5-SP100-20250619	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			11
Q2373-02	RW5-SP201-20250619	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			12
Q2373-03	RW5-SP303-20250619	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			13
Q2374-01	RW7-SP100-20250619	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			14
Q2374-02	RW7-SP201-20250619	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			15
Q2374-03	RW7-SP302-20250619	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			16
Q2374-04	RW7-SP303-20250619	SVOC-SIMGrou p1	1000	6	RUPESH	ritesh	1			SEP-1
Q2375-01	RW8-SP100-20250619	SVOC-SIMGrou p1	990	6	RUPESH	ritesh	1	D		2
Q2375-02	RW8-SP303-20250619	SVOC-SIMGrou p1	990	6	RUPESH	ritesh	1	D		3
Q2377-01	PW-B6-L66-061925	SVOC-SIMGrou p1	980	6	RUPESH	ritesh	1	D		4

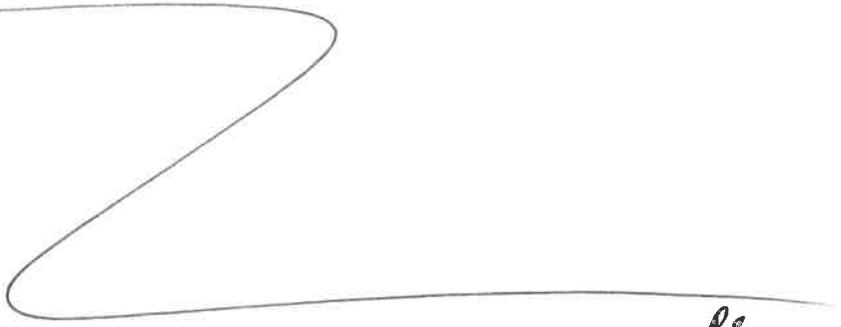  
 RS  
 6/20

\* Extracts relinquished on the same date as received.

168567  
9-32

## WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q2361

WorkList ID : 190289

Department : Extraction

Date : 06-20-2025 09:26:55

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2345-01	EB02-20250616	Water	SVOC-SIMGroup1	Cool 4 deg C	AECO15	D61	06/16/2025	8270-Modified
Q2345-13	TT189D2-2050617	Water	SVOC-SIMGroup1	Cool 4 deg C	AECO15	D61	06/17/2025	8270-Modified
Q2345-14	TT150S1-2050617	Water	SVOC-SIMGroup1	Cool 4 deg C	AECO15	D61	06/17/2025	8270-Modified
Q2345-15	RW8-MW01D1-20250617	Water	SVOC-SIMGroup1	Cool 4 deg C	AECO15	D61	06/17/2025	8270-Modified
Q2345-16	TT192D2-2050617	Water	SVOC-SIMGroup1	Cool 4 deg C	AECO15	D61	06/17/2025	8270-Modified
Q2361-01	TT205S1-20250617	Water	SVOC-SIMGroup1	Cool 4 deg C	AECO15	D51	06/17/2025	8270-Modified
Q2372-01	GAV1W	Water	SVOC-SIMGroup1	Cool 4 deg C	GENV01	D51	06/19/2025	8270-Modified

Date/Time 6/20/25 9:27  
Raw Sample Received by: RS (ECT (g-b))  
Raw Sample Relinquished by: QF8  
Q2375-SVOC-SIMGroup1

Date/Time 6/20/25 10:10  
Raw Sample Received by: CF8  
Raw Sample Relinquished by: RS (ECT (g-b))  
578 of 767

1695b7

## WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q2373

WorkList ID : 190300

Department : Extraction

Date : 06-20-2025 12:02:27

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2373-01	RW5-SP100-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2373-02	RW5-SP201-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2373-03	RW5-SP303-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2374-01	RW7-SP100-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2374-02	RW7-SP201-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2374-03	RW7-SP302-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2374-04	RW7-SP303-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2375-01	RW8-SP100-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2375-02	RW8-SP303-20250619	Water	SVOC-SIMGroup1	Cool 4 deg C	TETR06	D51	06/19/2025	8270-Modified
Q2377-01	PW-B6-L66-061925	Water	SVOC-SIMGroup1	Cool 4 deg C	JACO05	D51	06/19/2025	8270-Modified

Date/Time 6/20/25 12:03  
 Raw Sample Received by: RS (Ext (lab))  
 Raw Sample Relinquished by: OF S

Date/Time 6/20/25 12:35  
 Raw Sample Received by: OF S  
 Raw Sample Relinquished by: RS (Ext (lab))

## Prep Standard - Chemical Standard Summary

**Order ID :** Q2375

**Test :** SVOC-SIMGroup1

**Prepbatch ID :** PB168563,

**Sequence ID/Qc Batch ID:** BN062125, BN062625,

**Standard ID :**

EP2609,EP2610,EP2622,SP6740,SP6756,SP6757,SP6767,SP6768,SP6774,SP6775,SP6776,SP6777,SP6778,SP6779,SP6780,SP6781,SP6830,SP6831,SP6841,SP6842,SP6843,SP6844,SP6845,SP6846,SP6847,SP6848,

**Chemical ID :**

1ul/100ul  
sample,E3551,E3657,E3874,E3902,E3904,E3926,E3940,E3942,E3943,M6157,S10104,S10105,S11496,S11650,S11788,S11828,S11832,S12115,S12195,S12216,S12271,S12273,S12486,S12533,S12577,S12651,S12670,S12792,S12974,S13058,W3112,

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1874	10 N SODIUM HYDROXIDE SOLN	<a href="#">EP2609</a>	05/07/2025	11/07/2025	RUPESHKUMA R SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/07/2025

FROM 1000.00000ml of W3112 + 400.00000gram of E3657 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	<a href="#">EP2610</a>	05/07/2025	11/07/2025	RUPESHKUMA R SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 05/07/2025

FROM 1000.00000ml of M6157 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2622</a>	06/13/2025	12/04/2025	RUPESHKUMA R SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 06/16/2025

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3493	Internal Standard 0.4 PPM	<a href="#">SP6740</a>	02/13/2025	07/30/2025	Rahul Chavli	None	None	Yogesh Patel 02/28/2025

FROM 0.10000ml of S12651 + 4.90000ml of E3874 = Final Quantity: 5.000 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3492	8270-SIM-Spike 0.4 PPM	<a href="#">SP6756</a>	03/24/2025	07/29/2025	Rahul Chavli	None	None	mohammad ahmed 04/07/2025

**FROM** 0.00160ml of S11650 + 0.02000ml of S11788 + 0.04000ml of S12486 + 0.04000ml of S12533 + 0.04000ml of S12974 + 99.85840ml of E3902 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3895	50 ug/ml DFTPP 8270E	<a href="#">SP6757</a>	03/31/2025	09/30/2025	Rahul Chavli	None	None	Jagrut Upadhyay 04/01/2025

**FROM** 1.00000ml of S12577 + 19.00000ml of E3904 = Final Quantity: 20.000 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3355	8270-SIM MDL-3.2PPM CALIBRATION STOCK SOL- 2ND	<a href="#">SP6767</a>	04/10/2025	07/24/2025	Jagrut Upadhyay	None	None	Sohil Jodhani 04/16/2025
<u>SOURCE</u>								
<u>FROM</u> 0.00630ml of S12195 + 0.01280ml of S12216 + 0.03200ml of S11788 + 0.03200ml of S11832 + 0.06400ml of S12486 + 0.06400ml of S12533 + 0.06400ml of S12974 + 19.72490ml of E3926 = Final Quantity: 20.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3356	8270-SIM MDL-0.4PPM CALIBRATION SOL ICV-2ND	<a href="#">SP6768</a>	04/10/2025	07/24/2025	Jagrut Upadhyay	None	None	Sohil Jodhani 04/16/2025
<u>SOURCE</u>								
<u>FROM</u> 0.87500ml of E3926 + 0.01000ml of SP6740 + 0.12500ml of SP6767 = Final Quantity: 1.010 ml								

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3339	8270 sim calibration stock 10ppm (CPI)	<a href="#">SP6774</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.03350ml of S10104 + 0.05000ml of S11496 + 0.12500ml of S11832 + 0.12500ml of S12115 + 0.25000ml of S12271 + 0.25000ml of S12792 + 24.16650ml of E3926 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3361	8270-SIM MDL-5PPM CALIBRATION SOLUTION	<a href="#">SP6775</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.50000ml of E3926 + 0.01000ml of SP6740 + 0.50000ml of SP6774 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3341	8270-SIM MDL-3.2PPM CALIBRATION SOLUTION	<a href="#">SP6776</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.68000ml of E3926 + 0.01000ml of SP6740 + 0.32000ml of SP6774 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3344	8270-SIM MDL-1.6PPM CALIBRATION SOLUTION	<a href="#">SP6777</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.84000ml of E3926 + 0.01000ml of SP6740 + 0.16000ml of SP6774 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3342	8270-SIM MDL-0.8PPM CALIBRATION SOLUTION	<a href="#">SP6778</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.92000ml of E3926 + 0.01000ml of SP6740 + 0.08000ml of SP6774 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3343	8270-SIM MDL-0.4PPM CALIBRATION SOLUTION	<a href="#">SP6779</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.96000ml of E3926 + 0.01000ml of SP6740 + 0.04000ml of SP6774 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3345	8270-SIM MDL-0.2PPM CALIBRATION SOLUTION	<a href="#">SP6780</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.50000ml of E3926 + 0.01000ml of SP6740 + 0.50000ml of SP6779 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3346	8270-SIM MDL-0.1PPM CALIBRATION SOLUTION	<a href="#">SP6781</a>	04/28/2025	06/21/2025	Jagrut Upadhyay	None	None	Rahul Chavli 05/16/2025

FROM 0.75000ml of E3926 + 0.01000ml of SP6740 + 0.25000ml of SP6779 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3493	Internal Standard 0.4 PPM	<a href="#">SP6830</a>	06/17/2025	12/13/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/19/2025

FROM 0.10000ml of S12670 + 4.90000ml of E3942 = Final Quantity: 5.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3491	8270-SIM-Surrogate 0.4 PPM	<a href="#">SP6831</a>	06/18/2025	09/18/2025	Rahul Chavli	None	None	Jagrut Upadhyay 06/18/2025

FROM 0.00800ml of S12195 + 0.01600ml of S12216 + 0.04000ml of S11828 + 199.93600ml of E3940 = Final Quantity: 200.000 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3339	8270 sim calibration stock 10ppm (CPI)	<a href="#">SP6841</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.03350ml of S10105 + 0.05000ml of S11496 + 0.12500ml of S11828 + 0.12500ml of S12115 + 0.25000ml of S12273 + 0.25000ml of S13058 + 24.16650ml of E3943 = Final Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3361	8270-SIM MDL-5PPM CALIBRATION SOLUTION	<a href="#">SP6842</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.50000ml of E3943 + 0.01000ml of SP6830 + 0.50000ml of SP6841 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3341	8270-SIM MDL-3.2PPM CALIBRATION SOLUTION	<a href="#">SP6843</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.68000ml of E3943 + 0.01000ml of SP6830 + 0.32000ml of SP6841 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3344	8270-SIM MDL-1.6PPM CALIBRATION SOLUTION	<a href="#">SP6844</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.84000ml of E3943 + 0.01000ml of SP6830 + 0.16000ml of SP6841 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3342	8270-SIM MDL-0.8PPM CALIBRATION SOLUTION	<a href="#">SP6845</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.92000ml of E3943 + 0.01000ml of SP6830 + 0.08000ml of SP6841 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3343	8270-SIM MDL-0.4PPM CALIBRATION SOLUTION	<a href="#">SP6846</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.96000ml of E3943 + 0.01000ml of SP6830 + 0.04000ml of SP6841 = Final Quantity: 1.010 ml

## SVOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3345	8270-SIM MDL-0.2PPM CALIBRATION SOLUTION	<a href="#">SP6847</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.50000ml of E3943 + 0.01000ml of SP6830 + 0.50000ml of SP6846 = Final Quantity: 1.010 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3346	8270-SIM MDL-0.1PPM CALIBRATION SOLUTION	<a href="#">SP6848</a>	06/25/2025	10/28/2025	Jagrut Upadhyay	None	None	Rahul Chavli 06/25/2025

FROM 0.75000ml of E3943 + 0.01000ml of SP6830 + 0.25000ml of SP6846 = Final Quantity: 1.010 ml

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	12/04/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551
PCI Scientific Supply, Inc.	PC19510-5 / Sodium Hydroxide Pellets 2.5 Kg, Pk of 4	23B1556310	12/31/2025	12/04/2023 / Rajesh	12/01/2023 / Rajesh	E3657
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A0262002	07/30/2025	01/30/2025 / Rajesh	01/20/2025 / Rajesh	E3874
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	09/18/2025	03/18/2025 / RUPESH	02/12/2025 / RUPESH	E3902
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24K1762005	01/07/2026	03/13/2025 /	12/27/2024 / RUPESH	E3904
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A0262002	10/08/2025	04/08/2025 / Rajesh	02/07/2025 / Rajesh	E3926

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	12/11/2025	06/11/2025 / Rajesh	06/04/2025 / Rajesh	E3940
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A2862010	12/13/2025	06/13/2025 / Rajesh	02/28/2025 / Rajesh	E3942
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	25A2862010	12/13/2025	06/13/2025 / Rajesh	02/28/2025 / Rajesh	E3943
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	24i1262013	11/07/2025	05/07/2025 / RUPESH	02/18/2025 / Mohan	M6157
CPI International	Z-112090-04 / CLP Acid Surrogate Solution, 7500 mg/L, 1ml	440246	07/30/2025	01/30/2025 / anahy	12/09/2021 / Christian	S10104
CPI International	Z-112090-04 / CLP Acid Surrogate Solution, 7500 mg/L, 1ml	440246	12/19/2025	06/19/2025 / Jagrut	12/09/2021 / Christian	S10105

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110094-02 / CLP Base/Neutral Surrogate Solution, 5000 mg/L, 1ml	506889	10/28/2025	04/28/2025 / Jagrut	08/11/2023 / Yogesh	S11496
Restek	555872 / Custom Standard, pentachlorophenol Std [CS 5328-5]	A0201728	07/29/2025	01/29/2025 / anahy	11/09/2023 / Yogesh	S11650
Restek	31853 / 1,4-Dioxane, 2000 ug/ml , Solvent: Methylene Chloride	A0196453	09/10/2025	03/10/2025 / anahy	11/21/2023 / Rahul	S11788
Restek	33913 / SOM01.0 SIM Analysis Standard (Surrogate), 2000 PPM	A0201976	12/09/2025	06/09/2025 / Jagrut	11/21/2023 / rahul	S11828
Restek	33913 / SOM01.0 SIM Analysis Standard (Surrogate), 2000 PPM	A0201976	07/24/2025	01/24/2025 / anahy	11/21/2023 / rahul	S11832
CPI International	z-010223-01 / 1,4-Dioxane Solution, 2,000mg/L, 1ml	454157	10/28/2025	04/28/2025 / Jagrut	03/08/2024 / Rahul	S12115

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31087 / Acid Surrogate 10,000ug/ml,methanol,5ml/ ampul	A0206206	09/18/2025	03/18/2025 / anahy	03/15/2024 / Rahul	S12195
Restek	31086 / Base Neutral Surrogate 5000ug/ml,CH2Cl2,5ml	A0206381	09/18/2025	03/18/2025 / anahy	03/15/2024 / Rahul	S12216
CPI International	z-110381-01 / 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1ml	520963	10/28/2025	04/28/2025 / Jagrut	05/24/2024 / Rahul	S12271
CPI International	z-110381-01 / 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1ml	520963	12/25/2025	06/25/2025 / Jagrut	05/24/2024 / Rahul	S12273
Restek	555223 / Custom 8270 Plus Std #1 [2nd lot at \$100 per ampul if requested - contact ARM with Request]	A0214021	09/10/2025	03/10/2025 / anahy	07/23/2024 / RAHUL	S12486
[CS 4978-1]						
Restek	555224 / Custom 8270 Plus Std #2 [2nd lot at \$85 per ampul if requested - contact ARM with Request]	A0214017	09/10/2025	03/10/2025 / anahy	07/23/2024 / RAHUL	S12533
[CS 4978-2]						

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31615 / SV Mixture, GC/MS Tuning Mixture, CH <sub>2</sub> Cl <sub>2</sub> , 1mL,	A0212955	06/30/2027	03/31/2025 / Rahul	08/01/2024 / Rahul	S12577
Restek	31206 / SV Mix, CLP method, Internal Std, 2000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> , 1mL	A0212266	08/07/2025	02/07/2025 / anahy	09/20/2024 / anahy	S12651
Restek	31206 / SV Mix, CLP method, Internal Std, 2000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> , 1mL	A0212266	12/16/2025	06/16/2025 / anahy	09/20/2024 / anahy	S12670
CPI International	Z-110816-01 / Custom 8270 Mix, 4-79, 1000 mg/L, 1 mL, (Maximum Expiration: 180 Days)	414127	06/21/2025	04/28/2025 / Jagrut	05/24/2024 / Rahul	S12792
Restek	31850 / 8270 SV Mix, 8270 Mega Mix 1mL, 1000ug/mL, CH <sub>2</sub> Cl <sub>2</sub> [New Solvent 100% CH <sub>2</sub> Cl <sub>2</sub> ]	A0219438	09/10/2025	03/10/2025 / anahy	12/11/2024 / anahy	S12974
CPI International	Z-110816-01 / Custom 8270 Mix, 4-79, 1000 mg/L, 1 mL, (Maximum Expiration: 180 Days)	531243	12/25/2025	06/25/2025 / Jagrut	01/16/2025 / anahy	S13058

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18



5580 Skylane Blvd  
Santa Rosa, CA 95403

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage: Solvent: Exp. Date: Description:  
Z-112090 440246  $\leq -10^{\circ}\text{C}$  Methylene Chloride 2/16/2026 CLP Acid Surrogate Solution, 7,500 mg/L, 1 mL  
-04

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
2-chlorophenol-d <sub>4</sub>	93951-73-6	99.3	248.12.7P	7487 $\pm$ 17.2
2-fluorophenol	367-12-4	99.8	10.7.3.3P	7513 $\pm$ 17.26
phenol-d <sub>6</sub>	13127-88-3	99.9	949.120.8P	7481 $\pm$ 17.19
2,4,6-tribromophenol	118-79-6	99.8	12.1.6P	7469 $\pm$ 17.17

Received on

02/25/21

by  
CG

S9236  
+0

S9240

\*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

Certified By:

Erica Castiglione  
Chemist



5580 Skylane Blvd  
Santa Rosa, CA 95403

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage: Solvent: Exp. Date: Description:  
Z-112090 440246  $\leq -10^{\circ}\text{C}$  Methylene Chloride 2/16/2026 CLP Acid Surrogate Solution, 7,500 mg/L, 1 mL  
-04

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
2-chlorophenol-d <sub>4</sub>	93951-73-6	99.3	248.12.7P	7487 $\pm$ 17.2
2-fluorophenol	367-12-4	99.8	10.7.3.3P	7513 $\pm$ 17.26
phenol-d <sub>6</sub>	13127-88-3	99.9	949.120.8P	7481 $\pm$ 17.19
2,4,6-tribromophenol	118-79-6	99.8	12.1.6P	7469 $\pm$ 17.17

Received on

02/25/21

by  
CG

S9236  
+0

S9240

\*Not a certified value

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

Certified By:



Erica Castiglione  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.



PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreing matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

### COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/29/23 [E 3551]

RC-02-01, Ed. 3



# Certificate of Analysis

## Sodium Hydroxide (Pellets)

**Material:** 0583  
**Grade:** ACS GRADE  
**Batch Number:** 23B1556310

Chemical Formula: NaOH  
Molecular Weight: 40  
CAS #: 1310-73-2  
Appearance:  
Pellets

Manufacture Date: 12/14/2022  
Expiration Date: 12/31/2025  
Storage: Room Temperature

TEST	SPECIFICATION	ANALYSIS	DISPOSITION
Calcium	<= 0.005 %	<0.005 %	PASS
Chloride	<= 0.005 %	0.002 %	PASS
Heavy Metals	<= 0.002 %	<0.002 %	PASS
Iron	<= 0.001 %	<0.001 %	PASS
Magnesium	<= 0.002 %	<0.002 %	PASS
Mercury	<= 0.1 ppm	<0.1 ppm	PASS
Nickel	<= 0.001 %	<0.001 %	PASS
Nitrogen Compounds	<= 0.001 %	<0.001 %	PASS
Phosphate	<= 0.001 %	<0.001 %	PASS
Potassium	<= 0.02 %	<0.02 %	PASS
Purity	>= 97.0 %	99.2 %	PASS
Sodium Carbonate	<= 1.0 %	0.5 %	PASS
Sulfate	<= 0.003 %	<0.003 %	PASS

Internal ID #: 710

Signature

Additional Information

We certify that this batch conforms to the specifications listed.

Analysis may have been rounded to significant digits in specification limits.

This document has been electronically produced and is valid without a signature.

Product meets analytical specifications of the grades listed.

Leona Edwardson, Quality Control Sr. Manager - Solon  
VWR Chemicals, LLC.  
28600 Fountain Parkway, Solon OH 44139 USA

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4

Batch No.: 25A0262002

Manufactured Date: 2024-11-21

Expiration Date: 2026-02-20

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) (ng/mL)	Single Impurity Peak <= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide)	Single Peak <= 10 (pg/mL)	4
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	>= 99.8 %	99.9 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.8 ppm
Titrable Acid (μeq/g)	<= 0.3	<0.1
Chloride (Cl)	<= 10 ppm	<5 ppm
Water (by KF, coulometric)	<= 0.02 %	<0.01 %

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr &amp; DC

E 3874

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials,LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03  
Batch No.: 24H2762008  
Manufactured Date: 2024-04-18  
Expiration Date: 2027-04-18  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	0.2
Titrable Base (μeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3902

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087, U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4

Batch No.: 25A0262002

Manufactured Date: 2024-11-21

Expiration Date: 2026-02-20

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	4
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	>= 99.8 %	99.9 %
Color (APHA)	<= 10	10
Residue after Evaporation	<= 1.0 ppm	0.8 ppm
Titrable Acid (μeq/g)	<= 0.3	<0.1
Chloride (Cl)	<= 10 ppm	<5 ppm
Water (by KF, coulometric)	<= 0.02 %	<0.01 %

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr &amp; DC

E 3926

 A handwritten signature of the name 'Jamie Croak' is written over a dark rectangular background.
 

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials,LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087 U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone

BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titrable Acid (μeq/g)	<= 0.3	0.2
Titrable Base (μeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 6/11/25

E3940

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 25A2862010  
Manufactured Date: 2024-12-18  
Expiration Date: 2026-03-19  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	2
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	>= 99.8 %	99.9 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.3 ppm
Titrable Acid ( $\mu\text{eq/g}$ )	<= 0.3	<0.1
Chloride (Cl)	<= 10 ppm	<5 ppm
Water (by KF, coulometric)	<= 0.02 %	<0.01 %

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3942

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 25A2862010  
Manufactured Date: 2024-12-18  
Expiration Date: 2026-03-19  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	2
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	>= 99.8 %	99.9 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.3 ppm
Titrable Acid ( $\mu\text{eq/g}$ )	<= 0.3	<0.1
Chloride (Cl)	<= 10 ppm	<5 ppm
Water (by KF, coulometric)	<= 0.02 %	<0.01 %

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3942

A handwritten signature in black ink that reads "Croak".

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Sulfuric Acid  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis  
Low Selenium



M6157  
B

Material No.: 9673-33

Batch No.: 24I1262013

Manufactured Date: 2024-08-07

Retest Date: 2029-08-06

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
ACS - Assay (H <sub>2</sub> SO <sub>4</sub> )	95.0 – 98.0 %	96.2 %
Appearance	Passes Test	Passes Test
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	<1 ppm
ACS - Substances Reducing Permanganate(as SO <sub>2</sub> )	<= 2 ppm	<2 ppm
Ammonium (NH <sub>4</sub> )	<= 1 ppm	<1 ppm
Chloride (Cl)	<= 0.1 ppm	<0.1 ppm
Nitrate (NO <sub>3</sub> )	<= 0.2 ppm	0.1 ppm
Phosphate (PO <sub>4</sub> )	<= 0.5 ppm	<0.1 ppm
Trace Impurities - Aluminum (Al)	<= 30.0 ppb	<5.0 ppb
Arsenic & Antimony (as As)	<= 4.0 ppb	<2.0 ppb
Trace Impurities - Boron (B)	<= 10.0 ppb	<5.0 ppb
Trace Impurities - Cadmium (Cd)	<= 2.0 ppb	<1.0 ppb
Trace Impurities - Chromium (Cr)	<= 6.0 ppb	<1.0 ppb
Trace Impurities - Cobalt (Co)	<= 0.5 ppb	<0.3 ppb
Trace Impurities - Copper (Cu)	<= 1.0 ppb	<1.0 ppb
Trace Impurities - Gold (Au)	<= 10.0 ppb	<5.0 ppb
Heavy Metals (as Pb)	<= 500.0 ppb	<100.0 ppb
Trace Impurities - Iron (Fe)	<= 50.0 ppb	<1.0 ppb
Trace Impurities - Lead (Pb)	<= 0.5 ppb	<0.5 ppb
Trace Impurities - Magnesium (Mg)	<= 7.0 ppb	<1.0 ppb
Trace Impurities - Manganese (Mn)	<= 1.0 ppb	<1.0 ppb
Trace Impurities - Mercury (Hg)	<= 0.5 ppb	<0.1 ppb
Trace Impurities - Nickel (Ni)	<= 2.0 ppb	<0.3 ppb
Trace Impurities - Potassium (K)	<= 500.0 ppb	<10.0 ppb
Trace Impurities - Selenium (Se)	<= 50.0 ppb	7.2 ppb
Trace Impurities - Silicon (Si)	<= 100.0 ppb	12.8 ppb
Trace Impurities - Silver (Ag)	<= 1.0 ppb	<1.0 ppb

Sulfuric Acid  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis  
Low Selenium



Material No.: 9673-33  
Batch No.: 24I1262013

Test	Specification	Result
Trace Impurities – Sodium (Na)	<= 500.0 ppb	<5.0 ppb
Trace Impurities – Strontium (Sr)	<= 5.0 ppb	<1.0 ppb
Trace Impurities – Tin (Sn)	<= 5.0 ppb	1.1 ppb
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	<1.0 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak  
Director Quality Operations, Bioscience Production



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage: Solvent: Exp. Date: Description:  
Z-110094-02 506889 ≤ -10 °C Methylene Chloride 7/25/2028 CLP Base/Neutral Surrogate Solution, 5,000 mg/L, 1 ml

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
1,2-dichlorobenzene-d <sub>4</sub>	2199-69-1	99.7	247.29.3P	5035 ± 28.02
2-fluorobiphenyl	321-60-8	99.69	8.286.1.1P	4999 ± 103.66
nitrobenzene-d <sub>5</sub>	4165-60-0	99.67	7.9.3P	4988 ± 27.32
p-terphenyl-d <sub>14</sub>	1718-51-0	99.3	9.120.8P	5005 ± 27.85

511494 } Y.P.  
↓ } 08/11/2023  
511498

\*Not a certified value

Certified By: \_\_\_\_\_

Clint Tipton  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*gravimetric*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No.:** 555872

**Lot No.:** A0201728

**Description :** Custom Pentachlorophenol Standard

Custom Pentachlorophenol Standard 25,000 $\mu$ g/mL, Methanol,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2026

**Storage:** 10°C or colder

**Ship:** Ambient

511649  
↓  
511658 } Y.P.  
} 11/13/23

### C E R T I F I E D V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Pentachlorophenol	87-86-5	RP230530RSR	99%	25,000.0 $\mu$ g/mL	+/- 777.0837

**Solvent:** Methanol  
**CAS #** 67-56-1  
**Purity** 99%

Josh McCloskey - Operations Technician I

Date Mixed: 05-Sep-2023 Balance: B251644995

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31853

**Lot No.:** A0196453

**Description :** 1,4-dioxane

1,4-Dioxane 2,000 $\mu$ g/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** March 31, 2028

**Storage:** 0°C or colder

**Ship:** Ambient

SI1749  
↓ { RC /  
SI1794 } 11/30/23

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dioxane	123-91-1	SHBN3770	99%	2,013.0 $\mu$ g/mL	+/- 25.0521

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant flow 1.8 mL/min.

**Temp. Program:**

80°C (hold 0.1 min.) to 330°C  
@ 9.6°C/min. (hold 2.86 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

340°C

**Det. Type:**


FID

**Split Vent:**

100 mL/min.

**Inj. Vol**

1 $\mu$ L

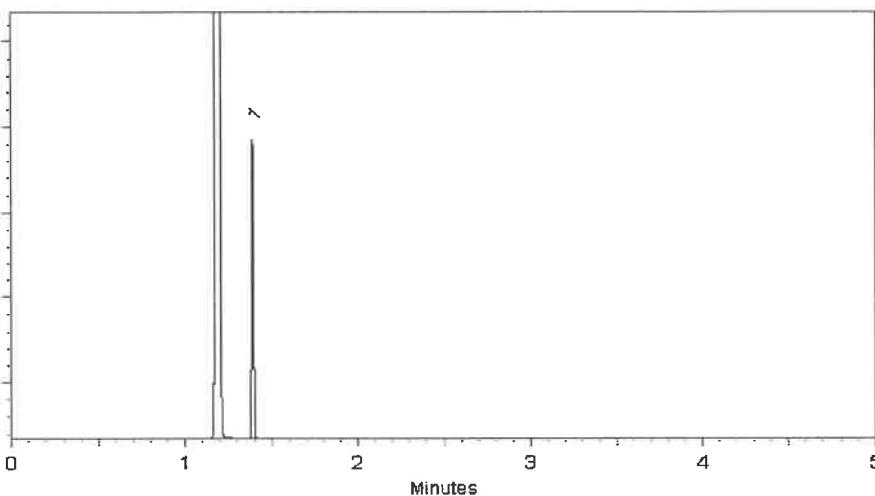

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodier*  
Sam Moodier - Operations Tech I

Date Mixed: 30-Mar-2023 Balance Serial #: B707717271

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 31-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/µECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 33913

**Lot No.:** A0201976

**Description :** SOM01.0 SIM Analysis Standard

SOM01.0 SIM Analysis Standard 2000 $\mu$ g/mL, Methylene chloride, 1mL /ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** August 31, 2029

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

511828  
↓  
511832 } RC/  
11/30/23 }

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Methylnaphthalene-d10	7297-45-2	EF-135	98%	2,015.9 $\mu$ g/mL	+/- 90.8098
2	Fluoranthene-d10	93951-69-0	PR-32557	99%	2,020.0 $\mu$ g/mL	+/- 90.9963

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride

**CAS #** 75-09-2

**Purity** 99%

# Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25 $\mu$ m

Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C

@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

**Split Vent:**

10 ml/min.

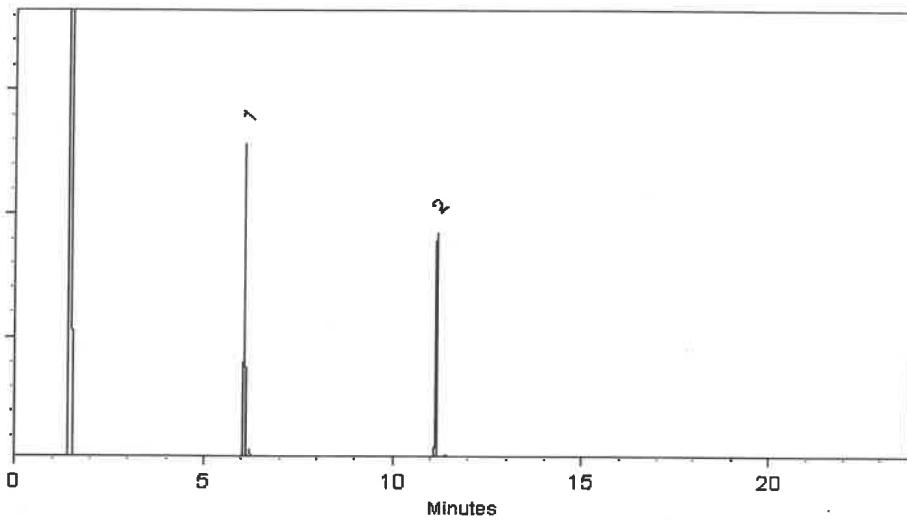**Inj. Vol**1 $\mu$ l

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I

Date Mixed: 13-Sep-2023      Balance Serial #: B442140311

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 28-Sep-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 33913

**Lot No.:** A0201976

**Description :** SOM01.0 SIM Analysis Standard

SOM01.0 SIM Analysis Standard 2000 $\mu$ g/mL, Methylene chloride, 1mL  
/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** August 31, 2029

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is  
photosensitive.

**Ship:** Ambient

511828  
↓  
511832 } RC/  
11/30/23 }

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Methylnaphthalene-d10	7297-45-2	EF-135	98%	2,015.9 $\mu$ g/mL	+/- 90.8098
2	Fluoranthene-d10	93951-69-0	PR-32557	99%	2,020.0 $\mu$ g/mL	+/- 90.9963

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride

**CAS #** 75-09-2

**Purity** 99%

# Quality Confirmation Test

**Column:**30m x 0.25mm x 0.25 $\mu$ m

Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C

@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

**Split Vent:**


10 ml/min.

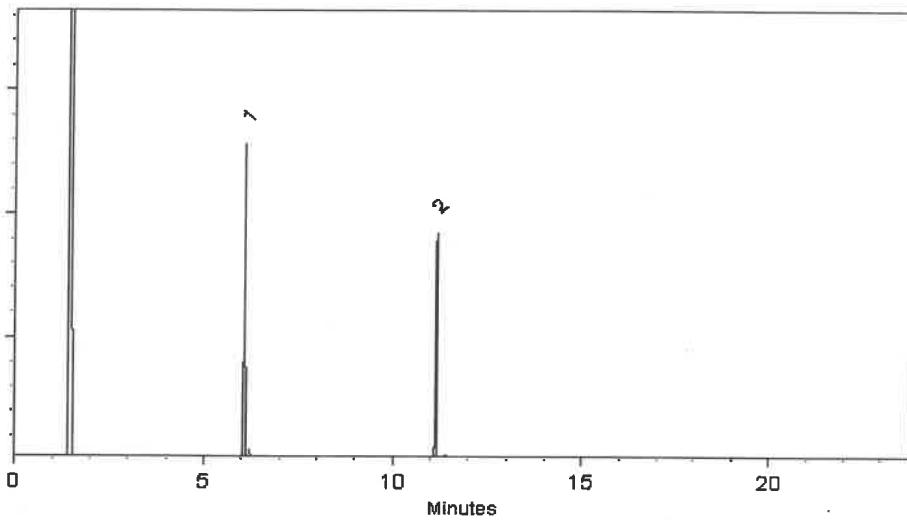**Inj. Vol**1 $\mu$ l

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I

Date Mixed: 13-Sep-2023      Balance Serial #: B442140311

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 28-Sep-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage: Solvent: Exp. Date: Description:  
Z-020223-01 454157 ≤ -10 °C P/T Methanol 6/10/2026 1,4-Dioxane Solution, 2000 mg/L,  
1 mL

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
1,4-dioxane	123-91-1	100	223.1.3P	1997 ± 57.08

512112 } RC/  
↓  
512116 } 03/08/24

\*Not a certified value

Certified By:

Melissa Workoff  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



## Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31087

**Lot No.:** A0206206

512187 } RC/  
↓ } 03/18/24  
512206 }

**Description :** Acid Surrogate Mix (4/89 SOW)

Acid Surrogate 10,000 $\mu$ g/mL, Methanol, 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** January 31, 2032

**Storage:** 10°C or colder

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2-Fluorophenol	367-12-4	STBK1705	99%	10,005.3 $\mu$ g/mL	+/- 302.5390
2	Phenol-d6	13127-88-3	PR-33287A	99%	10,005.5 $\mu$ g/mL	+/- 302.5475
3	2,4,6-Tribromophenol	118-79-6	RP230831RSR	99%	10,006.6 $\mu$ g/mL	+/- 302.5783

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methanol

**CAS #** 67-56-1

**Purity** 99%

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 mL/min.

**Inj. Vol**

1 $\mu$ L

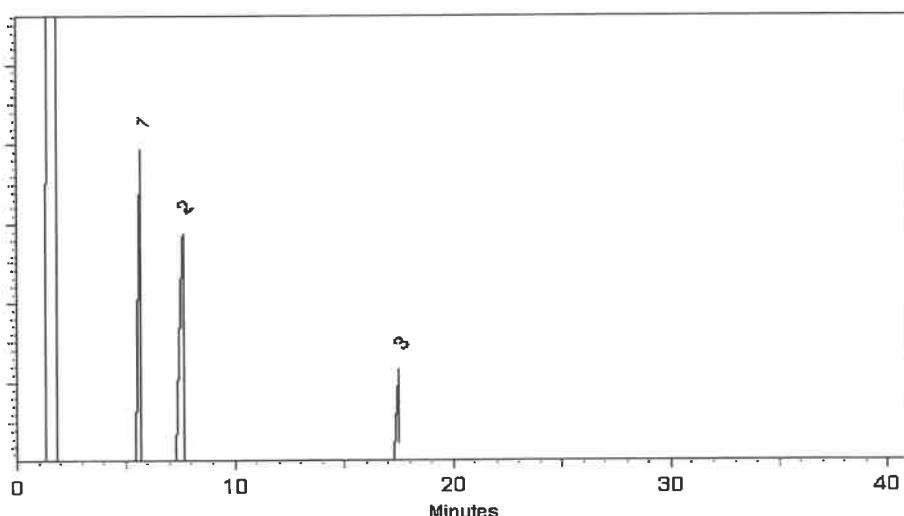

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope Regin - Operations Tech |

Date Mixed: 04-Jan-2024      Balance Serial #: 1128360905

Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 08-Jan-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31086

**Lot No.:** A0206381

**Description :** B/N Surrogate Mix (4/89 SOW)

Base Neutral Surrogate 5000 $\mu$ g/mL, Methylene Chloride, 5mL/ampul

**Container Size :** 5 mL

**Pkg Amt:** > 5 mL

**Expiration Date :** December 31, 2029

**Storage:** 10°C or colder

**Handling:** Sonicate prior to use.

**Ship:** Ambient

512207 } RC /  
↓ } 03/18/24  
512221 }

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Nitrobenzene-d5	4165-60-0	I-25158	99%	5,029.3 $\mu$ g/mL	+/- 226.5204
2	2-Fluorobiphenyl	321-60-8	00021384	99%	5,030.9 $\mu$ g/mL	+/- 226.5936
3	p-Terphenyl-d14	1718-51-0	PR-32599	99%	5,026.4 $\mu$ g/mL	+/- 226.3909

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride

**CAS #** 75-09-2

**Purity** 99%

### Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 mL/min.

**Inj. Vol**

1 $\mu$ L

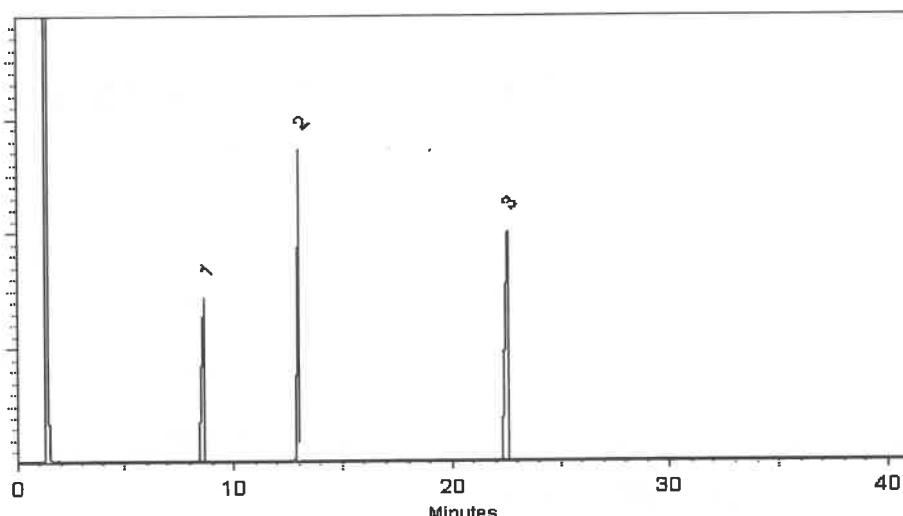

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Jess Hoy - Operations Tech I

Date Mixed: 09-Jan-2024 Balance Serial #: 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 11-Jan-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 4

Catalog No.: Lot No.:	Storage:	Solvent:	Exp. Date:	Description:
Z-110381-01 520963	≤ -10 °C	Methylene Chloride	10/10/2028	Method 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1 mL

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
acenaphthene	83-32-9	99.9	13.1.5P	1010 ± 9.89
acenaphthylene	208-96-8	97.6	14.290.1P	1014 ± 9.93
aniline	62-53-3	99.97	64.1.4P	1001 ± 9.8
anthracene	120-12-7	99.5	15.7.1P	999.6 ± 9.79
azobenzene	103-33-3	98.1	252.7.2P	999.1 ± 9.8
benzo[a]anthracene	56-55-3	100	16.7.3P	1007 ± 9.86
benzo[b]fluoranthene	205-99-2	99.8	17.421.3P	1011 ± 14.11
benzo[k]fluoranthene	207-08-9	98.9	18.421.4P	1001 ± 10.96
benzo[ghi]perylene	191-24-2	93	19.286.4P	999.6 ± 13.95
benzo[a]pyrene	50-32-8	97	20.286.2P	999.9 ± 22.24
benzyl alcohol	100-51-6	99.9	65.18.1P	1001 ± 9.82
bis(2-chloroethoxy)methane	111-91-1	99.1	31.3.15P	1000 ± 14.69
bis(2-chloroethyl)ether	111-44-4	99.8	32.7.1P	1003 ± 13.89
bis(2-chloro-1-methylethyl) ether	108-60-1	99.5	34.3.15P	999.4 ± 14.68
bis(2-ethylhexyl)adipate	103-23-1	99.5	874.7.1P	999.5 ± 9.8
bis(2-ethylhexyl)phthalate	117-81-7	99.4	33.29.1P	998.8 ± 17.03
4-bromophenyl phenyl ether	101-55-3	99.4	35.7.1.1P	1000 ± 13.85
butyl benzyl phthalate	85-68-7	98.4	36.1.6P	984.7 ± 16.79
carbazole	86-74-8	99.4	239.7.2P	1000 ± 9.8

512270 } Rcf  
↓ 512274 } 05/24/24

\*Not a certified value

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.

Certified By: \_\_\_\_\_

Kerry Kane  
Chemist

# Certificate of Analysis

Page 2 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
4-chloroaniline	106-47-8	100	66.7.1P	1000 ± 9.79
4-chlorophenylphenyl ether	7005-72-3	98	37.158.2P	1001 ± 17.07
4-chloro-3-methylphenol	59-50-7	99	102.1.2P	1006 ± 17.16
2-chloronaphthalene	91-58-7	99.9	42.7.6P	1000 ± 9.79
2-chlorophenol	95-57-8	99.8	103.7.1P	1007 ± 13.96
chrysene	218-01-9	96	21.286.2P	998.4 ± 12.85
dibenz[a,h]anthracene	53-70-3	99.44	22.286.3P	1000 ± 9.74
dibenzofuran	132-64-9	100	67.7.2.1P	1002 ± 9.77
di-n-butyl phthalate	84-74-2	99.84	40.286.1P	1007 ± 24.48
1,2-dichlorobenzene	95-50-1	99.8	43.7.1P	1000 ± 9.79
1,3-dichlorobenzene	541-73-1	99.5	44.1.3P	999.4 ± 9.79
1,4-dichlorobenzene	106-46-7	99.9	45.29.2P	1000 ± 9.79
2,4-dichlorophenol	120-83-2	99.6	104.7.1.1P	1005 ± 13.93
diethyl phthalate	84-66-2	99.8	38.7.1P	1011 ± 14
2,4-dimethylphenol	105-67-9	99.6	105.7.1.1P	1009 ± 13.98
dimethyl phthalate	131-11-3	99.9	39.9.2P	996.5 ± 13.8
1,2-dinitrobenzene	528-29-0	99.86	86.7.3.1P	999.5 ± 9.75
1,3-dinitrobenzene	99-65-0	100	313.7.2P	998 ± 9.79
1,4-dinitrobenzene	100-25-4	100	907.7.1P	999.5 ± 9.8
2,4-dinitrophenol	51-28-5	99.9	106.1.6DP	1002 ± 13.89
2,4-dinitrotoluene	121-14-2	100	87.7.3P	999.8 ± 13.85
2,6-dinitrotoluene	606-20-2	99.4	88.7.2.1P	999.6 ± 13.85
di-n-octyl phthalate	117-84-0	99.1	41.7.5P	991.6 ± 13.74
diphenylamine	122-39-4	100	78.1.6P	998 ± 13.79
2,3,5,6-tetrachlorophenol	935-95-5	97	1112.286.1P	1004 ± 14.02
fluoranthene	206-44-0	98.6	23.7.4P	999.6 ± 9.79
fluorene	86-73-7	98.4	24.7.1P	999.7 ± 9.79

\*Not a certified value

Certified By:

Kerry Kane  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

# Certificate of Analysis

Page 3 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
hexachlorobenzene	118-74-1	99	46.158.4P	999.9 ± 13.96
hexachlorobutadiene	87-68-3	97.4	47.1.4P	1000 ± 9.79
hexachlorocyclopentadiene	77-47-4	99.2	48.2.2P	1001 ± 9.8
hexachloroethane	67-72-1	99.9	49.1.4P	1003 ± 9.82
indeno[1,2,3-cd]pyrene	193-39-5	98	25.286.4P	999.4 ± 22.23
isophorone	78-59-1	98.9	90.1.4P	999.9 ± 13.85
2-methyl-4,6-dinitrophenol	534-52-1	99.6	107.421.2DP	991 ± 24.09
1-methylnaphthalene	90-12-0	97.1	249.7.5P	999.2 ± 13.95
2-methylnaphthalene	91-57-6	97.4	68.7.2P	1006 ± 22.38
2-methylphenol	95-48-7	99.6	114.7.3P	1001 ± 13.87
3-methylphenol	108-39-4	99.1	115.7.4P	499.7 ± 6.92
4-methylphenol	106-44-5	99.5	116.7.1P	501.2 ± 6.94
naphthalene	91-20-3	99.8	26.9.1P	1018 ± 9.97
2-nitroaniline	88-74-4	99.7	69.29.1P	999.6 ± 9.79
3-nitroaniline	99-09-2	100	70.7.3P	1000 ± 9.74
4-nitroaniline	100-01-6	99.7	71.29.1P	1001 ± 9.8
nitrobenzene	98-95-3	100	94.7.1P	1000 ± 13.85
2-nitrophenol	88-75-5	99.1	108.29.1P	996.5 ± 13.81
4-nitrophenol	100-02-7	100	109.7.1P	1000 ± 13.82
N-nitrosodimethylamine	62-75-9	99.5	57.3.19P	998.5 ± 14.67
N-nitrosodi-n-propylamine	621-64-7	99.8	59.286.1P	996.8 ± 17
pentachlorophenol	87-86-5	99	110.1.7P	1004 ± 13.92
phenanthrene	85-01-8	99.7	27.1.5P	999 ± 12.87
phenol	108-95-2	100	112.7.1P	998.5 ± 13.8
pyrene	129-00-0	99.2	28.9.2P	998.9 ± 9.78
pyridine	110-86-1	100	101.24.1P	999 ± 9.73
2,3,4,6-Tetrachlorophenol	58-90-2	91.8	120.421.1P	996.5 ± 13.92

\*Not a certified value

Certified By:

Kerry Kane  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

# Certificate of Analysis

Page 4 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
1,2,4-trichlorobenzene	120-82-1	99.6	54.29.1P	999.6 ± 9.79
2,4,5-trichlorophenol	95-95-4	96.5	121.7.1.1P	999.5 ± 13.85
2,4,6-trichlorophenol	88-06-2	99.6	113.7.1P	996 ± 13.8

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18

\*Not a certified value

Certified By:



Kerry Kane  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 4

Catalog No.: Lot No.:	Storage:	Solvent:	Exp. Date:	Description:
Z-110381-01 520963	≤ -10 °C	Methylene Chloride	10/10/2028	Method 8270 Calibration Solution, 76-1, 500 & 1,000 mg/L, 1 mL

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
acenaphthene	83-32-9	99.9	13.1.5P	1010 ± 9.89
acenaphthylene	208-96-8	97.6	14.290.1P	1014 ± 9.93
aniline	62-53-3	99.97	64.1.4P	1001 ± 9.8
anthracene	120-12-7	99.5	15.7.1P	999.6 ± 9.79
azobenzene	103-33-3	98.1	252.7.2P	999.1 ± 9.8
benzo[a]anthracene	56-55-3	100	16.7.3P	1007 ± 9.86
benzo[b]fluoranthene	205-99-2	99.8	17.421.3P	1011 ± 14.11
benzo[k]fluoranthene	207-08-9	98.9	18.421.4P	1001 ± 10.96
benzo[ghi]perylene	191-24-2	93	19.286.4P	999.6 ± 13.95
benzo[a]pyrene	50-32-8	97	20.286.2P	999.9 ± 22.24
benzyl alcohol	100-51-6	99.9	65.18.1P	1001 ± 9.82
bis(2-chloroethoxy)methane	111-91-1	99.1	31.3.15P	1000 ± 14.69
bis(2-chloroethyl)ether	111-44-4	99.8	32.7.1P	1003 ± 13.89
bis(2-chloro-1-methylethyl) ether	108-60-1	99.5	34.3.15P	999.4 ± 14.68
bis(2-ethylhexyl)adipate	103-23-1	99.5	874.7.1P	999.5 ± 9.8
bis(2-ethylhexyl)phthalate	117-81-7	99.4	33.29.1P	998.8 ± 17.03
4-bromophenyl phenyl ether	101-55-3	99.4	35.7.1.1P	1000 ± 13.85
butyl benzyl phthalate	85-68-7	98.4	36.1.6P	984.7 ± 16.79
carbazole	86-74-8	99.4	239.7.2P	1000 ± 9.8

512270 } Rcf  
↓ 512274 } 05/24/24

\*Not a certified value

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.

Certified By: \_\_\_\_\_

Kerry Kane  
Chemist

# Certificate of Analysis

Page 2 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
4-chloroaniline	106-47-8	100	66.7.1P	1000 ± 9.79
4-chlorophenylphenyl ether	7005-72-3	98	37.158.2P	1001 ± 17.07
4-chloro-3-methylphenol	59-50-7	99	102.1.2P	1006 ± 17.16
2-chloronaphthalene	91-58-7	99.9	42.7.6P	1000 ± 9.79
2-chlorophenol	95-57-8	99.8	103.7.1P	1007 ± 13.96
chrysene	218-01-9	96	21.286.2P	998.4 ± 12.85
dibenz[a,h]anthracene	53-70-3	99.44	22.286.3P	1000 ± 9.74
dibenzofuran	132-64-9	100	67.7.2.1P	1002 ± 9.77
di-n-butyl phthalate	84-74-2	99.84	40.286.1P	1007 ± 24.48
1,2-dichlorobenzene	95-50-1	99.8	43.7.1P	1000 ± 9.79
1,3-dichlorobenzene	541-73-1	99.5	44.1.3P	999.4 ± 9.79
1,4-dichlorobenzene	106-46-7	99.9	45.29.2P	1000 ± 9.79
2,4-dichlorophenol	120-83-2	99.6	104.7.1.1P	1005 ± 13.93
diethyl phthalate	84-66-2	99.8	38.7.1P	1011 ± 14
2,4-dimethylphenol	105-67-9	99.6	105.7.1.1P	1009 ± 13.98
dimethyl phthalate	131-11-3	99.9	39.9.2P	996.5 ± 13.8
1,2-dinitrobenzene	528-29-0	99.86	86.7.3.1P	999.5 ± 9.75
1,3-dinitrobenzene	99-65-0	100	313.7.2P	998 ± 9.79
1,4-dinitrobenzene	100-25-4	100	907.7.1P	999.5 ± 9.8
2,4-dinitrophenol	51-28-5	99.9	106.1.6DP	1002 ± 13.89
2,4-dinitrotoluene	121-14-2	100	87.7.3P	999.8 ± 13.85
2,6-dinitrotoluene	606-20-2	99.4	88.7.2.1P	999.6 ± 13.85
di-n-octyl phthalate	117-84-0	99.1	41.7.5P	991.6 ± 13.74
diphenylamine	122-39-4	100	78.1.6P	998 ± 13.79
2,3,5,6-tetrachlorophenol	935-95-5	97	1112.286.1P	1004 ± 14.02
fluoranthene	206-44-0	98.6	23.7.4P	999.6 ± 9.79
fluorene	86-73-7	98.4	24.7.1P	999.7 ± 9.79

\*Not a certified value

Certified By:

Kerry Kane  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

# Certificate of Analysis

Page 3 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
hexachlorobenzene	118-74-1	99	46.158.4P	999.9 ± 13.96
hexachlorobutadiene	87-68-3	97.4	47.1.4P	1000 ± 9.79
hexachlorocyclopentadiene	77-47-4	99.2	48.2.2P	1001 ± 9.8
hexachloroethane	67-72-1	99.9	49.1.4P	1003 ± 9.82
indeno[1,2,3-cd]pyrene	193-39-5	98	25.286.4P	999.4 ± 22.23
isophorone	78-59-1	98.9	90.1.4P	999.9 ± 13.85
2-methyl-4,6-dinitrophenol	534-52-1	99.6	107.421.2DP	991 ± 24.09
1-methylnaphthalene	90-12-0	97.1	249.7.5P	999.2 ± 13.95
2-methylnaphthalene	91-57-6	97.4	68.7.2P	1006 ± 22.38
2-methylphenol	95-48-7	99.6	114.7.3P	1001 ± 13.87
3-methylphenol	108-39-4	99.1	115.7.4P	499.7 ± 6.92
4-methylphenol	106-44-5	99.5	116.7.1P	501.2 ± 6.94
naphthalene	91-20-3	99.8	26.9.1P	1018 ± 9.97
2-nitroaniline	88-74-4	99.7	69.29.1P	999.6 ± 9.79
3-nitroaniline	99-09-2	100	70.7.3P	1000 ± 9.74
4-nitroaniline	100-01-6	99.7	71.29.1P	1001 ± 9.8
nitrobenzene	98-95-3	100	94.7.1P	1000 ± 13.85
2-nitrophenol	88-75-5	99.1	108.29.1P	996.5 ± 13.81
4-nitrophenol	100-02-7	100	109.7.1P	1000 ± 13.82
N-nitrosodimethylamine	62-75-9	99.5	57.3.19P	998.5 ± 14.67
N-nitrosodi-n-propylamine	621-64-7	99.8	59.286.1P	996.8 ± 17
pentachlorophenol	87-86-5	99	110.1.7P	1004 ± 13.92
phenanthrene	85-01-8	99.7	27.1.5P	999 ± 12.87
phenol	108-95-2	100	112.7.1P	998.5 ± 13.8
pyrene	129-00-0	99.2	28.9.2P	998.9 ± 9.78
pyridine	110-86-1	100	101.24.1P	999 ± 9.73
2,3,4,6-Tetrachlorophenol	58-90-2	91.8	120.421.1P	996.5 ± 13.92

\*Not a certified value

Certified By:

Kerry Kane  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.

# Certificate of Analysis

Page 4 of 4

Catalog No.: Z-110381-01

Lot No.: 520963

Expiration Date: 10/10/2028

Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
1,2,4-trichlorobenzene	120-82-1	99.6	54.29.1P	999.6 ± 9.79
2,4,5-trichlorophenol	95-95-4	96.5	121.7.1.1P	999.5 ± 13.85
2,4,6-trichlorophenol	88-06-2	99.6	113.7.1P	996 ± 13.8

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18

\*Not a certified value



Certified By:

Kerry Kane  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*gravimetric*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 555223 **Lot No.:** A0214021

**Description :** Custom 8270 Plus Standard #1

Custom 8270 Plus Standard #1 1,000 $\mu$ g/mL, Methylene Chloride,  
1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** July 31, 2026 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

### C E R T I F I E D V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	3,3'-Dichlorobenzidine	91-94-1	S240326RSR	99%	1,004.0 $\mu$ g/mL	+/- 23.0487
2	Atrazine	1912-24-9	5FYWL	99%	1,005.0 $\mu$ g/mL	+/- 23.0717
3	Benzidine	92-87-5	S240430RSR	99%	1,006.0 $\mu$ g/mL	+/- 23.0947
4	epsilon-Caprolactam	105-60-2	Y16H012	99%	1,000.0 $\mu$ g/mL	+/- 22.9569

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

S12449 } RC/  
↓ } 7/24/24  
S12508 }

Rebecca Gingerich - Operations Tech II

Date Mixed: 18-Jul-2024

Balance: 1128353505

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



## Certificate of Analysis

gravimetric

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555224

Lot No.: A0214017

Description : Custom 8270 Plus Standard #2

Custom 8270 Plus Standard #2 1,000 $\mu$ g/mL, Methylene Chloride,  
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2026

Storage: 10°C or colder

Ship: Ambient

### C E R T I F I E D   V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2,4,5-Tetrachlorobenzene	95-94-3	MKCT9480	99%	1,005.0 $\mu$ g/mL	+/- 29.541899
2	Acetophenone	98-86-2	STBH8205	99%	1,005.0 $\mu$ g/mL	+/- 29.541899
3	Benzaldehyde	100-52-7	RD231129RSRA	99%	1,008.0 $\mu$ g/mL	+/- 29.630084
4	Benzoic acid	65-85-0	MKCR2694	99%	1,010.0 $\mu$ g/mL	+/- 29.688874
5	Biphenyl	92-52-4	MKCS5928	99%	1,008.0 $\mu$ g/mL	+/- 29.630084

Solvent: Methylene chloride  
CAS # 75-09-2  
Purity 99%

512509  
↓  
512568 } RC / 7/24/24

  
Jess Hoy - Operations Tech I

Date Mixed: 18-Jul-2024 Balance: 1128360905

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# General Certified Reference Material Notes

## Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

## Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

## Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

## Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

## Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



ILAC  
ACCREDITED  
ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ILAC  
ACCREDITED  
ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

## Certificate of Analysis *chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31615

**Lot No.:** A0212955

**Description :** GC/MS Tuning Mixture

GC/MS Tuning Mixture 1,000 $\mu$ g/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** June 30, 2027

**Storage:** 10°C or colder

**Handling:** Contains carcinogen/reproductive toxin.

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Pentachlorophenol	87-86-5	RP240517RSR	99%	1,004.5 $\mu$ g/mL	+/- 44.8902
2	DFTPP (Decafluorotriphenylphosphine)	5074-71-5	Q117-147	99%	1,004.5 $\mu$ g/mL	+/- 44.8902
3	Benzidine	92-87-5	S240430RSR	99%	1,006.0 $\mu$ g/mL	+/- 44.9572
4	4,4'-DDT	50-29-3	S240530RSR	97%	1,000.1 $\mu$ g/mL	+/- 44.6922

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

S12577  
↓  
S12579 } 8/2/24

# Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25 $\mu$ m  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1 $\mu$ l

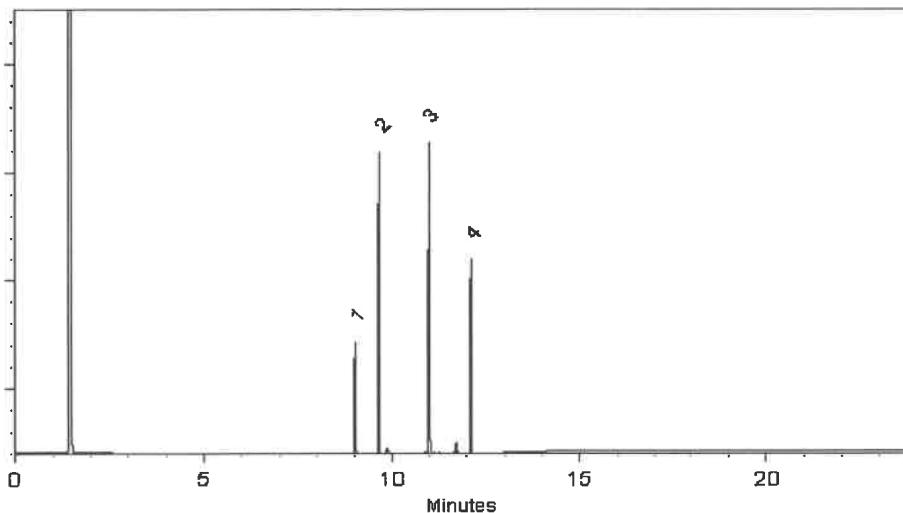

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Ethan Winiarski*  
Ethan Winiarski - Operations Tech I

Date Mixed: 19-Jun-2024 Balance Serial #: 1128353505

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 26-Jun-2024

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



## Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31206

**Lot No.:** A0212266

**Description :** SV Internal Standard Mix 2mg/ml

SV Internal Standard Mix 2mg/ml 2000 µg/ml, Methylene Chloride,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is  
photosensitive.

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	2,000.6 µg/mL	+/- 90.1075
2	Naphthalene-d8	1146-65-2	M-2180	99%	2,000.3 µg/mL	+/- 90.0925
3	Acenaphthene-d10	15067-26-2	PR-33507	99%	2,000.4 µg/mL	+/- 90.1000
4	Phenanthrene-d10	1517-22-2	PR-34099	99%	2,000.5 µg/mL	+/- 90.1037
5	Chrysene-d12	1719-03-5	PR-33506	99%	2,000.7 µg/mL	+/- 90.1112
6	Perylene-d12	1520-96-3	PR-33205	99%	2,000.6 µg/mL	+/- 90.1075

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

S12645 } AC  
↓  
S12674 } ID/1/24



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



## Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31206

**Lot No.:** A0212266

**Description :** SV Internal Standard Mix 2mg/ml

SV Internal Standard Mix 2mg/ml 2000 µg/ml, Methylene Chloride,  
1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** April 30, 2030

**Storage:** 10°C or colder

**Handling:** Sonication required. Mix is  
photosensitive.

**Ship:** Ambient

### C E R T I F I E D   V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	2,000.6 µg/mL	+/- 90.1075
2	Naphthalene-d8	1146-65-2	M-2180	99%	2,000.3 µg/mL	+/- 90.0925
3	Acenaphthene-d10	15067-26-2	PR-33507	99%	2,000.4 µg/mL	+/- 90.1000
4	Phenanthrene-d10	1517-22-2	PR-34099	99%	2,000.5 µg/mL	+/- 90.1037
5	Chrysene-d12	1719-03-5	PR-33506	99%	2,000.7 µg/mL	+/- 90.1112
6	Perylene-d12	1520-96-3	PR-33205	99%	2,000.6 µg/mL	+/- 90.1075

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride  
**CAS #** 75-09-2  
**Purity** 99%

S12645 } AC  
↓  
S12674 } ID/1/24



5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.:	Storage:	Solvent:	Exp. Date:	Description:	
Z-110816-01 414127	≤ -10 °C	Methylene Chloride	6/21/2025	Custom 8270 Mix, 4-79, 1000 mg/L, 1 mL	
Compound		CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
atrazine		1912-24-9	99.5	337.7.3P	997 ± 5.81
benzidine		92-87-5	99.9	124.18.6.2P	991.8 ± 5.77
caprolactam		105-60-2	99.9	271.1.6P	999 ± 5.82

~~S12280~~ } RC/  
~~S12284~~ } 05/24/24

New numbers generated.

S12790 } RC/  
↓            } 11/12/24  
S12794

Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

\*Not a certified value

Certified By:

Shane Overcash  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values listed are determined gravimetrically.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL



# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31850

**Lot No.:** A0219438

**Description :** 8270 MegaMix®

8270 MegaMix® 500-1000 µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL

**Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2025

**Storage:** 0°C or colder

**Handling:** Sonication required. Mix is photosensitive.

**Ship:** Ambient

S12963 }  
↓ AC  
S12992 } 12/17/22

### C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Pyridine	110-86-1	SHBP6240	99%	1,008.3 µg/mL	+/- 36.6849
2	N-Nitrosodimethylamine	62-75-9	S240313RSR	99%	1,008.6 µg/mL	+/- 36.6985
3	Phenol	108-95-2	MKCK1120	99%	1,003.5 µg/mL	+/- 36.5120
4	Aniline	62-53-3	X22F726	99%	1,002.9 µg/mL	+/- 36.4893
5	Bis(2-chloroethyl)ether	111-44-4	002891T24M	99%	1,003.0 µg/mL	+/- 36.4938
6	2-Chlorophenol	95-57-8	STBJ3909	99%	1,005.6 µg/mL	+/- 36.5894
7	1,3-Dichlorobenzene	541-73-1	BCCD5315	99%	1,004.1 µg/mL	+/- 36.5348
8	1,4-Dichlorobenzene	106-46-7	MKBS7929V	99%	1,002.1 µg/mL	+/- 36.4620
9	Benzyl alcohol	100-51-6	SHBK5469	99%	1,003.5 µg/mL	+/- 36.5120
10	1,2-Dichlorobenzene	95-50-1	SHBL6287	99%	1,005.3 µg/mL	+/- 36.5757
11	2-Methylphenol (o-cresol)	95-48-7	SHBN7598	99%	1,008.4 µg/mL	+/- 36.6894
12	2,2'-oxybis(1-chloropropane)	108-60-1	29-MAR-45-5	99%	1,004.6 µg/mL	+/- 36.5530
13	3-Methylphenol (m-cresol)	108-39-4	STBJ0710	99%	502.1 µg/mL	+/- 18.2697
14	4-Methylphenol (p-cresol)	106-44-5	SHBN3411	99%	503.8 µg/mL	+/- 18.3288
15	N-Nitroso-di-n-propylamine	621-64-7	N63MG	99%	1,006.5 µg/mL	+/- 36.6212
16	Hexachloroethane	67-72-1	DAXRI	99%	1,004.5 µg/mL	+/- 36.5484
17	Nitrobenzene	98-95-3	10224044	99%	1,002.5 µg/mL	+/- 36.4757

18	Isophorone	78-59-1	MKCR3249	99%	1,003.4	µg/mL	+/-	36.5075
19	2-Nitrophenol	88-75-5	RP230710	99%	1,002.5	µg/mL	+/-	36.4757
20	2,4-Dimethylphenol	105-67-9	XW5GK	99%	1,006.5	µg/mL	+/-	36.6212
21	Bis(2-chloroethoxy)methane	111-91-1	15705100	99%	1,006.6	µg/mL	+/-	36.6257
22	2,4-Dichlorophenol	120-83-2	BCCK6969	99%	1,001.5	µg/mL	+/-	36.4393
23	1,2,4-Trichlorobenzene	120-82-1	SHBP5900	99%	1,006.4	µg/mL	+/-	36.6166
24	Naphthalene	91-20-3	STBL1057	99%	1,002.1	µg/mL	+/-	36.4620
25	4-Chloroaniline	106-47-8	BCCJ3217	99%	1,004.4	µg/mL	+/-	36.5439
26	Hexachlorobutadiene	87-68-3	X05J	98%	1,002.5	µg/mL	+/-	36.4771
27	4-Chloro-3-methylphenol	59-50-7	BCCD4461	99%	1,004.5	µg/mL	+/-	36.5484
28	2-Methylnaphthalene	91-57-6	STBL3028	99%	1,000.0	µg/mL	+/-	36.3847
29	1-Methylnaphthalene	90-12-0	5234.00-8	98%	990.2	µg/mL	+/-	36.0269
30	Hexachlorocyclopentadiene	77-47-4	099063I14L	98%	1,001.3	µg/mL	+/-	36.4325
31	2,4,6-Trichlorophenol	88-06-2	STBK8870	99%	1,006.4	µg/mL	+/-	36.6166
32	2,4,5-Trichlorophenol	95-95-4	3YFRE	97%	1,004.6	µg/mL	+/-	36.5505
33	2-Chloronaphthalene	91-58-7	RPN7O	99%	1,004.3	µg/mL	+/-	36.5393
34	2-Nitroaniline	88-74-4	RP240715RSR	99%	1,004.4	µg/mL	+/-	36.5439
35	1,4-Dinitrobenzene	100-25-4	RP240703RSR	99%	1,002.8	µg/mL	+/-	36.4847
36	Acenaphthylene	208-96-8	RP241029RSR	98%	1,000.0	µg/mL	+/-	36.3835
37	1,3-Dinitrobenzene	99-65-0	TRC3-1075941-2-1	99%	1,006.3	µg/mL	+/-	36.6121
38	Dimethylphthalate	131-11-3	358221L17K	99%	1,008.9	µg/mL	+/-	36.7076
39	2,6-Dinitrotoluene	606-20-2	BCCG1833	99%	1,006.6	µg/mL	+/-	36.6257
40	1,2-Dinitrobenzene	528-29-0	RP240701RSR	99%	1,002.5	µg/mL	+/-	36.4757
41	Acenaphthene	83-32-9	MKCR7169	99%	1,000.0	µg/mL	+/-	36.3847
42	3-Nitroaniline	99-09-2	RP240708RSR	99%	1,004.6	µg/mL	+/-	36.5530
43	2,4-Dinitrophenol	51-28-5	D240927RSR	----%	1,005.6	µg/mL	+/-	36.5894
44	Dibenzofuran	132-64-9	MKCN1772	99%	1,003.5	µg/mL	+/-	36.5120
45	2,4-Dinitrotoluene	121-14-2	102869V26E	99%	1,008.3	µg/mL	+/-	36.6849
46	4-Nitrophenol	100-02-7	20241029-2-AN	99%	1,004.8	µg/mL	+/-	36.5575
47	2,3,4,6-Tetrachlorophenol	58-90-2	PR-34476	99%	1,005.8	µg/mL	+/-	36.5939
48	2,3,5,6-Tetrachlorophenol	935-95-5	RP231219RSR	99%	1,006.4	µg/mL	+/-	36.6166
49	Fluorene	86-73-7	10246250	98%	1,000.7	µg/mL	+/-	36.4102
50	4-Chlorophenyl phenyl ether	7005-72-3	MKCT7248	99%	1,004.9	µg/mL	+/-	36.5621
51	Diethylphthalate	84-66-2	BCCJ6241	99%	1,003.9	µg/mL	+/-	36.5257
52	4-Nitroaniline	100-01-6	RP230111	99%	1,006.6	µg/mL	+/-	36.6257
53	4,6-Dinitro-2-methylphenol (Dinitro-o-cresol)	534-52-1	S241008RSR	99%	1,001.3	µg/mL	+/-	36.4302

54	Diphenylamine	122-39-4	MKCT1512	99%	1,003.0	µg/mL	+/-	36.4938
55	Azobenzene	103-33-3	BCCK0887	99%	1,002.4	µg/mL	+/-	36.4711
56	4-Bromophenyl phenyl ether	101-55-3	STBH6361	99%	1,008.8	µg/mL	+/-	36.7031
57	Hexachlorobenzene	118-74-1	15458400	99%	1,005.1	µg/mL	+/-	36.5712
58	Pentachlorophenol	87-86-5	RP240517RSR	99%	1,005.9	µg/mL	+/-	36.5984
59	Phenanthrene	85-01-8	MKCT3391	99%	1,004.9	µg/mL	+/-	36.5621
60	Anthracene	120-12-7	101492T18R	99%	1,005.1	µg/mL	+/-	36.5712
61	Carbazole	86-74-8	15276700	99%	1,005.4	µg/mL	+/-	36.5803
62	Di-n-butylphthalate	84-74-2	MKCN4337	99%	1,006.3	µg/mL	+/-	36.6121
63	Fluoranthene	206-44-0	MKCQ4728	99%	1,003.5	µg/mL	+/-	36.5120
64	Pyrene	129-00-0	BCCK2592	99%	1,002.0	µg/mL	+/-	36.4575
65	Benzyl butyl phthalate	85-68-7	X12I018	99%	1,007.5	µg/mL	+/-	36.6576
66	Bis(2-ethylhexyl)adipate	103-23-1	MKCM1988	99%	1,005.9	µg/mL	+/-	36.5984
67	Benz(a)anthracene	56-55-3	I70012022BAA	99%	1,005.5	µg/mL	+/-	36.5848
68	Chrysene	218-01-9	RP241007RSR	99%	1,005.3	µg/mL	+/-	36.5757
69	Bis(2-ethylhexyl)phthalate	117-81-7	MKCS8065	99%	1,007.5	µg/mL	+/-	36.6576
70	Di-n-octyl phthalate	117-84-0	15566400	99%	1,002.3	µg/mL	+/-	36.4666
71	Benzo(b)fluoranthene	205-99-2	052013B	99%	1,004.1	µg/mL	+/-	36.5348
72	Benzo(k)fluoranthene	207-08-9	012022K	99%	1,002.8	µg/mL	+/-	36.4847
73	Benzo(a)pyrene	50-32-8	NQLXA	98%	1,006.2	µg/mL	+/-	36.6108
74	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	97%	1,001.8	µg/mL	+/-	36.4490
75	Dibenz(a,h)anthracene	53-70-3	2-ASA-59-1	99%	1,003.3	µg/mL	+/-	36.5029
76	Benzo(g,h,i)perylene	191-24-2	RP241014RSR	98%	1,003.8	µg/mL	+/-	36.5217

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Methylene chloride

**CAS #** 75-09-2

**Purity** 99%

#### Tech Tips:

N-Nitrosodiphenylamine (86-30-6) is prone to breakdown in the injection port and will be converted to Diphenylamine (122-39-4). When comparing the response of Diphenylamine to mixtures manufactured using N-Nitrosodiphenylamine, a difference in response will be observed. The ratio of the MW can be used to calculate the theoretical concentration of the N-Nitrosodiphenylamine.





5580 Skylane Blvd  
Santa Rosa, CA 95403

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.:	Storage:	Solvent:	Exp. Date:	Description:	
Z-110816-01 531243	≤ -10 °C	Methylene Chloride	1/2/2030	Custom 8270 Mix, 4-79, 1000 mg/L, 1 mL	
Compound		CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
atrazine		1912-24-9	99.5	337.7.4P	997 ± 5.81
benzidine		92-87-5	99.9	124.18.6.2P	993.8 ± 5.78
caprolactam		105-60-2	99.9	271.1.6P	999 ± 5.82

SI3057 } AC  
↓ SI3061 } 1/16/25

\*Not a certified value  
Manufactured by o2si smart solutions, Accredited to ISO 9001:2008 by NSF and ISO/IEC 17025:2005 (Certification No. 3031.01) and ISO Guide 34:2009 (Certification No. 3031.02) by A2LA

Certified By:

Melissa Workoff  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



# SHIPPING DOCUMENTS

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18

**CHEMTECH**  
CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092

(908) 789-8900 Fax: (908) 78-8922  
www.chemtech.net

Chemtech Project Number: Q2375

COC Number:

CLIENT INFORMATION		PROJECT INFORMATION				BILLING INFORMATION												
COMPANY: Tetra Tech ADDRESS: 4433 Corporation Ln, Suite 300 CITY: Virginia Beach STATE: VA ZIP: 23462 ATTENTION: Ernie Wu PHONE: 757-466-4901 FAX: 757-461-4148		PROJECT NAME: NWIRP Bethpage PROJECT #: 112G08005-WE13 LOCATION: RW8 PROJECT MANAGER: Ernie Wu E-MAIL: ernie.wu@tetrach.com PHONE: 757-466-4901 FAX: 757-461-4148				BILL TO: PO# ADDRESS: CITY: STATE: ZIP: ATTENTION: PHONE:												
DATA TURNAROUND INFORMATION		DATA DELIVERABLE INFORMATION				ANALYSIS												
FAX: 10 DAYS* HARD COPY: 10 DAYS* EDD 10 DAYS* * TO BE APPROVED BY CHEMTECH STANDARD TURNAROUND TIME IS 10 BUSINESS DAYS		<input type="checkbox"/> RESEULTS ONLY <input type="checkbox"/> USEPA CLP <input type="checkbox"/> RESULTS + QC <input type="checkbox"/> New York State ASP "B" <input type="checkbox"/> New Jersey REDUCED <input type="checkbox"/> New York State ASP "A" <input type="checkbox"/> New Jersey CLP <input type="checkbox"/> Other _____ <input type="checkbox"/> EDD Format _____				14-Dioxane SW846 8270 SIM    Iron, Total    TSS    TDS 1 2 3 4 5 6 7 8 9												
PROJECT SAMPLE IDENTIFICATION		SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles	PRESERVATIVES									COMMENTS	
CHEMTECH SAMPLE ID	COMP		GRAB	DATE	TIME	B		1	2	3	4	5	6	7	8	9	<-- Specify Preservatives A-HCl    B-HNO3 C-H2SO4    D-NaOH E-ICE    F-Other	
1.	RW8-SP100-20250619	GW	X	6/19/25	13:05	4	X	X	X	X						pH 1.3 # 80A0441		
2.	RW8-SP303-20250619	GW	X	6/19/25	13:13	4	X	X	X	X						pH 1.3 # 80A0441		
3.																		
4.																		
5.																		
6.																		
7.																		
8.																		
9.																		
10.																		
SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE PROSSESSION INCLUDING COURIER DELIVERY																		
RELINQUISHED BY SAMPLER <i>U. H. L.</i>	DATE/TIME 6/19/25 15:00	RECEIVED BY <i>1. S. S.</i>	1553	Conditions of bottles or coolers at receipt: <input type="checkbox"/> Compliant <input type="checkbox"/> Non Compliant <input type="checkbox"/> Cooler Temp 22°C MeOH extraction requires an additional 4oz. Jar for percent solid Comments:														
RELINQUISHED BY <i>2.</i>	DATE/TIME 6/19/25	RECEIVED BY <i>2.</i>	6-19-25															
RELINQUISHED BY <i>3.</i>	DATE/TIME 6/19/25	RECEIVED FOR LAB BY <i>3.</i>	183	Page _____ of _____				SHIPPED VIA: CLIENT: <input type="checkbox"/> Hand Delivered <input type="checkbox"/> Overnight CHEMTECH: <input type="checkbox"/> Picked Up <input type="checkbox"/> Overnight				Shipment Complete <input type="checkbox"/> YES <input type="checkbox"/> NO						
WHITE - CHEMTECH COPY FOR RETURN TO CLIENT				YELLOW - CHEMTECH COPY				PINK - SAMPLER COPY										

### Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037355.D  
 Acq On : 20 Jun 2025 18:03  
 Operator : RC/JU  
 Sample : SSTDICCC0.4  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**SSTDICCC0.4**

Quant Time: Jun 20 23:26:55 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1912	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4157	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2811	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5776	0.400	ng	# 0.00
29) Chrysene-d12	21.171	240	4813	0.400	ng	# 0.00
35) Perylene-d12	23.354	264	4943	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1436	0.411	ng	0.00
5) Phenol-d6	6.752	99	1465	0.424	ng	0.00
8) Nitrobenzene-d5	8.717	82	1327	0.385	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	2768	0.411	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	646	0.321	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	4996	0.405	ng	0.00
27) Fluoranthene-d10	19.008	212	6705	0.373	ng	0.00
31) Terphenyl-d14	19.616	244	4452	0.405	ng	0.00
<b>Target Compounds</b>						
					<b>Qvalue</b>	
2) 1,4-Dioxane	3.104	88	745	0.441	ng	94
3) n-Nitrosodimethylamine	3.422	42	754	0.383	ng	81
6) bis(2-Chloroethyl)ether	7.004	93	1351	0.446	ng	94
9) Naphthalene	10.394	128	4347	0.403	ng	# 89
10) Hexachlorobutadiene	10.682	225	1832	0.348	ng	# 99
12) 2-Methylnaphthalene	12.021	142	2957	0.390	ng	92
16) Acenaphthylene	13.935	152	4490	0.381	ng	99
17) Acenaphthene	14.277	154	2983	0.381	ng	98
18) Fluorene	15.272	166	4232	0.382	ng	100
20) 4,6-Dinitro-2-methylph...	15.368	198	459	0.263	ng	89
21) 4-Bromophenyl-phenylether	16.165	248	1611	0.342	ng	# 85
22) Hexachlorobenzene	16.276	284	1814	0.369	ng	98
23) Atrazine	16.450	200	1262	0.342	ng	# 85
24) Pentachlorophenol	16.624	266	792	0.293	ng	98
25) Phenanthrene	17.009	178	6374	0.391	ng	99
26) Anthracene	17.108	178	5717	0.375	ng	98
28) Fluoranthene	19.040	202	7896	0.354	ng	# 98
30) Pyrene	19.402	202	7990	0.434	ng	100
32) Benzo(a)anthracene	21.153	228	5851	0.377	ng	98
33) Chrysene	21.207	228	7754	0.394	ng	98
34) Bis(2-ethylhexyl)phtha...	21.099	149	2603	0.409	ng	98
36) Indeno(1,2,3-cd)pyrene	25.541	276	8379	0.400	ng	# 93
37) Benzo(b)fluoranthene	22.746	252	7755	0.442	ng	95
38) Benzo(k)fluoranthene	22.746	252	7755	0.407	ng	95
39) Benzo(a)pyrene	23.257	252	6298	0.393	ng	# 92
40) Dibenzo(a,h)anthracene	25.555	278	6108	0.366	ng	# 88
41) Benzo(g,h,i)perylene	26.204	276	7852	0.408	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037355.D  
 Acq On : 20 Jun 2025 18:03  
 Operator : RC/JU  
 Sample : SSTDICCC0.4  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICCC0.4


Quant Time: Jun 20 23:26:55 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:25:11 2025  
 Response via : Initial Calibration

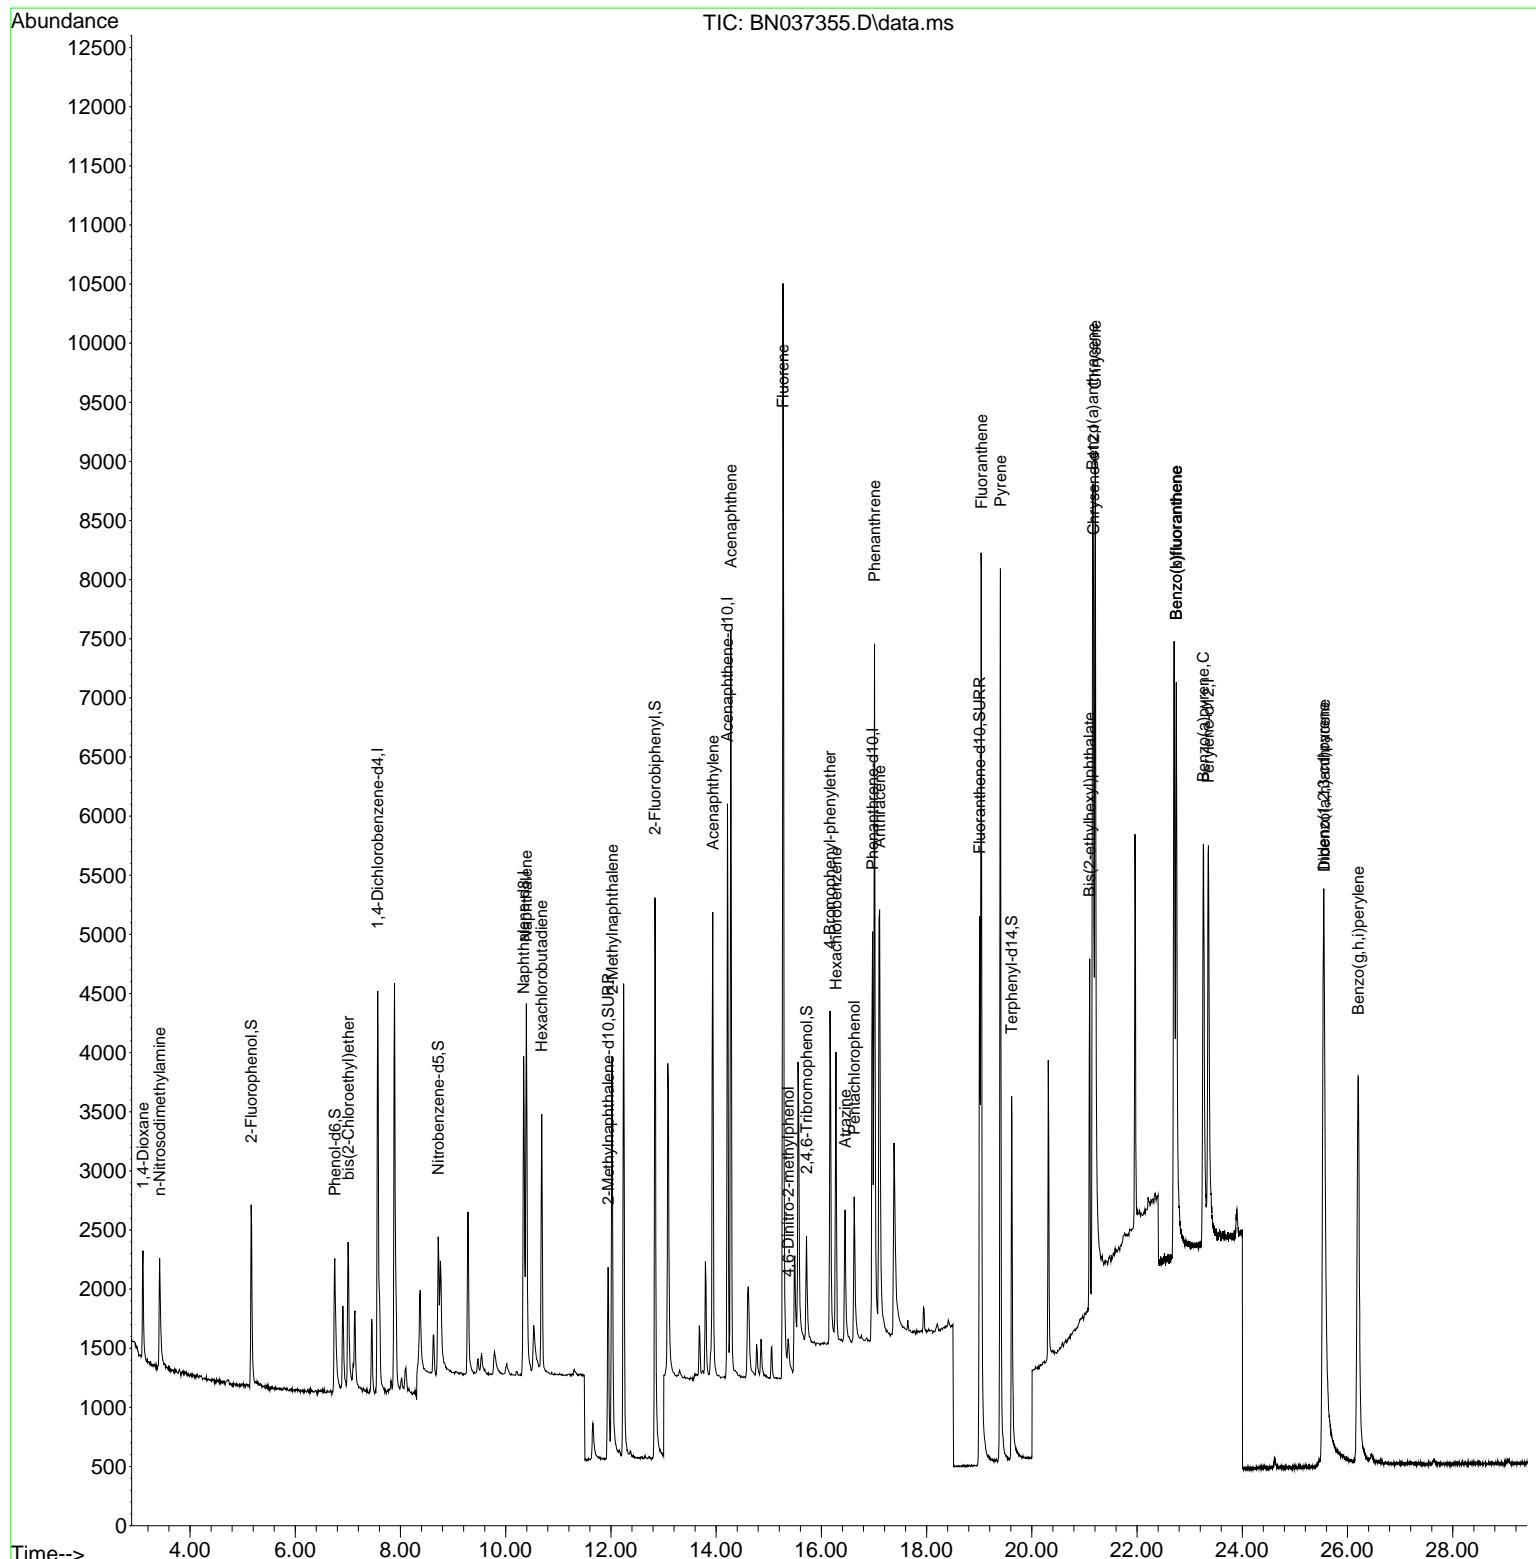






#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 64  
Delta R.T. -0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4





Tgt Ion:152 Resp: 1912  
Ion Ratio Lower Upper  
152 100  
150 147.0 112.7 169.1  
115 53.9 45.9 68.9






#2  
1,4-Dioxane  
Concen: 0.441 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03



Tgt Ion: 88 Resp: 745  
Ion Ratio Lower Upper  
88 100  
43 26.3 21.0 31.6  
58 54.1 38.0 57.0



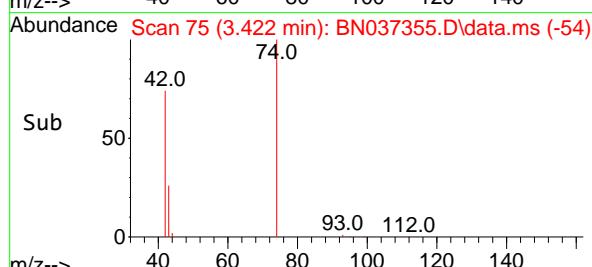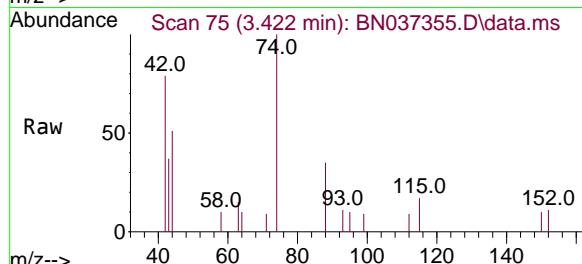

#3

n-Nitrosodimethylamine

Concen: 0.383 ng

RT: 3.422 min Scan# 7

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N

ClientSampleId :

SSTDICCC0.4

Tgt Ion: 42 Resp: 754





Ion Ratio Lower Upper

42 100

74 126.4 84.3 126.5

44 5.7 5.0 7.4

Abundance

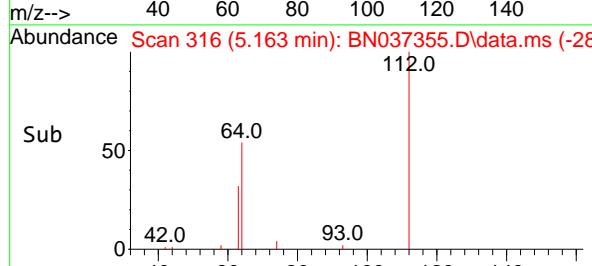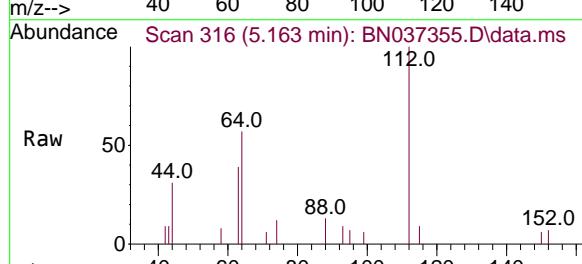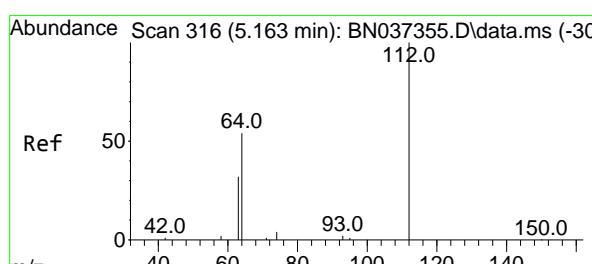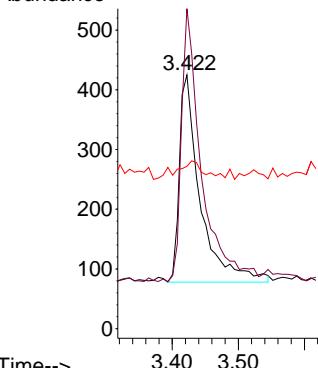

#4

2-Fluorophenol

Concen: 0.411 ng

RT: 5.163 min Scan# 316

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Tgt Ion: 112 Resp: 1436


Ion Ratio Lower Upper


112 100

64 49.6 38.7 58.1

63 31.1 26.4 39.6


Abundance

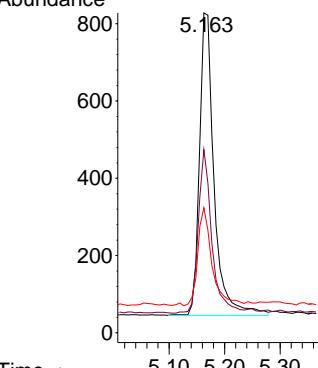






#5  
 Phenol-d6  
 Concen: 0.424 ng  
 RT: 6.752 min Scan# 5  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4

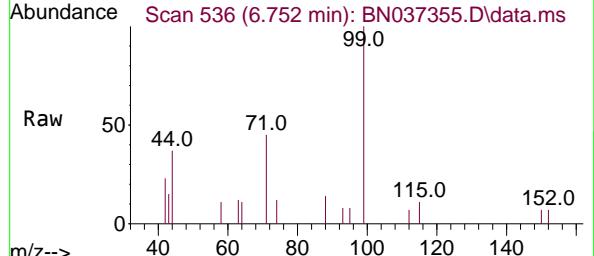



Tgt Ion: 99 Resp: 1465  
 Ion Ratio Lower Upper  
 99 100  
 42 17.0 19.8 29.8#  
 71 43.2 42.6 64.0

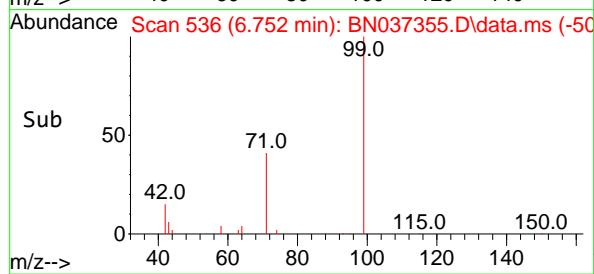


#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.446 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

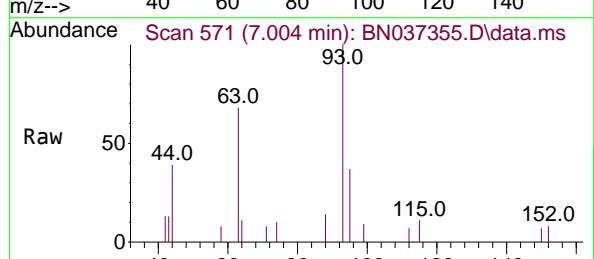


Tgt Ion: 93 Resp: 1351  
 Ion Ratio Lower Upper  
 93 100  
 63 60.9 53.2 79.8  
 95 31.1 27.3 40.9








#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 942  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4

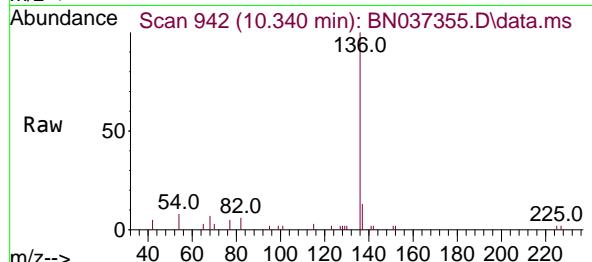



Tgt Ion:136 Resp: 4157  
 Ion Ratio Lower Upper  
 136 100  
 137 12.9 12.2 18.2  
 54 8.1 8.8 13.2#  
 68 6.6 7.0 10.4#

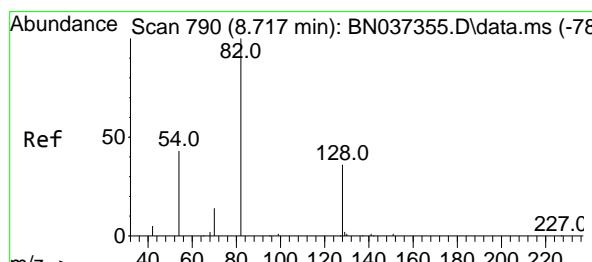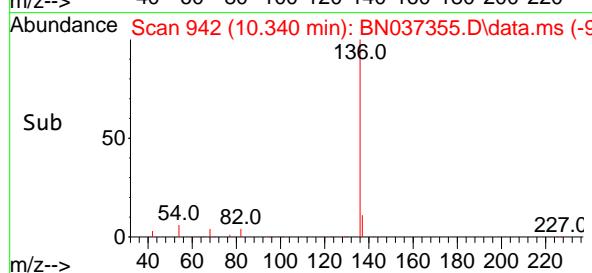


#8  
 Nitrobenzene-d5  
 Concen: 0.385 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

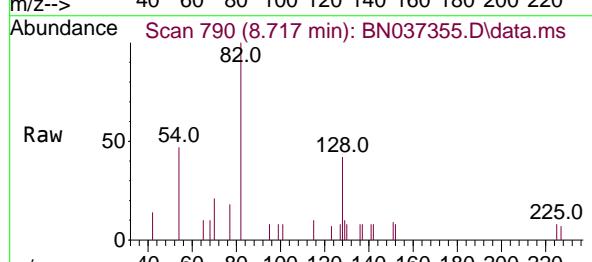


Tgt Ion: 82 Resp: 1327  
 Ion Ratio Lower Upper  
 82 100  
 128 41.8 42.5 63.7#  
 54 47.4 43.2 64.8

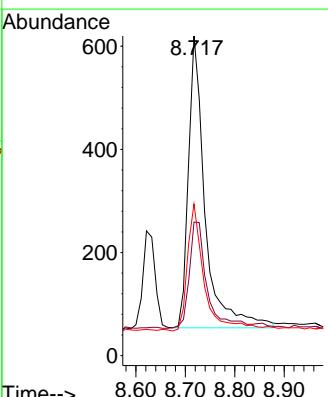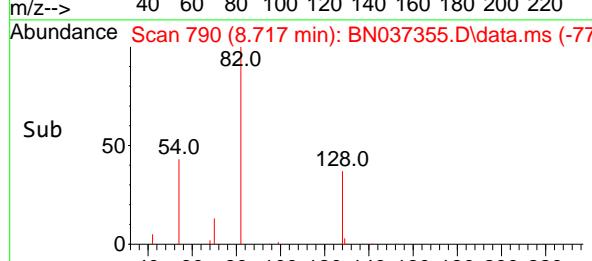






#9  
Naphthalene  
Concen: 0.403 ng  
RT: 10.394 min Scan# 947  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4

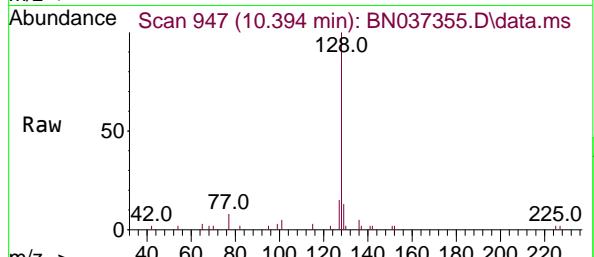



Tgt Ion:128 Resp: 4347  
Ion Ratio Lower Upper  
128 100  
129 12.5 14.0 21.0#  
127 14.9 15.8 23.8#

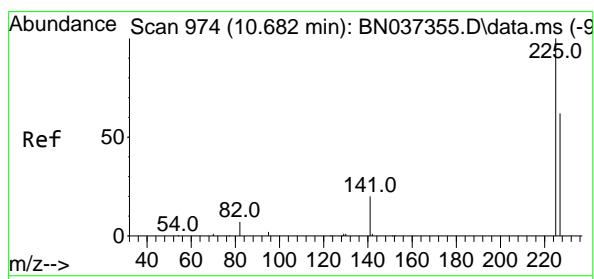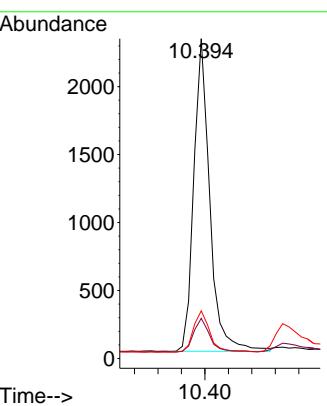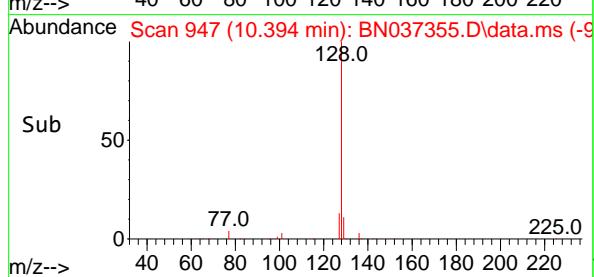


#10  
Hexachlorobutadiene  
Concen: 0.348 ng  
RT: 10.682 min Scan# 974  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

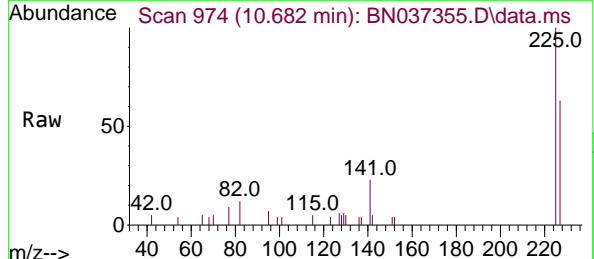


Tgt Ion:225 Resp: 1832  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 62.4 50.3 75.5


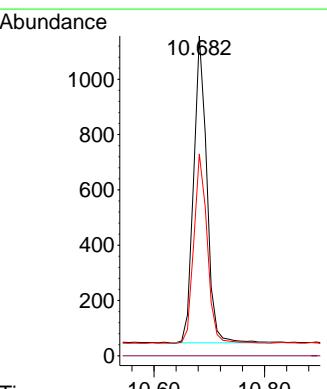
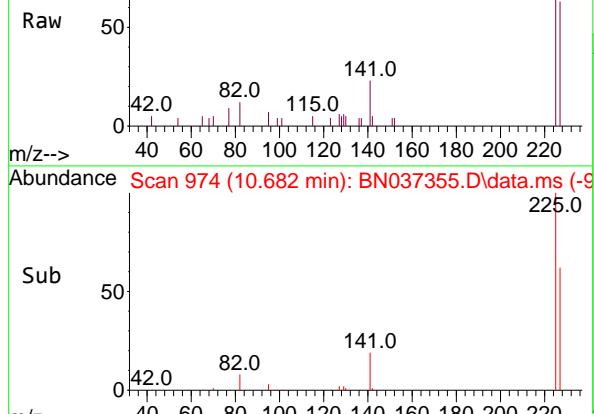





#11  
2-Methylnaphthalene-d10  
Concen: 0.411 ng  
RT: 11.945 min Scan# 1:Instrument :  
Delta R.T. 0.000 min BNA\_N  
Lab File: BN037355.D ClientSampleId :  
Acq: 20 Jun 2025 18:03 SSTDICCC0.4

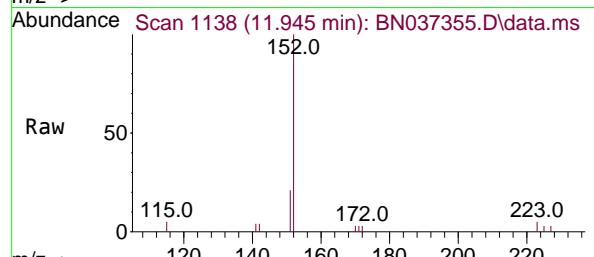



Tgt Ion:152 Resp: 2768  
Ion Ratio Lower Upper  
152 100  
151 21.9 17.4 26.0

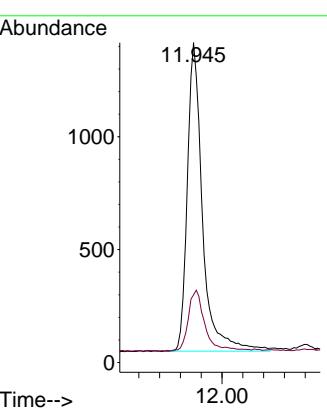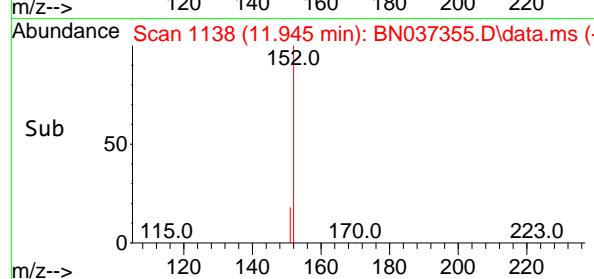


#12  
2-Methylnaphthalene  
Concen: 0.390 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03



Tgt Ion:142 Resp: 2957  
Ion Ratio Lower Upper  
142 100  
141 91.8 70.2 105.2  
115 44.5 43.0 64.4

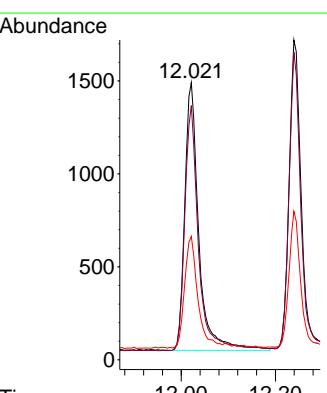



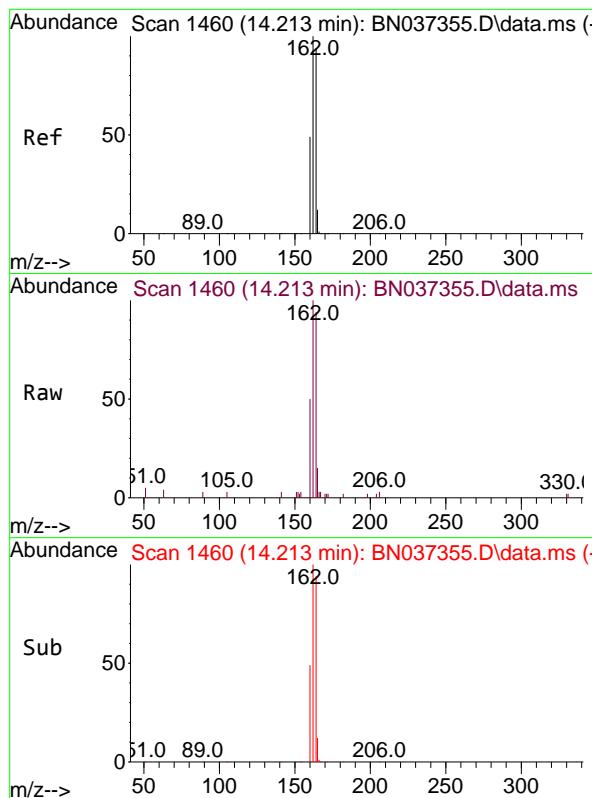

#13  
 Acenaphthene-d10  
 Concen: 0.400 ng  
 RT: 14.213 min Scan# 14  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:164 Resp: 2811  
 Ion Ratio Lower Upper  
 164 100  
 162 106.2 81.5 122.3  
 160 52.8 43.0 64.4

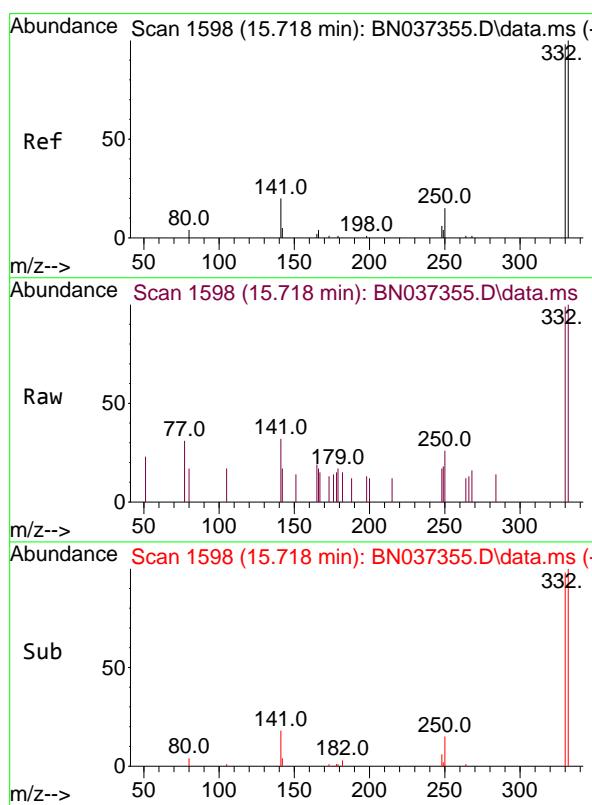

#14  
 2,4,6-Tribromophenol  
 Concen: 0.321 ng  
 RT: 15.718 min Scan# 1598  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03



Tgt Ion:330 Resp: 646  
 Ion Ratio Lower Upper  
 330 100  
 332 96.3 78.4 117.6  
 141 29.6 24.4 36.6

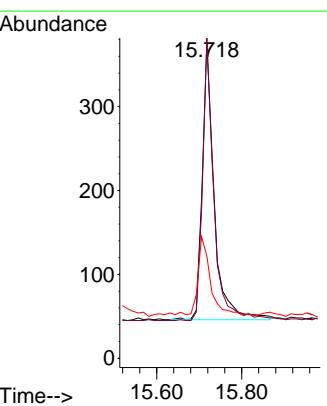

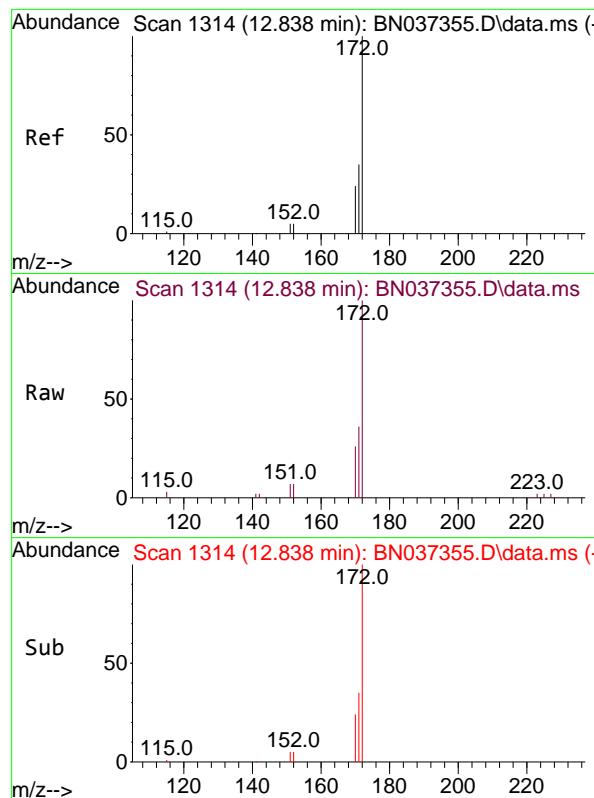


#15  
2-Fluorobiphenyl  
Concen: 0.405 ng  
RT: 12.838 min Scan# 1:Instrument :  
Delta R.T. 0.000 min BNA\_N  
Lab File: BN037355.D ClientSampleId :  
Acq: 20 Jun 2025 18:03 SSTDICCC0.4


Tgt Ion:172 Resp: 4996  
Ion Ratio Lower Upper  
172 100  
171 36.2 30.8 46.2  
170 25.6 21.9 32.9

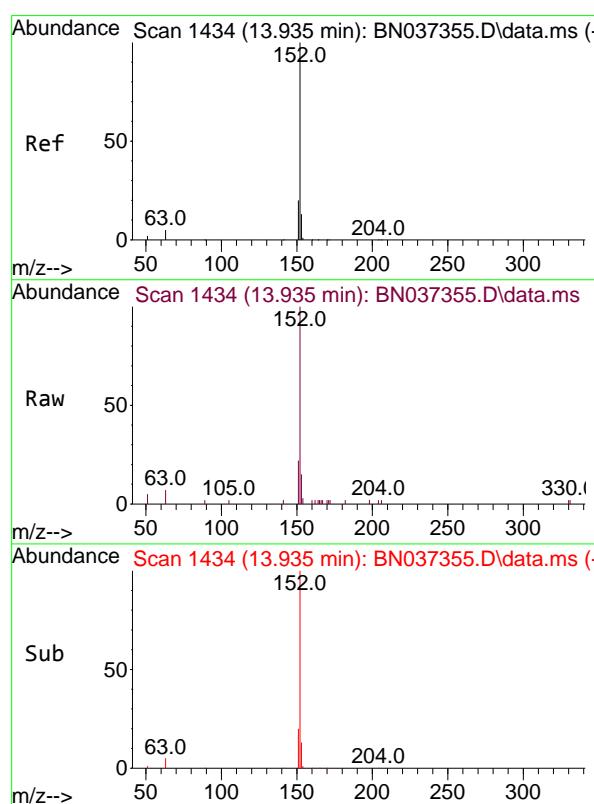


#16  
Acenaphthylene  
Concen: 0.381 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:152 Resp: 4490  
Ion Ratio Lower Upper  
152 100  
151 20.3 16.6 24.8  
153 13.1 10.2 15.2









#17  
 Acenaphthene  
 Concen: 0.381 ng  
 RT: 14.277 min Scan# 14  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03  
**Instrument :** BNA\_N  
**ClientSampleId :** SSTDICCC0.4





Tgt Ion:154 Resp: 2983  
 Ion Ratio Lower Upper  
 154 100  
 153 117.6 93.1 139.7  
 152 63.0 48.6 73.0

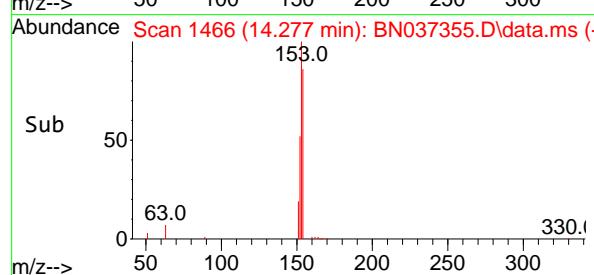


#18  
 Fluorene  
 Concen: 0.382 ng  
 RT: 15.272 min Scan# 1559  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

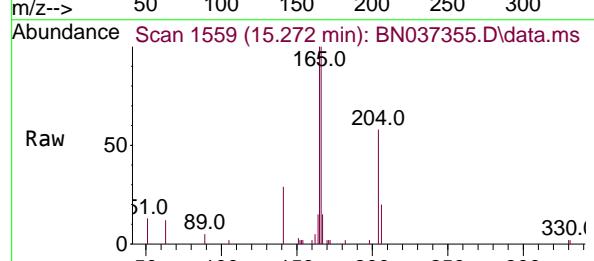

Tgt Ion:166 Resp: 4232  
 Ion Ratio Lower Upper  
 166 100  
 165 99.8 79.5 119.3  
 167 13.6 10.7 16.1

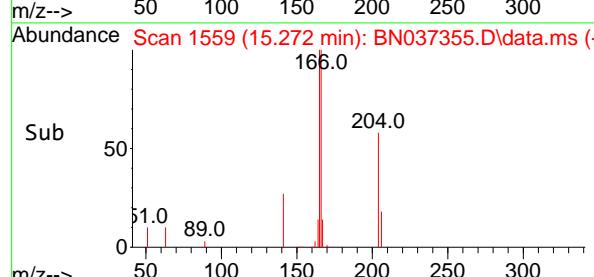



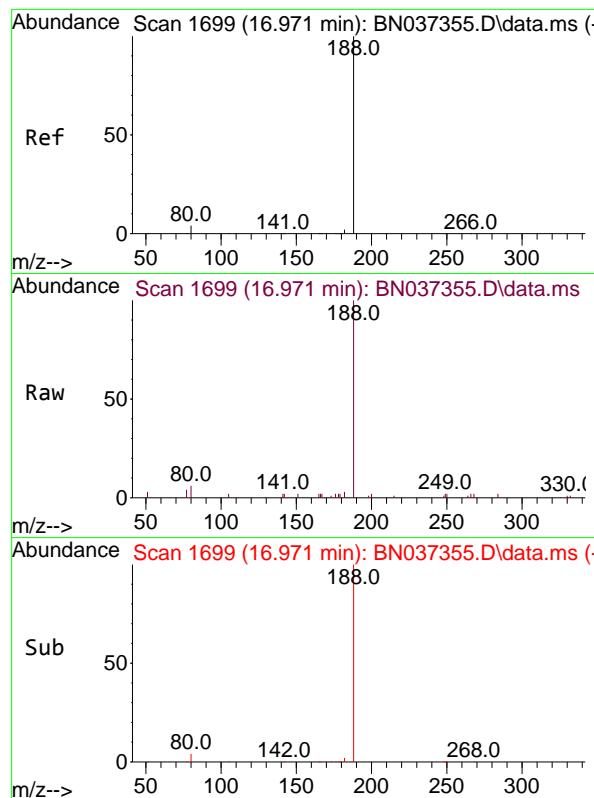

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:188 Resp: 5776  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 5.6 6.2 9.2#

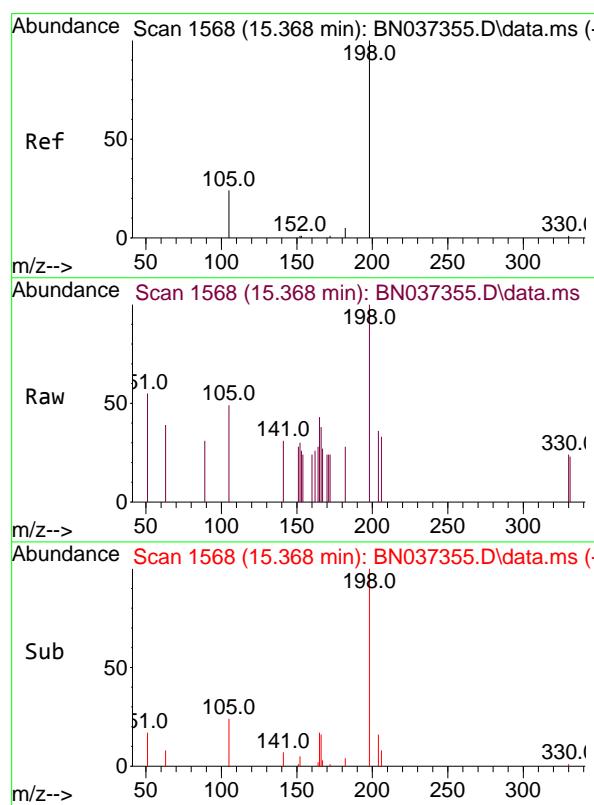

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.263 ng  
 RT: 15.368 min Scan# 1568  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03



Tgt Ion:198 Resp: 459  
 Ion Ratio Lower Upper  
 198 100  
 51 55.4 51.4 77.0  
 105 49.2 45.5 68.3

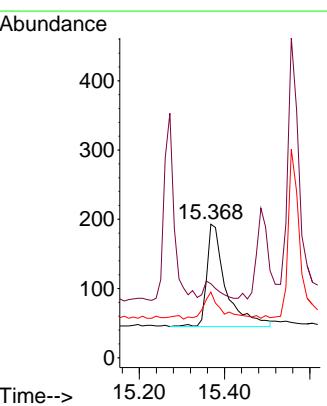

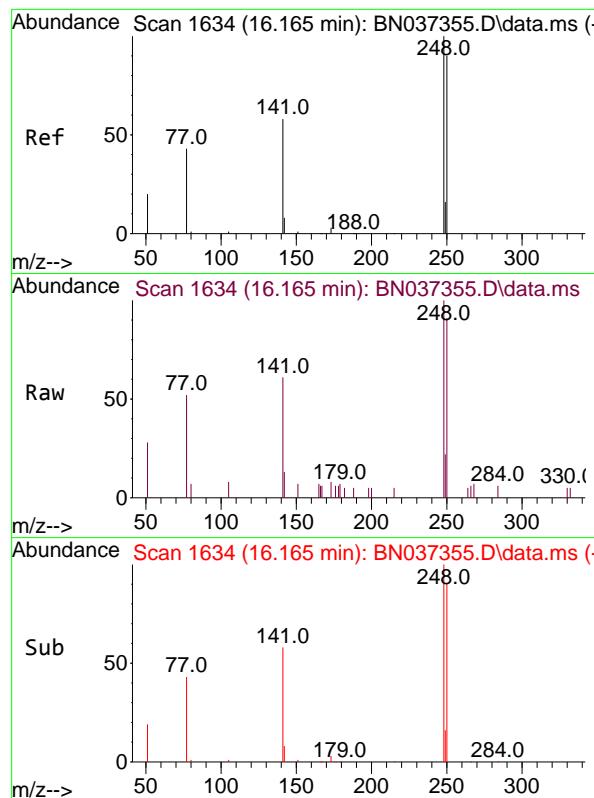


#21  
4-Bromophenyl-phenylether  
Concen: 0.342 ng  
RT: 16.165 min Scan# 1  
Instrument: BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037355.D ClientSampleId : SSTDICCC0.4  
Acq: 20 Jun 2025 18:03


Tgt Ion:248 Resp: 1611  
Ion Ratio Lower Upper  
248 100  
250 91.4 80.4 120.6  
141 61.2 33.3 49.9#

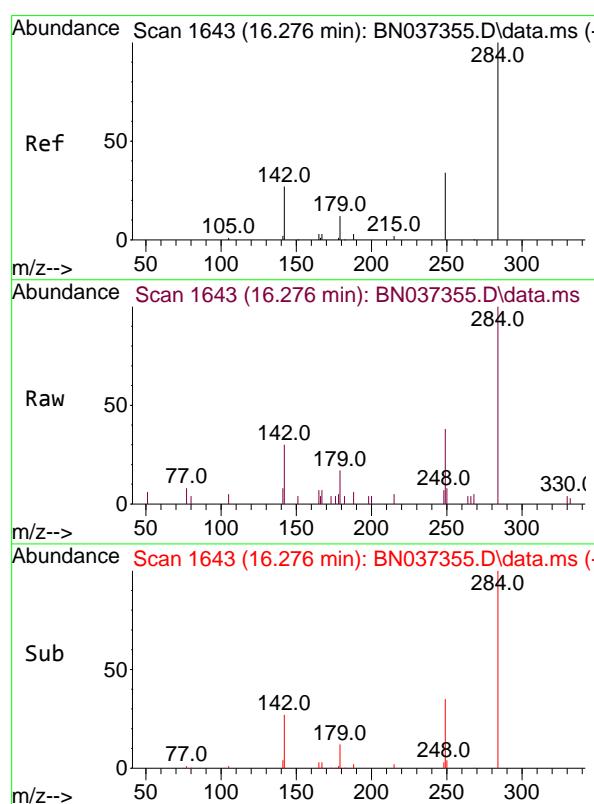

#22  
Hexachlorobenzene  
Concen: 0.369 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:284 Resp: 1814  
Ion Ratio Lower Upper  
284 100  
142 34.2 27.0 40.6  
249 34.2 28.8 43.2


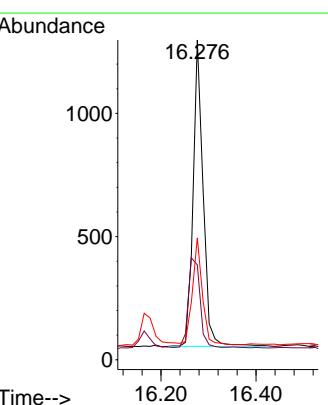


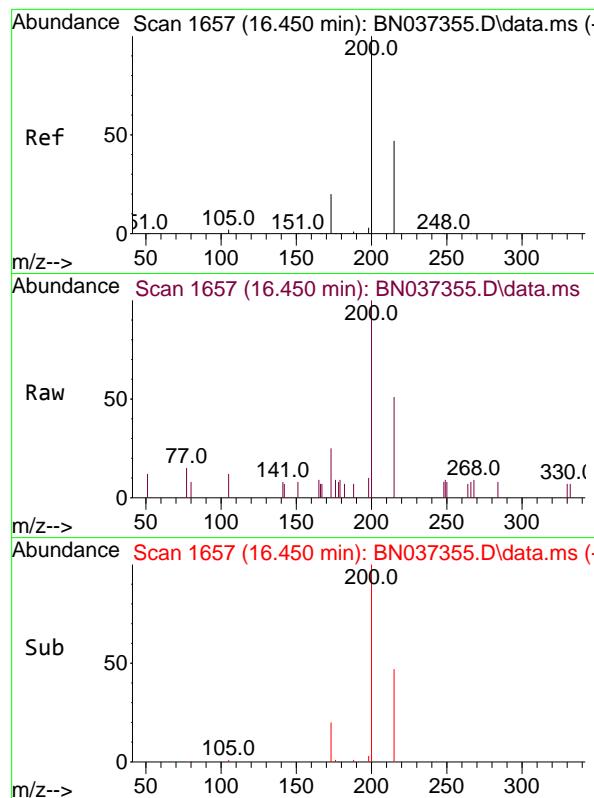

#23  
Atrazine  
Concen: 0.342 ng  
RT: 16.450 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4




Tgt Ion:200 Resp: 1262  
Ion Ratio Lower Upper  
200 100  
173 25.4 29.2 43.8#  
215 51.1 48.8 73.2

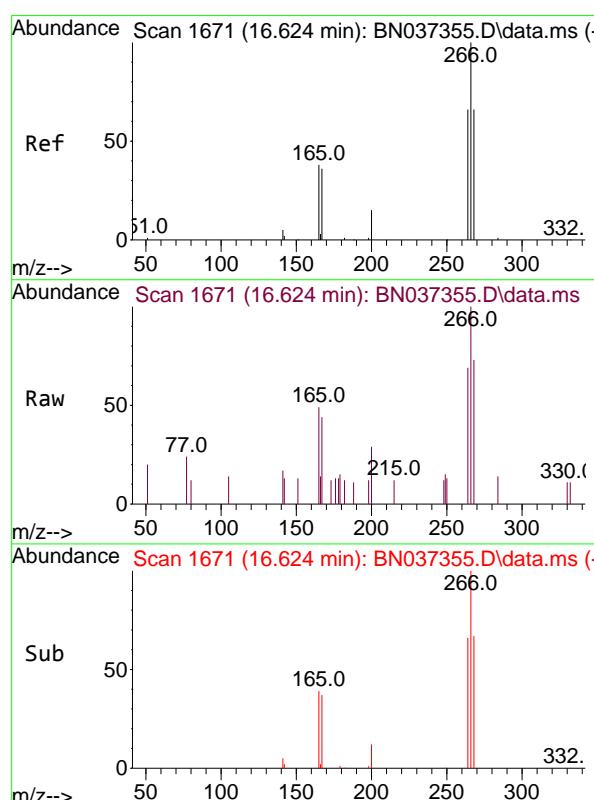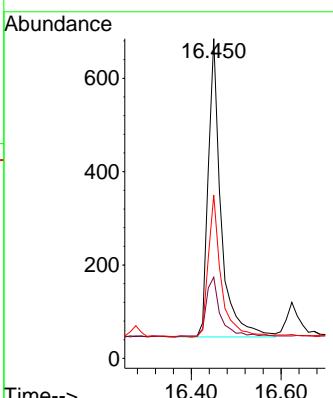

#24  
Pentachlorophenol  
Concen: 0.293 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03

Tgt Ion:266 Resp: 792  
Ion Ratio Lower Upper  
266 100  
264 64.3 50.3 75.5  
268 67.4 55.3 82.9



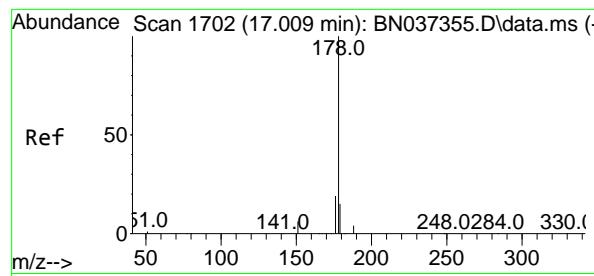

#25

Phenanthrene

Concen: 0.391 ng

RT: 17.009 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03

Instrument :

BNA\_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:178 Resp: 6374

Ion Ratio Lower Upper

178 100

176 19.7 15.2 22.8

179 15.8 12.9 19.3

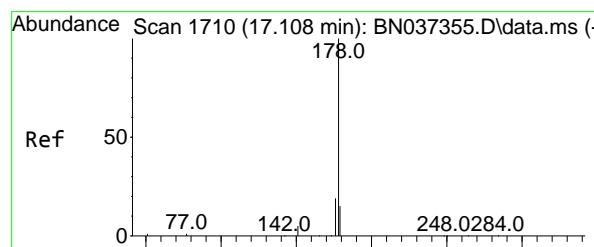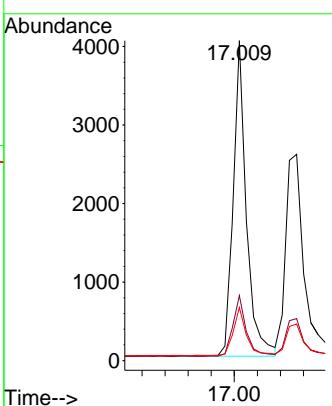

#26

Anthracene

Concen: 0.375 ng

RT: 17.108 min Scan# 1710

Delta R.T. 0.000 min

Lab File: BN037355.D

Acq: 20 Jun 2025 18:03


Tgt Ion:178 Resp: 5717


Ion Ratio Lower Upper

178 100

176 18.2 14.7 22.1

179 15.2 13.0 19.6


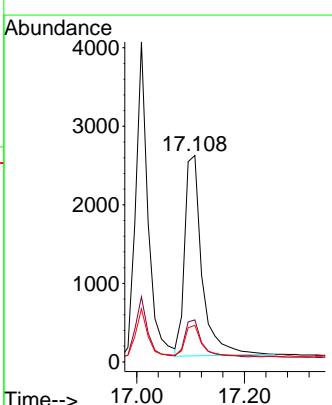


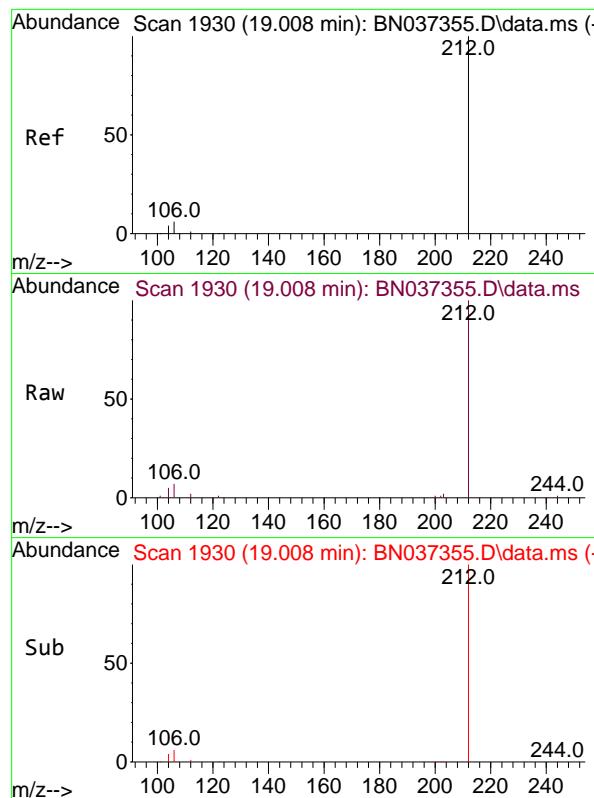

#27  
 Fluoranthene-d10  
 Concen: 0.373 ng  
 RT: 19.008 min Scan# 1930  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:212 Resp: 6705  
 Ion Ratio Lower Upper  
 212 100  
 106 5.8 3.0 4.4#  
 104 3.8 2.0 3.0#

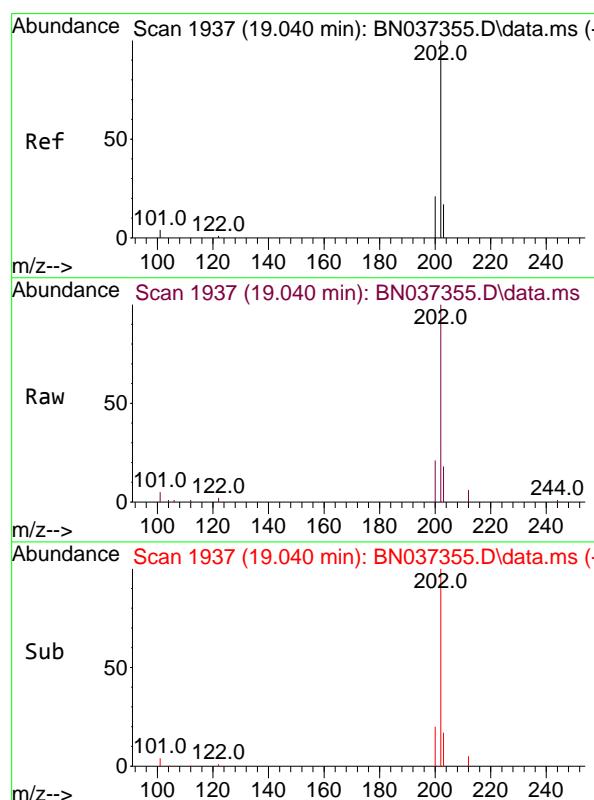

#28  
 Fluoranthene  
 Concen: 0.354 ng  
 RT: 19.040 min Scan# 1937  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

Tgt Ion:202 Resp: 7896  
 Ion Ratio Lower Upper  
 202 100  
 101 5.2 3.0 4.6#  
 203 16.6 13.7 20.5





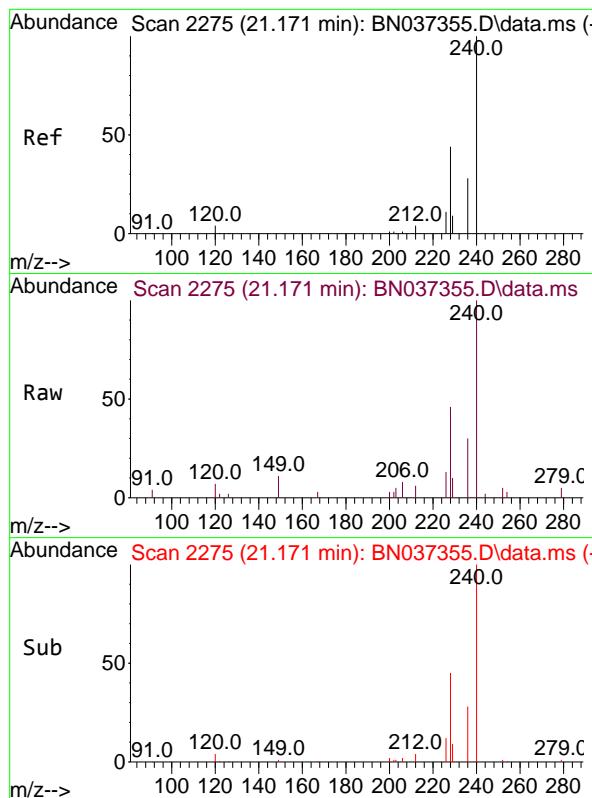

#29  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.171 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:240 Resp: 4813  
 Ion Ratio Lower Upper  
 240 100  
 120 6.9 7.5 11.3#  
 236 29.5 24.9 37.3

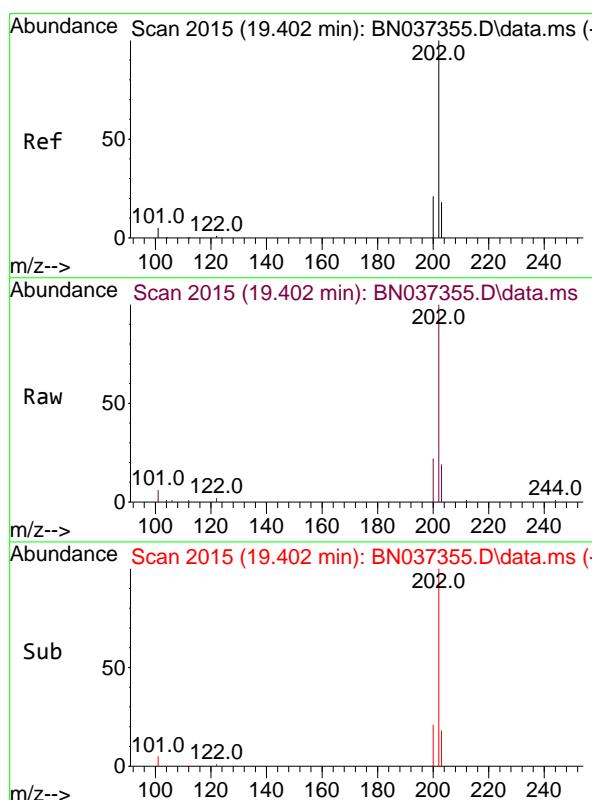

#30  
 Pyrene  
 Concen: 0.434 ng  
 RT: 19.402 min Scan# 2015  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

Tgt Ion:202 Resp: 7990  
 Ion Ratio Lower Upper  
 202 100  
 200 21.1 16.8 25.2  
 203 18.0 14.5 21.7





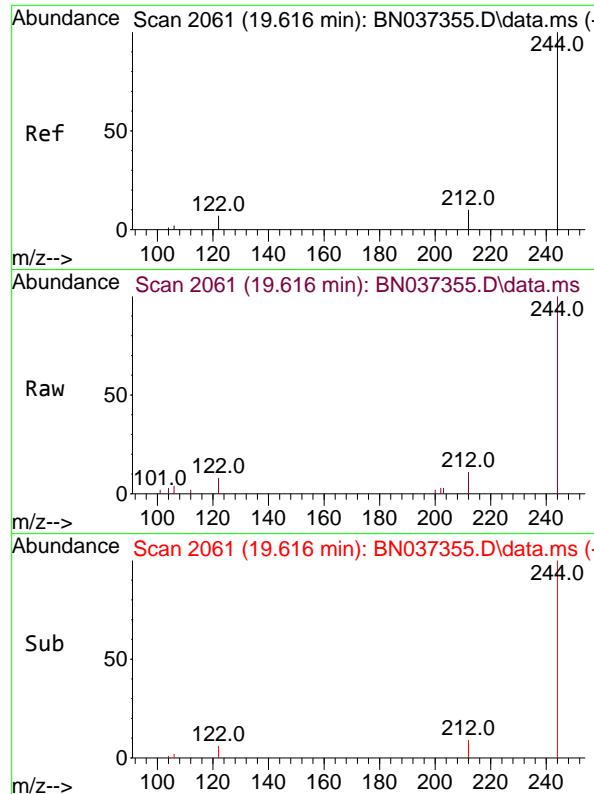

#31  
**Terphenyl-d14**  
Concen: 0.405 ng  
RT: 19.616 min Scan# 2061  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
ClientSampleId : SSTDICCC0.4


Tgt Ion:244 Resp: 4452  
Ion Ratio Lower Upper  
244 100  
212 11.4 11.1 16.7  
122 8.5 7.2 10.8

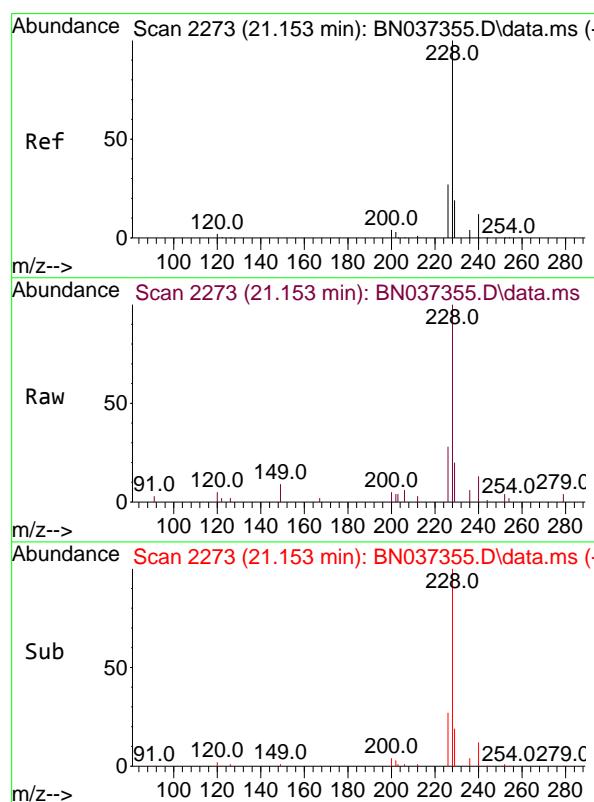

#32  
**Benzo(a)anthracene**  
Concen: 0.377 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.000 min  
Lab File: BN037355.D  
Acq: 20 Jun 2025 18:03



Tgt Ion:228 Resp: 5851  
Ion Ratio Lower Upper  
228 100  
226 28.4 23.0 34.4  
229 20.3 17.4 26.0

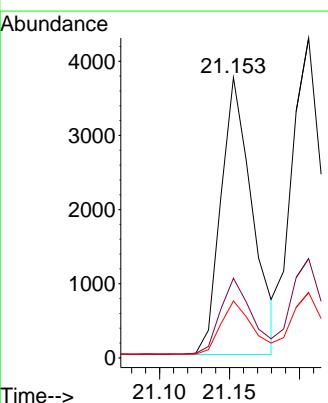

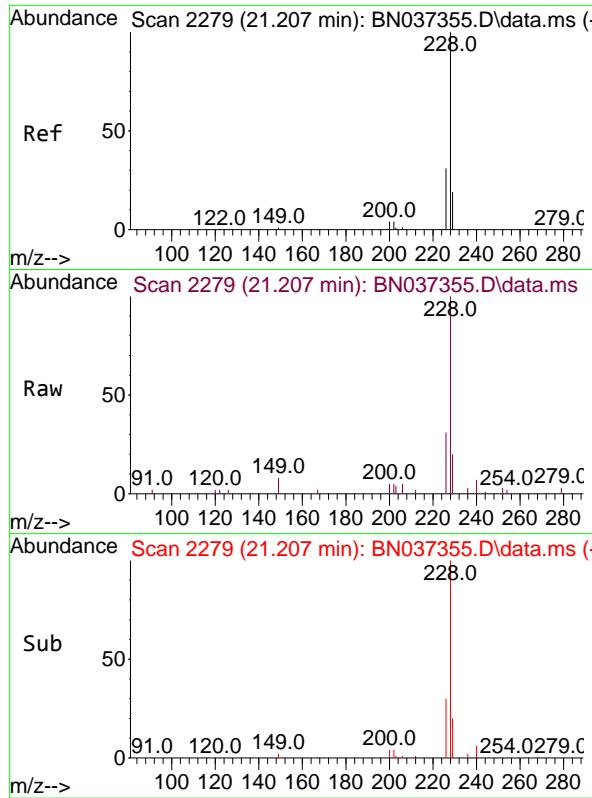


#33  
 Chrysene  
 Concen: 0.394 ng  
 RT: 21.207 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03  
**Instrument:** BNA\_N  
**ClientSampleId :** SSTDICCC0.4


Tgt Ion:228 Resp: 7754  
 Ion Ratio Lower Upper  
 228 100  
 226 31.0 25.4 38.2  
 229 20.4 17.3 25.9

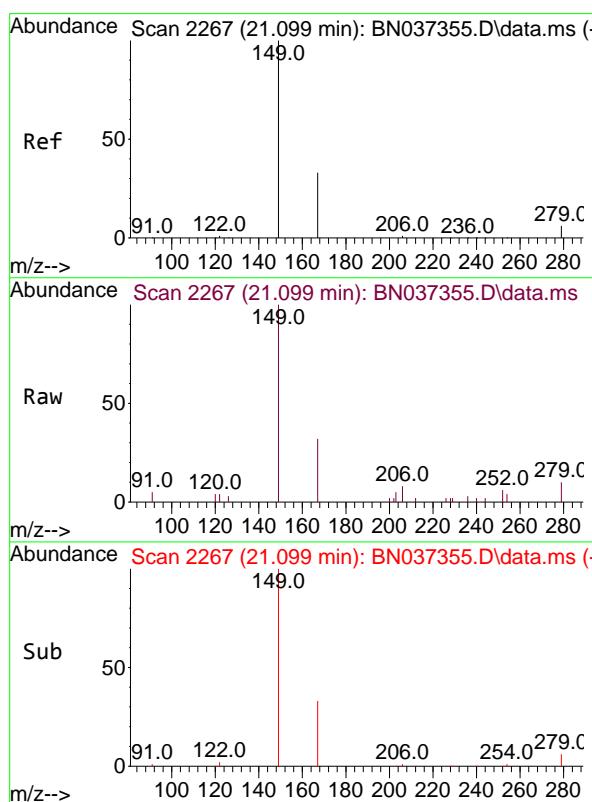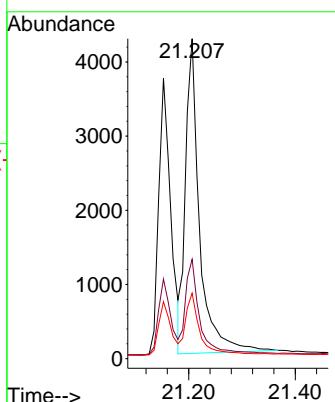

#34  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.409 ng  
 RT: 21.099 min Scan# 2267  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03



Tgt Ion:149 Resp: 2603  
 Ion Ratio Lower Upper  
 149 100  
 167 31.9 24.6 37.0  
 279 7.2 6.5 9.7



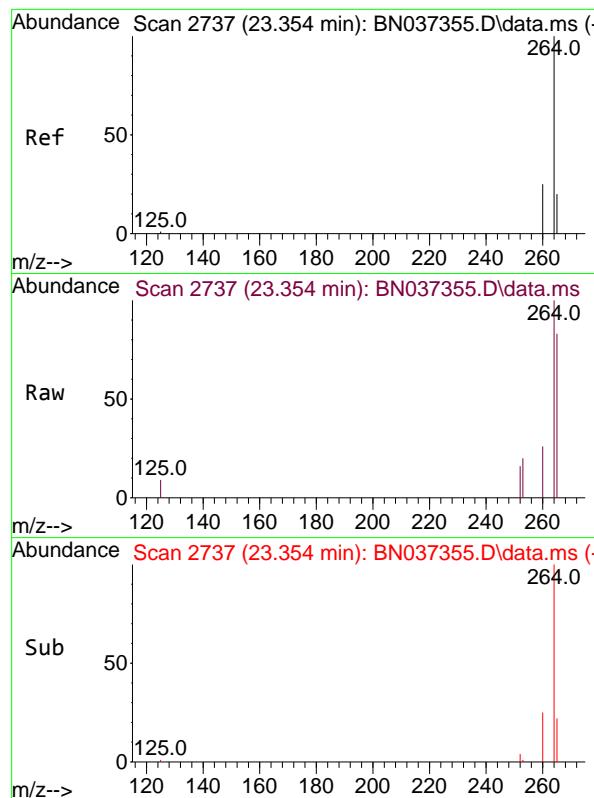


#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.354 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03  
**Instrument:** BNA\_N  
**ClientSampleId:** SSTDICCC0.4


Tgt Ion:264 Resp: 4943  
 Ion Ratio Lower Upper  
 264 100  
 260 26.5 21.4 32.2  
 265 82.6 71.4 107.0

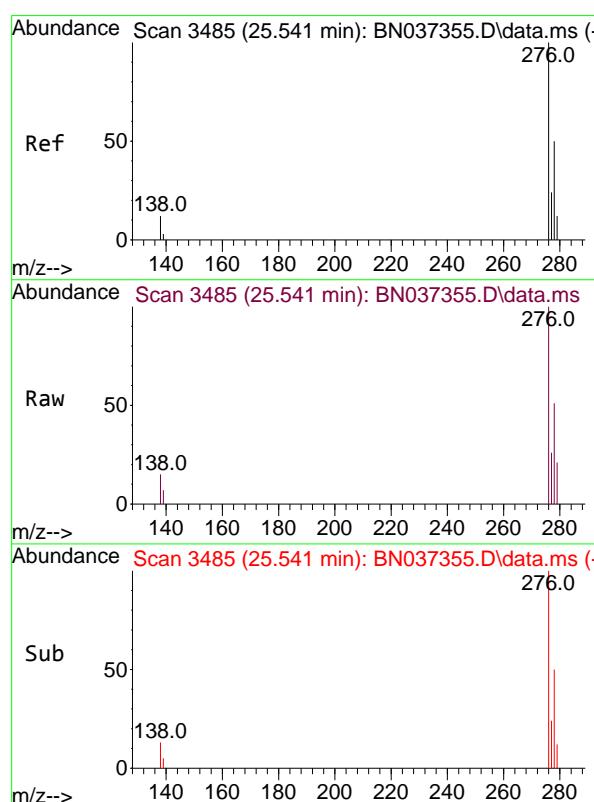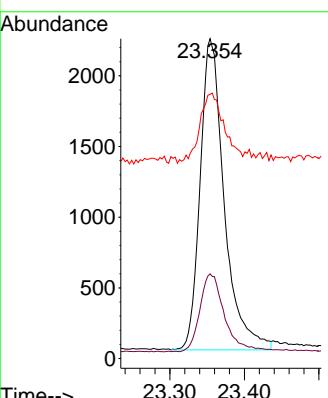

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.400 ng  
 RT: 25.541 min Scan# 3485  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

Tgt Ion:276 Resp: 8379  
 Ion Ratio Lower Upper  
 276 100  
 138 11.3 2.2 3.2#  
 277 23.4 17.1 25.7


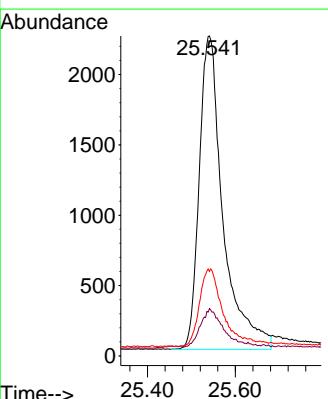


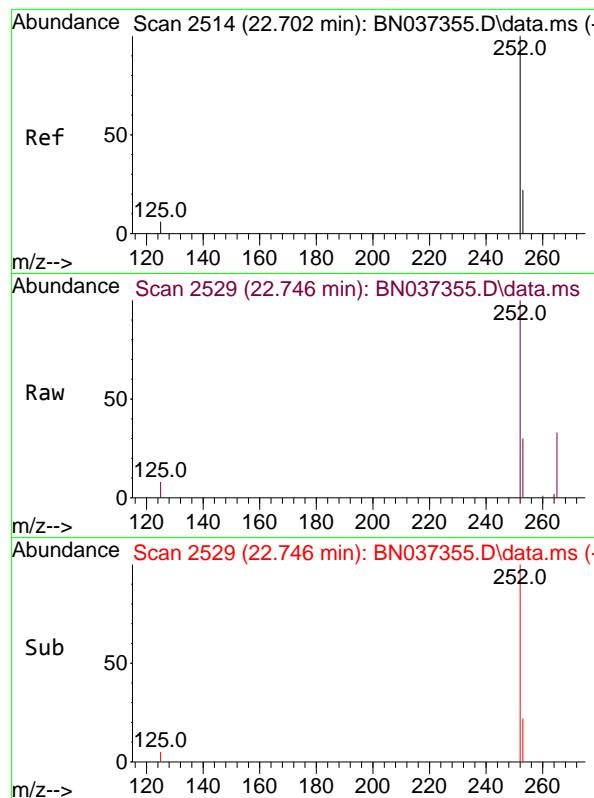

#37  
 Benzo(b)fluoranthene  
 Concen: 0.442 ng  
 RT: 22.746 min Scan# 21  
 Delta R.T. 0.044 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03


Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4


Tgt Ion:252 Resp: 7755  
 Ion Ratio Lower Upper  
 252 100  
 253 30.3 26.6 40.0  
 125 8.5 6.1 9.1

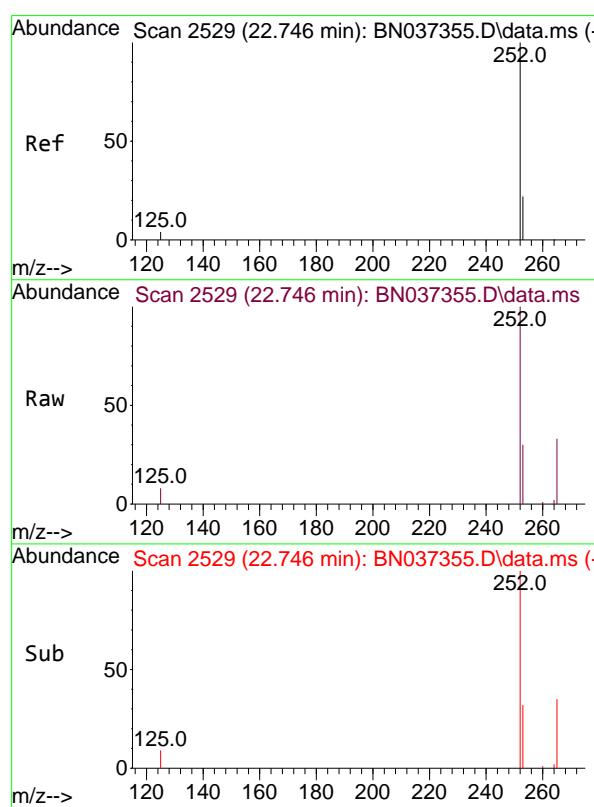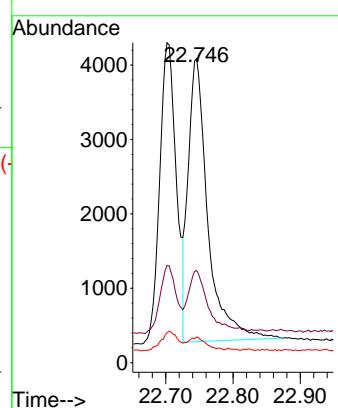

#38  
 Benzo(k)fluoranthene  
 Concen: 0.407 ng  
 RT: 22.746 min Scan# 2529  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03



Tgt Ion:252 Resp: 7755  
 Ion Ratio Lower Upper  
 252 100  
 253 30.3 26.7 40.1  
 125 8.5 6.5 9.7

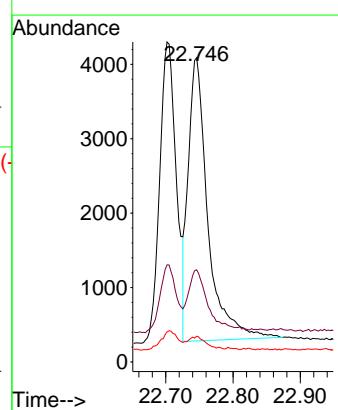

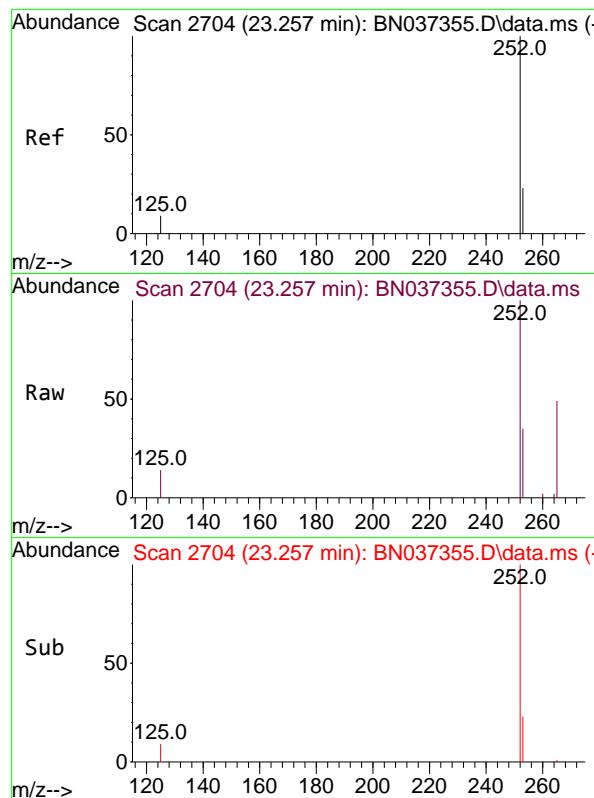


#39  
 Benzo(a)pyrene  
 Concen: 0.393 ng  
 RT: 23.257 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03  
**Instrument:** BNA\_N  
**ClientSampleId:** SSTDICCC0.4


Tgt Ion:252 Resp: 6298  
 Ion Ratio Lower Upper  
 252 100  
 253 35.2 31.6 47.4  
 125 14.0 8.4 12.6#

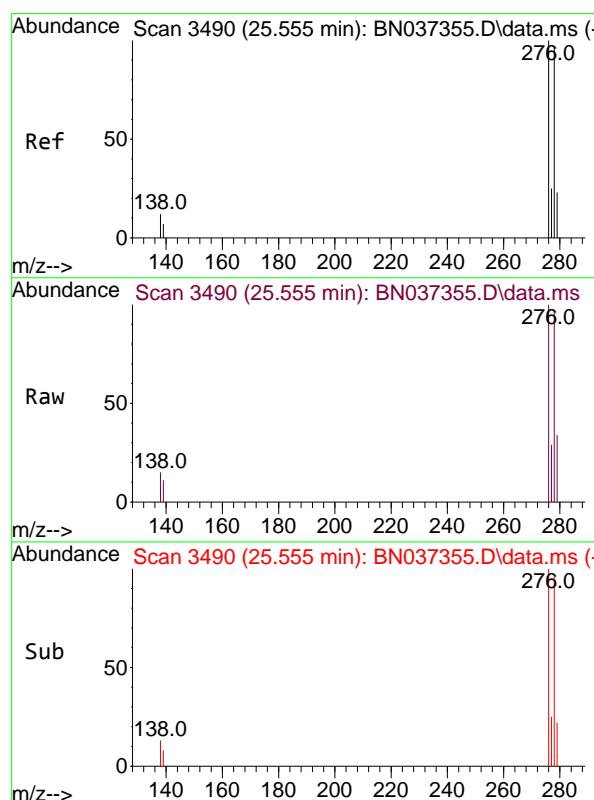

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.366 ng  
 RT: 25.555 min Scan# 3490  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

Tgt Ion:278 Resp: 6108  
 Ion Ratio Lower Upper  
 278 100  
 139 11.3 10.2 15.4  
 279 35.1 35.6 53.4#




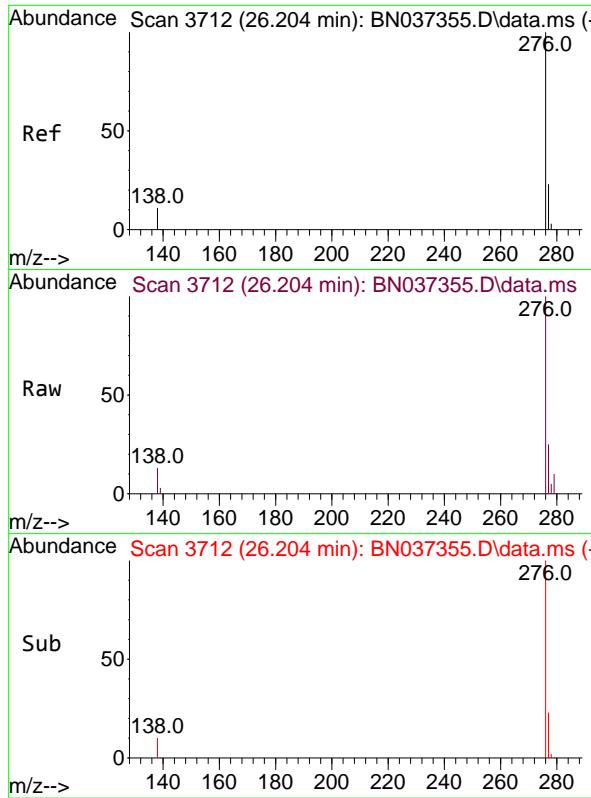

#41  
 Benzo(g,h,i)perylene  
 Concen: 0.408 ng  
 RT: 26.204 min Scan# 3  
 Delta R.T. 0.000 min  
 Lab File: BN037355.D  
 Acq: 20 Jun 2025 18:03

Instrument : BNA\_N  
 ClientSampleId : SSTDICCC0.4

Tgt Ion:276 Resp: 7852  
 Ion Ratio Lower Upper  
 276 100  
 277 25.4 22.7 34.1  
 138 12.7 9.4 14.2

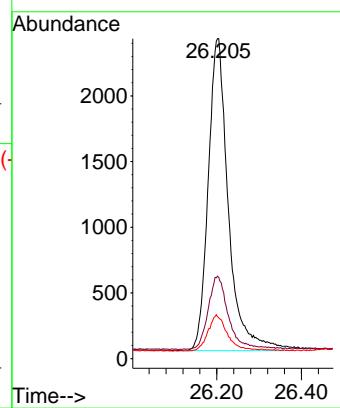

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037360.D  
 Acq On : 20 Jun 2025 21:39  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**ICVBN062125**

Quant Time: Jun 20 23:48:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	2309	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	5064	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	3457	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	7065	0.400	ng	# 0.00
29) Chrysene-d12	21.171	240	5560	0.400	ng	# 0.00
35) Perylene-d12	23.354	264	5756	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1841	0.399	ng	0.00
5) Phenol-d6	6.752	99	1797	0.378	ng	0.00
8) Nitrobenzene-d5	8.717	82	1658	0.405	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	3394	0.414	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	756	0.373	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	6049	0.398	ng	0.00
27) Fluoranthene-d10	19.008	212	7940	0.392	ng	0.00
31) Terphenyl-d14	19.616	244	5266	0.416	ng	0.00
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) 1,4-Dioxane	3.104	88	942	0.401	ng	91
3) n-Nitrosodimethylamine	3.422	42	845	0.393	ng	# 70
6) bis(2-Chloroethyl)ether	7.004	93	1718	0.407	ng	93
9) Naphthalene	10.394	128	5338	0.399	ng	# 89
10) Hexachlorobutadiene	10.682	225	2157	0.409	ng	# 99
12) 2-Methylnaphthalene	12.021	142	3620	0.388	ng	# 91
16) Acenaphthylene	13.935	152	5463	0.376	ng	98
17) Acenaphthene	14.277	154	3720	0.389	ng	99
18) Fluorene	15.272	166	5193	0.386	ng	99
20) 4,6-Dinitro-2-methylph...	15.368	198	491	0.289	ng	92
21) 4-Bromophenyl-phenylether	16.165	248	1905	0.379	ng	# 84
22) Hexachlorobenzene	16.276	284	2222	0.406	ng	98
23) Atrazine	16.450	200	1453	0.362	ng	# 84
24) Pentachlorophenol	16.624	266	881	0.323	ng	97
25) Phenanthrene	17.009	178	7743	0.378	ng	99
26) Anthracene	17.108	178	6739	0.357	ng	99
28) Fluoranthene	19.036	202	9535	0.369	ng	# 99
30) Pyrene	19.398	202	9570	0.424	ng	100
32) Benzo(a)anthracene	21.153	228	6805	0.372	ng	99
33) Chrysene	21.207	228	9119	0.412	ng	98
34) Bis(2-ethylhexyl)phtha...	21.099	149	3022	0.403	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.541	276	9492	0.368	ng	# 92
37) Benzo(b)fluoranthene	22.746	252	9472	0.447	ng	95
38) Benzo(k)fluoranthene	22.746	252	9472	0.412	ng	95
39) Benzo(a)pyrene	23.260	252	7258	0.382	ng	# 89
40) Dibenzo(a,h)anthracene	25.553	278	7116	0.367	ng	# 87
41) Benzo(g,h,i)perylene	26.199	276	8707	0.378	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037360.D  
 Acq On : 20 Jun 2025 21:39  
 Operator : RC/JU  
 Sample : SSTDICV0.4  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 ICVBN062125


Quant Time: Jun 20 23:48:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

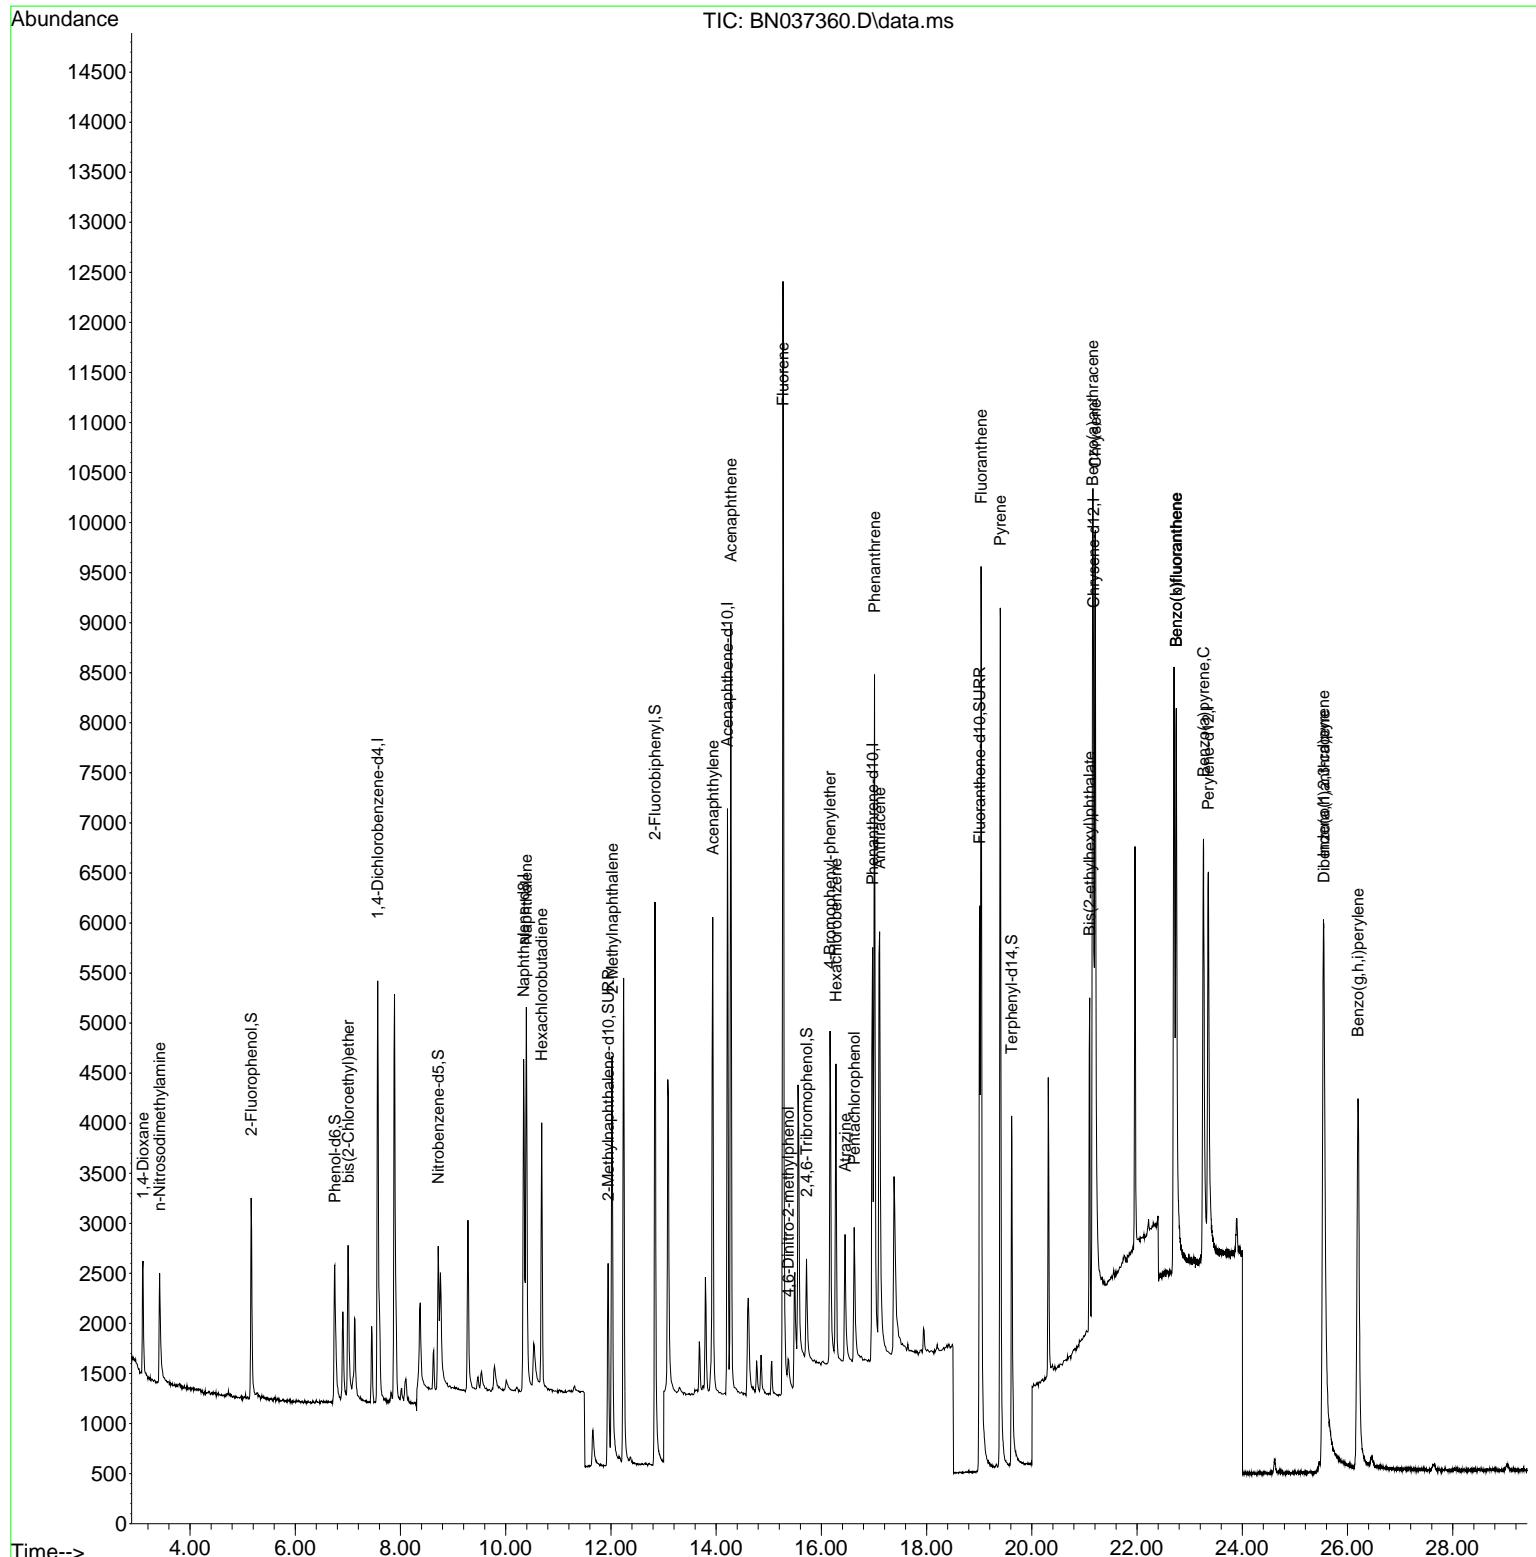






#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 64  
Delta R.T. -0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
ClientSampleId : ICVBN062125





Tgt Ion:152 Resp: 2309  
Ion Ratio Lower Upper  
152 100  
150 151.6 112.7 169.1  
115 54.6 45.9 68.9




#2  
1,4-Dioxane  
Concen: 0.401 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39




Tgt Ion: 88 Resp: 942  
Ion Ratio Lower Upper  
88 100  
43 24.5 21.0 31.6  
58 55.4 38.0 57.0






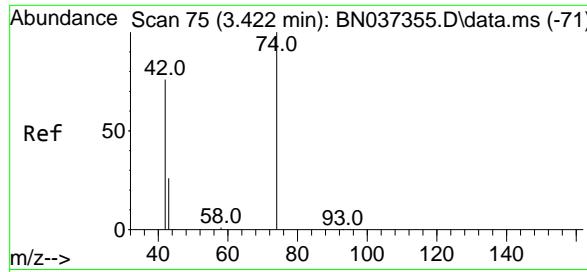


#3  
n-Nitrosodimethylamine  
Concen: 0.393 ng  
RT: 3.422 min Scan# 7  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
ClientSampleId : ICVBN062125  
Acq: 20 Jun 2025 21:39

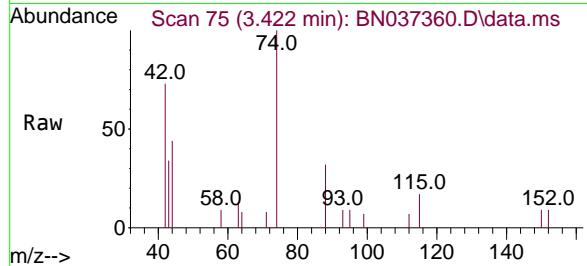



Tgt Ion: 42 Resp: 845  
Ion Ratio Lower Upper  
42 100  
74 137.3 84.3 126.5#  
44 2.5 5.0 7.4#

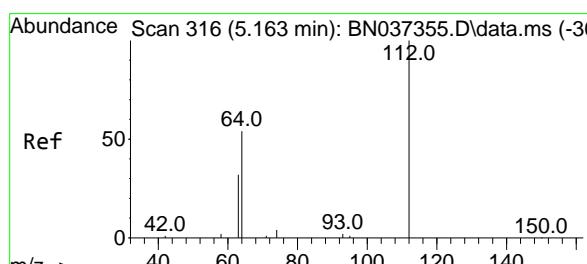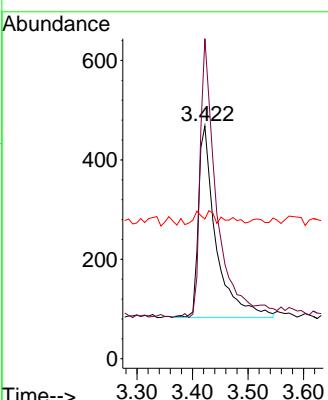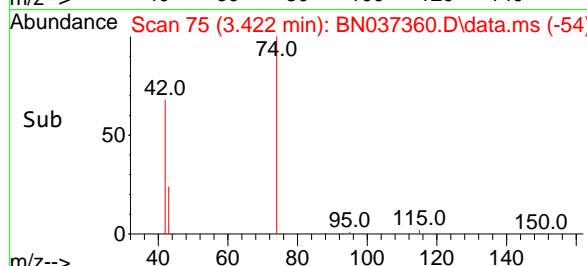


#4  
2-Fluorophenol  
Concen: 0.399 ng  
RT: 5.163 min Scan# 316  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

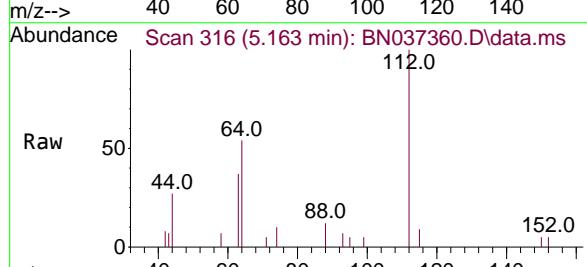


Tgt Ion: 112 Resp: 1841  
Ion Ratio Lower Upper  
112 100  
64 50.3 38.7 58.1  
63 31.9 26.4 39.6

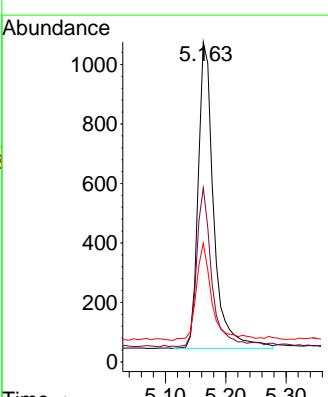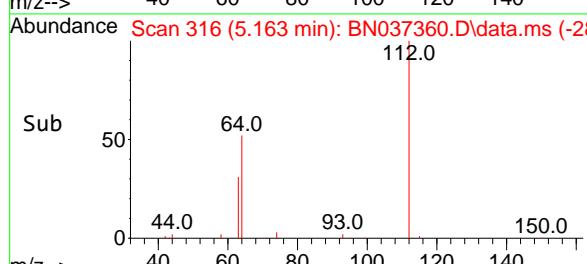



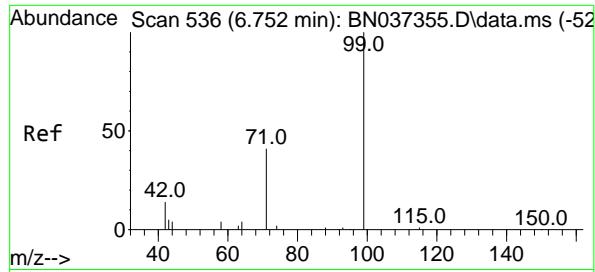


#5  
 Phenol-d6  
 Concen: 0.378 ng  
 RT: 6.752 min Scan# 51  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICVBN062125

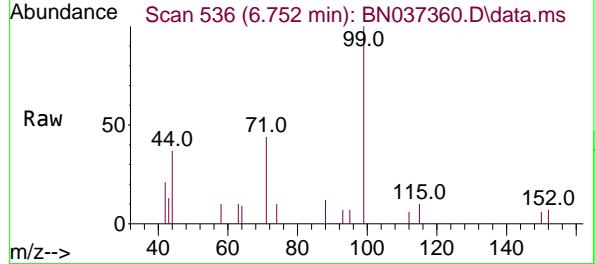



Tgt Ion: 99 Resp: 1797  
 Ion Ratio Lower Upper  
 99 100  
 42 15.9 19.8 29.8#  
 71 43.3 42.6 64.0

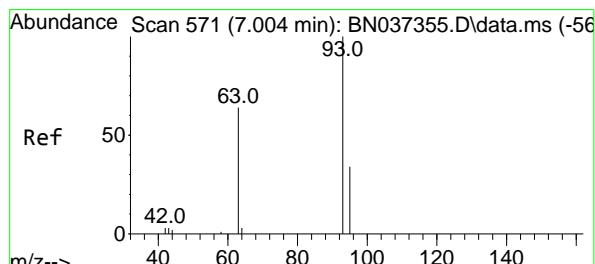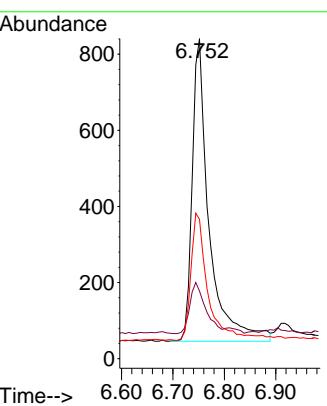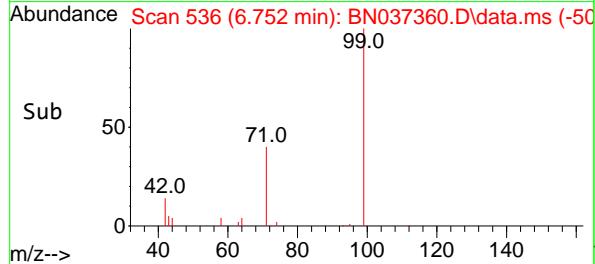


#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.407 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

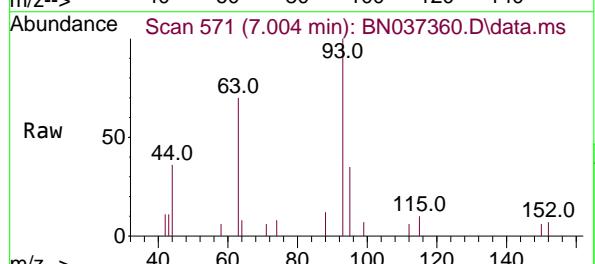


Tgt Ion: 93 Resp: 1718  
 Ion Ratio Lower Upper  
 93 100  
 63 61.8 53.2 79.8  
 95 29.5 27.3 40.9

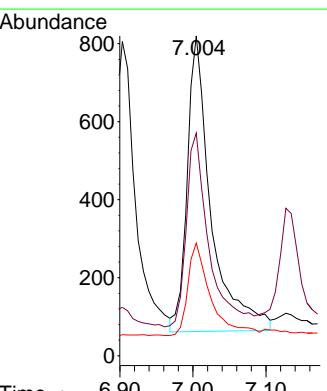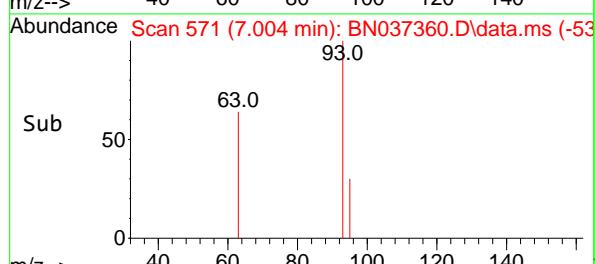





#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.340 min Scan# 942  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
ClientSampleId : ICVBN062125


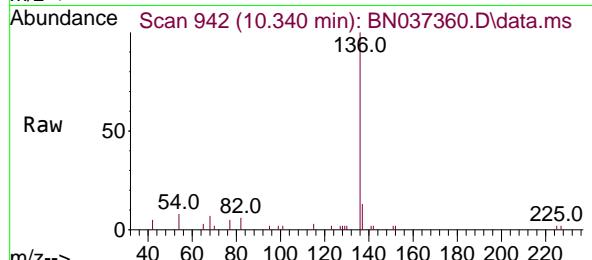


Tgt Ion:136 Resp: 5064  
Ion Ratio Lower Upper  
136 100  
137 12.7 12.2 18.2  
54 7.6 8.8 13.2#  
68 6.7 7.0 10.4#

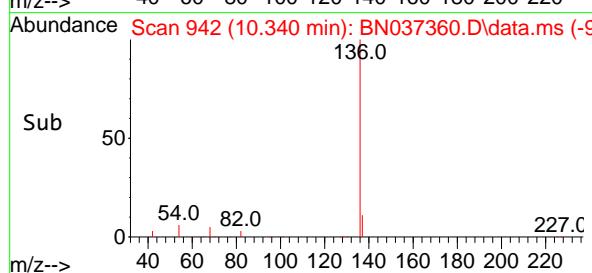




#8  
Nitrobenzene-d5  
Concen: 0.405 ng  
RT: 8.717 min Scan# 790  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Tgt Ion: 82 Resp: 1658  
Ion Ratio Lower Upper  
82 100  
128 39.6 42.5 63.7#  
54 43.9 43.2 64.8



Abundance Scan 790 (8.717 min): BN037360.D\data.ms


Raw 54.0 82.0 128.0 225.0

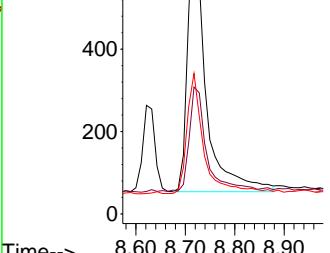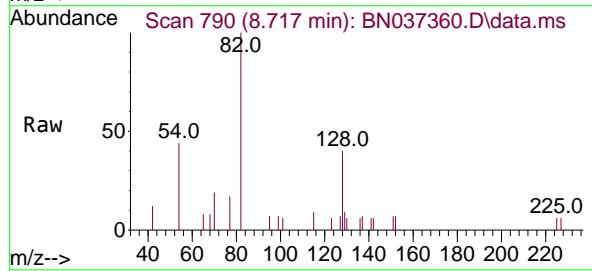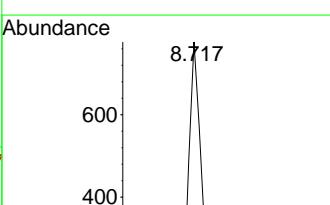


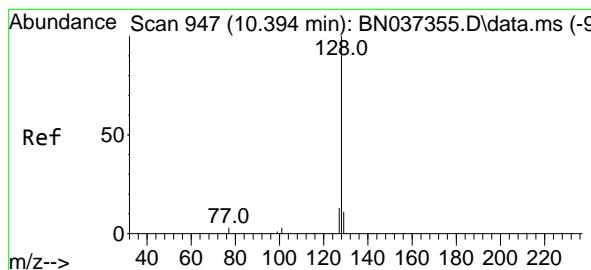


#9  
Naphthalene  
Concen: 0.399 ng  
RT: 10.394 min Scan# 947  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument :  
BNA\_N  
ClientSampleId :  
ICVBN062125


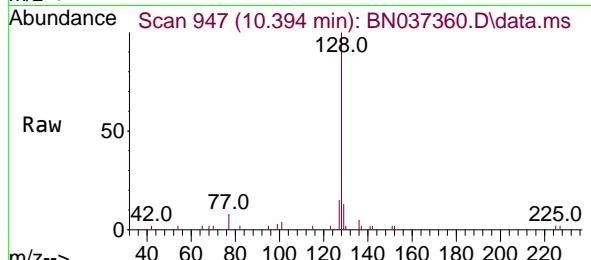


Tgt Ion:128 Resp: 5338  
Ion Ratio Lower Upper  
128 100  
129 12.7 14.0 21.0#  
127 15.0 15.8 23.8#

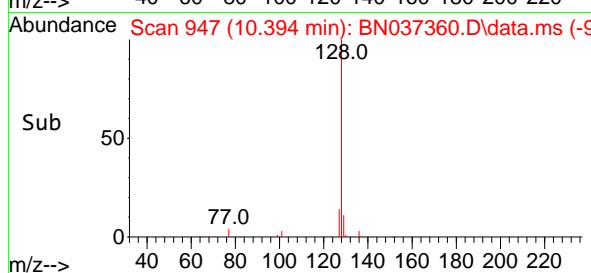


#10  
Hexachlorobutadiene  
Concen: 0.409 ng  
RT: 10.682 min Scan# 974  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Tgt Ion:225 Resp: 2157  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 63.3 50.3 75.5

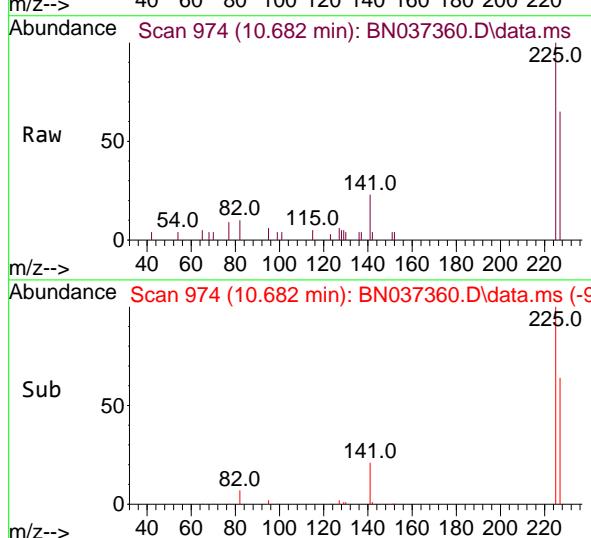




Sub 50




#11  
2-Methylnaphthalene-d10  
Concen: 0.414 ng  
RT: 11.945 min Scan# 1:Instrument :  
Delta R.T. 0.000 min BNA\_N  
Lab File: BN037360.D ClientSampleId :  
Acq: 20 Jun 2025 21:39 ICBN062125





Tgt Ion:152 Resp: 3394  
Ion Ratio Lower Upper  
152 100  
151 22.0 17.4 26.0

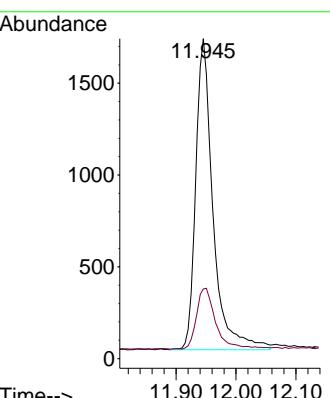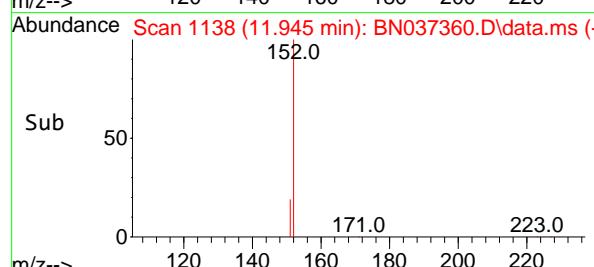


#12  
2-Methylnaphthalene  
Concen: 0.388 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39



Tgt Ion:142 Resp: 3620  
Ion Ratio Lower Upper  
142 100  
141 90.6 70.2 105.2  
115 41.2 43.0 64.4#

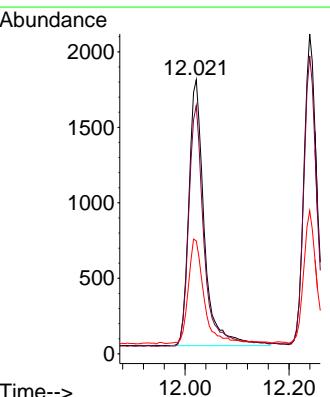



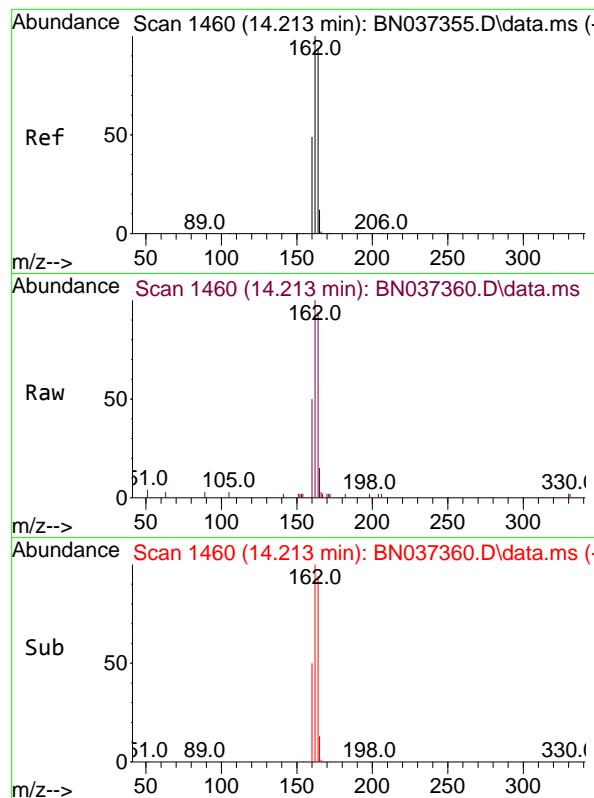

#13  
 Acenaphthene-d10  
 Concen: 0.400 ng  
 RT: 14.213 min Scan# 14  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICVBN062125


Tgt Ion:164 Resp: 3457  
 Ion Ratio Lower Upper  
 164 100  
 162 106.3 81.5 122.3  
 160 53.6 43.0 64.4

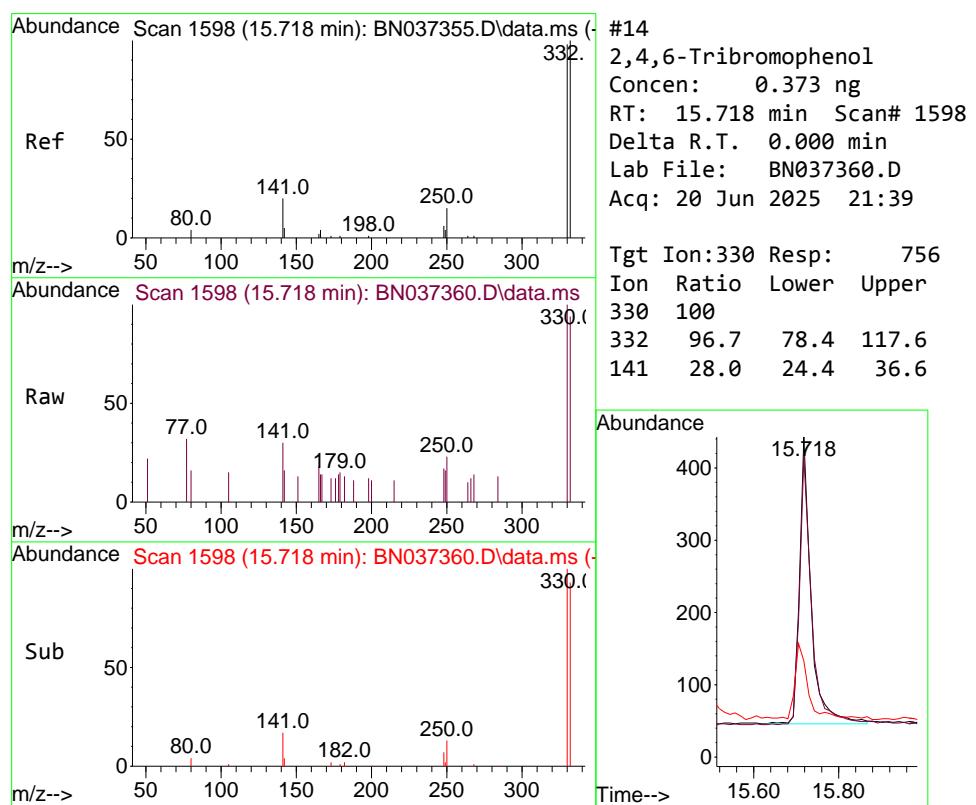

#14  
 2,4,6-Tribromophenol  
 Concen: 0.373 ng  
 RT: 15.718 min Scan# 1598  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39



Tgt Ion:330 Resp: 756  
 Ion Ratio Lower Upper  
 330 100  
 332 96.7 78.4 117.6  
 141 28.0 24.4 36.6



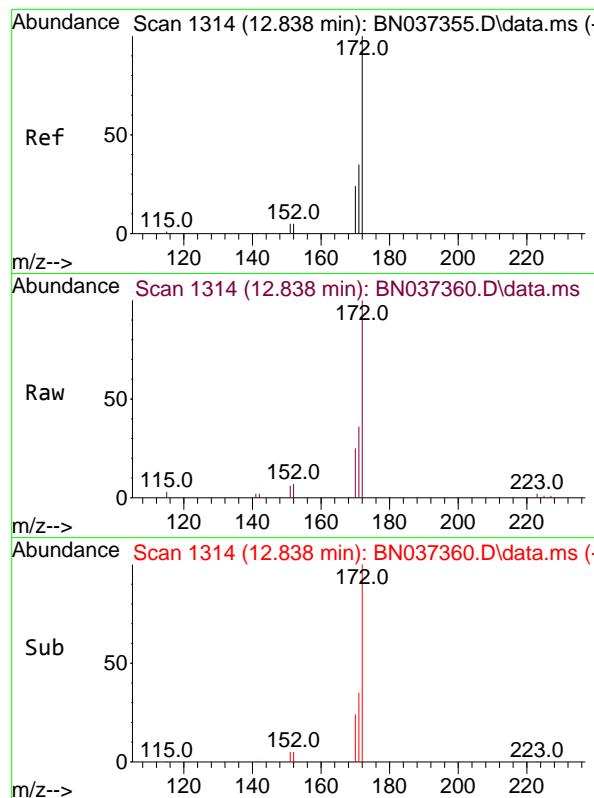


#15  
2-Fluorobiphenyl  
Concen: 0.398 ng  
RT: 12.838 min Scan# 1  
Instrument: BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
ClientSampleId : ICBN062125  
Acq: 20 Jun 2025 21:39




Tgt Ion:172 Resp: 6049  
Ion Ratio Lower Upper  
172 100  
171 36.2 30.8 46.2  
170 25.1 21.9 32.9

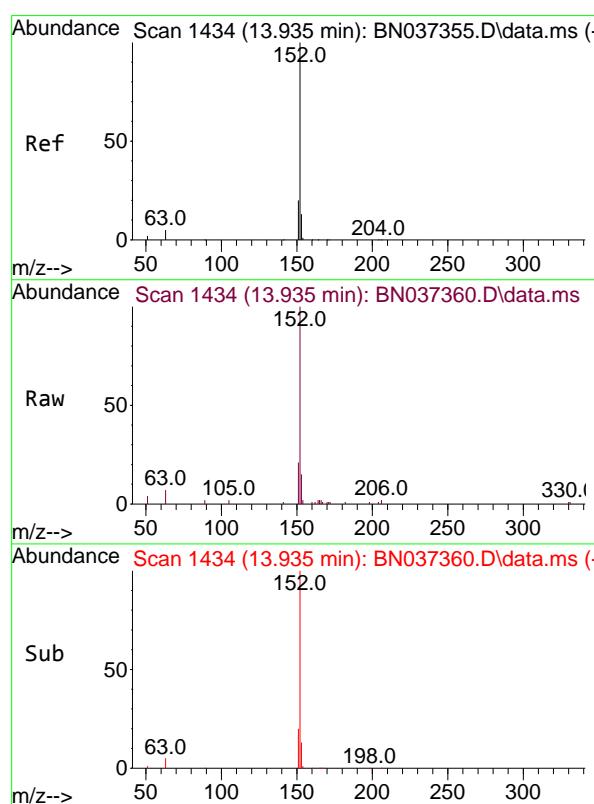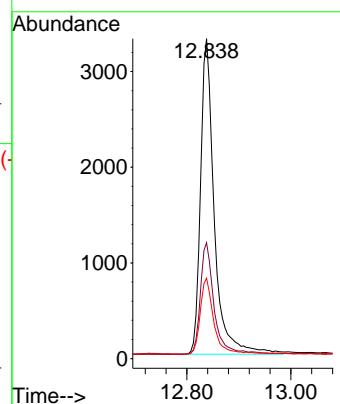

#16  
Acenaphthylene  
Concen: 0.376 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Tgt Ion:152 Resp: 5463  
Ion Ratio Lower Upper  
152 100  
151 19.8 16.6 24.8  
153 13.3 10.2 15.2

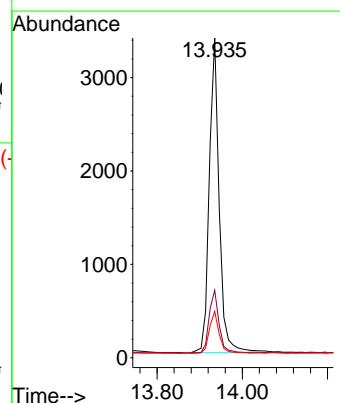

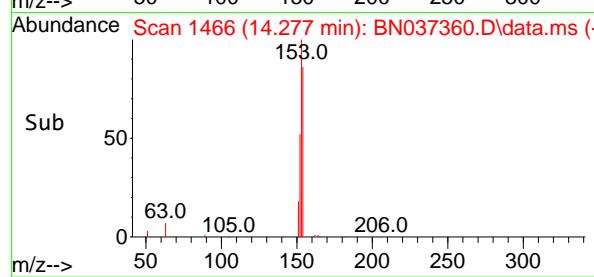

#17

Acenaphthene

Concen: 0.389 ng

RT: 14.277 min Scan# 1466

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Instrument :

BNA\_N

ClientSampleId :

ICVBN062125

Tgt Ion:154 Resp: 3720

Ion Ratio Lower Upper





154 100

153 117.1 93.1 139.7

152 62.3 48.6 73.0

Abundance

14.277

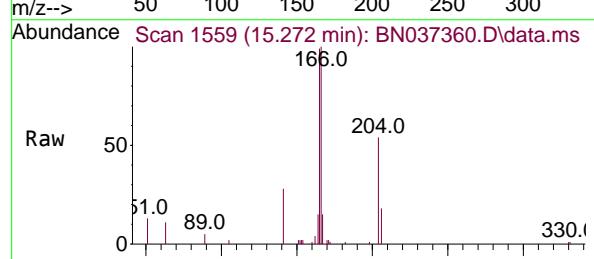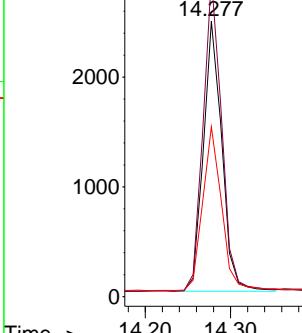

#18

Fluorene

Concen: 0.386 ng

RT: 15.272 min Scan# 1559

Delta R.T. 0.000 min

Lab File: BN037360.D

Acq: 20 Jun 2025 21:39

Tgt Ion:166 Resp: 5193

Ion Ratio Lower Upper


166 100


165 98.8 79.5 119.3

167 13.4 10.7 16.1

Abundance

15.272


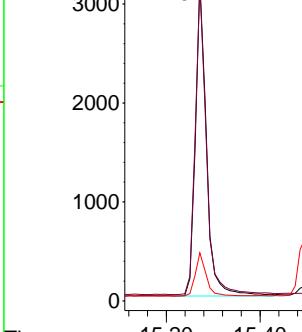


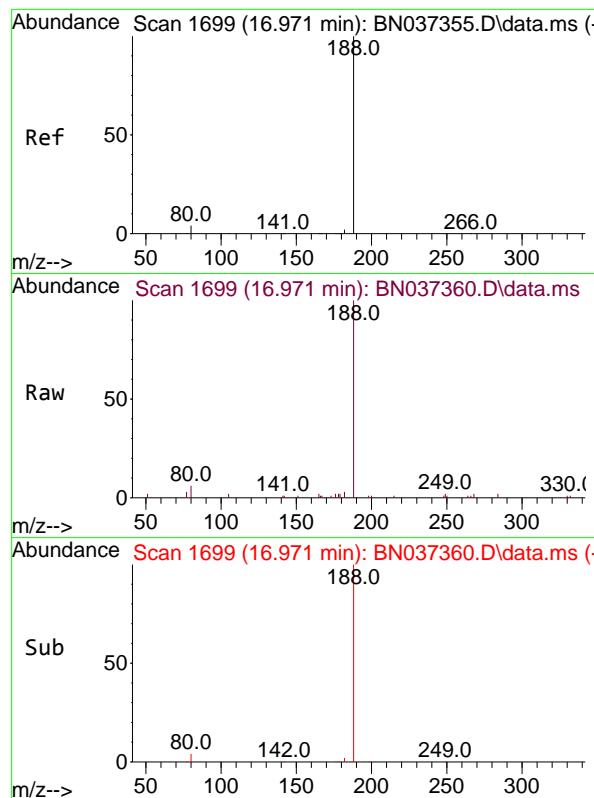

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICBN062125


Tgt Ion:188 Resp: 7065  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 5.7 6.2 9.2#

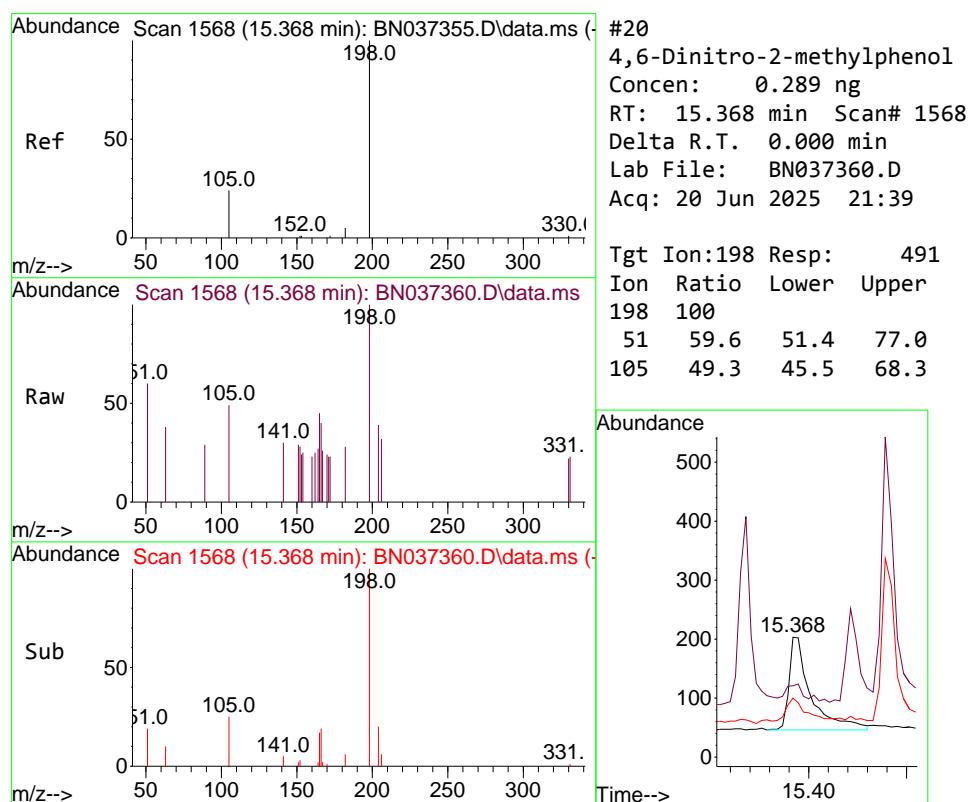

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.289 ng  
 RT: 15.368 min Scan# 1568  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39



Tgt Ion:198 Resp: 491  
 Ion Ratio Lower Upper  
 198 100  
 51 59.6 51.4 77.0  
 105 49.3 45.5 68.3



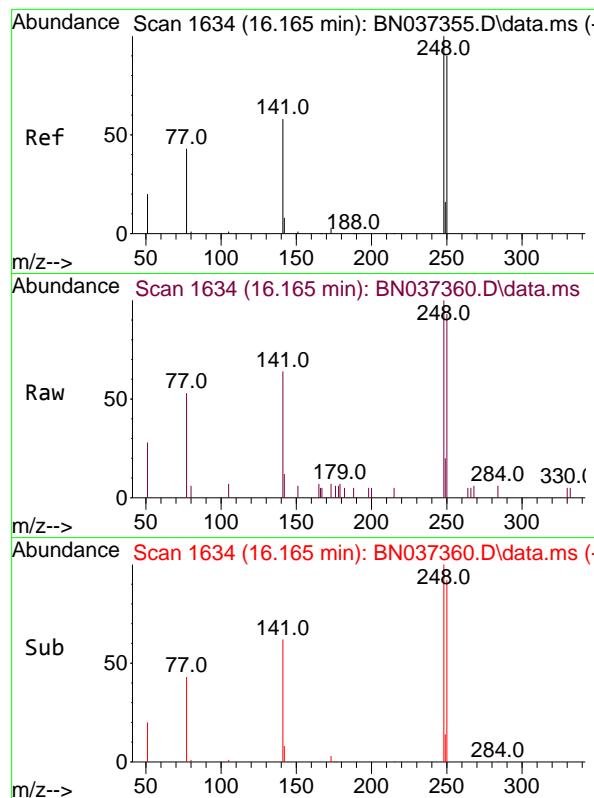


#21  
4-Bromophenyl-phenylether  
Concen: 0.379 ng  
RT: 16.165 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.000 min  
Lab File: BN037360.D ClientSampleId :  
Acq: 20 Jun 2025 21:39 ICBN062125


Tgt Ion:248 Resp: 1905  
Ion Ratio Lower Upper  
248 100  
250 92.7 80.4 120.6  
141 64.3 33.3 49.9#

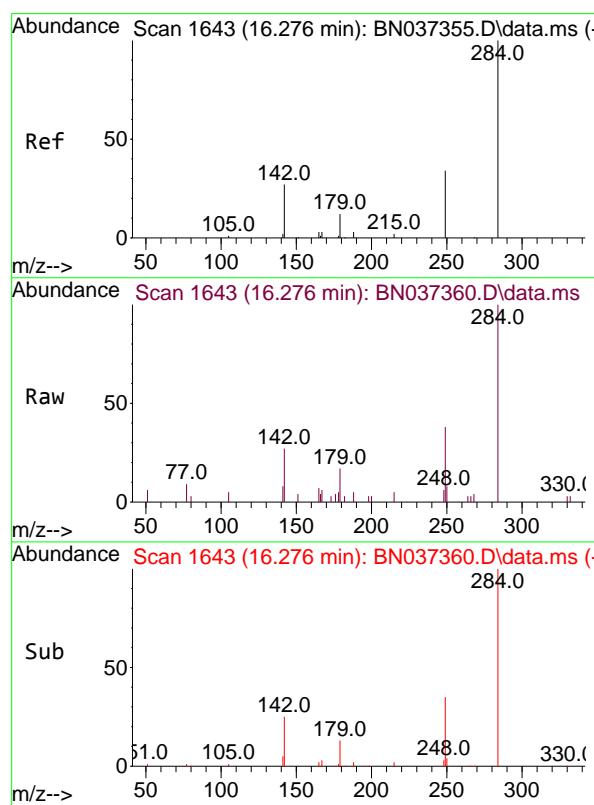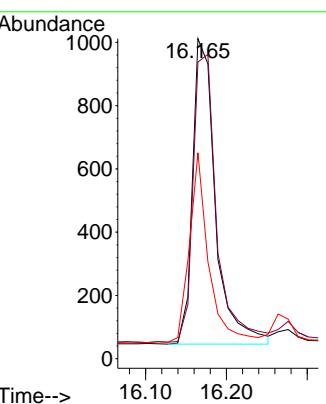

#22  
Hexachlorobenzene  
Concen: 0.406 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Tgt Ion:284 Resp: 2222  
Ion Ratio Lower Upper  
284 100  
142 33.0 27.0 40.6  
249 35.0 28.8 43.2

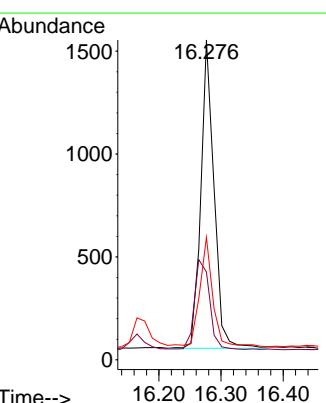






#23  
Atrazine  
Concen: 0.362 ng  
RT: 16.450 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
ClientSampleId : ICVBN062125





Tgt Ion:200 Resp: 1453  
Ion Ratio Lower Upper  
200 100  
173 24.2 29.2 43.8#  
215 51.2 48.8 73.2

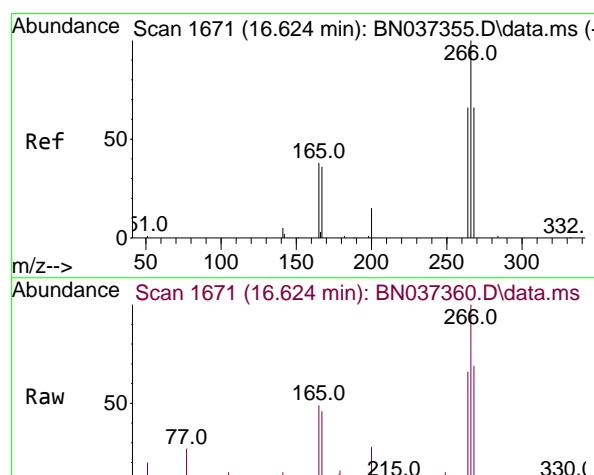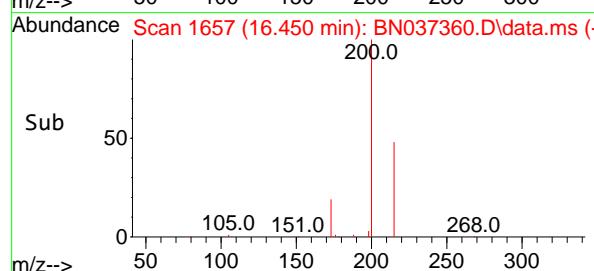


#24  
Pentachlorophenol  
Concen: 0.323 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

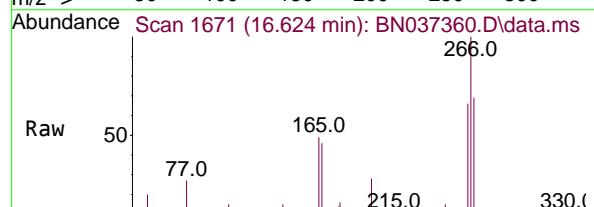


Tgt Ion:266 Resp: 881  
Ion Ratio Lower Upper  
266 100  
264 63.5 50.3 75.5  
268 65.0 55.3 82.9

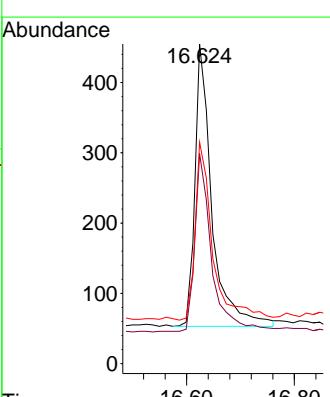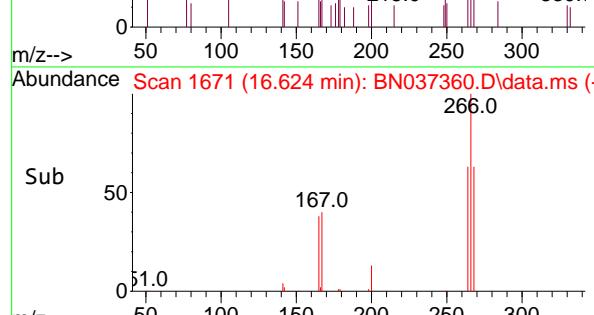






#25  
Phenanthrene  
Concen: 0.378 ng  
RT: 17.009 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
ClientSampleId : ICVBN062125





Tgt Ion:178 Resp: 7743  
Ion Ratio Lower Upper  
178 100  
176 19.3 15.2 22.8  
179 15.5 12.9 19.3

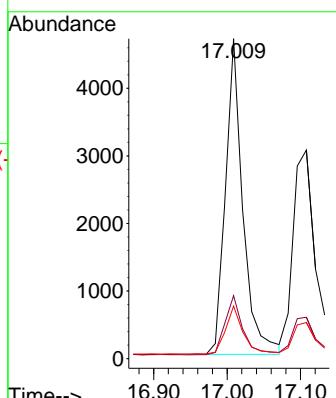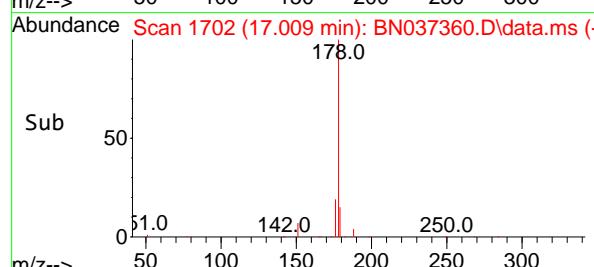


#26  
Anthracene  
Concen: 0.357 ng  
RT: 17.108 min Scan# 1710  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39



Tgt Ion:178 Resp: 6739  
Ion Ratio Lower Upper  
178 100  
176 19.0 14.7 22.1  
179 15.7 13.0 19.6

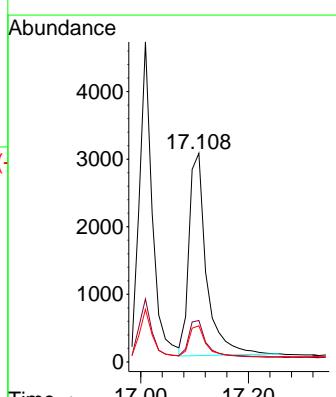



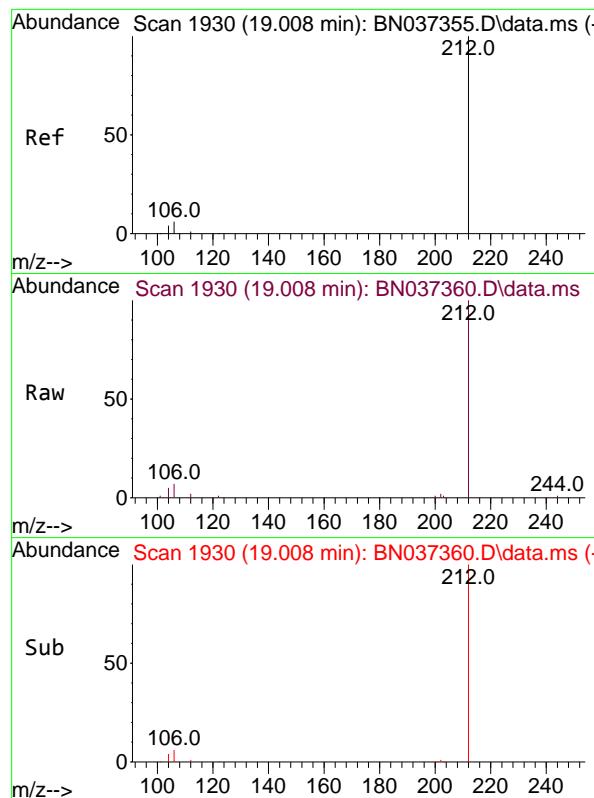

#27  
 Fluoranthene-d10  
 Concen: 0.392 ng  
 RT: 19.008 min Scan# 1930  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICVBN062125


Tgt Ion:212 Resp: 7940  
 Ion Ratio Lower Upper  
 212 100  
 106 6.2 3.0 4.4#  
 104 3.9 2.0 3.0#

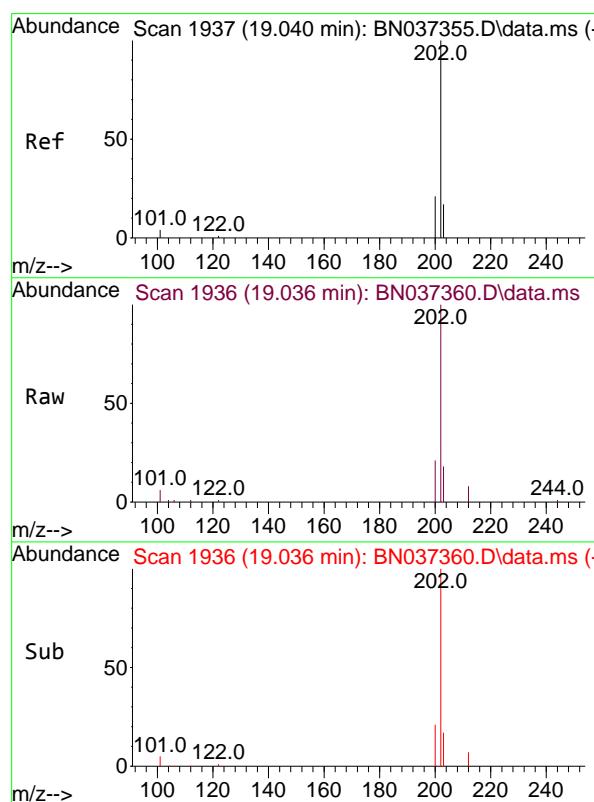

#28  
 Fluoranthene  
 Concen: 0.369 ng  
 RT: 19.036 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

Tgt Ion:202 Resp: 9535  
 Ion Ratio Lower Upper  
 202 100  
 101 5.3 3.0 4.6#  
 203 16.8 13.7 20.5





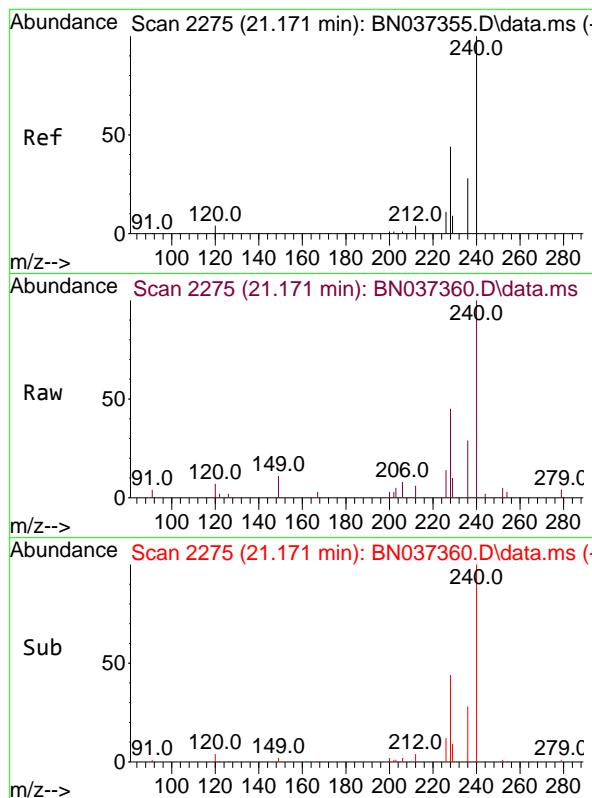

#29  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.171 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICVBN062125


Tgt Ion:240 Resp: 5560  
 Ion Ratio Lower Upper  
 240 100  
 120 7.3 7.5 11.3#  
 236 29.5 24.9 37.3

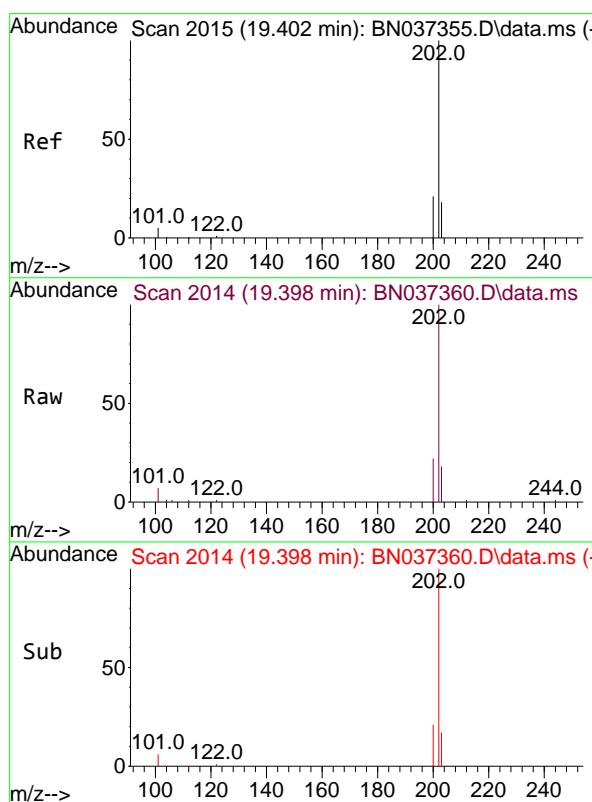

#30  
 Pyrene  
 Concen: 0.424 ng  
 RT: 19.398 min Scan# 2014  
 Delta R.T. -0.005 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

Tgt Ion:202 Resp: 9570  
 Ion Ratio Lower Upper  
 202 100  
 200 20.7 16.8 25.2  
 203 18.0 14.5 21.7





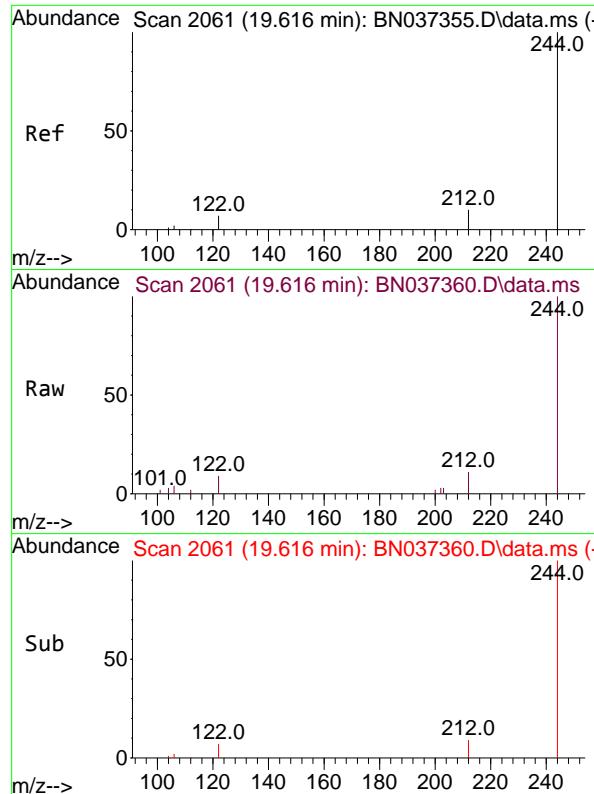

#31  
**Terphenyl-d14**  
Concen: 0.416 ng  
RT: 19.616 min Scan# 2061  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
ClientSampleId : ICVBN062125


Tgt Ion:244 Resp: 5266  
Ion Ratio Lower Upper  
244 100  
212 11.3 11.1 16.7  
122 9.0 7.2 10.8

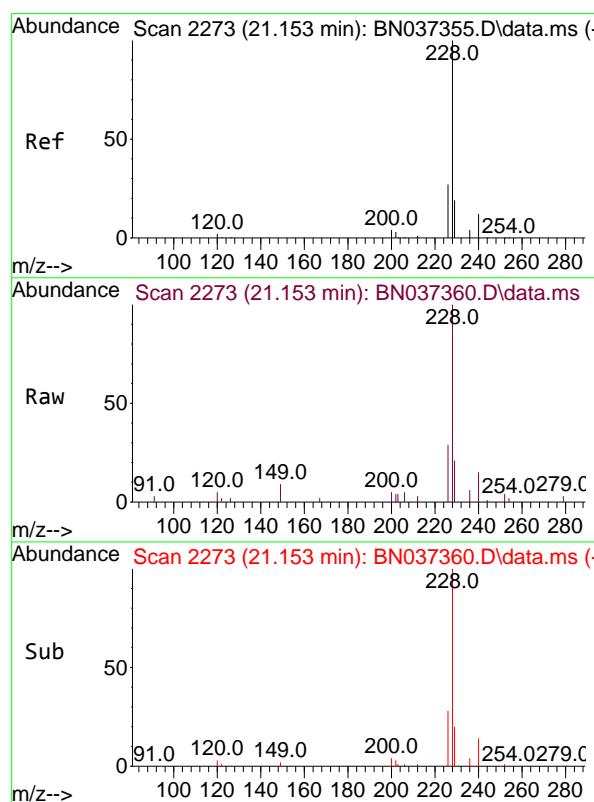

#32  
**Benzo(a)anthracene**  
Concen: 0.372 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39


Tgt Ion:228 Resp: 6805  
Ion Ratio Lower Upper  
228 100  
226 29.0 23.0 34.4  
229 20.9 17.4 26.0

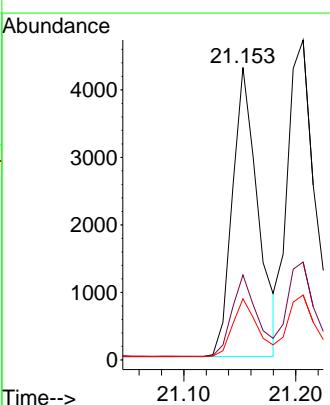





#33  
Chrysene  
Concen: 0.412 ng  
RT: 21.207 min Scan# 2139  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
ClientSampleId : ICBN062125


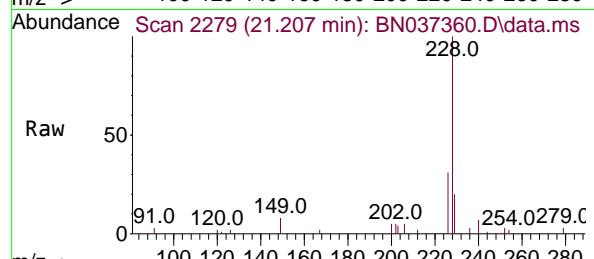



Tgt Ion:228 Resp: 9119  
Ion Ratio Lower Upper  
228 100  
226 30.6 25.4 38.2  
229 20.3 17.3 25.9

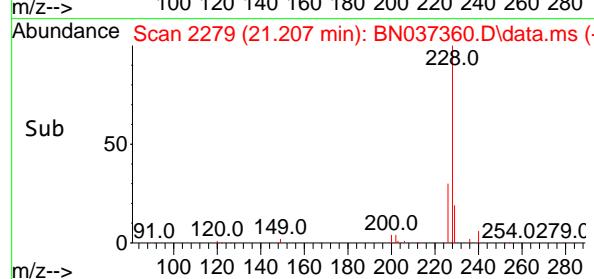

#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.403 ng  
RT: 21.099 min Scan# 2267  
Delta R.T. 0.000 min  
Lab File: BN037360.D  
Acq: 20 Jun 2025 21:39

Tgt Ion:149 Resp: 3022  
Ion Ratio Lower Upper  
149 100  
167 31.4 24.6 37.0  
279 5.6 6.5 9.7#

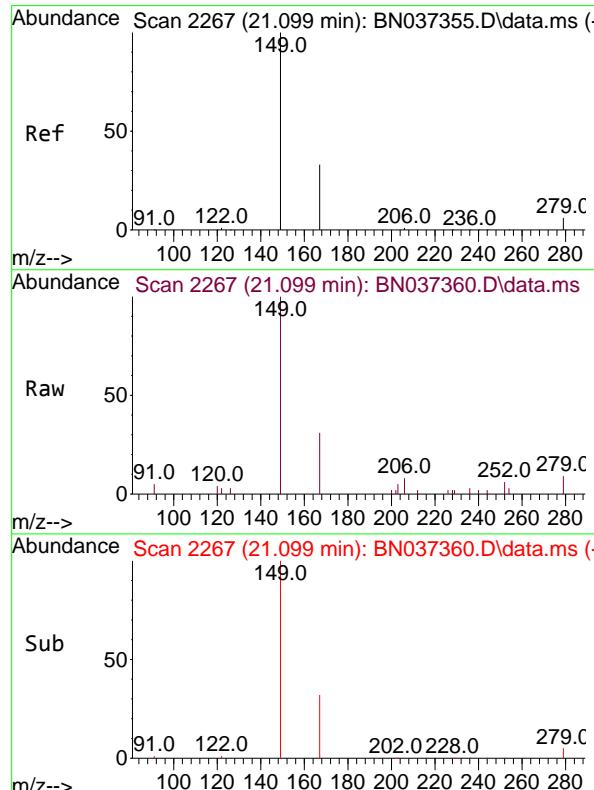
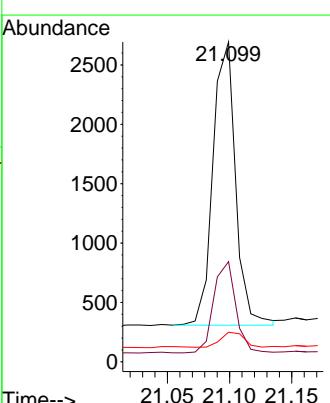


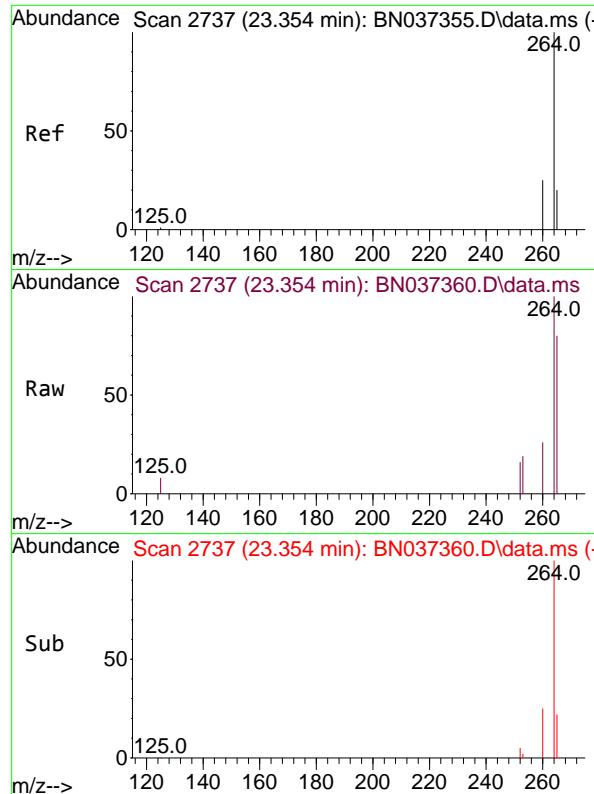

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.354 min Scan# 21  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICVBN062125


Tgt Ion:264 Resp: 5756  
 Ion Ratio Lower Upper  
 264 100  
 260 26.4 21.4 32.2  
 265 80.4 71.4 107.0

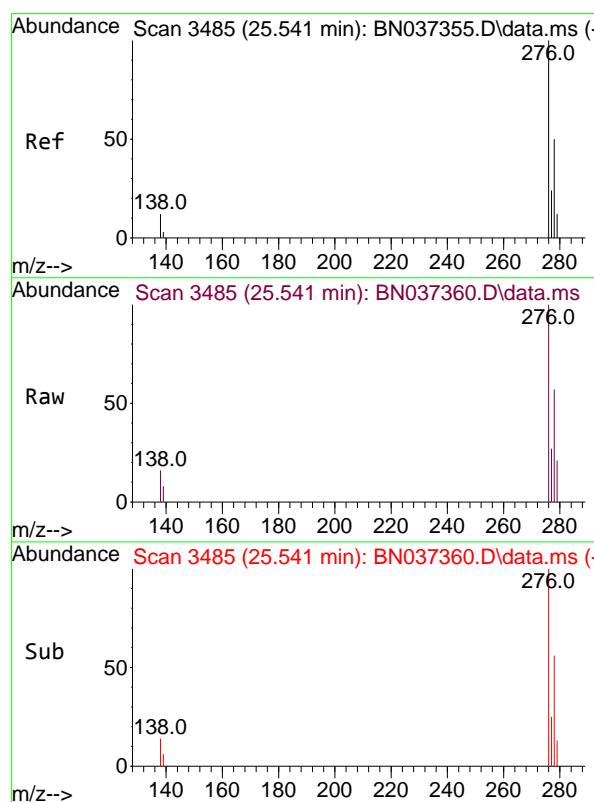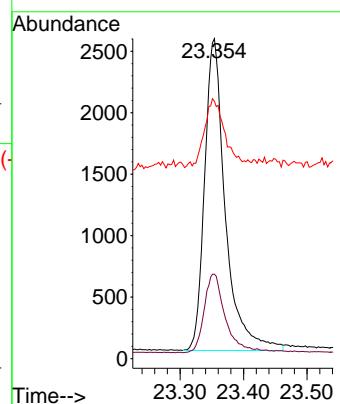

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.368 ng  
 RT: 25.541 min Scan# 3485  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

Tgt Ion:276 Resp: 9492  
 Ion Ratio Lower Upper  
 276 100  
 138 11.7 2.2 3.2#  
 277 24.2 17.1 25.7


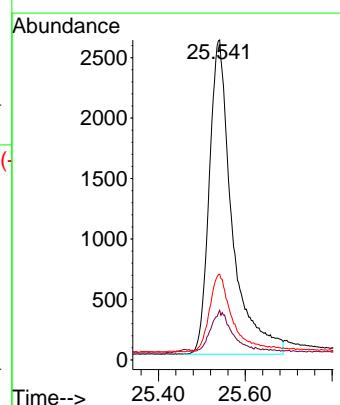


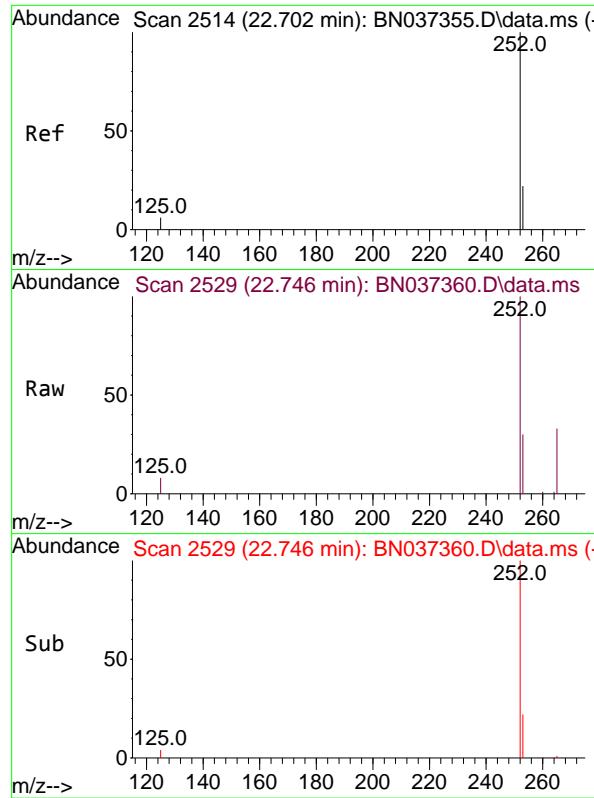

#37  
 Benzo(b)fluoranthene  
 Concen: 0.447 ng  
 RT: 22.746 min Scan# 21  
 Delta R.T. 0.044 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICVBN062125


Tgt Ion:252 Resp: 9472  
 Ion Ratio Lower Upper  
 252 100  
 253 29.9 26.6 40.0  
 125 8.4 6.1 9.1

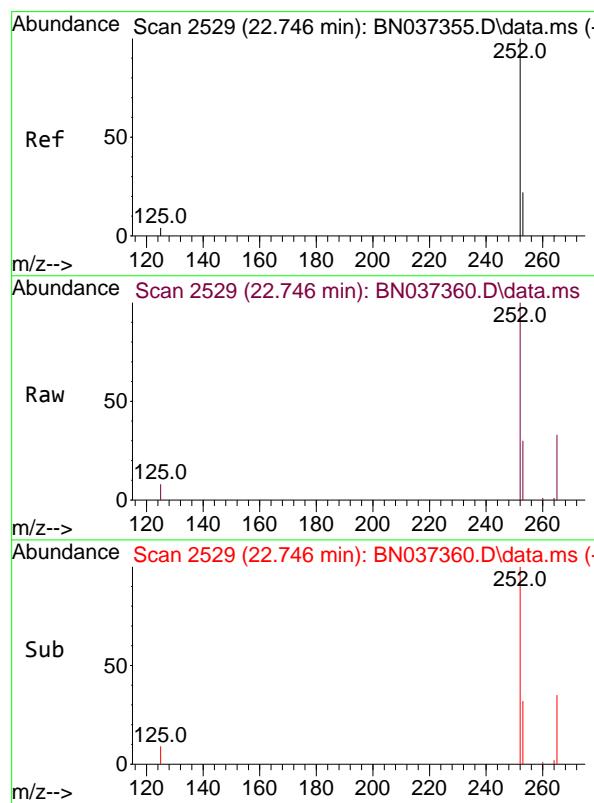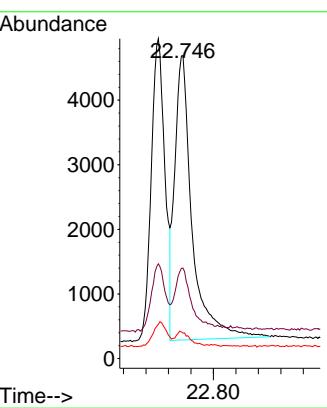

#38  
 Benzo(k)fluoranthene  
 Concen: 0.412 ng  
 RT: 22.746 min Scan# 2529  
 Delta R.T. 0.000 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

Tgt Ion:252 Resp: 9472  
 Ion Ratio Lower Upper  
 252 100  
 253 29.9 26.7 40.1  
 125 8.4 6.5 9.7


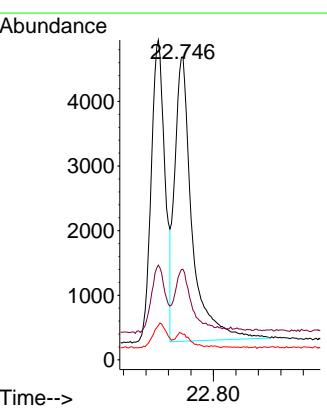


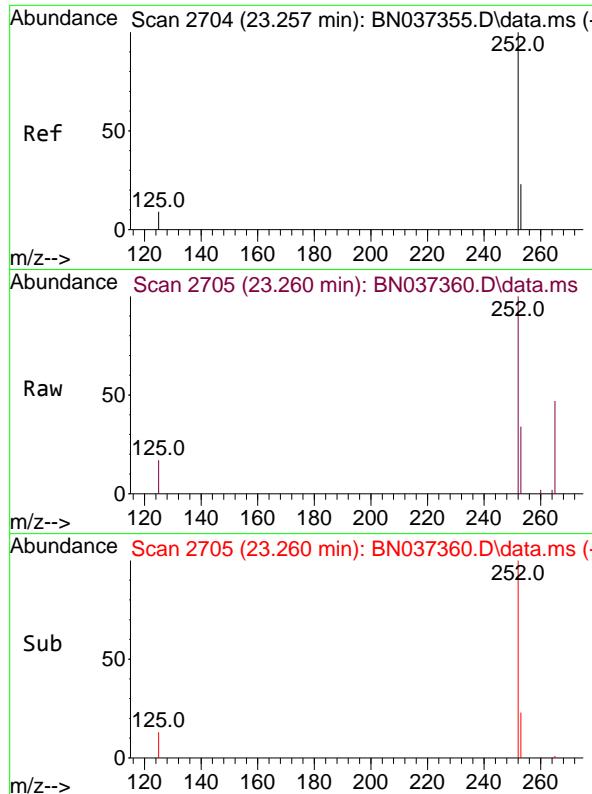

#39  
 Benzo(a)pyrene  
 Concen: 0.382 ng  
 RT: 23.260 min Scan# 21  
 Delta R.T. 0.003 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39


Instrument : BNA\_N  
 ClientSampleId : ICVBN062125


Tgt Ion:252 Resp: 7258  
 Ion Ratio Lower Upper  
 252 100  
 253 34.3 31.6 47.4  
 125 17.4 8.4 12.6#

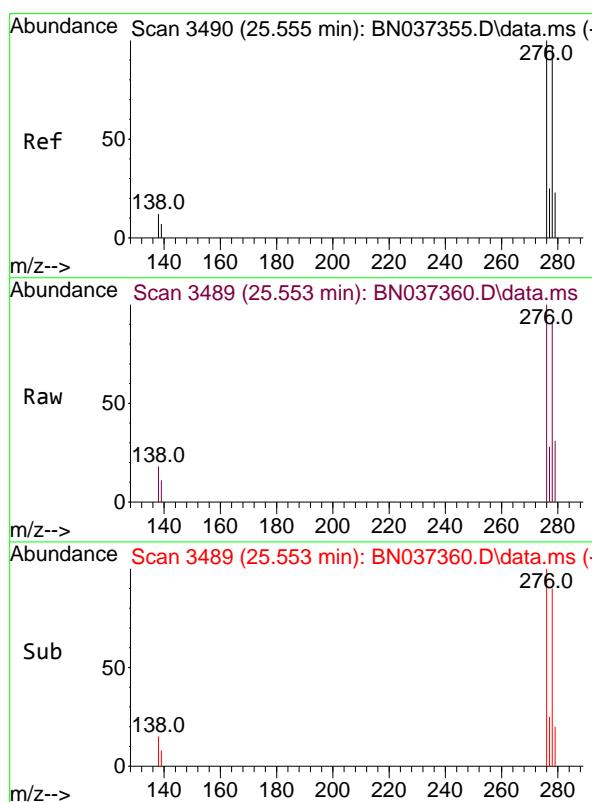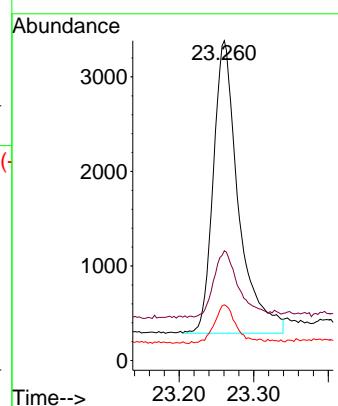

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.367 ng  
 RT: 25.553 min Scan# 3489  
 Delta R.T. -0.003 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

Tgt Ion:278 Resp: 7116  
 Ion Ratio Lower Upper  
 278 100  
 139 11.8 10.2 15.4  
 279 33.7 35.6 53.4#

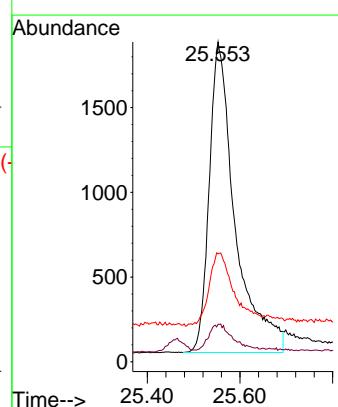


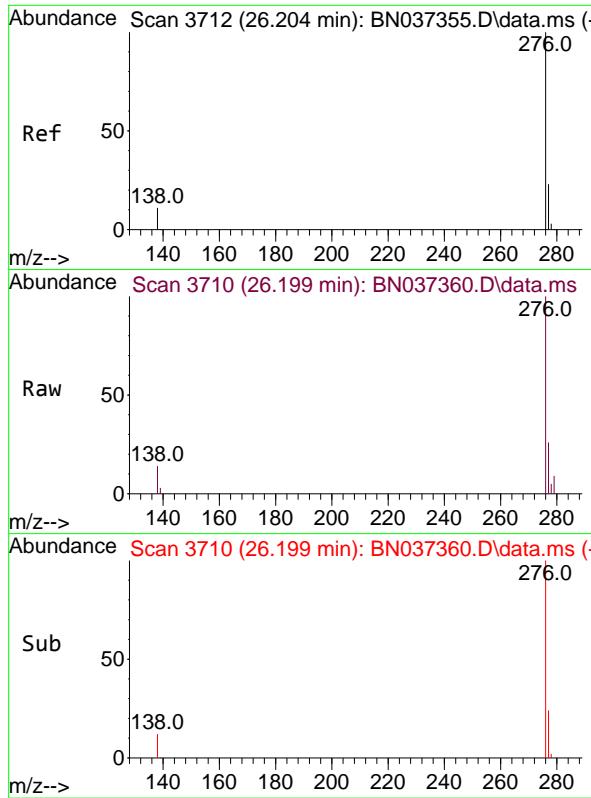

#41  
 Benzo(g,h,i)perylene  
 Concen: 0.378 ng  
 RT: 26.199 min Scan# 3  
 Delta R.T. -0.006 min  
 Lab File: BN037360.D  
 Acq: 20 Jun 2025 21:39

Instrument : BNA\_N  
 ClientSampleId : ICBN062125

Tgt Ion:276 Resp: 8707  
 Ion Ratio Lower Upper  
 276 100  
 277 25.9 22.7 34.1  
 138 13.9 9.4 14.2

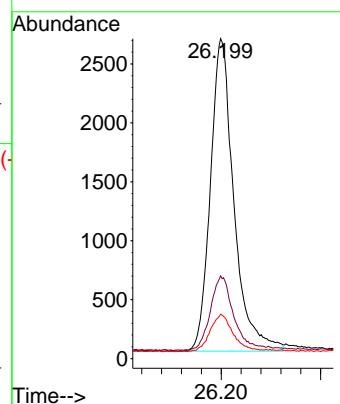

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037364.D  
 Acq On : 21 Jun 2025 00:04  
 Operator : RC/JU  
 Sample : PB168563BSD  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**PB168563BSD**

Quant Time: Jun 21 00:33:22 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1885	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4095	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2623	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5035	0.400	ng	# 0.00
29) Chrysene-d12	21.162	240	4193	0.400	ng	0.00
35) Perylene-d12	23.354	264	4470	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.170	112	1274	0.338	ng	0.00
5) Phenol-d6	6.752	99	1342	0.346	ng	0.00
8) Nitrobenzene-d5	8.717	82	1284	0.388	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	3901	0.588	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	522	0.339	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	4574	0.397	ng	0.00
27) Fluoranthene-d10	19.007	212	5003	0.346	ng	0.00
31) Terphenyl-d14	19.616	244	3587	0.375	ng	0.00
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) 1,4-Dioxane	3.104	88	583	0.304	ng	# 36
3) n-Nitrosodimethylamine	3.415	42	653	0.372	ng	# 70
6) bis(2-Chloroethyl)ether	7.004	93	1260	0.366	ng	99
9) Naphthalene	10.394	128	4026	0.372	ng	# 89
10) Hexachlorobutadiene	10.682	225	1748	0.410	ng	# 100
12) 2-Methylnaphthalene	12.021	142	2474	0.328	ng	93
16) Acenaphthylene	13.935	152	4445	0.403	ng	98
17) Acenaphthene	14.277	154	2642	0.364	ng	98
18) Fluorene	15.271	166	3709	0.364	ng	99
20) 4,6-Dinitro-2-methylph...	15.378	198	419	0.346	ng	# 81
21) 4-Bromophenyl-phenylether	16.177	248	1344	0.375	ng	96
22) Hexachlorobenzene	16.276	284	1596	0.409	ng	99
23) Atrazine	16.450	200	1011	0.354	ng	# 88
24) Pentachlorophenol	16.624	266	1337	0.688	ng	97
25) Phenanthrene	17.009	178	5370	0.368	ng	99
26) Anthracene	17.108	178	4862	0.362	ng	99
28) Fluoranthene	19.035	202	6244	0.339	ng	# 99
30) Pyrene	19.402	202	6351	0.373	ng	99
32) Benzo(a)anthracene	21.153	228	5141	0.373	ng	99
33) Chrysene	21.206	228	6472	0.387	ng	97
34) Bis(2-ethylhexyl)phtha...	21.090	149	2023	0.358	ng	96
36) Indeno(1,2,3-cd)pyrene	25.538	276	7744	0.386	ng	# 92
37) Benzo(b)fluoranthene	22.696	252	5838	0.355	ng	95
38) Benzo(k)fluoranthene	22.740	252	6945	0.389	ng	96
39) Benzo(a)pyrene	23.254	252	5888	0.399	ng	95
40) Dibenzo(a,h)anthracene	25.552	278	5912	0.392	ng	89
41) Benzo(g,h,i)perylene	26.199	276	7039	0.393	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037364.D  
 Acq On : 21 Jun 2025 00:04  
 Operator : RC/JU  
 Sample : PB168563BSD  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PB168563BSD


Quant Time: Jun 21 00:33:22 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

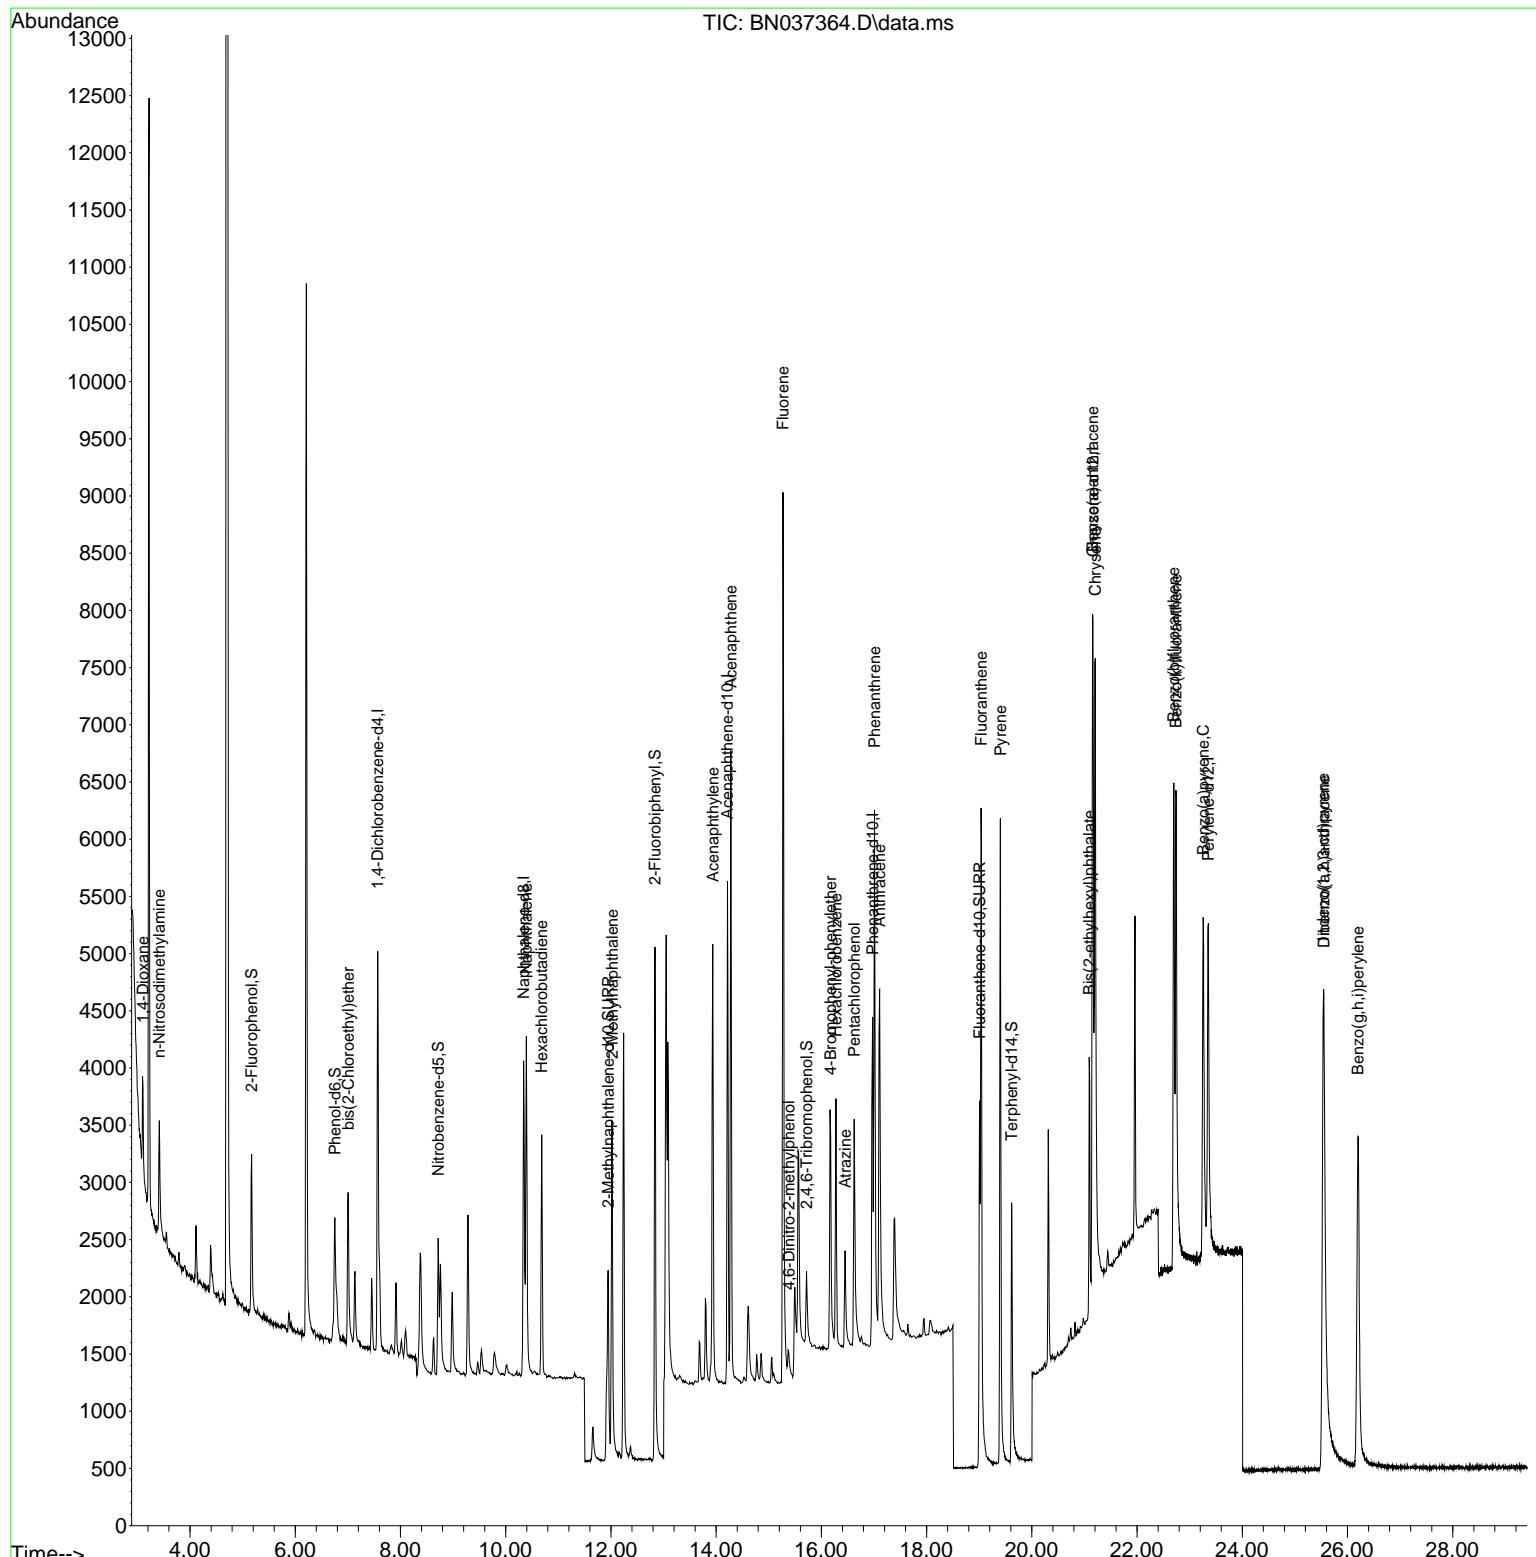



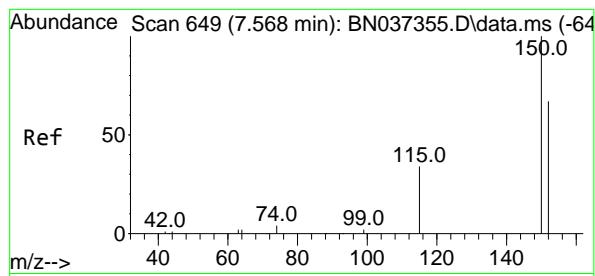


#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 64  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
ClientSampleId : PB168563BSD

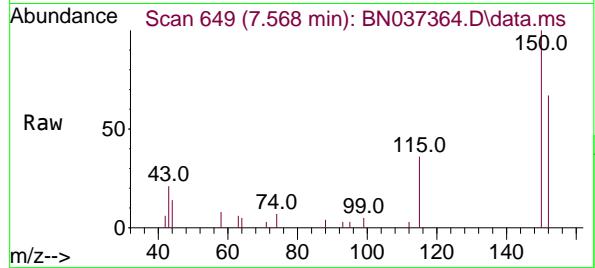



Tgt Ion:152 Resp: 1885  
Ion Ratio Lower Upper  
152 100  
150 149.8 112.7 169.1  
115 54.4 45.9 68.9

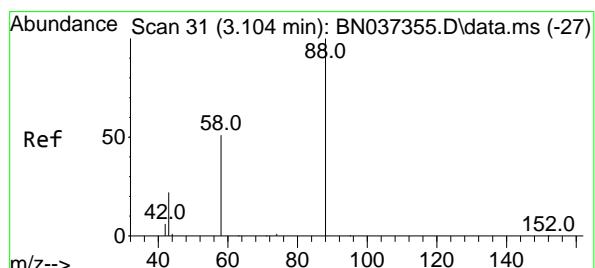

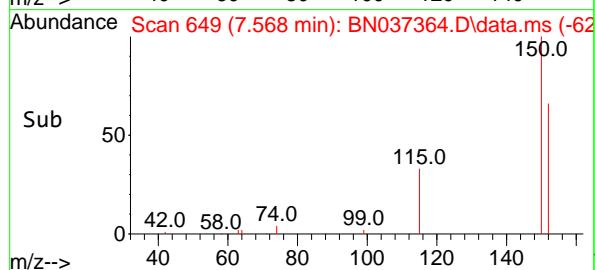


#2  
1,4-Dioxane  
Concen: 0.304 ng  
RT: 3.104 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

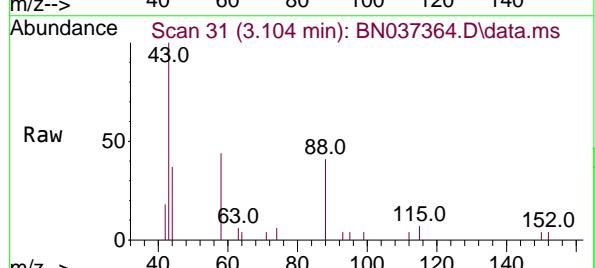

Tgt Ion: 88 Resp: 583  
Ion Ratio Lower Upper  
88 100  
43 101.0 21.0 31.6#  
58 59.7 38.0 57.0#

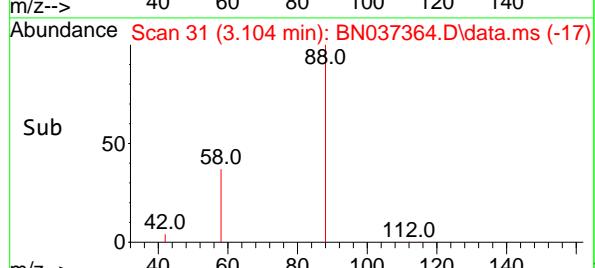

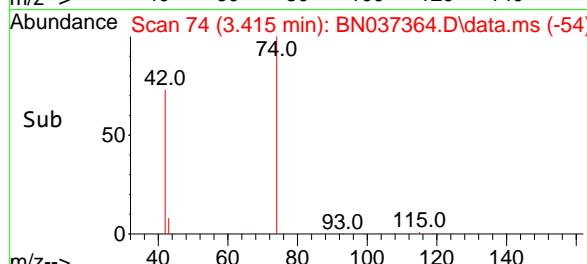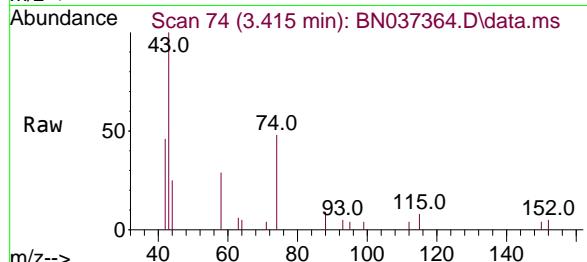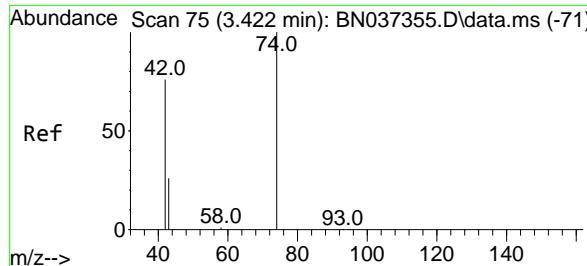

#3

n-Nitrosodimethylamine

Concen: 0.372 ng

RT: 3.415 min Scan# 74

Delta R.T. -0.007 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04

Instrument :

BNA\_N

ClientSampleId :

PB168563BSD





Tgt Ion: 42 Resp: 653

Ion Ratio Lower Upper

42 100

74 137.4 84.3 126.5#

44 10.1 5.0 7.4#

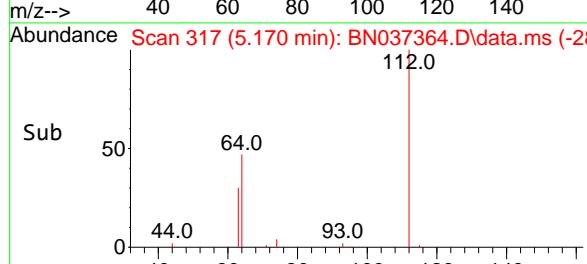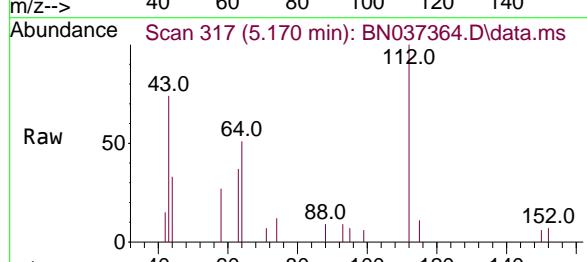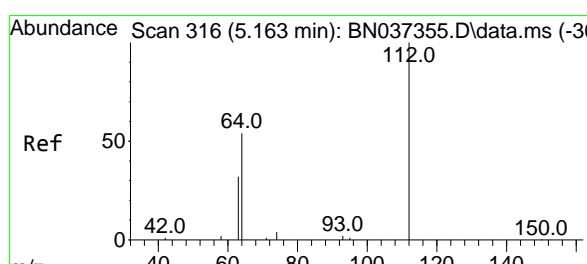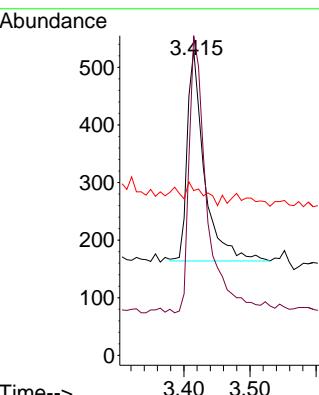

#4

2-Fluorophenol

Concen: 0.338 ng

RT: 5.170 min Scan# 317

Delta R.T. 0.007 min

Lab File: BN037364.D

Acq: 21 Jun 2025 00:04


Tgt Ion: 112 Resp: 1274


Ion Ratio Lower Upper

112 100


64 50.5 38.7 58.1

63 33.0 26.4 39.6



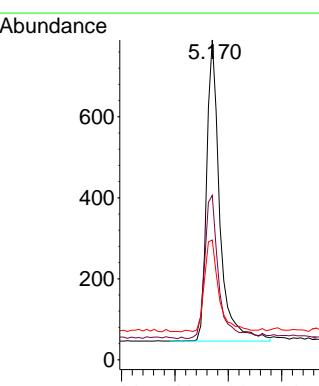





#5  
 Phenol-d6  
 Concen: 0.346 ng  
 RT: 6.752 min Scan# 5:Instrument :  
 Delta R.T. -0.000 min BNA\_N  
 Lab File: BN037364.D ClientSampleId :  
 Acq: 21 Jun 2025 00:04 PB168563BSD





Tgt Ion: 99 Resp: 1342  
 Ion Ratio Lower Upper  
 99 100  
 42 21.1 19.8 29.8  
 71 42.0 42.6 64.0#

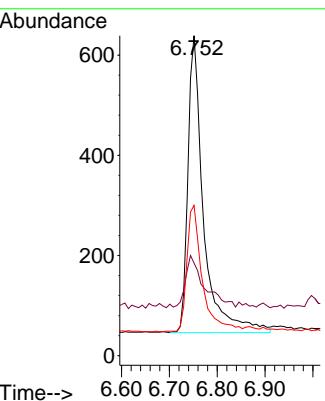


#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.366 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04




Tgt Ion: 93 Resp: 1260  
 Ion Ratio Lower Upper  
 93 100  
 63 66.8 53.2 79.8  
 95 32.7 27.3 40.9

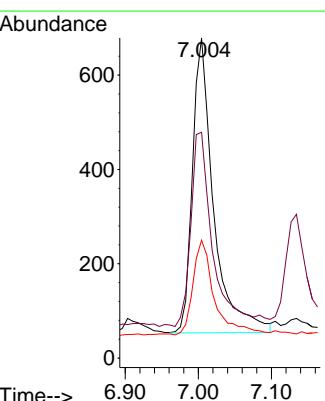






#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.340 min Scan# 942  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
ClientSampleId : PB168563BSD

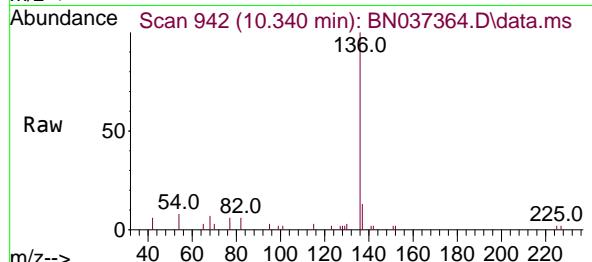



Tgt Ion:136 Resp: 4095  
Ion Ratio Lower Upper  
136 100  
137 13.1 12.2 18.2  
54 8.3 8.8 13.2#  
68 6.7 7.0 10.4#

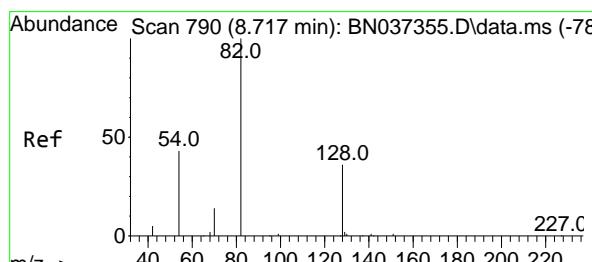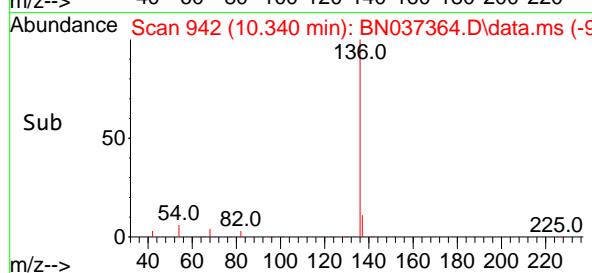


#8  
Nitrobenzene-d5  
Concen: 0.388 ng  
RT: 8.717 min Scan# 790  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

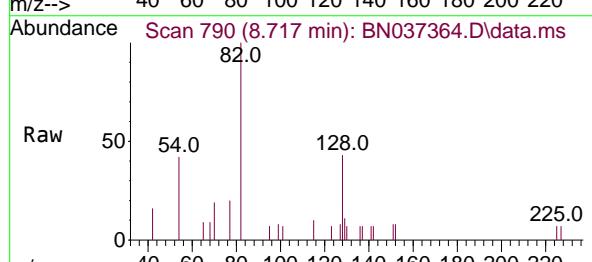


Tgt Ion: 82 Resp: 1284  
Ion Ratio Lower Upper  
82 100  
128 42.9 42.5 63.7  
54 41.7 43.2 64.8#

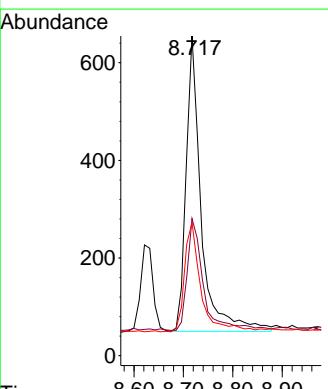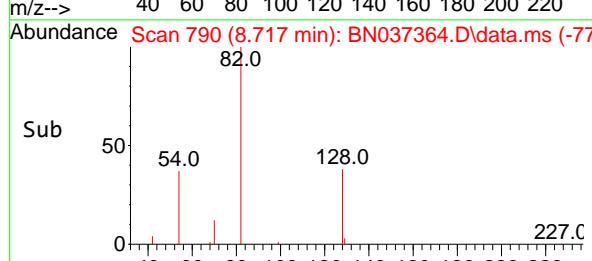






#9  
Naphthalene  
Concen: 0.372 ng  
RT: 10.394 min Scan# 947  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04


Instrument :  
BNA\_N  
ClientSampleId :  
PB168563BSD

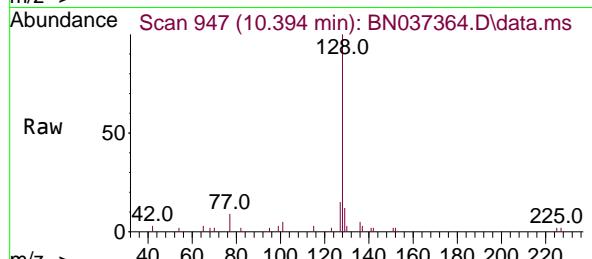



Tgt Ion:128 Resp: 4026  
Ion Ratio Lower Upper  
128 100  
129 12.4 14.0 21.0#  
127 14.9 15.8 23.8#

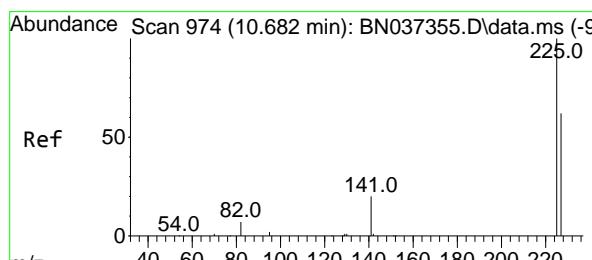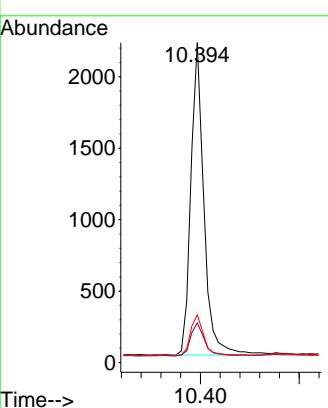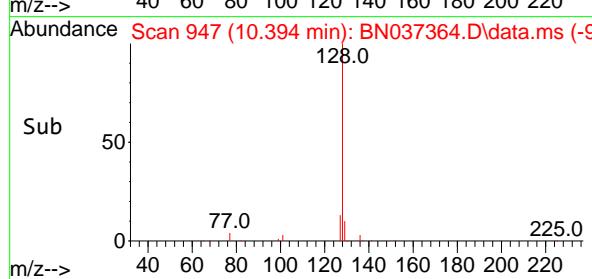


#10  
Hexachlorobutadiene  
Concen: 0.410 ng  
RT: 10.682 min Scan# 974  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

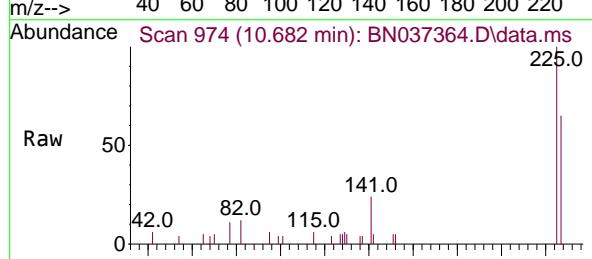


Tgt Ion:225 Resp: 1748  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 62.6 50.3 75.5


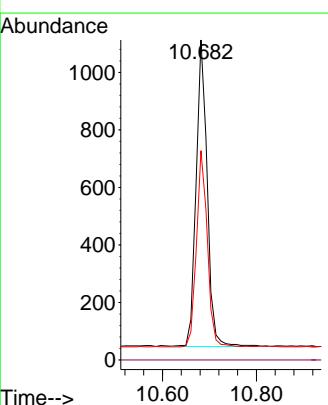
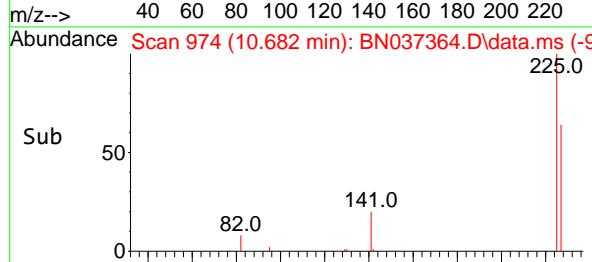





#11  
2-Methylnaphthalene-d10  
Concen: 0.588 ng  
RT: 11.945 min Scan# 1:Instrument :  
Delta R.T. -0.000 min BNA\_N  
Lab File: BN037364.D ClientSampleId :  
Acq: 21 Jun 2025 00:04 PB168563BSD

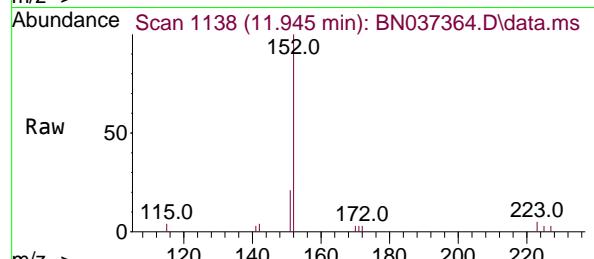



Tgt Ion:152 Resp: 3901  
Ion Ratio Lower Upper  
152 100  
151 13.8 17.4 26.0#

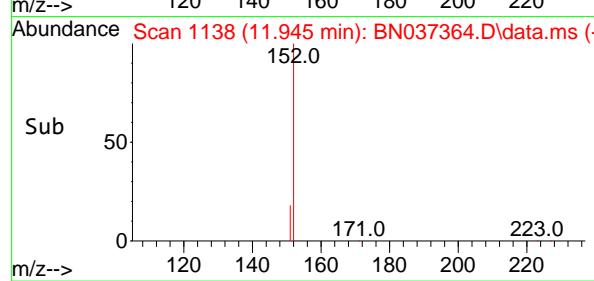


#12  
2-Methylnaphthalene  
Concen: 0.328 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

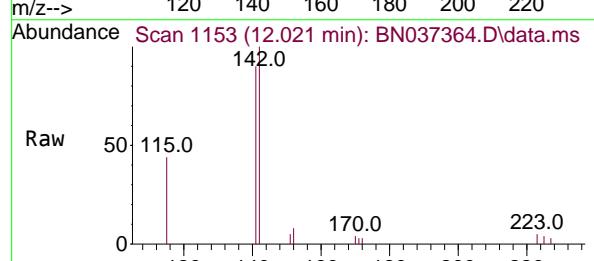

Tgt Ion:142 Resp: 2474  
Ion Ratio Lower Upper  
142 100  
141 90.0 70.2 105.2  
115 43.6 43.0 64.4

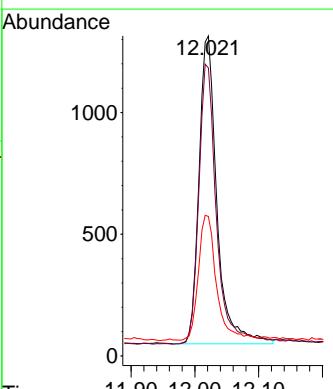



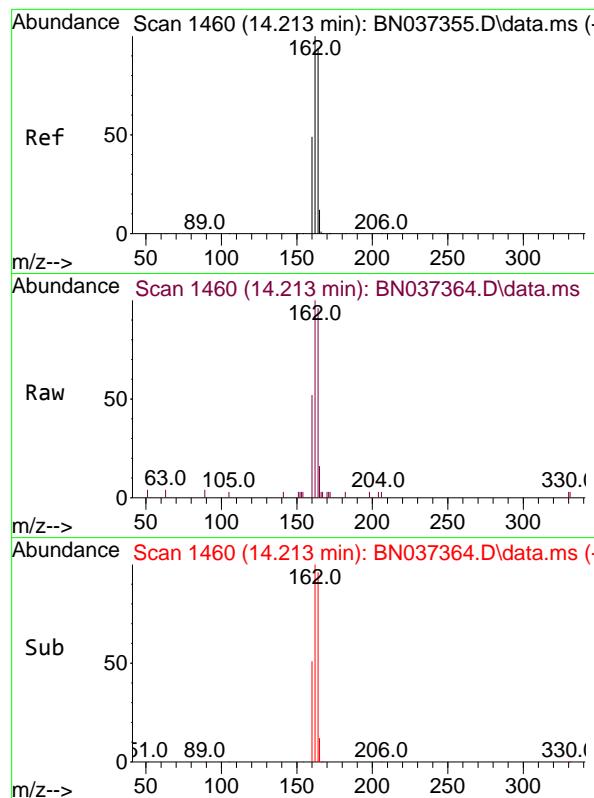

#13  
 Acenaphthene-d10  
 Concen: 0.400 ng  
 RT: 14.213 min Scan# 14  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


Tgt Ion:164 Resp: 2623  
 Ion Ratio Lower Upper  
 164 100  
 162 104.1 81.5 122.3  
 160 54.5 43.0 64.4

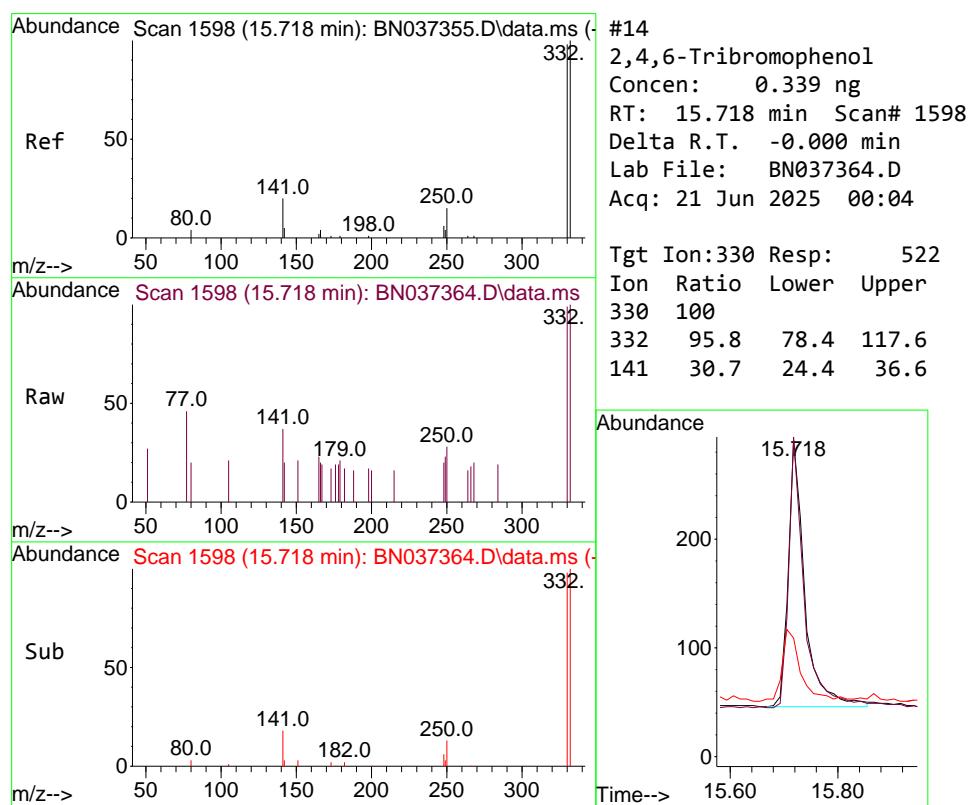

#14  
 2,4,6-Tribromophenol  
 Concen: 0.339 ng  
 RT: 15.718 min Scan# 1598  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04



Tgt Ion:330 Resp: 522  
 Ion Ratio Lower Upper  
 330 100  
 332 95.8 78.4 117.6  
 141 30.7 24.4 36.6

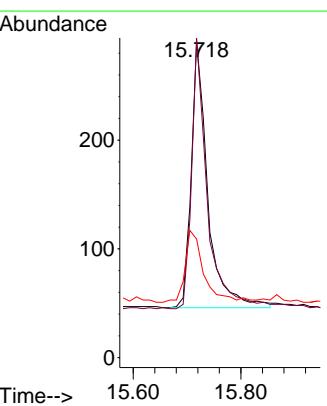

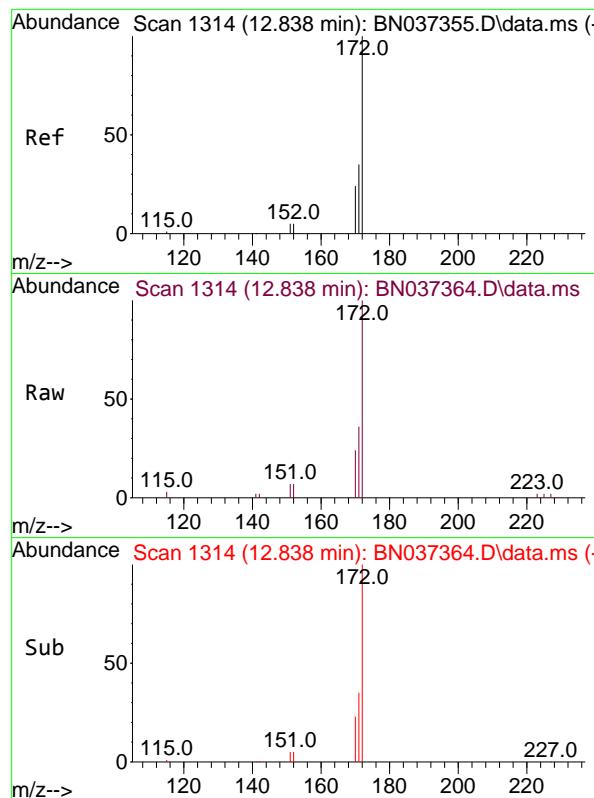


#15  
2-Fluorobiphenyl  
Concen: 0.397 ng  
RT: 12.838 min Scan# 1:Instrument :  
Delta R.T. -0.000 min BNA\_N  
Lab File: BN037364.D ClientSampleId :  
Acq: 21 Jun 2025 00:04 PB168563BSD


Tgt Ion:172 Resp: 4574  
Ion Ratio Lower Upper  
172 100  
171 36.5 30.8 46.2  
170 24.2 21.9 32.9

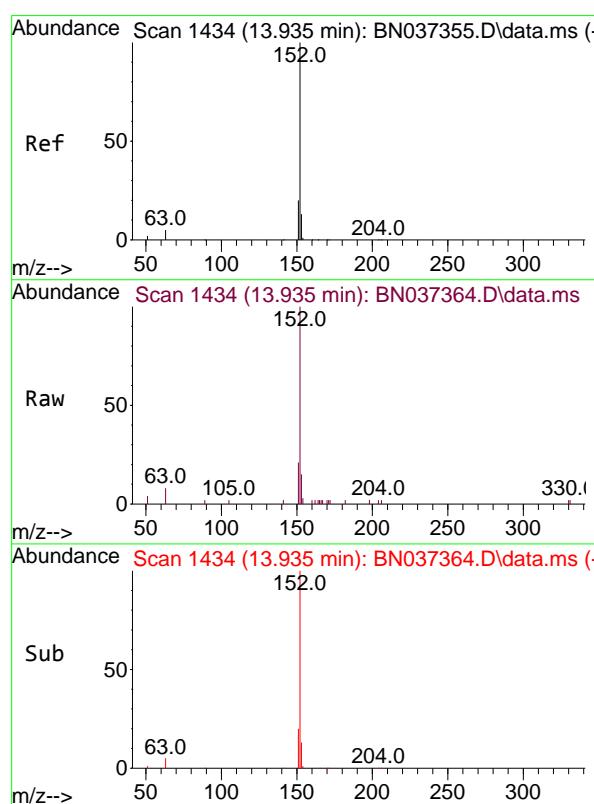


#16  
Acenaphthylene  
Concen: 0.403 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:152 Resp: 4445  
Ion Ratio Lower Upper  
152 100  
151 19.4 16.6 24.8  
153 13.3 10.2 15.2









#17  
Acenaphthene  
Concen: 0.364 ng  
RT: 14.277 min Scan# 14  
Instrument :  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04  
ClientSampleId : PB168563BSD





Tgt Ion:154 Resp: 2642  
Ion Ratio Lower Upper  
154 100  
153 118.2 93.1 139.7  
152 62.7 48.6 73.0

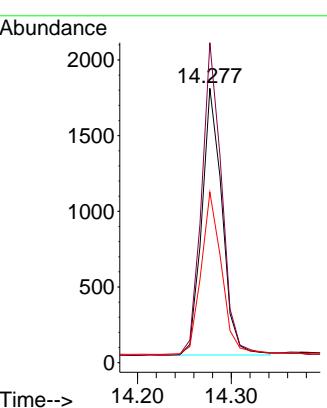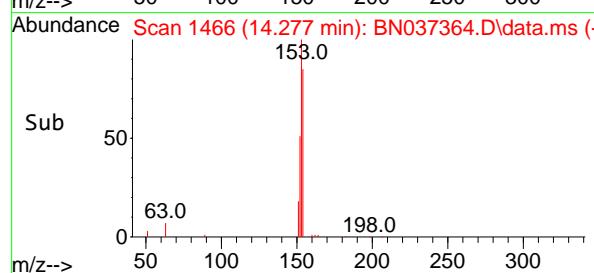


#18  
Fluorene  
Concen: 0.364 ng  
RT: 15.271 min Scan# 1559  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04




Tgt Ion:166 Resp: 3709  
Ion Ratio Lower Upper  
166 100  
165 100.1 79.5 119.3  
167 13.8 10.7 16.1





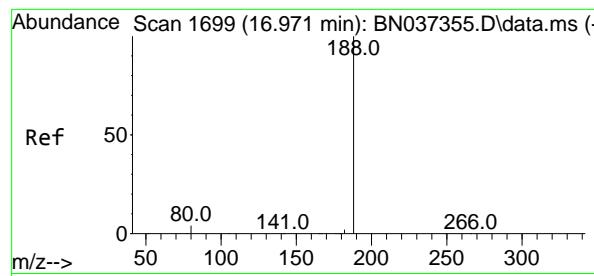


#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
 ClientSampleId : PB168563BSD






Tgt Ion:188 Resp: 5035  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 5.9 6.2 9.2#

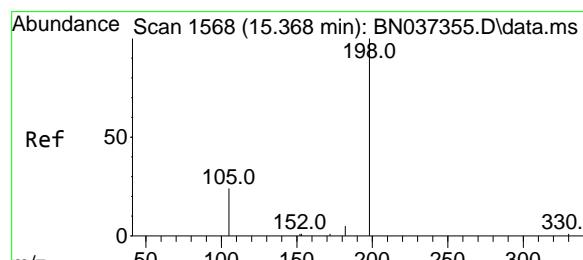

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.346 ng  
 RT: 15.378 min Scan# 1569  
 Delta R.T. 0.011 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04



Tgt Ion:198 Resp: 419  
 Ion Ratio Lower Upper  
 198 100  
 51 46.7 51.4 77.0#  
 105 46.2 45.5 68.3

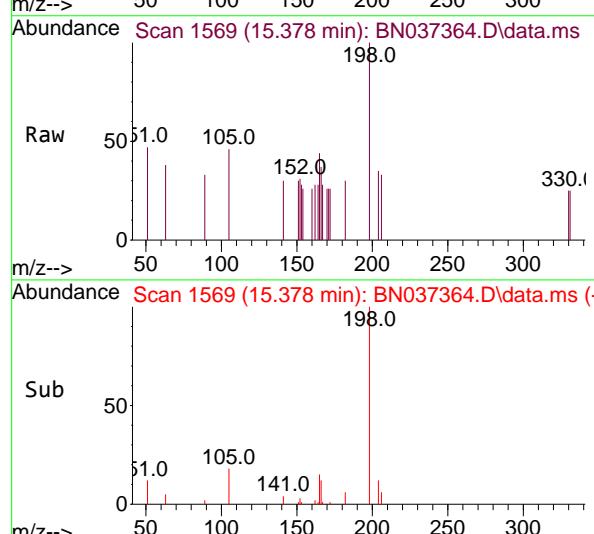

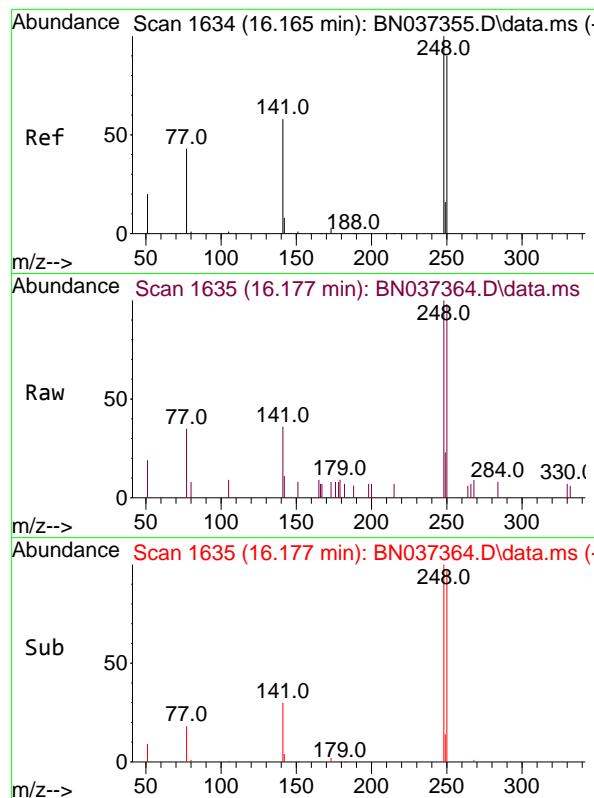


#21  
4-Bromophenyl-phenylether  
Concen: 0.375 ng  
RT: 16.177 min Scan# 1  
Instrument: BNA\_N  
Delta R.T. 0.012 min  
Lab File: BN037364.D  
ClientSampleId : PB168563BSD  
Acq: 21 Jun 2025 00:04


Tgt Ion:248 Resp: 1344  
Ion Ratio Lower Upper  
248 100  
250 98.2 80.4 120.6  
141 35.7 33.3 49.9

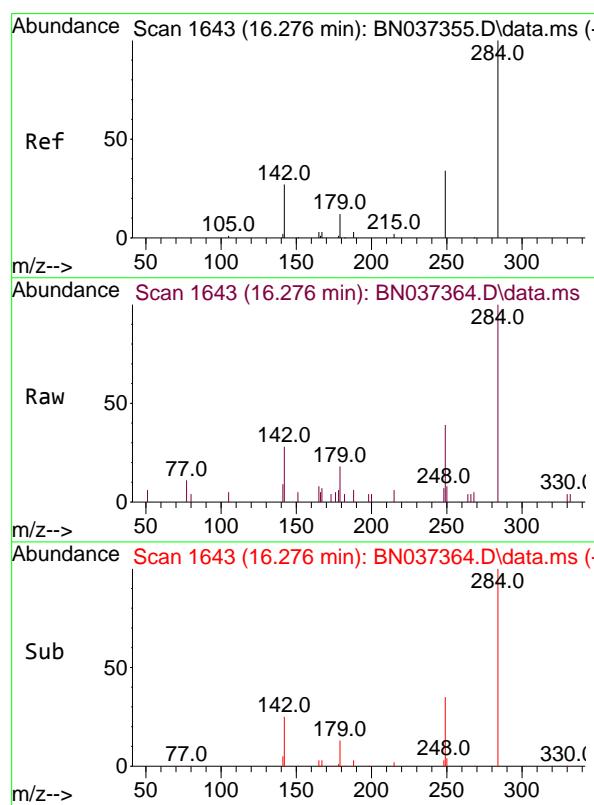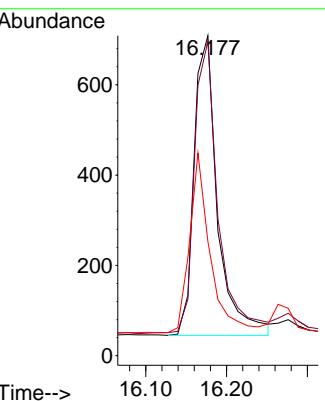

#22  
Hexachlorobenzene  
Concen: 0.409 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04


Tgt Ion:284 Resp: 1596  
Ion Ratio Lower Upper  
284 100  
142 33.3 27.0 40.6  
249 35.8 28.8 43.2

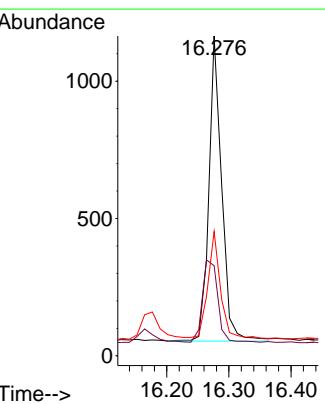



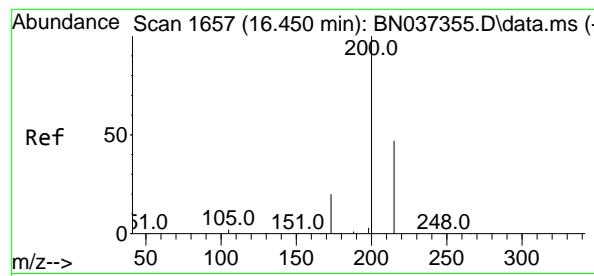


#23  
Atrazine  
Concen: 0.354 ng  
RT: 16.450 min Scan# 1  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
ClientSampleId : PB168563BSD





Tgt Ion:200 Resp: 1011  
Ion Ratio Lower Upper  
200 100  
173 28.3 29.2 43.8#  
215 53.3 48.8 73.2


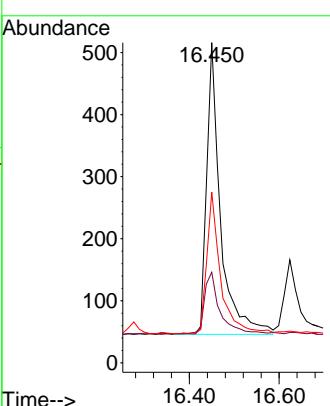
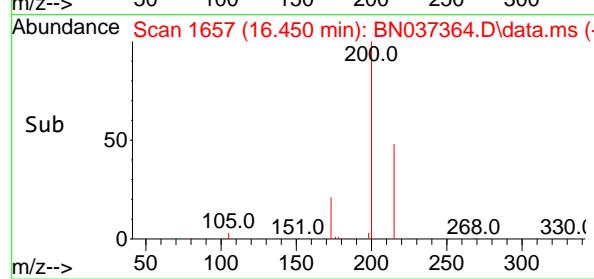


#24  
Pentachlorophenol  
Concen: 0.688 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04



Tgt Ion:266 Resp: 1337  
Ion Ratio Lower Upper  
266 100  
264 62.5 50.3 75.5  
268 65.4 55.3 82.9



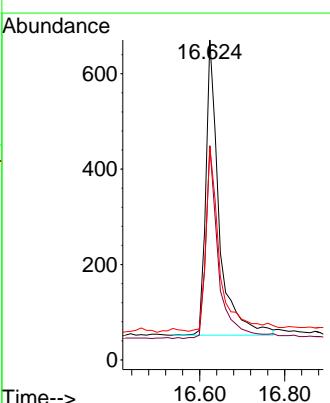





#25  
 Phenanthrene  
 Concen: 0.368 ng  
 RT: 17.009 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


Tgt Ion:178 Resp: 5370  
 Ion Ratio Lower Upper  
 178 100  
 176 19.5 15.2 22.8  
 179 15.8 12.9 19.3

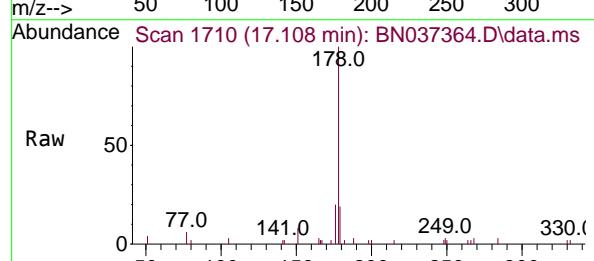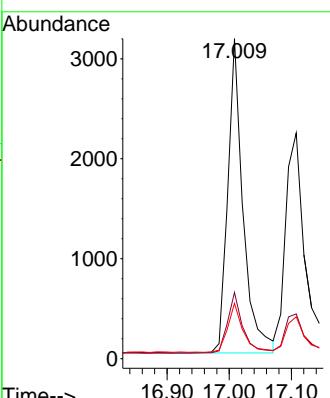

#26  
 Anthracene  
 Concen: 0.362 ng  
 RT: 17.108 min Scan# 1710  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Tgt Ion:178 Resp: 4862  
 Ion Ratio Lower Upper  
 178 100  
 176 18.5 14.7 22.1  
 179 15.5 13.0 19.6


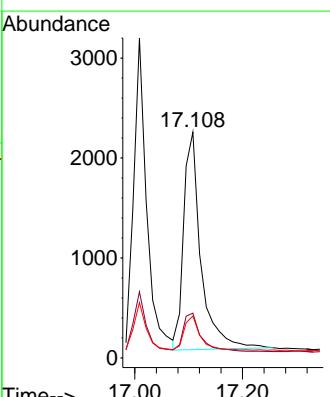


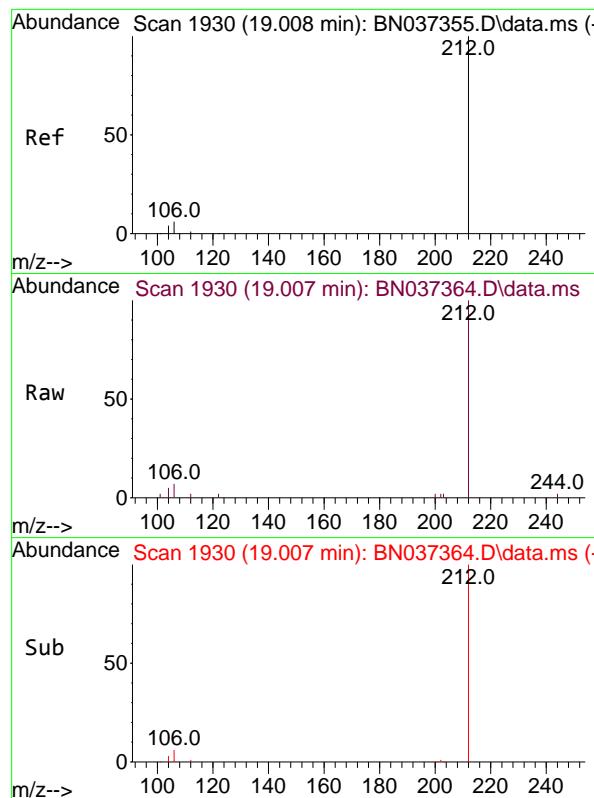

#27  
 Fluoranthene-d10  
 Concen: 0.346 ng  
 RT: 19.007 min Scan# 1930  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


Tgt Ion:212 Resp: 5003  
 Ion Ratio Lower Upper  
 212 100  
 106 6.2 3.0 4.4#  
 104 3.7 2.0 3.0#

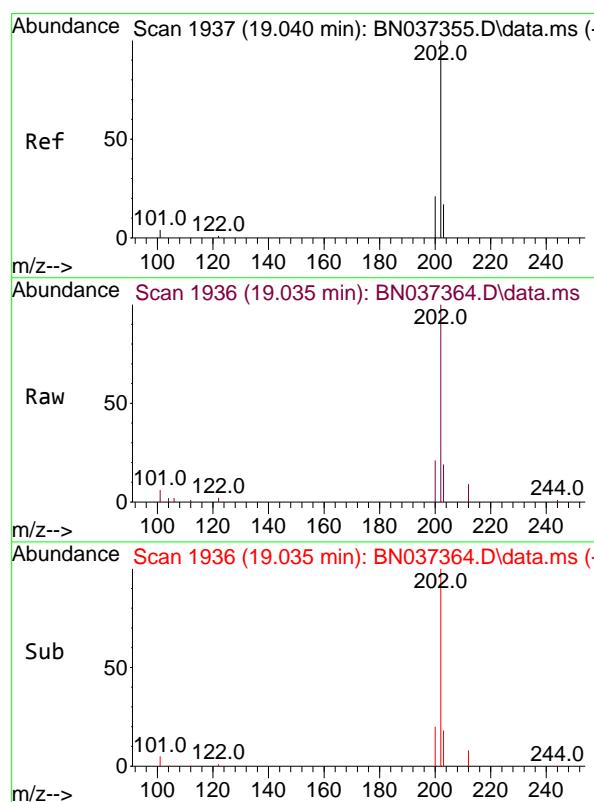

#28  
 Fluoranthene  
 Concen: 0.339 ng  
 RT: 19.035 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Tgt Ion:202 Resp: 6244  
 Ion Ratio Lower Upper  
 202 100  
 101 4.9 3.0 4.6#  
 203 16.9 13.7 20.5





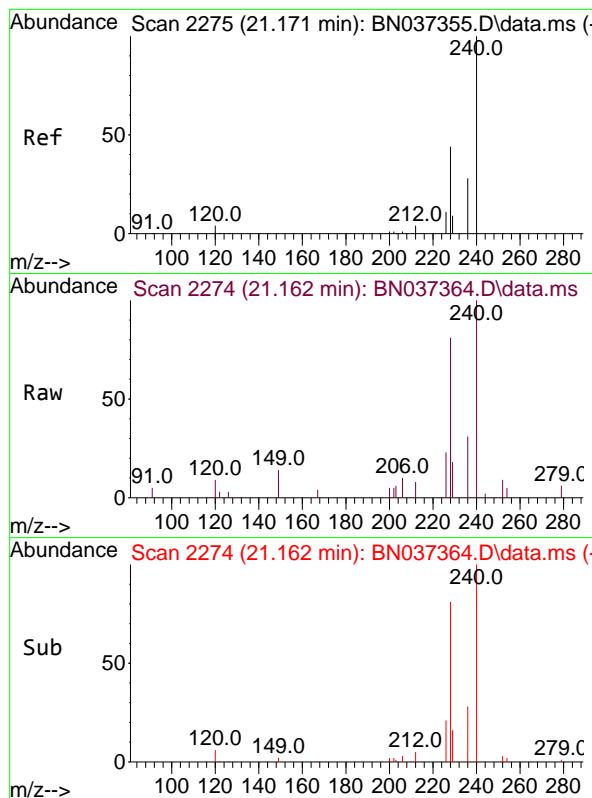

#29  
 Chrysene-d12  
 Concen: 0.400 ng  
 RT: 21.162 min Scan# 21  
 Delta R.T. -0.009 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


Tgt Ion:240 Resp: 4193  
 Ion Ratio Lower Upper  
 240 100  
 120 9.4 7.5 11.3  
 236 30.7 24.9 37.3

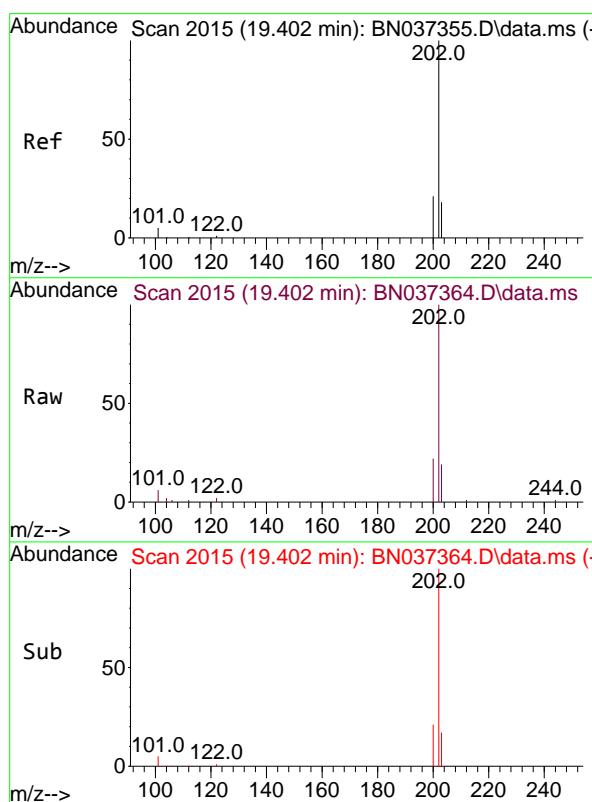

#30  
 Pyrene  
 Concen: 0.373 ng  
 RT: 19.402 min Scan# 2015  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Tgt Ion:202 Resp: 6351  
 Ion Ratio Lower Upper  
 202 100  
 200 20.7 16.8 25.2  
 203 18.4 14.5 21.7





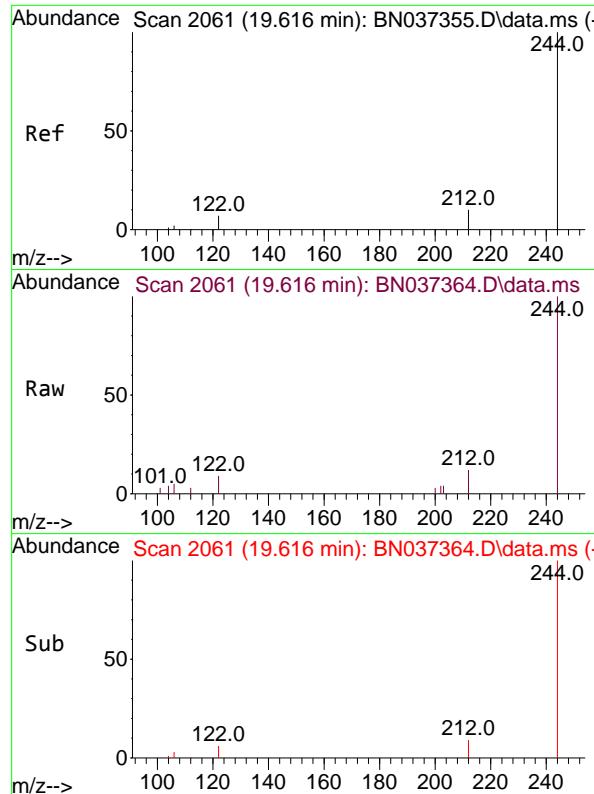

#31  
**Terphenyl-d14**  
Concen: 0.375 ng  
RT: 19.616 min Scan# 2061  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
ClientSampleId : PB168563BSD


Tgt Ion:244 Resp: 3587  
Ion Ratio Lower Upper  
244 100  
212 12.0 11.1 16.7  
122 8.8 7.2 10.8

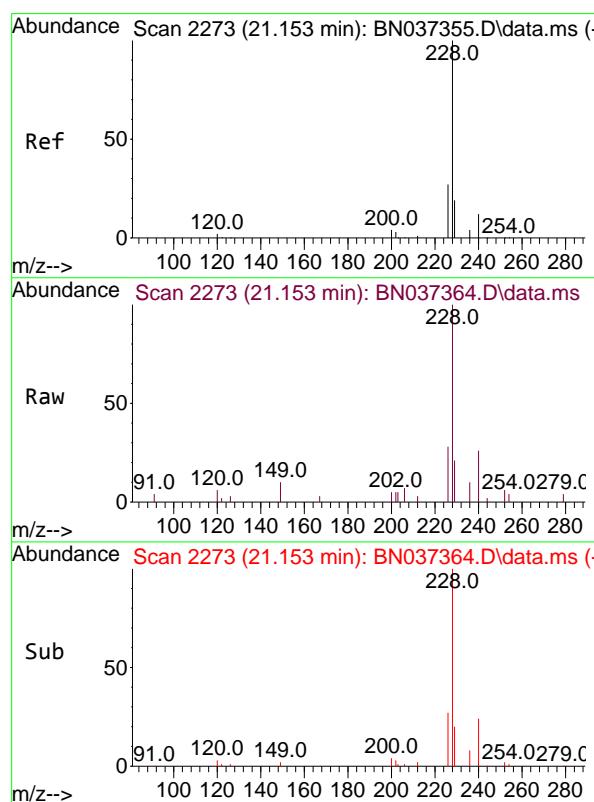

#32  
**Benzo(a)anthracene**  
Concen: 0.373 ng  
RT: 21.153 min Scan# 2273  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:228 Resp: 5141  
Ion Ratio Lower Upper  
228 100  
226 28.4 23.0 34.4  
229 21.1 17.4 26.0


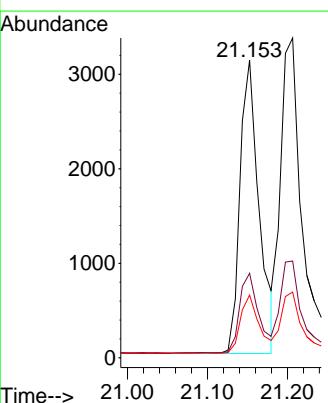


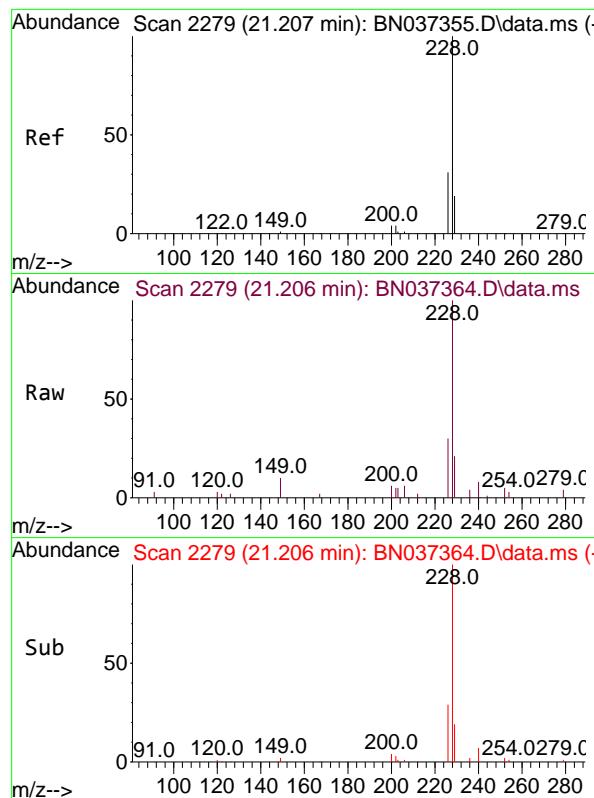

#33  
 Chrysene  
 Concen: 0.387 ng  
 RT: 21.206 min Scan# 21  
 Delta R.T. -0.000 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


Tgt Ion:228 Resp: 6472  
 Ion Ratio Lower Upper  
 228 100  
 226 30.3 25.4 38.2  
 229 20.6 17.3 25.9

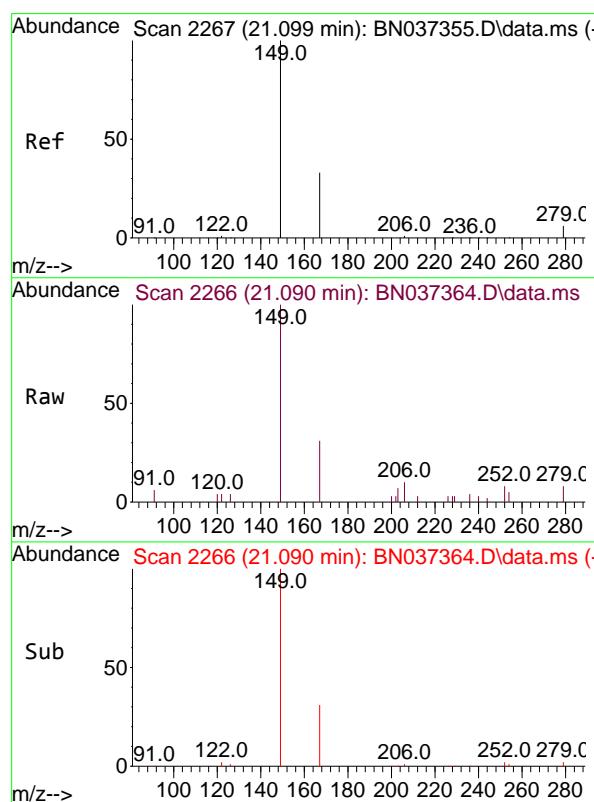

#34  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.358 ng  
 RT: 21.090 min Scan# 2266  
 Delta R.T. -0.009 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Tgt Ion:149 Resp: 2023  
 Ion Ratio Lower Upper  
 149 100  
 167 32.9 24.6 37.0  
 279 9.0 6.5 9.7





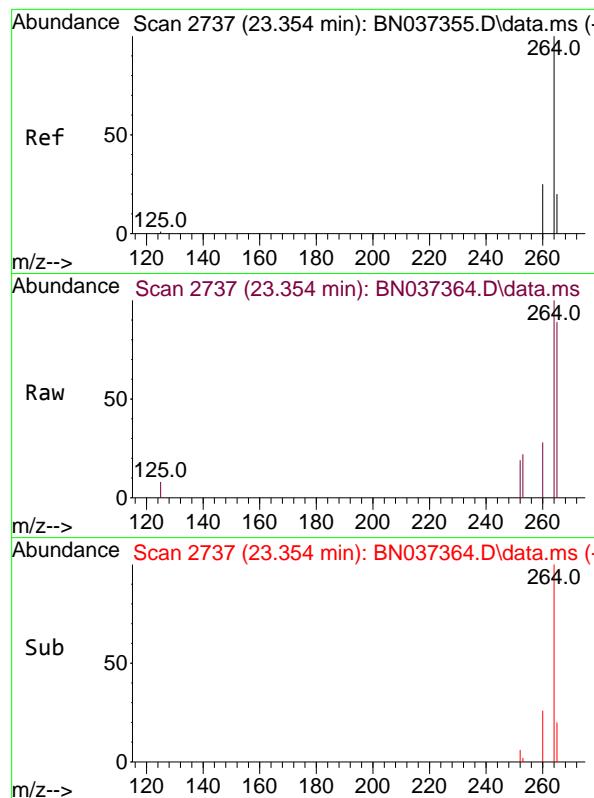

#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.354 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
ClientSampleId : PB168563BSD


Tgt Ion:264 Resp: 4470  
Ion Ratio Lower Upper  
264 100  
260 27.8 21.4 32.2  
265 89.4 71.4 107.0

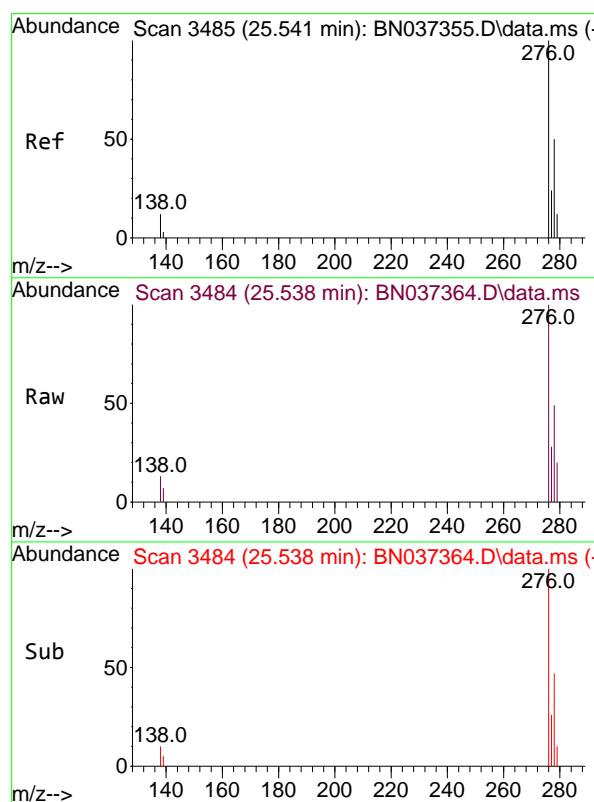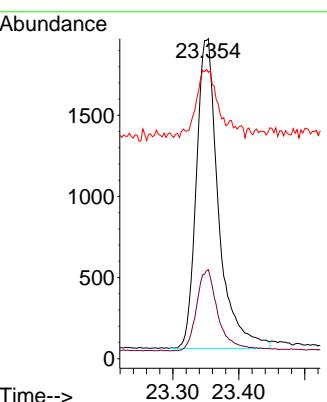

#36  
Indeno(1,2,3-cd)pyrene  
Concen: 0.386 ng  
RT: 25.538 min Scan# 3484  
Delta R.T. -0.003 min  
Lab File: BN037364.D  
Acq: 21 Jun 2025 00:04

Tgt Ion:276 Resp: 7744  
Ion Ratio Lower Upper  
276 100  
138 10.7 2.2 3.2#  
277 24.0 17.1 25.7





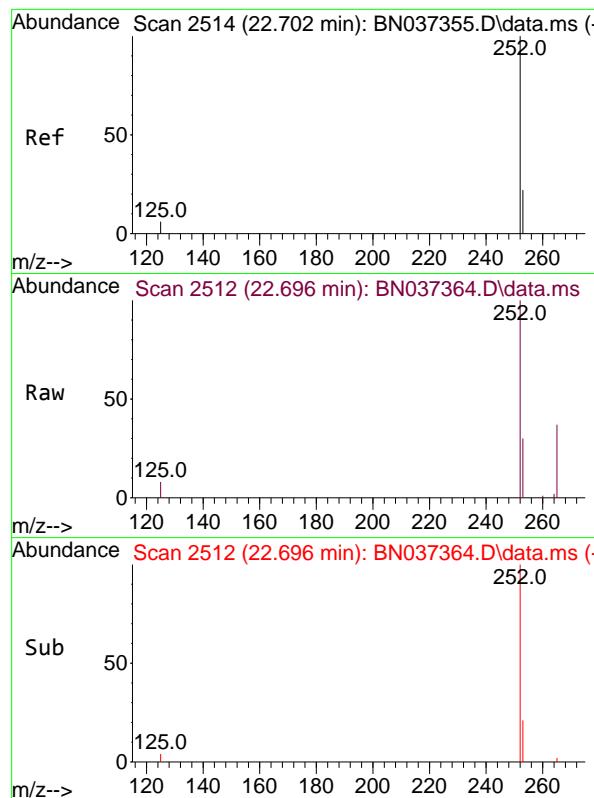

#37  
 Benzo(b)fluoranthene  
 Concen: 0.355 ng  
 RT: 22.696 min Scan# 21  
 Delta R.T. -0.006 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


Tgt Ion:252 Resp: 5838  
 Ion Ratio Lower Upper  
 252 100  
 253 30.4 26.6 40.0  
 125 8.3 6.1 9.1

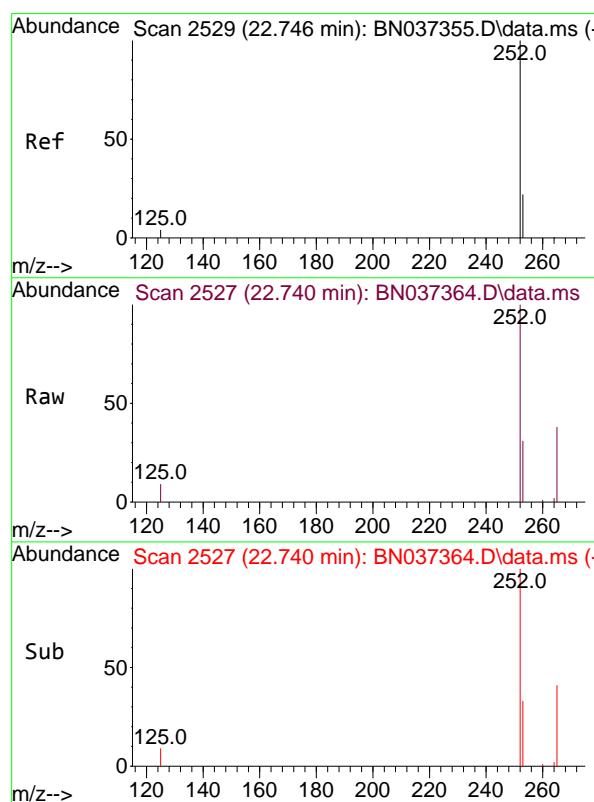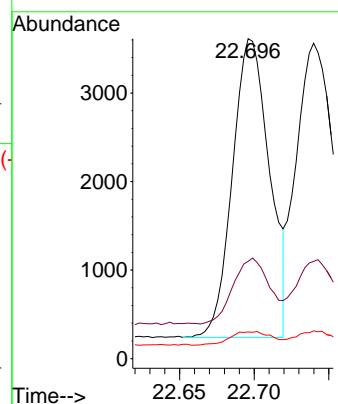

#38  
 Benzo(k)fluoranthene  
 Concen: 0.389 ng  
 RT: 22.740 min Scan# 2527  
 Delta R.T. -0.006 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Tgt Ion:252 Resp: 6945  
 Ion Ratio Lower Upper  
 252 100  
 253 30.8 26.7 40.1  
 125 8.8 6.5 9.7


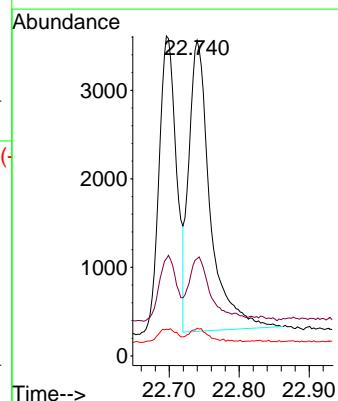


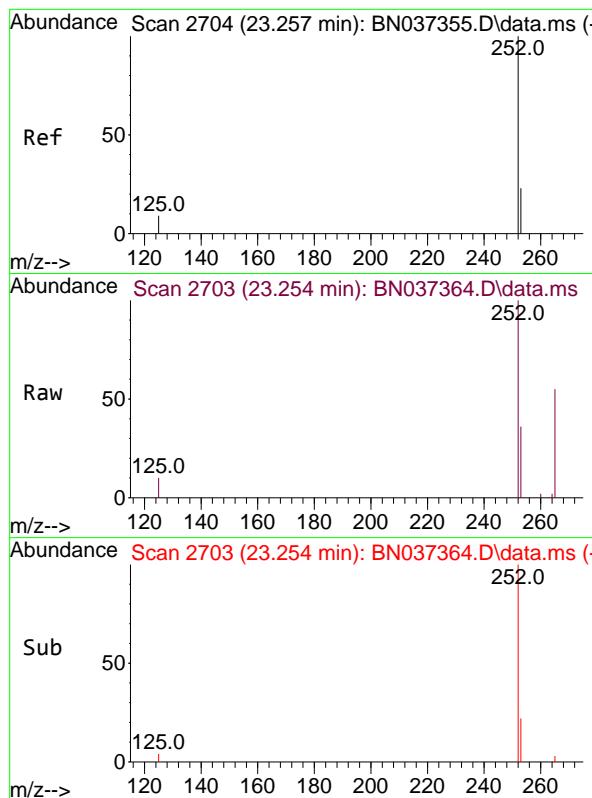

#39  
 Benzo(a)pyrene  
 Concen: 0.399 ng  
 RT: 23.254 min Scan# 21  
 Delta R.T. -0.003 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04


Instrument : BNA\_N  
 ClientSampleId : PB168563BSD


Tgt Ion:252 Resp: 5888  
 Ion Ratio Lower Upper  
 252 100  
 253 35.6 31.6 47.4  
 125 10.5 8.4 12.6

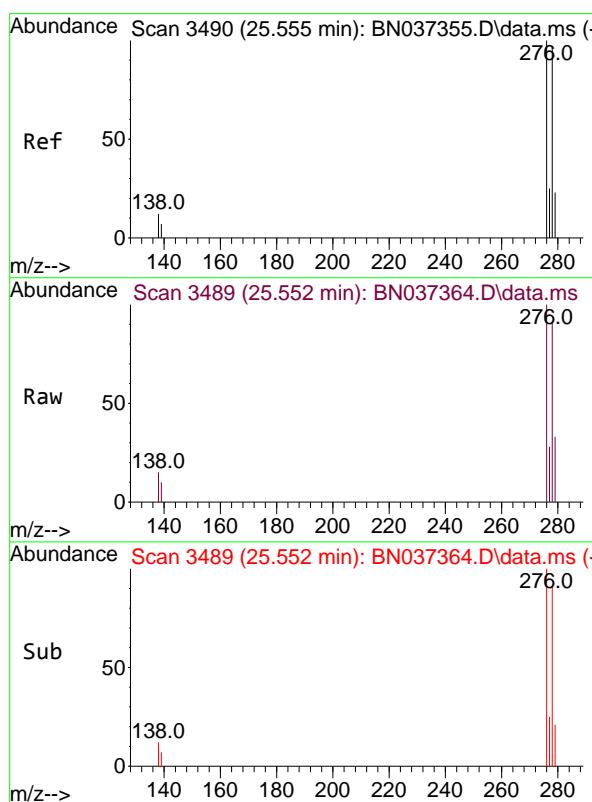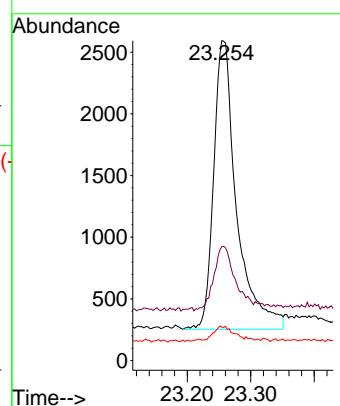

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.392 ng  
 RT: 25.552 min Scan# 3489  
 Delta R.T. -0.003 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Tgt Ion:278 Resp: 5912  
 Ion Ratio Lower Upper  
 278 100  
 139 11.3 10.2 15.4  
 279 36.2 35.6 53.4

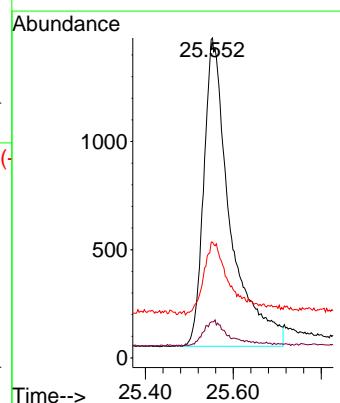


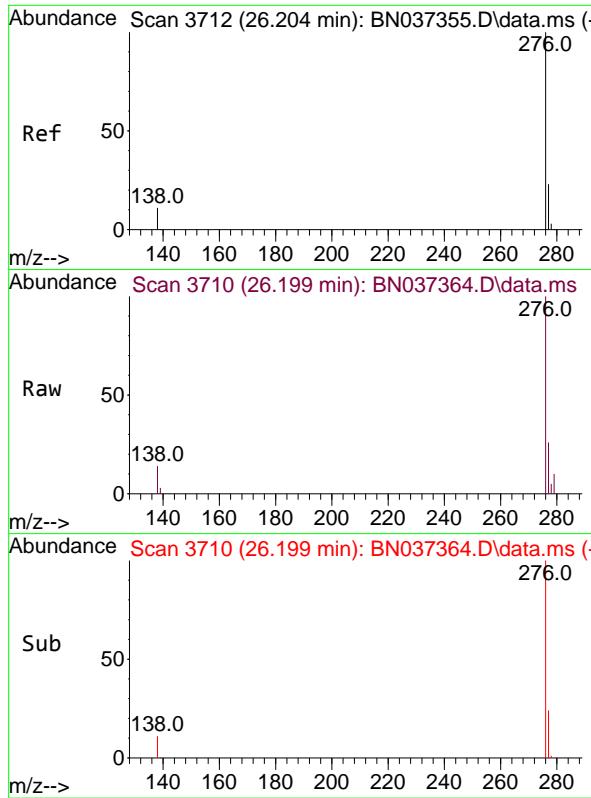

#41  
 Benzo(g,h,i)perylene  
 Concen: 0.393 ng  
 RT: 26.199 min Scan# 3  
 Delta R.T. -0.006 min  
 Lab File: BN037364.D  
 Acq: 21 Jun 2025 00:04

Instrument : BNA\_N  
 ClientSampleId : PB168563BSD

Tgt Ion:276 Resp: 7039  
 Ion Ratio Lower Upper  
 276 100  
 277 26.4 22.7 34.1  
 138 13.5 9.4 14.2

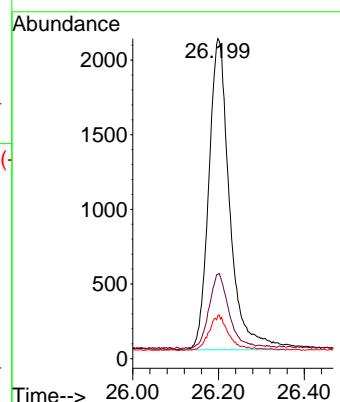

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037365.D  
 Acq On : 21 Jun 2025 01:17  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**SSTDCCC0.4EC**

Quant Time: Jun 21 01:41:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.568	152	1894	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4150	0.400	ng	# 0.00
13) Acenaphthene-d10	14.213	164	2786	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5748	0.400	ng	# 0.00
29) Chrysene-d12	21.162	240	5140	0.400	ng	0.00
35) Perylene-d12	23.351	264	5682	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	1402	0.370	ng	0.00
5) Phenol-d6	6.752	99	1426	0.366	ng	0.00
8) Nitrobenzene-d5	8.717	82	1321	0.394	ng	0.00
11) 2-Methylnaphthalene-d10	11.945	152	2780	0.413	ng	0.00
14) 2,4,6-Tribromophenol	15.718	330	608	0.372	ng	0.00
15) 2-Fluorobiphenyl	12.838	172	4951	0.405	ng	0.00
27) Fluoranthene-d10	19.008	212	6836	0.414	ng	0.00
31) Terphenyl-d14	19.616	244	4639	0.396	ng	0.00
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) 1,4-Dioxane	3.104	88	755	0.392	ng	95
3) n-Nitrosodimethylamine	3.422	42	701	0.397	ng	# 78
6) bis(2-Chloroethyl)ether	7.004	93	1274	0.368	ng	100
9) Naphthalene	10.394	128	4308	0.393	ng	# 90
10) Hexachlorobutadiene	10.682	225	1876	0.434	ng	# 100
12) 2-Methylnaphthalene	12.021	142	2941	0.385	ng	93
16) Acenaphthylene	13.935	152	4498	0.384	ng	98
17) Acenaphthene	14.277	154	2949	0.383	ng	98
18) Fluorene	15.272	166	4167	0.385	ng	99
20) 4,6-Dinitro-2-methylph...	15.379	198	483	0.350	ng	85
21) 4-Bromophenyl-phenylether	16.177	248	1621	0.396	ng	# 94
22) Hexachlorobenzene	16.276	284	1819	0.408	ng	99
23) Atrazine	16.450	200	1187	0.364	ng	# 87
24) Pentachlorophenol	16.624	266	805	0.363	ng	96
25) Phenanthrene	17.009	178	6282	0.377	ng	99
26) Anthracene	17.108	178	5522	0.360	ng	99
28) Fluoranthene	19.036	202	8102	0.385	ng	98
30) Pyrene	19.403	202	8105	0.388	ng	100
32) Benzo(a)anthracene	21.153	228	6359	0.376	ng	98
33) Chrysene	21.198	228	8015	0.391	ng	98
34) Bis(2-ethylhexyl)phtha...	21.090	149	2672	0.385	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.535	276	9725	0.382	ng	# 92
37) Benzo(b)fluoranthene	22.740	252	9018	0.431	ng	94
38) Benzo(k)fluoranthene	22.740	252	9018	0.398	ng	94
39) Benzo(a)pyrene	23.255	252	7122	0.380	ng	# 90
40) Dibenzo(a,h)anthracene	25.553	278	7424	0.388	ng	# 85
41) Benzo(g,h,i)perylene	26.199	276	8859	0.389	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062125\  
 Data File : BN037365.D  
 Acq On : 21 Jun 2025 01:17  
 Operator : RC/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4EC


Quant Time: Jun 21 01:41:01 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062125.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 20 23:41:54 2025  
 Response via : Initial Calibration

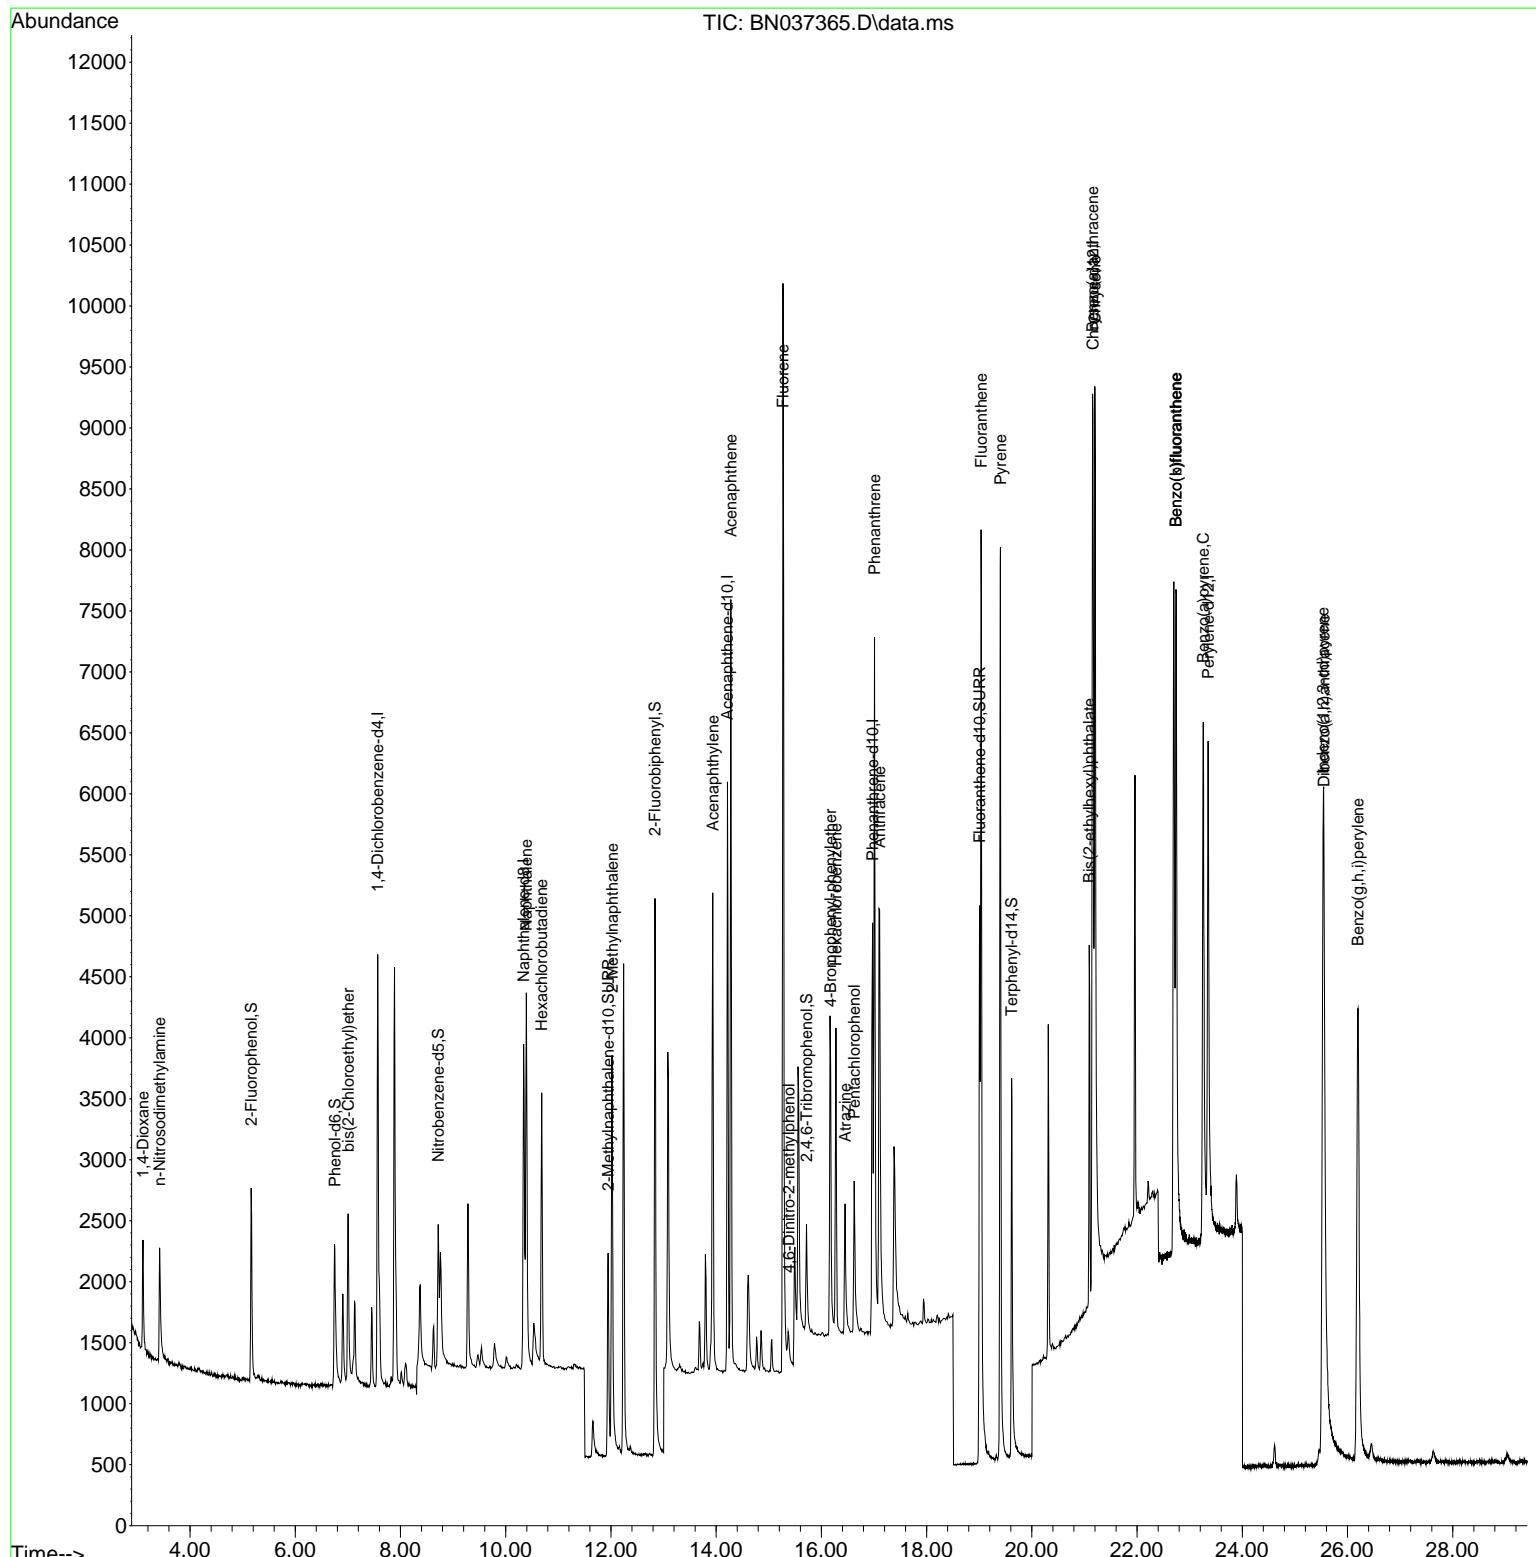






#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.568 min Scan# 64  
Delta R.T. -0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC





Tgt Ion:152 Resp: 1894  
Ion Ratio Lower Upper  
152 100  
150 149.8 112.7 169.1  
115 55.5 45.9 68.9






#2  
1,4-Dioxane  
Concen: 0.392 ng  
RT: 3.104 min Scan# 31  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17



Tgt Ion: 88 Resp: 755  
Ion Ratio Lower Upper  
88 100  
43 22.8 21.0 31.6  
58 49.9 38.0 57.0



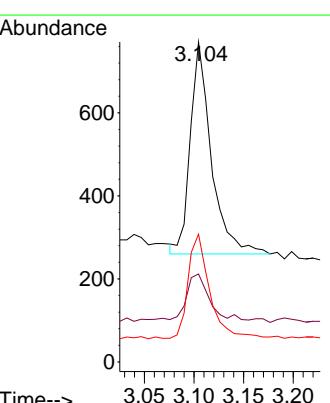



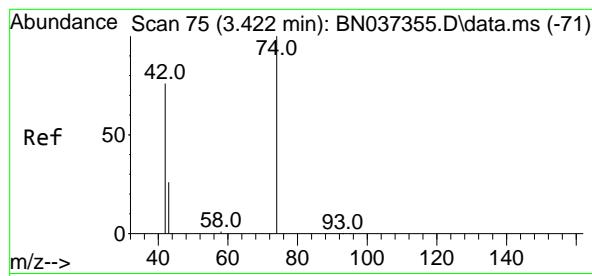

#3  
n-Nitrosodimethylamine  
Concen: 0.397 ng  
RT: 3.422 min Scan# 7  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17


Instrument :  
BNA\_N  
ClientSampleId :  
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 701  
Ion Ratio Lower Upper  
42 100  
74 129.2 84.3 126.5#  
44 9.3 5.0 7.4#

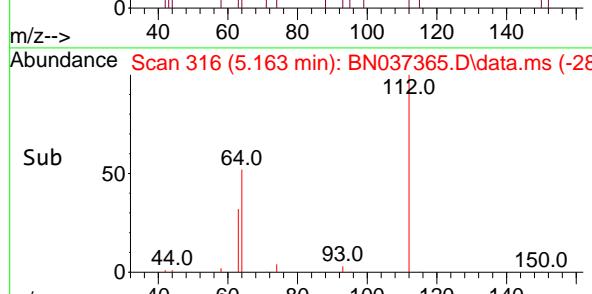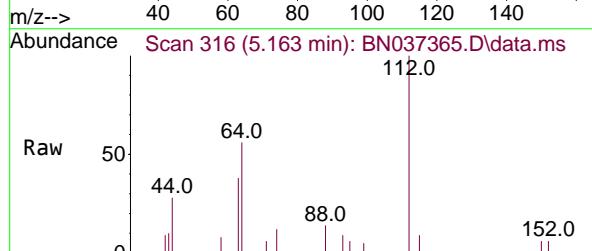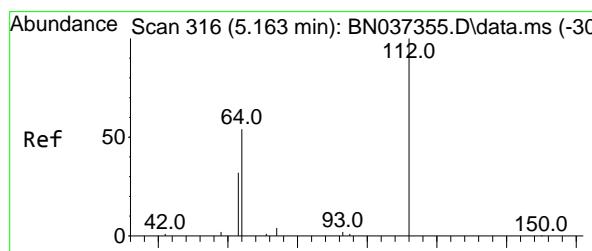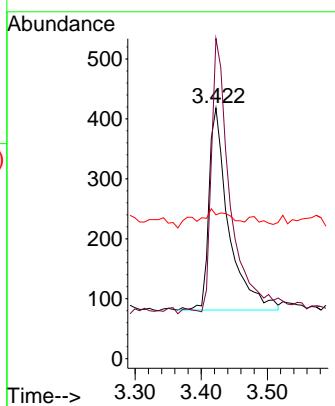


#4  
2-Fluorophenol  
Concen: 0.370 ng  
RT: 5.163 min Scan# 316  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion: 112 Resp: 1402  
Ion Ratio Lower Upper  
112 100  
64 52.2 38.7 58.1  
63 31.0 26.4 39.6



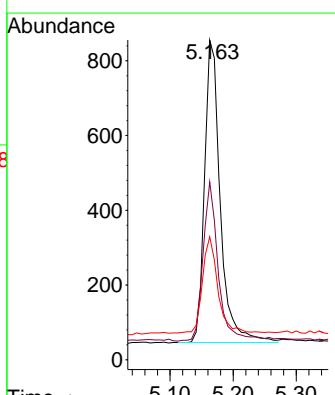


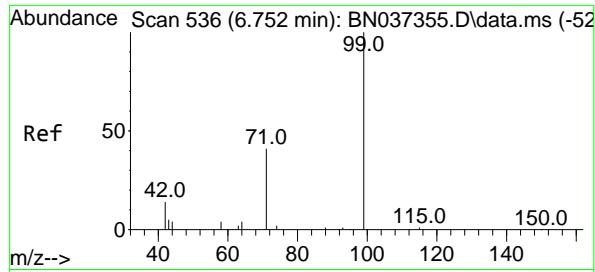


#5  
 Phenol-d6  
 Concen: 0.366 ng  
 RT: 6.752 min Scan# 5:Instrument :  
 Delta R.T. 0.000 min BNA\_N  
 Lab File: BN037365.D ClientSampleId :  
 Acq: 21 Jun 2025 01:17 SSTDCCC0.4EC

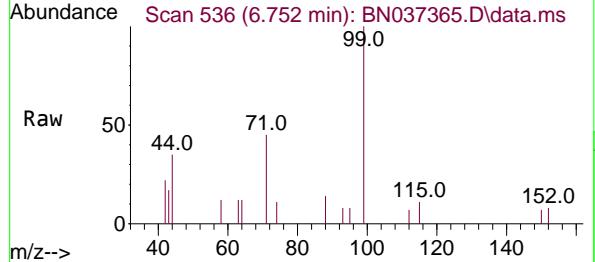



Tgt Ion: 99 Resp: 1426  
 Ion Ratio Lower Upper  
 99 100  
 42 18.2 19.8 29.8#  
 71 44.0 42.6 64.0

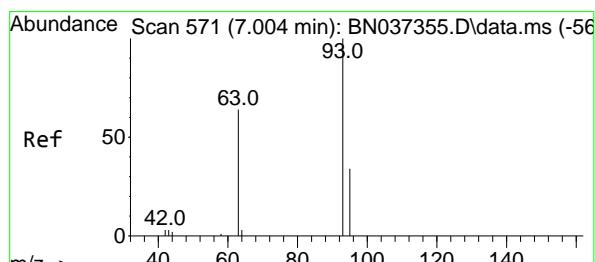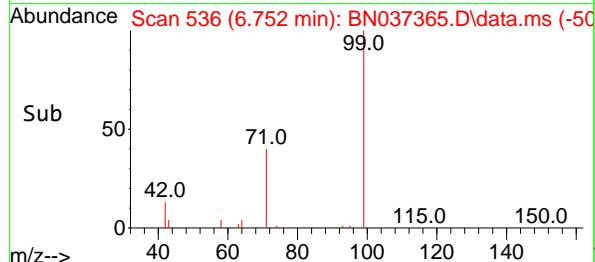


#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.368 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

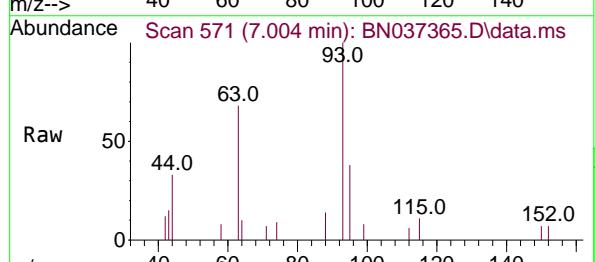


Tgt Ion: 93 Resp: 1274  
 Ion Ratio Lower Upper  
 93 100  
 63 66.6 53.2 79.8  
 95 33.8 27.3 40.9

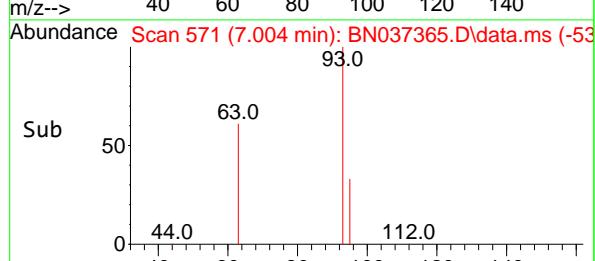



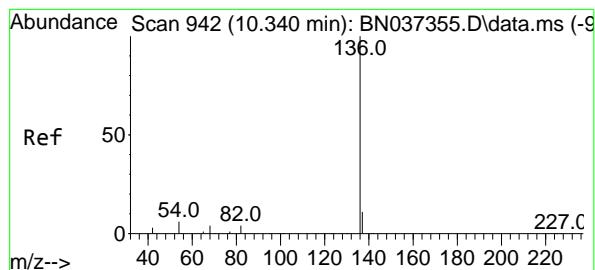


#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 942  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC

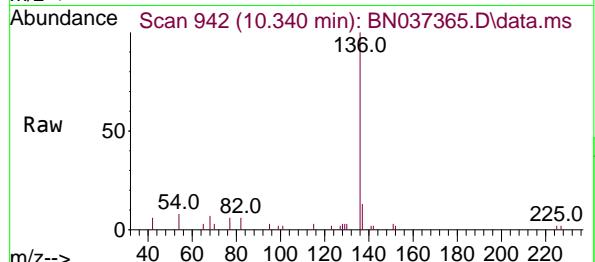



Tgt Ion:136 Resp: 4150  
 Ion Ratio Lower Upper  
 136 100  
 137 12.6 12.2 18.2  
 54 8.3 8.8 13.2#  
 68 6.8 7.0 10.4#

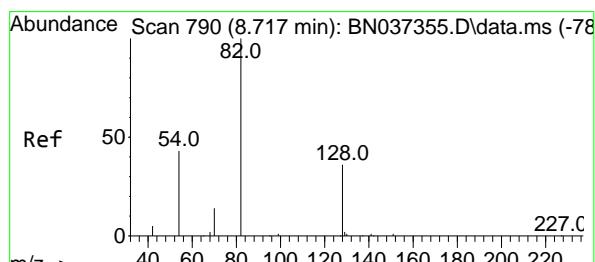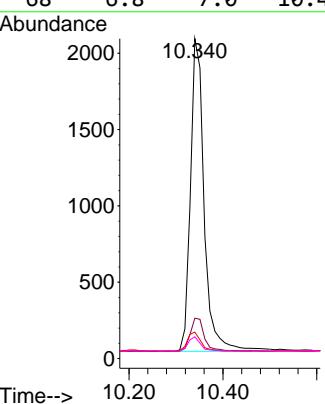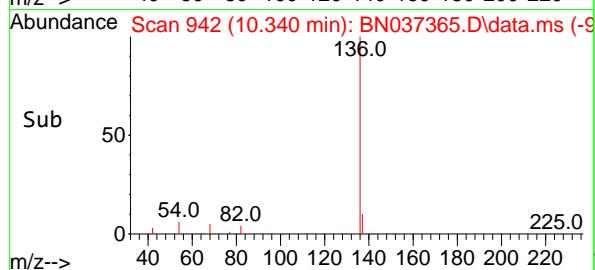


#8  
 Nitrobenzene-d5  
 Concen: 0.394 ng  
 RT: 8.717 min Scan# 790  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

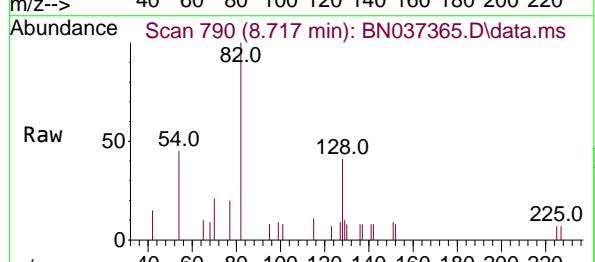


Tgt Ion: 82 Resp: 1321  
 Ion Ratio Lower Upper  
 82 100  
 128 41.4 42.5 63.7#  
 54 44.6 43.2 64.8

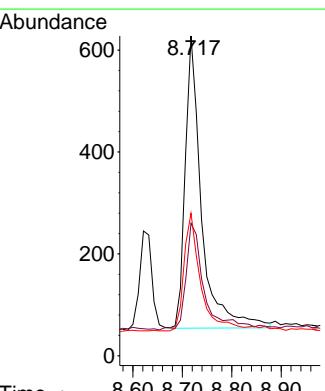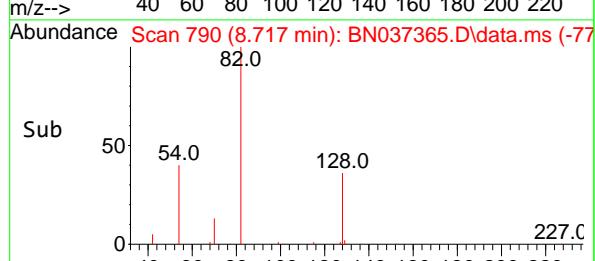



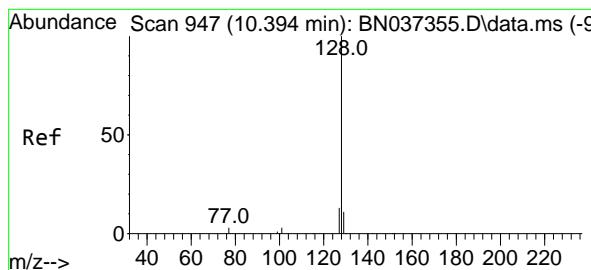


#9  
Naphthalene  
Concen: 0.393 ng  
RT: 10.394 min Scan# 947  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC

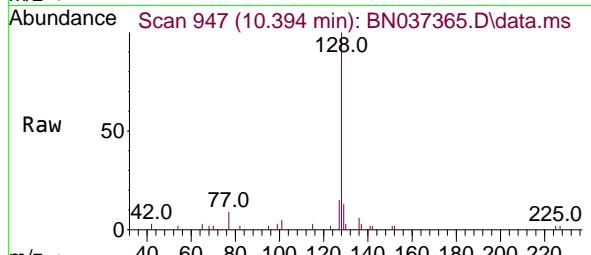



Tgt Ion:128 Resp: 4308  
Ion Ratio Lower Upper  
128 100  
129 12.7 14.0 21.0#  
127 15.2 15.8 23.8#

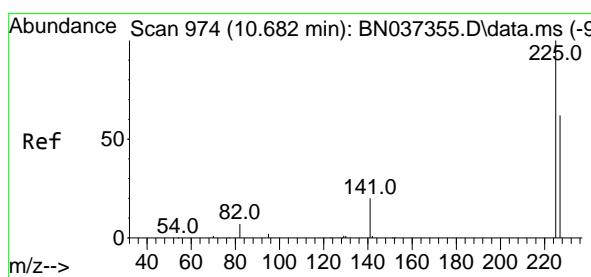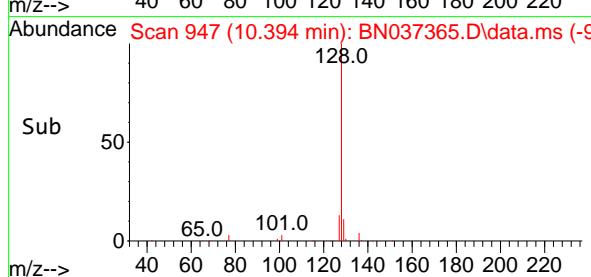


#10  
Hexachlorobutadiene  
Concen: 0.434 ng  
RT: 10.682 min Scan# 974  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

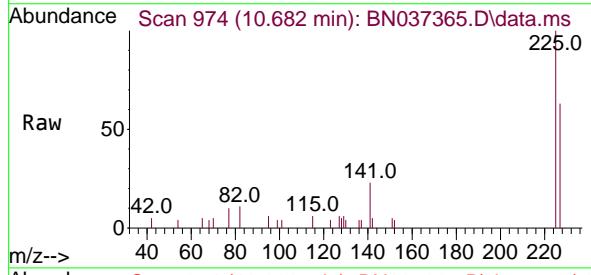

Tgt Ion:225 Resp: 1876  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 62.9 50.3 75.5


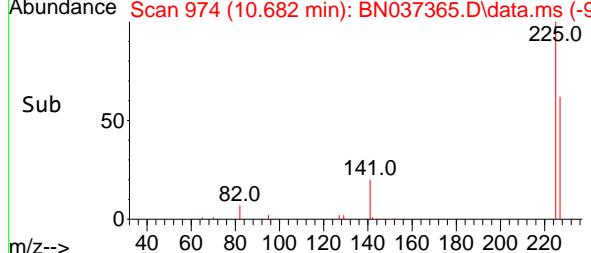


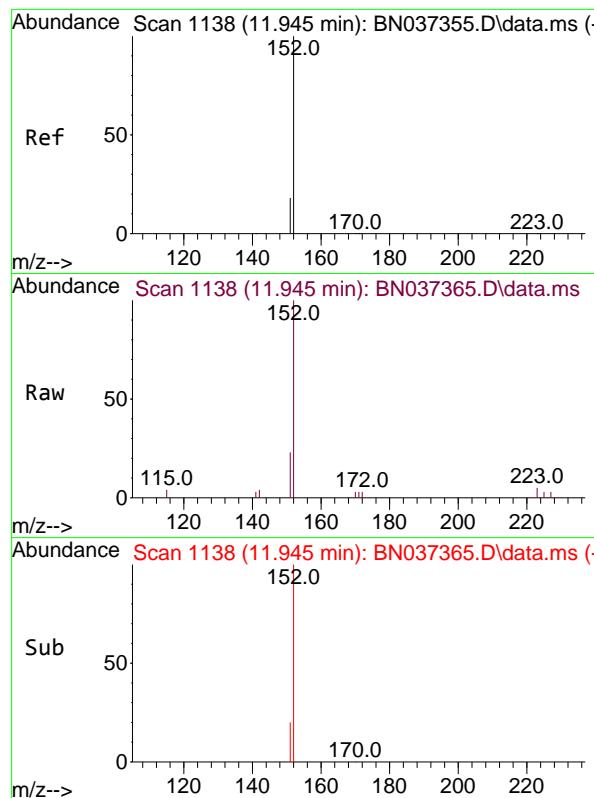

#11  
2-Methylnaphthalene-d10  
Concen: 0.413 ng  
RT: 11.945 min Scan# 1138  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC


Tgt Ion:152 Resp: 2780  
Ion Ratio Lower Upper  
152 100  
151 21.7 17.4 26.0

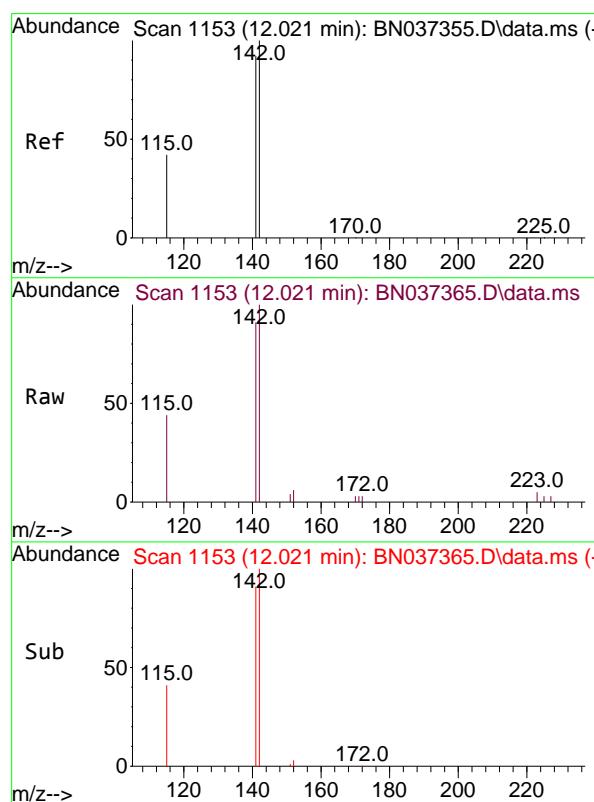

#12  
2-Methylnaphthalene  
Concen: 0.385 ng  
RT: 12.021 min Scan# 1153  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion:142 Resp: 2941  
Ion Ratio Lower Upper  
142 100  
141 90.9 70.2 105.2  
115 43.9 43.0 64.4





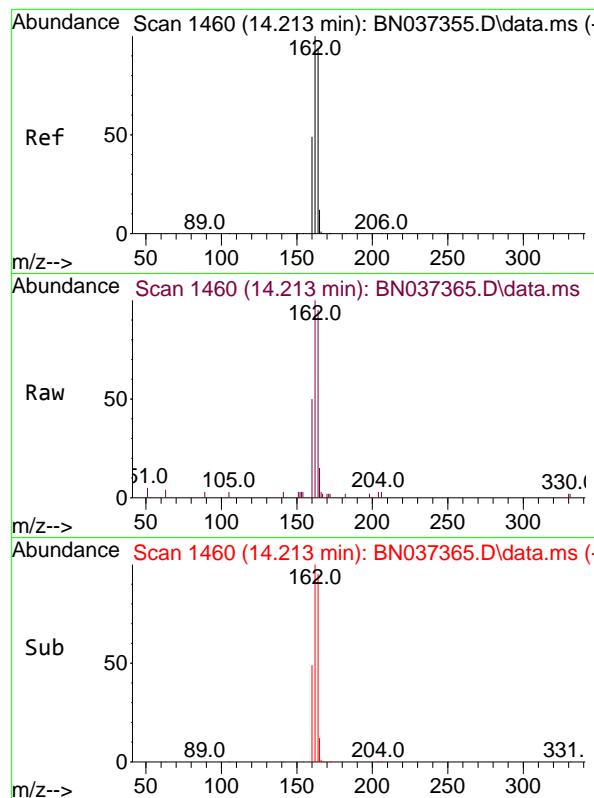

#13  
 Acenaphthene-d10  
 Concen: 0.400 ng  
 RT: 14.213 min Scan# 14  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:164 Resp: 2786  
 Ion Ratio Lower Upper  
 164 100  
 162 105.6 81.5 122.3  
 160 53.2 43.0 64.4

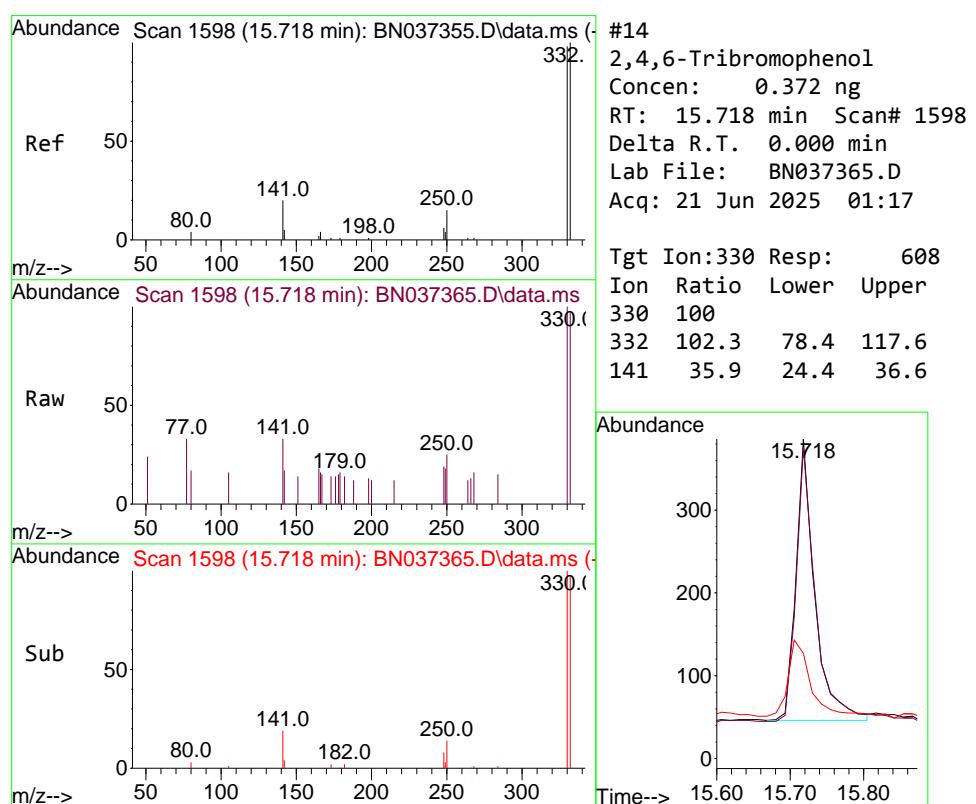

#14  
 2,4,6-Tribromophenol  
 Concen: 0.372 ng  
 RT: 15.718 min Scan# 1598  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17



Tgt Ion:330 Resp: 608  
 Ion Ratio Lower Upper  
 330 100  
 332 102.3 78.4 117.6  
 141 35.9 24.4 36.6

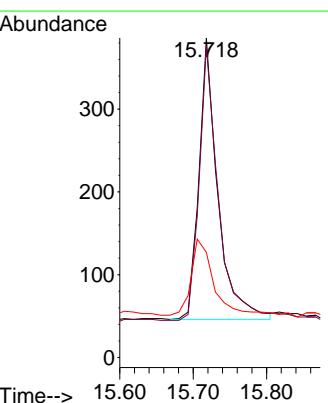

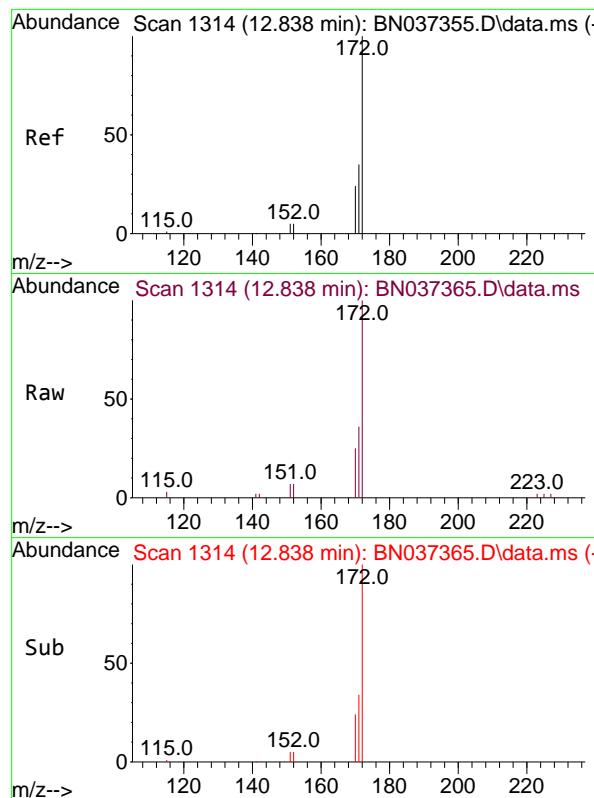


#15  
2-Fluorobiphenyl  
Concen: 0.405 ng  
RT: 12.838 min Scan# 1:Instrument :  
Delta R.T. 0.000 min BNA\_N  
Lab File: BN037365.D ClientSampleId :  
Acq: 21 Jun 2025 01:17 SSTDCCC0.4EC


Tgt Ion:172 Resp: 4951  
Ion Ratio Lower Upper  
172 100  
171 35.8 30.8 46.2  
170 25.4 21.9 32.9

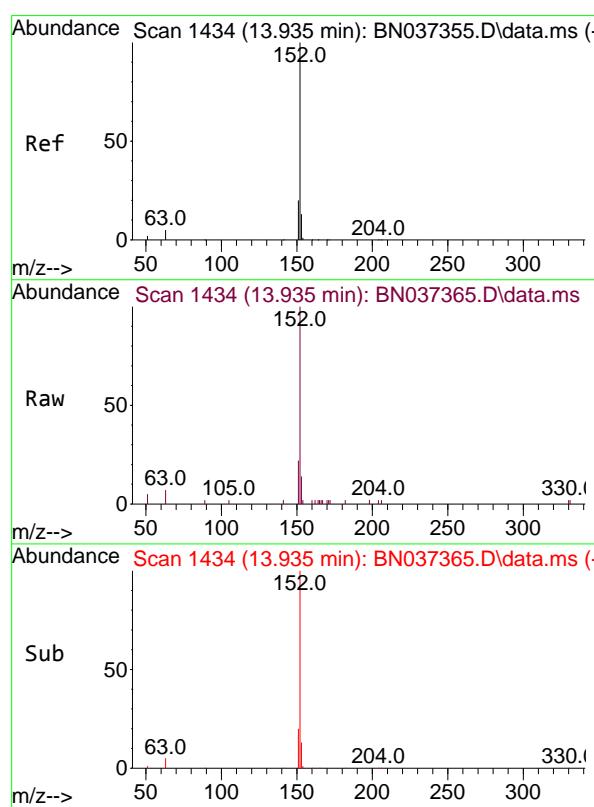


#16  
Acenaphthylene  
Concen: 0.384 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

Tgt Ion:152 Resp: 4498  
Ion Ratio Lower Upper  
152 100  
151 19.8 16.6 24.8  
153 13.1 10.2 15.2


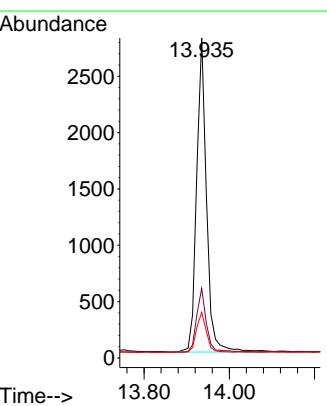





#17  
 Acenaphthene  
 Concen: 0.383 ng  
 RT: 14.277 min Scan# 14  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17  
**Instrument :**  
 BNA\_N  
**ClientSampleId :**  
 SSTDCCC0.4EC





Tgt Ion:154 Resp: 2949  
 Ion Ratio Lower Upper  
 154 100  
 153 118.3 93.1 139.7  
 152 63.2 48.6 73.0

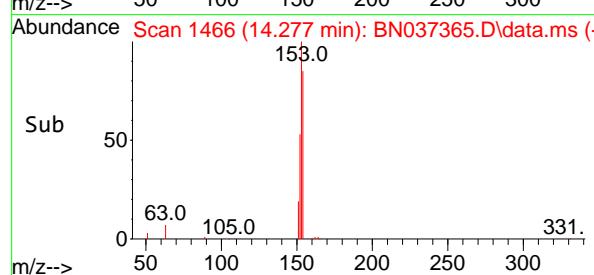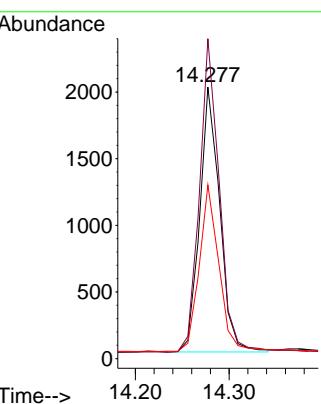


#18  
 Fluorene  
 Concen: 0.385 ng  
 RT: 15.272 min Scan# 1559  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

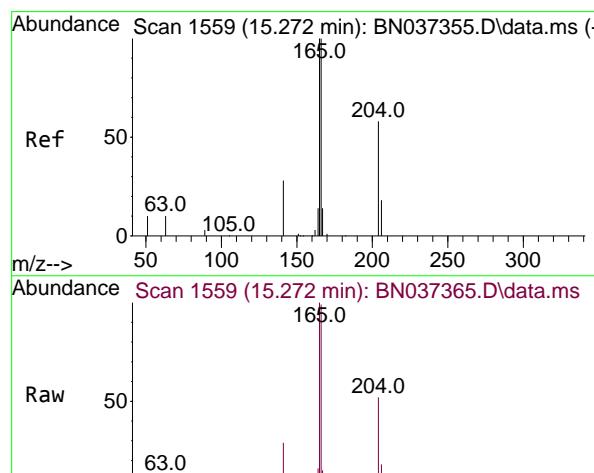

Tgt Ion:166 Resp: 4167  
 Ion Ratio Lower Upper  
 166 100  
 165 100.6 79.5 119.3  
 167 13.8 10.7 16.1

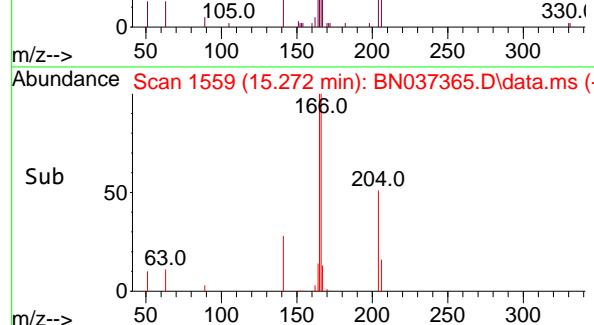
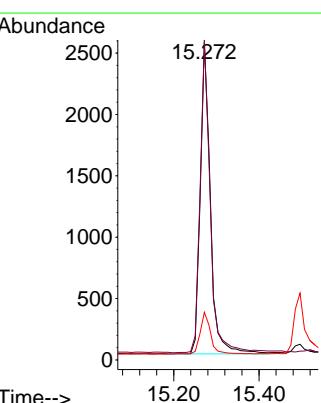


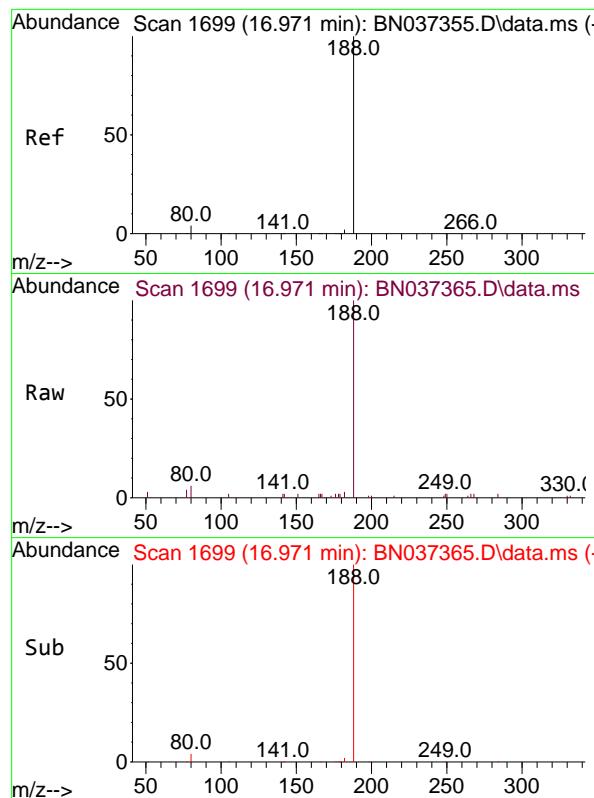

#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. 0.000 min Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:188 Resp: 5748  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 5.6 6.2 9.2#

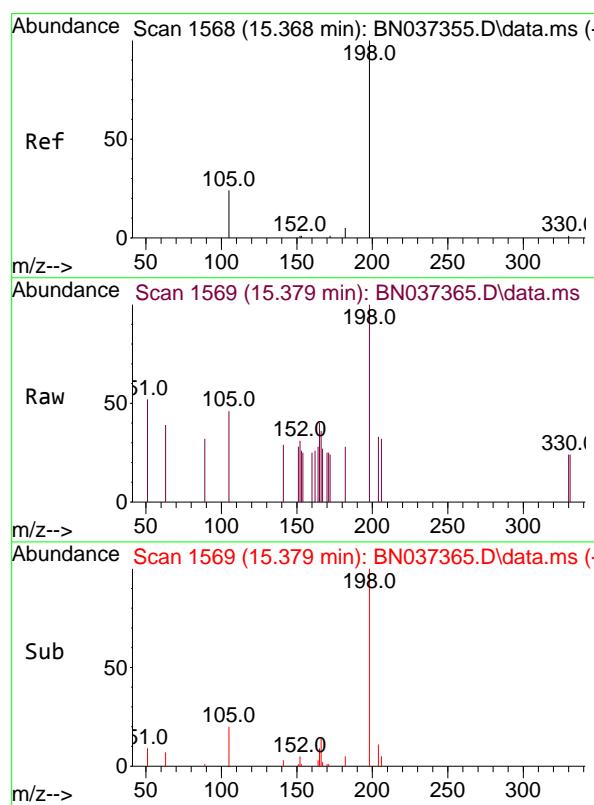

#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.350 ng  
 RT: 15.379 min Scan# 1569  
 Delta R.T. 0.011 min Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Tgt Ion:198 Resp: 483  
 Ion Ratio Lower Upper  
 198 100  
 51 52.1 51.4 77.0  
 105 45.9 45.5 68.3


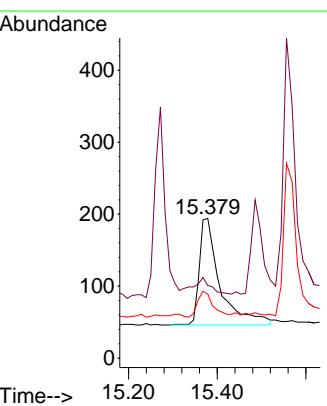


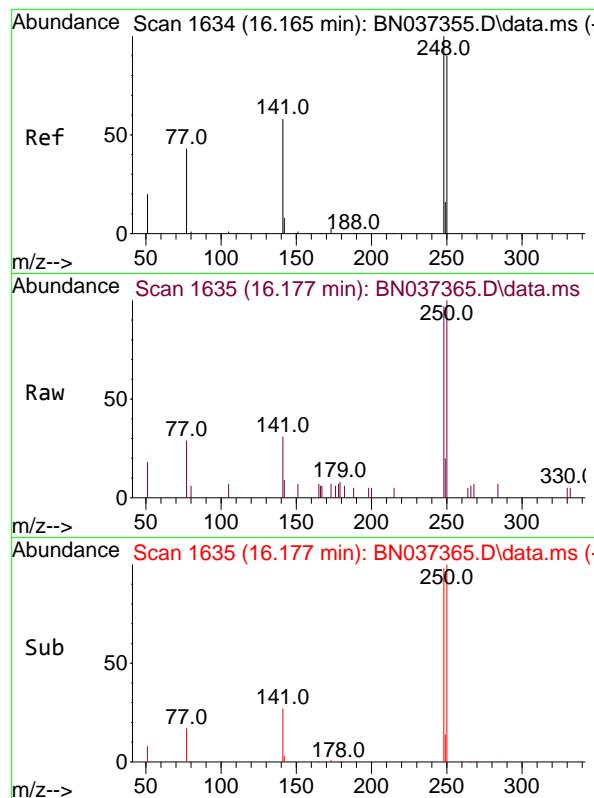

#21  
 4-Bromophenyl-phenylether  
 Concen: 0.396 ng  
 RT: 16.177 min Scan# 1  
 Delta R.T. 0.012 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:248 Resp: 1621  
 Ion Ratio Lower Upper  
 248 100  
 250 103.0 80.4 120.6  
 141 31.9 33.3 49.9#

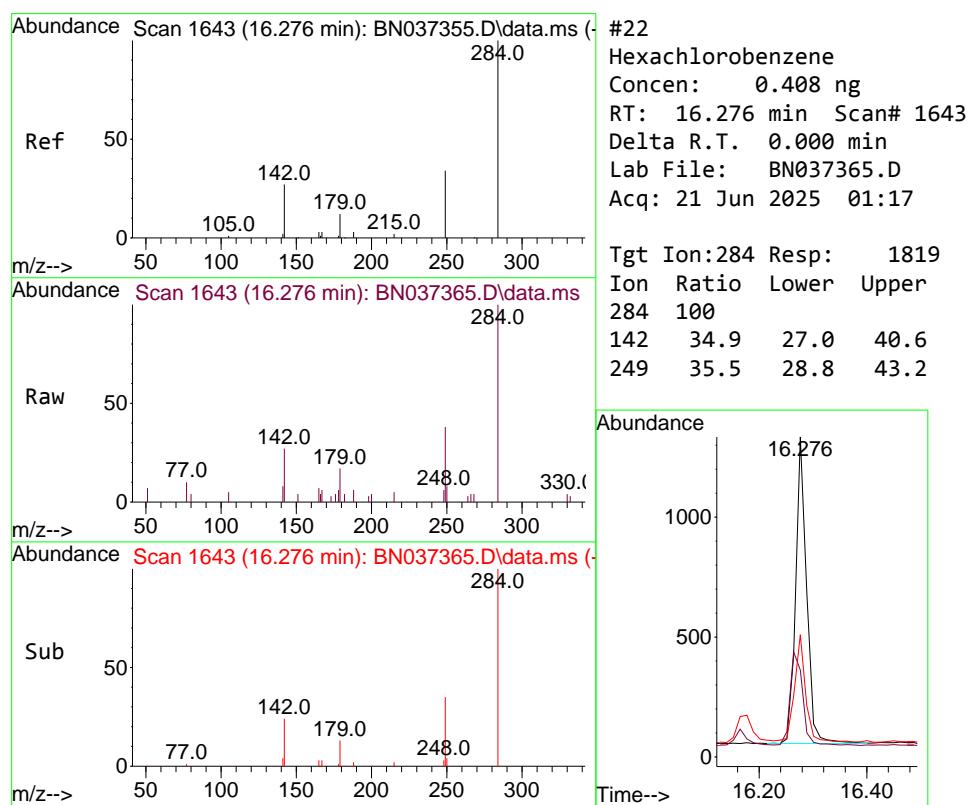

#22  
 Hexachlorobenzene  
 Concen: 0.408 ng  
 RT: 16.276 min Scan# 1643  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Tgt Ion:284 Resp: 1819  
 Ion Ratio Lower Upper  
 284 100  
 142 34.9 27.0 40.6  
 249 35.5 28.8 43.2








#23  
Atrazine  
Concen: 0.364 ng  
RT: 16.450 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
ClientSampleId : SSTDCCC0.4EC





Tgt Ion:200 Resp: 1187  
Ion Ratio Lower Upper  
200 100  
173 25.3 29.2 43.8#  
215 53.8 48.8 73.2



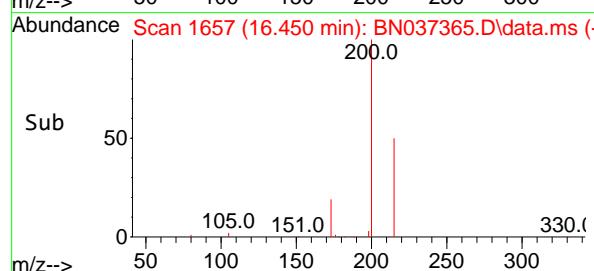


#24  
Pentachlorophenol  
Concen: 0.363 ng  
RT: 16.624 min Scan# 1671  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17



Tgt Ion:266 Resp: 805  
Ion Ratio Lower Upper  
266 100  
264 65.6 50.3 75.5  
268 66.2 55.3 82.9









#25  
 Phenanthrene  
 Concen: 0.377 ng  
 RT: 17.009 min Scan# 1  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDCCC0.4EC


Tgt Ion:178 Resp: 6282  
 Ion Ratio Lower Upper  
 178 100  
 176 19.5 15.2 22.8  
 179 15.5 12.9 19.3

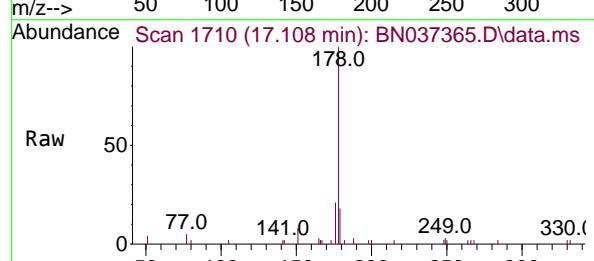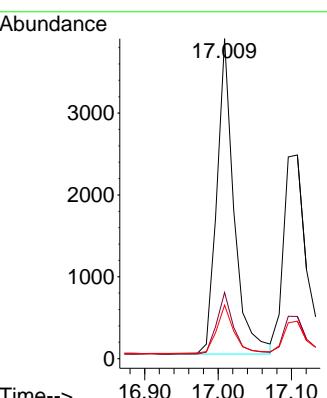

#26  
 Anthracene  
 Concen: 0.360 ng  
 RT: 17.108 min Scan# 1710  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Tgt Ion:178 Resp: 5522  
 Ion Ratio Lower Upper  
 178 100  
 176 19.0 14.7 22.1  
 179 16.2 13.0 19.6





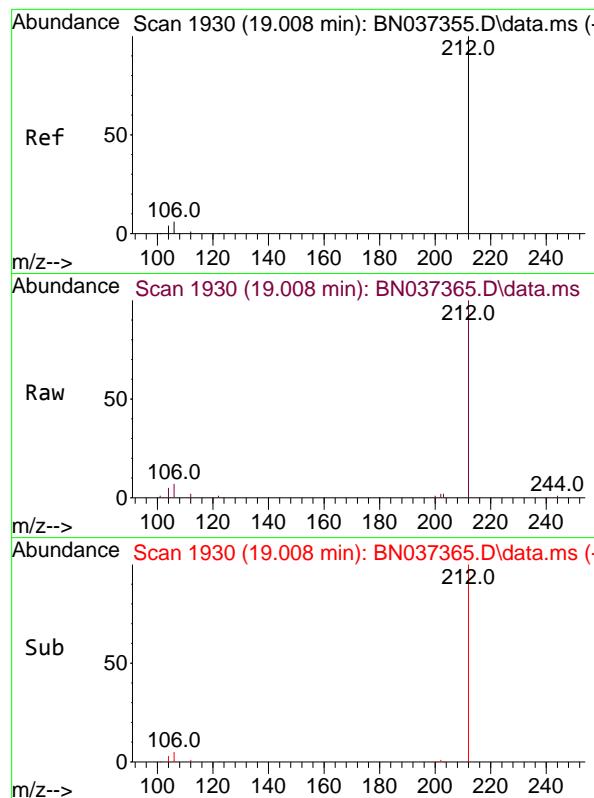

#27  
 Fluoranthene-d10  
 Concen: 0.414 ng  
 RT: 19.008 min Scan# 1930  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:212 Resp: 6836  
 Ion Ratio Lower Upper  
 212 100  
 106 5.5 3.0 4.4#  
 104 3.4 2.0 3.0#

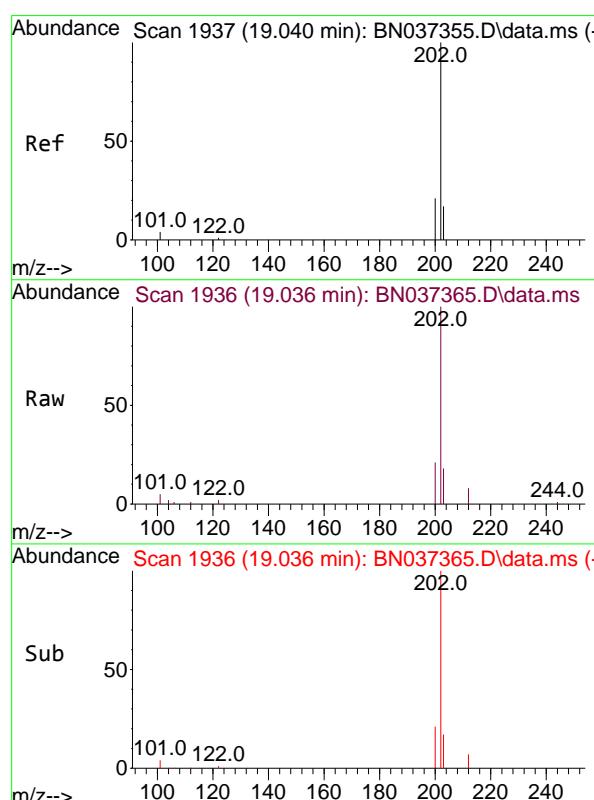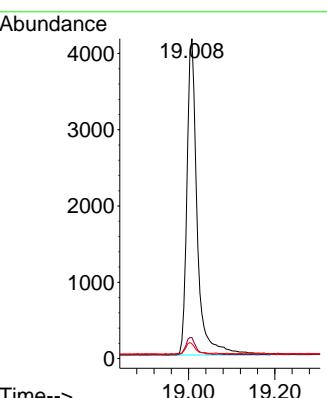

#28  
 Fluoranthene  
 Concen: 0.385 ng  
 RT: 19.036 min Scan# 1936  
 Delta R.T. -0.005 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Tgt Ion:202 Resp: 8102  
 Ion Ratio Lower Upper  
 202 100  
 101 4.5 3.0 4.6  
 203 16.4 13.7 20.5





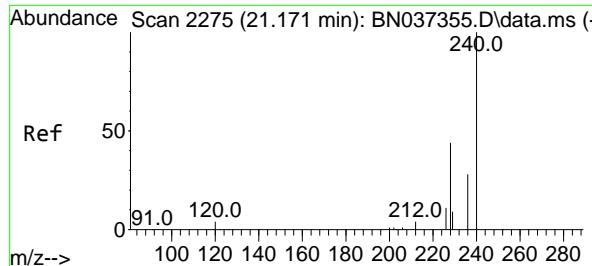


#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.162 min Scan# 21  
Delta R.T. -0.009 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17


**Instrument :** BNA\_N  
**ClientSampleId :** SSTDCCC0.4EC

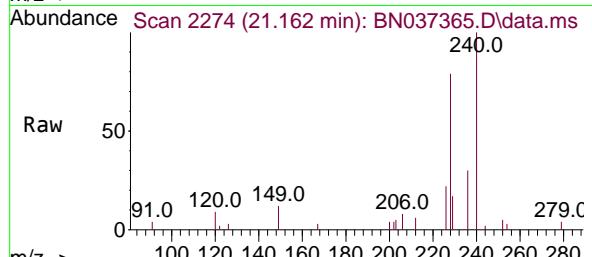



Tgt Ion:240 Resp: 5140  
Ion Ratio Lower Upper  
240 100  
120 9.3 7.5 11.3  
236 30.2 24.9 37.3

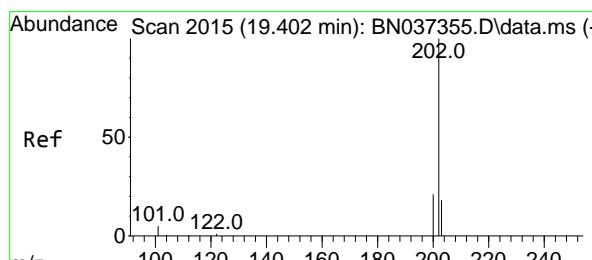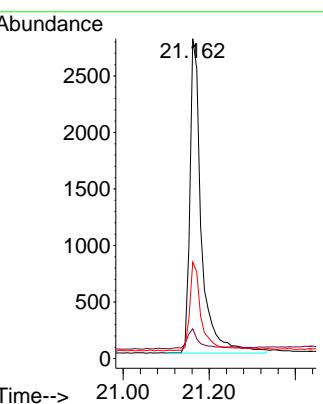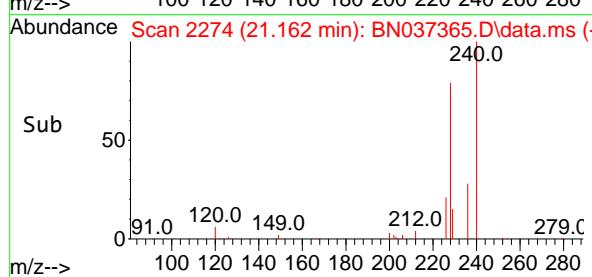


#30  
Pyrene  
Concen: 0.388 ng  
RT: 19.403 min Scan# 2015  
Delta R.T. 0.000 min  
Lab File: BN037365.D  
Acq: 21 Jun 2025 01:17

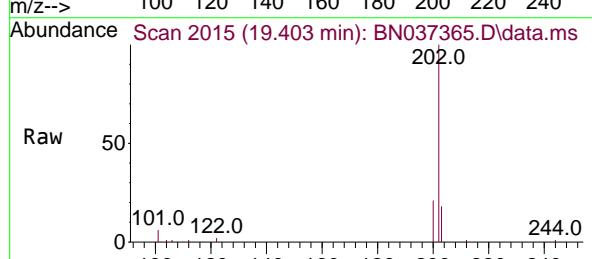

Tgt Ion:202 Resp: 8105  
Ion Ratio Lower Upper  
202 100  
200 21.0 16.8 25.2  
203 17.7 14.5 21.7

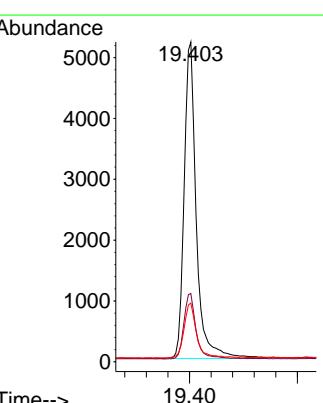
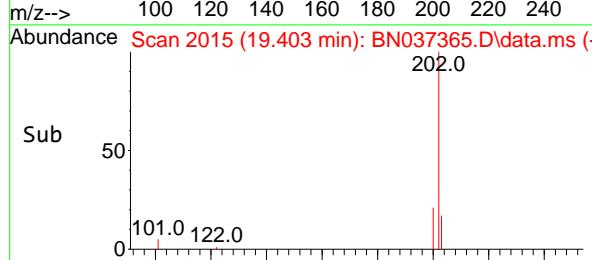


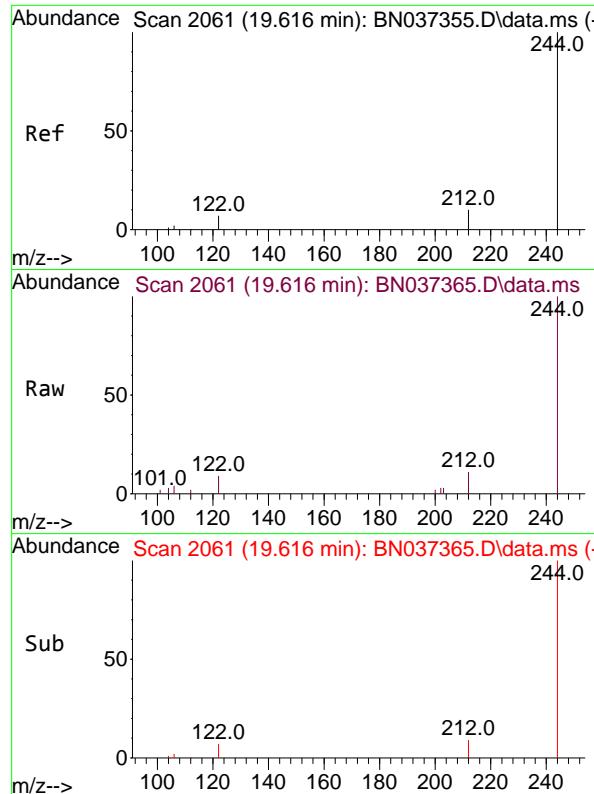

#31  
 Terphenyl-d14  
 Concen: 0.396 ng  
 RT: 19.616 min Scan# 2061  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:244 Resp: 4639  
 Ion Ratio Lower Upper  
 244 100  
 212 11.1 11.1 16.7  
 122 8.6 7.2 10.8

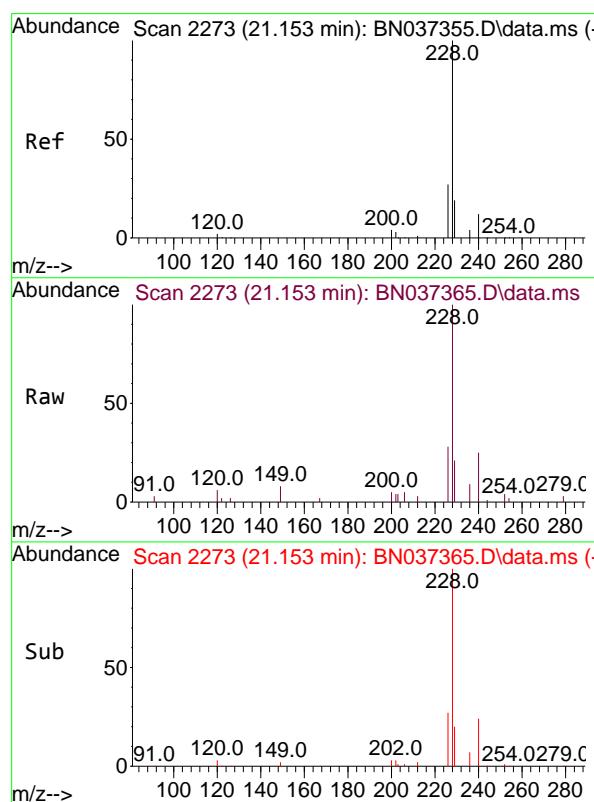

#32  
 Benzo(a)anthracene  
 Concen: 0.376 ng  
 RT: 21.153 min Scan# 2273  
 Delta R.T. 0.000 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Tgt Ion:228 Resp: 6359  
 Ion Ratio Lower Upper  
 228 100  
 226 27.5 23.0 34.4  
 229 20.7 17.4 26.0


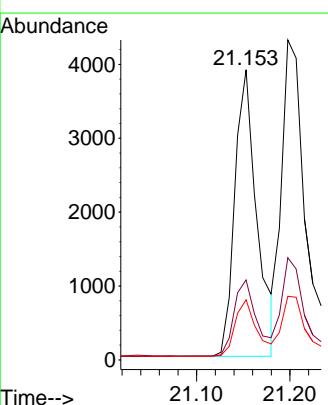


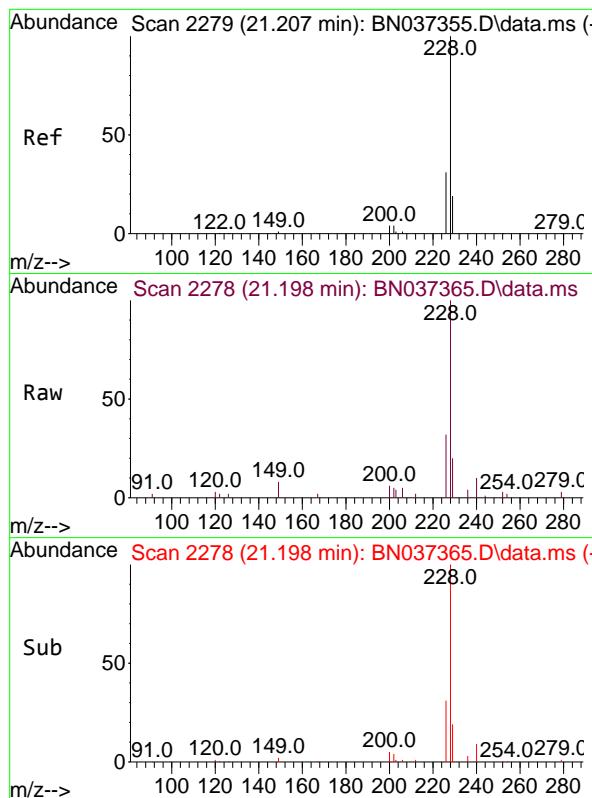

#33  
 Chrysene  
 Concen: 0.391 ng  
 RT: 21.198 min Scan# 21  
 Delta R.T. -0.009 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:228 Resp: 8015  
 Ion Ratio Lower Upper  
 228 100  
 226 31.9 25.4 38.2  
 229 19.9 17.3 25.9

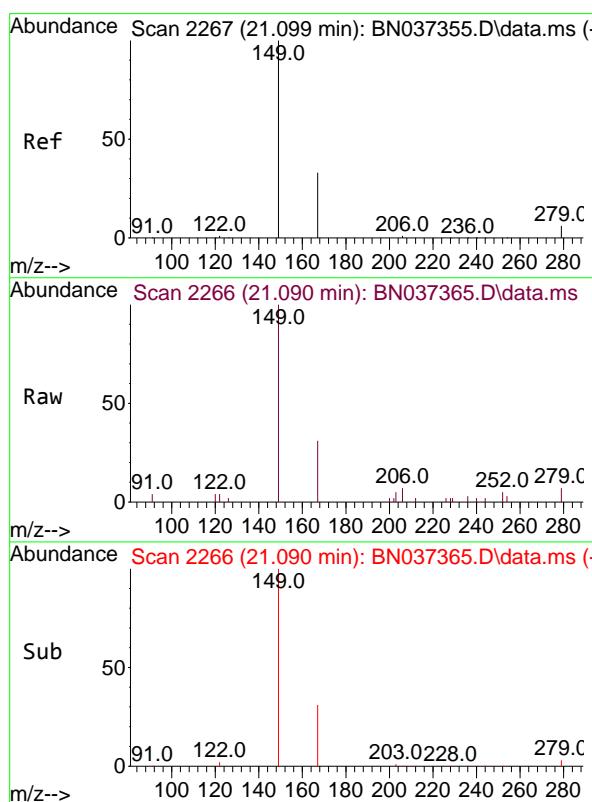

#34  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.385 ng  
 RT: 21.090 min Scan# 2266  
 Delta R.T. -0.009 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Tgt Ion:149 Resp: 2672  
 Ion Ratio Lower Upper  
 149 100  
 167 31.7 24.6 37.0  
 279 6.5 6.5 9.7#


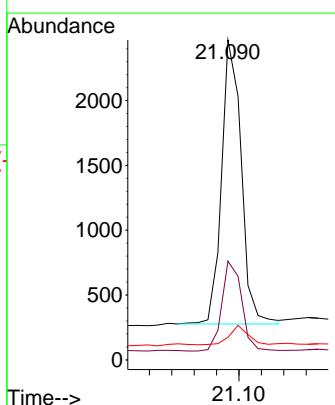


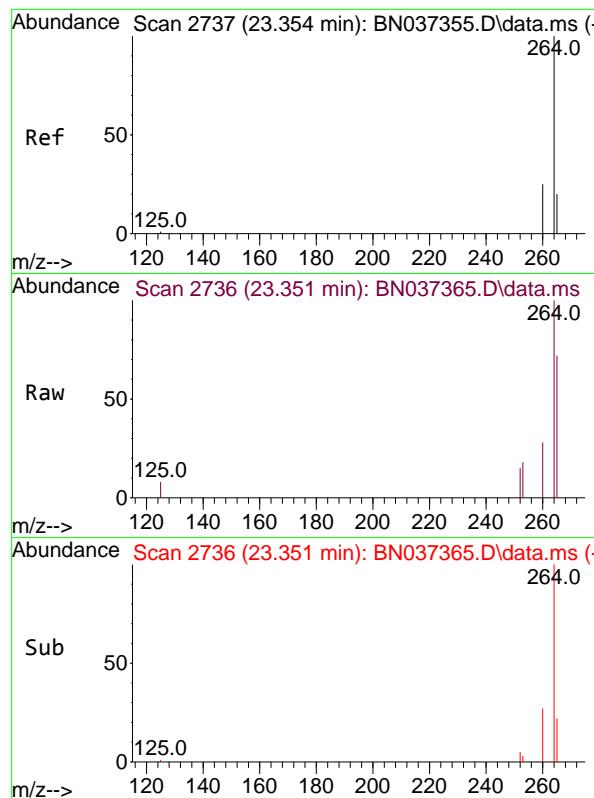

#35  
 Perylene-d12  
 Concen: 0.400 ng  
 RT: 23.351 min Scan# 21  
 Delta R.T. -0.003 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:264 Resp: 5682  
 Ion Ratio Lower Upper  
 264 100  
 260 27.9 21.4 32.2  
 265 72.3 71.4 107.0

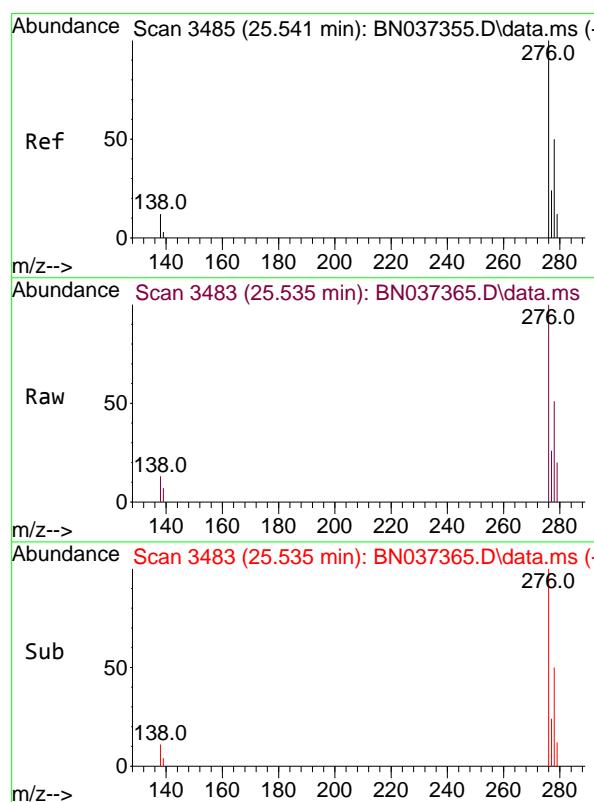

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.382 ng  
 RT: 25.535 min Scan# 3483  
 Delta R.T. -0.006 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Tgt Ion:276 Resp: 9725  
 Ion Ratio Lower Upper  
 276 100  
 138 11.2 2.2 3.2#  
 277 24.1 17.1 25.7





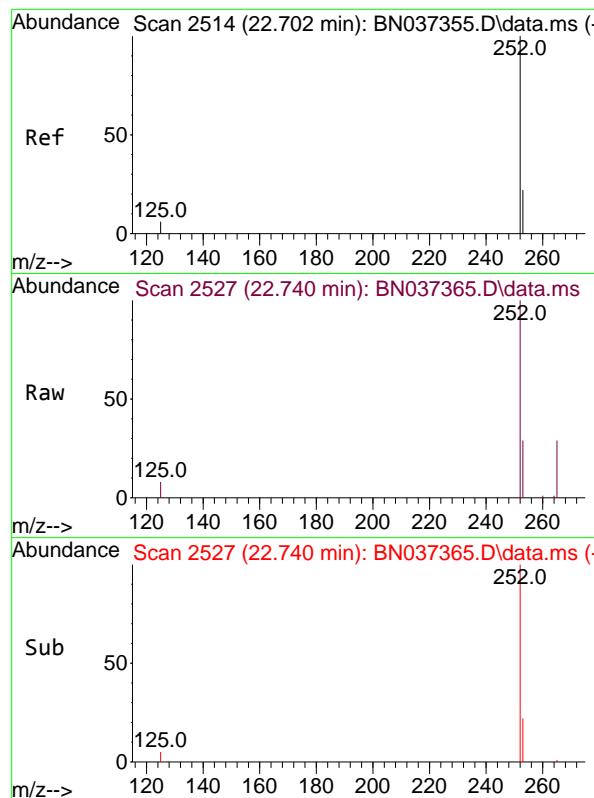

#37  
 Benzo(b)fluoranthene  
 Concen: 0.431 ng  
 RT: 22.740 min Scan# 21  
 Delta R.T. 0.038 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:252 Resp: 9018  
 Ion Ratio Lower Upper  
 252 100  
 253 29.0 26.6 40.0  
 125 8.1 6.1 9.1

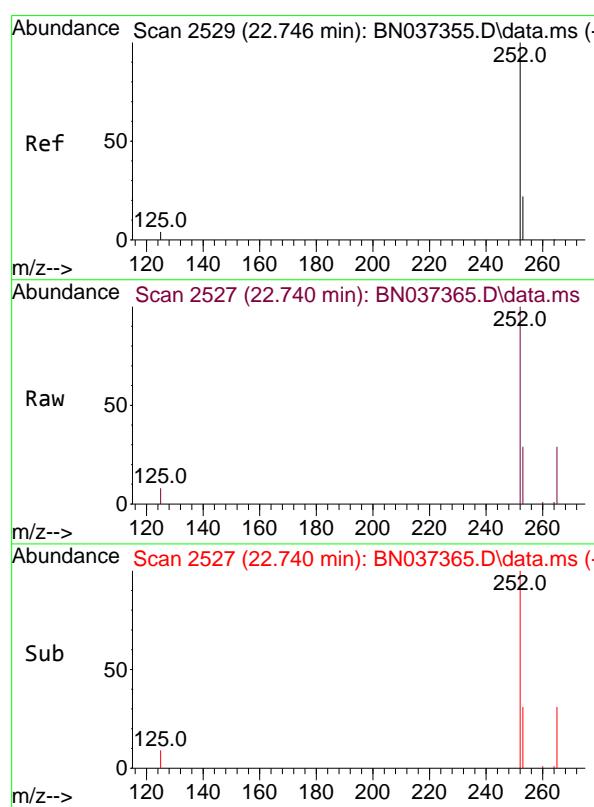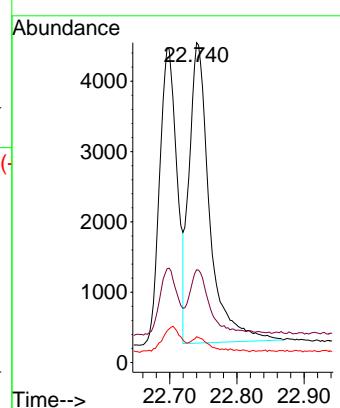

#38  
 Benzo(k)fluoranthene  
 Concen: 0.398 ng  
 RT: 22.740 min Scan# 2527  
 Delta R.T. -0.006 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Tgt Ion:252 Resp: 9018  
 Ion Ratio Lower Upper  
 252 100  
 253 29.0 26.7 40.1  
 125 8.1 6.5 9.7


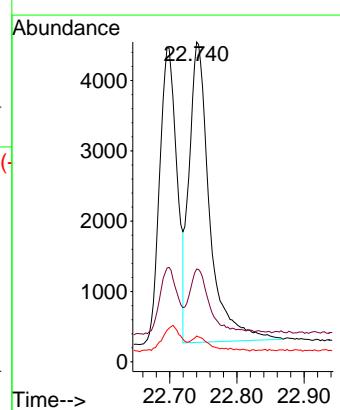


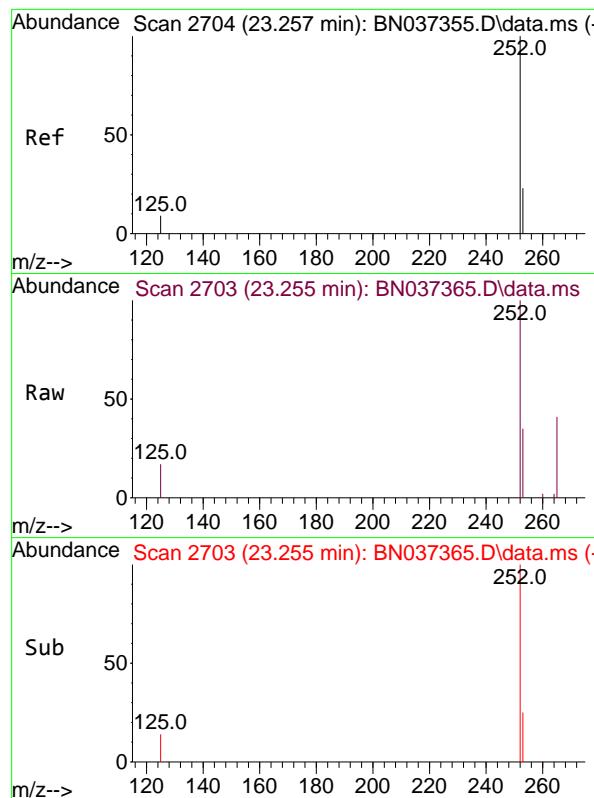

#39  
 Benzo(a)pyrene  
 Concen: 0.380 ng  
 RT: 23.255 min Scan# 21  
 Delta R.T. -0.003 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17


Instrument : BNA\_N  
 ClientSampleId : SSTDCCC0.4EC


Tgt Ion:252 Resp: 7122  
 Ion Ratio Lower Upper  
 252 100  
 253 34.6 31.6 47.4  
 125 17.3 8.4 12.6#

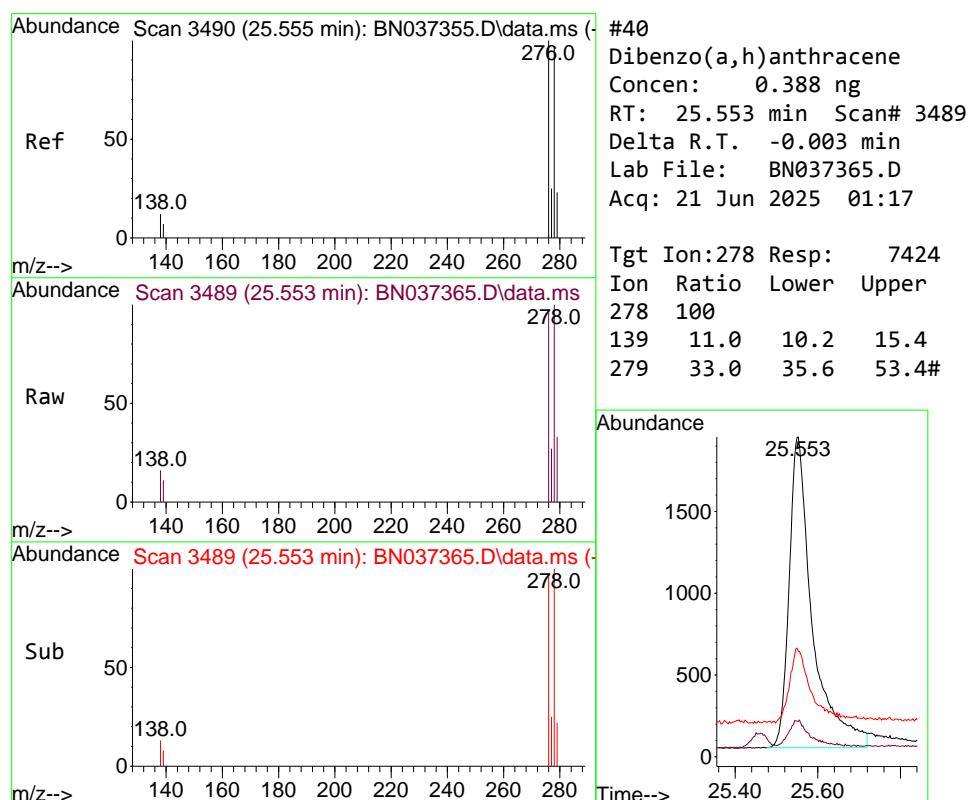

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.388 ng  
 RT: 25.553 min Scan# 3489  
 Delta R.T. -0.003 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Tgt Ion:278 Resp: 7424  
 Ion Ratio Lower Upper  
 278 100  
 139 11.0 10.2 15.4  
 279 33.0 35.6 53.4#

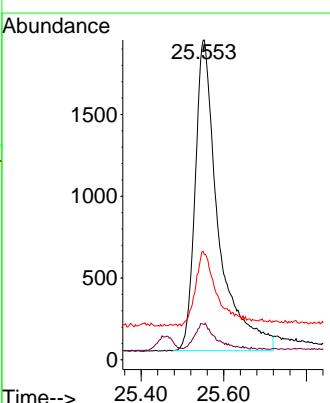


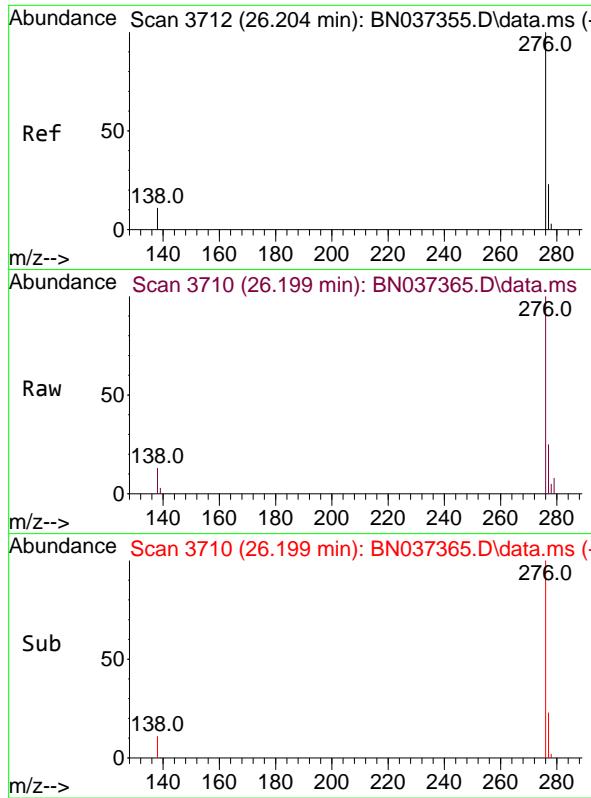

#41  
 Benzo(g,h,i)perylene  
 Concen: 0.389 ng  
 RT: 26.199 min Scan# 3  
 Delta R.T. -0.006 min  
 Lab File: BN037365.D  
 Acq: 21 Jun 2025 01:17

Instrument : BNA\_N  
 ClientSampleId : SSTDCCCC0.4EC

Tgt Ion:276 Resp: 8859  
 Ion Ratio Lower Upper  
 276 100  
 277 25.1 22.7 34.1  
 138 13.1 9.4 14.2

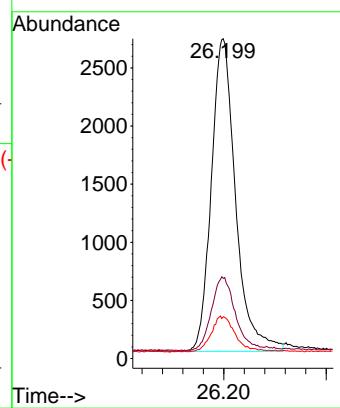

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037386.D  
 Acq On : 26 Jun 2025 10:41  
 Operator : RC/JU  
 Sample : SSTDICCO.1  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

**Instrument :**  
**BNA\_N**  
**ClientSampleId :**  
**SSTDICCO.1**

Quant Time: Jun 26 16:03:56 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:02:41 2025  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
<b>Internal Standards</b>						
1) 1,4-Dichlorobenzene-d4	7.560	152	2183	0.400	ng	0.00
7) Naphthalene-d8	10.340	136	4628	0.400	ng	0.00
13) Acenaphthene-d10	14.213	164	2945	0.400	ng	0.00
19) Phenanthrene-d10	16.971	188	5811	0.400	ng	0.01
29) Chrysene-d12	21.171	240	5498	0.400	ng	0.00
35) Perylene-d12	23.348	264	5798	0.400	ng	0.00
<b>System Monitoring Compounds</b>						
4) 2-Fluorophenol	5.163	112	421	0.100	ng	0.00
5) Phenol-d6	6.744	99	362	0.083	ng	0.00
8) Nitrobenzene-d5	8.621	82	95	0.026	ng	-0.10
11) 2-Methylnaphthalene-d10	11.955	152	615	0.086	ng	0.02
14) 2,4,6-Tribromophenol	15.730	330	143	0.083	ng	0.01
15) 2-Fluorobiphenyl	12.843	172	1140	0.090	ng	0.01
27) Fluoranthene-d10	19.008	212	1559	0.094	ng	0.00
31) Terphenyl-d14	19.625	244	1099	0.094	ng	0.00
<b>Target Compounds</b>						
				<b>Qvalue</b>		
2) 1,4-Dioxane	3.104	88	299	0.144	ng	# 85
3) n-Nitrosodimethylamine	3.429	42	207	0.101	ng	88
6) bis(2-Chloroethyl)ether	7.004	93	313	0.081	ng	# 85
9) Naphthalene	10.394	128	1206	0.101	ng	# 86
10) Hexachlorobutadiene	10.682	225	471	0.100	ng	# 98
12) 2-Methylnaphthalene	12.026	142	735	0.090	ng	96
16) Acenaphthylene	13.935	152	1167	0.096	ng	97
17) Acenaphthene	14.277	154	758	0.095	ng	98
18) Fluorene	15.272	166	1063	0.094	ng	100
20) 4,6-Dinitro-2-methylph...	15.389	198	81	0.054	ng	# 1
21) 4-Bromophenyl-phenylether	16.177	248	383	0.093	ng	# 93
22) Hexachlorobenzene	16.276	284	450	0.102	ng	98
23) Atrazine	16.462	200	291	0.090	ng	# 73
24) Pentachlorophenol	16.636	266	262	0.110	ng	95
25) Phenanthrene	17.009	178	1534	0.094	ng	97
26) Anthracene	17.108	178	1358	0.090	ng	100
28) Fluoranthene	19.040	202	2001	0.096	ng	99
30) Pyrene	19.402	202	2006	0.096	ng	99
32) Benzo(a)anthracene	21.153	228	1579	0.091	ng	92
33) Chrysene	21.198	228	2241	0.105	ng	94
34) Bis(2-ethylhexyl)phtha...	21.090	149	839	0.123	ng	# 98
36) Indeno(1,2,3-cd)pyrene	25.535	276	2156	0.088	ng	# 90
37) Benzo(b)fluoranthene	22.699	252	1927	0.094	ng	# 66
38) Benzo(k)fluoranthene	22.740	252	2041	0.093	ng	# 61
39) Benzo(a)pyrene	23.254	252	1755	0.097	ng	# 52
40) Dibenzo(a,h)anthracene	25.567	278	1522	0.081	ng	# 41
41) Benzo(g,h,i)perylene	26.193	276	2066	0.092	ng	# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062625\  
 Data File : BN037386.D  
 Acq On : 26 Jun 2025 10:41  
 Operator : RC/JU  
 Sample : SSTDICC0.1  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTDICC0.1


Quant Time: Jun 26 16:03:56 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN062625.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jun 26 16:02:41 2025  
 Response via : Initial Calibration

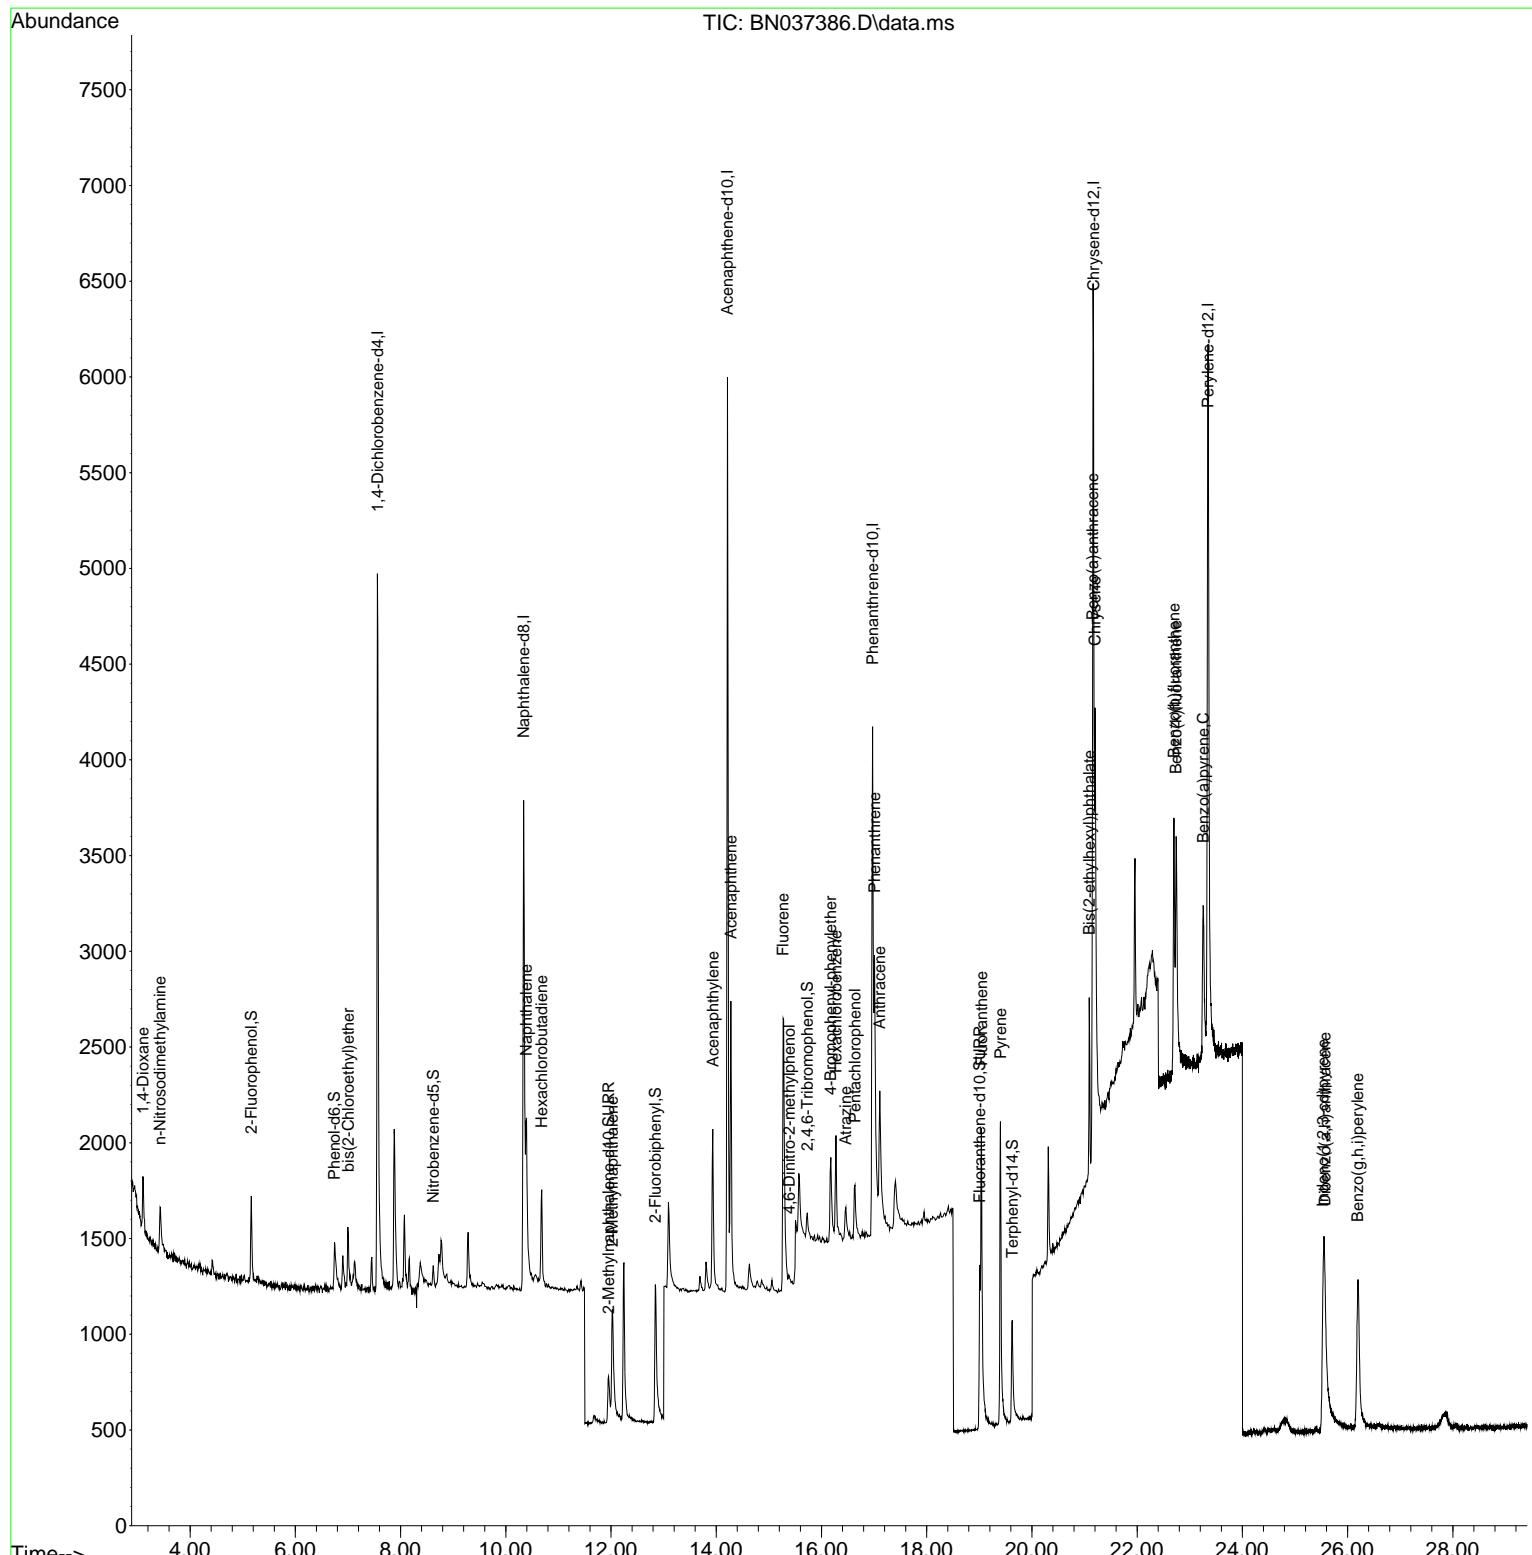



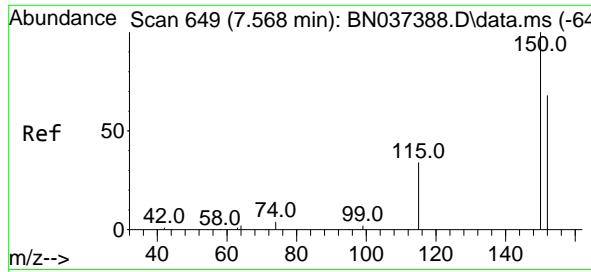


#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.560 min Scan# 6  
Delta R.T. -0.008 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1

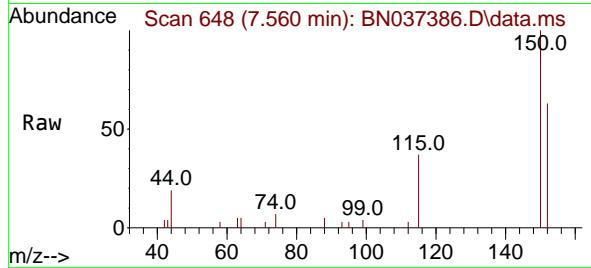



Tgt Ion:152 Resp: 2183  
Ion Ratio Lower Upper  
152 100  
150 157.8 116.2 174.2  
115 58.7 42.9 64.3

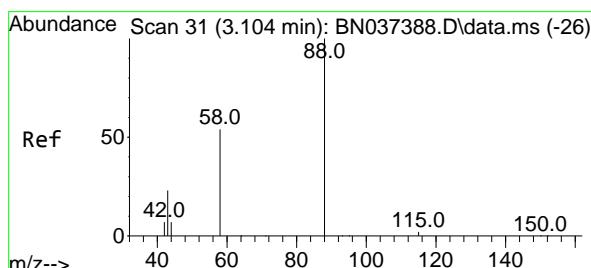

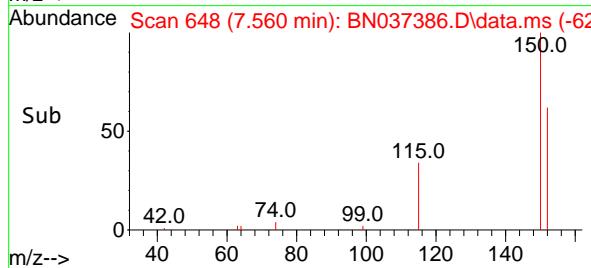


#2  
1,4-Dioxane  
Concen: 0.144 ng  
RT: 3.104 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

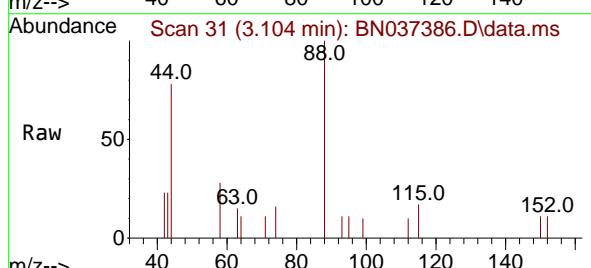





Tgt Ion: 88 Resp: 299  
Ion Ratio Lower Upper  
88 100  
43 23.1 21.6 32.4  
58 44.1 45.9 68.9#

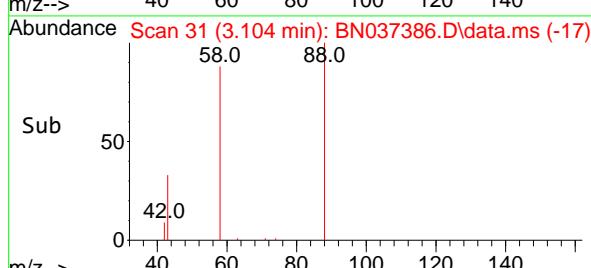

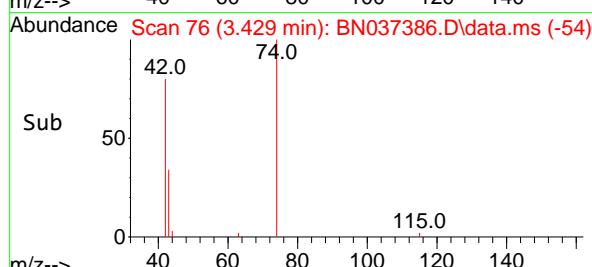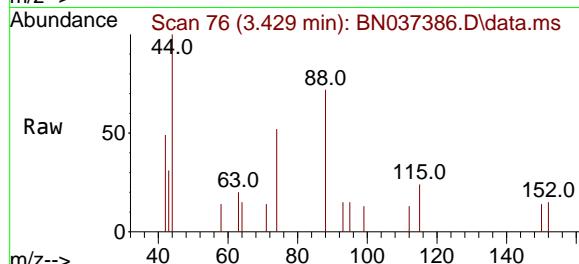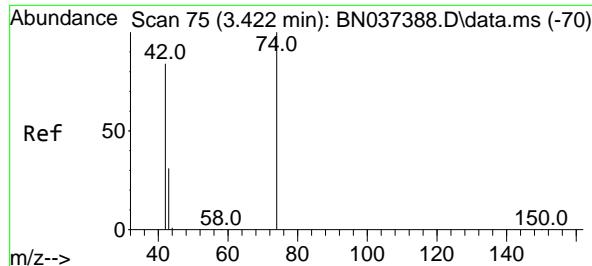


#3  
n-Nitrosodimethylamine  
Concen: 0.101 ng  
RT: 3.429 min Scan# 7  
Instrument : BNA\_N  
Delta R.T. 0.007 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41  
ClientSampleId : SSTDICCO.1


Tgt Ion: 42 Resp: 207  
Ion Ratio Lower Upper  
42 100  
74 136.2 97.8 146.8  
44 11.6 8.7 13.1

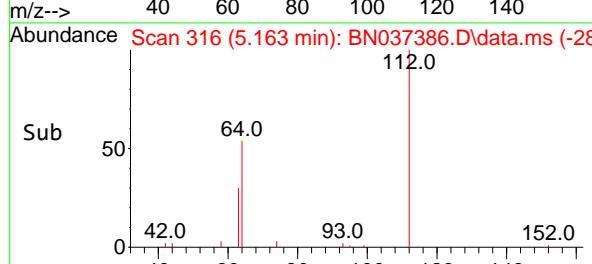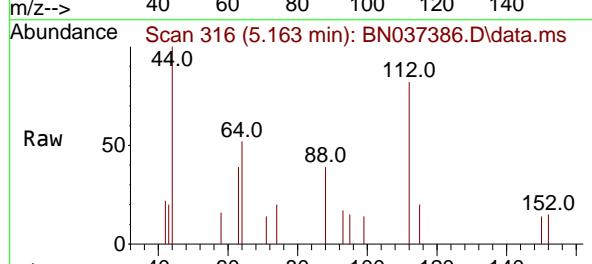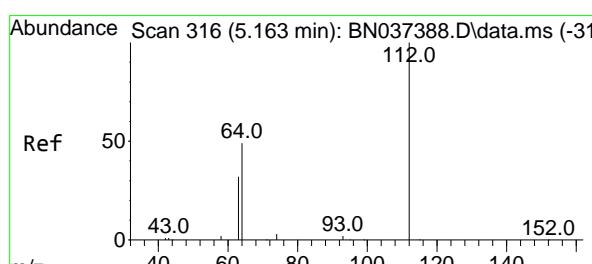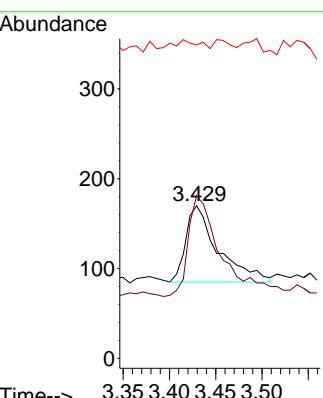

#4  
2-Fluorophenol  
Concen: 0.100 ng  
RT: 5.163 min Scan# 316  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41


Tgt Ion: 112 Resp: 421  
Ion Ratio Lower Upper  
112 100  
64 50.6 40.3 60.5  
63 34.0 26.1 39.1

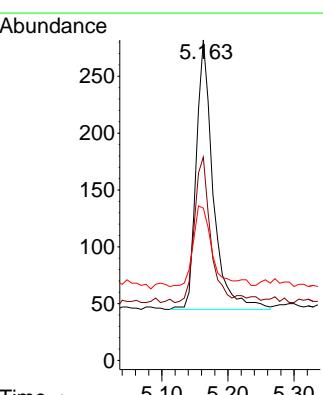



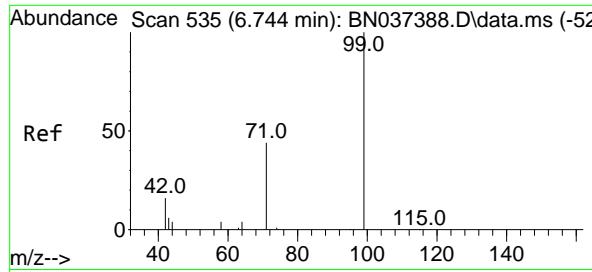


#5  
 Phenol-d6  
 Concen: 0.083 ng  
 RT: 6.744 min Scan# 5  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1

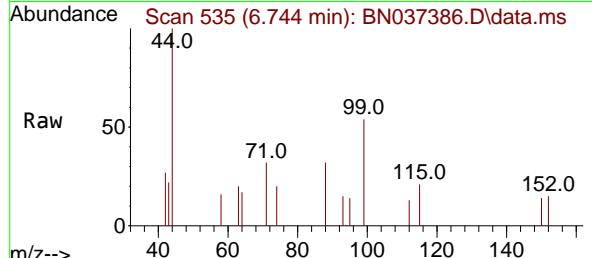



Tgt Ion: 99 Resp: 362  
 Ion Ratio Lower Upper  
 99 100  
 42 19.6 15.6 23.4  
 71 43.6 35.8 53.8

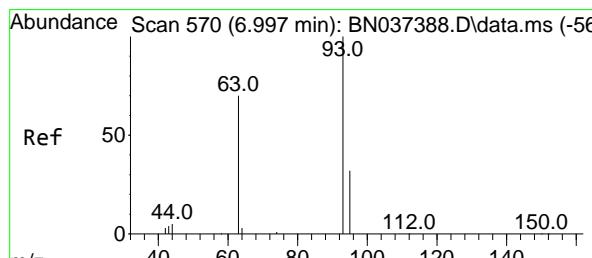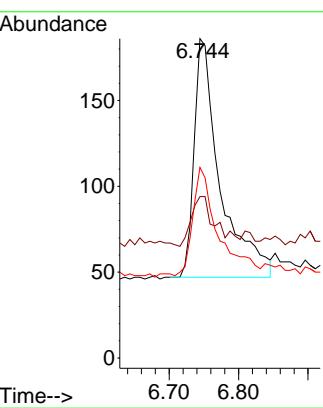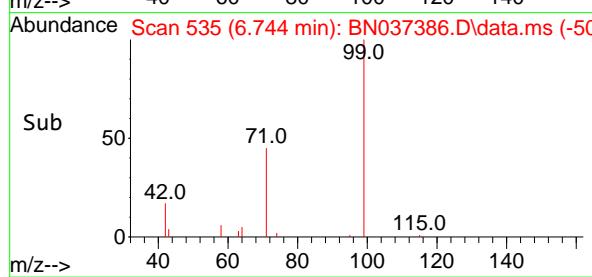


#6  
 bis(2-Chloroethyl)ether  
 Concen: 0.081 ng  
 RT: 7.004 min Scan# 571  
 Delta R.T. 0.007 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

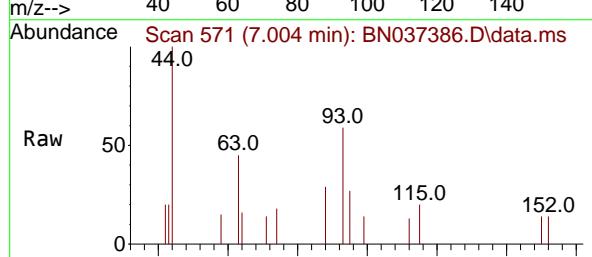


Tgt Ion: 93 Resp: 313  
 Ion Ratio Lower Upper  
 93 100  
 63 75.1 49.6 74.4#  
 95 35.5 23.9 35.9

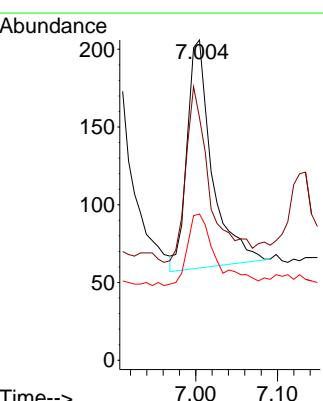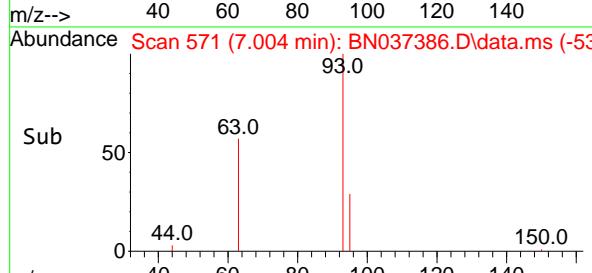





#7  
 Naphthalene-d8  
 Concen: 0.400 ng  
 RT: 10.340 min Scan# 9  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1

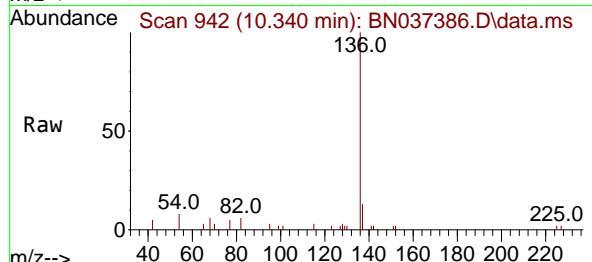



Tgt Ion:136 Resp: 4628


	Ion Ratio	Lower	Upper
136	100		
137	12.8	10.4	15.6
54	8.0	5.6	8.4
68	6.4	4.6	6.8

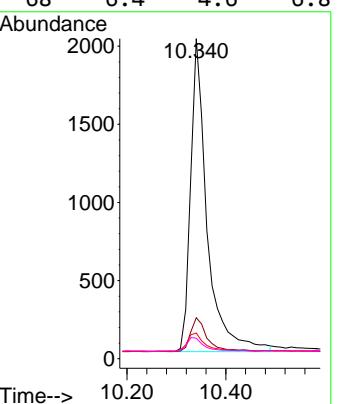


#8  
 Nitrobenzene-d5  
 Concen: 0.026 ng  
 RT: 8.621 min Scan# 781  
 Delta R.T. -0.096 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Tgt Ion: 82 Resp: 95  
 Ion Ratio Lower Upper  
 82 100  
 128 46.9 34.0 51.0  
 54 44.2 37.7 56.5


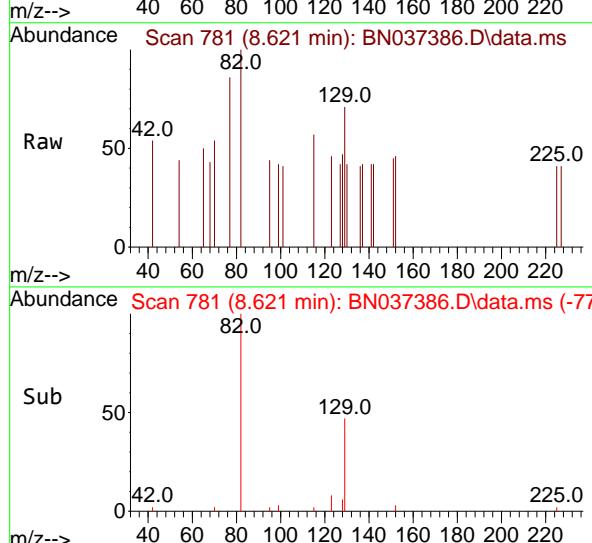
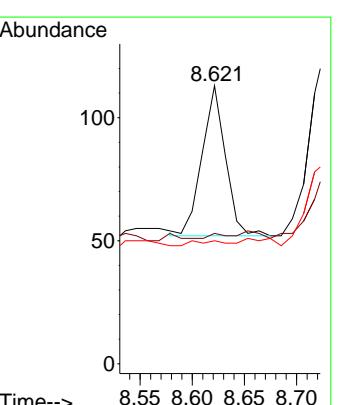


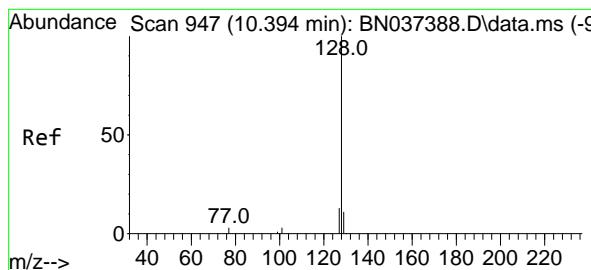


#9  
Naphthalene  
Concen: 0.101 ng  
RT: 10.394 min Scan# 9  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
ClientSampleId : SSTDICCO.1  
Acq: 26 Jun 2025 10:41

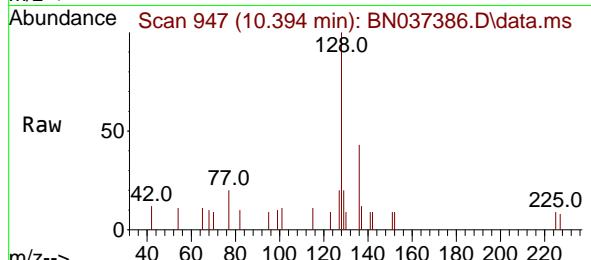



Tgt Ion:128 Resp: 1206  
Ion Ratio Lower Upper  
128 100  
129 19.9 10.4 15.6#  
127 20.3 12.2 18.4#

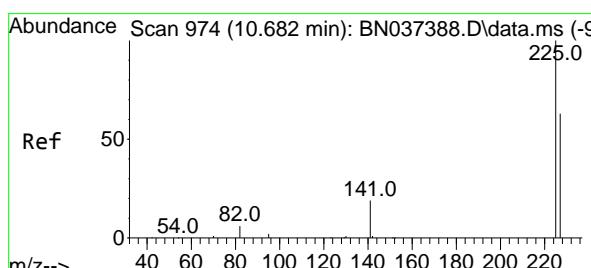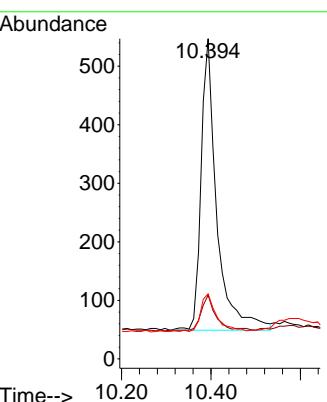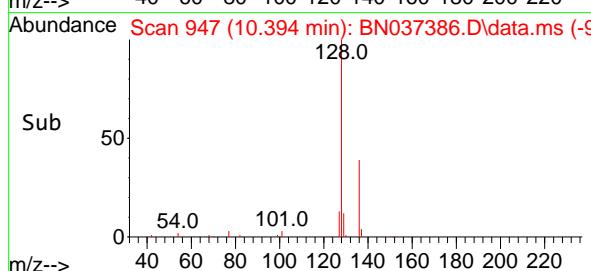


#10  
Hexachlorobutadiene  
Concen: 0.100 ng  
RT: 10.682 min Scan# 974  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

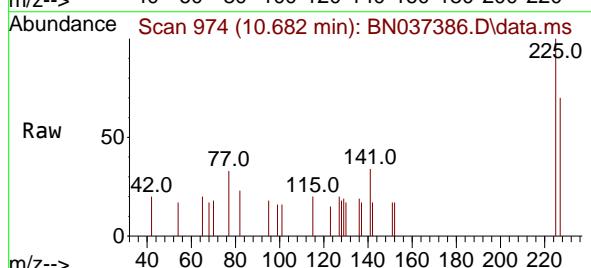


Tgt Ion:225 Resp: 471  
Ion Ratio Lower Upper  
225 100  
223 0.0 0.0 0.0  
227 60.7 49.9 74.9



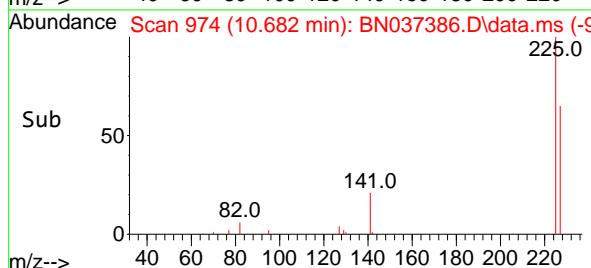





#11  
2-Methylnaphthalene-d10  
Concen: 0.086 ng  
RT: 11.955 min Scan# 1:Instrument :  
Delta R.T. 0.015 min BNA\_N  
Lab File: BN037386.D ClientSampleId :  
Acq: 26 Jun 2025 10:41 SSTDICCO.1





Tgt Ion:152 Resp: 615  
Ion Ratio Lower Upper  
152 100  
151 22.9 18.4 27.6

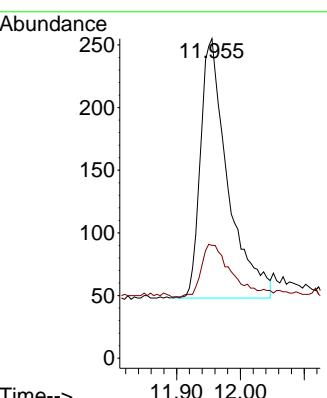


#12  
2-Methylnaphthalene  
Concen: 0.090 ng  
RT: 12.026 min Scan# 1154  
Delta R.T. 0.010 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41




Tgt Ion:142 Resp: 735  
Ion Ratio Lower Upper  
142 100  
141 85.4 70.1 105.1  
115 49.2 35.8 53.6


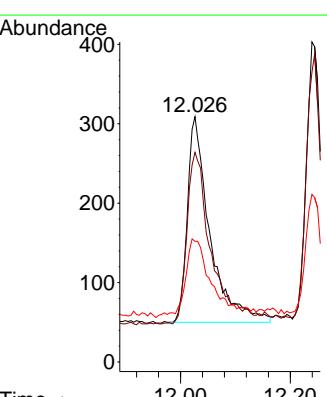
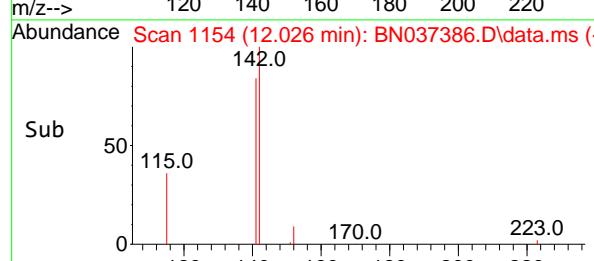





#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.213 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
ClientSampleId : SSTDICCO.1  
Acq: 26 Jun 2025 10:41





Tgt Ion:164 Resp: 2945  
Ion Ratio Lower Upper  
164 100  
162 105.7 82.6 123.8  
160 57.5 42.2 63.2

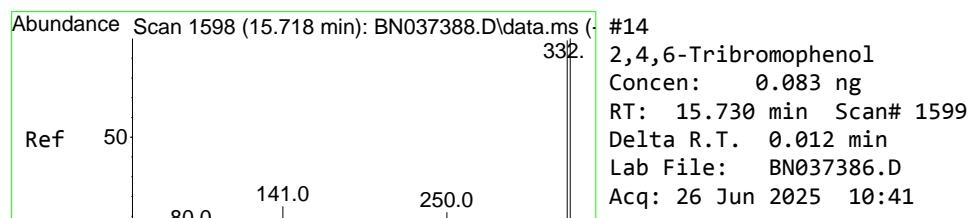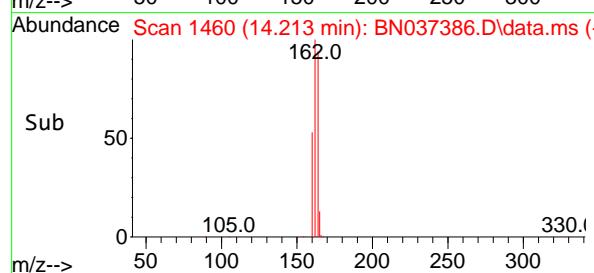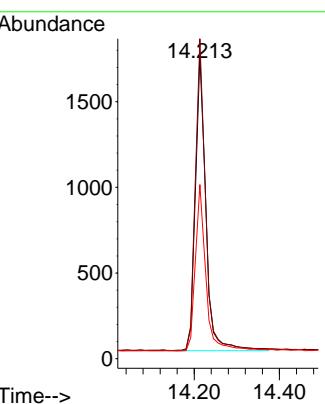


#14  
2,4,6-Tribromophenol  
Concen: 0.083 ng  
RT: 15.730 min Scan# 1599  
Delta R.T. 0.012 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

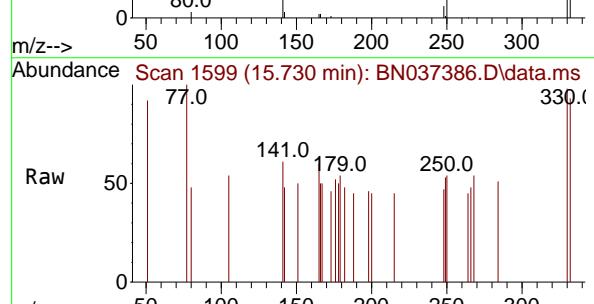


Tgt Ion:330 Resp: 143  
Ion Ratio Lower Upper  
330 100  
332 107.7 77.8 116.8  
141 33.6 24.0 36.0



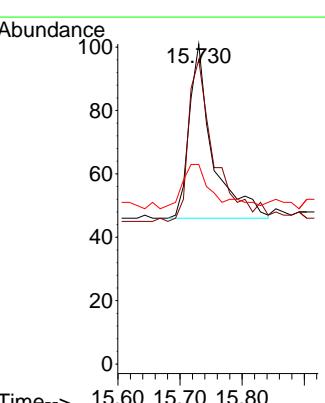





#15  
2-Fluorobiphenyl  
Concen: 0.090 ng  
RT: 12.843 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.010 min  
Lab File: BN037386.D ClientSampleId : SSTDICCO.1  
Acq: 26 Jun 2025 10:41





Tgt Ion:172 Resp: 1140  
Ion Ratio Lower Upper  
172 100  
171 40.4 28.8 43.2  
170 30.3 20.3 30.5

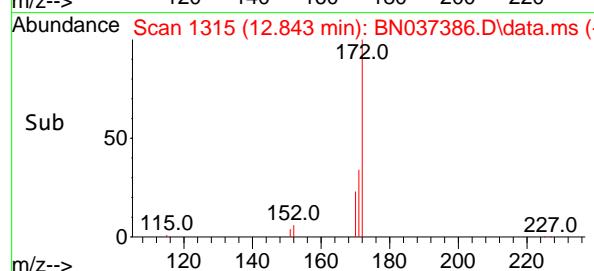


#16  
Acenaphthylene  
Concen: 0.096 ng  
RT: 13.935 min Scan# 1434  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41




Tgt Ion:152 Resp: 1167  
Ion Ratio Lower Upper  
152 100  
151 21.9 15.8 23.6  
153 13.1 10.3 15.5








#17  
 Acenaphthene  
 Concen: 0.095 ng  
 RT: 14.277 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1





Tgt Ion:154 Resp: 758  
 Ion Ratio Lower Upper  
 154 100  
 153 119.4 94.6 141.8  
 152 66.6 50.2 75.2

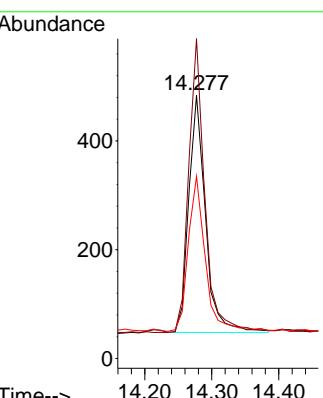


#18  
 Fluorene  
 Concen: 0.094 ng  
 RT: 15.272 min Scan# 1559  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41




Tgt Ion:166 Resp: 1063  
 Ion Ratio Lower Upper  
 166 100  
 165 99.1 79.4 119.2  
 167 12.2 10.6 15.8

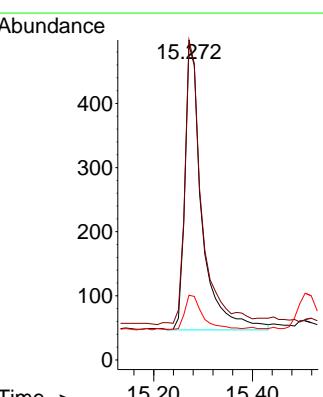






#19  
 Phenanthrene-d10  
 Concen: 0.400 ng  
 RT: 16.971 min Scan# 1  
 Delta R.T. 0.012 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1





Tgt Ion:188 Resp: 5811  
 Ion Ratio Lower Upper  
 188 100  
 94 0.0 0.0 0.0  
 80 7.1 6.2 9.4

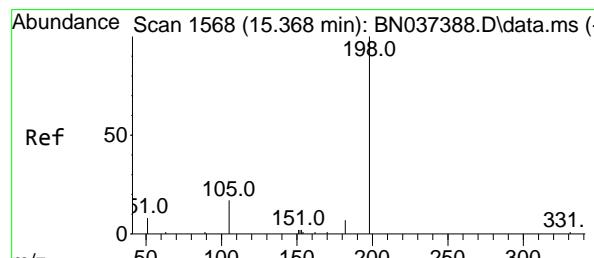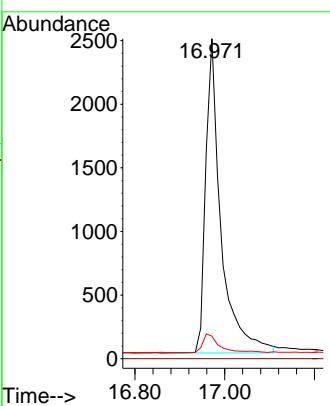


#20  
 4,6-Dinitro-2-methylphenol  
 Concen: 0.054 ng  
 RT: 15.389 min Scan# 1570  
 Delta R.T. 0.021 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41





Tgt Ion:198 Resp: 81  
 Ion Ratio Lower Upper  
 198 100  
 51 149.2 38.8 58.2#  
 105 90.8 29.8 44.6#

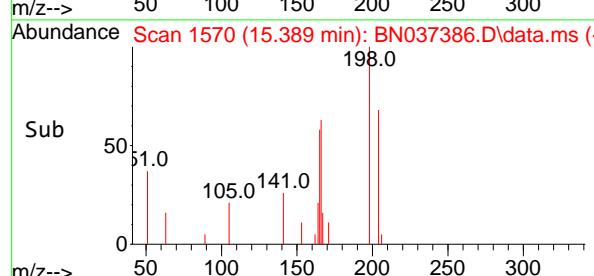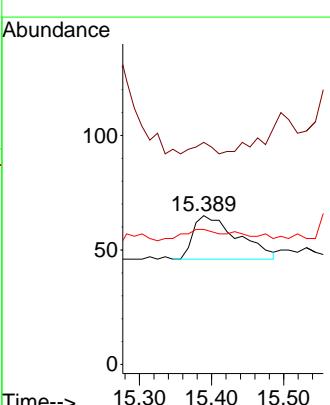

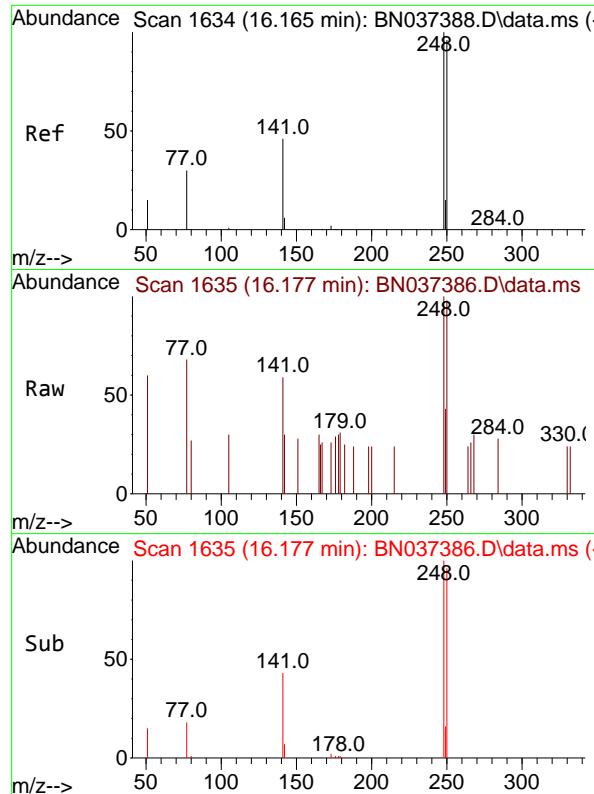


#21  
4-Bromophenyl-phenylether  
Concen: 0.093 ng  
RT: 16.177 min Scan# 1  
Instrument : BNA\_N  
Delta R.T. 0.012 min  
Lab File: BN037386.D ClientSampleId : SSTDICCO.1  
Acq: 26 Jun 2025 10:41


Tgt Ion:248 Resp: 383  
Ion Ratio Lower Upper  
248 100  
250 98.4 77.0 115.4  
141 58.7 38.7 58.1#

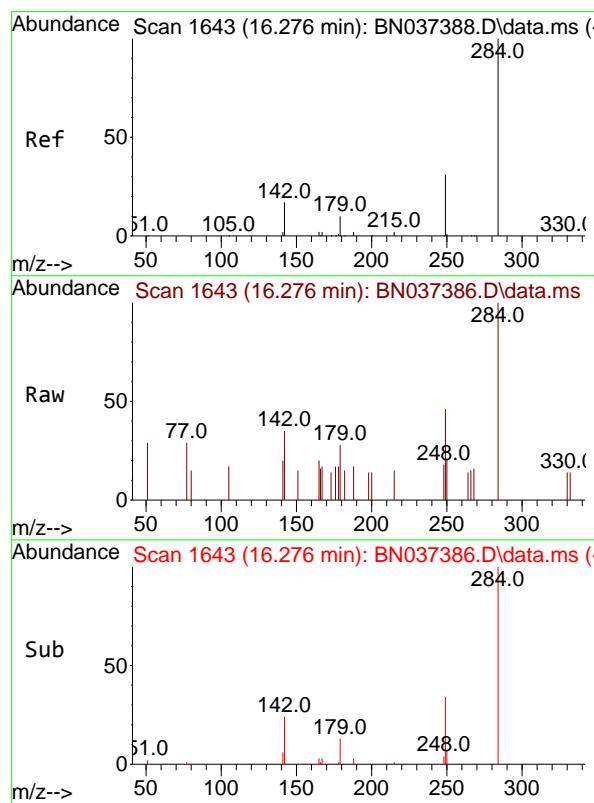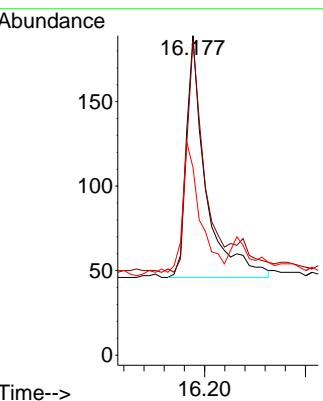

#22  
Hexachlorobenzene  
Concen: 0.102 ng  
RT: 16.276 min Scan# 1643  
Delta R.T. -0.000 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41


Tgt Ion:284 Resp: 450  
Ion Ratio Lower Upper  
284 100  
142 34.4 27.2 40.8  
249 35.1 26.7 40.1

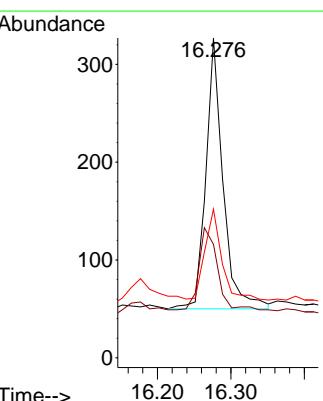






#23  
Atrazine  
Concen: 0.090 ng  
RT: 16.462 min Scan# 1  
Delta R.T. 0.012 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
ClientSampleId : SSTDICCO.1





Tgt Ion:200 Resp: 291  
Ion Ratio Lower Upper  
200 100  
173 47.0 19.0 28.6#  
215 64.2 41.3 61.9#

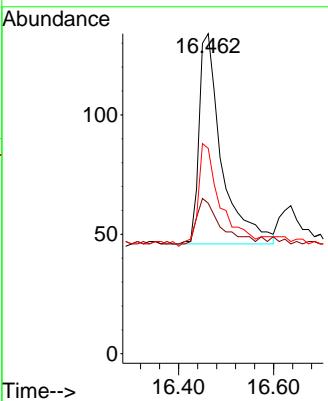


#24  
Pentachlorophenol  
Concen: 0.110 ng  
RT: 16.636 min Scan# 1672  
Delta R.T. 0.012 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41




Tgt Ion:266 Resp: 262  
Ion Ratio Lower Upper  
266 100  
264 61.5 49.2 73.8  
268 75.2 54.2 81.4

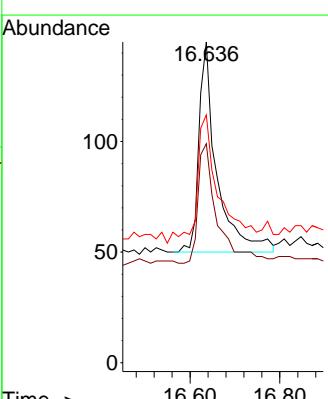






#25  
 Phenanthrene  
 Concen: 0.094 ng  
 RT: 17.009 min Scan# 1  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1





Tgt Ion:178 Resp: 1534  
 Ion Ratio Lower Upper  
 178 100  
 176 20.5 15.6 23.4  
 179 17.4 12.8 19.2

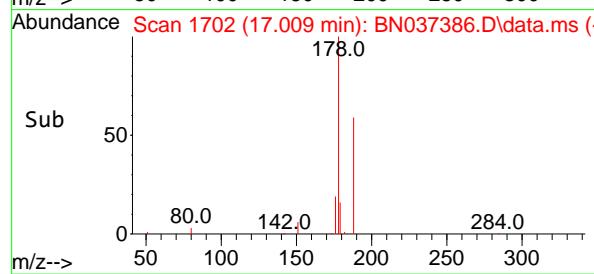


#26  
 Anthracene  
 Concen: 0.090 ng  
 RT: 17.108 min Scan# 1710  
 Delta R.T. 0.012 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41



Tgt Ion:178 Resp: 1358  
 Ion Ratio Lower Upper  
 178 100  
 176 18.6 14.9 22.3  
 179 15.2 12.4 18.6


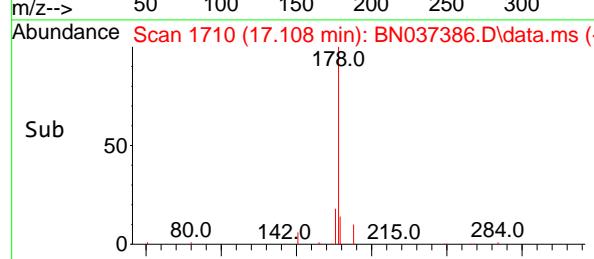


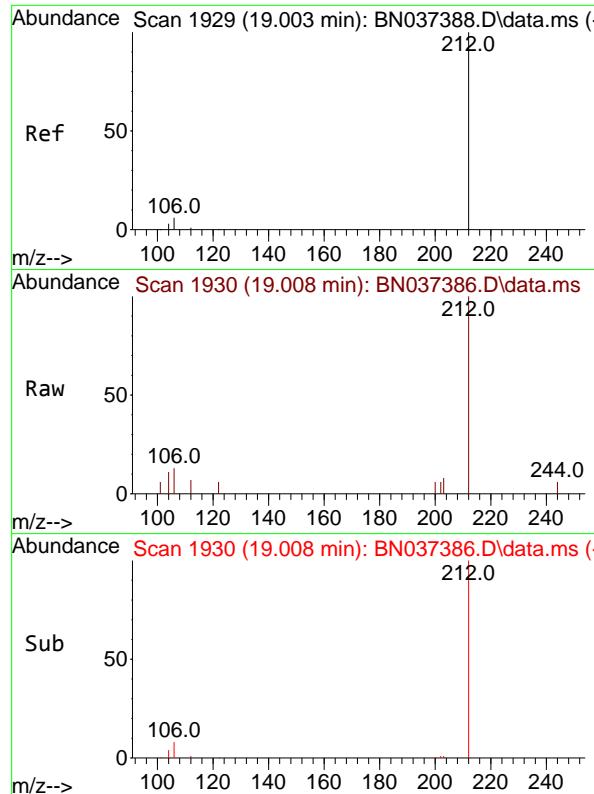

#27  
 Fluoranthene-d10  
 Concen: 0.094 ng  
 RT: 19.008 min Scan# 1  
 Delta R.T. 0.005 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:212 Resp: 1559  
 Ion Ratio Lower Upper  
 212 100  
 106 6.3 4.5 6.7  
 104 4.4 2.7 4.1#

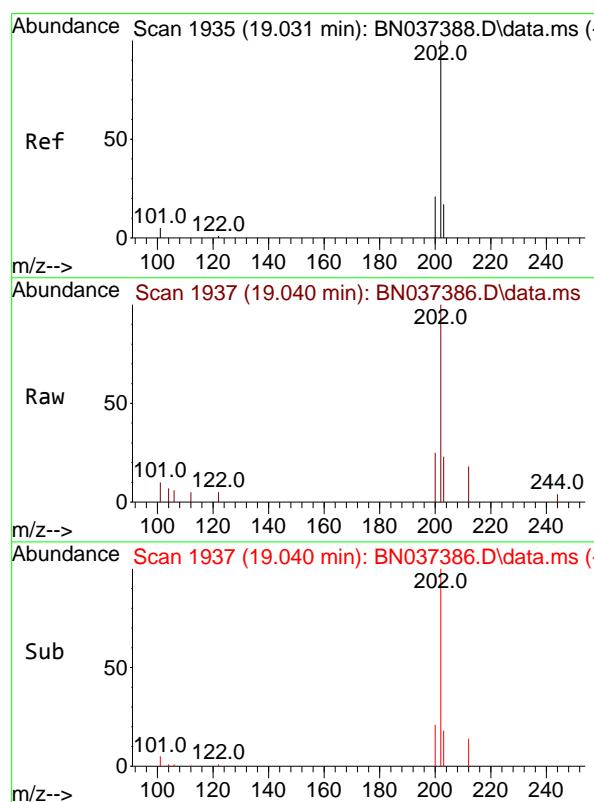

#28  
 Fluoranthene  
 Concen: 0.096 ng  
 RT: 19.040 min Scan# 1937  
 Delta R.T. 0.009 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41



Tgt Ion:202 Resp: 2001  
 Ion Ratio Lower Upper  
 202 100  
 101 5.3 3.8 5.6  
 203 17.4 13.5 20.3

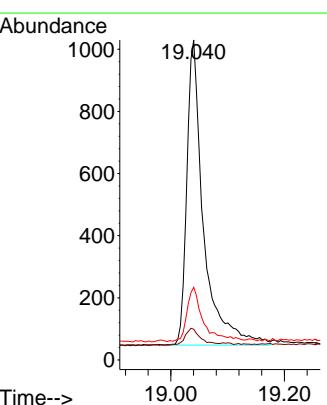

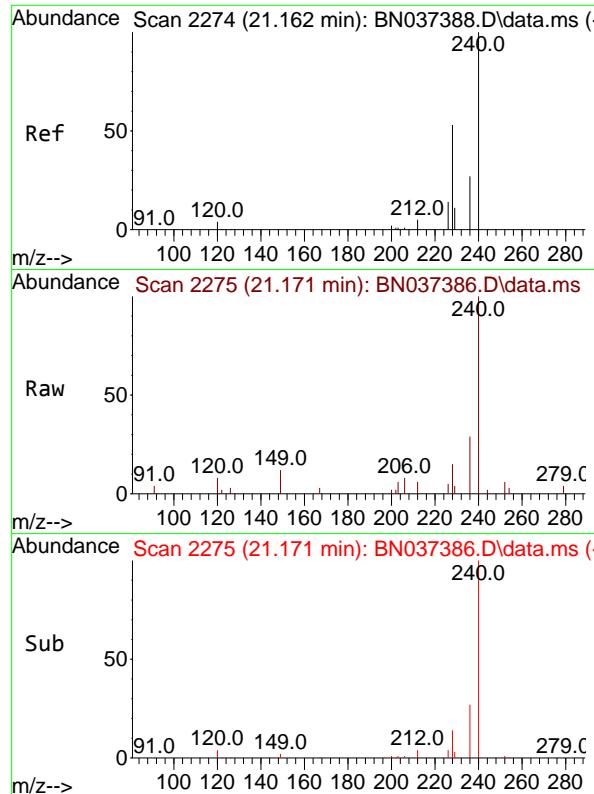


#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.171 min Scan# 2  
Instrument : BNA\_N  
Delta R.T. 0.009 min  
Lab File: BN037386.D ClientSampleId : SSTDICCO.1  
Acq: 26 Jun 2025 10:41


Tgt Ion:240 Resp: 5498  
Ion Ratio Lower Upper  
240 100  
120 7.6 5.3 7.9  
236 29.5 22.7 34.1

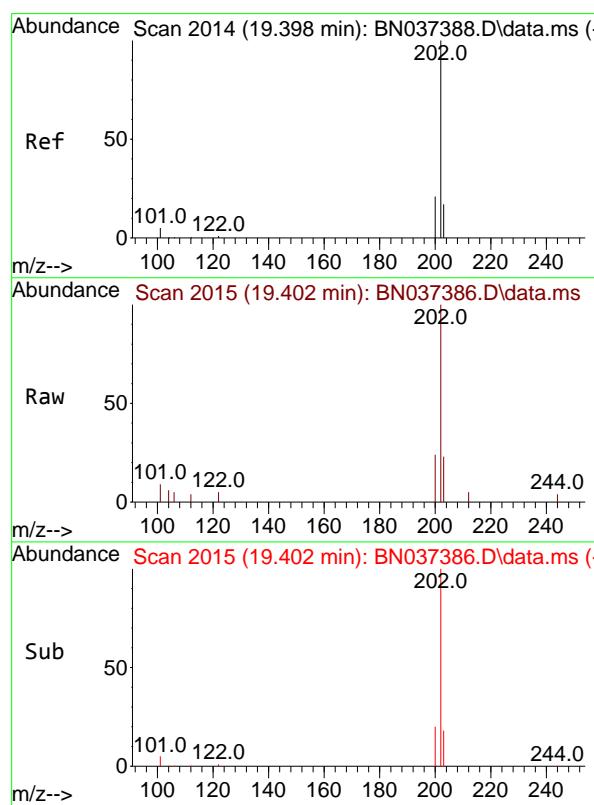

#30  
Pyrene  
Concen: 0.096 ng  
RT: 19.402 min Scan# 2015  
Delta R.T. 0.005 min  
Lab File: BN037386.D  
Acq: 26 Jun 2025 10:41

Tgt Ion:202 Resp: 2006  
Ion Ratio Lower Upper  
202 100  
200 21.0 16.5 24.7  
203 18.0 14.2 21.2





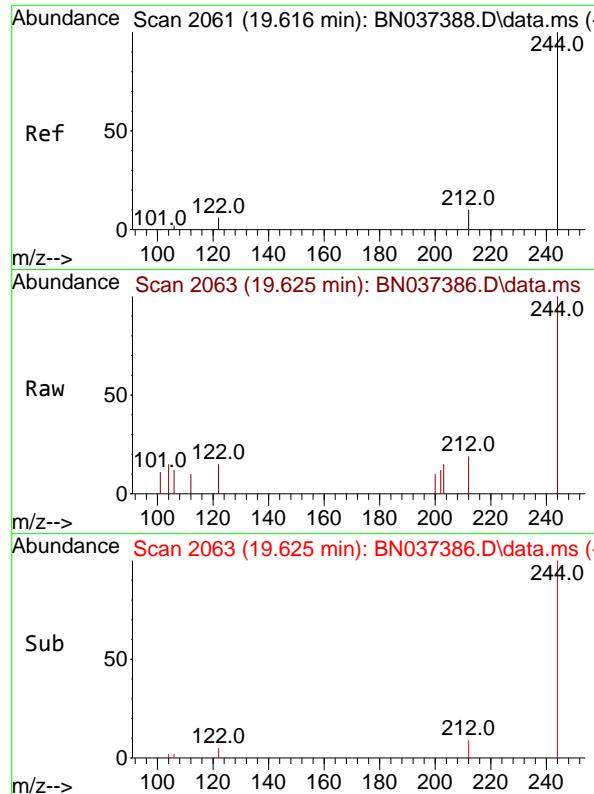

#31  
 Terphenyl-d14  
 Concen: 0.094 ng  
 RT: 19.625 min Scan# 21  
 Delta R.T. 0.009 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:244 Resp: 1099  
 Ion Ratio Lower Upper  
 244 100  
 212 18.9 9.1 13.7#  
 122 14.8 6.3 9.5#

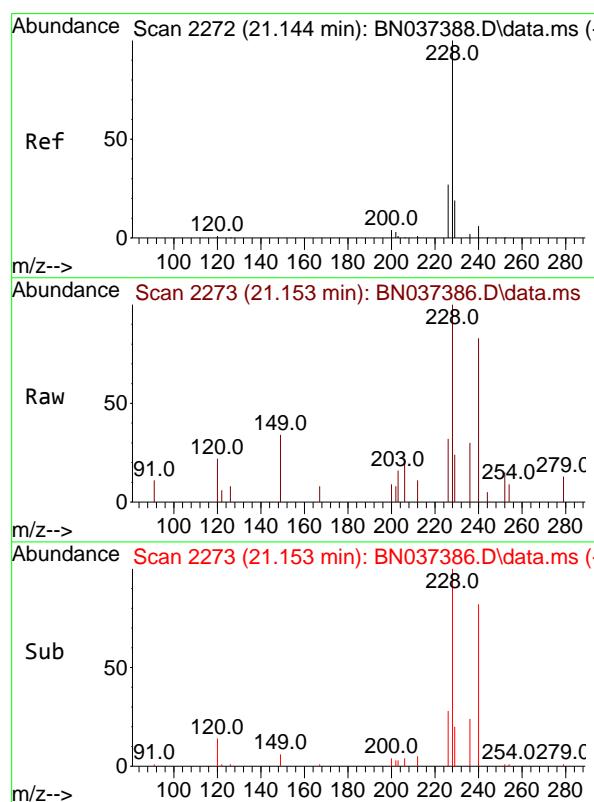

#32  
 Benzo(a)anthracene  
 Concen: 0.091 ng  
 RT: 21.153 min Scan# 2273  
 Delta R.T. 0.009 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Tgt Ion:228 Resp: 1579  
 Ion Ratio Lower Upper  
 228 100  
 226 32.2 22.6 34.0  
 229 24.2 16.2 24.2

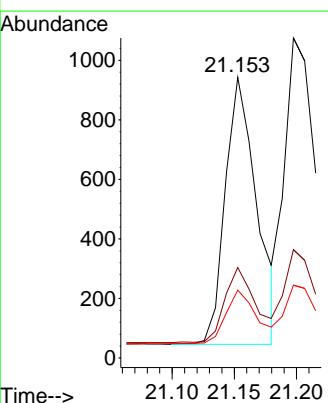






#33  
 Chrysene  
 Concen: 0.105 ng  
 RT: 21.198 min Scan# 2  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1





Tgt Ion:228 Resp: 2241  
 Ion Ratio Lower Upper  
 228 100  
 226 33.9 24.5 36.7  
 229 22.8 16.1 24.1

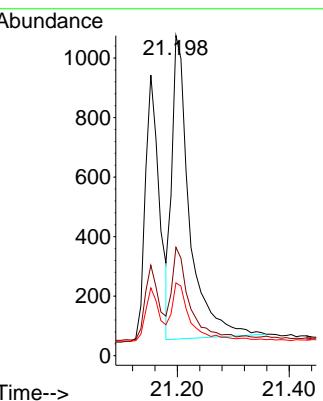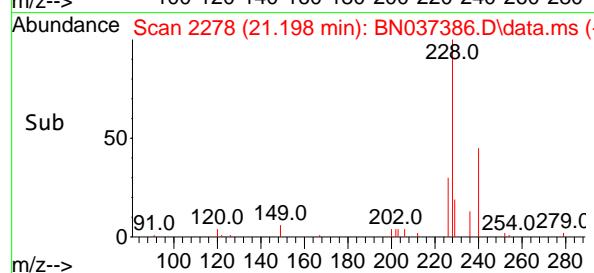


#34  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.123 ng  
 RT: 21.090 min Scan# 2266  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41



Tgt Ion:149 Resp: 839  
 Ion Ratio Lower Upper  
 149 100  
 167 30.3 24.8 37.2  
 279 8.9 5.0 7.6#

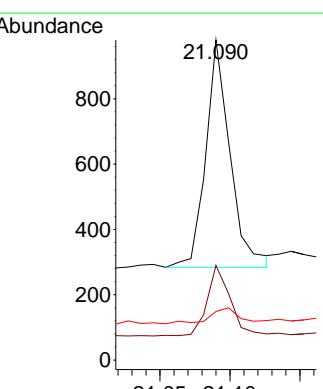



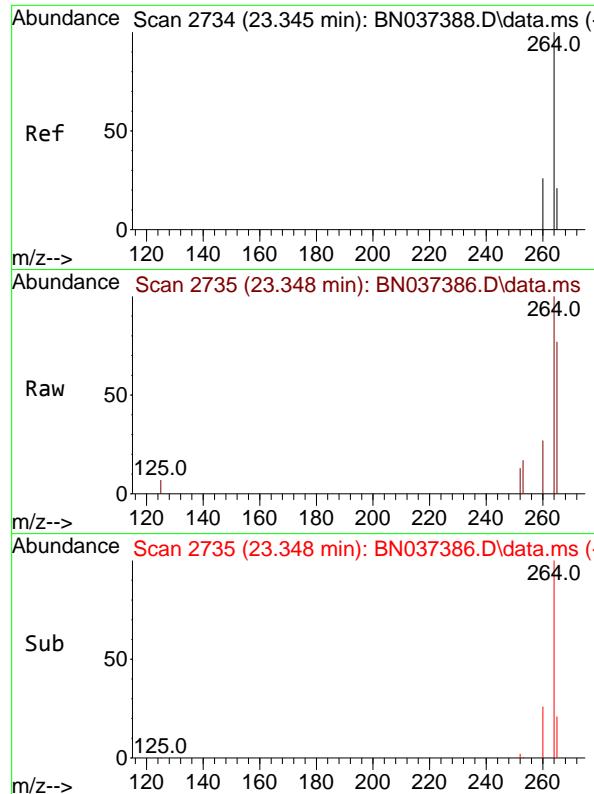

#35  
 Perylene-d<sub>12</sub>  
 Concen: 0.400 ng  
 RT: 23.348 min Scan# 2  
 Delta R.T. 0.003 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:264 Resp: 5798  
 Ion Ratio Lower Upper  
 264 100  
 260 26.9 21.4 32.0  
 265 77.1 56.2 84.4

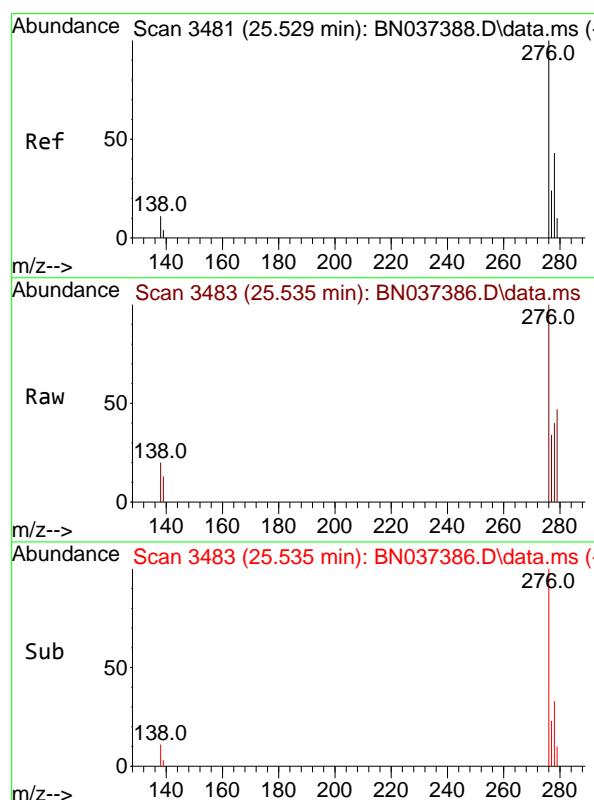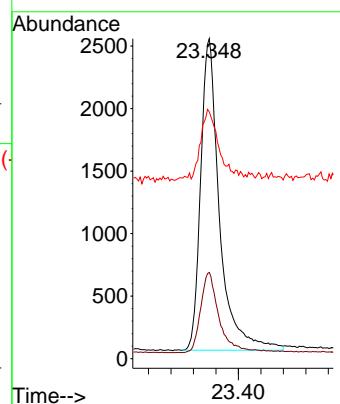

#36  
 Indeno(1,2,3-cd)pyrene  
 Concen: 0.088 ng  
 RT: 25.535 min Scan# 3483  
 Delta R.T. 0.006 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Tgt Ion:276 Resp: 2156  
 Ion Ratio Lower Upper  
 276 100  
 138 4.1 8.5 12.7#  
 277 21.2 19.7 29.5


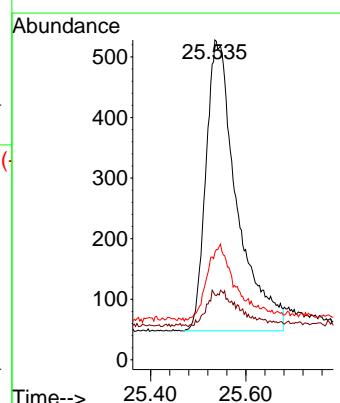


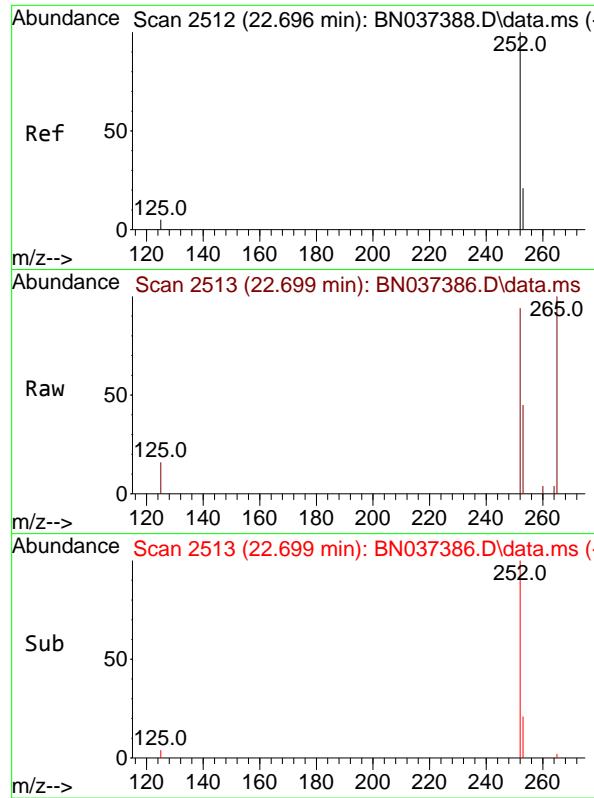

#37  
 Benzo(b)fluoranthene  
 Concen: 0.094 ng  
 RT: 22.699 min Scan# 2  
 Delta R.T. 0.003 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:252 Resp: 1927  
 Ion Ratio Lower Upper  
 252 100  
 253 47.9 22.8 34.2#  
 125 16.7 6.2 9.4#

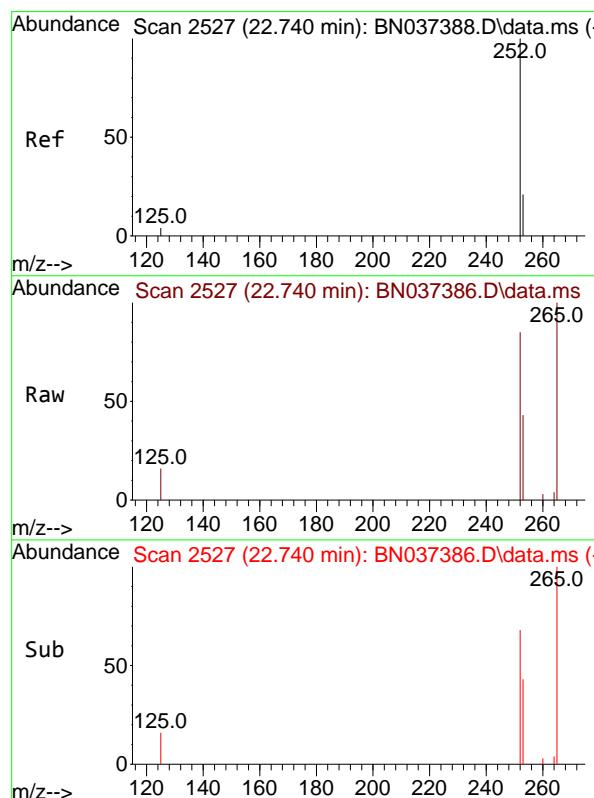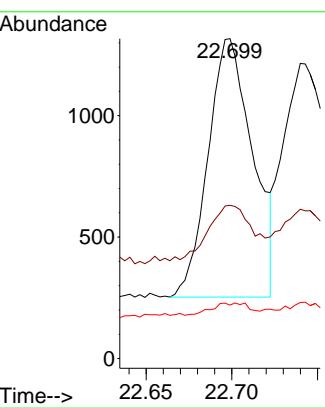

#38  
 Benzo(k)fluoranthene  
 Concen: 0.093 ng  
 RT: 22.740 min Scan# 2527  
 Delta R.T. -0.000 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Tgt Ion:252 Resp: 2041  
 Ion Ratio Lower Upper  
 252 100  
 253 50.6 23.2 34.8#  
 125 19.0 6.0 9.0#


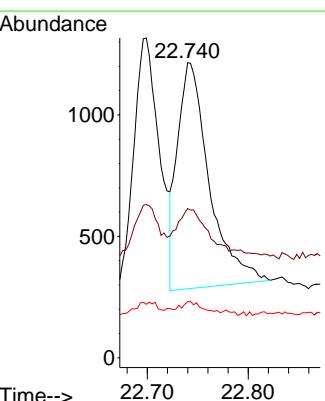


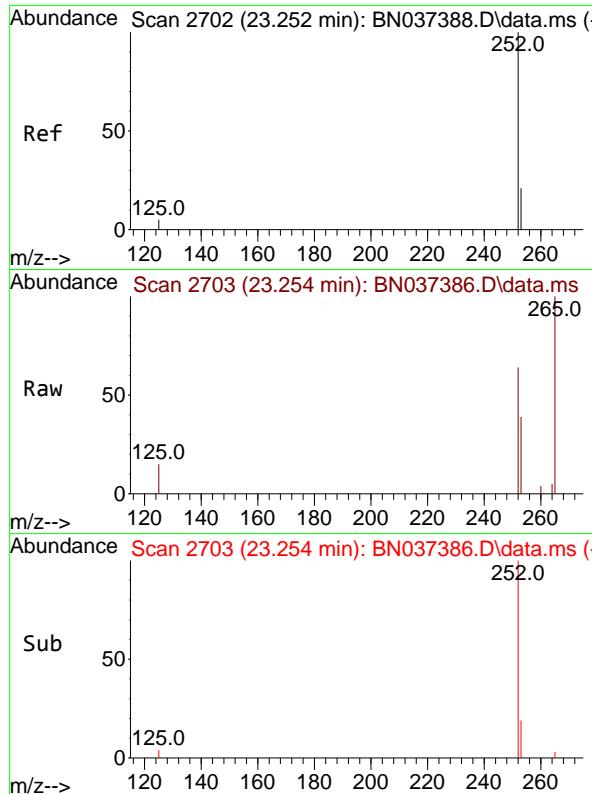

#39  
 Benzo(a)pyrene  
 Concen: 0.097 ng  
 RT: 23.254 min Scan# 2  
 Delta R.T. 0.003 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41


Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1


Tgt Ion:252 Resp: 1755  
 Ion Ratio Lower Upper  
 252 100  
 253 60.6 25.6 38.4#  
 125 22.9 7.5 11.3#

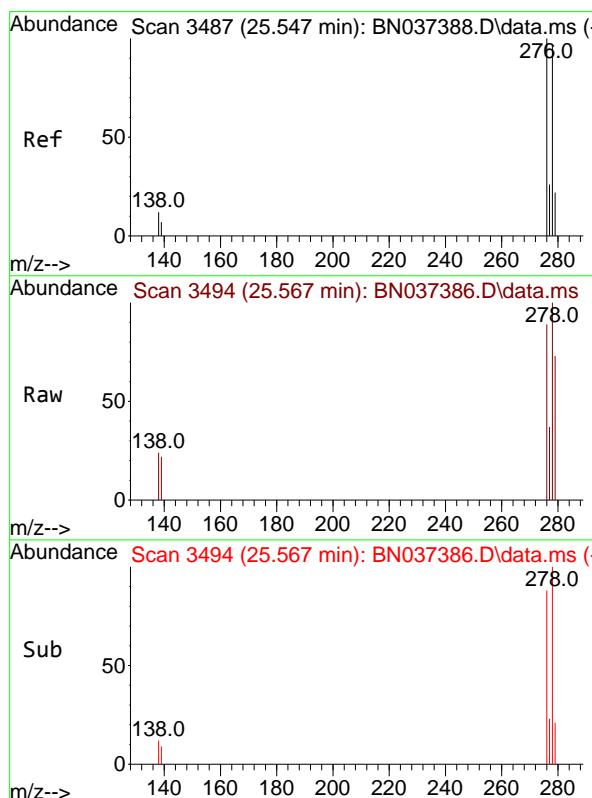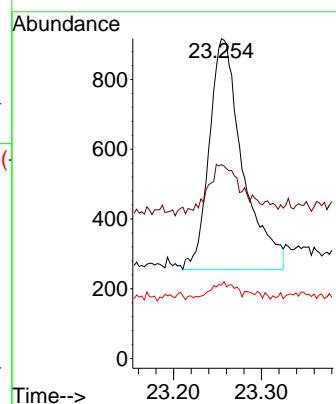

#40  
 Dibenzo(a,h)anthracene  
 Concen: 0.081 ng  
 RT: 25.567 min Scan# 3494  
 Delta R.T. 0.020 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Tgt Ion:278 Resp: 1522  
 Ion Ratio Lower Upper  
 278 100  
 139 22.1 8.5 12.7#  
 279 73.1 27.5 41.3#

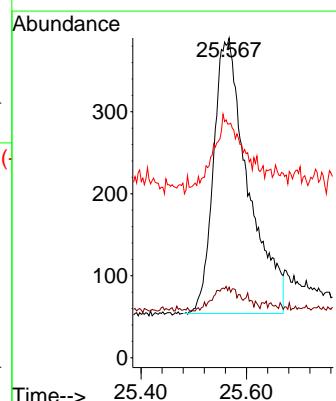

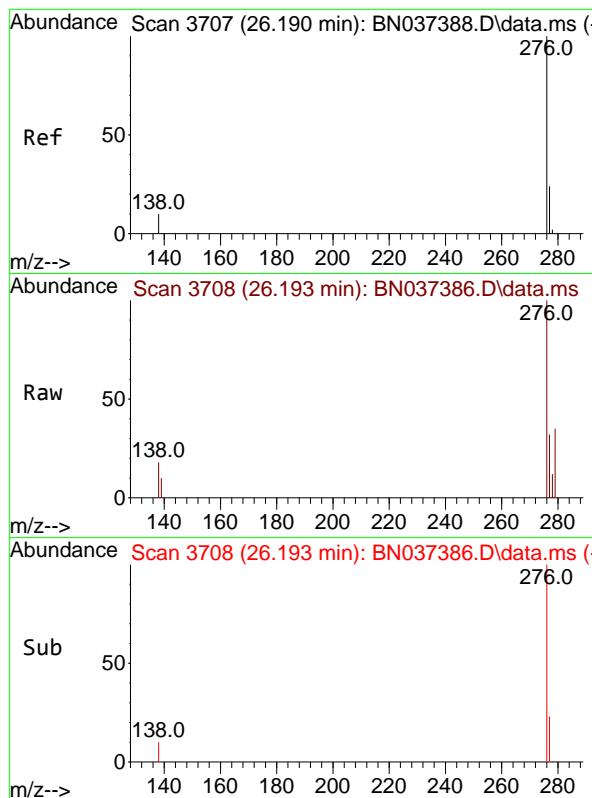

#41  
 Benzo(g,h,i)perylene  
 Concen: 0.092 ng  
 RT: 26.193 min Scan# 3  
 Delta R.T. 0.003 min  
 Lab File: BN037386.D  
 Acq: 26 Jun 2025 10:41

Instrument : BNA\_N  
 ClientSampleId : SSTDICCO.1

Tgt Ion:276 Resp: 2066  
 Ion Ratio Lower Upper  
 276 100  
 277 31.8 21.0 31.4#  
 138 18.4 9.6 14.4#

