


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062325\
Data File : VU063419.D
Acq On : 23 Jun 2025 08:48
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jun 24 05:06:50 2025

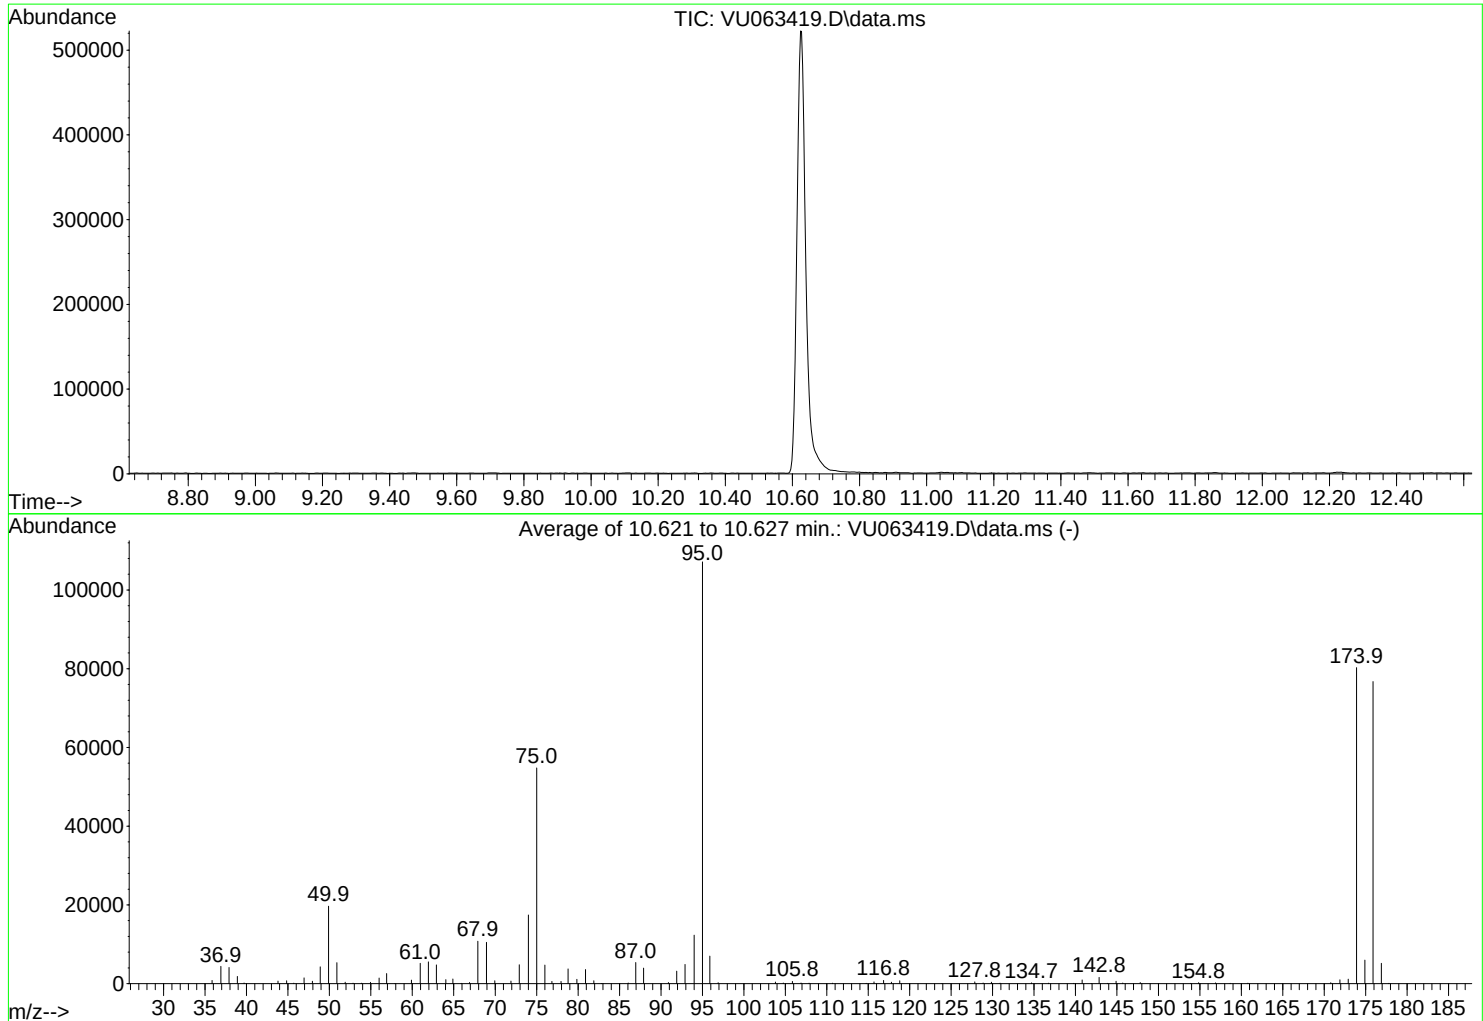

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	19656	PASS
75	95	30	60	51.2	54813	PASS
95	95	100	100	100.0	107157	PASS
96	95	5	9	6.5	6998	PASS
173	174	0.00	2	1.4	1128	PASS
174	95	50	100	74.9	80261	PASS
175	174	5	9	7.4	5961	PASS
176	174	95	101	95.6	76725	PASS
177	176	5	9	6.7	5172	PASS