


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063429.D
Acq On : 24 Jun 2025 09:49
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Jun 24 05:06:50 2025

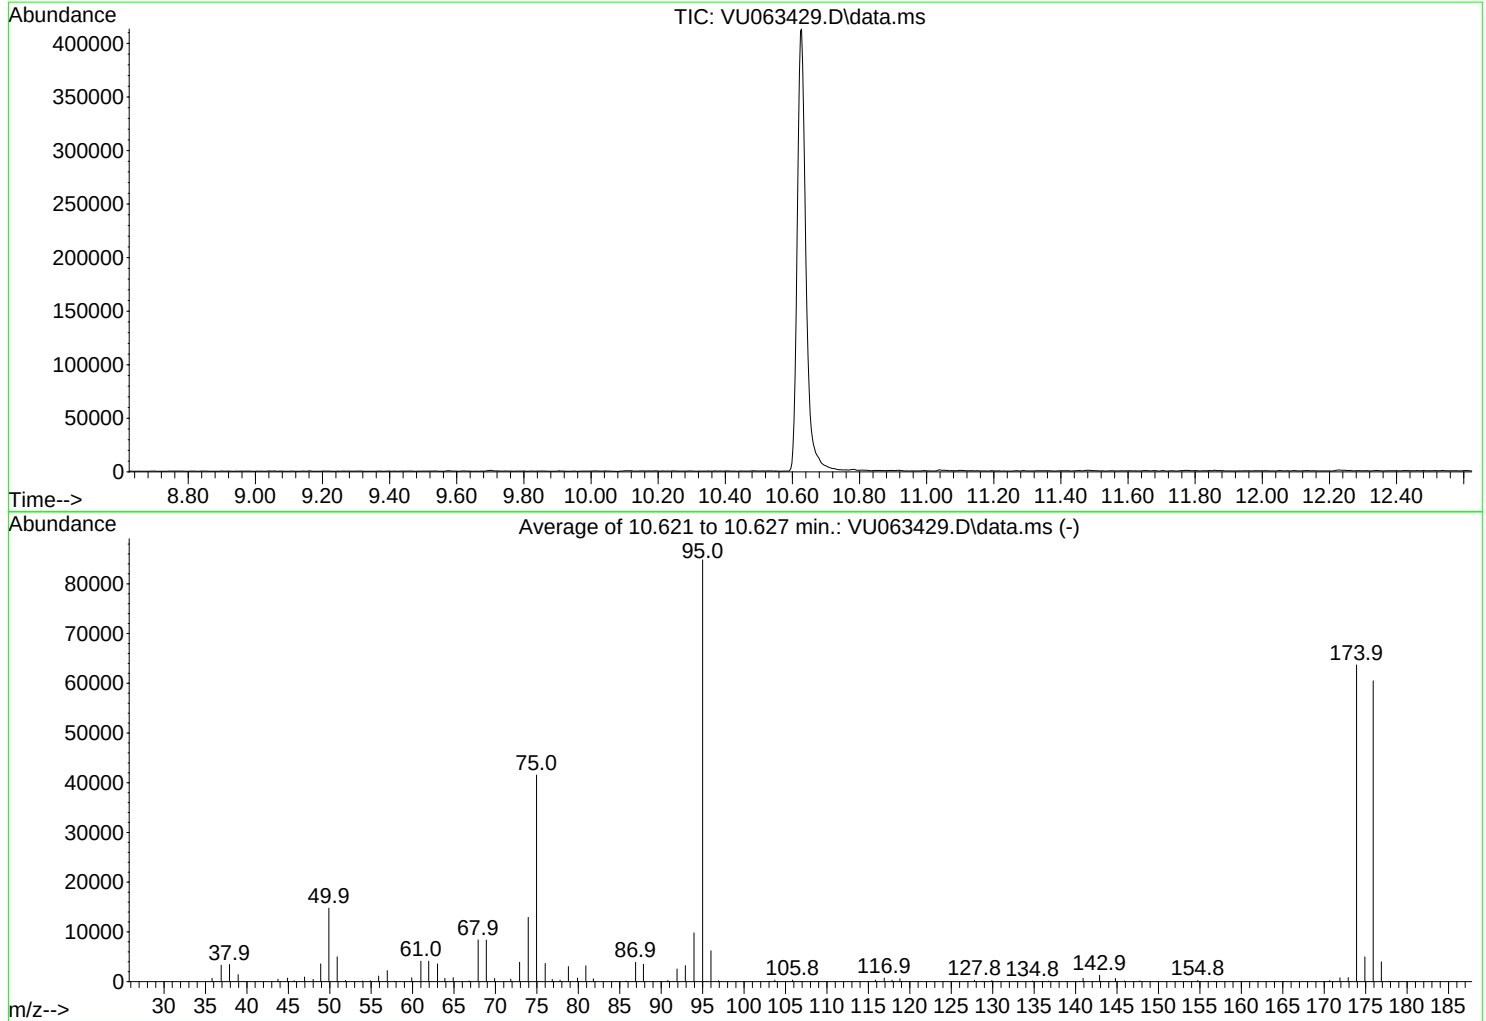

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	14761	PASS
75	95	30	60	49.0	41555	PASS
95	95	100	100	100.0	84821	PASS
96	95	5	9	7.3	6199	PASS
173	174	0.00	2	1.3	823	PASS
174	95	50	100	75.1	63677	PASS
175	174	5	9	7.8	4980	PASS
176	174	95	101	95.0	60499	PASS
177	176	5	9	6.6	3997	PASS