

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
 Data File : VU063431.D
 Acq On : 24 Jun 2025 11:14
 Operator : MD/SY
 Sample : VU0624WBL01
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0624WBL01

Quant Time: Jun 25 01:30:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Jun 24 05:06:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.106	96	48463	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.630	95	13246	0.744	ug/l	0.00
Spiked Amount	1.000		Recovery	=	74.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	13088	0.732	ug/l	0.00
Spiked Amount	1.000		Recovery	=	73.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062425\
Data File : VU063431.D
Acq On : 24 Jun 2025 11:14
Operator : MD/SY
Sample : VU0624WBL01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL01

Quant Time: Jun 25 01:30:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U062325DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Jun 24 05:06:50 2025
Response via : Initial Calibration




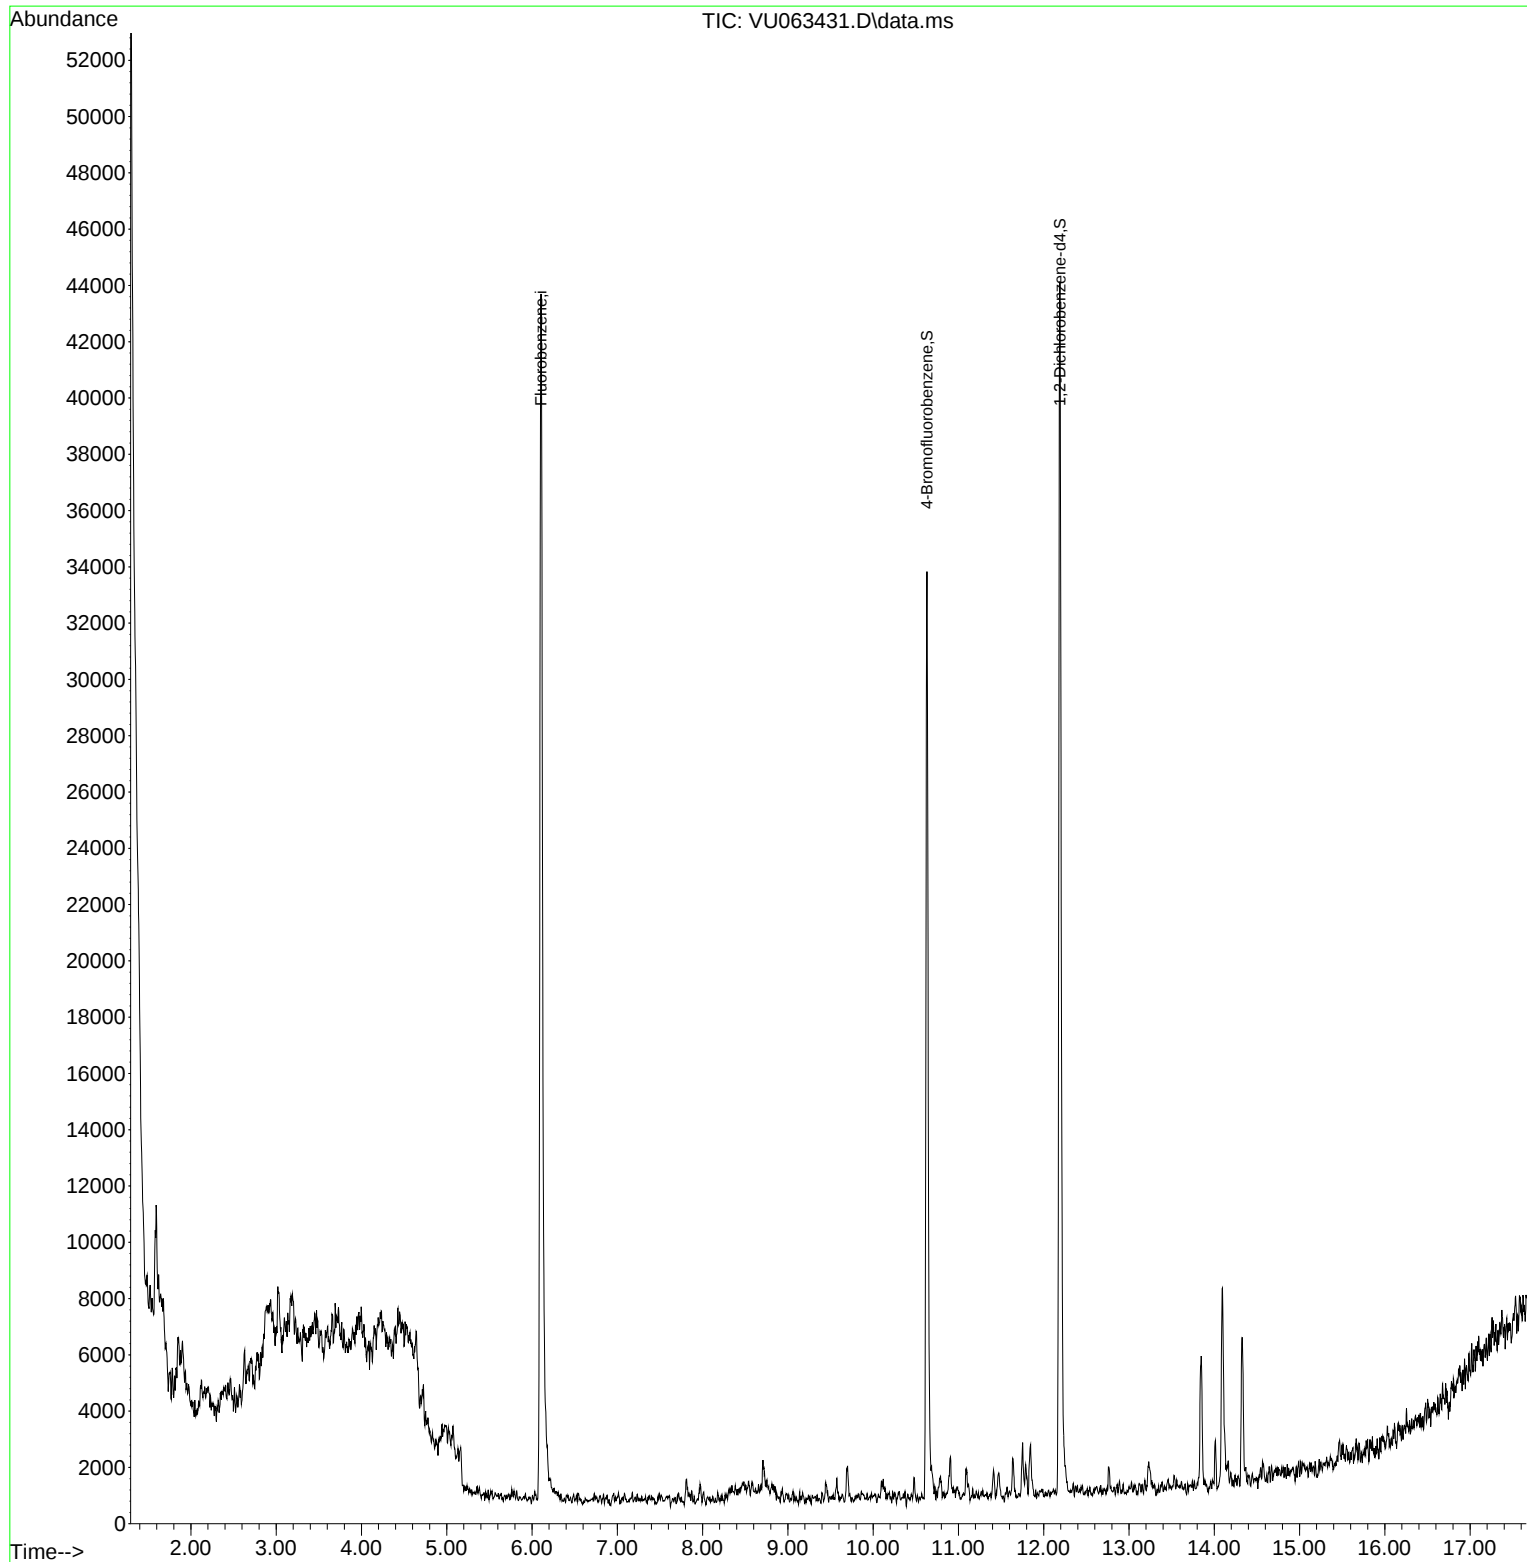


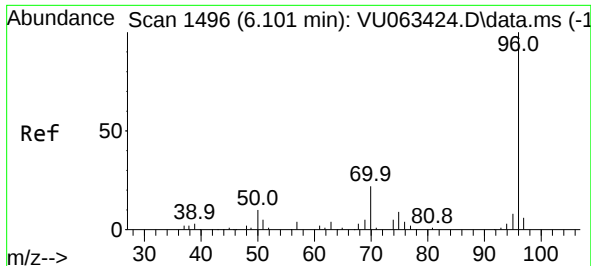

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.106 min Scan# 1496
Delta R.T. 0.005 min
Lab File: VU063431.D
Acq: 24 Jun 2025 11:14




Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL01


Tgt Ion: 96	Resp: 48463
Ion Ratio	Lower Upper
96 100	
70 20.6	16.4 24.6
95 8.1	6.2 9.2
97 5.6	0.0 0.0

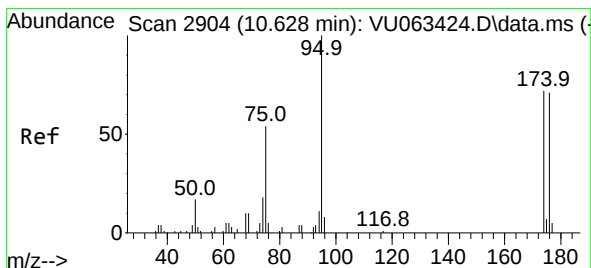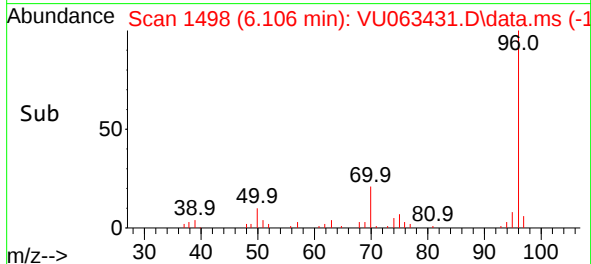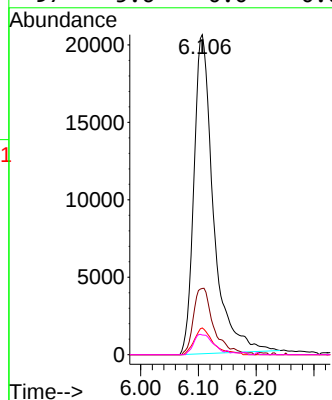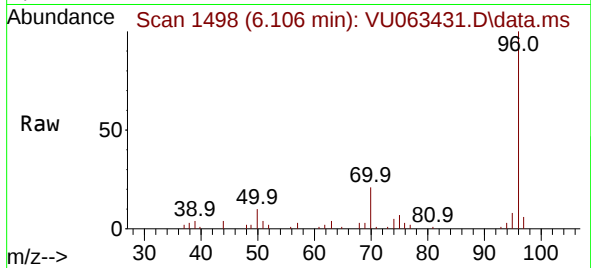

#57
4-Bromofluorobenzene
Concen: 0.744 ug/l
RT: 10.630 min Scan# 2905
Delta R.T. 0.002 min
Lab File: VU063431.D
Acq: 24 Jun 2025 11:14


Tgt Ion: 95	Resp: 13246
Ion Ratio	Lower Upper
95 100	
174 83.2	59.4 89.2
176 77.5	57.8 86.6

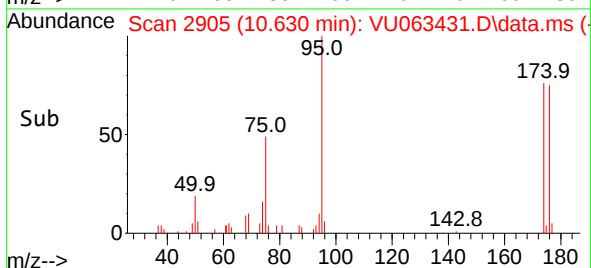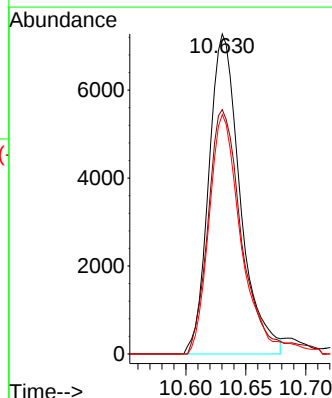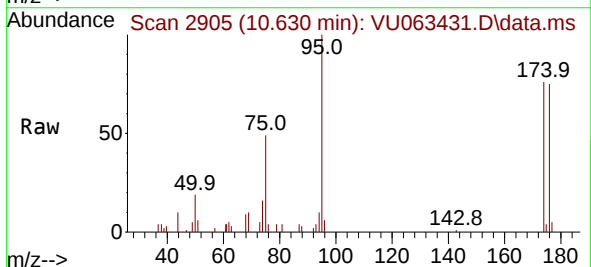

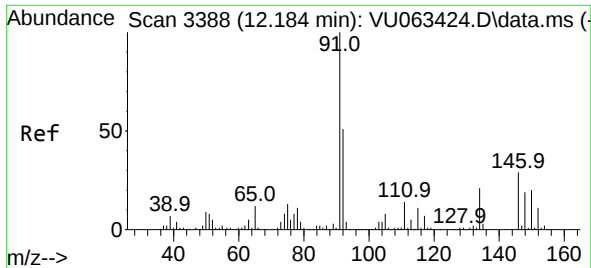

#68
1,2-Dichlorobenzene-d4
Concen: 0.732 ug/l
RT: 12.190 min Scan# 31
Delta R.T. 0.006 min
Lab File: VU063431.D
Acq: 24 Jun 2025 11:14

Instrument :
MSVOA_U
ClientSampleId :
VU0624WBL01

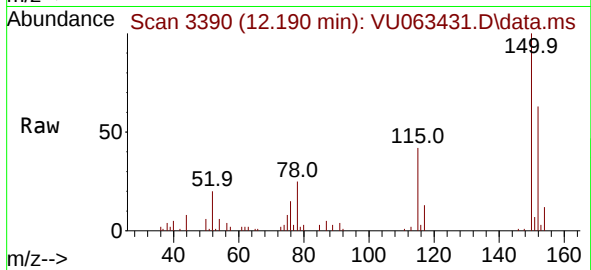

Tgt Ion	Ratio	Lower	Upper
152	100		
115	67.2	0.0	327.6
150	164.7	0.0	664.4

